



US00D938582S

(12) **United States Design Patent** (10) **Patent No.:** **US D938,582 S**
Pitulat et al. (45) **Date of Patent:** **** Dec. 14, 2021**

(54) **PLUNGER ROD FOR USE WITH A SYRINGE**

(71) Applicant: **Becton Dickinson France, Le**
Pont-de-Claix (FR)
(72) Inventors: **Loïc Pitulat**, Vaulnaveys le Haut (FR);
Yves-Eric Dufour, Saint Martin
d'Hères (FR)
(73) Assignee: **Becton Dickinson France, Le**
Pont-de-Claix (FR)
(**) Term: **15 Years**

(21) Appl. No.: **29/727,483**
(22) Filed: **Mar. 11, 2020**
(51) **LOC (13) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/130; D24/127**
(58) **Field of Classification Search**
USPC ... D24/127, 130, 133, 146, 147, 108, 110.6,
D24/112-114, 129, 224-226, 231, 232;
D23/262
CPC G09B 23/285; A61M 5/31501; A61M
2005/3151; A61M 5/3148; A61M
5/31513; A61M 2005/3128; A61M
5/31515
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D287,053 S * 12/1986 Bucchianeri D24/130
D432,231 S * 10/2000 Balestracci D24/112
D437,050 S * 1/2001 Balestracci D24/112
D462,441 S * 9/2002 Garner D24/133
D638,122 S * 5/2011 Kosinski A61M 5/3129
D24/130

(Continued)

FOREIGN PATENT DOCUMENTS

EM 008163687-0001 * 11/2020
EM 008163687-0002 * 11/2020

OTHER PUBLICATIONS

Usage Of Becton Dickinson Precise Luer Lok Syringes in Syringe
Pumps | Demo Film, Youtube, [Post date Jan. 4, 2021], [Site visited
Sep. 8, 2021], Seen at URL: <https://www.youtube.com/watch?v=xlQ5jxVHiol> (Year: 2021).*

(Continued)

Primary Examiner — Natasha Vujcic
Assistant Examiner — Gilbert B Ford

(74) *Attorney, Agent, or Firm* — The Webb Law Firm

(57) **CLAIM**


The ornamental design for a plunger rod for use with a
syringe, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a plunger rod for use with
syringe;
FIG. 2 is another perspective view of the plunger rod of FIG.
1.
FIG. 3 is another perspective view of the plunger rod of FIG.
1.
FIG. 4 is another perspective view of the plunger rod of FIG.
1.
FIG. 5 is another perspective view of the plunger rod of FIG.
1.
FIG. 6 is a front view of the plunger rod of FIG. 1.
FIG. 7 is a top view of the plunger rod of FIG. 1.
FIG. 8 is a right side view of the plunger rod of FIG. 1.
FIG. 9 is a left side view of the plunger rod of FIG. 1.
FIG. 10 is a rear view of the plunger rod of FIG. 1.
FIG. 11 is a bottom view of the plunger rod of FIG. 1; and,
FIG. 12 is a cross-sectional view of the plunger rod of FIG.
10, taken along line 12-12 of FIG. 10.

The broken lines representing ribs of the plunger rod, shown
in FIGS. 1-6, 9, and 10, form no part of the claimed design.

1 Claim, 8 Drawing Sheets

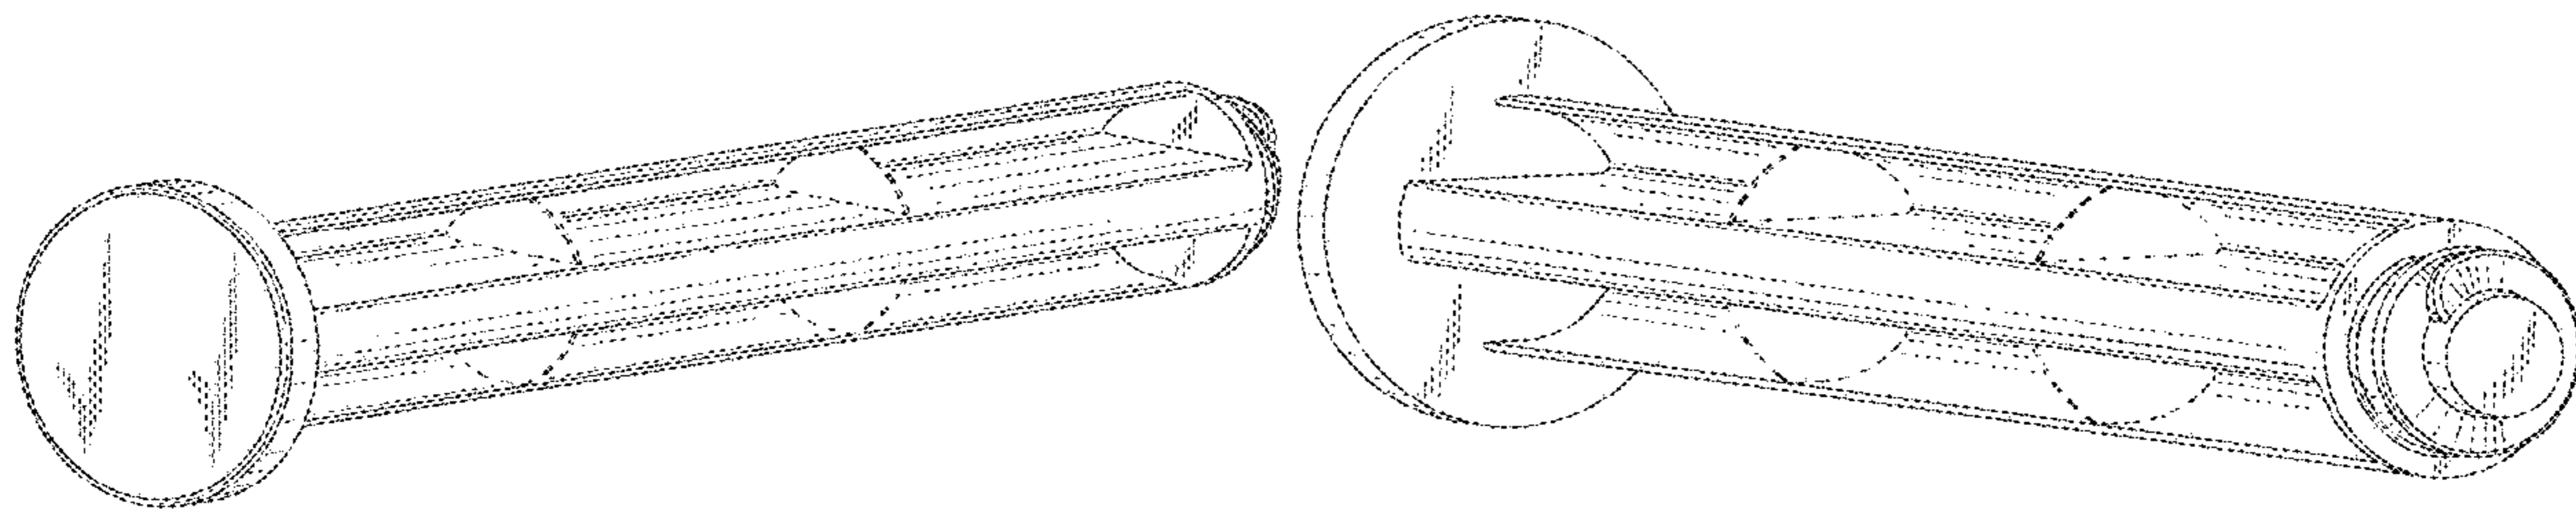

(56)

References Cited

U.S. PATENT DOCUMENTS

D663,415 S * 7/2012 Tamura D24/130
D667,108 S * 9/2012 Mottahed D24/130
D667,109 S * 9/2012 Mottahed D24/130
D673,268 S * 12/2012 Kommireddy D24/130
D673,675 S * 1/2013 Wong D24/130
D689,188 S * 9/2013 Lundquist D24/130
D713,525 S * 9/2014 Oguro D24/130
D865,947 S * 11/2019 Khalaj D24/114
D889,639 S * 7/2020 Johnson D24/114
D909,570 S * 2/2021 Ahmad D24/114
D911,519 S * 2/2021 Newlove D24/130
2017/0028135 A1 * 2/2017 Fransson A61M 5/3129
2017/0203046 A1 * 7/2017 LaRose A61L 31/048
2017/0209648 A1 * 7/2017 Butts A61L 31/14
2020/0405965 A1 * 12/2020 Marici A61L 2/08
2020/0410897 A1 * 12/2020 Baker A61M 5/31501
2021/0077738 A1 * 3/2021 Dadachanji A61M 5/31501

OTHER PUBLICATIONS

Syringe Loss-Of-Resistance BD Epilor, Simplibuy.ca, [Postdate Jan. 1, 2019n], [Site visited Sep. 8, 2021], Seen at URL: <https://www.simplibuy.ca/Product/Details/10863> (Year: 2019).*

LOR Syringe—Luer Slip Tip, Busse, insightneedles.com, [Post date unknoww], [Site visited Sep. 8, 2021], Seen at URL: <https://www.insightneedles.com/products/busse-lor-syringe> (Year: 2021).*

* cited by examiner

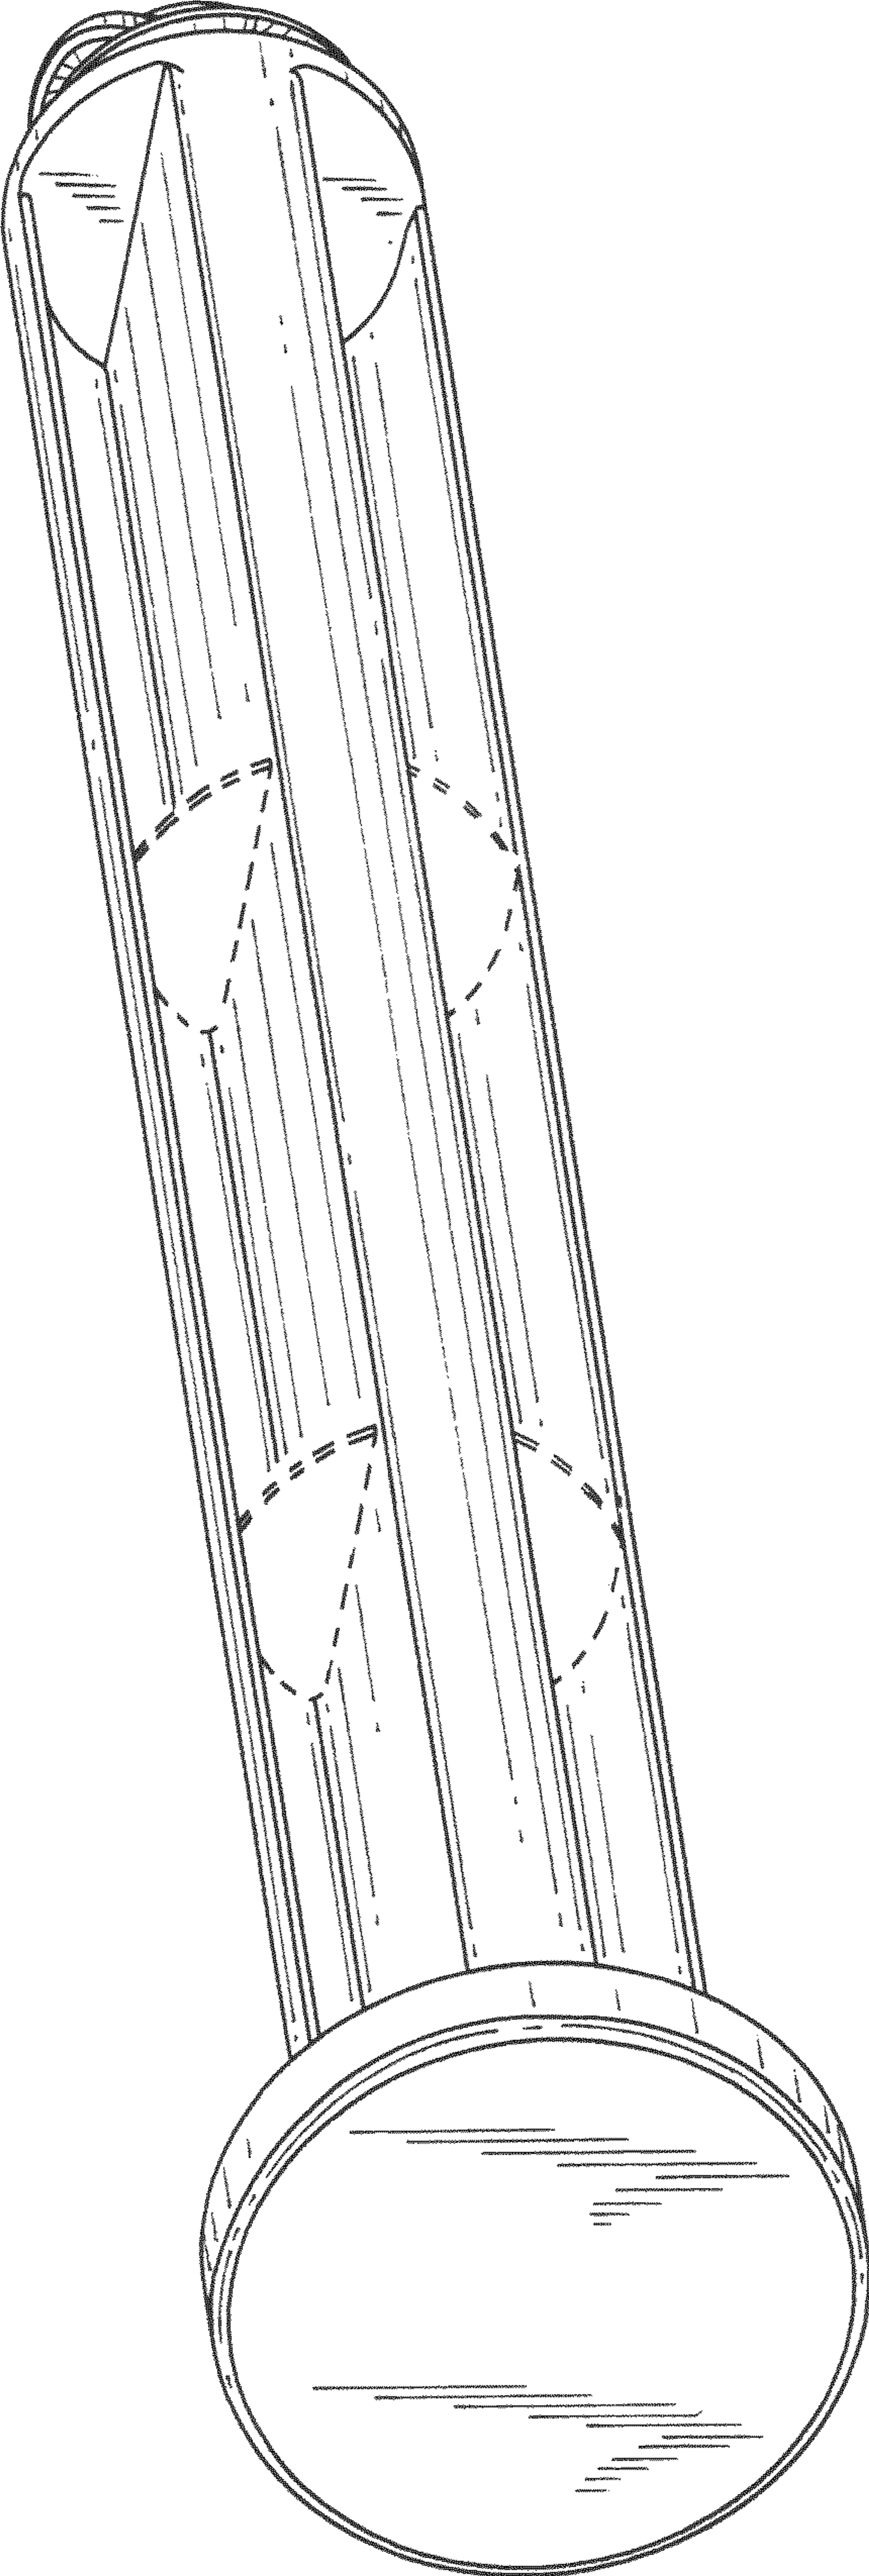


FIG.1

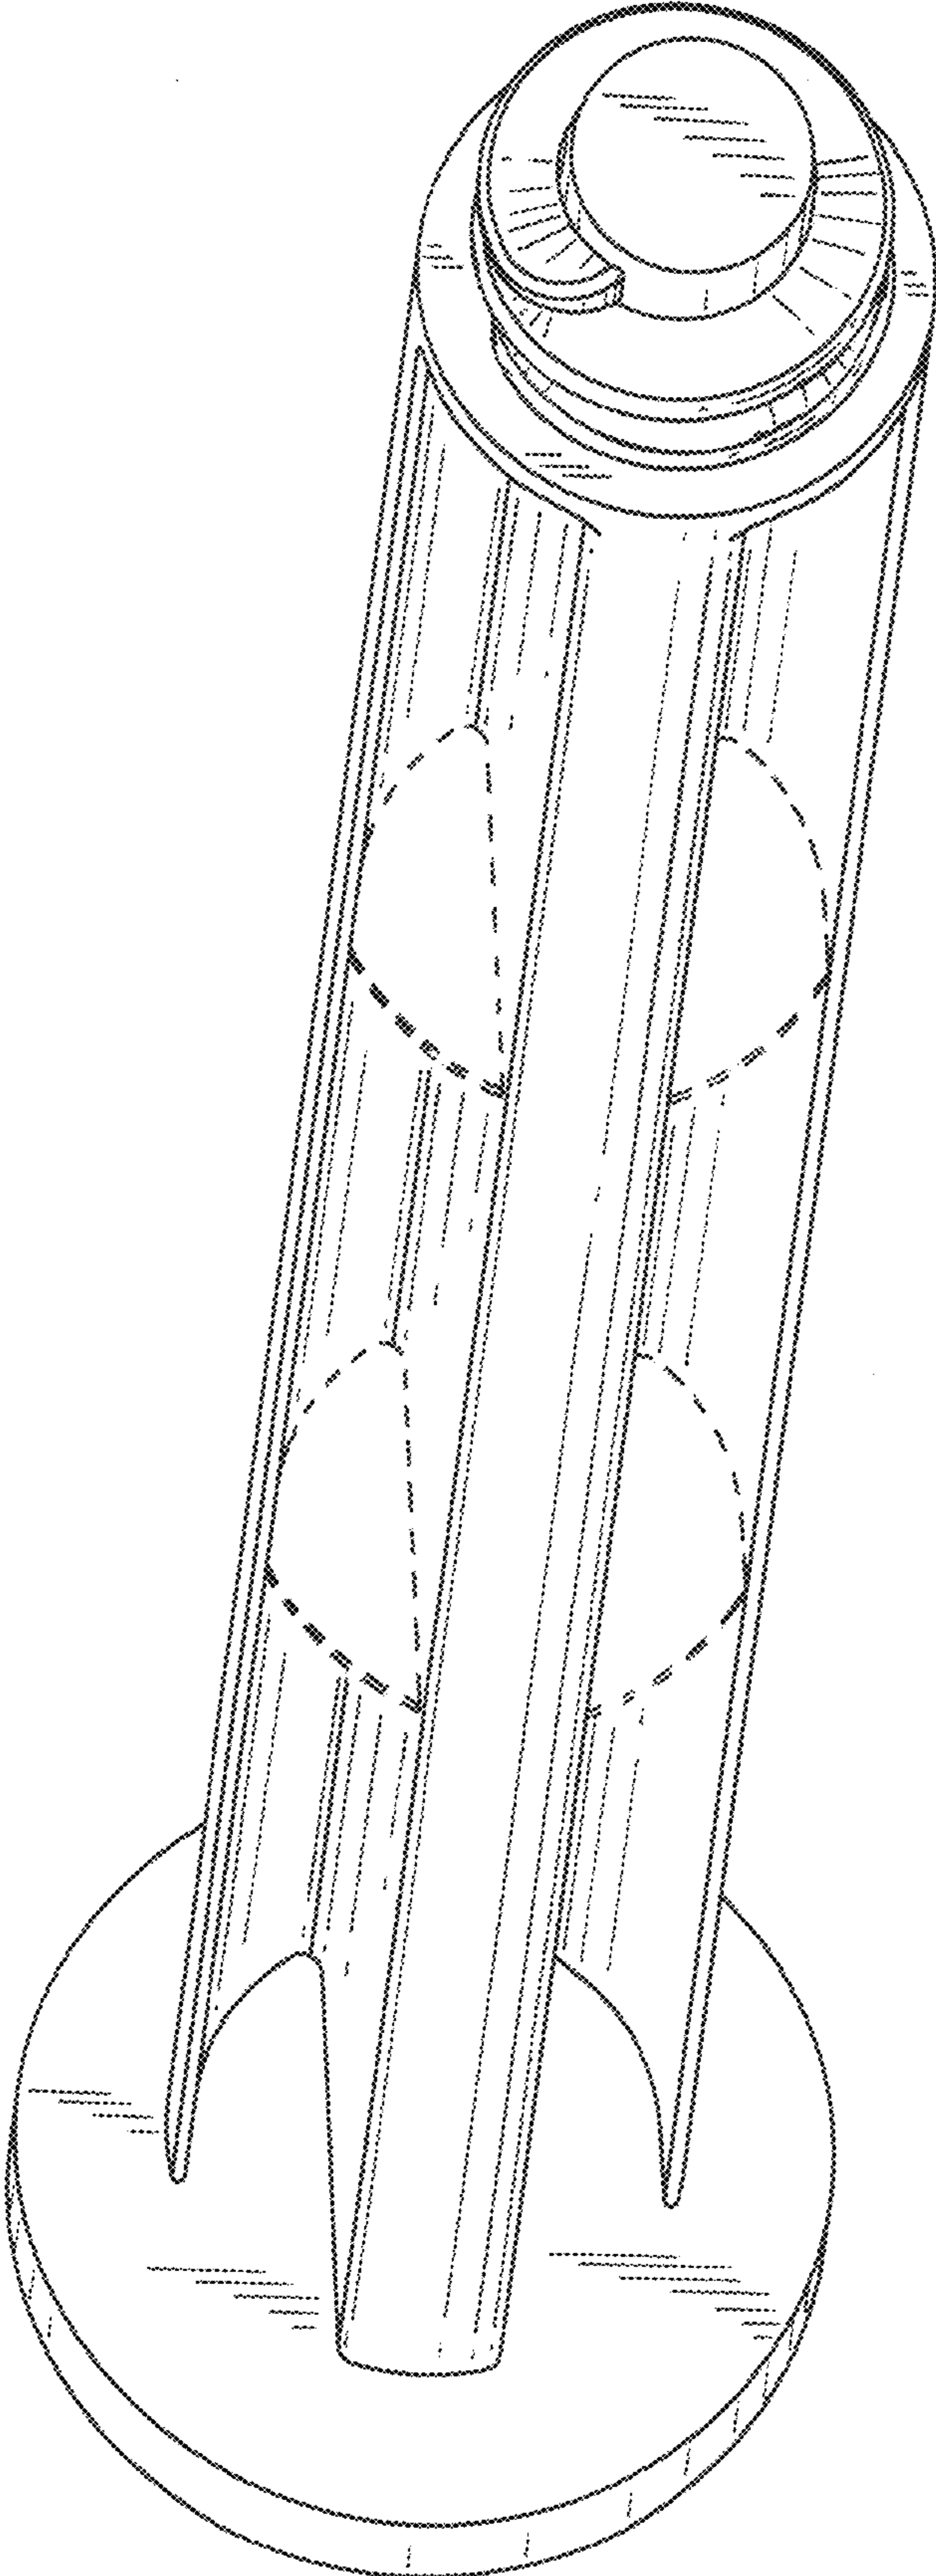


FIG.2

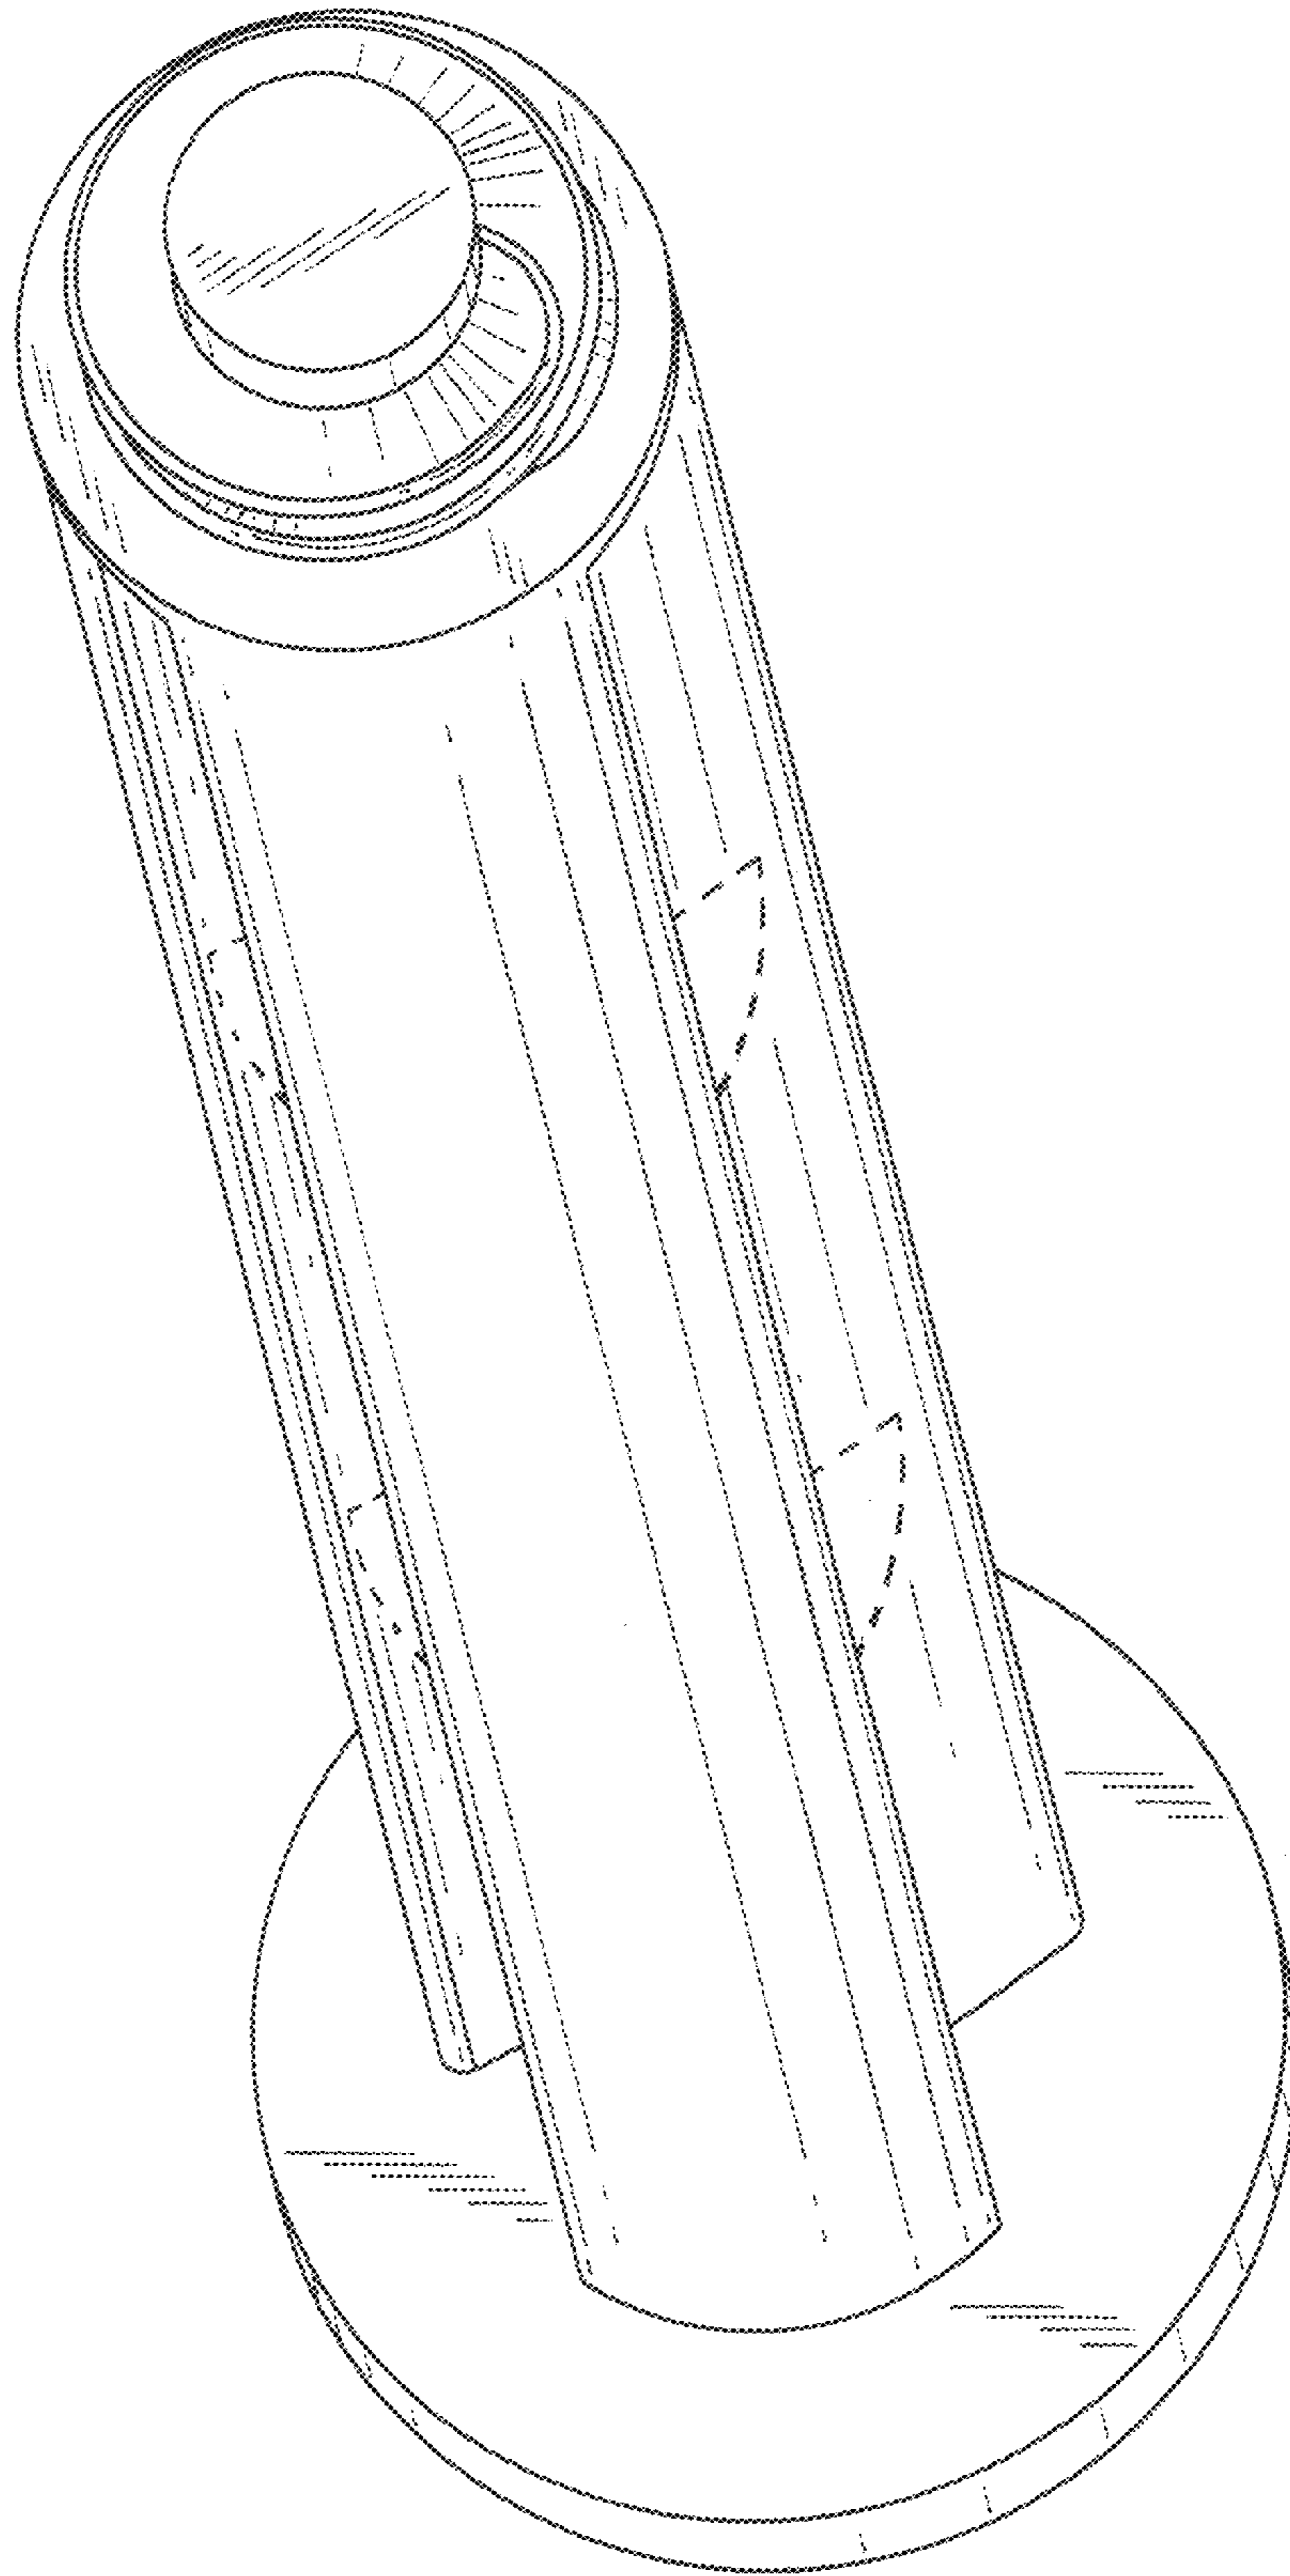


FIG. 3

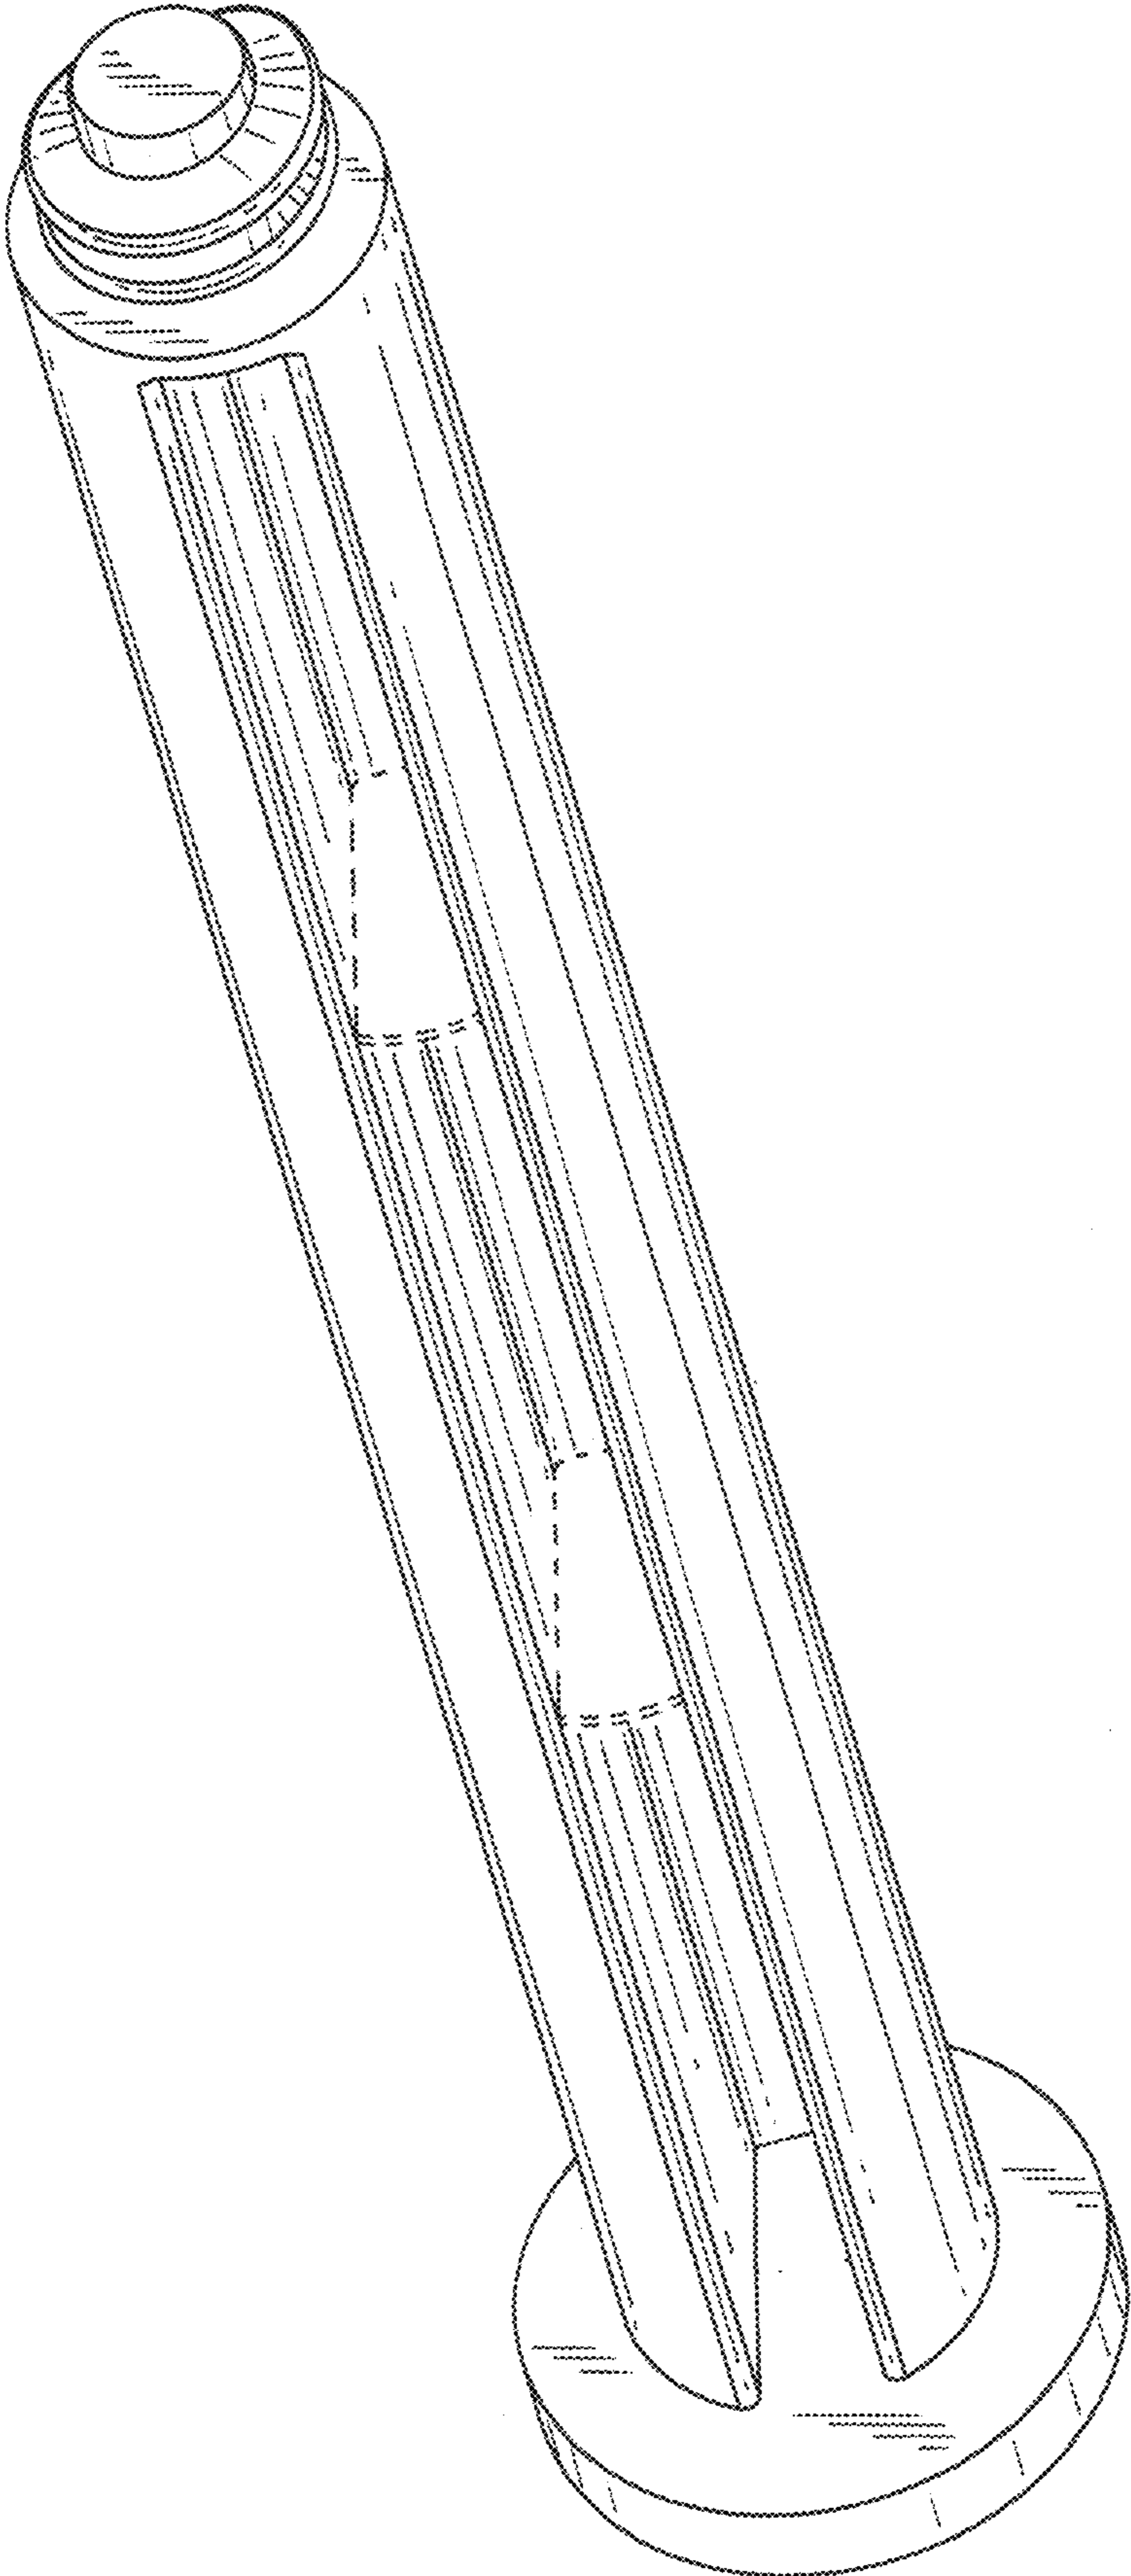


FIG.4

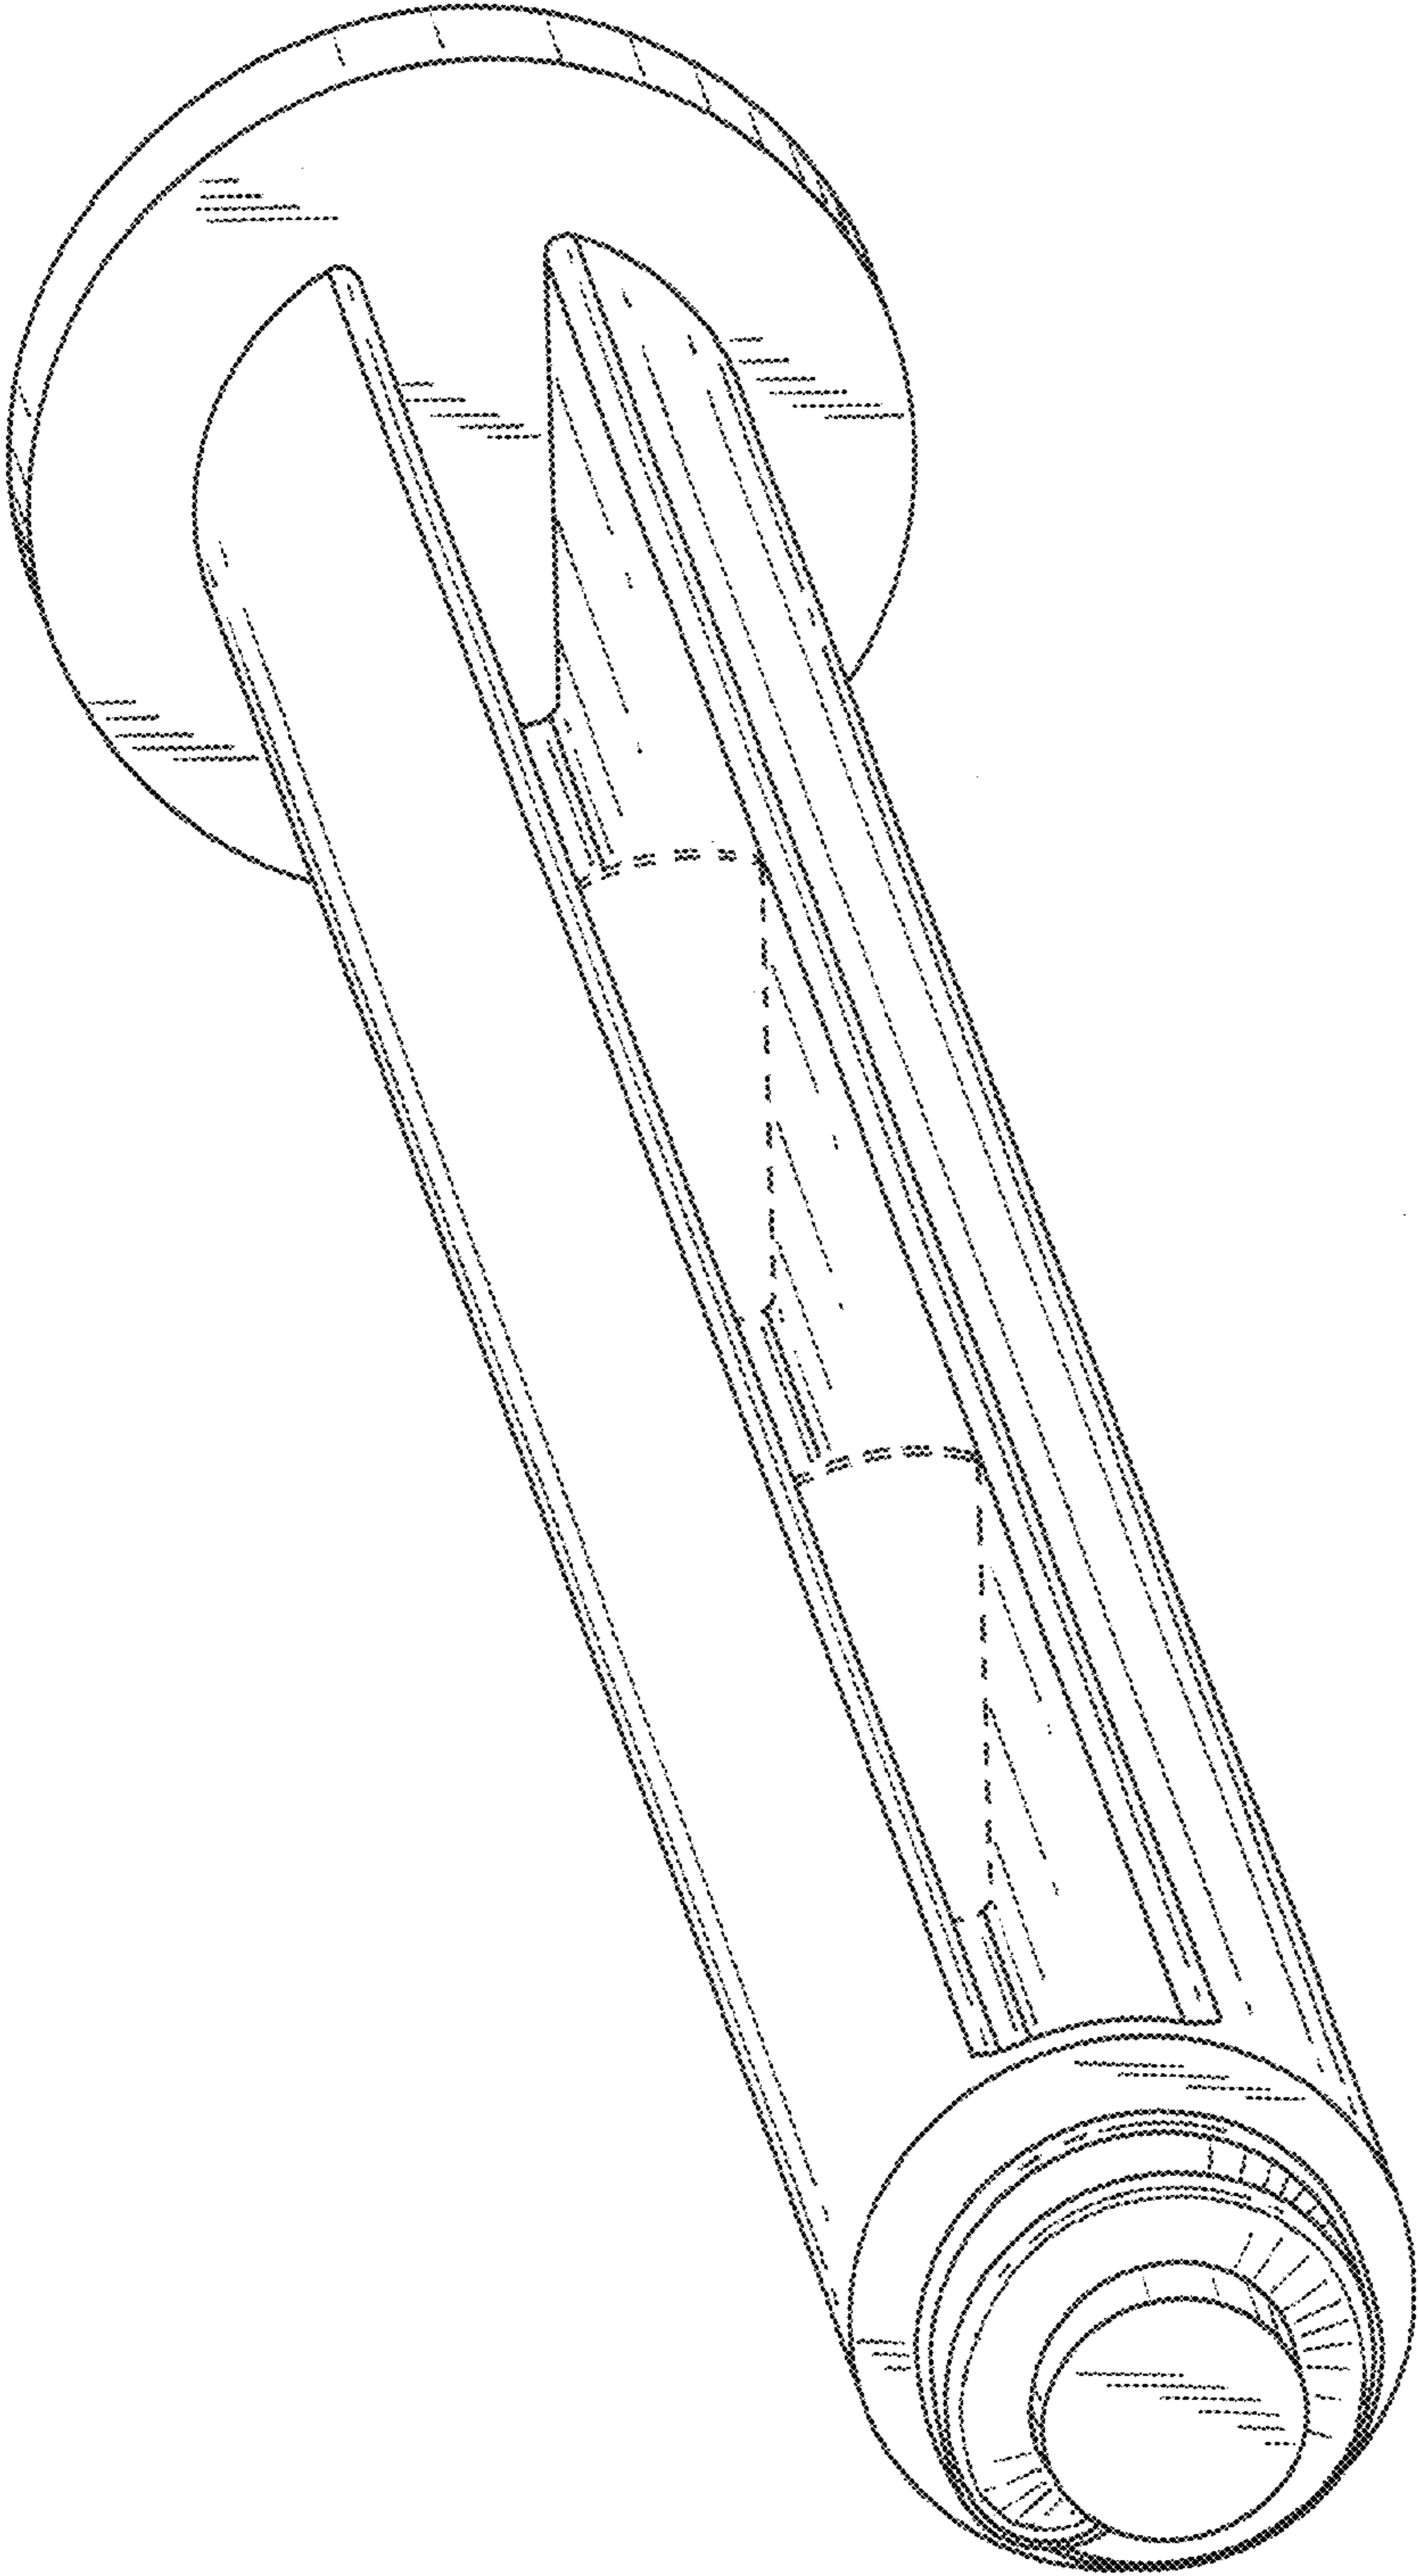


FIG. 5

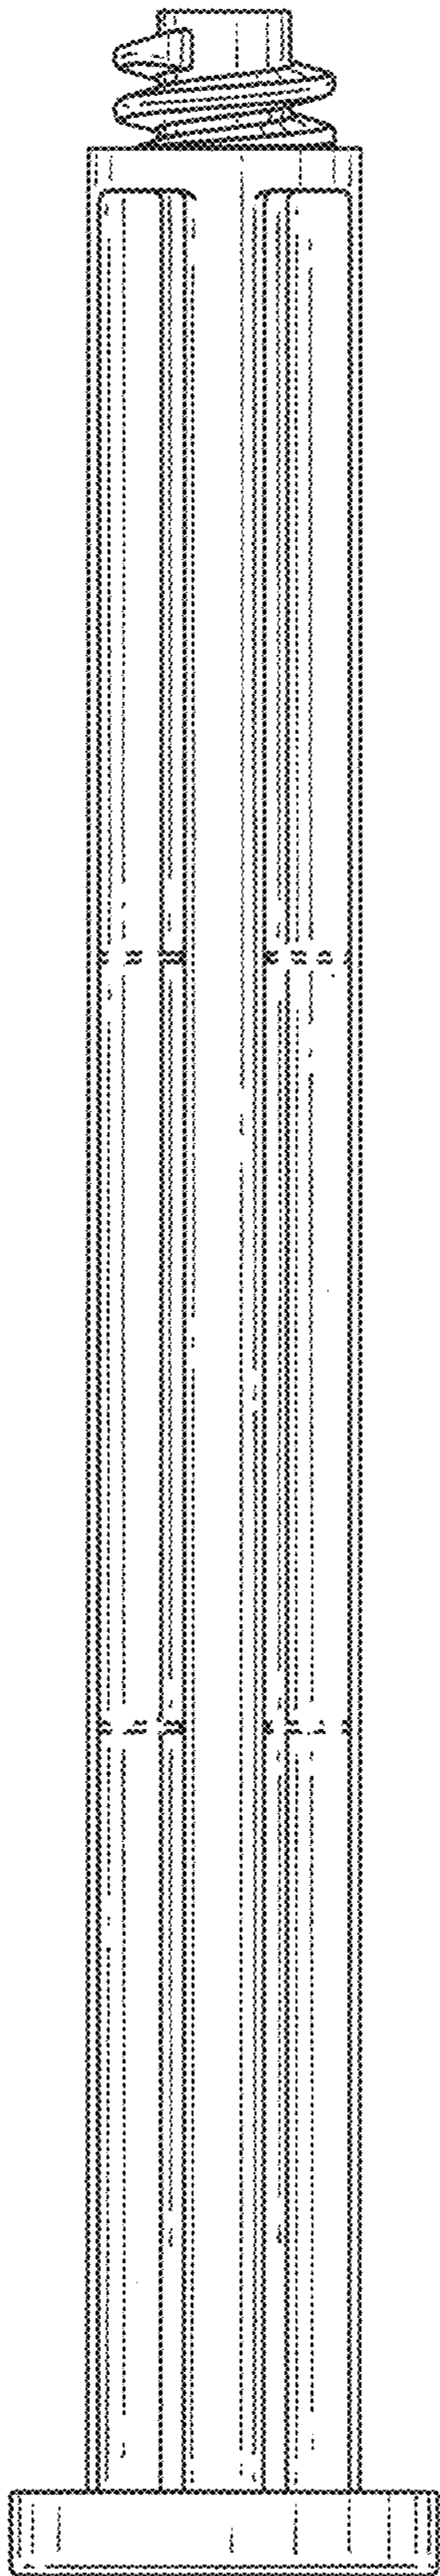


FIG. 6

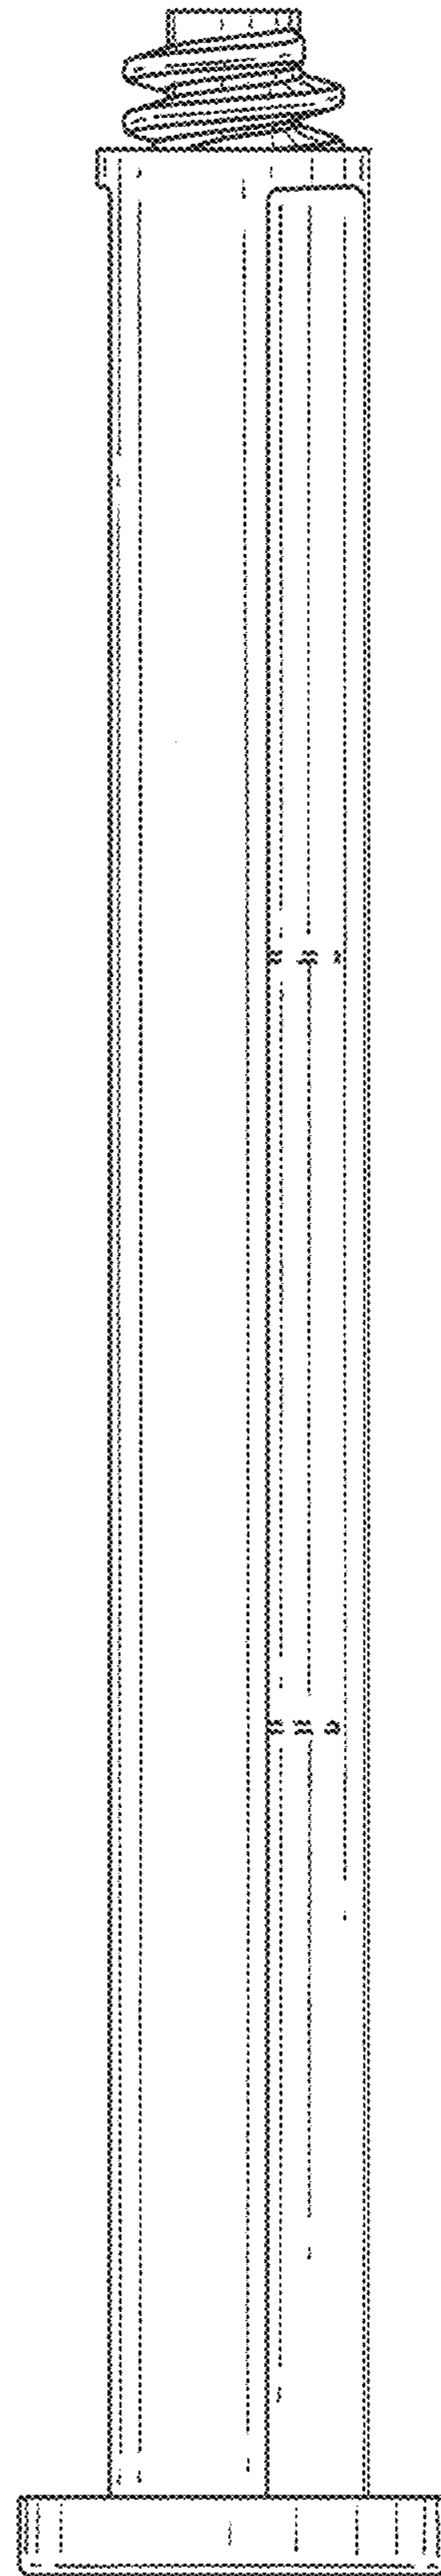


FIG. 7

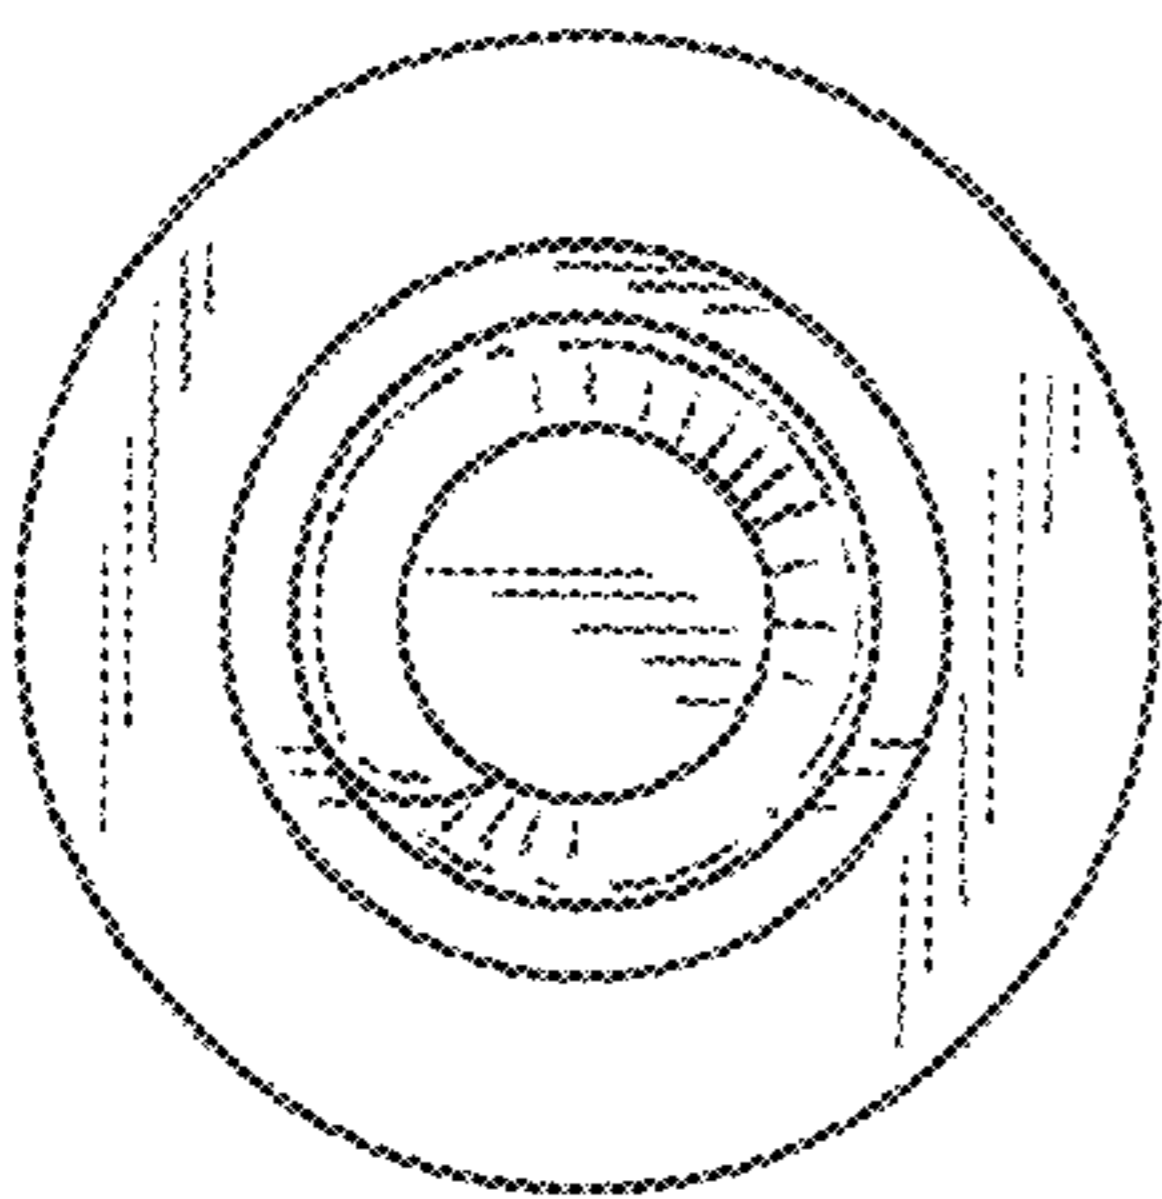


FIG. 8

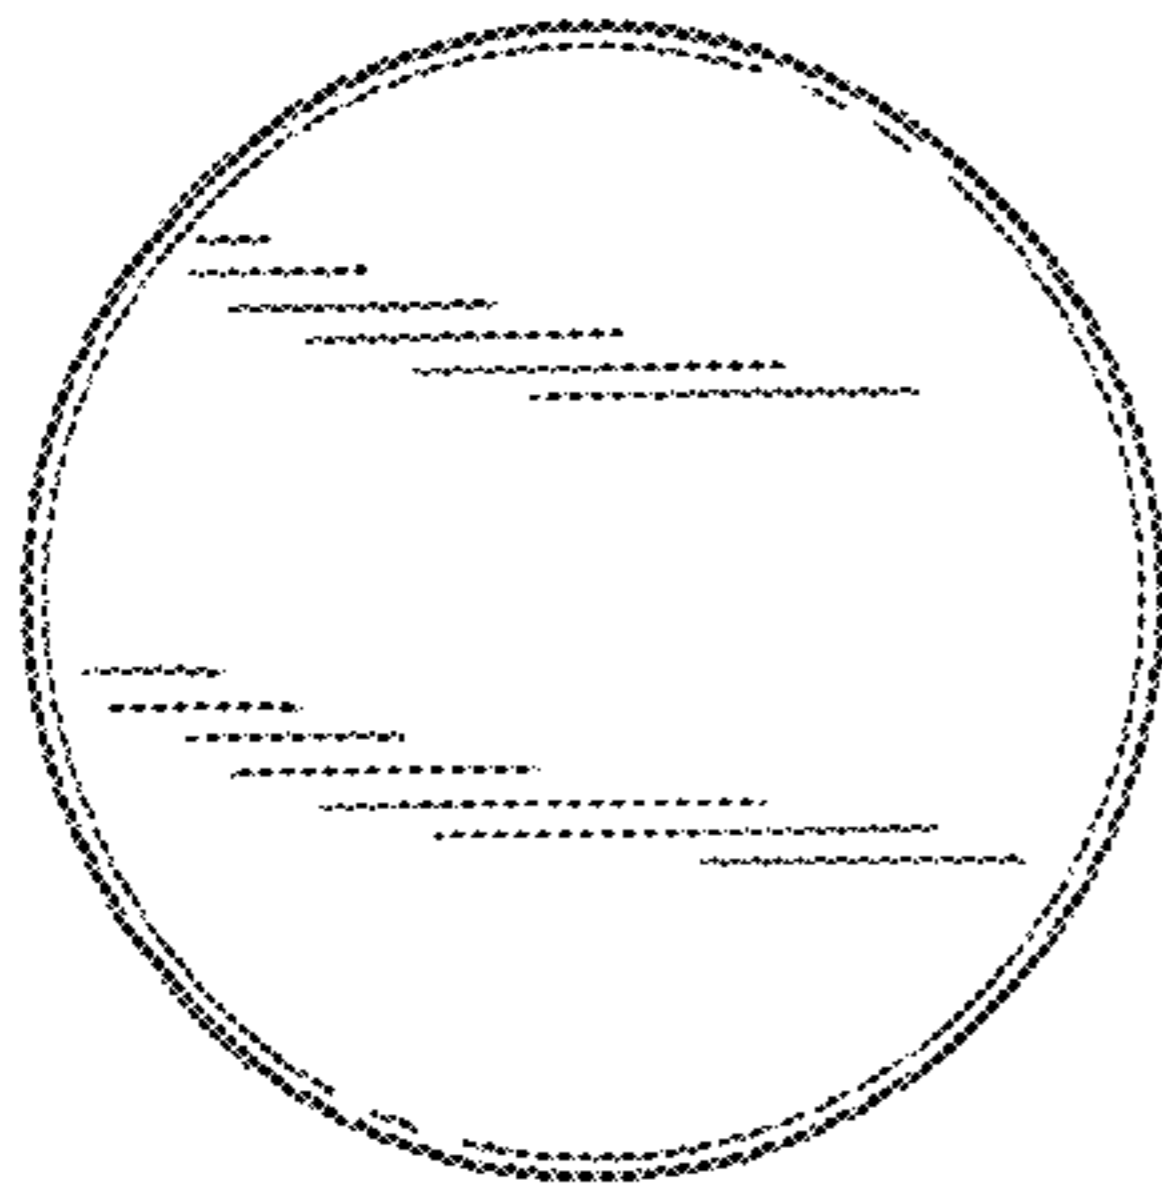


FIG. 9

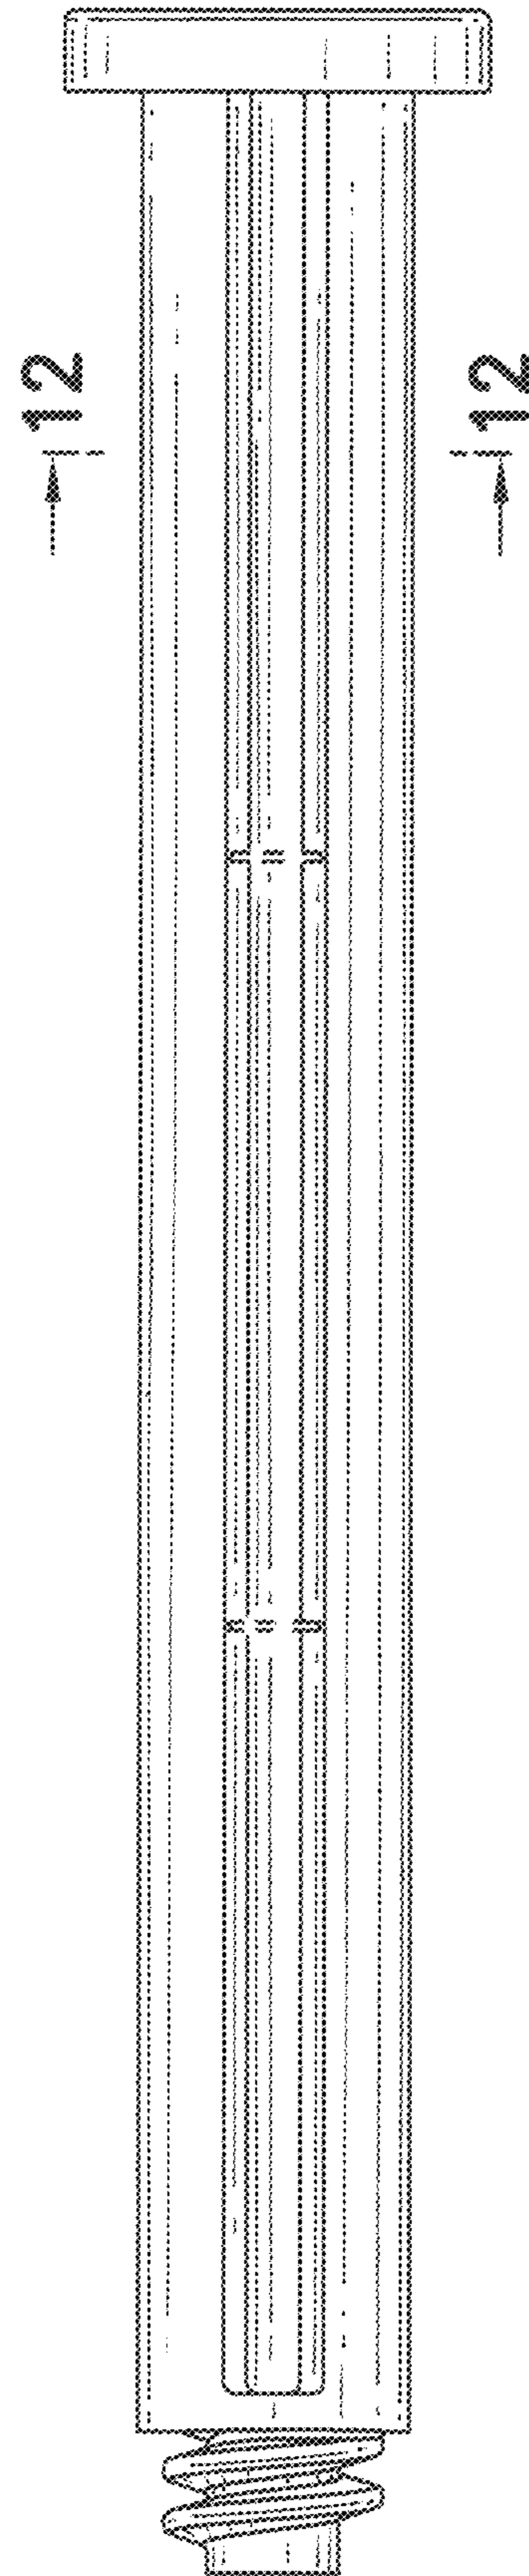


FIG. 10

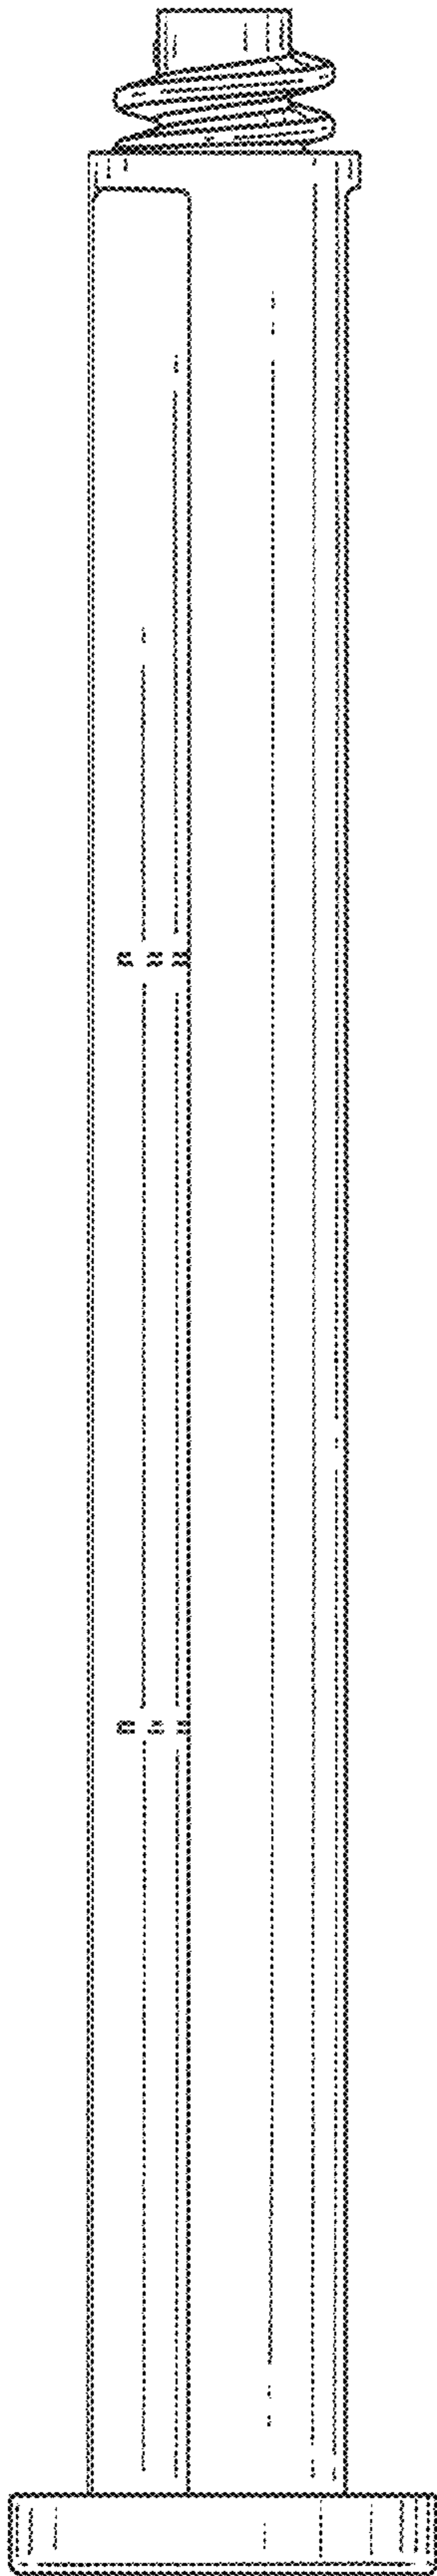


FIG. 11

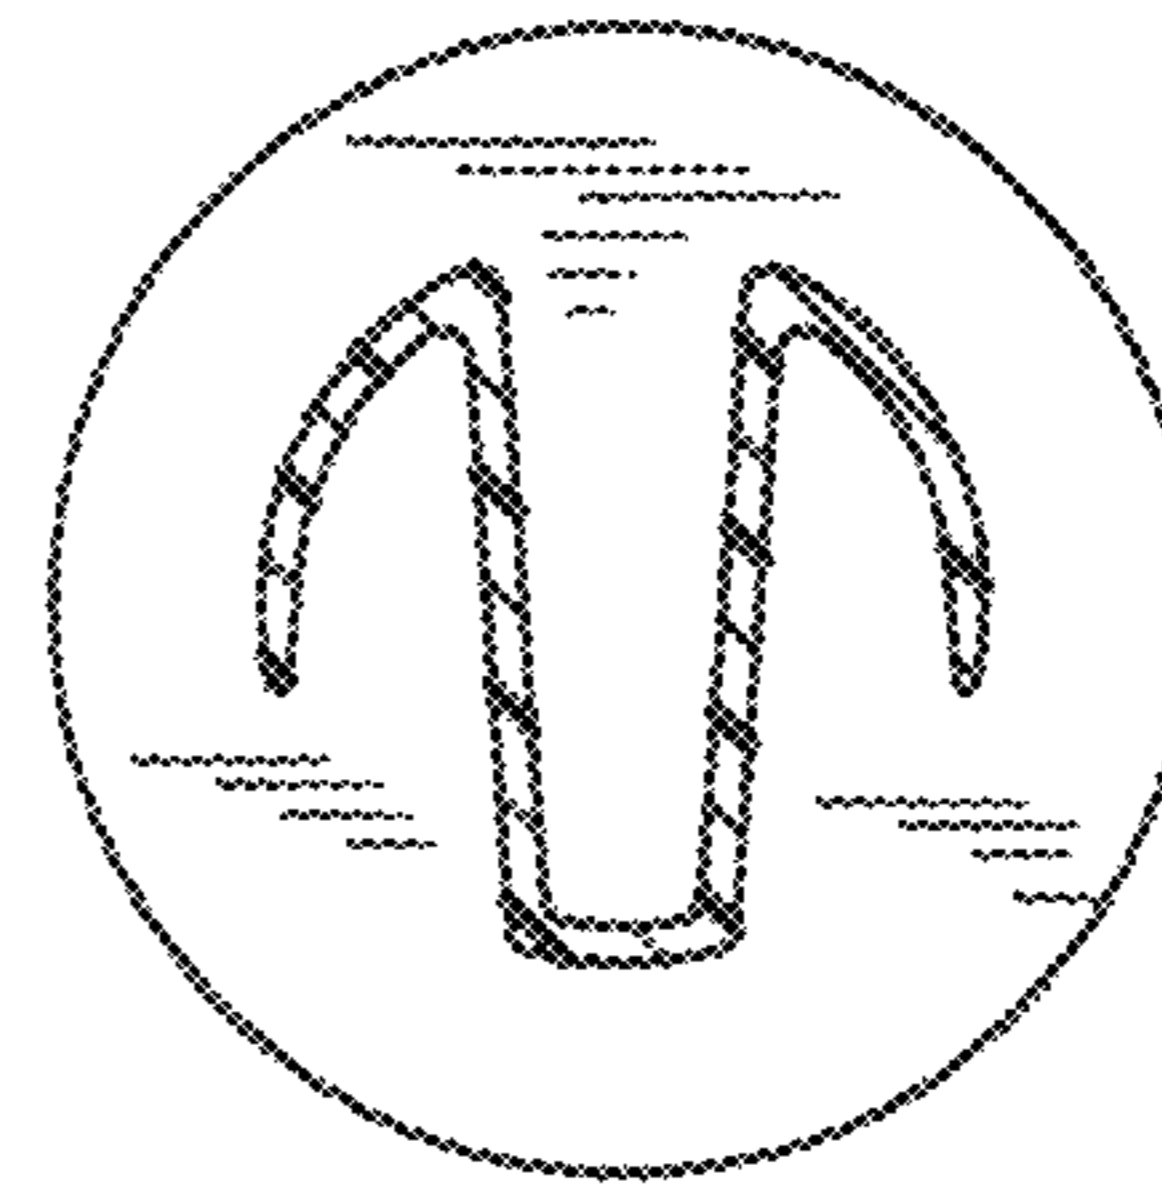


FIG. 12