



US00D939097S

(12) **United States Design Patent** (10) **Patent No.:** **US D939,097 S**  
**Zou** (45) **Date of Patent:** **\*\* Dec. 21, 2021**

(54) **RED LIGHT THERAPY DEVICE**  
(71) Applicant: **SHENZHEN MORSEN LIGHTING TECHNOLOGY CO. LTD.**, Shenzhen (CN)  
(72) Inventor: **Chen Zou**, Shenzhen (CN)  
(73) Assignee: **SHENZHEN MORSEN LIGHTING TECHNOLOGY CO., LTD.**, Shenzhen (CN)

D877,921 S 3/2020 Nelson et al.  
D877,922 S 3/2020 Strahan et al.  
D877,923 S 3/2020 Strahan et al.  
D887,571 S \* 6/2020 Liu ..... D24/209  
2006/0229689 A1\* 10/2006 Ferguson ..... A61N 5/0616  
607/88  
2007/0129777 A1\* 6/2007 Bolta ..... A61N 5/0618  
607/88  
2012/0104977 A1\* 5/2012 McKenzie ..... A01G 7/045  
315/312  
2018/0236259 A1\* 8/2018 Nelson ..... A61N 5/0616

(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/741,780**  
(22) Filed: **Jul. 15, 2020**  
(51) **LOC (13) Cl.** ..... **28-03**  
(52) **U.S. Cl.**  
USPC ..... **D24/210**  
(58) **Field of Classification Search**  
USPC ..... D24/107, 200, 209, 210, 214, 215;  
D26/37-39, 76, 104, 106, 120  
CPC .... A61N 5/062; A61N 5/0614; A61N 5/0616;  
A61N 5/0617; A61N 5/0618; A61N  
5/0624; A61N 5/0627; A61N 5/0625;  
A61N 2005/0643; A61N 2005/0644;  
A61N 2005/0645; A61N 2005/0647;  
A61N 2005/0651; A61N 2005/0652;  
A61N 2005/0654; A61N 2005/0662;  
A61B 2018/00452; A61B 2018/1807  
See application file for complete search history.

**OTHER PUBLICATIONS**

Bestqool Red Light Therapy Device, 660&850nm Near Infrared Light Therapy with Timer, 60 LEDs, Clinical Grade High Power LED Light Therapy Lamp for Anti-Aging, Pain Relief. Product first available on Nov. 23, 2019. Amazon.com.\*

\* cited by examiner

*Primary Examiner* — Anhdao Doan  
(74) *Attorney, Agent, or Firm* — Law Offices of Steven W. Weinrieb

(57) **CLAIM**

The ornamental design for a red light therapy device, as shown and described.


**DESCRIPTION**

FIG. 1 is a front, right side, top perspective view of a red light therapy device showing my new design;  
FIG. 2 is a rear, left side, bottom perspective view thereof;  
FIG. 3 is a front elevational view thereof;  
FIG. 4 is a rear elevational view thereof;  
FIG. 5 is a left side elevational view thereof;  
FIG. 6 is a right side elevational view thereof;  
FIG. 7 is a top plan view thereof; and,  
FIG. 8 is a bottom plan view thereof.  
The broken lines depict portions of the red light therapy device that form no part of the claimed design.

(56) **References Cited**  
U.S. PATENT DOCUMENTS

6,221,095 B1\* 4/2001 Van Zuylen ..... A61N 5/0616  
606/15  
D641,917 S \* 7/2011 Toratani ..... D26/106  
D700,973 S \* 3/2014 Douglas ..... D24/210  
D704,851 S \* 5/2014 Douglas ..... D24/209  
D865,256 S \* 10/2019 Zou ..... D26/71  
D877,920 S 3/2020 Nelson et al.

**1 Claim, 8 Drawing Sheets**

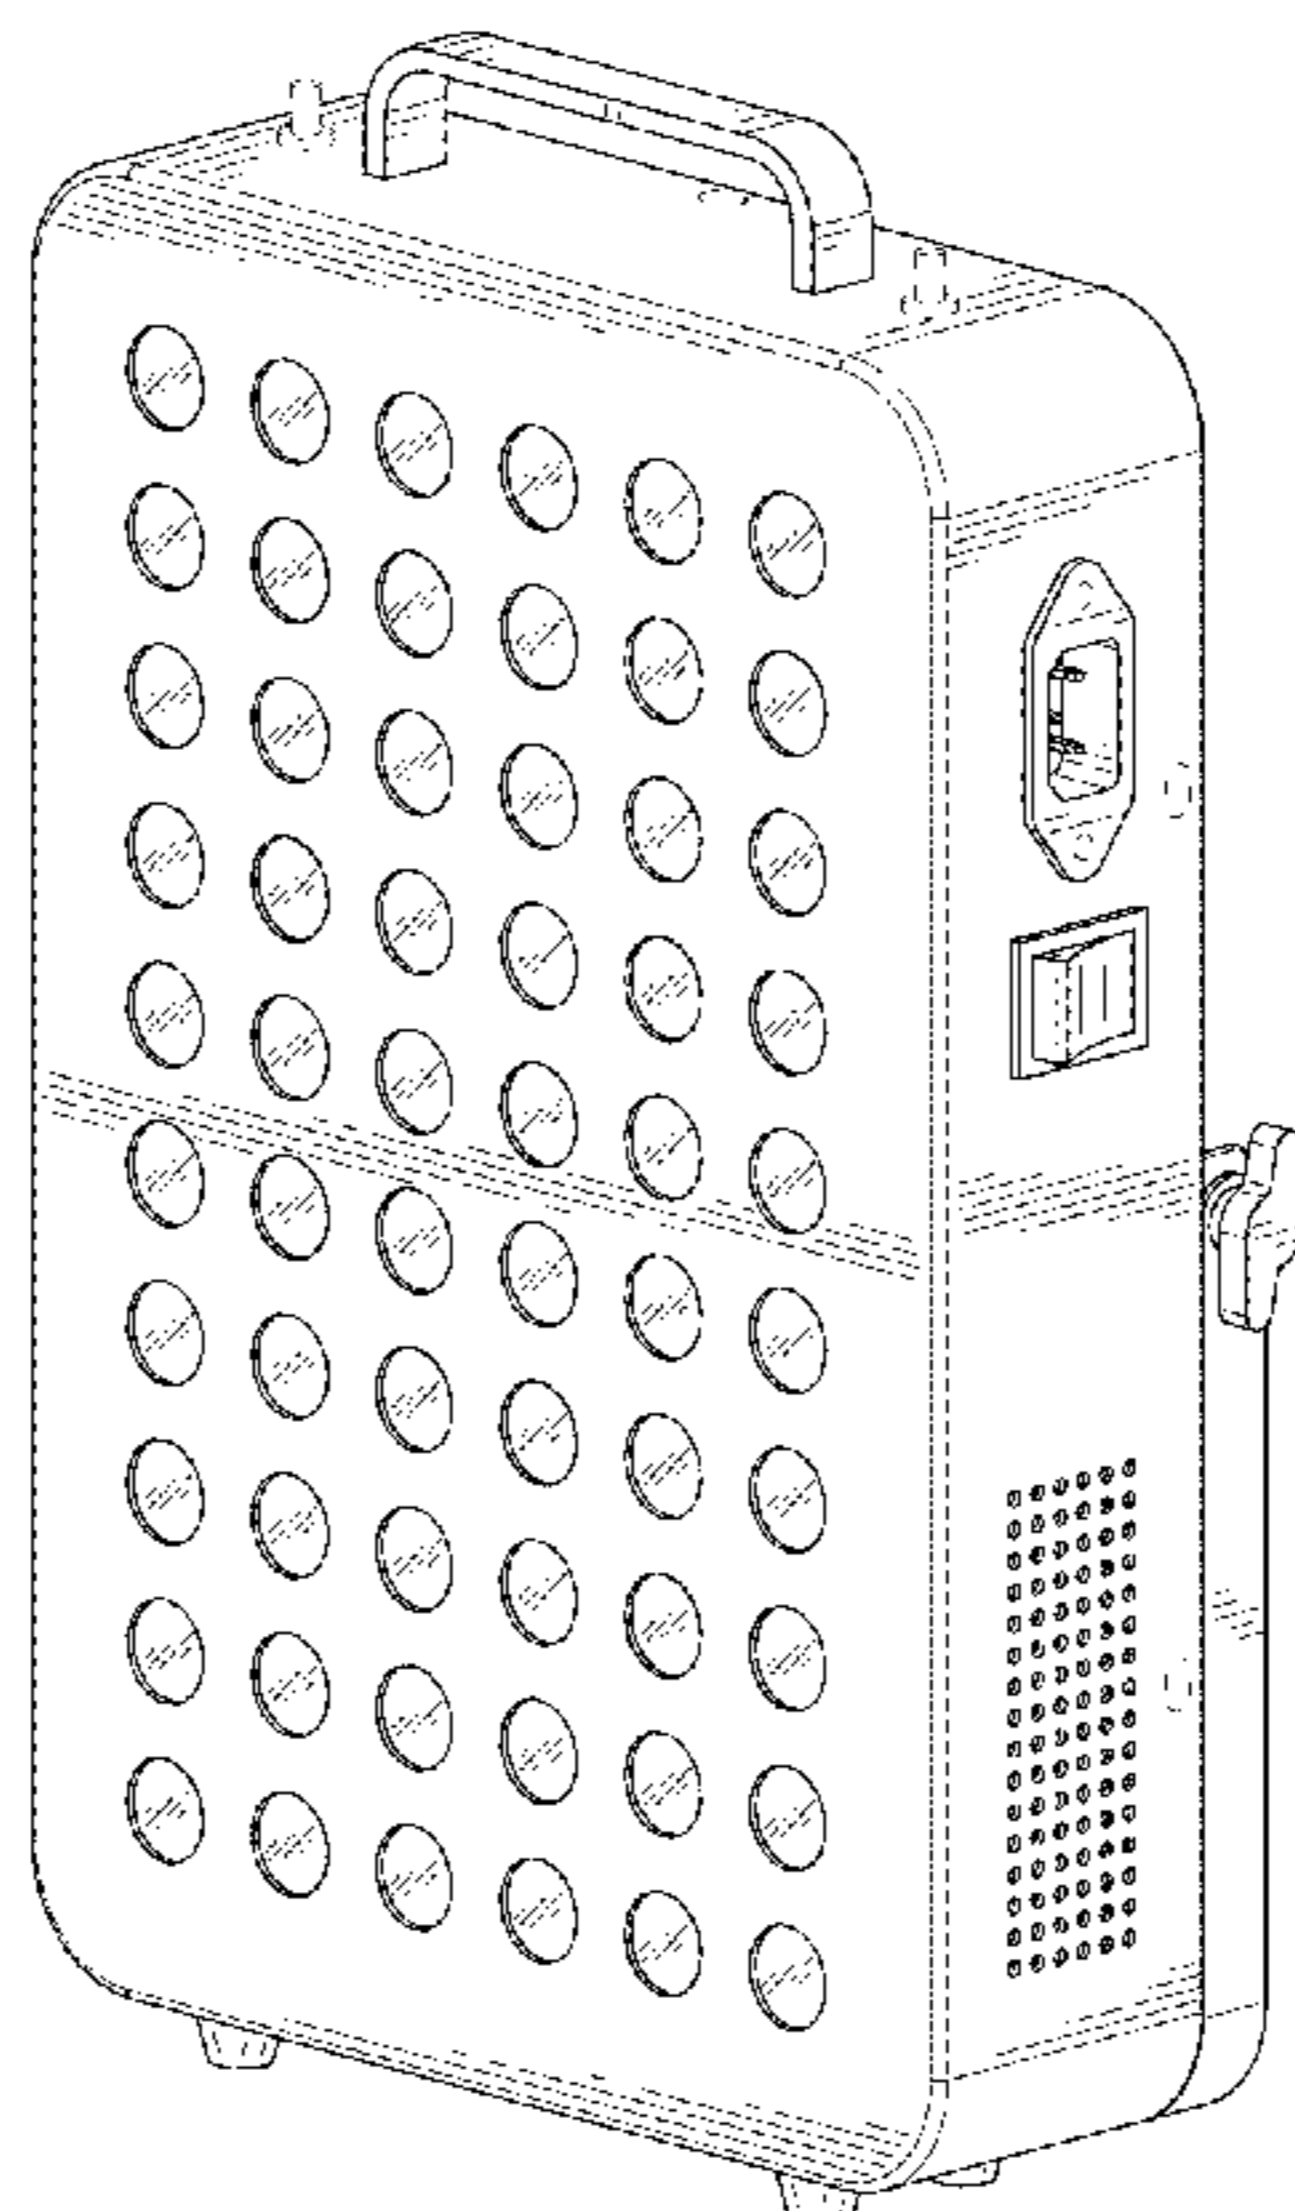

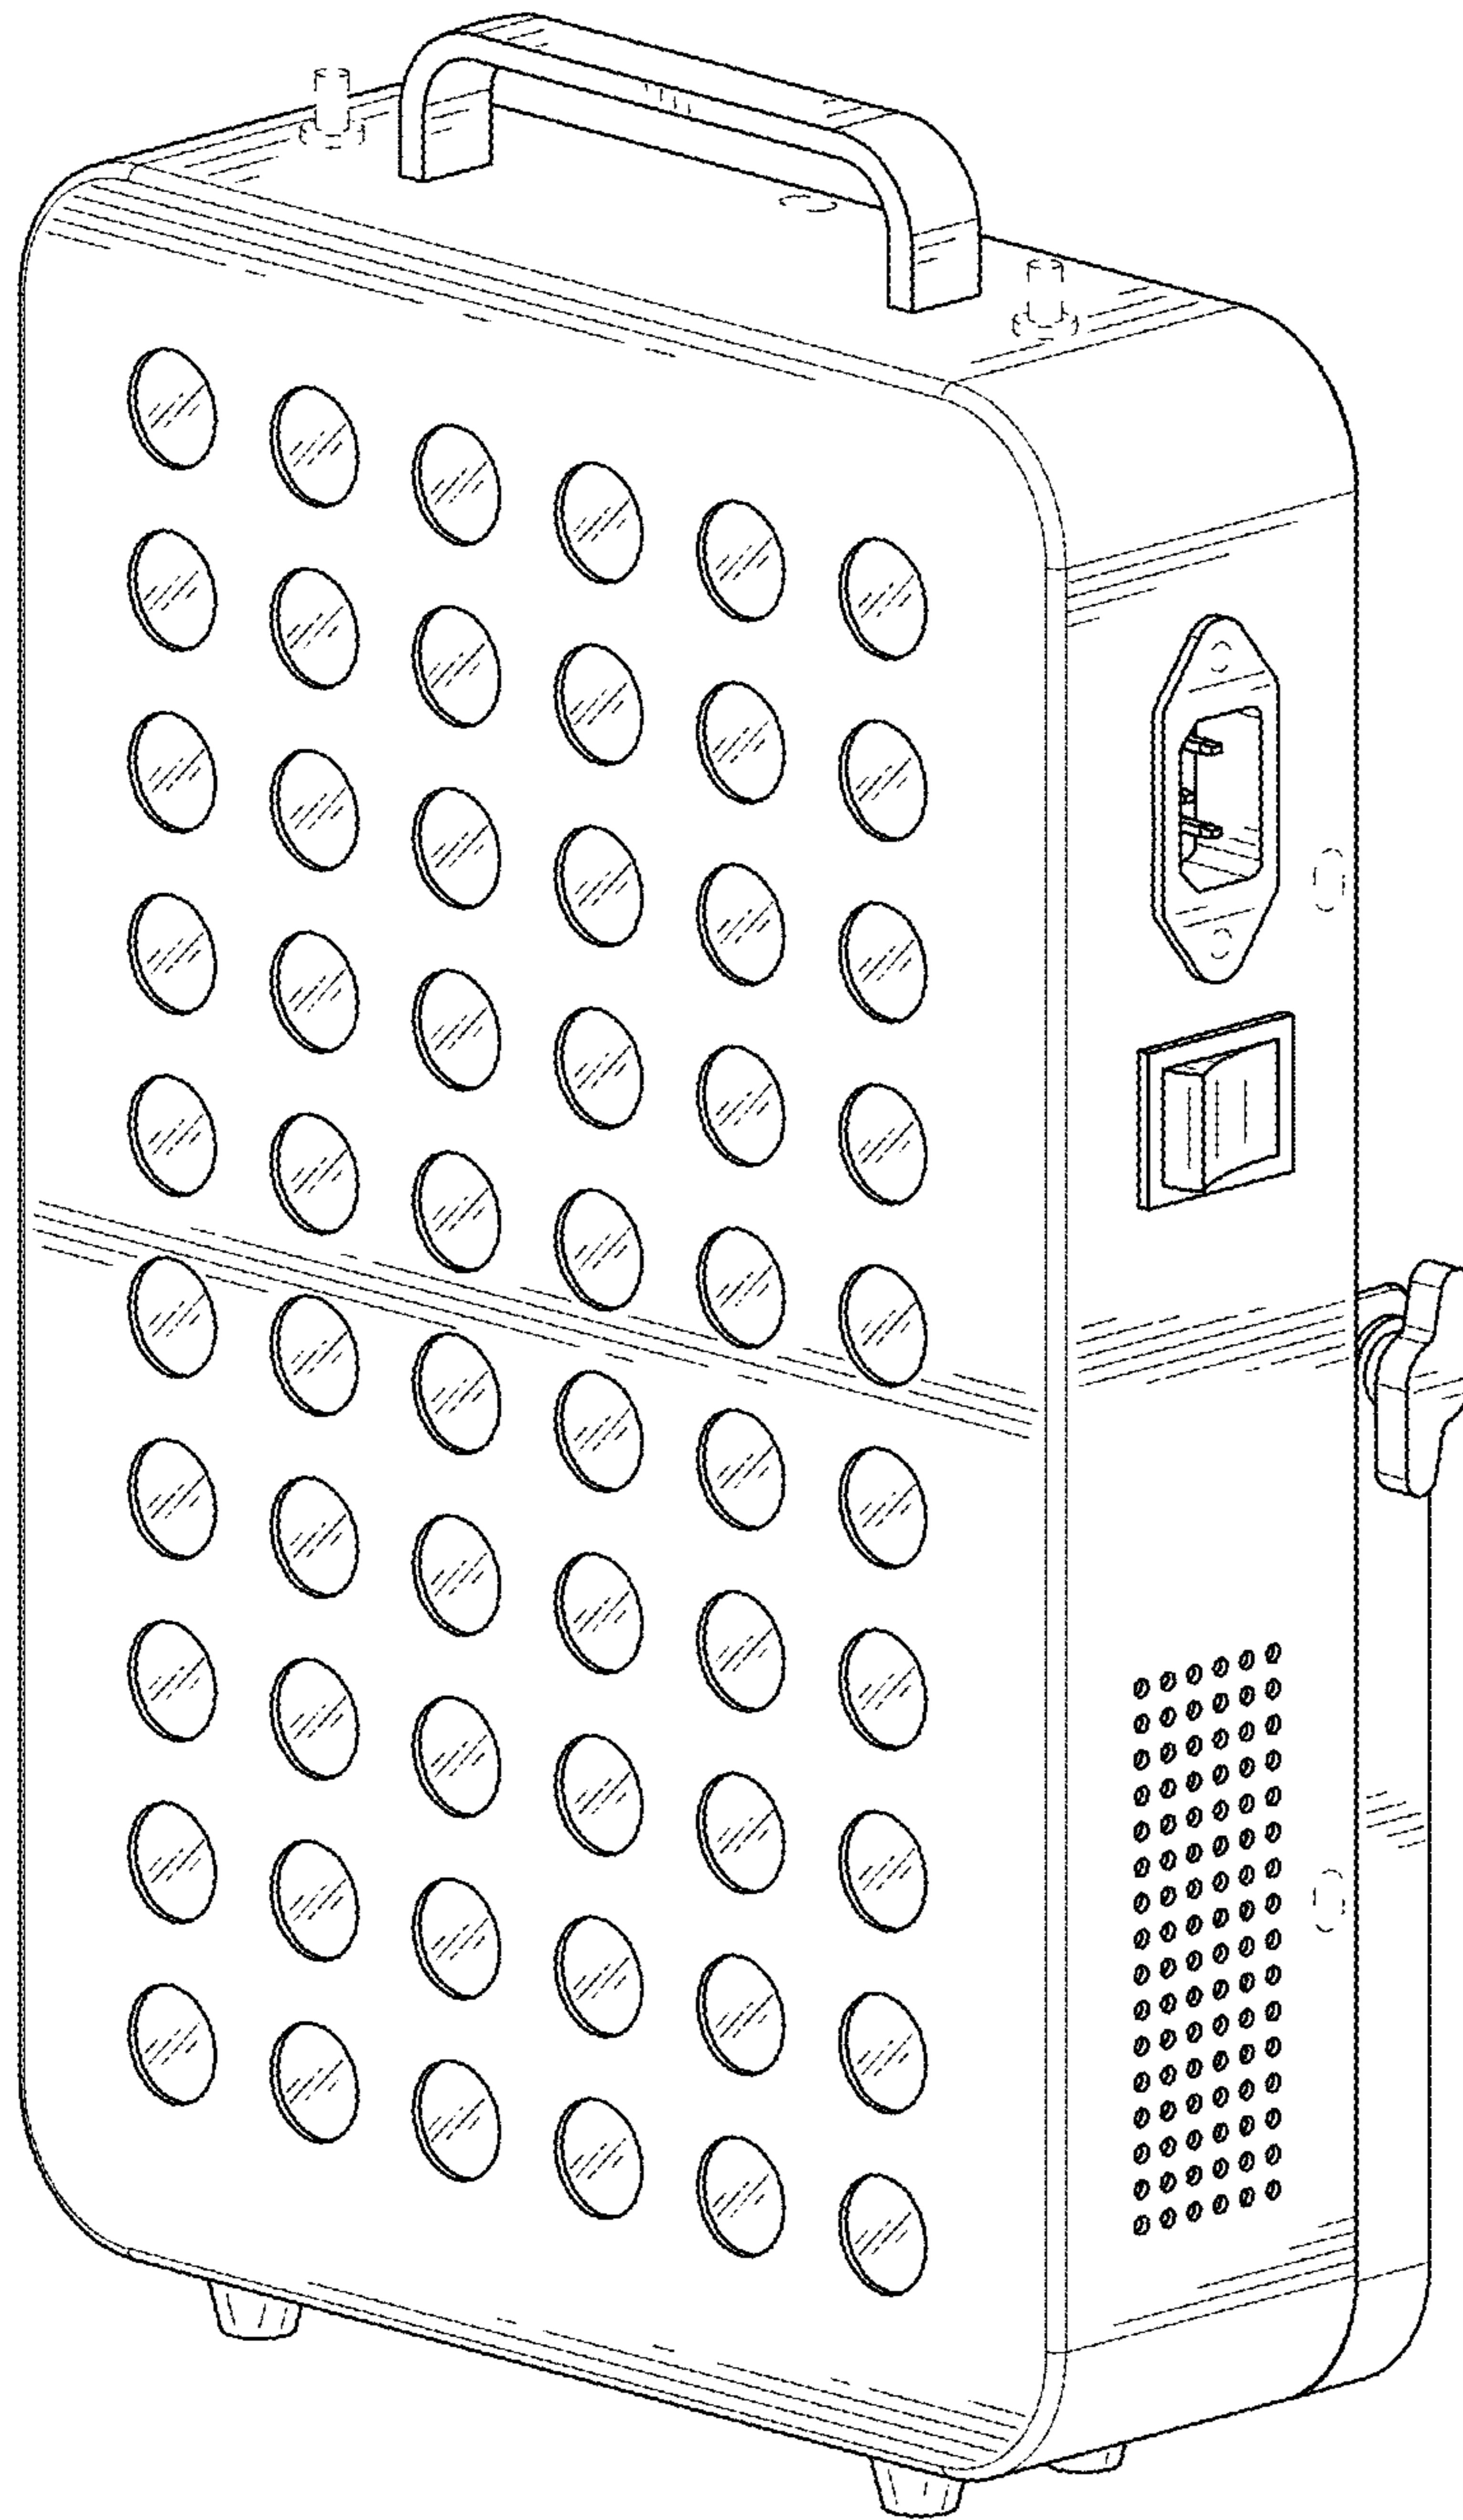


FIG.1

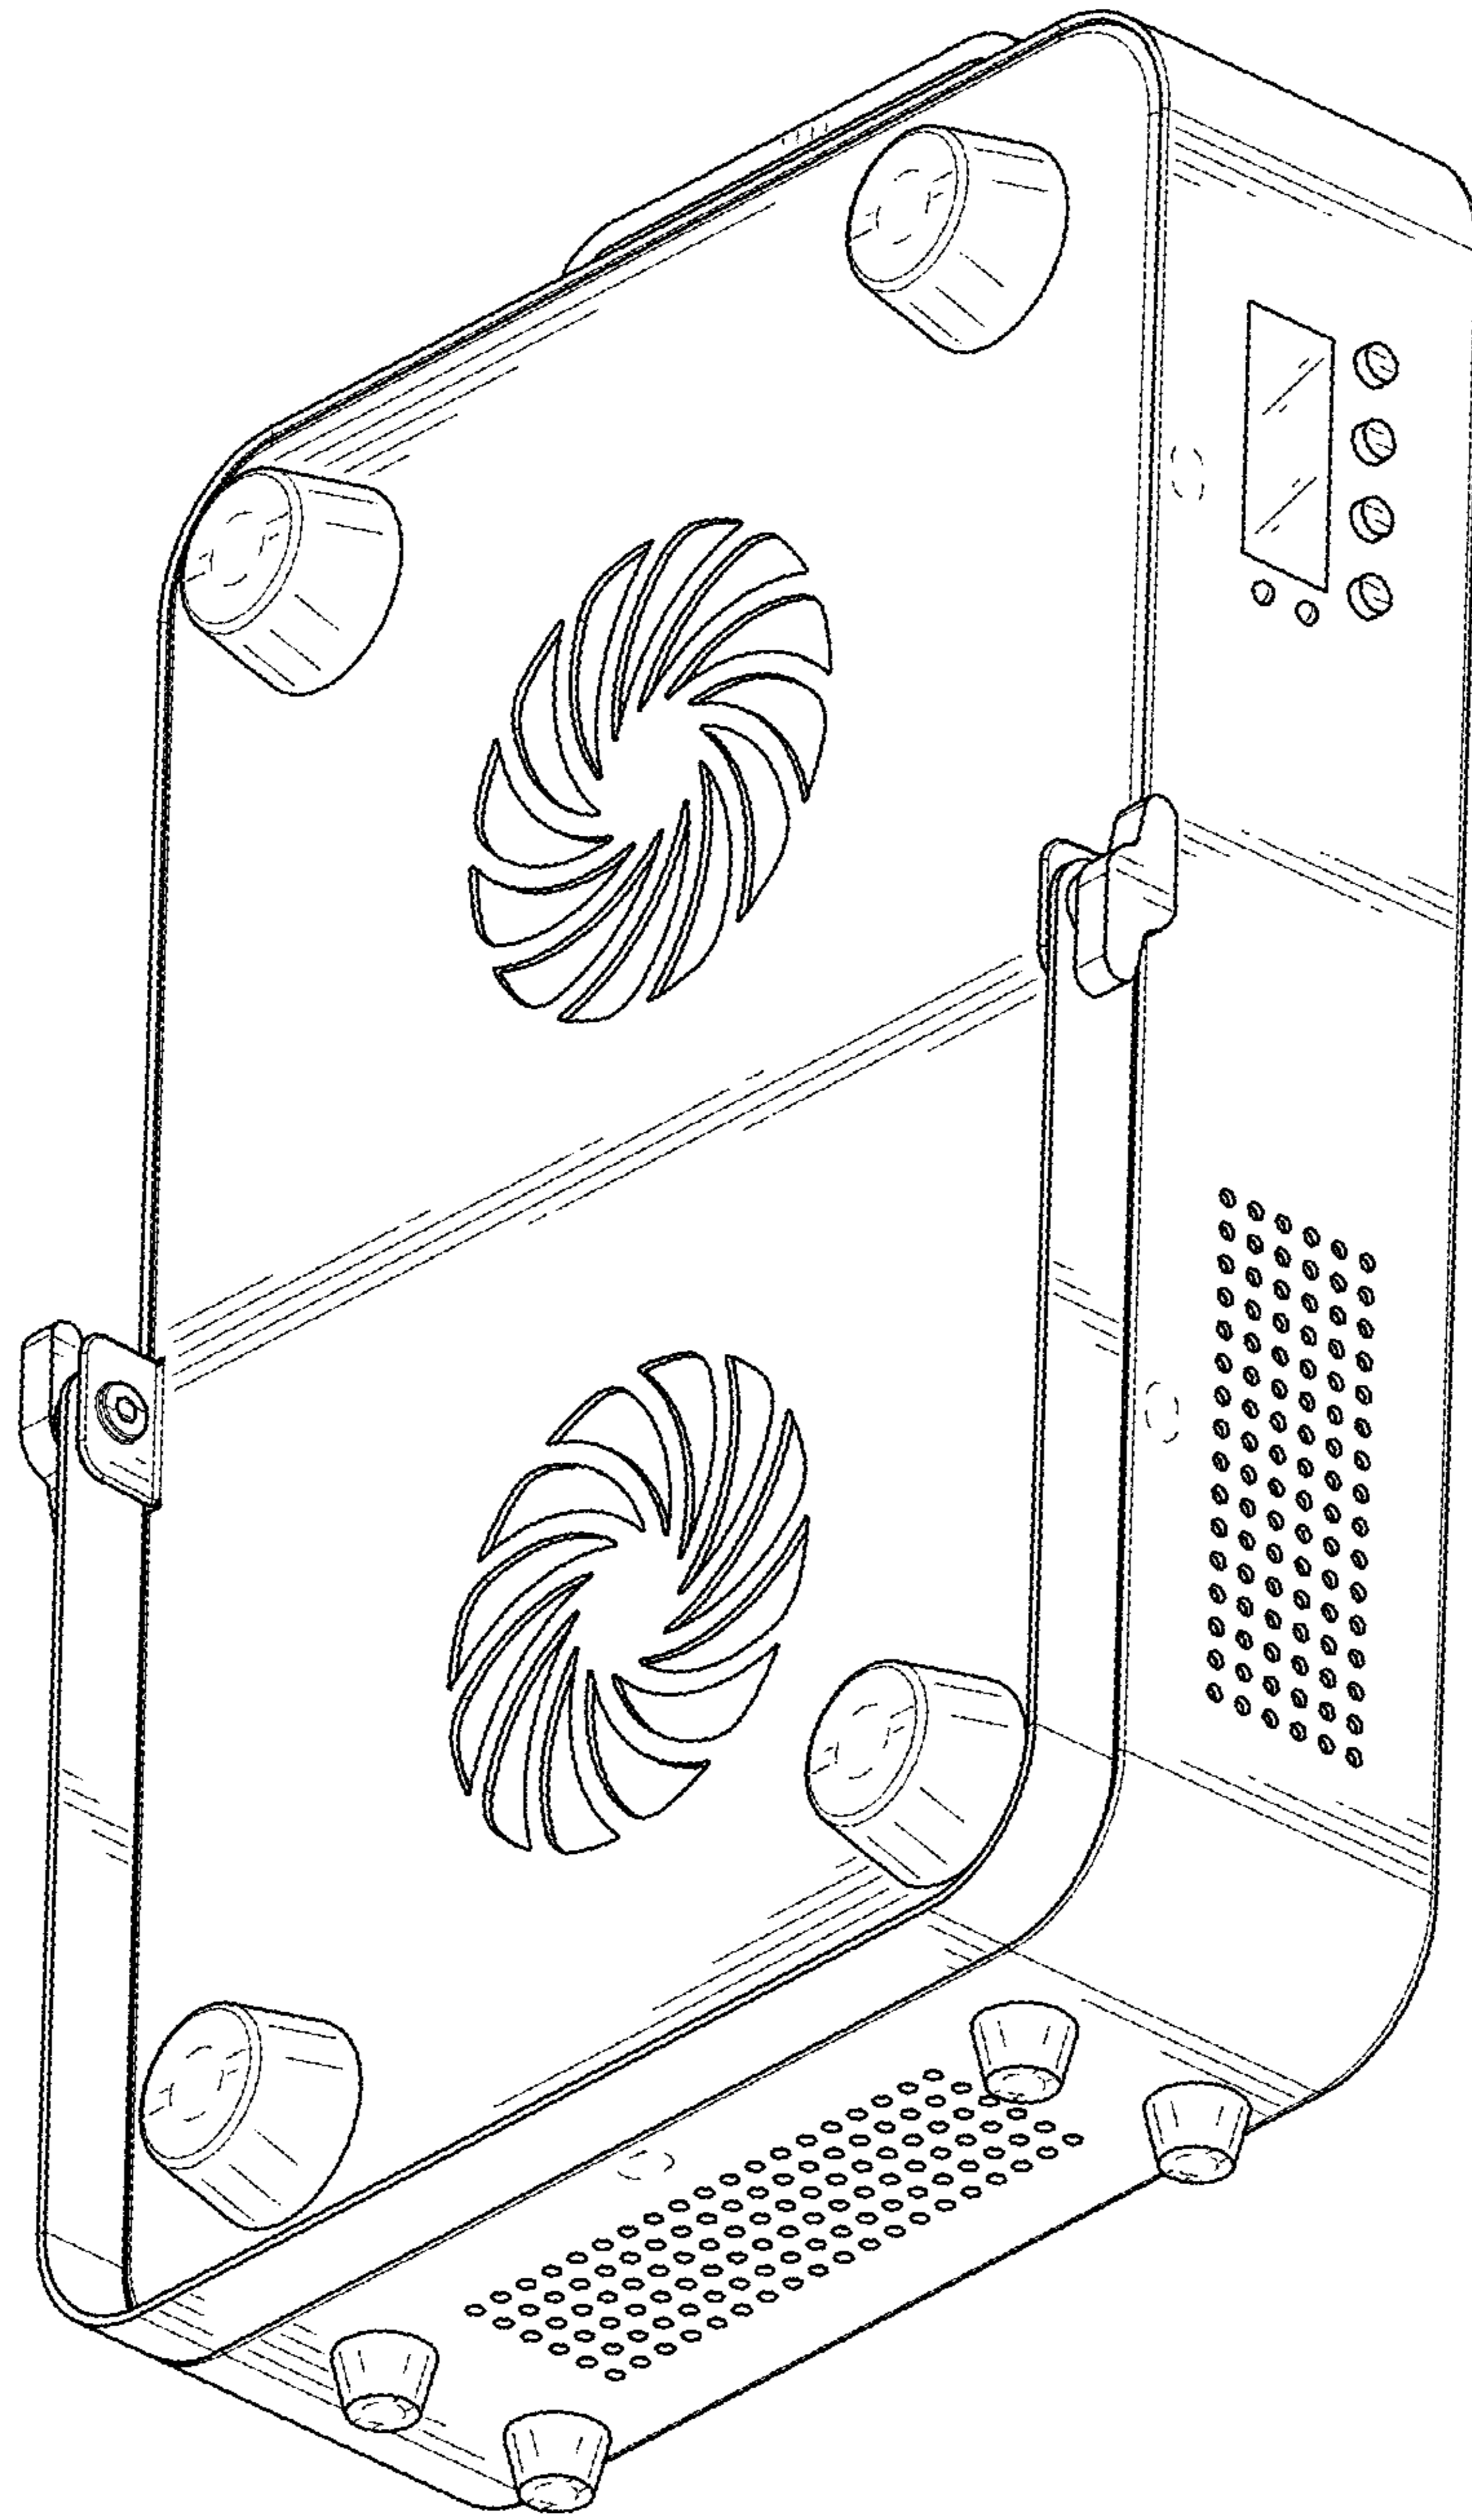


FIG.2

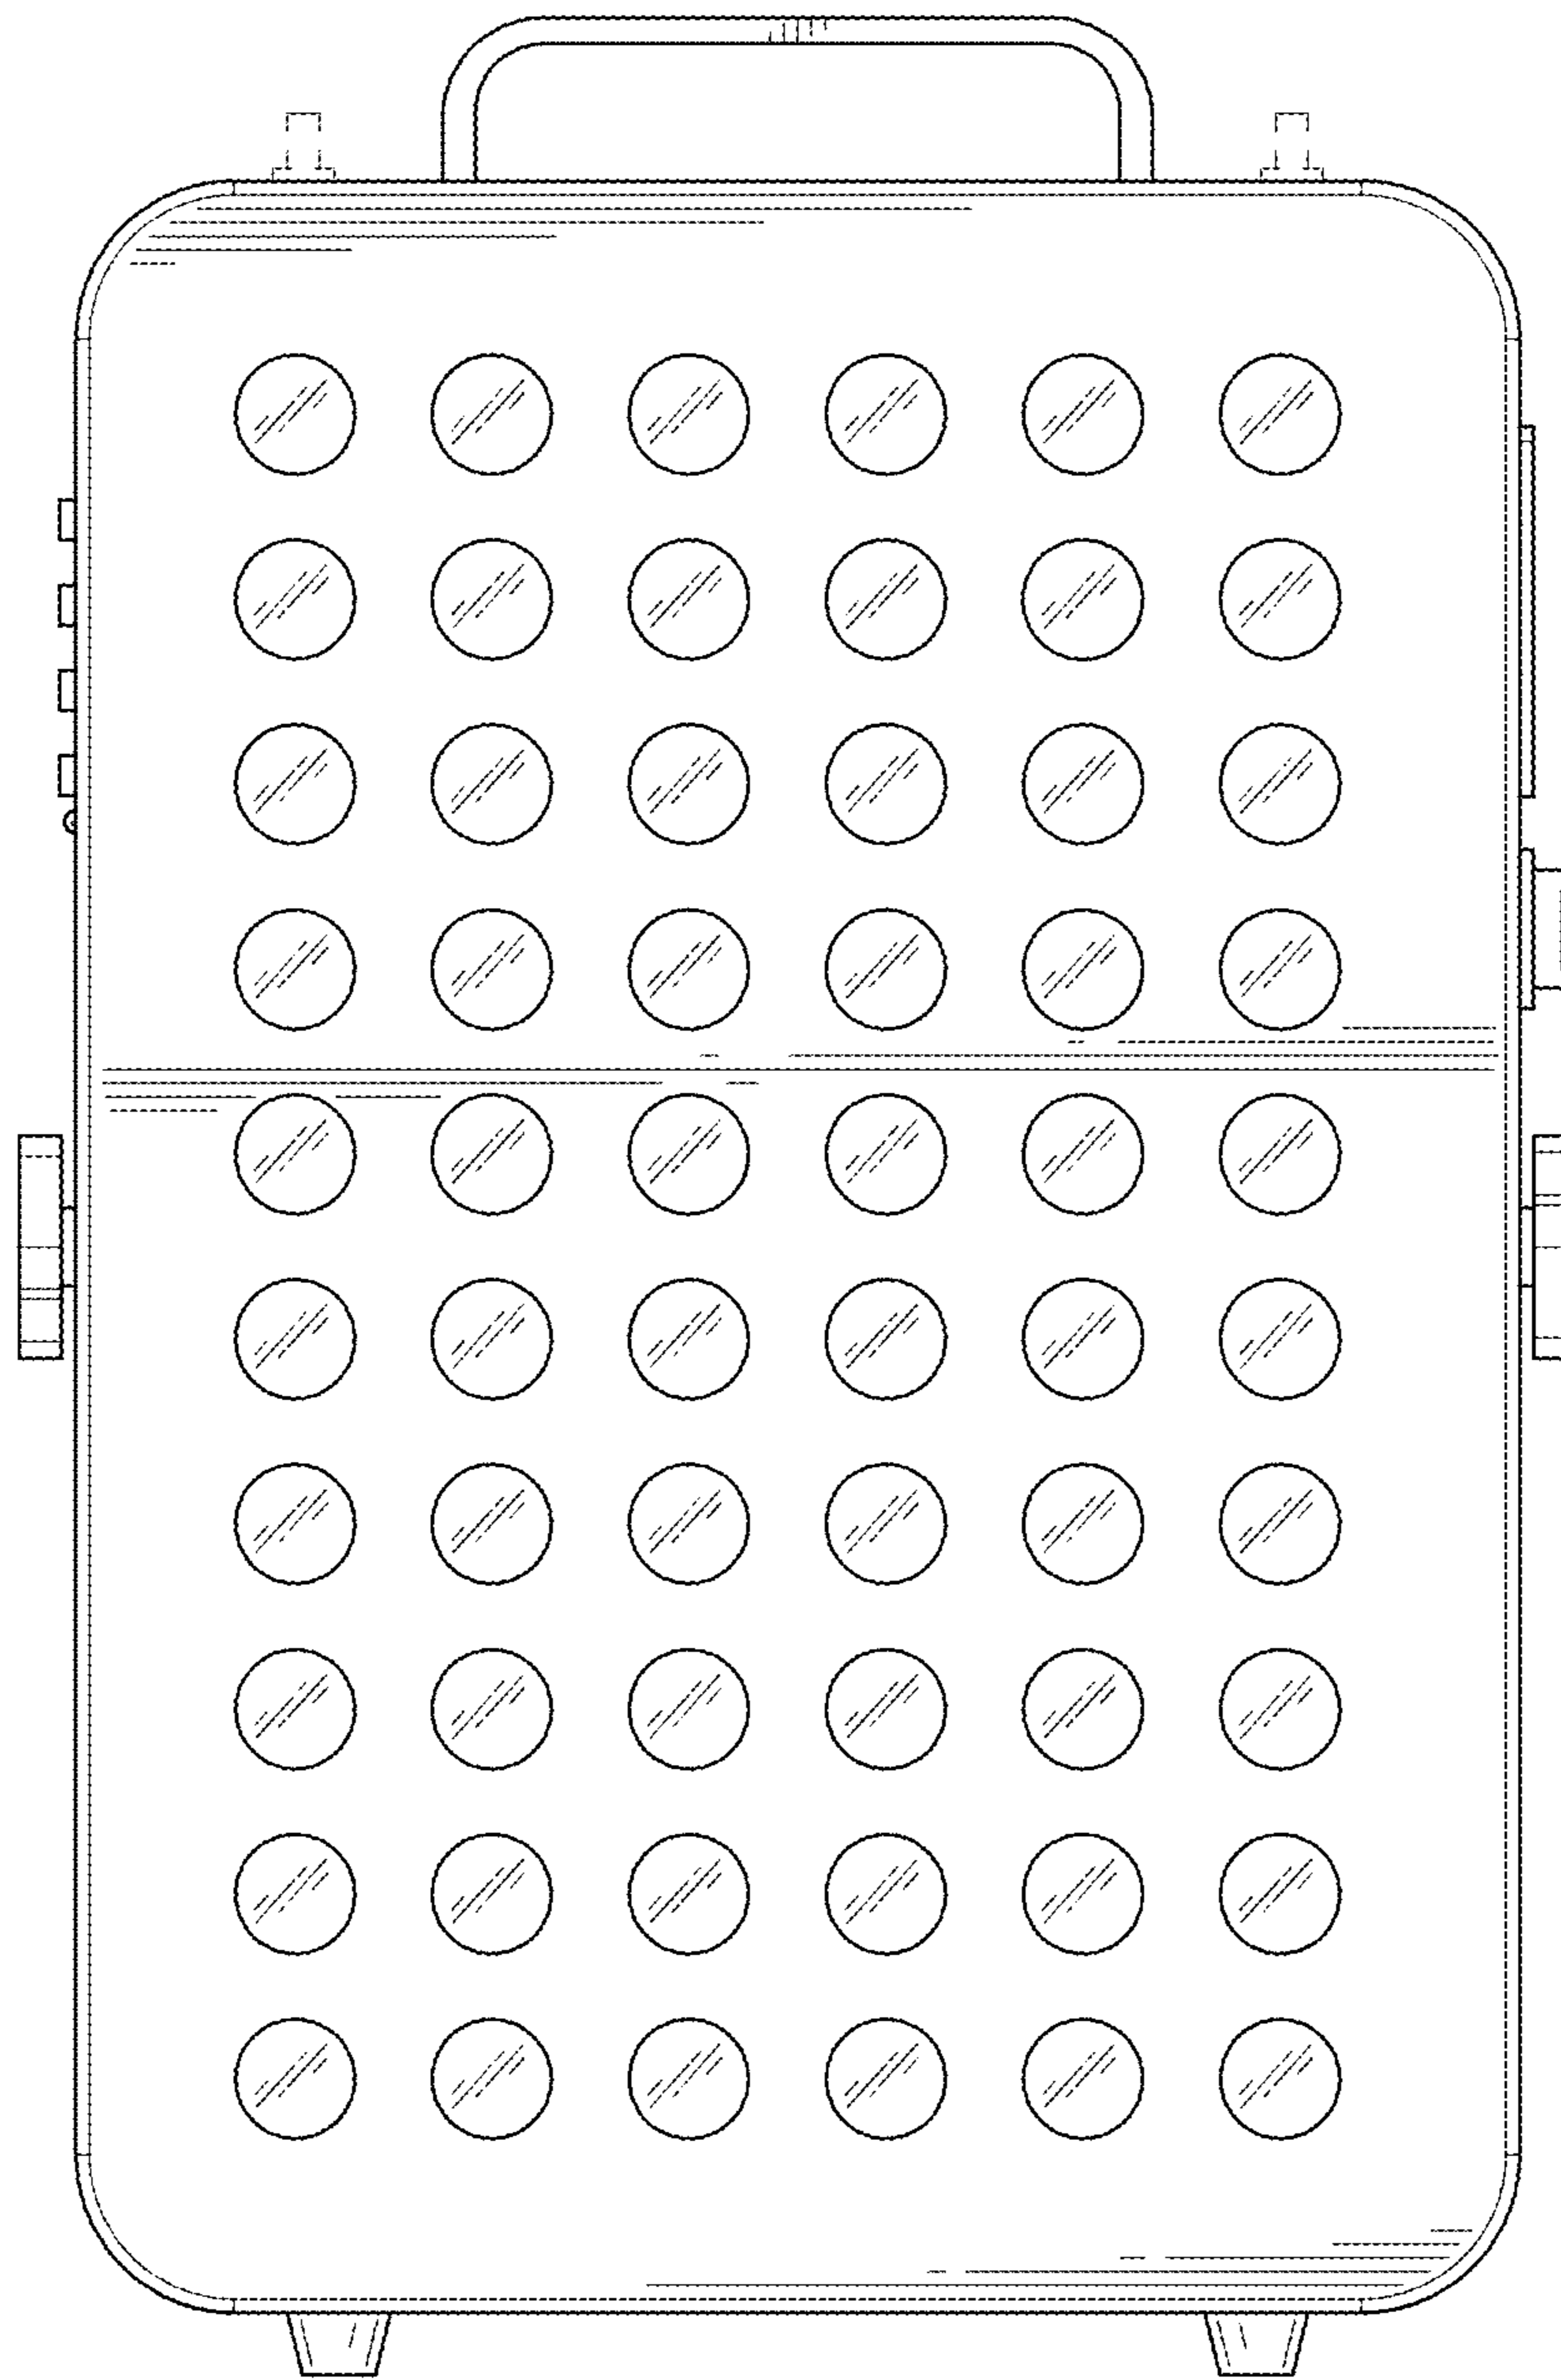


FIG. 3

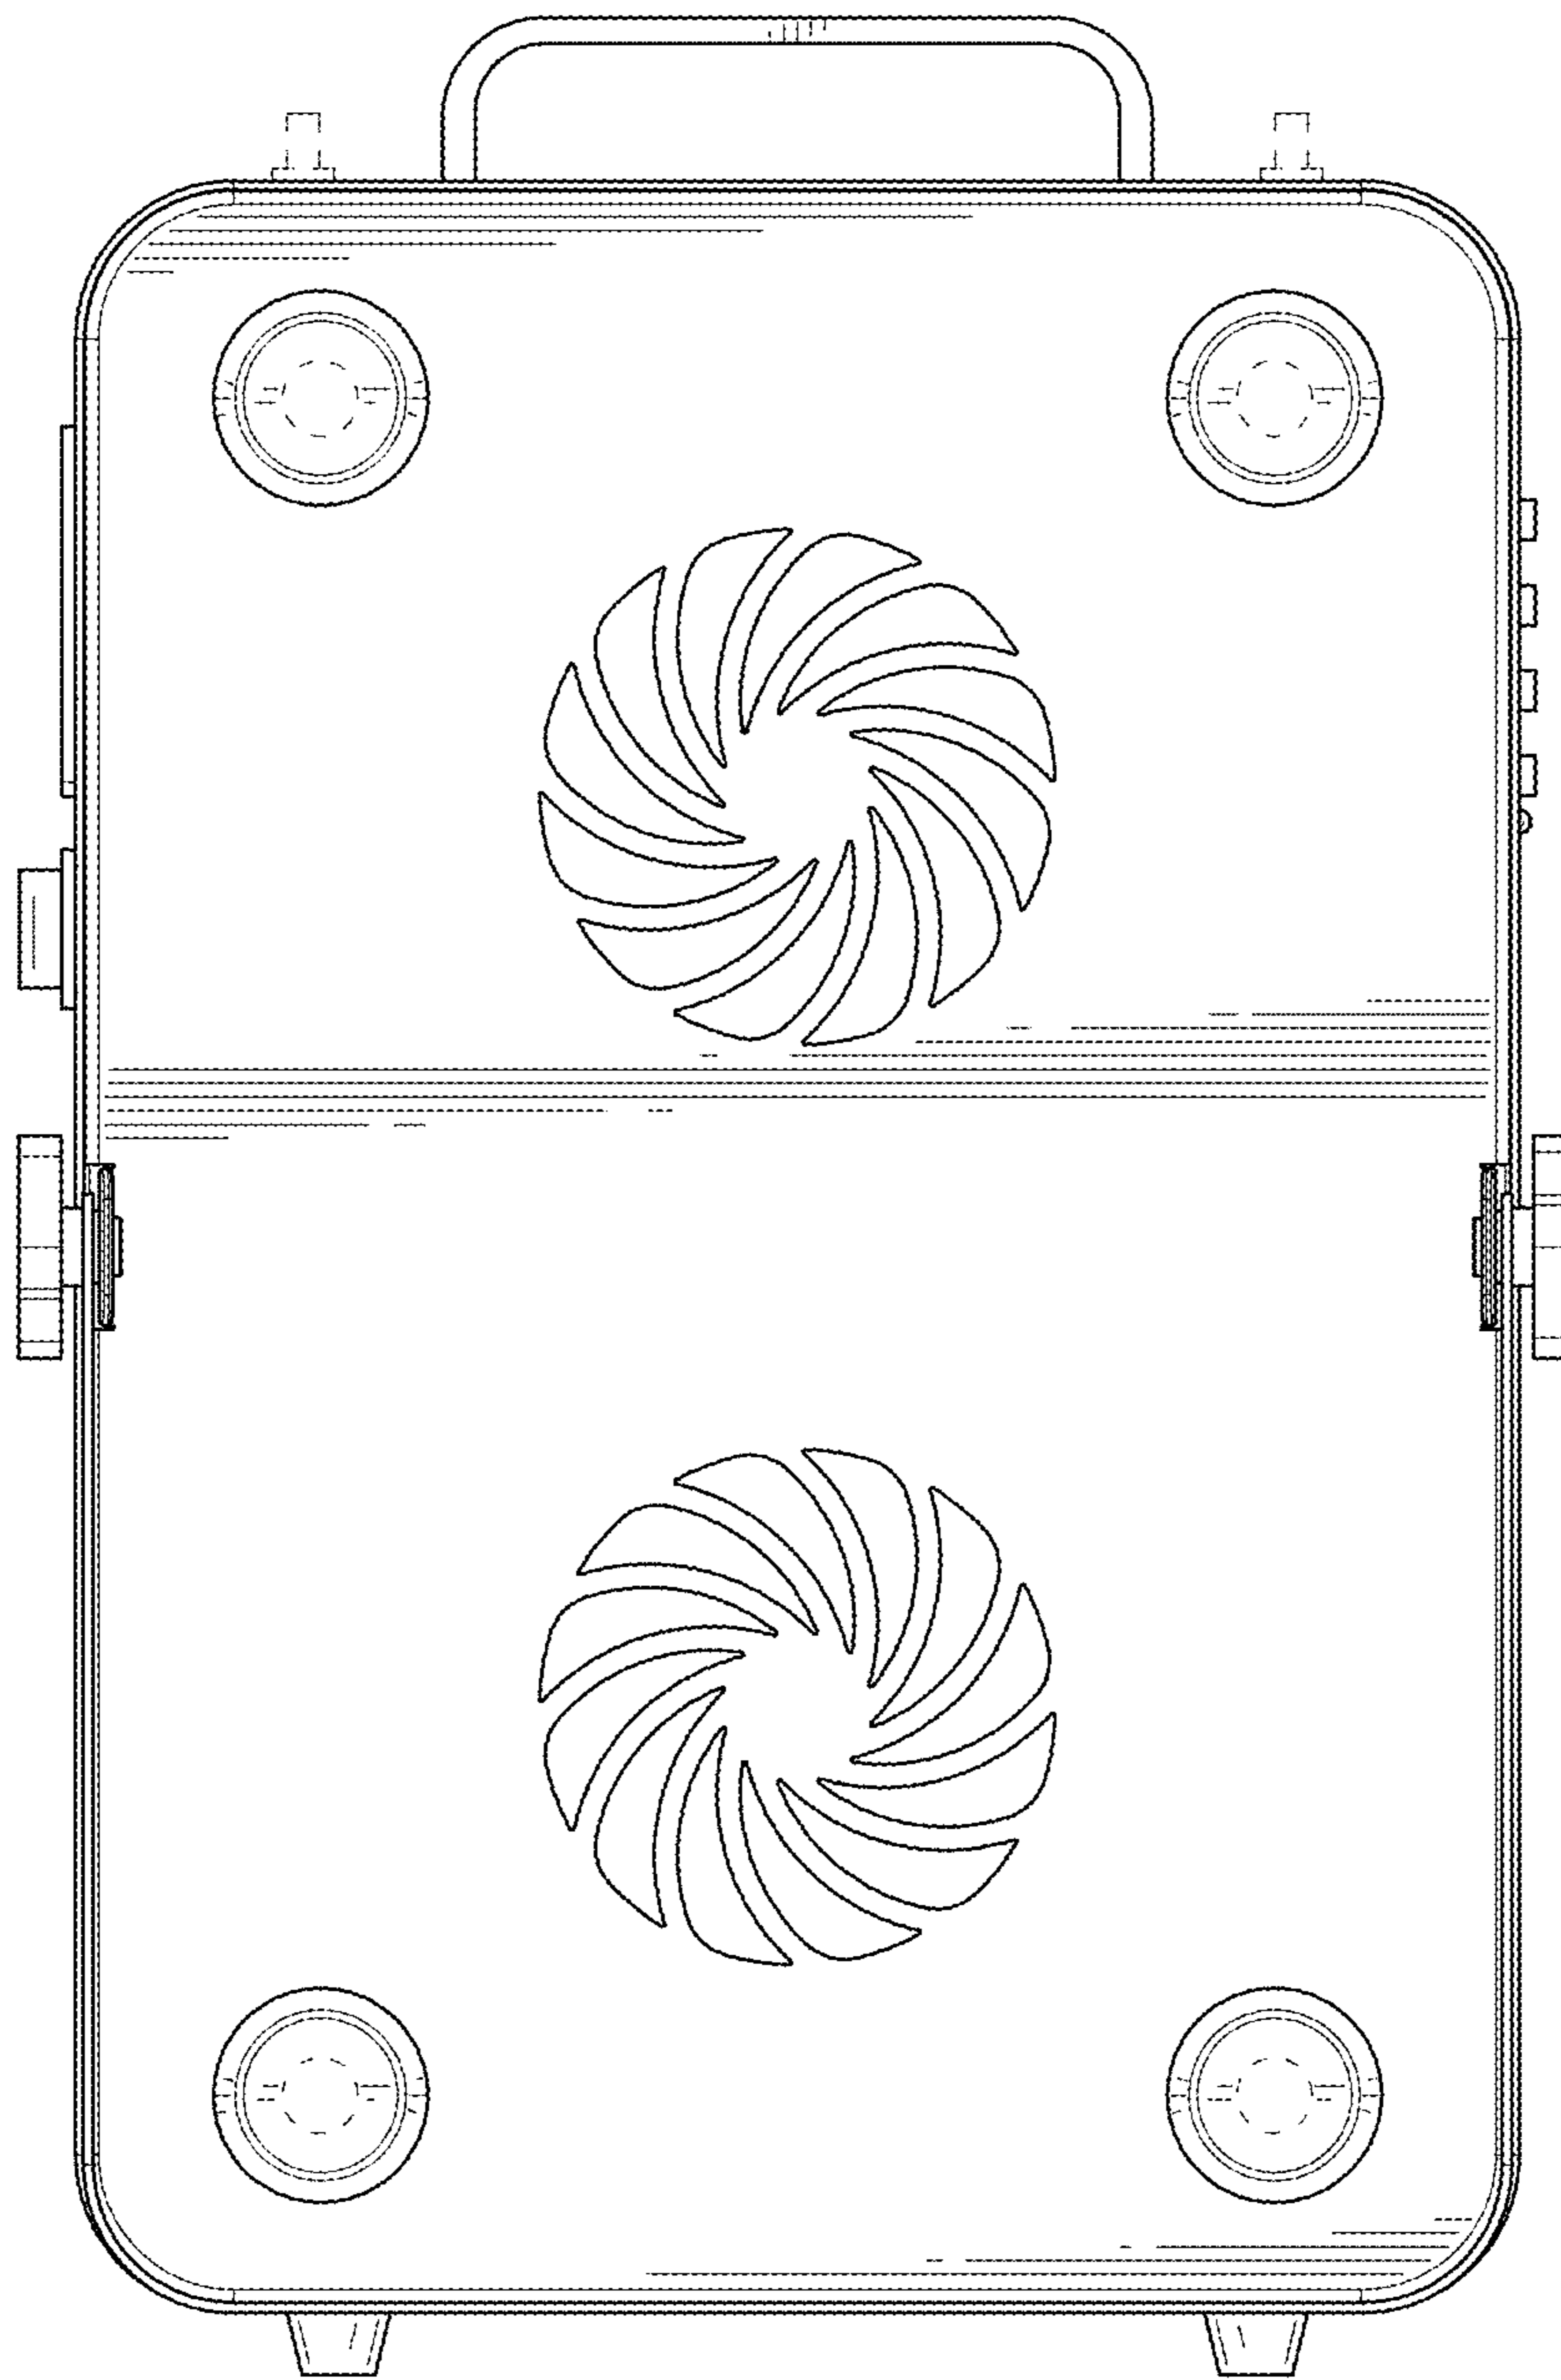


FIG.4

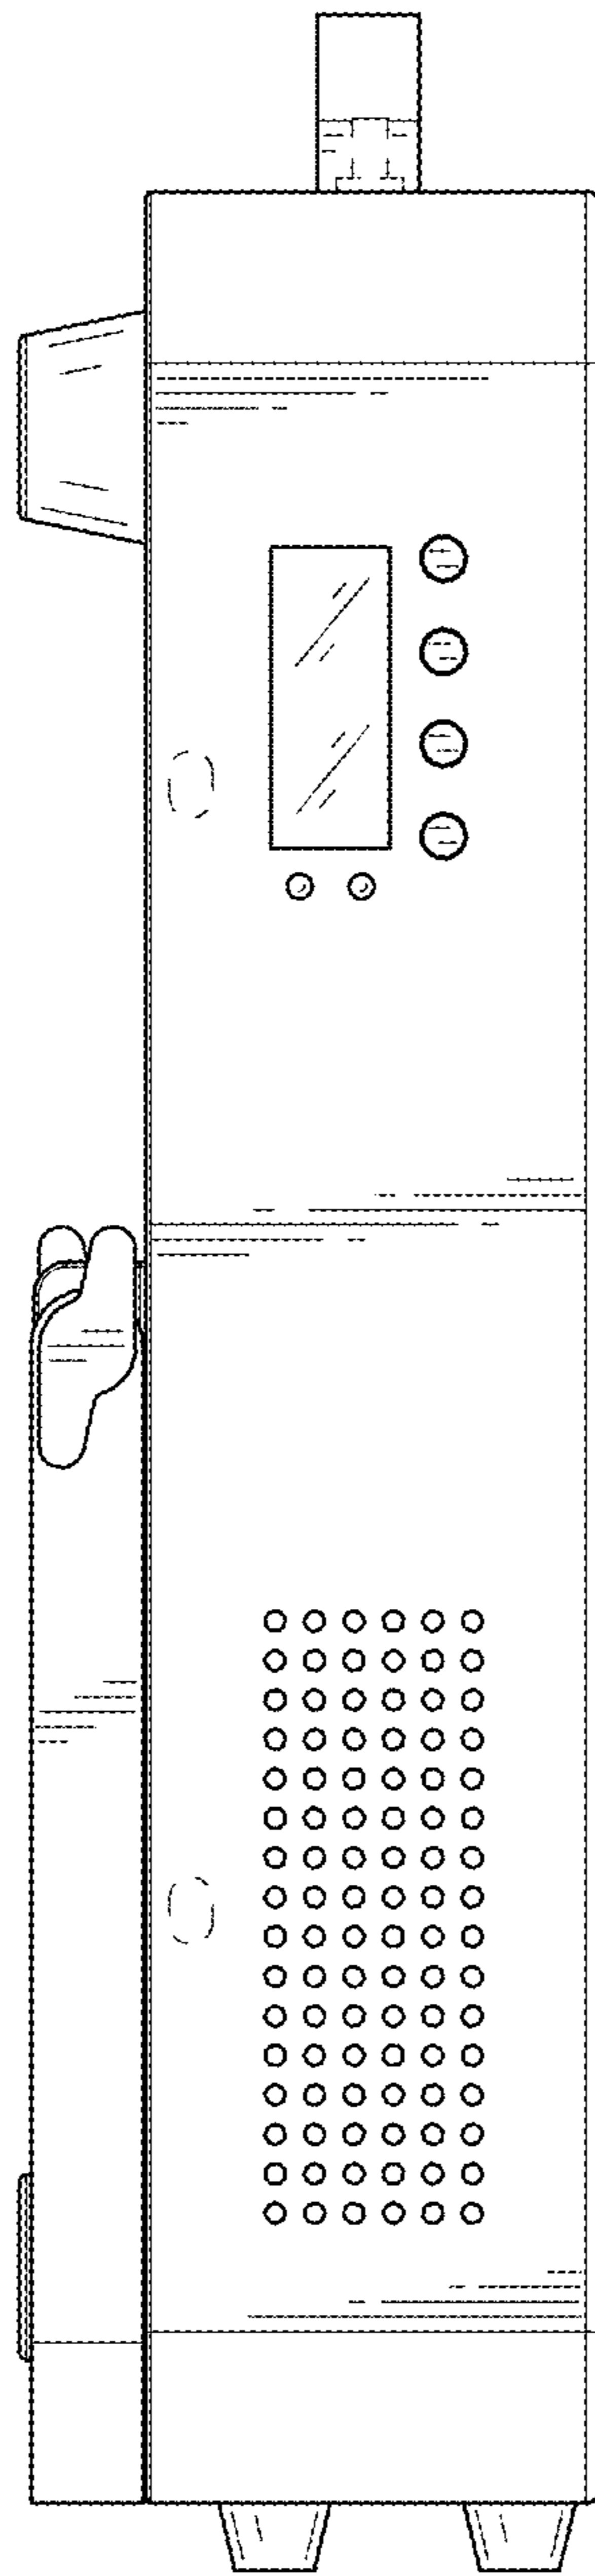


FIG.5

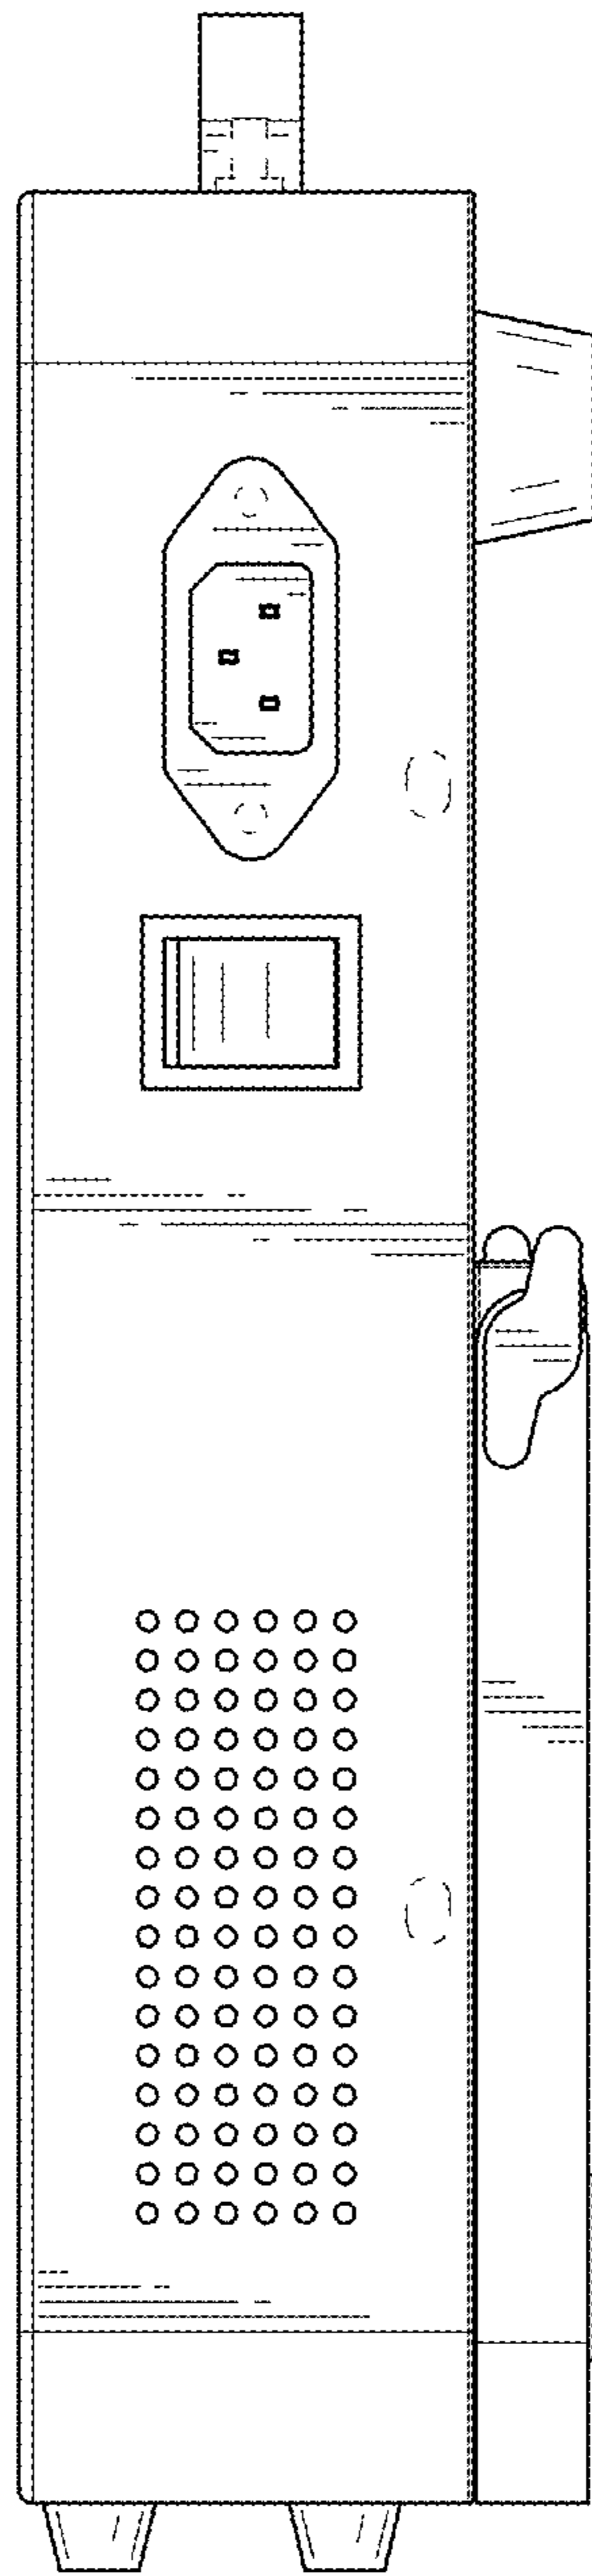


FIG. 6

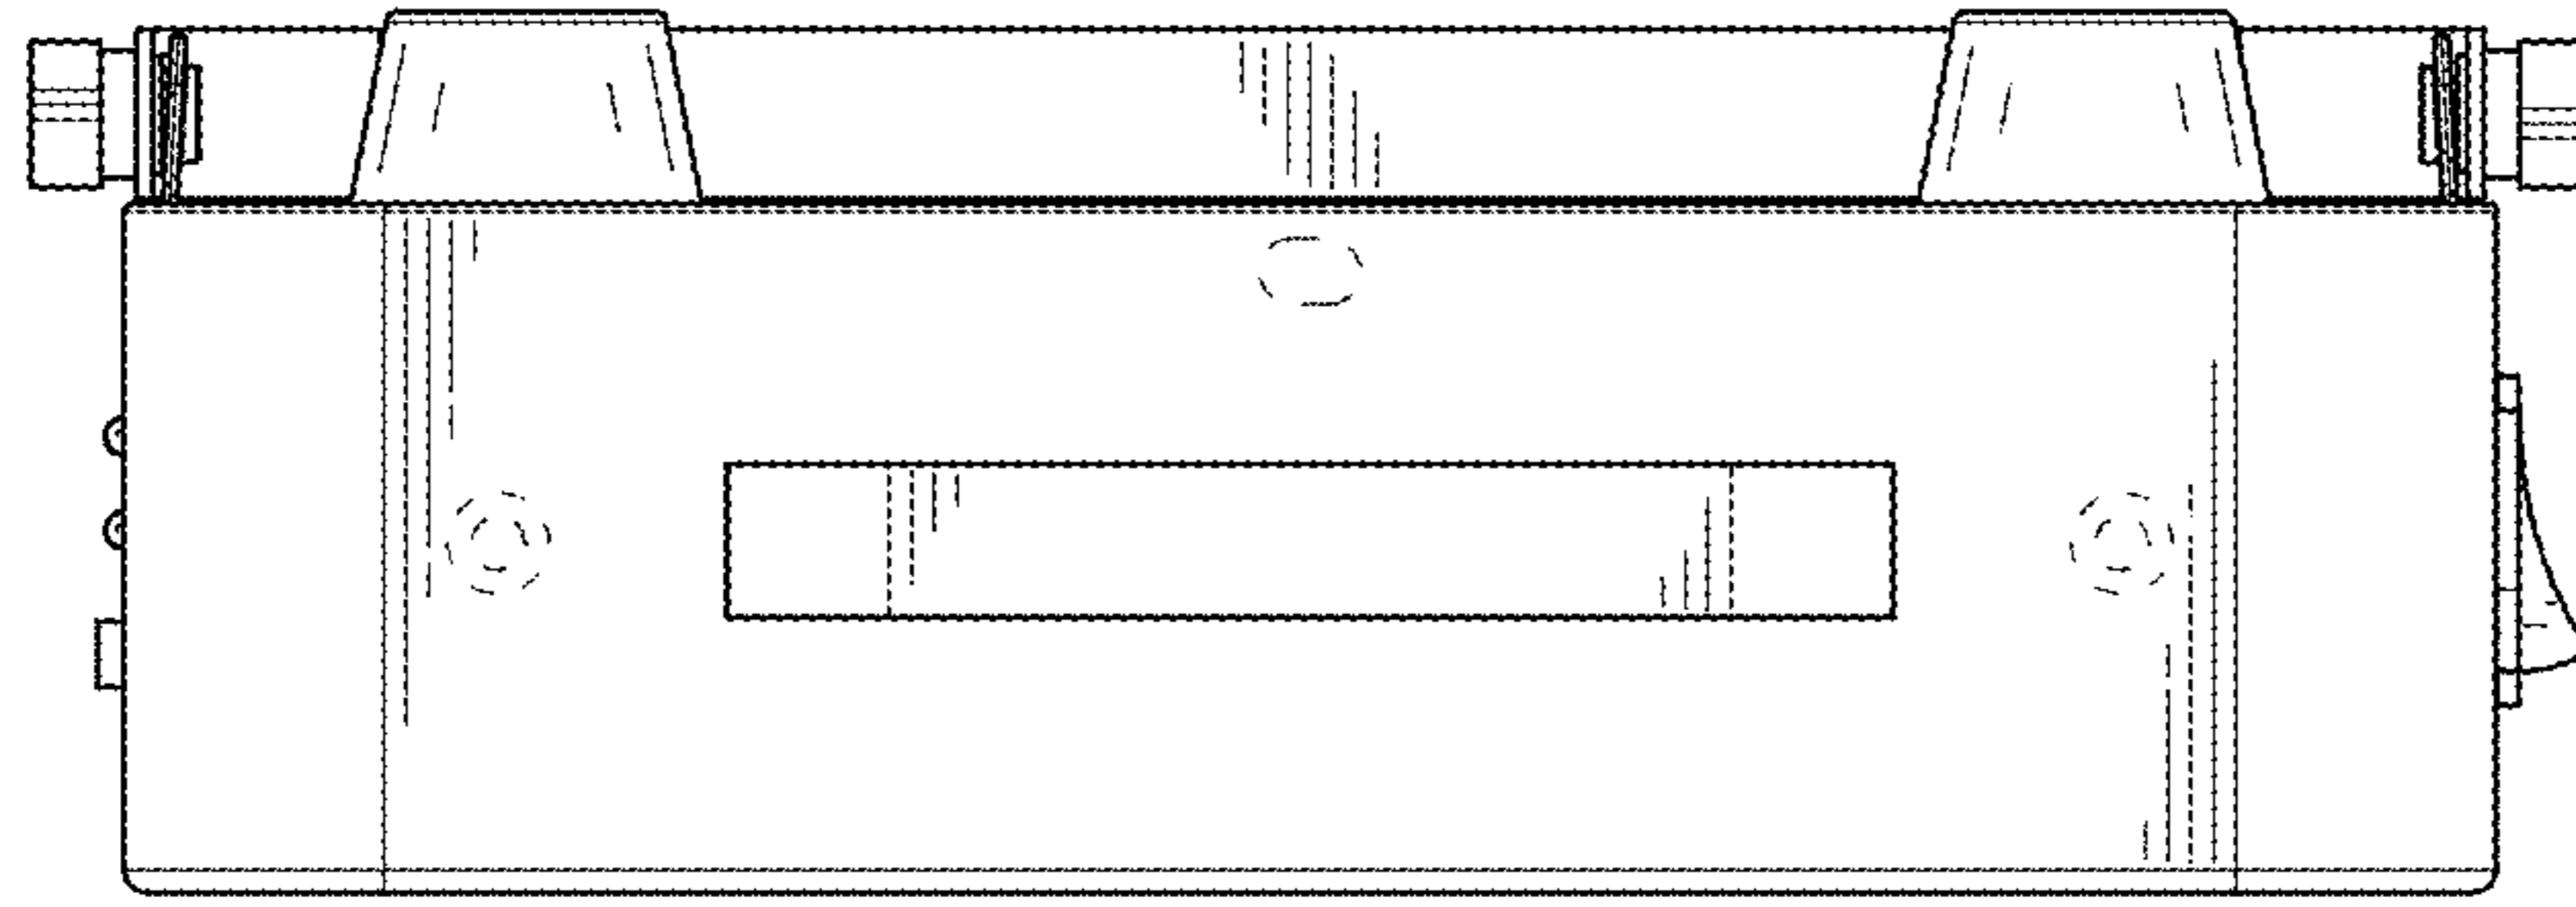


FIG. 7



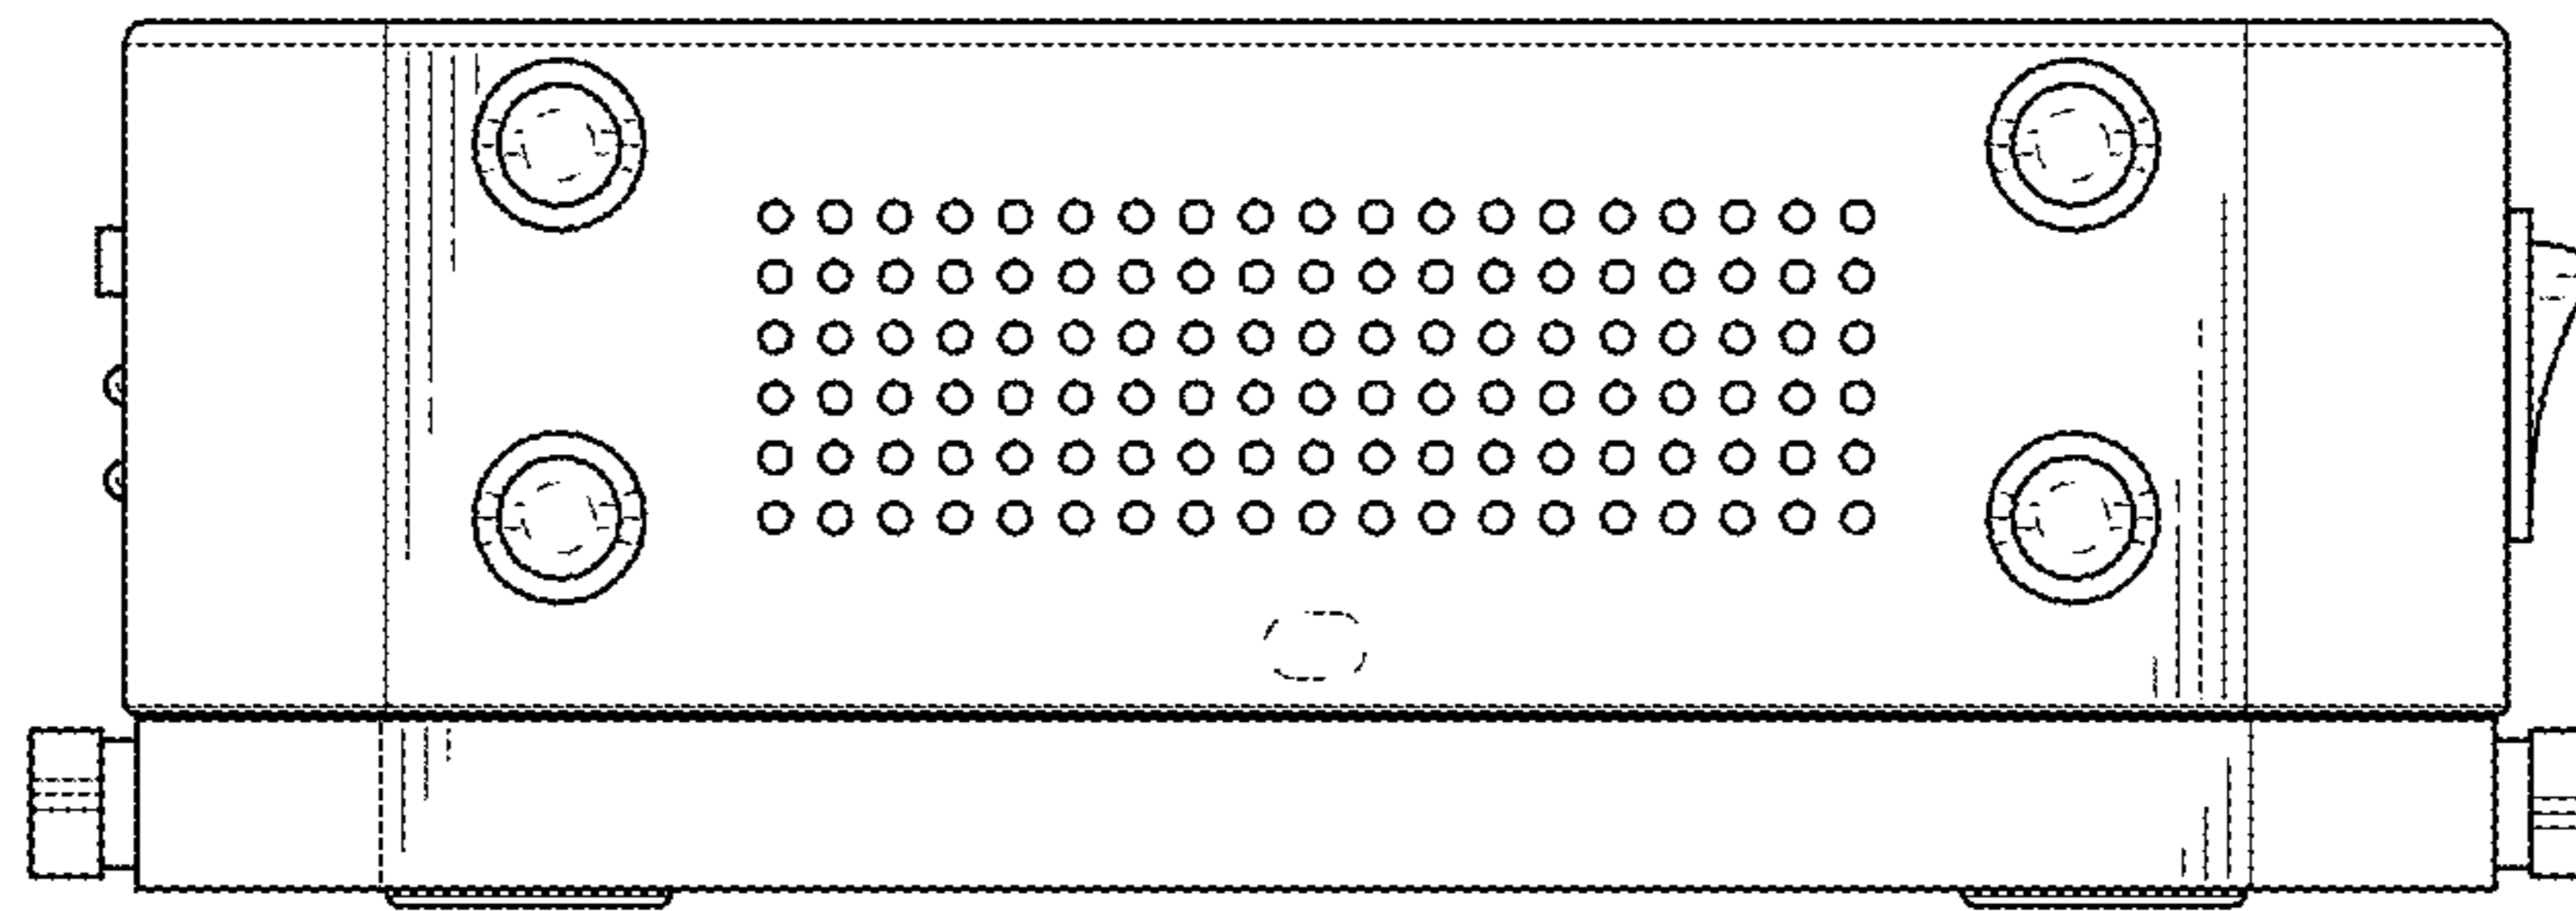


FIG.8