



US00D939105S

(12) **United States Design Patent** (10) **Patent No.:** **US D939,105 S**  
**Li** (45) **Date of Patent:** **\*\* Dec. 21, 2021**

(54) **TESTING CASSETTE**  
(71) Applicant: **Cellex, Inc.**, Research Triangle Park, NC (US)  
(72) Inventor: **Xingxiang Li**, Morrisville, NC (US)  
(73) Assignee: **CELLEX, INC.**, Research Triangle Park, NC (US)  
(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/749,034**  
(22) Filed: **Sep. 2, 2020**  
(51) **LOC (13) Cl.** ..... **24-01**  
(52) **U.S. Cl.**  
USPC ..... **D24/223**  
(58) **Field of Classification Search**  
USPC ..... D24/107, 186, 216, 219, 220, 221, D24/223-227, 231, 232; D10/81  
CPC ..... B01L 3/5027; B01L 3/50273; B01L 3/502738; B01L 2300/0609; B01L 2300/0672; B01L 2300/0829; B01L 2200/025; B01L 2200/026; B01L 2200/028; B01L 2200/16; G01N 21/01; G01N 21/75; G01N 33/66; G01N 33/49; G01N 33/493; A61B 5/14532; A61B 2560/0412; A61B 2560/0443; A61B 2560/0462  
See application file for complete search history.

(56) **References Cited**  
U.S. PATENT DOCUMENTS  
D310,265 S 8/1990 Mochnal et al.  
D342,575 S 12/1993 Ashihara et al.  
D391,373 S 2/1998 Shartle  
D432,244 S 10/2000 Anderson et al.  
D456,082 S 4/2002 Bouse et al.  
6,855,561 B2\* 2/2005 Jerome ..... G01N 21/8483 422/420  
6,867,051 B1 3/2005 Anderson et al.  
D532,520 S 11/2006 Kampmeier et al.  
7,270,970 B2 9/2007 Anderson et al.

D560,812 S \* 1/2008 Powell ..... D24/216  
D602,599 S \* 10/2009 Xiaowei ..... D24/225  
D655,424 S 3/2012 Castanon et al.  
D660,977 S \* 5/2012 Wagner ..... D24/223  
D676,570 S 2/2013 Chance et al.  
(Continued)

**FOREIGN PATENT DOCUMENTS**

IN 299769 \* 1/2019

**OTHER PUBLICATIONS**

Healgen COVID-19 Lateral Flow Rapid Antigen Test Single Test Pack. Primary Care Supplies. Posting date: unknown. Retrived from website on Jul. 26, 2021 at <https://www.primarycaresupplies.co.uk/healgen-covid-19-lateral-flow-rapid-antigen-test-single-test-pack/>.  
\*  
(Continued)

*Primary Examiner* — Anhdao Doan  
(74) *Attorney, Agent, or Firm* — Millen, White, Zelano & Branigan, PC; Ryan Pool


(57) **CLAIM**

The ornamental design for a testing cassette, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the testing cassette showing my new design.  
FIG. 2 is a front view thereof.  
FIG. 3 is a back view thereof.  
FIG. 4 is a side view thereof.  
FIG. 5 is another side view thereof.  
FIG. 6 is a top view thereof; and,  
FIG. 7 is a bottom view thereof.  
The broken lines in the drawings illustrate portions of the testing cassette which form no part of the claimed design. The dash-dot-dash lines represent the boundaries of the claim and form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

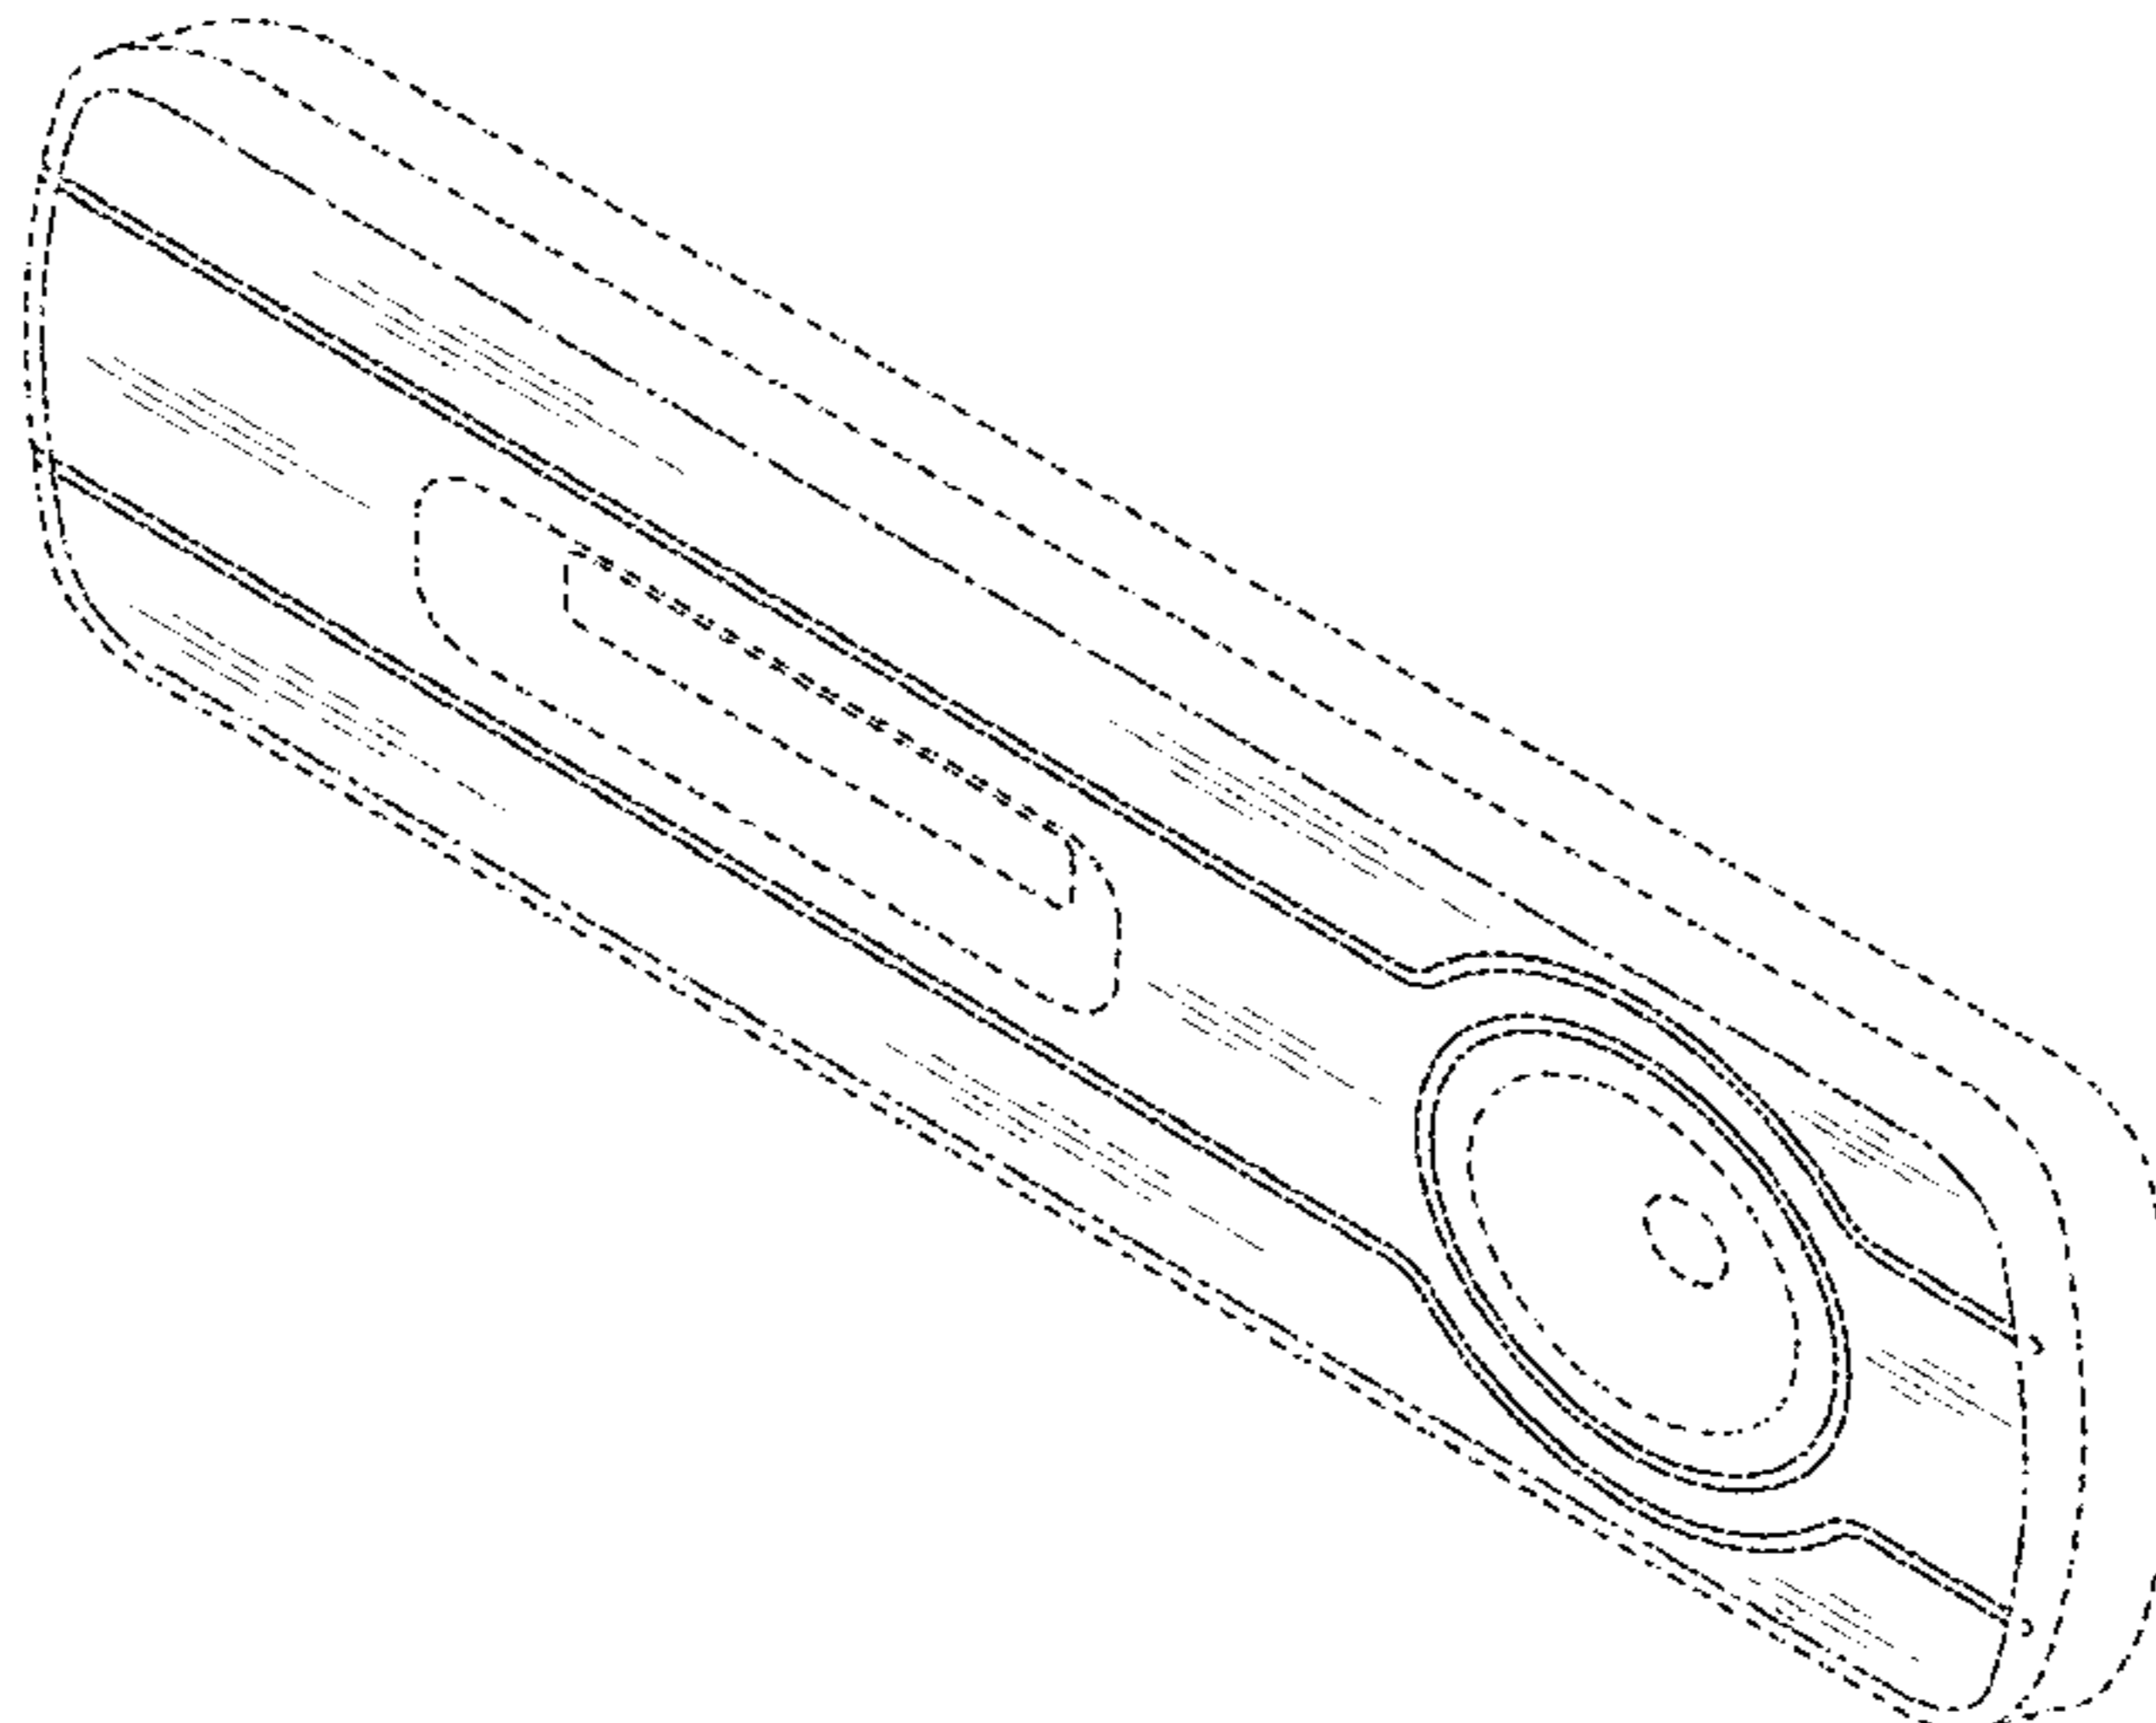

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D698,937	S	2/2014	Laverack et al.	
D726,329	S	4/2015	Sokolov et al.	
D734,482	S *	7/2015	Peterman .....	D24/216
D765,264	S *	8/2016	Zin .....	D24/223
9,404,911	B2	8/2016	Jacono et al.	
D772,428	S *	11/2016	Fumito .....	D24/225
D837,998	S	1/2019	Schaff et al.	
D888,275	S *	6/2020	Ito .....	D24/225
D894,422	S *	8/2020	Johnson .....	D24/224
D907,242	S	1/2021	Shinoda et al.	
2010/0024530	A1 *	2/2010	Hopkins, II .....	B01L 3/5023 73/64.56
2016/0011188	A1 *	1/2016	Anderberg .....	B01L 3/5023 422/420
2016/0153878	A1 *	6/2016	Candon .....	G01N 33/543 435/7.4
2021/0055284	A1 *	2/2021	Ding .....	G01N 33/5302

OTHER PUBLICATIONS

Image of Rapid Test Cassette for COVID-19 IgG/IgM. Made in Swiss. Image first appeared online on or before Jun. 2, 2020 (1 page) downloaded from <http://www-https://cbdwebmarket.com/product/test-cassette-for-covid-19/> Author unknown.

Image from Twitter Spring Healthcare Services Apr. 14, 2020 Spring Healthcare Services:@SpringHealthca1 COVID-19 Rapid Test offers High Accuracy and Fast Results with 10 minutes Assay Time #COVID2019 Author: unknown (1 page).

\* cited by examiner

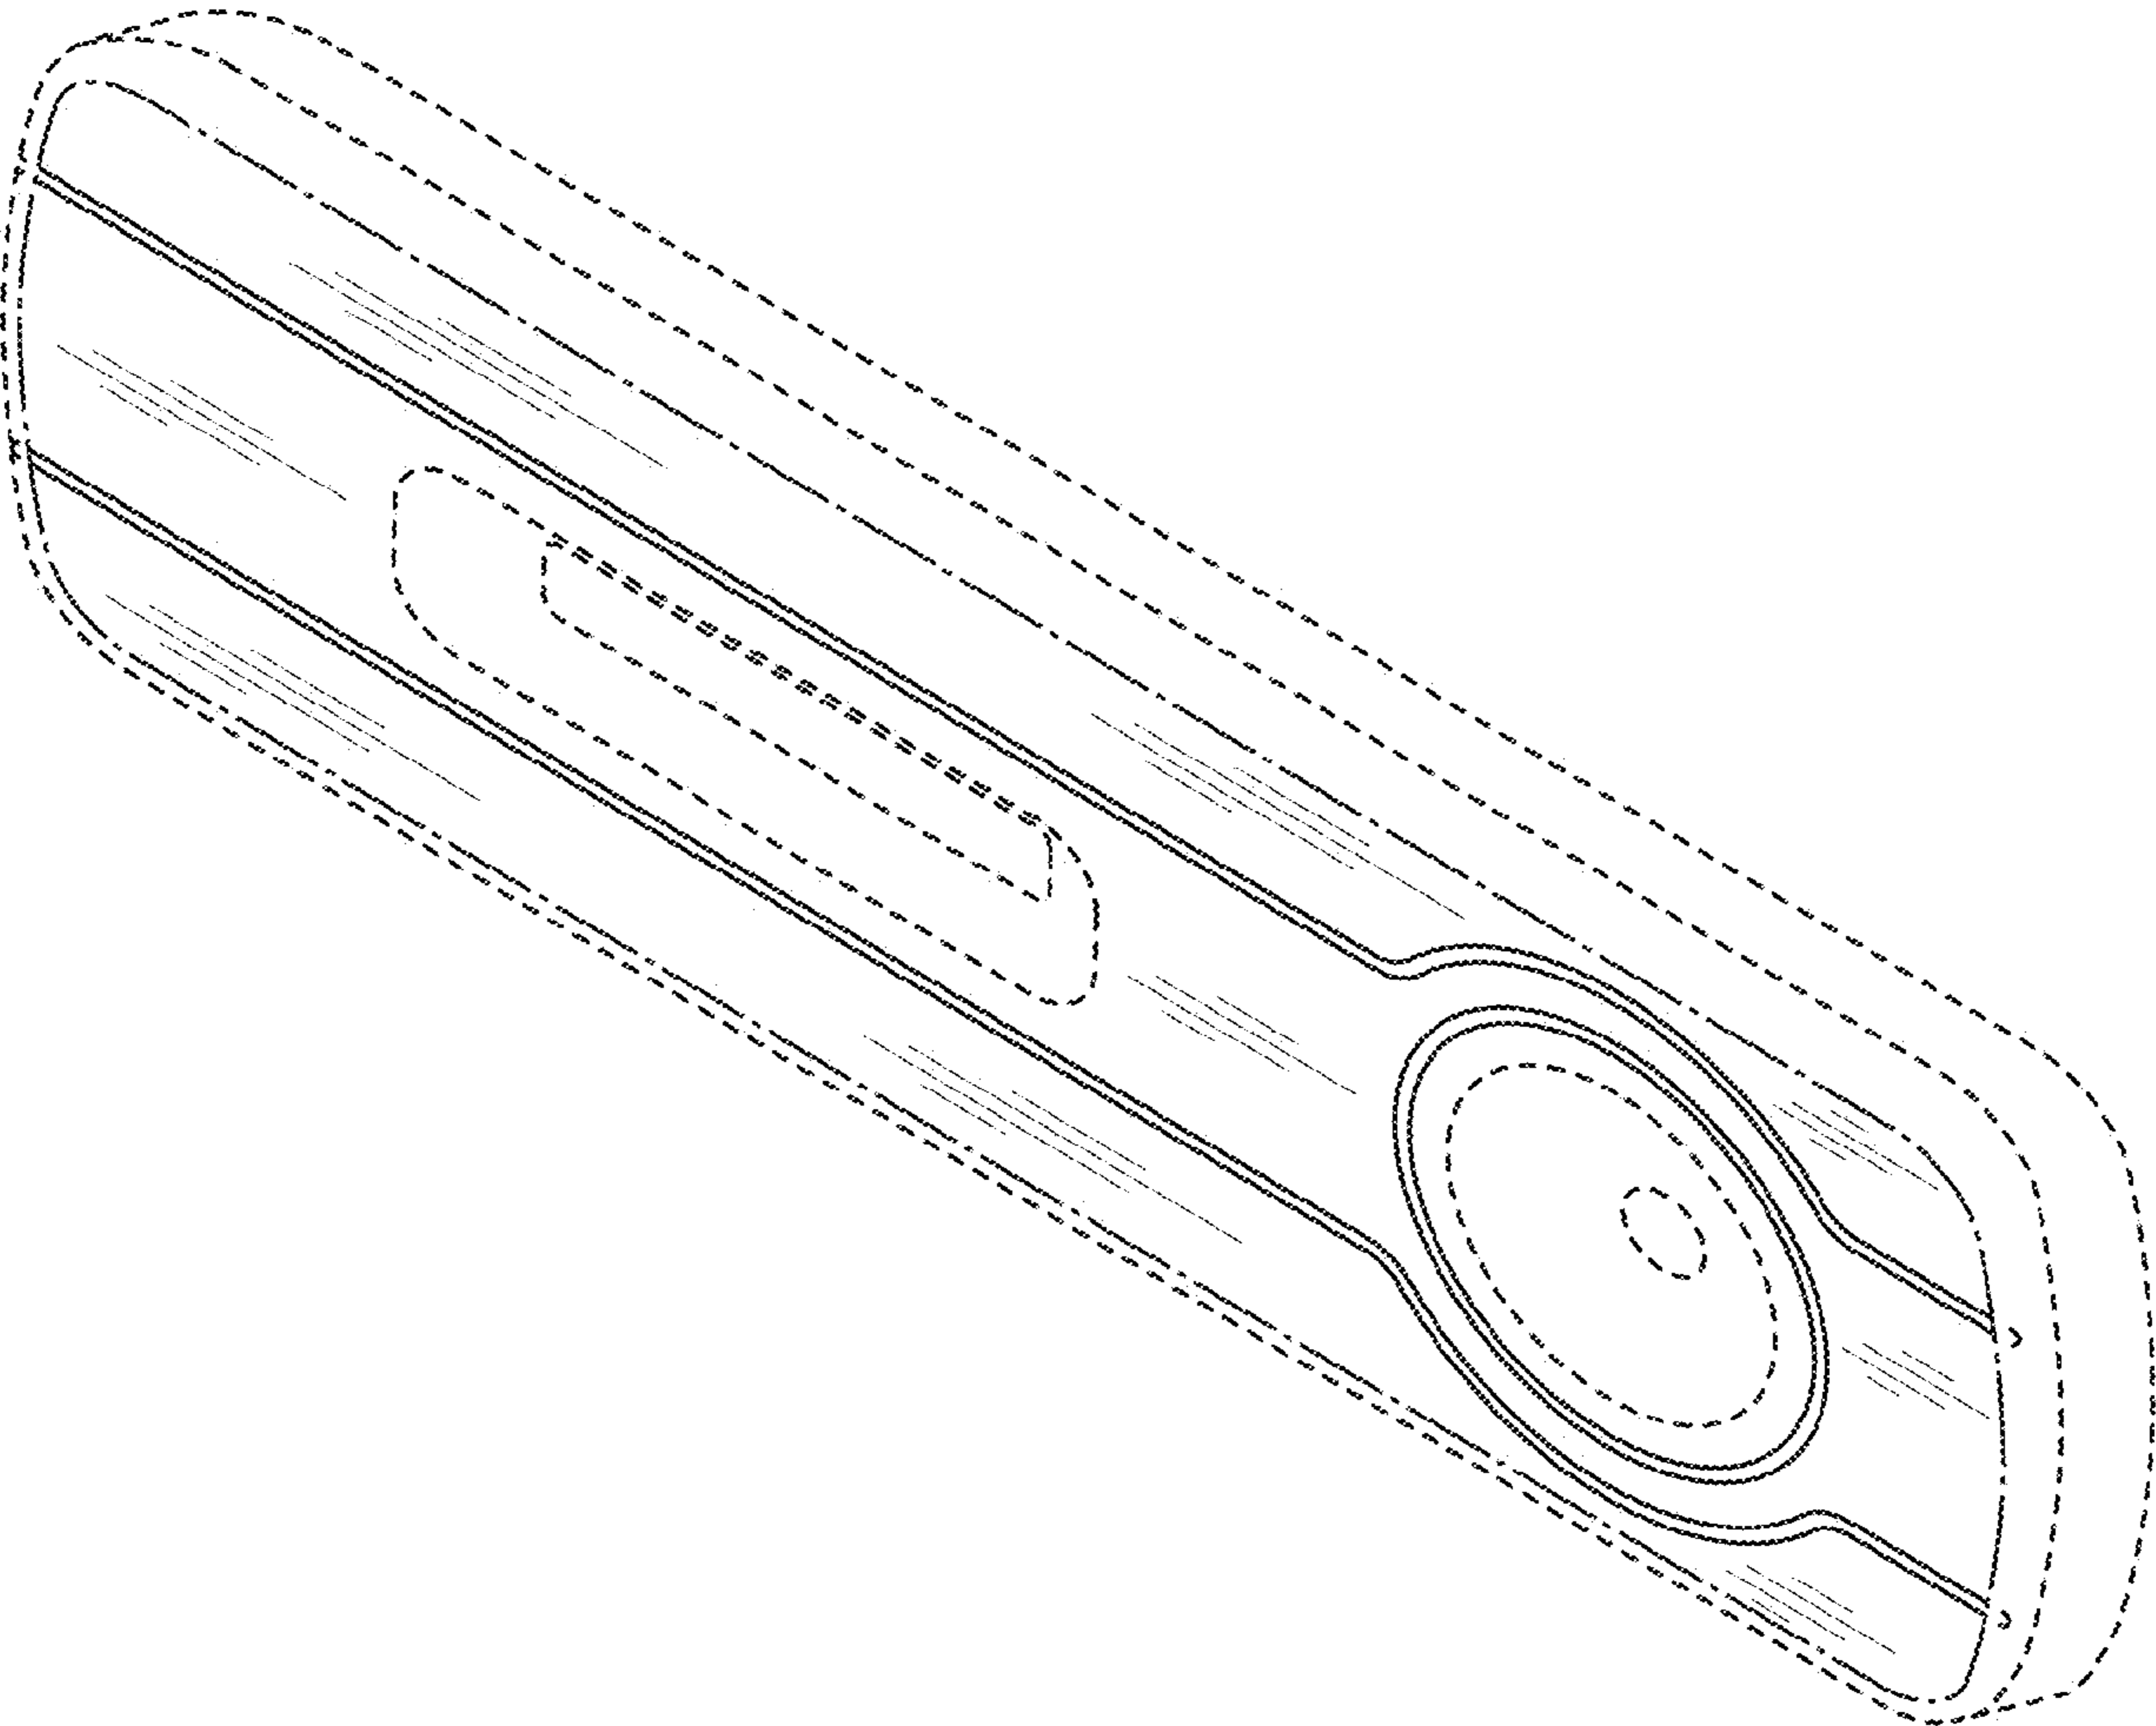


FIG. 1

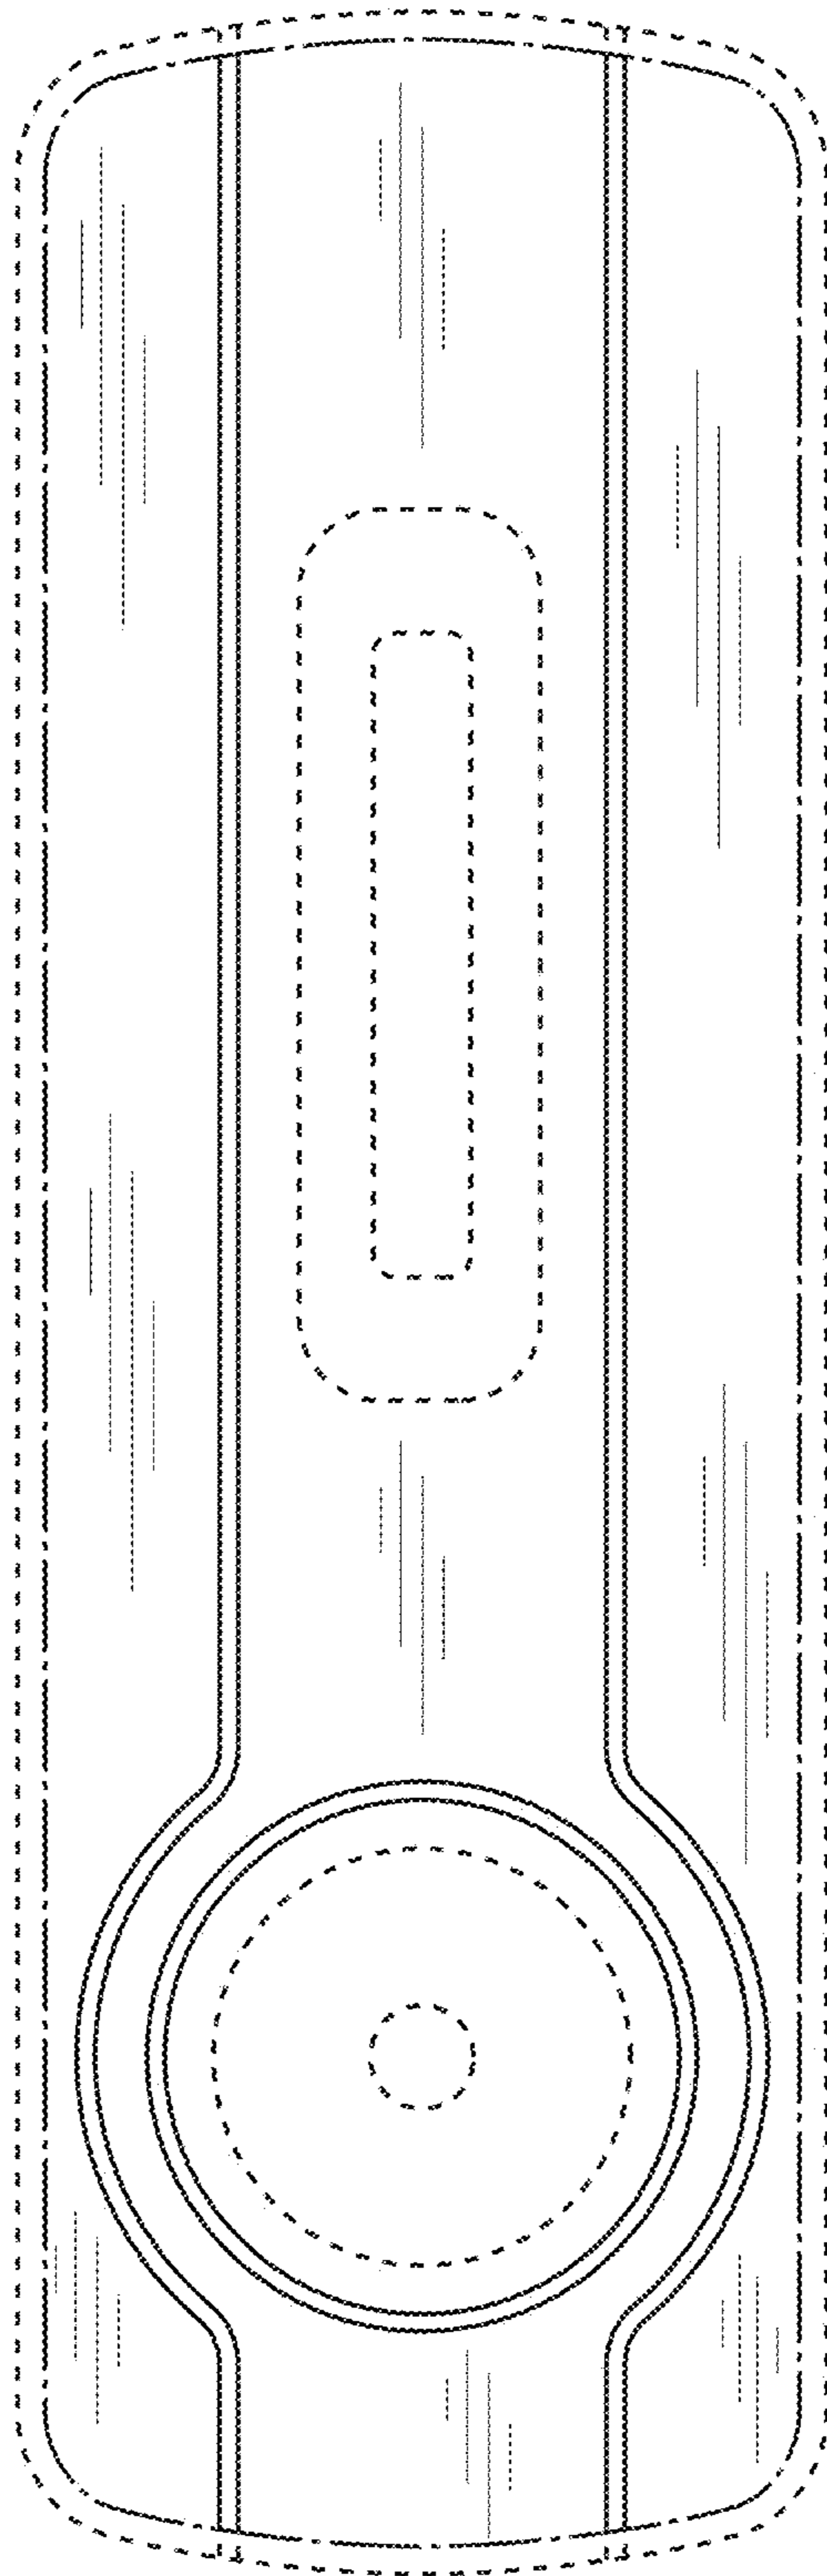


FIG. 2

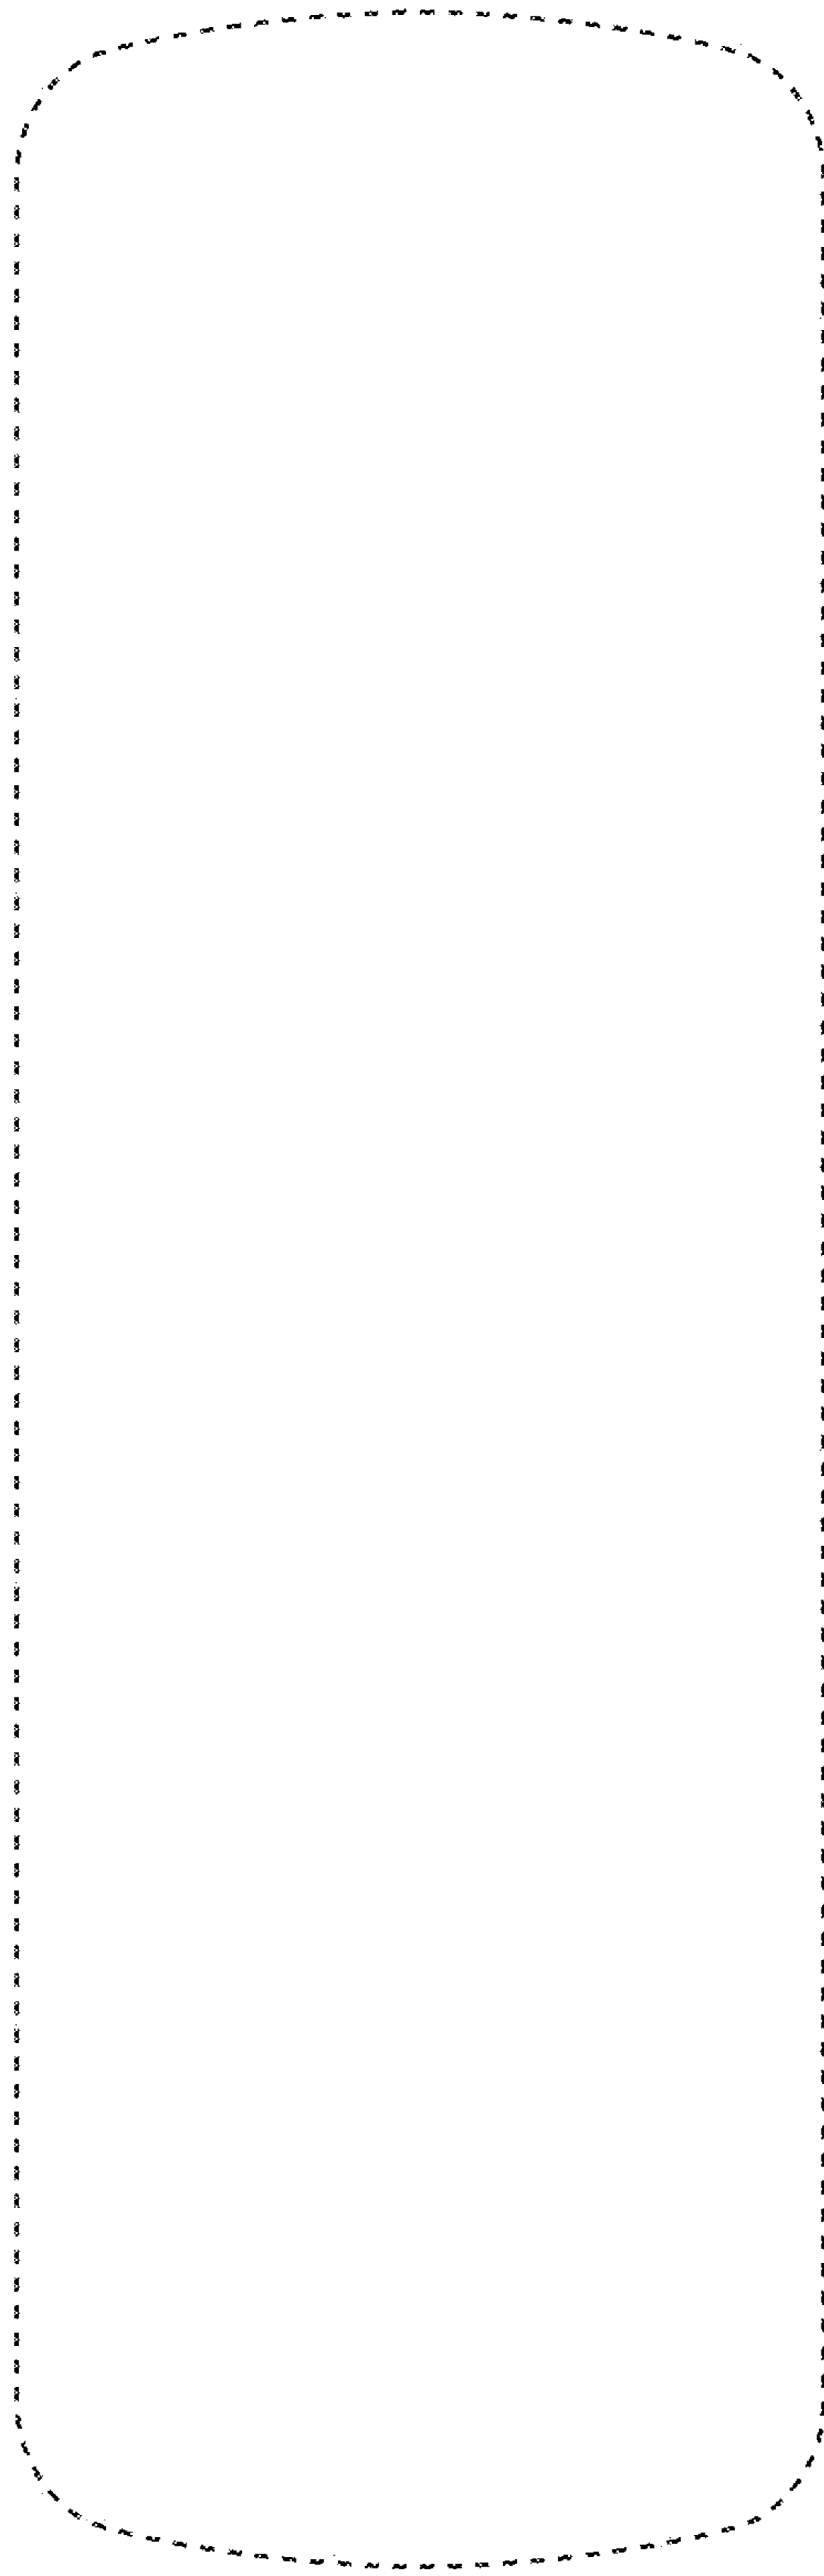


FIG. 3

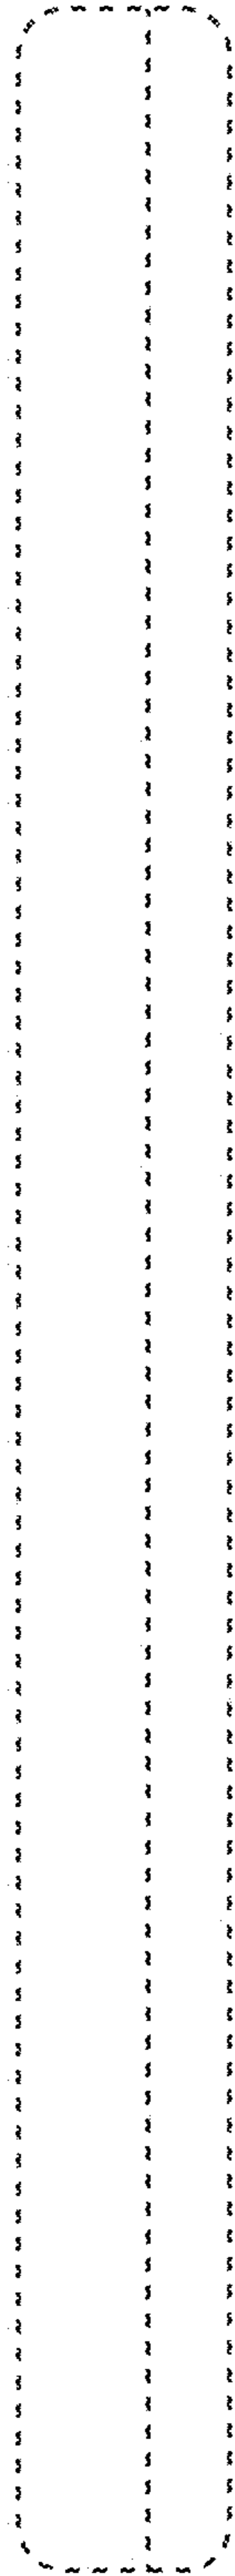


FIG. 4

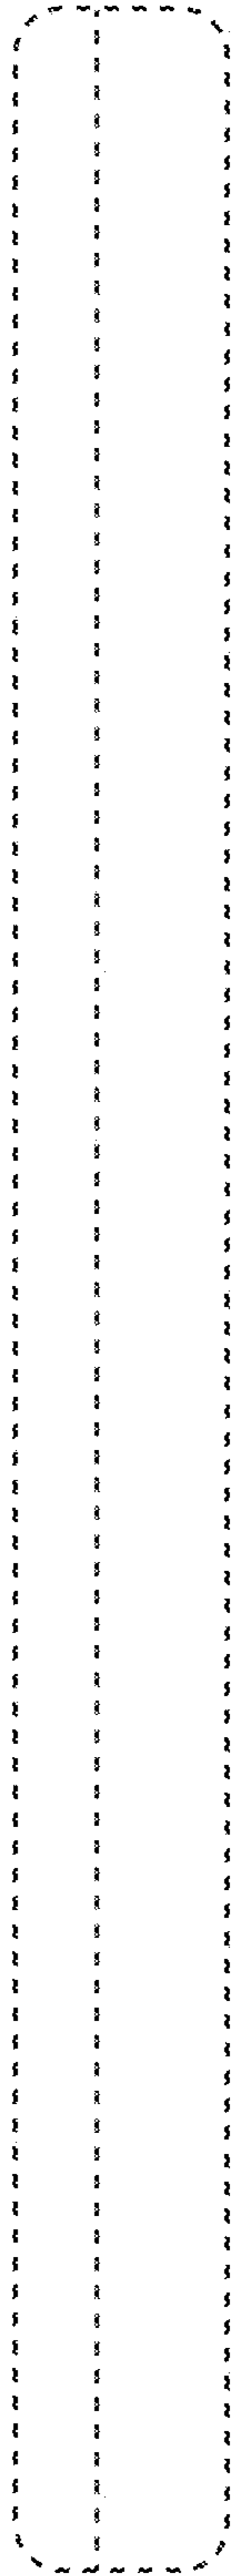


FIG. 5



FIG. 6



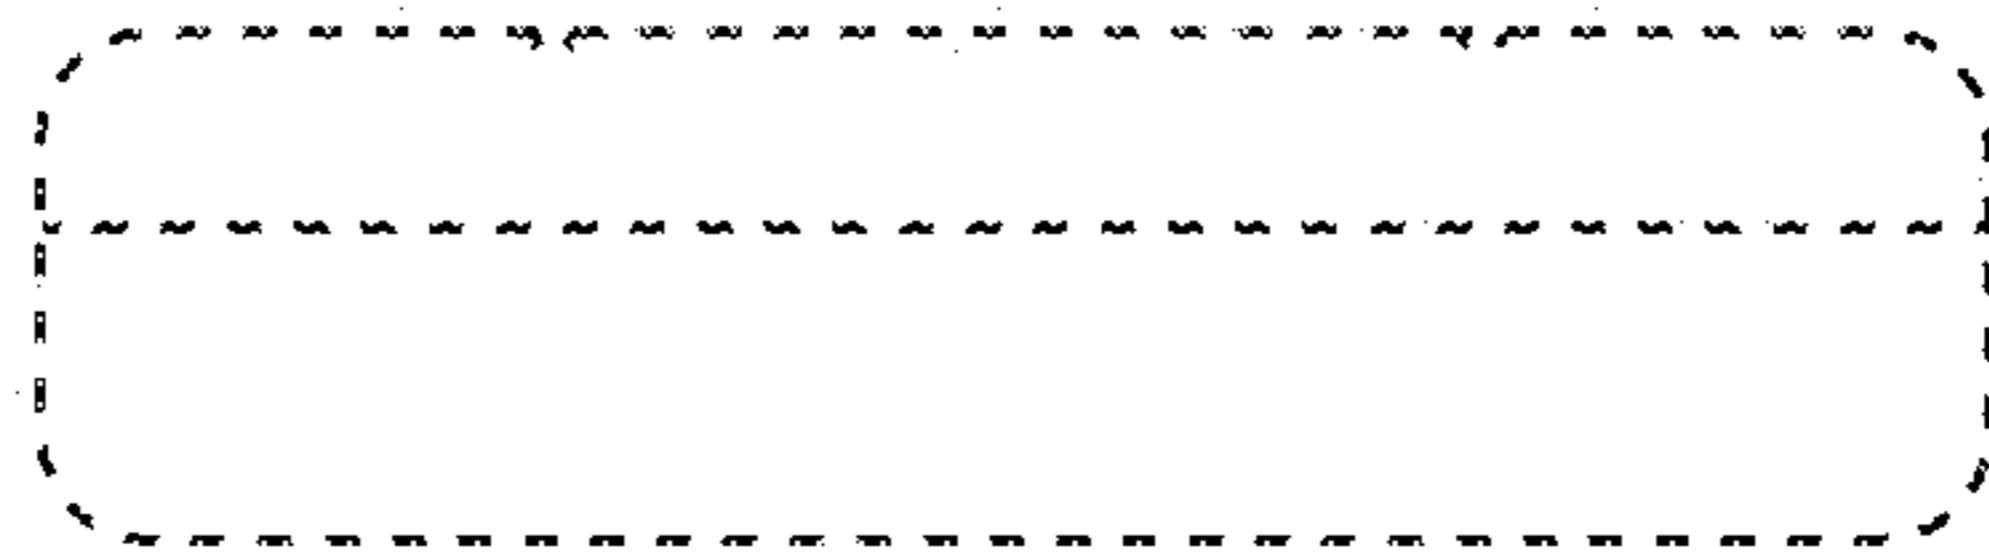


FIG. 7