



US00D939708S

(12) **United States Design Patent** (10) **Patent No.:** **US D939,708 S**
Rainville et al. (45) **Date of Patent:** **** Dec. 28, 2021**

(54) **MOBILE CLINICAL VIEWING TOOL**
(71) Applicant: **EchoNous, Inc.**, Redmond, WA (US)
(72) Inventors: **Donald James Rainville**, Sewickley, PA (US); **Nikolaos Pagoulatos**, Kirkland, WA (US); **Greg Nieminen**, Bothell, WA (US); **Bradley S. Melmon**, Seattle, WA (US); **Nidhi Jaiswal**, Redmond, WA (US); **Qianying Miao**, Redmond, WA (US); **Brandon Cheung**, San Francisco, CA (US); **Christopher Loew**, Palo Alto, CA (US)

D761,899 S 7/2016 Beatty et al.
D765,252 S 8/2016 Emeric et al.
D796,678 S 9/2017 Dekock et al.
D807,513 S 1/2018 Eslava et al.
D834,195 S 11/2018 Chamberlain et al.
D838,715 S 1/2019 Chen et al.

(Continued)

FOREIGN PATENT DOCUMENTS

CN 305094098 S 4/2019
TW D188935 S 3/2018

OTHER PUBLICATIONS

Search Report for Taiwan Application No. 108307397, dated Sep. 25, 20, 1 page.

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Seed Intellectual Property Law Group LLP

(73) Assignee: **ECHONOUS, INC.**, Redmond, WA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/751,383**

(22) Filed: **Sep. 21, 2020**

Related U.S. Application Data

(63) Continuation of application No. 29/693,105, filed on May 30, 2019, now Pat. No. Des. 897,535.

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/160; D24/186**

(58) **Field of Classification Search**
USPC D24/107, 158–161, 185, 186, 187, 137, D24/138; D14/315, 336, 371, 448
CPC A61B 6/4405; A61B 6/4411; A61B 6/435; A61B 6/4441; A61B 6/4447; A61B 8/4411; A61B 8/4427; A61B 8/462; A61B 8/0437; A61B 8/0883; A45F 2200/0516; A45F 2200/0525

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D451,603 S 12/2001 Bastyr et al.
D653,521 S 2/2012 Wike


(57) **CLAIM**

The ornamental design for a mobile clinical viewing tool, as shown and described.

DESCRIPTION

FIG. 1 is a top, front, right side perspective view of a mobile clinical viewing tool showing our new design.
FIG. 2 is a top, rear, left side perspective view thereof.
FIG. 3 is a front elevation view thereof.
FIG. 4 is a rear elevation view thereof.
FIG. 5 is a top plan view thereof.
FIG. 6 is a bottom plan view thereof.
FIG. 7 is a left side elevation view thereof; and,
FIG. 8 is a right side elevation view thereof.
The broken lines in the figures illustrate aspects of the mobile clinical viewing tool that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

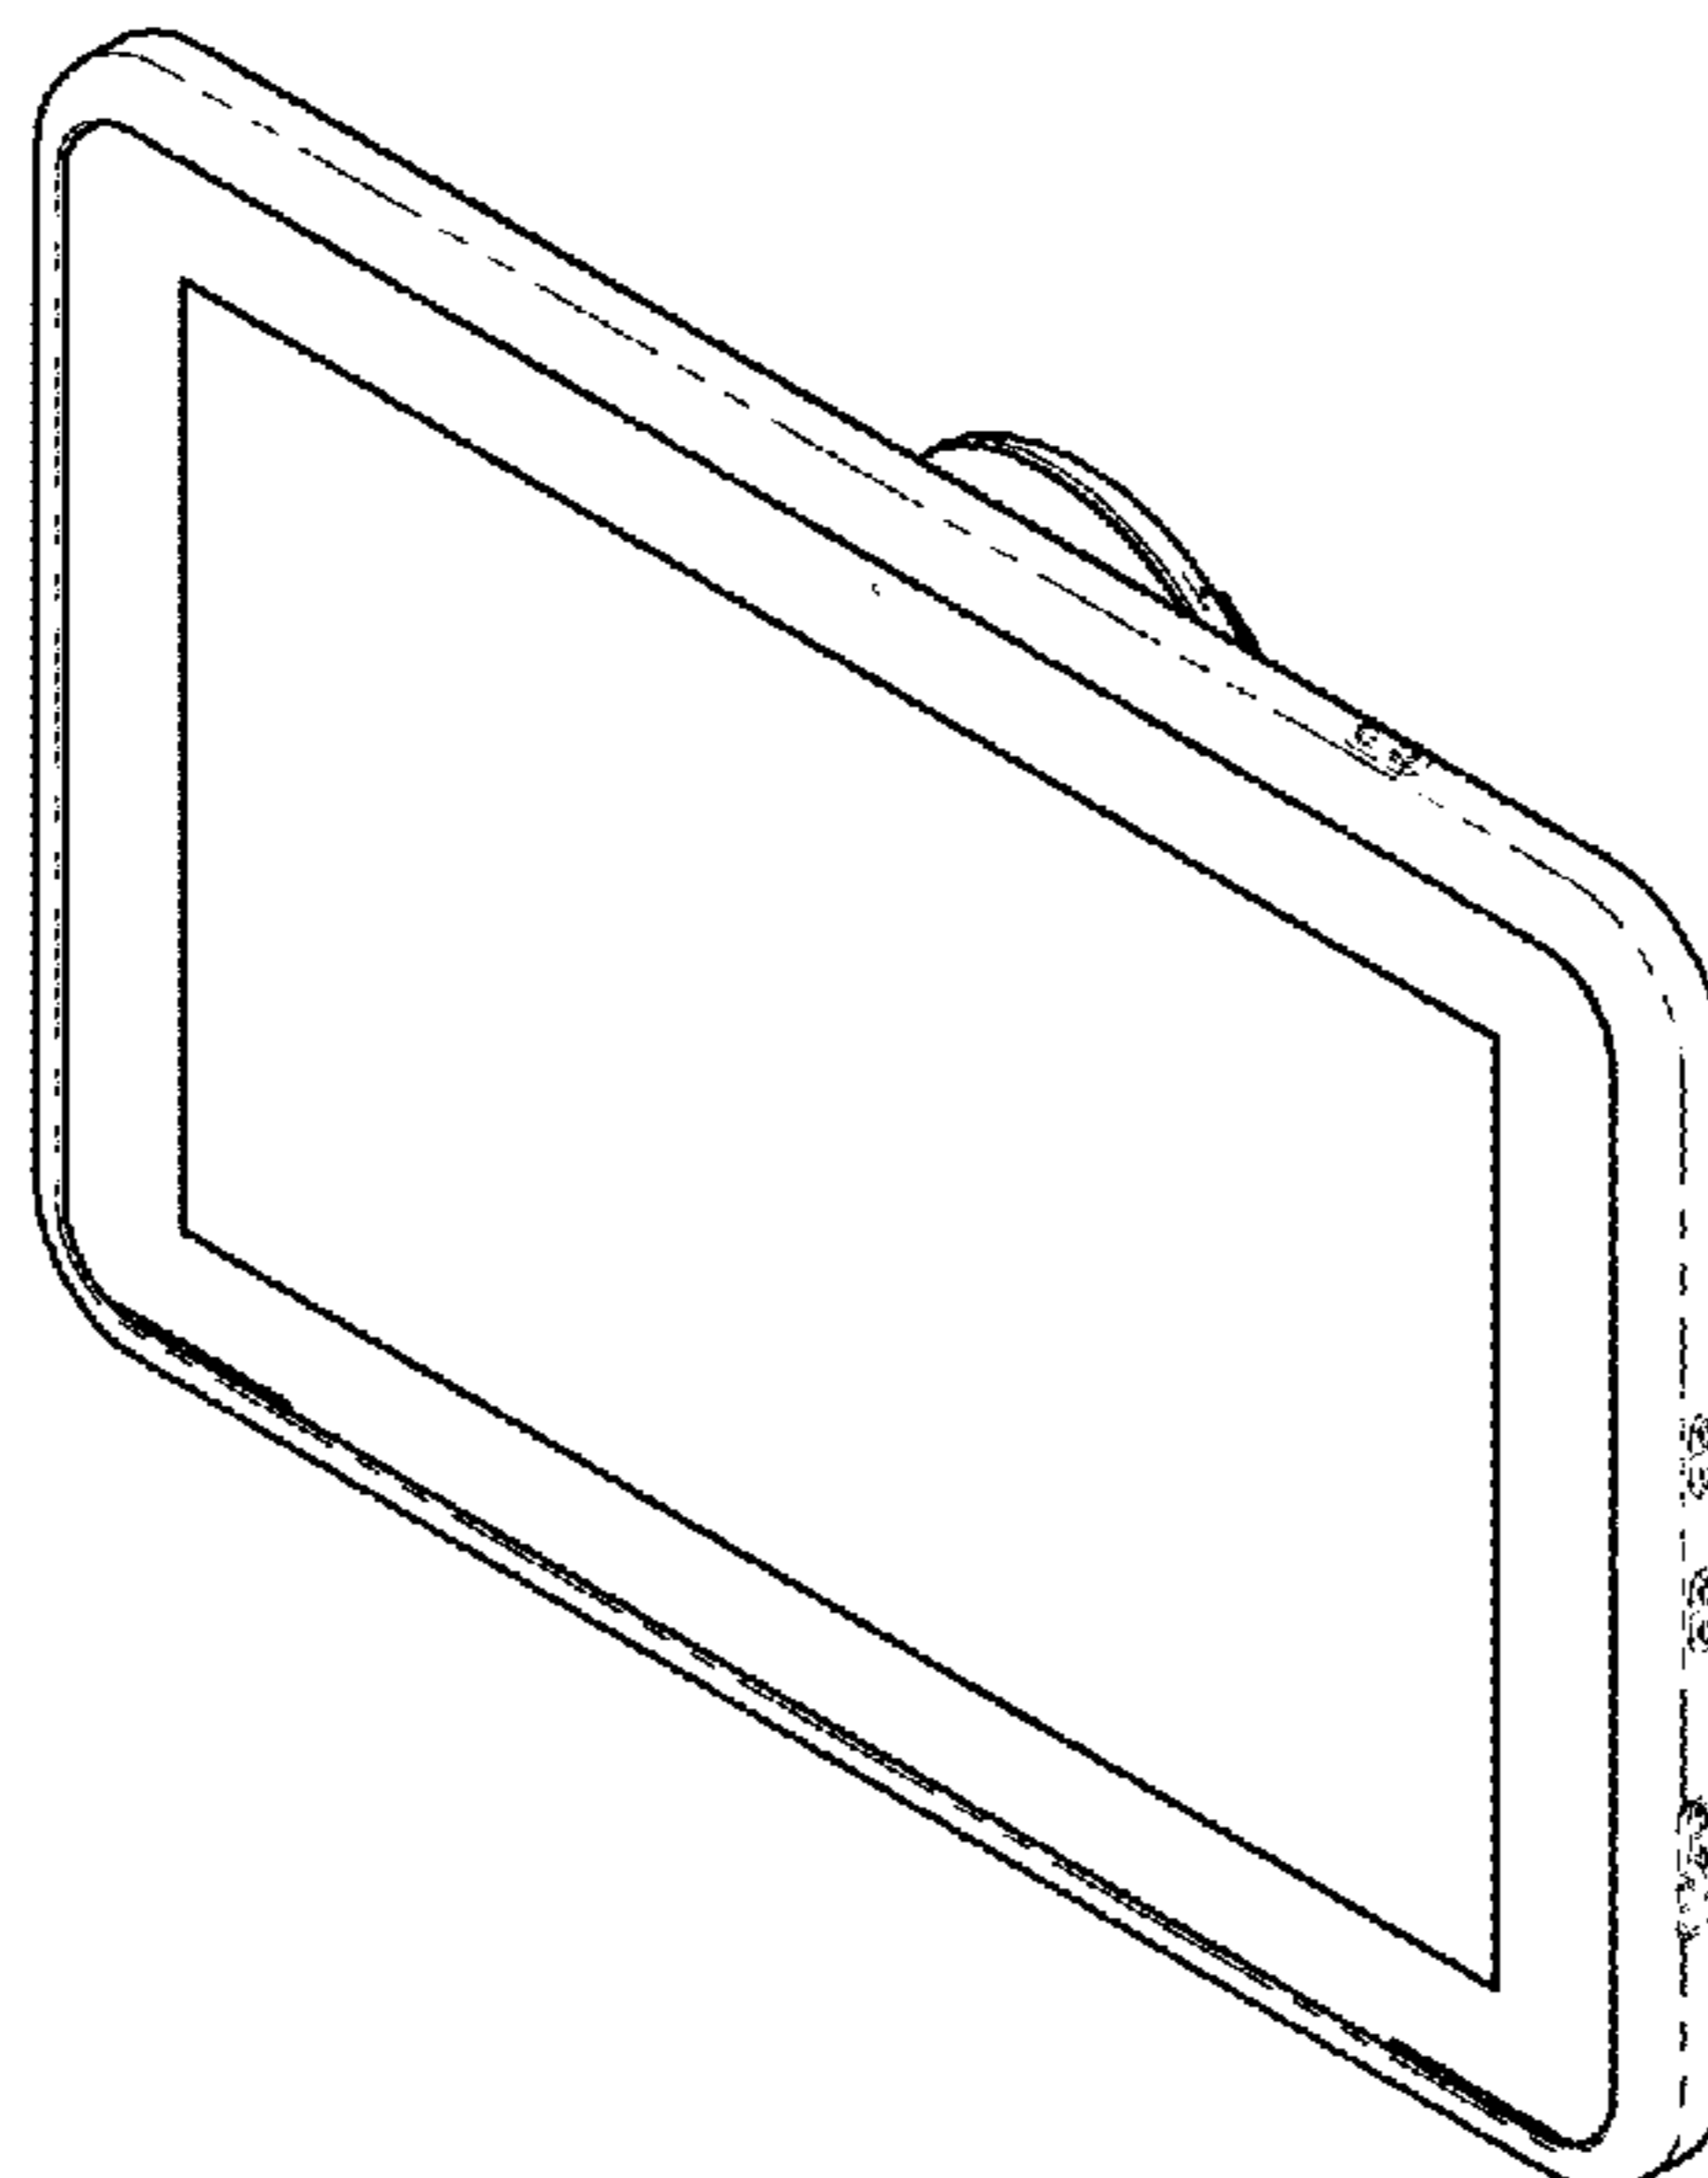

(56)

References Cited

U.S. PATENT DOCUMENTS

D852,268	S	6/2019	Lyons et al.	
D861,177	S *	9/2019	Kim	D24/186
D897,535	S *	9/2020	Rainville	D24/160
11,073,865	B1 *	7/2021	Lens-Rosal	G06F 1/1613
2012/0118770	A1	5/2012	Valls et al.	
2014/0267660	A1	9/2014	Pagoulatos et al.	
2018/0153287	A1 *	6/2018	William	A45F 5/00

* cited by examiner

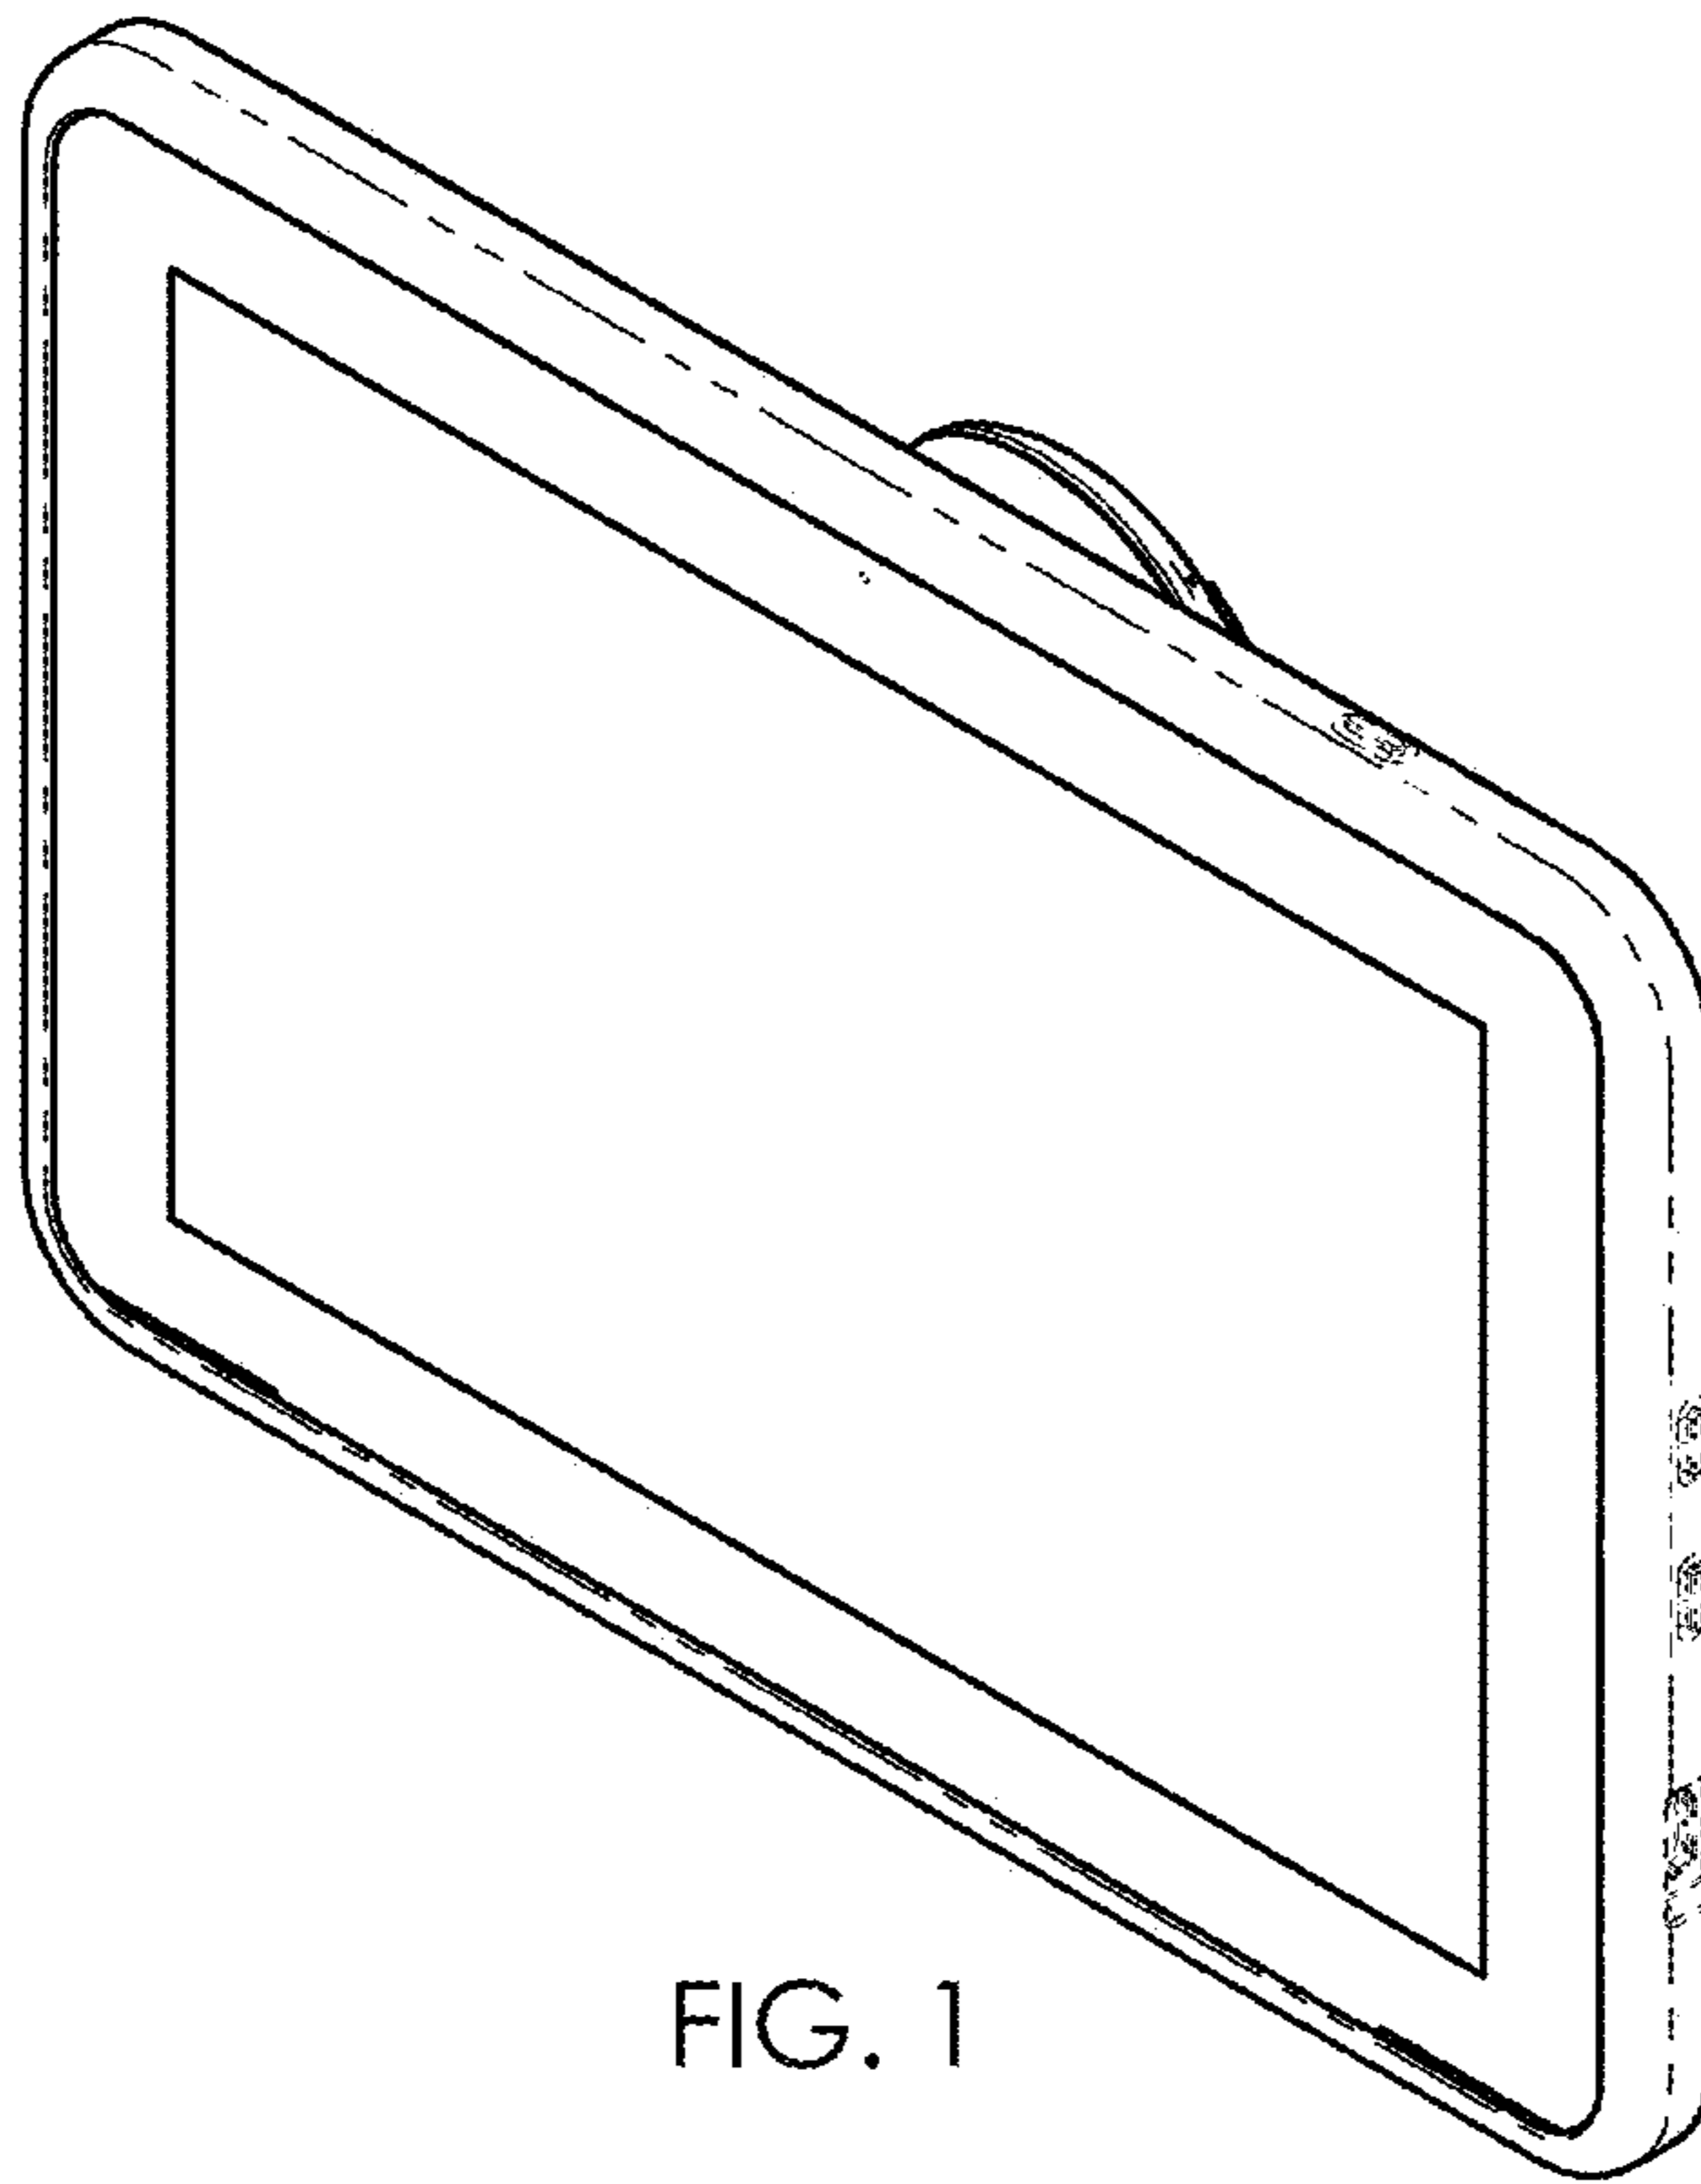


FIG. 1

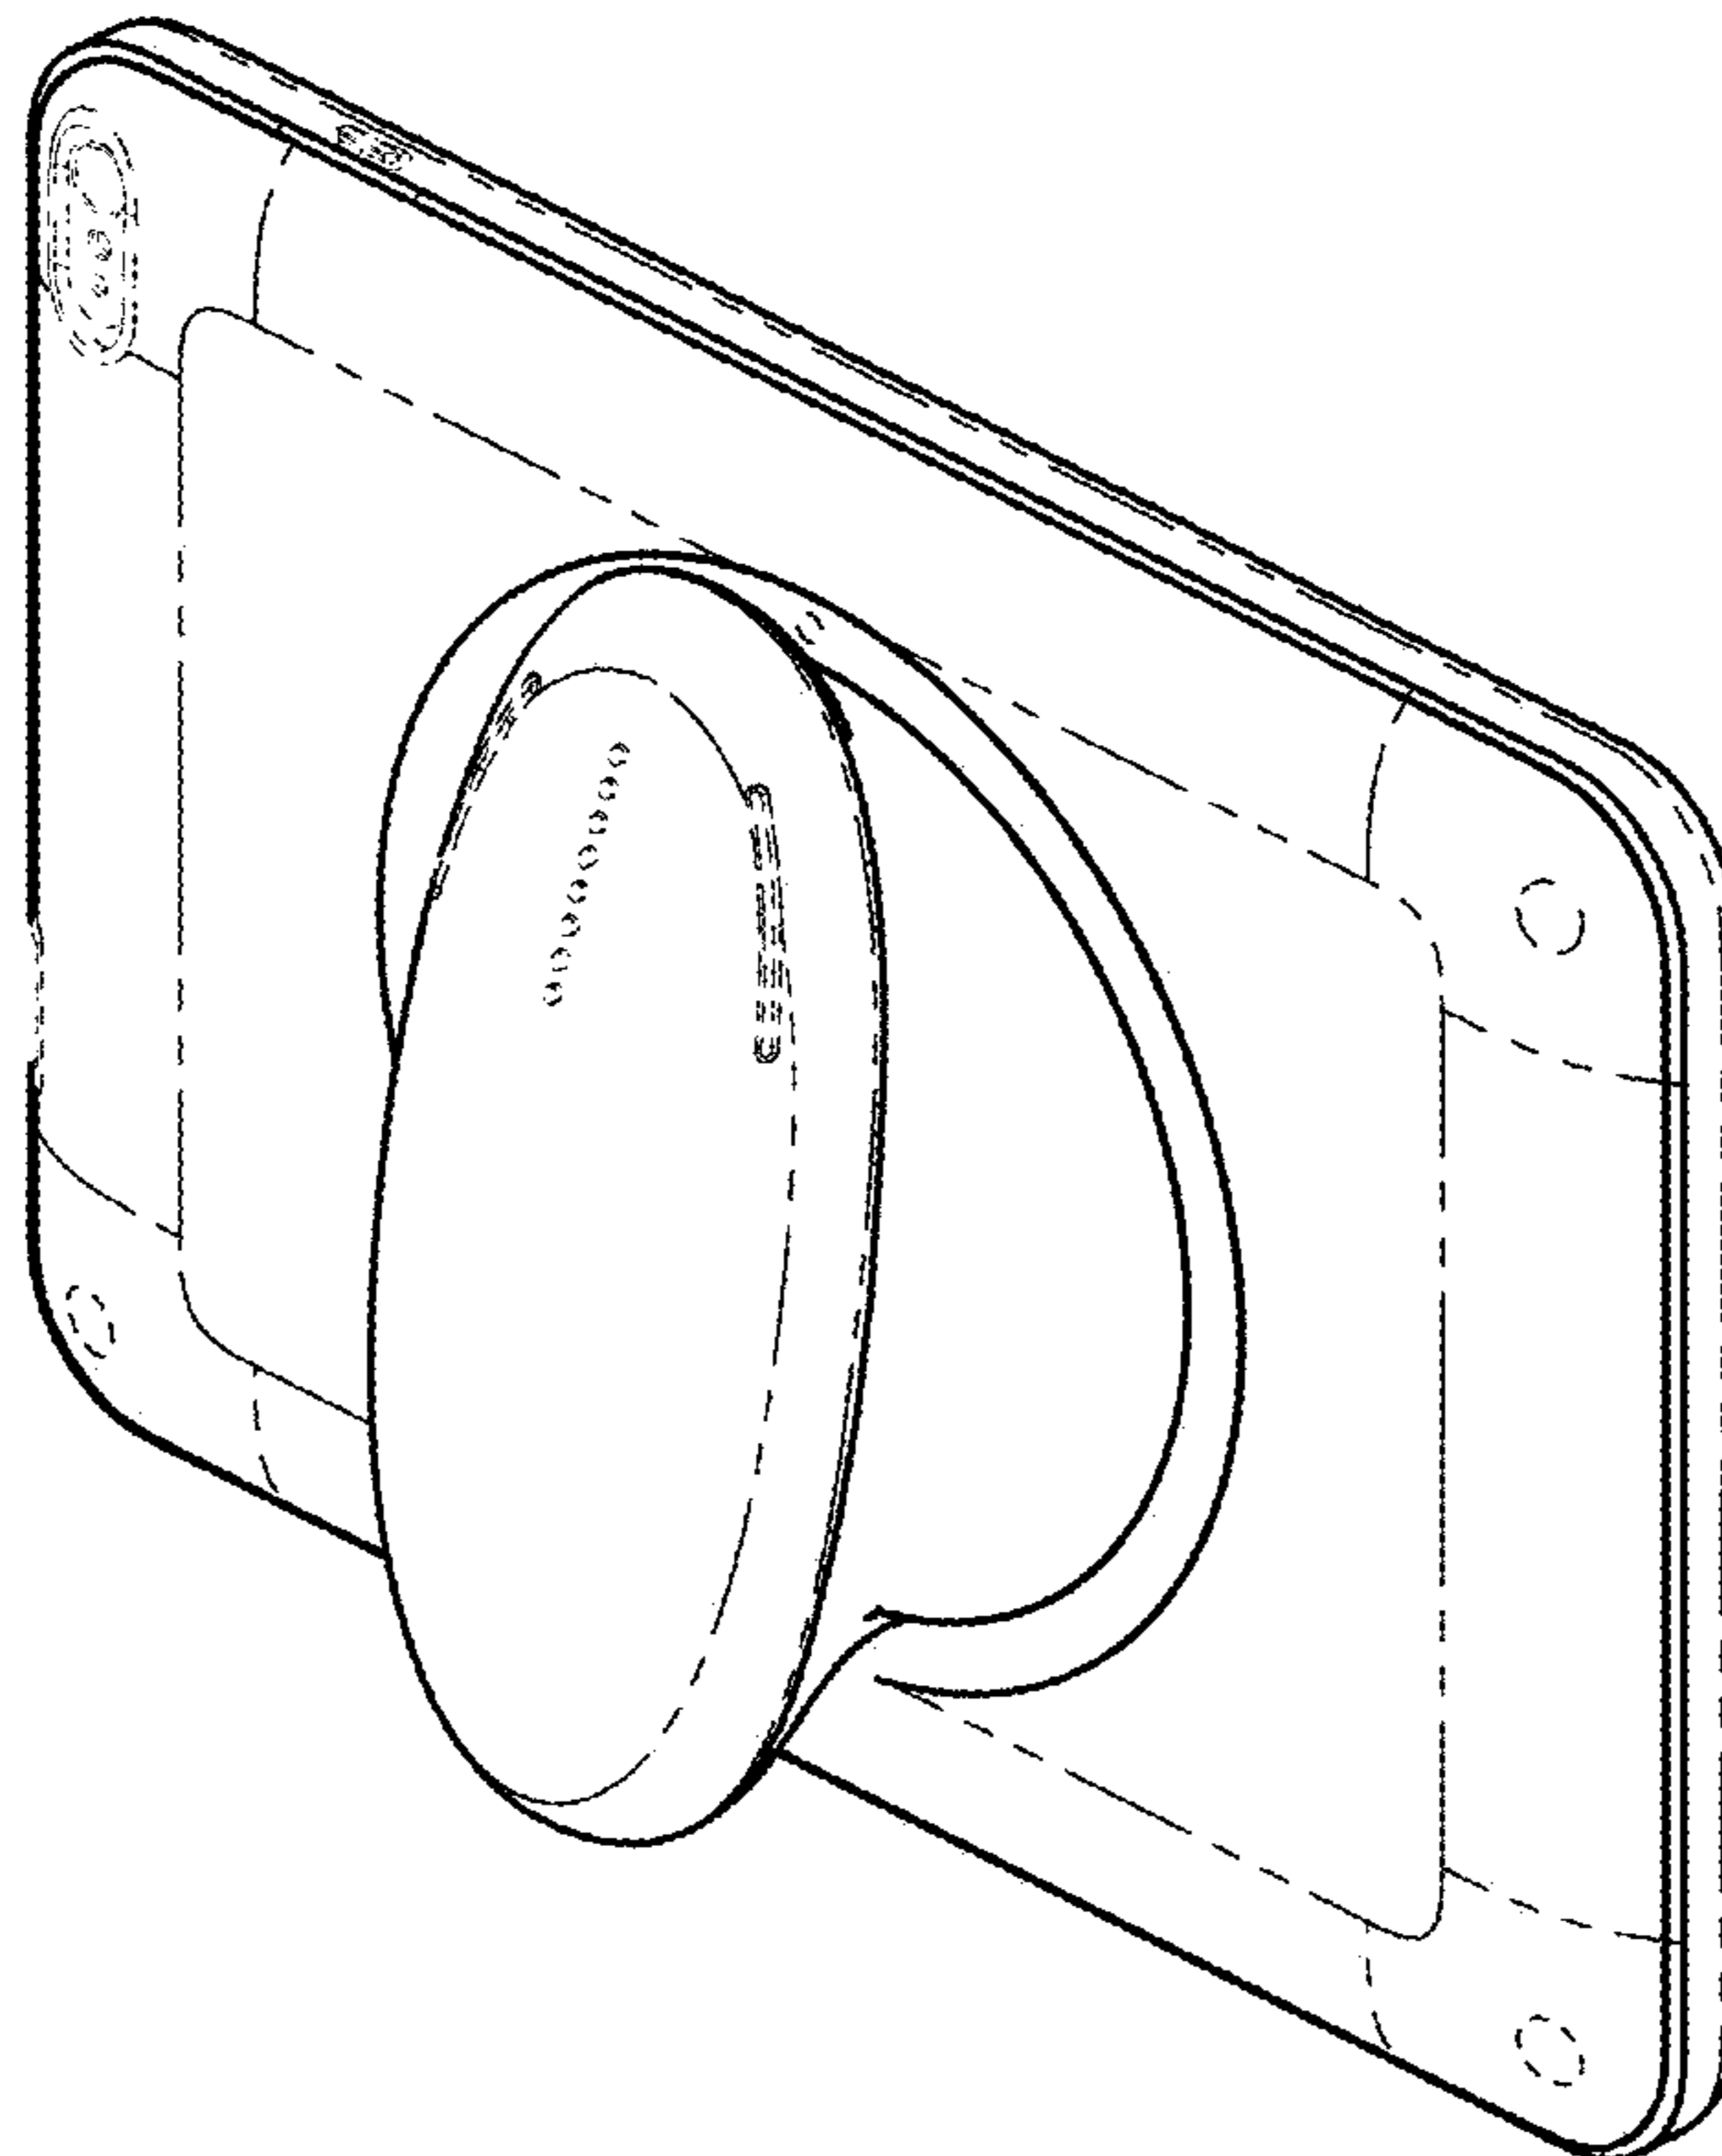


FIG. 2

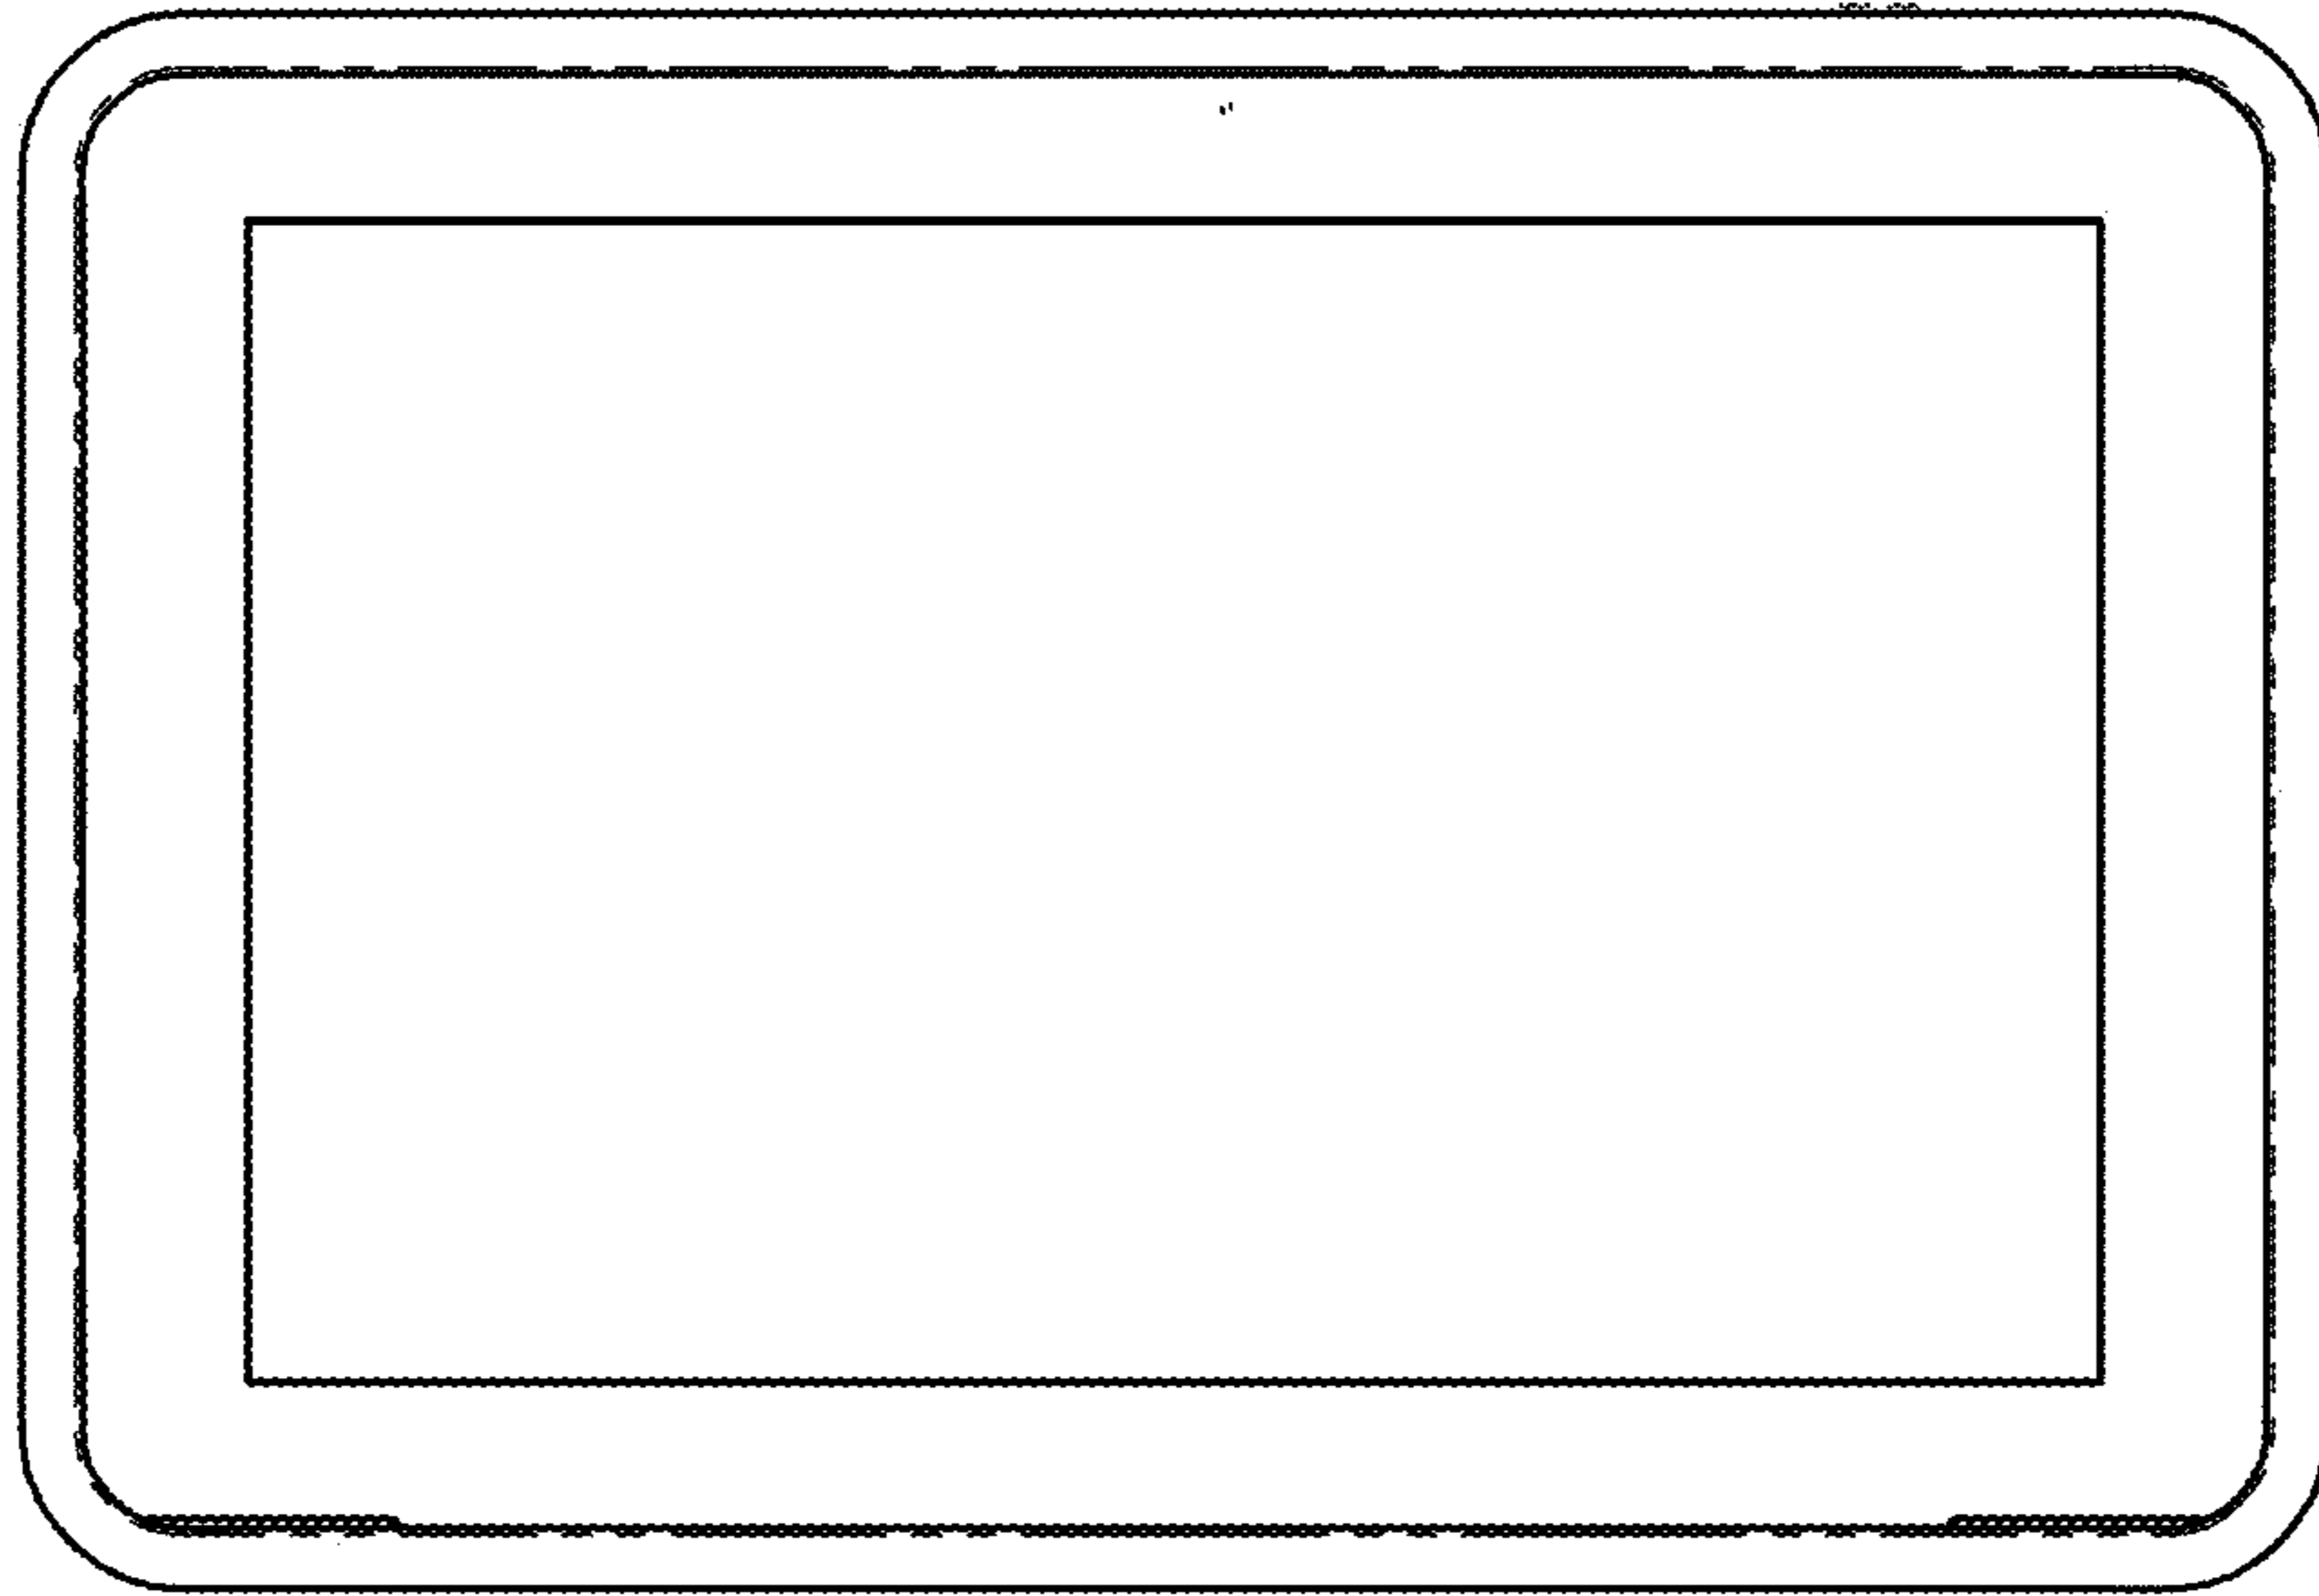


FIG. 3

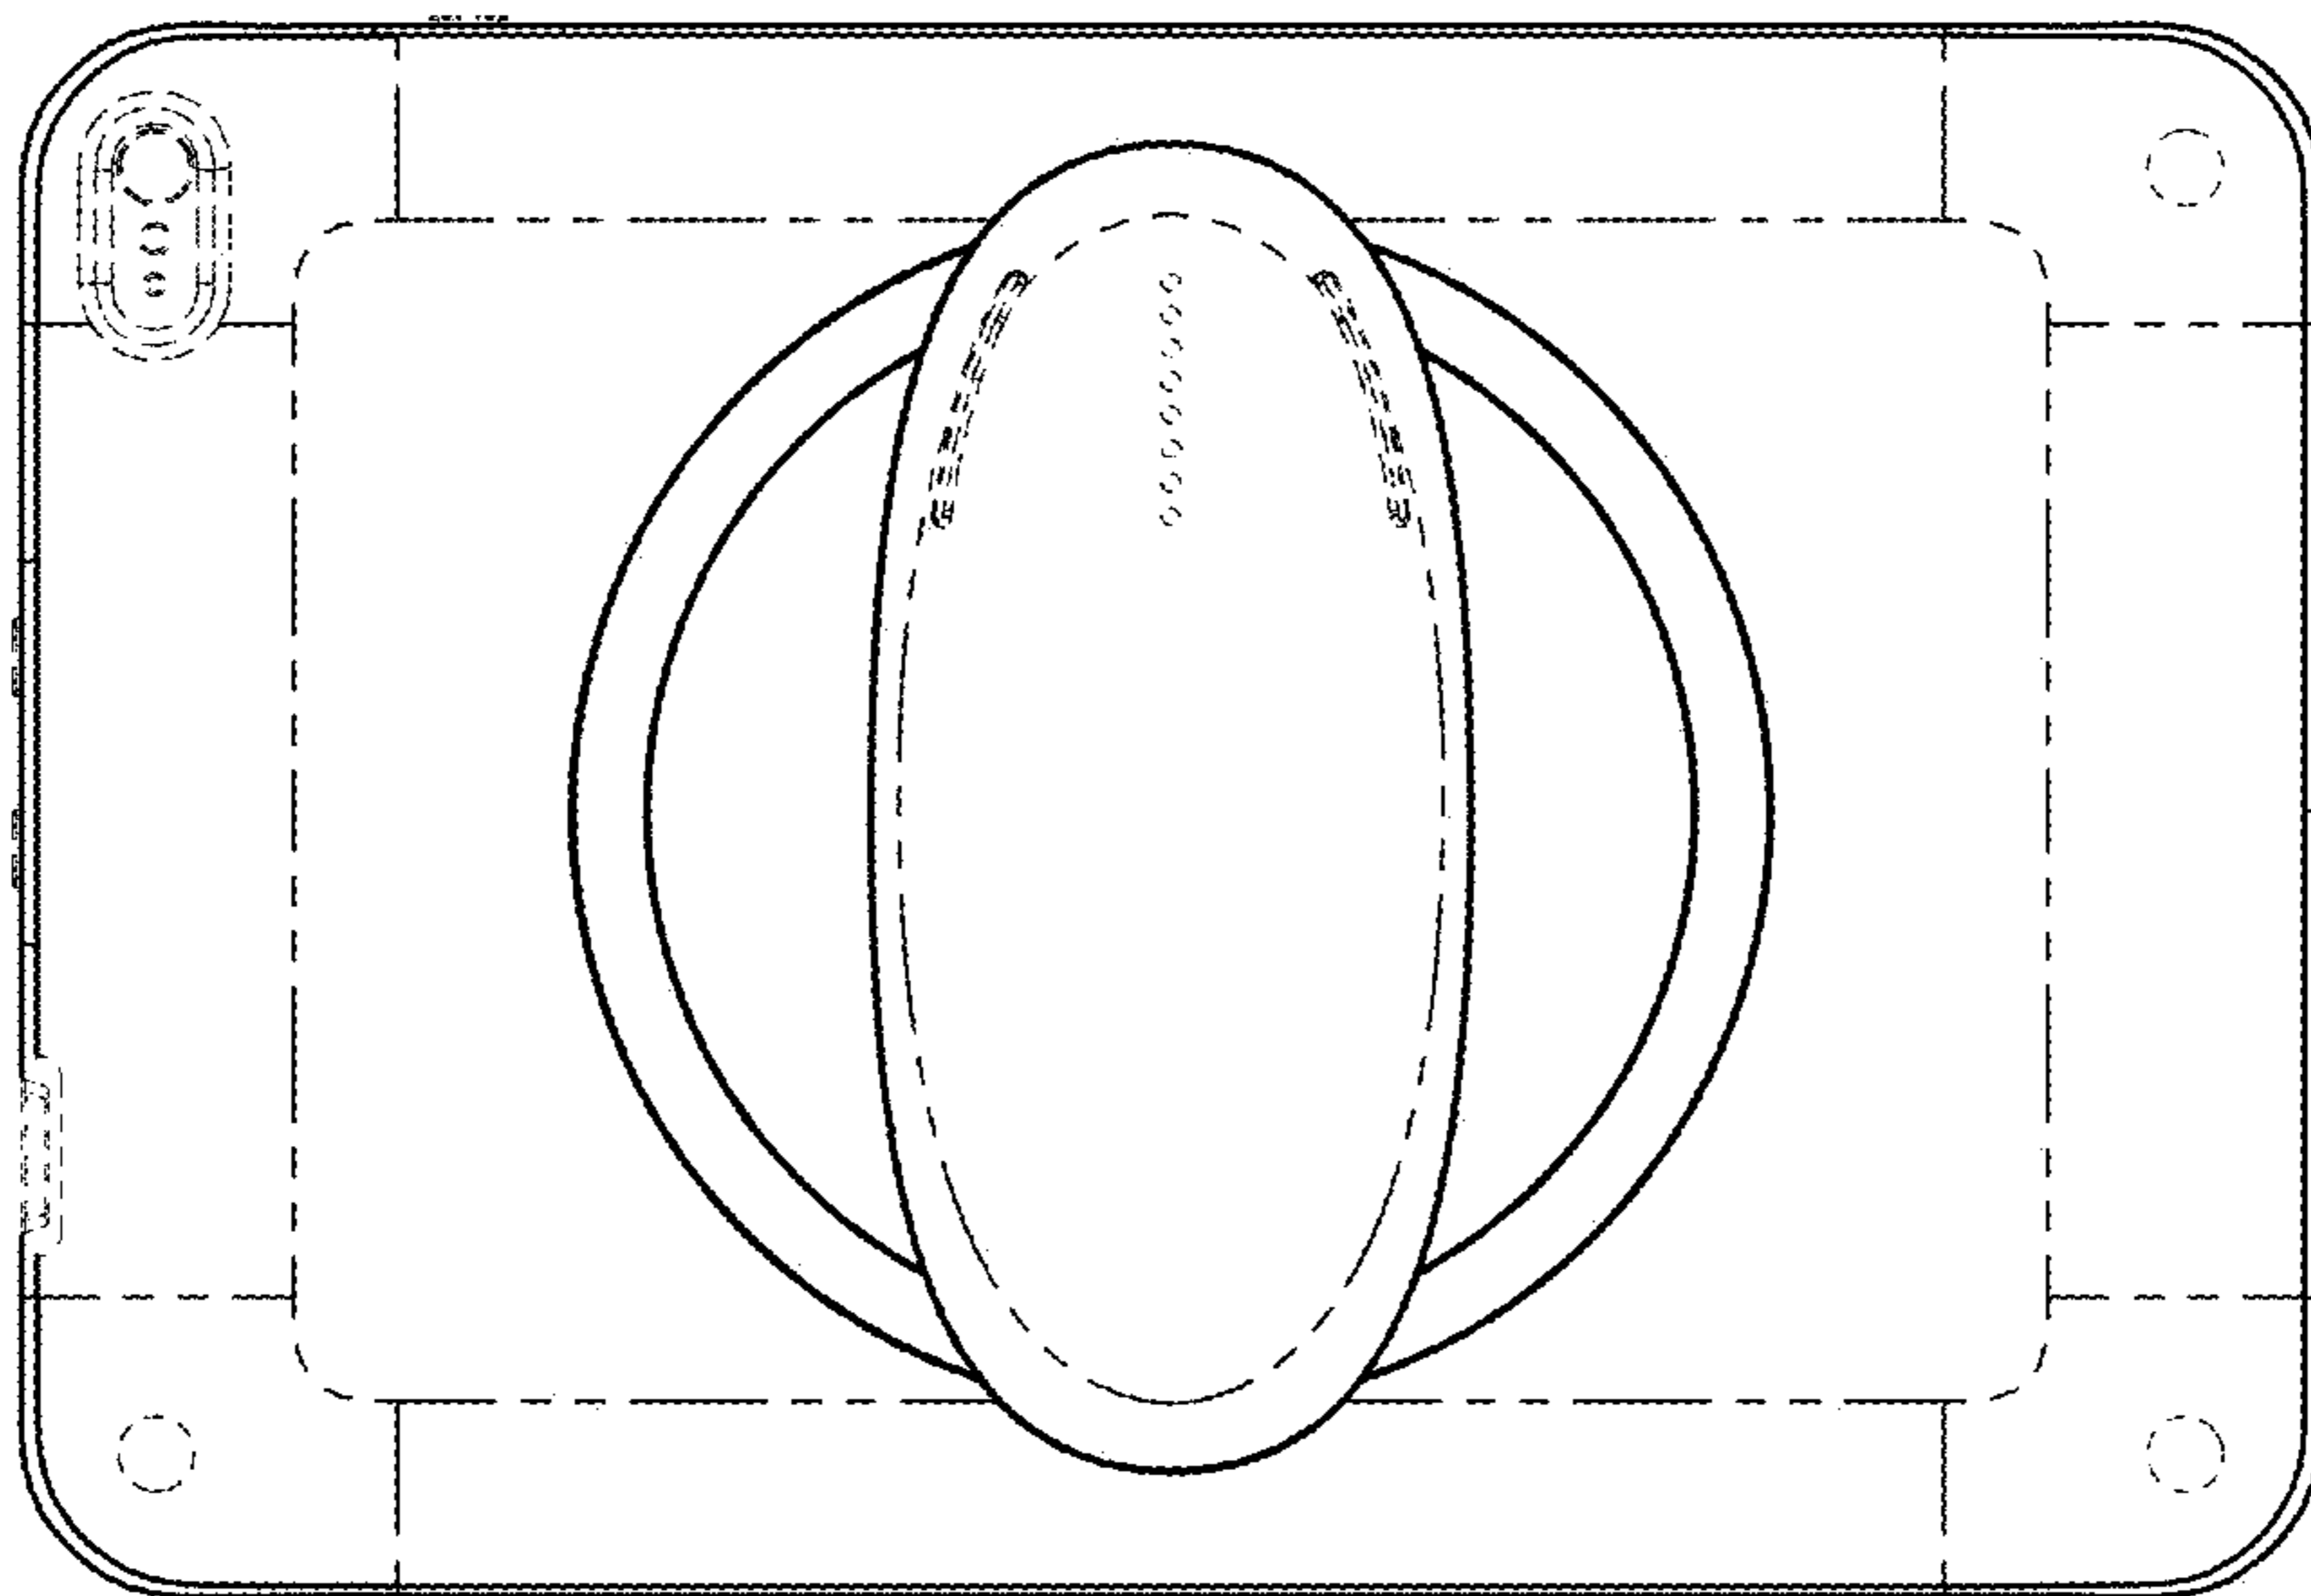


FIG. 4

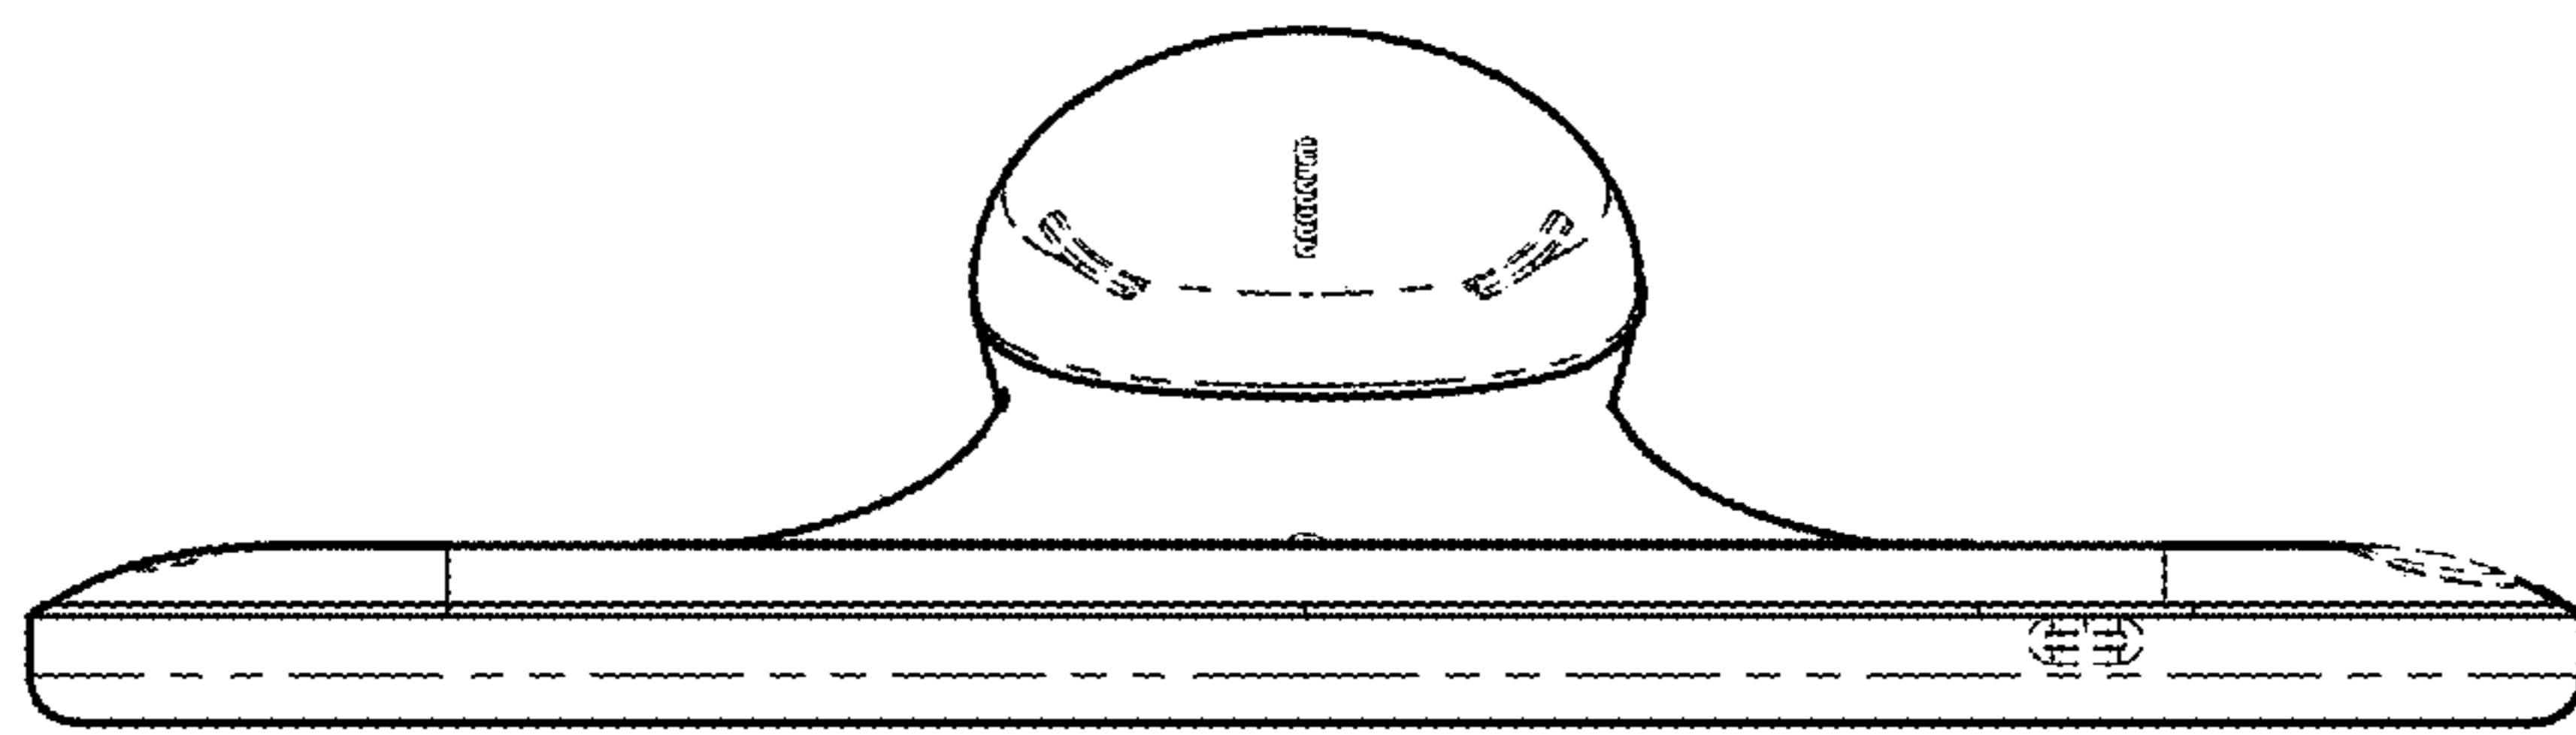


FIG. 5

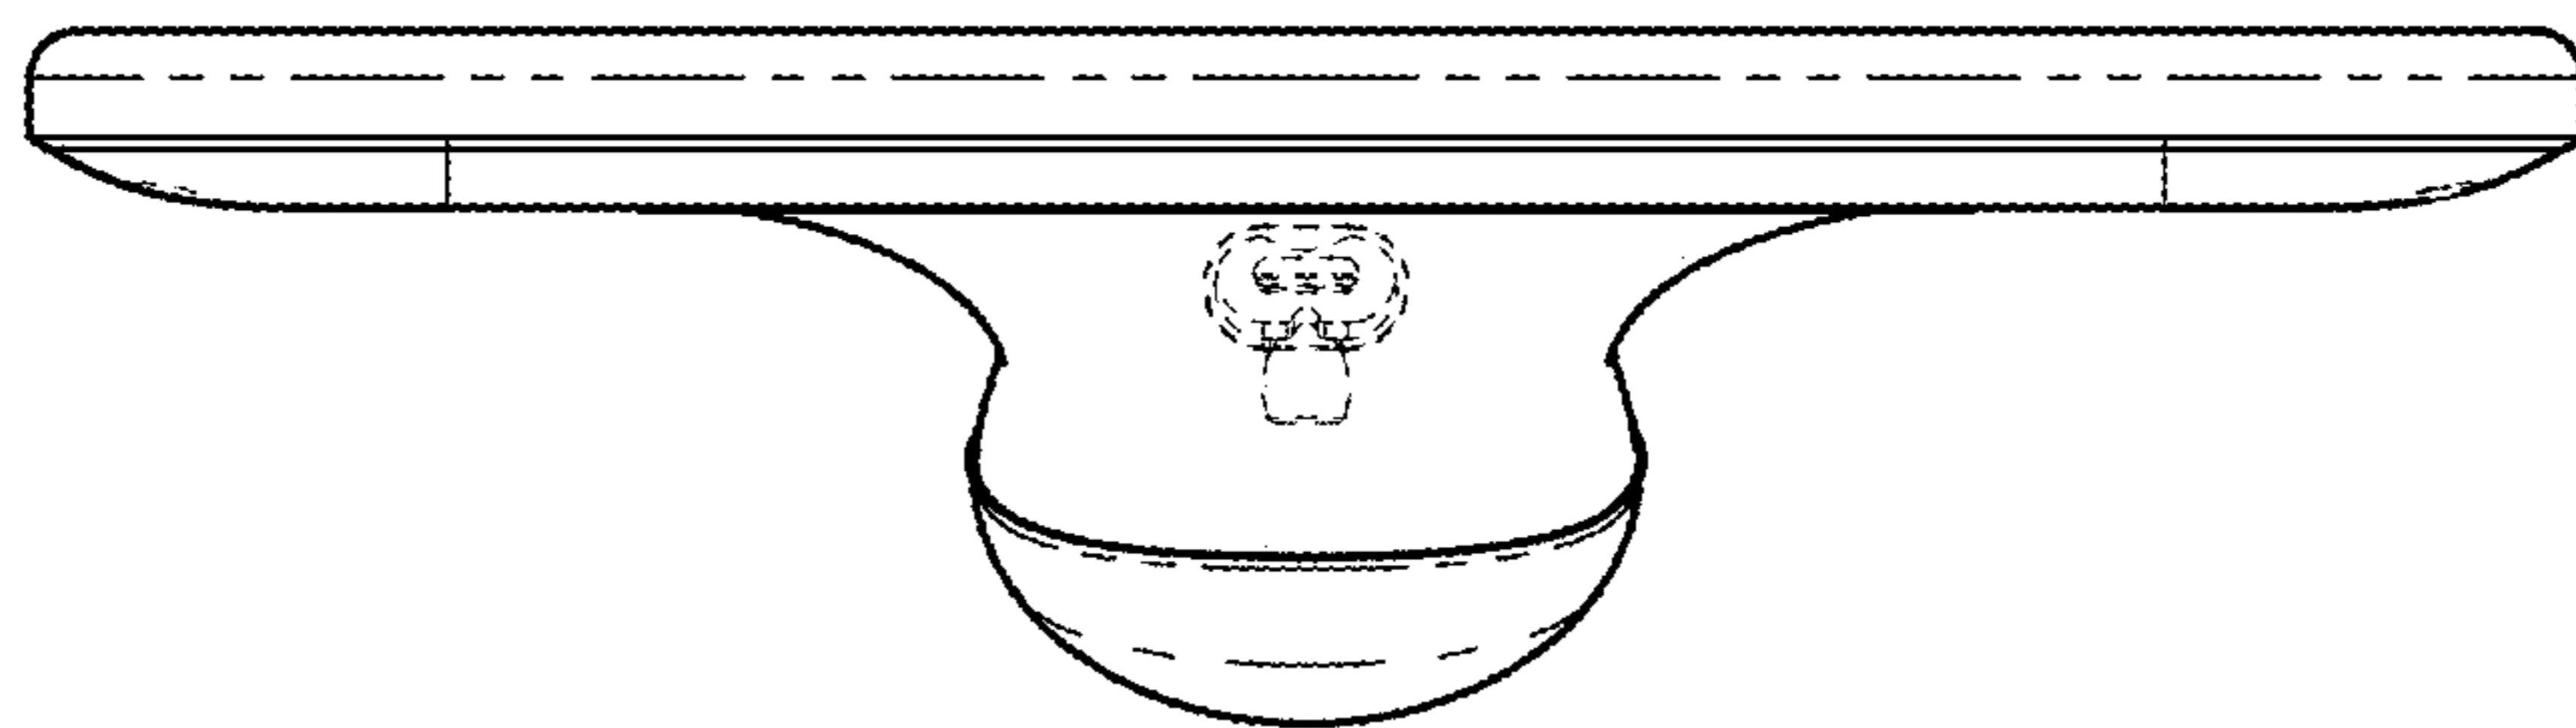


FIG. 6

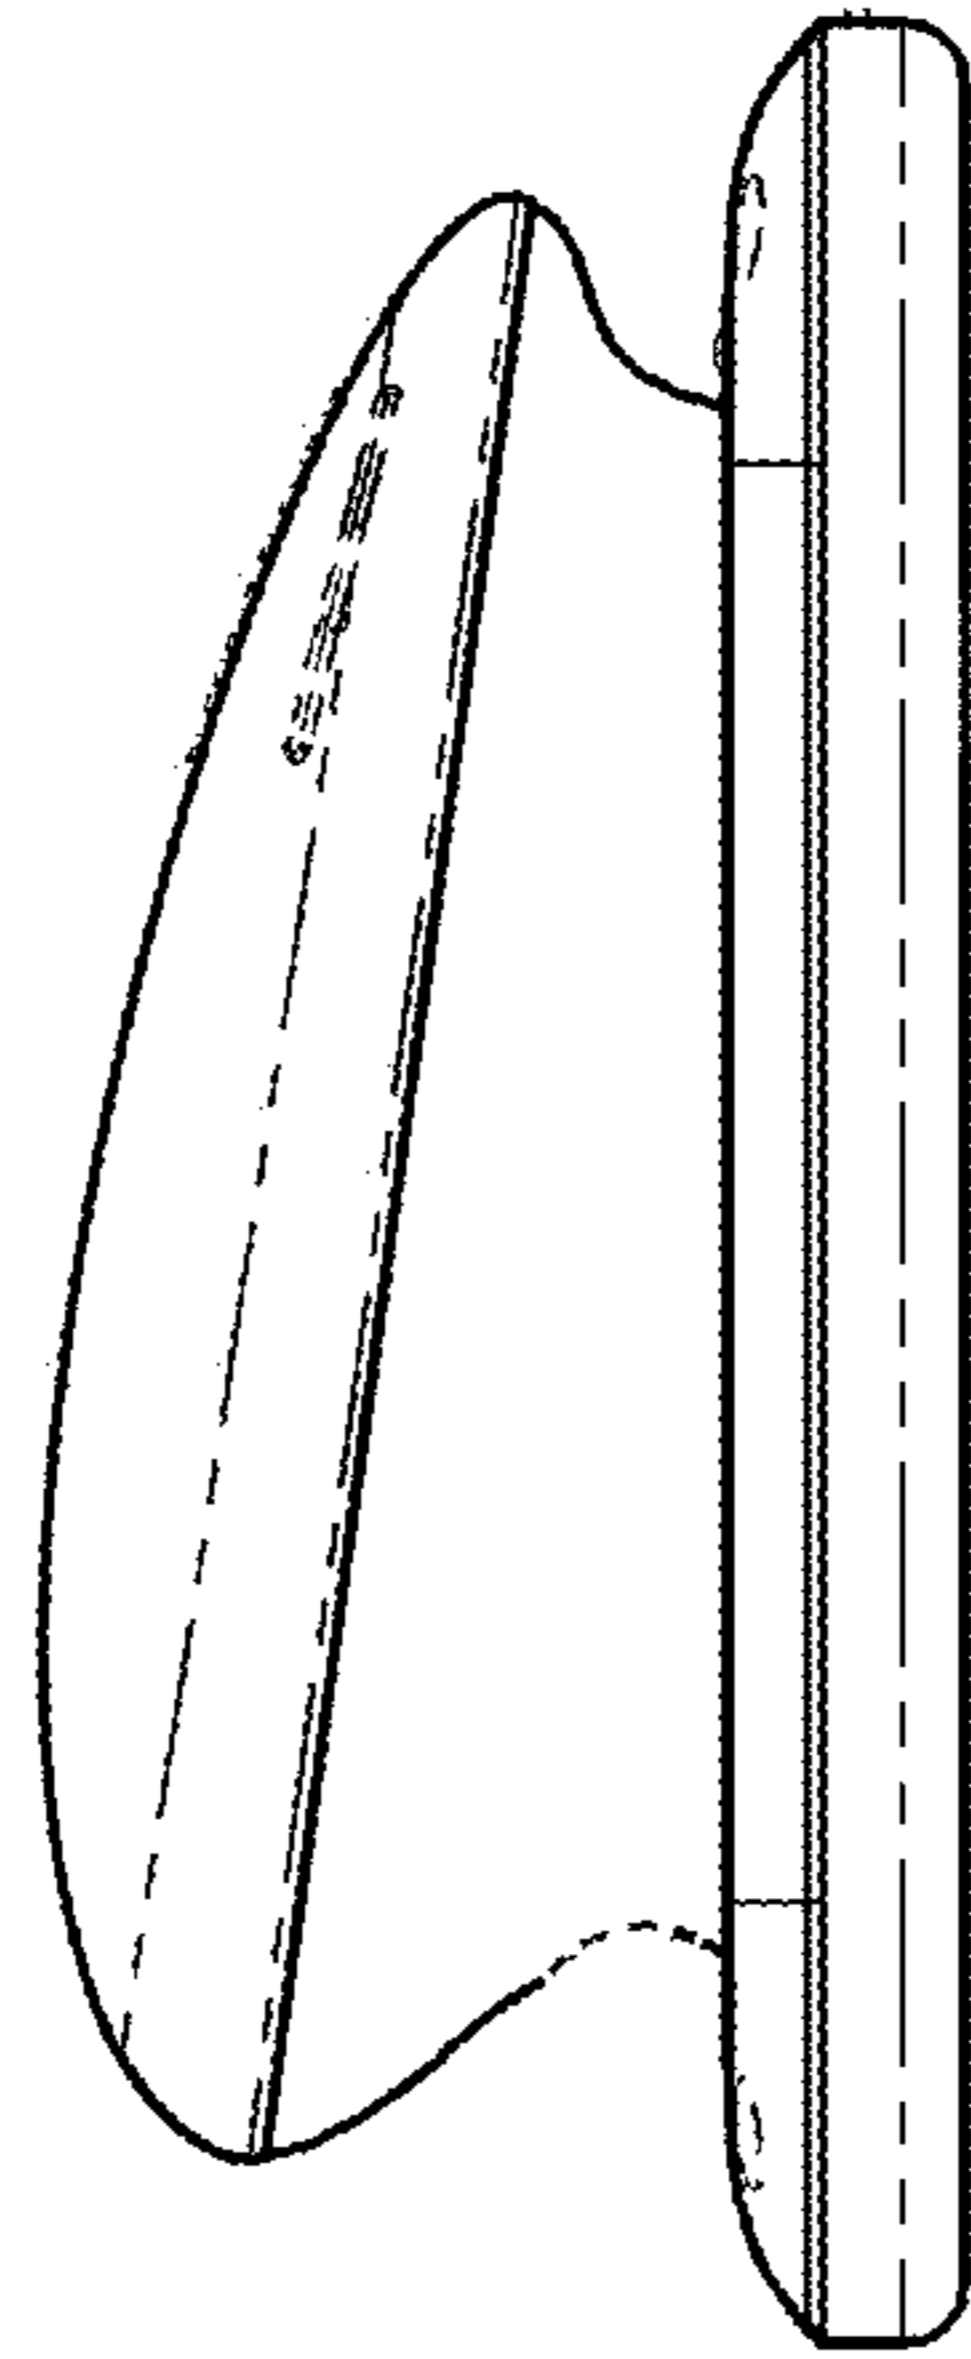


FIG. 7

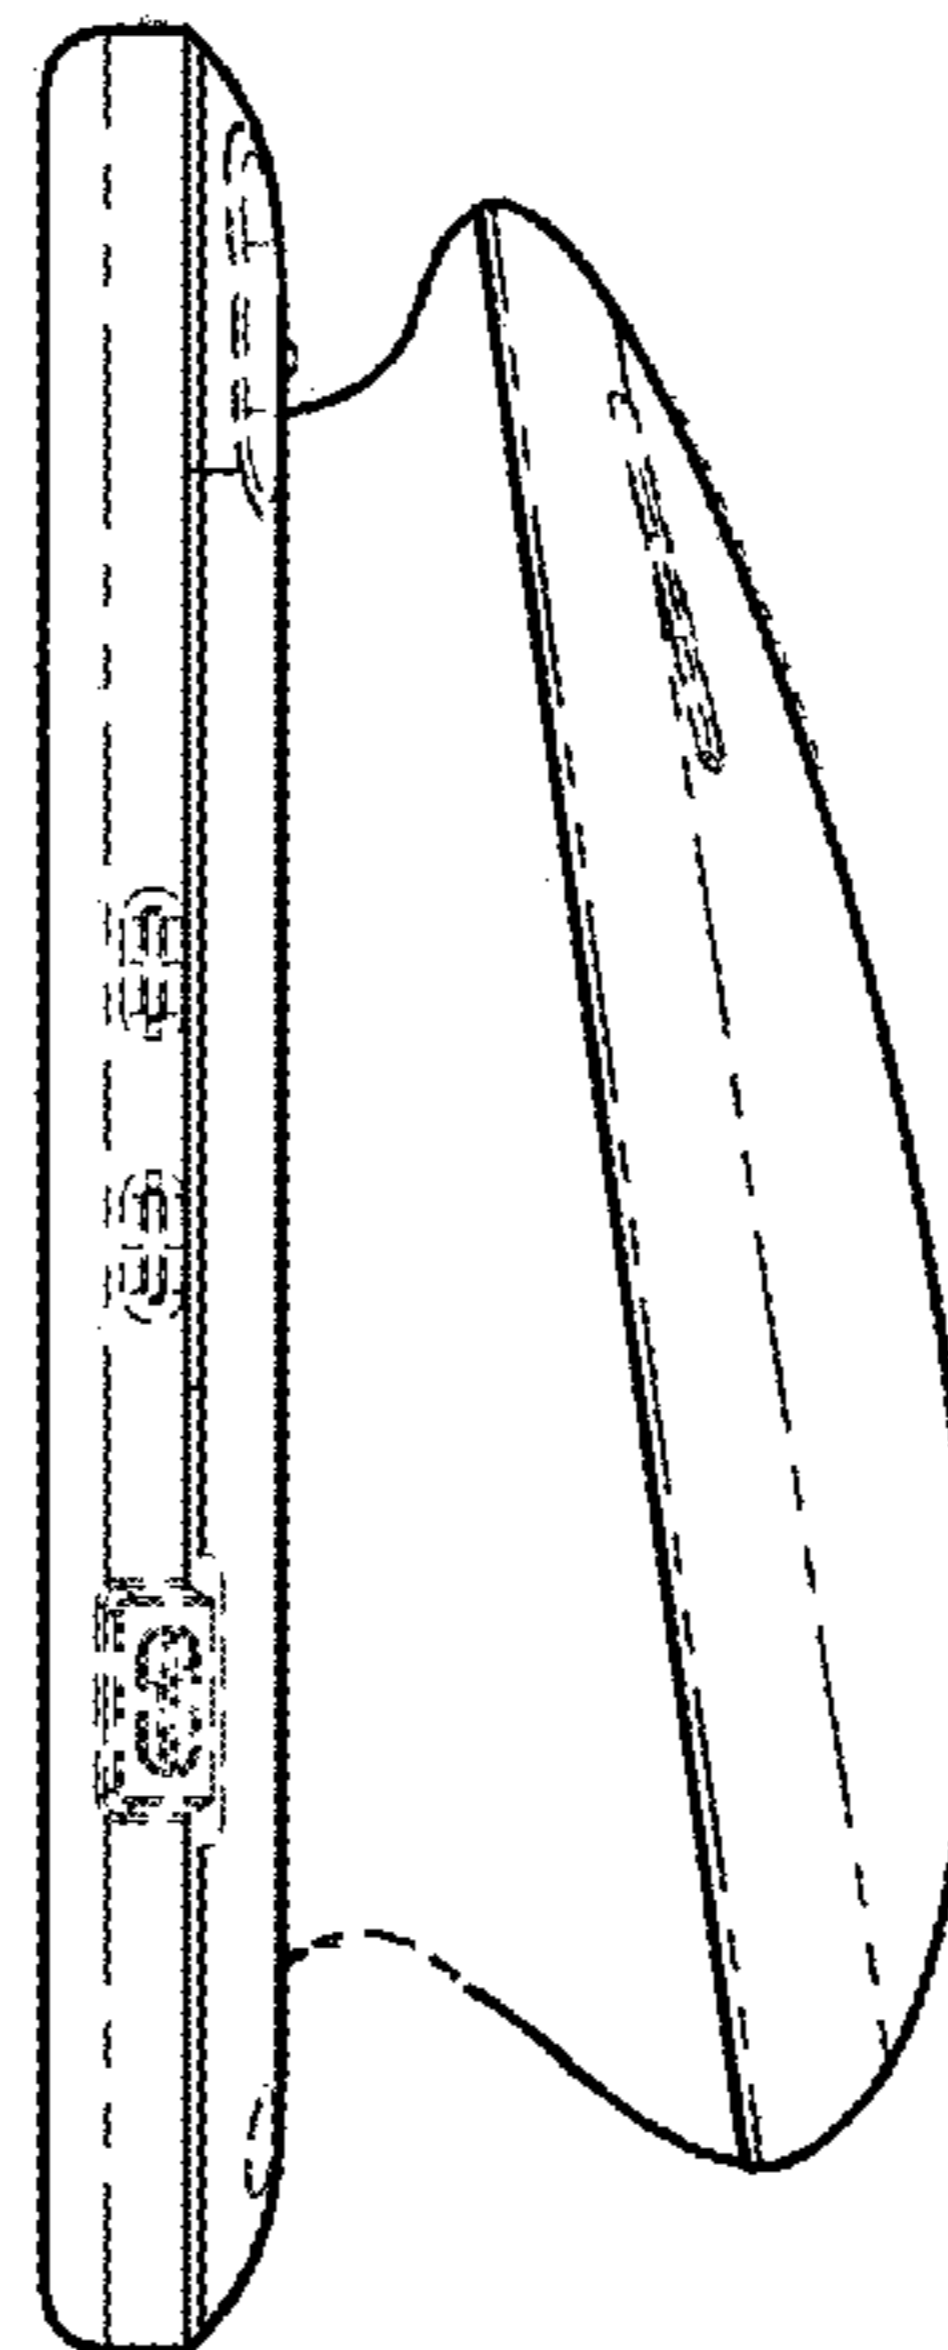


FIG. 8