



US00D940332S

(12) **United States Design Patent** (10) **Patent No.:** **US D940,332 S**  
**Weichert et al.** (45) **Date of Patent:** **\*\* Jan. 4, 2022**

(54) **PHYSIOLOGICAL MEASUREMENT DEVICE**

(56) **References Cited**

(71) Applicant: **KONINKLIJKE PHILIPS N.V.**,  
Eindhoven (NL)

U.S. PATENT DOCUMENTS

(72) Inventors: **Sven Weichert**, Waalre (NL); **Anne Stas**, Eindhoven (NL); **Stefan Toonen**, Eindhoven (NL)

D614,979 S \* 5/2010 McNames ..... D10/70  
 D821,595 S \* 6/2018 Ito ..... D24/200  
 D846,748 S \* 4/2019 Benedikter ..... D24/186  
 D850,627 S \* 6/2019 Purani ..... D24/186  
 D852,965 S \* 7/2019 Bahney ..... A61B 5/721  
 D24/186

(73) Assignee: **KONINKLIJKE PHILIPS N.V.**,  
Eindhoven (NL)

D854,162 S \* 7/2019 Rihu ..... D24/167  
 D874,659 S \* 2/2020 Wetmore ..... D24/187  
 D886,303 S \* 6/2020 Huang ..... D24/187  
 D890,348 S \* 7/2020 Lam ..... D24/167  
 D910,187 S \* 2/2021 Benedikter ..... D24/186  
 D914,218 S \* 3/2021 Govari ..... D24/186  
 D914,219 S \* 3/2021 Huang ..... D24/187

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/745,652**

2015/0282712 A1 \* 10/2015 Presura ..... A61B 5/6831  
600/301

(22) Filed: **Aug. 7, 2020**

2016/0120434 A1 \* 5/2016 Park ..... A61B 5/0006  
600/301

(30) **Foreign Application Priority Data**

2021/0007623 A1 \* 1/2021 Sano ..... A61B 5/282

Feb. 7, 2020 (EM) ..... 007673140

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(51) **LOC (13) Cl.** ..... **24-02**

(57) **CLAIM**

(52) **U.S. Cl.**  
USPC ..... **D24/186**

The ornamental design for a physiological measurement device, as shown.


(58) **Field of Classification Search**  
 USPC ..... D24/107, 165–169, 186, 187, 200;  
 D10/70, 98; D14/341, 344  
 CPC ..... A61B 5/006; A61B 5/0245; A61B 5/346;  
 A61B 5/332; A61B 5/6833; A61B 5/257;  
 A61B 5/256; A61B 2560/0412; A61B  
 2560/0462; A61B 5/0205; A61B 5/02405;  
 A61B 5/02438; A61B 5/6823; A61B  
 5/6824; A61B 5/68335; A61B 2562/18;  
 A61B 2562/0209

**DESCRIPTION**

FIG. 1 is a perspective view showing a physiological measurement device design;  
 FIG. 2 is a front elevational view thereof;  
 FIG. 3 is a rear elevational view thereof;  
 FIG. 4 is a right side elevational view thereof;  
 FIG. 5 is a left side elevational view thereof;  
 FIG. 6 is a top plan view thereof; and,  
 FIG. 7 is a bottom plan view thereof.

See application file for complete search history.

**1 Claim, 7 Drawing Sheets**

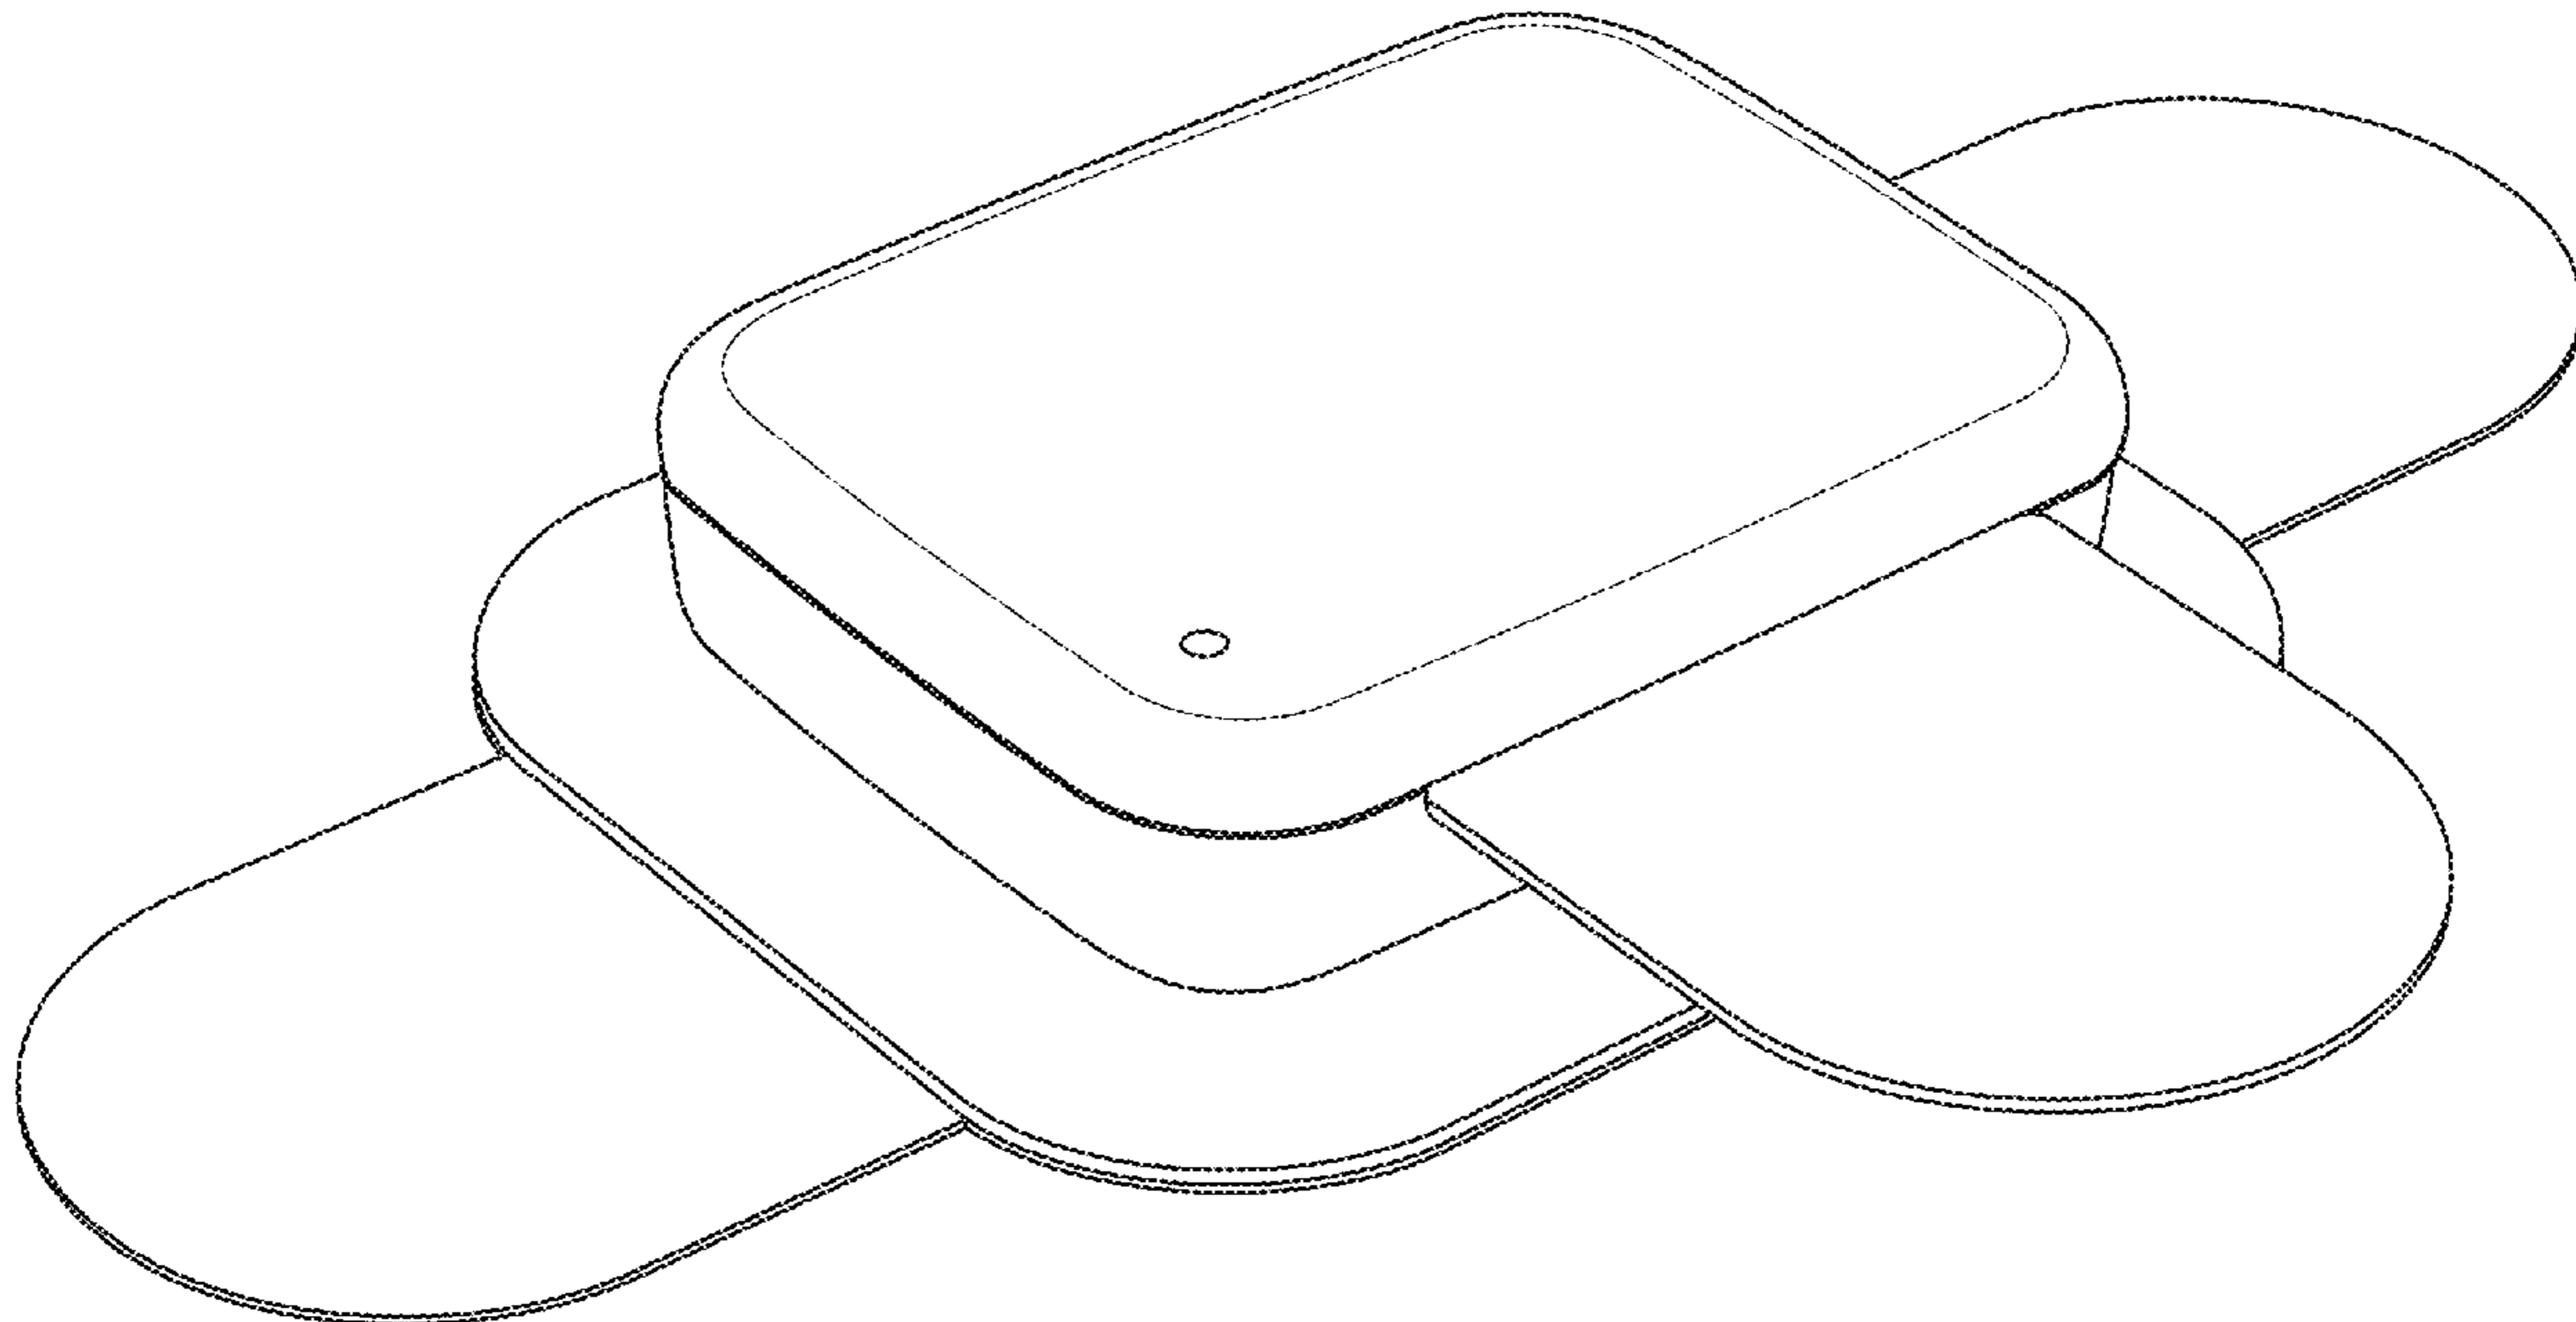

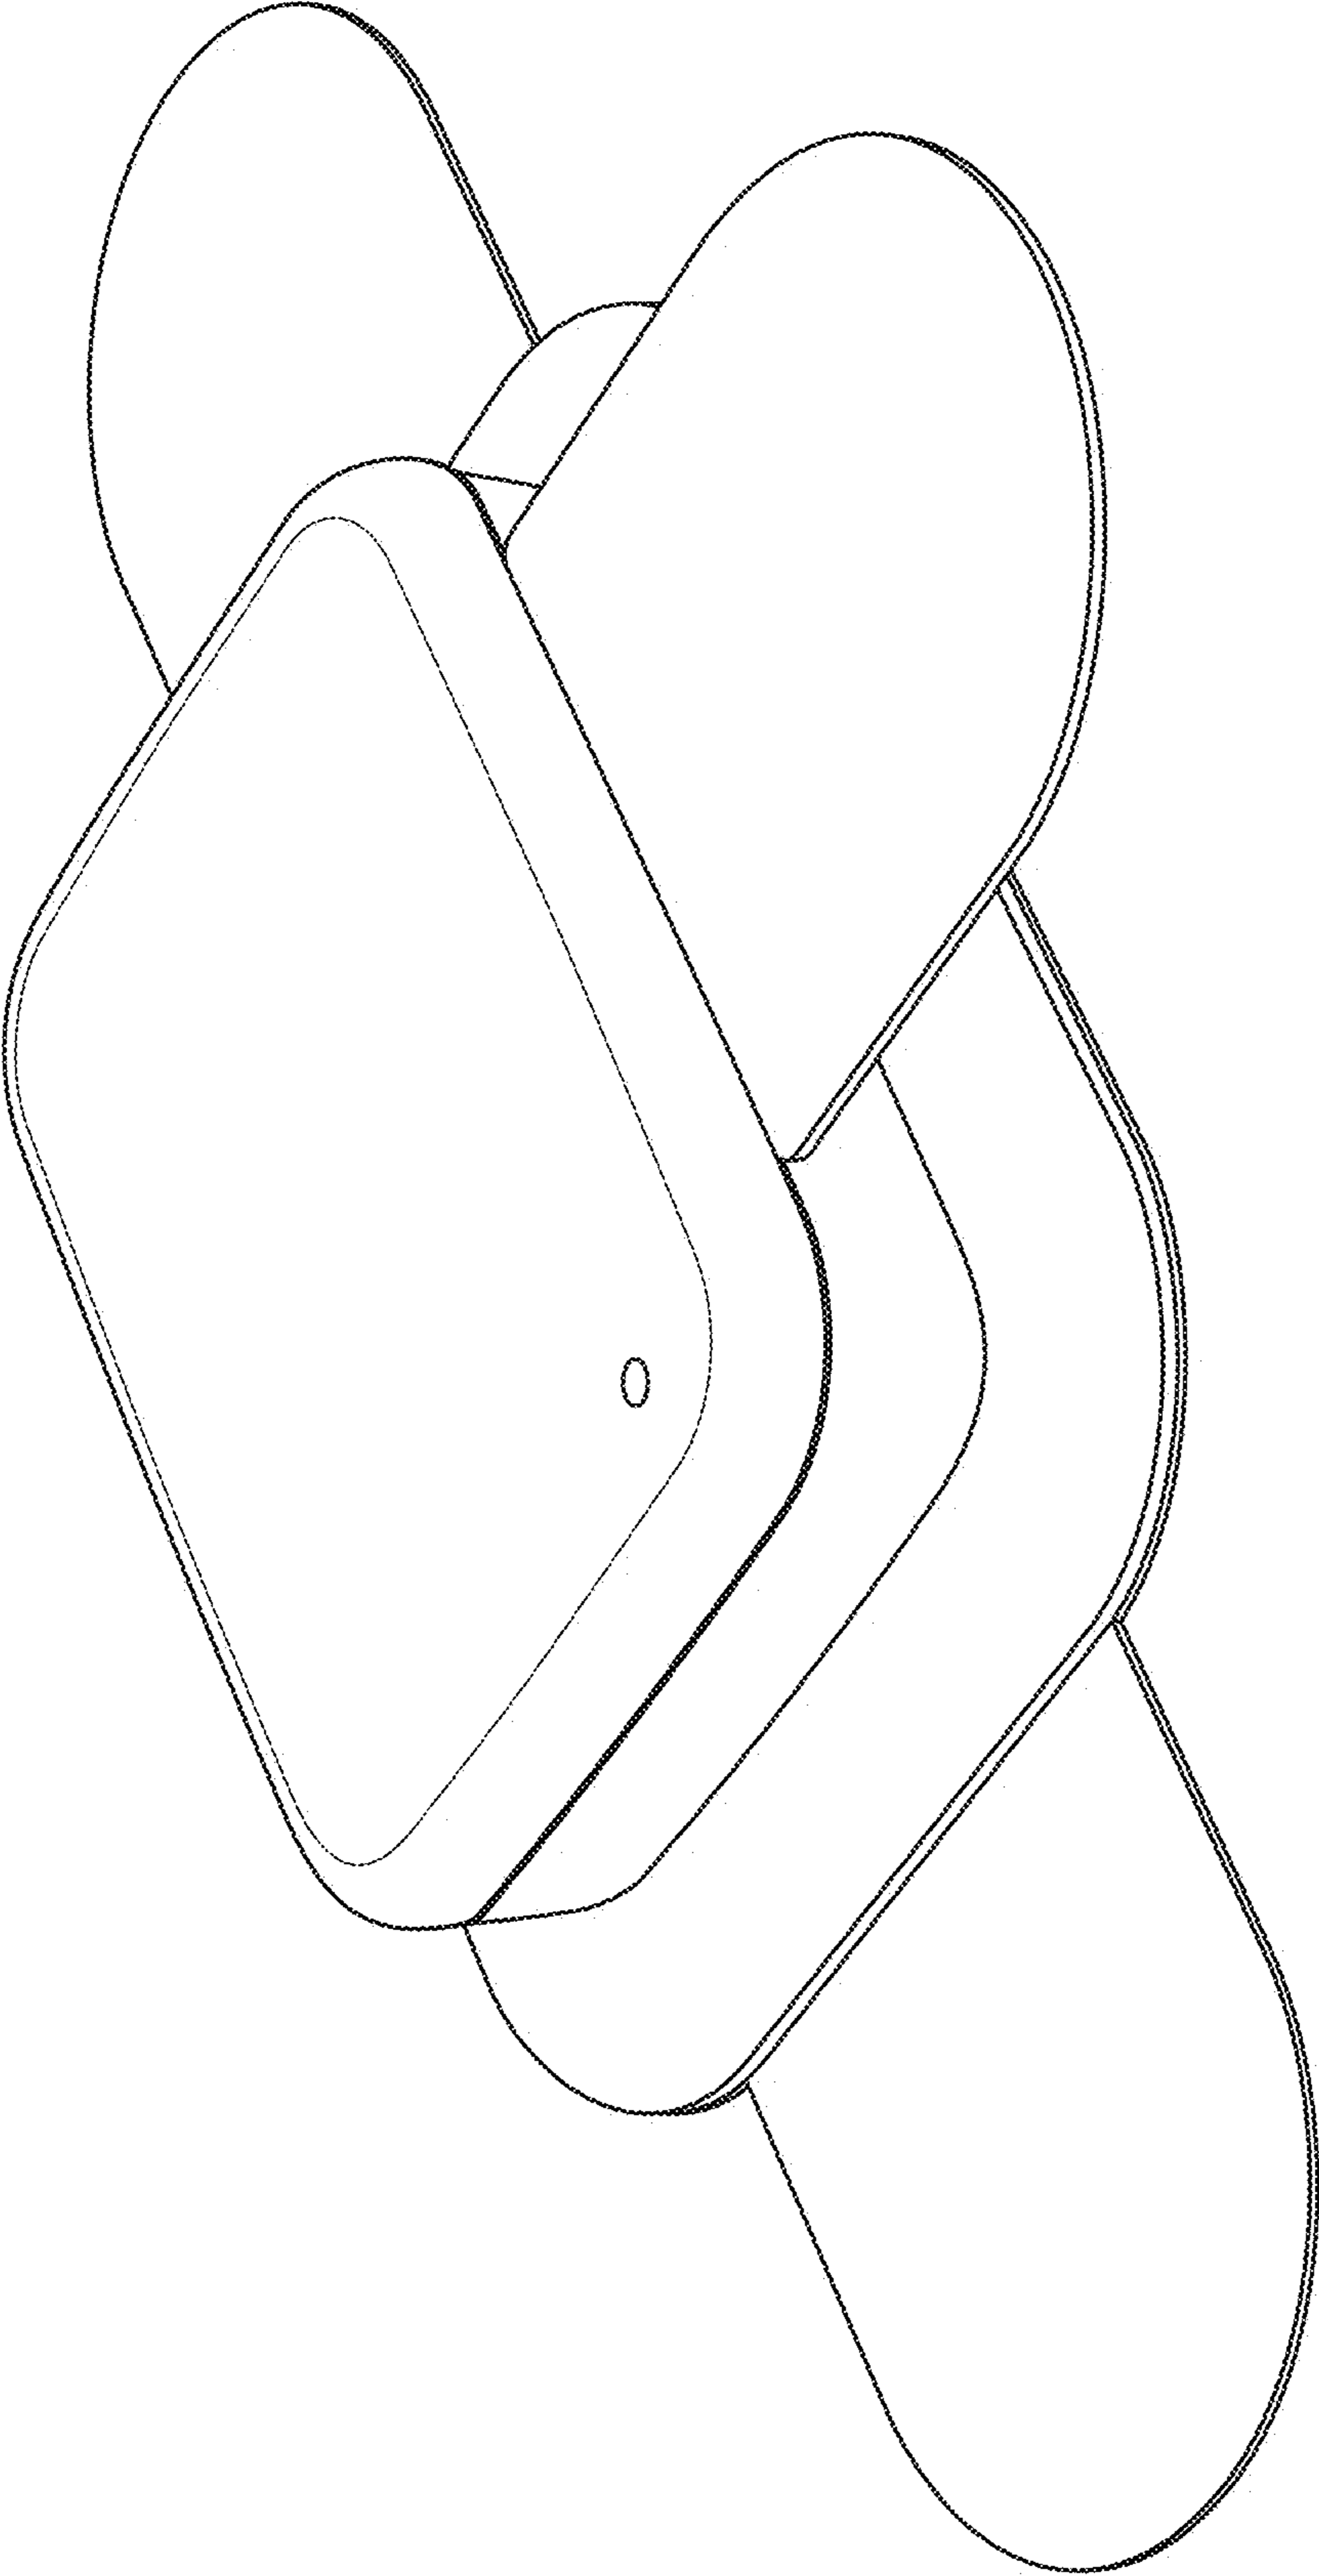


FIG. 1

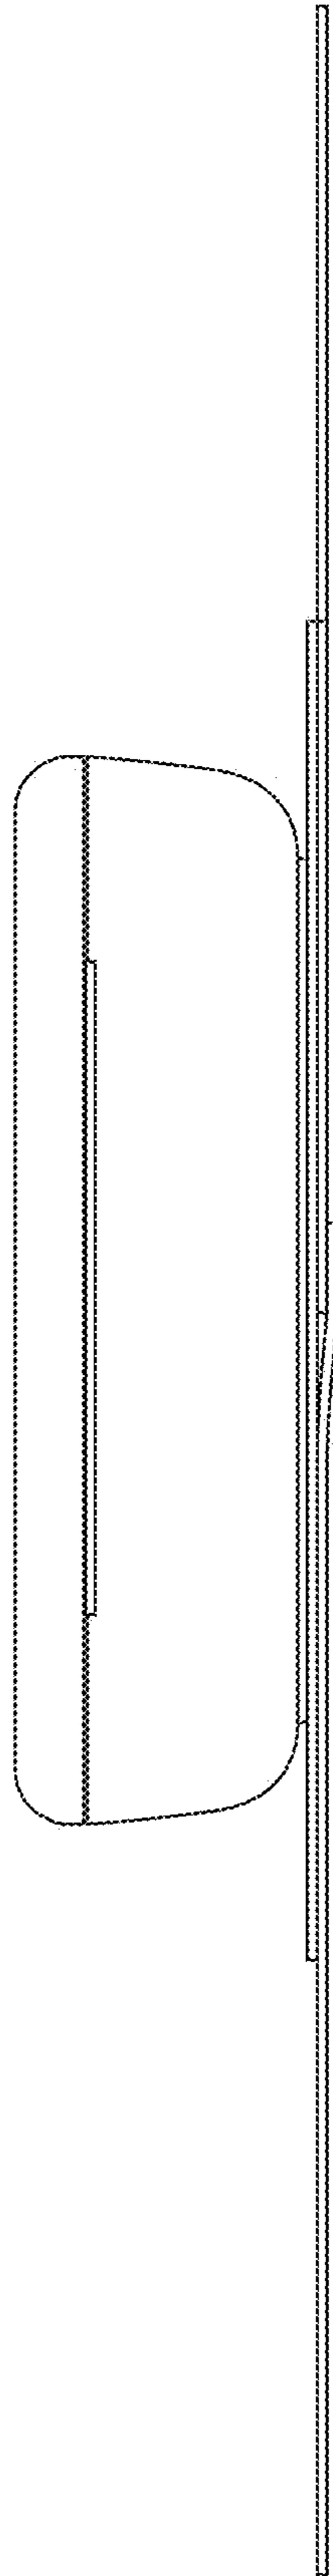


FIG. 2

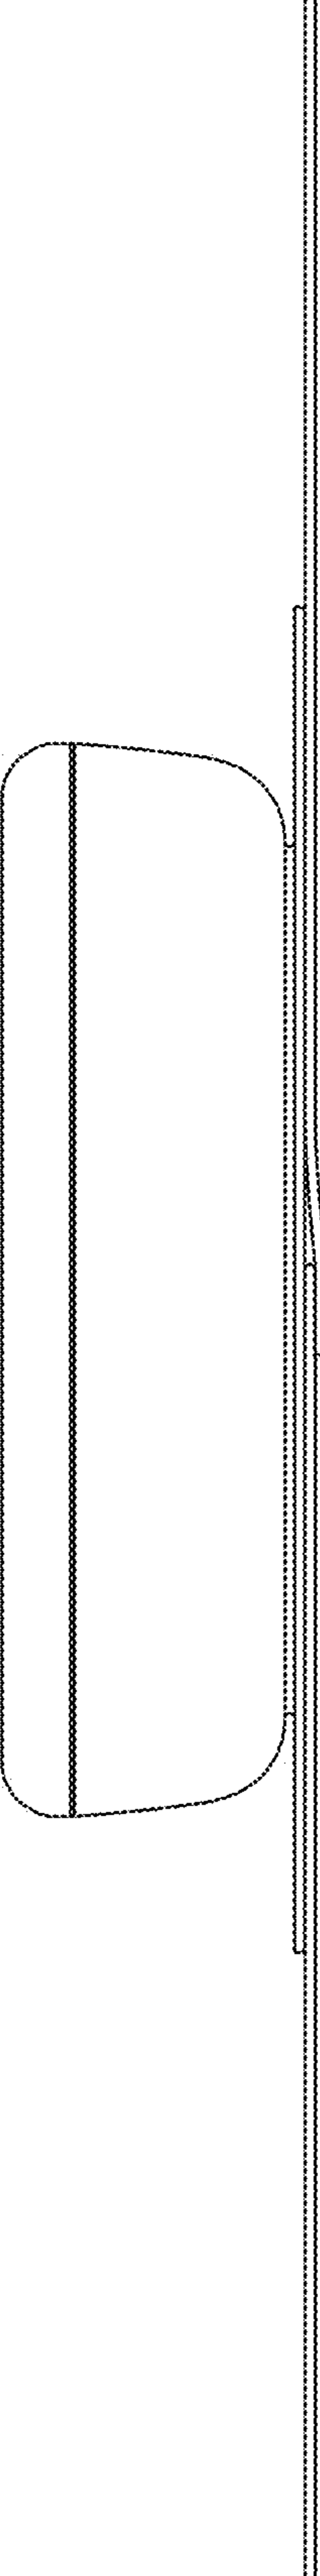


FIG. 3

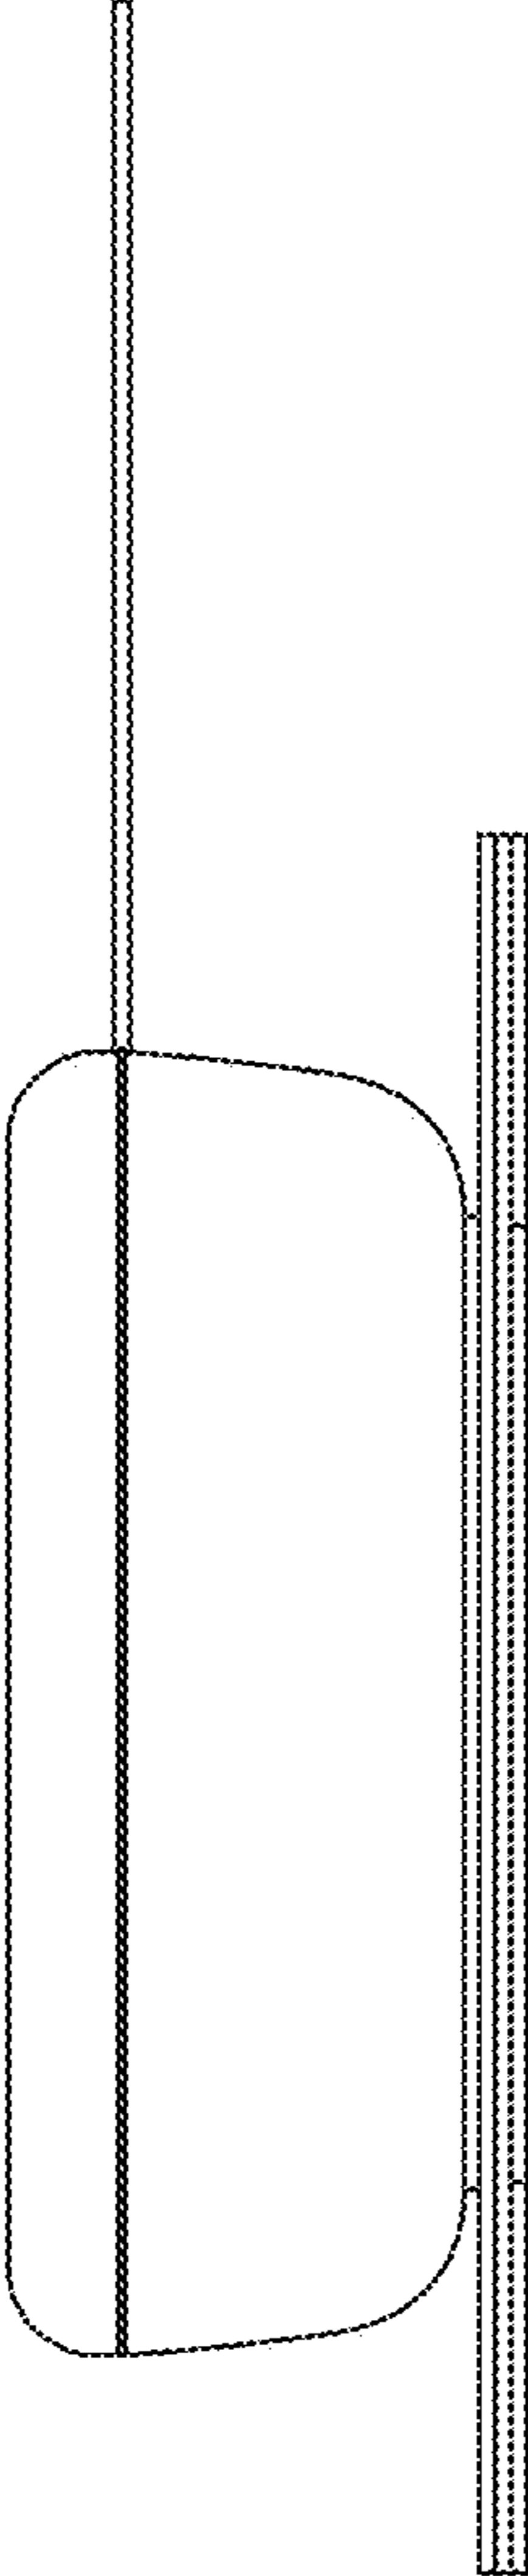


FIG. 4

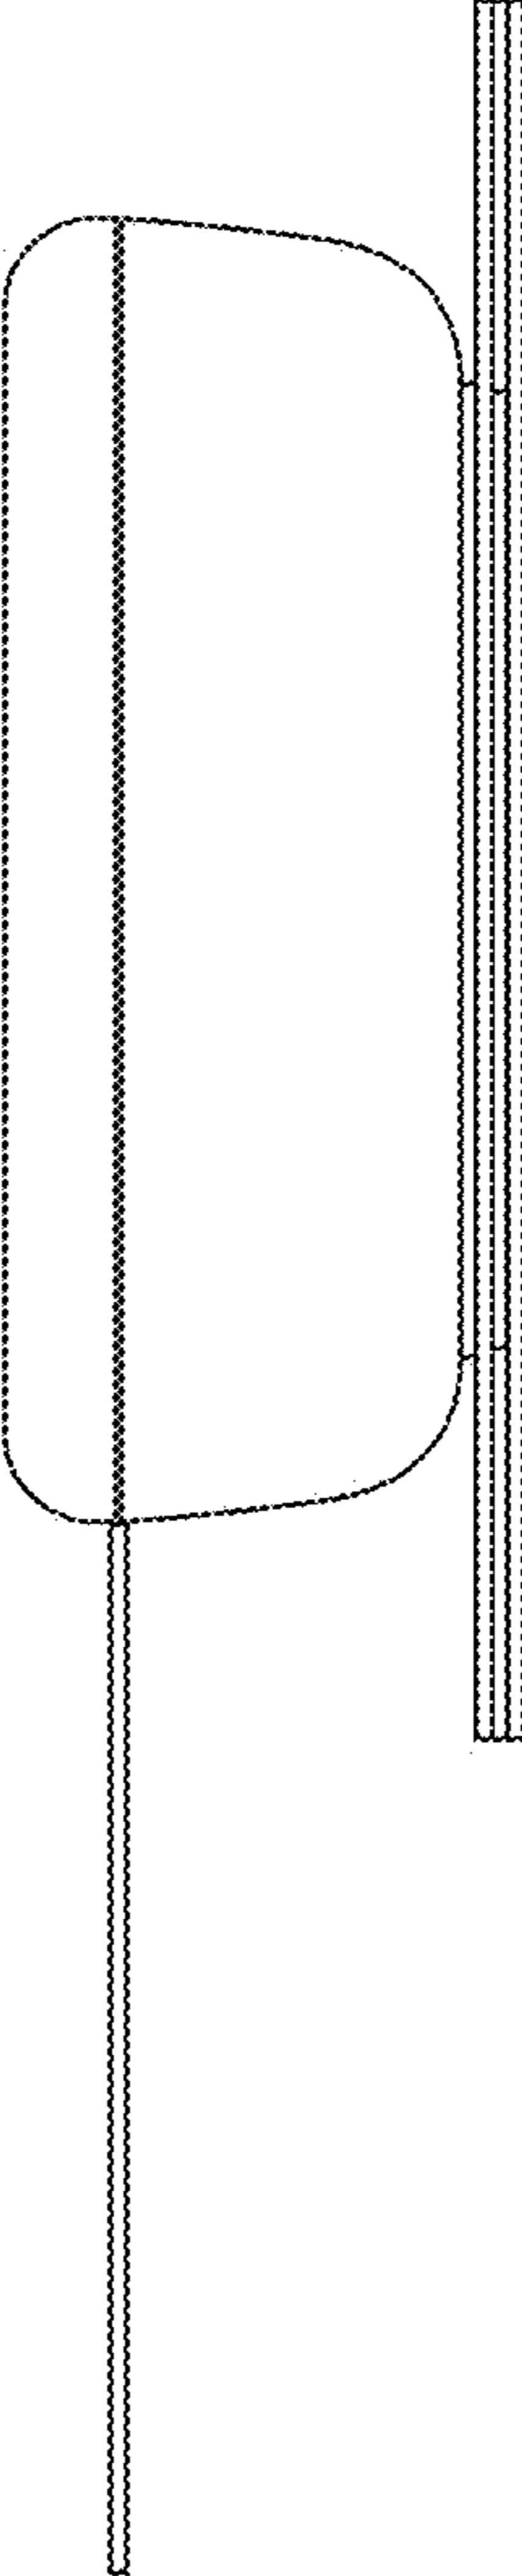


FIG. 5

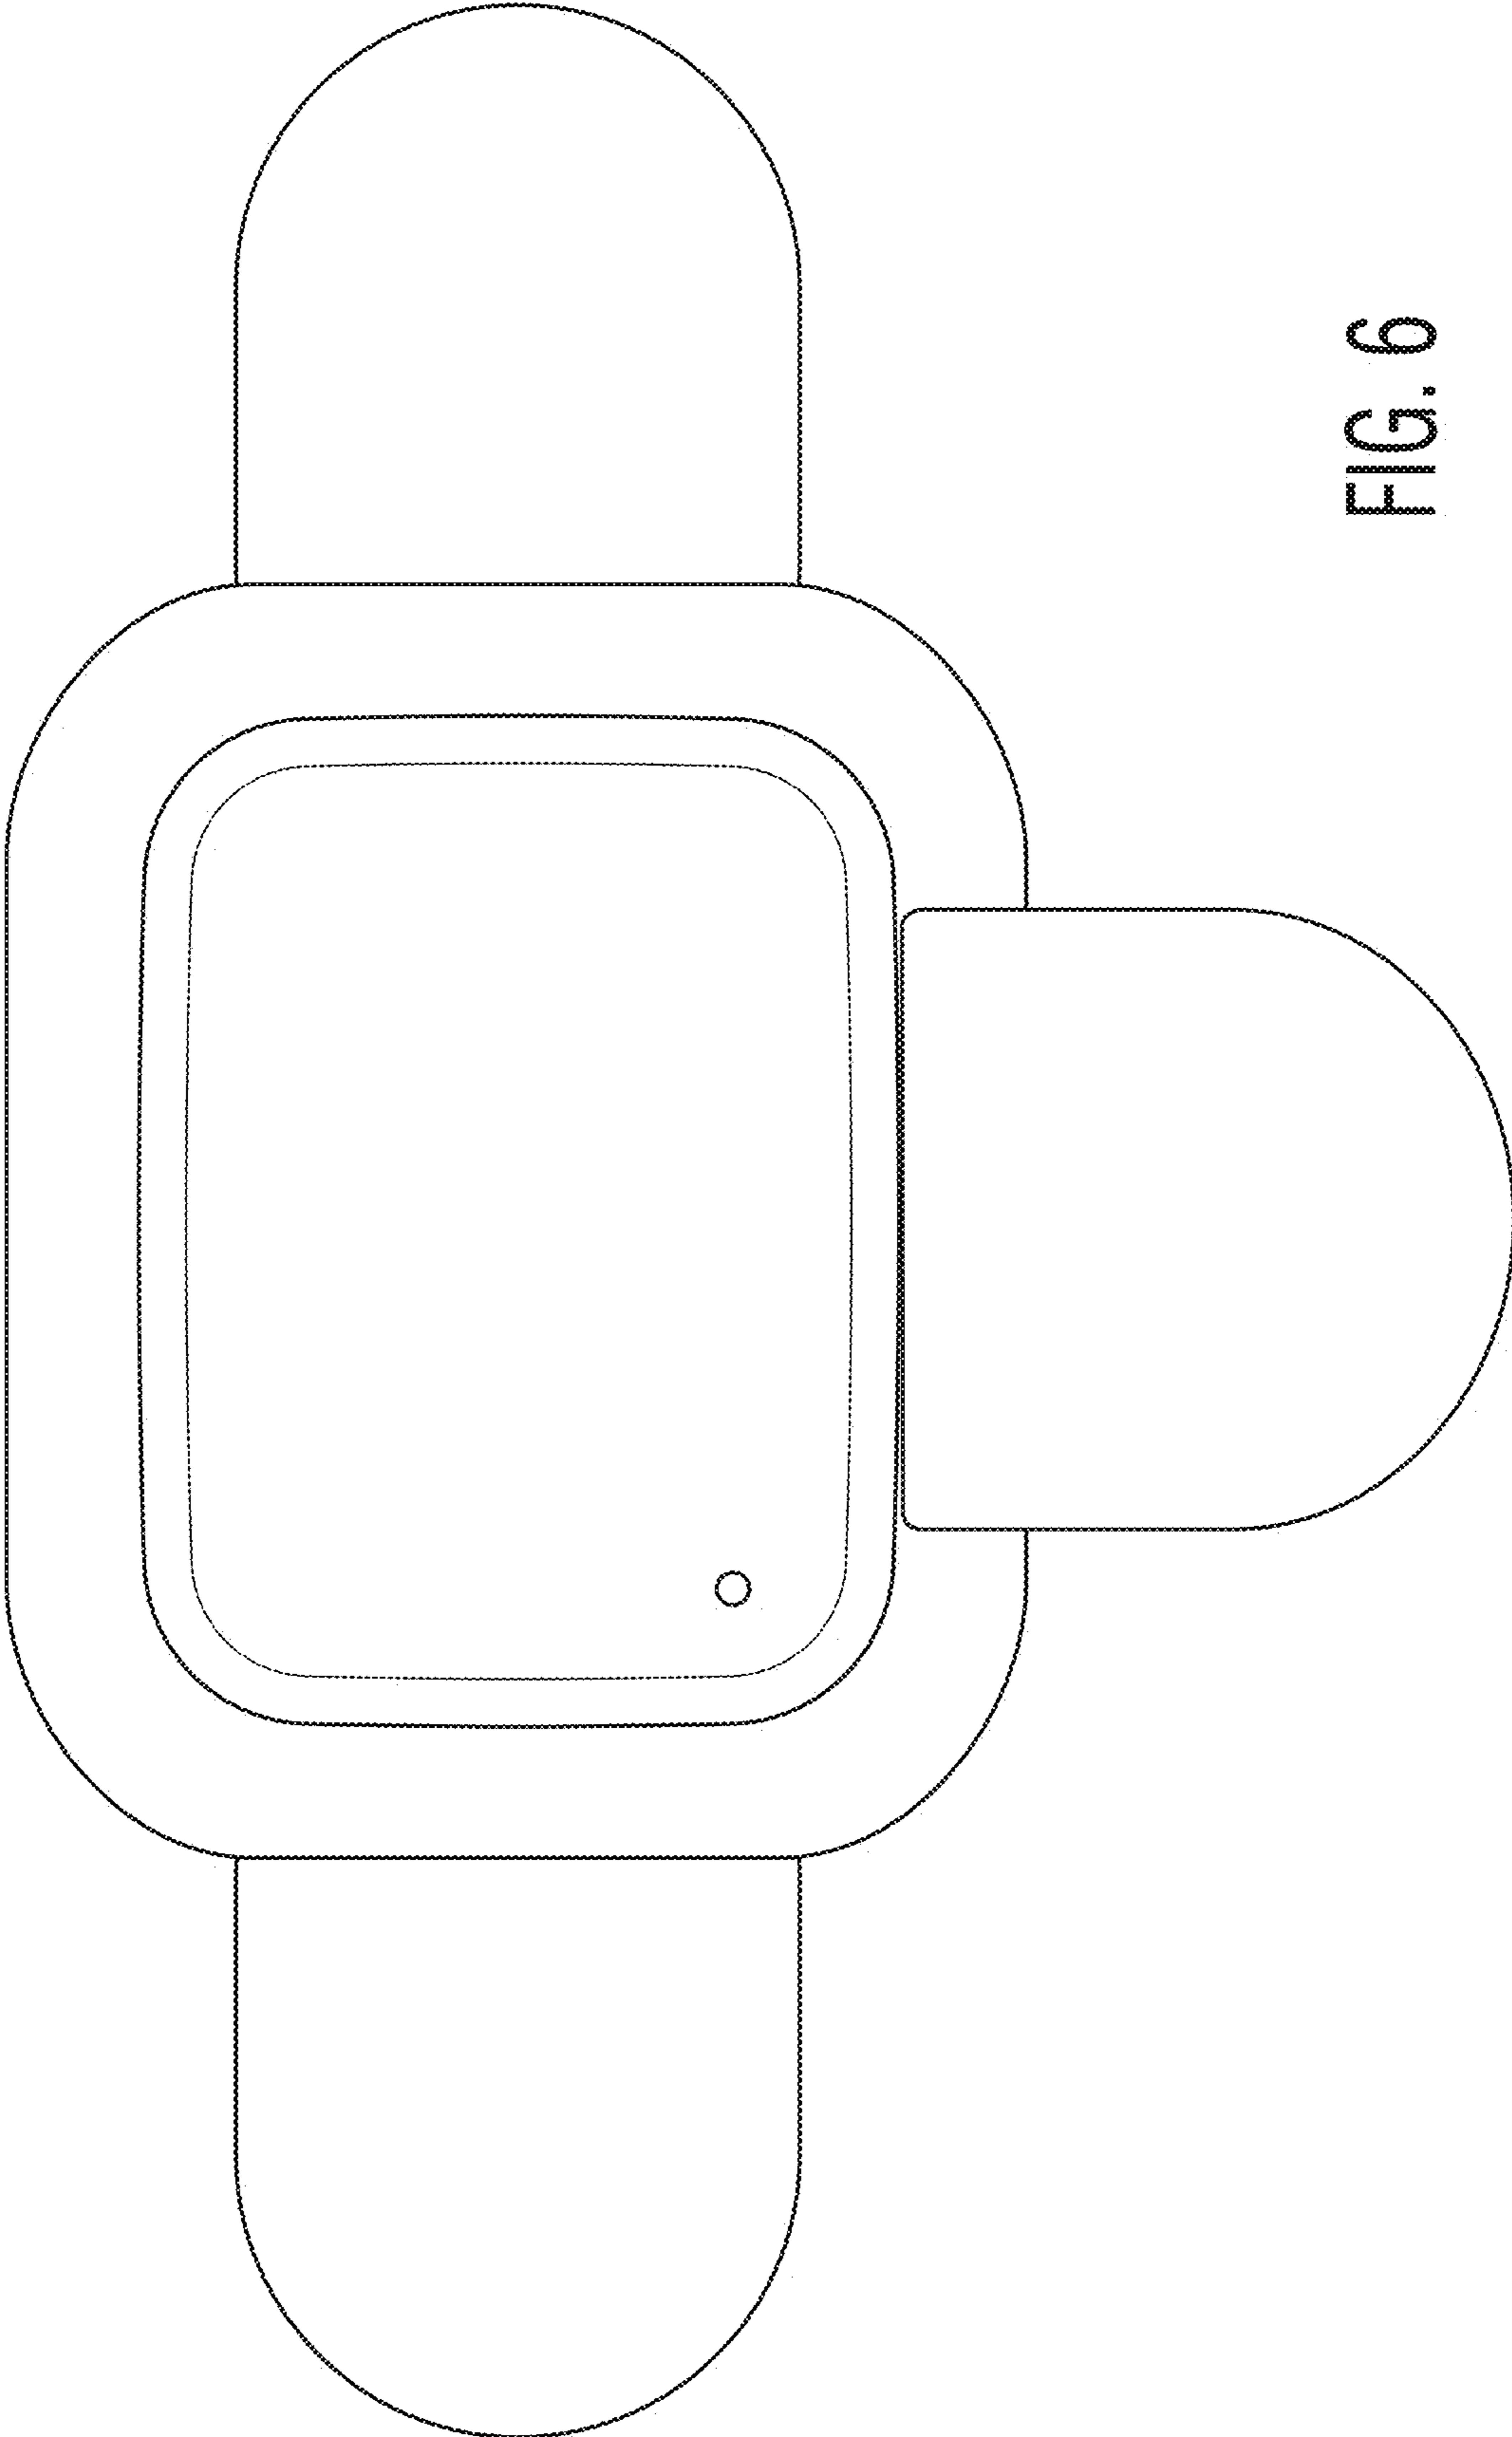


FIG. 6

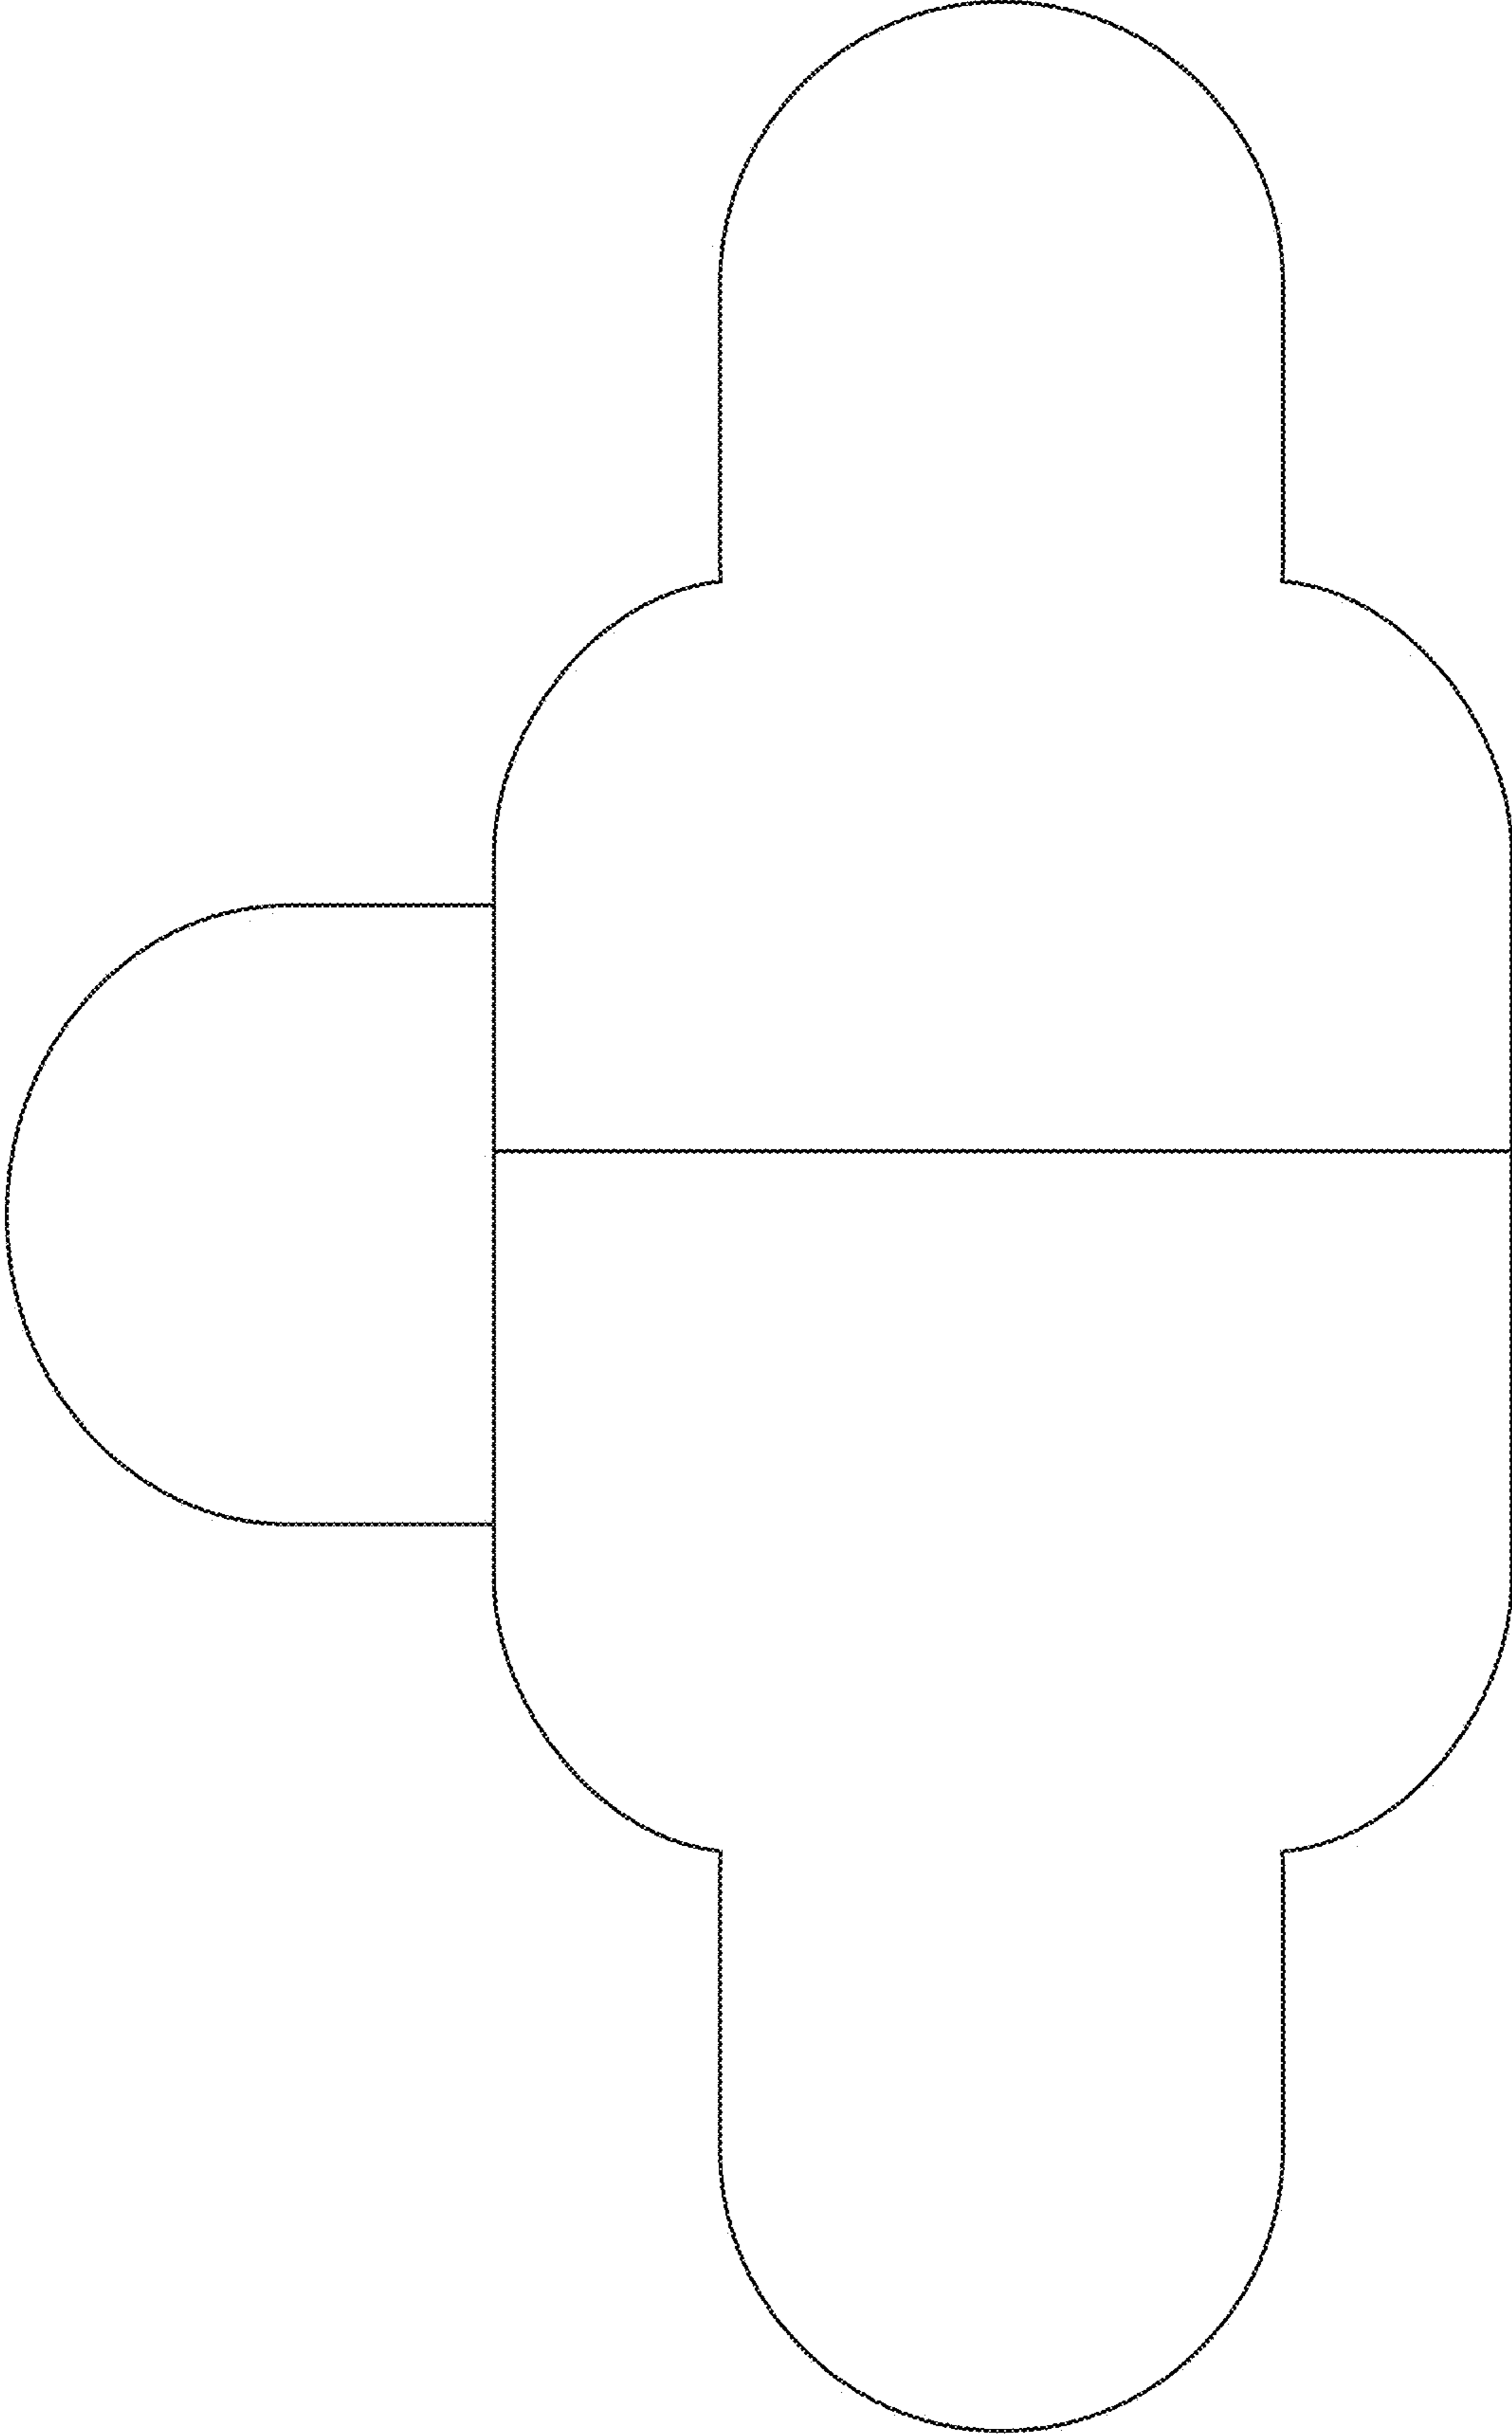


FIG. 7