



US00D940868S

(12) **United States Design Patent**
Achleitner et al.

(10) **Patent No.:** **US D940,868 S**
(45) **Date of Patent:** **** Jan. 11, 2022**

- (54) **ELECTROMEDICAL DEVICE**
- (71) Applicant: **Siemens Healthcare GmbH**, Erlangen (DE)
- (72) Inventors: **Roman Achleitner**, Nuremberg (DE); **Stefanie Guegel-Wild**, Langensendelbach (DE); **Tobias Kotulla**, Spardorf (DE)
- (73) Assignee: **Siemens Healthcare GmbH**, Erlangen (DE)

D785,801 S *	5/2017	Grosshauser	D24/158
D842,994 S *	3/2019	Avranches	D24/158
D843,577 S *	3/2019	Zhi	D24/158
D843,578 S *	3/2019	Avranches	D24/158
D868,262 S *	11/2019	Achleitner	D24/158
2012/0140899 A1 *	6/2012	Bailey	A61B 6/035 378/198
2020/0175733 A1 *	6/2020	Yu	A61B 6/485

- (**) Term: **15 Years**
- (21) Appl. No.: **29/712,176**
- (22) Filed: **Nov. 6, 2019**

- (30) **Foreign Application Priority Data**
May 6, 2019 (EM) 006427159
- (51) **LOC (13) Cl.** **24-01**
- (52) **U.S. Cl.**
USPC **D24/158**
- (58) **Field of Classification Search**
USPC D24/158-161, 185, 186, 107
CPC .. A61B 5/05; A61B 5/055; A61B 6/03; A61B 6/035
See application file for complete search history.

- (56) **References Cited**
U.S. PATENT DOCUMENTS
D420,134 S * 2/2000 Kitayama D24/159
D683,023 S * 5/2013 Andersson D24/158
D701,313 S * 3/2014 Ohmukai D24/158
D716,948 S * 11/2014 Yokoyama D24/158
D785,181 S * 4/2017 Grosshauser D24/158
D785,182 S * 4/2017 Grosshauser D24/158

OTHER PUBLICATIONS

Computed Tomography, posted at siemens-healthineers.com, no posting date, retrieved Nov. 7, 2020, online, URL: <https://www.siemens-healthineers.com/en-US/computed-tomography> (Year: 2020).*

* cited by examiner

Primary Examiner — Lilyana Bekic
Assistant Examiner — Mary Shannon Malley
(74) *Attorney, Agent, or Firm* — Schiff Hardin LLP


(57) **CLAIM**

The ornamental design for an electromedical device, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of an electromedical device showing our new design;
FIG. 2 is a back elevational view thereof;
FIG. 3 is a top plan view thereof;
FIG. 4 is a bottom plan view thereof;
FIG. 5 is a right side elevational view thereof;
FIG. 6 is a left side elevational view thereof; and,
FIG. 7 is a perspective view taken generally from the top, front, right-hand side thereof.
The broken lines shown in the drawings represent portions of the electromedical device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

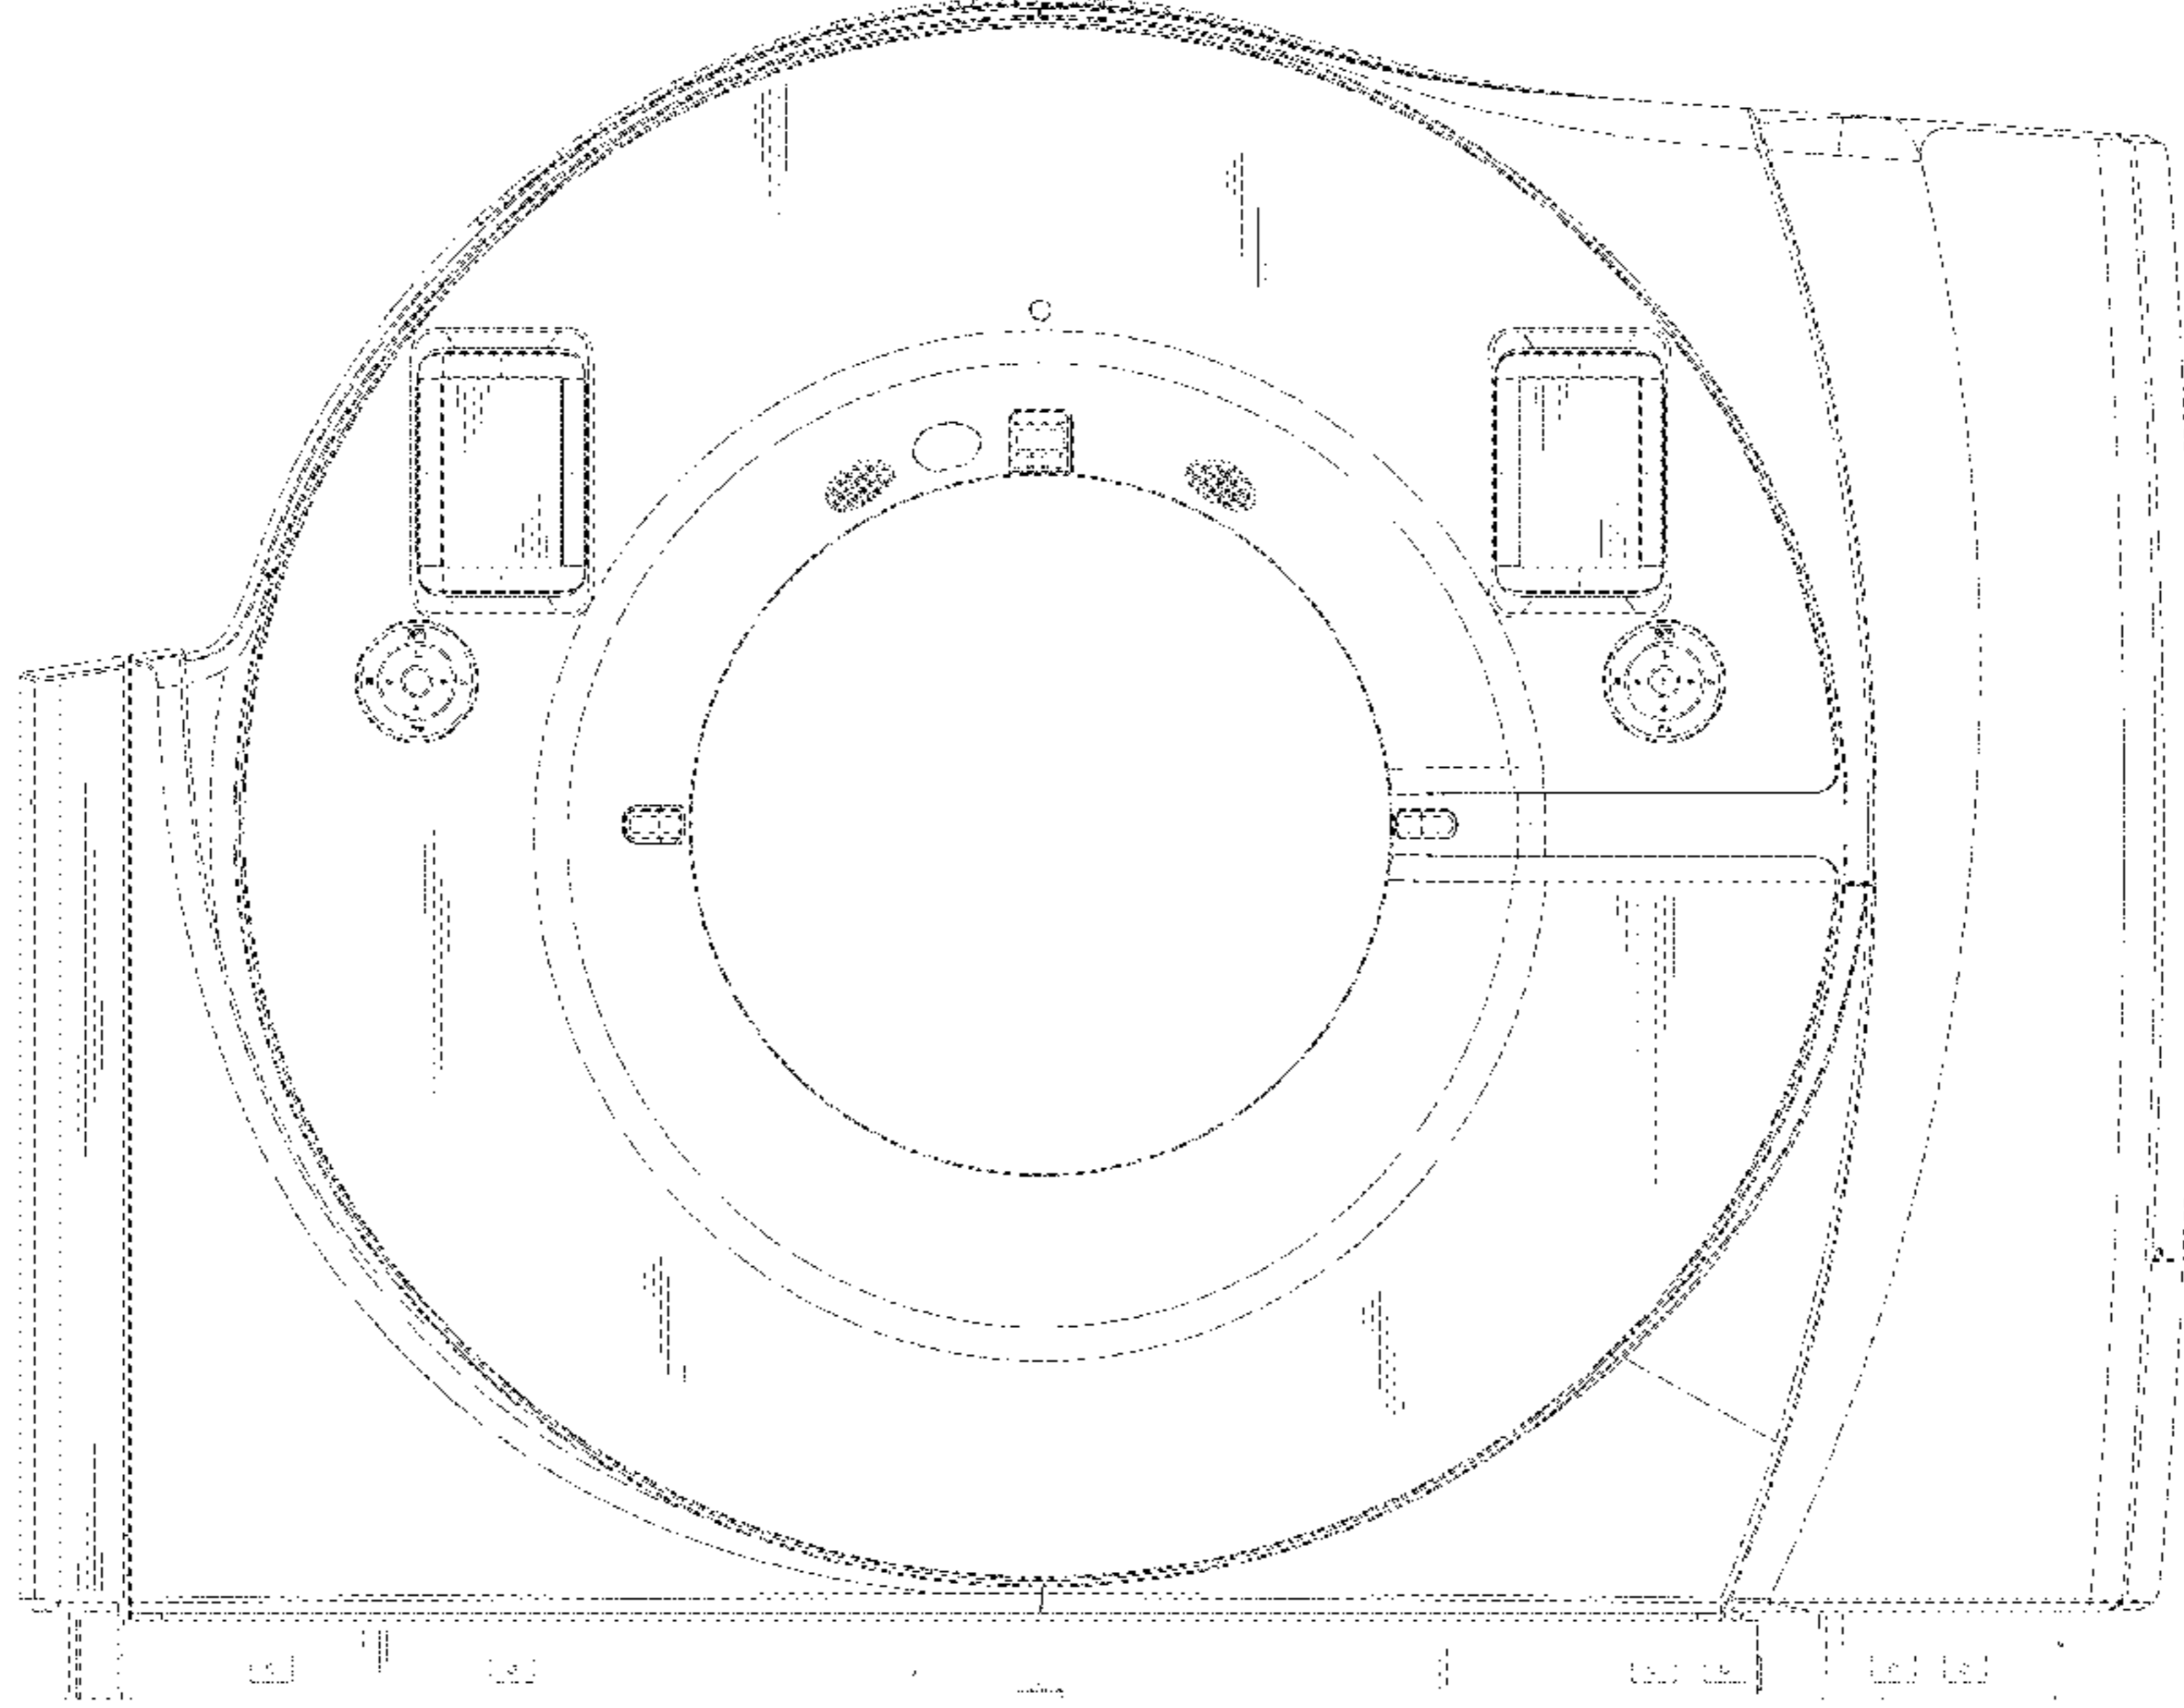

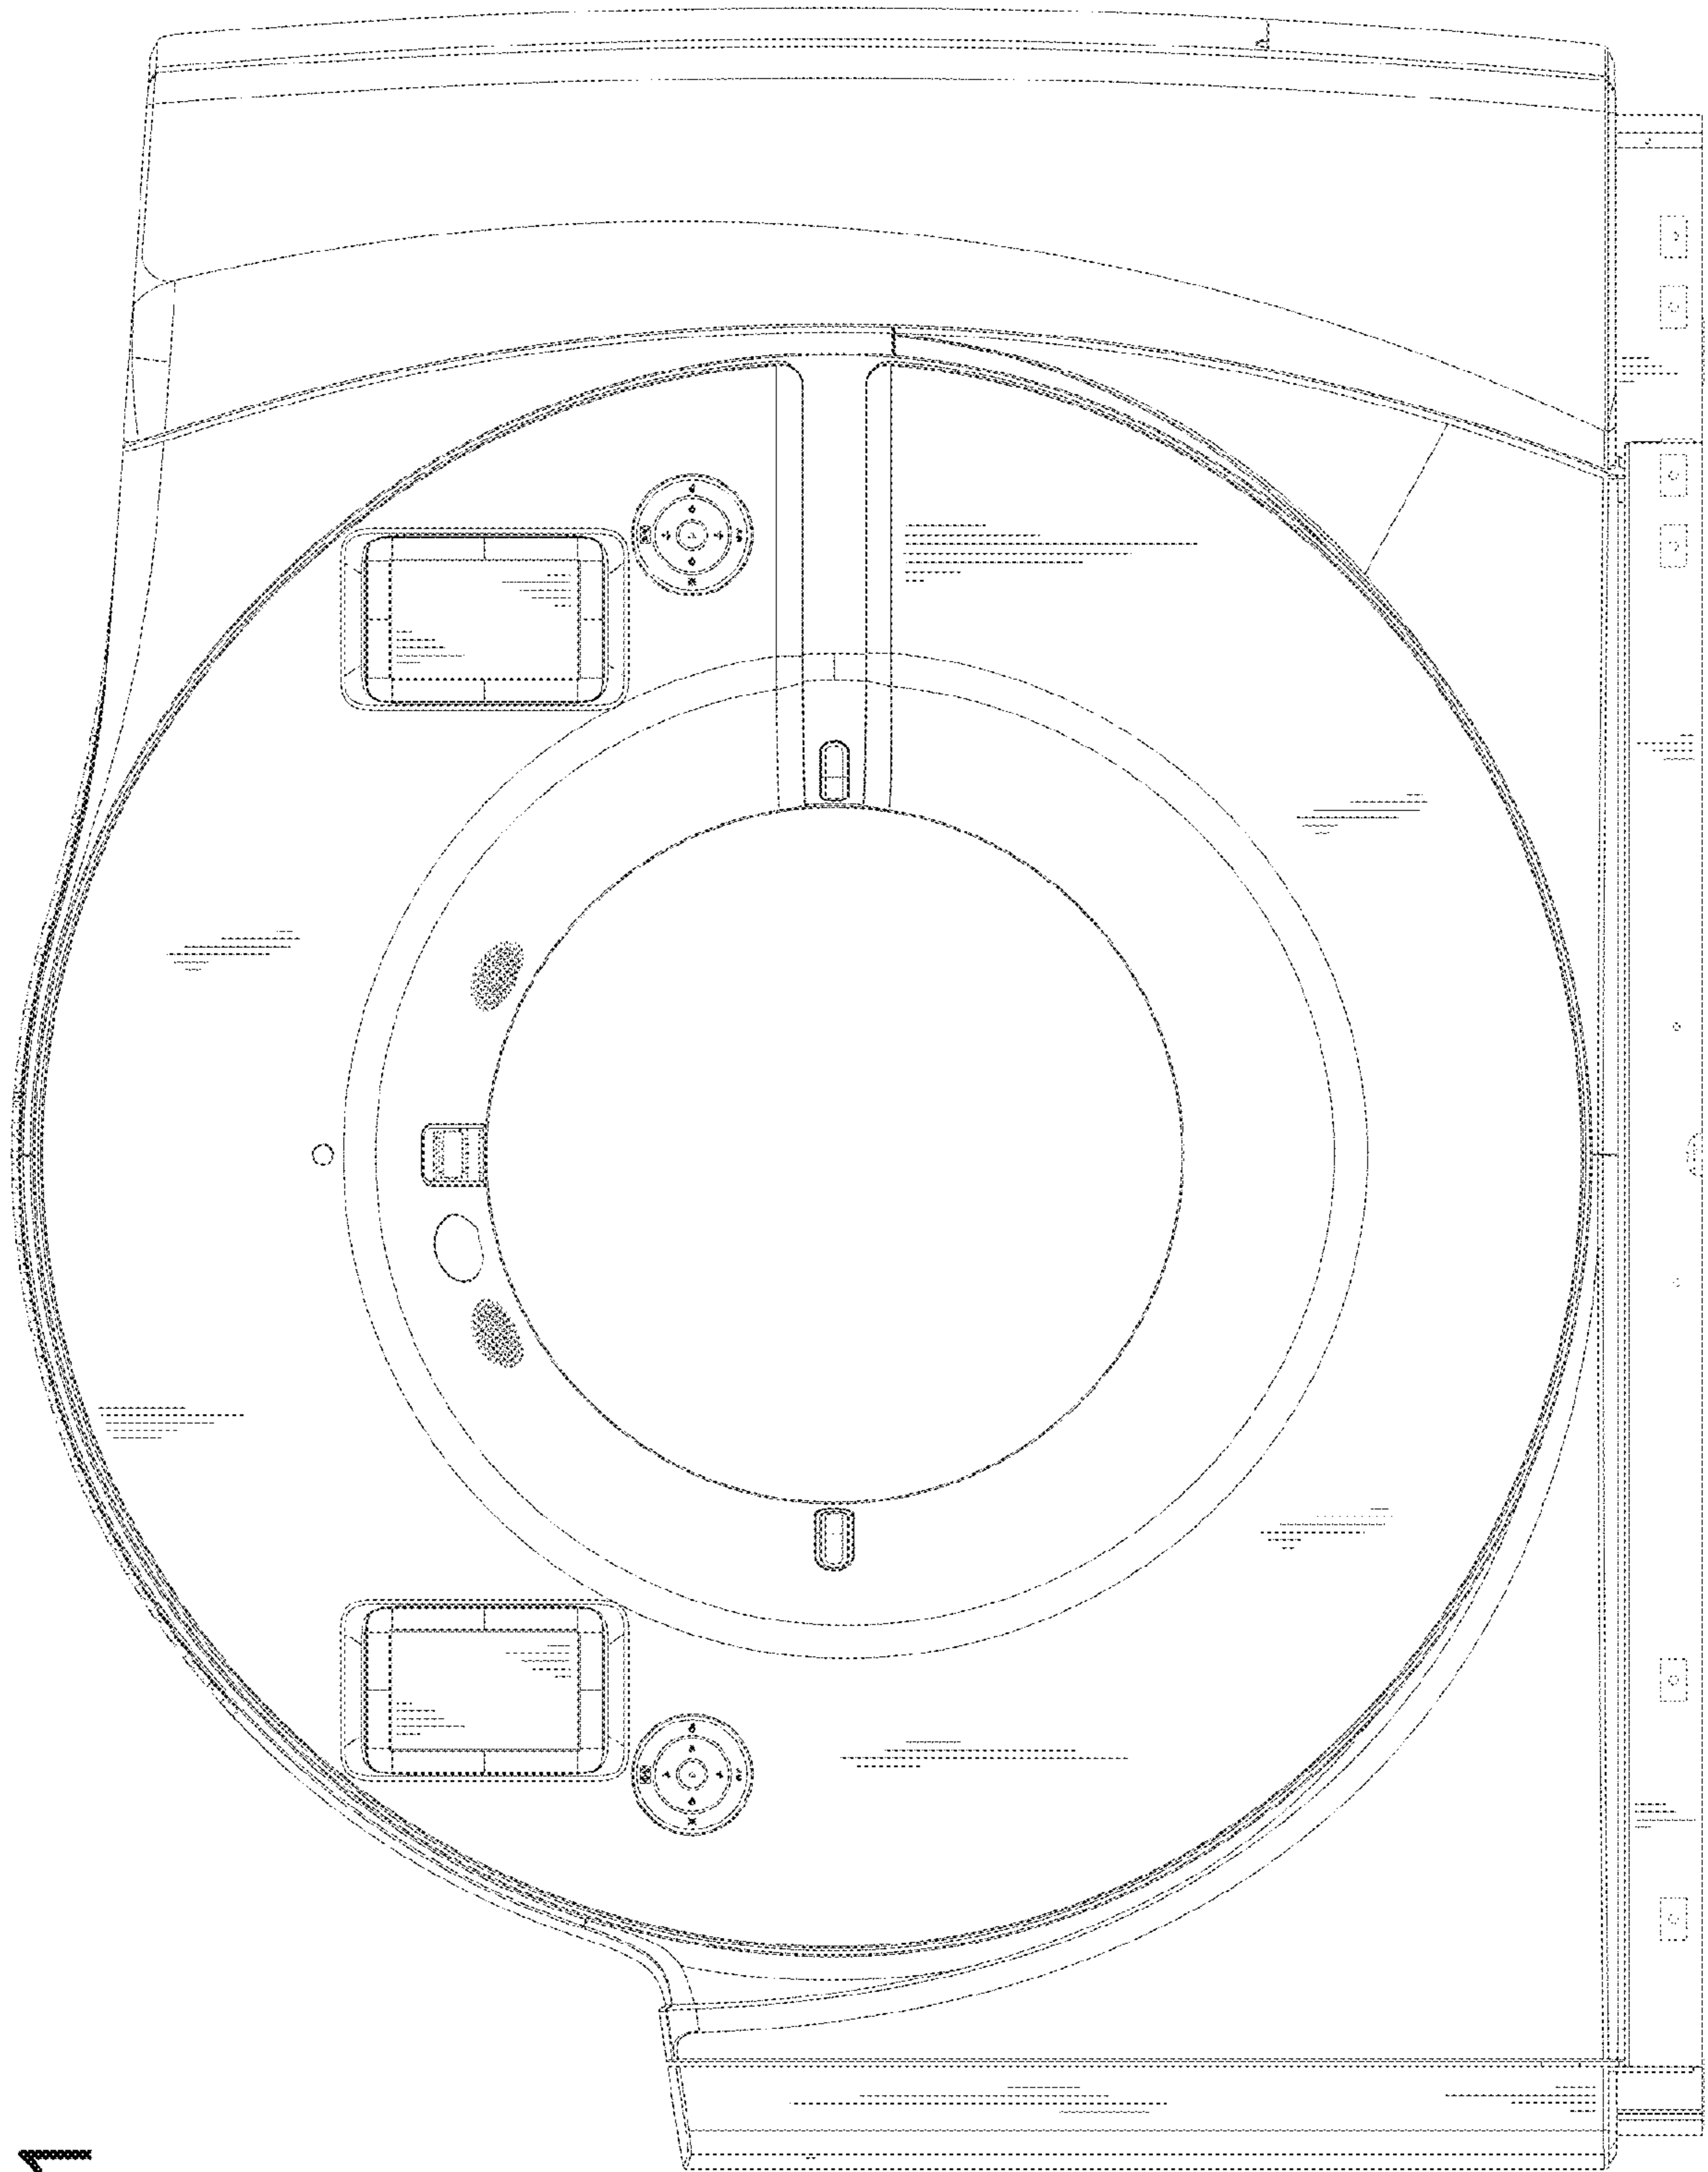
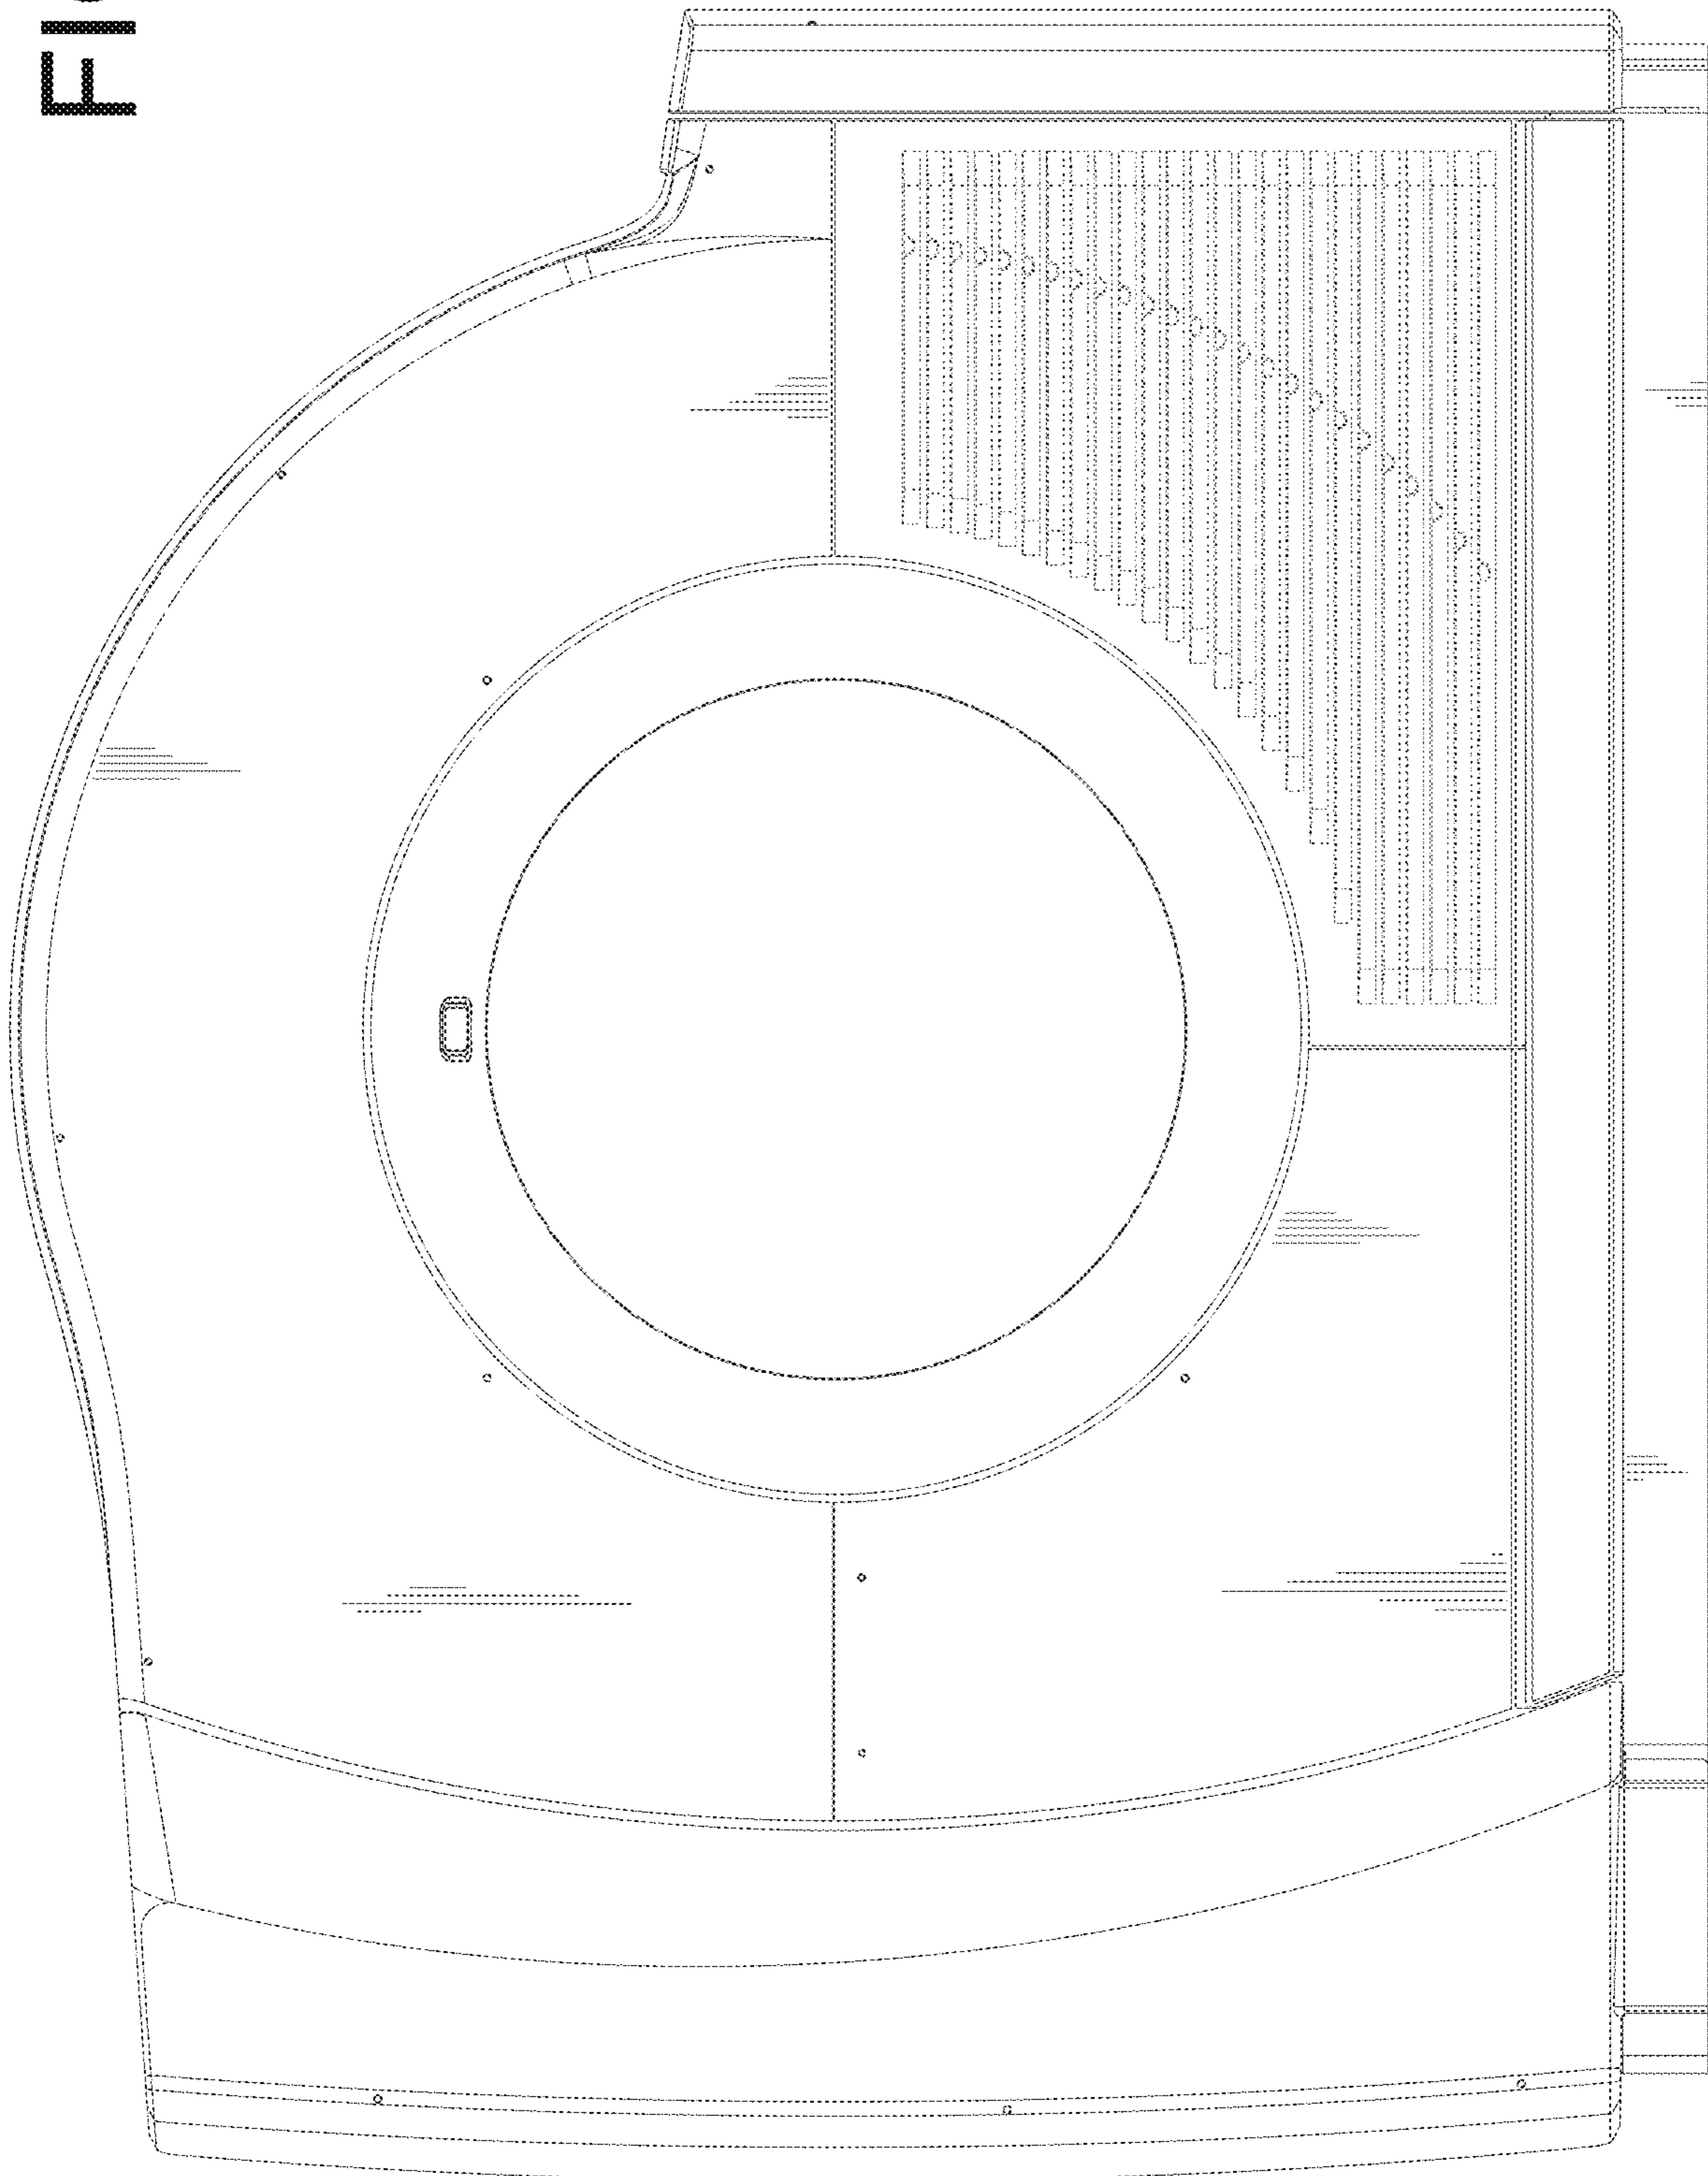


FIG. 1

FIG. 2



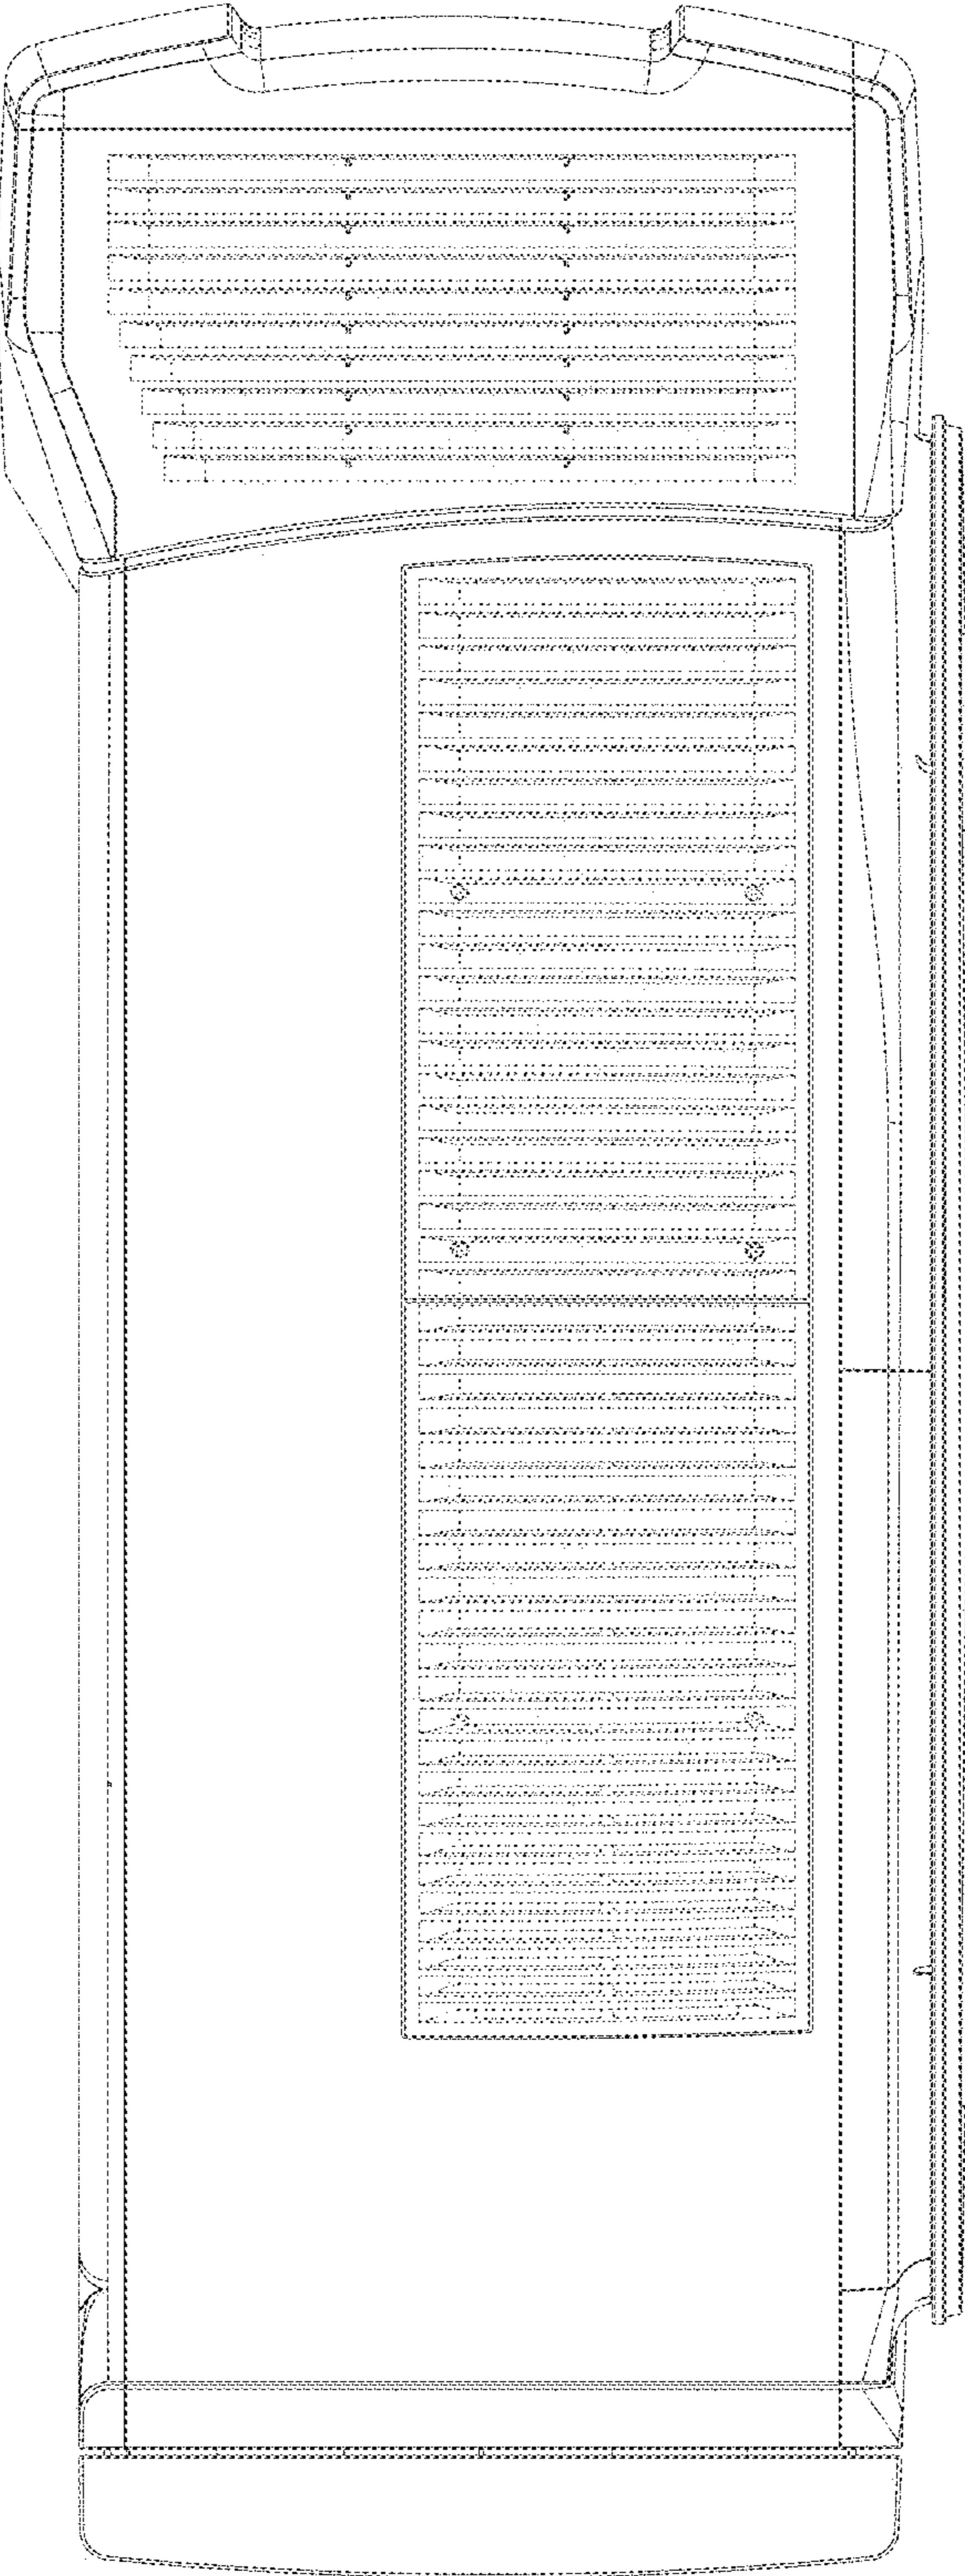


FIG. 3

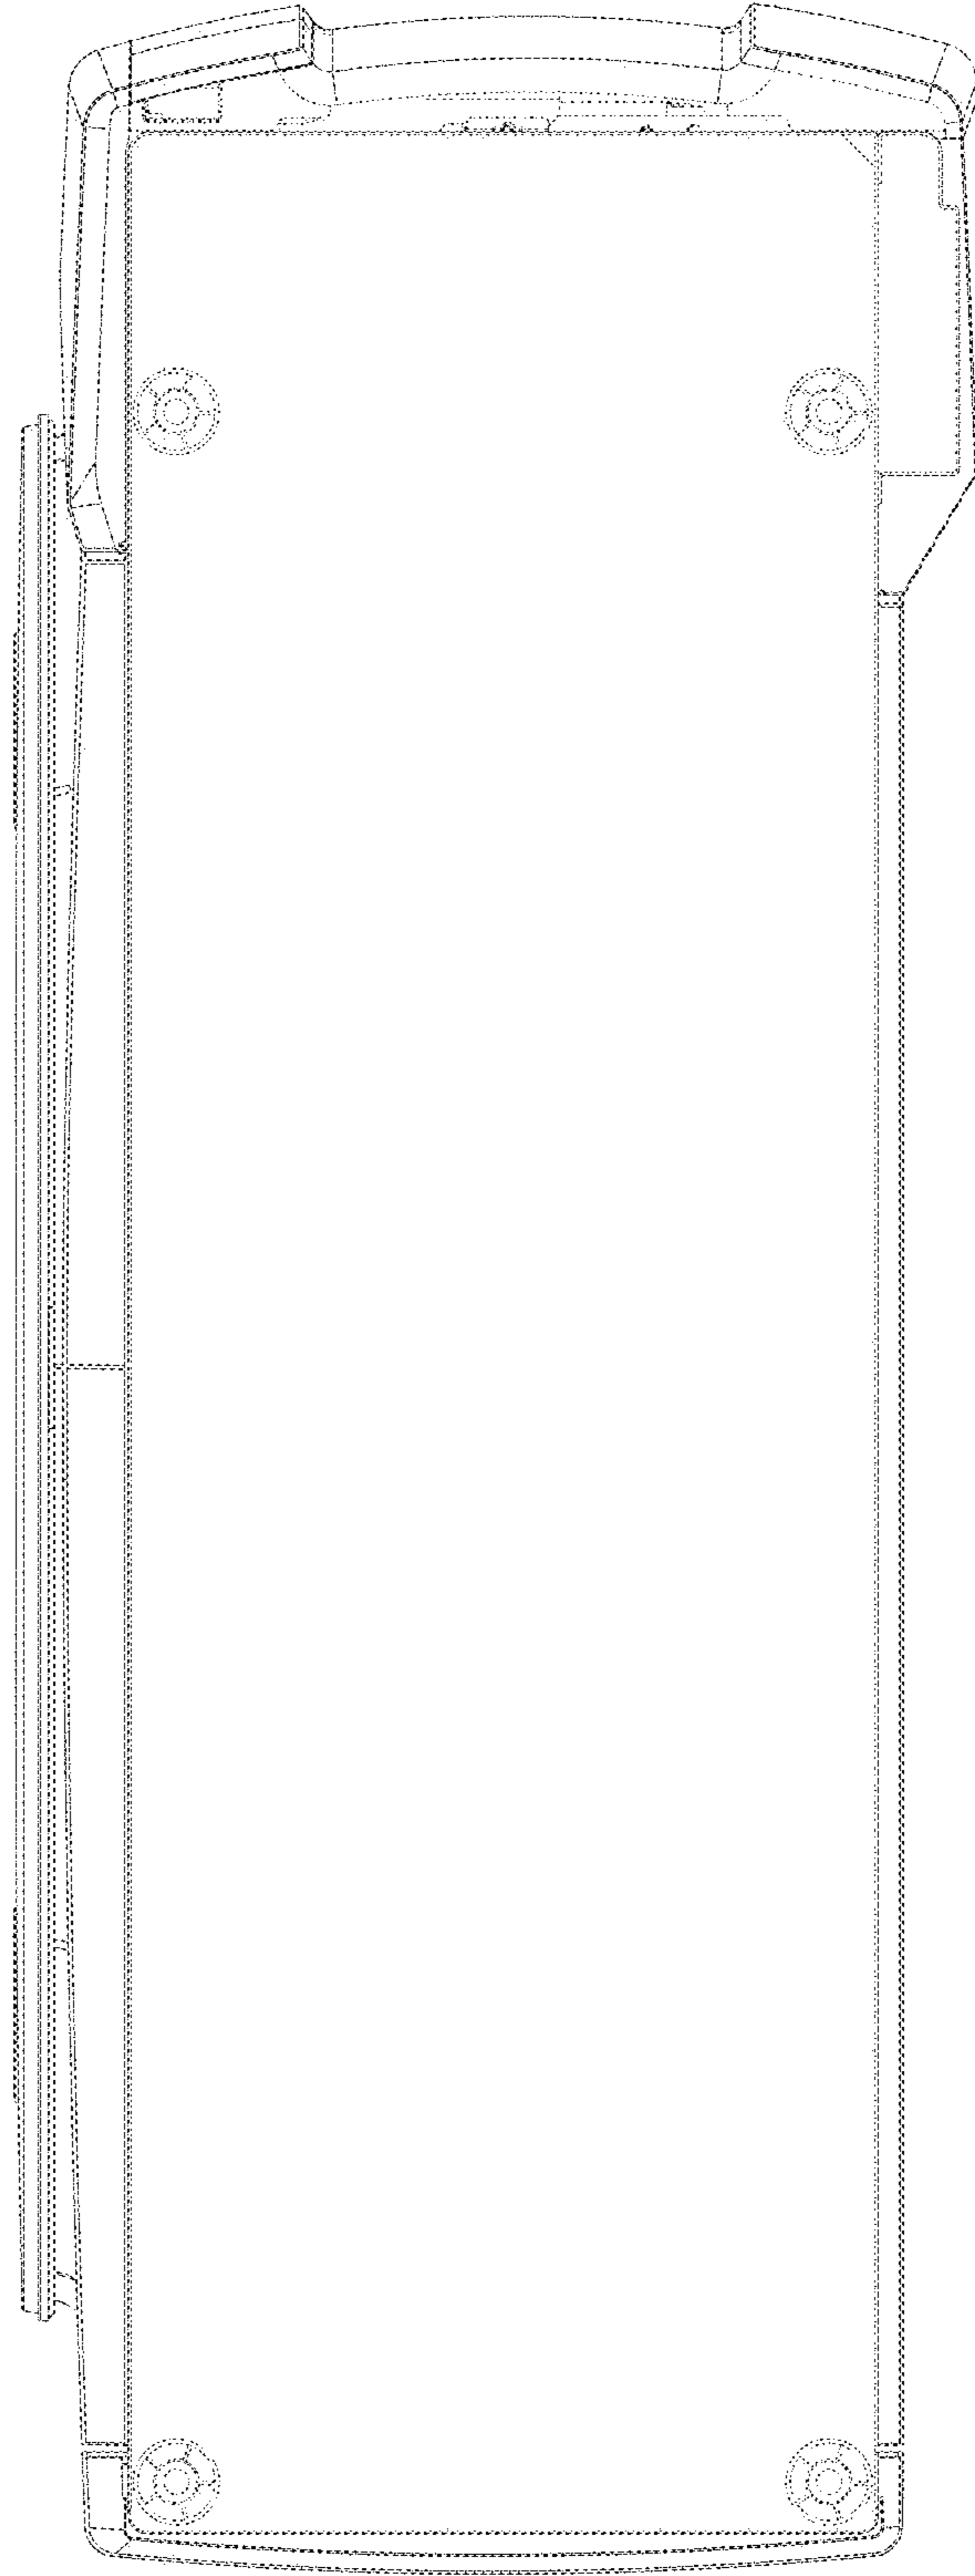


FIG. 4

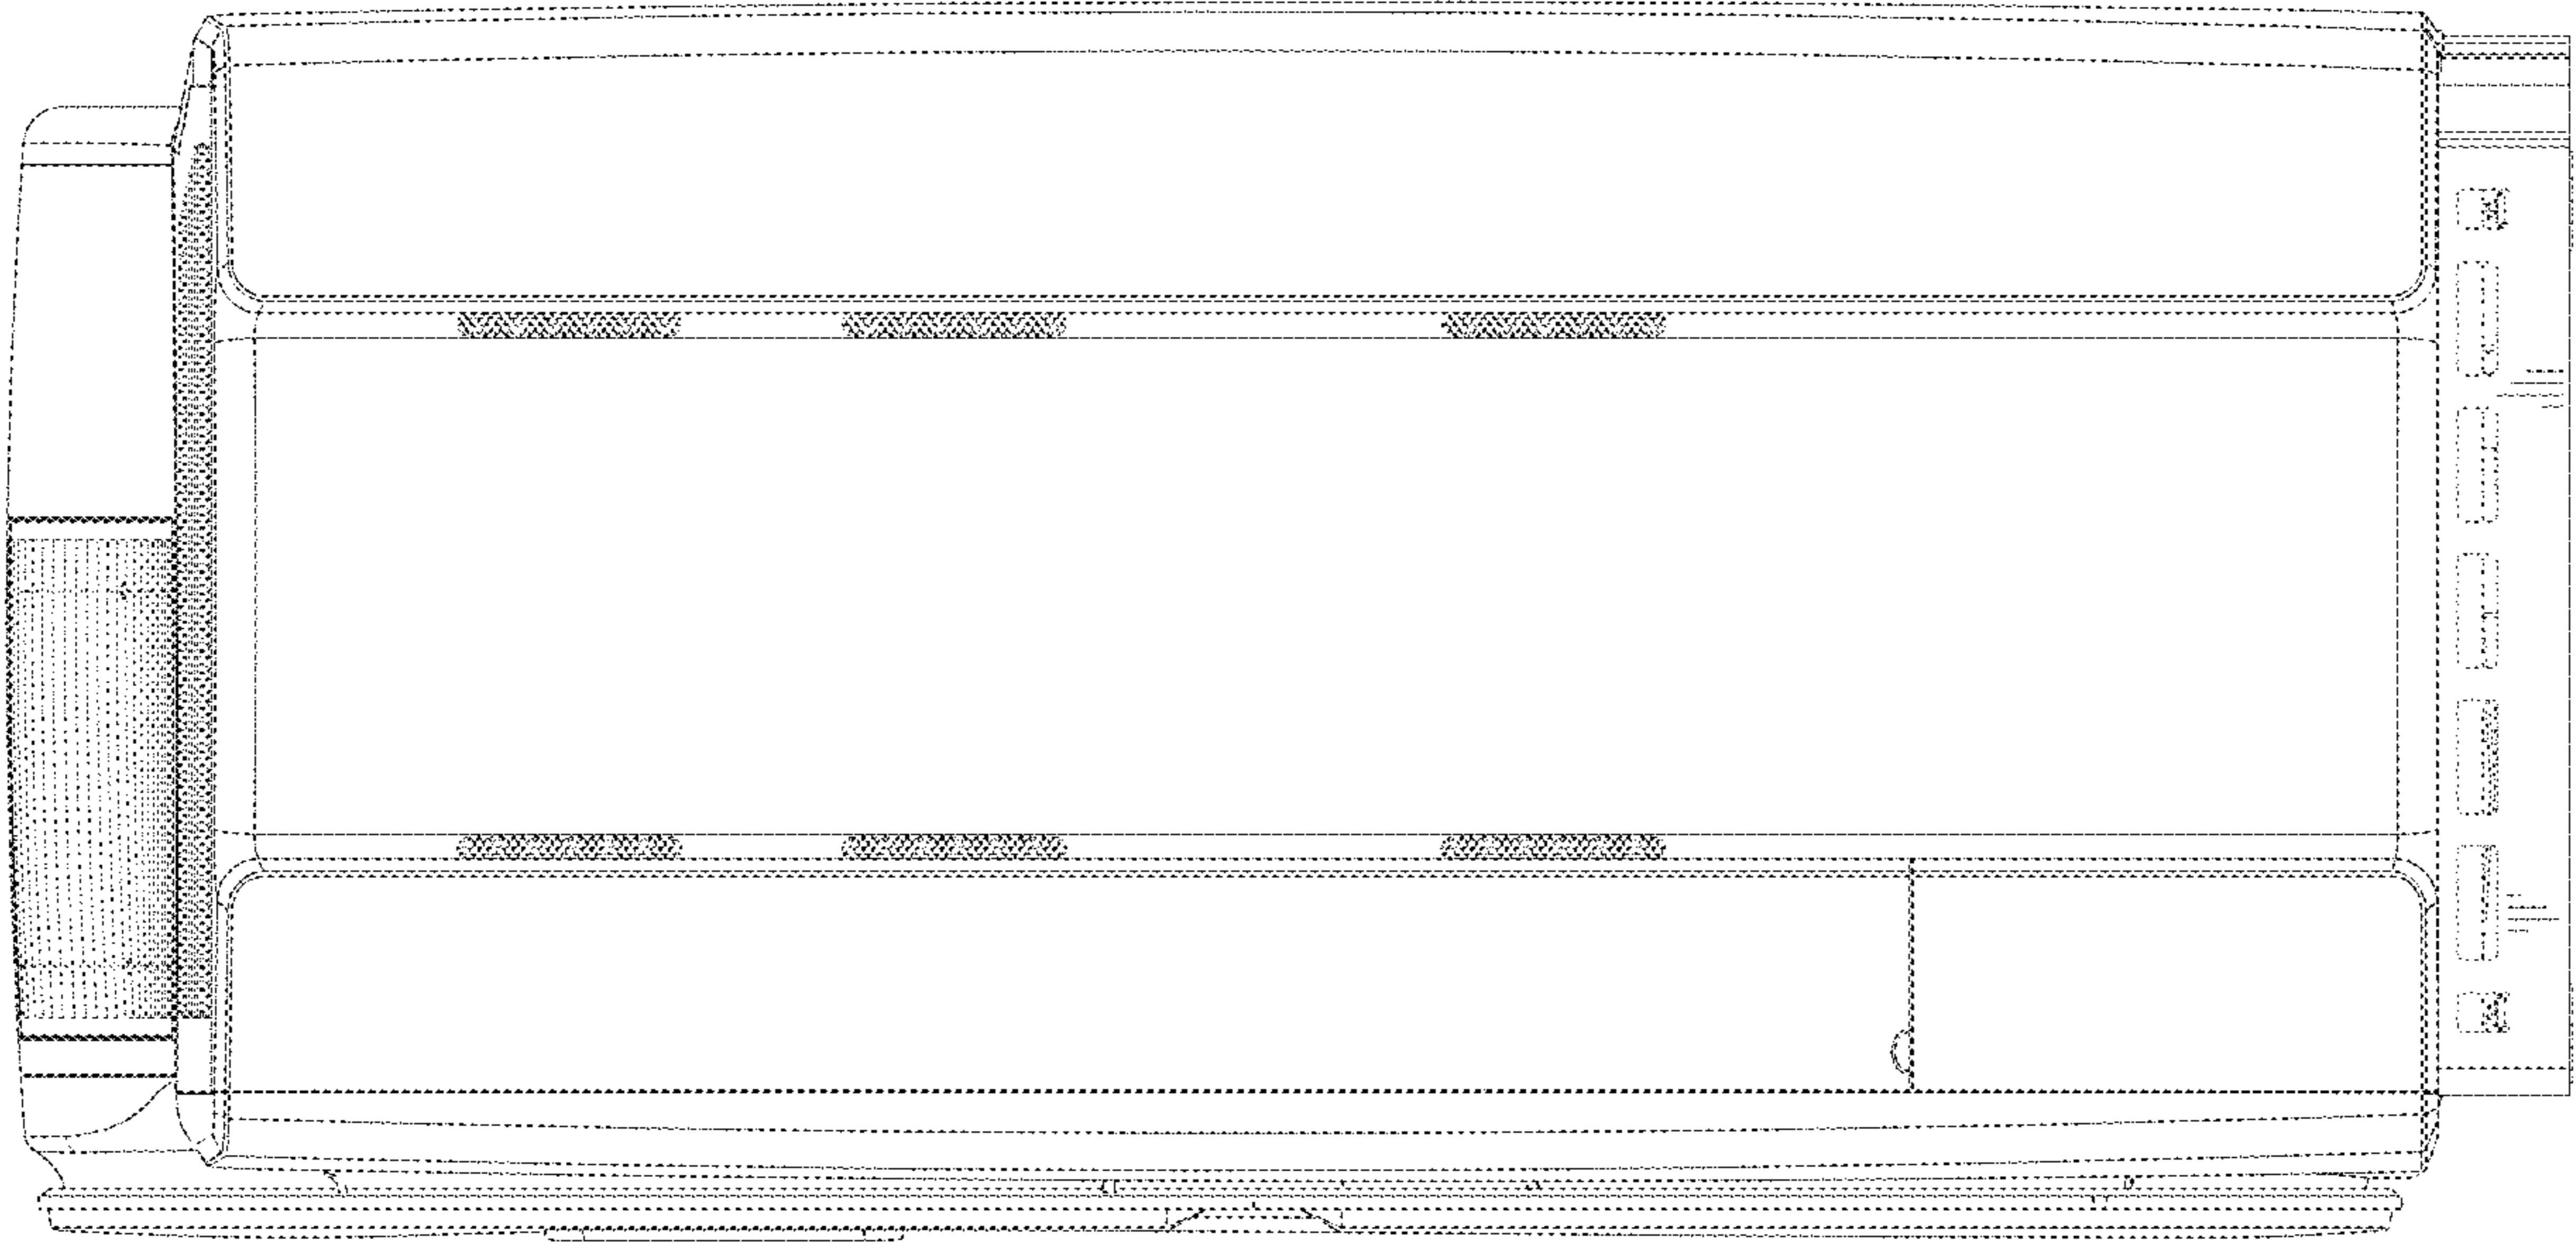


FIG. 5

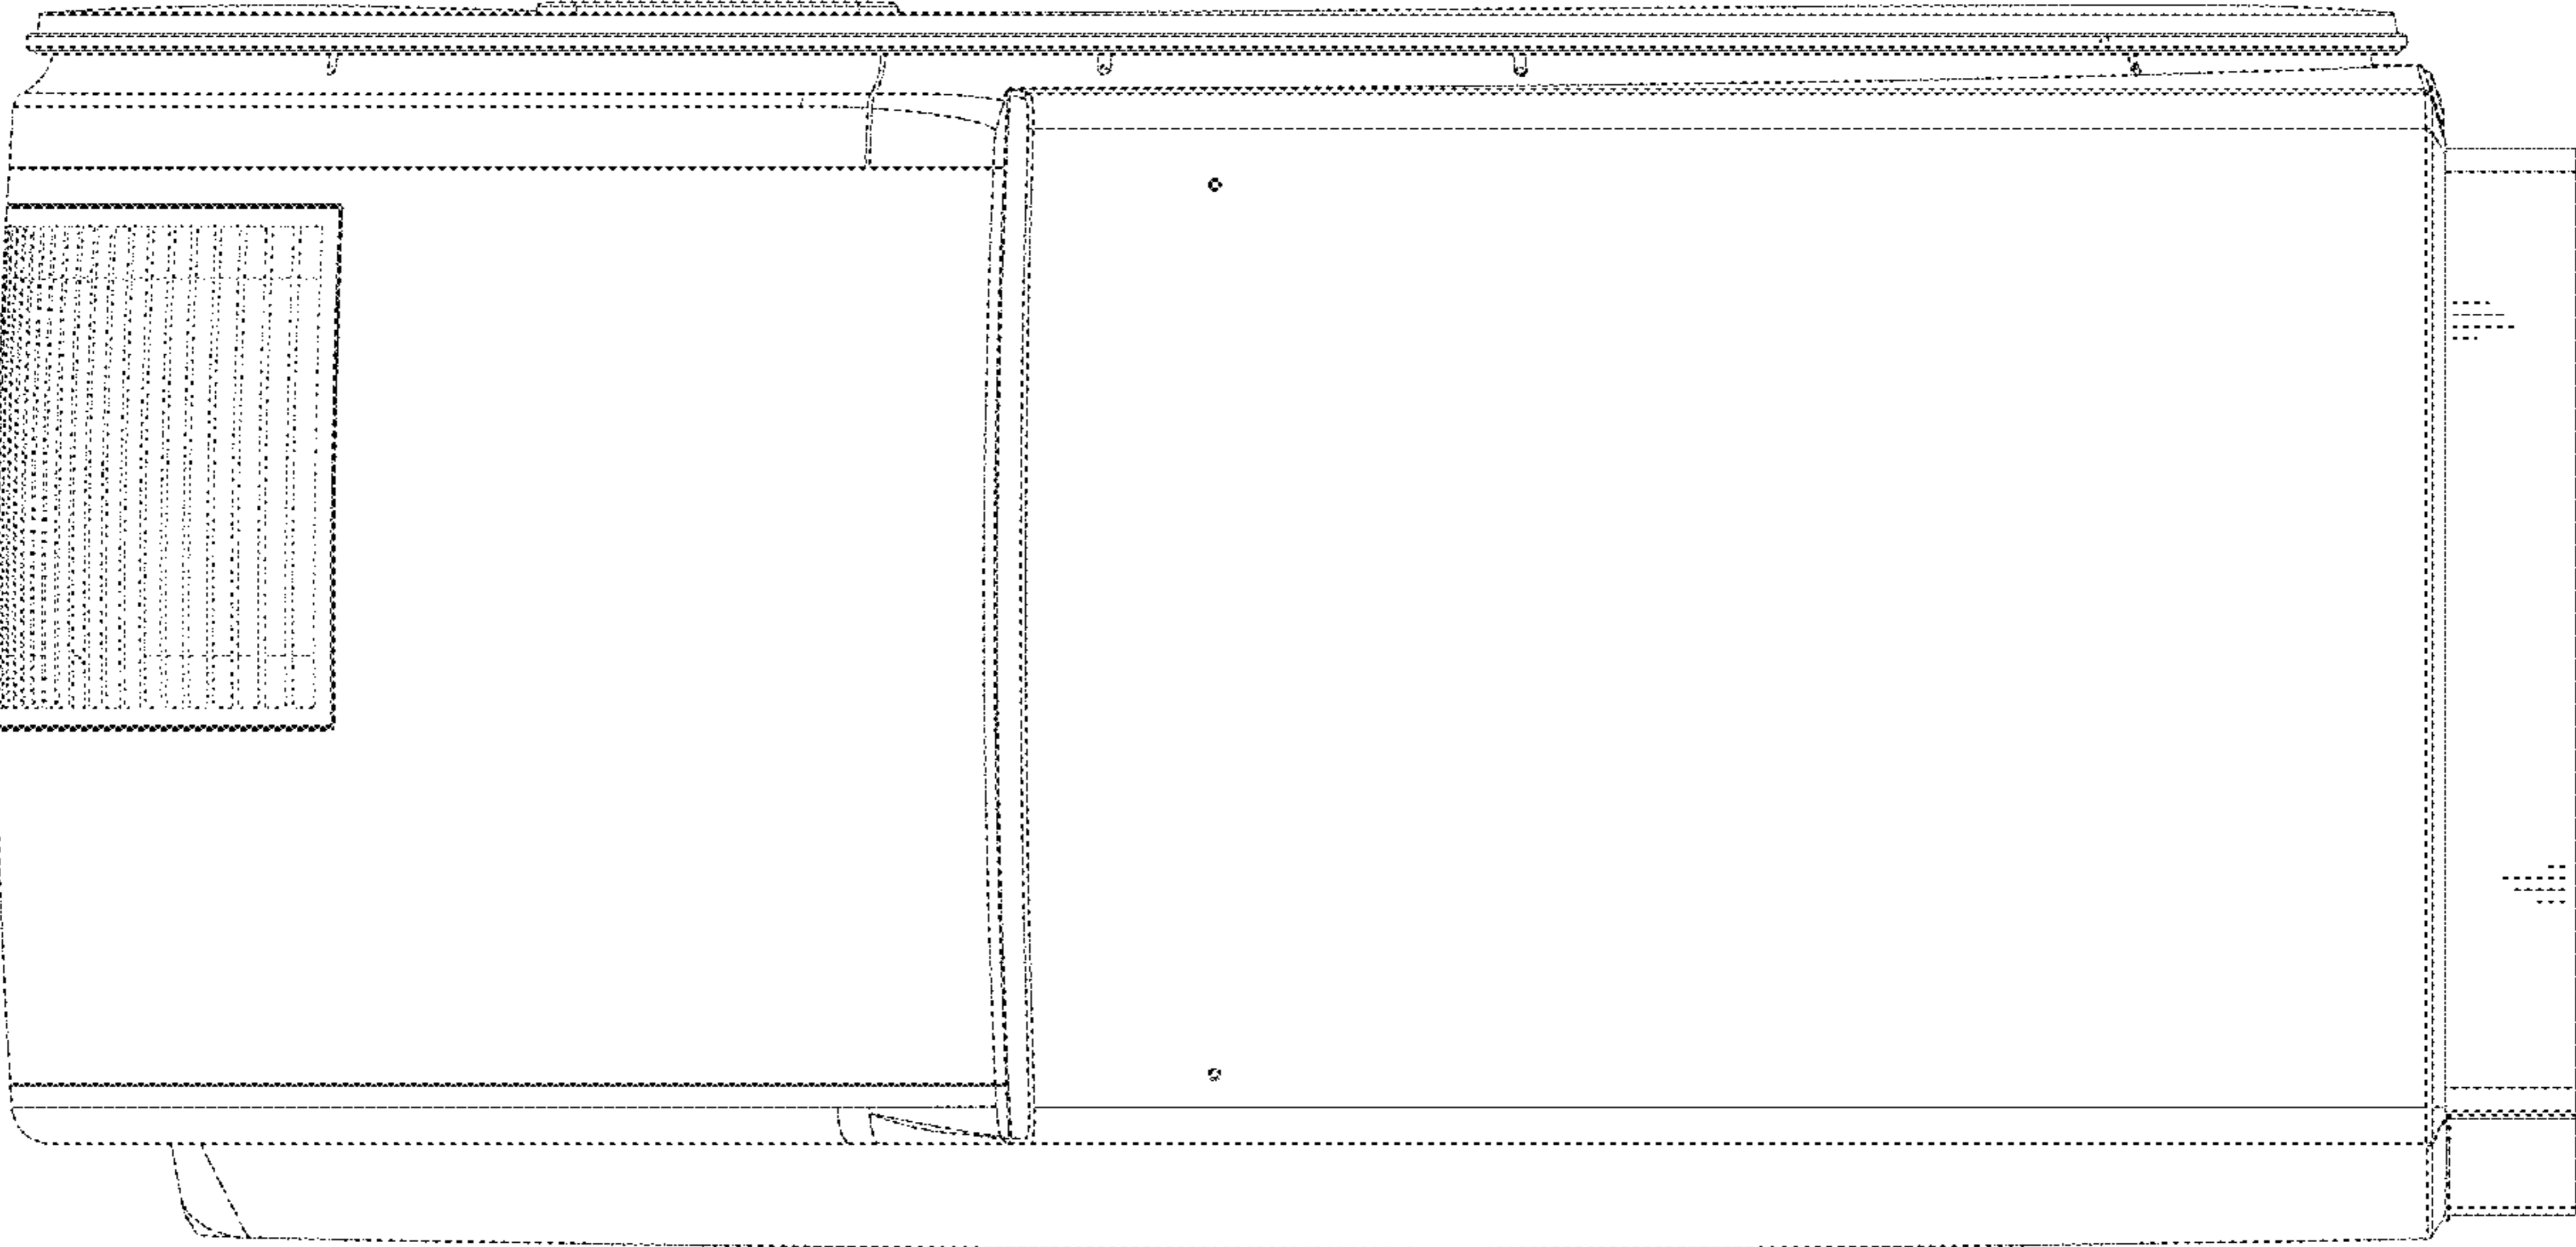


FIG. 6

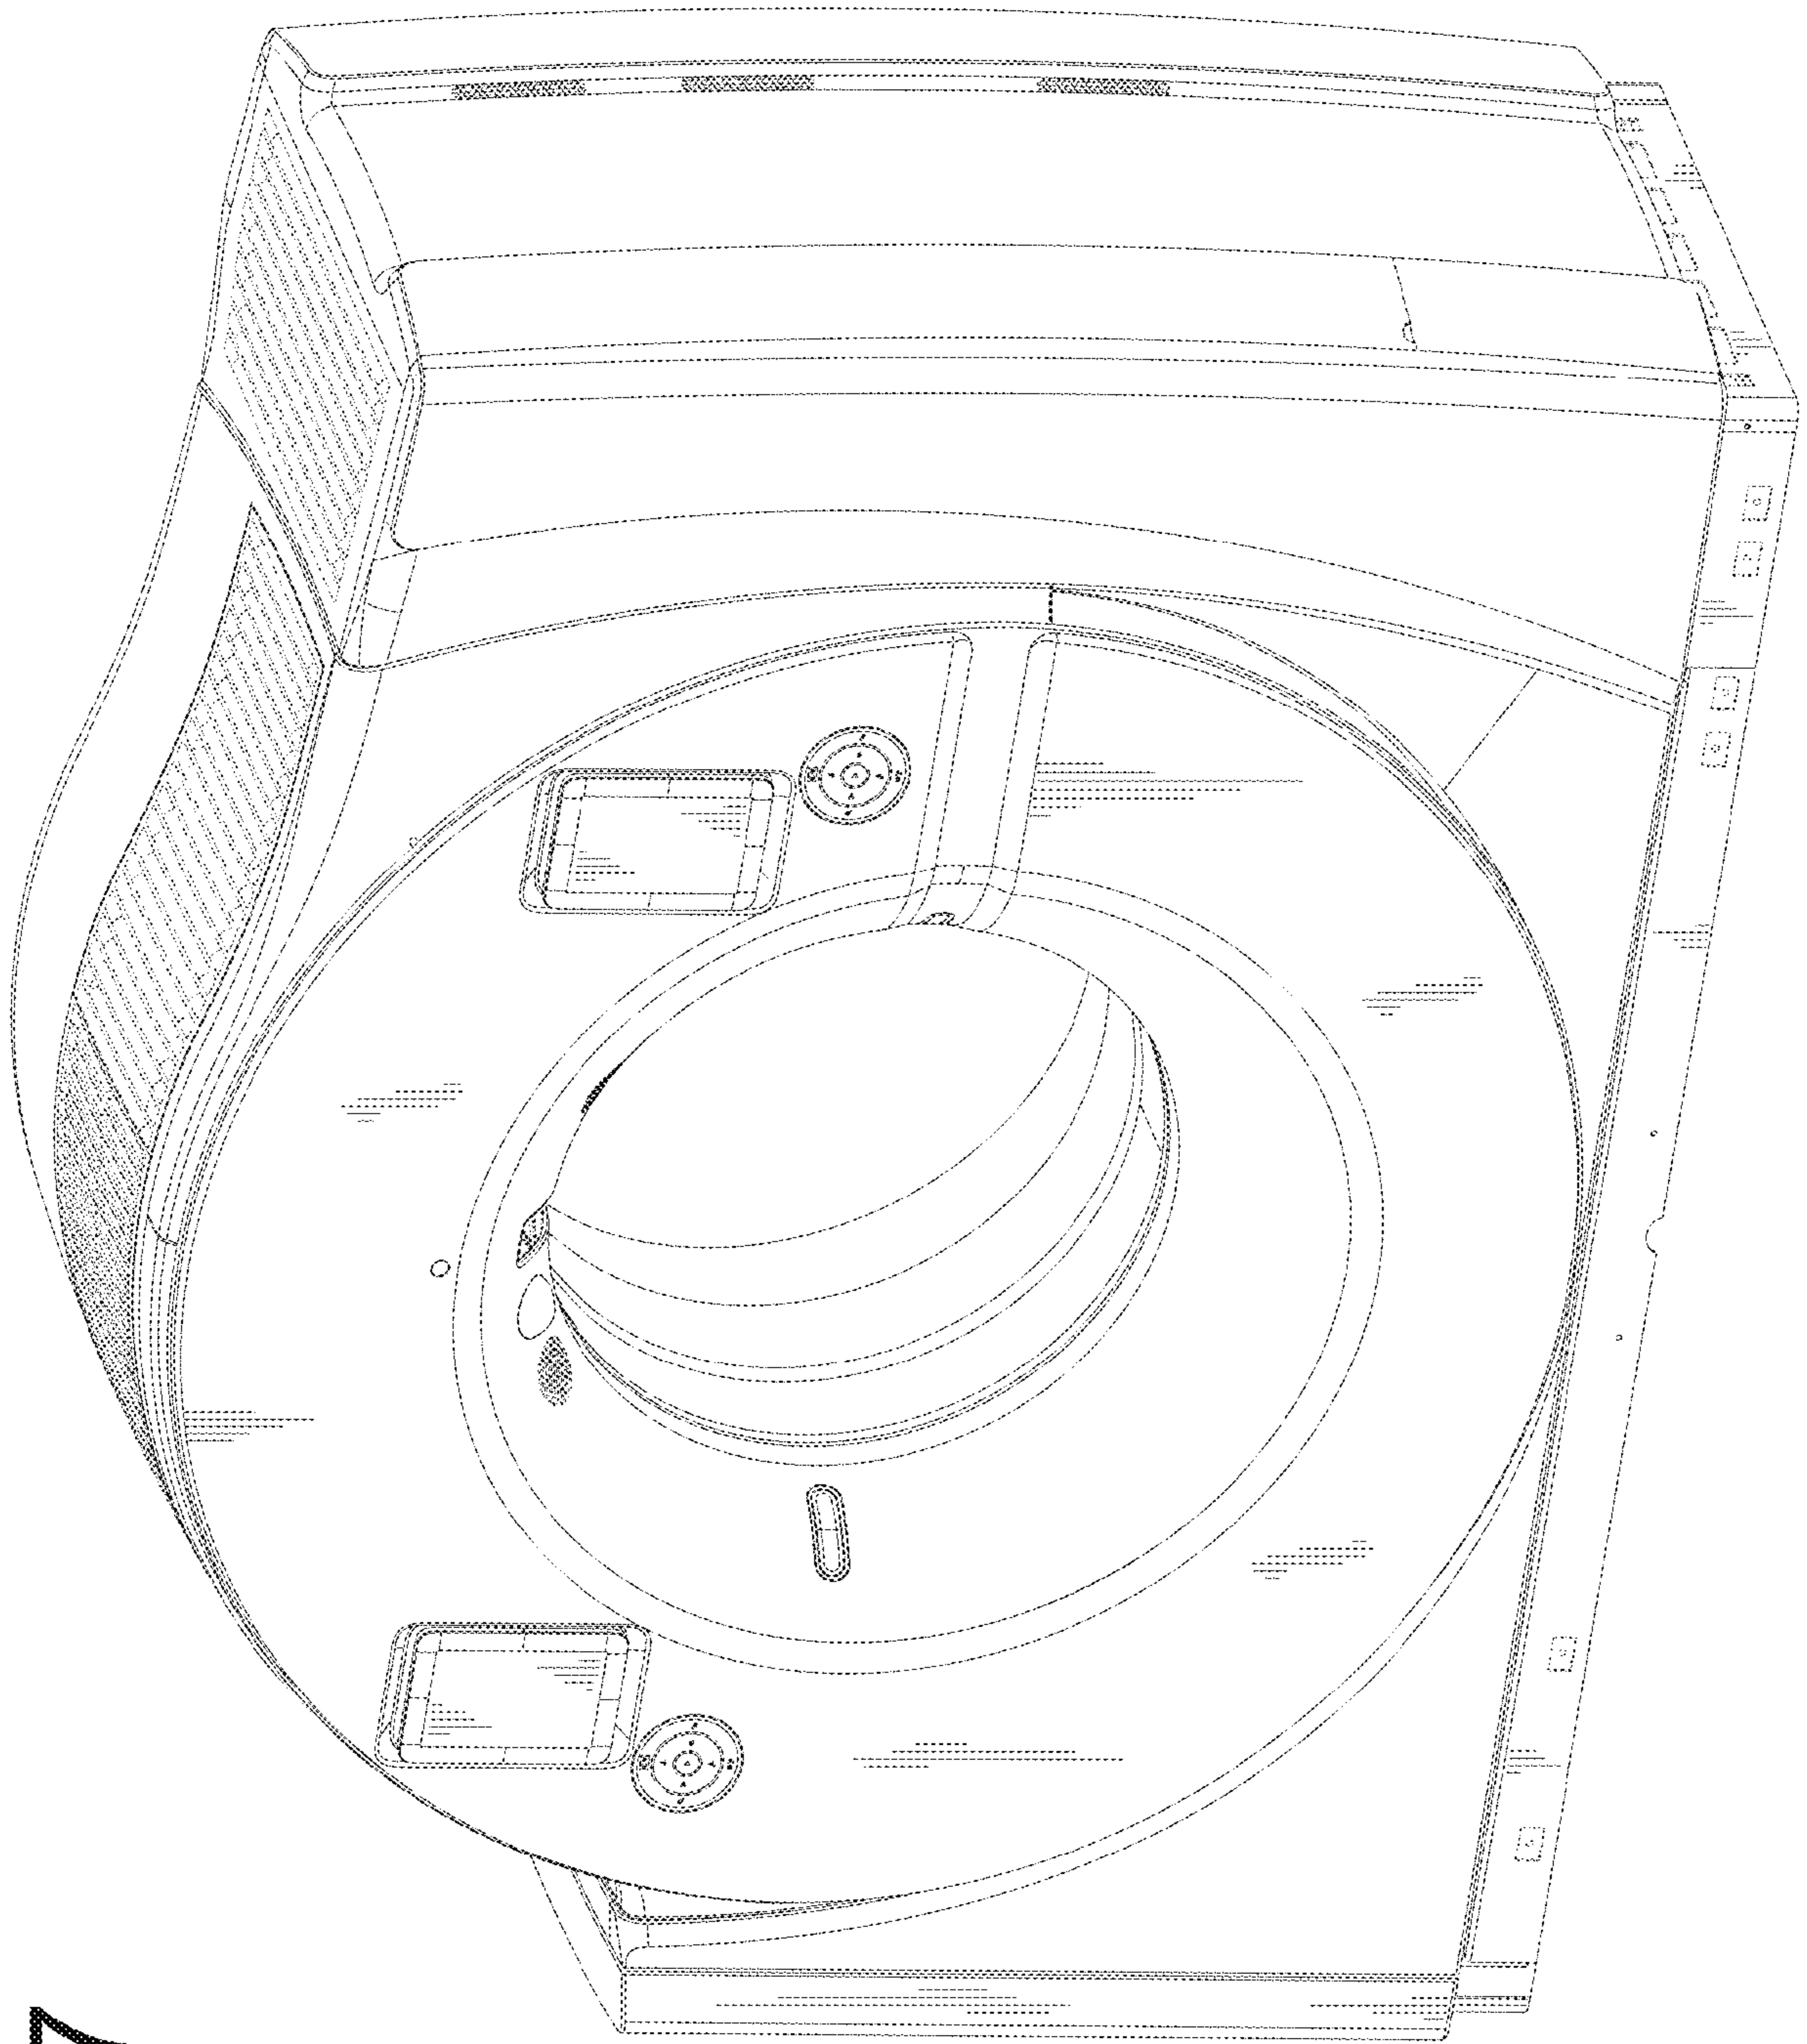


FIG. 7