



US00D940868S

(12) **United States Design Patent**  
**Achleitner et al.**

(10) **Patent No.:** **US D940,868 S**  
(45) **Date of Patent:** **\*\* Jan. 11, 2022**

- (54) **ELECTROMEDICAL DEVICE**
- (71) Applicant: **Siemens Healthcare GmbH**, Erlangen (DE)
- (72) Inventors: **Roman Achleitner**, Nuremberg (DE); **Stefanie Guegel-Wild**, Langensendelbach (DE); **Tobias Kotulla**, Spardorf (DE)
- (73) Assignee: **Siemens Healthcare GmbH**, Erlangen (DE)

D785,801 S *	5/2017	Grosshauser	.....	D24/158
D842,994 S *	3/2019	Avranches	.....	D24/158
D843,577 S *	3/2019	Zhi	.....	D24/158
D843,578 S *	3/2019	Avranches	.....	D24/158
D868,262 S *	11/2019	Achleitner	.....	D24/158
2012/0140899 A1 *	6/2012	Bailey	.....	A61B 6/035 378/198
2020/0175733 A1 *	6/2020	Yu	.....	A61B 6/485

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/712,176**

(22) Filed: **Nov. 6, 2019**

(30) **Foreign Application Priority Data**

May 6, 2019 (EM) ..... 006427159

(51) **LOC (13) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/158**

(58) **Field of Classification Search**  
USPC ..... D24/158-161, 185, 186, 107  
CPC .. A61B 5/05; A61B 5/055; A61B 6/03; A61B  
6/035  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D420,134 S *	2/2000	Kitayama	.....	D24/159
D683,023 S *	5/2013	Andersson	.....	D24/158
D701,313 S *	3/2014	Ohmukai	.....	D24/158
D716,948 S *	11/2014	Yokoyama	.....	D24/158
D785,181 S *	4/2017	Grosshauser	.....	D24/158
D785,182 S *	4/2017	Grosshauser	.....	D24/158

**OTHER PUBLICATIONS**

Computed Tomography, posted at siemens-healthineers.com, no posting date, retrieved Nov. 7, 2020, online, URL: <https://www.siemens-healthineers.com/en-US/computed-tomography> (Year: 2020).\*

\* cited by examiner

*Primary Examiner* — Lilyana Bekic  
*Assistant Examiner* — Mary Shannon Malley  
(74) *Attorney, Agent, or Firm* — Schiff Hardin LLP

(57) **CLAIM**


The ornamental design for an electromedical device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front elevational view of an electromedical device showing our new design;  
FIG. 2 is a back elevational view thereof;  
FIG. 3 is a top plan view thereof;  
FIG. 4 is a bottom plan view thereof;  
FIG. 5 is a right side elevational view thereof;  
FIG. 6 is a left side elevational view thereof; and,  
FIG. 7 is a perspective view taken generally from the top, front, right-hand side thereof.

The broken lines shown in the drawings represent portions of the electromedical device that form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

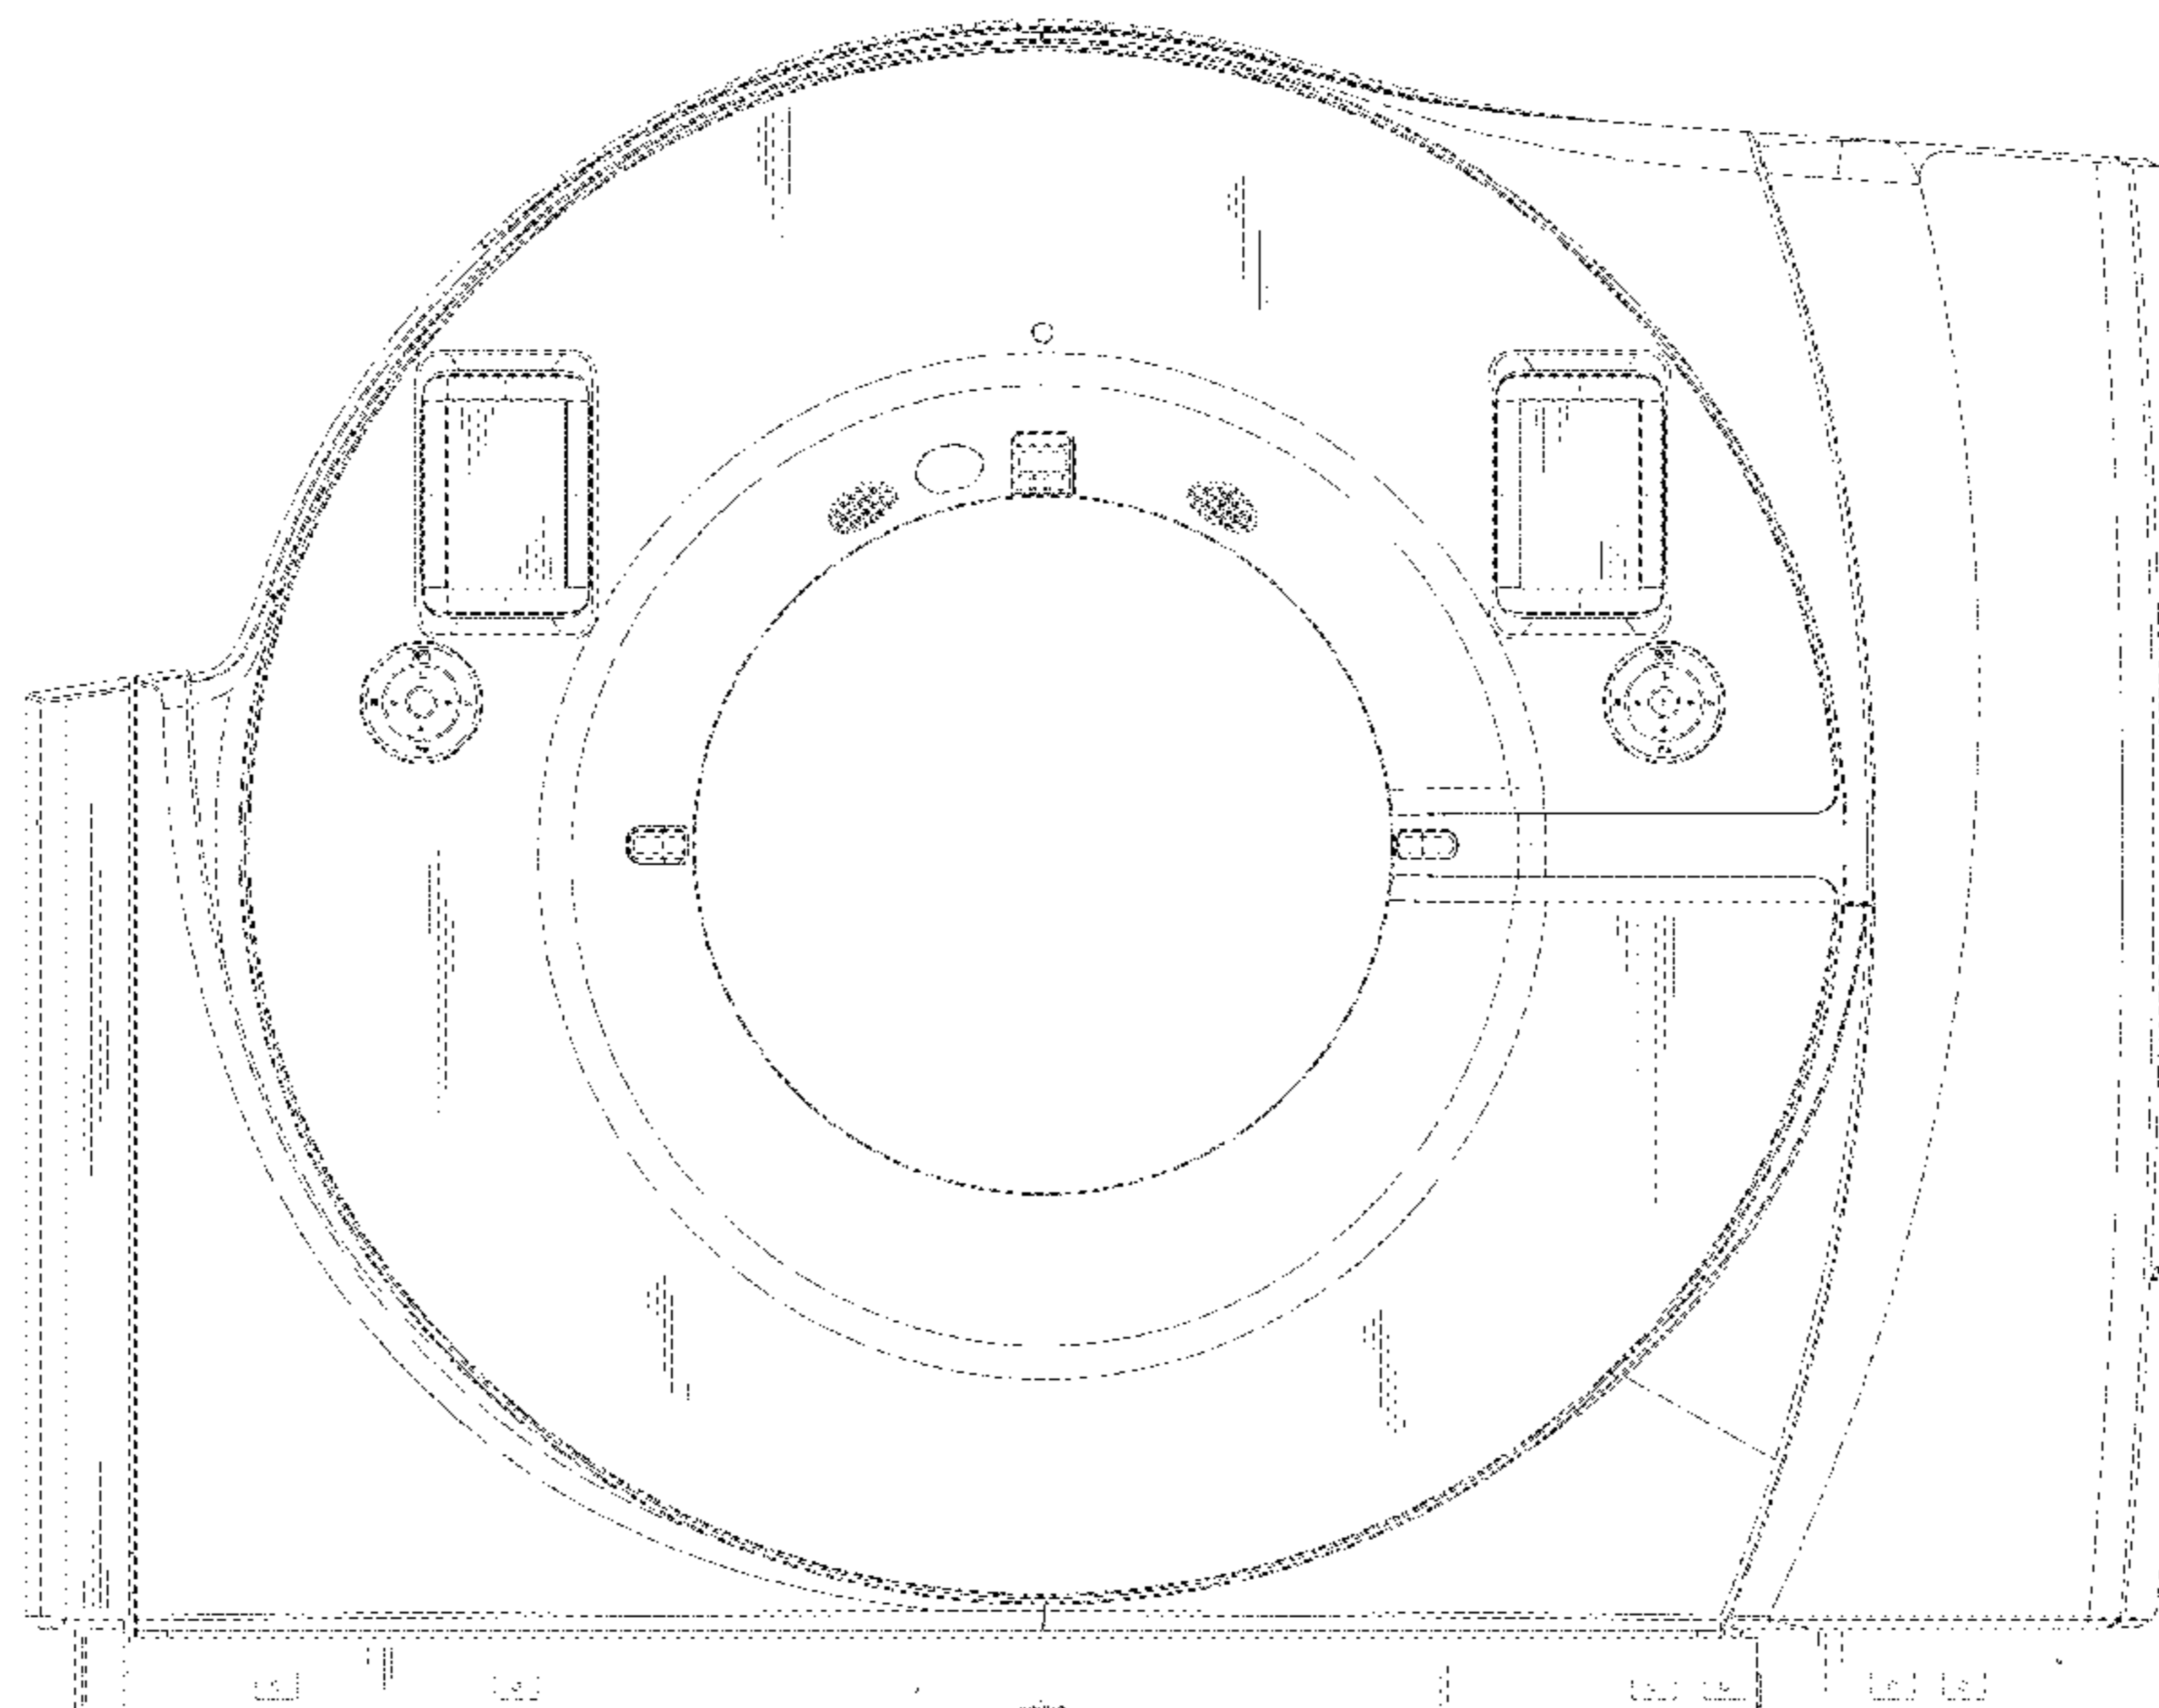

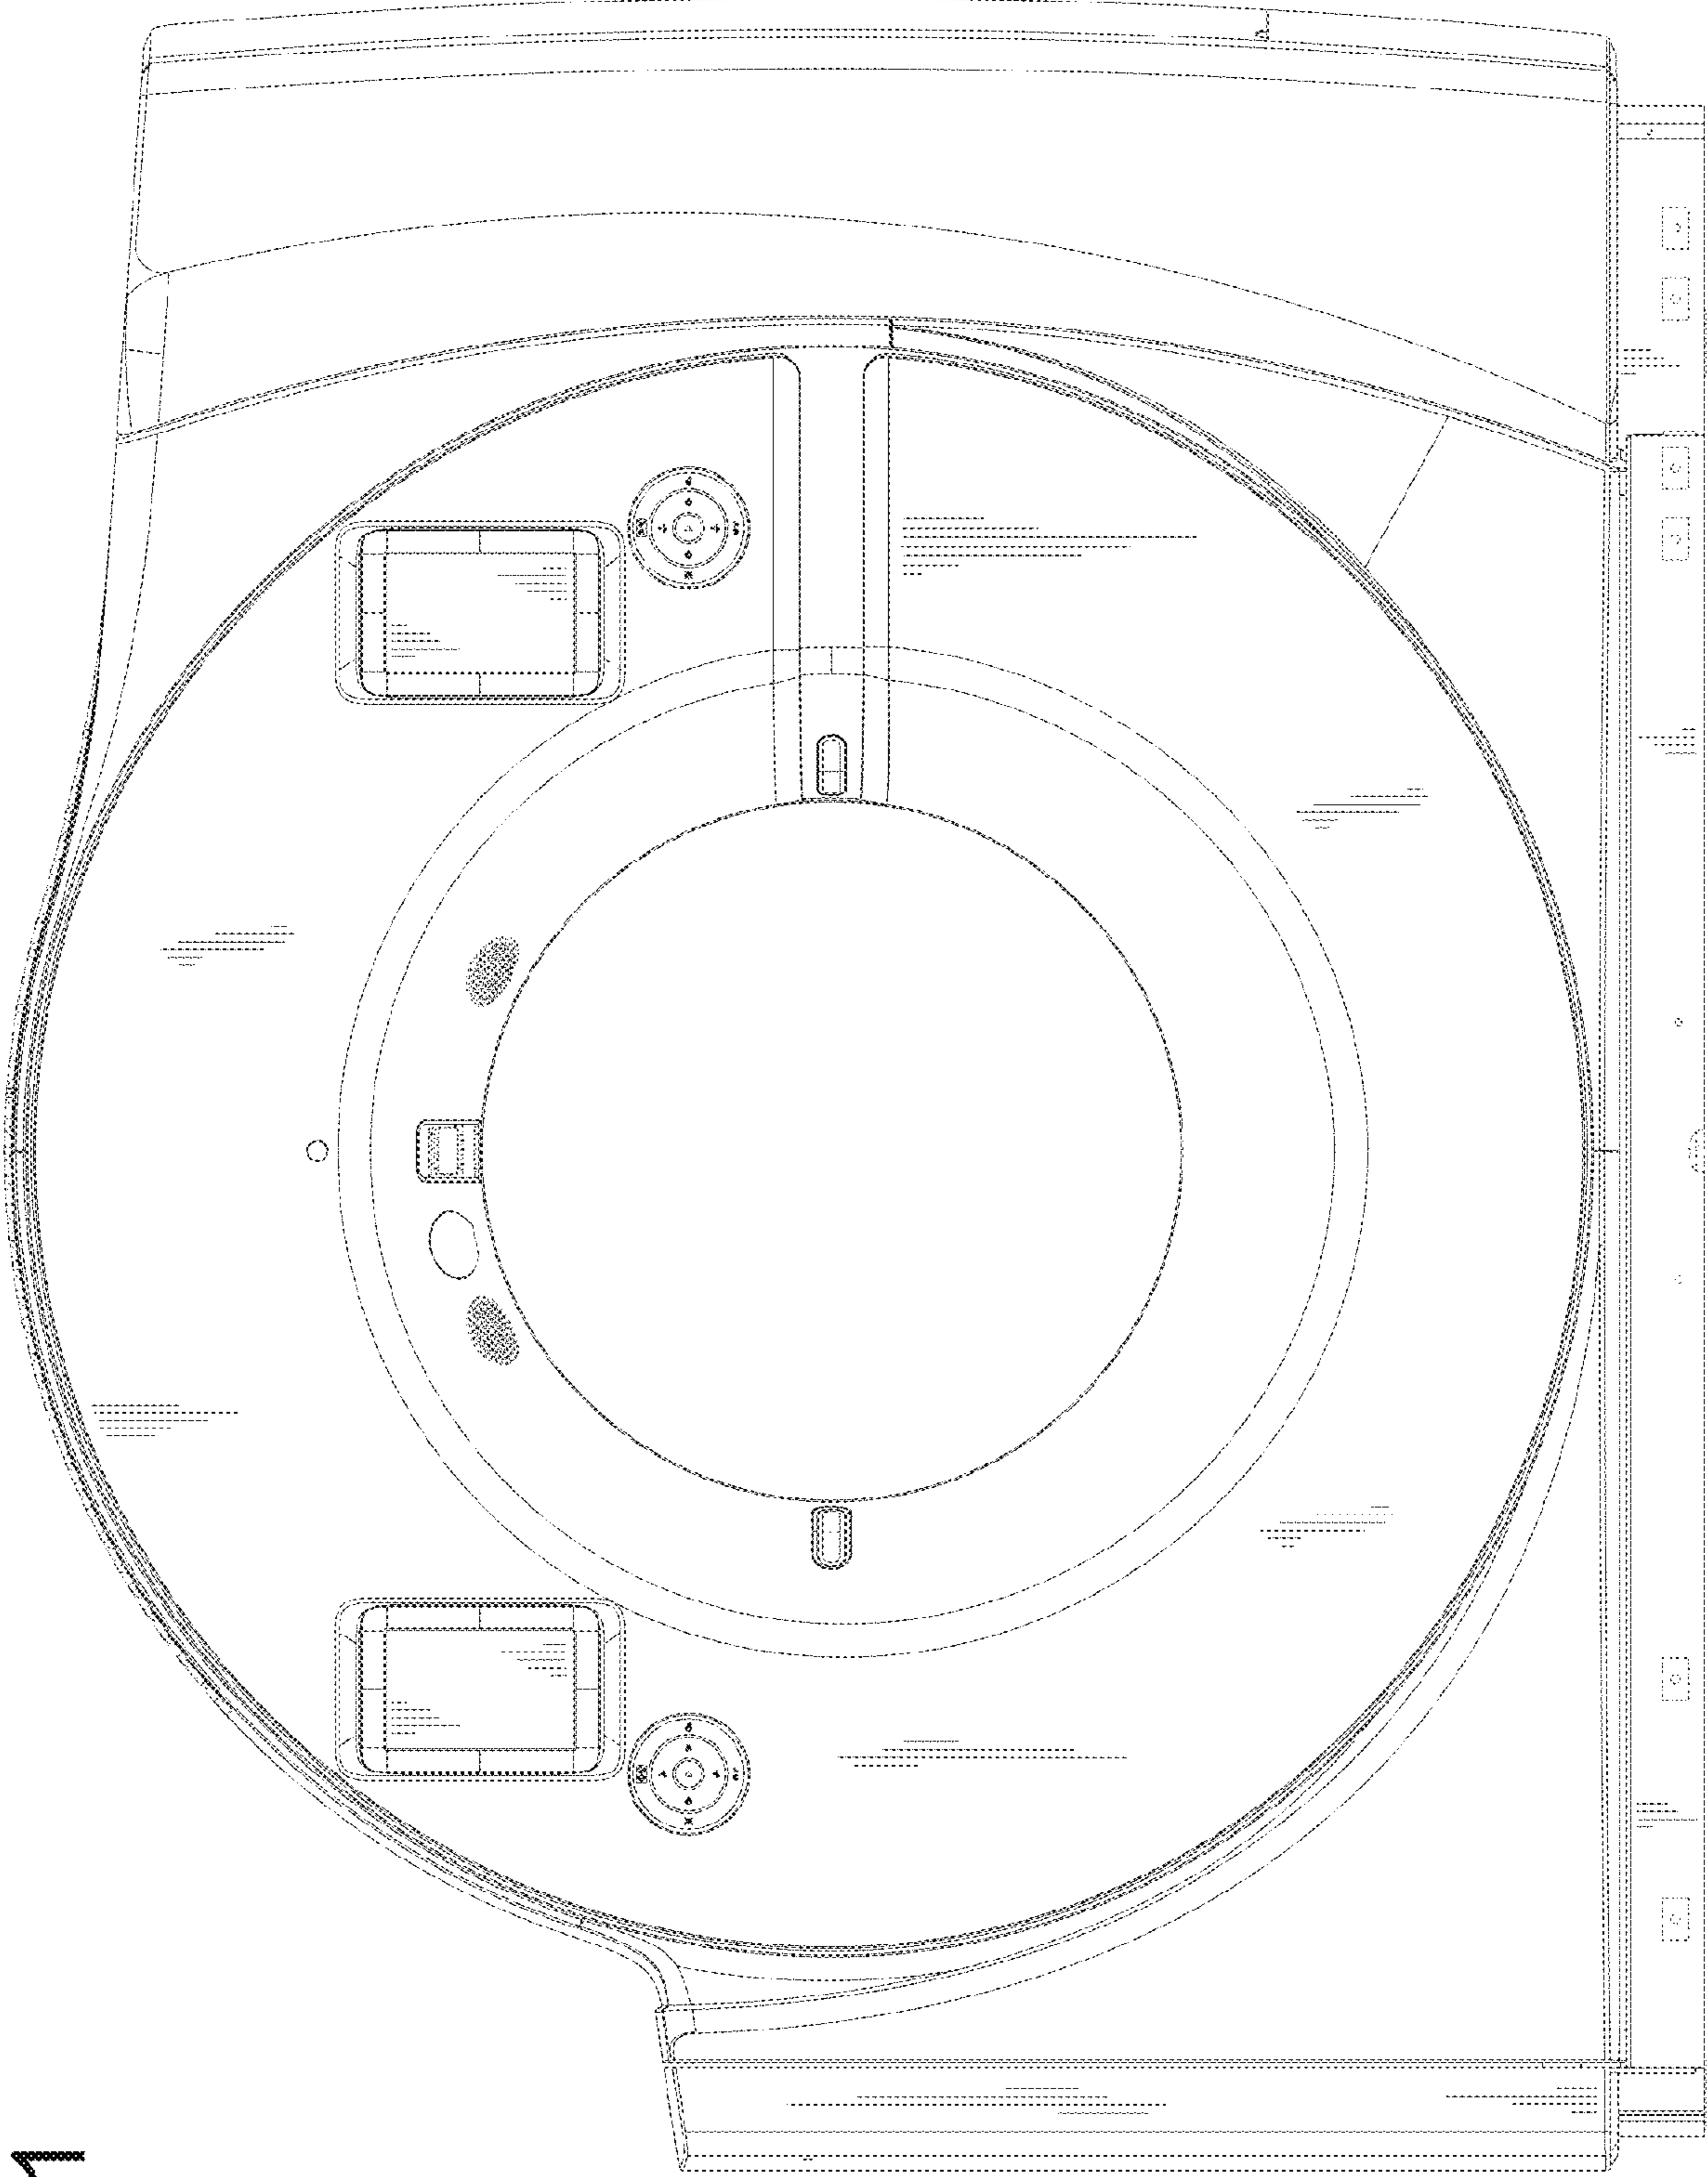
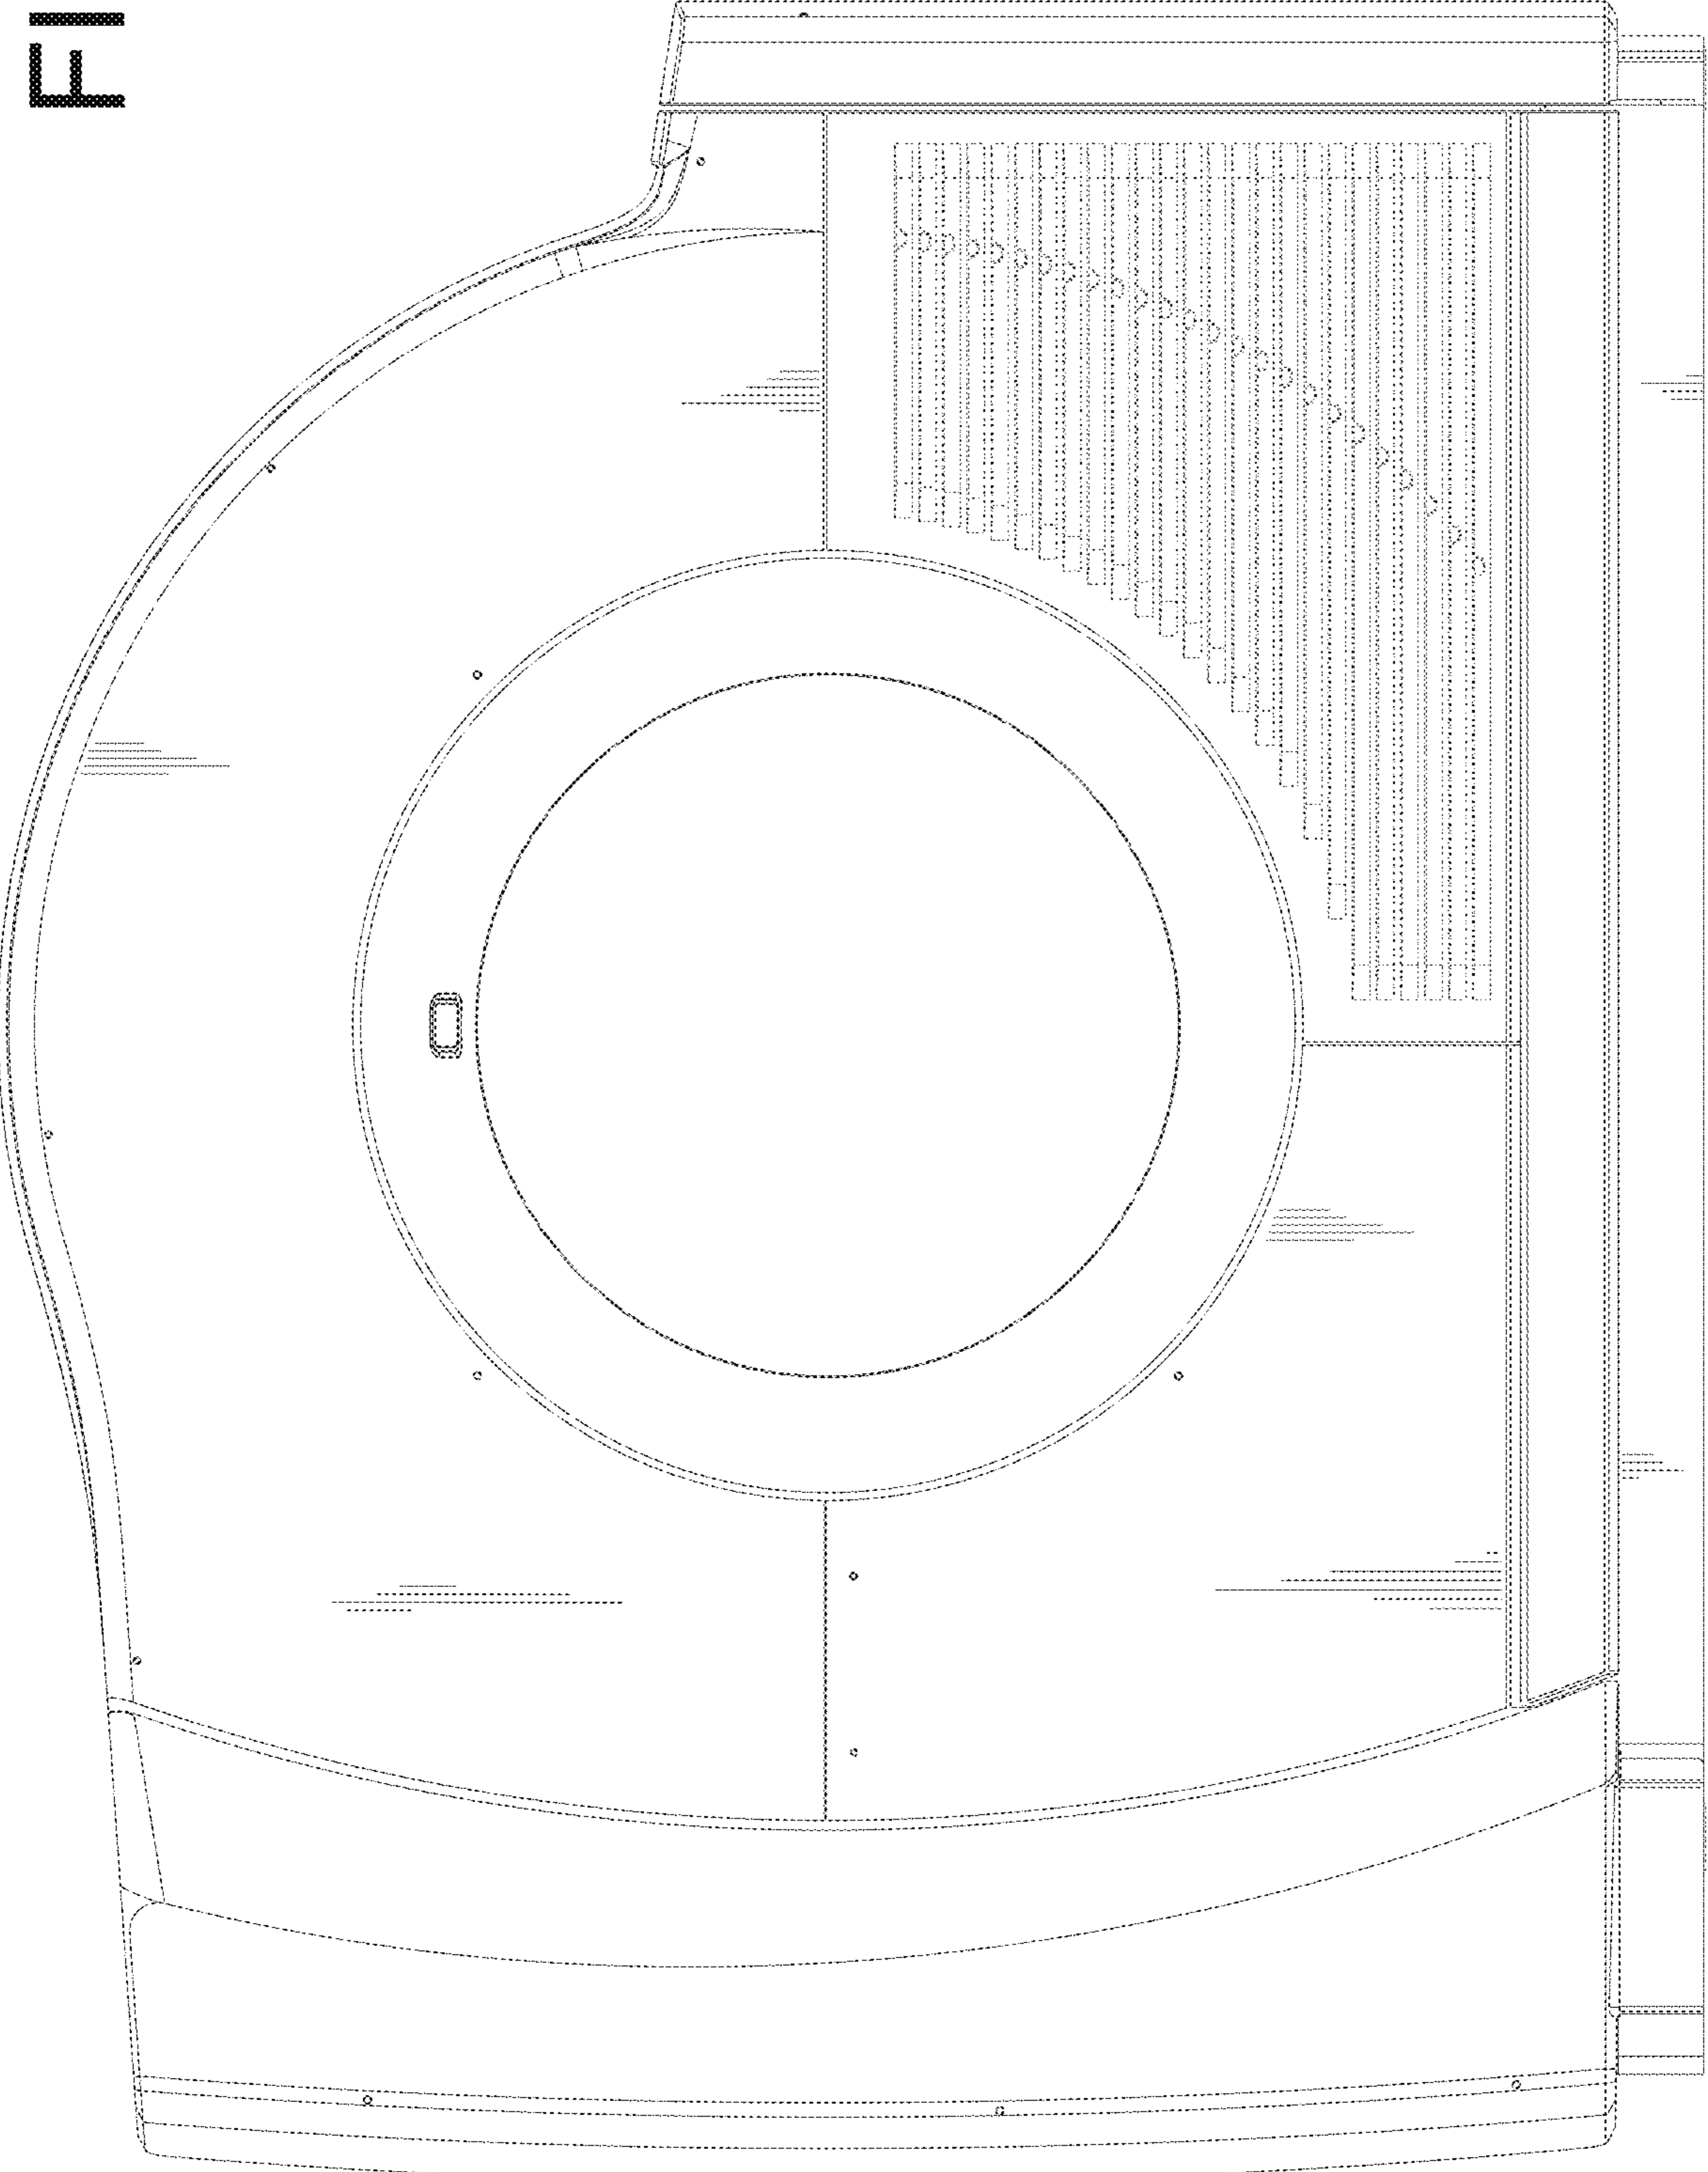


FIG. 1

FIG. 2



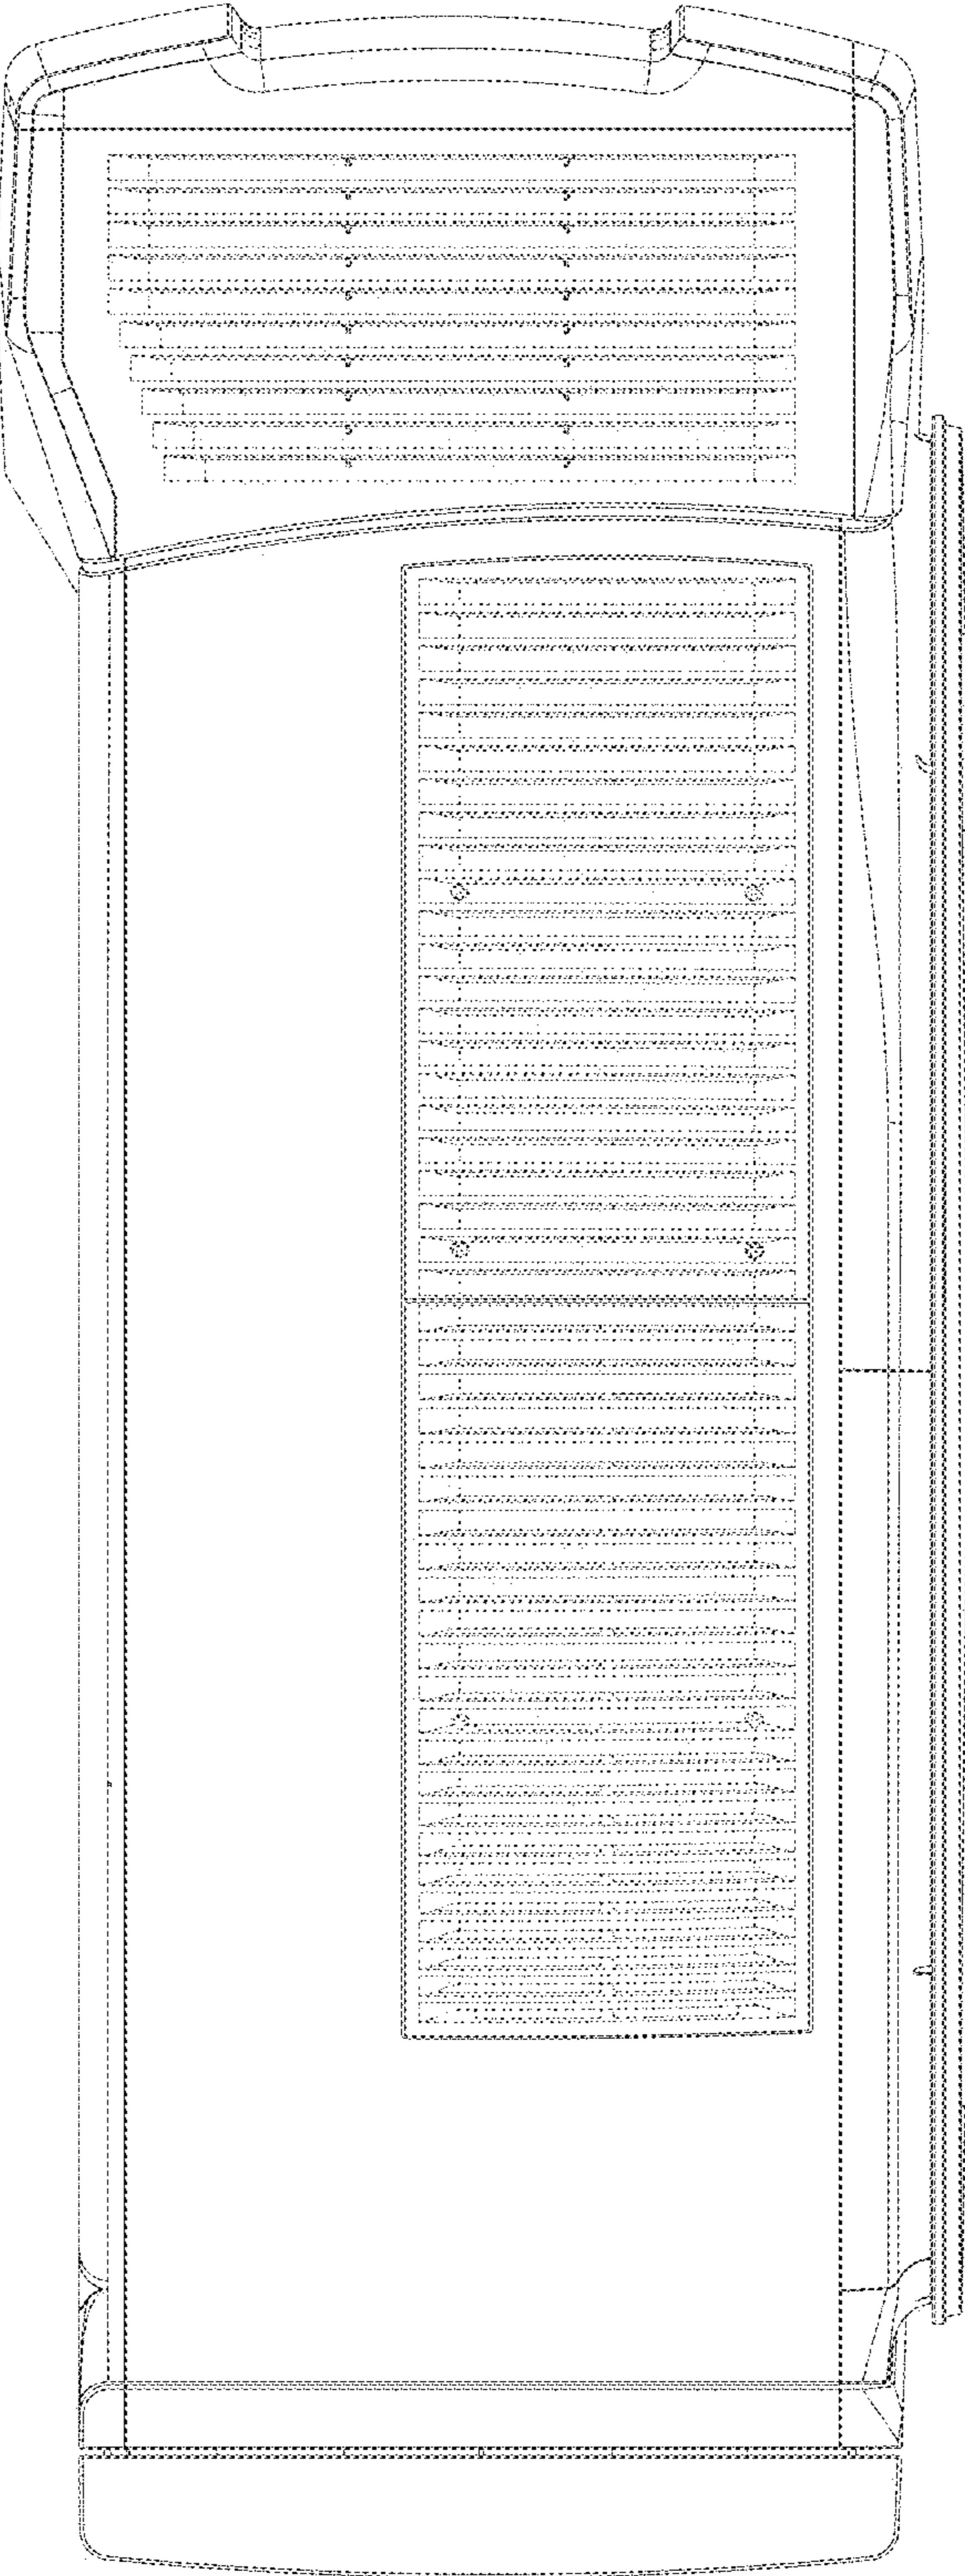


FIG. 3

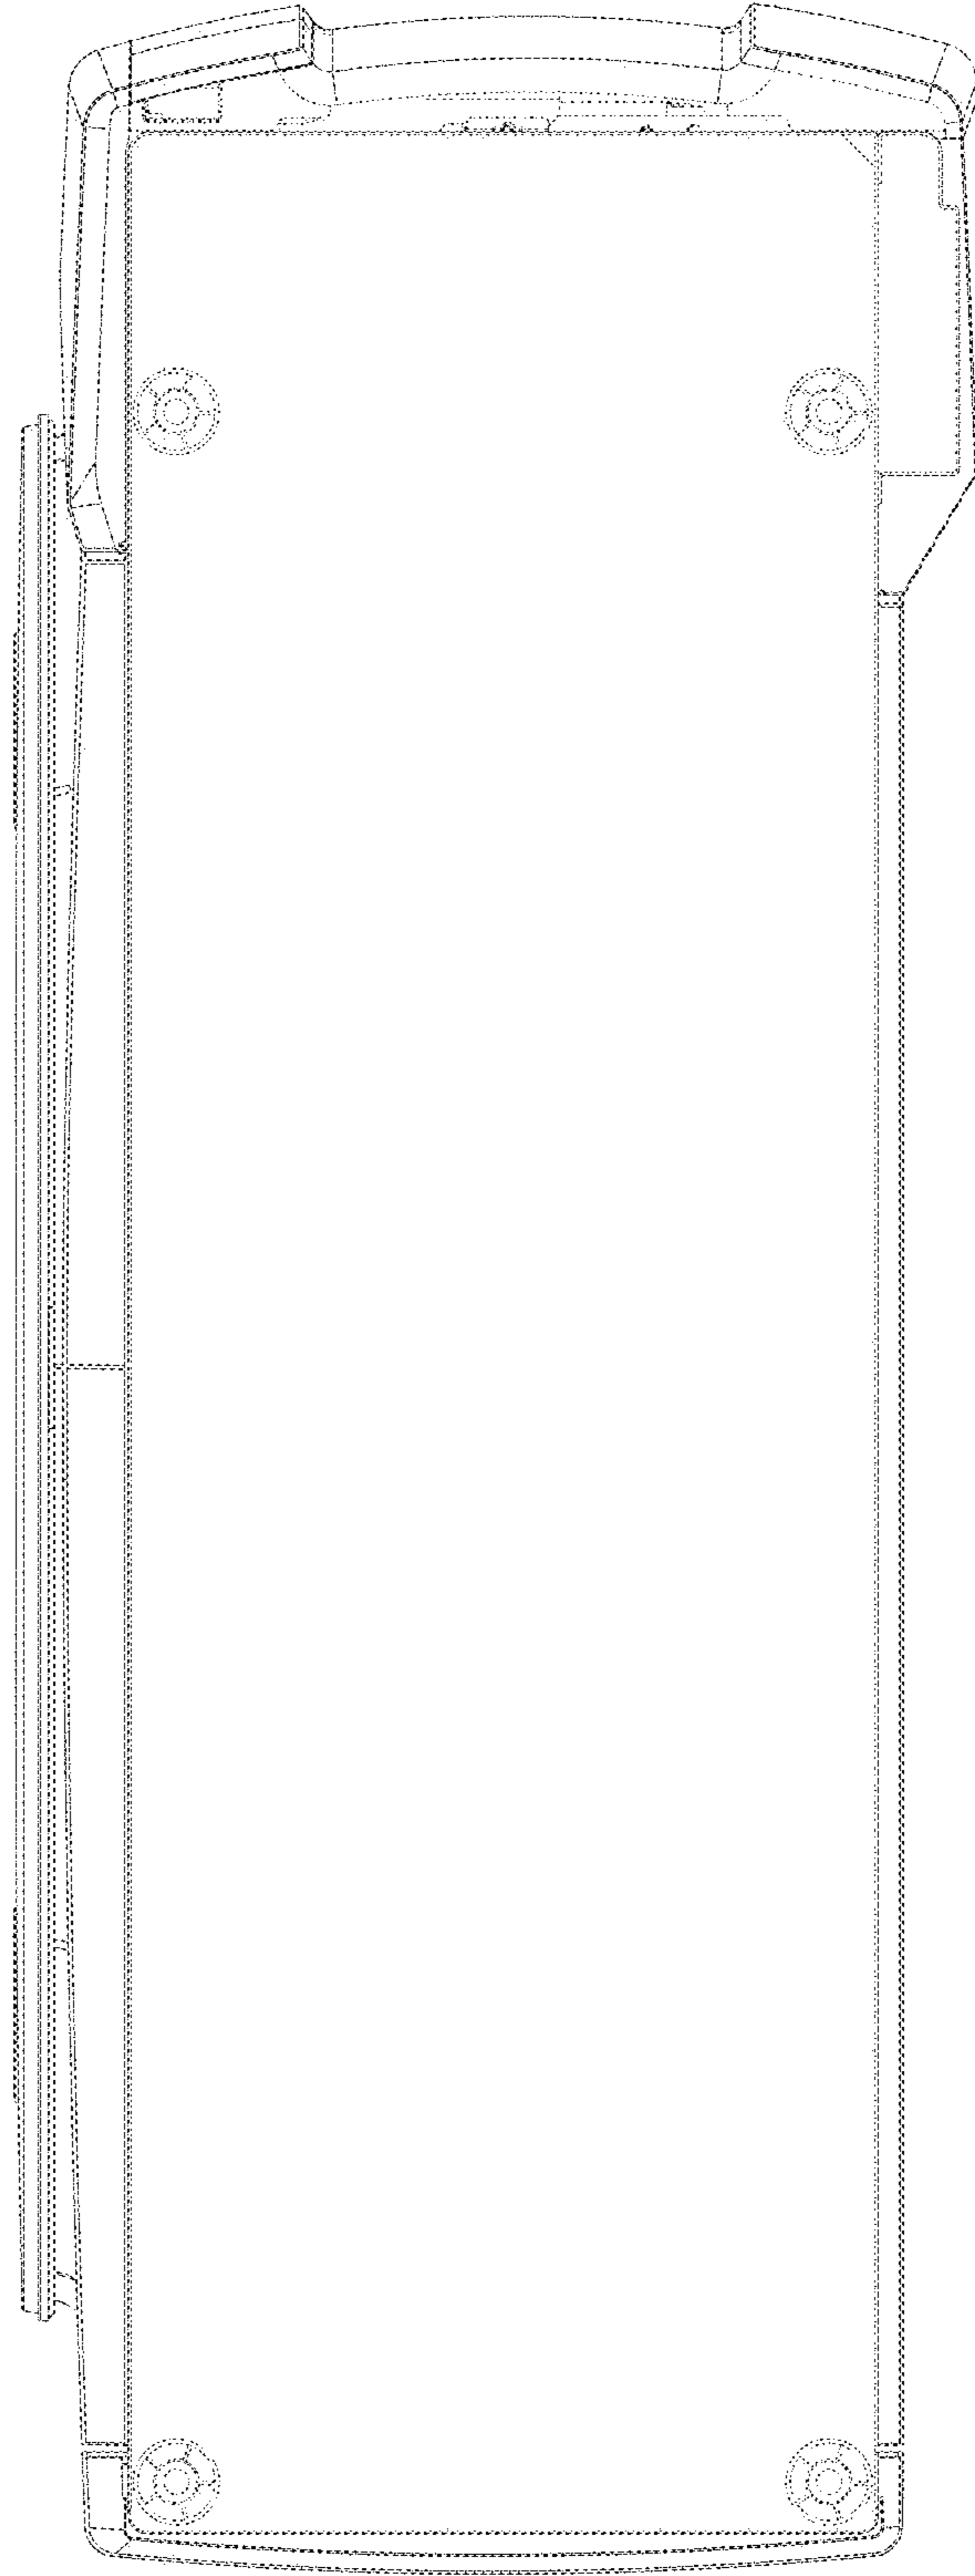


FIG. 4

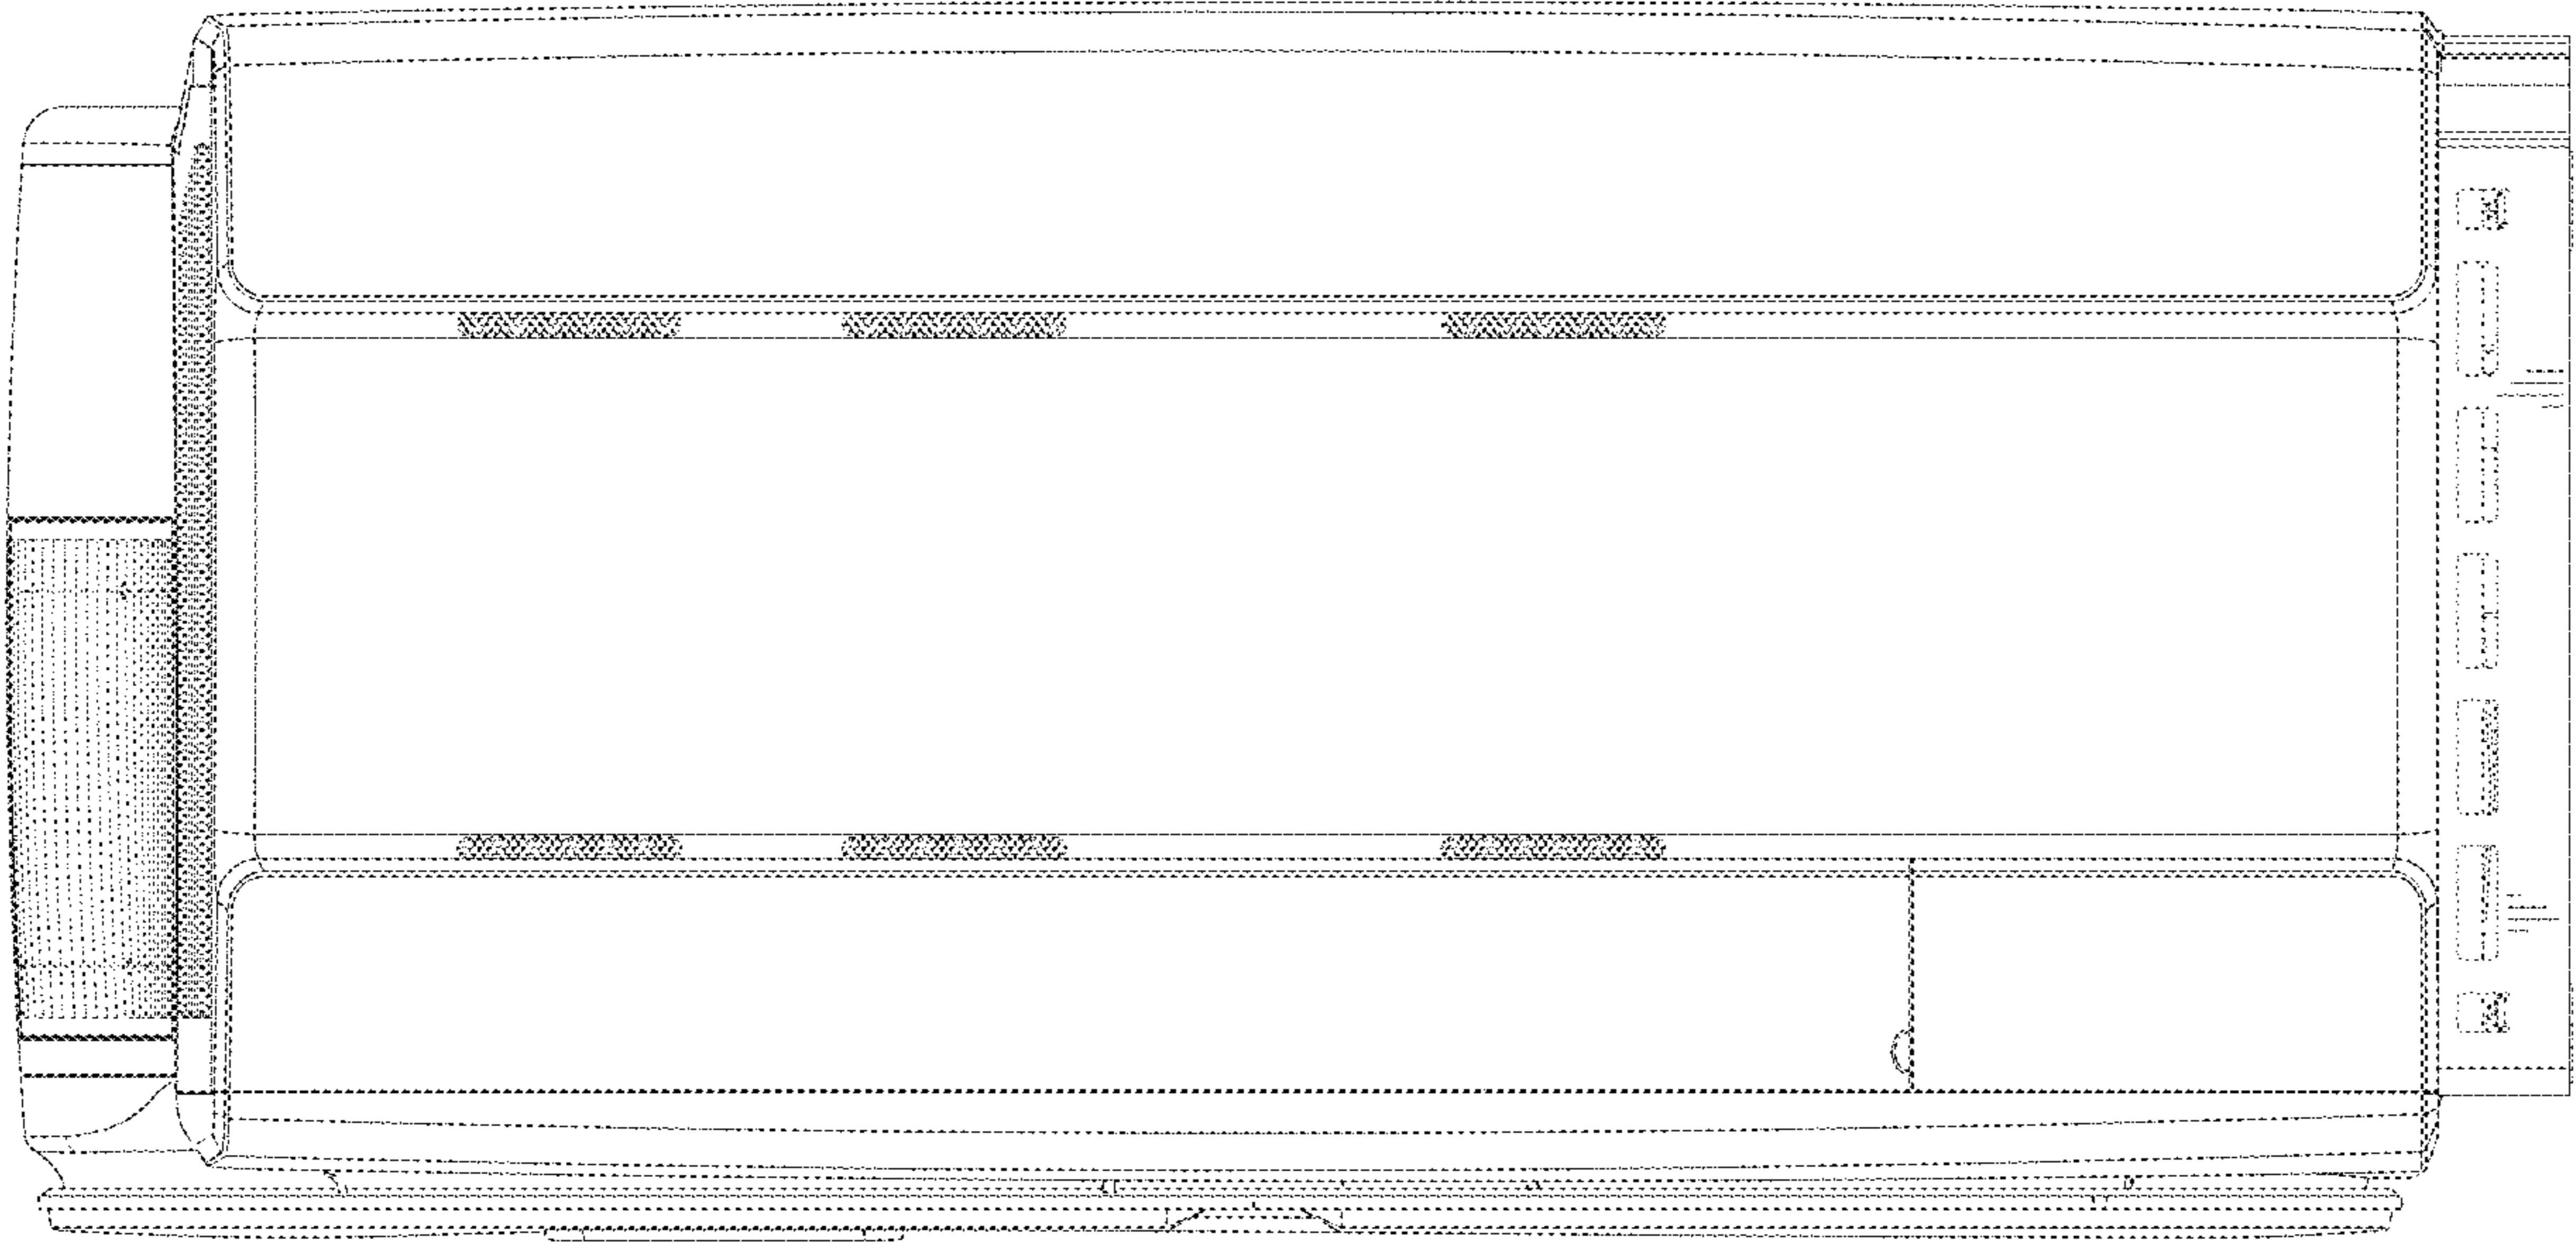


FIG. 5

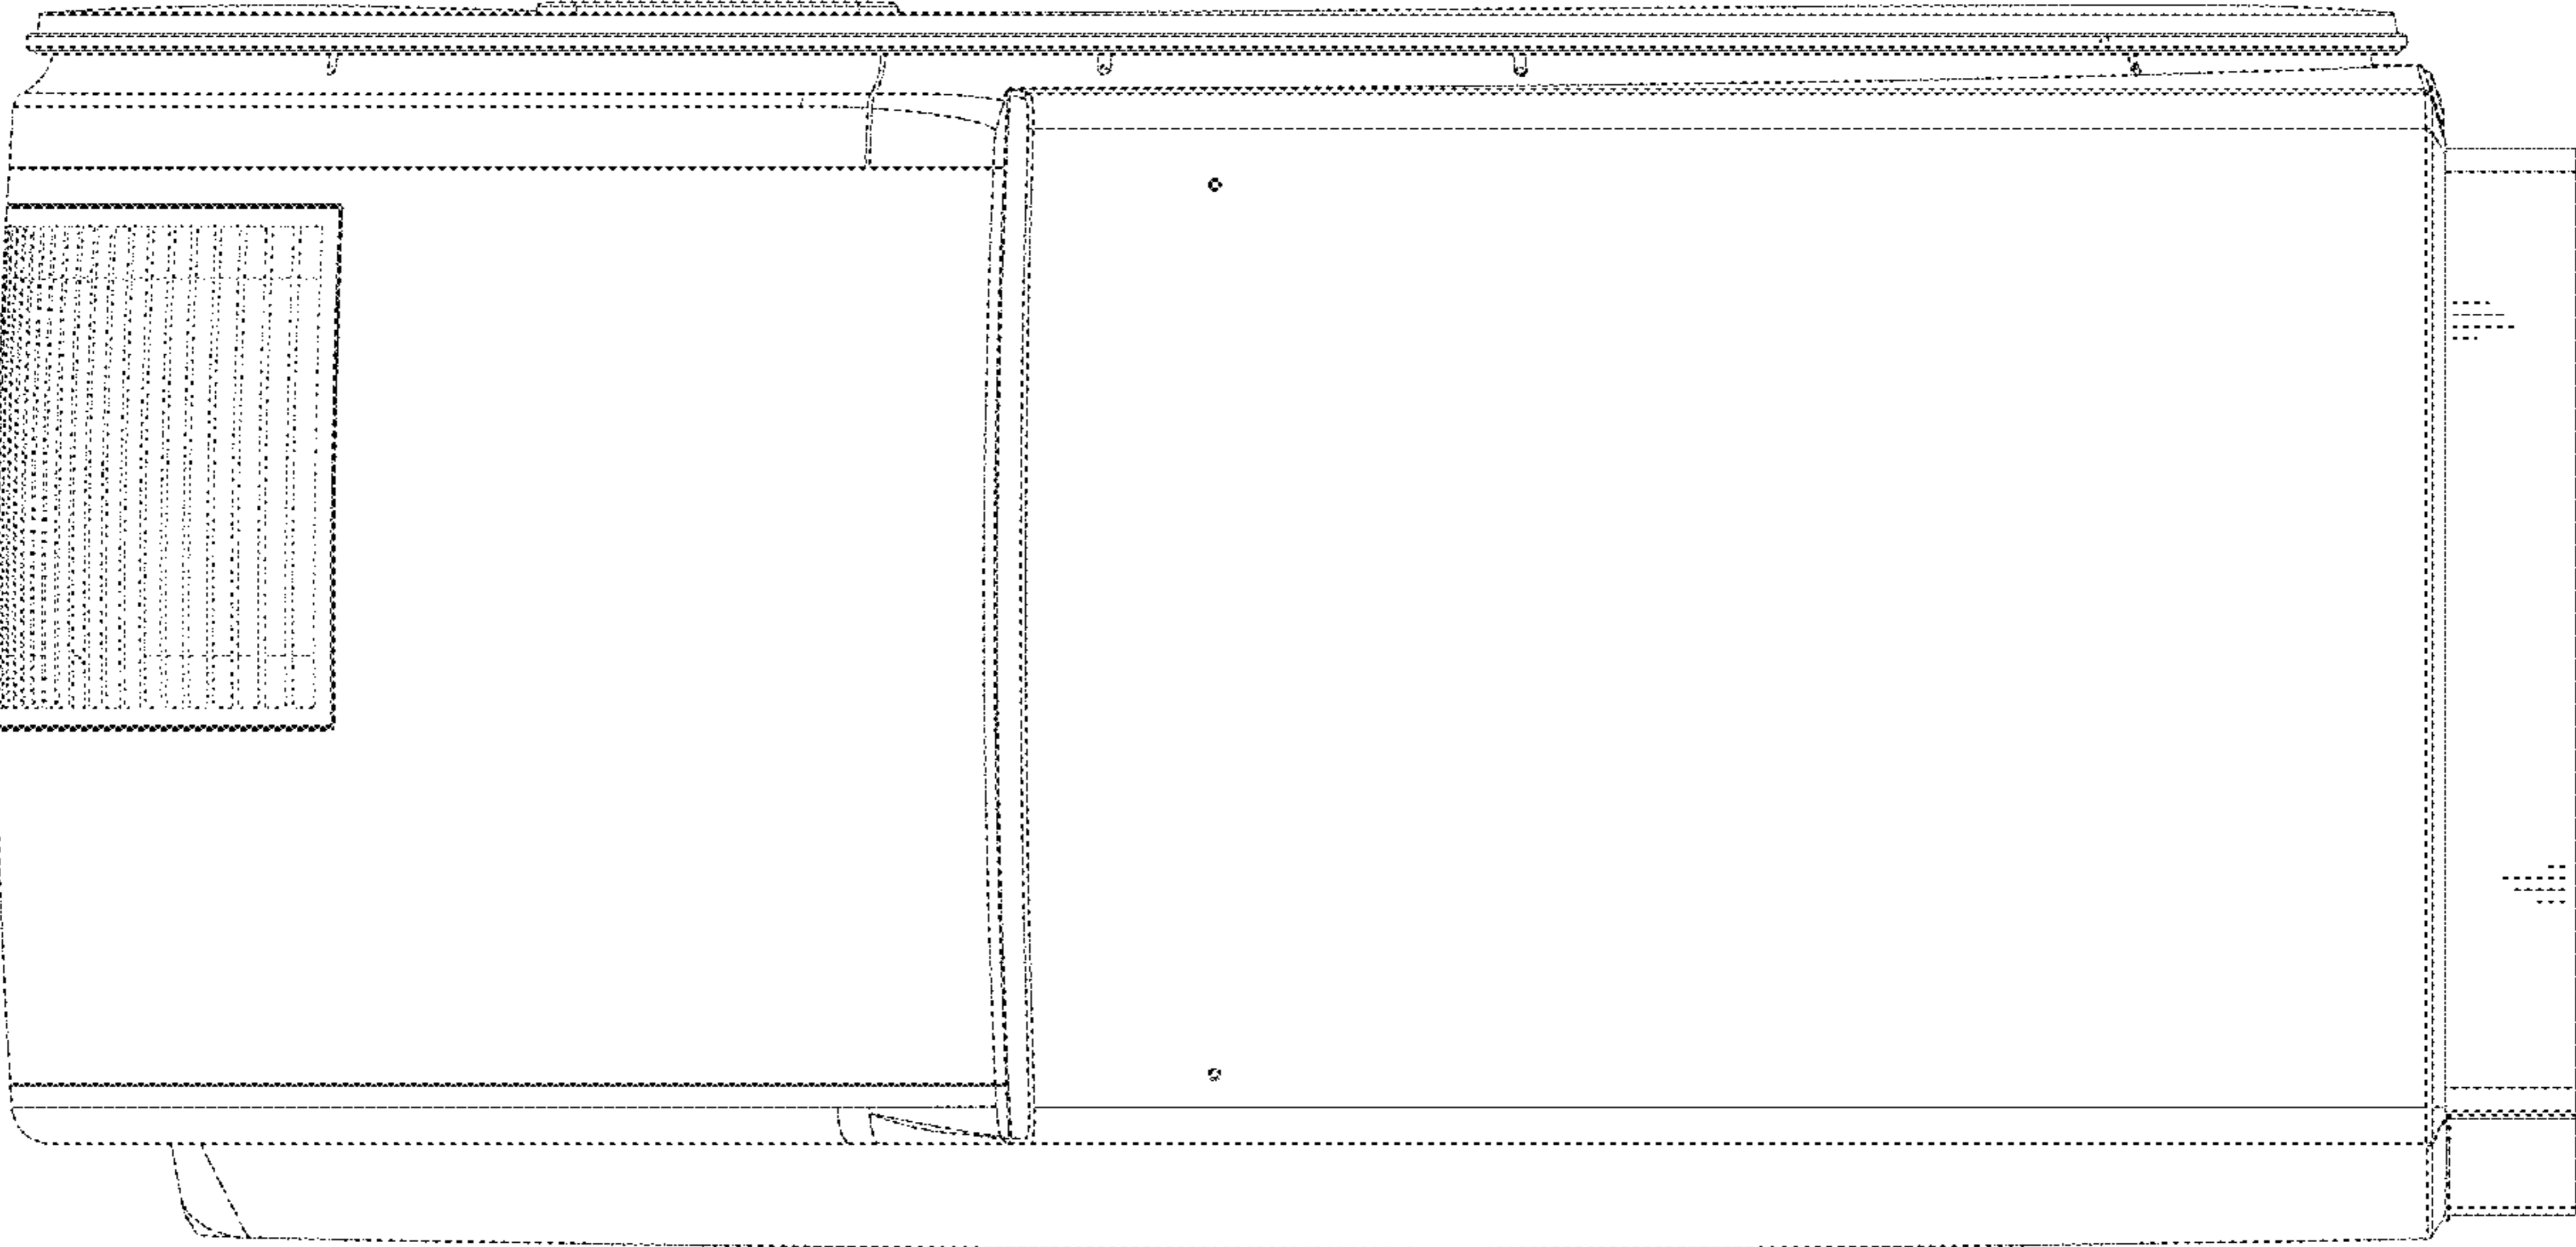


FIG. 6

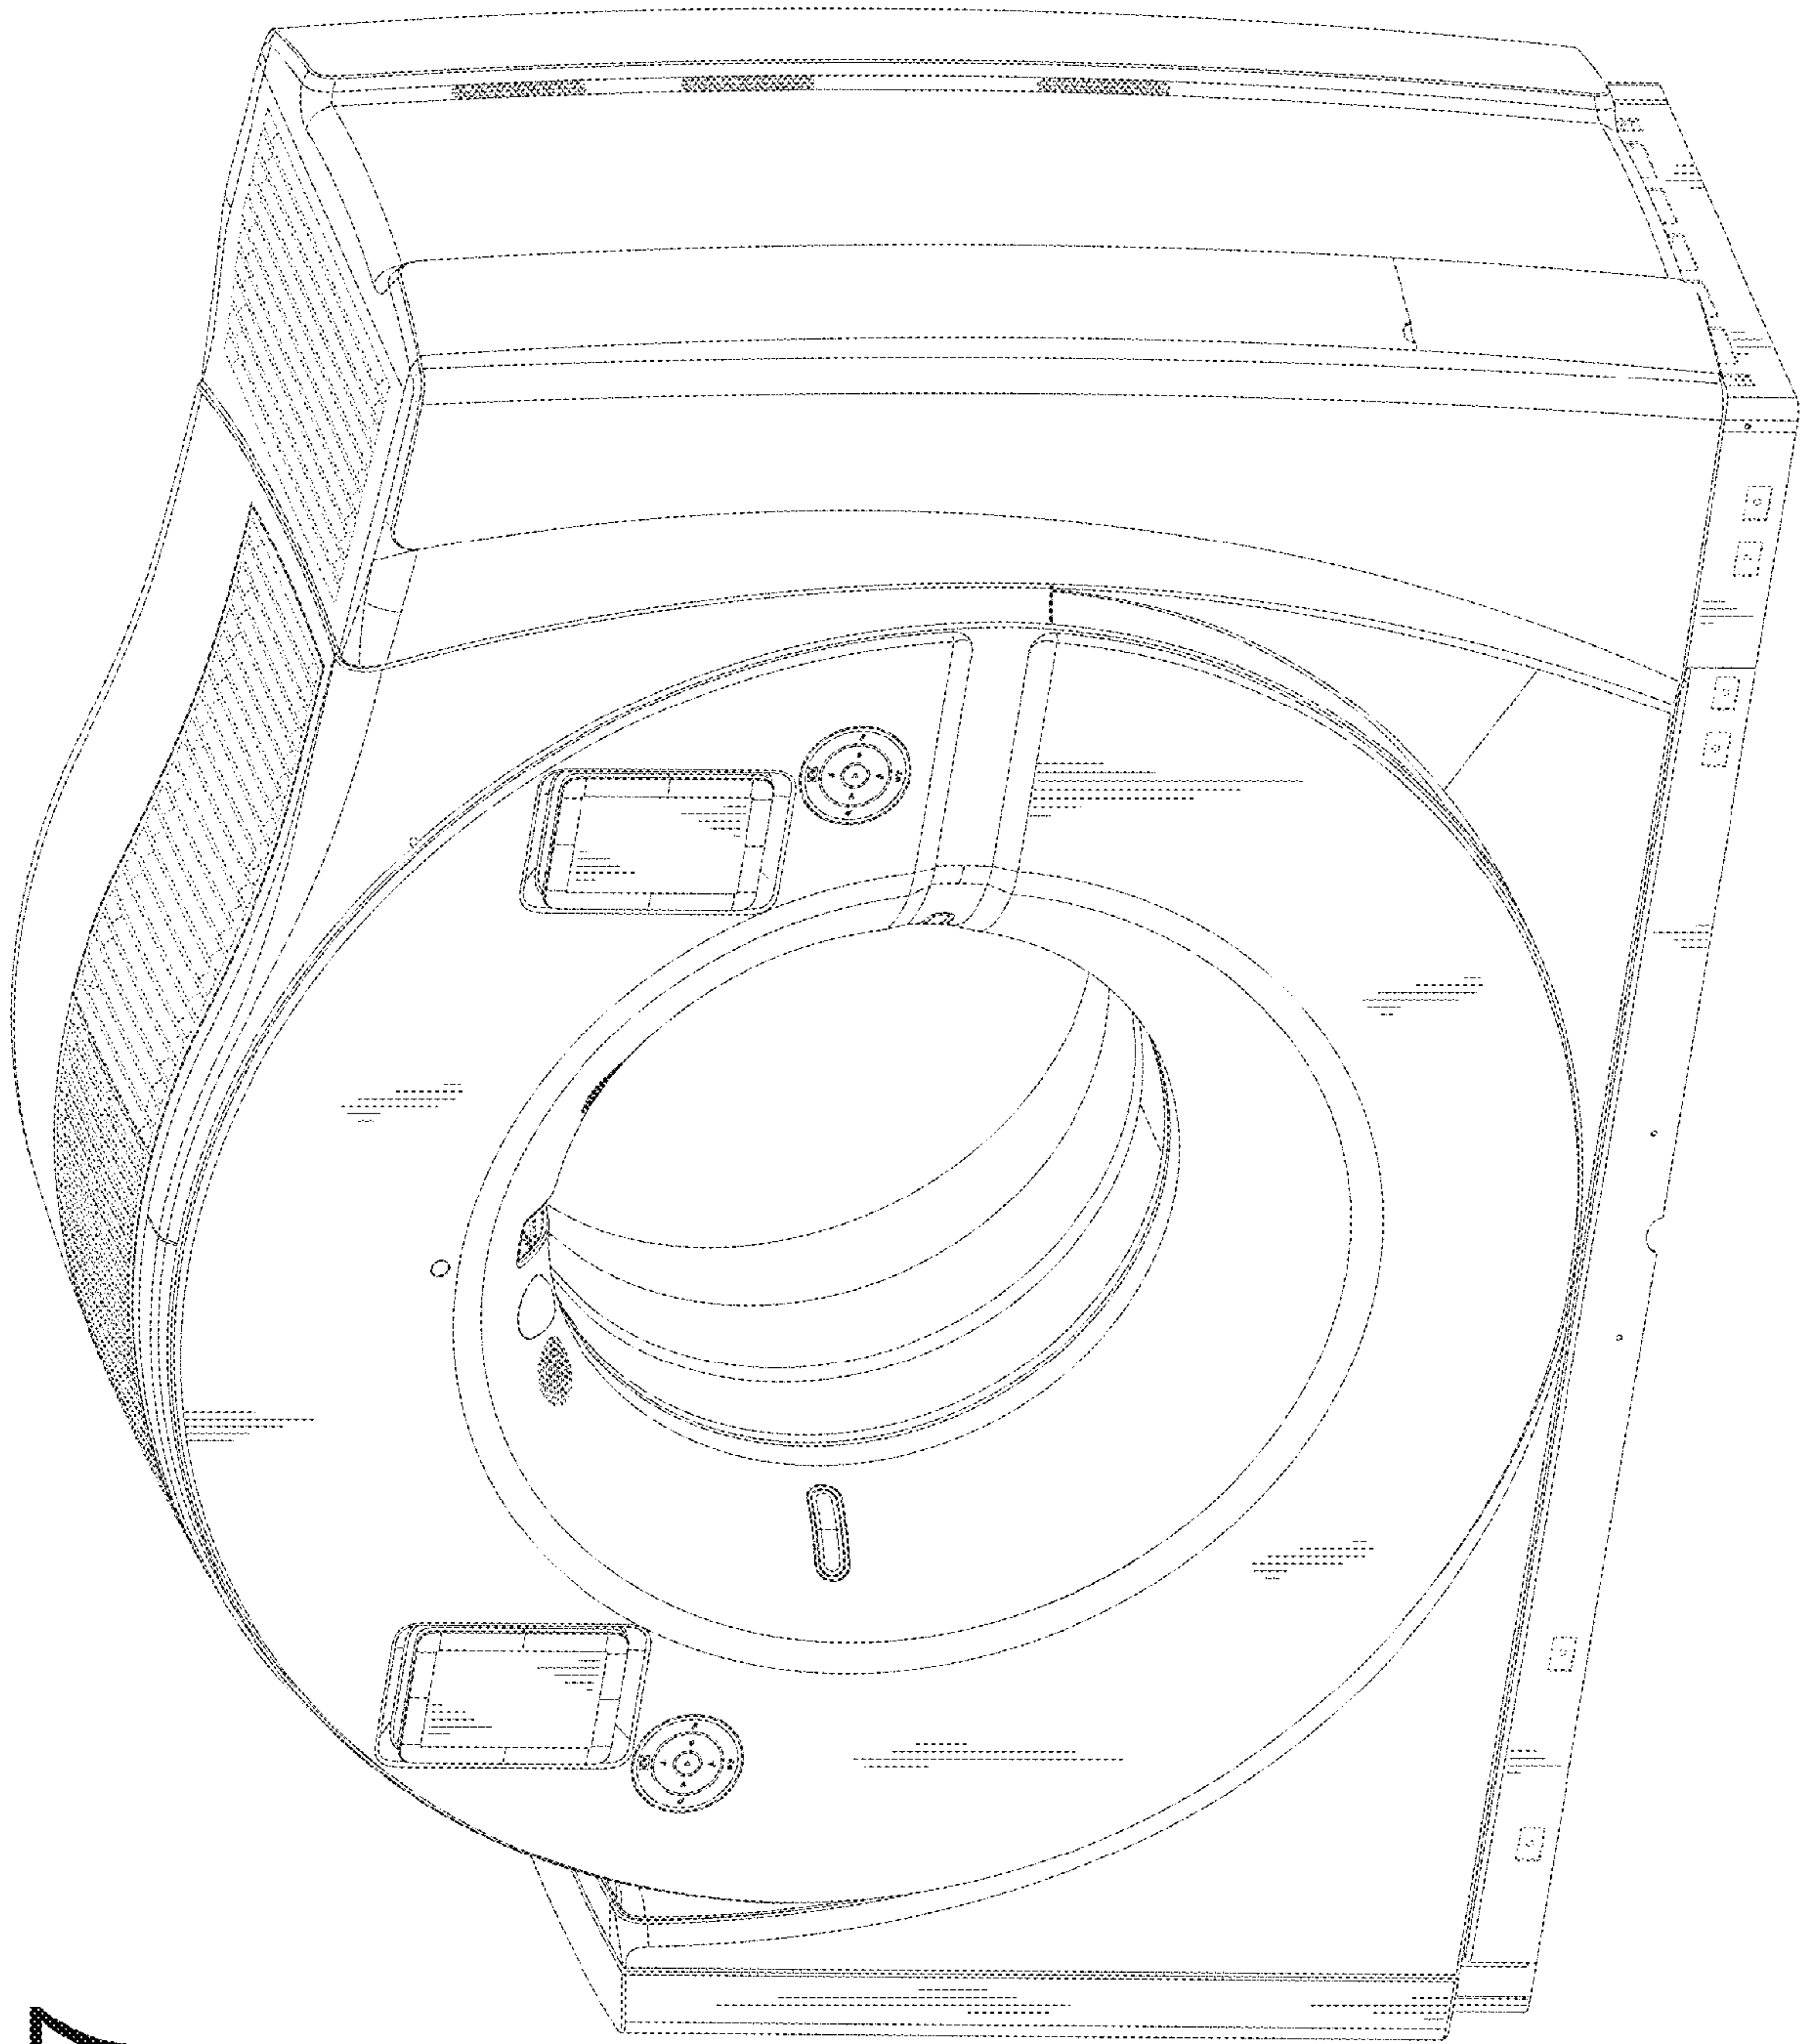


FIG. 7