



US00D940873S

(12) **United States Design Patent** (10) **Patent No.:** **US D940,873 S**
Gupta et al. (45) **Date of Patent:** **** Jan. 11, 2022**

(54) **MOBILE OPHTHALMOSCOPE**

(71) Applicant: **Spect Inc.**, Palo Alto, CA (US)

(72) Inventors: **Satish Chander Gupta**, New Delhi (IN); **Ankur Sudhir Gupta**, San Mateo, CA (US); **Bradley Cohen**, Evans, CO (US); **Michael Christopher Leung**, San Francisco, CA (US)

(73) Assignee: **SPECT, INC.**, Palo Alto, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/687,875**

(22) Filed: **Apr. 16, 2019**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
 USPC **D24/172**

(58) **Field of Classification Search**
 USPC D3/201, 203.1; D14/240, 250, 252, 255, D14/372; D16/100, 130, 131, 132, 133, D16/134, 135, 136, 137, 208, 218, 219, D16/220, 221, 237, 242, 243, 300, 331; D24/107, 133, 137, 138, 150, 158, 159, D24/160, 172, 183, 185, 186, 188, 216, D24/217, 218, 234

CPC A61B 3/00; A61B 3/0008; A61B 3/0016; A61B 3/0033; A61B 3/0041; A61B 3/005; A61B 3/0058; A61B 3/0075; A61B 3/0091; A61B 3/02; A61B 3/10; A61B 3/1176; A61B 3/12; A61B 3/1208; A61B 3/13; A61B 3/132; A61B 3/14; A61B 3/18; A61B 2017/00017; A61B 3/1005; A61F 9/00; A61F 9/007; A63F 2300/8082; B24B 1/00; B24B 1/002; B24B 1/005; B24B 1/007; B24B 1/04; B24B 1/24; B24B 1/0025

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,673,097 A * 9/1997 Heacock A61B 3/1025 351/215

D626,744 S * 11/2010 Roman A61B 3/107 D3/269

D669,587 S * 10/2012 Mayer A61B 3/1025 D24/158

D682,903 S * 5/2013 Bratt D16/131

D697,957 S * 1/2014 Glasse D16/134

D712,389 S * 9/2014 Namminga D14/250

D739,452 S * 9/2015 Adams D16/208

(Continued)

OTHER PUBLICATIONS

Youtube, "How To: Setting Up and Using the Welch Allyn iExaminer", first available Aug. 22, 2012. (<https://www.youtube.com/watch?v=sDYnY7q0UBY&t=3s>) (Year: 2012).*

(Continued)

Primary Examiner — Lauren D McVey
Assistant Examiner — Justin A Johnson
 (74) *Attorney, Agent, or Firm* — Jonathan D. Feuchtwang


(57) **CLAIM**

The ornamental design for a mobile ophthalmoscope, as shown and described.

DESCRIPTION

FIG. 1 is a front view of the mobile ophthalmoscope showing our new design;
 FIG. 2 is a rear view of the mobile ophthalmoscope;
 FIG. 3 is a left view of the mobile ophthalmoscope;
 FIG. 4 is a right view of the mobile ophthalmoscope;
 FIG. 5 is a top view of the mobile ophthalmoscope;
 FIG. 6 is a bottom view of the mobile ophthalmoscope; and,
 FIG. 7 is a front perspective view of the mobile ophthalmoscope.
 The broken lines illustrate portions of the mobile ophthalmoscope and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

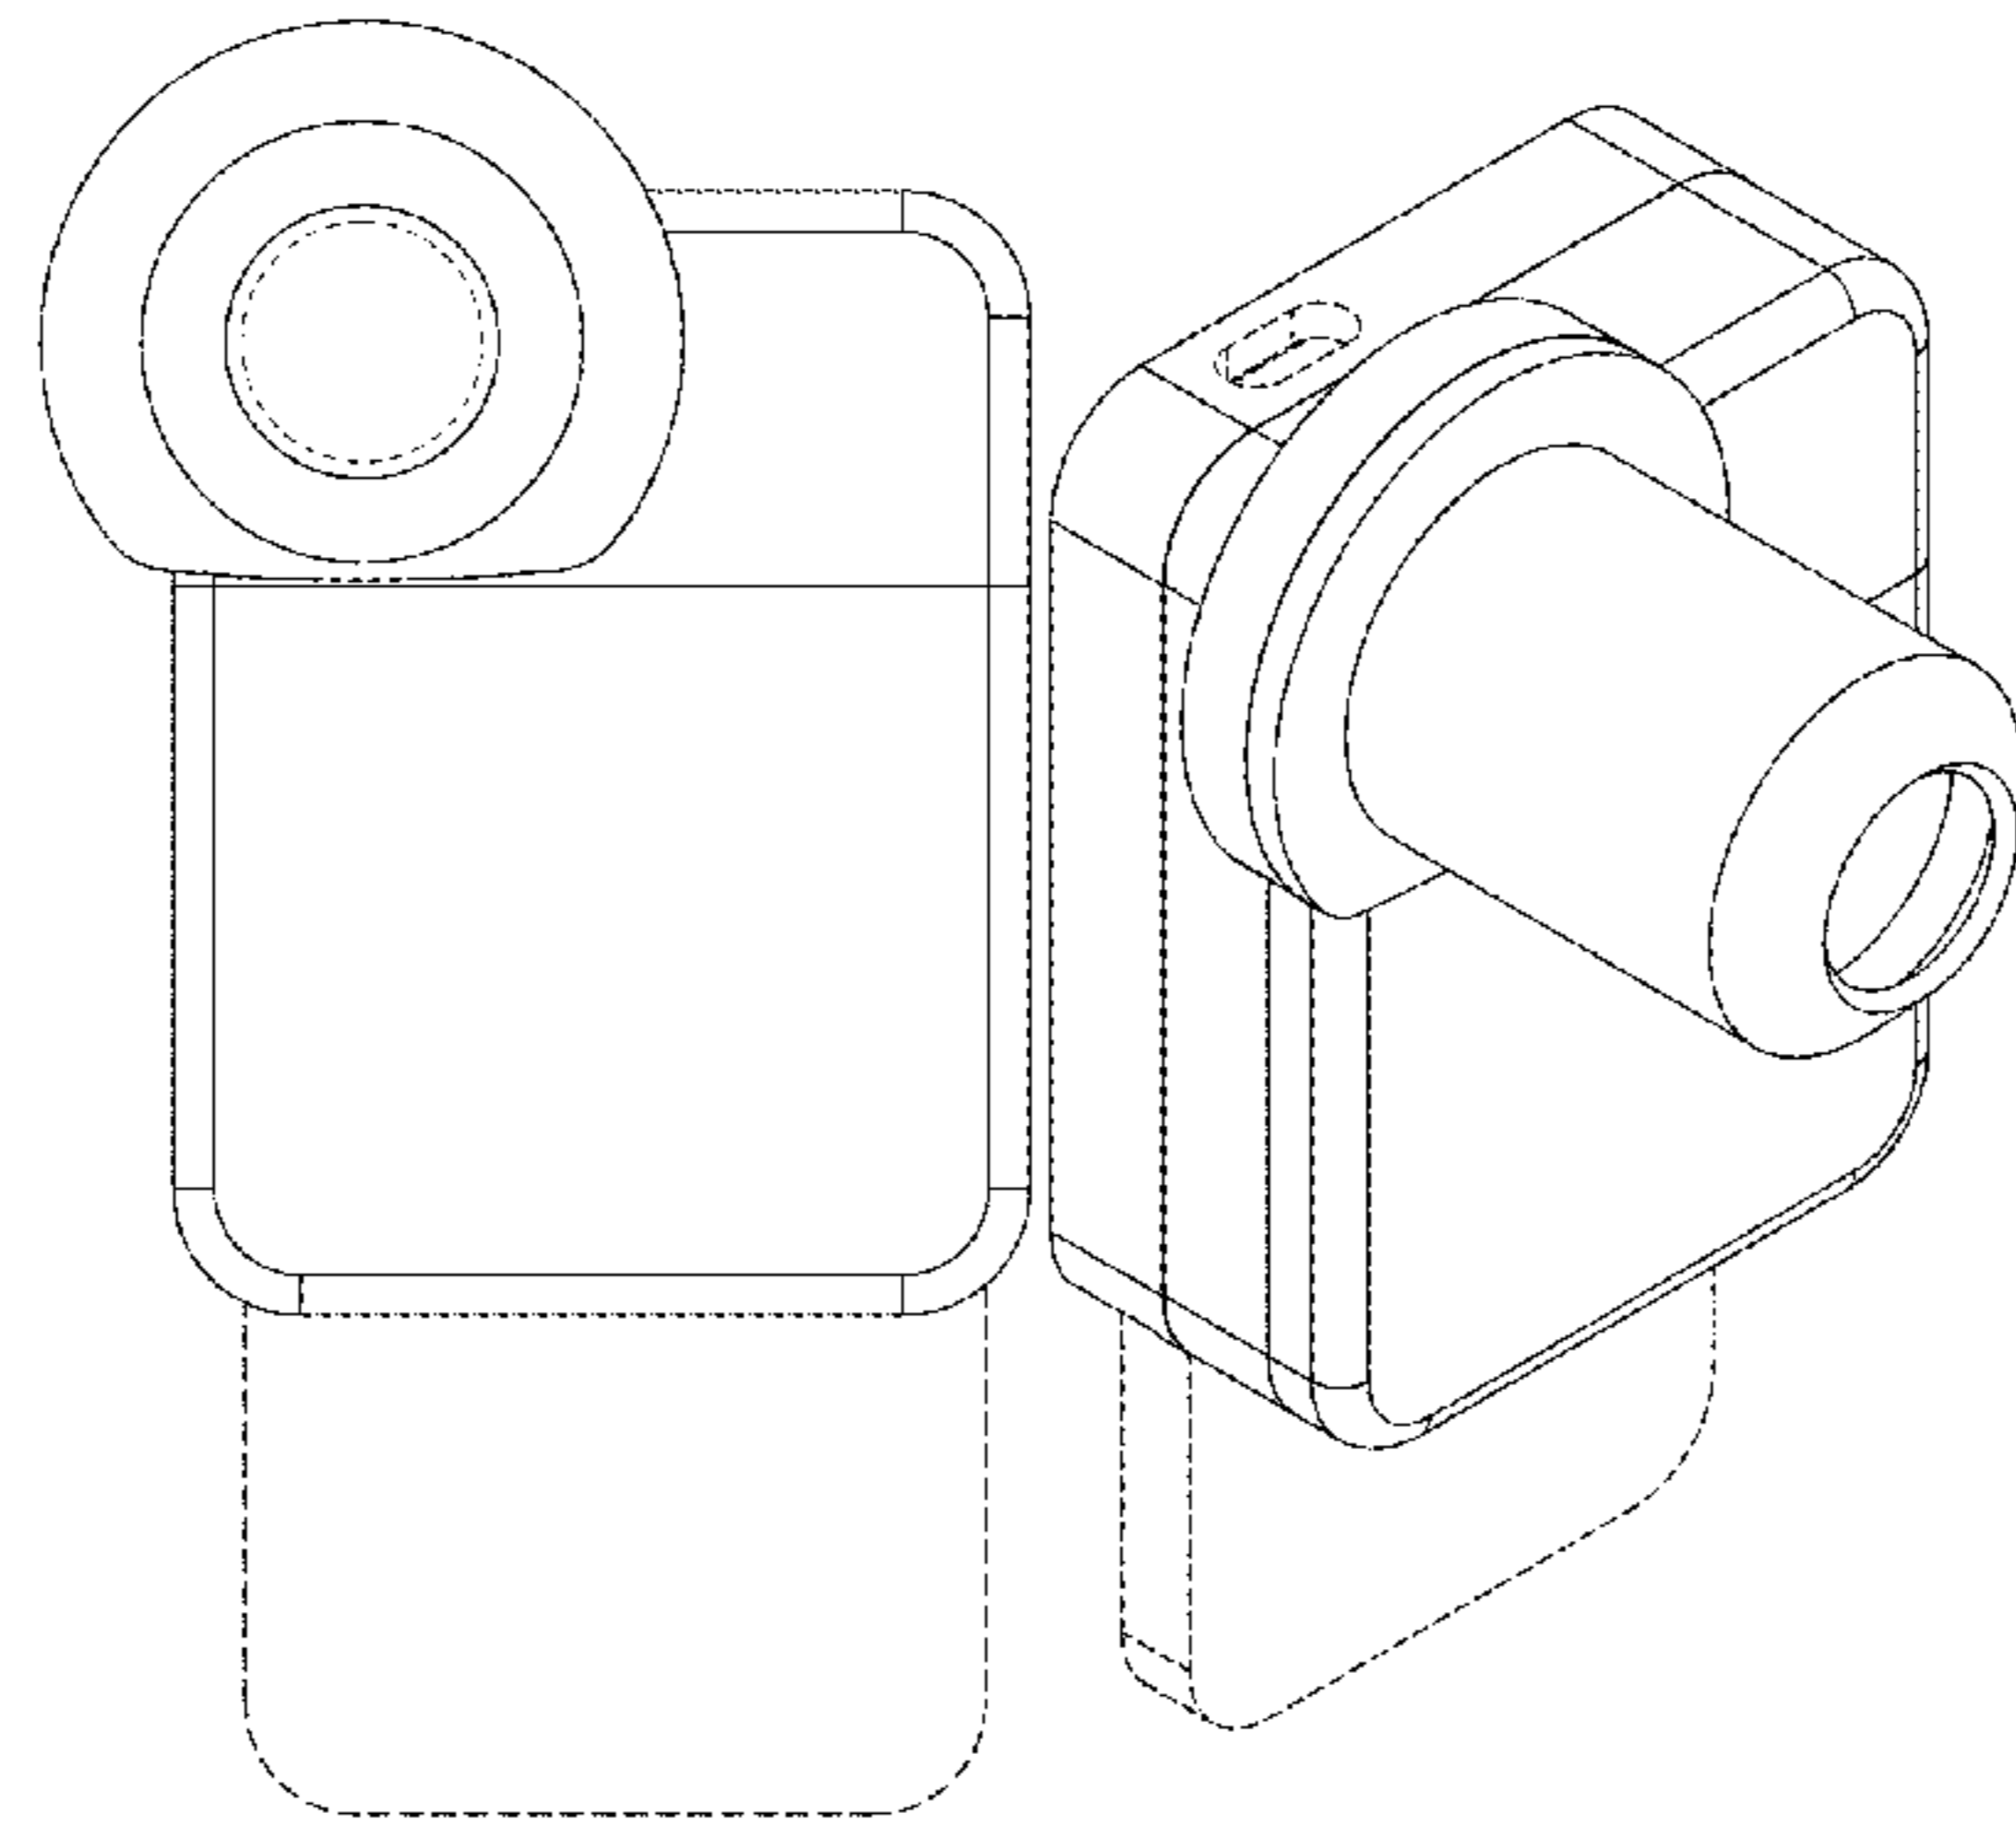

(56)

References Cited

U.S. PATENT DOCUMENTS

D757,696 S * 5/2016 Eski D14/240
D772,215 S * 11/2016 Mulumudi D14/250
D852,251 S * 6/2019 Skolianos D16/130
D915,490 S * 4/2021 Grant D16/208
2018/0092534 A1 * 4/2018 Nabhan G16H 50/20
2021/0093185 A1 * 4/2021 Obszanski A61B 3/107

OTHER PUBLICATIONS

DH Gate, "Cell Phone Camera Lens Zoom Mobile Monocular Telescope", first available Mar. 10, 2017. (<https://www.dhgate.com/product/waterproof-monocular-telescope-day-and-night/391308279.html>) (Year: 2017).*

Reddit, "I modeled and printed some lens adapters for my phone camera", first available Jul. 13, 2018. (https://www.reddit.com/r/3Dprinting/comments/8yn15t/i_modeled_and_printed_some_lens_adapters_for_my/) (Year: 2018).*

Youtube, "QuikVue Smartphone Eye Imaging Adaptor Operation Video", first available Mar. 25, 2019. (<https://www.youtube.com/watch?v=cZzTvuVQmx4>) (Year: 2019).*

* cited by examiner

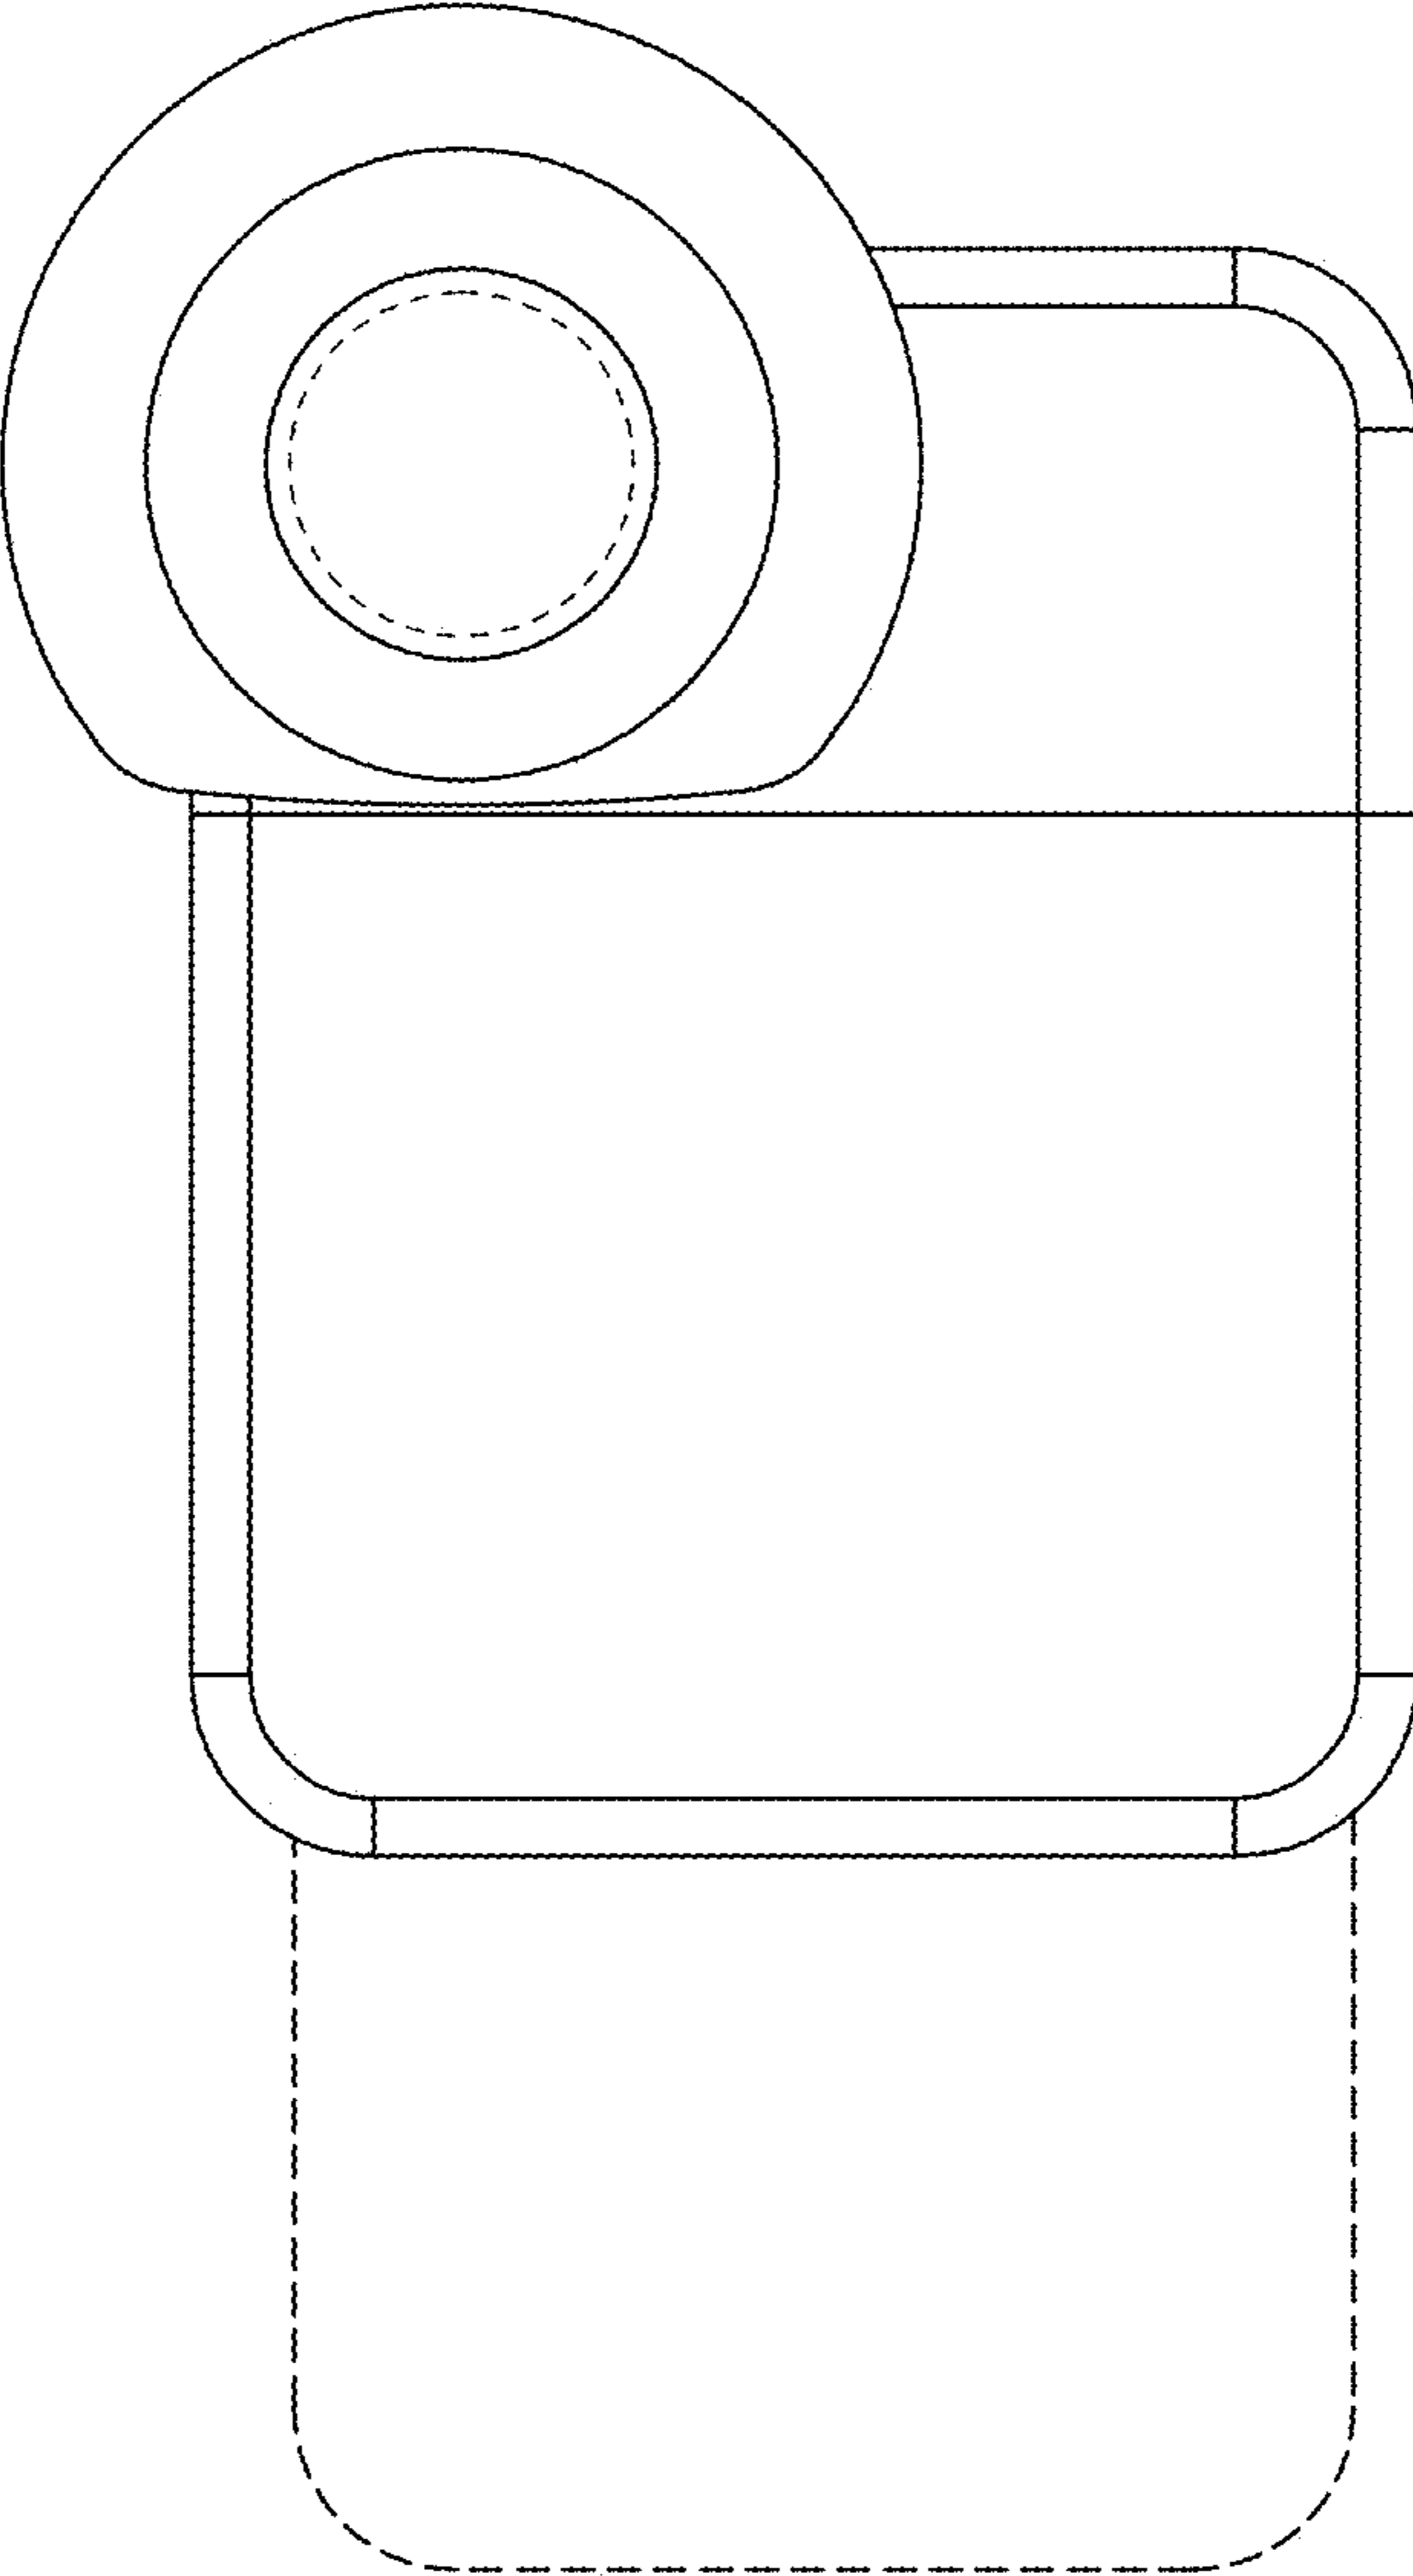


FIG. 1

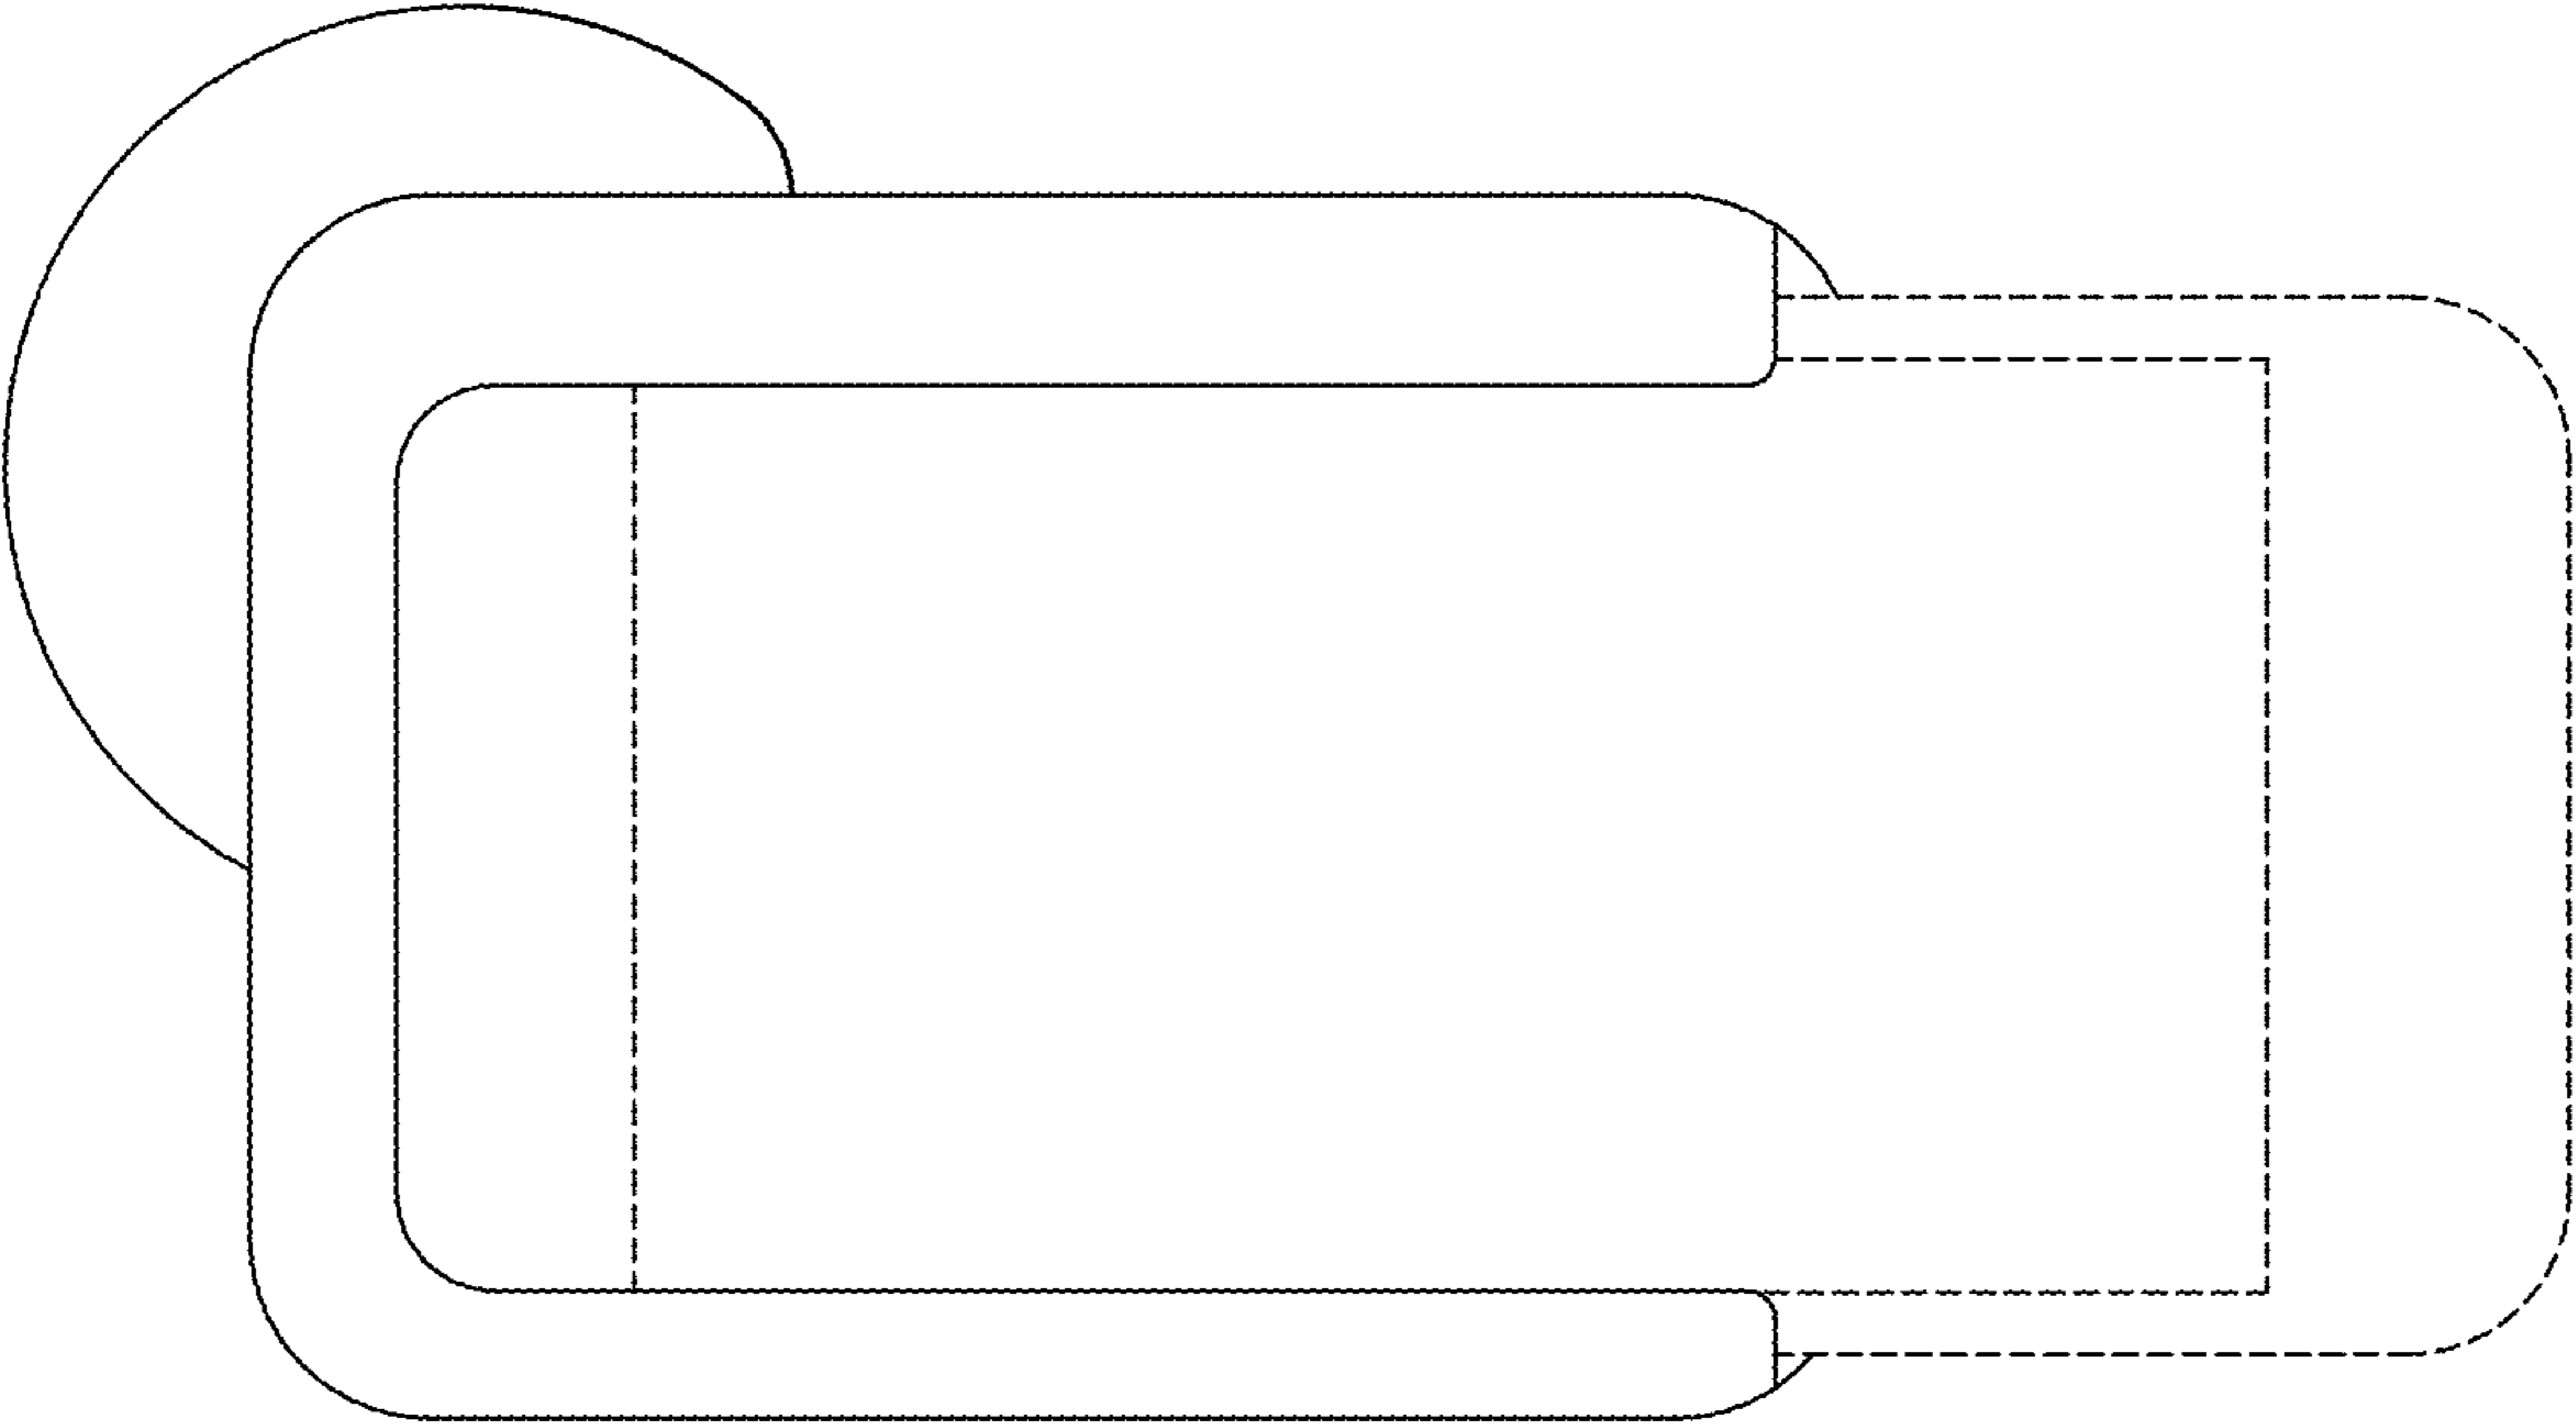


Fig. 2

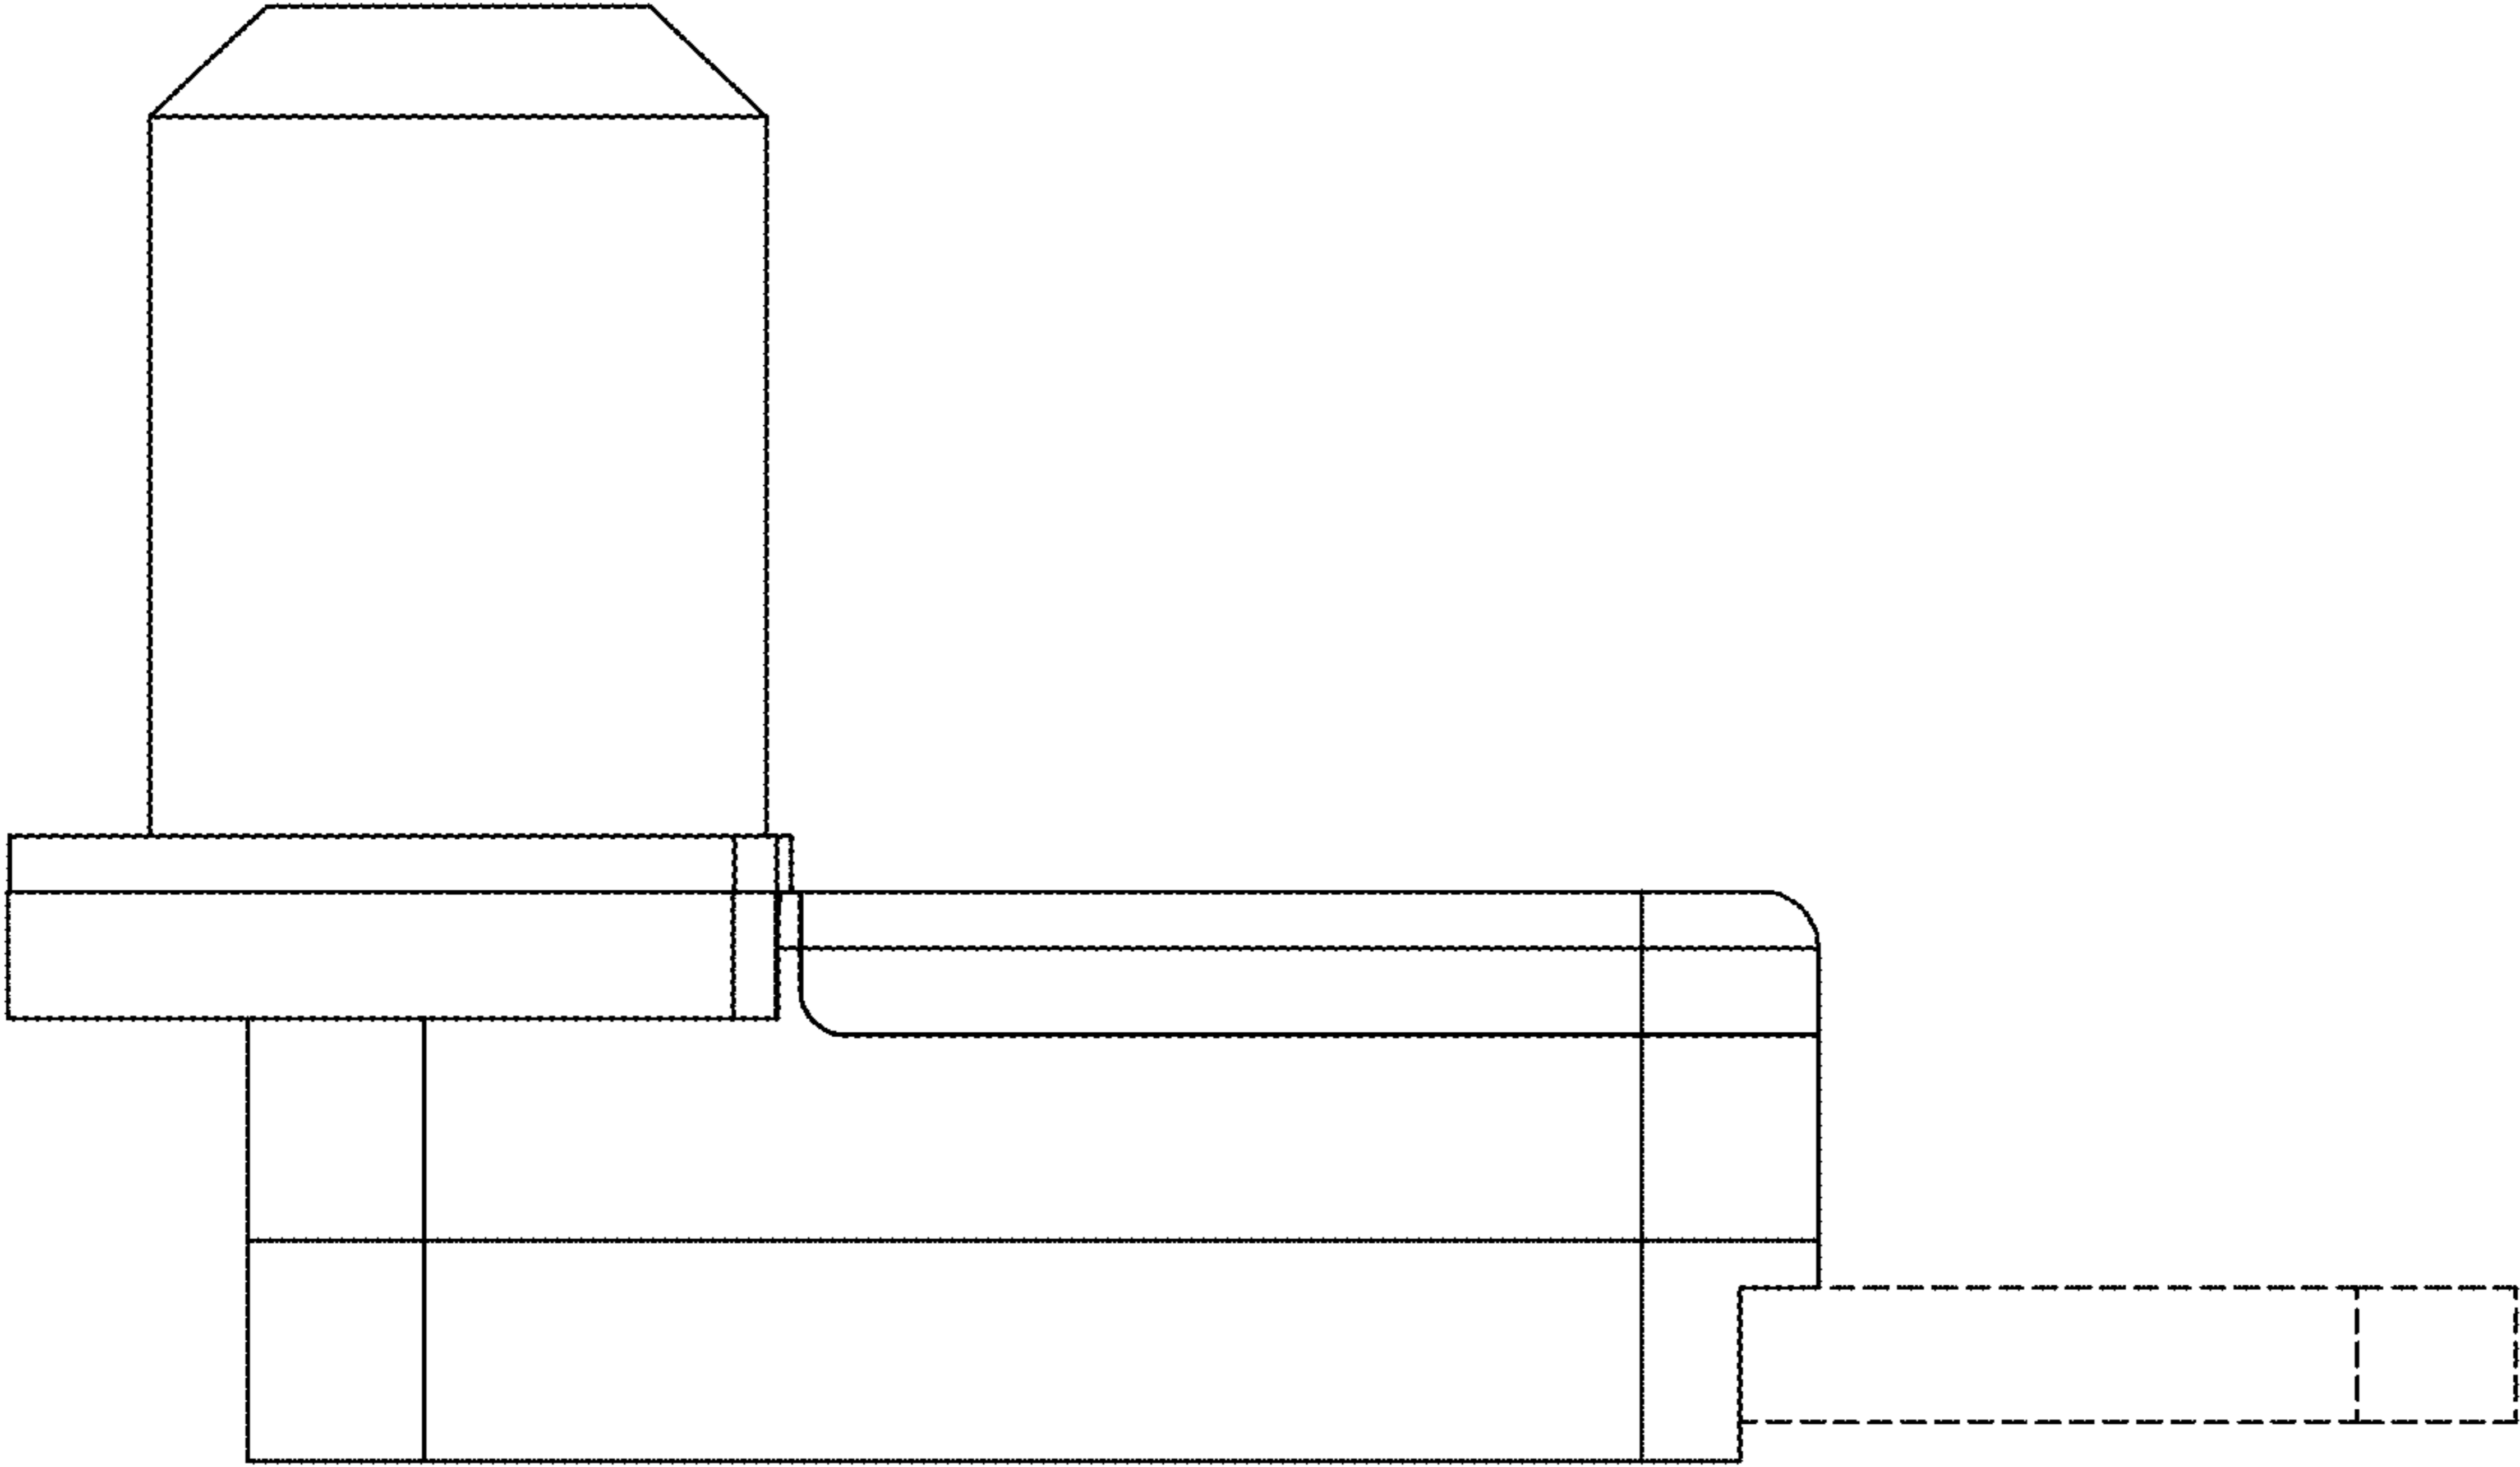


Fig. 3

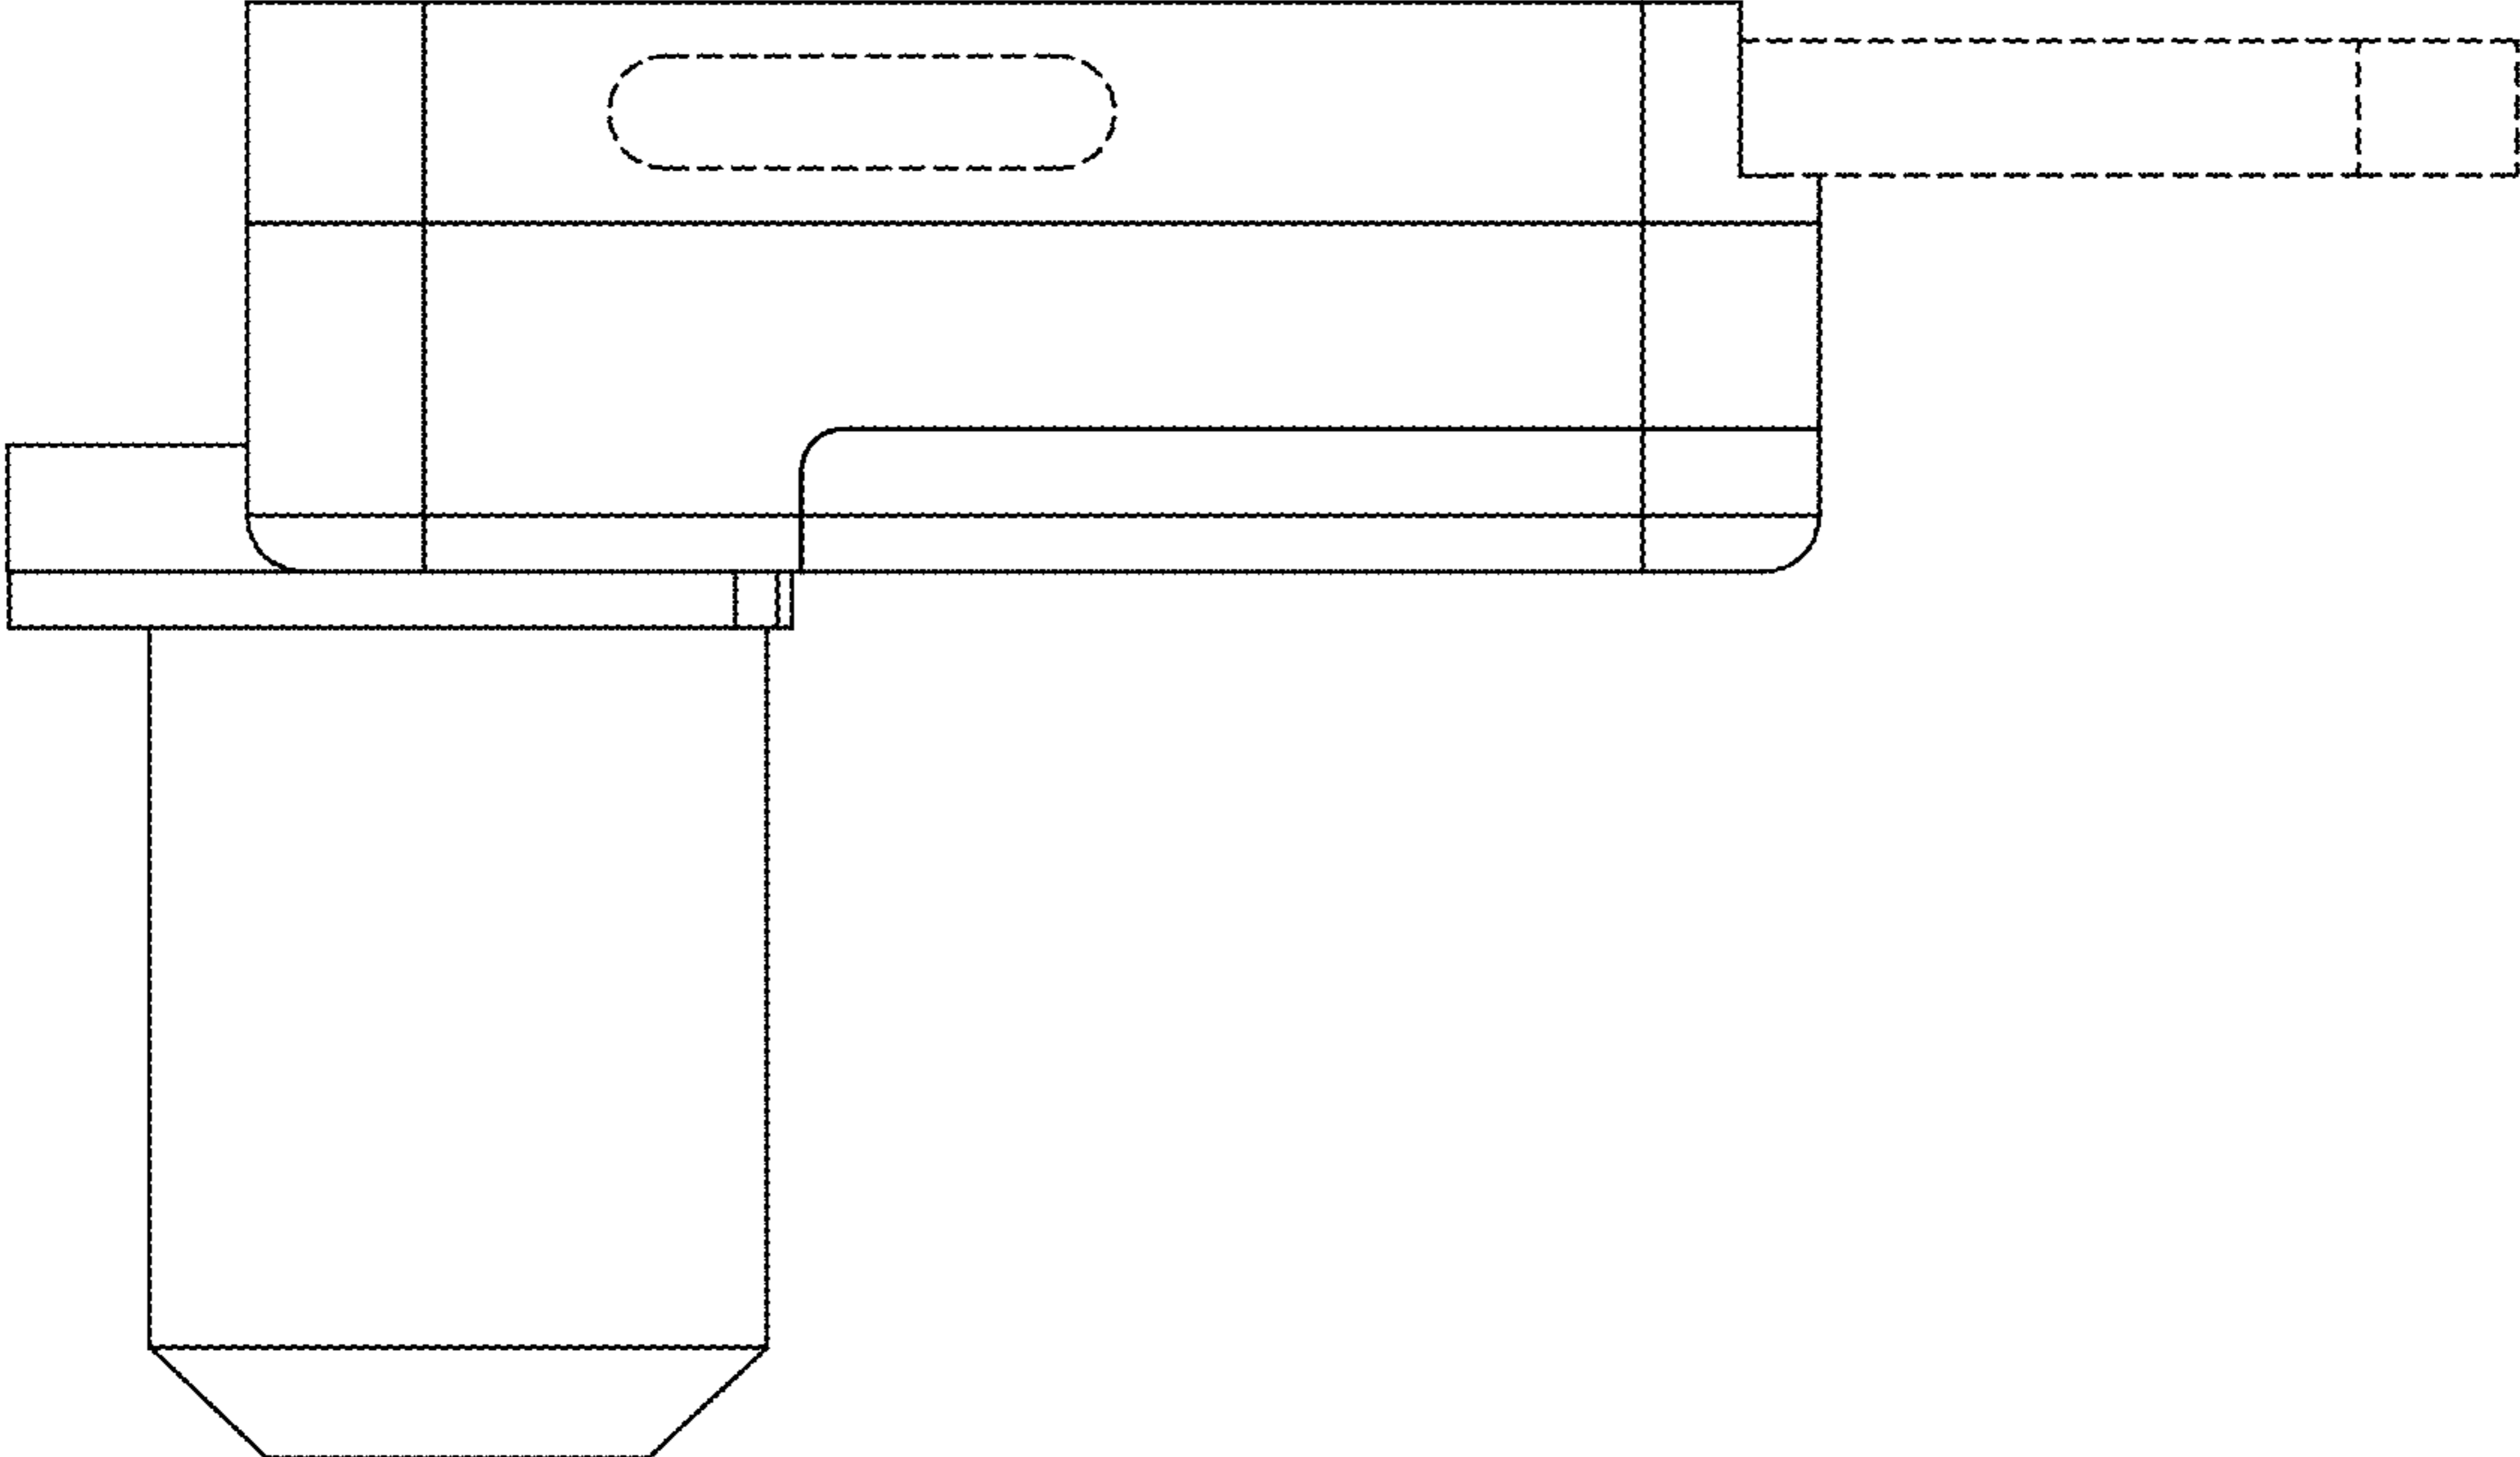


Fig. 4

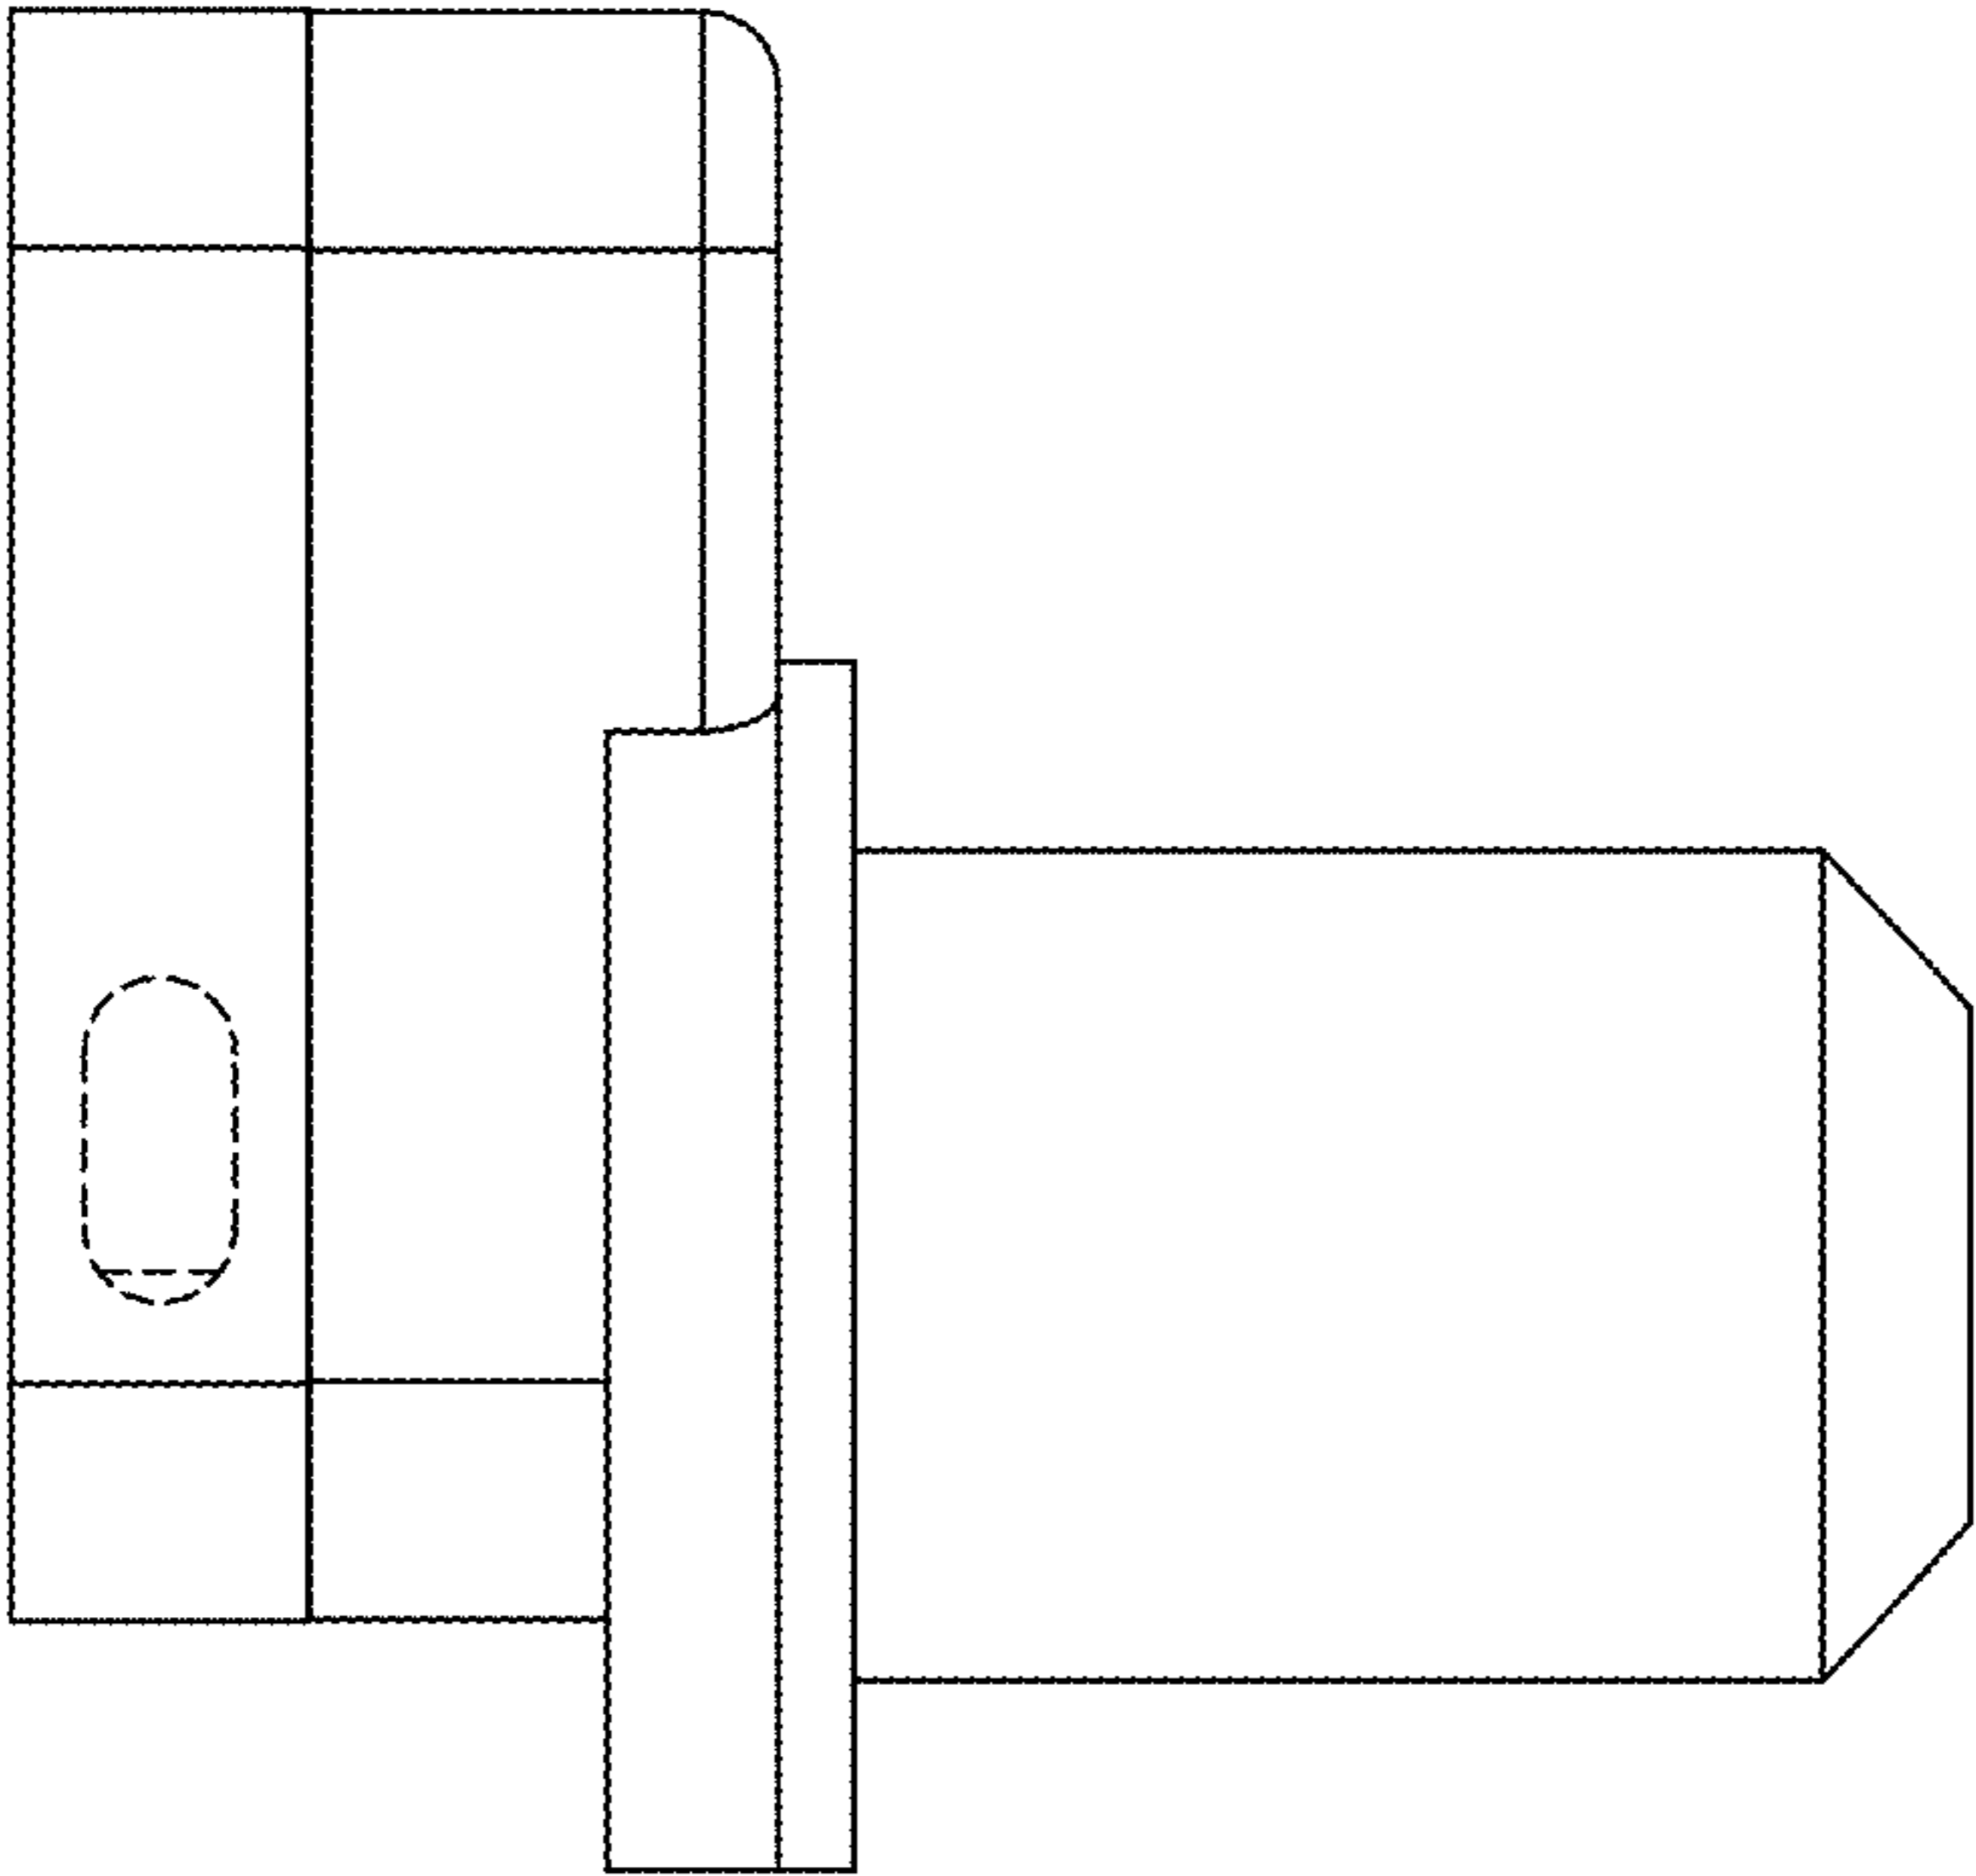


Fig. 5

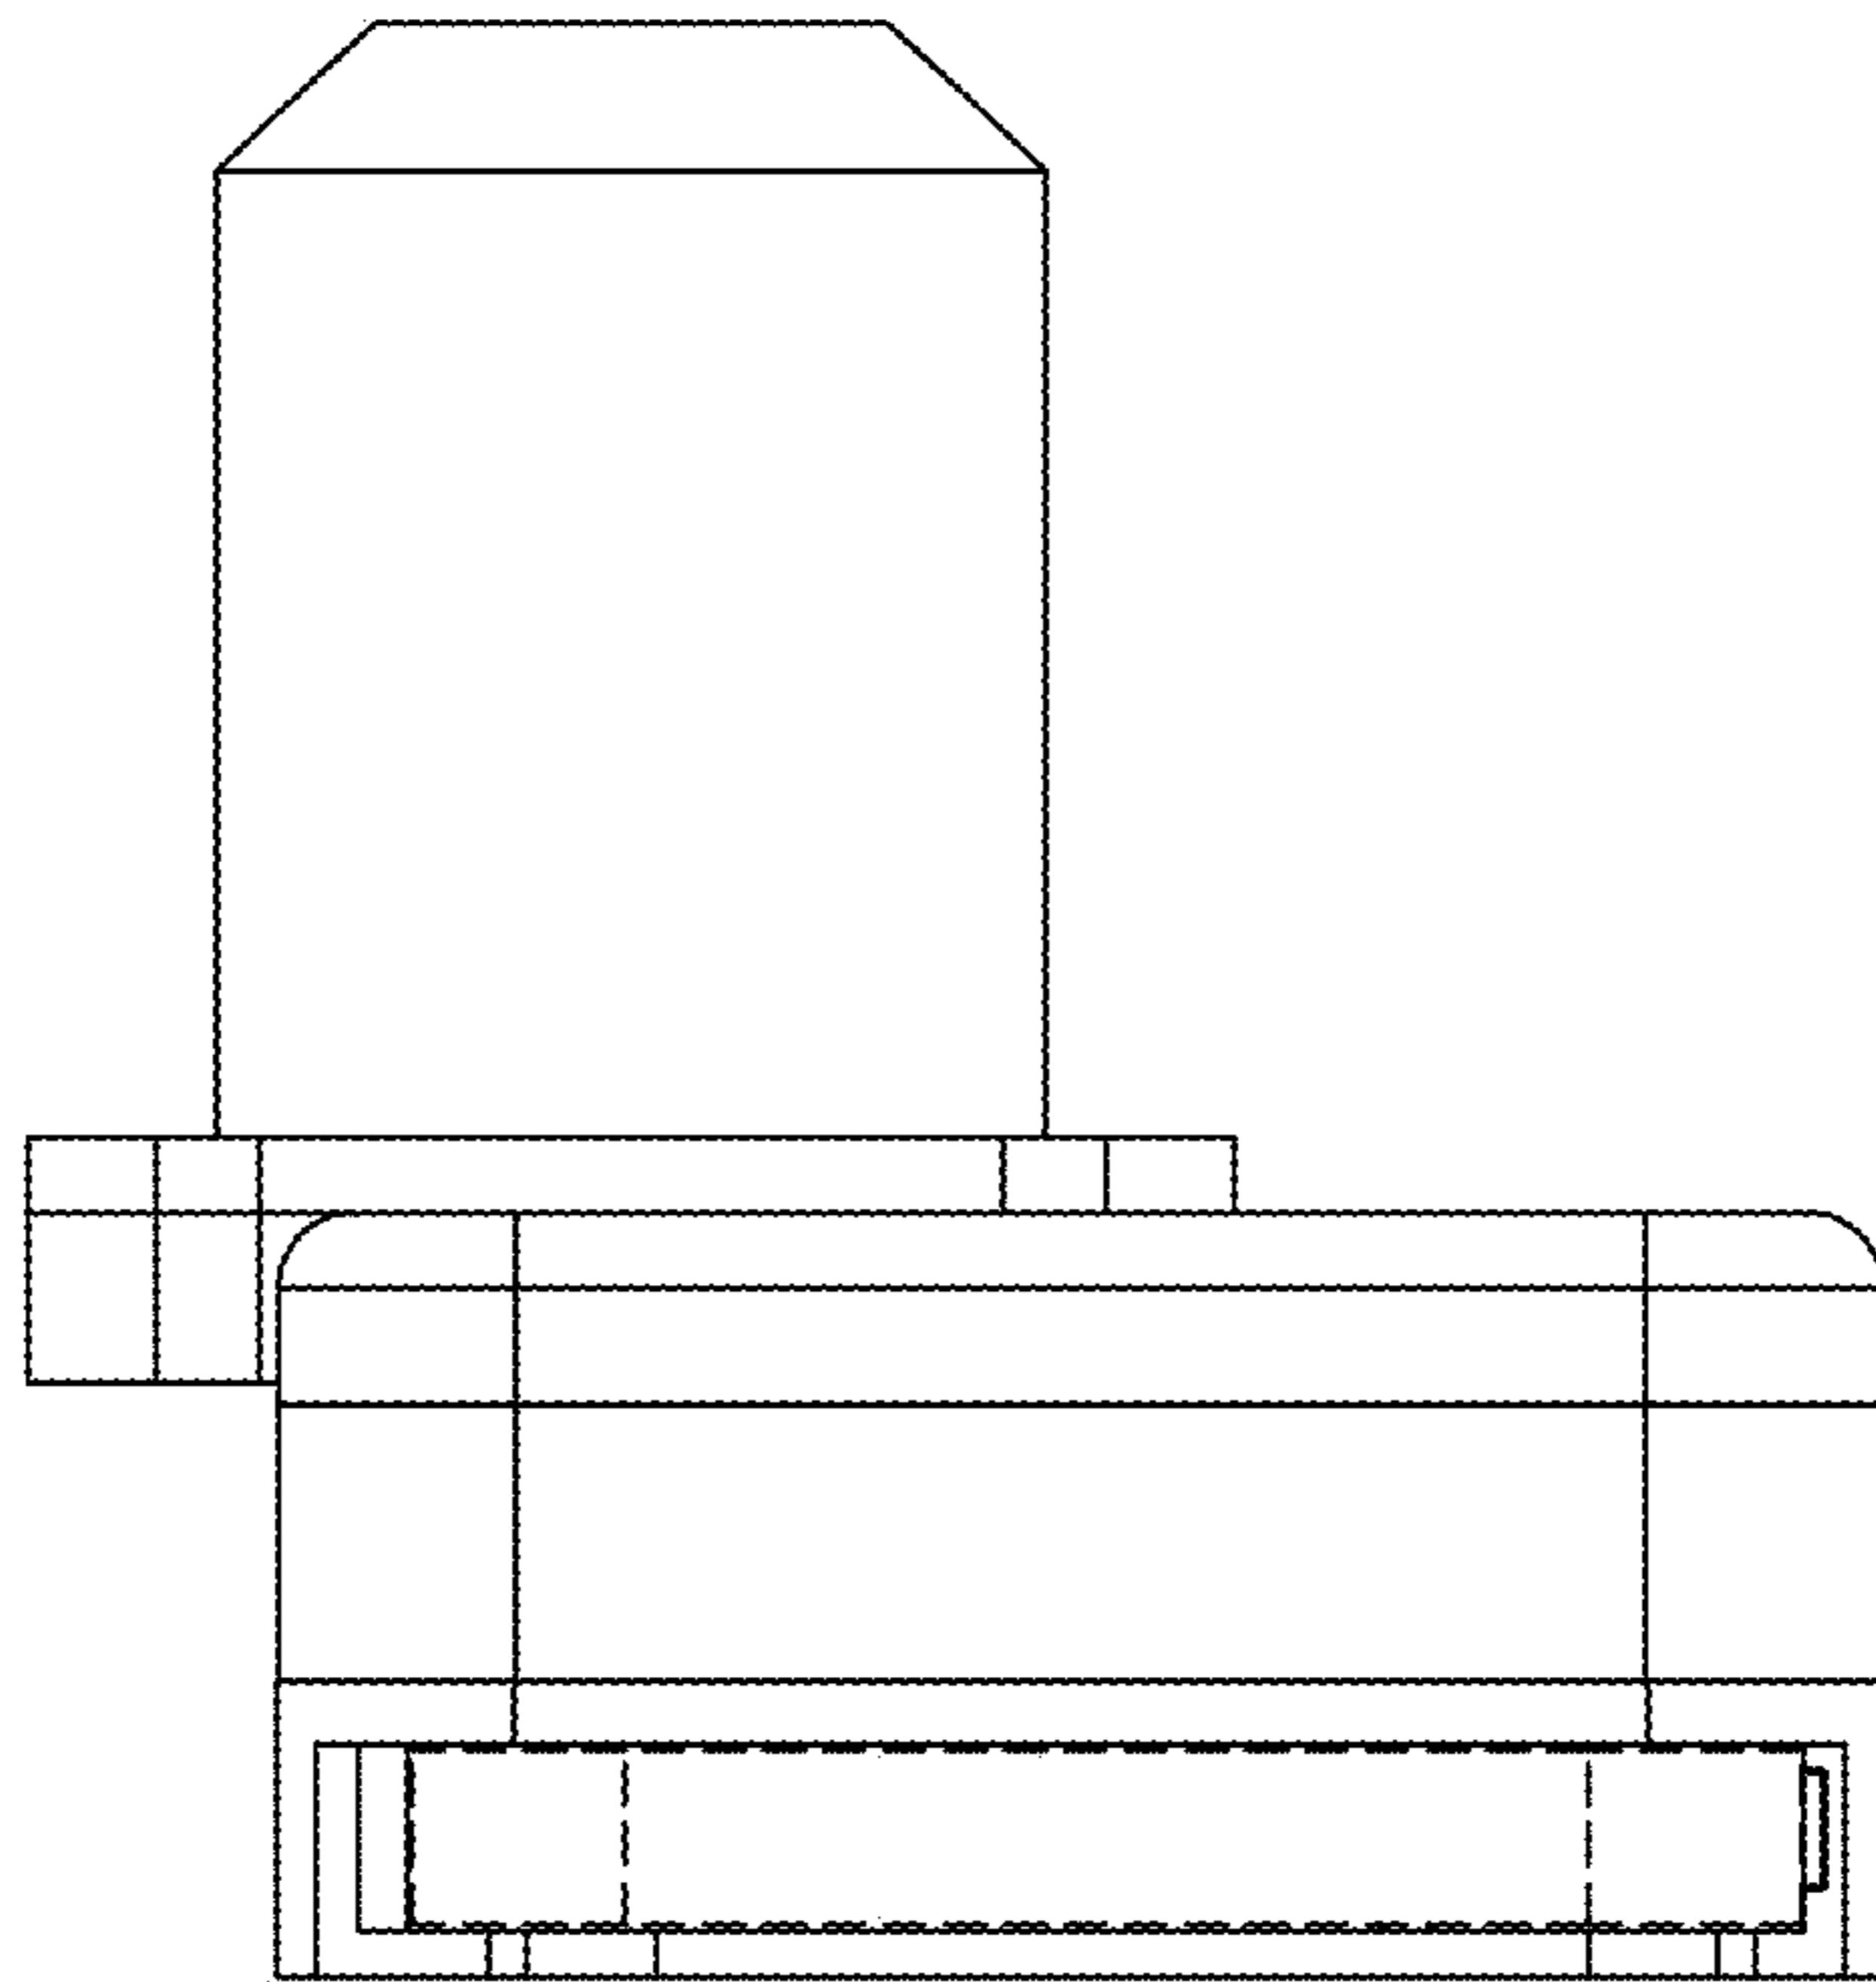


FIG. 6

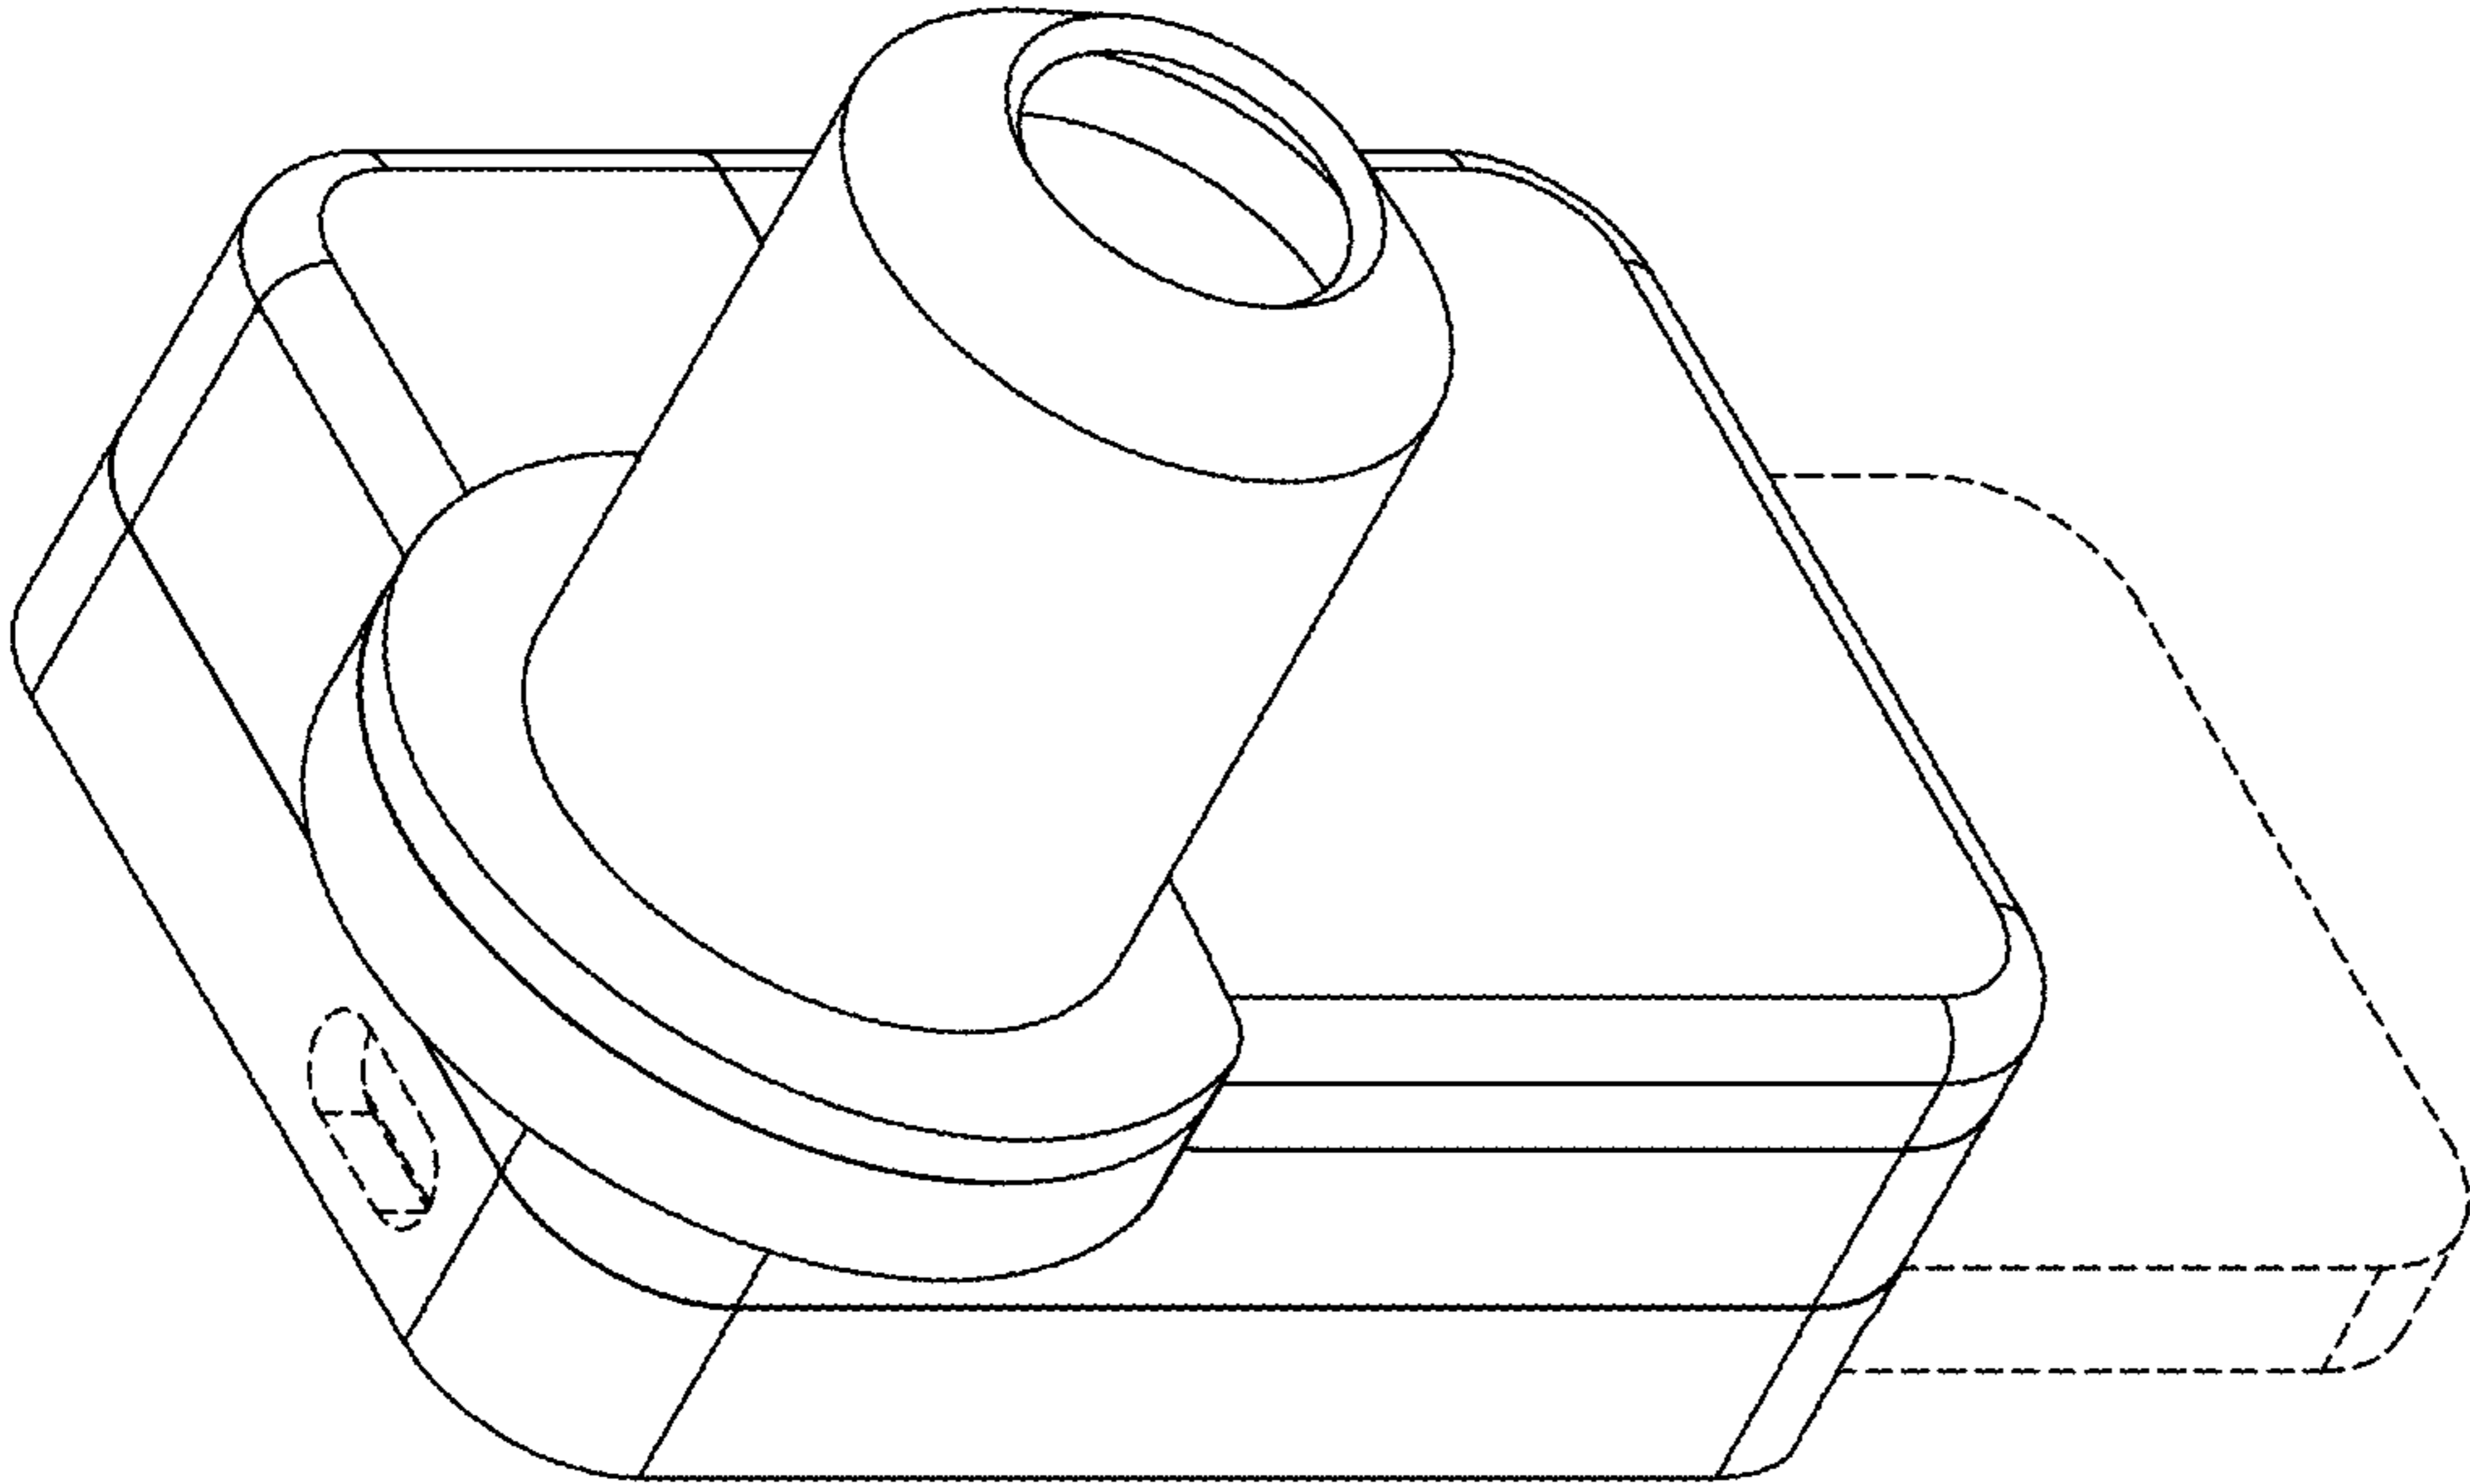


Fig. 7