

US00D940880S

(12) **United States Design Patent** (10) **Patent No.:** **US D940,880 S**
Rondoni et al. (45) **Date of Patent:** **** Jan. 11, 2022**

(54) **PATIENT CONTROL**
(71) Applicant: **Inspire Medical Systems, Inc.**, Golden Valley, MN (US)
(72) Inventors: **John Rondoni**, Golden Valley, MN (US); **Blake D. Johnson**, Golden Valley, MN (US); **Jordan McIver**, Golden Valley, MN (US); **Casimir Sienkiewicz**, Golden Valley, MN (US); **Peter Young**, Golden Valley, MN (US); **Travis Yoch**, Golden Valley, MN (US); **Kevin Verzal**, Golden Valley, MN (US)

D544,605 S 6/2007 Gumisawa et al.
D570,791 S * 6/2008 Takach D13/162
D642,281 S 7/2011 Bachinski
D726,160 S * 4/2015 Chang D14/218
D732,673 S 6/2015 Lewis, Jr. et al.
D748,066 S 1/2016 Lee
D752,763 S 3/2016 Rondoni et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO 9749454 12/1997

OTHER PUBLICATIONS

Inspire Sleep Apnea Innovation—About Inspire Medical Systems, Inc. Testimonial “Diane’s story” dated Sep. 1, 2016.*

(Continued)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Dicke, Billig & Czaja, PLLC

(73) Assignee: **Inspire Medical Systems, Inc.**, Golden Valley, MN (US)
(**) Term: **15 Years**
(21) Appl. No.: **29/688,085**
(22) Filed: **Apr. 18, 2019**

Related U.S. Application Data

(63) Continuation of application No. 29/623,409, filed on Oct. 25, 2017, now Pat. No. Des. 849,252, which is a continuation of application No. 29/548,747, filed on Dec. 16, 2015, now Pat. No. Des. 801,538.

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/186**; D24/200

(58) **Field of Classification Search**
USPC D24/185, 186, 187, 107, 108, 200, 164; D13/162, 164, 168, 171, 218
CPC A61N 1/3611; A61N 1/37247; A61N 1/37235
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,172,698 A 12/1992 Stanko
D490,525 S 5/2004 Stein et al.


(57) **CLAIM**

The ornamental design for a patient control, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, right perspective view of a patient control;
FIG. 2 is a top plan view thereof;
FIG. 3 is a bottom plan view thereof;
FIG. 4 is a front elevational view thereof;
FIG. 5 is a back elevational view thereof;
FIG. 6 is a right side elevational view thereof; and,
FIG. 7 is a left side elevational view thereof.
The broken lines in the Figures are included for the purpose of illustrating portions of the patient control that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

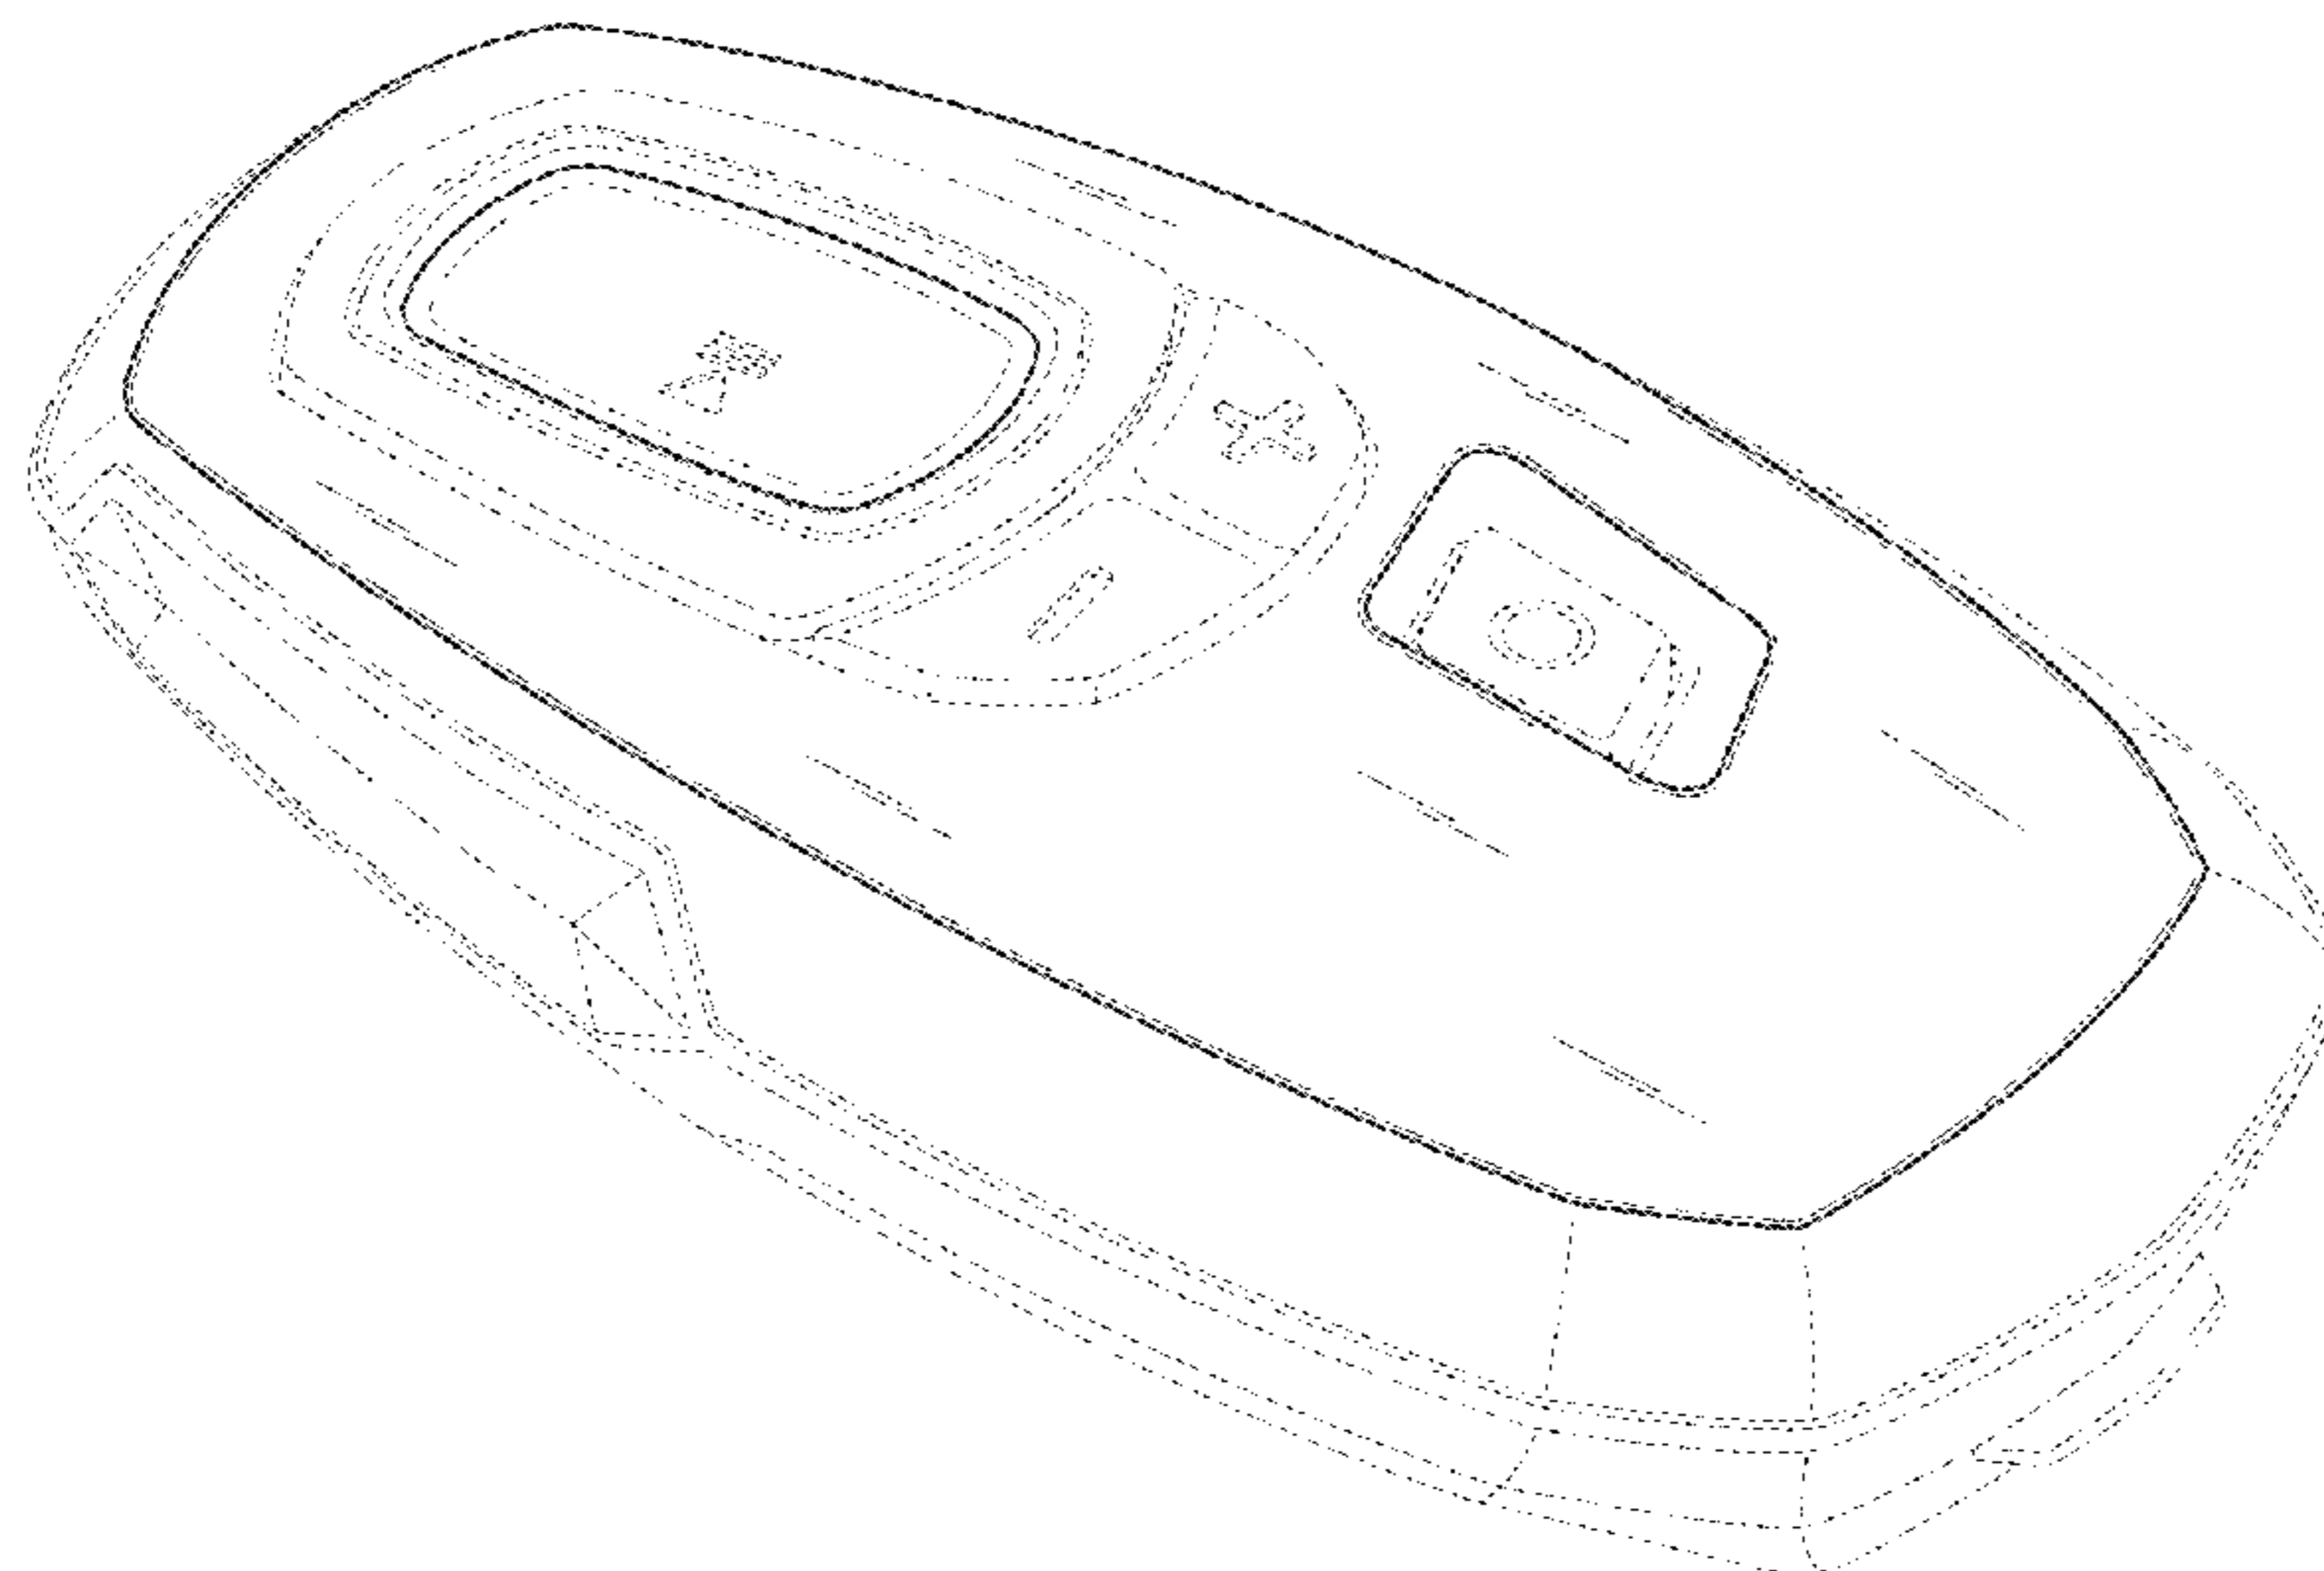

(56)

References Cited

U.S. PATENT DOCUMENTS

D768,866	S	10/2016	Shigeno	
D774,007	S	12/2016	Ryan	
D786,770	S *	5/2017	Smallhorn D12/345
D788,017	S *	5/2017	Smallhorn D12/345
D797,949	S	9/2017	Carreon et al.	
D801,538	S *	10/2017	Rondoni D24/186
D810,306	S	2/2018	Rondoni et al.	
D849,252	S	5/2019	Rondoni et al.	
2004/0230246	A1	11/2004	Stein et al.	
2007/0270921	A1	11/2007	Strother et al.	
2008/0249591	A1	10/2008	Gaw et al.	
2010/0064212	A1	3/2010	Snyder	
2010/0318159	A1	12/2010	Aghassian et al.	
2010/0318519	A1	12/2010	Hadjieleftheriou et al.	
2012/0101551	A1	4/2012	Aghassian et al.	
2013/0197607	A1	8/2013	Wilder et al.	
2013/0204314	A1	8/2013	Miller, III et al.	

OTHER PUBLICATIONS

Inspire Sleep Apnea Innovation—Testimonials. The “Diane’s story” dated Sep. 1, 2016.*
Partial International Search Report, dated Dec. 3, 2014, 6 pages.

* cited by examiner

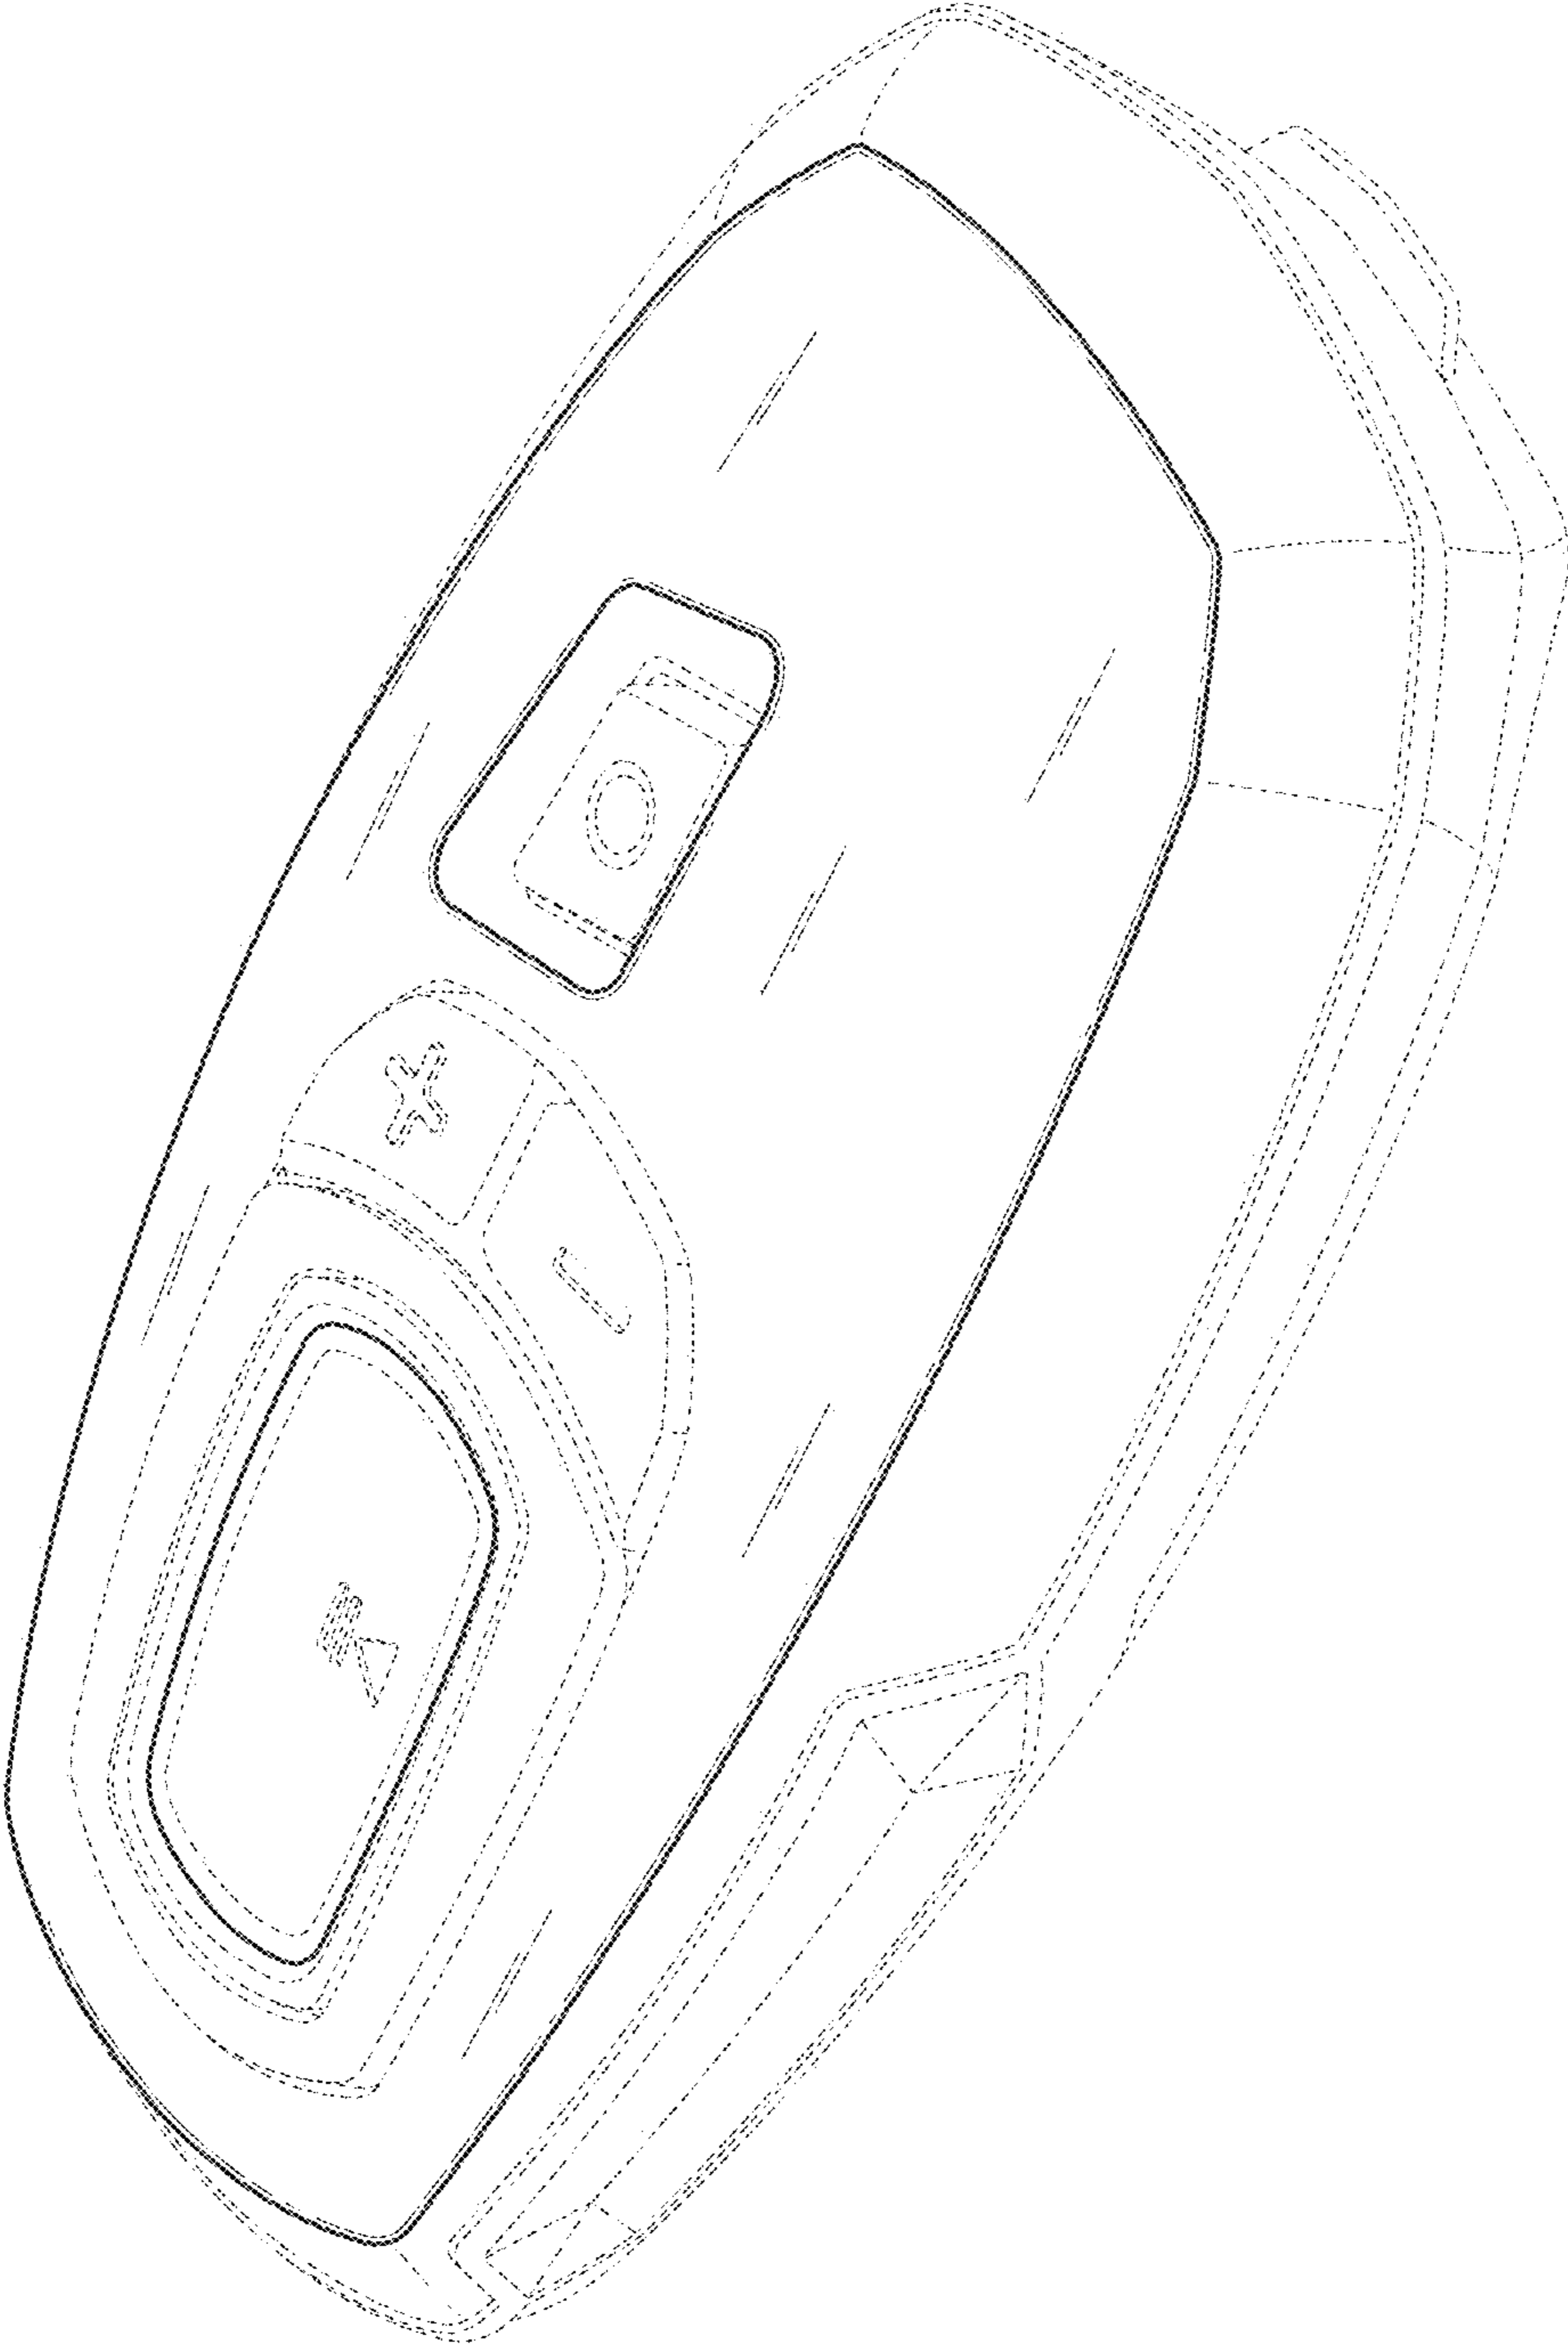


Fig. 1

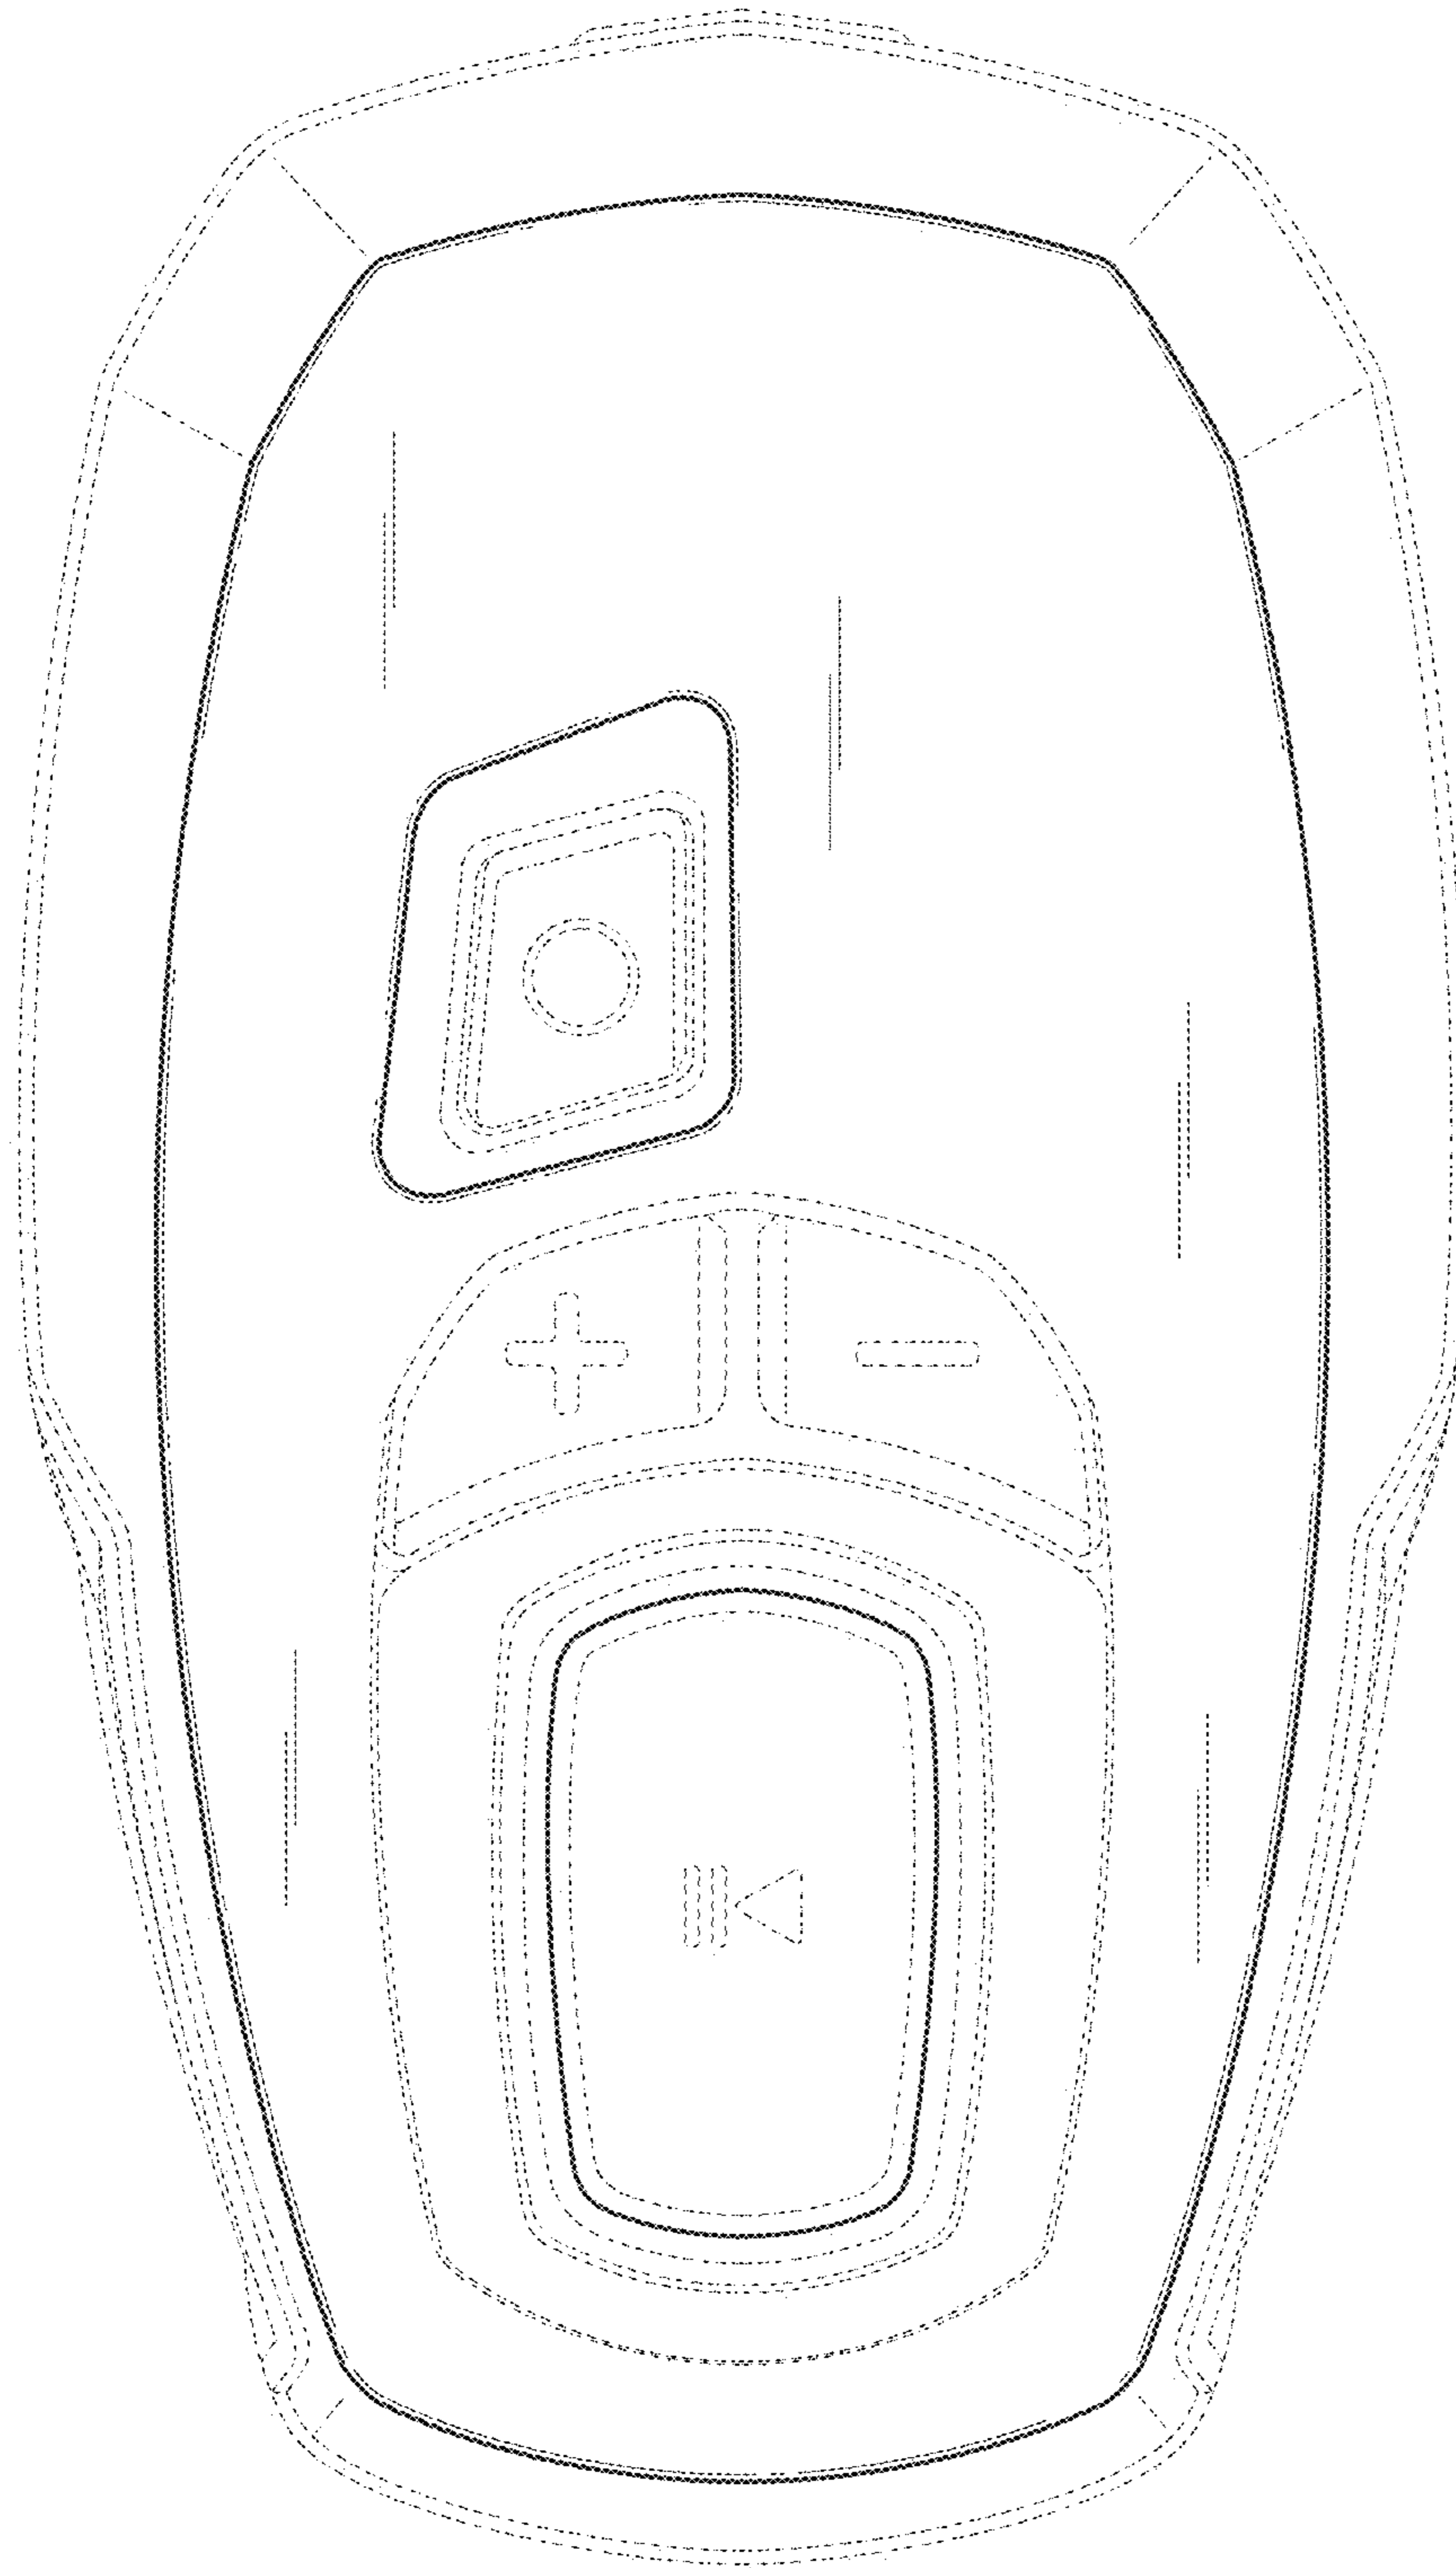


Fig. 2

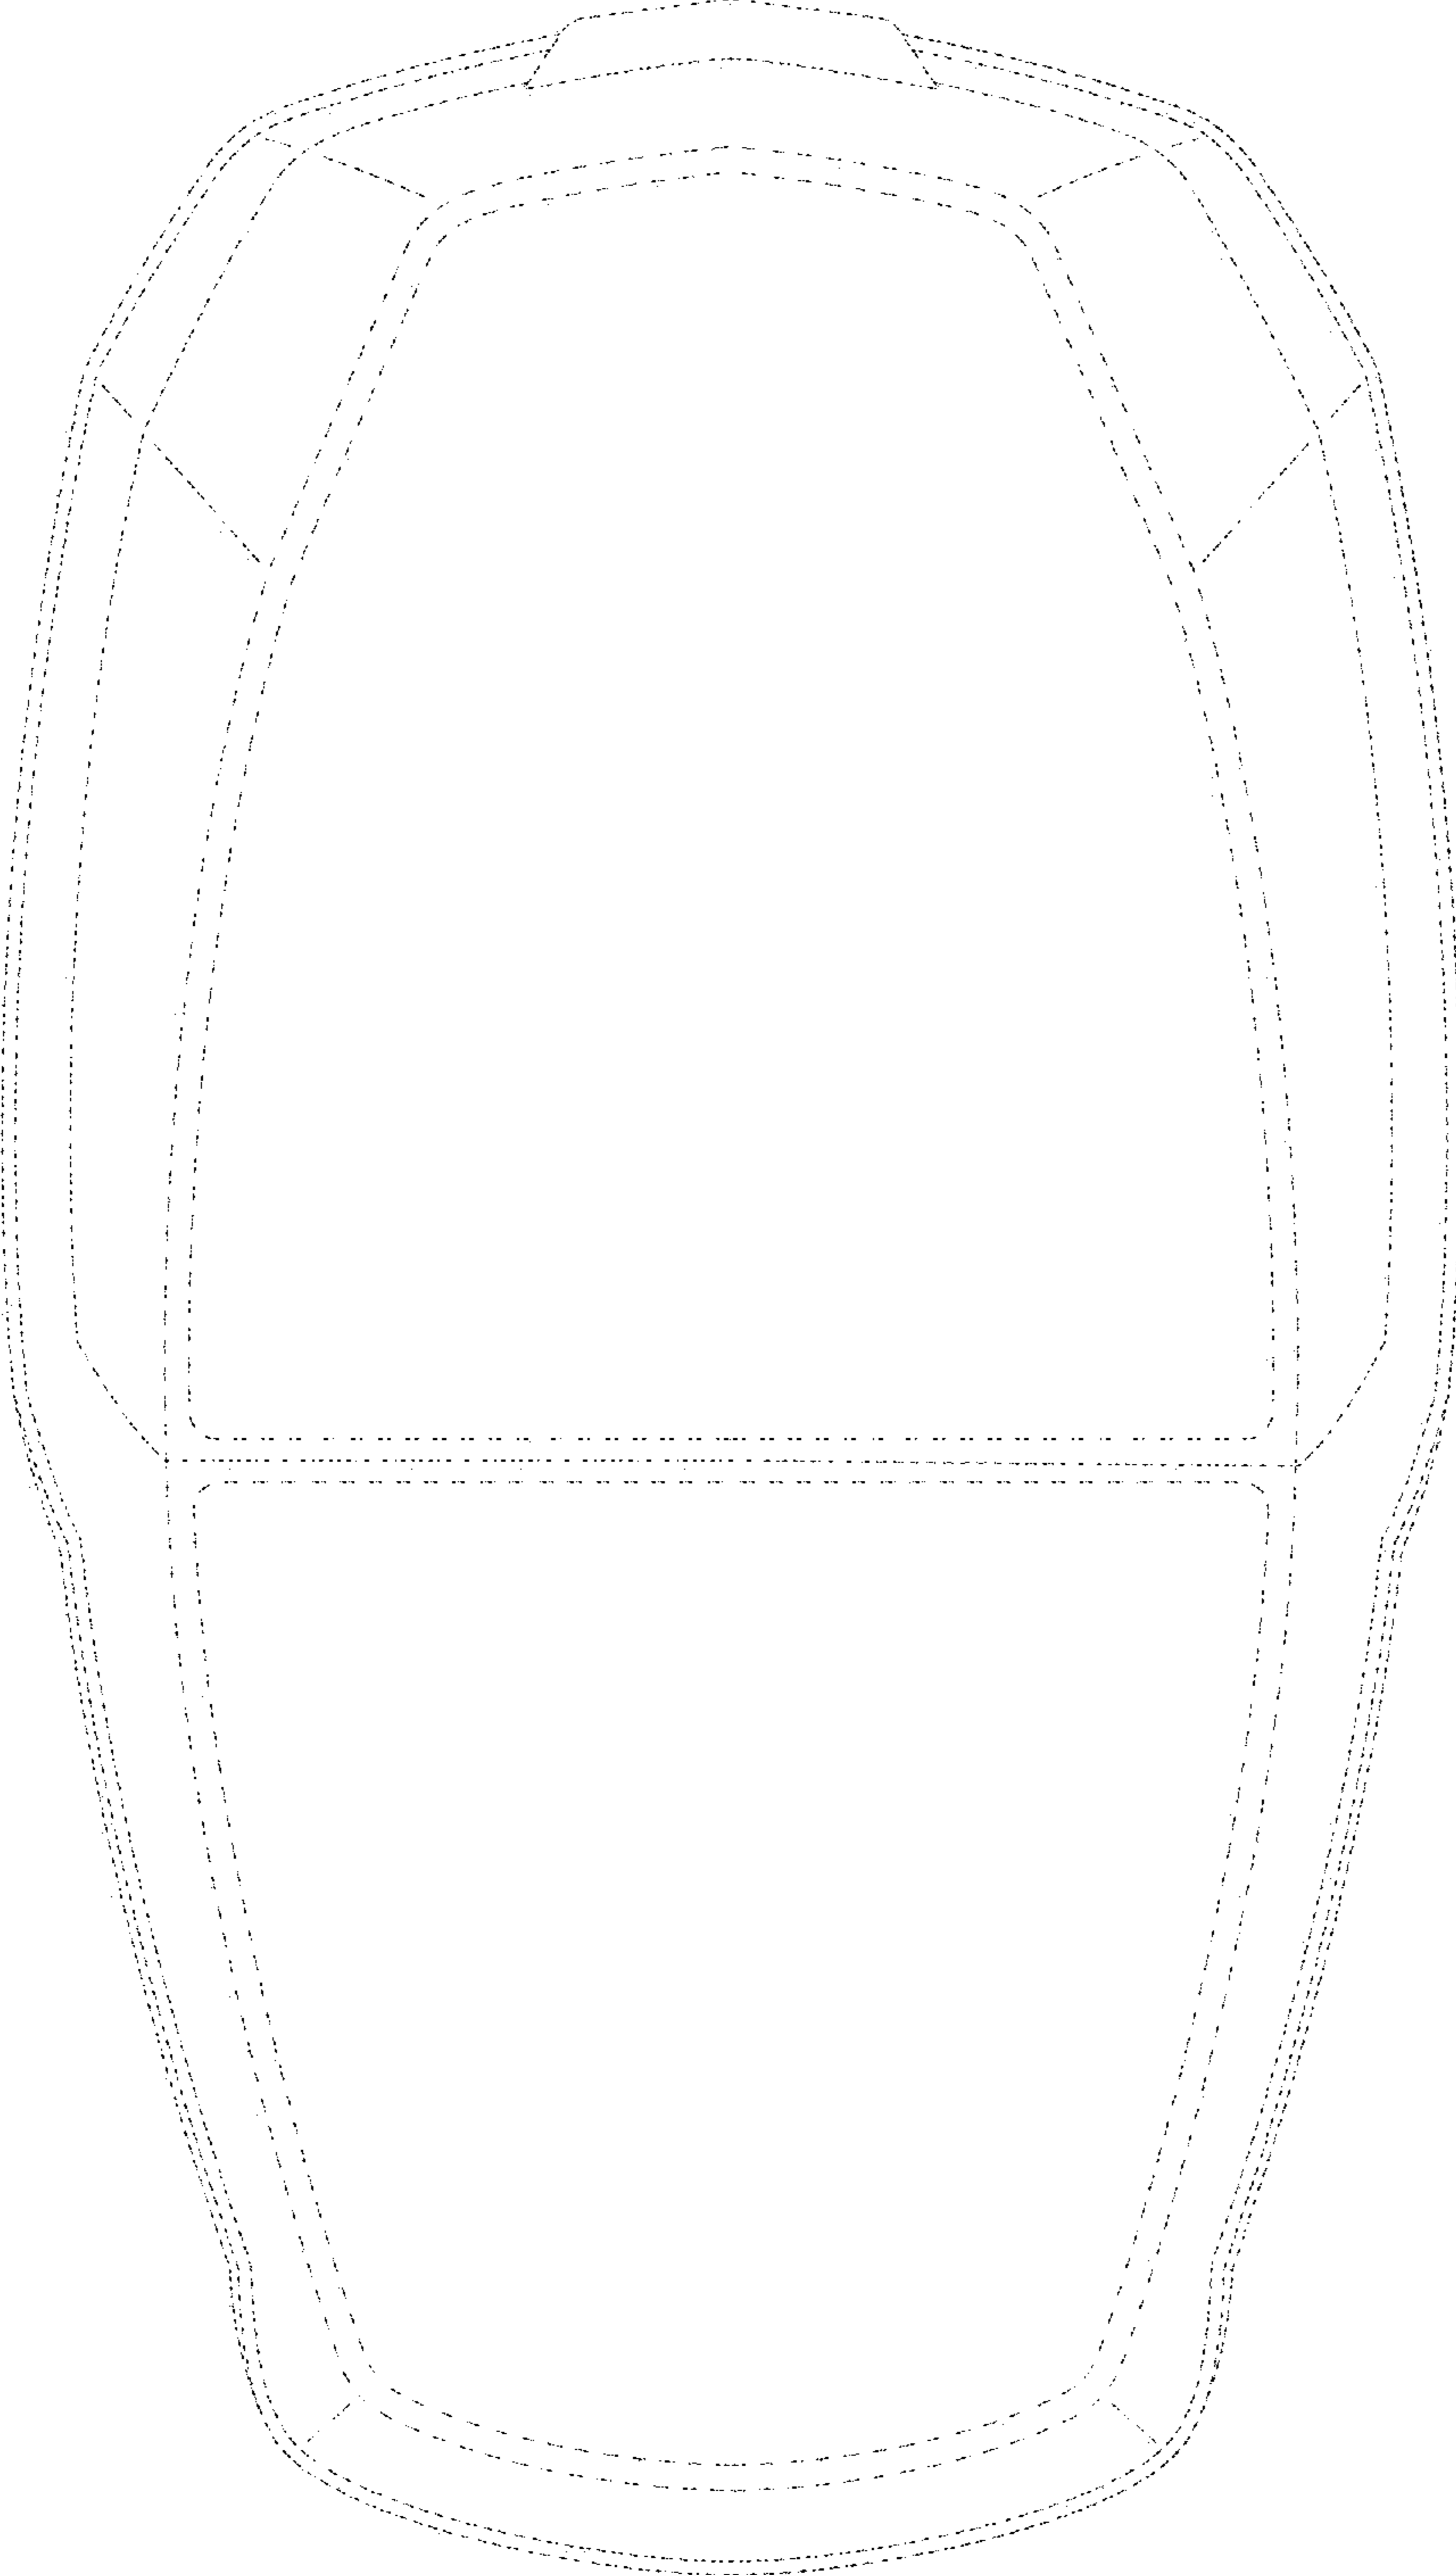


Fig. 3

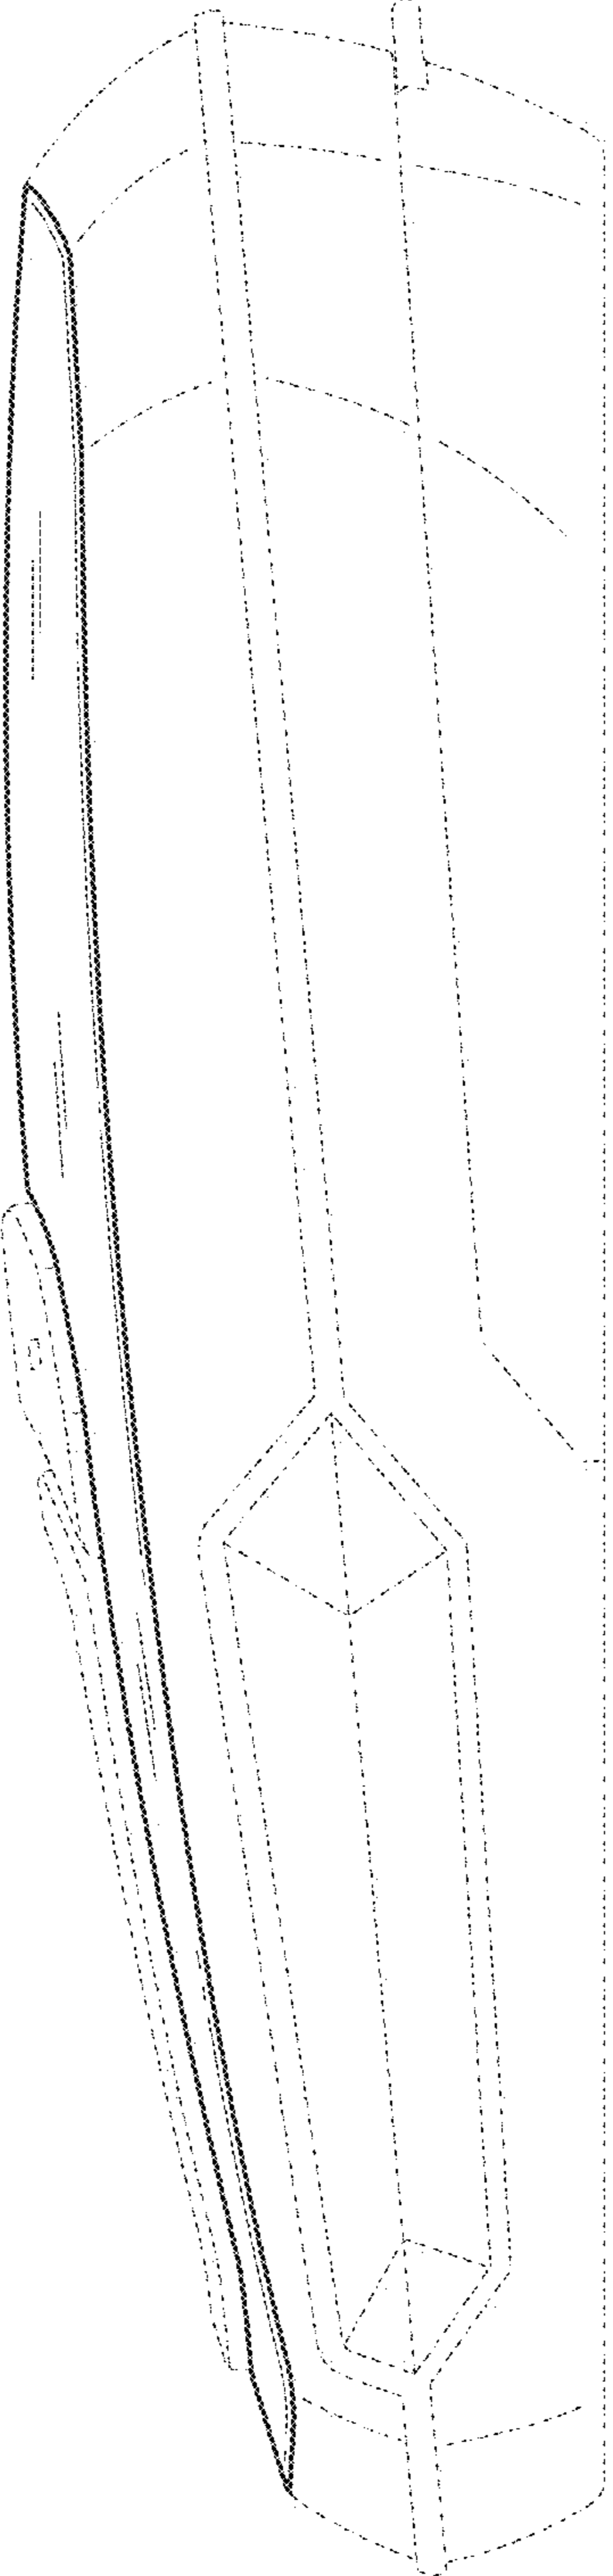


Fig. 4

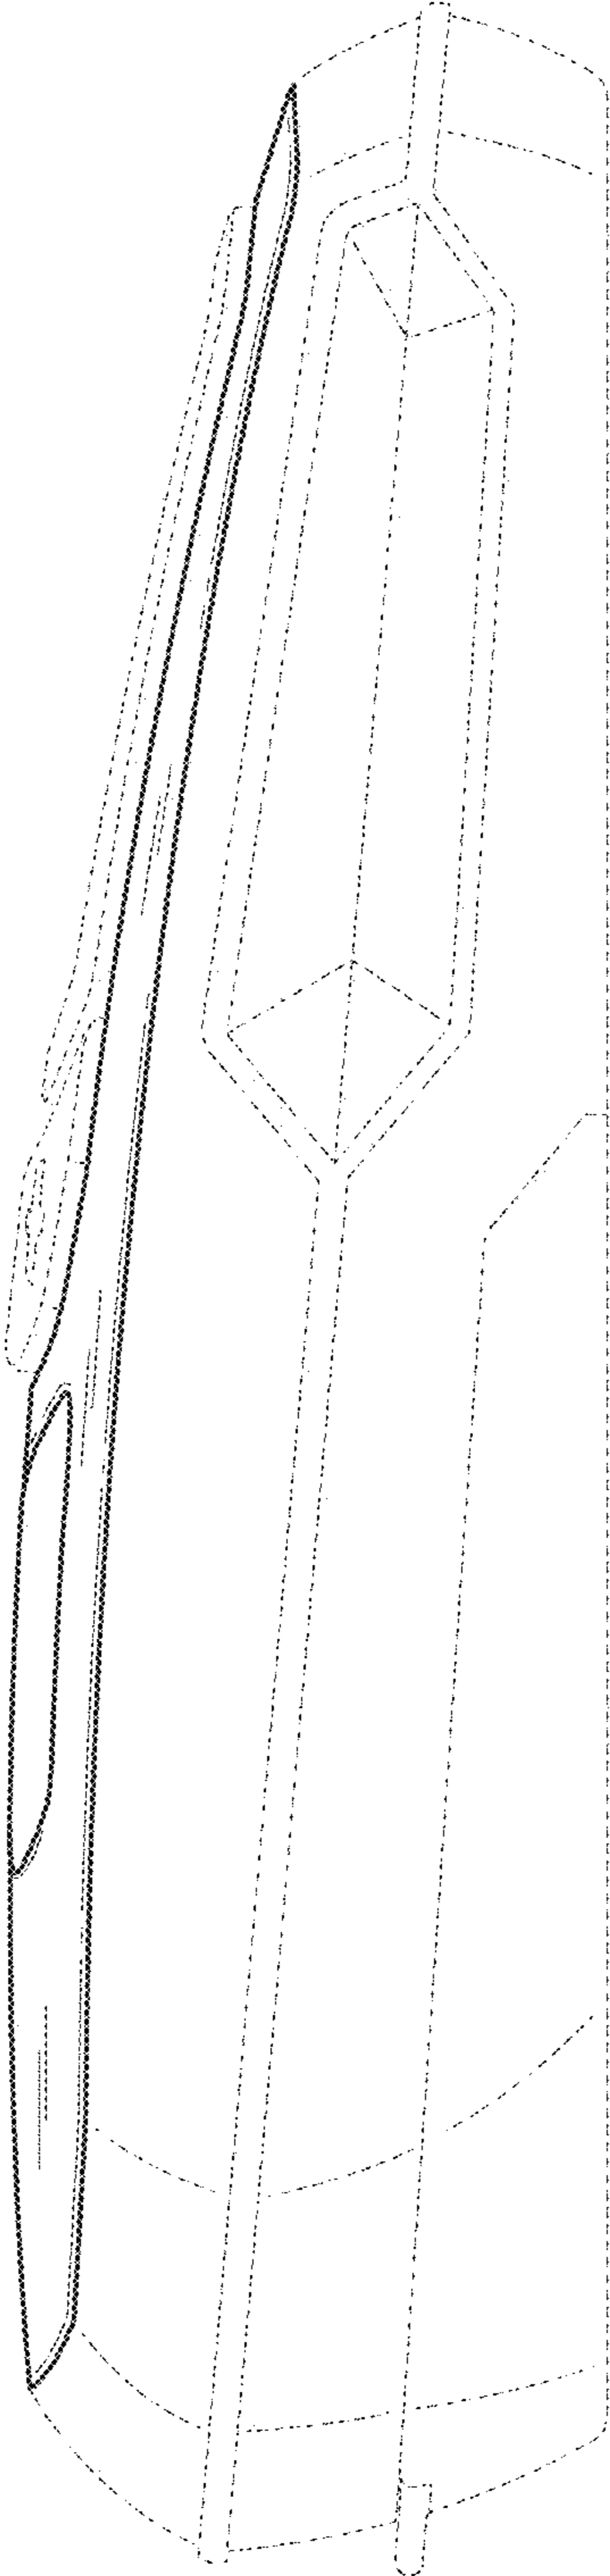


Fig. 5

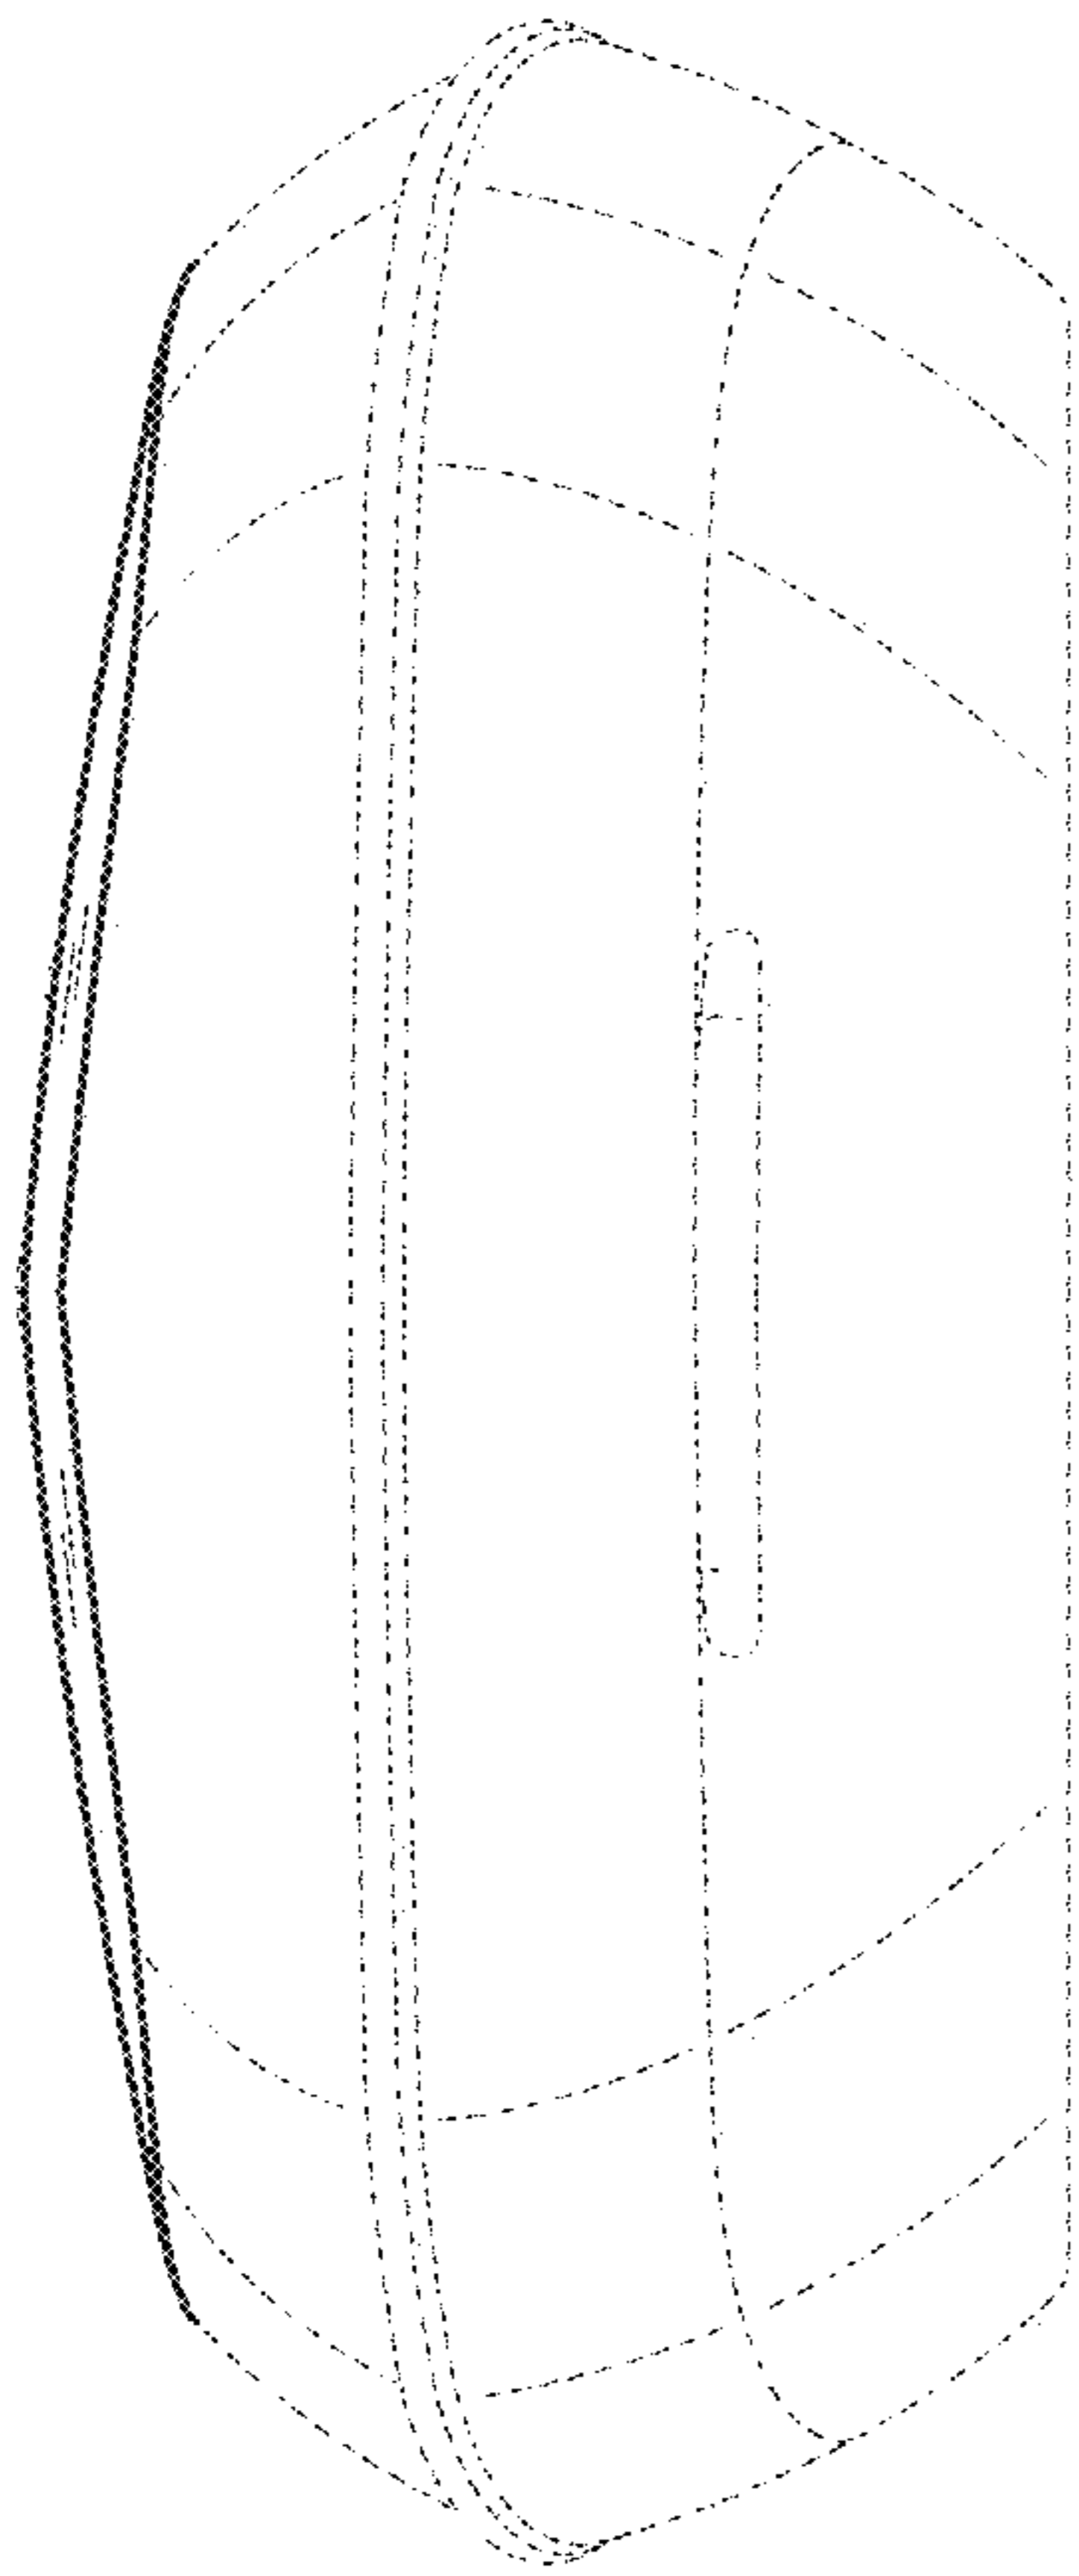


Fig. 6

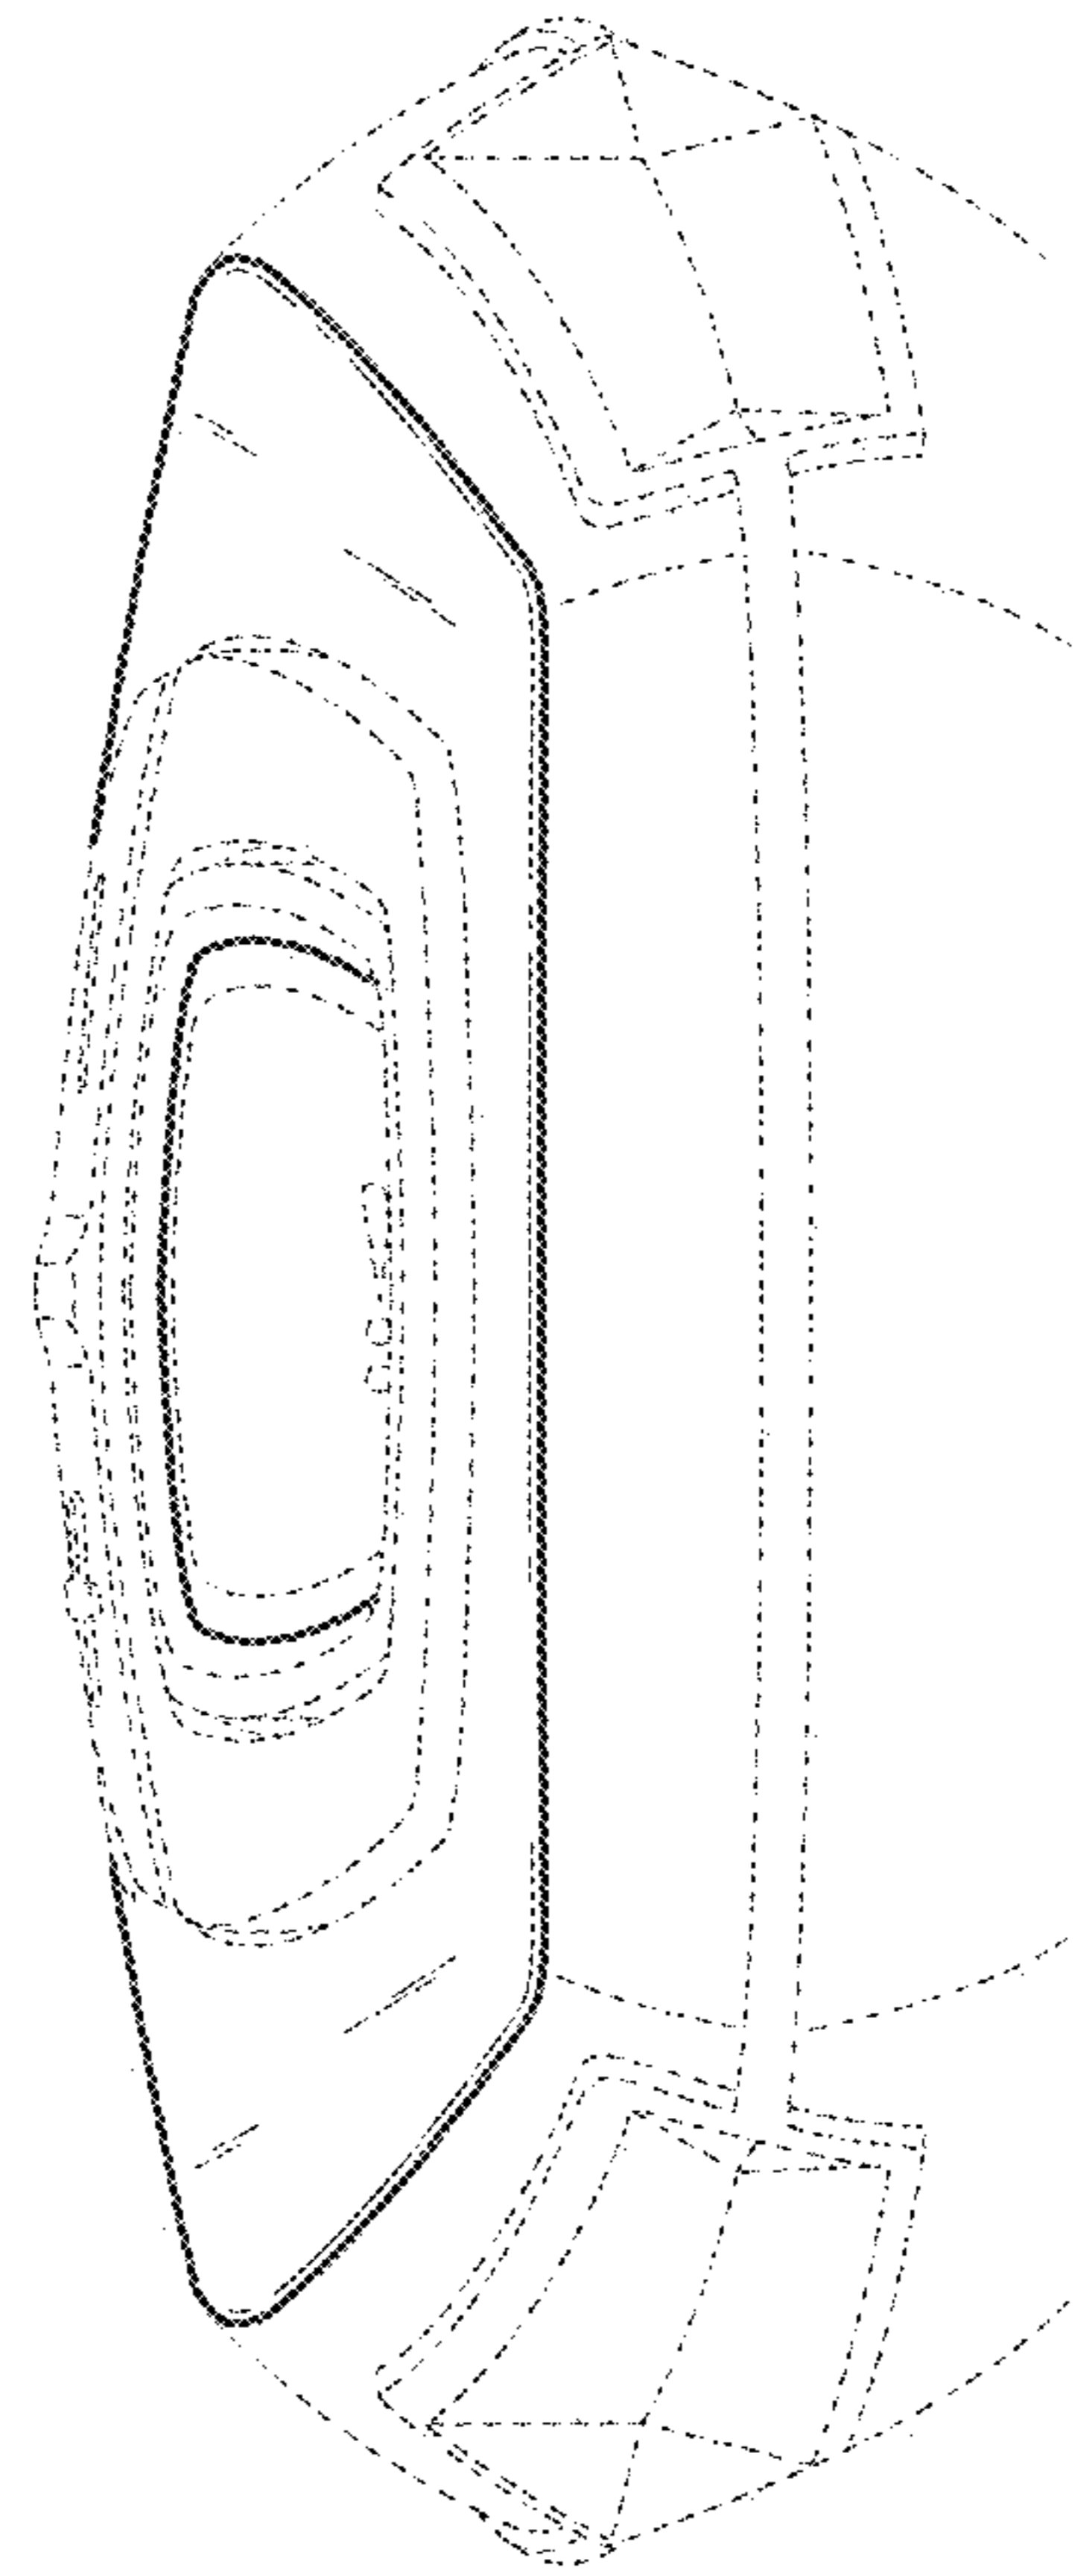


Fig. 7