



US00D941328S

(12) **United States Design Patent**
Balter et al.

(10) **Patent No.:** **US D941,328 S**
(45) **Date of Patent:** **** Jan. 18, 2022**

(54) **DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE**

(71) Applicant: **Fresenius Medical Care Holdings, Inc.**, Waltham, MA (US)

(72) Inventors: **Paul Balter**, River Forest, IL (US);
Linda Ficociello, Littleton, MA (US);
Christina Rossi, Concord, MA (US)

(73) Assignee: **Fresenius Medical Care Holdings, Inc.**, Waltham, MA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/728,817**

(22) Filed: **Mar. 20, 2020**

Related U.S. Application Data

(63) Continuation-in-part of application No. 16/730,749, filed on Dec. 30, 2019.

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**

USPC D14/485-495; D20/11; D21/324, 325
CPC G06F 3/048; G06F 3/0481; G06F 3/04817;
G06F 3/0482; G06F 3/0483; G06F 3/04842; G06F 3/0485; G06F 3/04855;
G06F 3/0486; G06F 3/0488; G06F 3/04886; G06F 9/4443; G06F 17/211;
G06F 17/212; G06F 9/451; G06F 40/103; G06F 40/106; G06F 40/189; G06F 40/191; H04L 41/0213; A61M 1/16; A61M 1/30; G16H 20/17; G16H 40/63

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D420,340 S * 2/2000 Bailer D14/486
6,381,635 B1 * 4/2002 Hoyer H04L 41/0213
707/999.01

D467,252 S * 12/2002 Lee D14/486
7,248,263 B2 * 7/2007 Freeman G06T 11/206
345/440
7,974,983 B2 * 7/2011 Goeldi G06Q 30/0251
707/769
D694,252 S * 11/2013 Helm D14/485
8,856,668 B2 * 10/2014 Niesslein G16H 20/17
715/764
D717,328 S * 11/2014 Lin D14/486
D732,053 S * 6/2015 Tomita D14/486
9,155,823 B2 * 10/2015 Tarn A61M 1/16

(Continued)

OTHER PUBLICATIONS

“2008T Hemodialysis Machine with CLiC Device” 2015, posted at fmcna.com, [site visited Jun. 8, 2021]. https://fmcna.com/content/dam/fmcna/live/support/documents/fluid-management/clic/CLiC_TraintheTrainer.pdf (Year: 2015).*

(Continued)

Primary Examiner — John M Otte

(74) *Attorney, Agent, or Firm* — Leydig, Voit & Mayer, Ltd.


(57) **CLAIM**

The ornamental design for a display screen with graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a display screen with graphical user interface showing our new design; FIG. 2 is a second embodiment thereof; and, FIG. 3 is a third embodiment thereof. The broken line showing portions of the graphical user interface in FIG. 1 form part of the claimed design. Broken lines showing portions of the graphical user interface in FIG. 2-3 form no part of the claimed design.

1 Claim, 3 Drawing Sheets

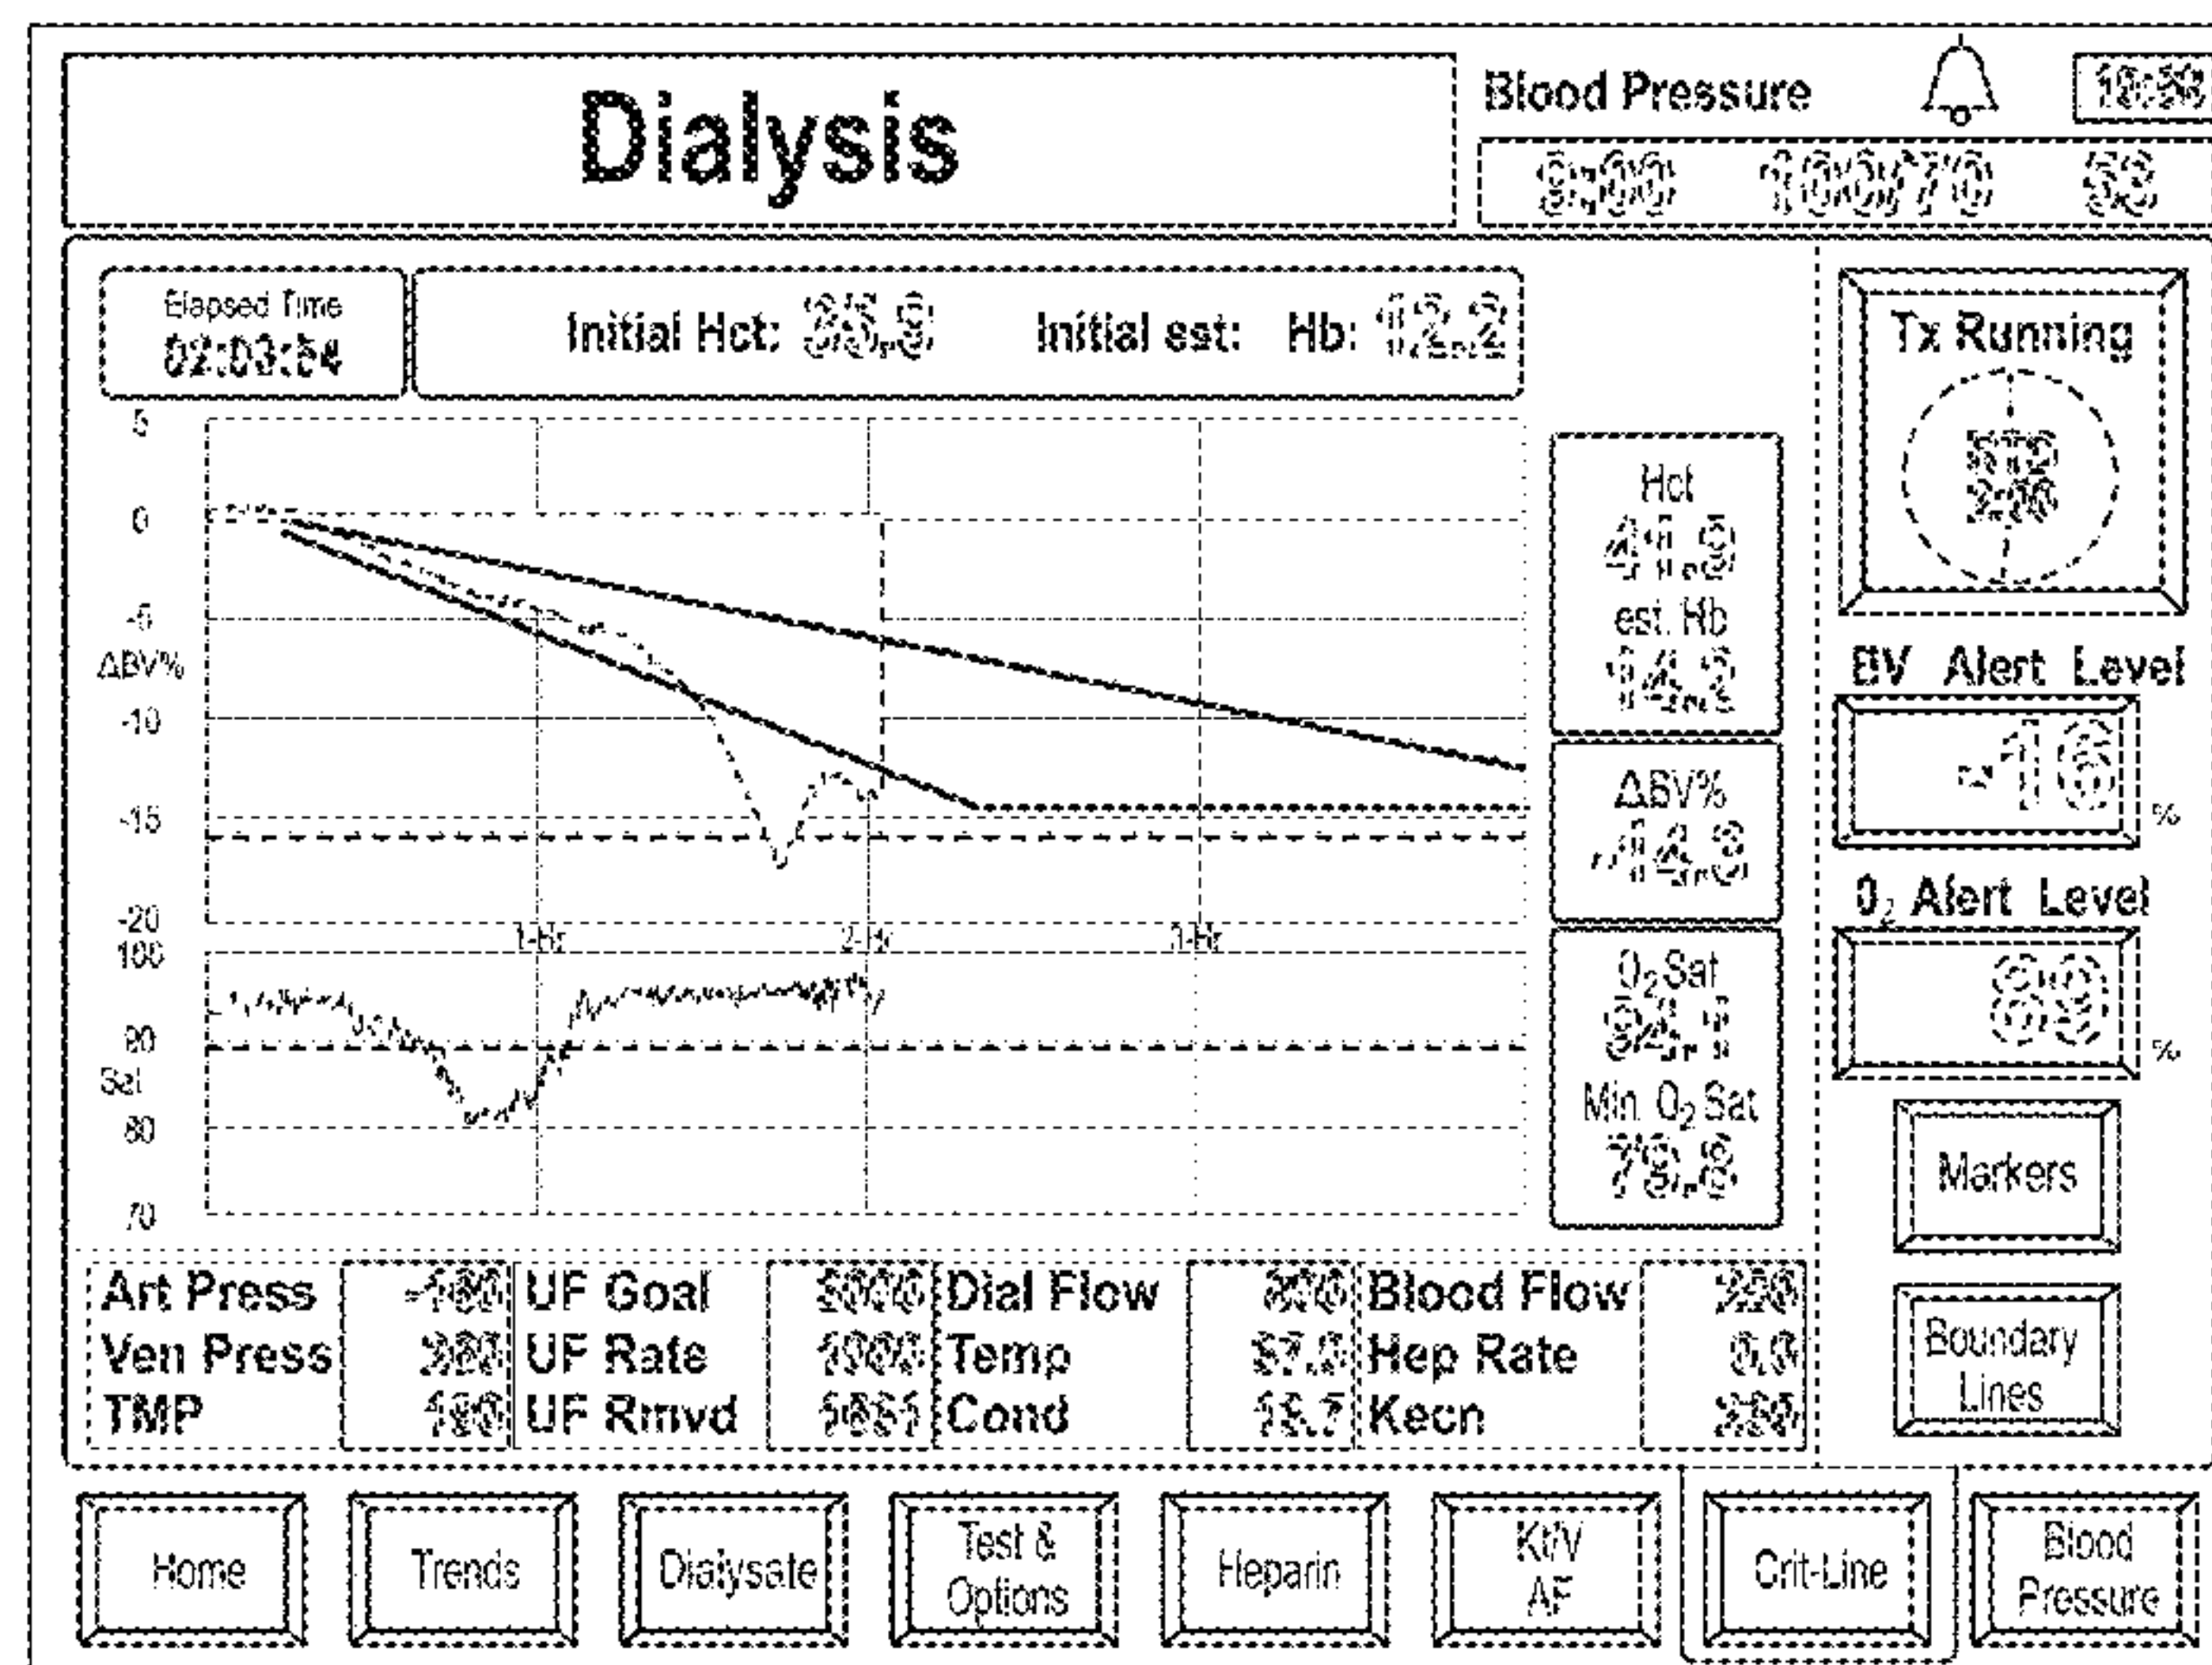

(56)

References Cited

U.S. PATENT DOCUMENTS

9,165,112 B2 * 10/2015 Doyle G16H 40/63
 D780,199 S * 2/2017 Croan D14/486
 9,801,993 B2 10/2017 Barrett et al.
 D804,496 S * 12/2017 Wahila D14/485
 D812,634 S * 3/2018 Tuthill D14/486
 D813,883 S * 3/2018 Amin D14/485
 D816,689 S * 5/2018 Chalker D14/485
 D820,288 S * 6/2018 Howell D14/486
 D872,757 S * 1/2020 Howell D14/486
 D874,481 S * 2/2020 Kumar D14/485
 D896,828 S * 9/2020 Linares D14/486
 D924,910 S * 7/2021 Laumann D14/486
 2002/0052820 A1 * 5/2002 Gatto G06Q 40/02
 705/36 R
 2002/0154156 A1 * 10/2002 Moriwake G11B 27/34
 715/716
 2007/0138069 A1 * 6/2007 Roncadi A61M 1/16
 210/96.2

2008/0105601 A1 5/2008 Ikeda
 2014/0028682 A1 * 1/2014 Omiya G06T 11/206
 345/440
 2017/0180482 A1 6/2017 Wang et al.
 2019/0200921 A1 7/2019 Barrett et al.

OTHER PUBLICATIONS

“A flexible dialysis system to drive advanced treatments” Jul. 13, 2019, posted at nikkisomedical.com, [site visited Jun. 8, 2021]. https://web.archive.org/web/20190713004114/http://nikkisomedical.com/wp-content/uploads/2017/06/NIKKISO_DBB-07_EN_2017-04_ver7pkt4.pdf (Year: 2019).*

International Patent Application No. PCT/US2020/066498, International Search Report (dated Mar. 18, 2021).

“CLiC Device Profile Guide,” Fresenius Medical Care Renal Technologies, https://fmcna.com/content/dam/fmcna/live/support/documents/fluid-management/clic/CLiC_ProfileGuide.pdf (2016).

* cited by examiner

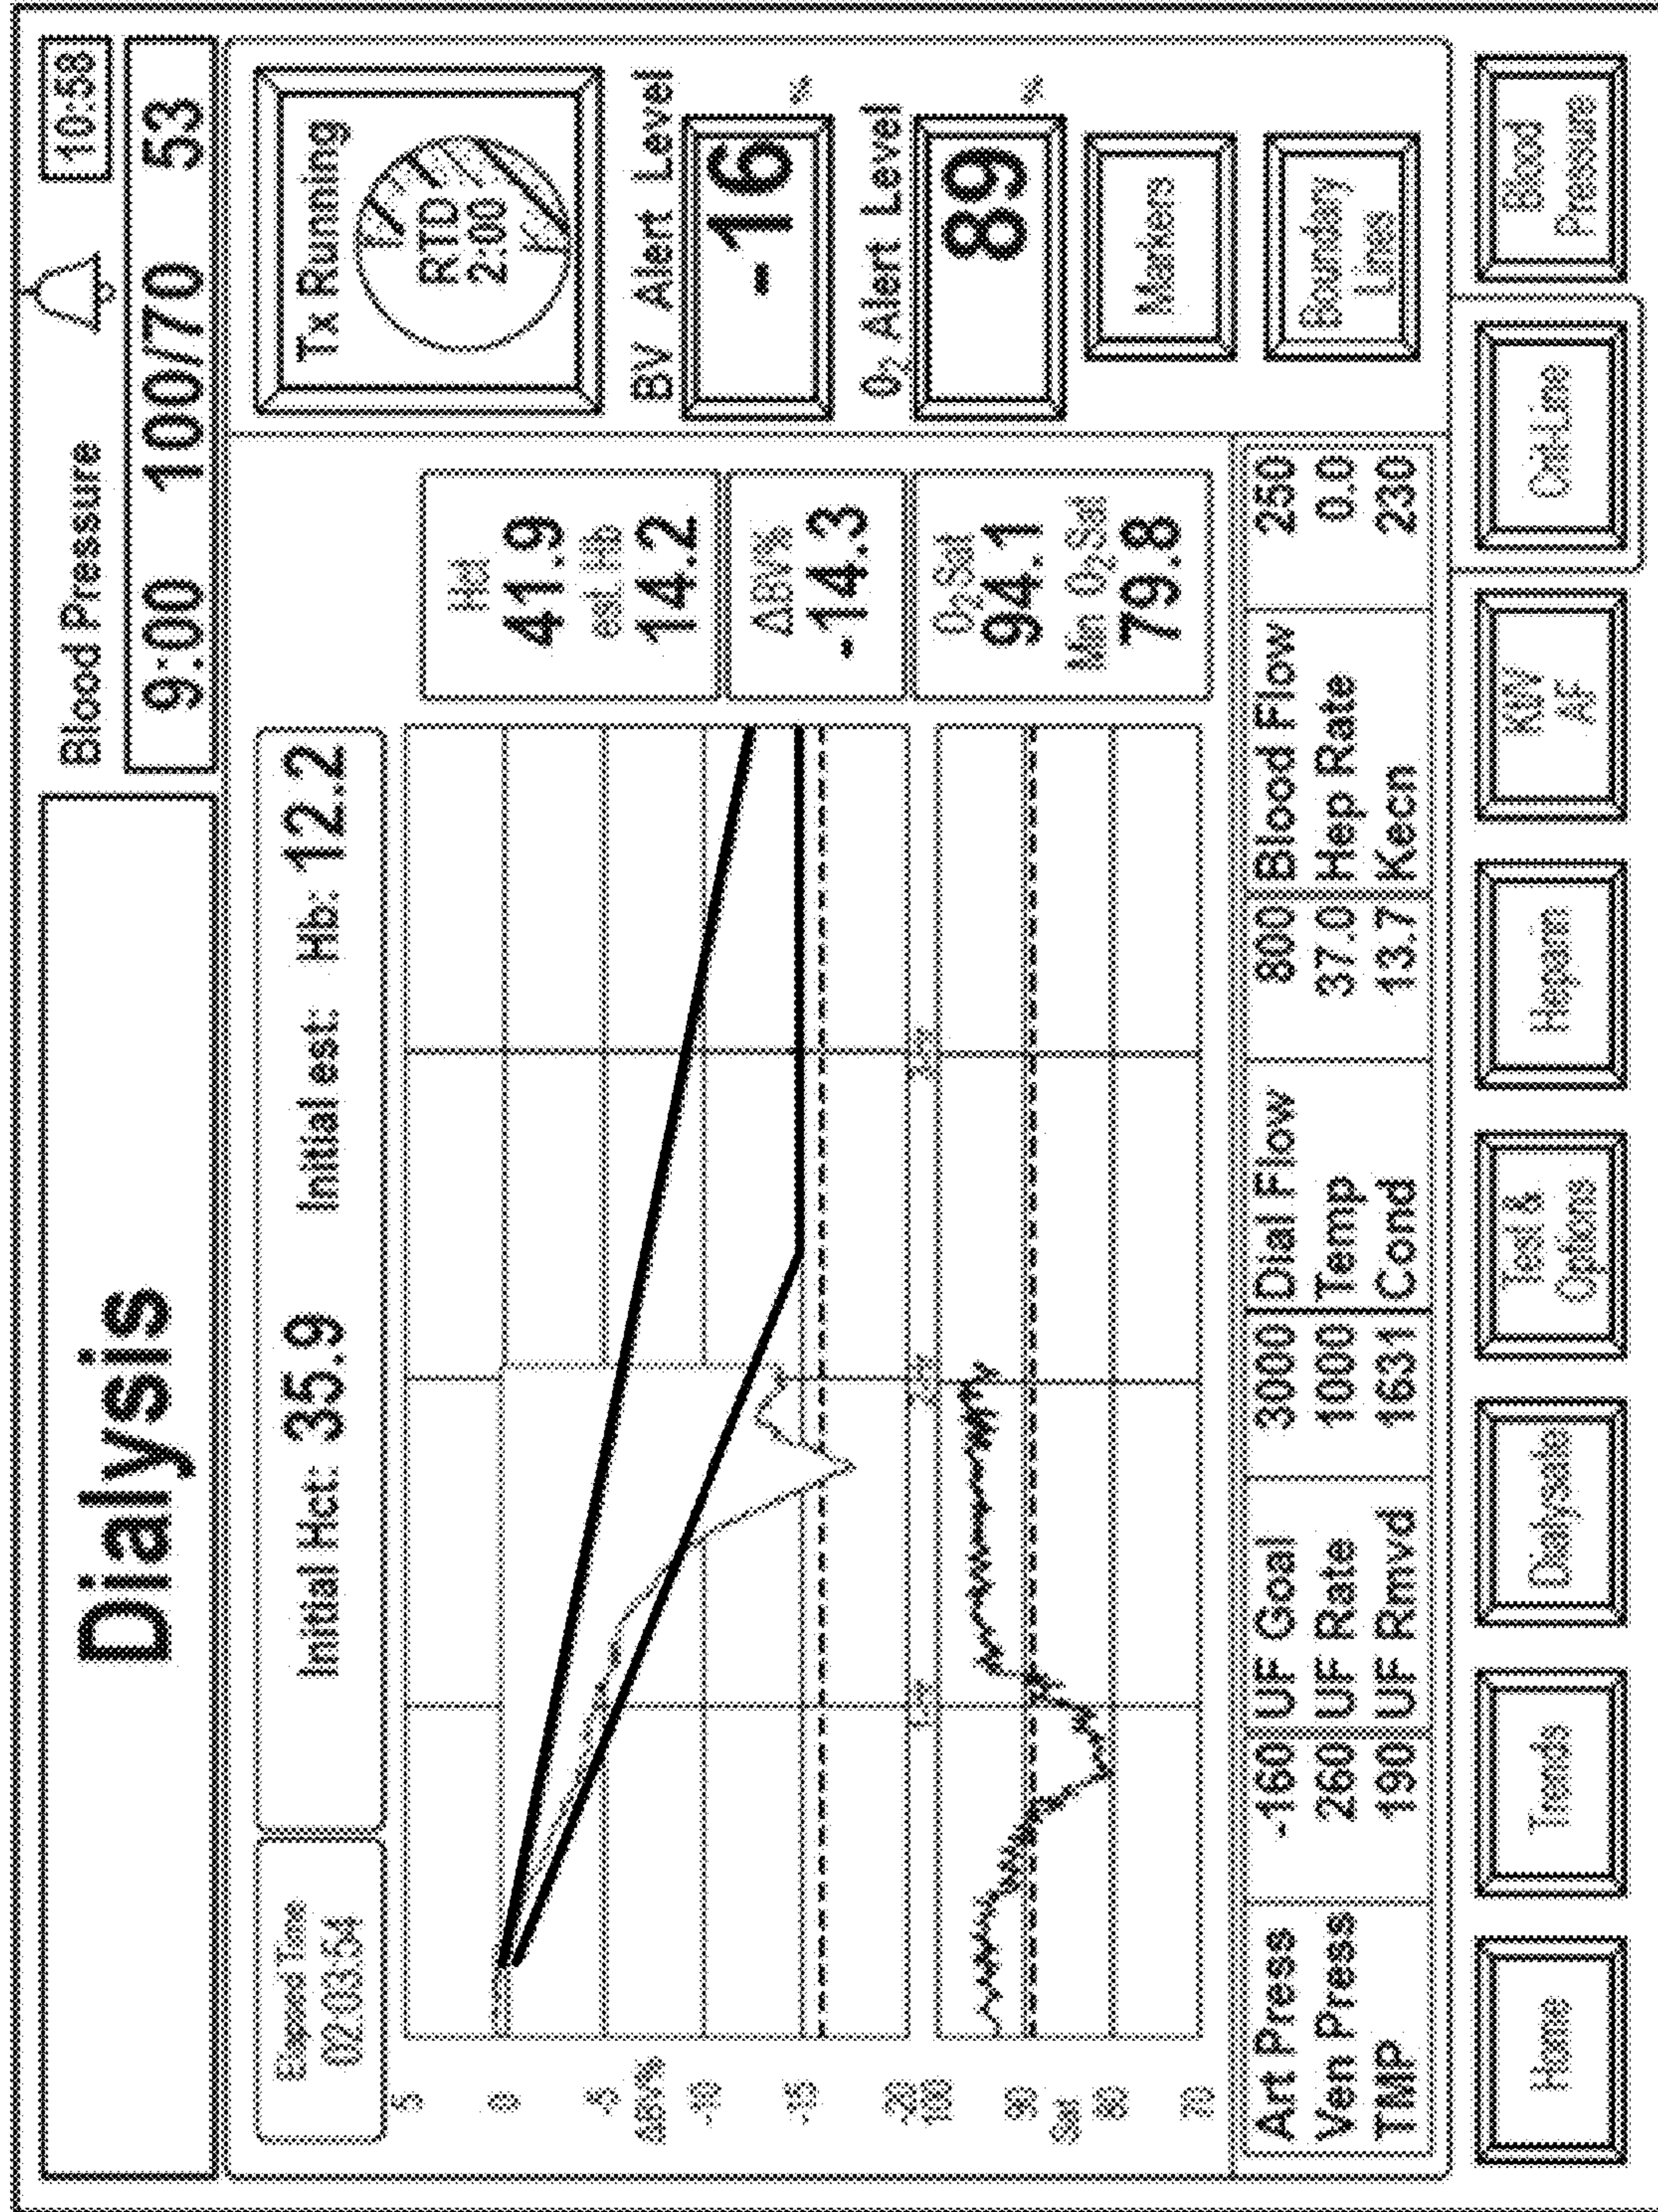


FIG. 1

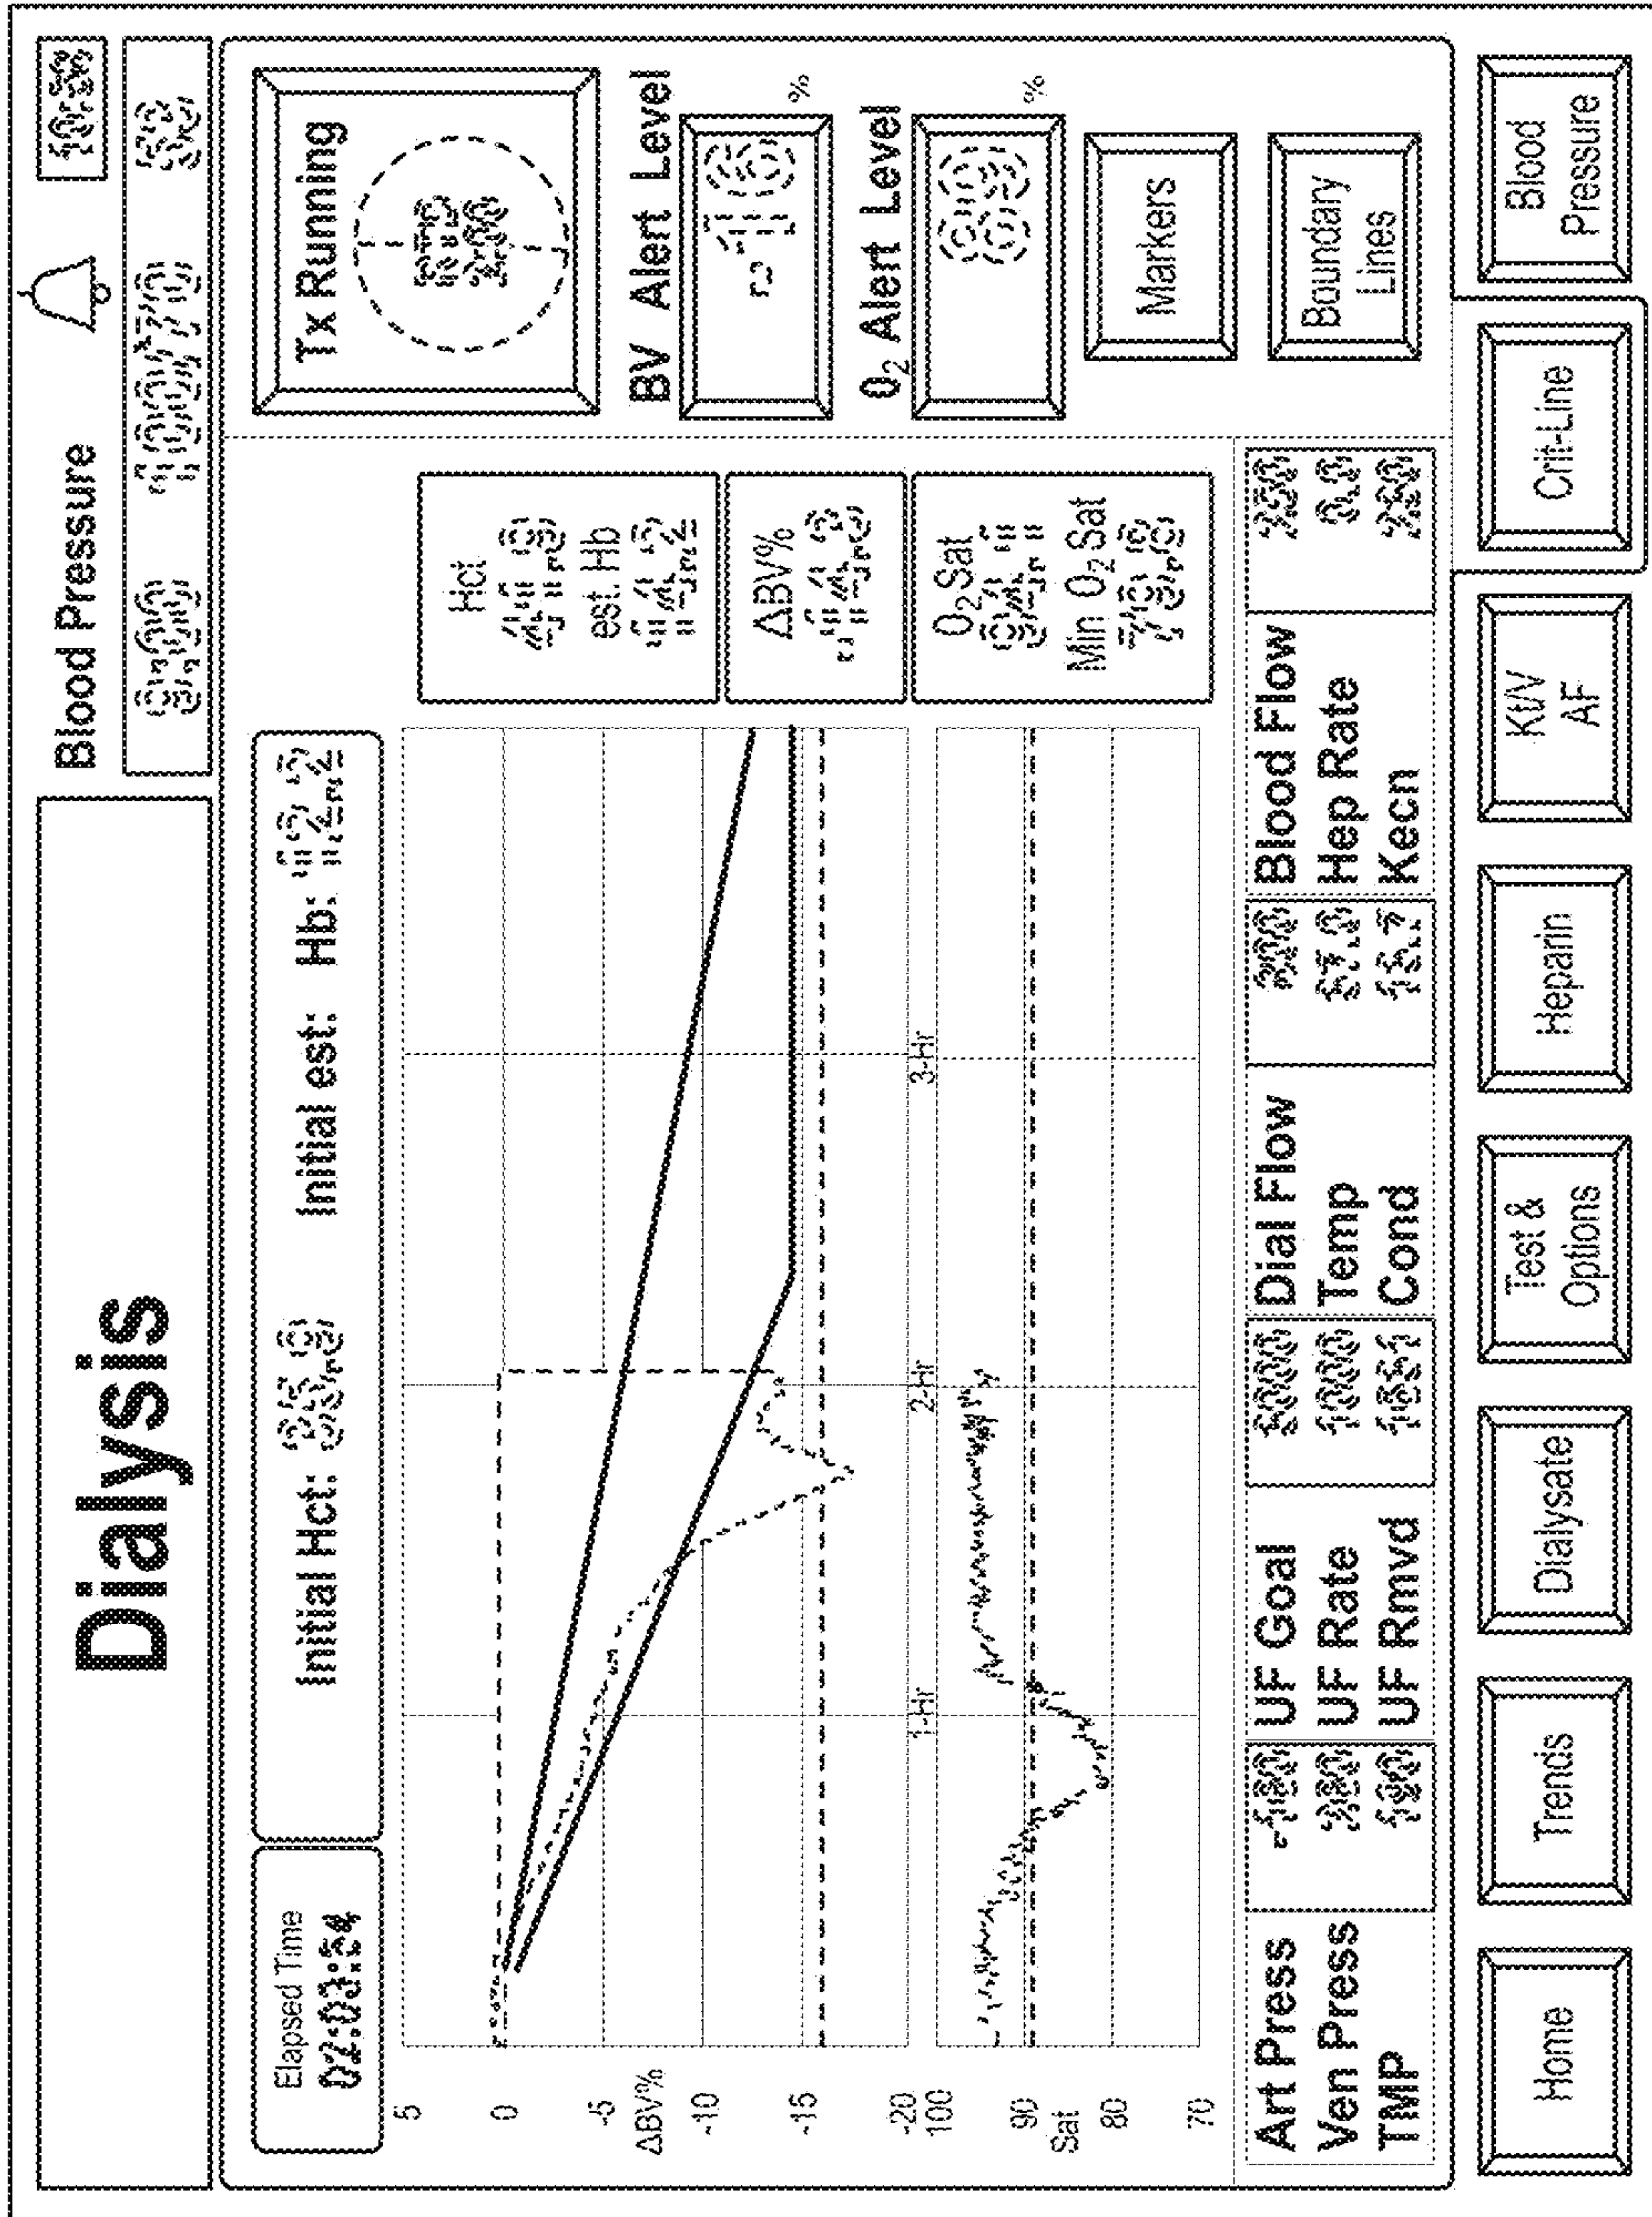


FIG. 2

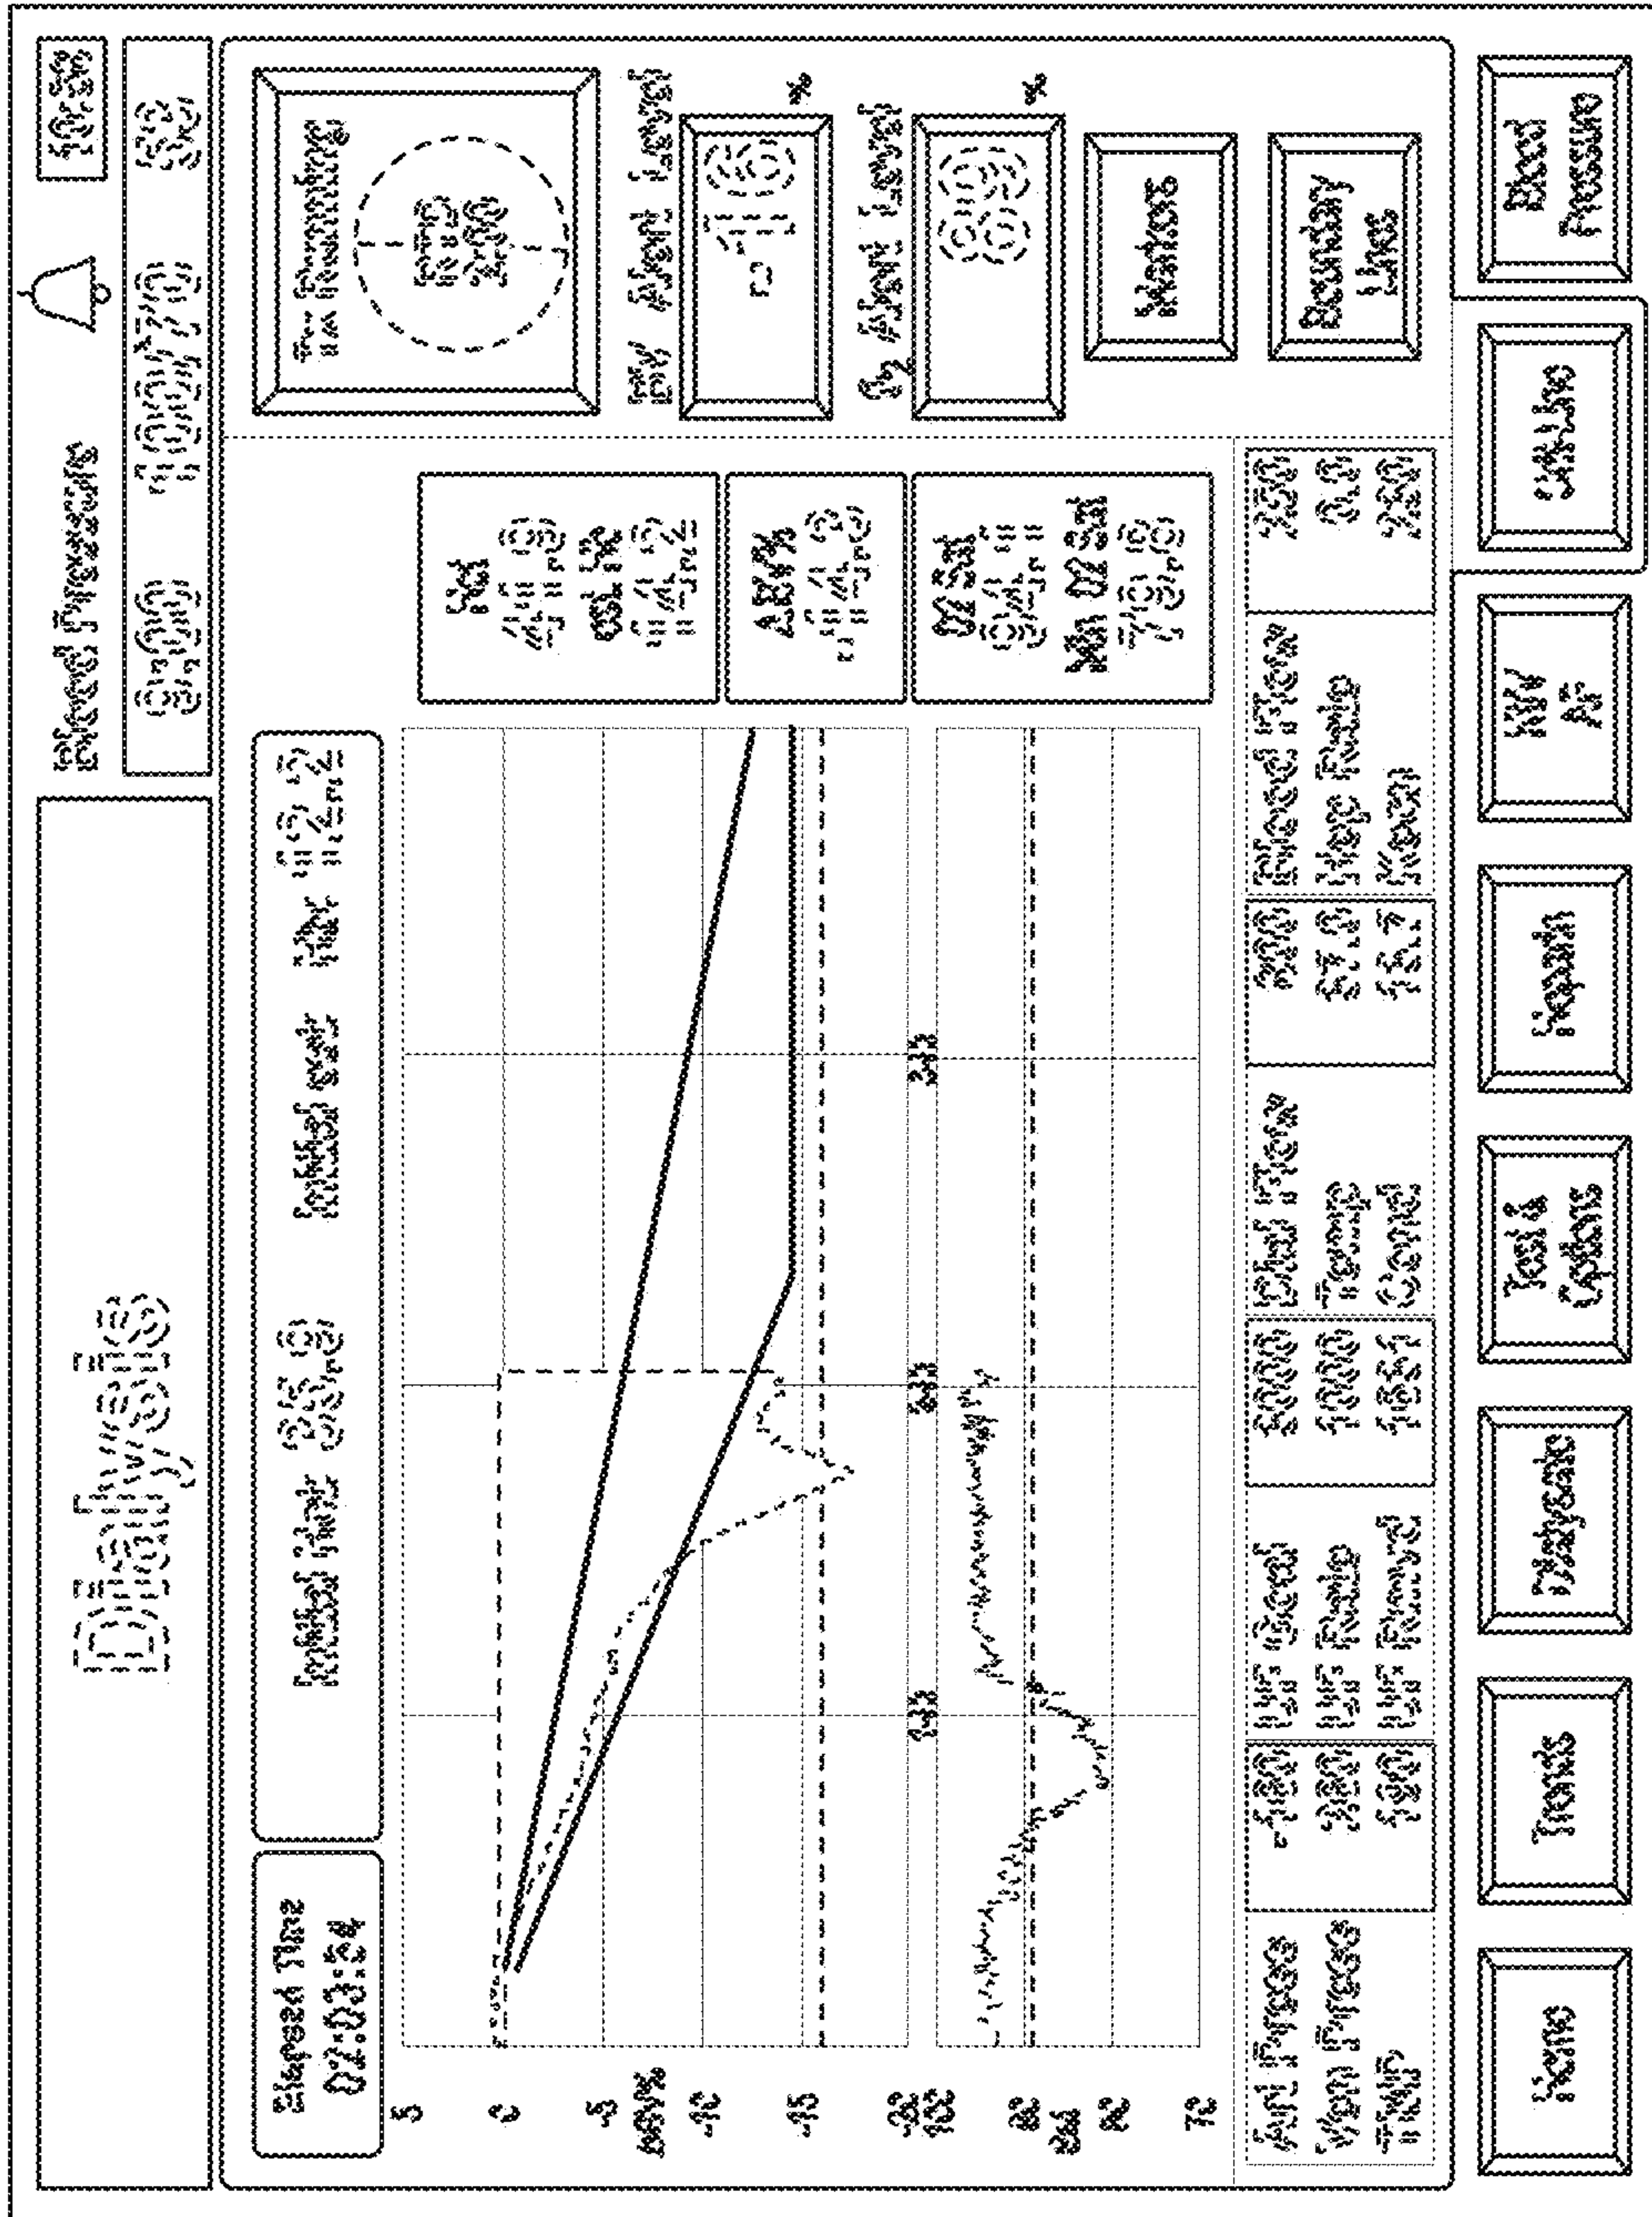


FIG. 3