



US00D941343S

(12) **United States Design Patent** (10) **Patent No.:** **US D941,343 S**
Langan et al. (45) **Date of Patent:** **** Jan. 18, 2022**

(54) **DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE FOR AN INFUSION DEVICE**

D611,994 S 3/2010 Lanman
D658,667 S 5/2012 Cho
D697,940 S 1/2014 Bitran
D726,736 S * 4/2015 Smirin G06F 3/04817
D14/485
D730,981 S * 6/2015 Solomon D19/1
D740,850 S * 10/2015 Zhang D14/487
D752,604 S 3/2016 Zhang
D770,487 S 11/2016 Li
D794,049 S 3/2017 Gupta
D783,641 S * 4/2017 Elston D14/486
D794,660 S 8/2017 Lonergan
(Continued)

(71) Applicant: **CareFusion 303, Inc.**, San Diego, CA (US)

(72) Inventors: **John Langan**, San Diego, CA (US);
Kelly Daoust, San Diego, CA (US);
Luis Shriner, San Diego, CA (US);
Craig Mitchell, Carlsbad, CA (US);
Wendy Smyth, San Diego, CA (US)

(73) Assignee: **CareFusion 303, Inc.**, San Diego, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/802,017**

(22) Filed: **Aug. 2, 2021**

Related U.S. Application Data

(62) Division of application No. 29/648,278, filed on May 18, 2018, now Pat. No. Des. 926,794.

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495; D20/10, 11, 22-33, 39, D20/40

CPC G06F 3/048-04897; G06F 19/3456; A61M 2205/35; A61M 5/003; A61M 2039/0205; A61M 2205/505

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D599,373 S * 9/2009 Kobayashi D14/486
D606,085 S 12/2009 Agnetta

OTHER PUBLICATIONS

Match List & Calendar Exploration, by Xiaochu, dribbble.com [online], published on Jun. 6, 2017, [retrieved on Sep. 6, 2021], retrieved from the Internet <URL: https://dribbble.com/shots/3549171-Match-List-Calendar-Exploration> (Year: 2017).*

(Continued)

Primary Examiner — Ian F Whitmore

(74) *Attorney, Agent, or Firm* — Morgan, Lewis & Bockius LLP

(57) **CLAIM**


The ornamental design for a display screen with graphical user interface for an infusion device, as shown and described.

DESCRIPTION

The sole FIGURE is a front view of a display screen with graphical user interface for an infusion device showing our new design.

The outermost broken-line shows the perimeter of a display screen or portion thereof and forms no part of the claimed design. The remaining broken lines illustrate portions of a graphical user interface and form no part of the claimed design.

1 Claim, 1 Drawing Sheet

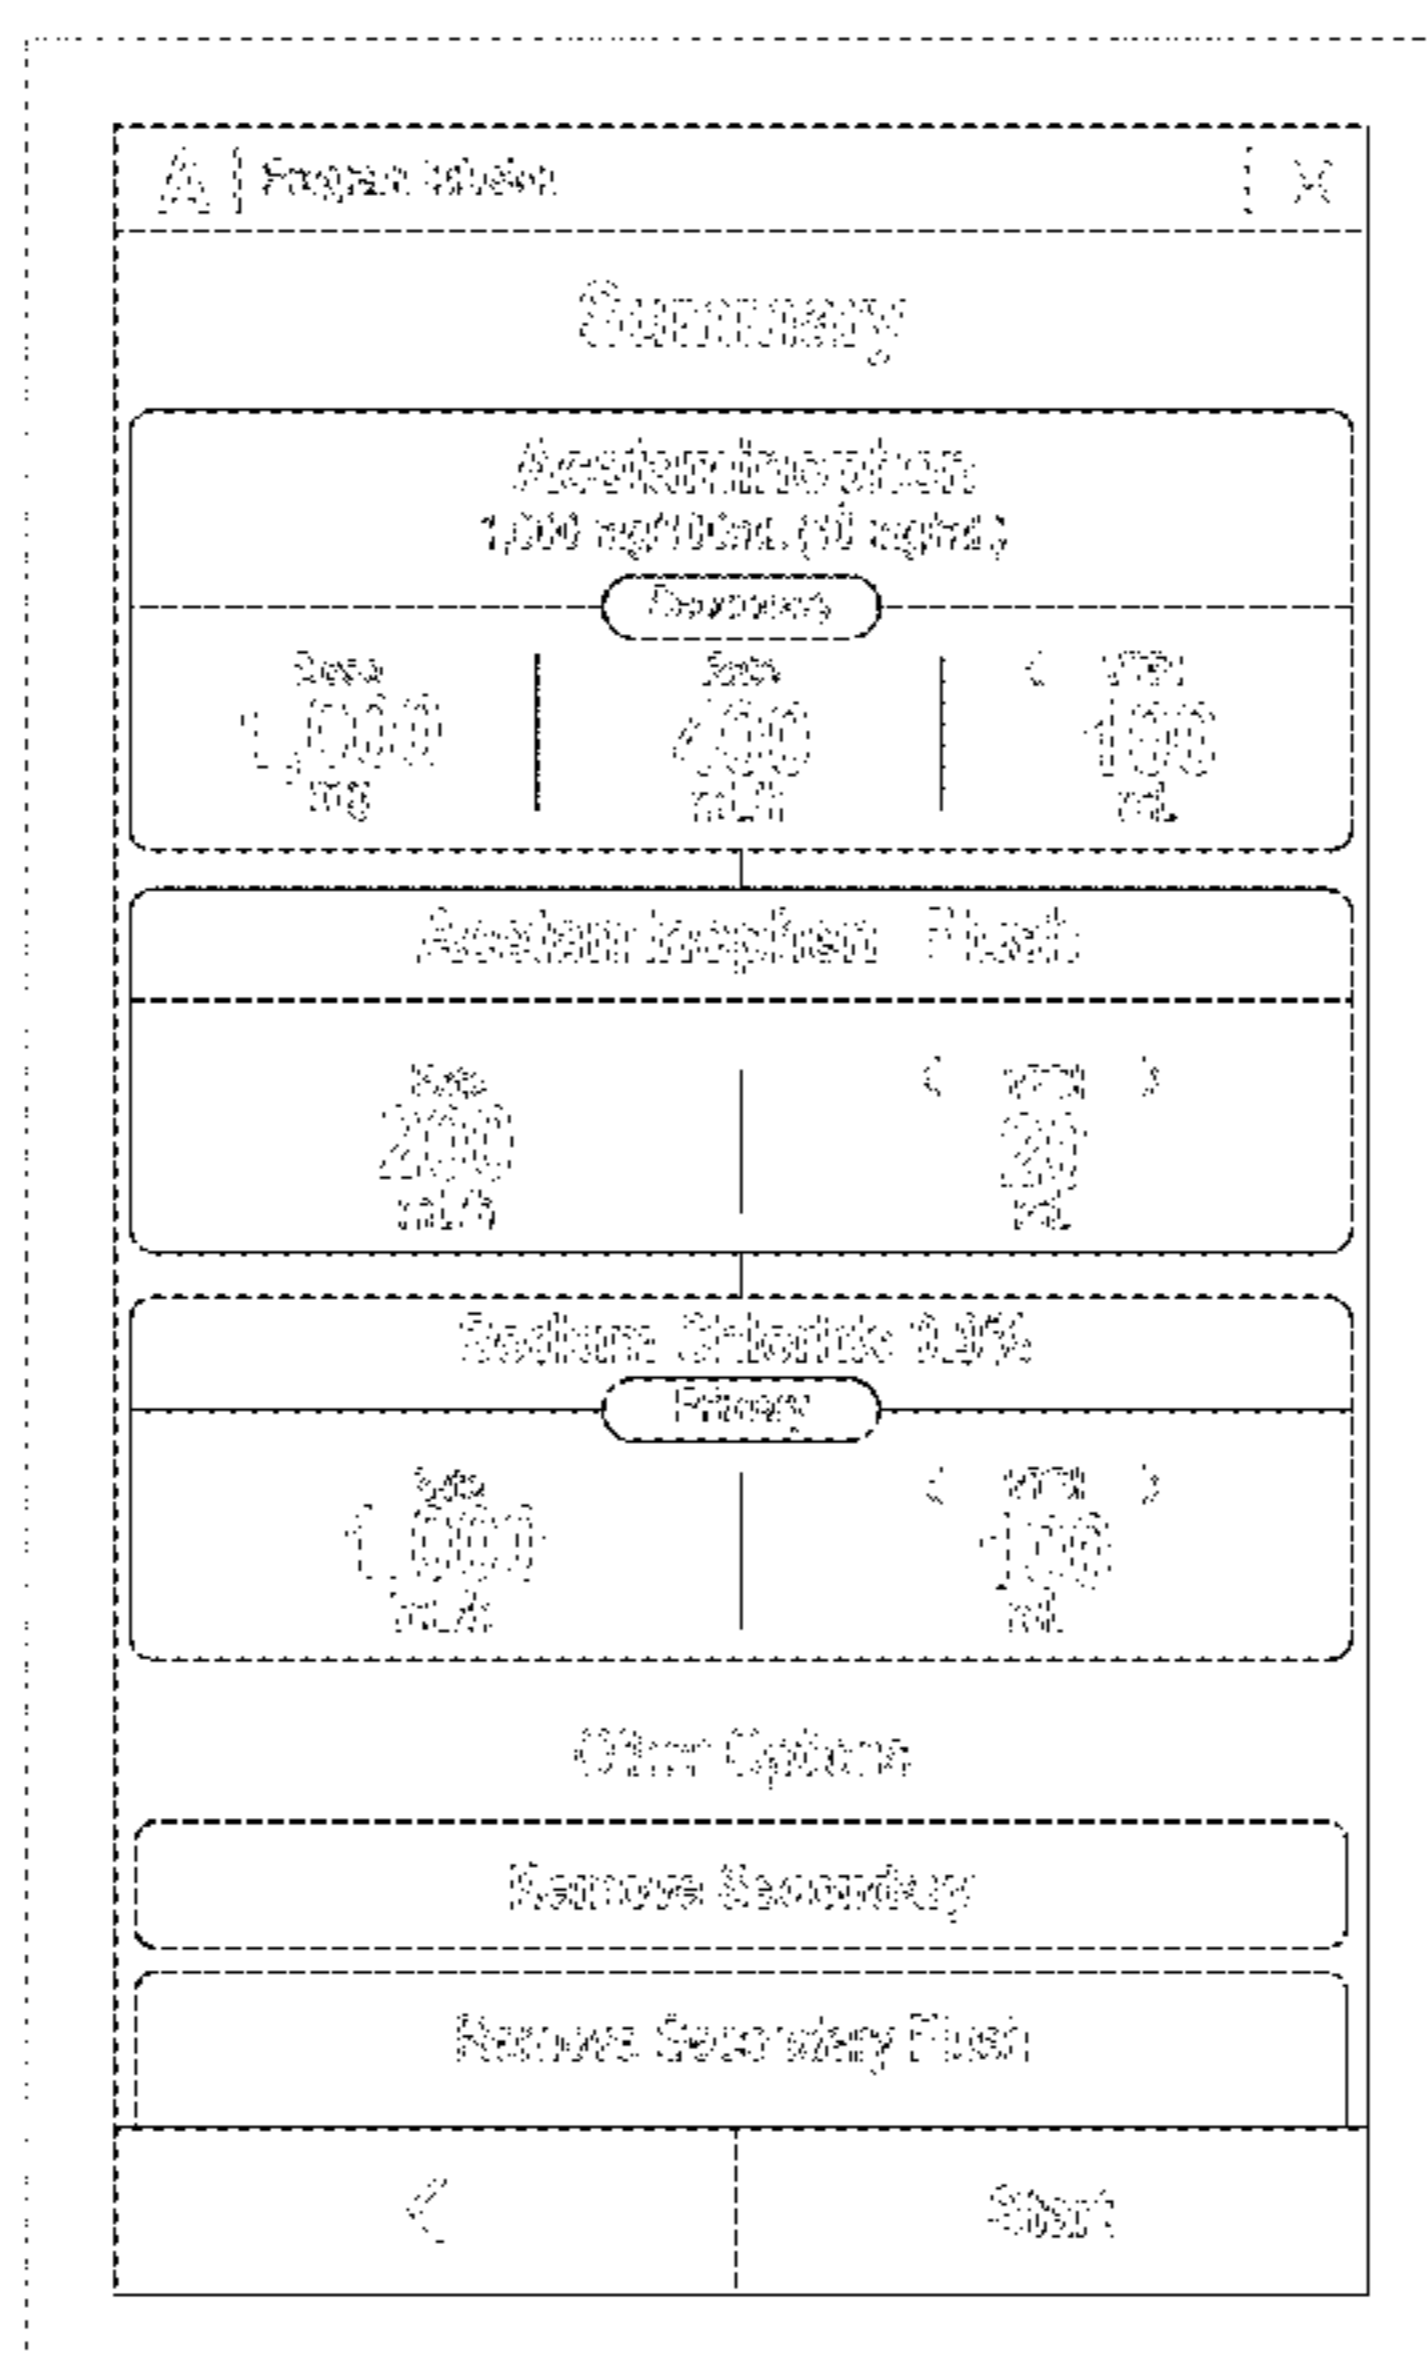

(56)

References Cited

U.S. PATENT DOCUMENTS

D801,378 S 10/2017 Sachtleben
 D824,930 S 3/2018 Spector
 D816,704 S * 5/2018 Spector D14/486
 D824,945 S 8/2018 Sagrillo
 D824,950 S * 8/2018 Spector D14/486
 D829,750 S * 10/2018 Phillips D14/486
 D830,375 S * 10/2018 Phillips D14/485
 10,218,938 B2 2/2019 Taylor
 D844,020 S 3/2019 Spector
 D845,972 S 4/2019 Pranger
 D854,042 S 7/2019 Sagrillo
 D892,820 S * 8/2020 Jee D14/485
 D896,824 S * 9/2020 Langan D14/486
 D897,361 S * 9/2020 Langan D14/486
 D905,725 S 12/2020 Derusseau
 D910,054 S * 2/2021 Silfver D14/486
 D910,694 S * 2/2021 Norman D14/488
 D926,794 S * 8/2021 Langan D14/486
 D929,437 S * 8/2021 Langan D14/486
 2005/0120940 A1 6/2005 Sinclair
 2006/0020538 A1 1/2006 Ram
 2009/0187359 A1 7/2009 Tuerk
 2011/0082808 A1 * 4/2011 Beykpour G09B 5/00
 705/327
 2011/0144586 A1 * 6/2011 Michaud F16J 15/56
 604/151
 2013/0132854 A1 5/2013 Raleigh
 2013/0132908 A1 * 5/2013 Lee G06F 3/04842
 715/838

2014/0330241 A1 11/2014 Bollish
 2015/0304270 A1 * 10/2015 Cook H04L 51/32
 709/206
 2018/0025309 A1 1/2018 Absher
 2019/0354243 A1 * 11/2019 Langan A61M 5/1413

OTHER PUBLICATIONS

Canadian Office Action for Industrial Design Application No. 184671, dated Oct. 21, 2019, 2 pages.
 Create a Parallax Scrolling Header with Tabs in Android, by Shakir, android.jlelse.eu [online], published on Sep. 15, 2015, [retrieved on Dec. 9, 2020], retrieved from the internet (Year: 2015).
 EMS Apps to Improve Patient Care, by Grange, ems1.com [online], published on Nov. 7, 2016, [retrieved on May 17, 2019], retrieved from the Internet [URL: <https://www.ems1.com/ems-products/technology/articles/141906048-EMS-apps-to-improve-patient-care/>] (Year: 2016).
 Folding Cell—UI Animation Library for Swift & Java, by Ramotion, dribbble.com [online], published on Jun. 25, 2015, [retrieved on May 17, 2019], retrieved from the Internet [URL: <https://dribbble.com/shots/2121350-Folding-Cell-UI-Animation-Library-for-Swift-Java>] (Year: 2015).
 Realistic Cinema Tickets Vector, freepik.com [online], published on or before Jul. 17, 2016, [retrieved on May 17, 2019], retrieved from the Internet [URL: https://freepik.com/free-vector/realistic-cinema-tickets_848041.htm] (Year: 2016).

* cited by examiner

A | Program Inclusion | X

Summary

Acetaminophen
1,000 mg/100ml. (10 mg/ml)

Secondary

Dose 1,000 mg	Rate 400 ml/h	< VTEI > 100 ml
---------------------	---------------------	-----------------------

Acetaminophen- Flush

Rate 200 ml/h	< VTEI > 20 ml
---------------------	----------------------

Sodium Chloride 0.9%

Primary

Rate 1,000 ml/h	< VTEI > 100 ml
-----------------------	-----------------------

Other Options

Remove Secondary

Remove Secondary Flush

< Start