

US00D942006S

(12) **United States Design Patent**  
**Takemoto**

(10) **Patent No.:** **US D942,006 S**  
(45) **Date of Patent:** **\*\* Jan. 25, 2022**

(54) **GUIDE WIRE**

(71) Applicant: **ASAHI INTECC CO., LTD.**, Seto (JP)

(72) Inventor: **Hirokatsu Takemoto**, Seto (JP)

(73) Assignee: **ASAHI INTECC CO., LTD.**, Seto (JP)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/724,770**

(22) Filed: **Feb. 19, 2020**

(30) **Foreign Application Priority Data**

Aug. 30, 2019 (JP) ..... 2019-019480

(51) **LOC (13) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/140**

(58) **Field of Classification Search**  
USPC ..... D24/140, 135, 133  
CPC ..... A61M 25/09; A61M 25/09033; A61M  
25/0041; A61M 2025/09175; A61M  
2025/09133; A61M 2025/0915; A61M  
2025/09083  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D247,512 S \* 3/1978 Sandler ..... 606/191  
D363,544 S \* 10/1995 Rowland ..... D24/112  
5,849,005 A \* 12/1998 Garrison ..... A61B 90/40  
606/1  
6,161,543 A \* 12/2000 Cox ..... A61B 18/1492  
128/898  
D533,270 S \* 12/2006 Kierce ..... D24/112  
D704,335 S \* 5/2014 Bolia ..... D24/140  
D706,421 S \* 6/2014 Brannon ..... D24/140  
D741,999 S \* 10/2015 Kanazawa ..... D24/140  
D742,000 S \* 10/2015 Kanazawa ..... D24/140  
D757,268 S \* 5/2016 Norenberg ..... D24/147  
D758,574 S \* 6/2016 Fojtik ..... D24/133

D777,916 S \* 1/2017 Kuroda ..... D24/140  
D847,335 S \* 4/2019 Kuwada ..... D24/140  
D861,156 S \* 9/2019 Greenhalgh ..... D24/108  
D901,009 S \* 11/2020 Fojtik ..... D24/133

(Continued)

**OTHER PUBLICATIONS**

Internet Publication by mpo-mag.com, FDA Clears St. Jude Medical's Pressurewire X Guidewire, Publication Date: Oct. 10, 2016, [online], [retrieved on Sep. 24, 2021]. Retrieved from Internet, <URL: [https://www.mpo-mag.com/contents/view\\_breaking-news/2016-10-10/fda-clears-st-jude-medicals-pressurewire-x-guidewire-designed-to-optimize-pci-procedures/](https://www.mpo-mag.com/contents/view_breaking-news/2016-10-10/fda-clears-st-jude-medicals-pressurewire-x-guidewire-designed-to-optimize-pci-procedures/)>.\*

(Continued)

*Primary Examiner* — Bridget L Eland

(74) *Attorney, Agent, or Firm* — Oliff PLC


(57) **CLAIM**

The ornamental design for a guide wire, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the guide wire;  
FIG. 2 is a front elevational view thereof;  
FIG. 3 is a rear elevational view thereof;  
FIG. 4 is a top plan view thereof;  
FIG. 5 is a bottom plan view thereof;  
FIG. 6 is a right-side elevational view thereof; and,  
FIG. 7 is a left-side elevational view thereof.  
The evenly spaced broken lines in the drawings are for the purpose of illustrating portions of the guide wire that form no part of the claimed design. The dot-dash broken lines depict a boundary of the claimed subject matter and form no part of the claimed design. The broken line break lines in the drawings indicate that the appearance of any portion of the article between the broken break lines forms no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

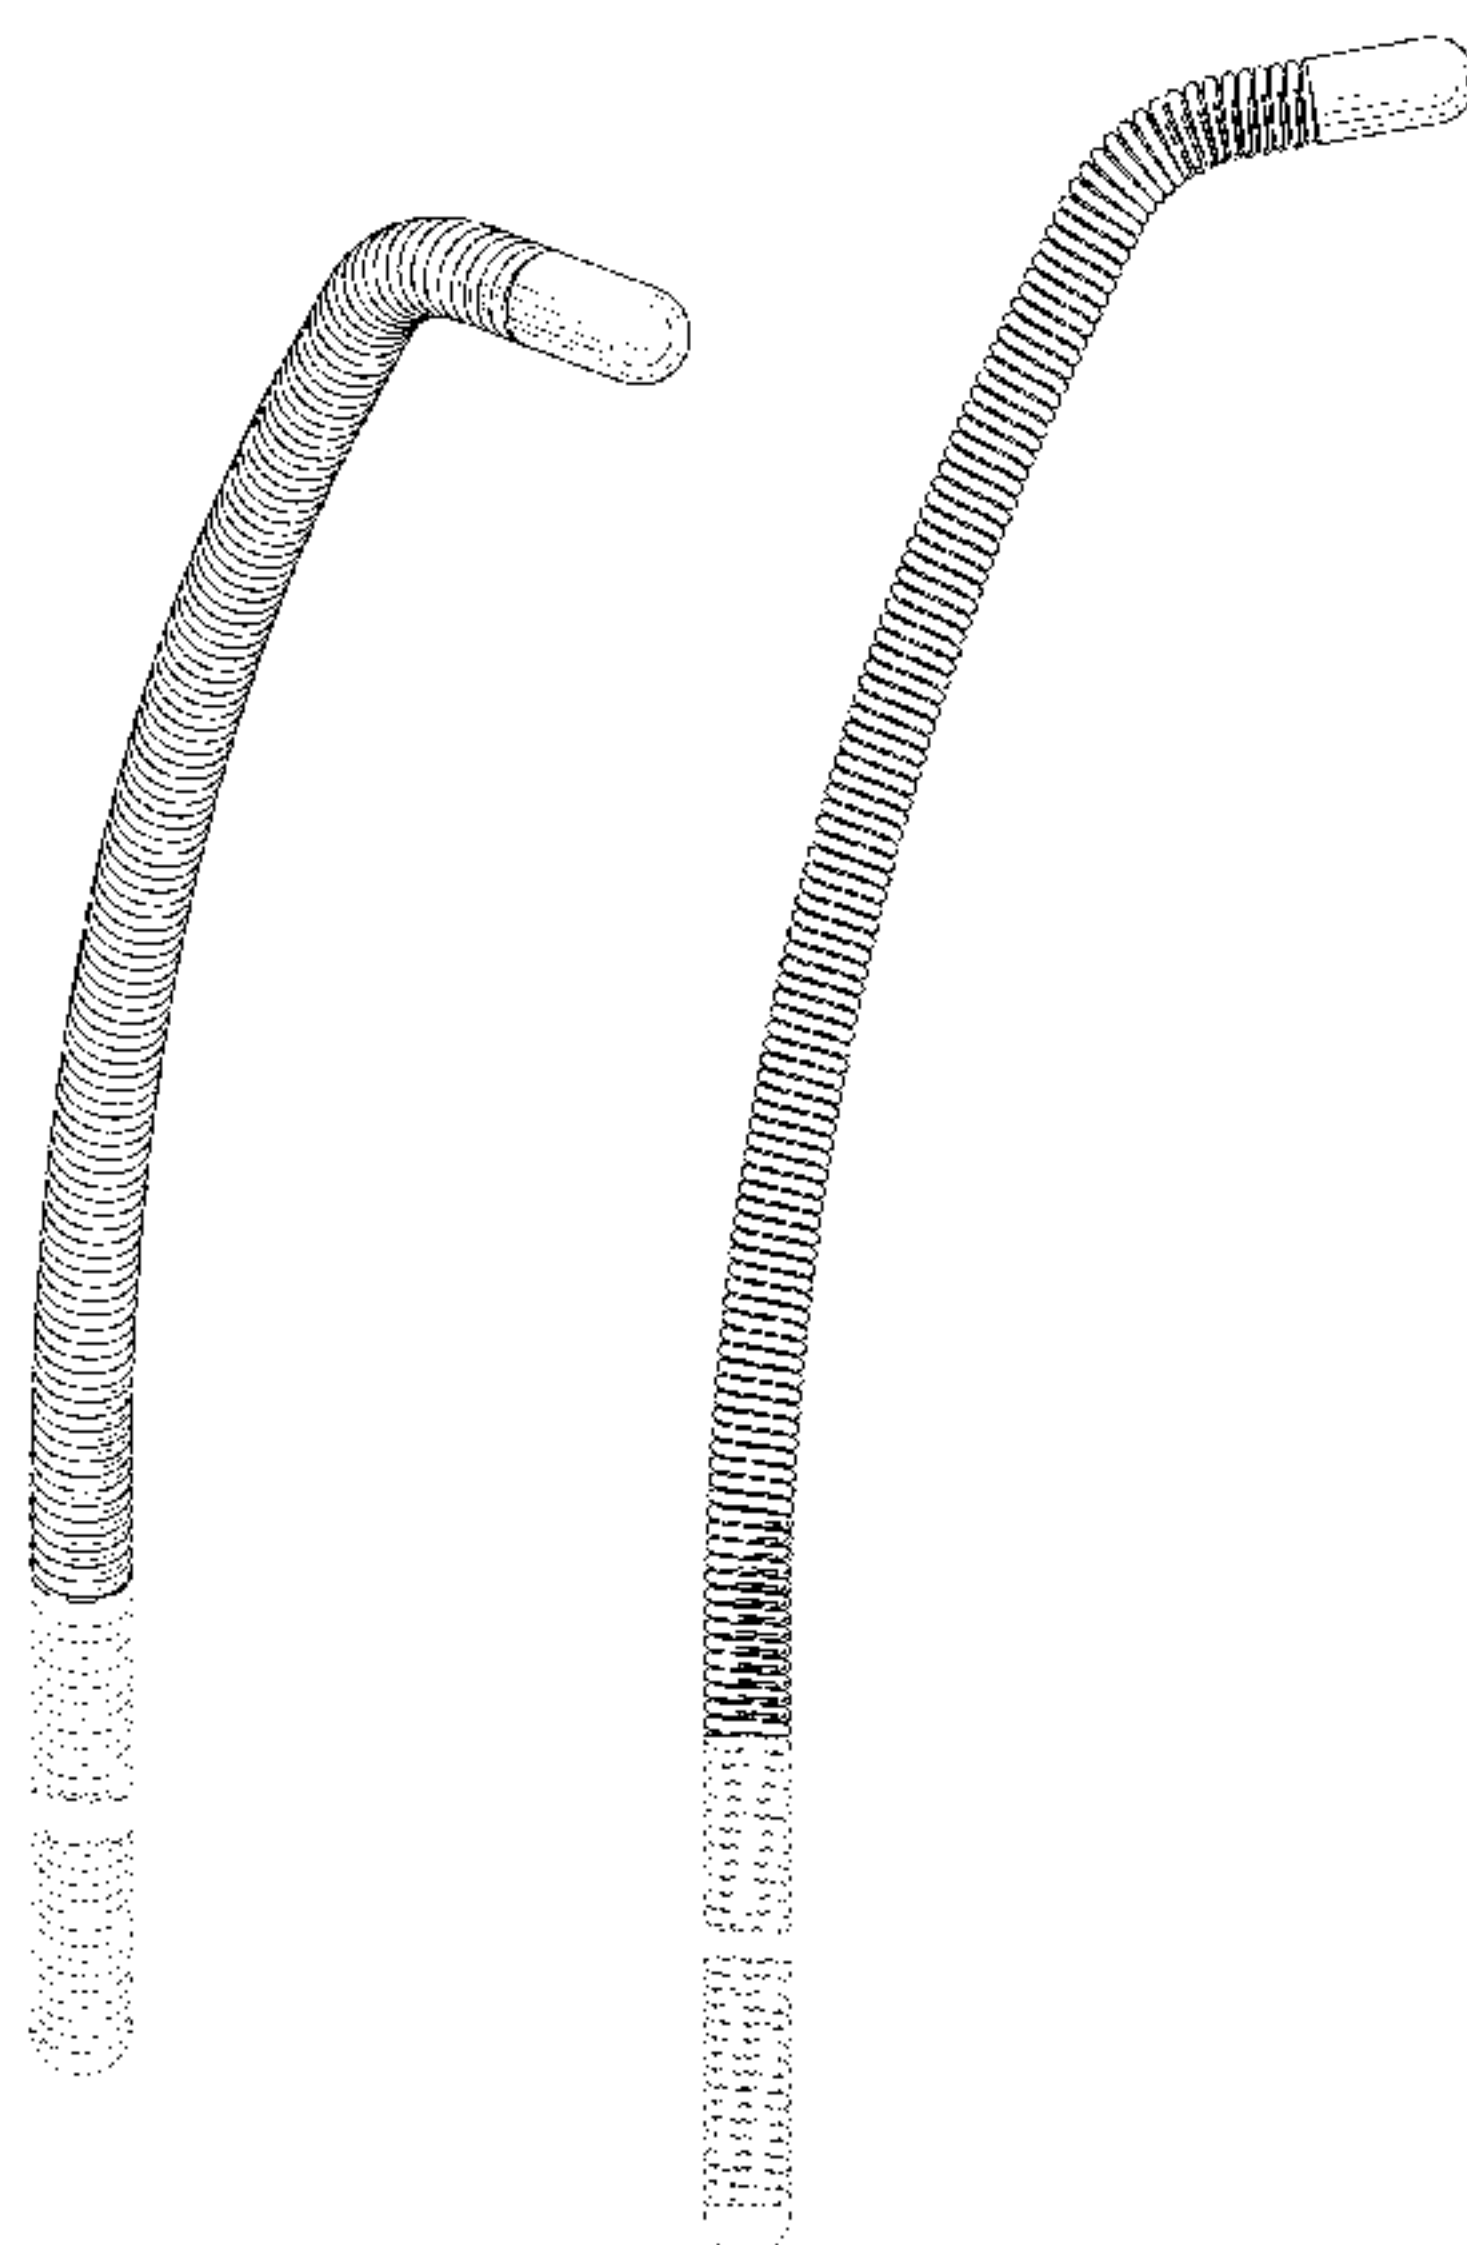

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2002/0055748 A1\* 5/2002 Gellman ..... A61B 17/32  
606/139  
2002/0091338 A1\* 7/2002 Frautschi ..... A61M 25/09  
600/585  
2008/0004546 A1\* 1/2008 Kato ..... A61M 25/09  
600/585  
2012/0024099 A1\* 2/2012 Main ..... A61B 17/0218  
74/470  
2013/0289445 A1\* 10/2013 Edamatsu ..... A61M 25/09  
600/585  
2014/0350568 A1\* 11/2014 Shekalim ..... A61B 17/22  
606/127  
2017/0113024 A1\* 4/2017 Hess ..... A61B 17/8897  
2017/0119473 A1\* 5/2017 Clopp ..... A61B 17/24  
2020/0069921 A1\* 3/2020 Mangiardi ..... A61M 25/104  
2020/0330729 A1\* 10/2020 Petitpierre ..... A61M 25/0136  
2020/0330730 A1\* 10/2020 Creighton ..... A61L 29/16

OTHER PUBLICATIONS

Internet Publication by Esticast, Medical Guide Wire Market By Material, Publication Date: May 2018, [online], [retrieved on Sep. 24, 2021]. Retrieved from Internet ,<URL: <https://www.esticastresearch.com/report/medical-guide-wire-market/>>.\*

\* cited by examiner

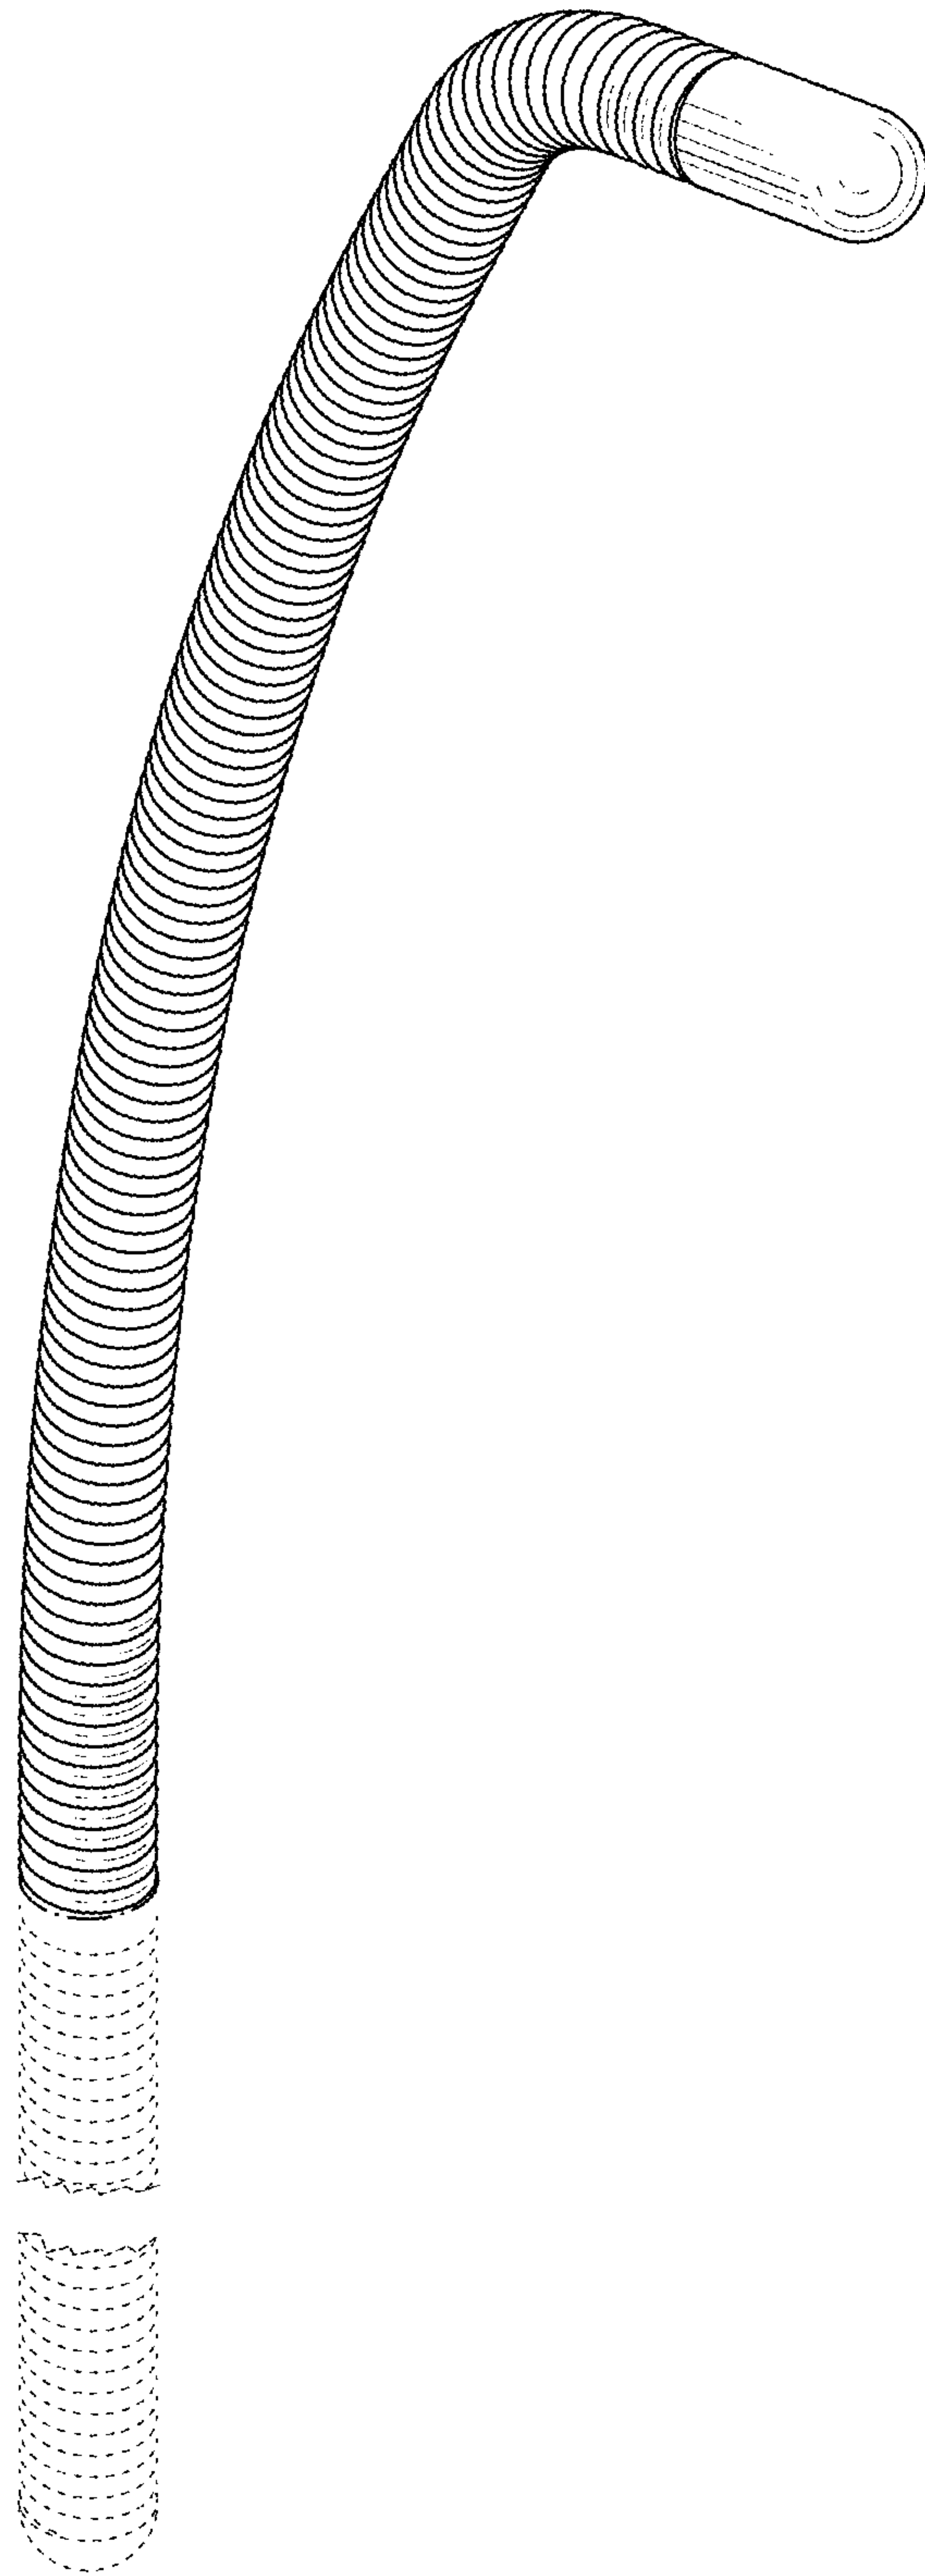


FIG. 1

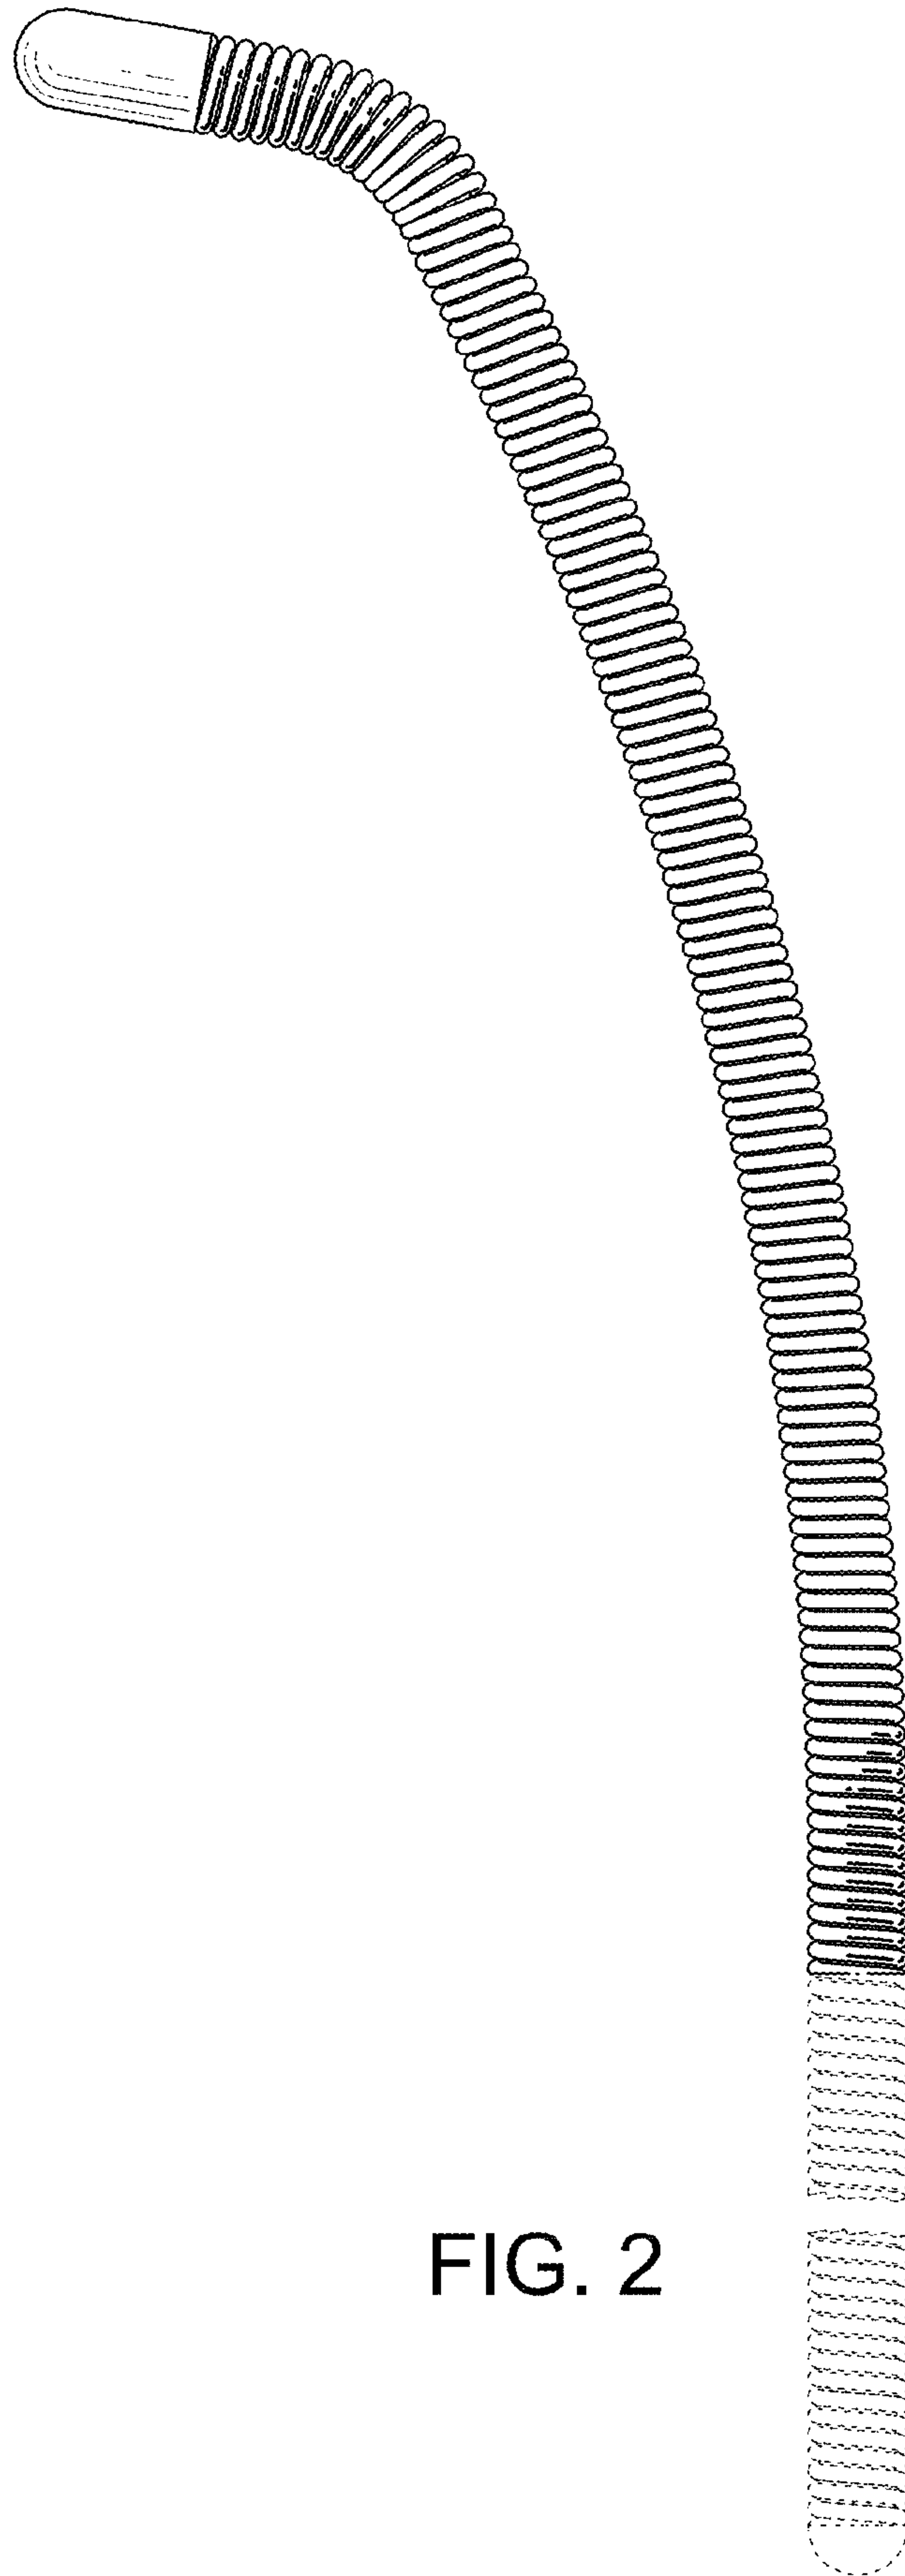


FIG. 2

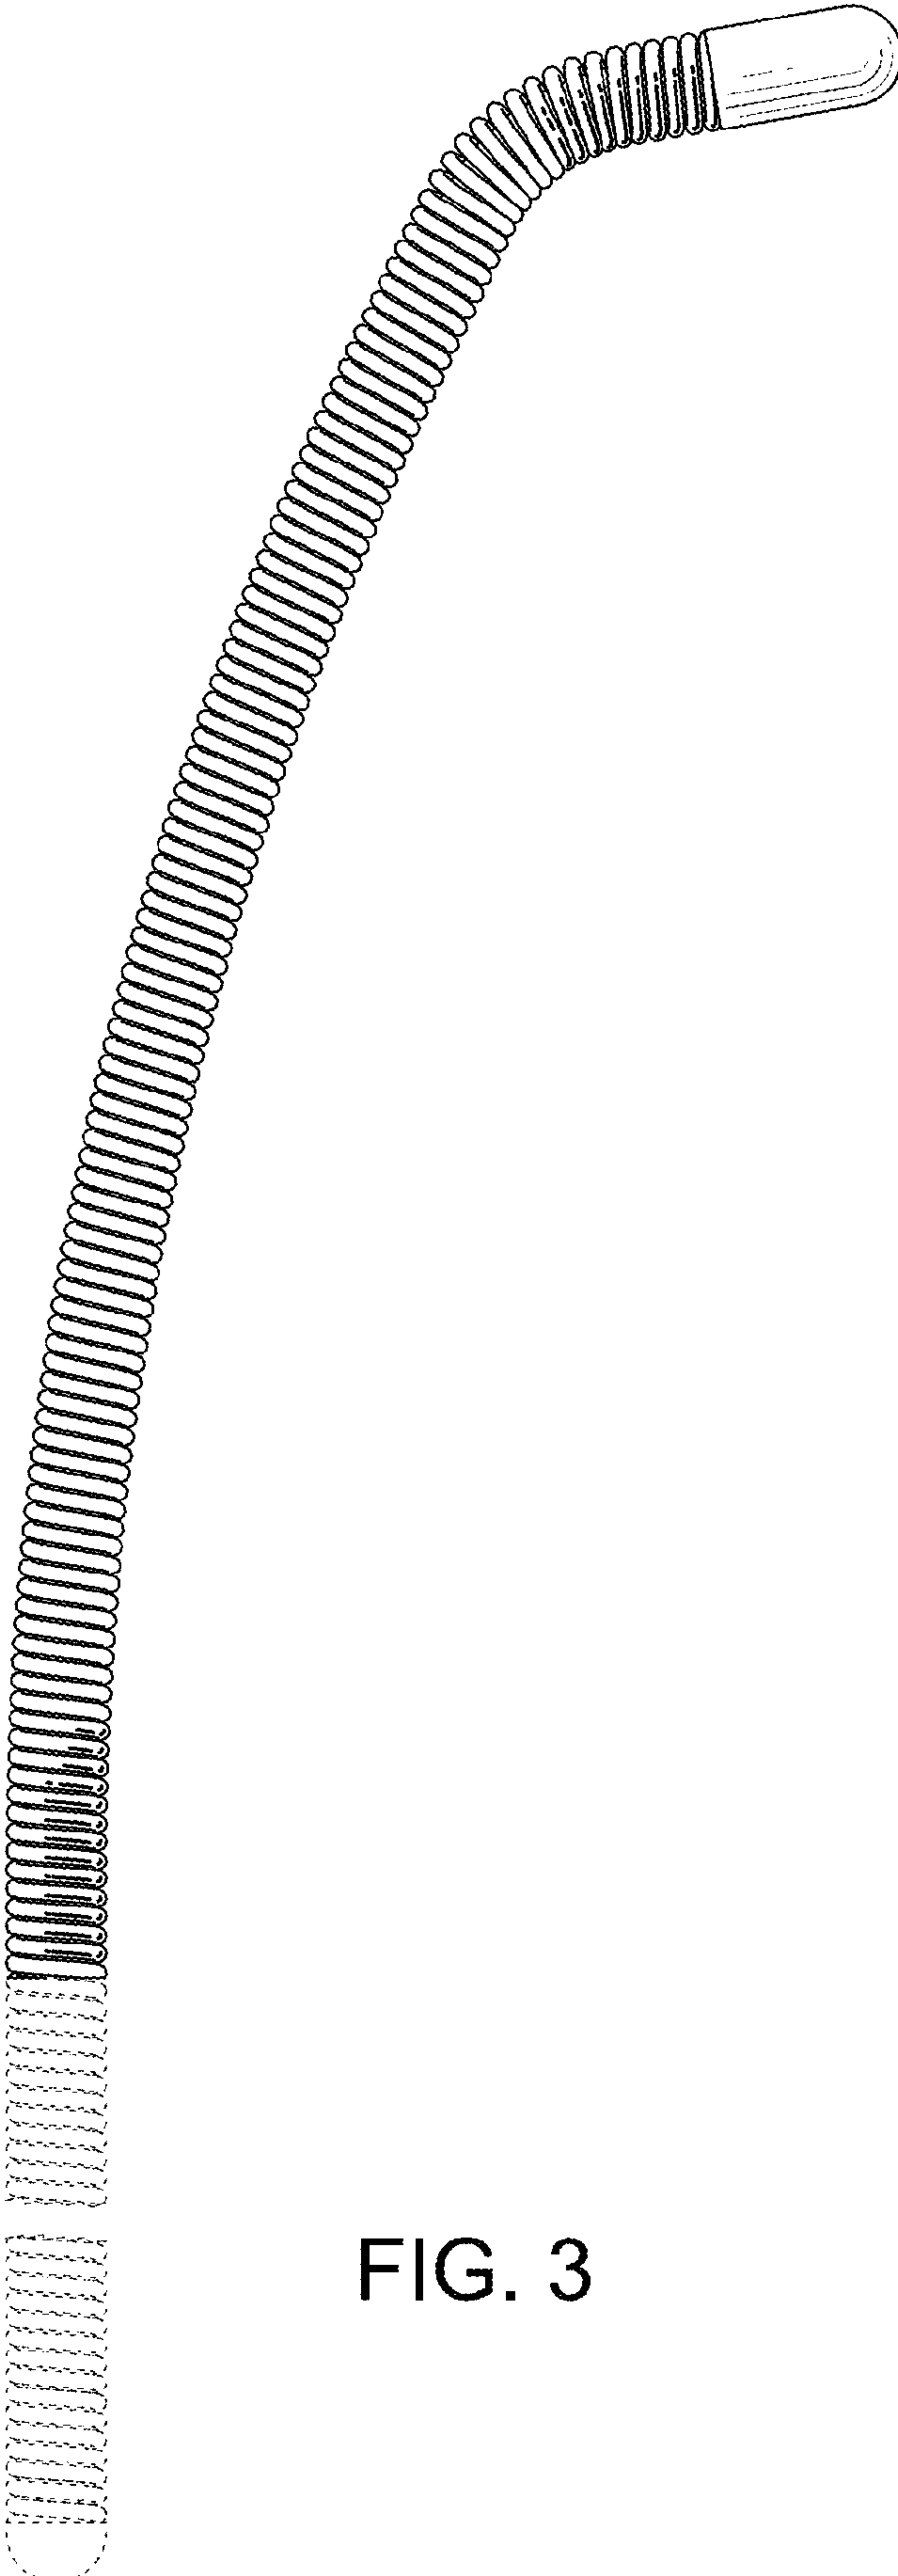


FIG. 3



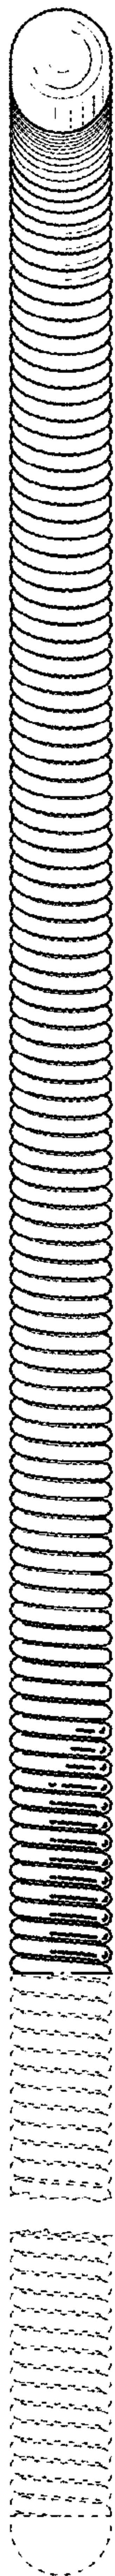


FIG. 4



FIG. 5

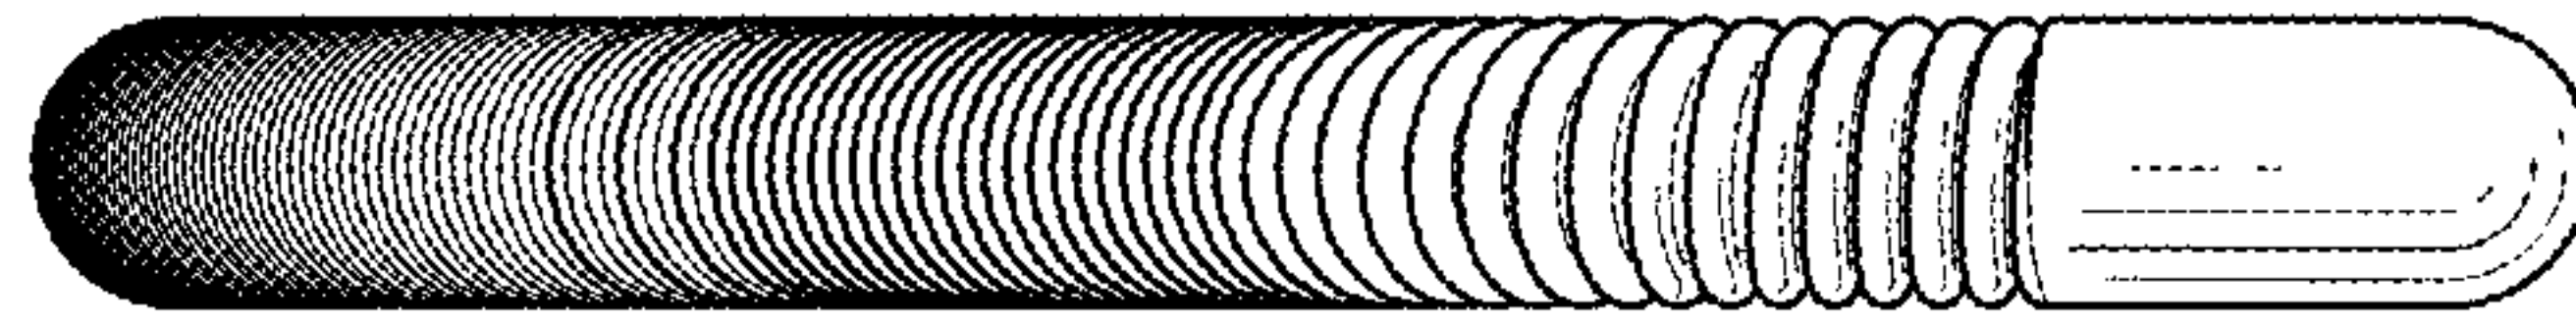


FIG. 6

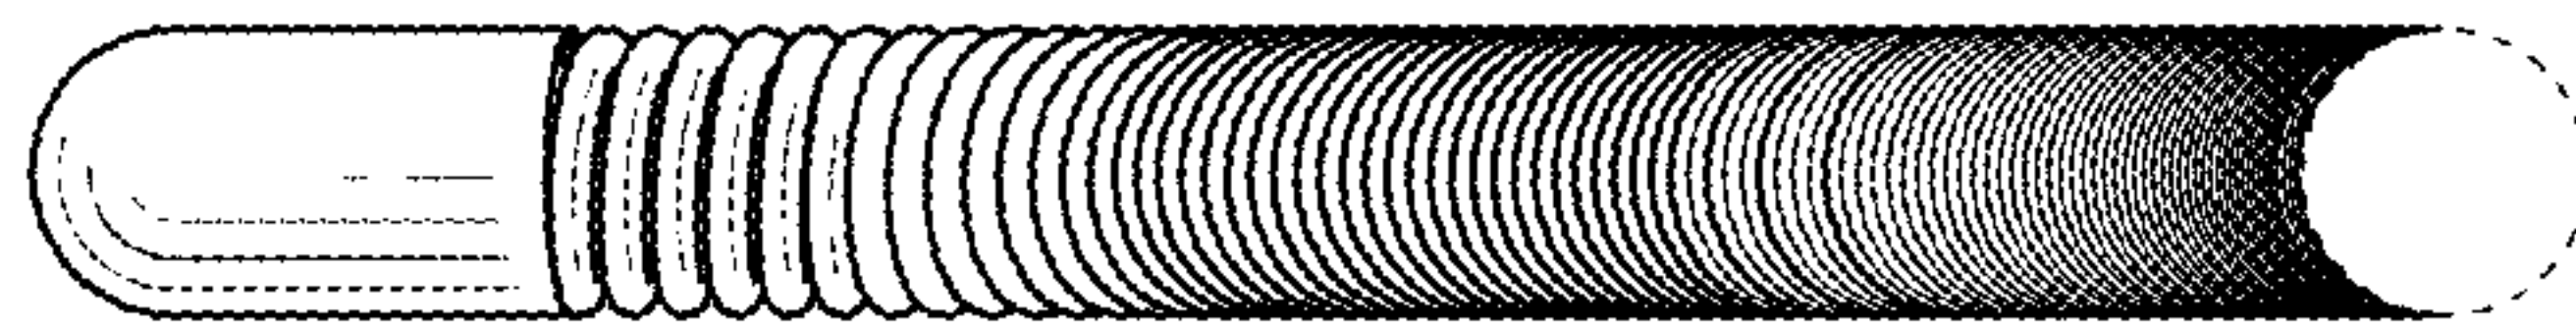


FIG. 7