



US00D943743S

(12) **United States Design Patent**
Kobayashi et al.


(10) **Patent No.:** **US D943,743 S**

(45) **Date of Patent:** **** Feb. 15, 2022**

- (54) **STONE RETRIEVAL BASKET FOR MEDICAL DEVICE**
- (71) Applicant: **OLYMPUS CORPORATION**,
Hachioji (JP)
- (72) Inventors: **Tsukasa Kobayashi**, Hachioji (JP);
Yutaka Yanuma, Hachioji (JP);
Mitsunori Kubo, Hachioji (JP); **Aya Mori**,
Hachioji (JP); **Nao Tsuruta**, Hachioji (JP);
Miho Naka, Hachioji (JP); **Yoshino Nagasuka**,
Hachioji (JP)
- (73) Assignee: **OLYMPUS CORPORATION**,
Hachioji (JP)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/676,841**
- (22) Filed: **Jan. 15, 2019**
- (51) **LOC (13) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/141**
- (58) **Field of Classification Search**
USPC D24/107, 112, 133, 135, 138, 141, 144,
D24/227, 228, 231; 606/46, 113, 114;
D7/213, 368, 380, 690
CPC A61B 17/221; A61B 2017/2212; A61B
2017/2215; A61B 2017/2217; A61B
1/0008; A61B 1/00085; A61B 1/00101
See application file for complete search history.

- (56) **References Cited**
U.S. PATENT DOCUMENTS
4,347,846 A * 9/1982 Dormia A61B 17/221
606/127
5,057,114 A * 10/1991 Wittich A61B 17/221
606/127
5,496,330 A * 3/1996 Bates A61B 17/221
606/127

- 6,187,017 B1 * 2/2001 Gregory, Jr. A61B 17/221
606/127
- 6,190,394 B1 * 2/2001 Lind A61B 17/221
606/127
- 6,656,191 B2 * 12/2003 Ouchi A61B 17/221
606/113
- 7,004,954 B1 2/2006 Larry et al.
- D684,437 S * 6/2013 Joseph D7/690
- D730,705 S * 6/2015 Brown D7/690
- 10,105,154 B1 * 10/2018 Green A61B 5/6858
- 10,117,661 B2 * 11/2018 Lippitt A61B 17/221
- D864,662 S * 10/2019 Sorensen D7/412
- D875,470 S * 2/2020 Sorensen D7/412
- D876,164 S * 2/2020 Sorensen D7/412
- D876,165 S * 2/2020 Sorensen D7/412
- 10,973,539 B2 * 4/2021 Green A61B 17/221
- 2002/0068944 A1 * 6/2002 White A61B 17/221
606/114
- 2003/0088254 A1 * 5/2003 Gregory, Jr. A61B 17/221
606/127
- 2005/0182433 A1 * 8/2005 Nady A61B 17/32056
606/170
- 2007/0260266 A1 * 11/2007 Karpel A61B 17/221
606/127
- 2007/0288037 A1 * 12/2007 Cheng A61B 17/221
606/127
- 2011/0264106 A1 * 10/2011 Taube A61B 17/221
606/113
- 2013/0184738 A1 * 7/2013 Laroya A61F 2/01
606/200
- 2015/0142005 A1 * 5/2015 Taube A61B 90/39
606/113
- 2015/0142009 A1 * 5/2015 Ahn A61B 17/221
606/127
- 2015/0342624 A1 * 12/2015 Lippitt A61B 17/221
606/127
- 2016/0192957 A1 * 7/2016 Okada A61B 17/221
606/127
- 2016/0242795 A1 * 8/2016 Iwabuchi A61B 17/221
- 2016/0256179 A1 * 9/2016 Walsh A61M 25/0074
- 2018/0280042 A1 * 10/2018 Okada A61B 17/00234
- 2019/0000500 A1 * 1/2019 Masubuchi A61B 17/320758
- 2019/0133618 A1 * 5/2019 Green A61B 17/221
- 2019/0151615 A1 * 5/2019 Kitaoka A61B 17/34
- 2020/0078031 A1 * 3/2020 Bonneau A61B 1/307
- 2020/0197094 A1 * 6/2020 Fan A61B 18/26
- 2021/0085161 A1 * 3/2021 Roberts A61B 1/00133
- 2021/0085360 A1 * 3/2021 Leon-Yip A61B 17/1204
- 2021/0212708 A1 * 7/2021 Bartholomai A61B 17/221

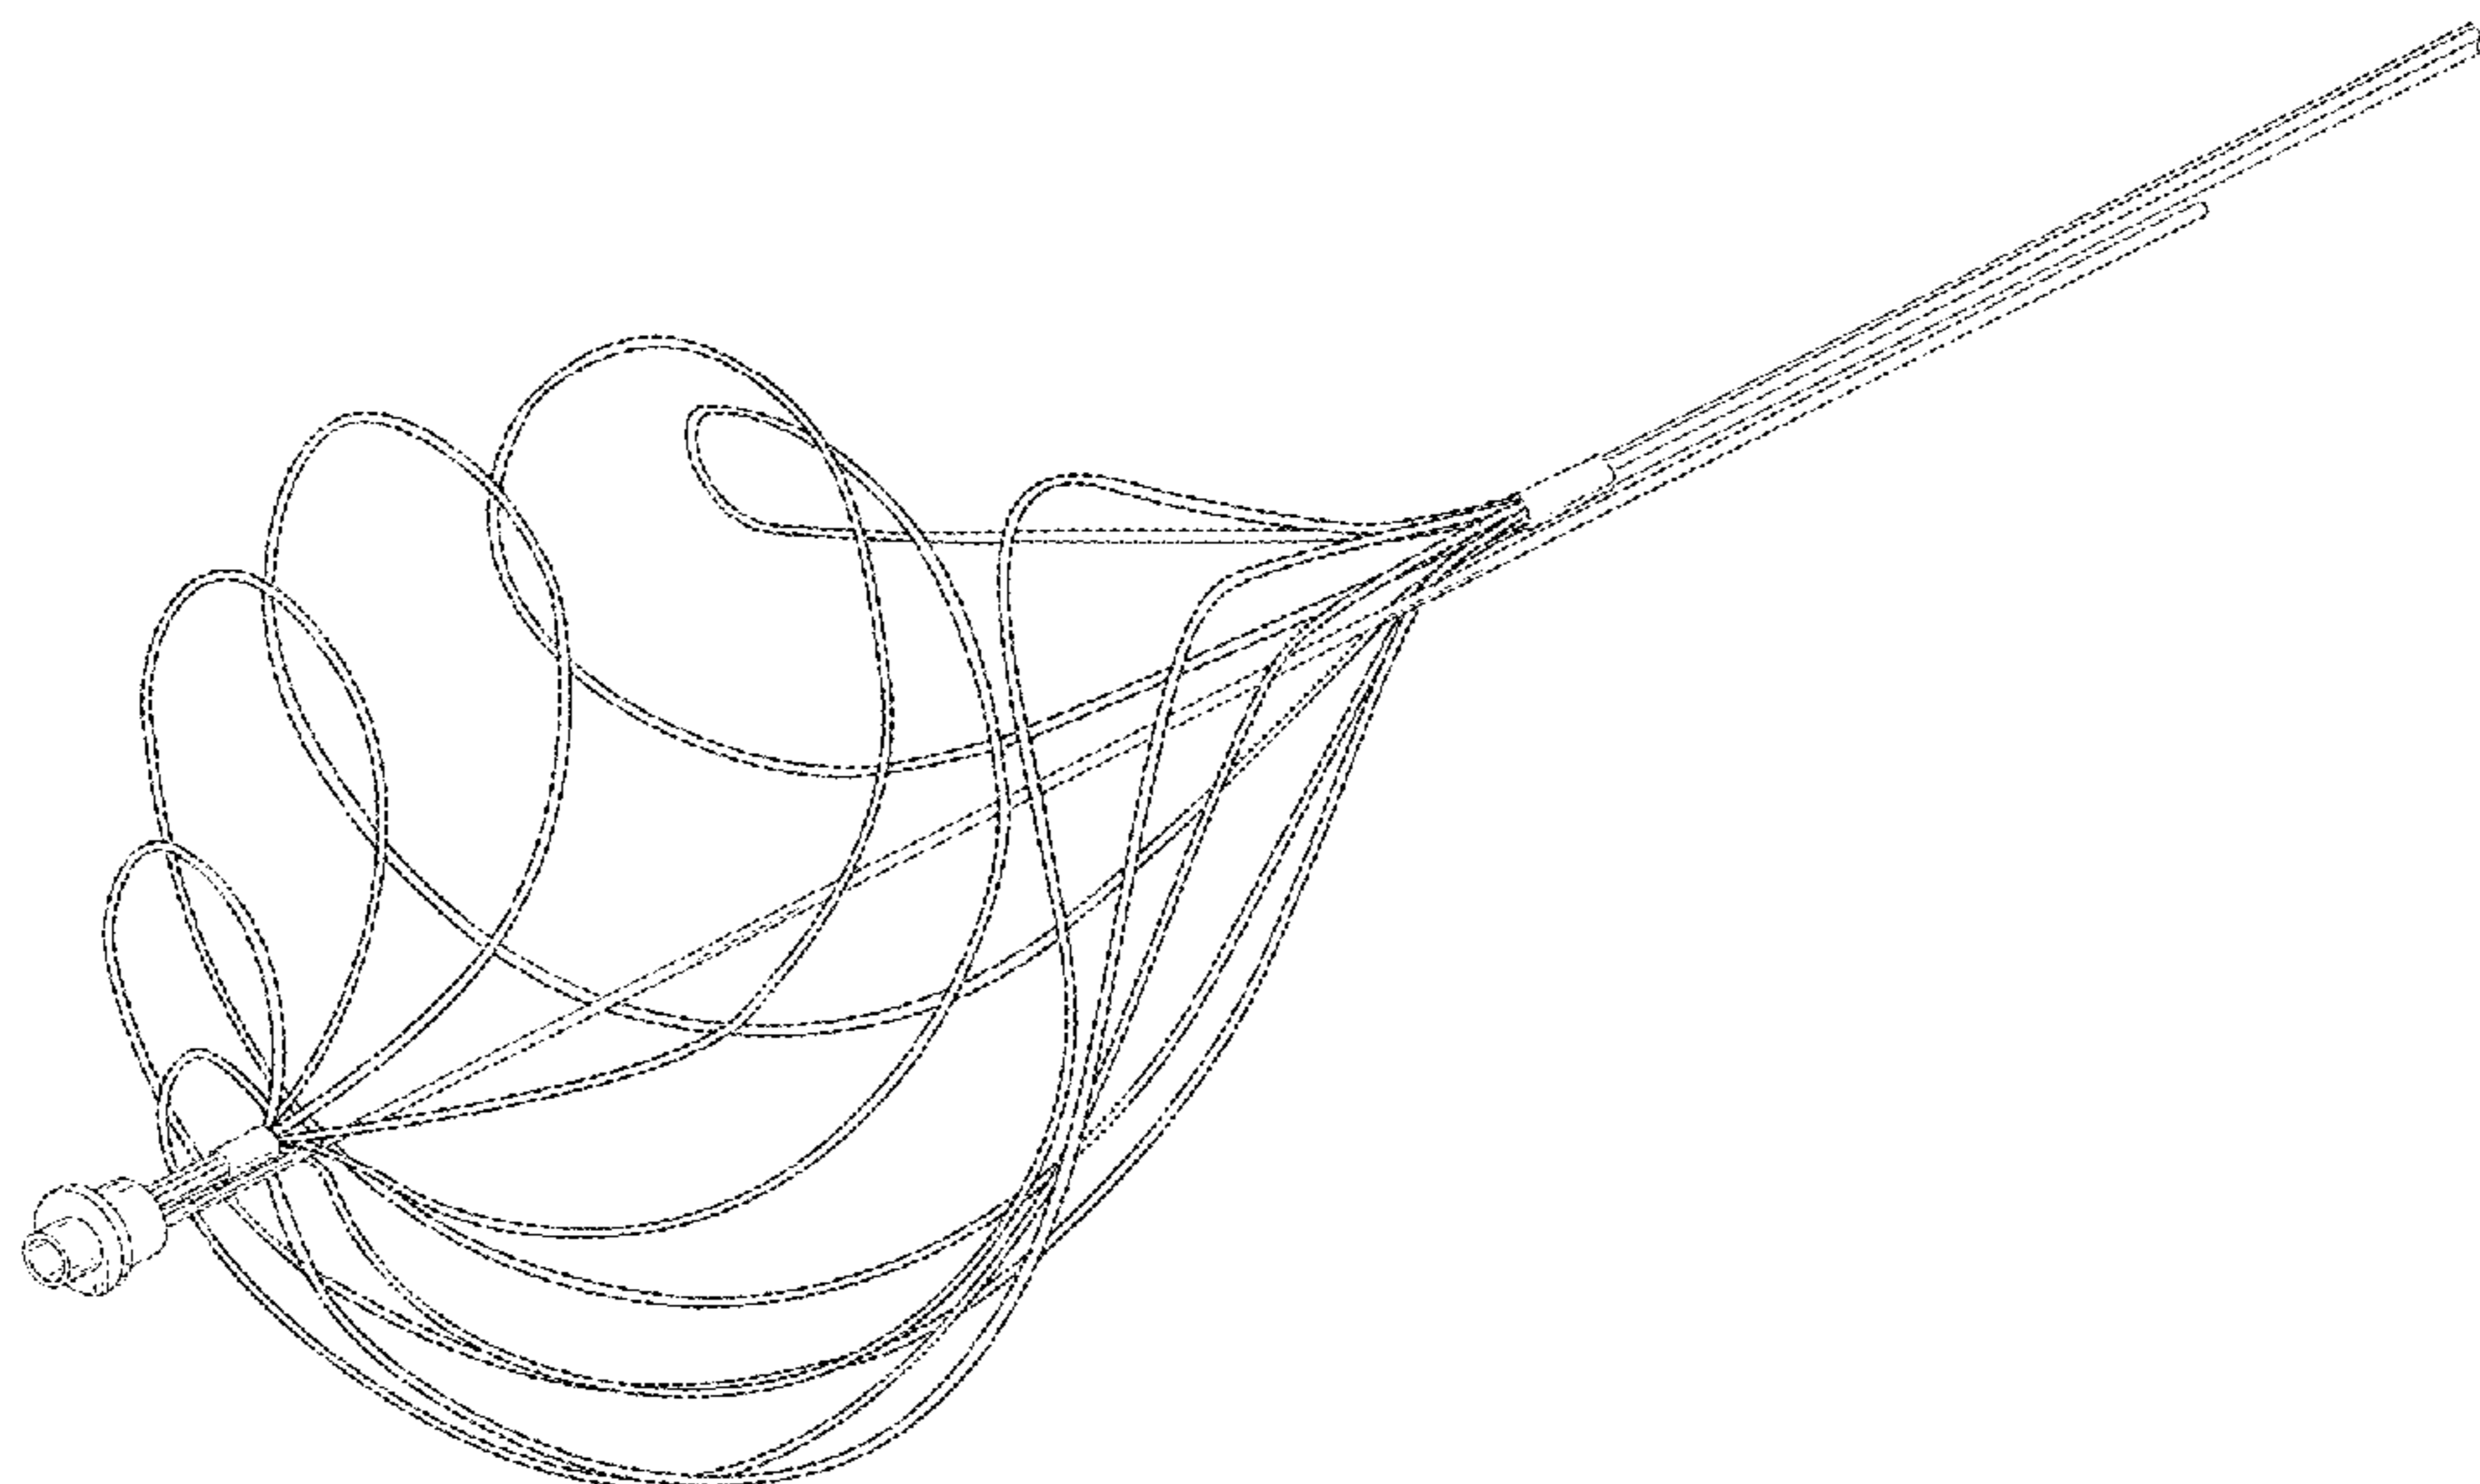

FOREIGN PATENT DOCUMENTS

JP	H10127648 A	5/1998
JP	2003033359 A	2/2003
JP	2004135945 A	5/2004
WO	2012141213 A1	10/2012

OTHER PUBLICATIONS

medical.olympusamerica.com, Retrieved on Dec. 26, 2018, from URL: <http://medical.olympusamerica.com/products/sur-catch-cross-paired-wire-baskets>.

medical.olympusamerica.com, Retrieved on Dec. 26, 2018, from URL: <http://medical.olympusamerica.com/products/sur-catch-nt-no-tip-nitinol-basket>.

www.bostonscientific.com, Retrieved on Jan. 11, 2019, from URL: <http://www.bostonscientific.com/en-US/products/baskets/trapezoid-rx-wireguided-retrieval-basket.html>.

www.cookmedical.com, Retrieved on Dec. 26, 2018, from URL: https://www.cookmedical.com/products/esc_mwbhw_webds/.

www.olympus.co.jp, Published on May 9, 2018, from URL: https://www.olympus.co.jp/news/2018/contents/nr00783/nr00783_00002.pdf.

www.olympuscanada.com, Published in 2005, from URL: http://www.olympuscanada.com/msg_section/ET/files/F1091SB.pdf.

* cited by examiner

Primary Examiner — Clint A Samuel

(74) *Attorney, Agent, or Firm* — Kenja IP Law PC

(57) CLAIM

The ornamental design for a stone retrieval basket for medical device, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a first embodiment of the stone retrieval basket for medical device showing our new design;

FIG. 2 is a front view thereof;

FIG. 3 is a rear view thereof;

FIG. 4 is a left side view thereof;

FIG. 5 is a right side view thereof;

FIG. 6 is a top plan view thereof;

FIG. 7 is a bottom view thereof;

FIG. 8 is a cross-sectional end view thereof taken along the line 8-8 in FIG. 2;

FIG. 9 is a front perspective view of a second embodiment of the stone retrieval basket for medical device showing our new design;

FIG. 10 is a front view thereof;

FIG. 11 is a rear view thereof;

FIG. 12 is a left side view thereof;

FIG. 13 is a right side view thereof;

FIG. 14 is a top plan view thereof;

FIG. 15 is a bottom view thereof;

FIG. 16 is a cross-sectional end view thereof taken along the line 16-16 in FIG. 10;

FIG. 17 is a front perspective view of a third embodiment of the stone retrieval basket for medical device showing our new design;

FIG. 18 is a front view thereof;

FIG. 19 is a rear view thereof;

FIG. 20 is a left side view thereof;

FIG. 21 is a right side view thereof;

FIG. 22 is a top plan view thereof;

FIG. 23 is a bottom view thereof;

FIG. 24 is a cross-sectional end view thereof taken along the line 24-24 in FIG. 18;

FIG. 25 is a front perspective view of a fourth embodiment of the stone retrieval basket for medical device showing our new design;

FIG. 26 is a front view thereof;

FIG. 27 is a rear view thereof;

FIG. 28 is a left side view thereof;

FIG. 29 is a right side view thereof;

FIG. 30 is a top plan view thereof;

FIG. 31 is a bottom view thereof;

FIG. 32 is a cross-sectional end view thereof taken along the line 32-32 in FIG. 26;

FIG. 33 is a front perspective view of a fifth embodiment of the stone retrieval basket for medical device showing our new design;

FIG. 34 is a front view thereof;

FIG. 35 is a rear view thereof;

FIG. 36 is a left side view thereof;

FIG. 37 is a right side view thereof;

FIG. 38 is a top plan view thereof;

FIG. 39 is a bottom view thereof;

FIG. 40 is a cross-sectional end view thereof taken along the line 40-40 in FIG. 34;

FIG. 41 is a cross-sectional end view thereof taken along the line 41-41 in FIG. 34;

FIG. 42 is a front perspective view of a sixth embodiment of the stone retrieval basket for medical device showing our new design;

FIG. 43 is a front view thereof;

FIG. 44 is a rear view thereof;

FIG. 45 is a left side view thereof;

FIG. 46 is a right side view thereof;

FIG. 47 is a top plan view thereof;

FIG. 48 is a bottom view thereof;

FIG. 49 is a cross-sectional end view thereof taken along the line 49-49 in FIG. 43;

FIG. 50 is a front perspective view of a seventh embodiment of the stone retrieval basket for medical device showing our new design;

FIG. 51 is a front view thereof, a rearview, a top view, a bottom view being the same image thereof;

FIG. 52 is a left side view thereof;

FIG. 53 is a right side view thereof;

FIG. 54 is a cross-sectional end view thereof taken along the line 54-54 in FIG. 51;

FIG. 55 is a front perspective view of an eighth embodiment of the stone retrieval basket for medical device showing our new design;

FIG. 56 is a front view thereof;

FIG. 57 is a rear view thereof;

FIG. 58 is a left side view thereof;

FIG. 59 is a right side view thereof;

FIG. 60 is a top plan view thereof;

FIG. 61 is a bottom view thereof; and,

FIG. 62 is a cross-sectional end view thereof taken along the line 62-62 in FIG. 56.

FIG. 1

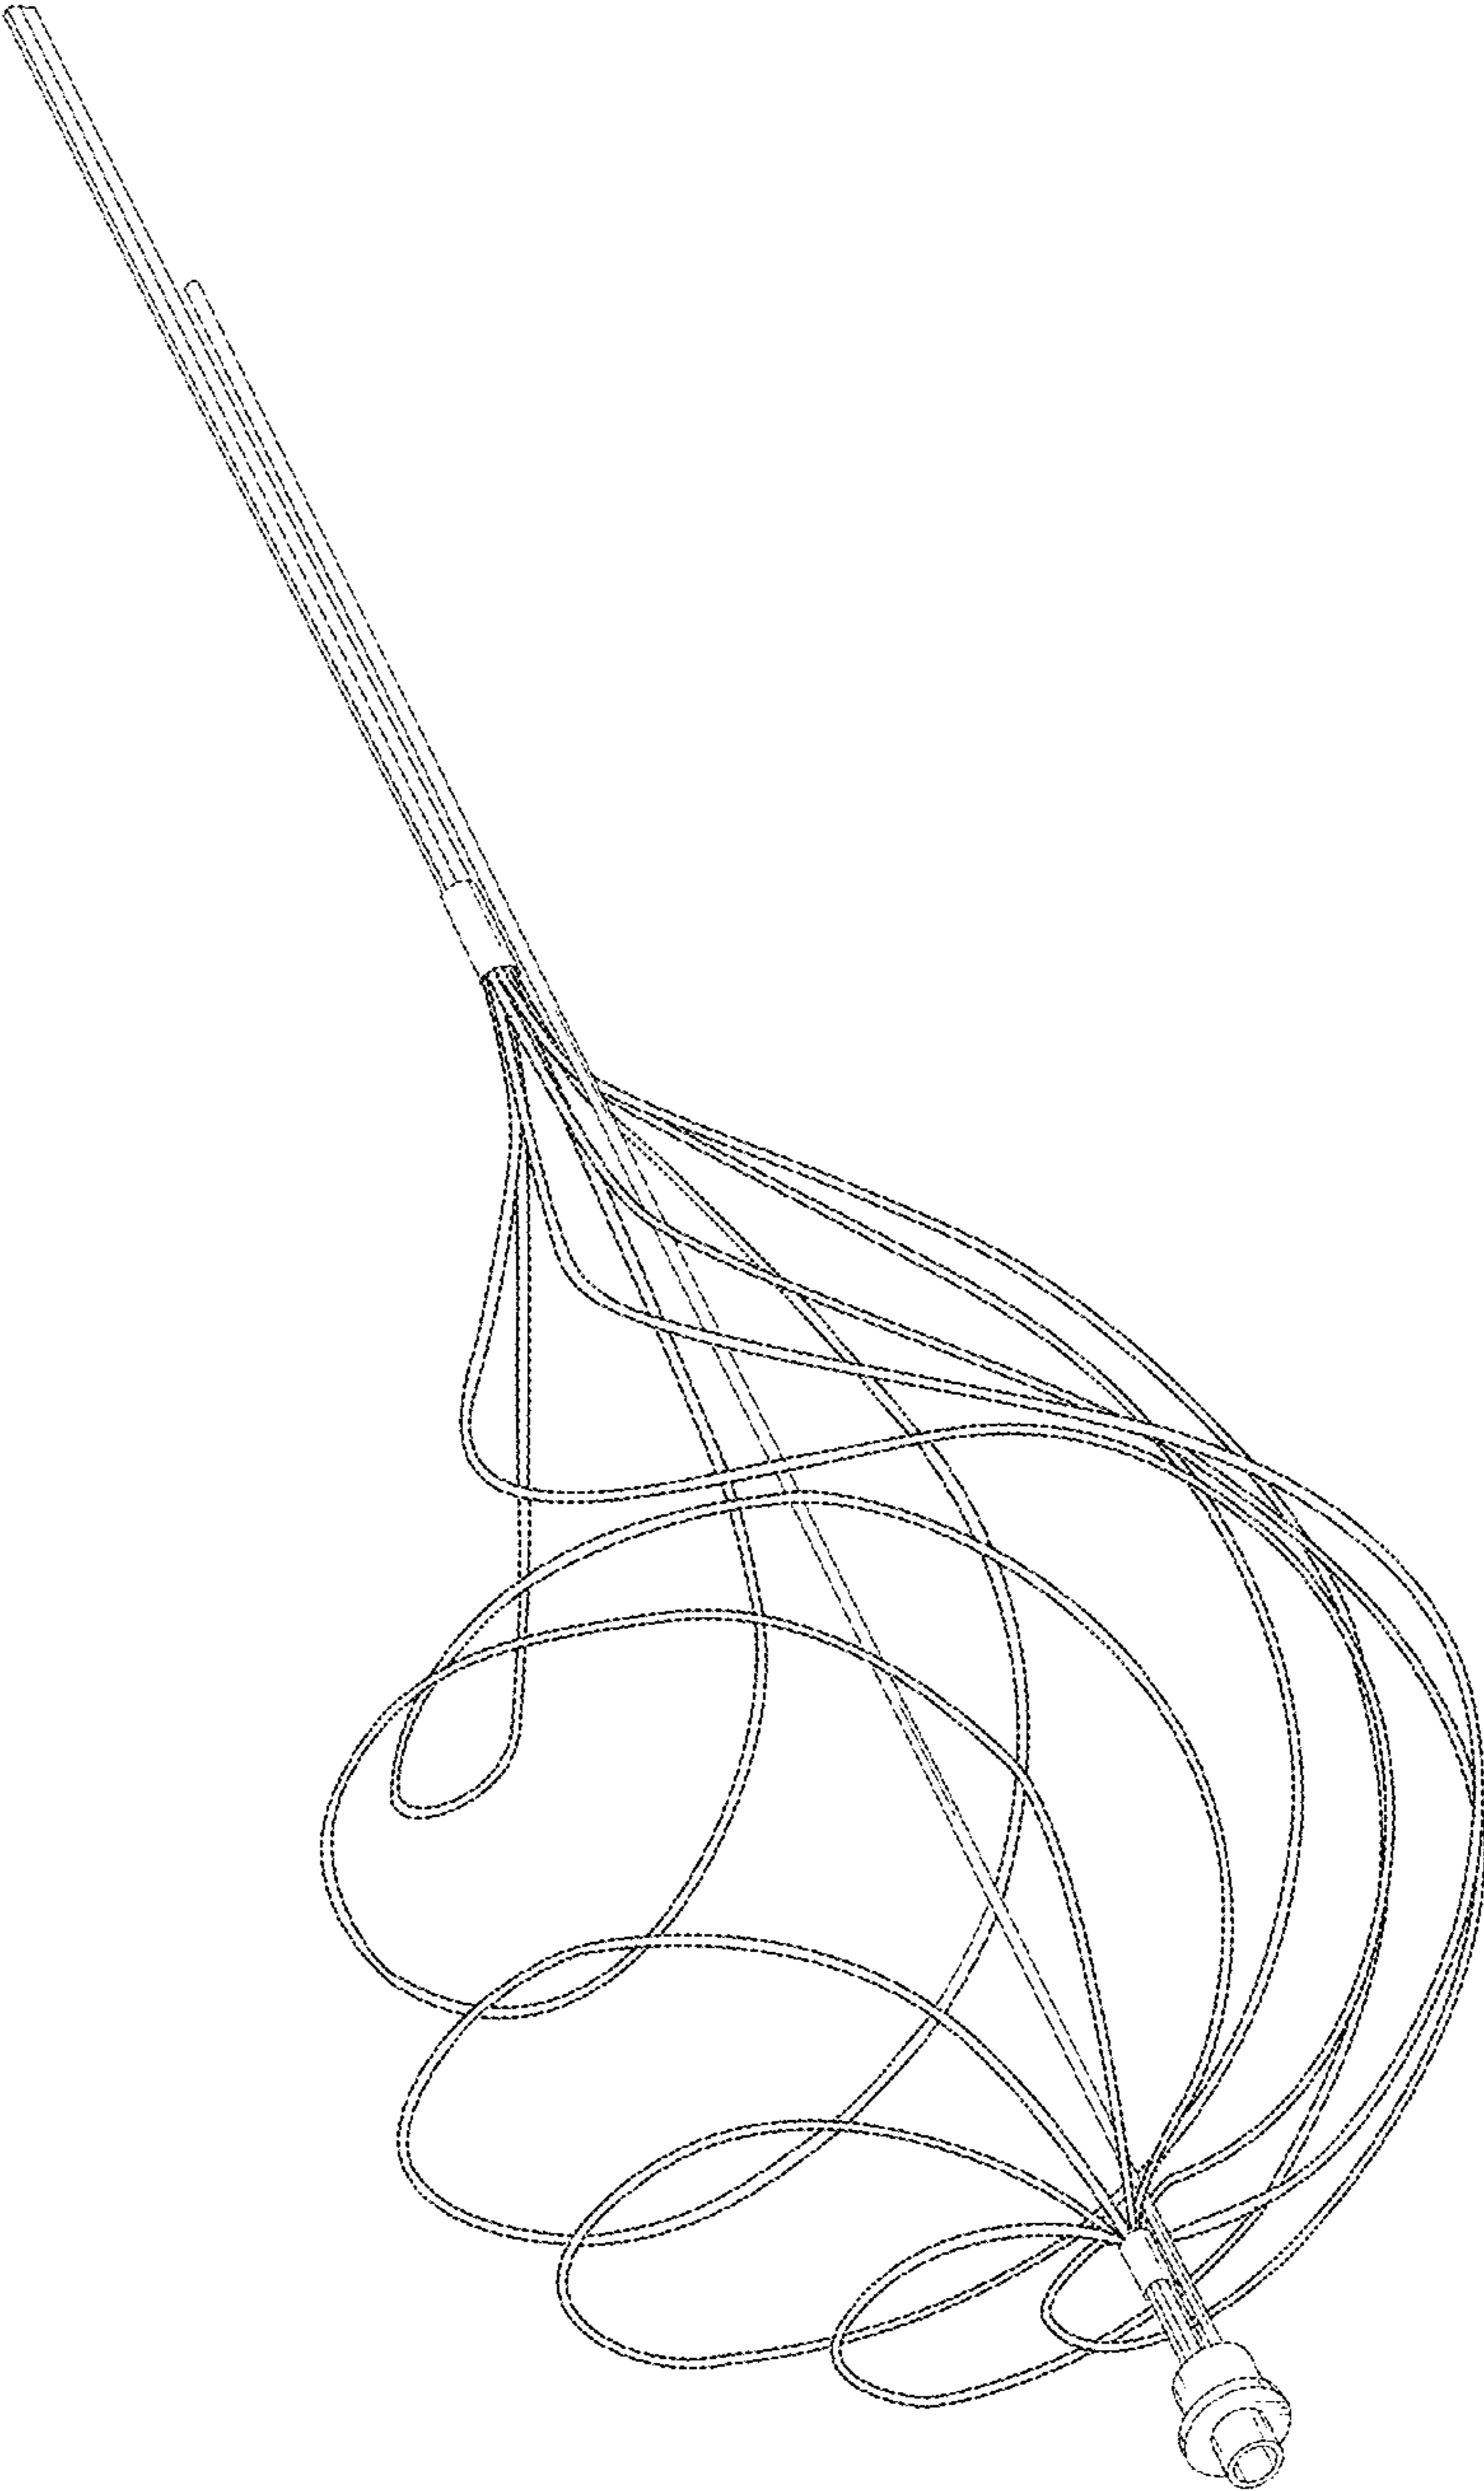


FIG. 2

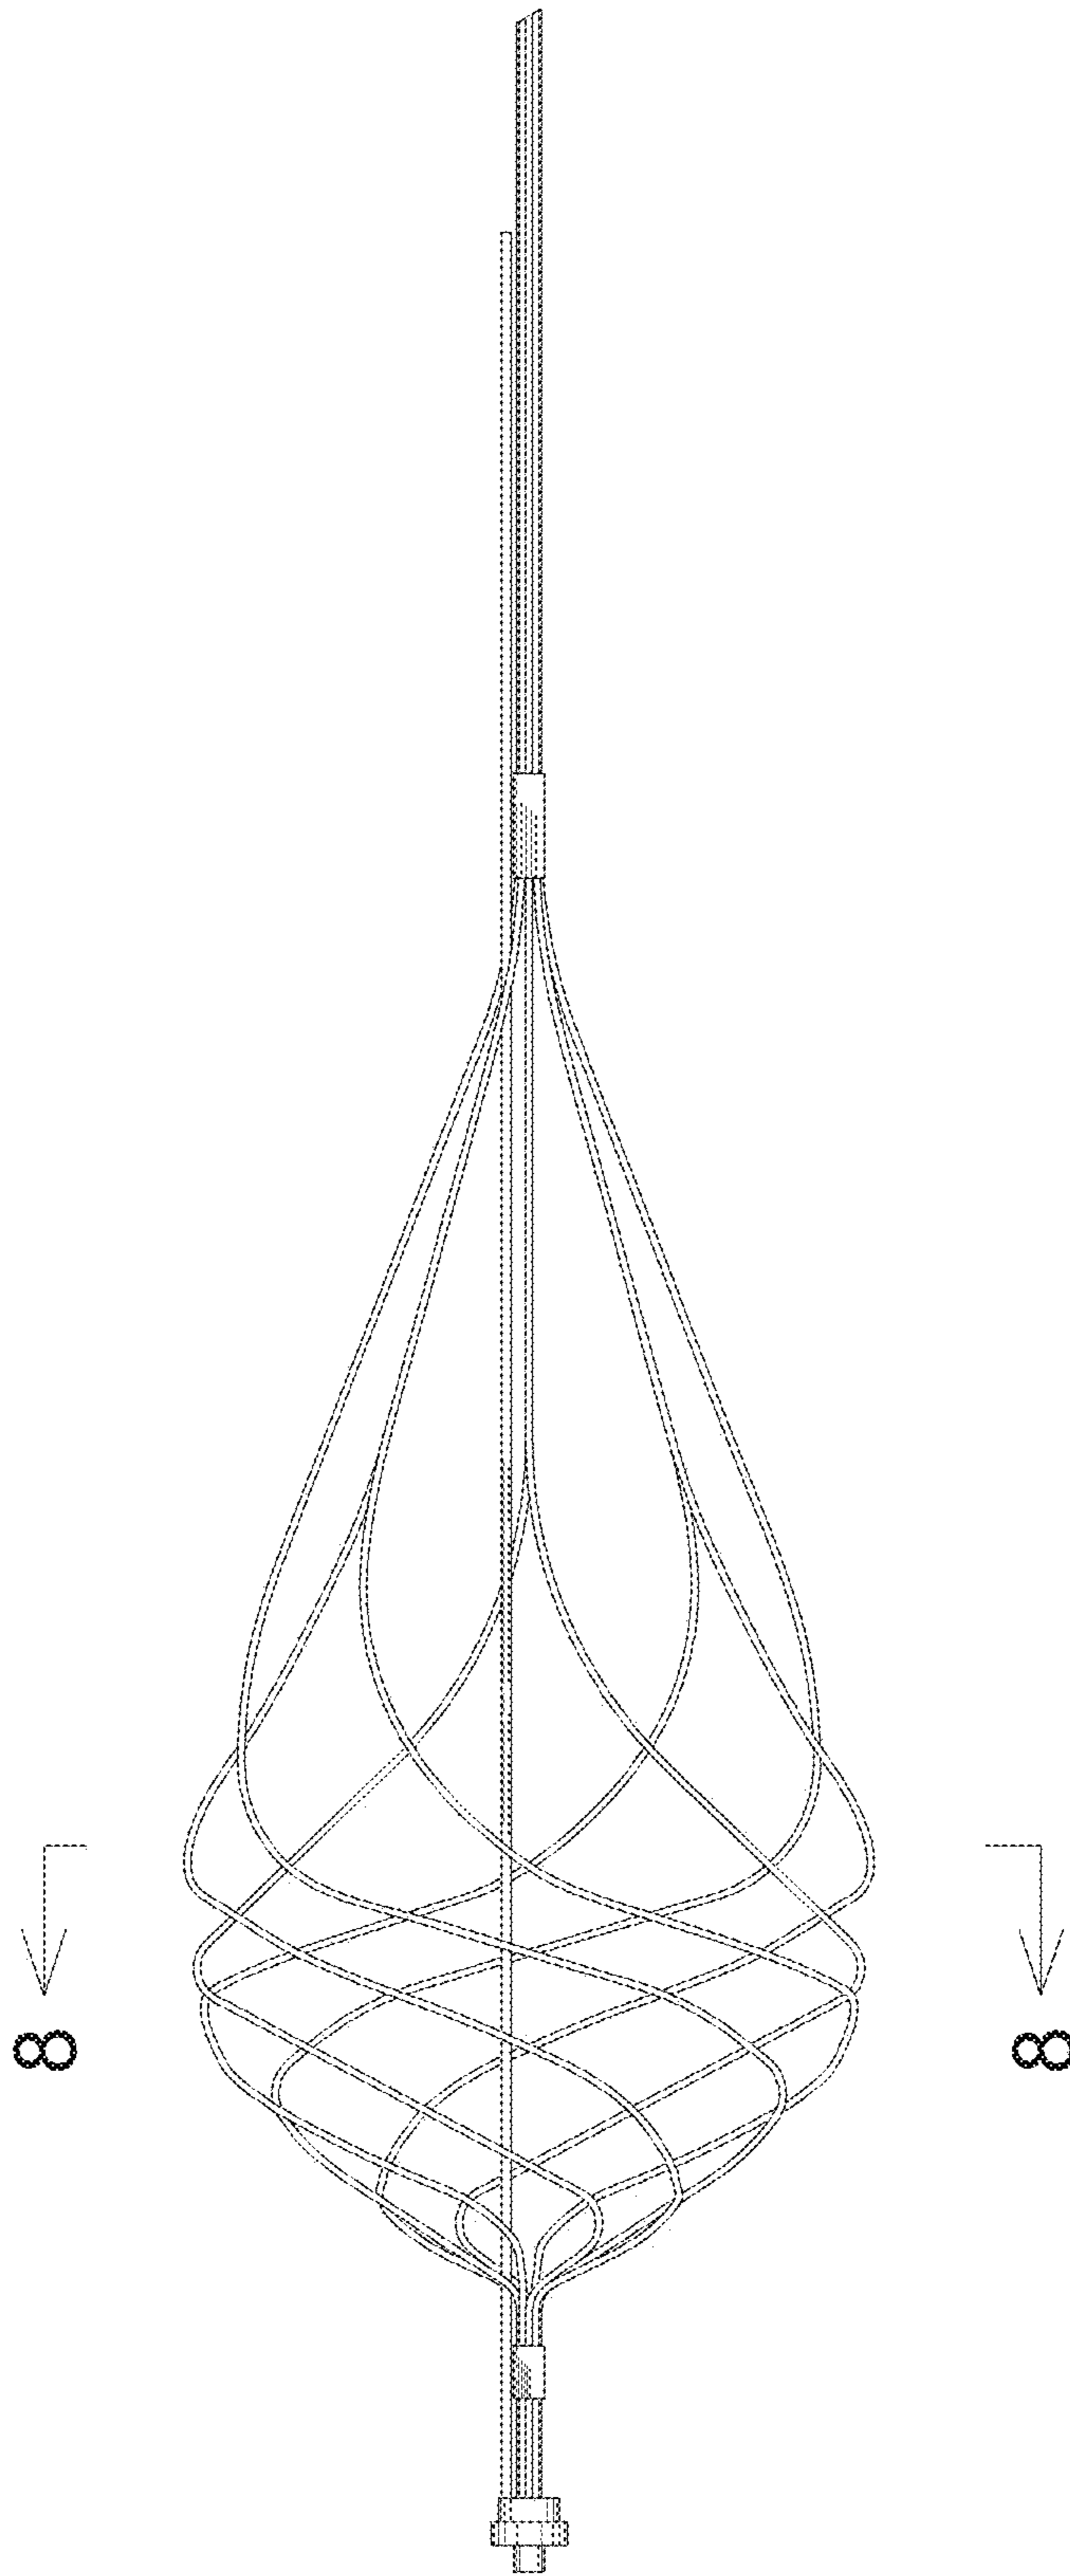


FIG. 3

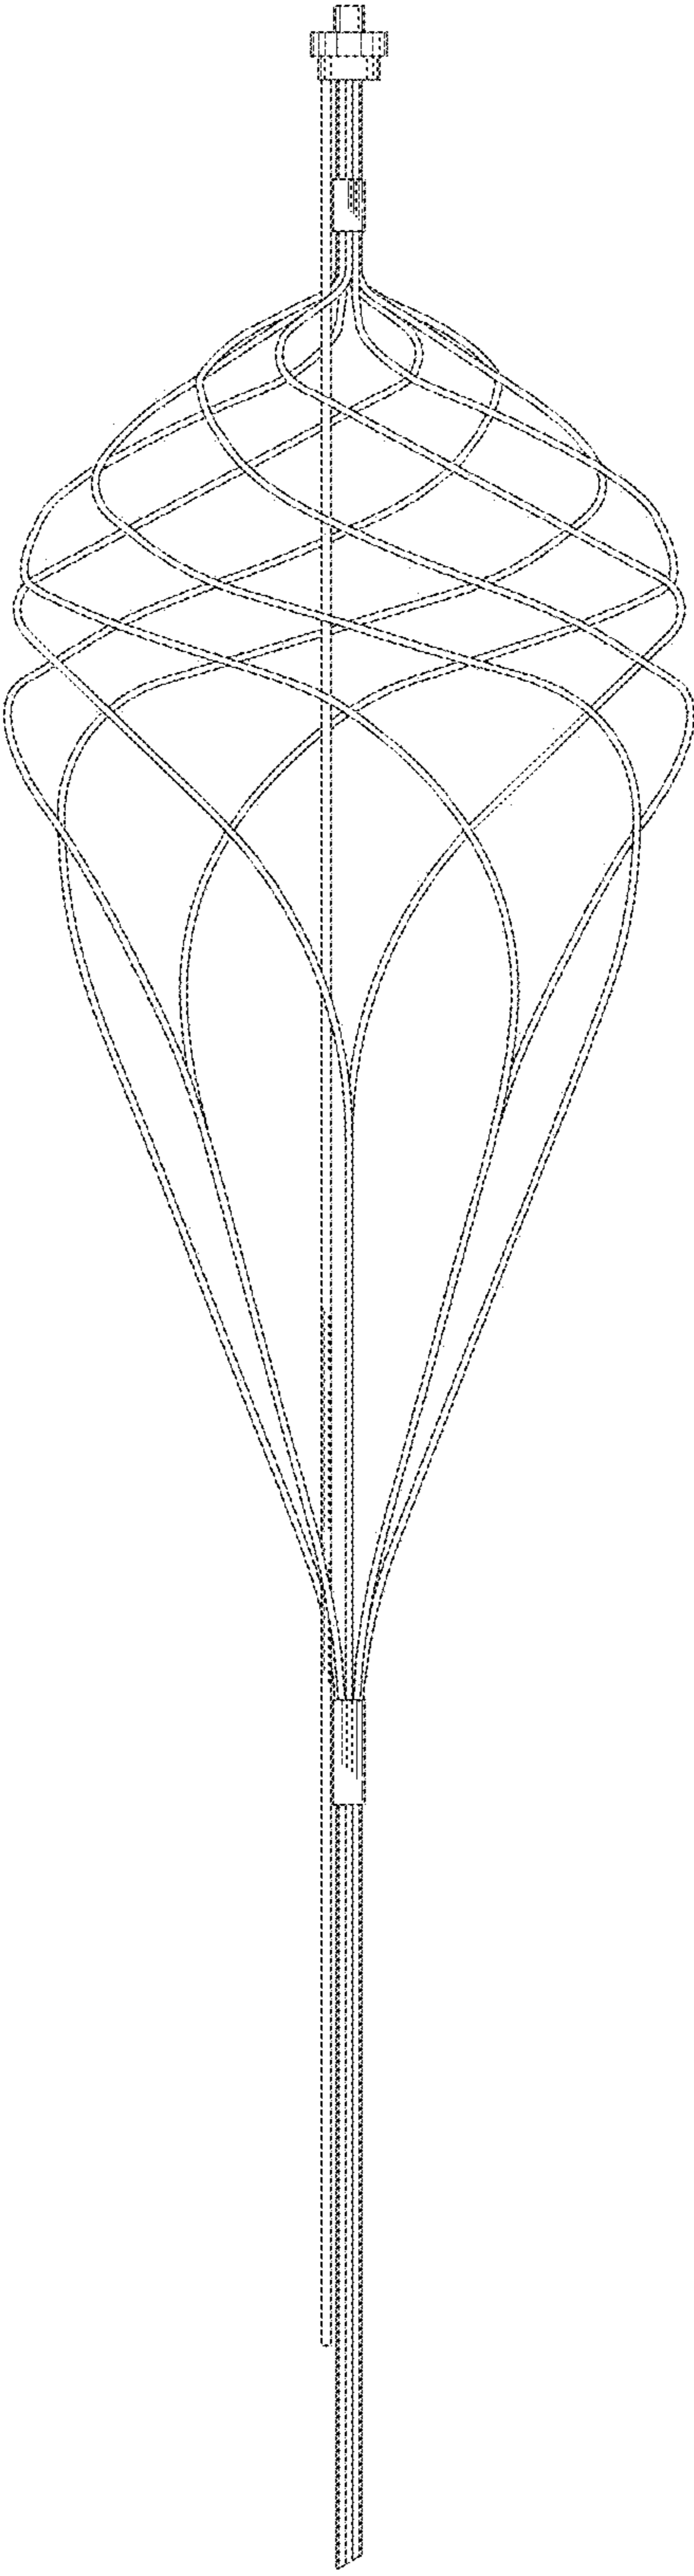


FIG. 4

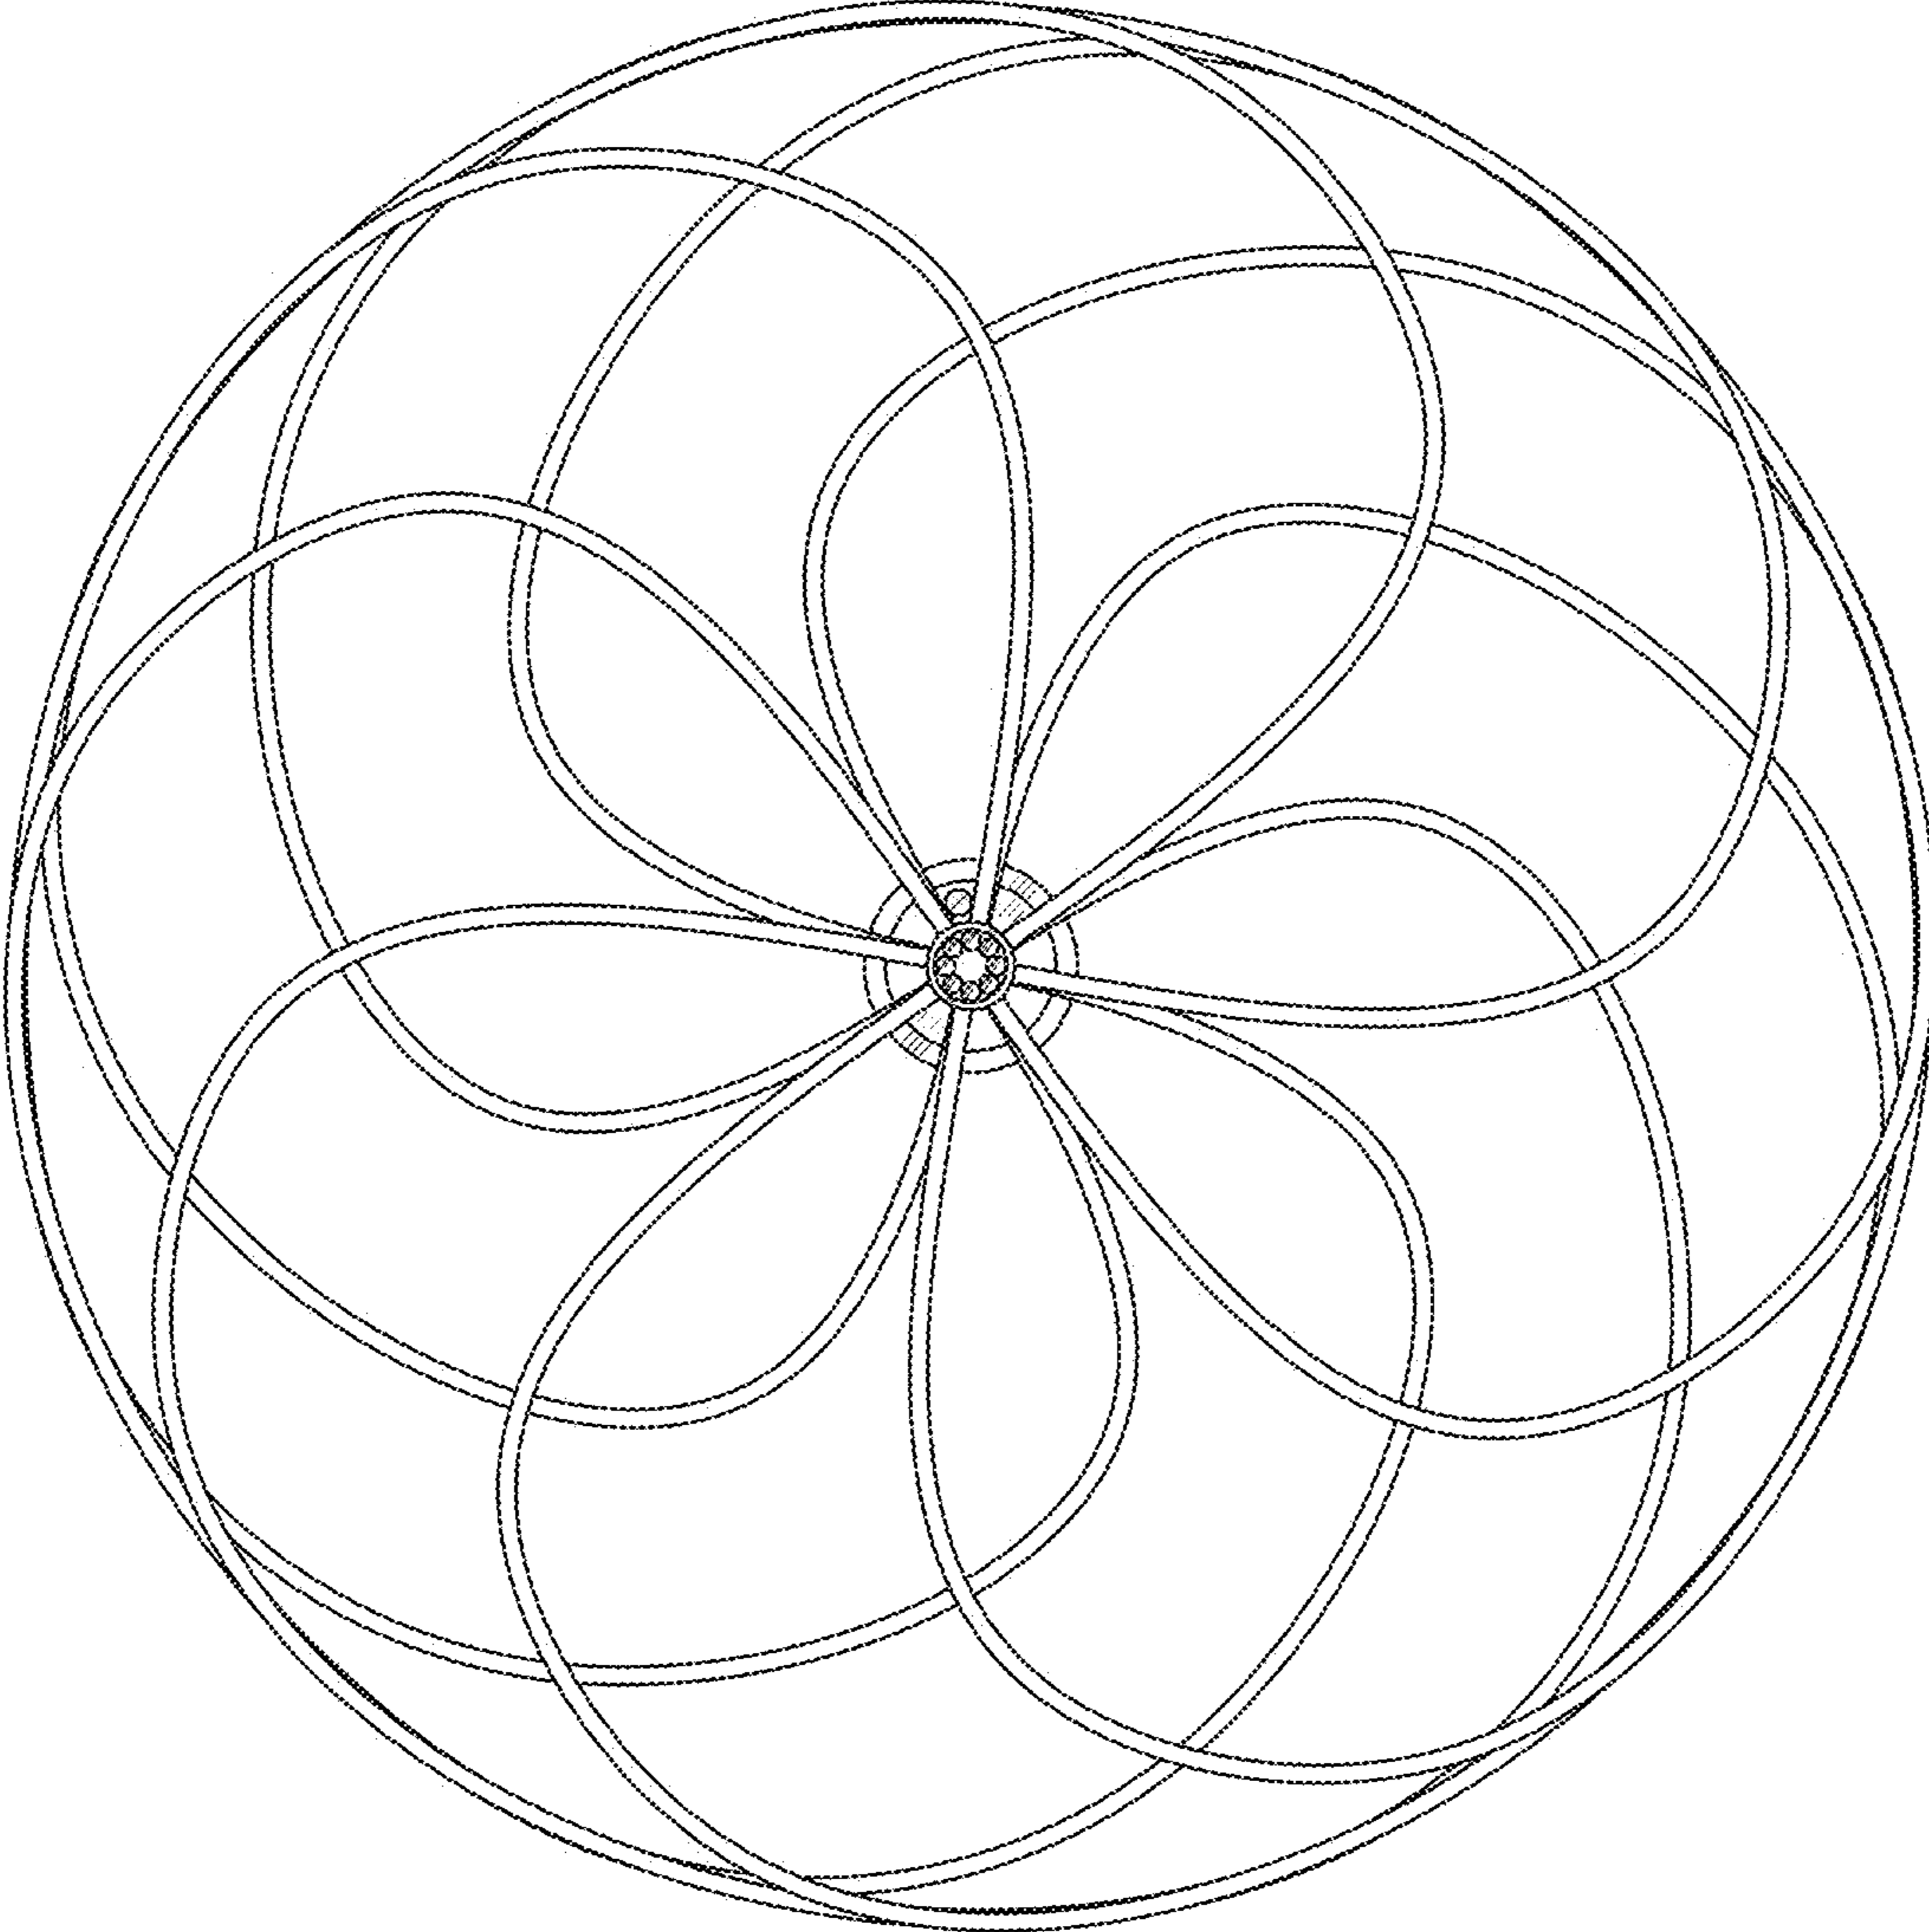


FIG. 5

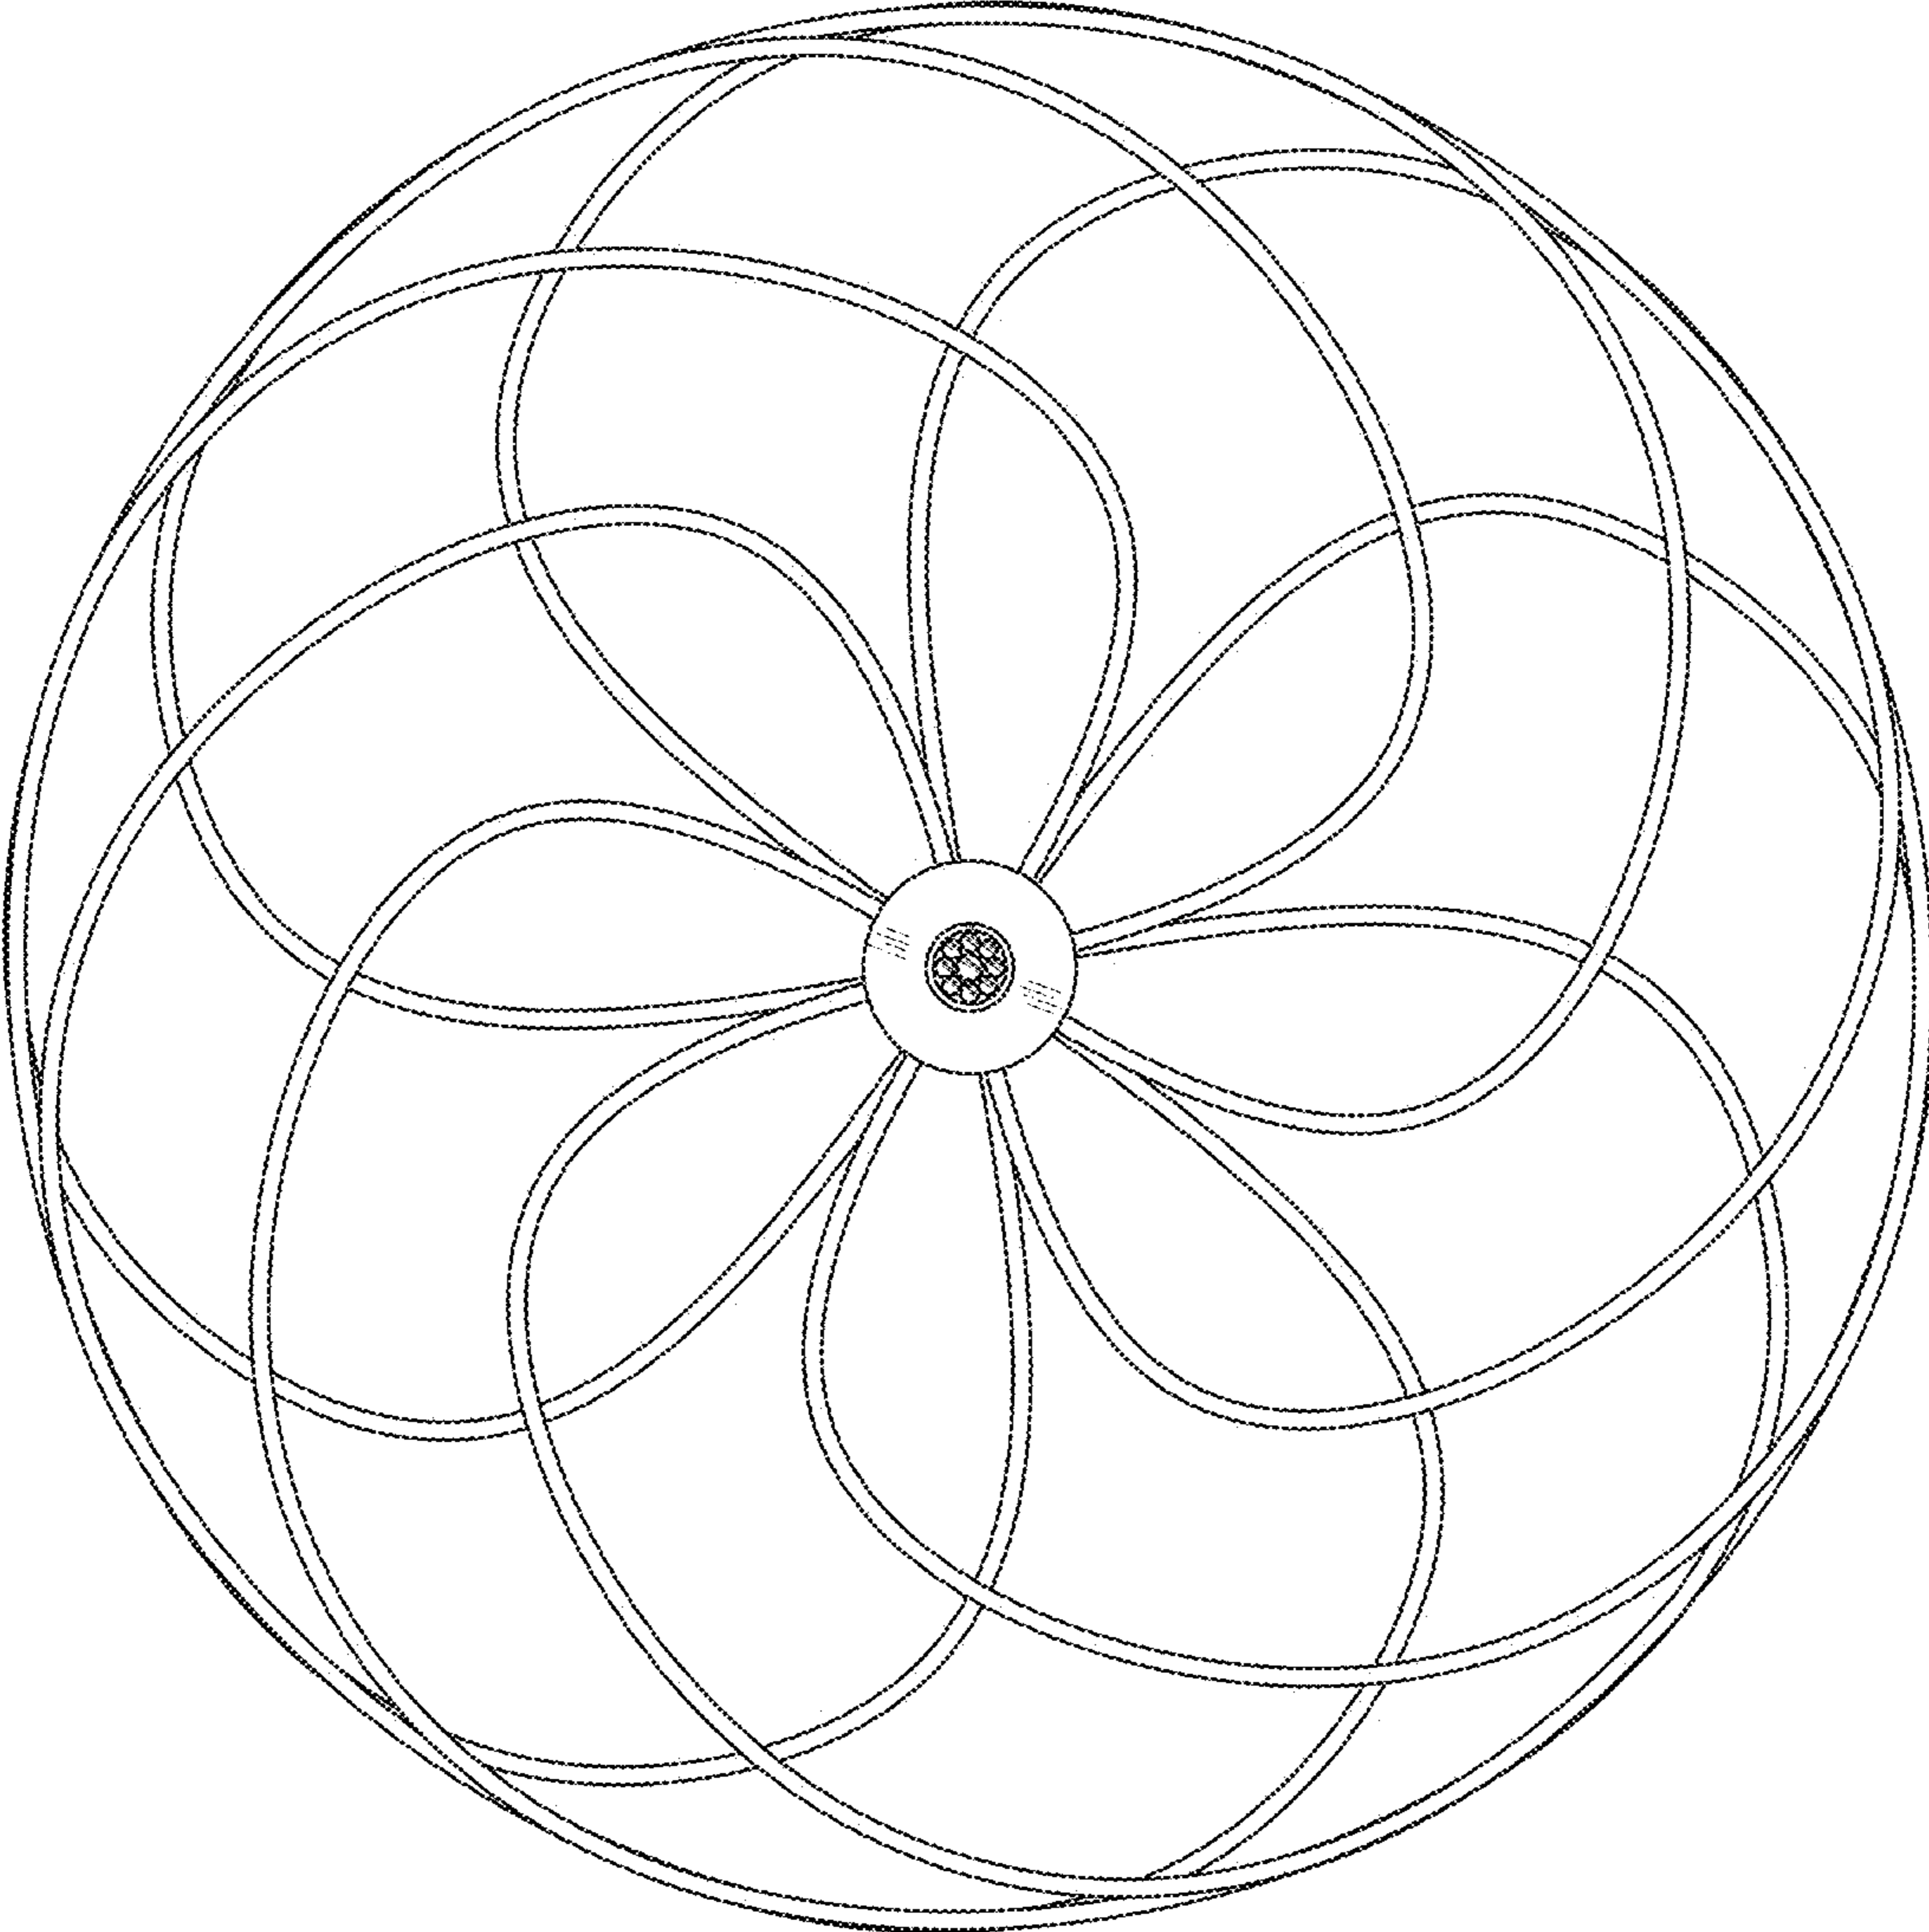


FIG. 6

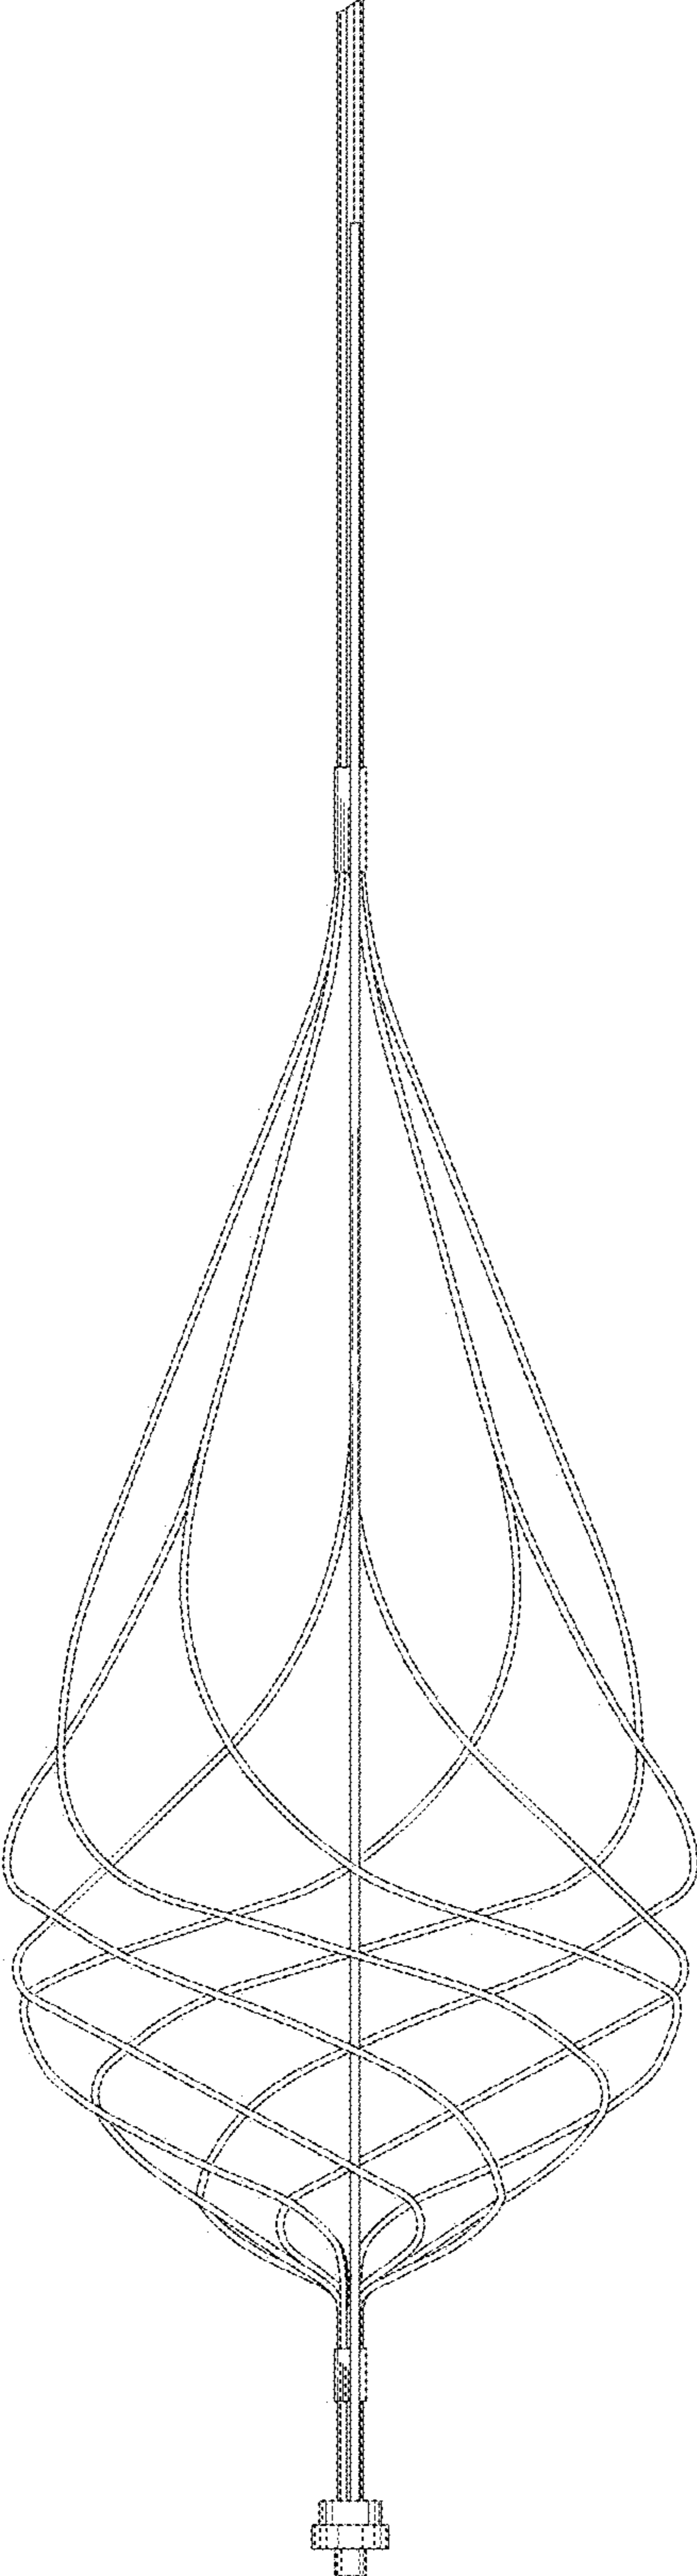


FIG. 7

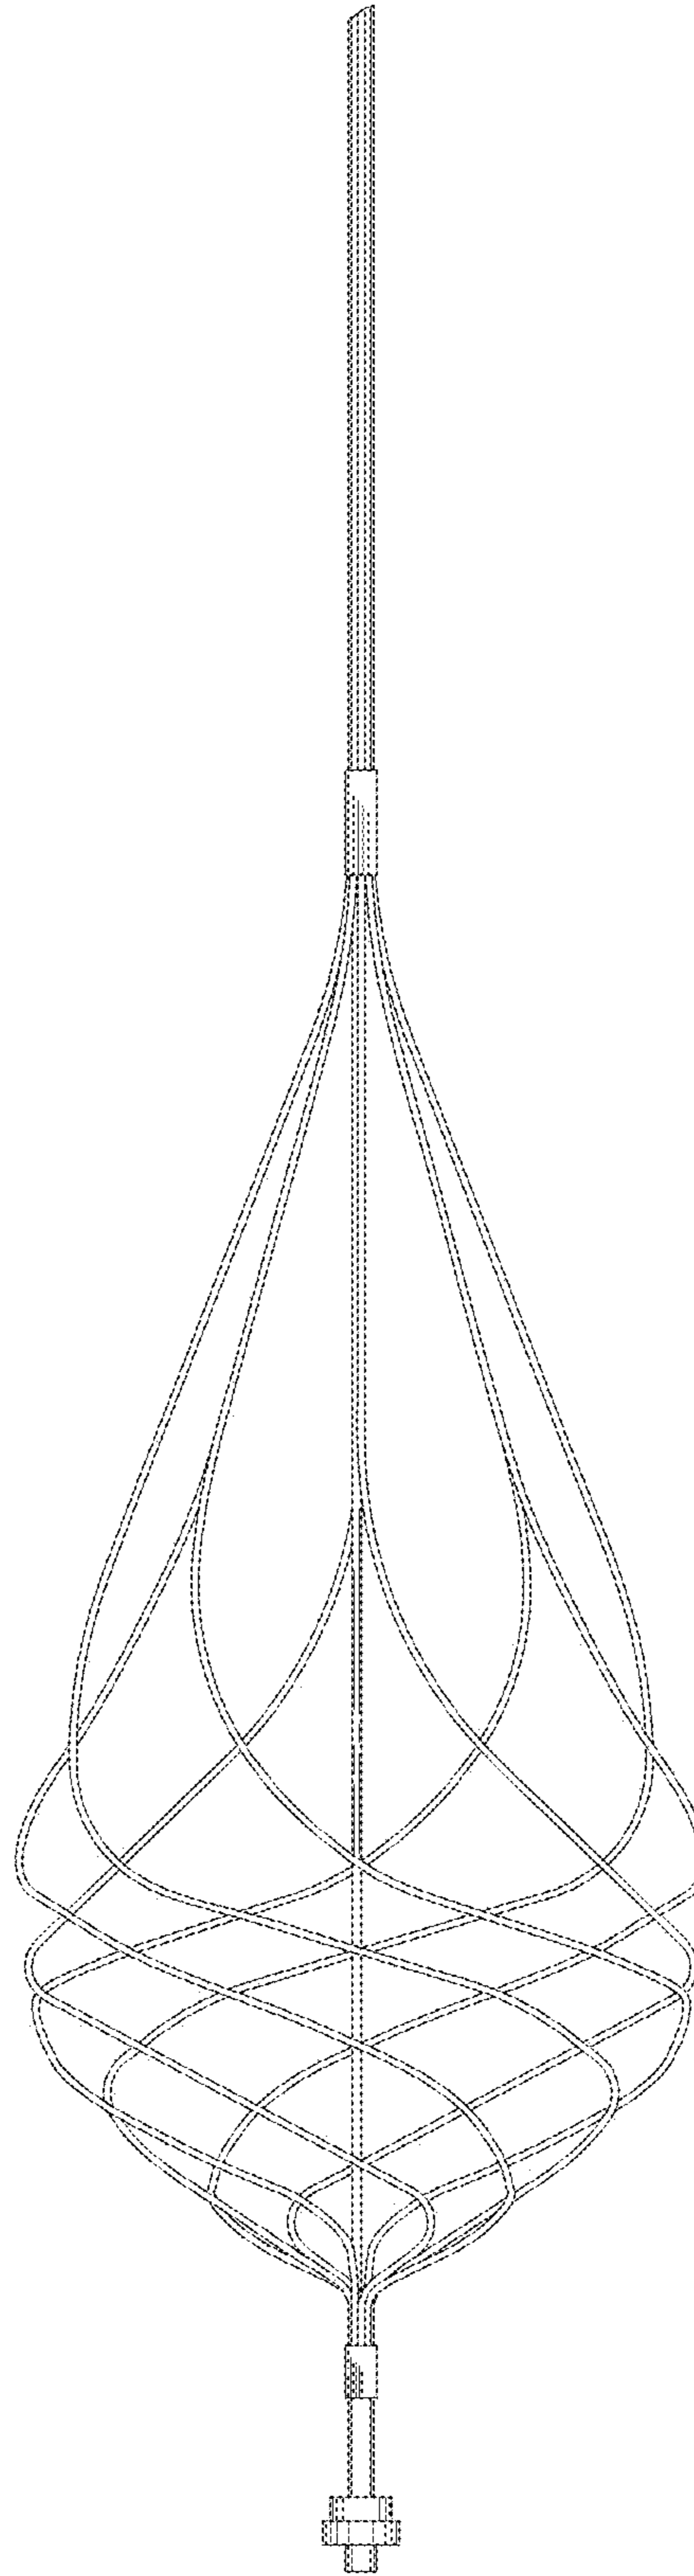


FIG. 8




FIG. 9

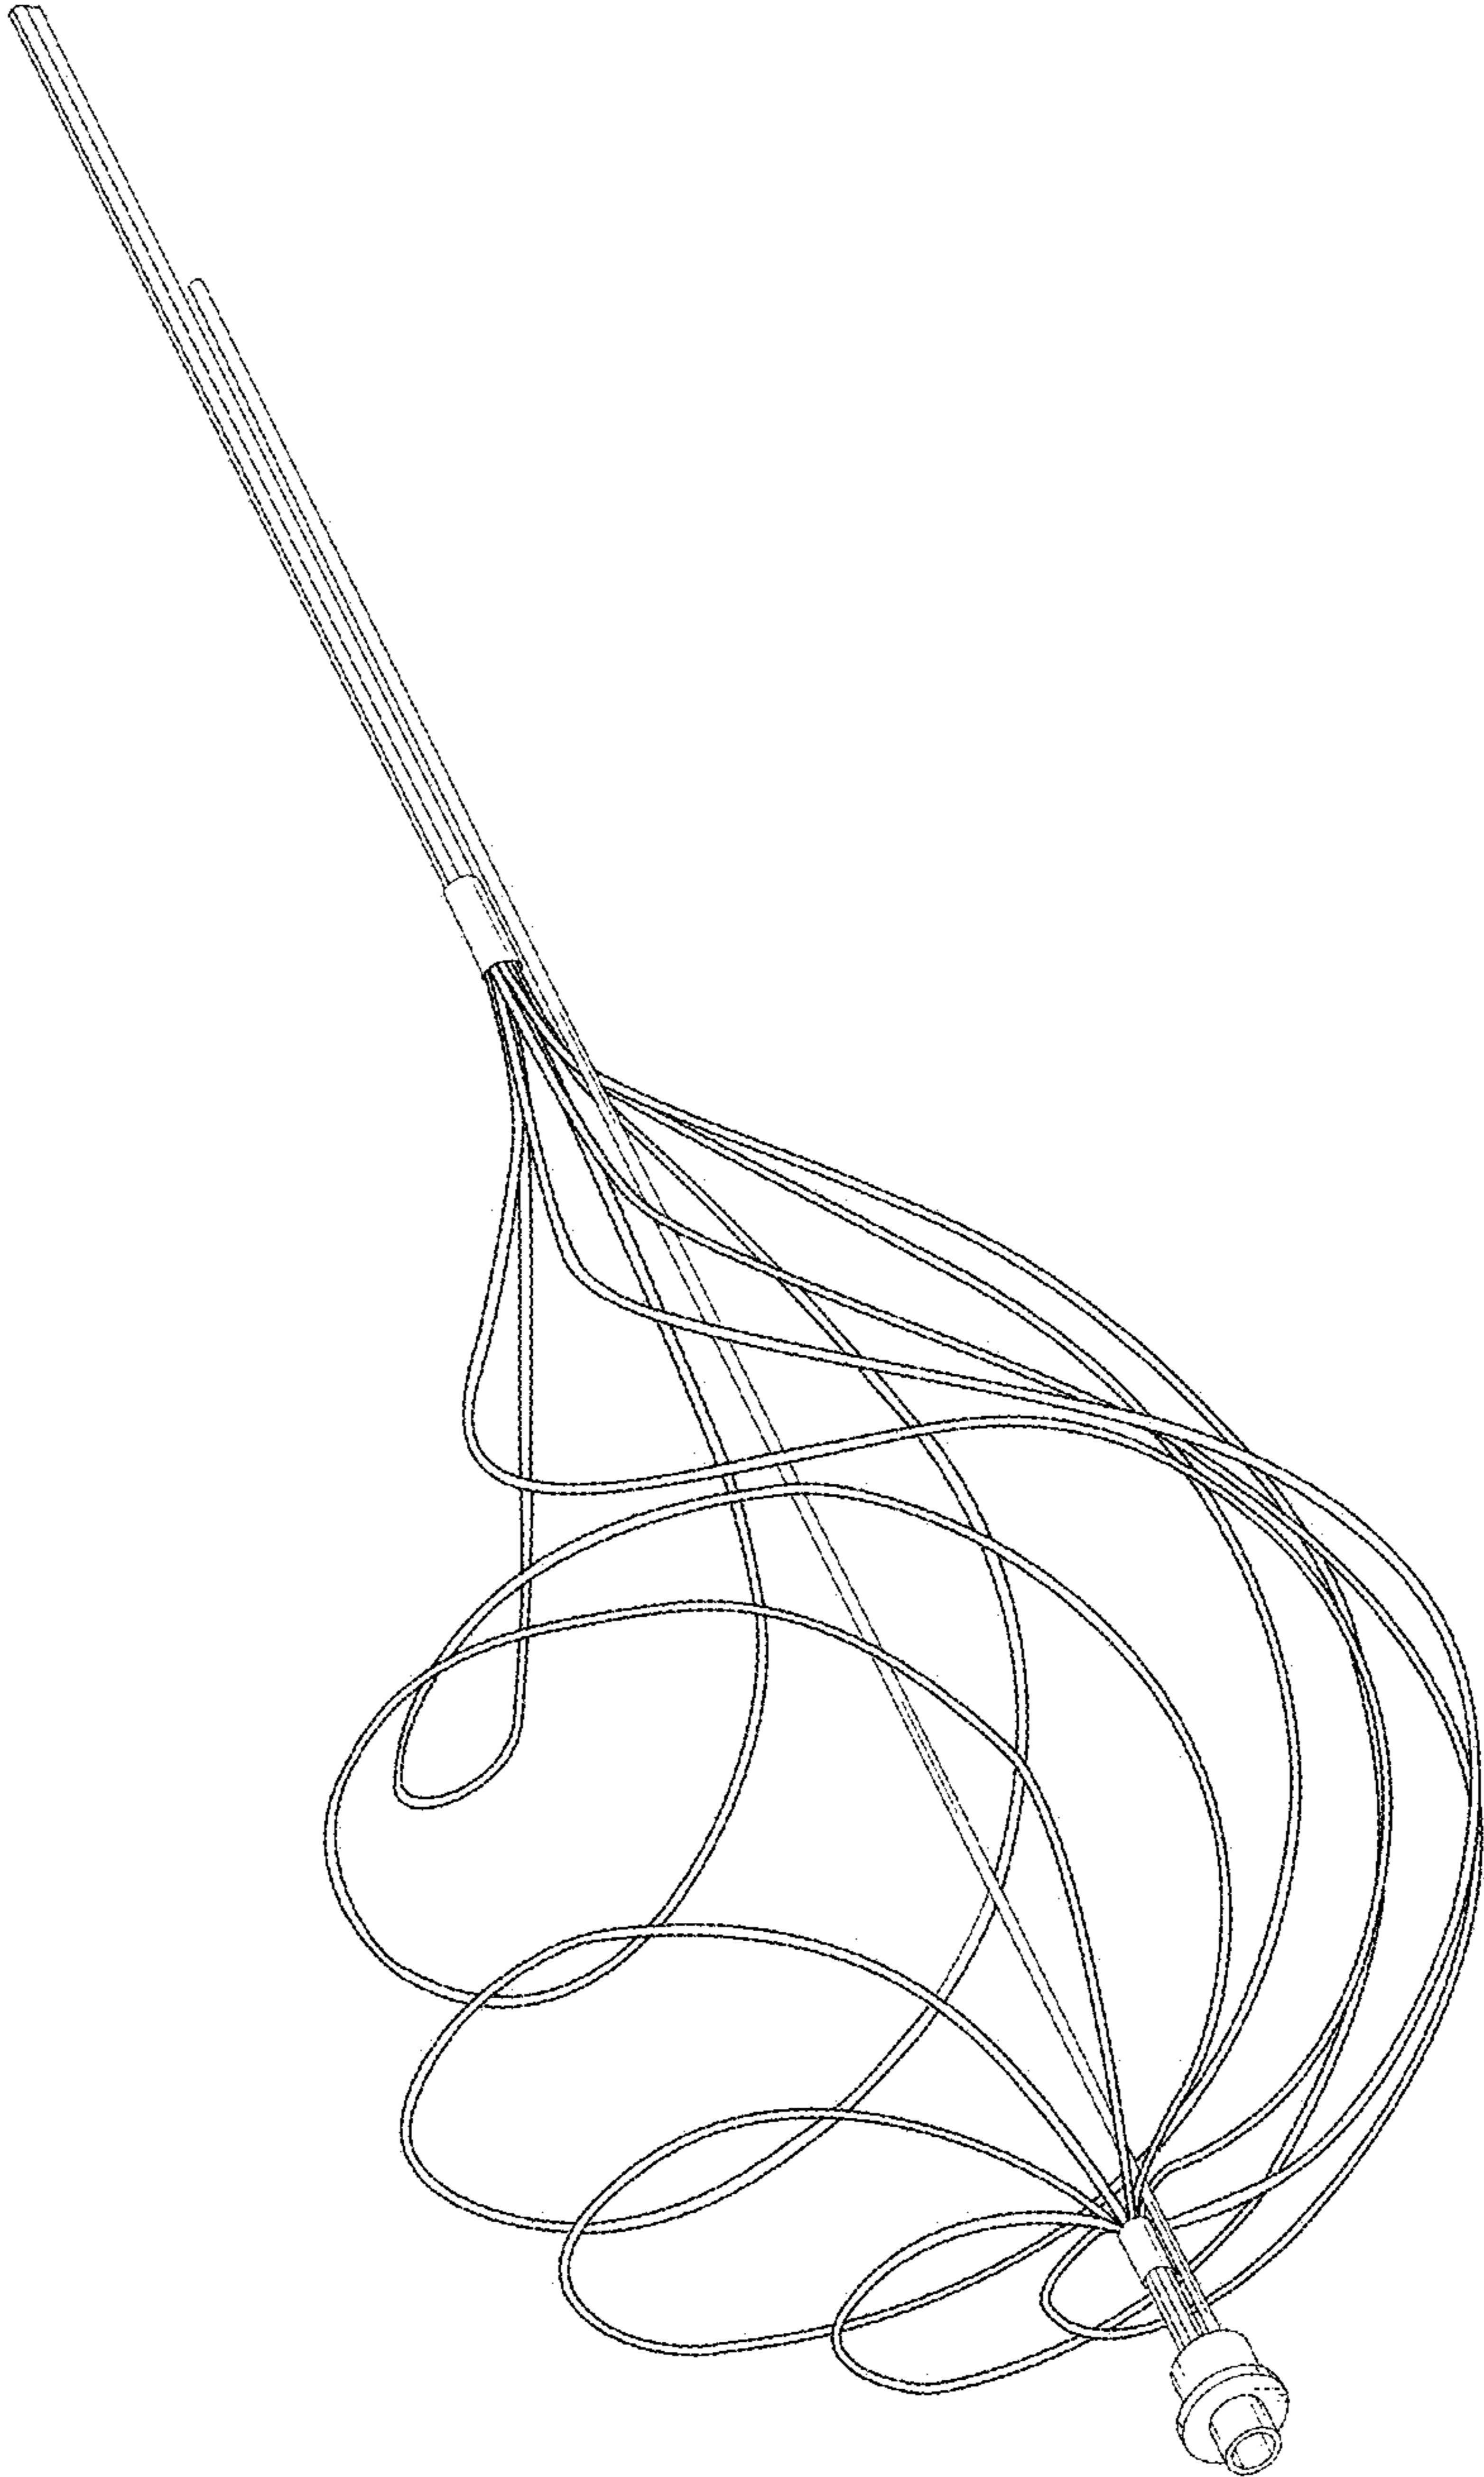


FIG. 10

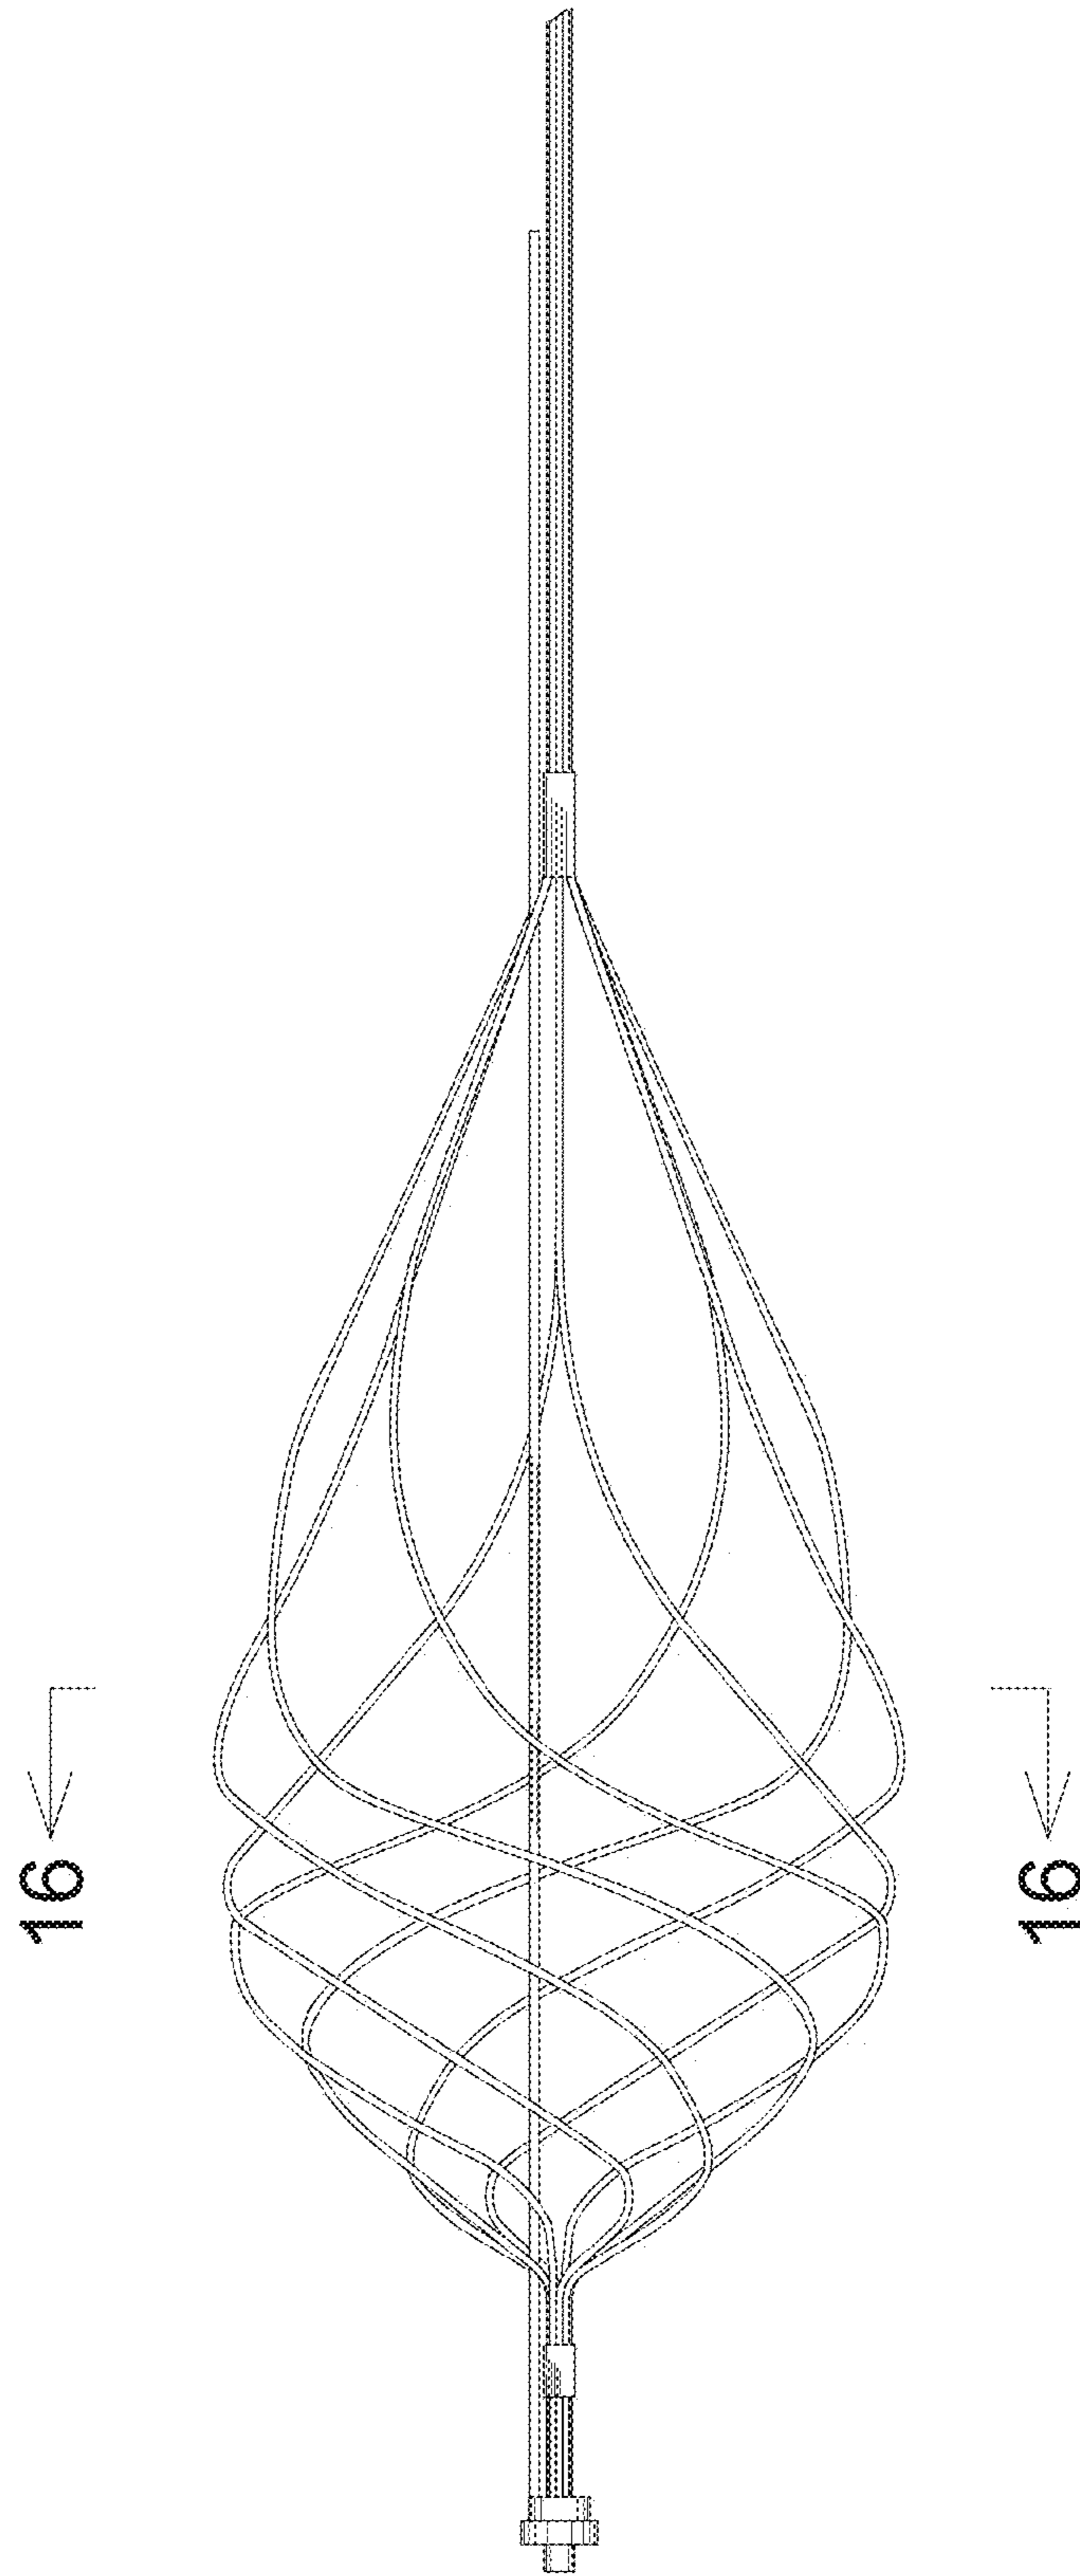


FIG. 11

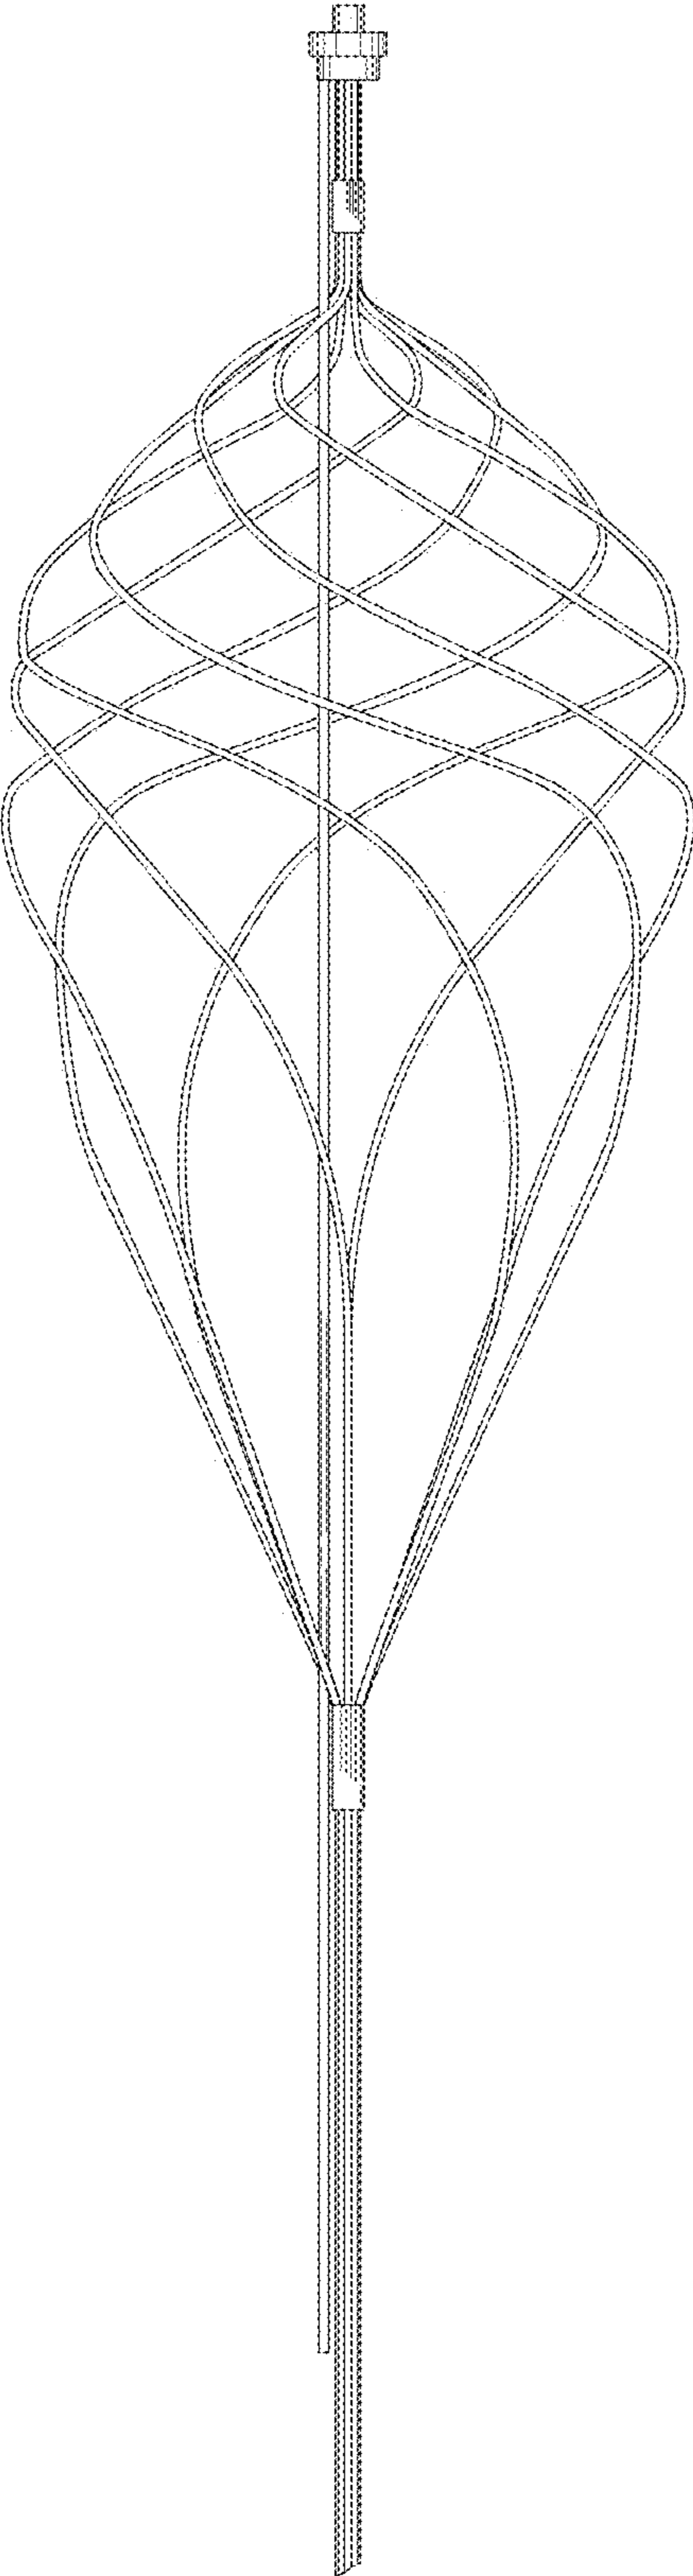


FIG. 12

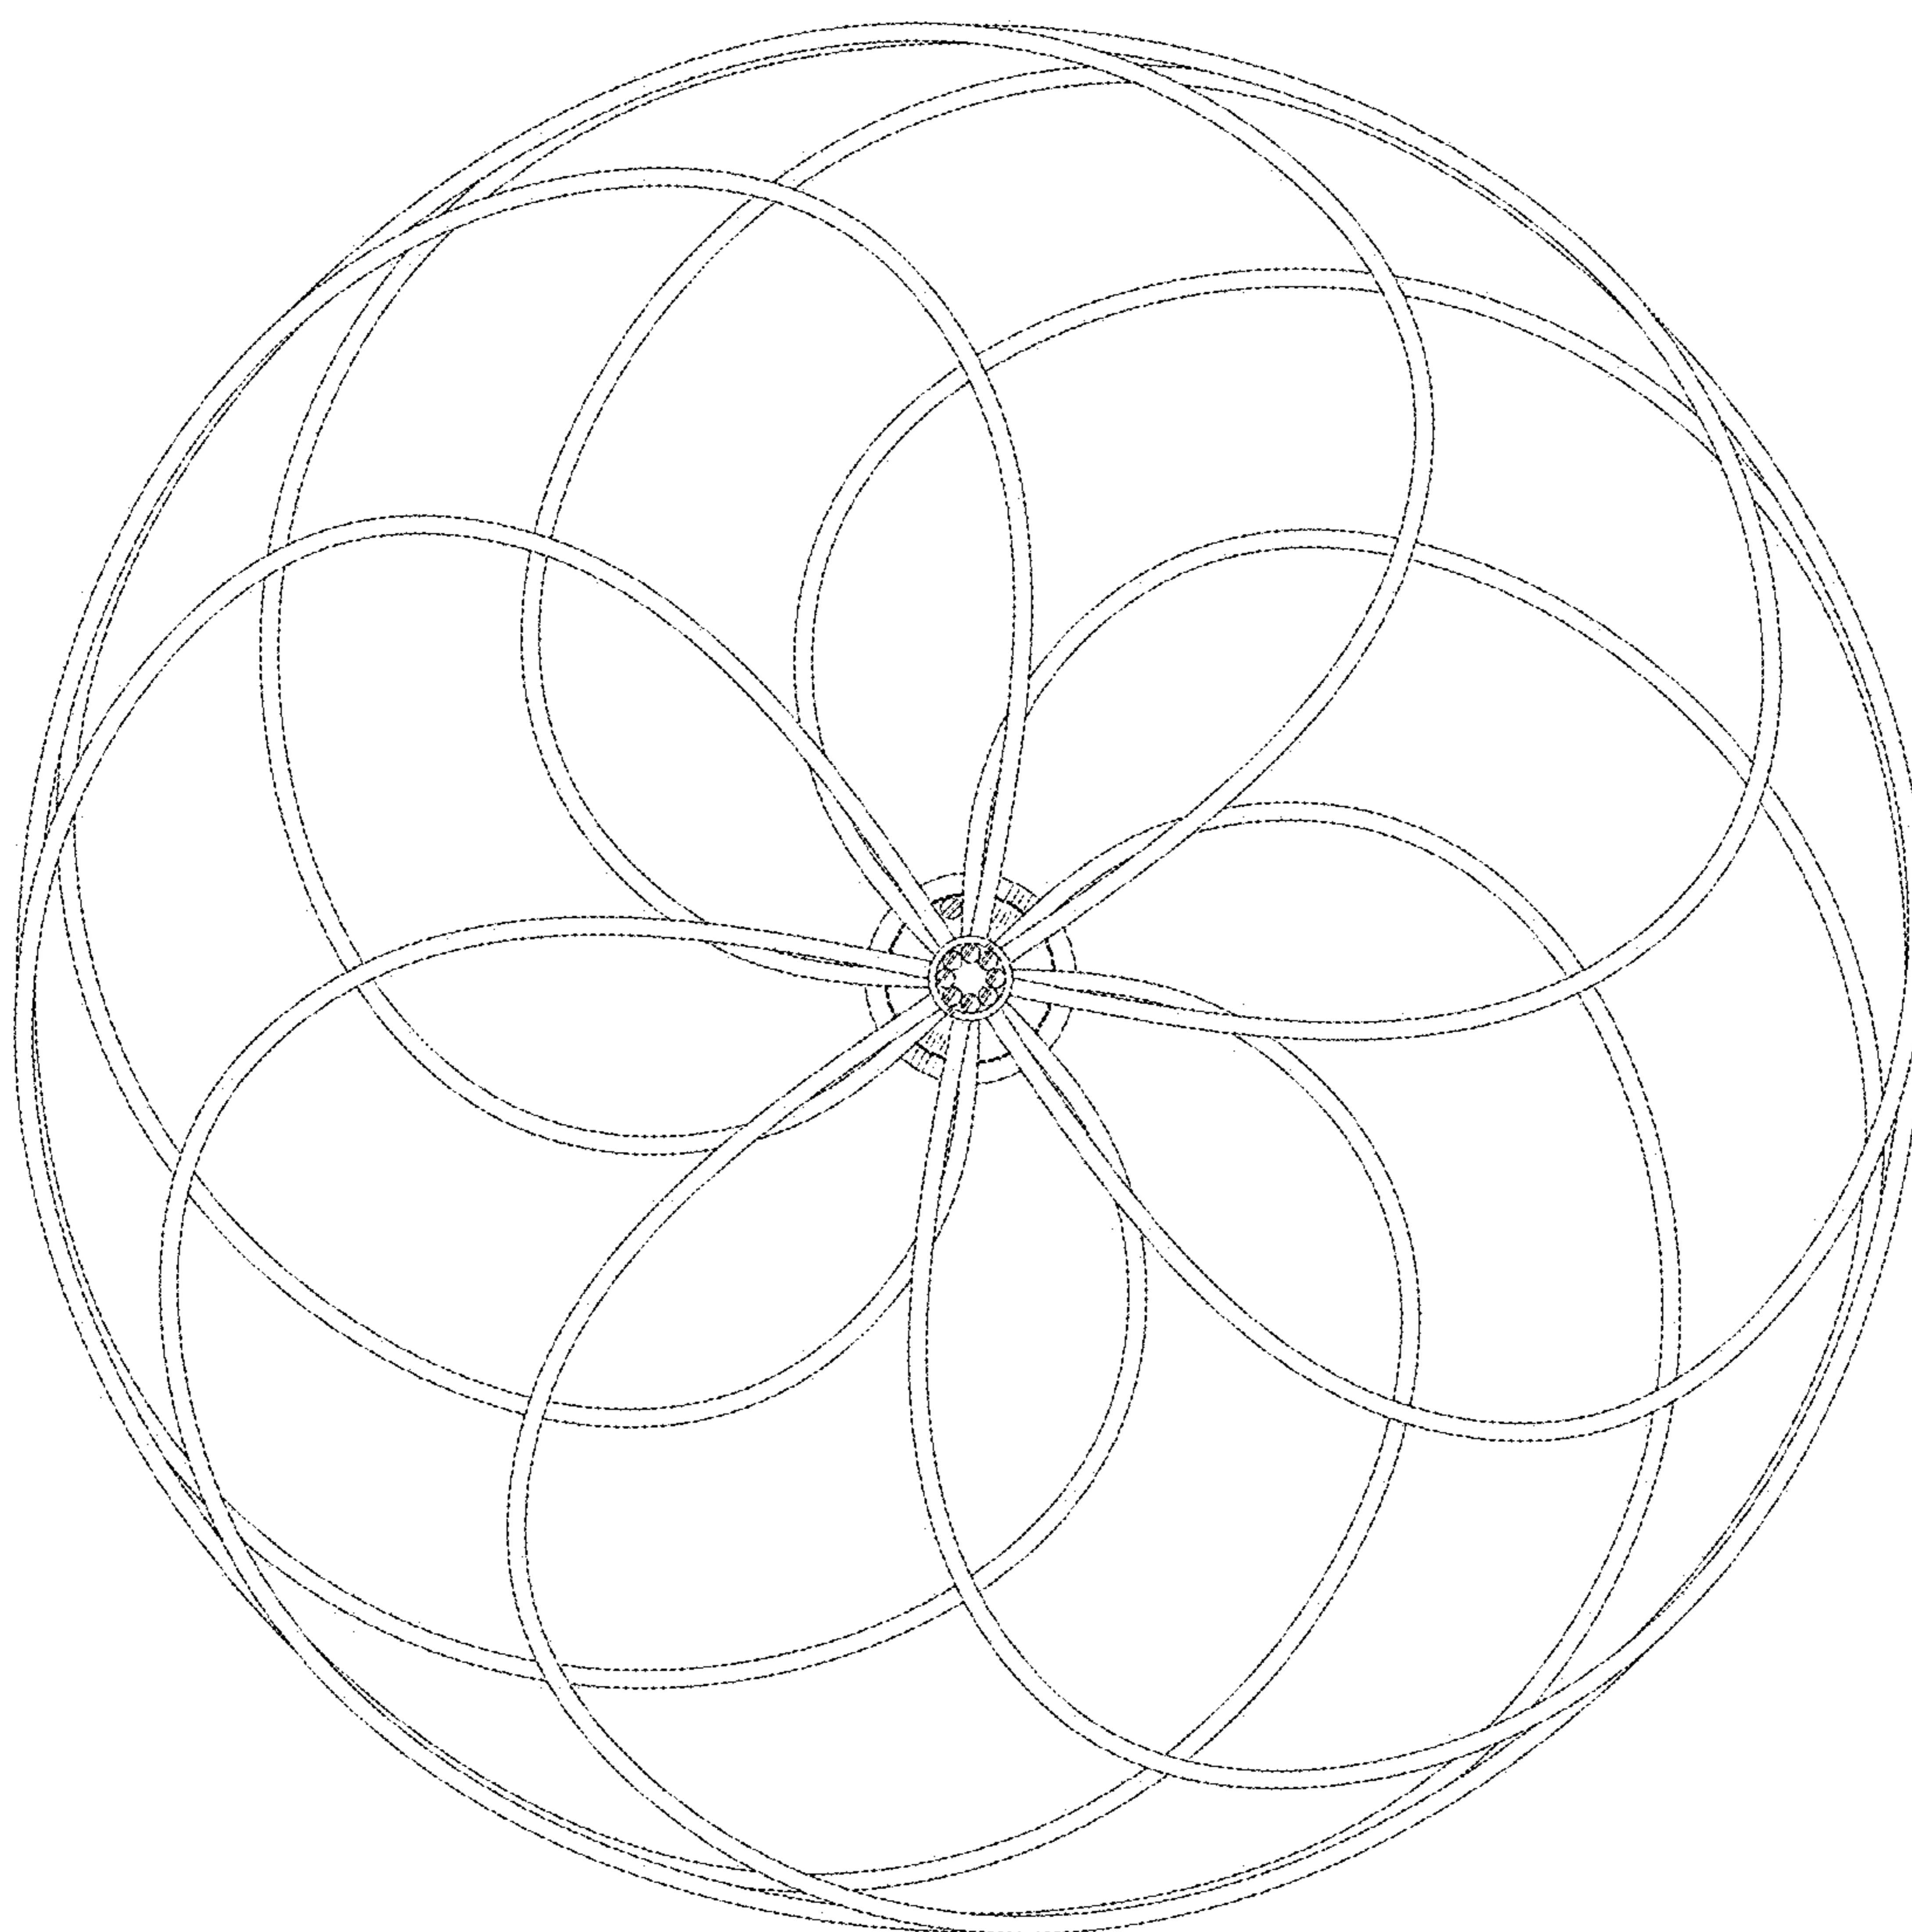


FIG. 13

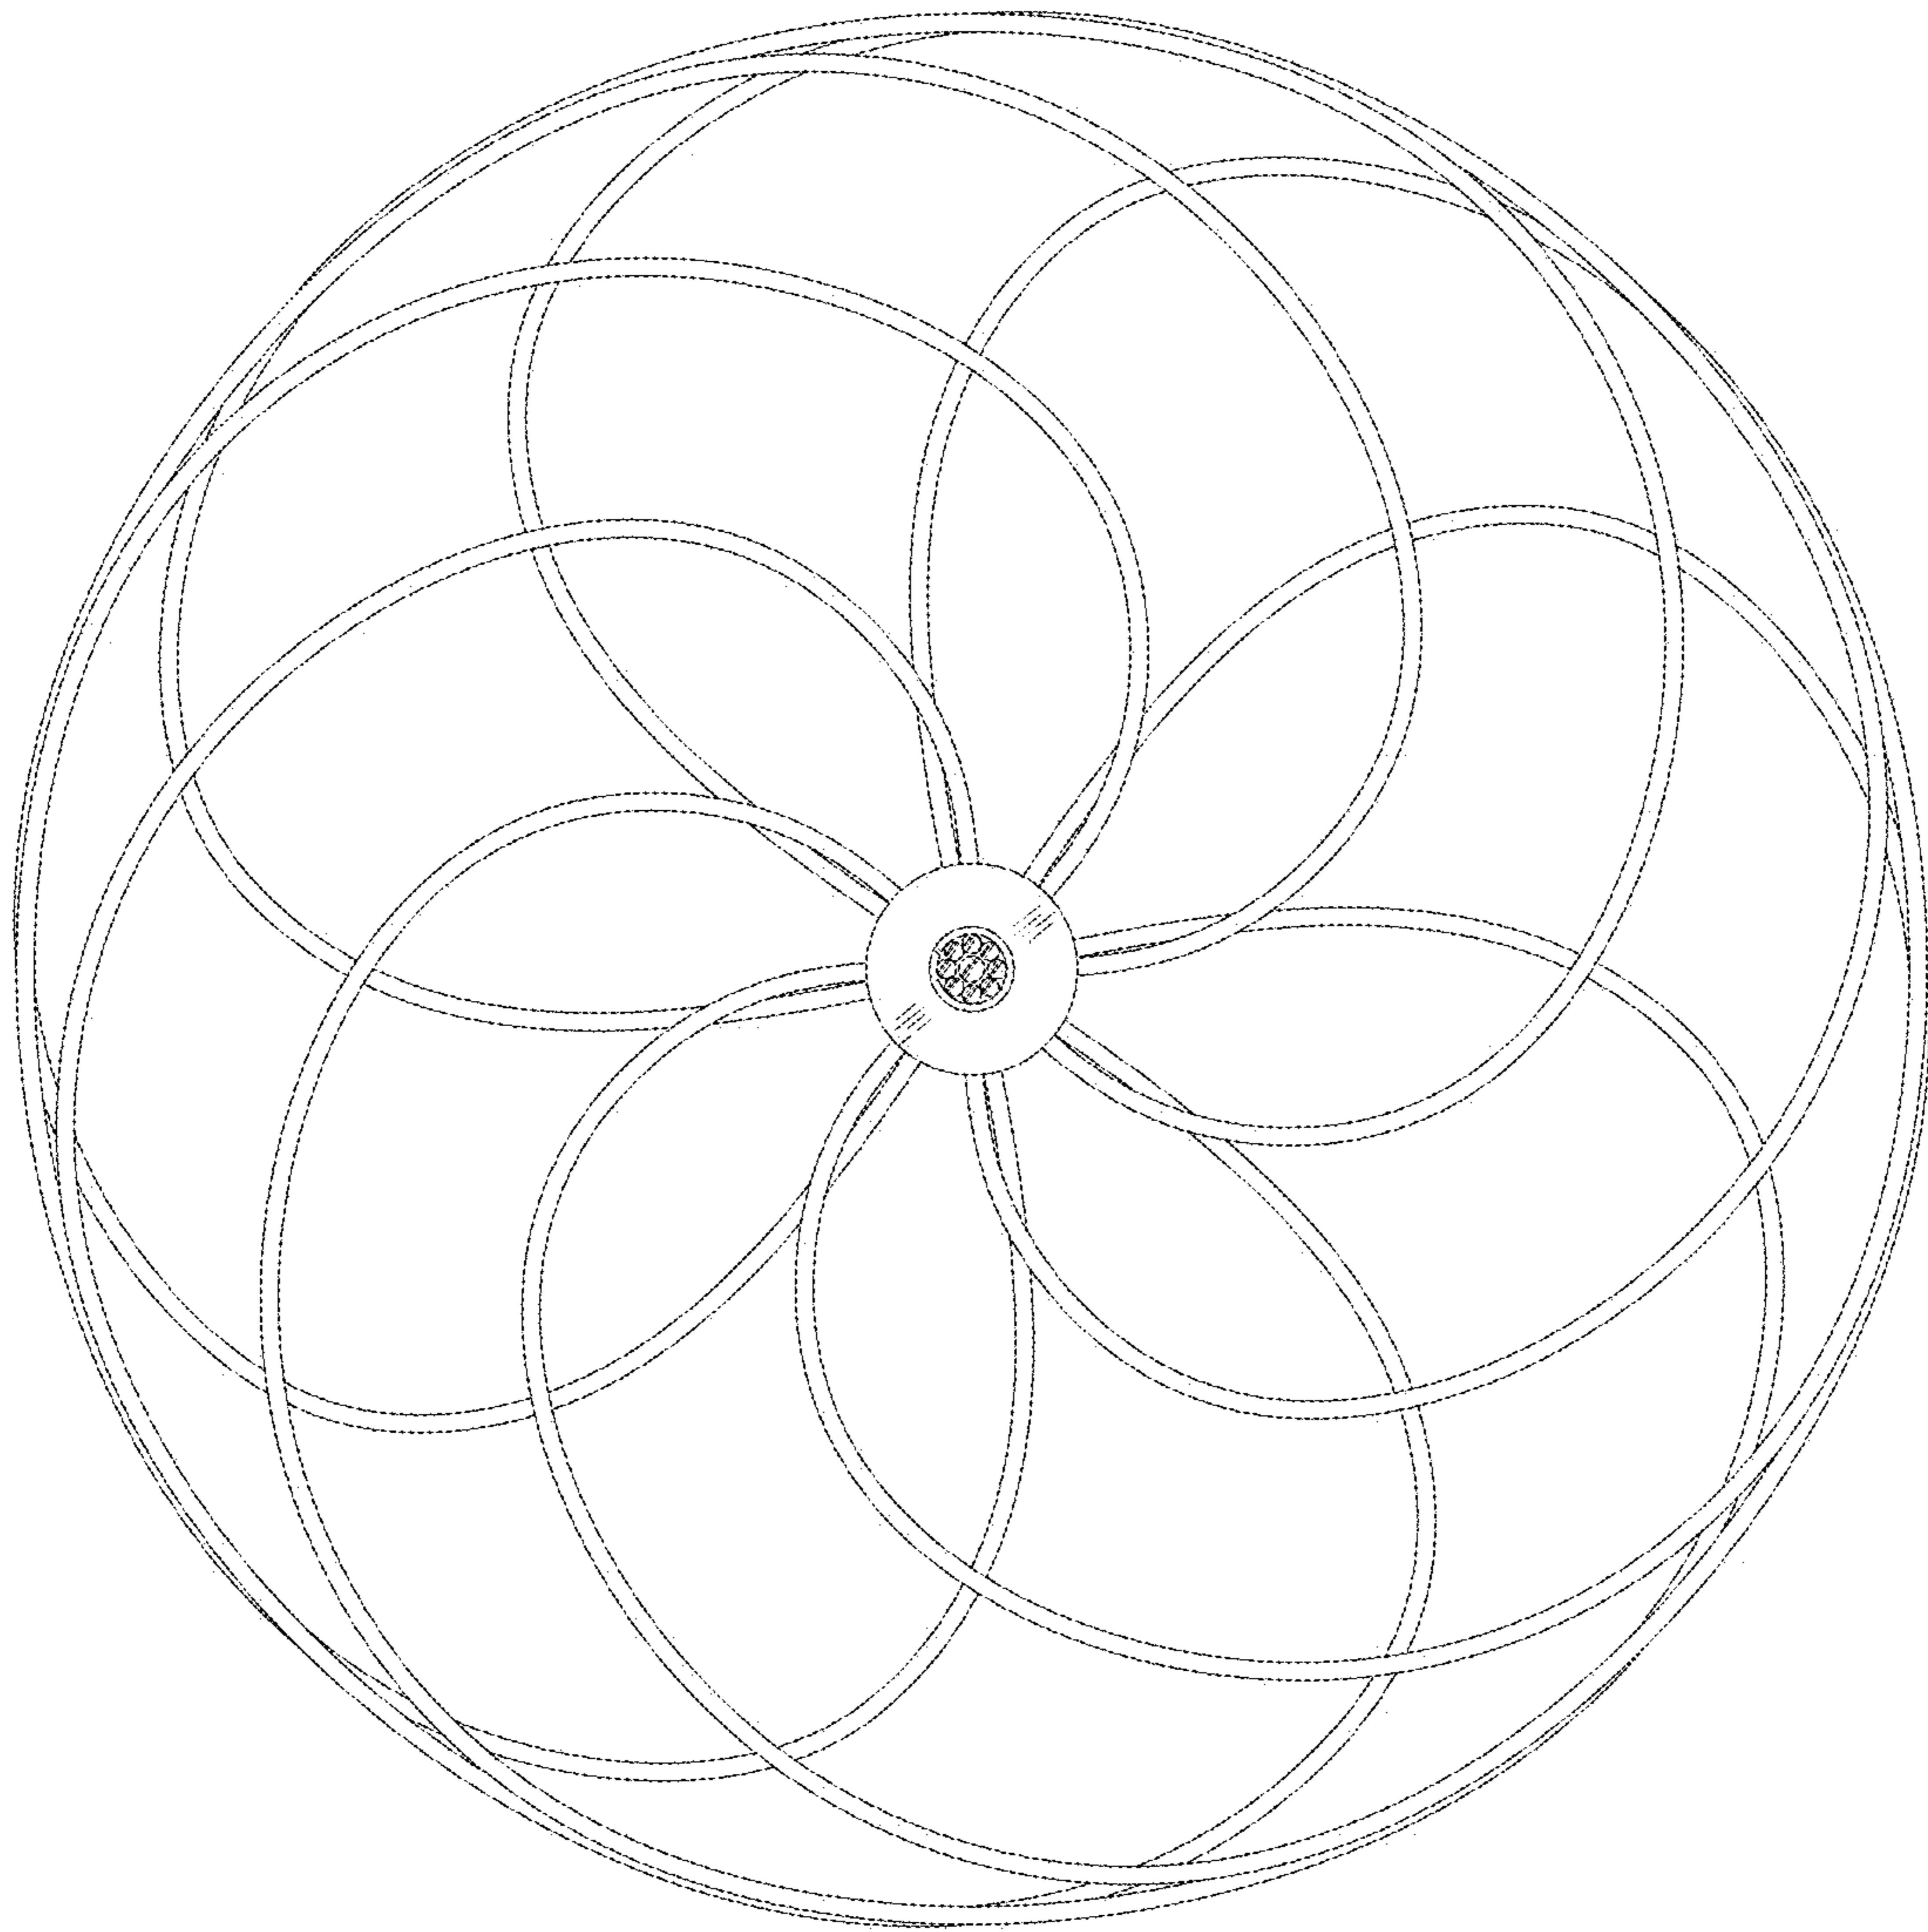


FIG. 14

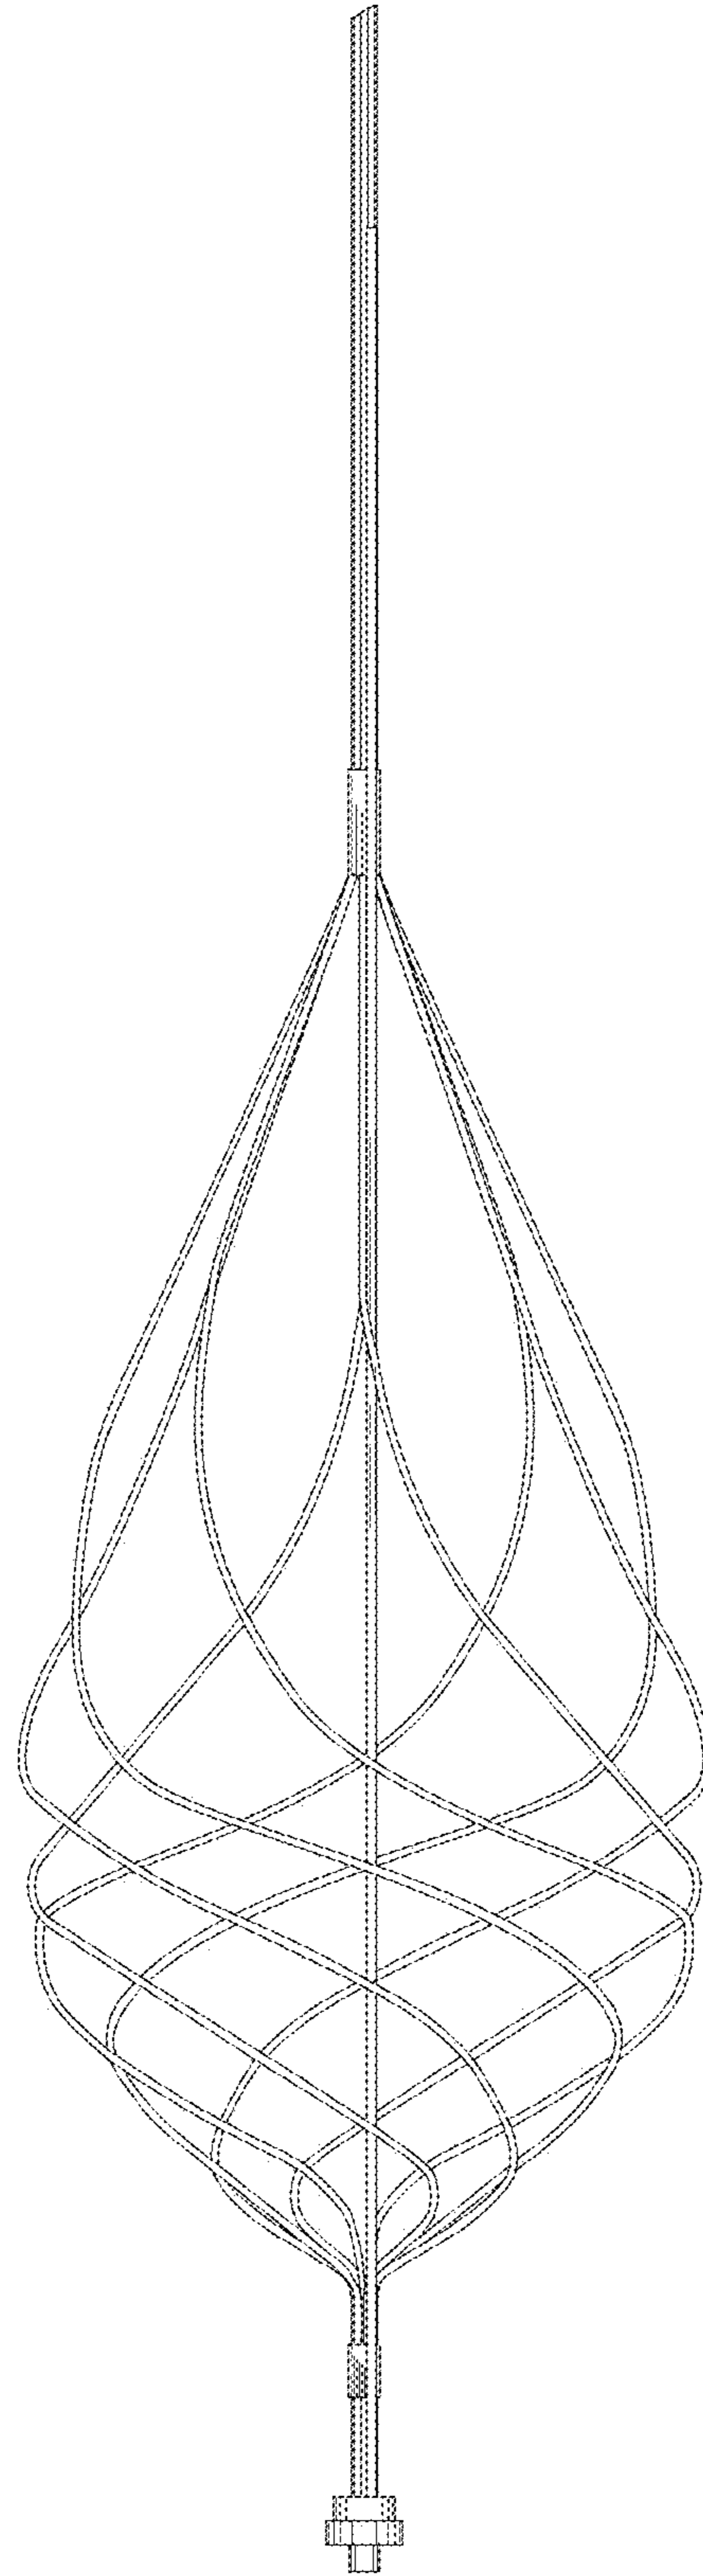


FIG. 15

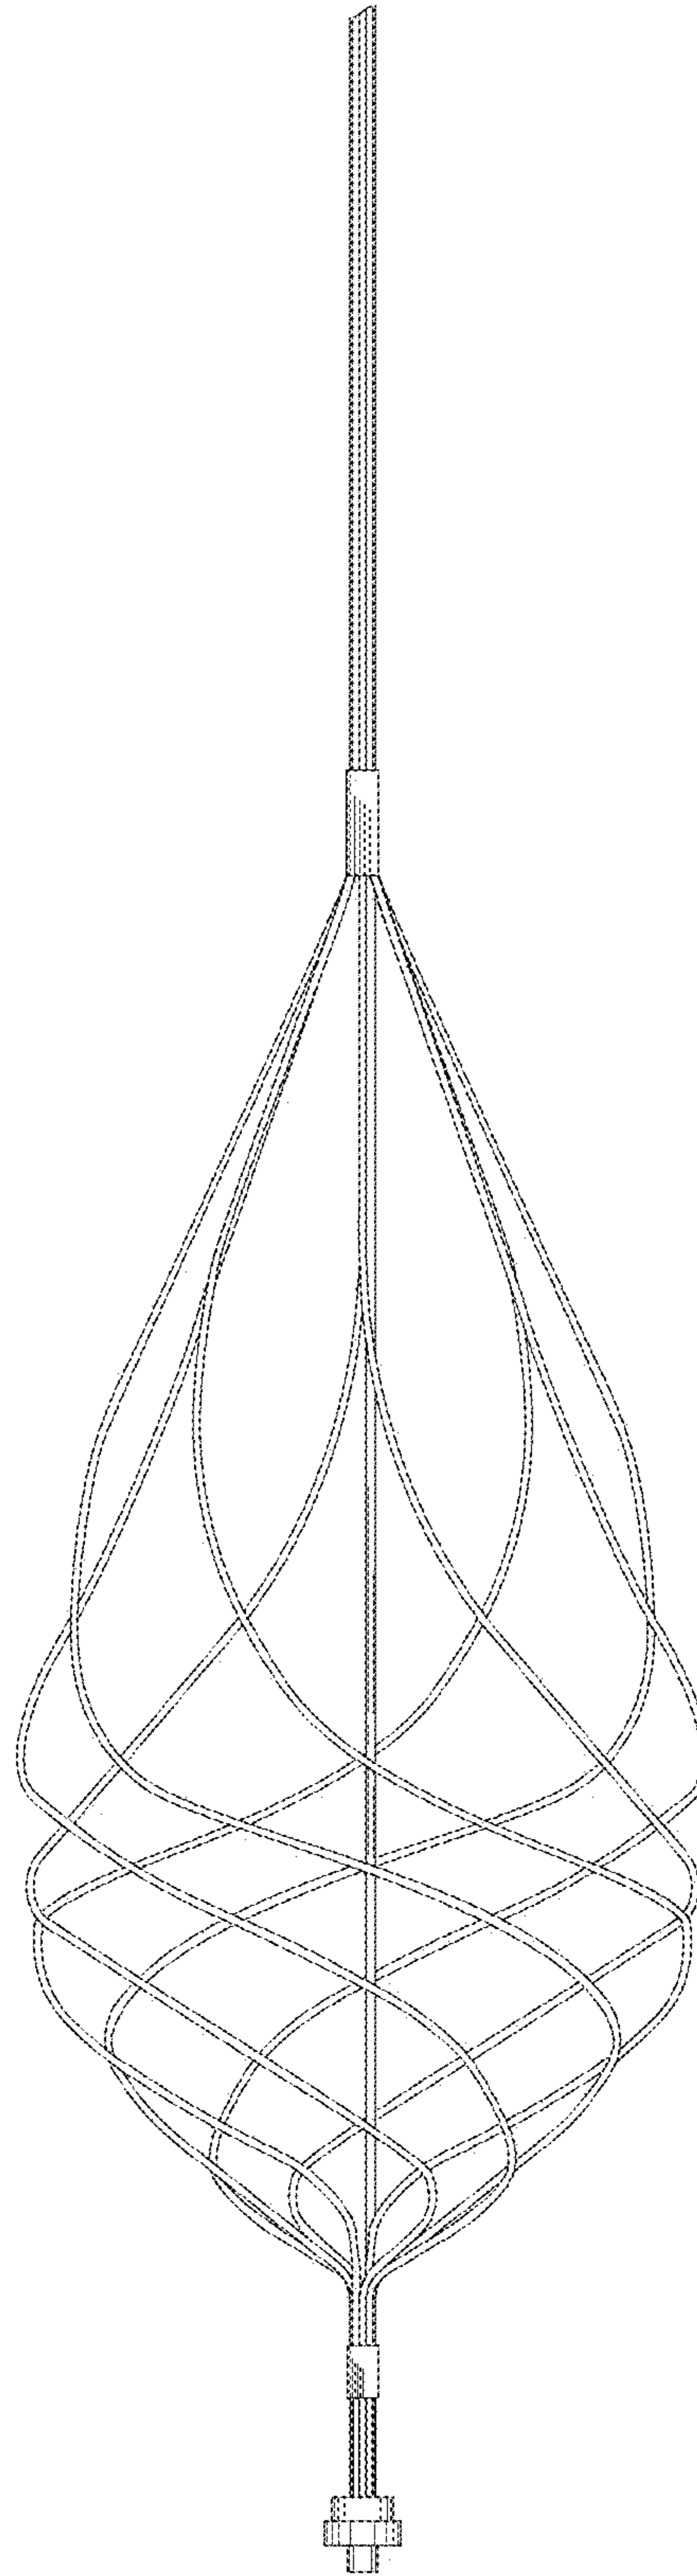


FIG. 16



FIG. 17

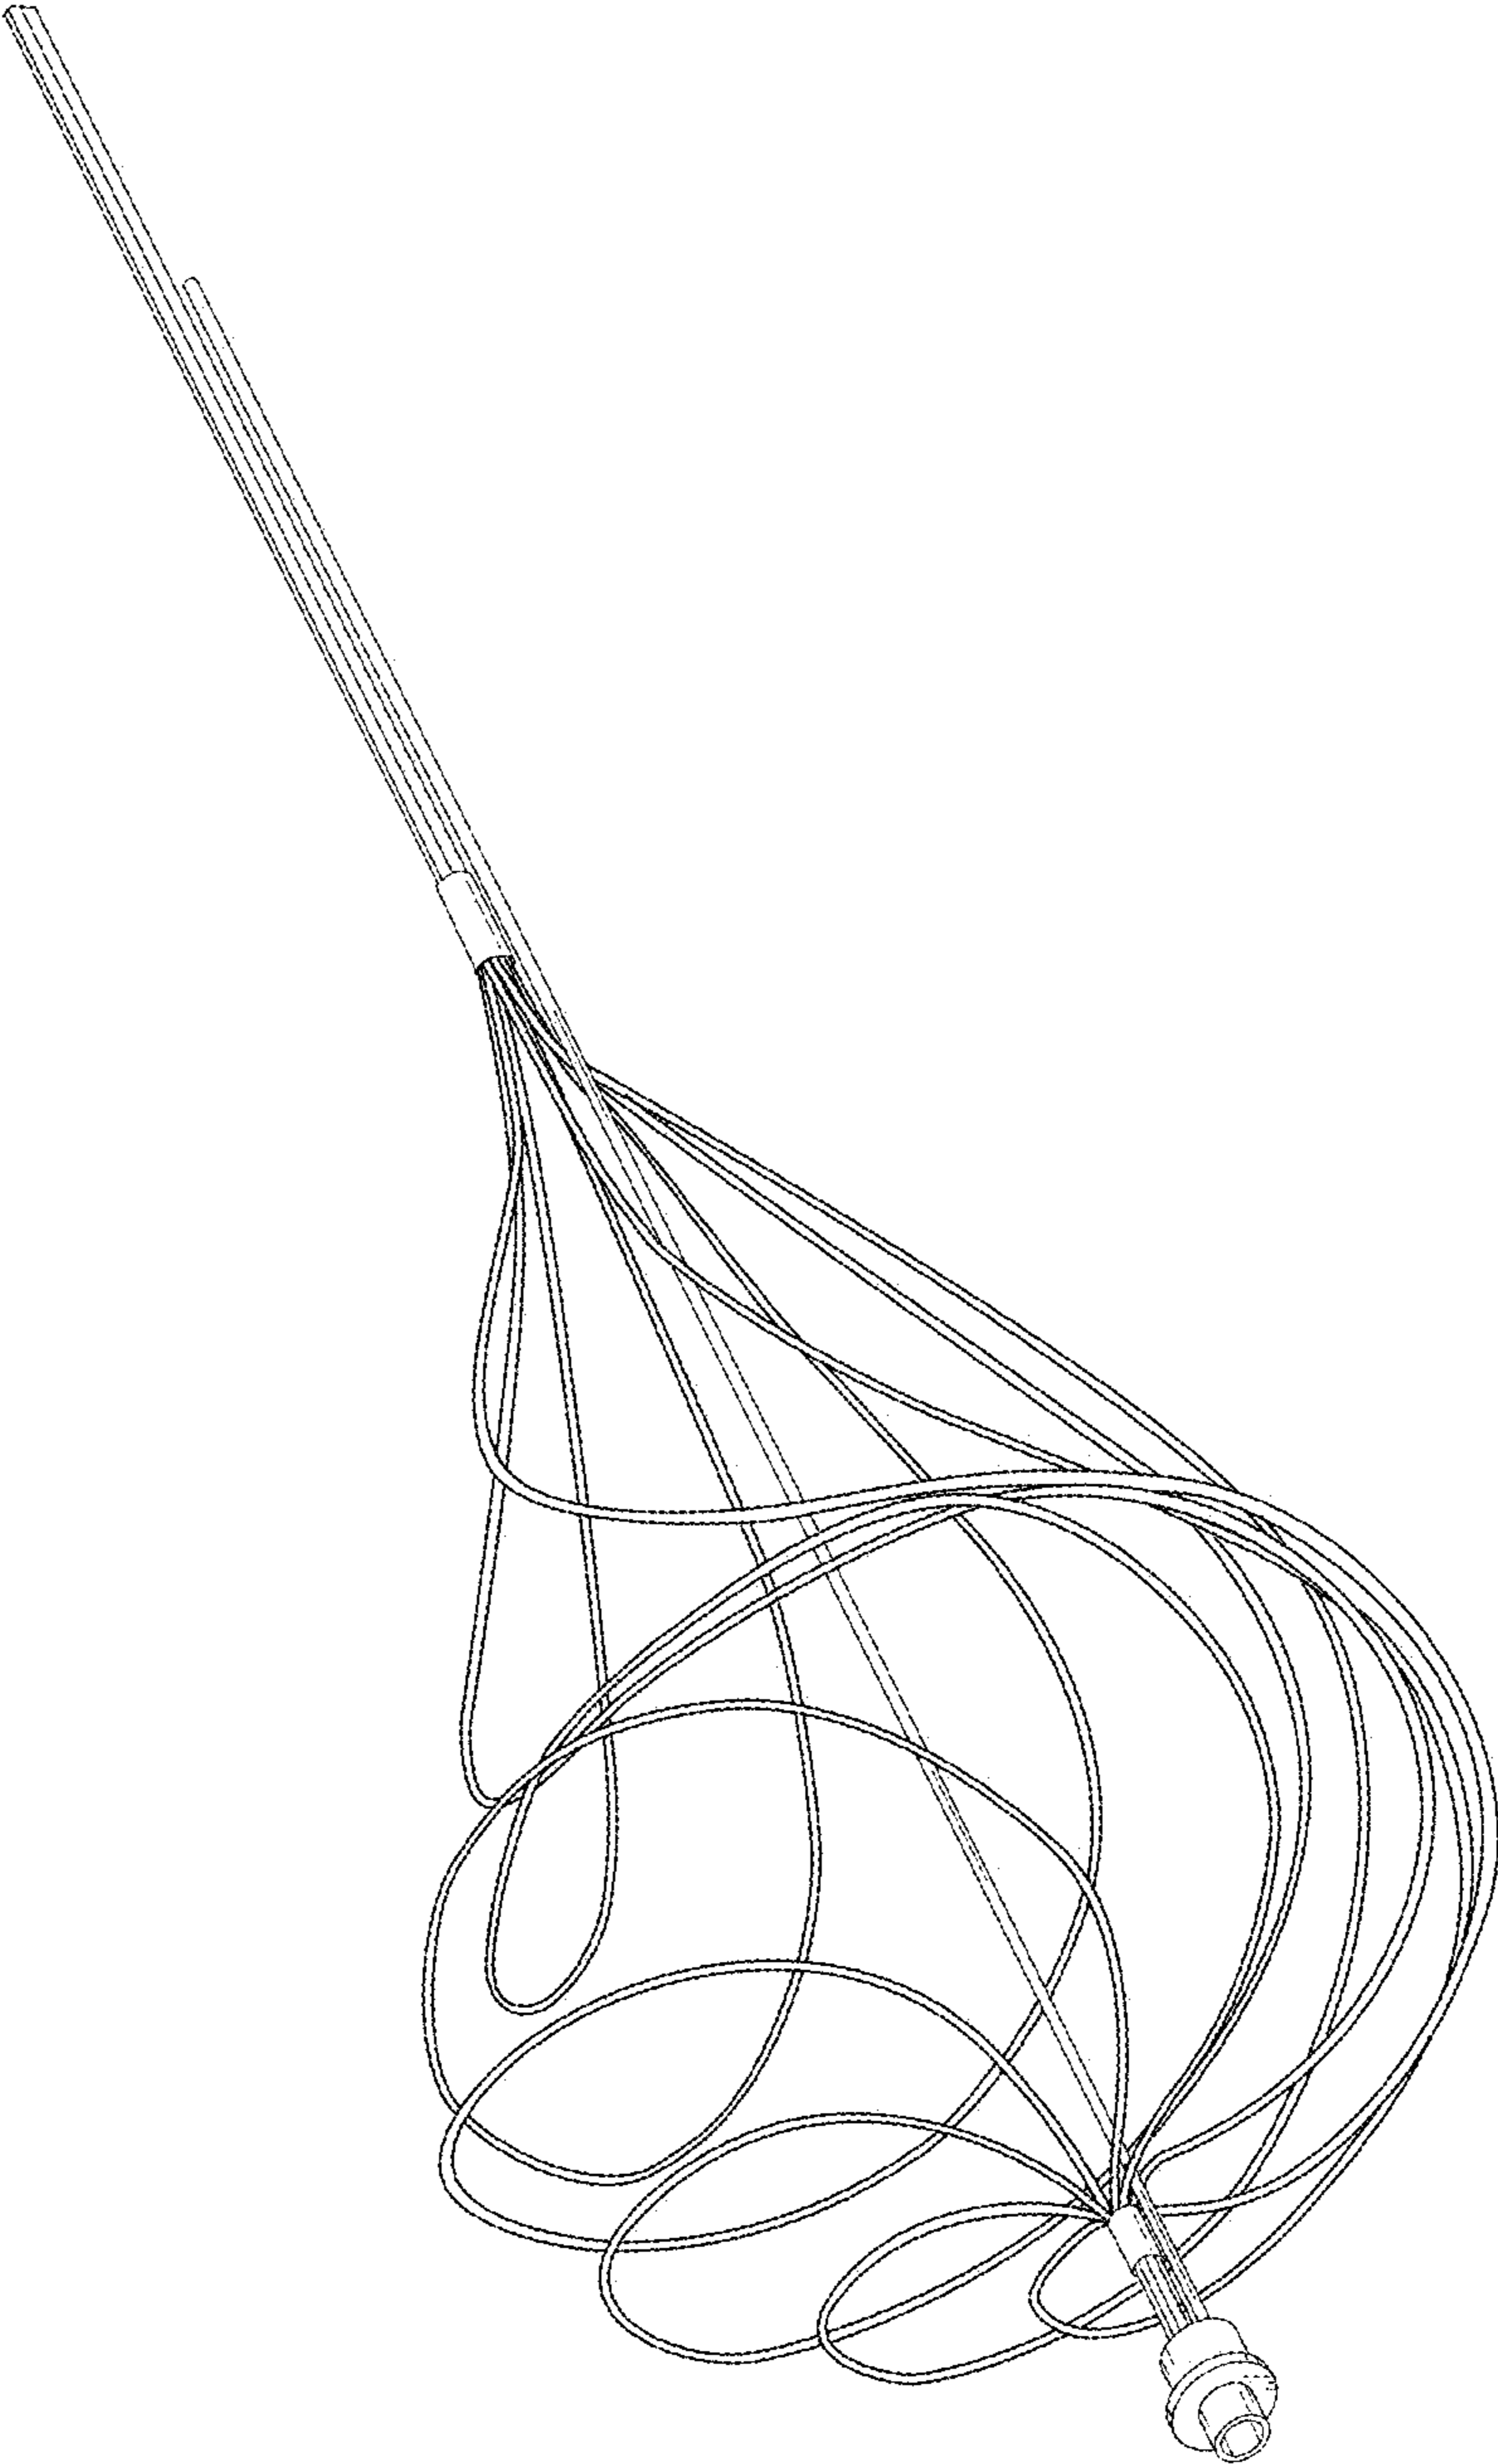


FIG. 18



FIG. 19

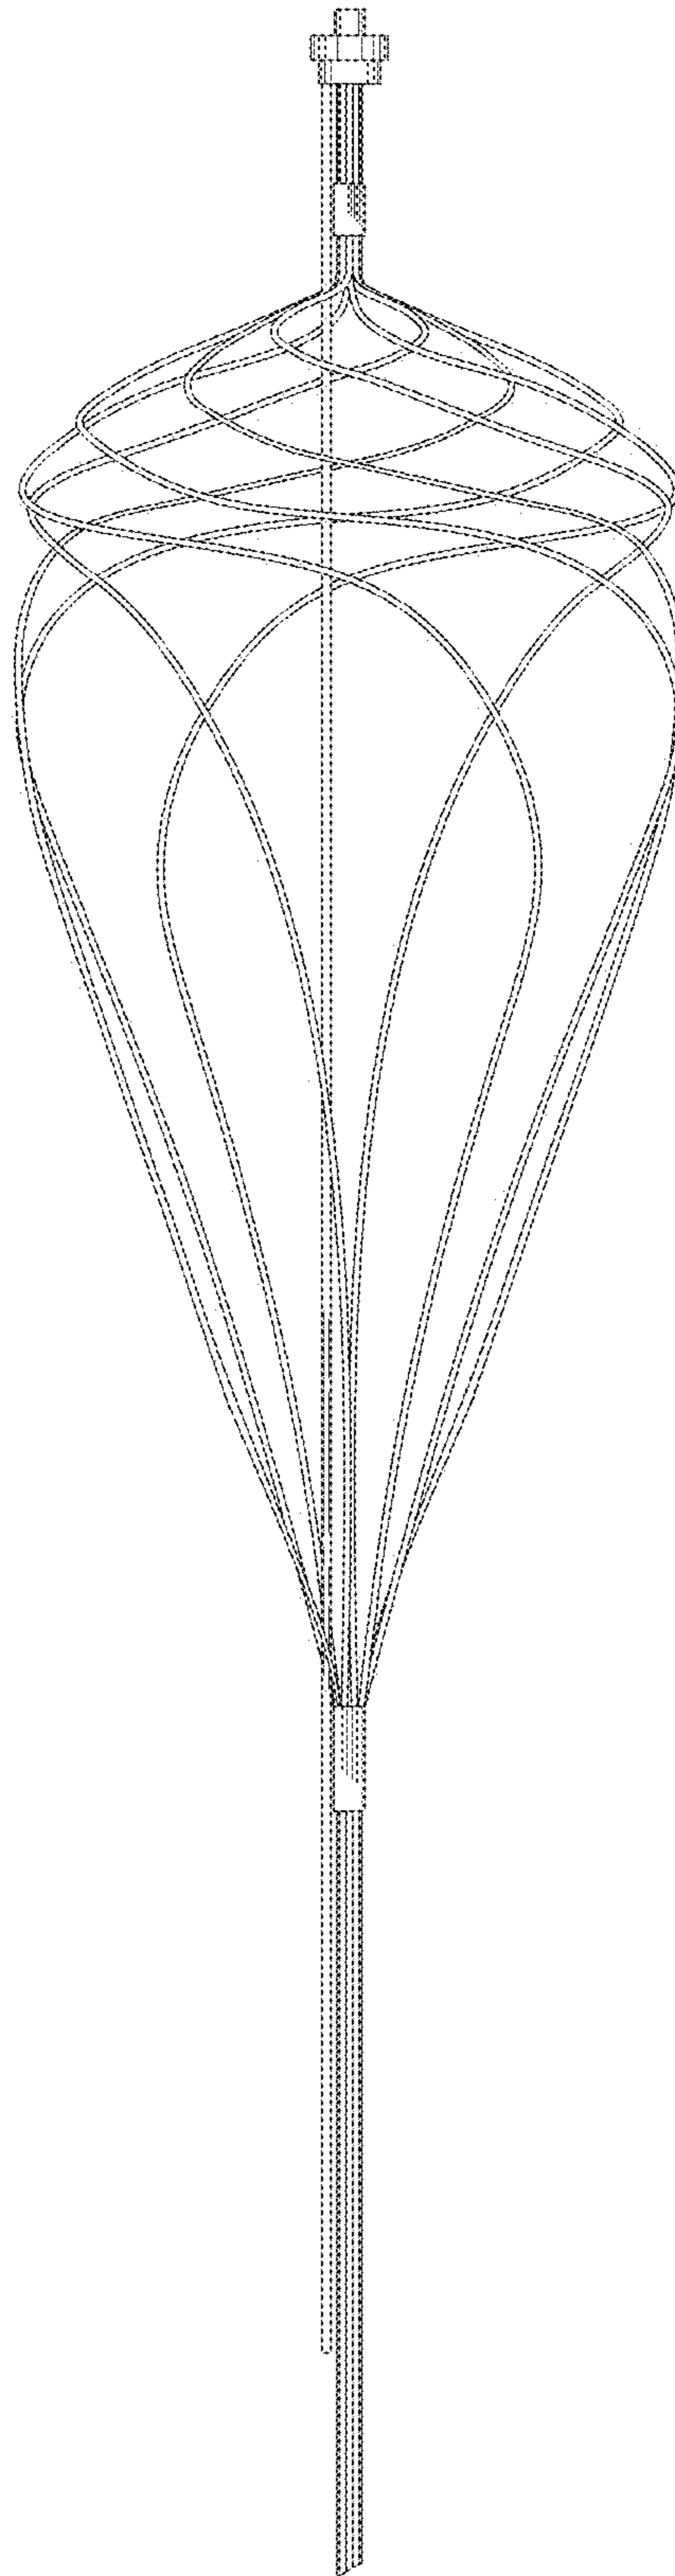


FIG. 20

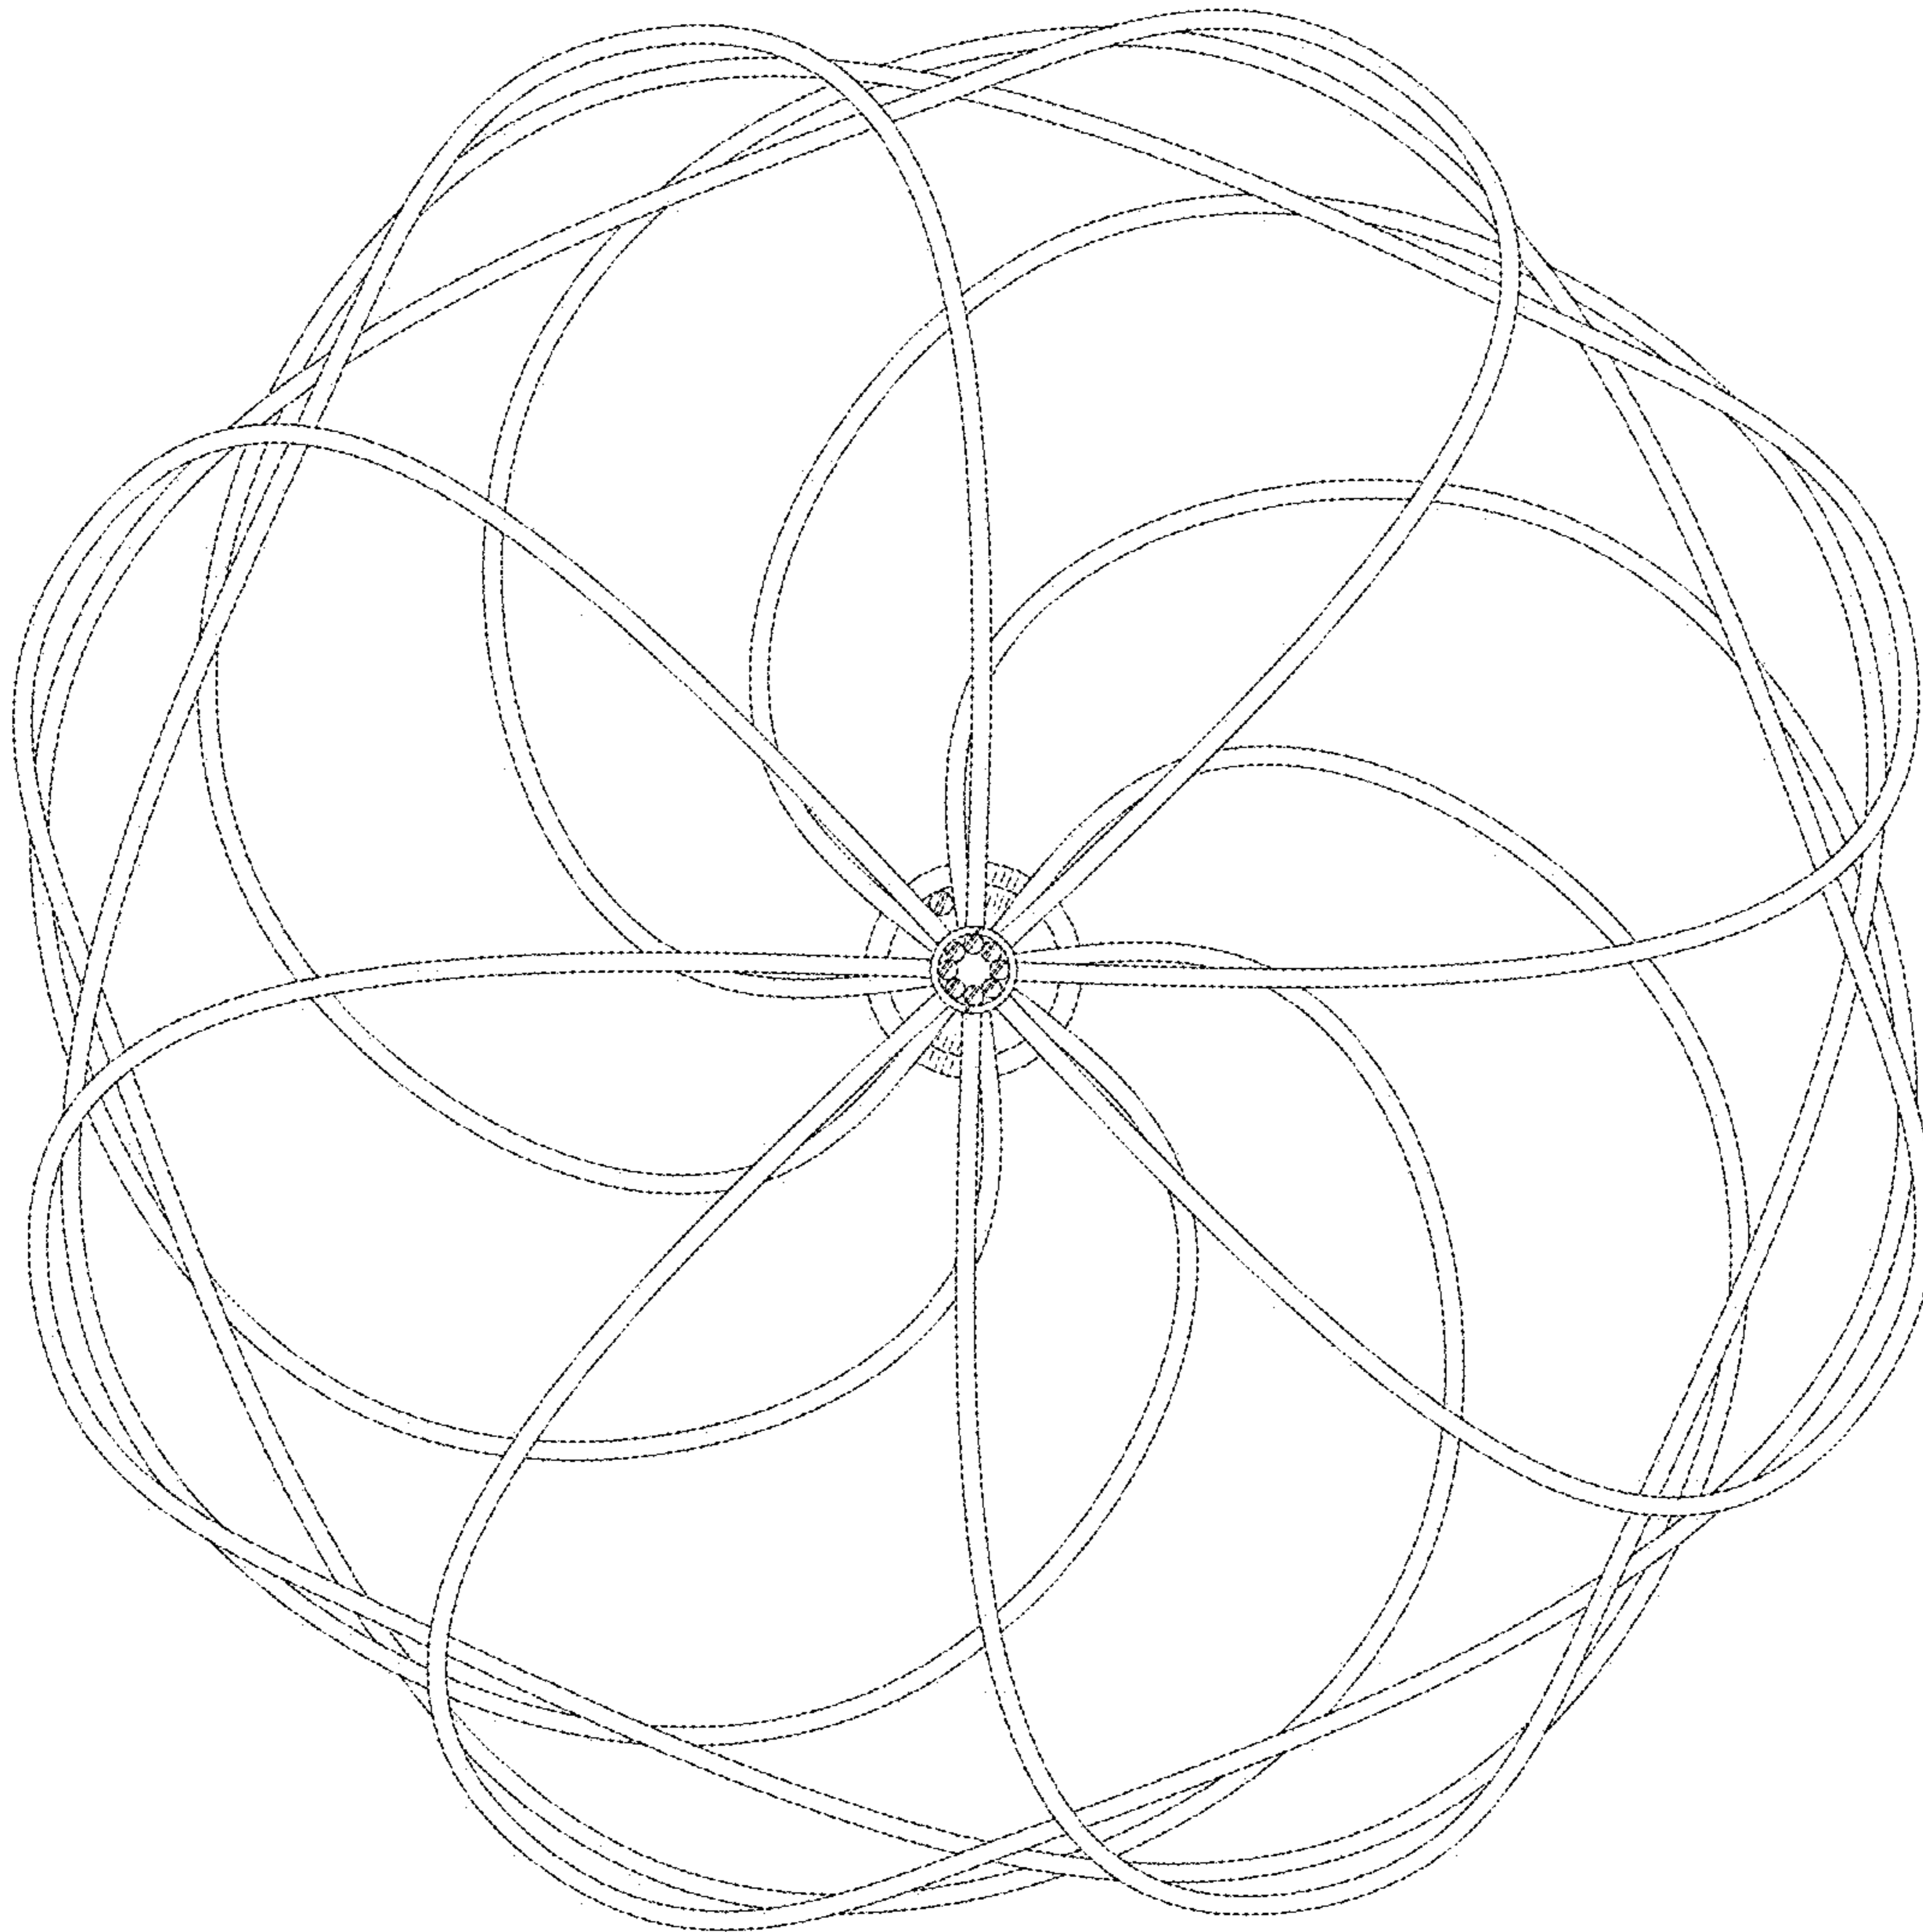


FIG. 21

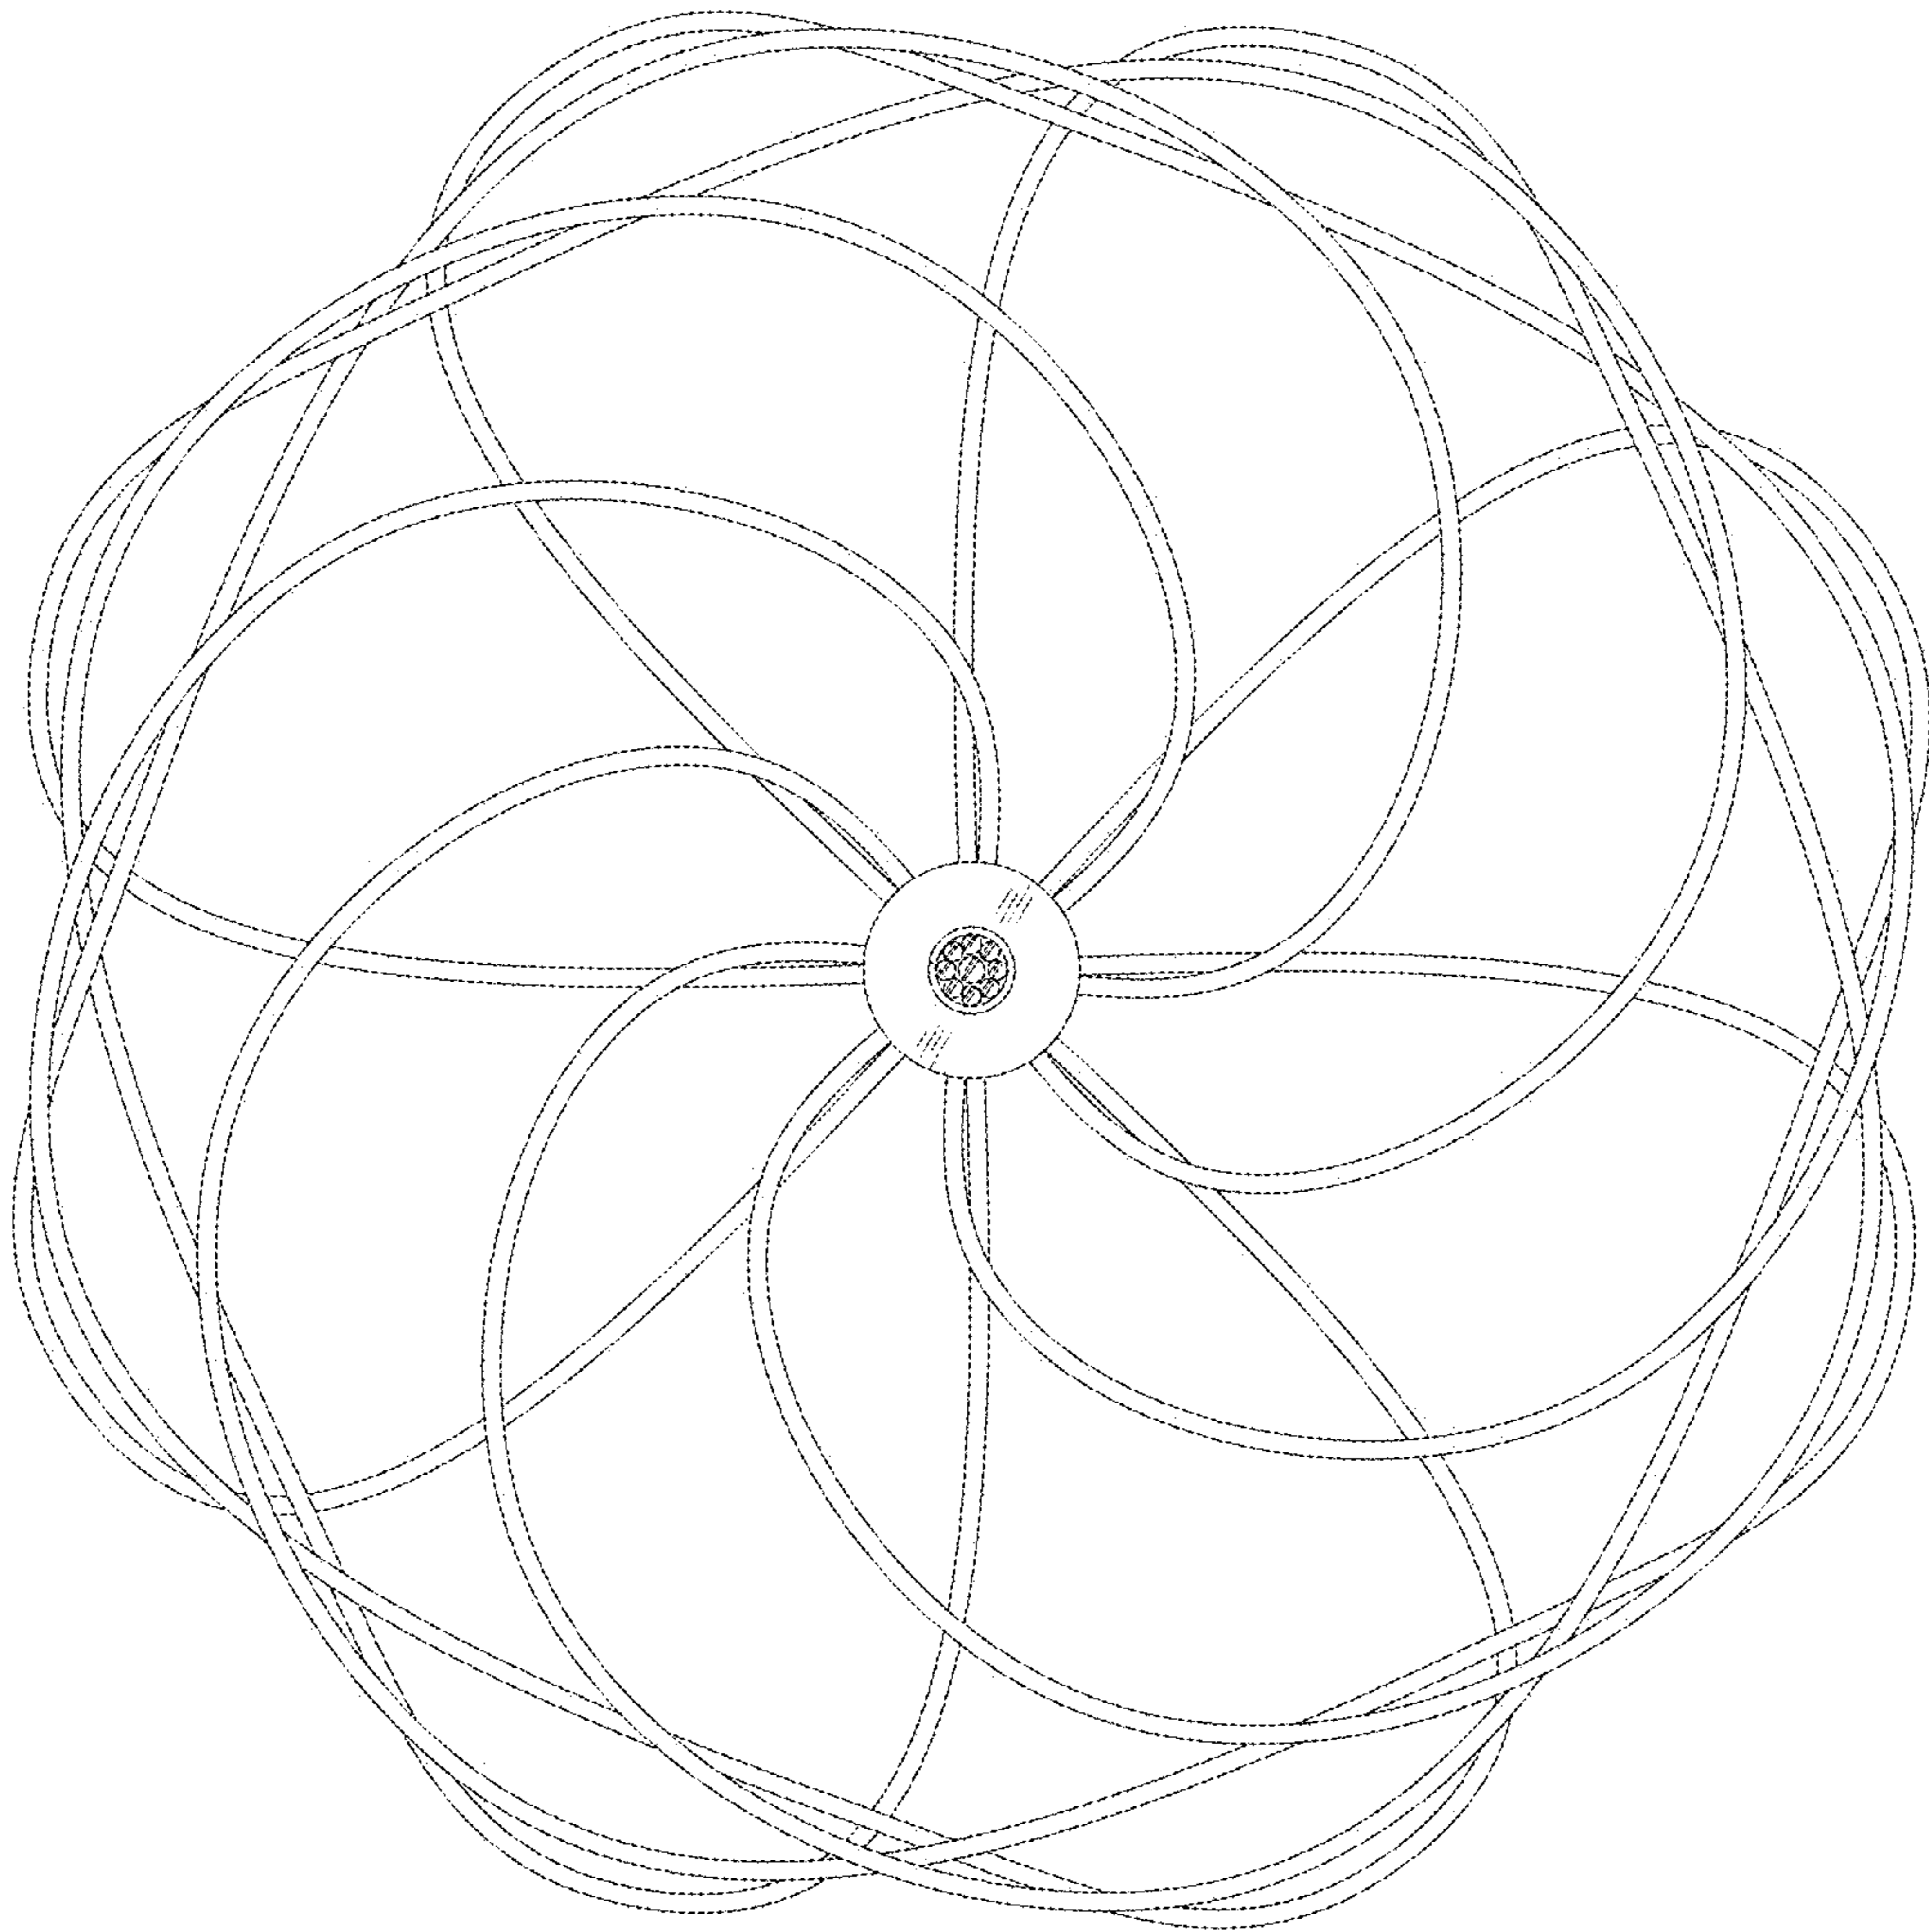


FIG. 22

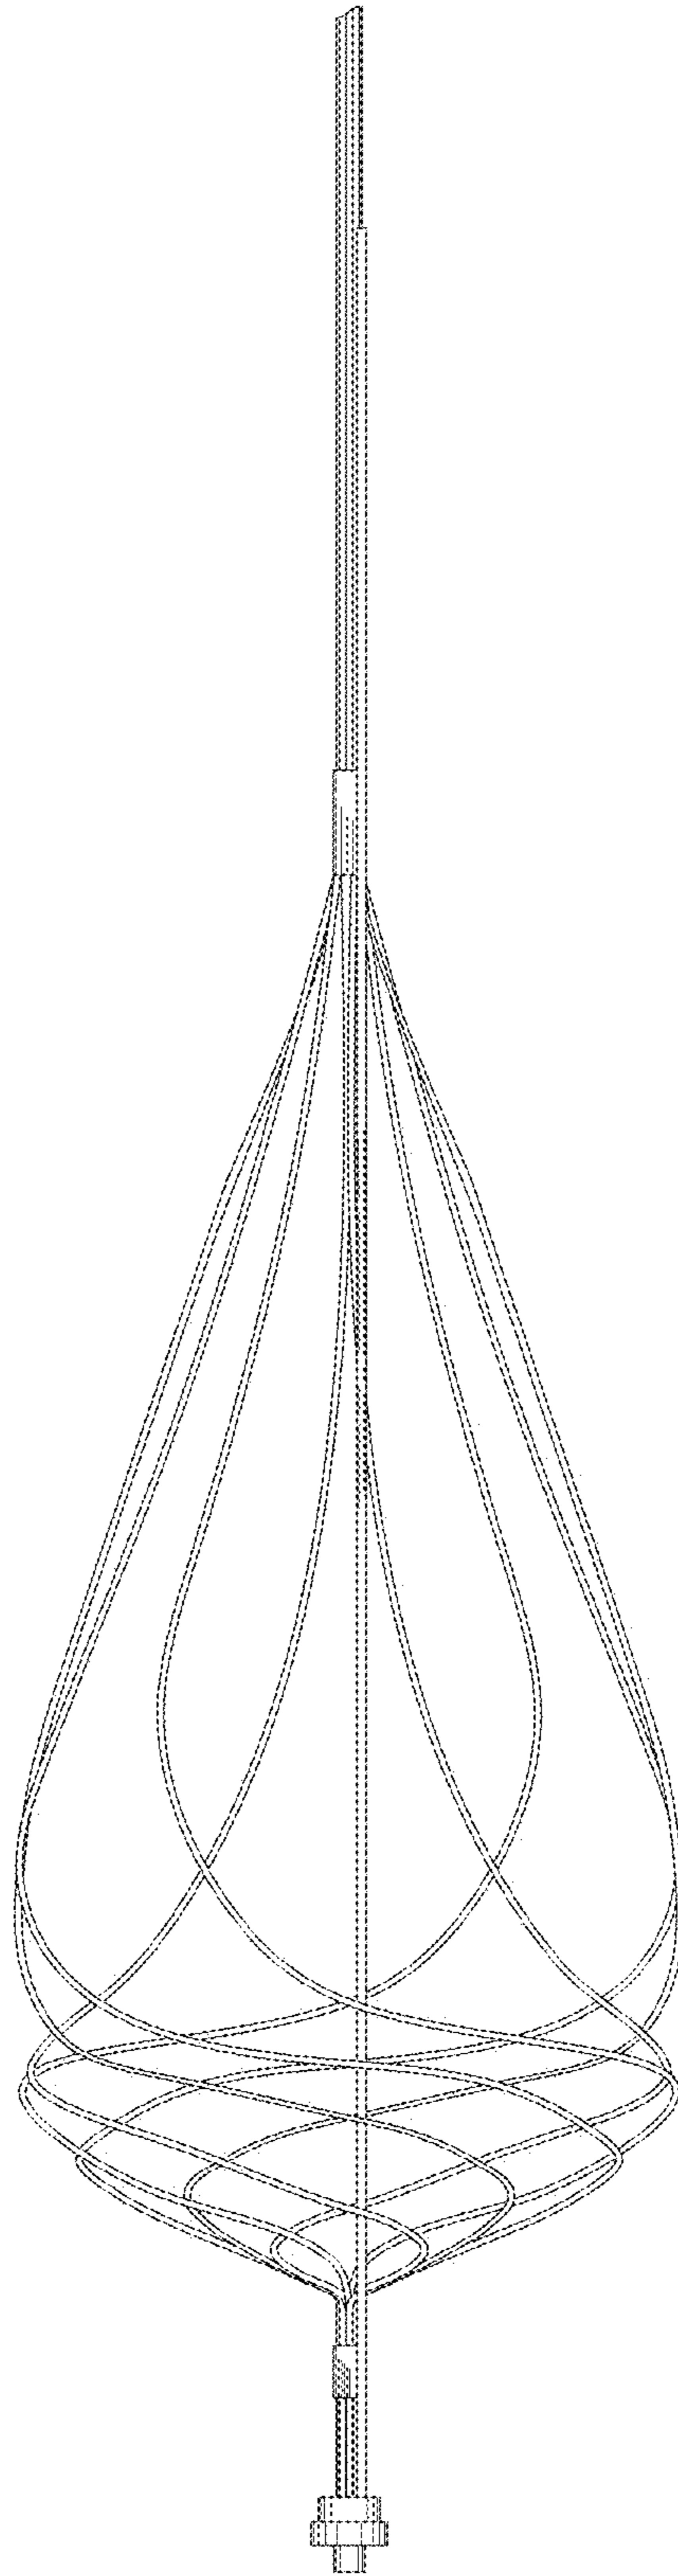


FIG. 23

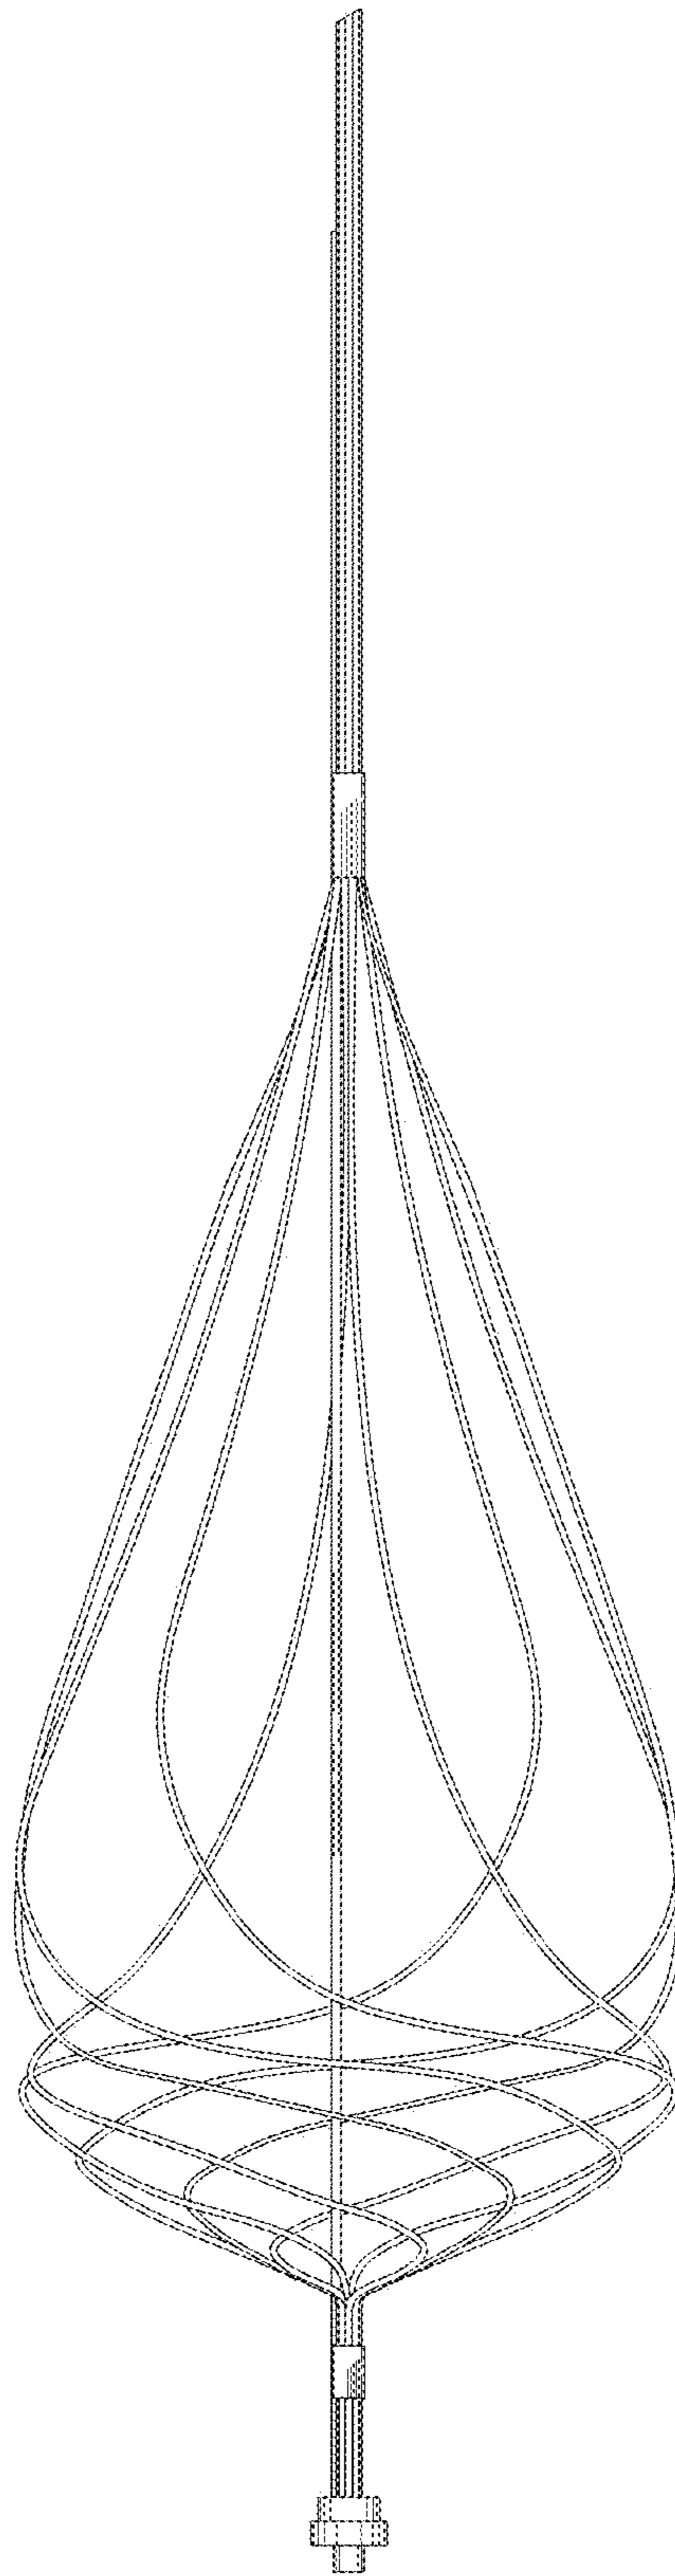


FIG. 24




FIG. 25

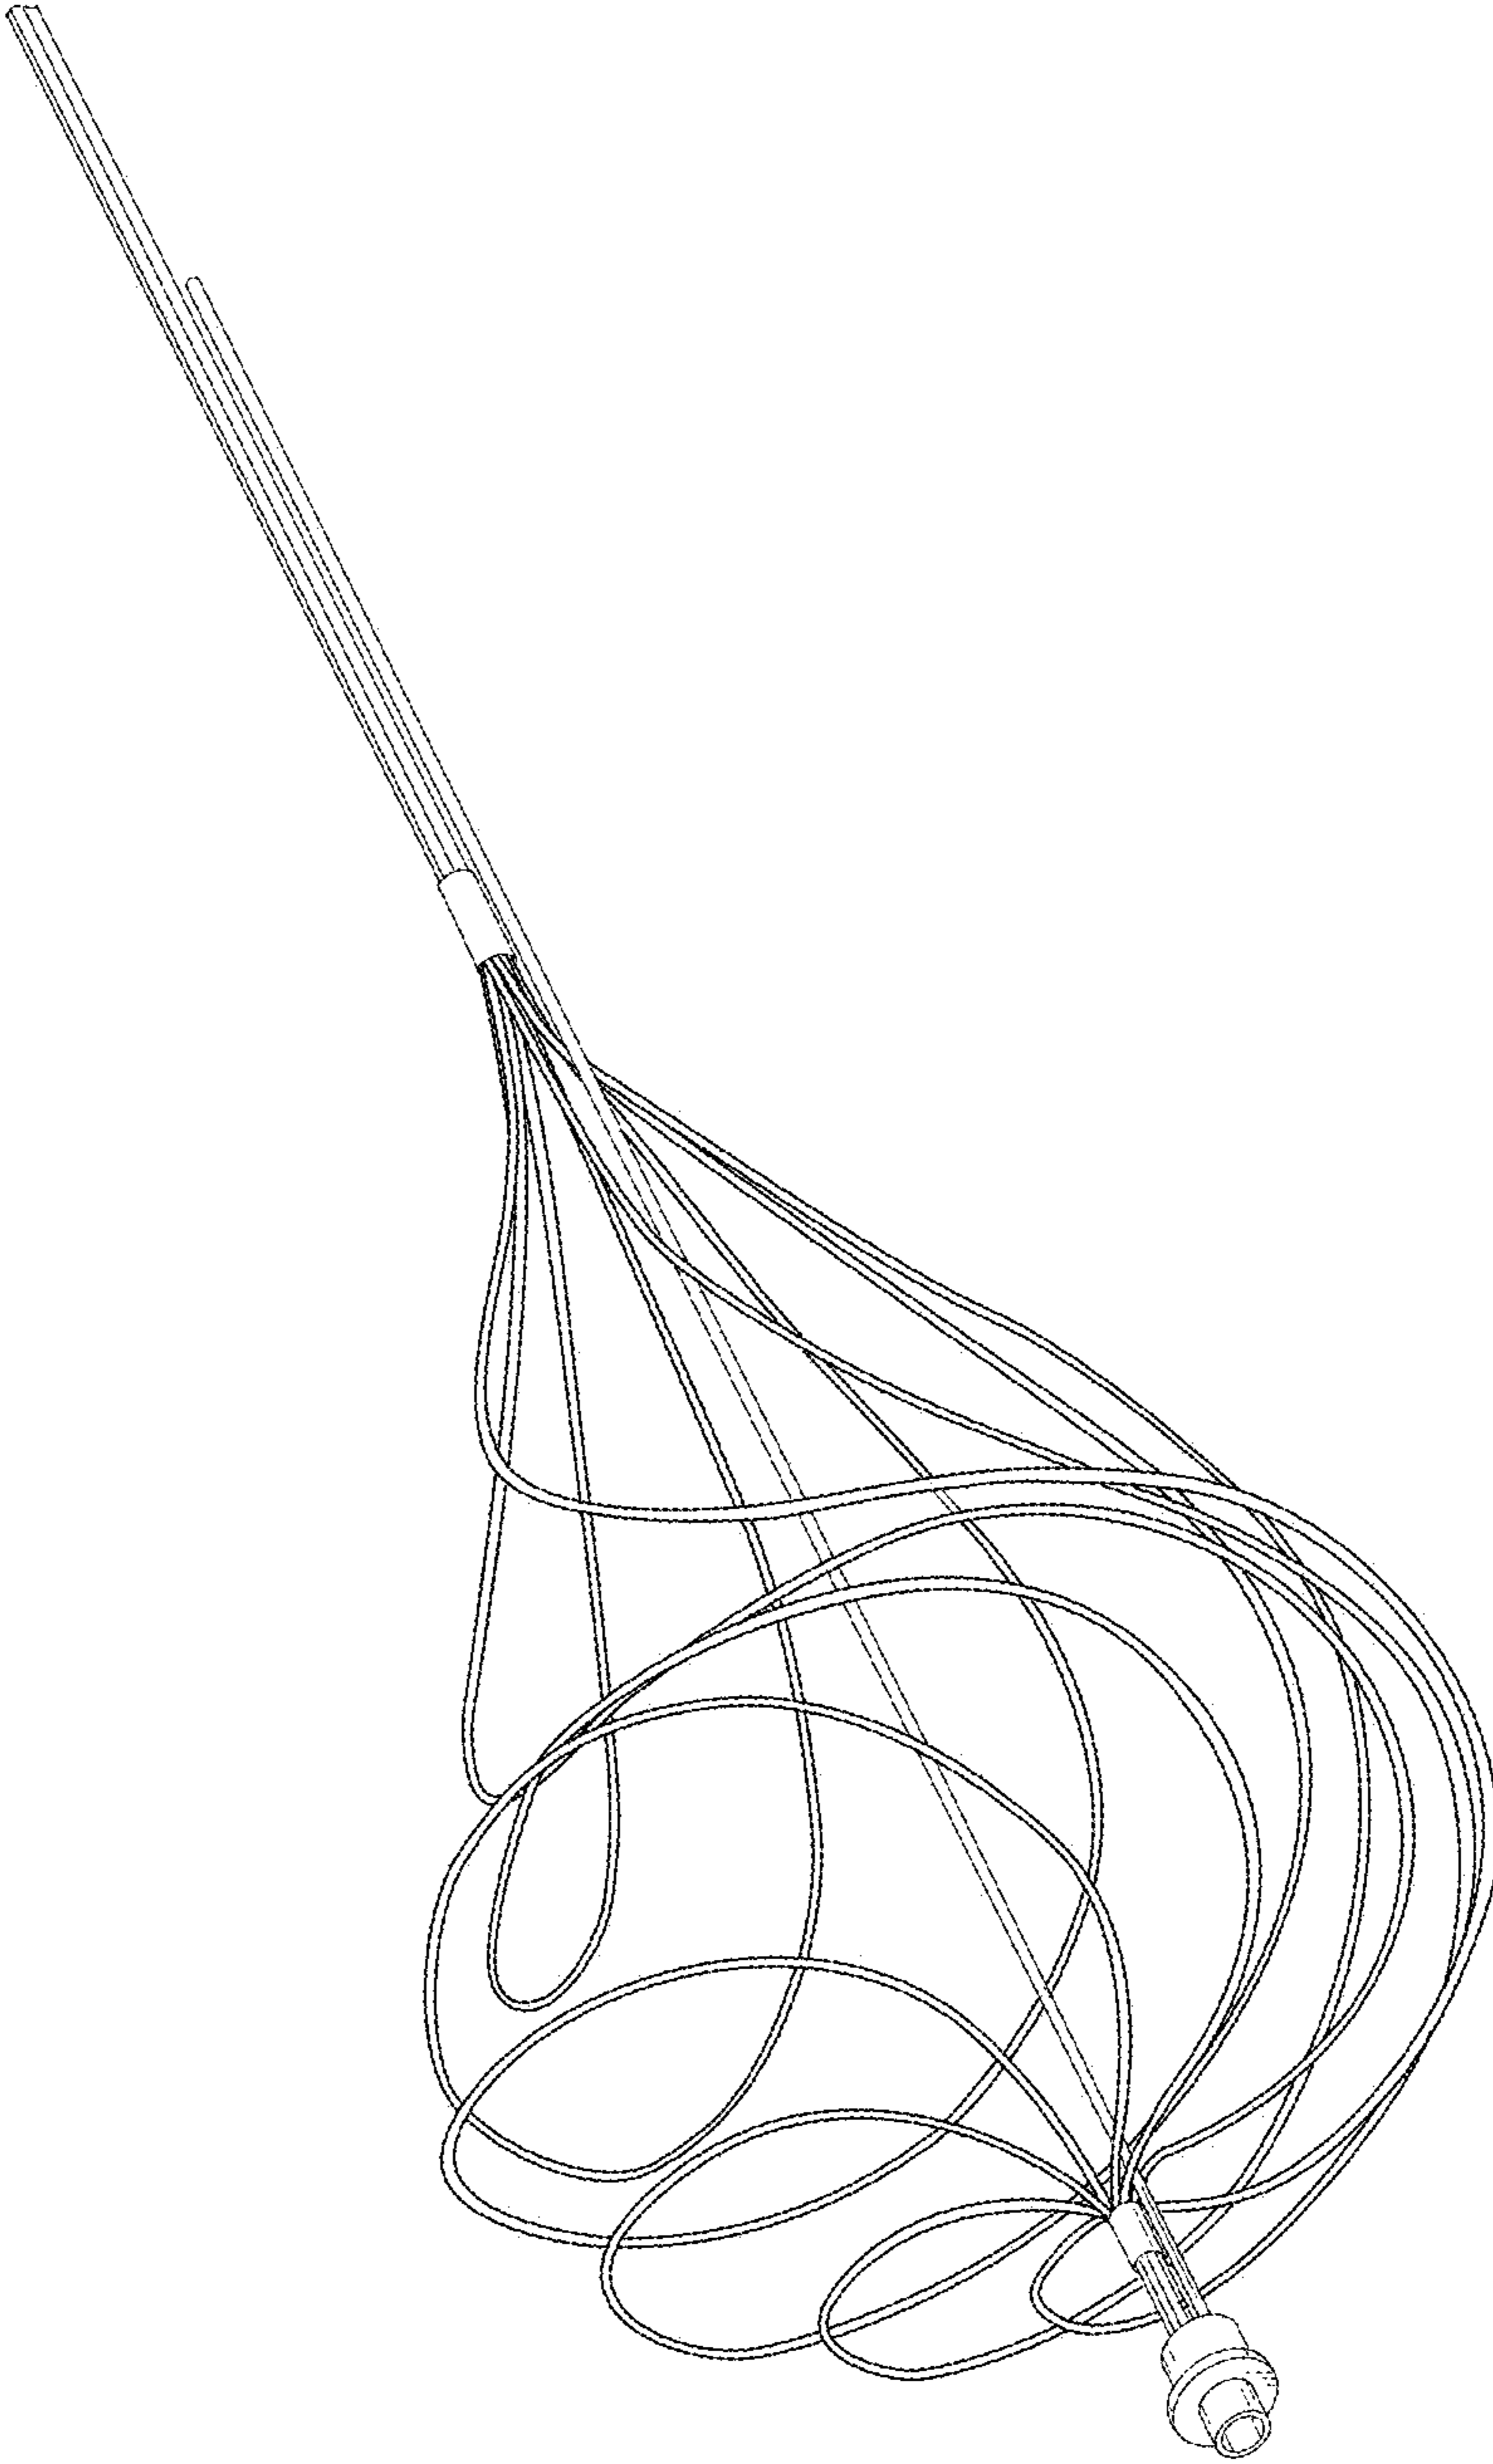


FIG. 26

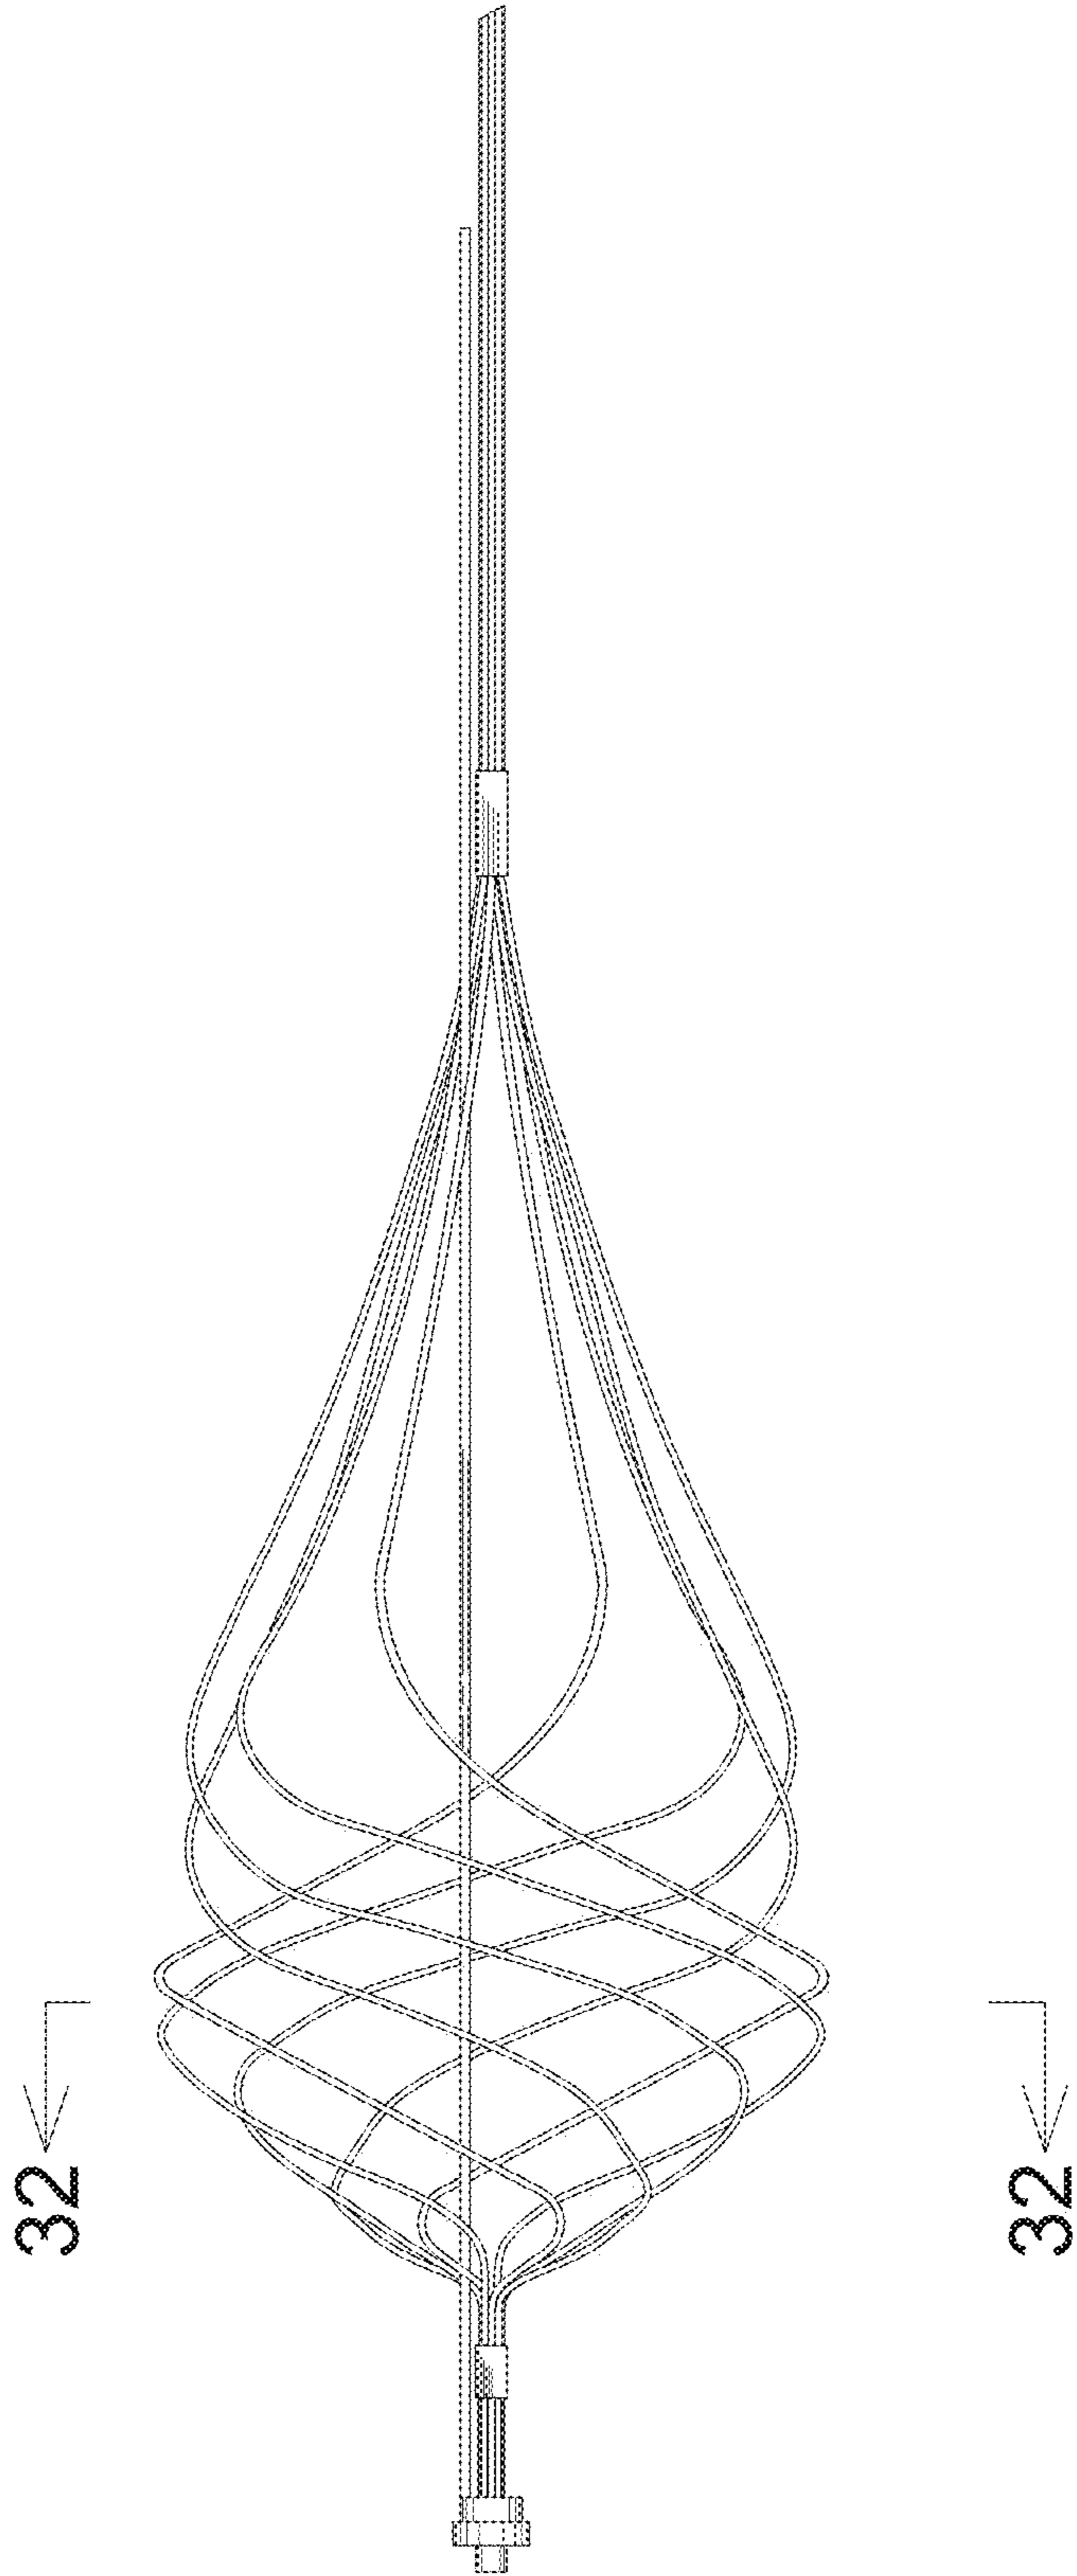


FIG. 27

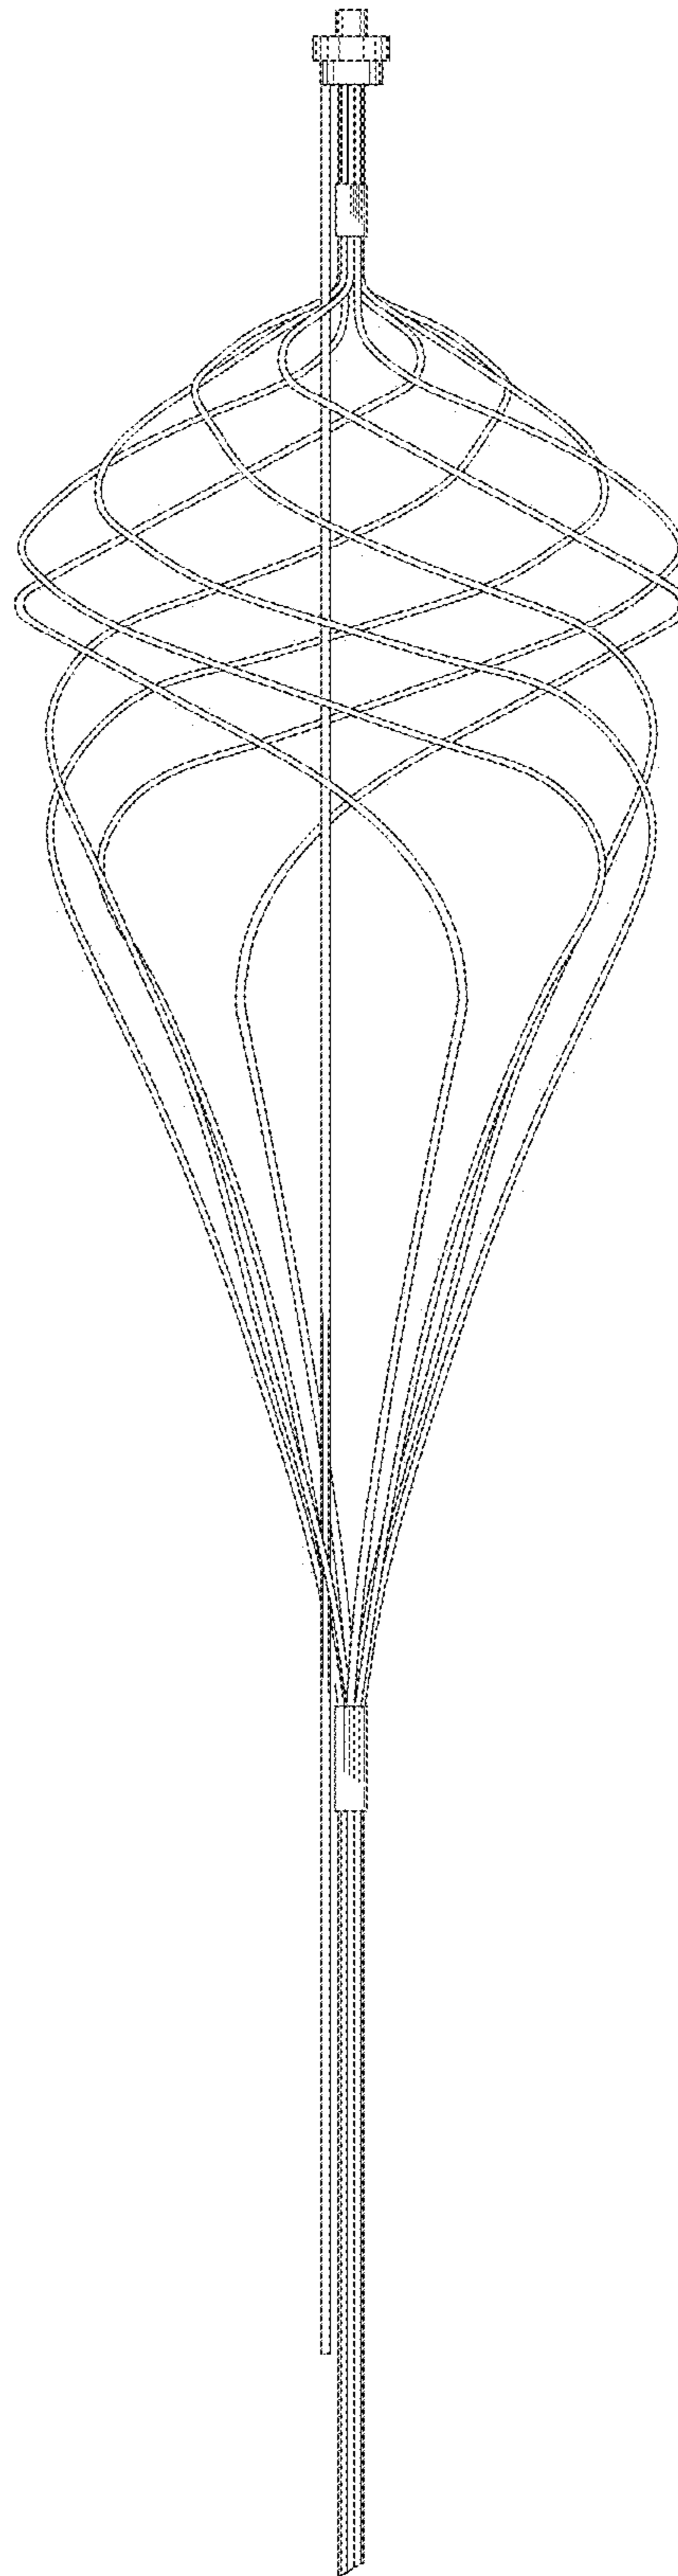


FIG. 28

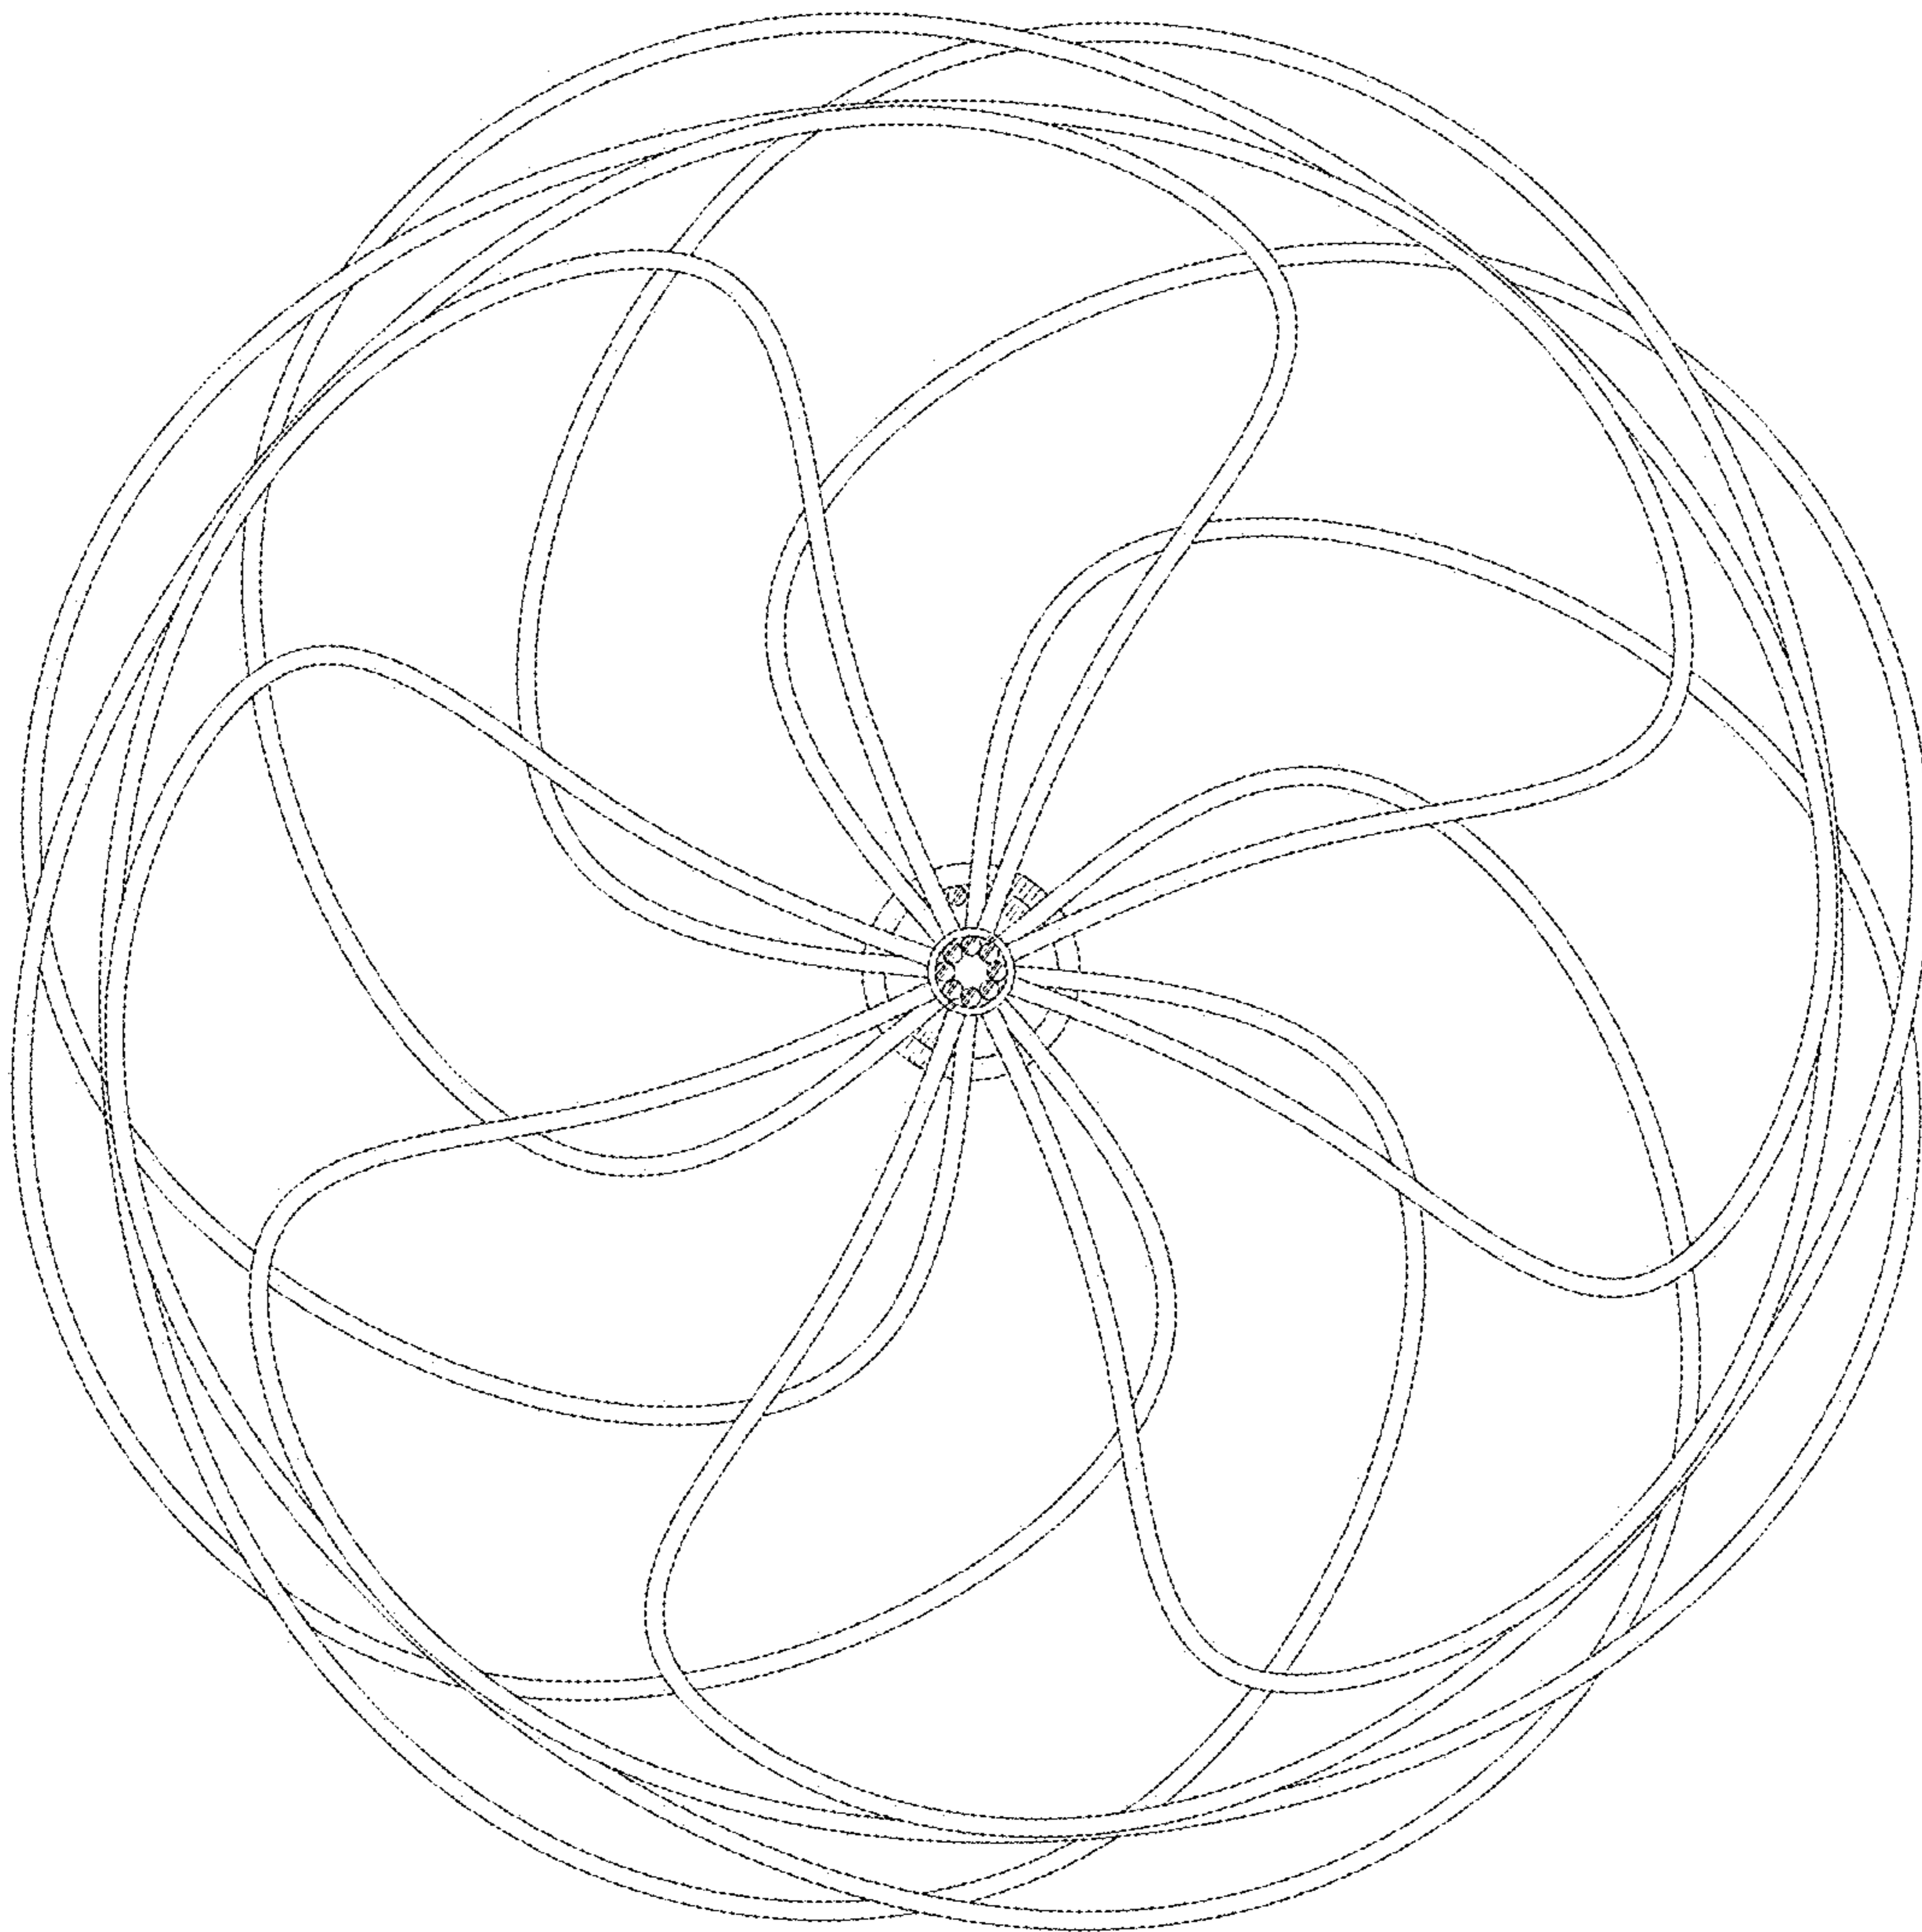


FIG. 29

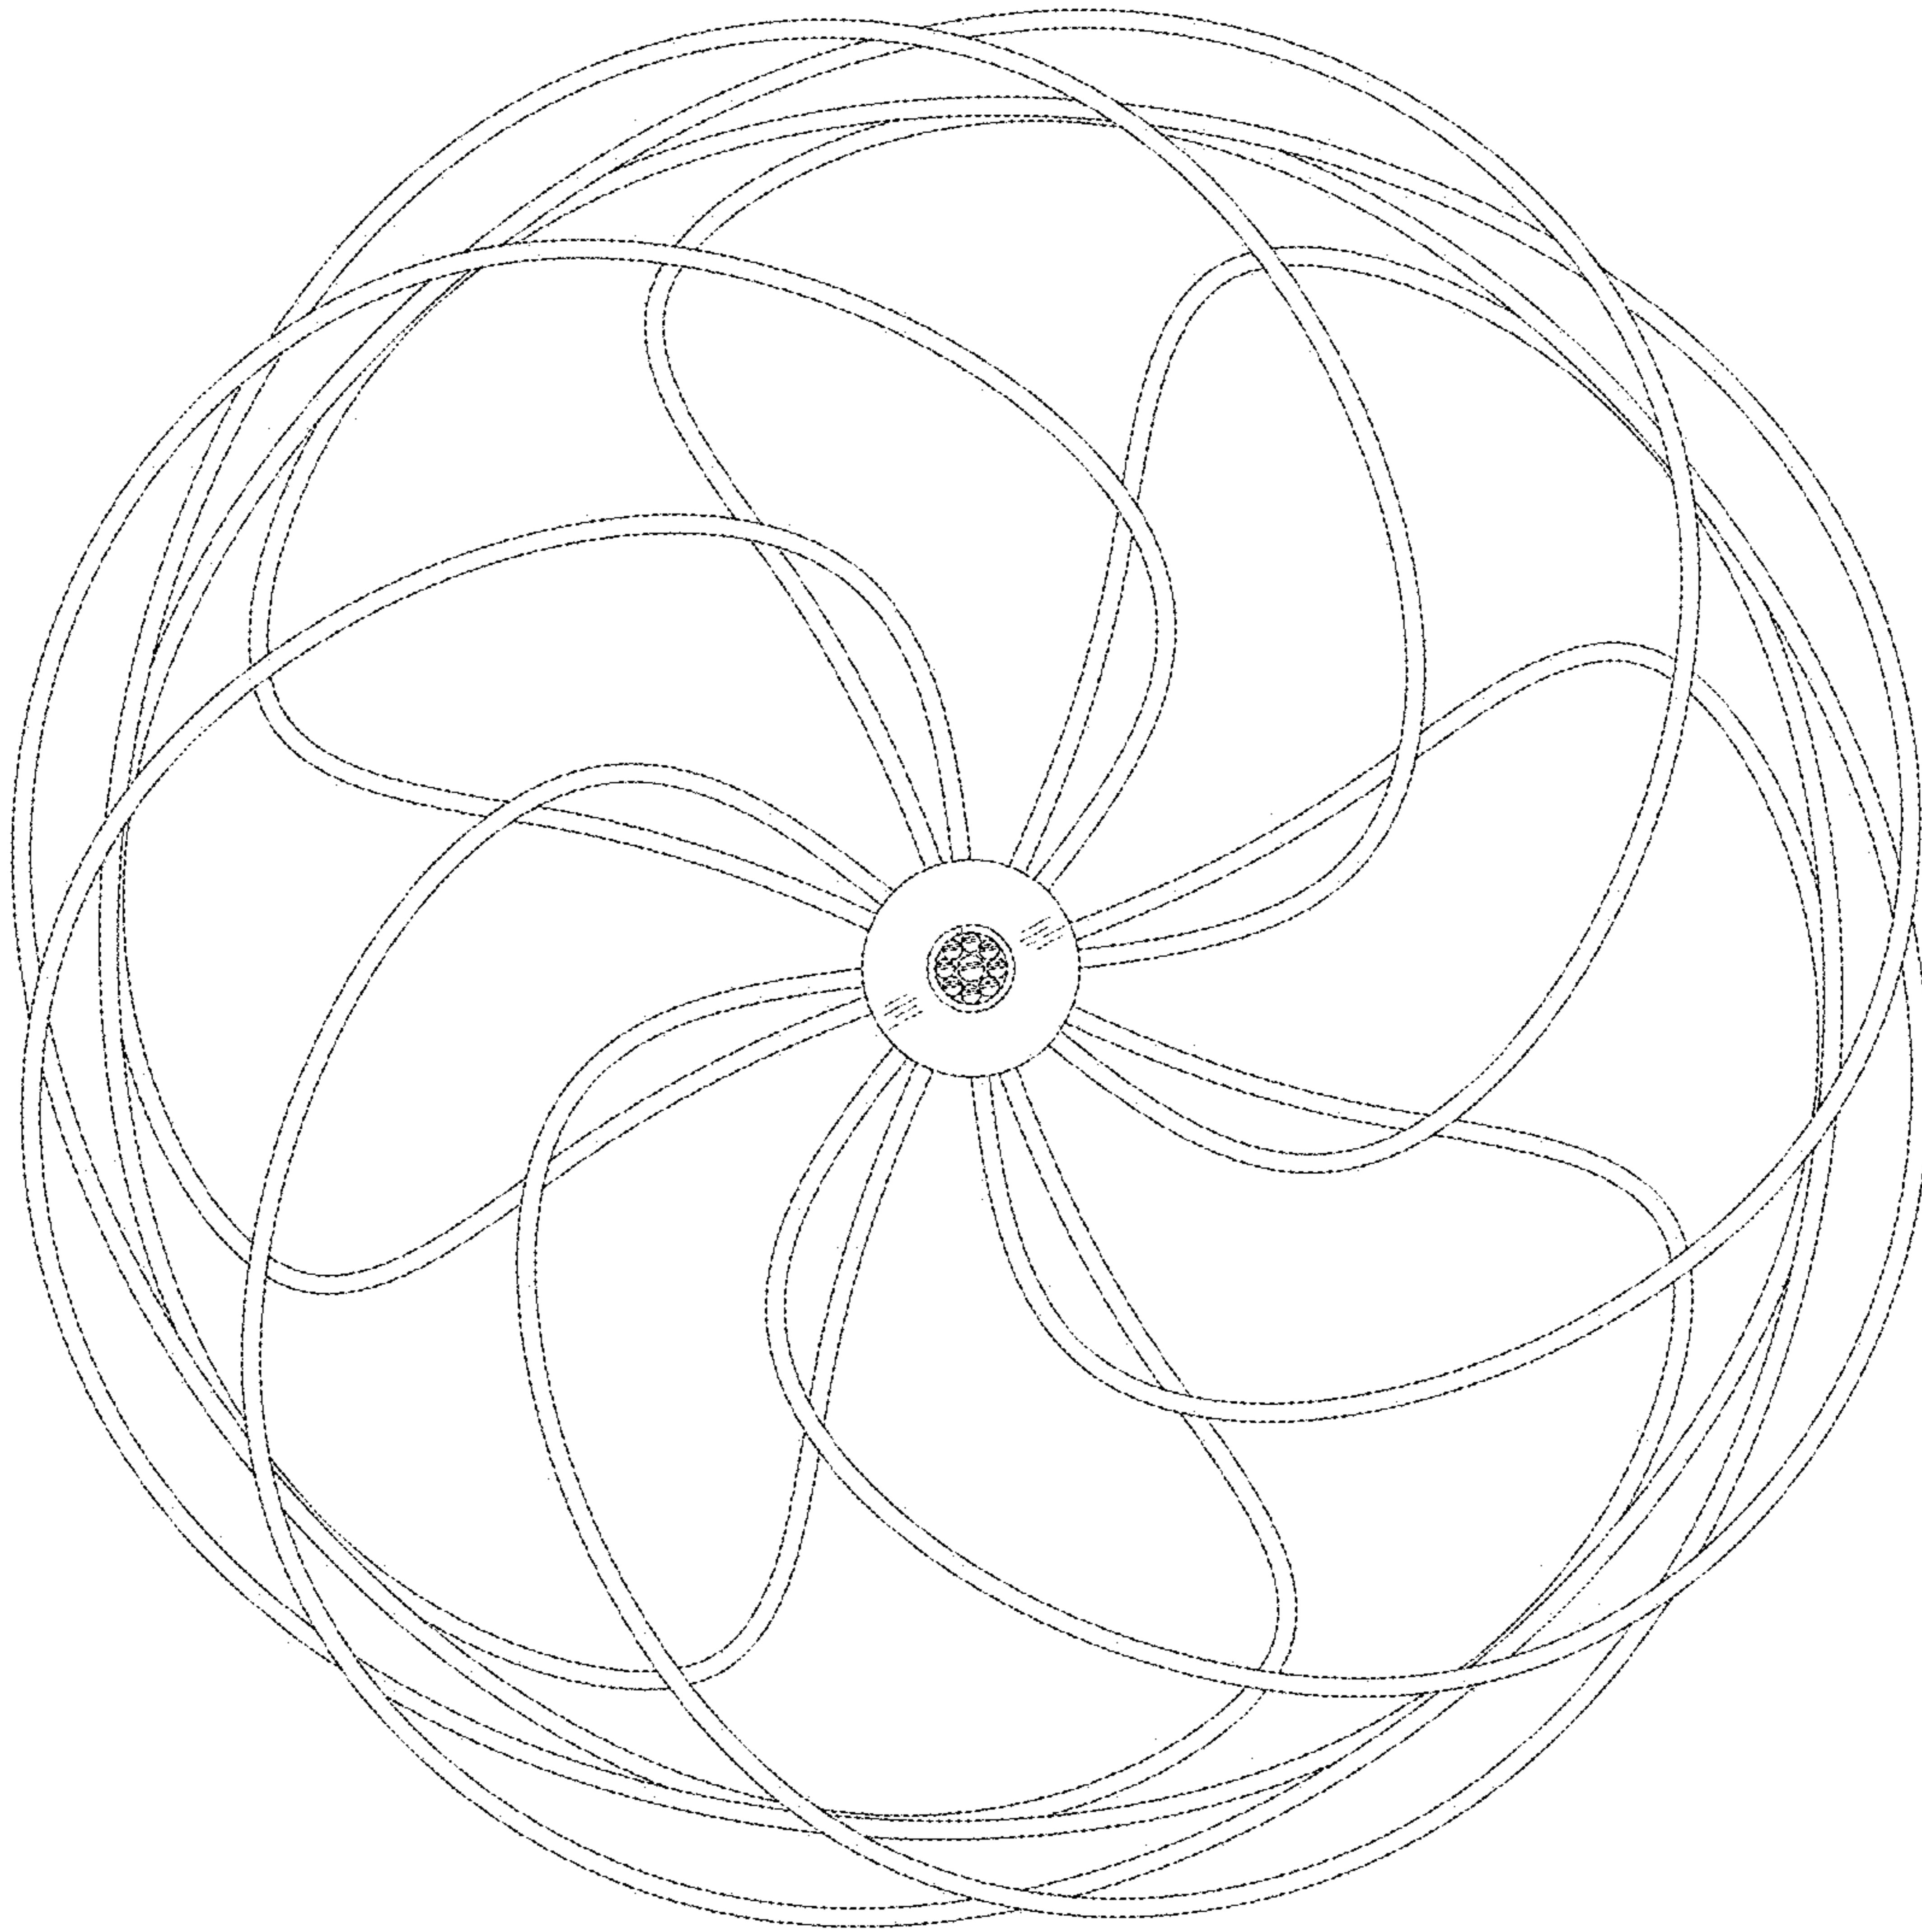


FIG. 30

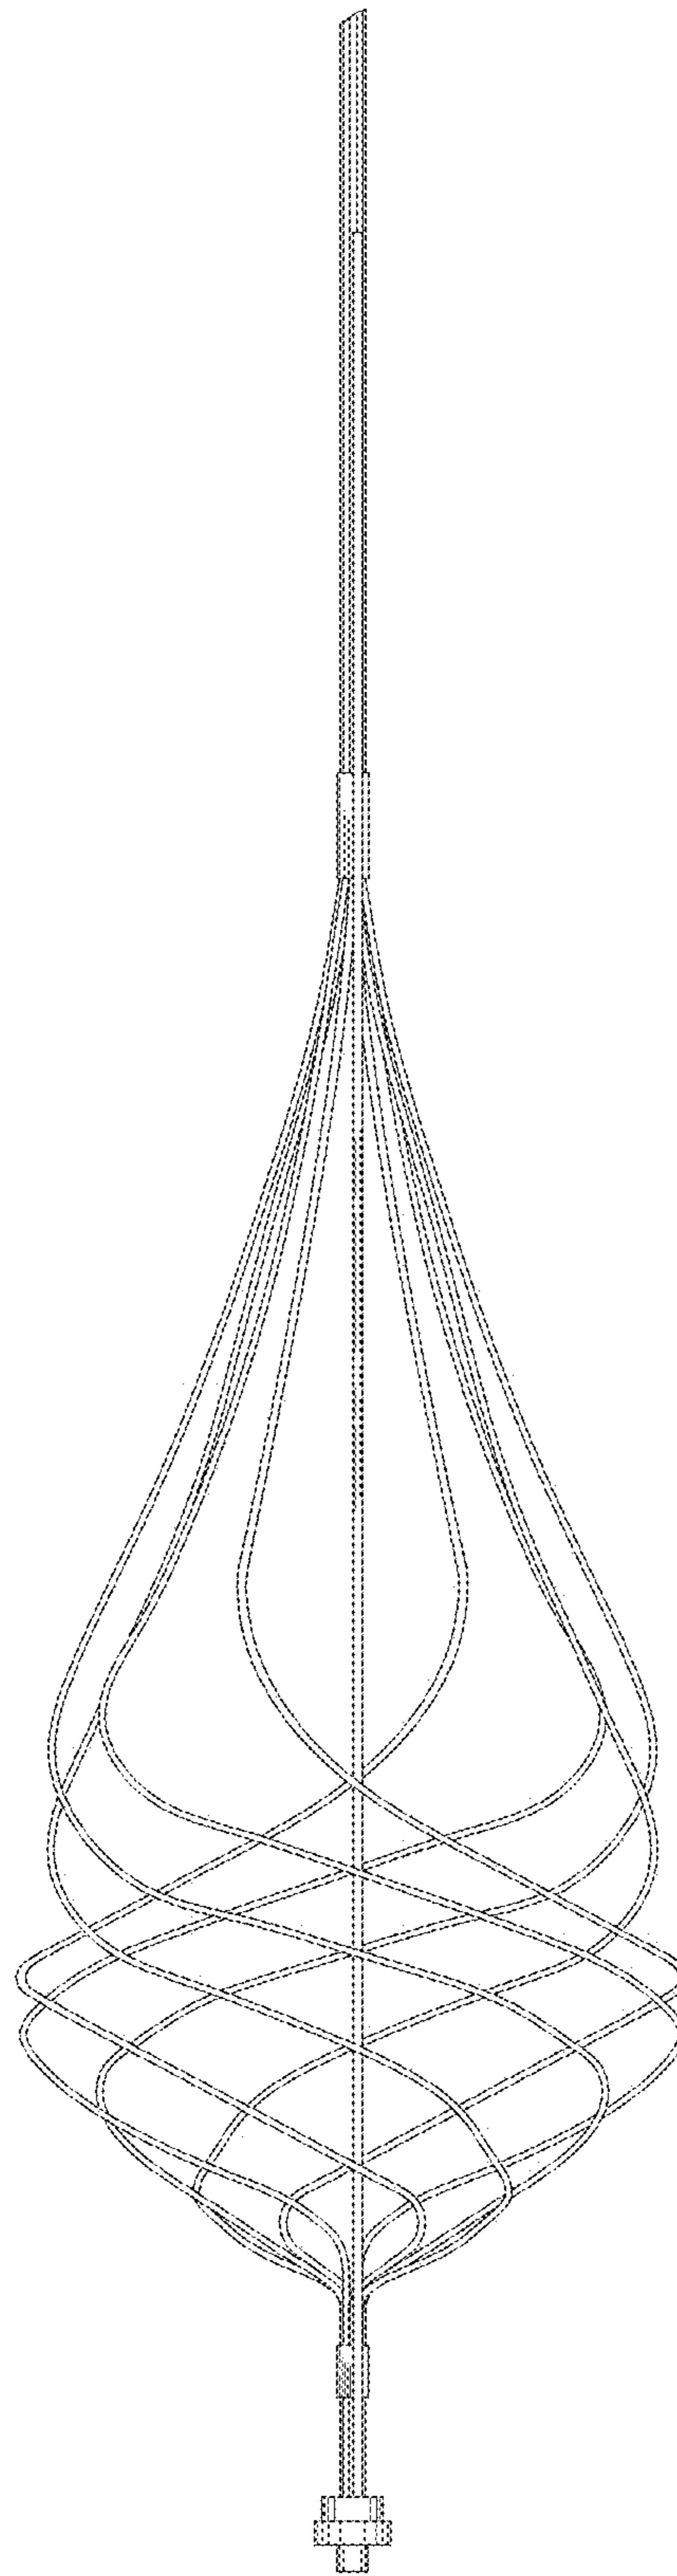


FIG. 31

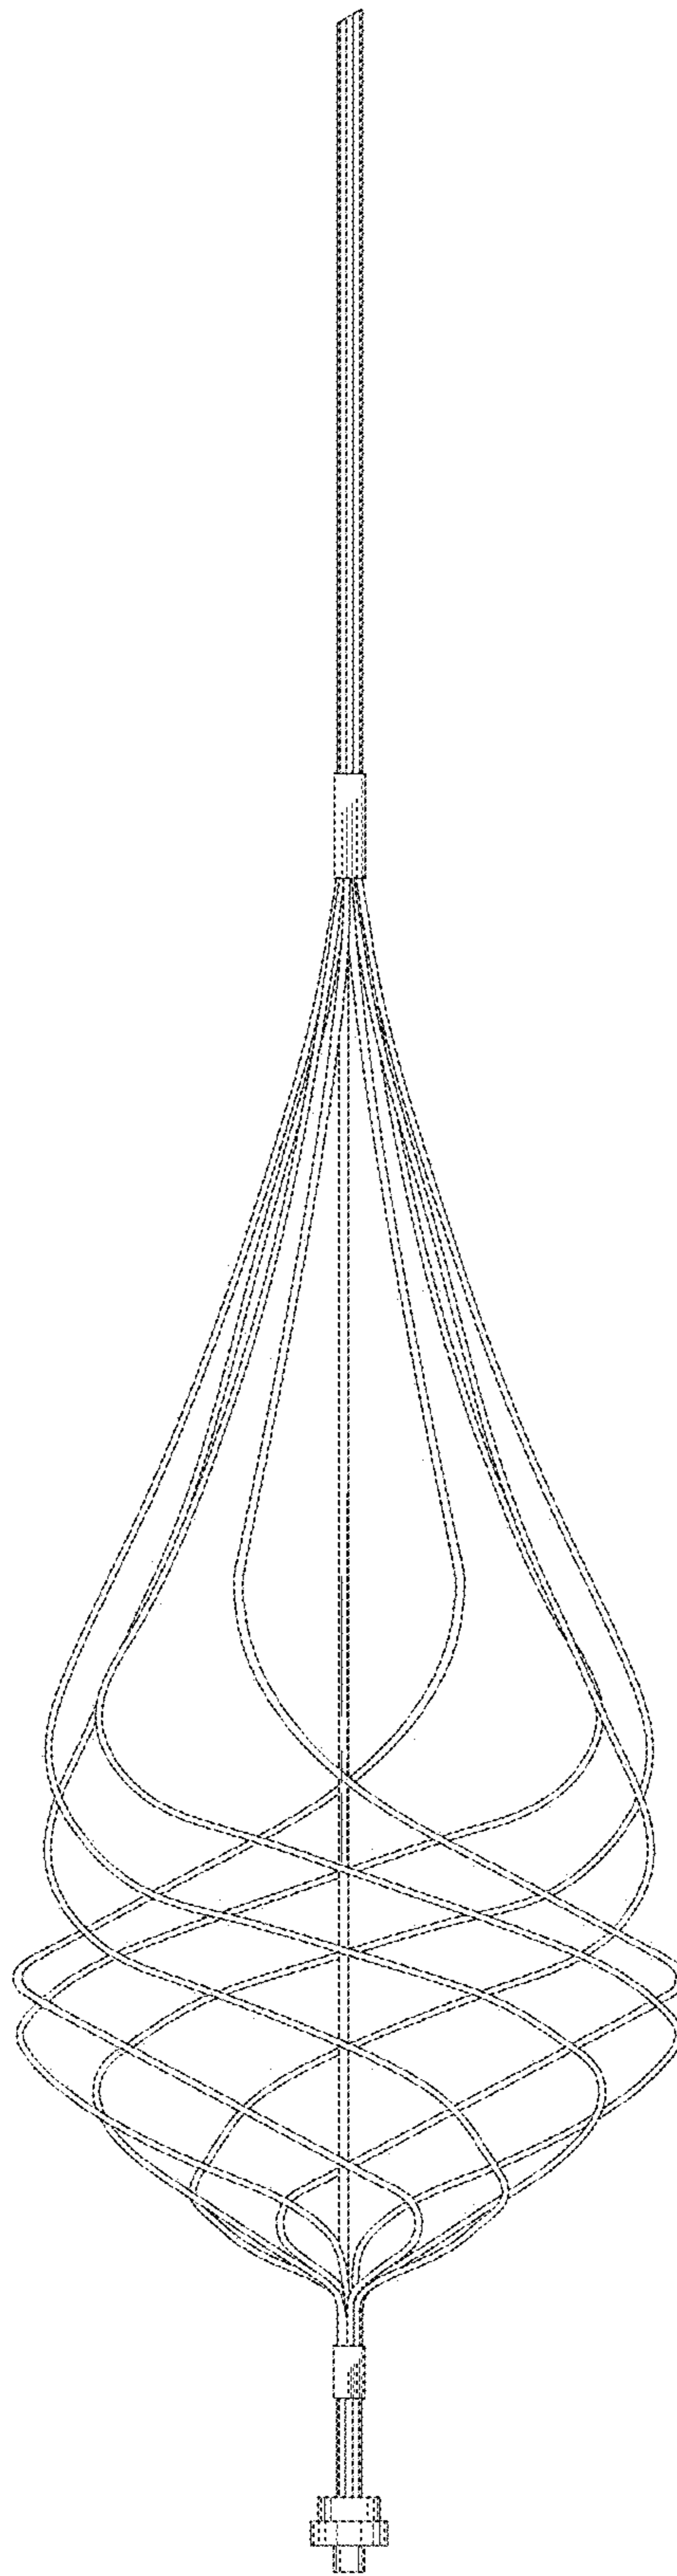


FIG. 32




FIG. 33

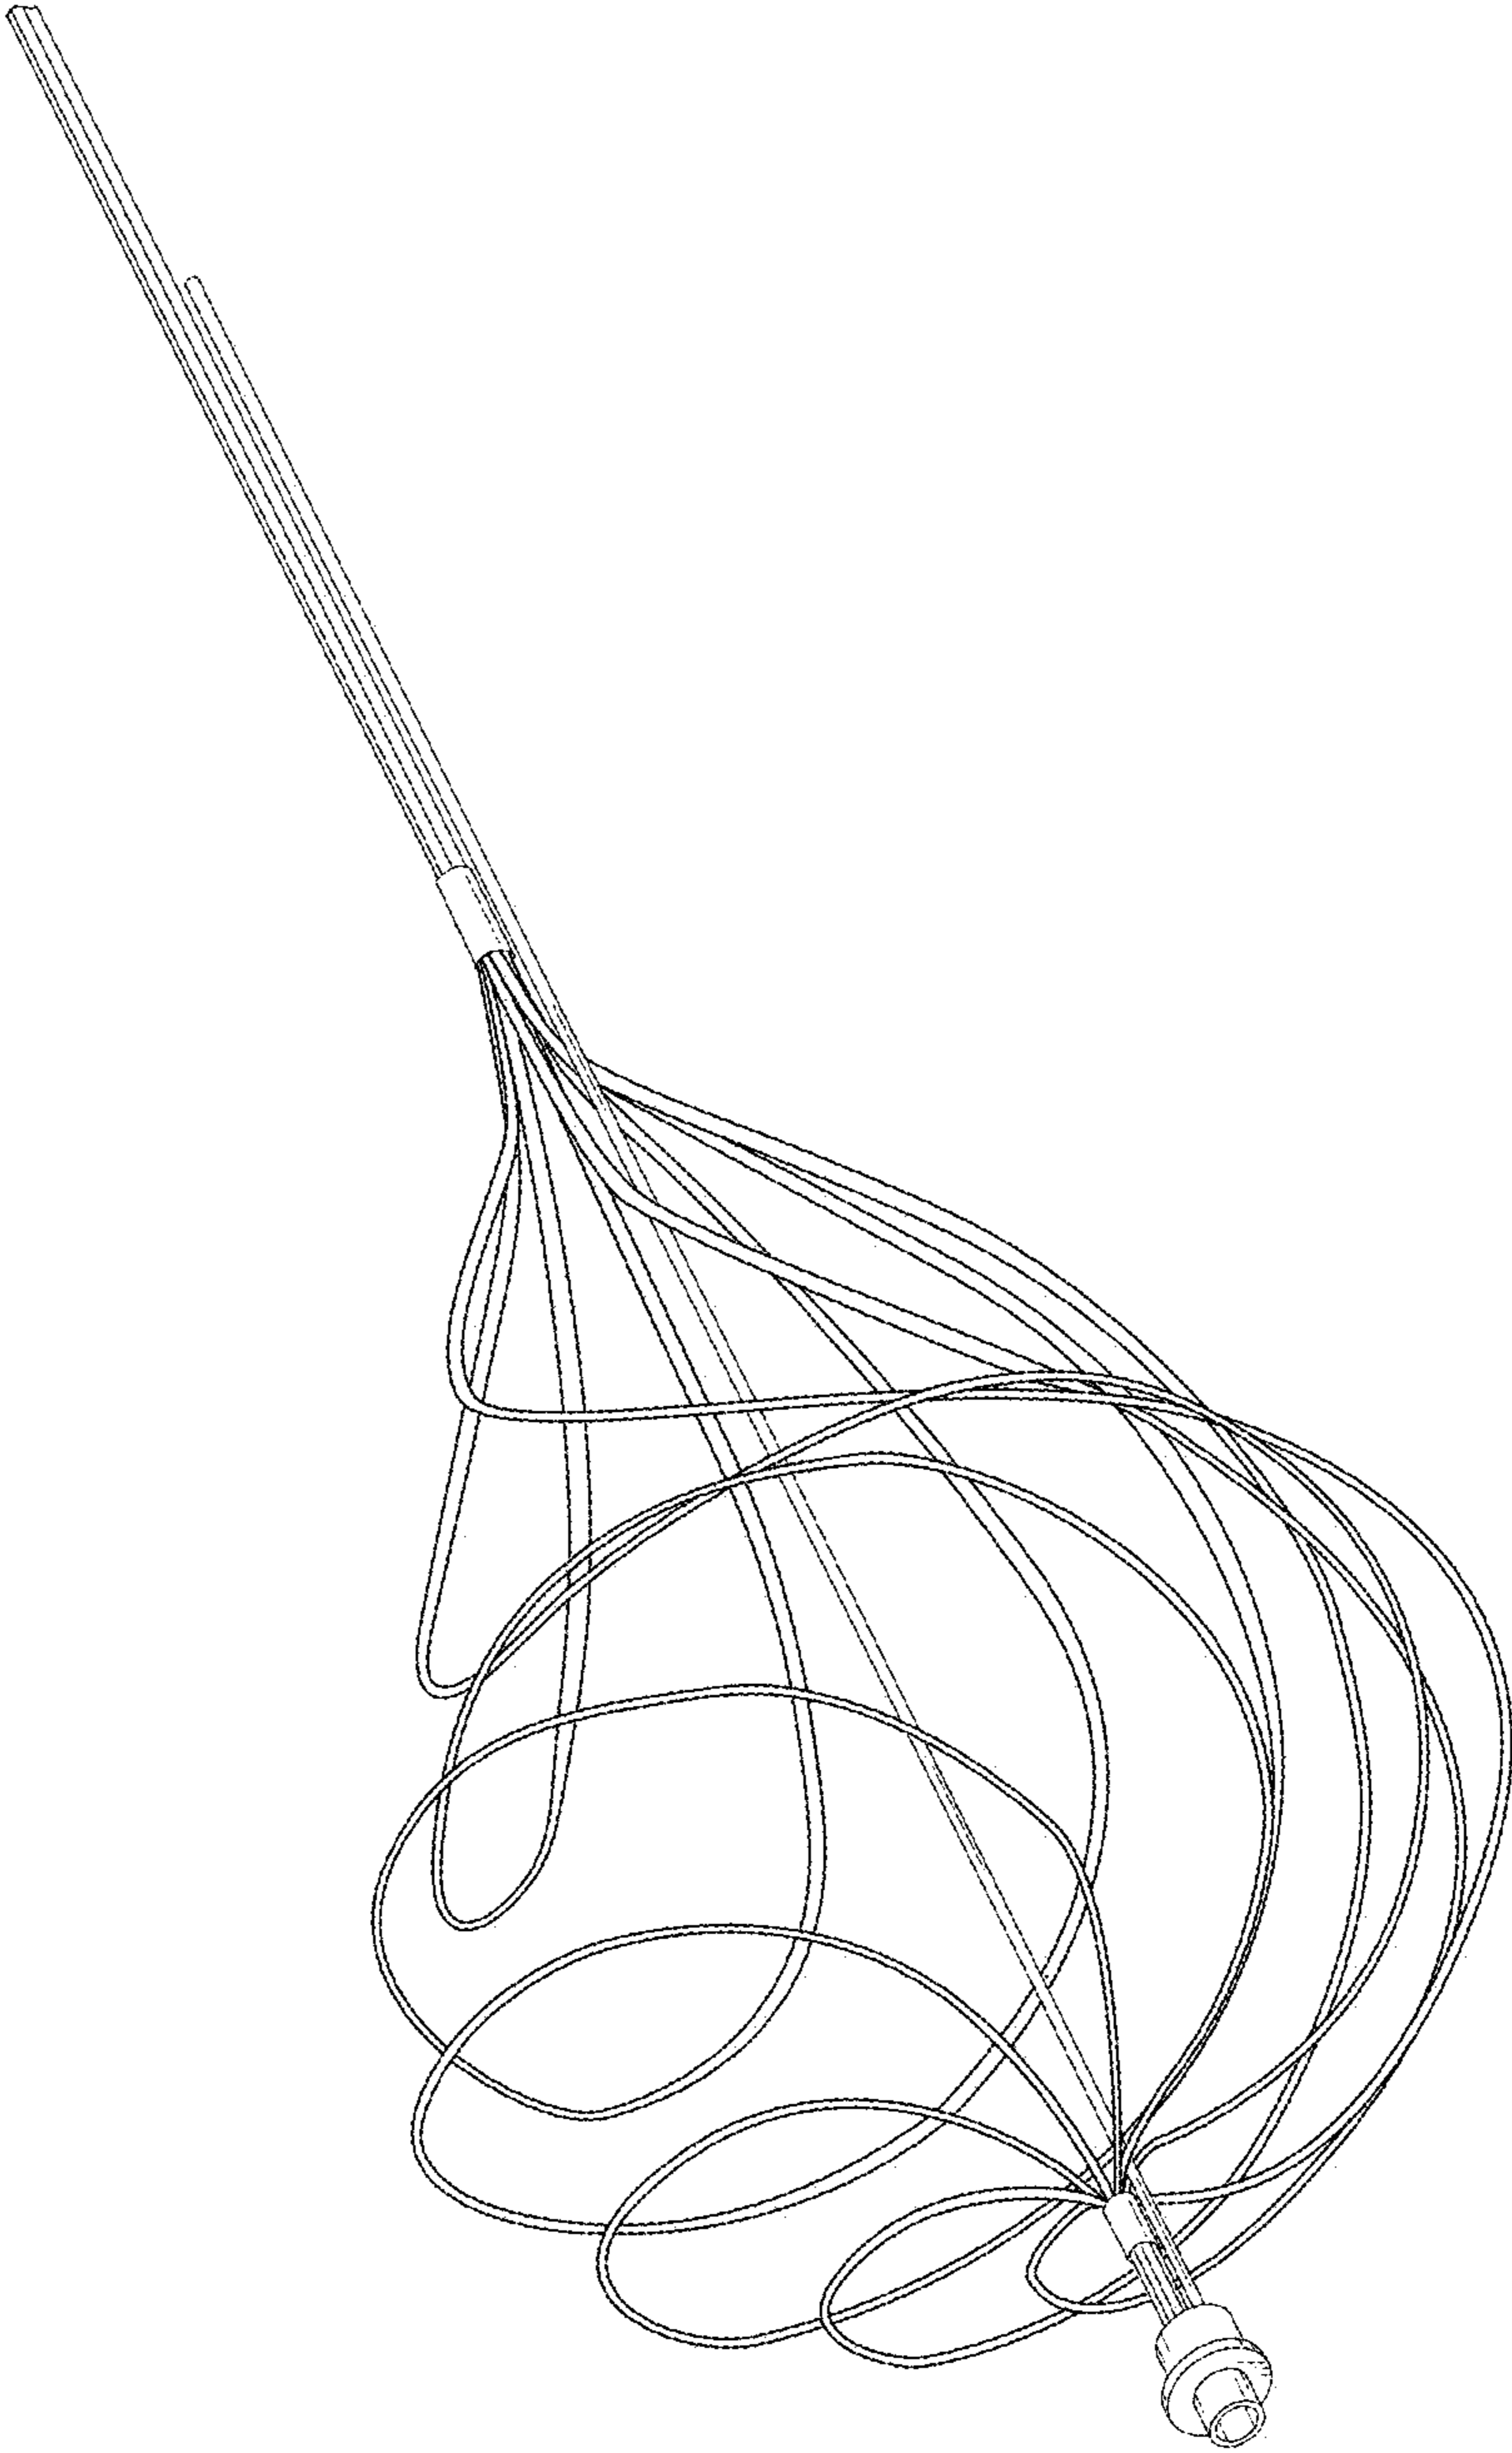


FIG. 34

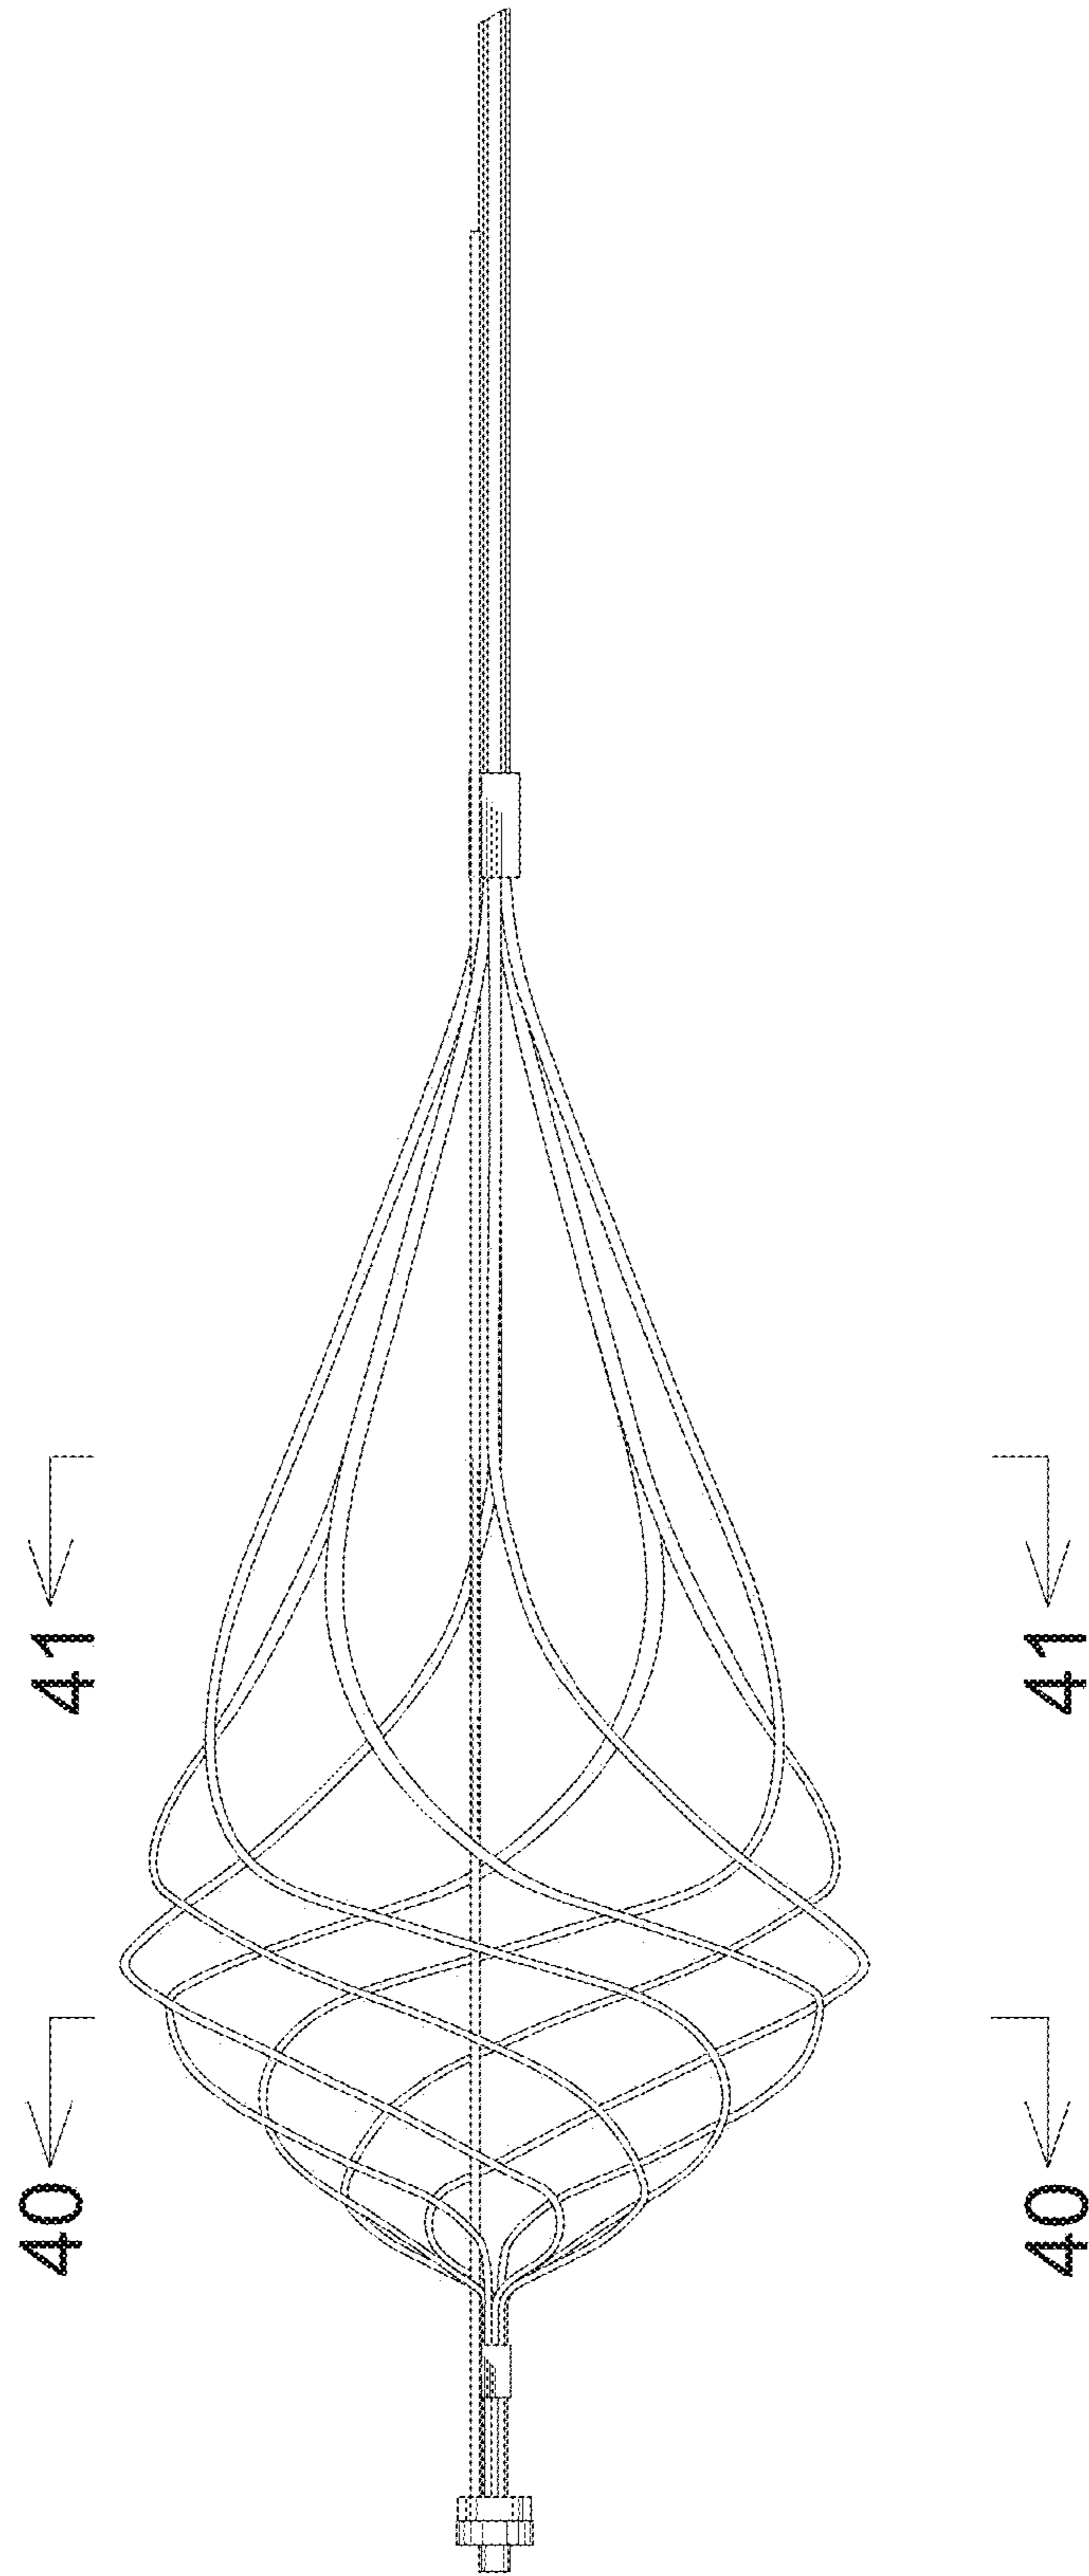


FIG. 35

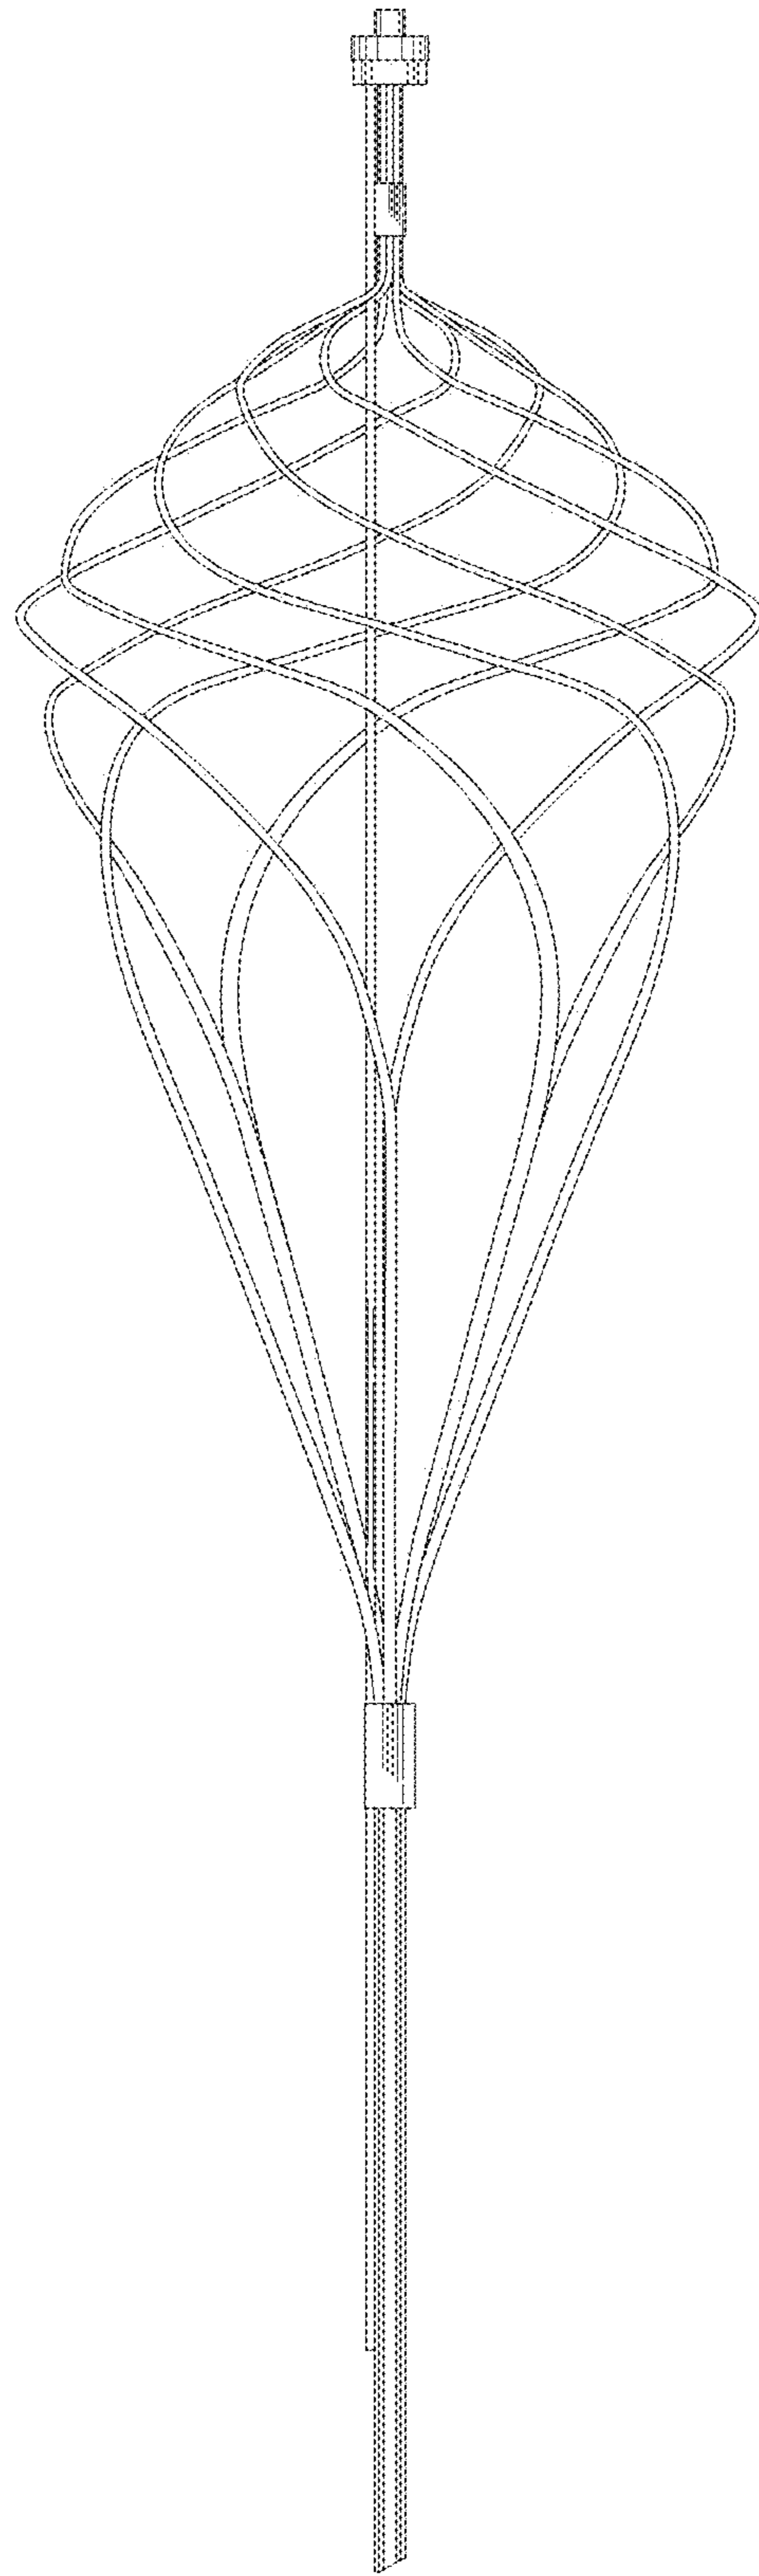


FIG. 36

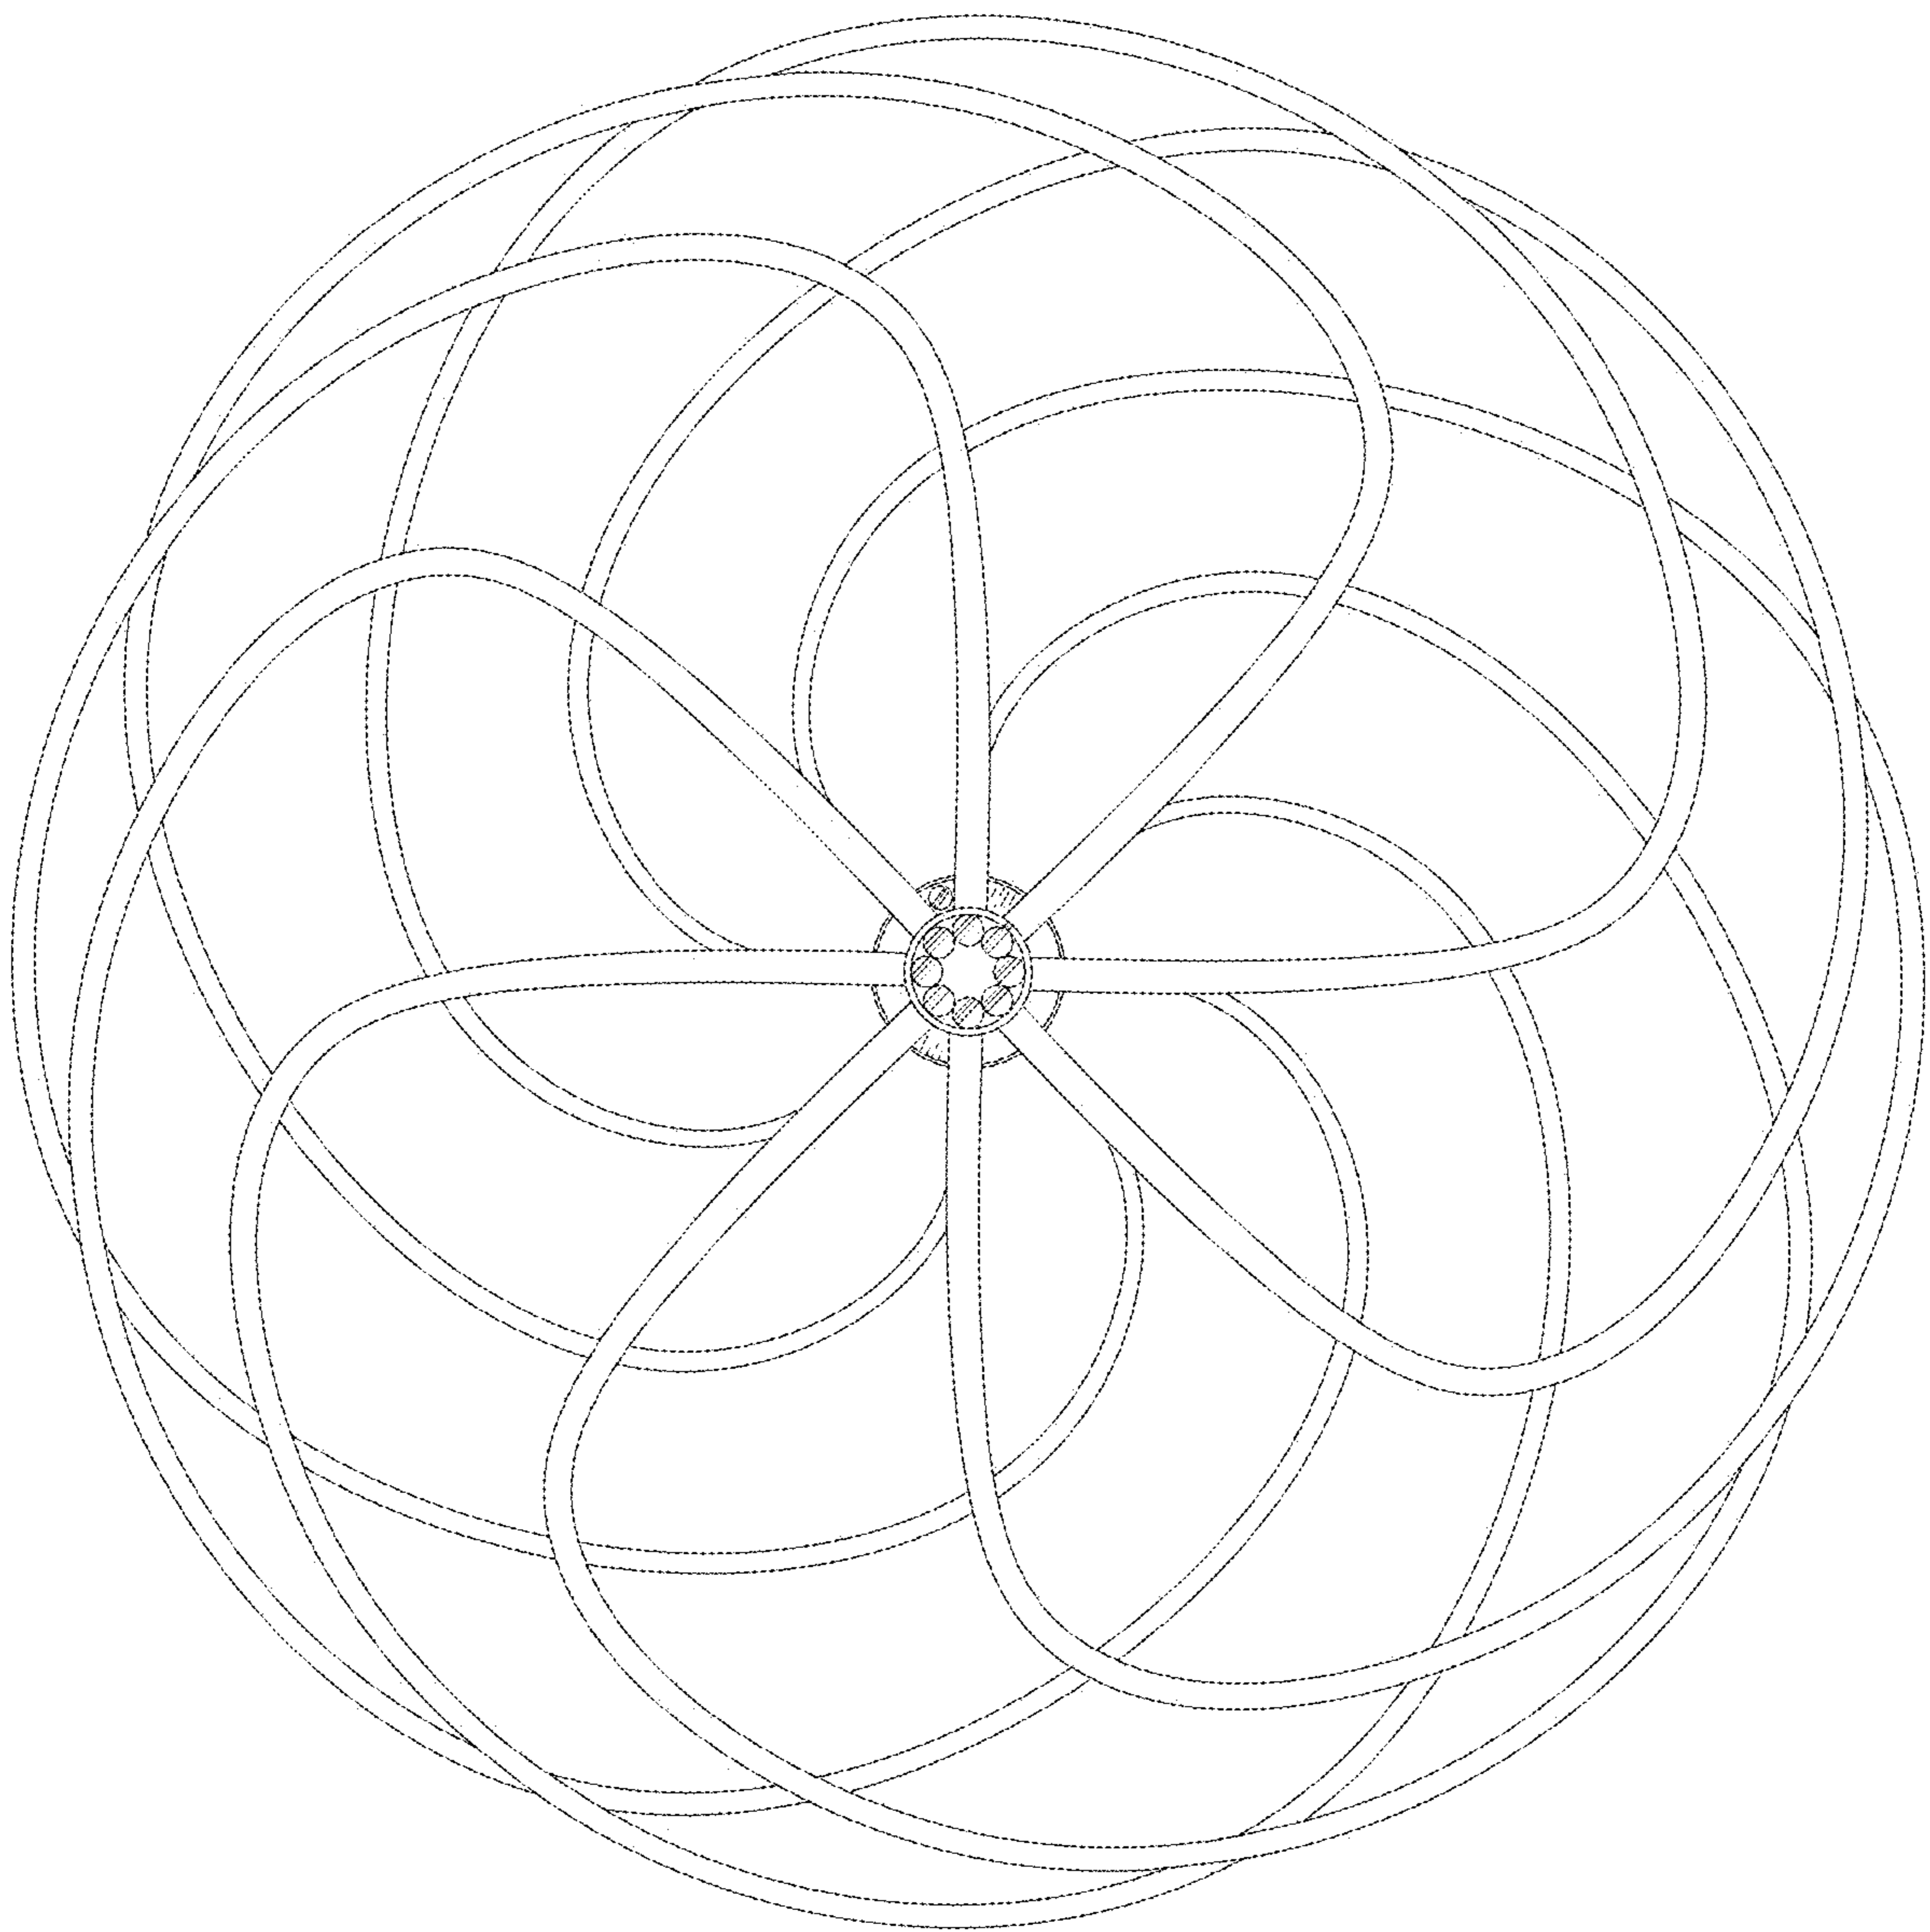


FIG. 37

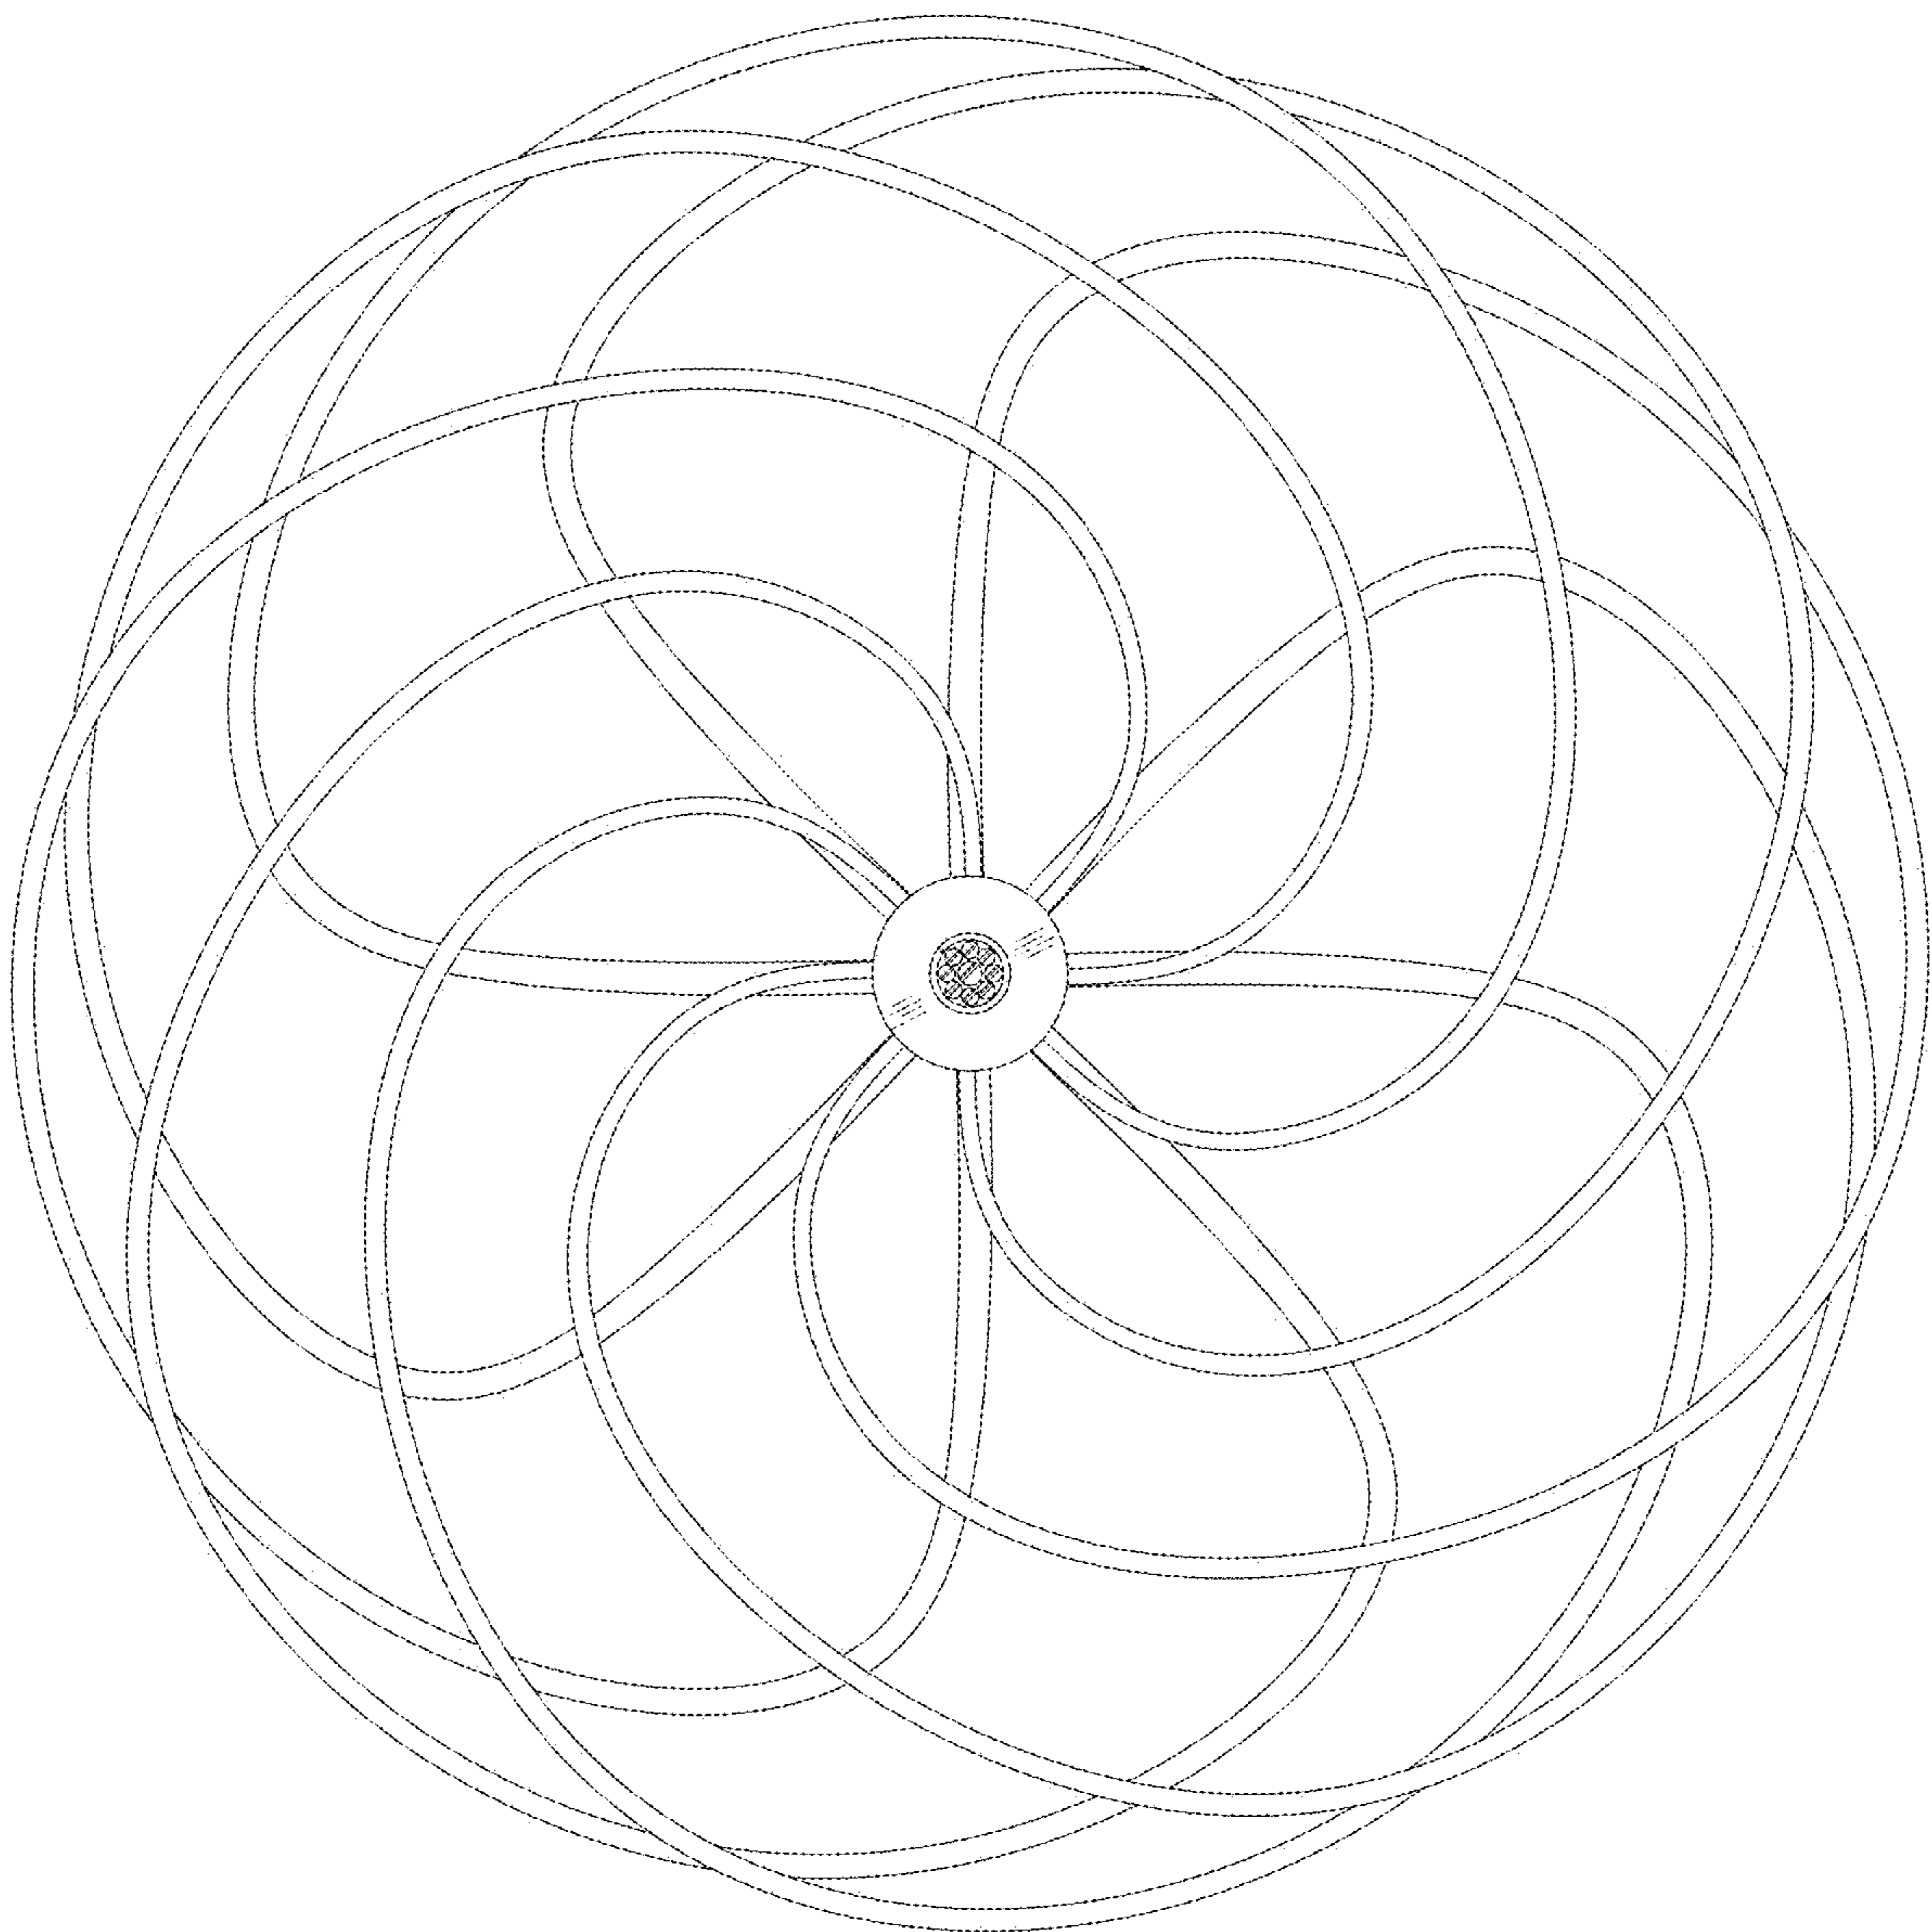


FIG. 38

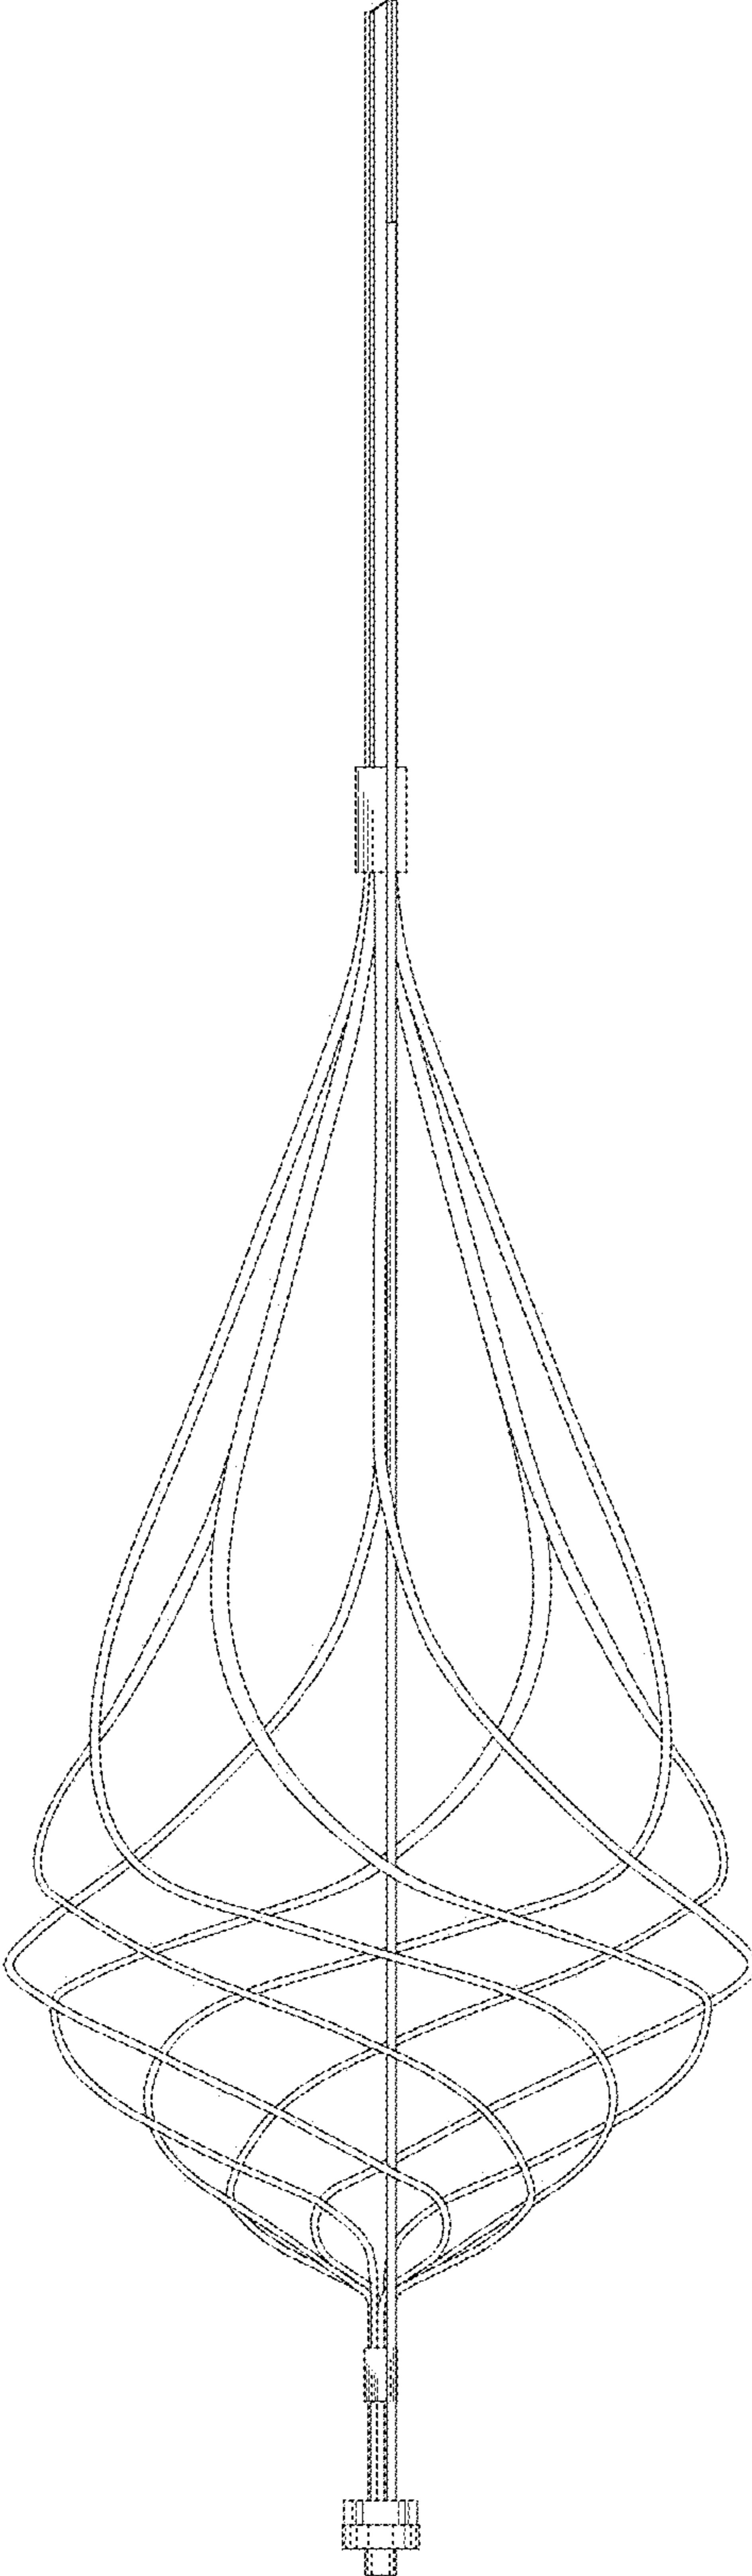


FIG. 39

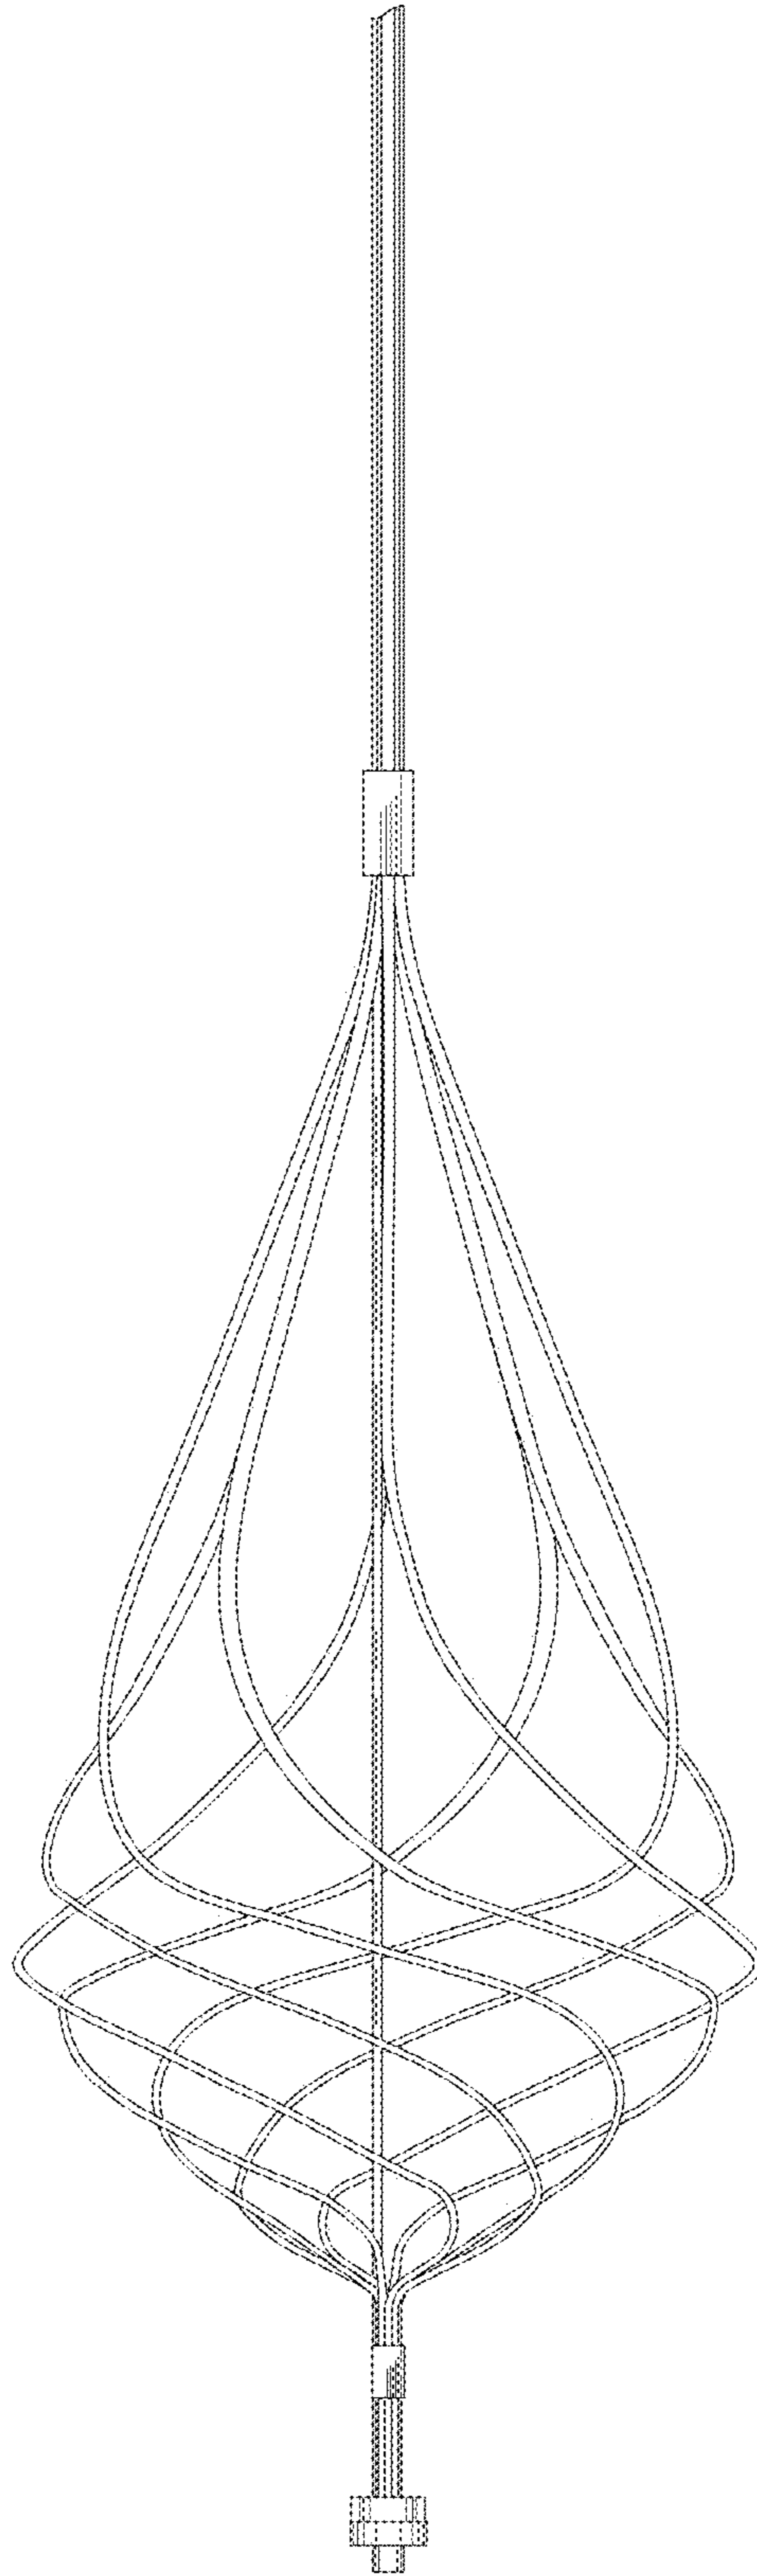


FIG. 40



FIG. 41

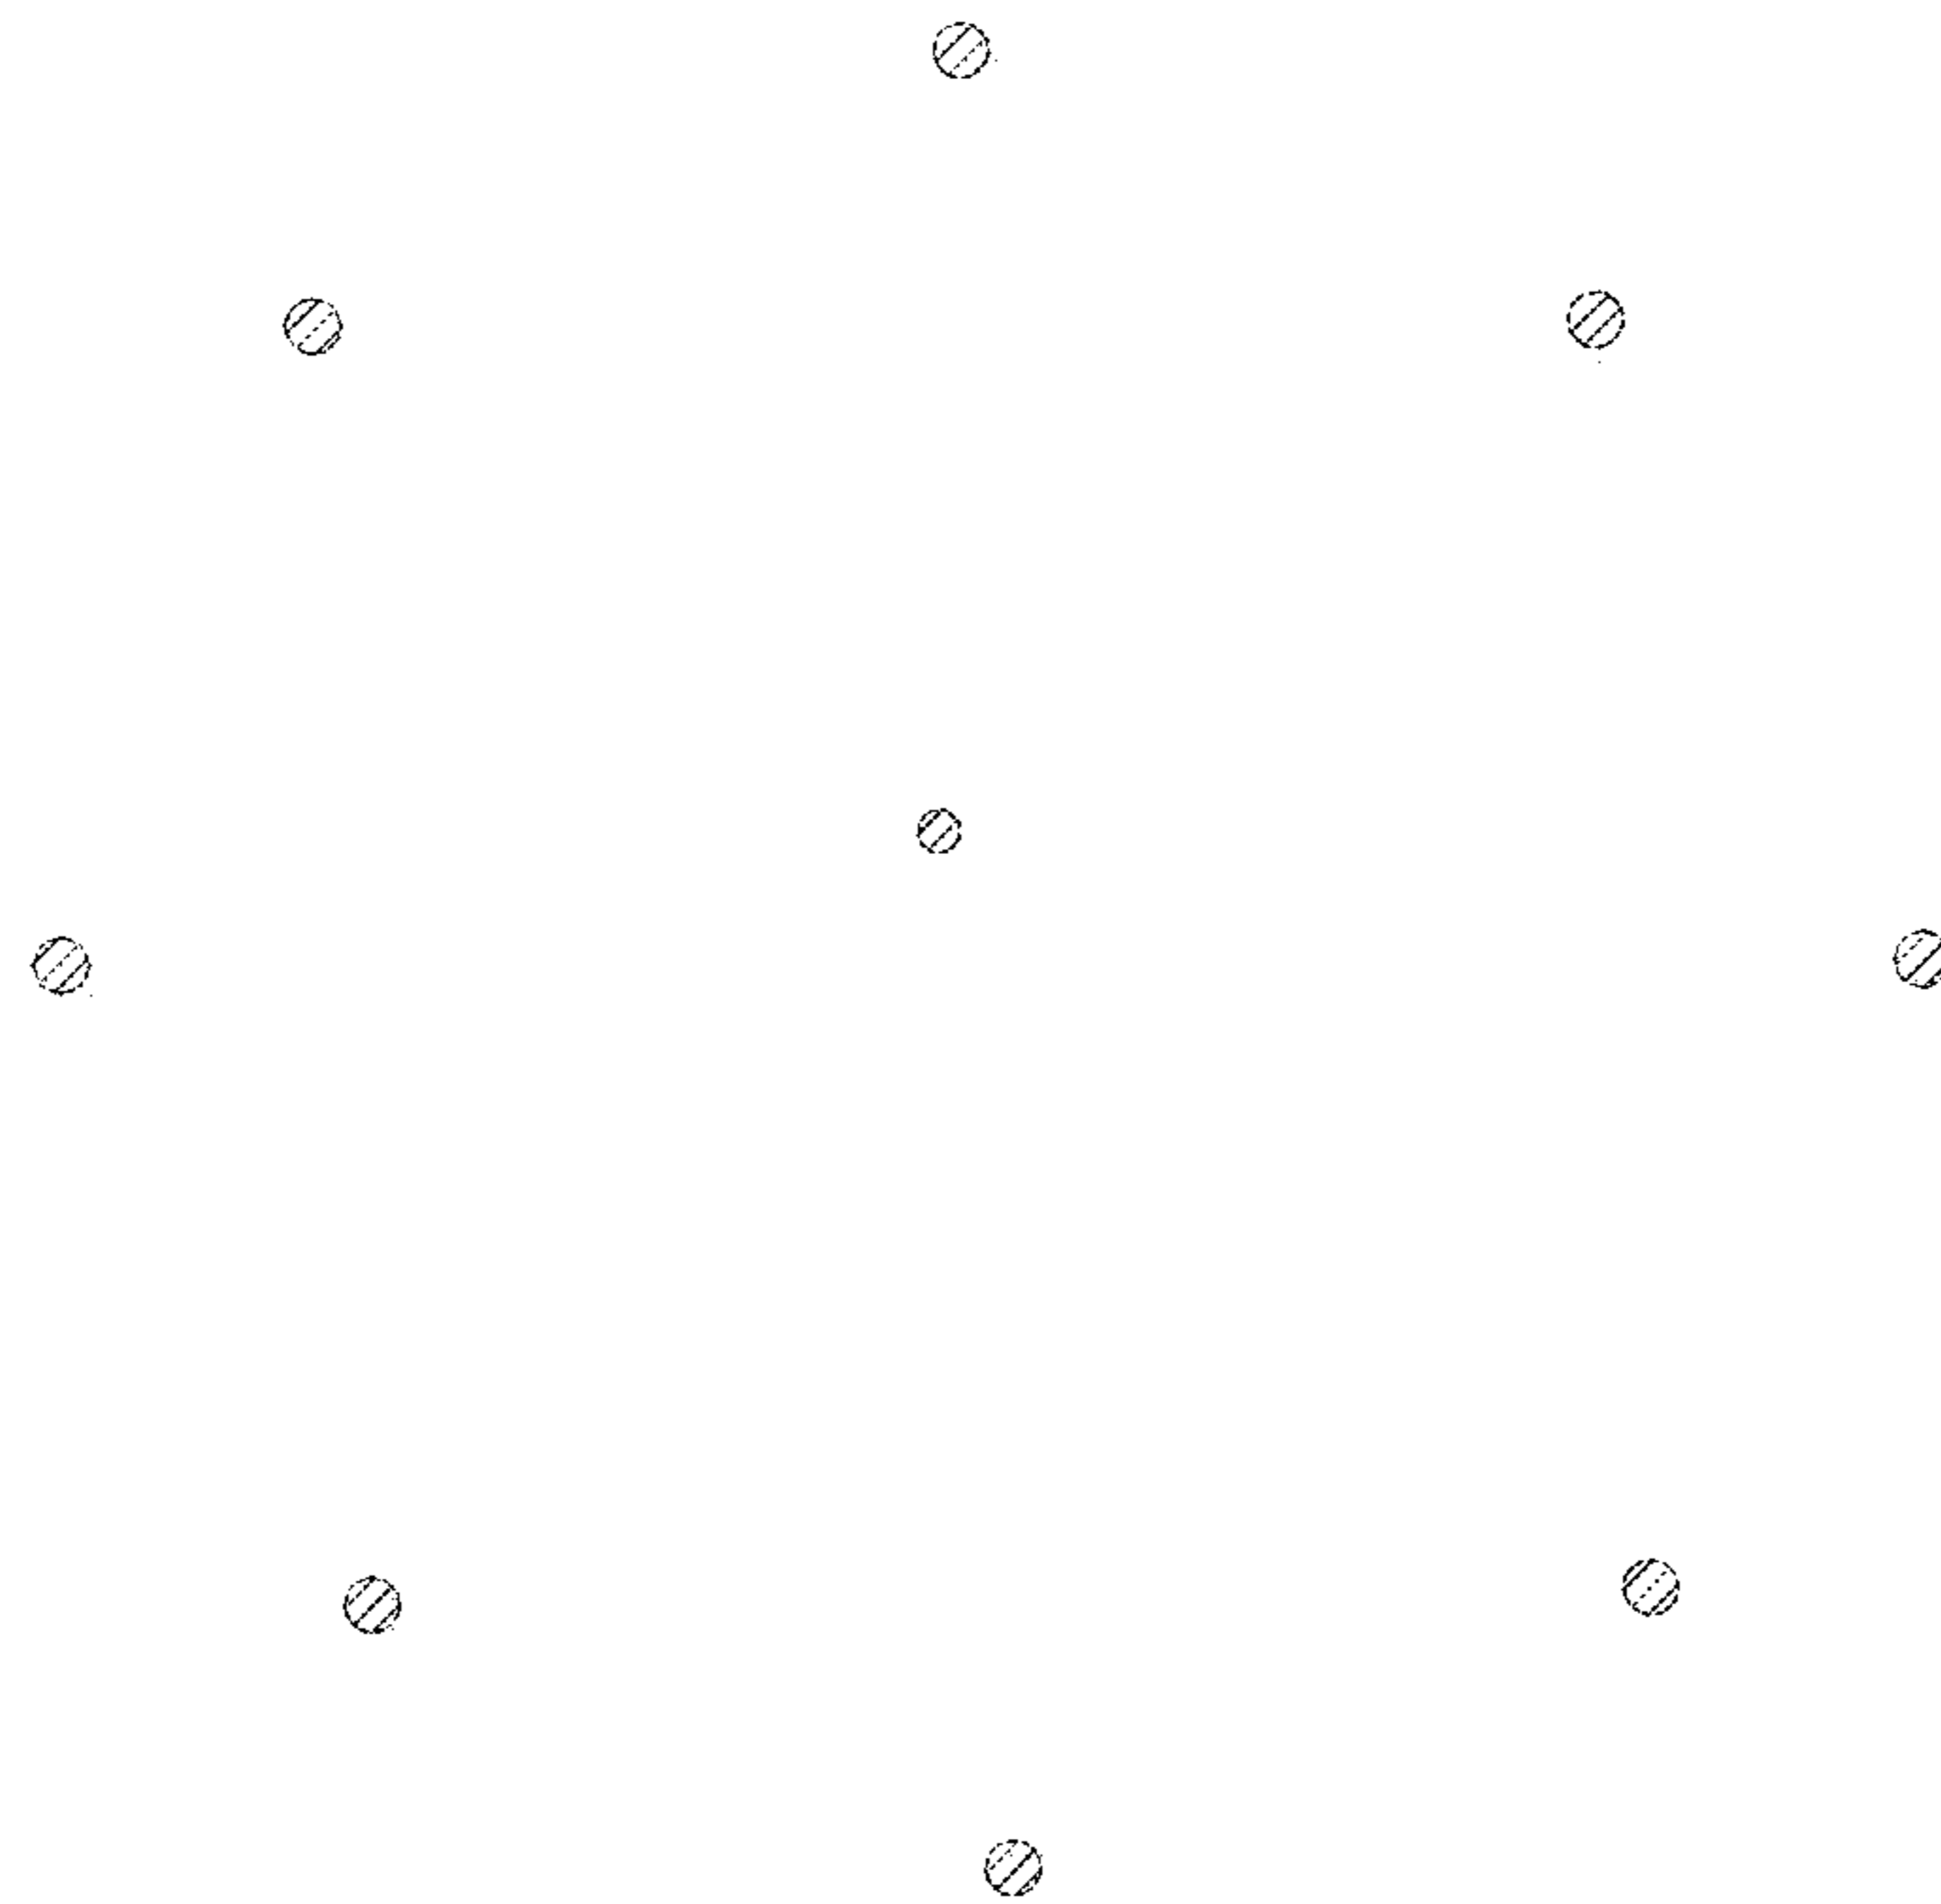


FIG. 42


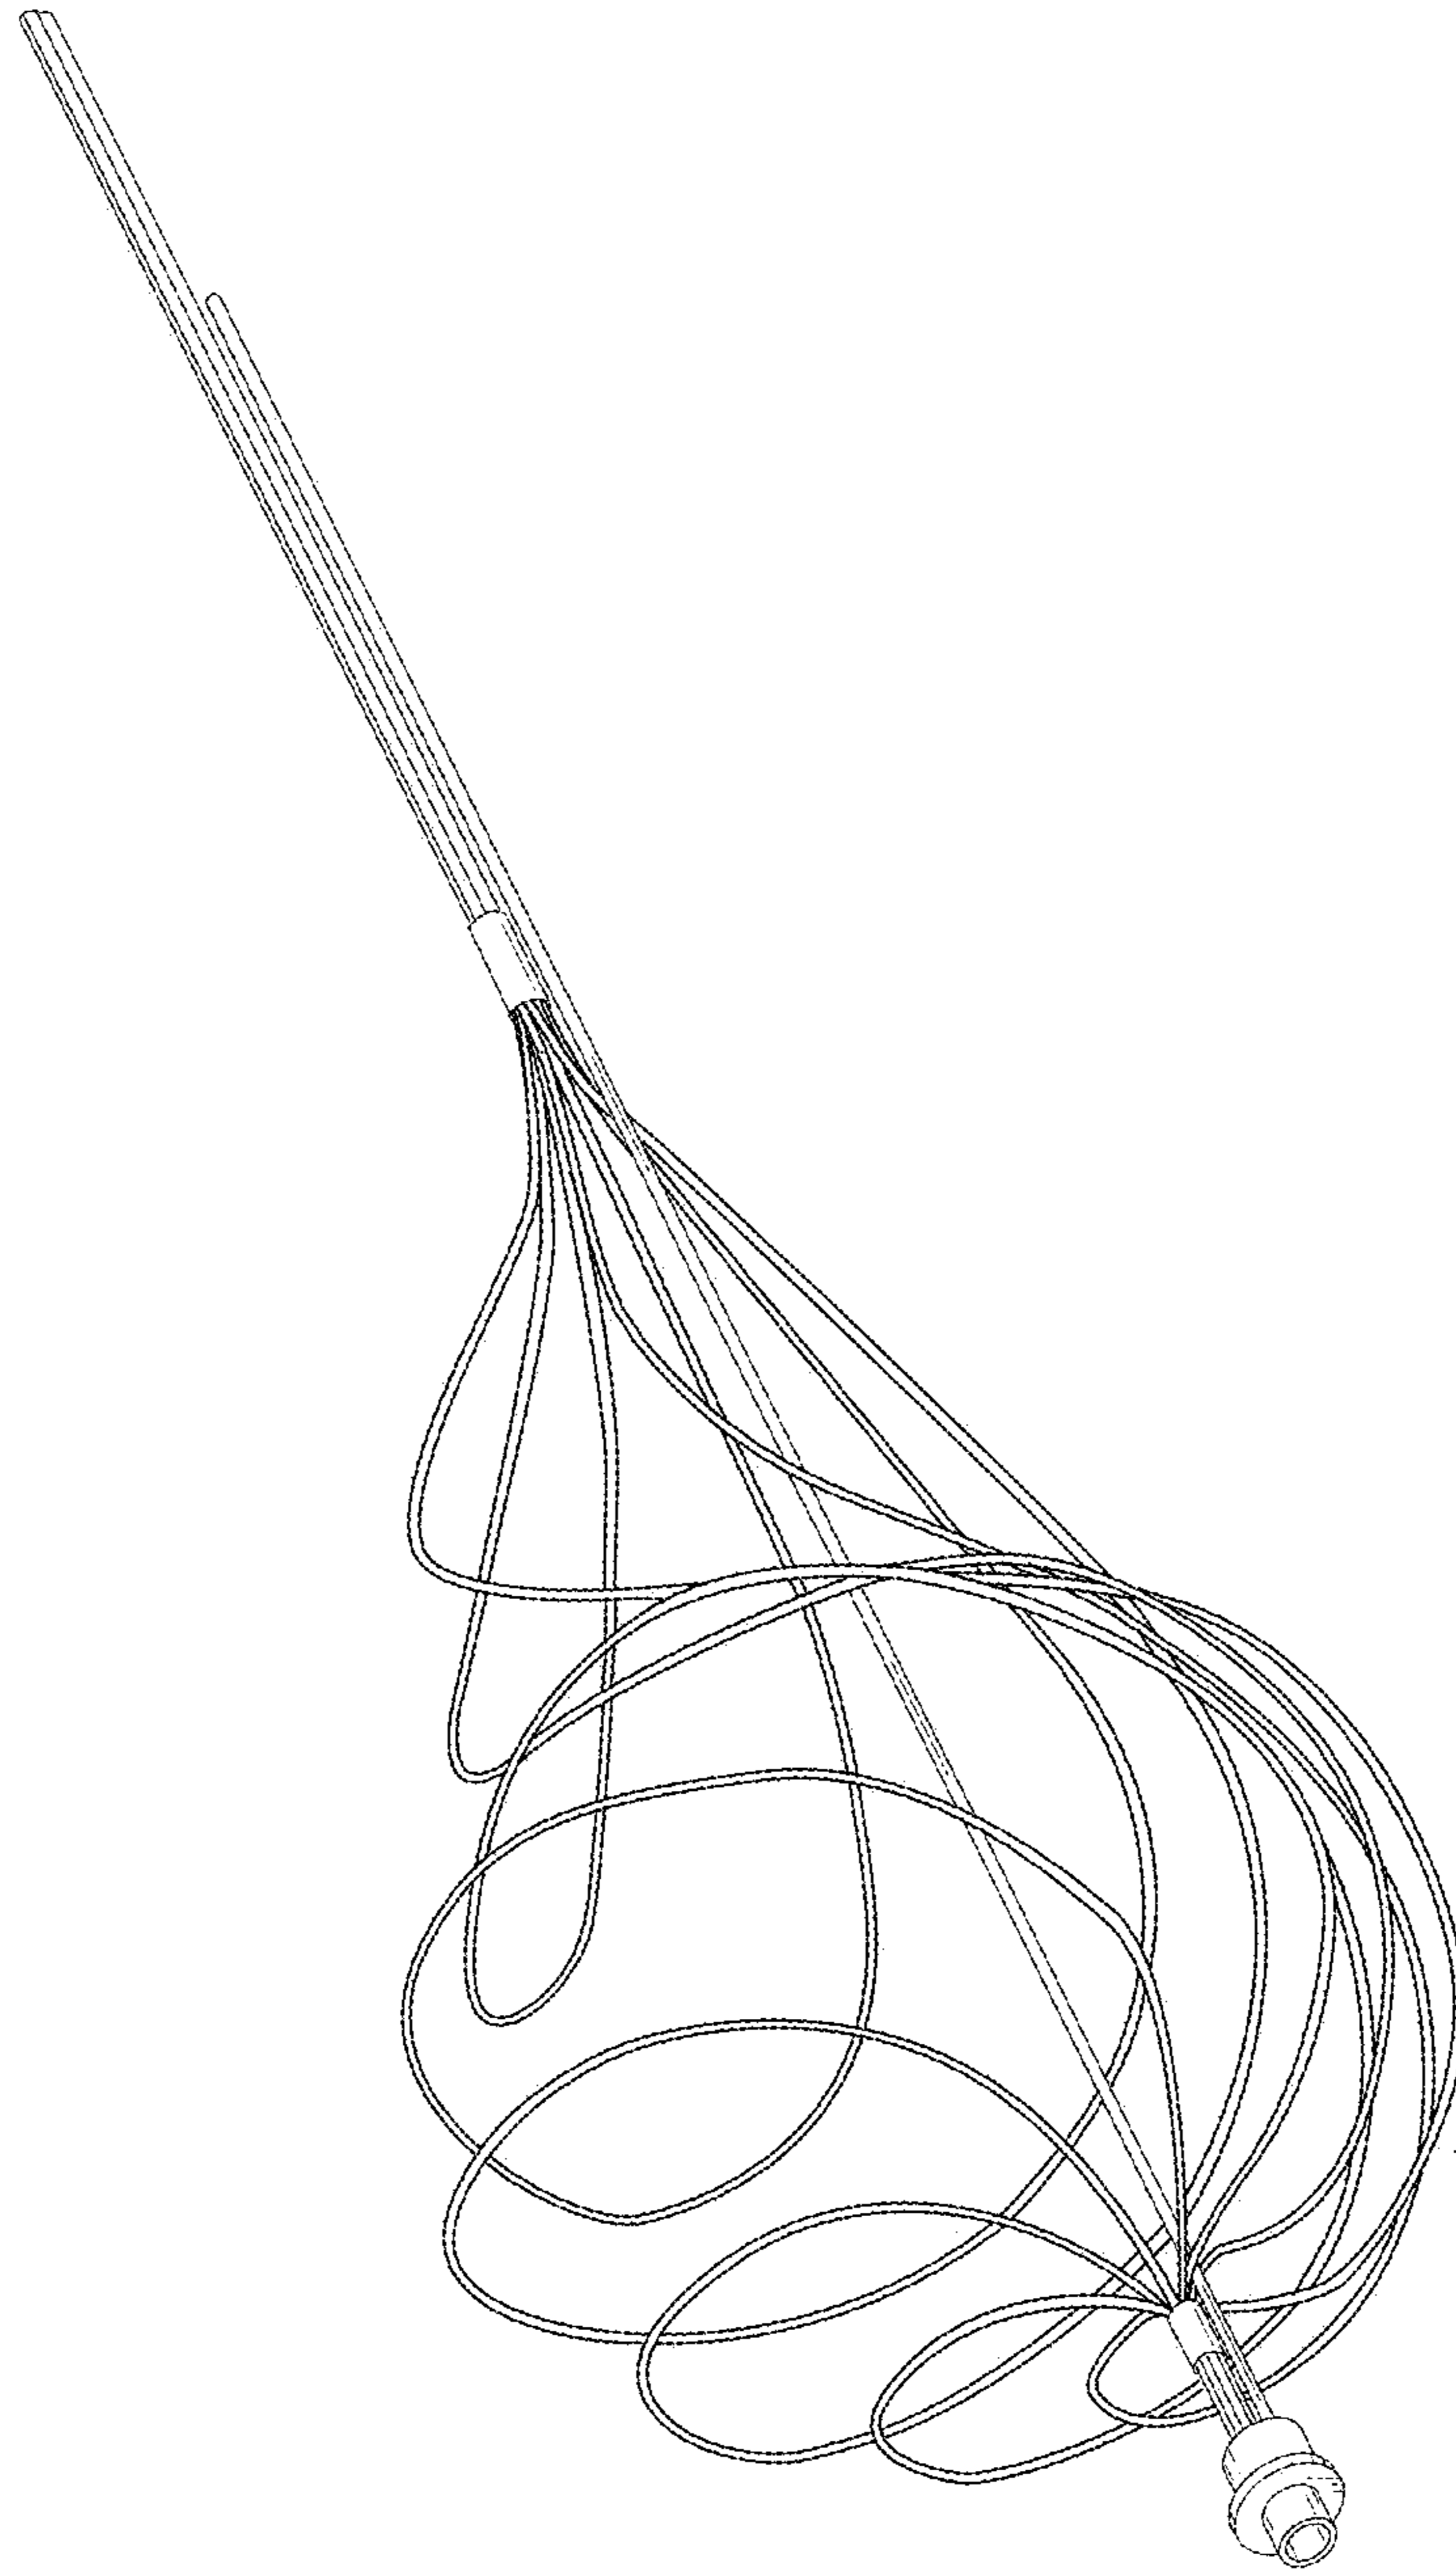


FIG. 43

49

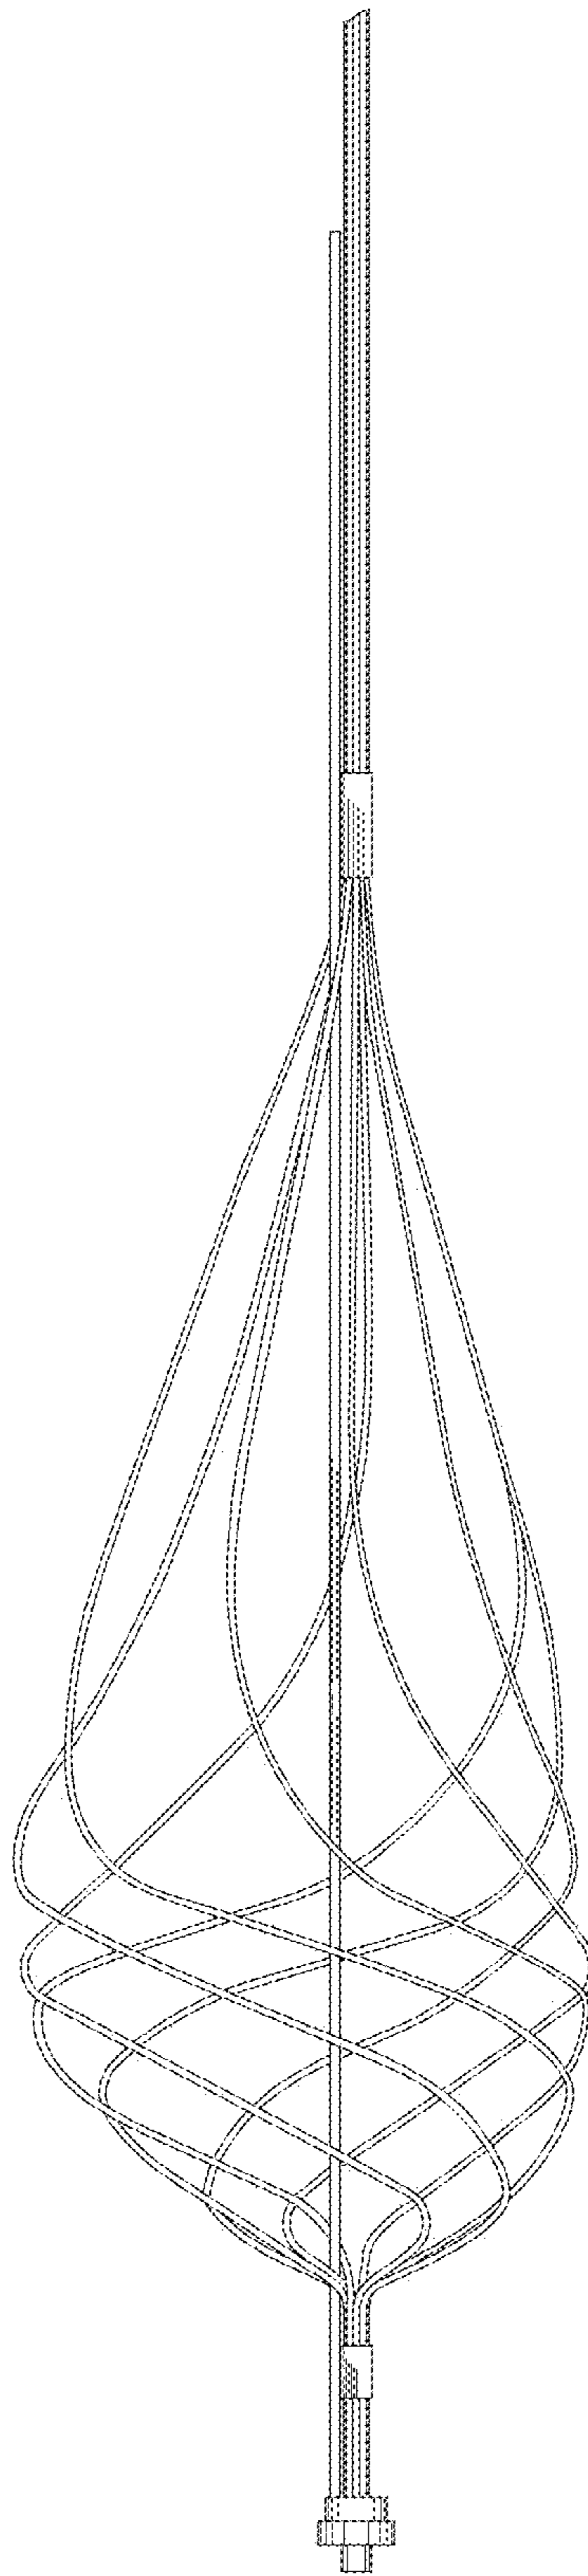

49

FIG. 44

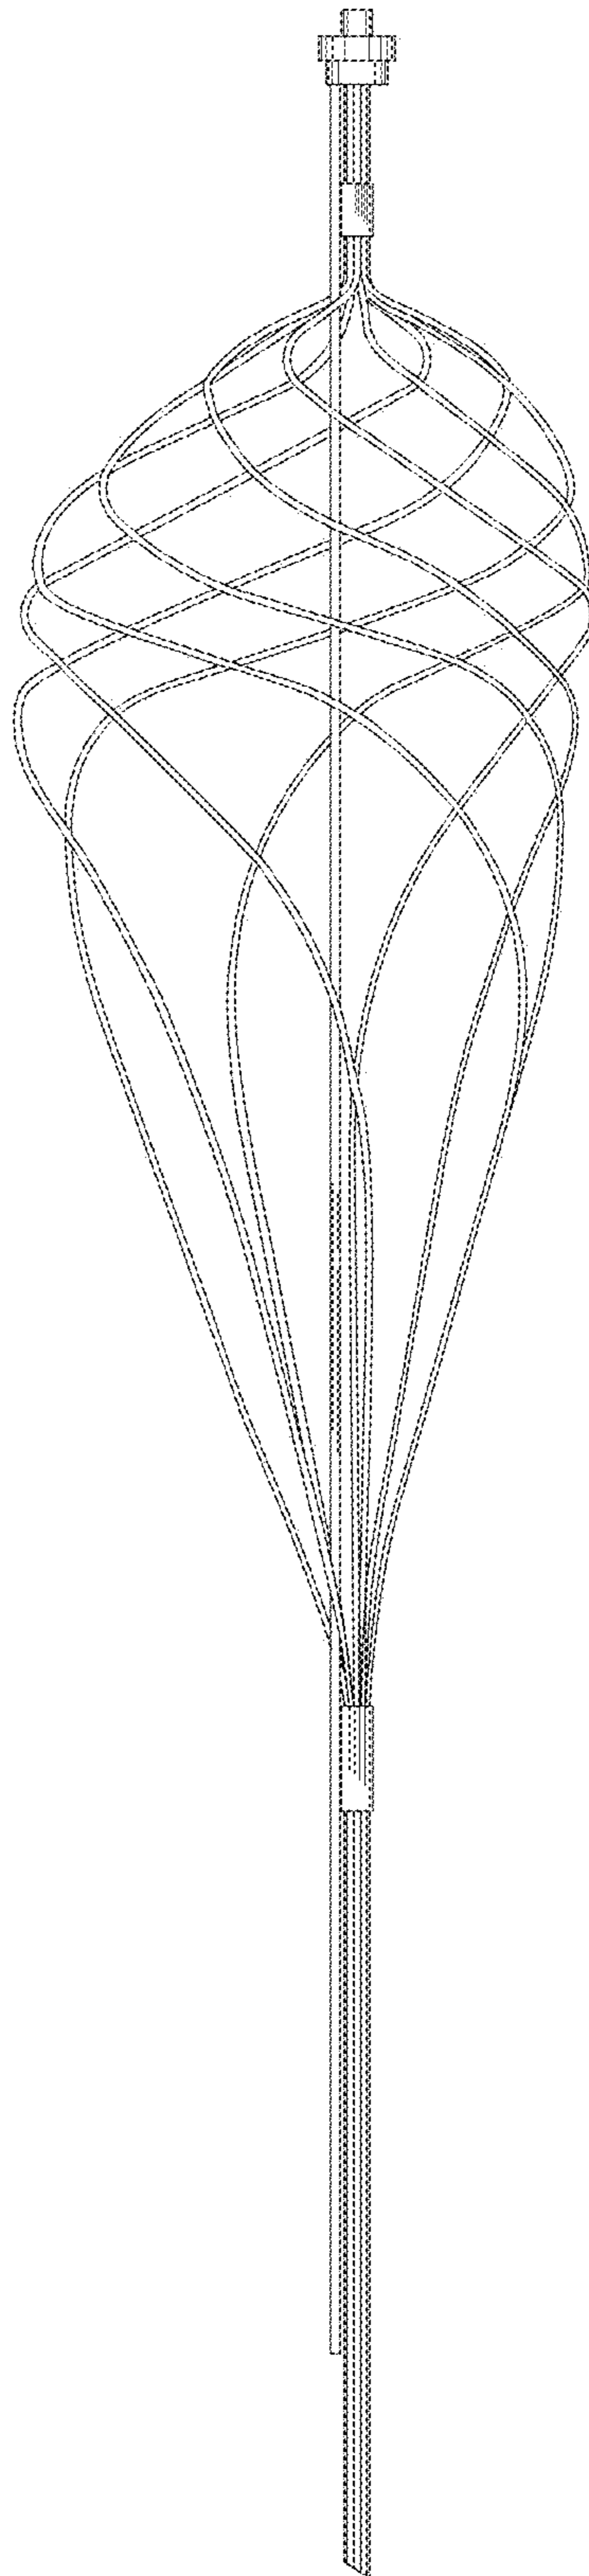


FIG. 45

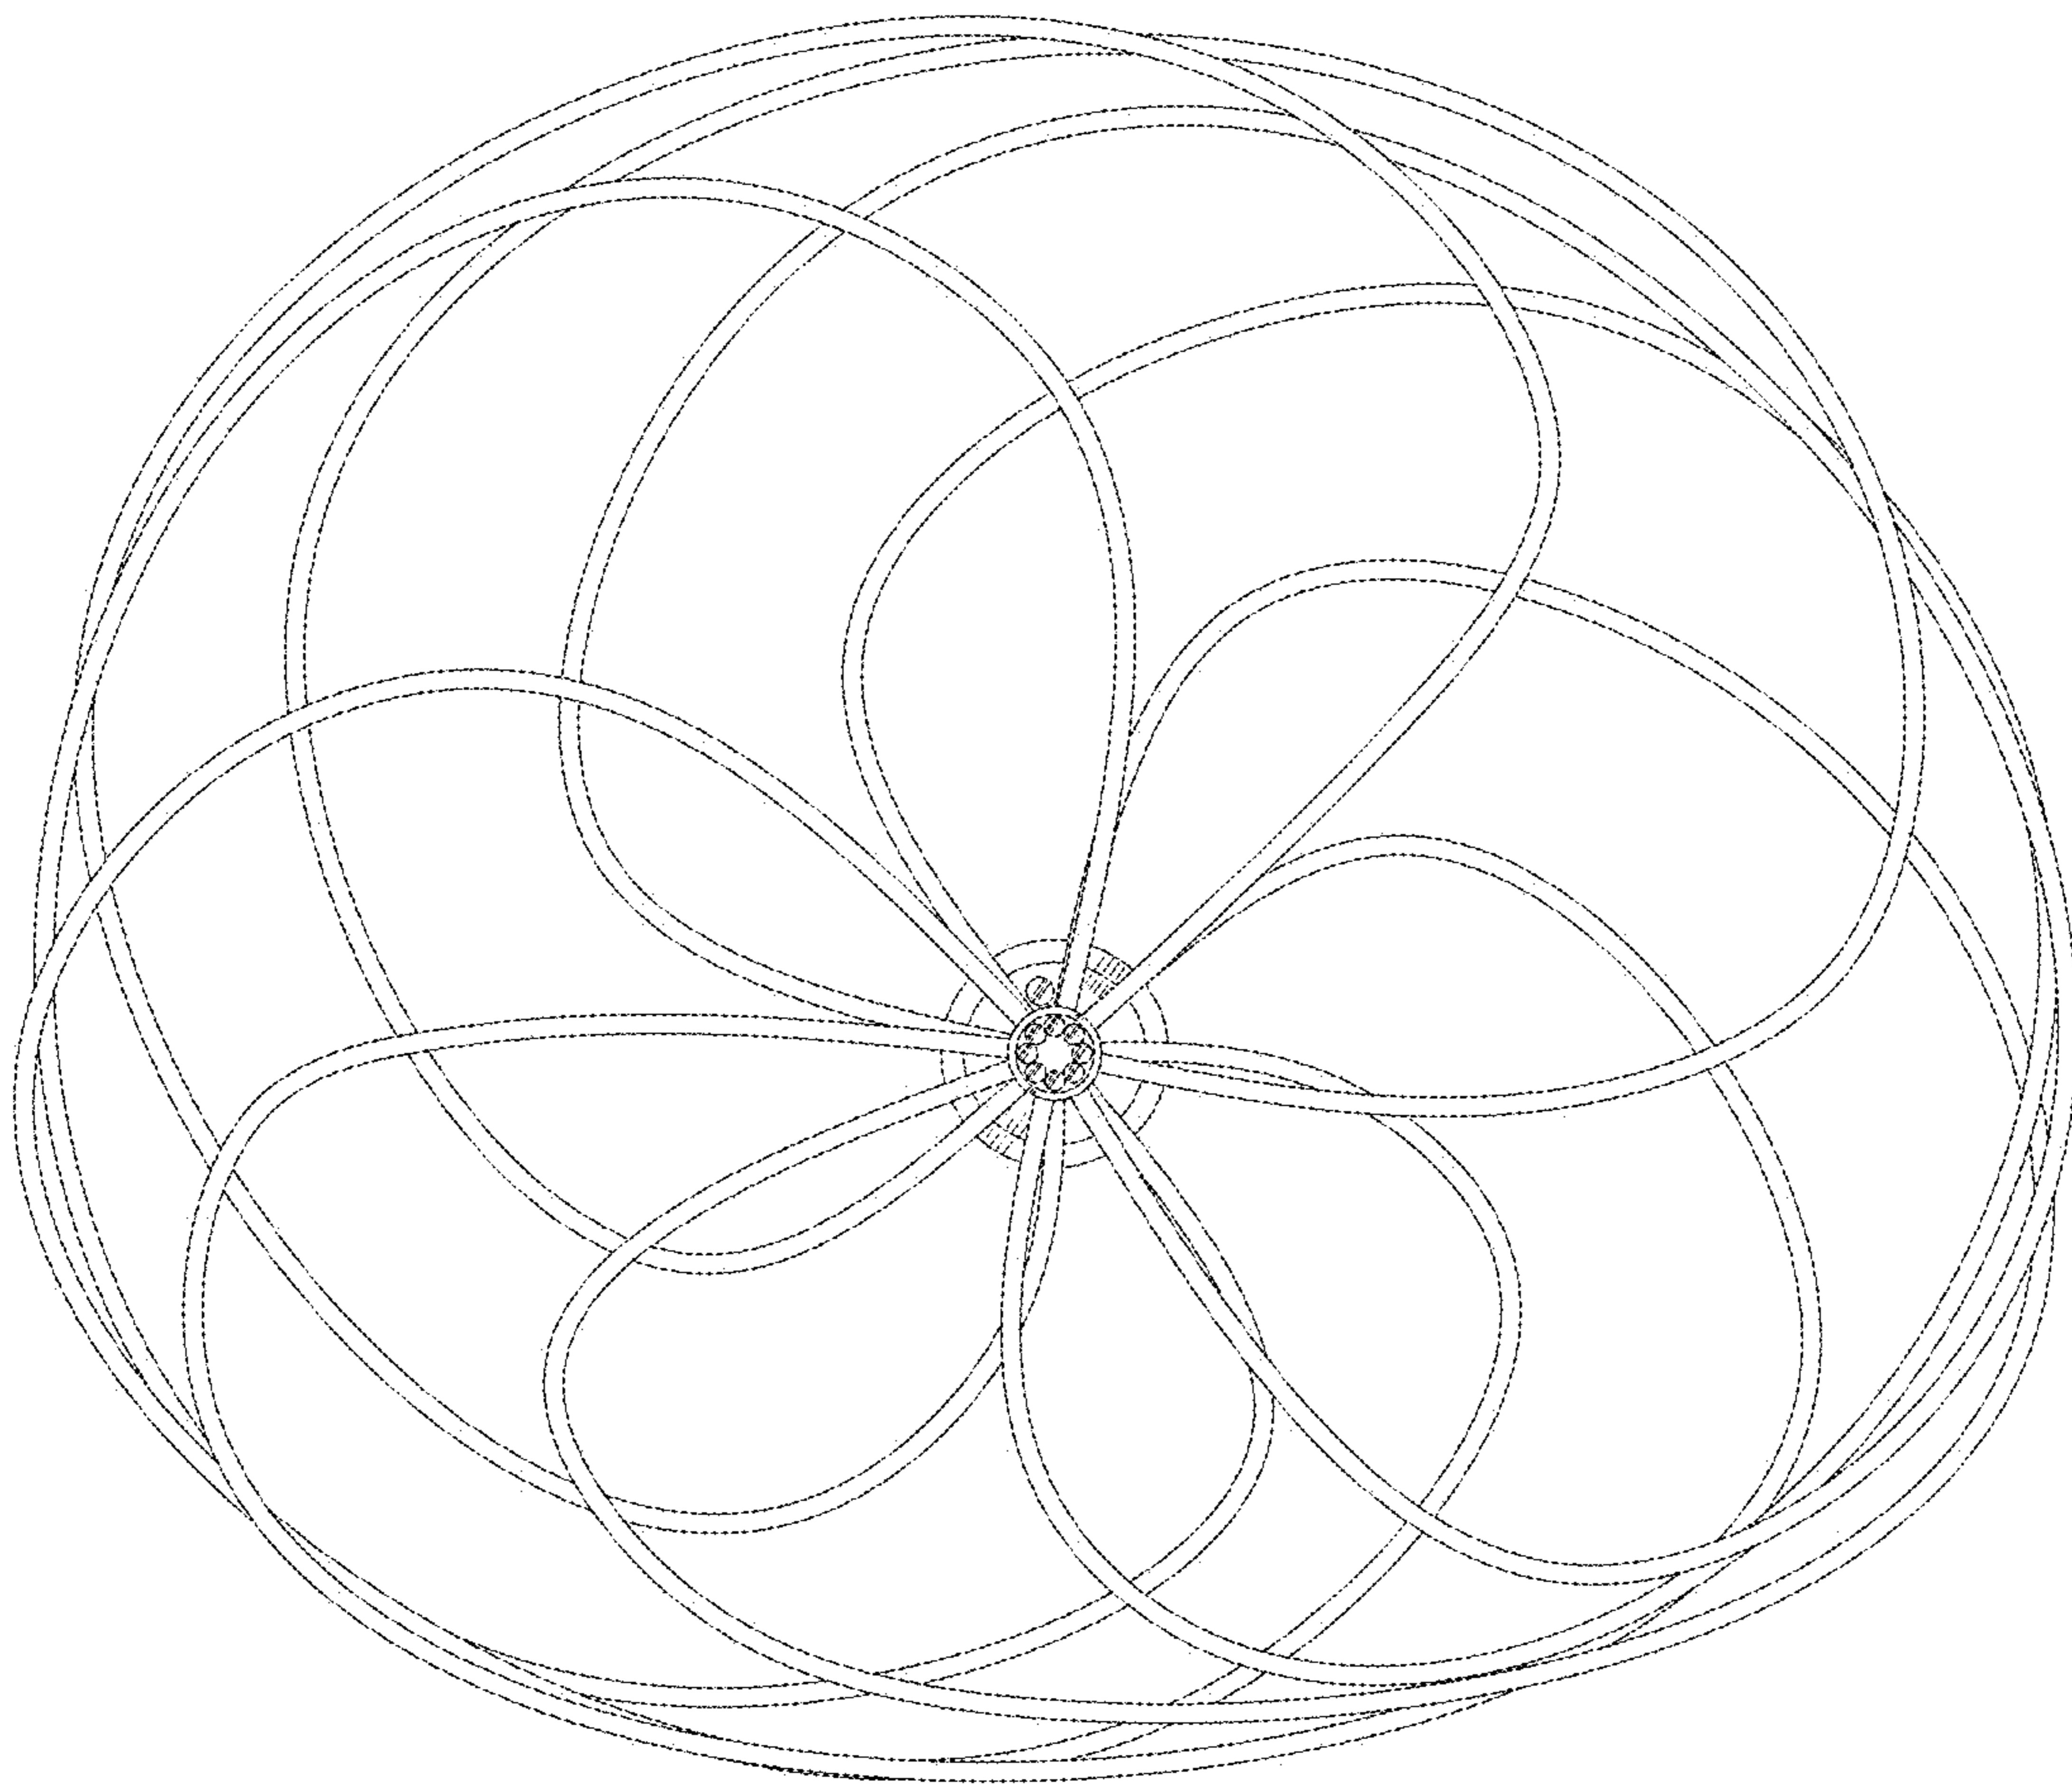


FIG. 46

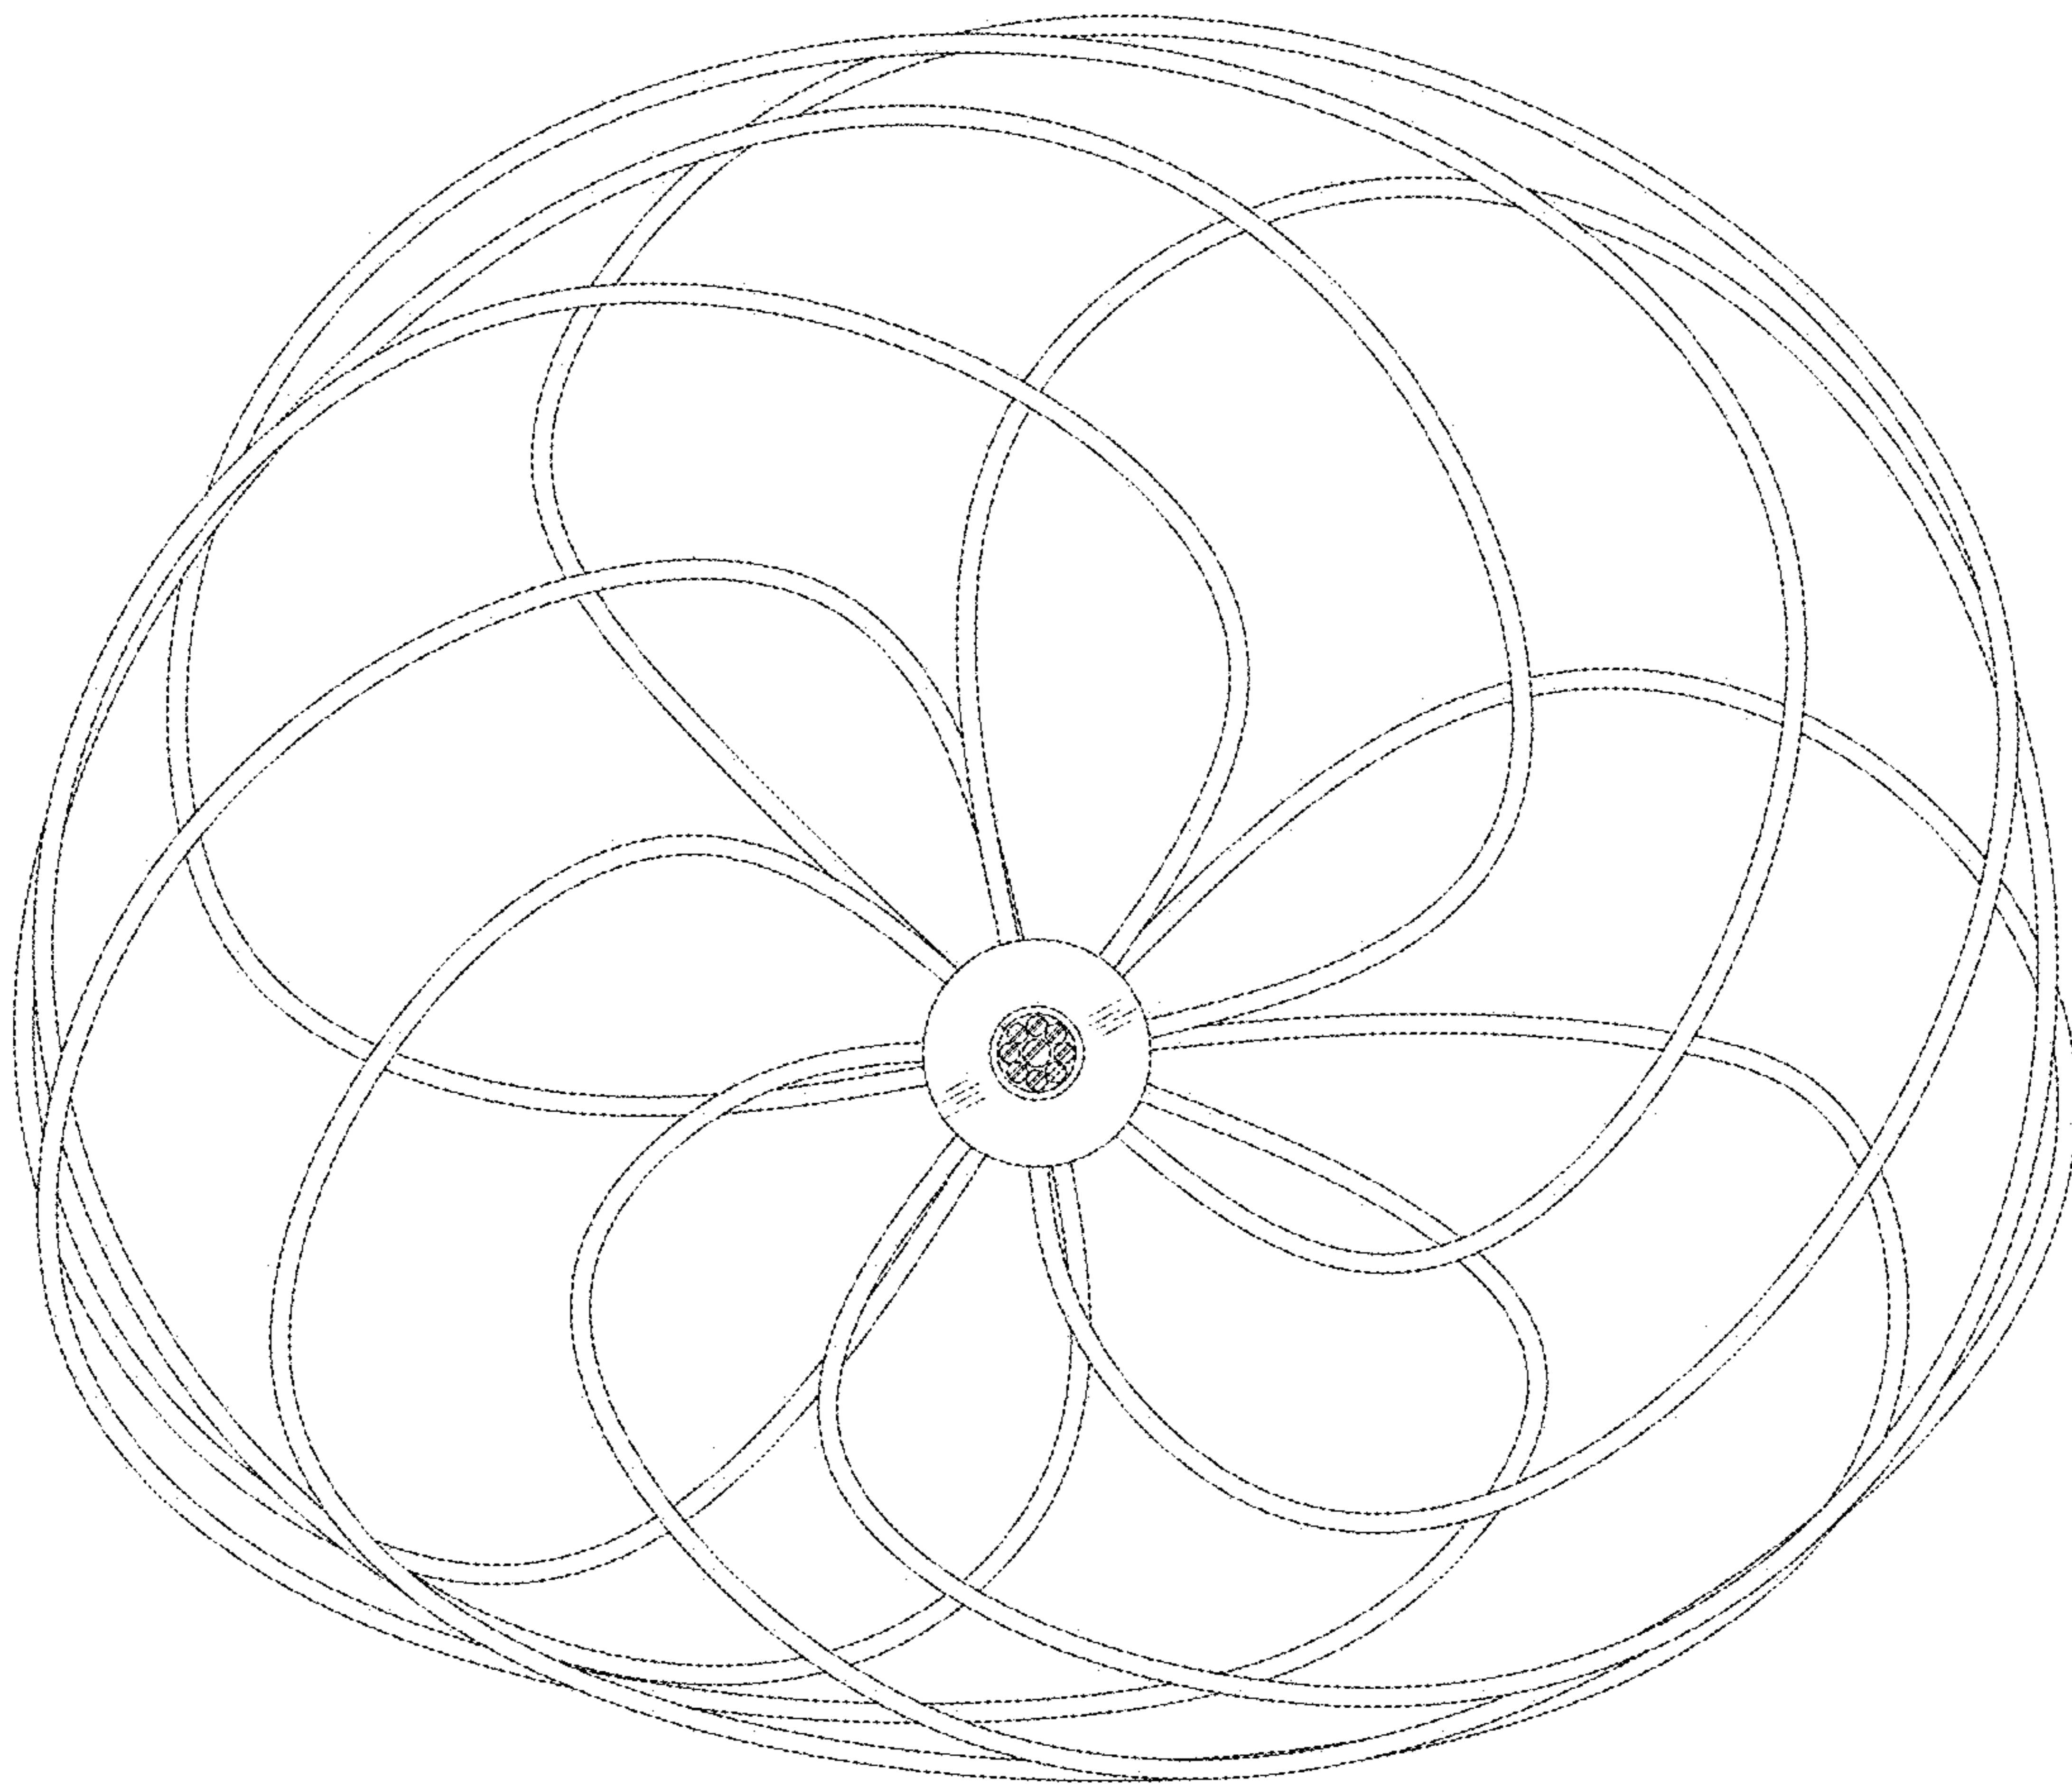


FIG. 47

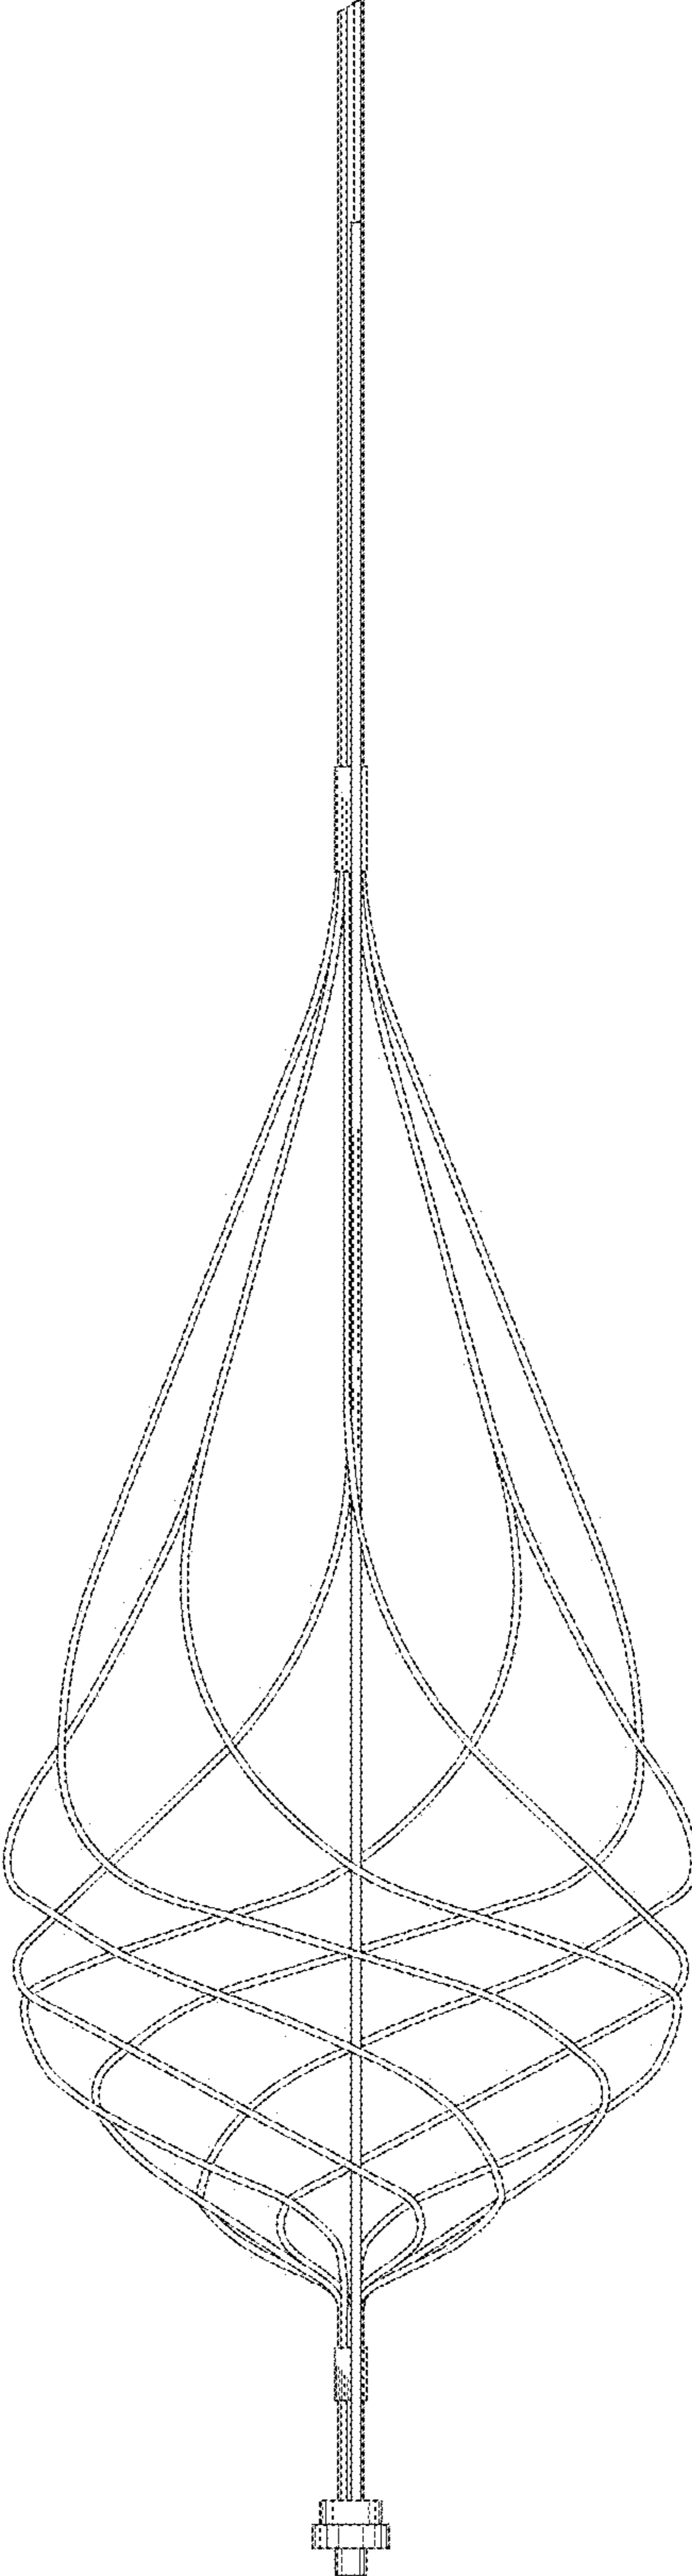


FIG. 48

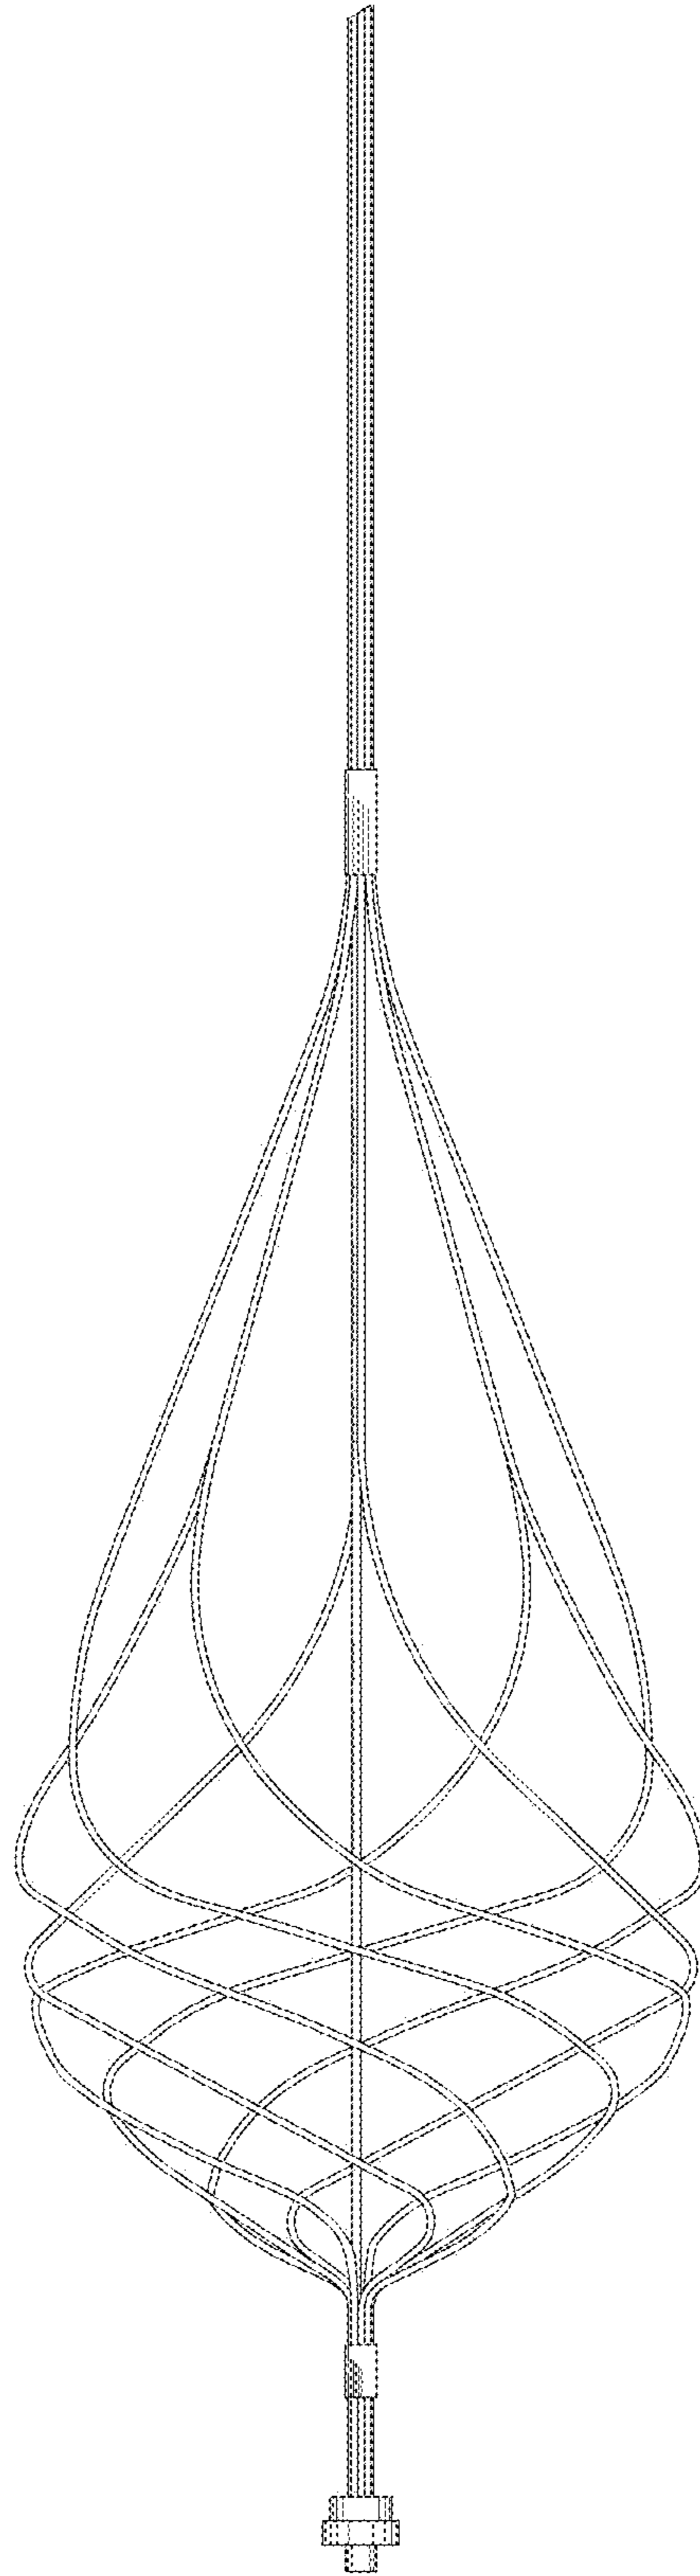


FIG. 49




FIG. 50

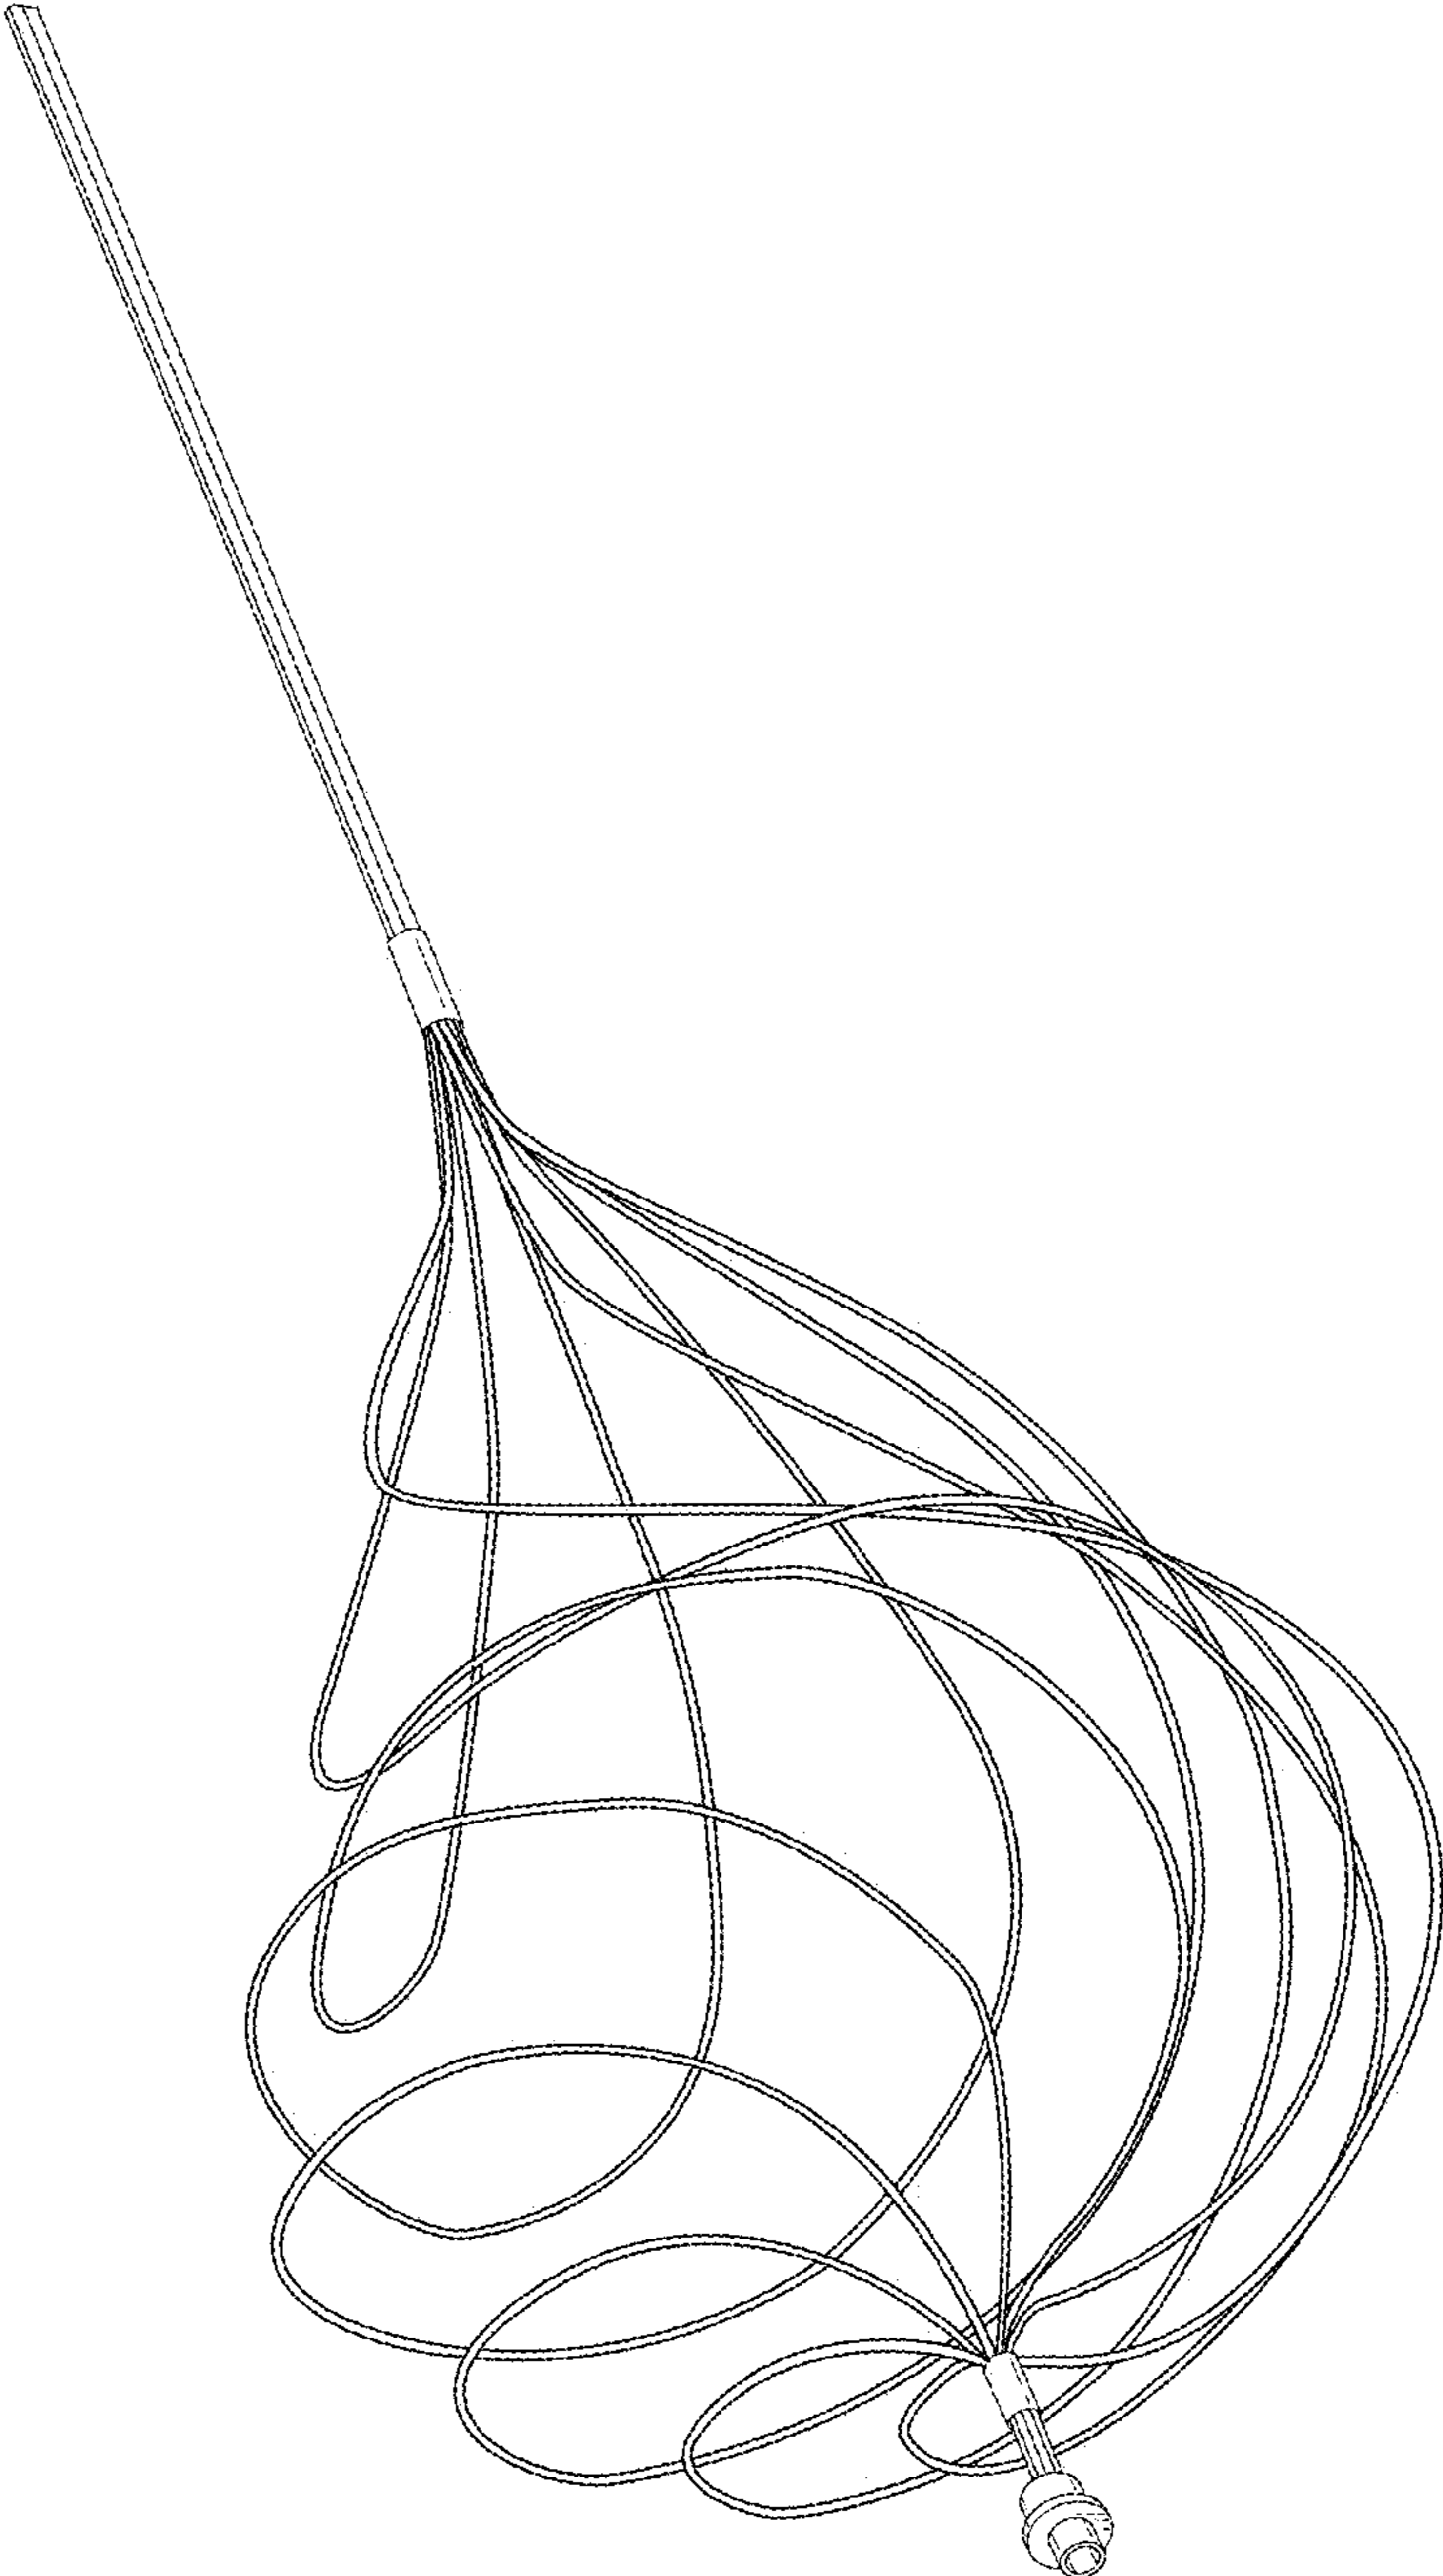


FIG. 51

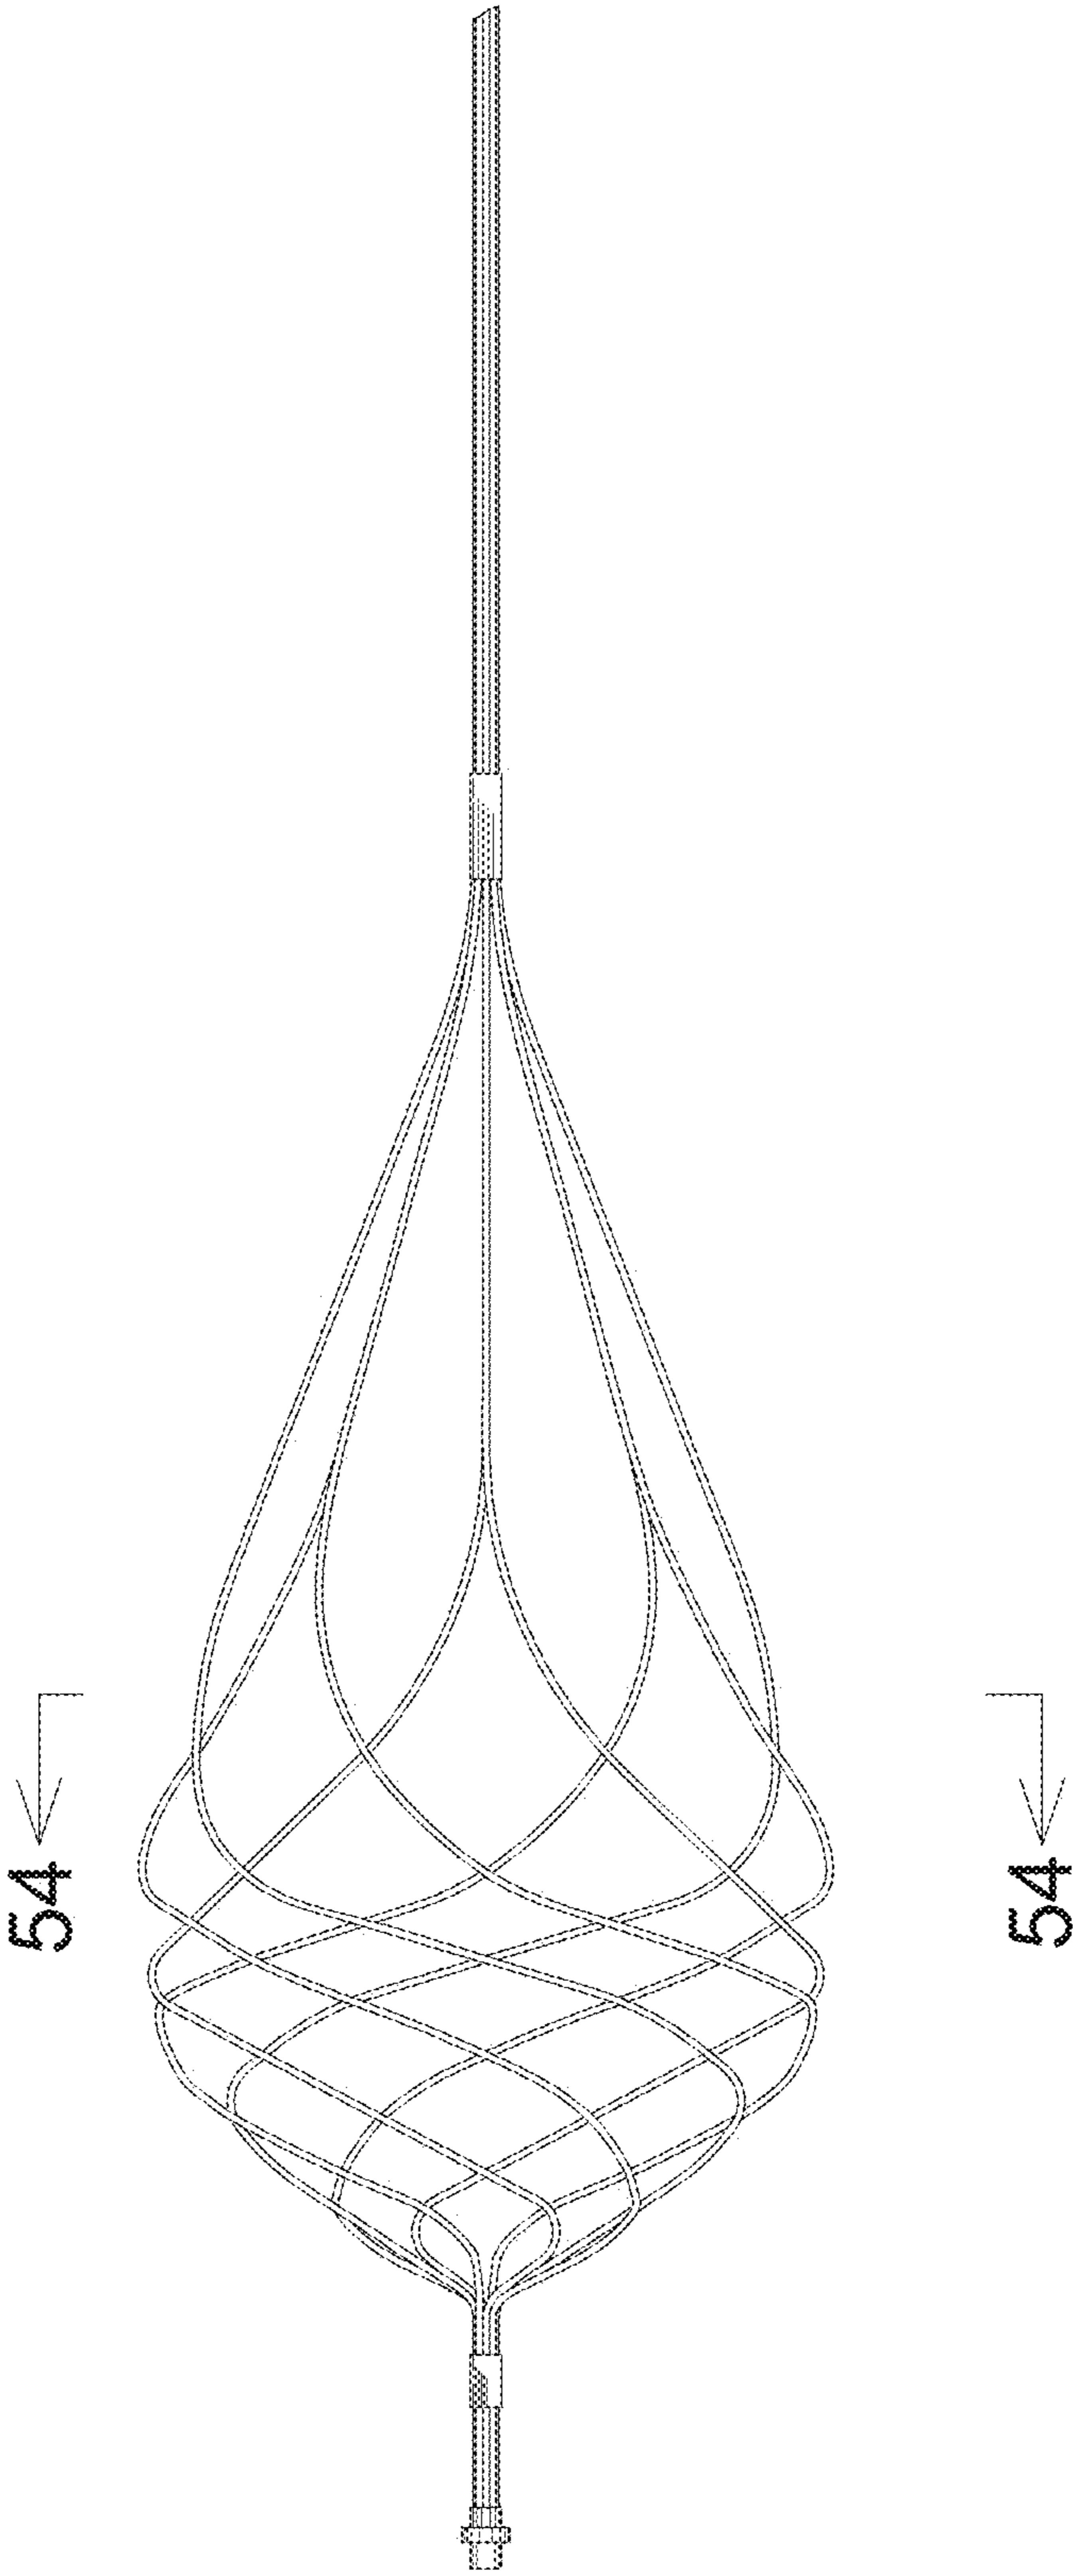


FIG. 52

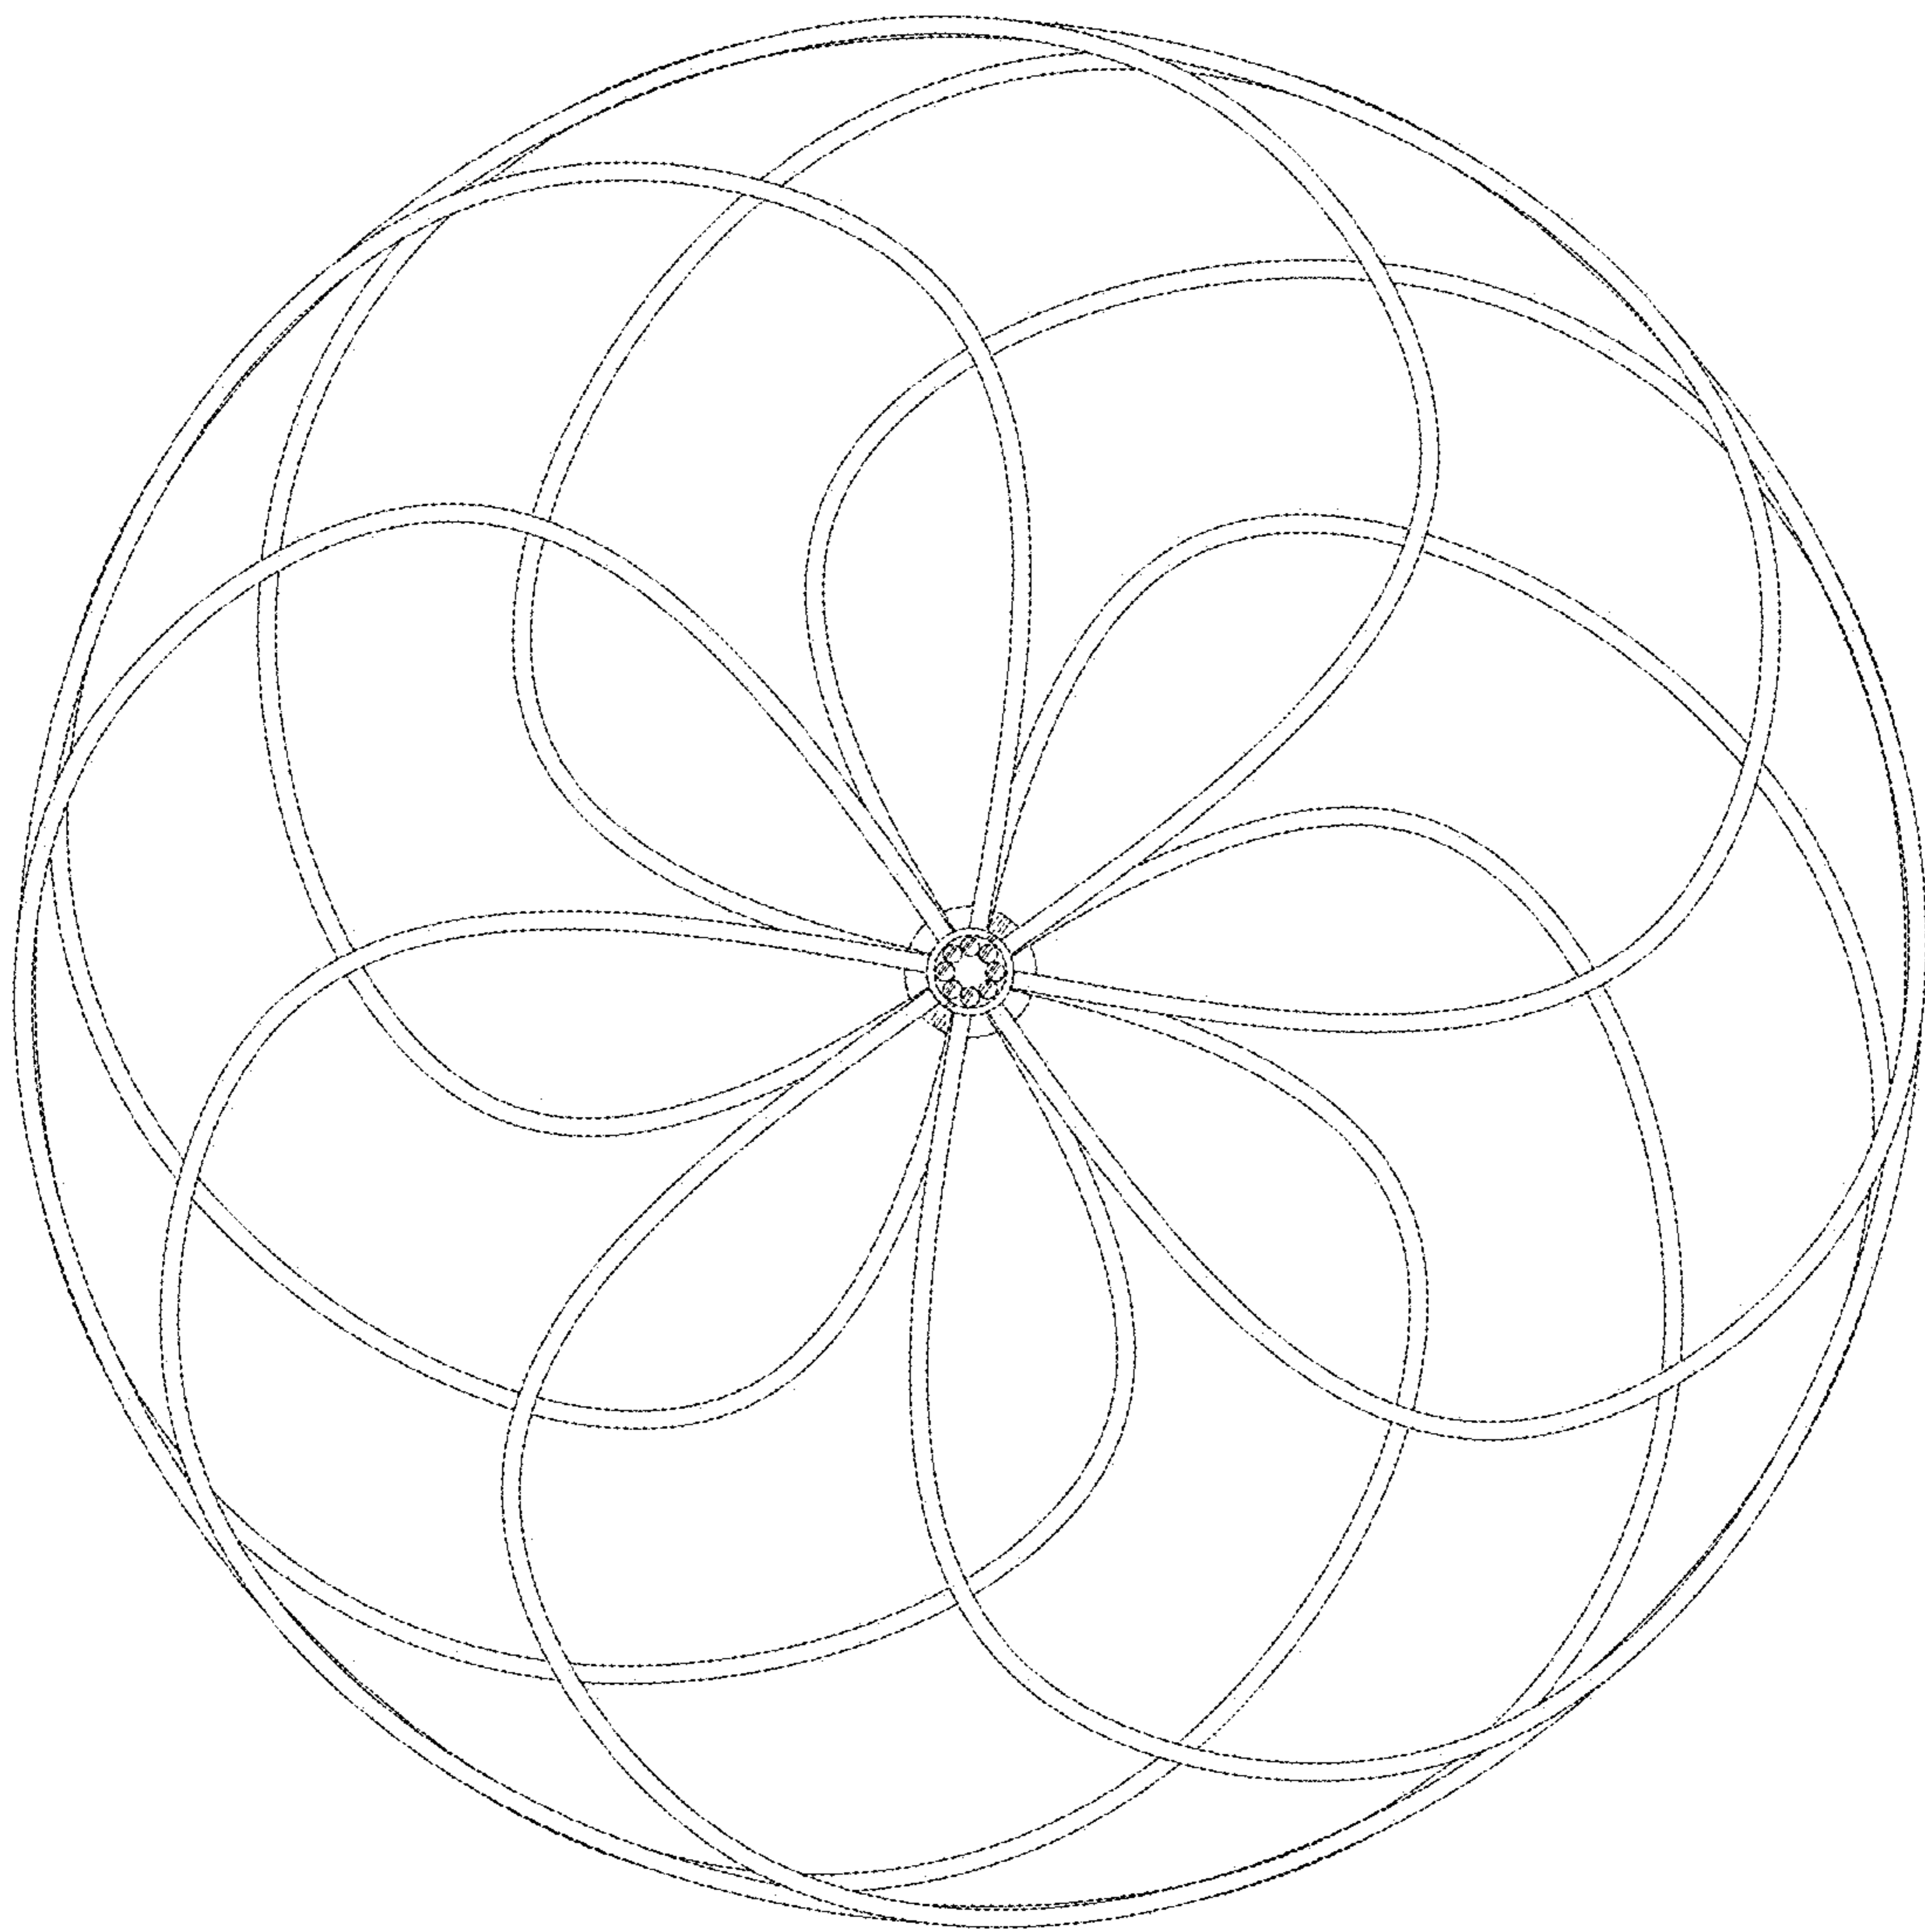


FIG. 53

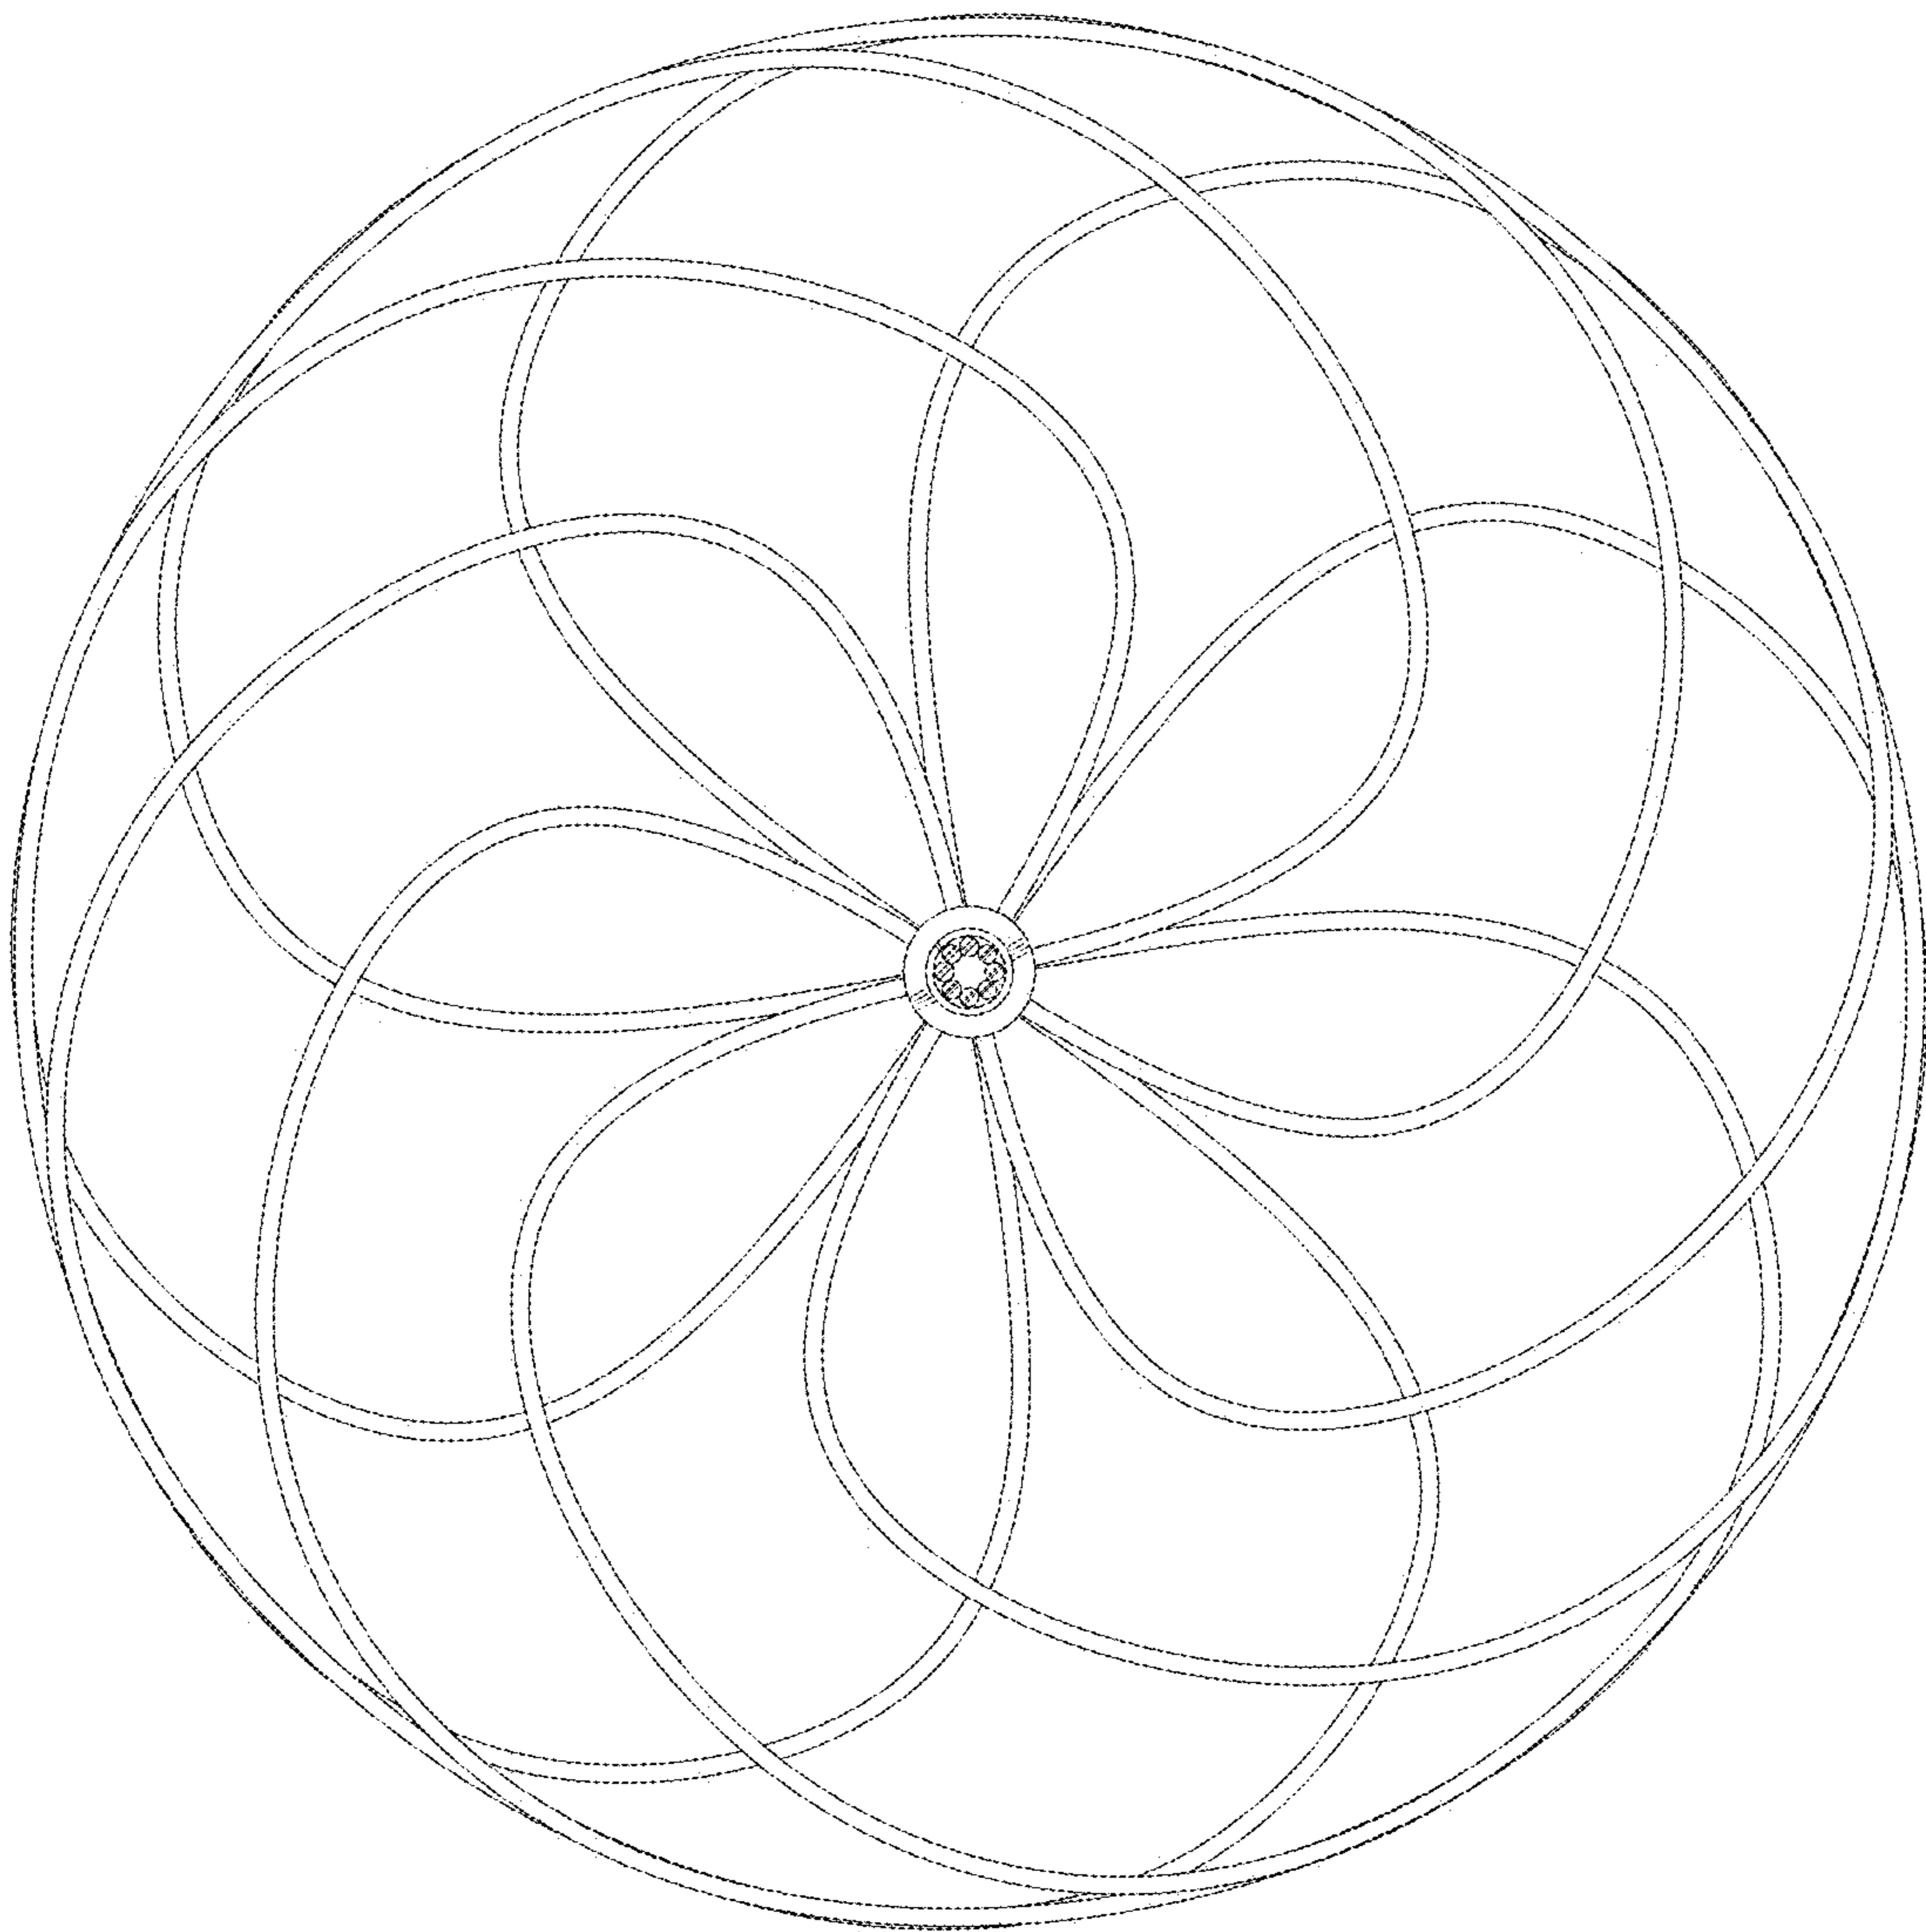


FIG. 54



FIG. 55


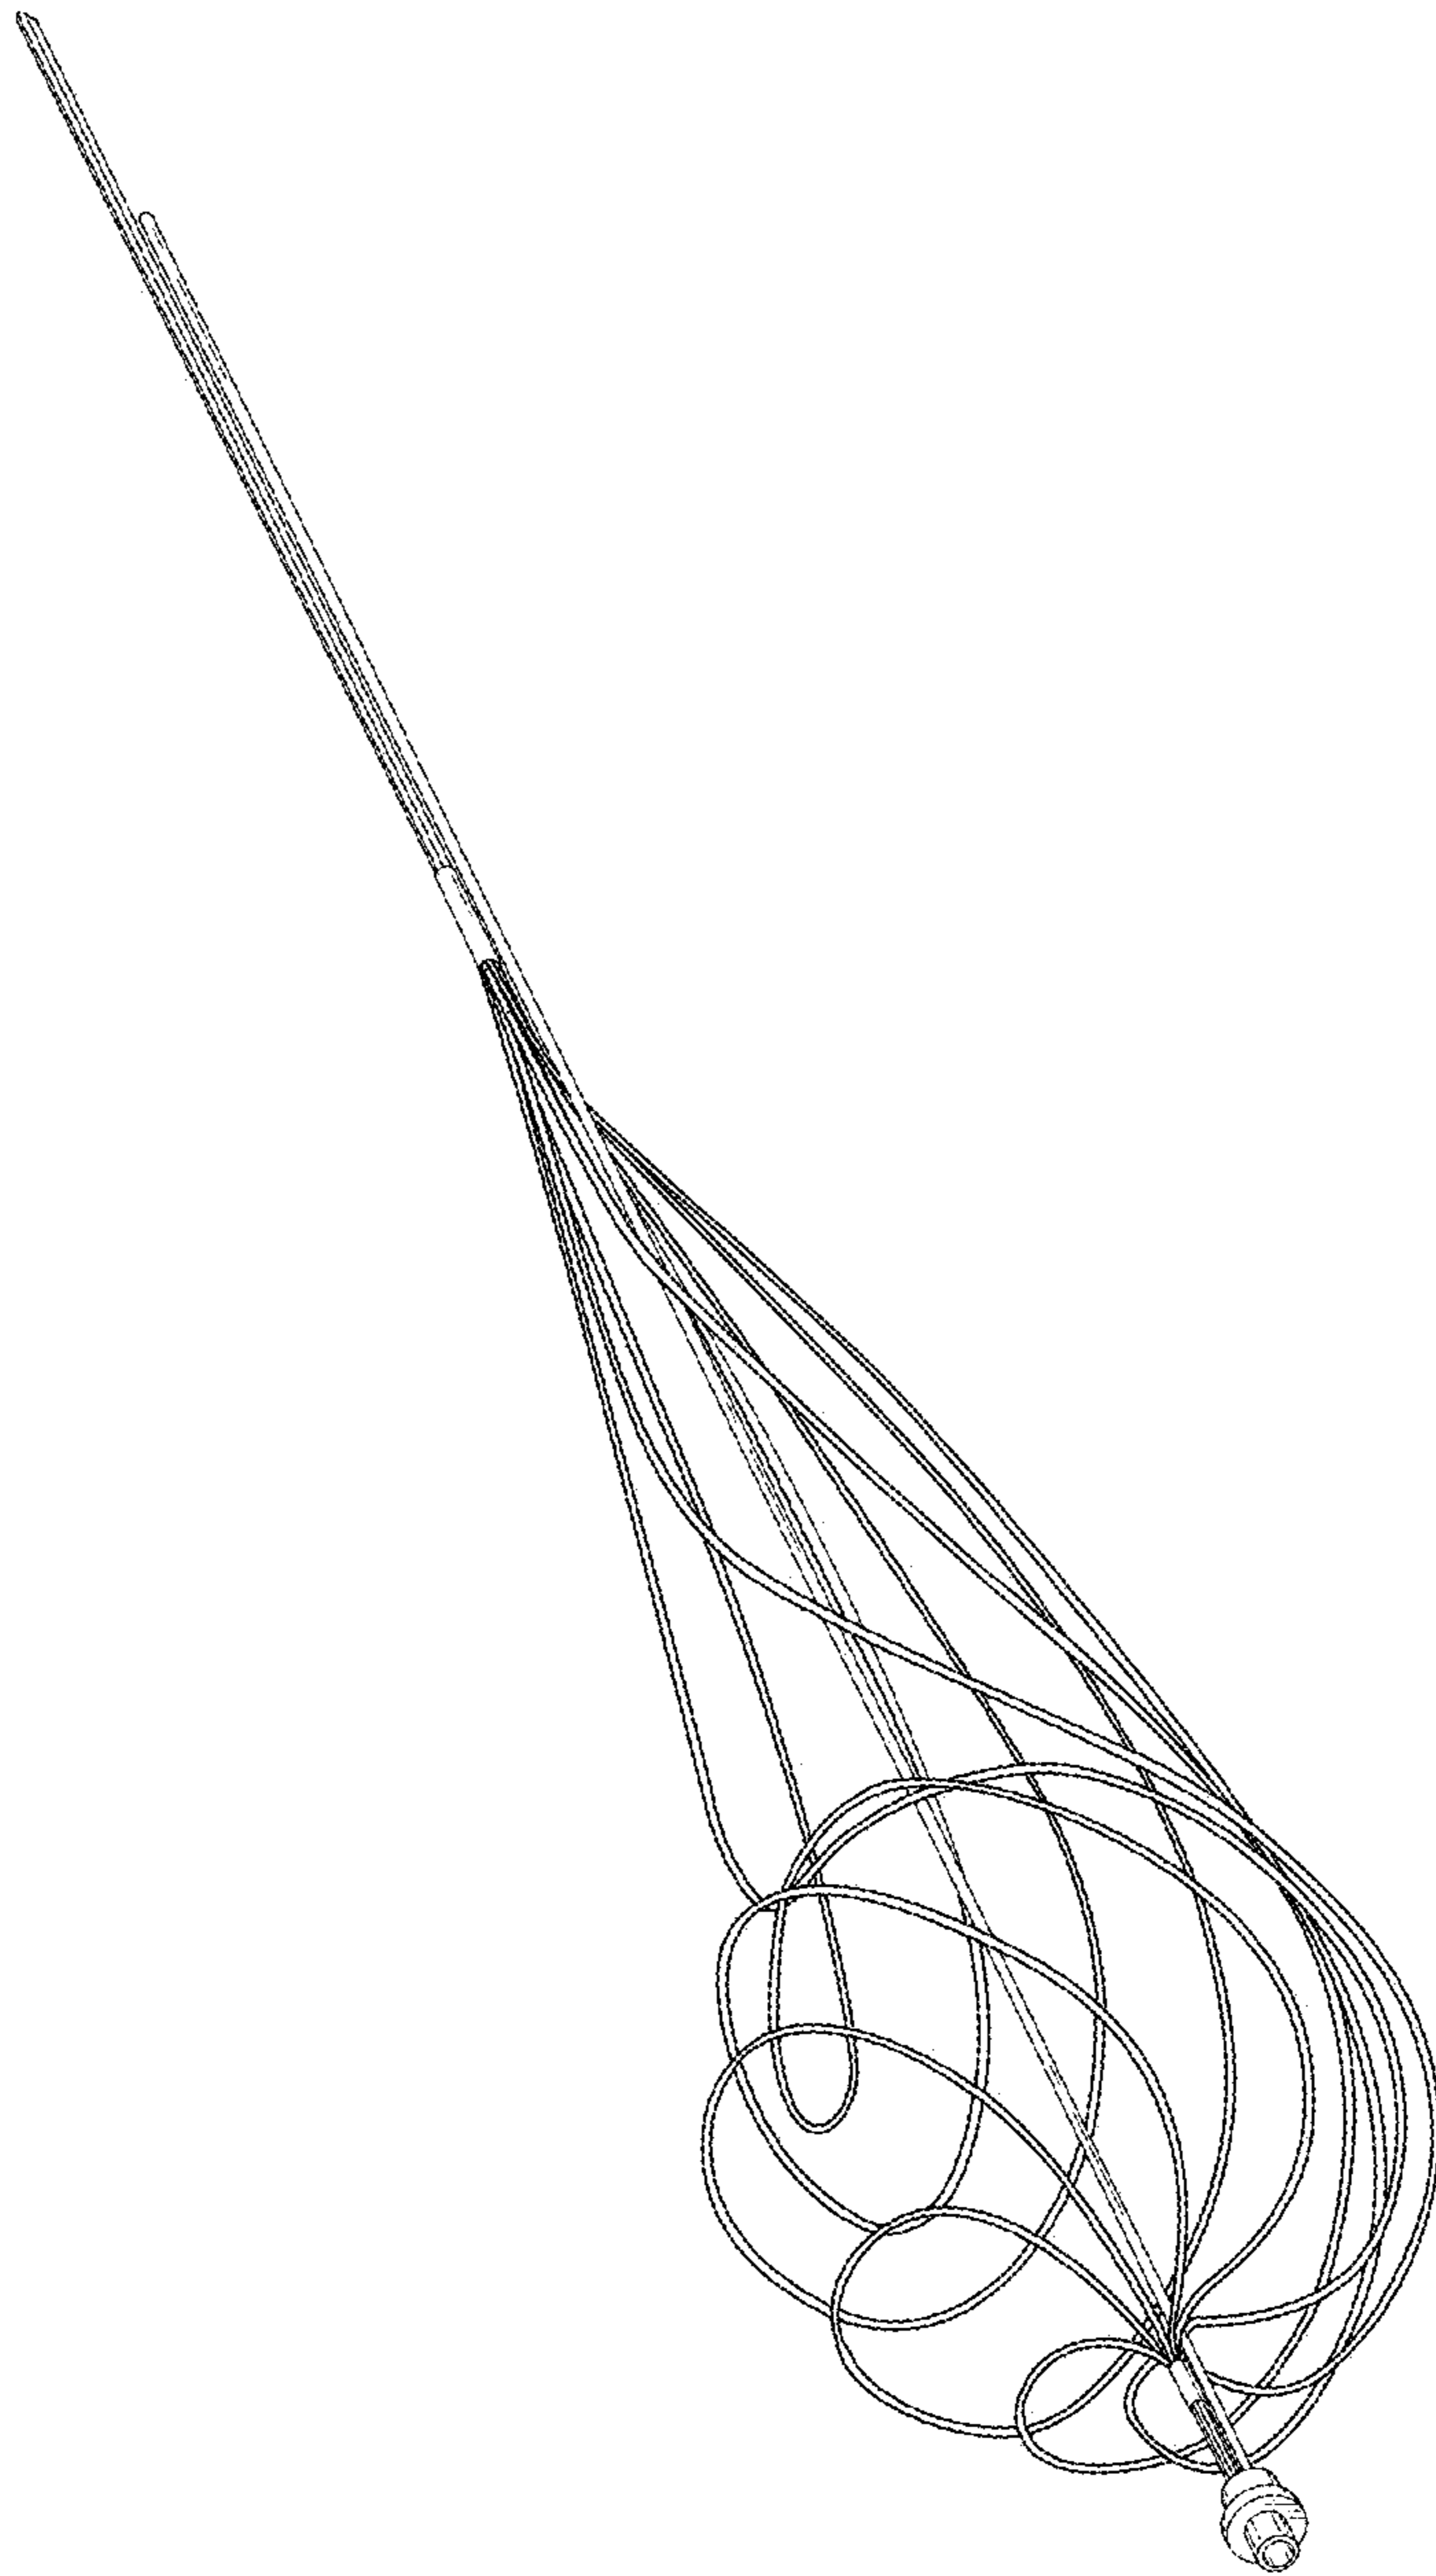


FIG. 56

62

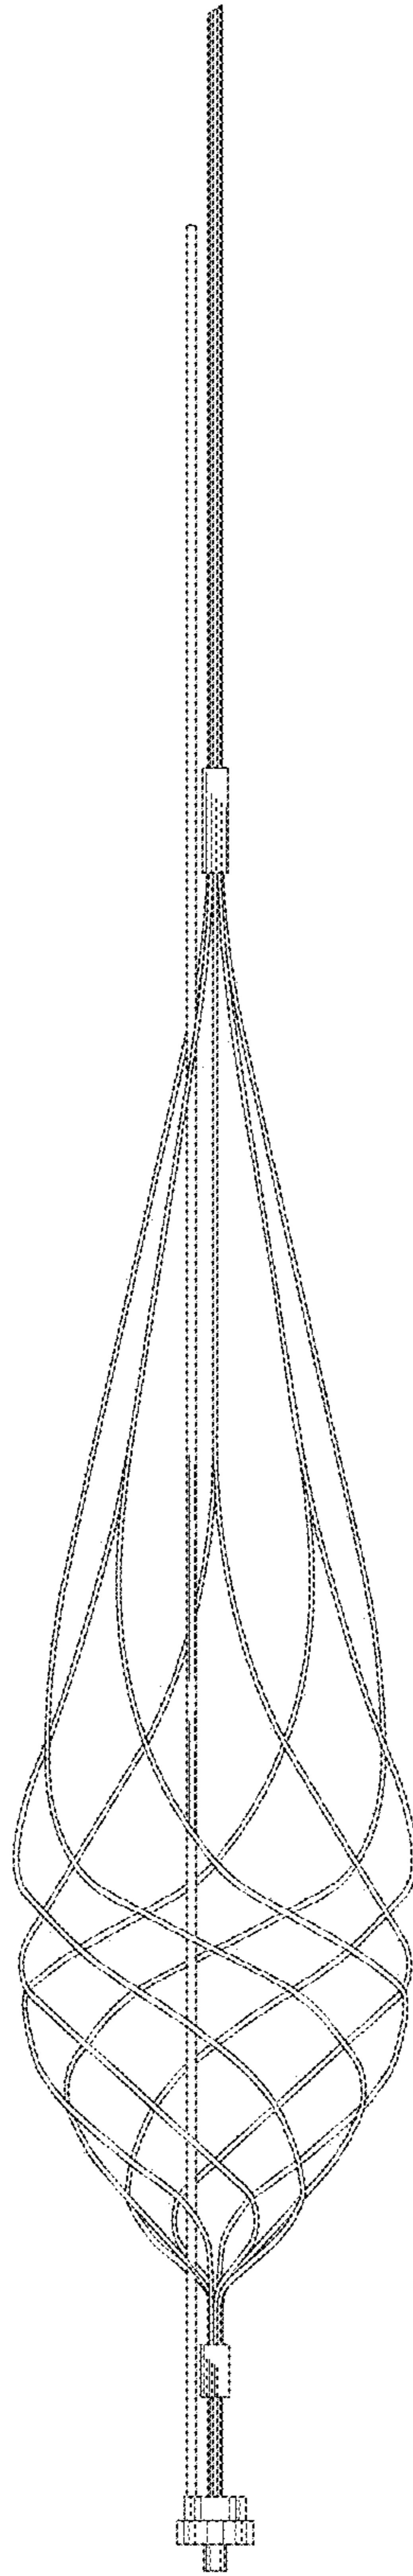

62

FIG. 57

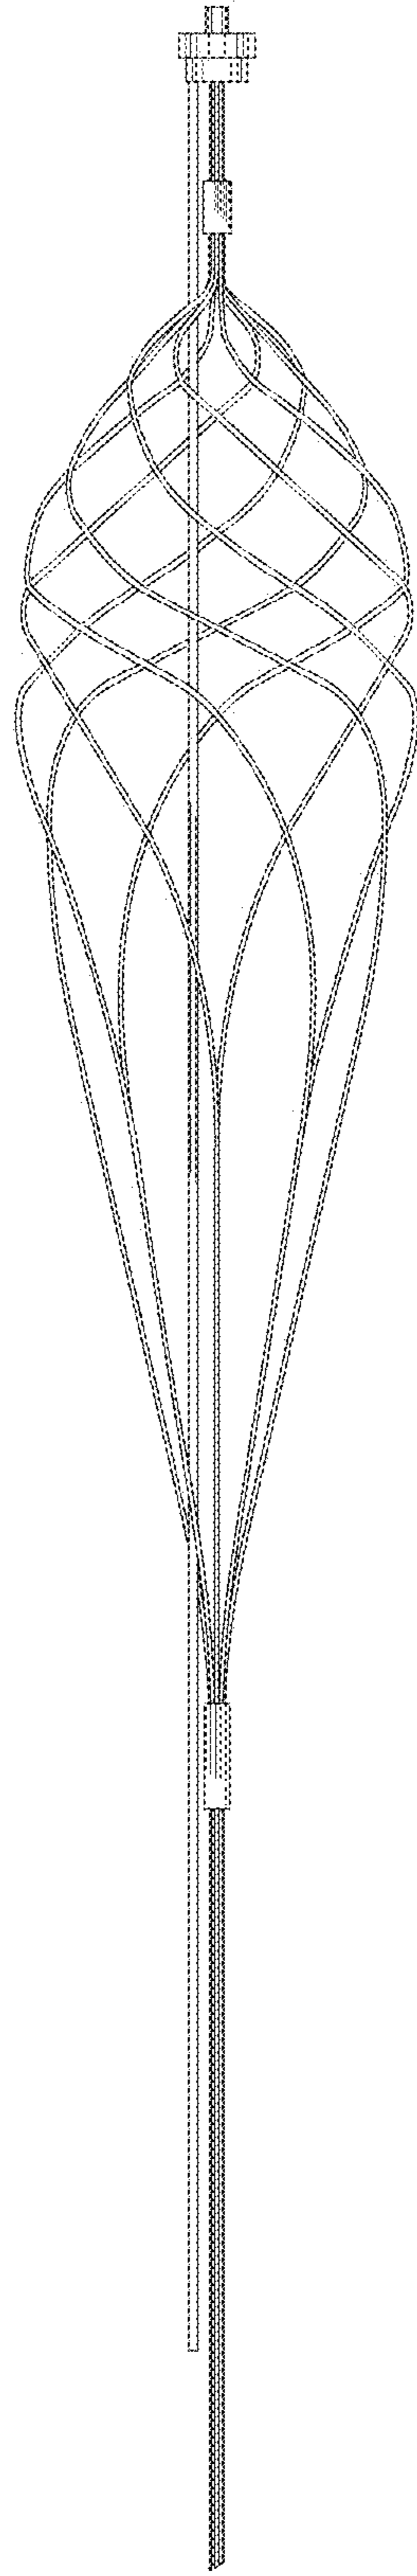


FIG. 58

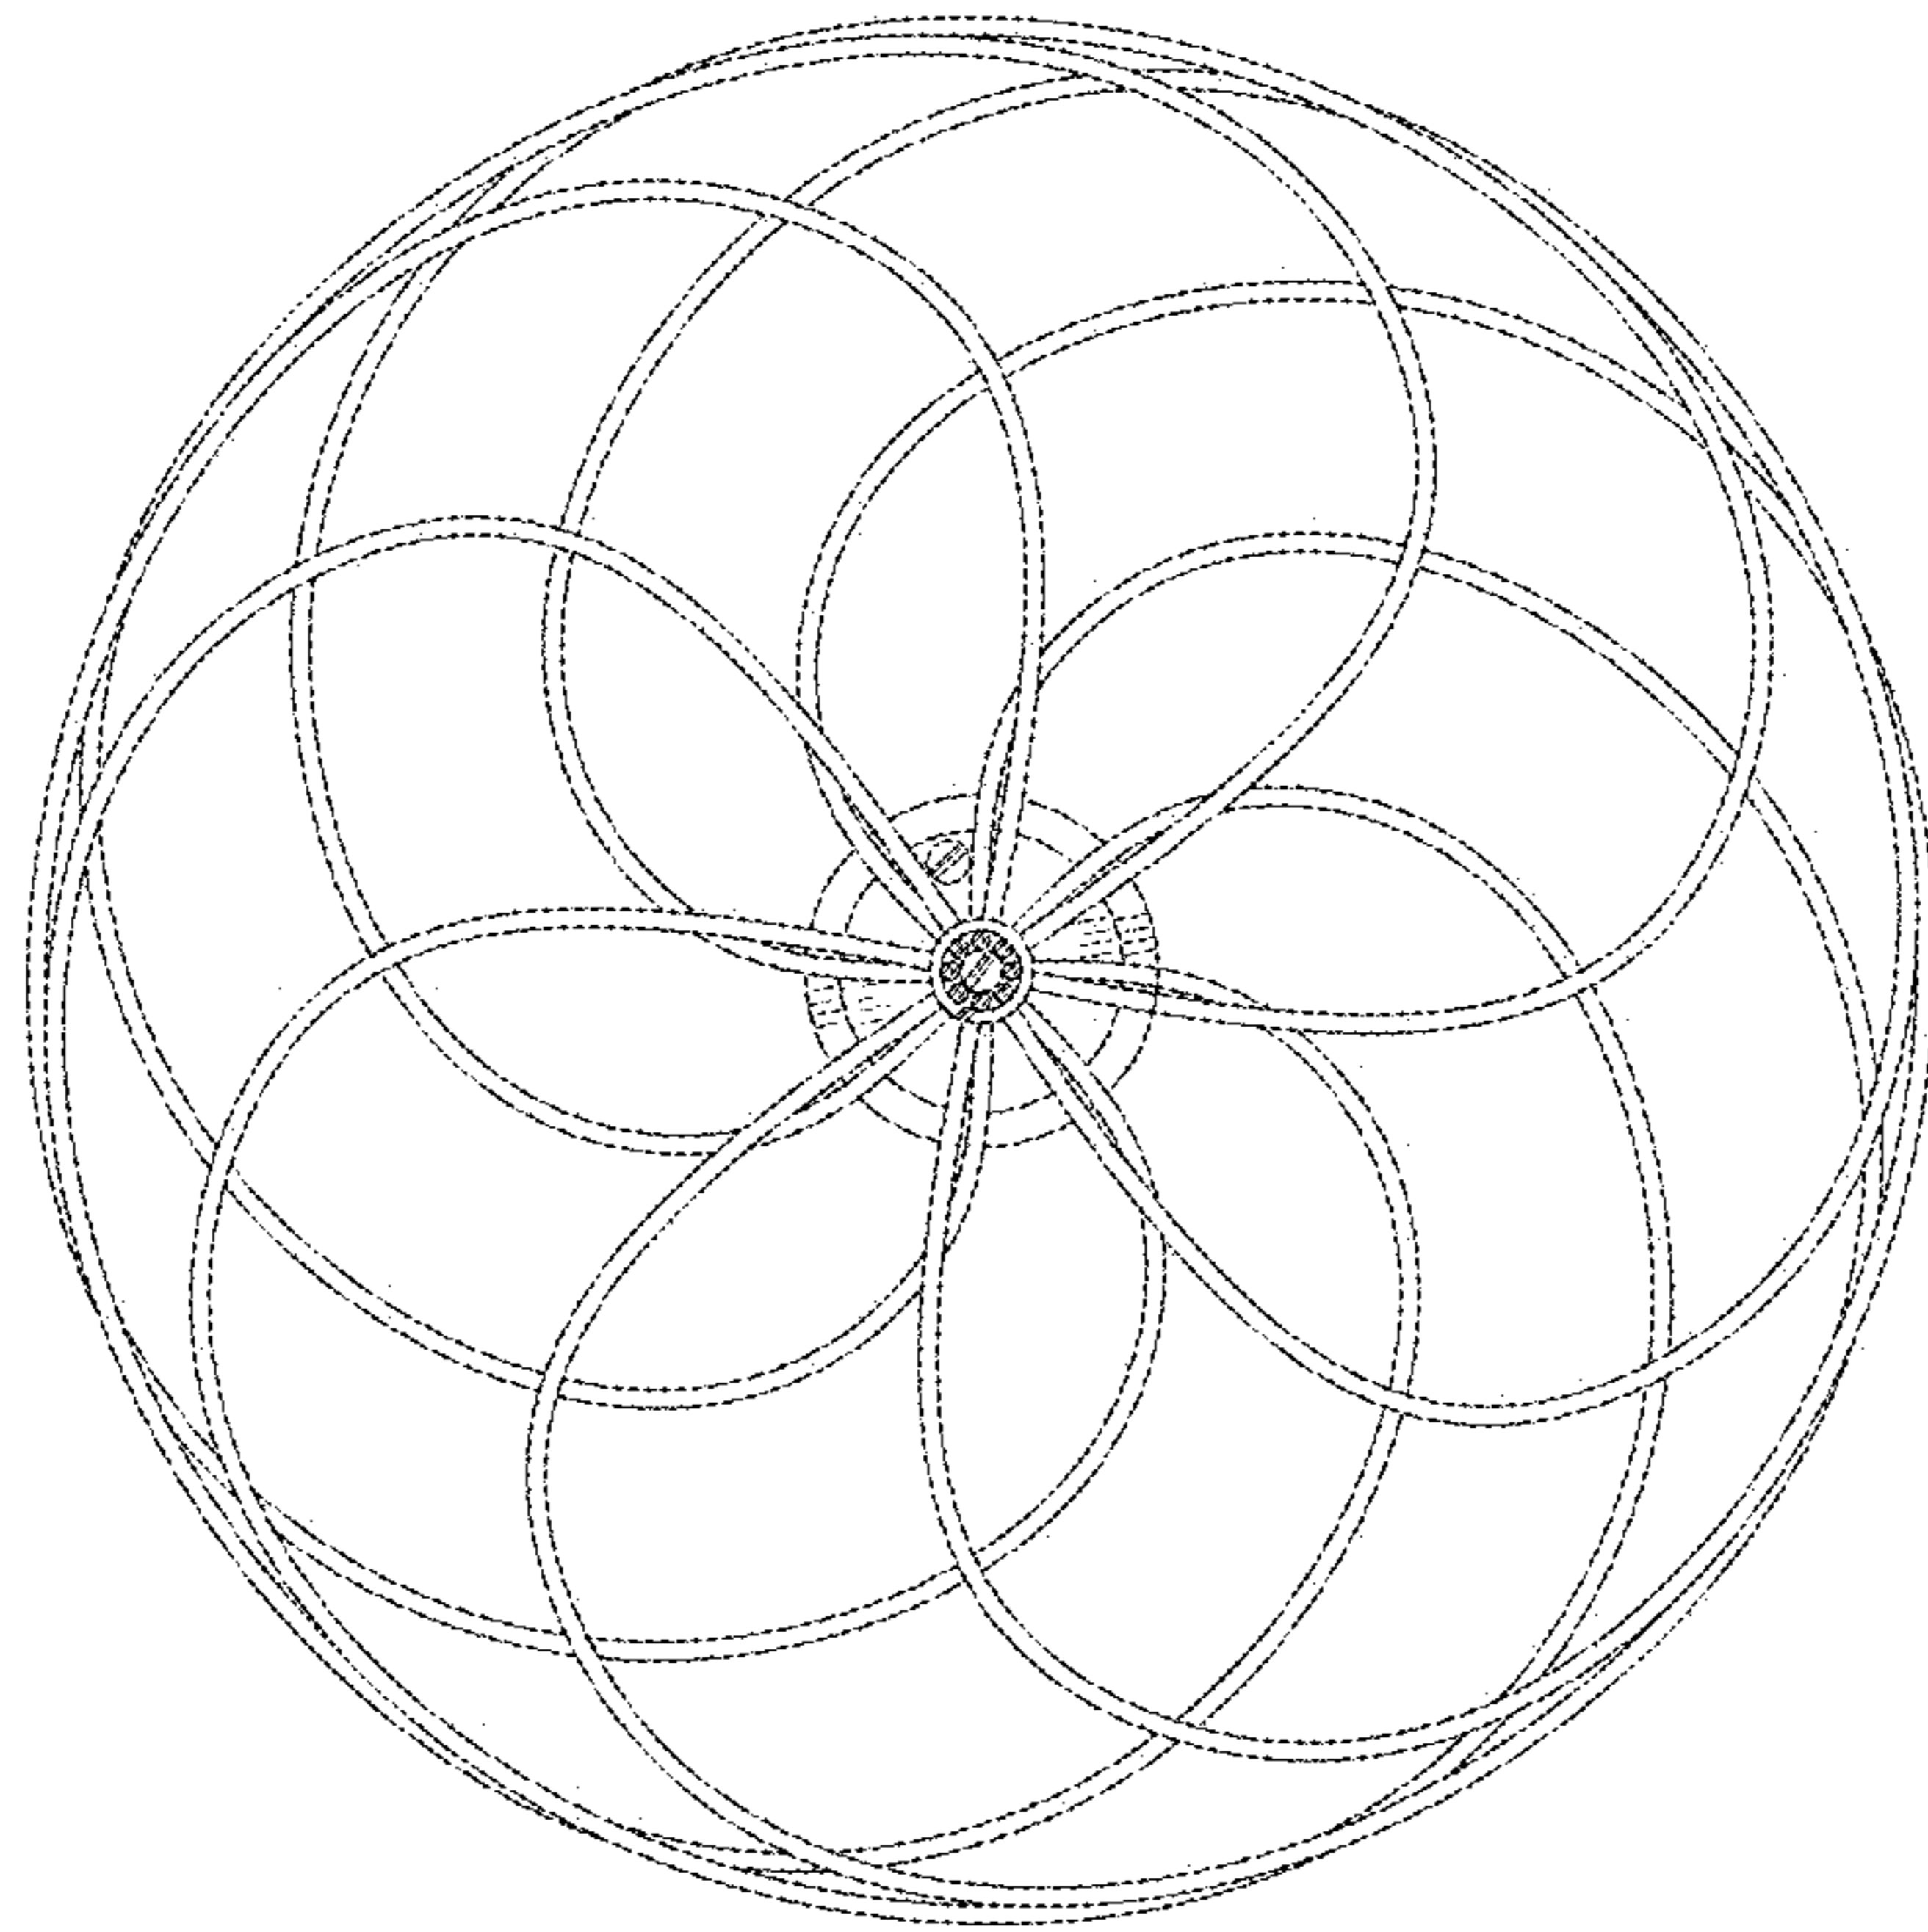


FIG. 59

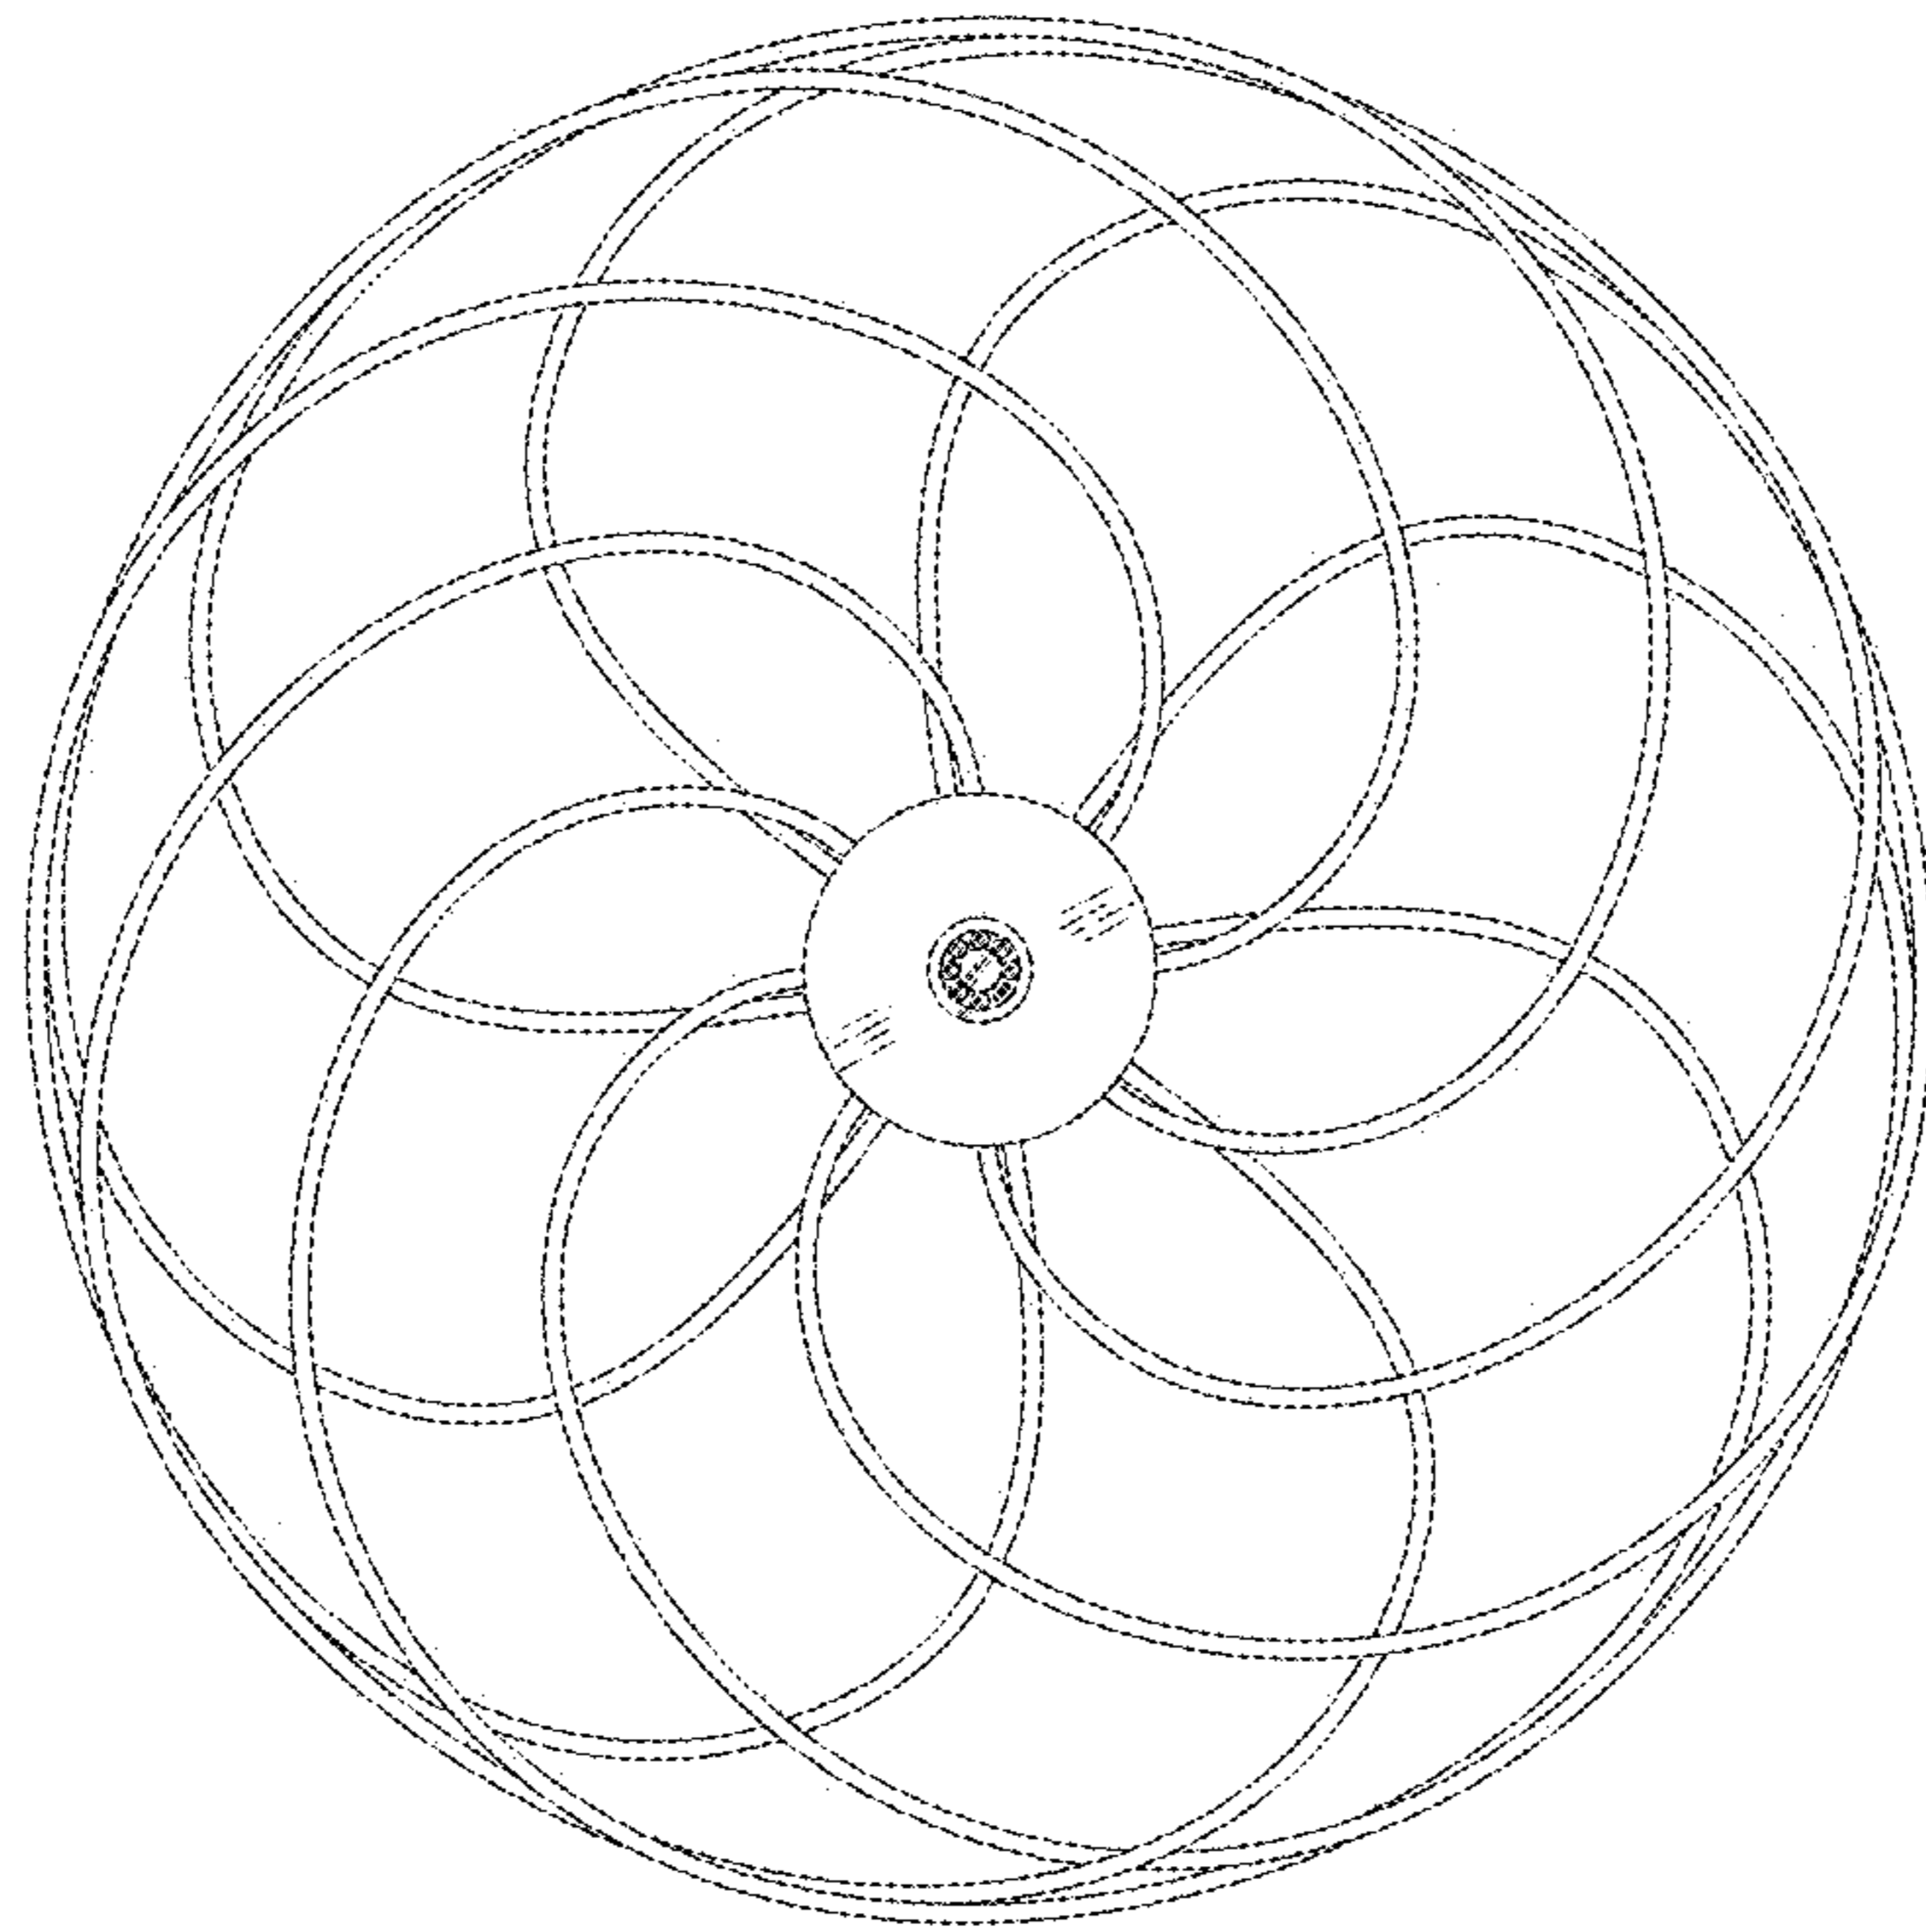


FIG. 60

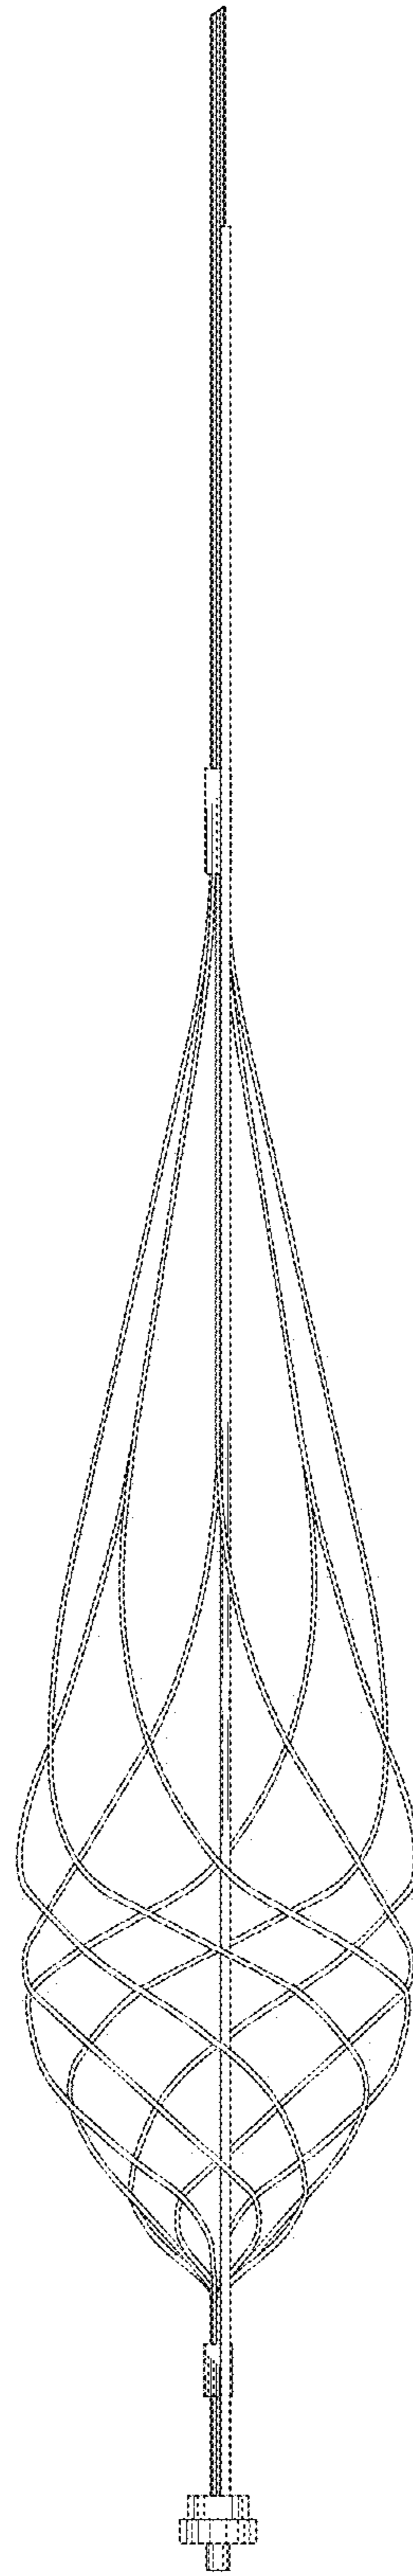


FIG. 61

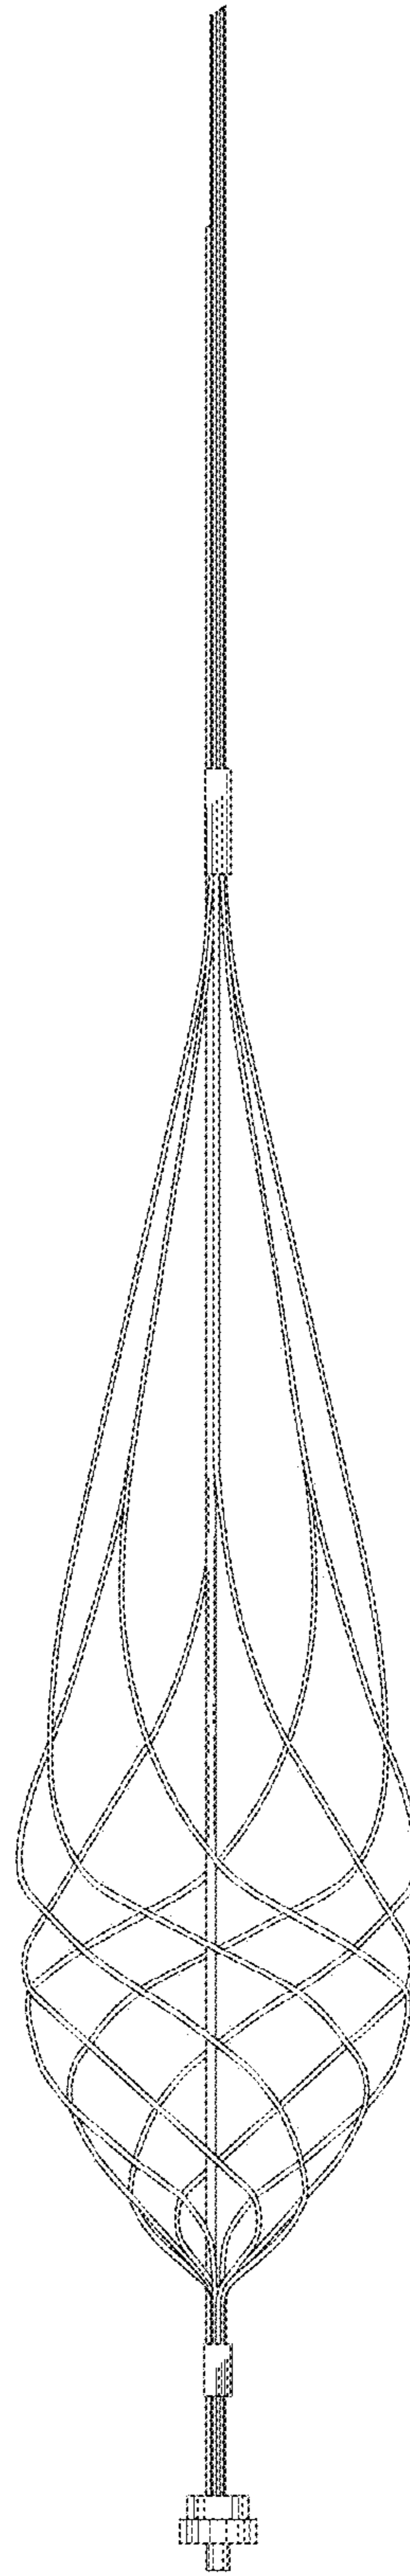


FIG. 62

