



US00D944105S

(12) **United States Design Patent** (10) **Patent No.:** **US D944,105 S**
Barton et al. (45) **Date of Patent:** **** Feb. 22, 2022**

(54) **DIAGNOSTIC ANALYZER**

(71) Applicant: **Abbott Laboratories**, Abbott Park, IL (US)

(72) Inventors: **Christina A. Barton**, Irving, TX (US); **Vladlena Belozero**va, Philadelphia, PA (US); **Ami Marie Verhalen**, Sun Prairie, WI (US); **Jesse Charles Darley**, Madison, WI (US); **Sherry Sue Eckholm**, Sun Prairie, WI (US)

(73) Assignee: **Abbott Laboratories**, Abbott Park, IL (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/722,391**

(22) Filed: **Jan. 29, 2020**

Related U.S. Application Data

(63) Continuation of application No. 29/692,206, filed on May 23, 2019, now Pat. No. Des. 876,259, which is (Continued)

(51) **LOC (13) Cl.** **10-04**

(52) **U.S. Cl.**
USPC **D10/81; D24/216**

(58) **Field of Classification Search**
USPC **D10/81; D24/216, 219, 220, 232, 233, D24/234**

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D662,431 S * 6/2012 Kimura D10/81
D724,753 S * 3/2015 Gutmann D24/216
(Continued)

OTHER PUBLICATIONS

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2016-19293, dated Nov. 8, 2016, 3 pages.

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2016-19292, dated Nov. 8, 2016, 3 pages.

(Continued)

Primary Examiner — Antoine Duval Davis
(74) *Attorney, Agent, or Firm* — Hanley, Flight & Zimmerman, LLC

(57) **CLAIM**

The ornamental design for a "diagnostic analyzer," as shown and described.

DESCRIPTION

FIG. 1 is a front left perspective view of a diagnostic analyzer.

FIG. 2 is a front view of the diagnostic analyzer of FIG. 1.

FIG. 3 is a rear view of the diagnostic analyzer of FIG. 1.

FIG. 4 is a right side view of the diagnostic analyzer of FIG. 1.

FIG. 5 is a left side view of the diagnostic analyzer of FIG. 1.

FIG. 6 is a top view of the diagnostic analyzer of FIG. 1.

FIG. 7 is a bottom view of the diagnostic analyzer of FIG. 1.

FIG. 8 is a front left perspective view of a diagnostic analyzer.

FIG. 9 is a front view of the diagnostic analyzer of FIG. 8.

FIG. 10 is a rear view of the diagnostic analyzer of FIG. 8.

FIG. 11 is a right side view of the diagnostic analyzer of FIG. 8.


FIG. 12 is a left side view of the diagnostic analyzer of FIG. 8.

FIG. 13 is a top view of the diagnostic analyzer of FIG. 8; and,

FIG. 14 is a bottom view of the diagnostic analyzer of FIG. 8.

The features shown in broken lines form no part of the claimed design.

1 Claim, 12 Drawing Sheets

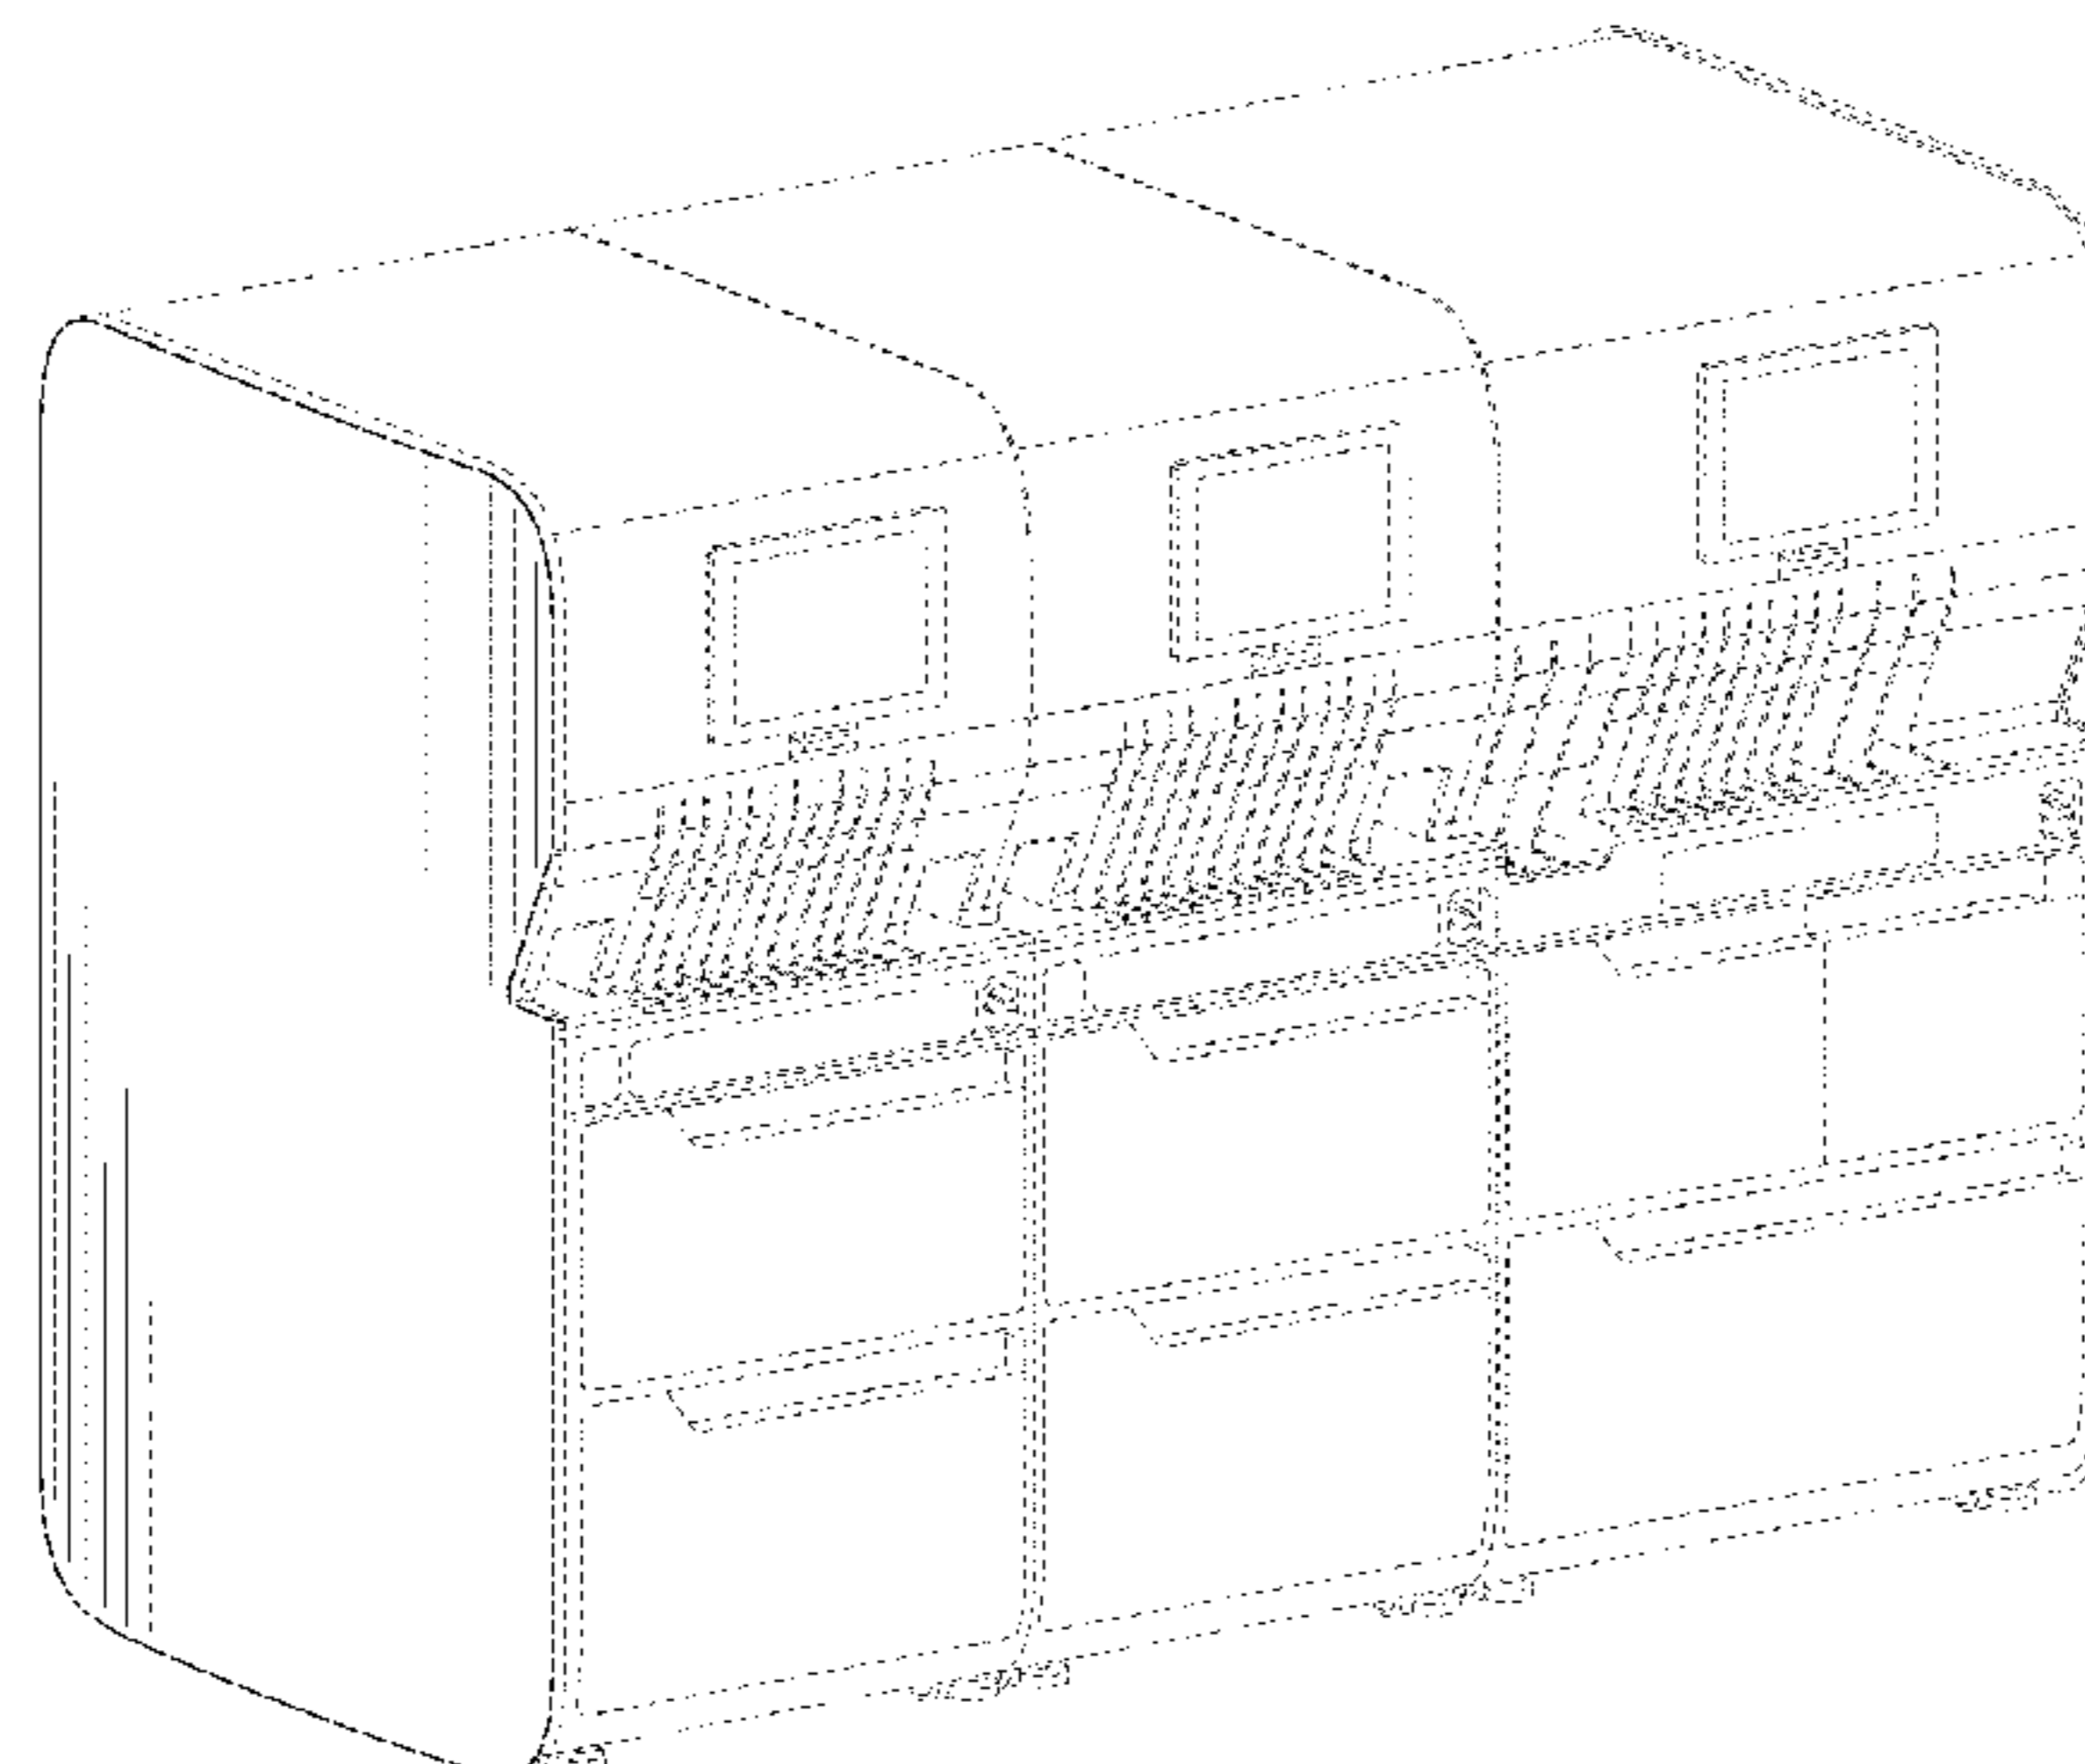

Related U.S. Application Data

a continuation of application No. 29/633,292, filed on Jan. 12, 2018, now Pat. No. Des. 850,955, which is a continuation of application No. 29/587,978, filed on Dec. 16, 2016, now Pat. No. Des. 811,913, which is a continuation of application No. 29/531,578, filed on Jun. 26, 2015, now Pat. No. Des. 777,049.

(58) **Field of Classification Search**

CPC .. G01N 21/00; G01N 21/01; G01N 2201/022; G01N 2201/0221; G01N 2201/0222; G01N 2201/0224; G01N 2201/0225; G01N 2201/0227; G01N 2201/0228; G01N 2201/024; G01N 2201/0245; G01N 2021/0112–21/958; G01N 2021/0106–2021/9586; G01N 35/00–35/1097; G01N 2035/00019–2035/1093; G01N 2204/022–2204/0228

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D773,071 S	11/2016	Hakoda	
D777,049 S	1/2017	Barton et al.	
D788,617 S	6/2017	Barton et al.	
D799,999 S	10/2017	Barton et al.	
D800,000 S	10/2017	Barton et al.	
D802,156 S *	11/2017	Barton	D24/216
D811,913 S	3/2018	Barton et al.	
9,997,266 B2	6/2018	Zhang et al.	
D824,536 S	7/2018	Barton et al.	
D825,776 S	8/2018	Quick et al.	
D828,575 S	9/2018	Ohno	
D830,210 S	10/2018	Ihara	
10,220,387 B2	3/2019	Granier et al.	
D850,955 S	6/2019	Barton et al.	
D850,956 S	6/2019	Barton et al.	

OTHER PUBLICATIONS

Japanese Patent Office, “Notice of Reason for Rejection,” issued in connection with Japanese Design Application No. 2016-19291, dated Nov. 8, 2016, 3 pages.
 State Intellectual Property Office of China, “Notice of Grant of Patent Right,” issued in connection with Chinese Patent Application No. 201530555258.3, dated Oct. 20, 2016, 5 pages.
 Japanese Patent Office, “Notice of Reason for Rejection,” issued in connection with Japanese Design Application No. 2015-28872 dated Jun. 14, 2016, 5 pages.
 Office For Harmonization in the Internal Market, “Notification of the Registration of the Community Designs,” issued in connection with European Community Design Nos. 002930230-0001 through 002930230-0029, dated Mar. 17, 2016, 6 pages.
 United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/531,578, dated Sep. 8, 2016, 14 pages.
 United States Patent and Trademark Office, “Restriction and/or Election Requirement,” issued in connection with U.S. Appl. No. 29/531,578, dated Jul. 6, 2016, 18 pages.
 Japanese Patent Office, “Directive,” issued in connection with Japanese Patent Application No. 2016-19292, mailed Mar. 7, 2017, 5 pages.
 State Intellectual Property Office of China, “Notice of Grant of Patent Right for a Design,” issued in connection with Chinese Patent Application No. 201630657956.9, dated Jul. 6, 2017, 2 pages.
 United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/587,978, dated Nov. 3, 2017, 8 pages.
 United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/633,295, dated Jan. 17, 2019, 24 pages.
 United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/633,292, dated Jan. 17, 2019, 25 pages.
 United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/692,206, dated Oct. 17, 2019, 9 pages.

* cited by examiner

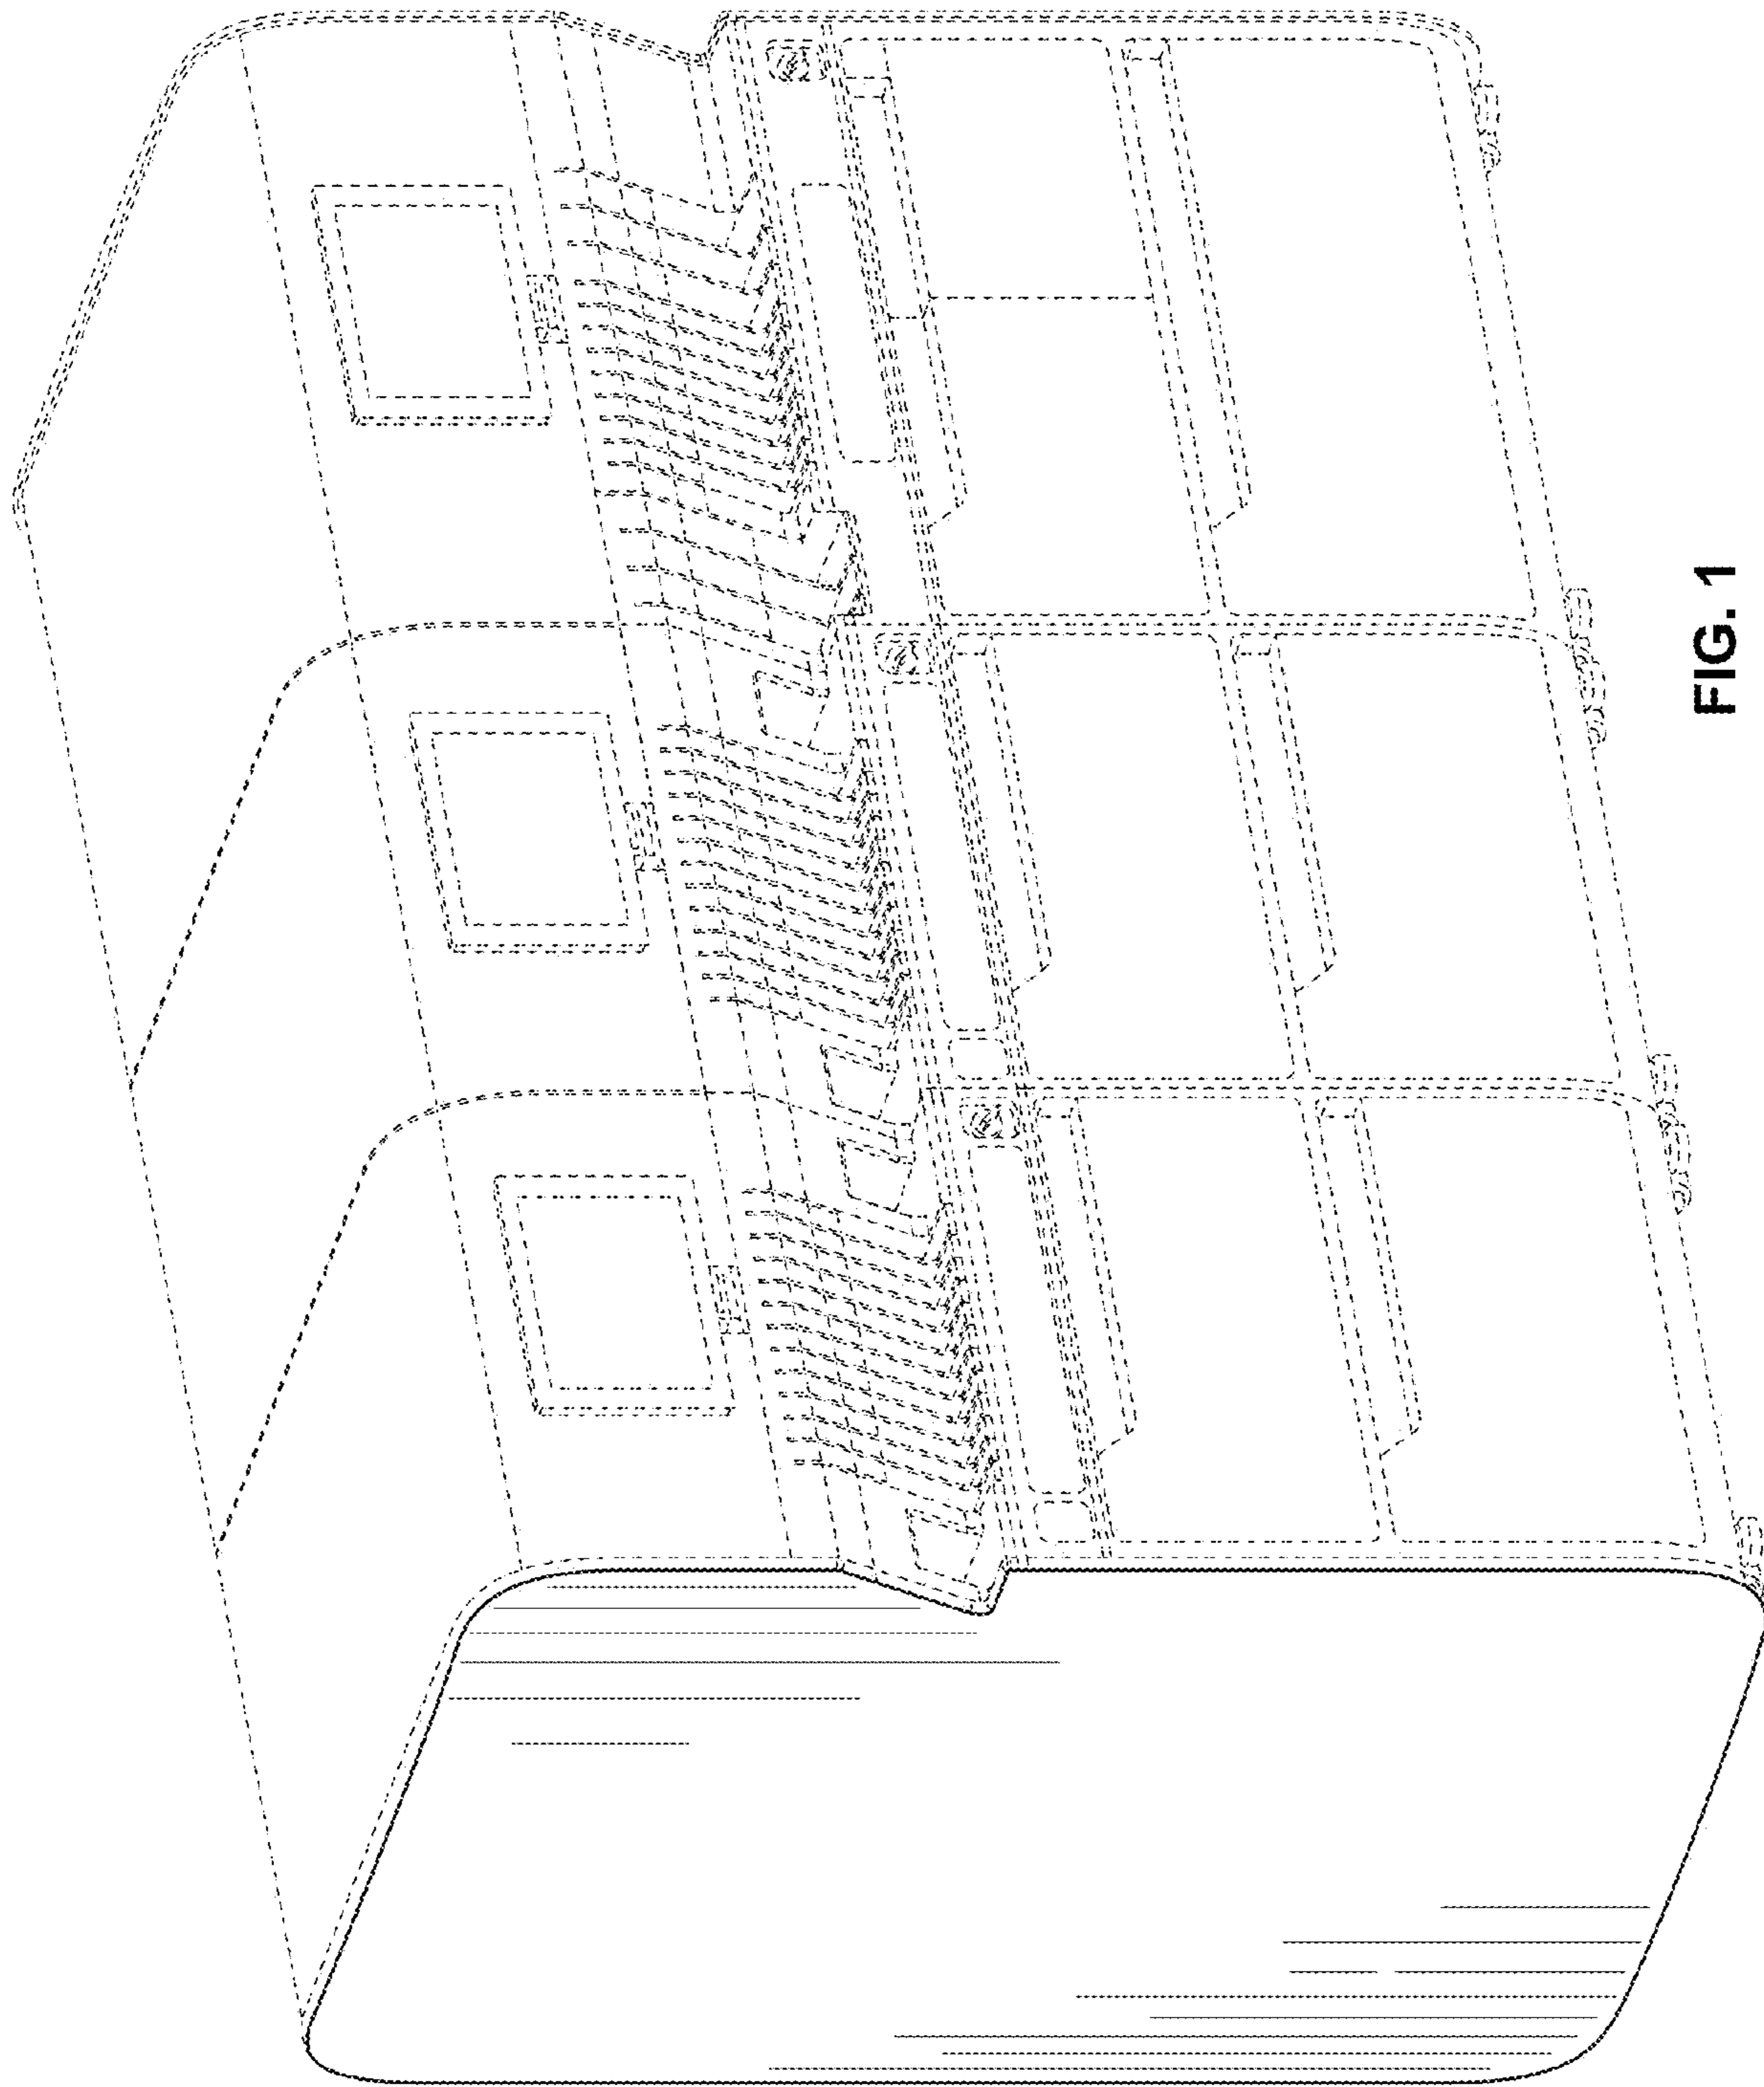


FIG. 1

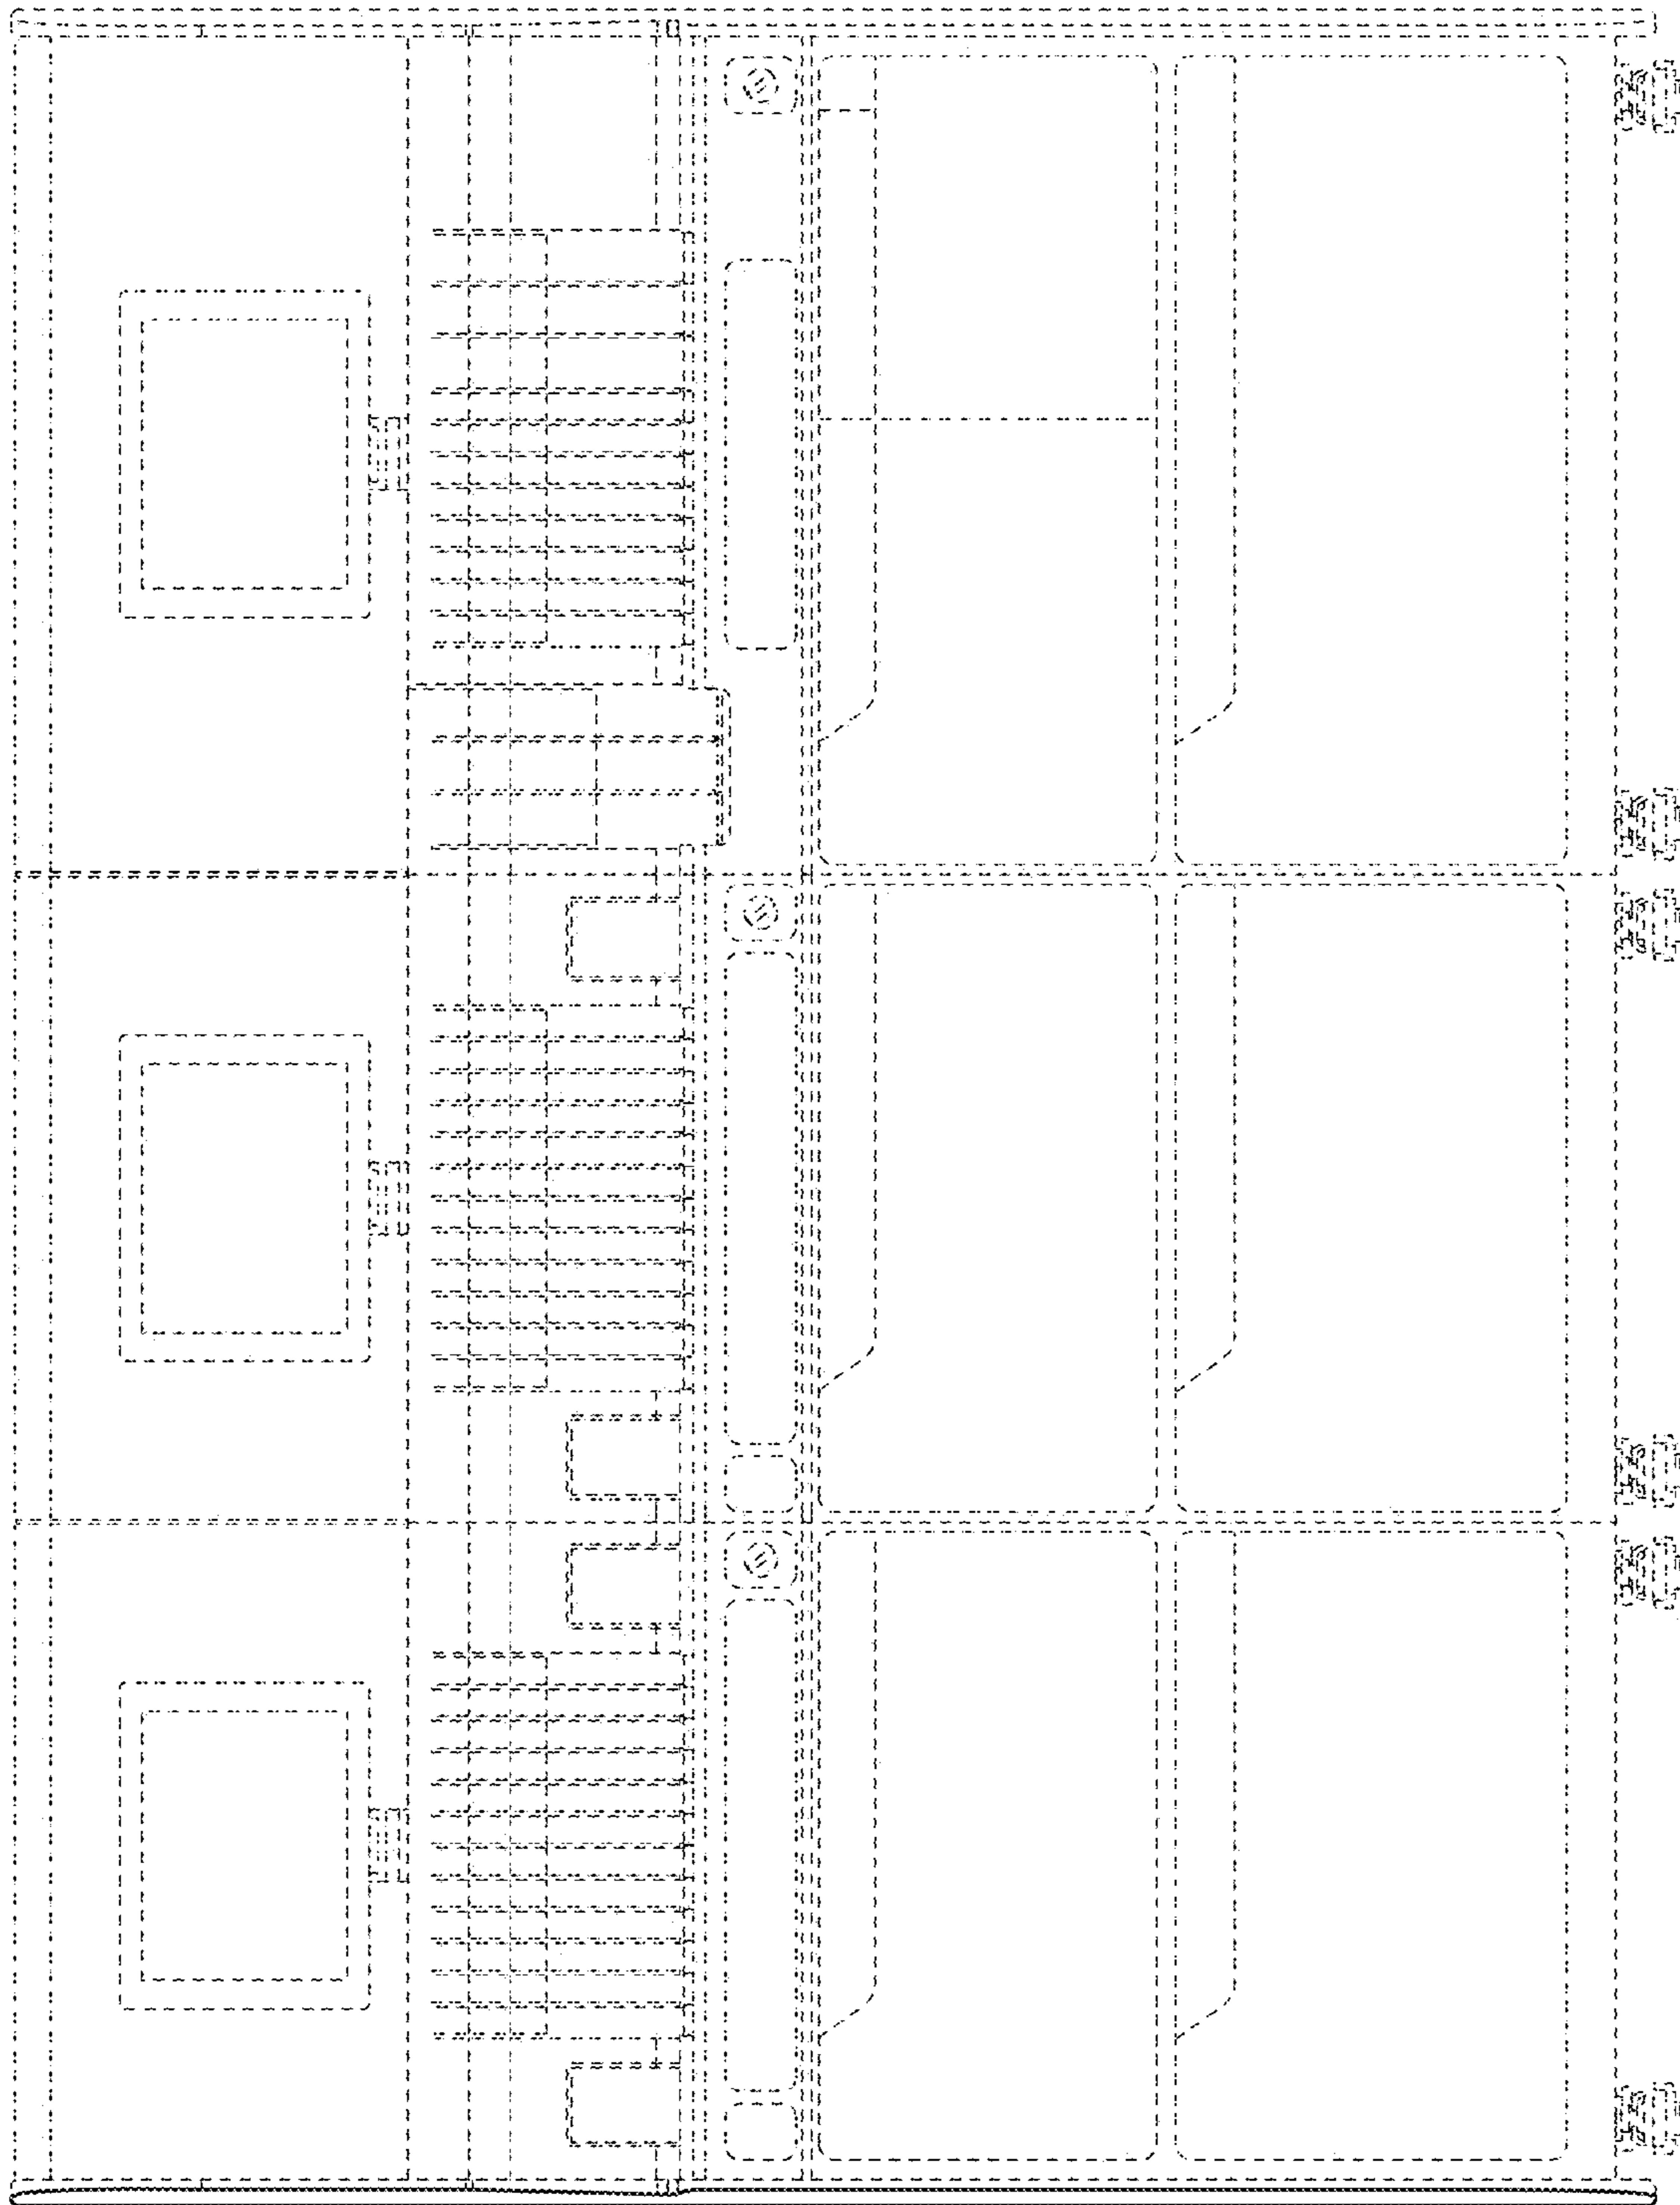


FIG. 2



FIG. 3

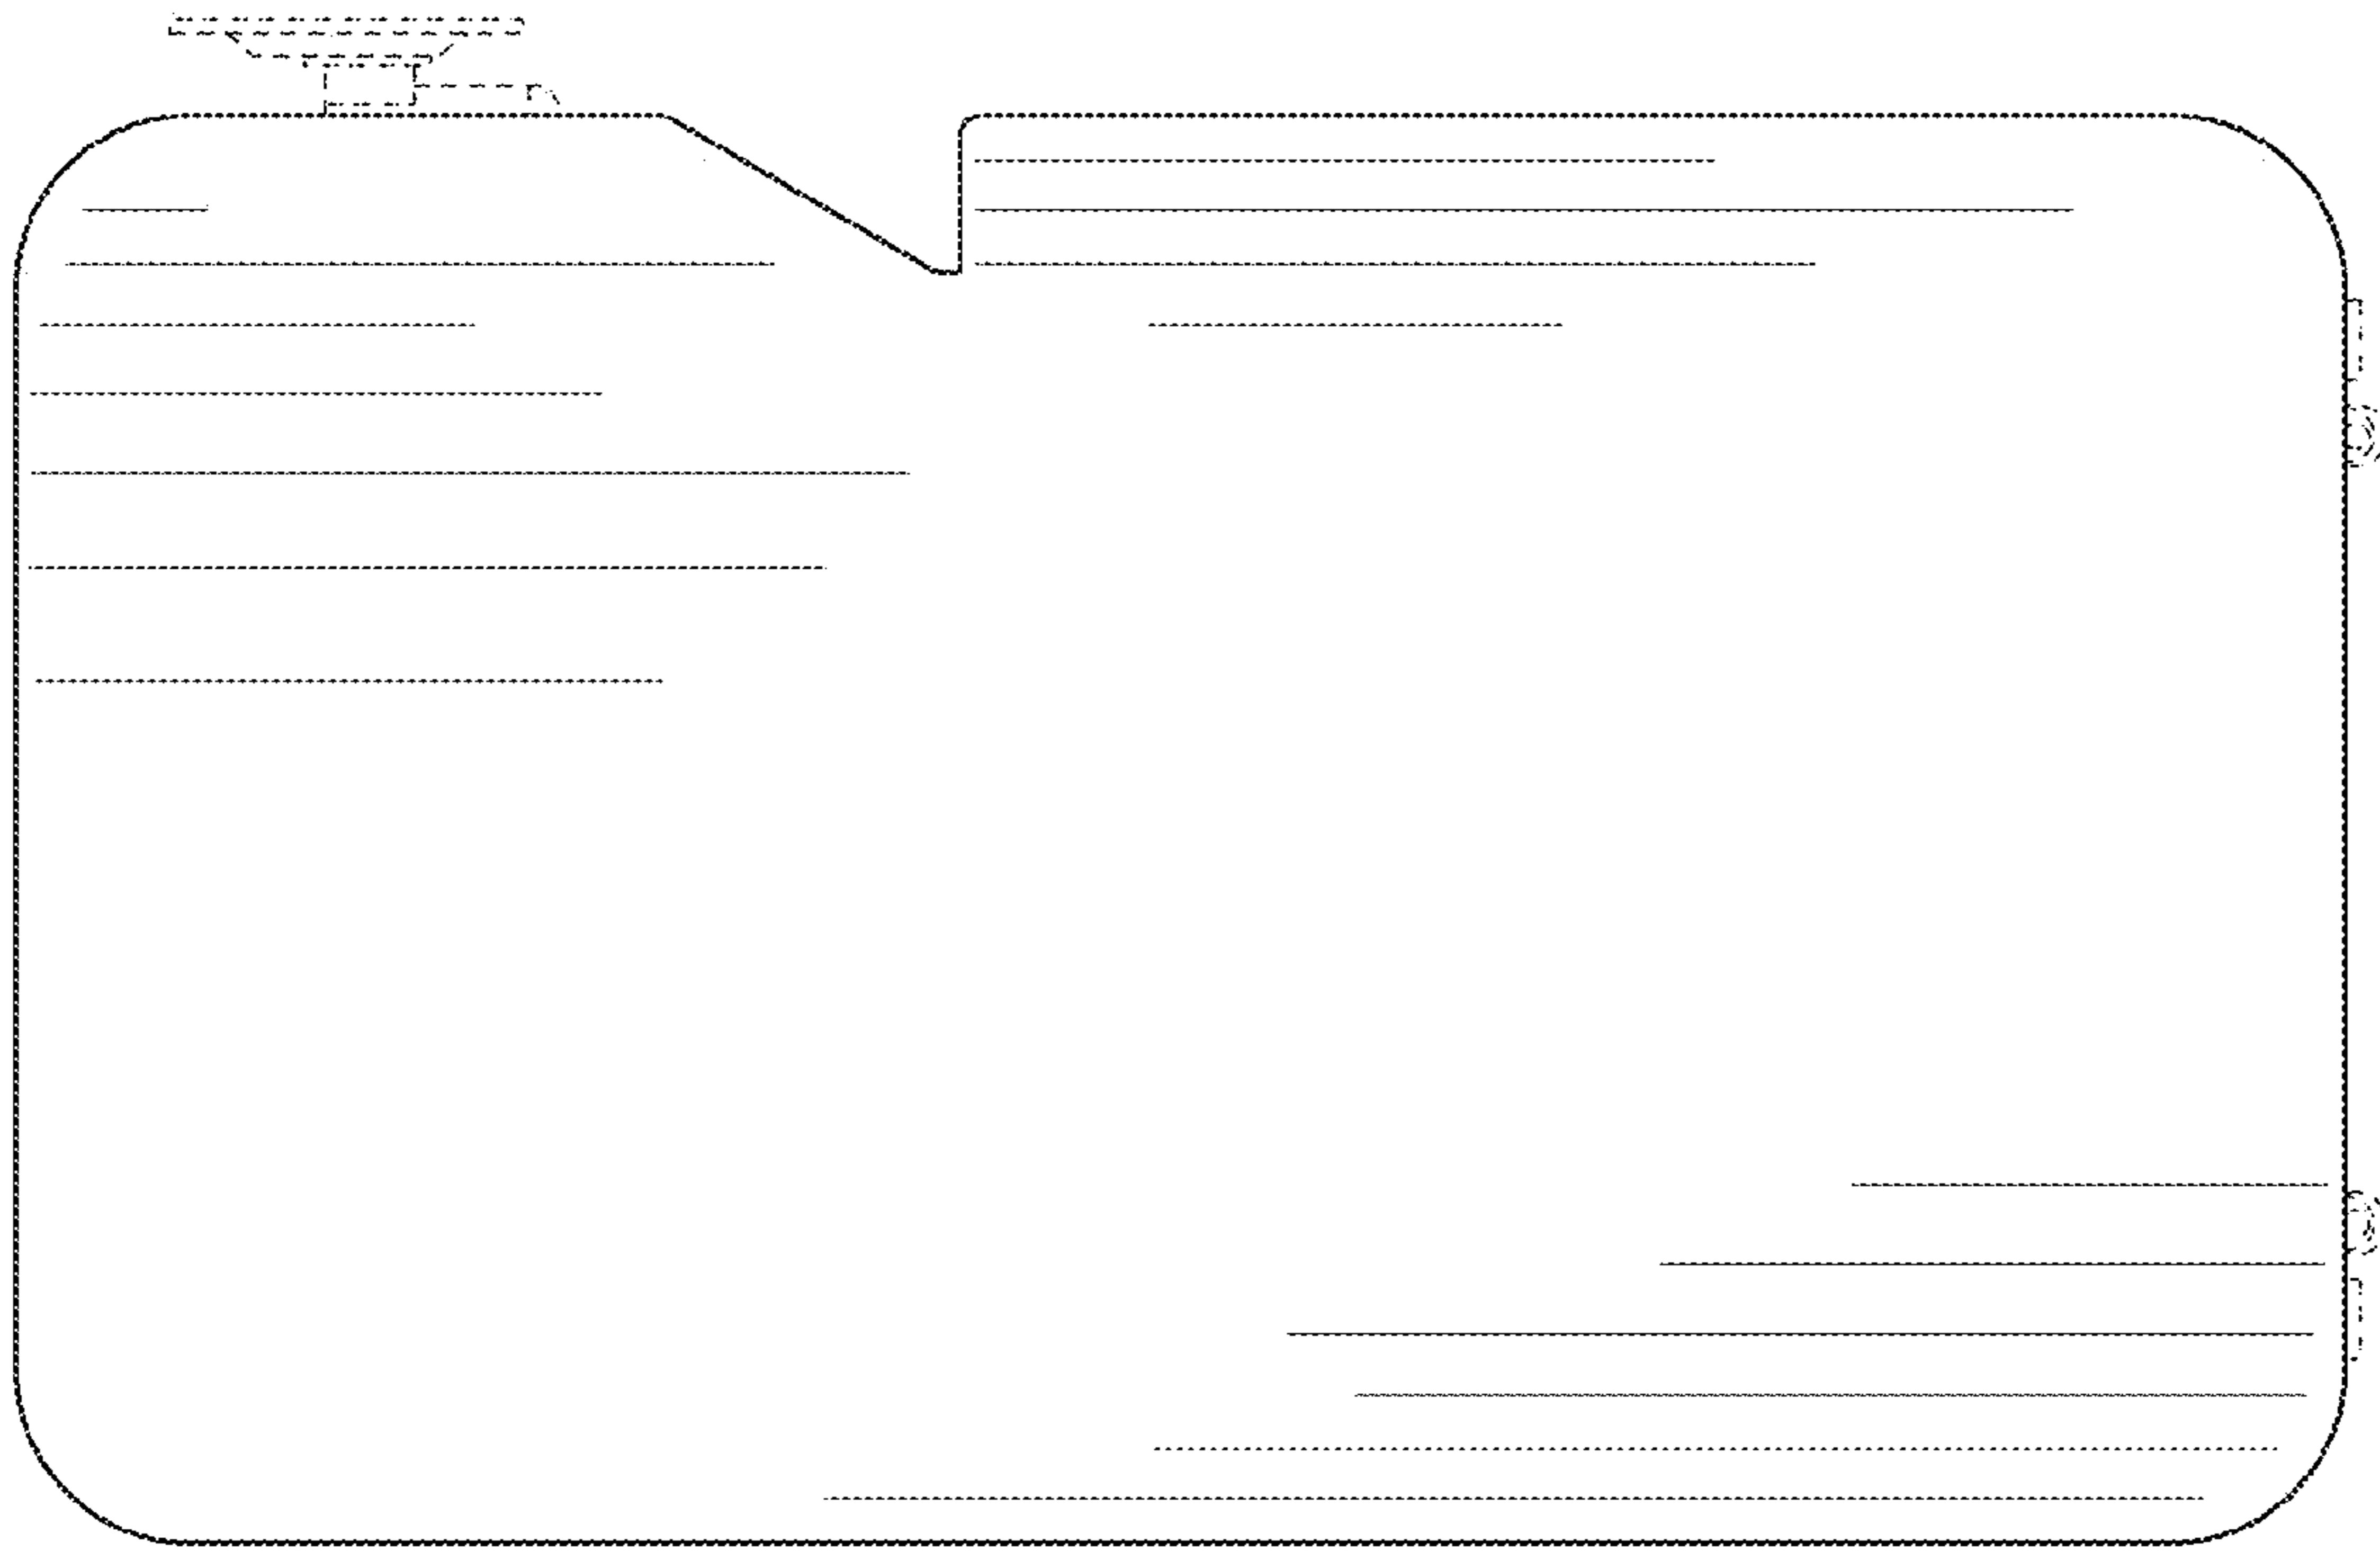


FIG. 4

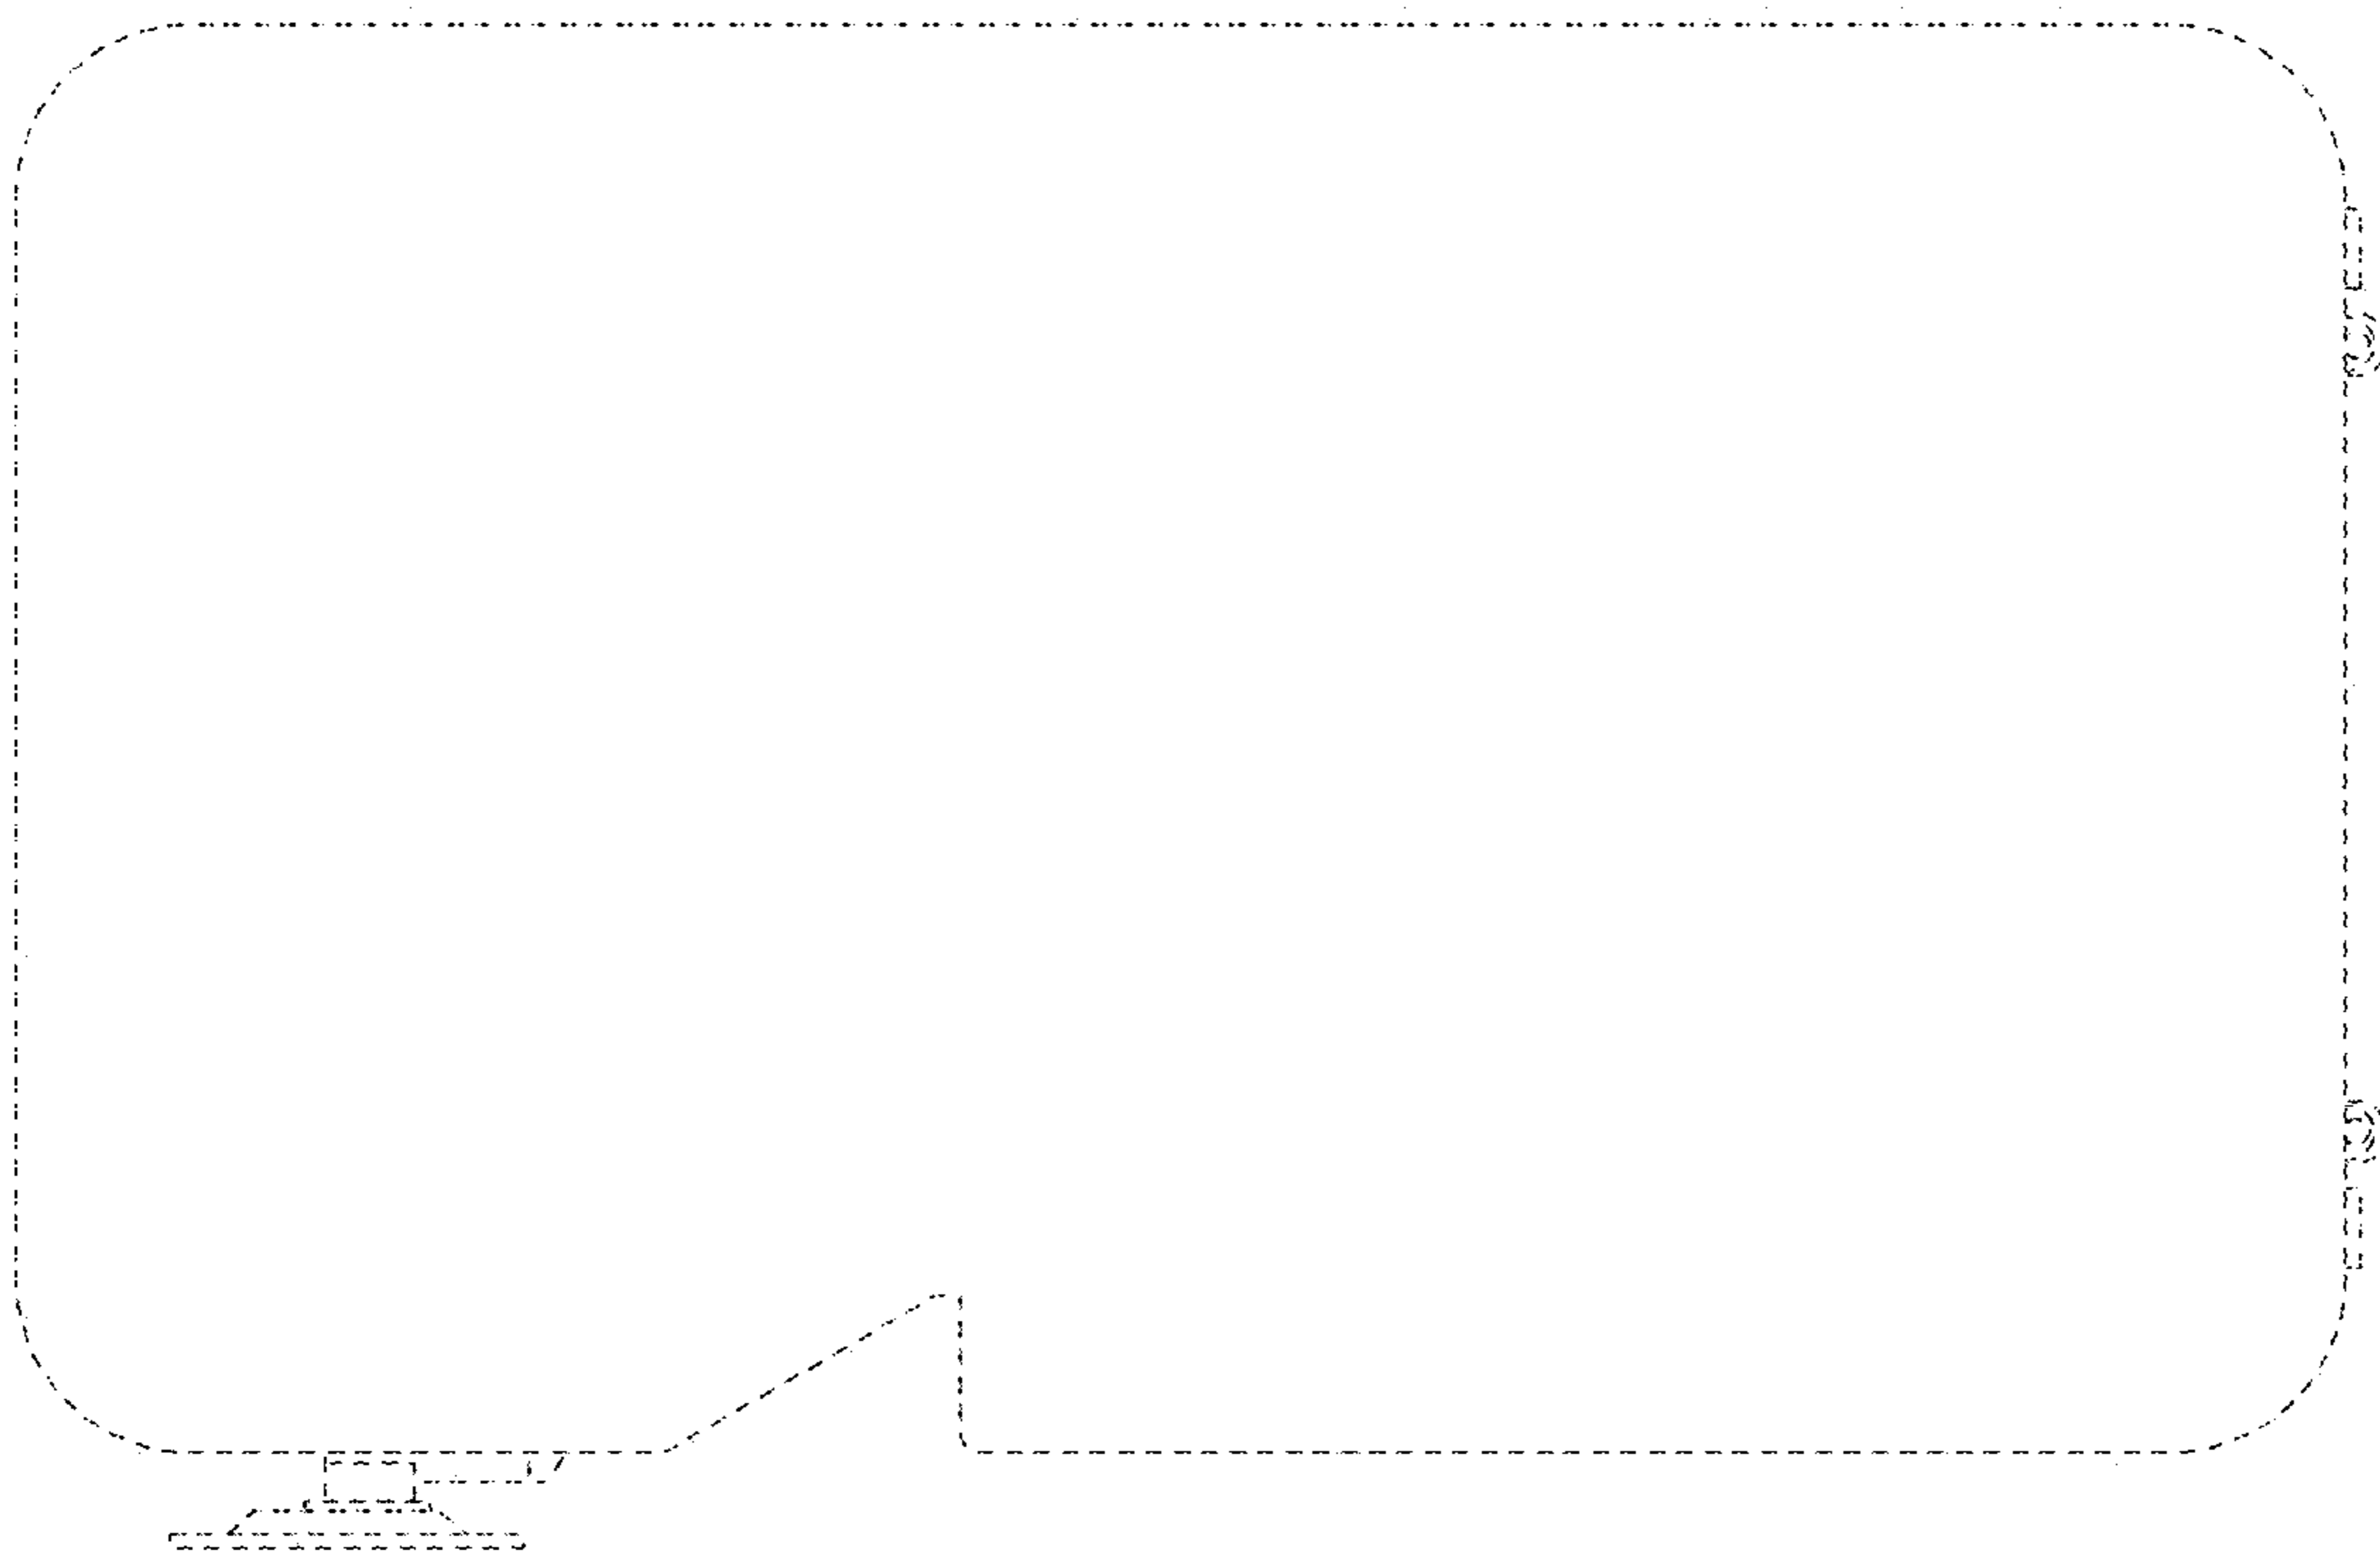


FIG. 5

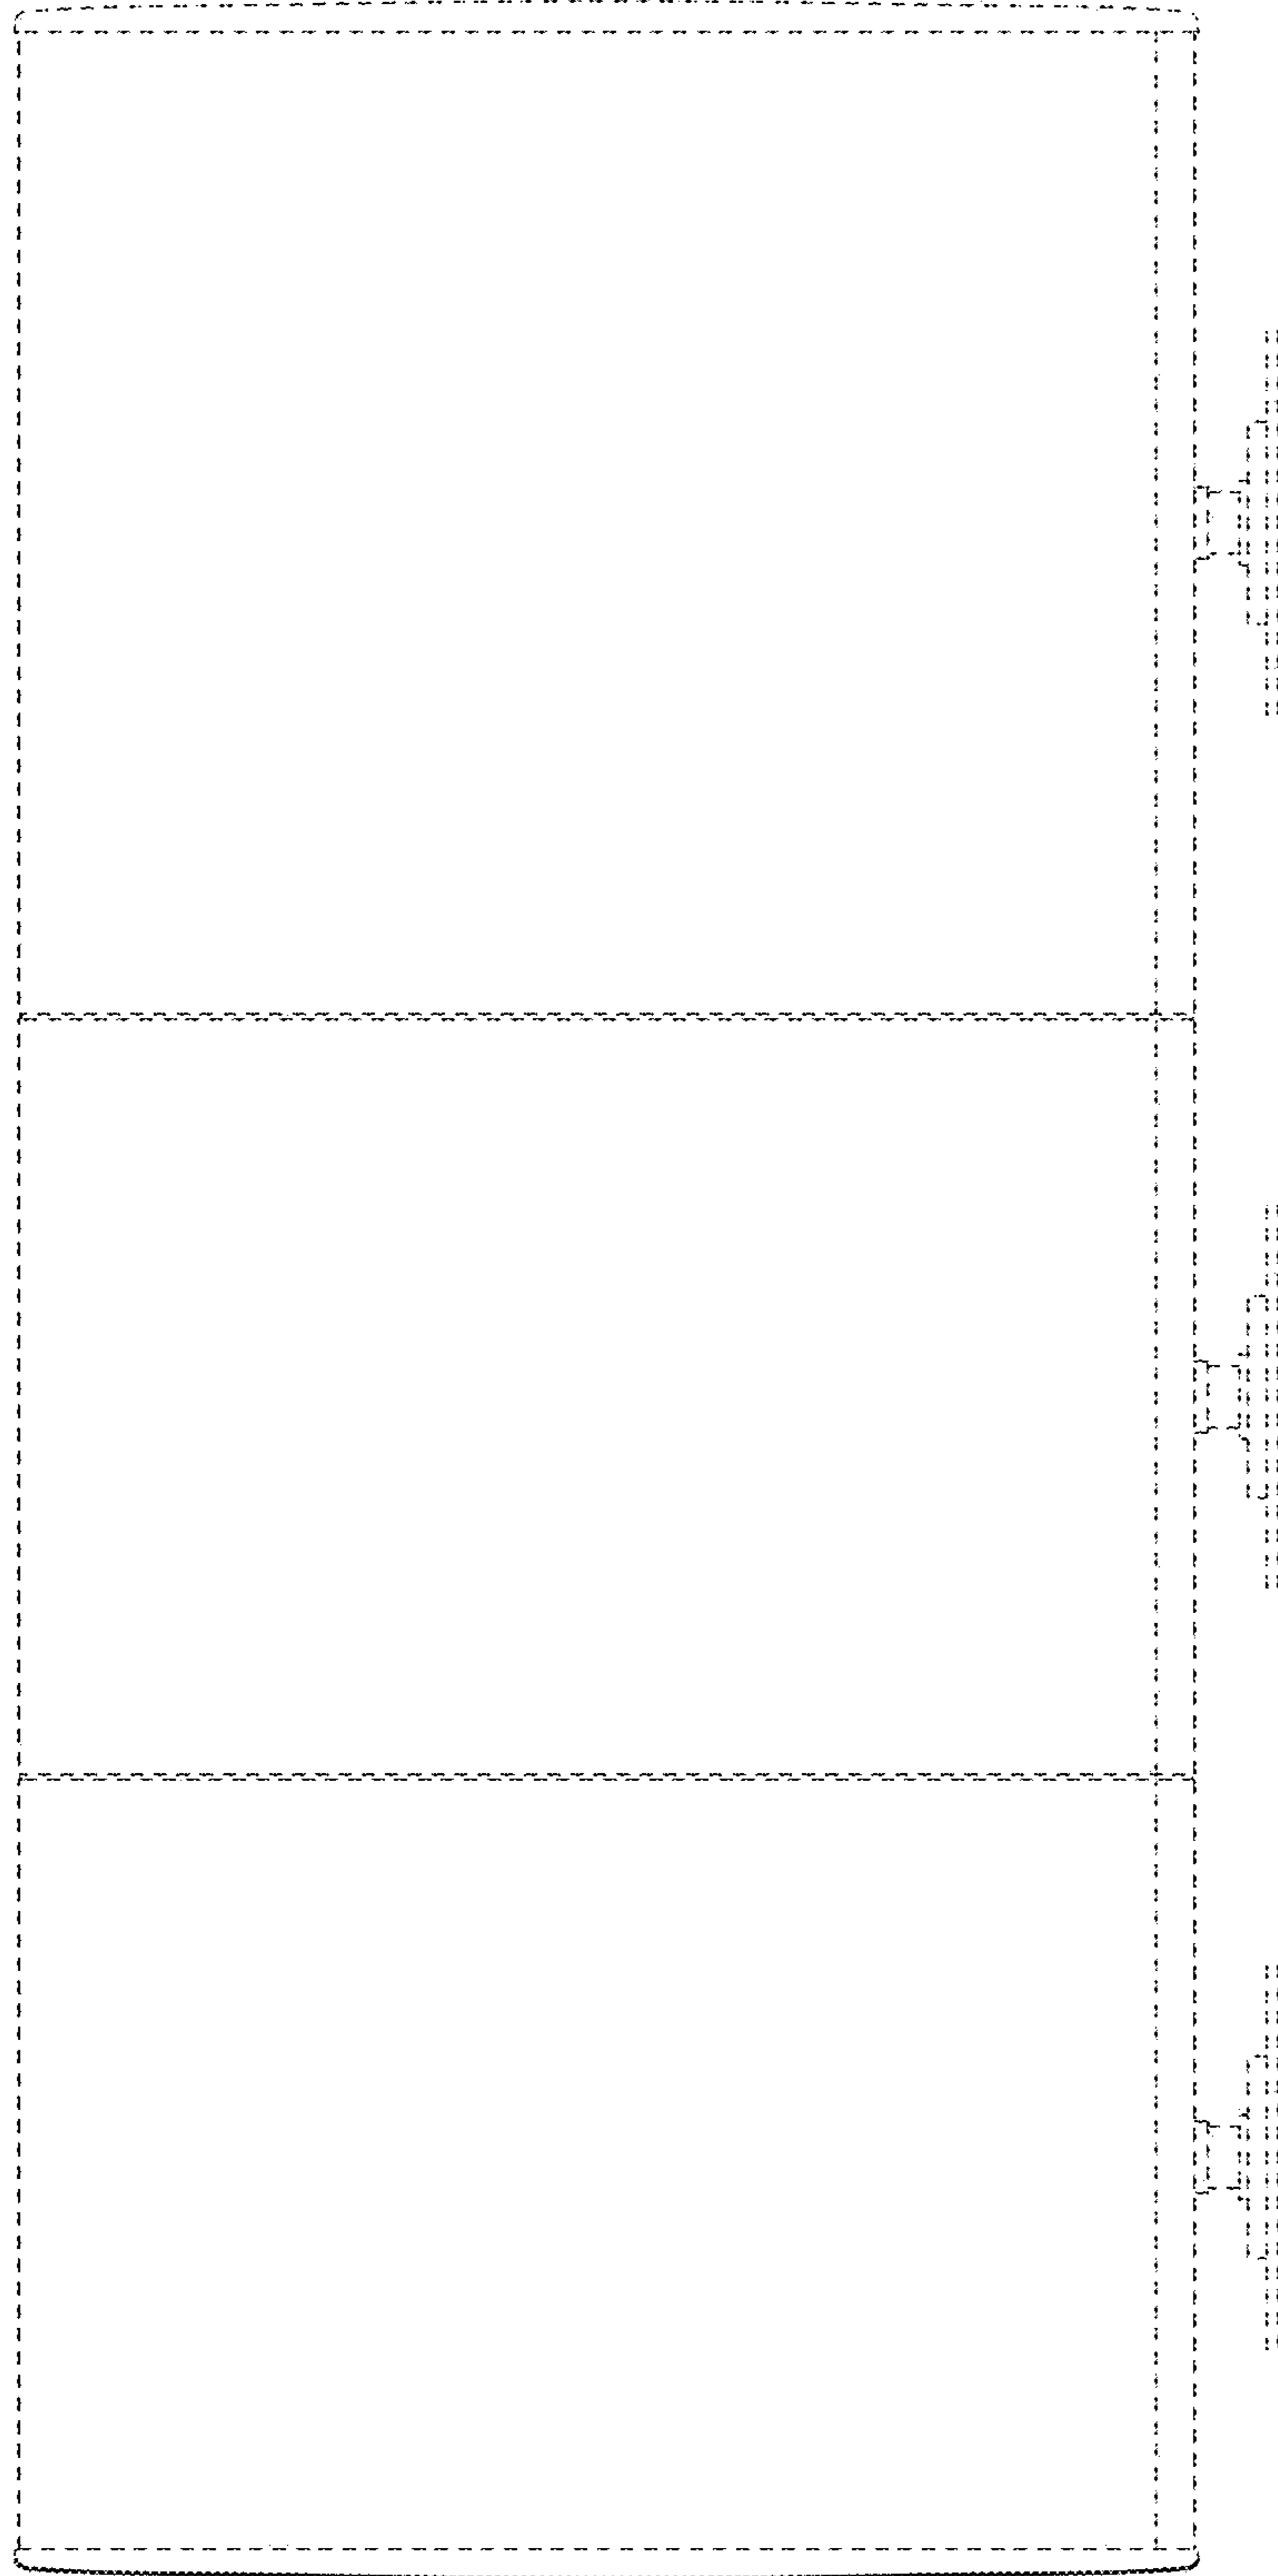


FIG. 6

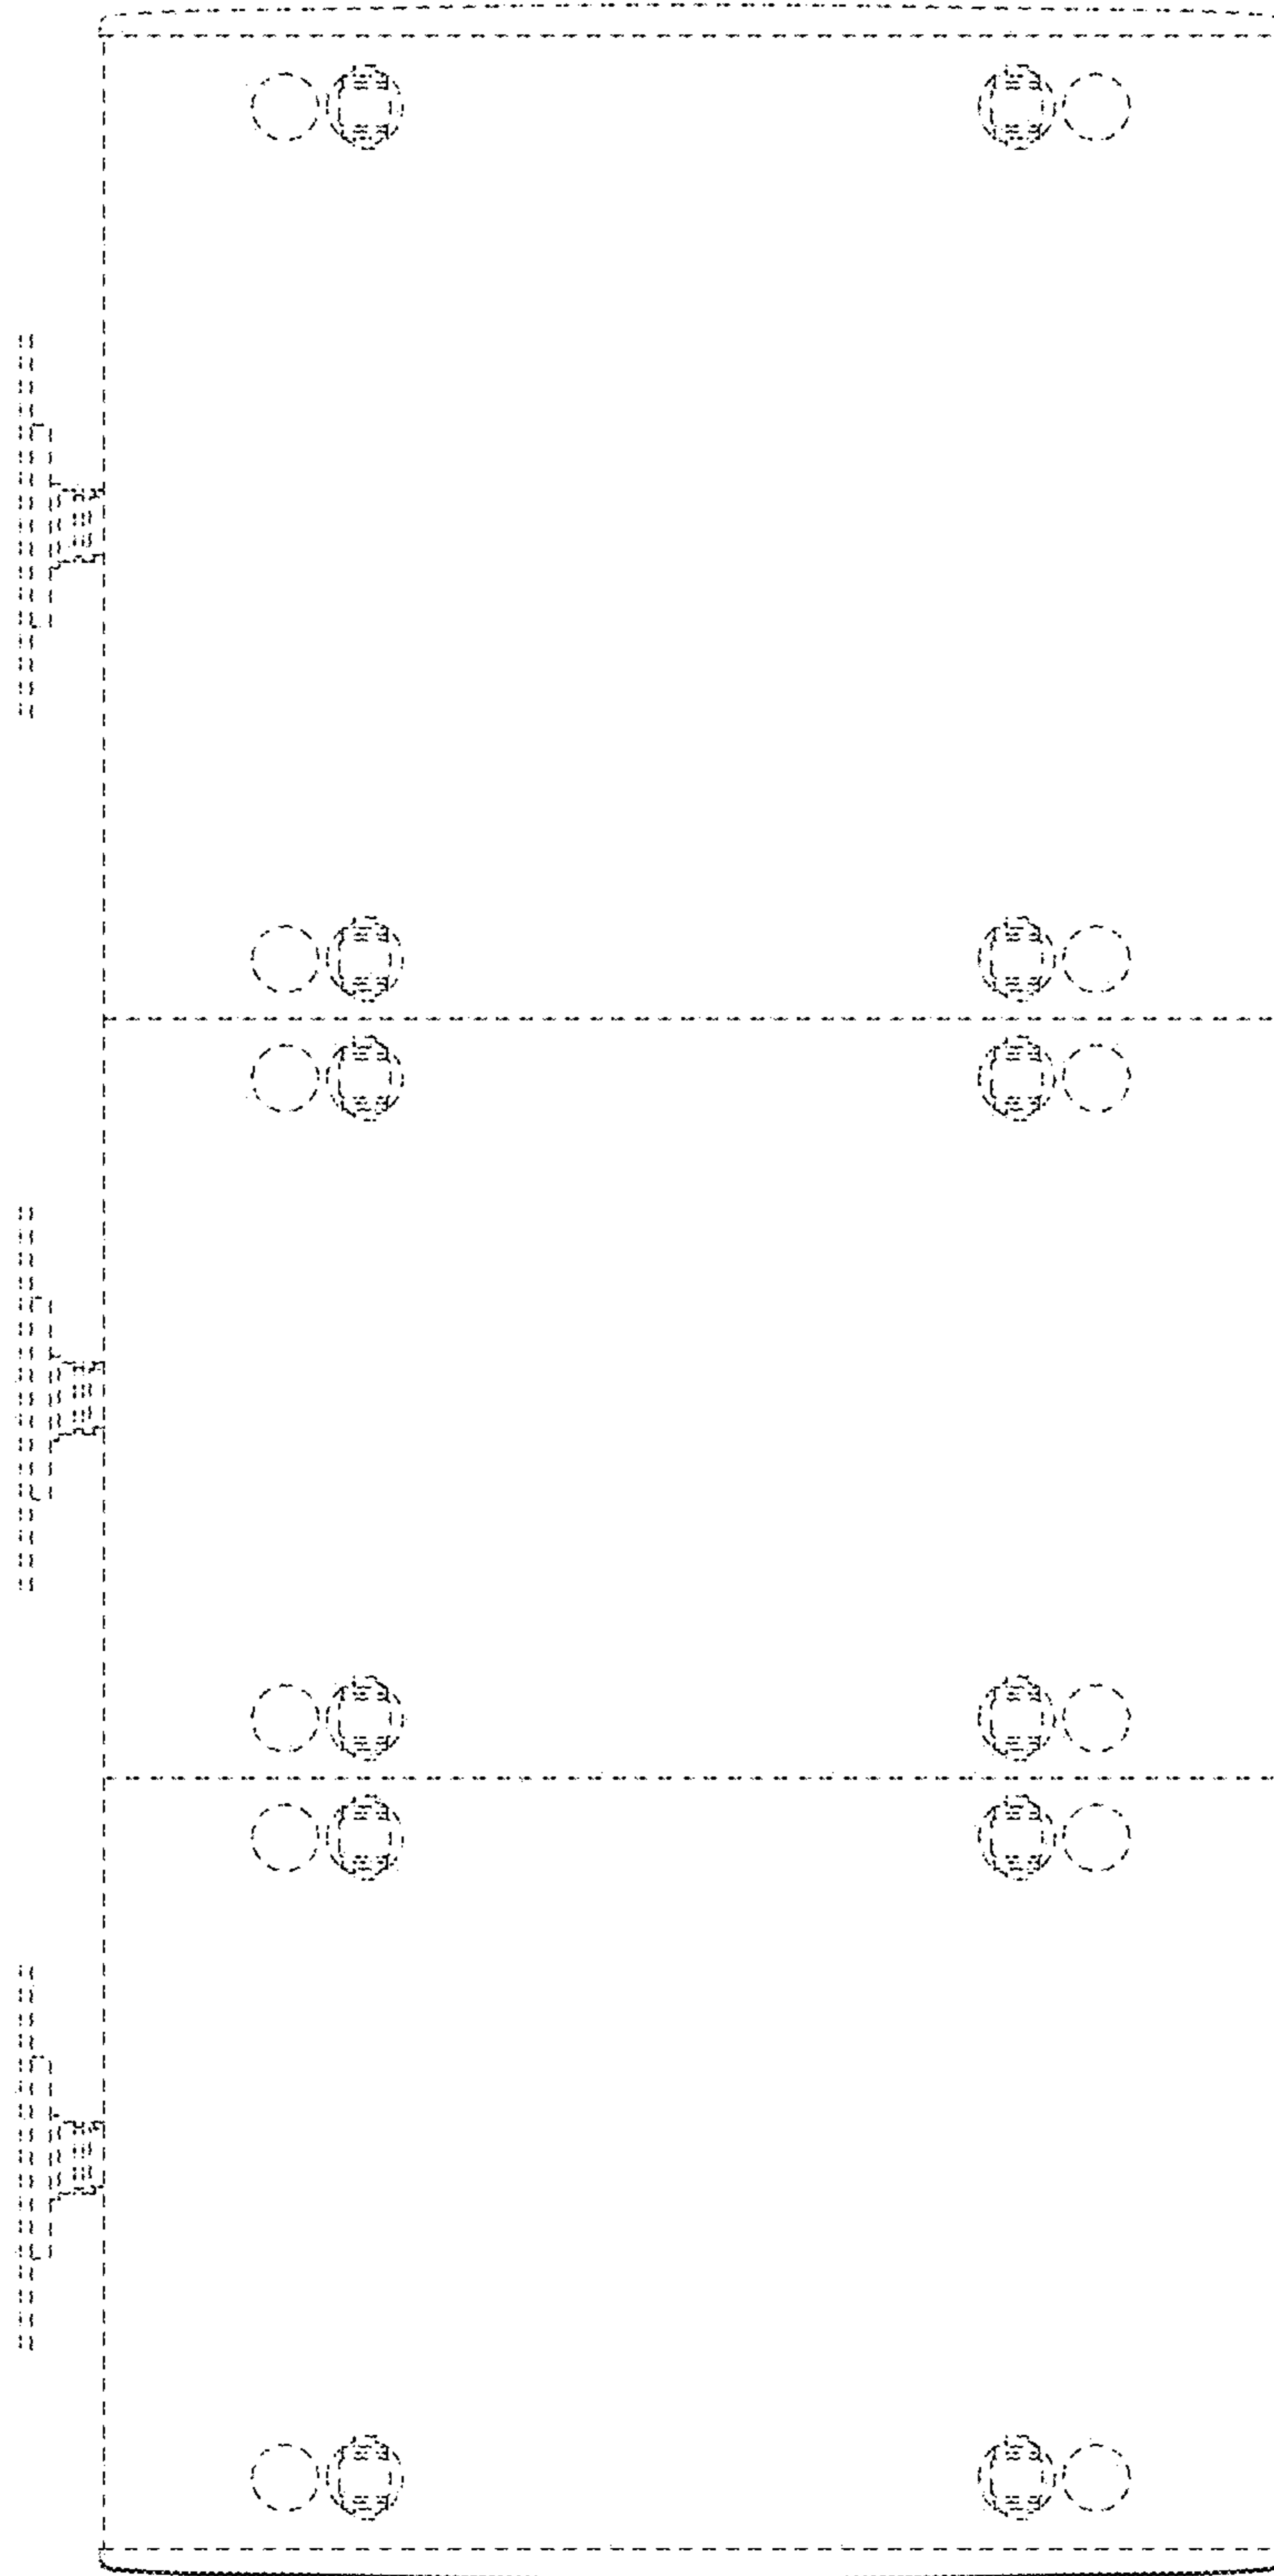


FIG. 7

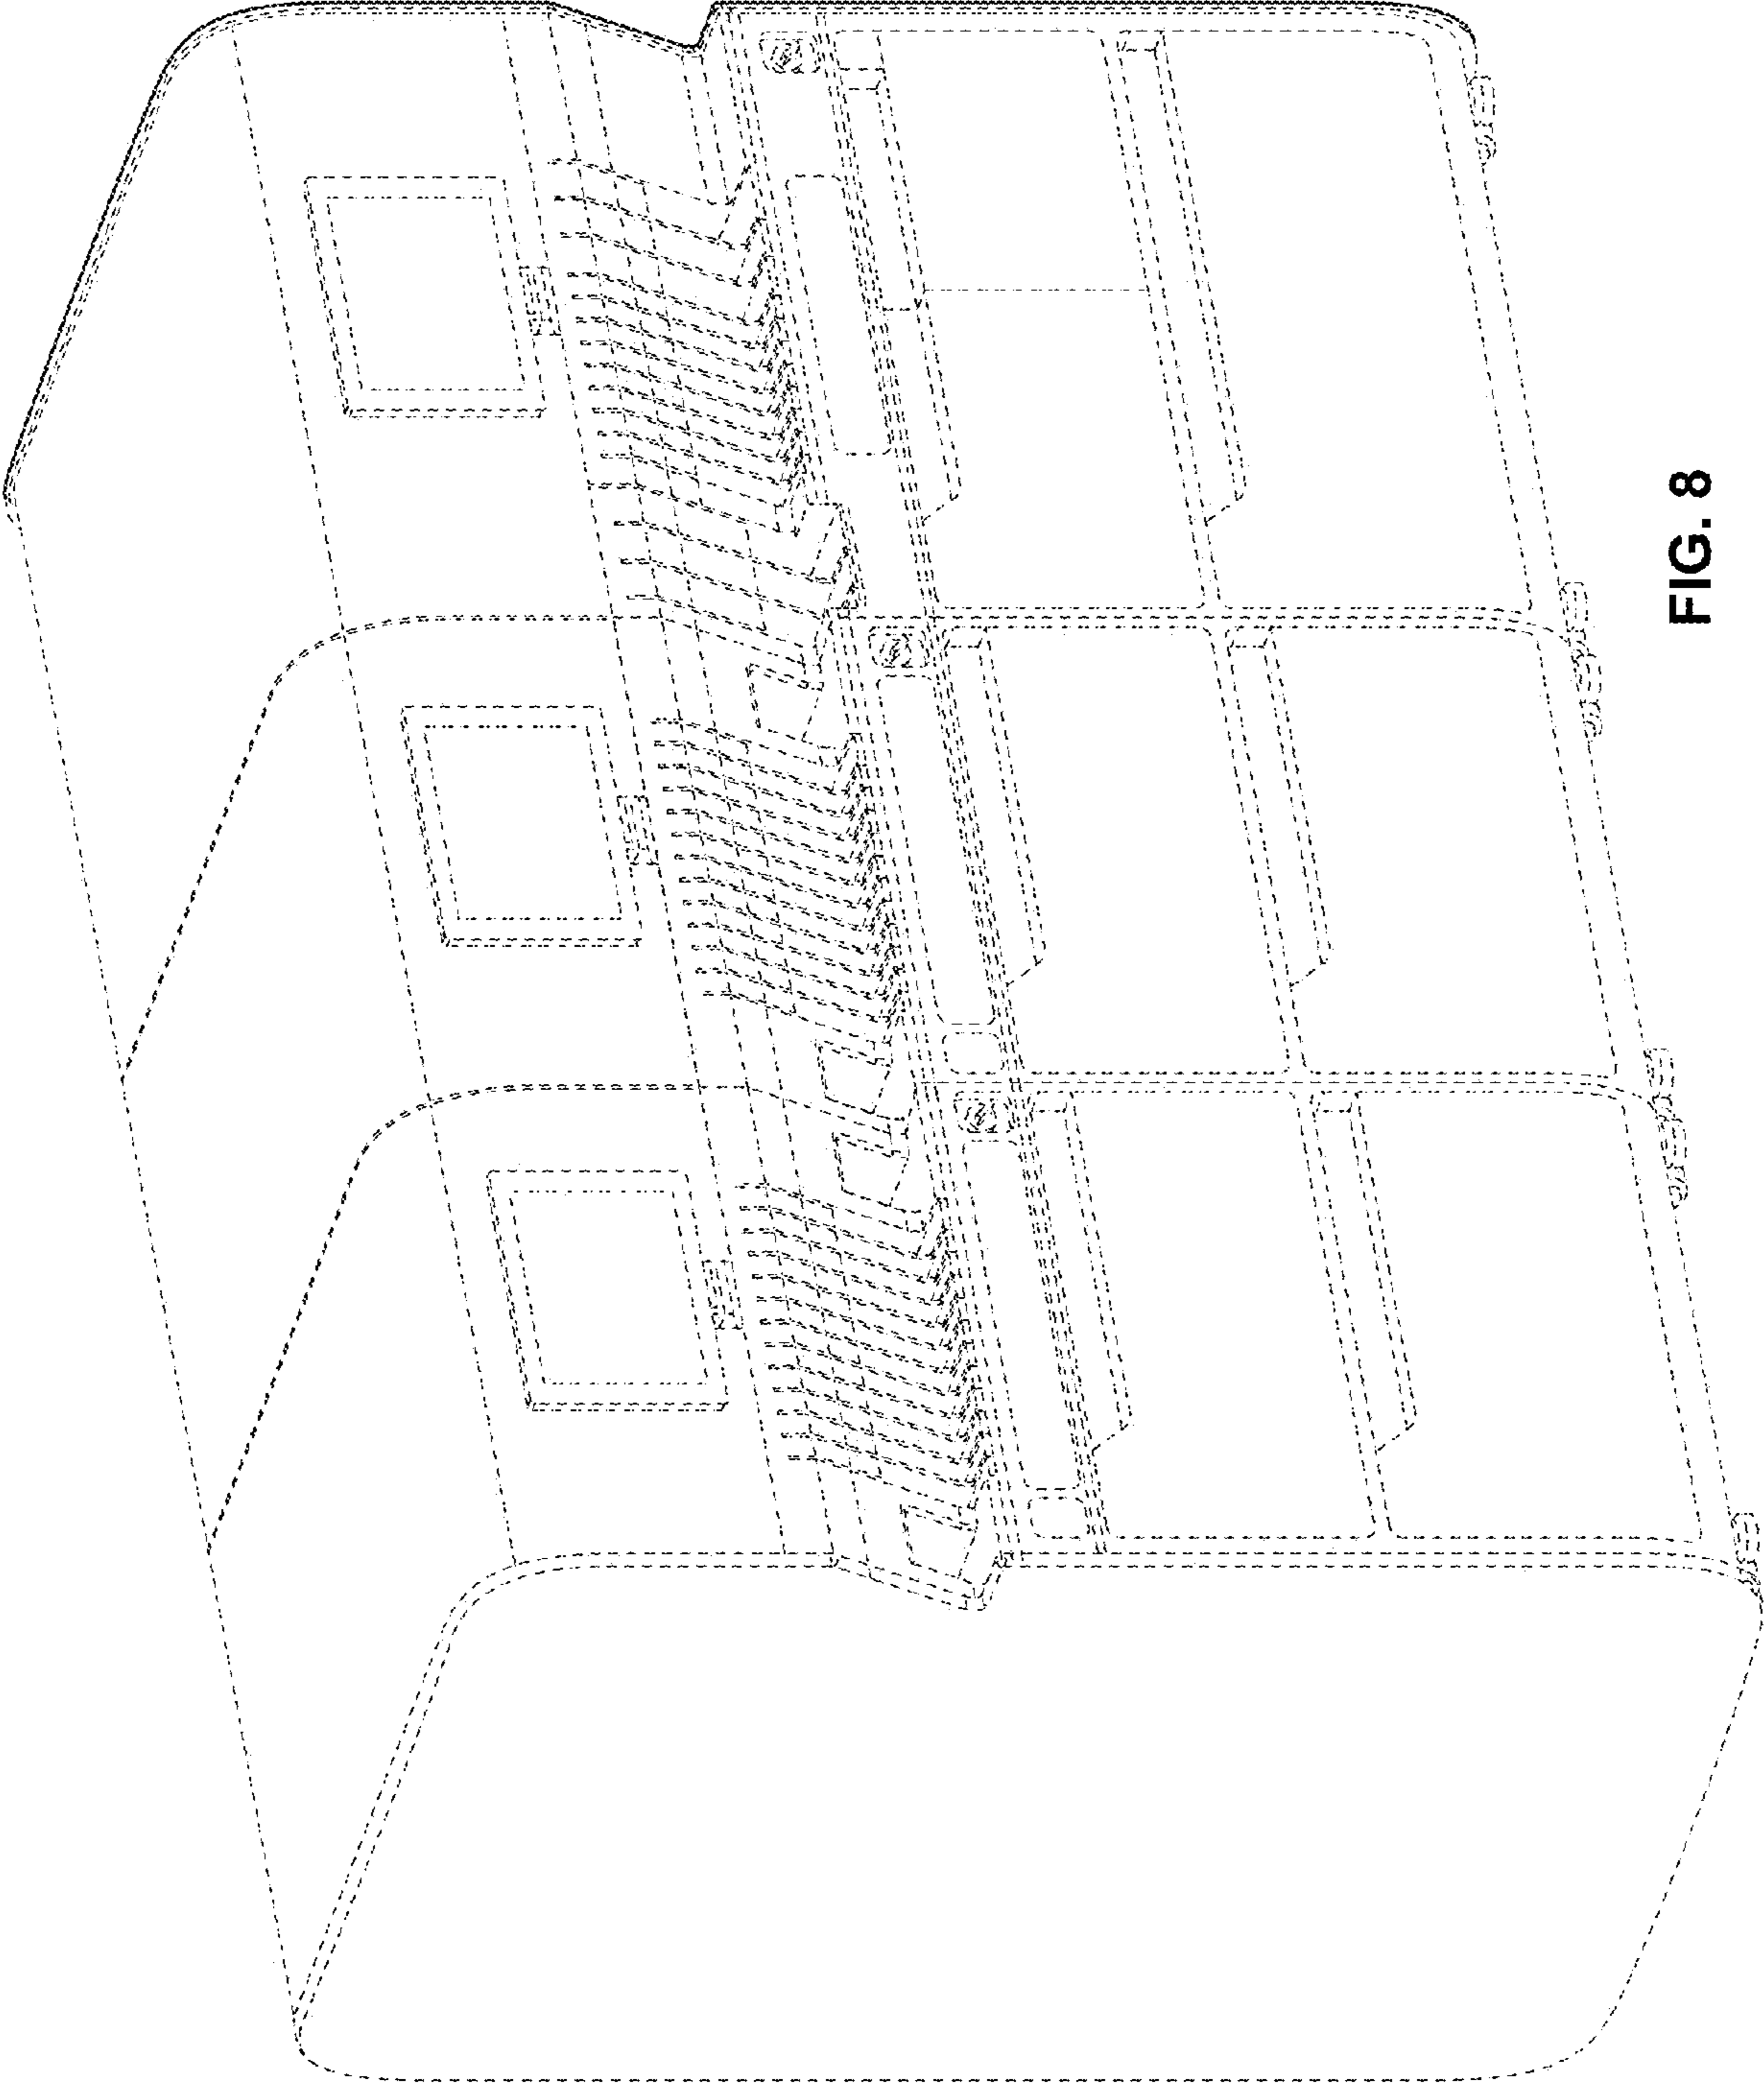


FIG. 8

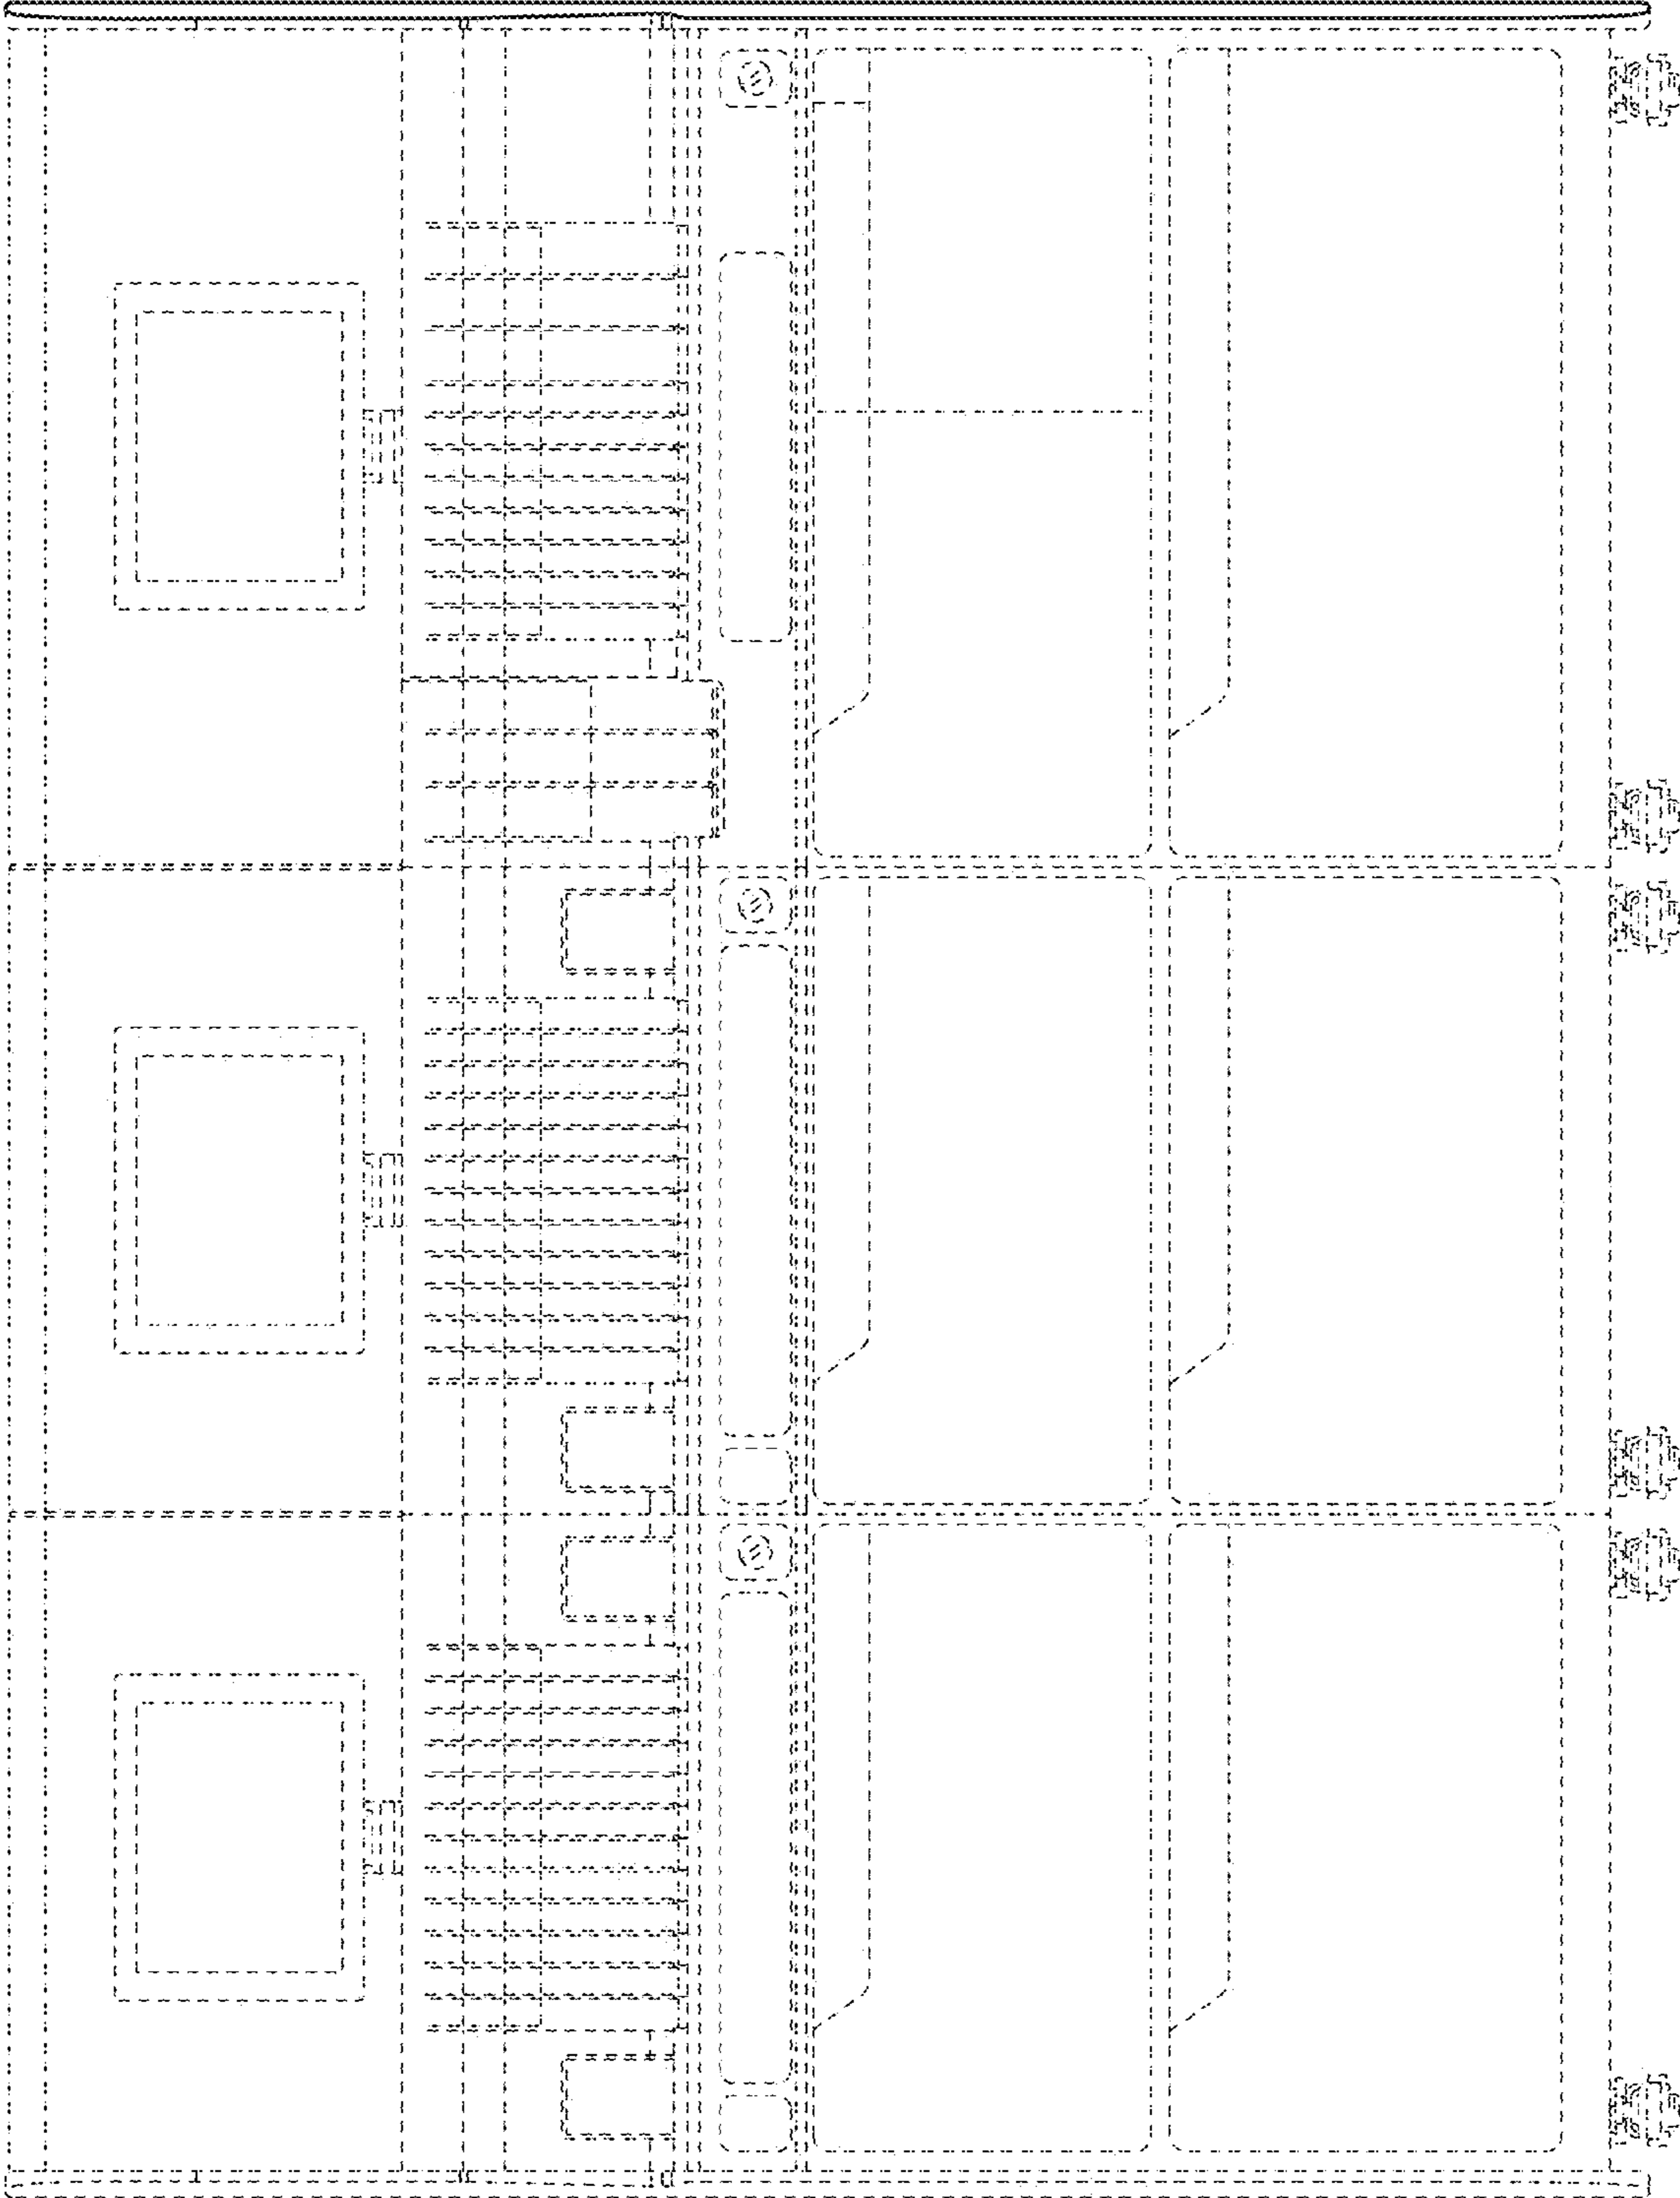


FIG. 9

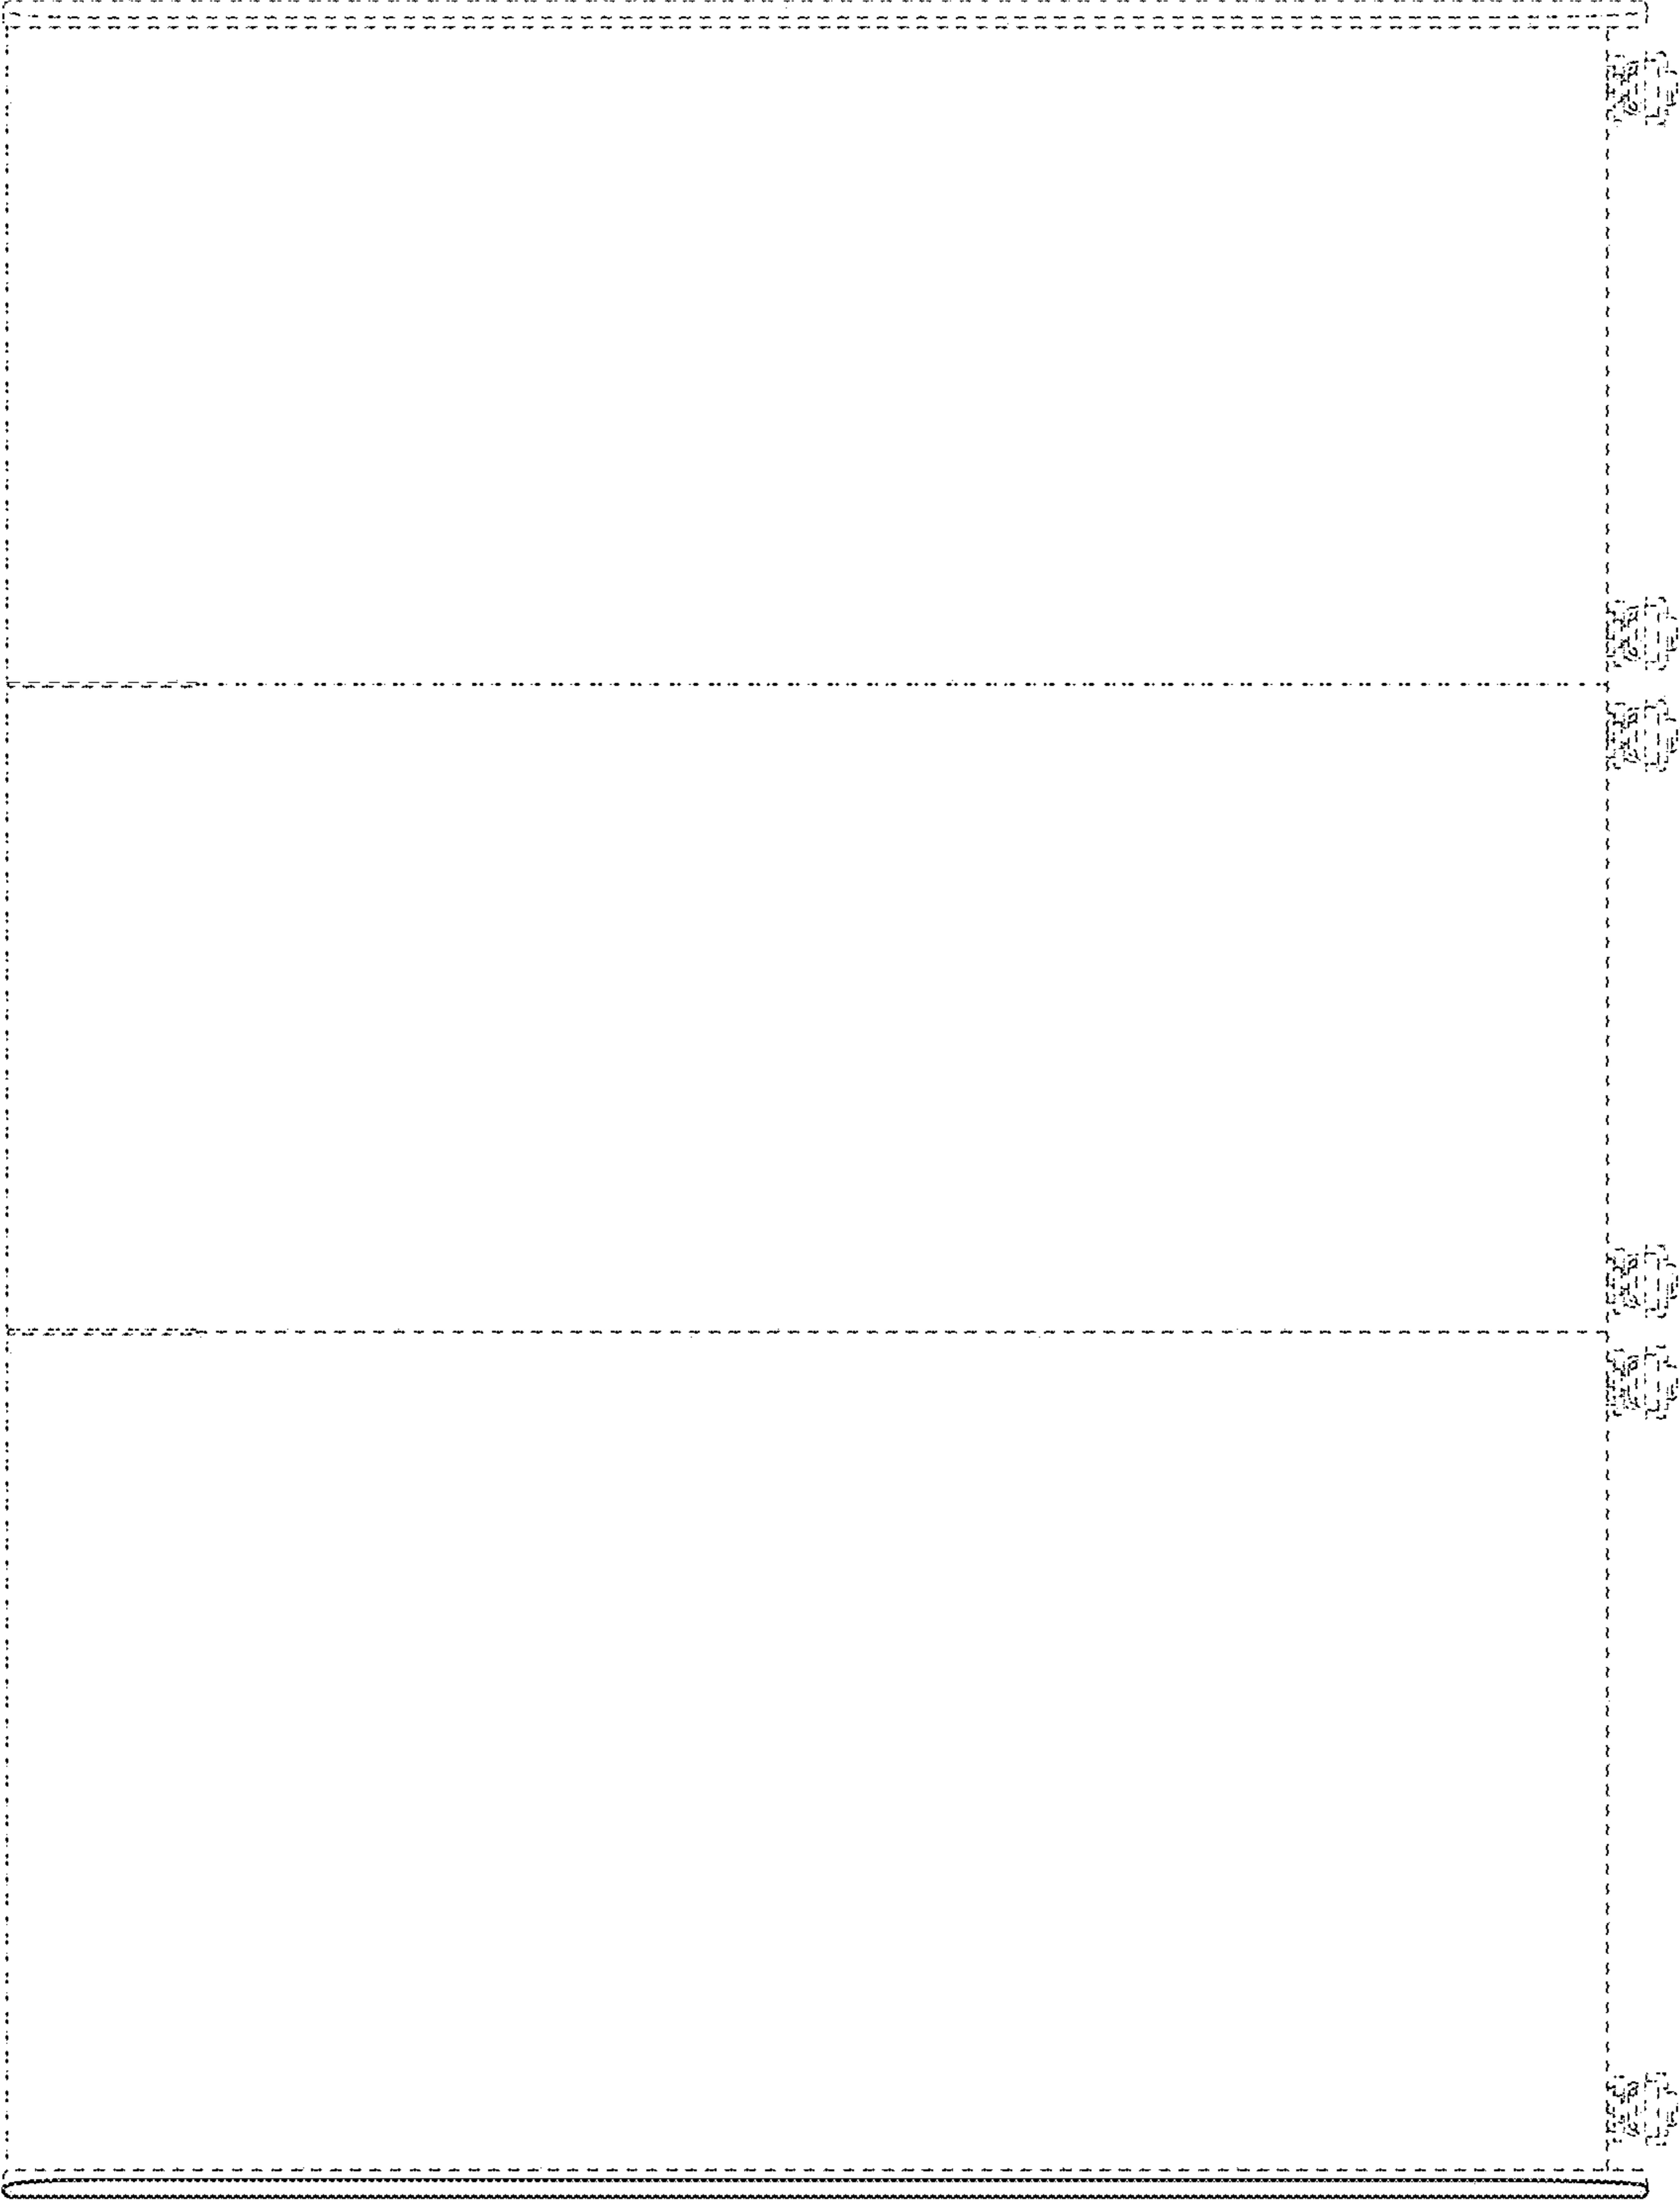


FIG. 10

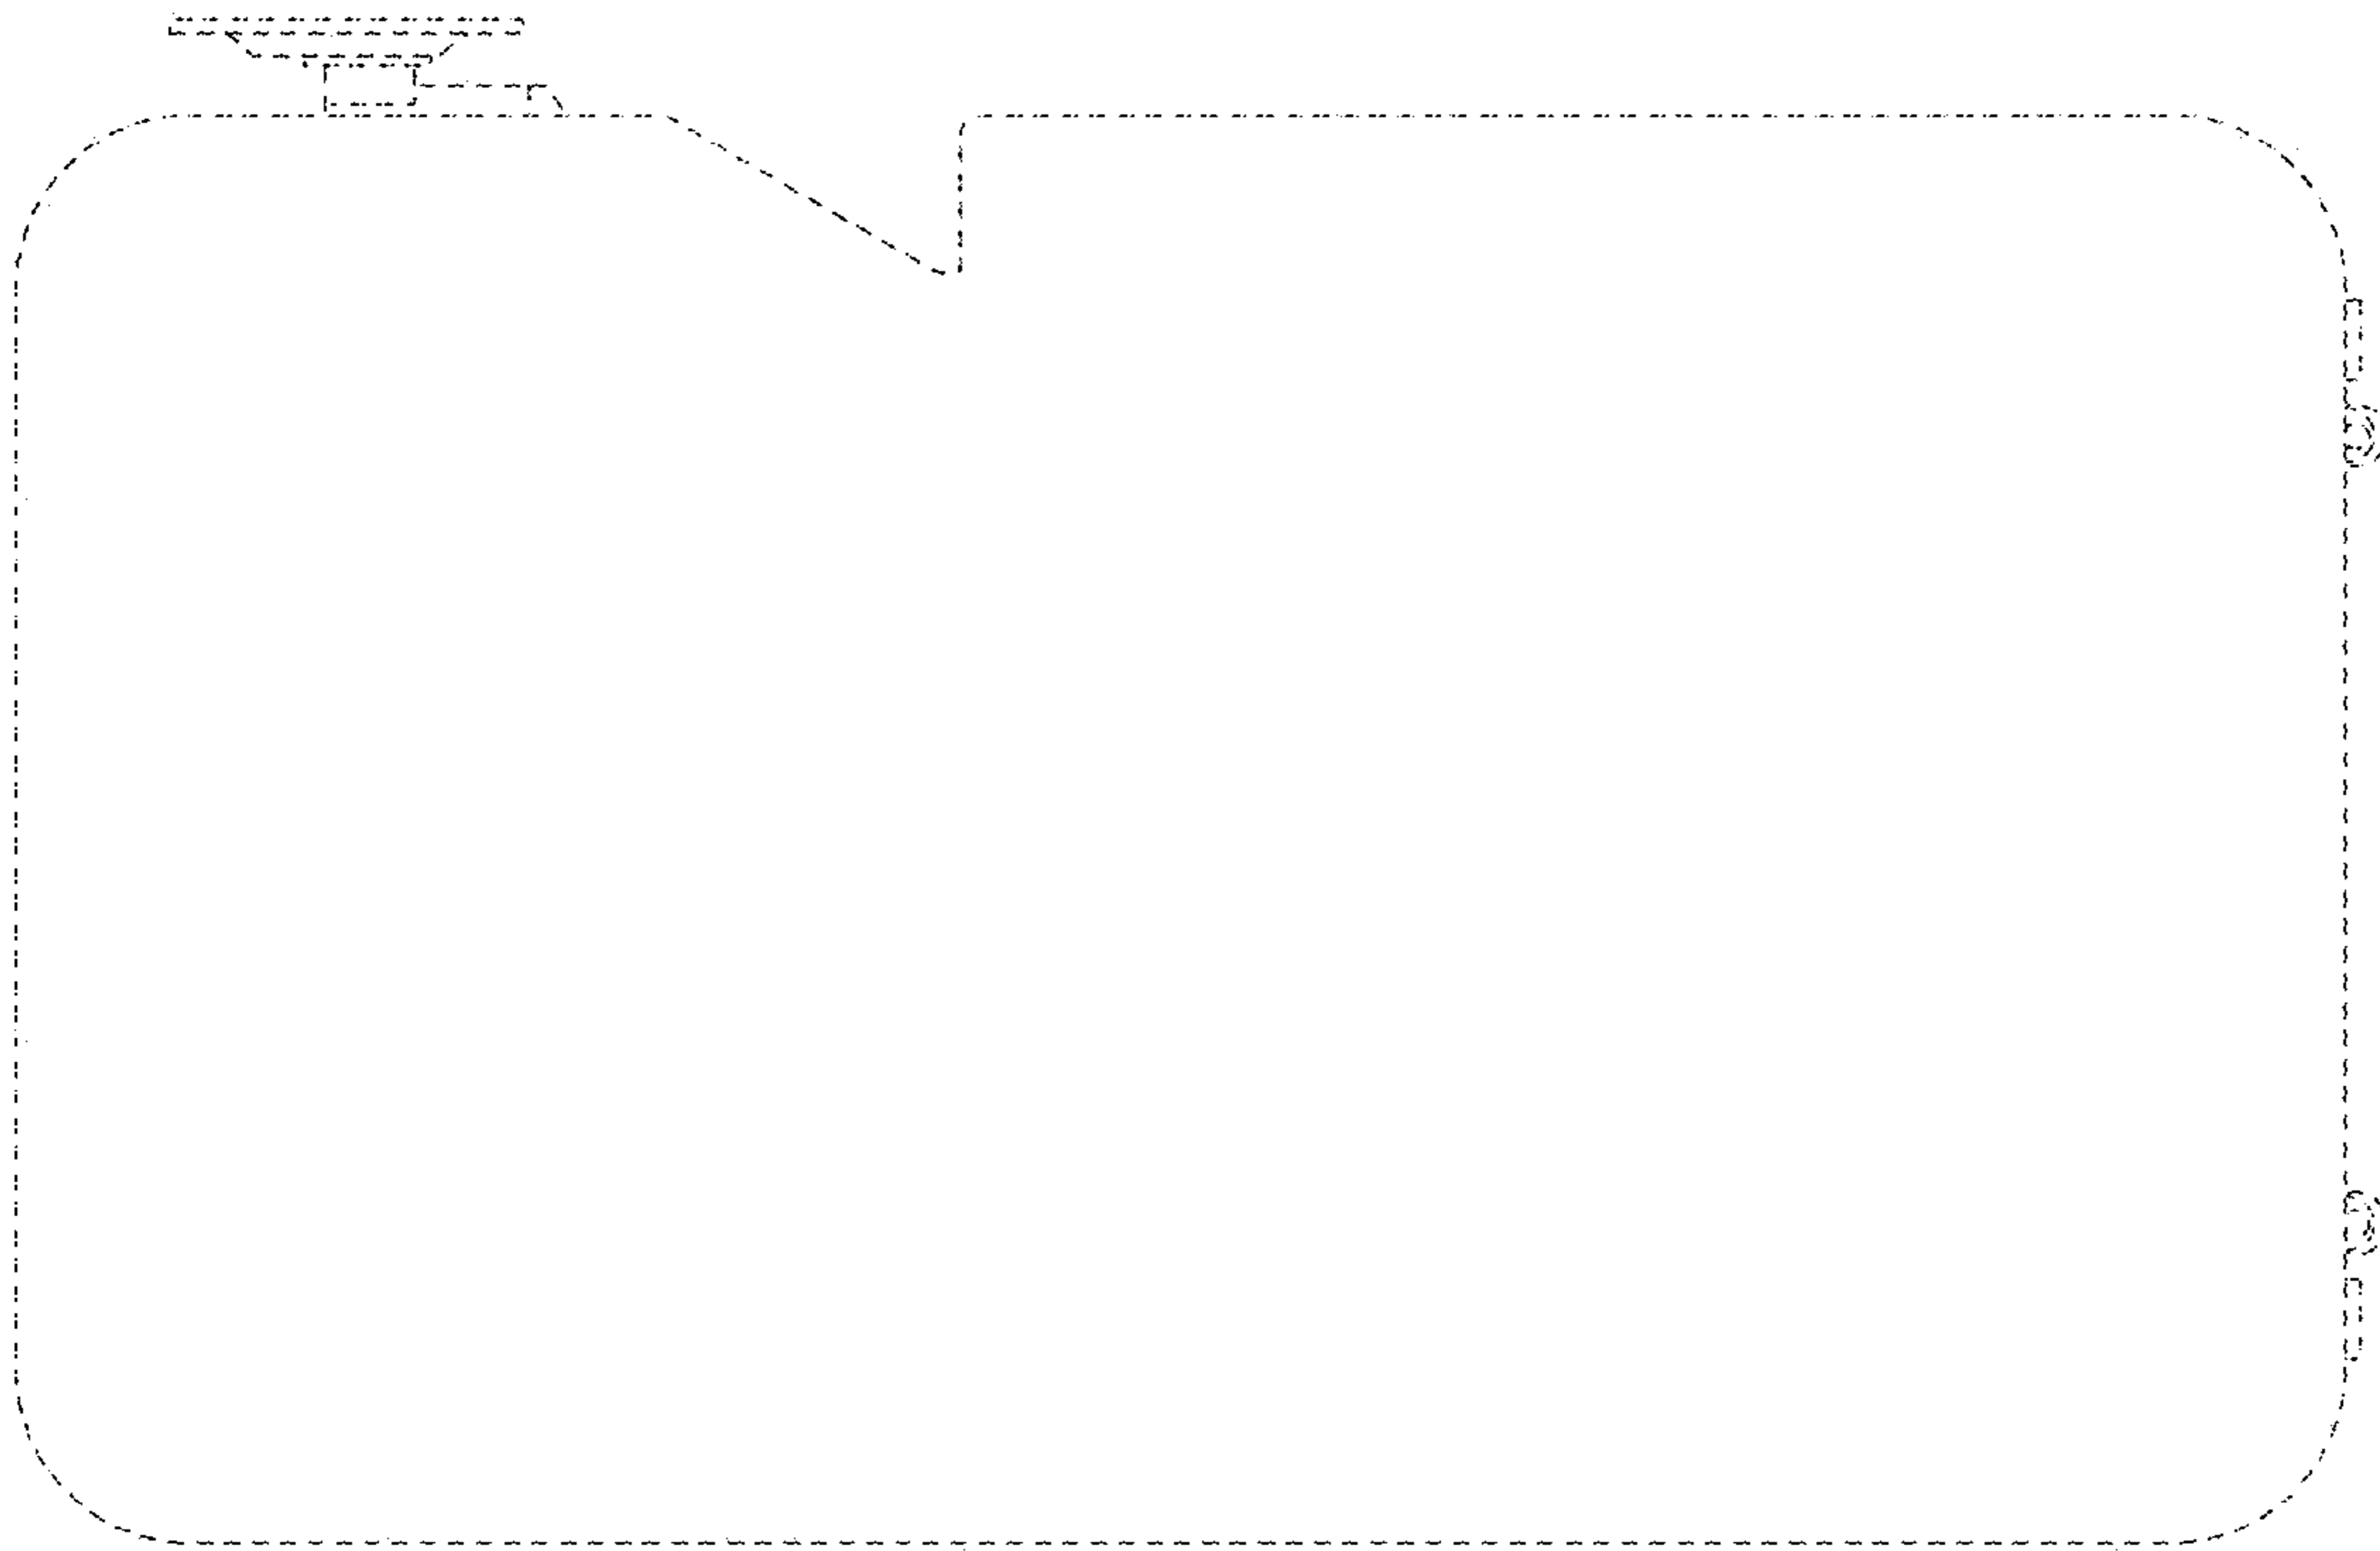


FIG. 12

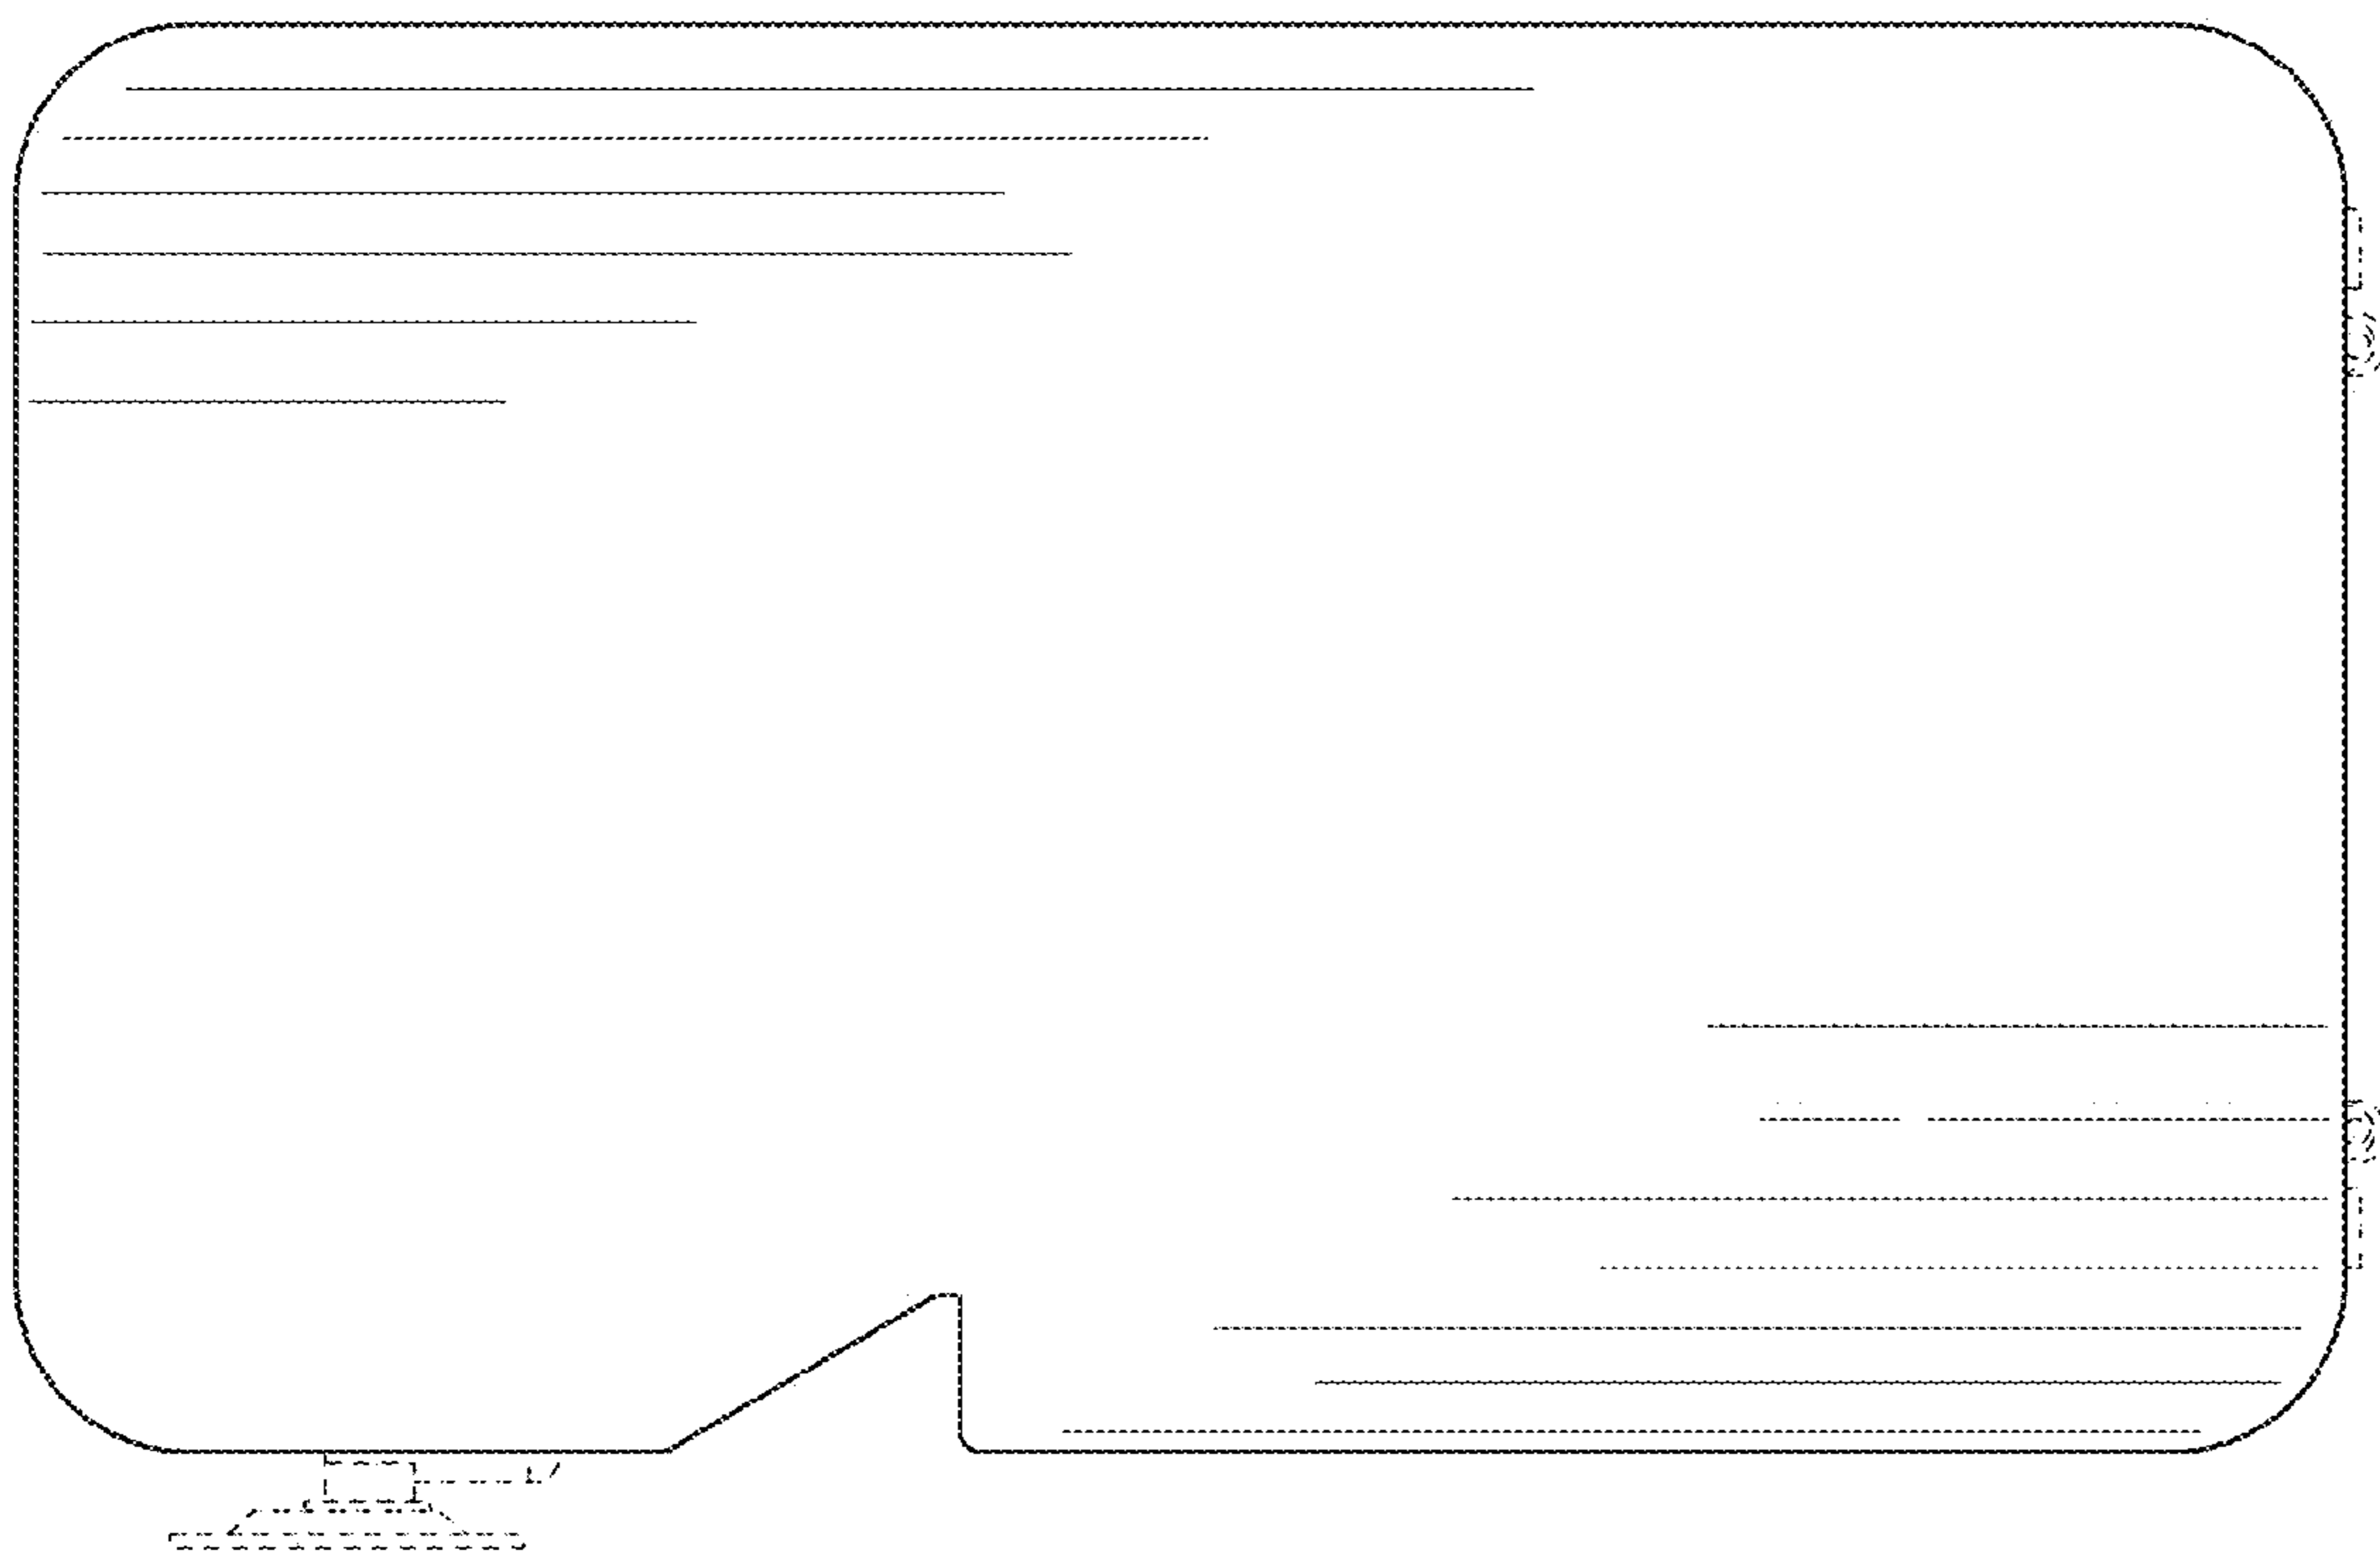


FIG. 11

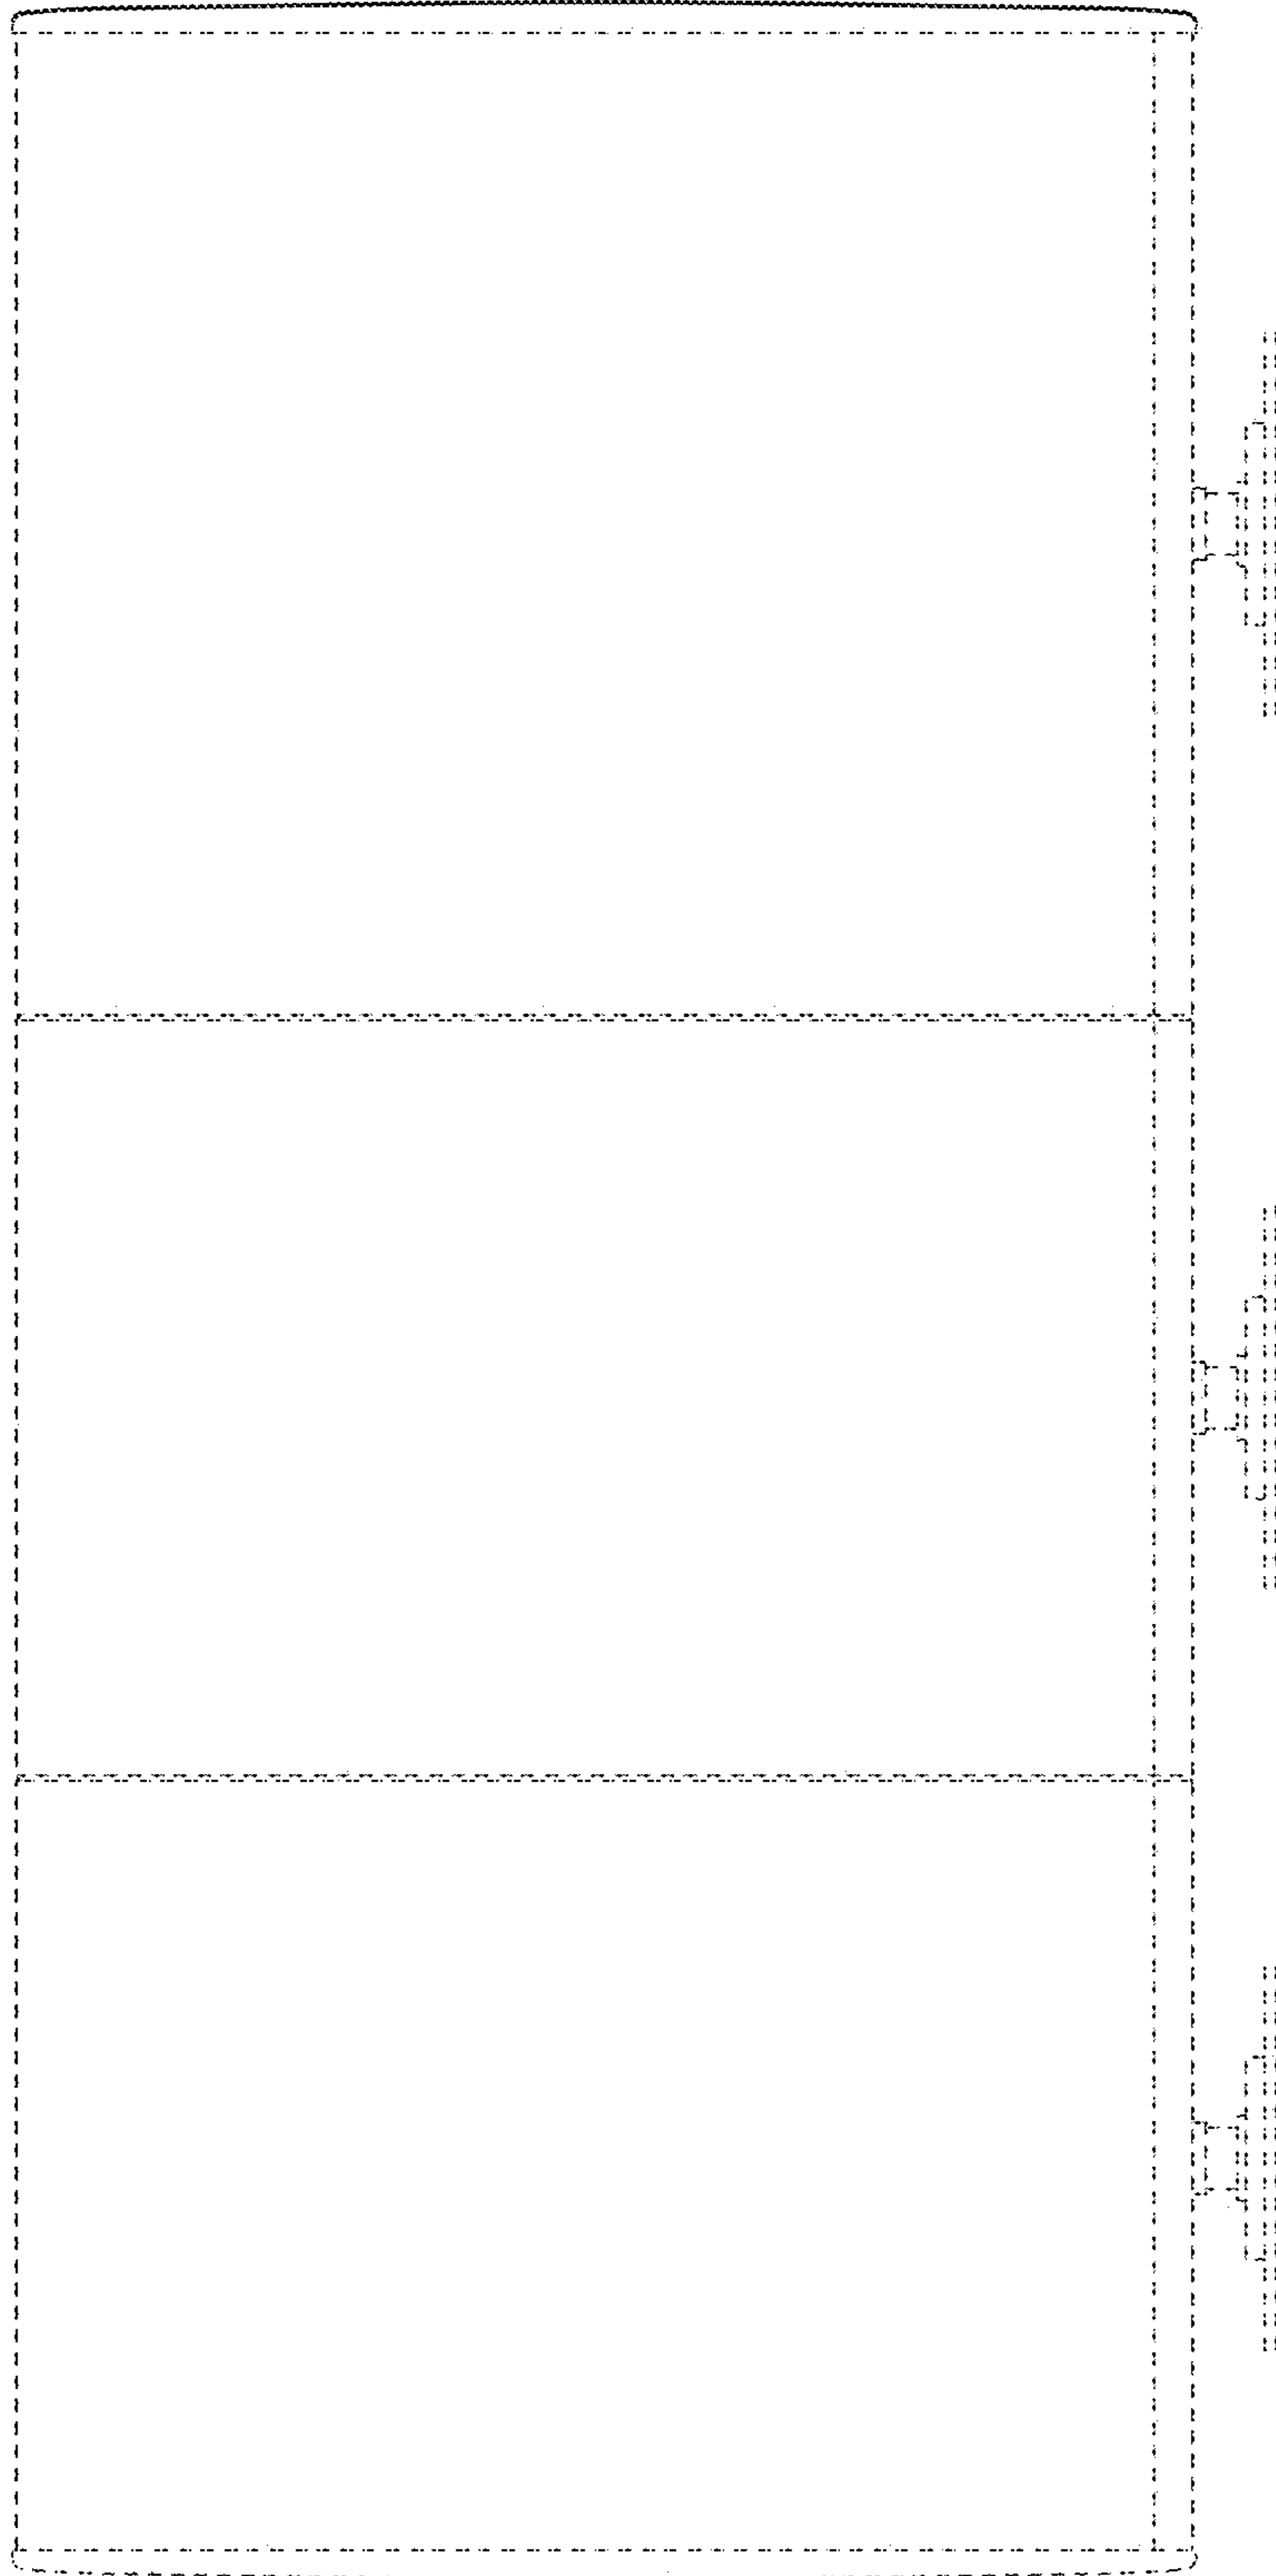


FIG. 13

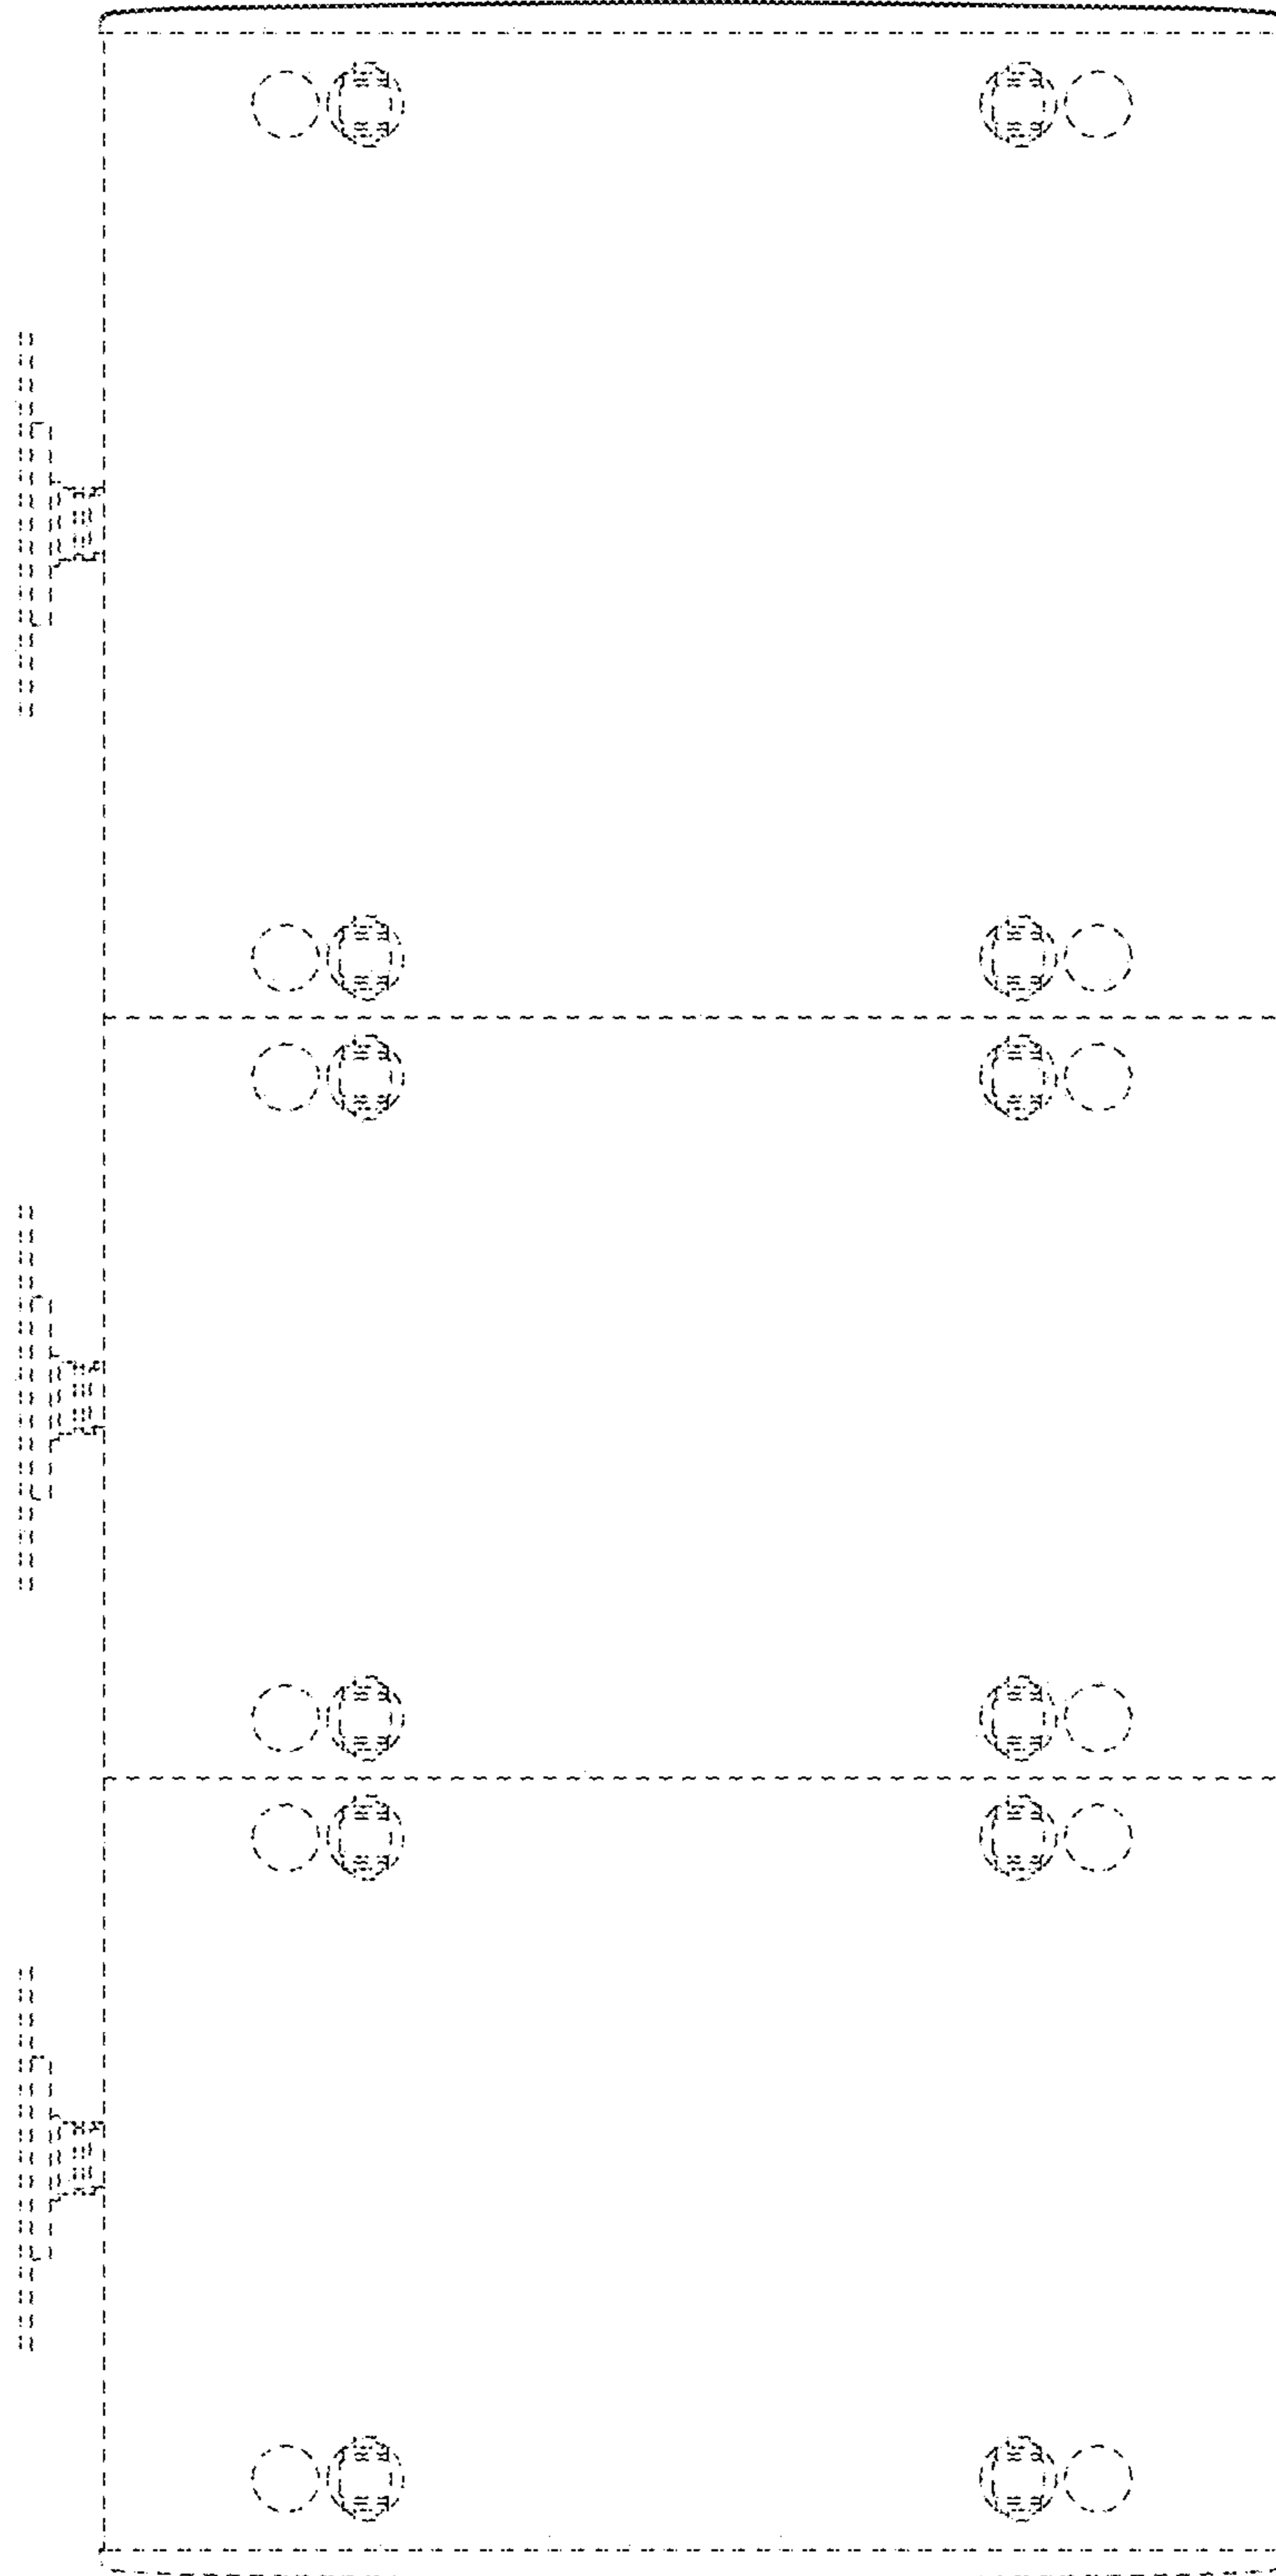


FIG. 14