



US00D944225S

(12) **United States Design Patent**
Shi

(10) **Patent No.:** **US D944,225 S**

(45) **Date of Patent:** **** Feb. 22, 2022**

(54) **LANCING DEVICE**

(71) Applicant: **SteriLance Medical (Suzhou) Inc.**,
Suzhou (CN)

(72) Inventor: **Guoping Shi**, Suzhou (CN)

(73) Assignee: **SteriLance Medical (Suzhou) Inc.**,
Suzhou (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/743,821**

(22) Filed: **Jul. 24, 2020**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D14/146**

(58) **Field of Classification Search**

USPC D28/57, 59, 62; D4/104, 120, 137, 138,
D4/100, 108, 111; D8/90-94, 107, 300,
D8/310-311, 313, 97; D24/146-147,
D24/10.5, 107, 110, 112-118, 121, 127,
D24/130, 133, 148, 152, 172-174,
D24/176-178; D19/110, 115; D7/649
CPC A61B 17/089; A61B 17/1617; A61B
17/3211; A61B 17/3417; A61B 5/1411;
A61H 39/08; A61M 2025/0246; A61M
16/04; A61M 16/0463; A61M 16/0486;
A61M 16/0484; A61M 25/0009; A61M
25/007; A61M 25/02; A61M 25/09033;
A61M 5/3286; A61M 5/343; B26B 3/00;
B26B 1/10; B26B 5/005

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D428,150 S * 7/2000 Ruf D24/146
D429,814 S * 8/2000 Lorwald D24/140
D550,363 S * 9/2007 Hannant D24/186
D560,805 S * 1/2008 Young D24/146
D617,904 S * 6/2010 Lai D24/146

D648,024 S * 11/2011 Harkin D24/146
8,313,470 B2 * 11/2012 Abry A61M 5/3202
604/198
9,149,221 B2 * 10/2015 Kan A61B 5/150412
D768,856 S * 10/2016 Harkin D24/147
(Continued)

FOREIGN PATENT DOCUMENTS

FR 008034243-0002 * 10/2020

OTHER PUBLICATIONS

GlucoGorx Adjustable Lancing Device, first available Oct. 14, 2020, amazon.com, [online], [site visited Sep. 2, 2021], Available from internet URL: https://www.amazon.com/GlucoGorx-Adjustable-Lancing-Ejector-Monitoring/dp/B08L6YY492/ref=pd_sbs_14/131-4543789-4001142?pd_rd_w=Qyauw%E2%80%A6 (Year: 2020).*
(Continued)

Primary Examiner — Samantha Q Lawrence
Assistant Examiner — Holly M Rodriguez
(74) *Attorney, Agent, or Firm* — Banner & Witcoff, Ltd.

(57) **CLAIM**


The ornamental design for a lancing device, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, right perspective view of a lancing device showing our new design;
FIG. 2 is a front, bottom, right perspective view thereof;
FIG. 3 is a front elevation view thereof;
FIG. 4 is a rear elevation view thereof;
FIG. 5 is a left side view thereof;
FIG. 6 is a right side view thereof;
FIG. 7 is a top view thereof; and,
FIG. 8 is a bottom view thereof.

The broken lines in the drawings are for the purpose of illustrating unclaimed portions of the lancing device and form no part of the claimed design.

1 Claim, 8 Drawing Sheets

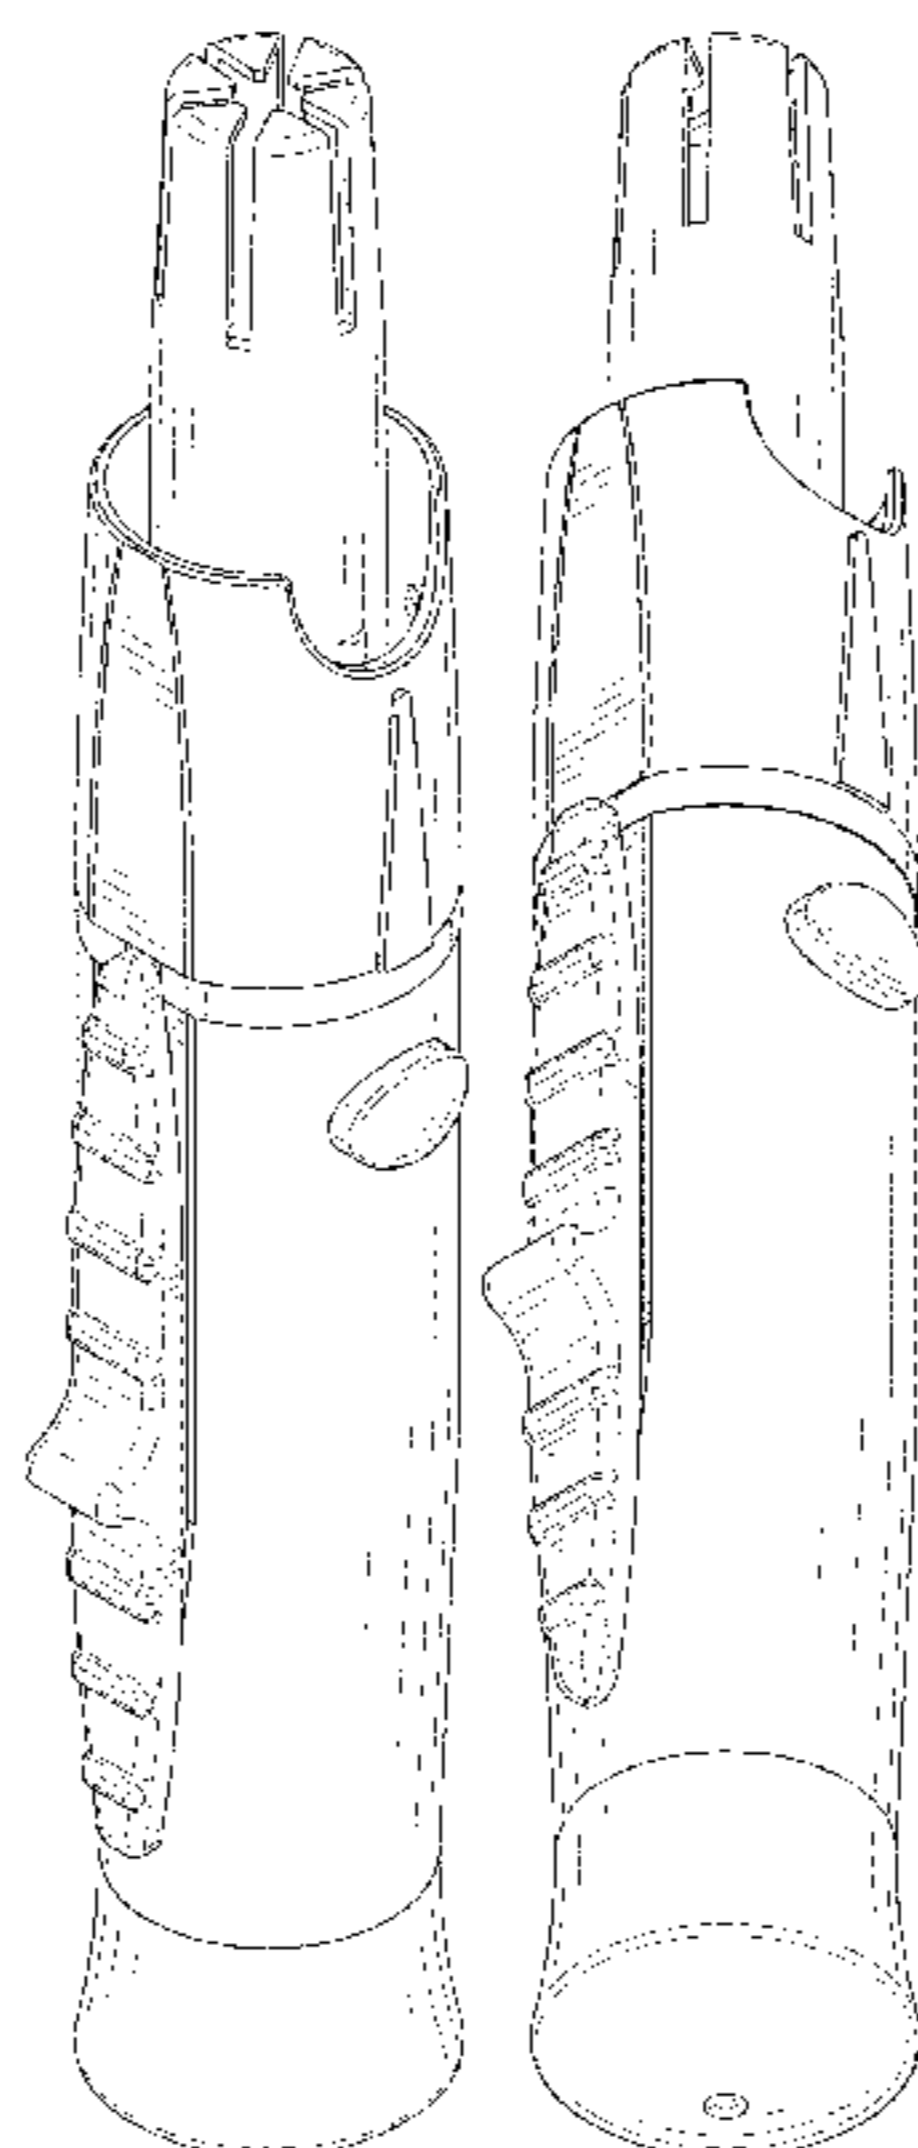

(56)

References Cited

U.S. PATENT DOCUMENTS

9,943,649 B2 * 4/2018 Shang A61M 5/31566
10,010,283 B2 * 7/2018 Volkmuth A61B 5/15113
D917,064 S * 4/2021 Ribeiro D24/217
2015/0224259 A1 * 8/2015 Giambattista A61M 5/3146
604/89
2016/0106929 A1 * 4/2016 Fournier A61M 5/3204
604/192
2016/0129195 A1 * 5/2016 Jennings A61M 5/31586
604/198
2017/0000517 A1 * 1/2017 Lee A61B 5/1519

OTHER PUBLICATIONS

Medline MPHLANCINGPEN Medline Lancing Device, first available Oct. 18, 2014, amazon.com, [online], [site visited Sep. 2, 2021], Available from internet URL: <https://www.amazon.com/Medline-MPHLANCINGPEN-Lancing-Device/dp/B00PU0ICE6> (Year: 2014).*

Lancing Device with Ejector (LDE4) , sterilance.com, [online], [site visited Sep. 2, 2021], Available from internet URL: <http://www.sterilance.com/english/pro1/pro2/pro7/2019-06-26/111.html> (Year: 2021).*

EasyTouch Lancing Device w/Ejector, first available Feb. 17, 2012, amazon.com, [online], [site visited 9/82021], Available from internet URL: https://www.amazon.com/EasyTouch-Lancing-Device-Ejector-Box/dp/B007AIPK1Y/ref=pd_sbs_5/131-4543789-4001142?pd_rd_w=ULPaV&pf_rd_p=0f56f70f-21e6-4d11-bb4a-bcdb92 (Year: 2012).*

* cited by examiner

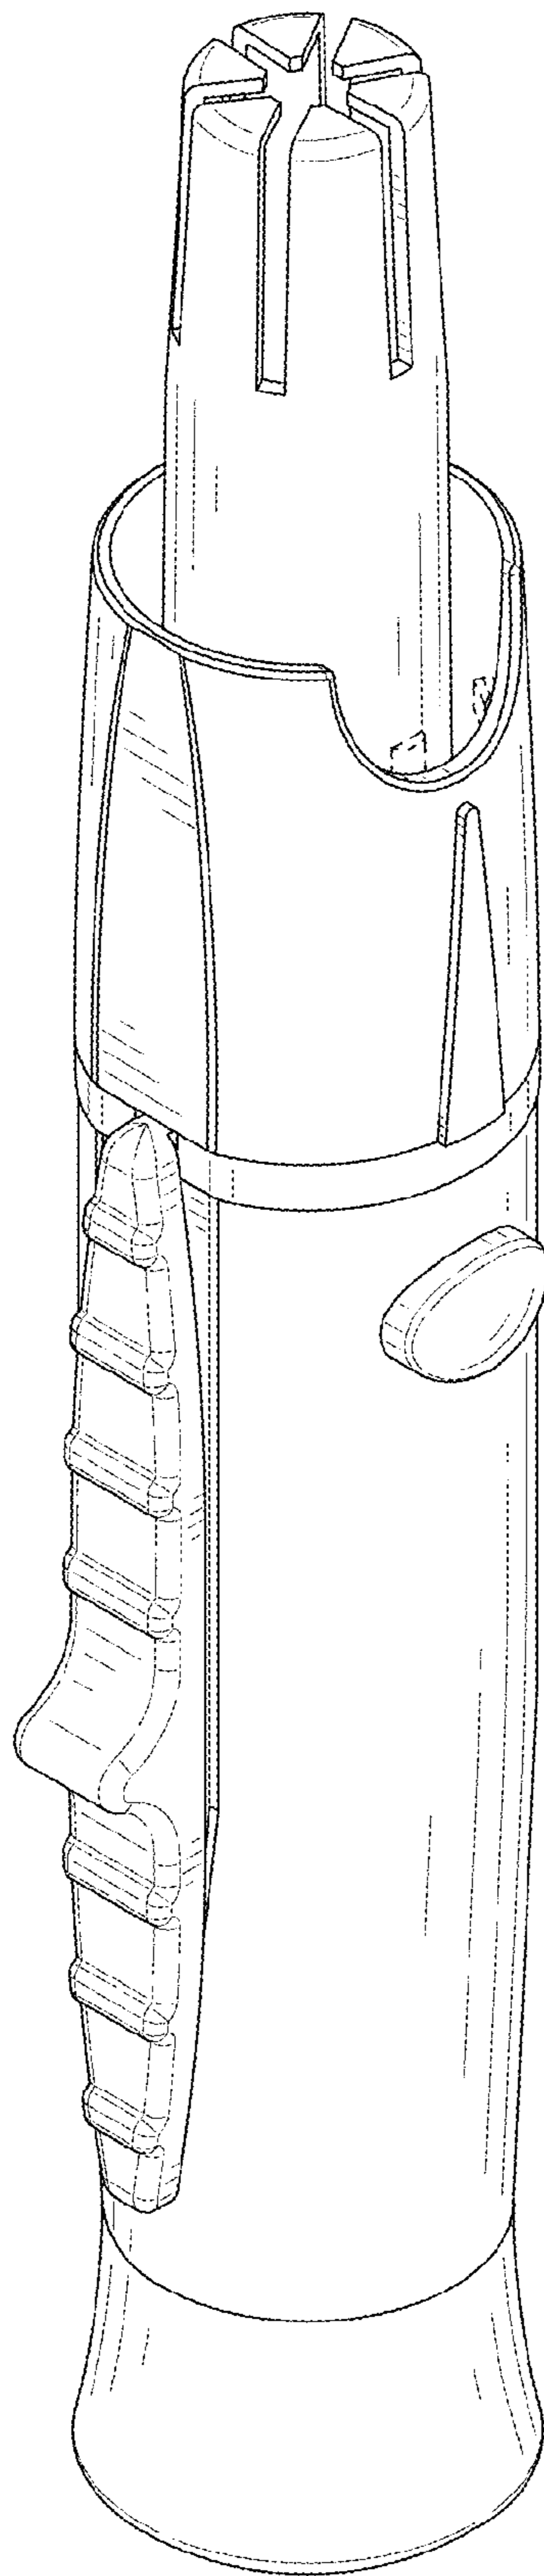


FIG. 1

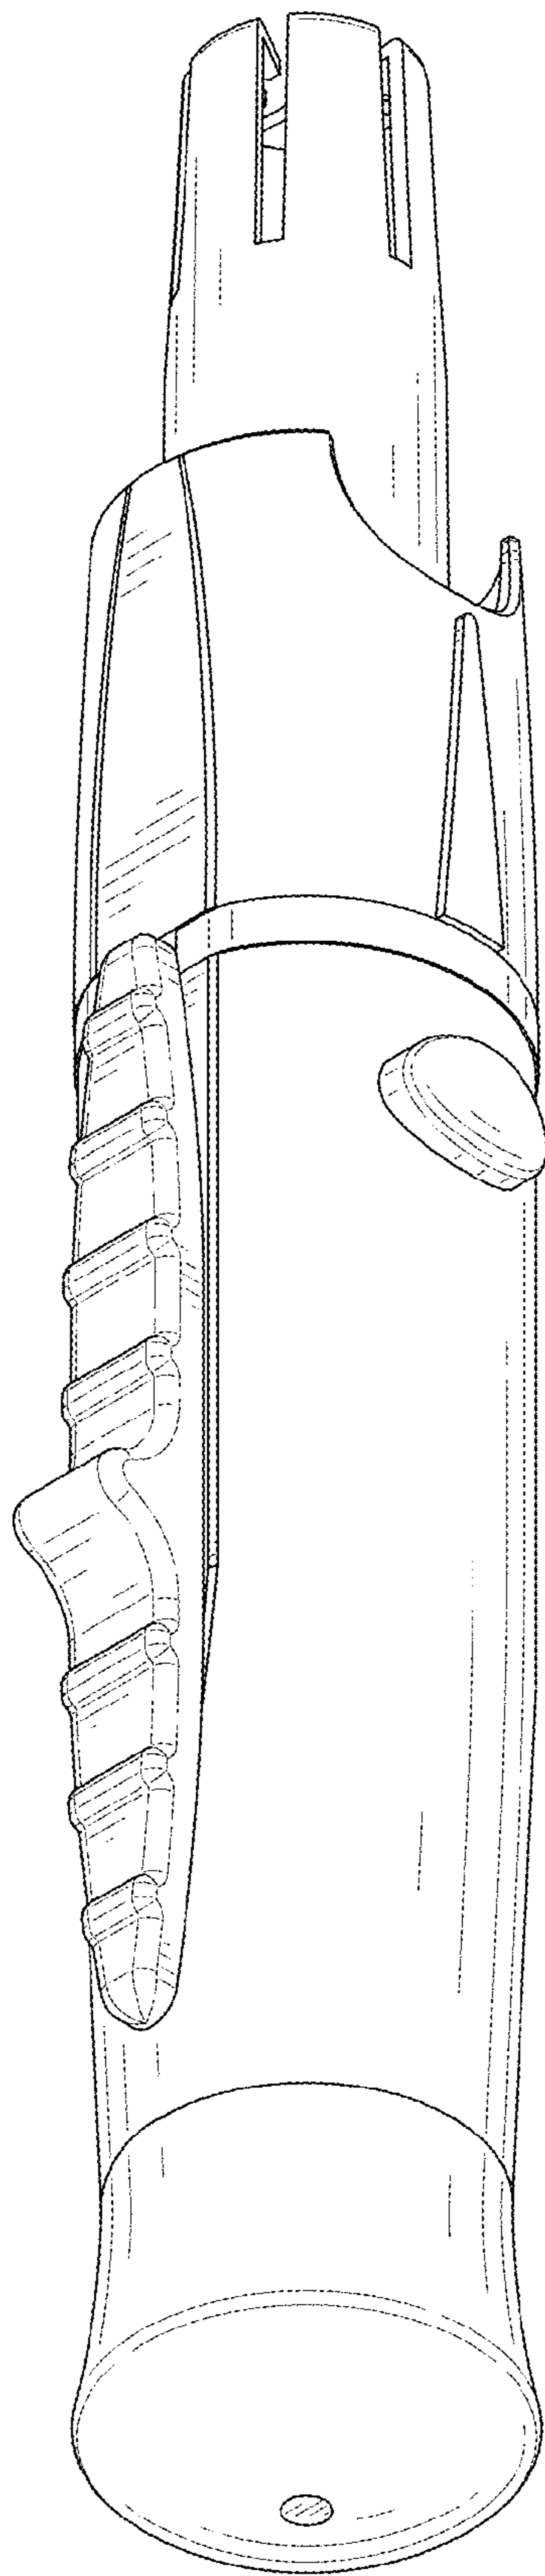


FIG. 2

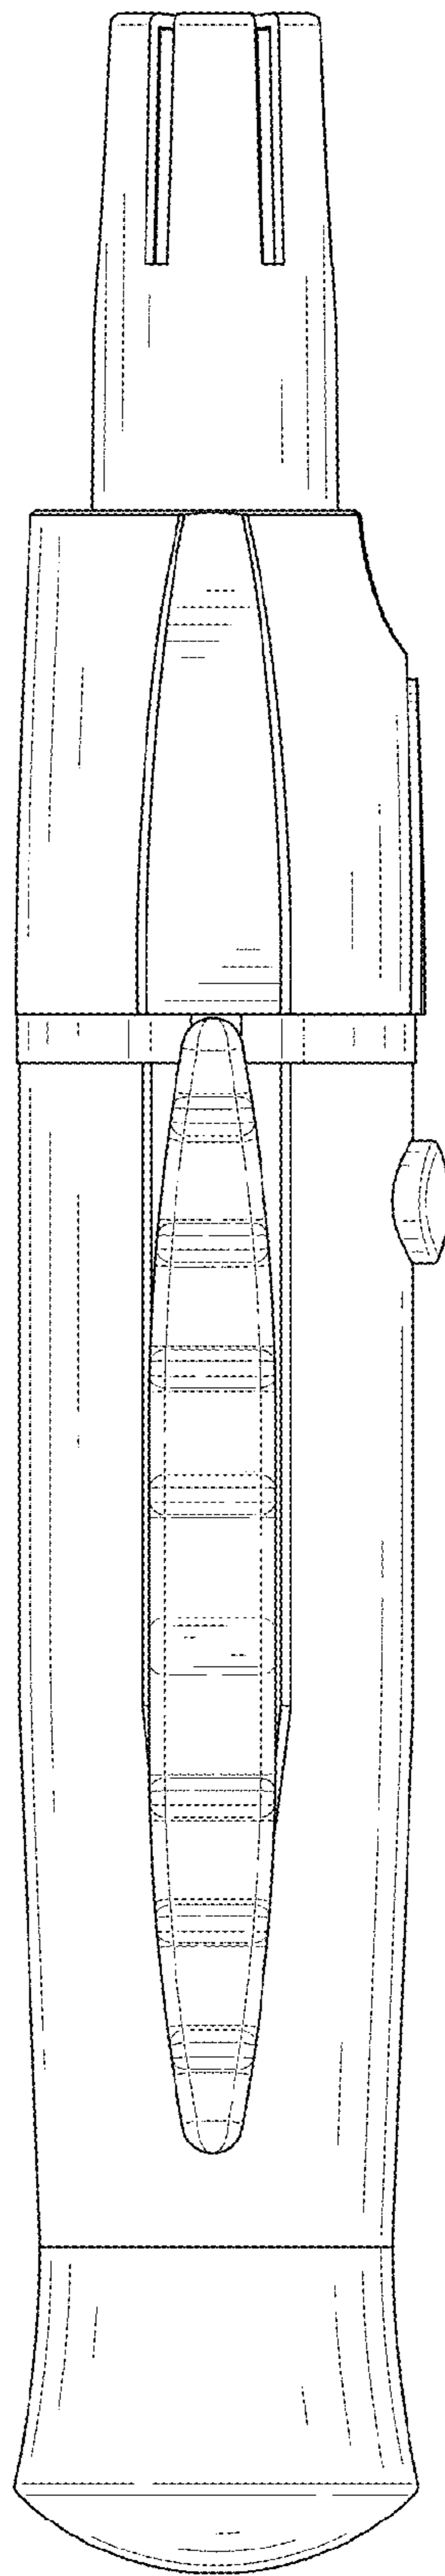


FIG. 3

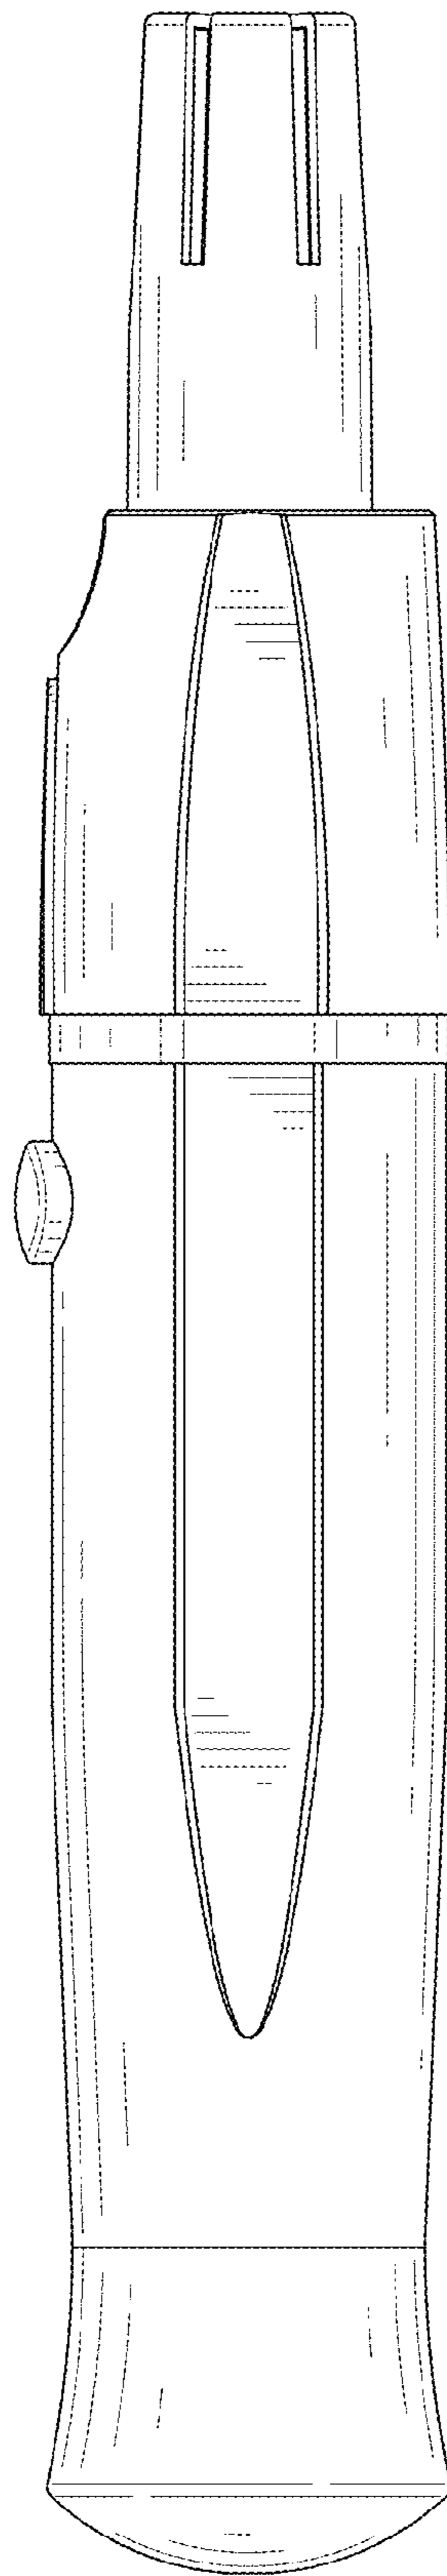


FIG. 4

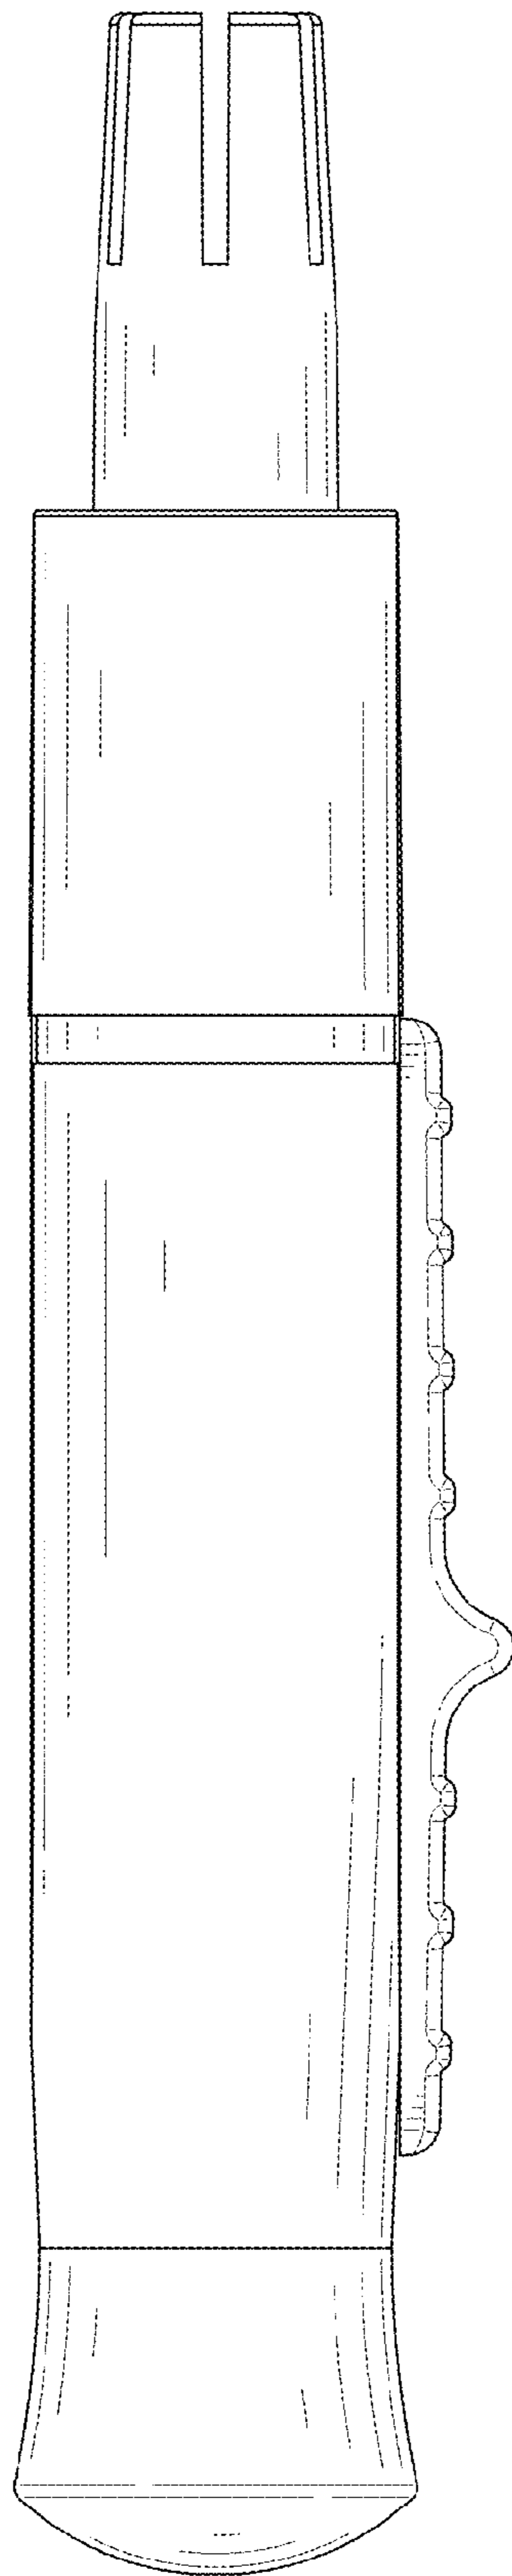


FIG. 5

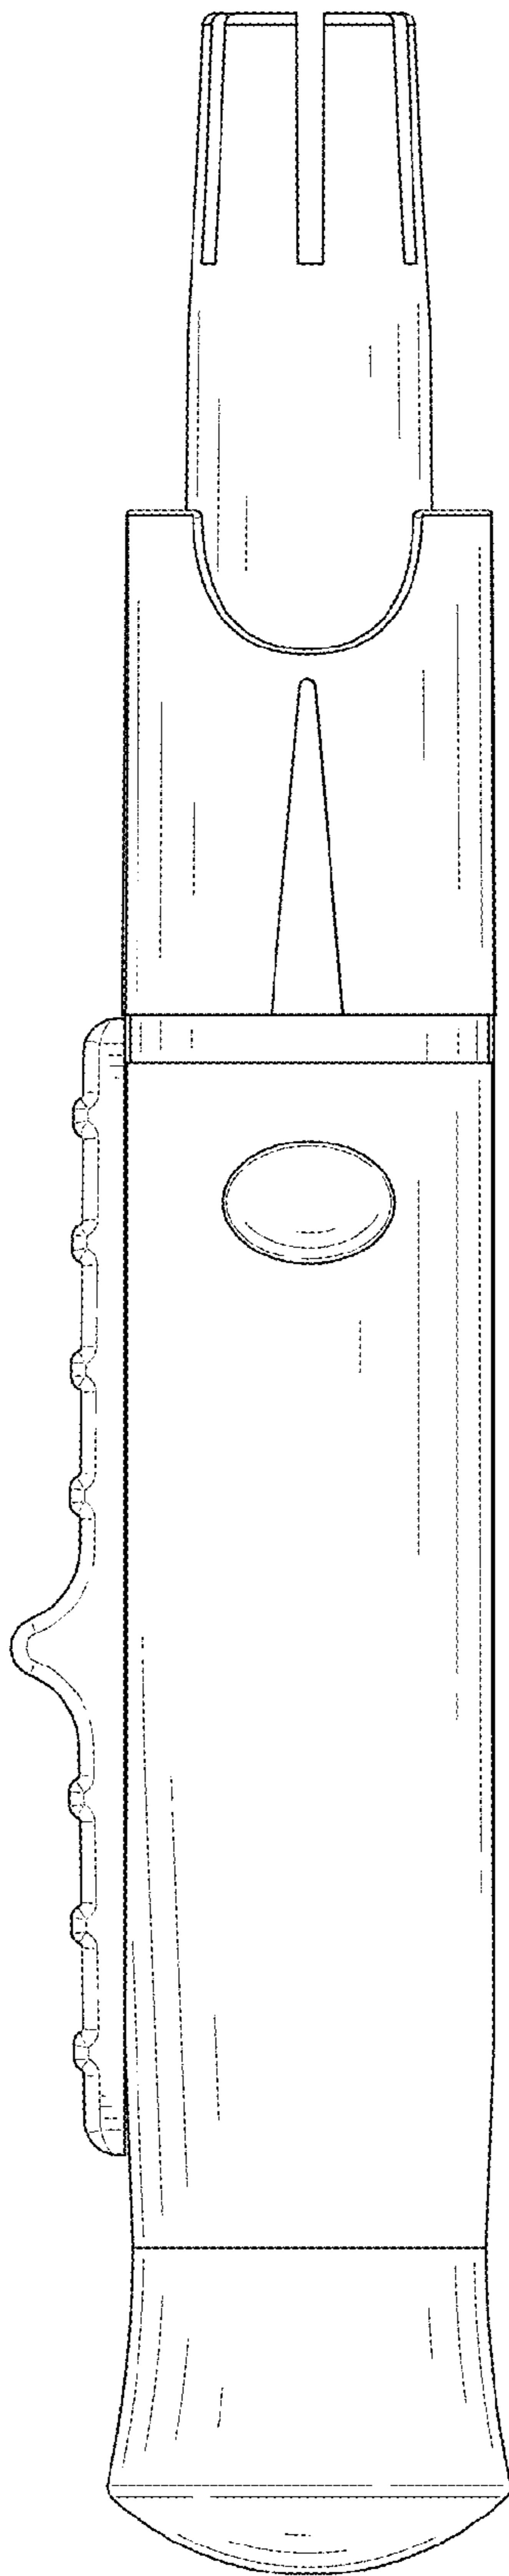


FIG. 6

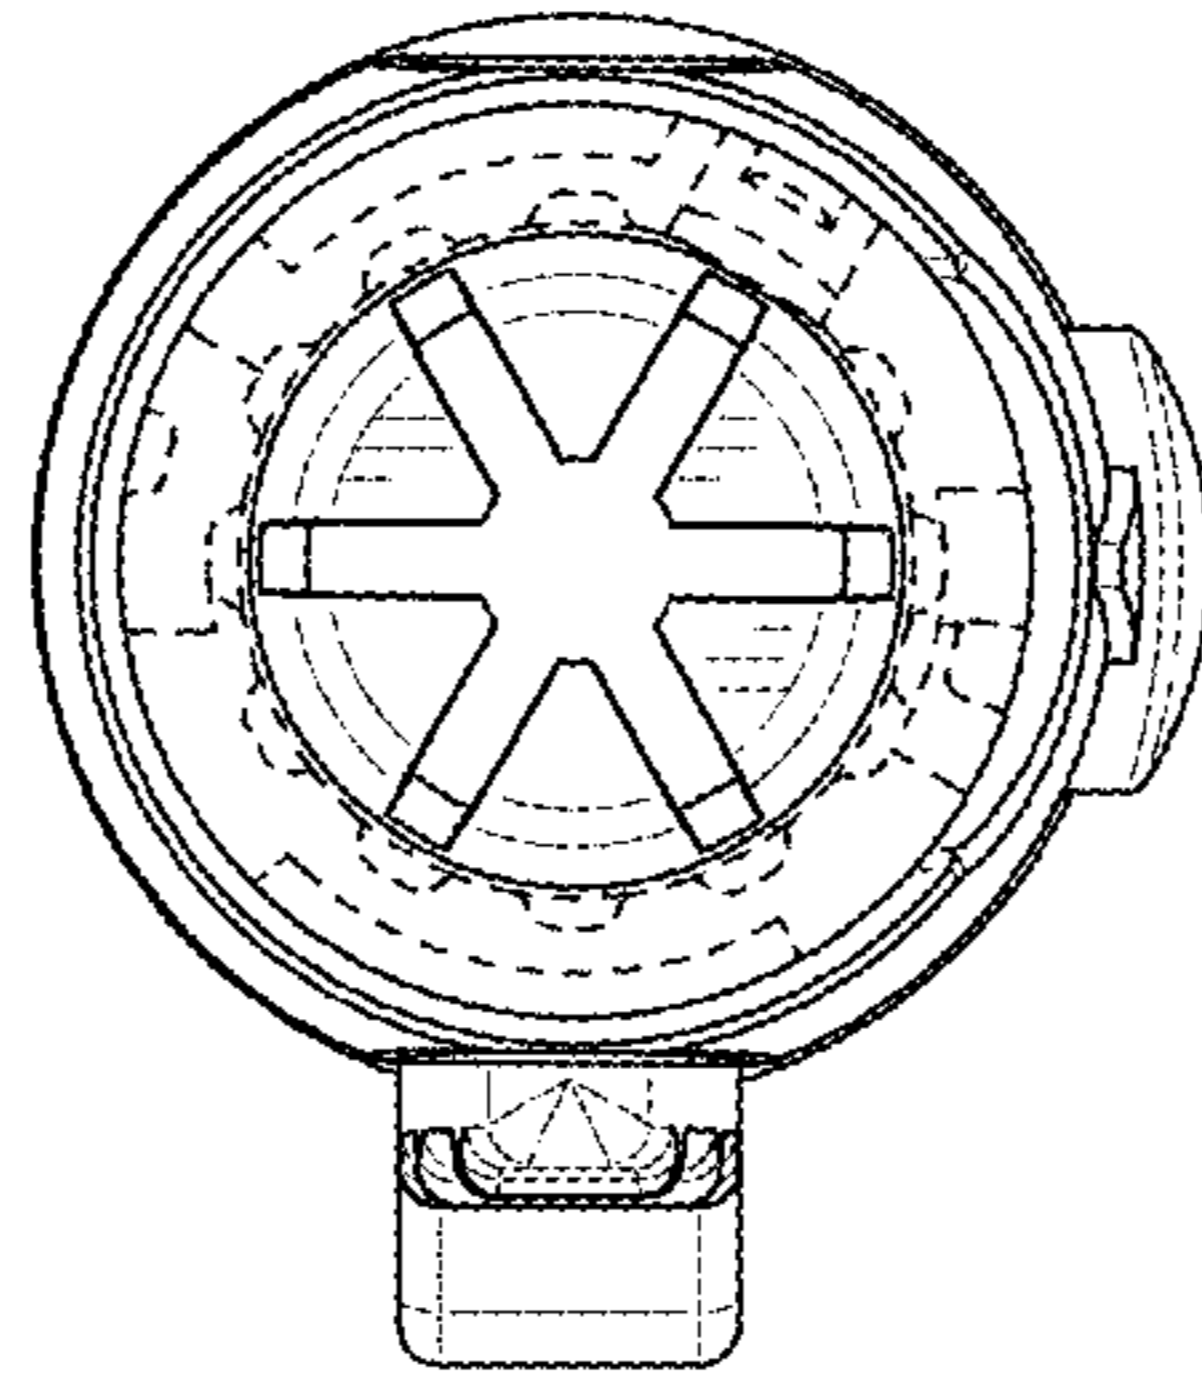


FIG. 7

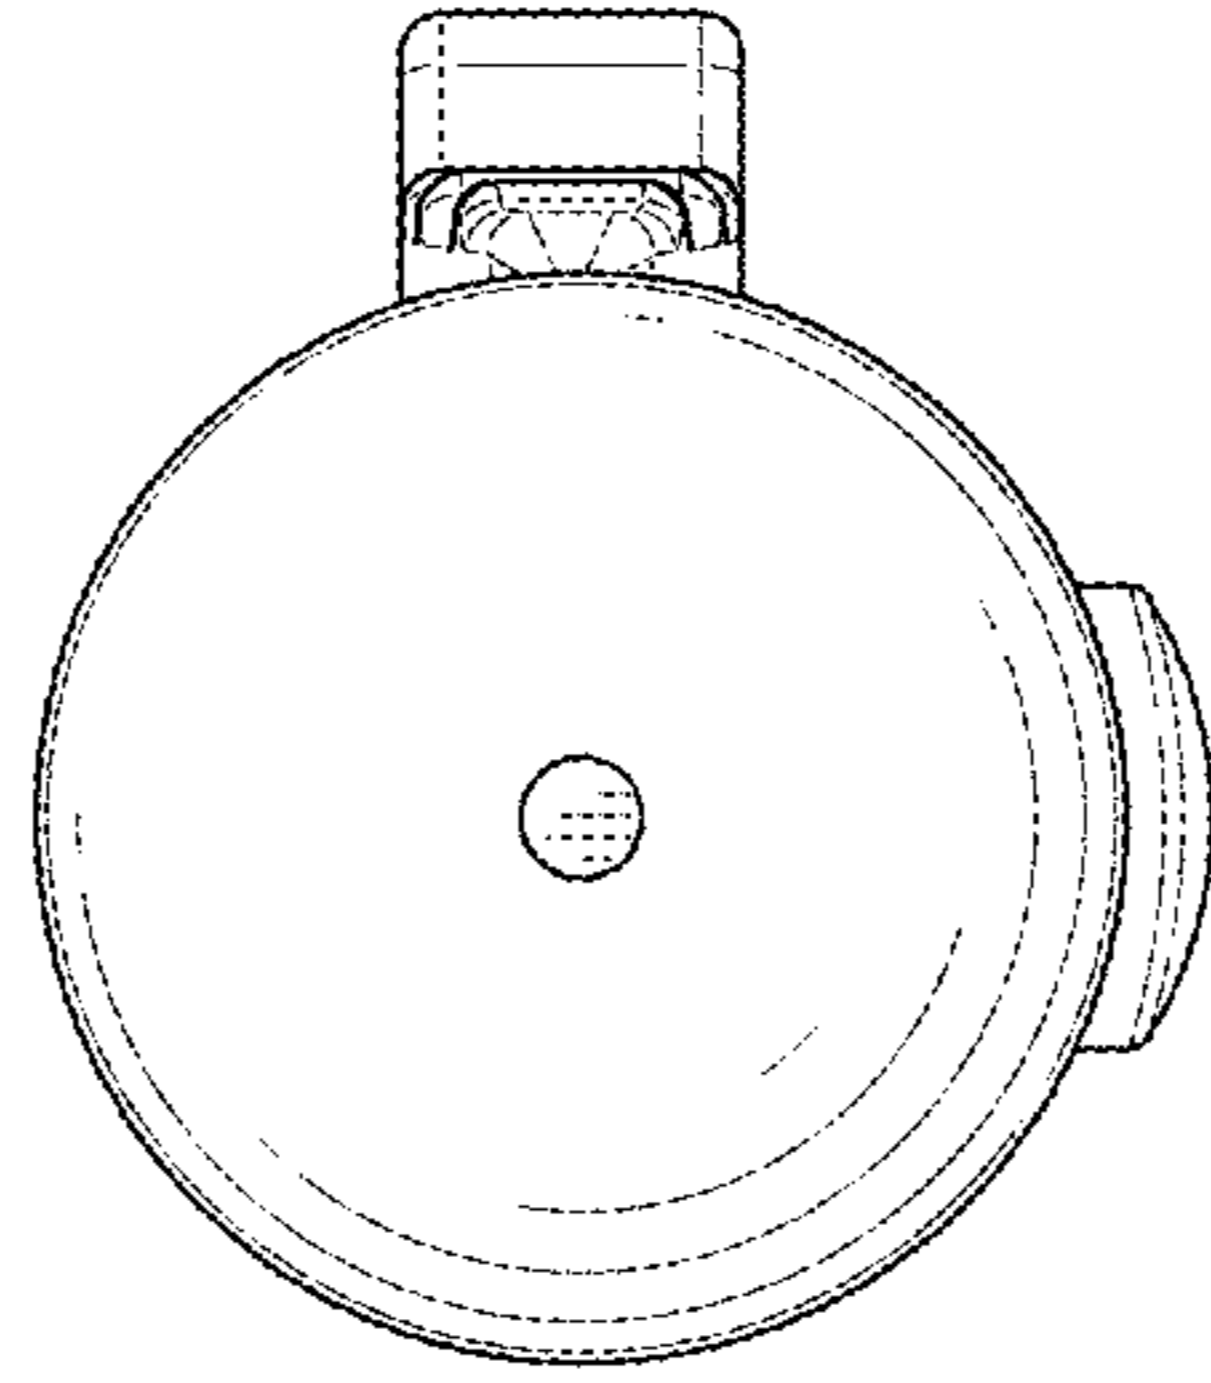


FIG. 8