



US00D944403S

(12) **United States Design Patent** (10) **Patent No.:** **US D944,403 S**
Laurino et al. (45) **Date of Patent:** **** Feb. 22, 2022**

- (54) **VAPOR ANESTHESIA TESTER**
- (71) Applicant: **Fluke Corporation**, Everett, WA (US)
- (72) Inventors: **Ferdinand Y. Laurino**, Seattle, WA (US); **Michael A. Schoch**, Granite Falls, WA (US)
- (73) Assignee: **Fluke Corporation**, Everett, WA (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/753,958**
- (22) Filed: **Oct. 5, 2020**

D698,925 S	2/2014	Marzynski	
D701,780 S	4/2014	Marzynski et al.	
D711,001 S *	8/2014	Boudier	D24/186
D712,543 S	9/2014	Maier	
D741,492 S *	10/2015	Formica	D24/164
D765,258 S	8/2016	Marzynski	
D774,182 S	12/2016	Davidian et al.	
D777,902 S	1/2017	Souney	
D833,022 S	11/2018	Corrigan et al.	
D842,736 S	3/2019	Laurino et al.	
D852,072 S *	6/2019	Laurino	D10/78
D869,311 S *	12/2019	Khattak	D10/81
D884,522 S *	5/2020	Mou	D10/81
D900,655 S *	11/2020	Rocholl Gullon	D10/78
D902,413 S *	11/2020	Laurino	D24/186

* cited by examiner

Related U.S. Application Data

- (62) Division of application No. 29/670,592, filed on Nov. 16, 2018, now Pat. No. Des. 902,413.
- (51) **LOC (13) Cl.** **24-01**
- (52) **U.S. Cl.**
USPC **D24/186**
- (58) **Field of Classification Search**
USPC D24/107, 163, 164, 167, 185, 186, 216, D24/231, 232; D10/81, 78, 96
CPC A61G 11/00; A61G 11/002; A61G 11/005; A61G 11/009; A01K 41/00; A01K 41/02; A01K 41/04; A61B 5/08; A61B 5/0803
See application file for complete search history.

References Cited

U.S. PATENT DOCUMENTS

D423,665 S	4/2000	Herbst et al.
D471,271 S	3/2003	Strömberg et al.
D579,540 S	10/2008	Hochman et al.
D590,734 S	4/2009	Mendelson et al.

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Merchant & Gould P.C.


(57) **CLAIM**

The ornamental design for a vapor anesthesia tester, as shown and described.

DESCRIPTION

FIG. 1 is a top, front, right side perspective view of a vapor anesthesia tester showing our new design.
 FIG. 2 is a bottom, rear, left side perspective view thereof.
 FIG. 3 is a front elevation view thereof.
 FIG. 4 is a left side elevation view thereof.
 FIG. 5 is a rear elevation view thereof.
 FIG. 6 is a right side elevation view thereof.
 FIG. 7 is a top plan view thereof; and,
 FIG. 8 is a bottom plan view thereof.
 The broken lines in the figures illustrate portions of the vapor anesthesia tester in which the design is embodied that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

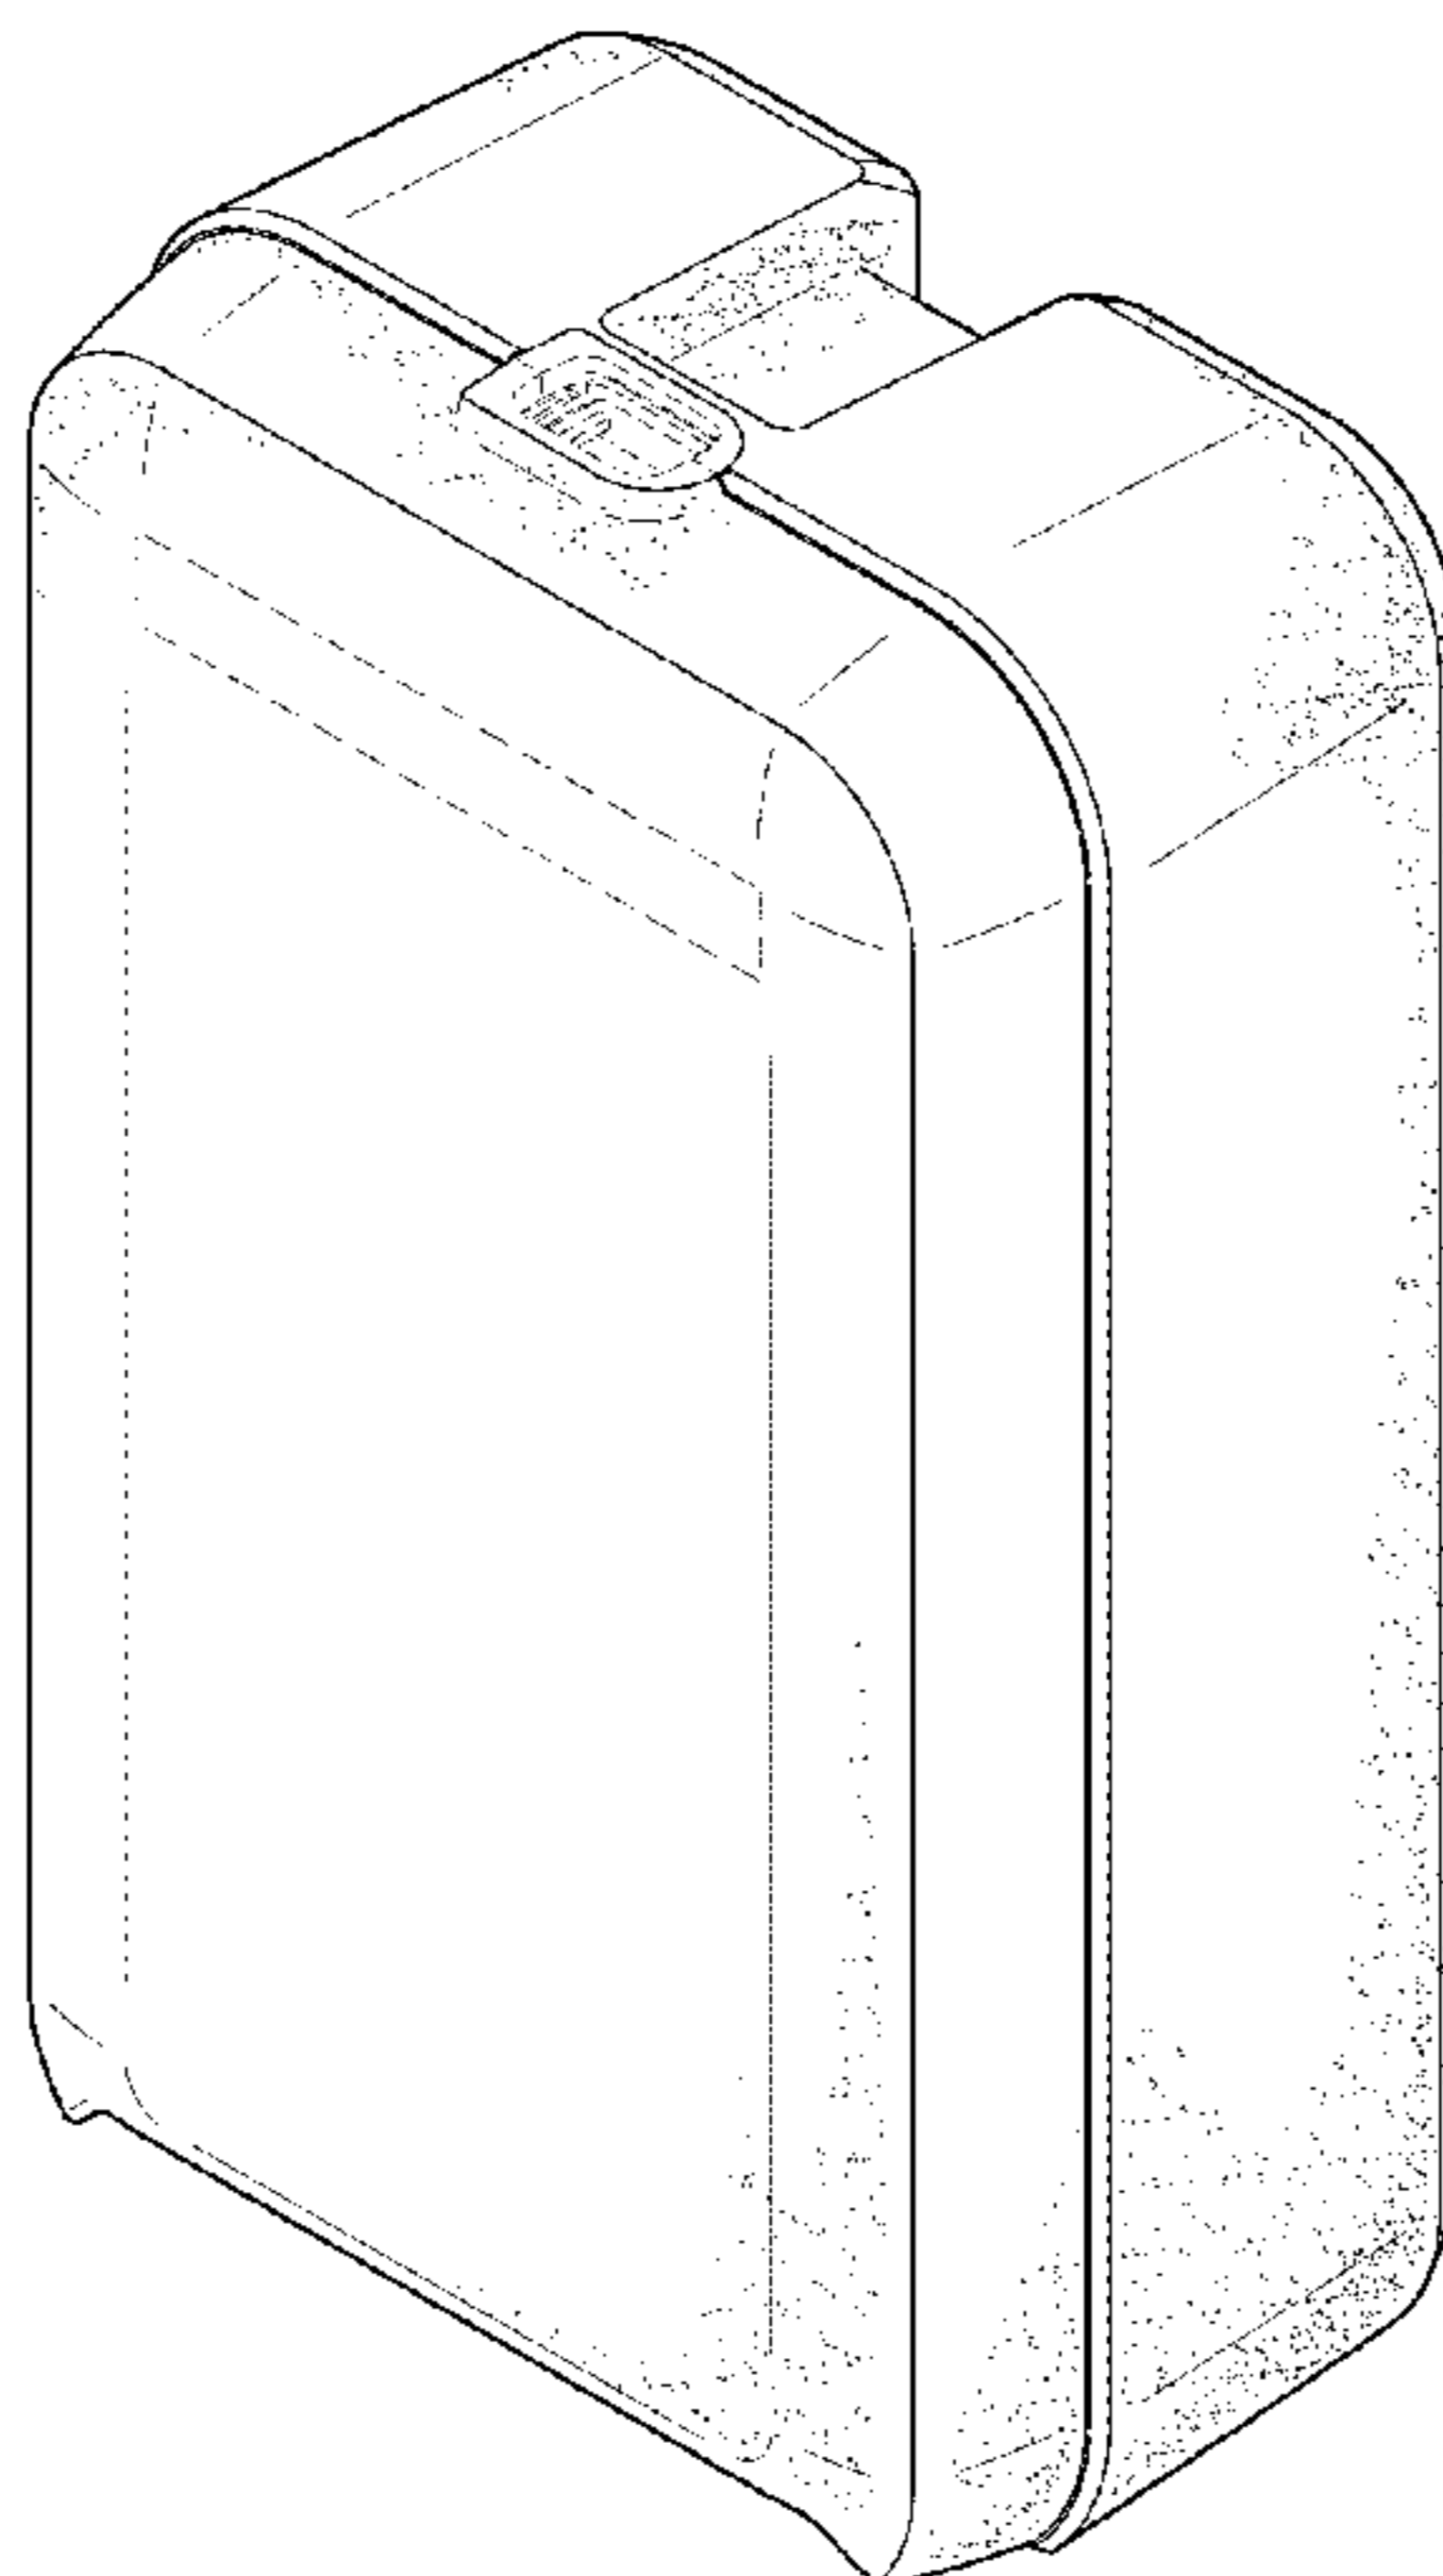

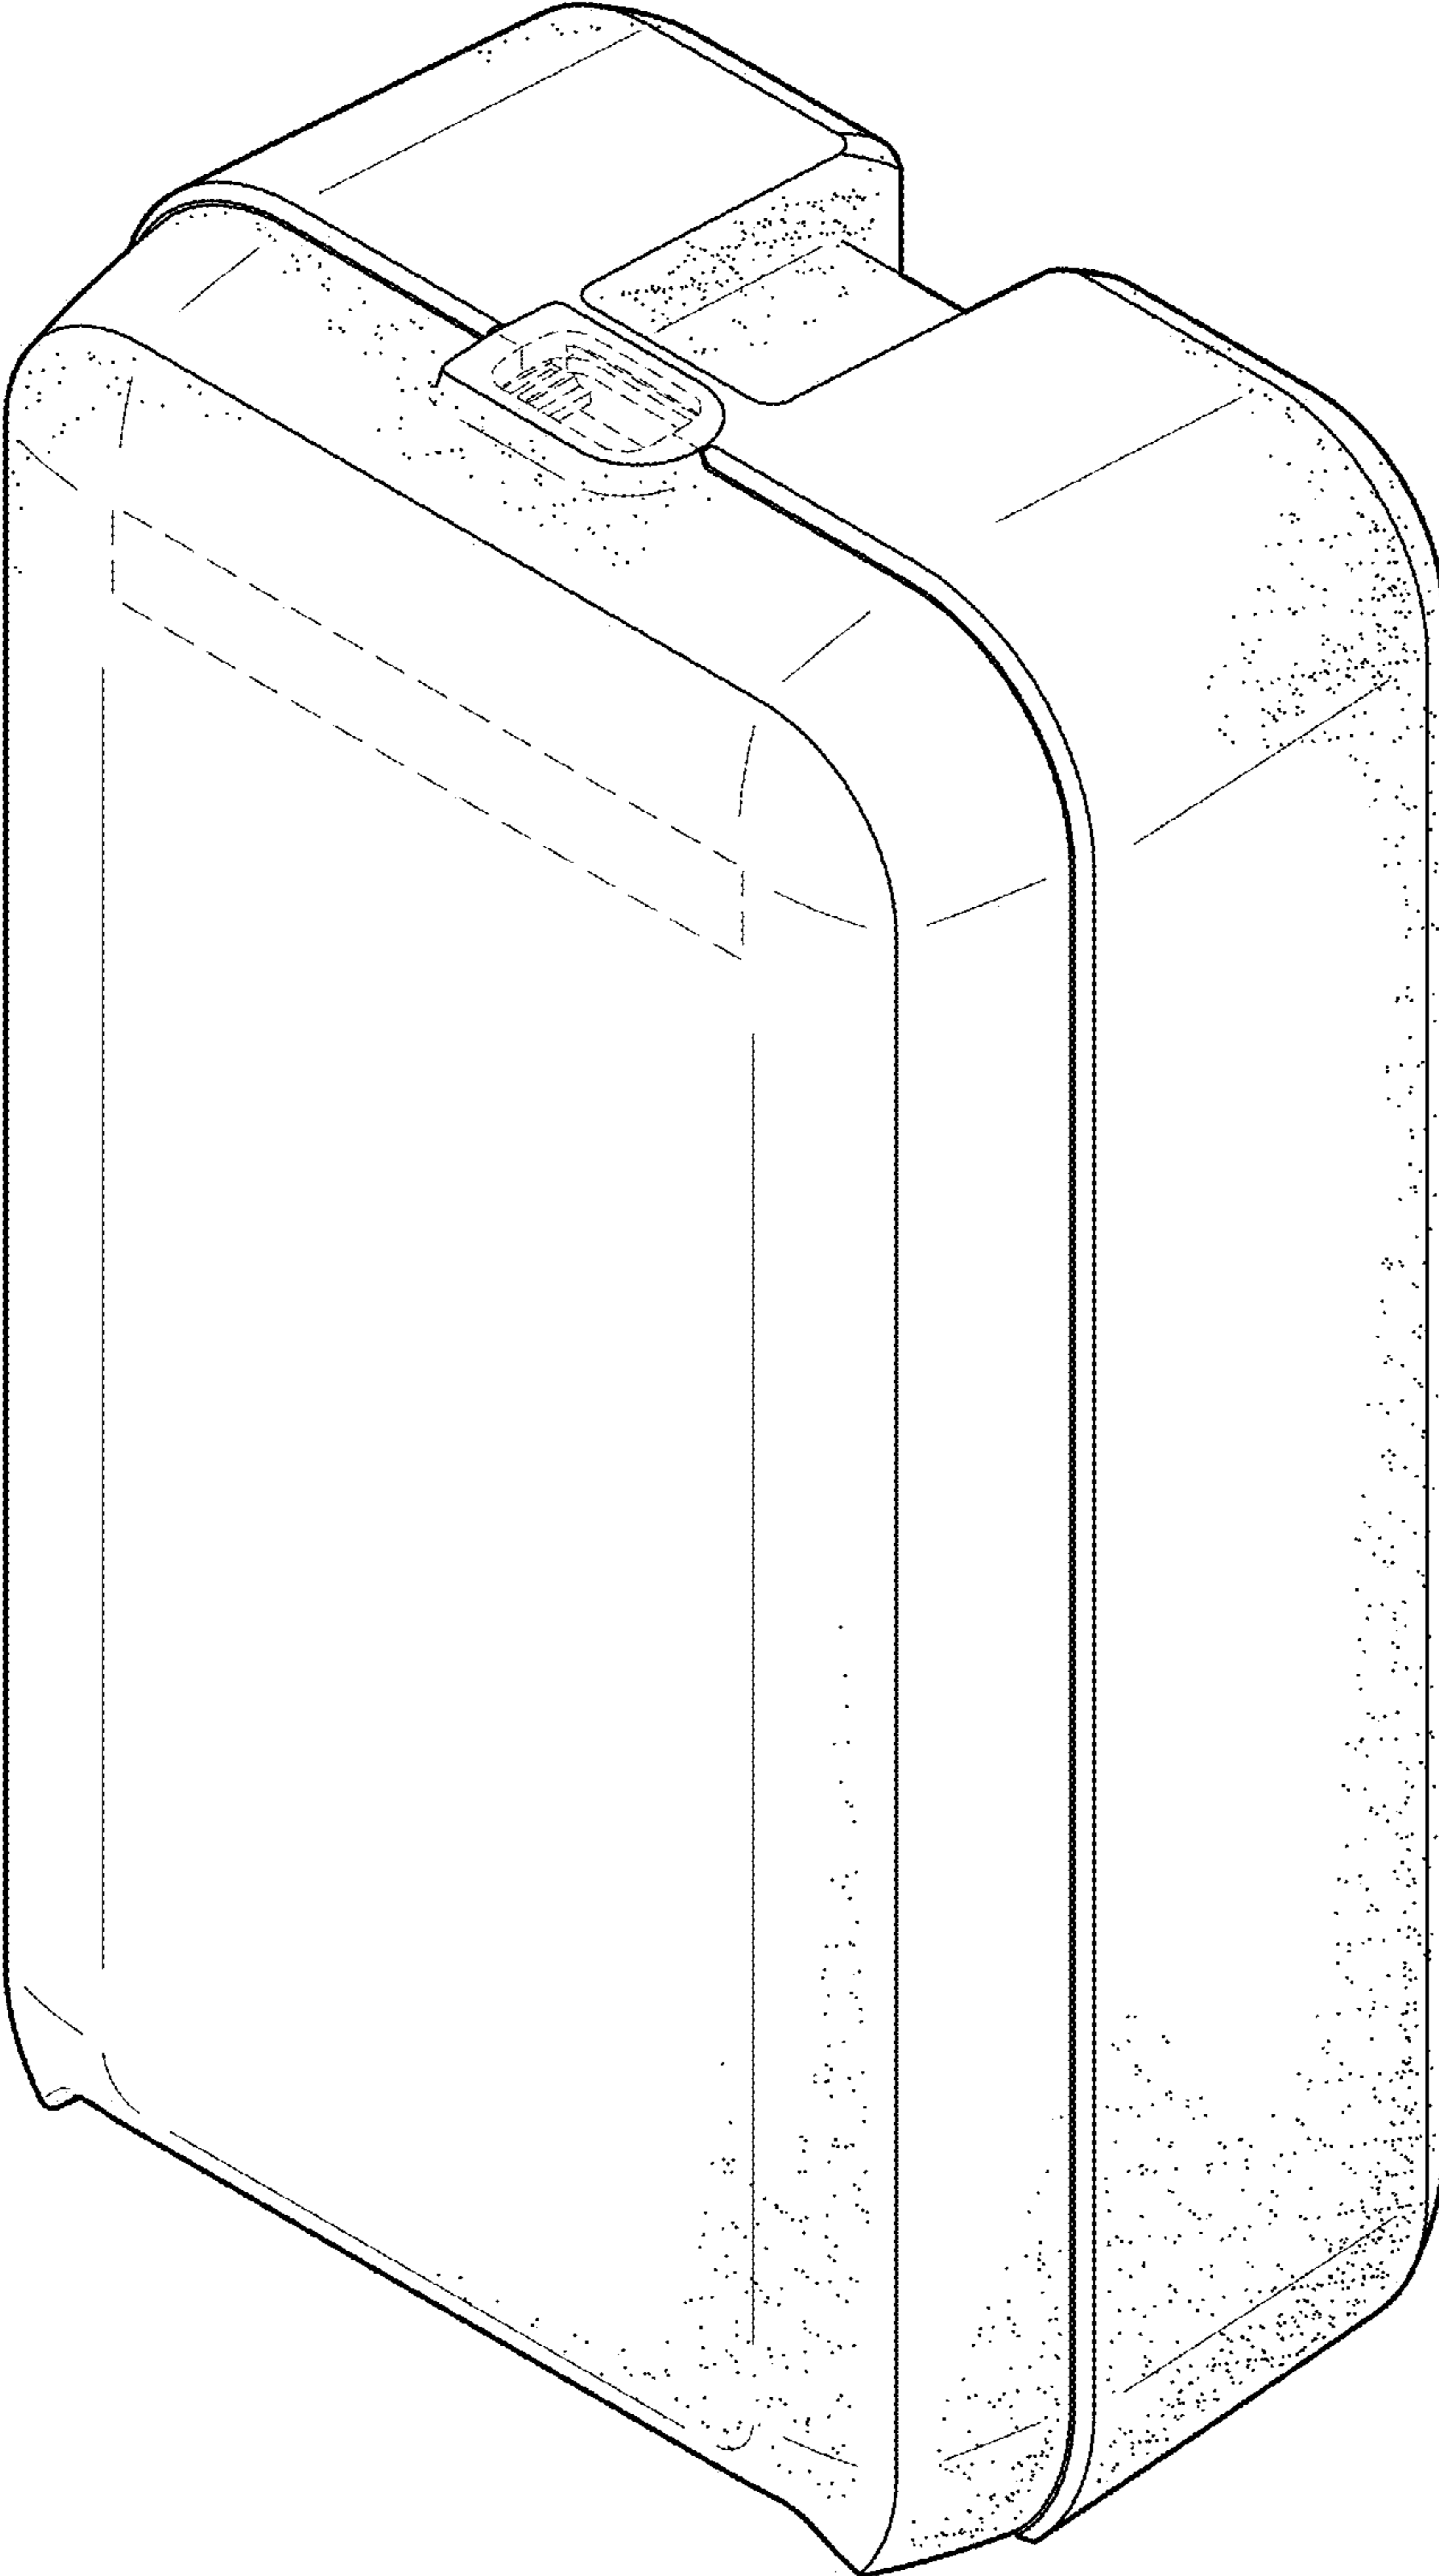


FIG. 1

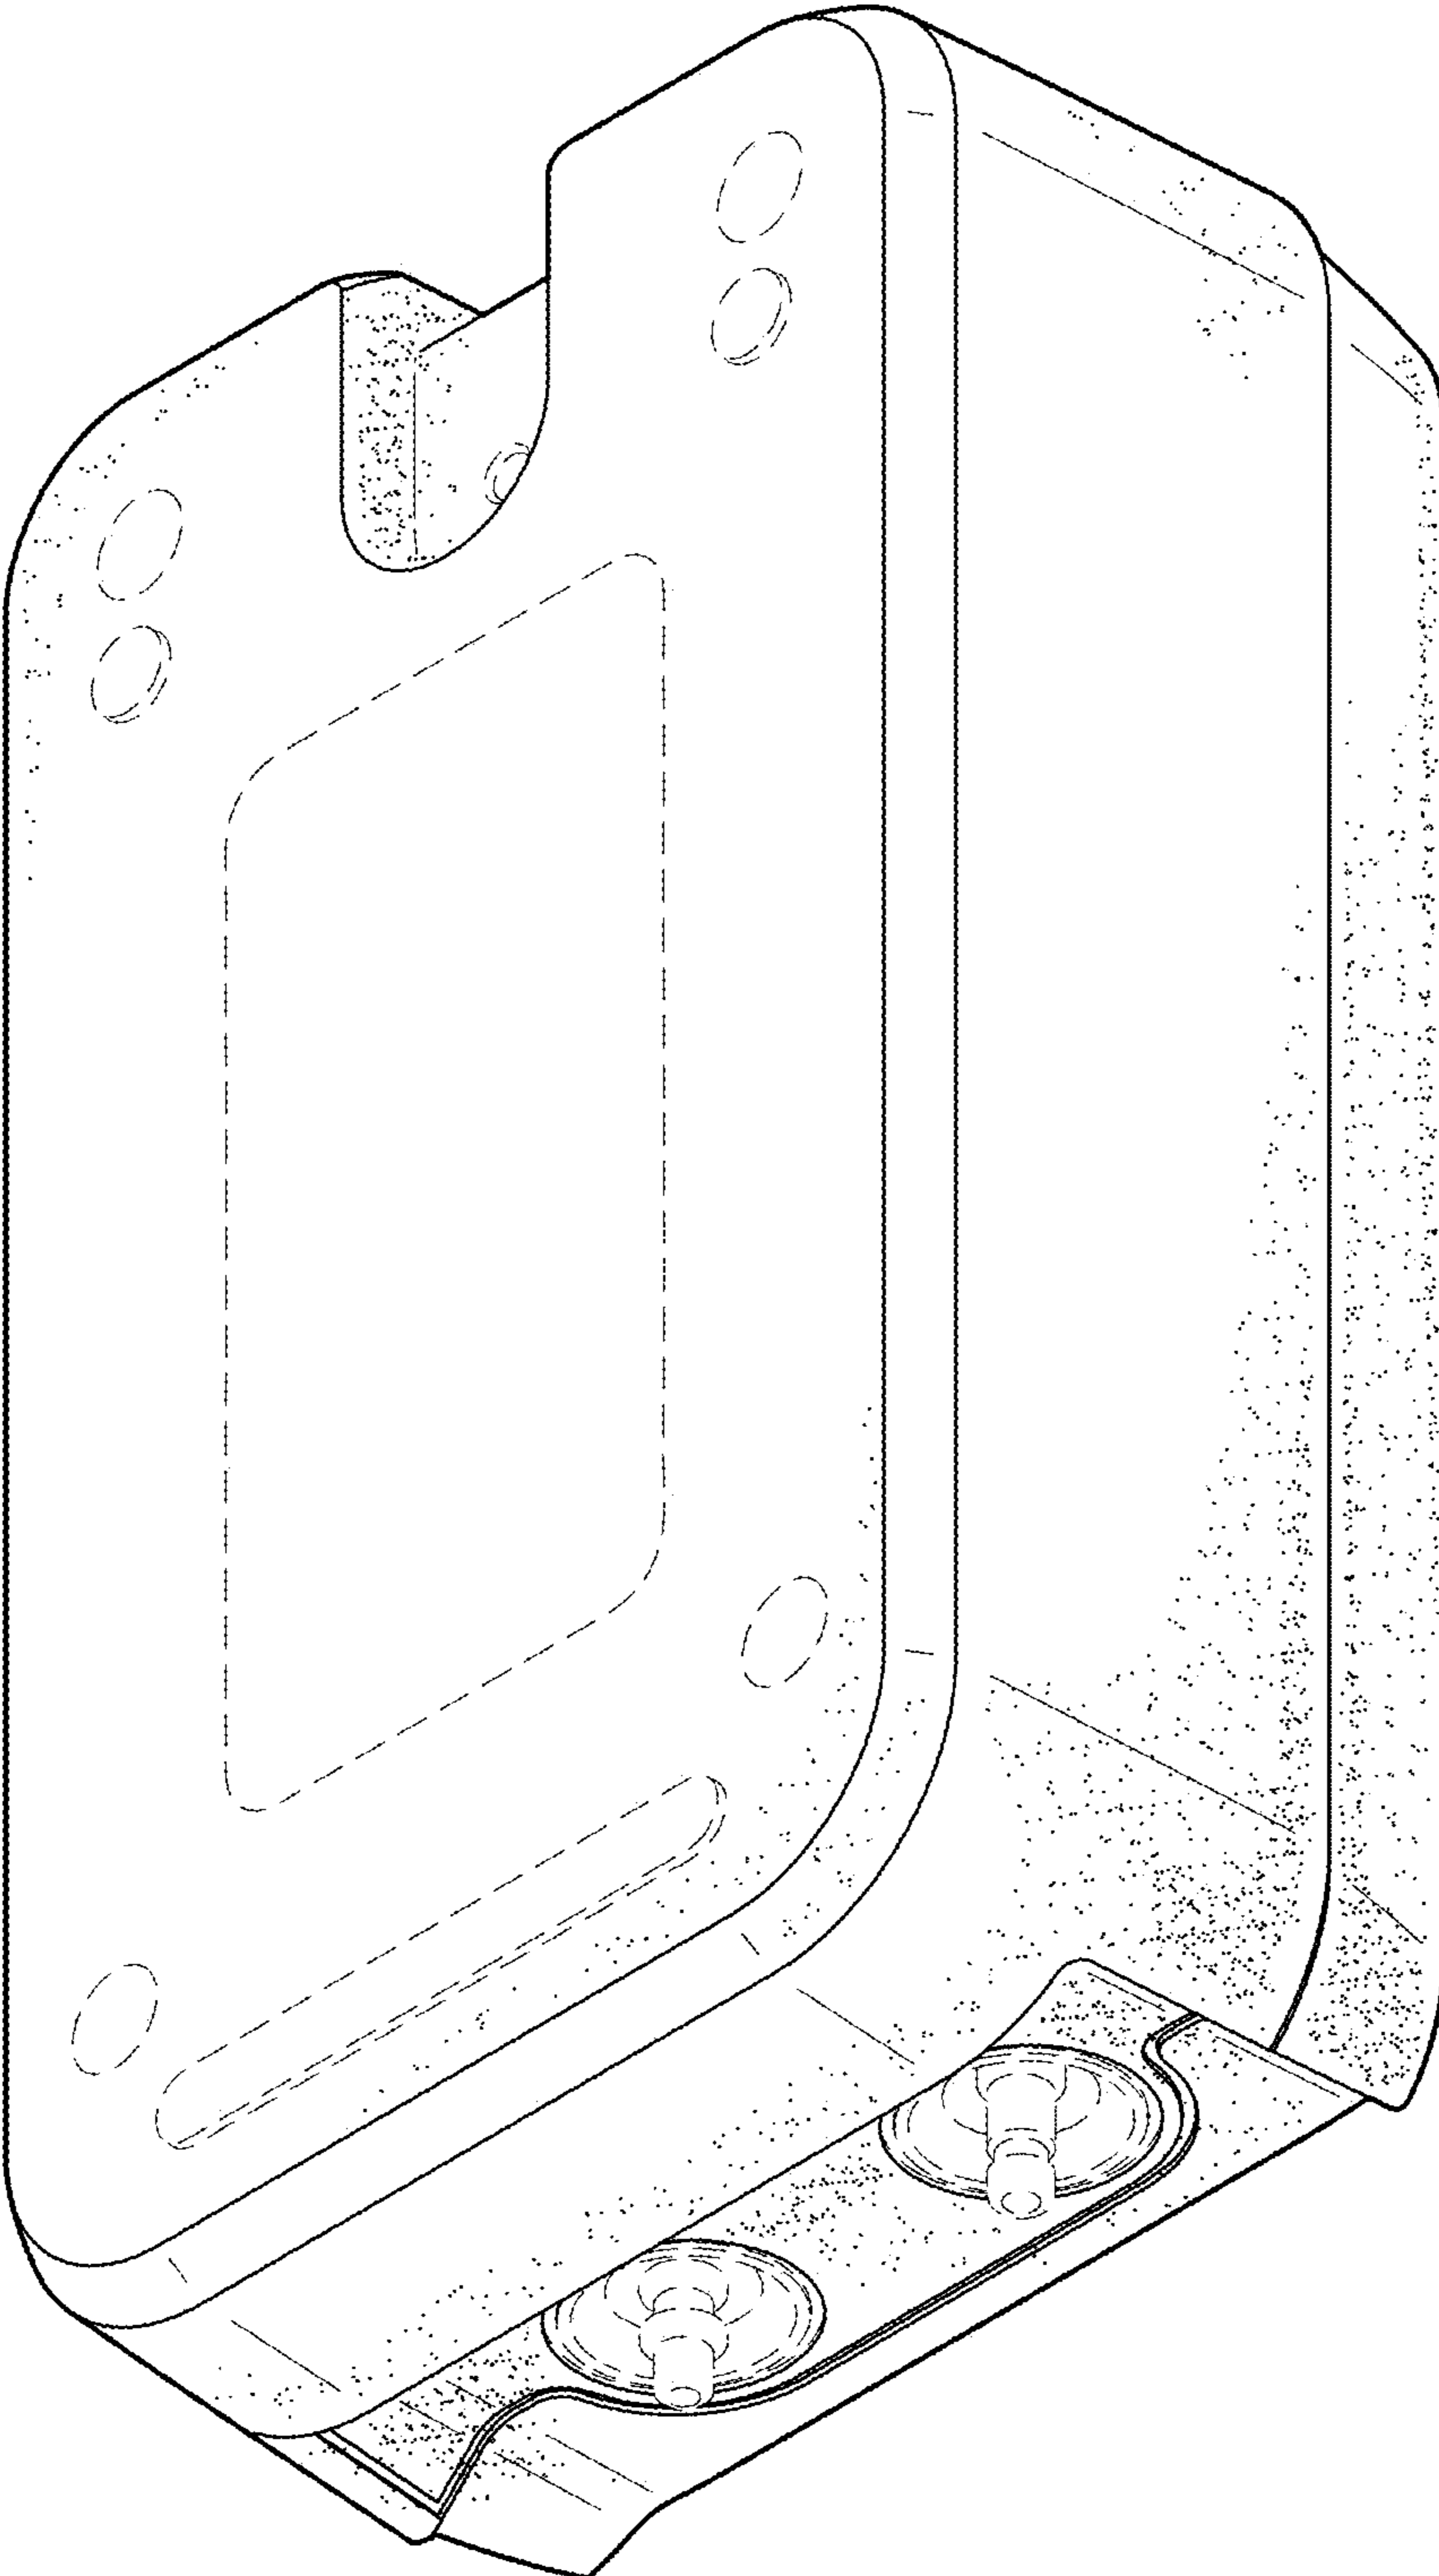


FIG. 2

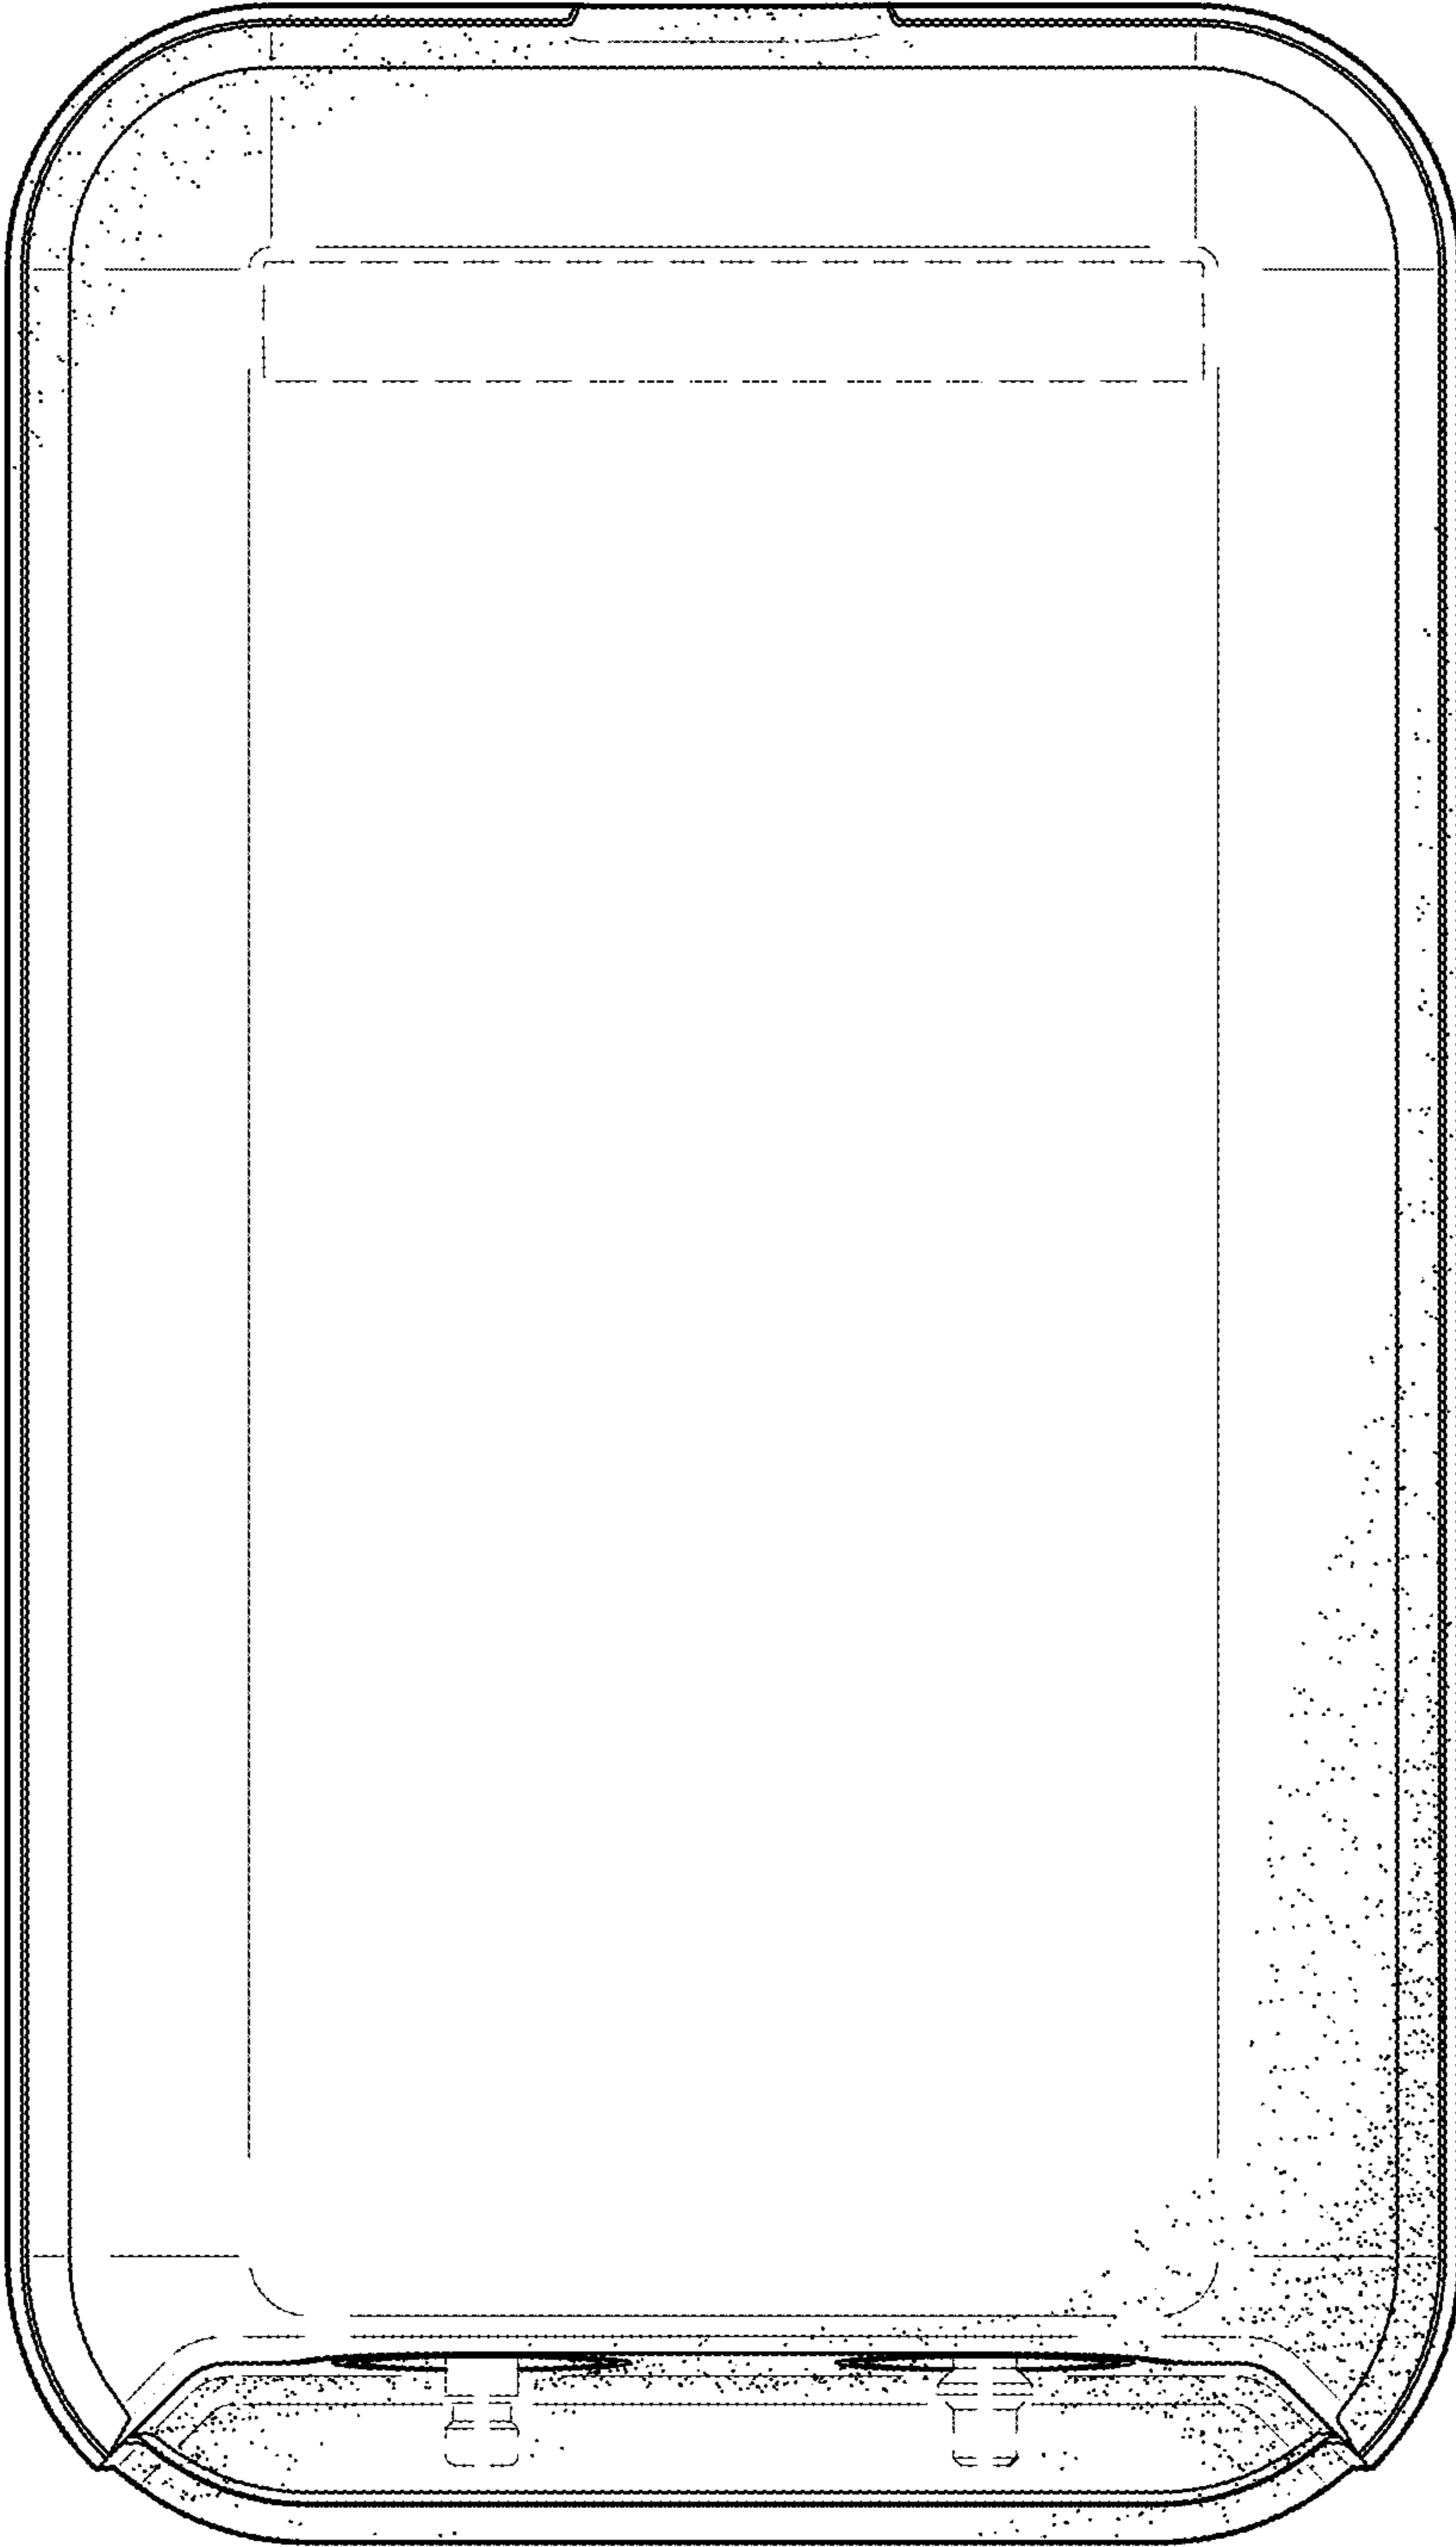


FIG. 3

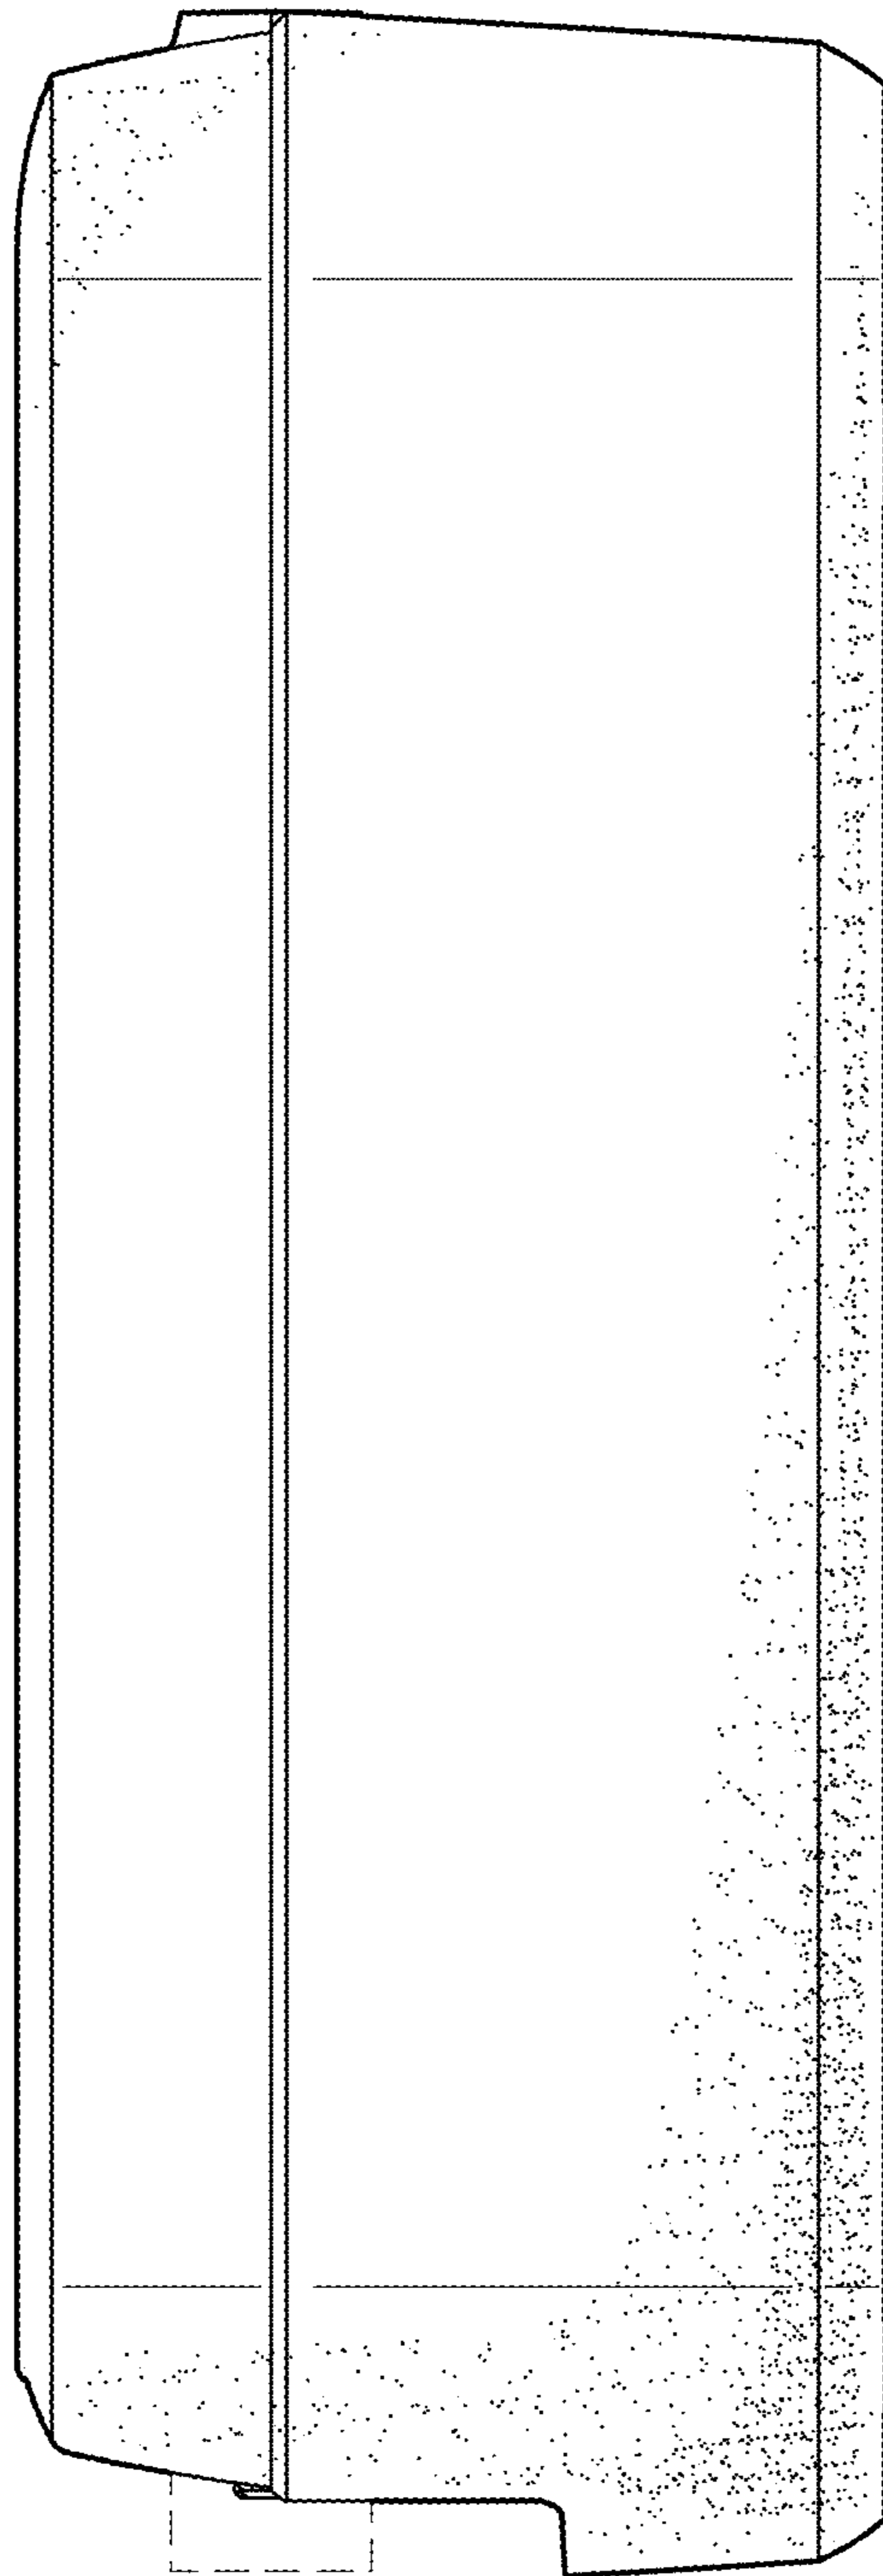


FIG. 4

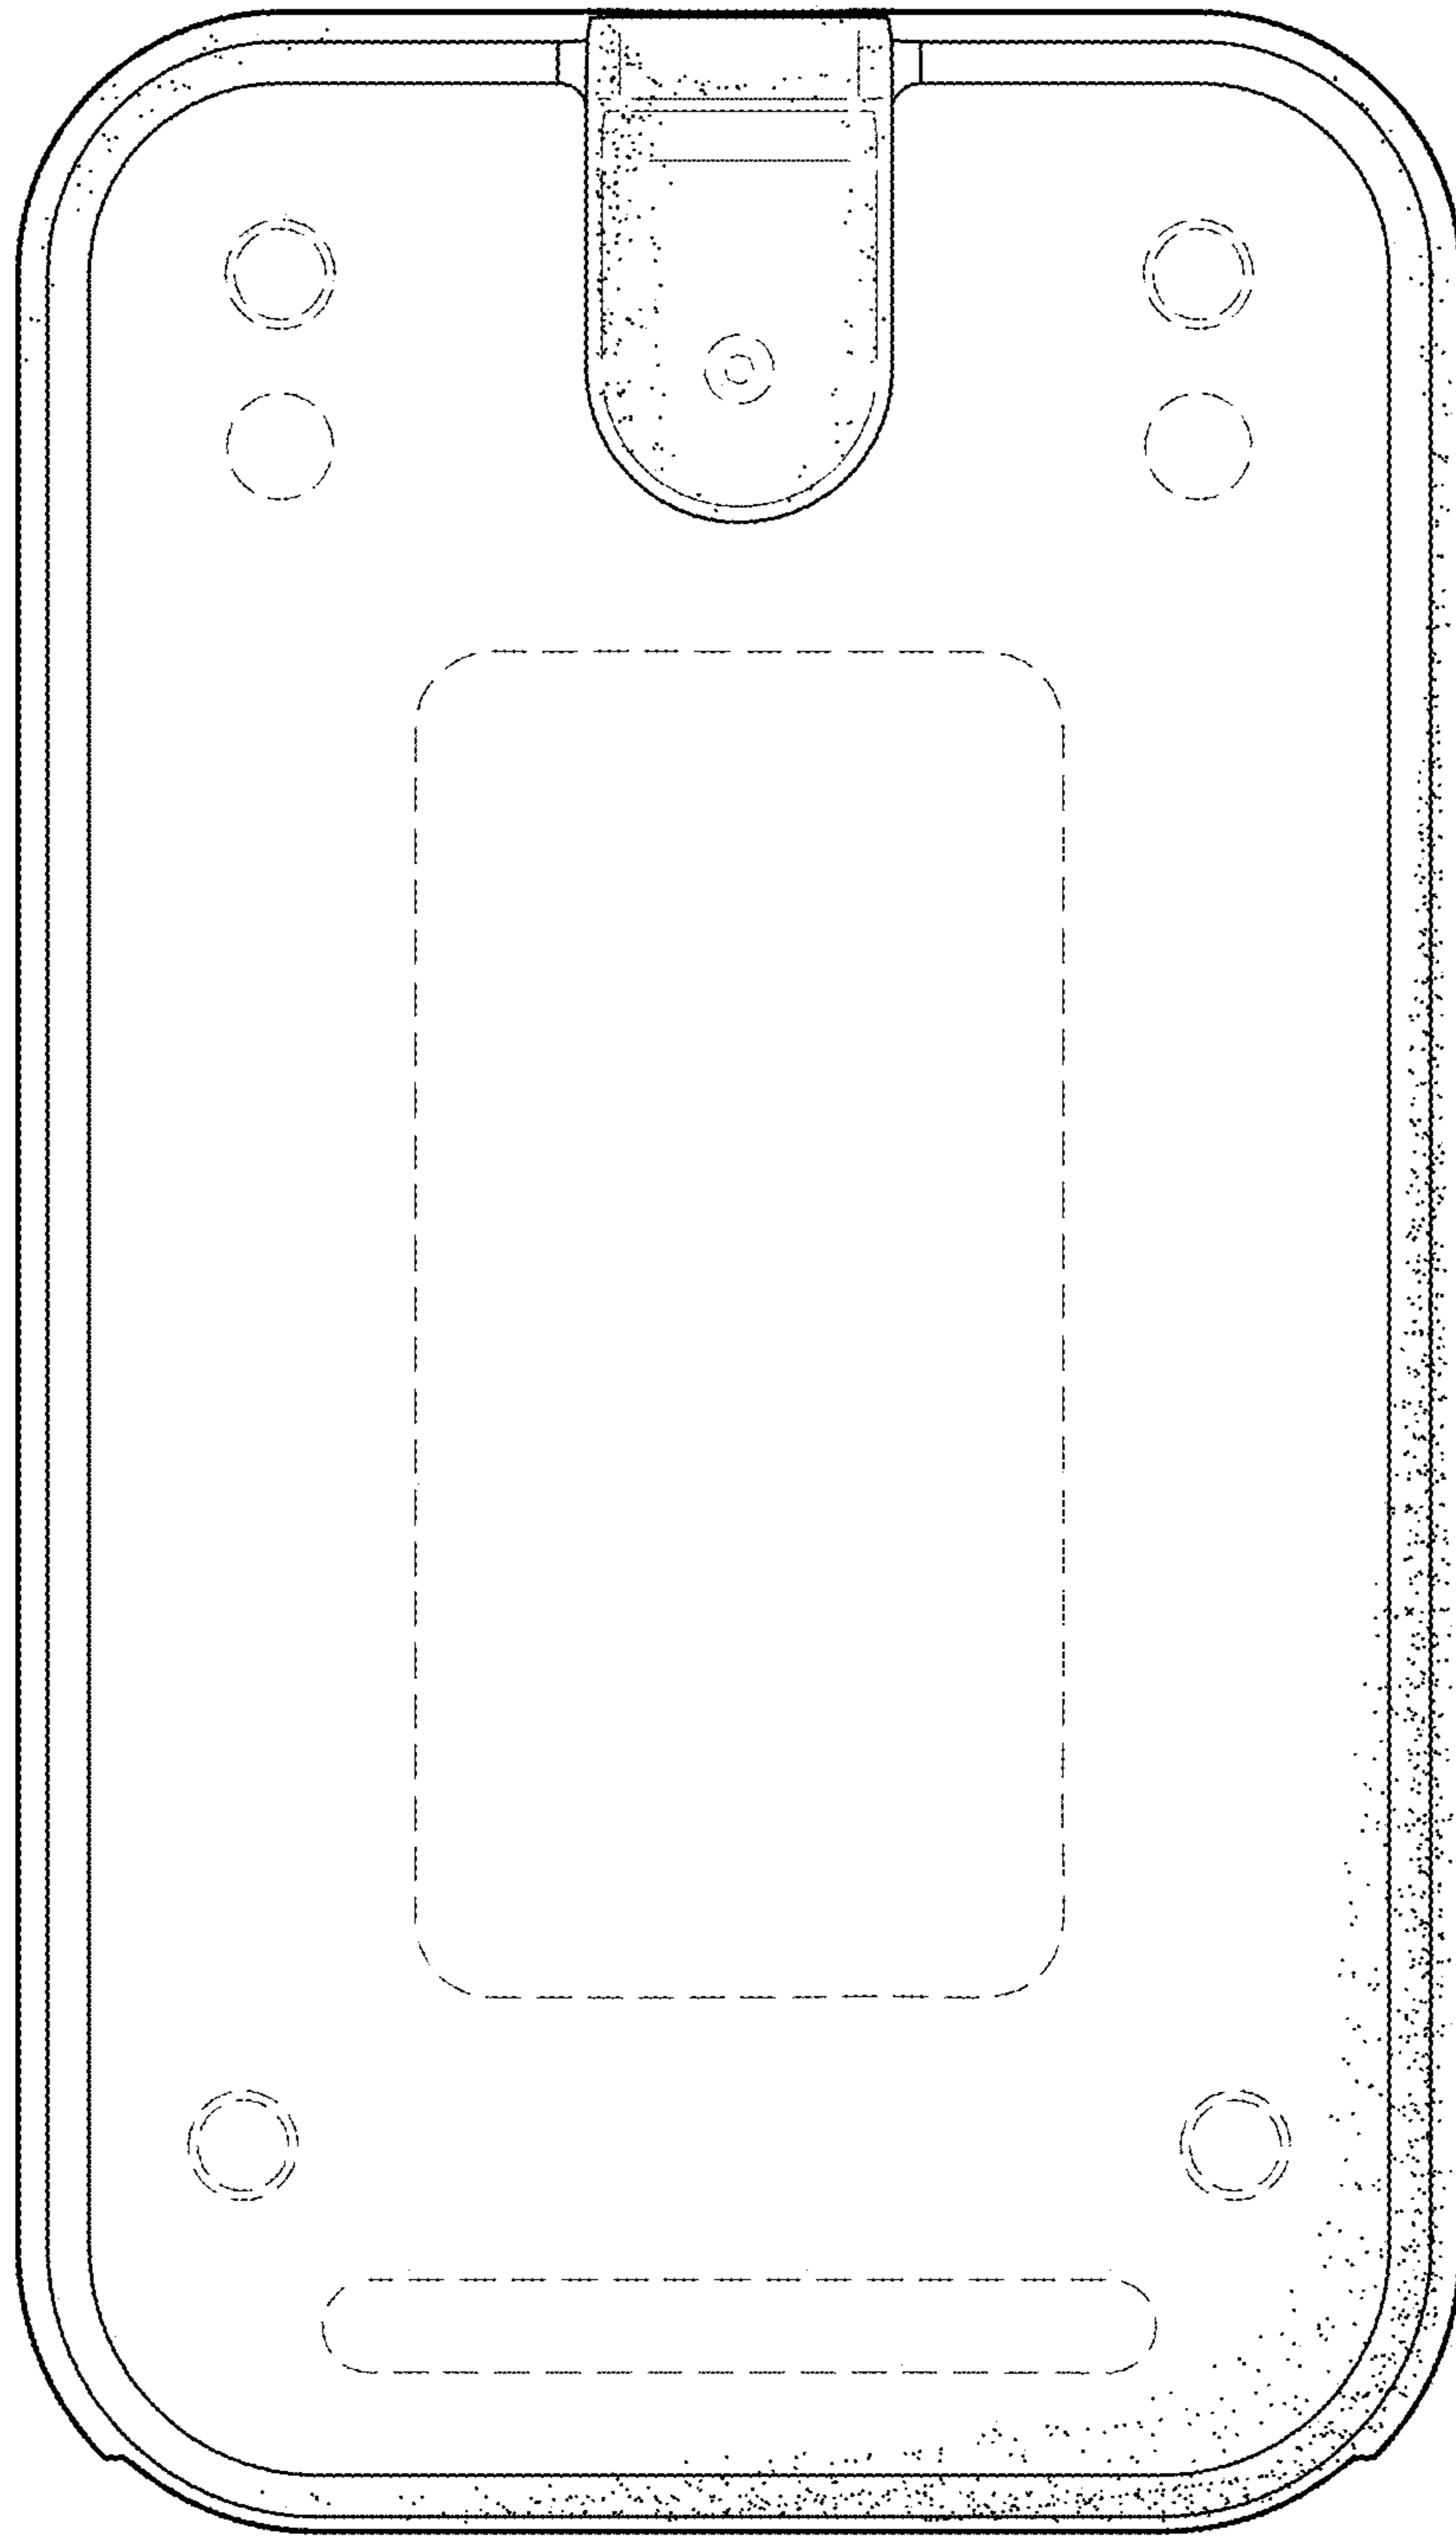


FIG. 5

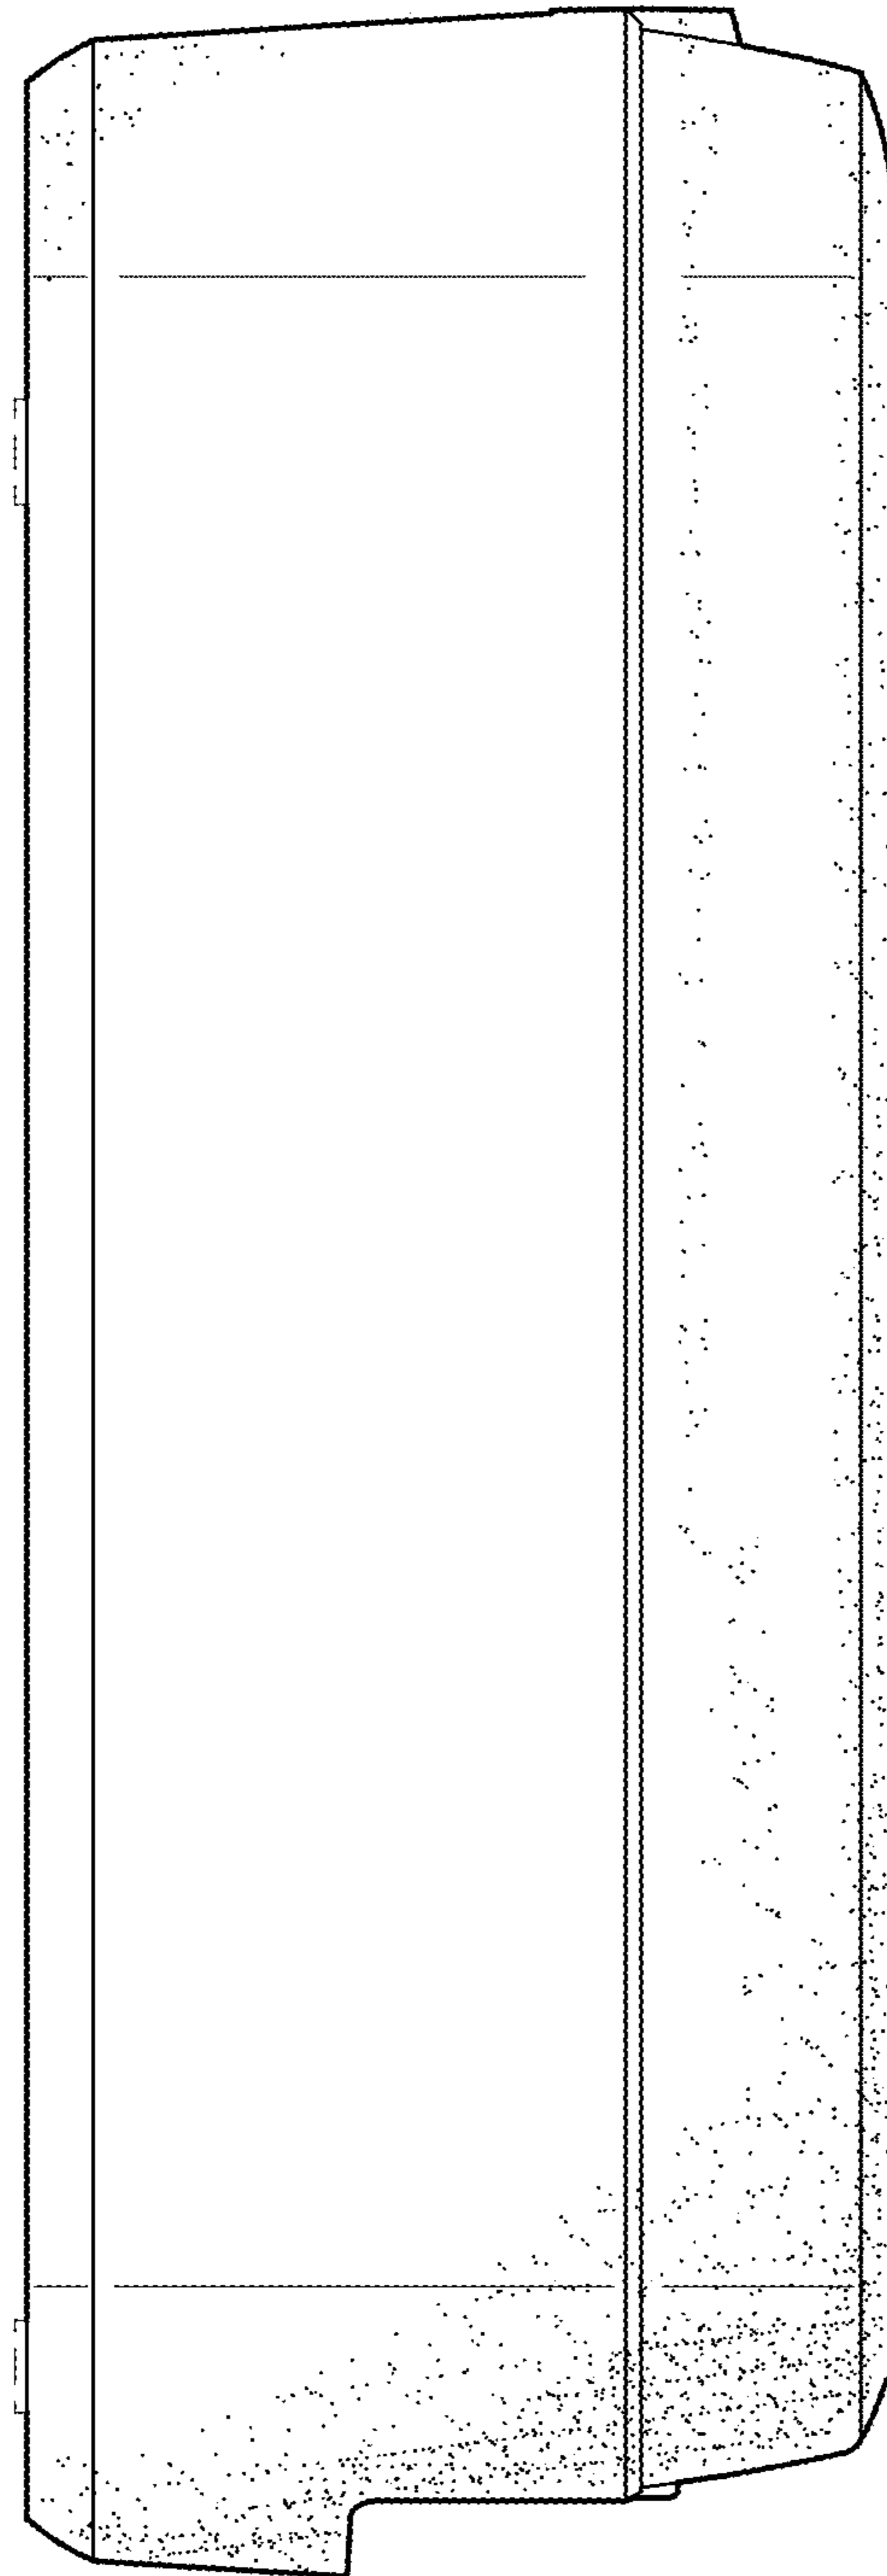


FIG. 6

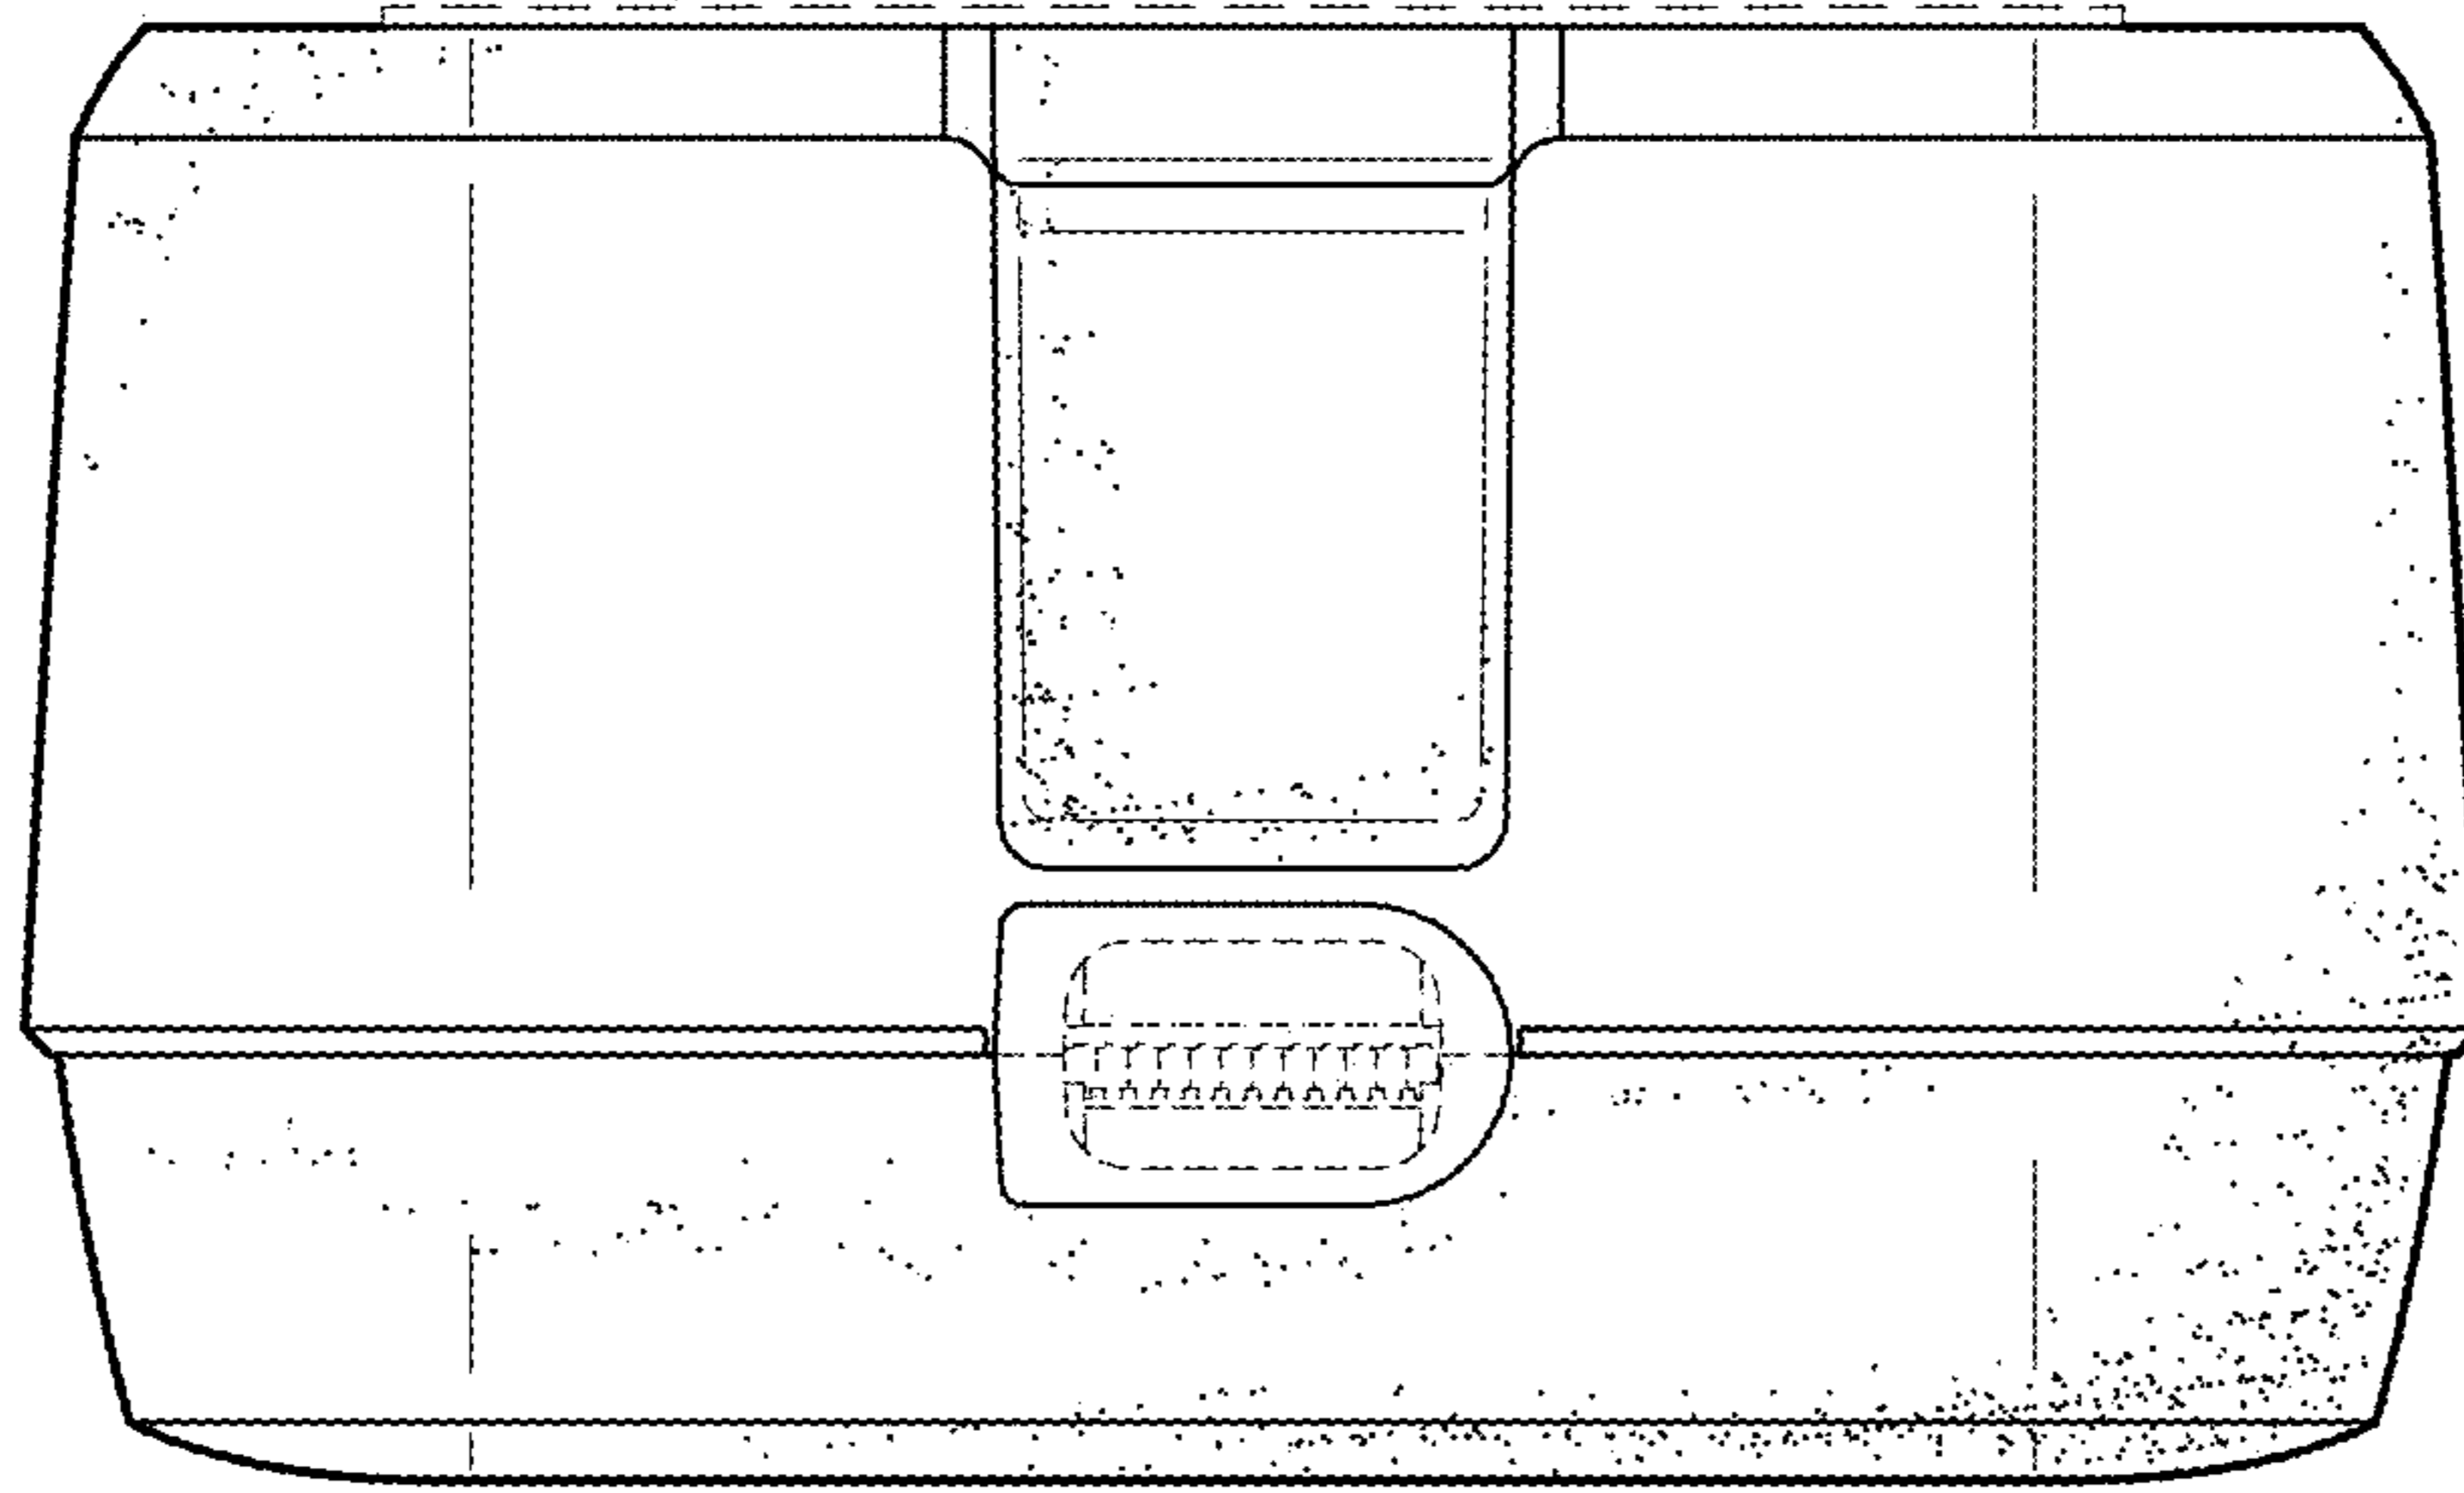


FIG. 7

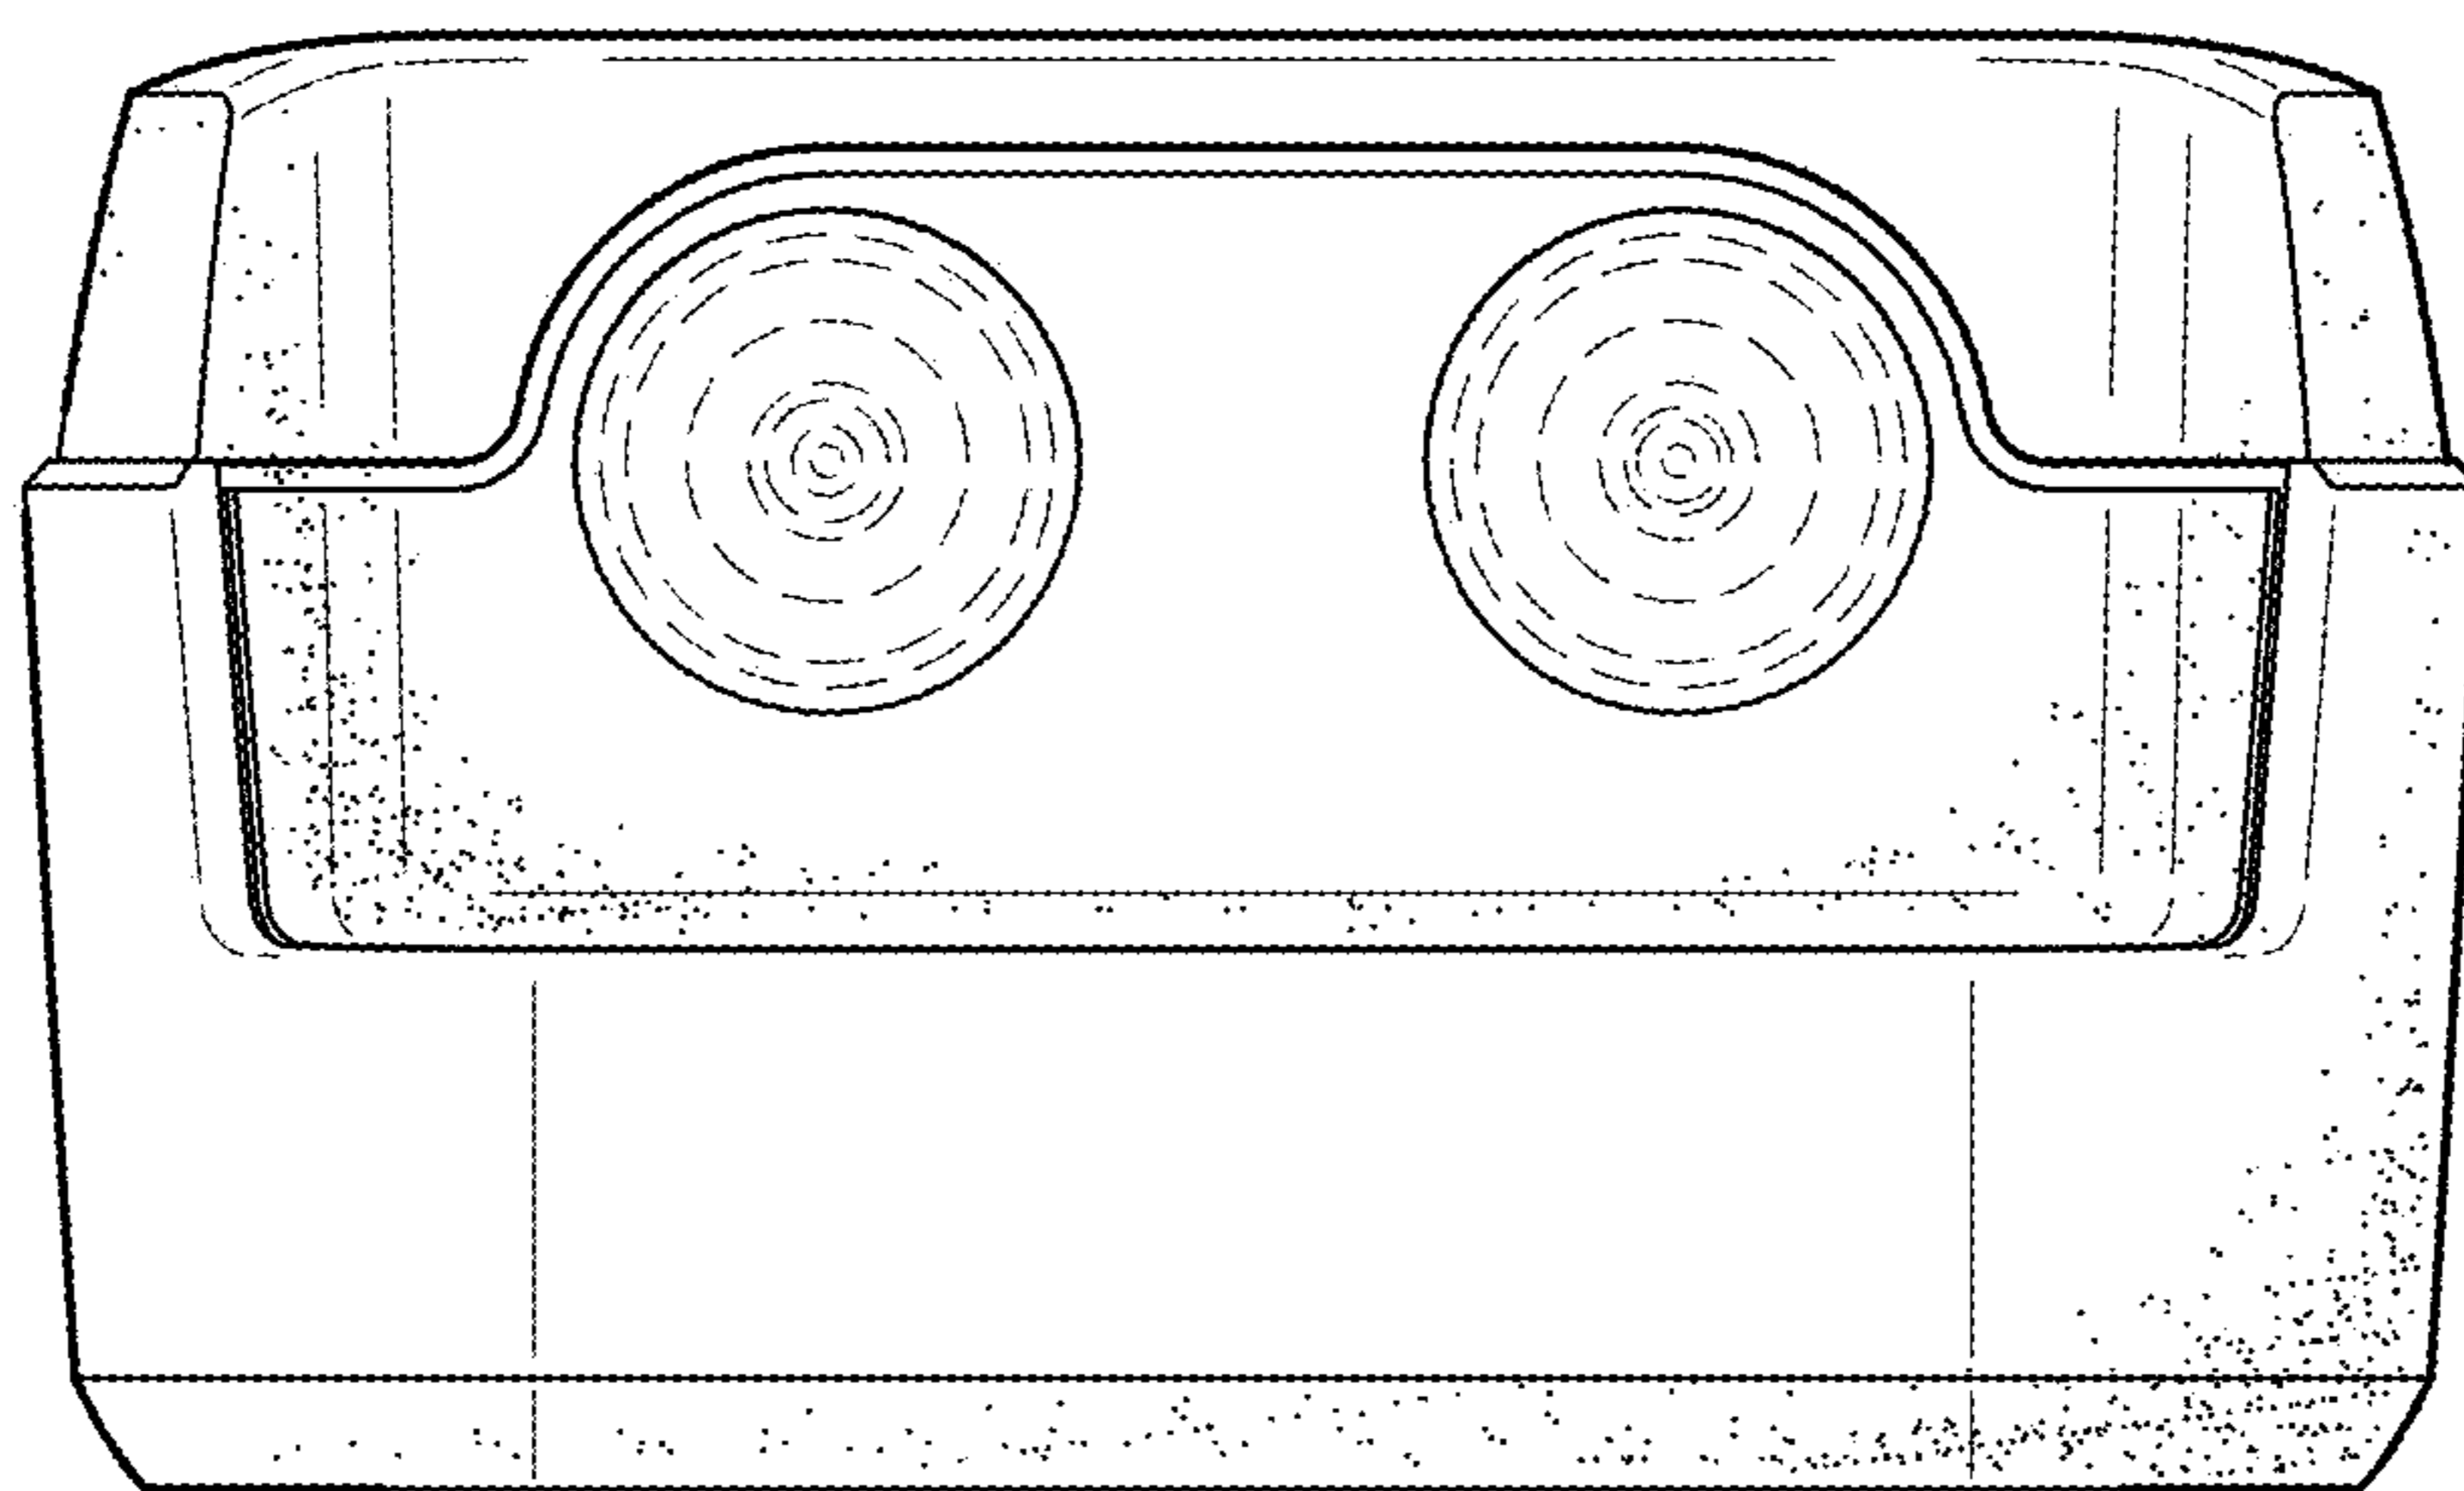


FIG. 8