



US00D946153S

(12) **United States Design Patent** (10) **Patent No.:** **US D946,153 S**
Schafer et al. (45) **Date of Patent:** **** Mar. 15, 2022**

(54) **TRANSDUCER HOLDER**
(71) Applicant: **BRAINSONIX CORPORATION**,
Sherman Oaks, CA (US)
(72) Inventors: **Mark Evan Schafer**, Ambler, PA (US);
Christopher H. Scholl, West Chester,
PA (US); **Joseph Jackson**, Wilmington,
DE (US)
(73) Assignee: **BRAINSONIX CORPORATION**,
Sherman Oaks, CA (US)
(**) Term: **15 Years**
(21) Appl. No.: **29/735,396**
(22) Filed: **May 20, 2020**
(51) **LOC (13) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/187**
(58) **Field of Classification Search**
USPC D24/133, 137, 138, 141, 158, 160, 164,
D24/165, 167, 170, 186, 187, 200;
D10/57, 60, 78, 80; D3/318, 319;
D16/211, 213, 218, 219, 237, 242
CPC G01F 15/18; A61B 8/4455; A61B 8/445;
A61B 8/4209; A61B 5/0095; A61B
8/4444; G01N 29/265; G01S 7/5208
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS
D224,955 S * 10/1972 Tipton D6/716.1
4,920,966 A * 5/1990 Hon A61B 5/4356
600/459
D383,968 S * 9/1997 Bidwell D8/356
D391,838 S * 3/1998 Bidwell D8/356
D742,530 S * 11/2015 Pippel D24/187
D776,295 S * 1/2017 Wainwright D24/224
D776,296 S * 1/2017 Wainwright D24/224
D782,685 S * 3/2017 Pippel D24/186

D879,313 S * 3/2020 Pounders D24/200
D897,543 S * 9/2020 Jones D24/187
2006/0199425 A1* 9/2006 Izuchi H04R 1/083
439/500
2012/0281977 A1* 11/2012 Stevenson G03B 11/041
396/544

FOREIGN PATENT DOCUMENTS

KR 3020190000781 * 1/2020

OTHER PUBLICATIONS

Design, Development, and Operation of a Low-Intensity Focused
Ultrasound Pulsation (LIFUP) System for Clinical Use. Online,
published date Jan. 2021. Retrieved on Sep. 11, 2021 from URL:
<https://ieeexplore.ieee.org/stamp/stamp.jsp?arnumber=9131840>.*

(Continued)

Primary Examiner — Susan Bennett Hattan
Assistant Examiner — Omeed Agilee
(74) *Attorney, Agent, or Firm* — Schwabe Williamson &
Wyatt, PC


(57) **CLAIM**

We claim the ornamental design for a transducer holder, as
shown and described.

DESCRIPTION

FIG. 1 is a first perspective view of a transducer holder,
showing our new design;
FIG. 2 is a left side view thereof;
FIG. 3 is a right side view thereof;
FIG. 4 is a rear view thereof;
FIG. 5 is a front view thereof;
FIG. 6 is a top view thereof;
FIG. 7 is a bottom view thereof;
FIG. 8 is a second perspective view thereof; and,
FIG. 9 is a cross-sectional view thereof, taken along line 9-9
in FIG. 6.

1 Claim, 7 Drawing Sheets

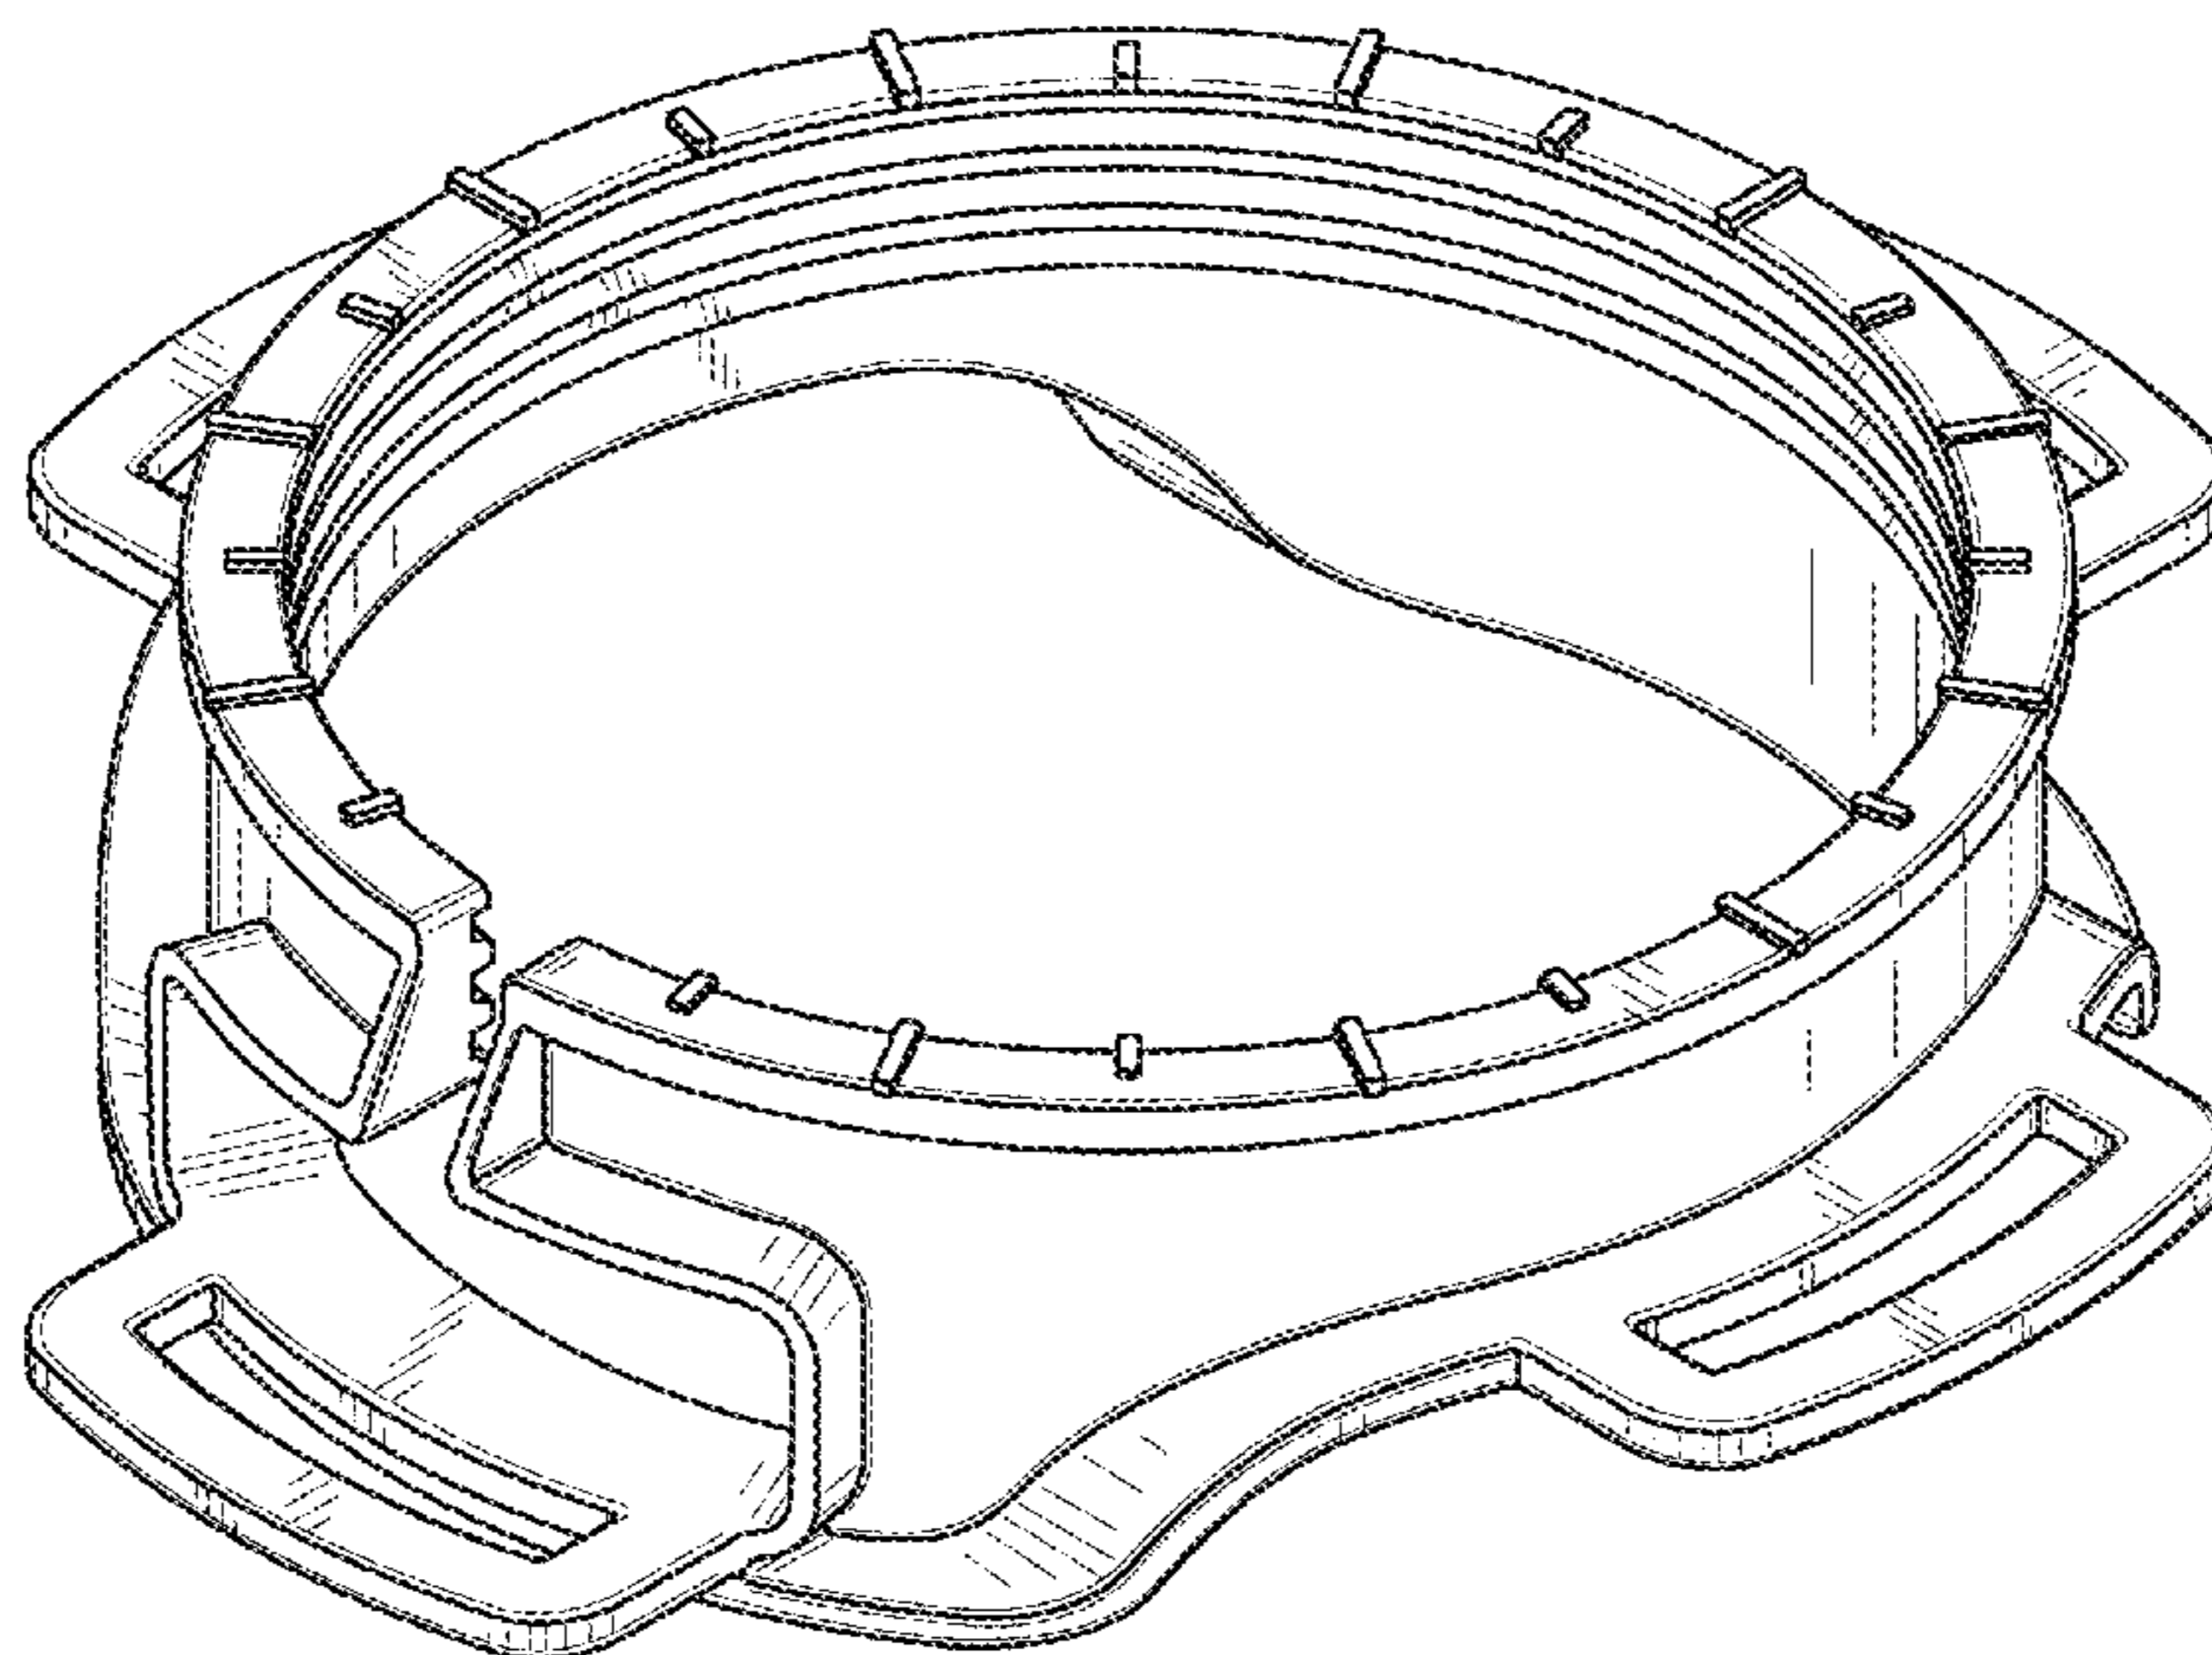

(56)

References Cited

OTHER PUBLICATIONS

MIT Open Access Article. Published date unknown. Retrieved on Sep. 11, 2021 from URL: <https://dspace.mit.edu/bitstream/handle/1721.1/84552/Ultrasound%20Probe%20Sheather%20for%20Publication%20Submission%2011%2022%2013.pdf?sequence=1&isAllowed=y>.*

* cited by examiner

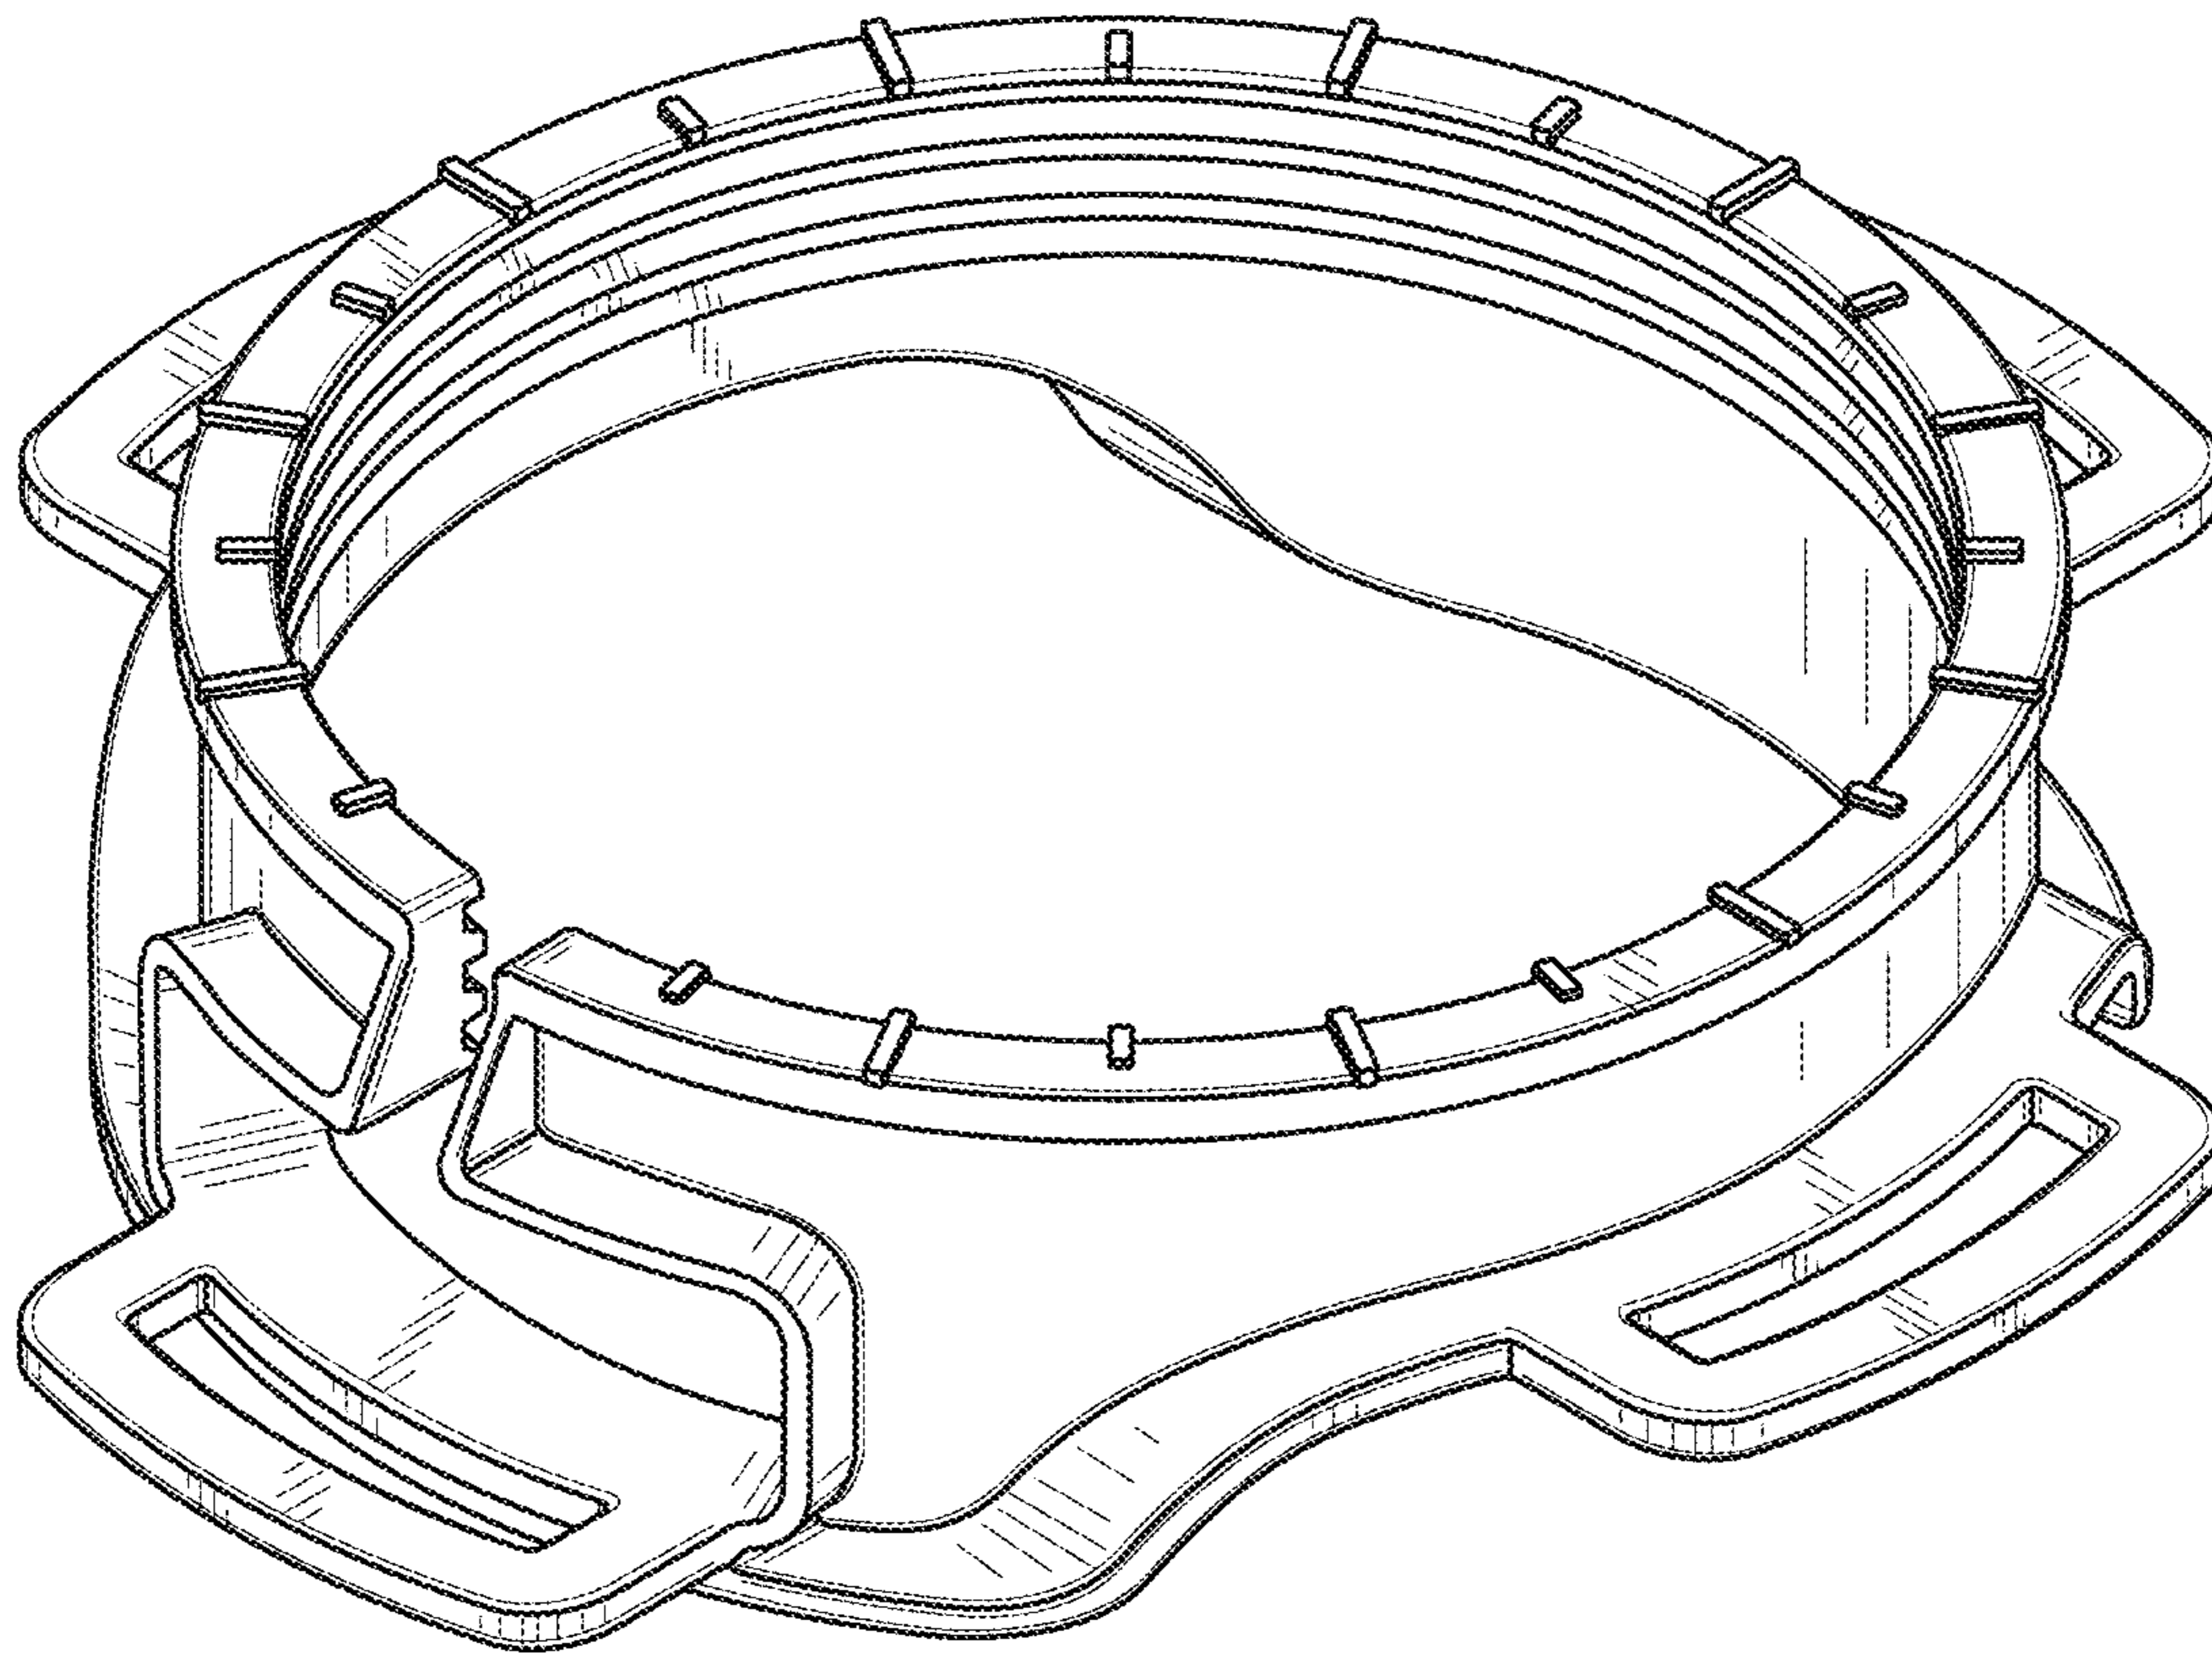


FIG. 1

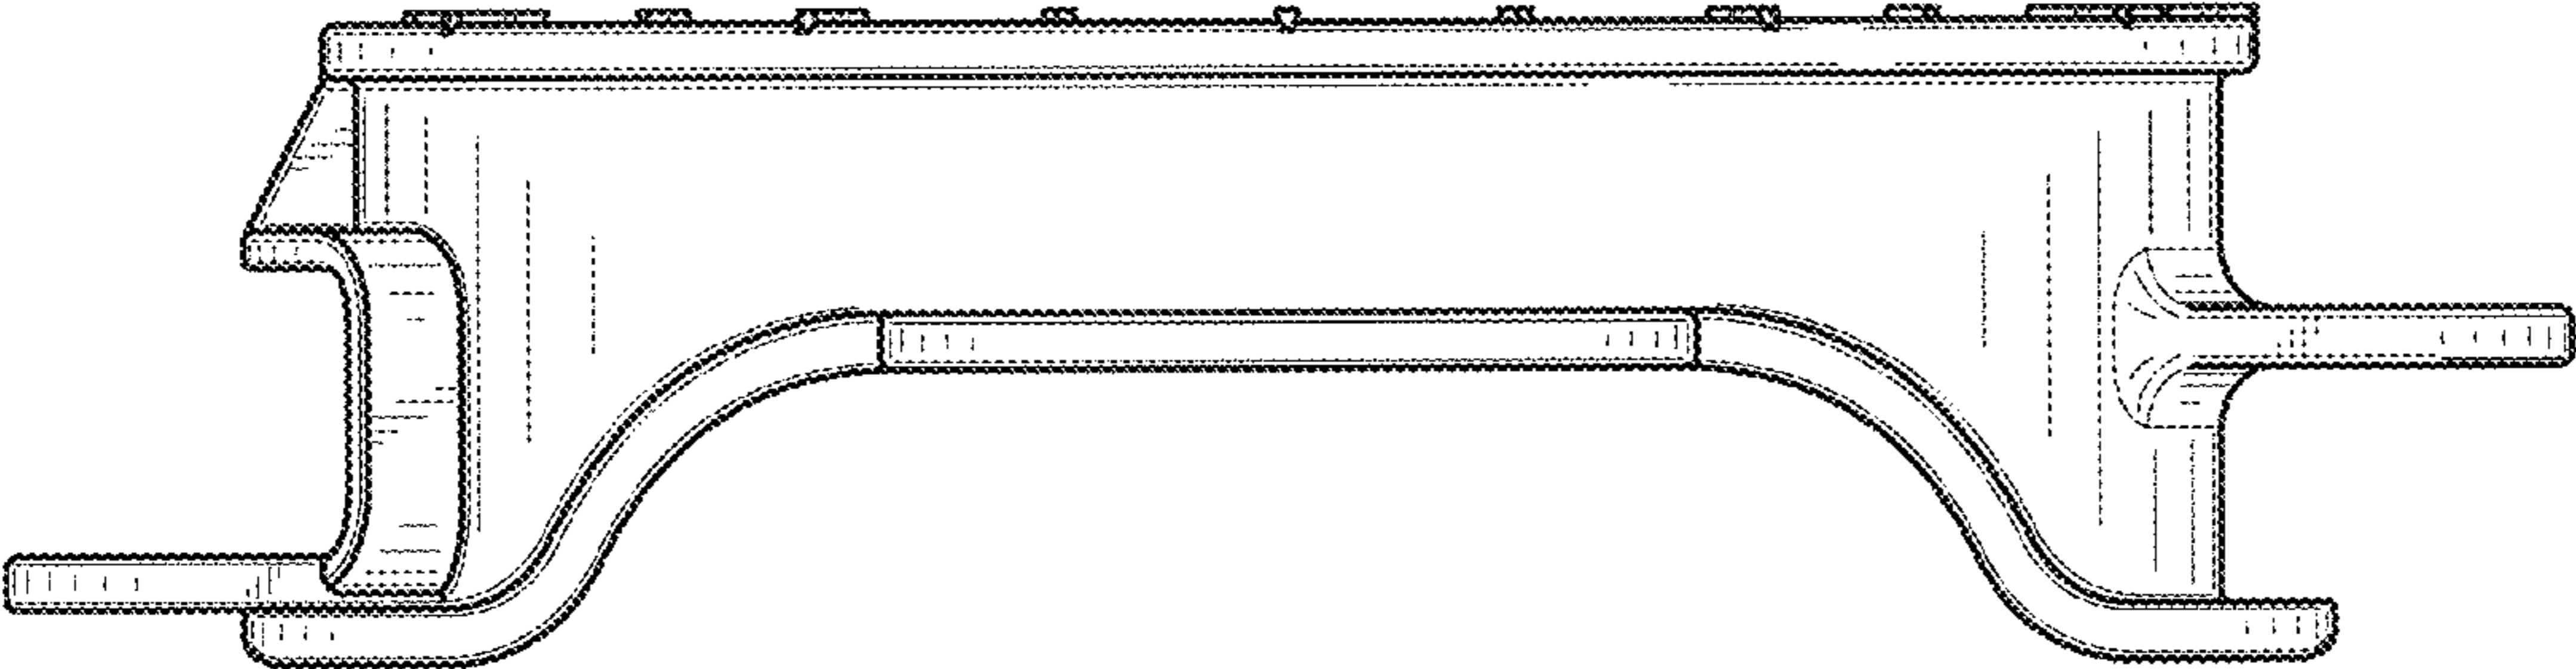


FIG. 2

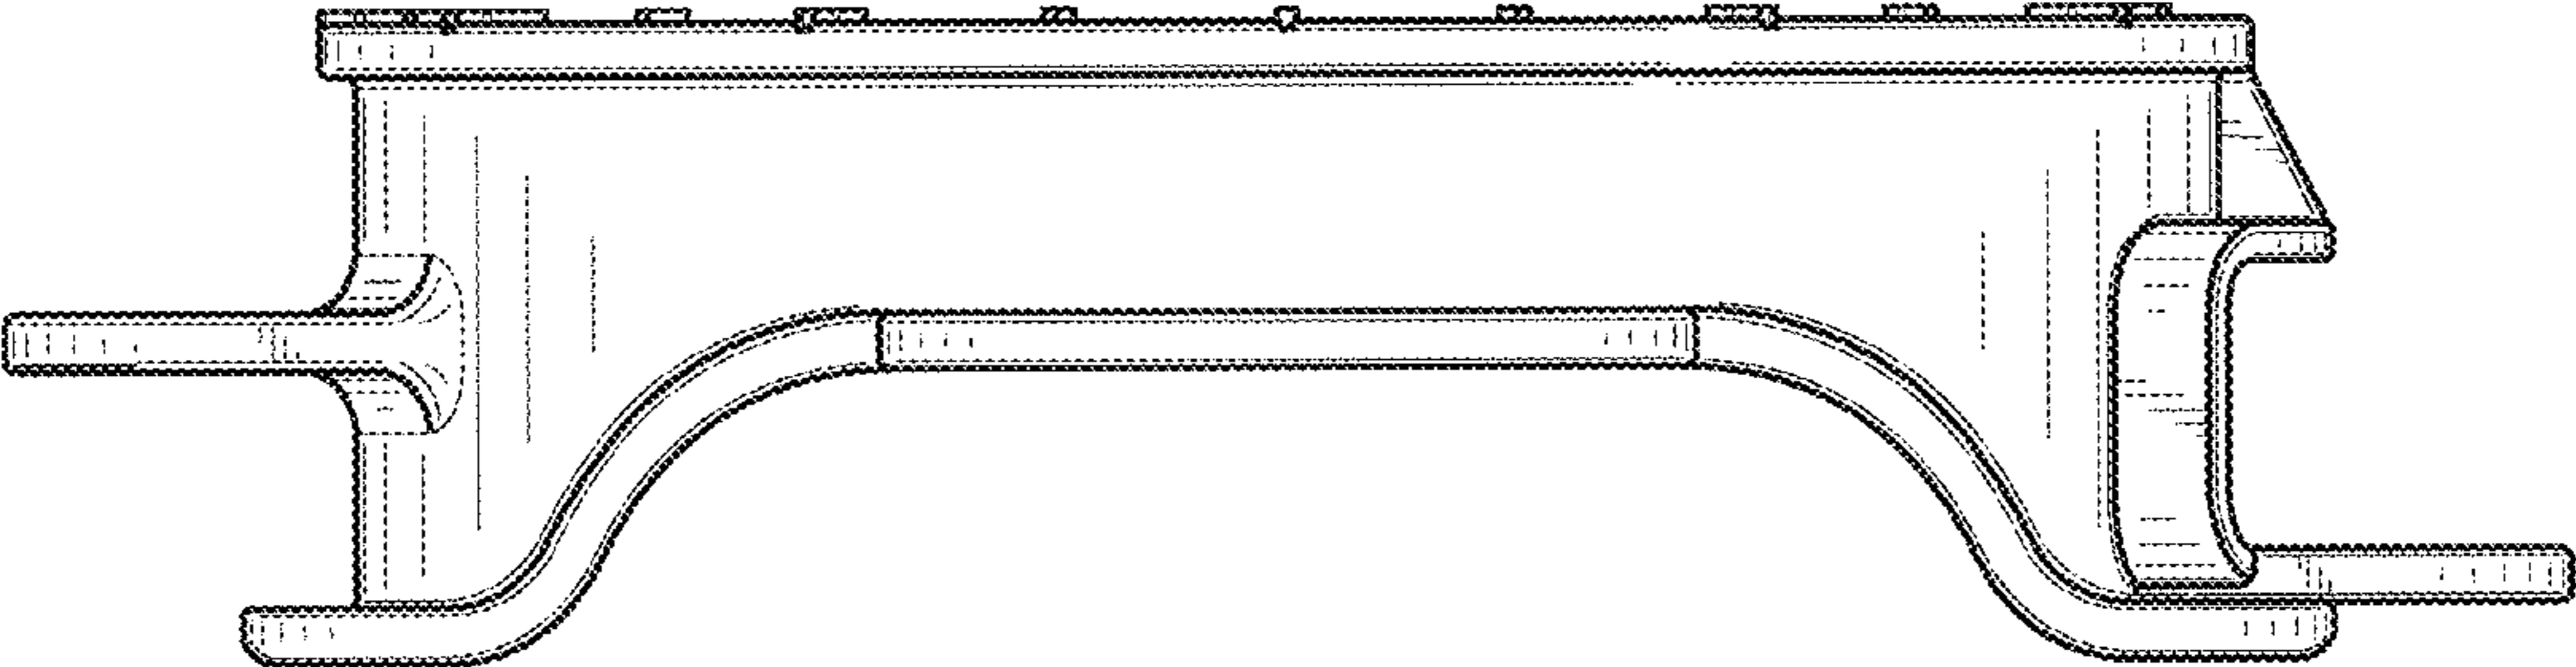


FIG. 3

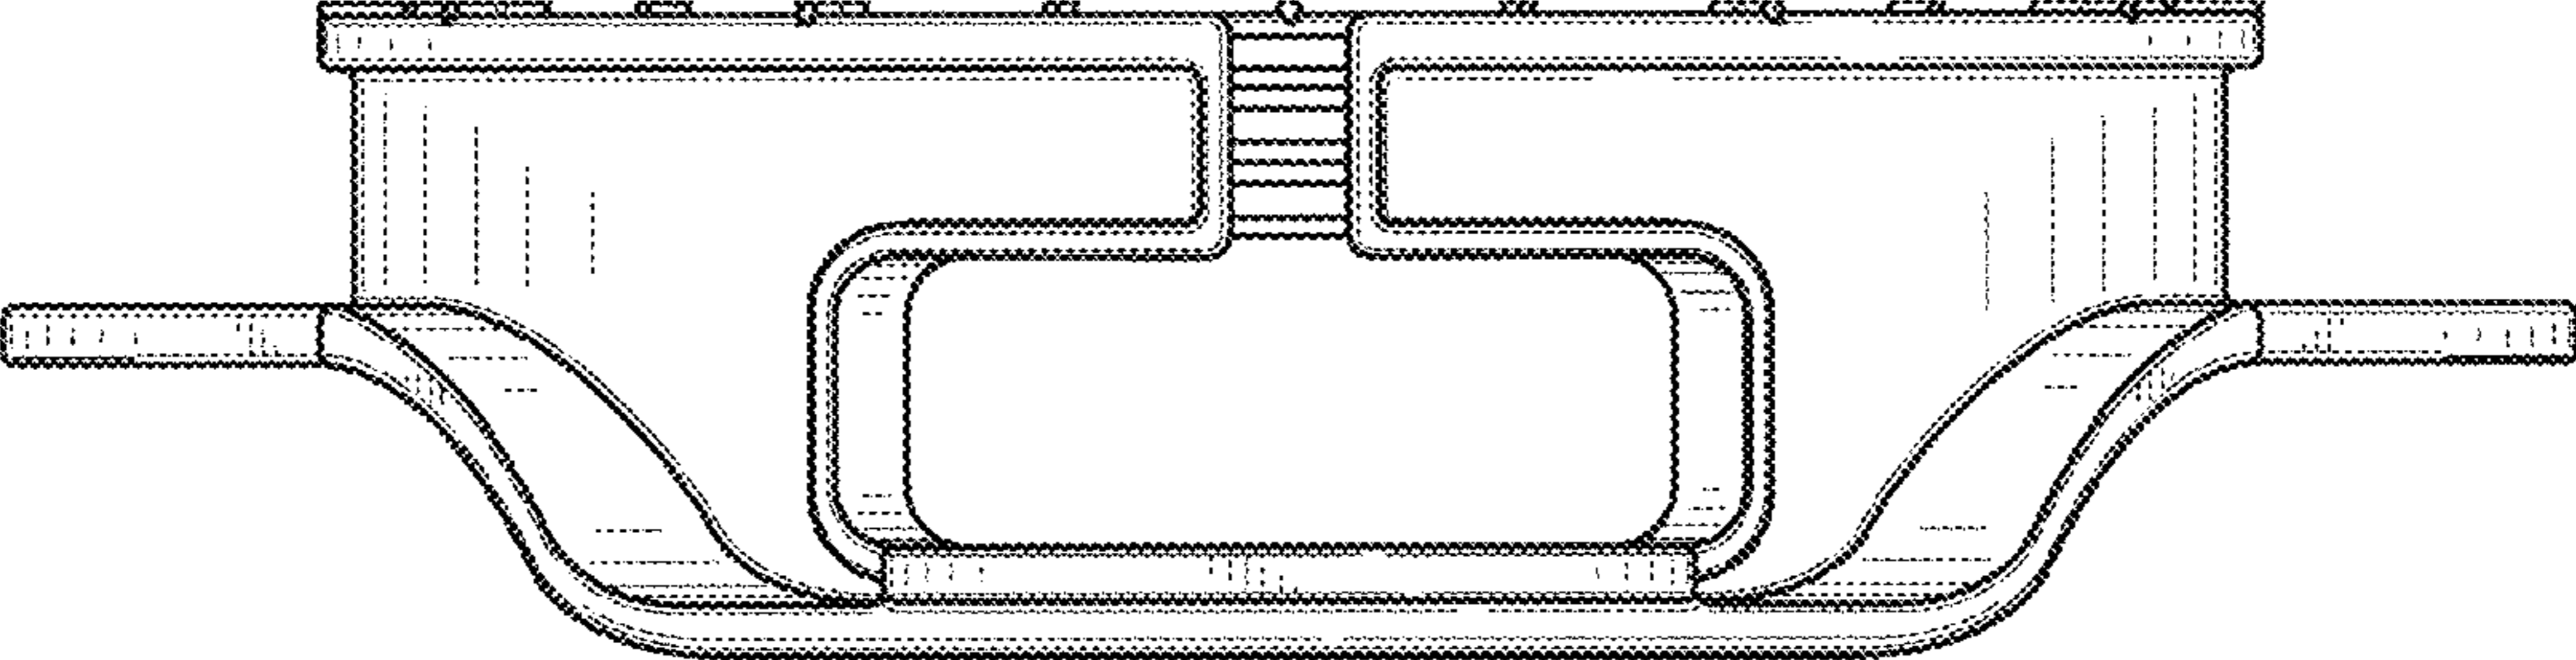


FIG. 4

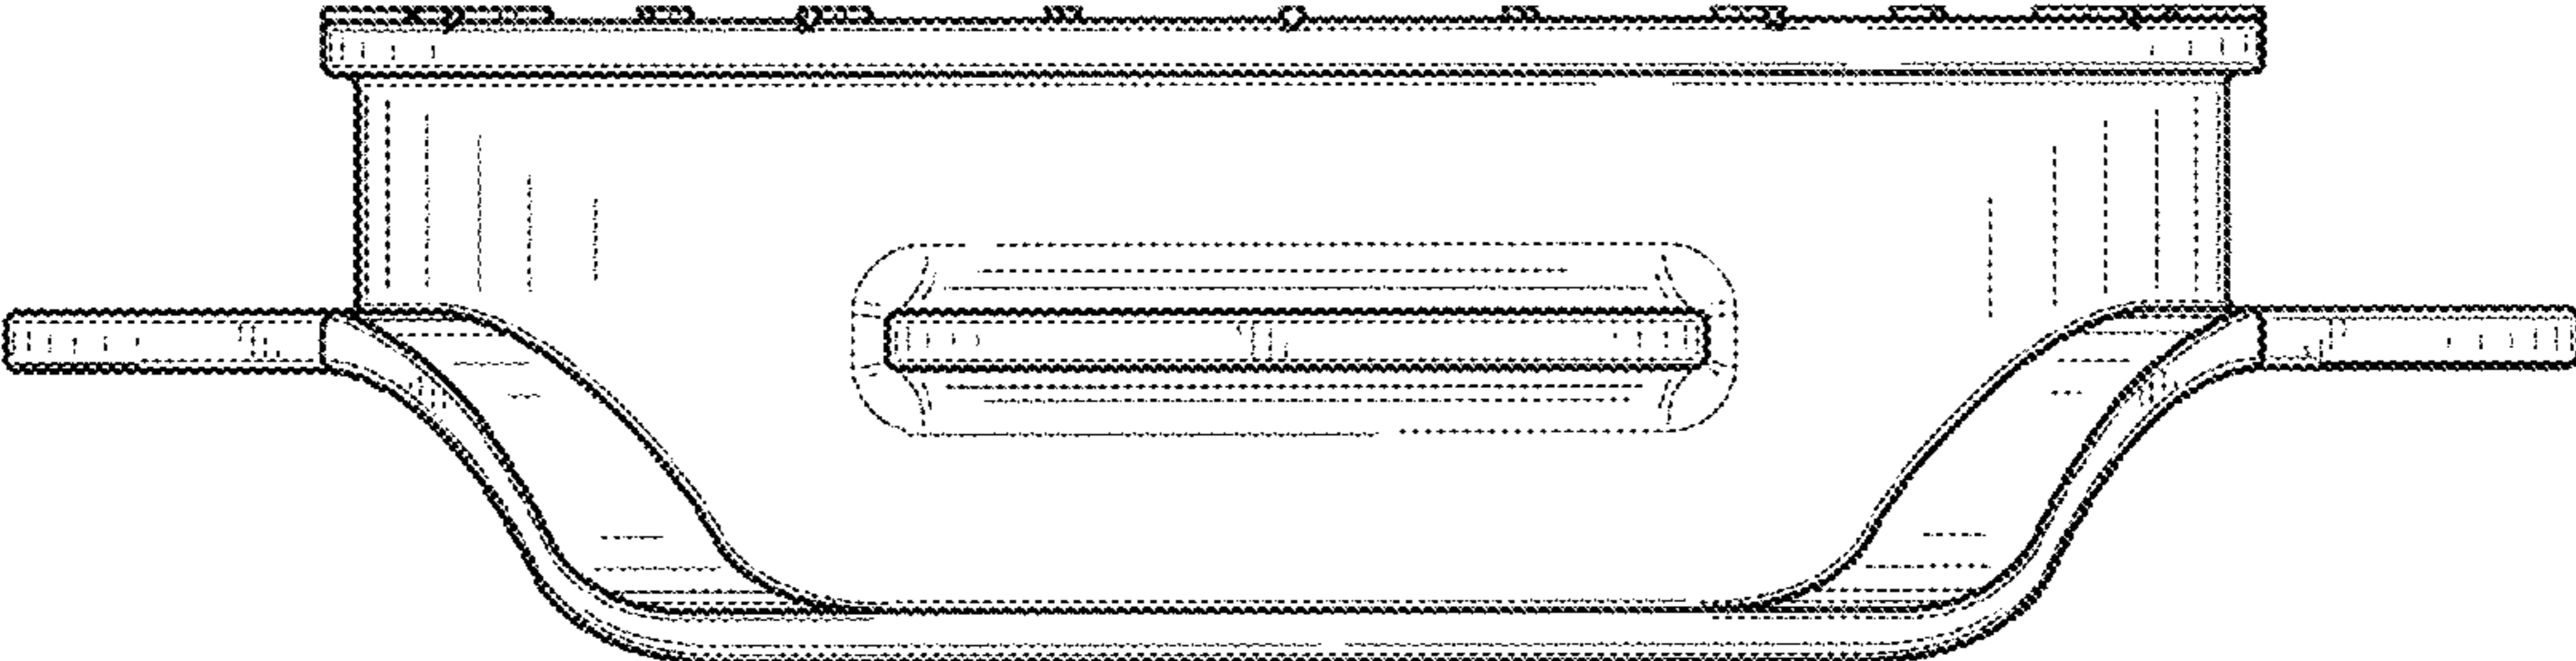


FIG. 5

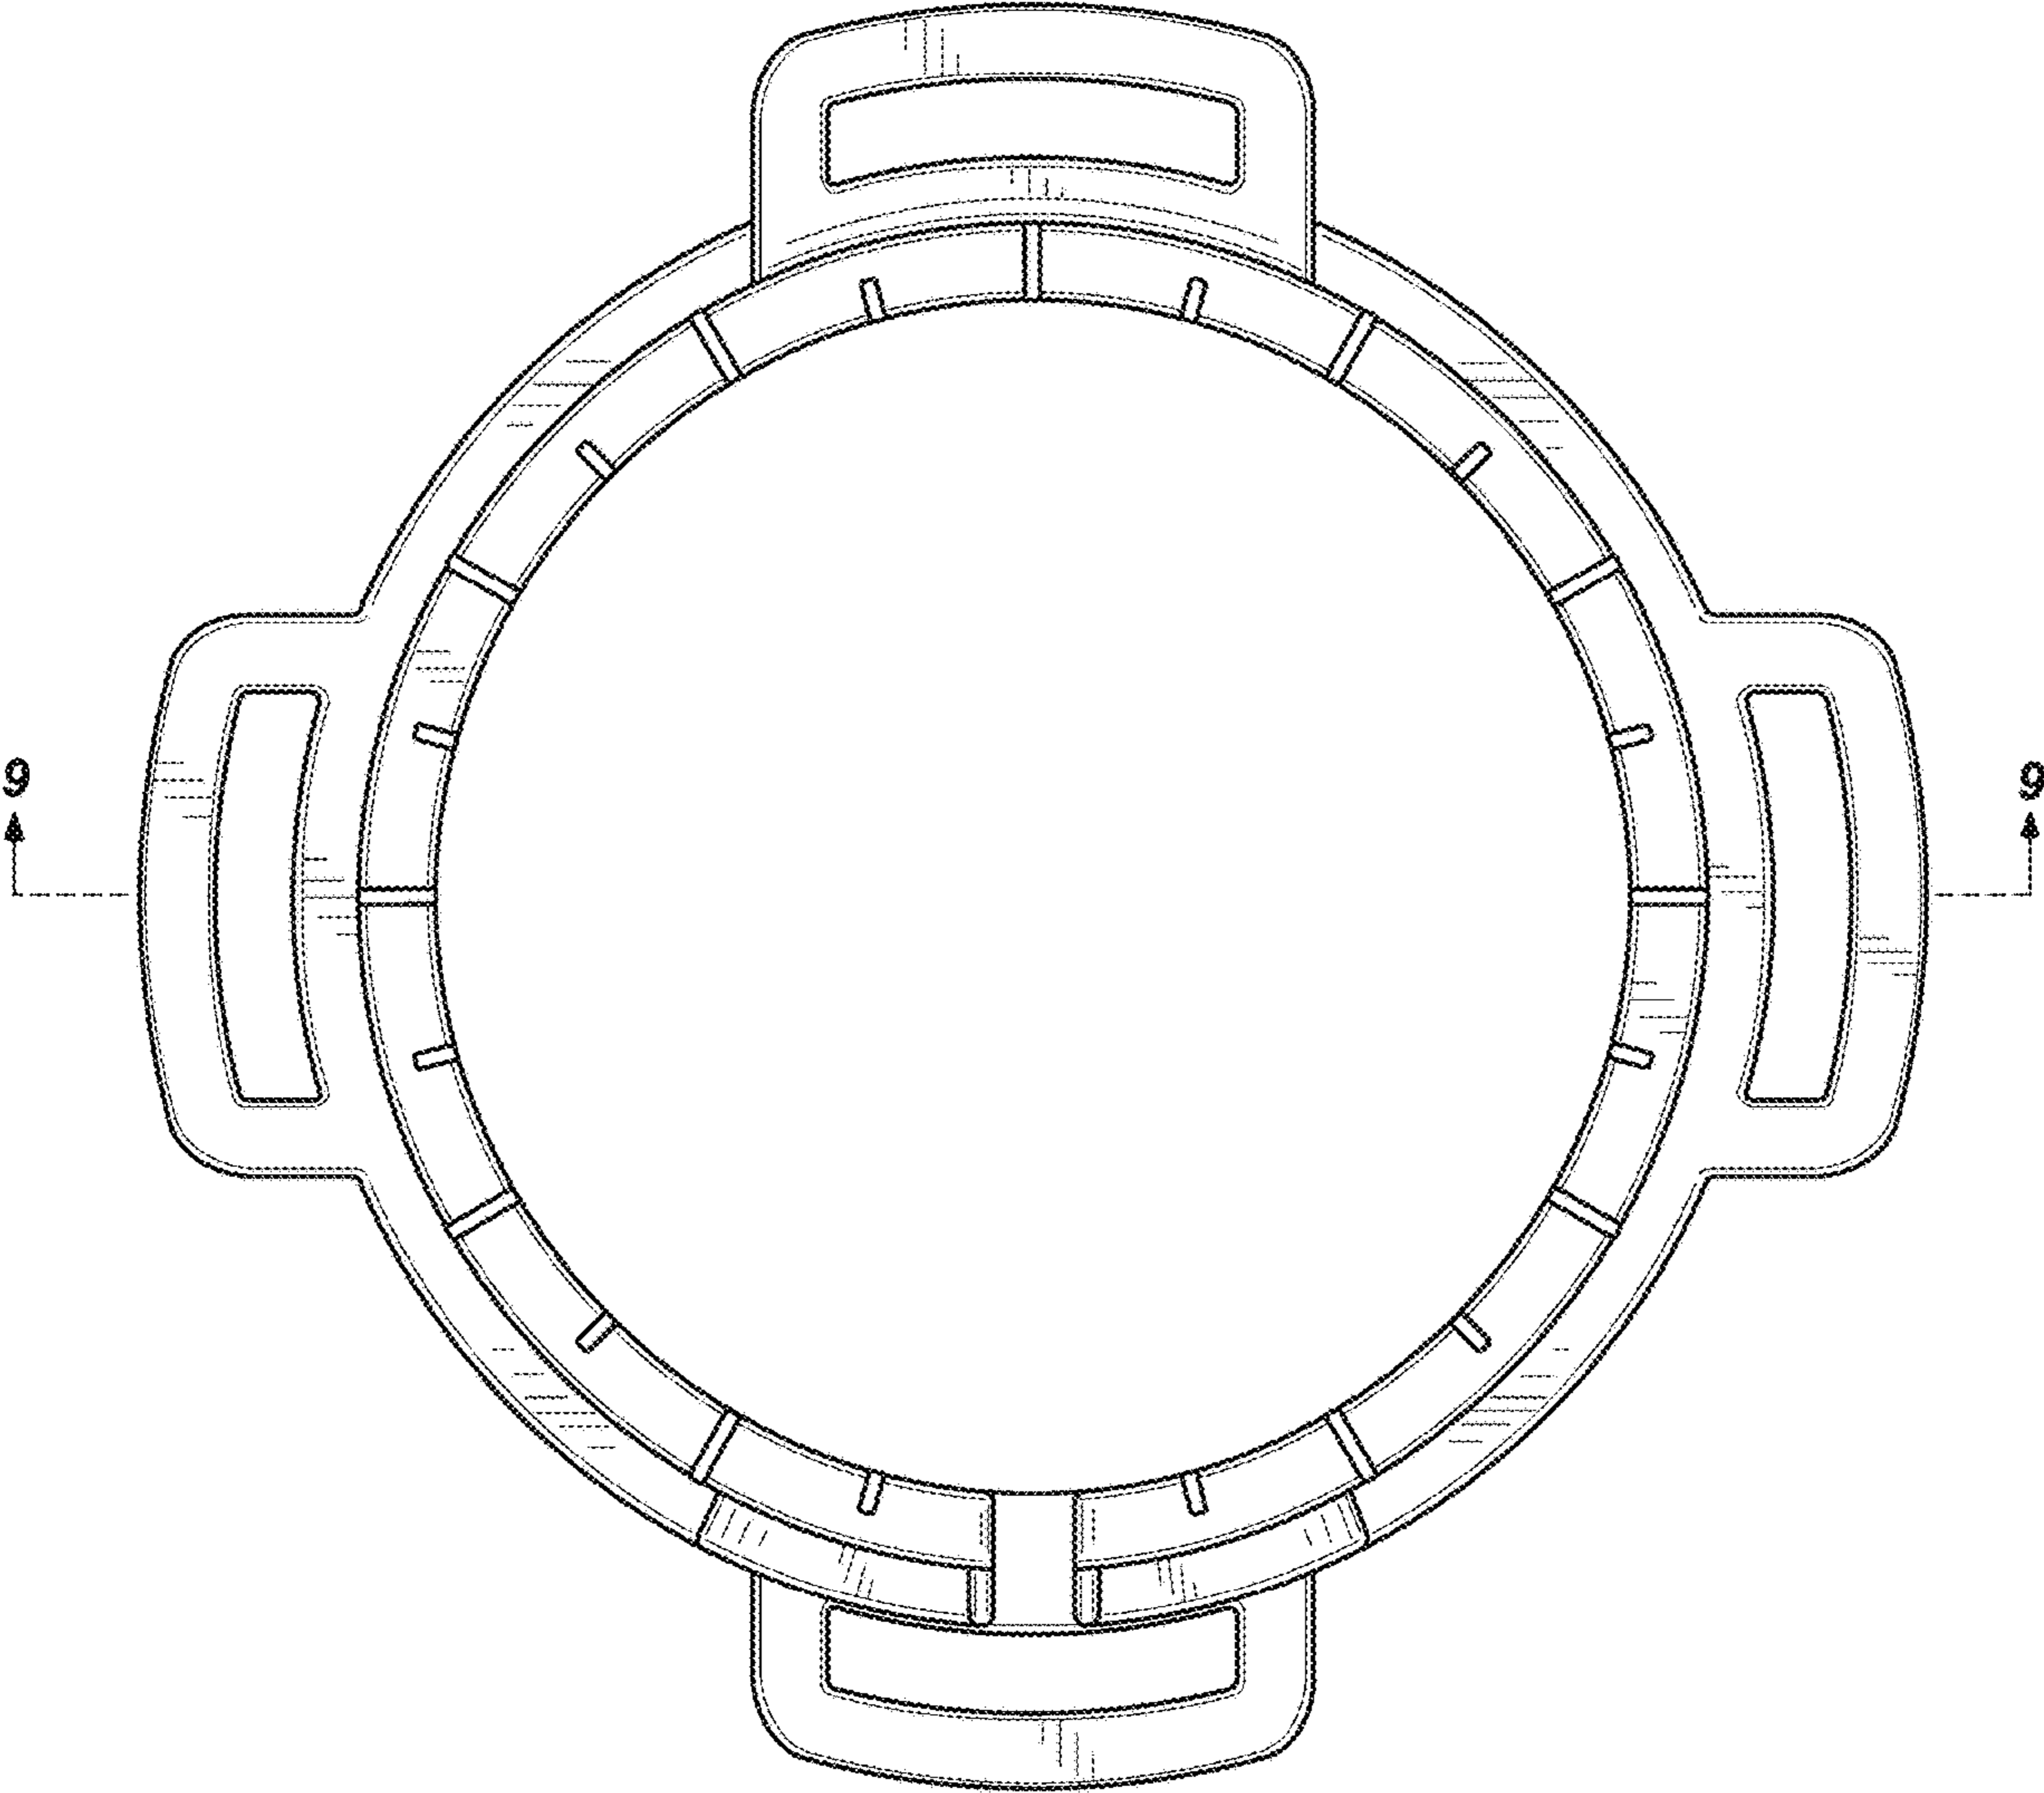


FIG. 6

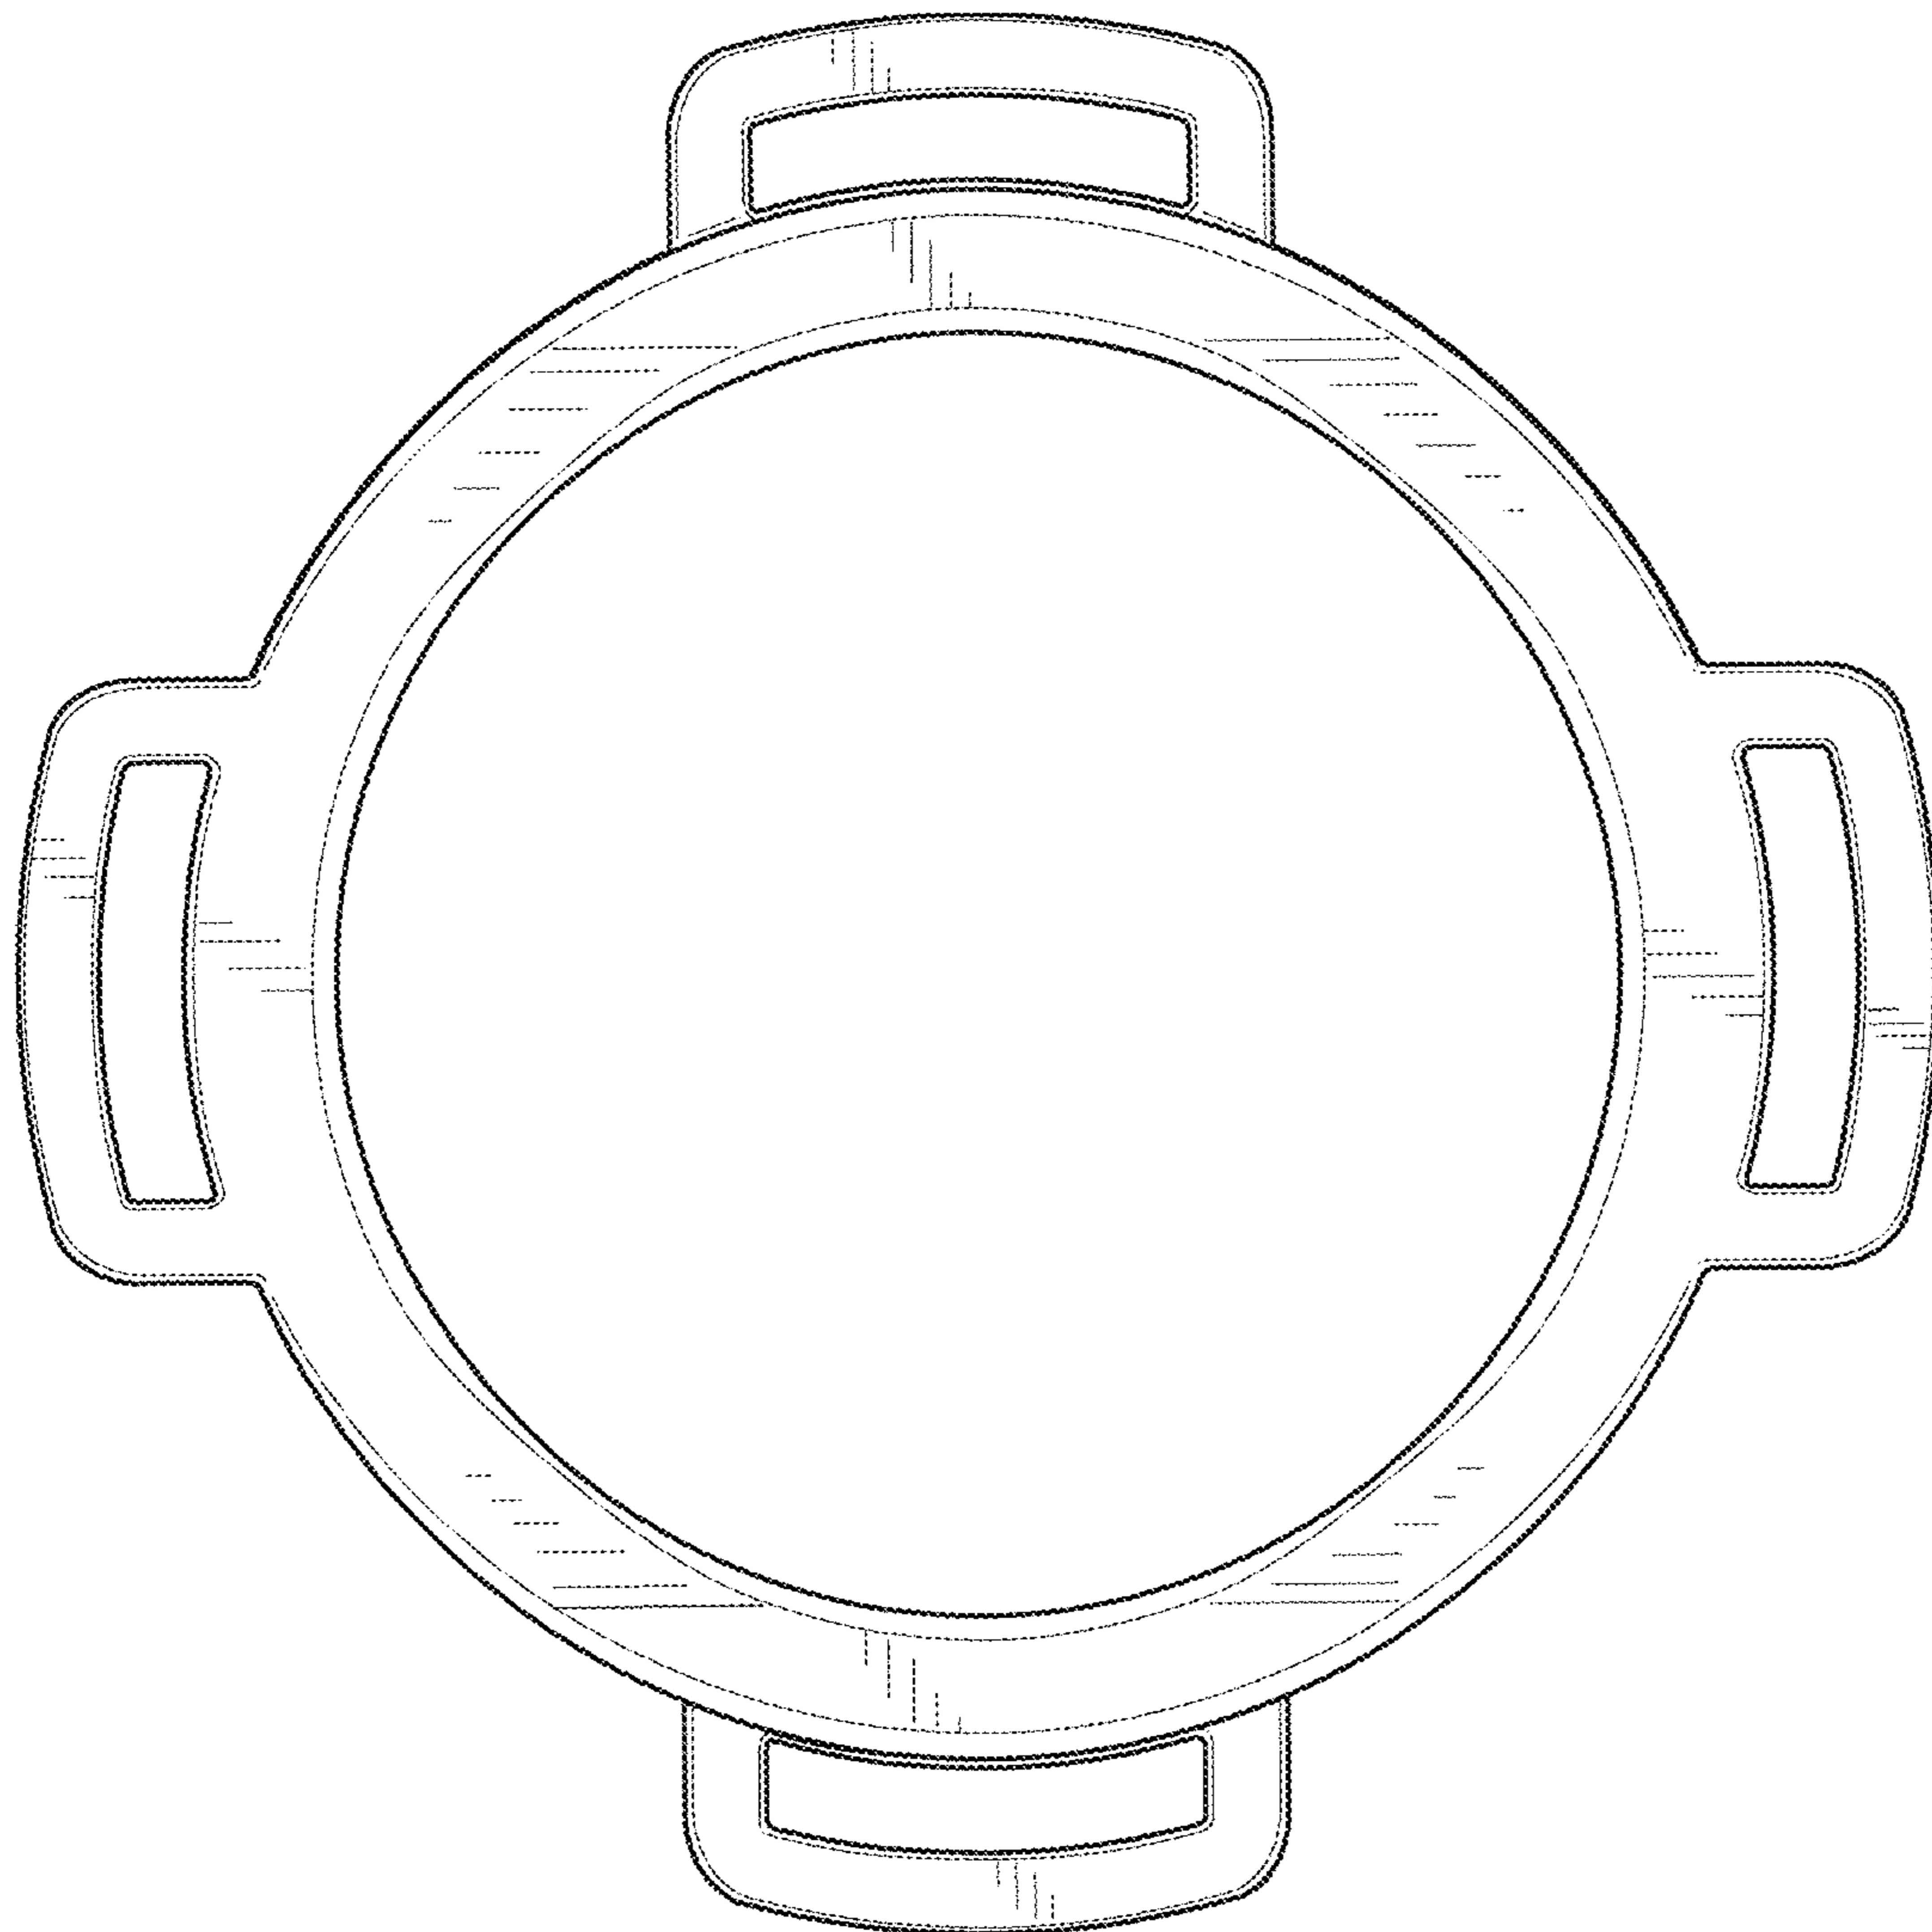


FIG. 7

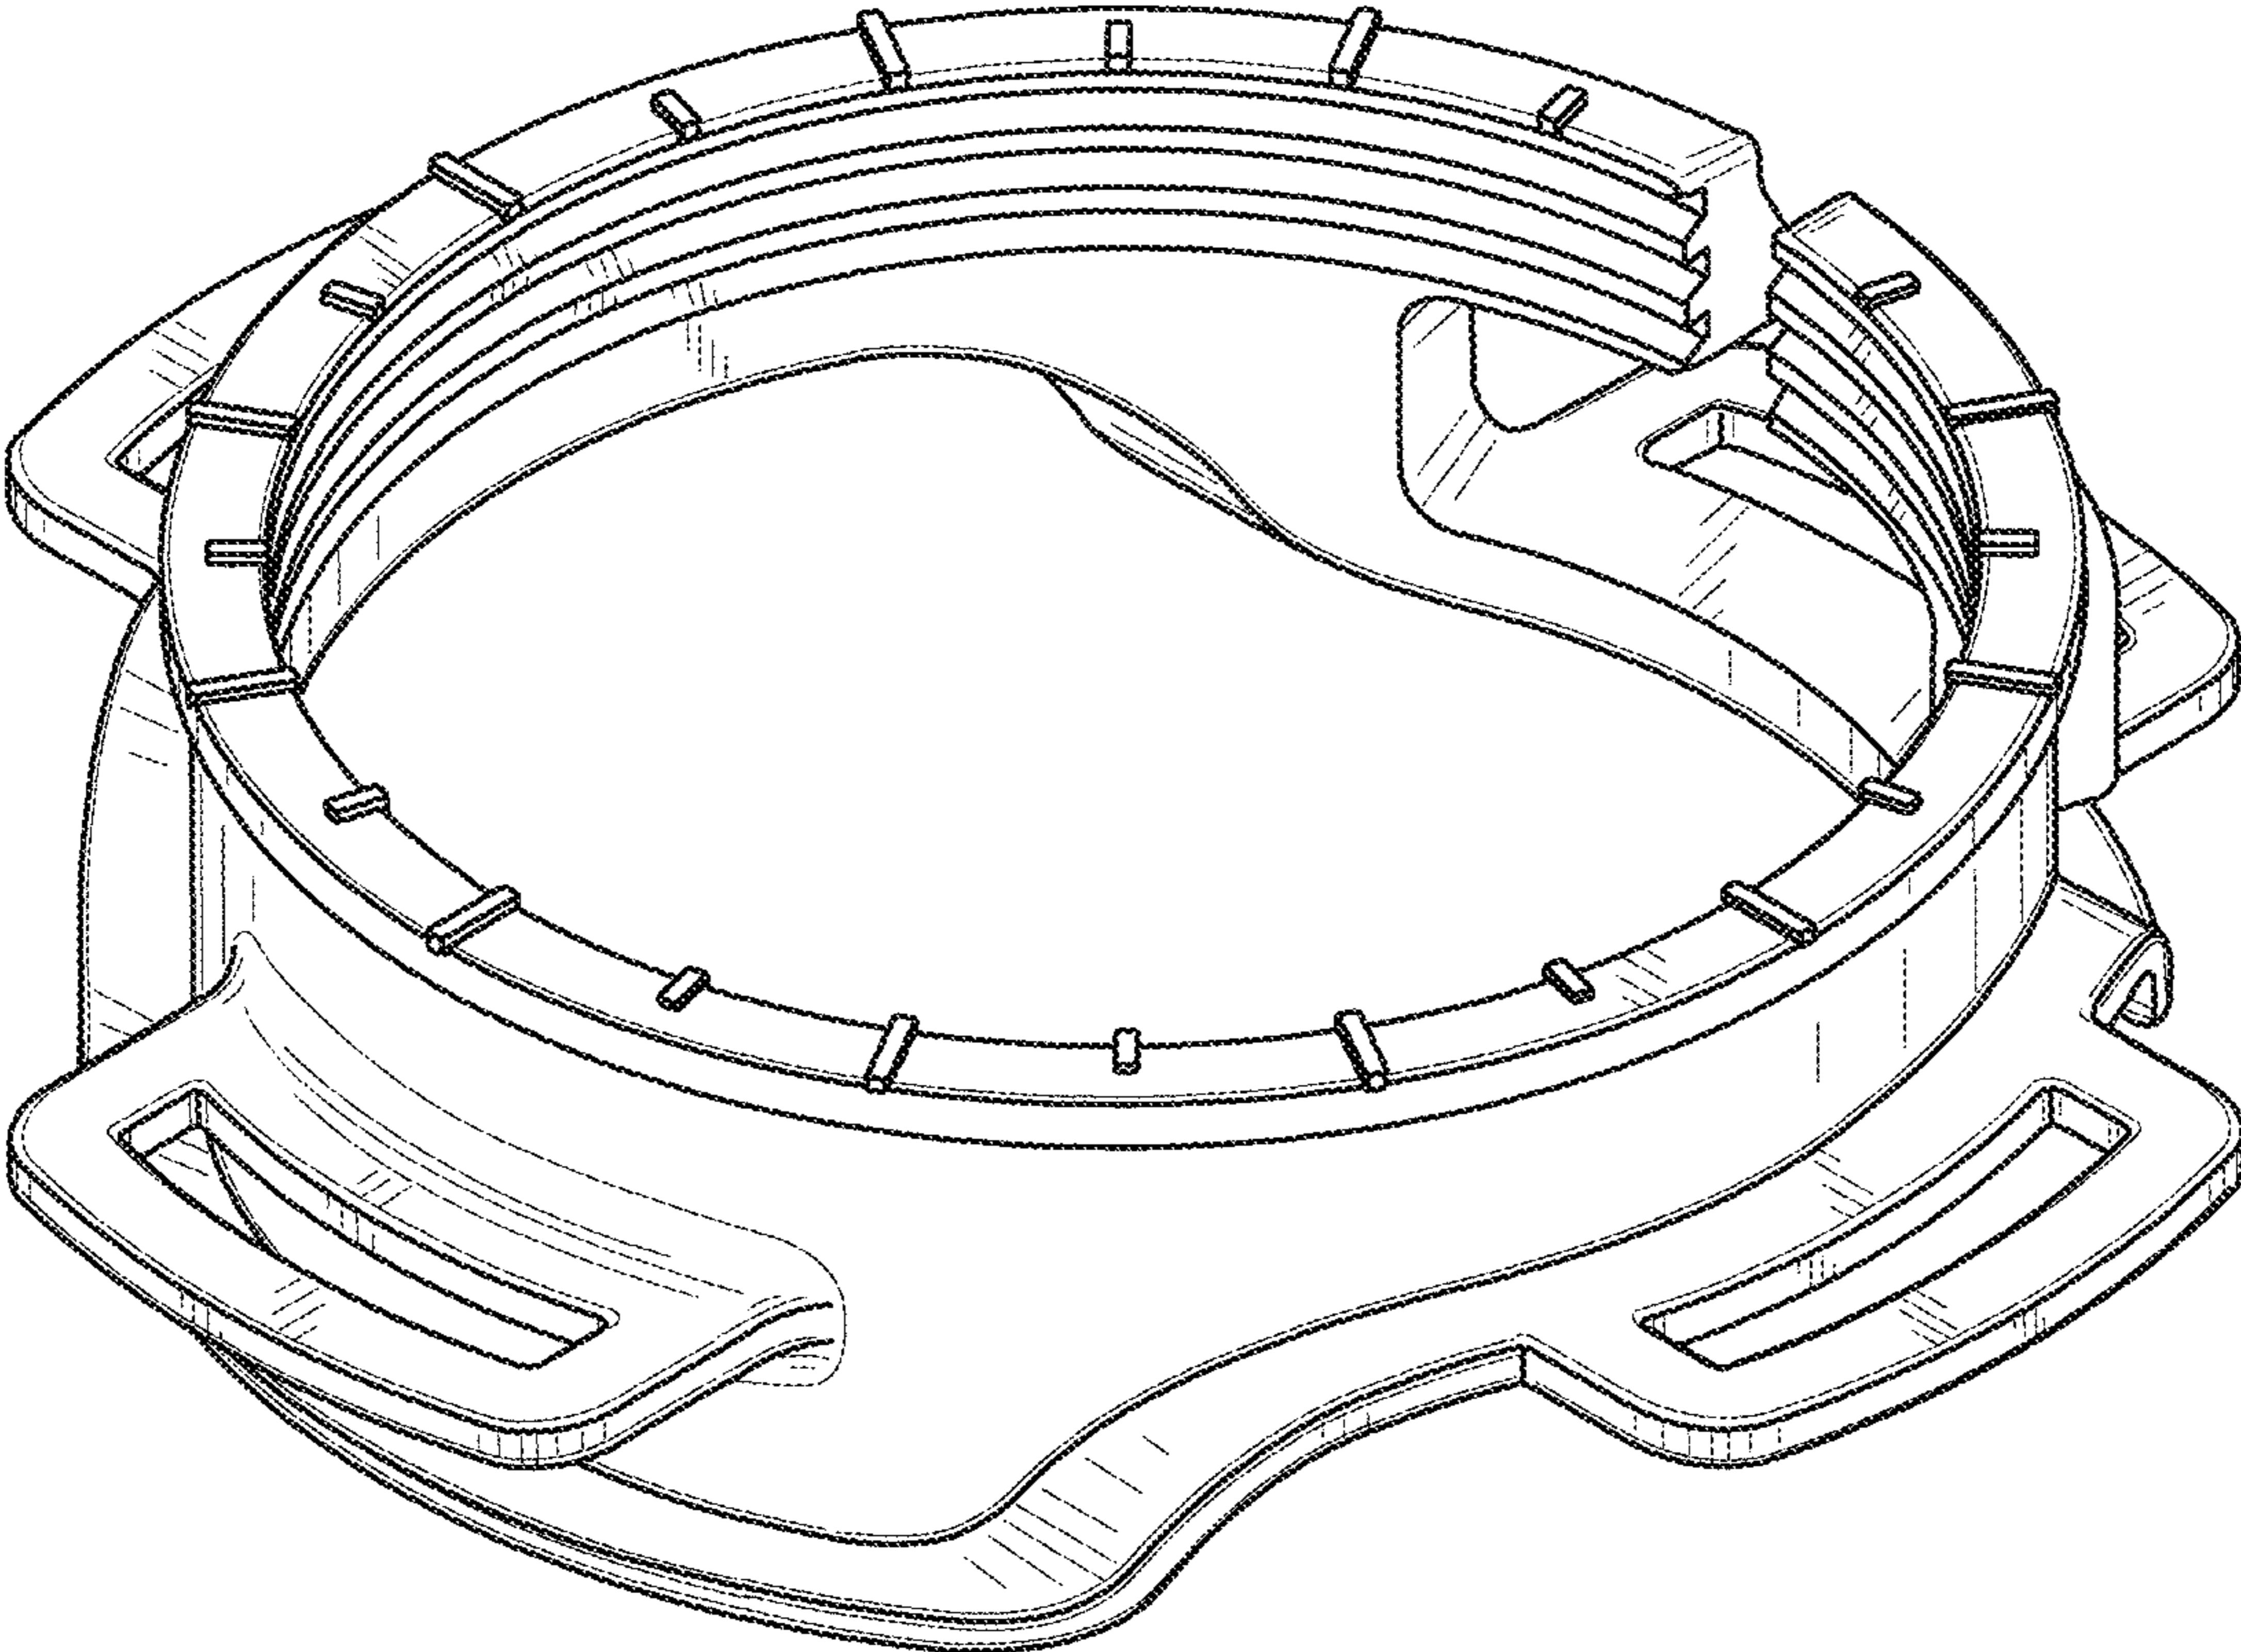


FIG. 8

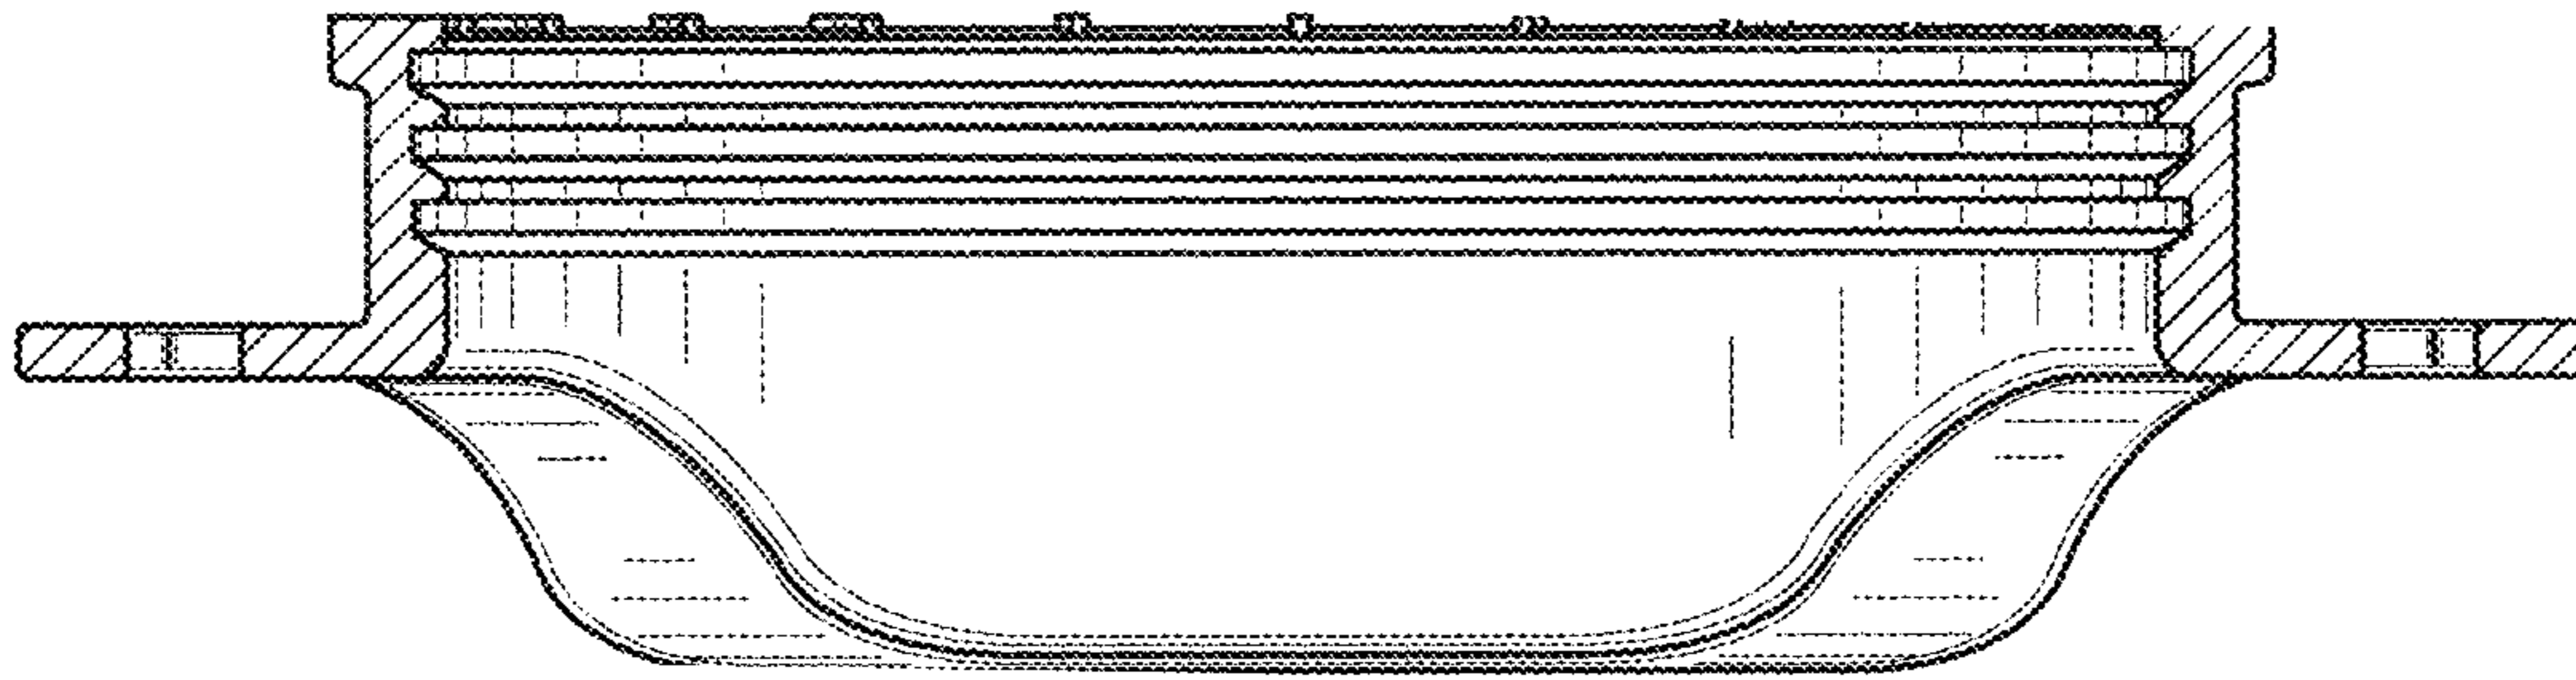


FIG. 9