

US00D946755S

(12) **United States Design Patent** (10) **Patent No.:** **US D946,755 S**
Diaz Mecchia et al. (45) **Date of Patent:** **** Mar. 22, 2022**

(54) **EYE TESTING EQUIPMENT**

(71) Applicant: **BRILL ENGINES, S.L.**, Barcelona (ES)

(72) Inventors: **Eva Diaz Mecchia**, Barcelona (ES);
Laura Nieto Cavia, Barcelona (ES)

(73) Assignee: **BRILL ENGINES, S.L.**, Barcelona (ES)

(**) Term: **15 Years**

(21) Appl. No.: **29/720,829**

(22) Filed: **Jan. 16, 2020**

(30) **Foreign Application Priority Data**

Jul. 17, 2019 (EM) 006632634-0001

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**

USPC **D24/150**

(58) **Field of Classification Search**

USPC D6/522, 523, 525, 526, 553, 566; D8/49,
D8/51, 52, 59, 60, 64, 82, 85, 86, 95, 97,
D8/300, 303, 349, 499; D14/372;
D15/138, 139; D16/100, 130, 309;
D24/108, 112, 113, 114, 115, 119, 127,
D24/128, 129, 130, 133, 137, 142, 144,
D24/145, 146, 147, 148, 150, 155, 158,
D24/160, 170, 171, 172, 173, 181, 185,
D24/186, 188, 200, 215, 216, 222, 231,
D24/232; D25/38.1, 41.1; D10/57

CPC A61B 3/00; A61B 3/0016; A61B 3/0025;
A61B 3/0033; A61B 3/0041; A61B
3/0075; A61B 3/0083; A61B 3/0091;
A61B 3/02; A61B 3/10; A61B 3/1005;
A61B 3/12; A61B 3/13; A61B 3/18;
A61B 17/00; A61B 2017/00349; A61B
2017/00455; A61B 2017/00464; A61B
2017/00473; A61B 2017/0053; A61B
17/0057; A61B 17/0231; A61B 17/04;

A61B 17/064; A61B 17/0642; A61B
17/0643; A61B 17/0644; A61B
2017/0688; A61B 17/14; A61B 17/142;
A61B 17/15; A61B 17/151; A61B
17/154; A61B 17/155; A61B 17/157;
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D329,092 S * 9/1992 Carusillo D24/146
D364,463 S * 11/1995 Pitzen D24/146
(Continued)

OTHER PUBLICATIONS

Grafton Optical, "Dedicated Dry Eye Clinic", first available Oct.
2018. (https://a1288510-a5b4-40cb-aba1-70bc25412541.filesusr.com/Ugd/6ce74b_fecde9e5d5964f80b3414b24fcdc4d66.pdf) (Year:
2018).*

(Continued)

Primary Examiner — Lauren D McVey

Assistant Examiner — Justin A Johnson

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(57) **CLAIM**

The ornamental design for an eye testing equipment, as
shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of an eye testing equip-
ment.

FIG. 2 is a front elevation view thereof.

FIG. 3 is a left side elevation view thereof.

FIG. 4 is a rear elevation view thereof.


FIG. 5 is a right side elevation view thereof.

FIG. 6 is a top plan view thereof.

FIG. 7 is a bottom plan view thereof; and,

FIG. 8 is a rear perspective view thereof.

1 Claim, 8 Drawing Sheets

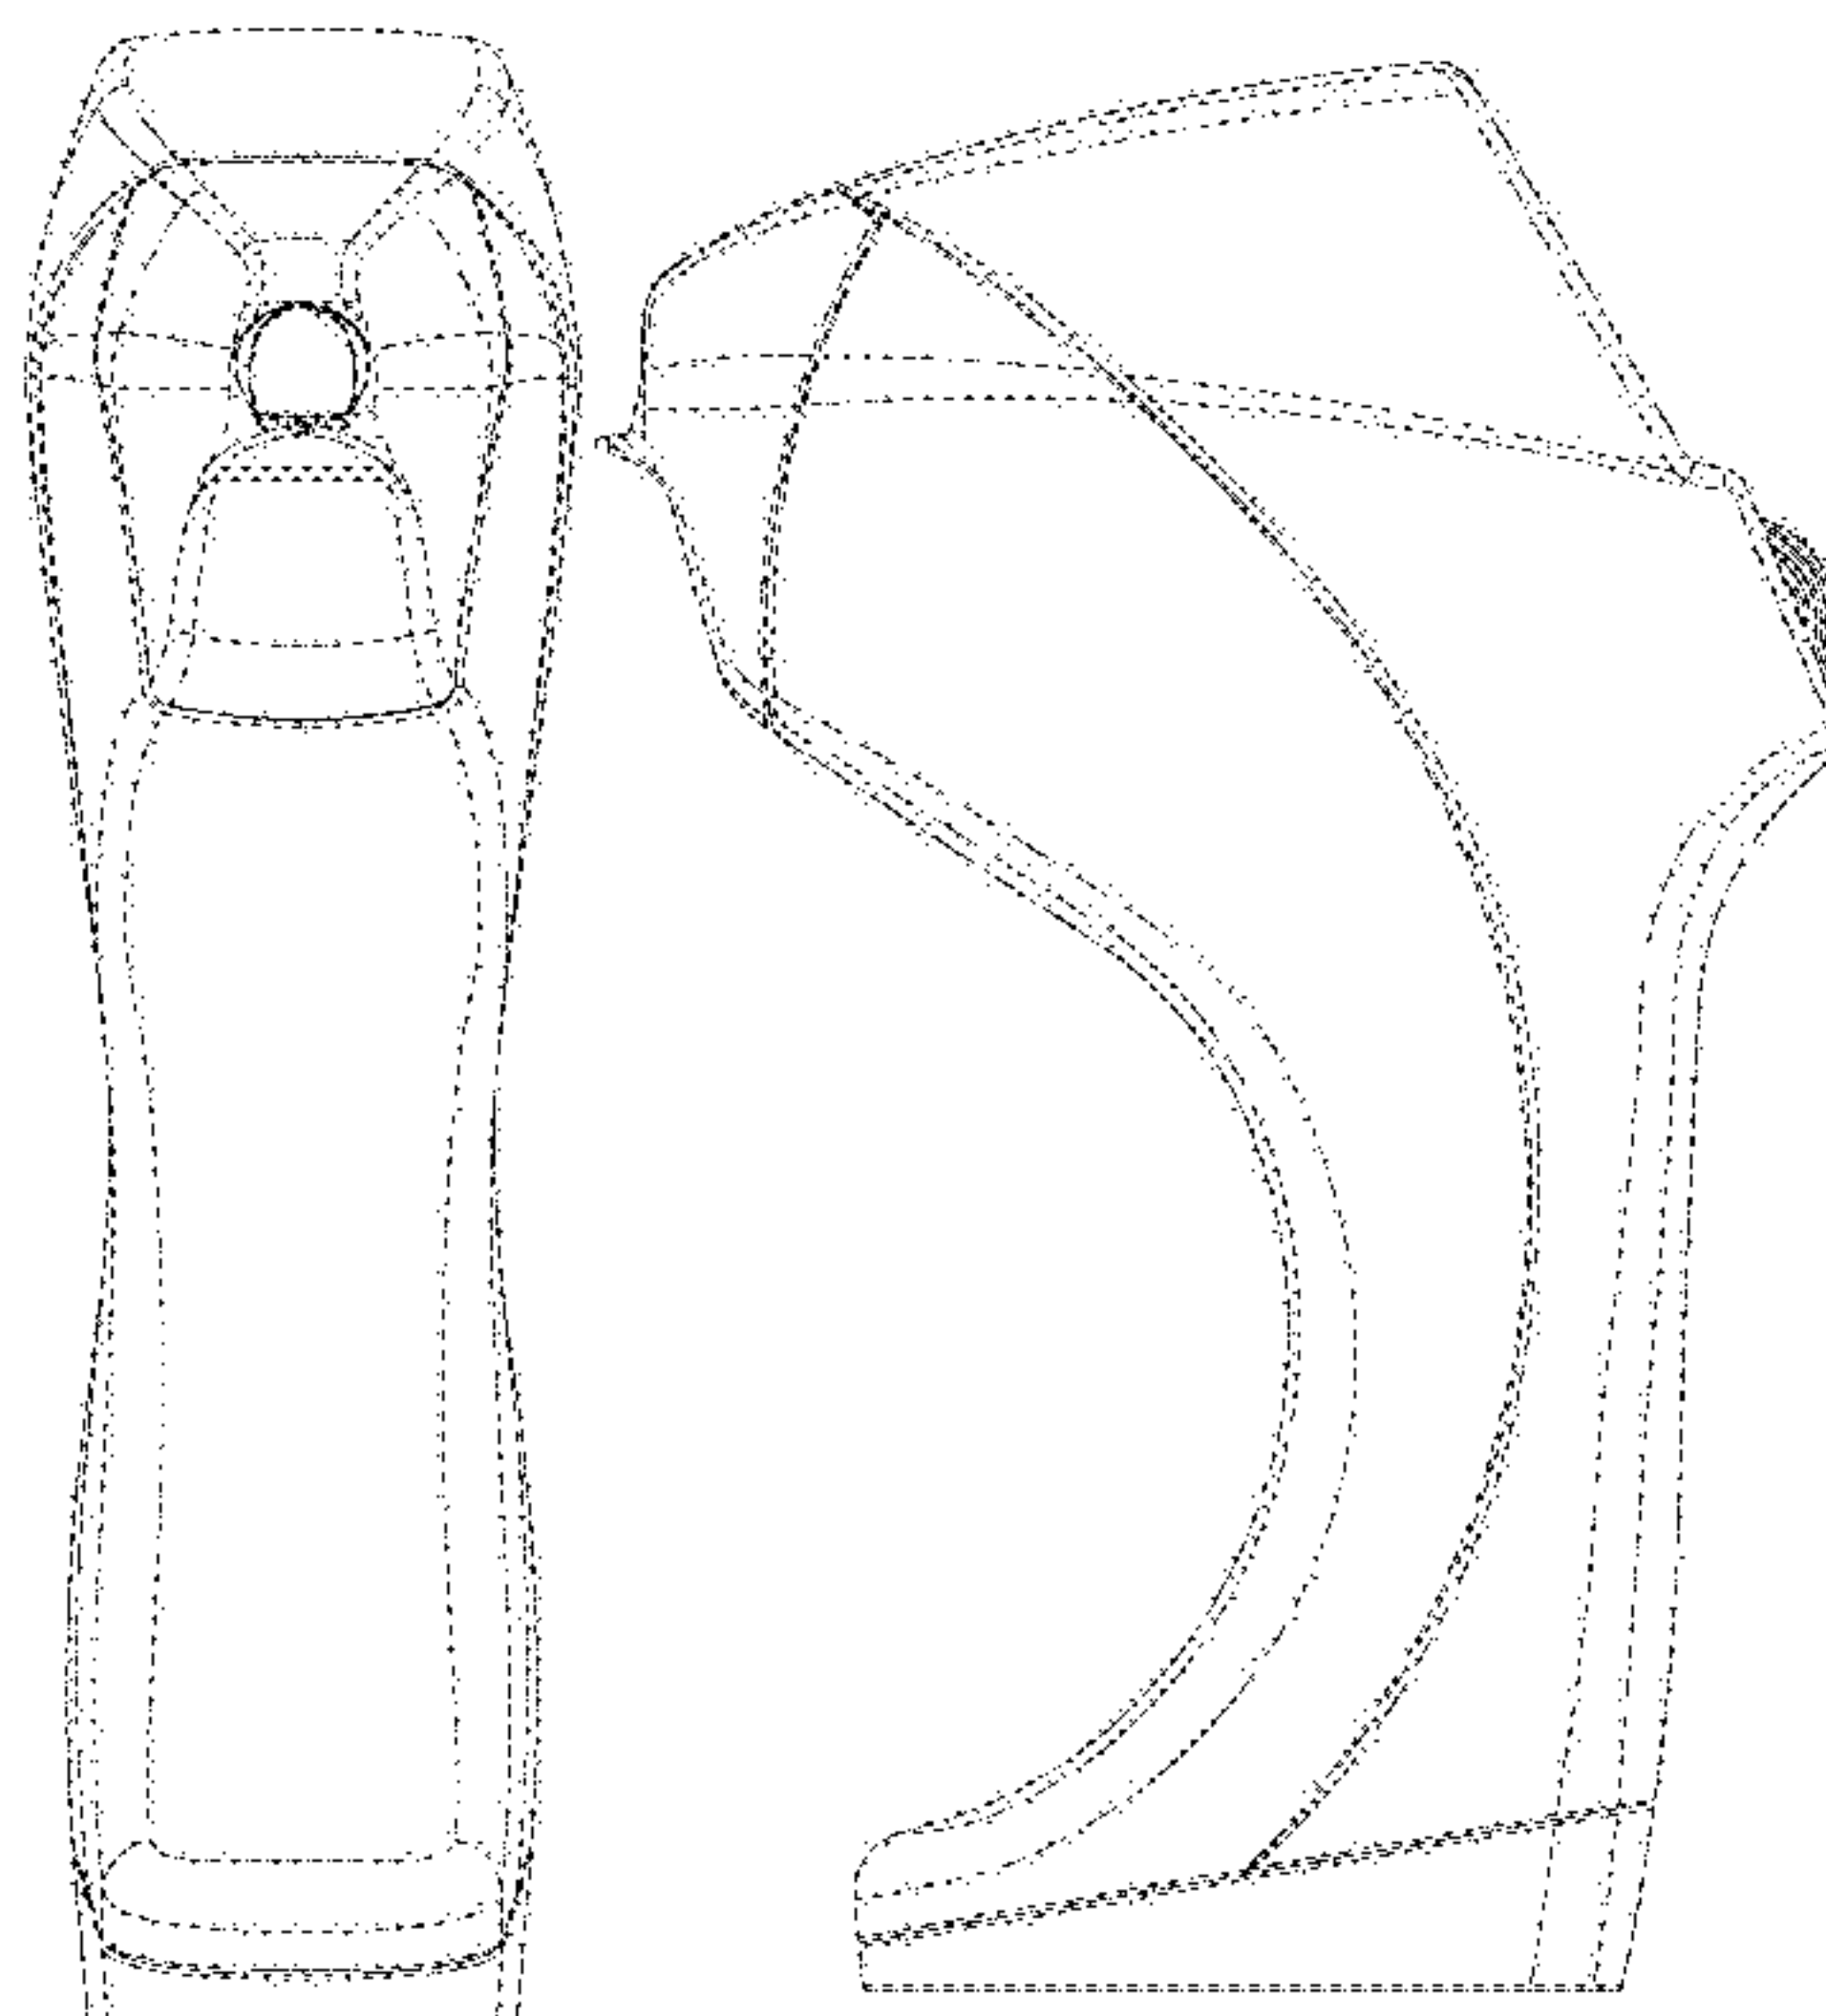

(58) Field of Classification Search

CPC ... A61B 17/158; A61B 17/16; A61B 17/1613;
A61B 17/1615; A61B 17/1617; A61B
2090/0817; A61B 2017/00663; A61B
17/0401; A61B 2017/0404; A61B 10/00;
A61B 10/02; A61B 2010/0208; A61B
10/04; A61B 2010/045; B23D 51/025;
A61F 9/00; A61F 9/007; A61F 9/0133;
A61F 2210/0004; E21B 10/00; A61H
2205/022; A61H 5/00; A61H 5/005;
B28B 7/00; B28B 7/0002; B28B 7/0032;
B28B 7/0094; B28B 7/16; B28B 7/18
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D457,443 S * 5/2002 Riester-Freudenmann ... D10/57
D473,652 S * 4/2003 Darley D24/173
D493,733 S * 8/2004 Chen H01J 37/165
D10/57

D589,650 S * 3/2009 Adriaenssen A61M 5/3273
D24/133
D597,206 S * 7/2009 Collins, Jr D24/150
D668,561 S * 10/2012 Dunkin G06K 7/10851
D10/57
D740,945 S * 10/2015 Booth D24/158
D877,338 S * 3/2020 Jones H01J 37/165
D24/158
D903,869 S * 12/2020 Noack D24/155
D917,313 S * 4/2021 Chen D10/57
2007/0057067 A1 * 3/2007 He G06K 7/10851
235/462.45
2018/0256209 A1 * 9/2018 Muse A61M 5/3273

OTHER PUBLICATIONS

Welch Allyn, “RETeval-DR”, first available Feb. 2018. (<https://ophthalmic.com.sg/Download/80020080LITPDF.pdf>) (Year: 2018).*
Instagram, “reicherteye”, first available Mar. 26, 2020. (<https://www.instagram.com/p/B-Lw3NqBc88/>) (Year: 2020).*
Dot Med, “Reichert PT 100 Hand Held NCT Tonometer”, first available May 20, 2021. (<https://www.dotmed.com/listing/tonometer-tono-pen/reichert/pt-100-hand-held-nct/2120949>) (Year: 2021).*

* cited by examiner

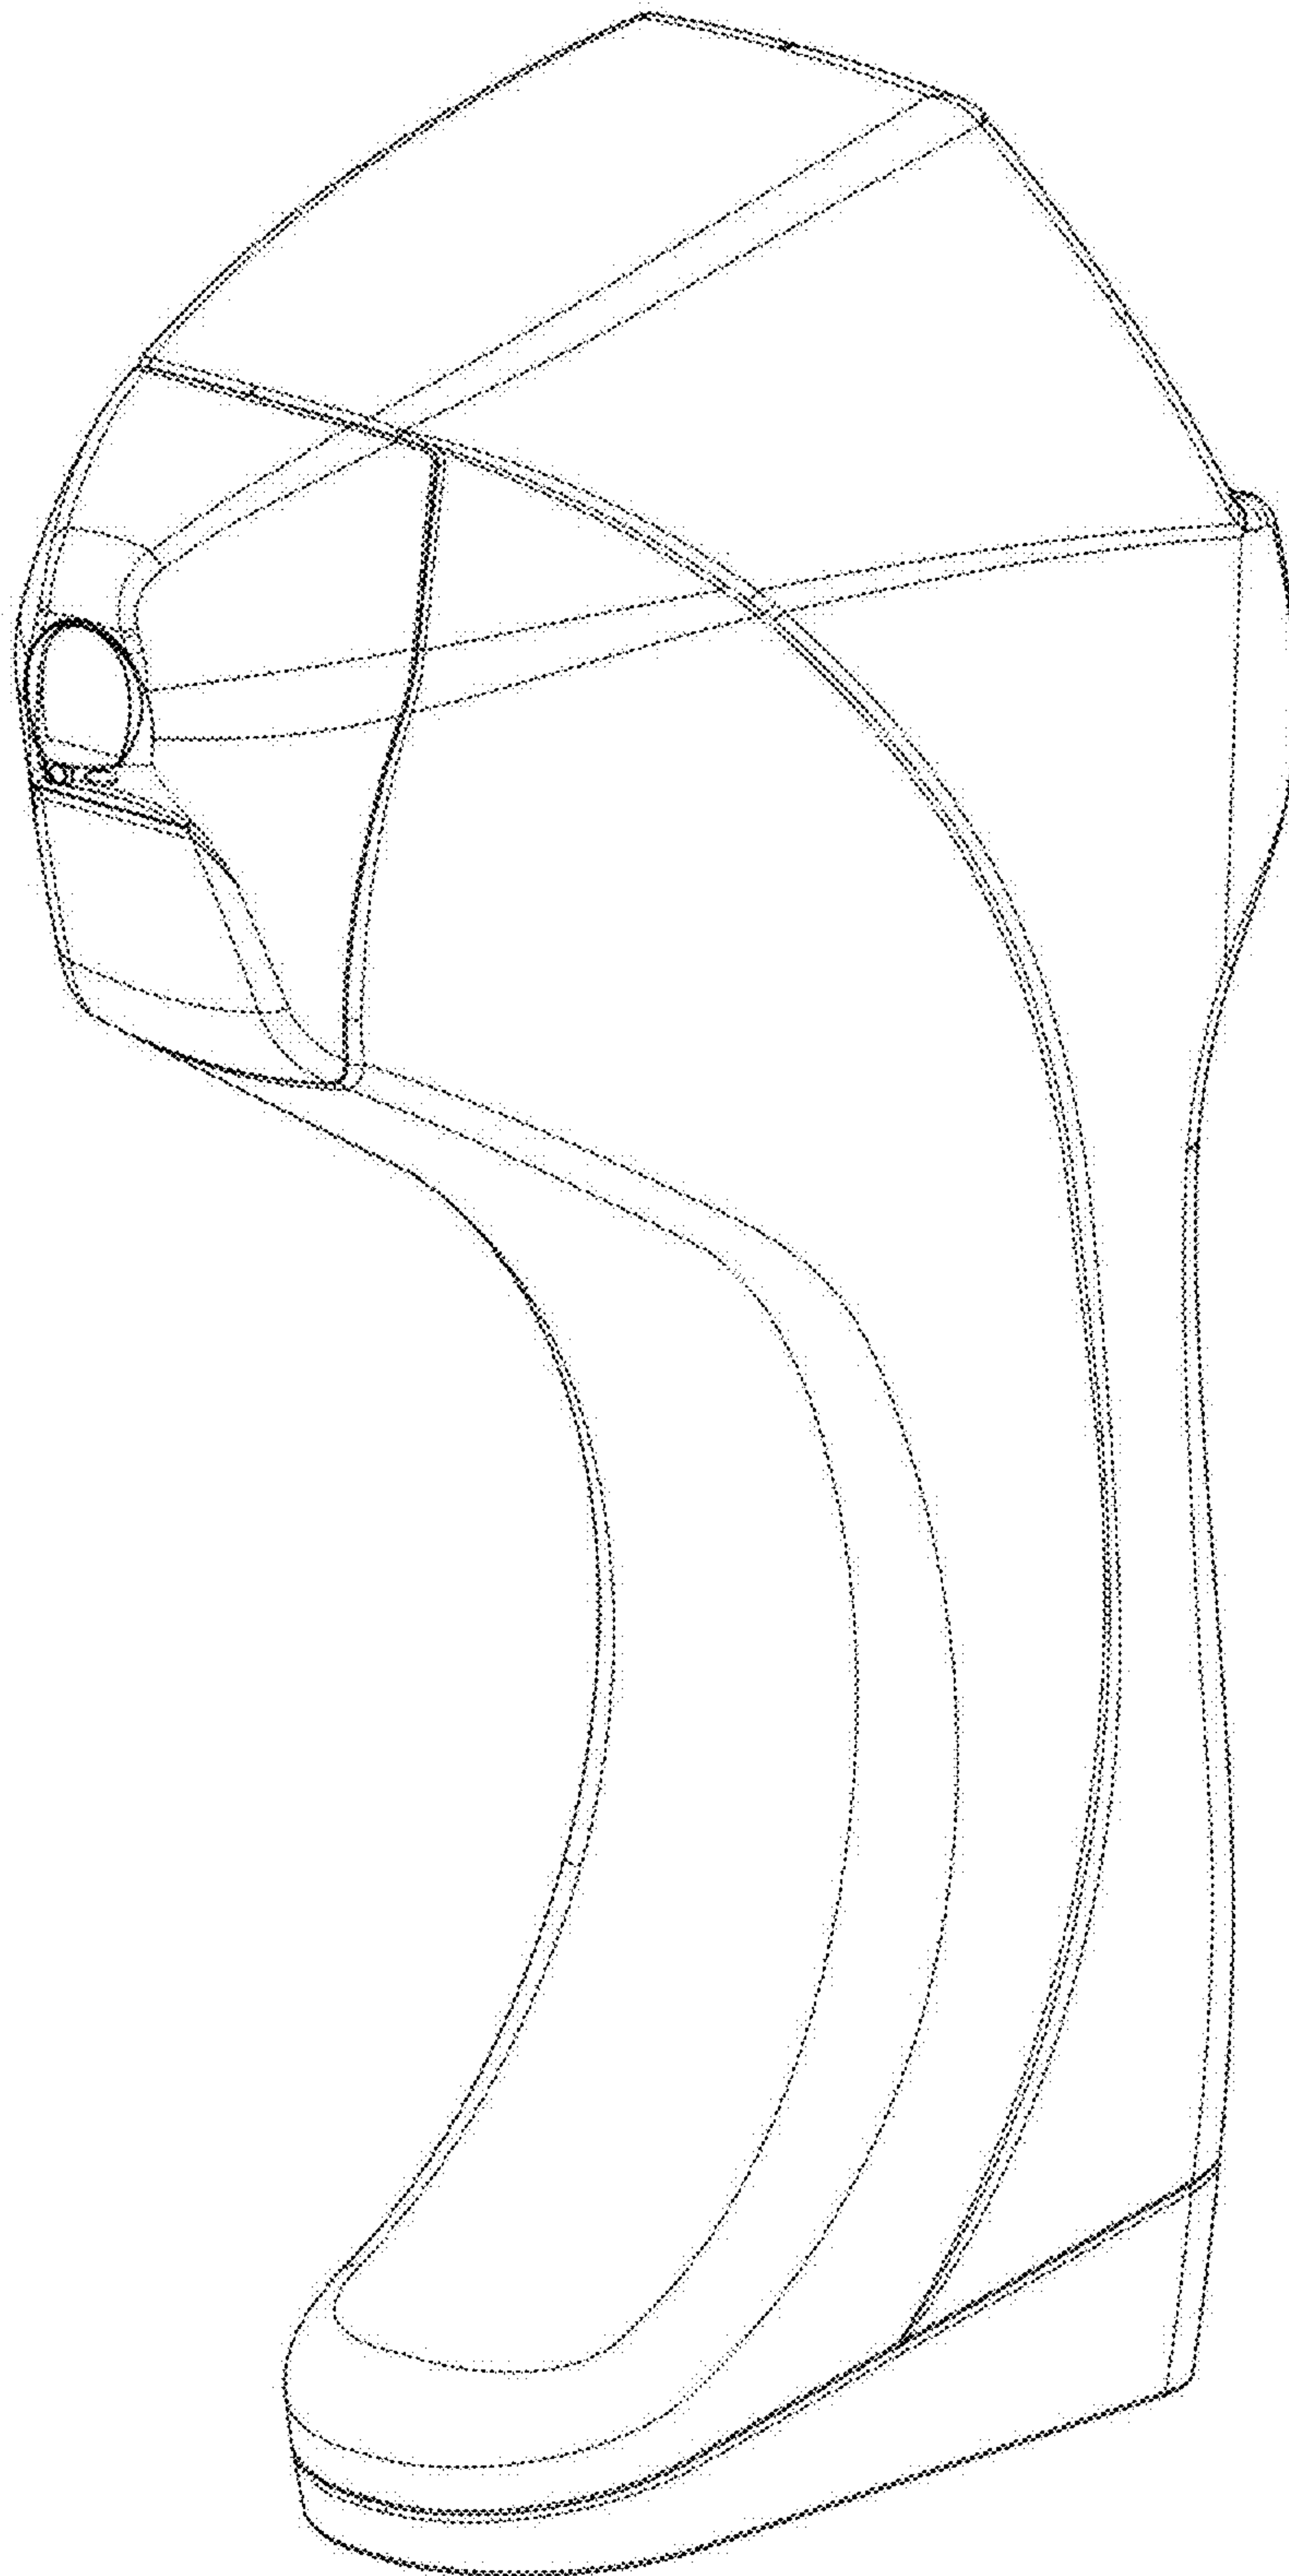


FIG. 1

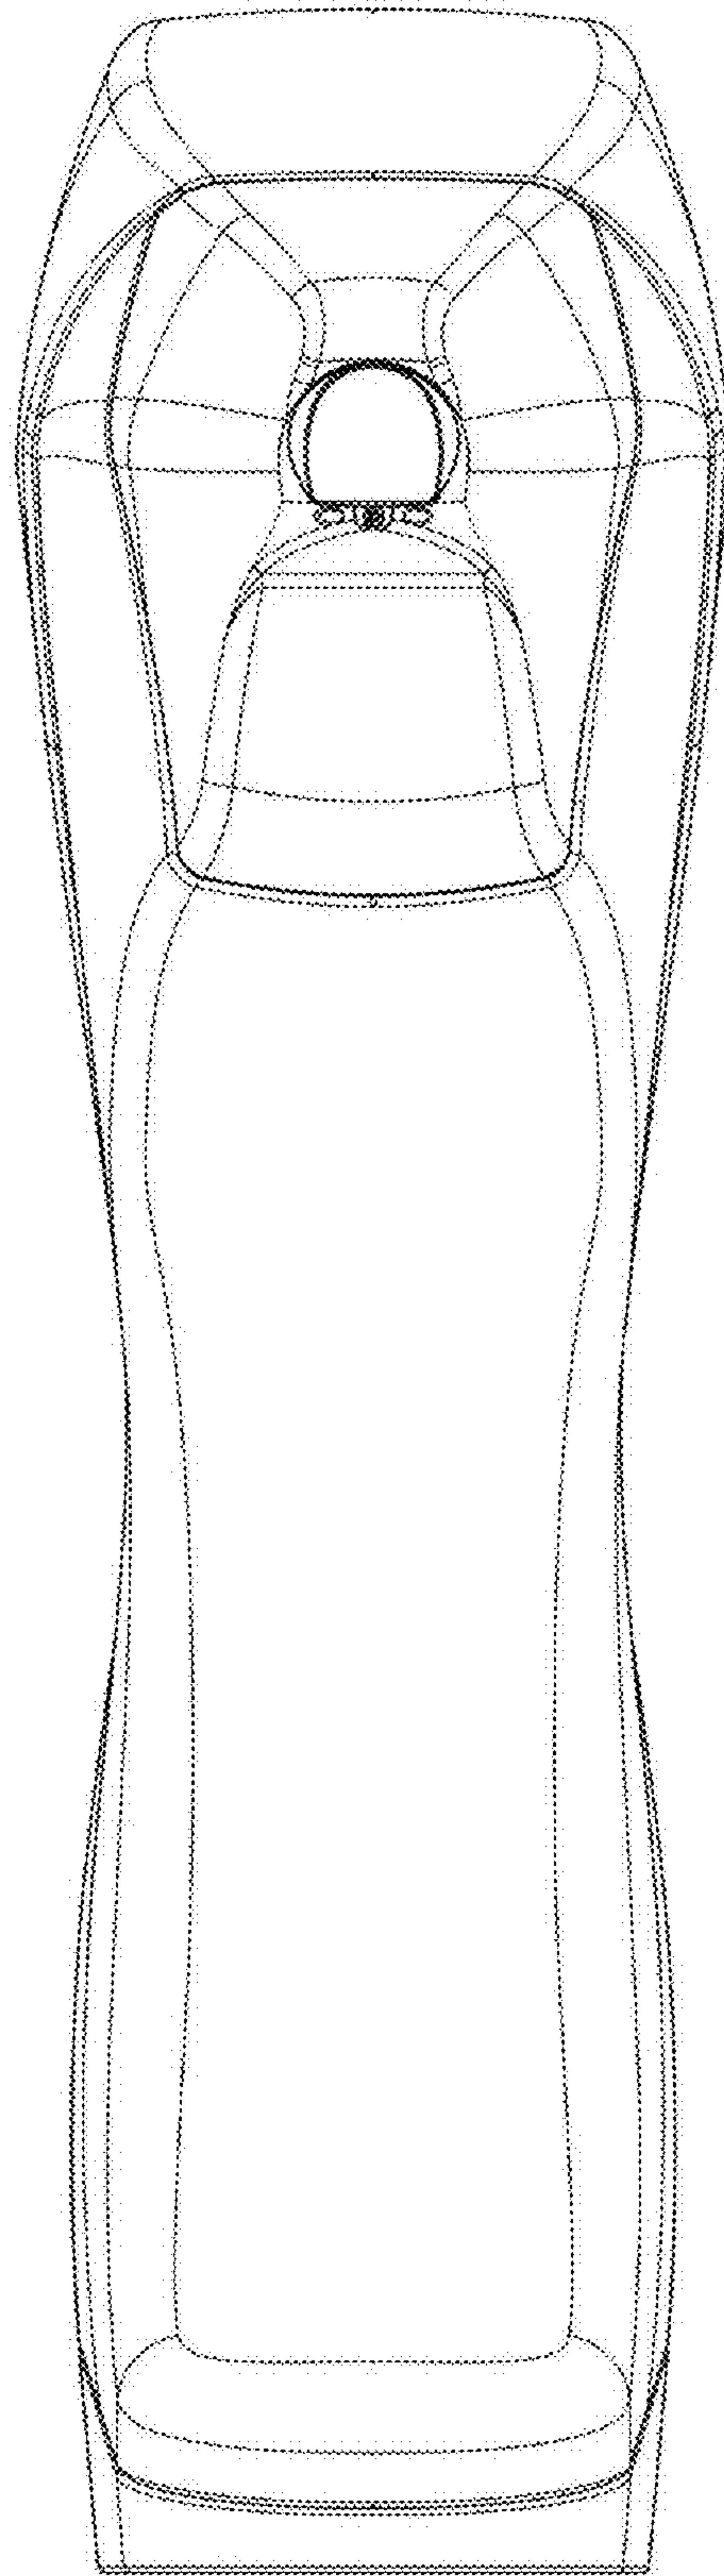


FIG. 2

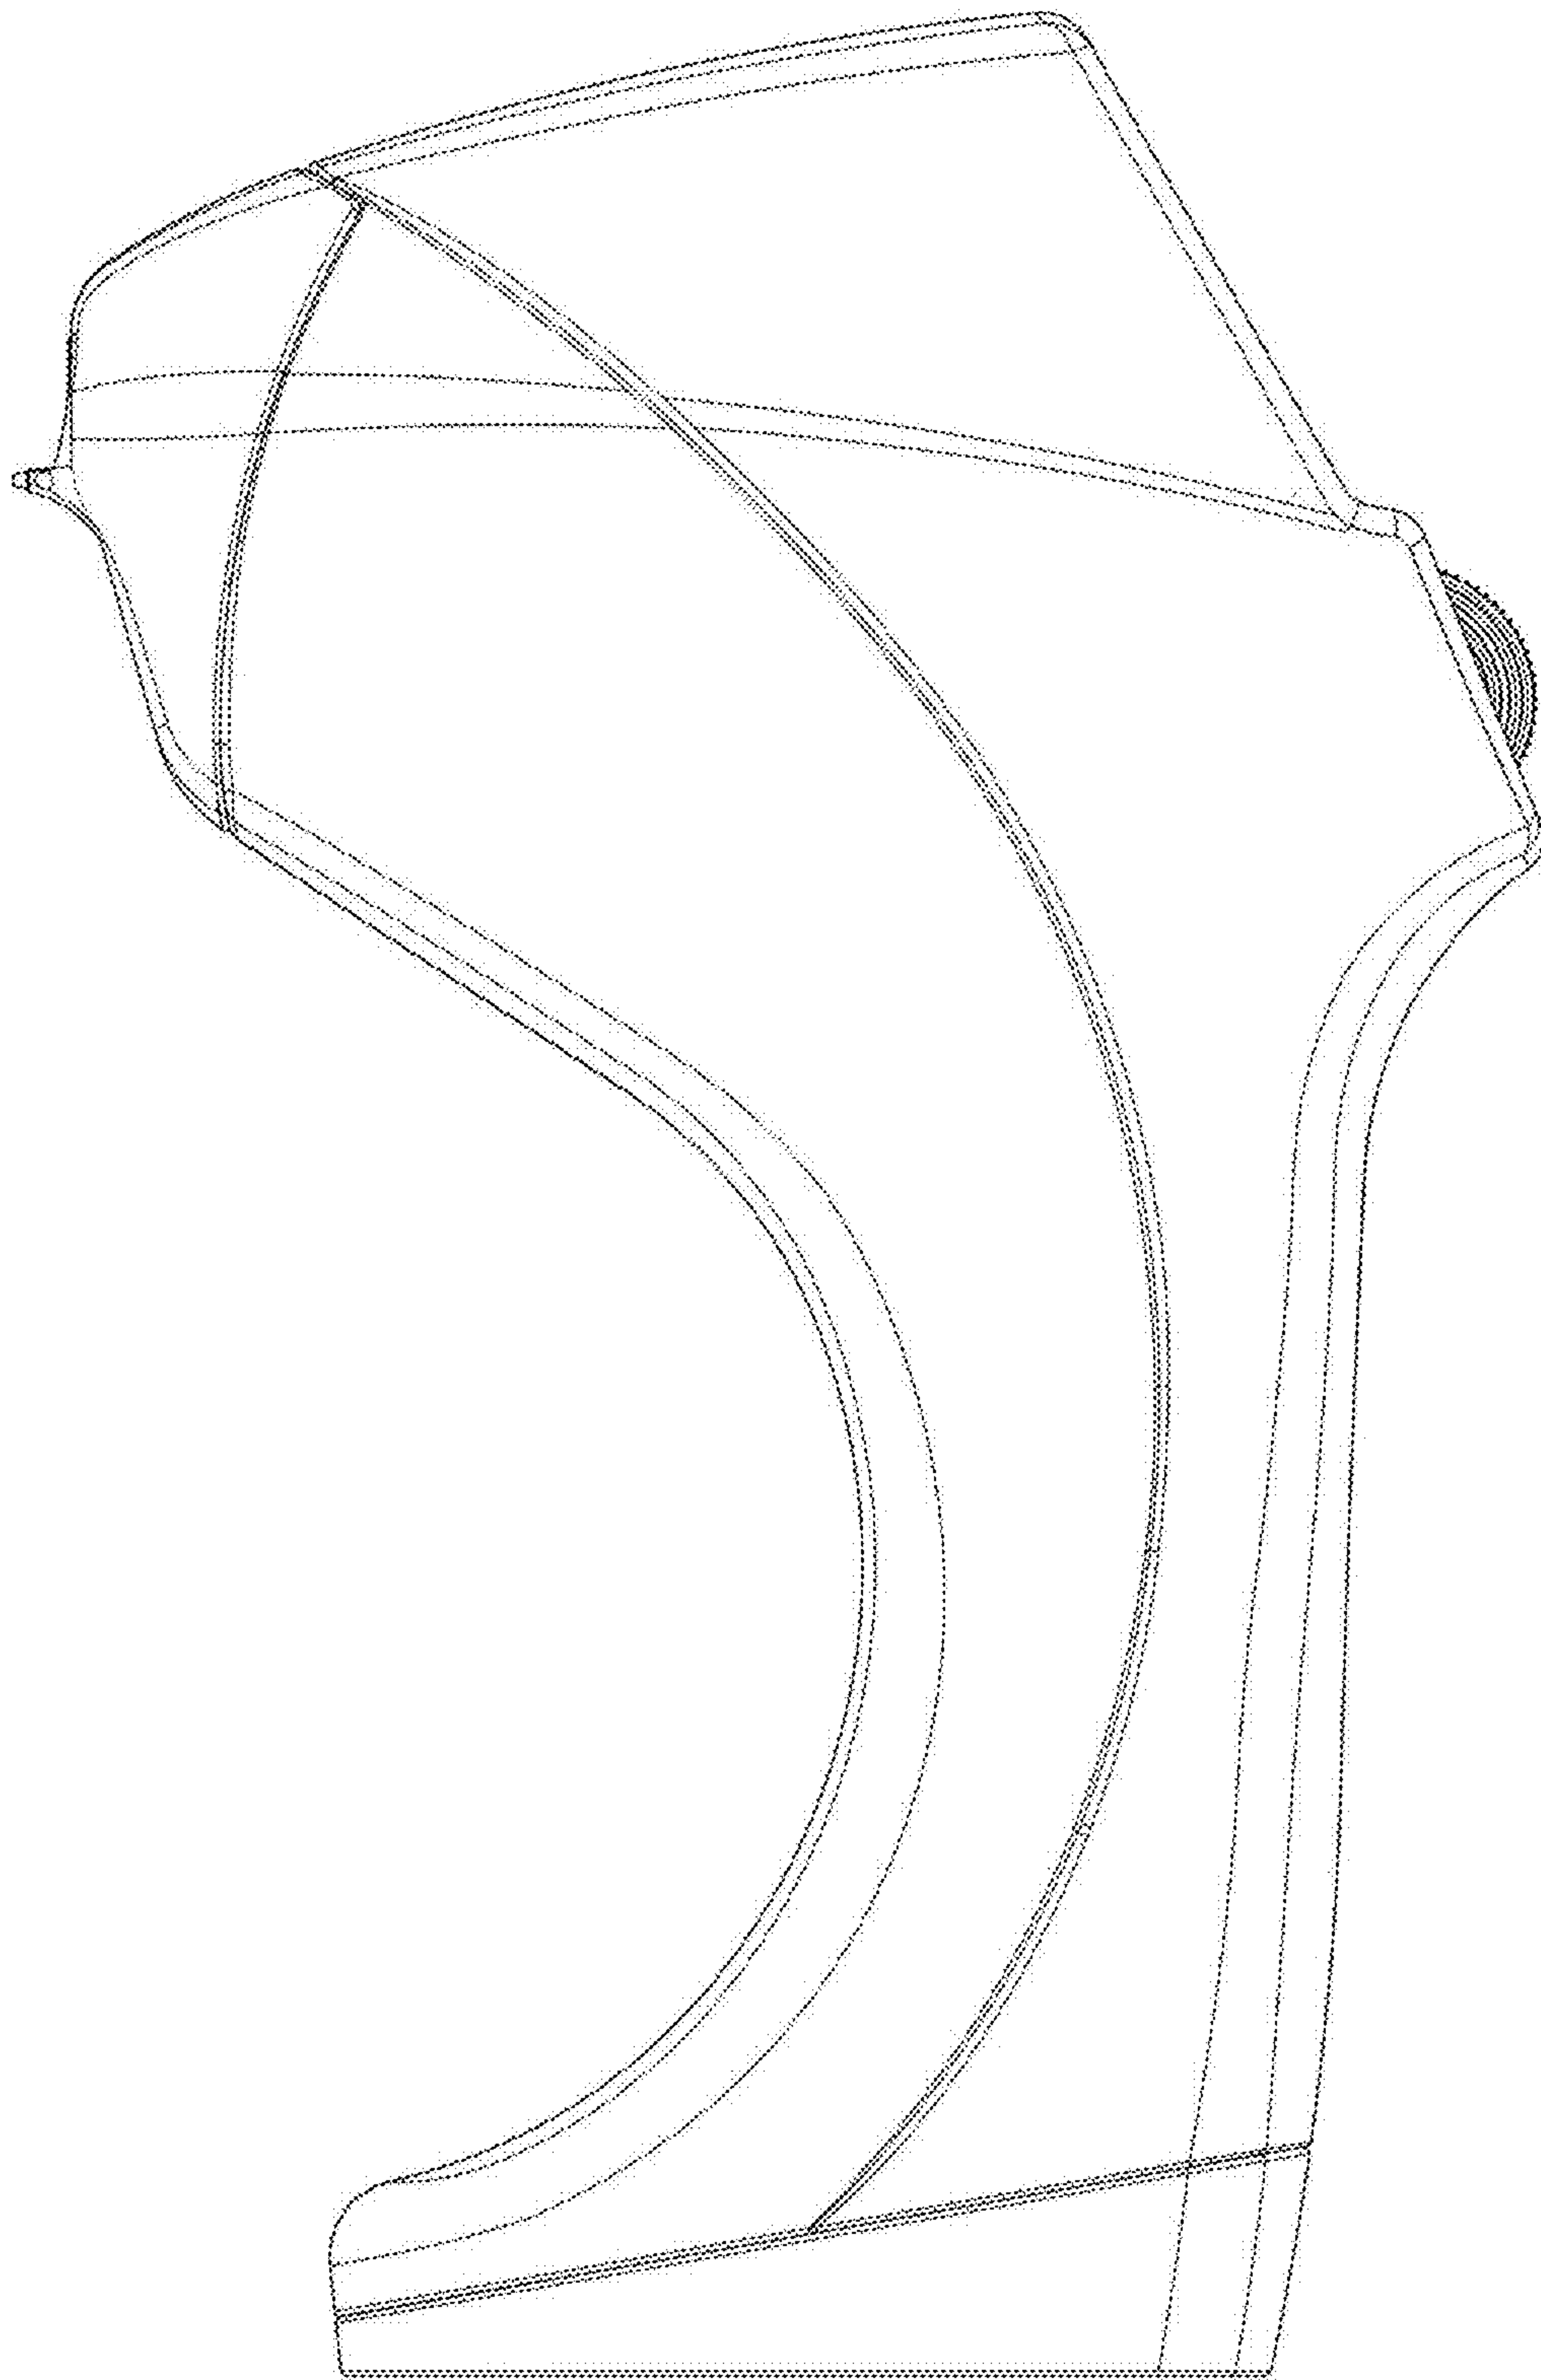


FIG. 3

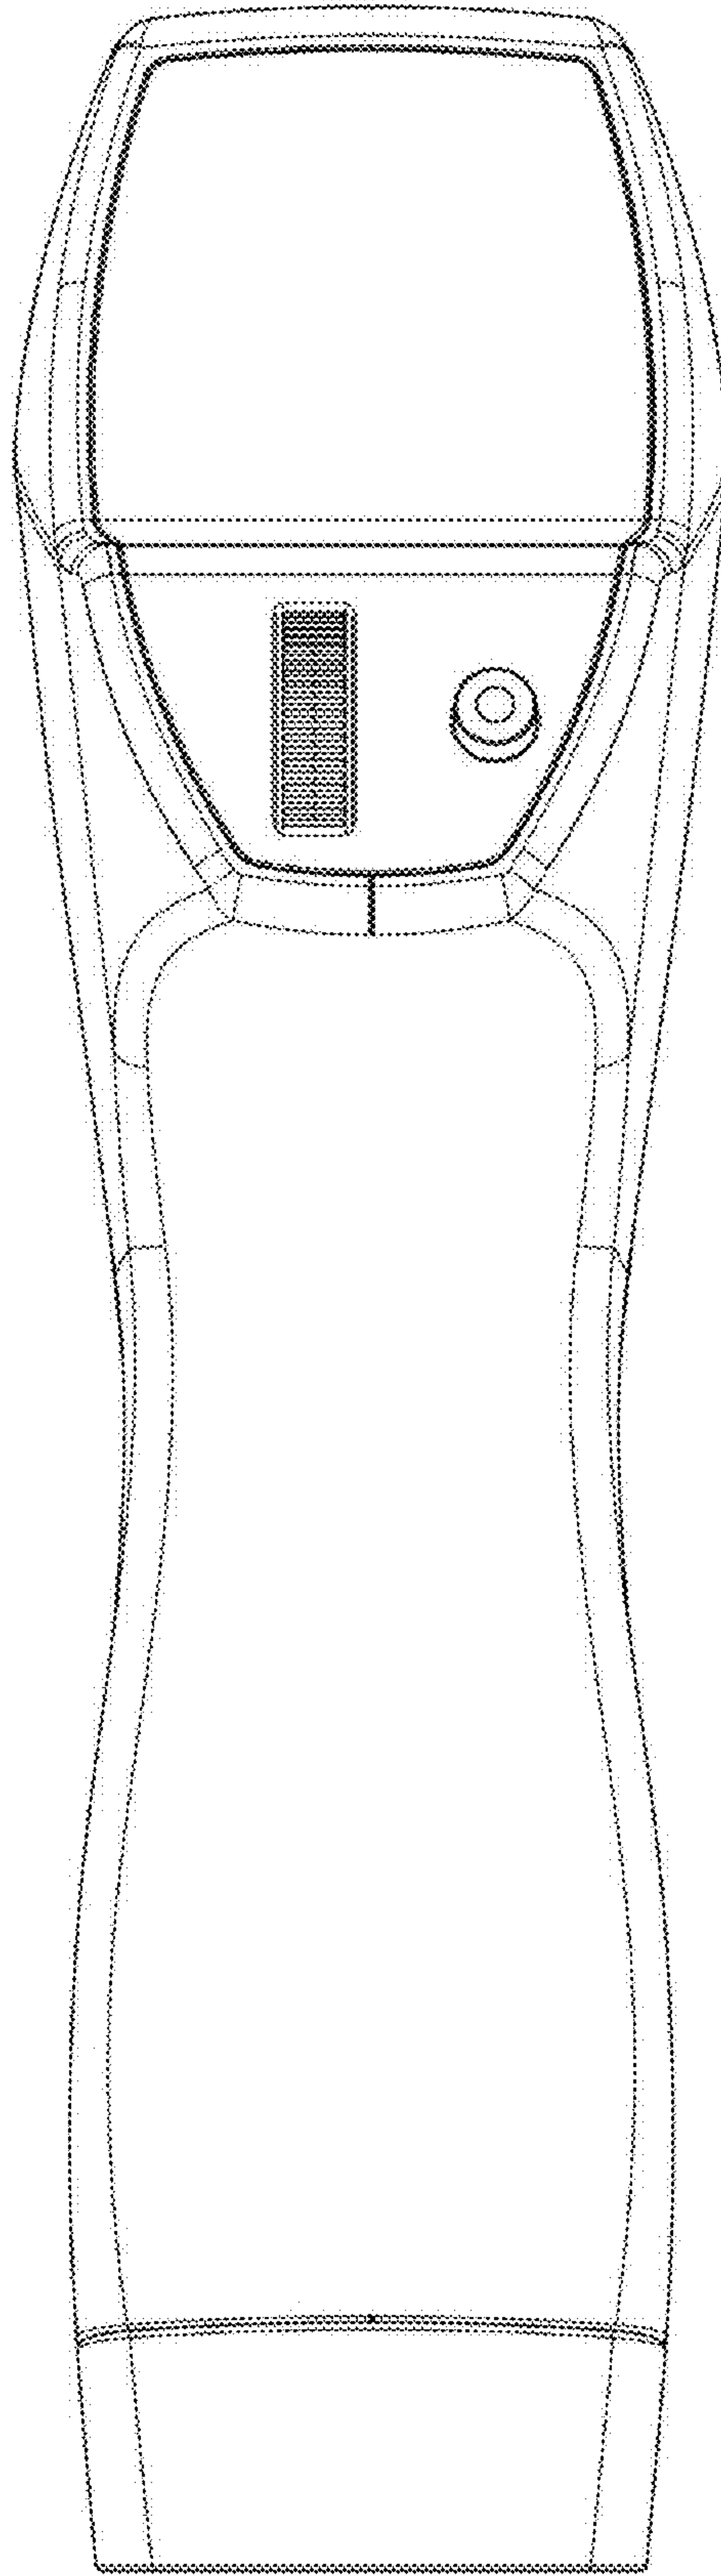


FIG. 4

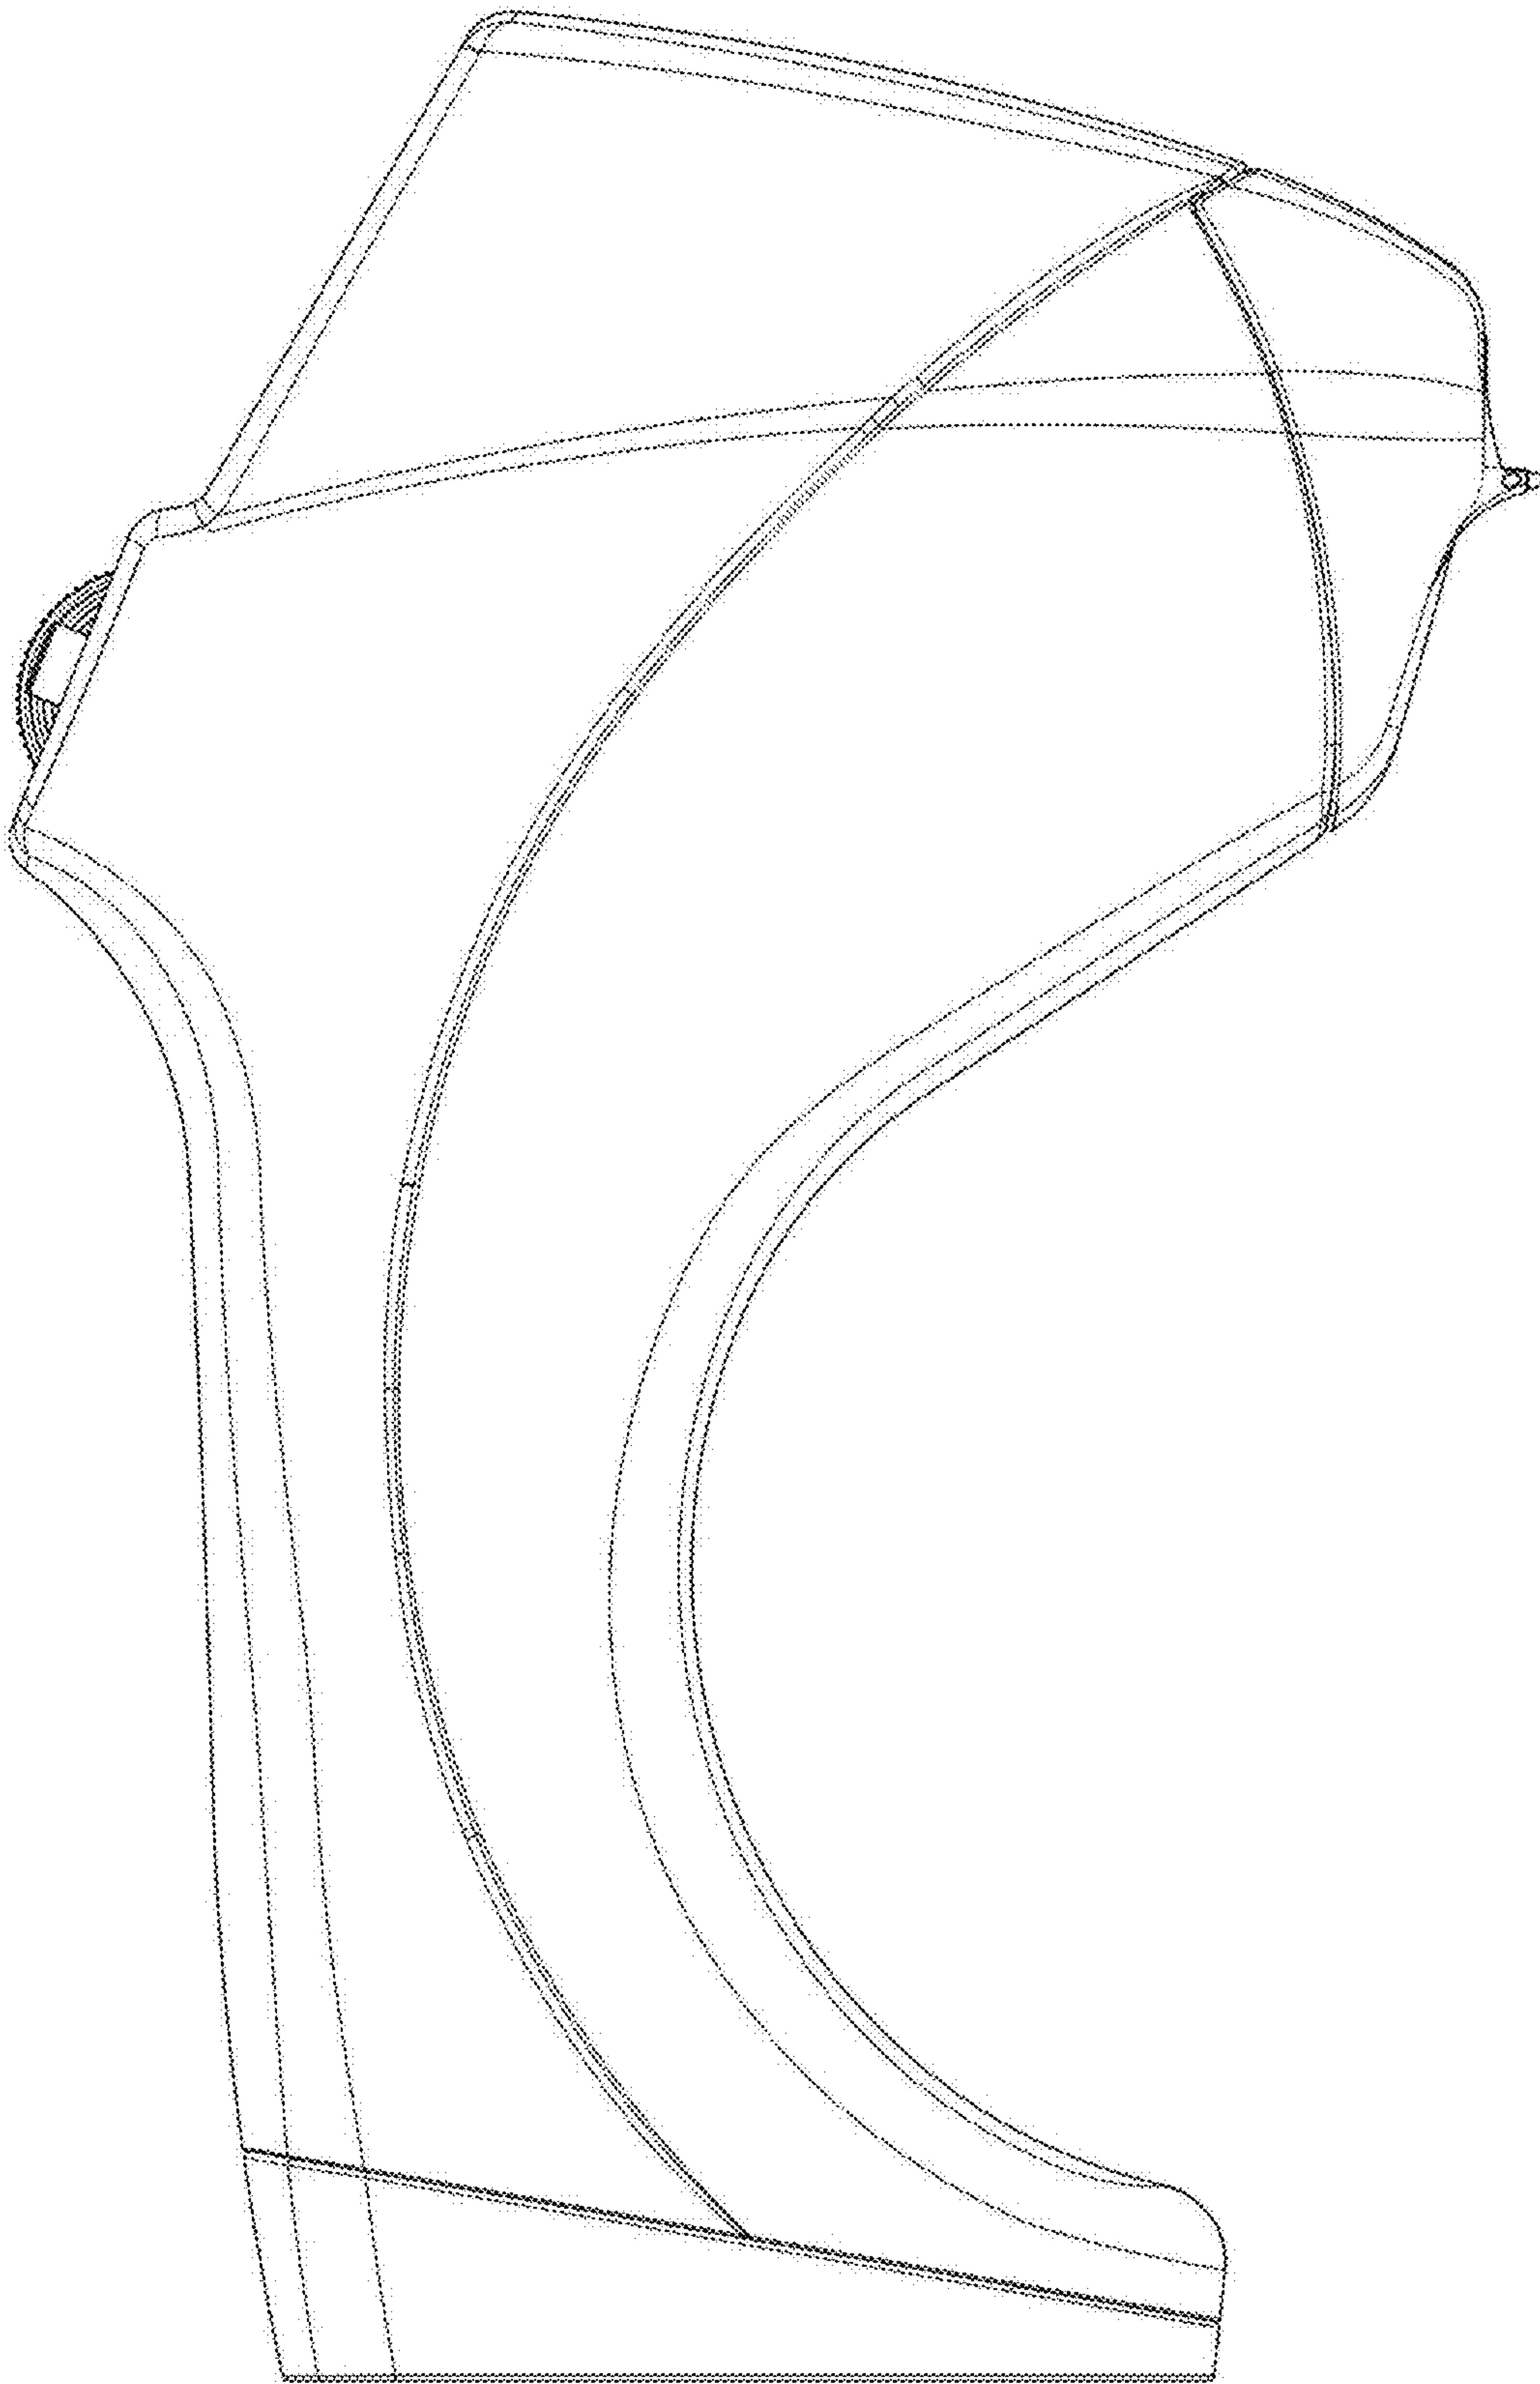


FIG. 5

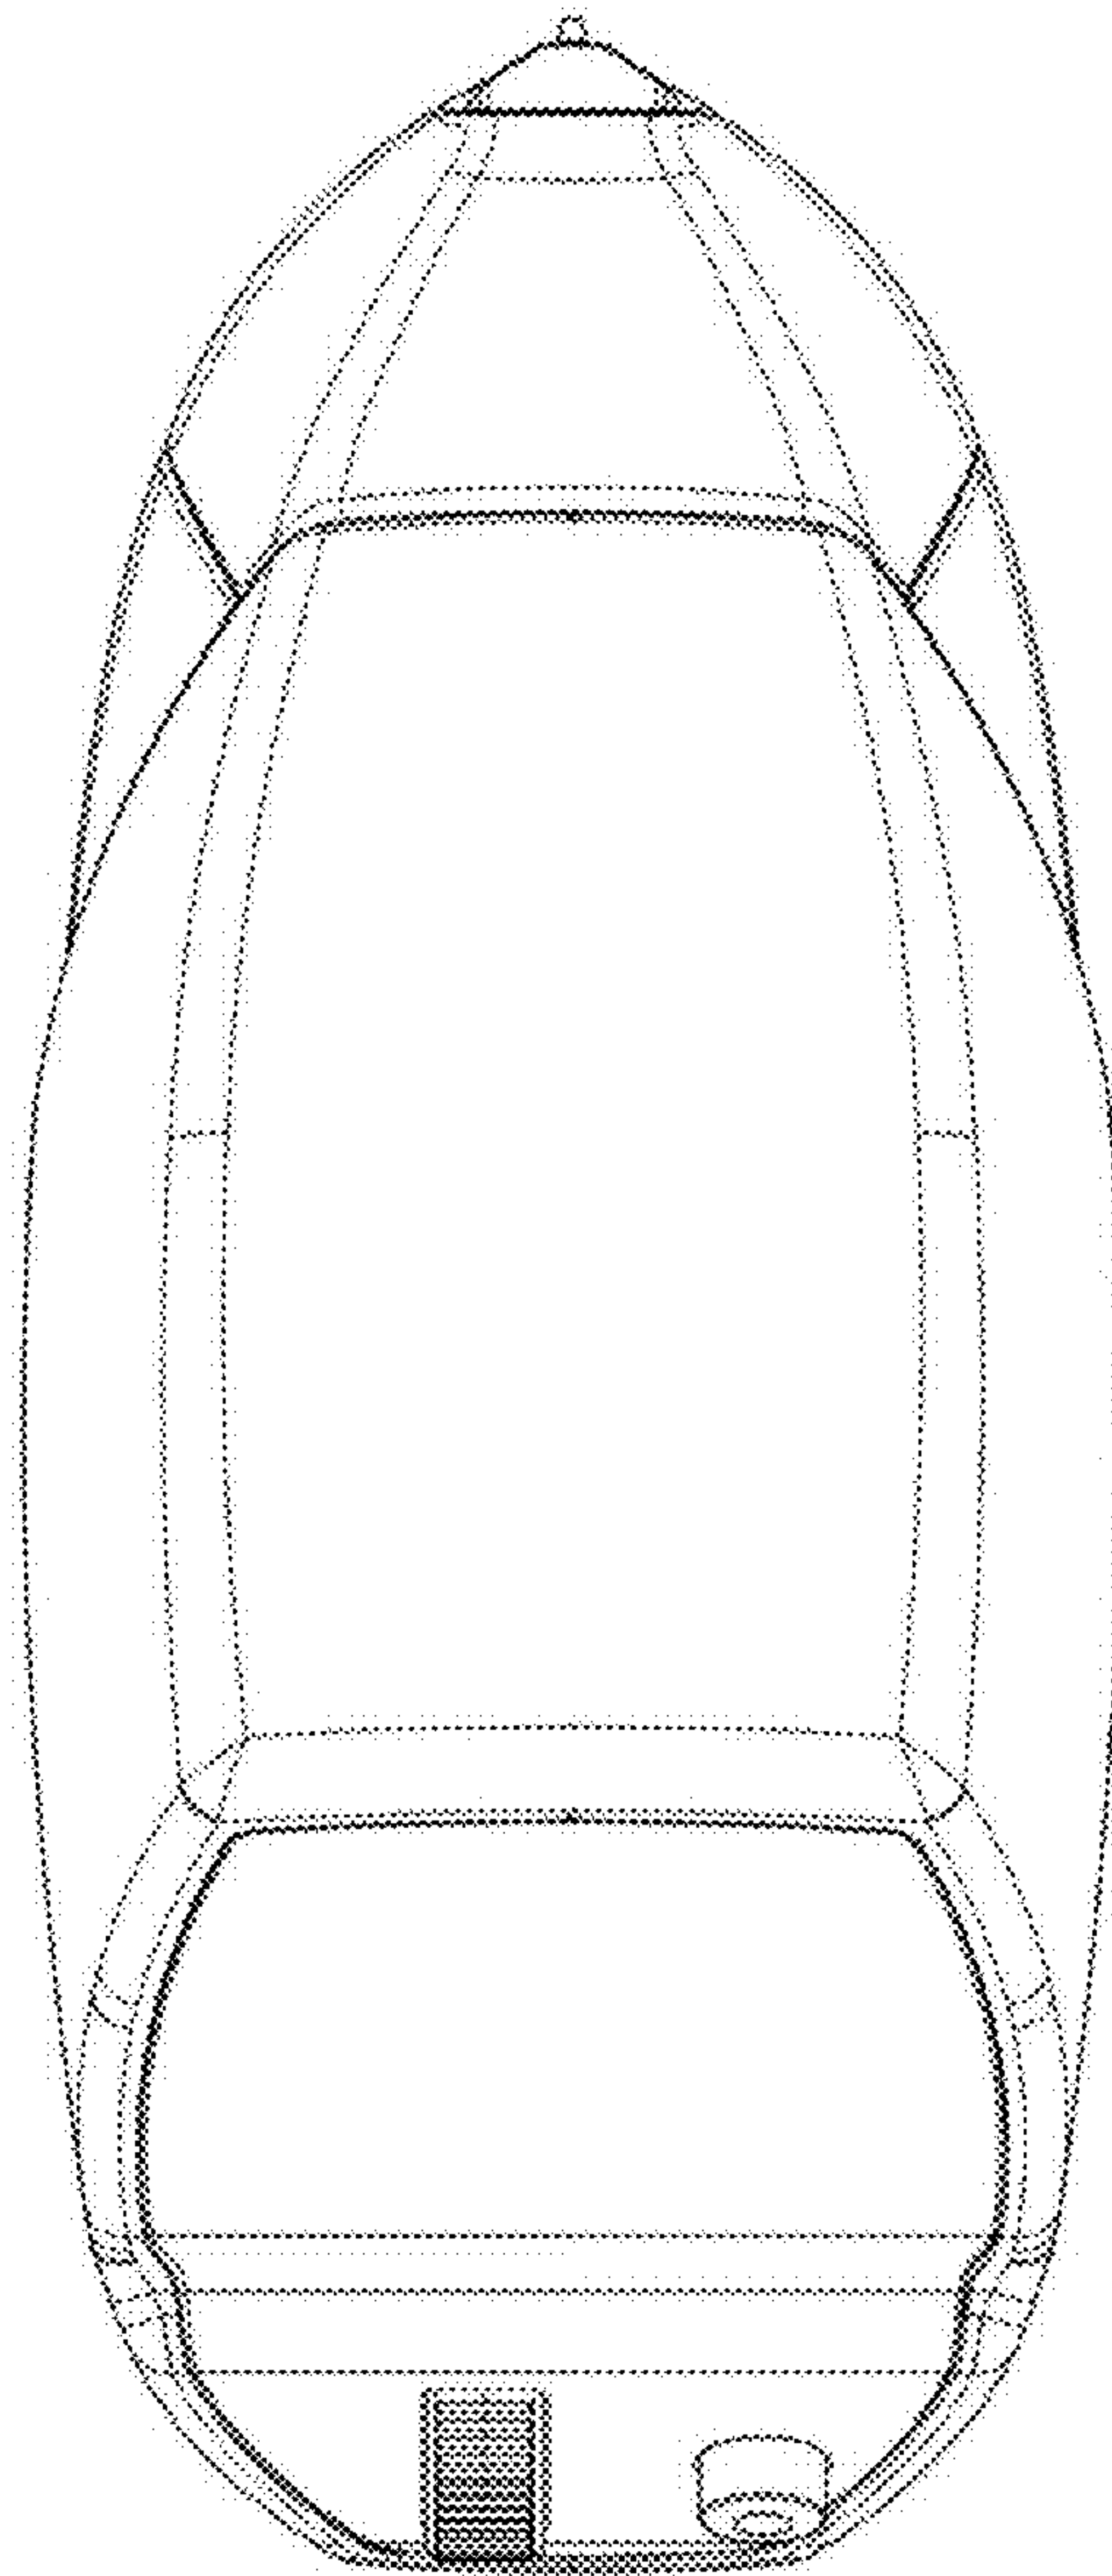


FIG. 6

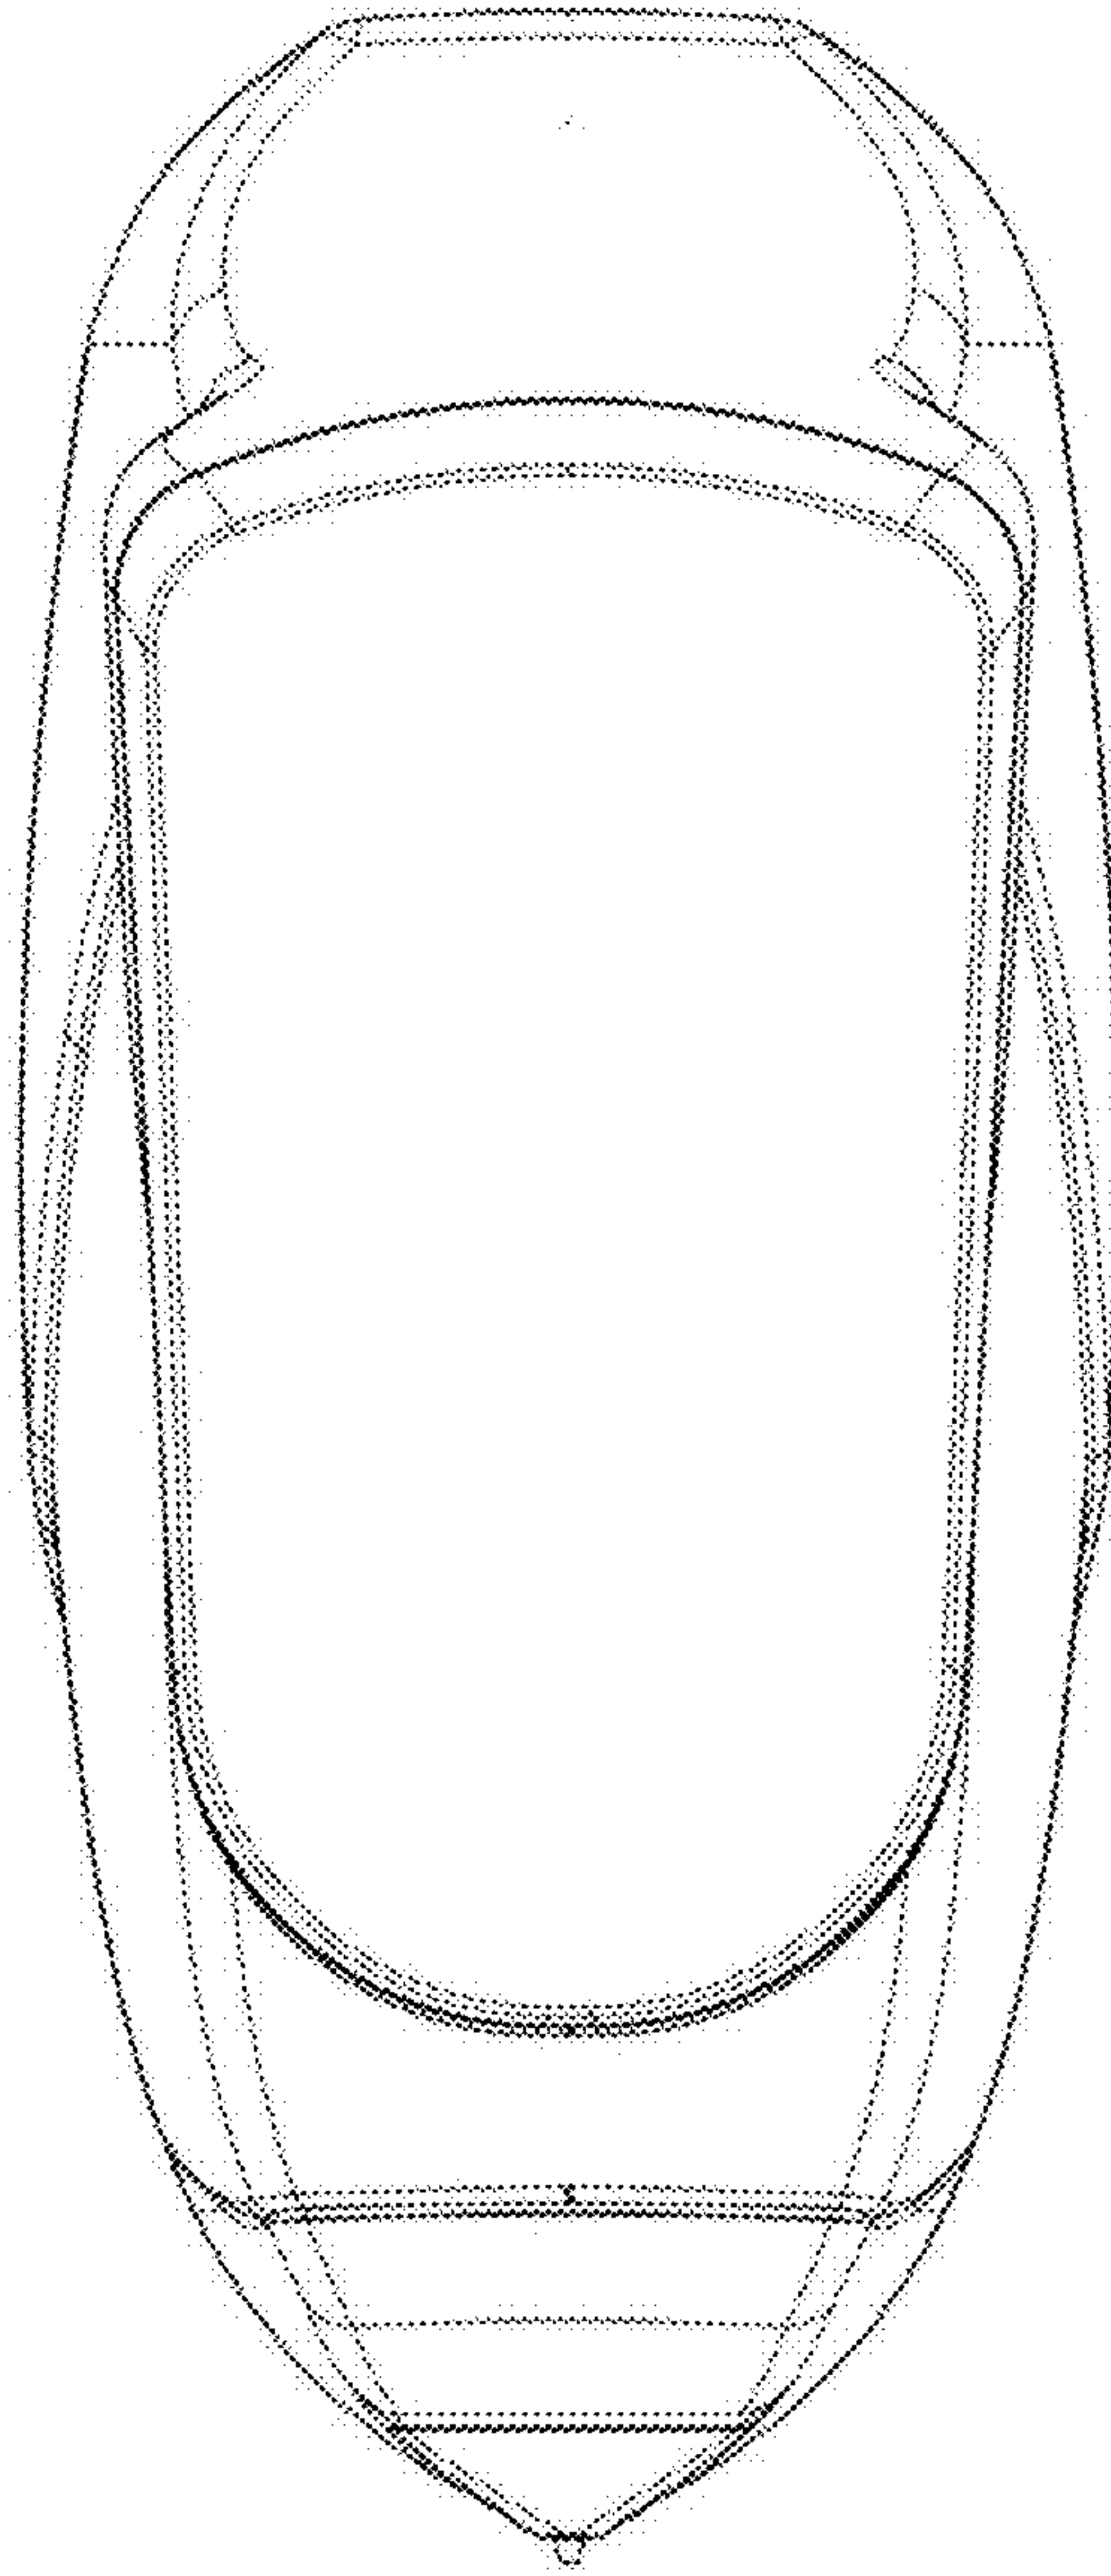


FIG. 7

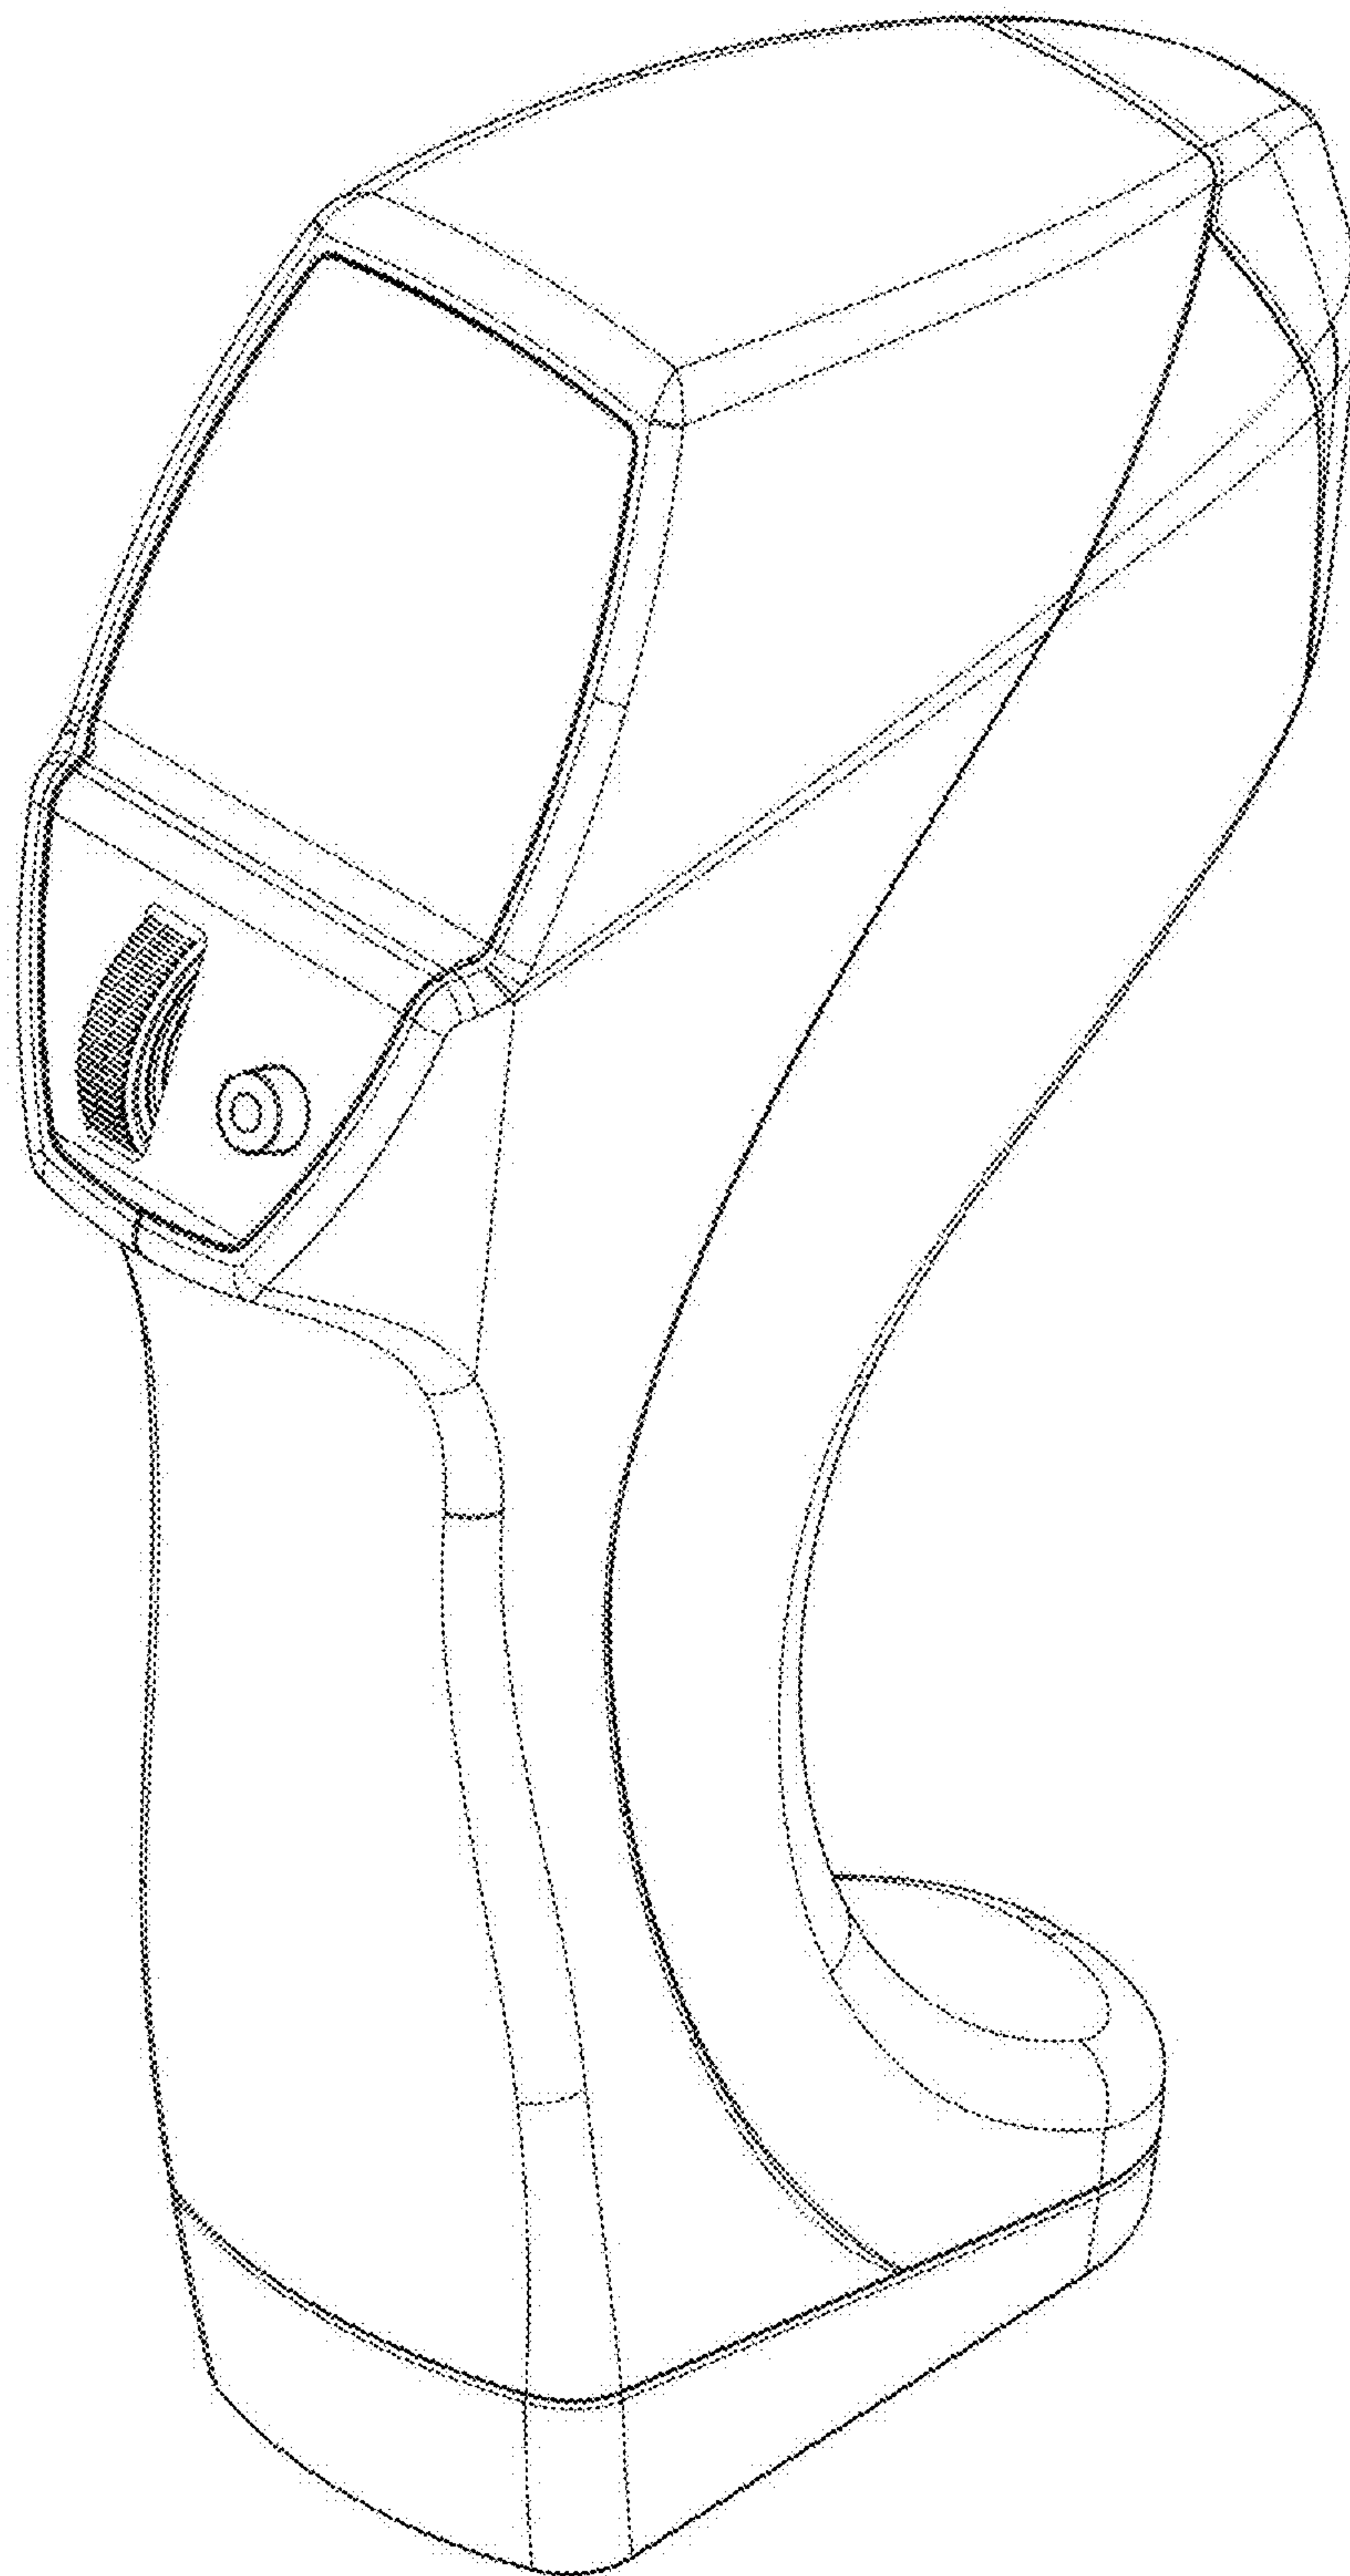


FIG. 8