

US00D946762S

(12) **United States Design Patent**
Reinke et al.

(10) **Patent No.:** **US D946,762 S**
(45) **Date of Patent:** **** Mar. 22, 2022**

- (54) **PEDESTAL**
- (71) Applicant: **WELCH ALLYN, INC.**, Skaneateles Falls, NY (US)
- (72) Inventors: **Christian H. Reinke**, Skaneateles Falls, NY (US); **Carlos Suarez**, Skaneateles Falls, NY (US); **Richard M. Farchione**, Skaneateles Falls, NY (US)
- (73) Assignee: **WELCH ALLYN, INC.**, Skaneateles Falls, NY (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/694,178**
- (22) Filed: **Jun. 7, 2019**
- (51) **LOC (13) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/186**
- (58) **Field of Classification Search**
USPC D6/522, 523, 525, 526, 553, 566; D8/49, D8/51, 52, 59, 60, 64, 82, 85, 86, 95, 97, D8/300, 303, 349, 499; D14/372; D15/138, 139; D16/100, 130, 309; D24/108, 112, 113, 114, 115, 119, 127, D24/128, 129, 130, 133, 137, 142, 144, D24/145, 146, 147, 148, 150, 155, 158, D24/160, 170, 171, 172, 173, 181, 185,
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D338,271 S * 8/1993 Yoshikawa D18/50
 - D390,662 S * 2/1998 Cooper D24/172
- (Continued)

OTHER PUBLICATIONS

Youtube, "Depisteo VT1 Vision Screener Product Review", first available Jul. 16, 2013. (<https://www.youtube.com/watch?v=L9QdU7W9X70>) (Year: 2013).*

(Continued)

Primary Examiner — Lauren D McVey
Assistant Examiner — Justin A Johnson
(74) *Attorney, Agent, or Firm* — Alston & Bird LLP

(57) **CLAIM**



We claim the ornamental design for a pedestal, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a pedestal showing our new design;
 FIG. 2 is another perspective view thereof, shown in another position of use;
 FIG. 3 is a front elevation view thereof;
 FIG. 4 is a rear elevation view thereof;
 FIG. 5 is a right side elevation view thereof;
 FIG. 6 is a left side elevation view thereof;
 FIG. 7 is a top plan view thereof;
 FIG. 8 is a bottom plan view thereof;
 FIG. 9 is a perspective view thereof, shown in another position of use;
 FIG. 10 is another perspective view thereof;
 FIG. 11 is a front elevation view thereof;
 FIG. 12 is a rear elevation view thereof;
 FIG. 13 is a right side elevation view thereof;
 FIG. 14 is a left side elevation view thereof;
 FIG. 15 is a top plan view thereof; and,
 FIG. 16 is a bottom plan view thereof.

The dash-dot-dash broken lines adjacent shaded areas represent bounds of the claimed design. The even dash-dash broken lines adjacent shaded areas represent features of the pedestal and bounds of the claimed design and form no part of the claimed design. All other broken lines are directed to features of the pedestal that form no part of the claimed design.

1 Claim, 16 Drawing Sheets

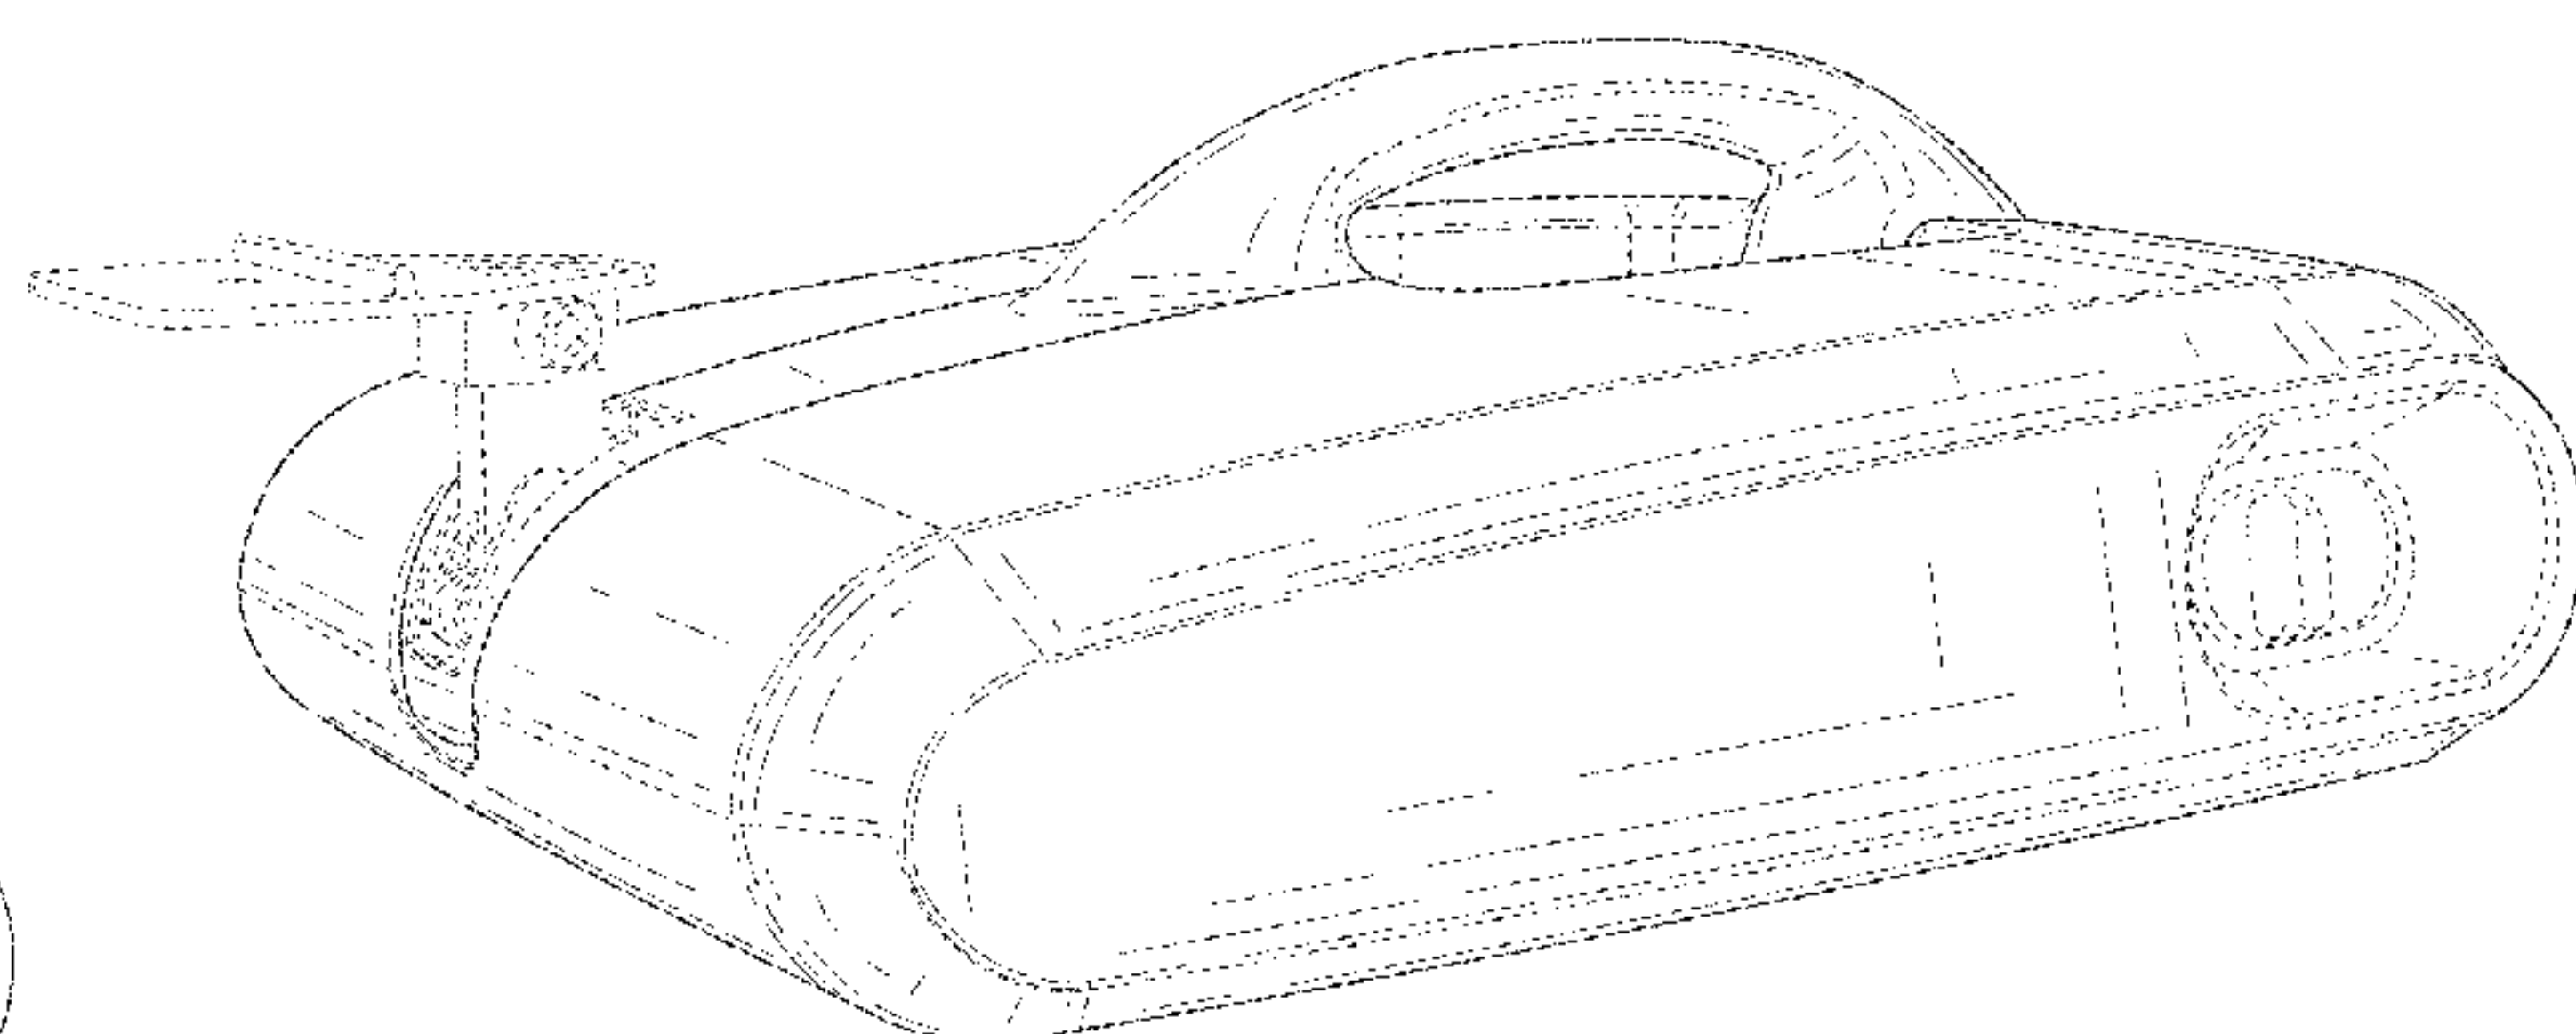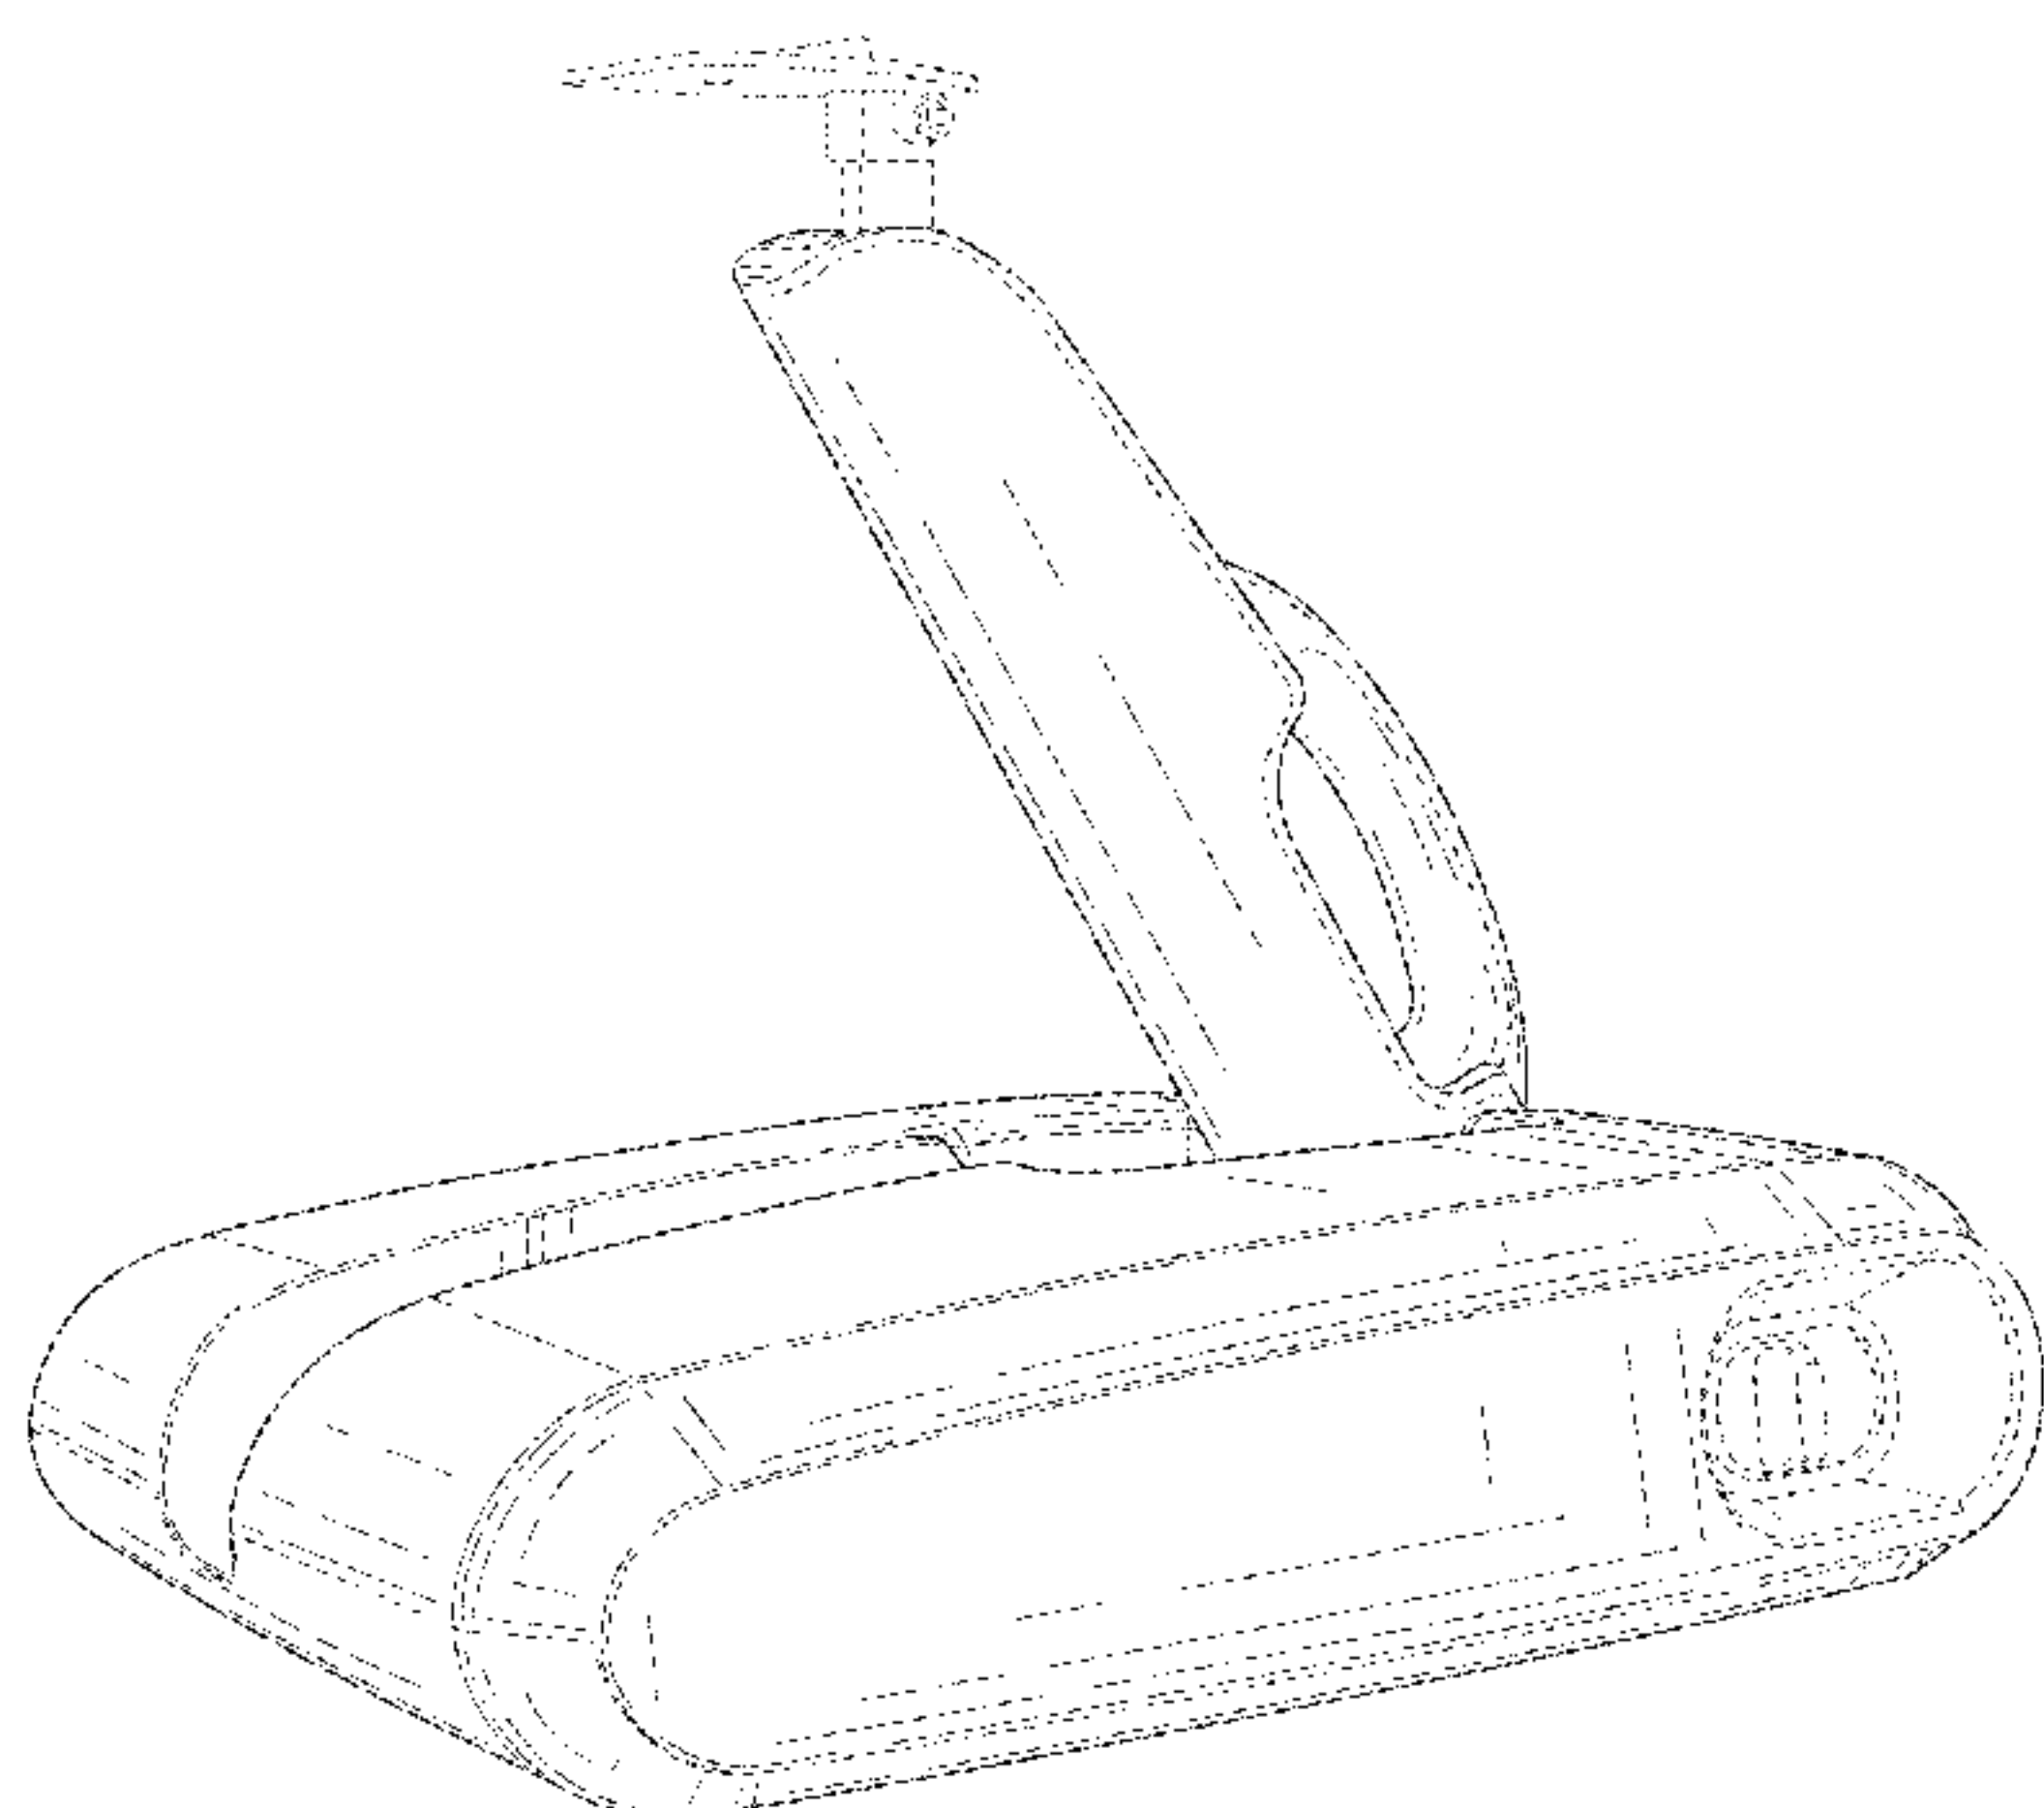

(58) **Field of Classification Search**

USPC D24/186, 188, 200, 215, 216, 222, 231,
D24/232; D25/38.1, 41.1; D10/57
CPC A61B 3/00; A61B 3/0016; A61B 3/0025;
A61B 3/0033; A61B 3/0041; A61B
3/0075; A61B 3/0083; A61B 3/0091;
A61B 3/02; A61B 3/10; A61B 3/1005;
A61B 3/12; A61B 3/13; A61B 3/18;
A61B 17/00; A61B 2017/00349; A61B
2017/00455; A61B 2017/00464; A61B
2017/00473; A61B 2017/0053; A61B
17/0057; A61B 17/0231; A61B 17/04;
A61B 17/064; A61B 17/0642; A61B
17/0643; A61B 17/0644; A61B
2017/0688; A61B 17/14; A61B 17/142;
A61B 17/15; A61B 17/151; A61B
17/154; A61B 17/155; A61B 17/157;
A61B 17/158; A61B 17/16; A61B
17/1613; A61B 17/1615; A61B 17/1617;
A61B 2090/0817; A61B 2017/00663;
A61B 17/0401; A61B 2017/0404; A61B
10/00; A61B 10/02; A61B 2010/0208;
A61B 10/04; A61B 2010/045; A61B
17/221; A61B 17/34; A61B 17/3415;
B23D 51/025; A61F 9/00; A61F 9/007;
A61F 9/0133; A61F 2210/0004; A61H
5/00; A61H 5/005; A61H 2205/022;
E21B 10/00; B28B 7/00; B28B 7/0002;
B28B 7/0032; B28B 7/0094; B28B 7/16;
B28B 7/18

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,796,086 A * 8/1998 Gannon G06K 7/084
235/449
5,838,424 A * 11/1998 Wawro A61B 3/10
351/245
D554,266 S * 10/2007 Striepe D24/186
D692,145 S * 10/2013 Al-Ali A61B 3/10
D24/186
D717,441 S * 11/2014 Neo D24/167
D748,272 S * 1/2016 Knieriem G06K 7/084
D24/186
D759,254 S * 6/2016 Knieriem H03K 17/962
D24/186
2012/0073930 A1 * 3/2012 Lansberry B25J 5/005
192/66.3

2013/0142709 A1 * 6/2013 Lin G01N 27/26
422/538
2019/0248020 A1 * 8/2019 Yoon H03K 17/962
2020/0383749 A1 * 12/2020 Reinke A61B 3/1208

OTHER PUBLICATIONS

Keystone View, “The VS-V Standard Vision Scanner”, first available Jan. 14, 2014. (https://www.keystoneview.com/wp-content/uploads/2009/08/VS-V_Standard_Brochure_2015.pdf) (Year: 2014).*

Kahntact Medical, “The Optec 5000/5000P”, first available Apr. 2017. (<https://www.kahntactmedical.com/wp-content/uploads/2019/10/Optec-5000-vision-screener-product-specifications.pdf>) (Year: 2017).*

Hillrom, “Welch Allyn RetinaVue 700 Pedestal”, first available May 20, 2020. (<https://www.hillrom.com/content/dam/hillrom-aem/us/en/sap-documents/MRC/80023/80023924MRCPDF.pdf>) (Year: 2020).*

“Welch Allyn Topcon TRC-NW400 Non-Mydriatic Retinal Camera 723427 from 4MD Medical” [online] [retrieved Mar. 12, 2019], retrieved from the Internet, URL: <https://www.4mdmedical.com/catalog/product/view/id/373571/7CAWELAID=120141310000056386&utm_source=google&utm_medium=cpc&adpos=1> dated Mar. 12, 2019.

“Spot Vision Screener” [online] [retrieved Mar. 12, 2019], retrieved from the Internet, URL: <<https://www.welchallyn.com/en/products/categories/physical-exam/eye-exam/vision-screeners/spot-vision-screener.html>> dated Mar. 12, 2019.

“Spot-Vision-Screener_rt-front-angle” [online] [retrieved Mar. 12, 2019], retrieved from the Internet, URL: <https://www.welchallyn.com/content/dam/welchallyn/images/Product-Images/Physical-Exam/Eye-Exam/Vision-Screeners/Spot-Vision-Screener/Spot-Vision-Screener_rt-front-angle.jpg> dated Mar. 12, 2019.

“Spot-Vision-Screener_left-front-angle.jpg” [online] [retrieved Mar. 12, 2019], retrieved from the Internet, URL: <https://www.welchallyn.com/content/dam/welchallyn/images/Product-Images/Physical-Exam/Eye-Exam/Vision-Screeners/Spot-Vision-Screener/Spot-Vision-Screener_left-front-angle.jpg> dated Mar. 12, 2019.

“Welch Allyn Spot Vision Screener” [online] [retrieved Mar. 12, 2019], retrieved from the Internet, URL: <https://www.https://cdn.shopify.com/s/files/1/1046/1086/products/welch-allyn-spot-vision-screener_448x448.jpg?v=1512172639> dated Mar. 12, 2019.

“Welch Allyn Spot Vision Screener3” [online] [retrieved Mar. 12, 2019], retrieved from the Internet, URL: <https://www.https://cdn.shopify.com/s/files/1/1046/1086/products/welch-allyn-spot-vision-screener3_448x448.jpg?v=1512172651> dated Mar. 12, 2019.

“Welch Allyn RV100-B Handheld RetinaVue 100 Imager—CME Corp” [online] [retrieved Mar. 12, 2019], retrieved from the Internet, URL: <https://www.cmecorp.com/welch-allyn-rv100-b-retinavue-network.html?gclid=EAIQobChMItsT2u5f94AIVybXACH2cvqg6EAQYasABEgJ93vD_Bwe> dated Mar. 12, 2019.

“CenterVue” [online] [retrieved Mar. 12, 2019], retrieved from the Internet, URL: <<https://www.centervue.com/products/>> dated Mar. 12, 2019.

* cited by examiner

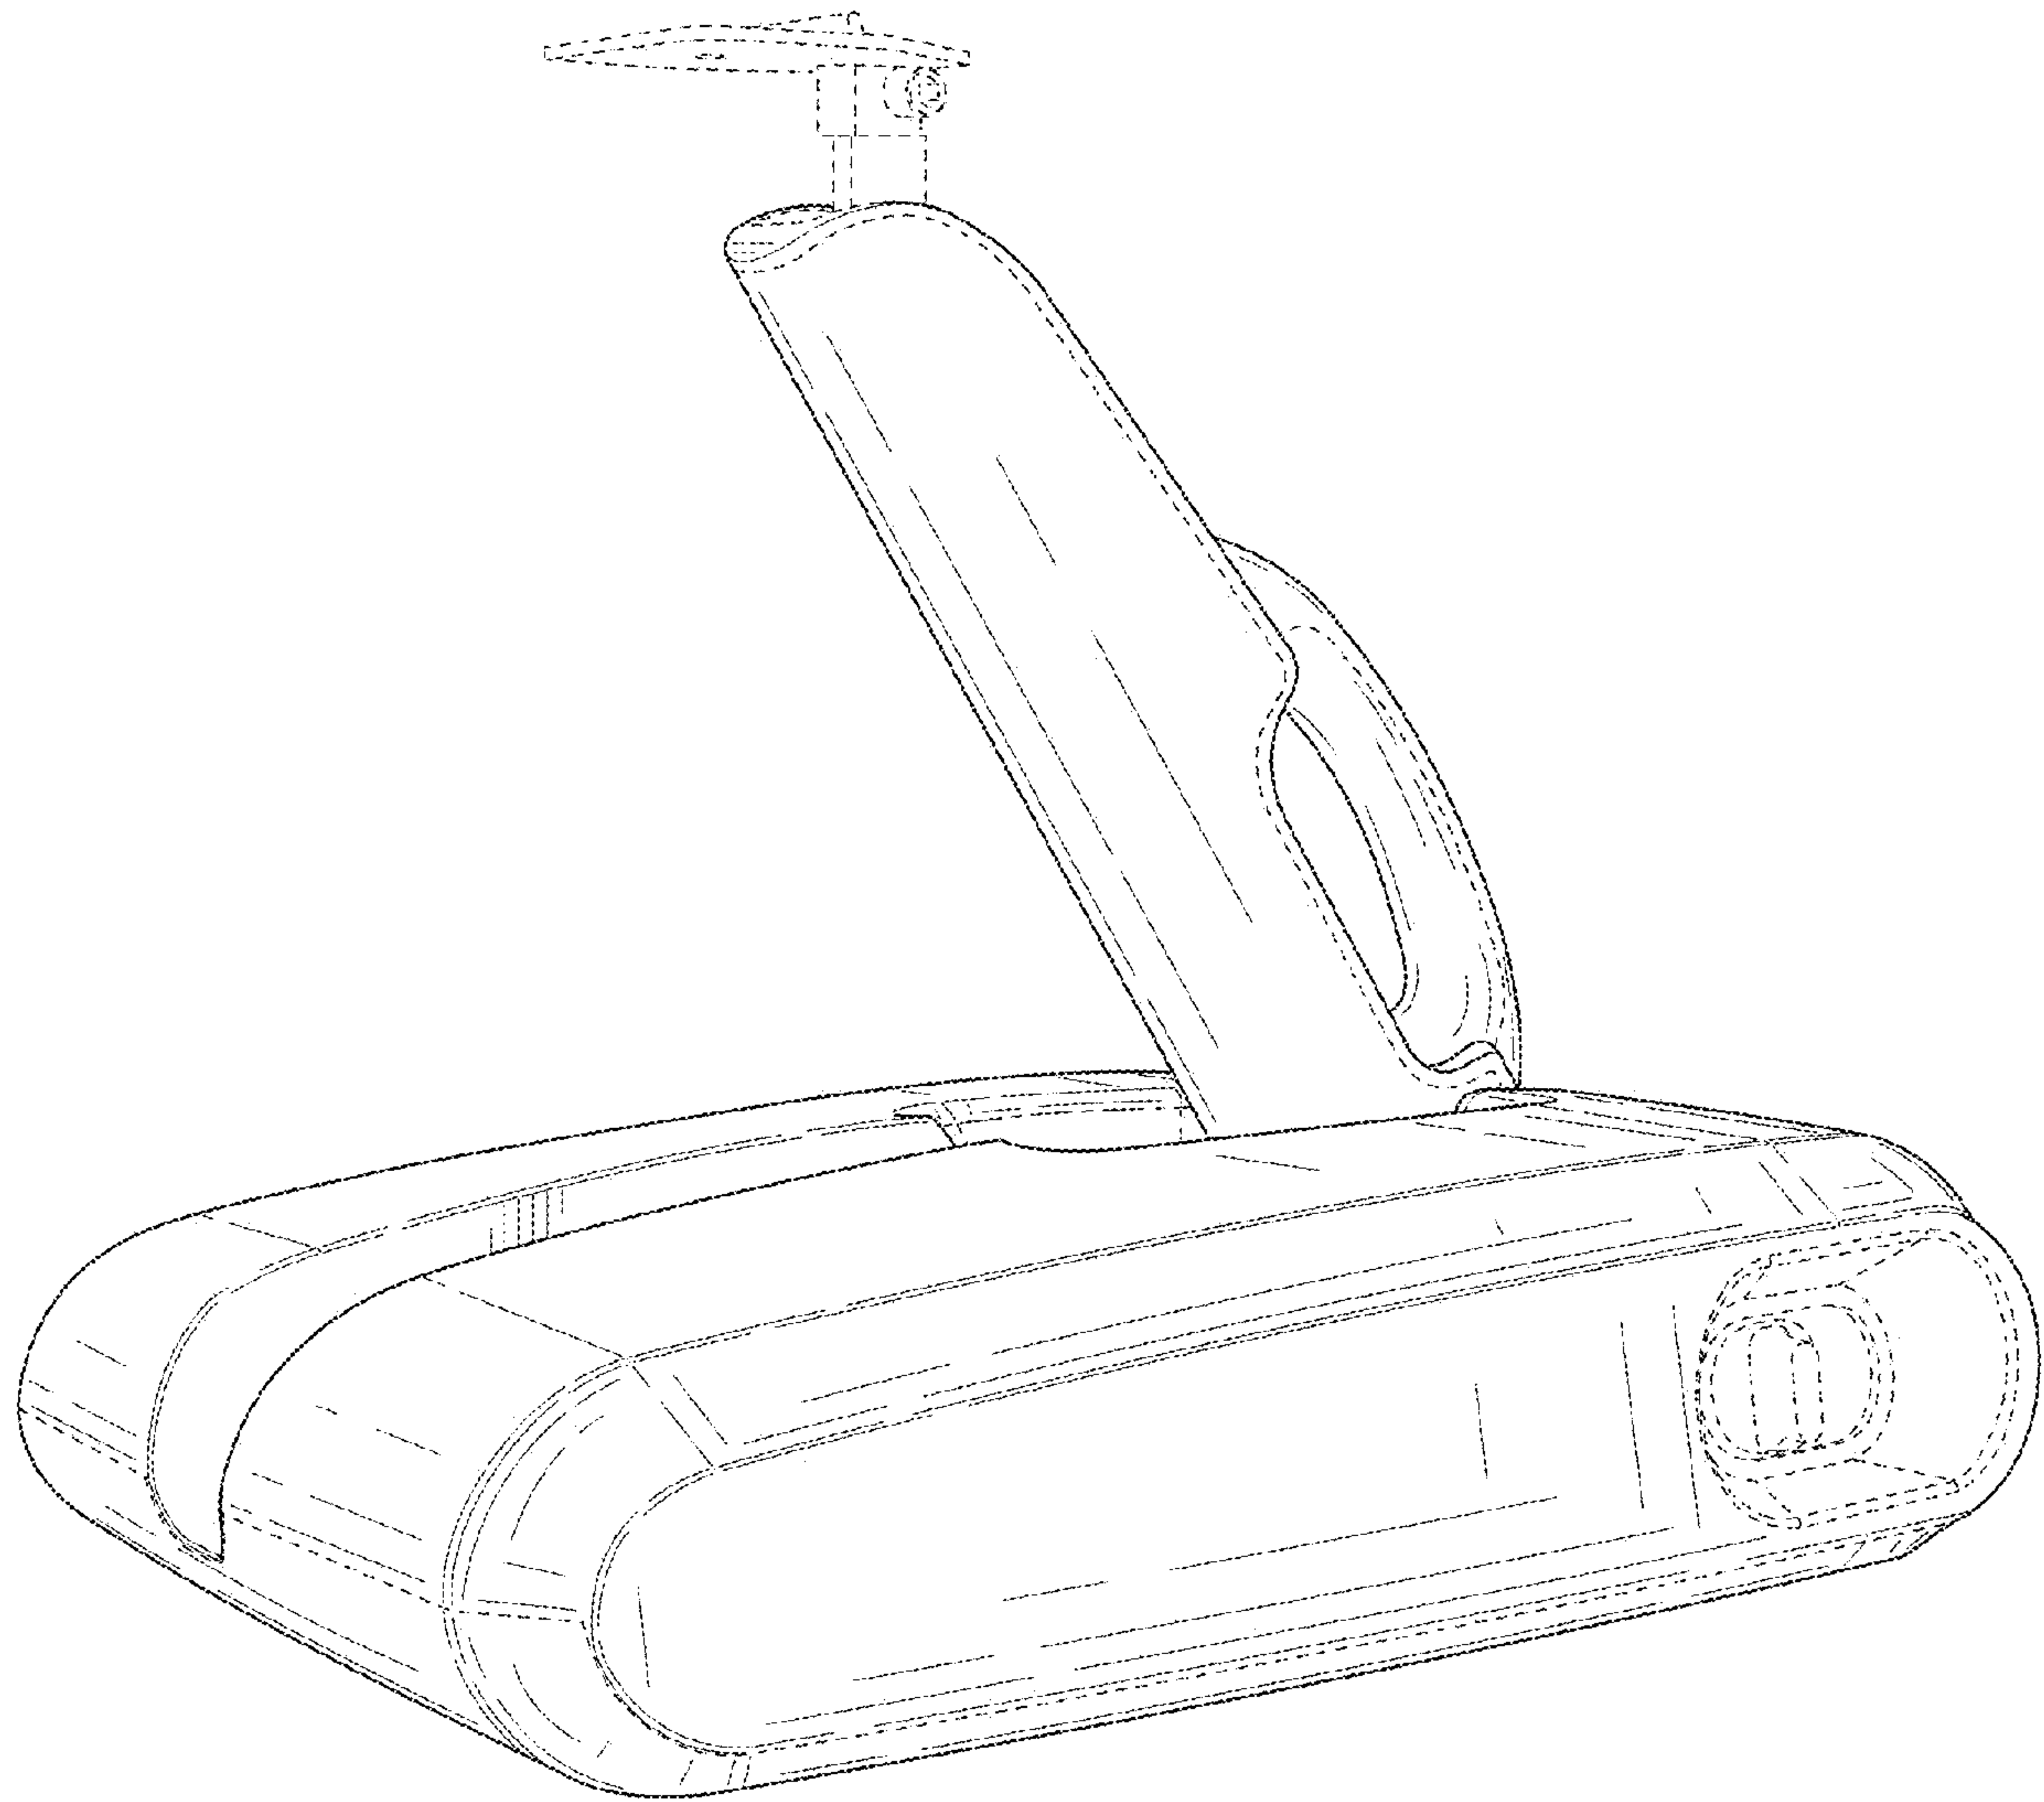


FIG. 1

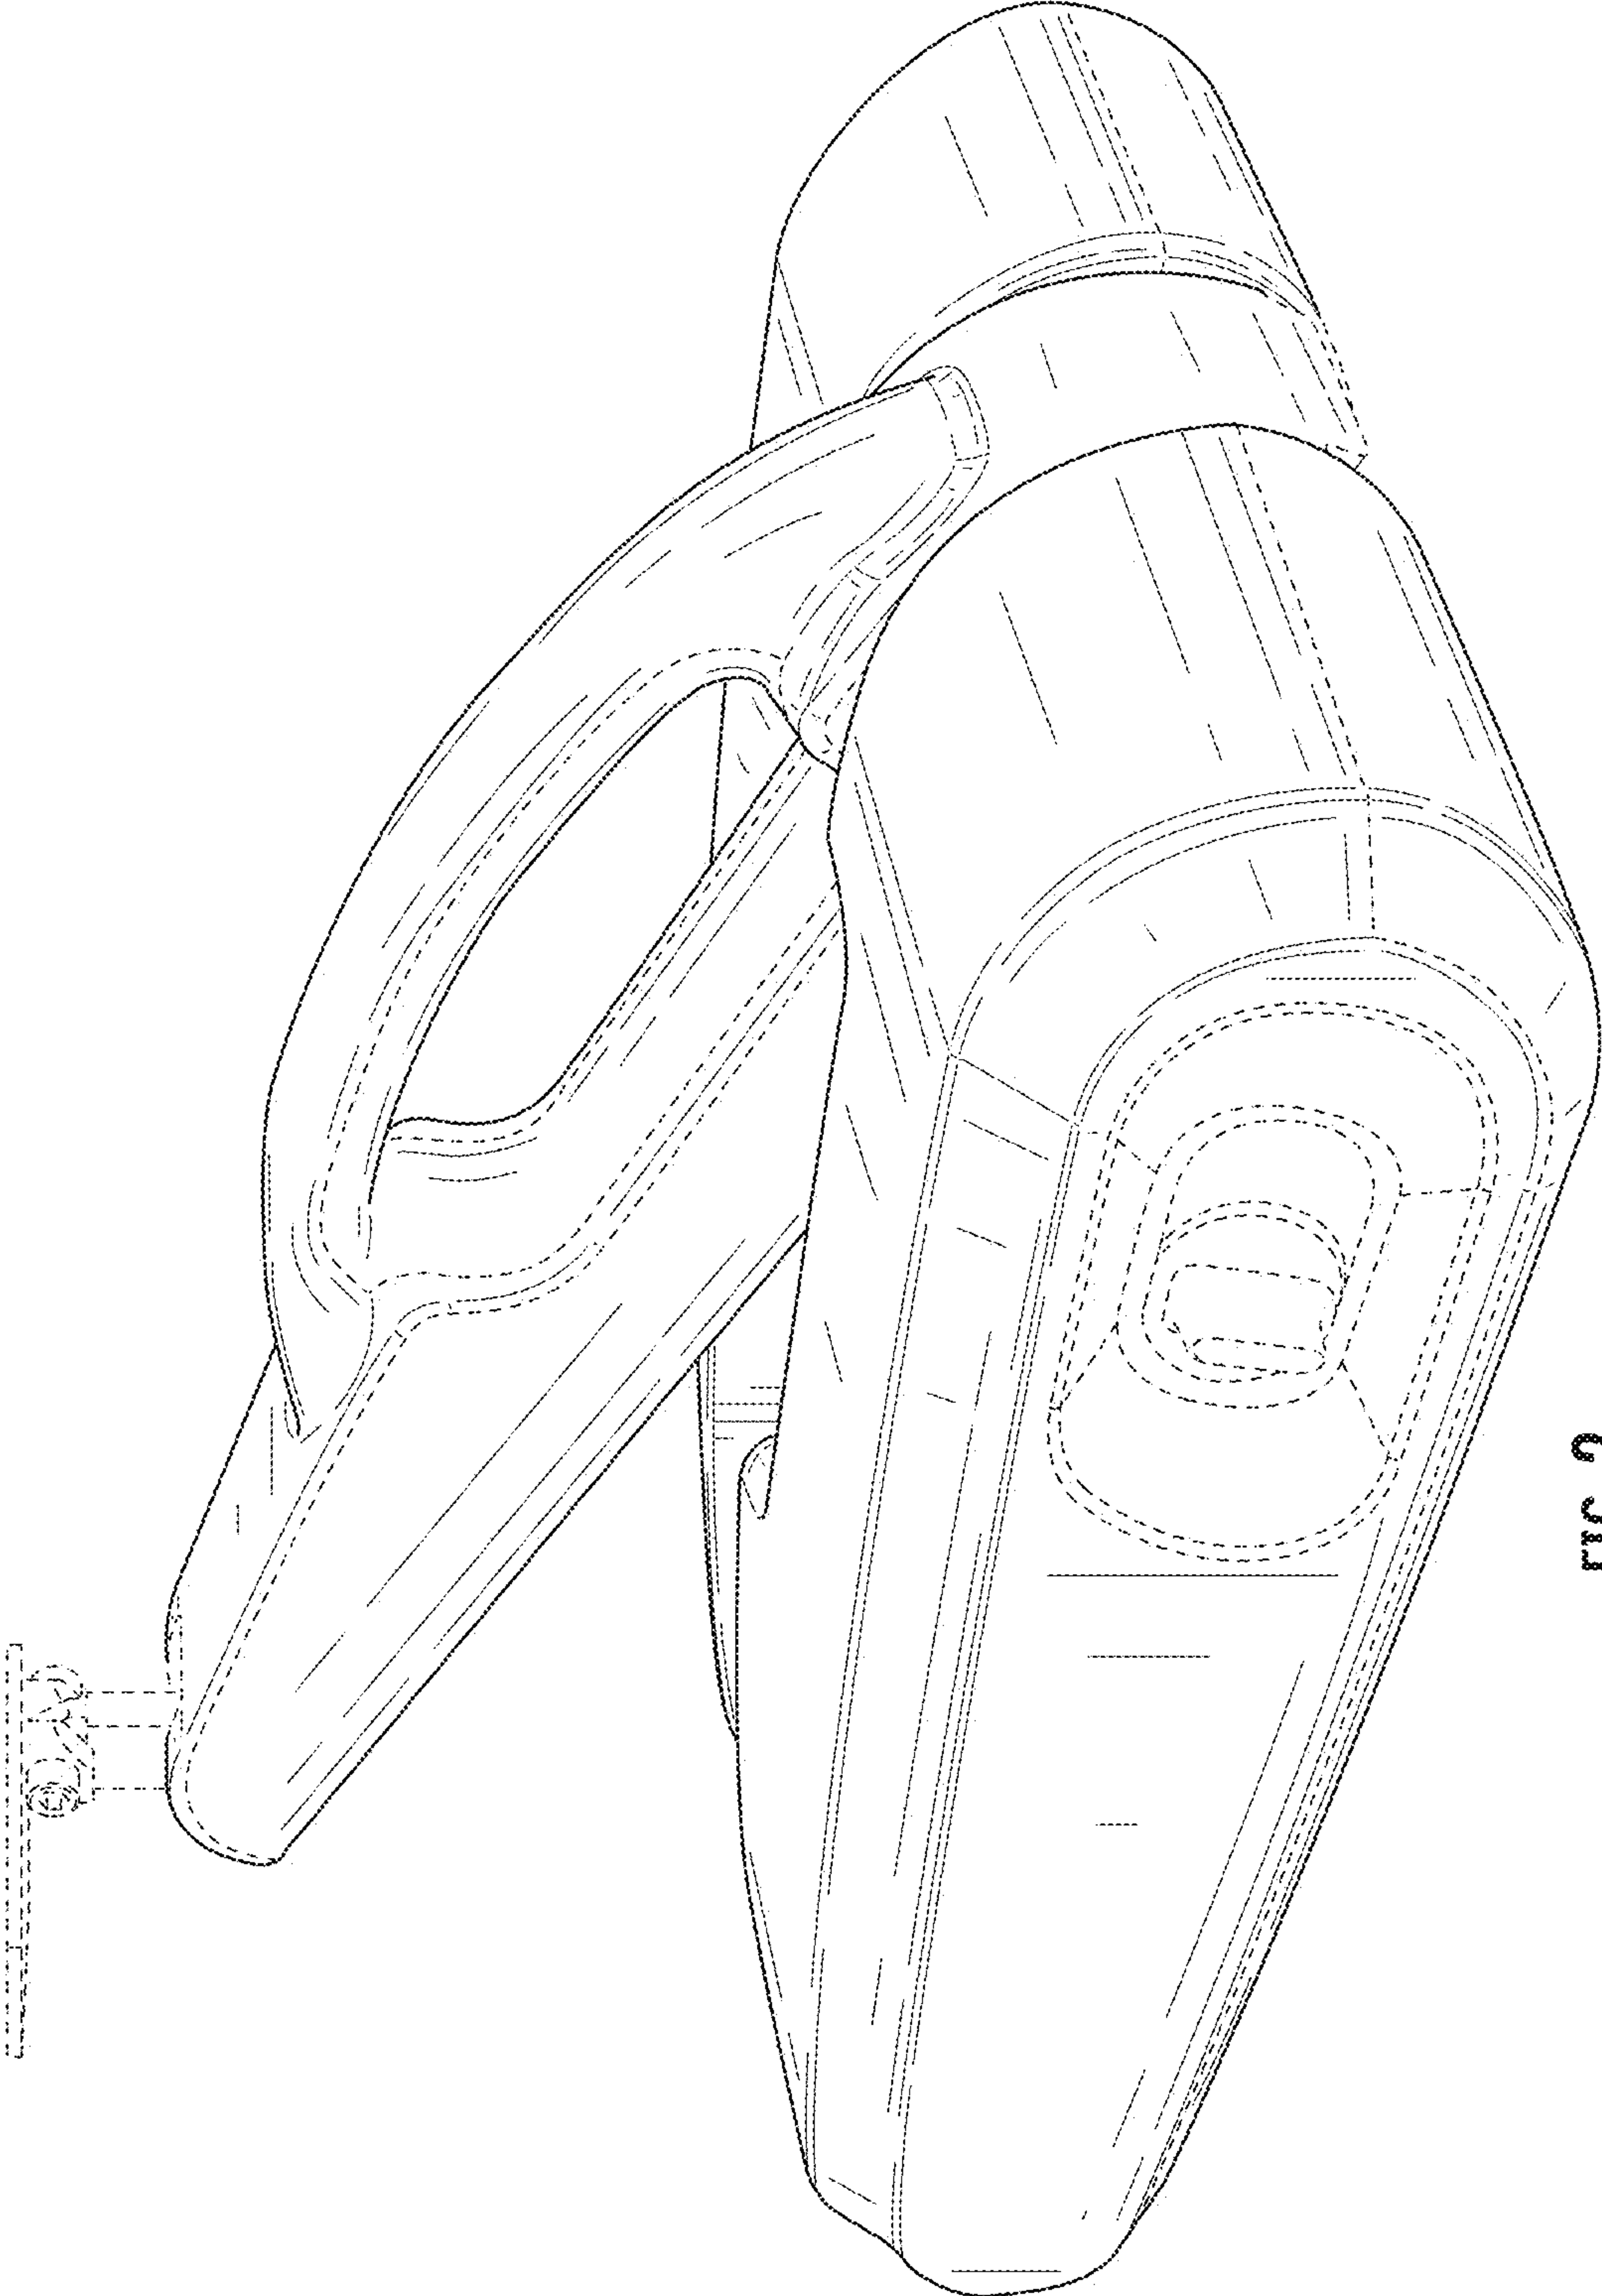


FIG. 2

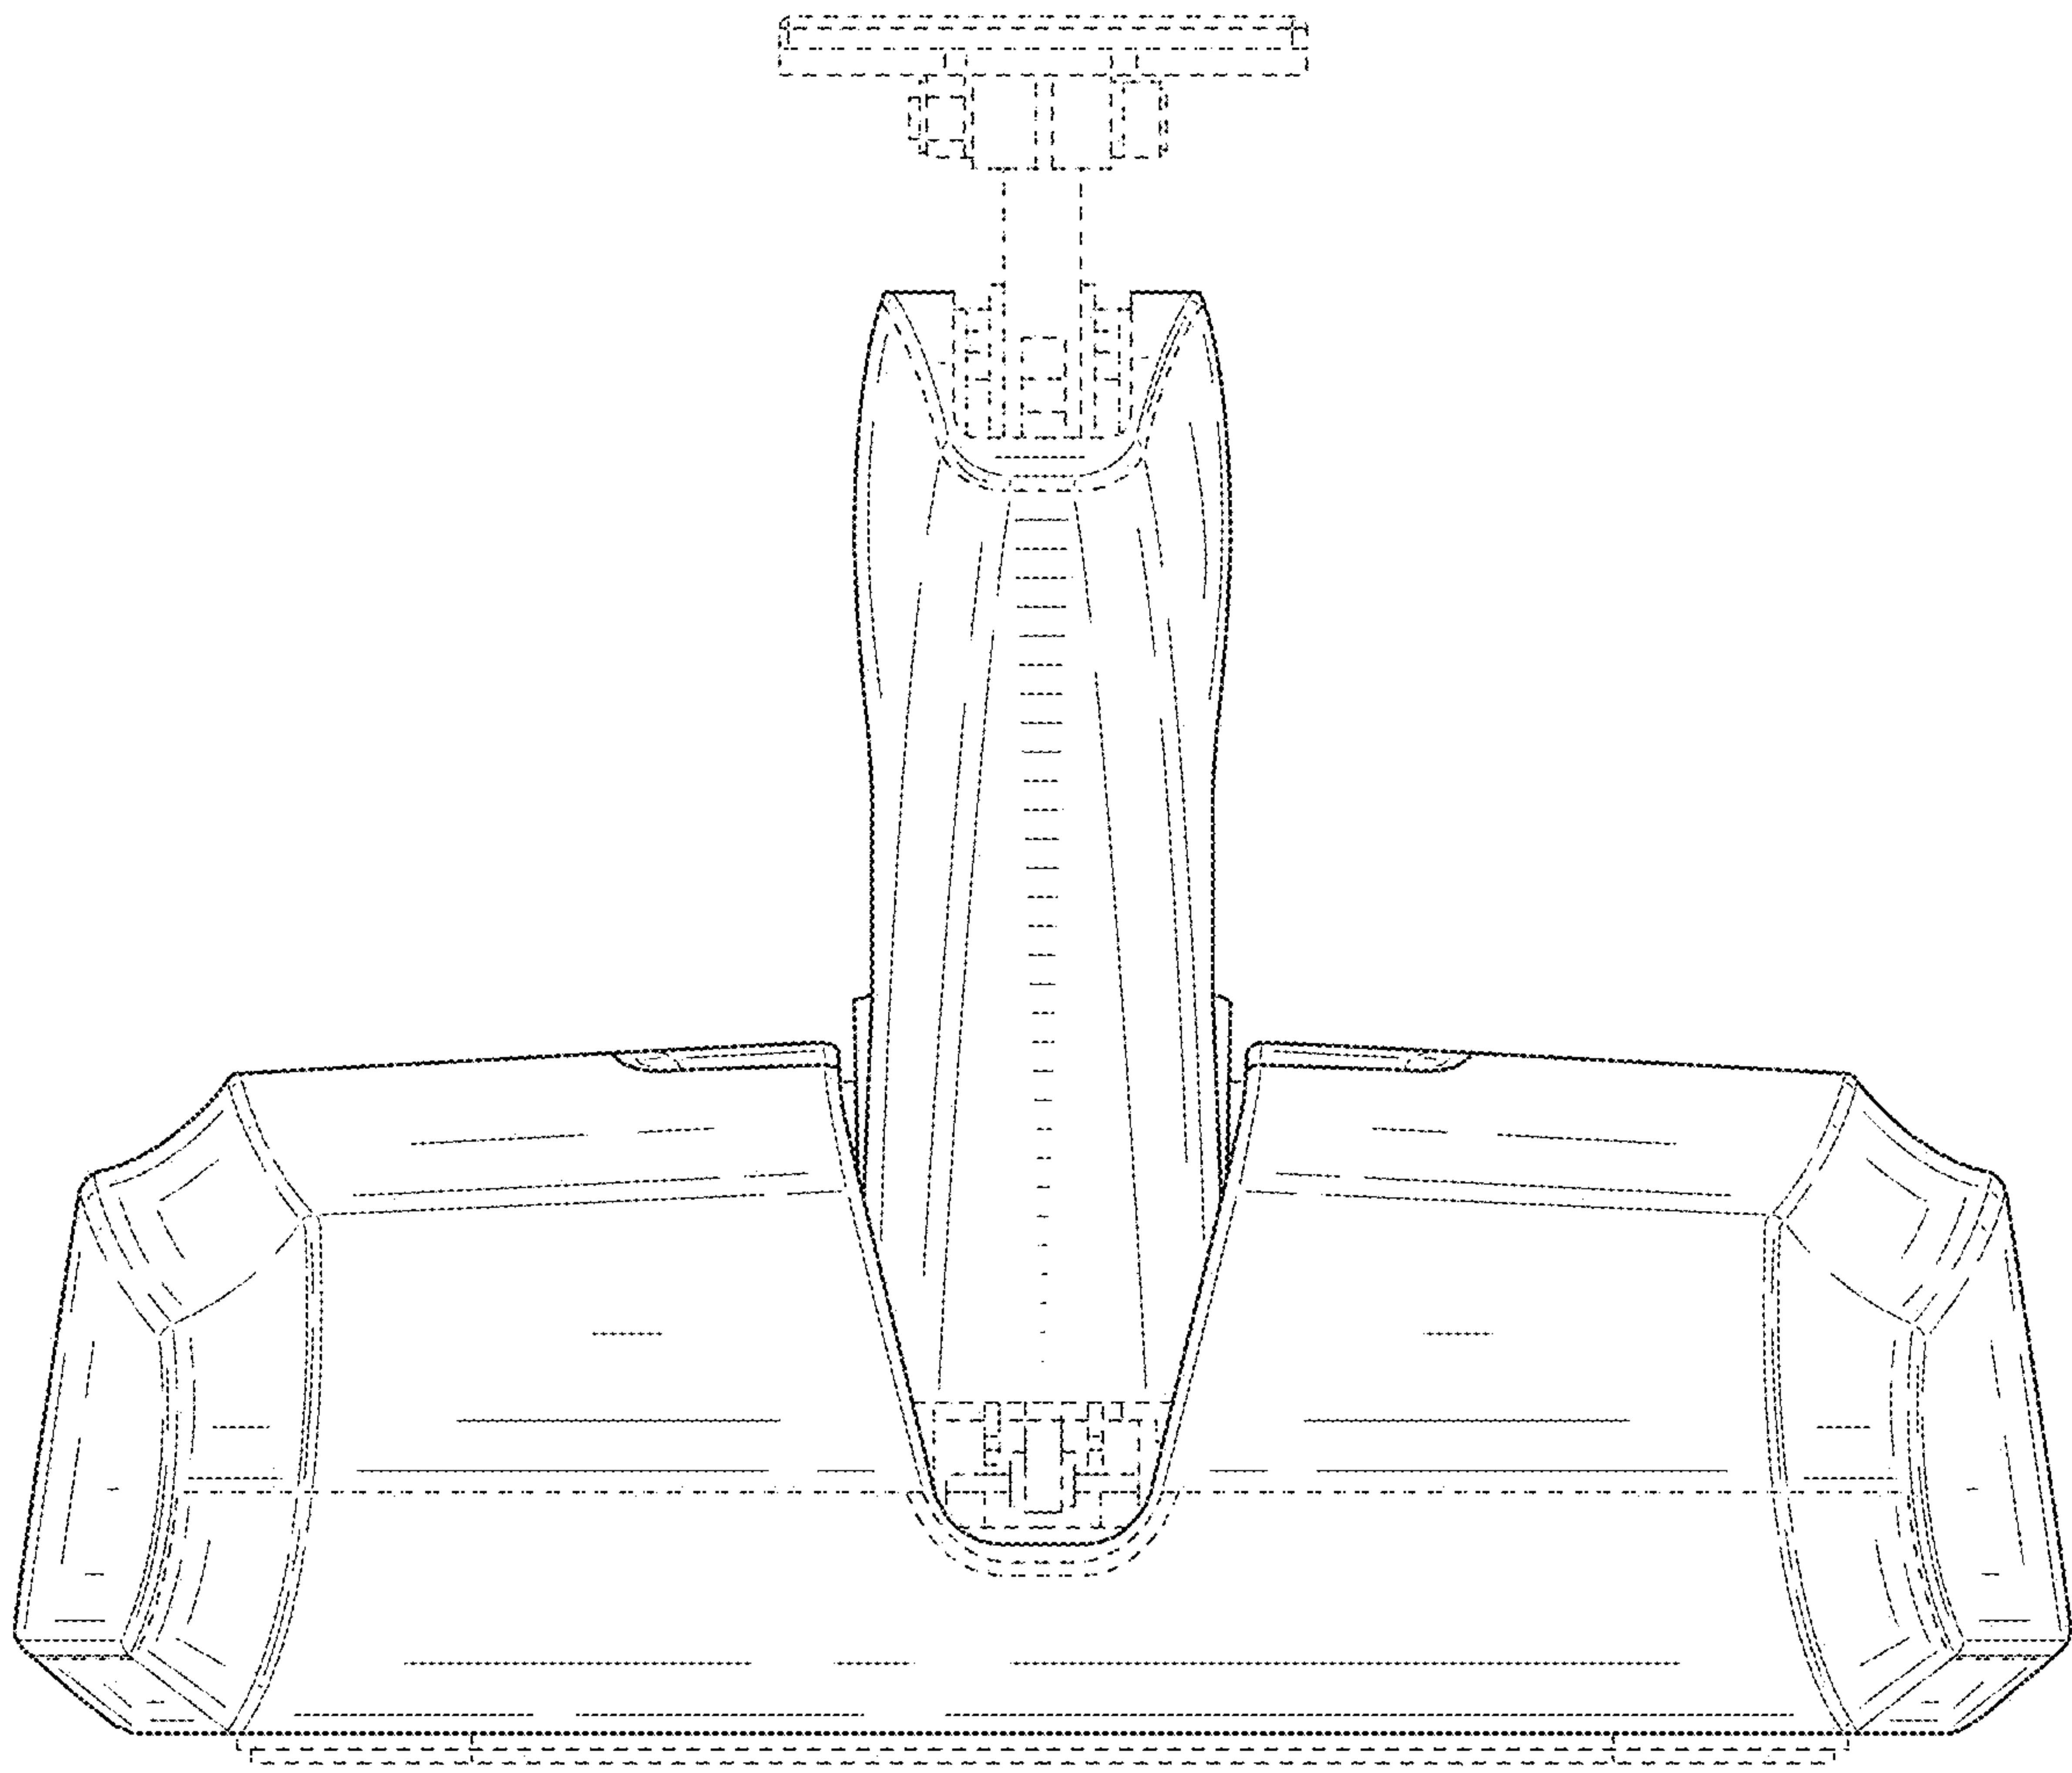


FIG. 3

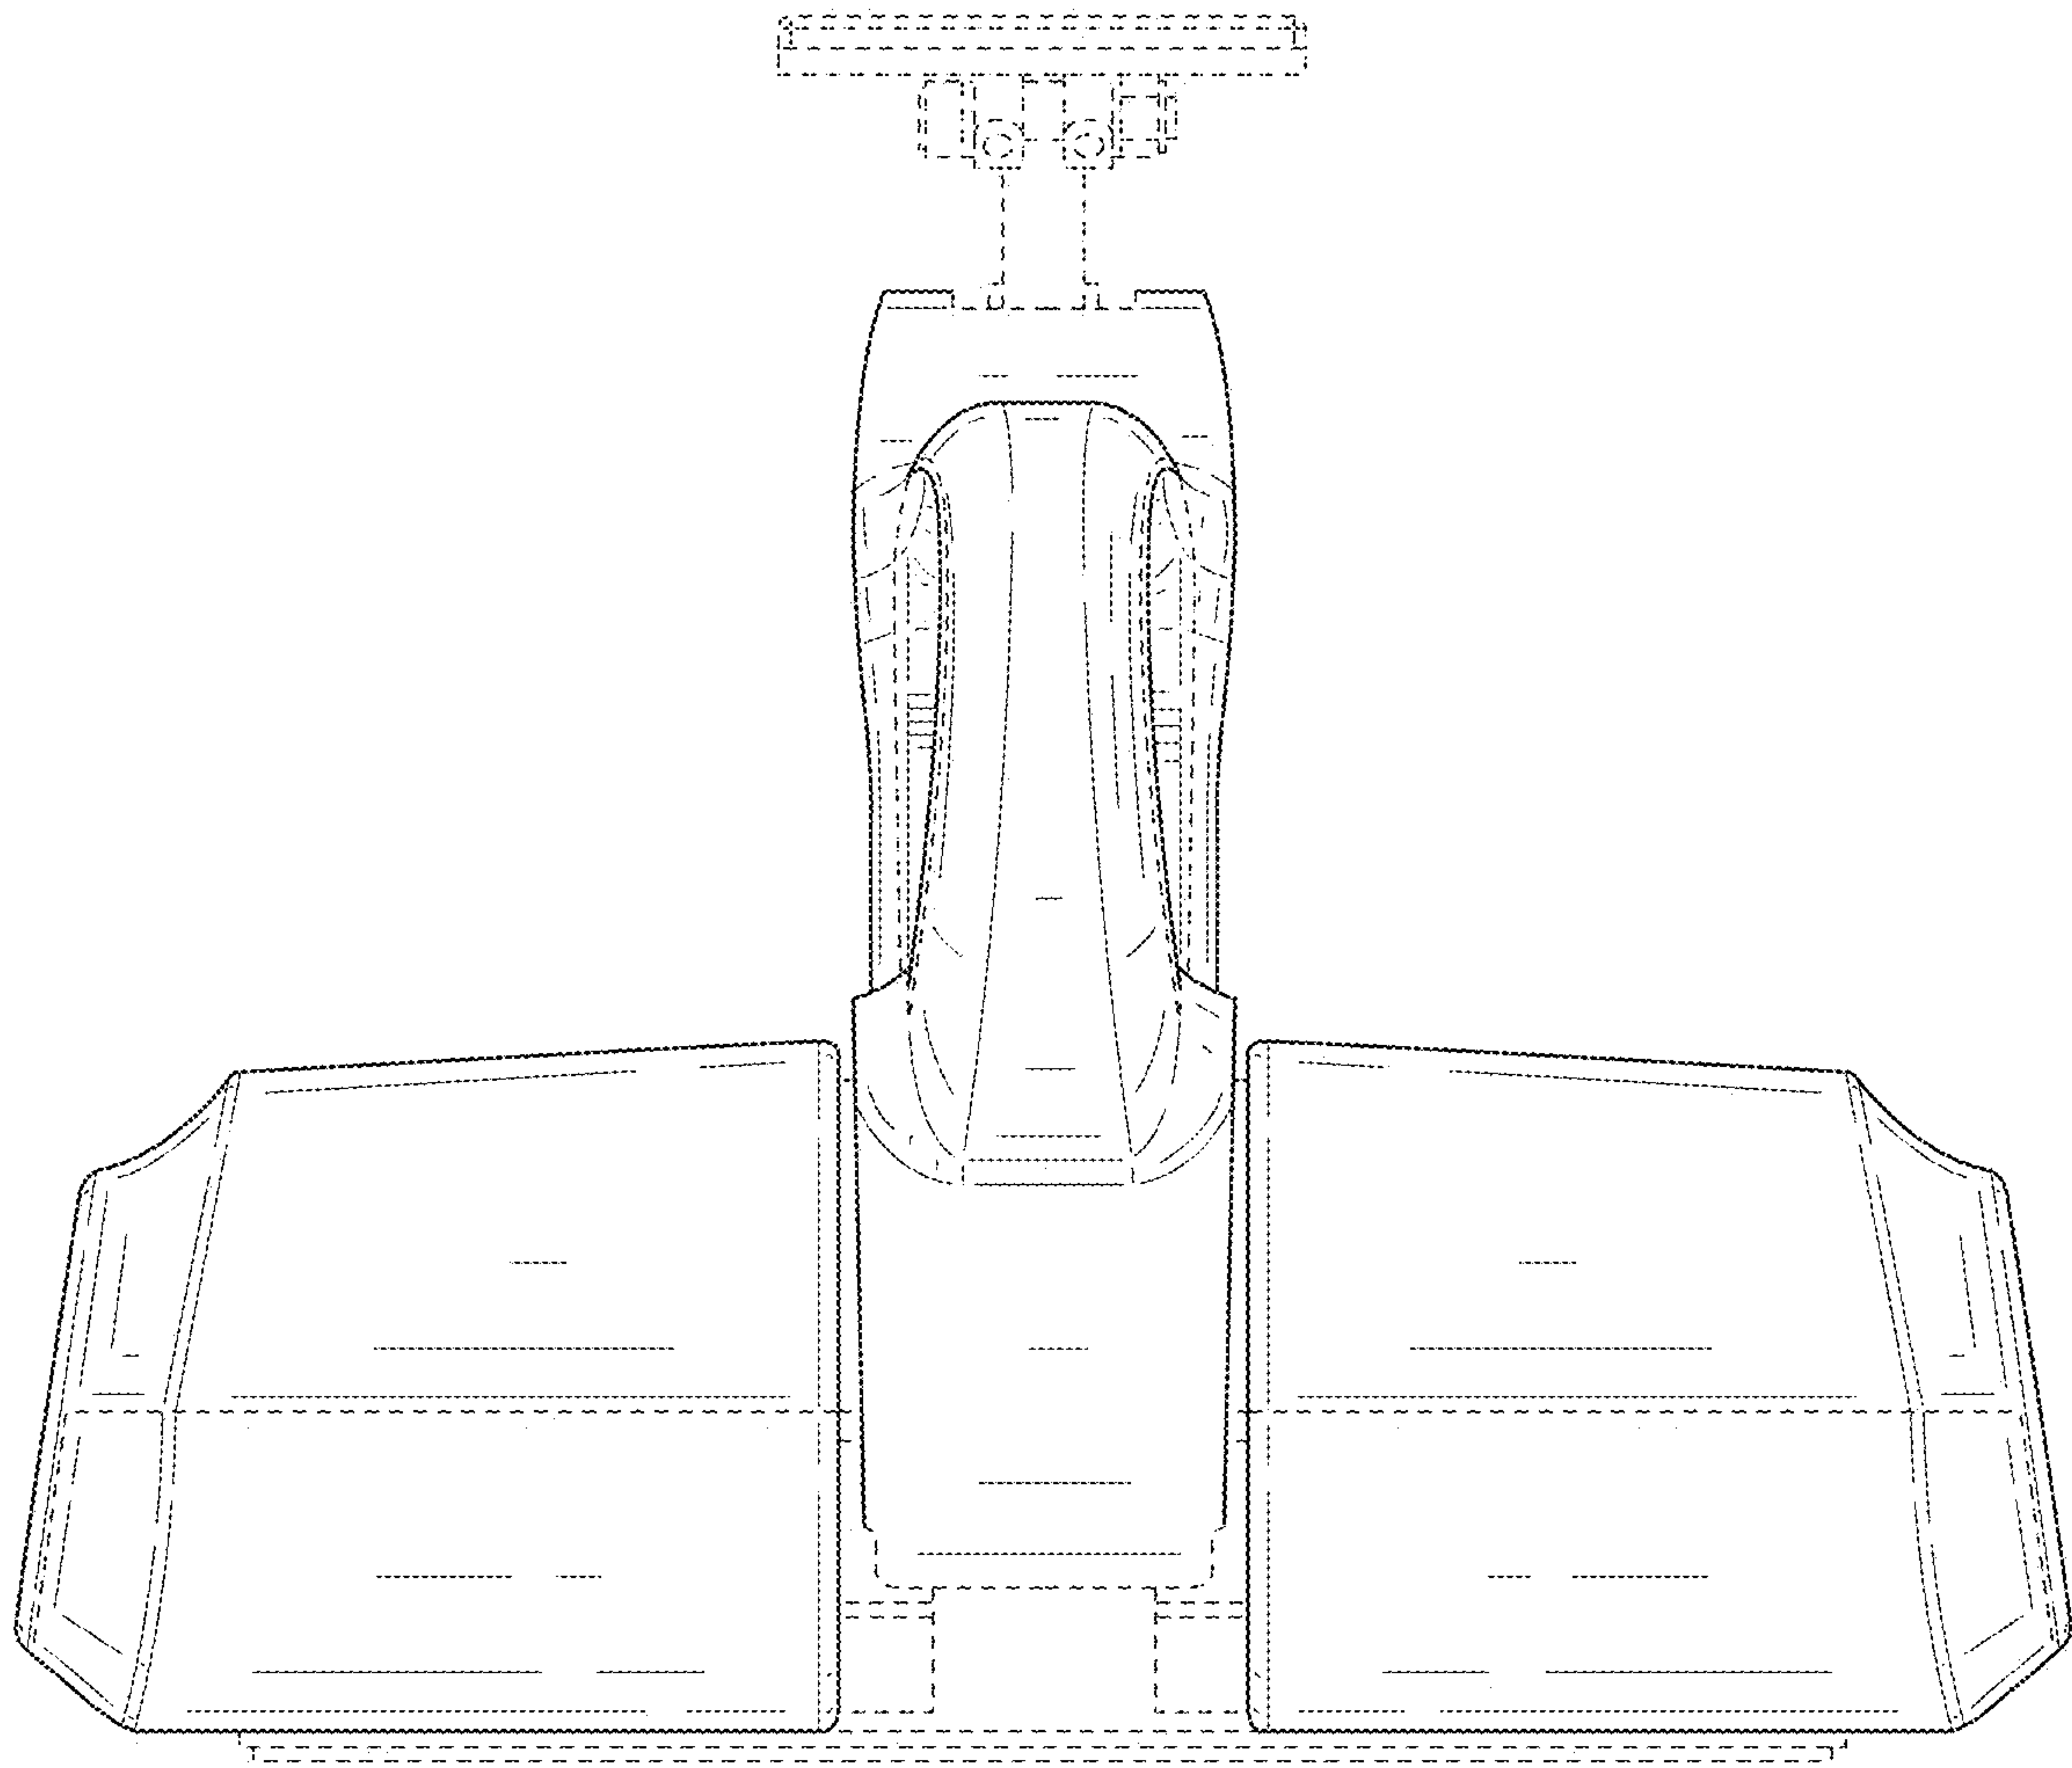


FIG. 4

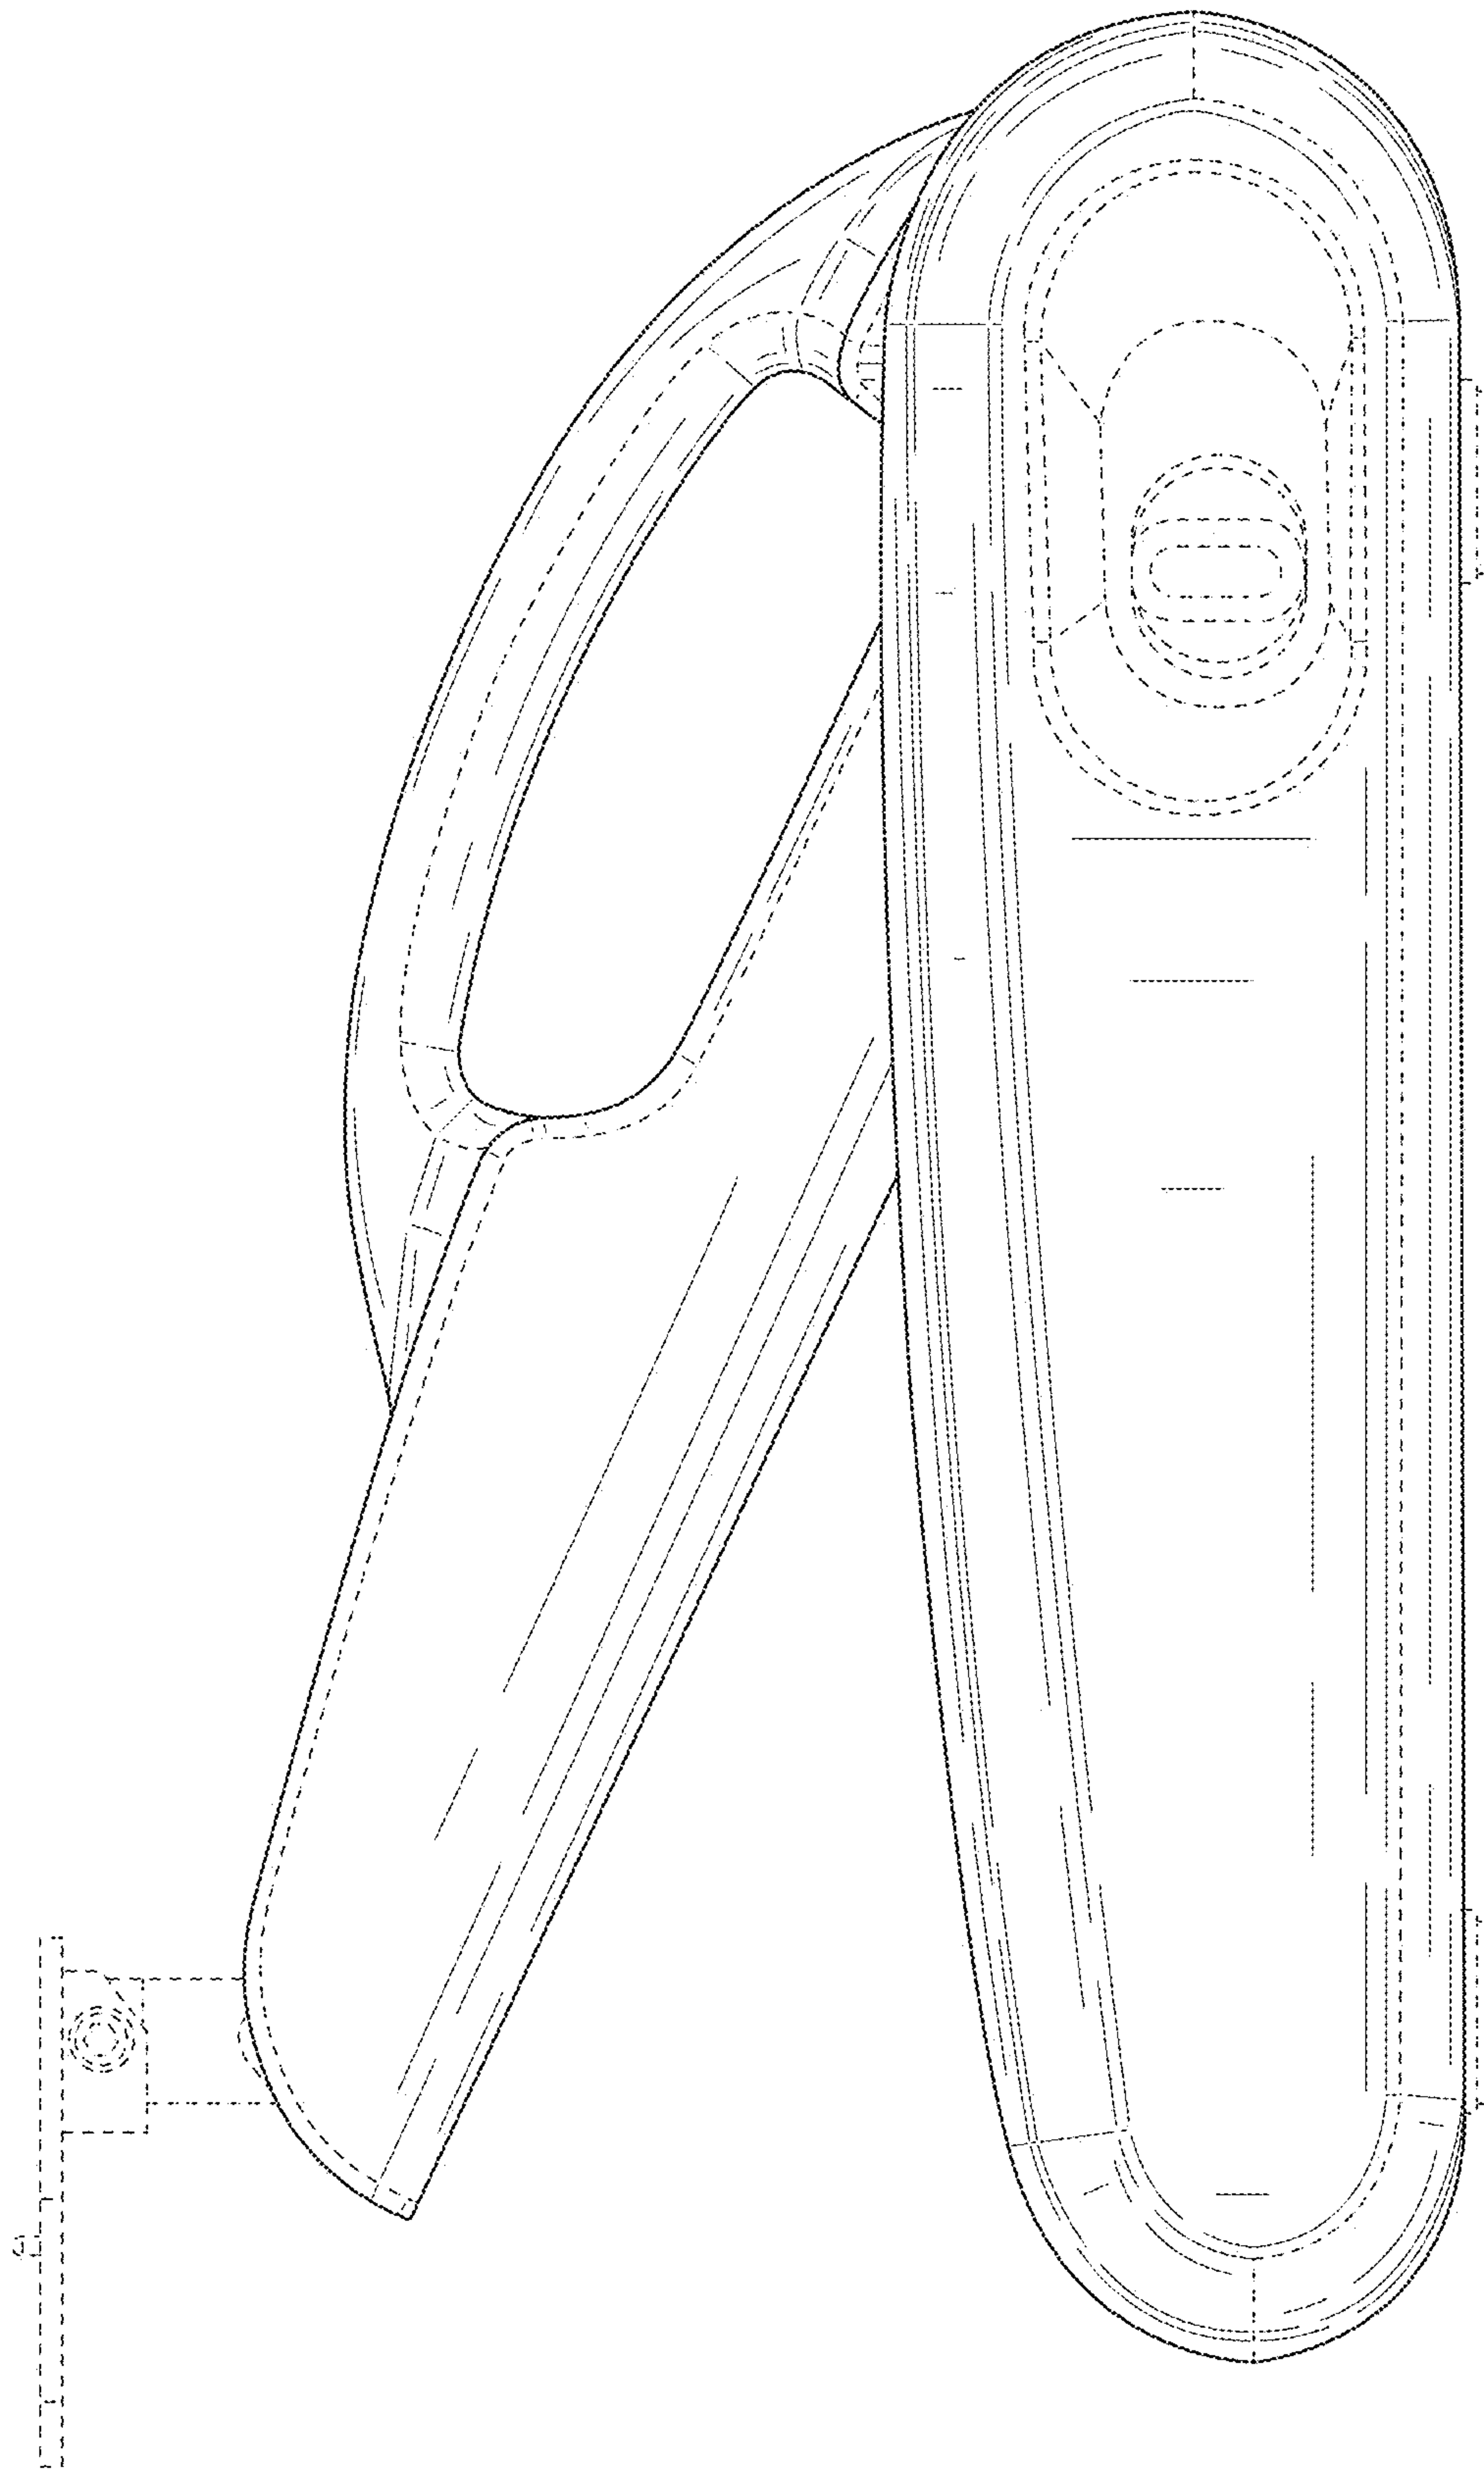


FIG. 5

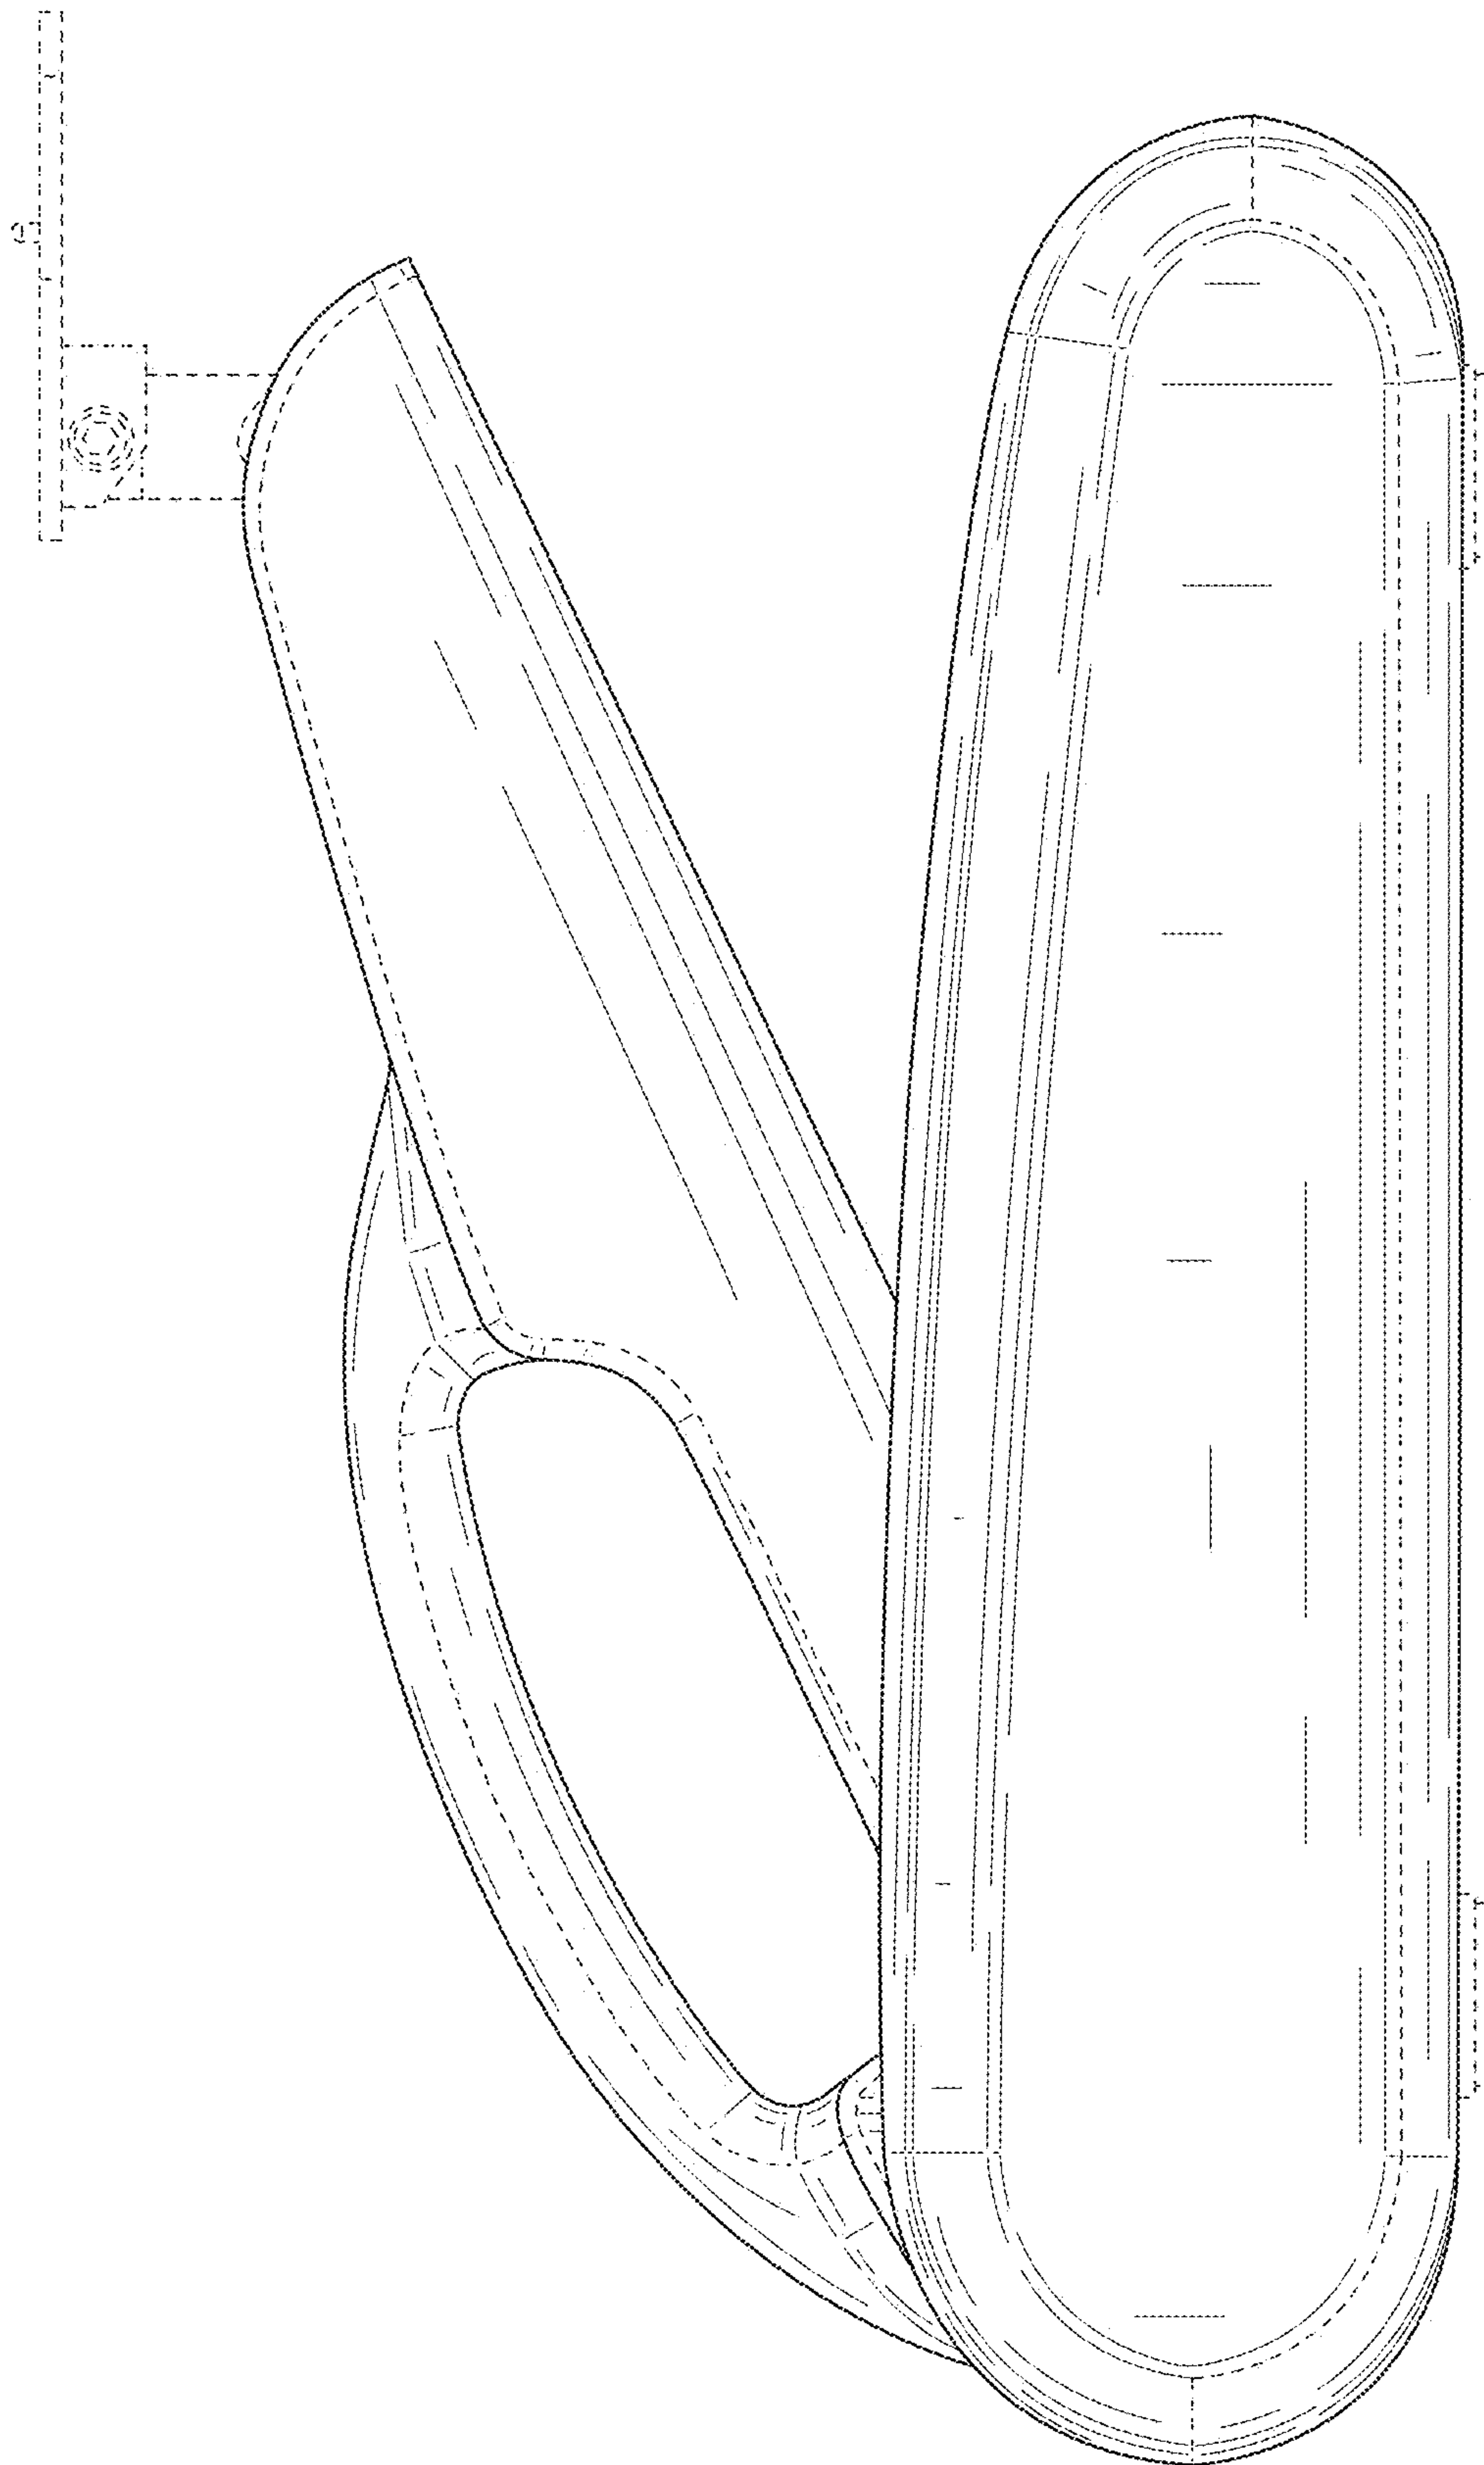


FIG. 6

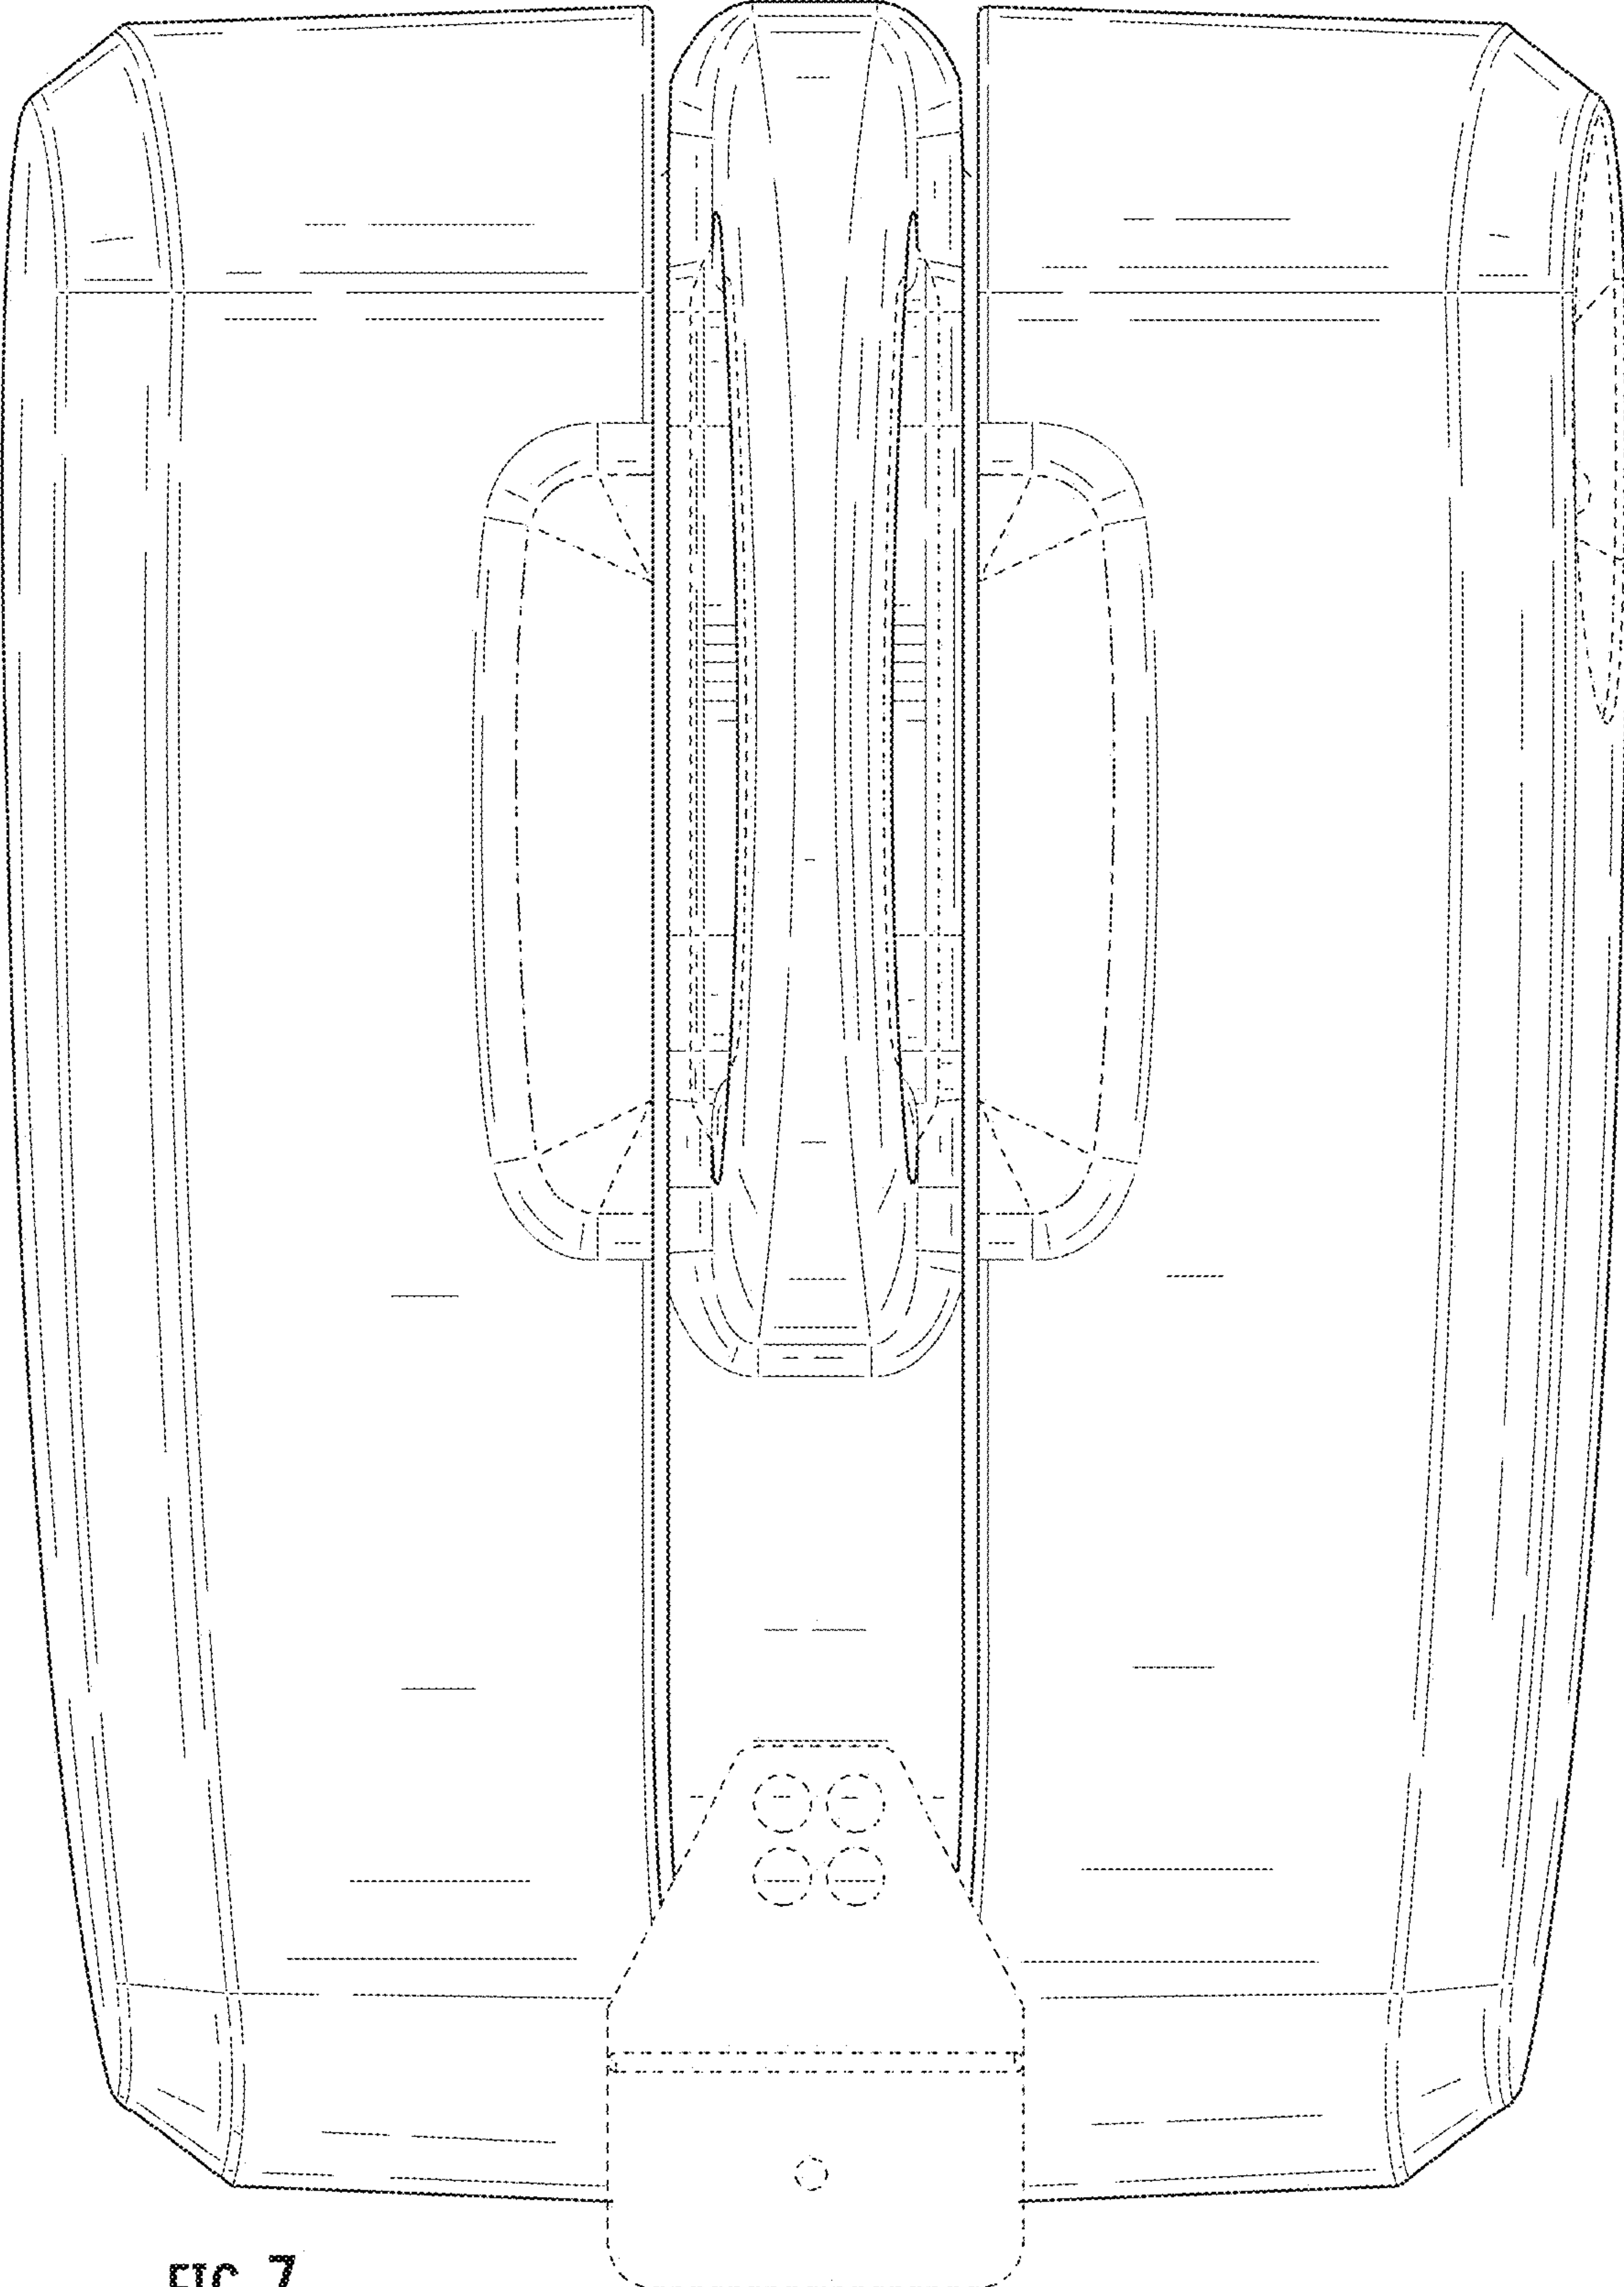


FIG. 7

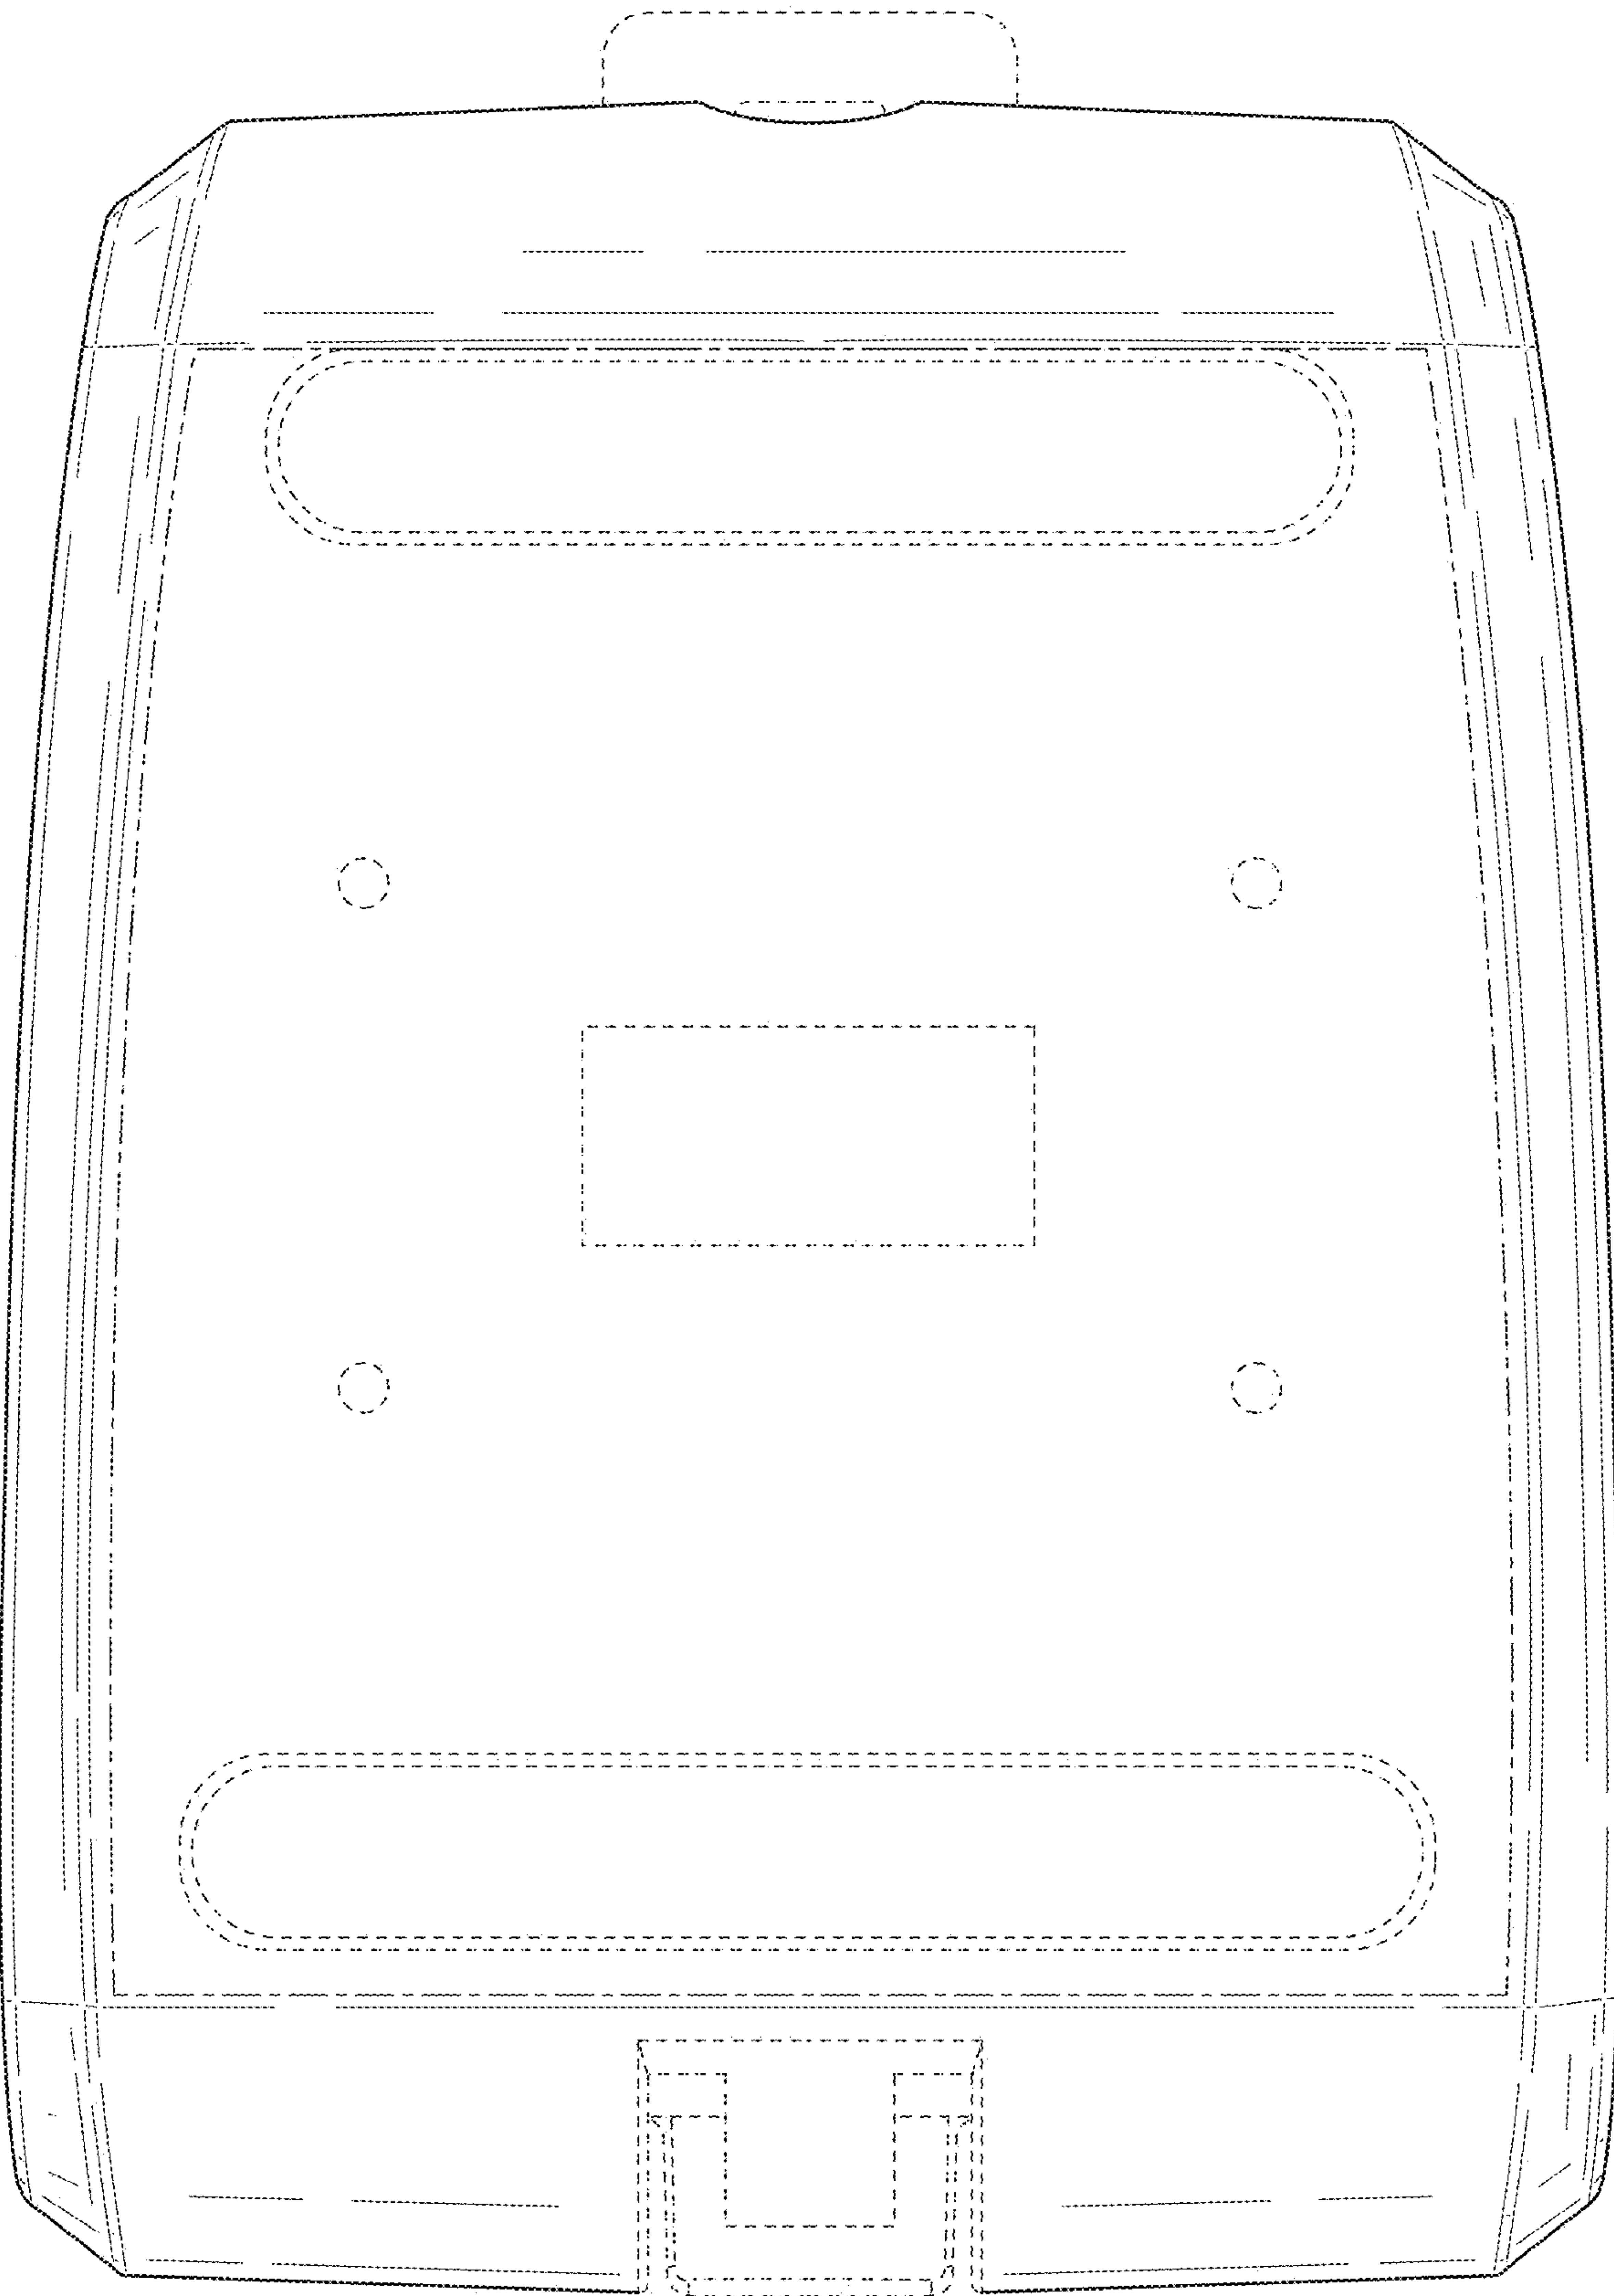


FIG. 8

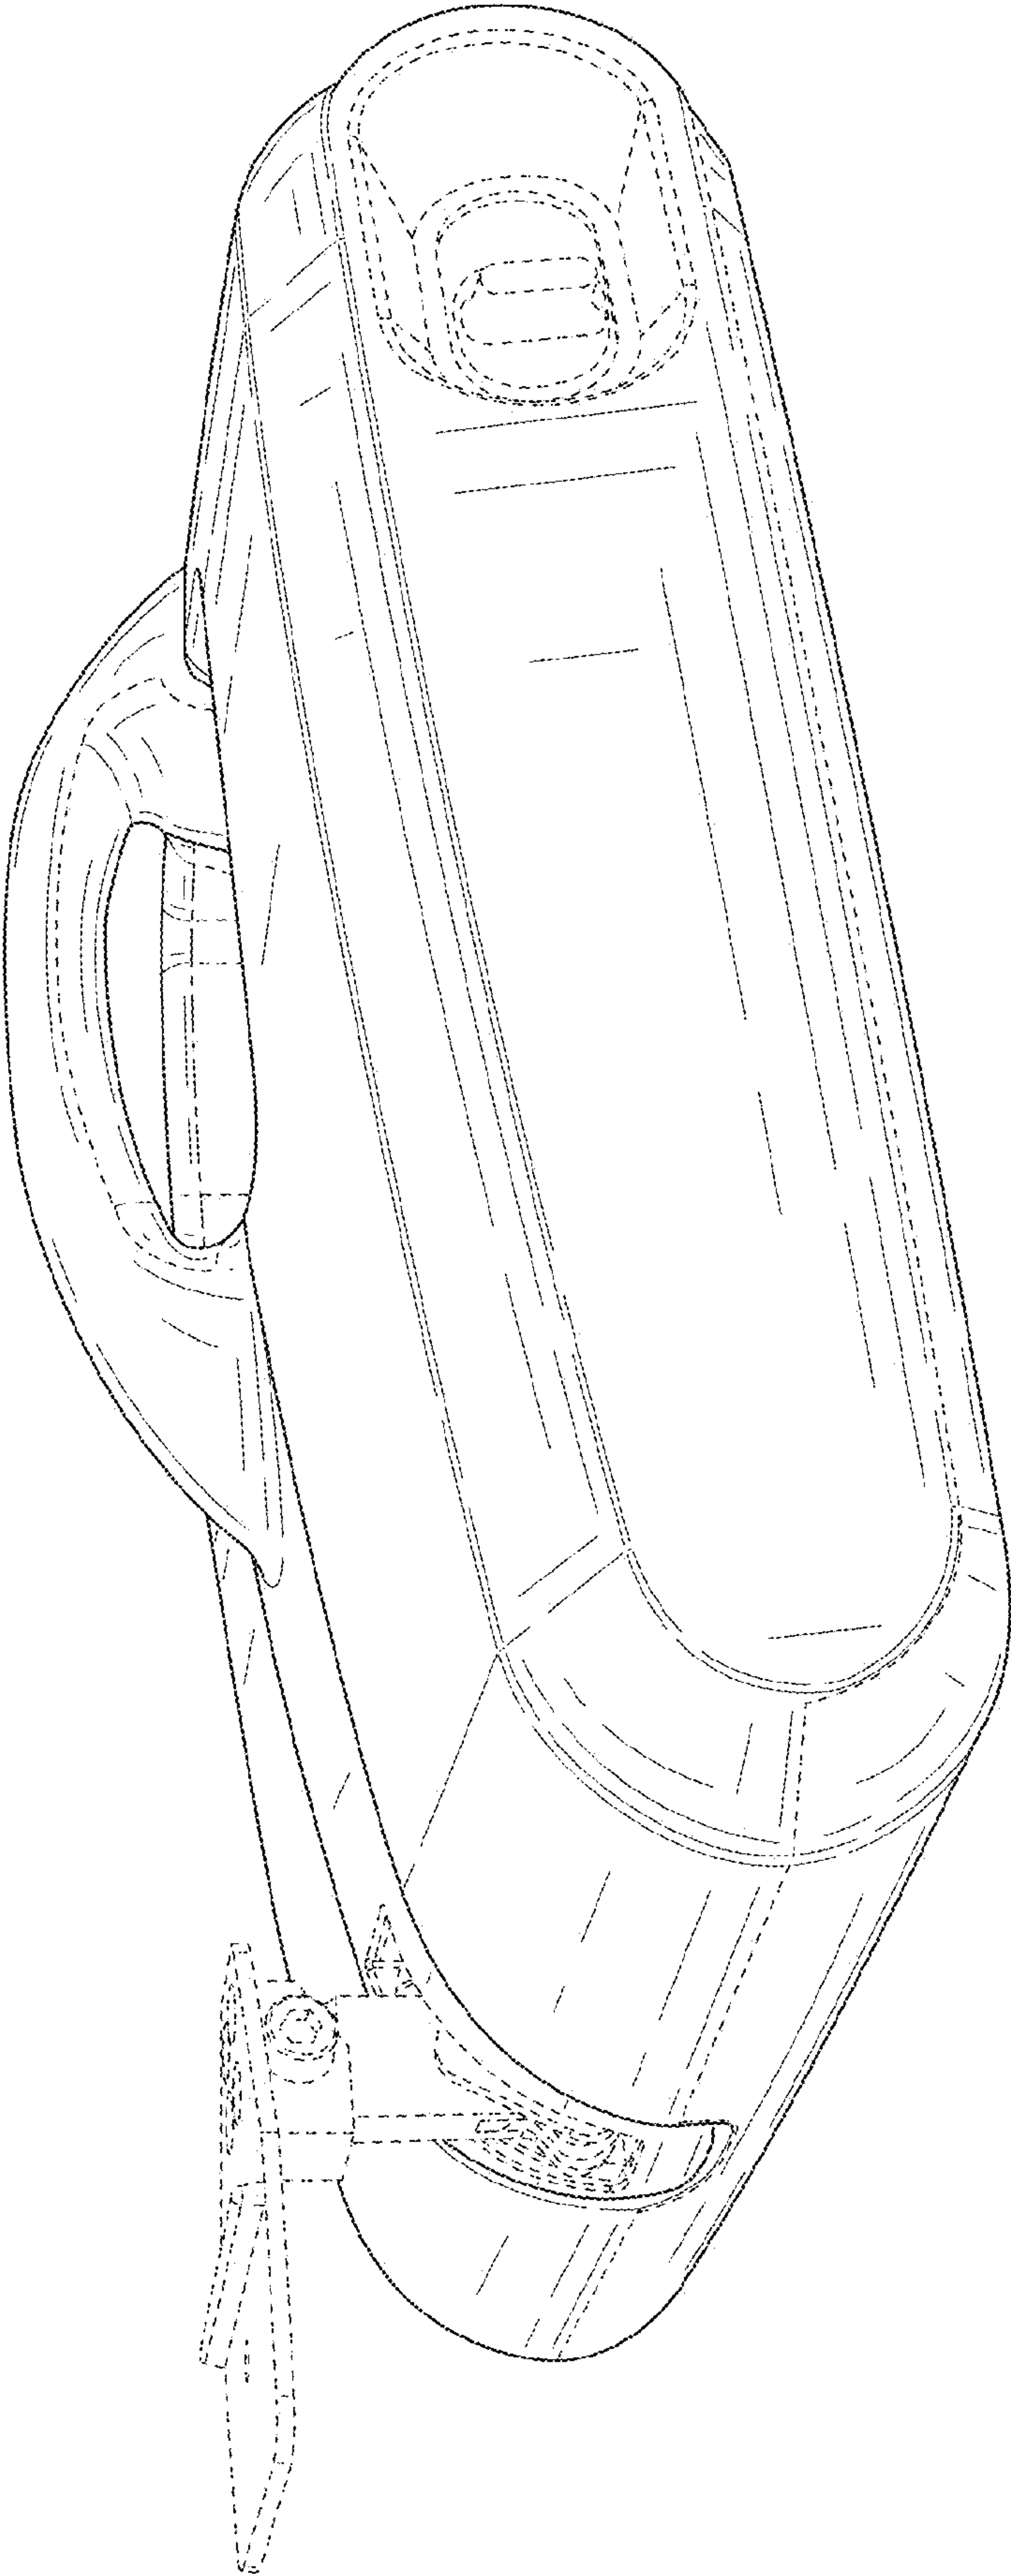


FIG. 9

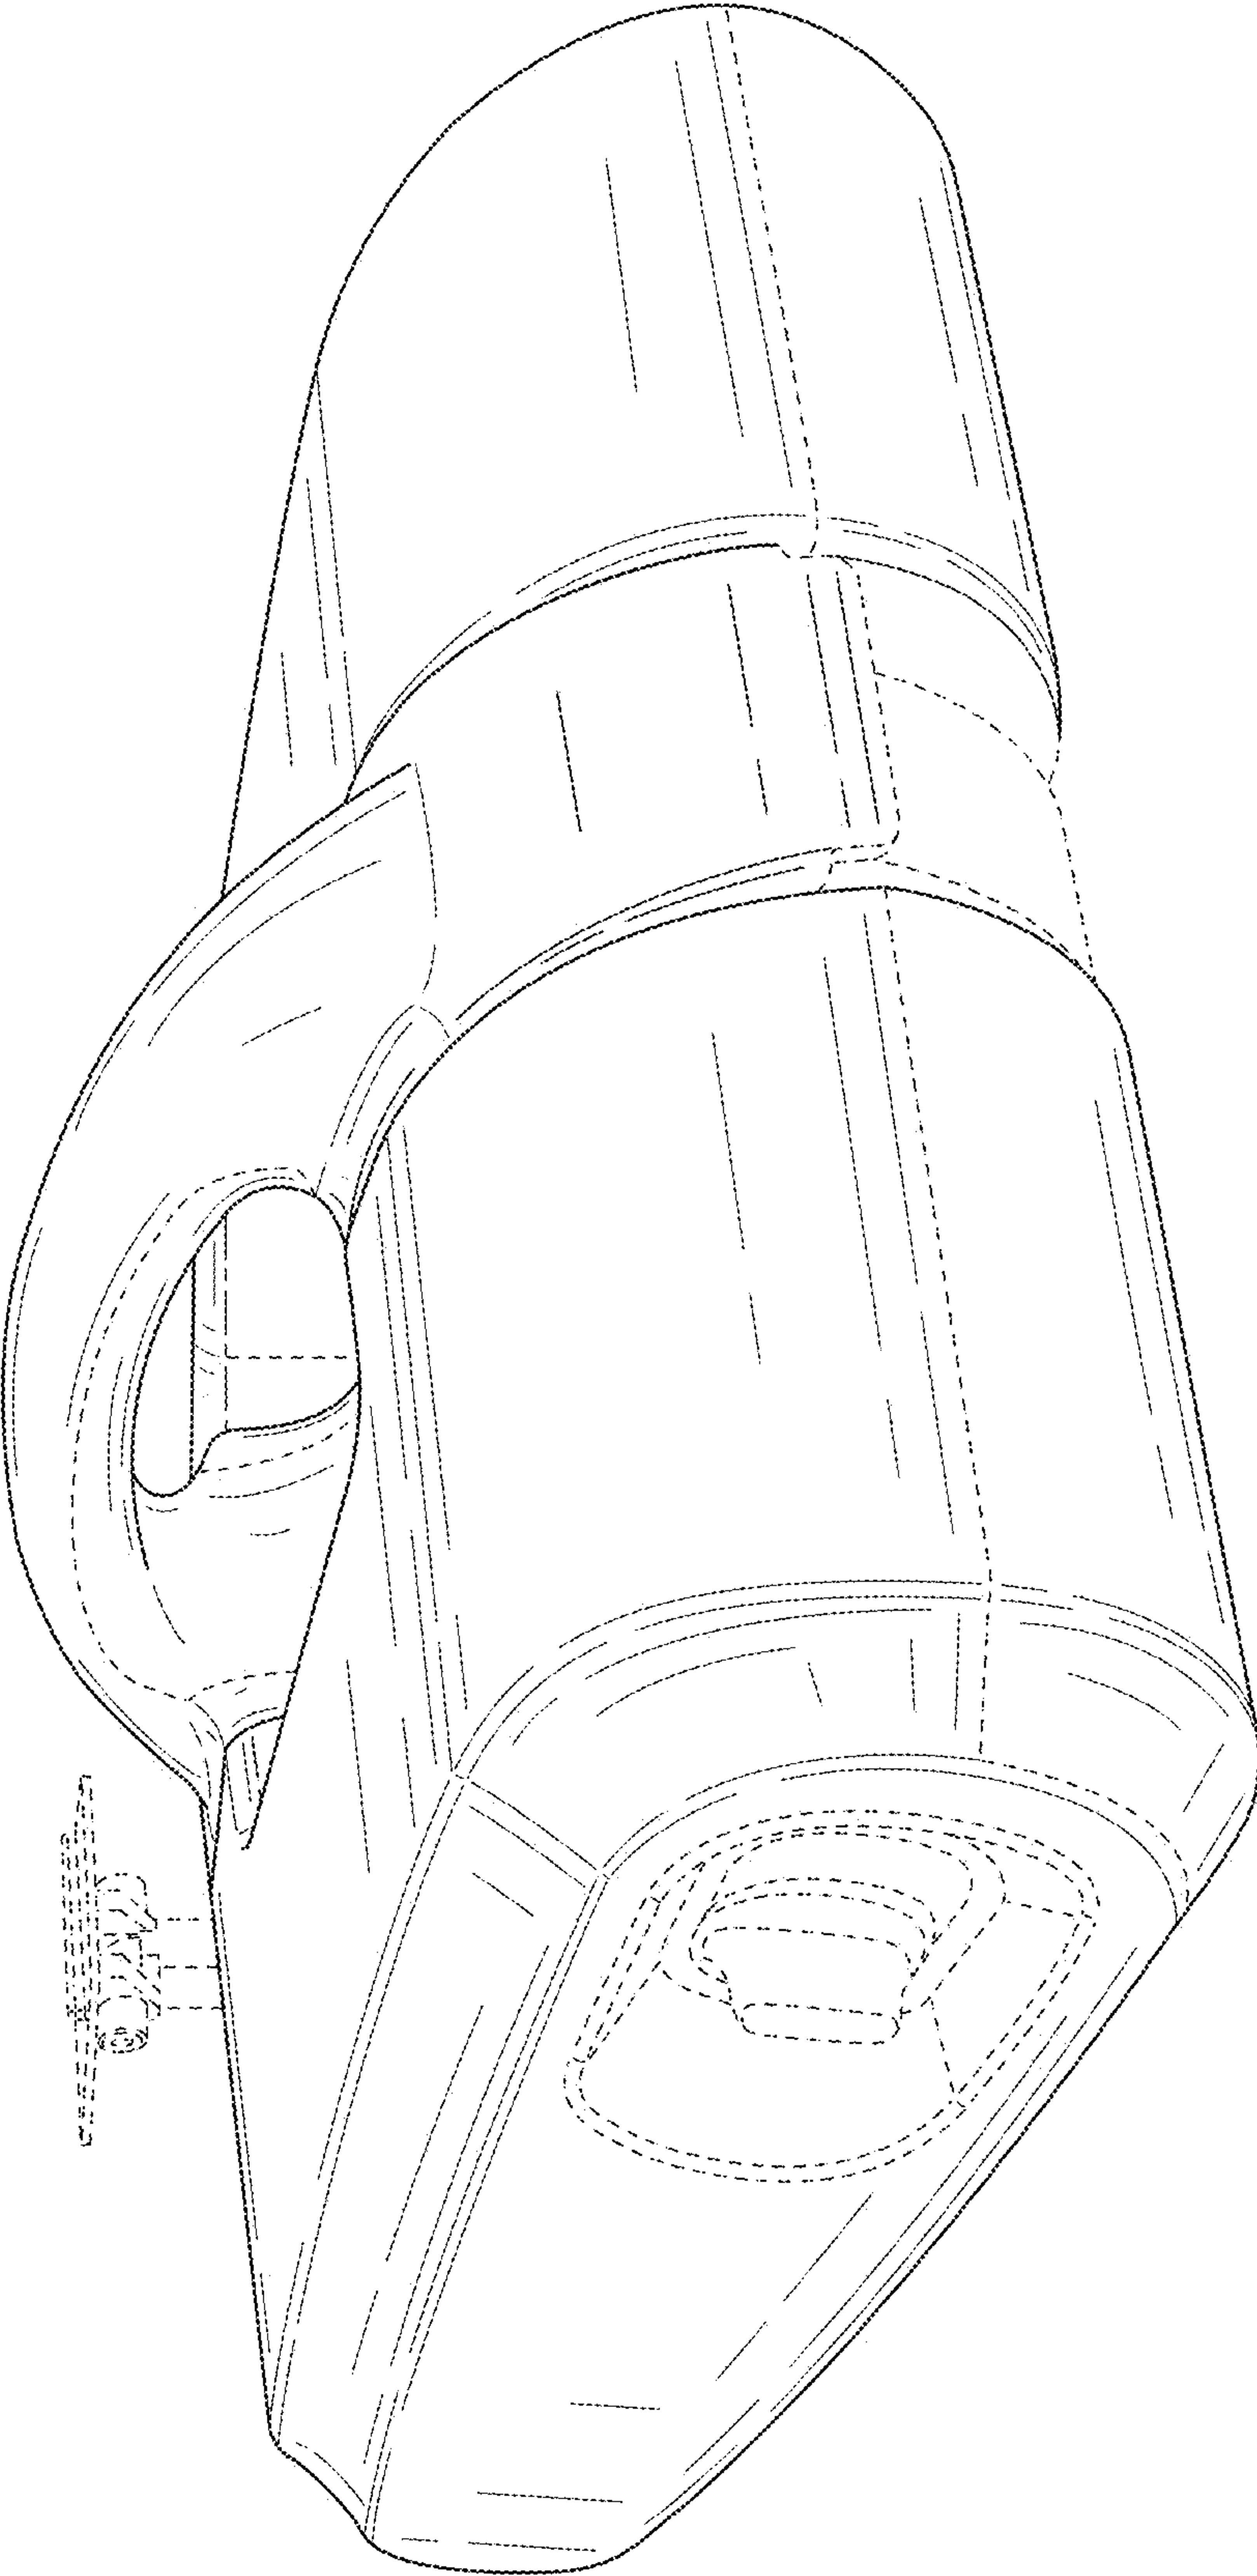


FIG. 10

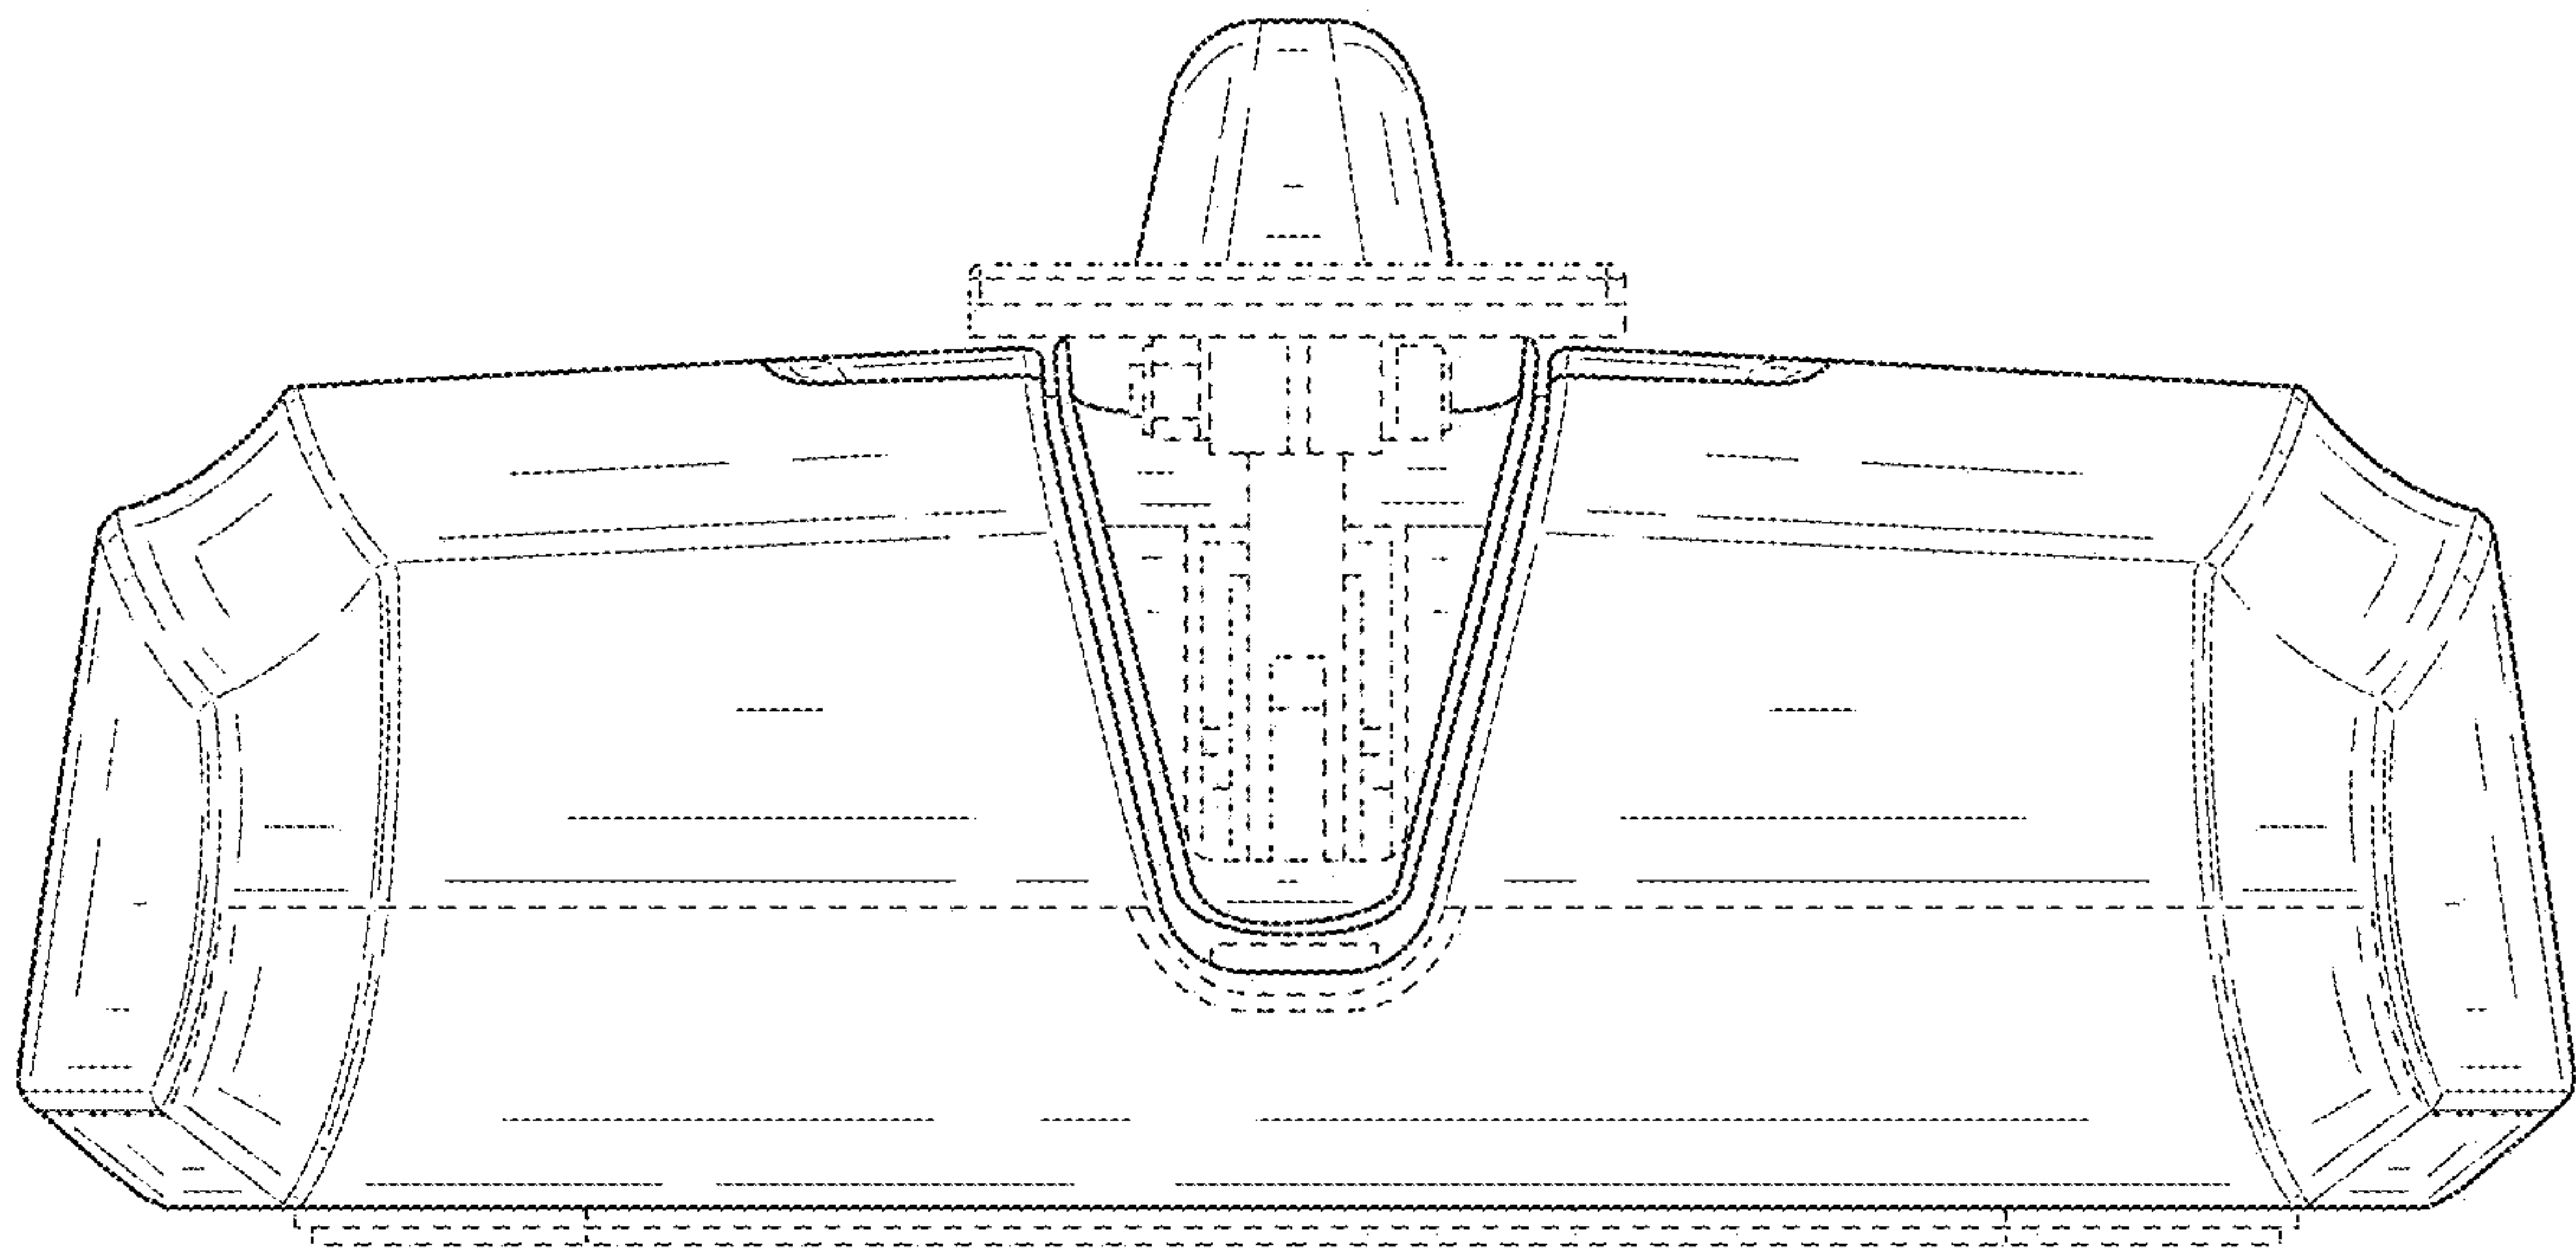


FIG. 11

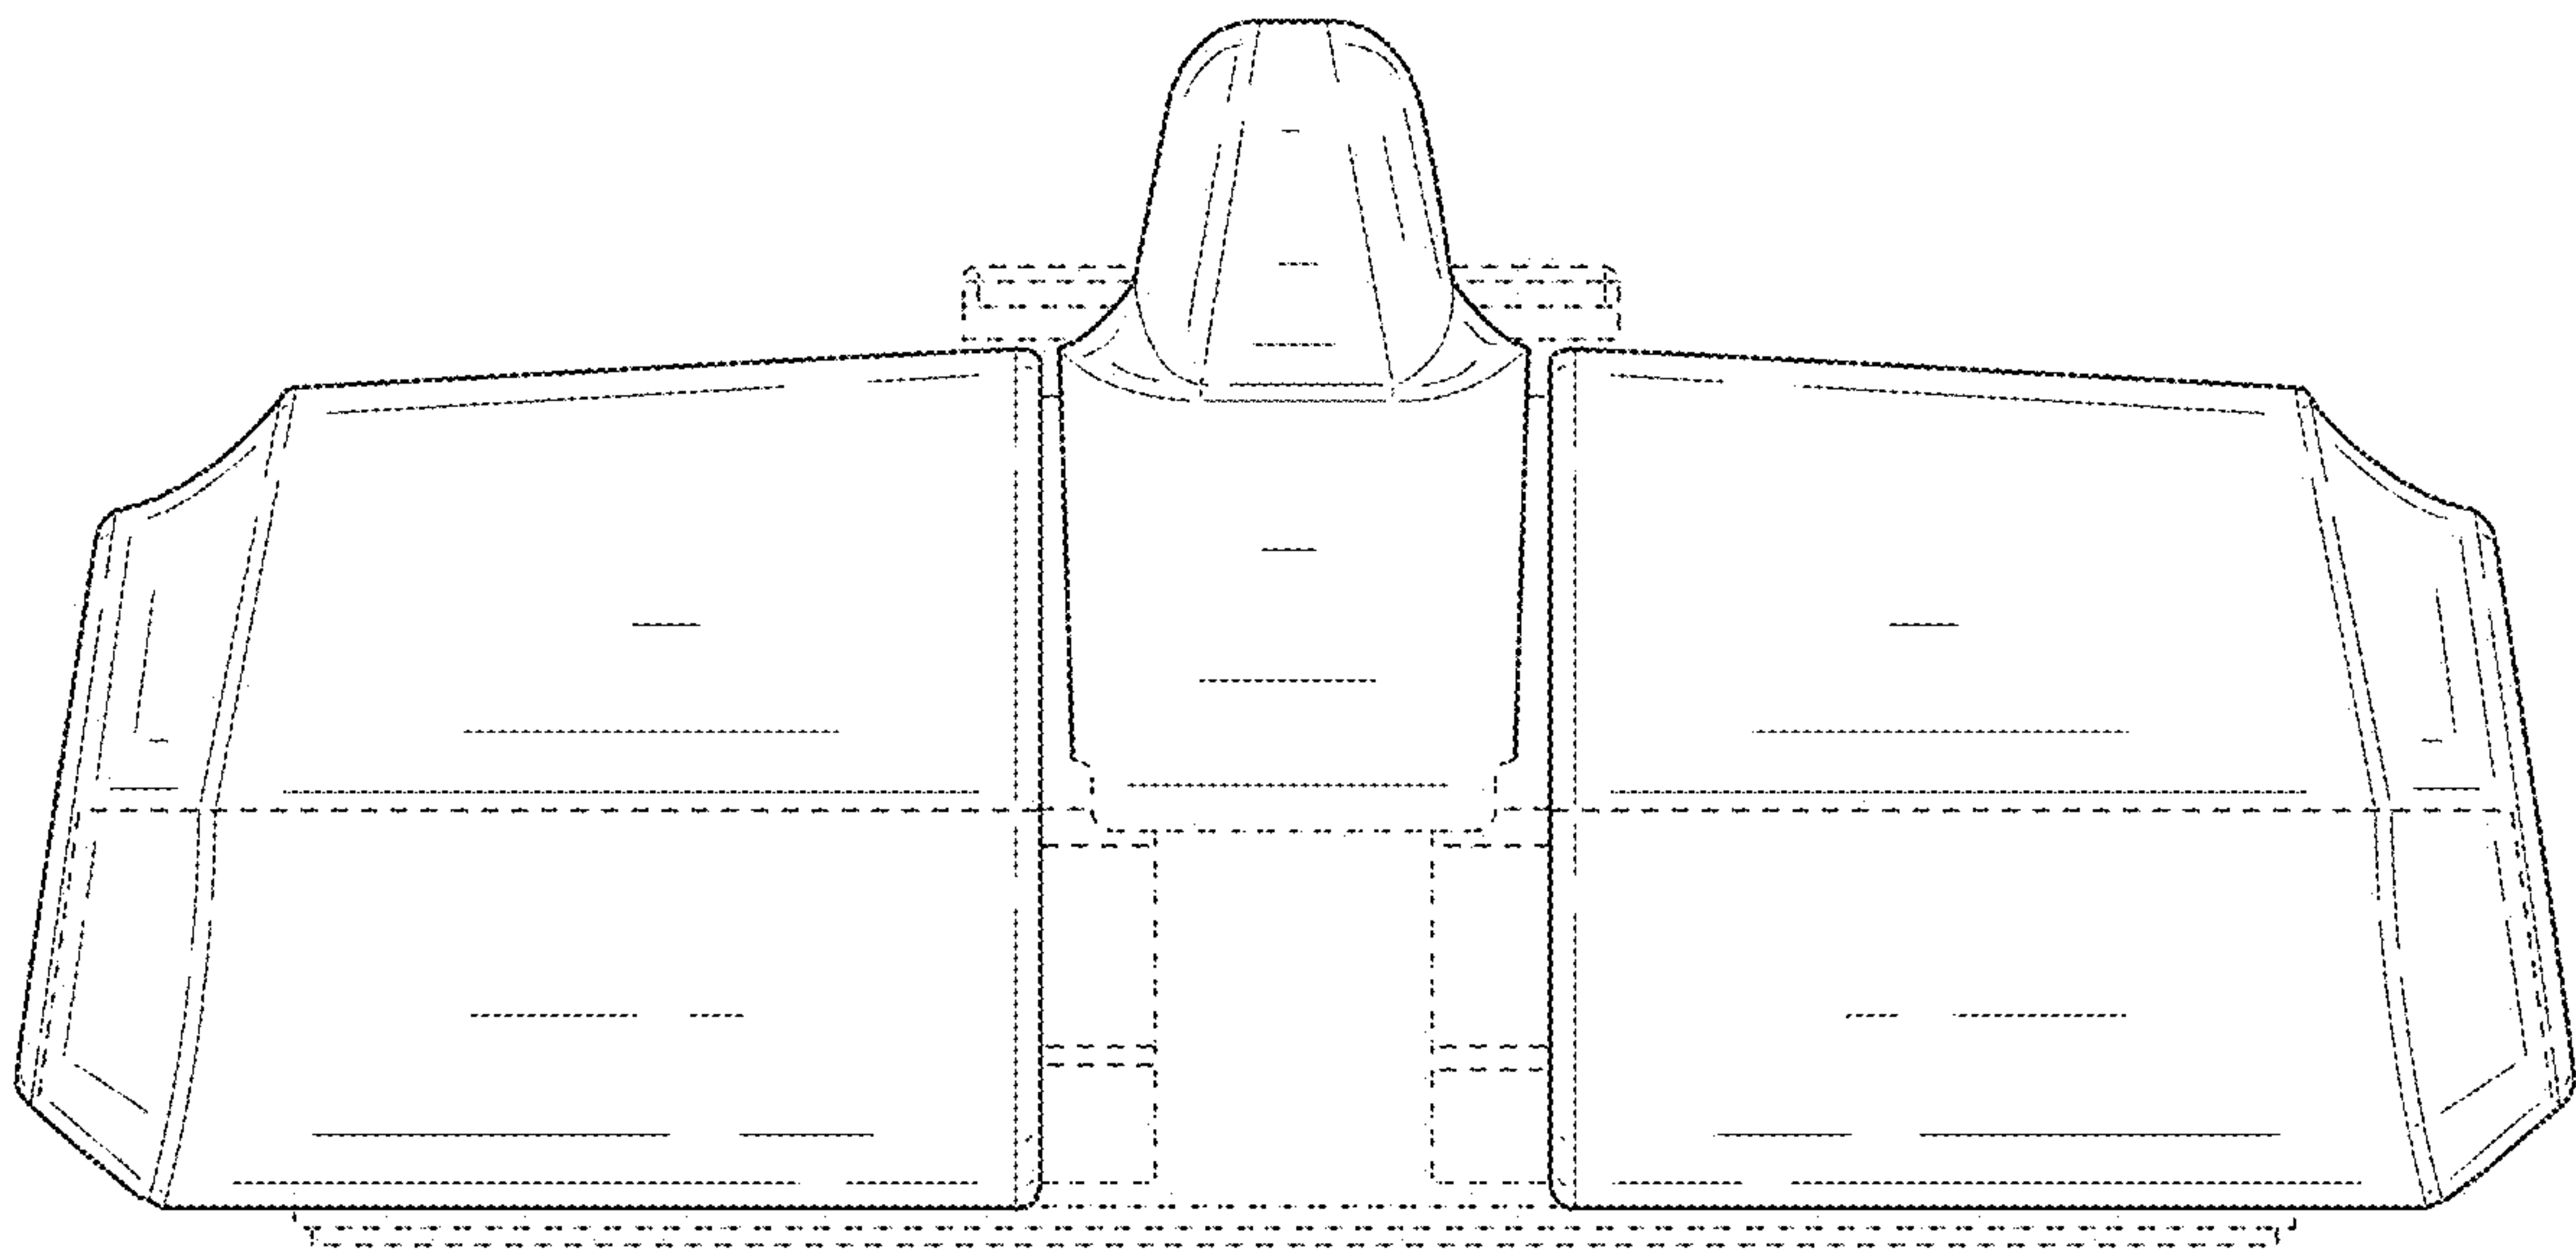


FIG. 12

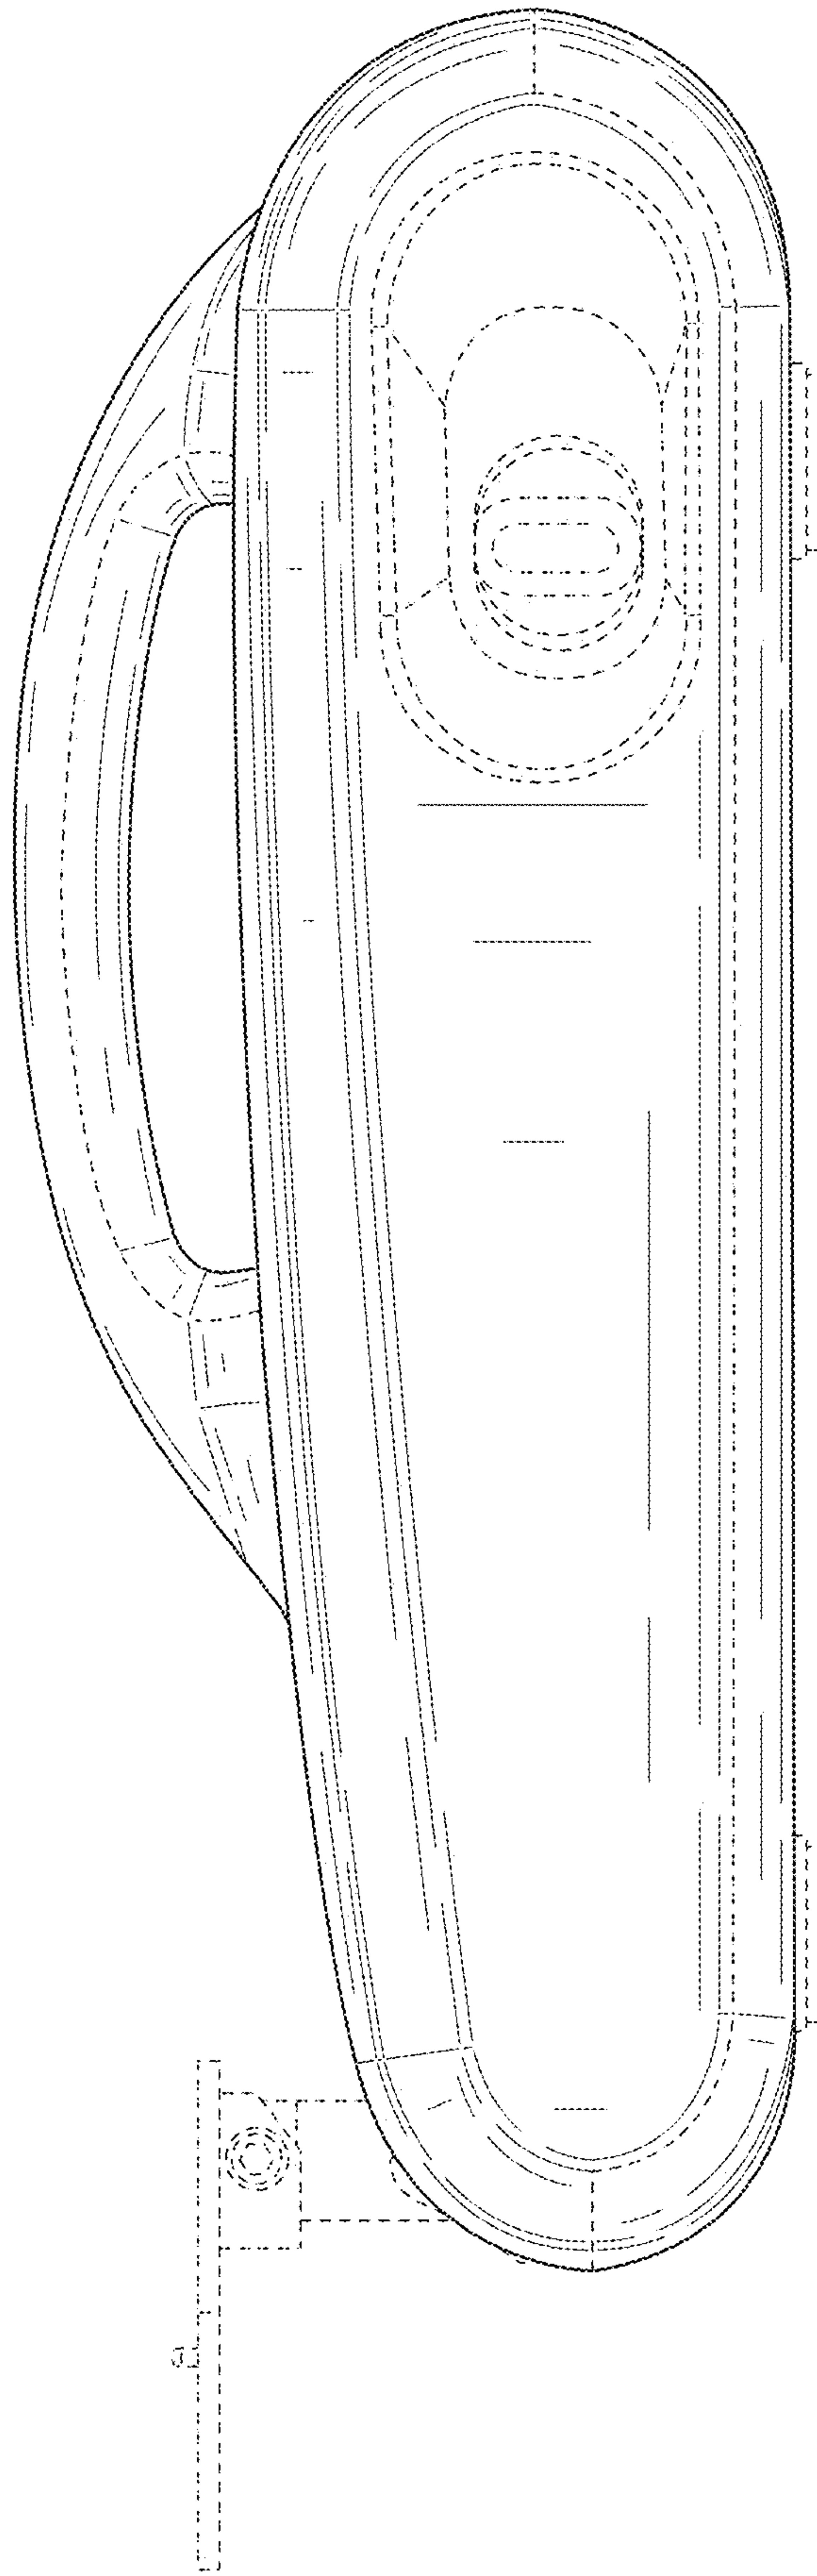


FIG. 13

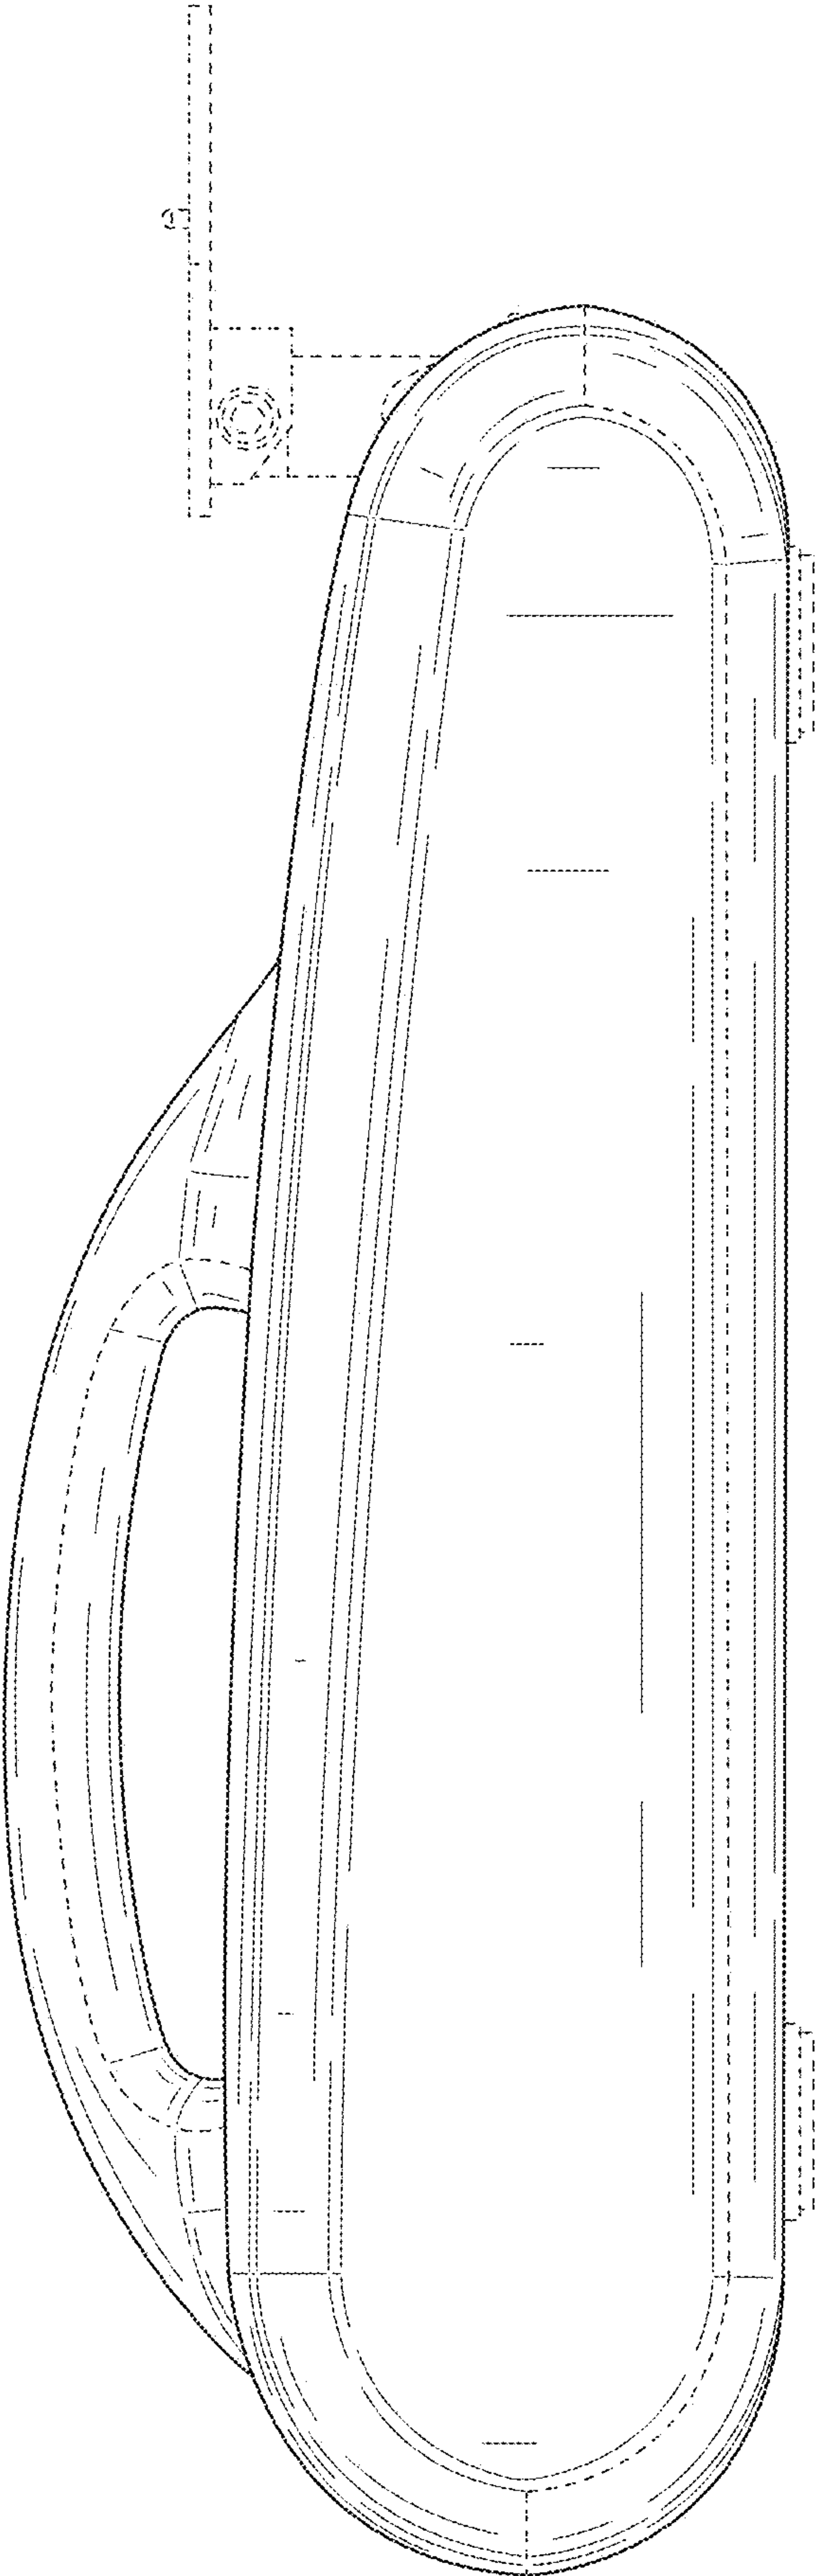


FIG. 14

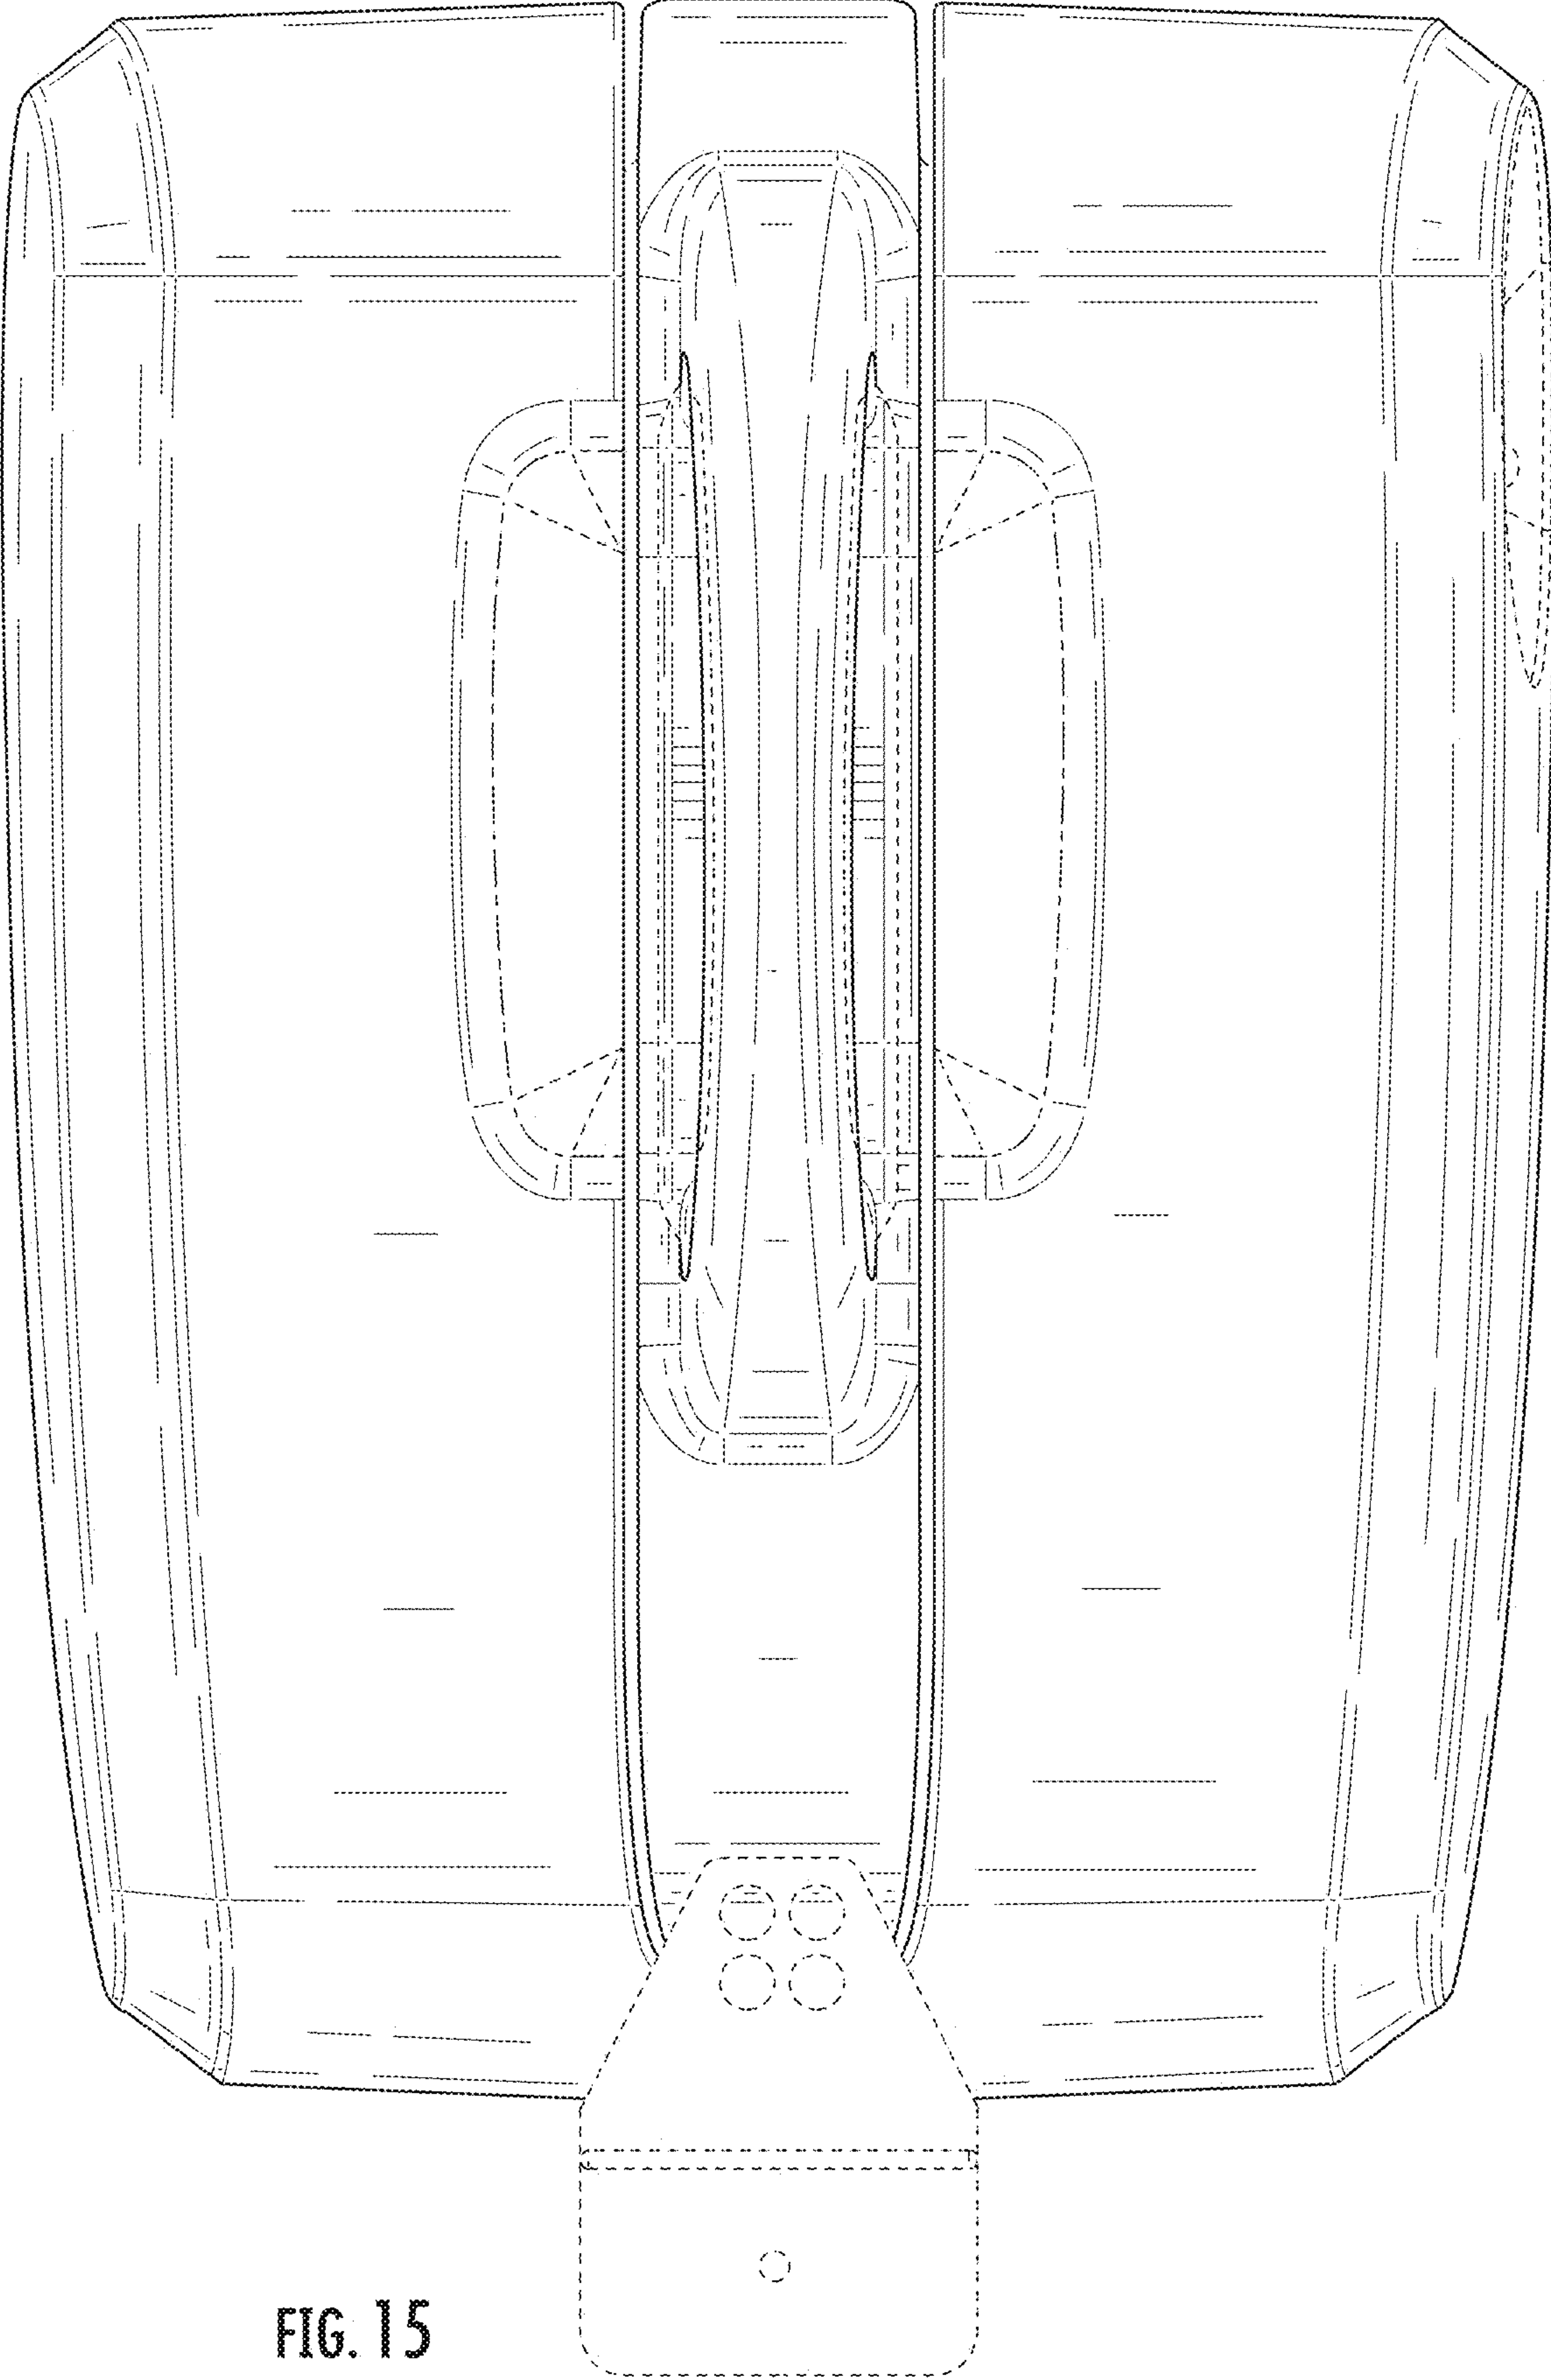


FIG. 15

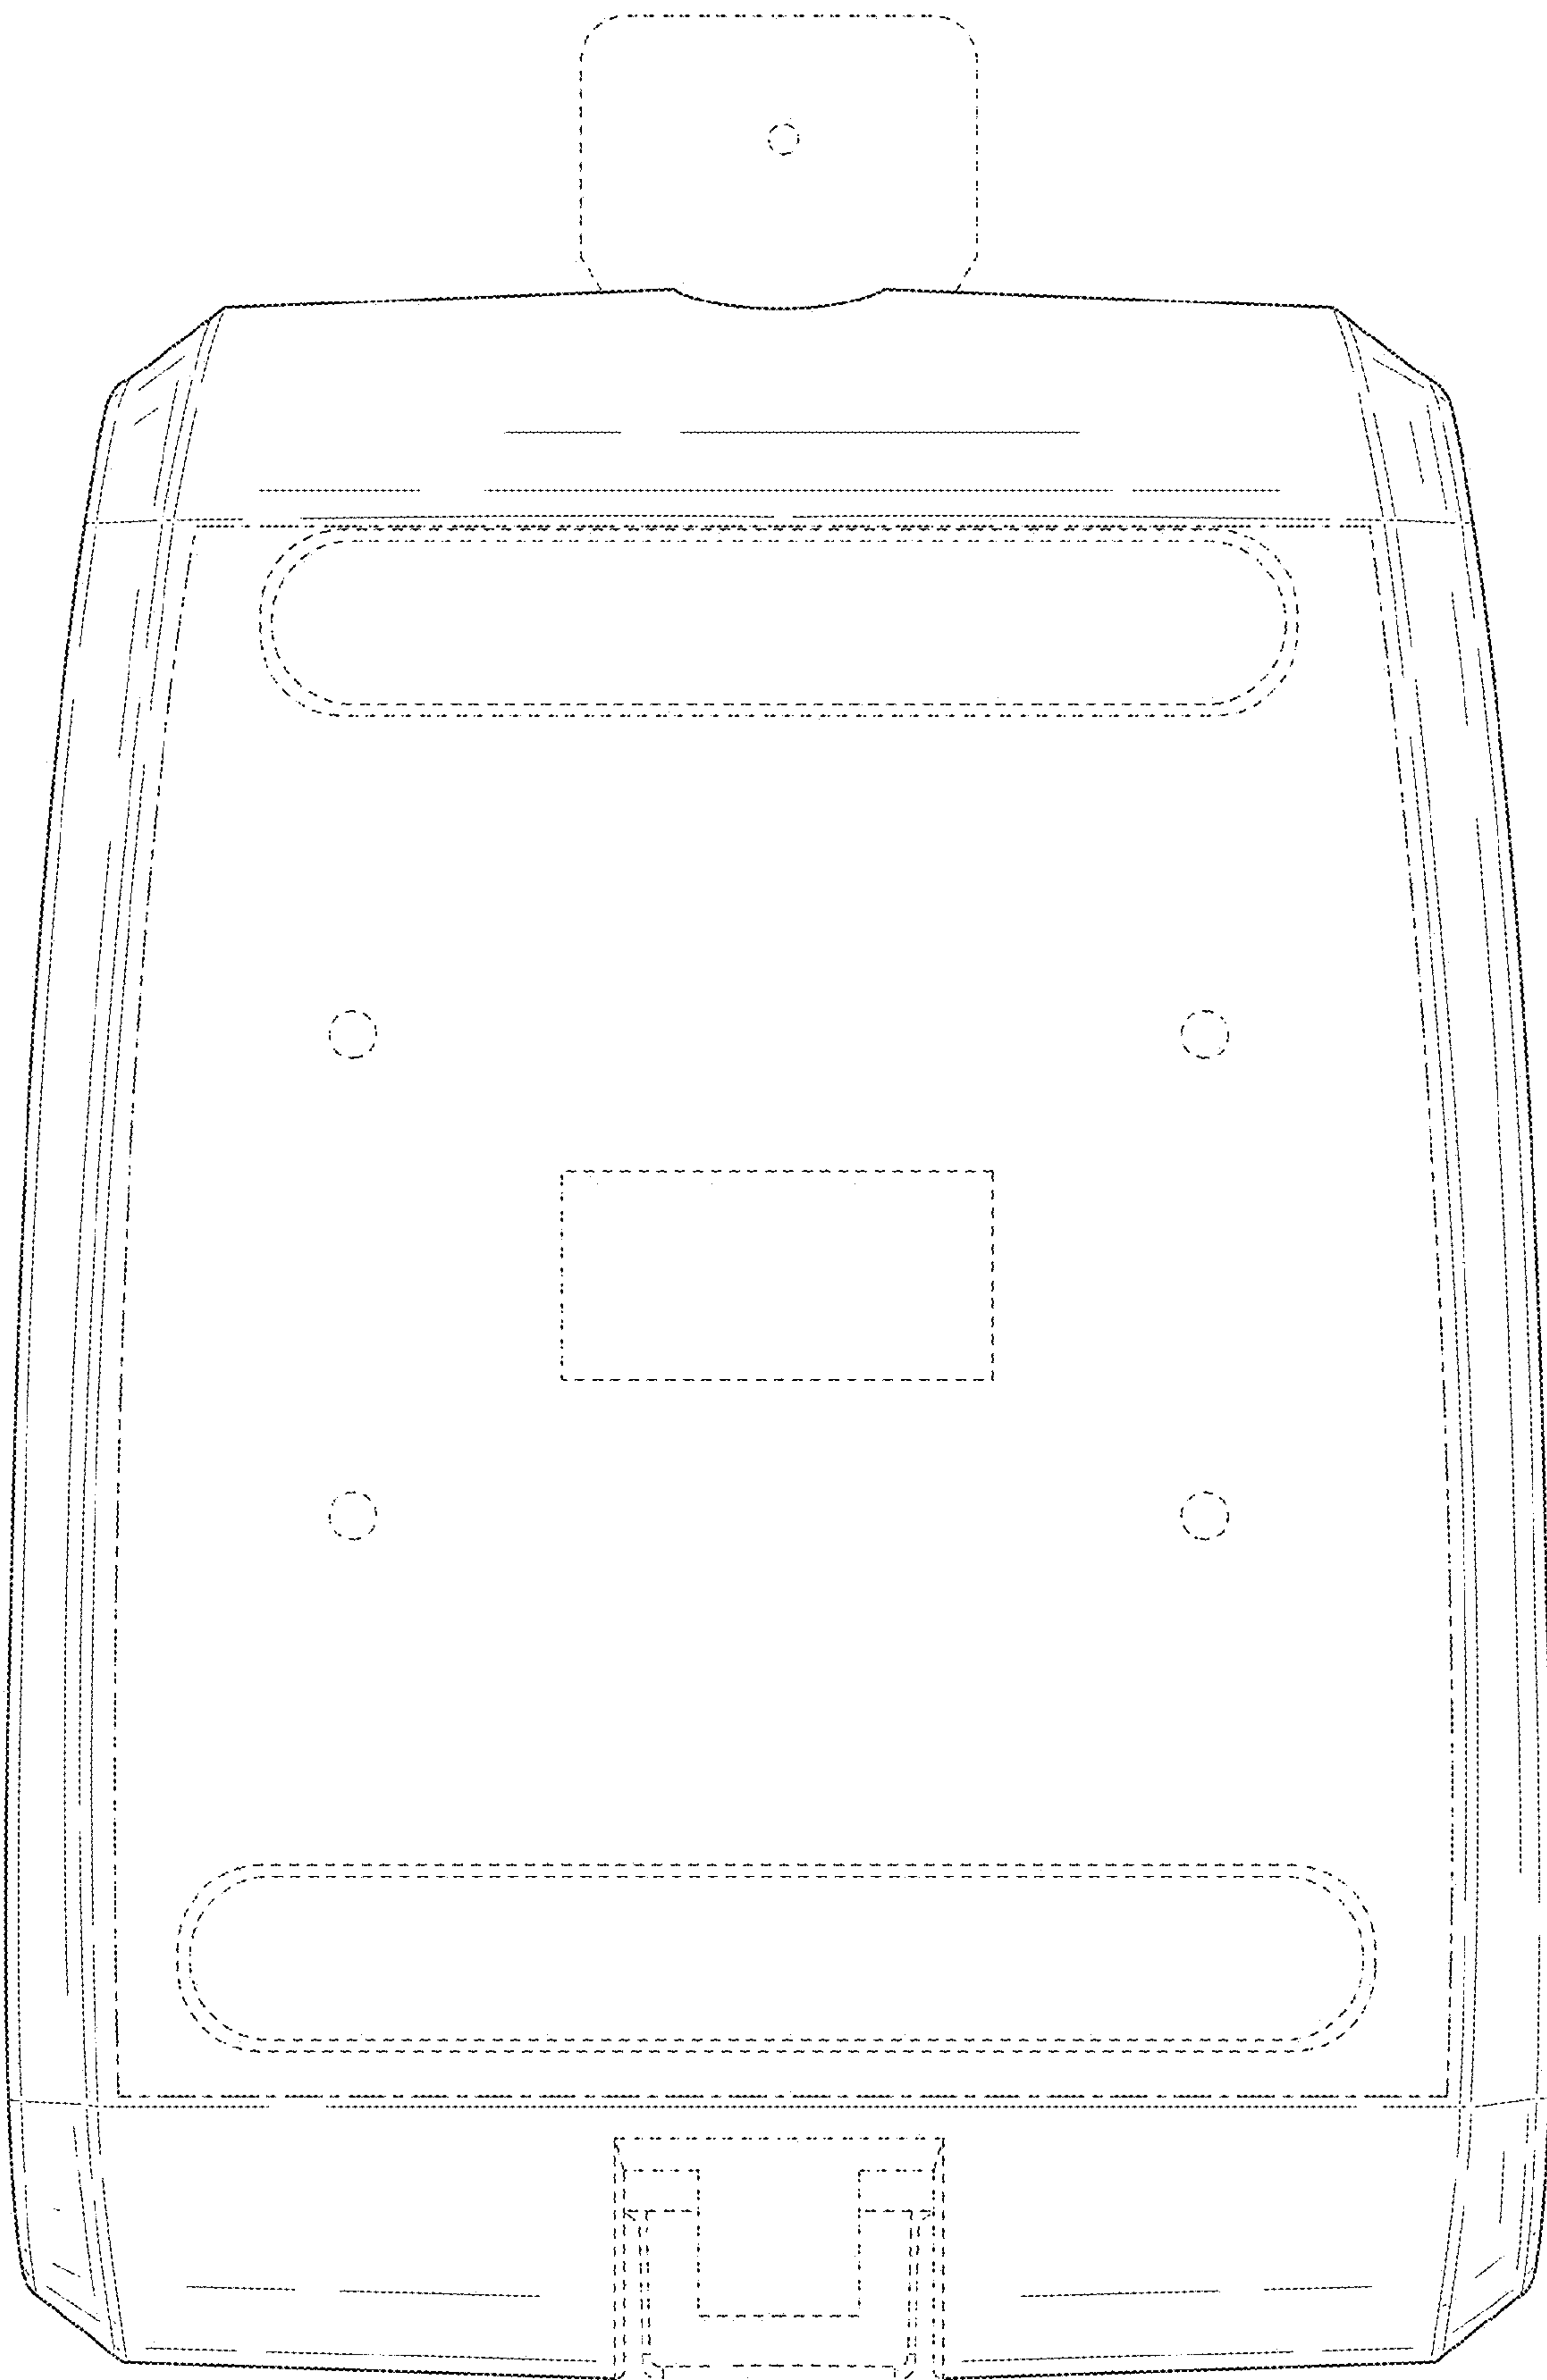


FIG. 16