

US00D946770S

(12) **United States Design Patent** (10) **Patent No.:** **US D946,770 S**
Theriot (45) **Date of Patent:** **** Mar. 22, 2022**

(54) **MEDICAL DEVICE**

(71) Applicant: **ManaMed Inc.**, Las Vegas, NV (US)

(72) Inventor: **Trevor James Theriot**, Flower Mound, TX (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/752,825**

(22) Filed: **Sep. 29, 2020**

(51) **LOC (13) Cl.** **24-04**

(52) **U.S. Cl.**

USPC **D24/190**

(58) **Field of Classification Search**

USPC D24/188, 190–192, 200, 206, 214, 215,
D24/171, 199, 212, 213; D2/970, 980,
D2/984–986, 989; D29/120.1, 121.2,
D29/121.1, 122, 100, 113, 114
CPC A61F 5/0111; A61F 5/0113; A61F 5/0127;
A61F 5/0585; A61F 5/0195; A61F
5/0123; A61F 5/0125; A61F 2005/0139;
A61F 2005/0176

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D546,955 S * 7/2007 Bauerfiend D24/190
D577,828 S * 9/2008 Ingimundarson D24/190
7,931,567 B2 * 4/2011 Rosenberg A61F 5/0195
482/57
D693,930 S * 11/2013 Manalo D24/190
8,945,035 B2 * 2/2015 Nace A61F 5/0123
602/23
D726,925 S * 4/2015 Fraser D24/190
D743,563 S * 11/2015 Wen D24/188
9,358,147 B1 * 6/2016 Ancinec A61F 5/0125
9,532,894 B2 * 1/2017 Gilbert F16D 65/065
D784,547 S * 4/2017 Kwon D24/190
9,622,900 B2 * 4/2017 Knecht A61F 5/0123
9,889,036 B2 * 2/2018 Chiang A61F 5/0123

9,918,864 B2 * 3/2018 Grant A61F 5/013
D819,212 S * 5/2018 Alexander A61F 5/0123
D24/171
9,980,843 B2 * 5/2018 Wang A61F 5/0102
9,987,151 B2 * 6/2018 Errico A61F 2/605
9,993,362 B2 * 6/2018 Costello A61F 5/0123
D835,289 S * 12/2018 Frost A61F 5/0125
D24/190

(Continued)

OTHER PUBLICATIONS

Orthomen Hip Abduction Brace, [site visited Dec. 1, 2021], Available from Internet. URL: <https://www.amazon.com/Orthomen-ROM-Post-Abduction-Brace/dp/B07LCCVRBY?th=1> (Year: 2021).*

Primary Examiner — T Chase Nelson

Assistant Examiner — Kelly L Gross

(74) *Attorney, Agent, or Firm* — Ted Masters

(57)


CLAIM

The ornamental design for a medical device, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of the medical device;
FIG. 2 is a top plan view of the medical device;
FIG. 3 is a bottom plan view of the medical device;
FIG. 4 is an end elevation view of the medical device;
FIG. 5 is an opposite end elevation view of the medical device;
FIG. 6 is a side elevation view of the medical device;
FIG. 7 is an opposite side elevation view of the medical device;
FIG. 8 is a top plan view of the medical device in an alternate position; and,
FIG. 9 is an opposite side elevation view of the medical device in an alternate position.
The broken lines in the drawings show portions of the medical device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

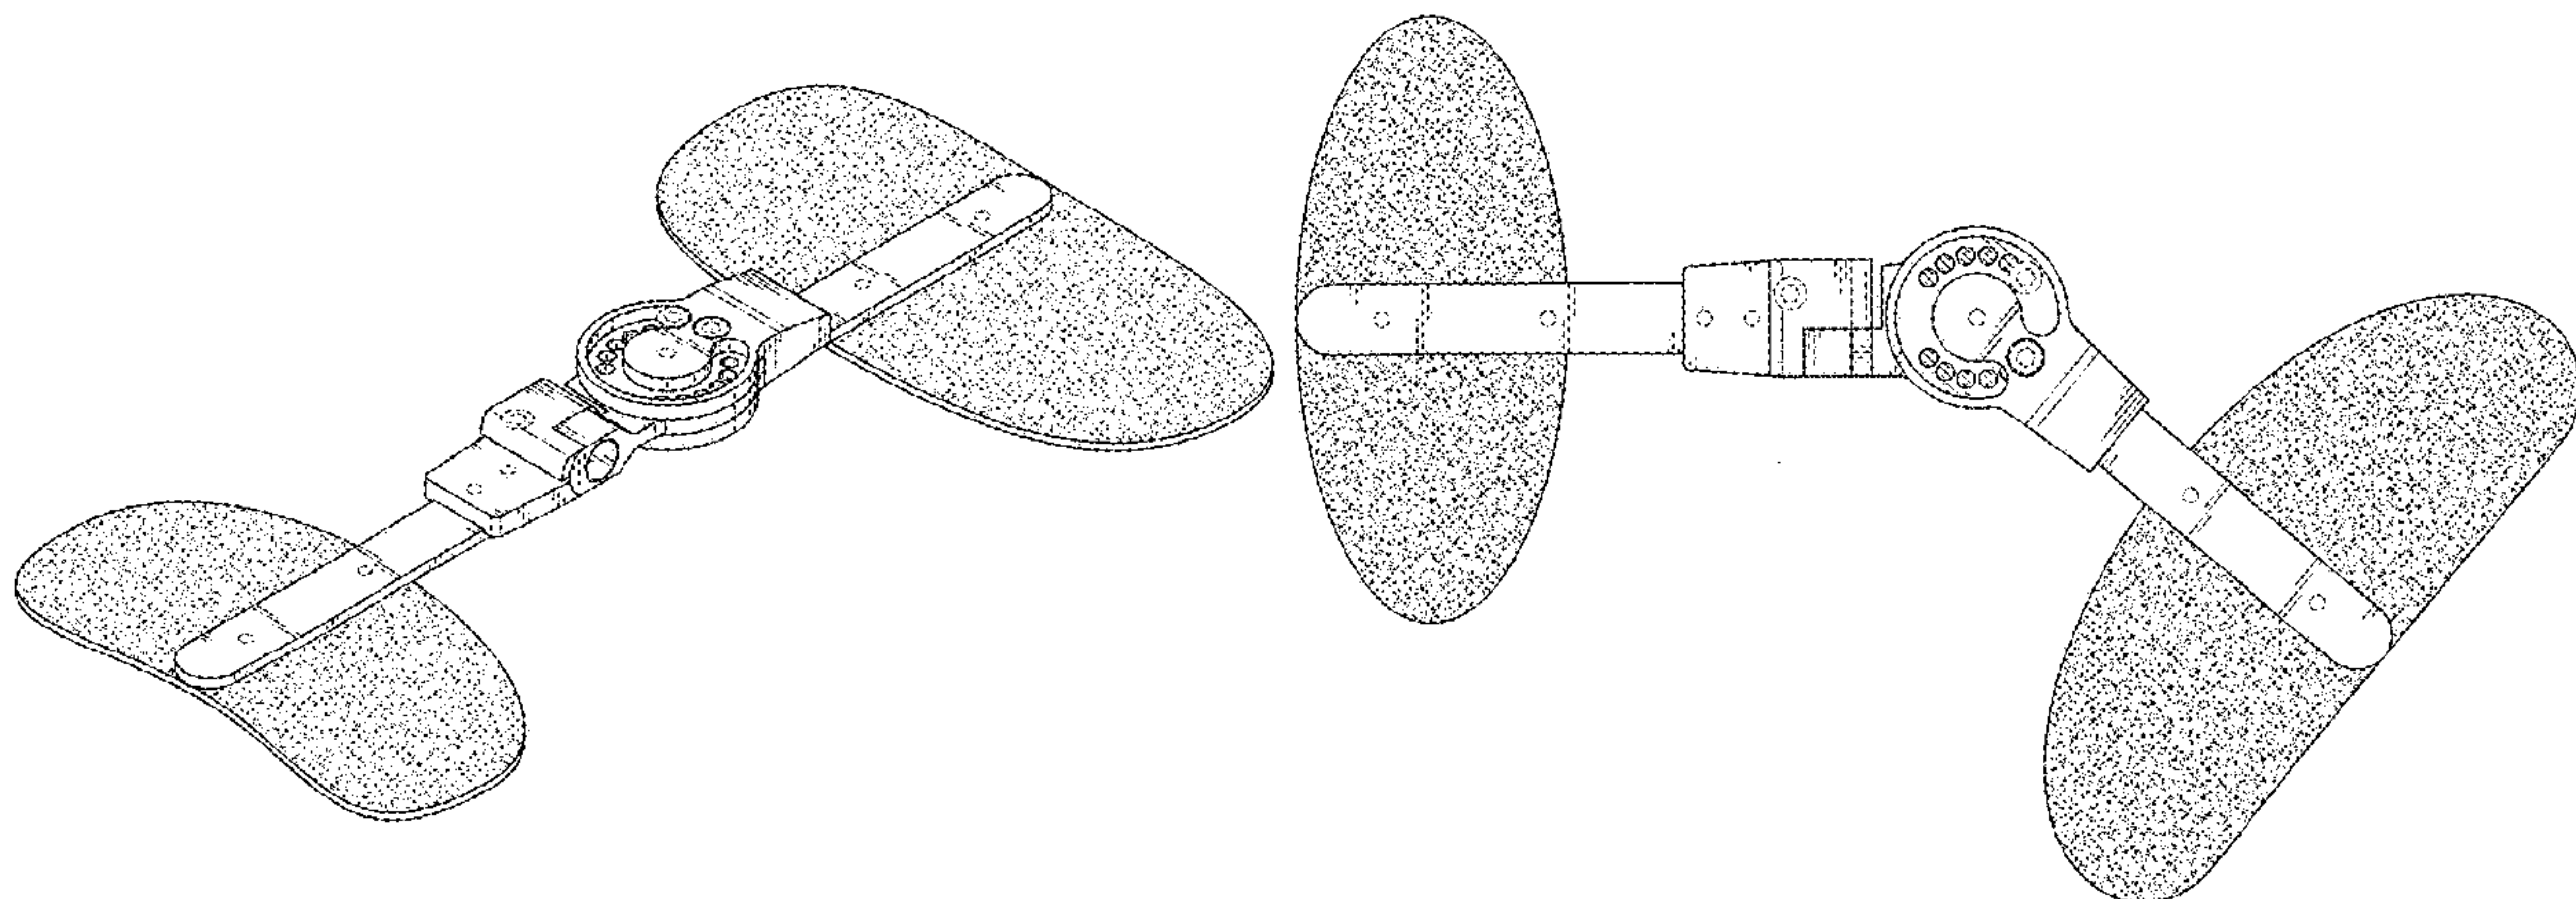

(56)

References Cited

U.S. PATENT DOCUMENTS

D846,130	S *	4/2019	Watabe	F16D 65/065 D24/190
D849,253	S *	5/2019	Siddiqui	D24/190
10,434,003	B2 *	10/2019	Robinson	A61F 5/30
10,617,549	B2 *	4/2020	Frost	A61F 5/0123
D888,257	S *	6/2020	Larouche	D24/190
10,736,765	B1 *	8/2020	Lahiff	A61F 5/0125
D898,204	S *	10/2020	Siddiqui	A61F 5/0123 D24/192
10,973,670	B2 *	4/2021	Wu	A63B 21/4011
D933,237	S *	10/2021	Sigurdsson	D24/171
2014/0276304	A1 *	9/2014	Dollar	A61F 5/0102 602/16
2014/0308065	A1 *	10/2014	DeHarde	A61F 5/013 403/113
2017/0298981	A1 *	10/2017	Sgeirsson	A61F 5/028
2020/0030179	A1 *	1/2020	Schwenn	A61F 5/0102

* cited by examiner

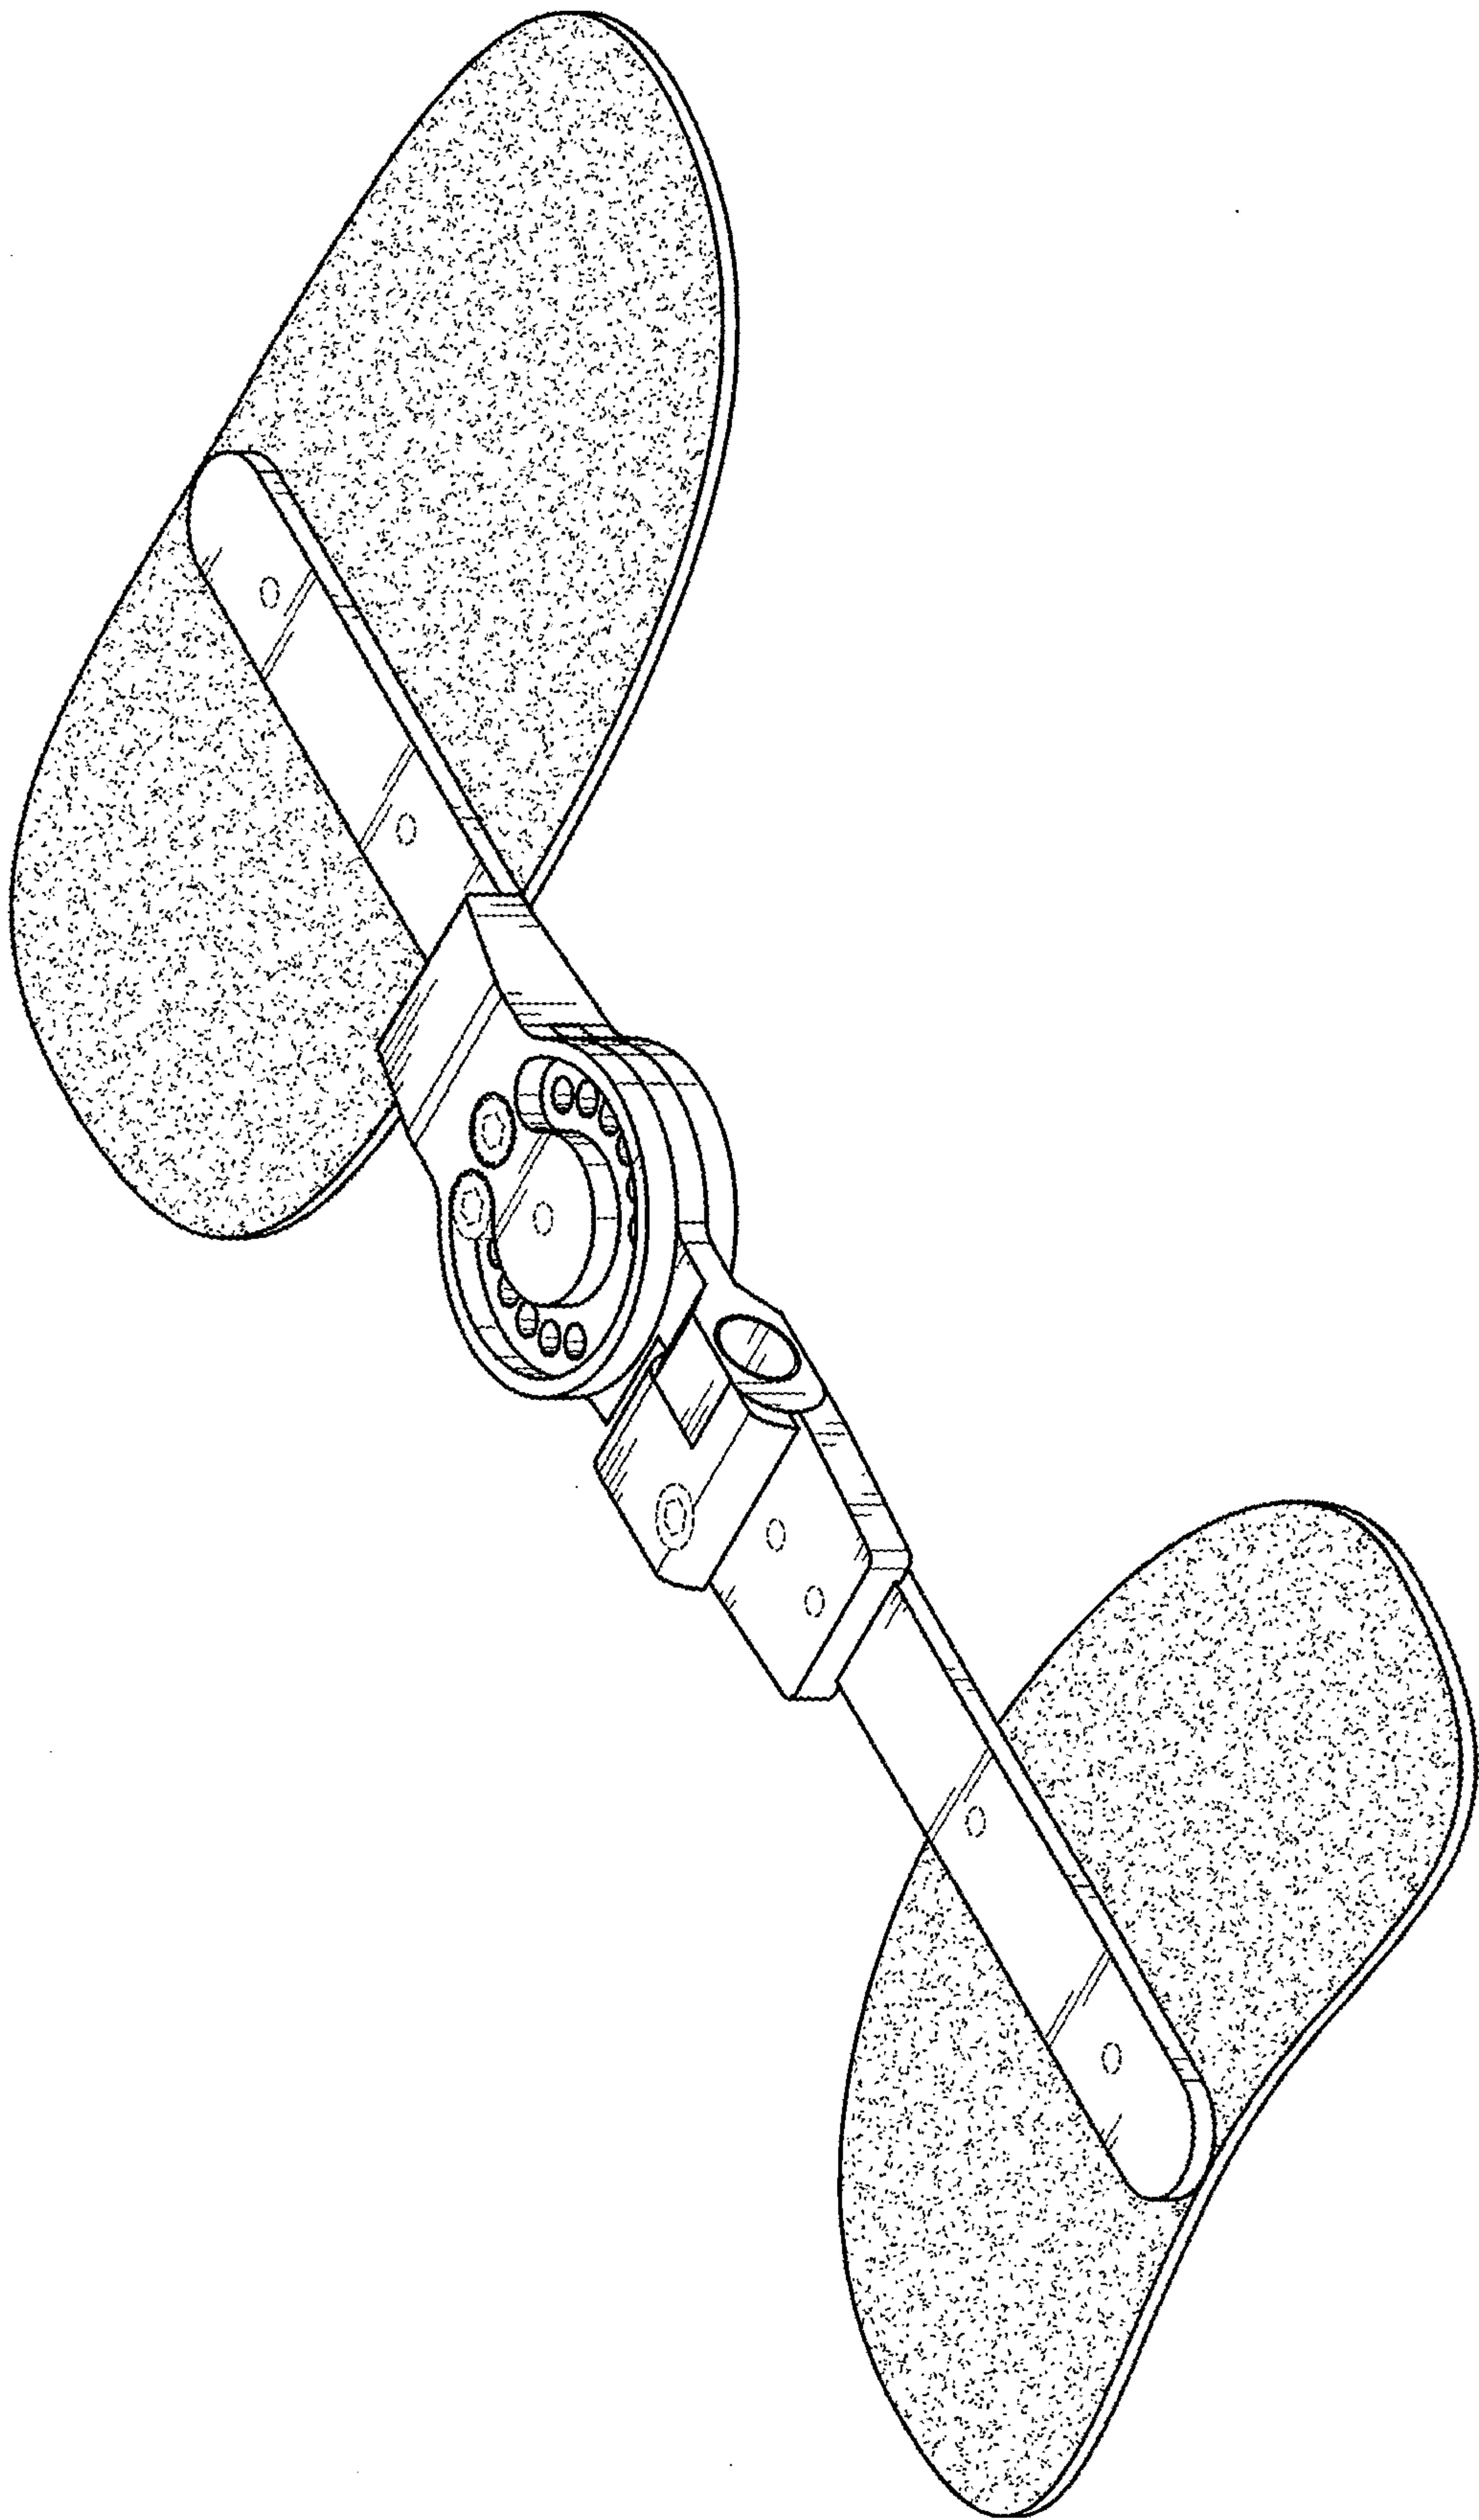


FIG. 1

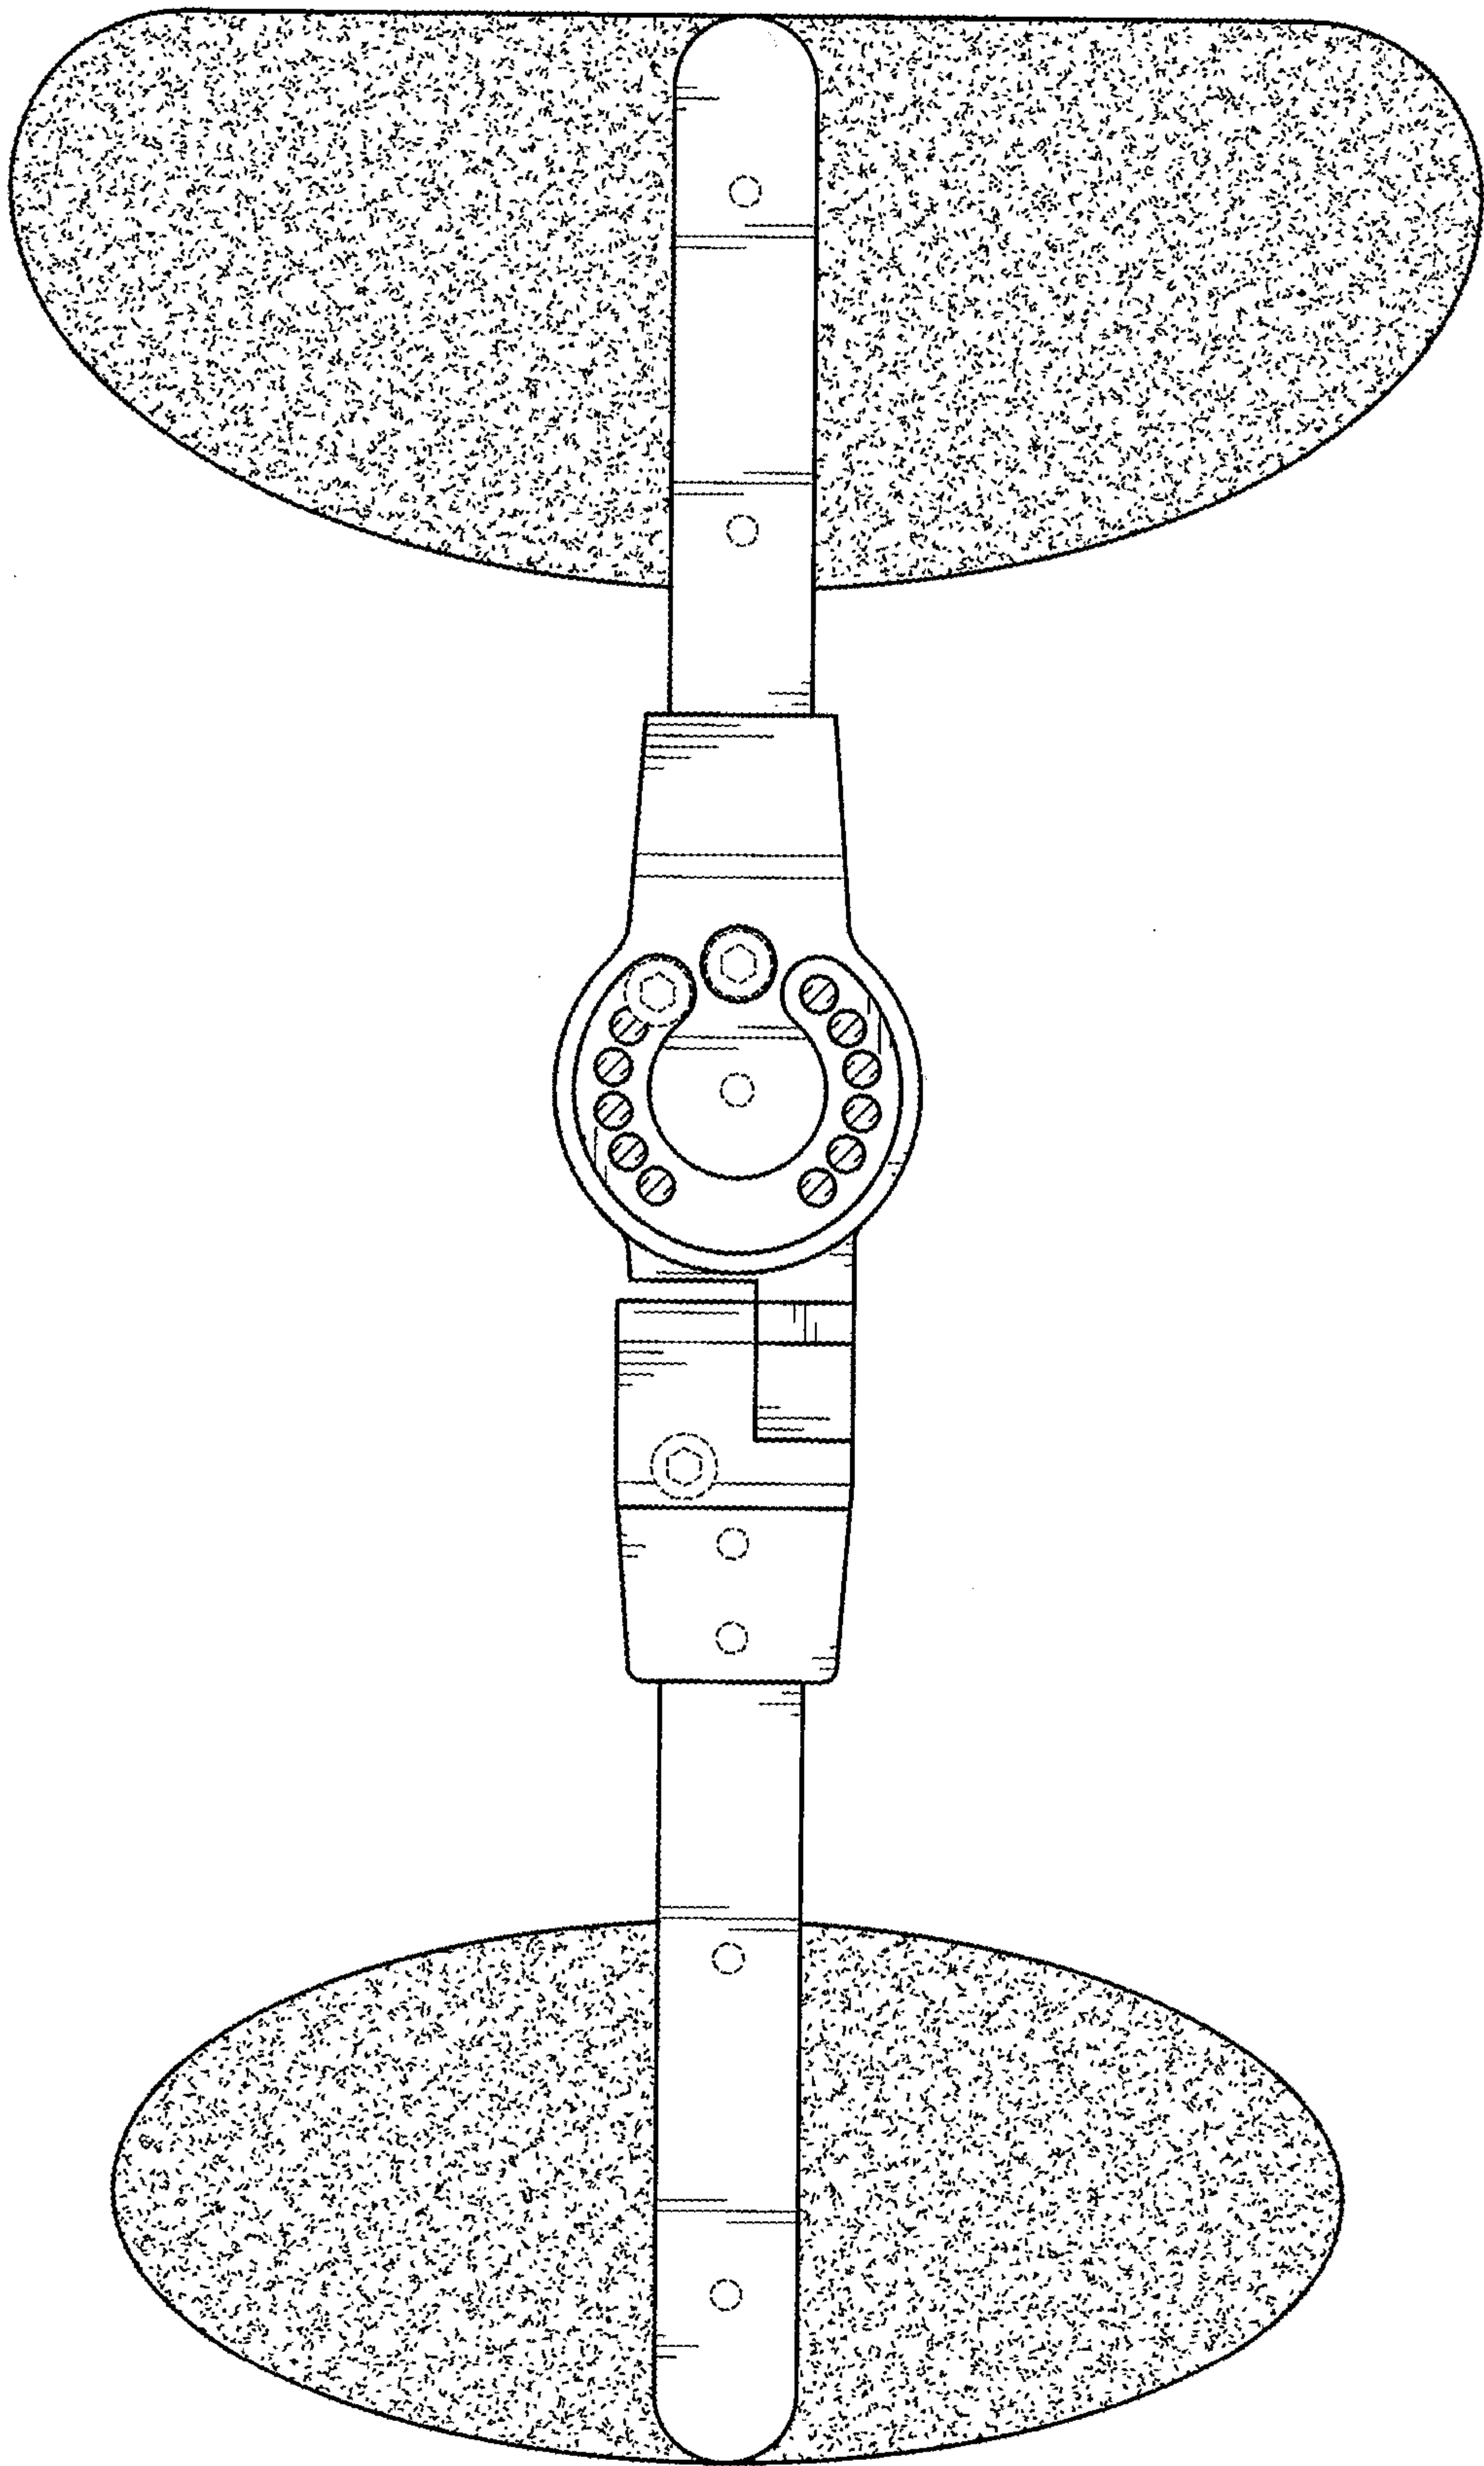


FIG. 2

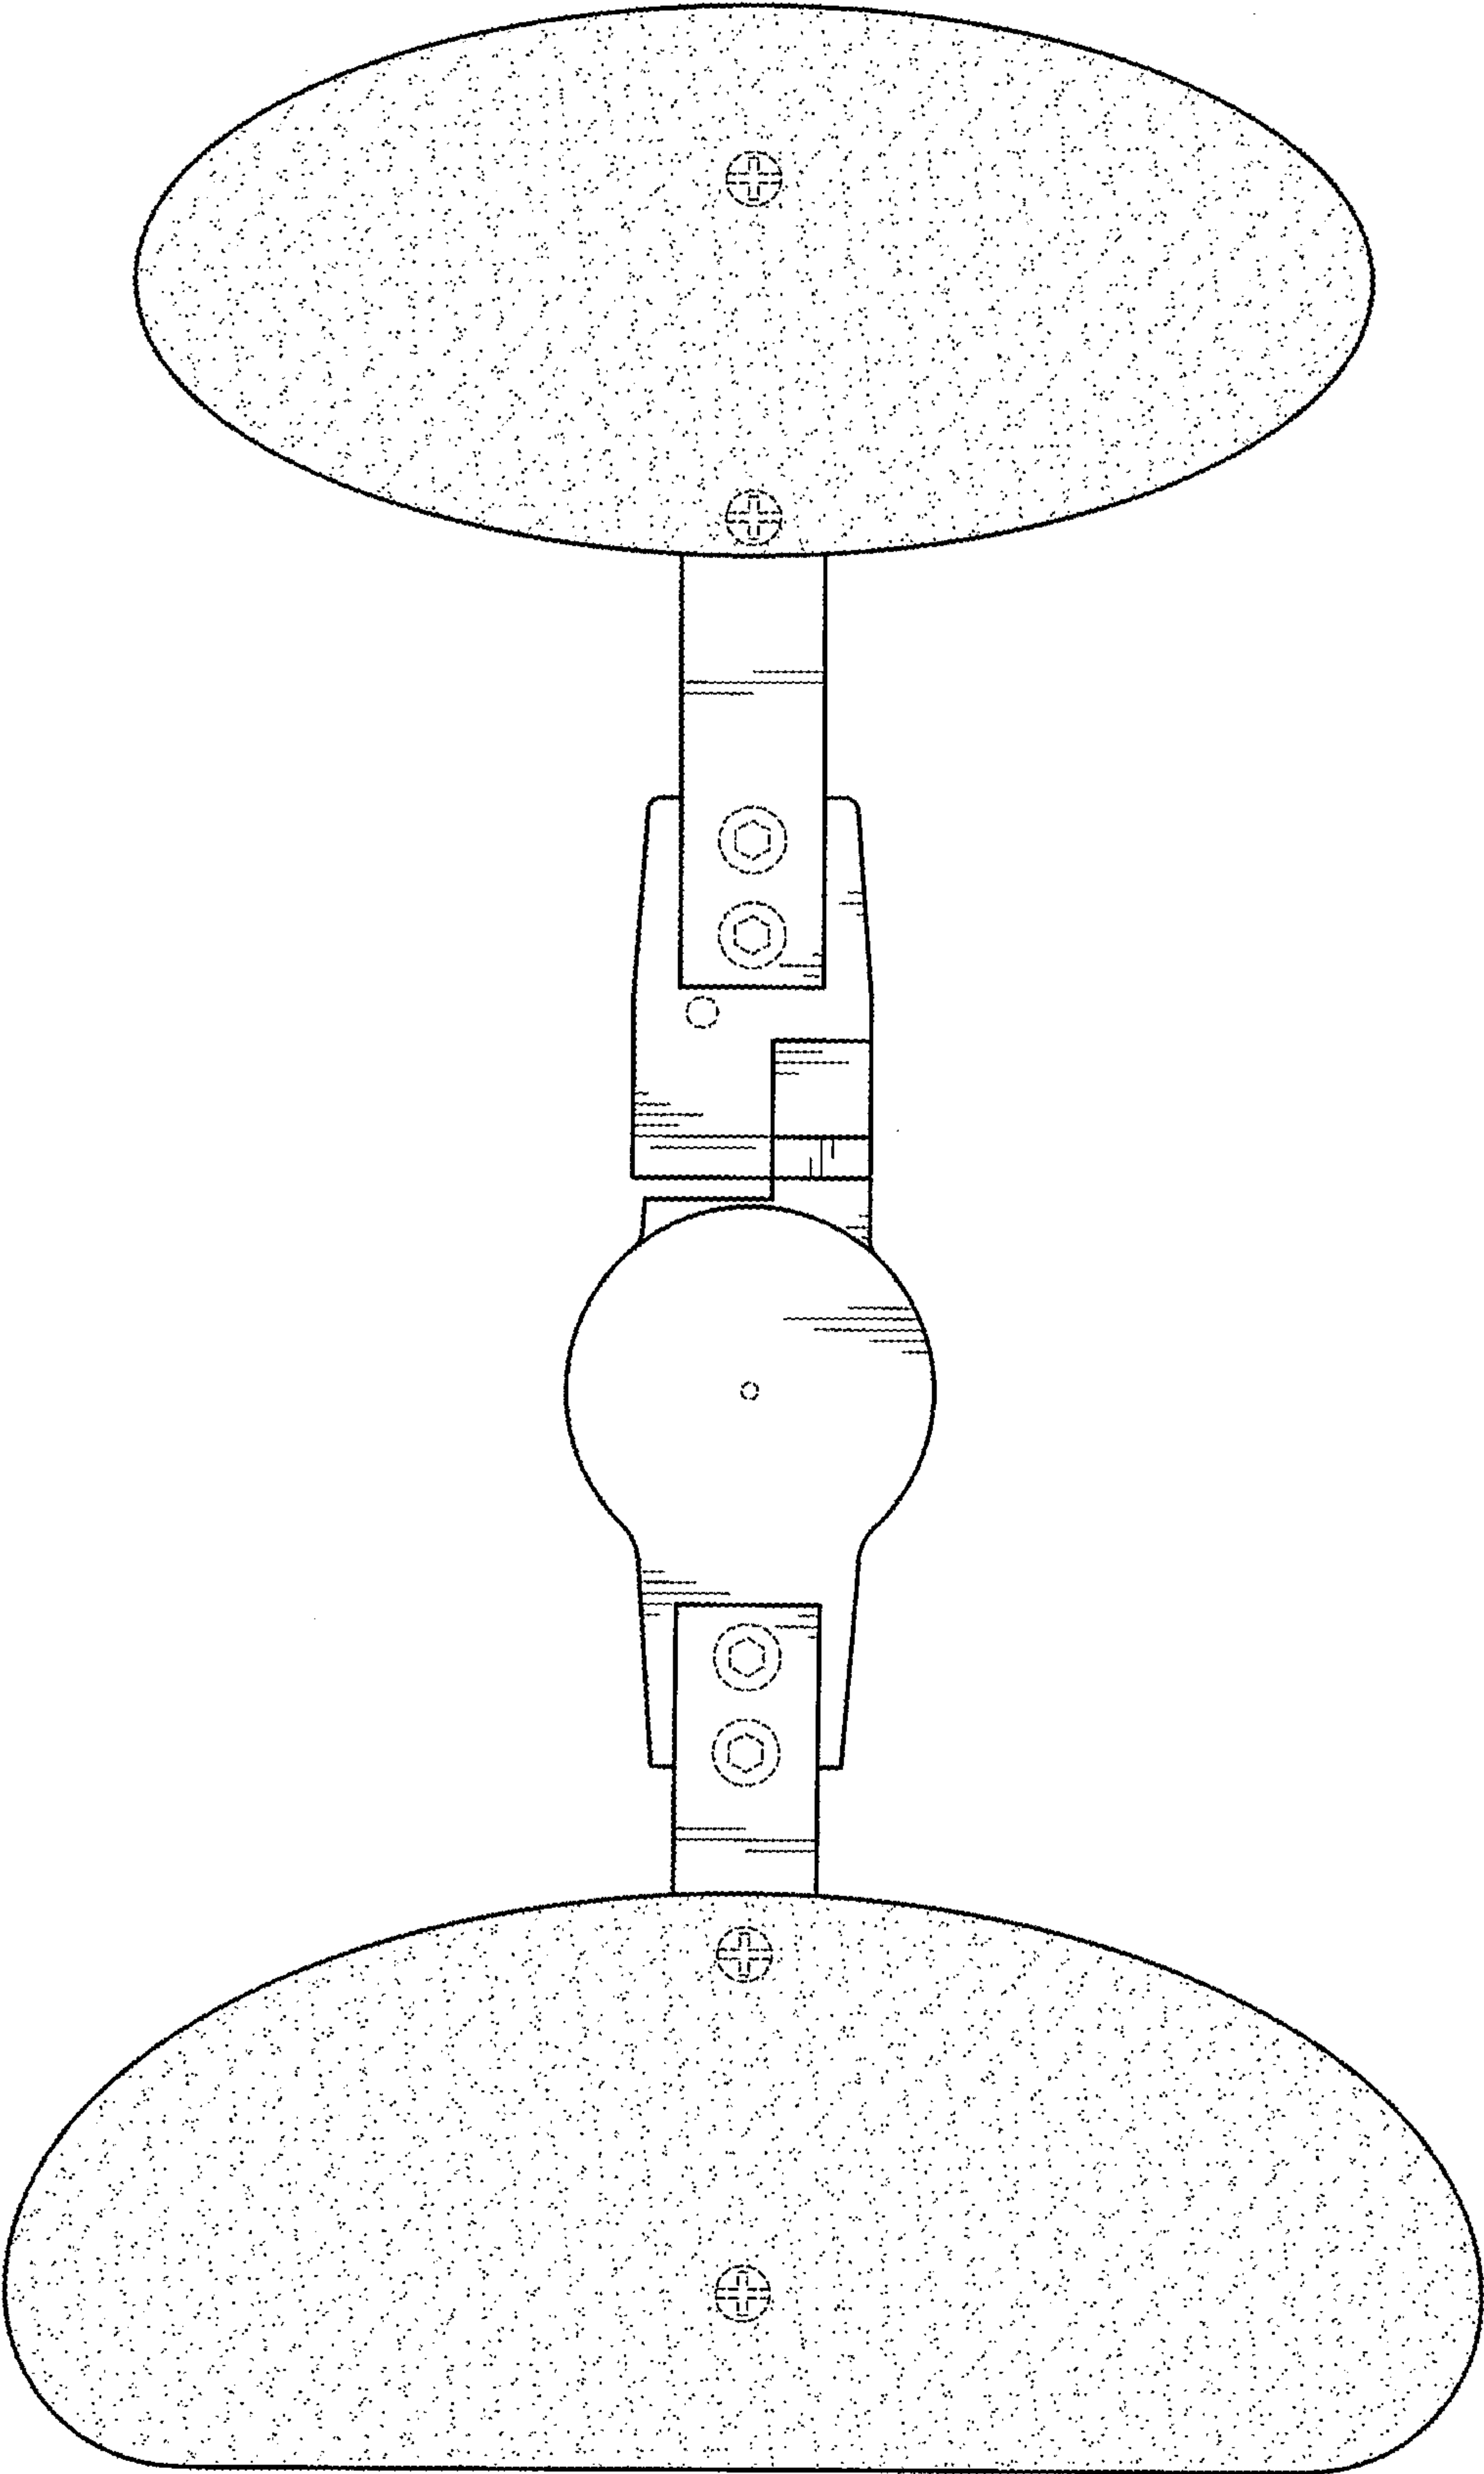


FIG. 3

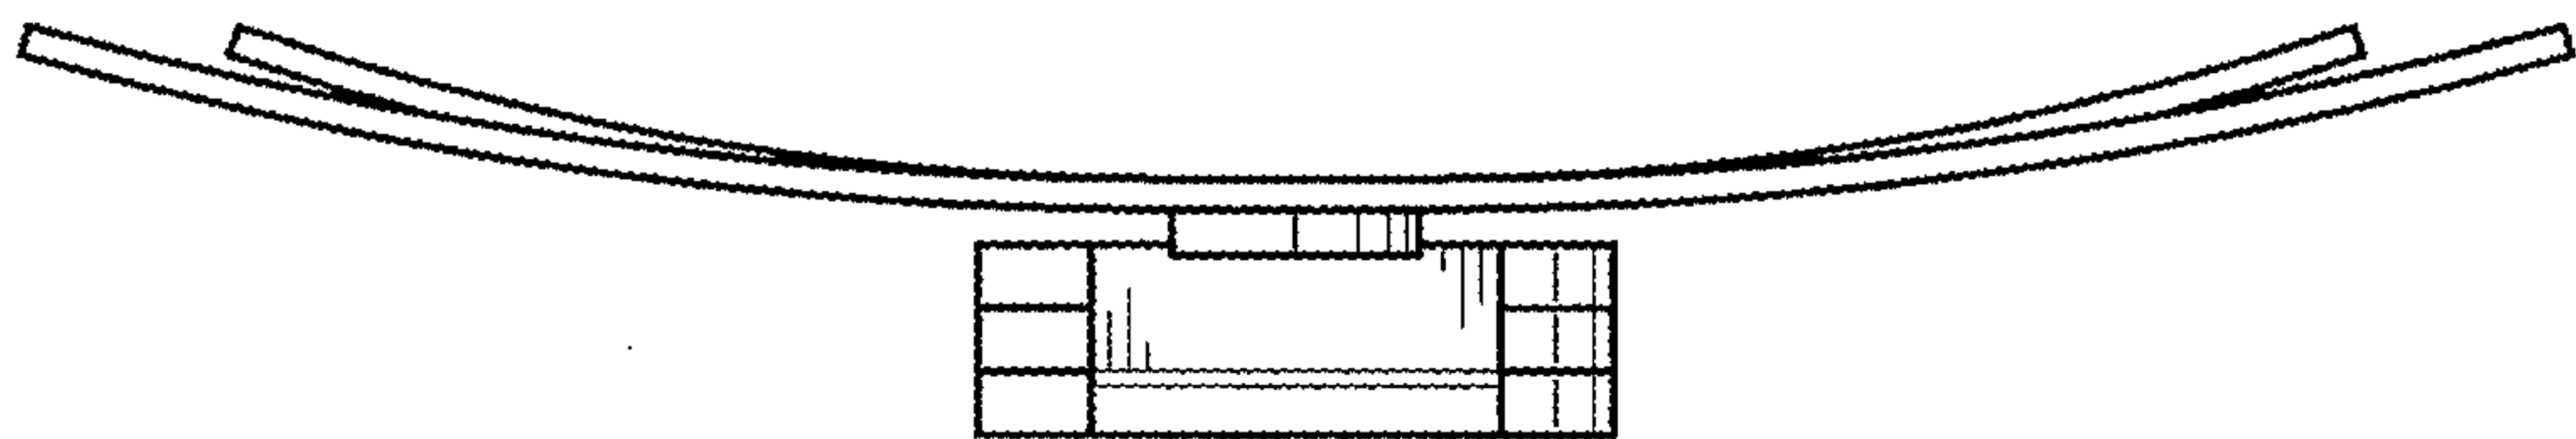


FIG. 4

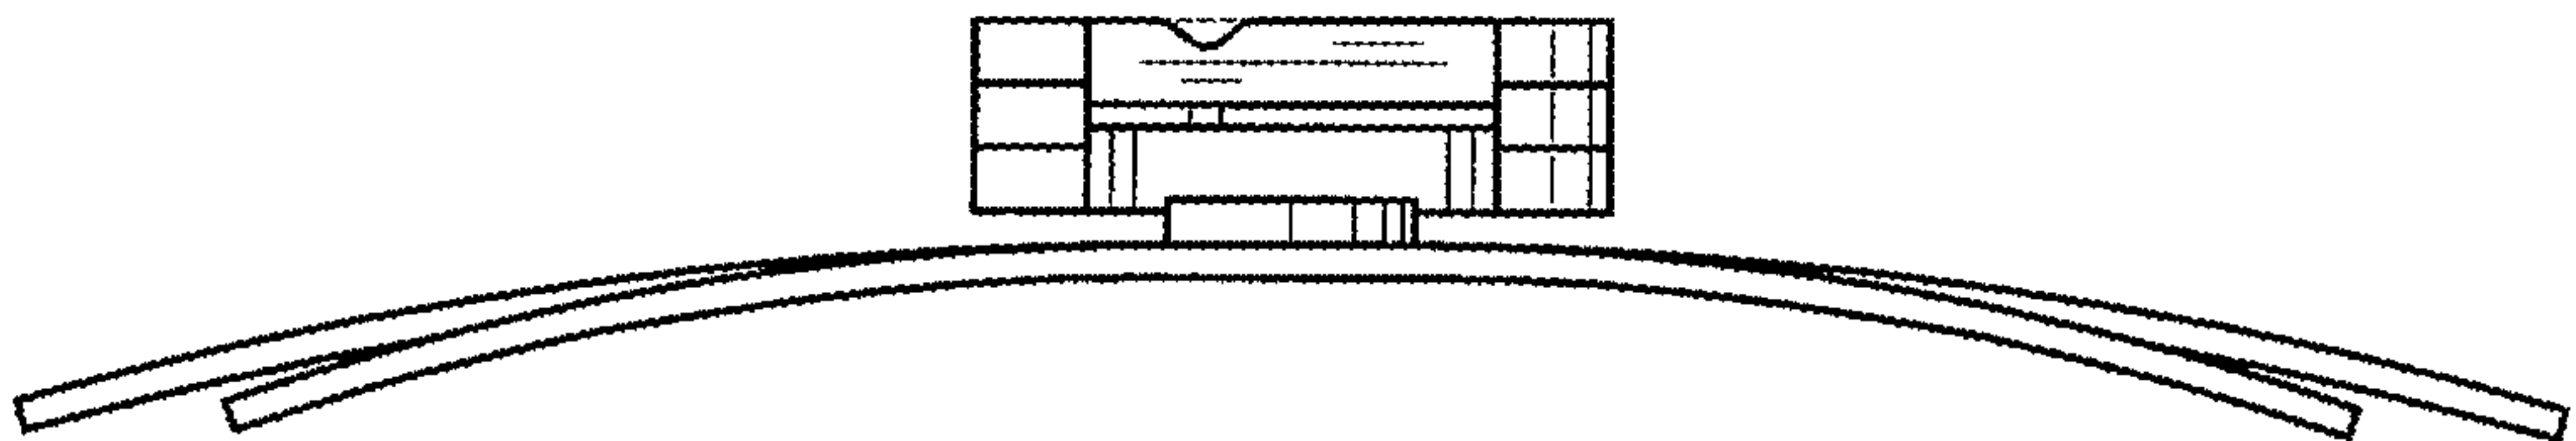


FIG. 5

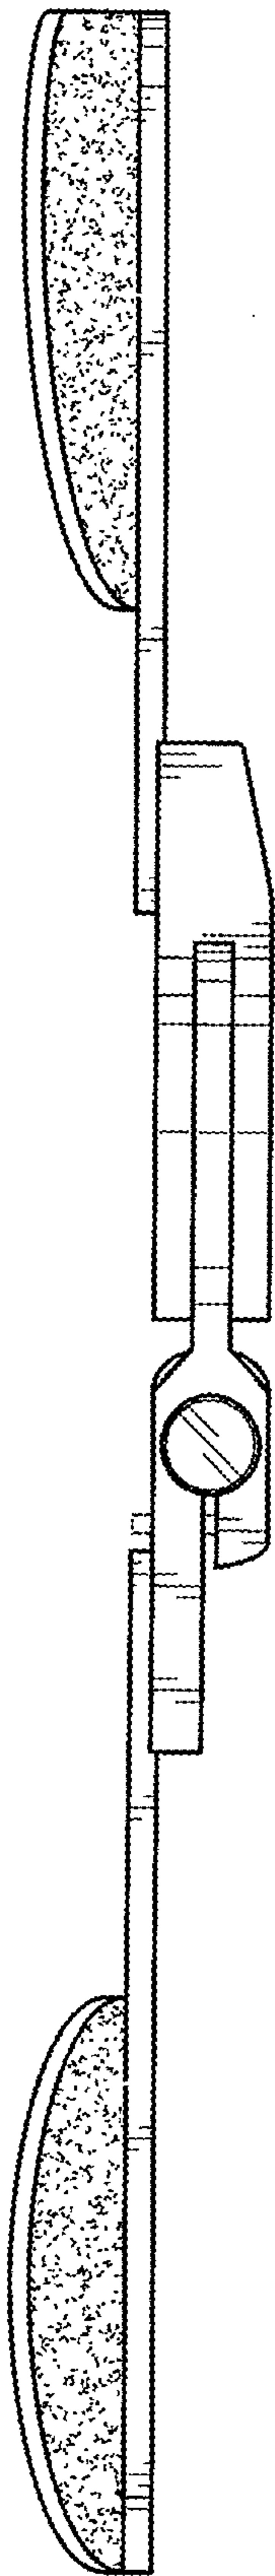


FIG. 6

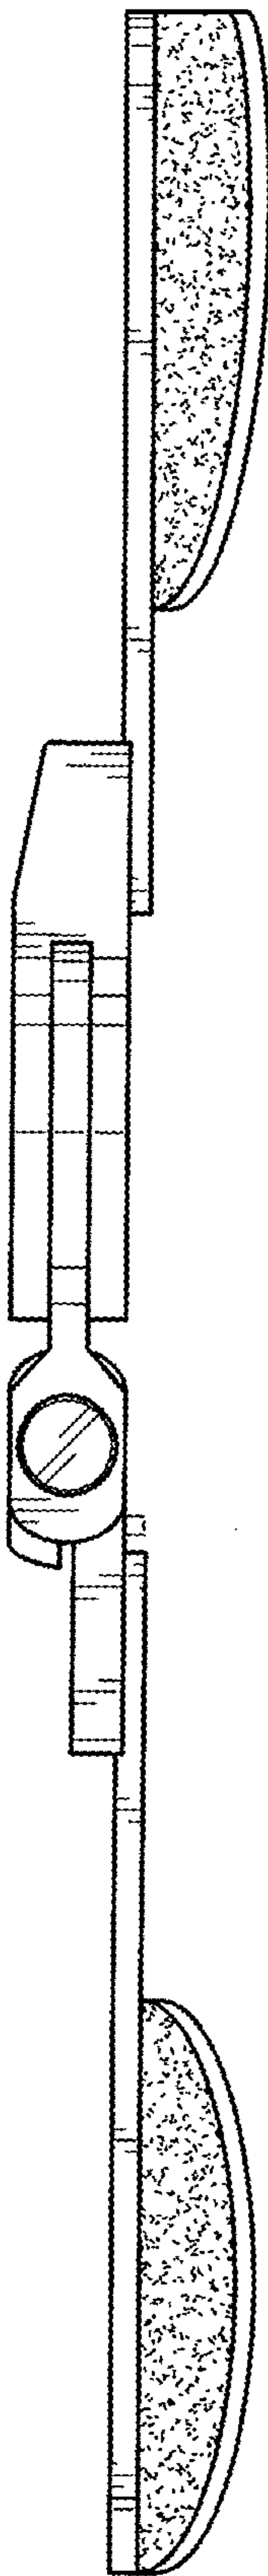


FIG. 7

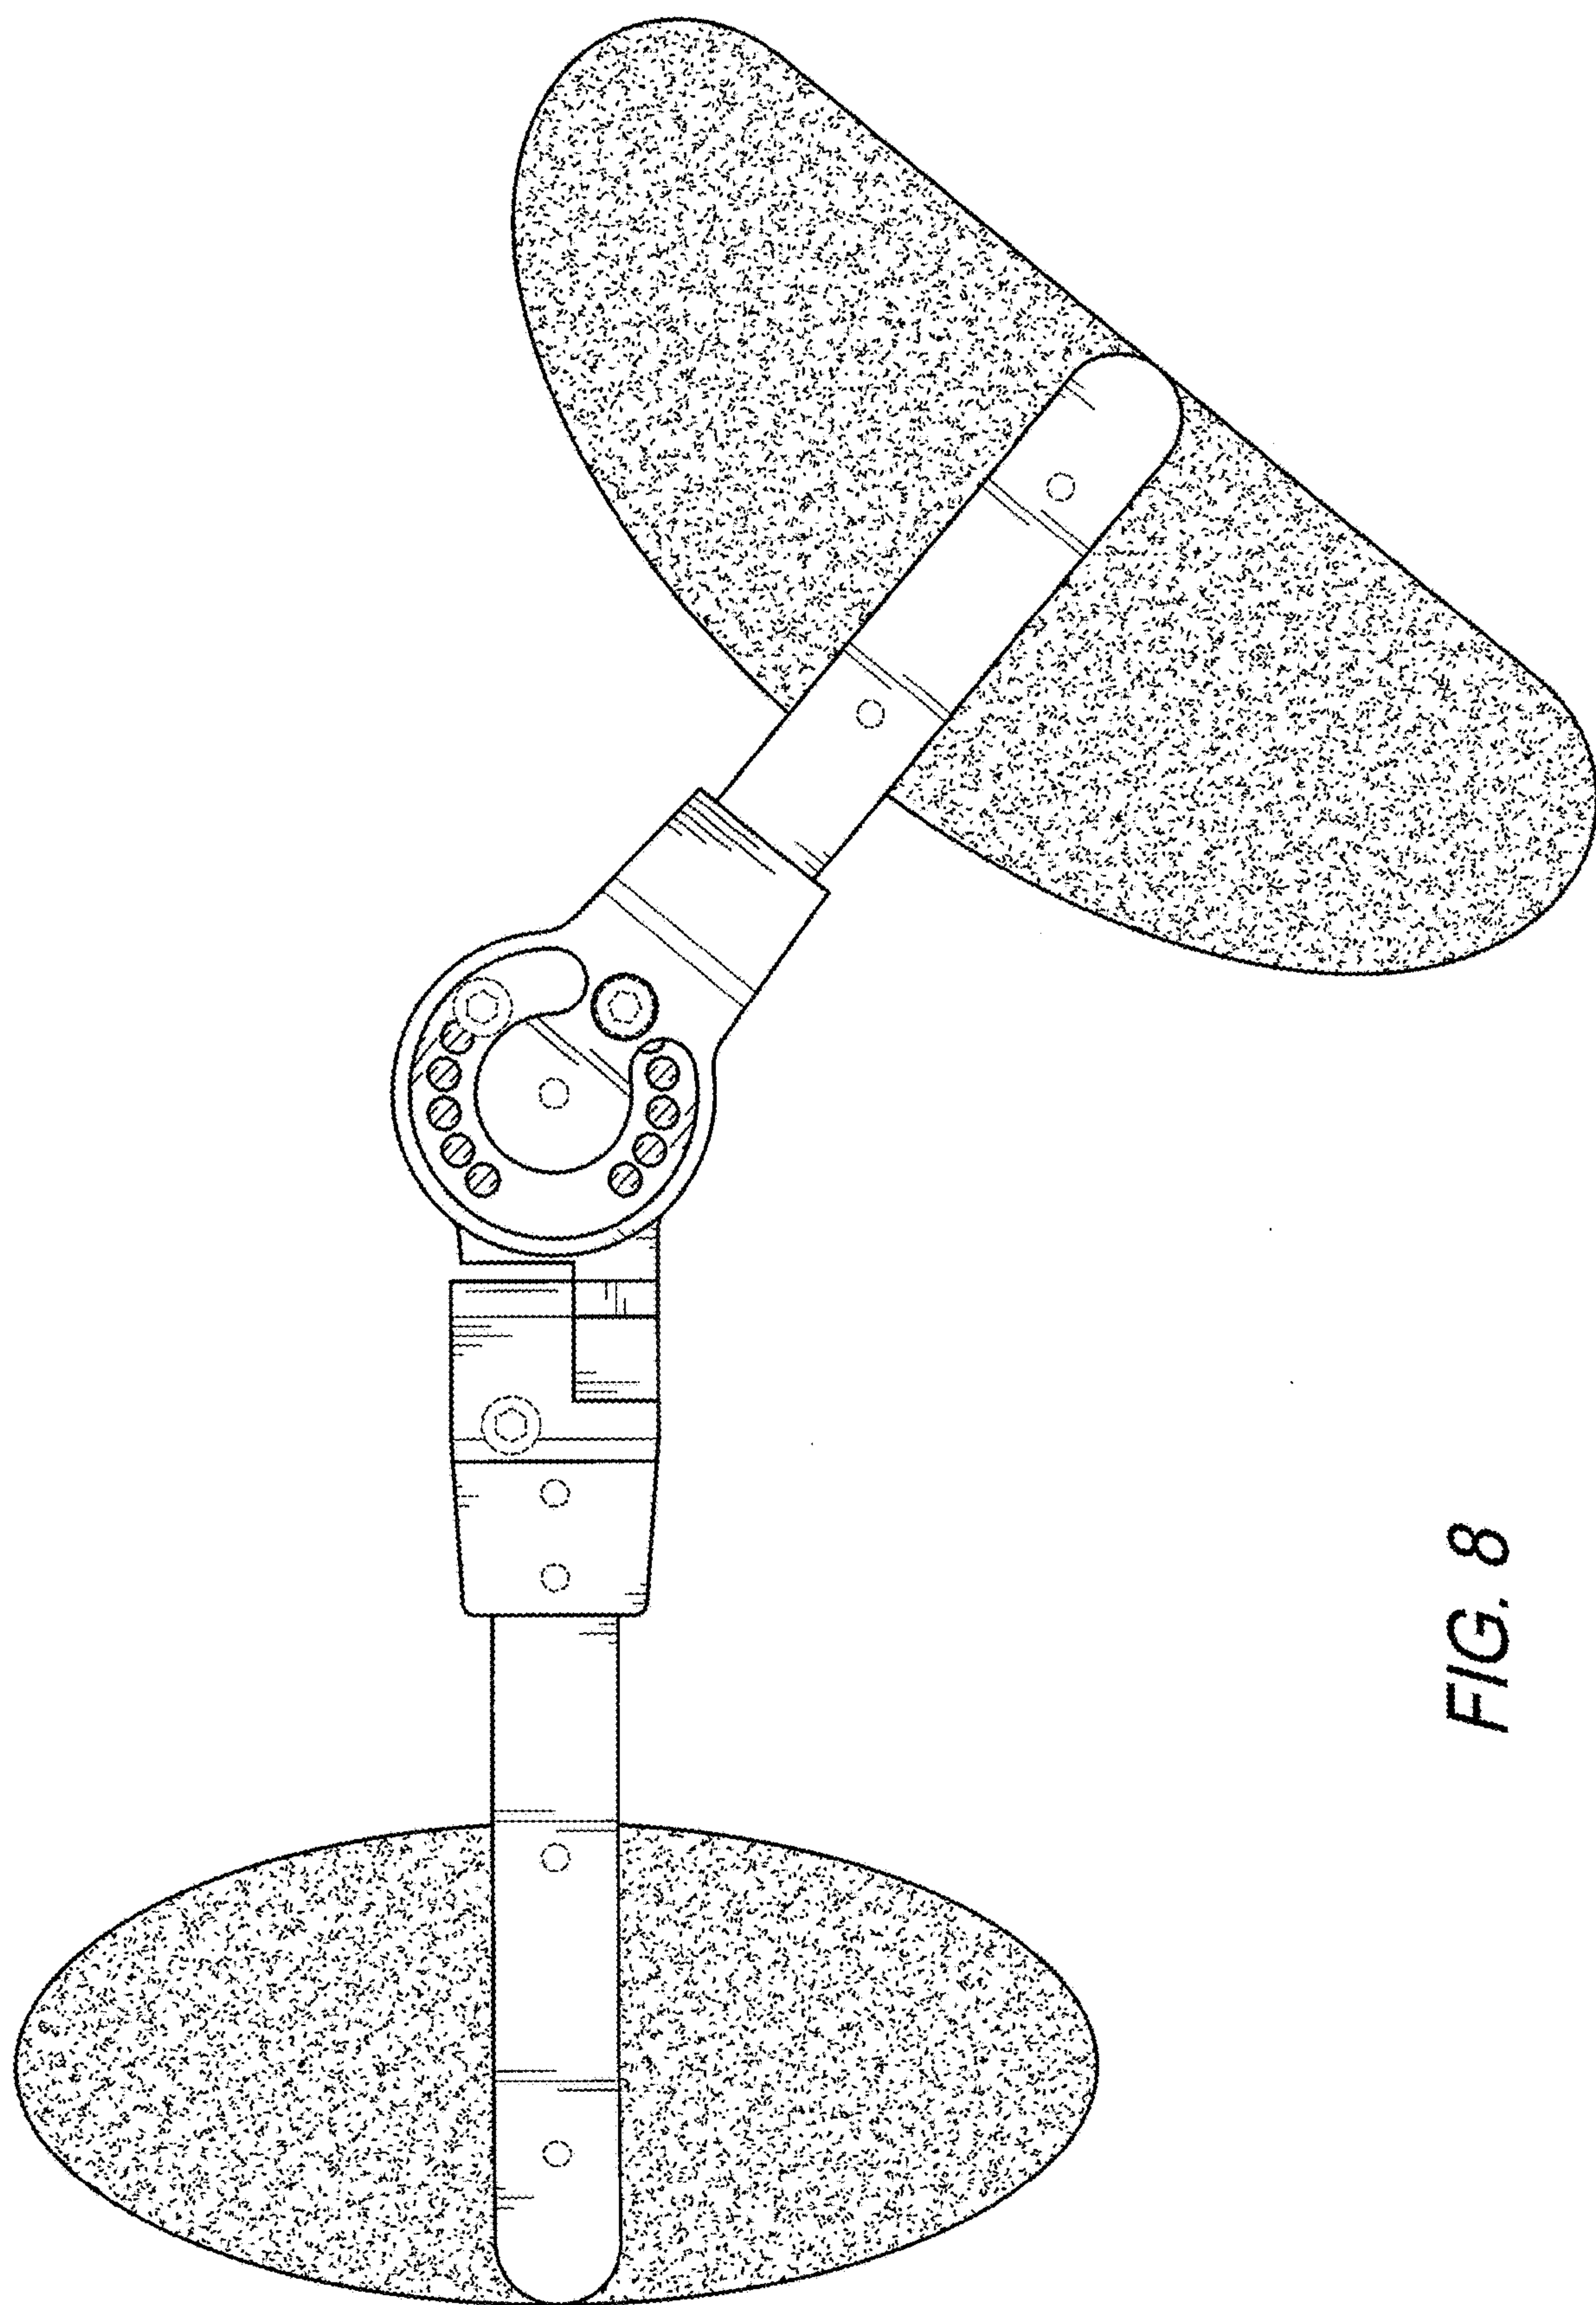


FIG. 8

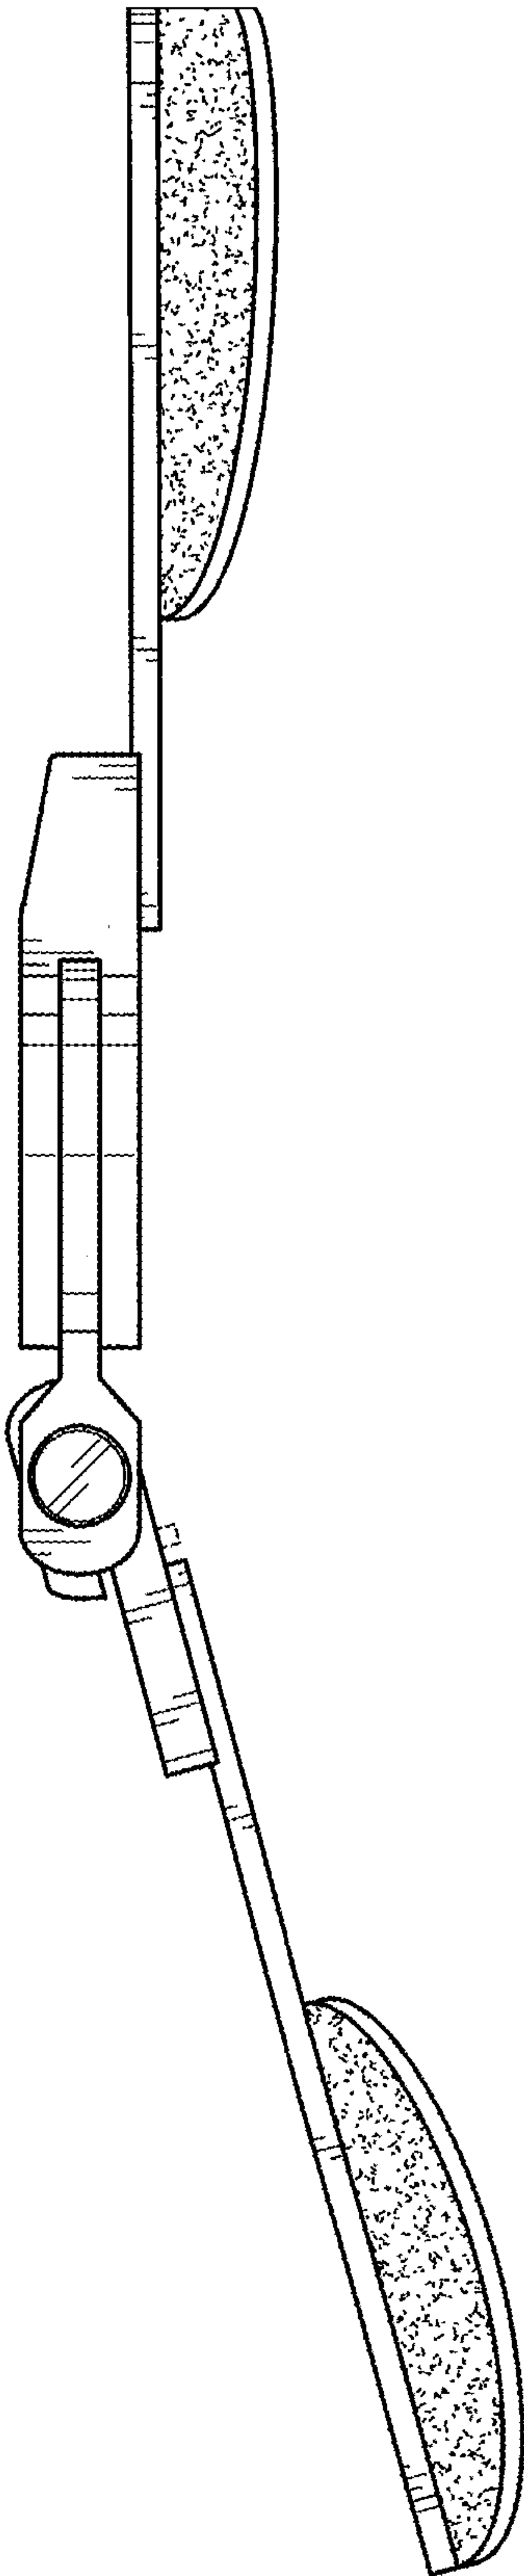


FIG. 9