



US00D947387S

(12) **United States Design Patent**
Ogura et al.

(10) **Patent No.:** **US D947,387 S**
(45) **Date of Patent:** **** Mar. 29, 2022**

(54) **ULTRASOUND PROBE**
(71) Applicant: **FUJIFILM Corporation**, Tokyo (JP)
(72) Inventors: **Ryosuke Ogura**, Ashigara-kami-gun (JP); **Shinsuke Noguchi**, Ashigara-kami-gun (JP)
(73) Assignee: **FUJIFILM Corporation**, Tokyo (JP)

D875,259 S 2/2020 Moon et al.
D878,603 S 3/2020 Zhang et al.
D879,298 S * 3/2020 Byung D24/165
10,816,650 B2 * 10/2020 Solek A61B 8/4488
D910,857 S * 2/2021 Shibayama D24/187
D916,295 S * 4/2021 Shibayama D24/187
D919,102 S * 5/2021 Ogura D24/187
2016/0113724 A1 * 4/2016 Stolka A61B 34/20
600/424

(**) Term: **15 Years**
(21) Appl. No.: **29/777,295**
(22) Filed: **Apr. 5, 2021**

Related U.S. Application Data

(62) Division of application No. 29/687,105, filed on Apr. 10, 2019, now Pat. No. Des. 919,102.
(51) **LOC (13) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/187**
(58) **Field of Classification Search**
USPC D24/133, 137, 138, 141, 158, 160, 164, D24/165, 167, 170, 186, 187, 200; D10/57, 60, 78, 80; D14/301, 462, 463, D14/487
CPC ... A61B 5/0095; A61B 8/4444; A61B 8/4455; A61B 8/565; G01S 7/5208; G01N 29/24
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D555,252 S 11/2007 Kitayama et al.
8,137,281 B2 * 3/2012 Huang A61B 8/0833
600/461
D681,820 S 5/2013 Shinohara et al.
D681,823 S 5/2013 Shinohara et al.
D703,330 S 4/2014 Saeki
D811,608 S 2/2018 Kitayama
D816,850 S 5/2018 Asai et al.
D865,973 S 11/2019 Chamberlain et al.

(Continued)

OTHER PUBLICATIONS

Wireless B&W Ultrasound Probe—CONVEX-3.5/ 5.0MHZ. Online, published date unknown. Retrieved on Jun. 30, 2021 from URL: https://interaktivhealth.com.au/products/wireless-ultrasound-scanner-ss-2ii-convex-3-5-5-0mhz.*

(Continued)

Primary Examiner — Susan Bennett Hattan
Assistant Examiner — Omeed Agilee
(74) *Attorney, Agent, or Firm* — Birch, Stewart, Kolasch & Birch, LLP


(57) **CLAIM**

The ornamental design for an ultrasound probe, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an ultrasound probe, FIG. 2 is a front view of the ultrasound probe, FIG. 3 is a back view of the ultrasound probe, FIG. 4 is a top view of the ultrasound probe, FIG. 5 is a bottom view of the ultrasound probe, FIG. 6 is a right side view of the ultrasound probe; and, FIG. 7 is a left side view of the ultrasound probe. The dash lines depict portions of the ultrasound probe that form no part of the claimed design. The dot dash dot broken lines depict the boundaries of the claim and form no part thereof.

1 Claim, 3 Drawing Sheets

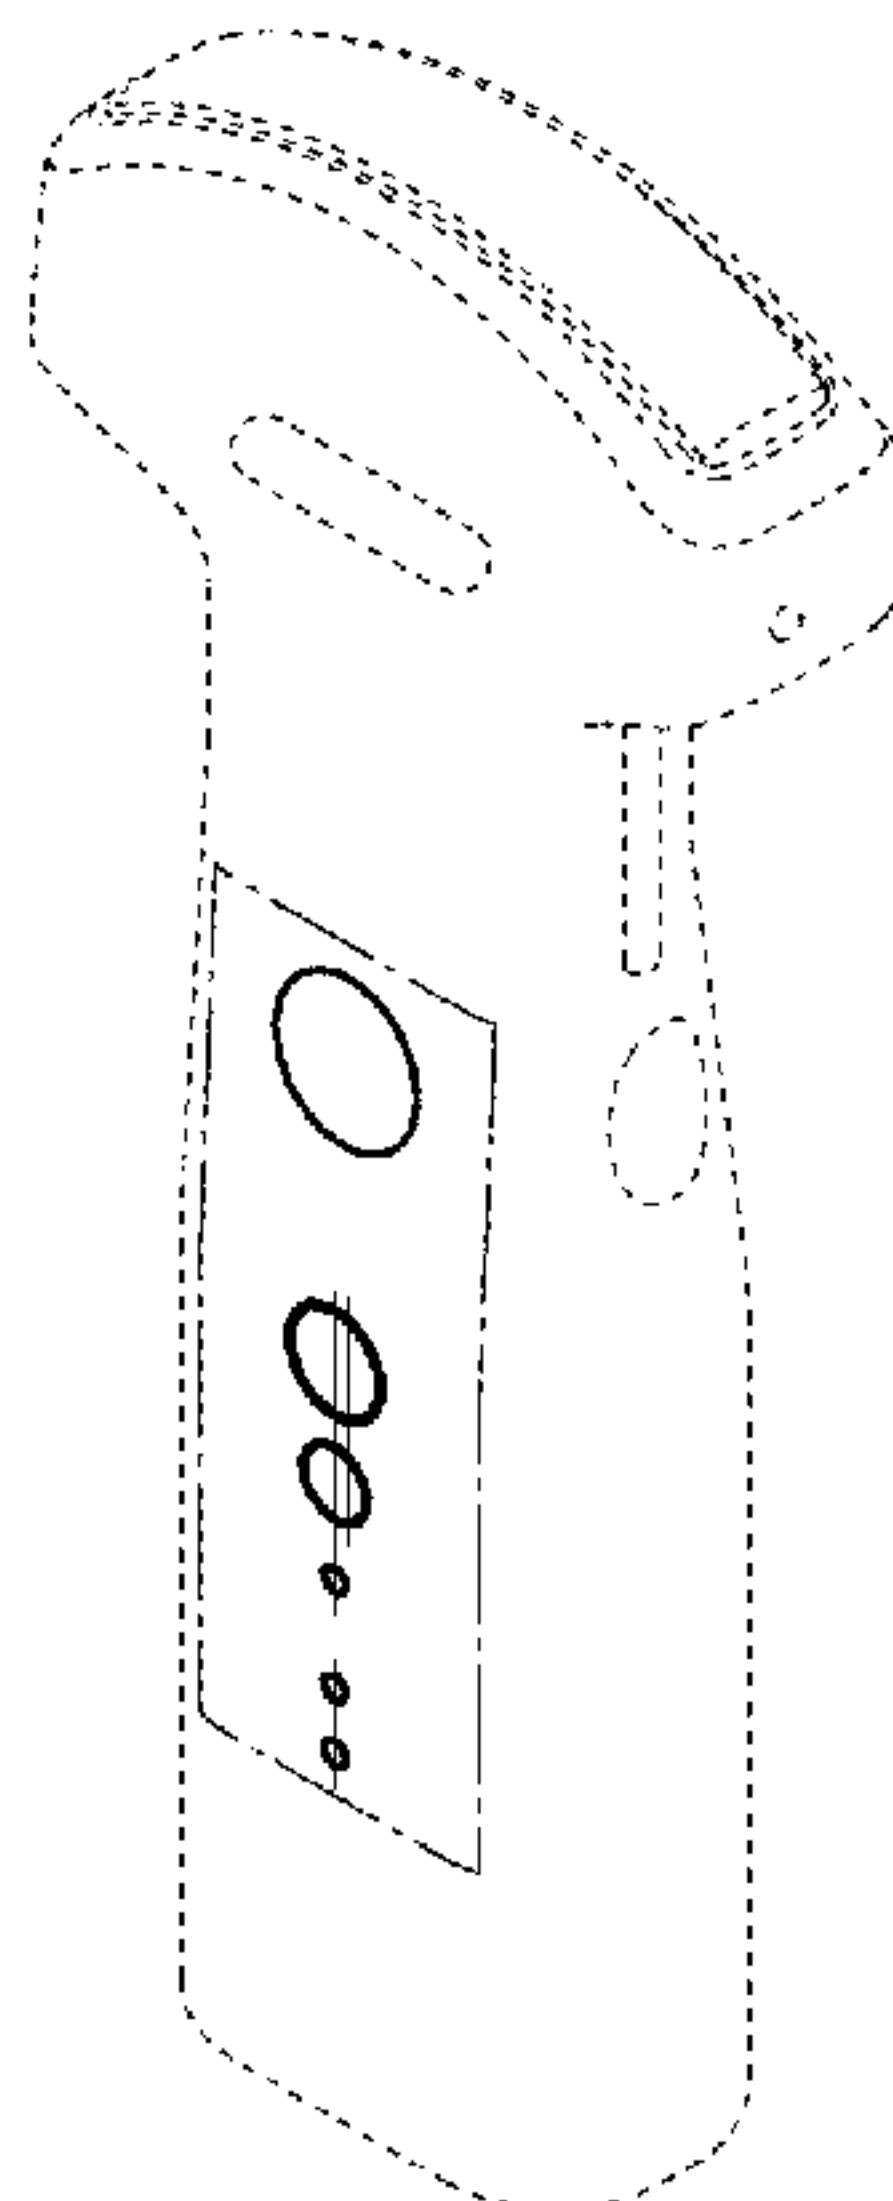

(56)

References Cited

U.S. PATENT DOCUMENTS

2018/0110497 A1* 4/2018 Beacham B33Y 80/00

OTHER PUBLICATIONS

Ultrasound Diagnostic Imaging Equipment. Online, published date unknown. Retrieved on Jun. 30, 2021 from URL: <http://www-g-mark-org-product.elasticbeanstalk.com/award/describe/49151?locale=en>.*

Notice of Allowance dated Jan. 6, 2021, in corresponding U.S. Appl. No. 29/687,105.

Office Action dated Sep. 1, 2020, in corresponding U.S. Appl. No. 29/687,105.

Office Action dated Sep. 14, 2020, in corresponding U.S. Appl. No. 26/687,105.

Restriction Requirement dated Jun. 8, 2020, in corresponding U.S. Appl. No. 29/687,105.

Wireless Color Ultrasound Scanner Convex Probe New Version 3.5-5Mhz/128 Android, New Look. Online, published date unknown. Retrieved on Jun. 2, 2020 from URL: <https://wififulras.com/products/wireless-color-ultrasound-scanner-convex-probe-new-version-3-5-5mhz-12>.

* cited by examiner

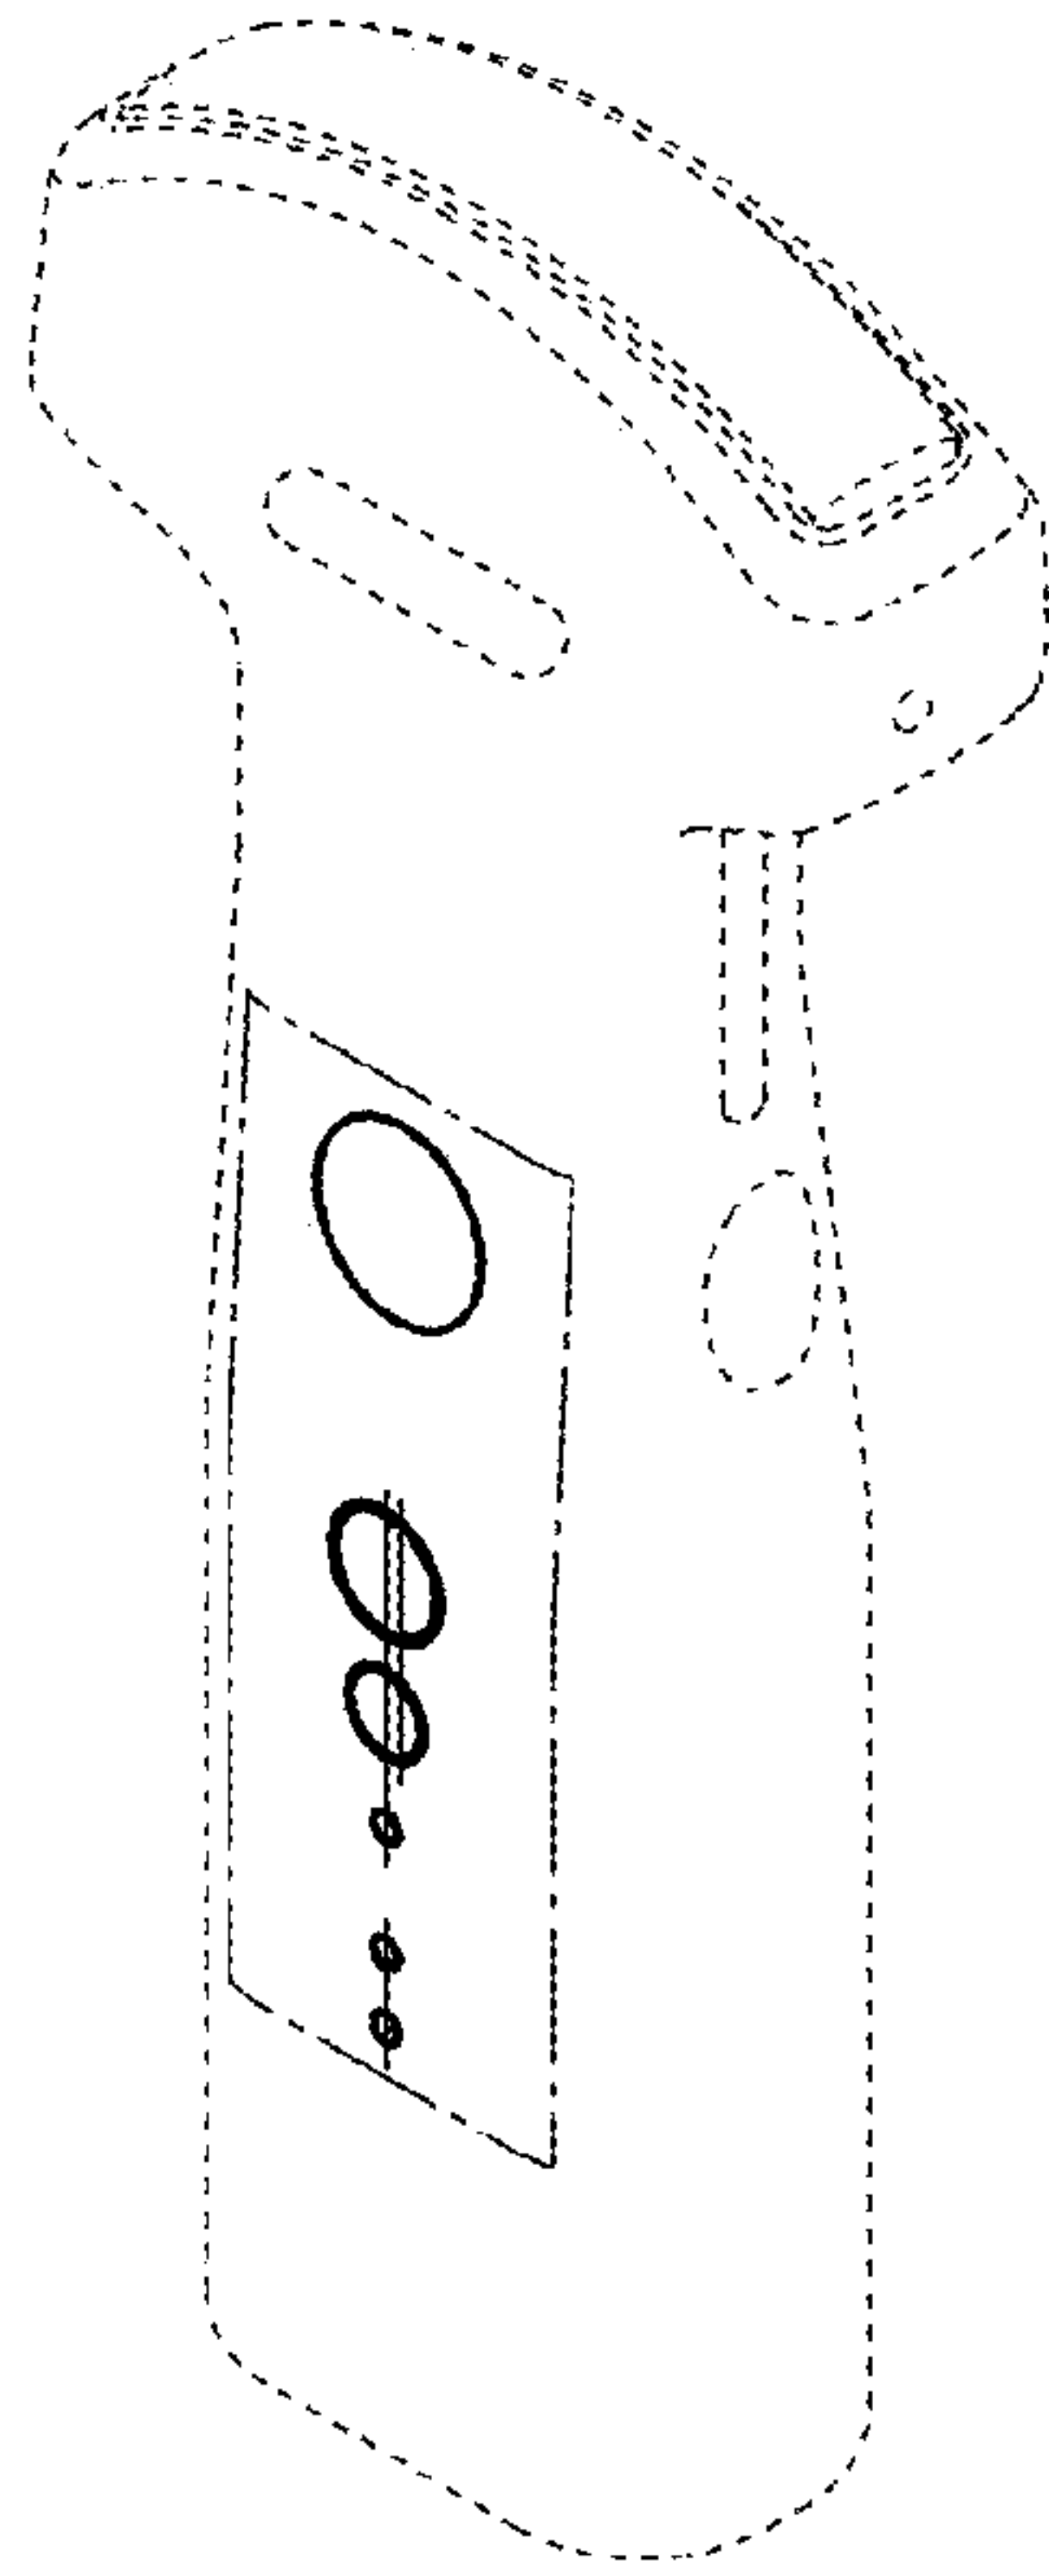


FIG. 1

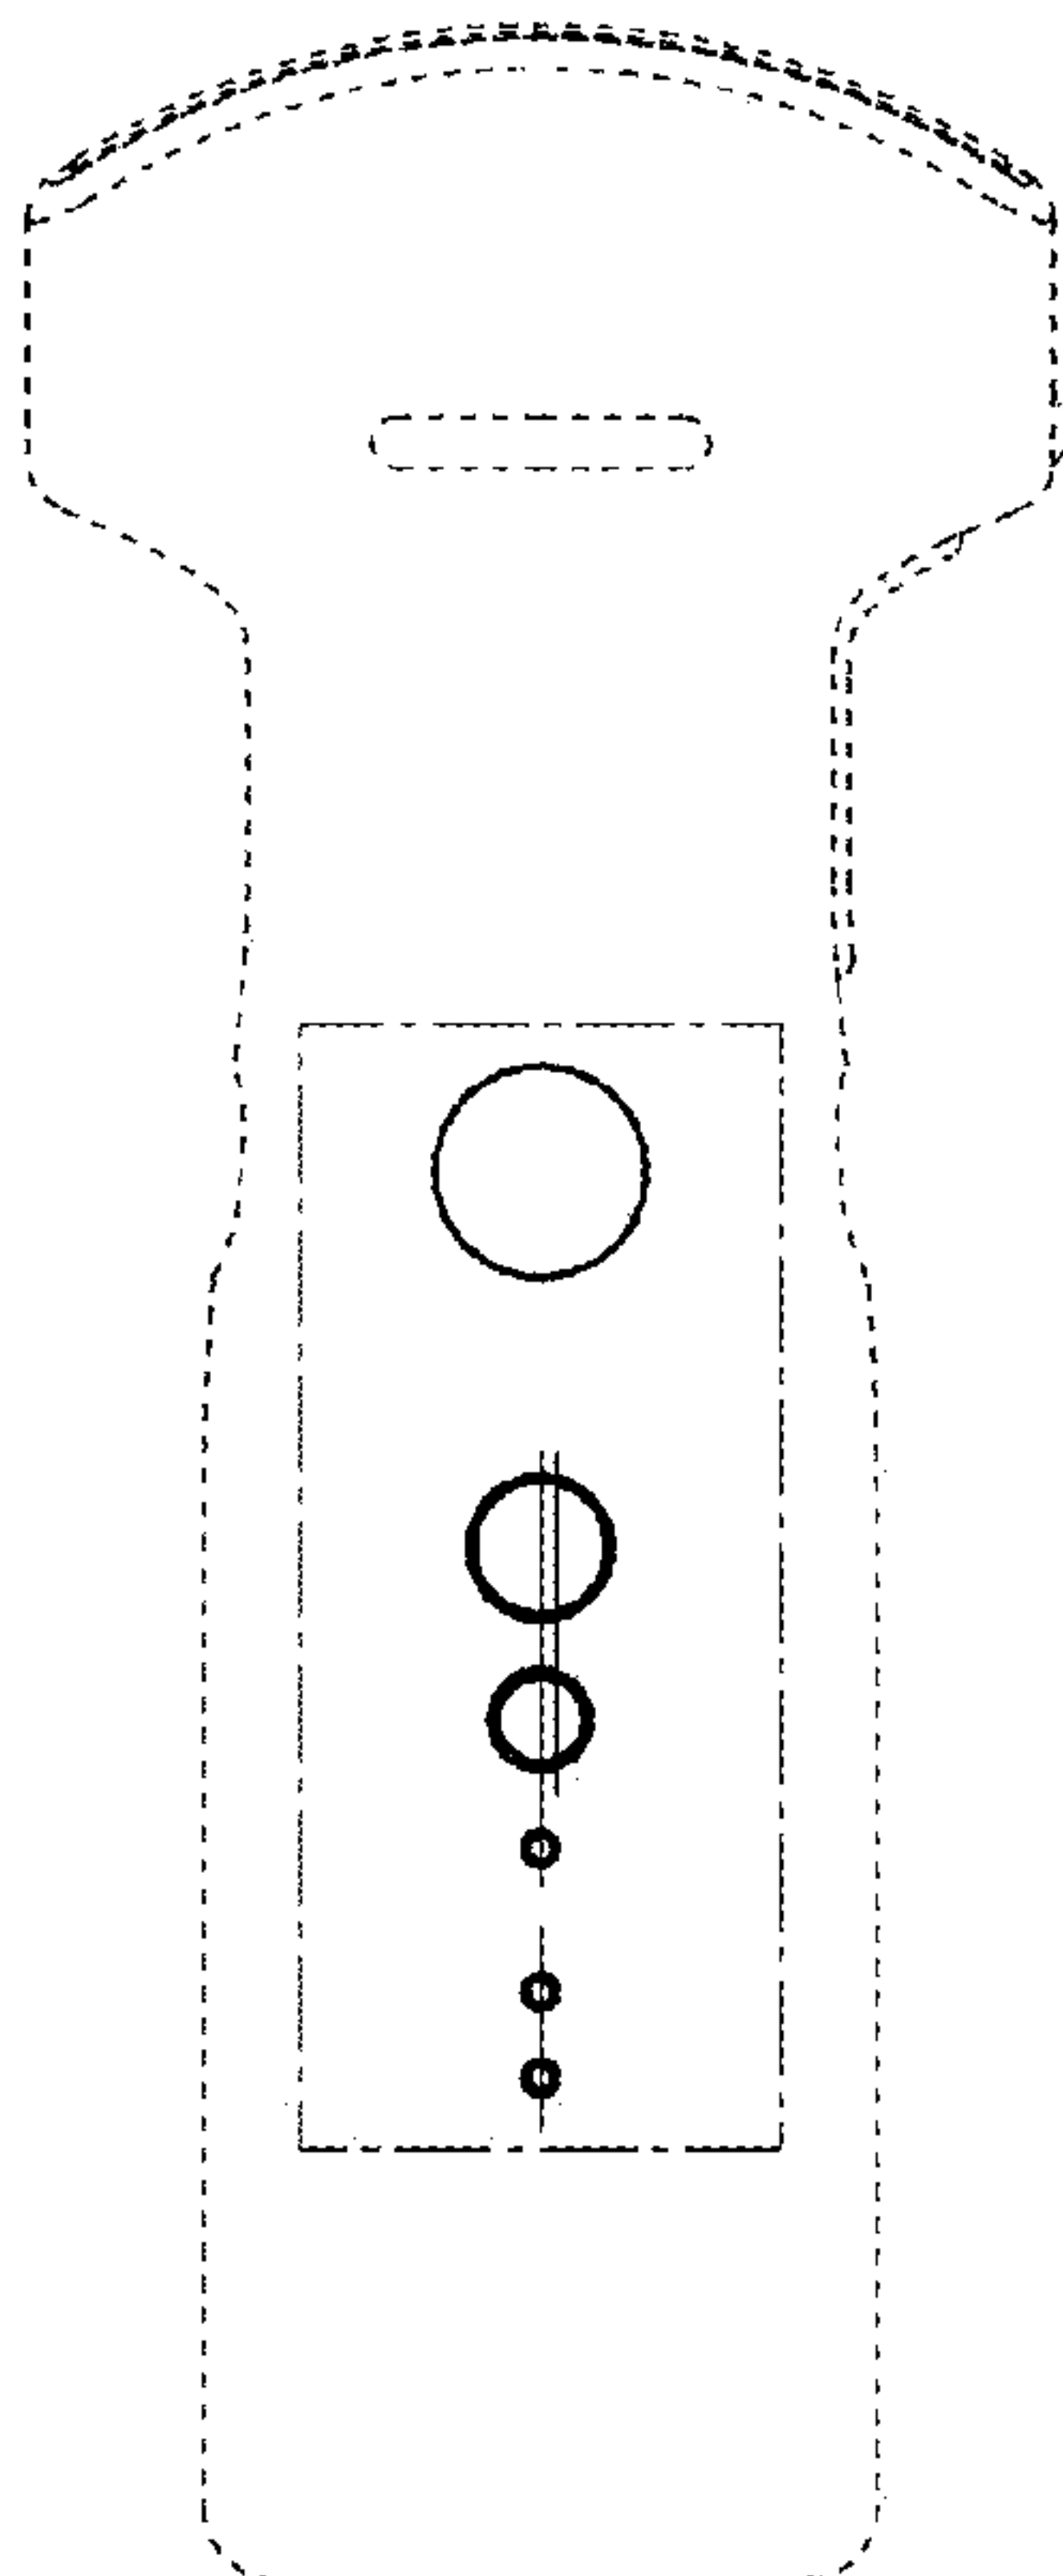


FIG. 2

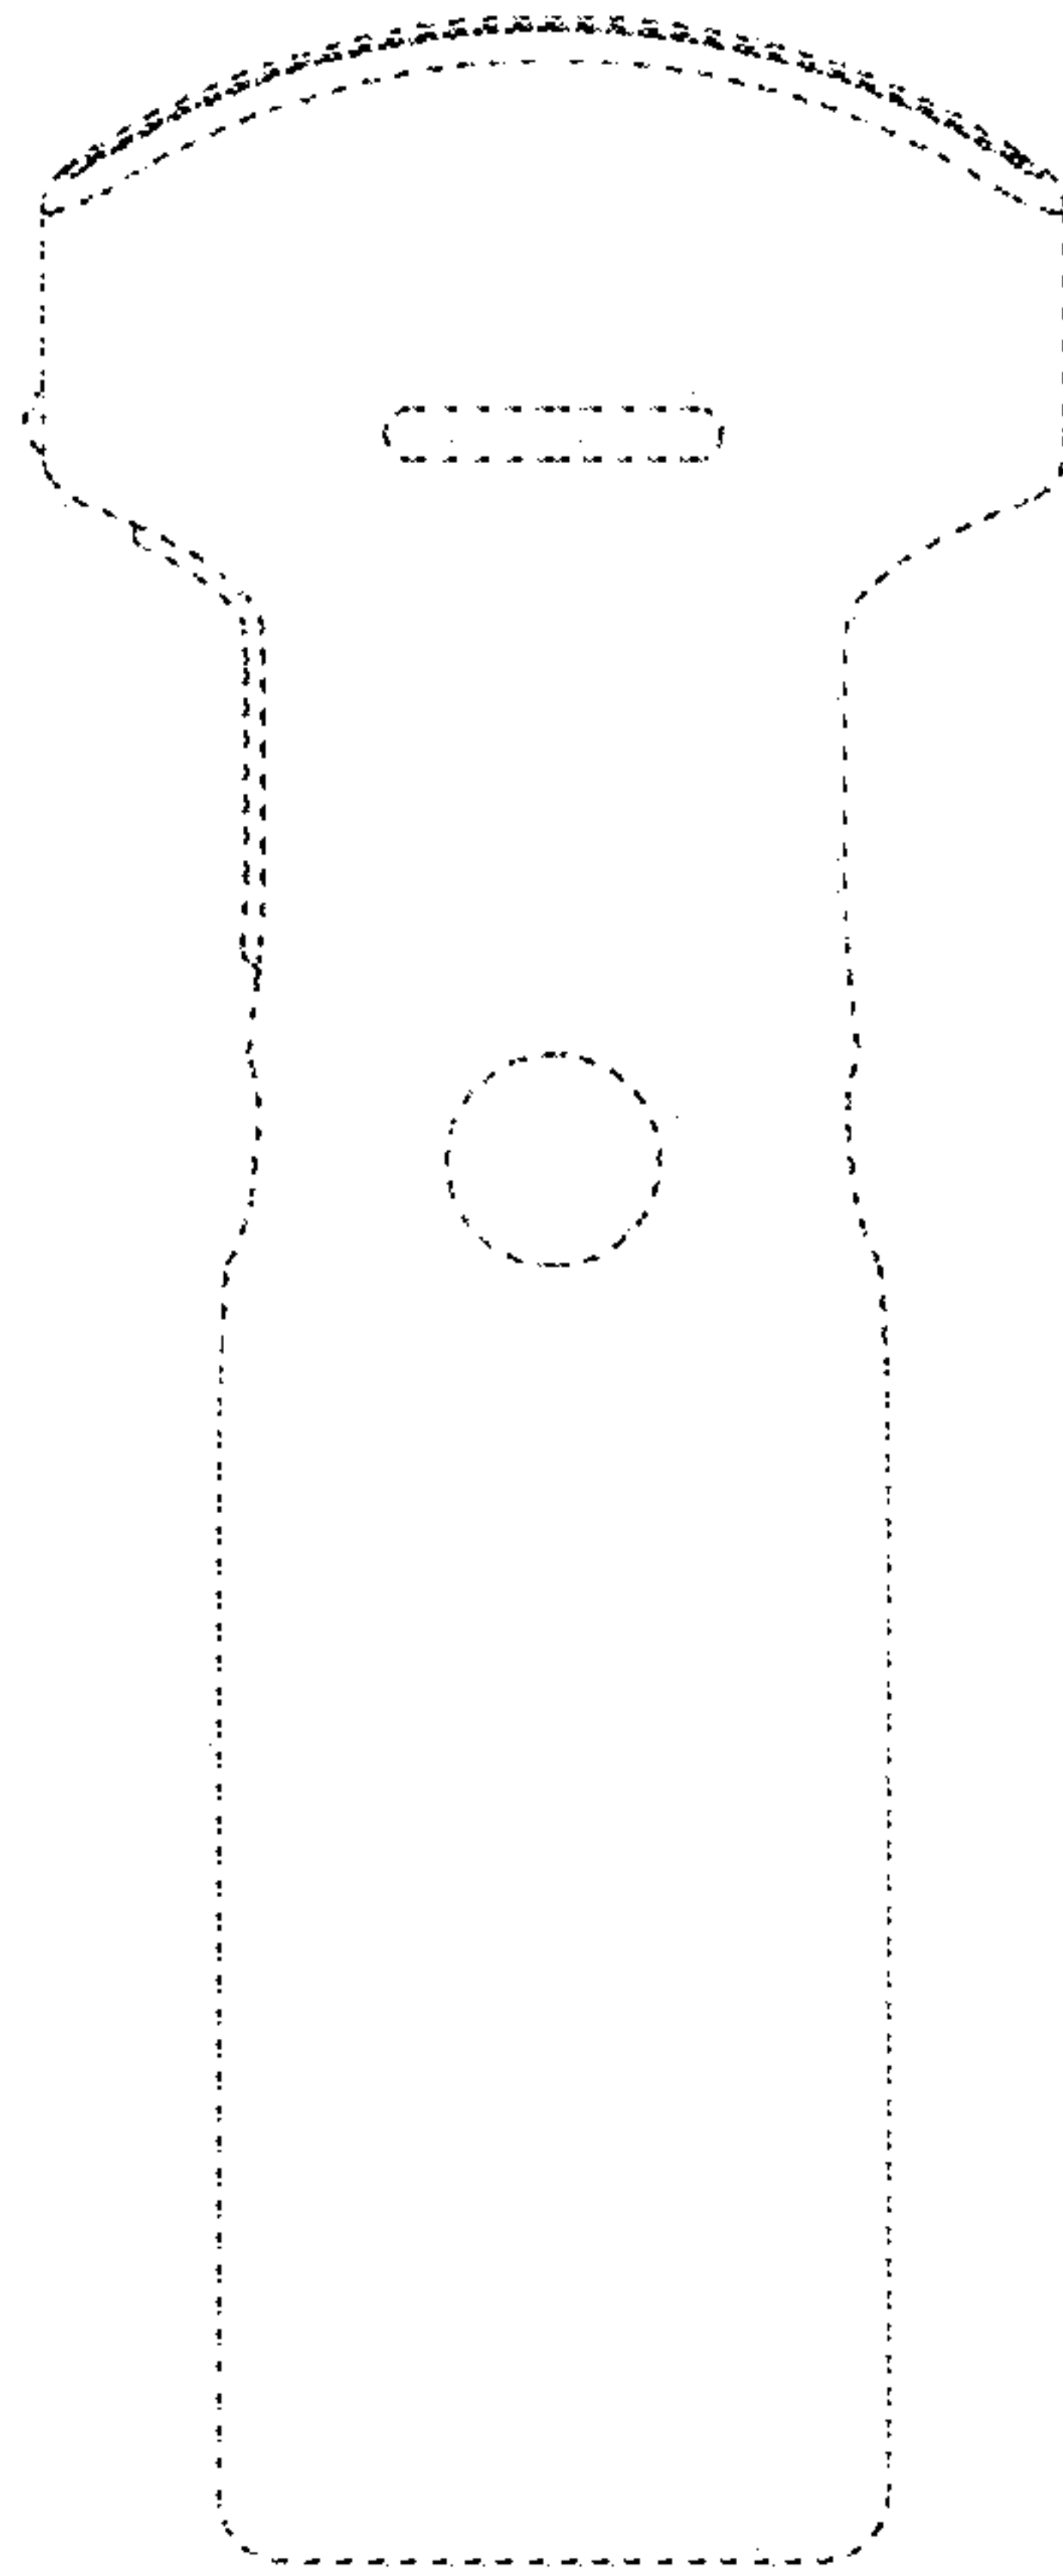


FIG. 3

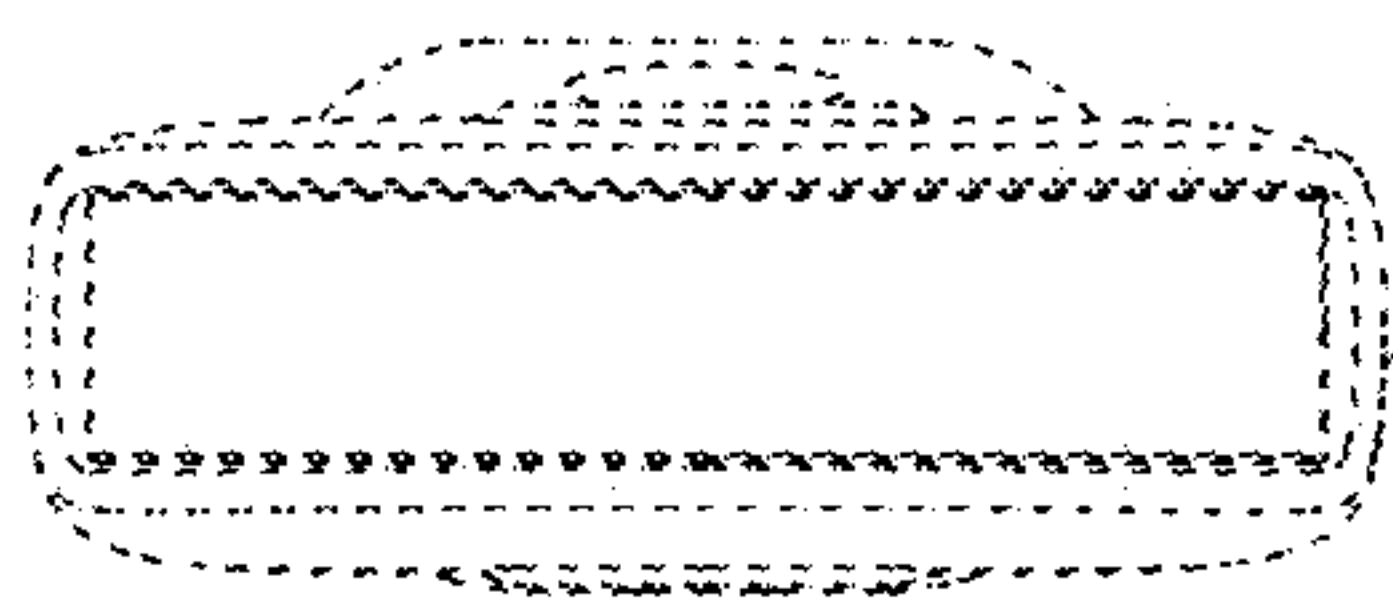


FIG. 4

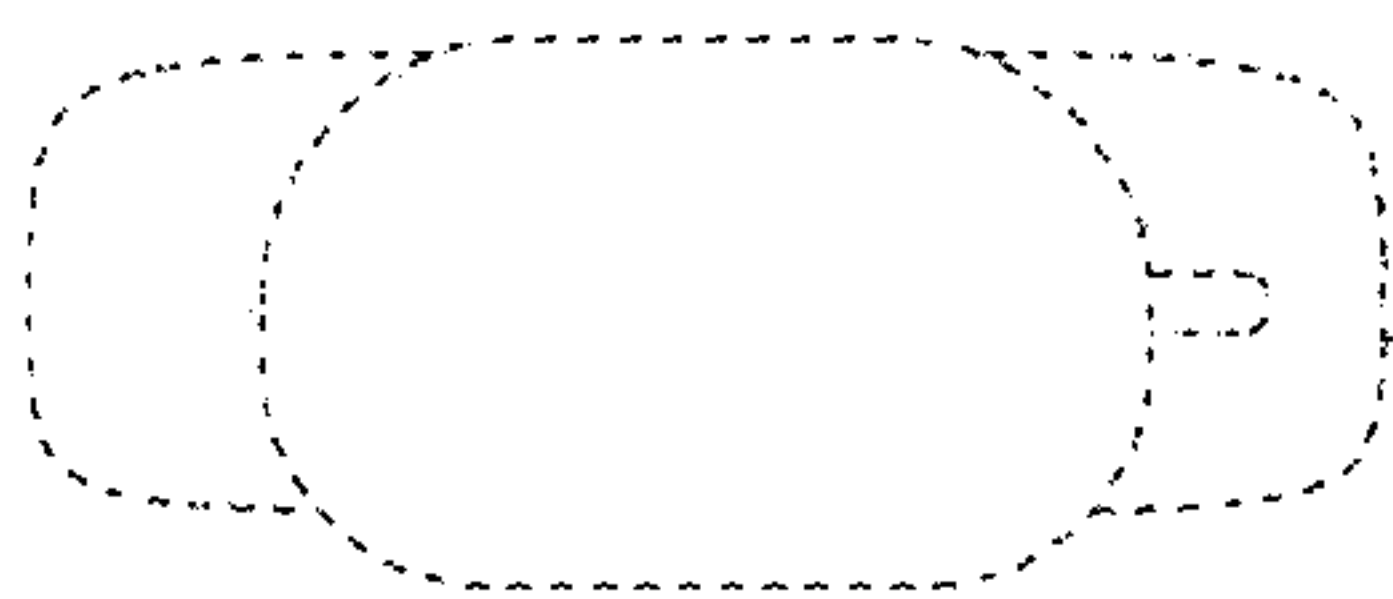


FIG. 5

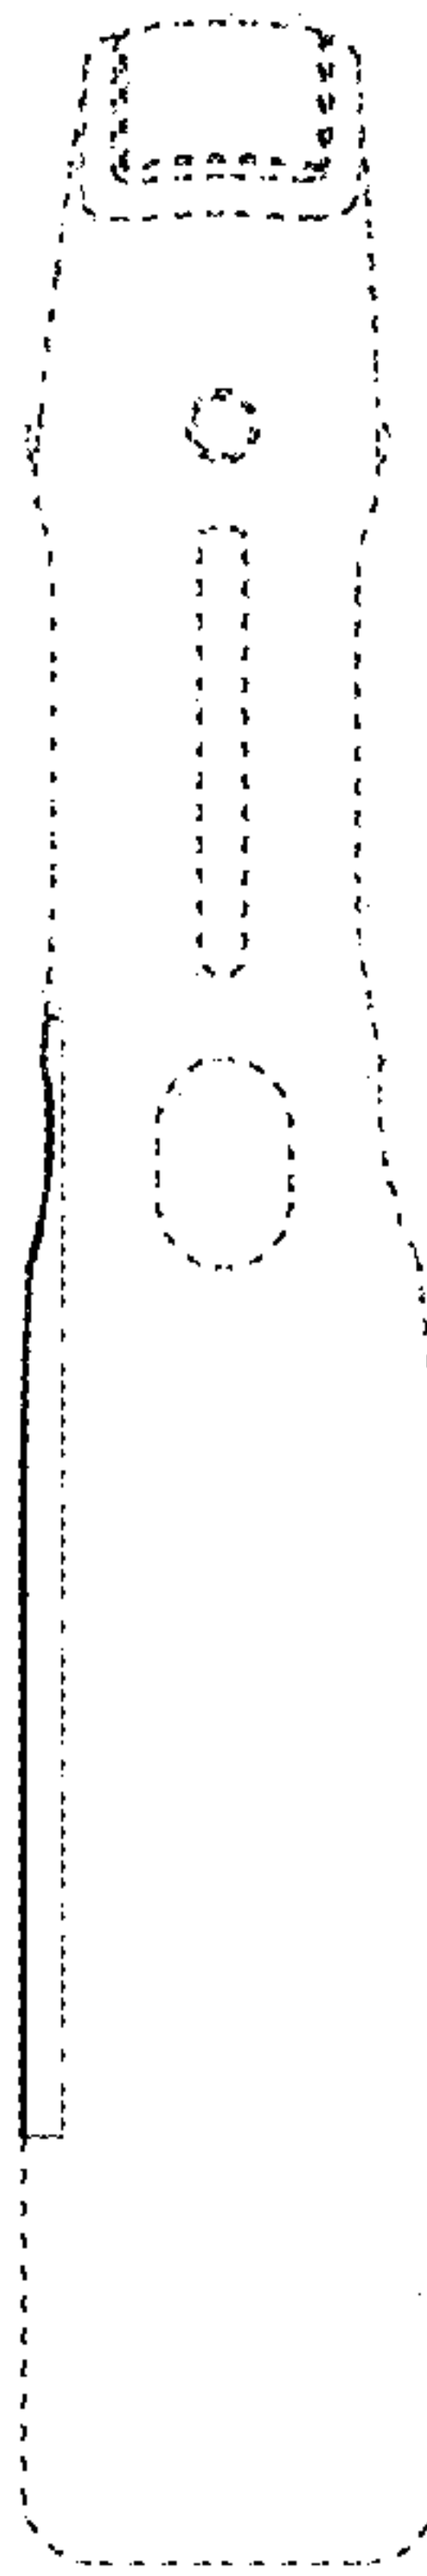


FIG. 6

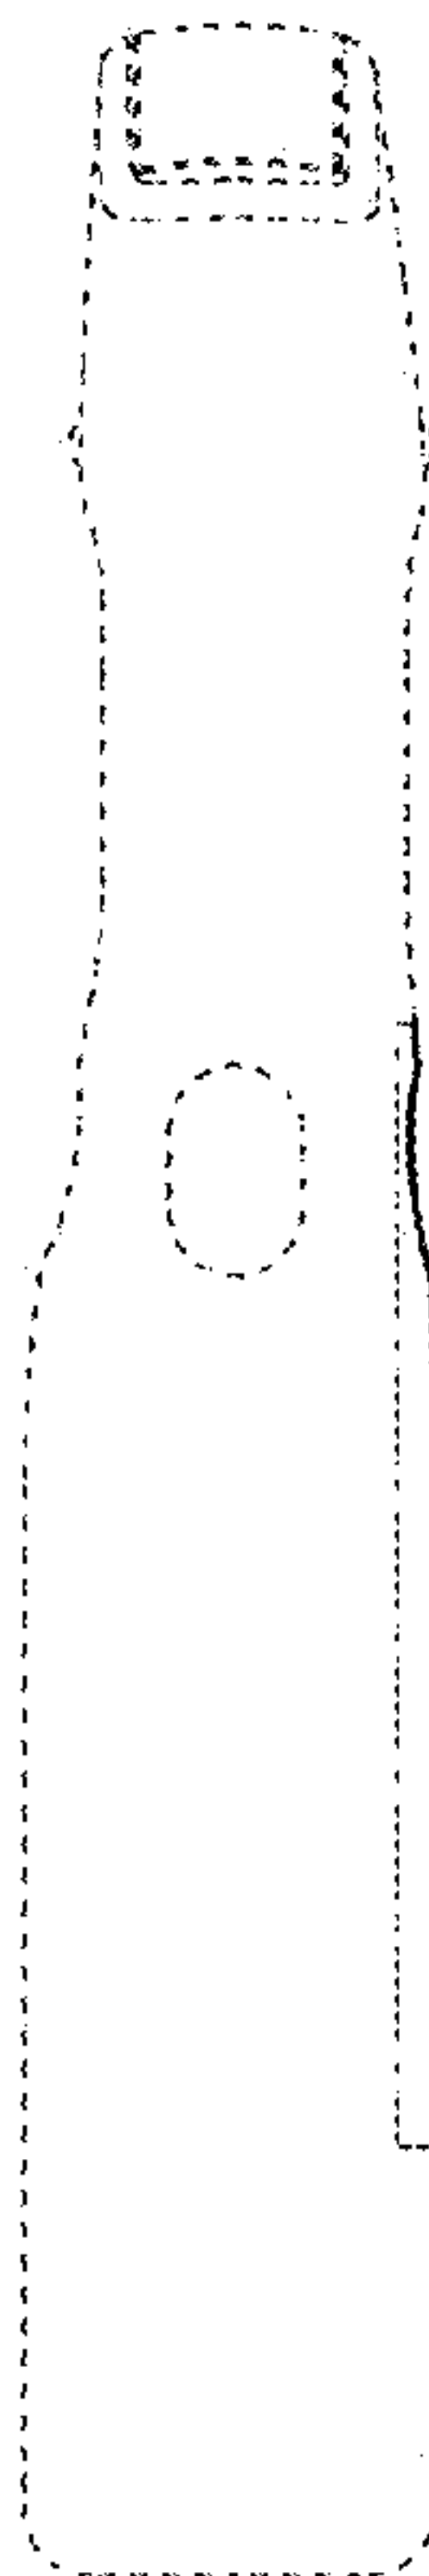


FIG. 7

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D947,387 S
APPLICATION NO. : 29/777295
DATED : March 29, 2022
INVENTOR(S) : Ryosuke Ogura et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

After item (22), please insert:

-- (30) **Foreign Application Priority Data**

Oct. 11, 2018 (JP) 2018-022302
Oct. 11, 2018 (JP) 2018-022303
Oct. 11, 2018 (JP) 2018-022327
Oct. 11, 2018 (JP) 2018-022346
Oct. 11, 2018 (JP) 2018-022347
Oct. 11, 2018 (JP) 2018-022348
Oct. 11, 2018 (JP) 2018-022349
Dec. 28, 2018 (JP) 2018-028879
Dec. 28, 2018 (JP) 2018-028899
Dec. 28, 2018 (JP) 2018-028900
Dec. 28, 2018 (JP) 2018-028945 --

Signed and Sealed this
Ninth Day of August, 2022
Katherine Kelly Vidal

Katherine Kelly Vidal
Director of the United States Patent and Trademark Office