



US00D949091S

(12) **United States Design Patent**
Baldwin et al.

(10) **Patent No.:** **US D949,091 S**

(45) **Date of Patent:** **** Apr. 19, 2022**

(54) **BATTERY PACK FOR A MEDICAL DEVICE**

(71) Applicant: **ViOptix, Inc.**, Newark, CA (US)

(72) Inventors: **Alan Baldwin**, San Jose, CA (US);
Mark Gil Martin, Hayward, CA (US);
Joseph G. Santiago, Fremont, CA
(US); **William Welch**, Sunnyvale, CA
(US)

(73) Assignee: **ViOptix, Inc.**, Newark, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/720,115**

(22) Filed: **Jan. 9, 2020**

(51) **LOC (13) Cl.** **13-02**

(52) **U.S. Cl.**
USPC **D13/103**

(58) **Field of Classification Search**
USPC D13/102, 103, 104, 105, 106, 107, 108,
D13/110, 118, 119, 184, 199; D3/273,
D3/274, 302, 201, 264
CPC Y02E 60/12; Y02E 60/122; Y02E 60/124;
Y02E 60/50; H01M 10/4257; H01M
10/0436; H01M 10/48; H01M 2/02;
H01M 2/022; H01M 2/0202; H01M
2/0207; H01M 2/0212; H01M 2/1061;
H01M 2/1022; H01M 2/1055; H01M
2/1066; H01M 2/105; H01M 2/204;
H01M 2/04; H01M 2/0404; H01M
2/0406; H01M 2/0465; H01M 2/06
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D695,217 S * 12/2013 Dasbach D13/110
D695,218 S * 12/2013 Dasbach D13/110

D695,219 S * 12/2013 Dasbach D13/110
D703,135 S * 4/2014 Dasbach D13/110
D720,693 S * 1/2015 Dasbach D13/110
D720,694 S * 1/2015 Dasbach D13/110
D721,035 S * 1/2015 Dasbach D13/110
D722,021 S * 2/2015 Dasbach D13/110
D722,022 S * 2/2015 Dasbach D13/110
D760,645 S * 7/2016 Chen D13/103
D853,320 S * 7/2019 Guo D13/103

* cited by examiner

Primary Examiner — Rosemary K Tarcza

Assistant Examiner — Seth David Kumpf

(74) *Attorney, Agent, or Firm* — Aka Chan LLP

(57) **CLAIM**


The ornamental design for a battery pack for a medical device, as shown and described.

DESCRIPTION

FIG. 1 shows a perspective view of a design for a battery pack for a medical device.
FIG. 2 shows a top view thereof.
FIG. 3 shows a bottom view thereof.
FIG. 4 shows a left side view thereof.
FIG. 5 shows a right side view thereof.
FIG. 6 shows a front side view thereof.
FIG. 7 shows a back side view thereof; and,
FIG. 8 shows a perspective view of the battery pack in use with the medical device.

The broken lines in the drawings represent structure or features that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

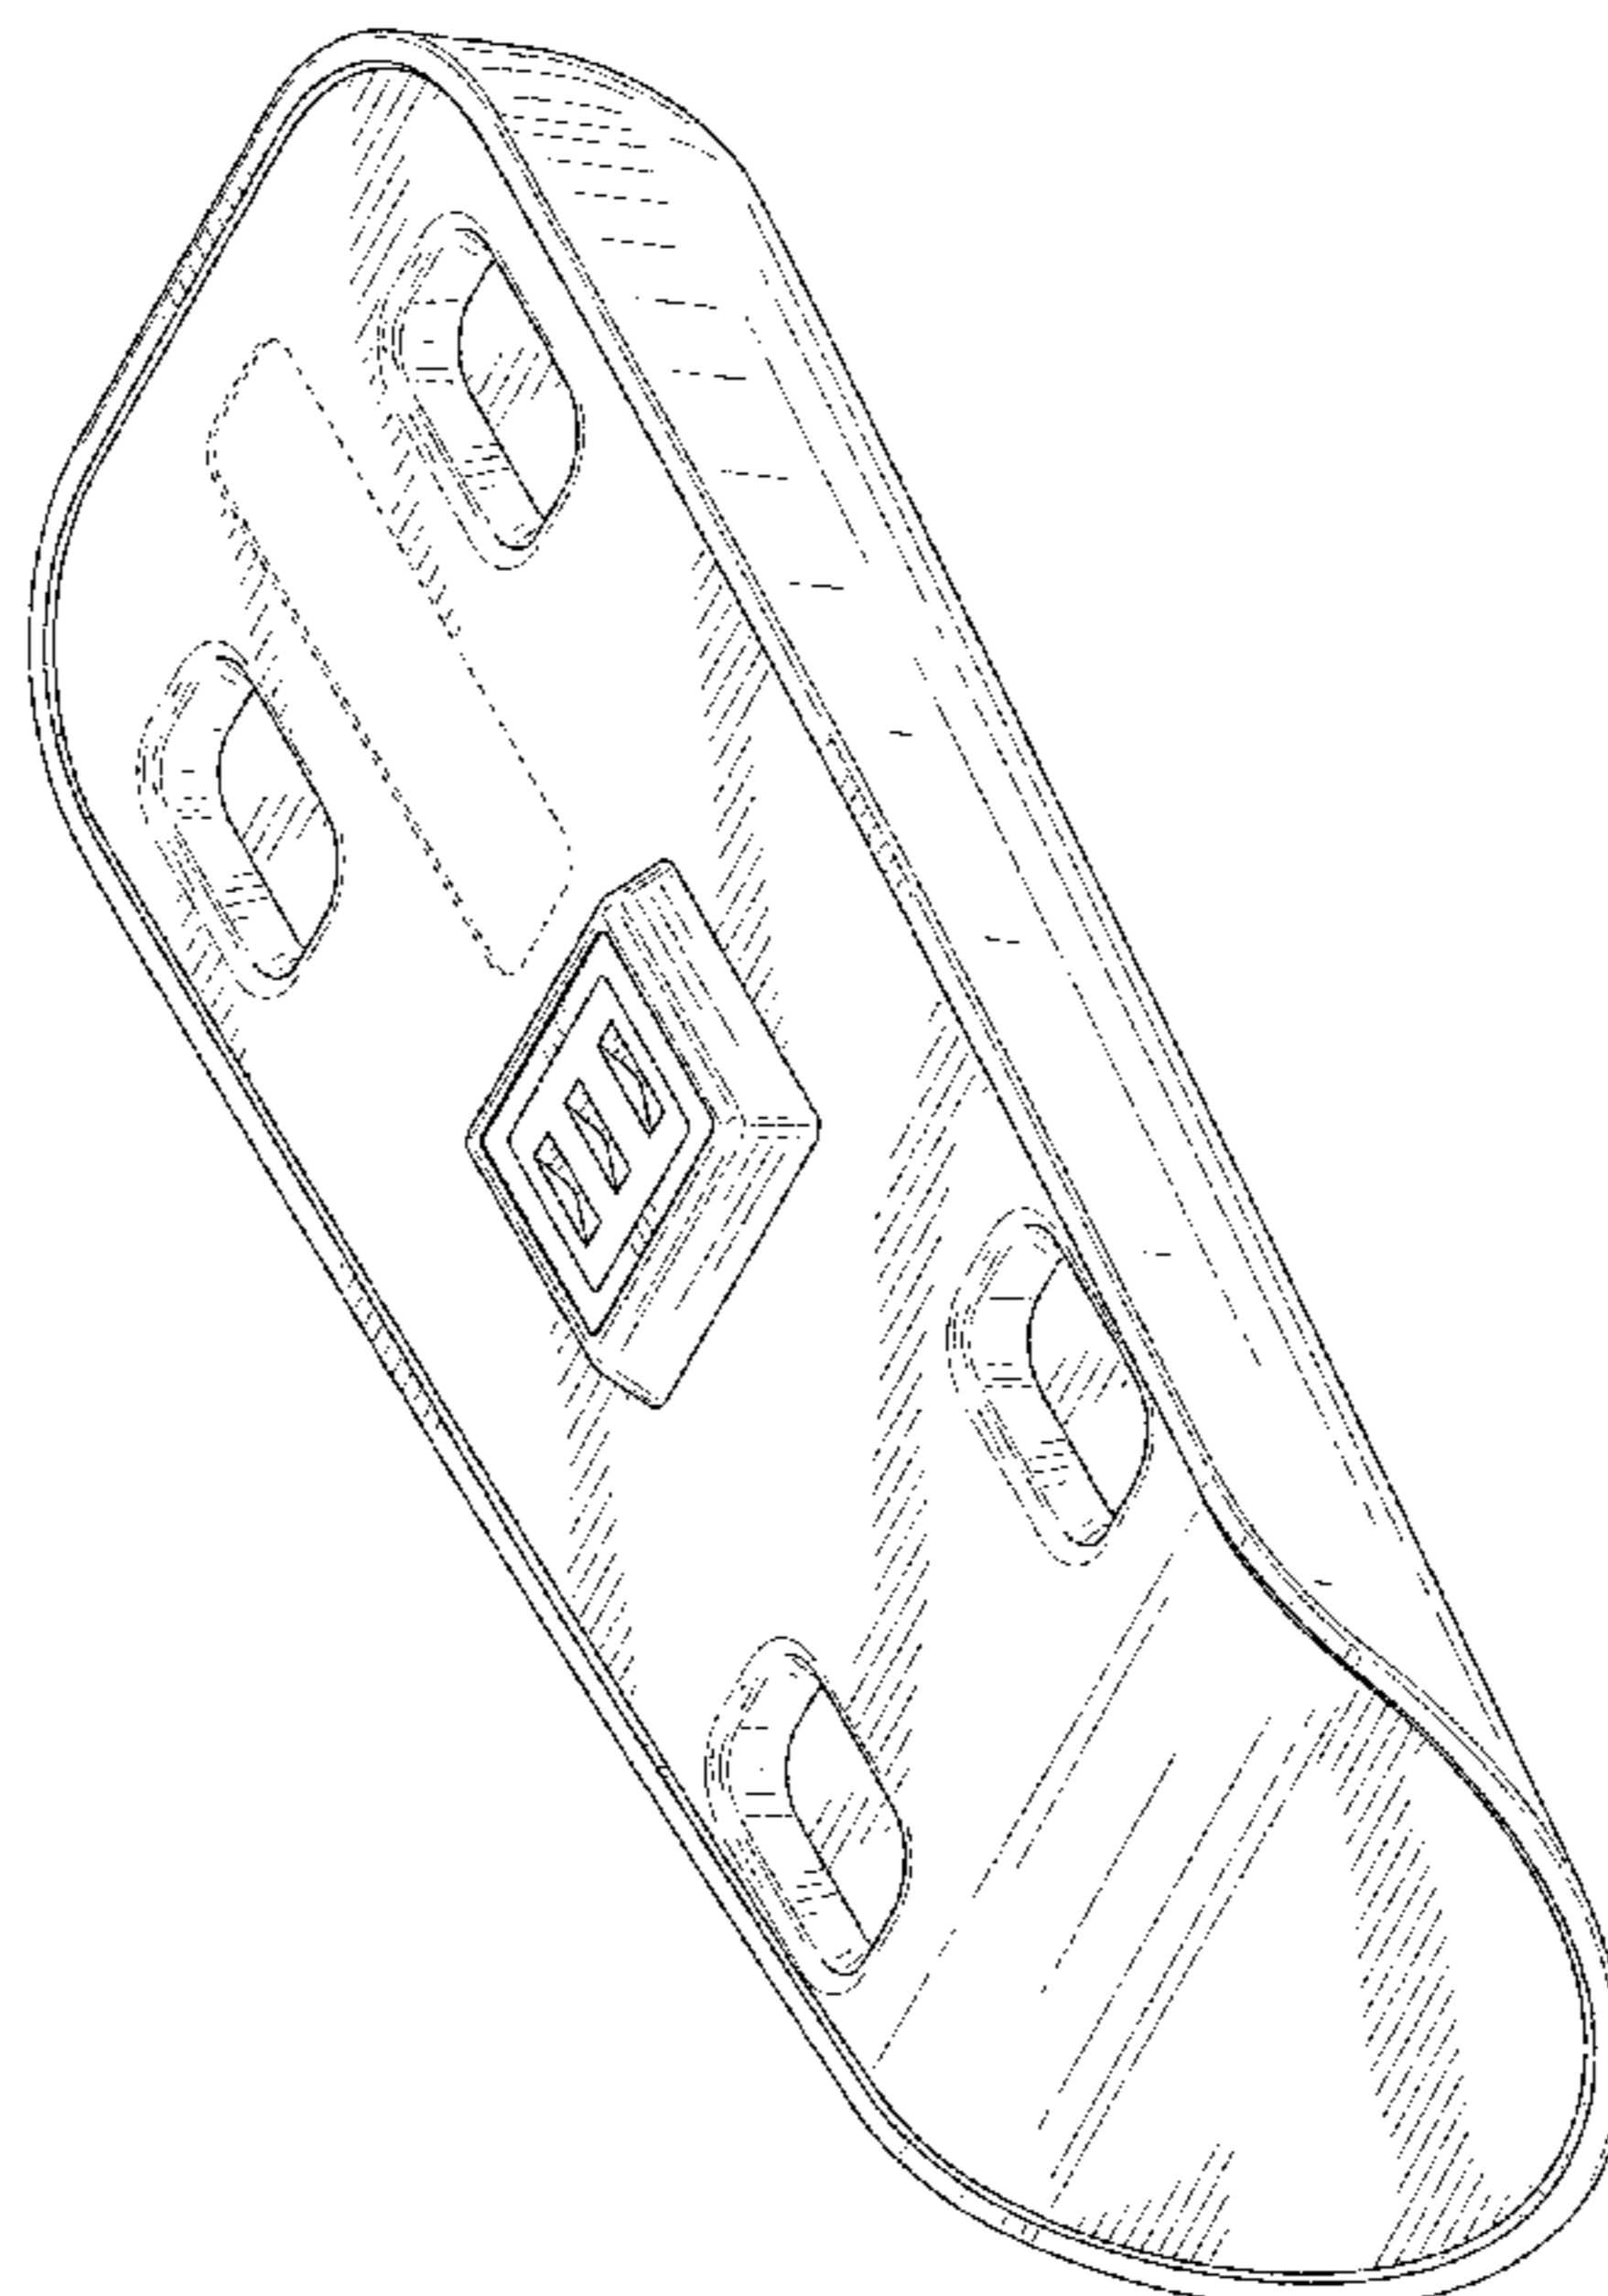

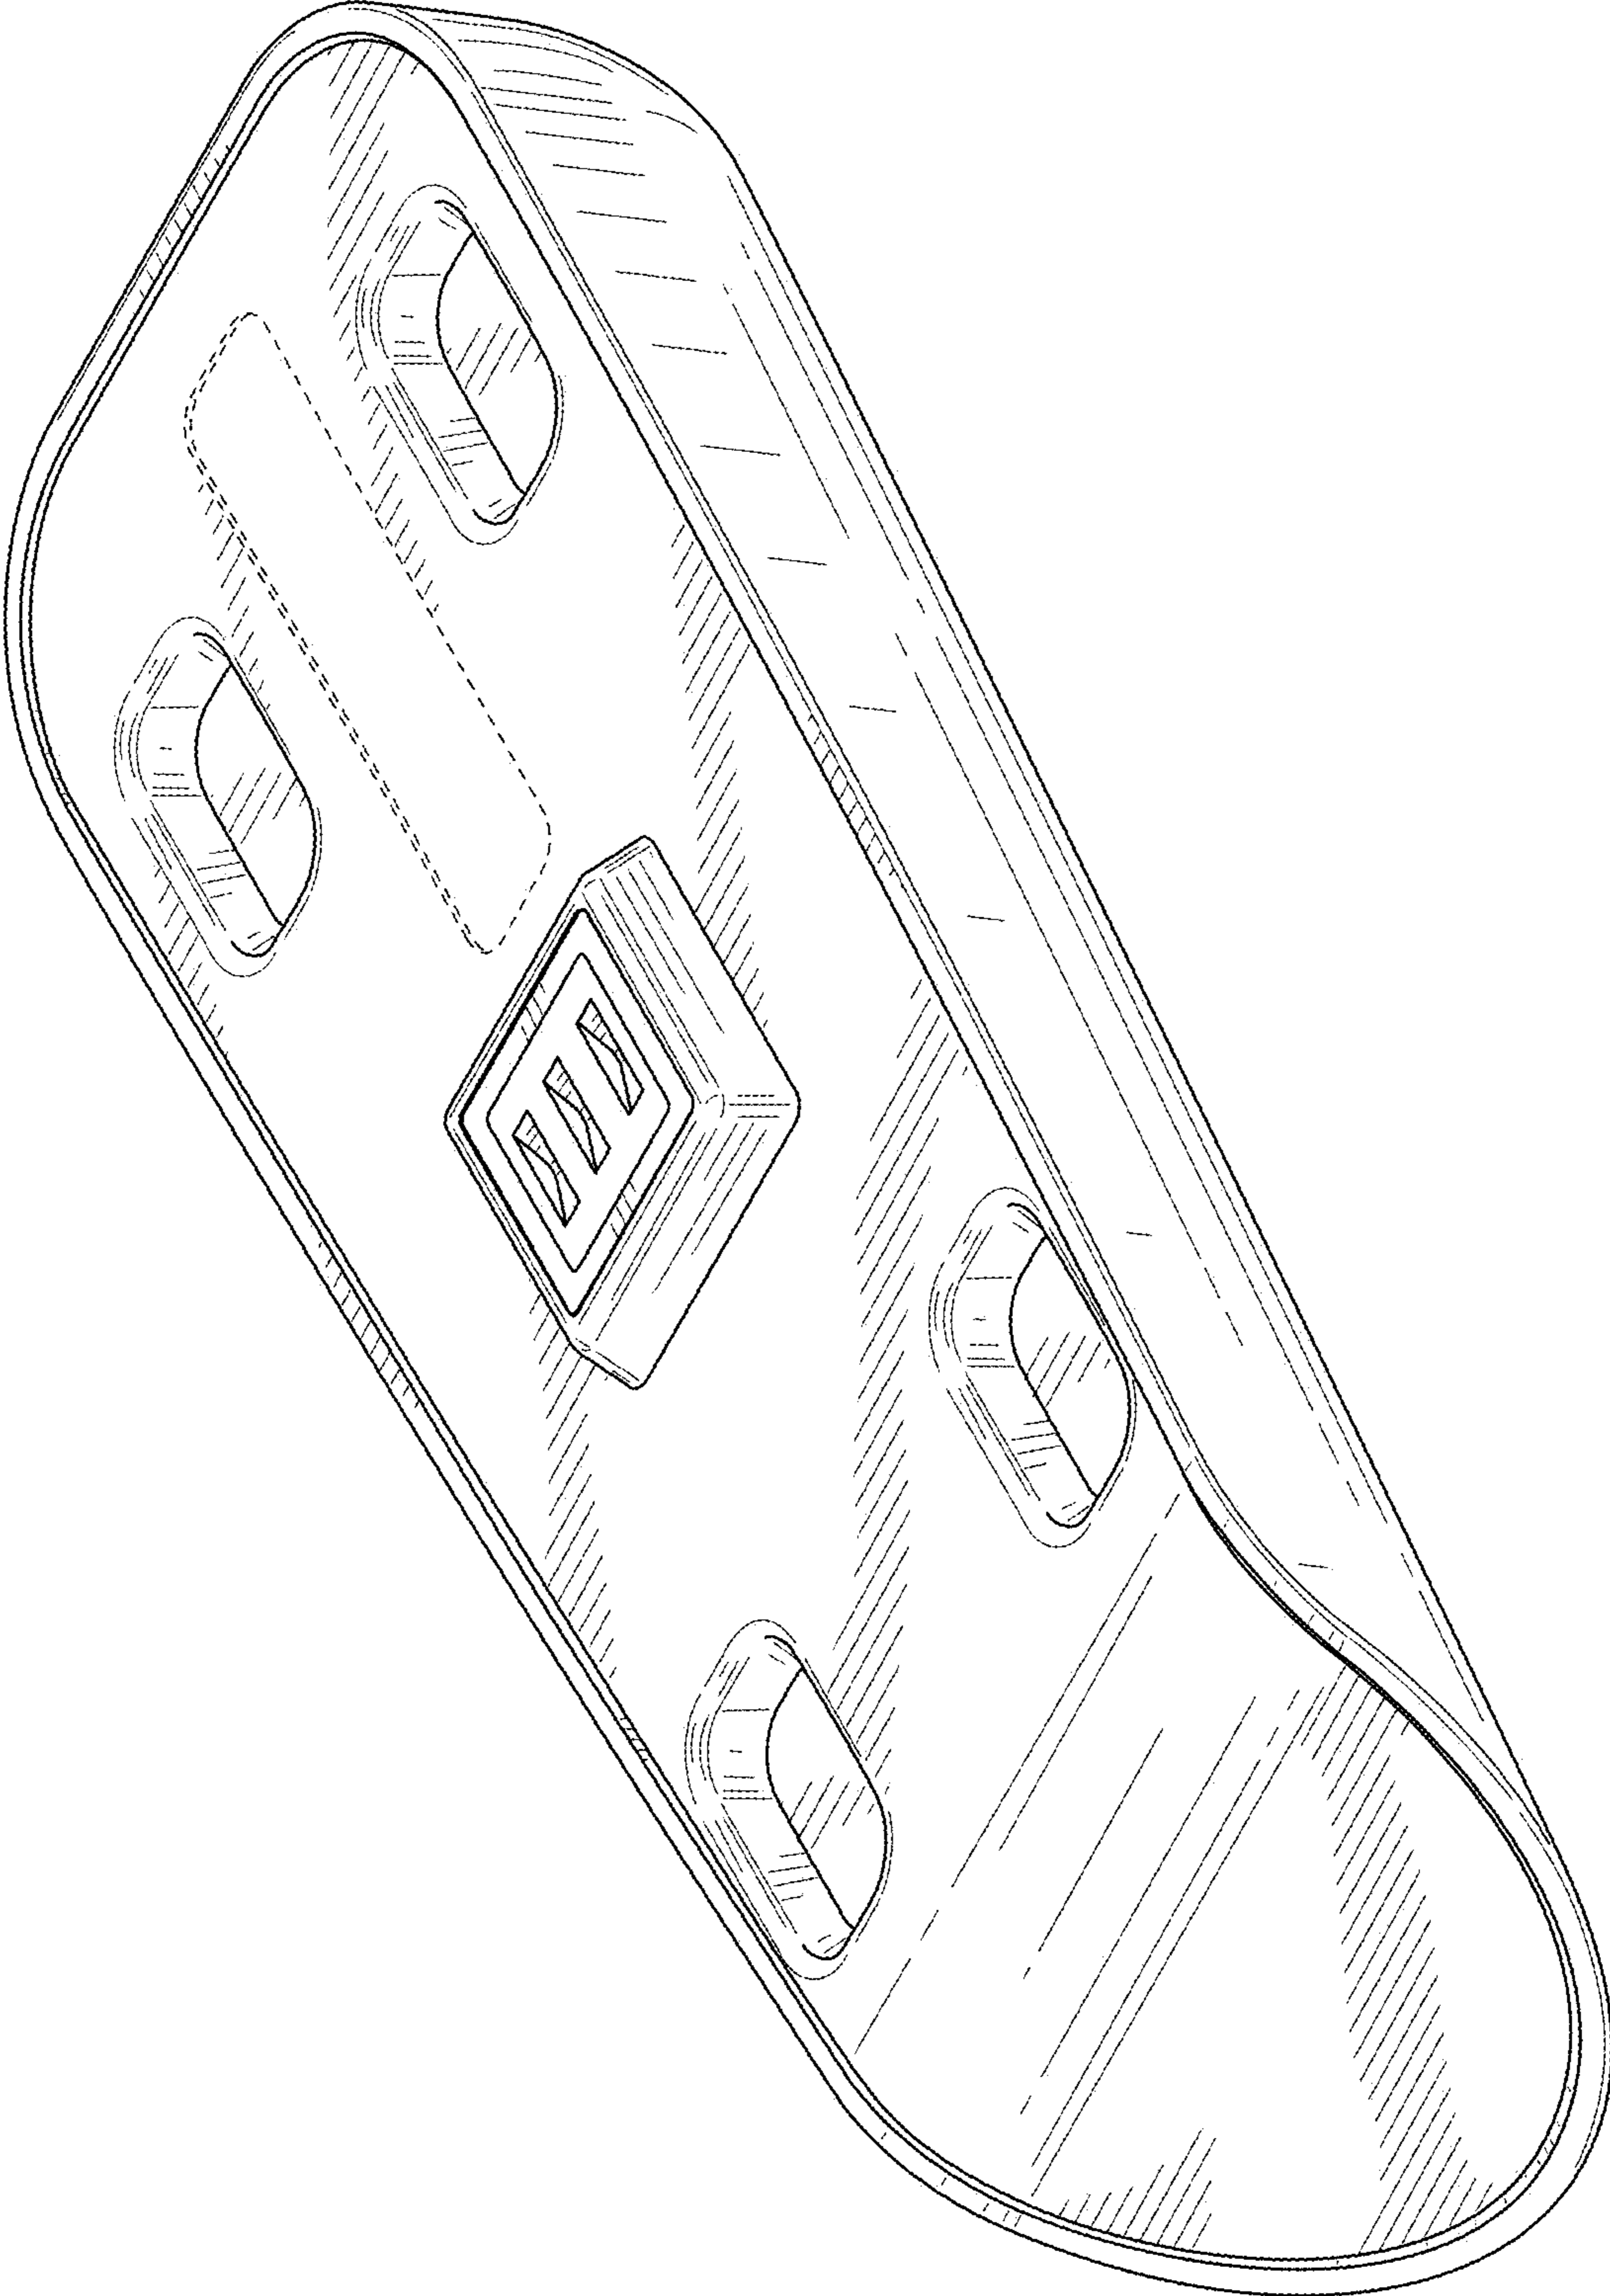


FIG. 1

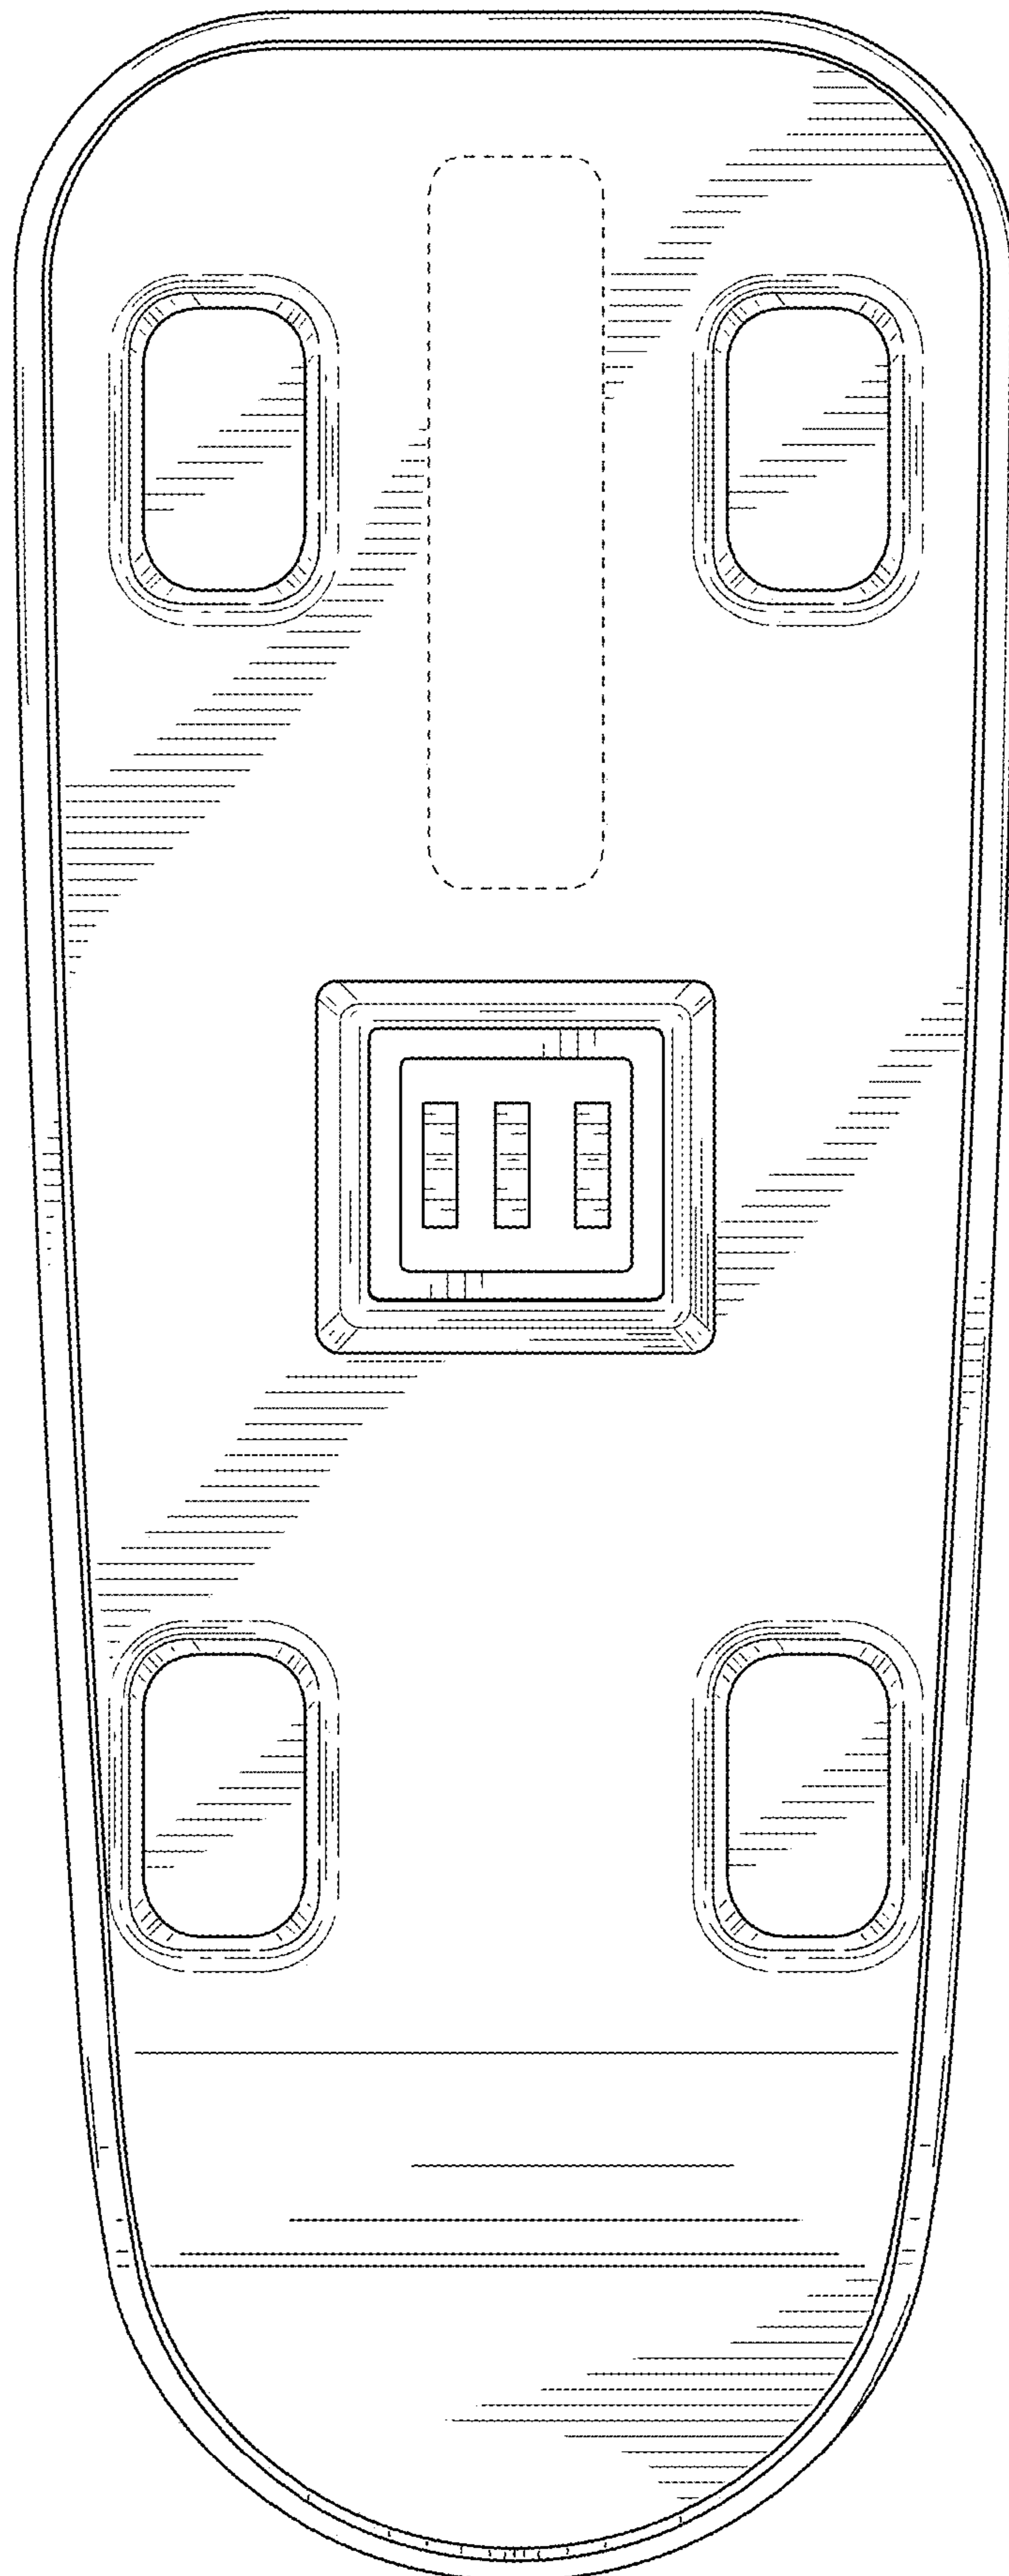


FIG. 2

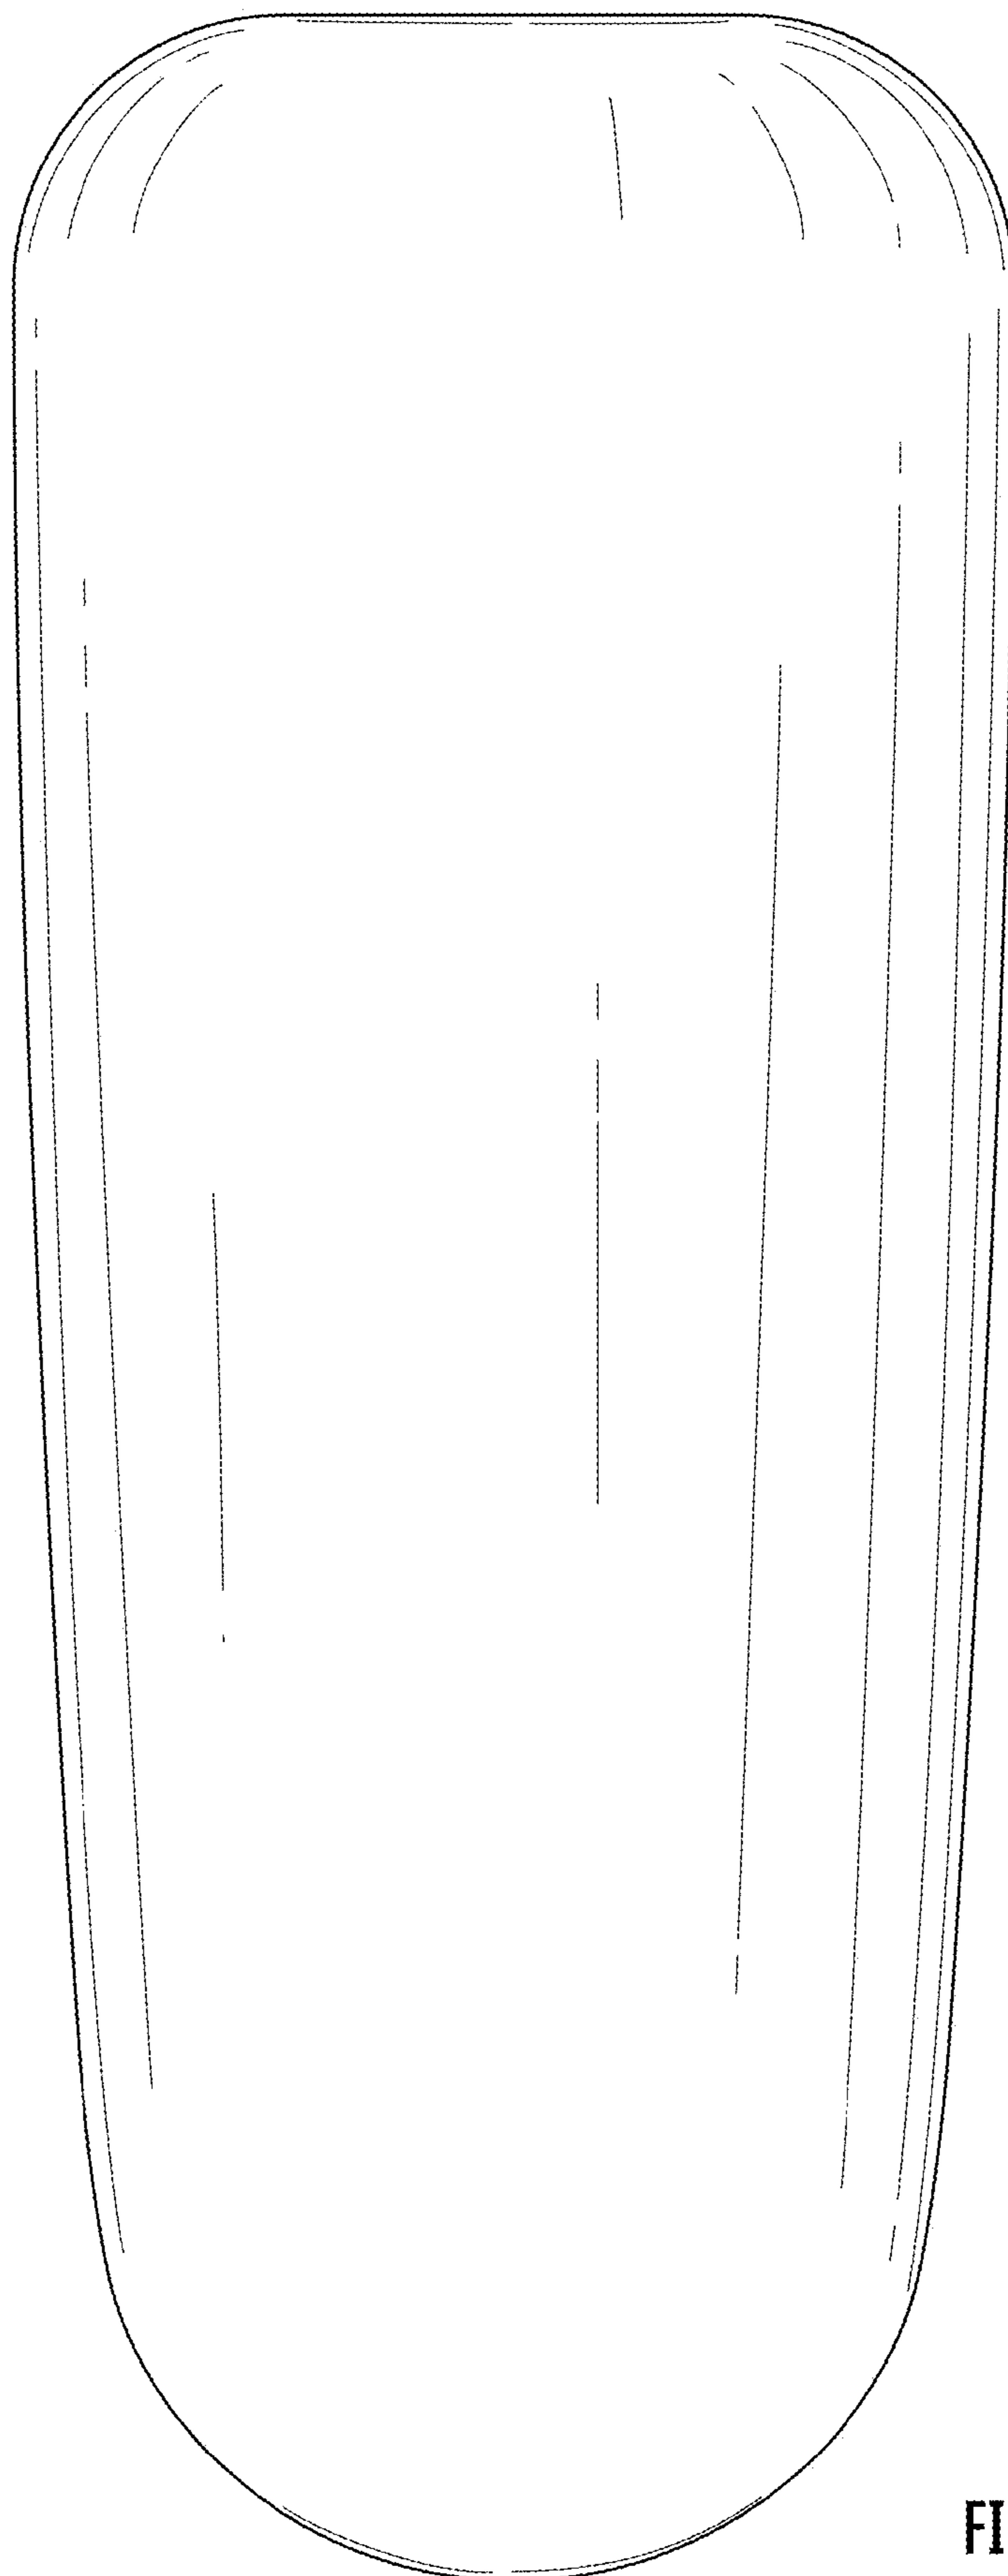


FIG. 3

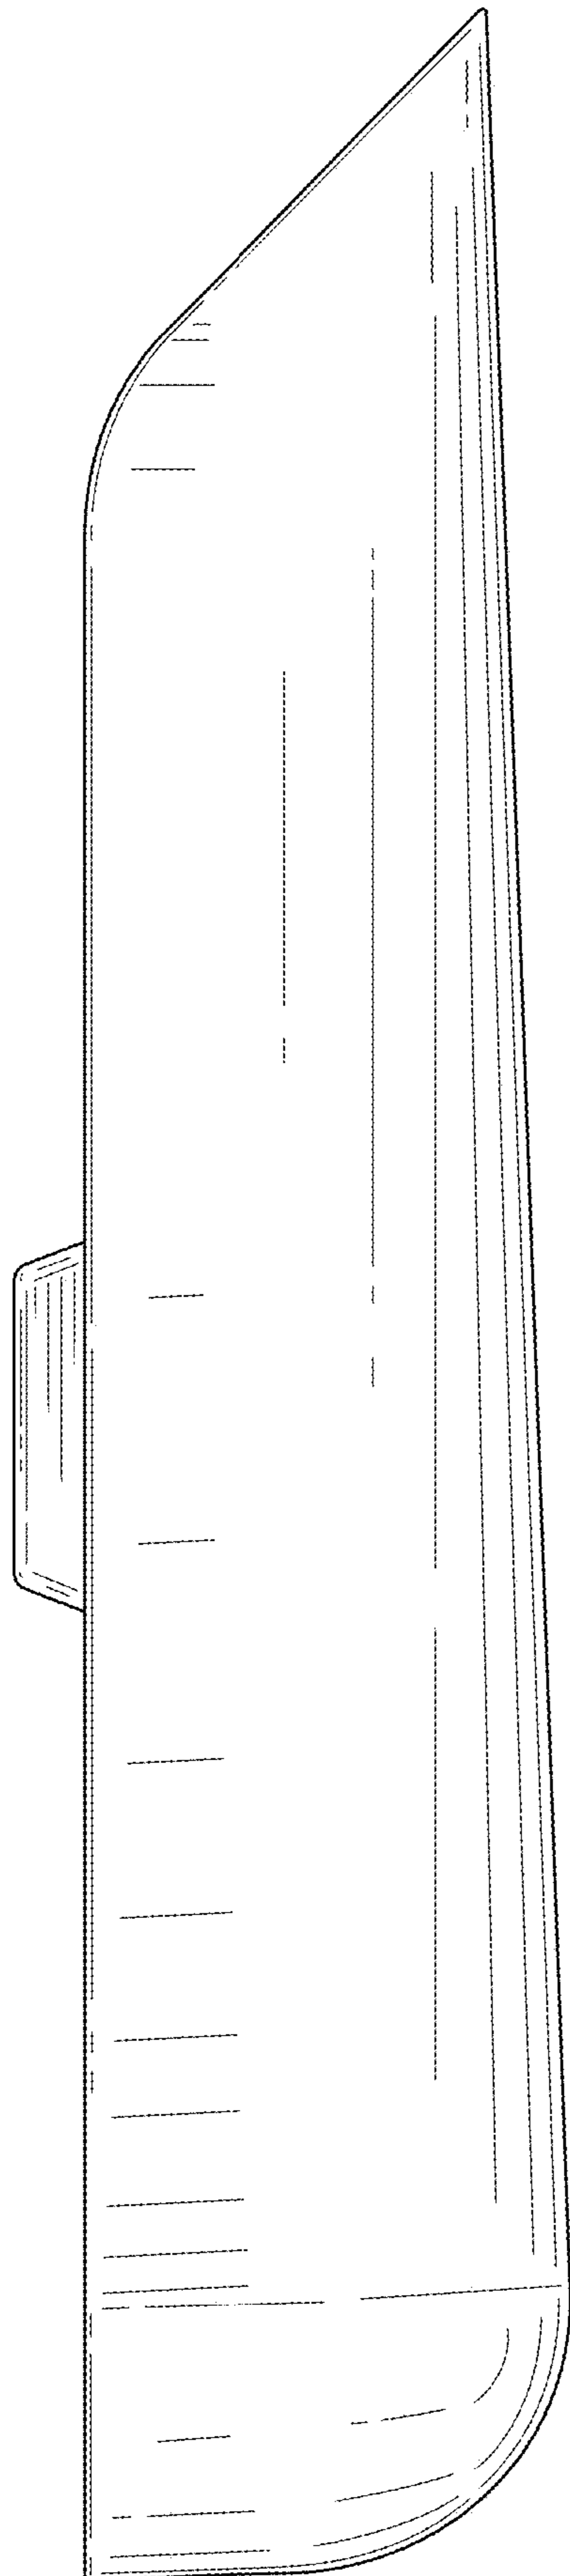


FIG. 4

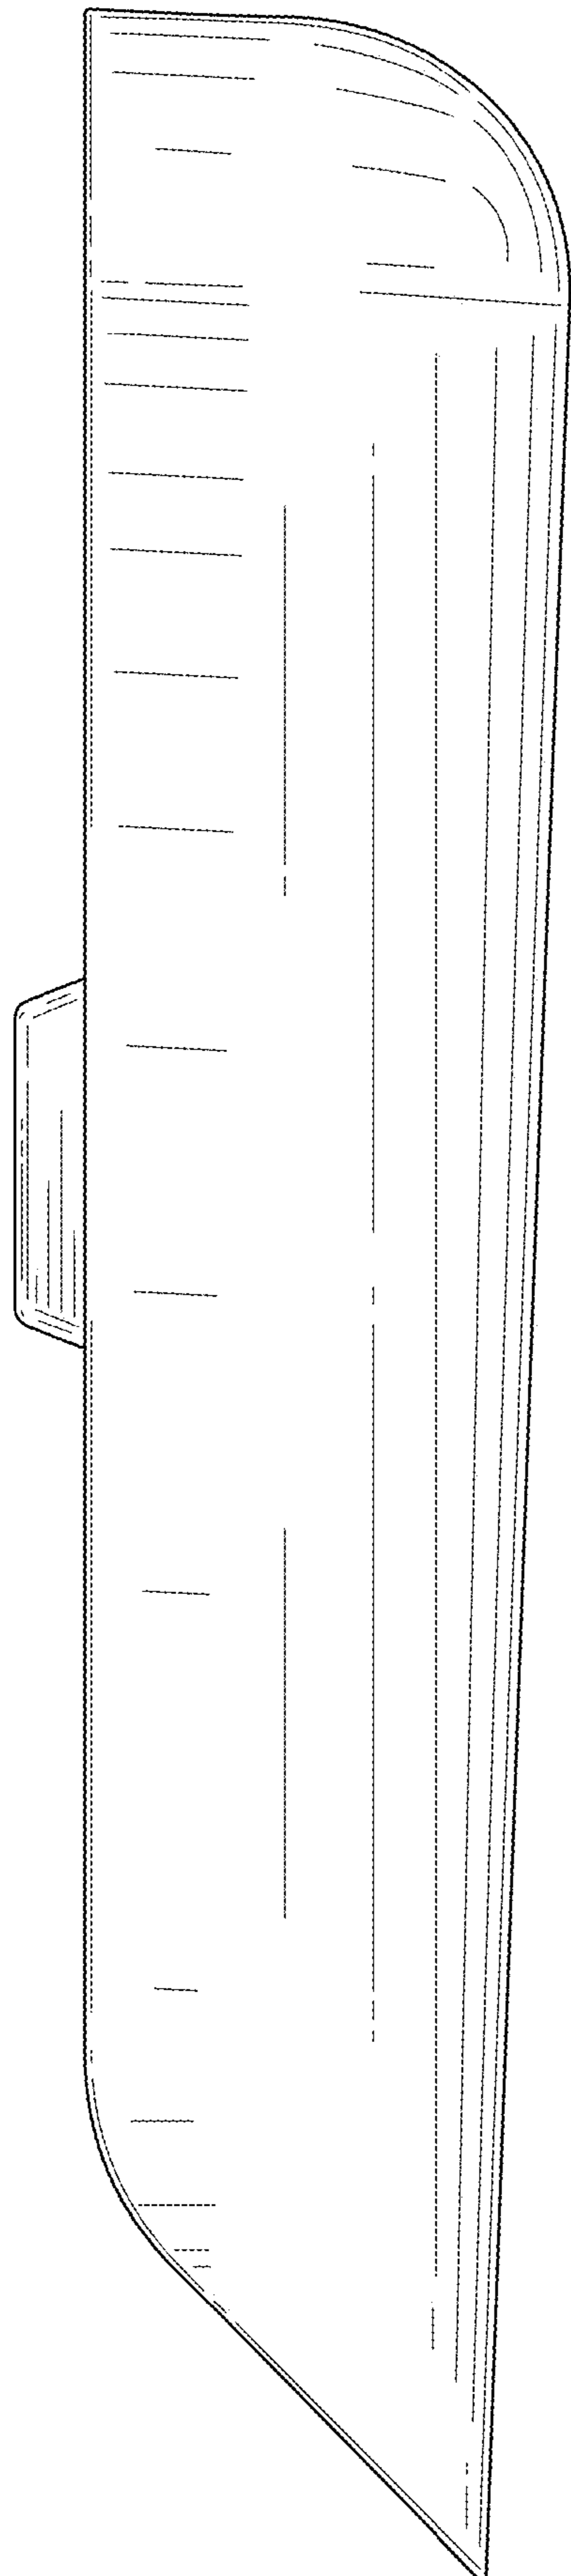


FIG. 5

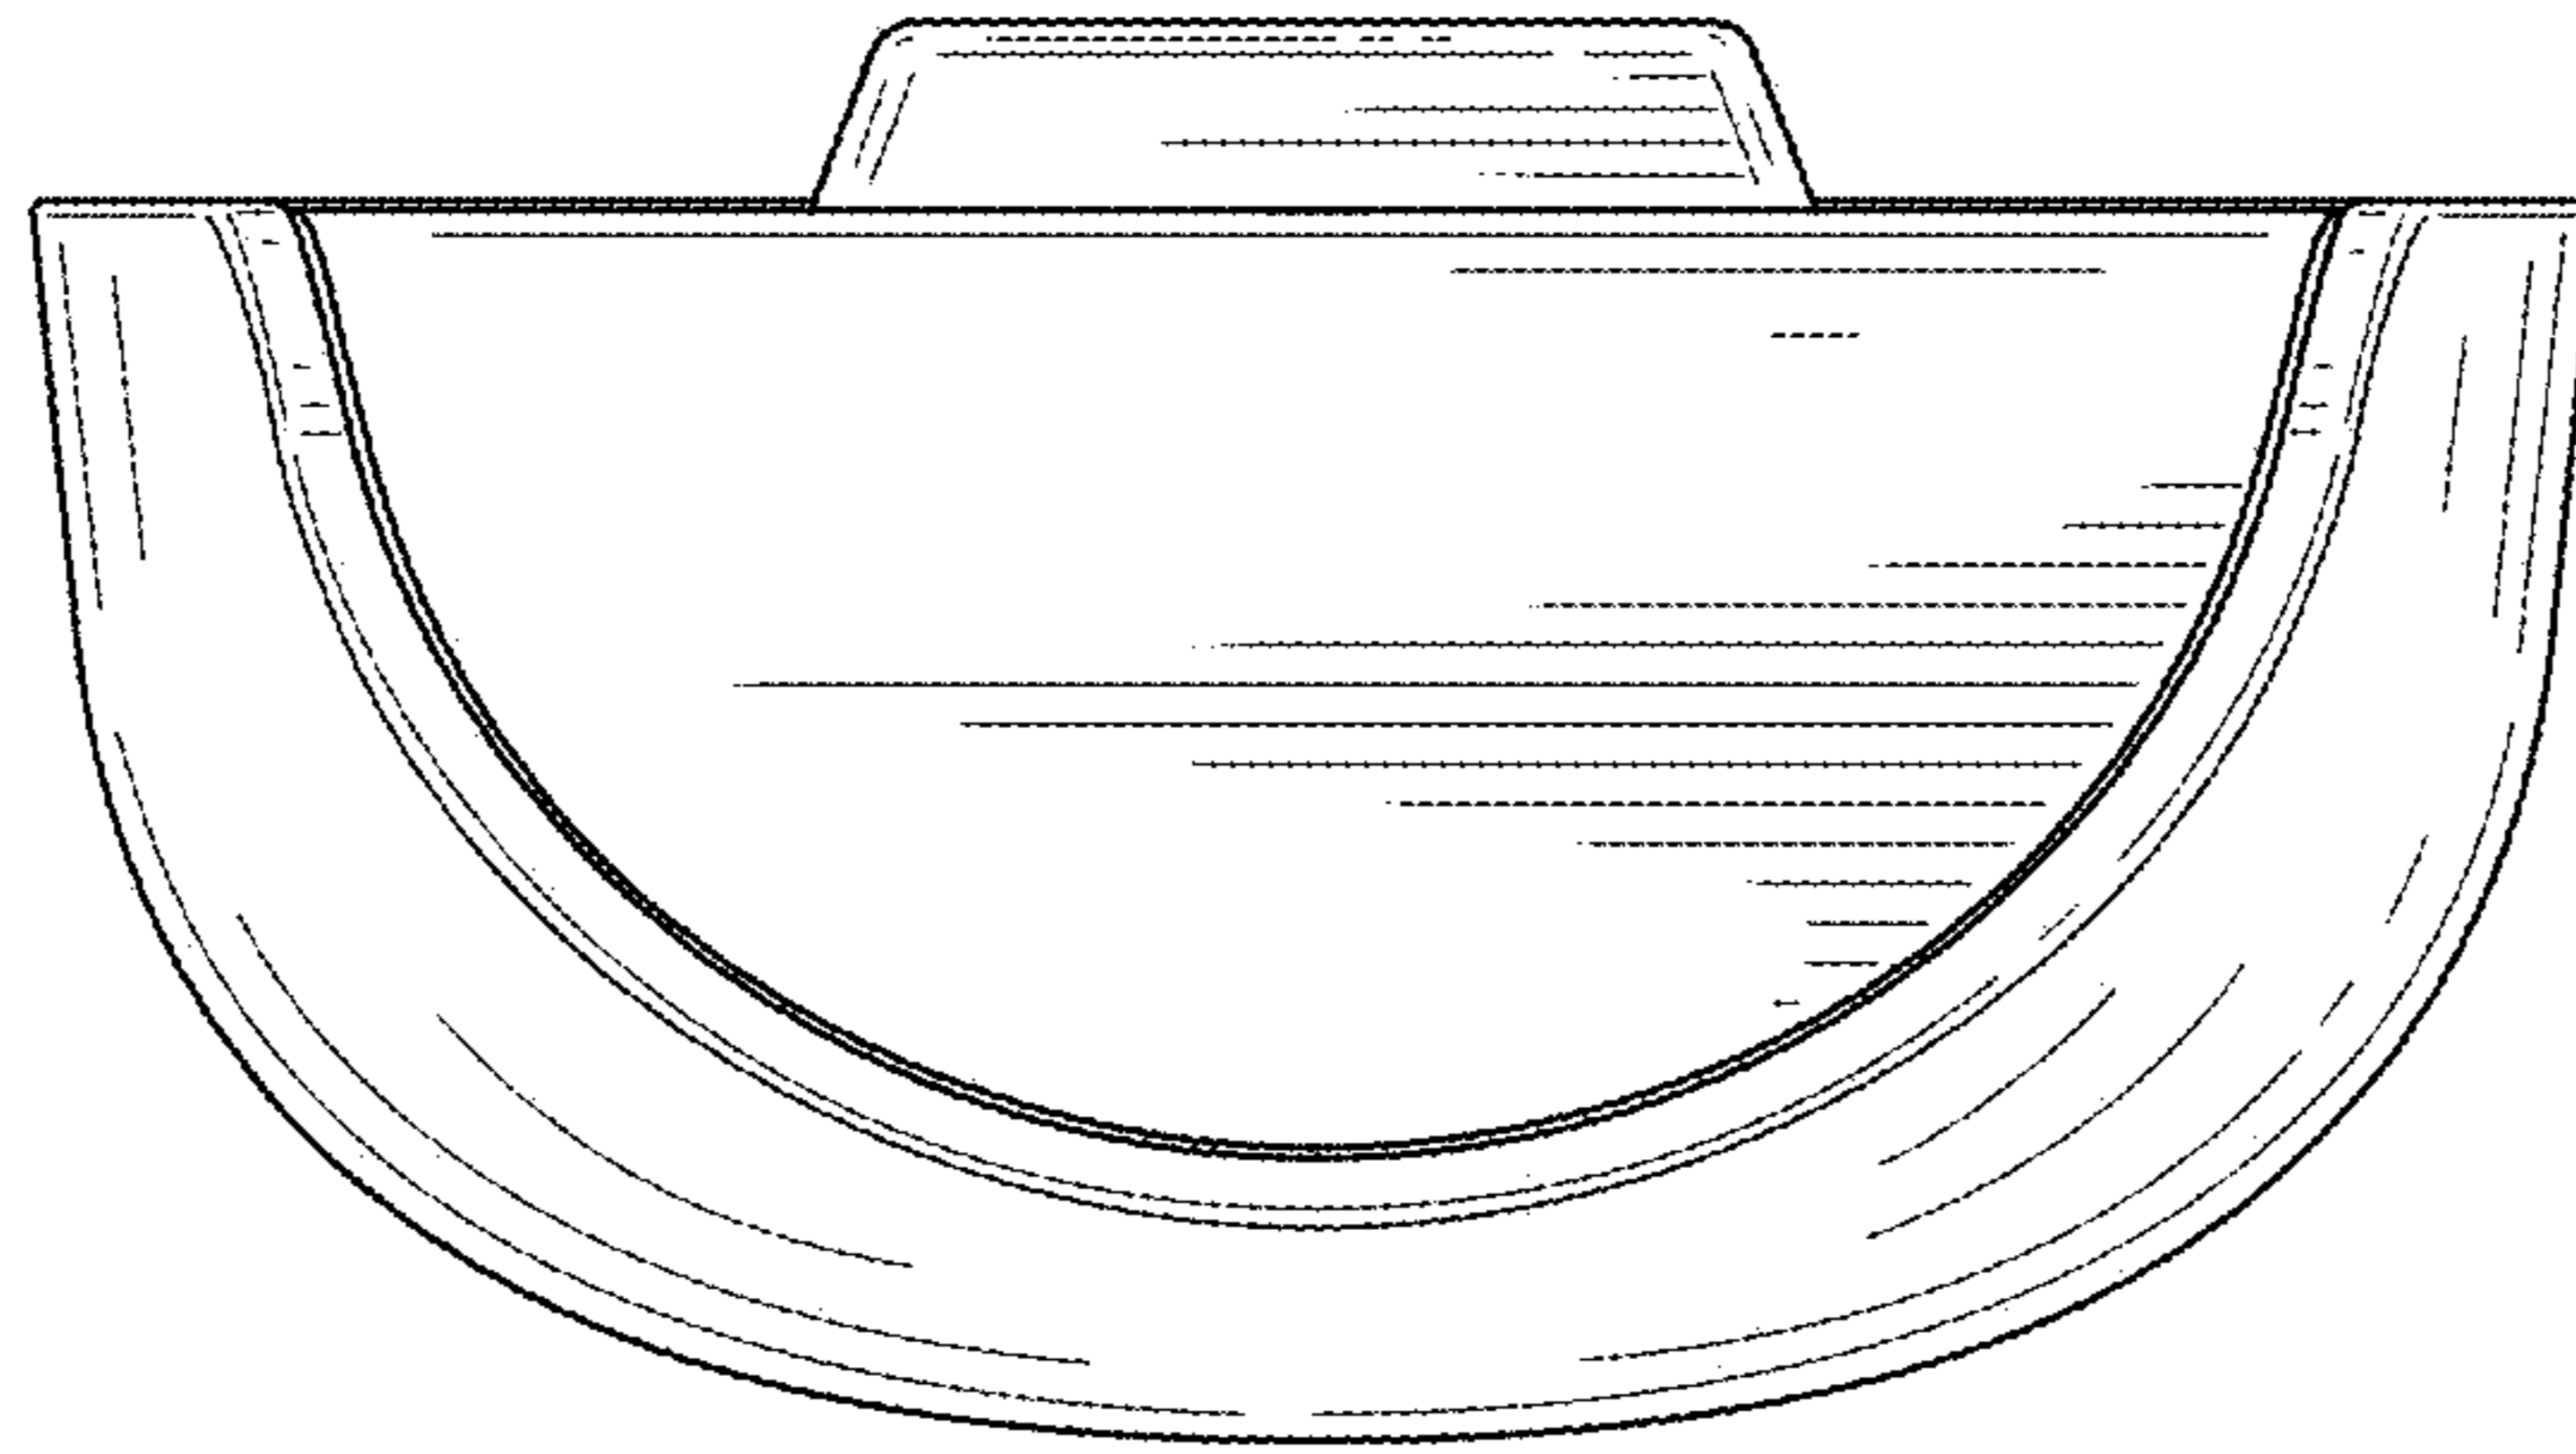


FIG. 6

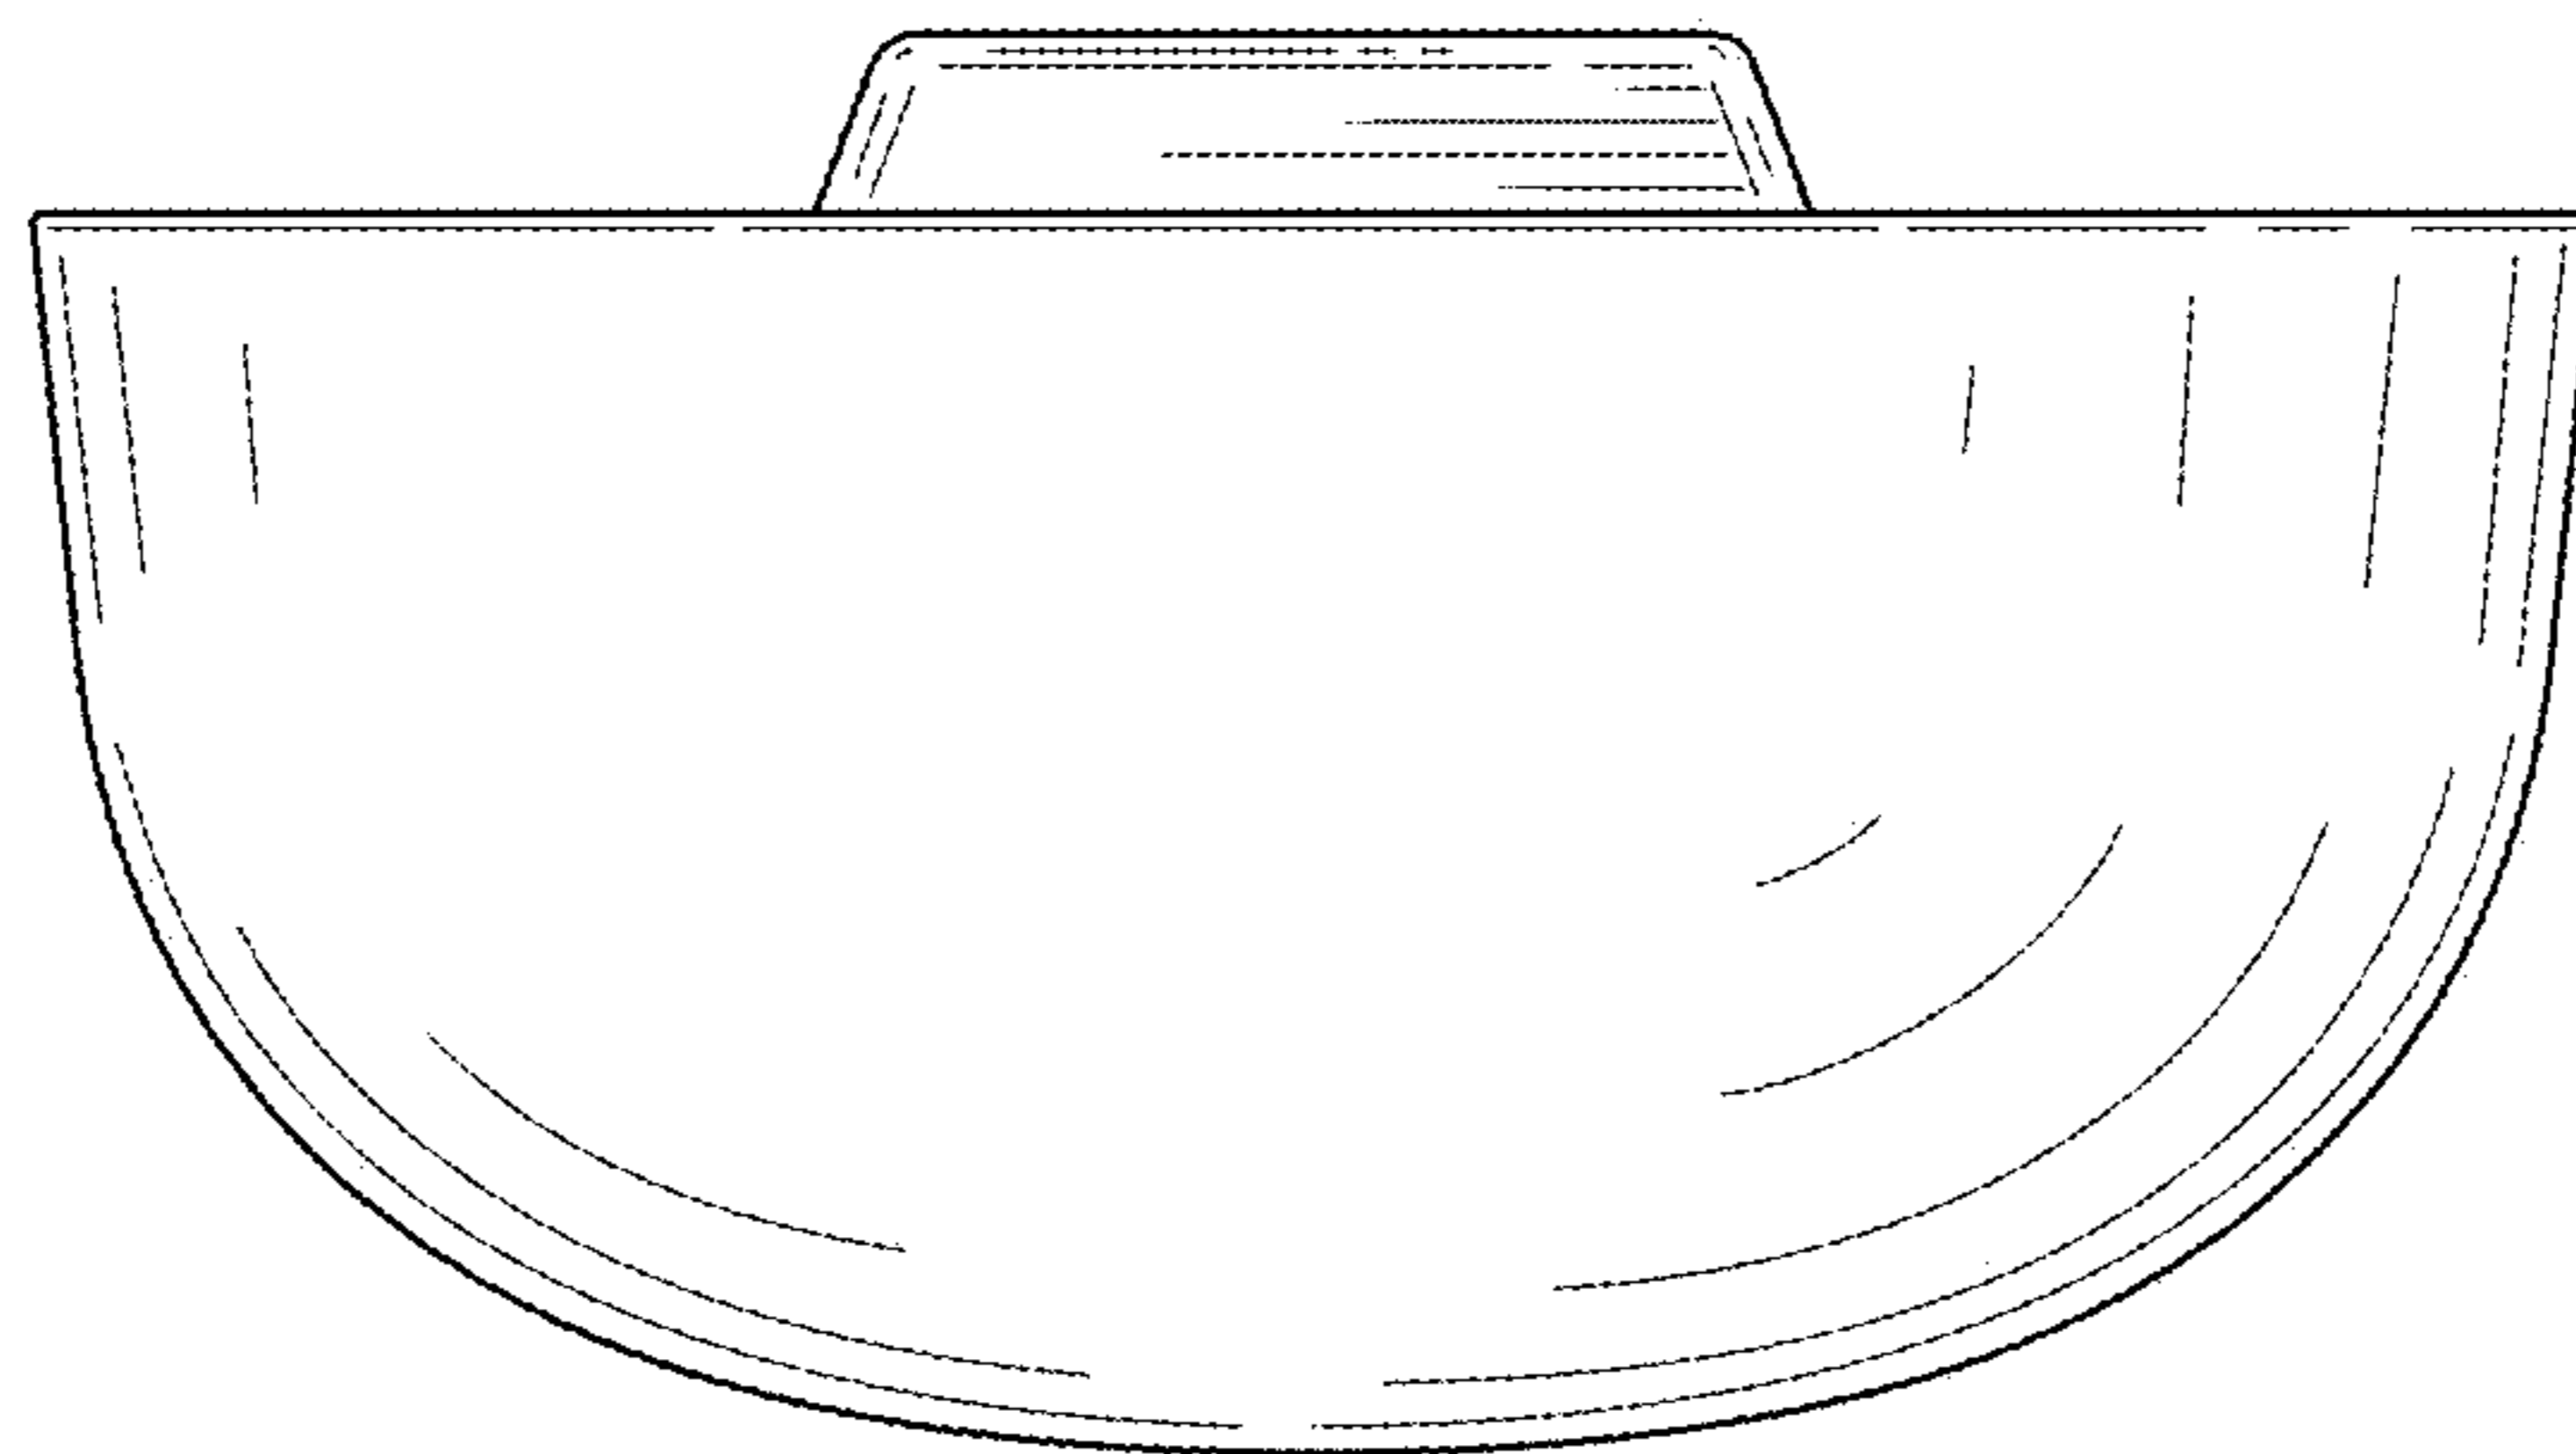


FIG. 7

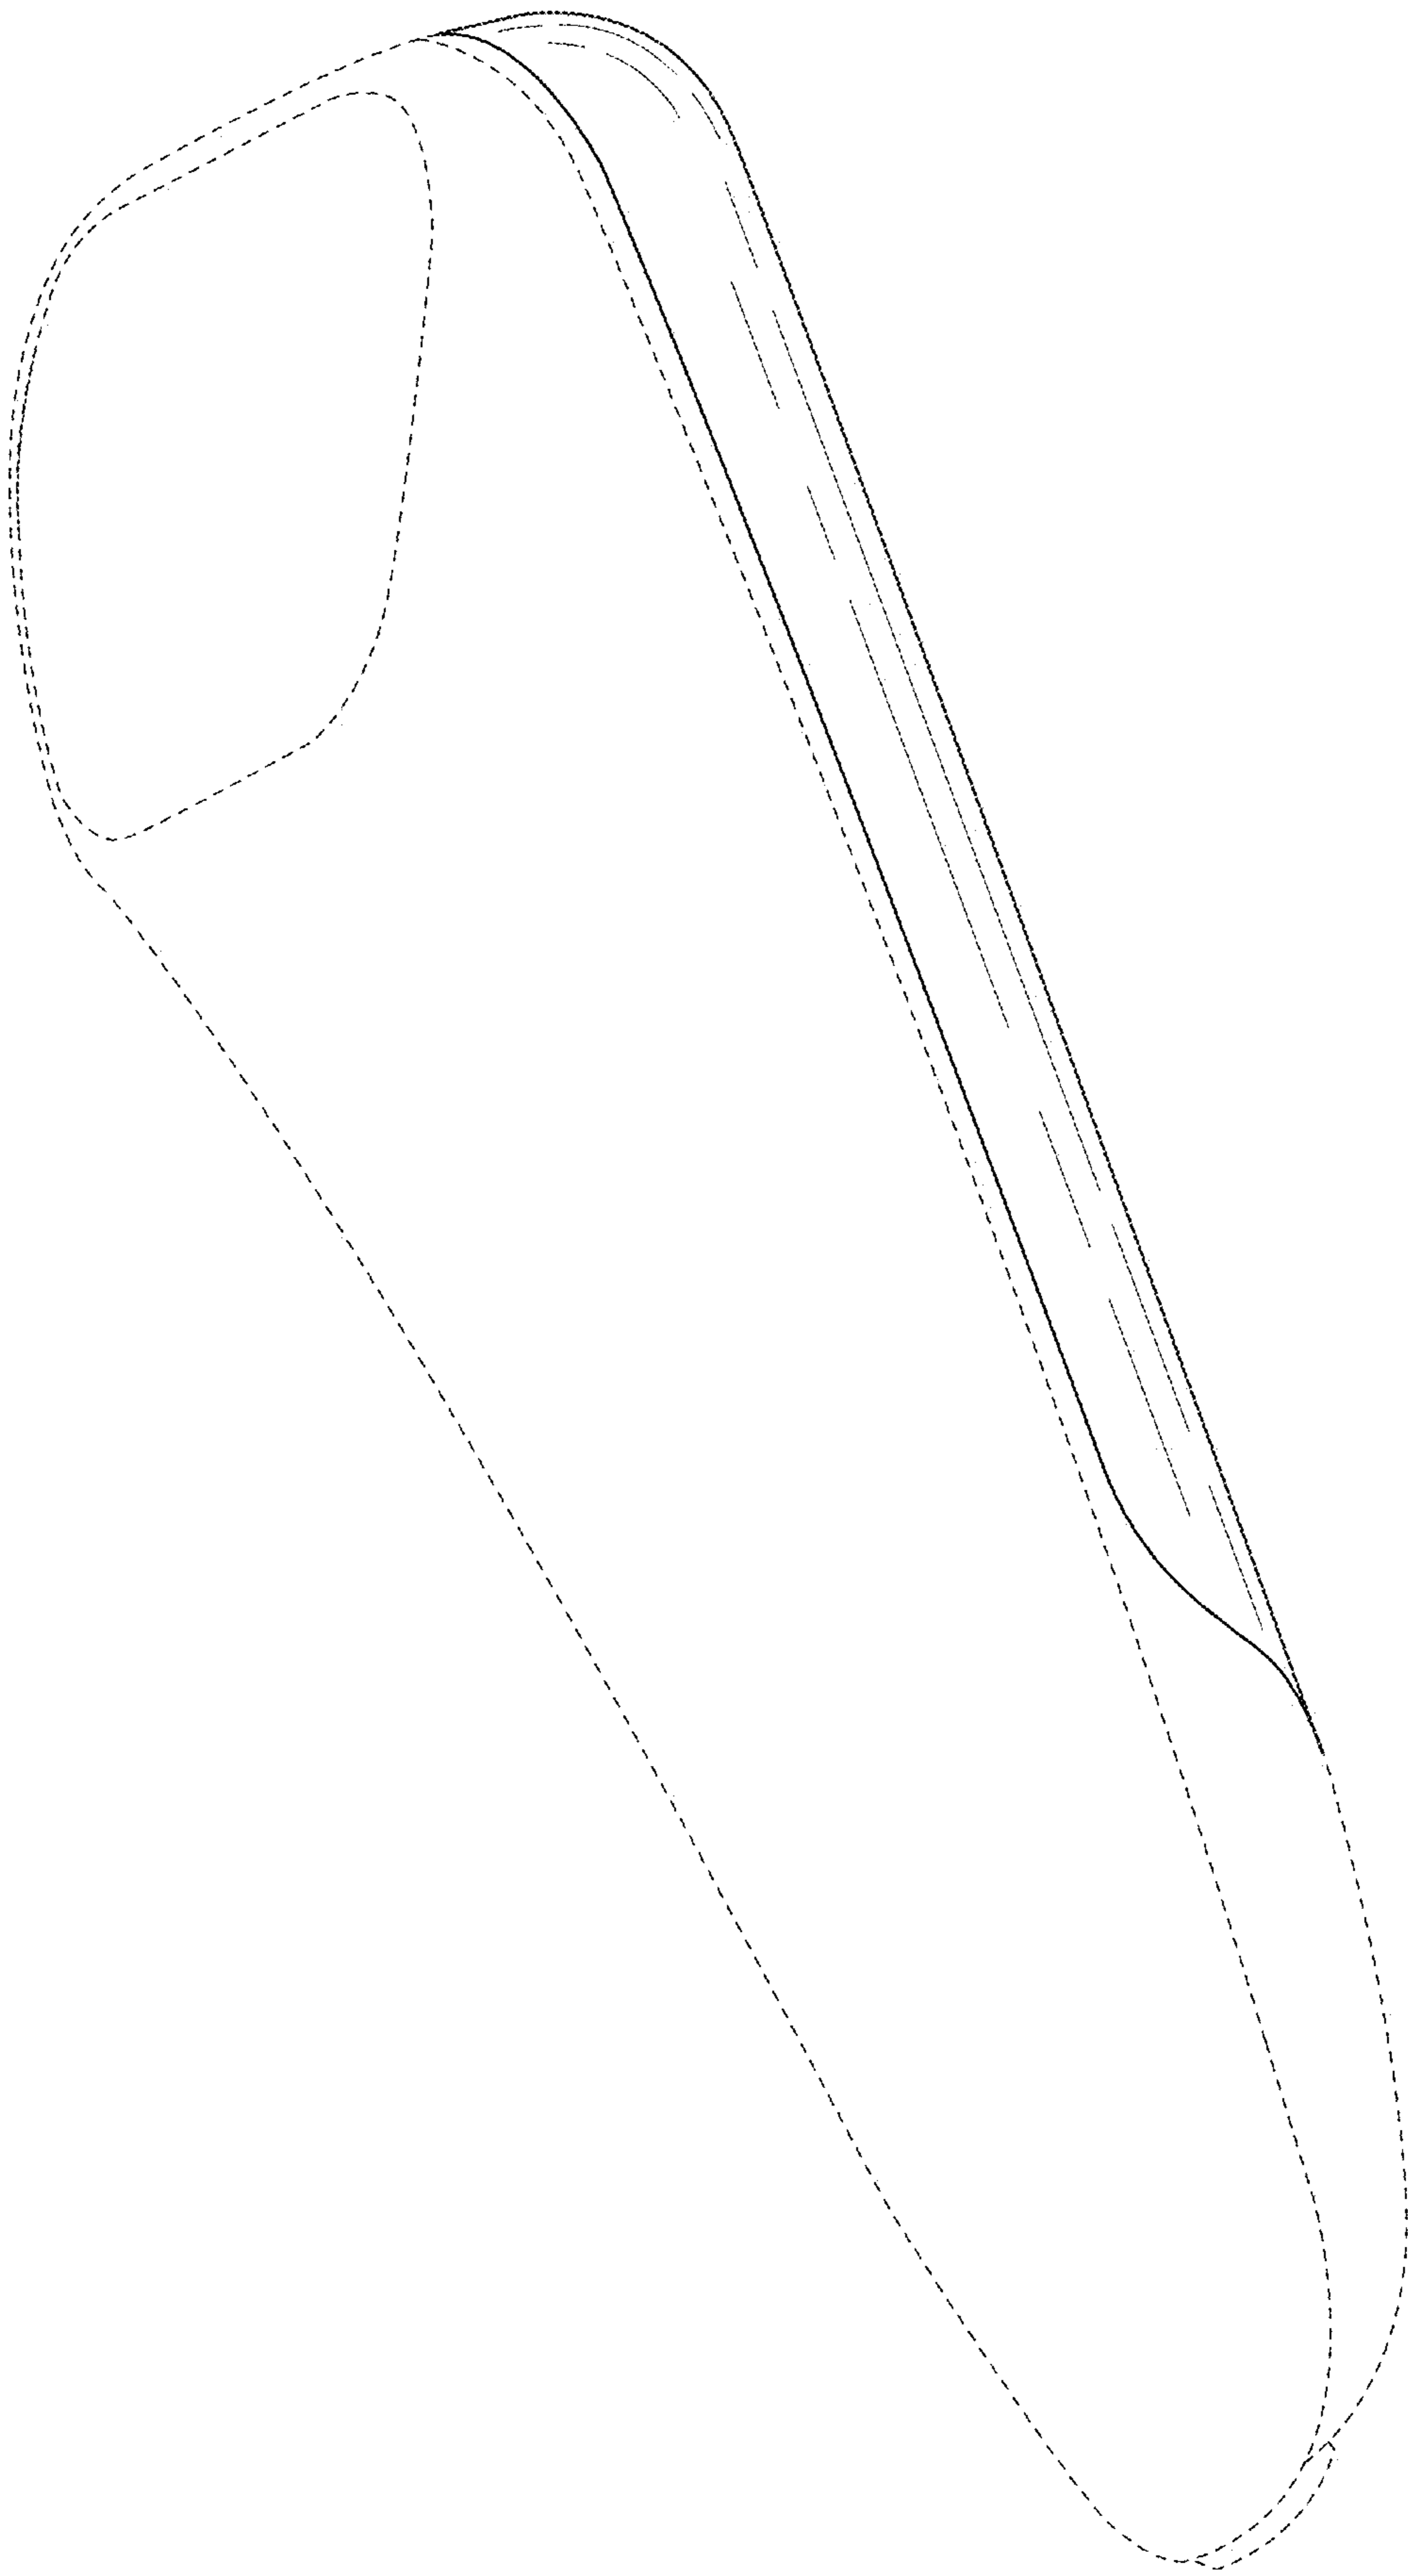


FIG. 8