



US00D950046S

(12) **United States Design Patent**
Black, III

(10) **Patent No.:** **US D950,046 S**

(45) **Date of Patent:** **** Apr. 26, 2022**

(54) **CANNULA RELEASE DEVICE**

(71) Applicant: **Norman M. Black, III**, Atlanta, GA
(US)

(72) Inventor: **Norman M. Black, III**, Atlanta, GA
(US)

(73) Assignee: **Black & Black Surgical, Inc.**, Tucker,
GA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/753,332**

(22) Filed: **Sep. 30, 2020**

Related U.S. Application Data

(63) Continuation of application No. 29/730,404, filed on
Apr. 3, 2020.

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/112; D24/127**

(58) **Field of Classification Search**
USPC D24/112, 129, 137, 138, 206, 108, 127;
D8/382; D13/133; 348/75; 600/131,
600/459, 132, 174, 461, 462; 604/523
CPC A61M 16/0465; A61M 16/0427; A61M
16/0488; A61M 16/08; A61M 16/0434;
A61M 2202/08; A61M 1/84; Y10S
604/902; A61B 17/320068; A61B
2017/32007
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,900,184 A * 8/1975 Burke A61M 39/286
251/6
- D243,635 S * 3/1977 Miller D24/129
- D283,641 S * 4/1986 Spetzler D24/129

- D353,198 S * 12/1994 Blasdell D24/129
- D371,340 S * 7/1996 Suzuki D13/123
- 5,651,773 A * 7/1997 Perry A61M 39/0247
604/174
- D415,102 S * 10/1999 Suzuki D13/133
- D456,356 S * 4/2002 Togashi D13/133
- 6,394,973 B1 * 5/2002 Cucin A61B 17/32002
604/22
- D461,771 S * 8/2002 Zhao D13/133
- D481,125 S * 10/2003 Hayamizu D24/129

(Continued)

OTHER PUBLICATIONS

[Microaire®—Type Power Cannula], available onblackandblacksurgical.com, Jun. 2020 [online], [site visited Nov. 26, 2021], Internet URL: <https://blackandblacksurgical.s3.amazonaws.com/PI+sheets/25-3024_MicroAirePI_Sheet-FINAL-R2.pdf>. (Year: 2020).*

(Continued)

Primary Examiner — Jonathan J Han

Assistant Examiner — Amanda J Berlinski

(74) *Attorney, Agent, or Firm* — Walter A. Rodgers



(57) **CLAIM**

The ornamental design for a cannula release device, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a cannula release device showing my new design;
FIG. 2 is a front elevation view thereof, the rear being a mirror image thereof;
FIG. 3 is a top plan view thereof;
FIG. 4 is a left-side elevation view thereof;
FIG. 5 is a right-side elevation view thereof;
FIG. 6 is a bottom plan thereof; and,
FIG. 7 is a bottom perspective view thereof.
The broken lines depict features of the cannula release device that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

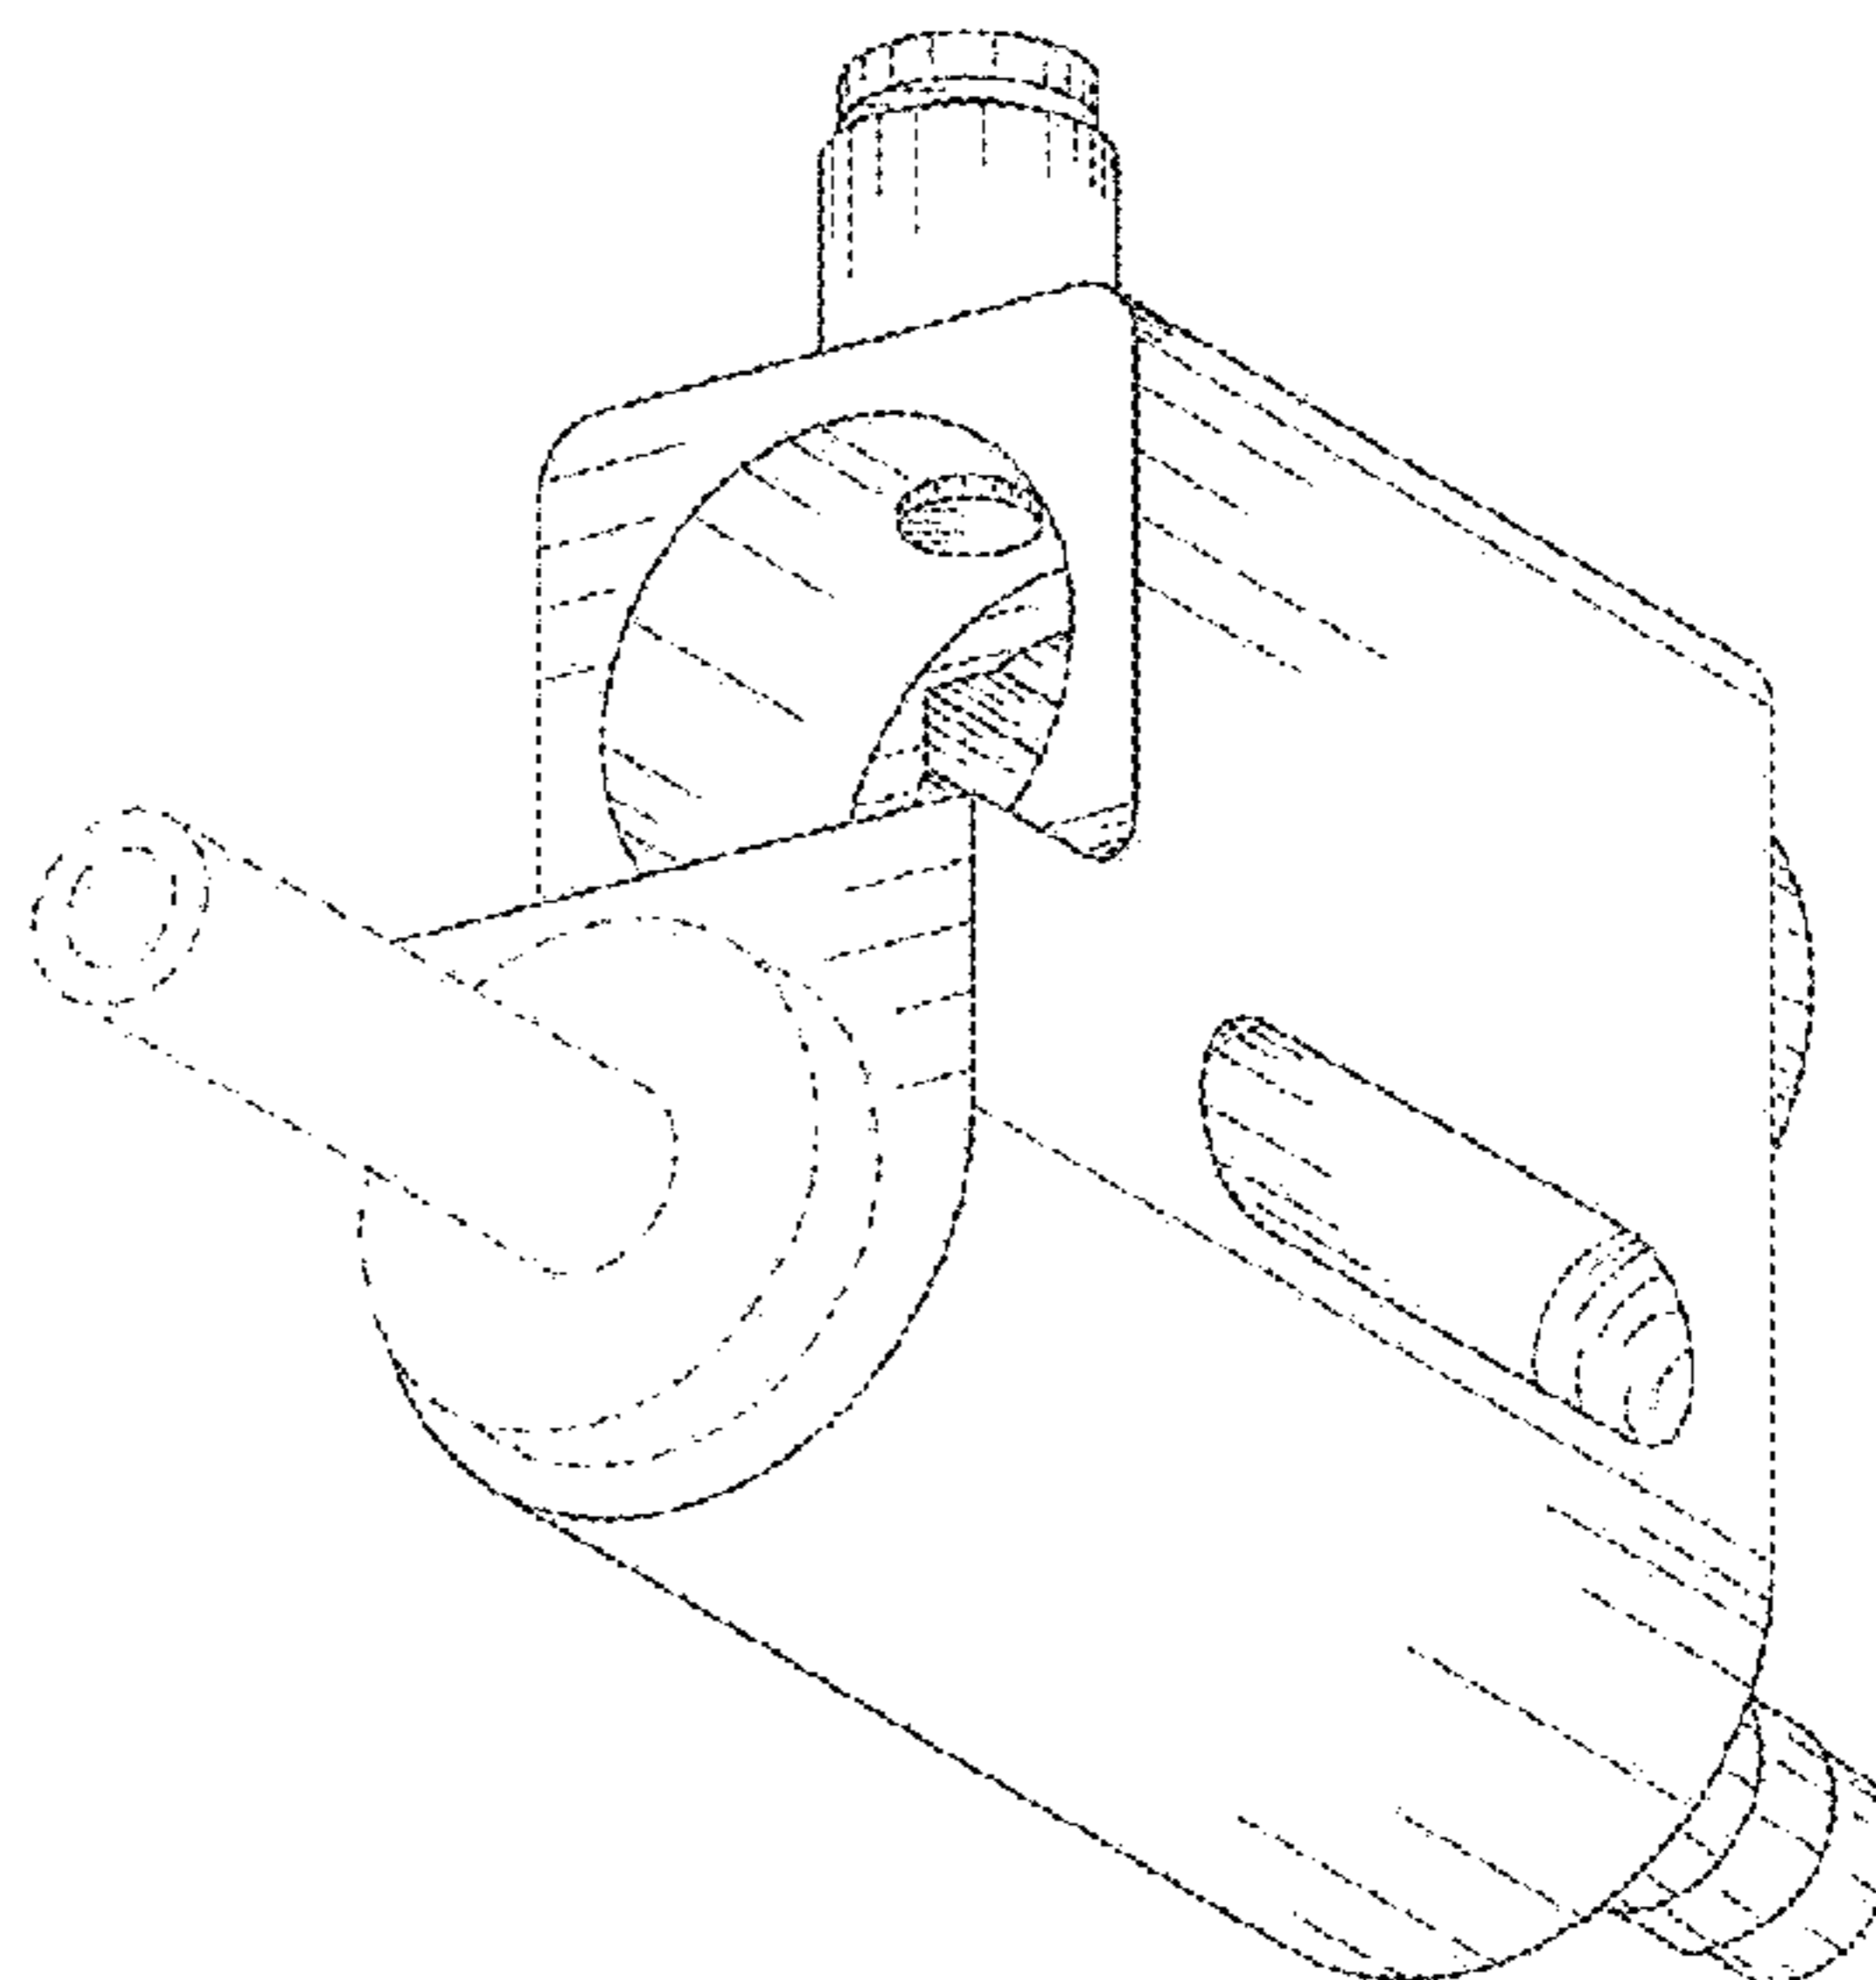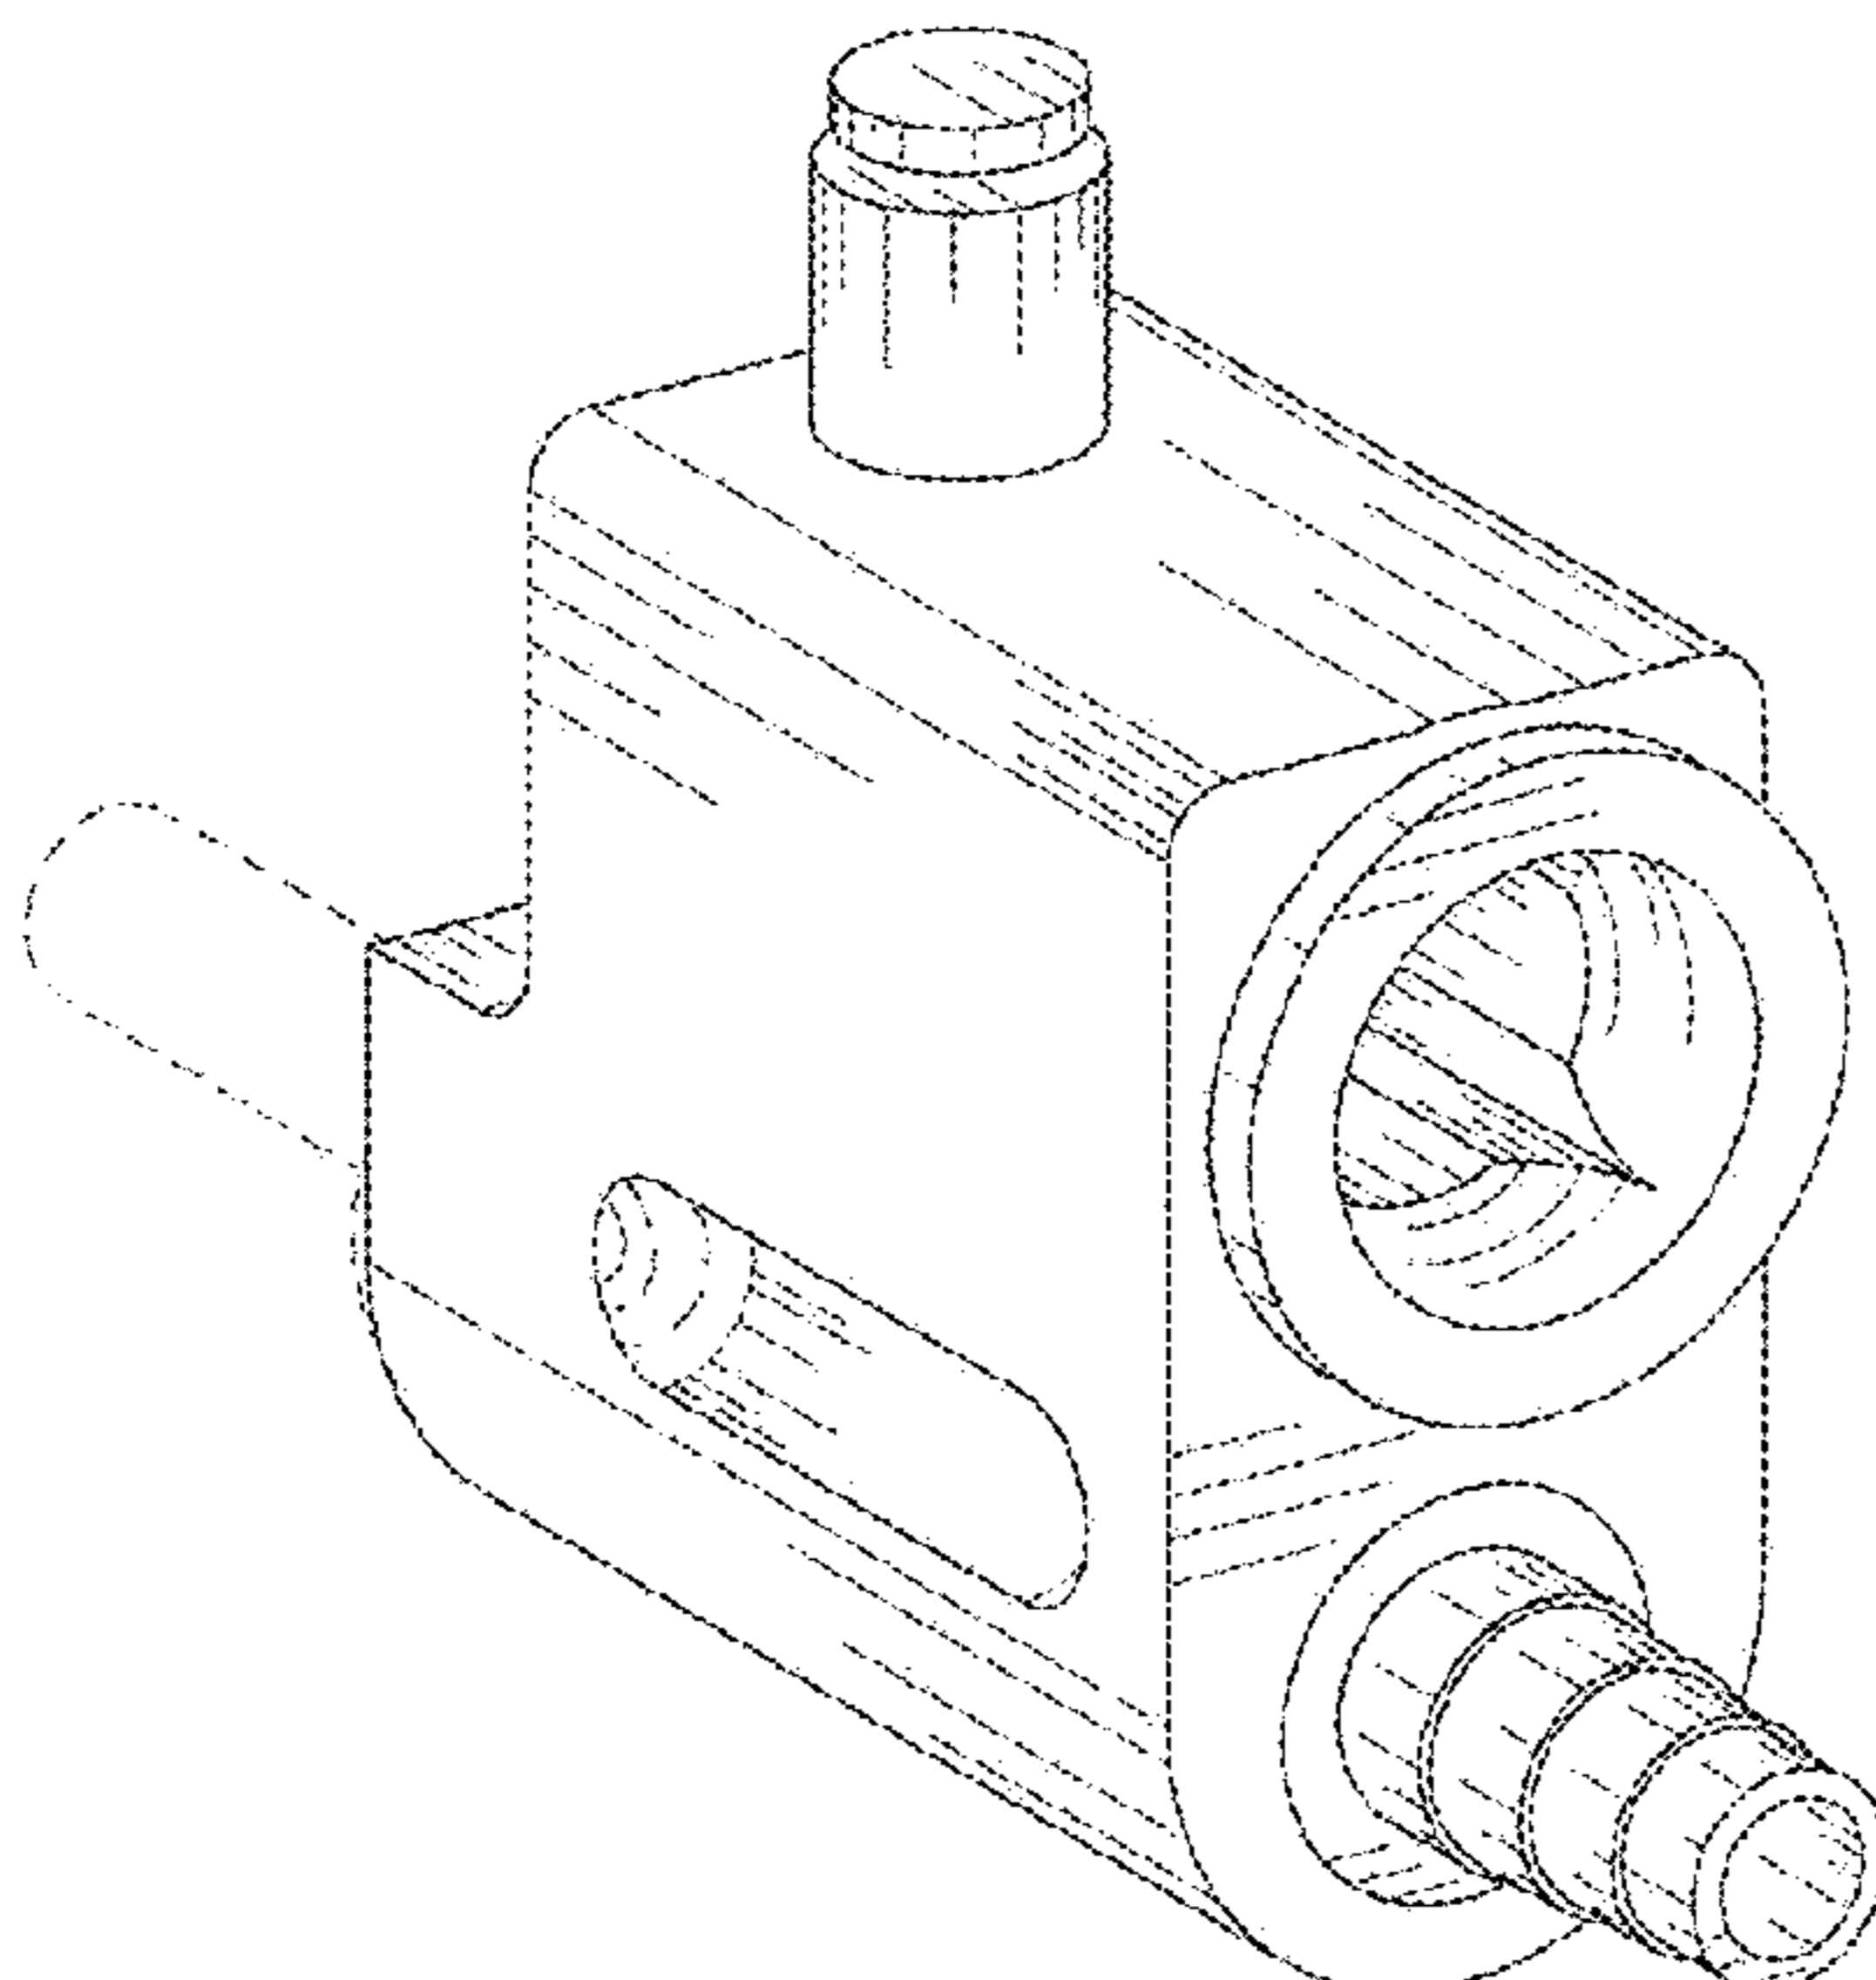

(56)

References Cited

U.S. PATENT DOCUMENTS

D482,657 S * 11/2003 Lai D13/133
 D497,428 S * 10/2004 Hayamizu D24/129
 D534,655 S * 1/2007 Iranyi D24/138
 D546,946 S * 7/2007 Blake D24/129
 D553,083 S * 10/2007 Han D13/133
 D559,193 S * 1/2008 Stavoe D13/133
 D596,569 S * 7/2009 Lin D13/133
 D614,769 S * 4/2010 Vogel D24/138
 D616,821 S * 6/2010 The D13/133
 D619,709 S * 7/2010 Scholly A61B 17/32002
 D24/138
 D678,512 S * 3/2013 Bow D24/112
 D721,036 S * 1/2015 Kreitzer D13/133
 D722,156 S * 2/2015 Wiegel D24/112
 D781,236 S * 3/2017 Esses D13/144
 D834,186 S * 11/2018 Lombardi, III H04N 5/23203
 D24/129
 D850,615 S * 6/2019 Chung A61M 25/0147
 D24/129
 D884,892 S * 5/2020 Hulford D24/145
 D928,711 S * 8/2021 Kunzendorf D13/133
 2003/0125681 A1 * 7/2003 Fard A61M 1/84
 604/353
 2005/0203485 A1 * 9/2005 Lee A61M 25/0147
 604/523
 2010/0128114 A1 * 5/2010 Cheung H04N 5/23203
 348/65

2011/0065991 A1 * 3/2011 Sarvazyan A61B 1/31
 600/131
 2015/0085093 A1 * 3/2015 Heni A61B 1/04
 348/65
 2020/0230340 A1 * 7/2020 Cheyne A61M 16/0488
 2020/0323550 A1 * 10/2020 Khouri A61B 17/32002

OTHER PUBLICATIONS

Liposales [@liposales], “Make the most out of your power cannulas with the Liposales’ Power Cannula Adapter! These high-quality reusable adapters are suited for aspiration with your Microaire Handle, with a power cannula end for a more extensive selection of cannulas. The power cannula compatibility gives you anesthesia access to areas of the body far away from the entry site without the need for additional incisions . . . ” Facebook.com, Published: [Oct. 30, 2020], Site Visited: [Nov. 26, 2021], URL: <<https://www.facebook.com/pg/liposales/posts/>>. (Year: 2020).*
 [Comparison: MicroAire VS Vibrasat Power Liposuction Units Cannulas], YouTube.com, Posted Jan. 16, 2020 [online], [Site Visited Nov. 26, 2021], URL: <<https://www.youtube.com/watch?v=COgRf1Ed5PE>>. (Year: 2020).*
 [MicroAire PAL—Power-Assisted Liposuction], YouTube.com, Posted Jul. 13, 2016 [online], [Site Visited Nov. 26, 2021], URL: <<https://www.youtube.com/watch?v=ESKV5iUySUo>>. (Year: 2016).*

* cited by examiner

Fig 1

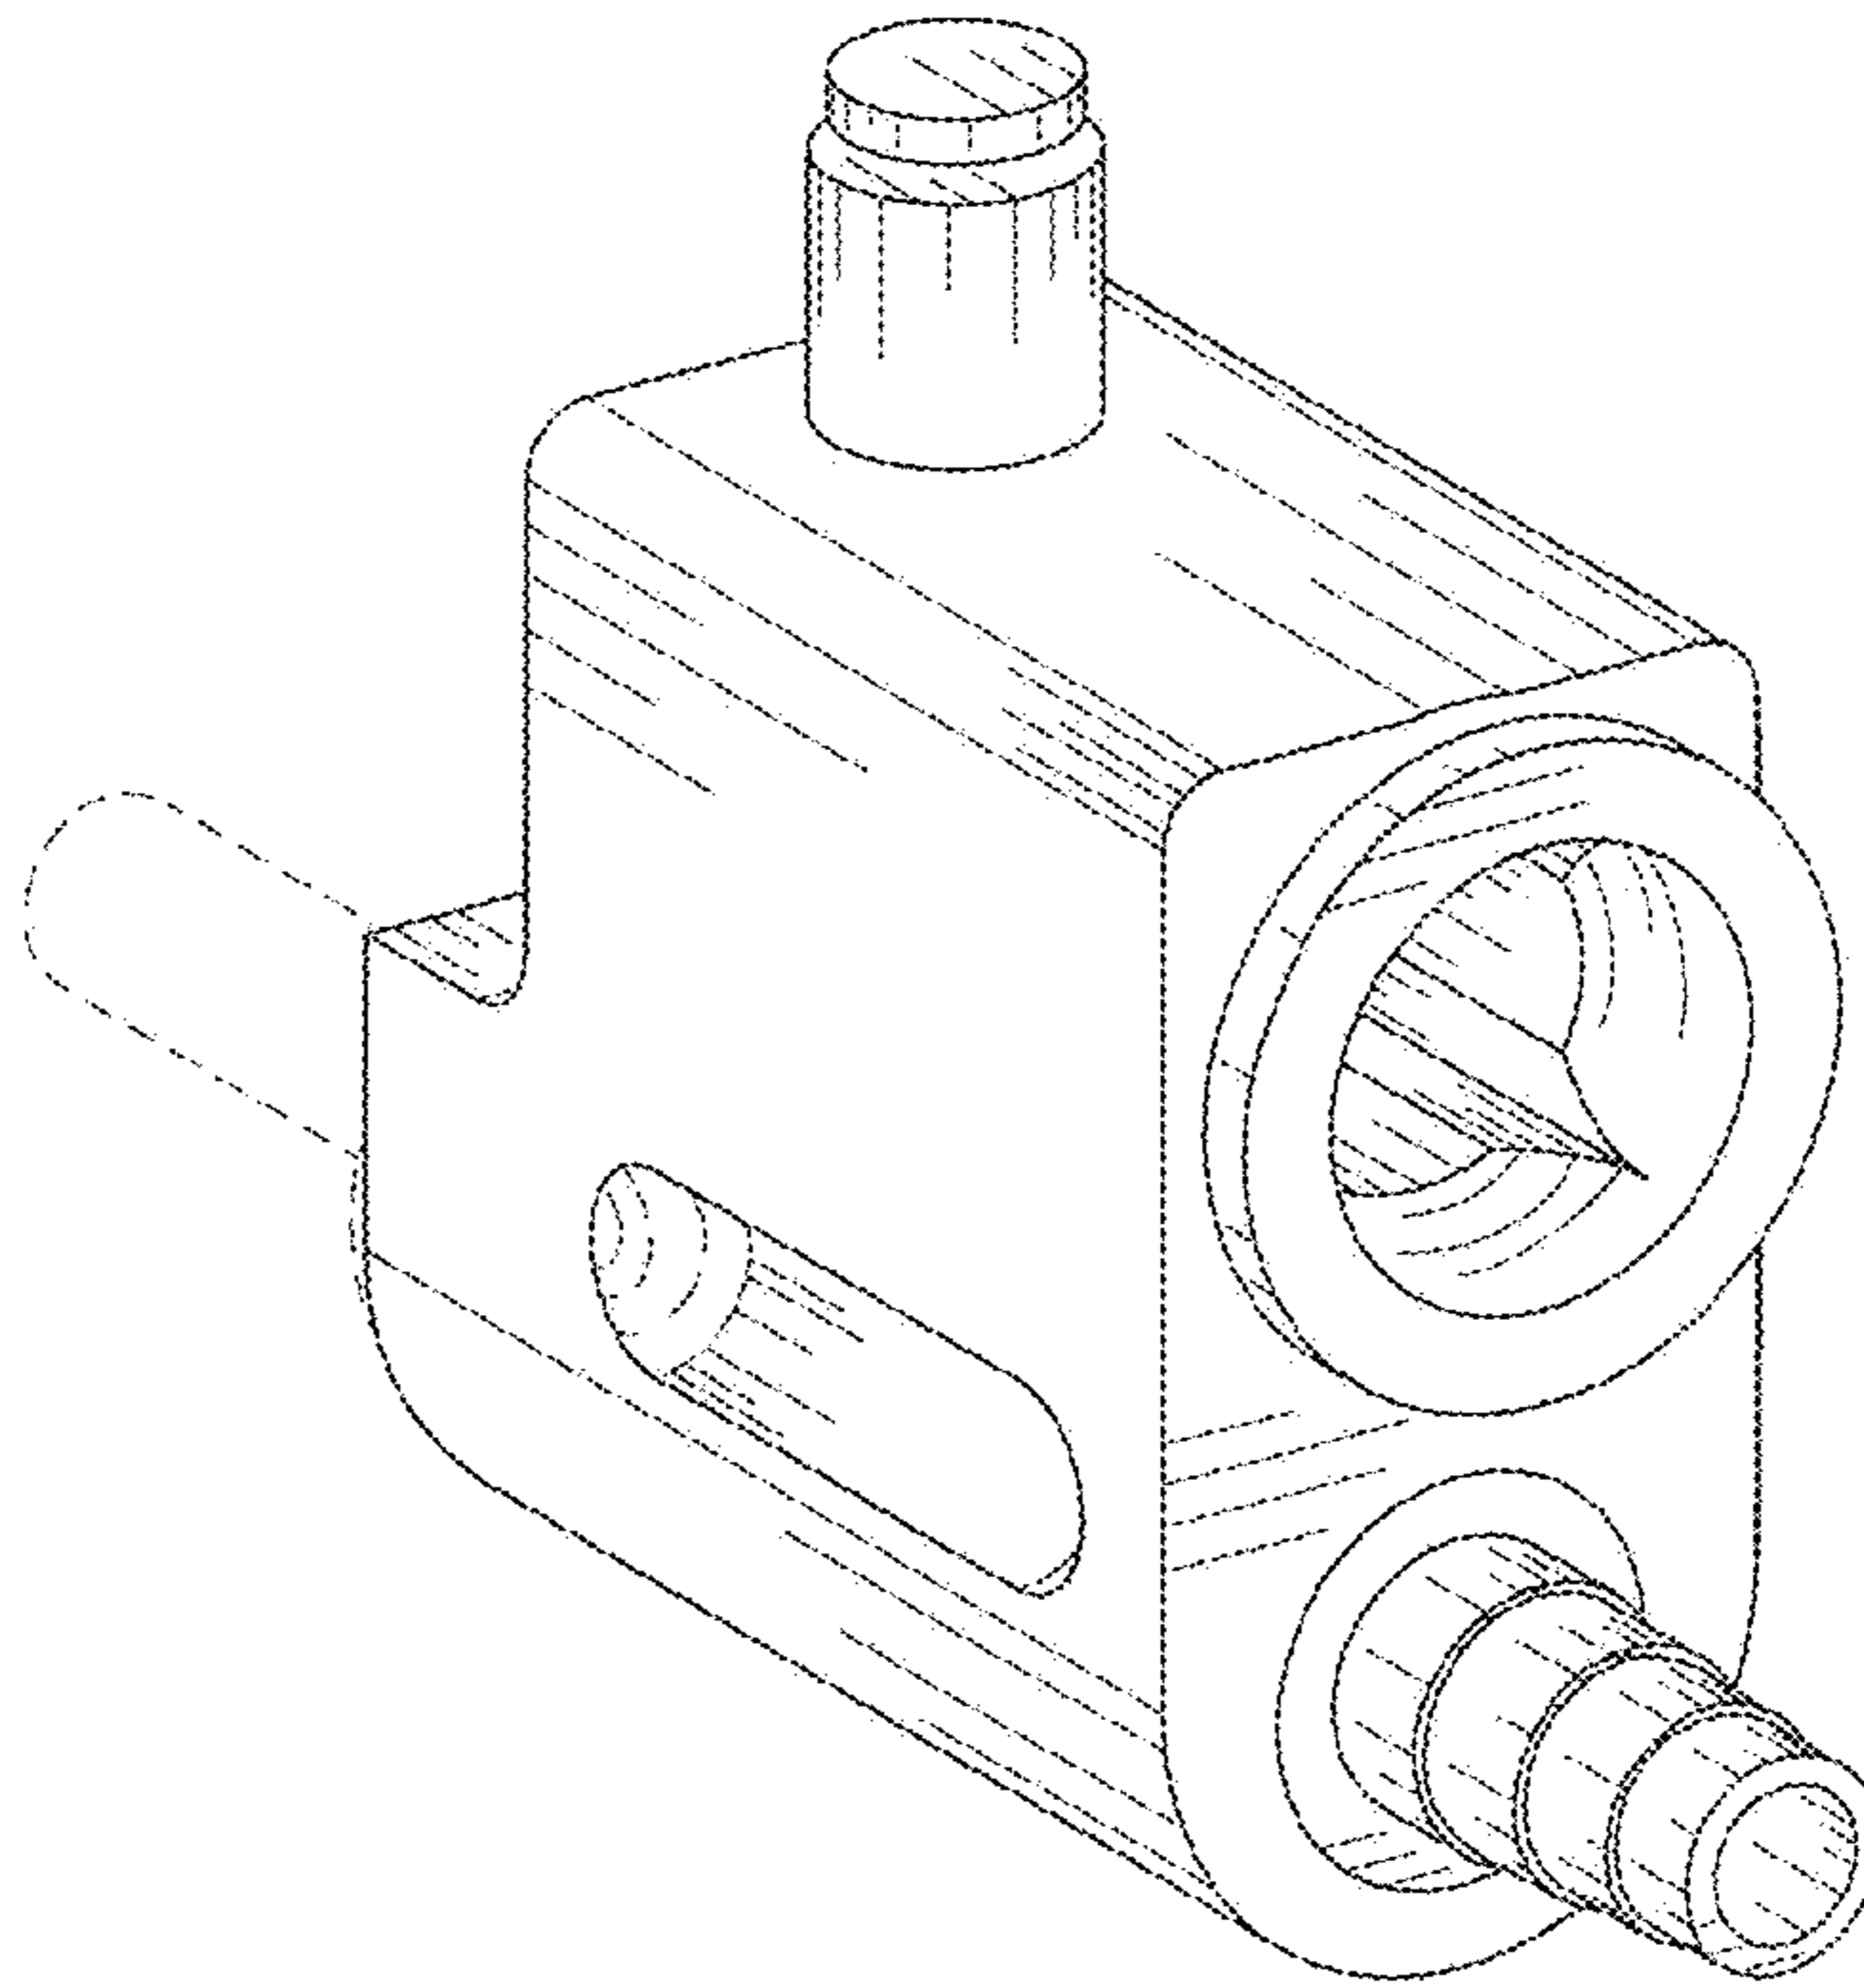


Fig 2

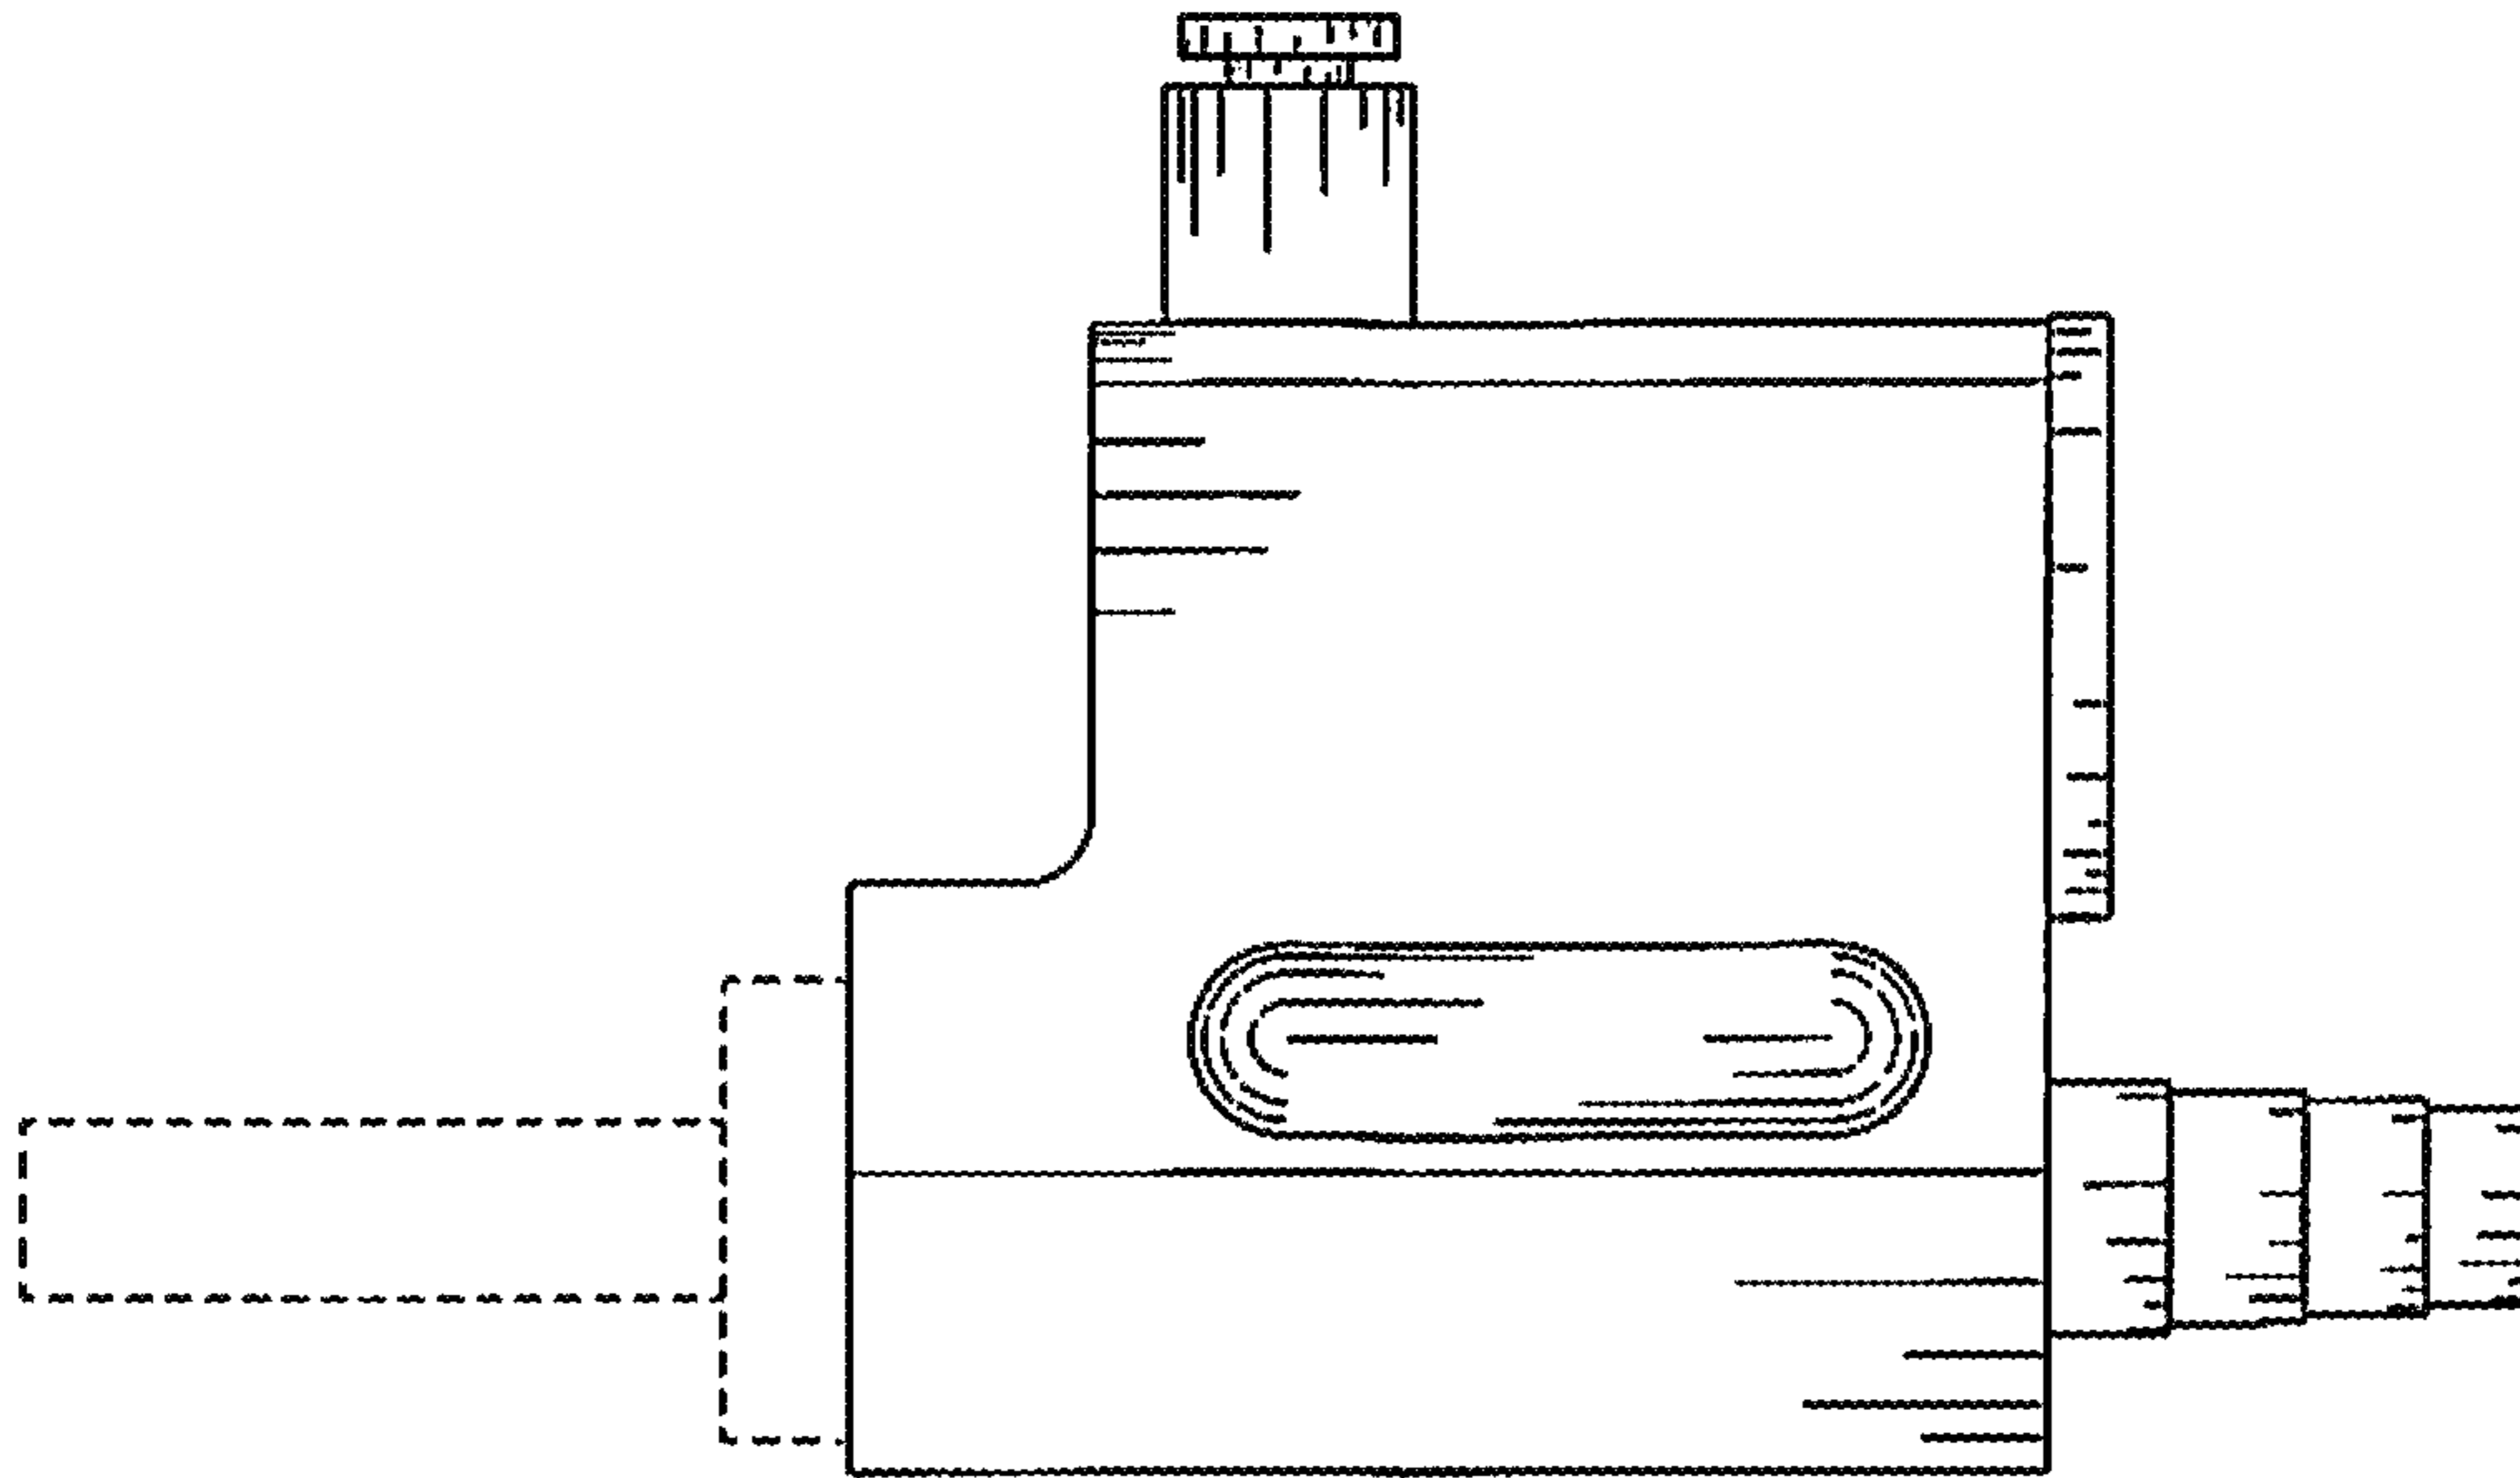


Fig 3

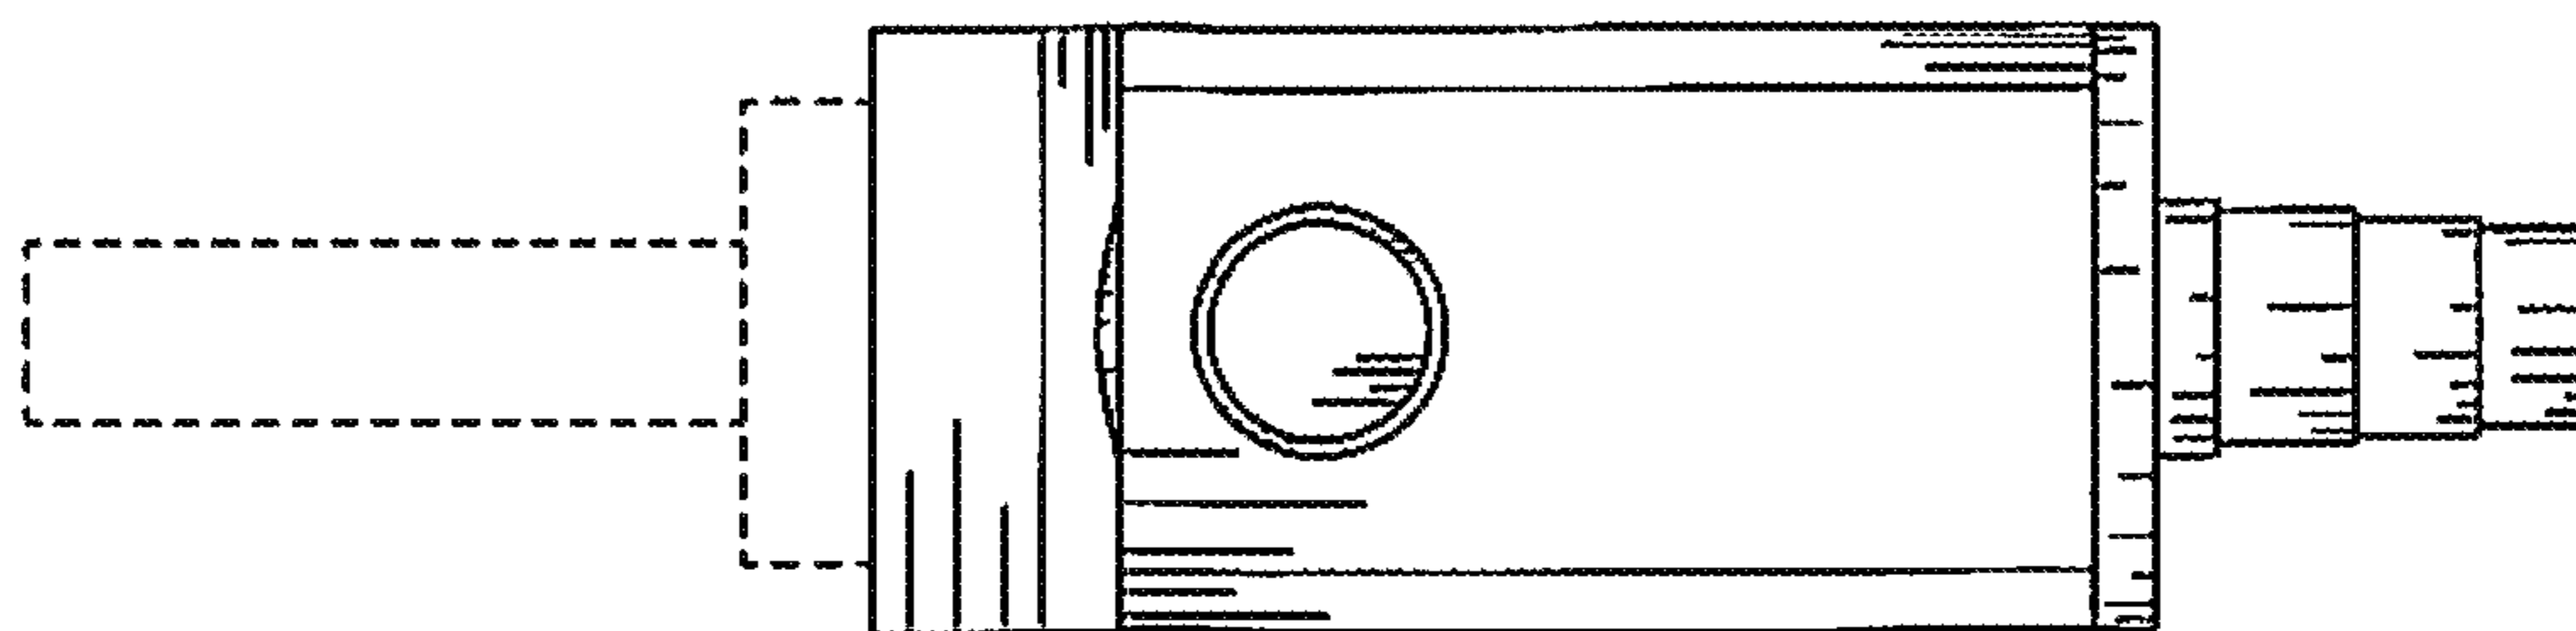


Fig 4

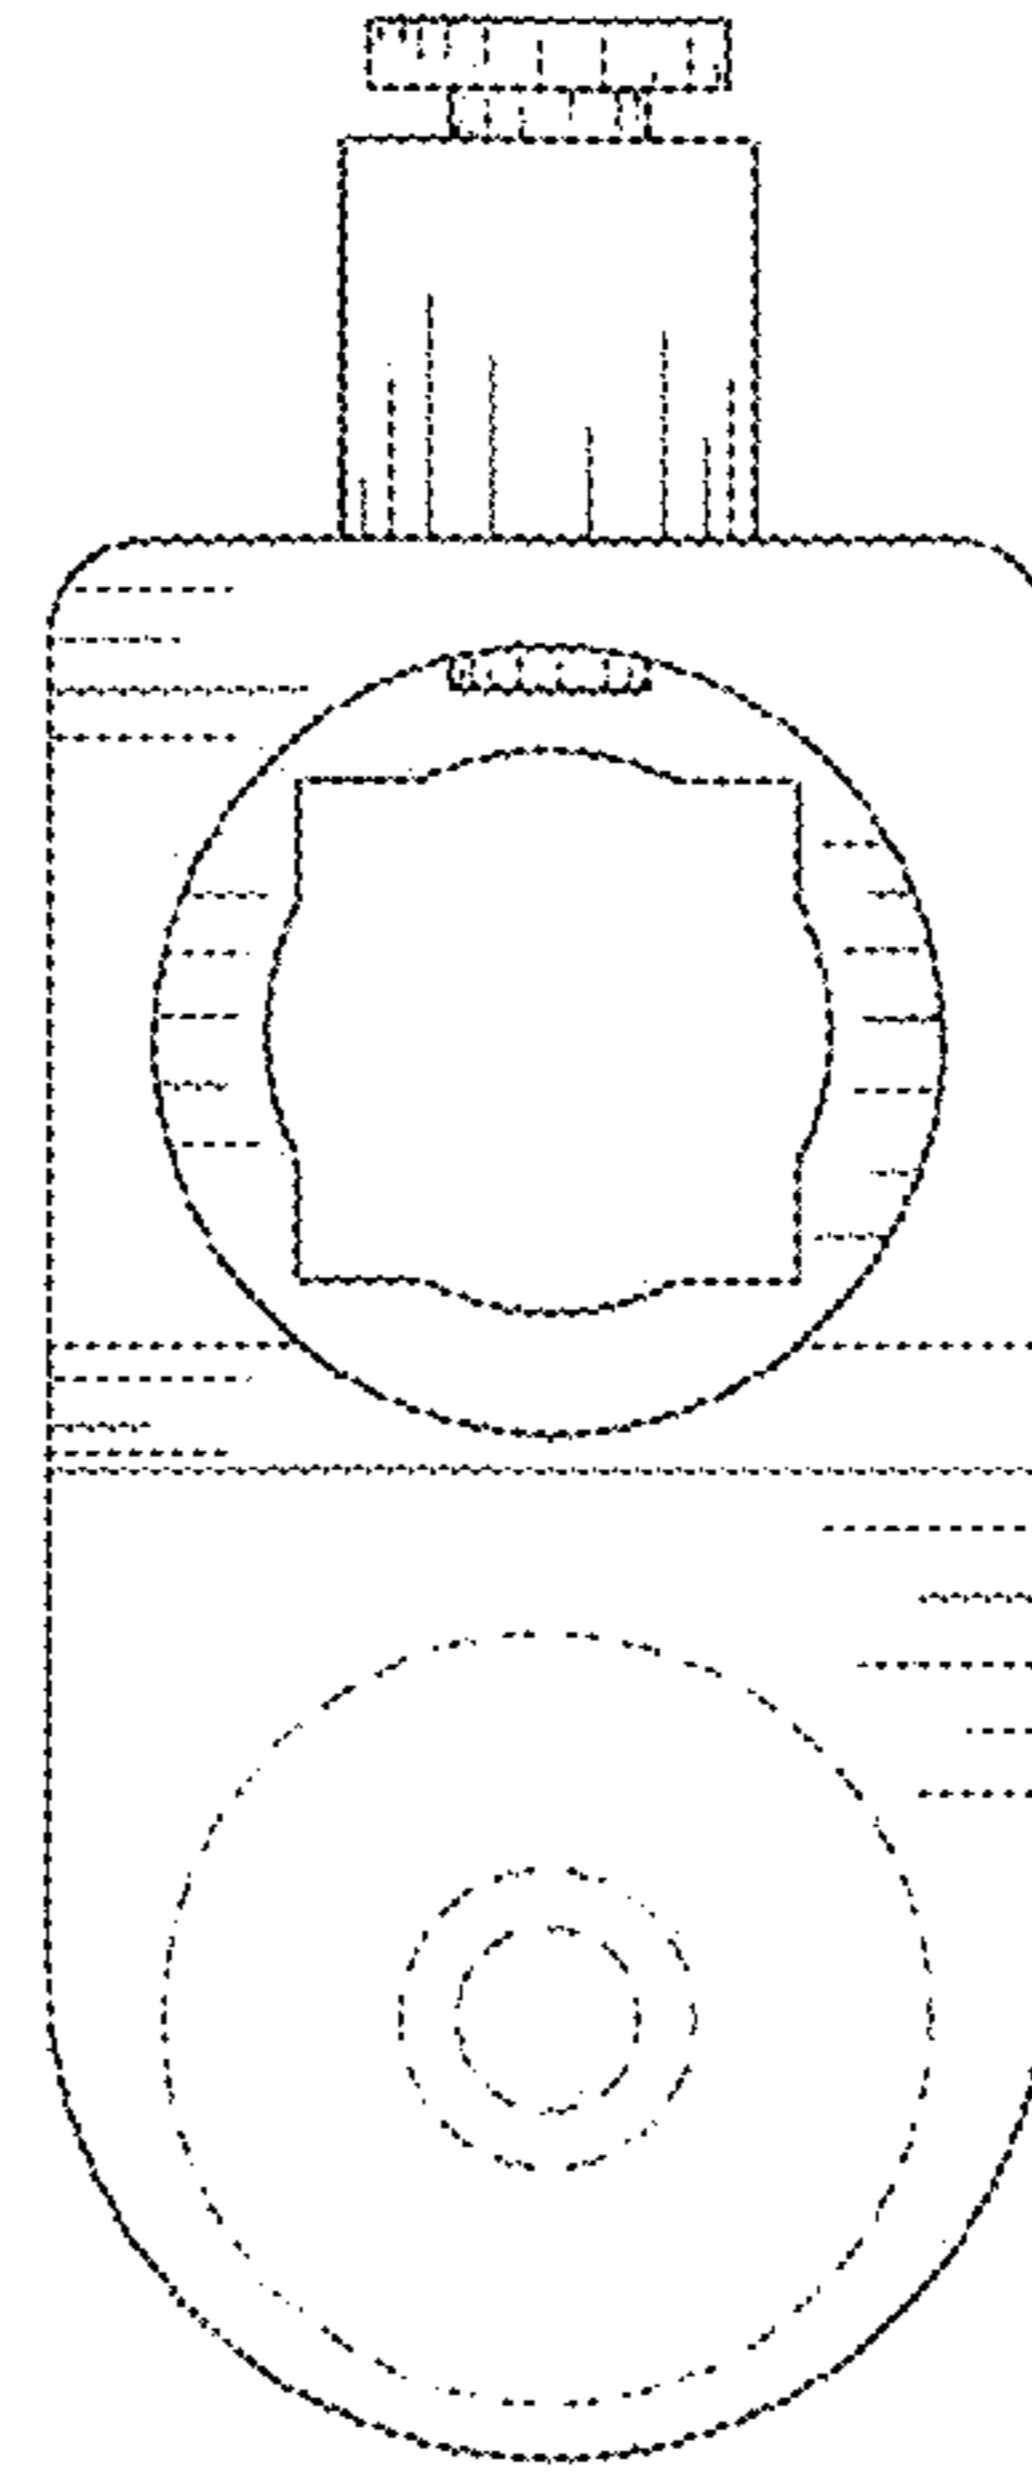


Fig 5

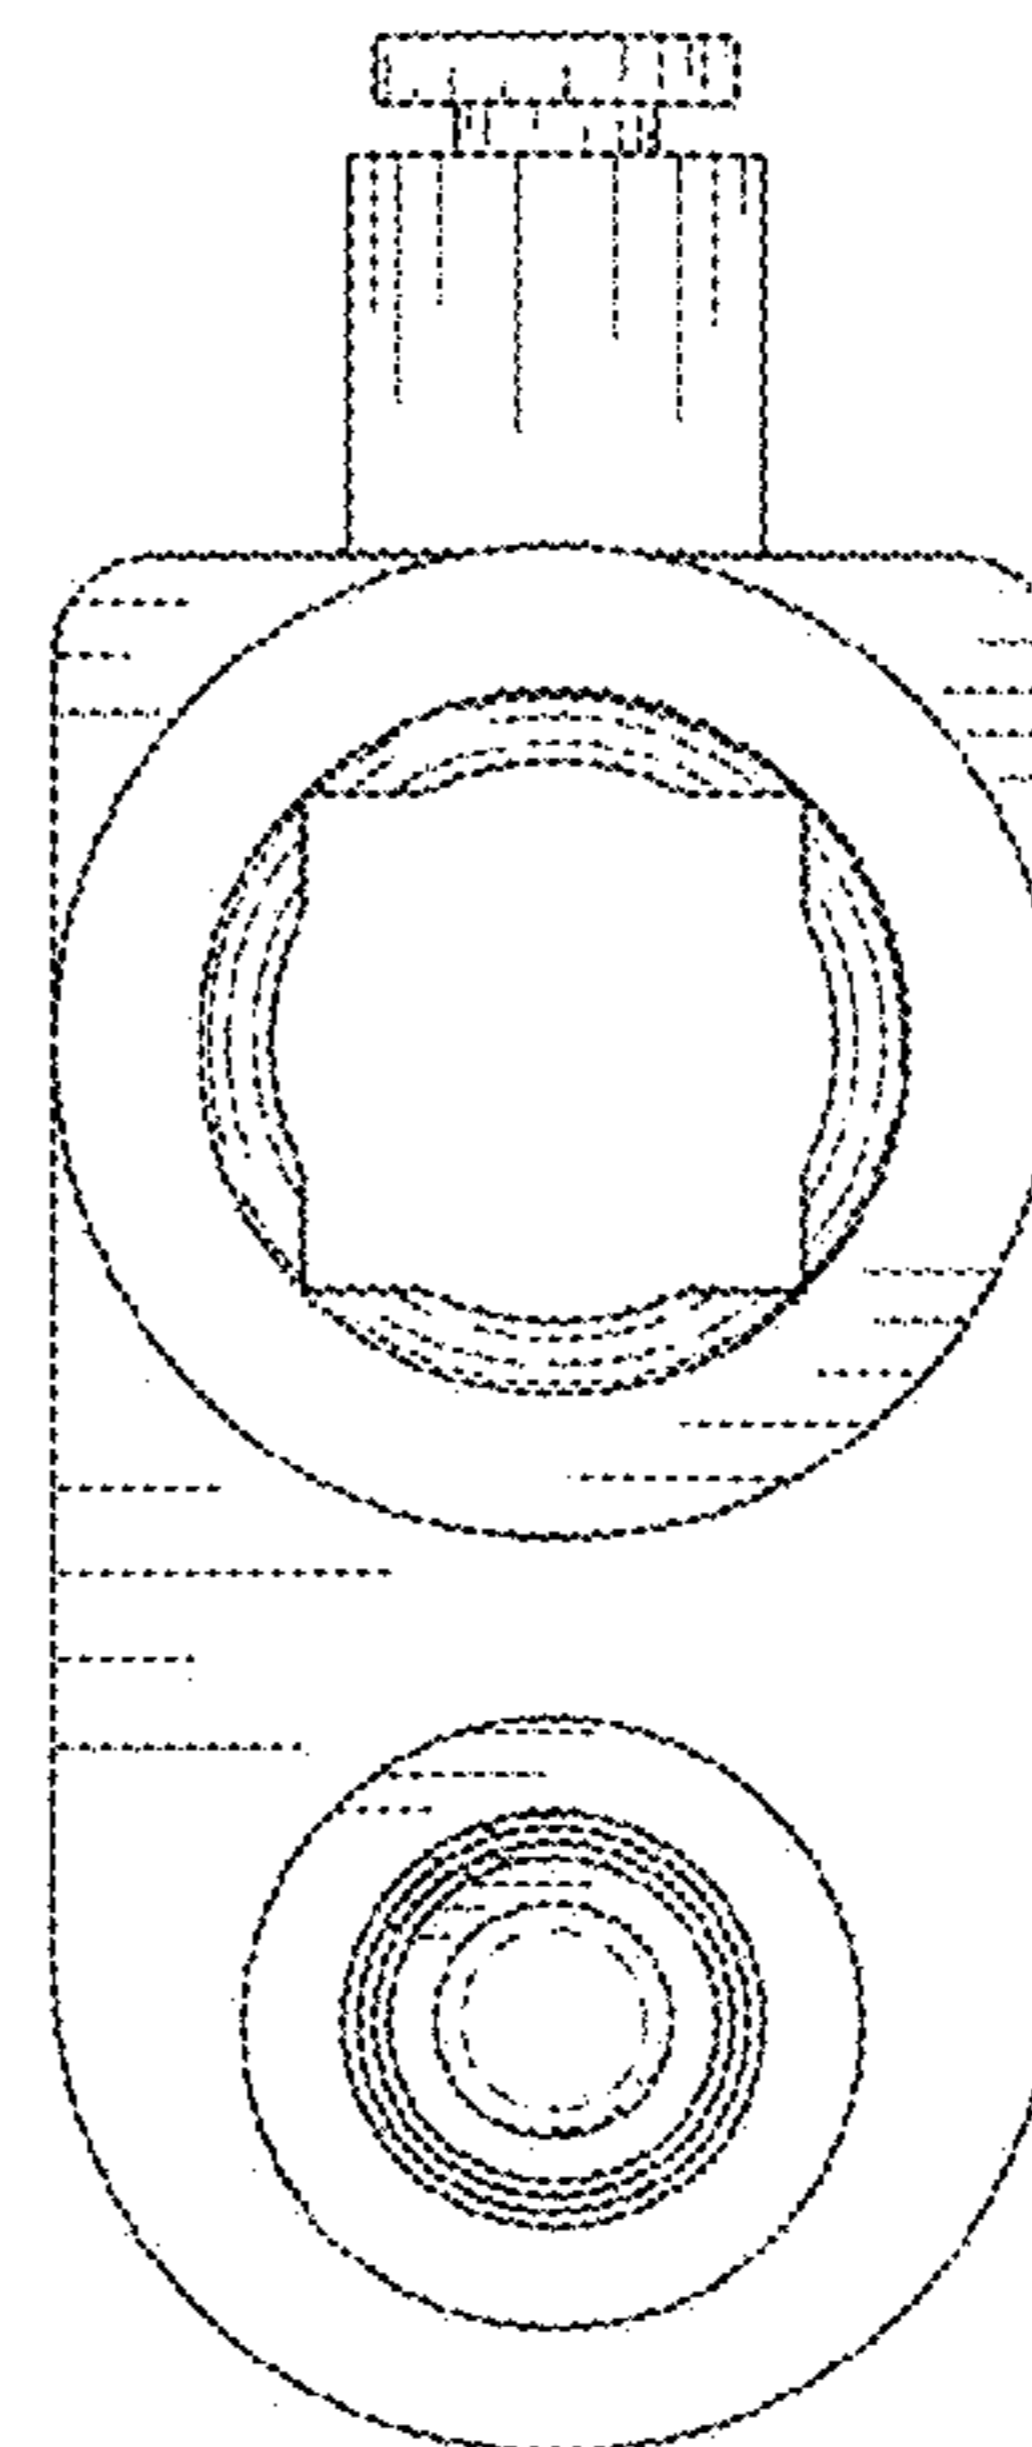


Fig 6

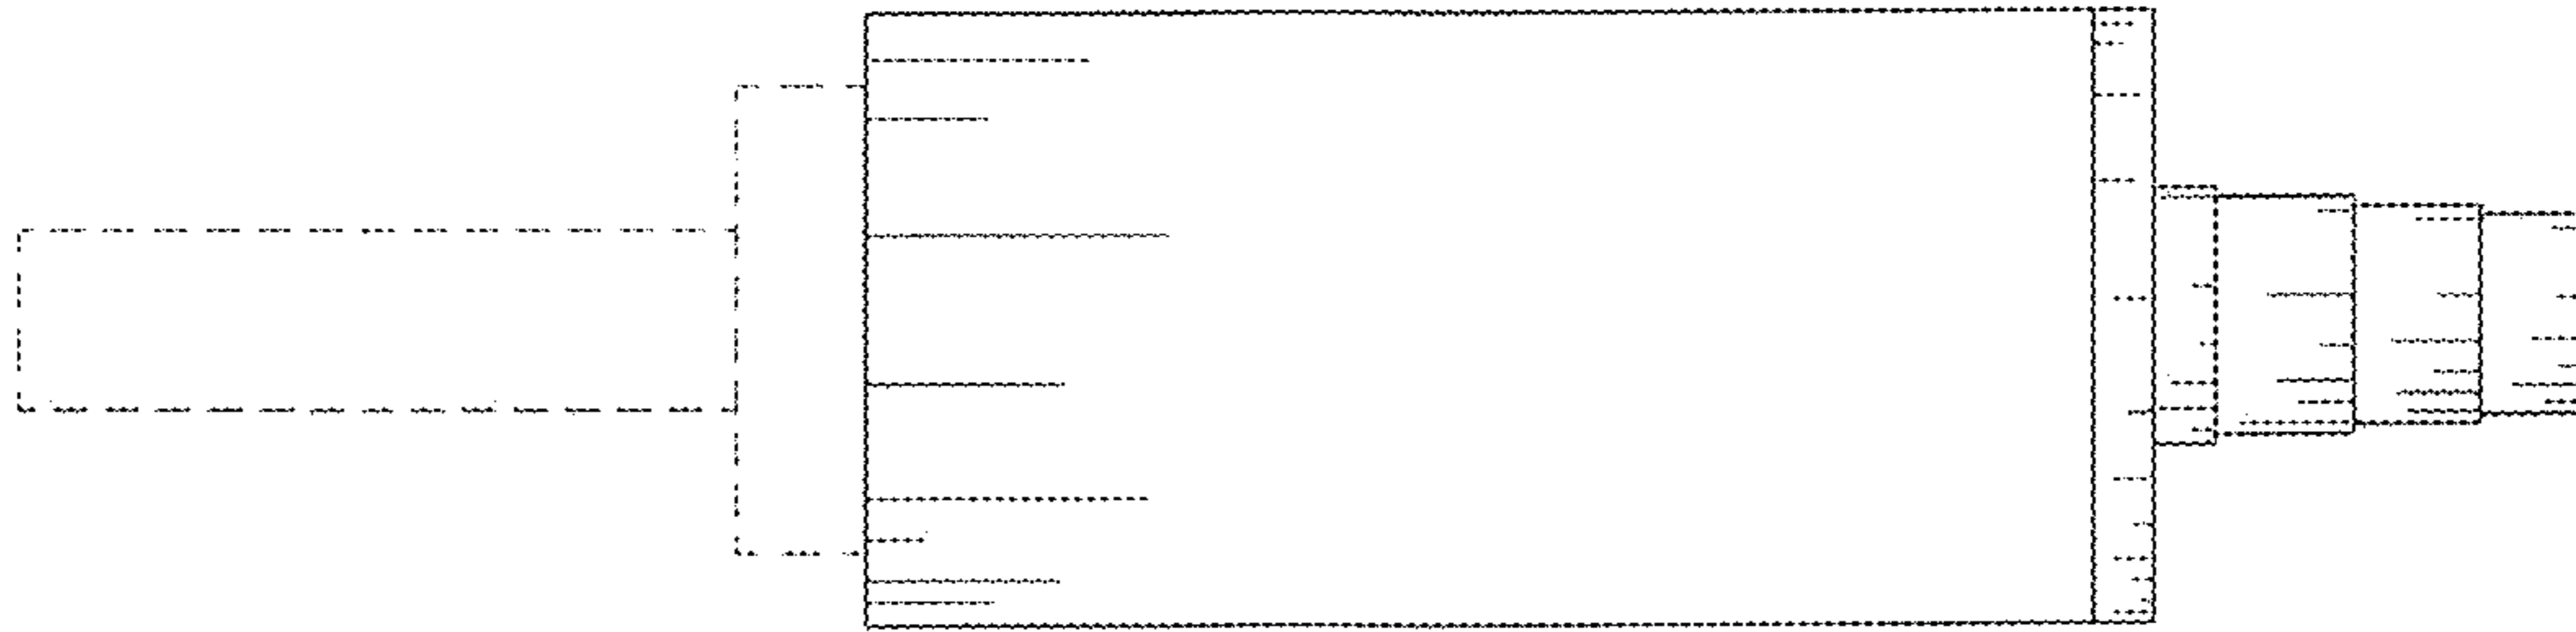


Fig 7

