



(12) **United States Design Patent**
Saenz Villalobos et al.

(10) **Patent No.:** **US D950,056 S**
(45) **Date of Patent:** **** Apr. 26, 2022**

(54) **DEVICE FOR TREATING TISSUE**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **BOSTON SCIENTIFIC SCIMED, INC.**, Maple Grove, MN (US)

JP H9173341 7/1997
JP 2004290675 10/2004
(Continued)

(72) Inventors: **Gonzalo Jose Saenz Villalobos**, Alajuela (CR); **Daniel Calvo Camacho**, Ciudad Colon (CR); **Rafael Berenzon**, La Union (CR); **Shawn Ryan**, Littleton, MA (US)

OTHER PUBLICATIONS

eickemeyer.co.uk, Endoscopy rat tooth forceps, undated online product page, retrieved Jun. 24, 2021 from <URL:https://www.eickemeyer.co.uk/Endoscopy/Broncho-Gastroscopy/Endoscopy-Rat-Tooth-Forceps.html> (Year: 2021).*
(Continued)

(73) Assignee: **BOSTON SCIENTIFIC SCIMED, INC.**, Maple Grove, MN (US)

Primary Examiner — Calvin E Vansant
(74) *Attorney, Agent, or Firm* — Fay Kaplun & Marcin, LLP

(**) Term: **15 Years**

(21) Appl. No.: **29/732,390**

(22) Filed: **Apr. 23, 2020**

(57) **CLAIM**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/148**

The ornamental design for a device for treating tissue, as shown and described.

(58) **Field of Classification Search**

USPC D24/148, 133, 143, 146, 147; D8/52, 57, D8/58
CPC A61B 17/28; A61B 17/122; A61B 17/282; A61B 17/295; A61B 17/1285; A61B 17/2841; A61B 2017/29; A61B 2017/2808; A61B 2017/2825; A61B 2017/2905; A61B 2017/2926; A61B 18/1442; A61B 18/1445; A61B 2018/1455

DESCRIPTION

FIG. 1 is a perspective view of an open configuration of our new design for a device for treating tissue.
FIG. 2 is a front view thereof;
FIG. 3 is a first side view thereof;
FIG. 4 is a top view thereof;
FIG. 5 is a rear view of thereof;
FIG. 6 is a second side view thereof;
FIG. 7 is a bottom view thereof;
FIG. 8 is a perspective view of a closed configuration of our new design for a device for treating tissue.
FIG. 9 is a front view thereof;
FIG. 10 is a rear view thereof;
FIG. 11 is a first side view thereof;
FIG. 12 is a second side view thereof;
FIG. 13 is a top view thereof; and,
FIG. 14 is a bottom view thereof.

See application file for complete search history.


(56) **References Cited**

U.S. PATENT DOCUMENTS

D446,581 S * 8/2001 Petersvik D24/133
6,824,548 B2 * 11/2004 Smith A61B 17/122 606/142

(Continued)

(Continued)

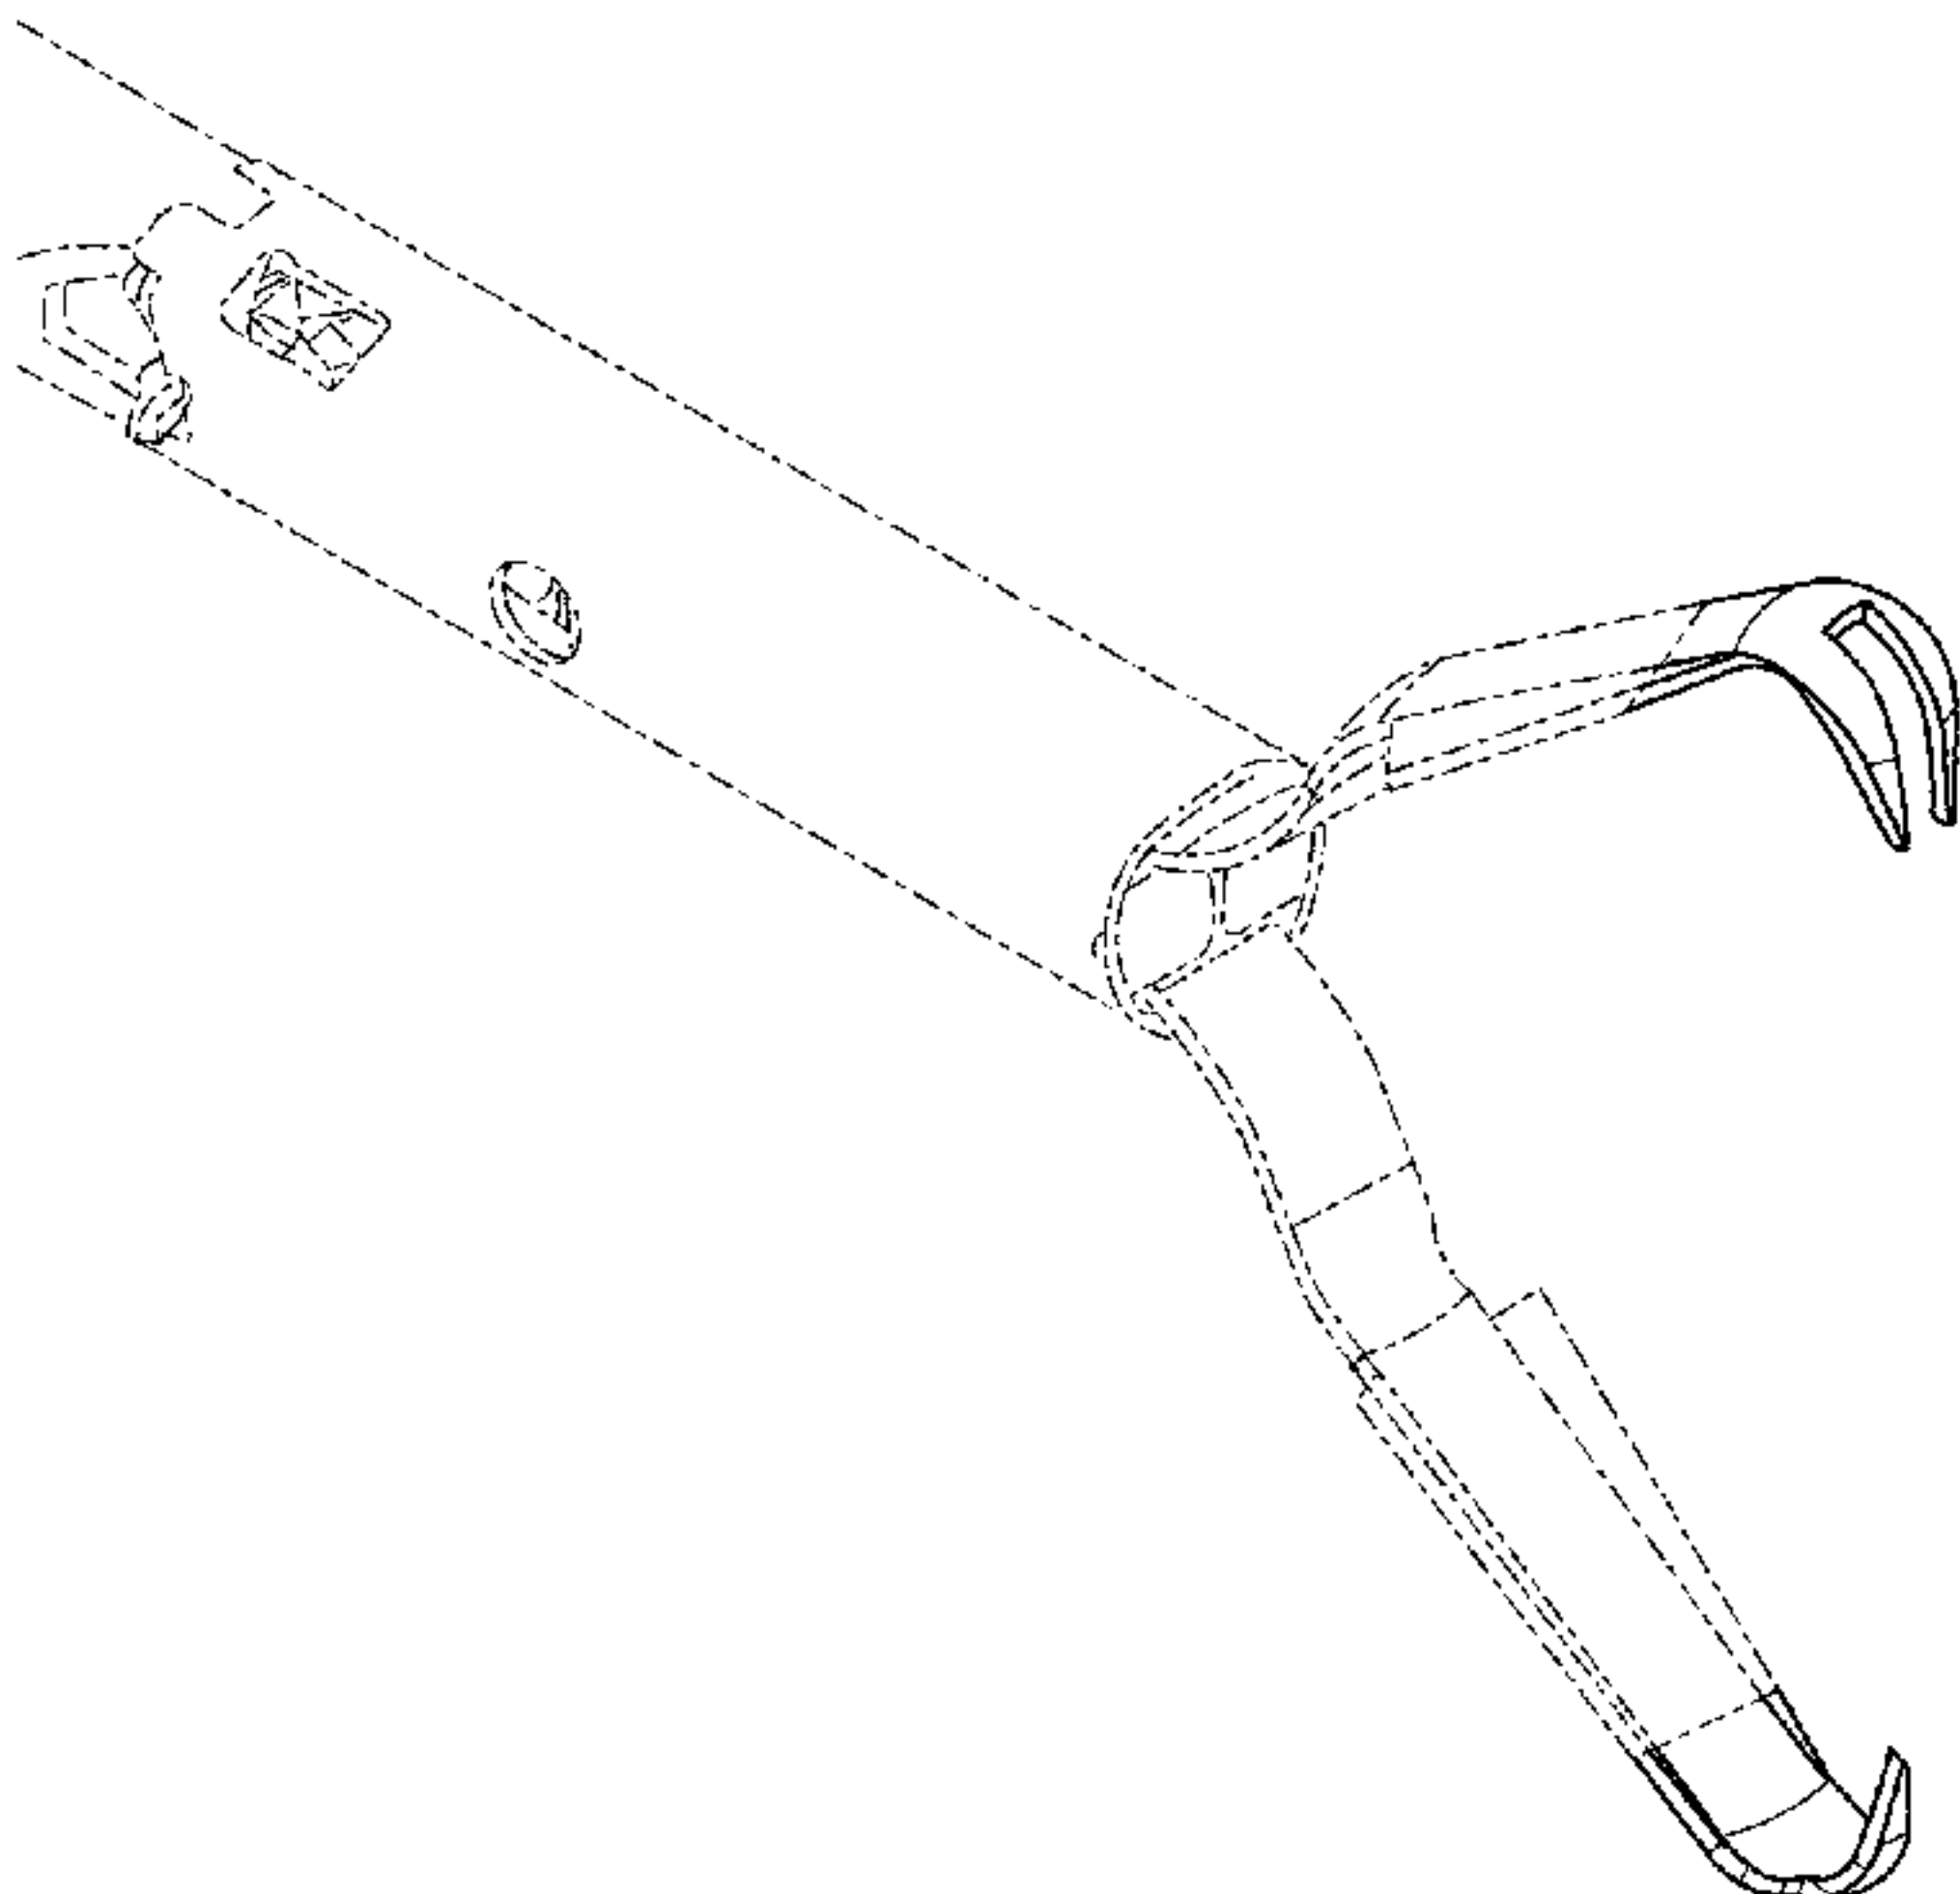

In the drawings, the broken lines are shown for the purpose of illustrating a portion of the device for treating tissue and form no part of the claimed design.

1 Claim, 5 Drawing Sheets

(56) References Cited

U.S. PATENT DOCUMENTS

D575,400 S * 8/2008 Patterson D24/143
7,828,811 B2 * 11/2010 Kortenbach A61B 17/1285
606/142
8,066,721 B2 * 11/2011 Kortenbach A61B 1/00087
606/142
8,070,759 B2 * 12/2011 Stefanchik A61B 17/0491
606/139
D689,606 S * 9/2013 John D24/133
D710,006 S 7/2014 John et al.
D725,265 S 3/2015 John et al.

D758,581 S * 6/2016 Michelini A61B 17/29
D24/143
D779,668 S * 2/2017 Michelini A61B 17/122
D24/143
D834,715 S * 11/2018 Alladu A61B 10/02
D24/147
10,863,998 B2 * 12/2020 Mottola A61B 10/02
2007/0250111 A1 * 10/2007 Lu A61B 17/29
606/205
2020/0093496 A1 * 3/2020 Ryan A61B 17/10
2020/0397455 A1 * 12/2020 Baril A61B 17/2816

FOREIGN PATENT DOCUMENTS

JP 2012045397 3/2012
JP 1553237 S 7/2016

OTHER PUBLICATIONS

“Toshiba Electronic Endoscope TRE-3600”, Denpa Shinbun, Sep. 1995, 5 sheets. (Orginial and English Translation).

* cited by examiner

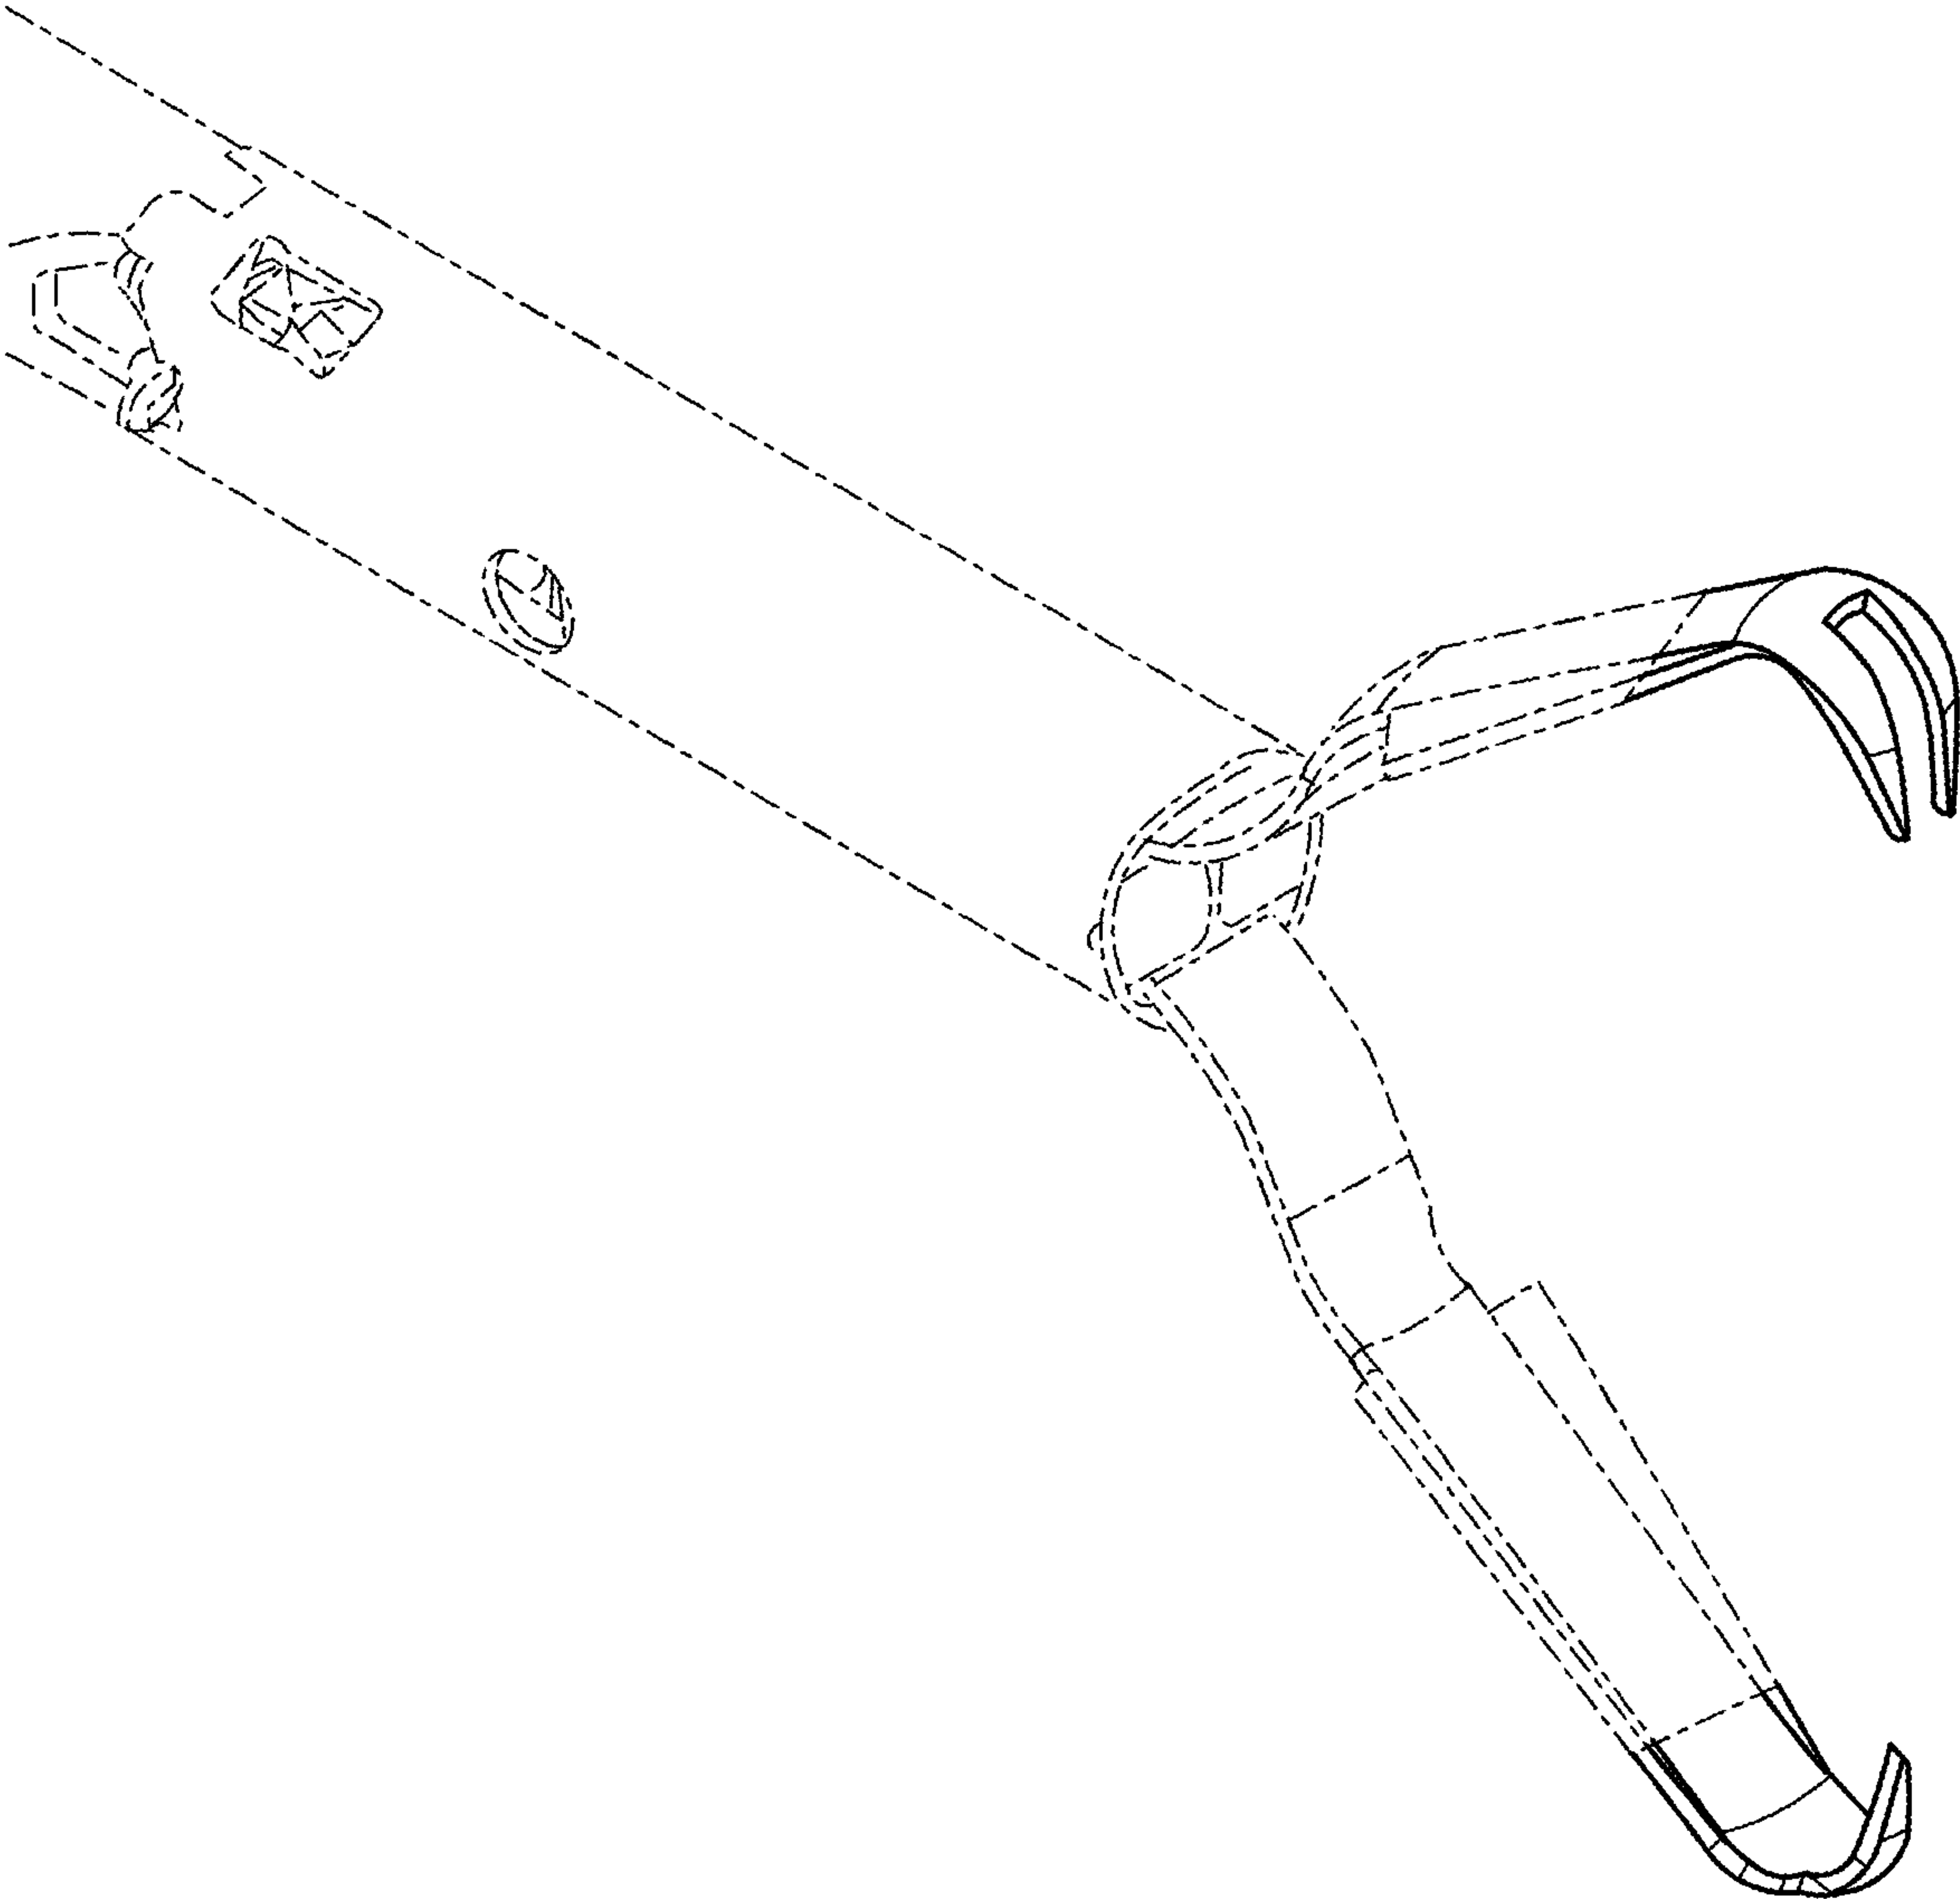


FIG. 1

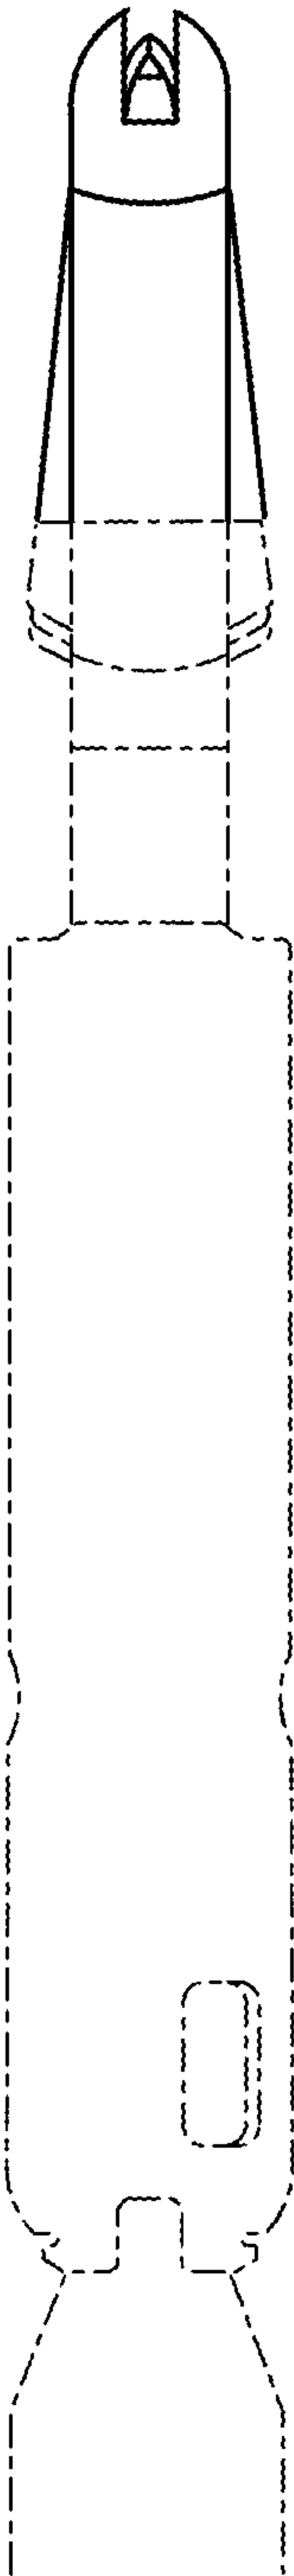


FIG. 4

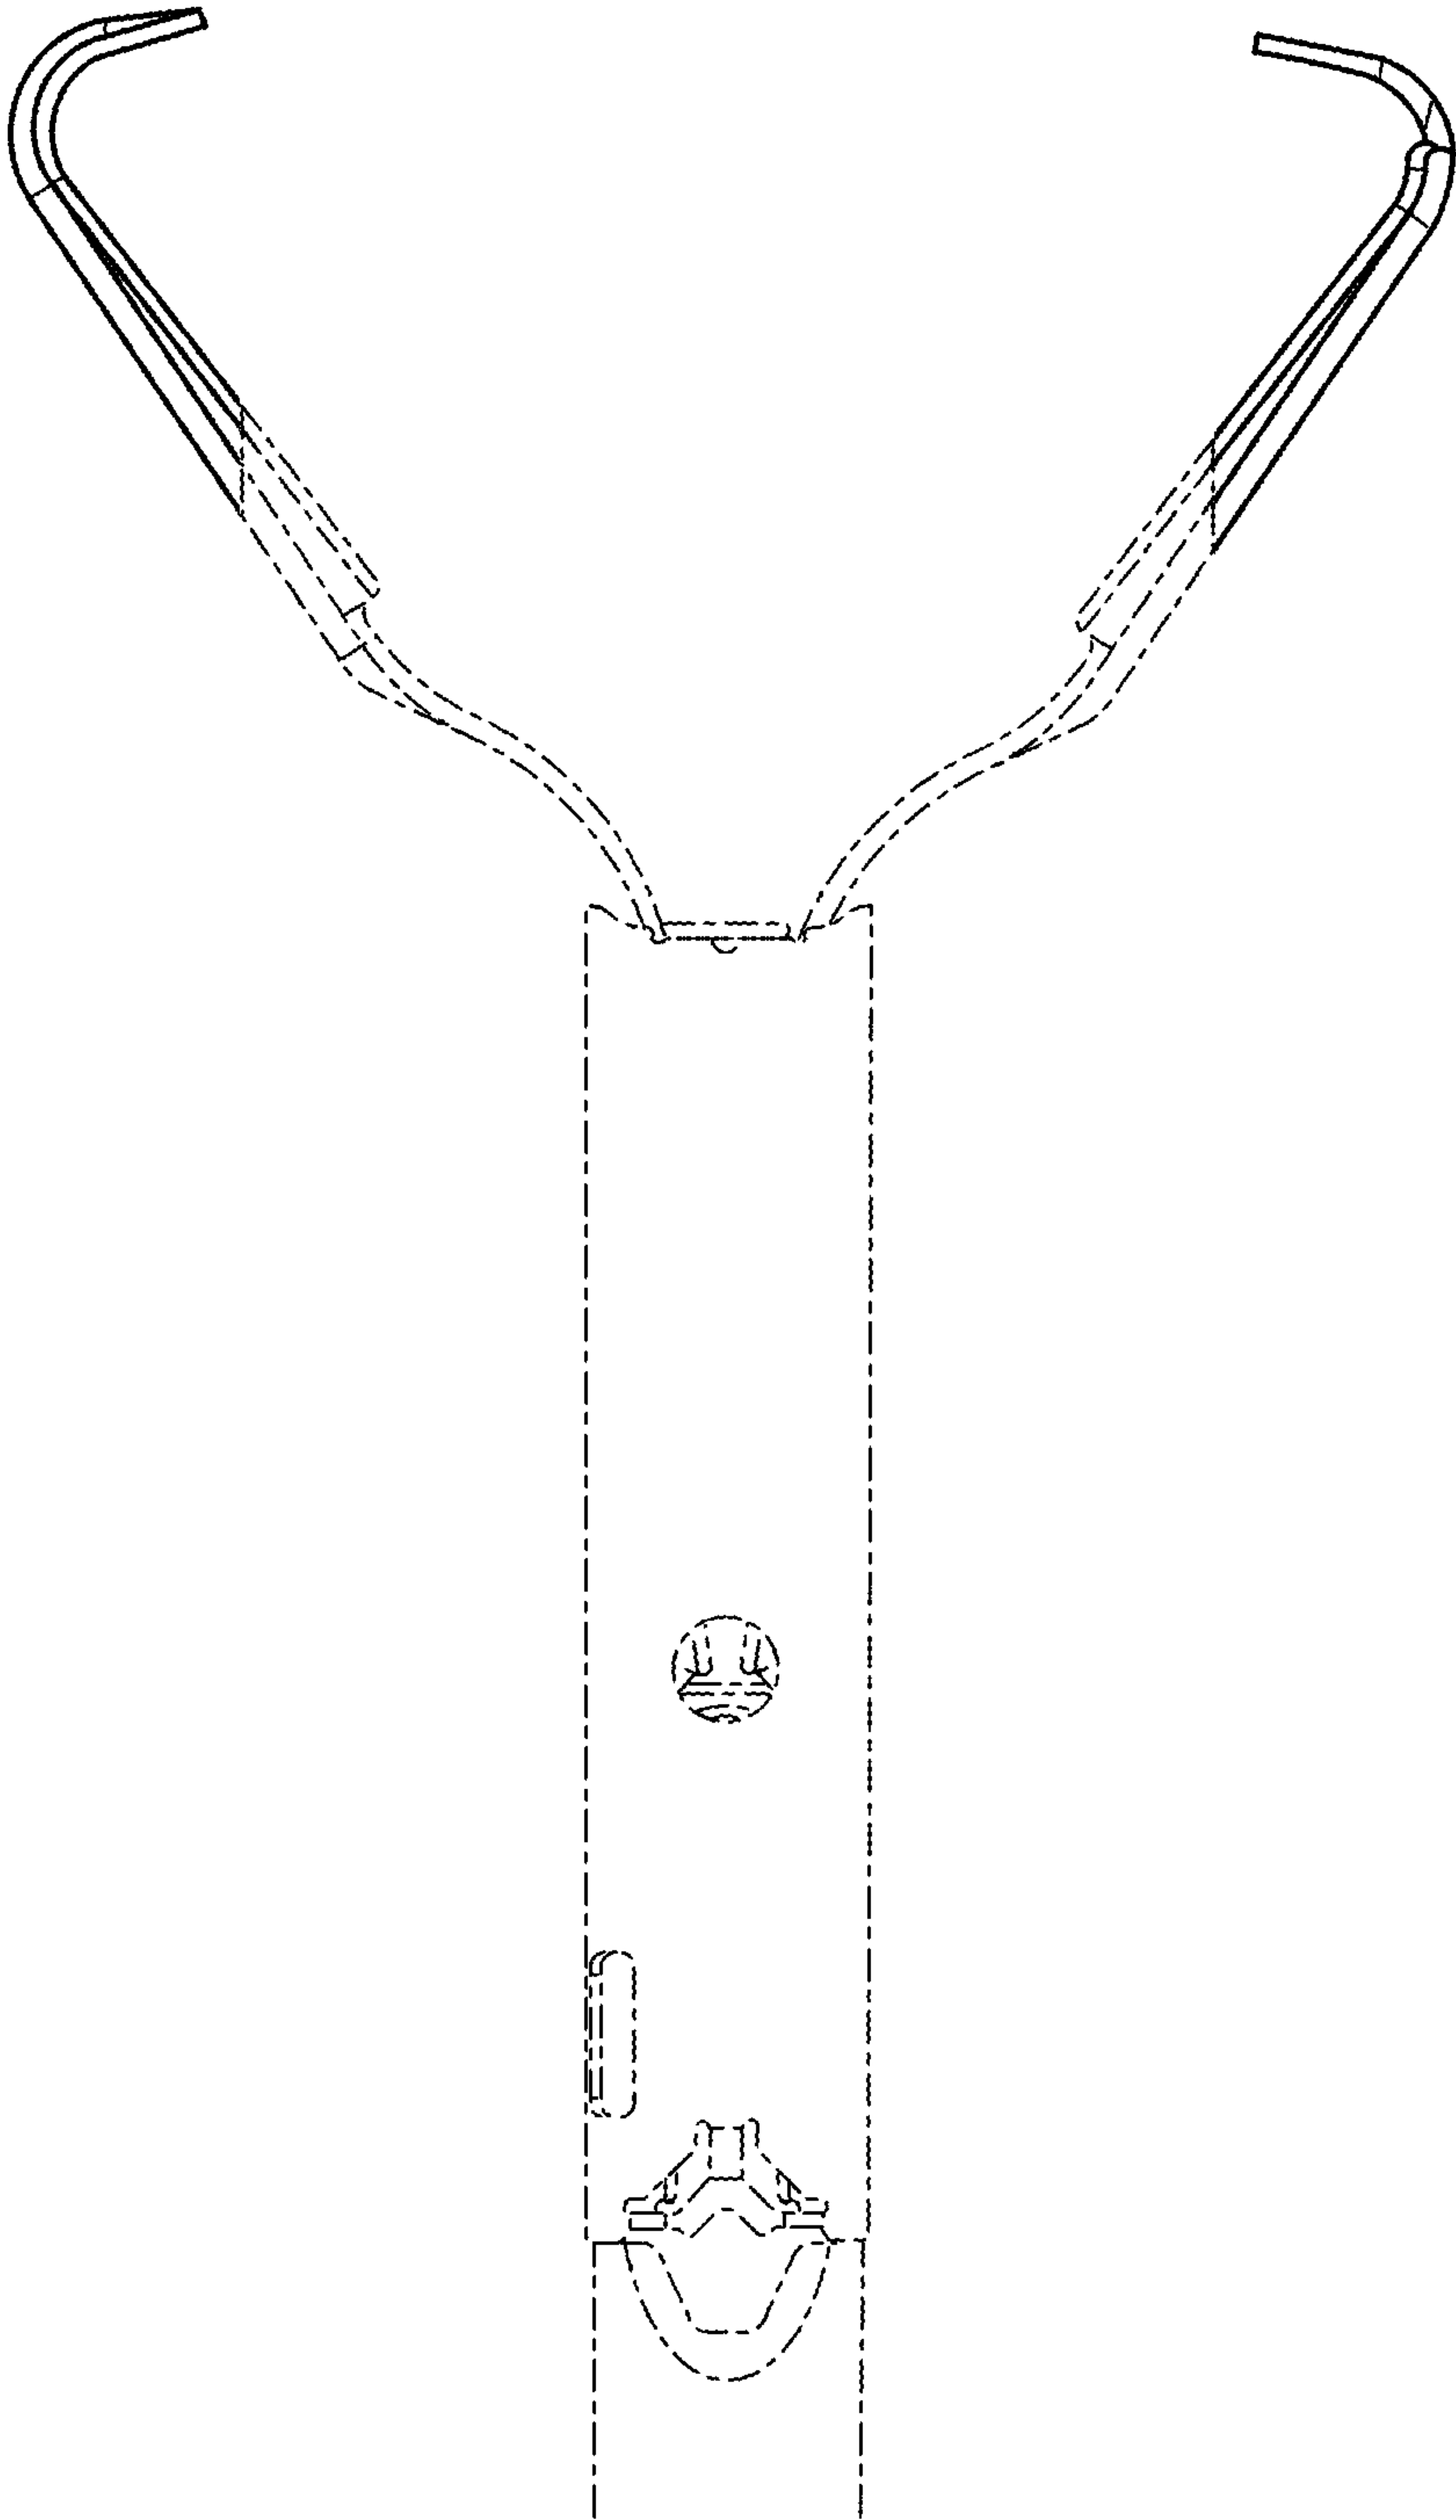


FIG. 3

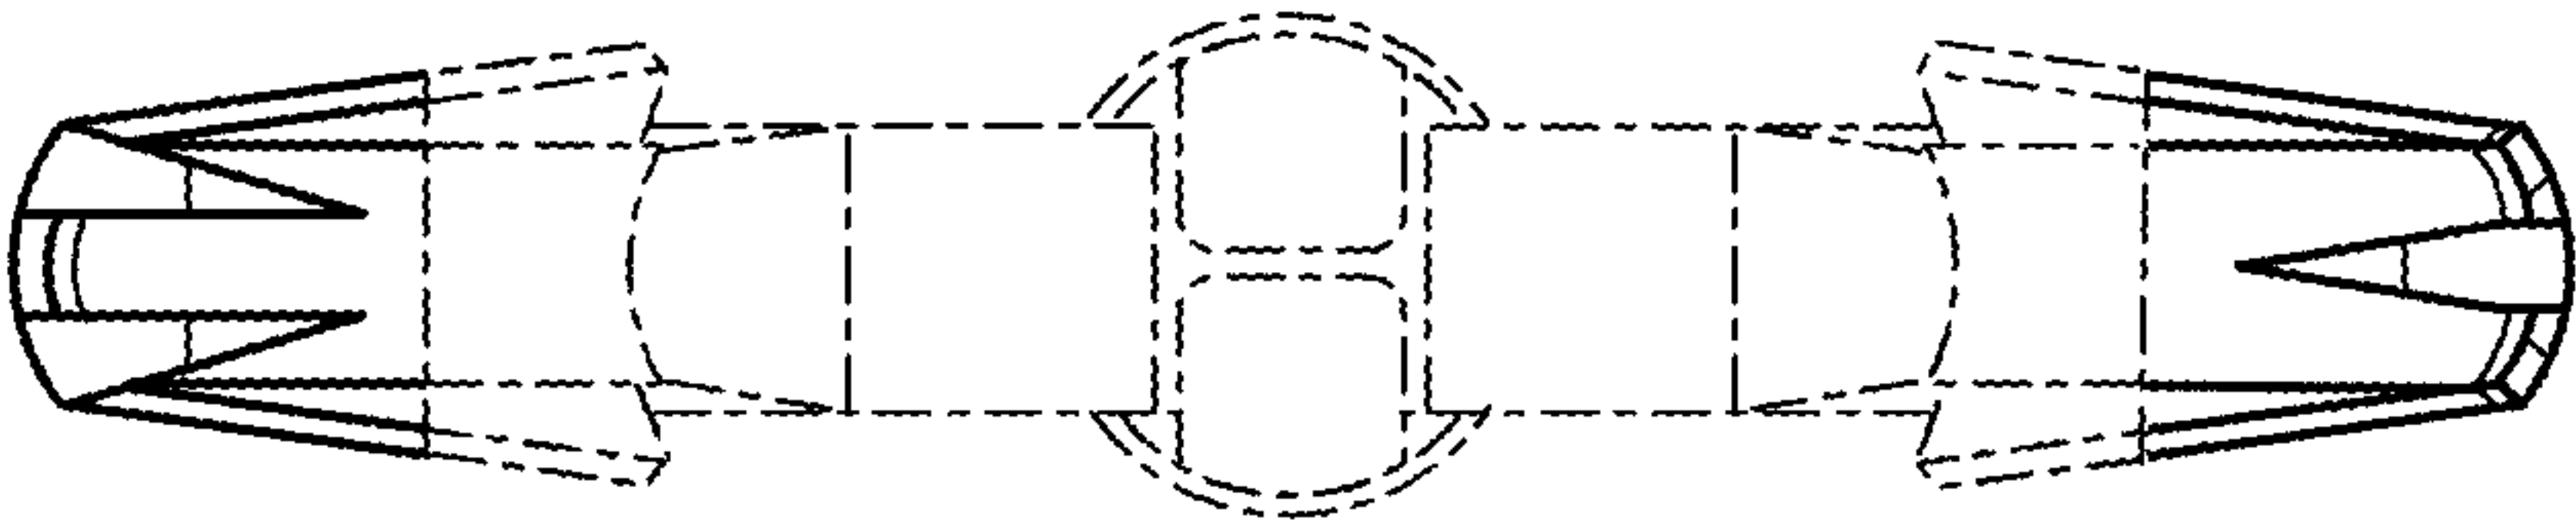


FIG. 2

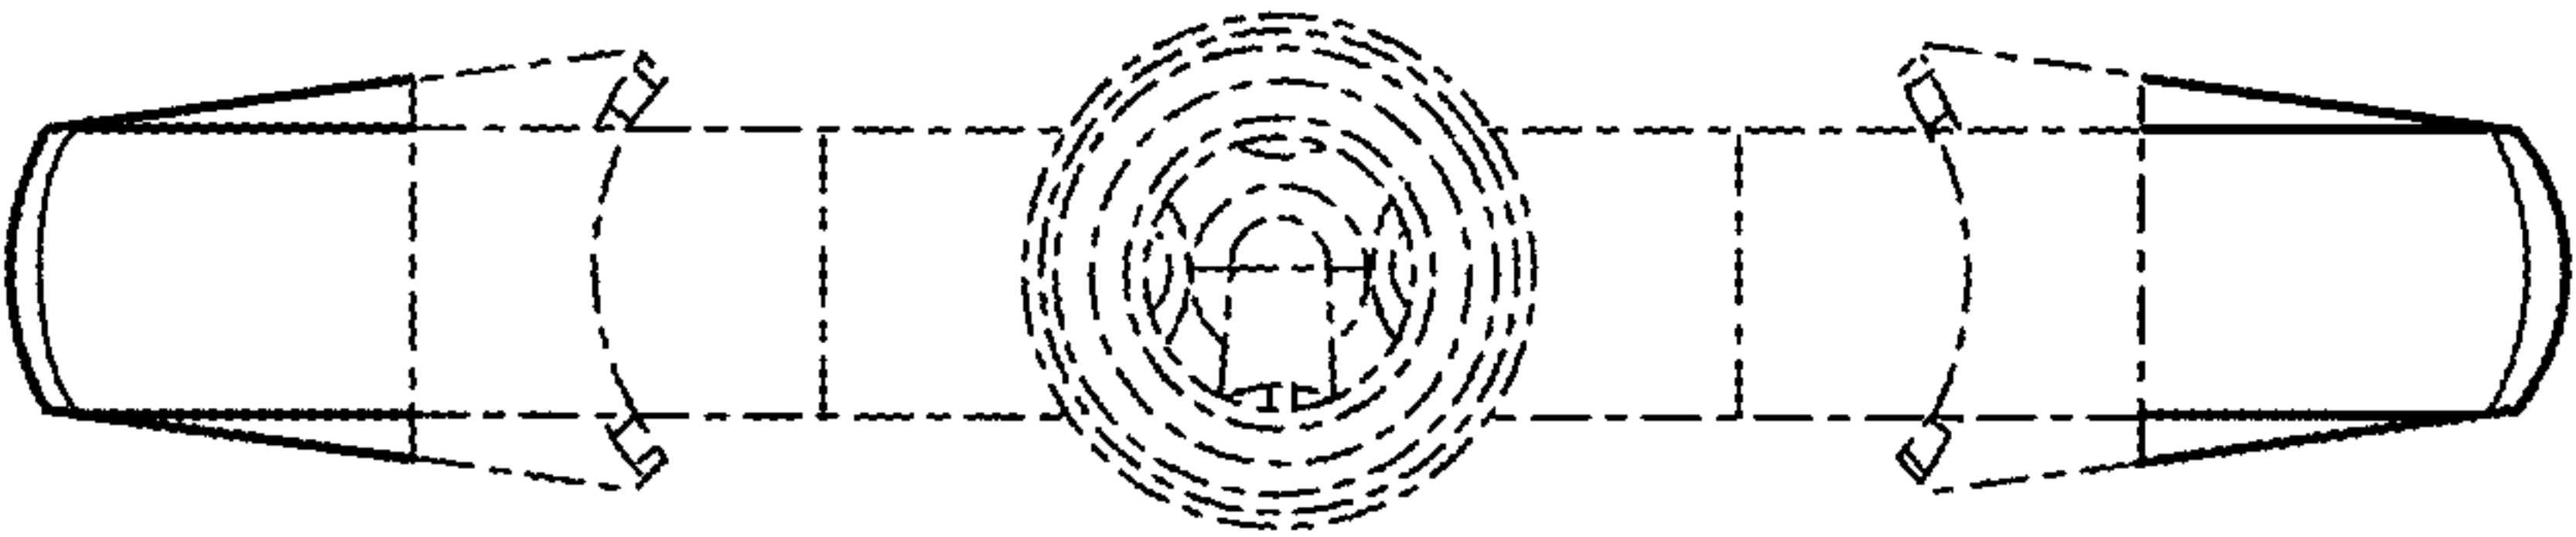


FIG. 5

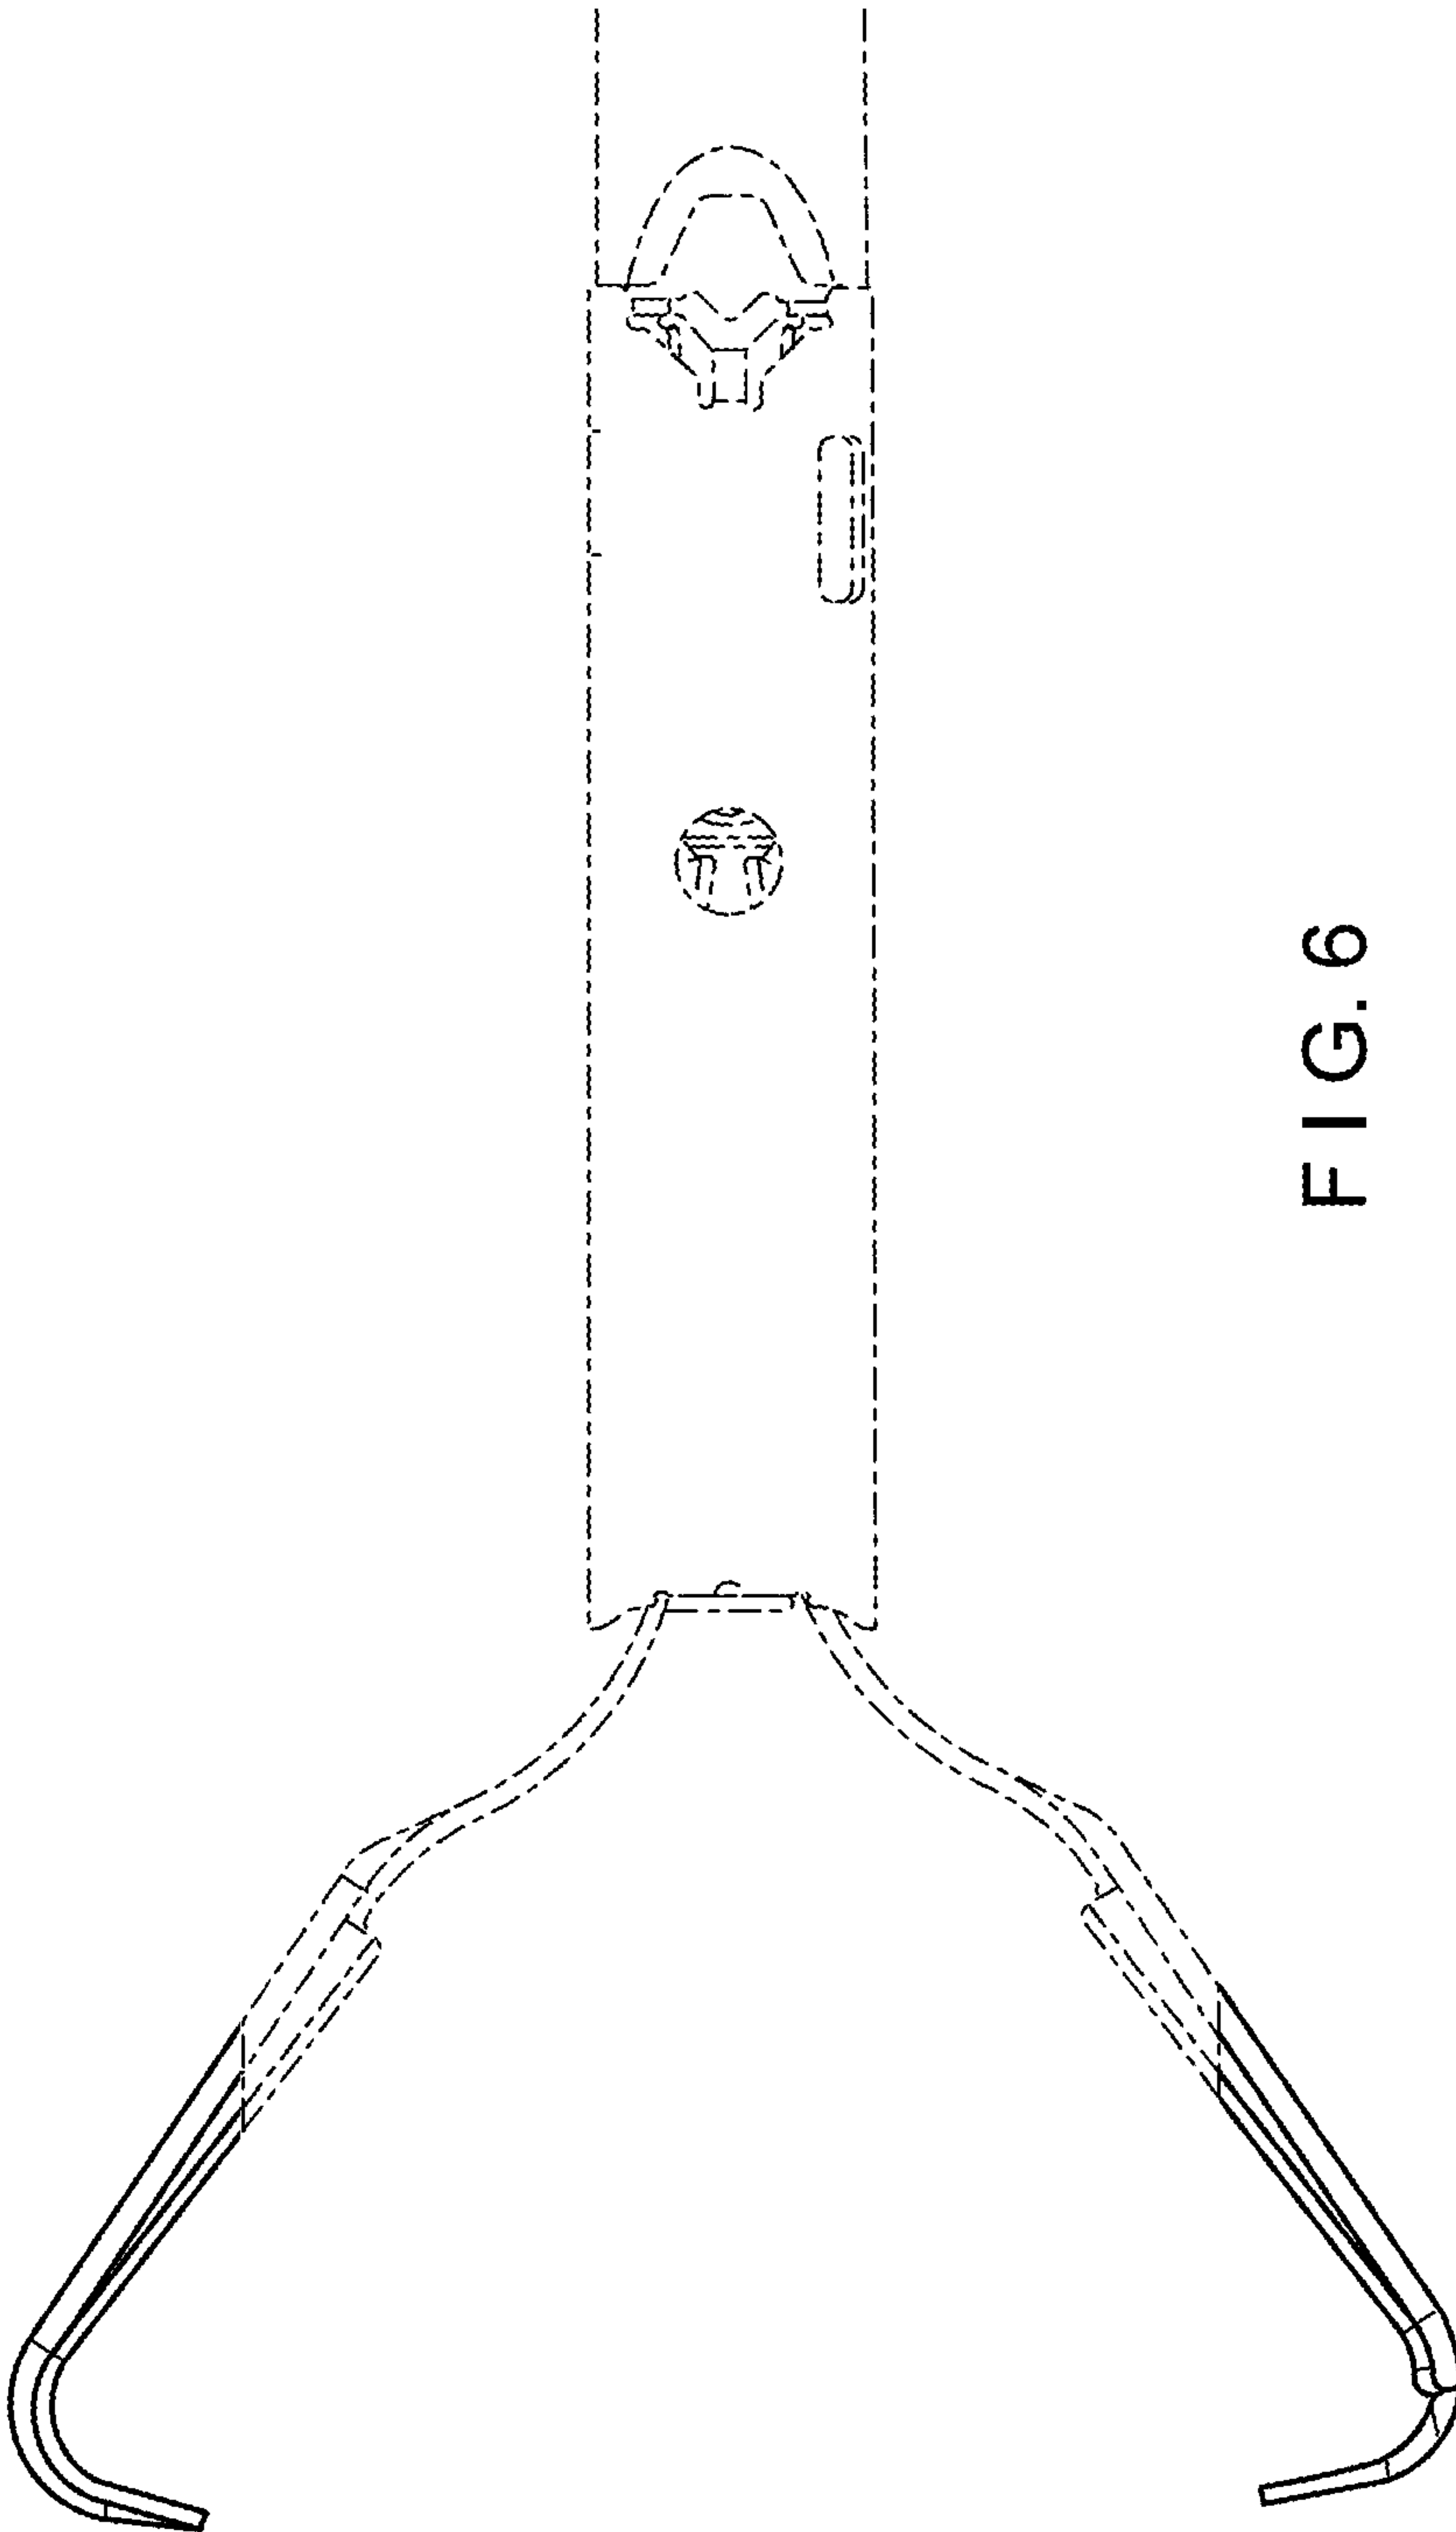


FIG. 6

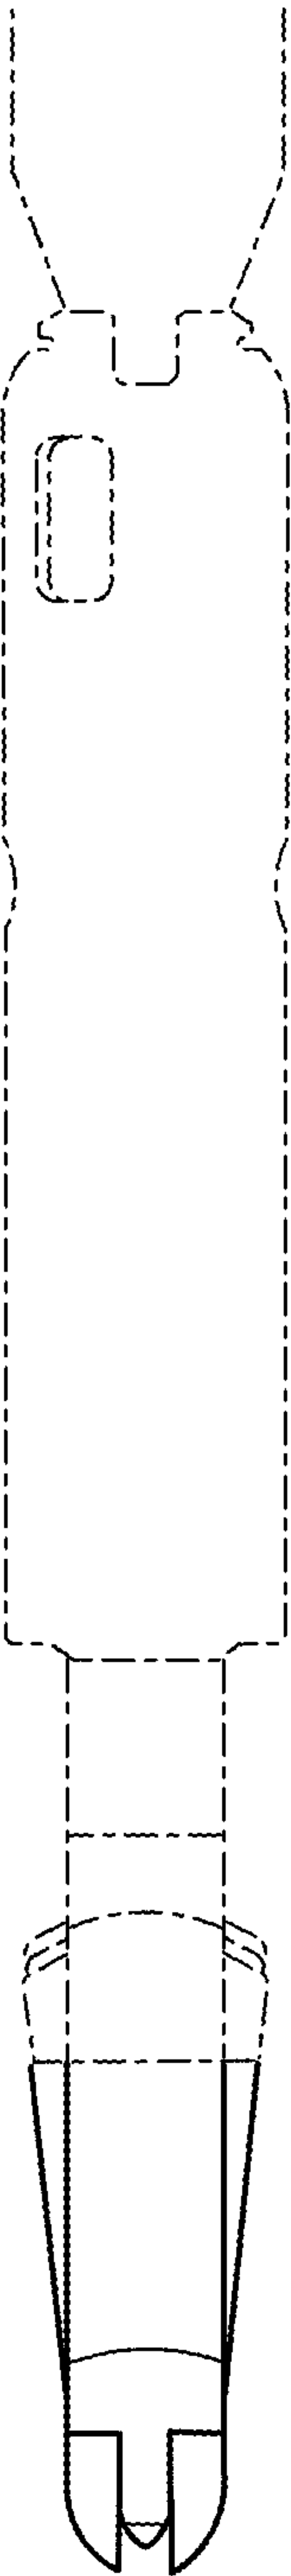


FIG. 7

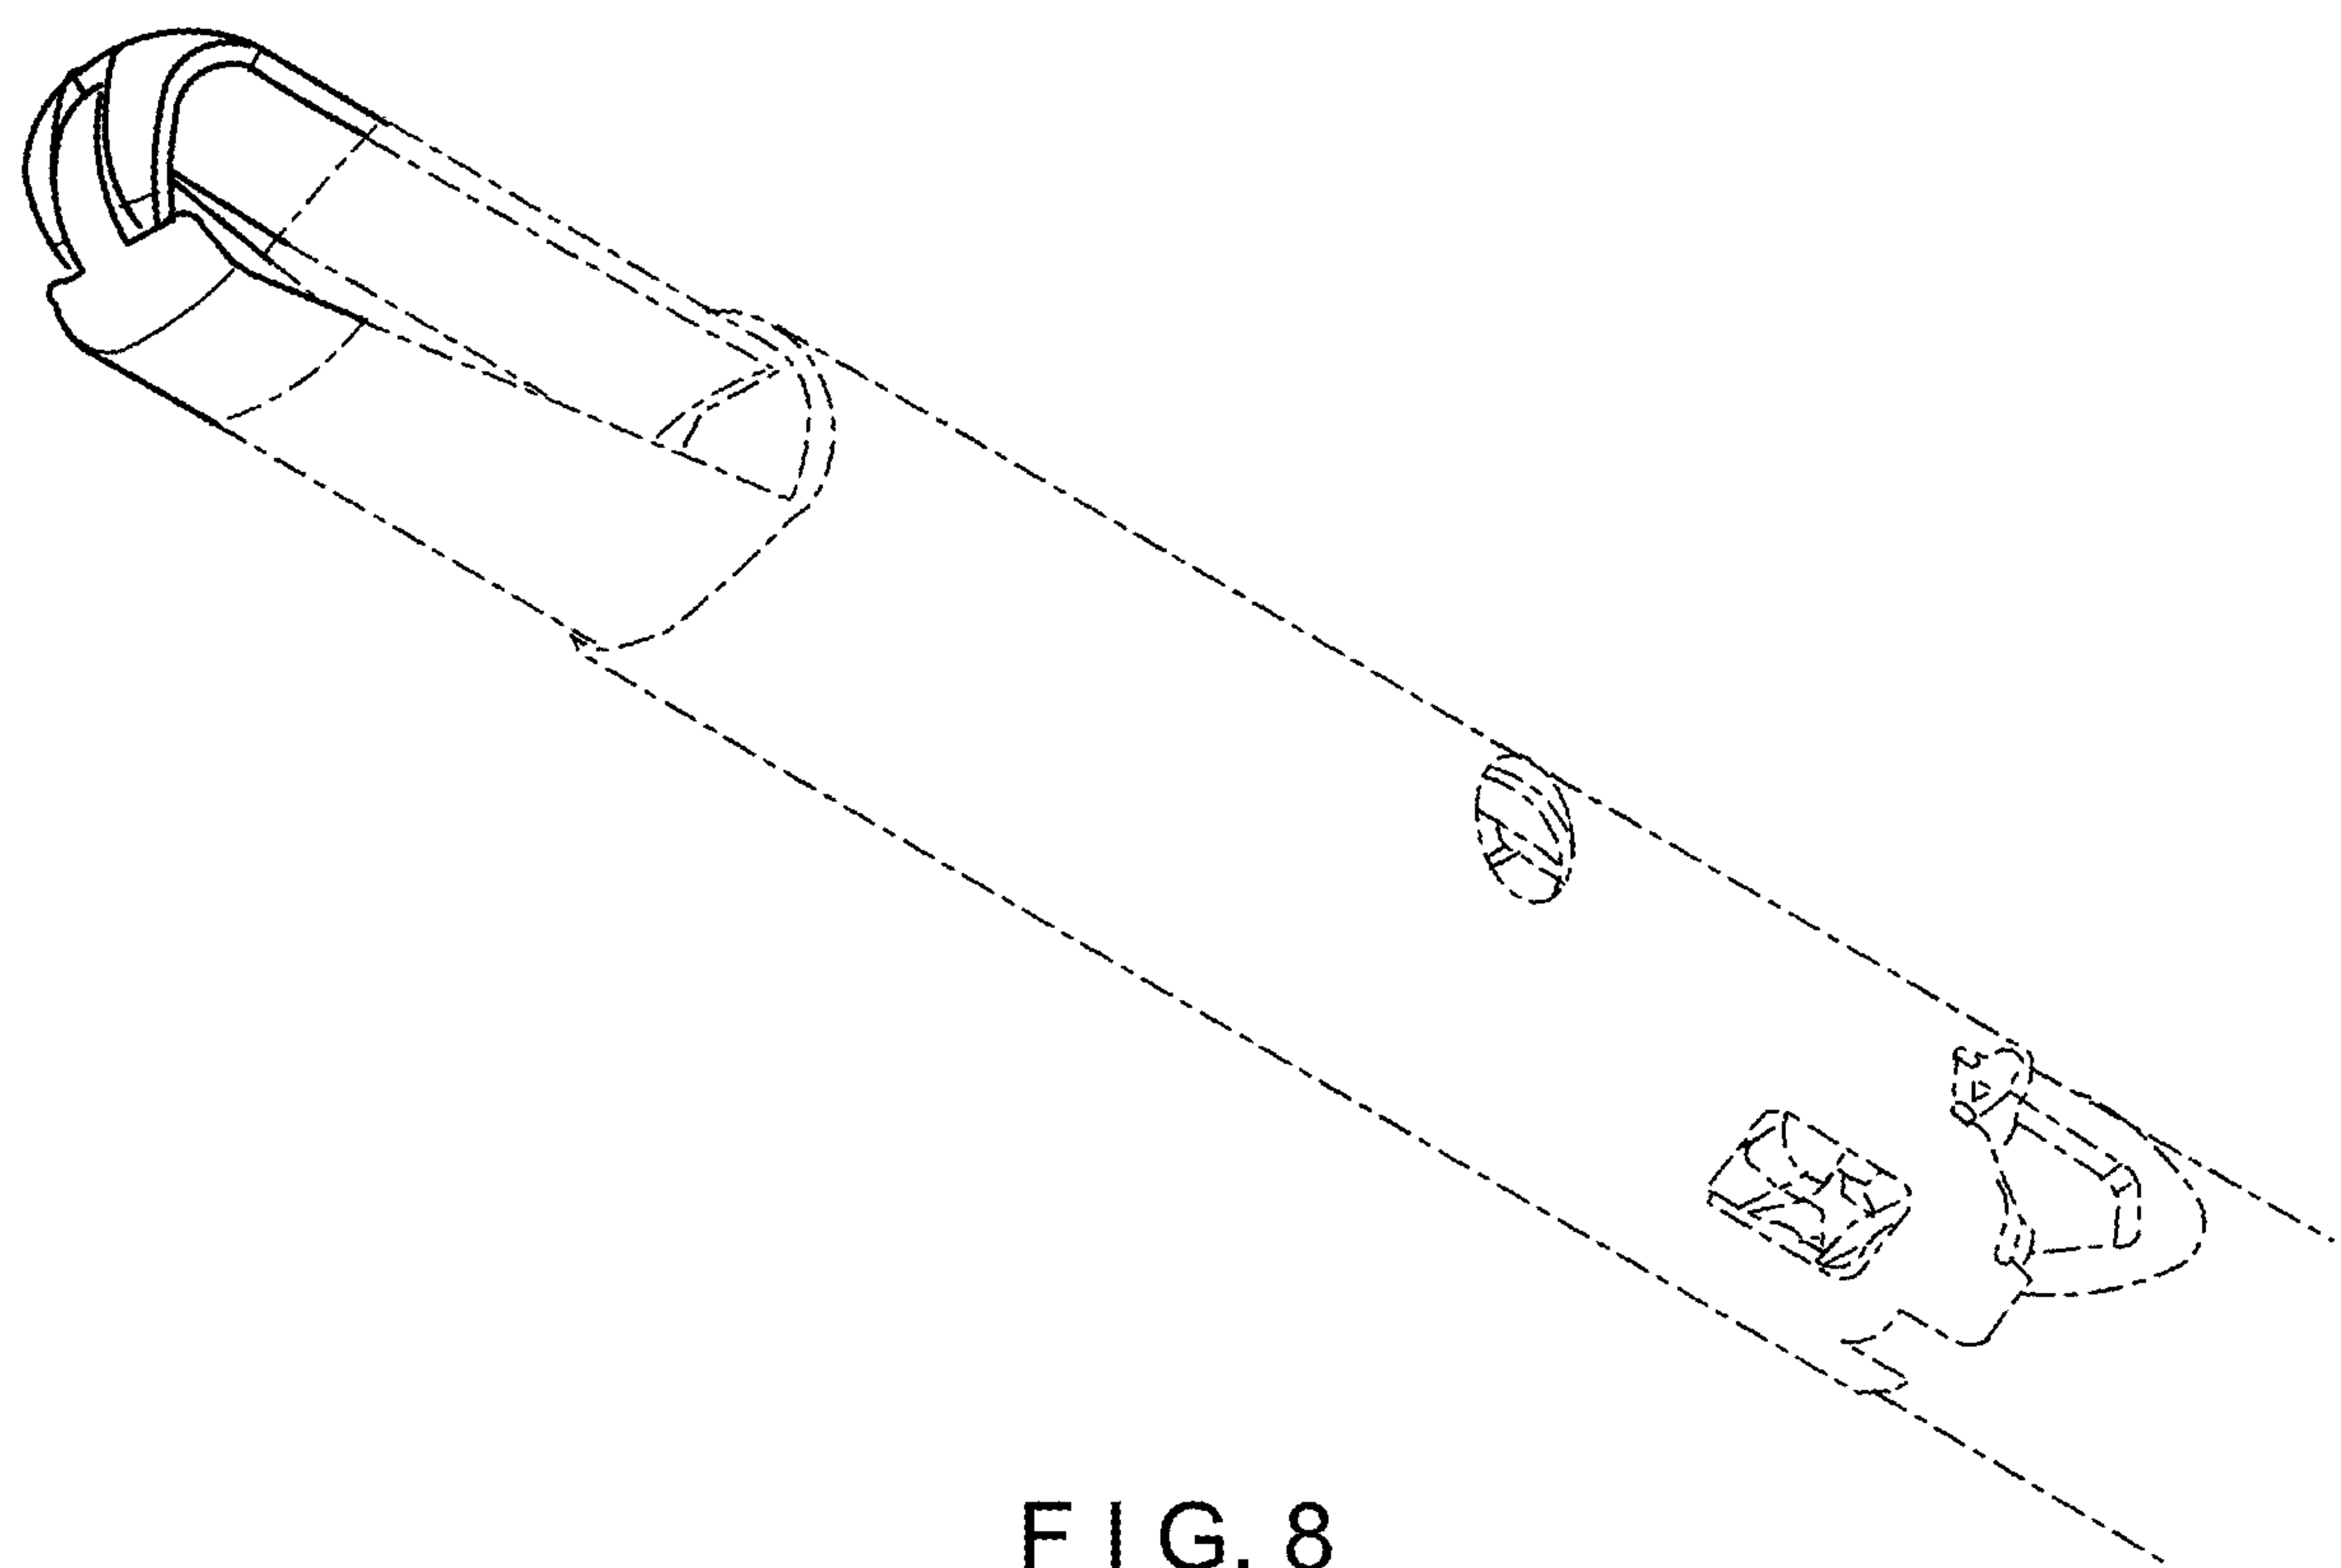


FIG. 8

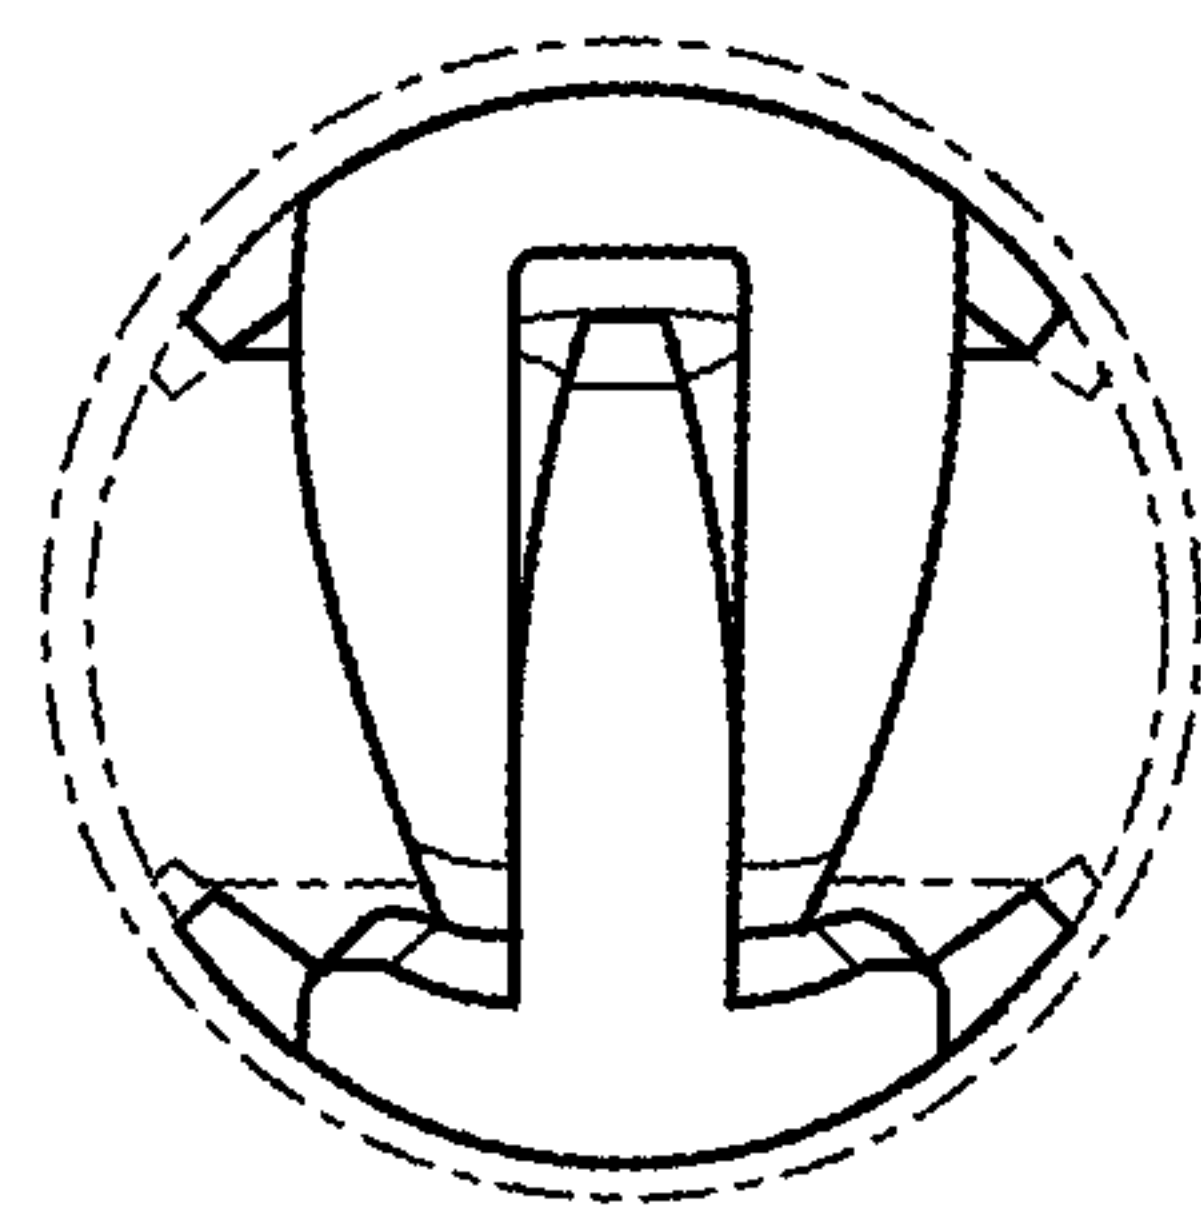


FIG. 9

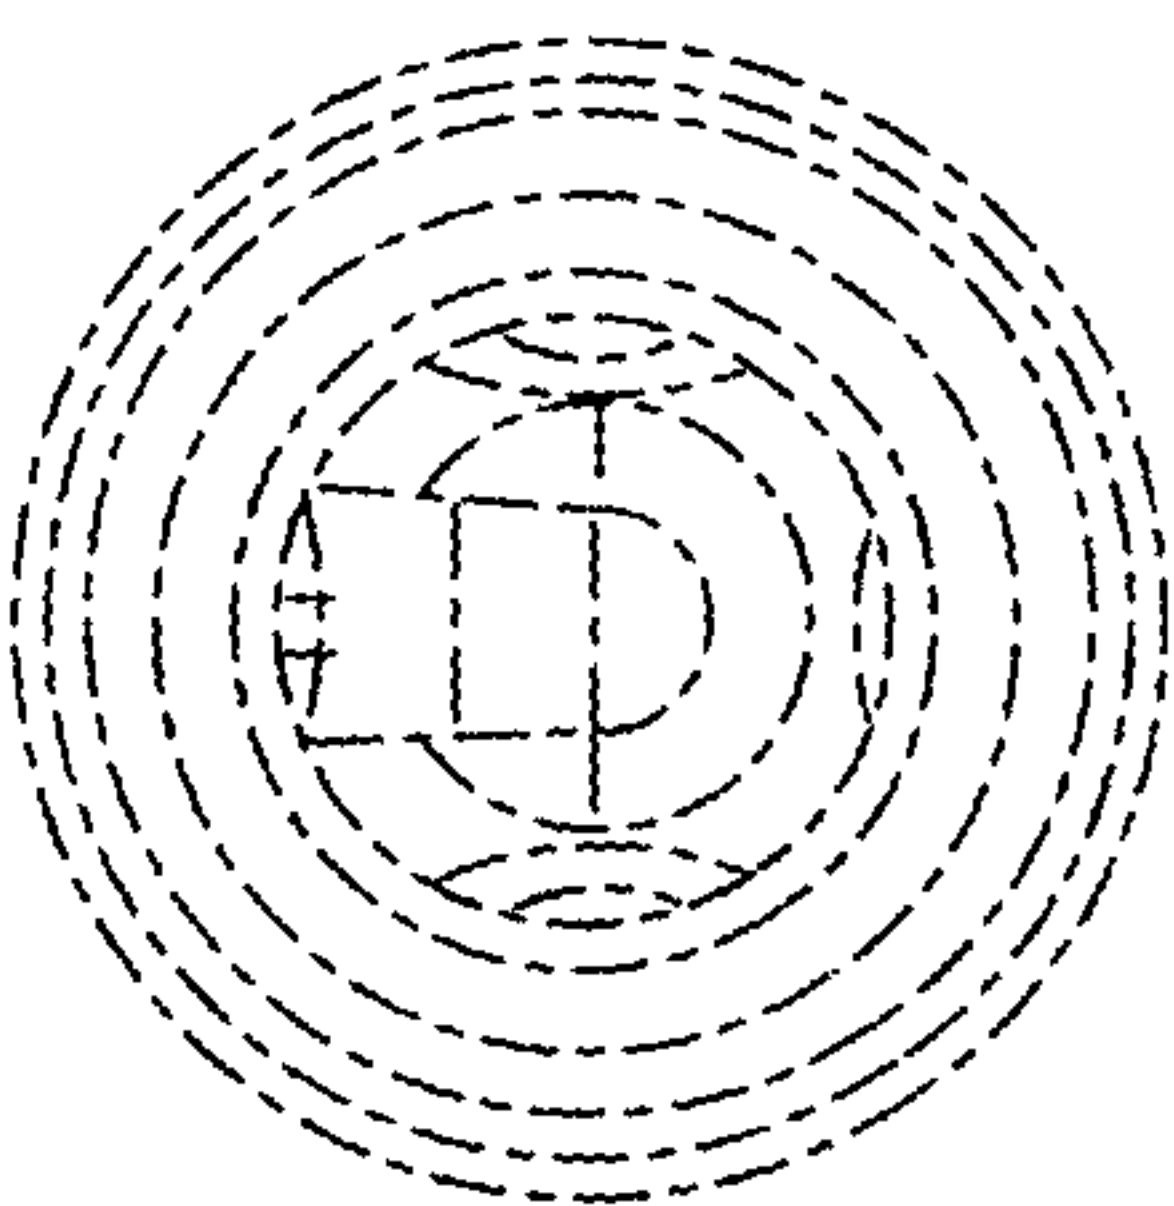


FIG. 10



FIG. 11



FIG. 12

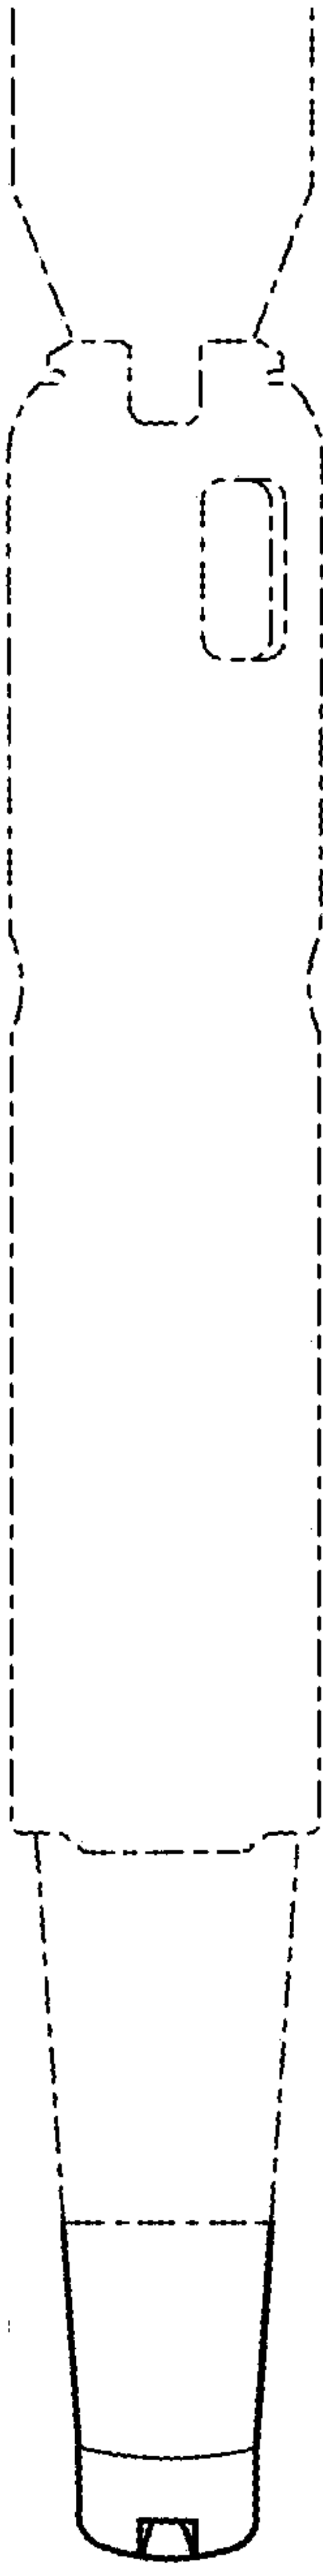


FIG. 13

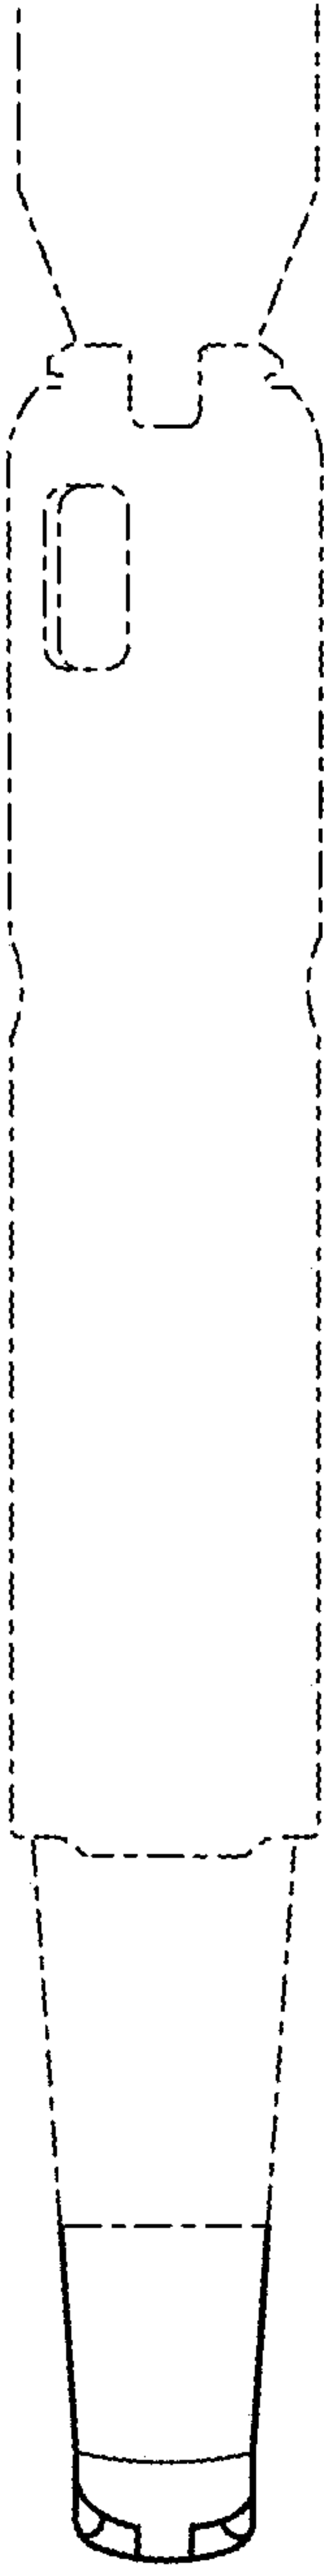


FIG. 14