



US00D950069S

(12) **United States Design Patent**  
**Ogura**

(10) **Patent No.:** **US D950,069 S**

(45) **Date of Patent:** **\*\* Apr. 26, 2022**

(54) **ULTRASOUND PROBE**

(71) Applicant: **FUJIFILM Corporation**, Tokyo (JP)

(72) Inventor: **Ryosuke Ogura**, Ashigara-kami-gun (JP)

(73) Assignee: **FUJIFILM Corporation**, Tokyo (JP)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/721,850**

(22) Filed: **Jan. 23, 2020**

(51) **LOC (13) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/187**

(58) **Field of Classification Search**  
USPC ..... D24/133, 137, 138, 141, 158, 160, 164,  
D24/165, 167, 170, 186, 187, 200;  
D10/57, 60, 78, 80  
CPC ..... A61B 8/565; A61B 8/4455; A61B 5/0095;  
A61B 8/4444; G01N 29/24; G01S 7/5208  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

8,137,281	B2 *	3/2012	Huang	.....	A61B 8/0833 600/461
D879,298	S *	3/2020	Byung	.....	D24/165
10,816,650	B2 *	10/2020	Solek	.....	A61B 8/4488
D910,857	S *	2/2021	Shibayama	.....	D24/187
D916,295	S *	4/2021	Shibayama	.....	D24/187
D919,102	S *	5/2021	Ogura	.....	D24/187
2016/0113724	A1 *	4/2016	Stolka	.....	A61B 34/20 600/424
2018/0110497	A1 *	4/2018	Beacham	.....	B33Y 80/00

**OTHER PUBLICATIONS**

Wireless B&W Ultrasound Probe—CONVEX-3.5/ 5.0MHZ. Online, published date unknown. Retrieved on Jun. 30, 2021 from URL: <https://interaktivhealth.com.au/products/wireless-ultrasound-scanner-ss-2ii-convex-3-5-5-0mhz>.\*

Ultrasound Diagnostic Imaging Equipment. Online, published date unknown. Retrieved on Jun. 30, 2021 from URL: <http://www-gmark-org-product.elasticbeanstalk.com/award/describe/49151?locale=en>.\*

\* cited by examiner

*Primary Examiner* — Susan Bennett Hattan

*Assistant Examiner* — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Birch, Stewart, Kolasch & Birch, LLP


(57) **CLAIM**

The ornamental design for an ultrasound probe, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of an ultrasound probe showing my new design,  
FIG. 2 is a front view of the ultrasound probe,  
FIG. 3 is a back view of the ultrasound probe,  
FIG. 4 is a top view of the ultrasound probe,  
FIG. 5 is a bottom view of the ultrasound probe,  
FIG. 6 is a right side view of the ultrasound probe; and,  
FIG. 7 is a left side view of the ultrasound probe.  
In FIGS. 1-4, the broken lines depict portions of the ultrasound probe that form no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

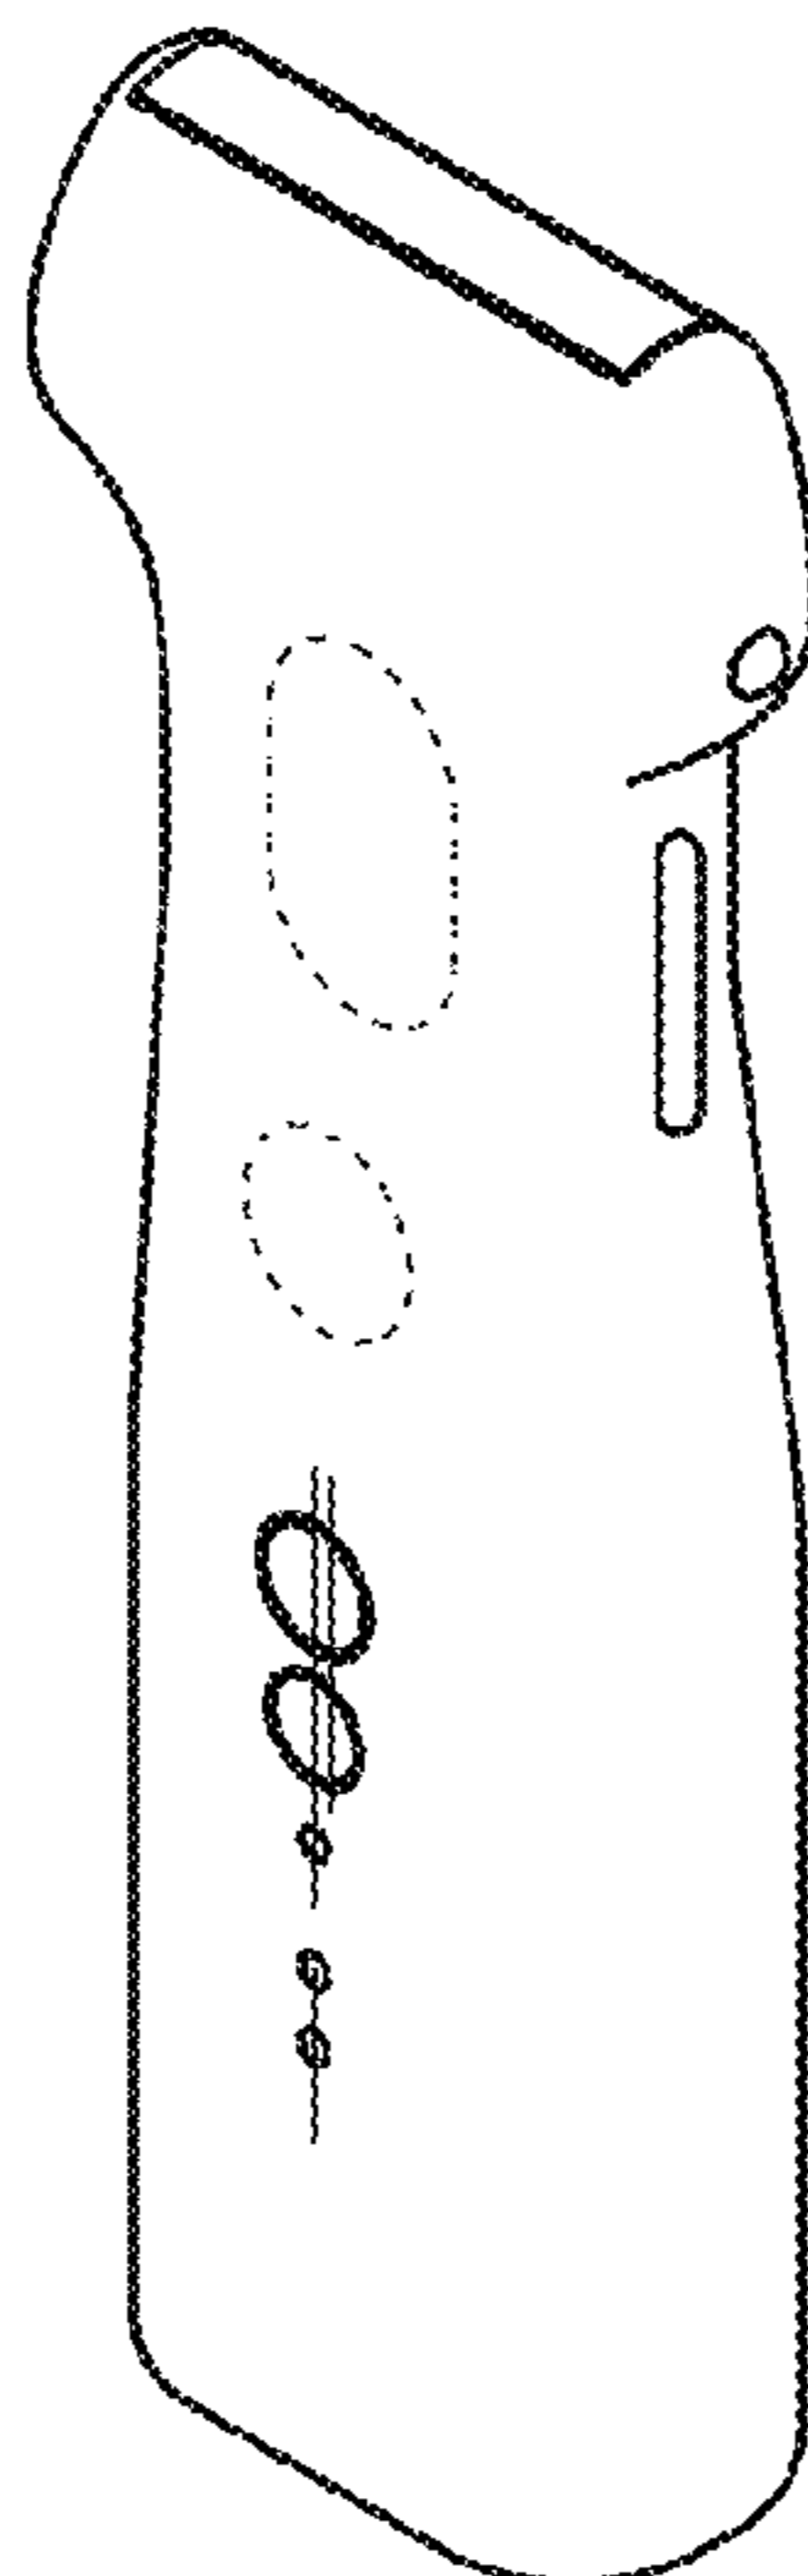

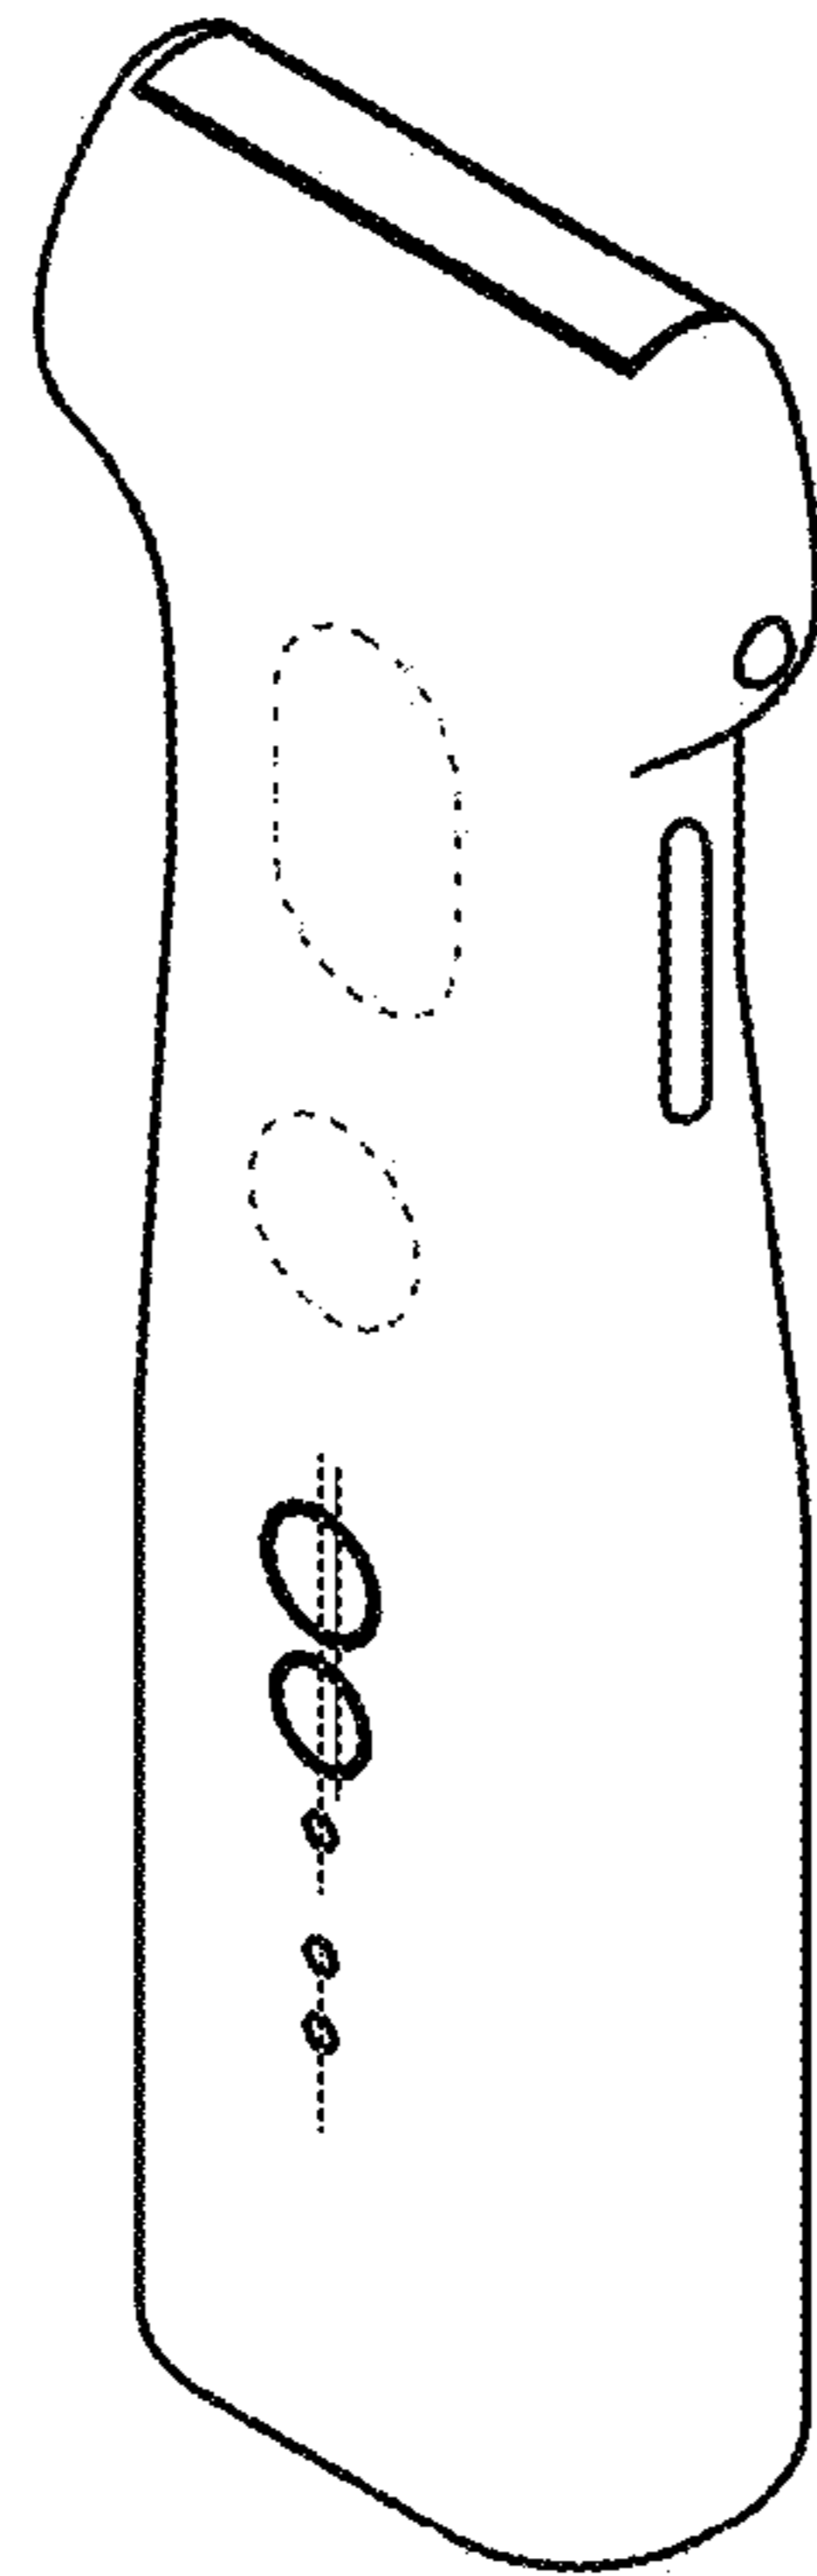


FIG. 1

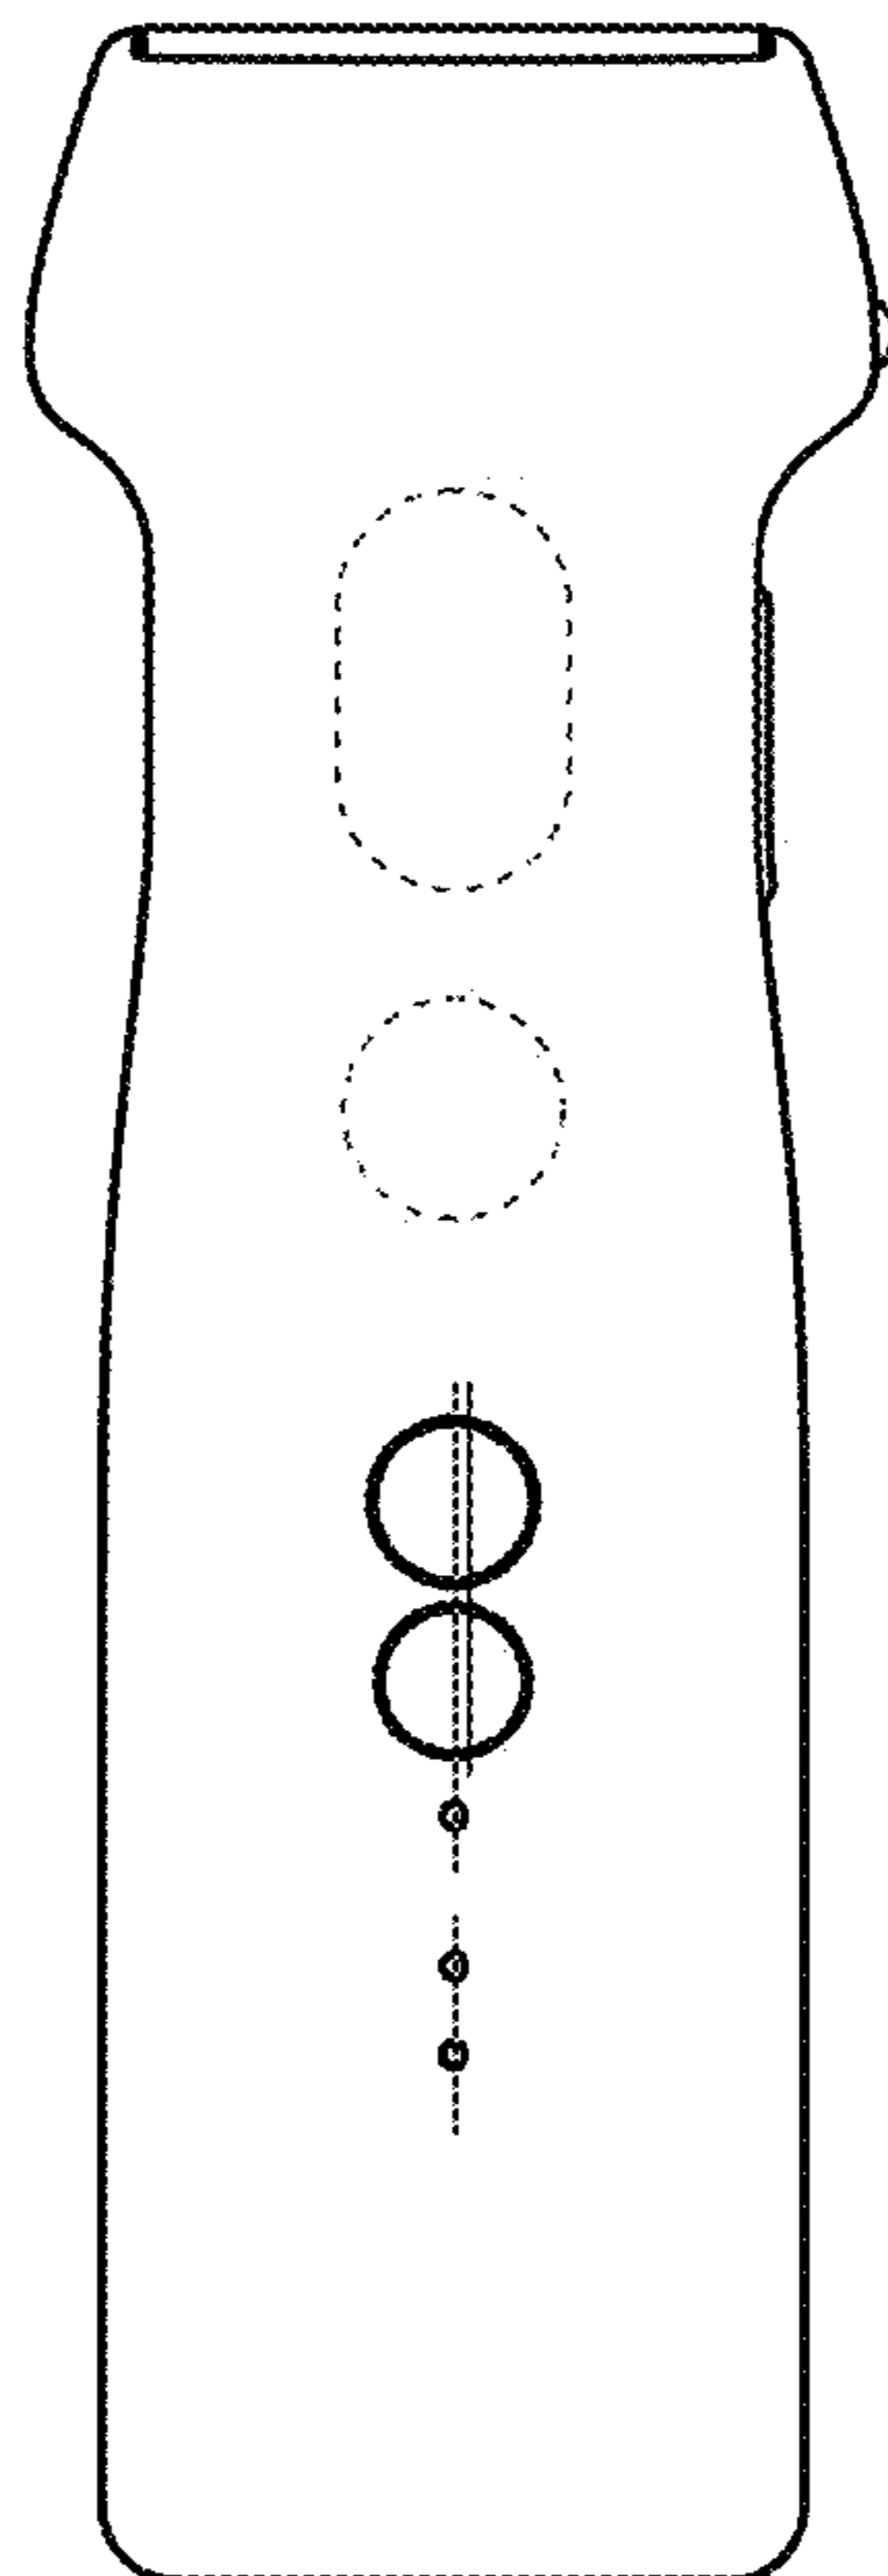


FIG. 2

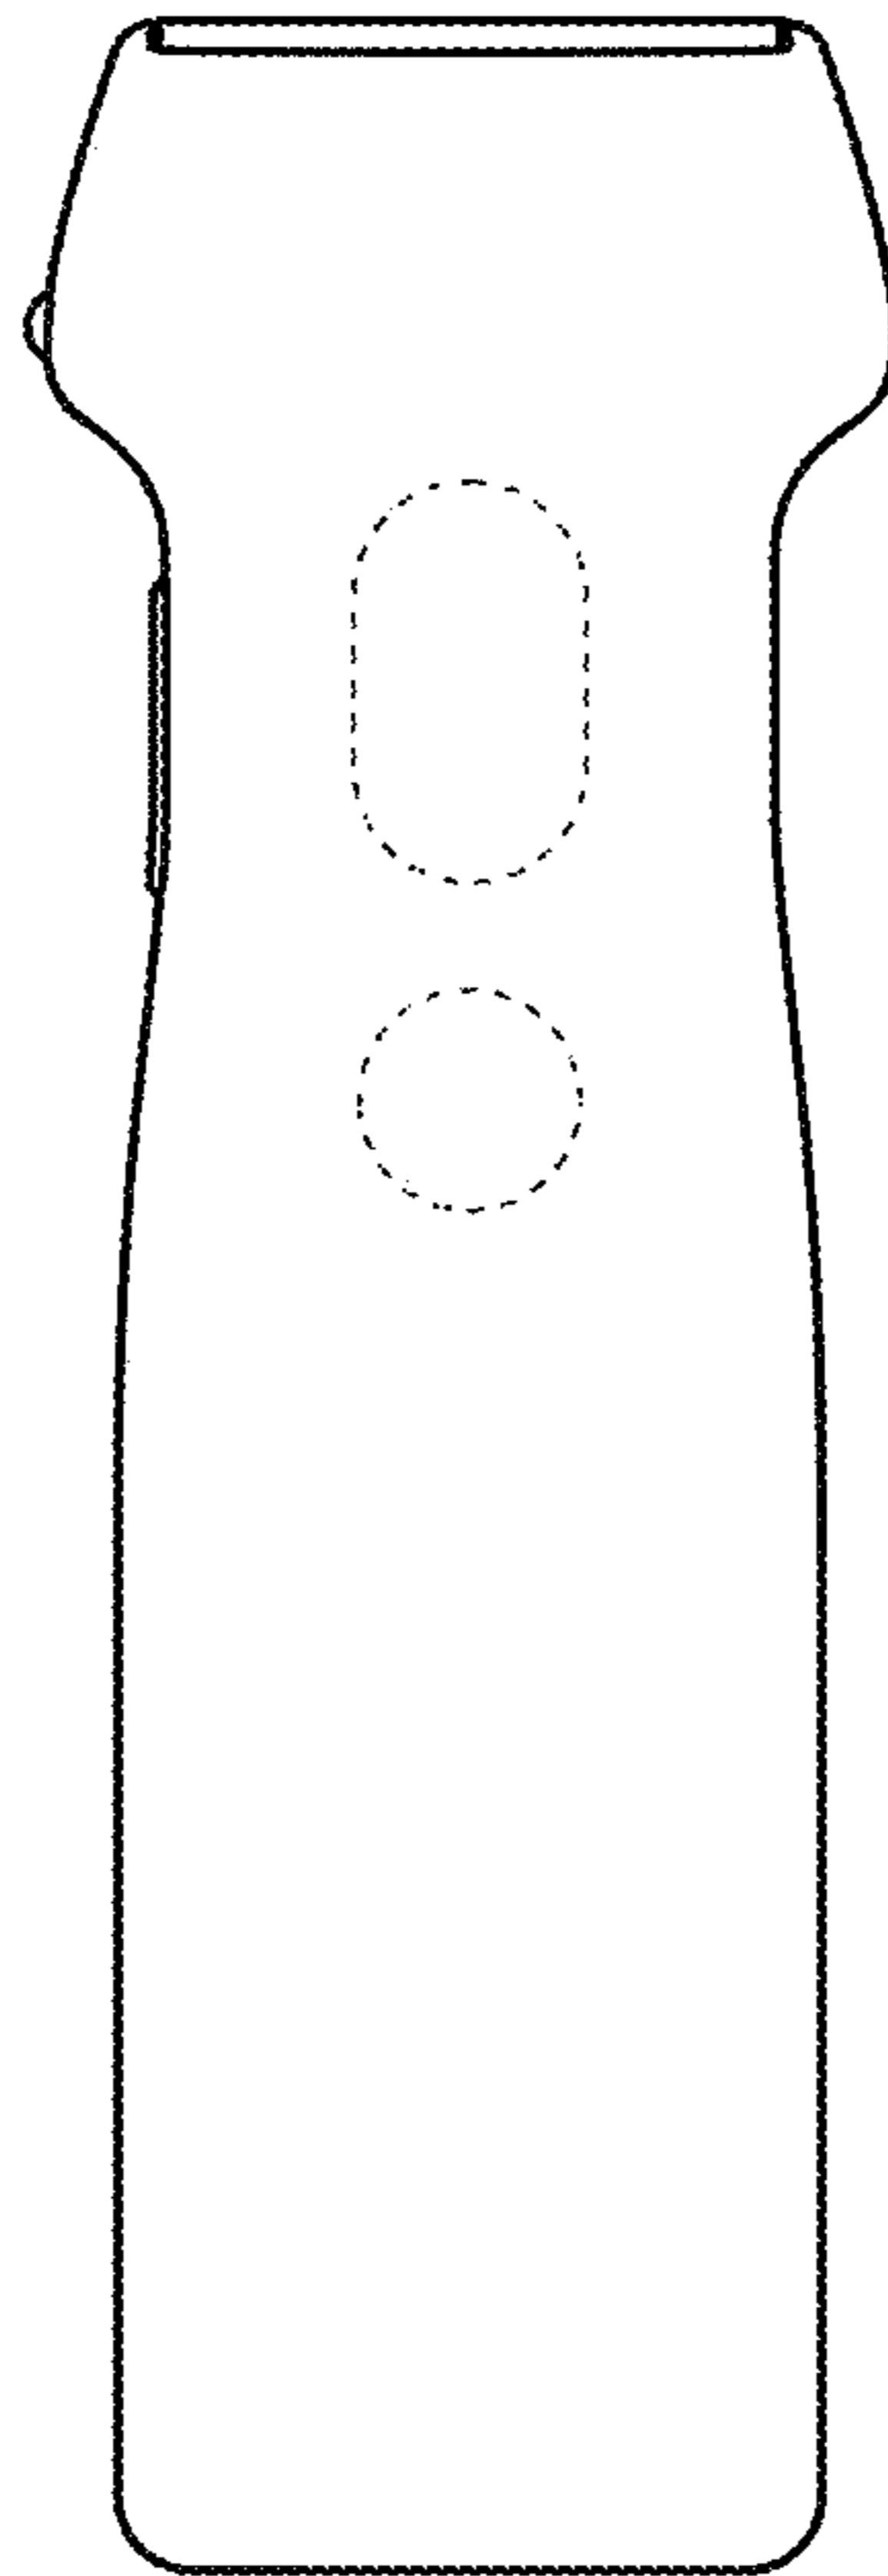


FIG. 3

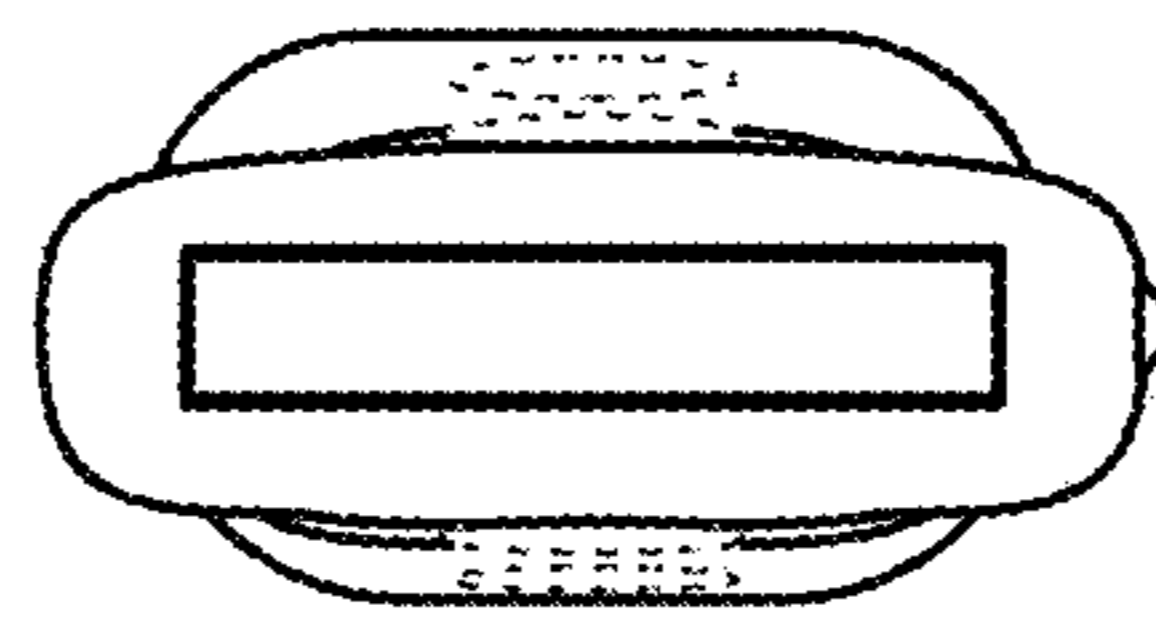


FIG. 4

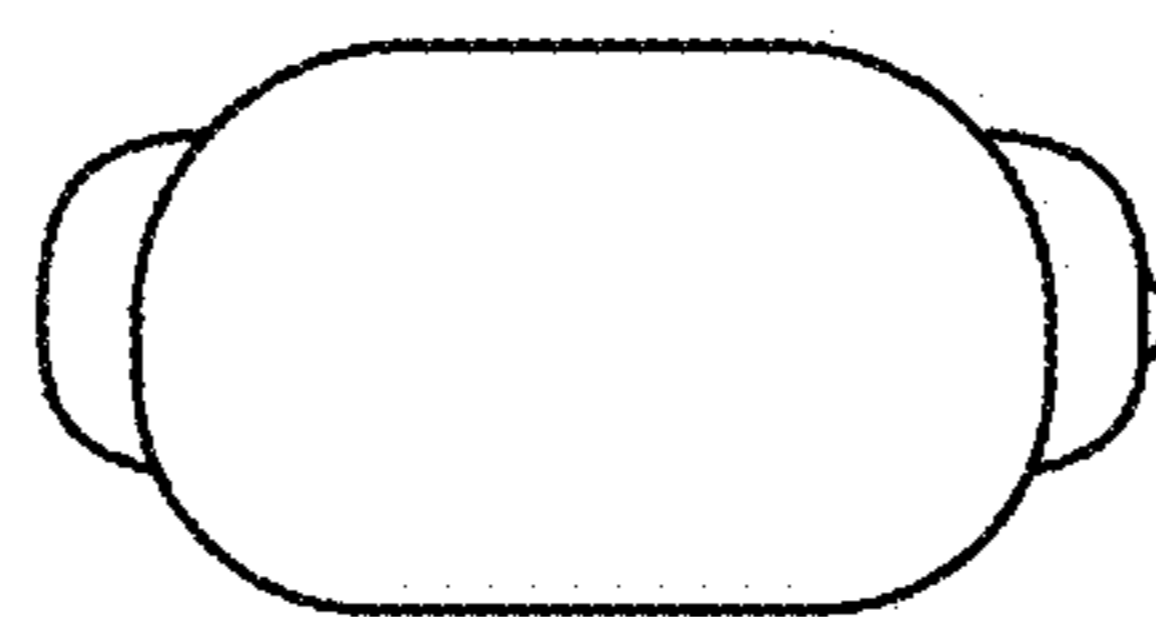


FIG. 5

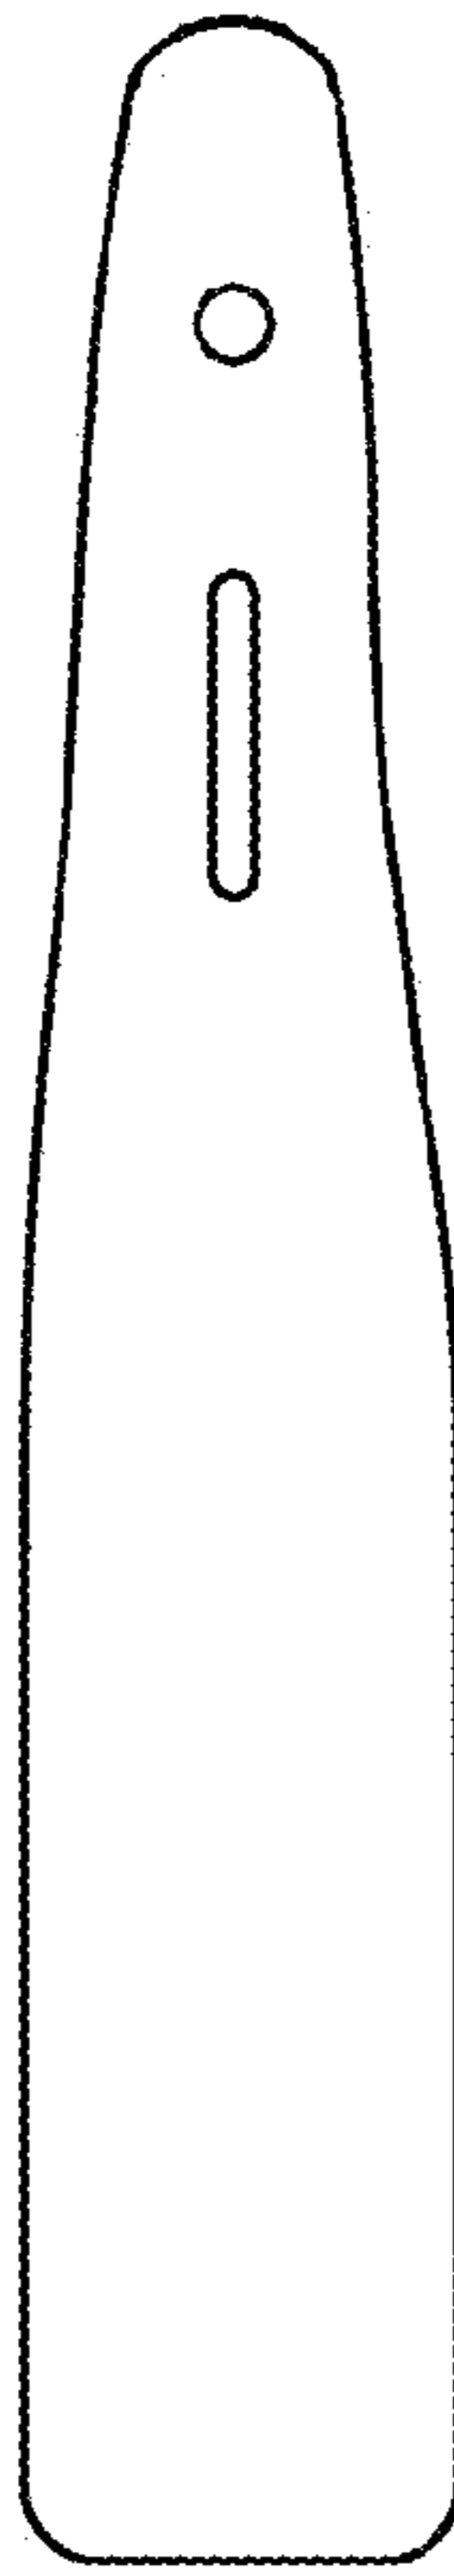


FIG. 6

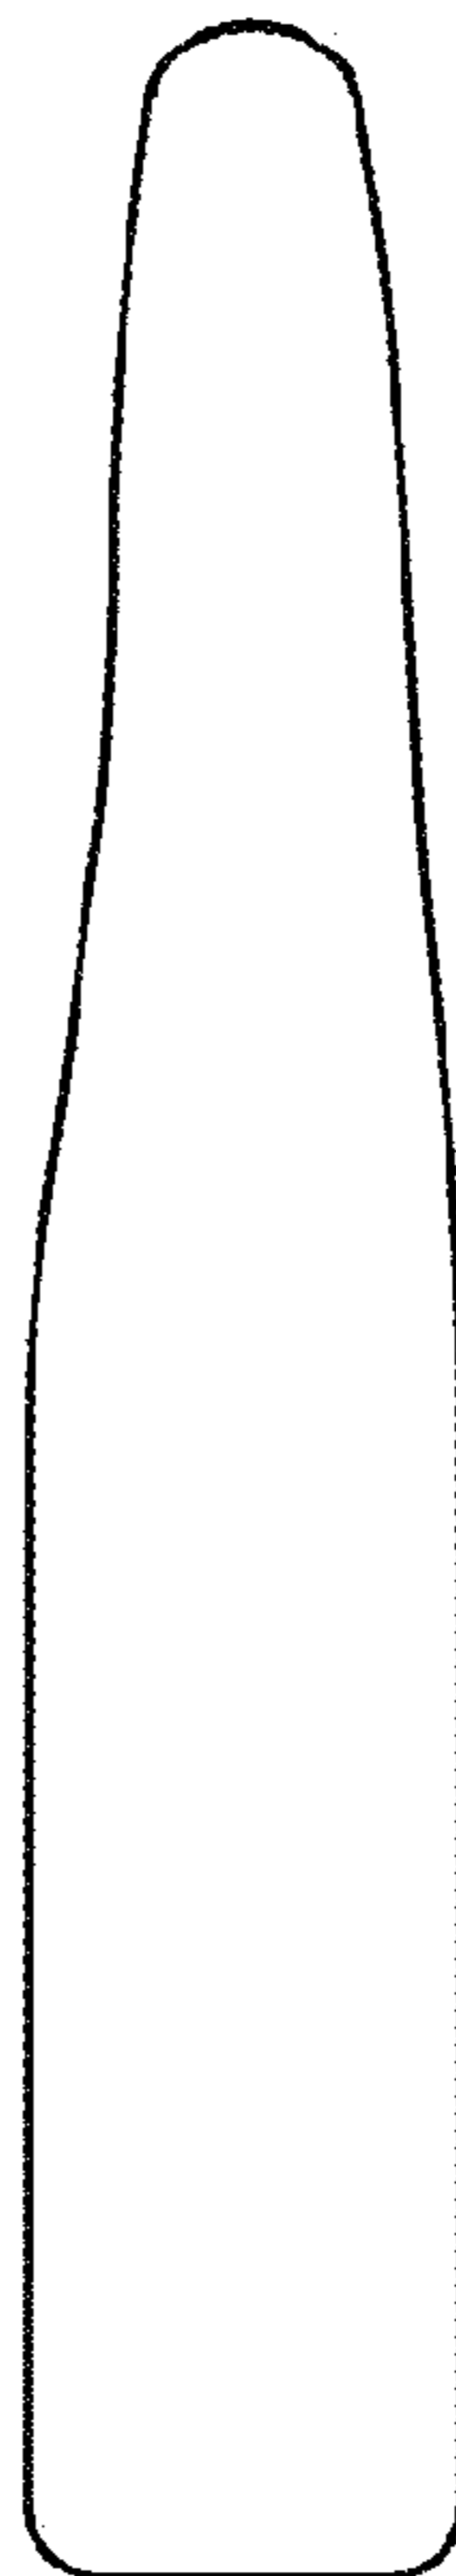


FIG. 7