



US00D950727S

(12) **United States Design Patent**
Dilbert et al.

(10) **Patent No.:** **US D950,727 S**

(45) **Date of Patent:** **** May 3, 2022**

(54) **MEDICAL DEVICE WITH A CURVE WITH A PROXIMAL CURVE INDICATOR**

(71) Applicant: **BAYLIS MEDICAL COMPANY INC.**, Montreal (CA)

(72) Inventors: **Chevis Delano Dilbert**, Toronto (CA); **David Jonathan Rees**, Toronto (CA); **James Dylan Klein**, Toronto (CA); **Thomas Barrett**, York (CA); **Yun Uhm**, North York (CA); **John Paul Urbanski**, Toronto (CA); **Jeffery D. Arnett**, Gilbert, AZ (US); **Moussa Chehade**, Toronto (CA); **Lyndsay Stephenson**, Toronto (CA); **Marina Spyridis**, Etobicoke (CA)

(73) Assignee: **Baylis Medical Company Inc.**, Mississauga (CA)

(**) Term: **15 Years**

(21) Appl. No.: **29/704,396**

(22) Filed: **Sep. 4, 2019**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/144**

(58) **Field of Classification Search**
USPC D24/133, 144, 146-147

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,537,193 A * 8/1985 Tanner A61B 18/24
D24/144

5,389,090 A * 2/1995 Fischell A61M 25/0662
604/528

(Continued)

Primary Examiner — Wan Laymon

(74) *Attorney, Agent, or Firm* — Glenn Arnold; Vincent Man; Samuel Tekle

(57) **CLAIM**

The ornamental design for a medical device with a curve with a proximal curve indicator, as shown and described.

DESCRIPTION

FIG. 1 is a front, left and top perspective view of a medical device with a curve with a proximal curve indicator showing our new design;

FIG. 2 is a left side view of the medical device of FIG. 1; FIG. 3 is a front view of the medical device of FIG. 1, shown at an enlarged view;

FIG. 4 is a rear view of the medical device of FIG. 1, shown at an enlarged view;

FIG. 5 is a right side view of the medical device of FIG. 1; FIG. 6 is a top plan view of the medical device of FIG. 1, shown at an enlarged view;

FIG. 7 is a bottom plan view of the medical device of FIG. 1, shown at an enlarged view;

FIG. 8 is a front, left and top perspective view of an alternative embodiment of a medical device with a curve with a proximal curve indicator;

FIG. 9 is a left side view of the medical device of FIG. 8; FIG. 10 is a front view of the medical device of FIG. 8, shown at an enlarged view;

FIG. 11 is a rear view of the medical device of FIG. 8, shown at an enlarged view;



FIG. 12 is a right side view of the medical device of FIG. 8; FIG. 13 is a top plan view of the medical device of FIG. 8, shown at an enlarged view; and,

FIG. 14 is a bottom plan view of the medical device of FIG. 8, shown at an enlarged view.

The broken lines immediately adjacent the shaded areas represent the bounds of the claimed design while all other broken lines are directed to environment and are for illustrative purposes only; the broken lines form no part of the claimed design.

The broken away symbols in FIGS. 1-2, 5-9, and 12-24 indicate that any portion of the article beyond what is shown forms no part of the claimed design.

1 Claim, 10 Drawing Sheets

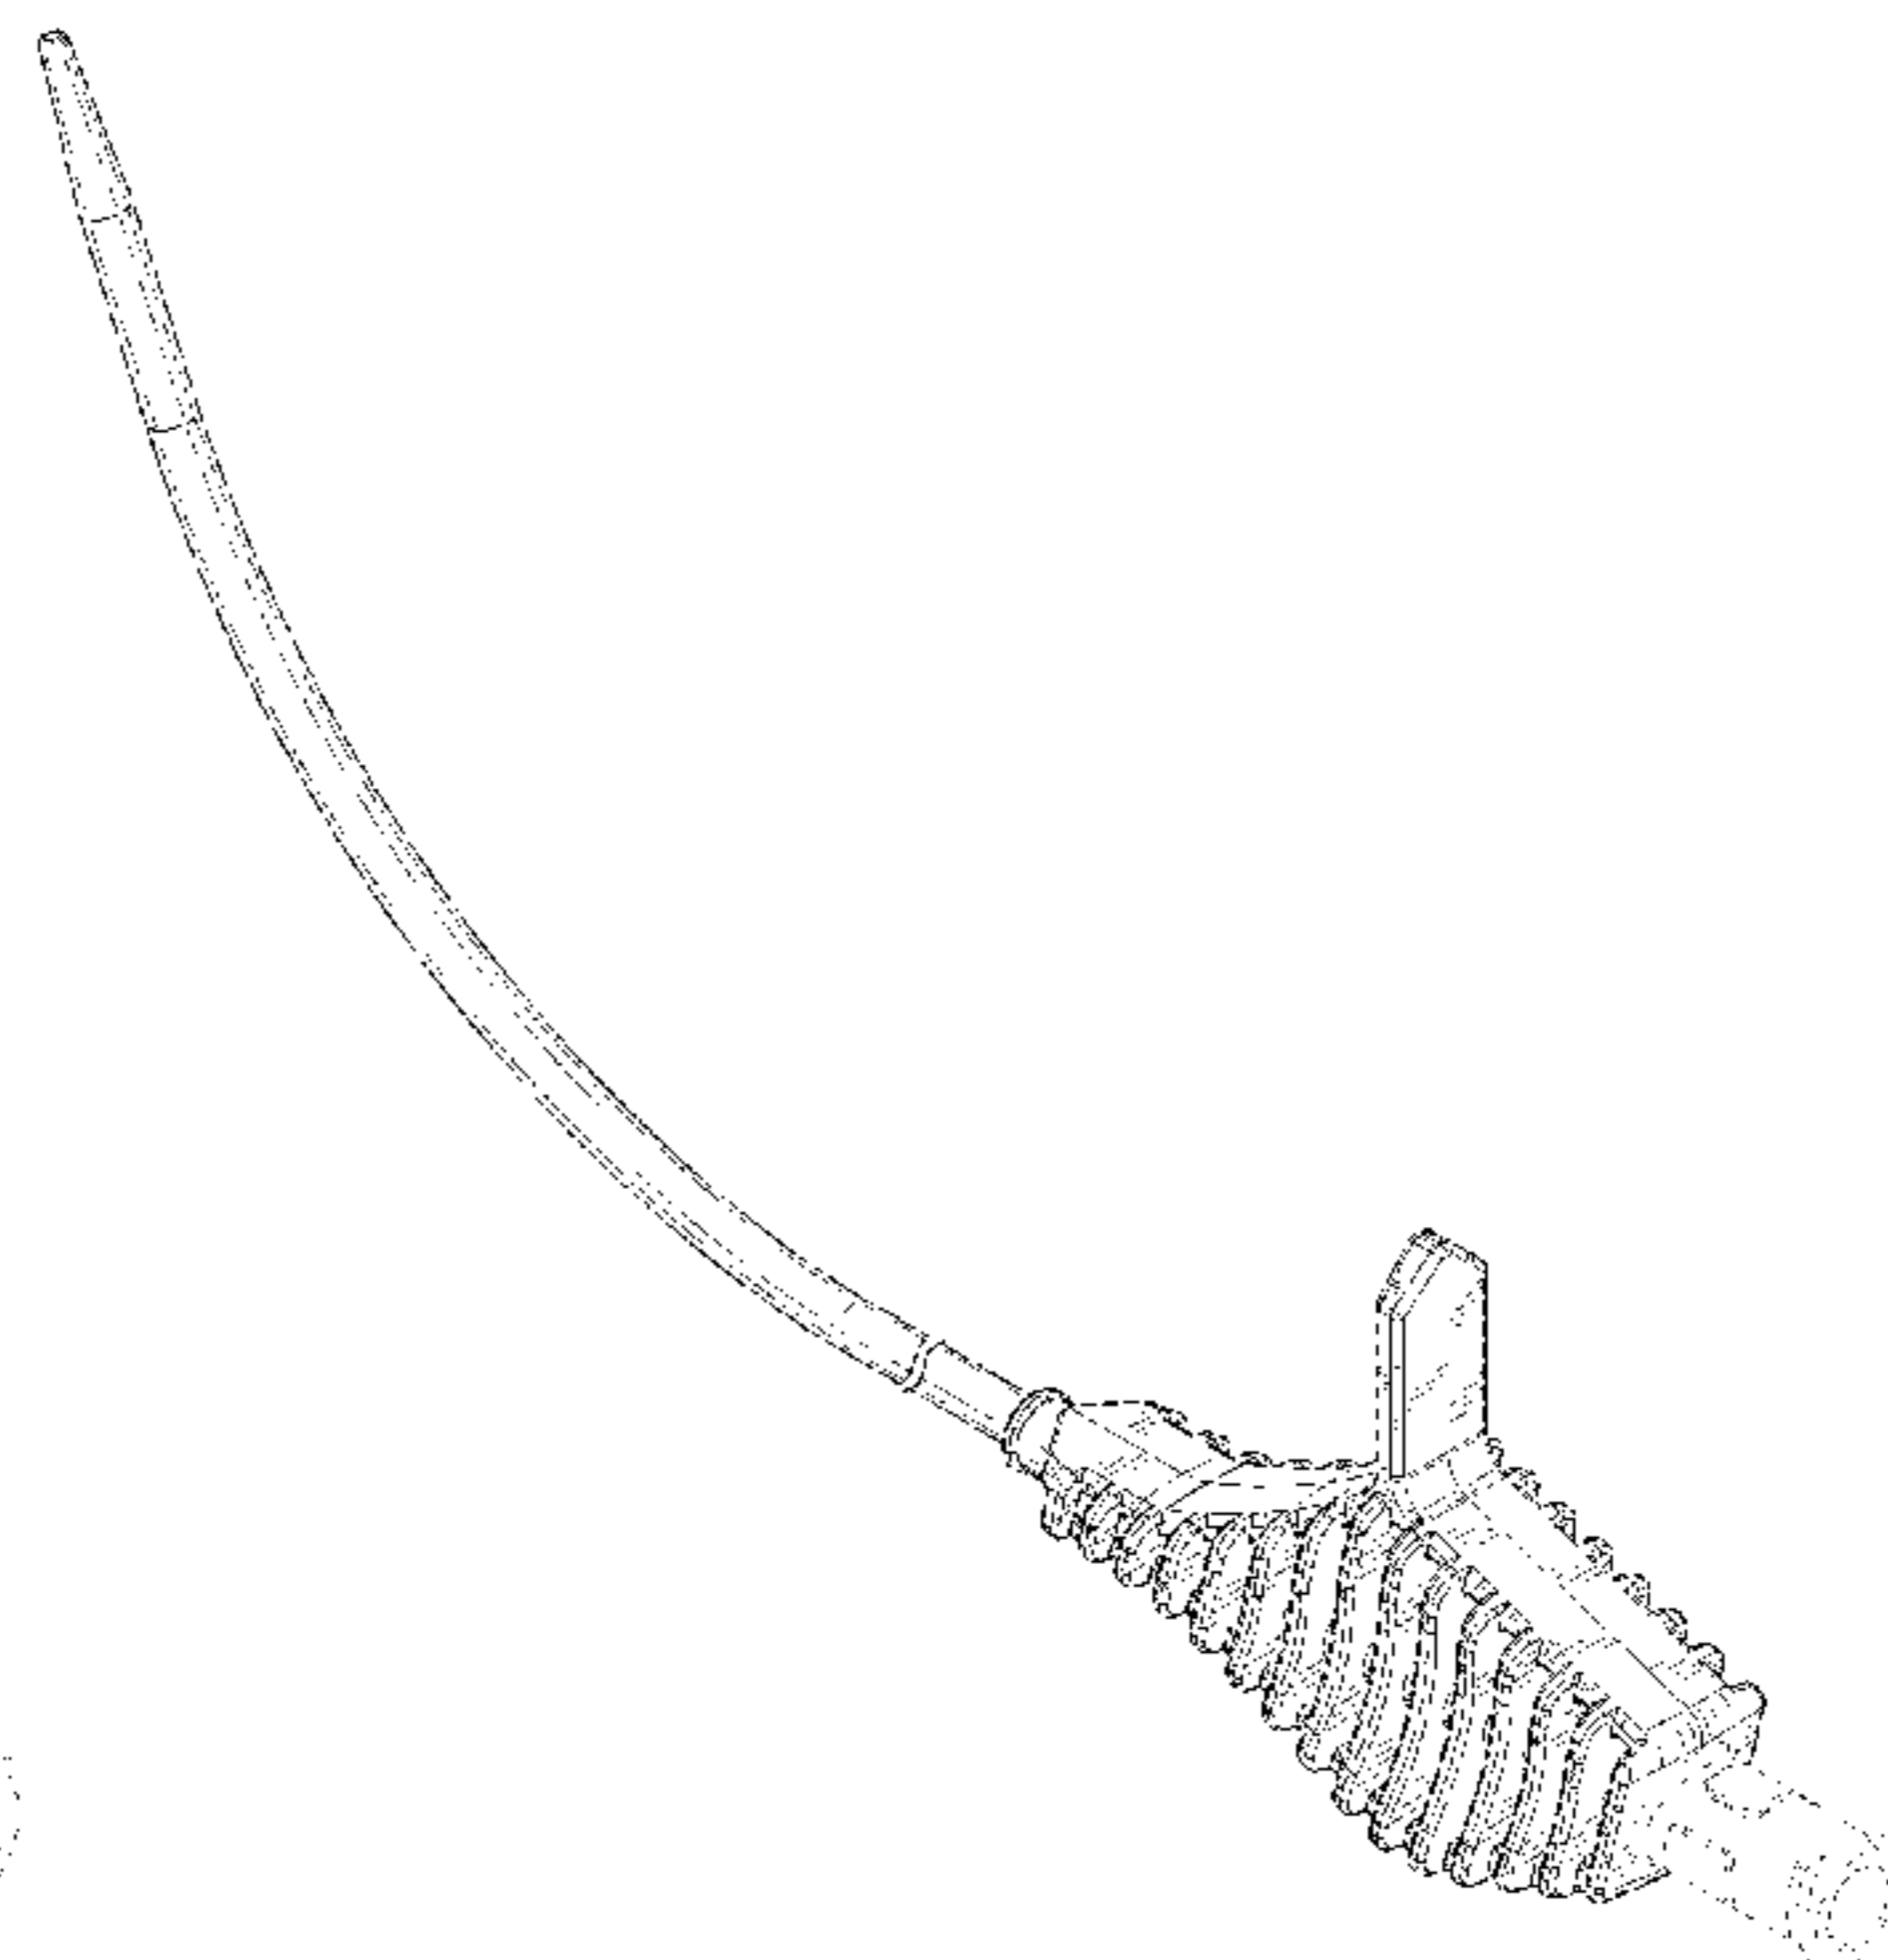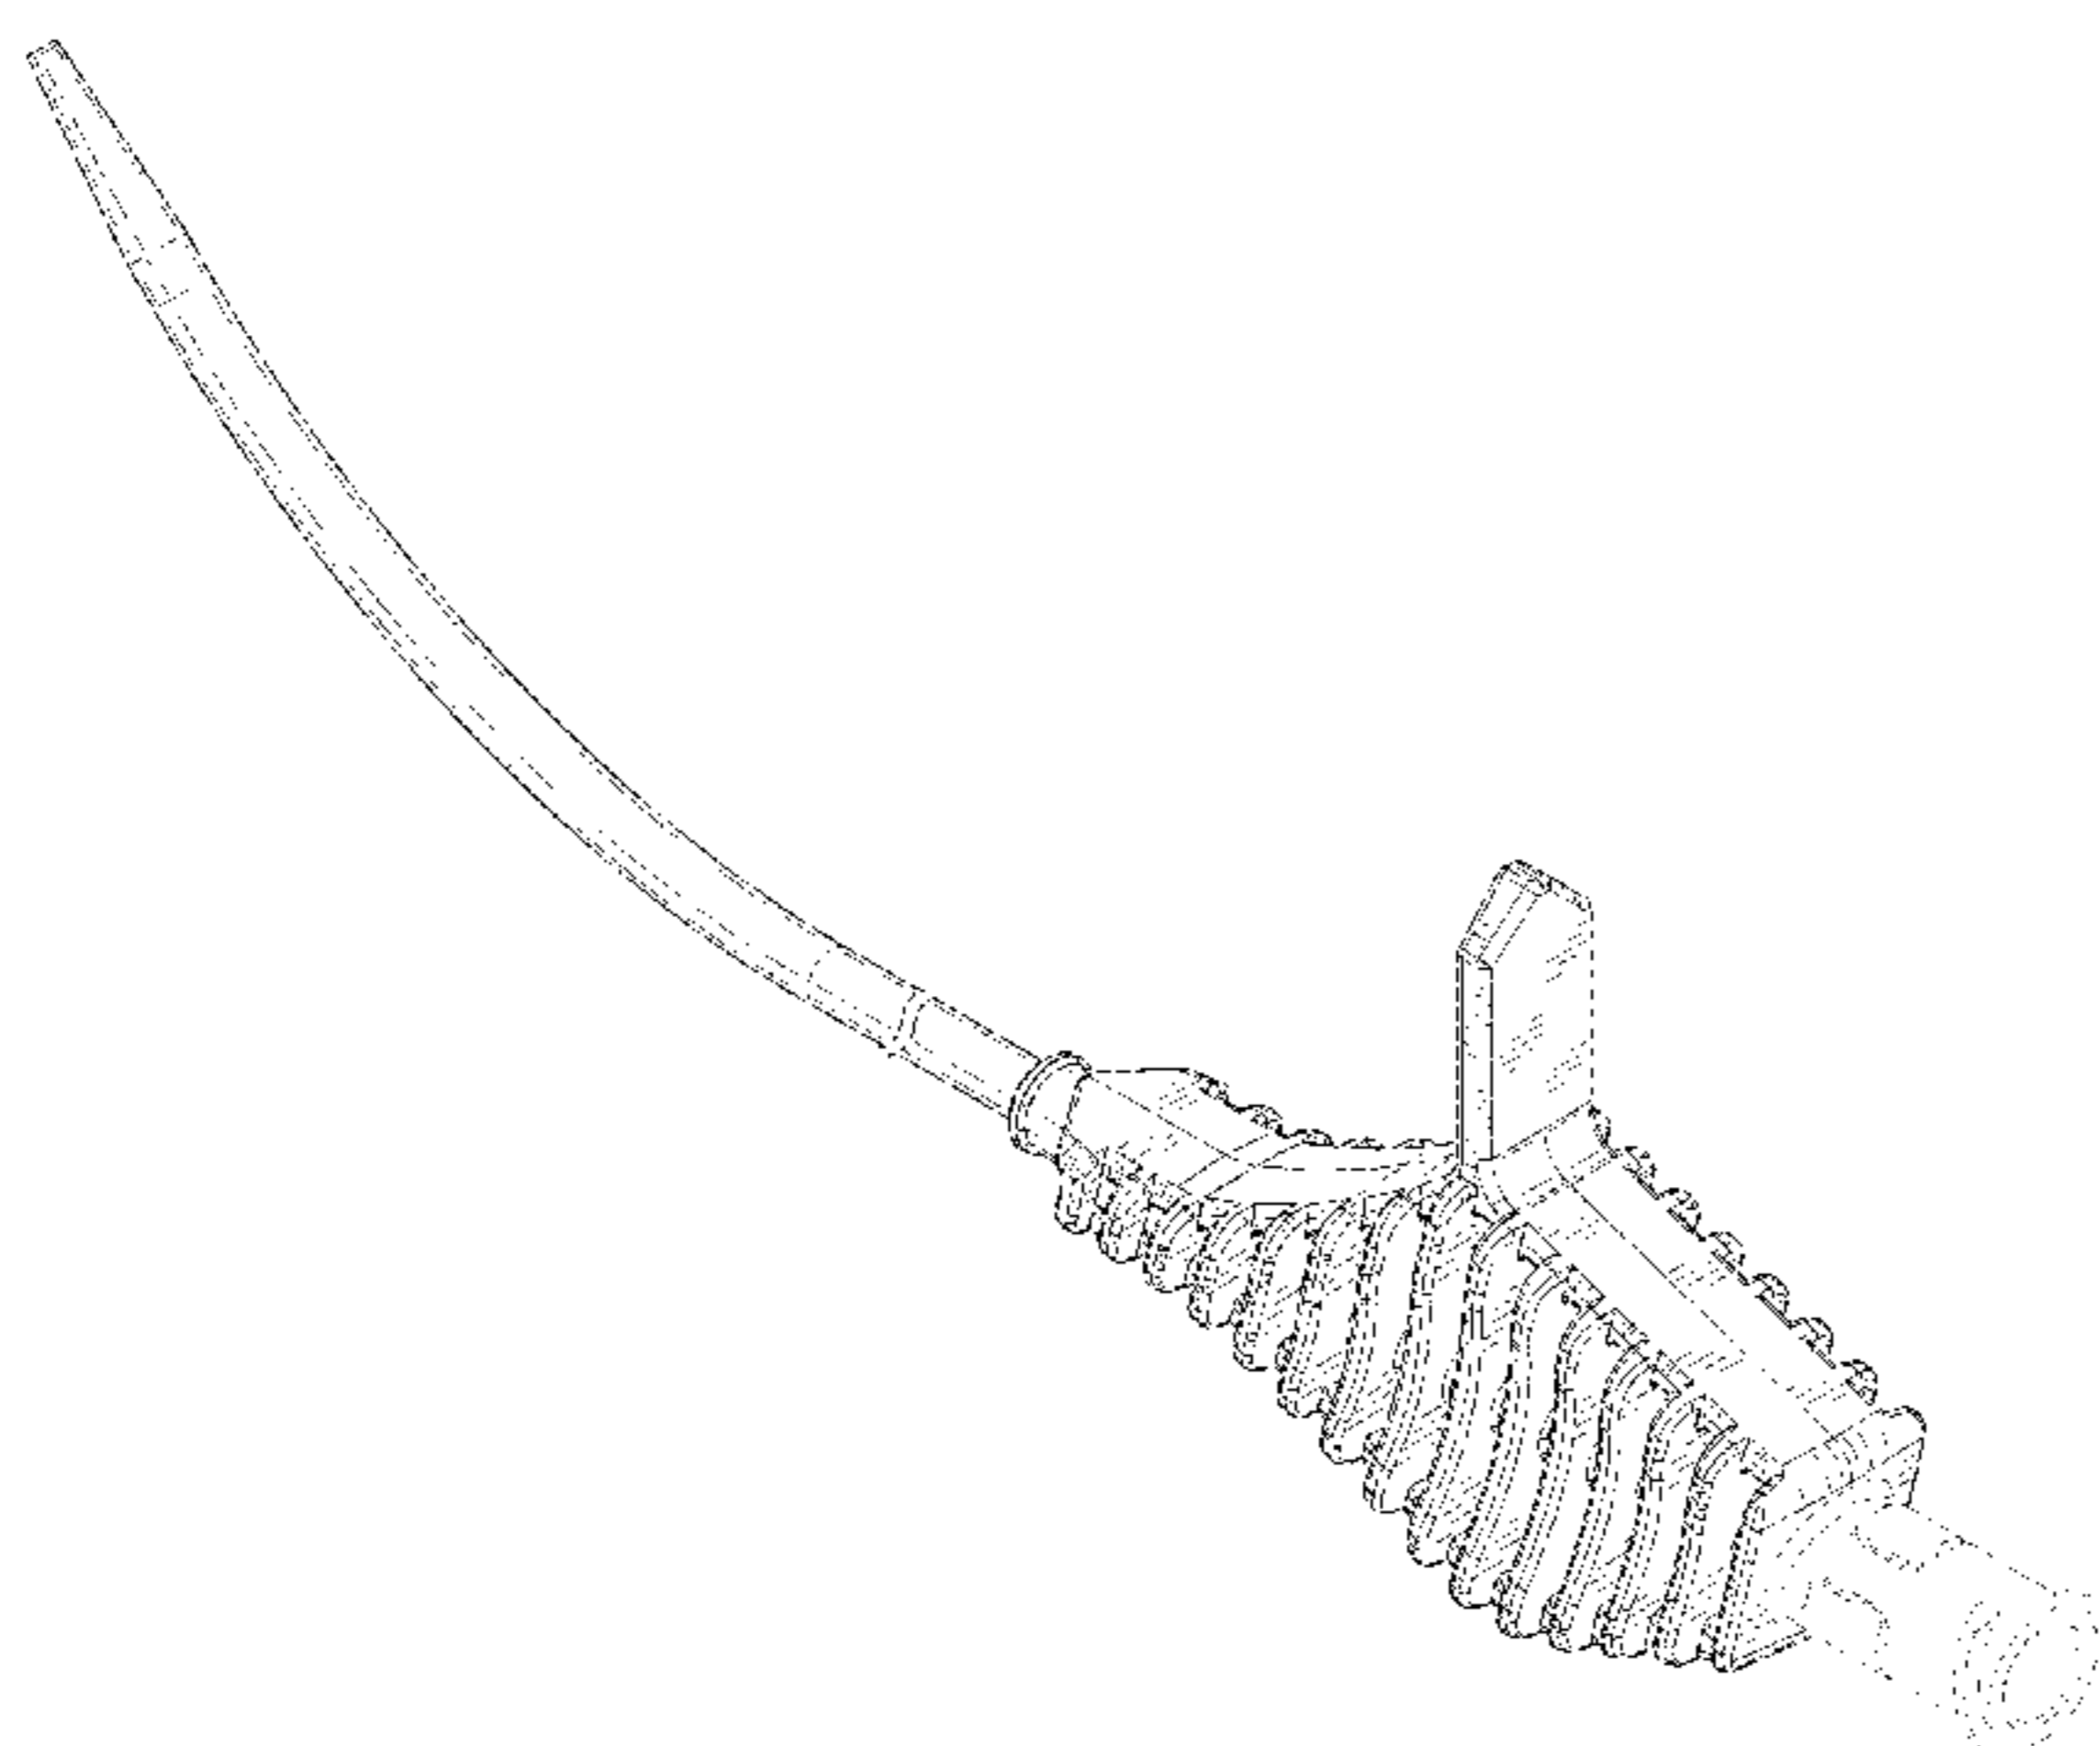

(58) **Field of Classification Search**

CPC A61M 25/0662; A61M 25/0136; A61B
18/1482; A61B 18/1487

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D683,452	S	*	5/2013	Davies	D24/144
D786,430	S	*	5/2017	Davies	D24/144
D818,586	S	*	5/2018	Hamel	D24/146
D847,988	S	*	5/2019	Schnitzer	D24/144
D854,155	S	*	7/2019	Arnett	D24/147
D914,211	S	*	3/2021	Hernandez Zendejas	...	D24/144
2020/0147360	A1	*	5/2020	Arnett	A61M 25/0662
2021/0068892	A1	*	3/2021	Urbanski	A61B 18/1487
2021/0137584	A1	*	5/2021	Urbanski	A61B 18/1477
2021/0228858	A1	*	7/2021	Arnett	A61M 25/0662

* cited by examiner

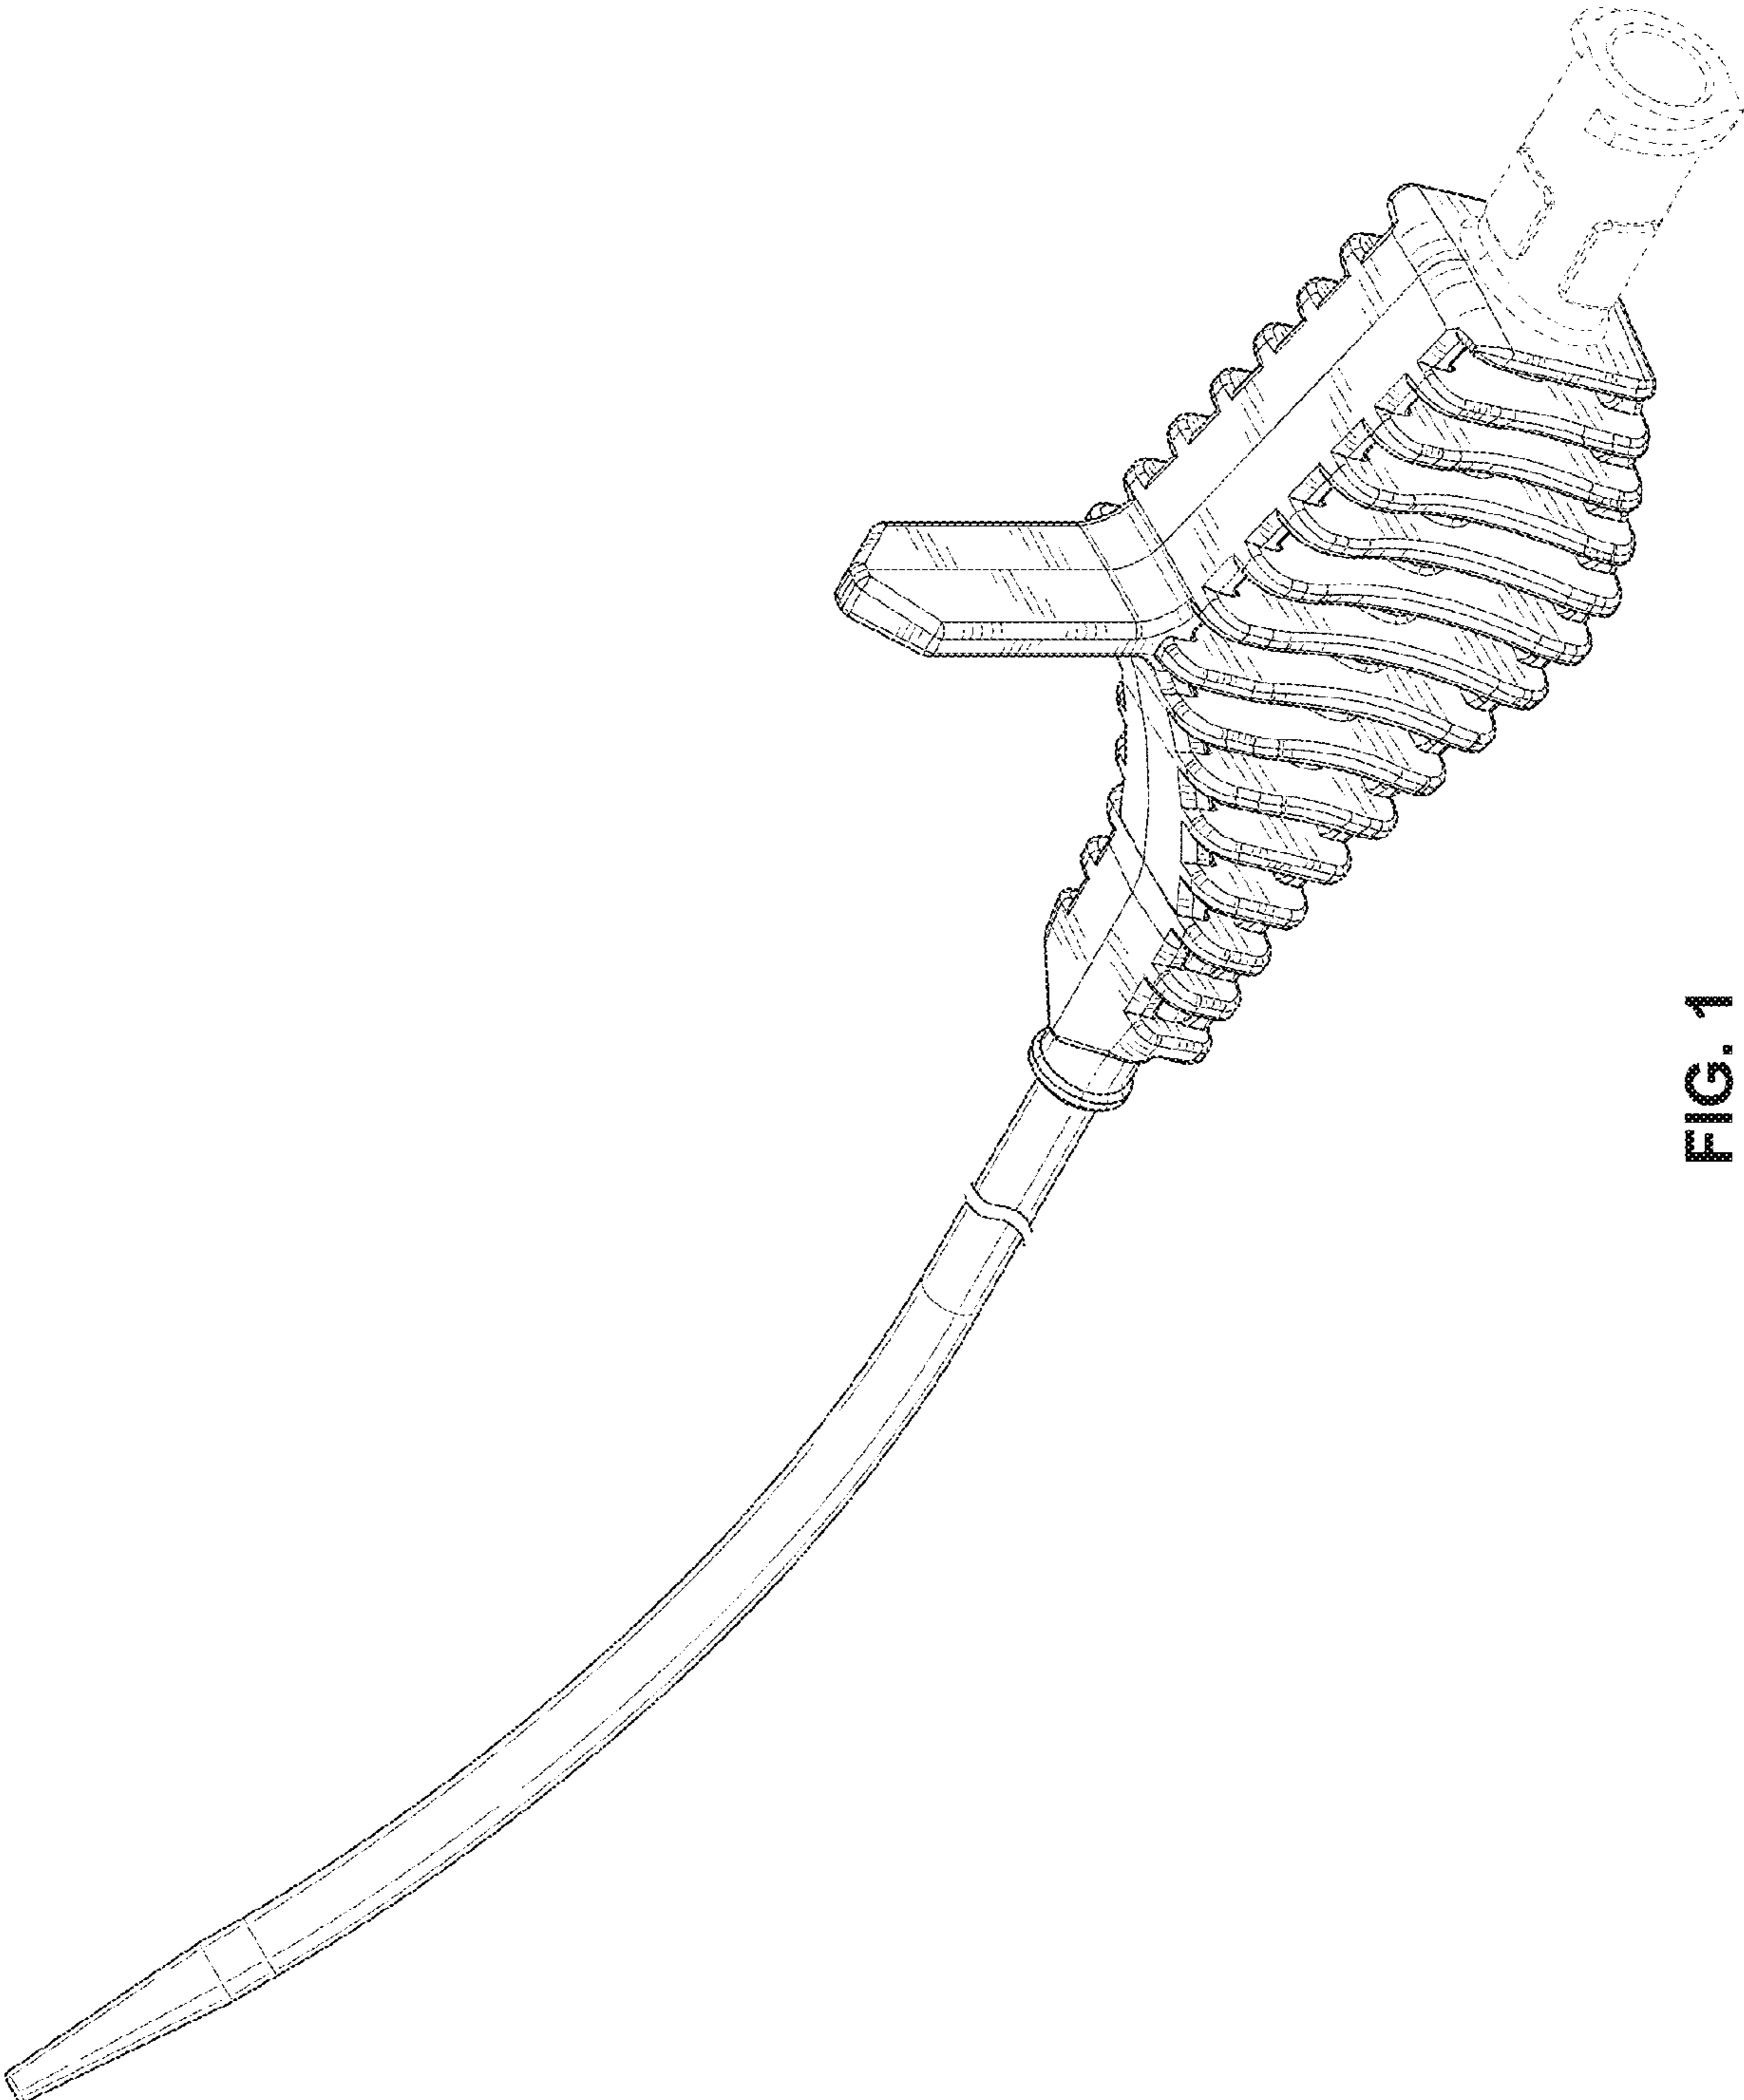


FIG. 1

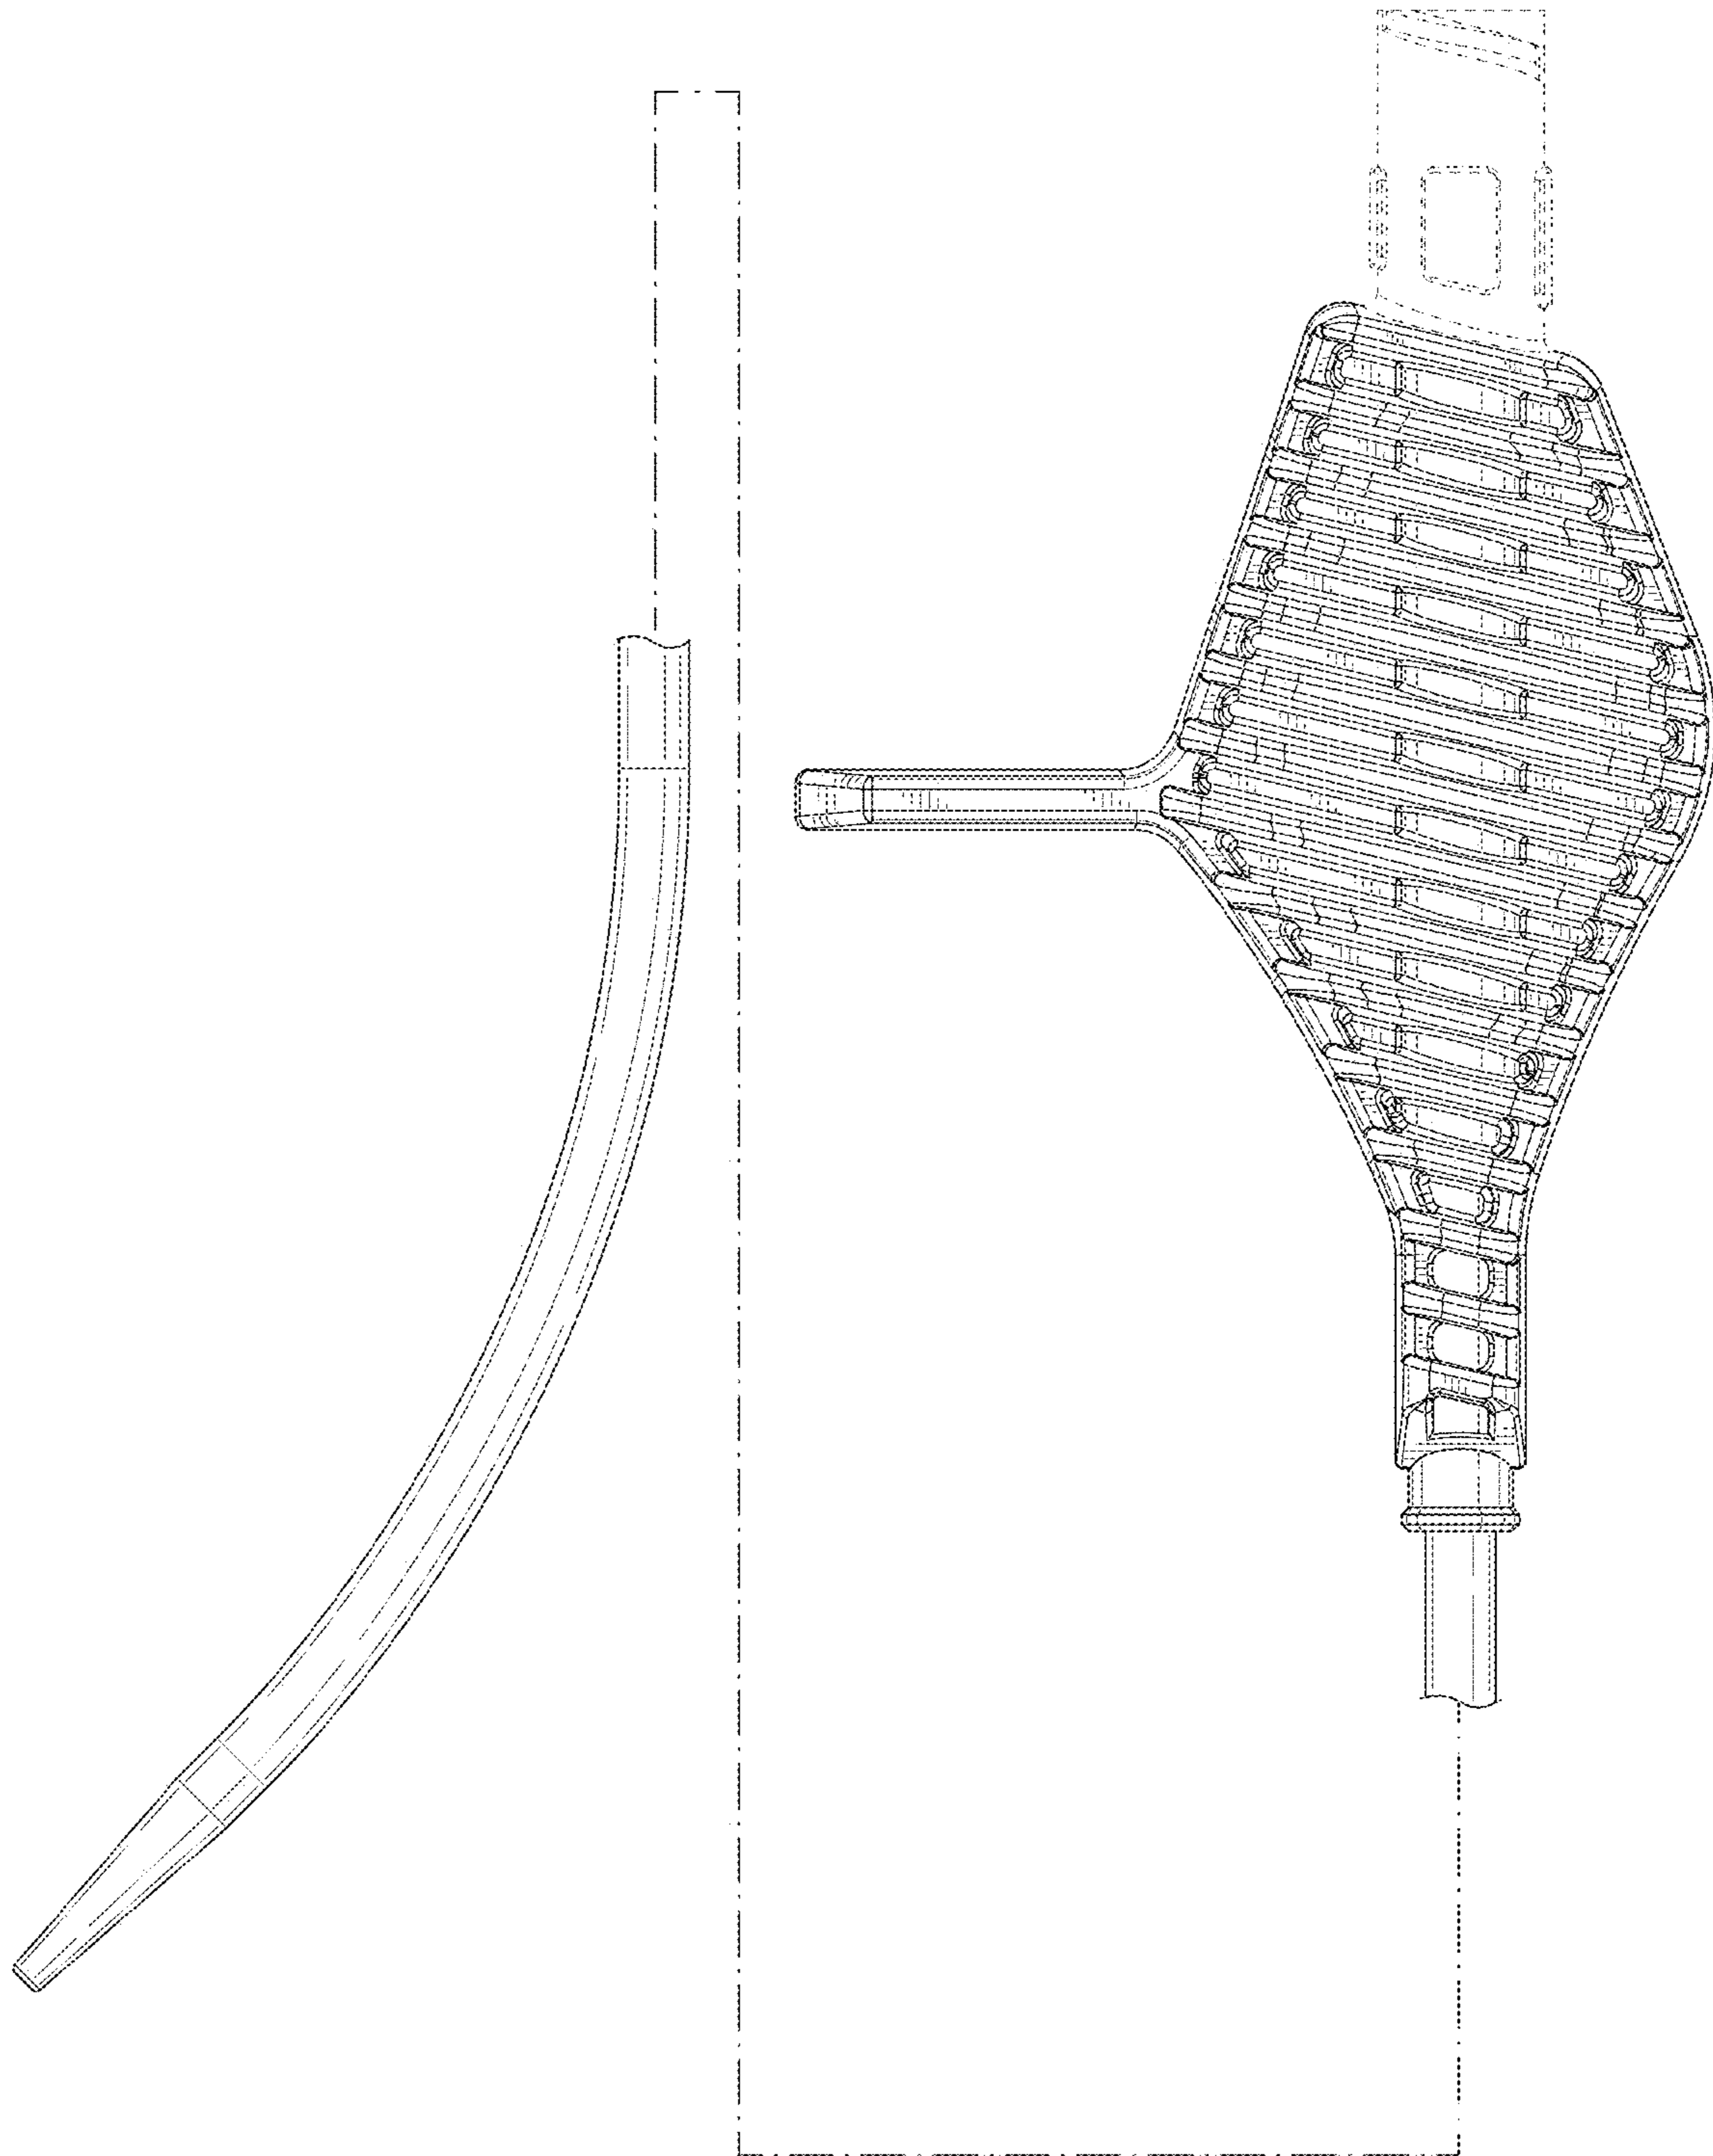


FIG. 2

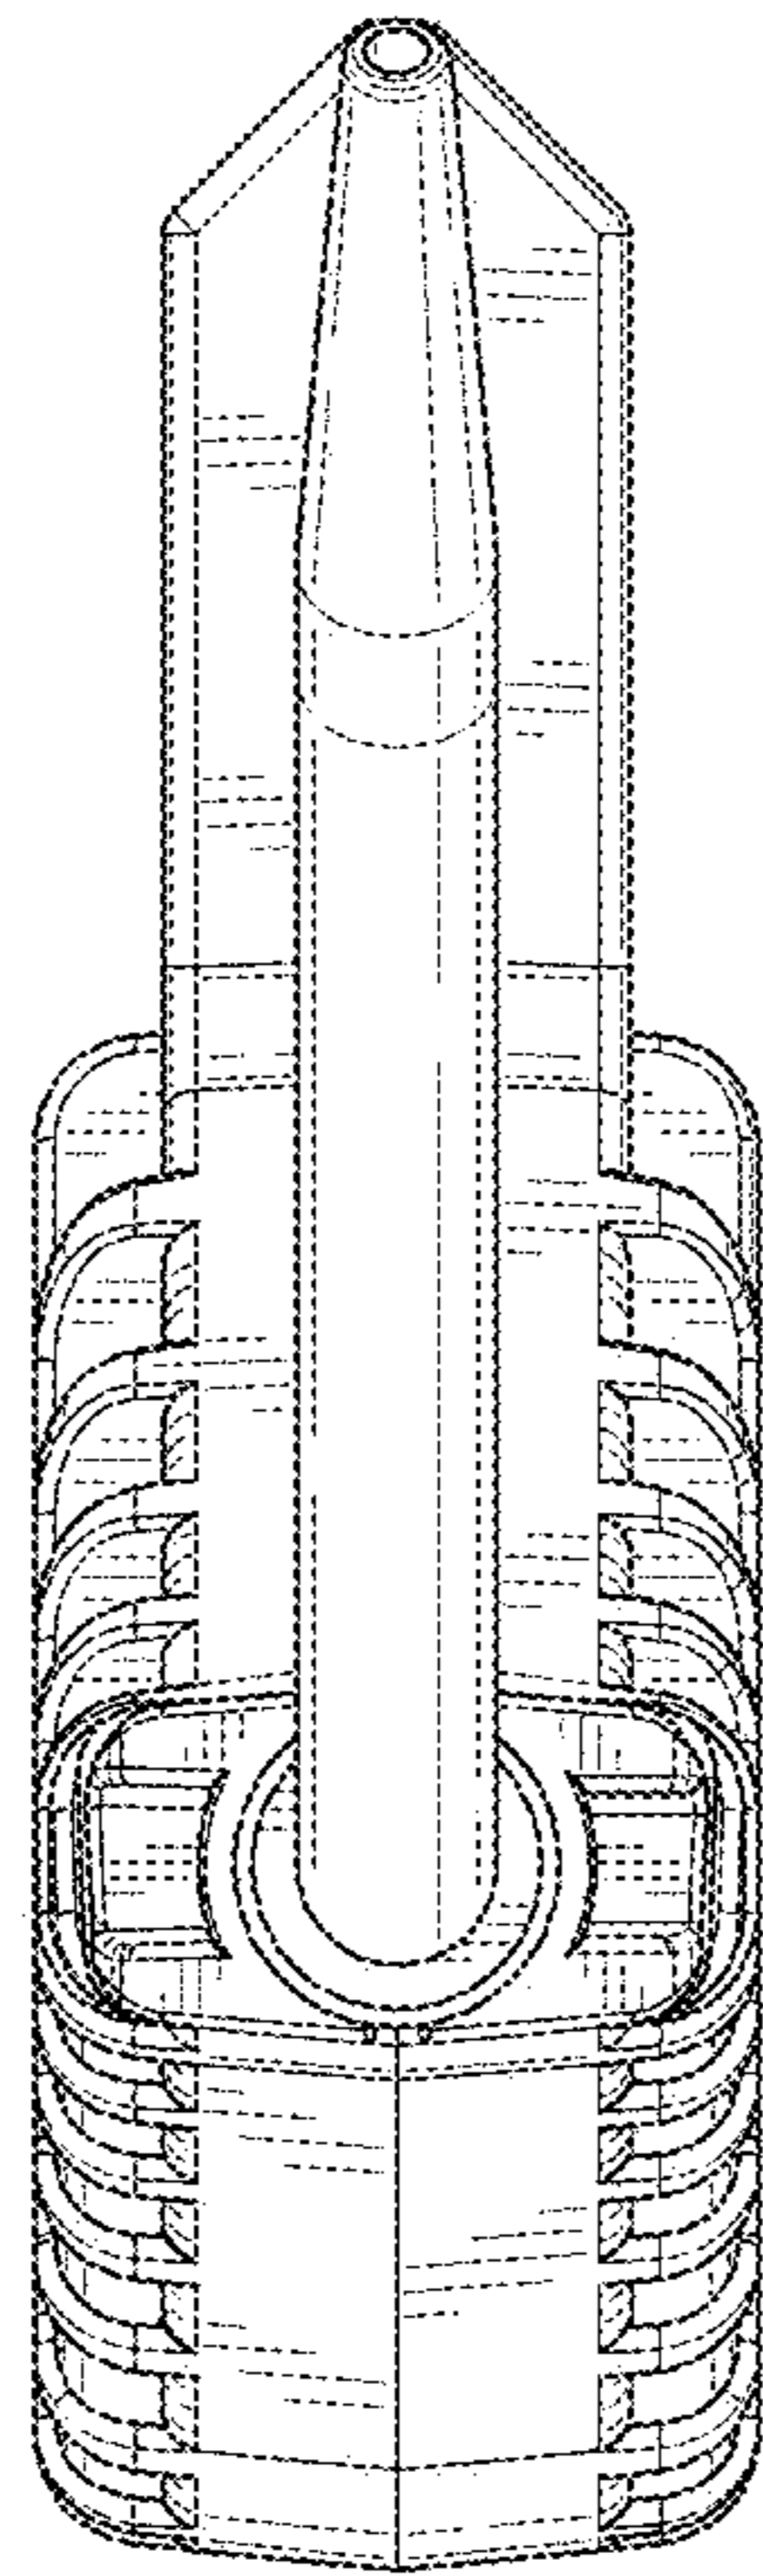


FIG. 3

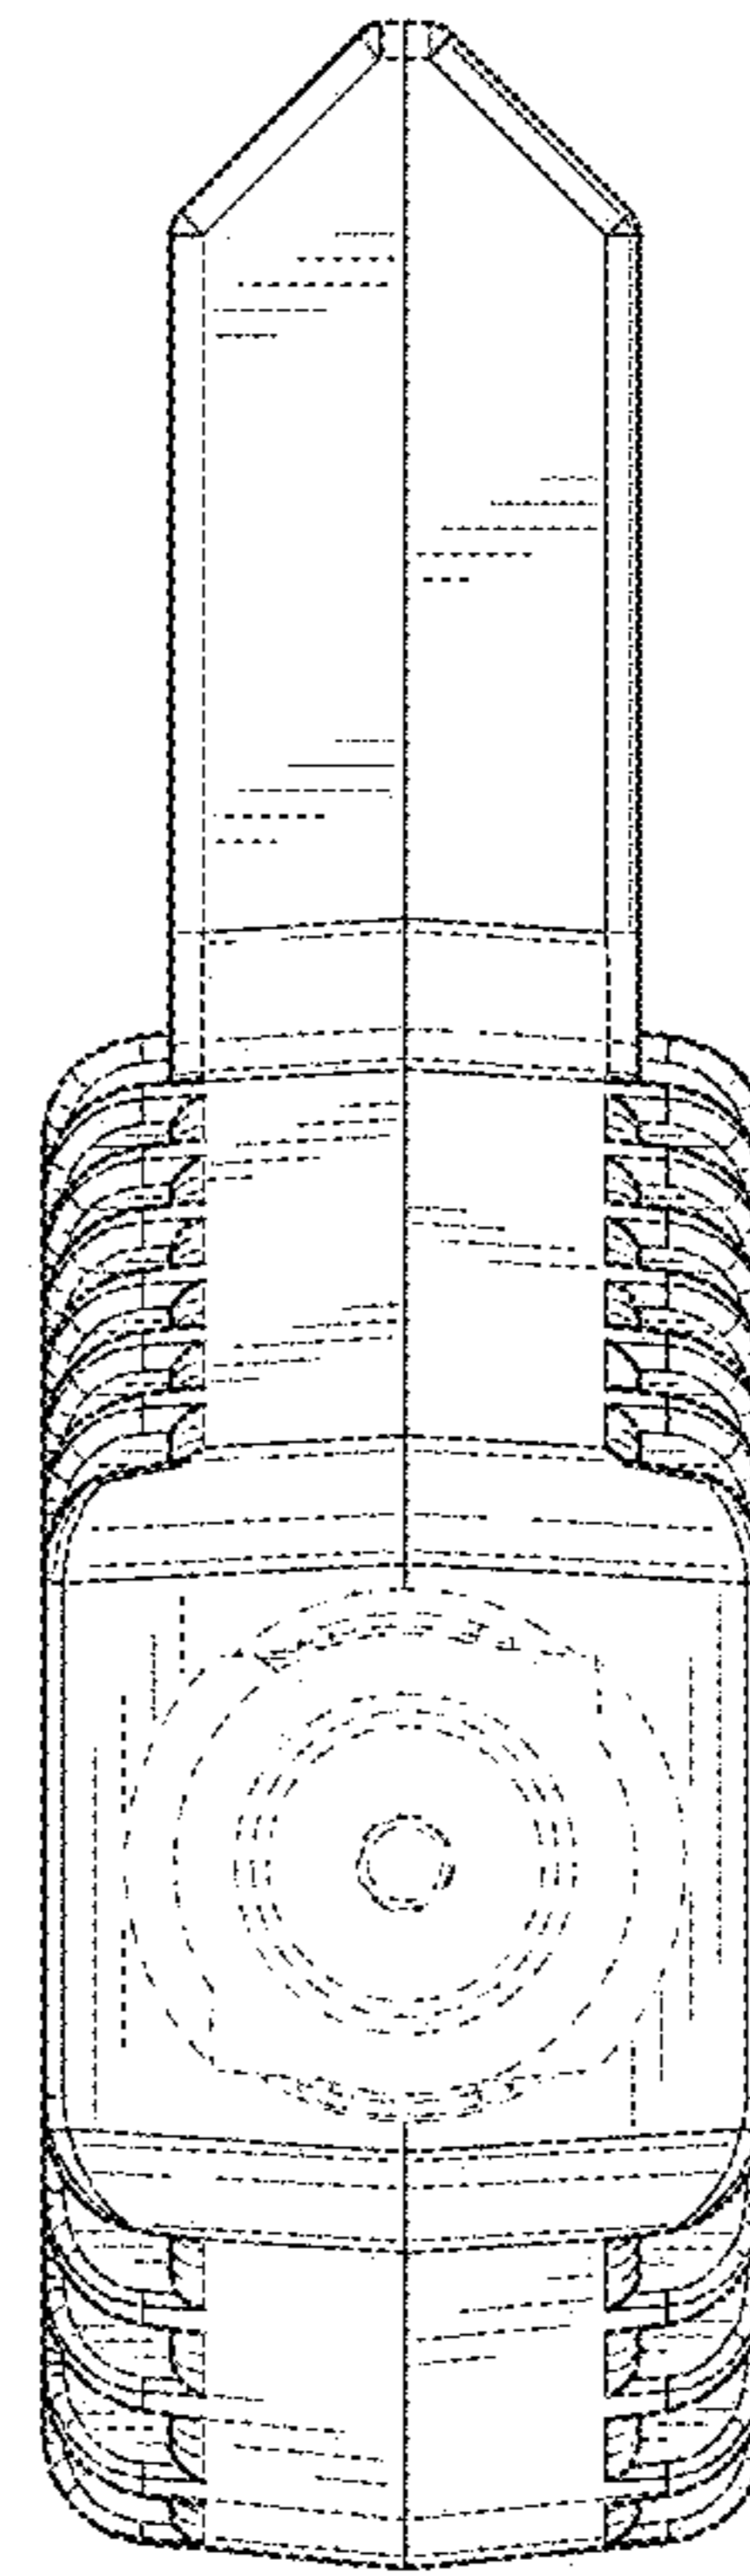


FIG. 4

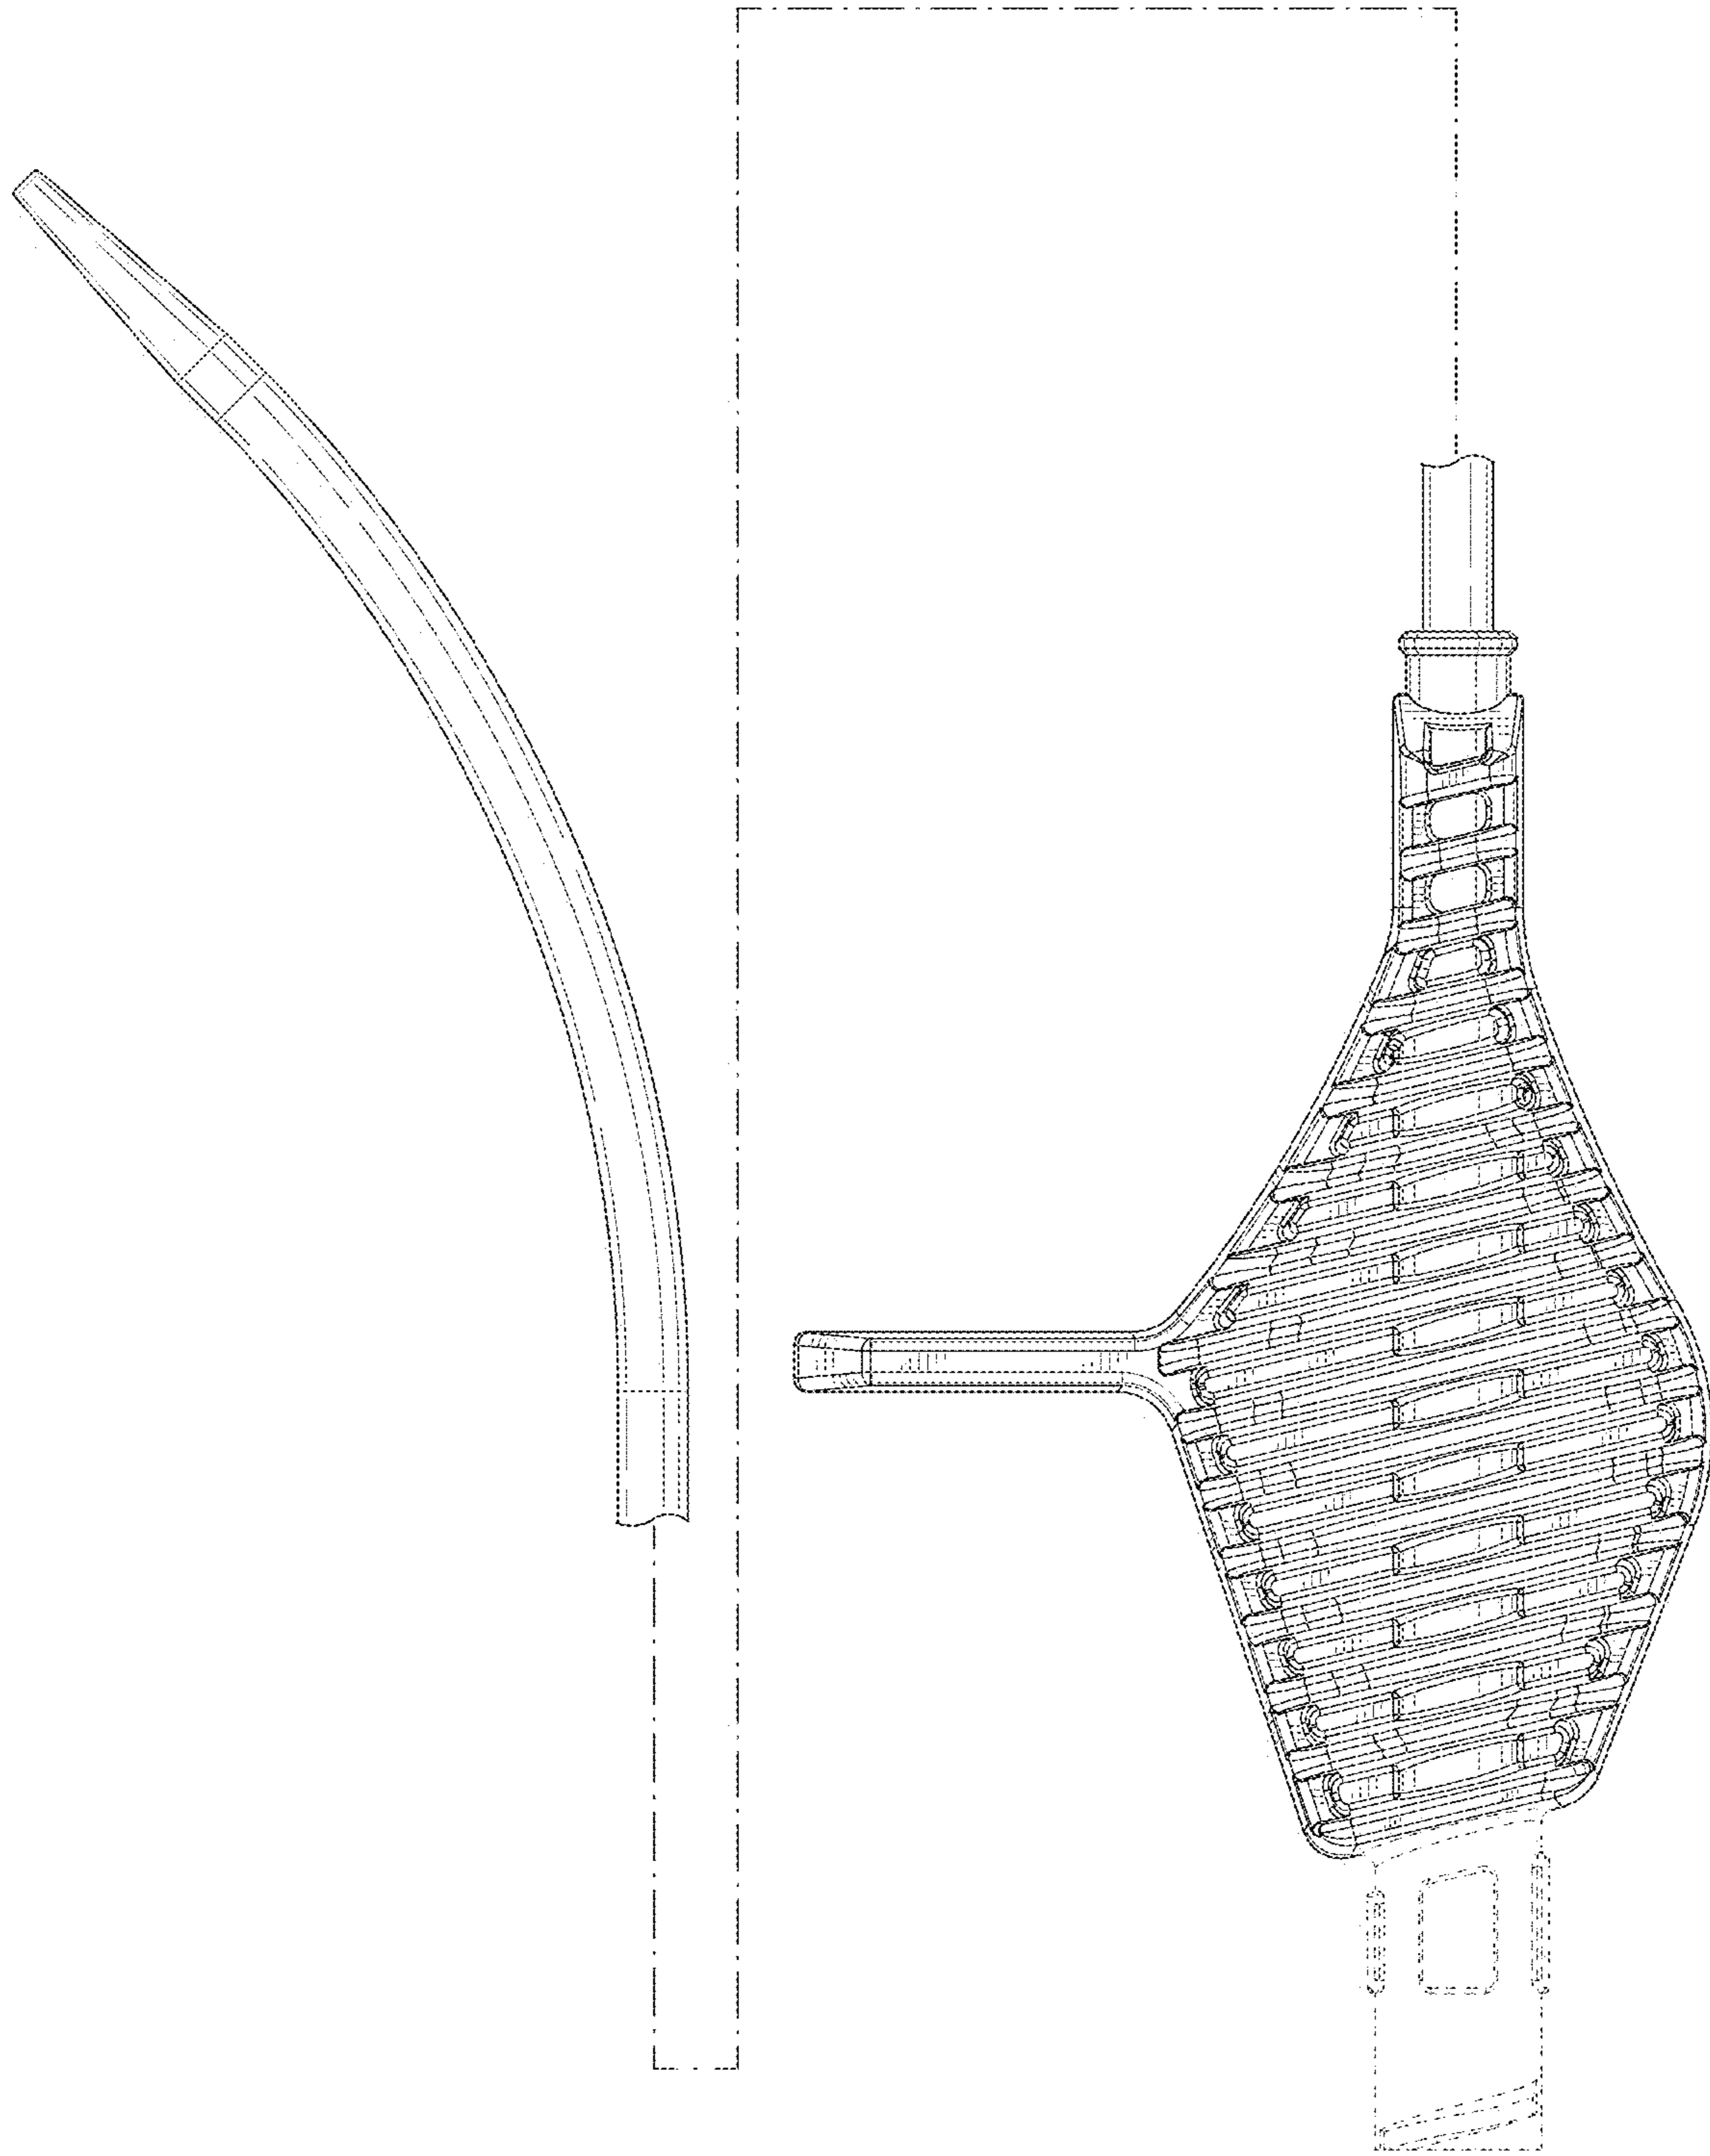


FIG. 5

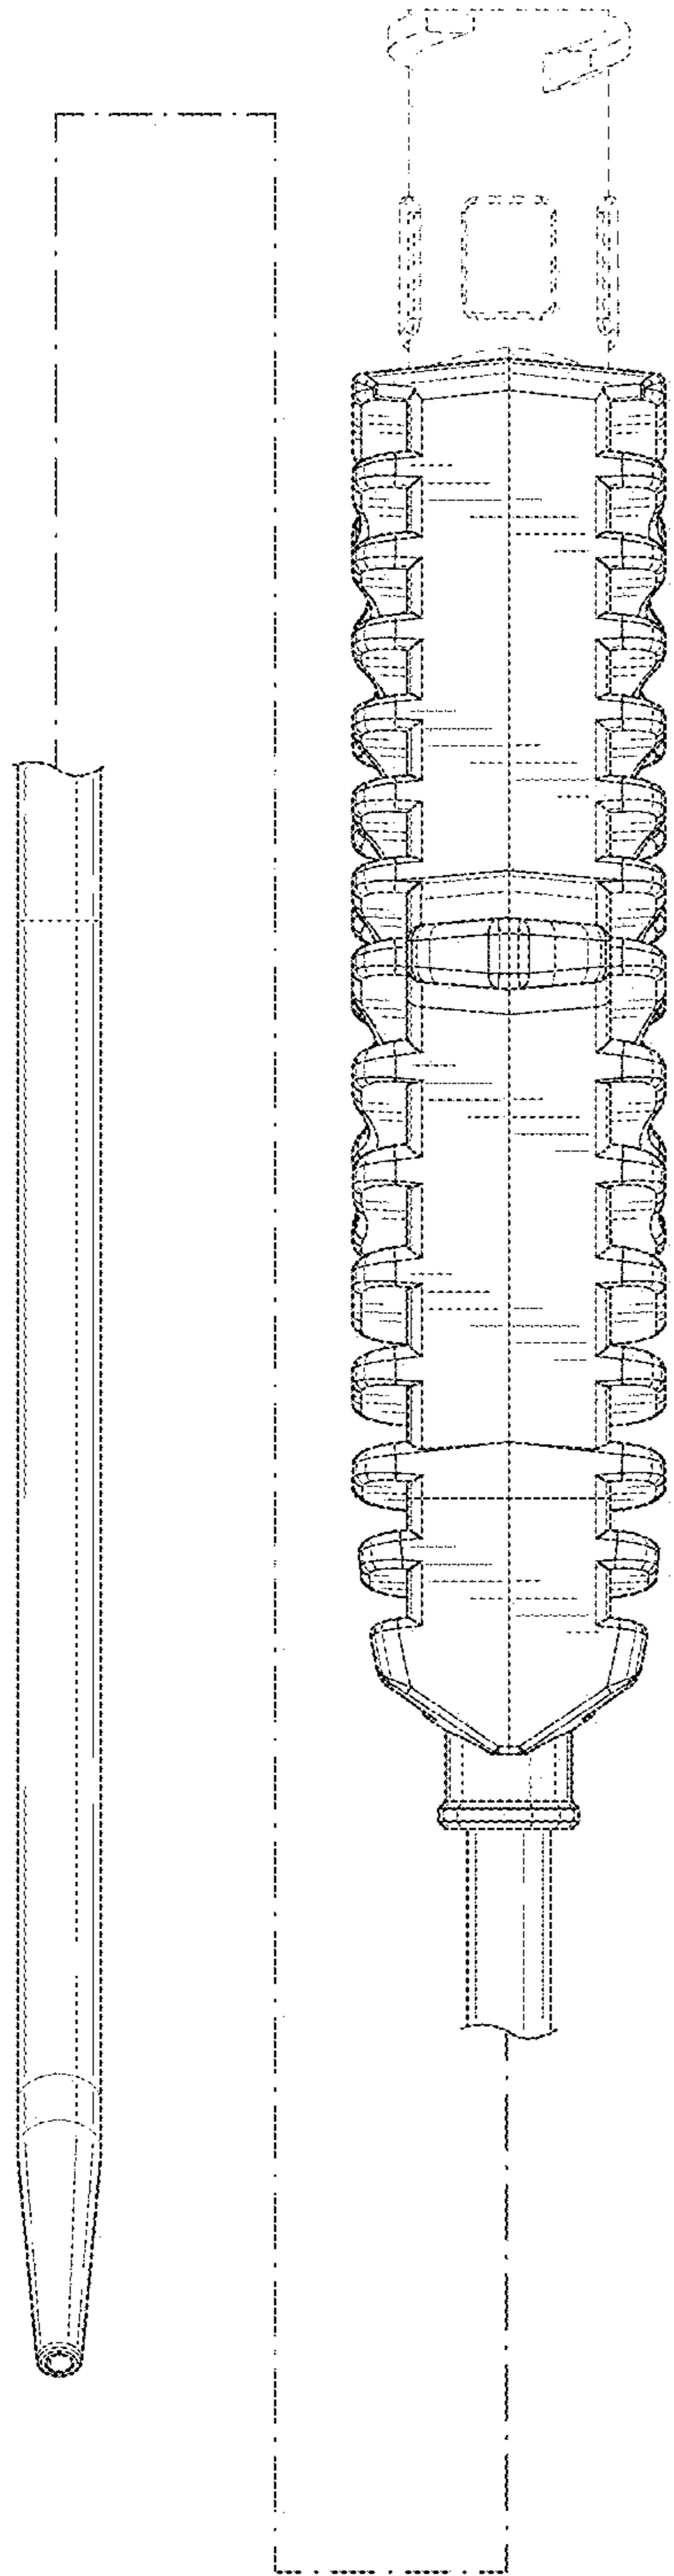


FIG. 6

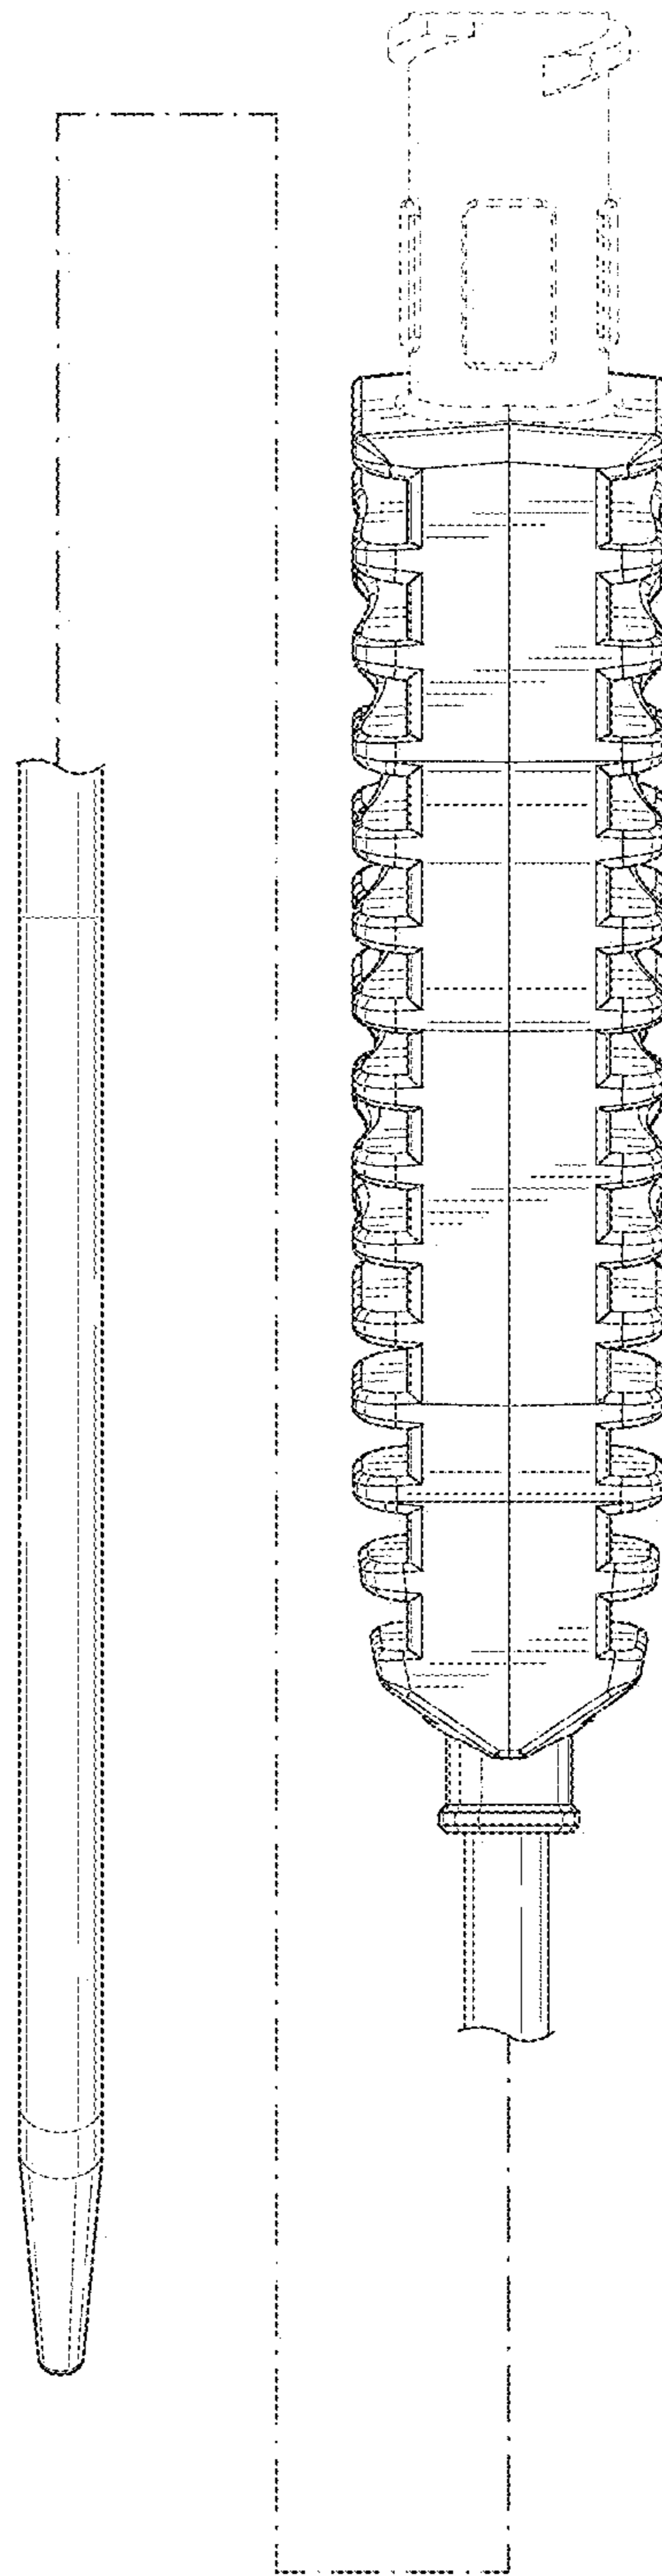


FIG. 7

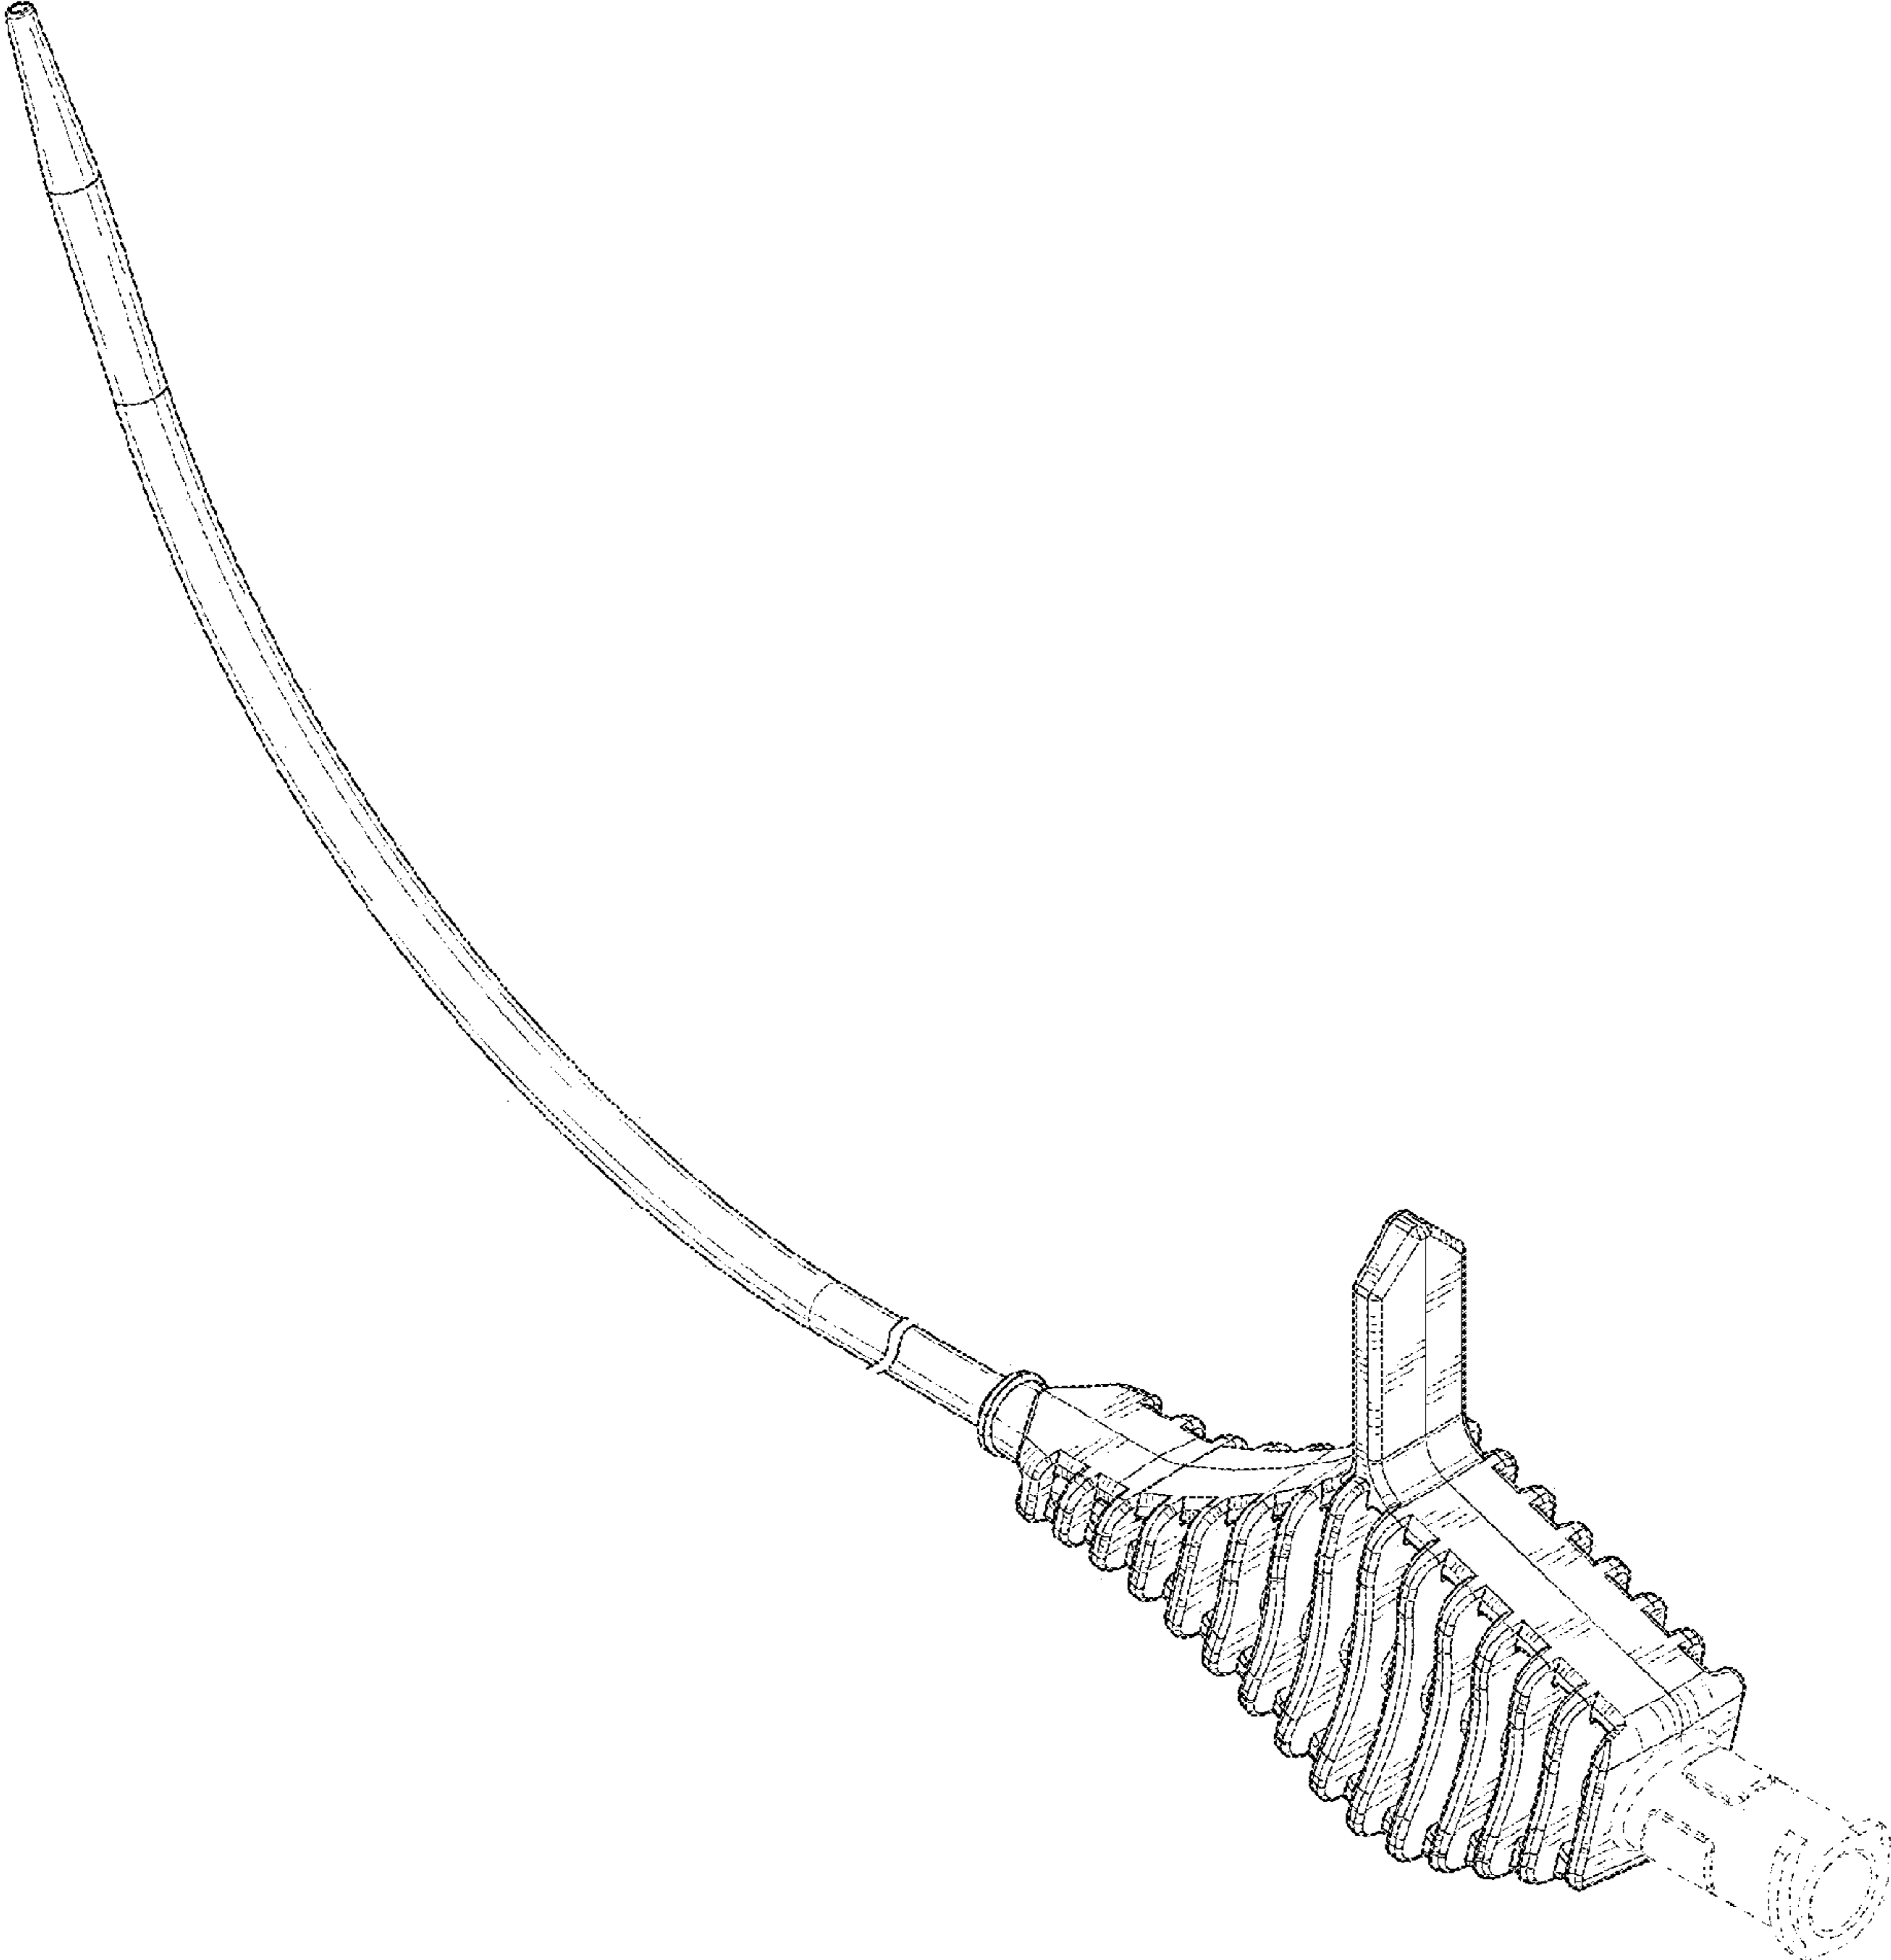


FIG. 8

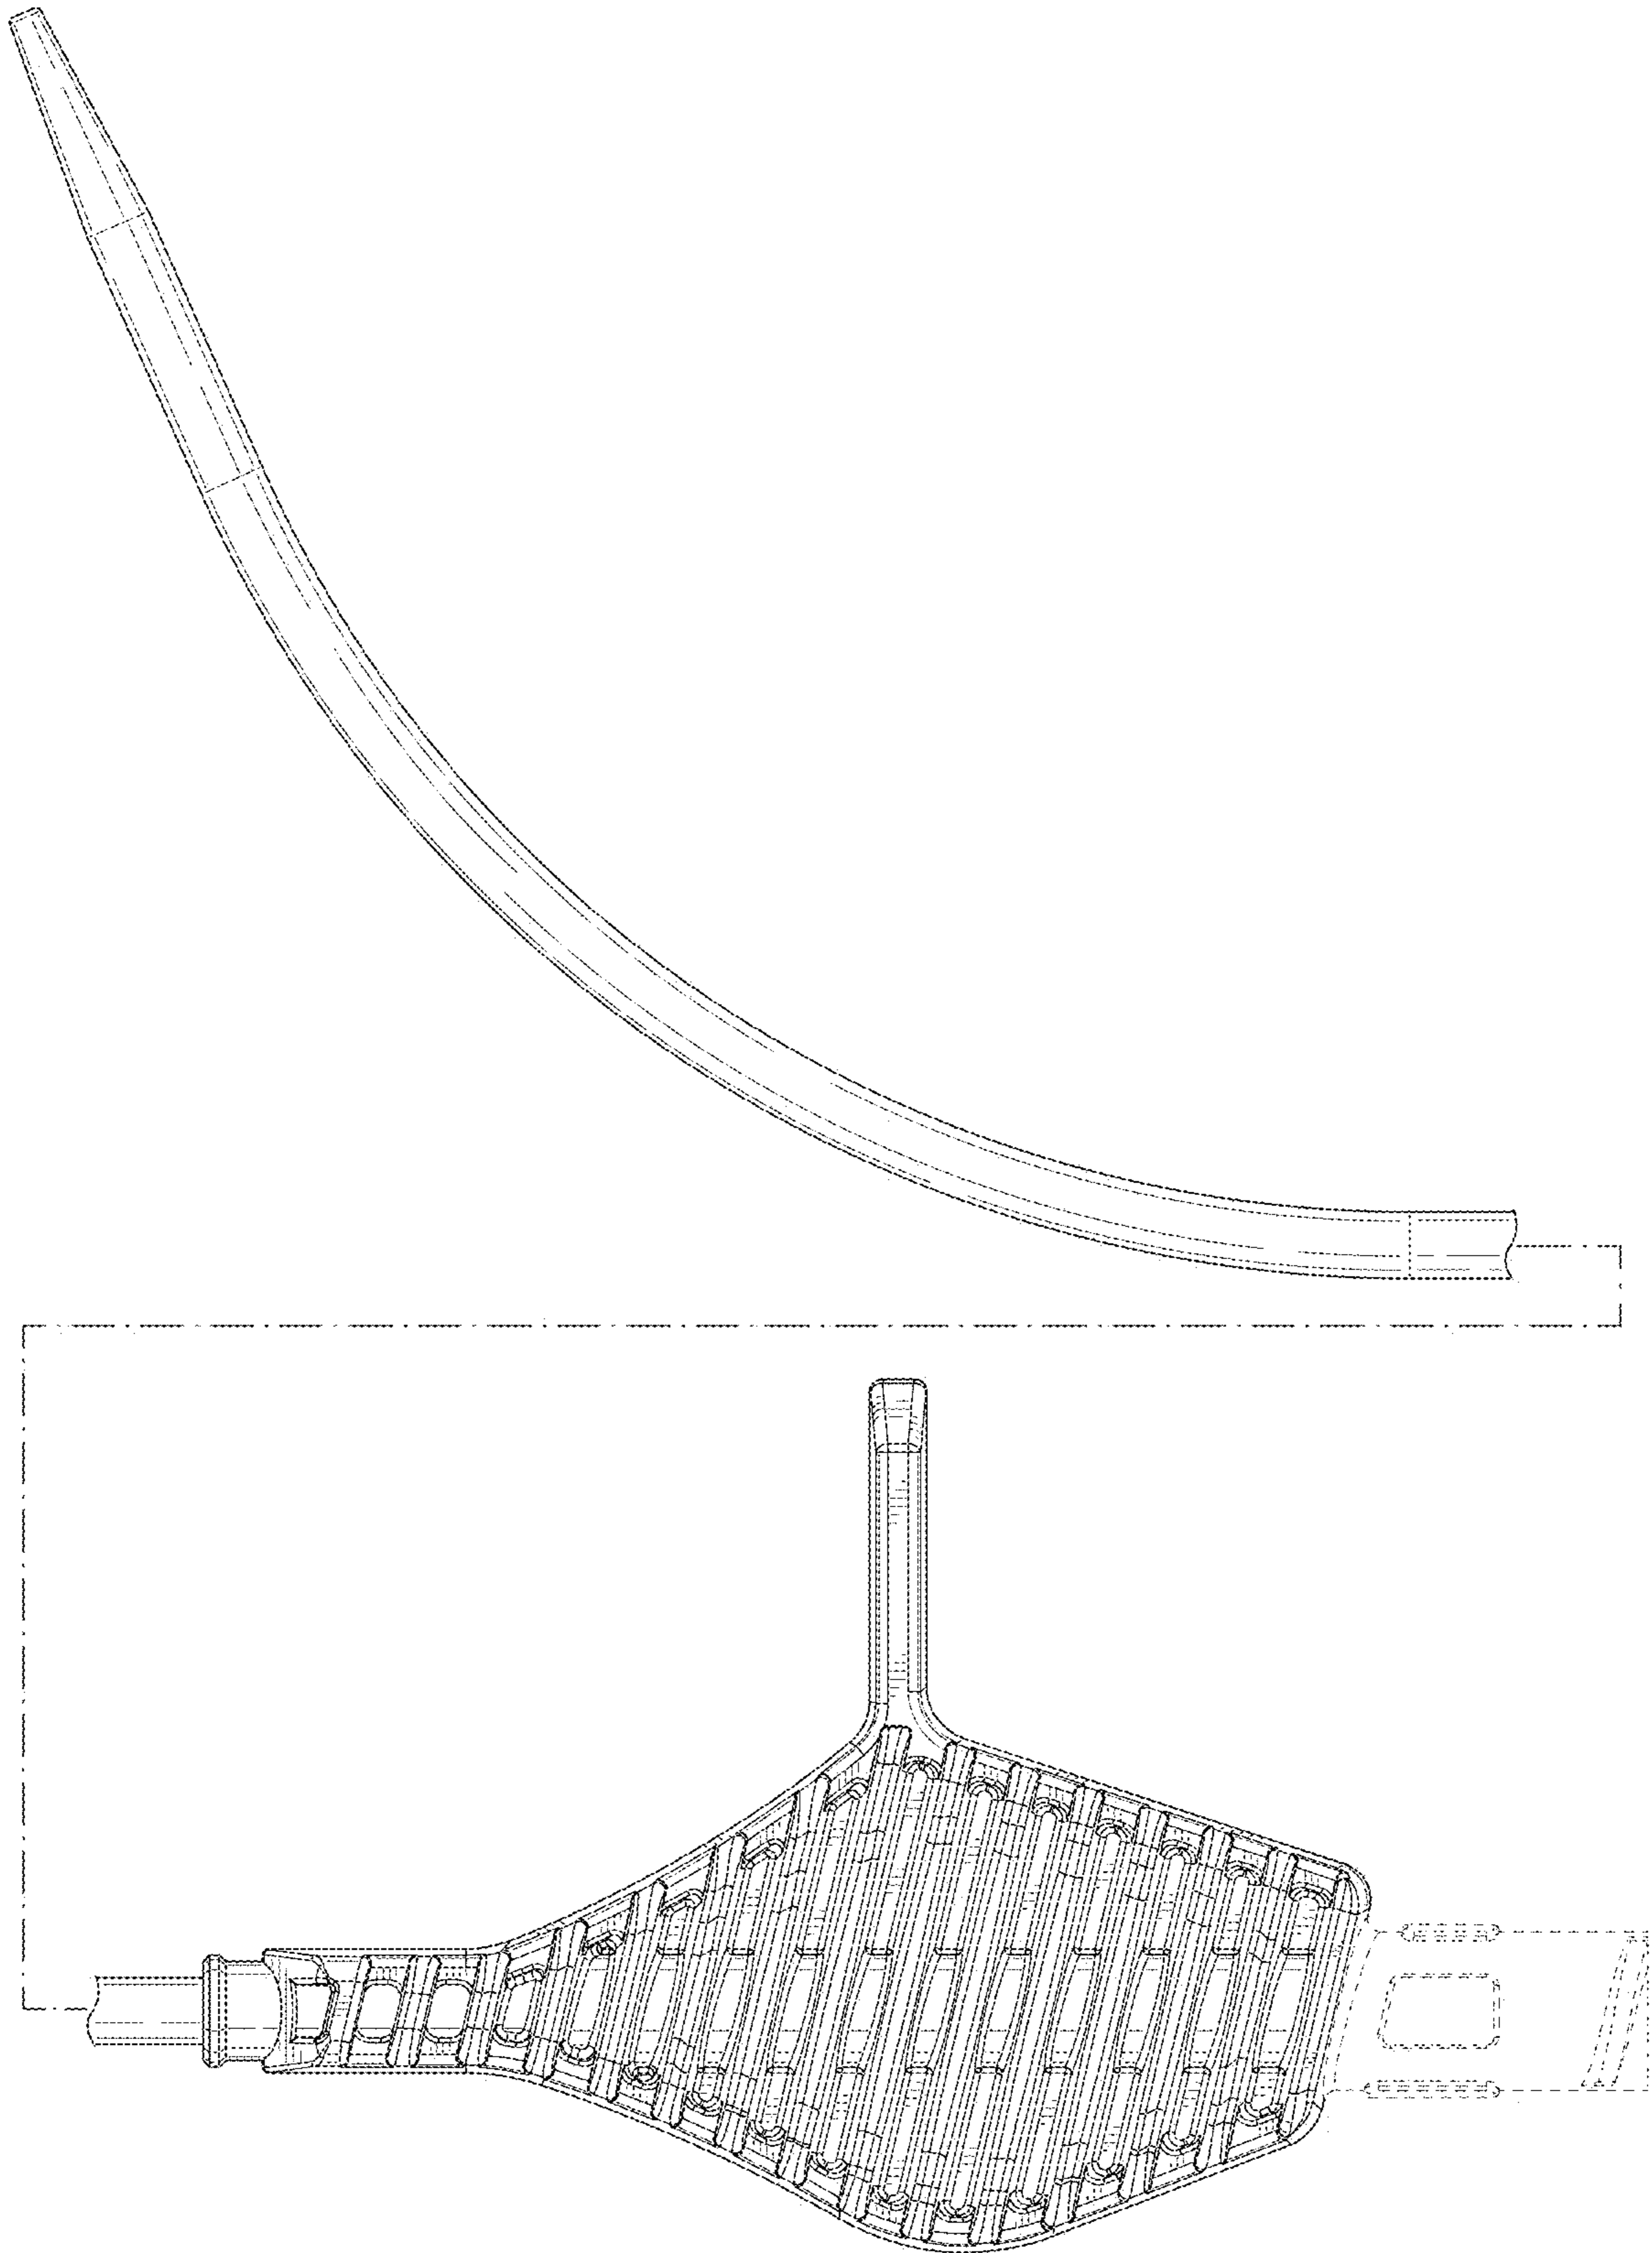


FIG. 9

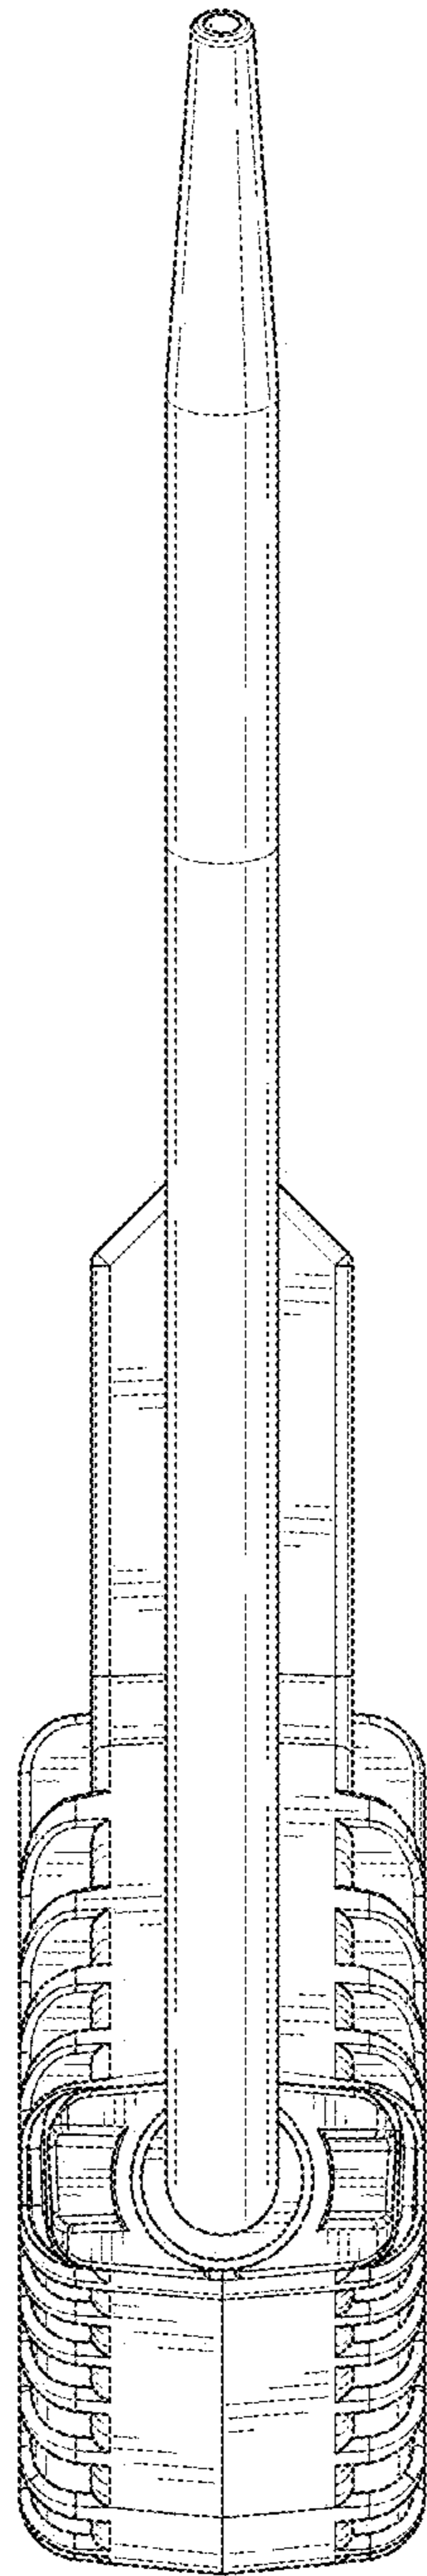


FIG. 10

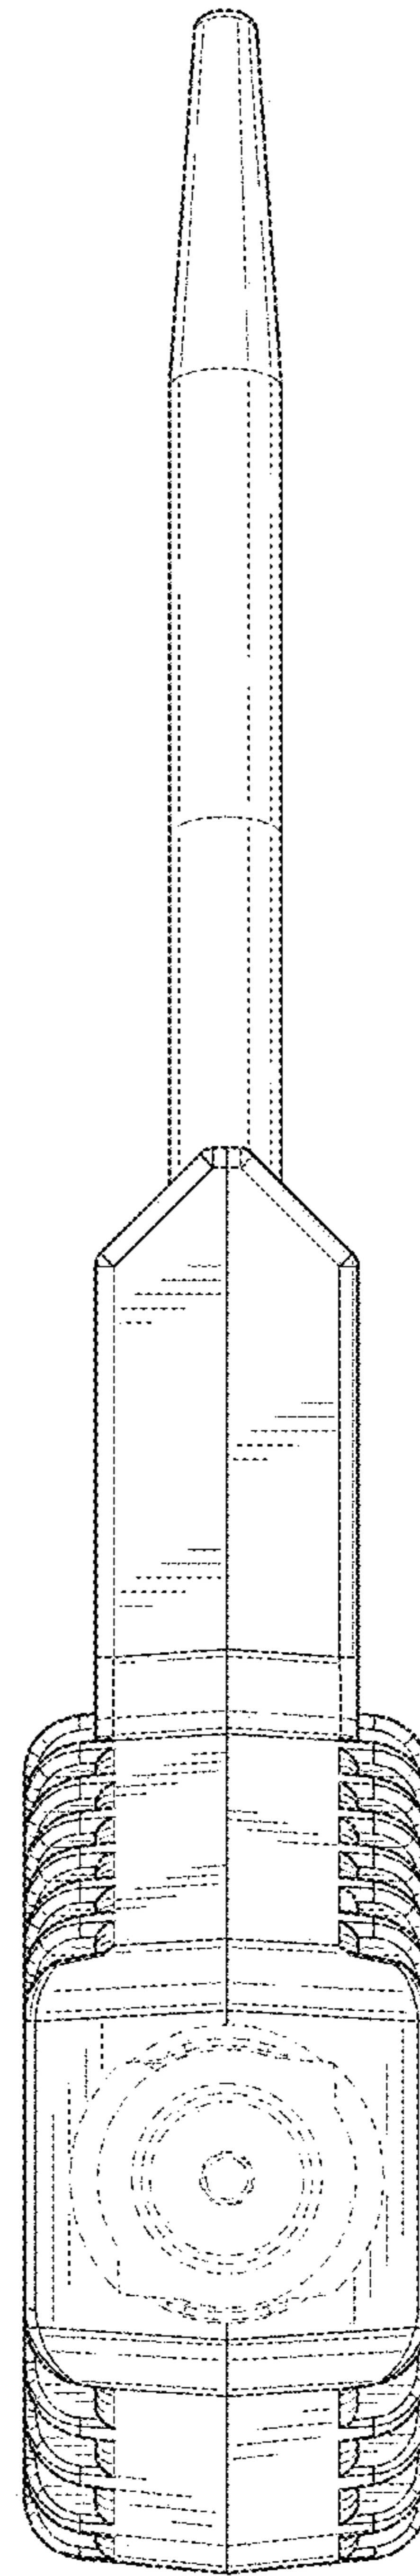


FIG. 11

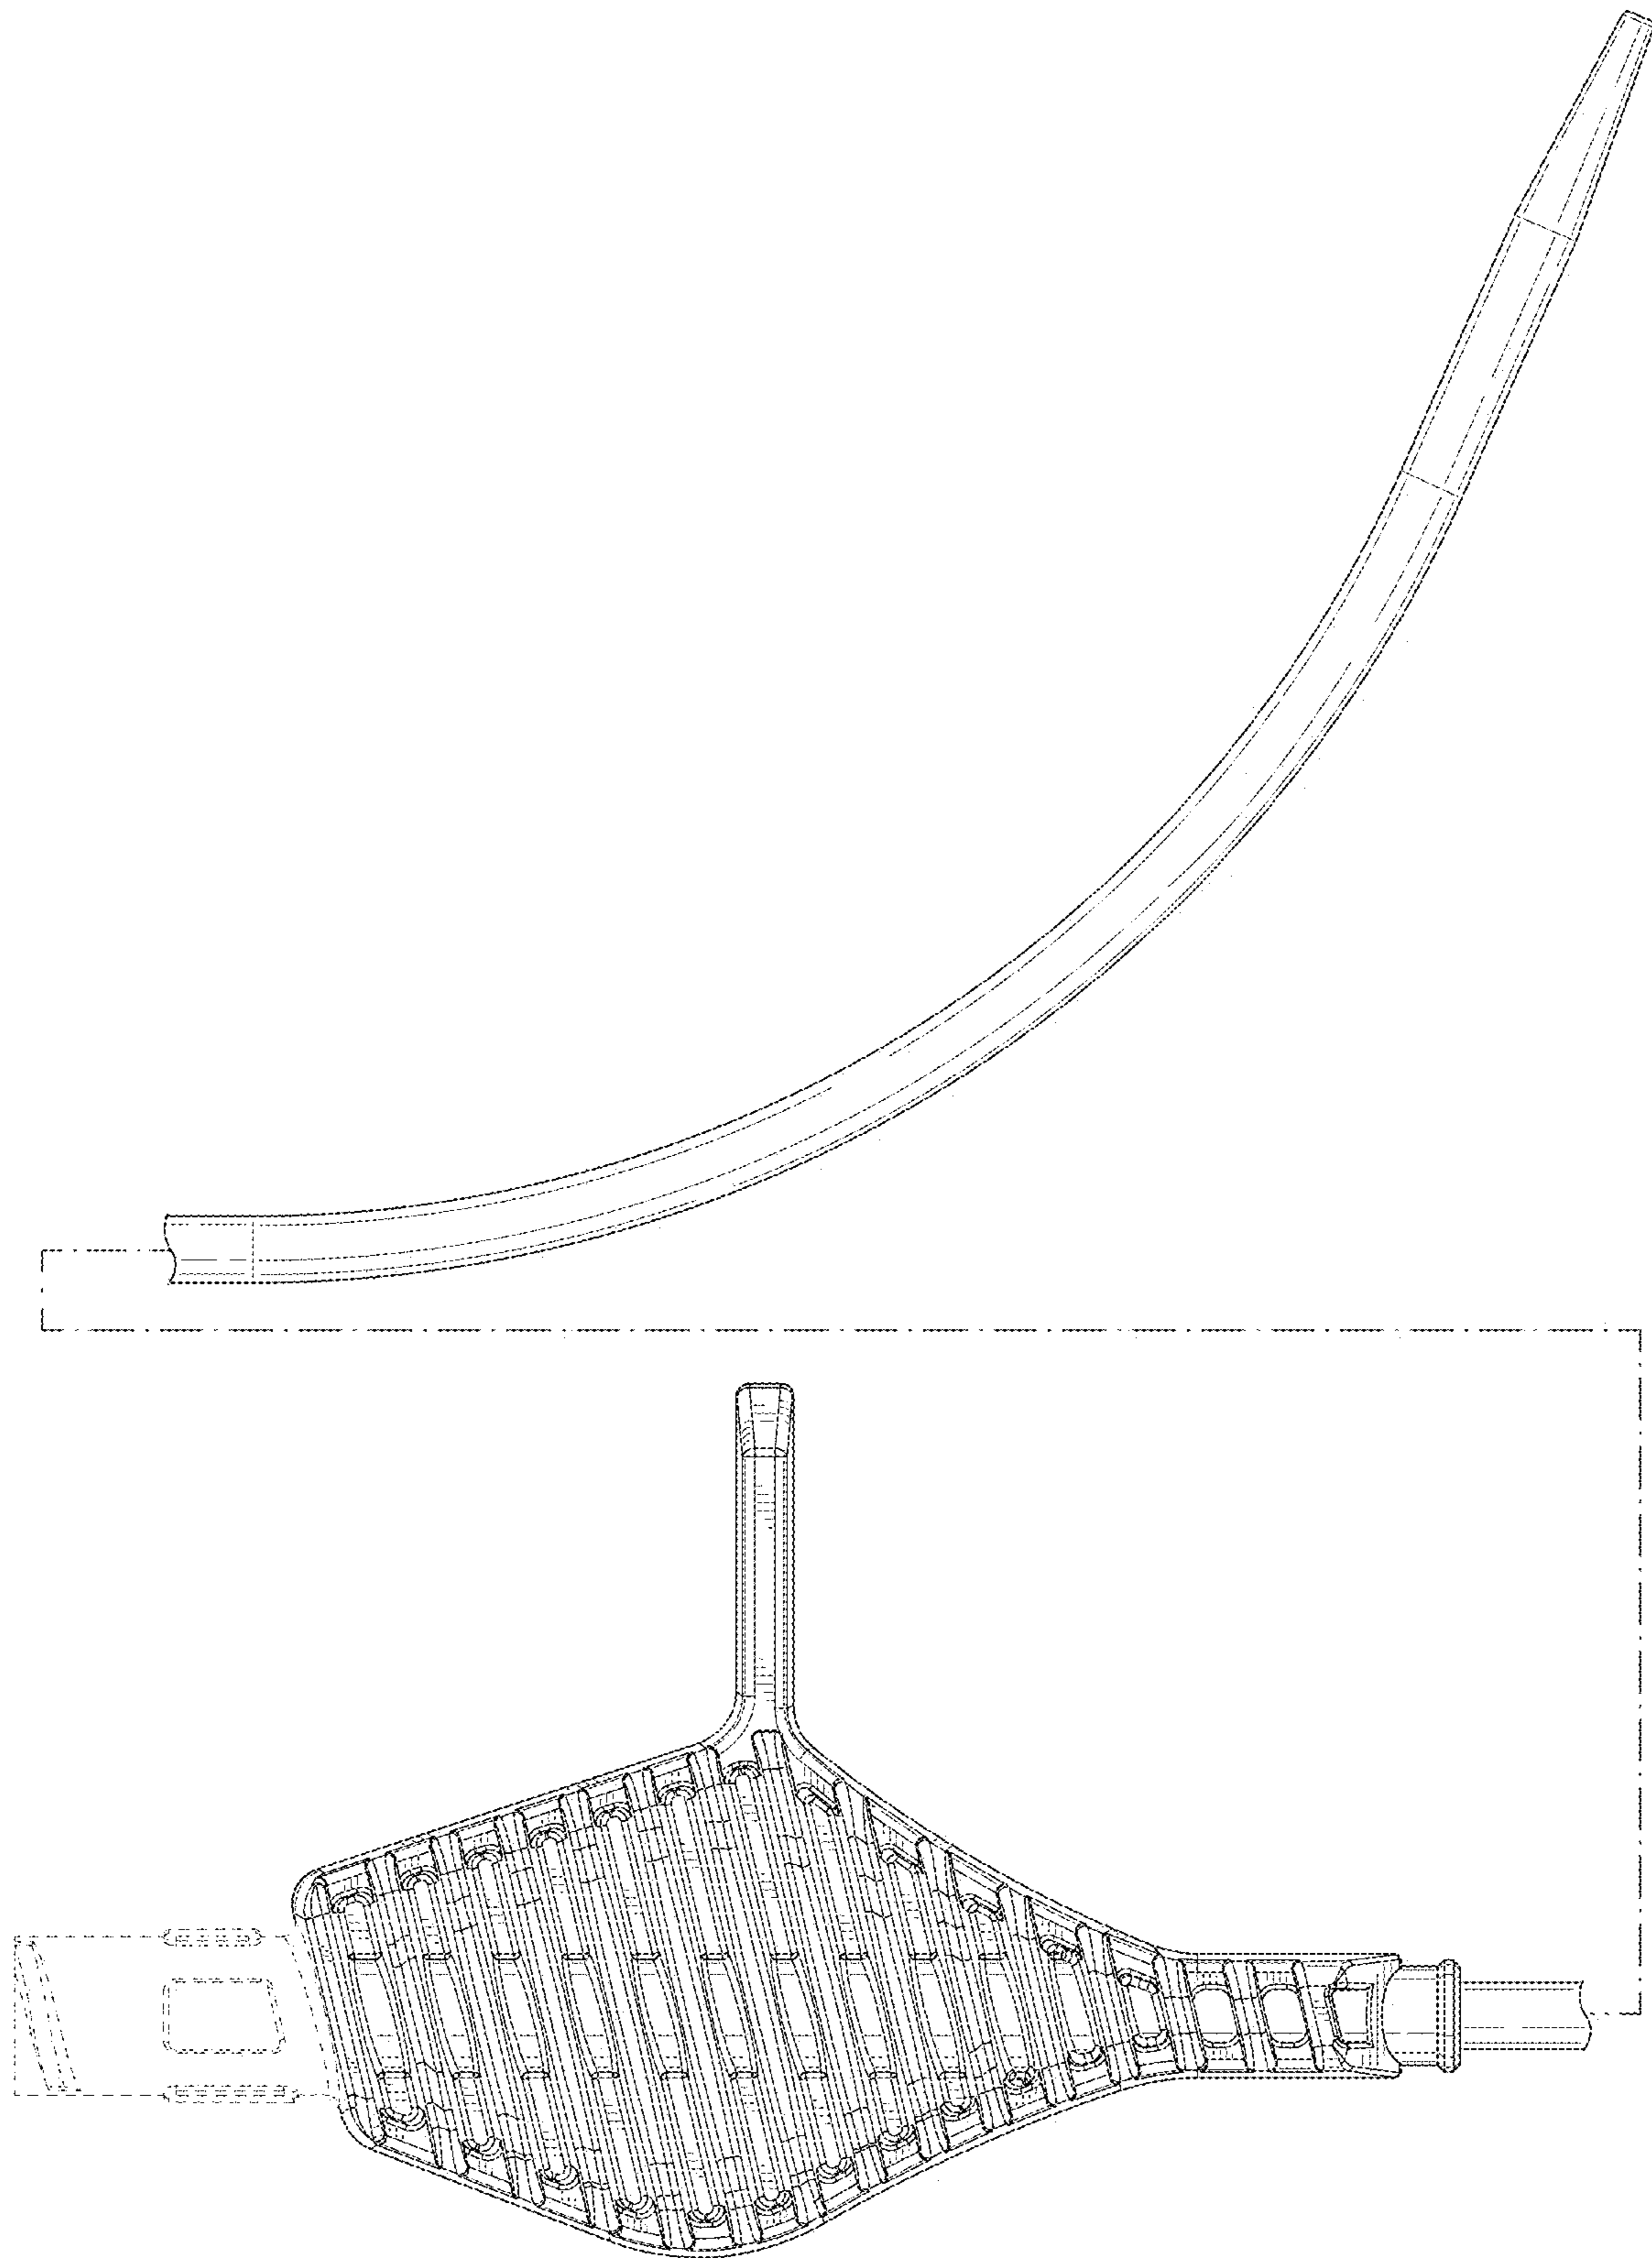


FIG. 12

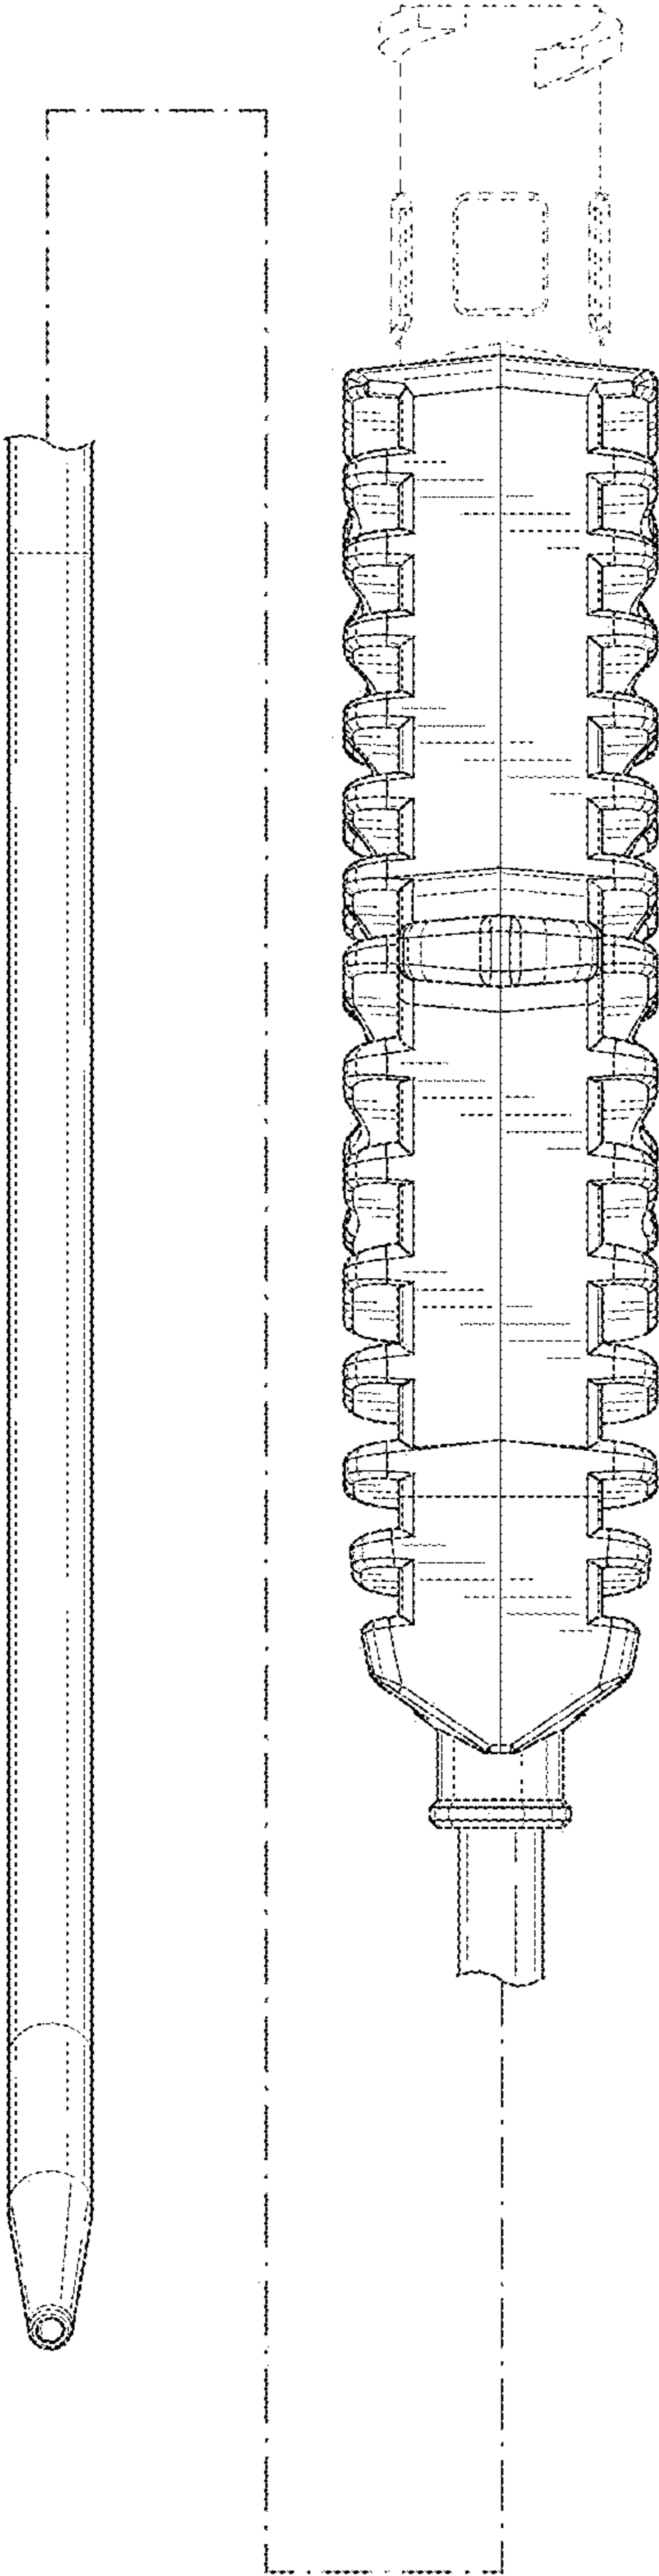


FIG. 13

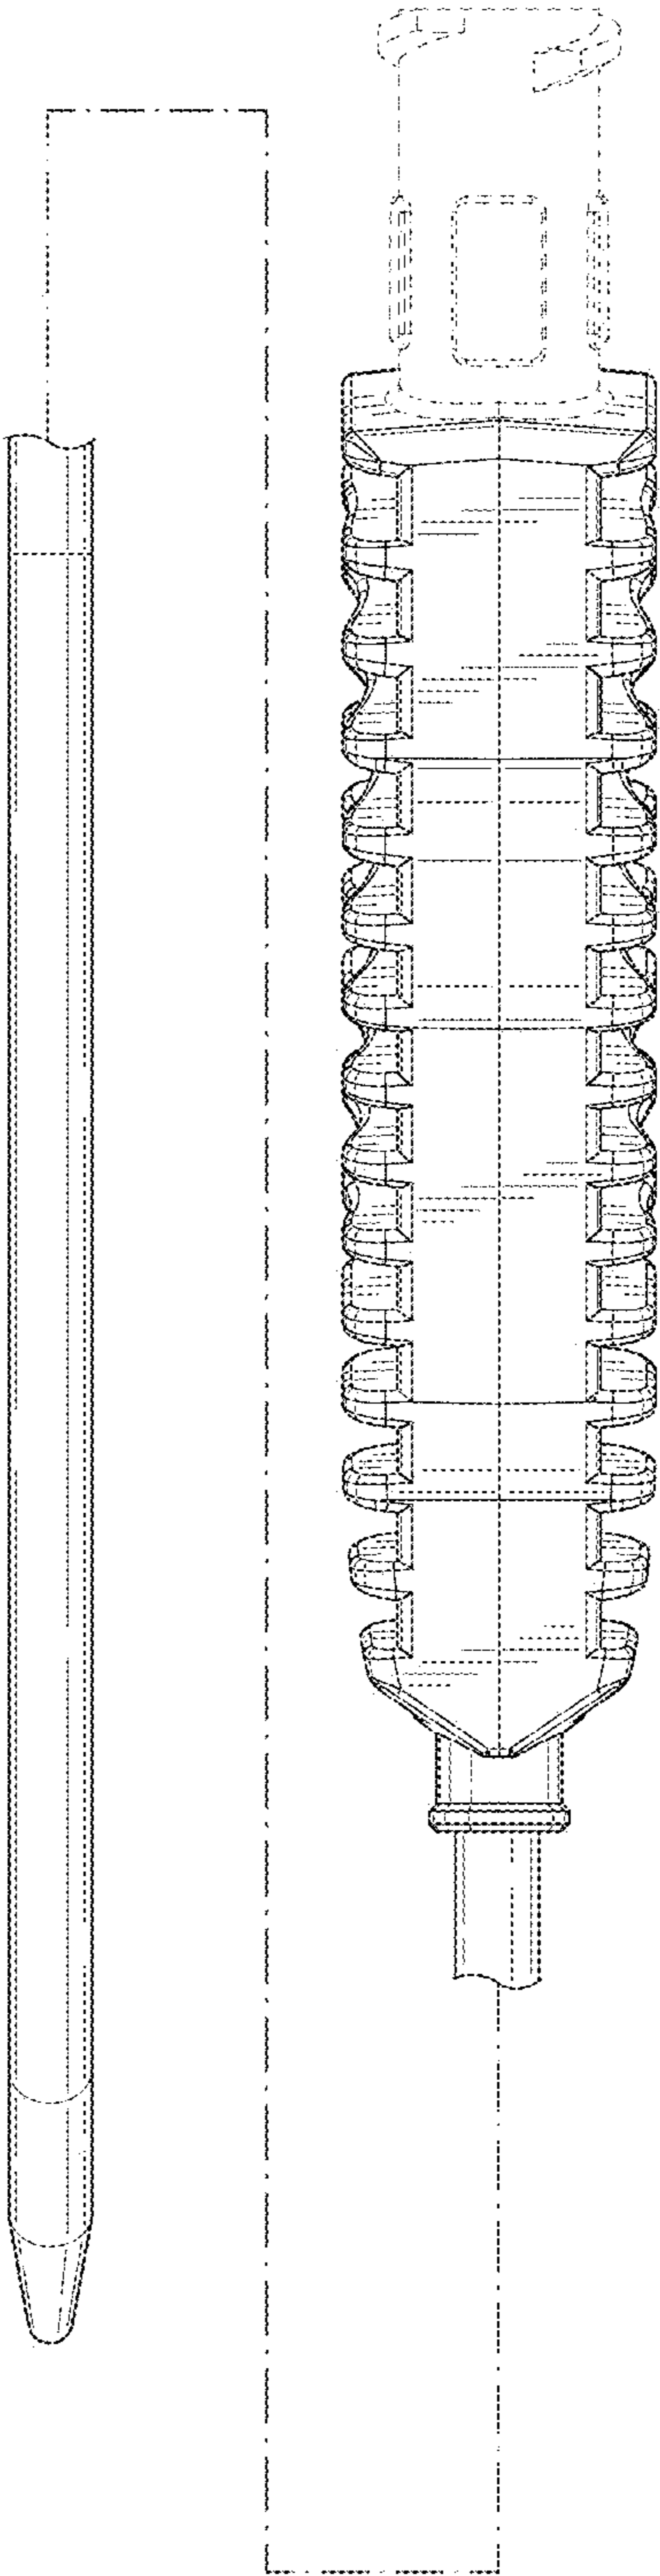


FIG. 14