



US00D952023S

(12) **United States Design Patent** (10) **Patent No.:** **US D952,023 S**  
**Dacosta et al.** (45) **Date of Patent:** **\*\* May 17, 2022**

(54) **HANDHELD IMAGING DEVICE**  
(71) Applicant: **MolecuLight Inc.**, Toronto (CA)  
(72) Inventors: **Ralph S. Dacosta**, Etobicoke (CA); **Simon Treadwell**, Toronto (CA); **Todd Daynes**, Aurora (CA); **Todd Meaney**, Thornhill (CA); **Danielle Dunham**, Toronto (CA); **Carl Annis**, Oakville (CA); **Connor Wright**, Toronto (CA); **Kimberlyn Dampitan**, Mississauga (CA); **Nitesh Mistry**, Toronto (CA)

D515,214 S 2/2006 Jackson, III et al.  
D569,378 S 5/2008 Wanamaker  
D585,554 S 1/2009 Suzuki  
D610,178 S 2/2010 Adolfsson et al.  
7,846,091 B2 12/2010 Fulghum  
(Continued)

**FOREIGN PATENT DOCUMENTS**

EP 2502551 9/2012  
EP 3372143 9/2018  
(Continued)

**OTHER PUBLICATIONS**

Notice of Allowance in Design U.S. Appl. No. 29/677,152, dated Apr. 1, 2020.

(Continued)

*Primary Examiner* — Ramzi Almatrahi  
(74) *Attorney, Agent, or Firm* — Jones Robb, PLLC

(73) Assignee: **MOLECULIGHT, LTD.**, Toronto (CA)  
(\*\*) Term: **15 Years**

(21) Appl. No.: **29/762,417**

(22) Filed: **Dec. 16, 2020**

**Related U.S. Application Data**

(62) Division of application No. 29/676,901, filed on Jan. 15, 2019, now Pat. No. Des. 908,161.

(51) **LOC (13) Cl.** ..... **16-05**

(52) **U.S. Cl.**  
USPC ..... **D16/219**

(58) **Field of Classification Search**

USPC ..... D16/200, 202–204, 208, 218, 219;  
348/143, 148, 164, 151, 347, 360,  
348/373–376; 396/419, 427–428, 535,  
396/539–541

CPC ..... G03B 15/03; G03B 17/02; G03B 17/04;  
G03B 17/48; G03B 17/56; G03B 19/04;  
G08G 1/0175; H04N 5/2251; H04N  
5/2252; H04N 5/2253; H04N 5/2254

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

6,601,997 B2 8/2003 Ngo  
D480,478 S 10/2003 Leonard et al.


(57) **CLAIM**

The ornamental design for a handheld imaging device, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, front and right side perspective view of a handheld imaging device showing our new design.  
FIG. 2 is a front elevation view thereof.  
FIG. 3 is a back elevation view thereof.  
FIG. 4 is a left side elevation view thereof.  
FIG. 5 is a right side elevation view thereof.  
FIG. 6 is a top plan view thereof; and,  
FIG. 7 is a bottom plan view thereof.  
The broken lines depict portions of the handheld imaging device in which the design is embodied that form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

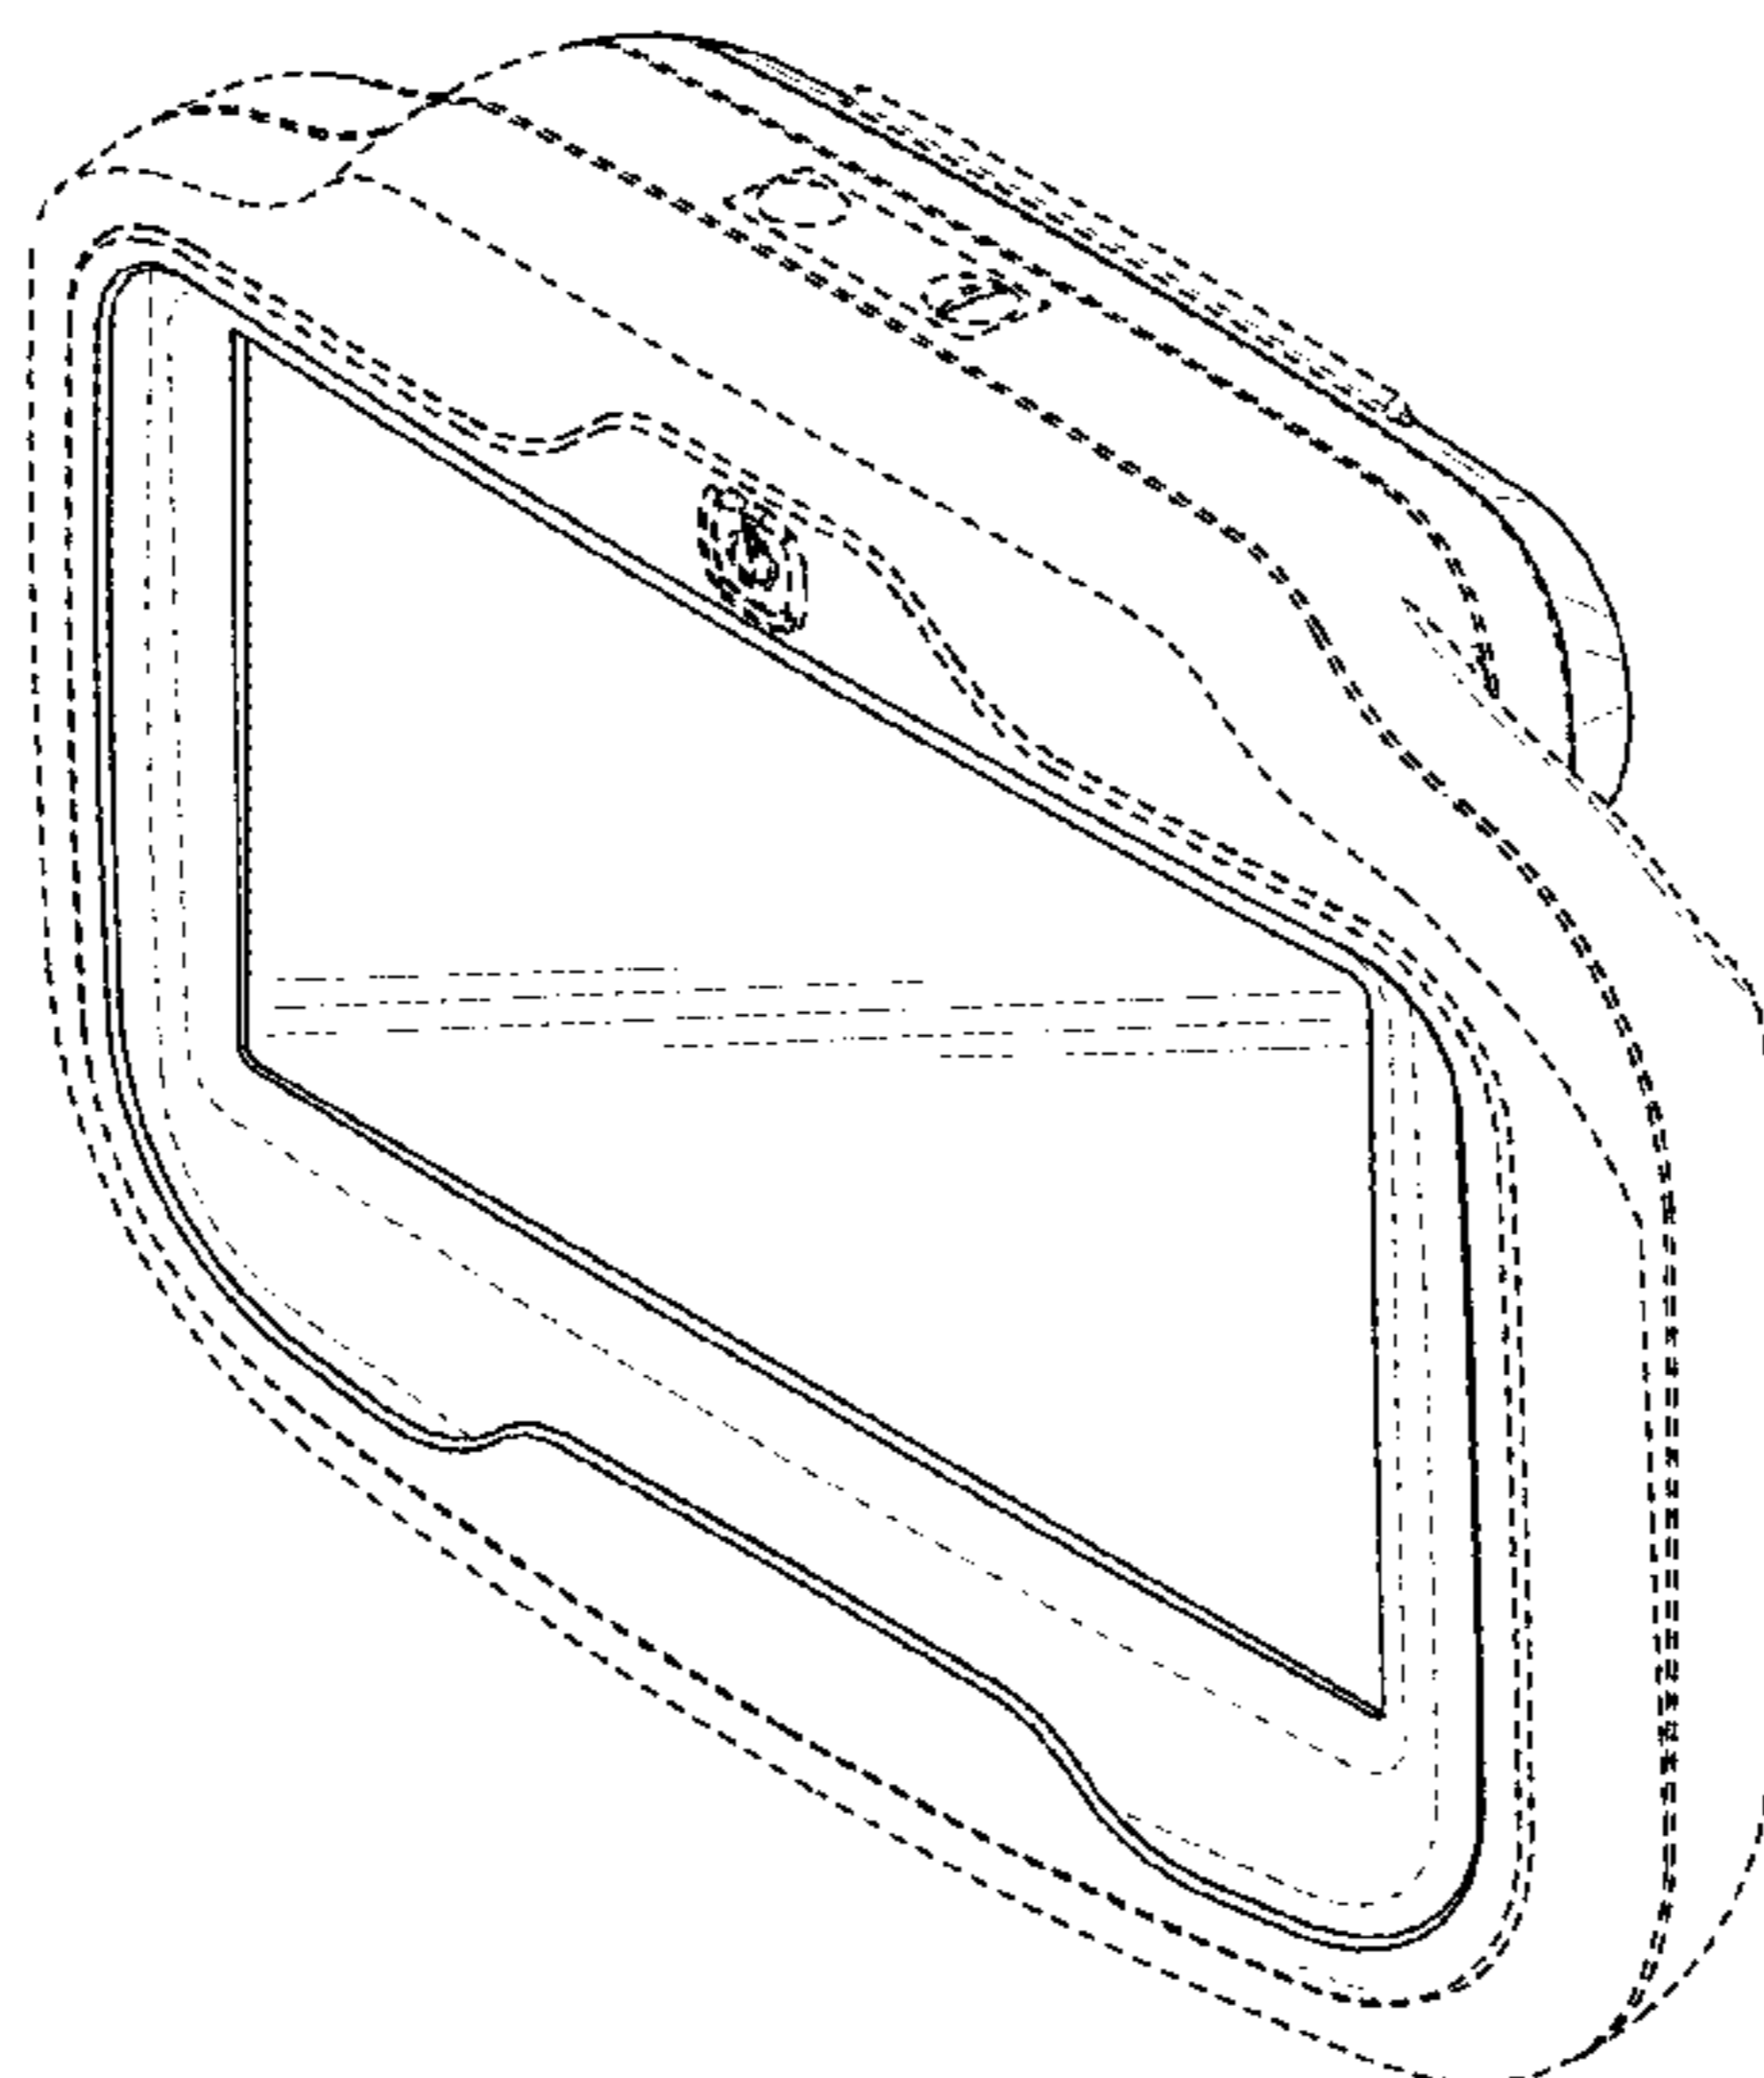

(56)

References Cited

FOREIGN PATENT DOCUMENTS

U.S. PATENT DOCUMENTS

D636,424 S 4/2011 Lin  
 D658,298 S 4/2012 Prpa  
 D677,793 S 3/2013 Prpa  
 D701,606 S 3/2014 Ohmukai  
 D703,331 S 4/2014 Kitayama  
 D703,333 S 4/2014 Saeki  
 D724,234 S 3/2015 Hagege  
 9,042,967 B2 5/2015 Dacosta et al.  
 D733,595 S 7/2015 Hoshino  
 D747,391 S \* 1/2016 Sakai ..... D16/218  
 D748,808 S 2/2016 Matsumura et al.  
 D750,260 S 2/2016 Sauer  
 D753,308 S 4/2016 Marinkovich et al.  
 9,451,882 B2 9/2016 Nie et al.  
 D787,684 S 5/2017 Vezina  
 D802,777 S 11/2017 Burachynsky et al.  
 D810,293 S 2/2018 Peel  
 D822,747 S 7/2018 Van Deusen et al.  
 D822,748 S 7/2018 Van Deusen et al.  
 D827,014 S 8/2018 Sakai  
 D835,271 S 12/2018 Myers et al.  
 D849,105 S 5/2019 Hogstedt et al.  
 D859,498 S 9/2019 Lin  
 D861,176 S 9/2019 Yoon et al.  
 D861,764 S 10/2019 Zhao  
 D862,697 S 10/2019 Kenworthy et al.  
 10,438,356 B2 10/2019 Dacosta  
 D865,836 S \* 11/2019 Puusaari ..... D16/202  
 D865,845 S 11/2019 Sakai  
 D866,764 S 11/2019 Pukall  
 D868,867 S 12/2019 Jean et al.  
 D873,890 S 1/2020 Fidler  
 D907,097 S \* 1/2021 Suurmeijer ..... D16/206  
 D908,161 S 1/2021 Dacosta et al.  
 D908,881 S \* 1/2021 Dacosta ..... D24/158  
 D910,105 S \* 2/2021 Lin ..... D16/202  
 D910,182 S 2/2021 Dacosta et al.  
 D913,354 S \* 3/2021 Marzette, Jr. .... D16/218  
 D914,220 S 3/2021 Nelson et al.  
 D916,294 S 4/2021 Murray et al.  
 D919,690 S \* 5/2021 Suurmeijer ..... D16/206  
 D921,736 S \* 6/2021 Yin ..... D16/208  
 D921,899 S 6/2021 Suarez et al.  
 D922,469 S \* 6/2021 Sjogren ..... D16/203  
 D924,306 S \* 7/2021 Melnicoff ..... D16/218  
 2006/0004292 A1 1/2006 Beylin  
 2010/0145146 A1 6/2010 Melder  
 2014/0180116 A1 6/2014 Lindekugel et al.  
 2014/0276102 A1 9/2014 Lee et al.  
 2015/0182196 A1 7/2015 Ninomiya et al.  
 2016/0045114 A1 2/2016 Dacosta et al.  
 2016/0287211 A1 10/2016 DaCosta et al.  
 2017/0290515 A1 10/2017 Butte et al.  
 2018/0242848 A1 8/2018 Dacosta et al.  
 2018/0279864 A1 10/2018 Frangioni

WO 2017079844 5/2017  
 WO 2019148268 8/2019  
 WO 2019213737 11/2019  
 WO 2020148724 7/2020  
 WO 2020148725 7/2020  
 WO 2020148726 7/2020

OTHER PUBLICATIONS

International Search Report and Written Opinion from International Patent Application No. PCT/IB2020/050384, dated Apr. 22, 2020.  
 International Search Report and Written Opinion from International Patent Application No. PCT/IB2020/050385 dated Apr. 8, 2020.  
 U.S. Appl. No. 62/793,842, filed Jan. 17, 2019.  
 U.S. Appl. No. 62/793,846, filed Jan. 17, 2019.  
 U.S. Appl. No. 621857,183, filed Jun. 4, 2019.  
 UDesign U.S. Appl. No. 29/677,152, filed Jan. 17, 2019.  
 Design U.S. Appl. No. 29/676,901, filed Jan. 15, 2019.  
 Ex Parte Quayle Action in Design U.S. Appl. No. 29/676,901, dated Mar. 5, 2020.  
 Notice of Allowance in Design U.S. Appl. No. 29/676,901, dated Sep. 18, 2020.  
 International Search Report and Written Opinion from International Patent Application No. PCT/CA2019/000015, dated Jun. 4, 2019.  
 “Fluorescent chemical probes for accurate tumor diagnosis and targeting therapy”, 2017, Gao et al. <https://www.researchgate.net/publication/315469453> Fluorescent chemical probes for accurate tumor diagnosis and targeting therapy.  
 “Current concepts and future perspectives on surgical optical imaging in cancer”, 2010, Ntziachristos et al., <https://www.snielibrary.com/Moumals/Jounial-of-Biomedical-Onticstvolume-15issue-61066024/> Current-concepts-and-future-perspeetives-on-surgical-optical-imaging-in/10.1117/1.3523364.full7SSO=I.  
 Notice of Allowance in Design U.S. Appl. No. 29/677,154, dated Apr. 1, 2020.  
 Notice of Allowance in Design U.S. Appl. No. 29/676,901, dated Jun. 4, 2020.  
 International Patent Application No. PCT/IB2020/050383, dated Jan. 17, 2020.  
 Notice of Allowance in Design U.S. Appl. No. 29/677,152, dated Sep. 22, 2020.  
 Ex Parte Quayle Action in Design U.S. Appl. No. 29/677,152, dated Dec. 20, 2019.  
 Design U.S. Appl. No. 29/767,502, filed Jan. 22, 2021.  
 U.S. Appl. No. 17/423,447, filed Jul. 15, 2021.  
 U.S. Appl. No. 17/423,576, filed Jul. 16, 2021.  
 U.S. Appl. No. 17/423,609, filed Jul. 16, 2021.  
 Design U.S. Appl. No. 29/804,808, filed Aug. 23, 2021.  
 European Search Report for EP Application No. EP19746801 dated Sep. 13, 2021, 2 pages.  
 “Nagaya et al. Fluorescence-Guided Surgery”, *Frontiers in Oncology*, vol. 7, Dec. 22, 2017, 16 pp.

\* cited by examiner

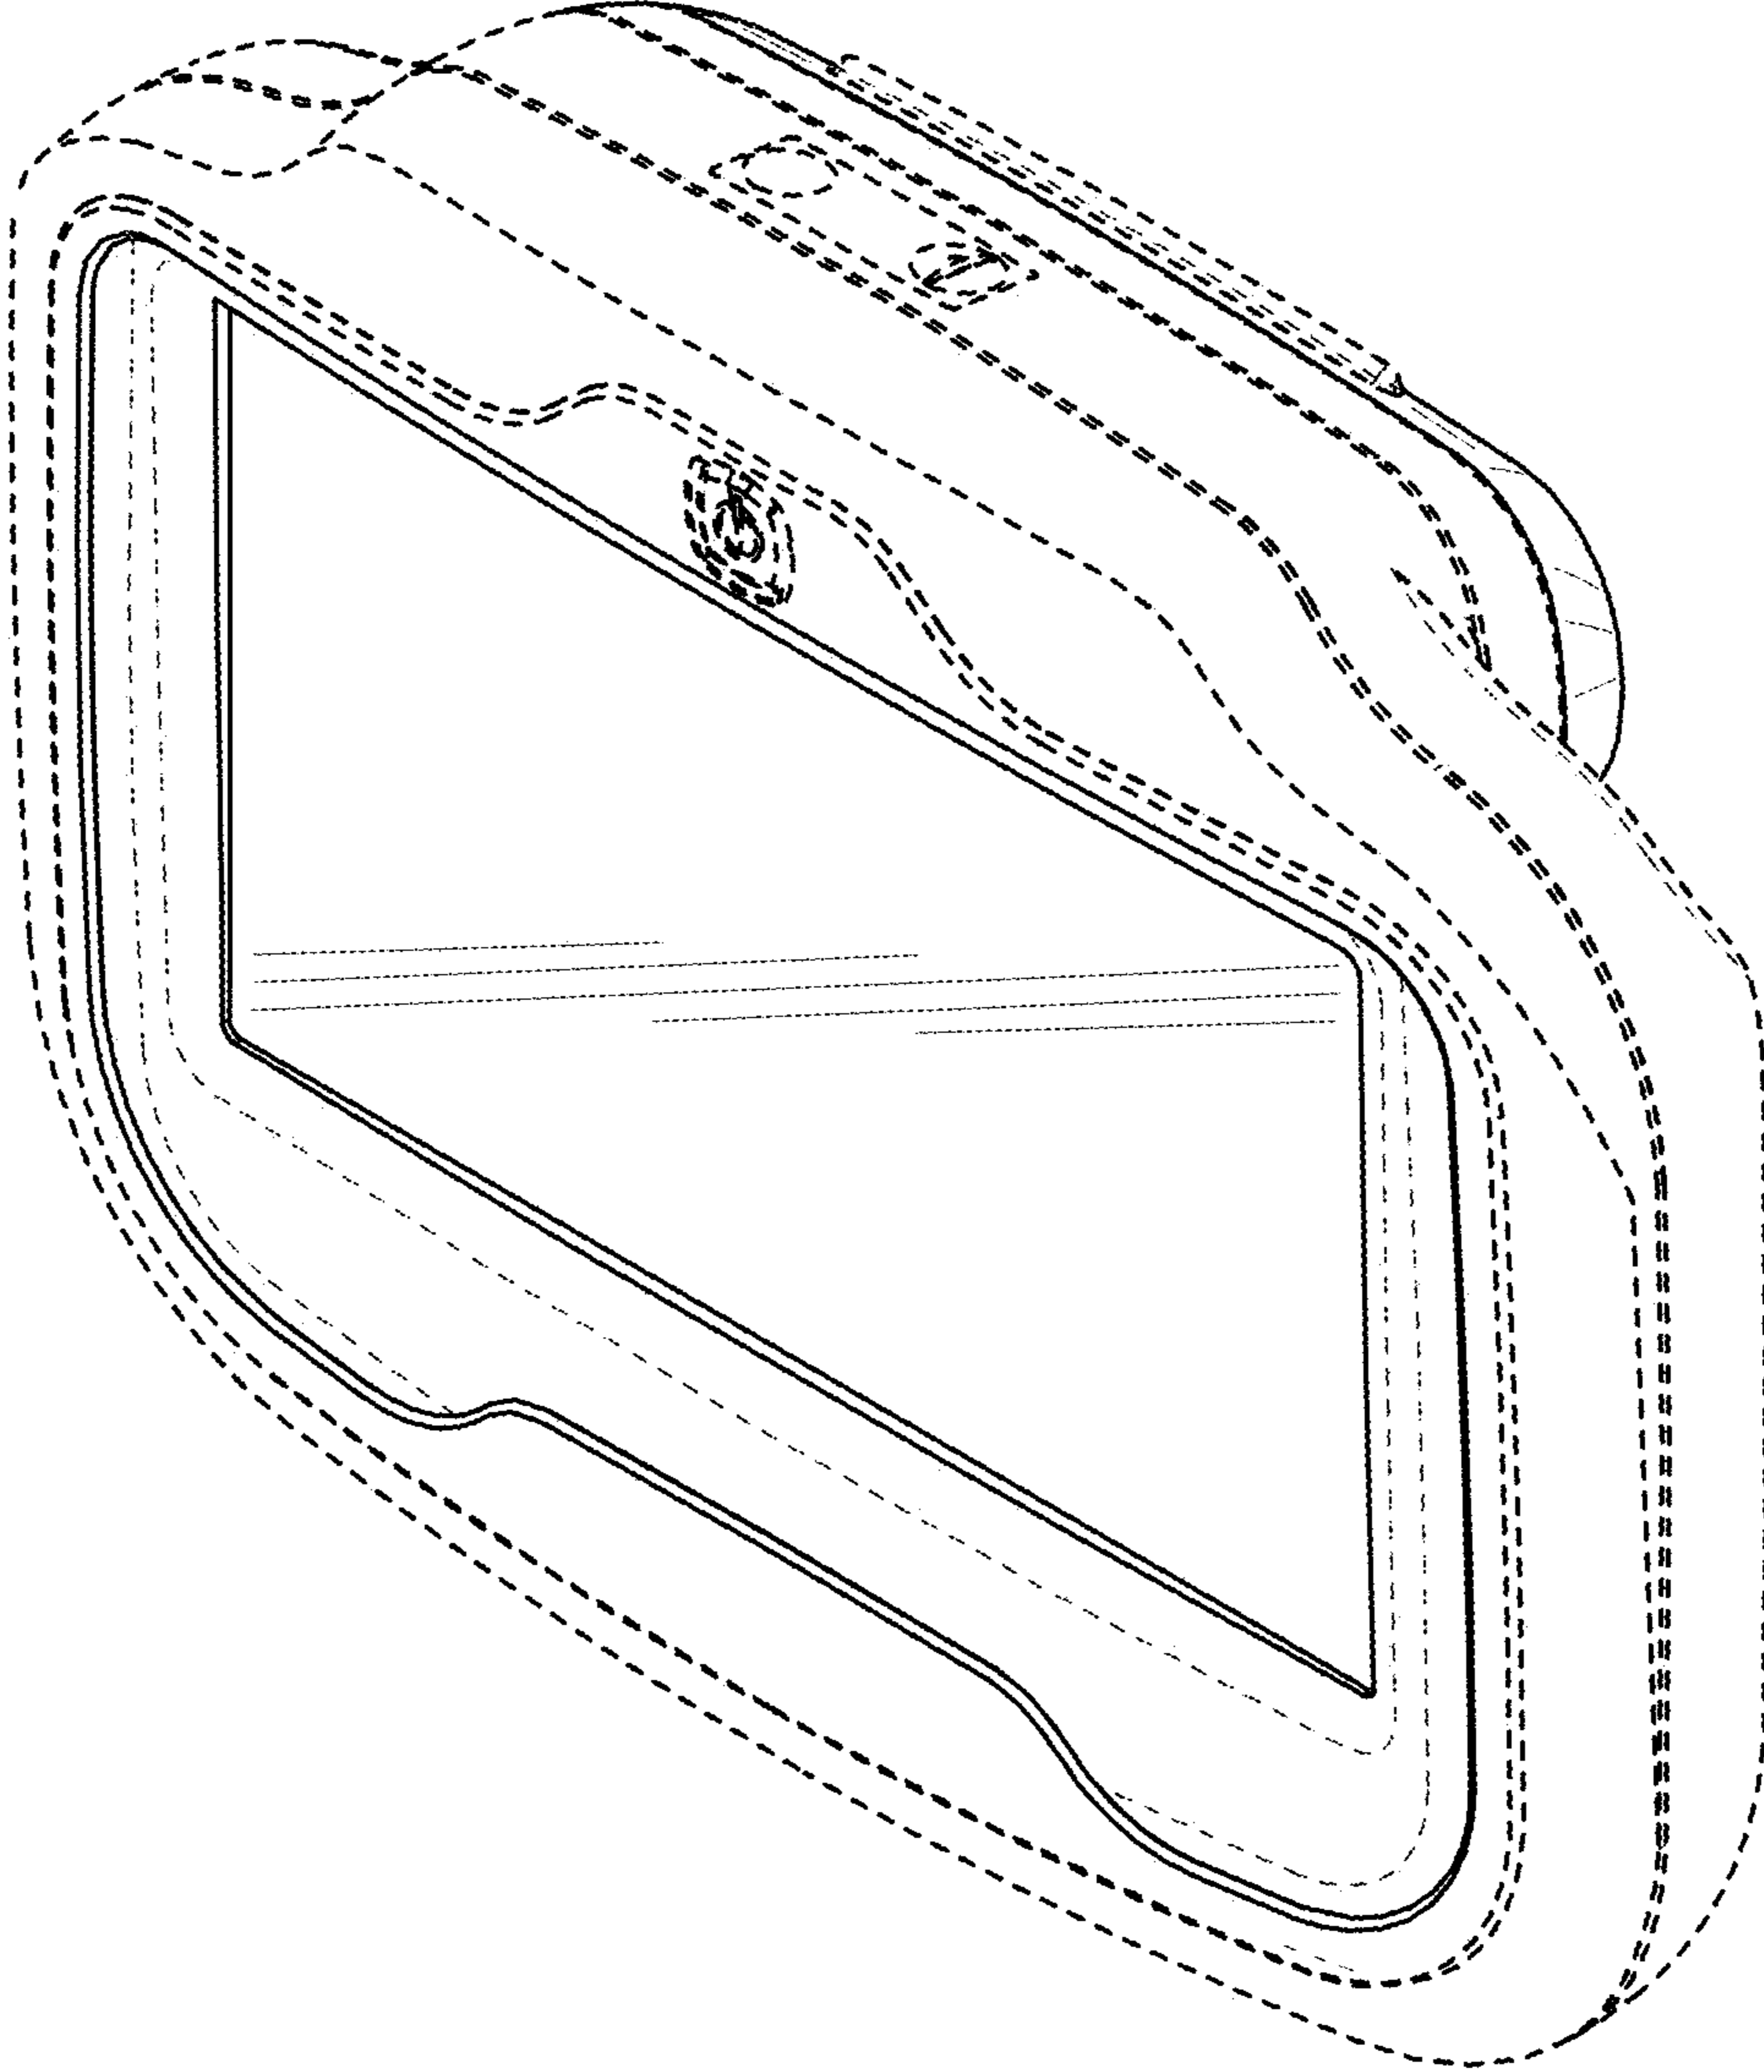


FIG. 1

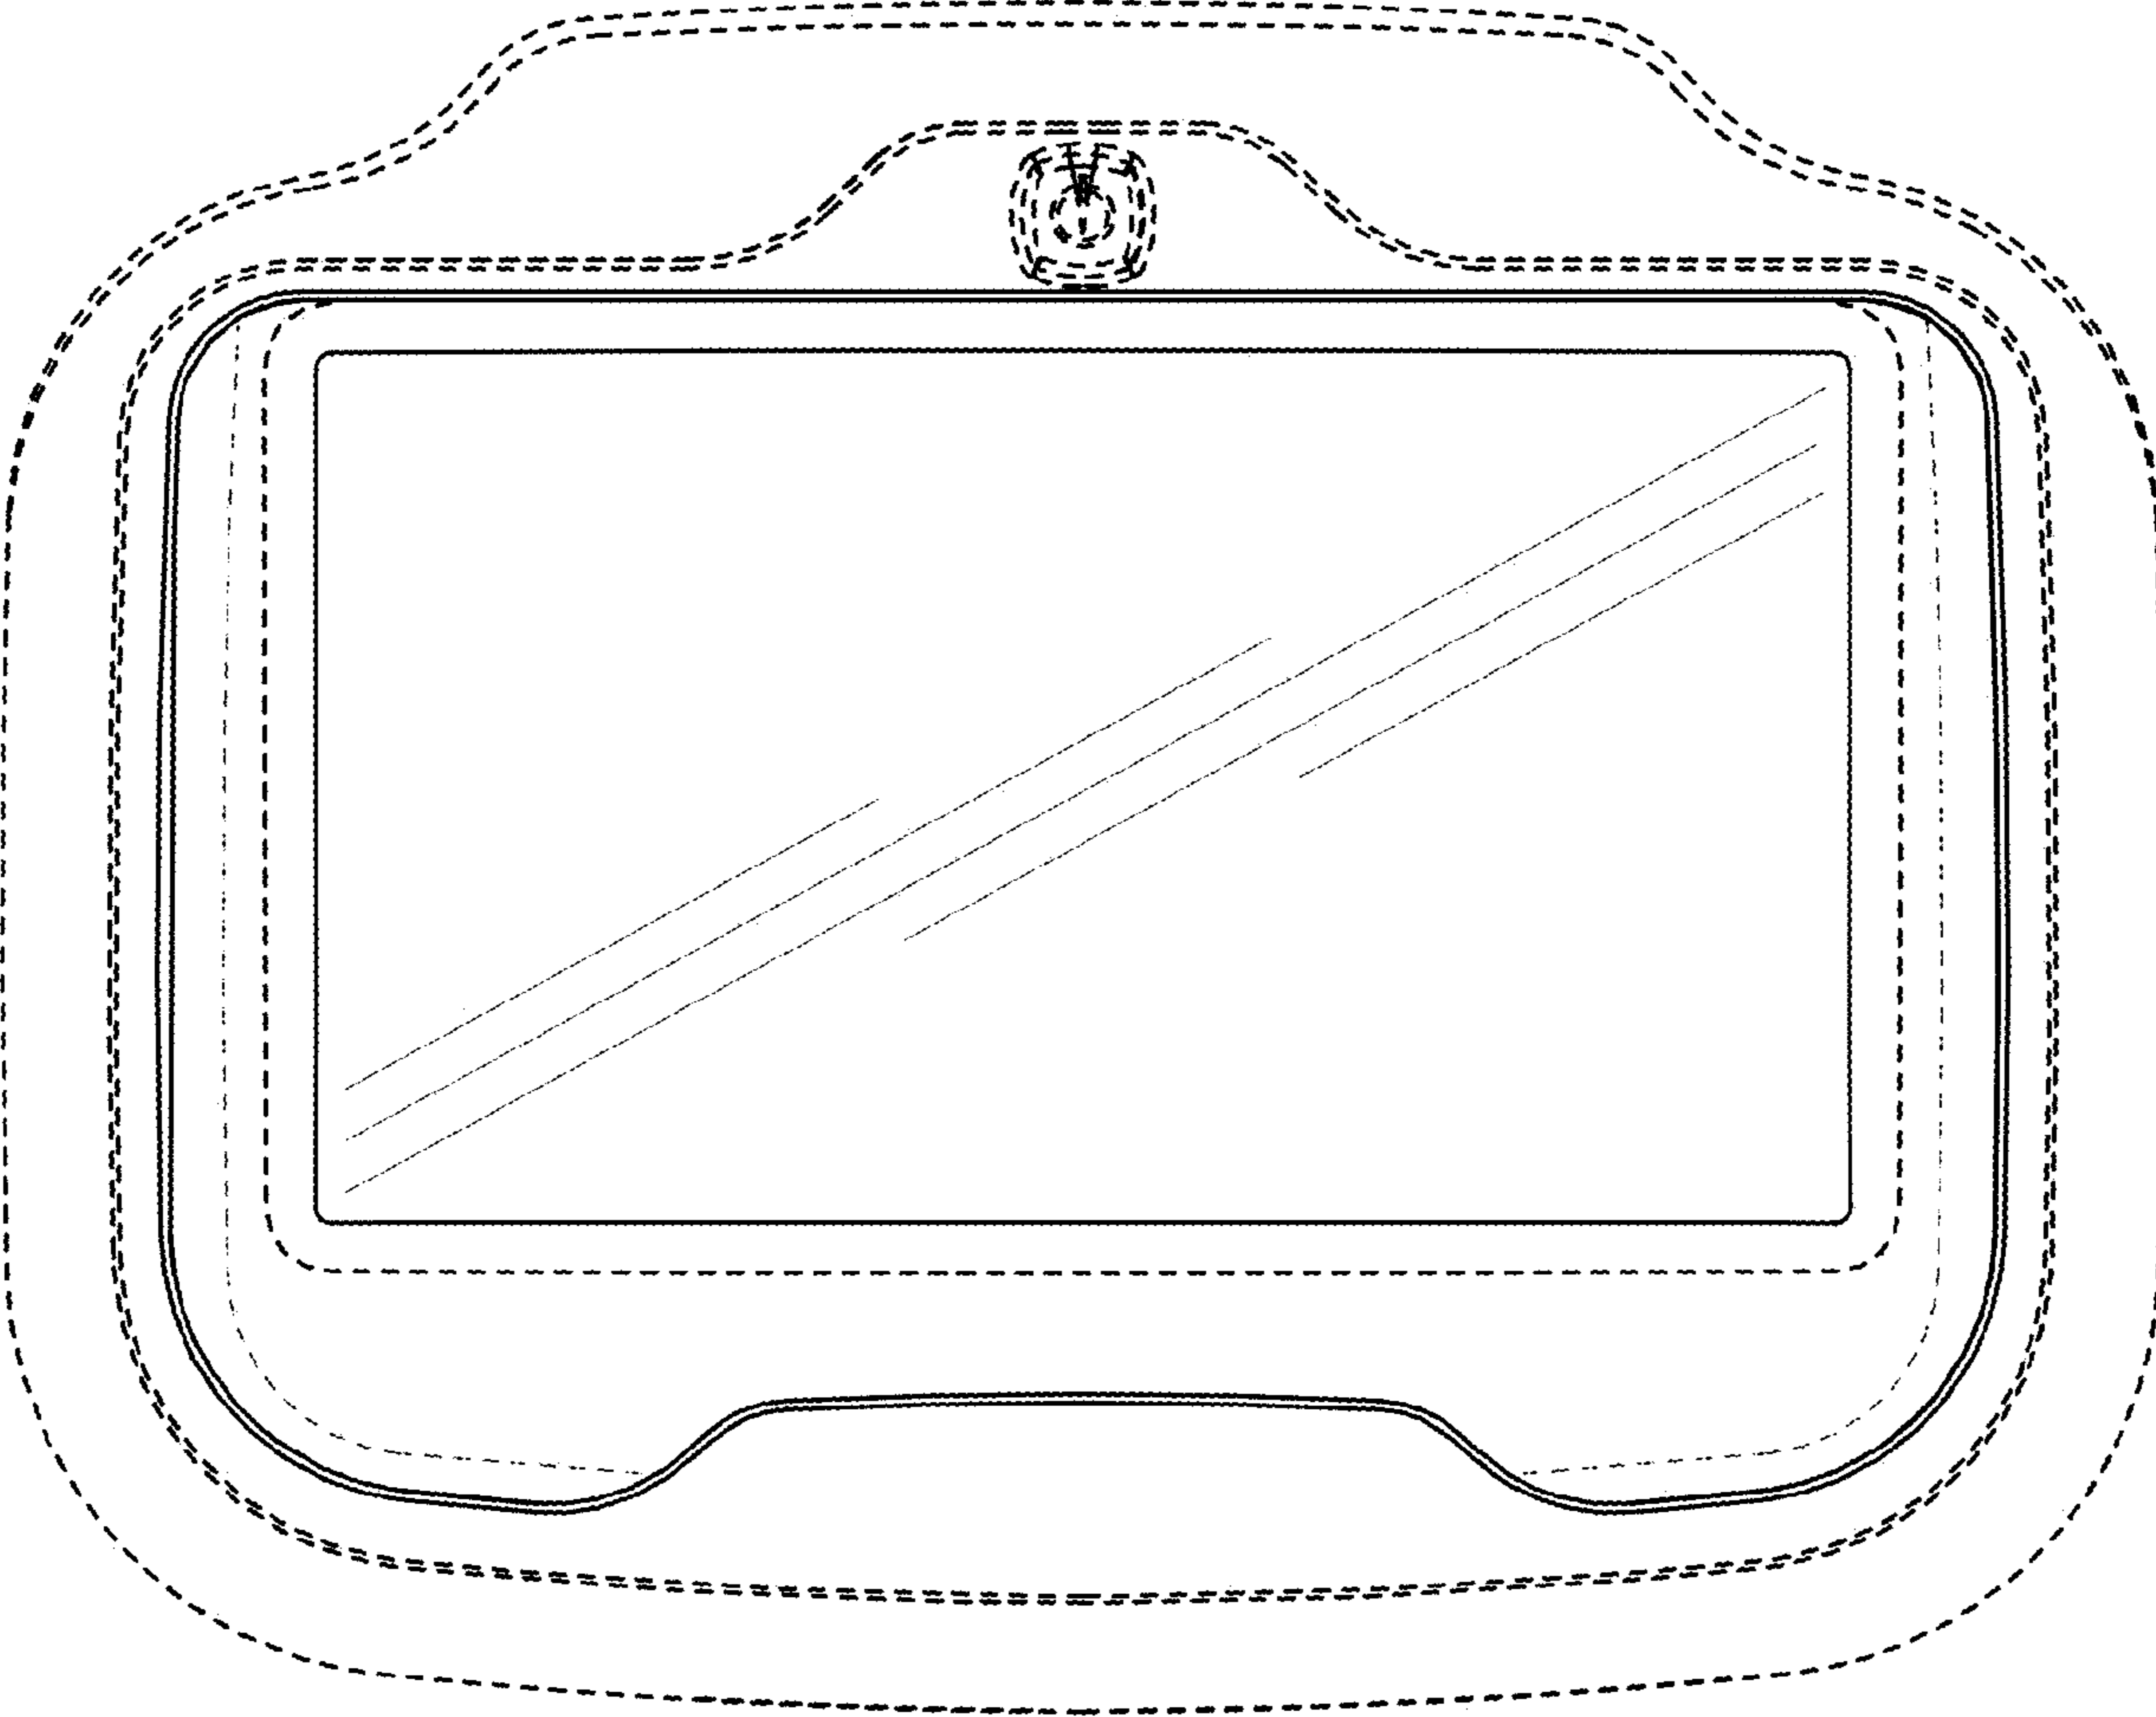


FIG. 2

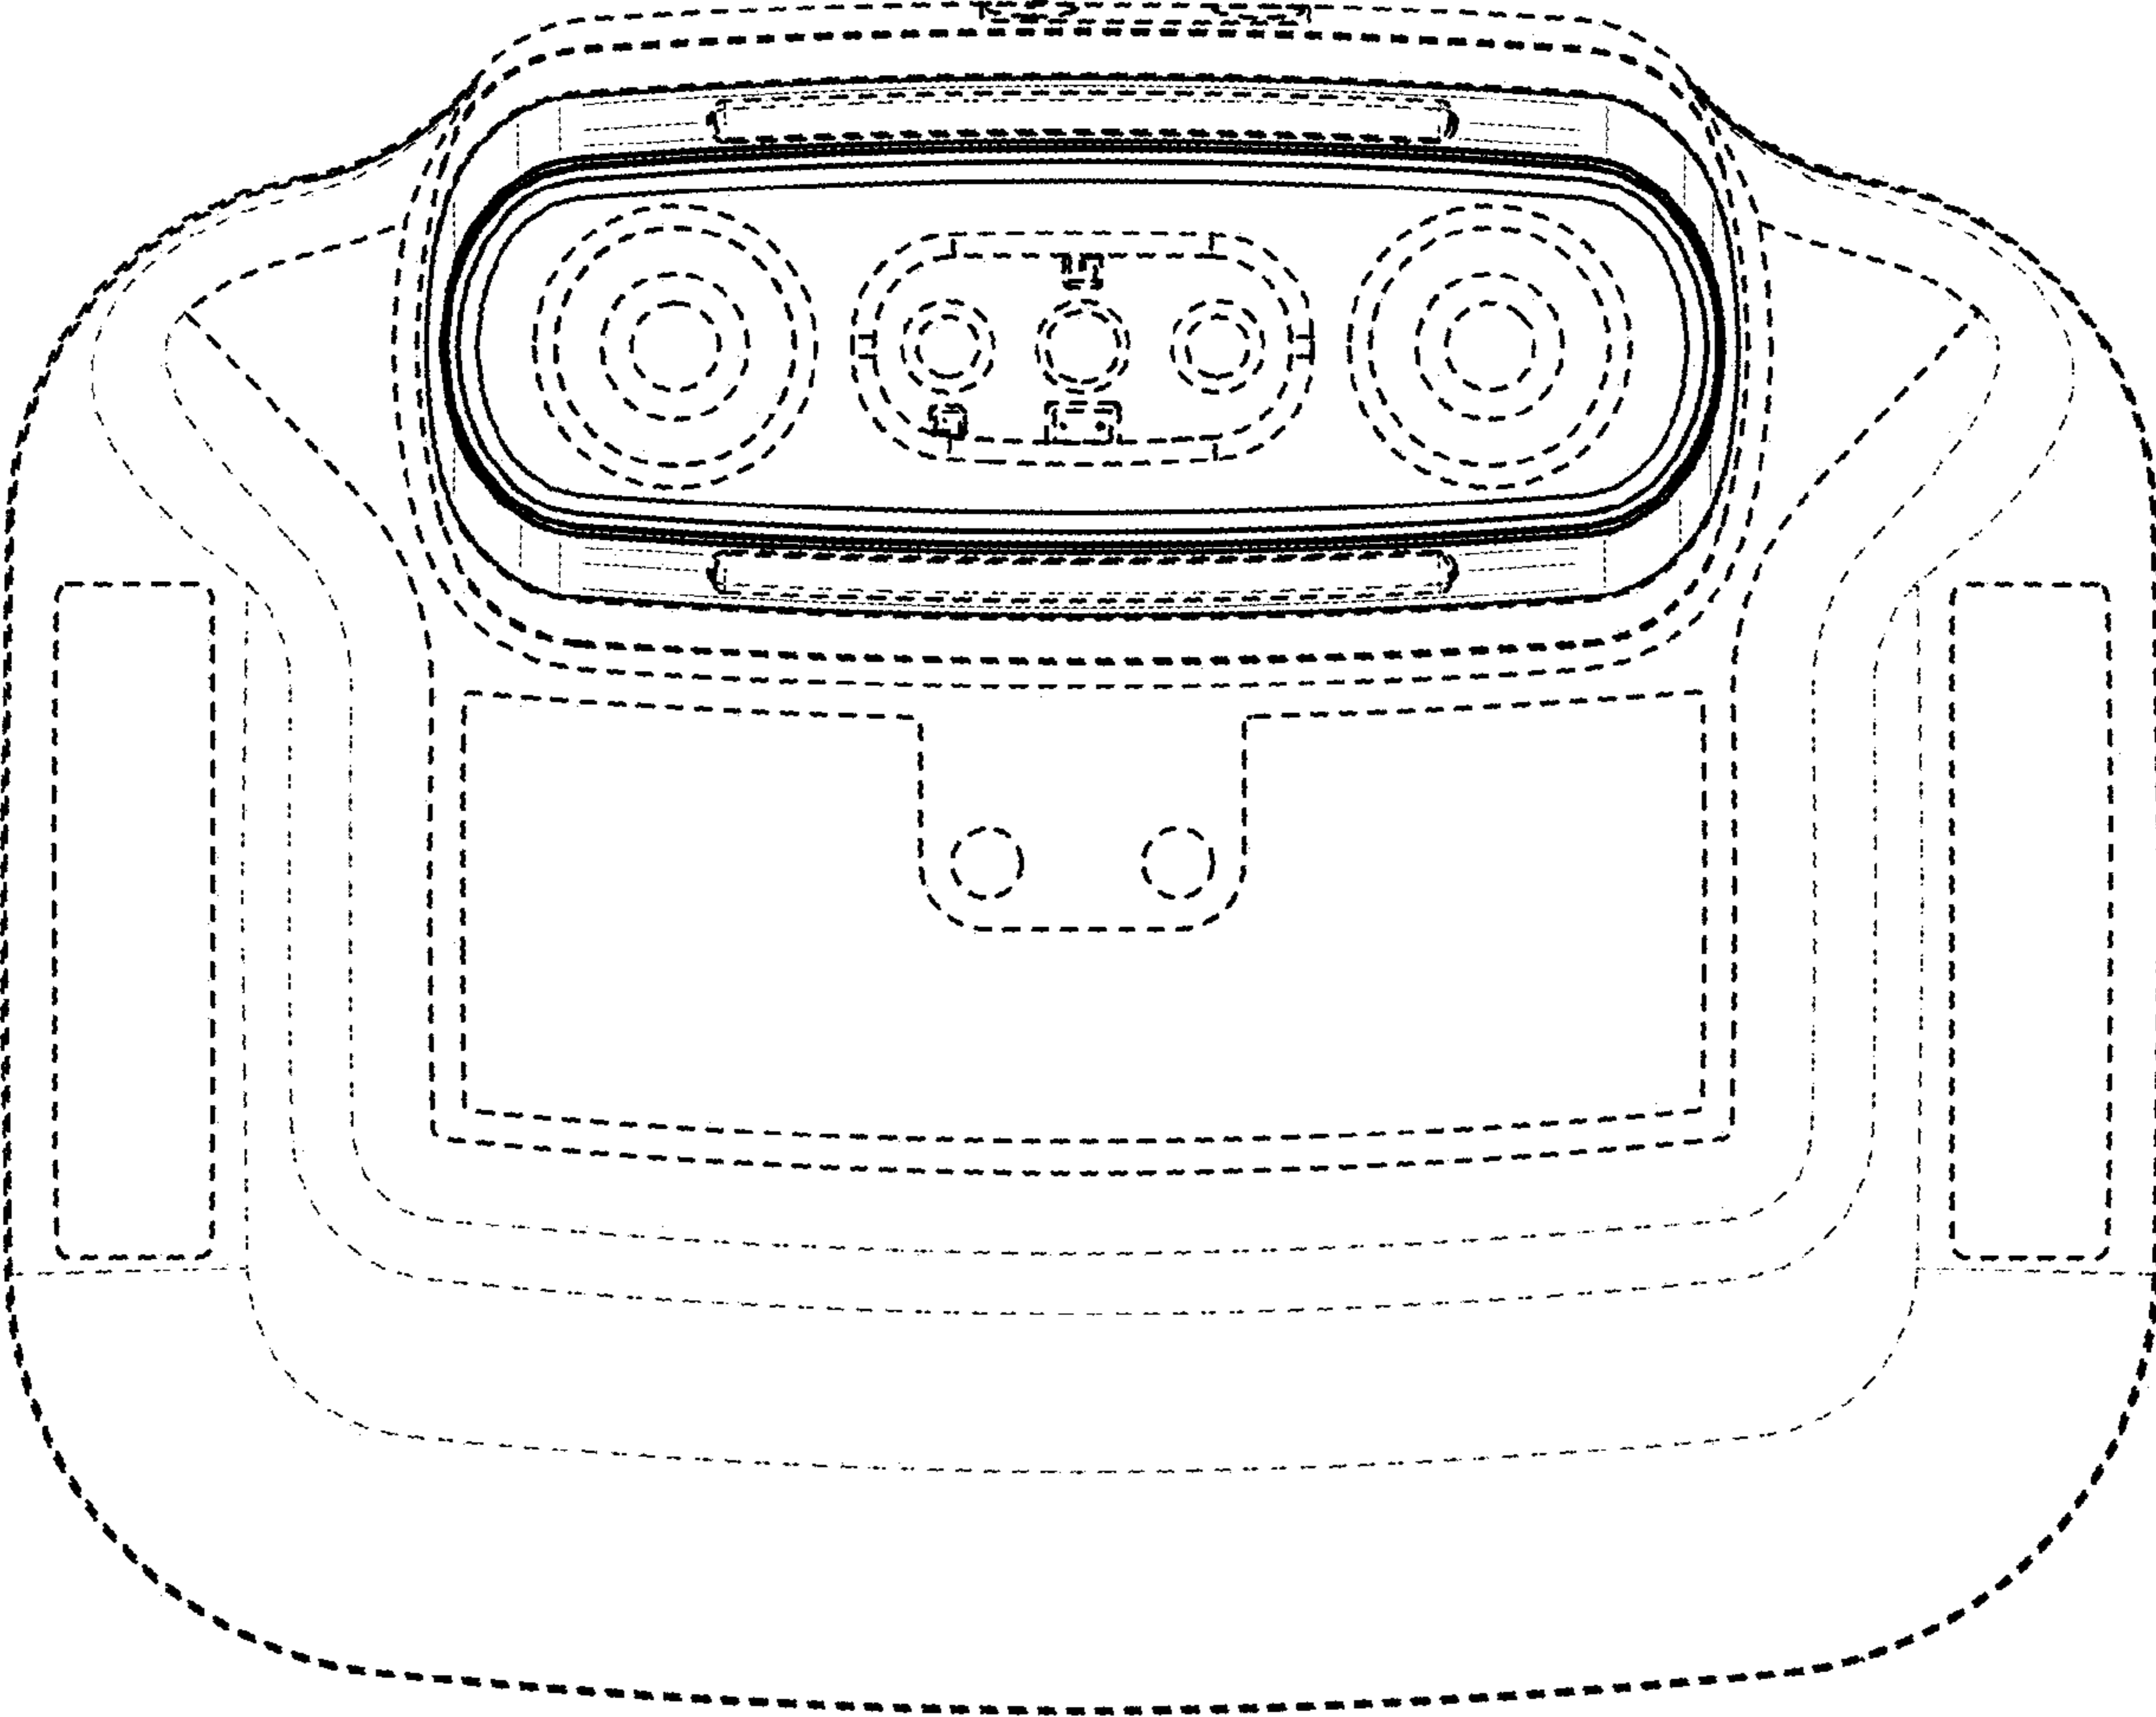


FIG. 3

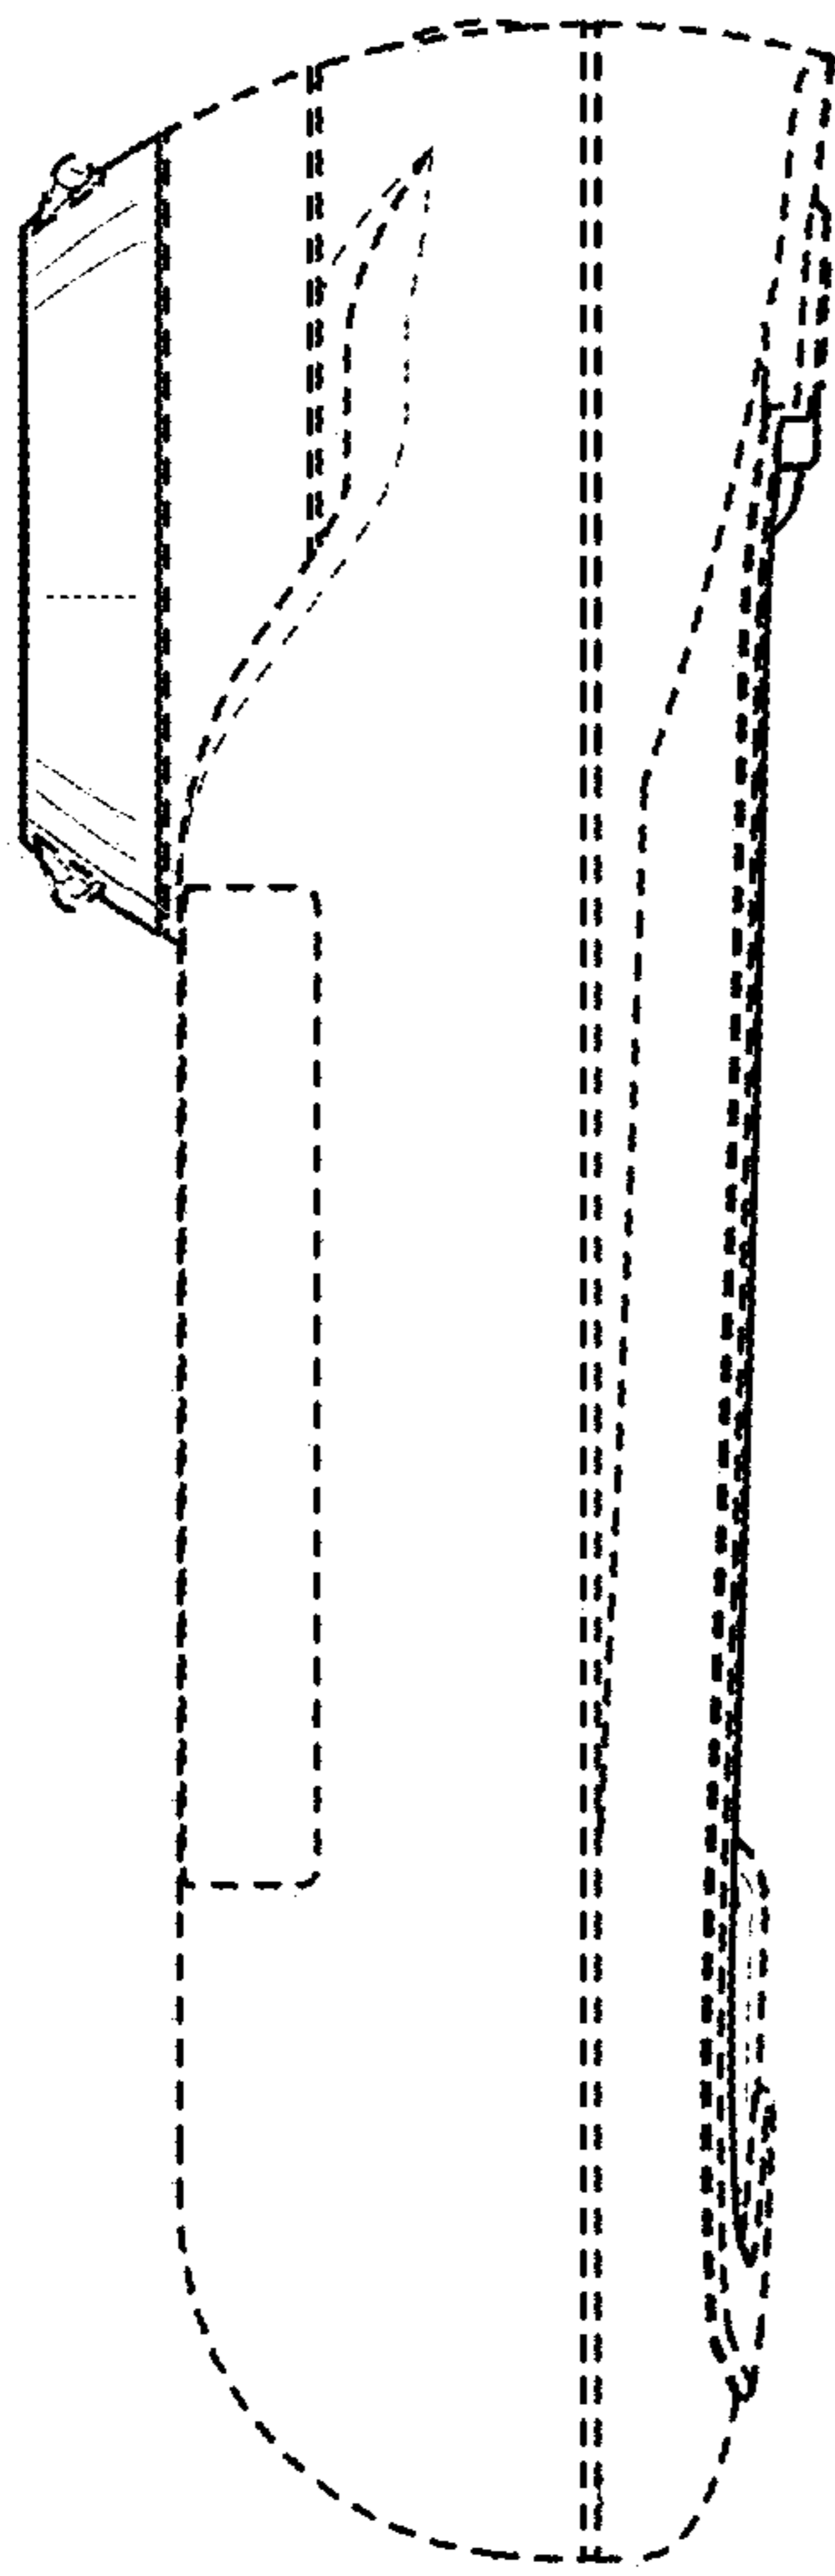


FIG. 4

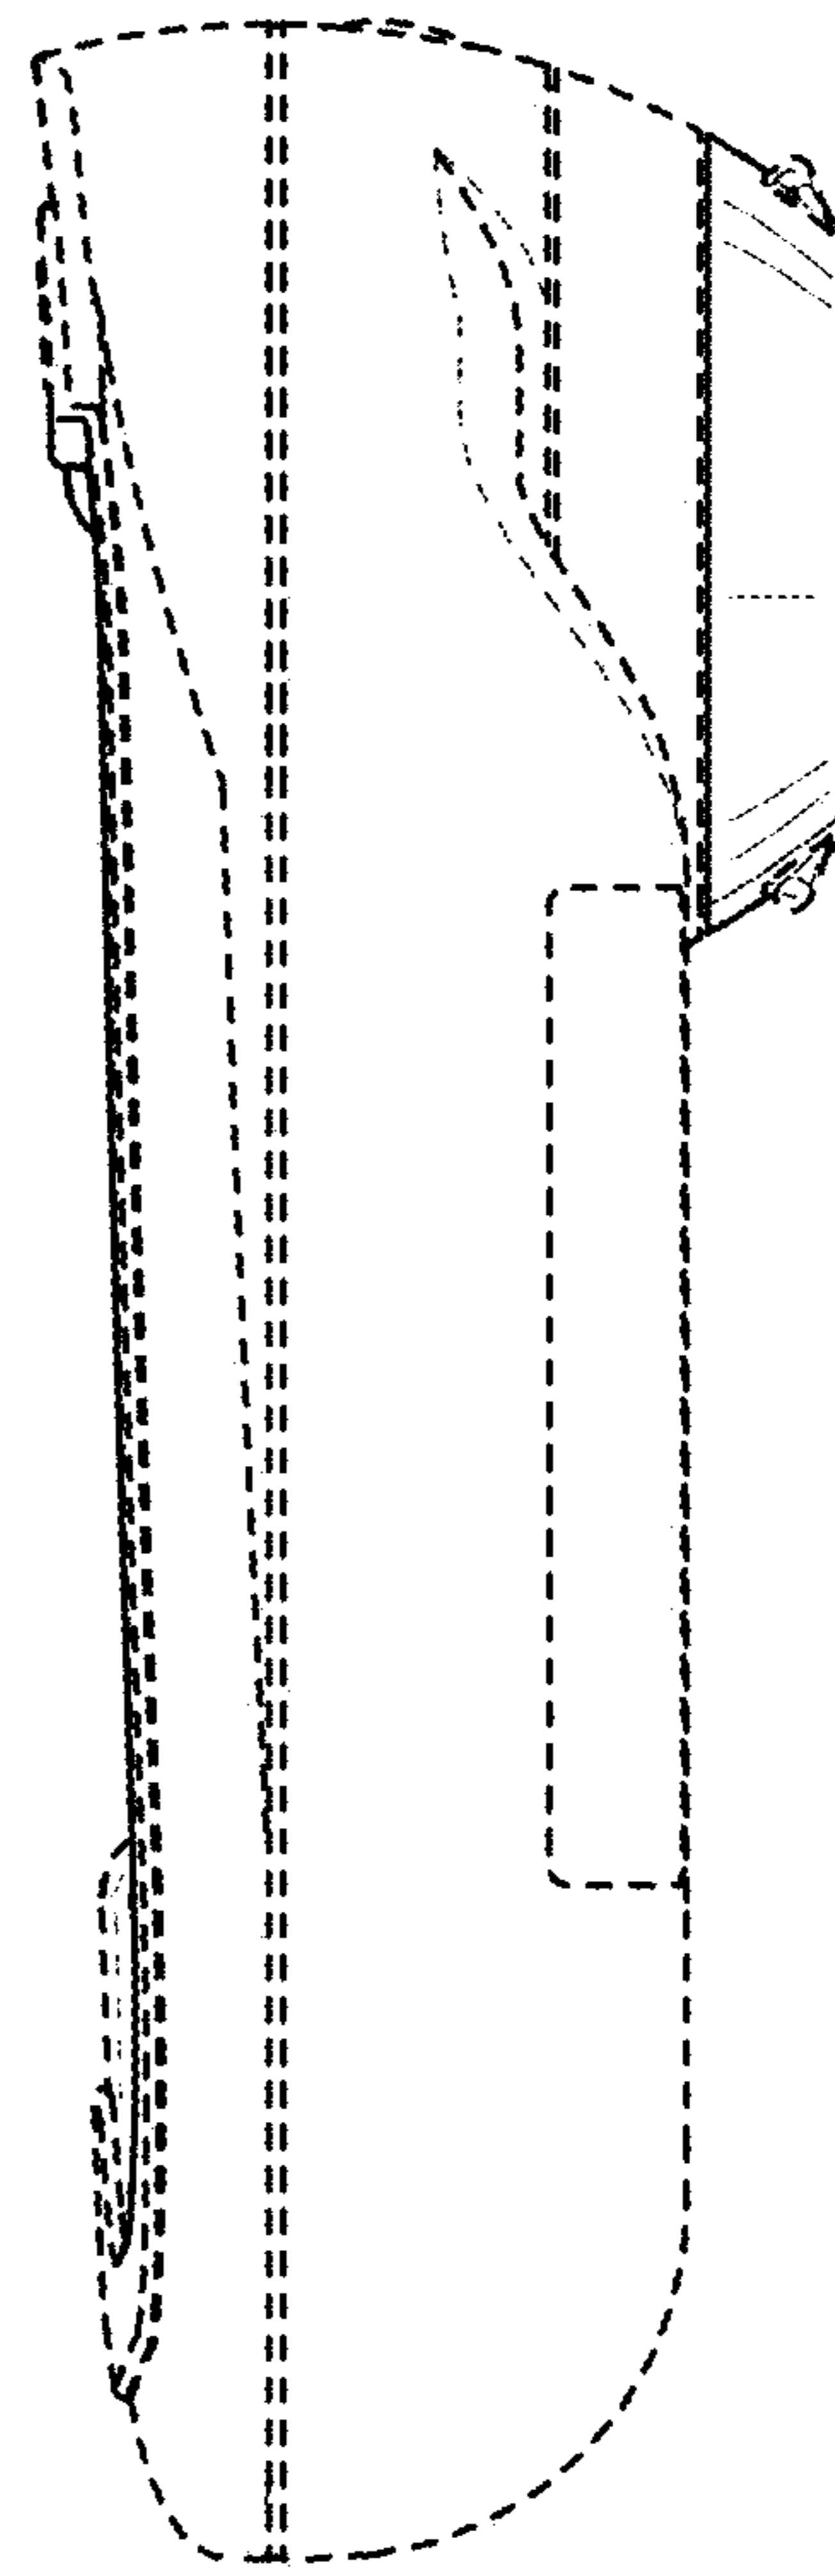


FIG. 5

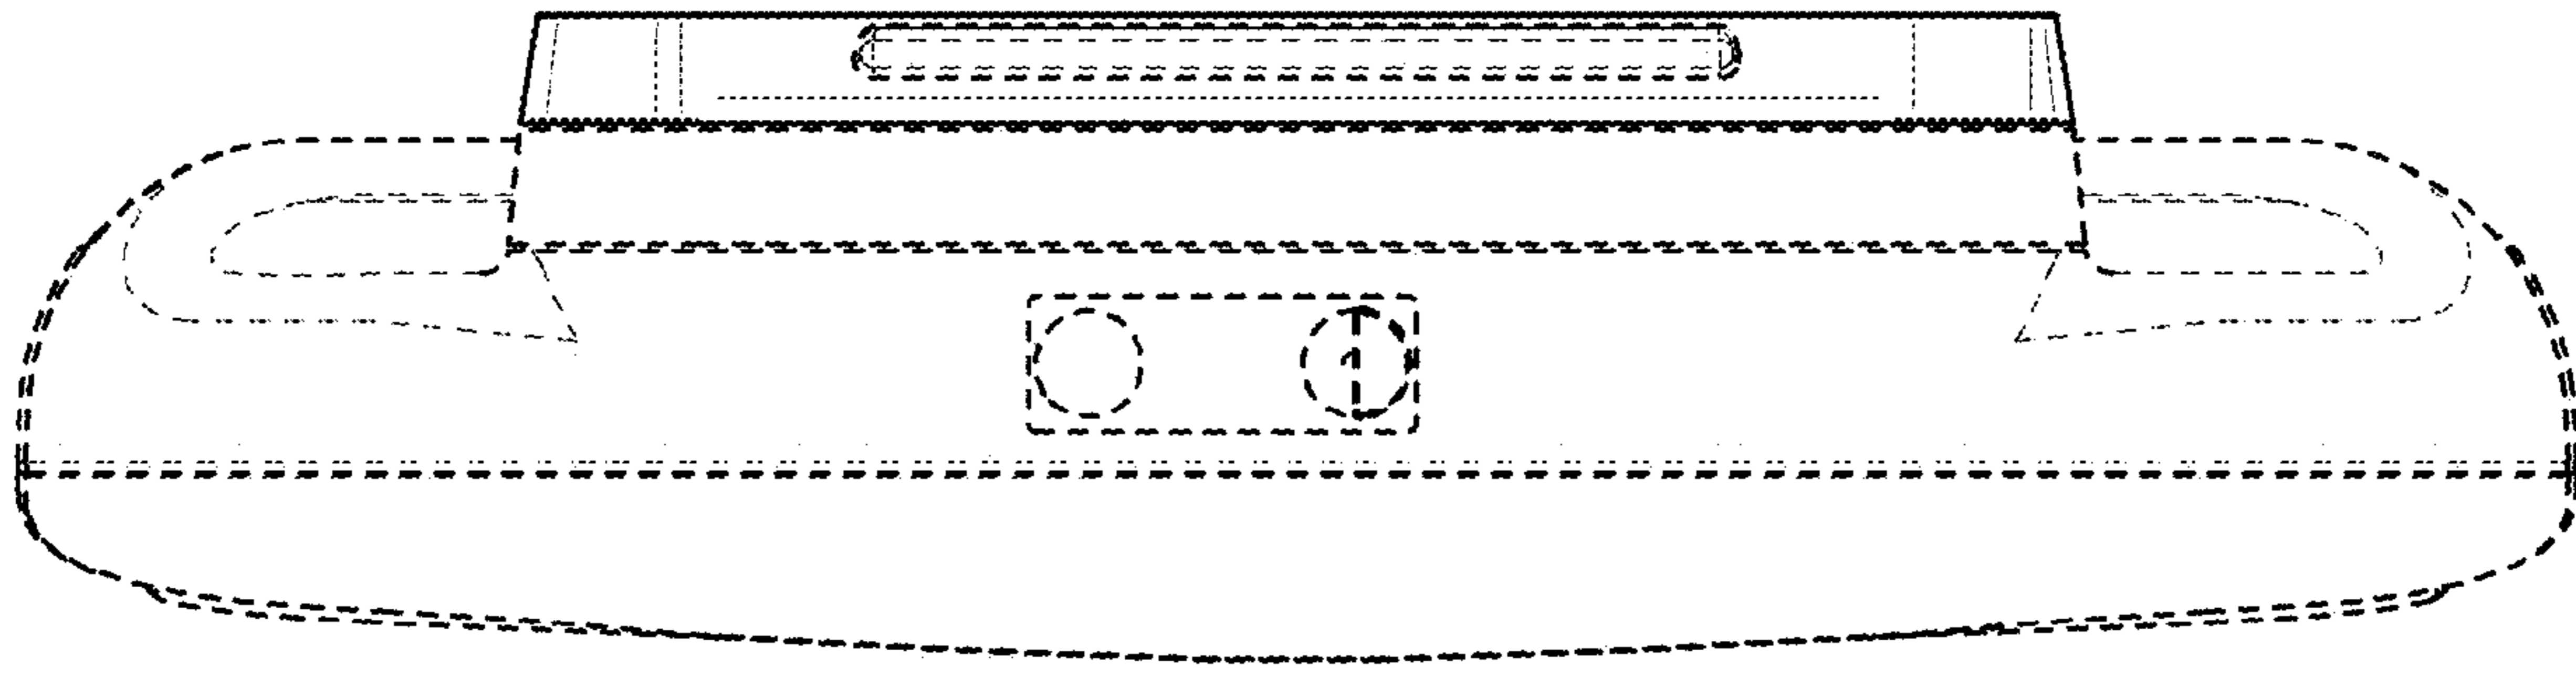


FIG. 6

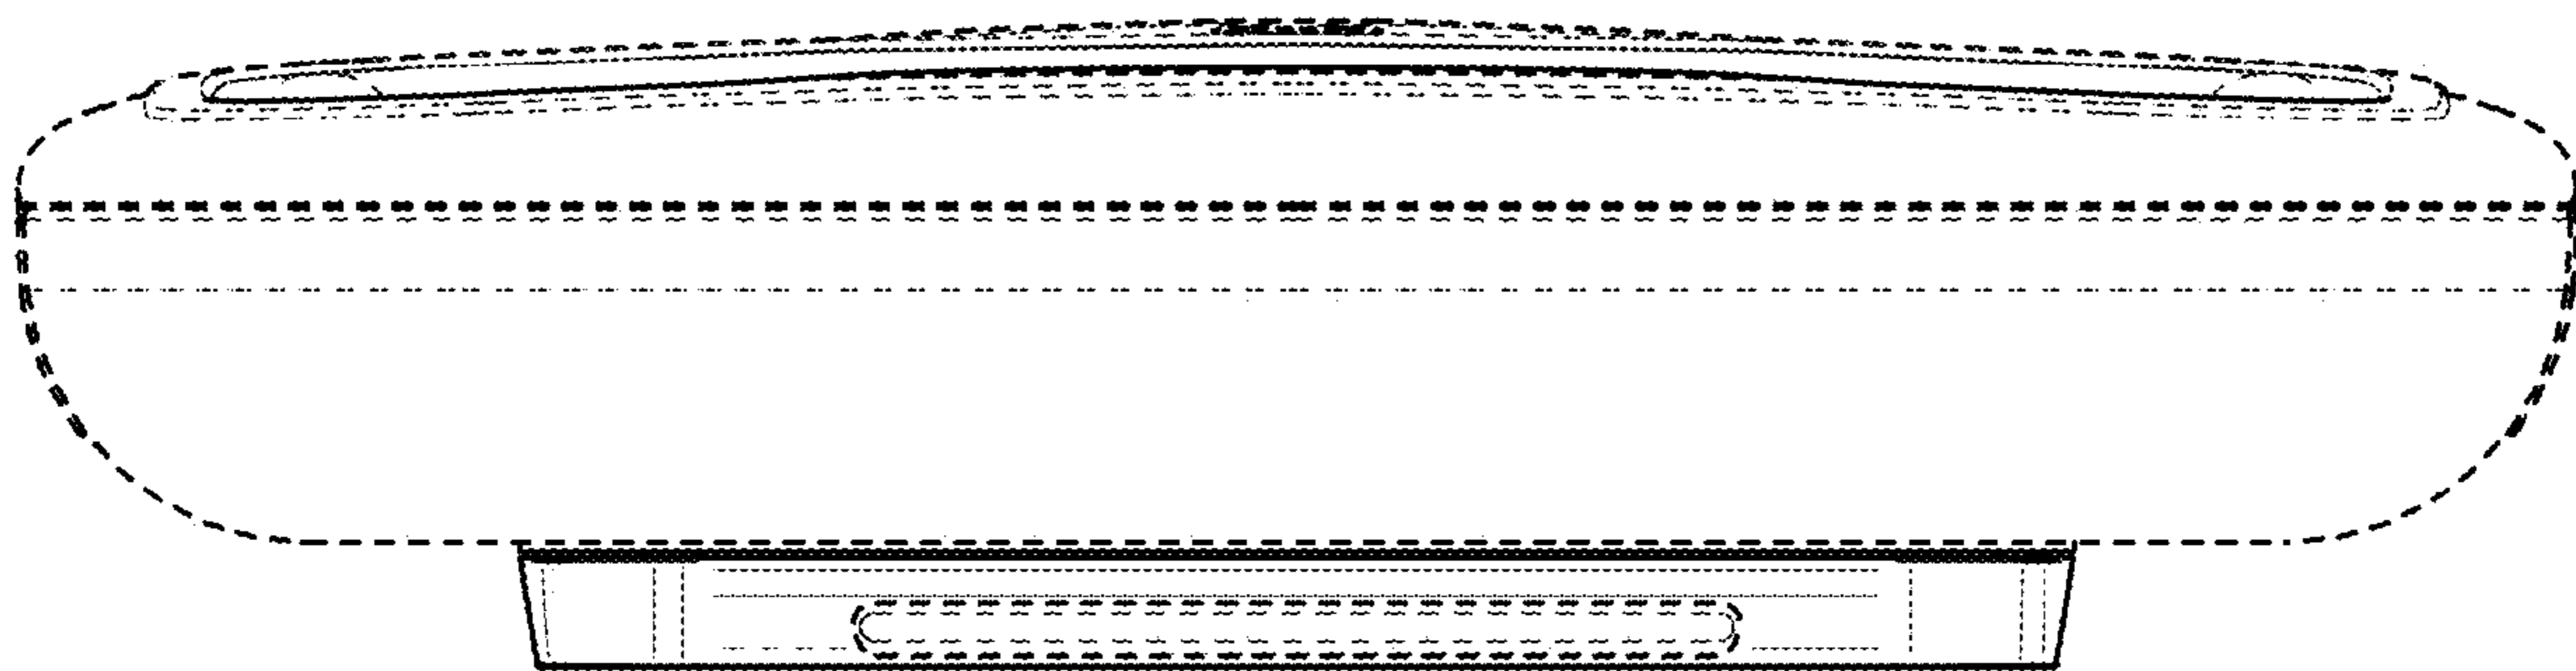


FIG. 7