



US00D952156S

(12) **United States Design Patent** (10) **Patent No.:** **US D952,156 S**  
**Hoan et al.** (45) **Date of Patent:** **\*\* May 17, 2022**

(54) **BRACKET WITH CLIPS** 4,904,245 A 2/1990 Chen et al.  
5,417,395 A 5/1995 Fowler et al.  
(71) Applicant: **Edwards Lifesciences Corporation,** 5,643,218 A 7/1997 Lynn et al.  
Irvine, CA (US) 5,961,472 A 10/1999 Swendson et al.  
6,105,912 A 8/2000 Lindsay et al.  
(72) Inventors: **Andrew Nguyen Hoan,** Irvine, CA 6,156,019 A 12/2000 Langevin  
(US); **Mandana Farhadieh,** Tustin, CA D494,049 S \* 8/2004 Ziaylek ..... D8/373  
(US); **Brian Patrick Murphy,** Costa 7,240,882 B2 7/2007 Degentesh et al.  
Mesa, CA (US) 7,744,573 B2 6/2010 Gordon et al.  
D618,987 S \* 7/2010 Ziaylek ..... D8/373  
D620,783 S \* 8/2010 Ziaylek ..... D8/373  
(73) Assignee: **Edwards Lifesciences Corporation,**  
Irvine, CA (US) (Continued)

**FOREIGN PATENT DOCUMENTS**

(\*\*) Term: **15 Years** CN 107374648 A 11/2017  
EP 2689797 A1 1/2014  
(21) Appl. No.: **29/665,012** (Continued)

(22) Filed: **Sep. 28, 2018**

**OTHER PUBLICATIONS**

**Related U.S. Application Data**

(63) Continuation of application No. 15/801,009, filed on  
Nov. 1, 2017, now abandoned.  
(51) **LOC (13) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/169**  
(58) **Field of Classification Search**  
USPC ..... D8/354, 366, 371, 372, 367, 374, 373,  
D8/376, 375, 16, 19, 45, 380, 381, 394,  
D8/71, 365; D24/111, 169  
See application file for complete search history.

BIOPAC Systems, Inc., NonInvasive Blood Pressure Amplifier,  
Oct. 2, 2017, Inset Figure—Clamp.  
(Continued)

*Primary Examiner* — Eliza Z Bennett-Hattan  
*Assistant Examiner* — Eliza Z Harvey

(57) **CLAIM**

The ornamental design for a bracket with clips, as shown  
and described.


**DESCRIPTION**

(56) **References Cited**  
U.S. PATENT DOCUMENTS

2,954,028 A 9/1960 Smith  
3,157,201 A 11/1964 Littman  
3,780,972 A 12/1973 Brodersen  
4,211,380 A 7/1980 Lillegard et al.  
4,428,383 A 1/1984 DeVroom  
4,858,127 A 8/1989 Kron et al.  
4,865,583 A 9/1989 Tu

FIG. 1 is a bottom right perspective view of the design.  
FIG. 2 is a front view thereof.  
FIG. 3 is a back view thereof.  
FIG. 4 is a right side view thereof.  
FIG. 5 is a left side view thereof; and,  
FIG. 6 is a top plan view thereof.

**1 Claim, 4 Drawing Sheets**

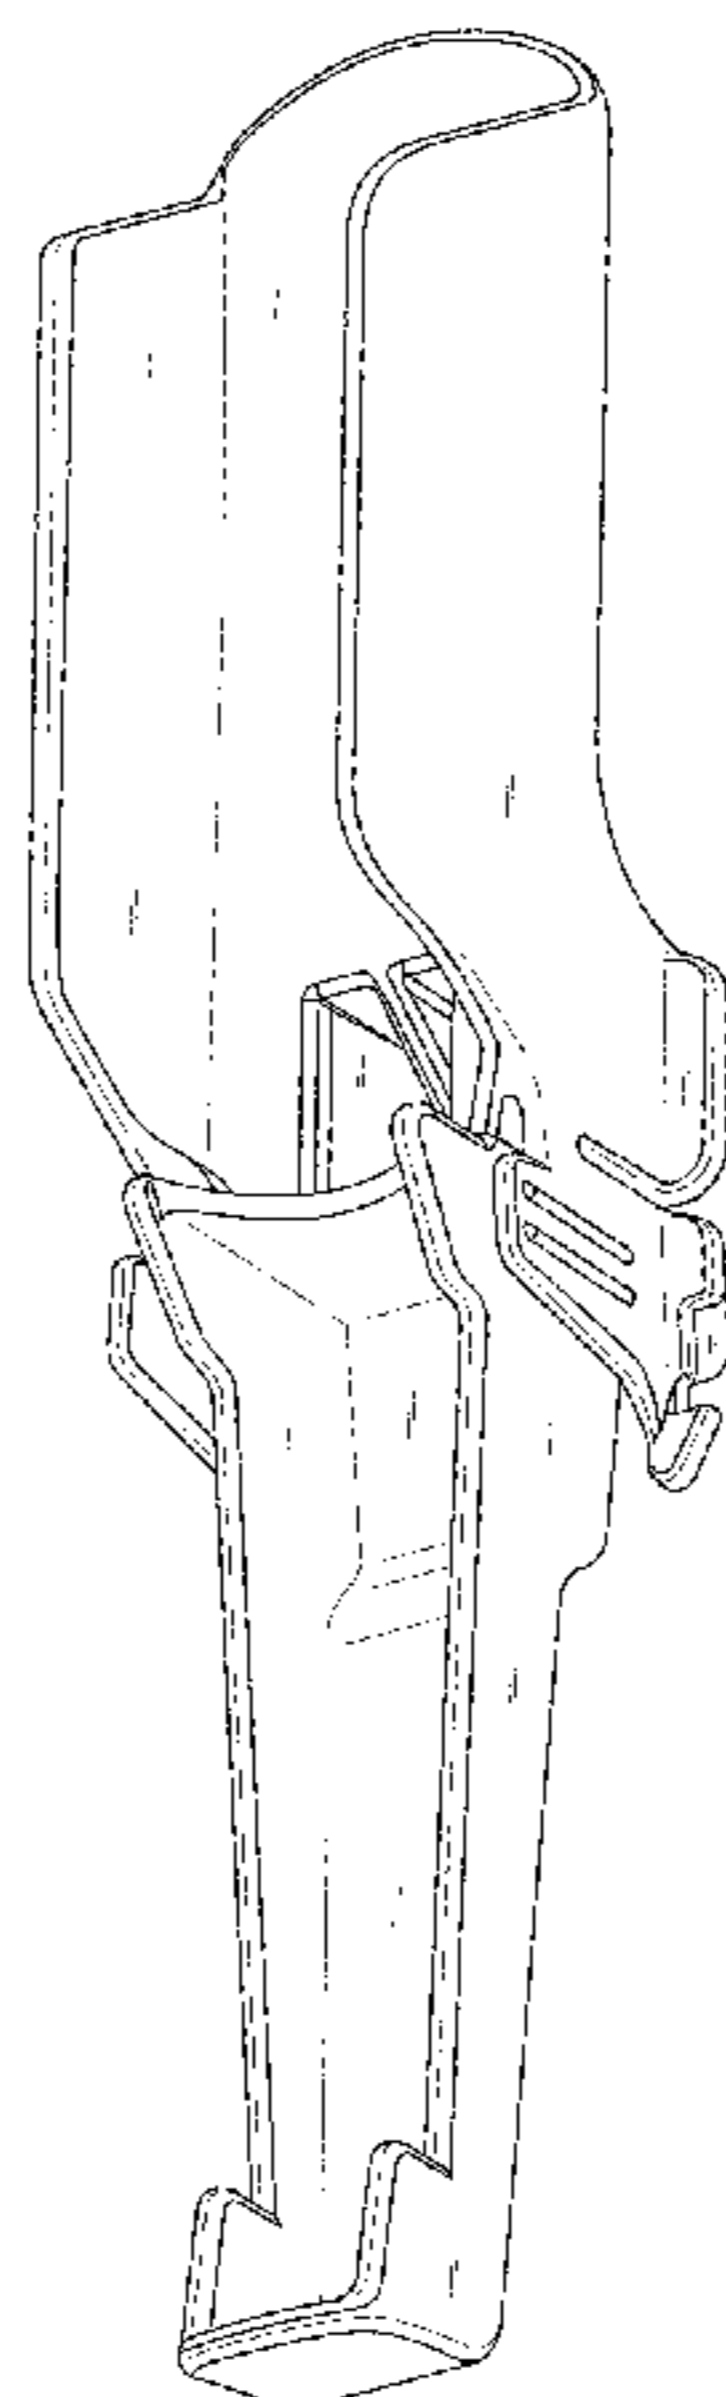

(56)

**References Cited**

U.S. PATENT DOCUMENTS

7,918,422 B2 4/2011 Blankenship et al.  
 7,963,951 B2 6/2011 Kitani et al.  
 D661,979 S \* 6/2012 Schwenkenberg ..... D8/373  
 8,348,844 B2 1/2013 Kunjan et al.  
 8,382,696 B2 2/2013 Beiriger et al.  
 8,403,874 B2 3/2013 Baraldi  
 8,662,458 B2 3/2014 Henault et al.  
 8,668,178 B2 3/2014 Ziaylek et al.  
 D707,543 S \* 6/2014 Schwenkenberg ..... D8/373  
 8,764,668 B2 7/2014 Roteliuk et al.  
 D715,135 S \* 10/2014 Vecchiarelli ..... D8/373  
 8,945,051 B2 2/2015 Schriver et al.  
 8,986,262 B2 3/2015 Young et al.  
 9,016,316 B2 4/2015 Ziv et al.  
 9,022,981 B2 5/2015 Oesterreich et al.  
 9,259,527 B2 2/2016 Spohn et al.  
 D754,001 S \* 4/2016 Barrier ..... D9/455  
 9,370,324 B2 6/2016 Barrett et al.  
 9,375,561 B2 6/2016 Mansour et al.  
 D773,292 S \* 12/2016 Ziaylek ..... D8/373  
 D777,562 S \* 1/2017 Ziaylek ..... D8/373  
 9,566,385 B2 2/2017 Franks

2004/0210162 A1 10/2004 Wyatt et al.  
 2007/0119508 A1 5/2007 West et al.  
 2008/0200837 A1 8/2008 Frazier et al.  
 2008/0302932 A1 12/2008 Mosler et al.  
 2013/0060205 A1 3/2013 Mansour et al.  
 2014/0276215 A1 9/2014 Nelson et al.  
 2015/0196749 A1 7/2015 Ziv et al.  
 2016/0144110 A1 5/2016 Ueda  
 2016/0346472 A1 12/2016 Mitchell et al.

FOREIGN PATENT DOCUMENTS

FR 2914840 A1 10/2008  
 WO 8500982 A1 3/1985  
 WO 2013146752 A1 10/2013  
 WO 2016041948 A1 3/2016  
 WO 2017051536 A1 3/2017

OTHER PUBLICATIONS

Mark Siobal, Analysis and Monitoring of Gas Exchange, <https://clinicalgate.com/analysis-and-monitoring-of-gas-exchange/>, Jan. 6, 2015.

\* cited by examiner

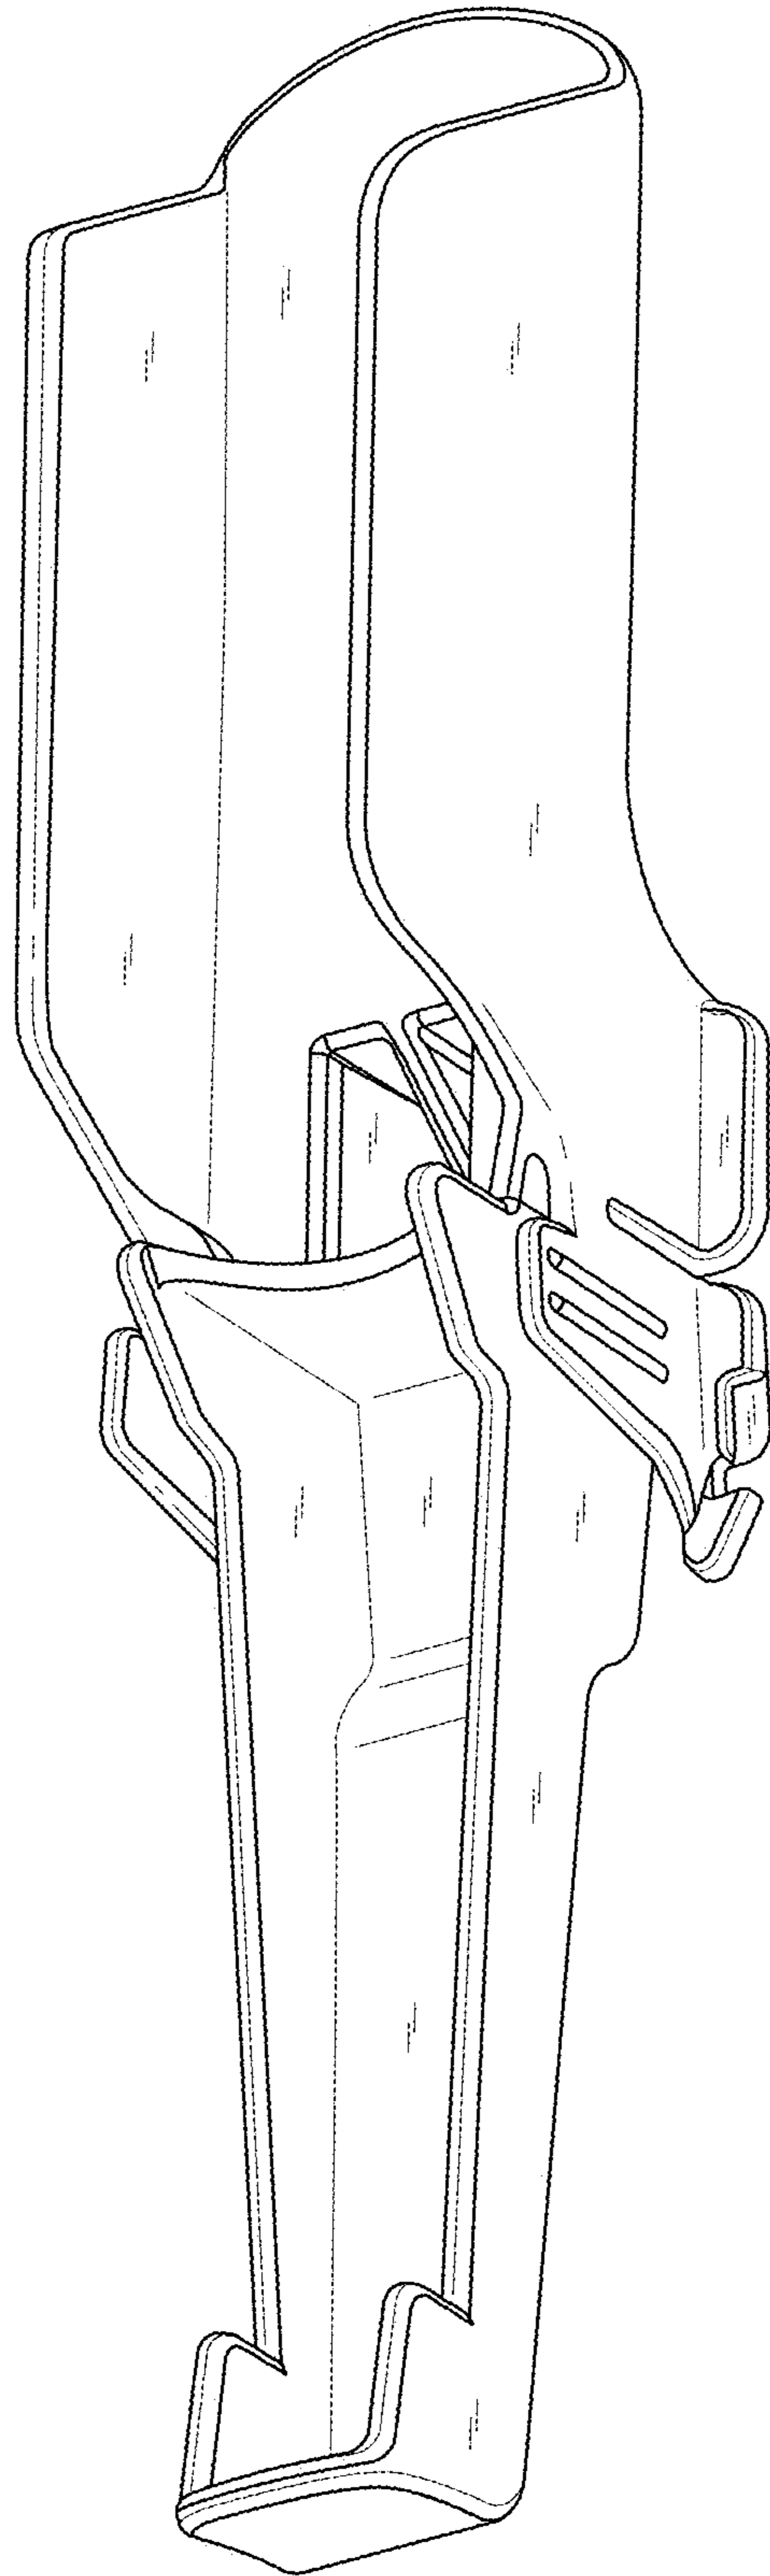


FIG. 1

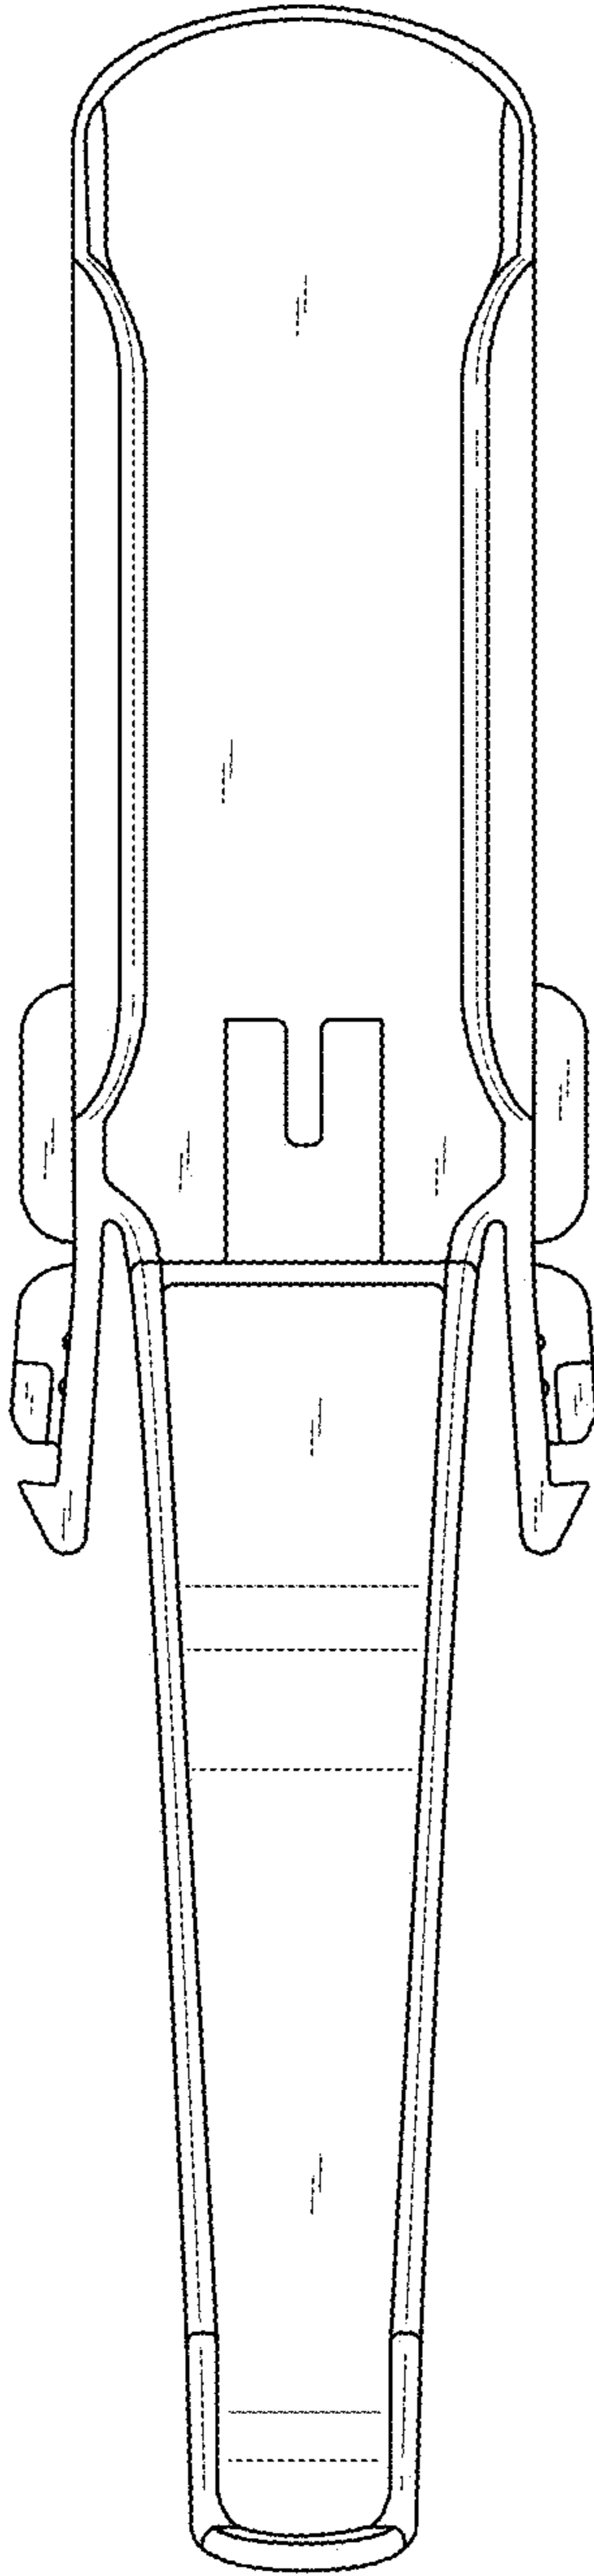


FIG. 2



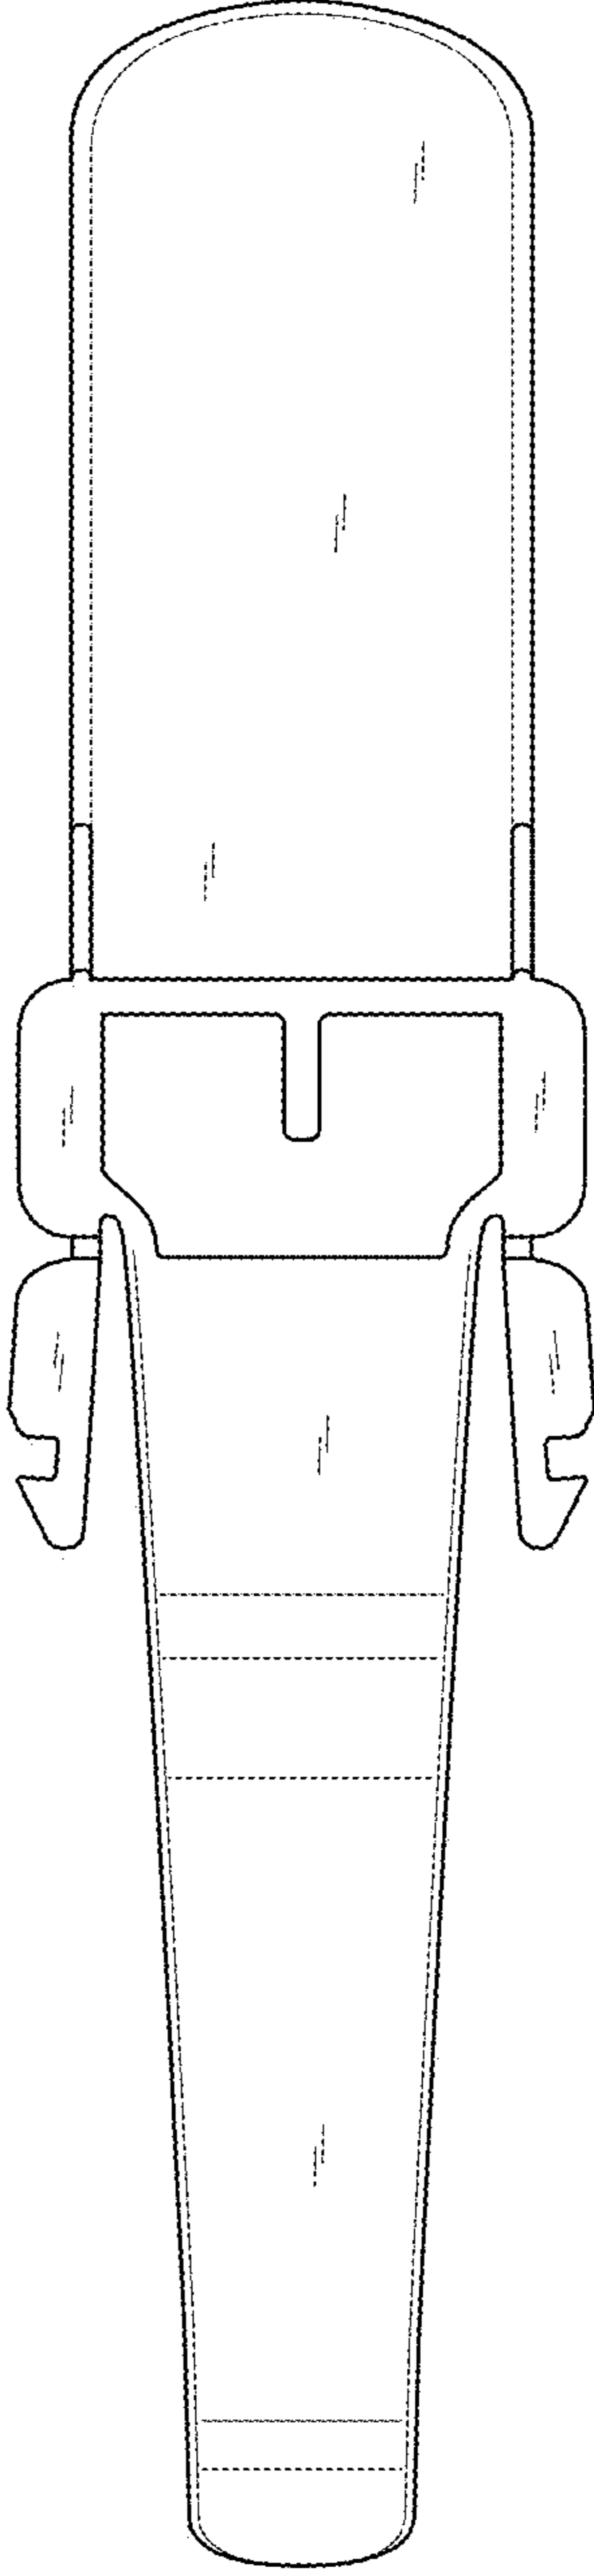



FIG. 3

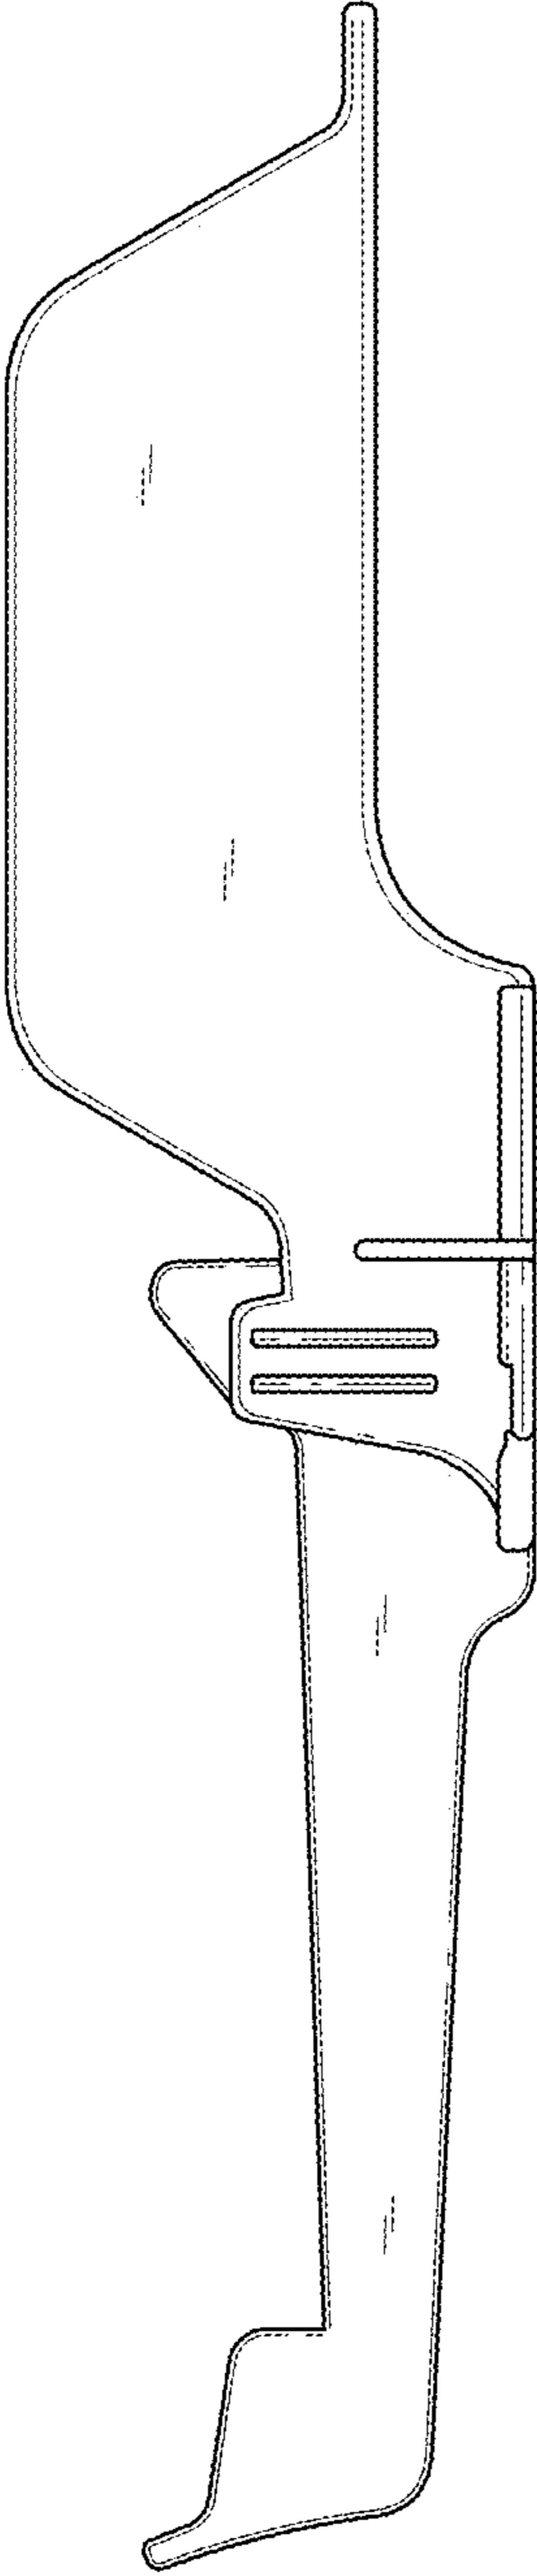

**FIG. 4**

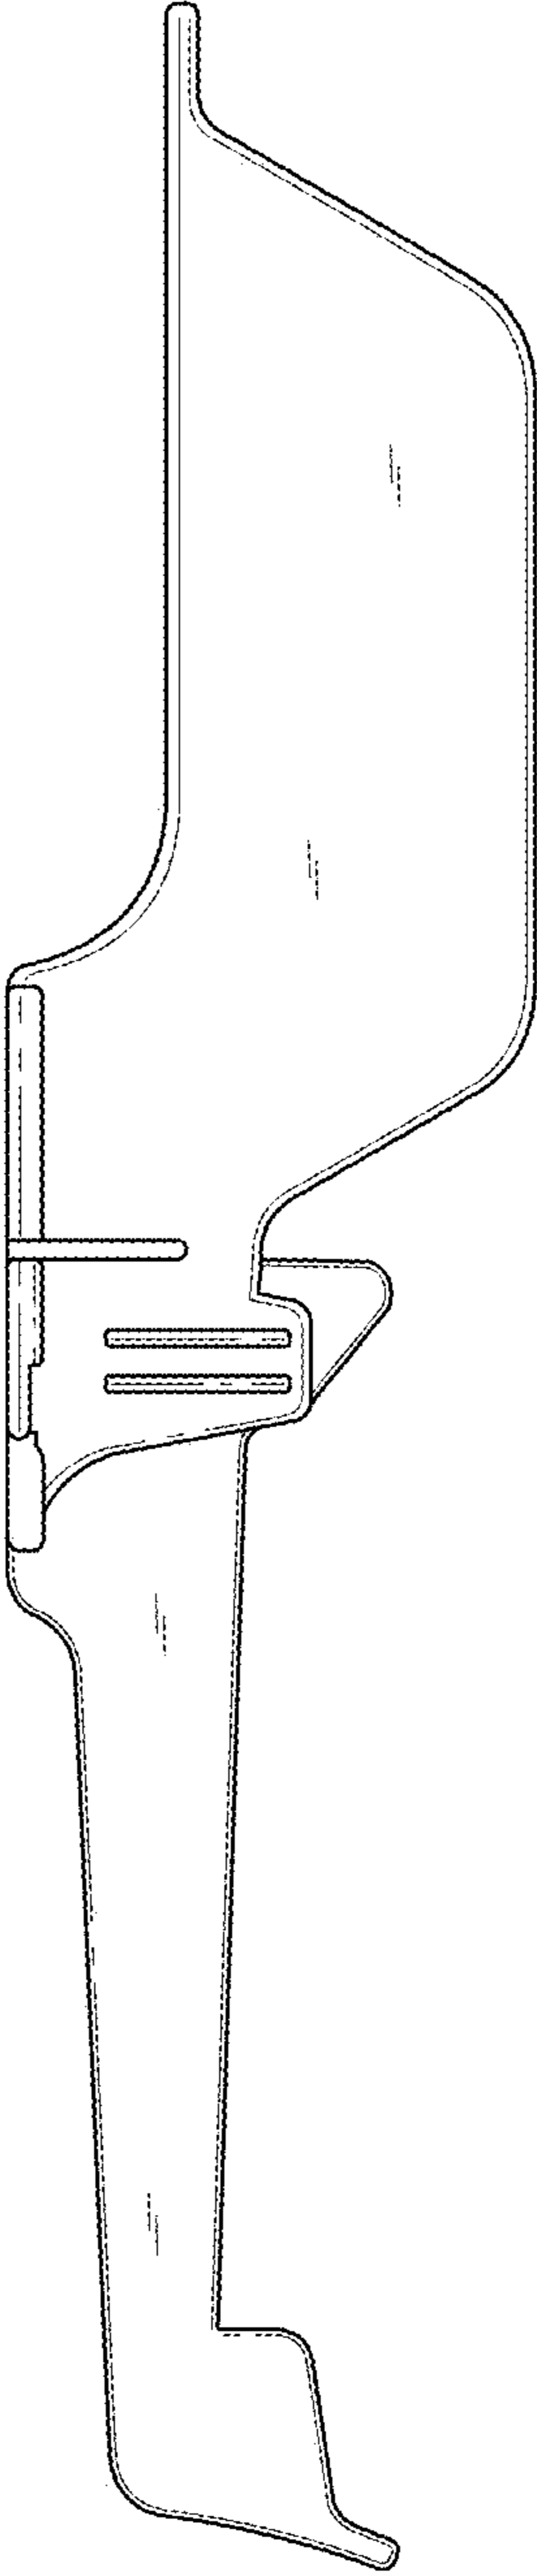

**FIG. 5**

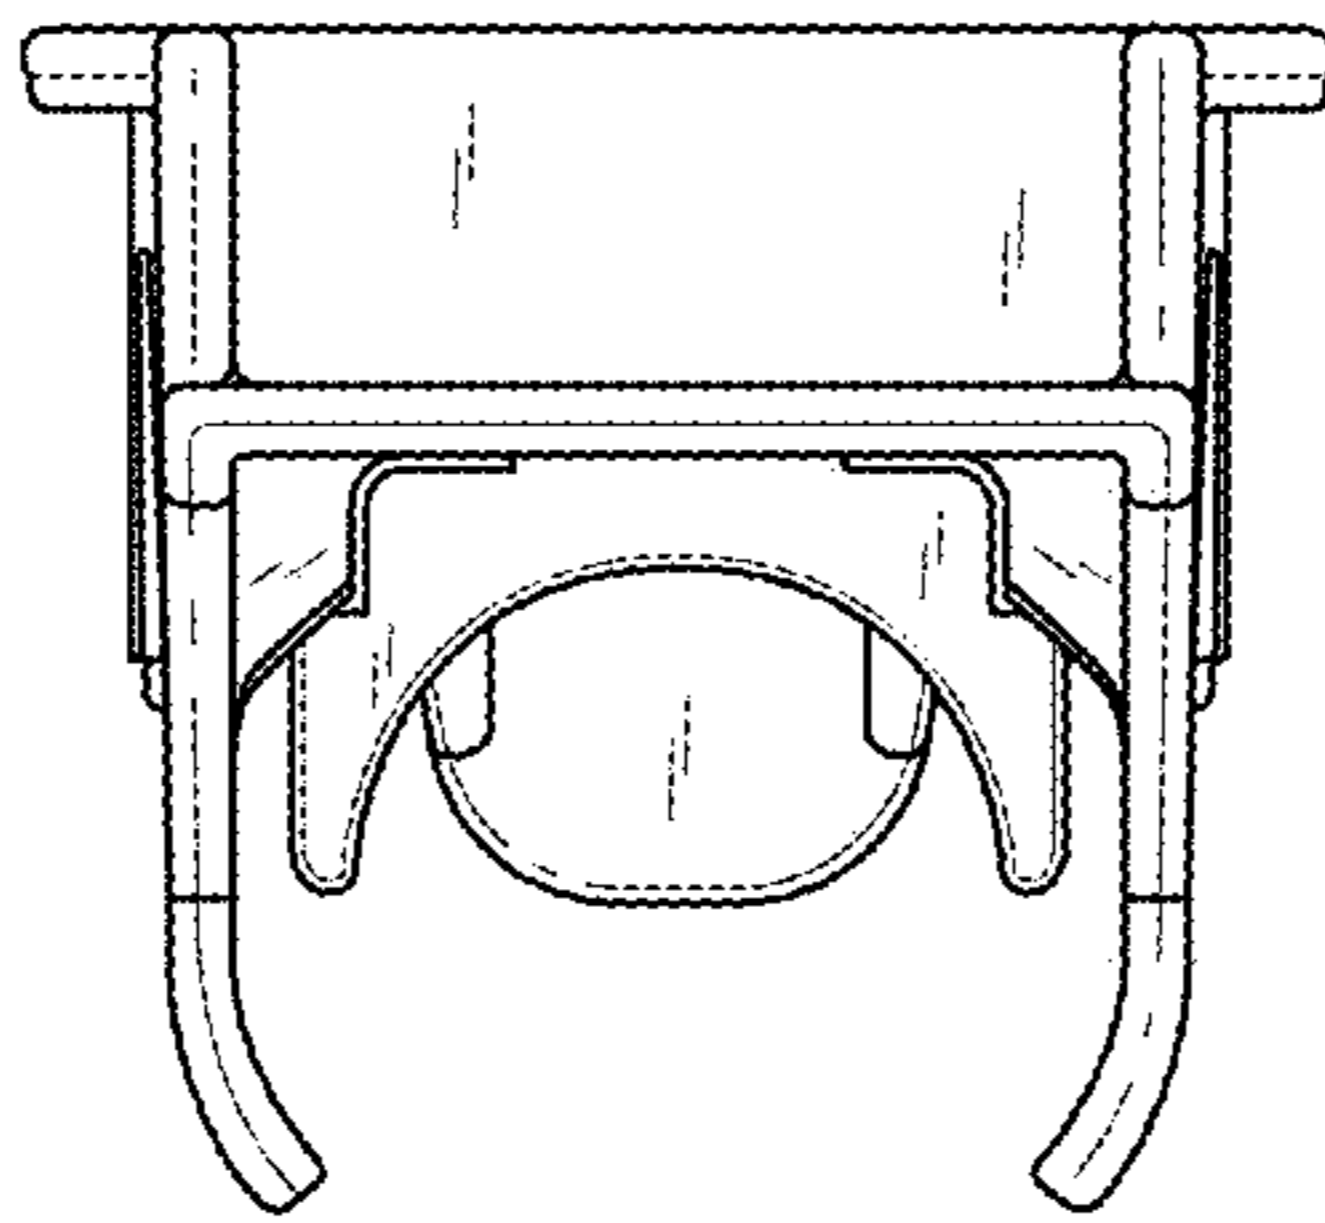

**FIG. 6**