



US00D952156S

(12) **United States Design Patent** (10) **Patent No.:** **US D952,156 S**
Hoan et al. (45) **Date of Patent:** **** May 17, 2022**

- (54) **BRACKET WITH CLIPS** 4,904,245 A 2/1990 Chen et al.
- (71) Applicant: **Edwards Lifesciences Corporation,** 5,417,395 A 5/1995 Fowler et al.
Irvine, CA (US) 5,643,218 A 7/1997 Lynn et al.
- (72) Inventors: **Andrew Nguyen Hoan,** Irvine, CA 5,961,472 A 10/1999 Swendson et al.
(US); **Mandana Farhadieh,** Tustin, CA 6,105,912 A 8/2000 Lindsay et al.
(US); **Brian Patrick Murphy,** Costa 6,156,019 A 12/2000 Langevin
Mesa, CA (US) D494,049 S * 8/2004 Ziaylek D8/373
7,240,882 B2 7/2007 Degentesh et al.
7,744,573 B2 6/2010 Gordon et al.
D618,987 S * 7/2010 Ziaylek D8/373
D620,783 S * 8/2010 Ziaylek D8/373
(Continued)
- (73) Assignee: **Edwards Lifesciences Corporation,**
Irvine, CA (US)

FOREIGN PATENT DOCUMENTS

- (**) Term: **15 Years** CN 107374648 A 11/2017
- (21) Appl. No.: **29/665,012** EP 2689797 A1 1/2014
(Continued)

(22) Filed: **Sep. 28, 2018**

OTHER PUBLICATIONS

- Related U.S. Application Data**
- (63) Continuation of application No. 15/801,009, filed on Nov. 1, 2017, now abandoned.
 - (51) **LOC (13) Cl.** **24-02**
 - (52) **U.S. Cl.**
USPC **D24/169**
 - (58) **Field of Classification Search**
USPC D8/354, 366, 371, 372, 367, 374, 373,
D8/376, 375, 16, 19, 45, 380, 381, 394,
D8/71, 365; D24/111, 169
See application file for complete search history.

BIOPAC Systems, Inc., NonInvasive Blood Pressure Amplifier, Oct. 2, 2017, Inset Figure—Clamp.
(Continued)

Primary Examiner — Eliza Z Bennett-Hattan
Assistant Examiner — Eliza Z Harvey

(57) **CLAIM**

The ornamental design for a bracket with clips, as shown and described.

(56) **References Cited**


DESCRIPTION

U.S. PATENT DOCUMENTS

- 2,954,028 A 9/1960 Smith
- 3,157,201 A 11/1964 Littman
- 3,780,972 A 12/1973 Brodersen
- 4,211,380 A 7/1980 Lillegard et al.
- 4,428,383 A 1/1984 DeVroom
- 4,858,127 A 8/1989 Kron et al.
- 4,865,583 A 9/1989 Tu

FIG. 1 is a bottom right perspective view of the design.
FIG. 2 is a front view thereof.
FIG. 3 is a back view thereof.
FIG. 4 is a right side view thereof.
FIG. 5 is a left side view thereof; and,
FIG. 6 is a top plan view thereof.

1 Claim, 4 Drawing Sheets

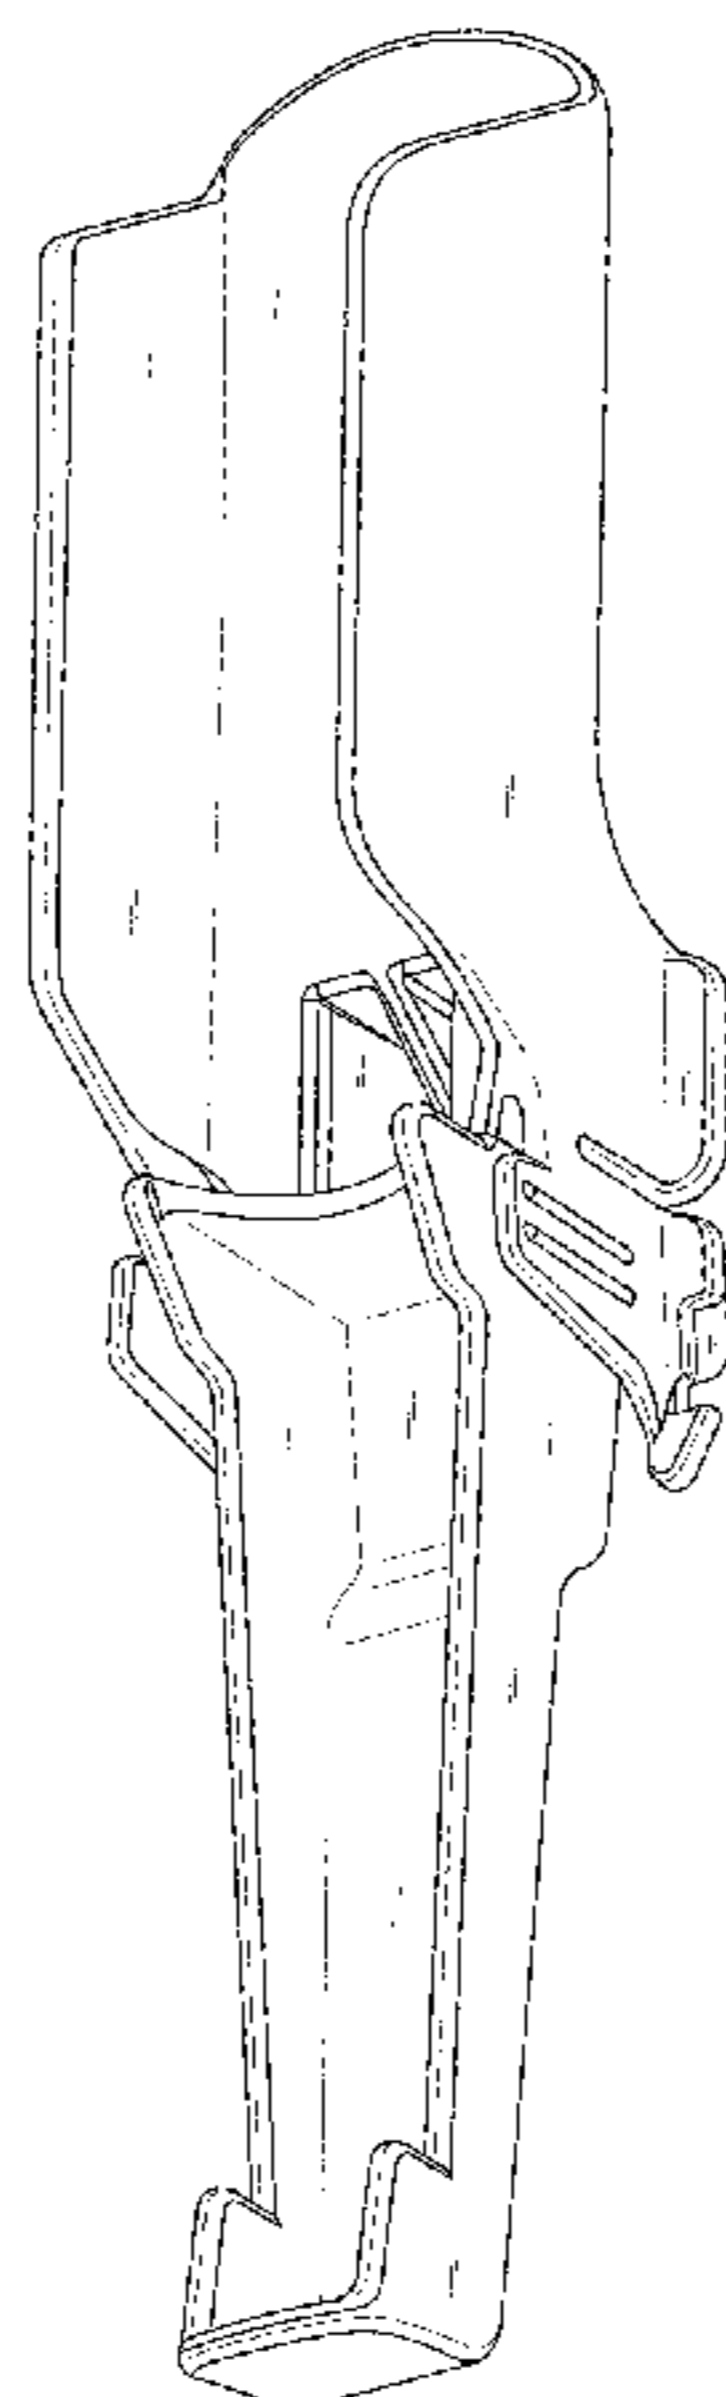

(56)

References Cited

U.S. PATENT DOCUMENTS

7,918,422 B2 4/2011 Blankenship et al.
 7,963,951 B2 6/2011 Kitani et al.
 D661,979 S * 6/2012 Schwenkenberg D8/373
 8,348,844 B2 1/2013 Kunjan et al.
 8,382,696 B2 2/2013 Beiriger et al.
 8,403,874 B2 3/2013 Baraldi
 8,662,458 B2 3/2014 Henault et al.
 8,668,178 B2 3/2014 Ziaylek et al.
 D707,543 S * 6/2014 Schwenkenberg D8/373
 8,764,668 B2 7/2014 Roteliuk et al.
 D715,135 S * 10/2014 Vecchiarelli D8/373
 8,945,051 B2 2/2015 Schriver et al.
 8,986,262 B2 3/2015 Young et al.
 9,016,316 B2 4/2015 Ziv et al.
 9,022,981 B2 5/2015 Oesterreich et al.
 9,259,527 B2 2/2016 Spohn et al.
 D754,001 S * 4/2016 Barrier D9/455
 9,370,324 B2 6/2016 Barrett et al.
 9,375,561 B2 6/2016 Mansour et al.
 D773,292 S * 12/2016 Ziaylek D8/373
 D777,562 S * 1/2017 Ziaylek D8/373
 9,566,385 B2 2/2017 Franks

2004/0210162 A1 10/2004 Wyatt et al.
 2007/0119508 A1 5/2007 West et al.
 2008/0200837 A1 8/2008 Frazier et al.
 2008/0302932 A1 12/2008 Mosler et al.
 2013/0060205 A1 3/2013 Mansour et al.
 2014/0276215 A1 9/2014 Nelson et al.
 2015/0196749 A1 7/2015 Ziv et al.
 2016/0144110 A1 5/2016 Ueda
 2016/0346472 A1 12/2016 Mitchell et al.

FOREIGN PATENT DOCUMENTS

FR 2914840 A1 10/2008
 WO 8500982 A1 3/1985
 WO 2013146752 A1 10/2013
 WO 2016041948 A1 3/2016
 WO 2017051536 A1 3/2017

OTHER PUBLICATIONS

Mark Siobal, Analysis and Monitoring of Gas Exchange, <https://clinicalgate.com/analysis-and-monitoring-of-gas-exchange/>, Jan. 6, 2015.

* cited by examiner

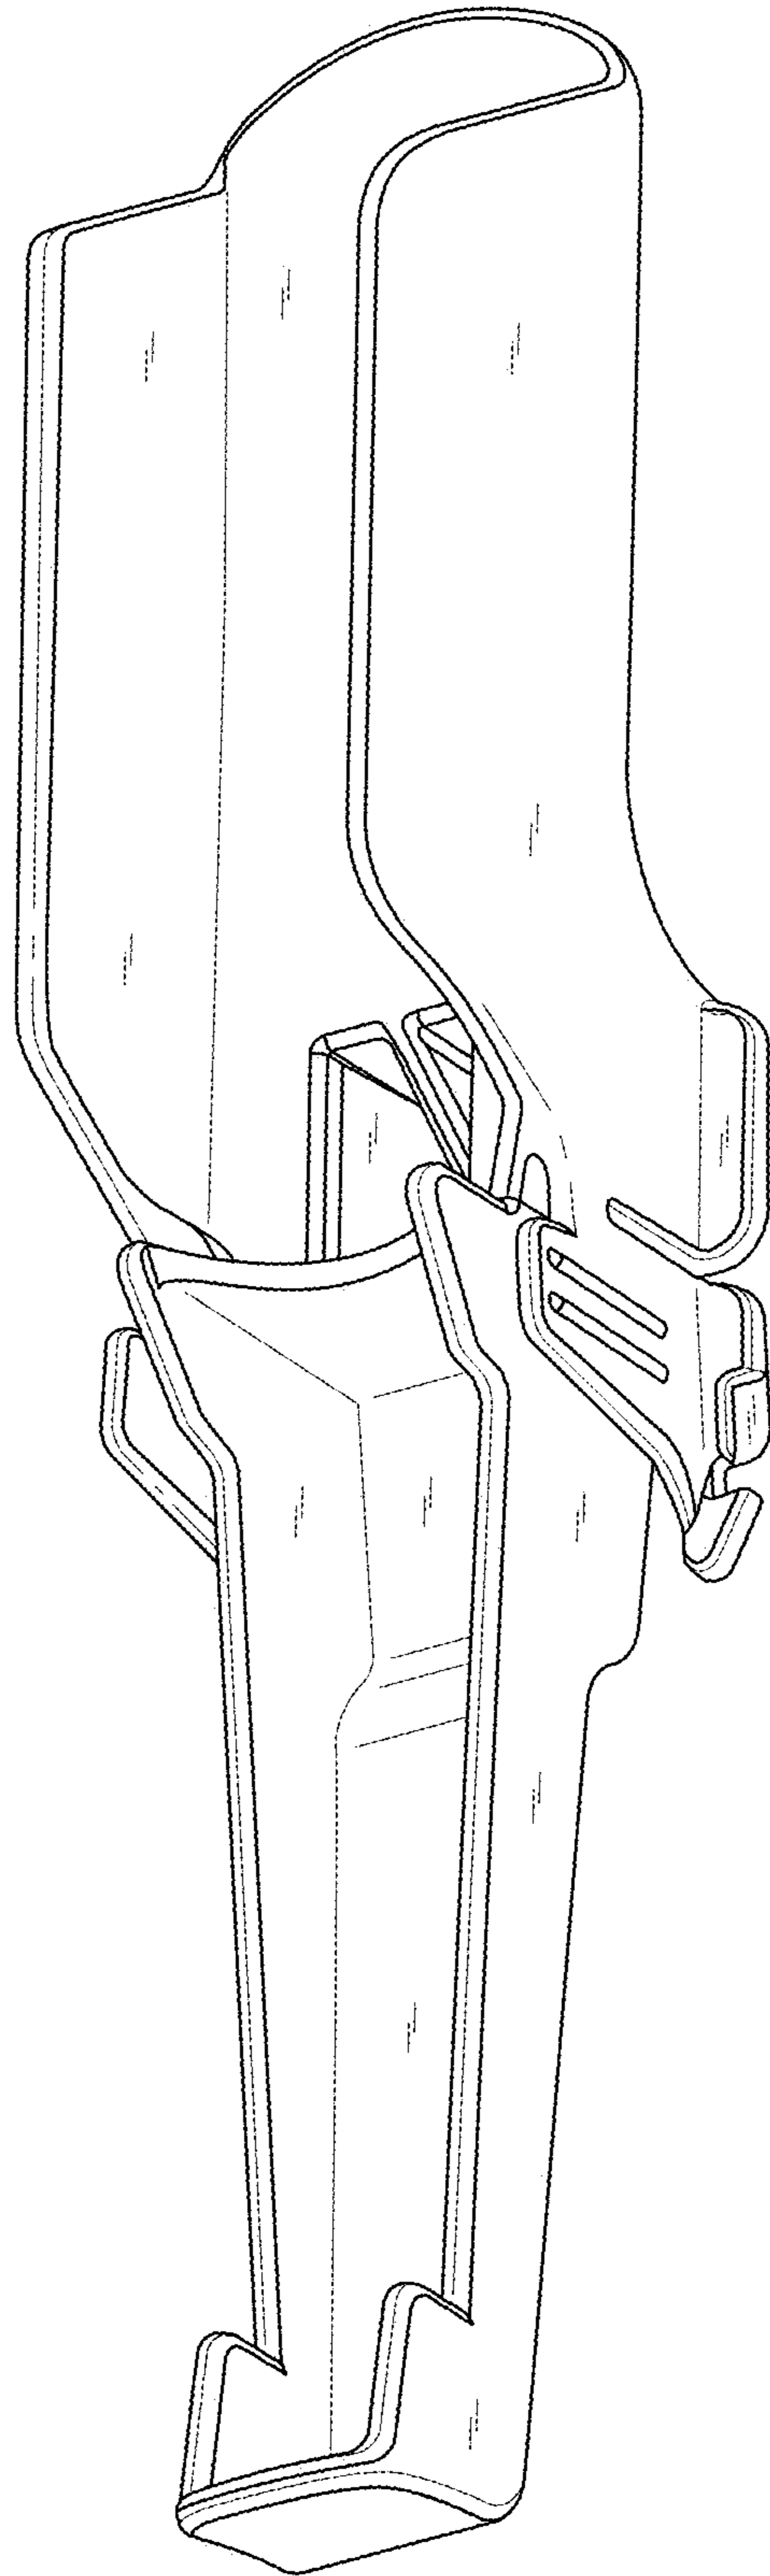


FIG. 1

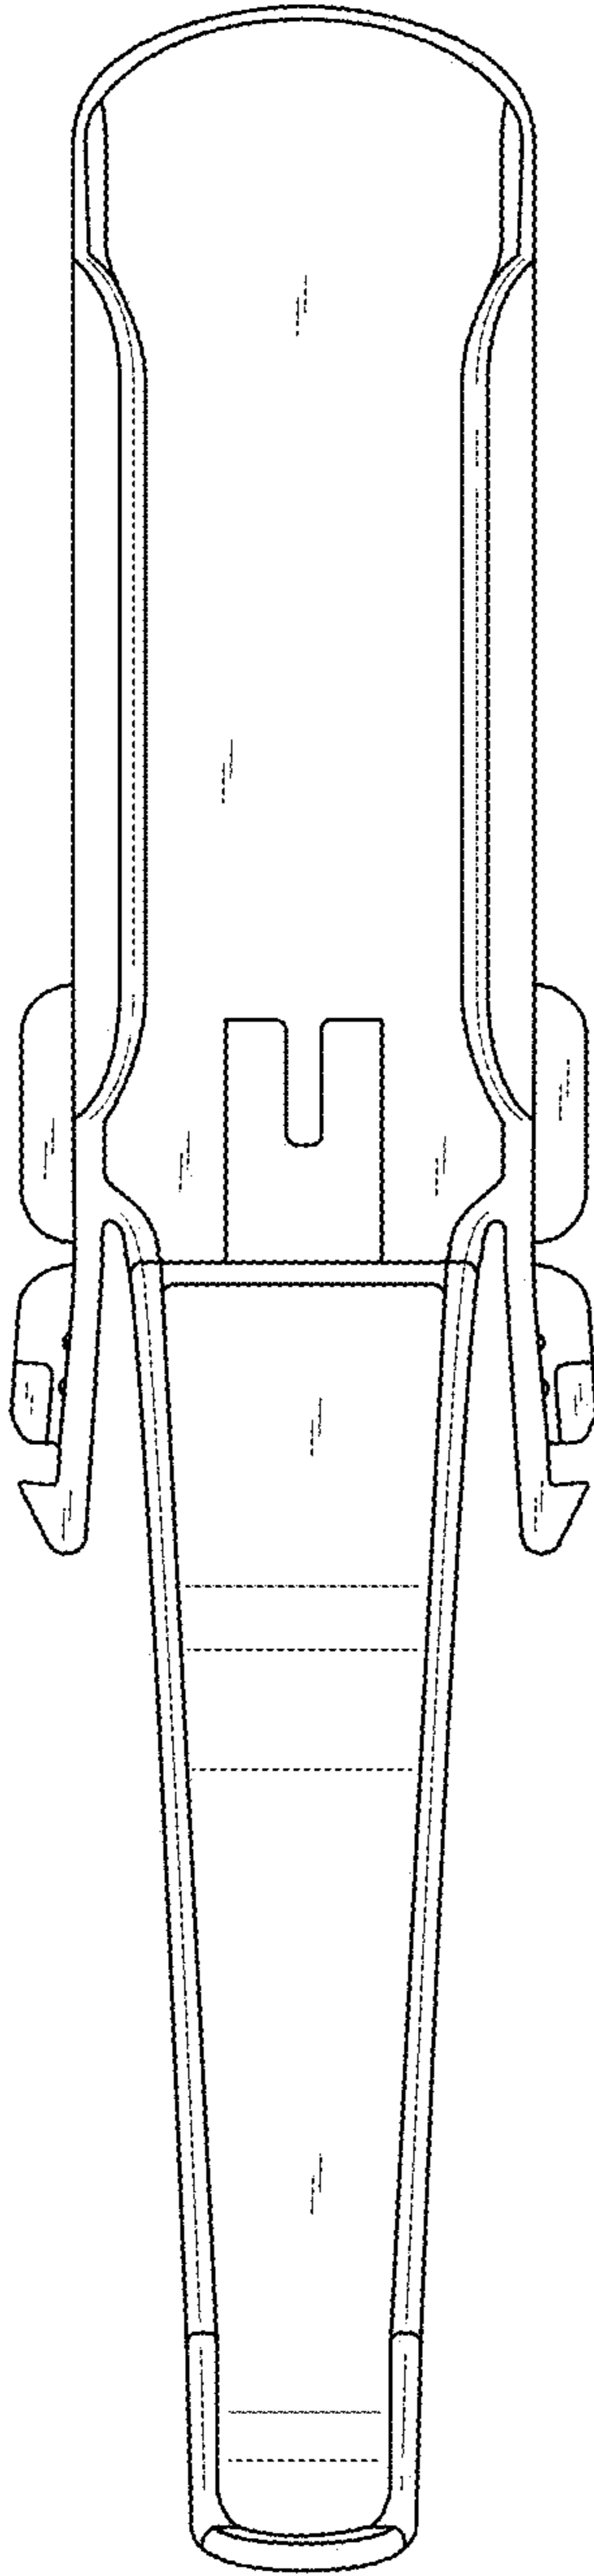


FIG. 2

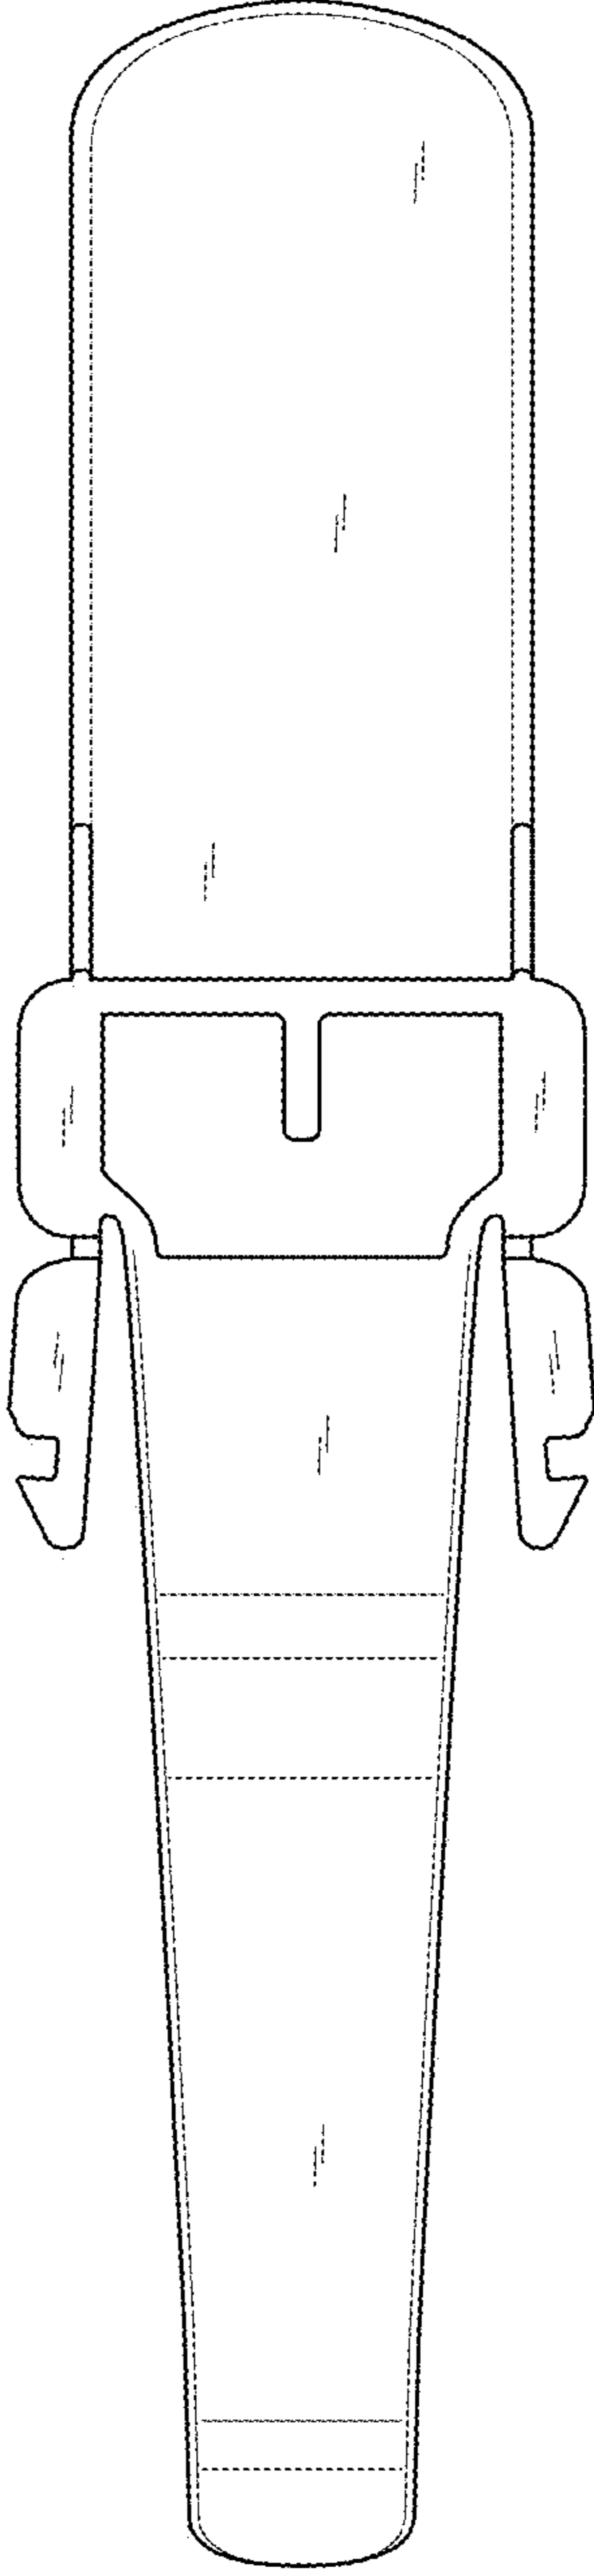


FIG. 3

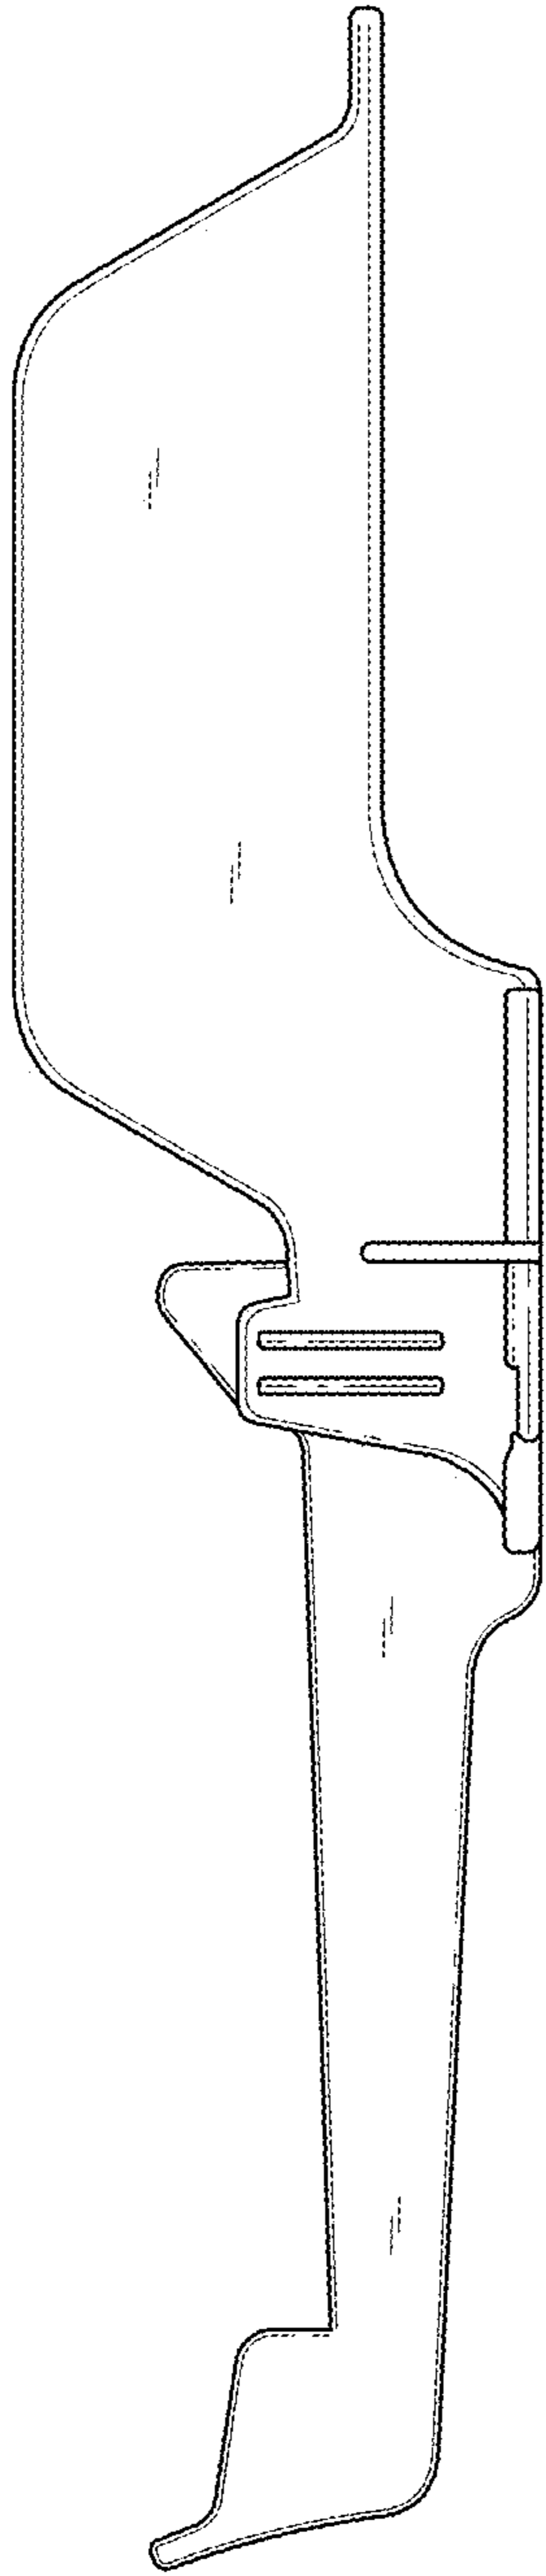


FIG. 4

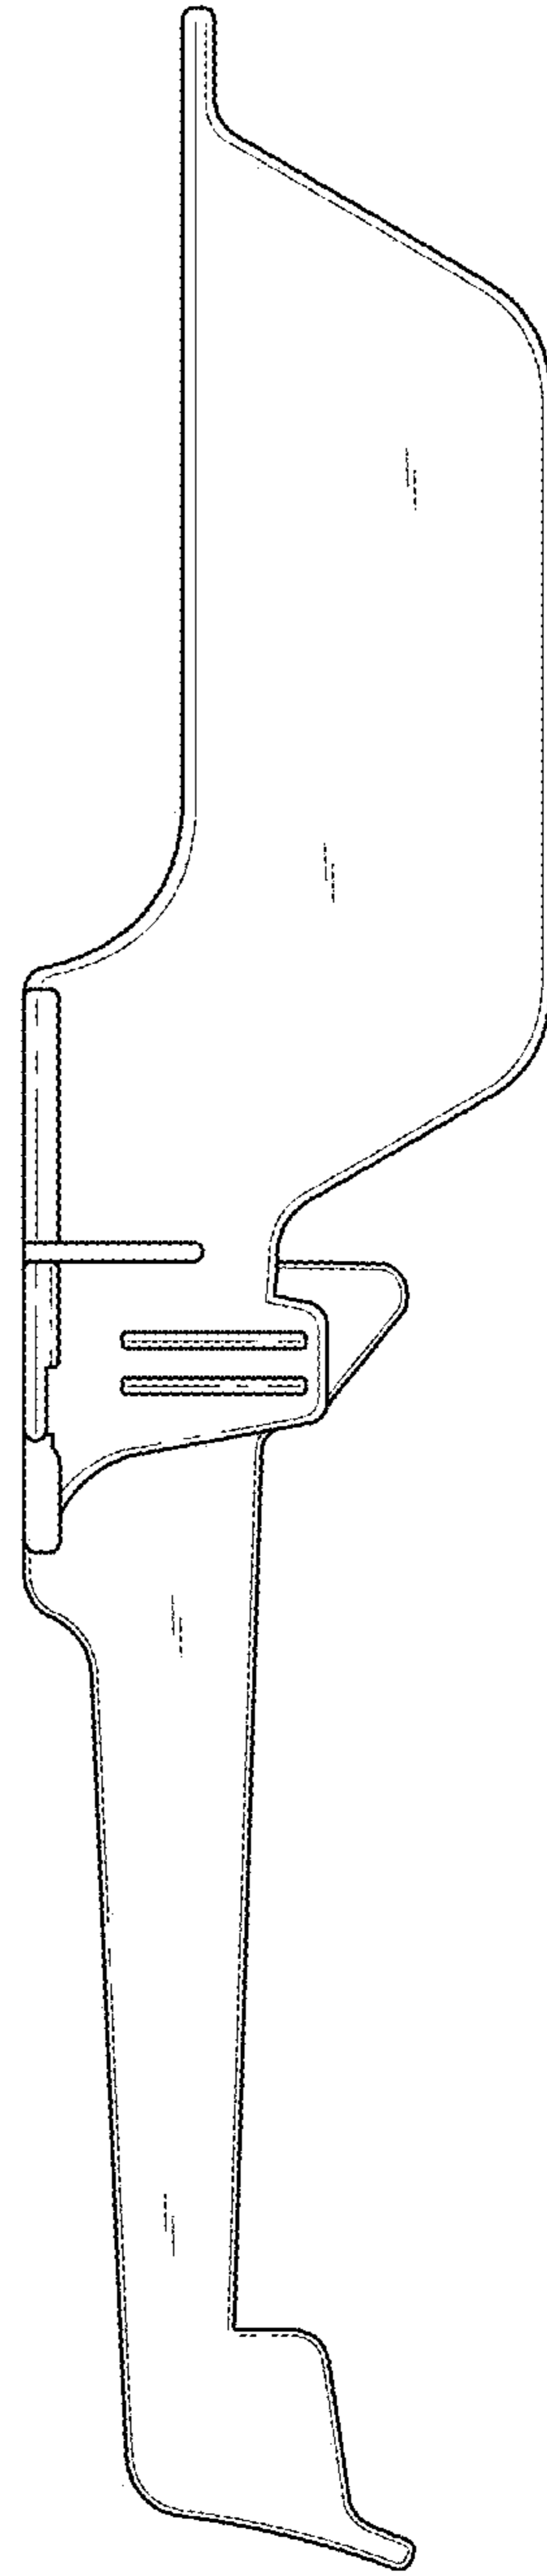


FIG. 5

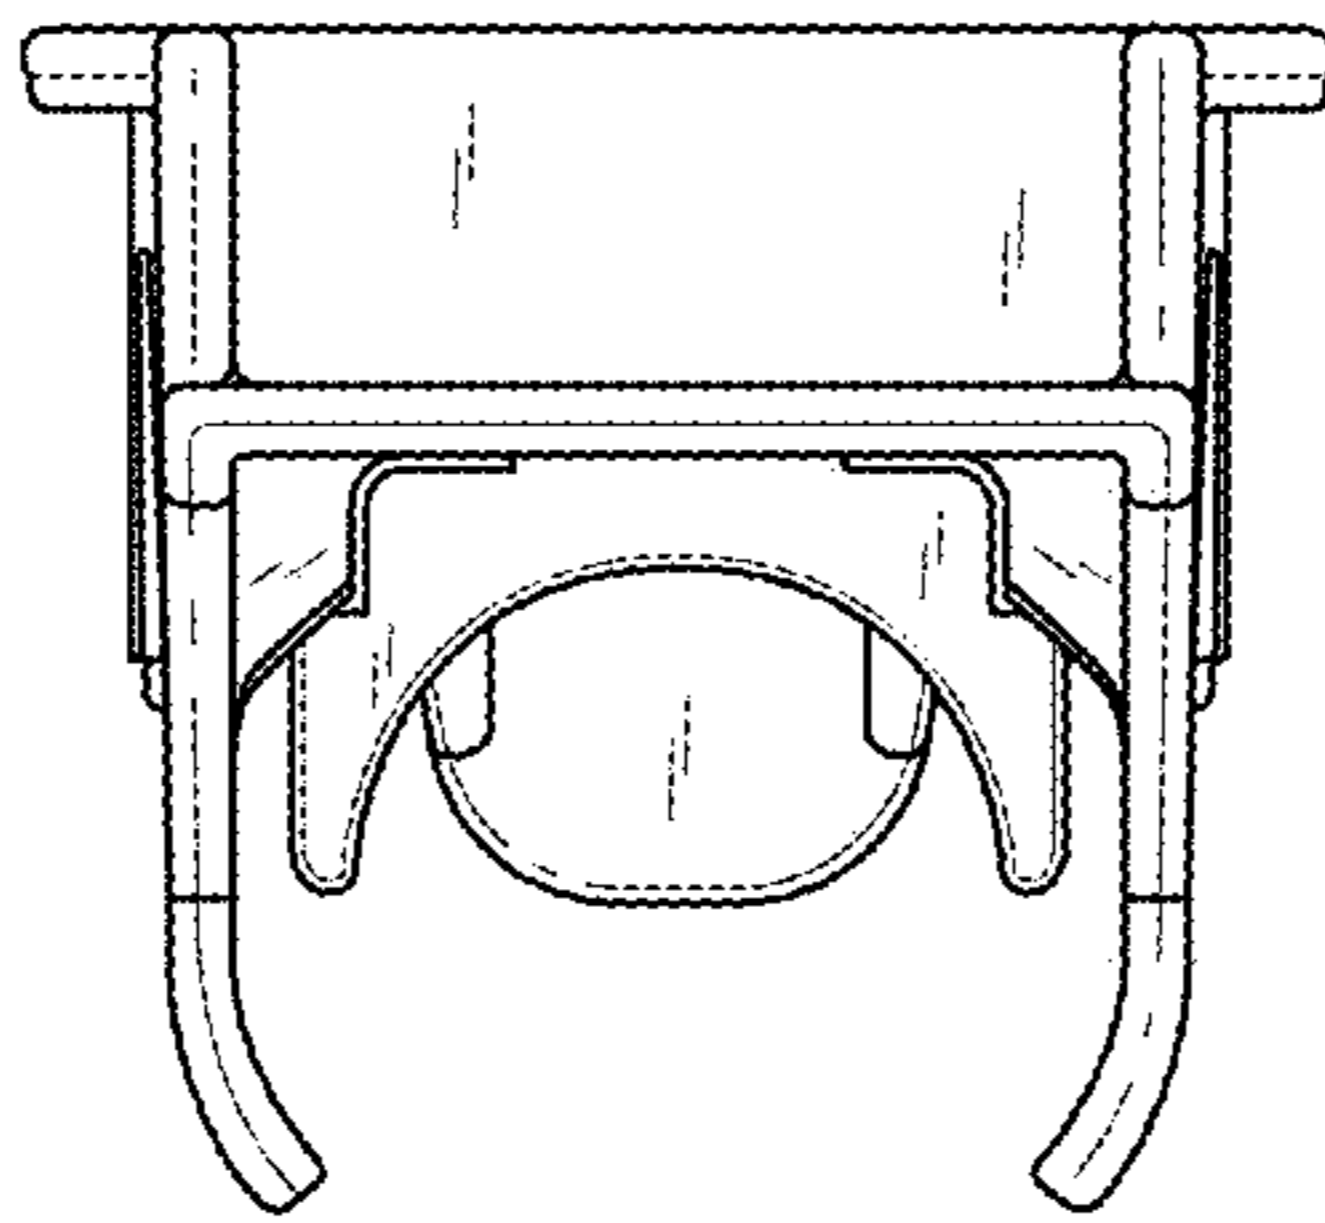


FIG. 6