



US00D952897S

(12) **United States Design Patent** (10) **Patent No.:** **US D952,897 S**
Decaluwé et al. (45) **Date of Patent:** **** May 24, 2022**

(54) **COLLECTION TUBE FOR LABORATORY ANALYSIS**

(71) Applicant: **Allflex Europe SAS**, Vitre (FR)

(72) Inventors: **Johan Decaluwé**, Laval (FR); **Bruno Teychene**, Mouzieys-Teulet (FR)

(73) Assignee: **ALLFLEX EUROPE SAS**, Vitre (FR)

(**) Term: **15 Years**

(21) Appl. No.: **29/741,830**

(22) Filed: **Jul. 16, 2020**

(30) **Foreign Application Priority Data**

May 28, 2020 (EM) 007974191-0001

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/224**

(58) **Field of Classification Search**
USPC D24/107, 121–123, 216–217, 219, D24/223–227, 229–231, 232; D9/504, D9/516, 519, 529, 549, 574, 715, 719; D3/201, 203.1, 203.2
CPC ... B29C 65/665; A61B 10/0045; A61B 5/154; A61J 1/1468; B01L 3/50825; B65D 41/04
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 4,020,975 A * 5/1977 Stauffer A47K 5/1211
222/93
- D308,475 S * 6/1990 Gastwirt D9/529
- D337,271 S * 7/1993 Pezzoli D9/453
- D457,452 S * 5/2002 Christiansen D10/96
- D500,773 S * 1/2005 Colson D15/144
- D605,765 S * 12/2009 Gaab D24/146
- D640,796 S * 6/2011 Wilkinson D24/224
- D672,463 S * 12/2012 Saad D24/138
- D802,121 S * 11/2017 Hamilton D24/122

- D868,254 S * 11/2019 Lintula D24/155
- D881,410 S * 4/2020 Motadel D24/224
- D931,730 S * 9/2021 Suid D9/504
- 2014/0249449 A1 9/2014 Hilpert et al.
- 2016/0007567 A1* 1/2016 Decaluwe A01K 11/003
600/564
- 2020/0071148 A1* 3/2020 Lin B67B 3/2066

FOREIGN PATENT DOCUMENTS

- JP D2004-33877 * 9/2005
- WO WO 2010/070130 6/2010
- WO WO 2017/153865 9/2017

OTHER PUBLICATIONS

Tissue Sampling. Online, published date unknown. Retrieved on Sep. 30, 2021 from URL: <https://www.allflex.global/product/tissue-sampling/>.*

* cited by examiner

Primary Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Hahn Loeser & Parks LLP


(57) **CLAIM**

The ornamental design for a collection tube for laboratory analysis, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a collection tube for laboratory analysis showing the new design;
FIG. 2 is a rear view thereof;
FIG. 3 is a right side view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a bottom view thereof;
FIG. 6 is a top view thereof; and,
FIG. 7 is a perspective view thereof.
The broken lines in the drawings depict portions of the collection tube for laboratory analysis that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

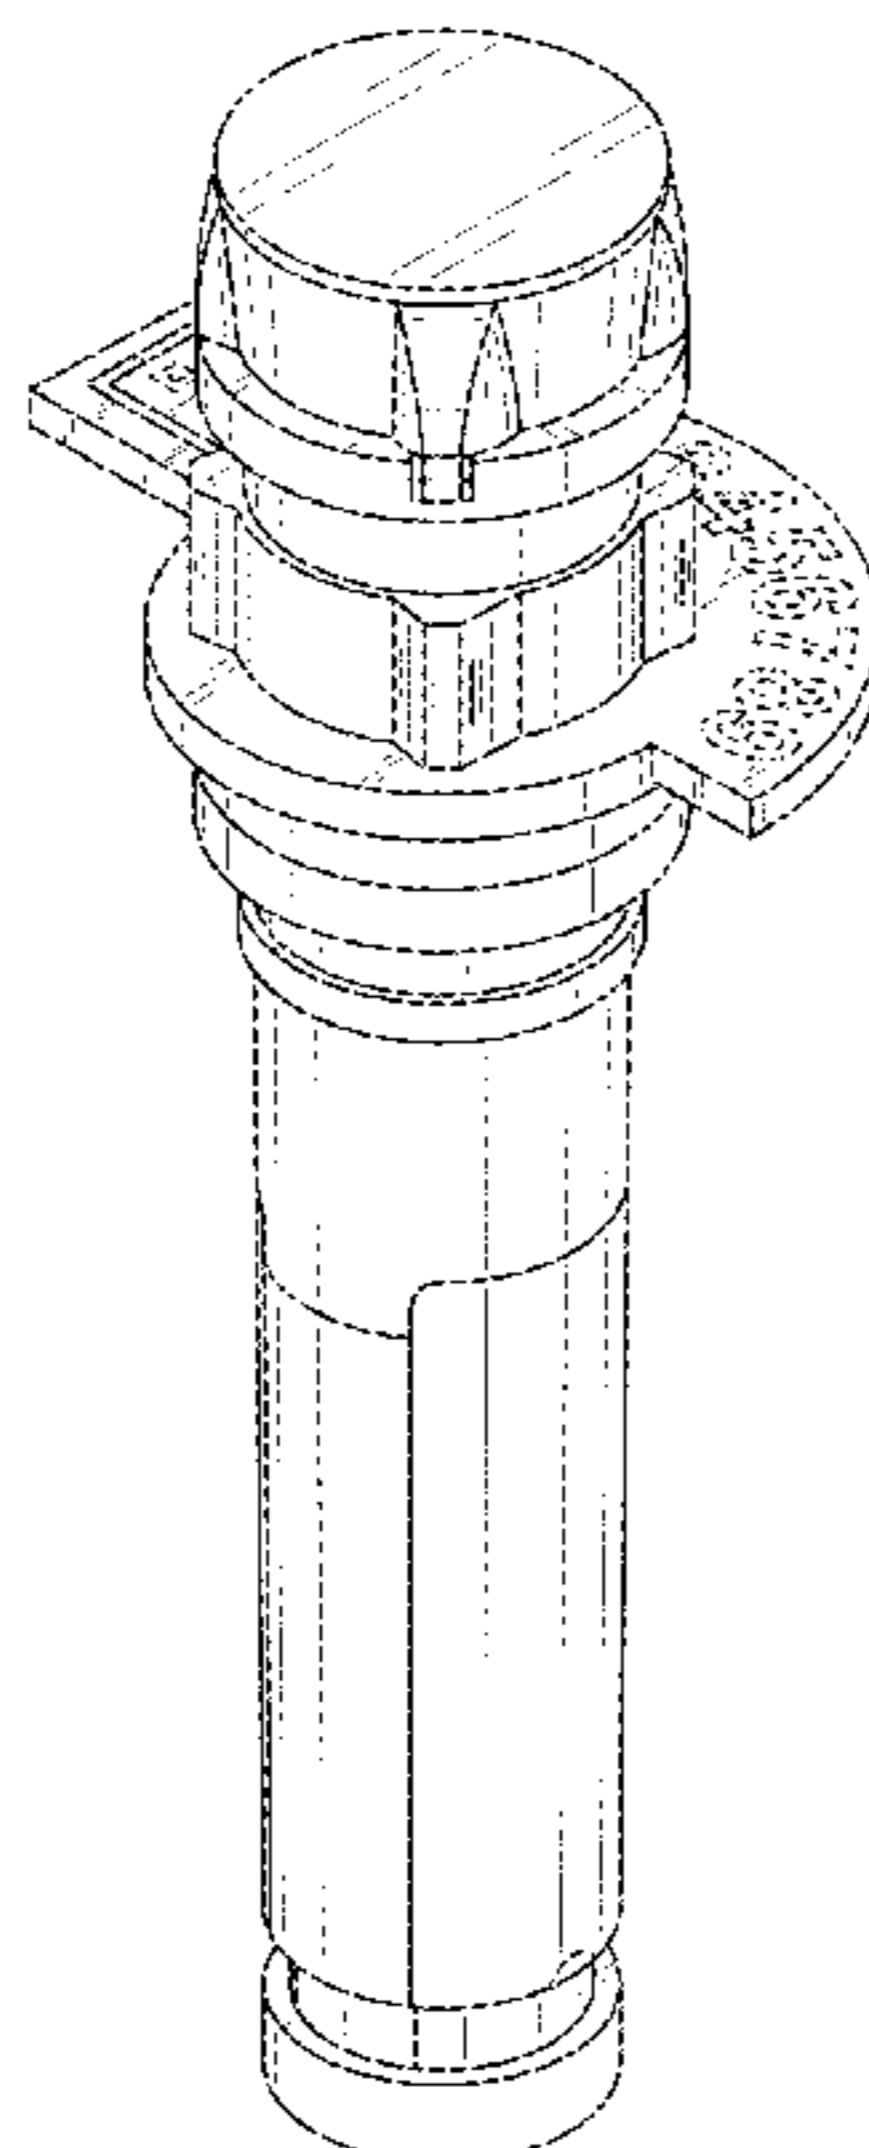

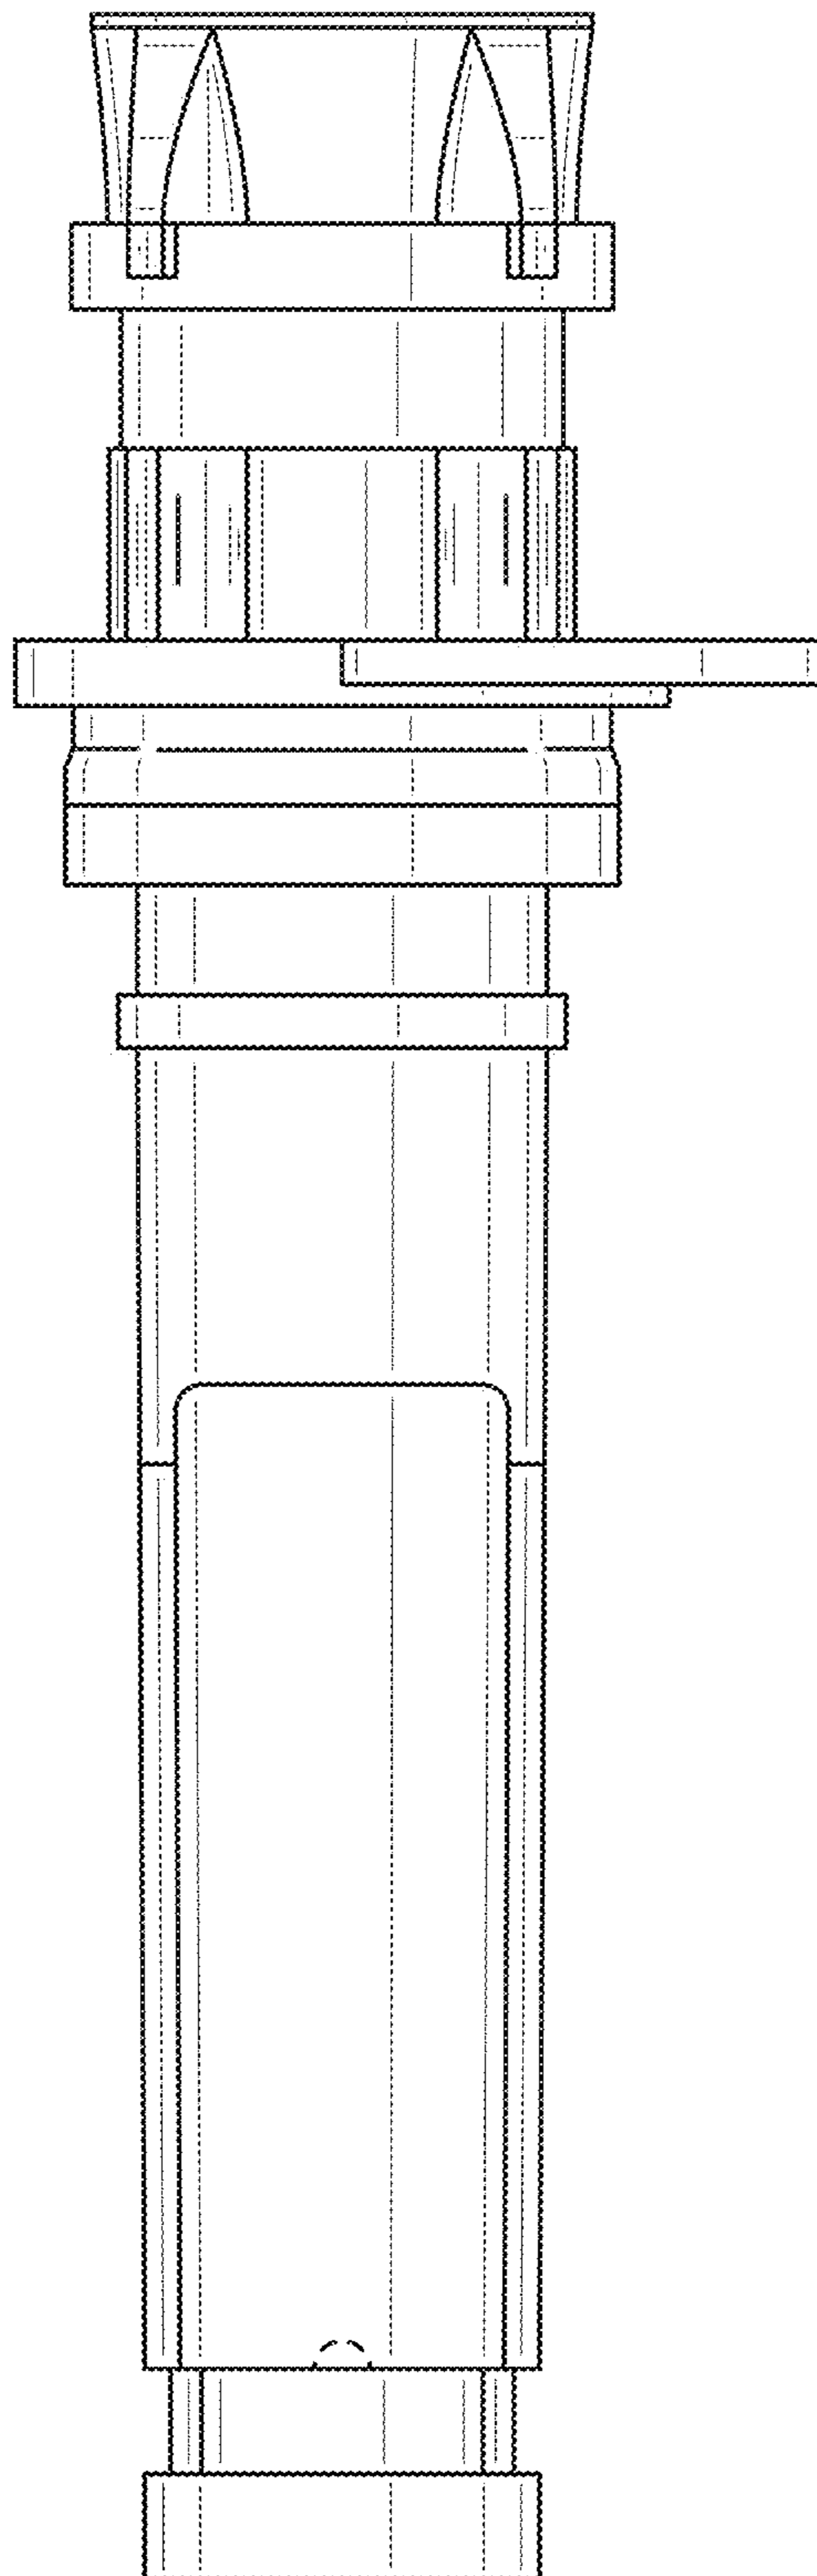


FIG. 1

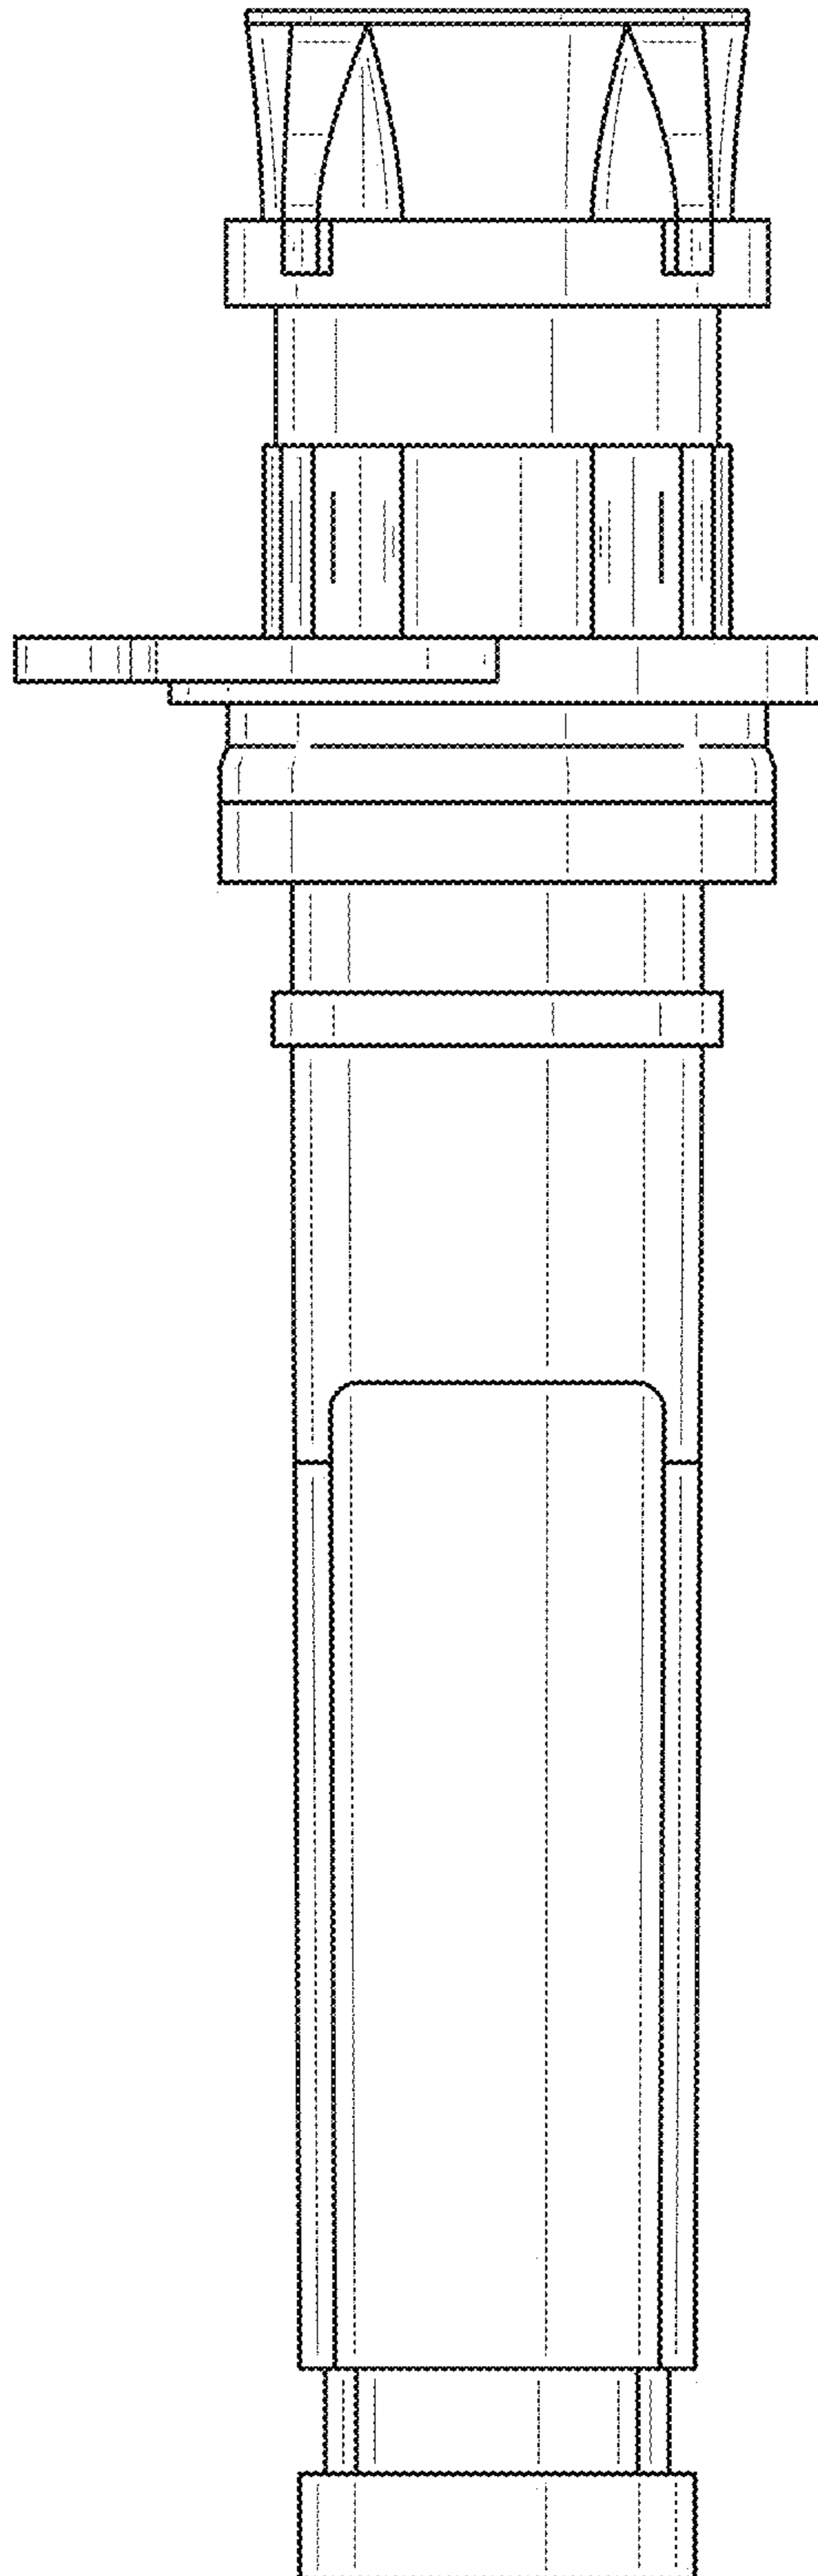


FIG. 2

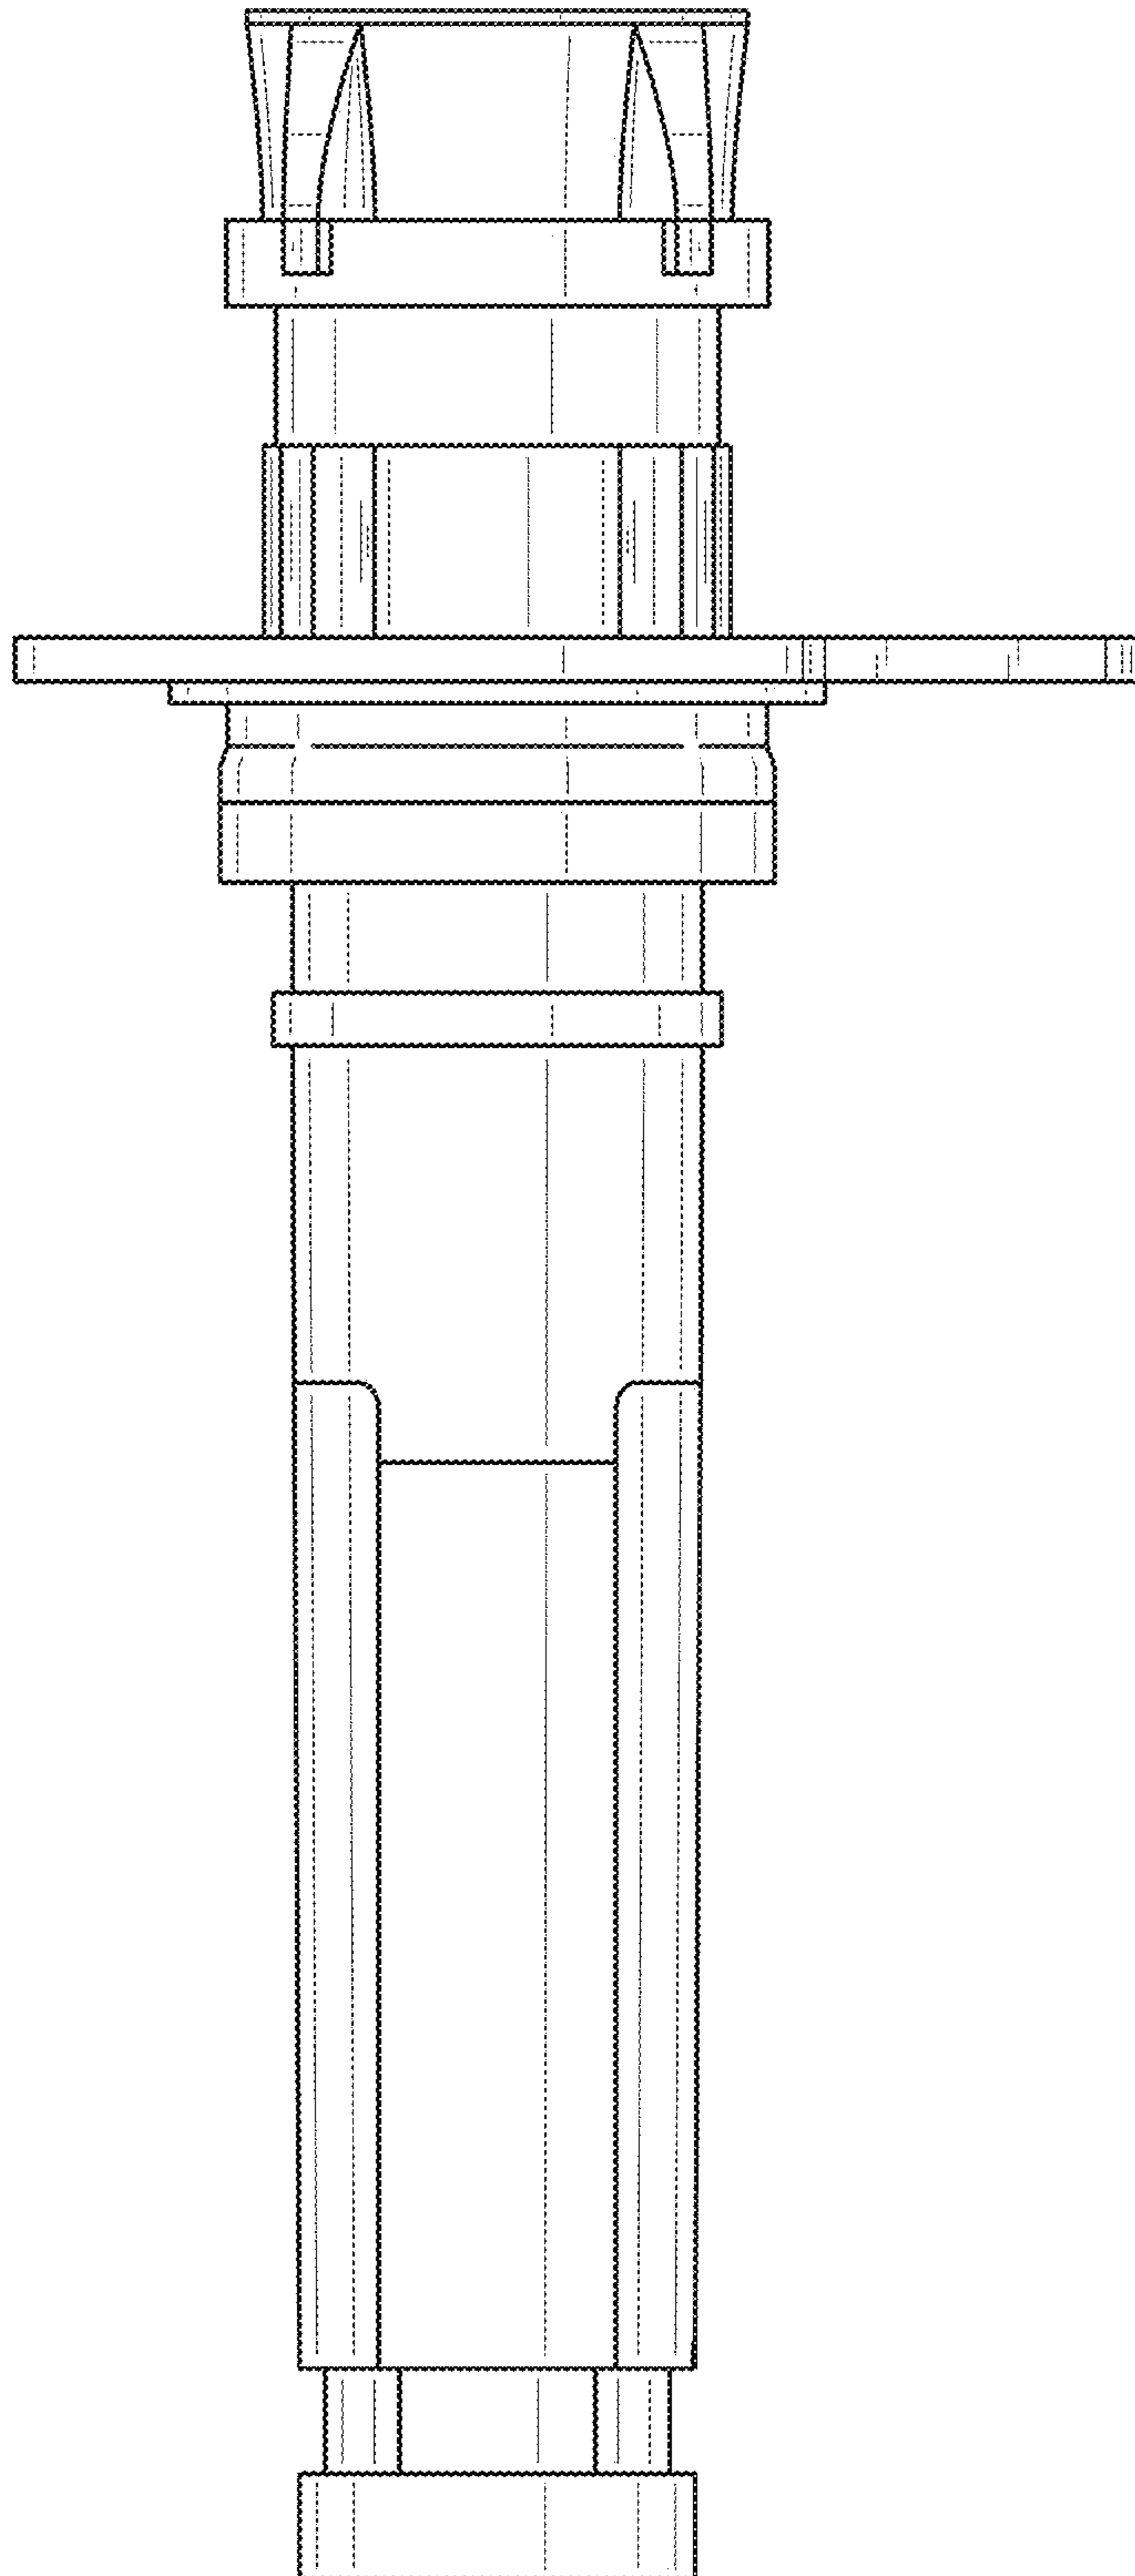


FIG. 3

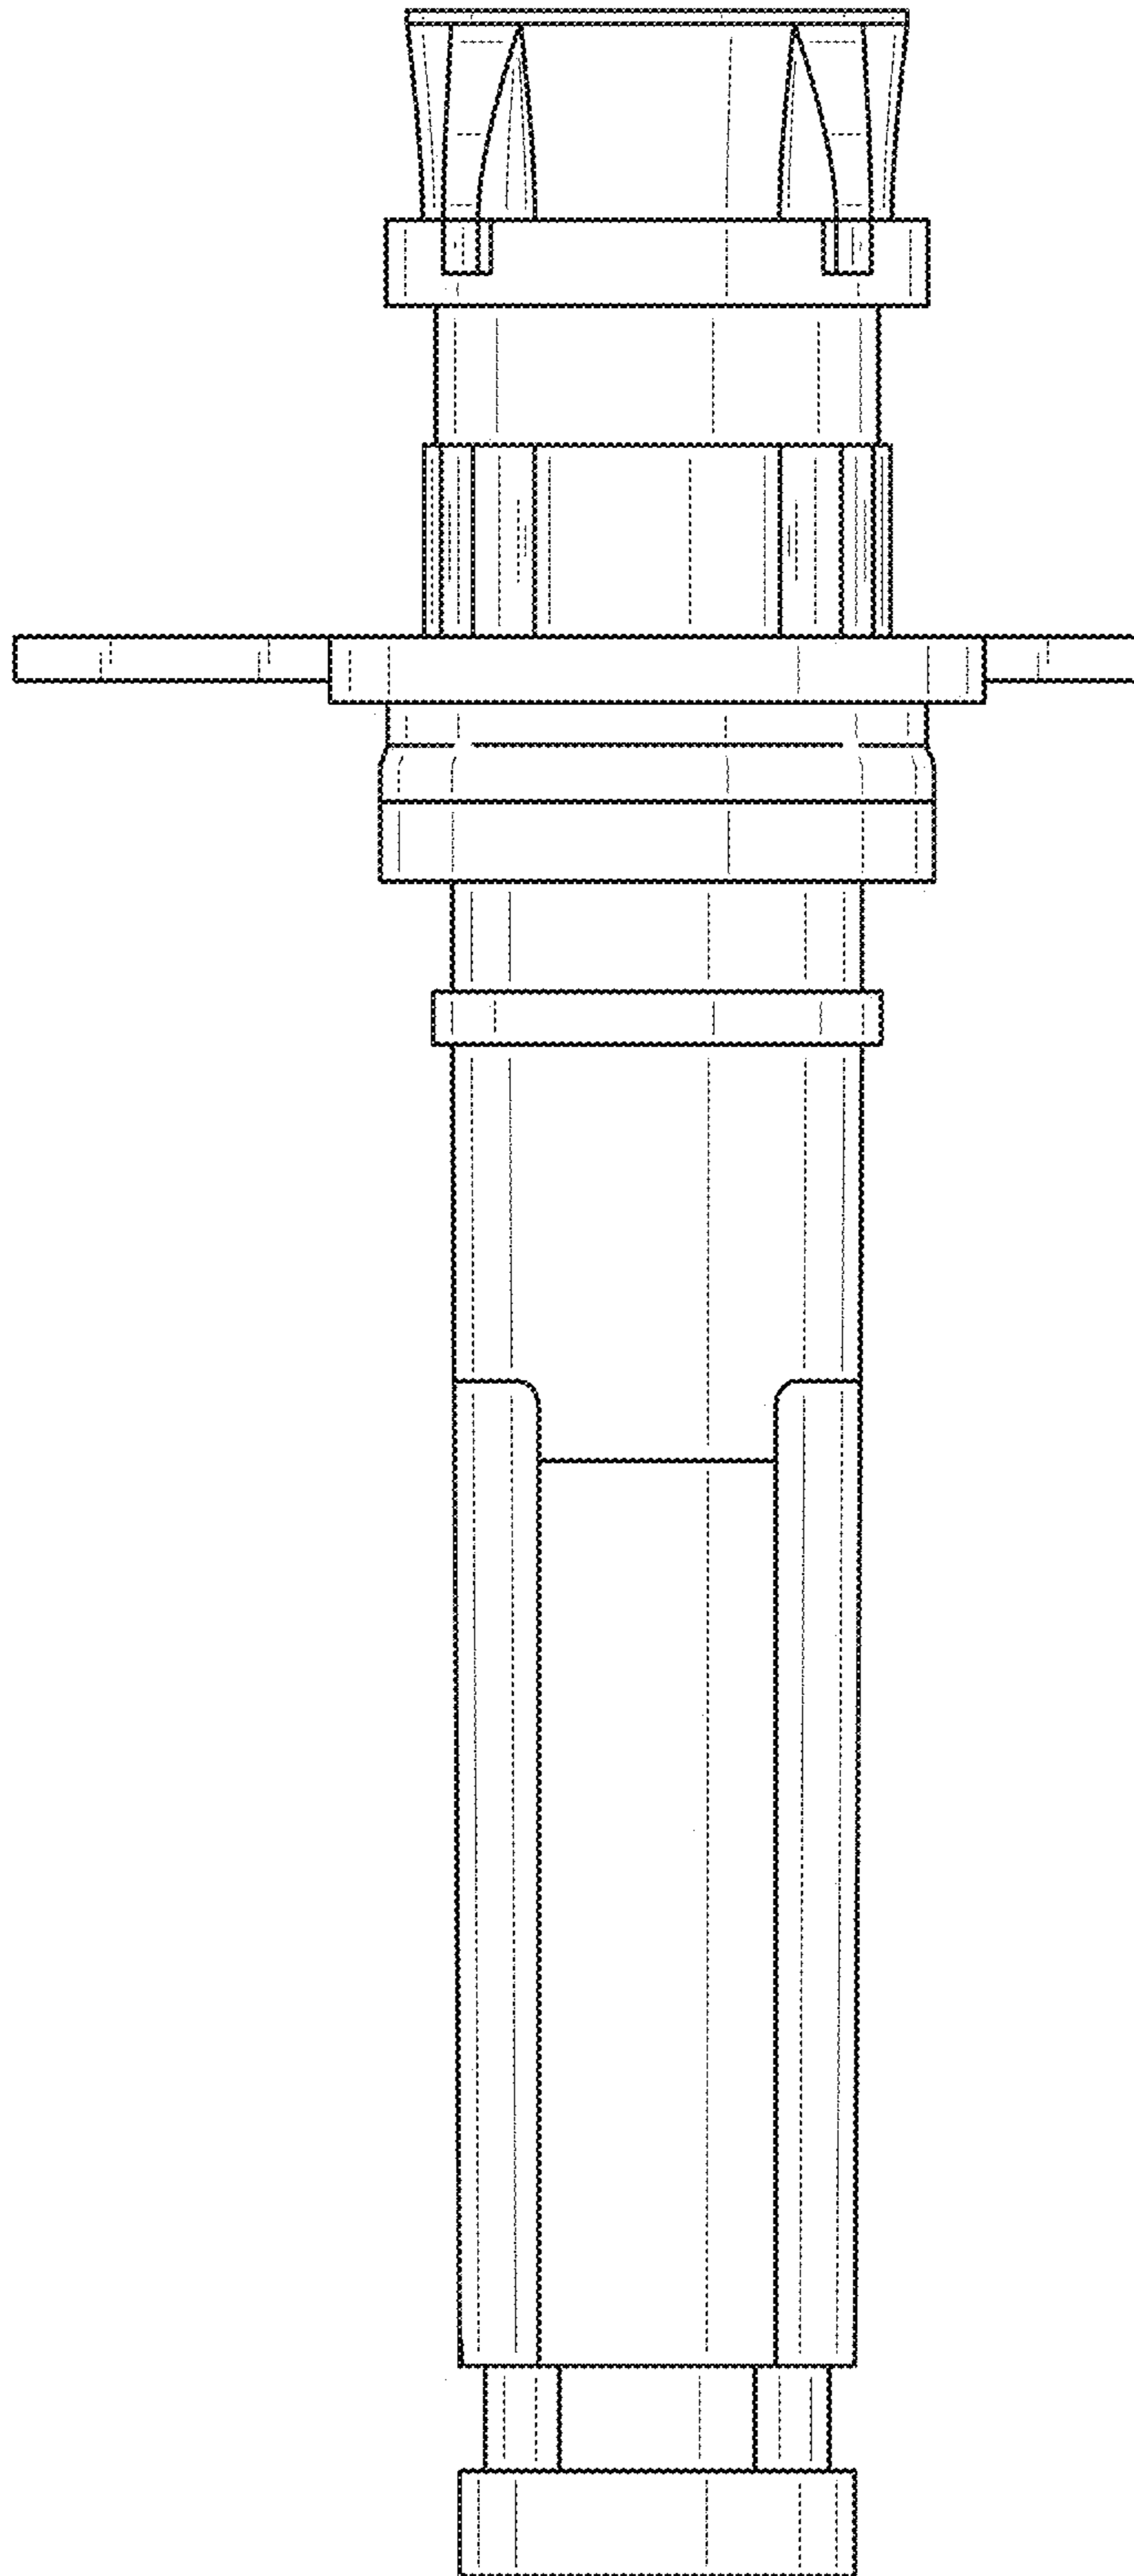


FIG. 4

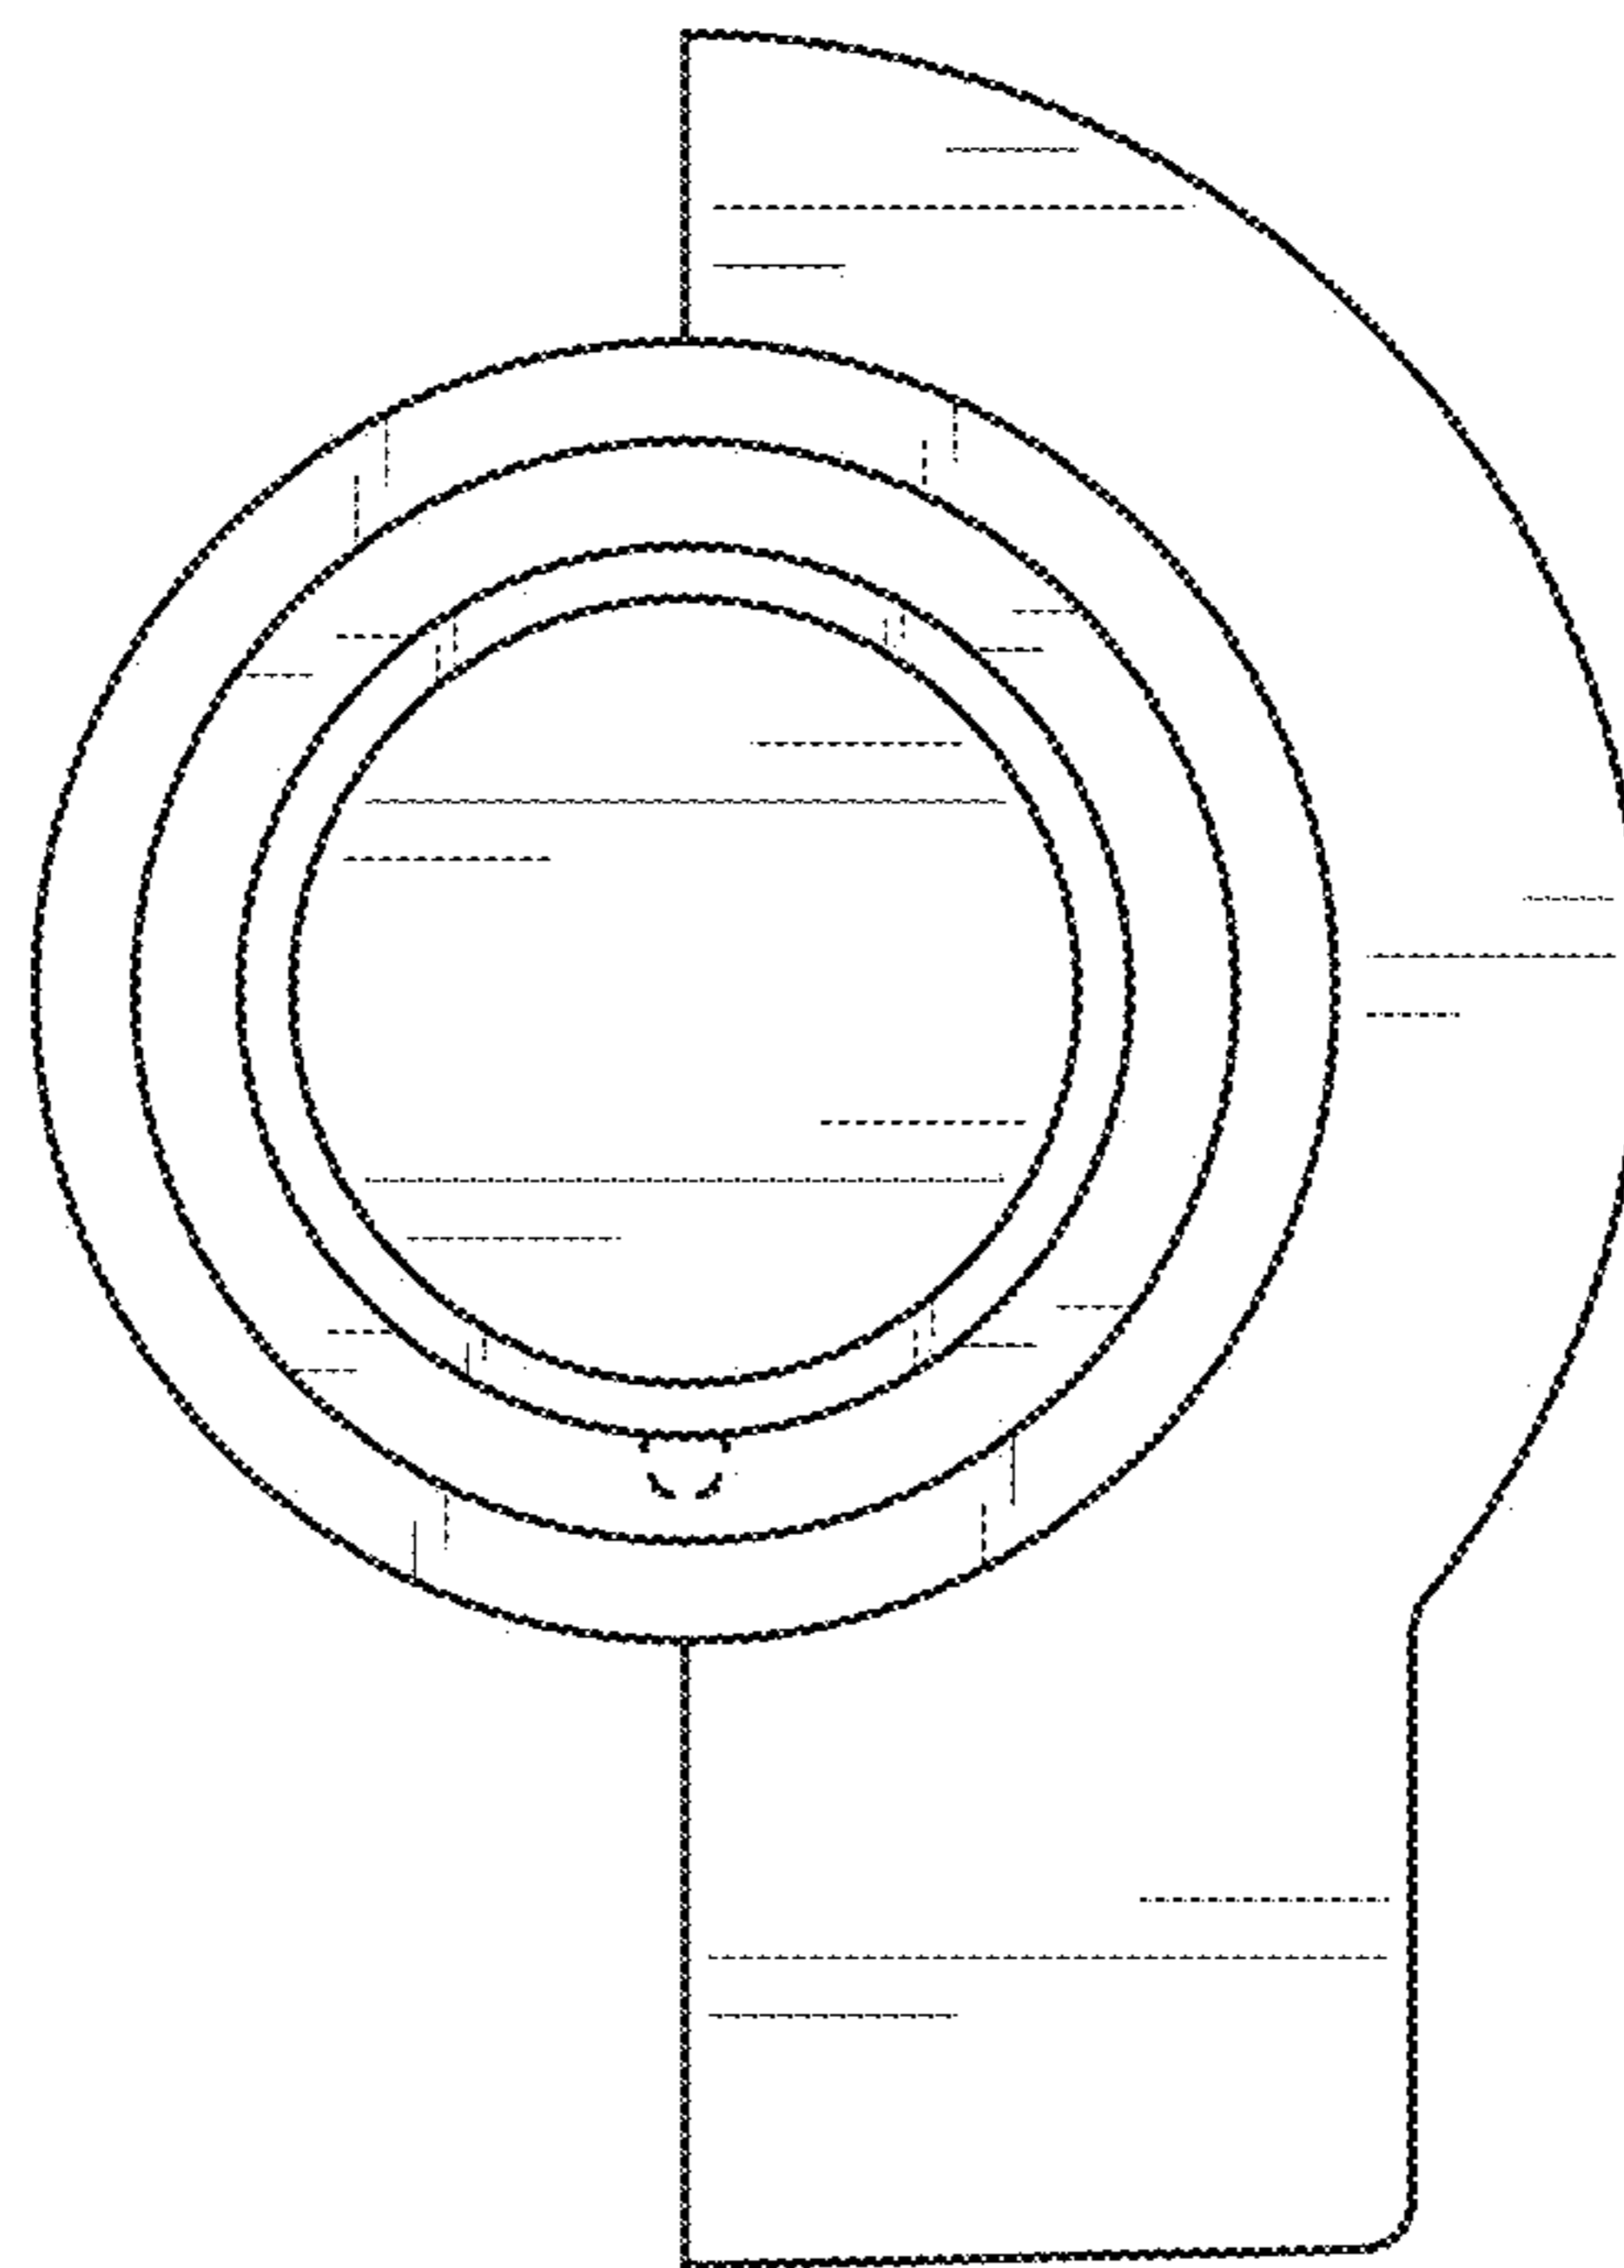


FIG. 5

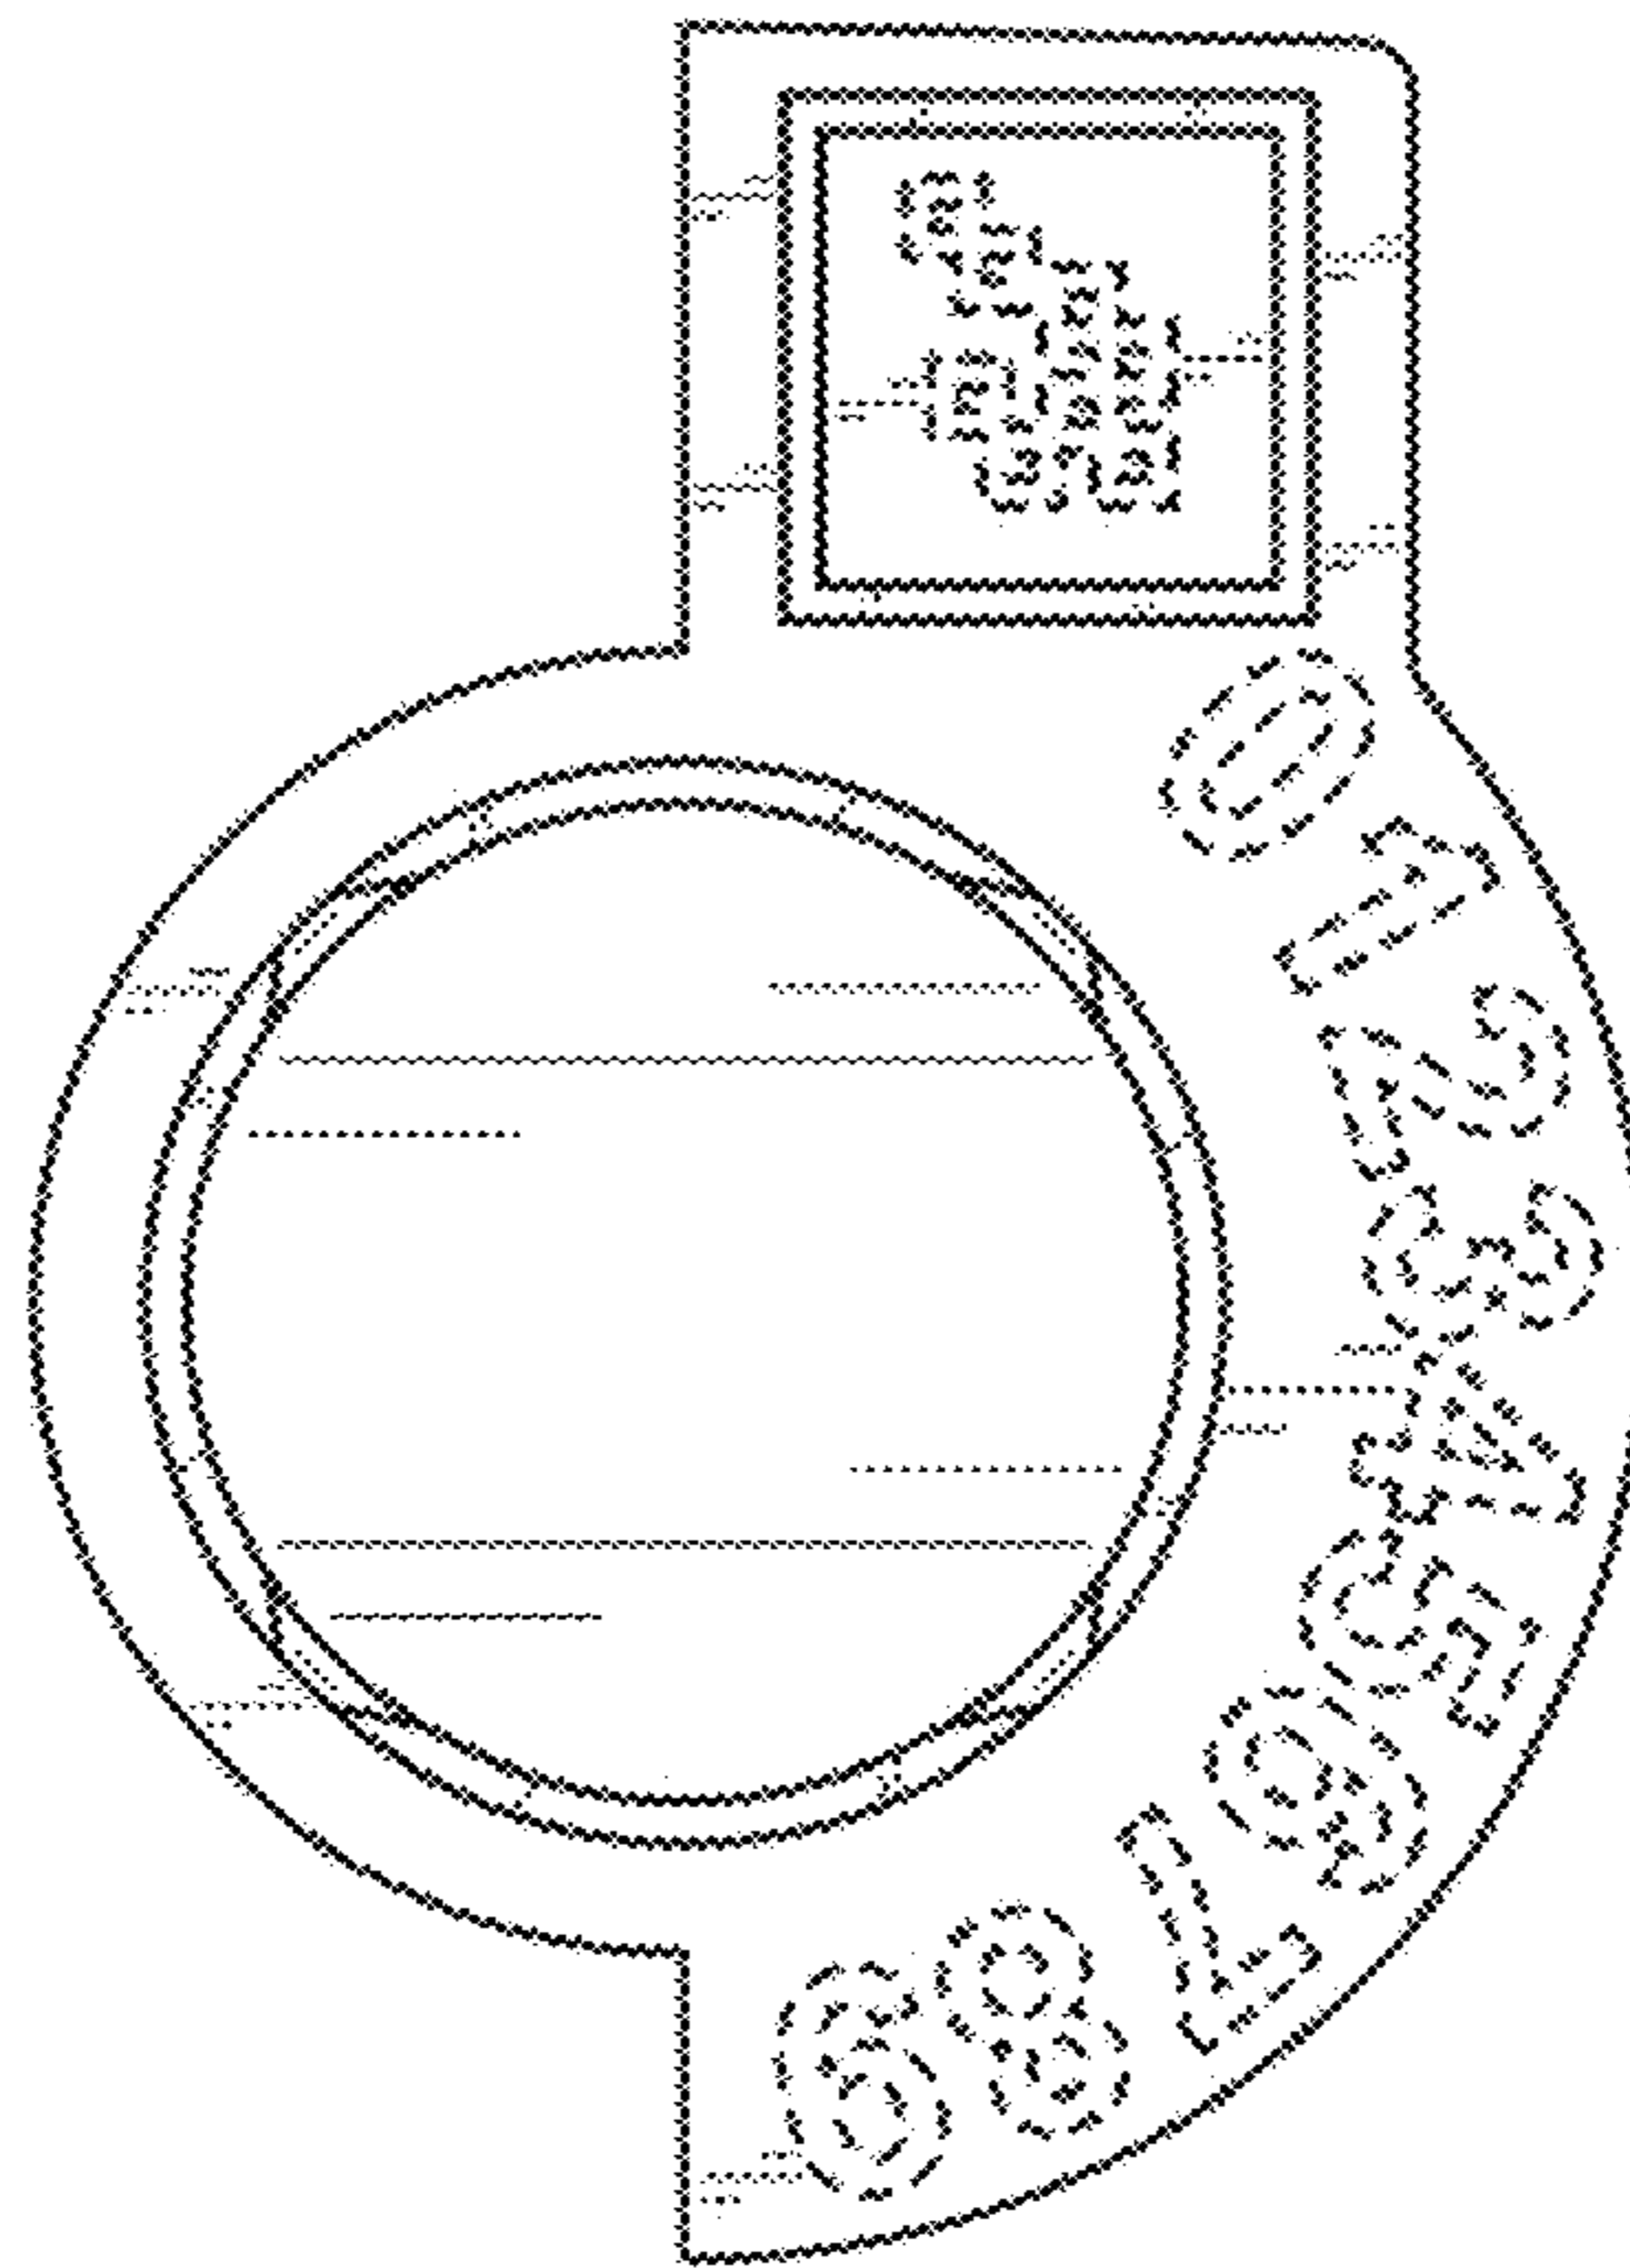


FIG. 6

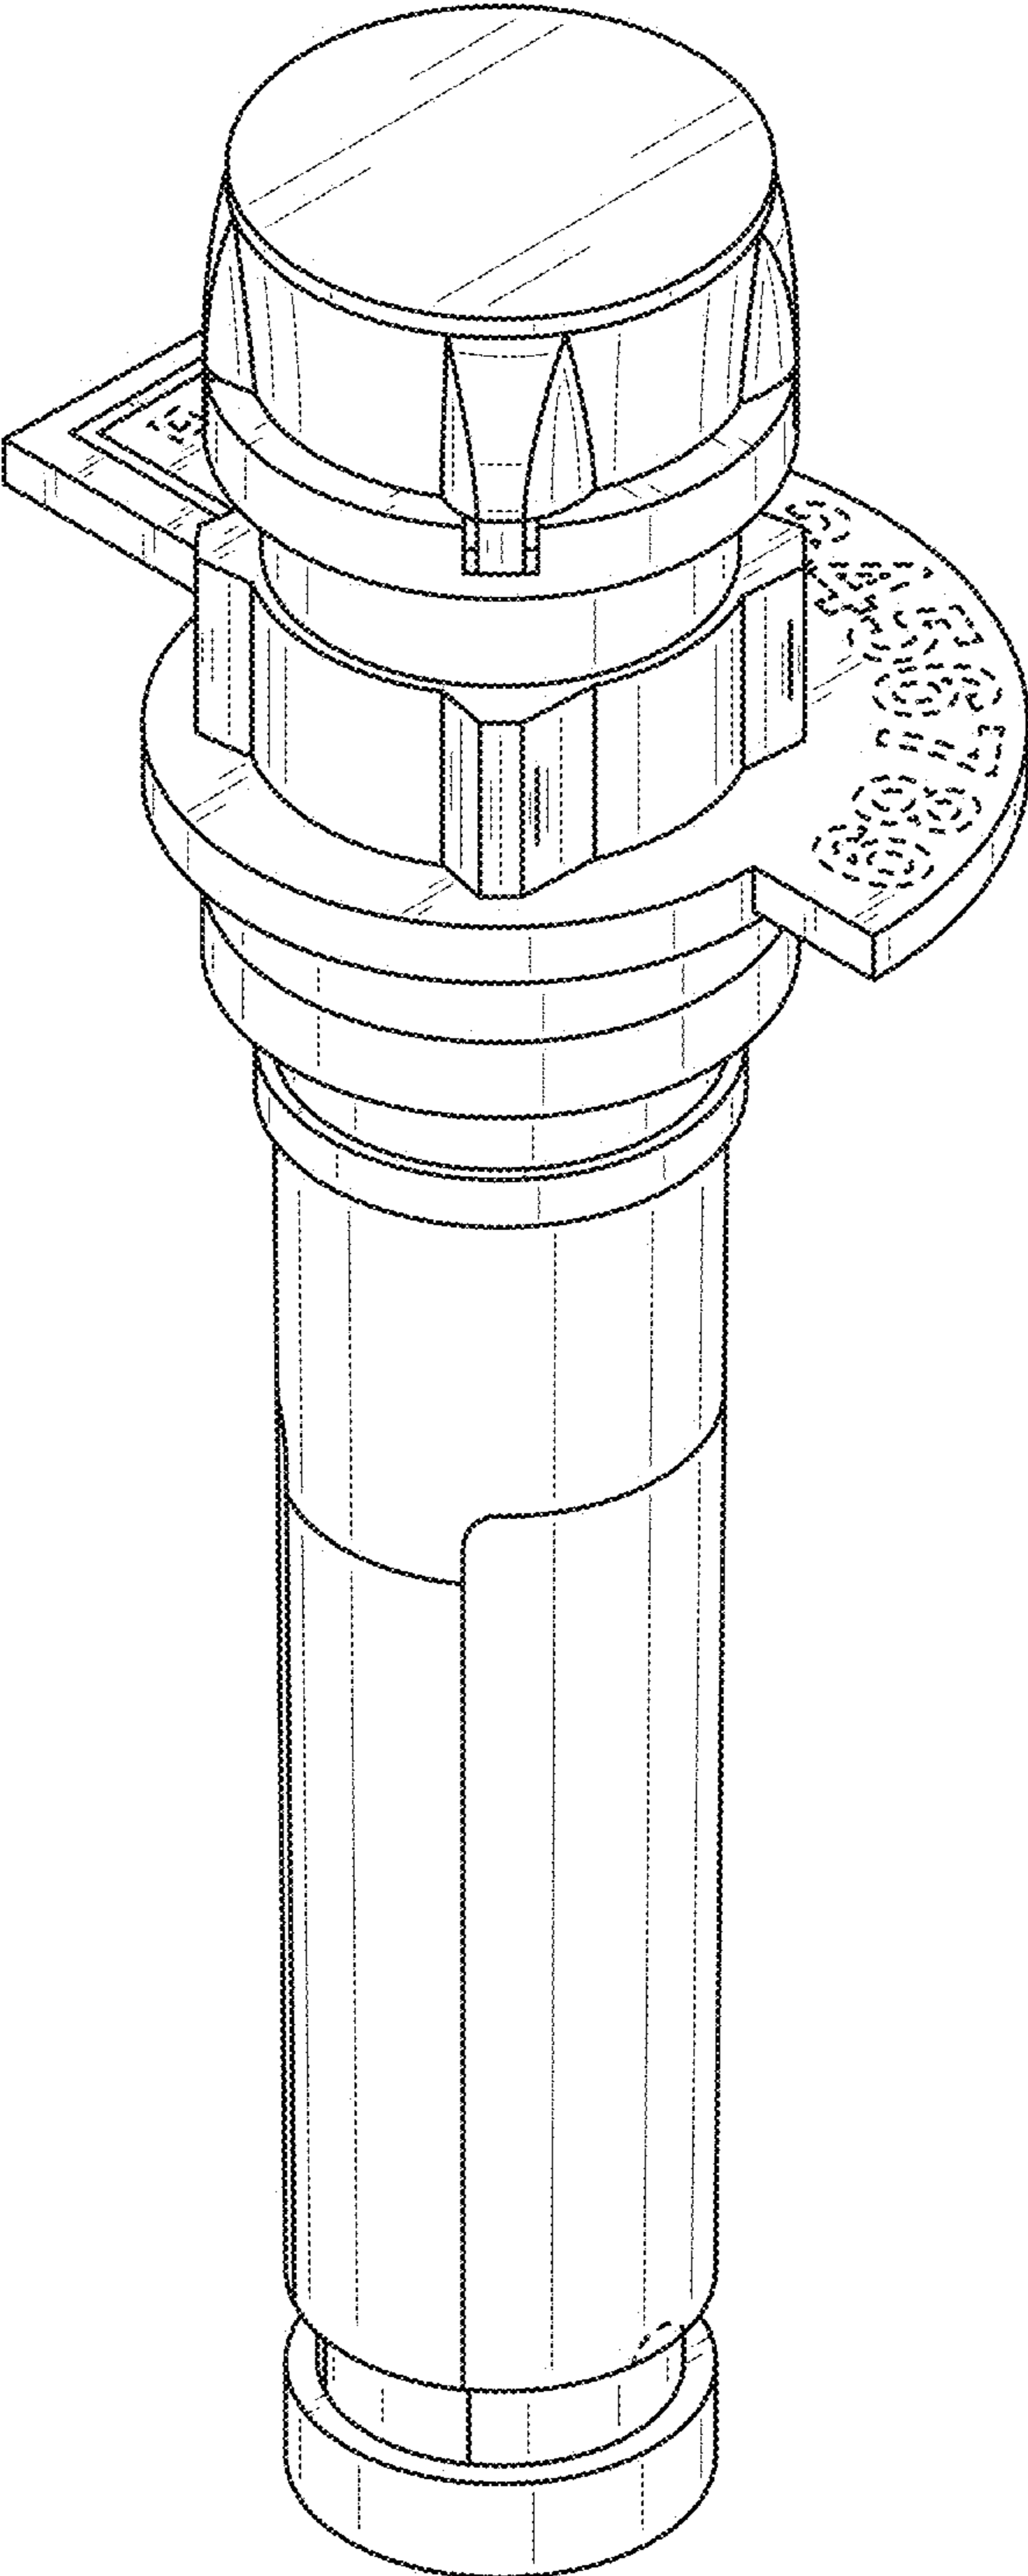


FIG. 7