



US00D954973S

(12) **United States Design Patent** (10) **Patent No.:** **US D954,973 S**  
**Mack et al.** (45) **Date of Patent:** **\*\* Jun. 14, 2022**

(54) **ULTRASOUND PROBE**

D846,749 S \* 4/2019 de Jonge ..... D24/187  
D869,663 S \* 12/2019 de Jonge ..... D24/187  
D869,664 S 12/2019 de Jonge et al.

(71) Applicant: **BFLY Operations, Inc.**, Guilford, CT (US)

(Continued)

(72) Inventors: **Adam Mekeel Mack**, Half Moon Bay, CA (US); **Ryan Silvestri**, Guilford, CT (US); **Timothy A. Hyde**, Columbia, SC (US); **Neil Ferrier**, Greenville, SC (US); **Kevin Coss**, Irvine, CA (US); **David Elgena**, Orlando, FL (US); **Matthew de Jonge**, Brooklyn, NY (US); **Jason Fischman**, Stamford, CT (US)

FOREIGN PATENT DOCUMENTS

CN 305760932 S 5/2020  
KR 3020180020019 \* 2/2019

(73) Assignee: **BFLY Operations, Inc.**, Guilford, CT (US)

OTHER PUBLICATIONS

Esaote SP2430 For Sale. Online, published date unknown. Retrieved on Aug. 23, 2021 from URL: [https://www.providianmedical.com/ultrasound-probes/esaote/esaote-sp2430.\\*](https://www.providianmedical.com/ultrasound-probes/esaote/esaote-sp2430.*)

(Continued)

*Primary Examiner* — Omeed Agilee

(\*\*) Term: **15 Years**

(74) *Attorney, Agent, or Firm* — Wolf, Greenfield & Sacks, P.C.

(21) Appl. No.: **29/740,055**

(57) **CLAIM**

The ornamental design for an ultrasound probe, as shown and described.

(22) Filed: **Jun. 30, 2020**

**DESCRIPTION**

(51) **LOC (13) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/187**

(58) **Field of Classification Search**  
USPC ..... D24/133, 137, 138, 141, 158, 160, 164, D24/165, 167, 170, 186, 187, 200; D10/57, 60, 78, 80  
CPC ... A61B 5/0095; A61B 8/4444; A61B 8/4455; A61B 8/445; G01S 7/5208; G01N 29/265  
See application file for complete search history.

FIG. 1 is a bottom, front, right side perspective view of an ultrasound probe showing our new design; FIG. 2 is a bottom plan view thereof; FIG. 3 is a top plan view thereof; FIG. 4 is a left side elevation view thereof; FIG. 5 is a front elevation view thereof; FIG. 6 is a rear elevation view thereof; and, FIG. 7 is a right side elevation view thereof.


The long dash-short dash broken lines in the figures represent boundaries of the claimed design and form no part thereof. All other broken lines represent portions of the ultrasound probe that form no part of the claimed design. The ultrasound probe is shown with a symbolic break in its length. The appearance of any portion of the article between the break lines forms no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,436,050 B2 \* 8/2002 Garrison ..... B25F 5/02 600/459  
D488,726 S 4/2004 Wong  
D545,433 S 6/2007 Messerly

**1 Claim, 3 Drawing Sheets**

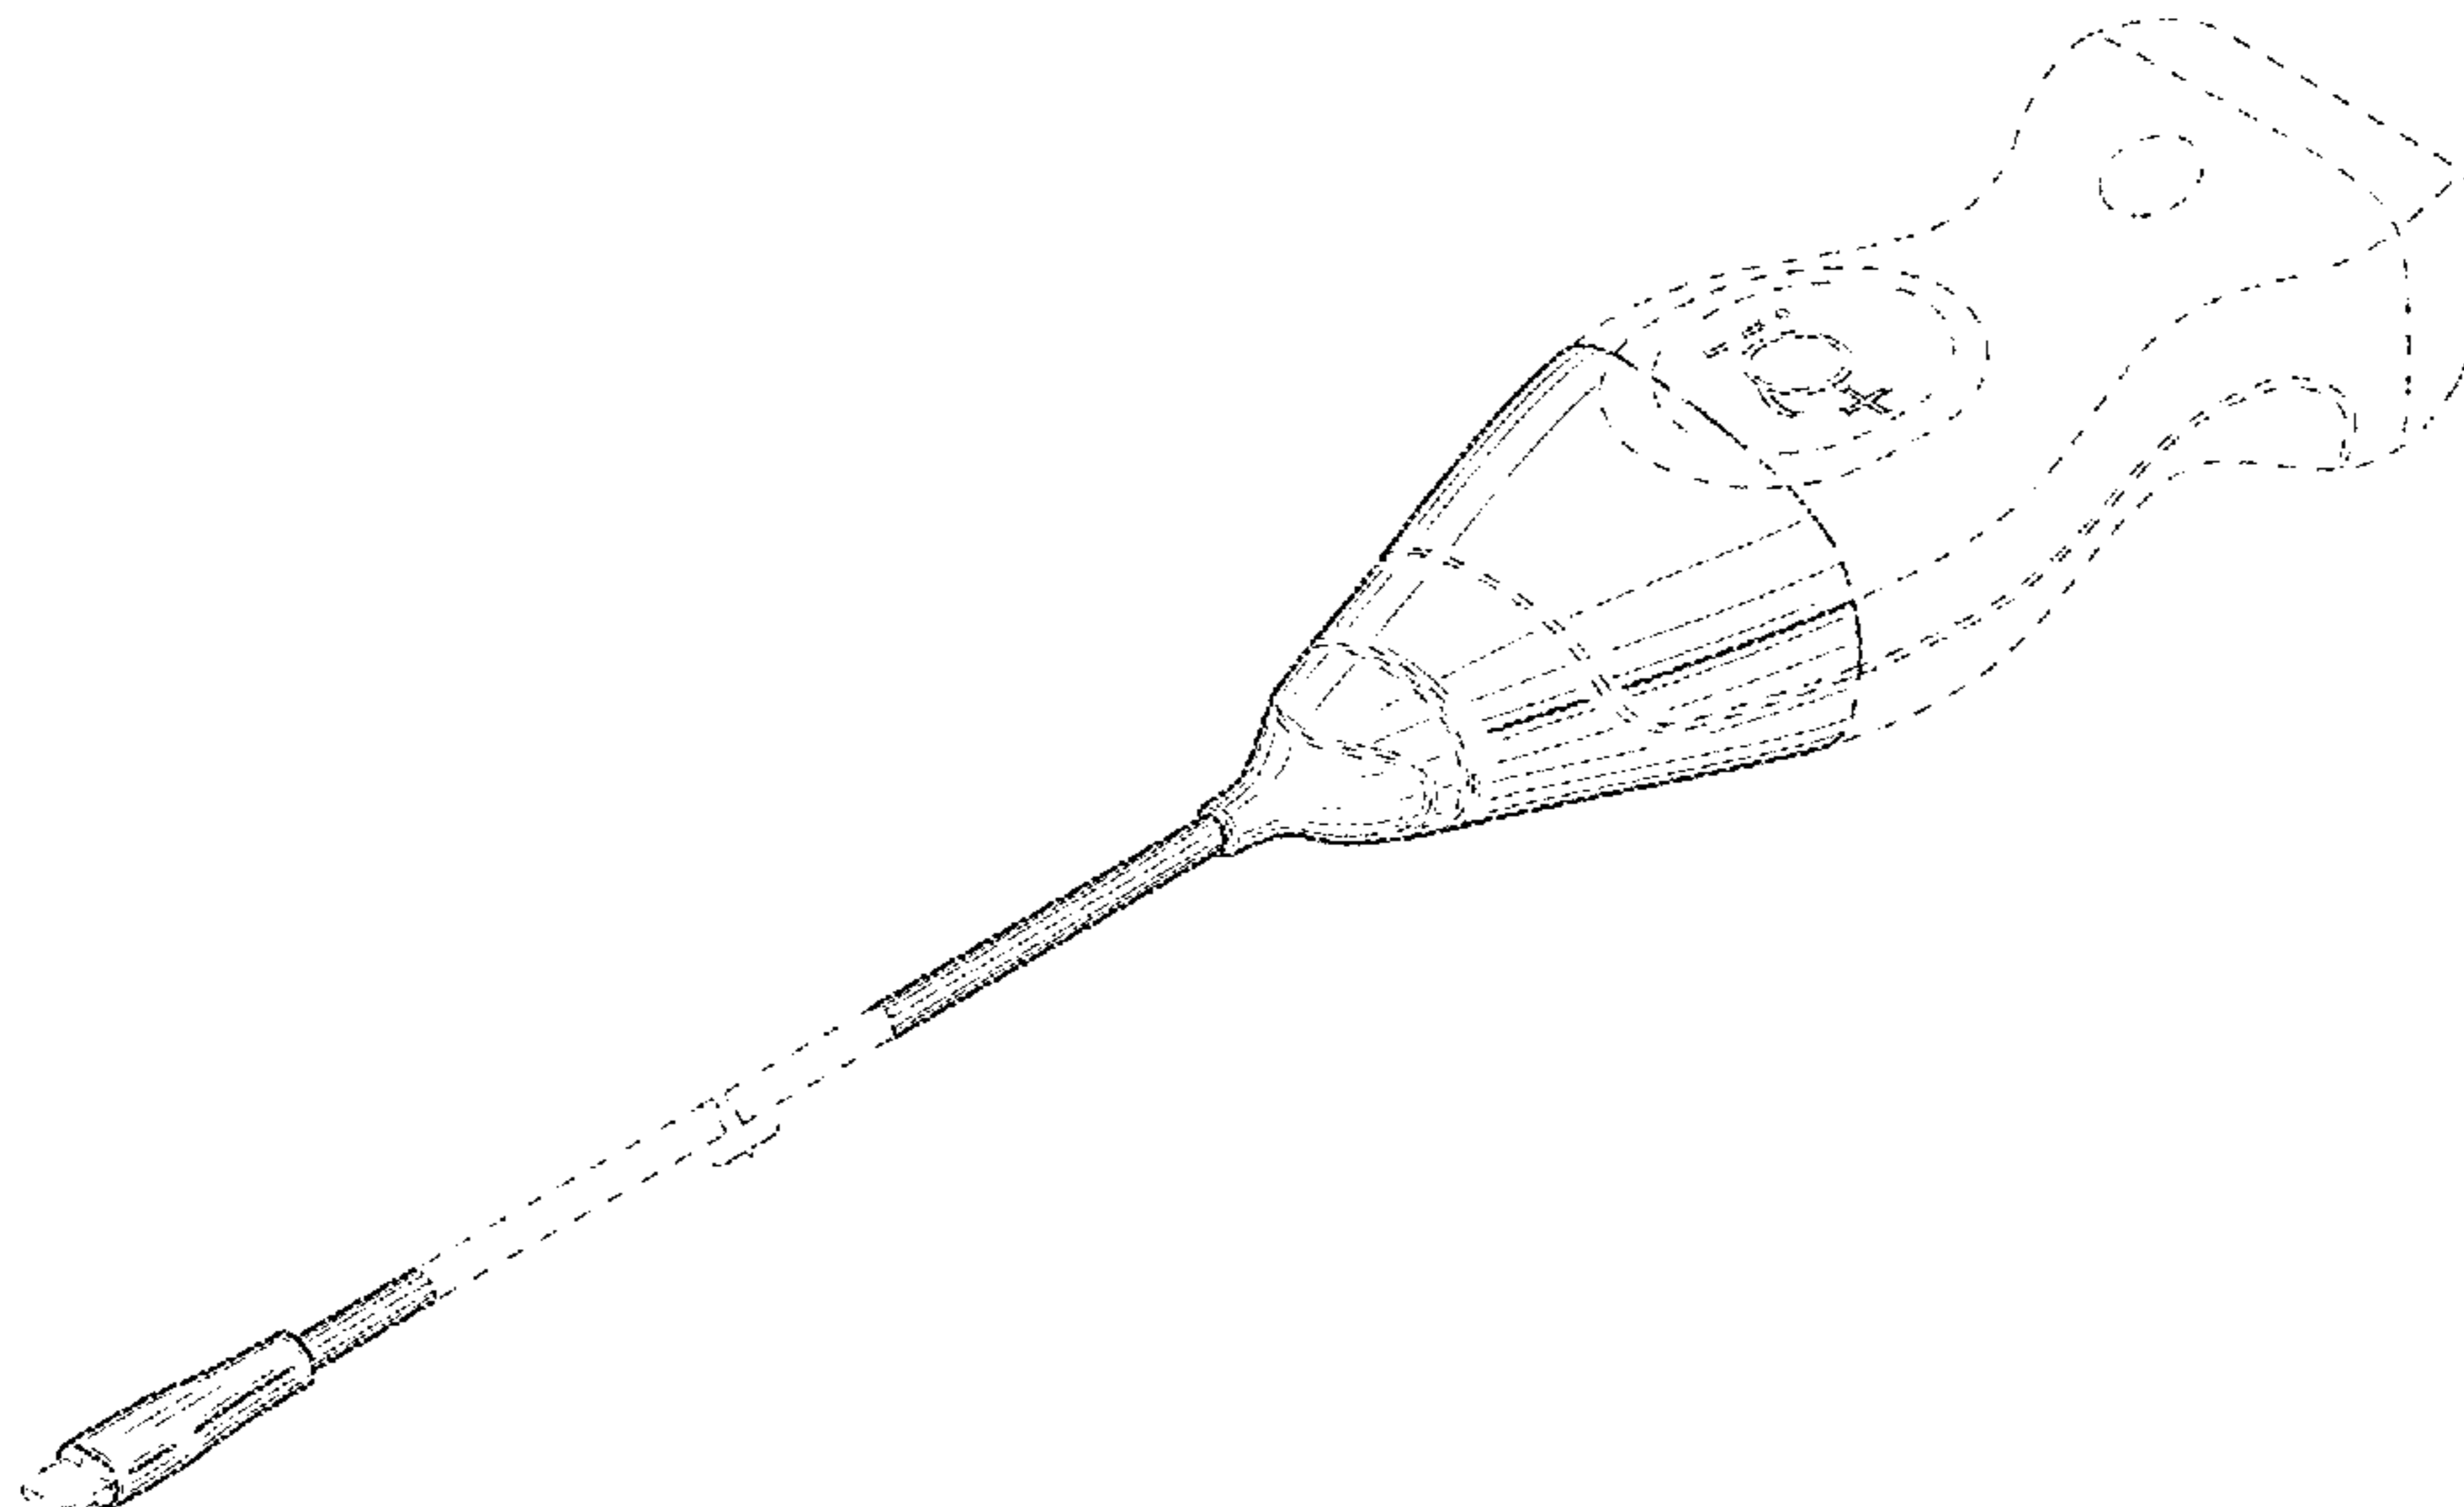

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D869,665 S \* 12/2019 de Jonge ..... D24/187  
 D870,295 S 12/2019 de Jonge et al.  
 D886,305 S 6/2020 de Jonge et al.  
 D887,562 S \* 6/2020 de Jonge ..... D24/187  
 D896,973 S \* 9/2020 Wight ..... D24/187  
 10,820,885 B2 \* 11/2020 Cohen ..... A61B 8/429  
 D916,295 S \* 4/2021 Shibayama ..... D24/187  
 D939,092 S \* 12/2021 Roy ..... D24/186  
 2013/0301395 A1 \* 11/2013 Hebrard ..... G01S 7/52079  
 367/189  
 2015/0112200 A1 \* 4/2015 Oberg ..... A61B 8/4444  
 600/461  
 2018/0028159 A1 2/2018 Hageman et al.  
 2021/0408716 A1 \* 12/2021 Schneider ..... H01R 13/5224  
 2022/0008037 A1 \* 1/2022 Hamada ..... G10K 11/26

OTHER PUBLICATIONS

Small Animal Ultrasound Probes. Online, published date unknown.  
 Retrieved on Jan. 14, 2022 from URL: <https://www.imotek.com/products/veterinary-ultrasound-/probes/155/small-animal-ultrasound-probes/>.  
 [No Author Listed] HDI 5000 Transducer Listing. Publicly known prior to Oct. 27, 2017. 4 pages.  
 Enriquez et al., An Introduction to Ultrasound Equipment and Knobology. Crit Care Clin. Jan. 2014; 30(1):25-45.

\* cited by examiner

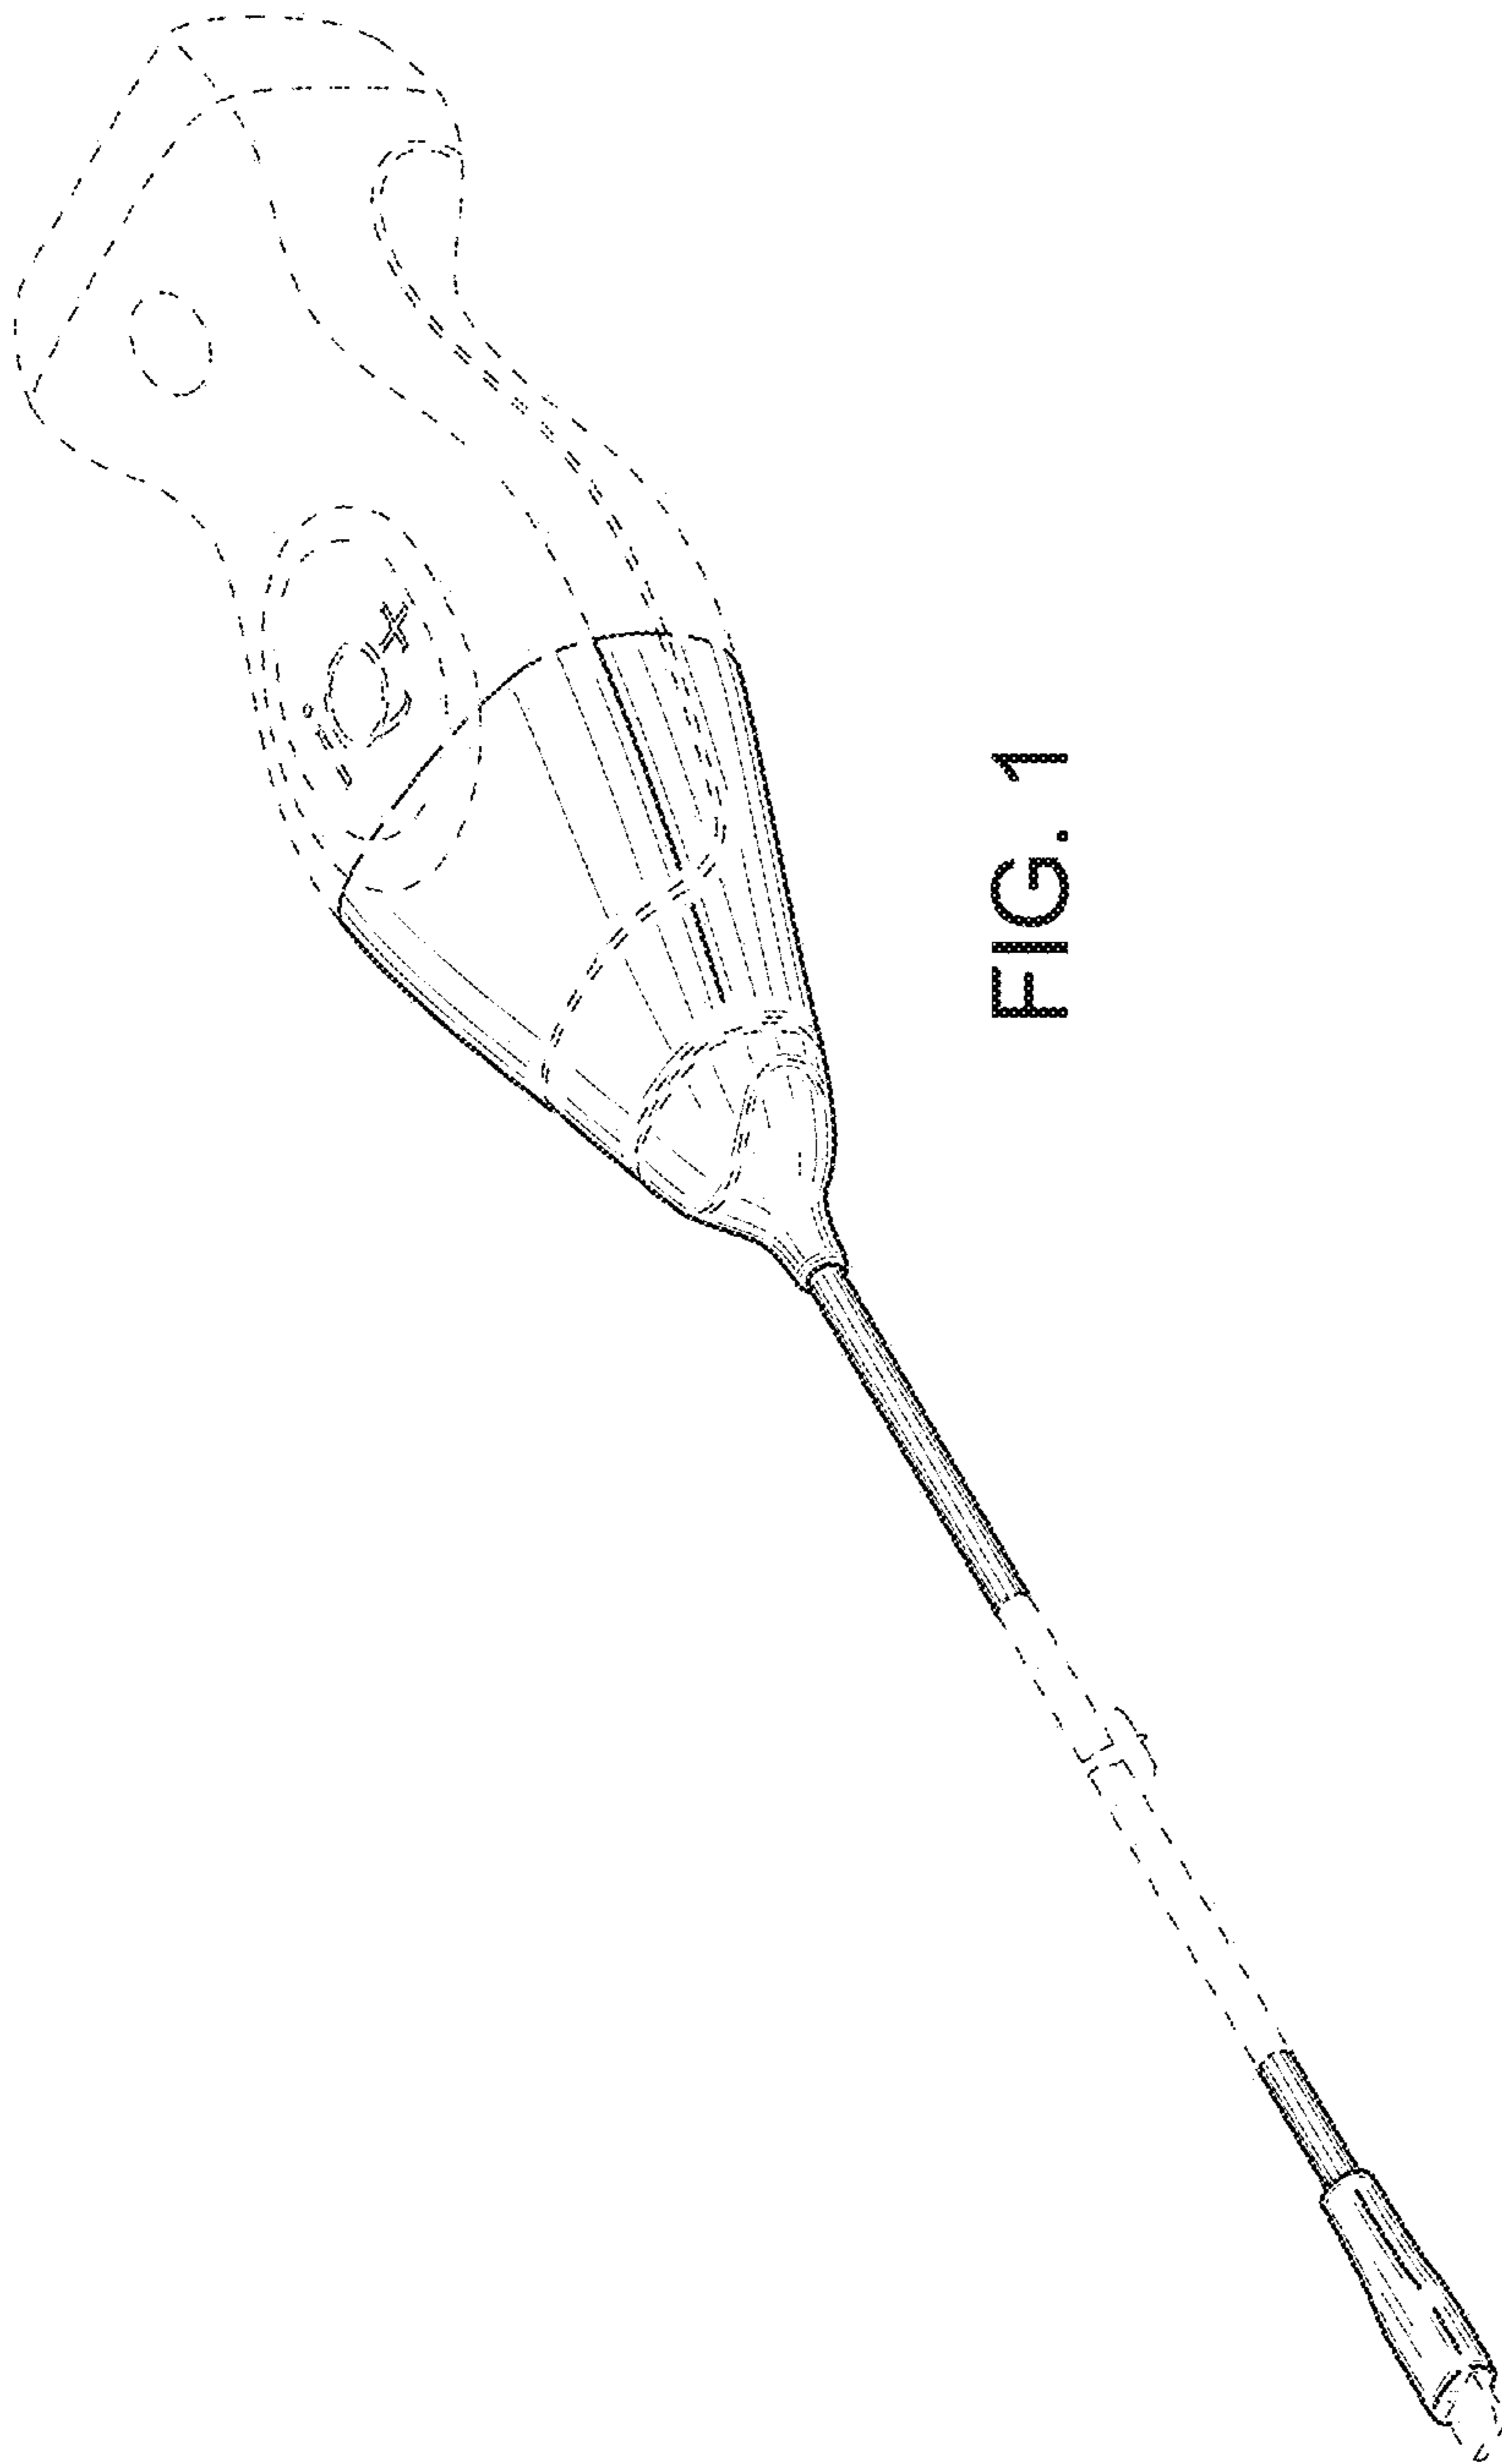


FIG. 1

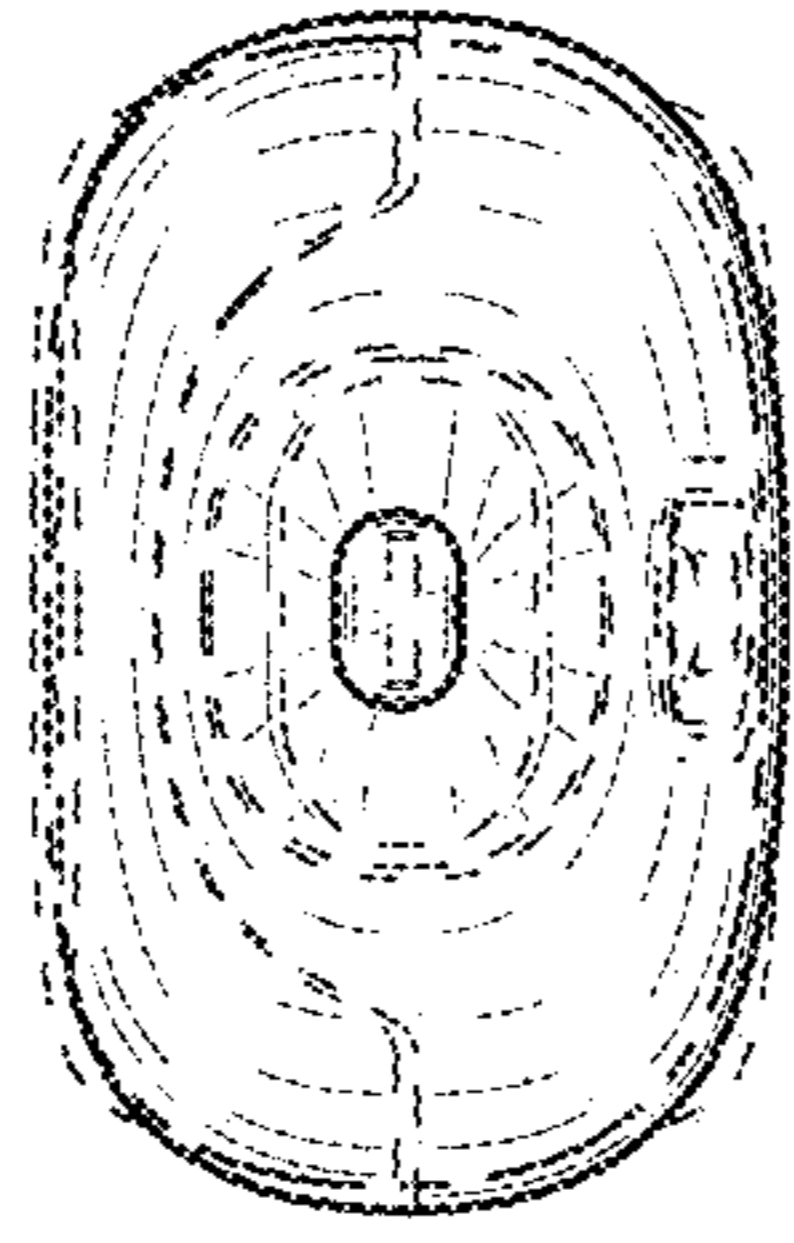


FIG. 2



FIG. 3

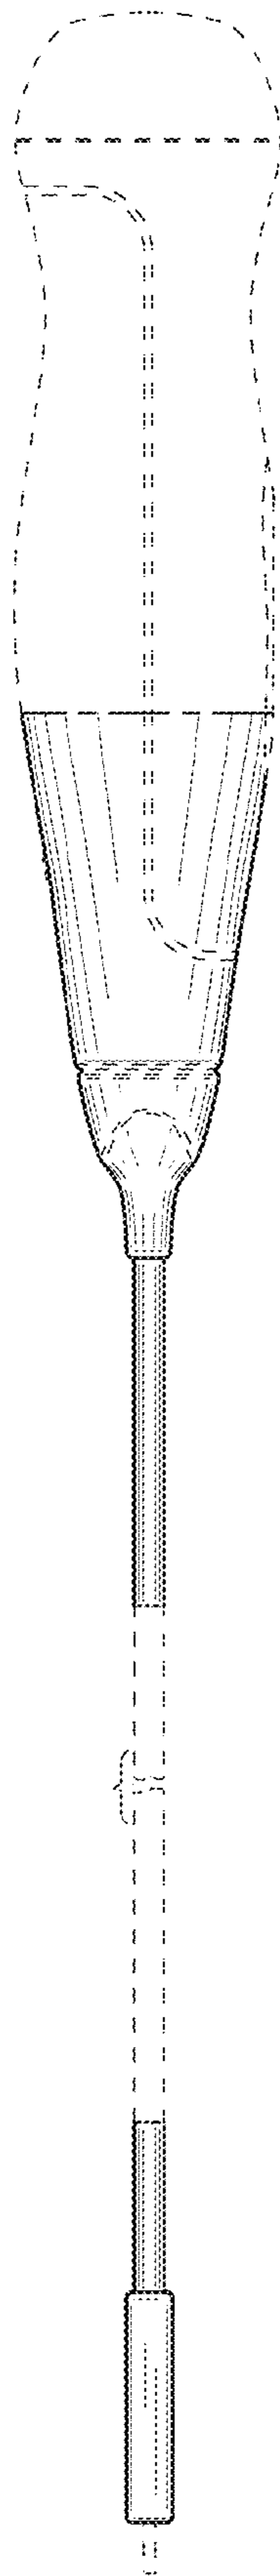


FIG. 4

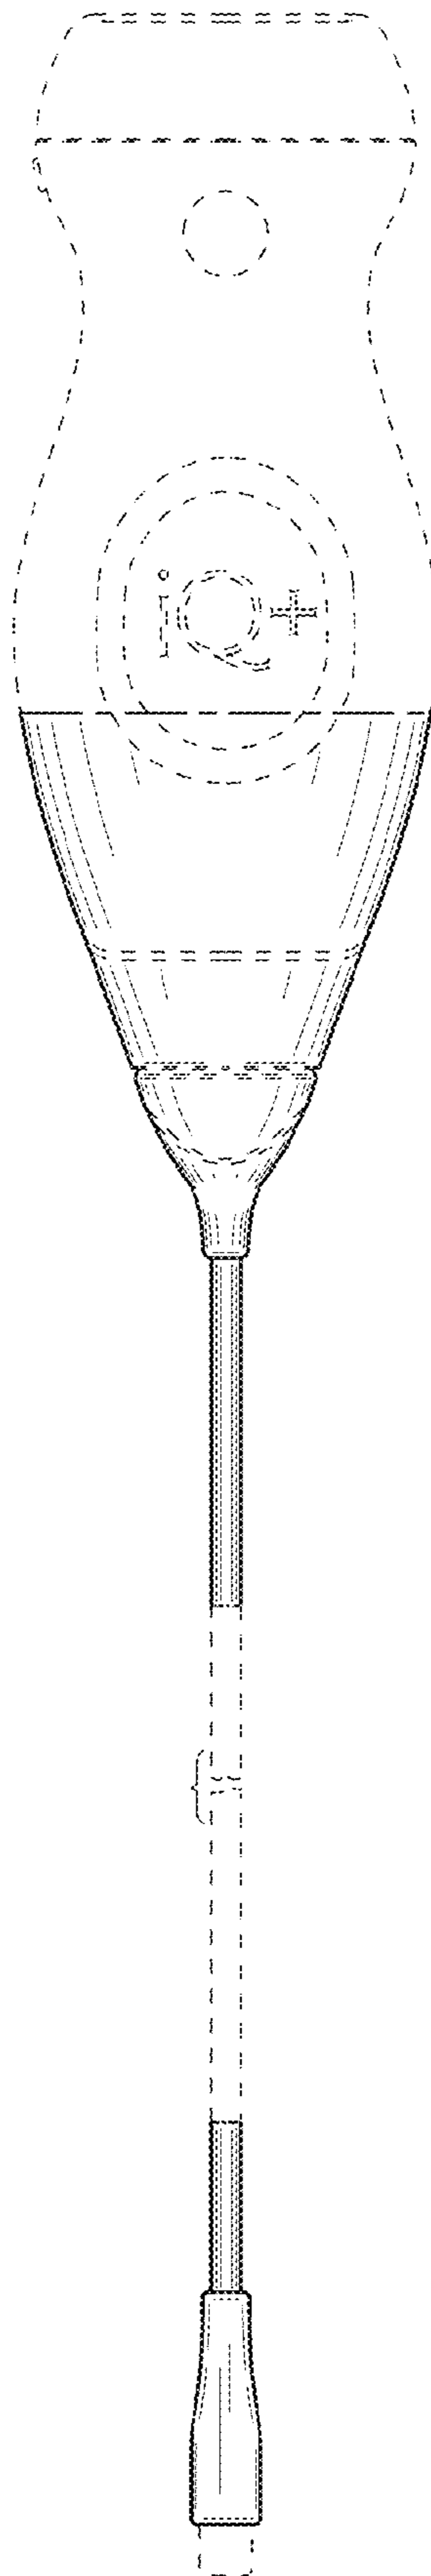


FIG. 5

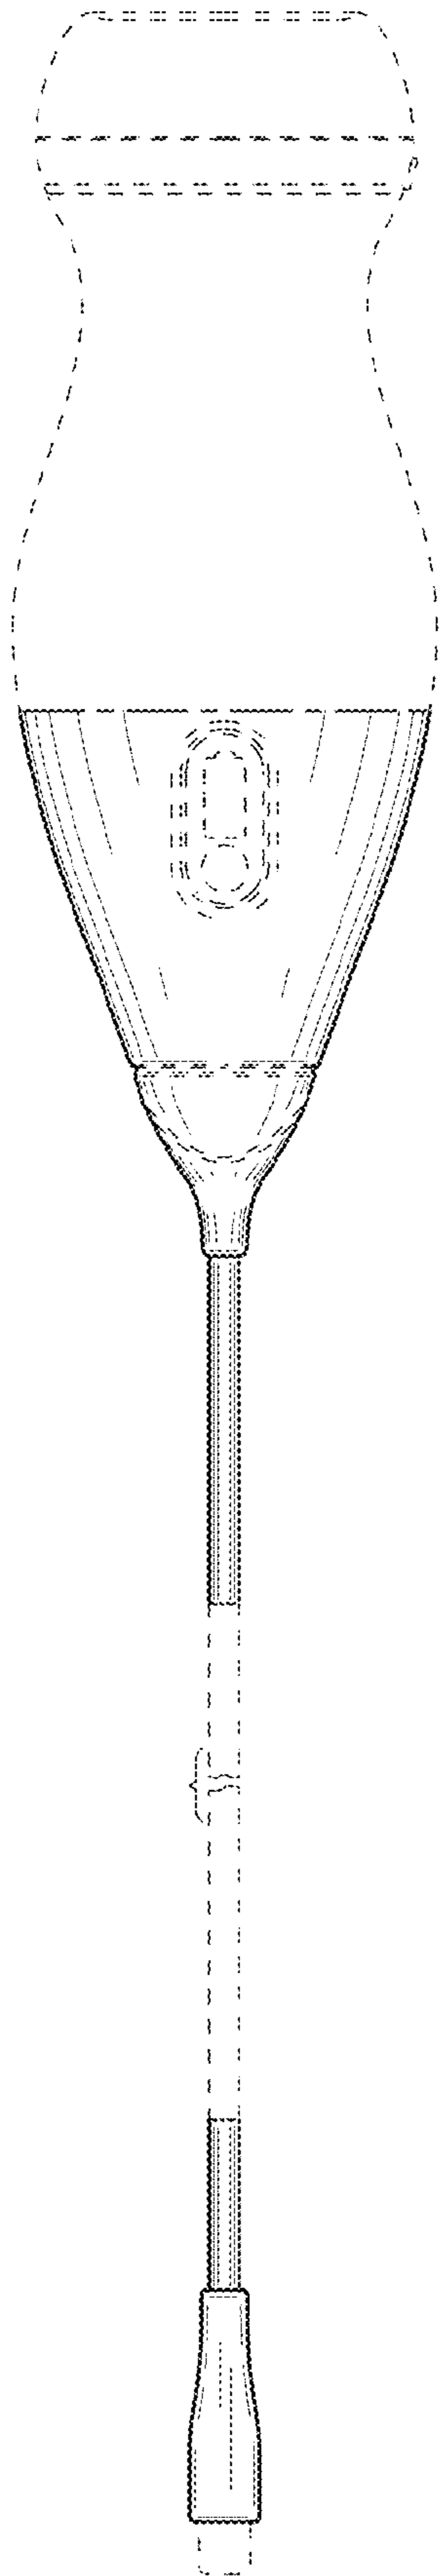


FIG. 6

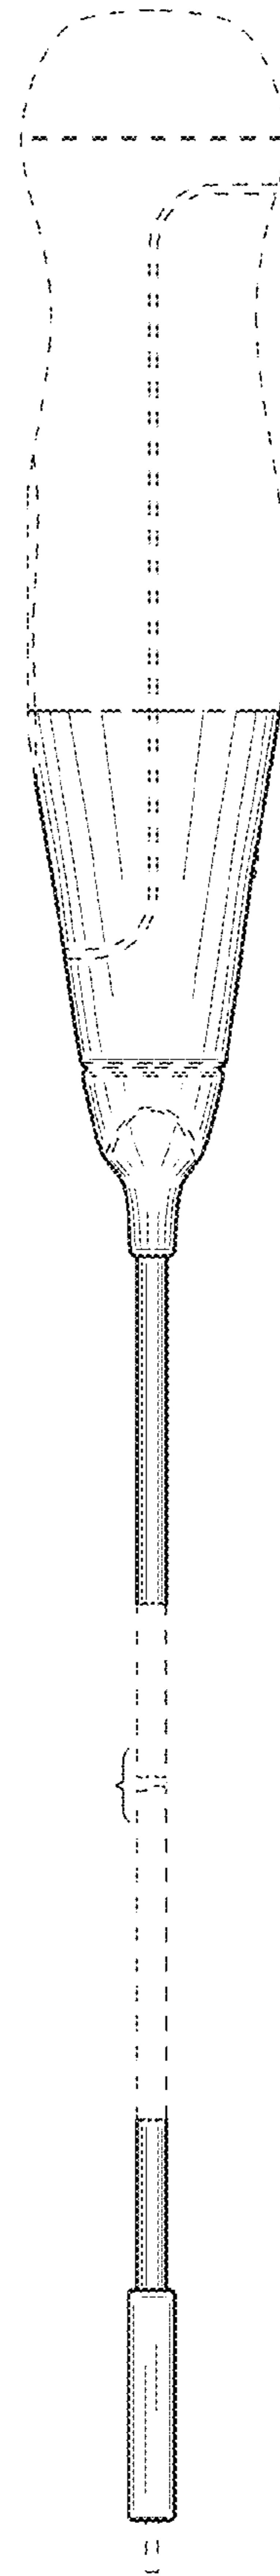


FIG. 7