



US00D954981S

(12) **United States Design Patent** (10) **Patent No.:** **US D954,981 S**  
**Laverack et al.** (45) **Date of Patent:** **\*\* Jun. 14, 2022**

(54) **TESTING DEVICE**

(71) Applicant: **SPD Swiss Precision Diagnostics GMBH**, Geneva (CH)

(72) Inventors: **Paul J. Laverack**, Leighton Buzzard (GB); **Sunil Kalbandi**, Redlodge (GB); **James Gani**, Bedford (GB)

(73) Assignee: **SPD Swiss Precision Diagnostics GmbH**, Geneva (CH)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/708,023**

(22) Filed: **Oct. 2, 2019**

(30) **Foreign Application Priority Data**

Apr. 3, 2019 (EM) ..... 006367363

(51) LOC (13) Cl. ..... **24-02**

(52) U.S. Cl.

USPC ..... **D24/223**

(58) **Field of Classification Search**

USPC ..... D24/107, 108, 112–114, 127, 130, 133, D24/169, 186, 216–217, 219, 222–226, D24/227, 231, 232; D10/81

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D531,735 S \* 11/2006 Lee ..... D24/223  
D571,020 S \* 6/2008 Laverack ..... D24/225

(Continued)

FOREIGN PATENT DOCUMENTS

EM 007337225-0002 \* 12/2019

OTHER PUBLICATIONS

Clearblue Plus Pregnancy Test, 3 Pregnancy Tests. Online, published date May 1, 2018. Retrieved on Mar. 24, 2021 from URL:

[https://www.amazon.com.au/Clearblue-Plus-Pregnancy-Test-Tests/dp/B000NDS2CC.\\*](https://www.amazon.com.au/Clearblue-Plus-Pregnancy-Test-Tests/dp/B000NDS2CC.*)

*Primary Examiner* — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Erik A. Huestis; Foley Hoag LLP

(57) **CLAIM**

The ornamental design for a testing device, as shown and described.

**DESCRIPTION**

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a top perspective view of a testing device with its cap on;

FIG. 2 is a bottom perspective view of the testing device with its cap on;

FIG. 3 is a side view of the testing device with its cap on;

FIG. 4 is a top view of the testing device with its cap on;

FIG. 5 is a bottom view of the testing device with its cap on;

FIG. 6 is an enlarged front view of the testing device with its cap on;

FIG. 7 is an enlarged rear view of the testing device with its cap on;

FIG. 8 is a top perspective view of the testing device with its cap off;

FIG. 9 is a bottom perspective view of the testing device with its cap off;

FIG. 10 is a side view of the testing device with its cap off;


FIG. 11 is a top view of the testing device with its cap off;

FIG. 12 is a bottom view of the testing device with its cap off;

FIG. 13 is an enlarged front view of the testing device with its cap off; and,

FIG. 14 is an enlarged rear view of the testing device with its cap off.

**1 Claim, 14 Drawing Sheets**  
**(14 of 14 Drawing Sheet(s) Filed in Color)**

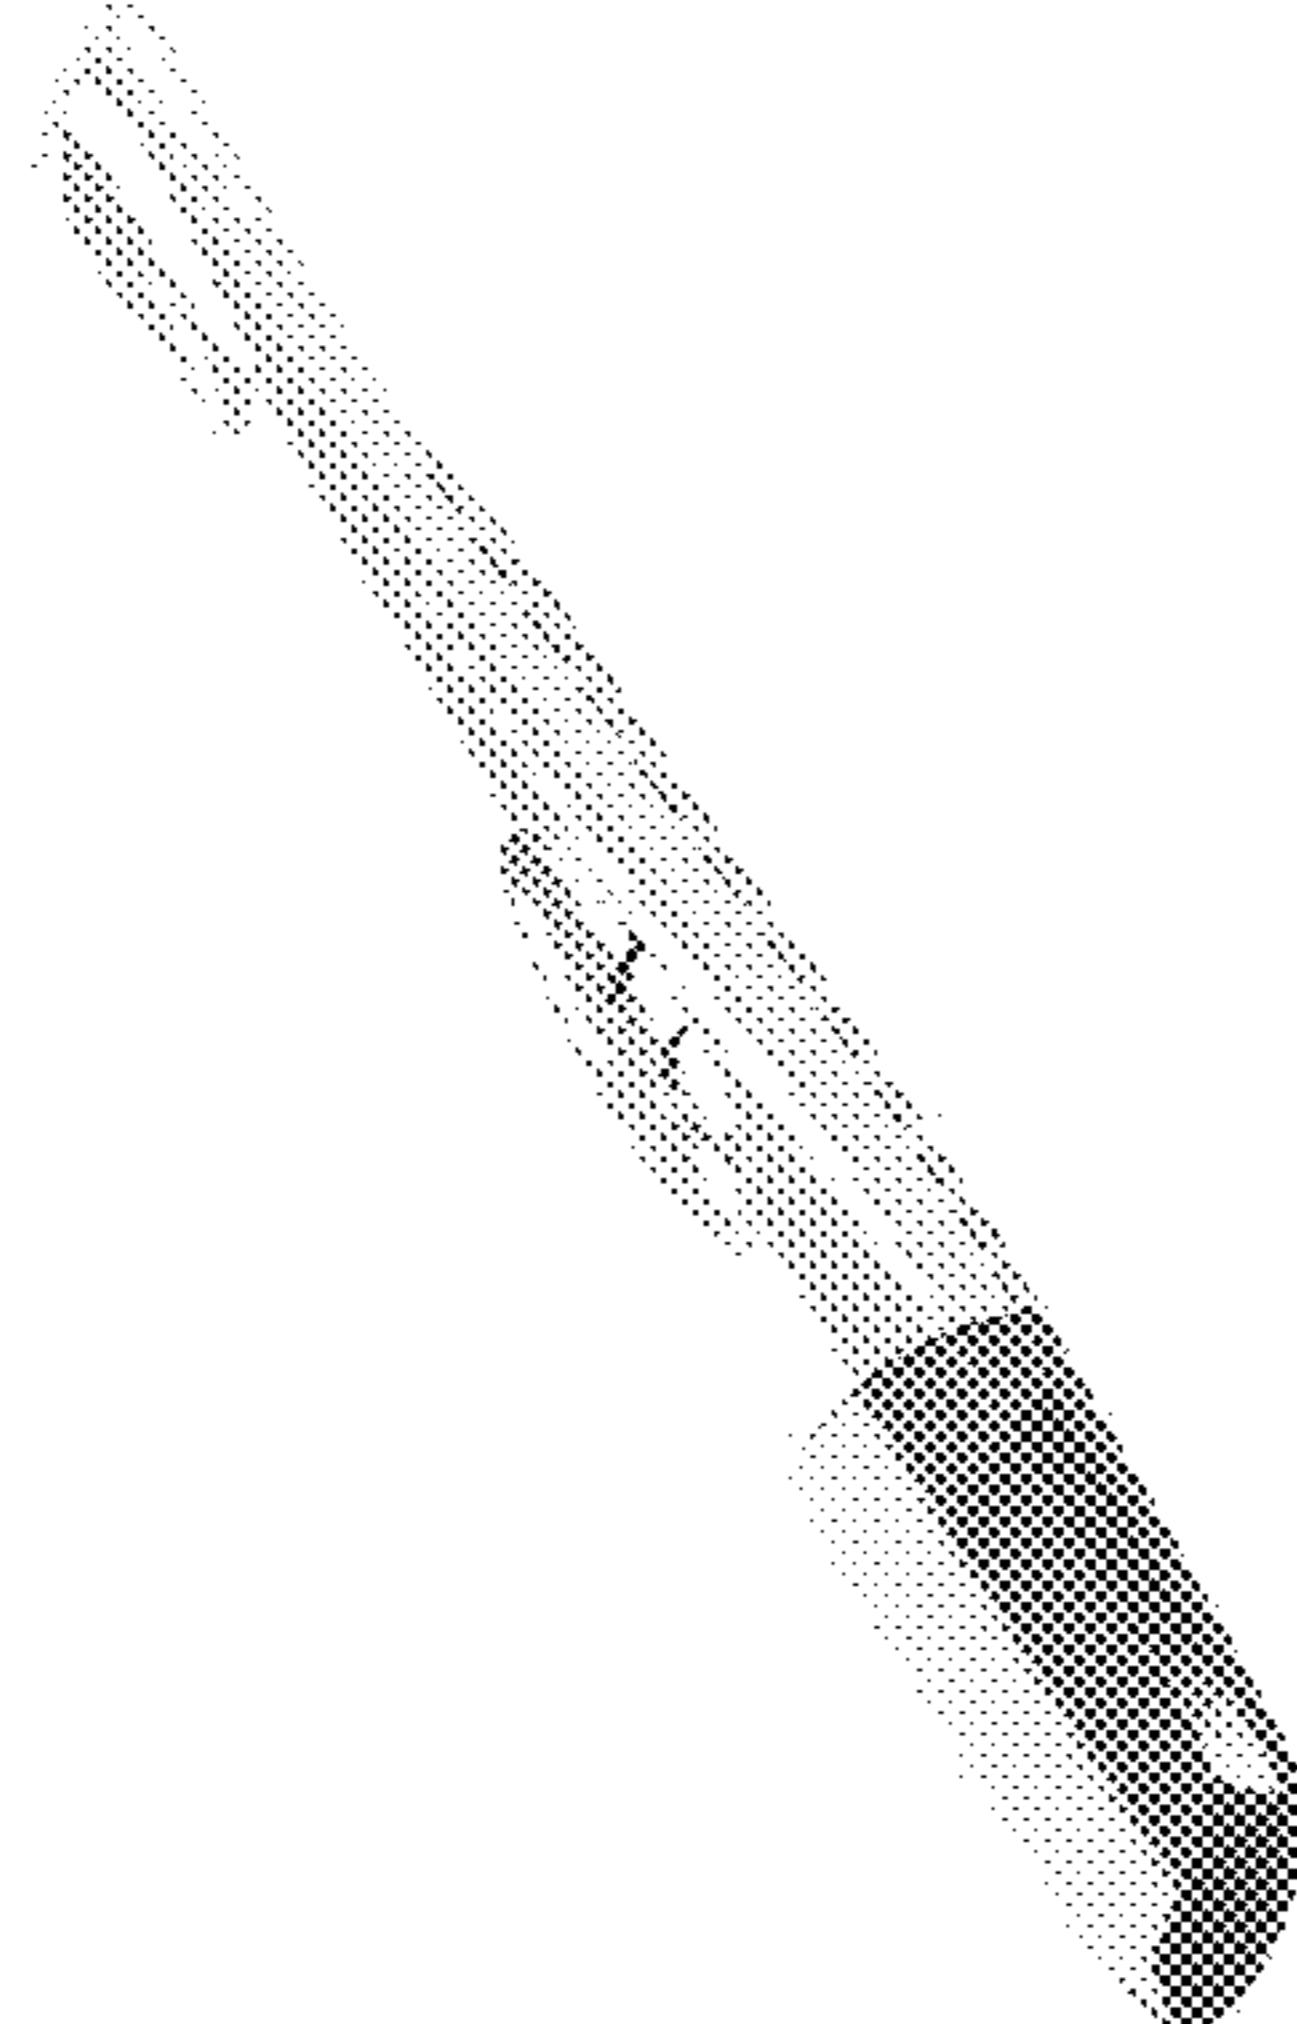

(58) **Field of Classification Search**

CPC ..... G01N 33/76; G01N 33/558; G01N  
33/54386; G01N 33/689

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D672,880	S	*	12/2012	Laverack .....	D24/223
D676,144	S	*	2/2013	Laverack .....	D24/223
D676,569	S	*	2/2013	Laverack .....	D24/223
D698,457	S	*	1/2014	Canova .....	D24/223
D698,937	S	*	2/2014	Laverack .....	D24/223
D735,351	S	*	7/2015	Laverack .....	D24/223
D875,965	S	*	2/2020	Gani .....	D24/223
2009/0061534	A1	*	3/2009	Sharrock .....	G01N 33/545 436/518
2012/0083047	A1	*	4/2012	Nazareth .....	G01N 33/54386 436/501


\* cited by examiner




**Fig. 1**




**Fig. 2**

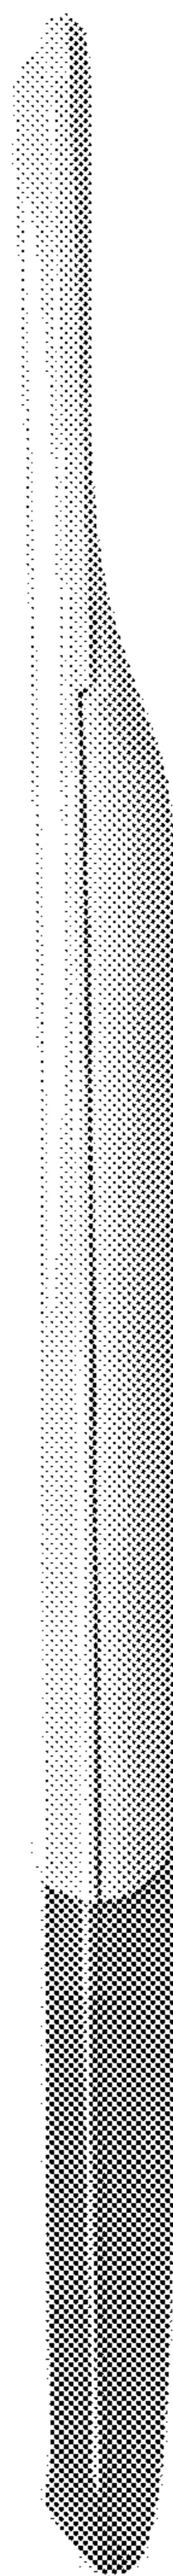


**Fig. 3**

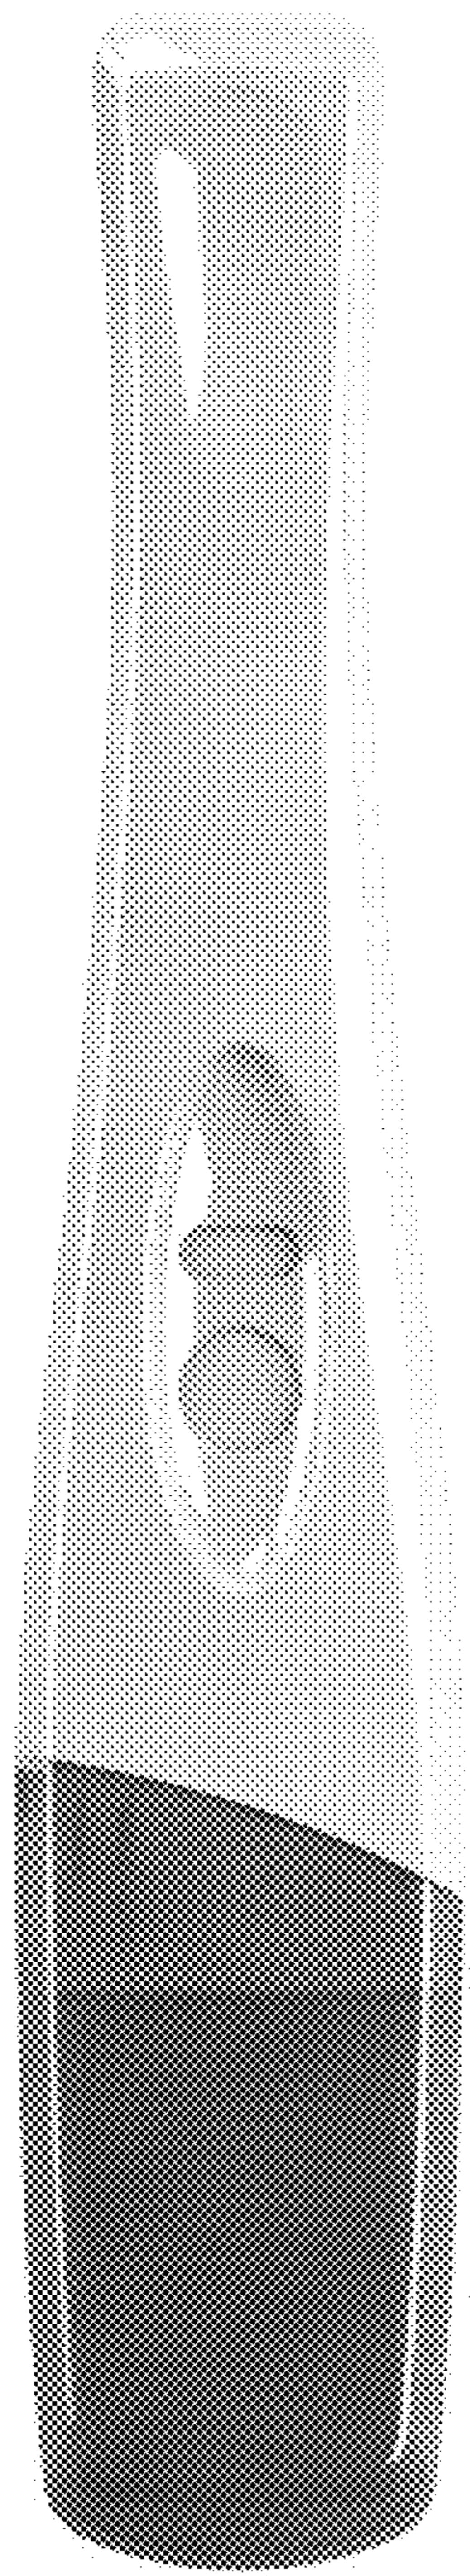


**Fig. 4**

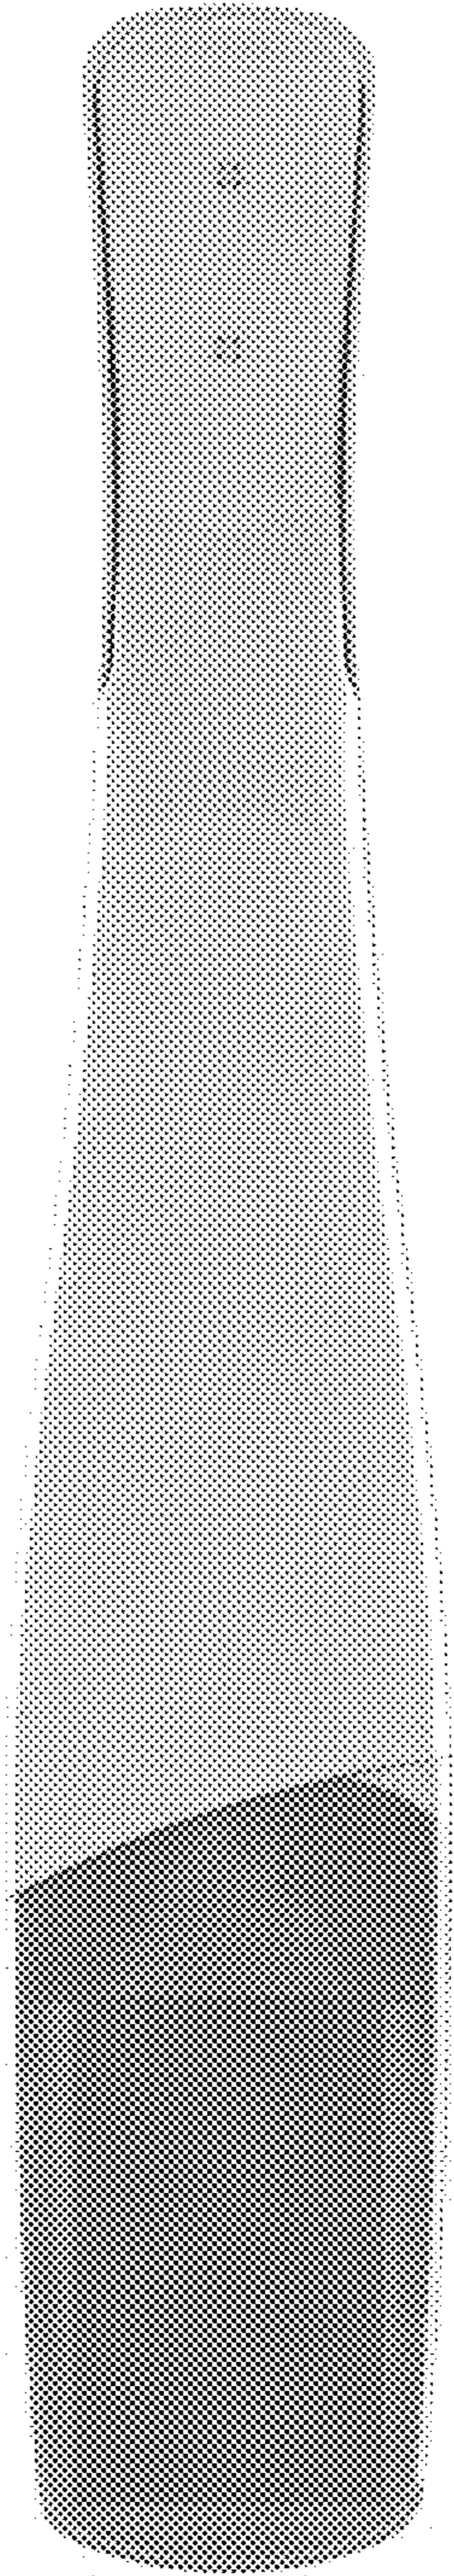

**Fig. 5**

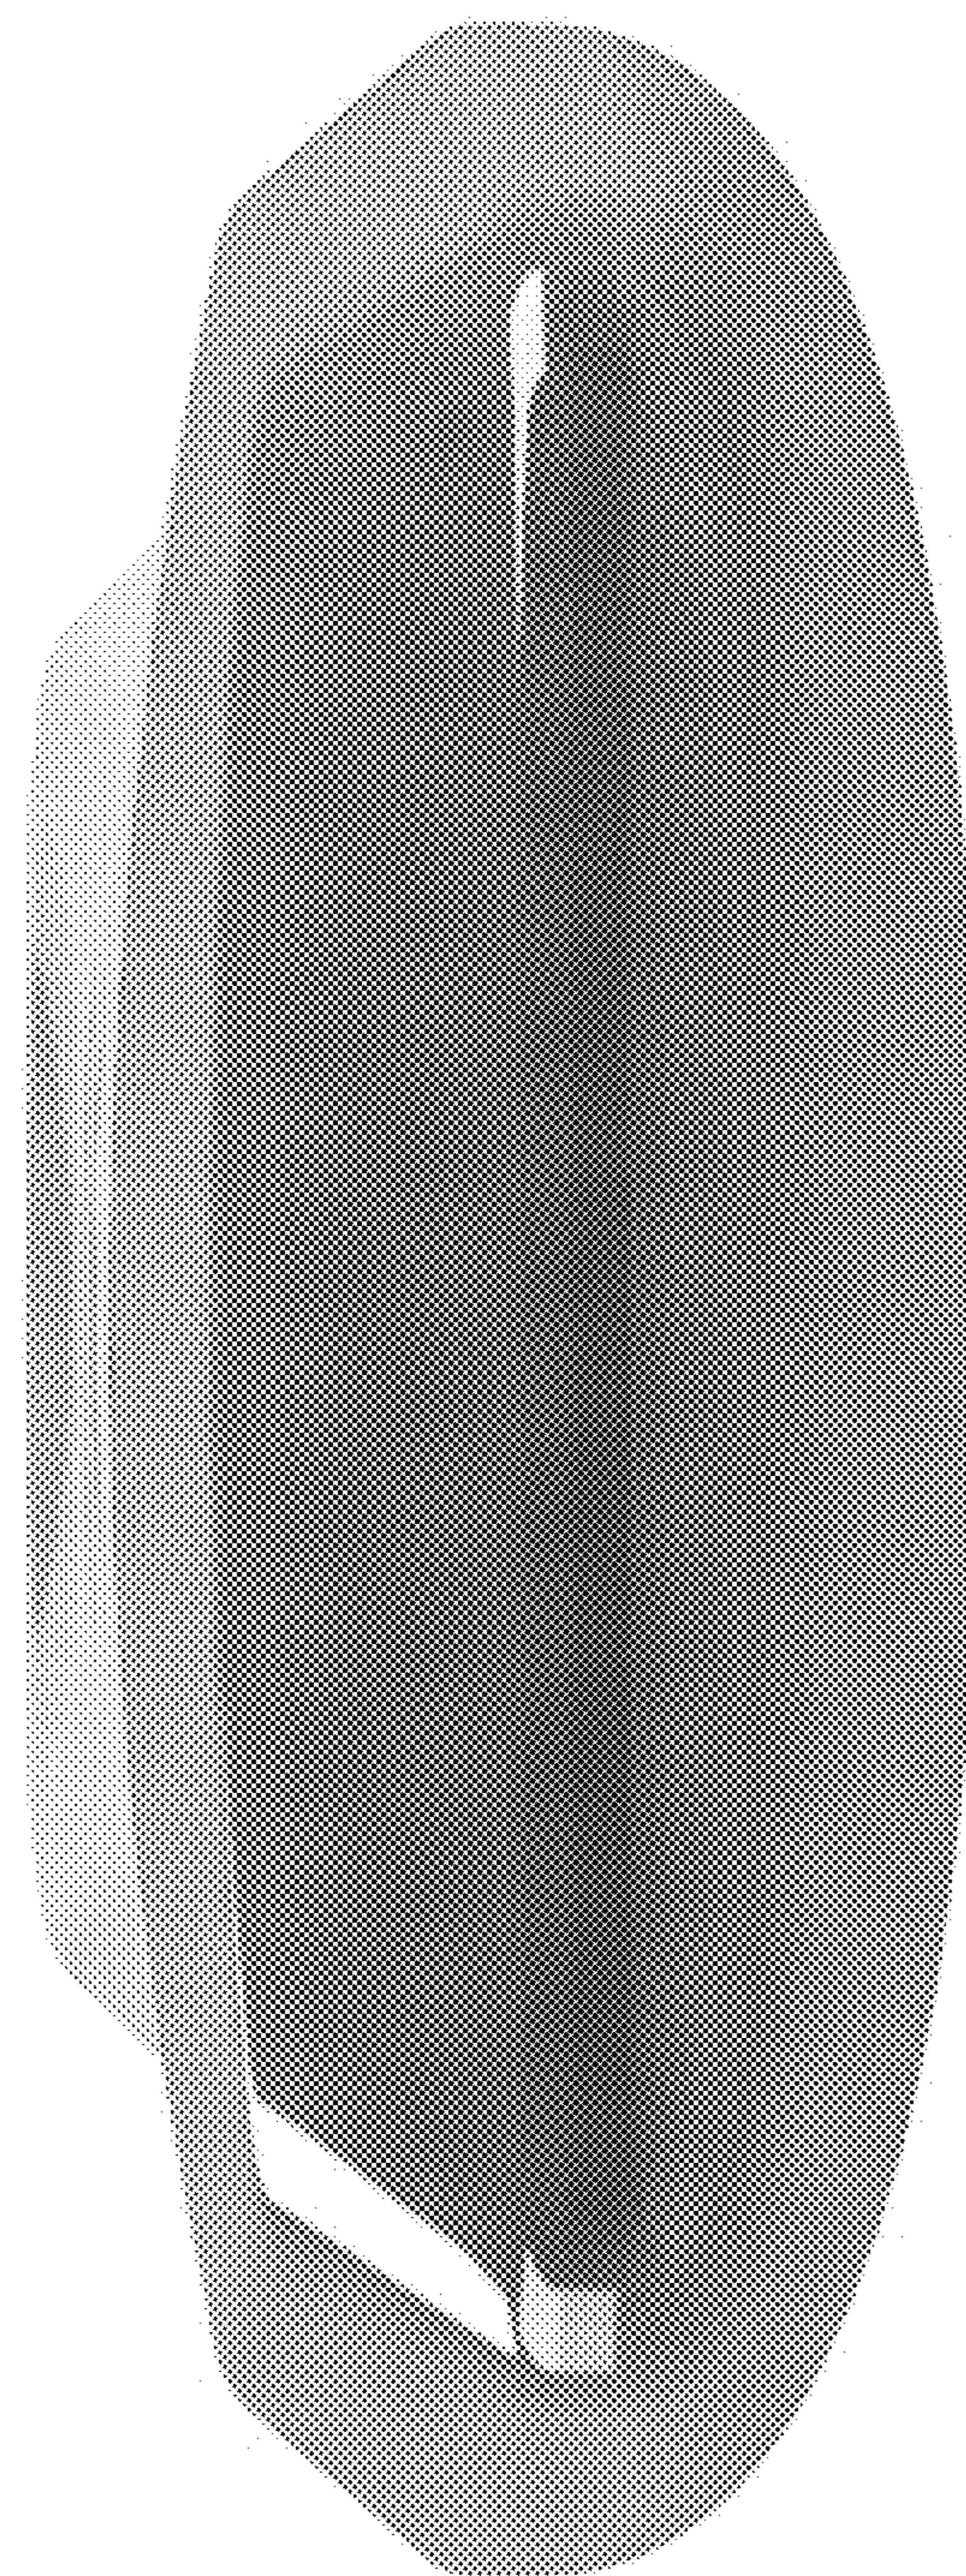

**Fig. 6**

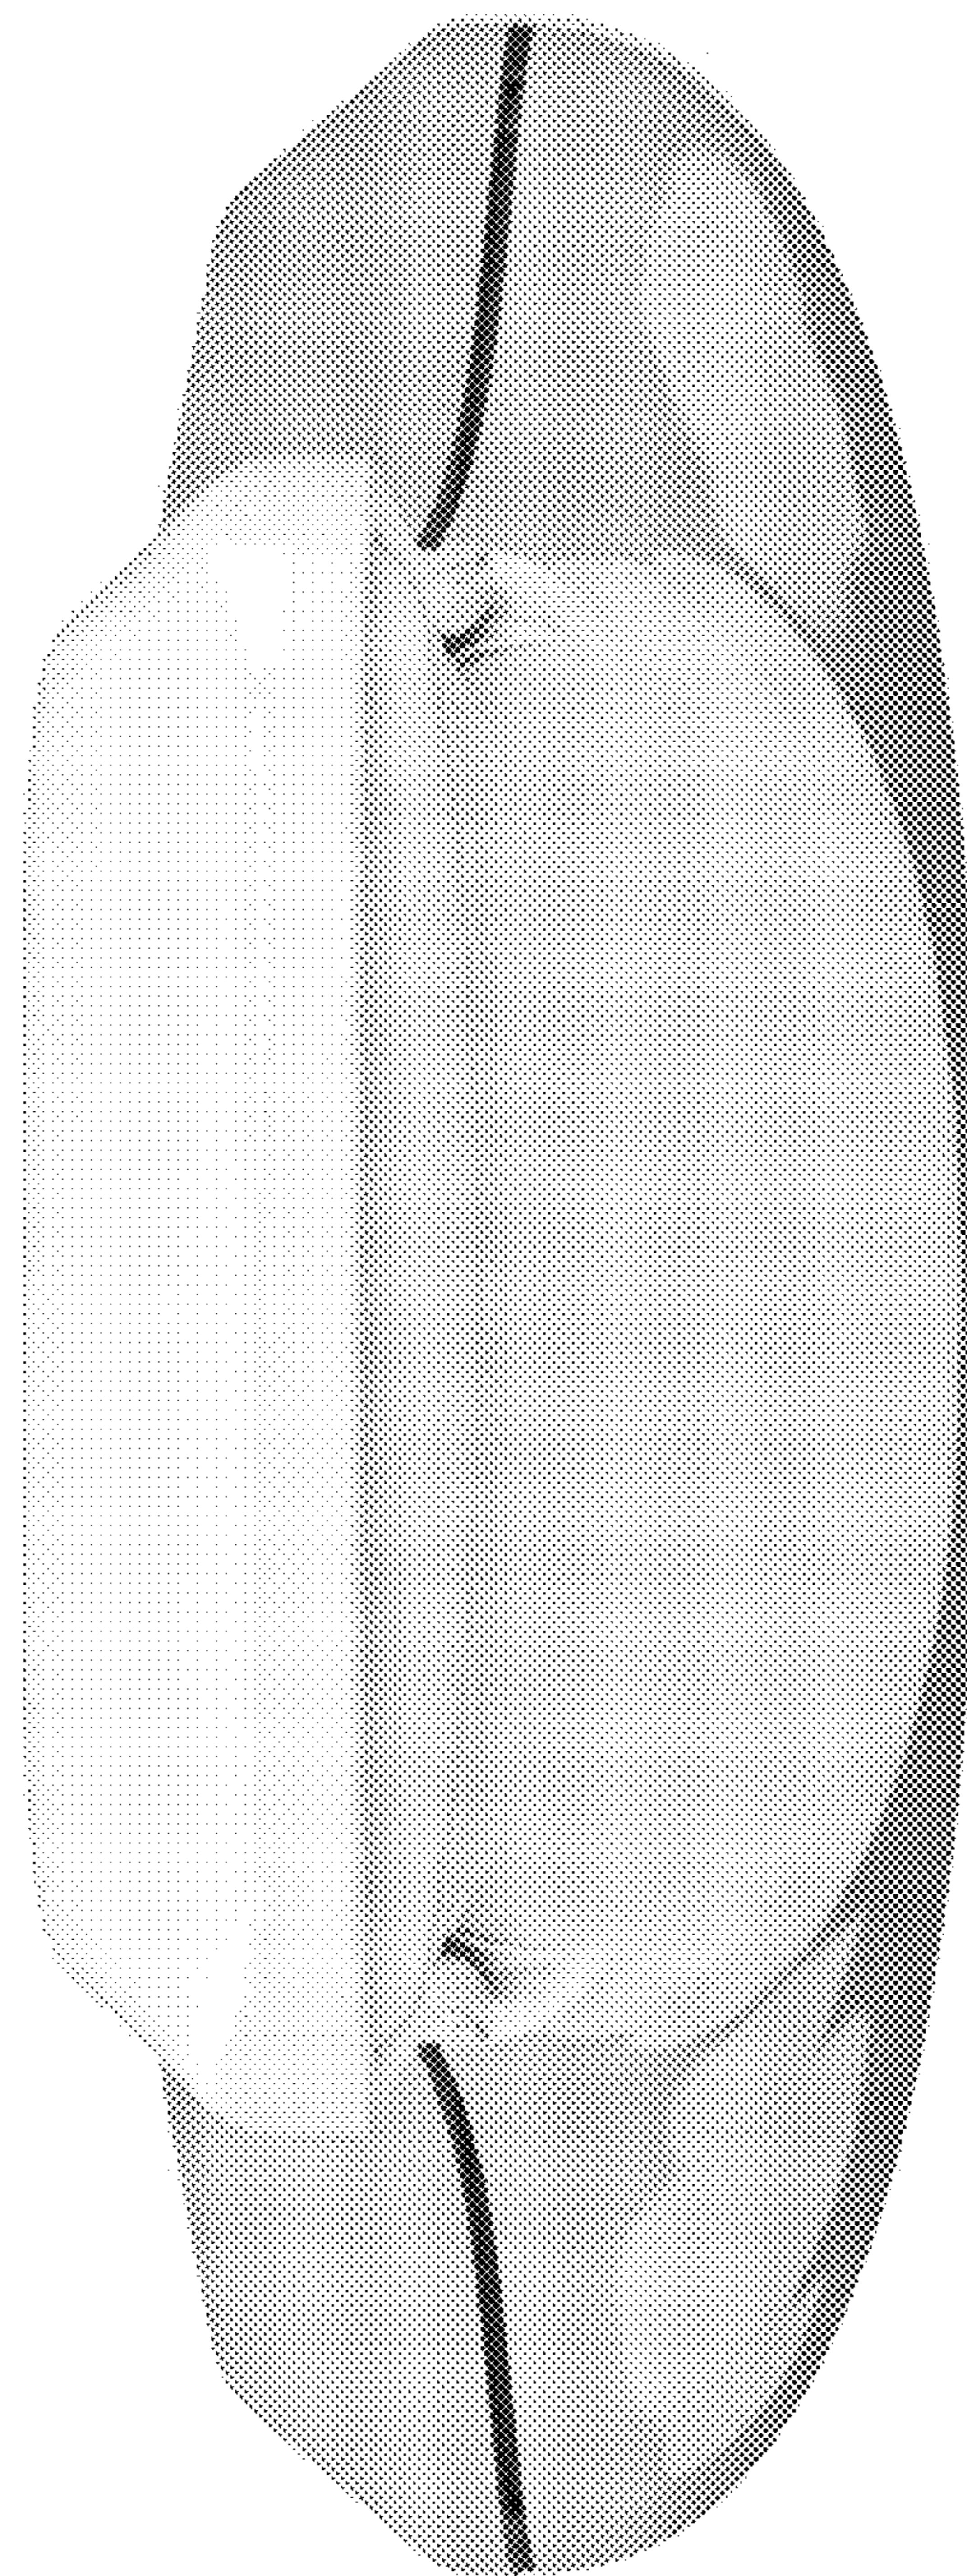


**Fig. 7**




**Fig. 8**




**Fig. 9**

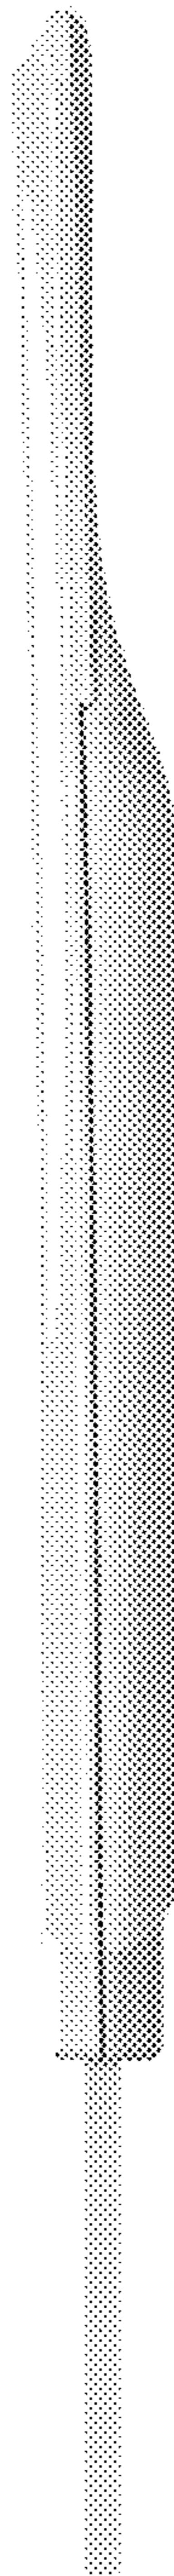


**Fig. 10**

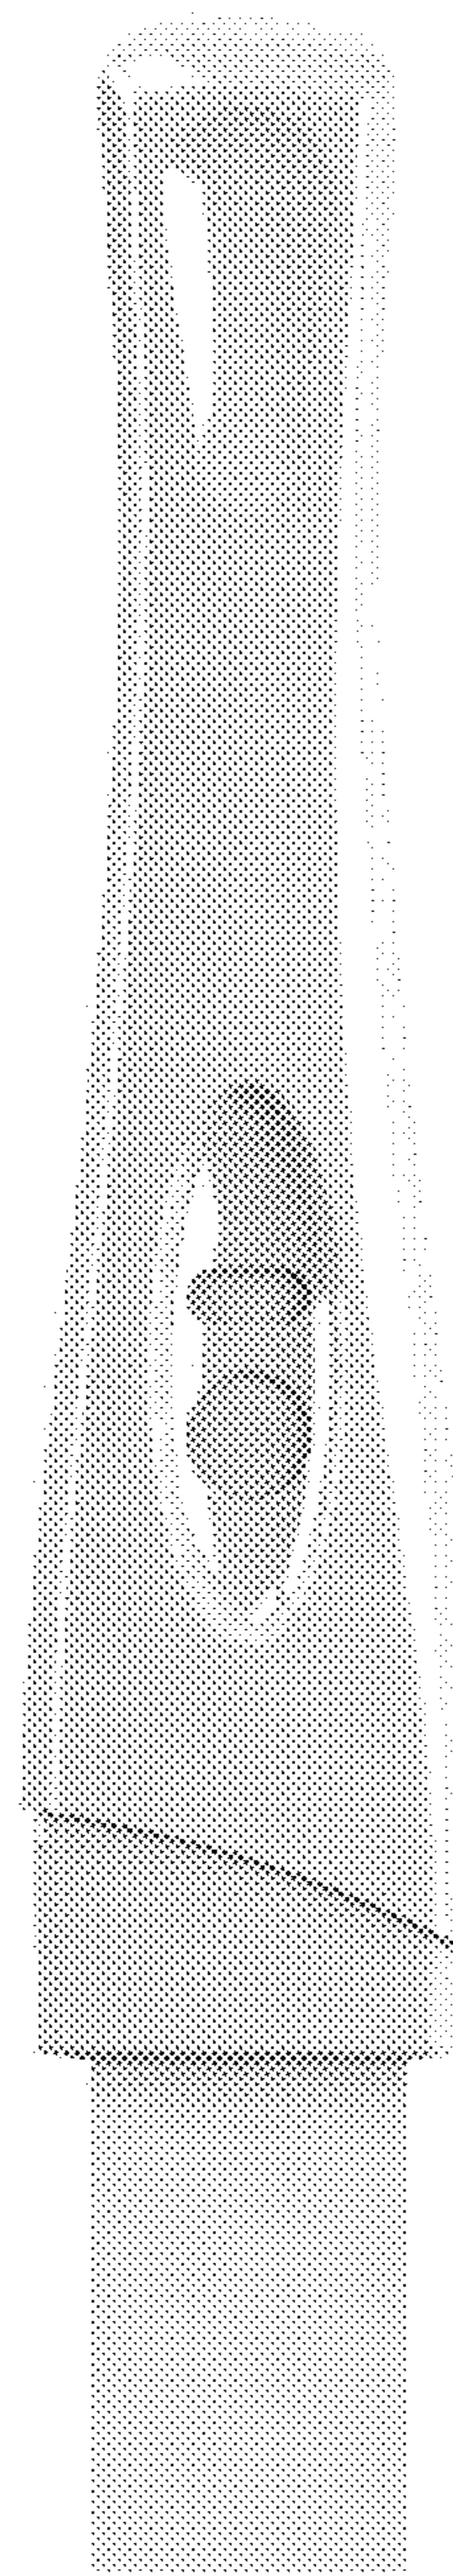


**Fig. 11**

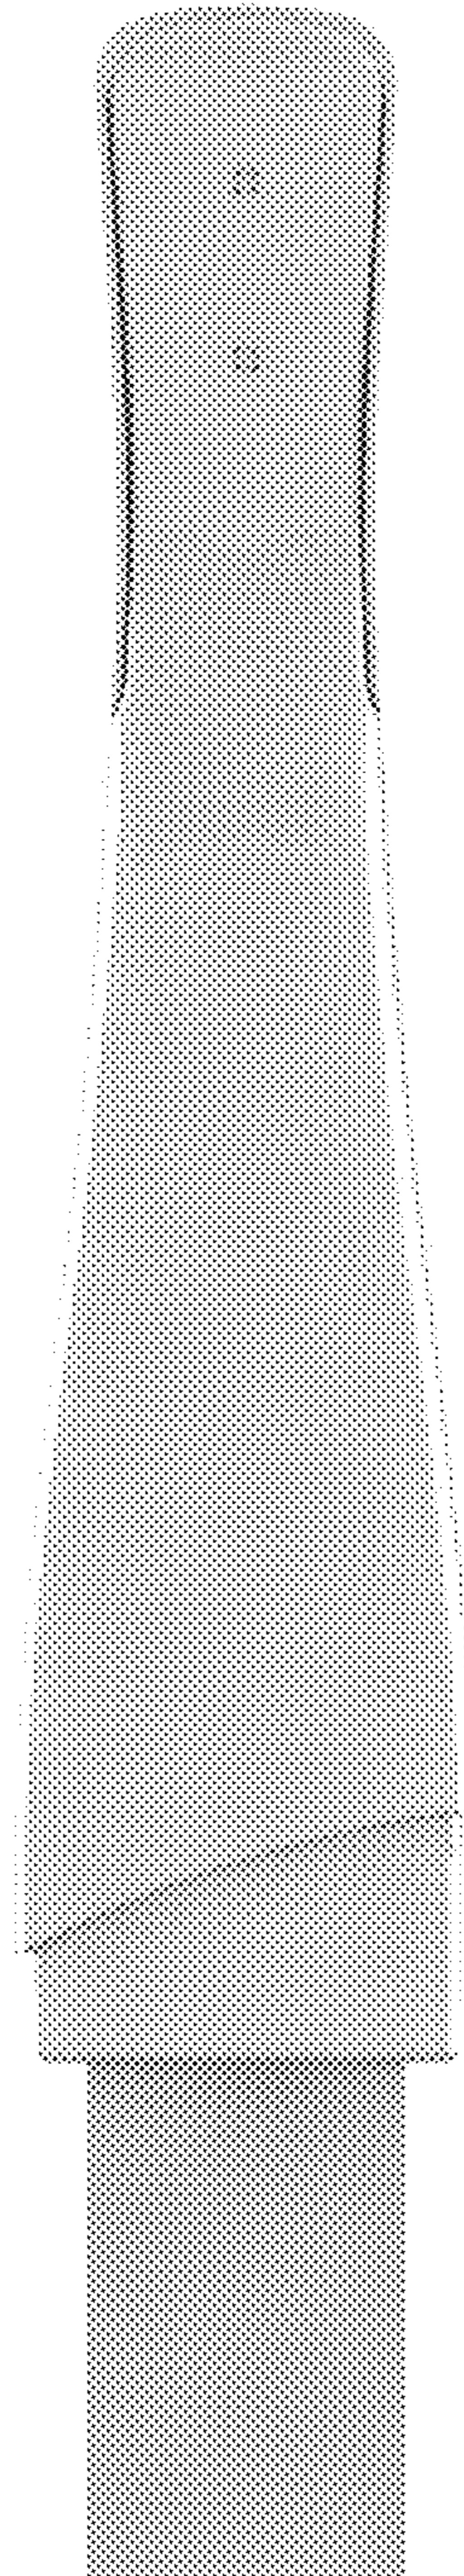

**Fig. 12**

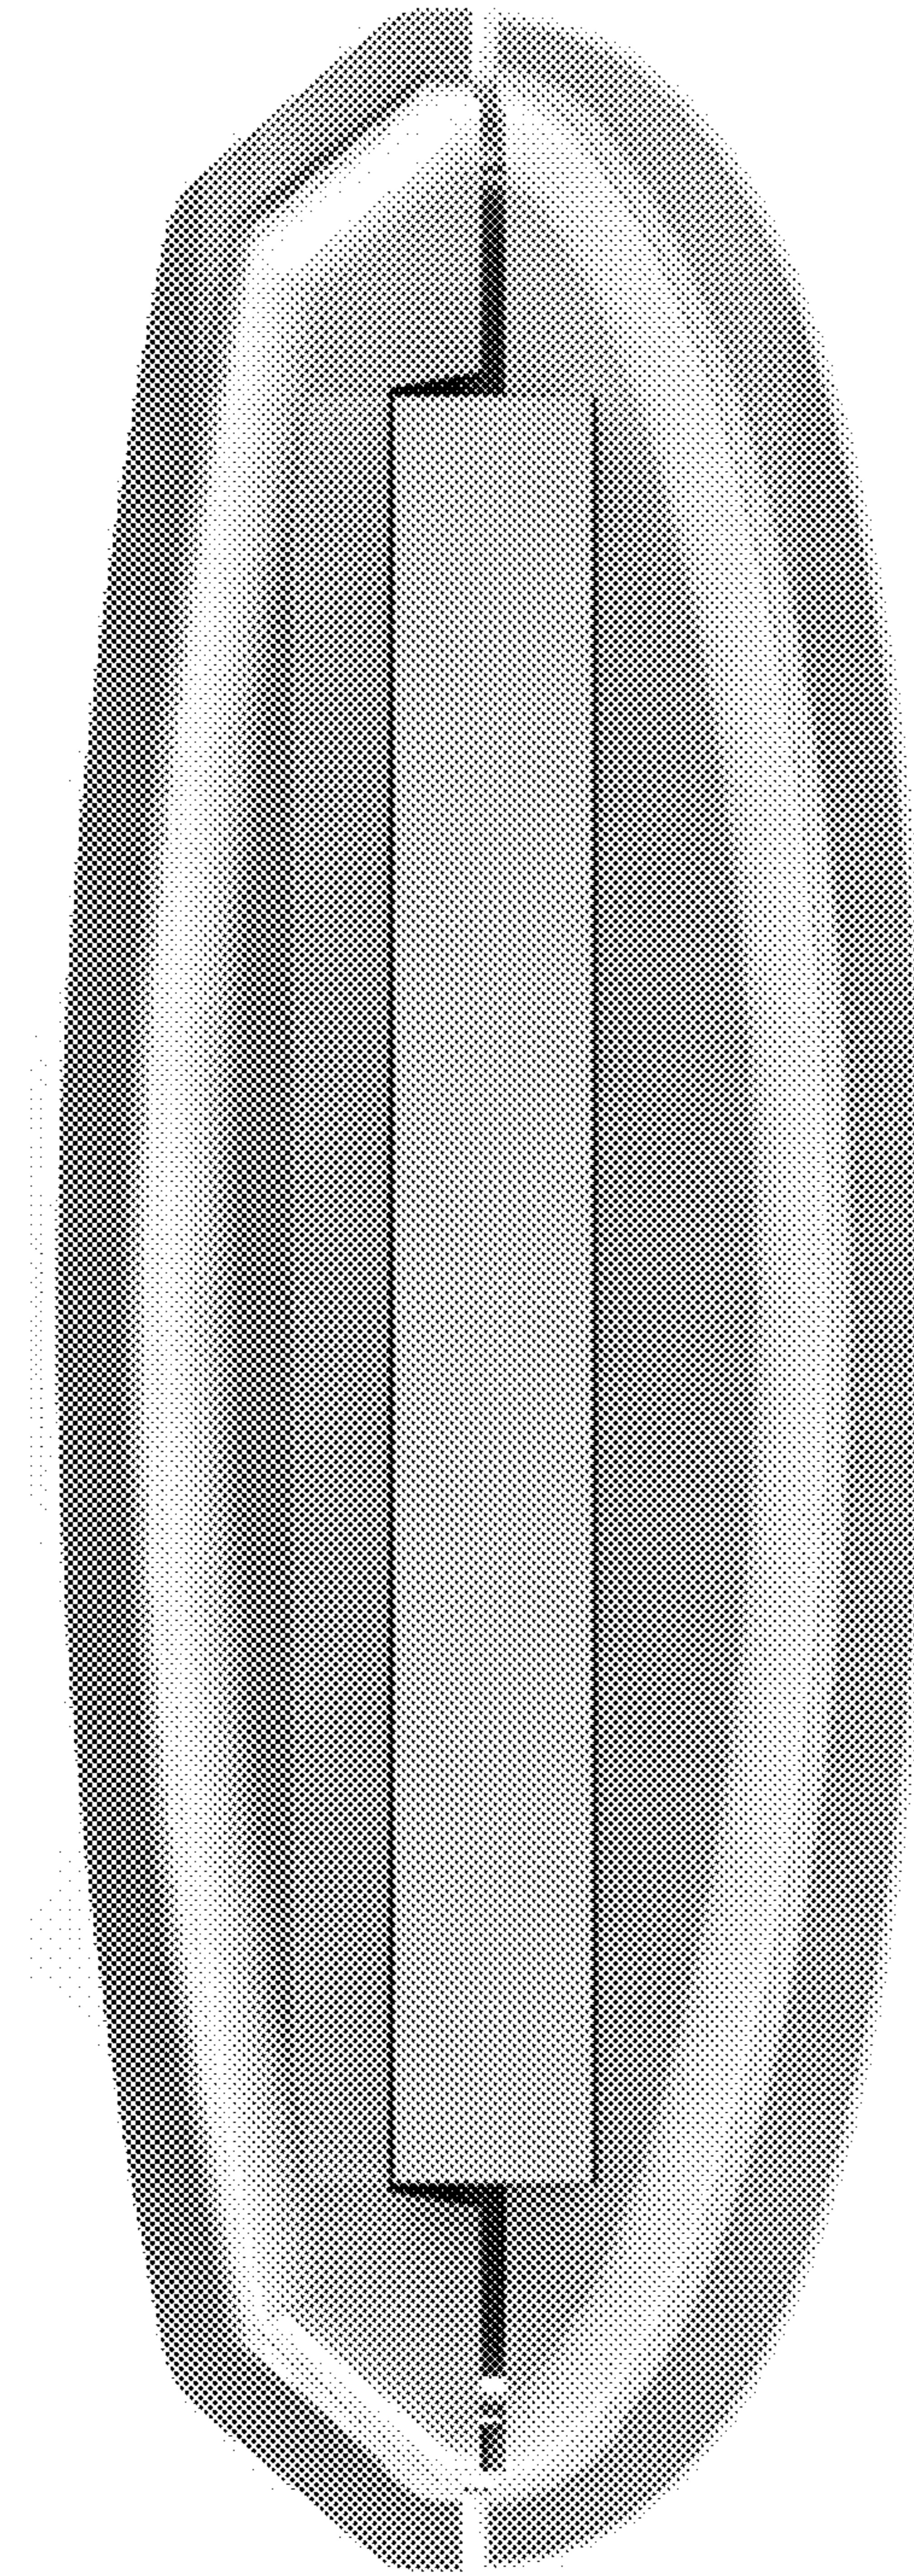

**Fig. 13**

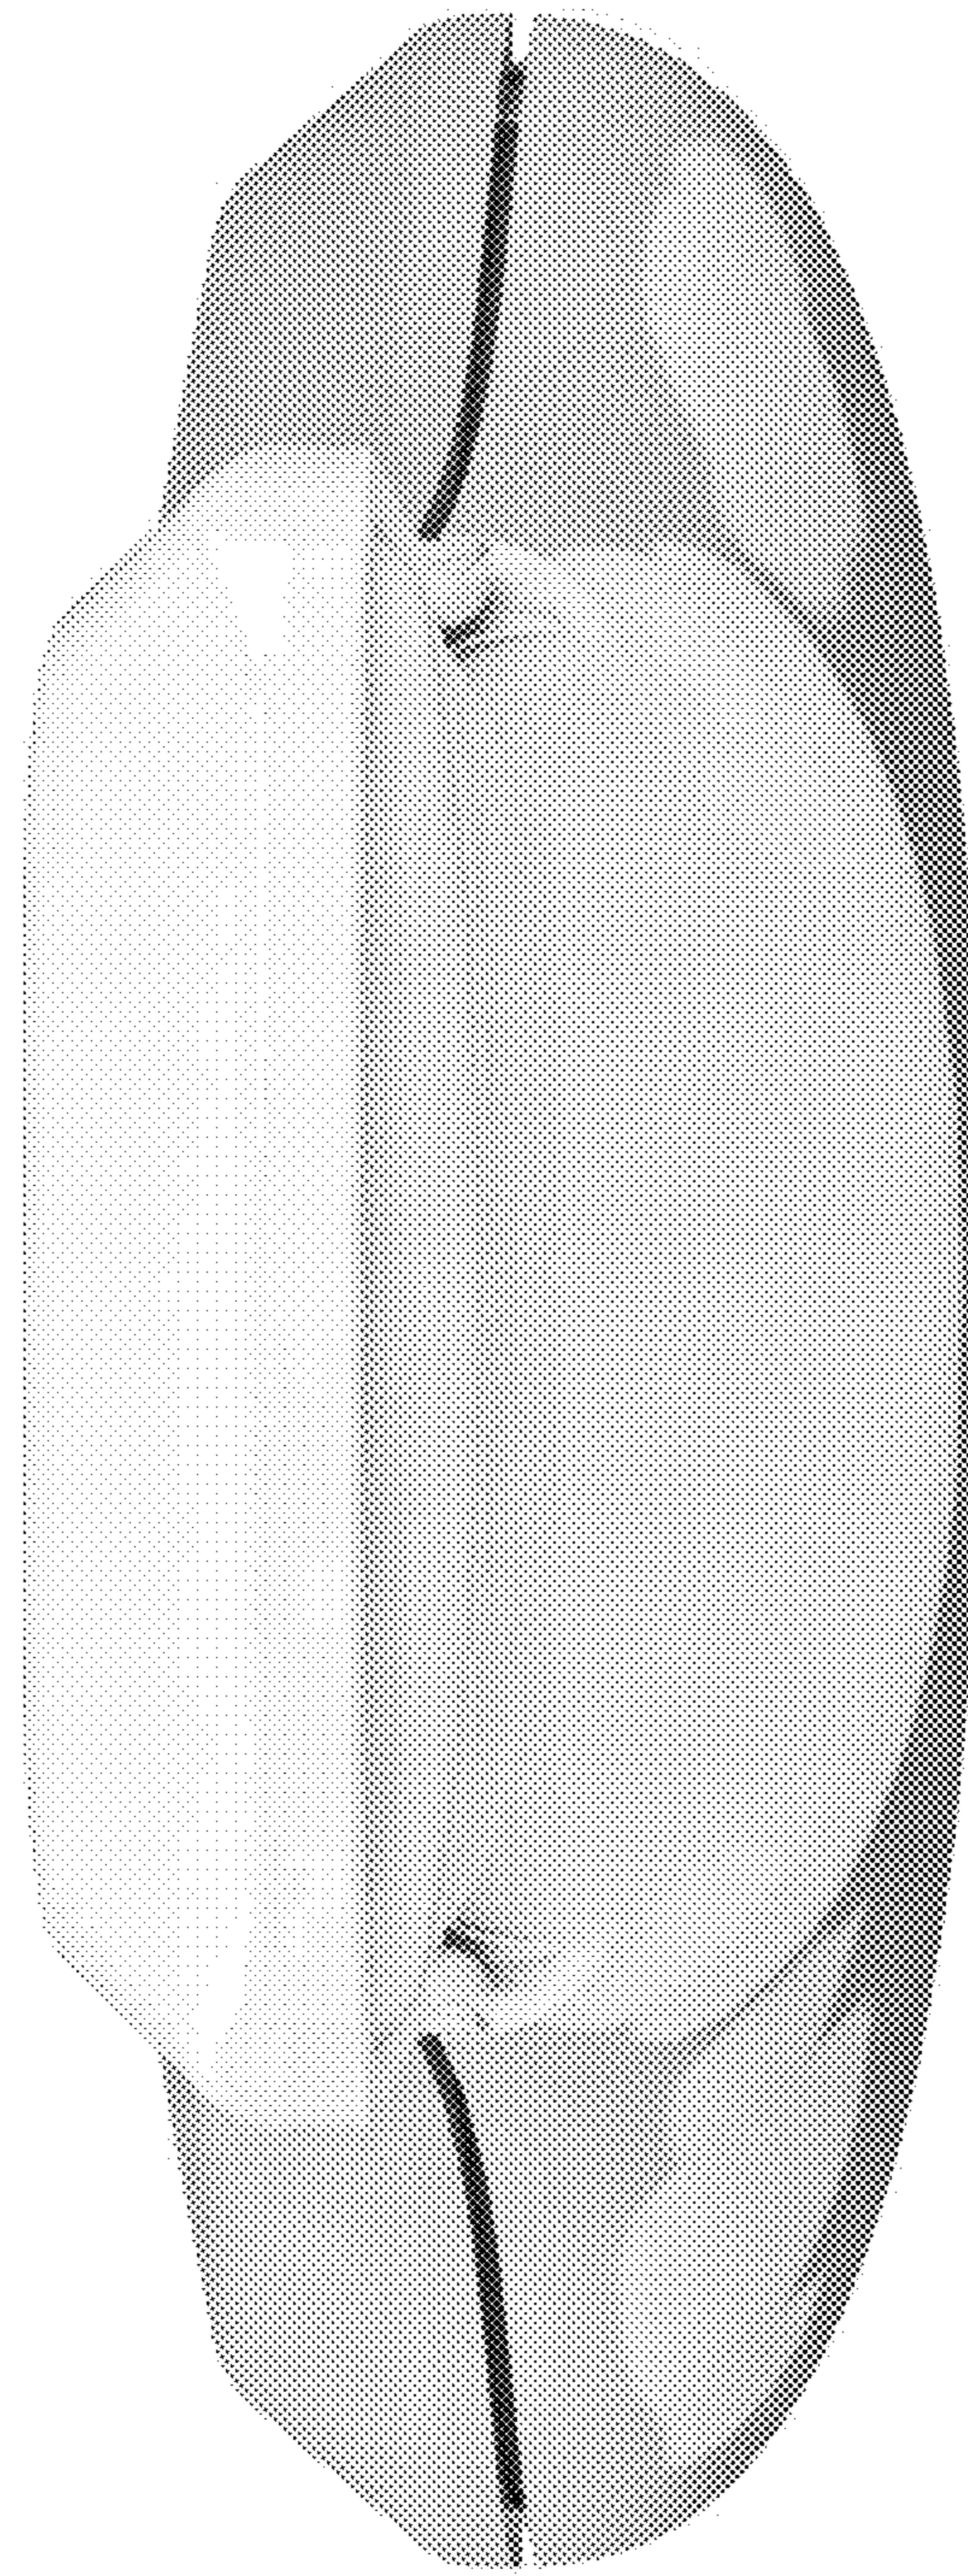

**Fig. 14**