



US00D955593S

(12) **United States Design Patent** (10) **Patent No.:** **US D955,593 S**  
**Bobey et al.** (45) **Date of Patent:** **\*\* Jun. 21, 2022**

(54) **REAR PORTION OF A PERCUSSIVE HIGH FREQUENCY CHEST WALL OSCILLATION SYSTEM**

23/02; A61H 23/0218; A61H 23/04; A61H 2023/045; A41D 13/0518

See application file for complete search history.

(71) Applicant: **HILL-ROM SERVICES PTE. LTD.**, Singapore (SG)

(56) **References Cited**

U.S. PATENT DOCUMENTS

(72) Inventors: **John A. Bobey**, Daniel Island, SC (US); **Harold M. Cabral**, Singapore (SG); **Deny D. Barilea**, Singapore (SG); **Suresha Venkataraya**, Singapore (SG); **Wei T. Tan**, Singapore (SG); **Clementine Pirio**, Vannes (FR); **Dirk Tjepkema**, Enschede (NL); **Sytze A. Spijksma**, Haaksbergen (NL); **Petrus J. van den Oever**, Rosmalen (NL)

2,869,537 A 1/1959 Chu  
3,053,250 A 9/1962 Stubbs  
(Continued)

OTHER PUBLICATIONS

Hodsden, Suzanne, "Hill-Rom Unveils Mobile, Connected Airway Clearance System for Patients on the Move" May 2, 2017, [online], [site visited Jun. 14, 2018]. Retrieved from Internet: <URL: https://www.meddeviceonline.com/doc/hill-rom-unveils-mobile-connected-airway-clearance-system-for-patients-on-the-move-0001>.

(Continued)

(73) Assignee: **HILL-ROM SERVICES PTE. LTD.**, Singapore (SG)

*Primary Examiner* — Wan Laymon

(\*\*) Term: **15 Years**

(74) *Attorney, Agent, or Firm* — Barnes & Thornburg LLP

(21) Appl. No.: **29/809,250**

(22) Filed: **Sep. 27, 2021**

**Related U.S. Application Data**

(62) Division of application No. 29/751,117, filed on Sep. 18, 2020, now Pat. No. Des. 933,841, which is a division of application No. 29/724,357, filed on Feb. 14, 2020, now Pat. No. Des. 898,926, which is a division of application No. 29/679,143, filed on Feb. 1, 2019, now Pat. No. Des. 879,982, which is a

(Continued)

(51) **LOC (13) Cl.** ..... **28-03**

(52) **U.S. Cl.**  
USPC ..... **D24/200**

(58) **Field of Classification Search**  
USPC ..... D24/200, 107, 164; D2/828-829  
CPC ..... A61H 9/00; A61H 9/005; A61H 9/0007; A61H 9/0071; A61H 9/0078; A61H 7/004; A61H 23/00; A61H 23/006; A61H


(57) **CLAIM**

The ornamental design for a rear portion of a percussive high frequency chest wall oscillation system, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a rear portion of a percussive high frequency chest wall oscillation system in accordance with the present design; FIG. 2 is a front elevation view thereof; FIG. 3 is a rear elevation view thereof; FIG. 4 is a right side elevation view thereof; FIG. 5 is left side elevation view thereof; FIG. 6 is a top plan view thereof; and, FIG. 7 is a bottom plan view thereof.

(Continued)

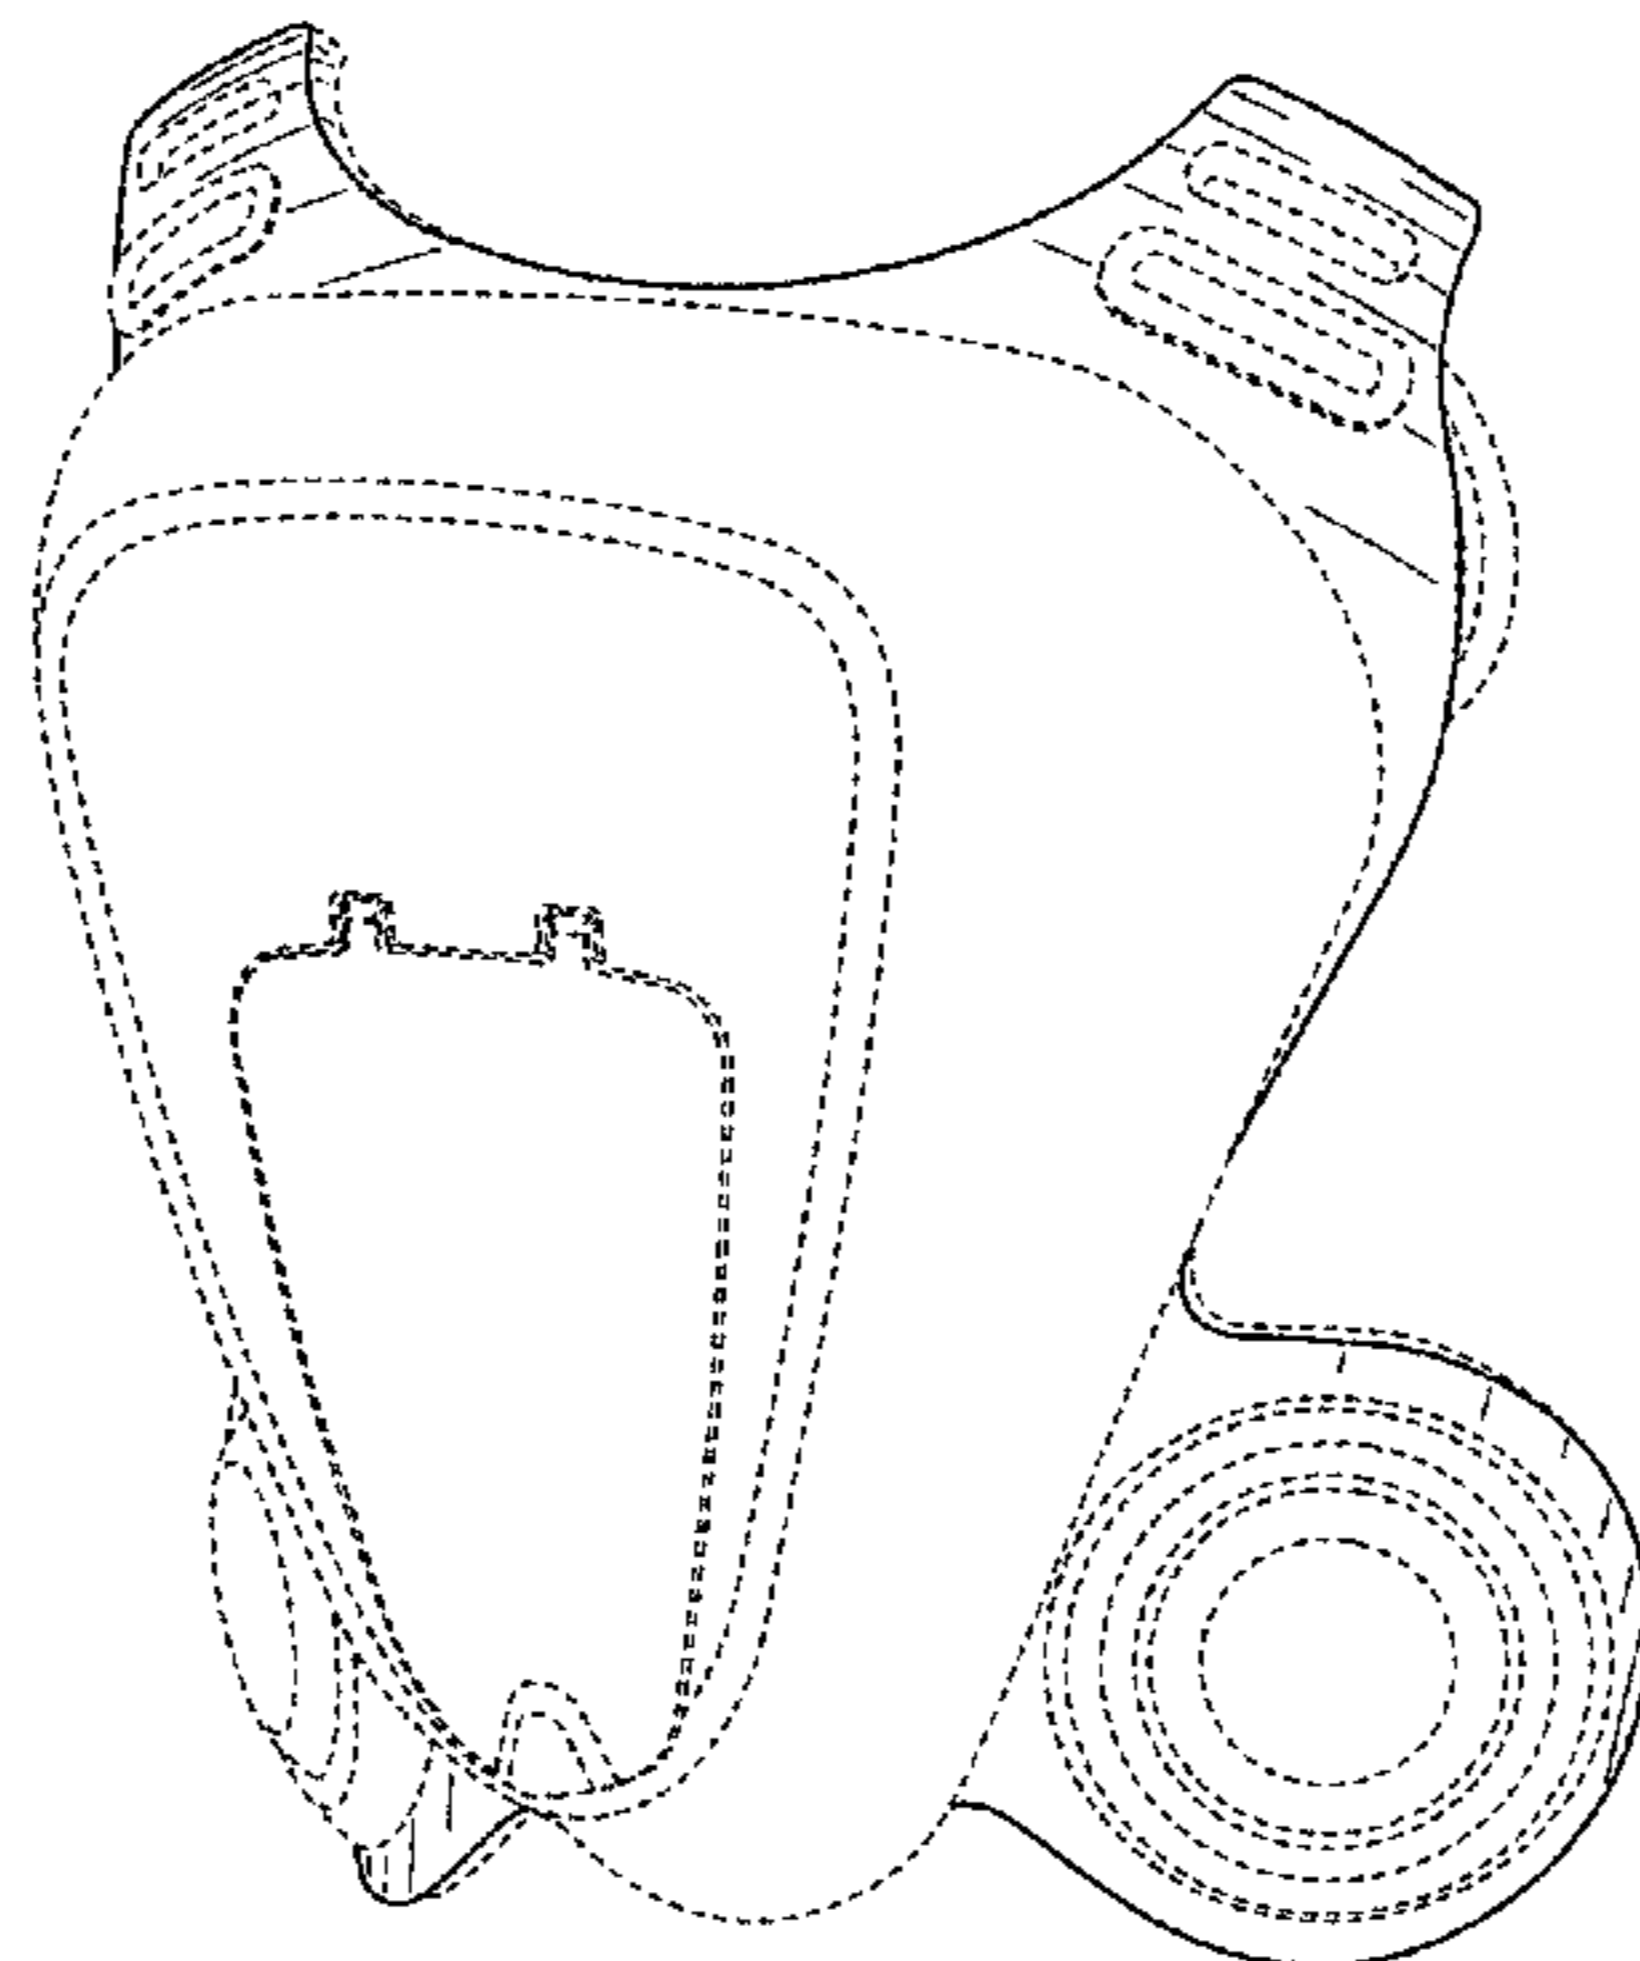

The broken lines depict portions of the rear portion of the percussive high frequency chest wall oscillation system and form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

**Related U.S. Application Data**

division of application No. 29/594,771, filed on Feb. 22, 2017, now Pat. No. Des. 852,969.

(56)

**References Cited**

U.S. PATENT DOCUMENTS


5,235,967	A	8/1993	Arbisi et al.
D456,591	S	5/2002	Hansen
D461,897	S	8/2002	Hansen et al.
D469,876	S	2/2003	Hansen et al.
D478,989	S	8/2003	Hansen et al.
D495,804	S	9/2004	Nan
6,958,047	B2	10/2005	DeVlieger
7,115,104	B2	10/2006	Van Brunt et al.
7,931,607	B2	4/2011	Biondo et al.
D639,954	S	6/2011	Helgeson et al.
8,460,223	B2	6/2013	Huster et al.
D704,849	S	5/2014	Hunter
9,237,982	B2 *	1/2016	Van Brunt ..... A61H 9/0078
9,549,869	B2	1/2017	DeVlieger et al.
9,744,097	B2	8/2017	DeVlieger et al.

9,895,287	B2	2/2018	Shockley, Jr. et al.
9,907,725	B2	3/2018	Shockley, Jr. et al.
9,968,511	B2	5/2018	Huster et al.
D834,718	S	11/2018	Bobey et al.
10,251,810	B2	4/2019	Shockley, Jr. et al.
D852,969	S	7/2019	Bobey et al.
D879,982	S	3/2020	Bobey et al.
D898,926	S	10/2020	Bobey et al.
D933,841	S	10/2021	Bobey et al.
2004/0133133	A1	7/2004	Dreimann et al.
2006/0005306	A1	1/2006	Call et al.
2008/0108914	A1	5/2008	Brouqueyre et al.
2008/0188834	A1	8/2008	Balducci
2009/0192421	A1	7/2009	Huster et al.
2011/0087143	A1	4/2011	Bobey et al.
2012/0291798	A1	11/2012	Park et al.
2013/0289456	A1	10/2013	Chang Guo et al.
2014/0005579	A1	1/2014	Drlik et al.
2014/0276271	A1	9/2014	Stryker et al.
2016/0095790	A1	4/2016	Shockley, Jr. et al.
2018/0049939	A1	2/2018	Bobey et al.
2018/0228687	A1	8/2018	Huster et al.
2019/0105225	A1	4/2019	Brenner et al.


OTHER PUBLICATIONS

Hill-Rom | Respiratory Care | Monarch™ Airway Clearance System 3D Animation Video, published on Jun. 26, 2017, [online], [site visited Jun. 14, 2018]. Retrieved from Internet: <URL: [https://www.youtube.com/results?search\\_query=monarch+airway+clearance+system](https://www.youtube.com/results?search_query=monarch+airway+clearance+system)>.


\* cited by examiner

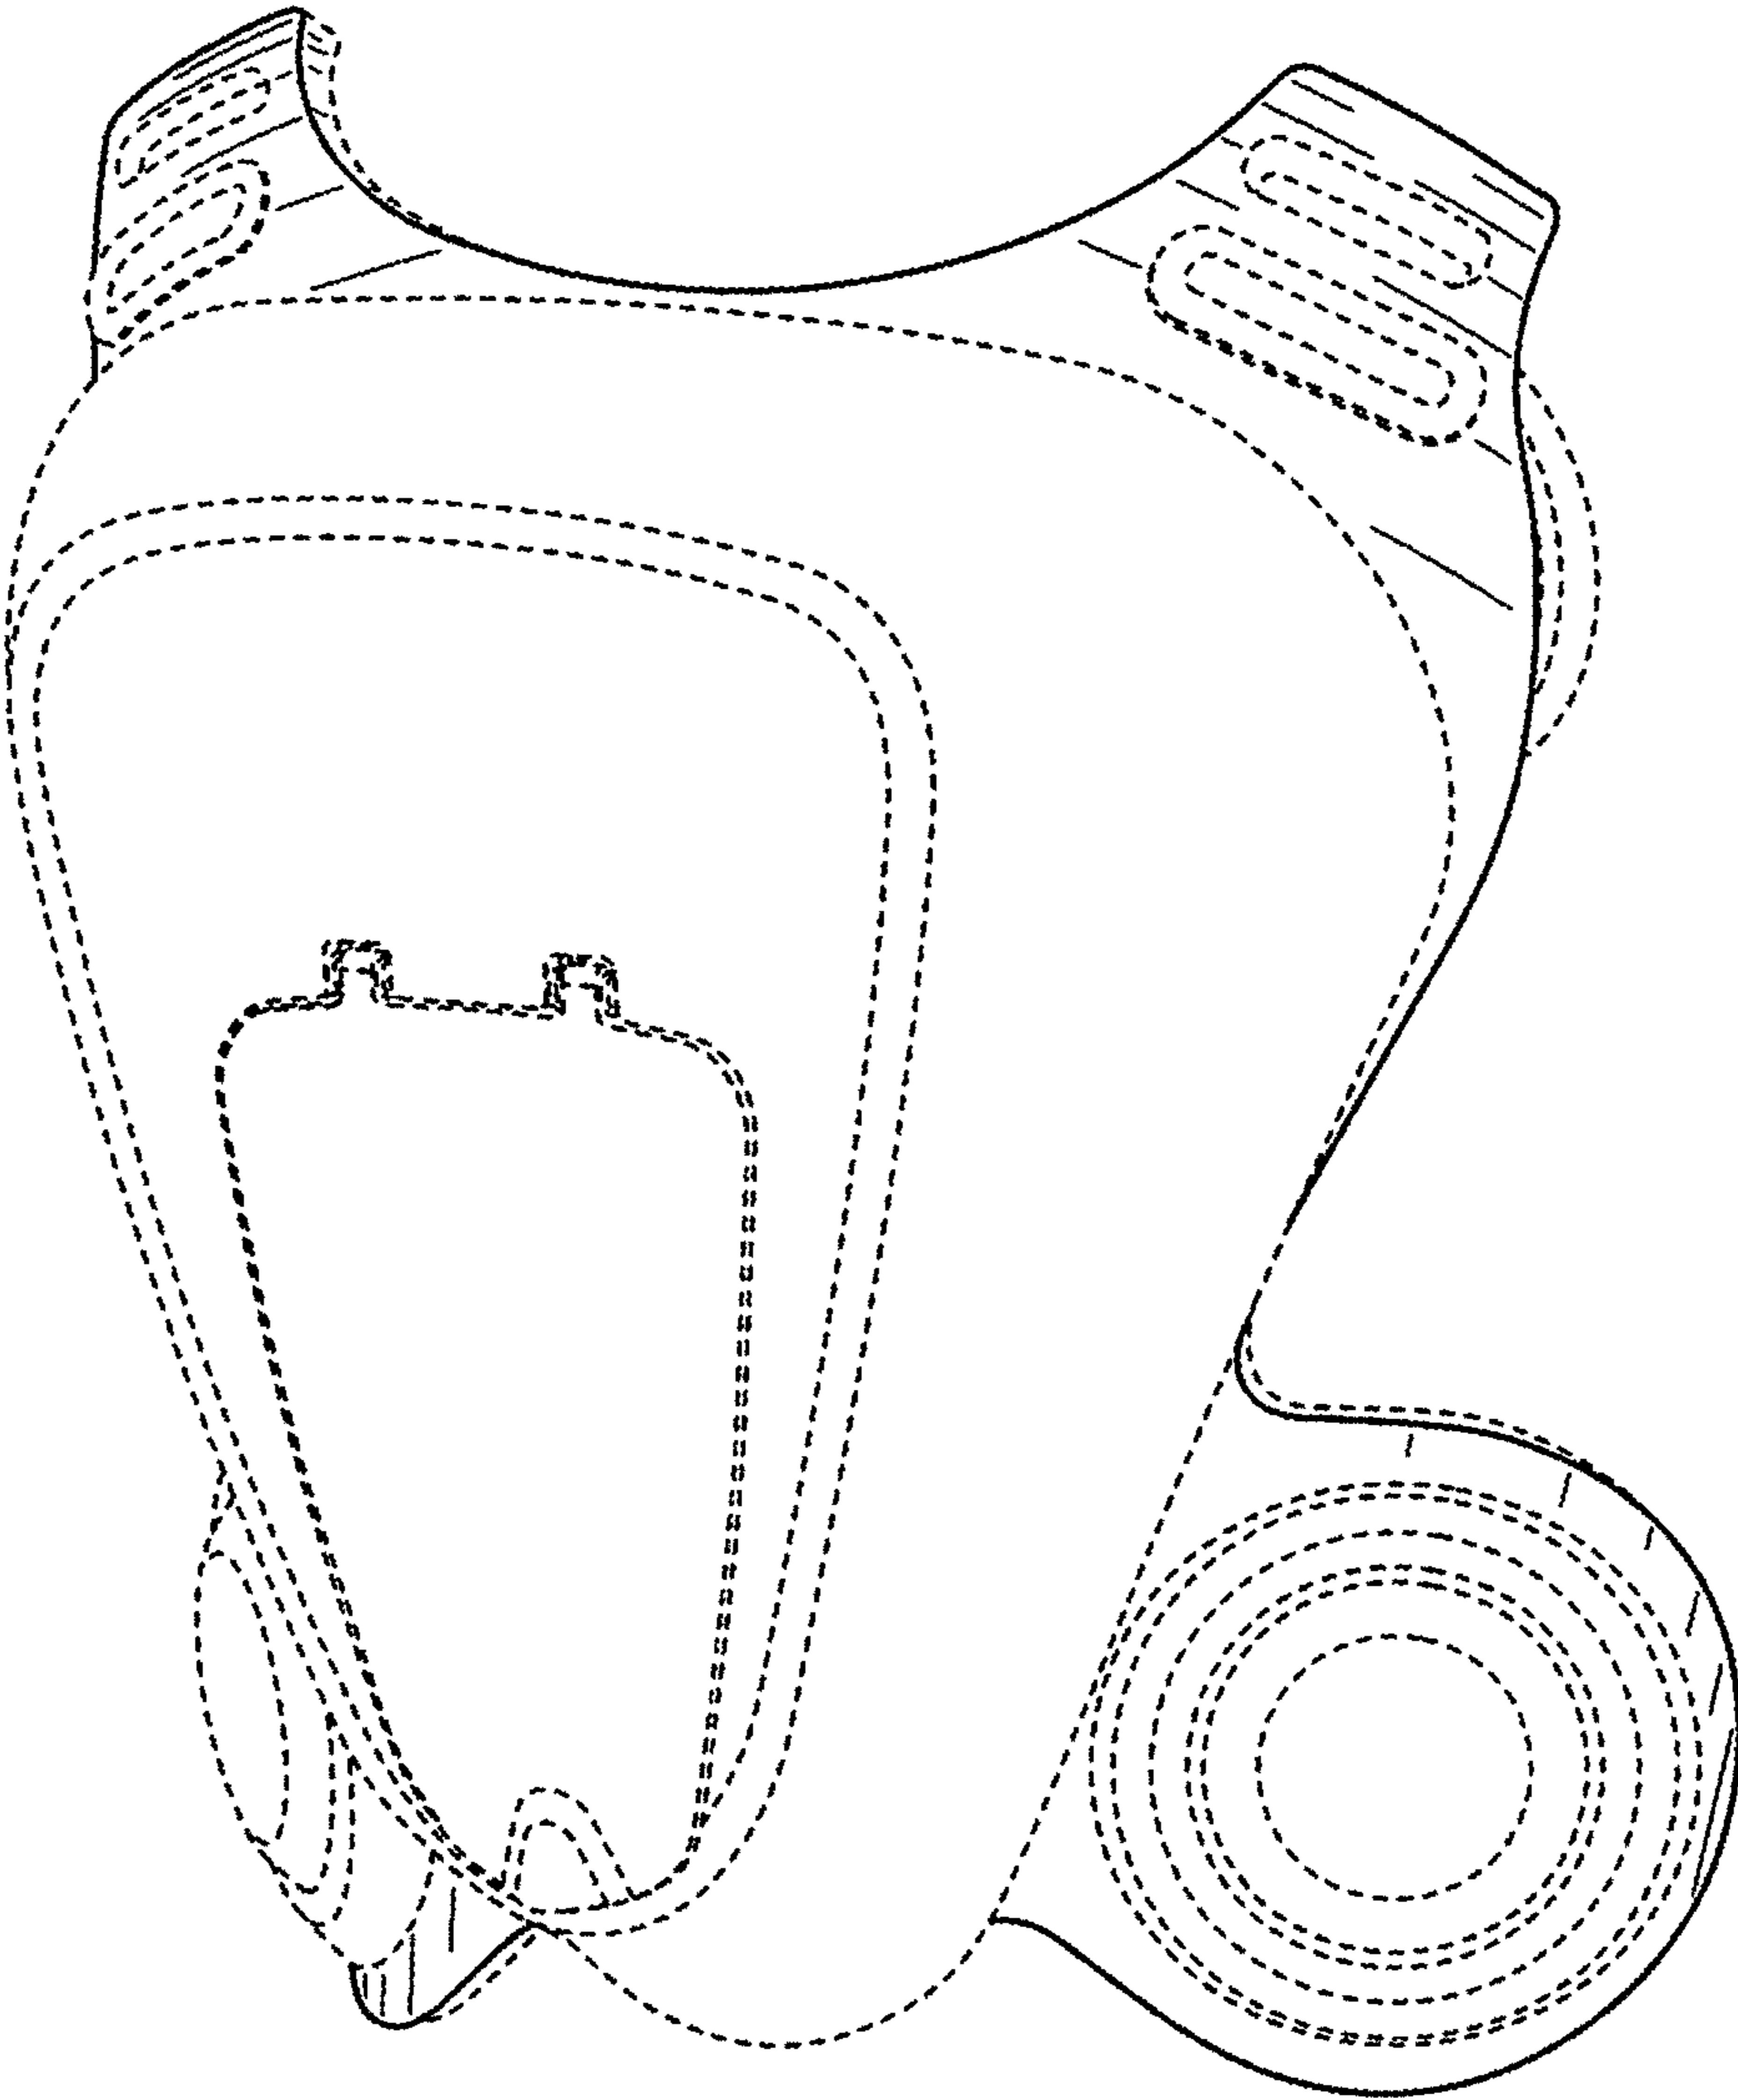


*FIG. 1*

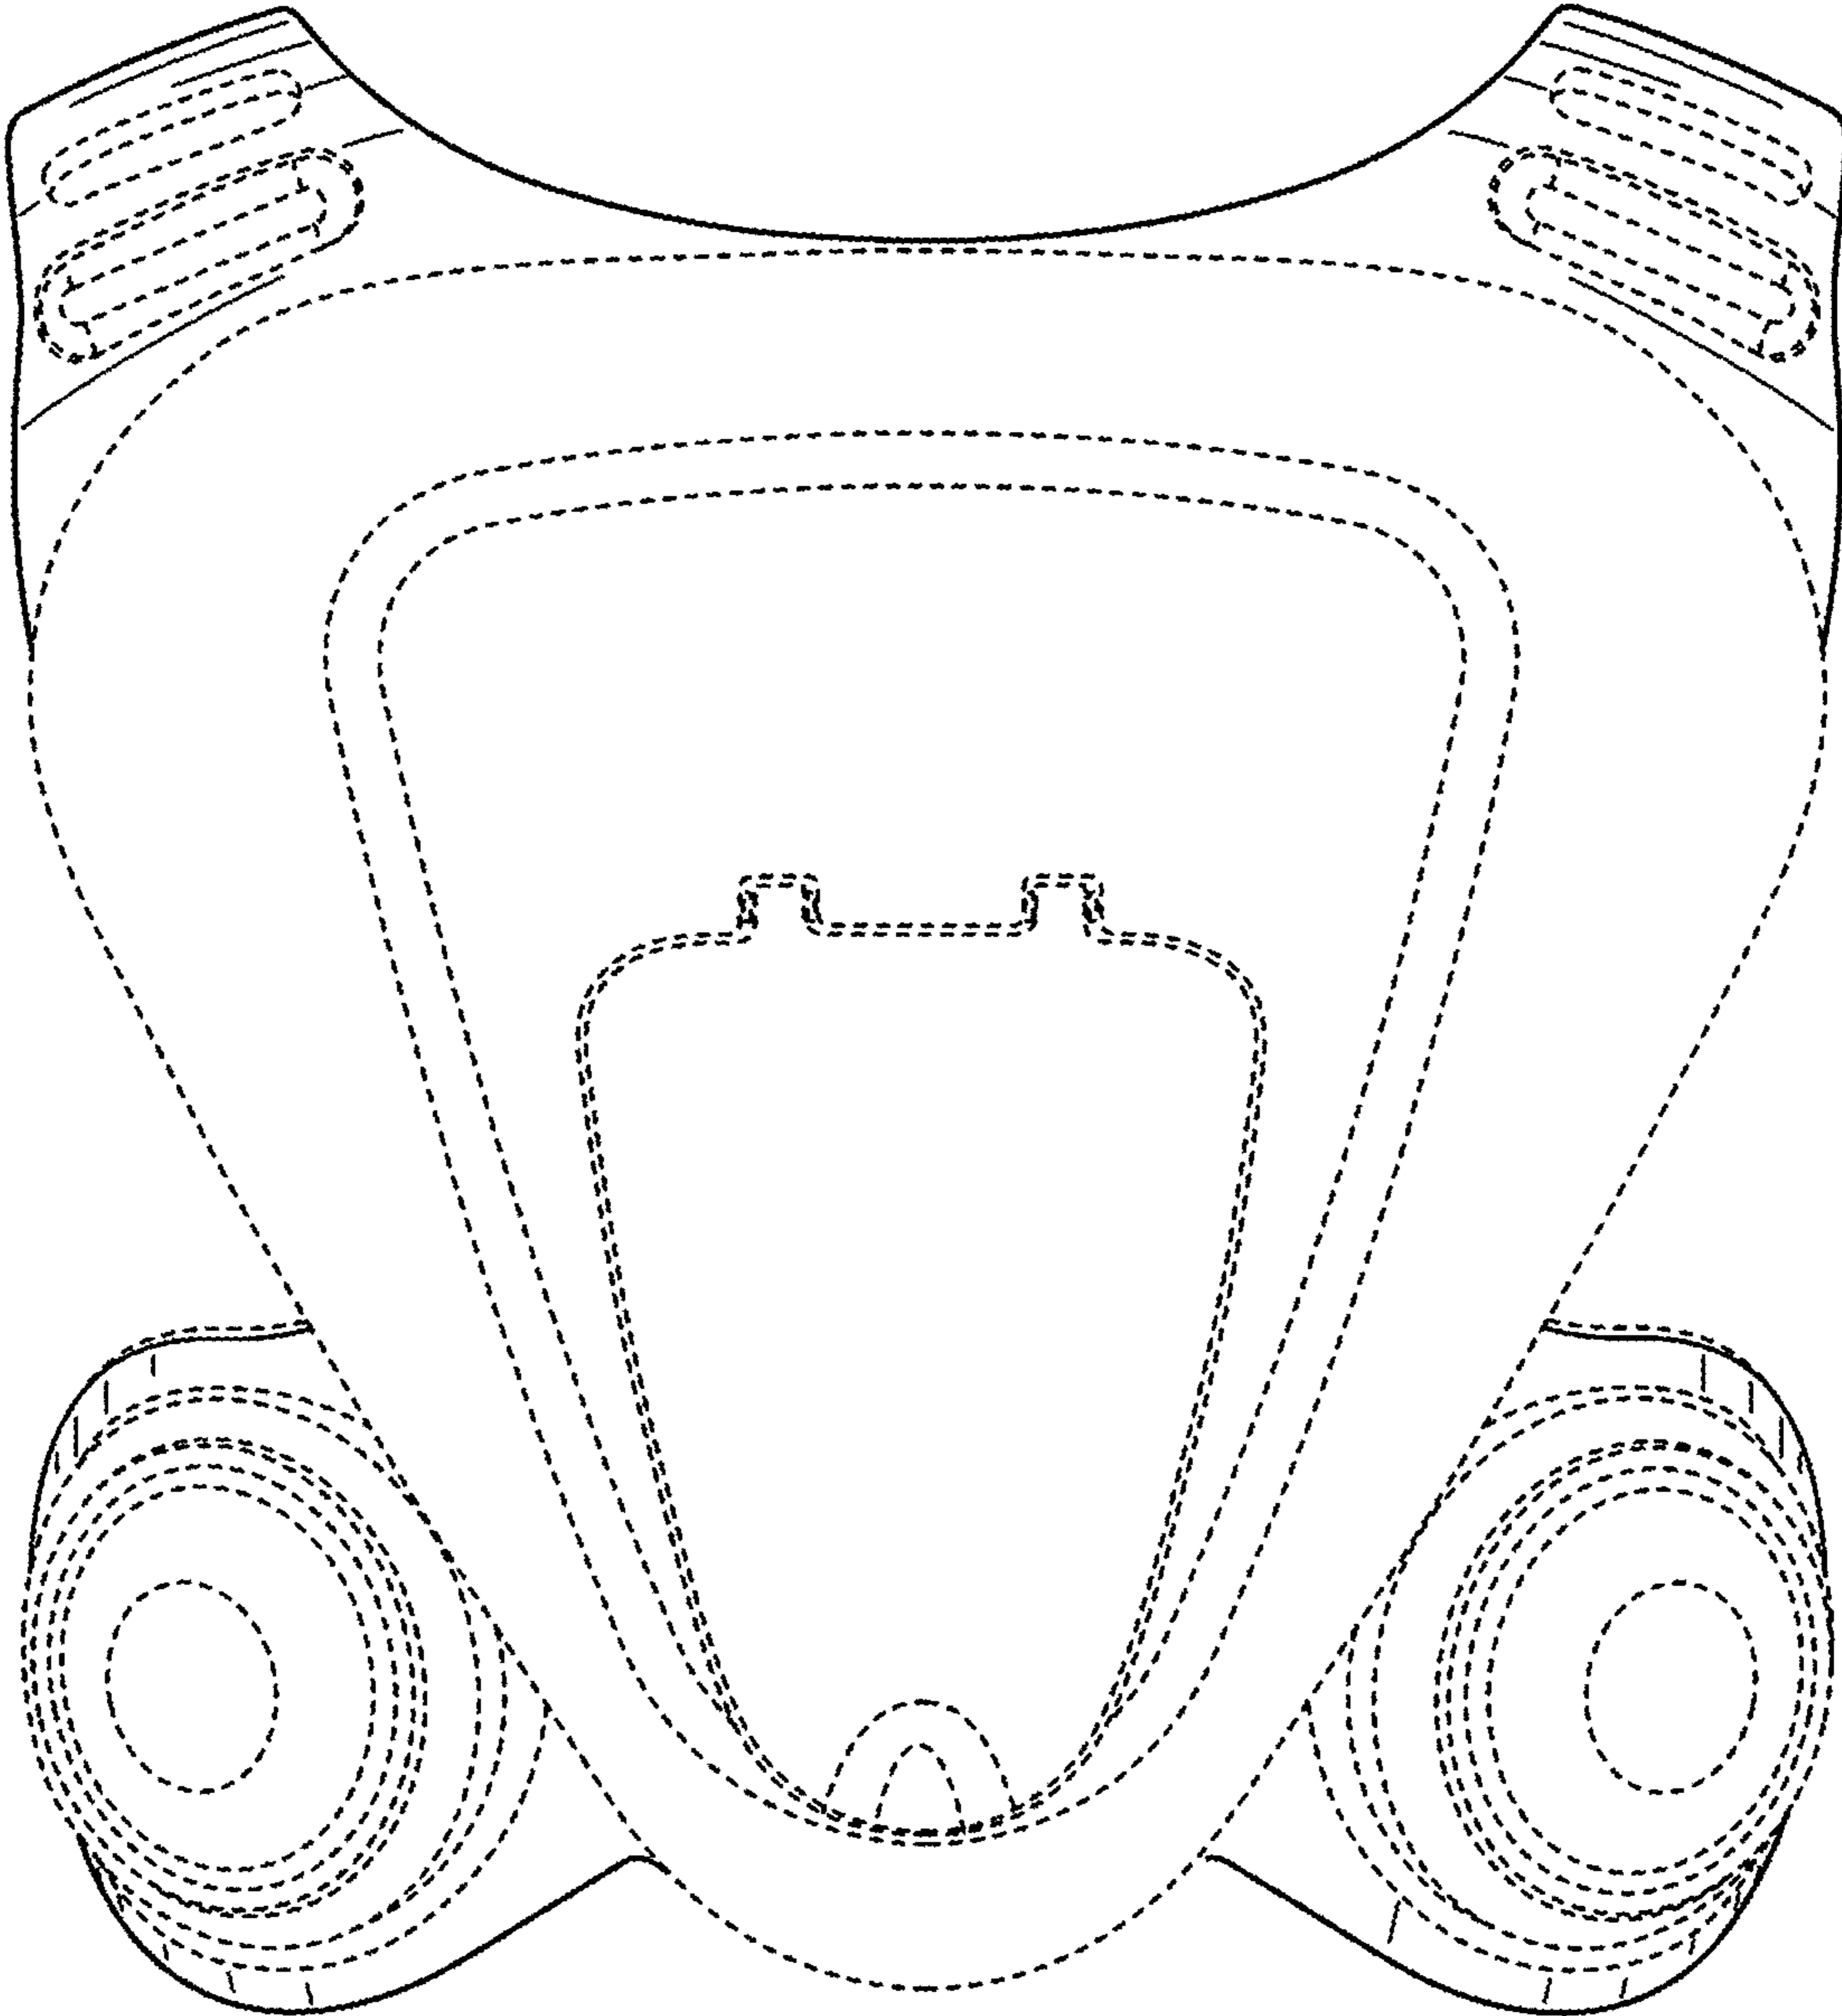


*FIG. 2*

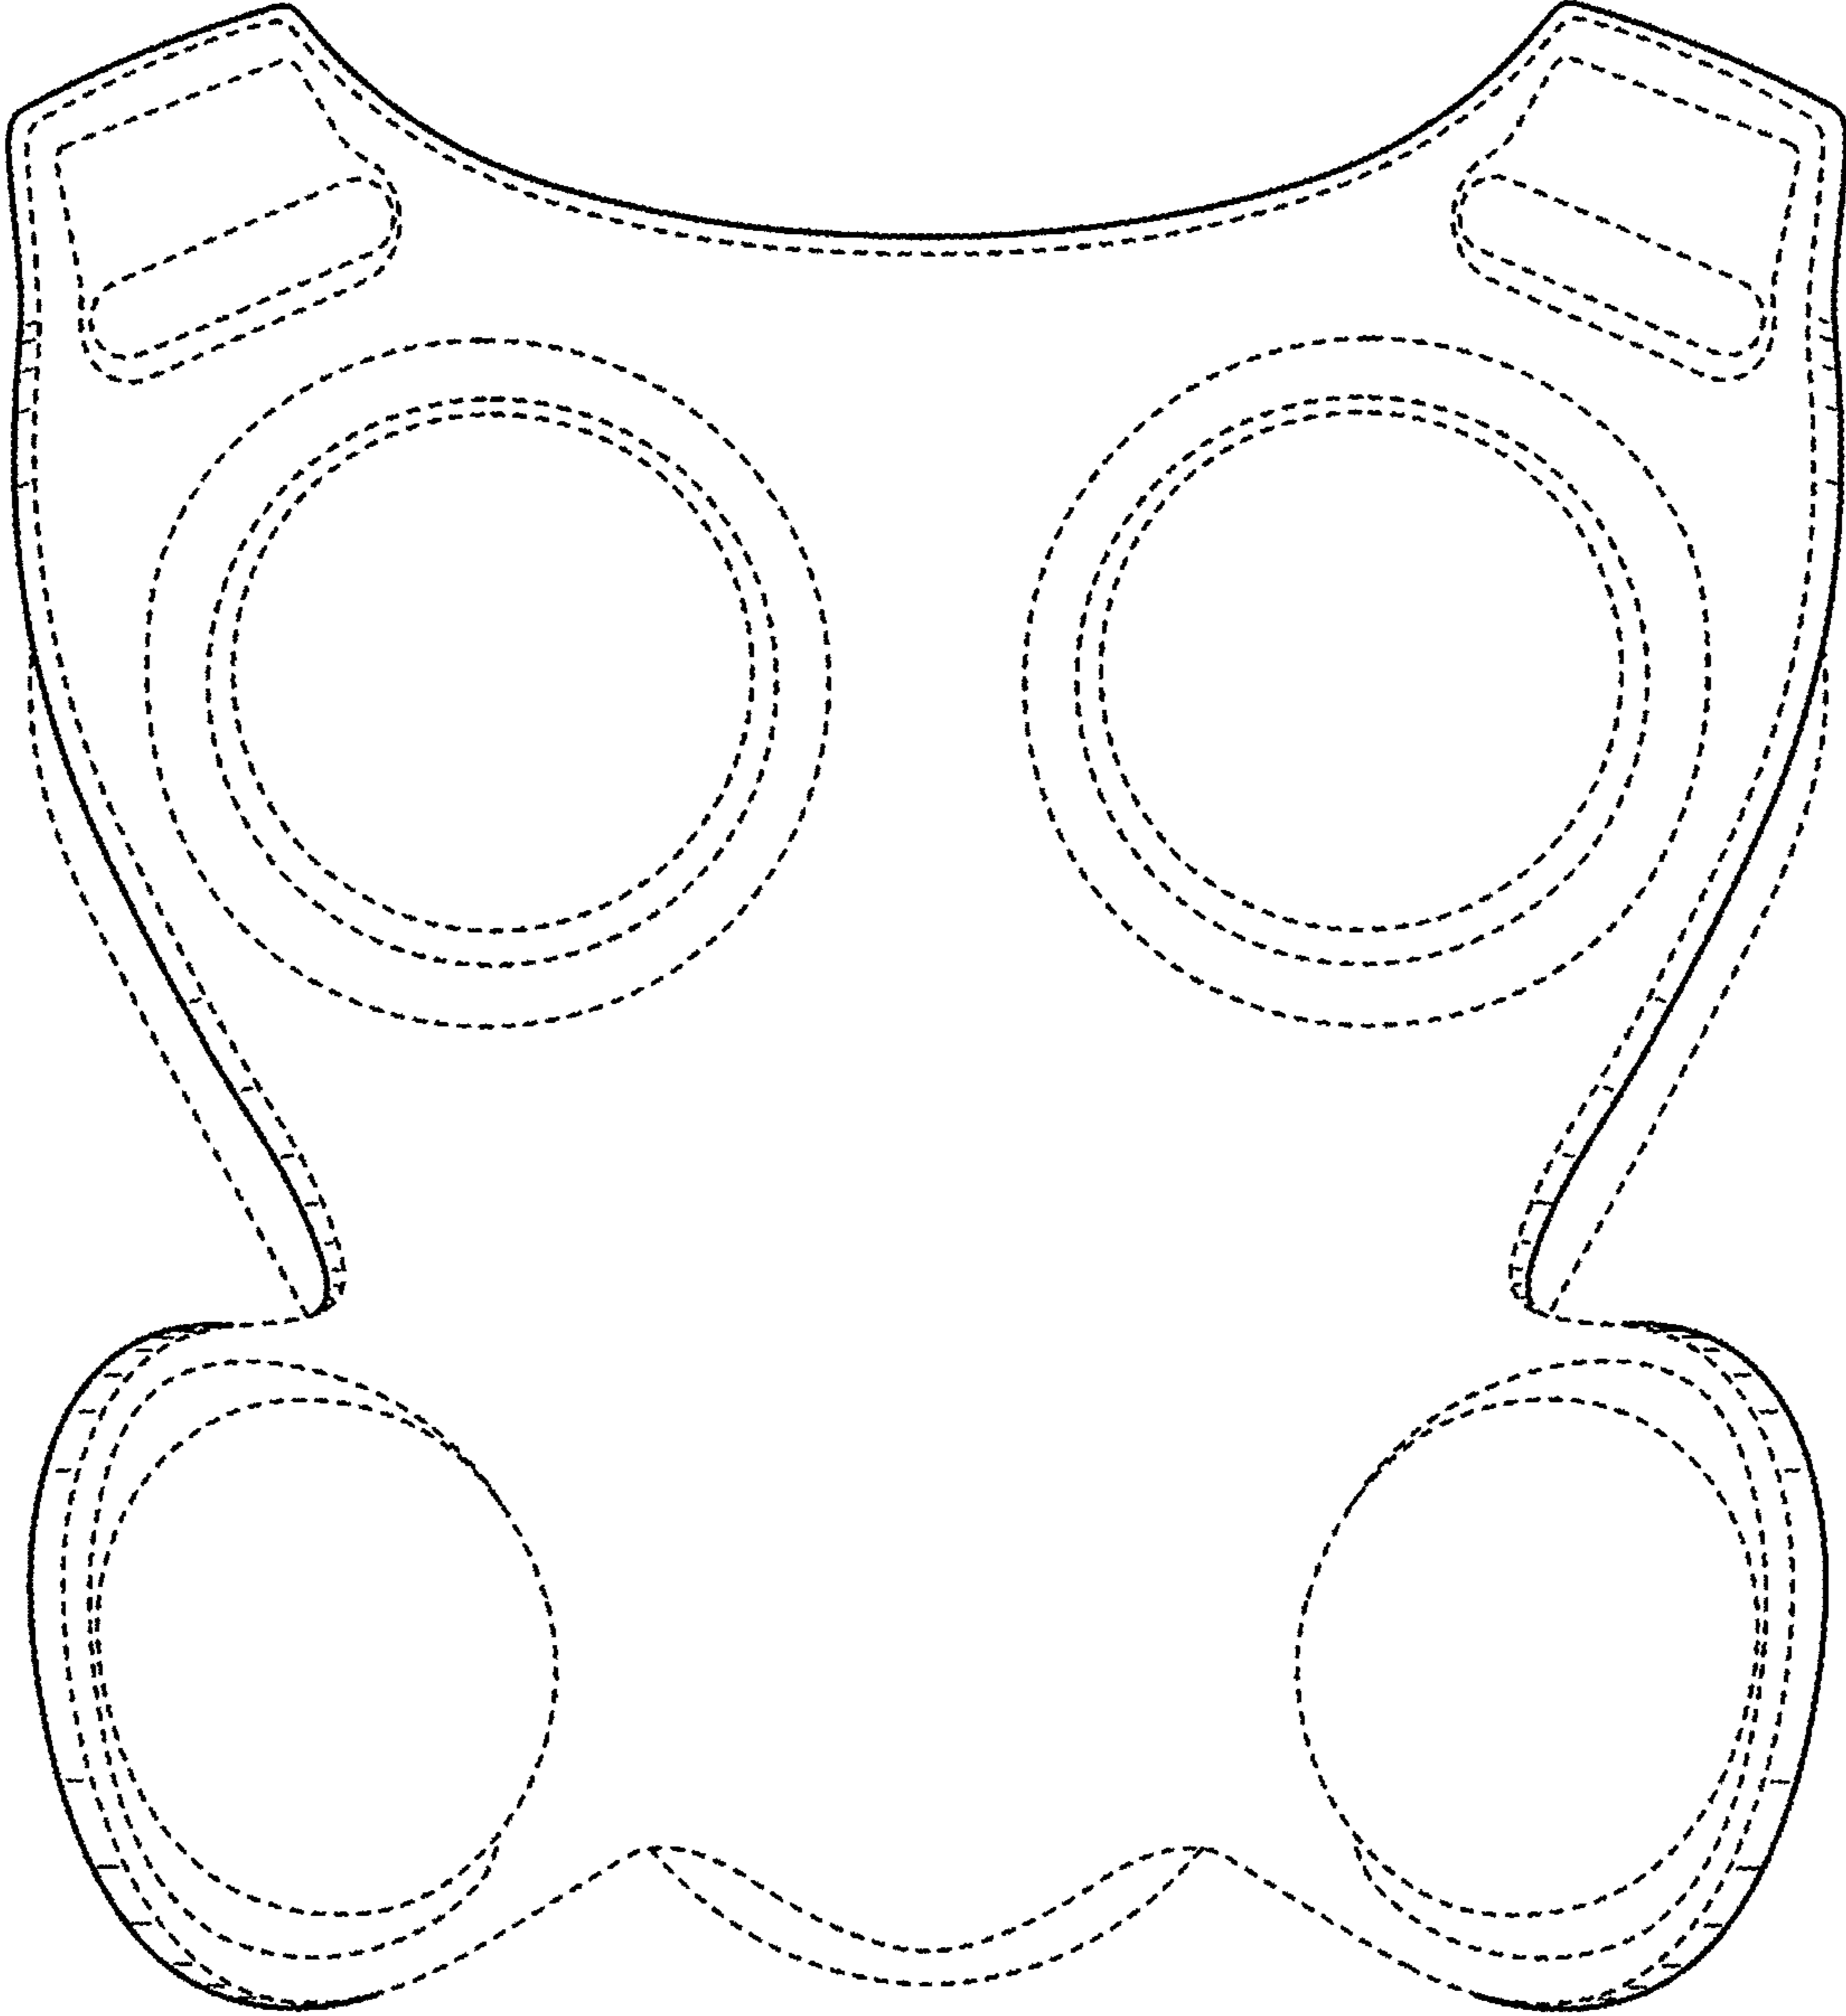


*FIG. 3*

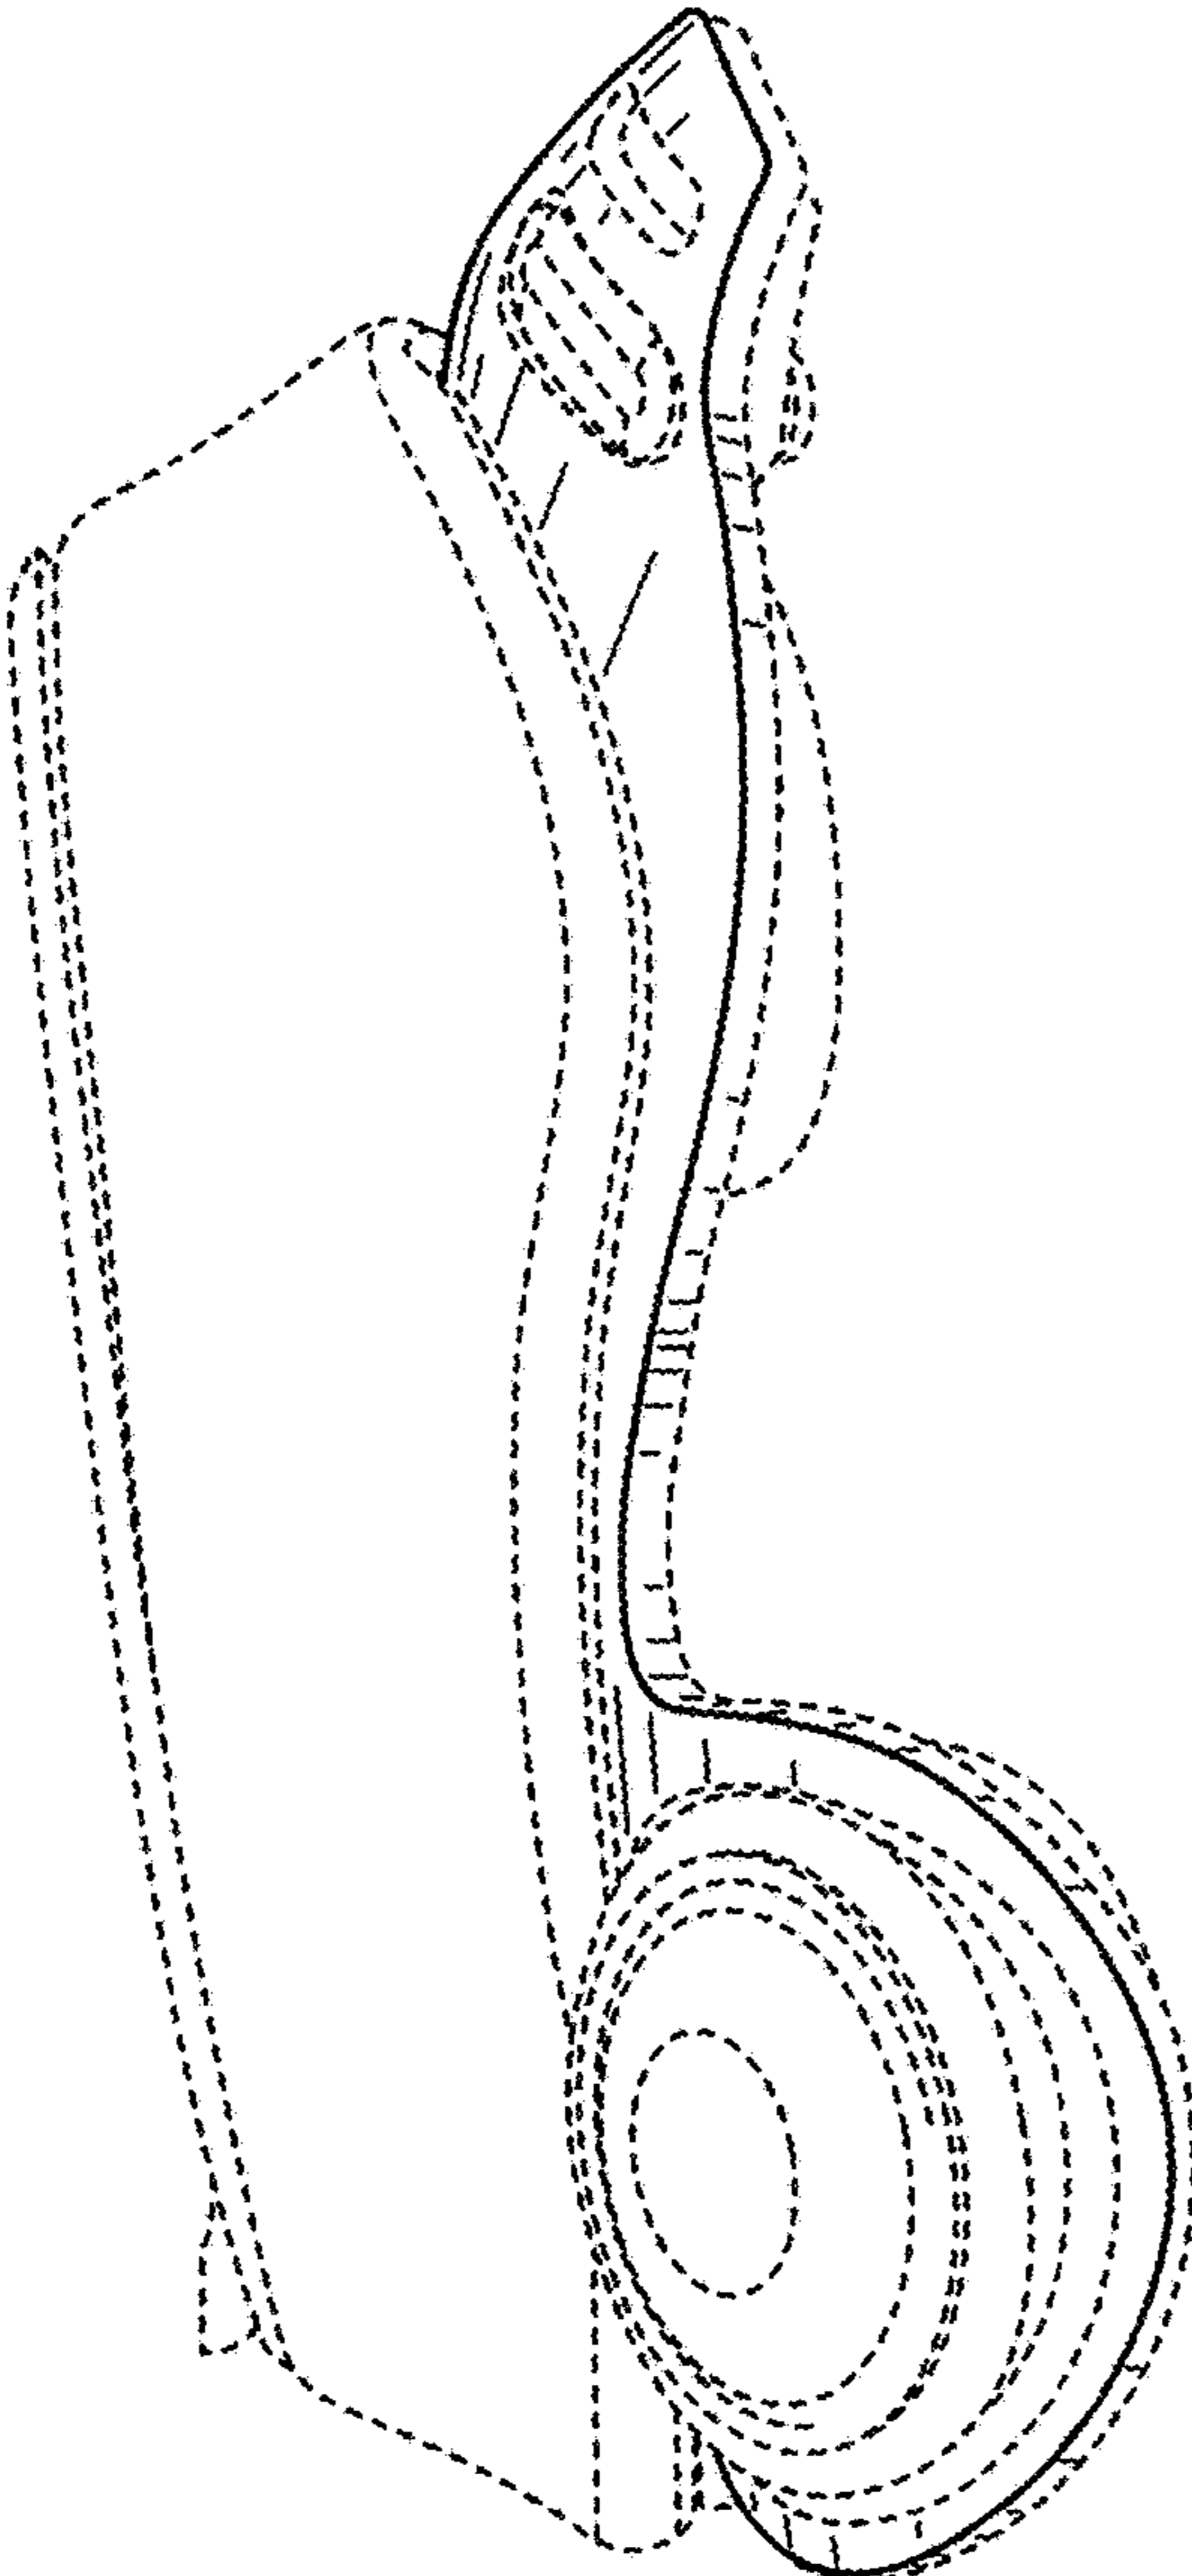


*FIG. 4*

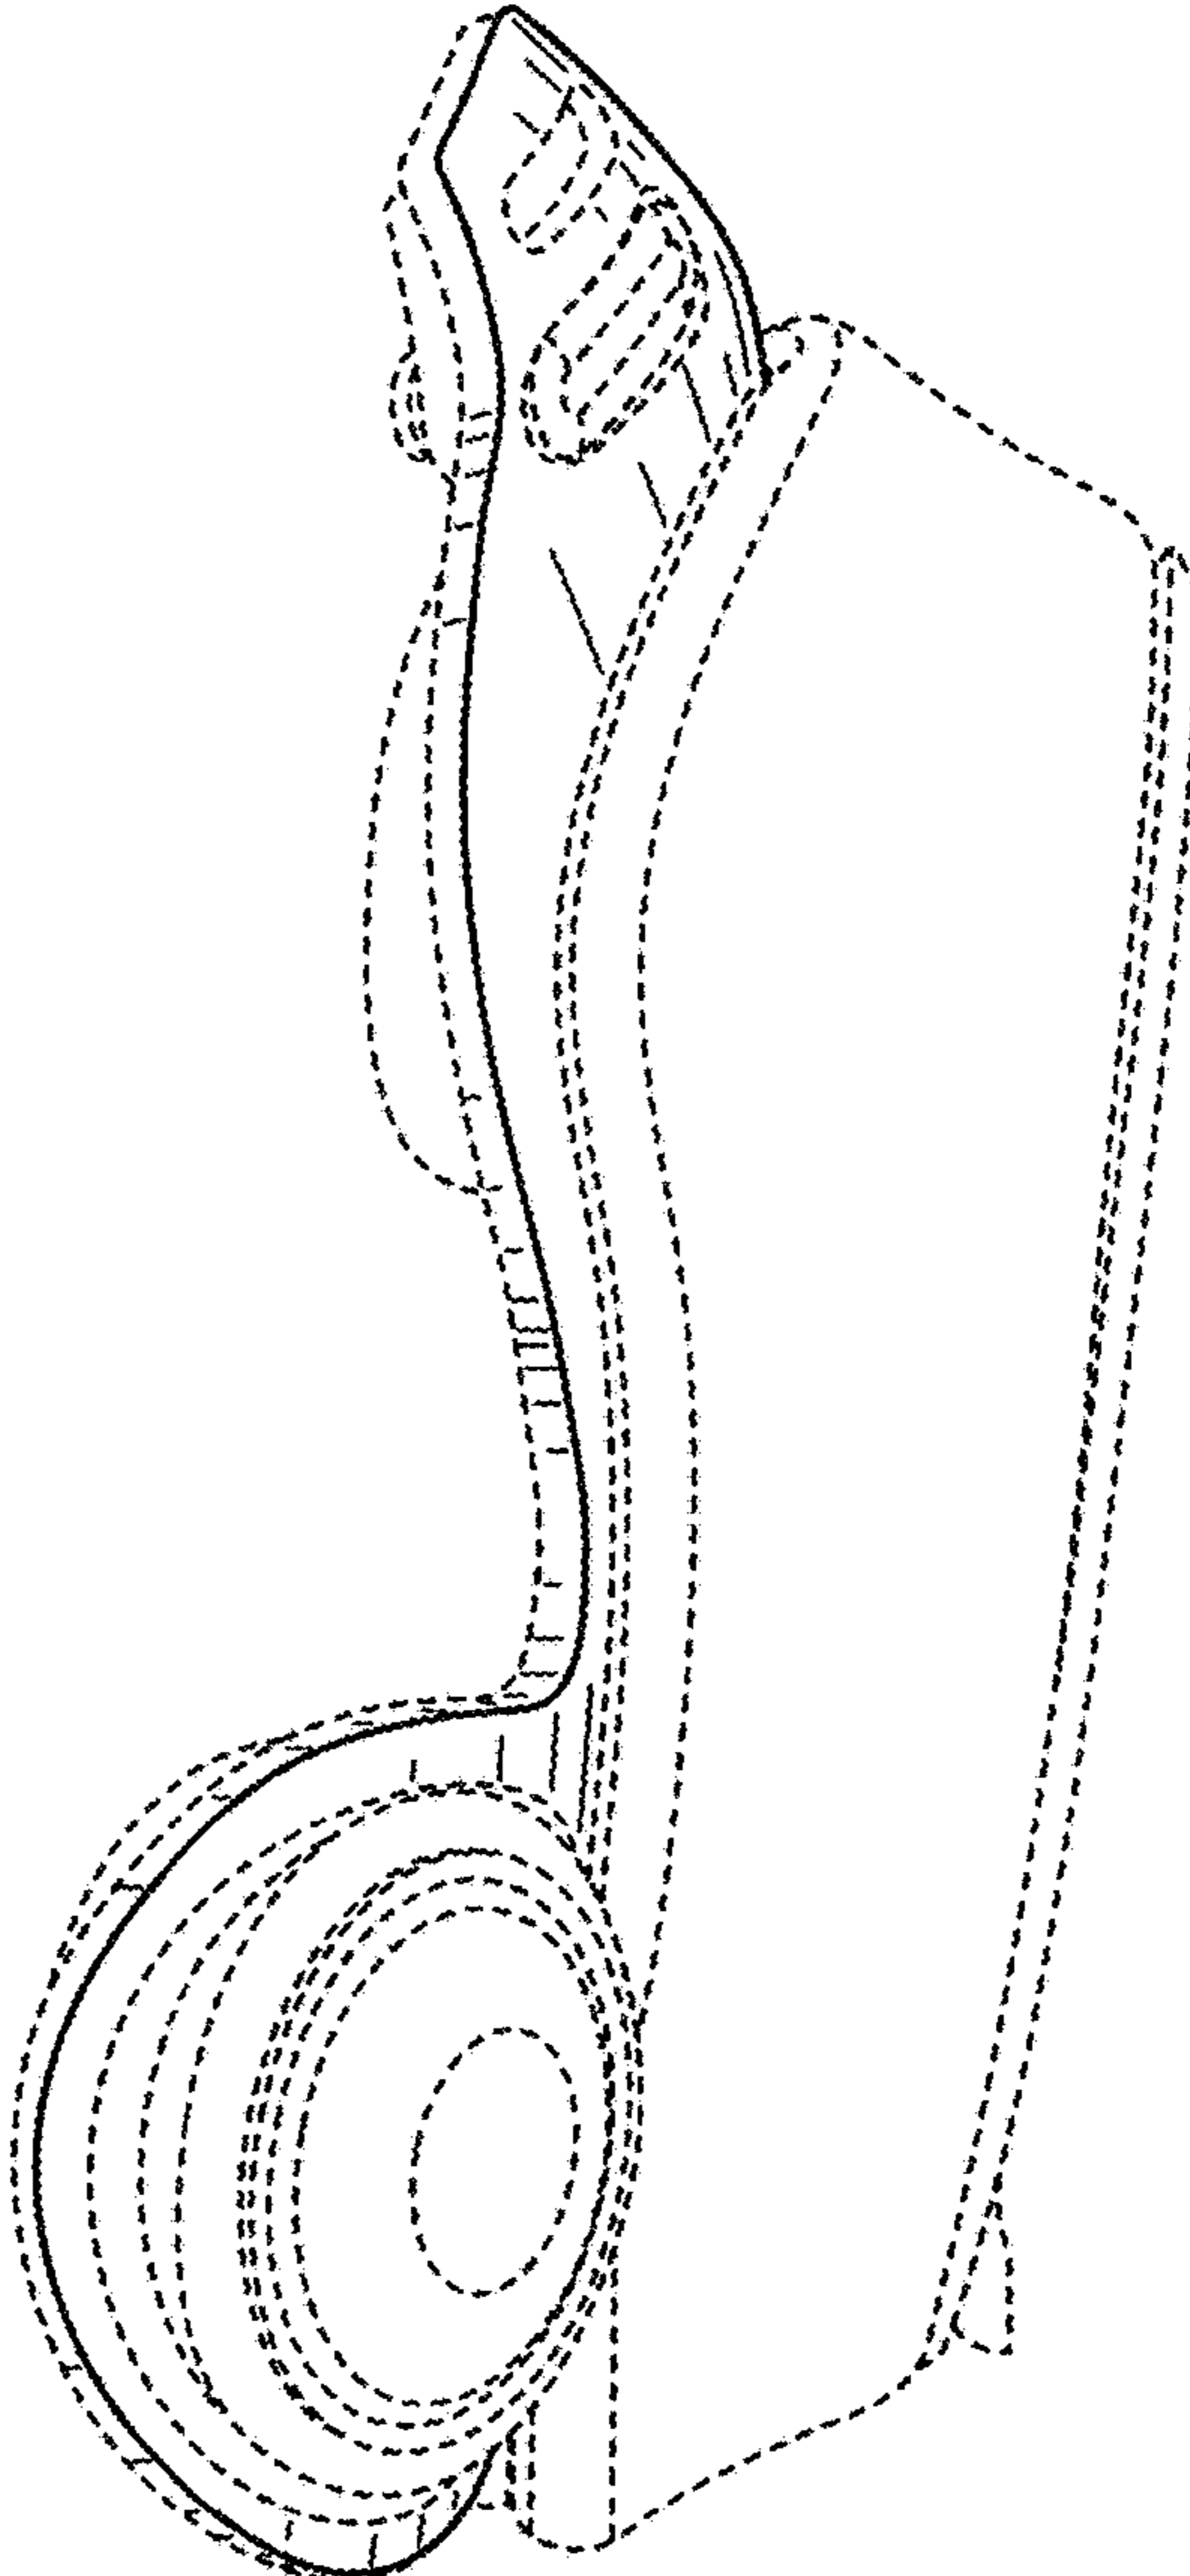

*FIG. 5*

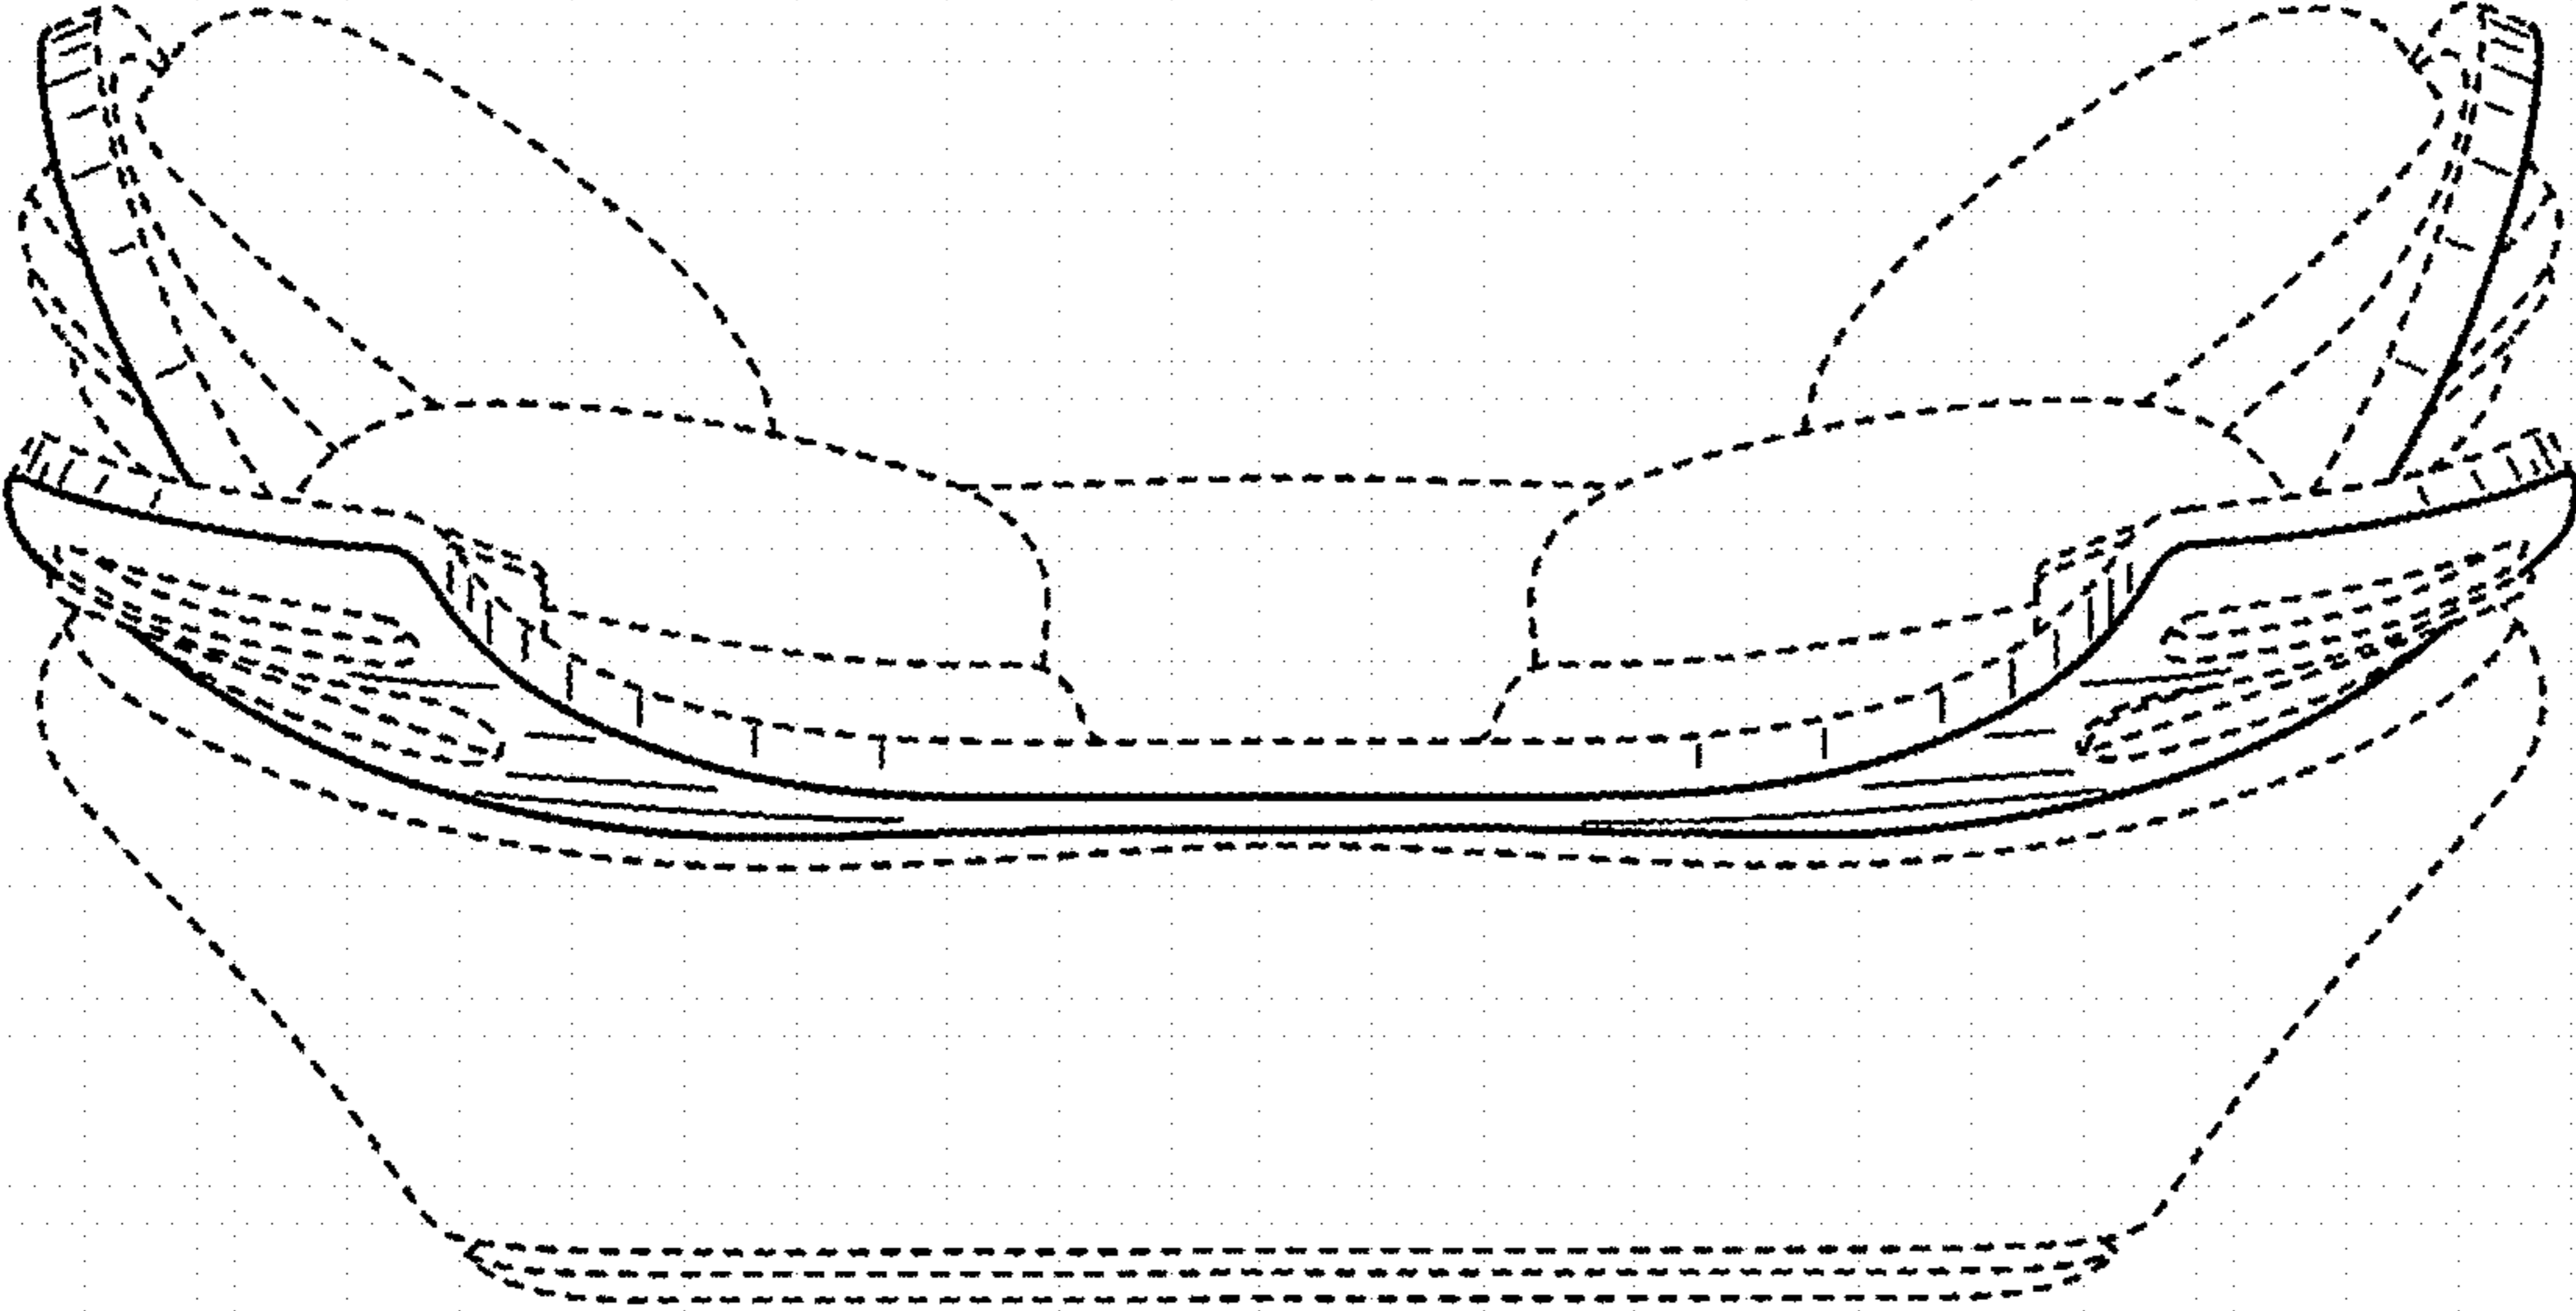

*FIG. 6*

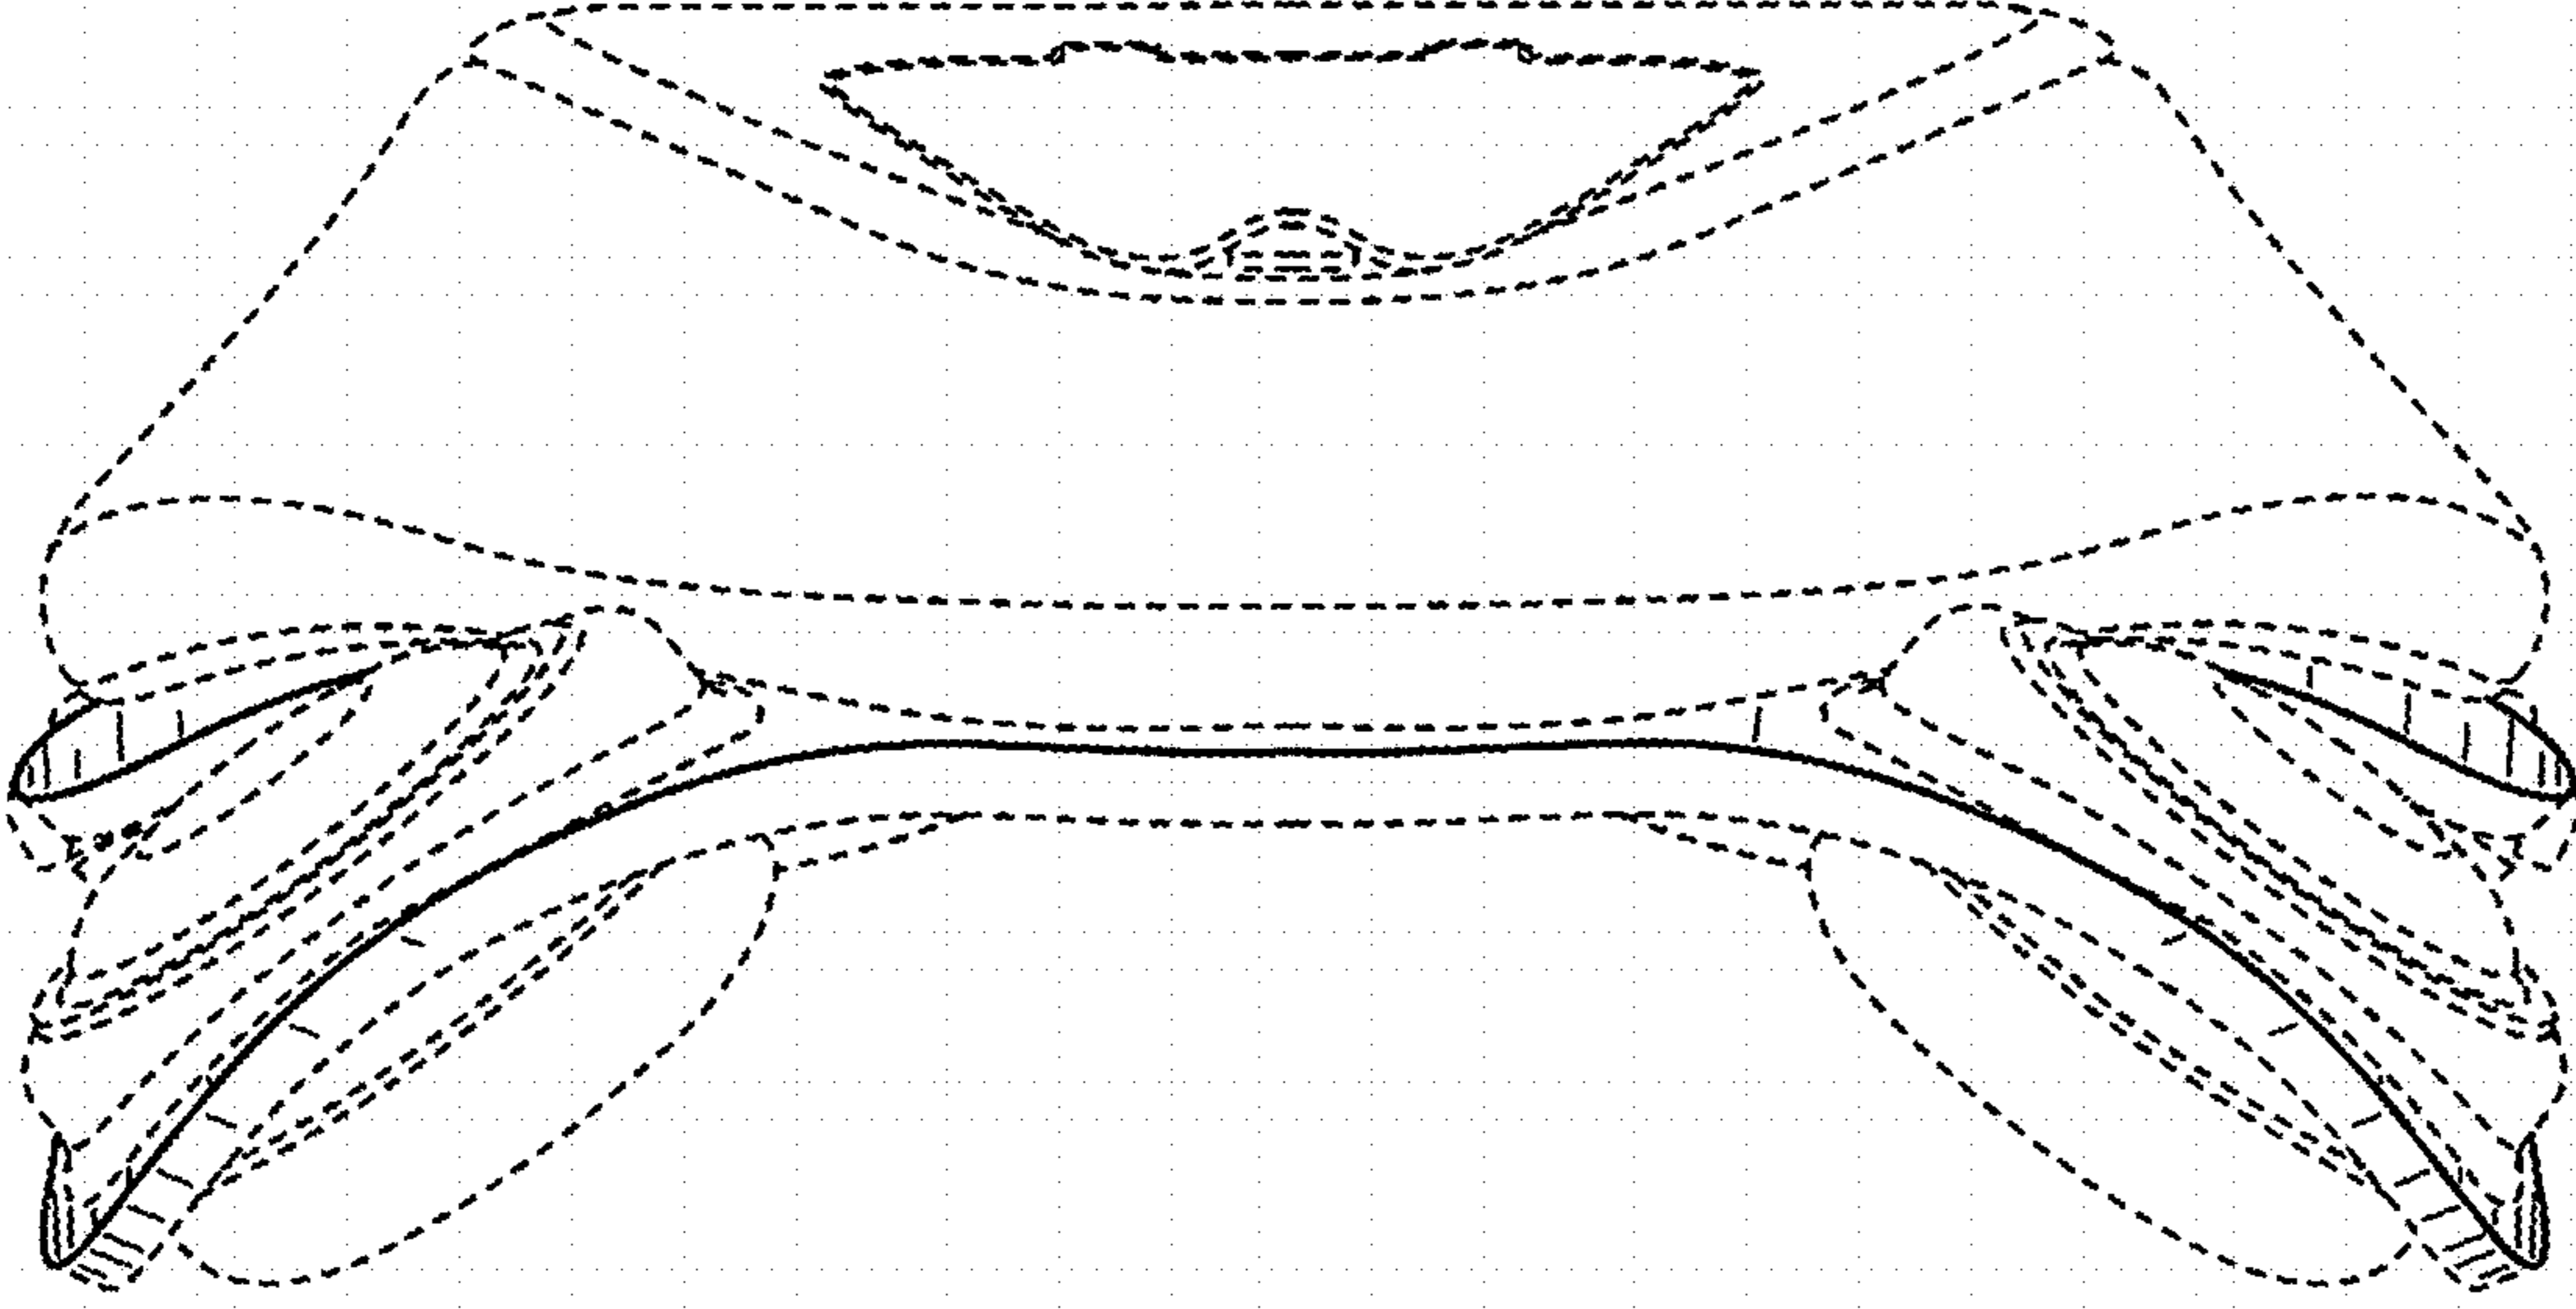

*FIG. 7*