



US00D956229S

(12) **United States Design Patent** (10) **Patent No.:** **US D956,229 S**
Beer et al. (45) **Date of Patent:** **** Jun. 28, 2022**

(54) **INTRAVAGINAL DEVICE ASSEMBLY**

(71) Applicant: **Renovia Inc.**, Boston, MA (US)

(72) Inventors: **Marc D. Beer**, Sudbury, MA (US);
Jose Bohorquez, Boston, MA (US);
Samantha J. Pulliam, Boston, MA (US);
Jessica L. McKinney, Boston, MA (US)

(73) Assignee: **Renovia Inc.**, Boston, MA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/754,374**

(22) Filed: **Oct. 9, 2020**

Related U.S. Application Data

(63) Continuation of application No. 29/686,273, filed on Apr. 3, 2019, now Pat. No. Des. 898,911.

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/141**

(58) **Field of Classification Search**

USPC D24/128, 135, 140, 141, 143, 152, 200,
D24/214, 215; 600/29, 30; D16/237,
D16/250; D28/4, 76, 83; D9/430, 432;
D10/57

CPC A61B 1/31; A61B 1/272; A61B 1/303;
A61B 1/00154; A61B 17/00; A61B
17/17; A61B 10/00; A61B 5/05; A61B
5/0215; A61B 5/4337; A61B 5/4368;
A61F 6/00; A61F 6/06; A61F 6/18; A61F
6/20; A61F 6/142; A61F 6/12; A61C
5/82; G03B 42/042; A61H 19/00


See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,830,582 A 4/1958 Ljung
3,854,476 A * 12/1974 Dickinson, III A61D 1/06
128/884

4,669,478 A 6/1987 Robertson
D309,866 S * 8/1990 Fukuda D10/57
D310,275 S * 8/1990 Su D28/76
5,328,077 A 7/1994 Lou
5,386,836 A 2/1995 Biswas
5,406,961 A 4/1995 Artal
5,562,717 A 10/1996 Tippey et al.
5,603,685 A 2/1997 Tutrone, Jr.
5,674,238 A 10/1997 Sample et al.
5,924,984 A 7/1999 Rao
6,001,060 A 12/1999 Churchill et al.
6,021,781 A 2/2000 Thompson et al.
6,039,701 A 3/2000 Sliwa et al.
6,056,699 A 5/2000 Sohn et al.
6,080,118 A * 6/2000 Blythe A61B 10/0012
600/549
6,086,549 A 7/2000 Neese et al.
6,264,582 B1 7/2001 Remes
6,272,371 B1 8/2001 Shlomo
D458,681 S 6/2002 Sherlock et al.
6,413,206 B2 7/2002 Biswas
6,432,037 B1 8/2002 Eini et al.
6,511,427 B1 1/2003 Sliwa, Jr. et al.
6,672,996 B2 1/2004 Ross et al.
6,679,854 B2 1/2004 Honda et al.
6,741,895 B1 * 5/2004 Gafni A61B 5/4337
600/38
D491,079 S * 6/2004 Lim D10/57
D491,274 S * 6/2004 Dubniczki D24/223
6,816,744 B2 11/2004 Garfield et al.
7,079,882 B1 7/2006 Schmidt
D535,203 S * 1/2007 Chen D10/57
D548,359 S * 8/2007 Illein D24/223
7,577,476 B2 8/2009 Hochman et al.
7,608,037 B2 10/2009 Levy
7,628,744 B2 12/2009 Hoffman et al.
7,645,220 B2 1/2010 Hoffman et al.
7,736,298 B2 6/2010 Guerquin et al.
7,837,682 B2 11/2010 Ostrovsky et al.
7,892,179 B2 * 2/2011 Rieth A61B 5/4277
600/551
7,955,241 B2 6/2011 Hoffman et al.
7,957,794 B2 6/2011 Hochman et al.
D651,531 S * 1/2012 Rothman D10/57
8,147,429 B2 4/2012 Mittal et al.
8,360,954 B2 1/2013 Kim
8,623,004 B2 1/2014 Johnson et al.
8,715,204 B2 5/2014 Webster et al.
8,728,140 B2 5/2014 Feemster et al.
8,740,767 B2 6/2014 Rosen et al.
8,805,472 B2 8/2014 Iglesias
8,821,407 B2 * 9/2014 Kirsner A61B 10/0012
600/551

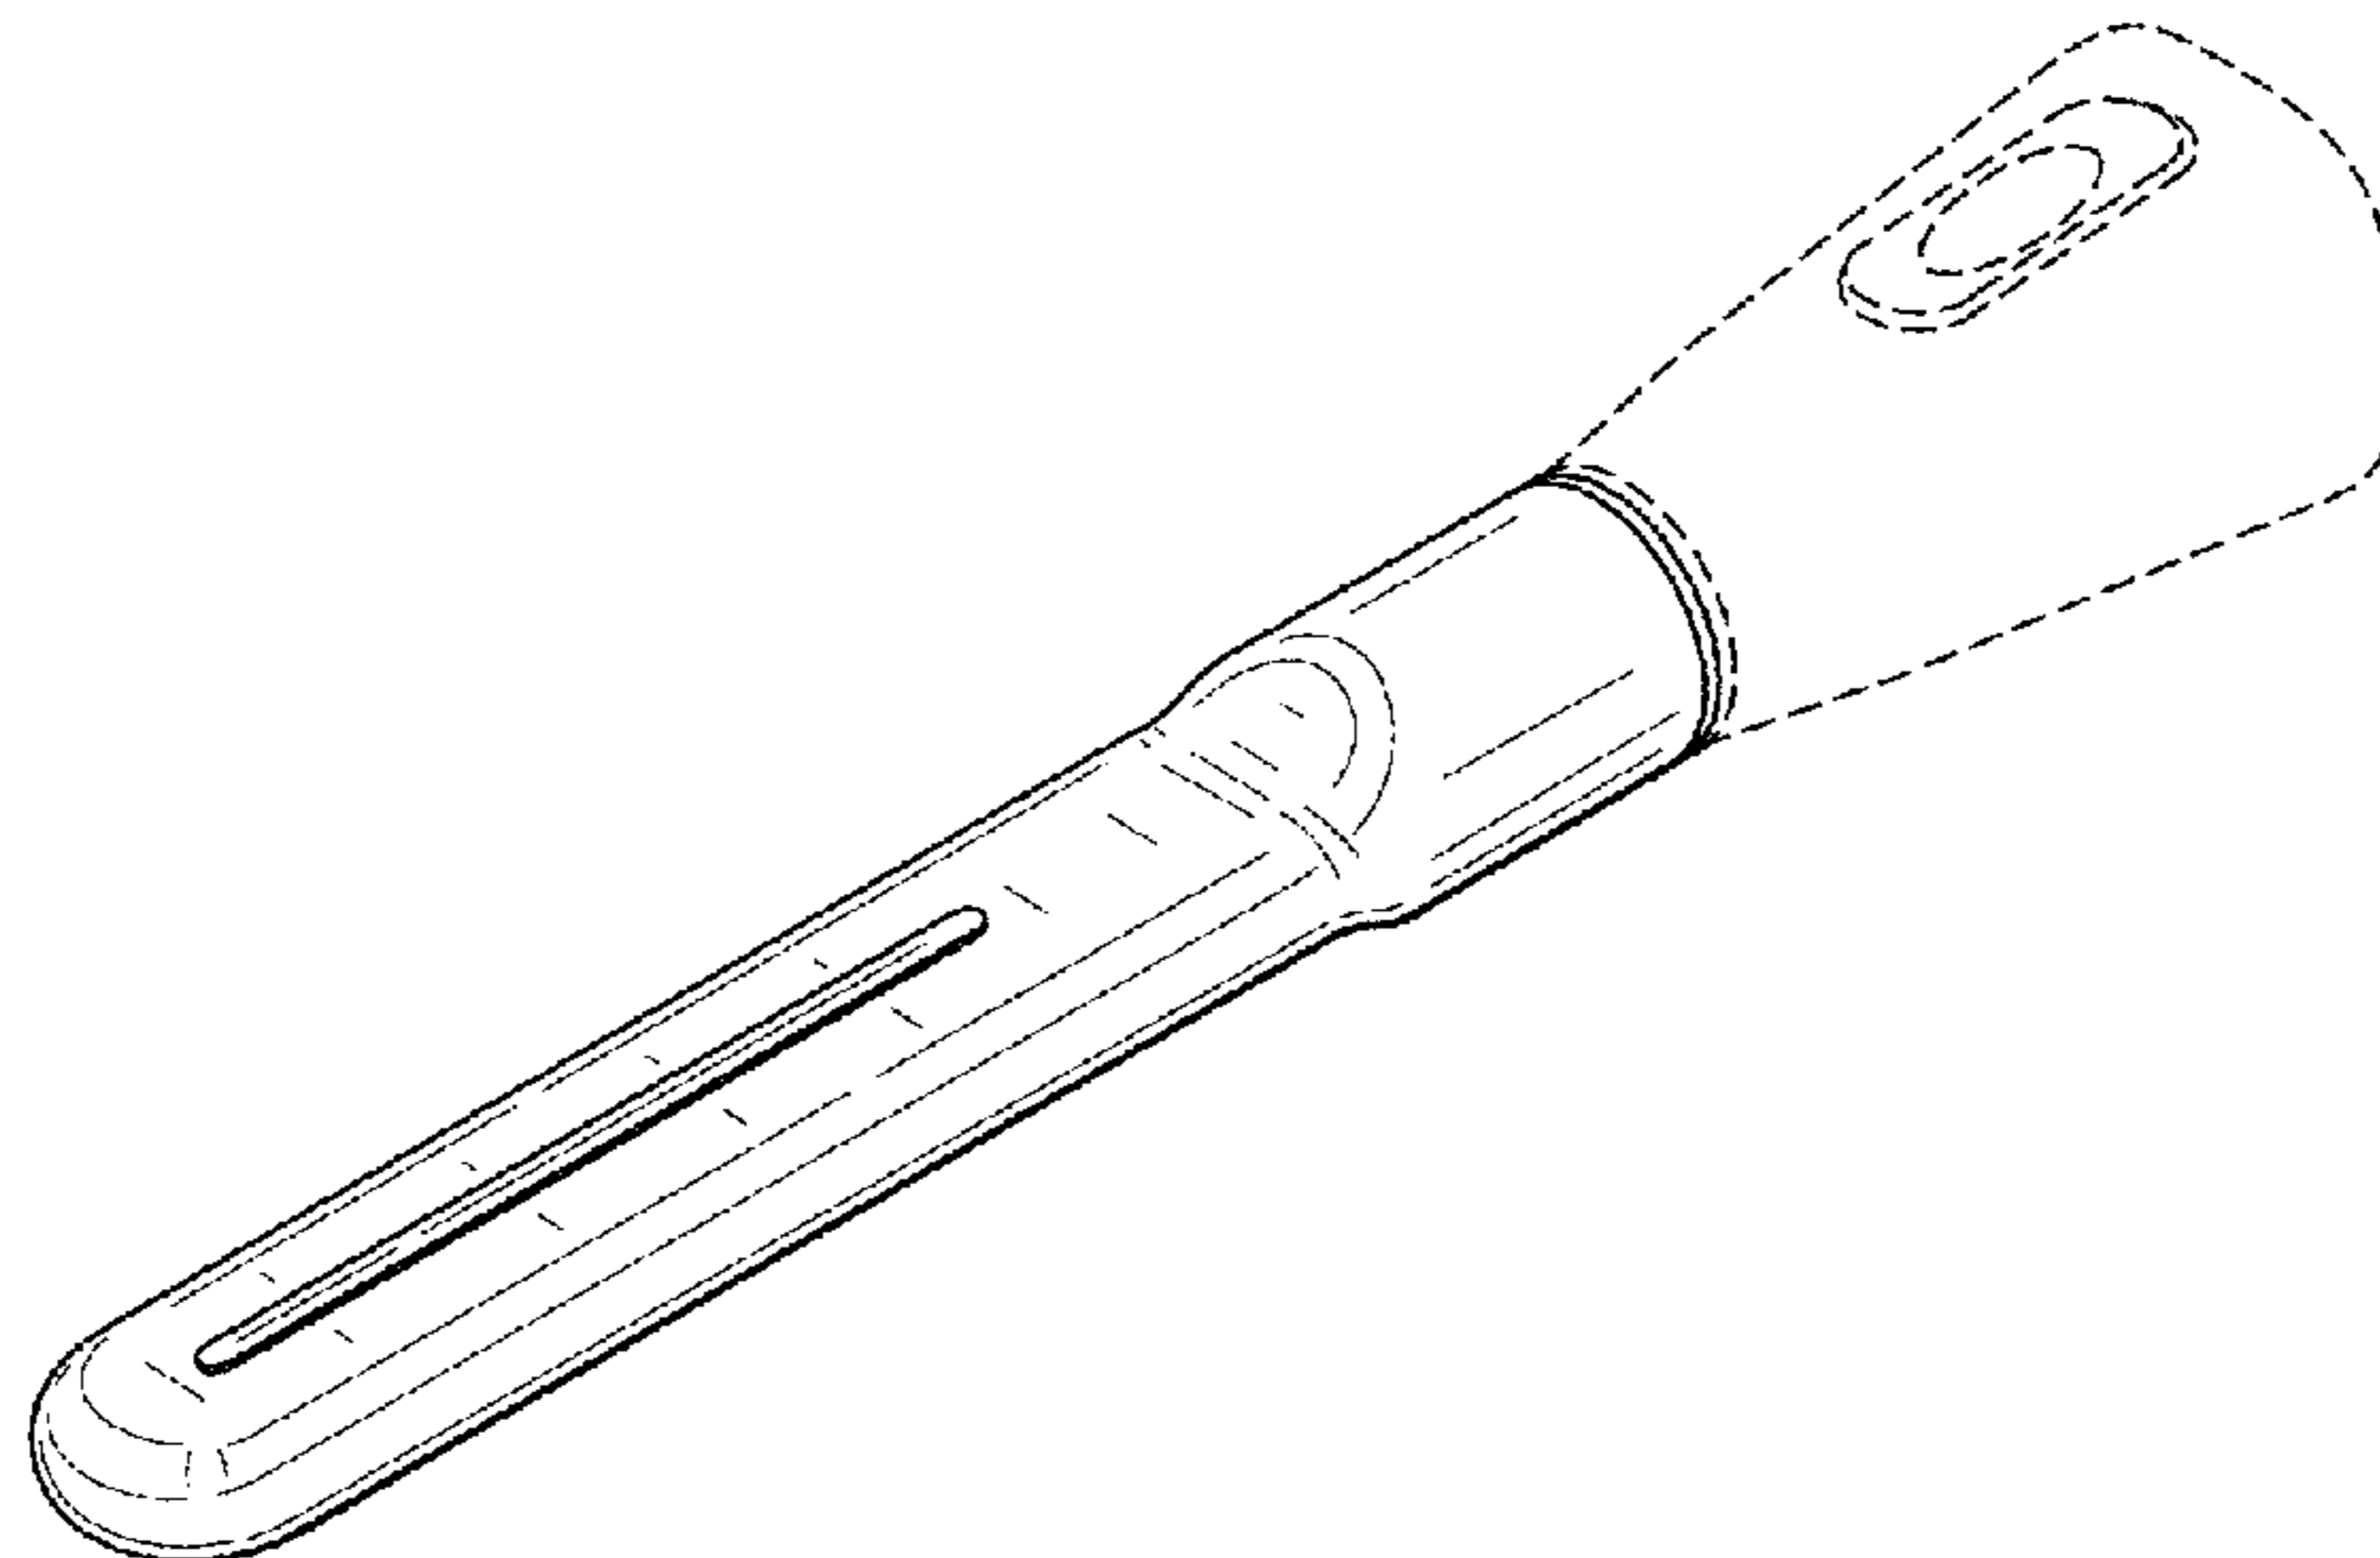

WO WO-2017/149688 A1 9/2017
 WO WO-2018/023037 A1 2/2018
 WO WO-2019/084468 A1 5/2019
 WO WO-2019/084469 A1 5/2019
 WO WO-2020/092343 A1 5/2020

OTHER PUBLICATIONS

Glazer et al., “Pelvic floor muscle biofeedback in the treatment of urinary incontinence: A literature review,” *Appl Psychophysiol Biofeedback*. 31(3):187-201 (2006) (Abstract only).
 Kandadai et al., “Correct Performance of Pelvic Muscle Exercises in Women Reporting Prior Knowledge,” *Female Pelvic Med Reconstr Surg*. 21(3):135-40 (2015).
 Malcovati et al., *Interface Circuitry and Microsystems. MEMS—A Practical Guide to Design, Analysis, and Applications*. Jan G. Korvink and Oliver Paul, 901-942 (2006).
 Moen et al., “Pelvic floor muscle function in women presenting with pelvic floor disorders,” *Int Urogynecol J Pelvic Floor Dysfunct*. 20(7):843-6 (2009).
 Nygaard et al., “Efficacy of pelvic floor muscle exercises in women with stress, urge, and mixed urinary incontinence,” *Am J Obstet Gynecol*. 174(1 Pt 1):120-125 (1996) (Abstract only).
 Parekh et al., “The role of pelvic floor exercises on post-prostatectomy incontinence,” *J Urol*. 170(1):130-33 (2003) (Abstract Only) (2 pages).
 Rosenbaum et al., “The Role of Pelvic Floor Physical Therapy in the Treatment of Pelvic and Genital Pain-Related Sexual Dysfunction,” *J Sex Med*. 5(3): 513-23 (2008).
 Rosenbaum, “Pelvic floor involvement in male and female sexual dysfunction and the role of pelvic floor rehabilitation in treatment: a literature review,” *J Sex Med*. 4(1):4-13 (2007) (Abstract only) (2 pages).
 Rosenblatt et al., “Evaluation of an accelerometer-based digital health system for the treatment of female urinary incontinence: A pilot study,” *Neurourol Urodyn*. 38(7): 1944-1952 (2019).
 Rosenblatt et al., “Interactive Pelvic Floor Muscle Training for Female Urinary Incontinence,” *Renovia, Inc.*, retrieved Apr. 30, 2019 from <renoviainc.com/wp-content/uploads/2018/04/REN005.01-White-Paper-12Apr18-FINAL.pdf> (2018) (6 pages).

* cited by examiner

Primary Examiner — Clint A Samuel
 (74) *Attorney, Agent, or Firm* — Clark & Elbing LLP

(57)

CLAIM

The ornamental design for an intravaginal device assembly, substantially as shown and described.

DESCRIPTION

FIG. 1 is a front and left side perspective view of an intravaginal device assembly, with the intravaginal device removed from the case for ease of illustration, embodying the claimed design;
 FIG. 2 is an enlarged front view of the intravaginal device of FIG. 1;
 FIG. 3 is an enlarged rear view of the intravaginal device of FIG. 1;
 FIG. 4 is a top view of the intravaginal device of FIG. 1;
 FIG. 5 is a bottom view of the intravaginal device of FIG. 1;
 FIG. 6 is a right side view of the intravaginal device of FIG. 1;
 FIG. 7 is a left side view of the intravaginal device of FIG. 1;
 FIG. 8 is a front and left side perspective view of a case, in a closed position, containing the intravaginal device shown in FIG. 1;
 FIG. 9 is an exploded view of the case and intravaginal device of FIG. 8;
 FIG. 10 is a front and left side perspective view of a partially opened case containing the intravaginal device shown in FIG. 1;
 FIG. 11 is an enlarged front view of the case containing the intravaginal device shown in FIG. 8;
 FIG. 12 is an enlarged rear view of the case containing the intravaginal device shown in FIG. 8;
 FIG. 13 is a right side view of the case and intravaginal device shown in FIG. 10;
 FIG. 14 is a left side view of the case and intravaginal device shown in FIG. 10;
 FIG. 15 is a top view of the case and intravaginal device shown in FIG. 10; and,
 FIG. 16 is a bottom view of the case and intravaginal device shown in FIG. 10.
 The broken lines show portions of the intravaginal device assembly that form no part of the claimed design.

1 Claim, 10 Drawing Sheets

FIG. 1

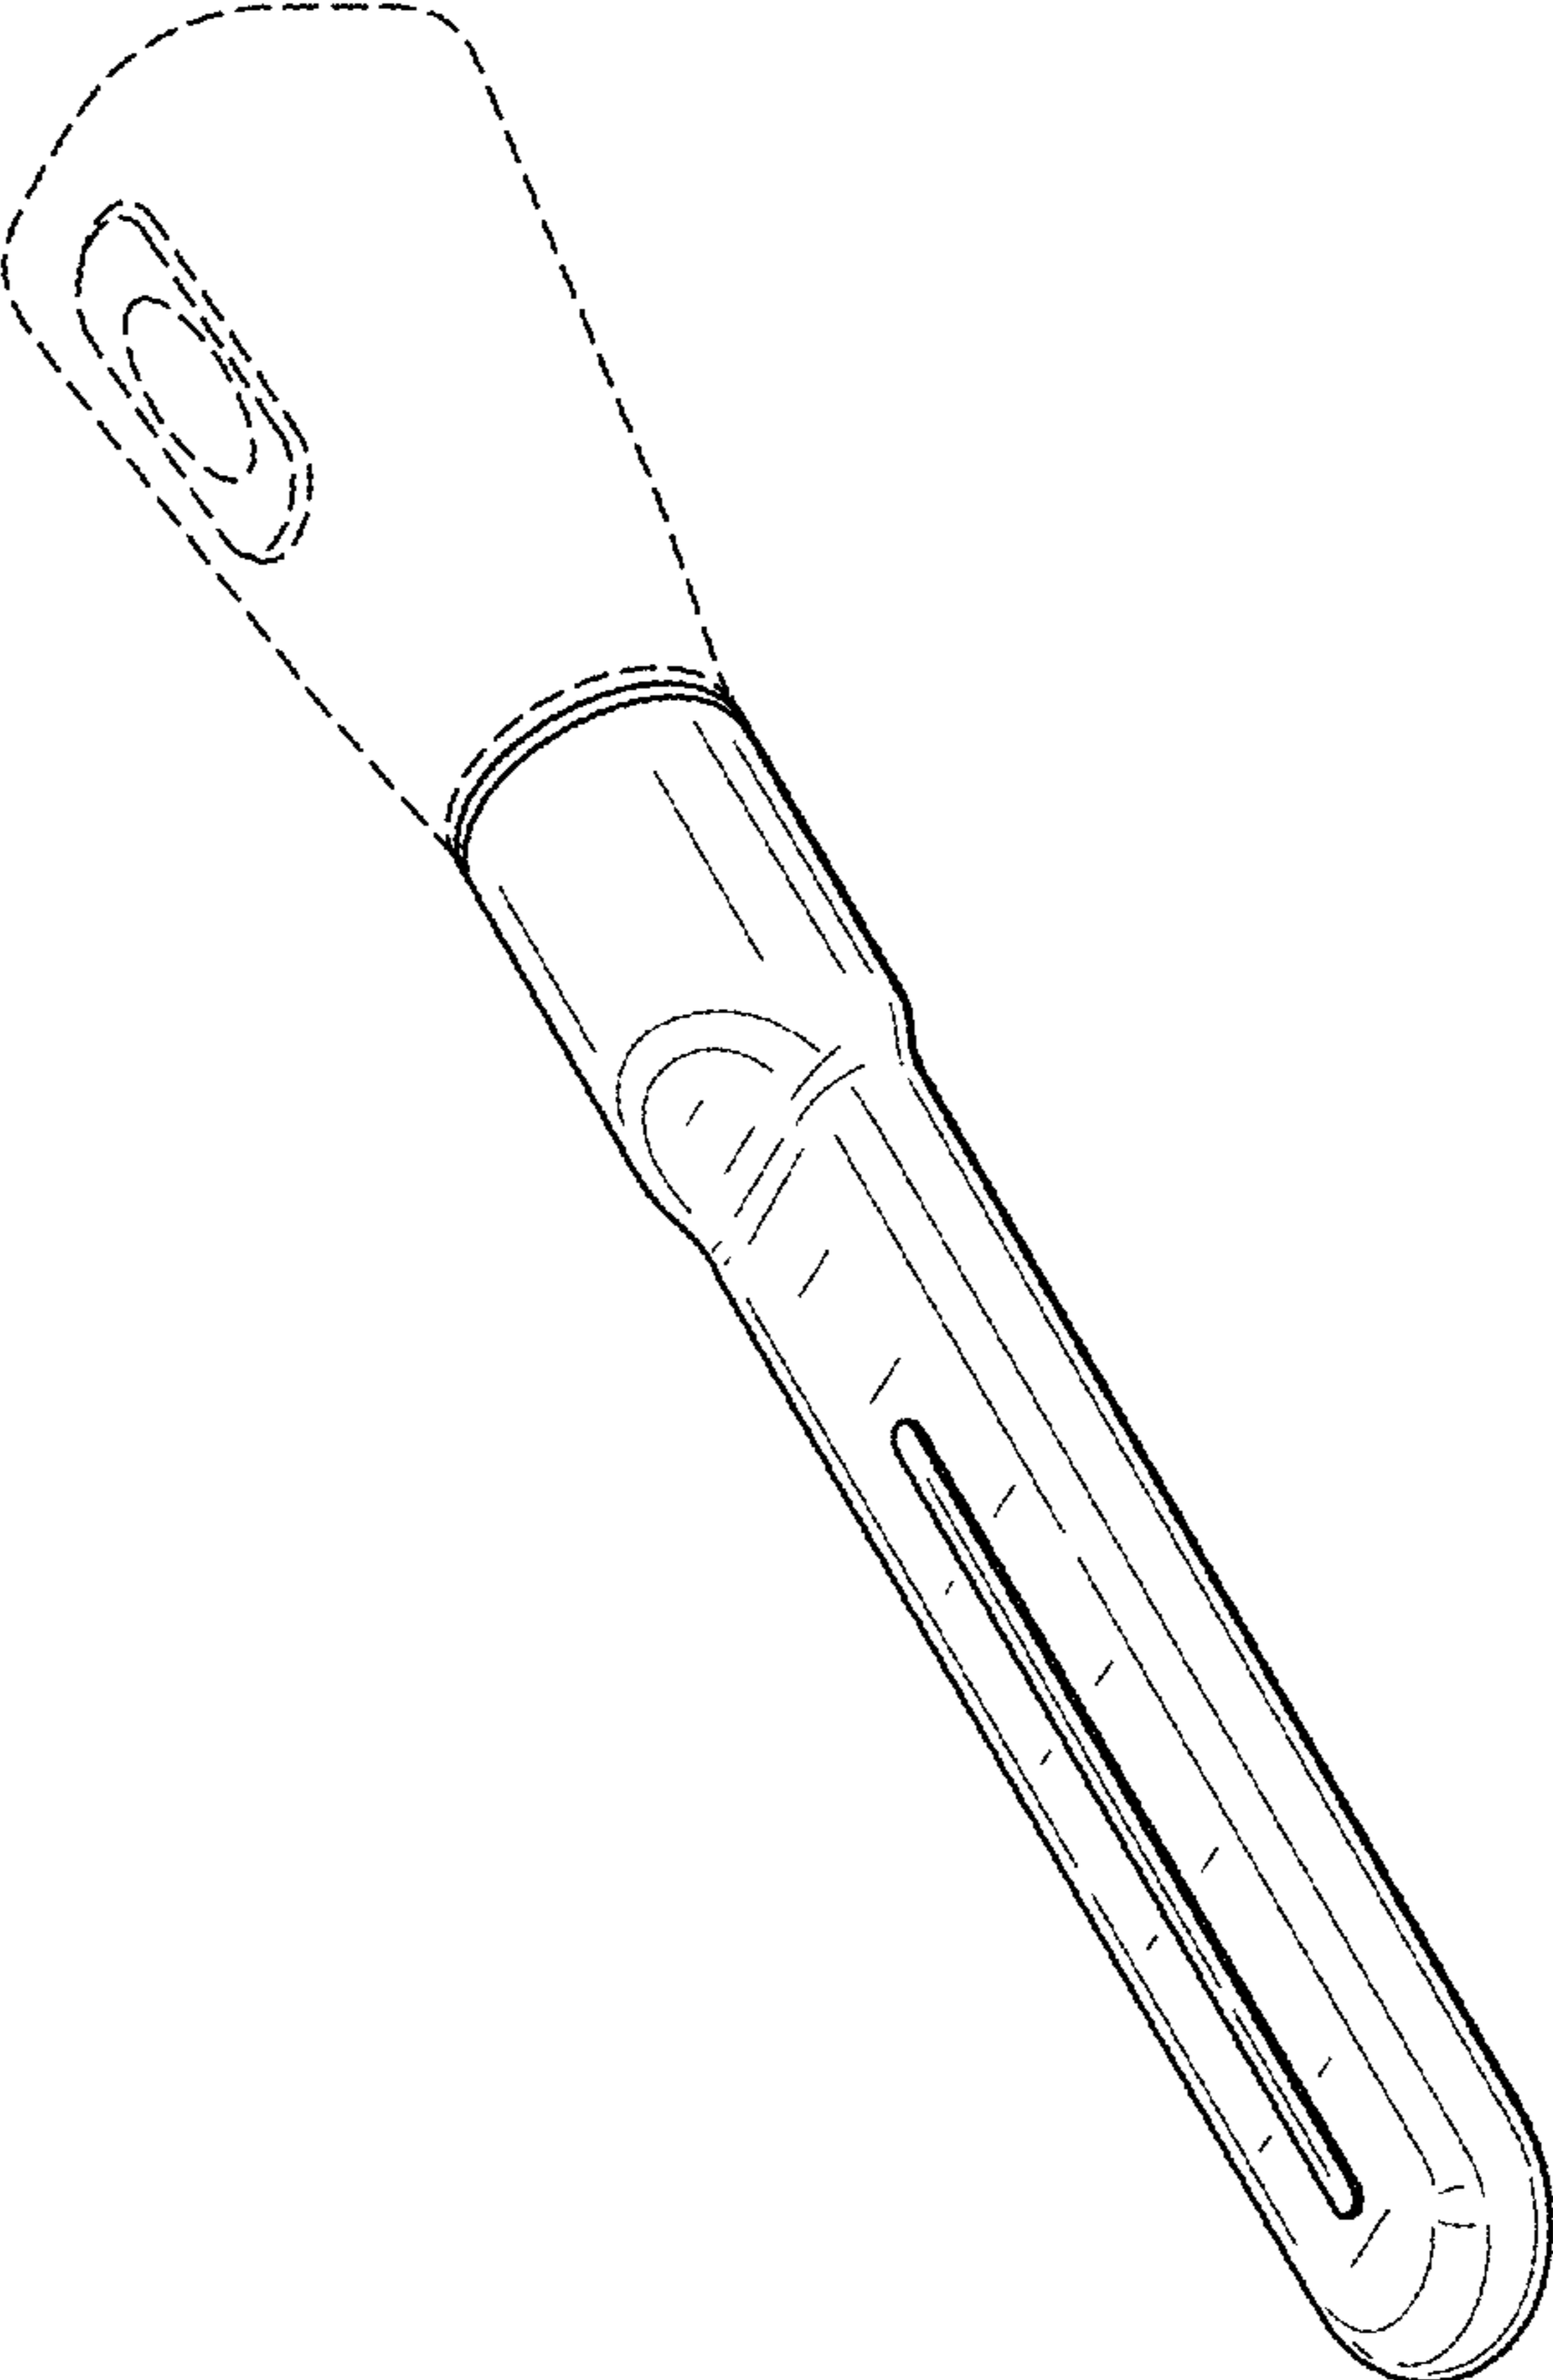


FIG. 2

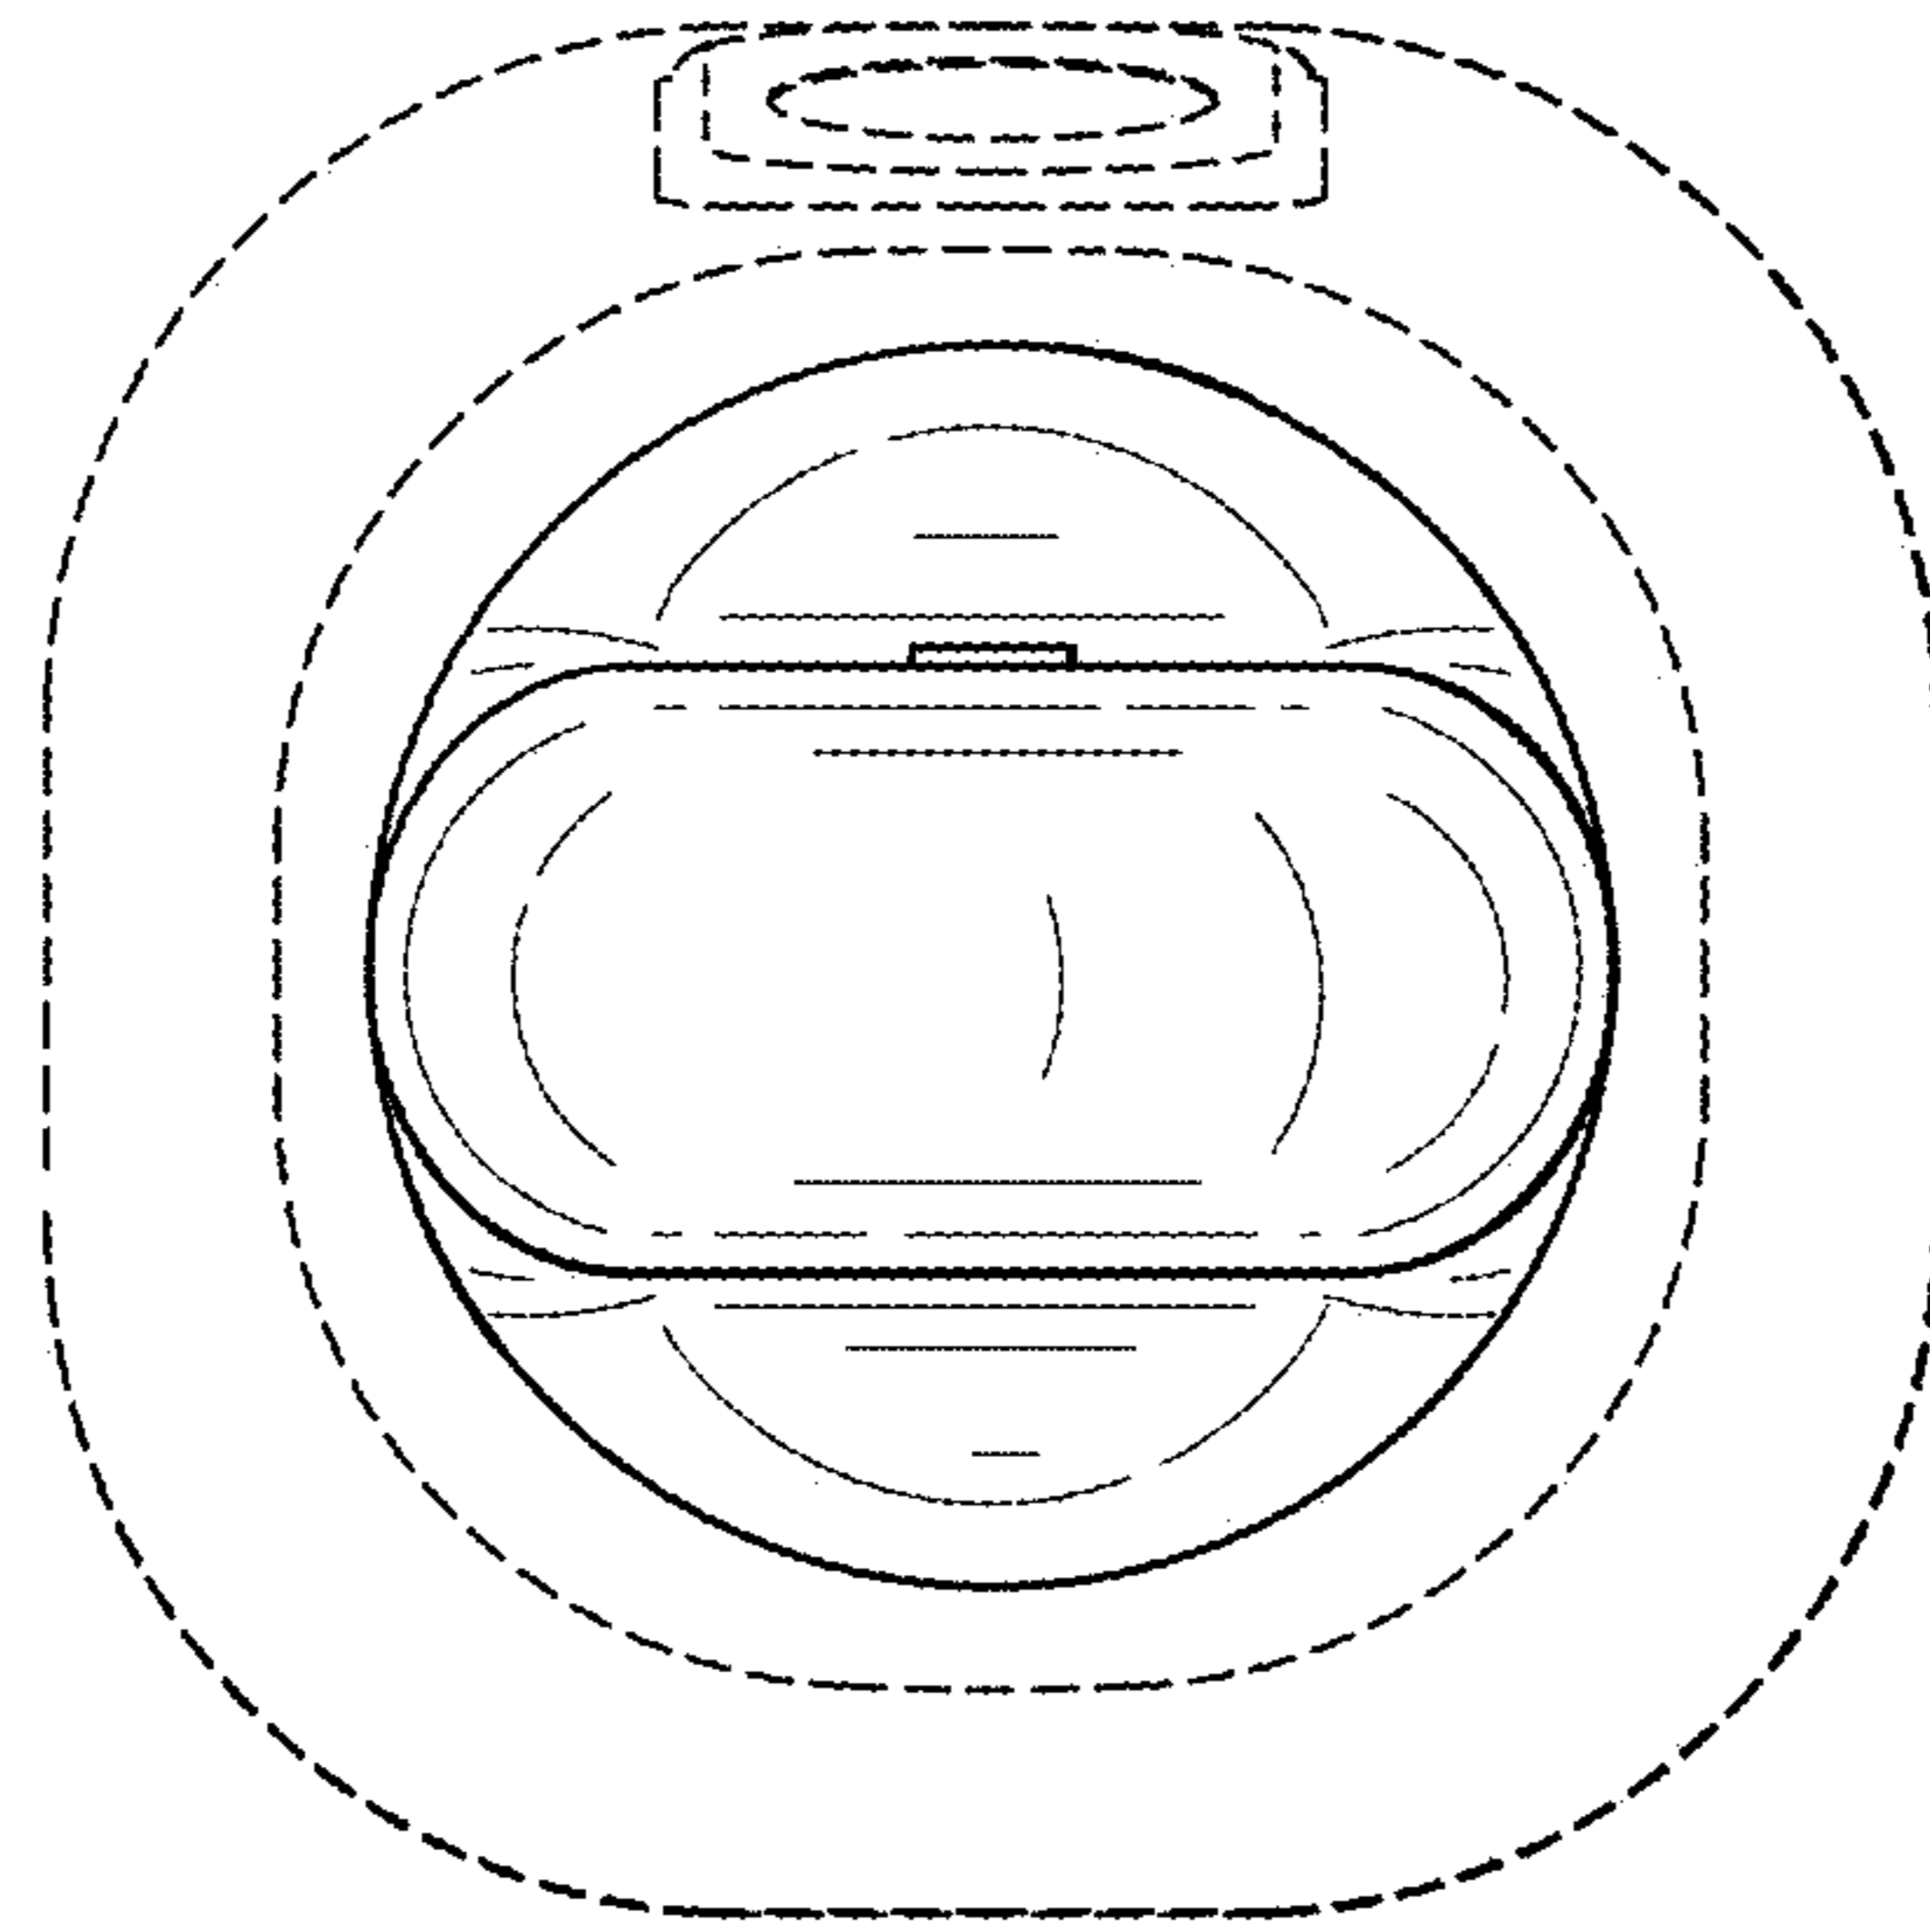


FIG. 3

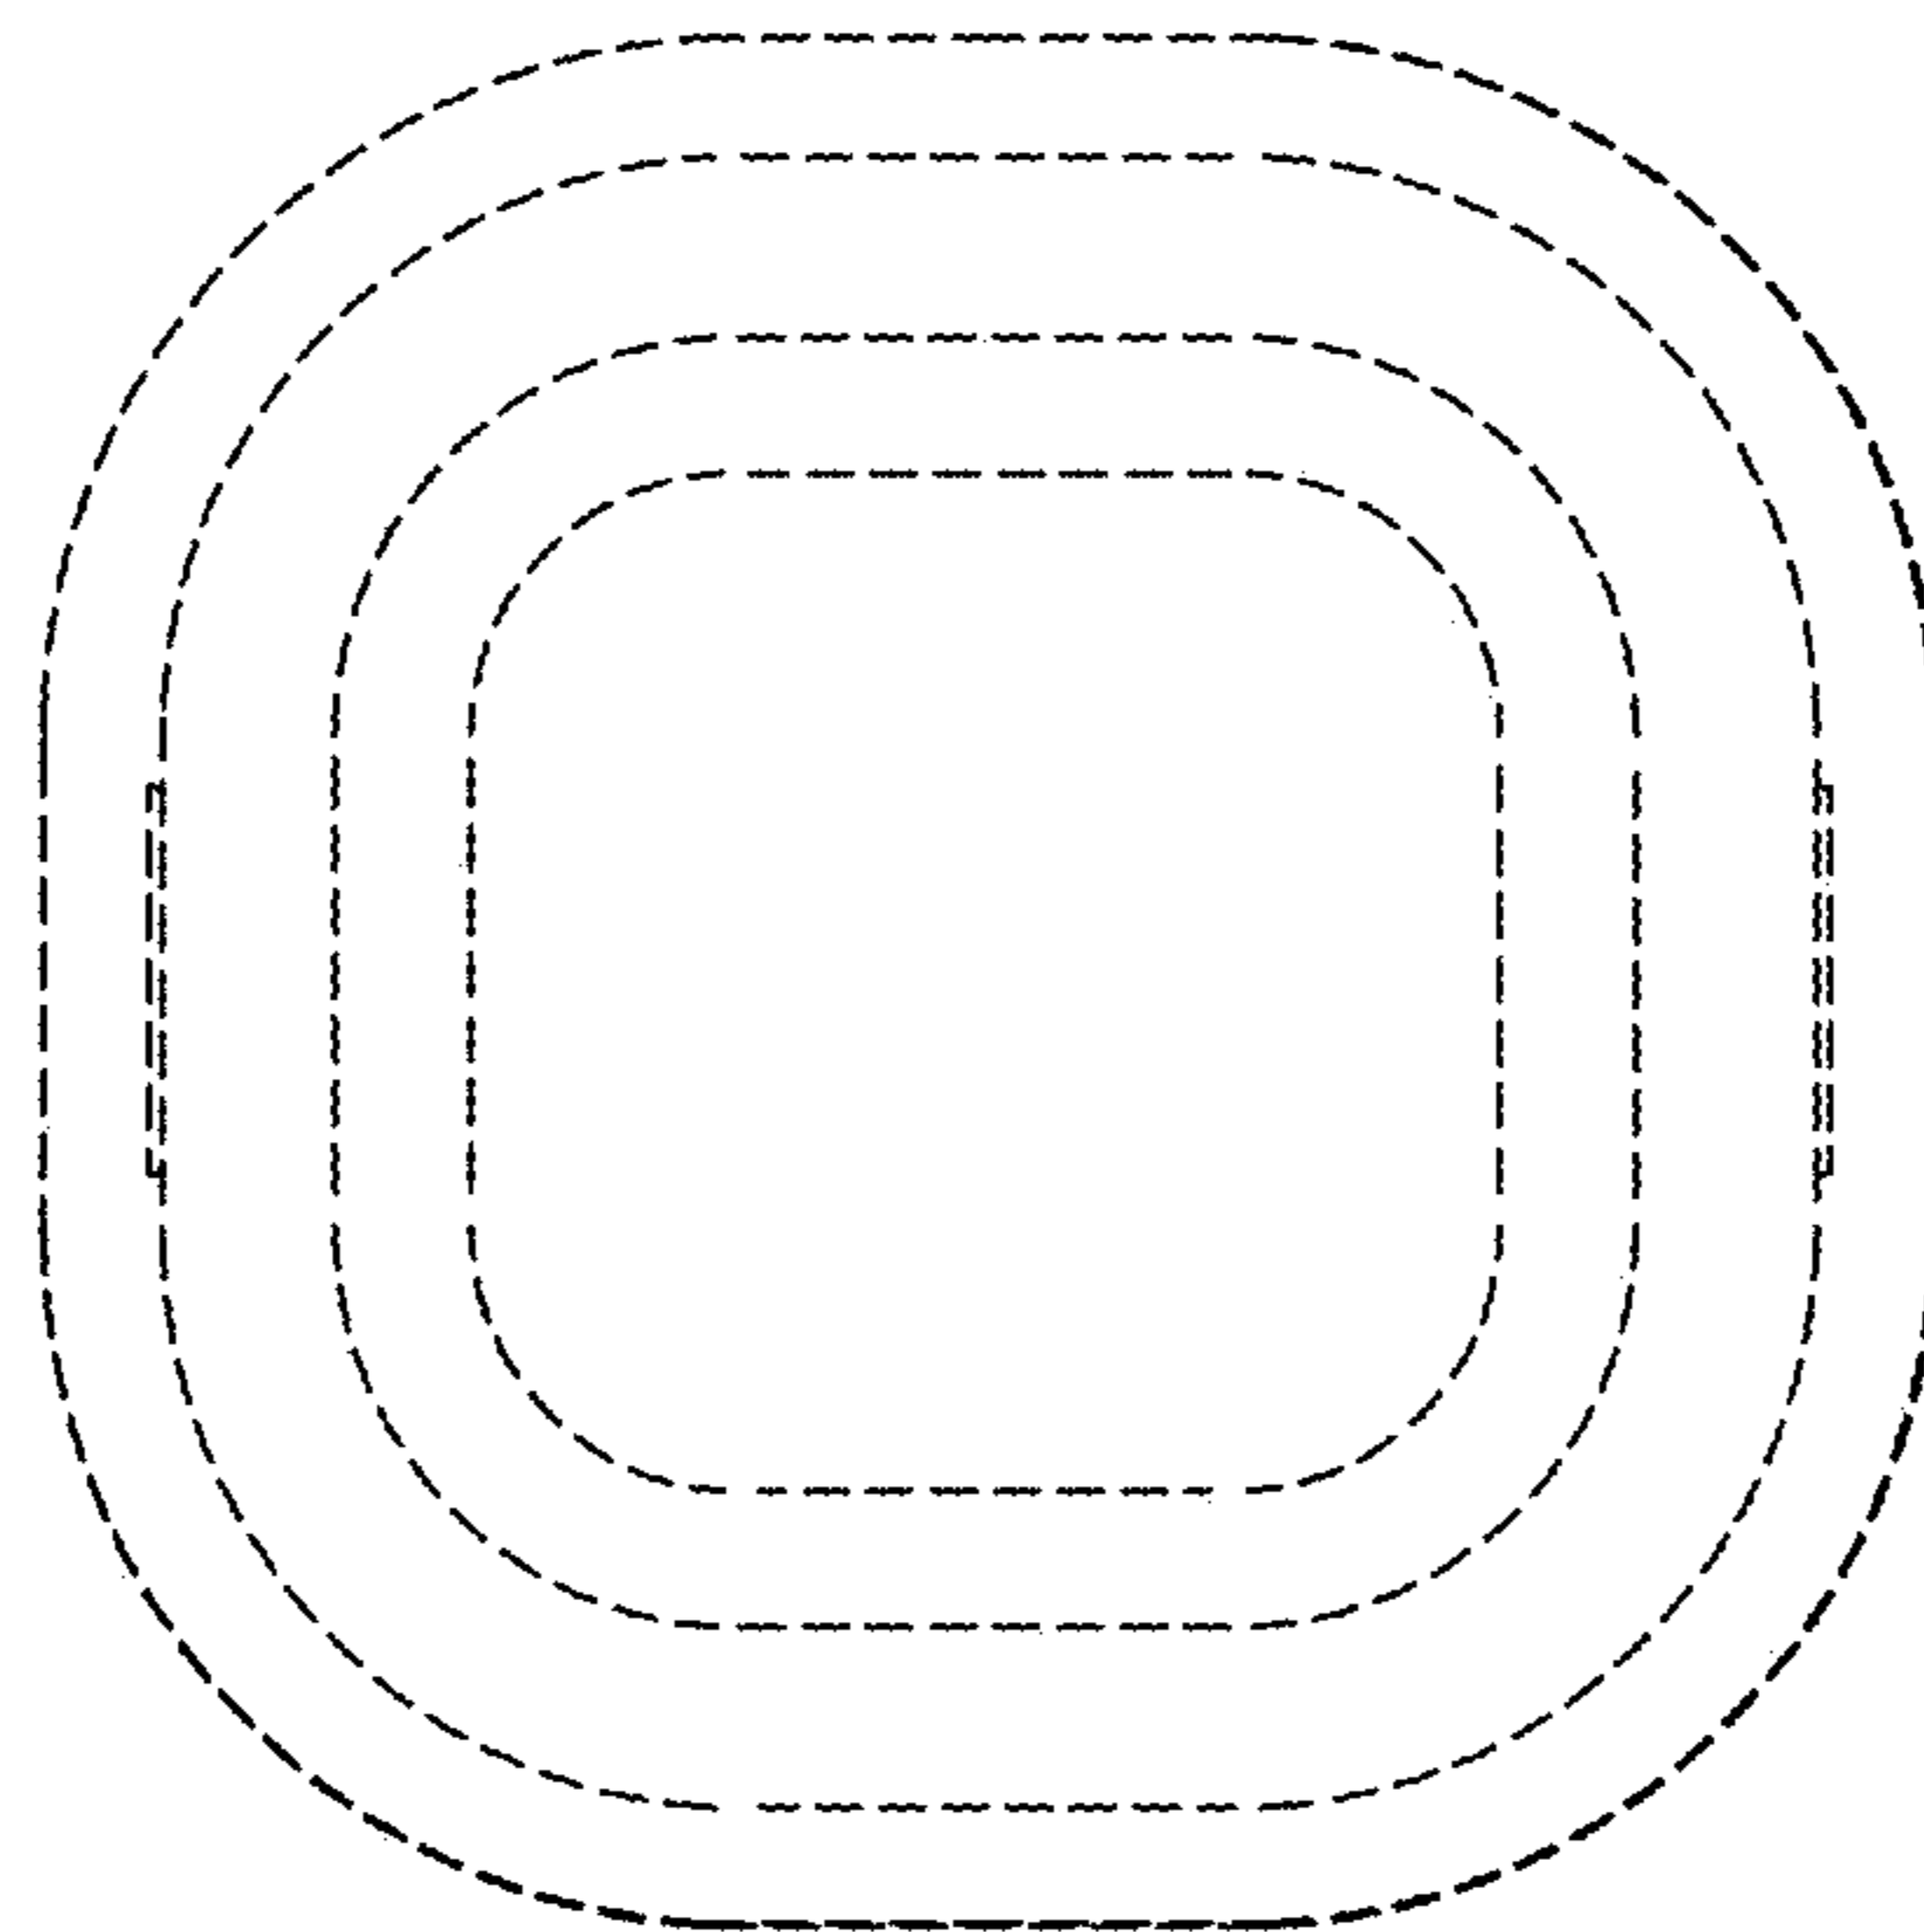


FIG. 4

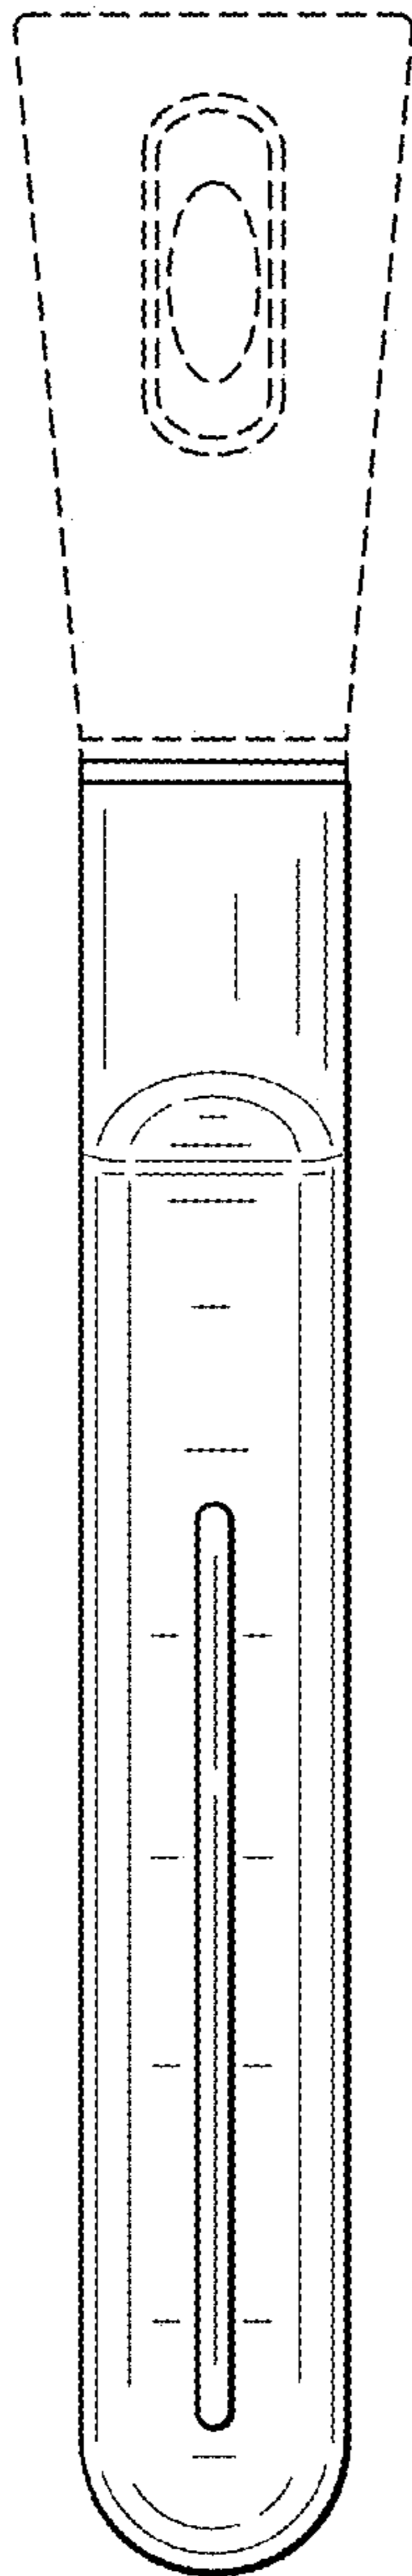


FIG. 5

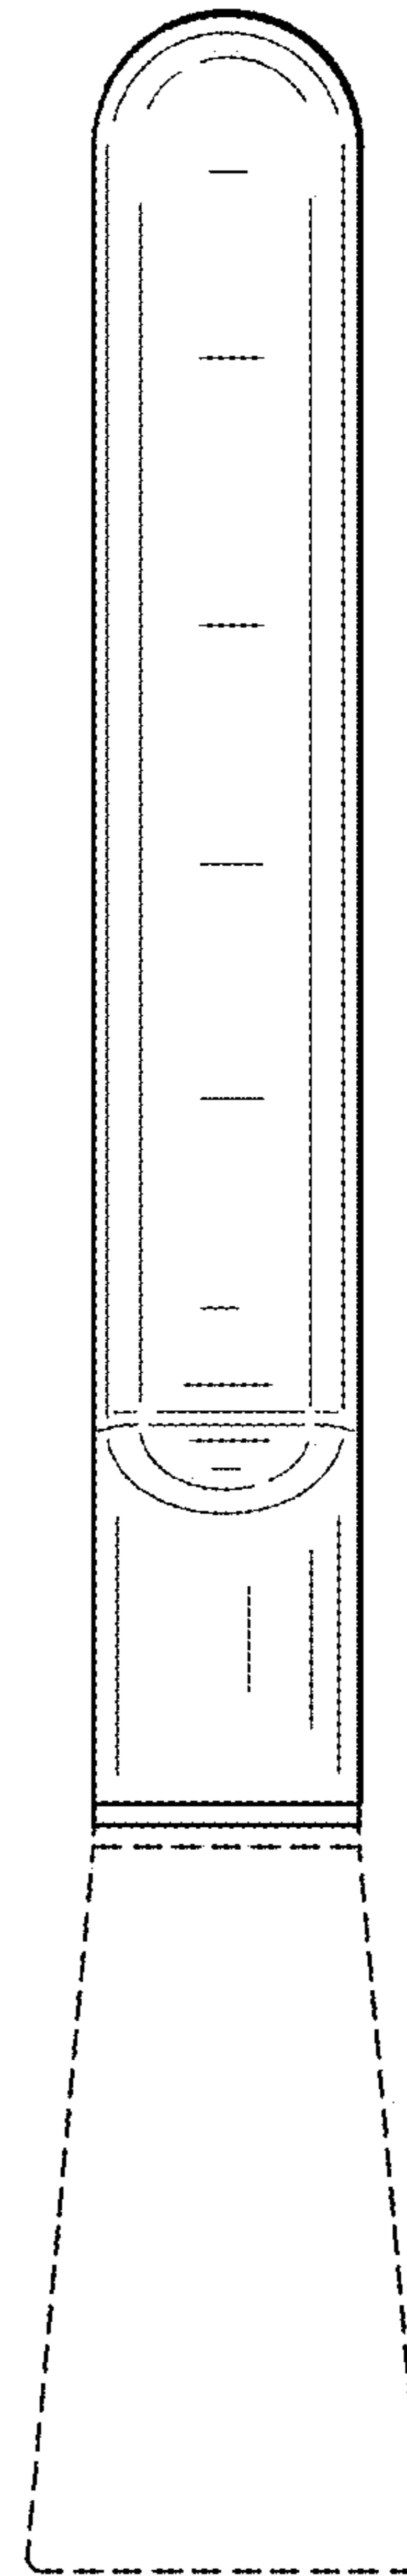


FIG. 6

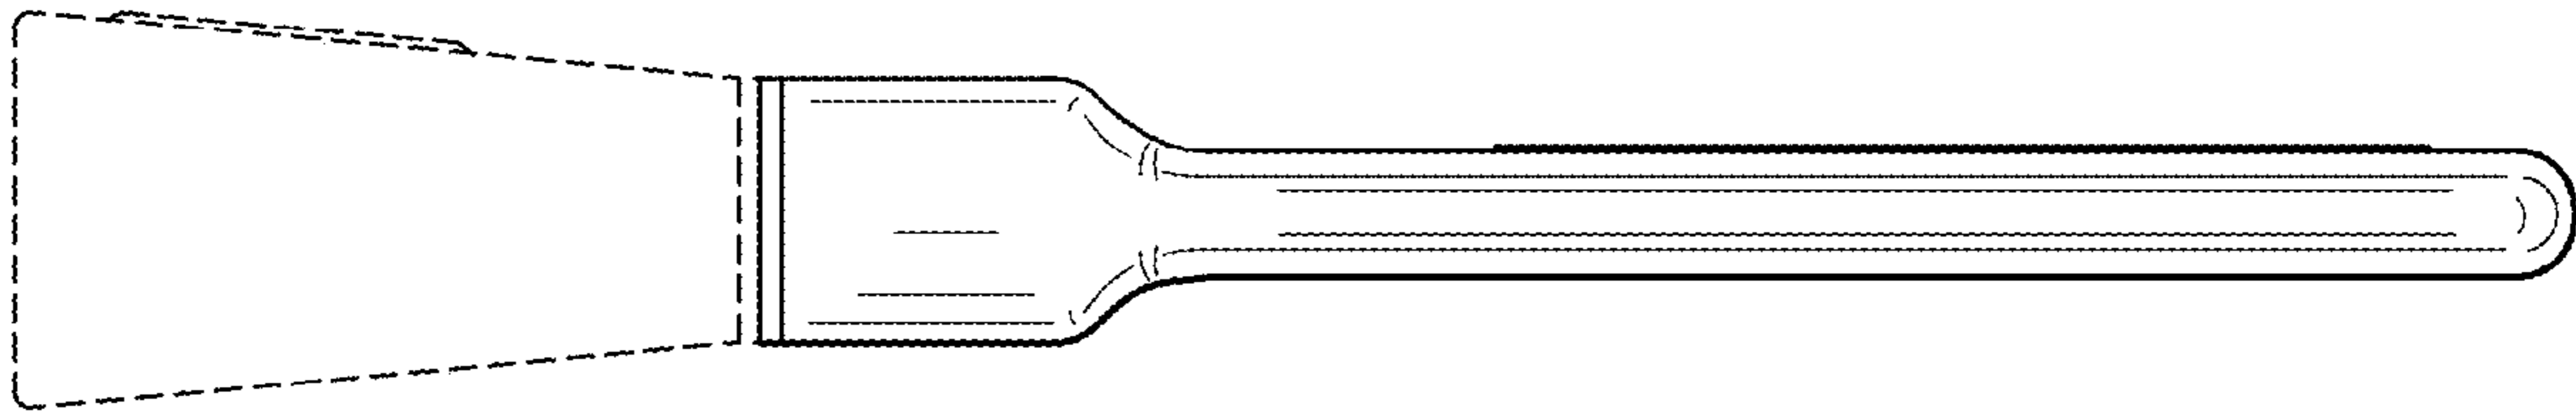


FIG. 7

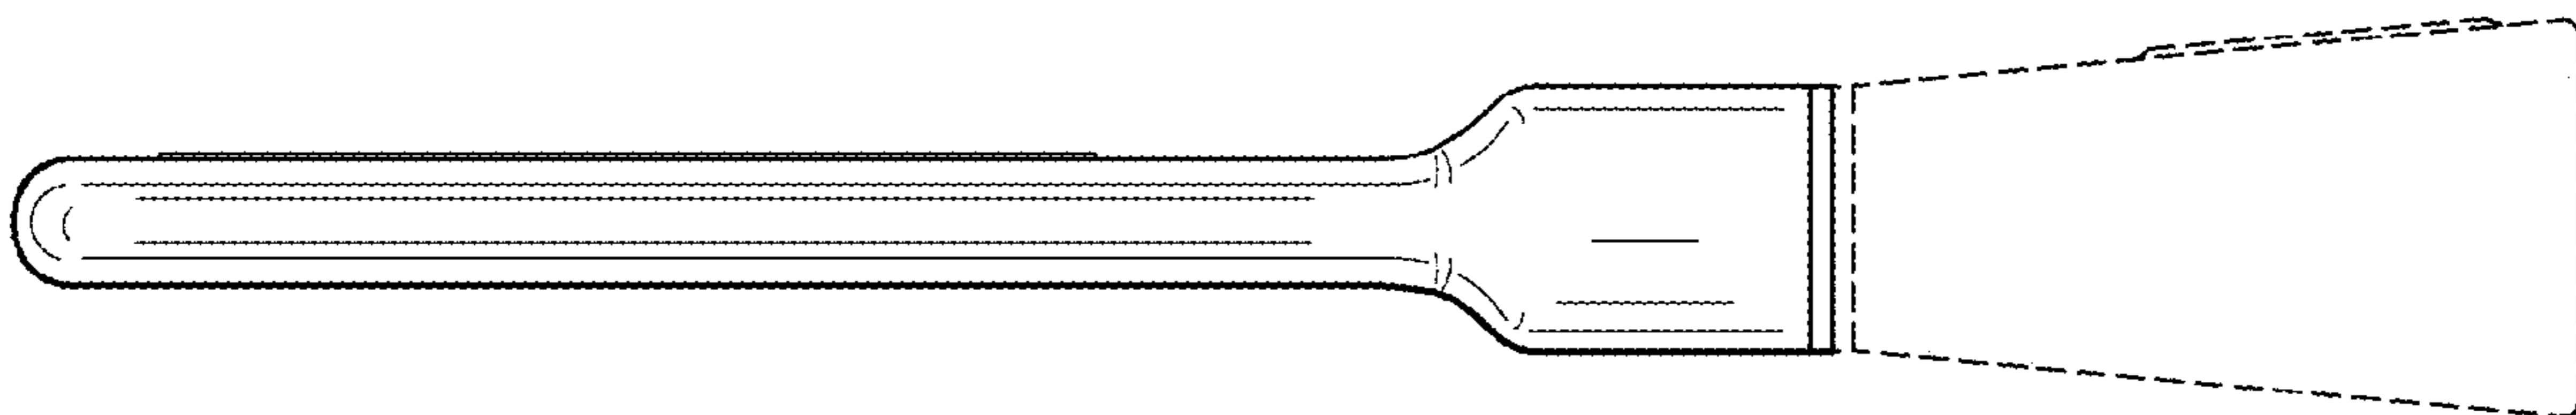
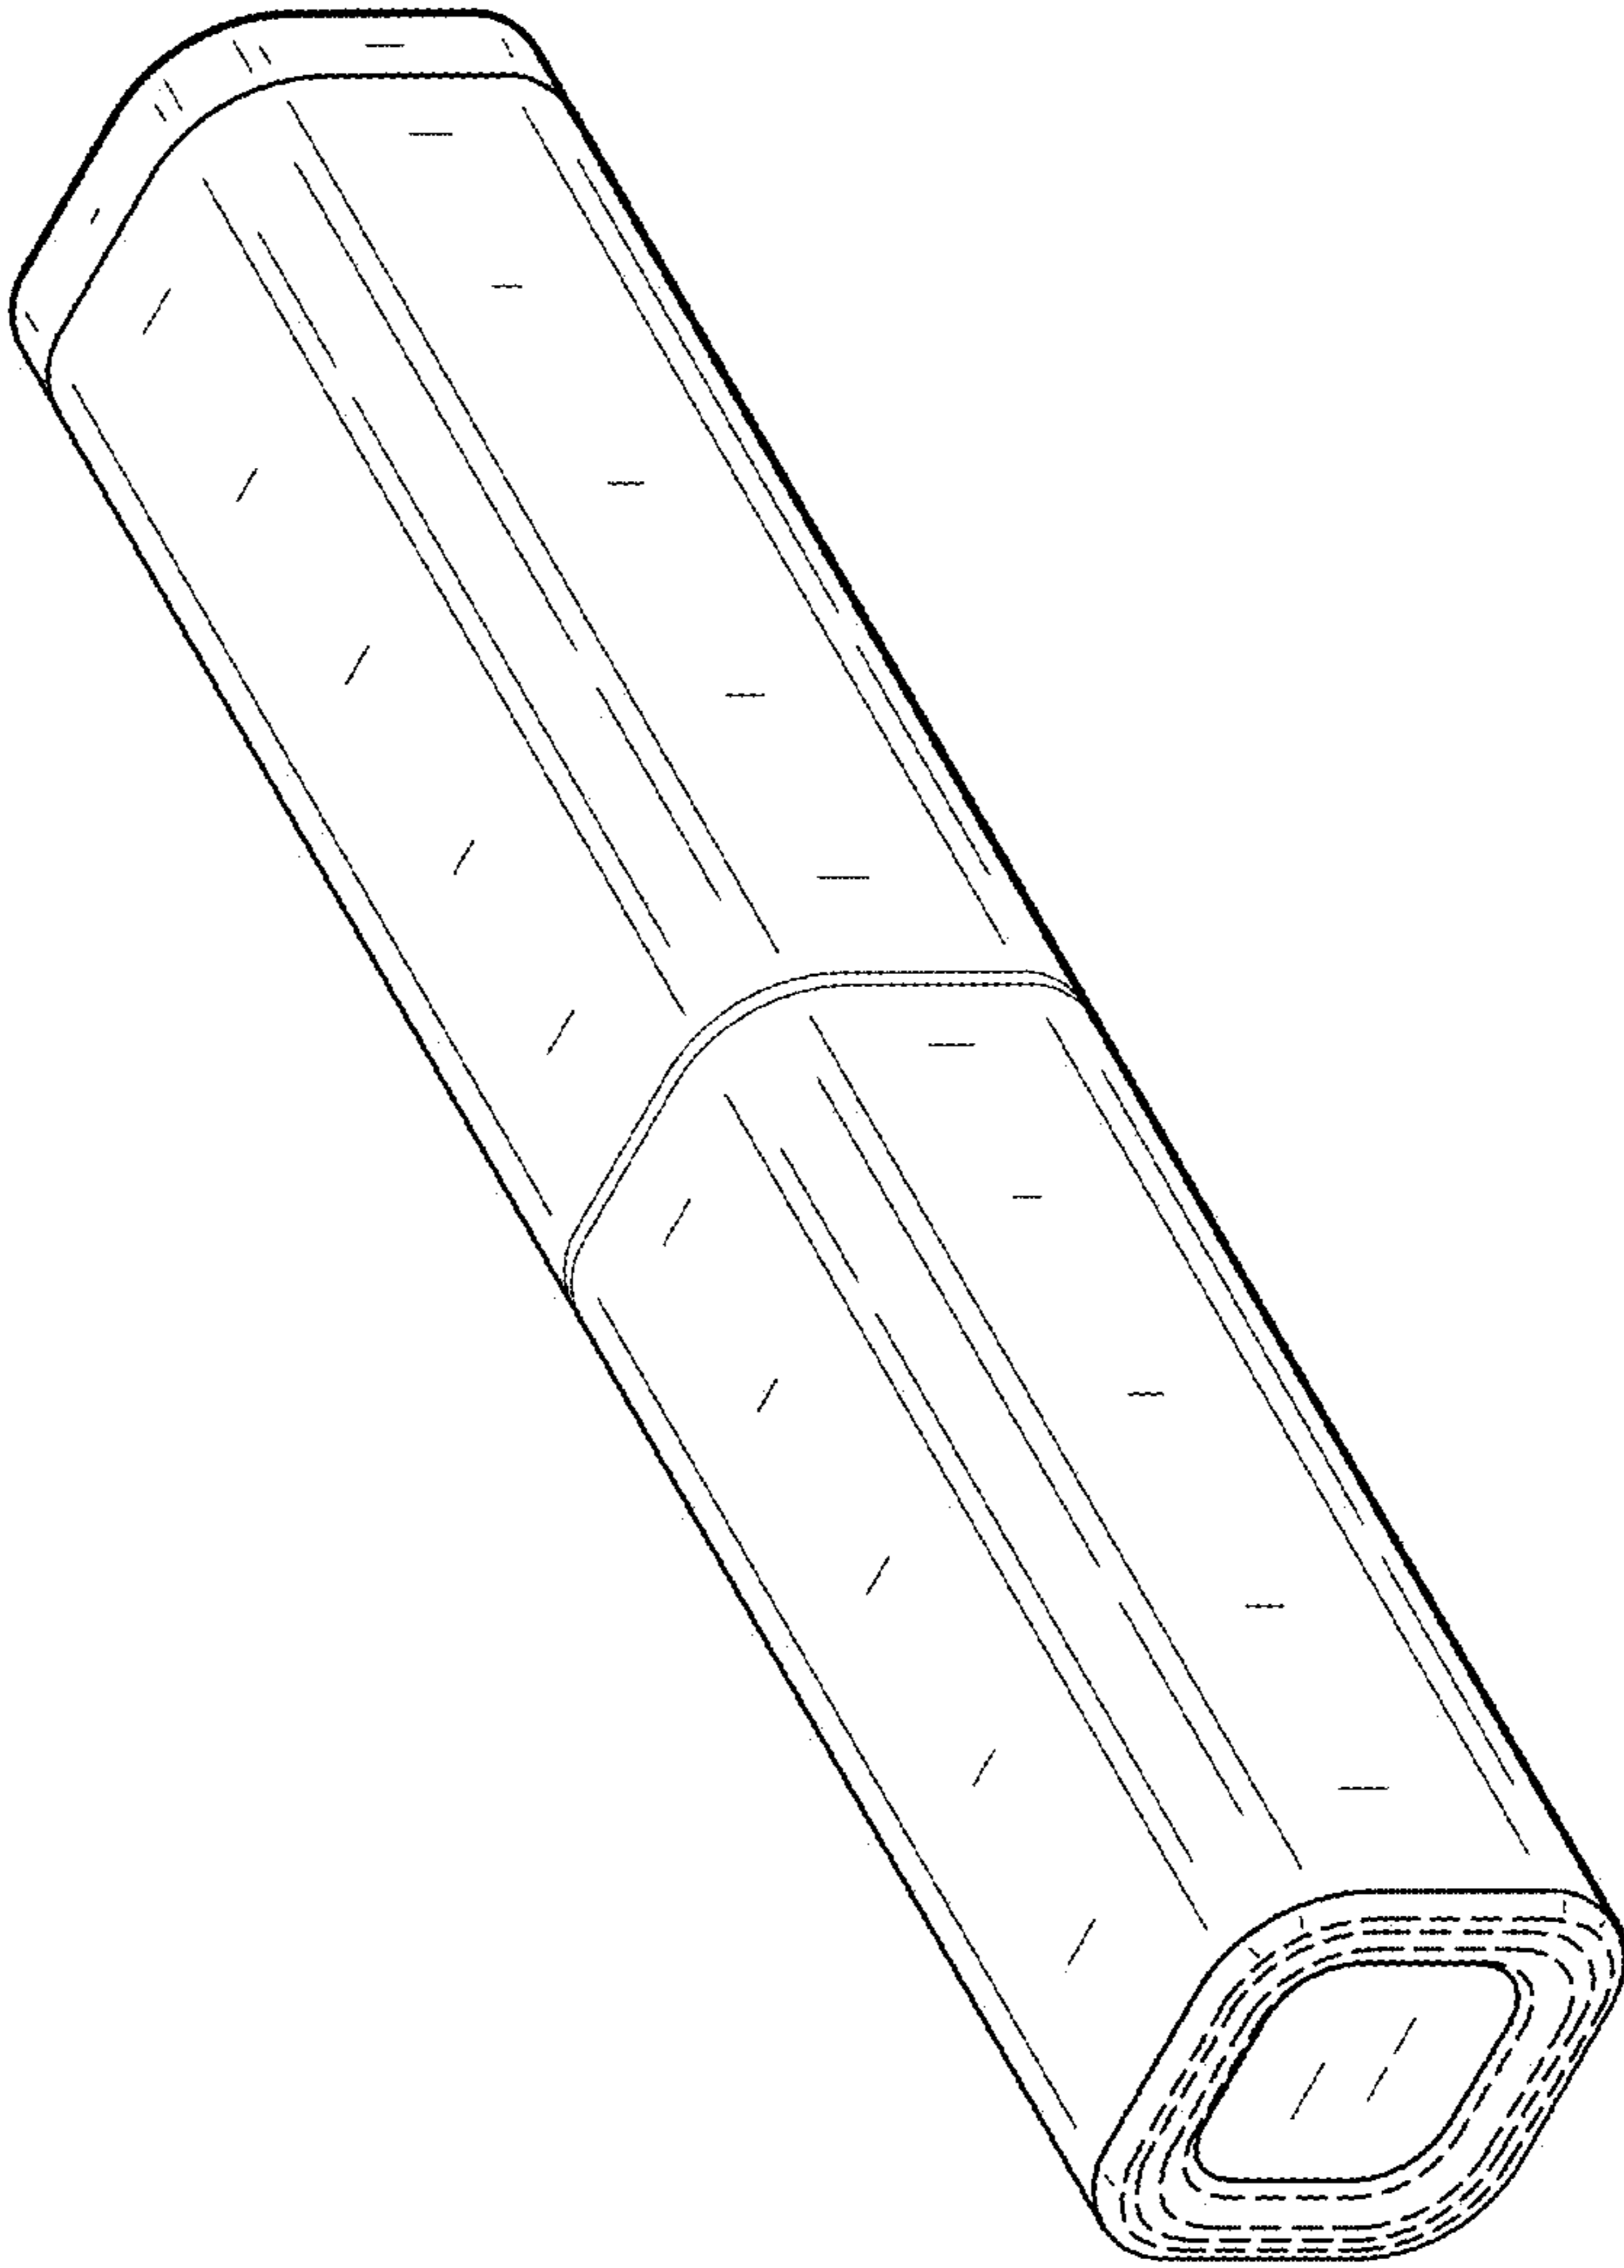


FIG. 8



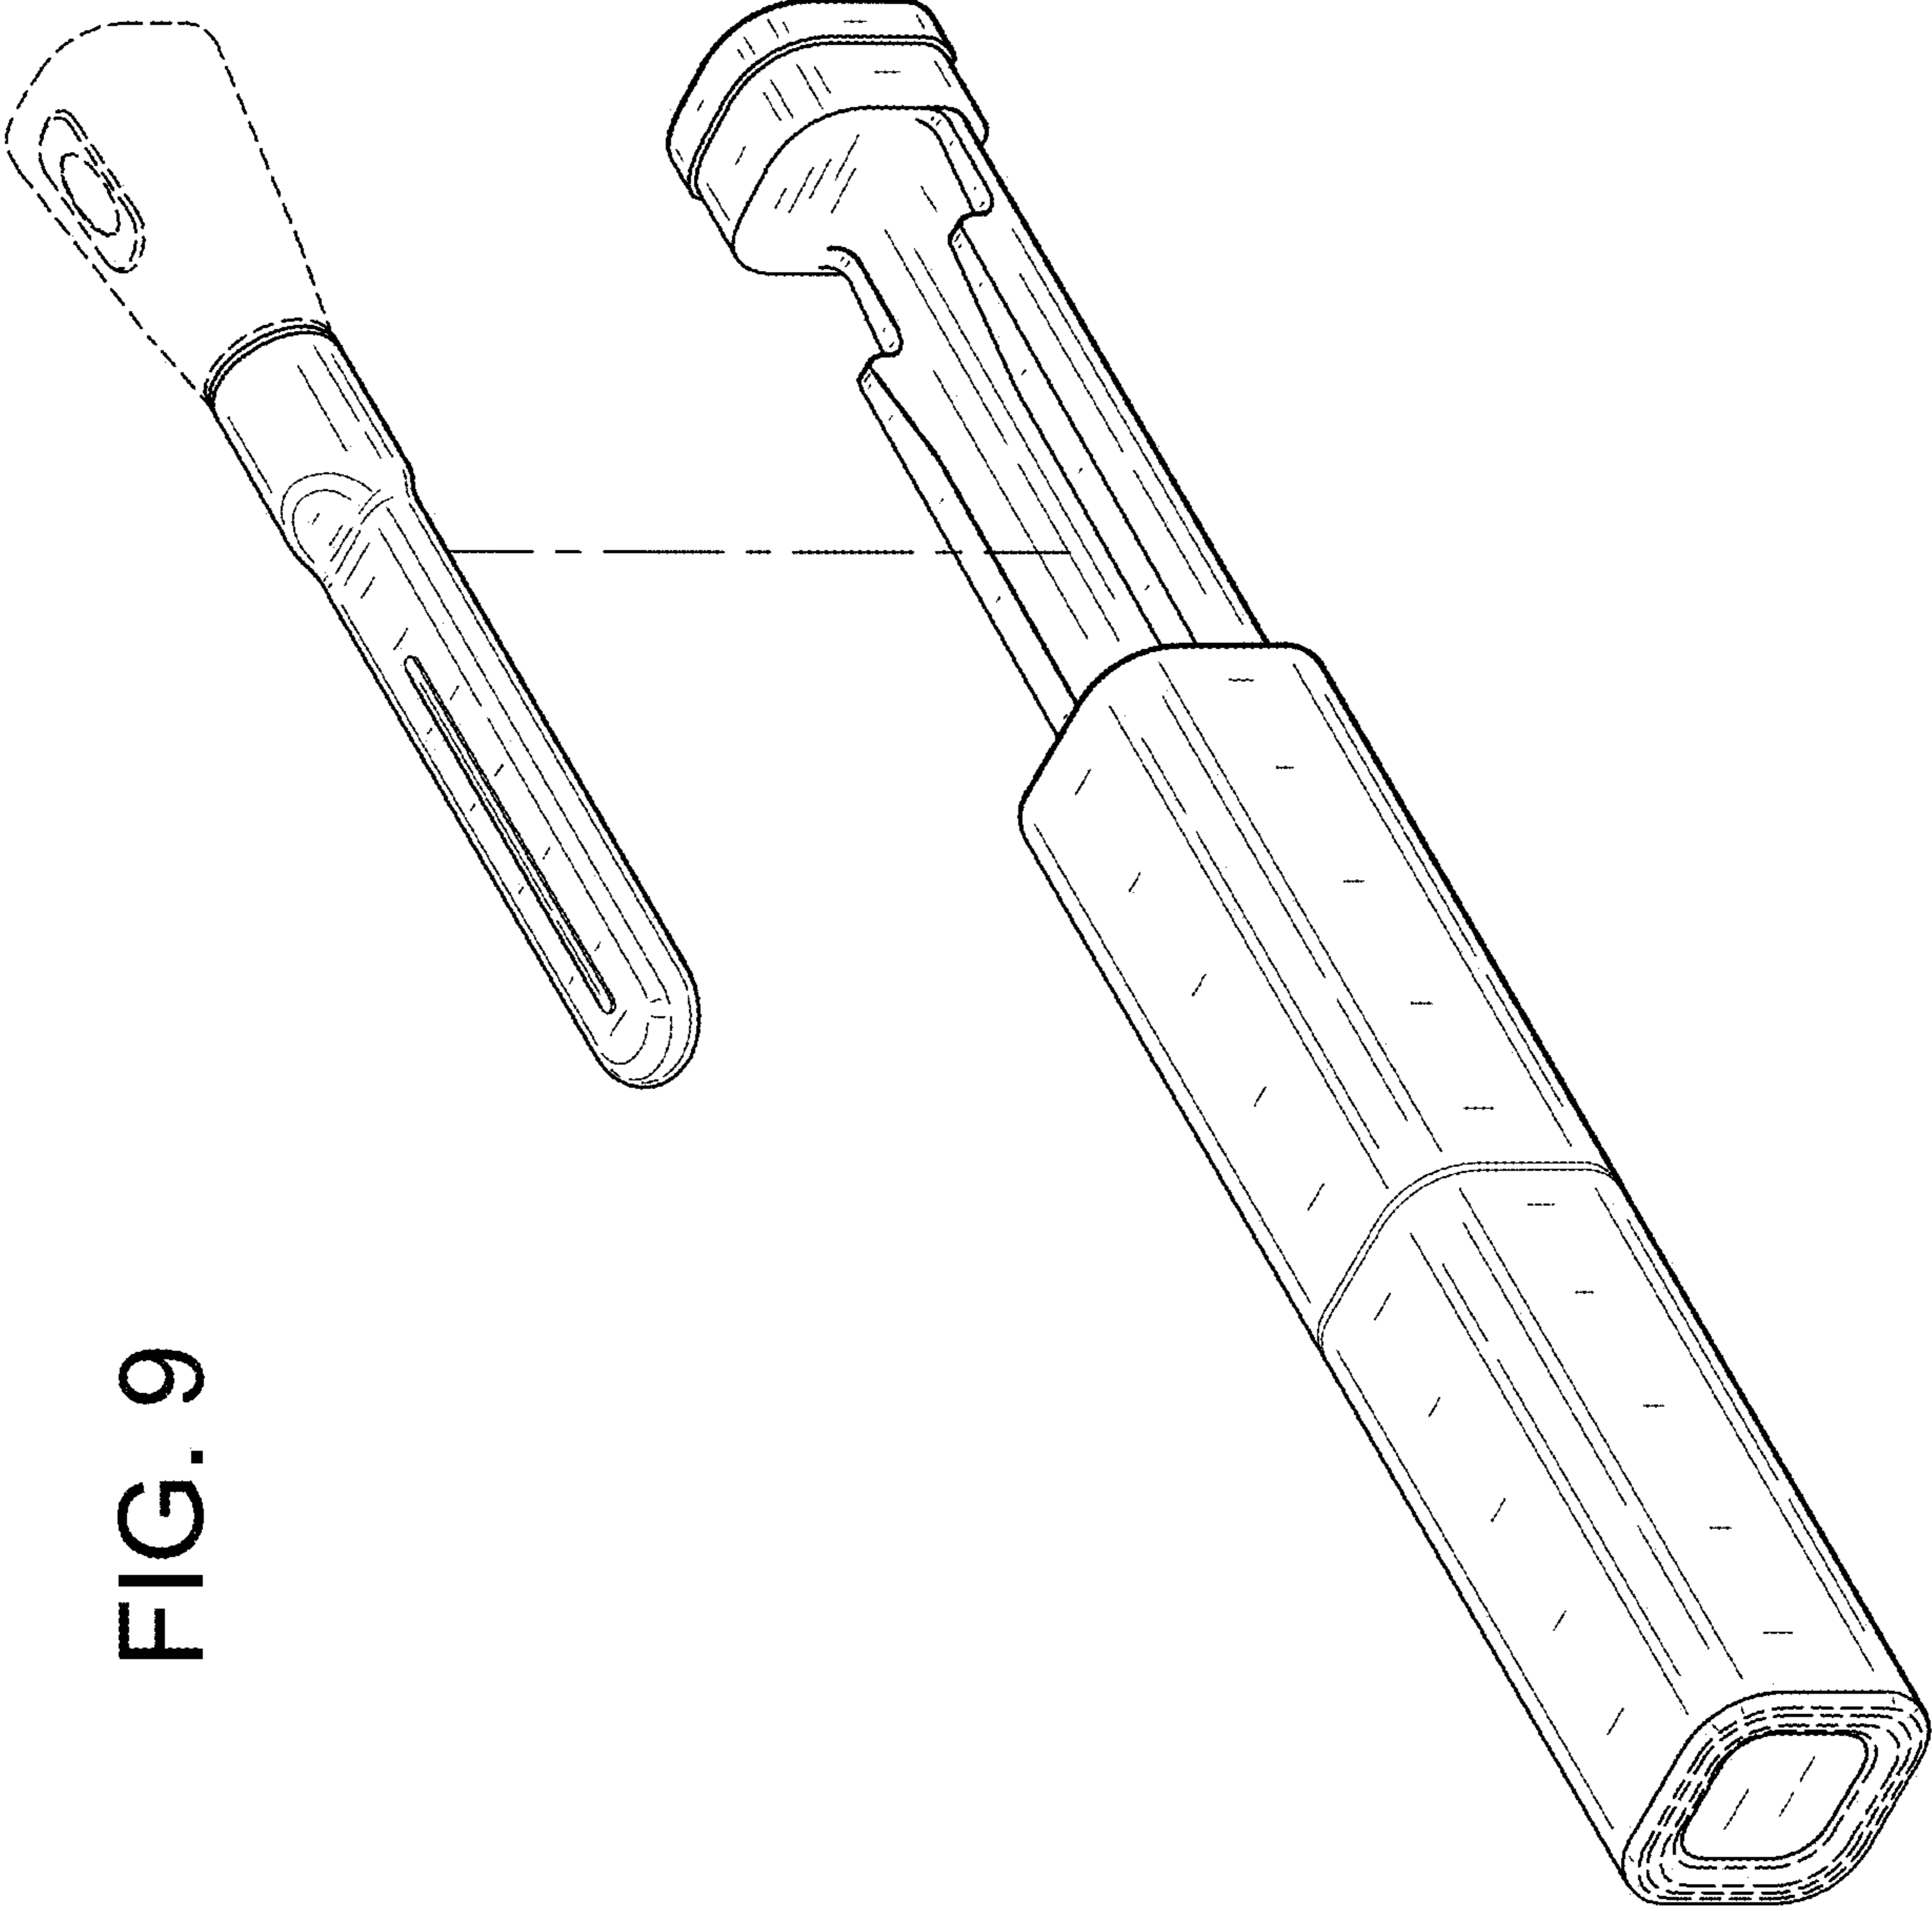


FIG. 9

FIG. 10

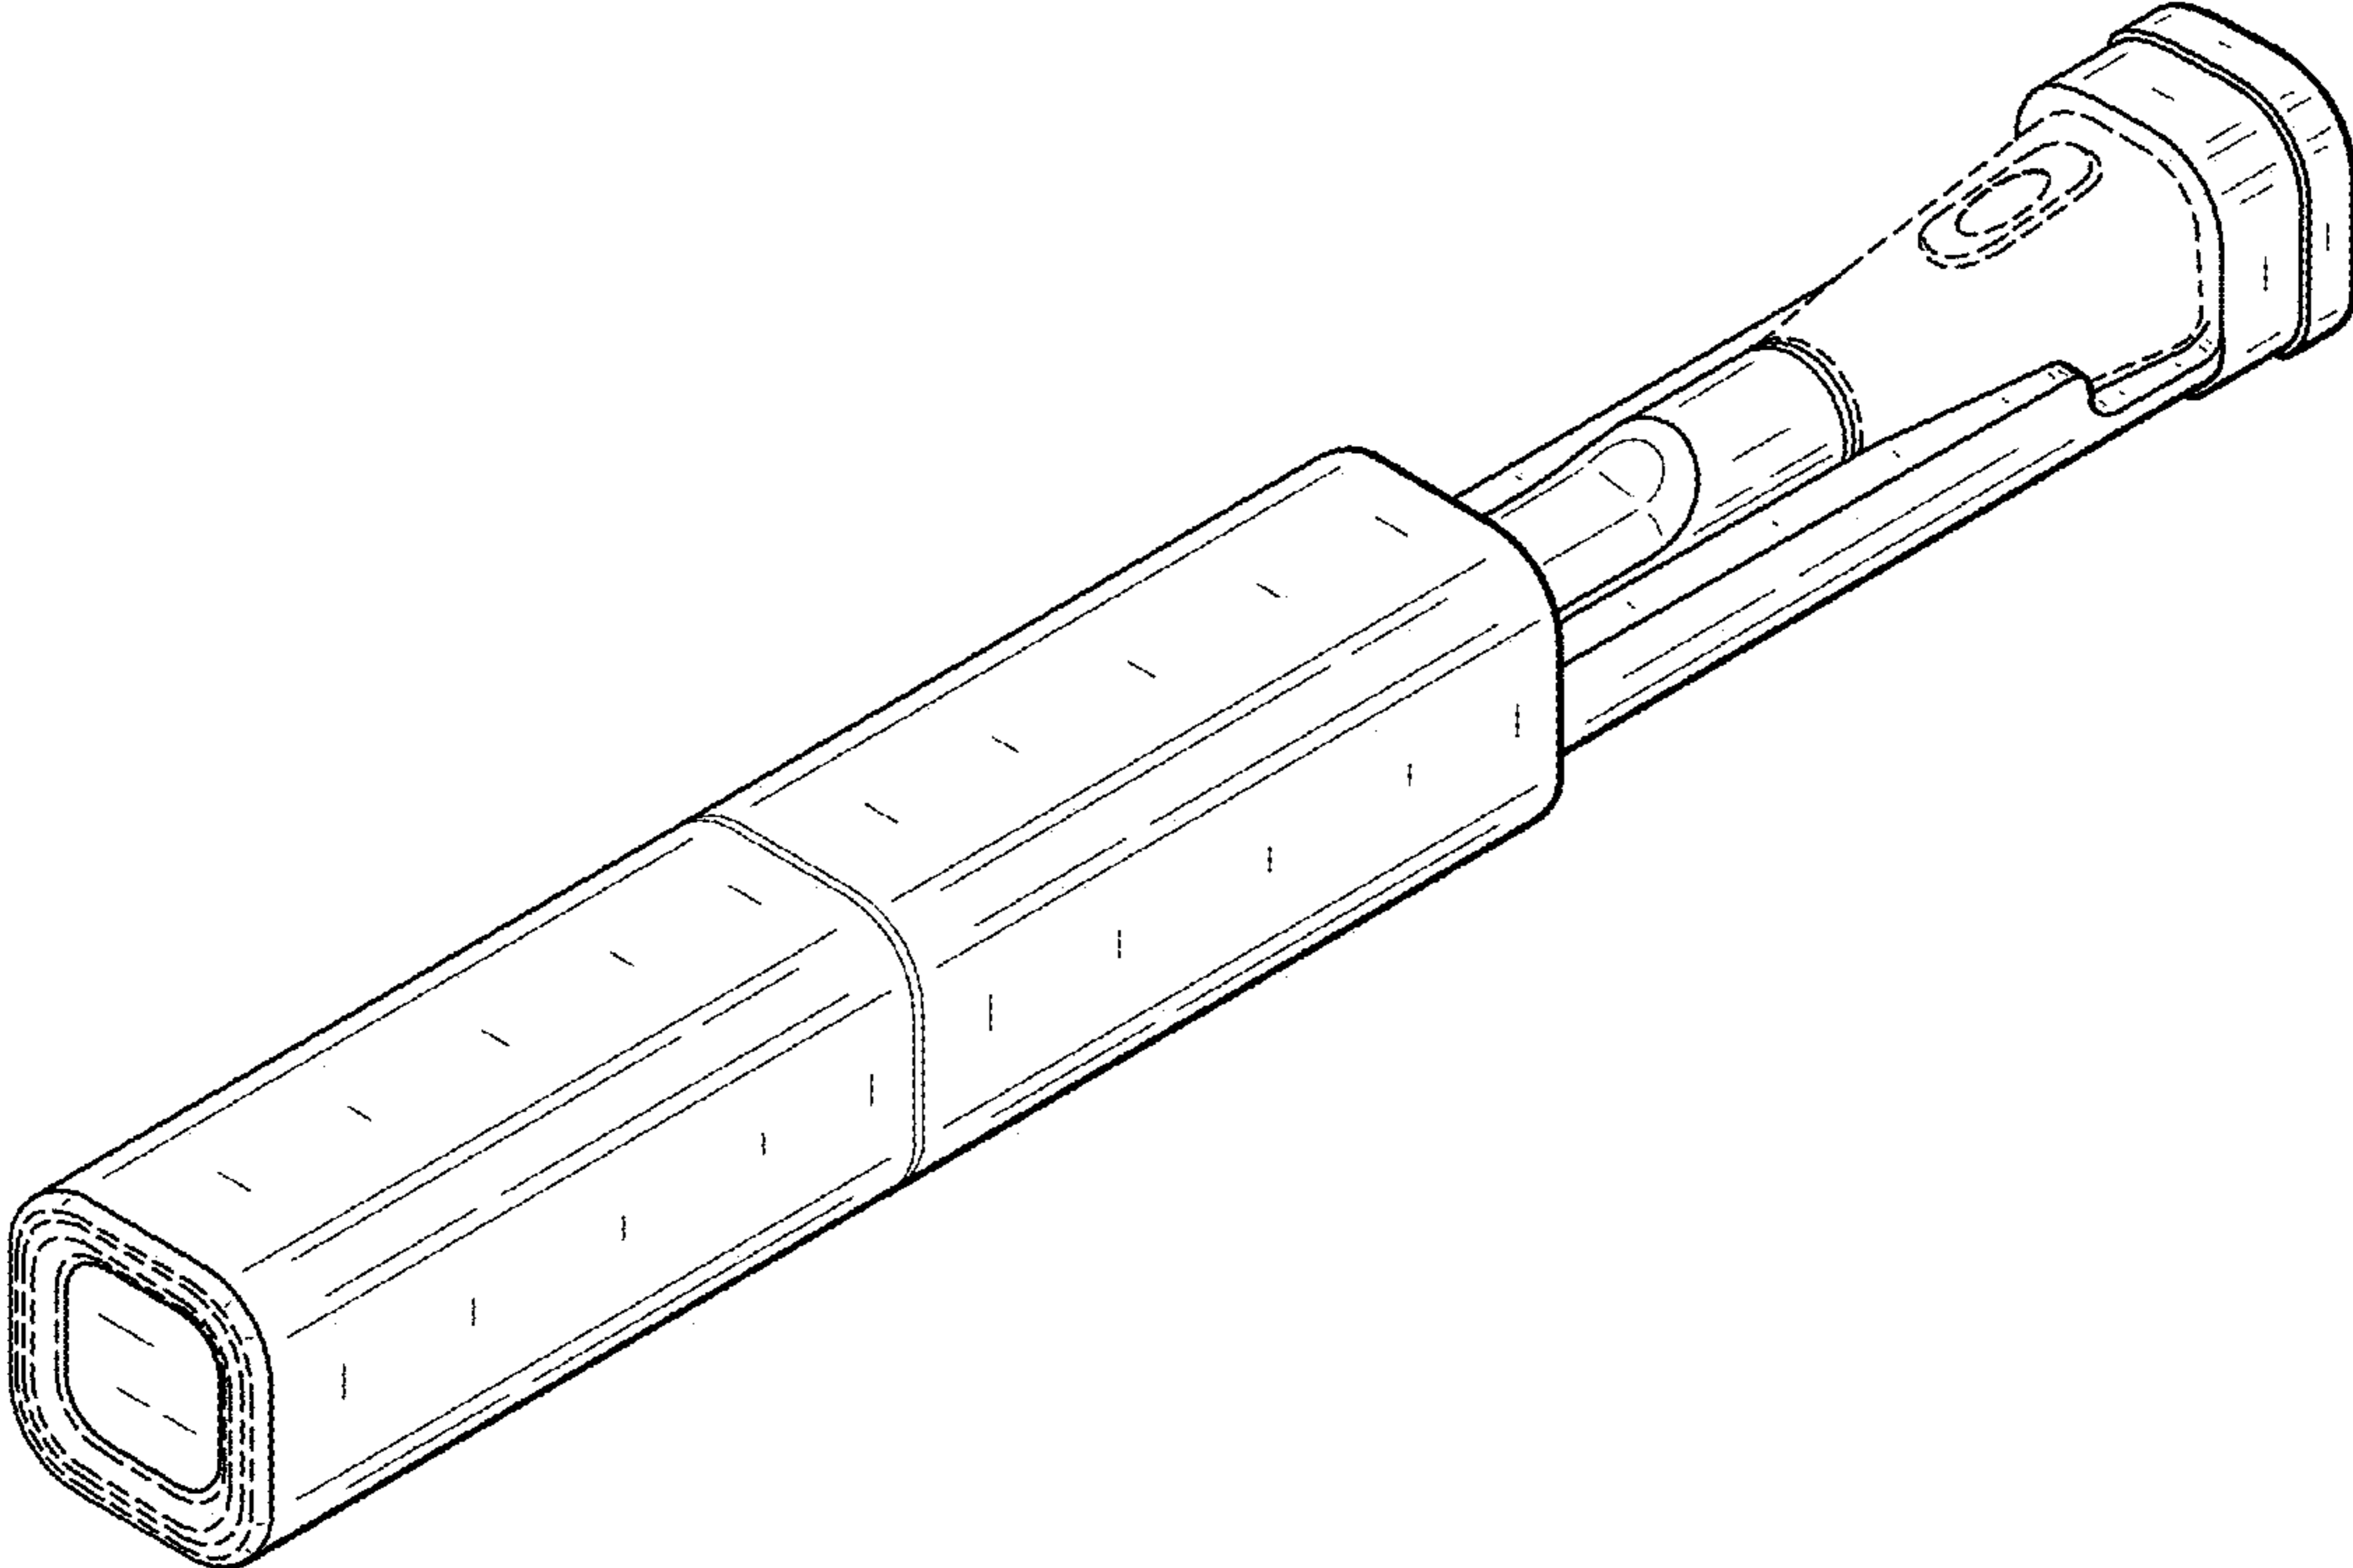


FIG. 11

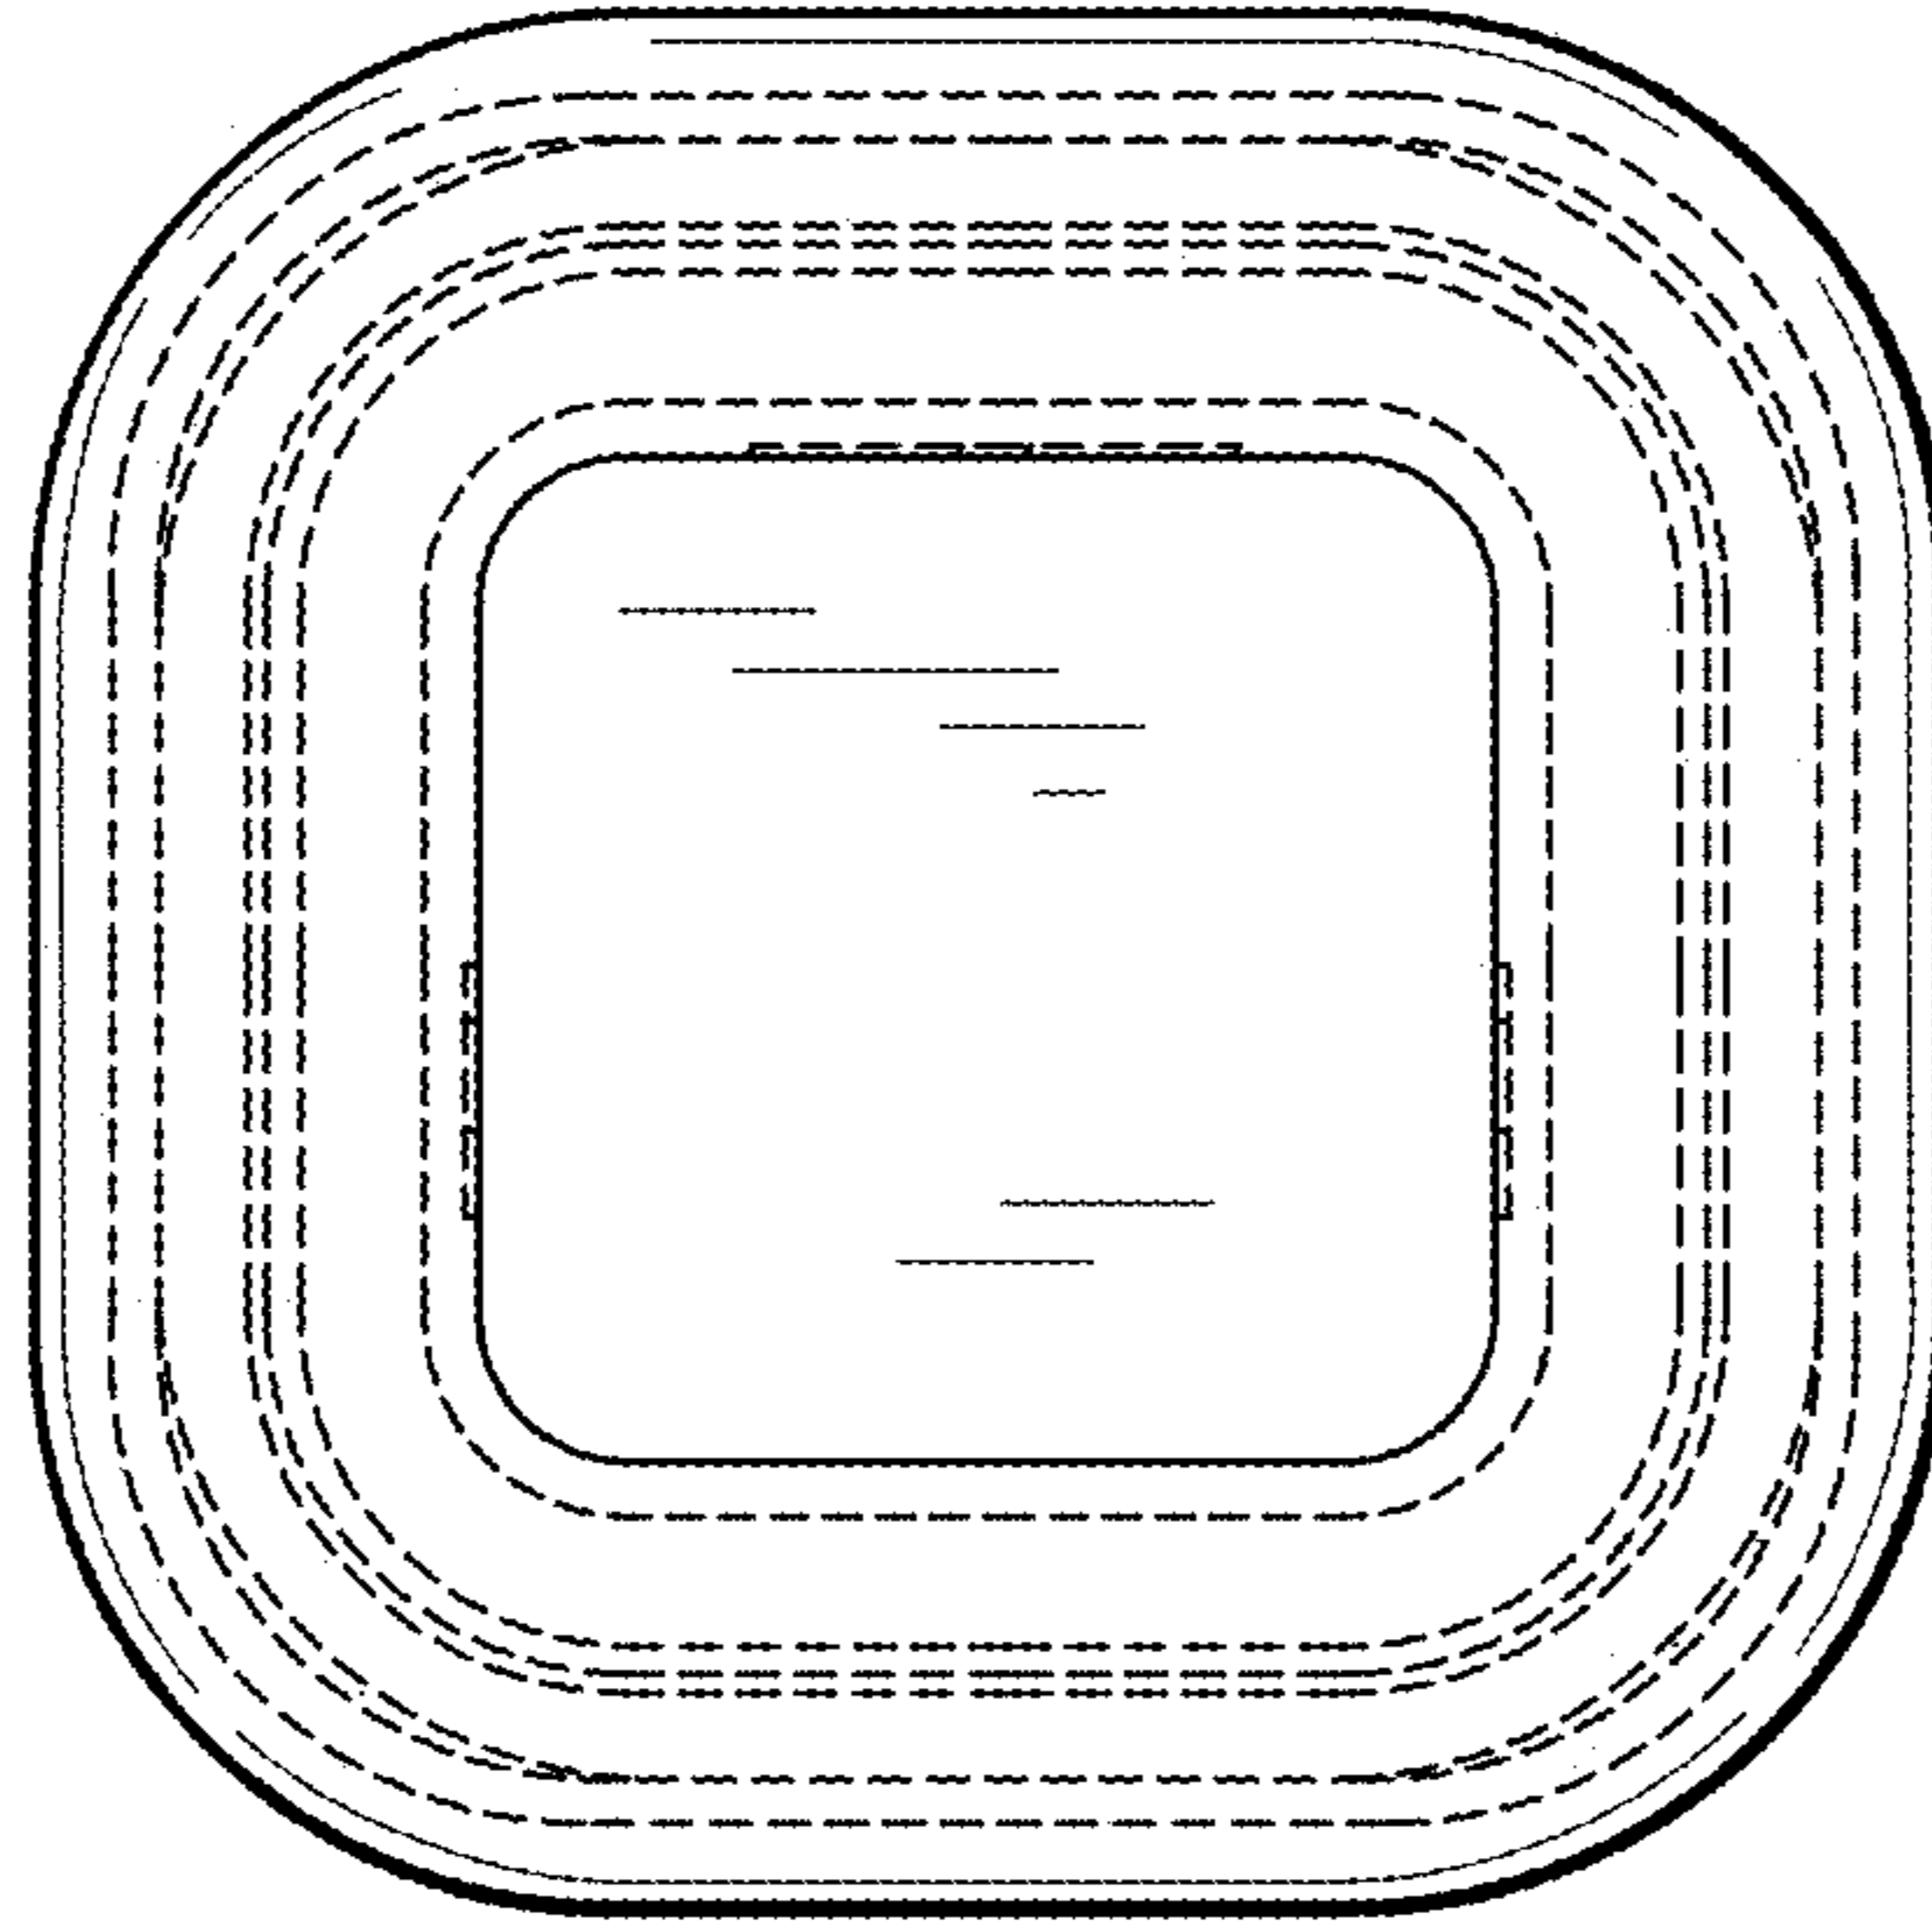


FIG. 12

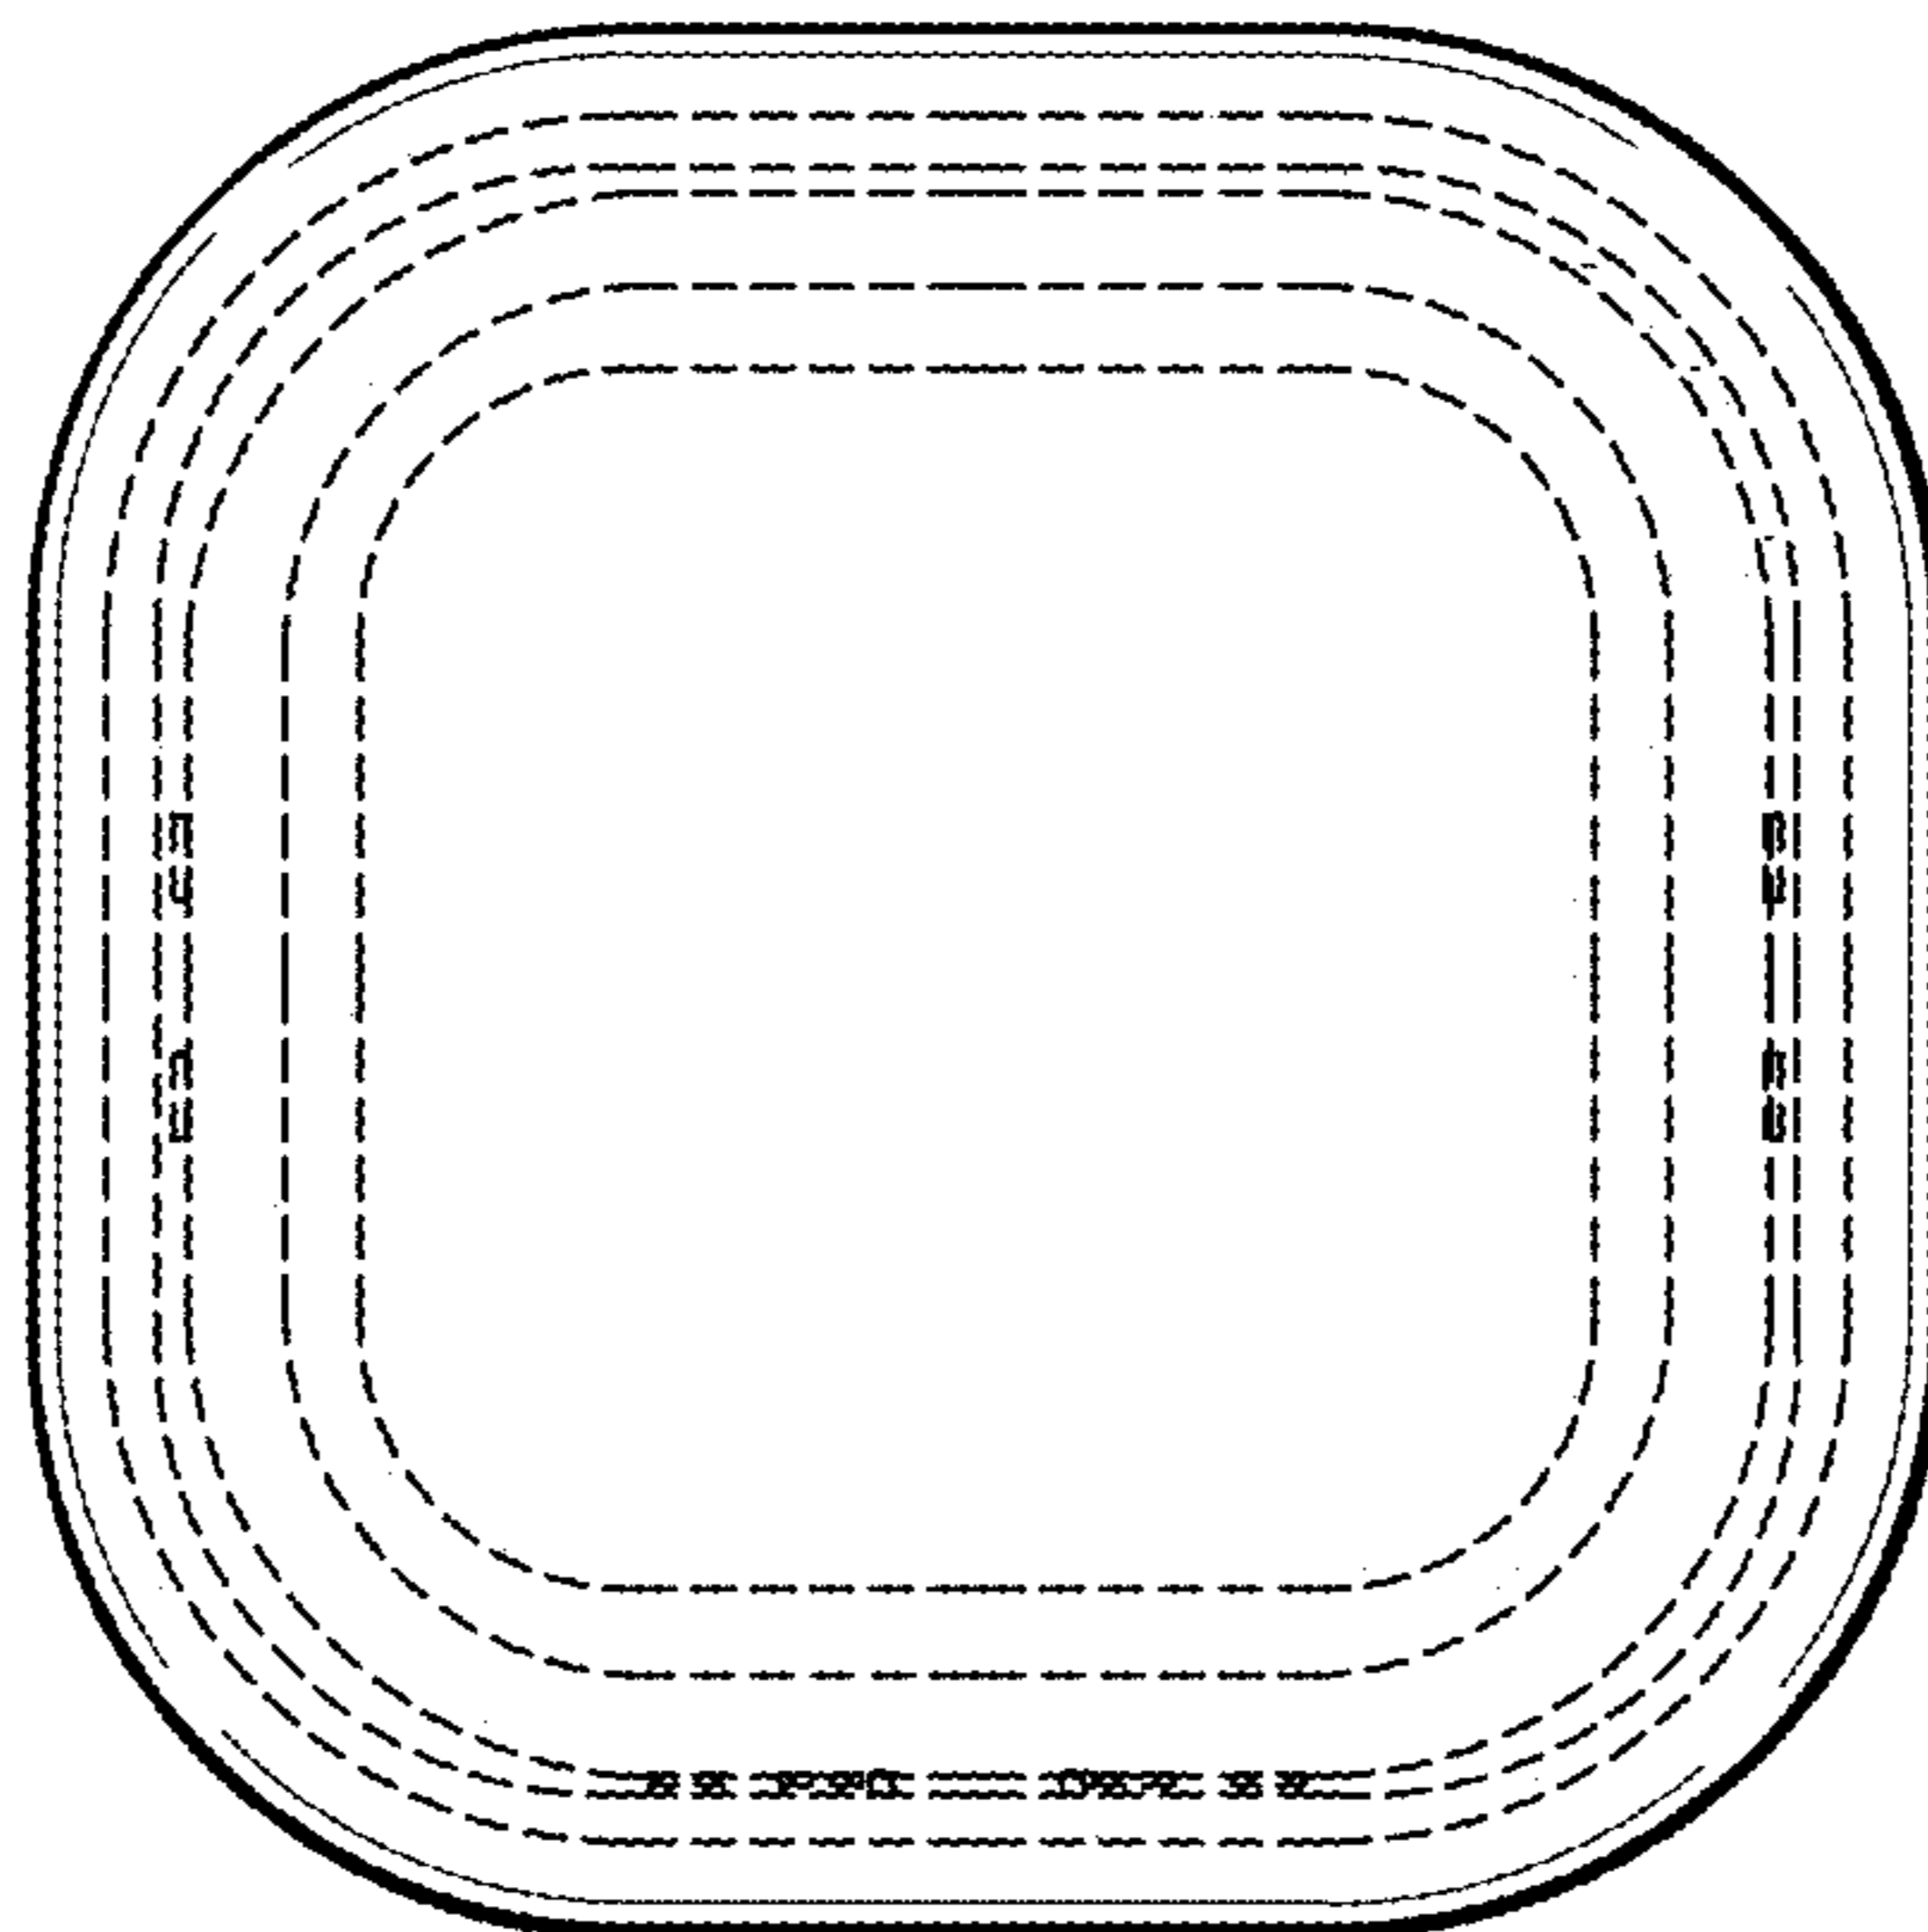


FIG. 13

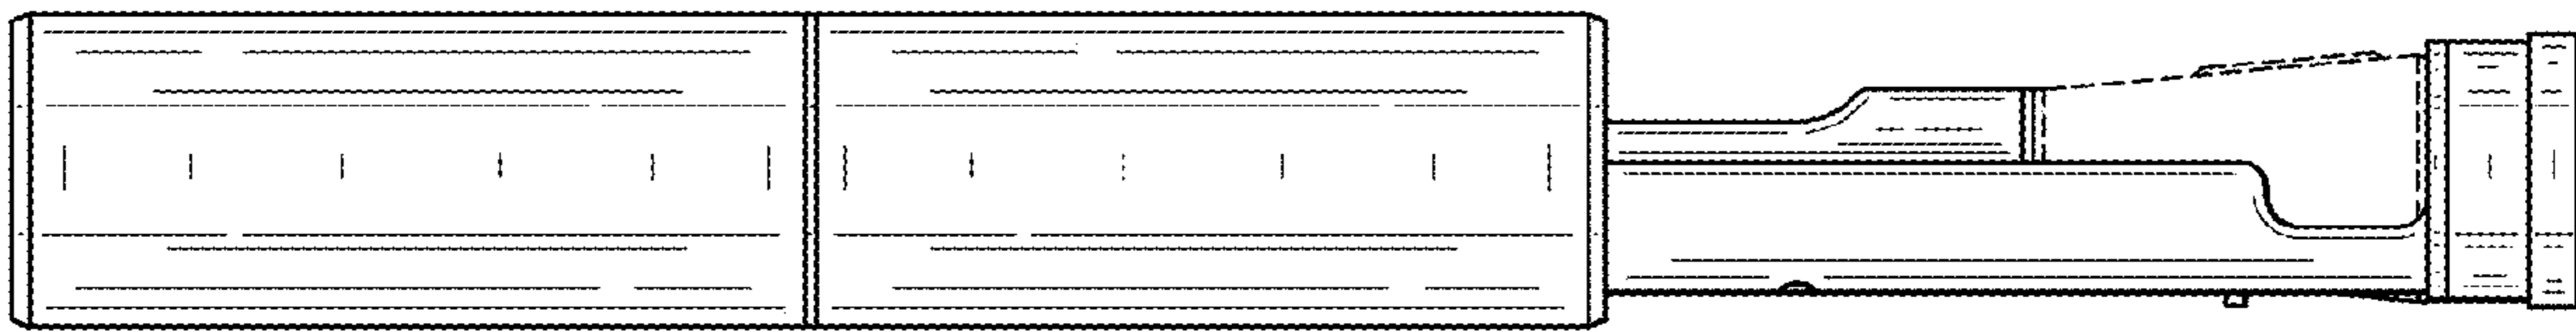


FIG. 14

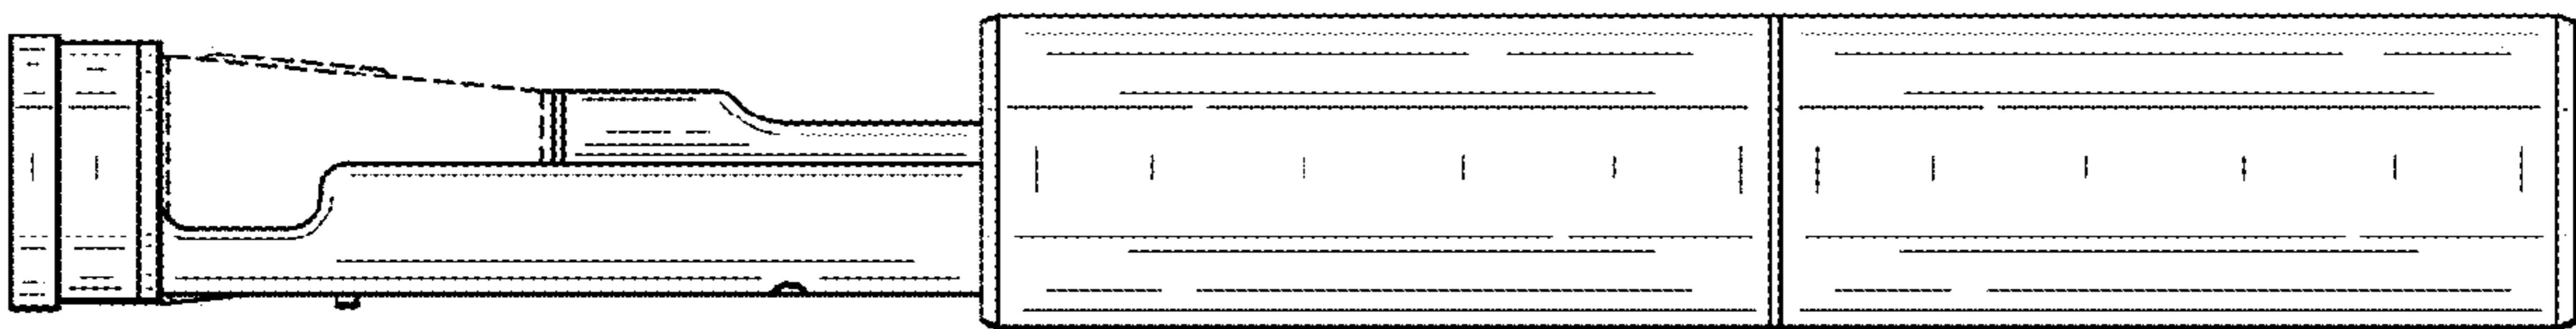


FIG. 15

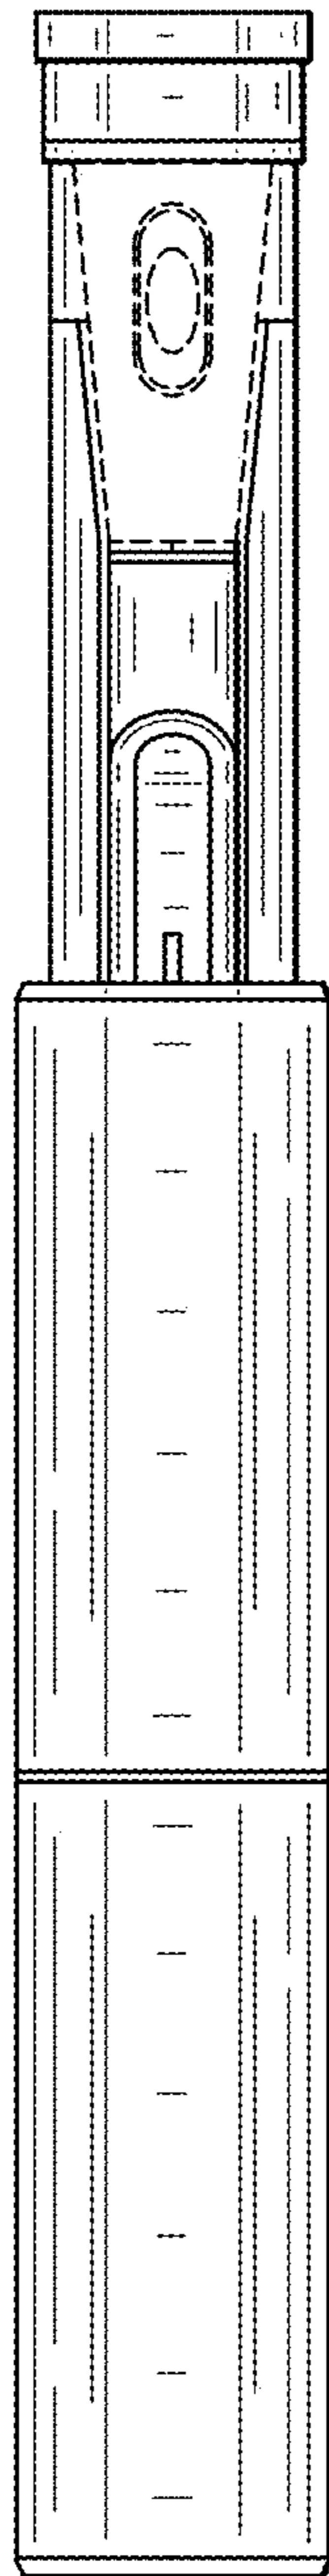


FIG. 16

