



US00D956263S

(12) **United States Design Patent**
Beckett et al.

(10) **Patent No.:** **US D956,263 S**
(45) **Date of Patent:** **** Jun. 28, 2022**

(54) **SAMPLE CARTRIDGE**

- (71) Applicant: **Ultima Genomics, Inc.**, Newark, CA (US)
- (72) Inventors: **Nathan Beckett**, Oakland, CA (US);
Joseph Anthony, Oakland, CA (US);
Phillip You Fai Lee, South San Francisco, CA (US); **Jose Martin Sosa**, San Jose, CA (US)
- (73) Assignee: **Ultima Genomics, Inc.**, Newark, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/740,346**

(22) Filed: **Jul. 2, 2020**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/226**

(58) **Field of Classification Search**
USPC D24/108, 127–130, 216, 222, 224–232;
D3/203.1, 203.3; D9/341, 756–758;
D19/37; D6/406.1–406.3, 406.6
CPC B01L 9/06; B01L 9/065; B01L 3/14; B01L 3/50; B01L 3/06; B01L 3/502; B01L 3/5025; A61B 5/150343; B01D 9/00
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D414,271 S *	9/1999	Mendoza	D24/224
D461,554 S *	8/2002	Lafond	D24/227
7,704,735 B2	4/2010	Facer et al.		
D631,557 S *	1/2011	Tajima	D24/229
D848,638 S *	5/2019	Sims	D24/226
D849,961 S *	5/2019	Muller	D24/224

(Continued)

FOREIGN PATENT DOCUMENTS

KR 3020190032223 * 12/2020

OTHER PUBLICATIONS

Dropix Sample Tray Holder. Online, published date unknown. Retrieved on Oct. 28, 2021 from URL:https://www.dolomite-microfluidics.com/product/dropix-sample-strip-holder/*

(Continued)

Primary Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Wilson Sonsini Goodrich & Rosati



(57) **CLAIM**

The ornamental design for a sample cartridge, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a sample cartridge, according to a first embodiment;
 FIG. 2 is a bottom perspective view of thereof;
 FIG. 3 is a top view of thereof;
 FIG. 4 is a front view of thereof;
 FIG. 5 is a back view of thereof;
 FIG. 6 is a right side view of thereof;
 FIG. 7 is a left side view of thereof; and
 FIG. 8 is a bottom view of thereof;
 FIG. 9 is a top perspective view of a sample cartridge, according to a second embodiment;
 FIG. 10 is a bottom perspective view of thereof;
 FIG. 11 is a top view of thereof;
 FIG. 12 is a front view of thereof;
 FIG. 13 is a back view of thereof;
 FIG. 14 is a right side view of thereof;
 FIG. 15 is a left side view of thereof; and,
 FIG. 16 is a bottom view of thereof.
 The dot-dash lines in the drawings depict the boundaries of the claim and form no part thereof.
 The dash lines in the drawings depict portions of the sample cartridge that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

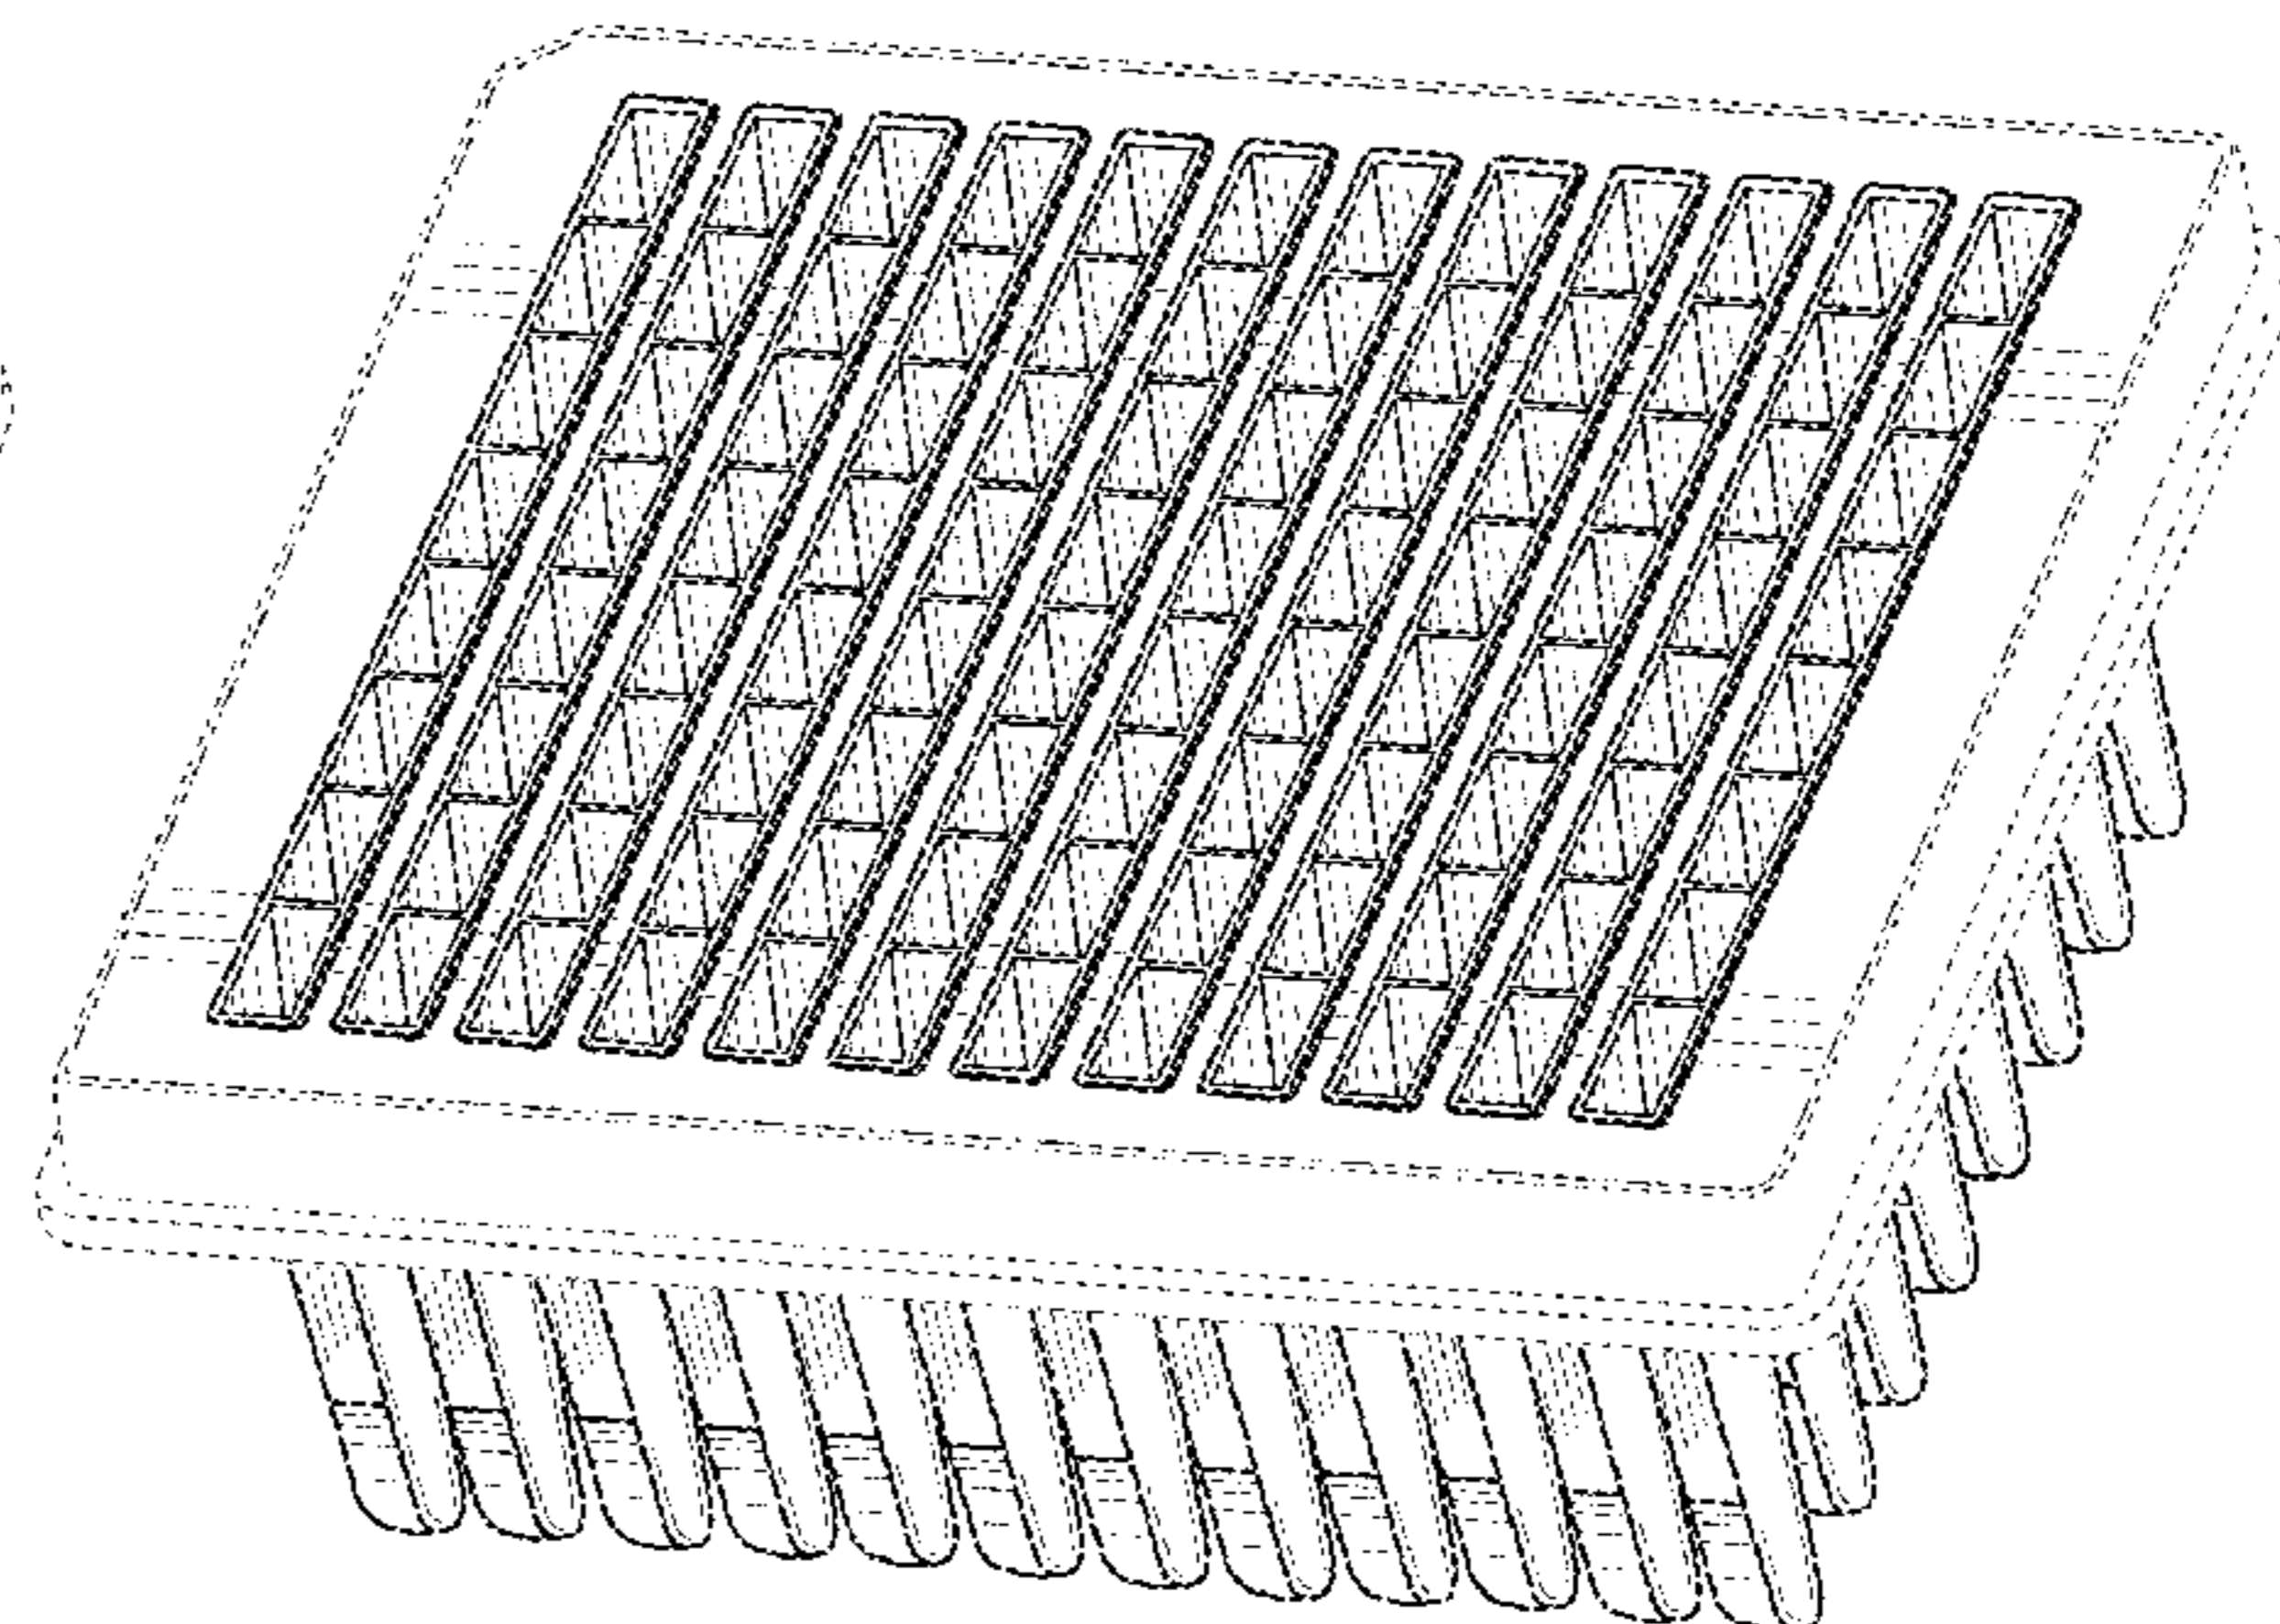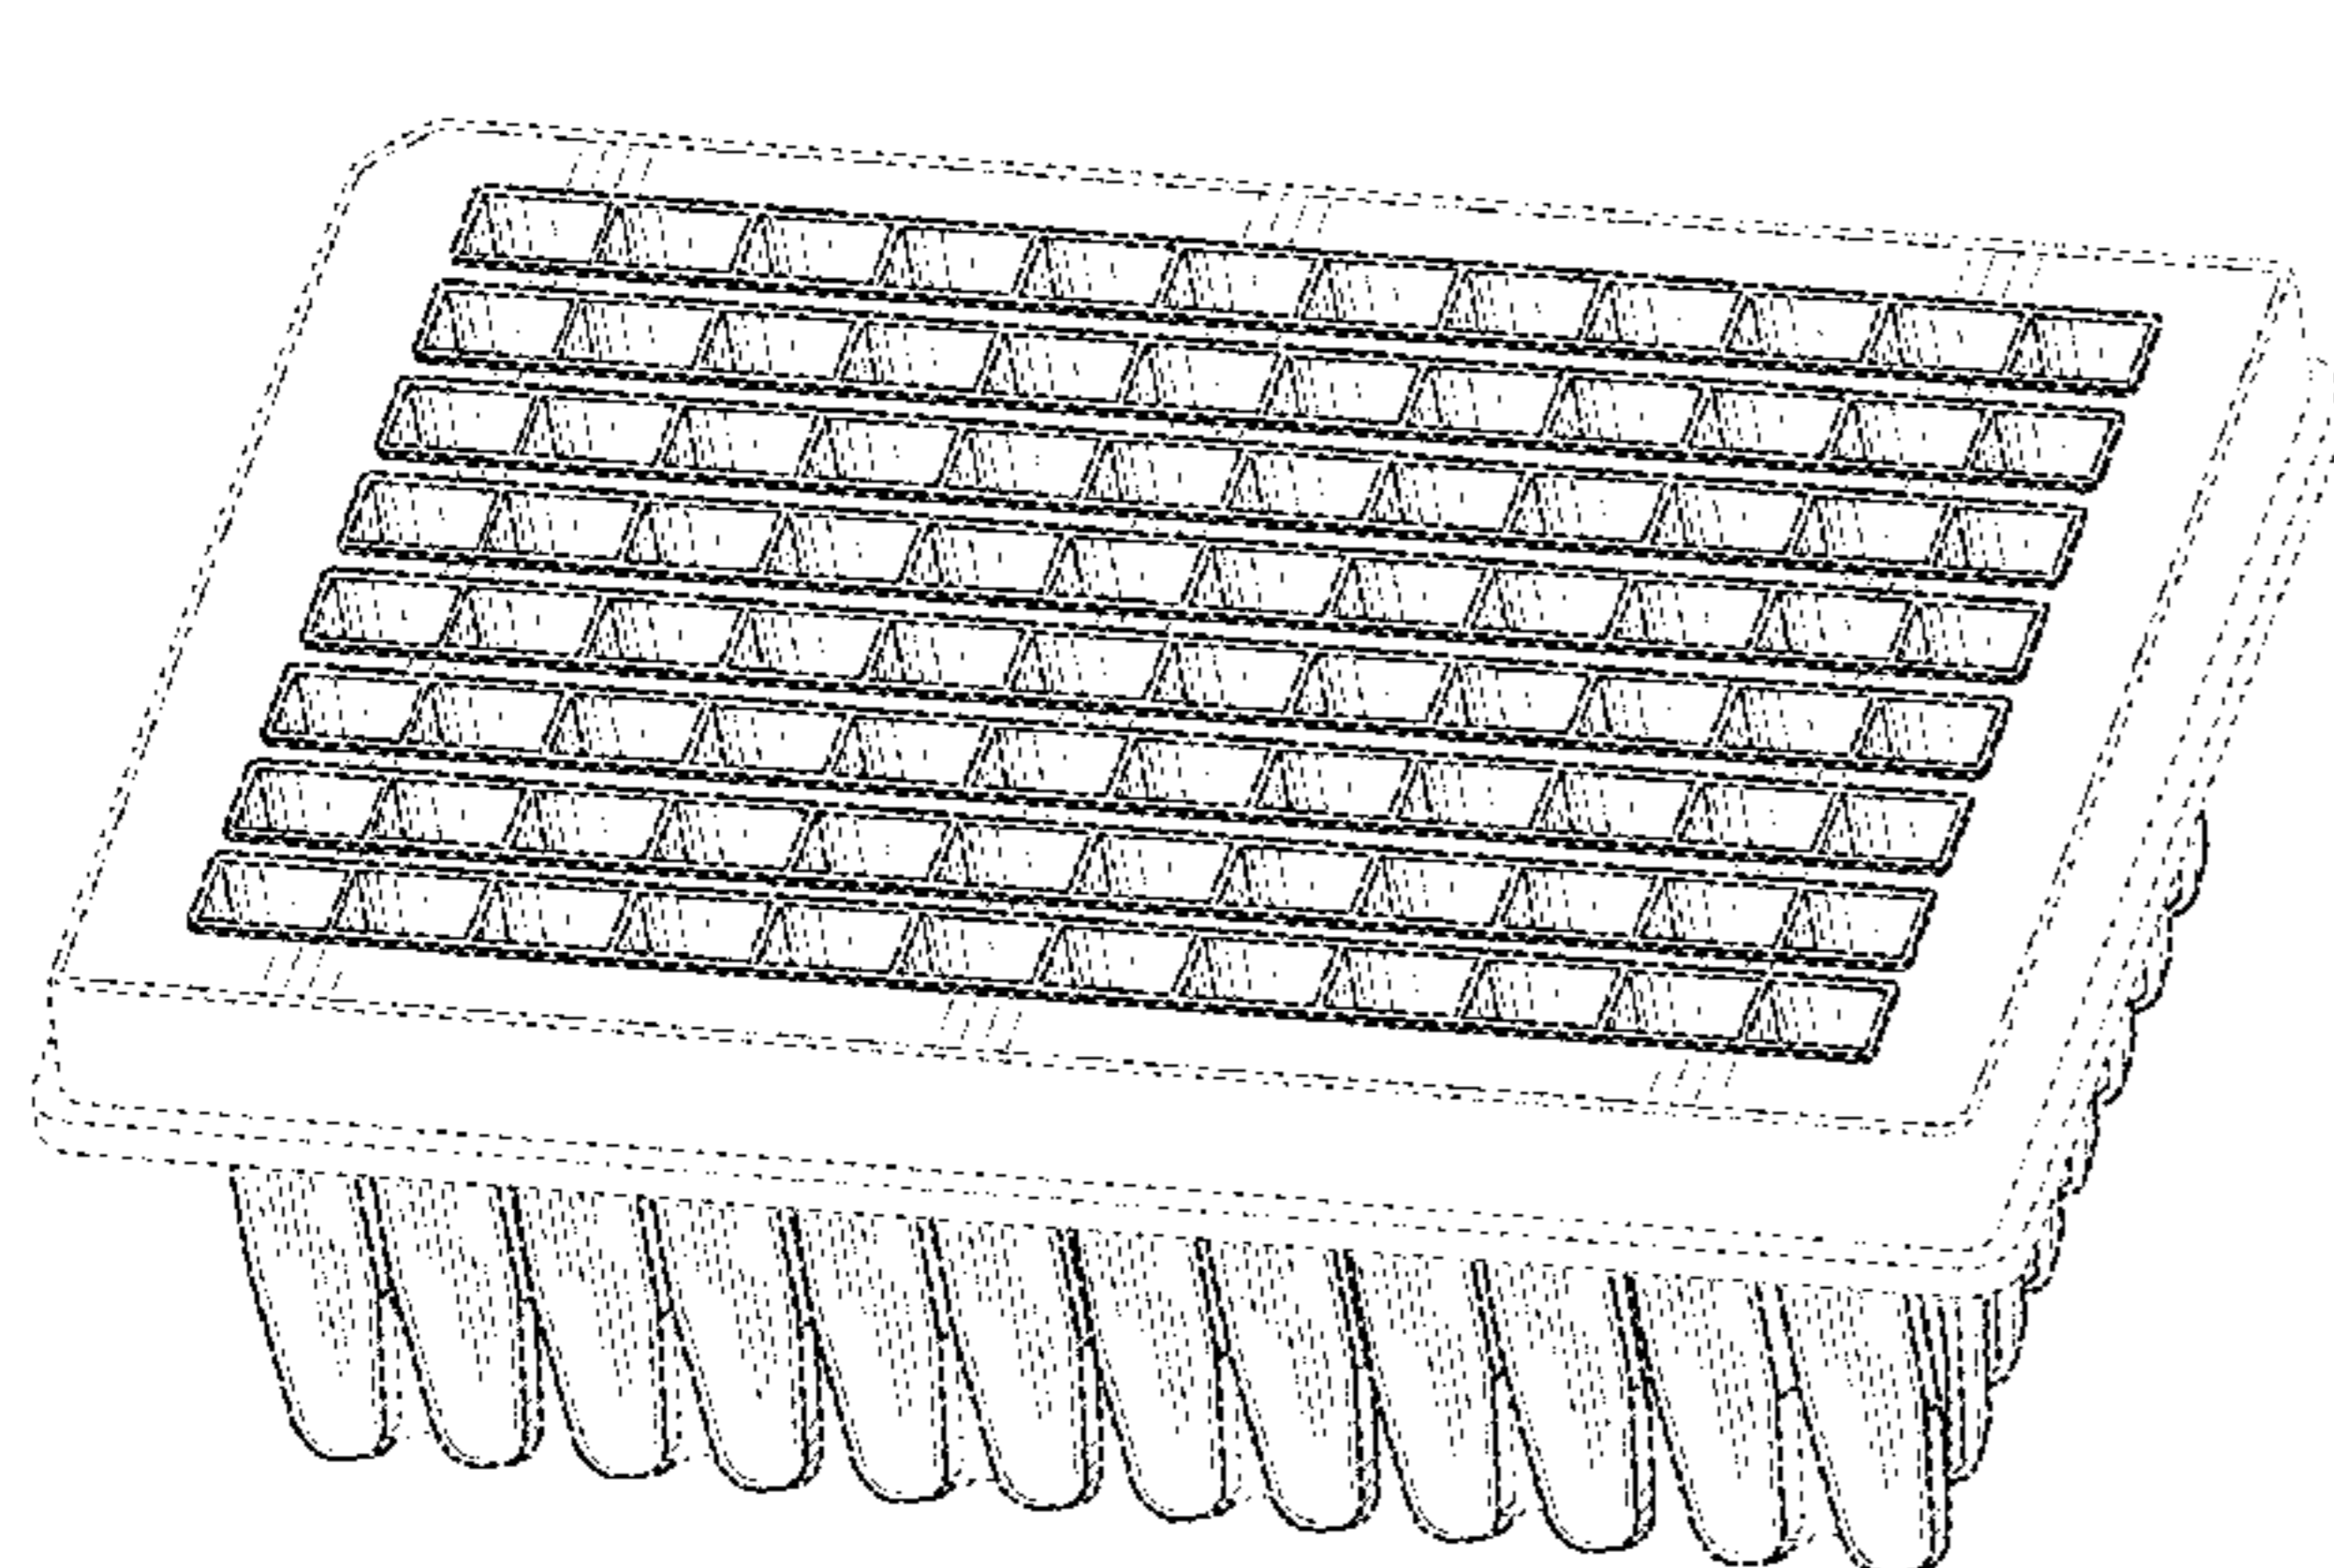

(56)

References Cited

U.S. PATENT DOCUMENTS

D854,707 S * 7/2019 Jakobsen D24/230
D902,433 S * 11/2020 Livingston D24/227
D918,417 S * 5/2021 O'Mahony D24/229
D922,212 S * 6/2021 Suchsland D9/761
2005/0170498 A1* 8/2005 Dolley B01L 3/5085
435/288.4
2010/0203643 A1* 8/2010 Self B01L 9/06
436/47
2011/0286897 A1* 11/2011 Uschkureit B29C 45/0081
422/553
2016/0319329 A1* 11/2016 Natale B01L 3/5453

OTHER PUBLICATIONS

Axygen™ 8-Strip PCR Tubes, 0.2mL. Available at <https://www.fishersci.com/shop/products/axygen-8-strip-pcr-tubes-flat-cap-0-2ml-color-maxyclear/14222252>. Accessed on Jun. 25, 2020 (2 pages).
Oilfield-Wiki. Electrostatic treater. Available at http://www.oilfieldwiki.com/wiki/Electrostatic_treater. Accessed on Mar. 13, 2020.
Co-pending U.S. Appl. No. 29/774,033, inventors WOLF; Jacob et al., filed Mar. 12, 2021.

* cited by examiner

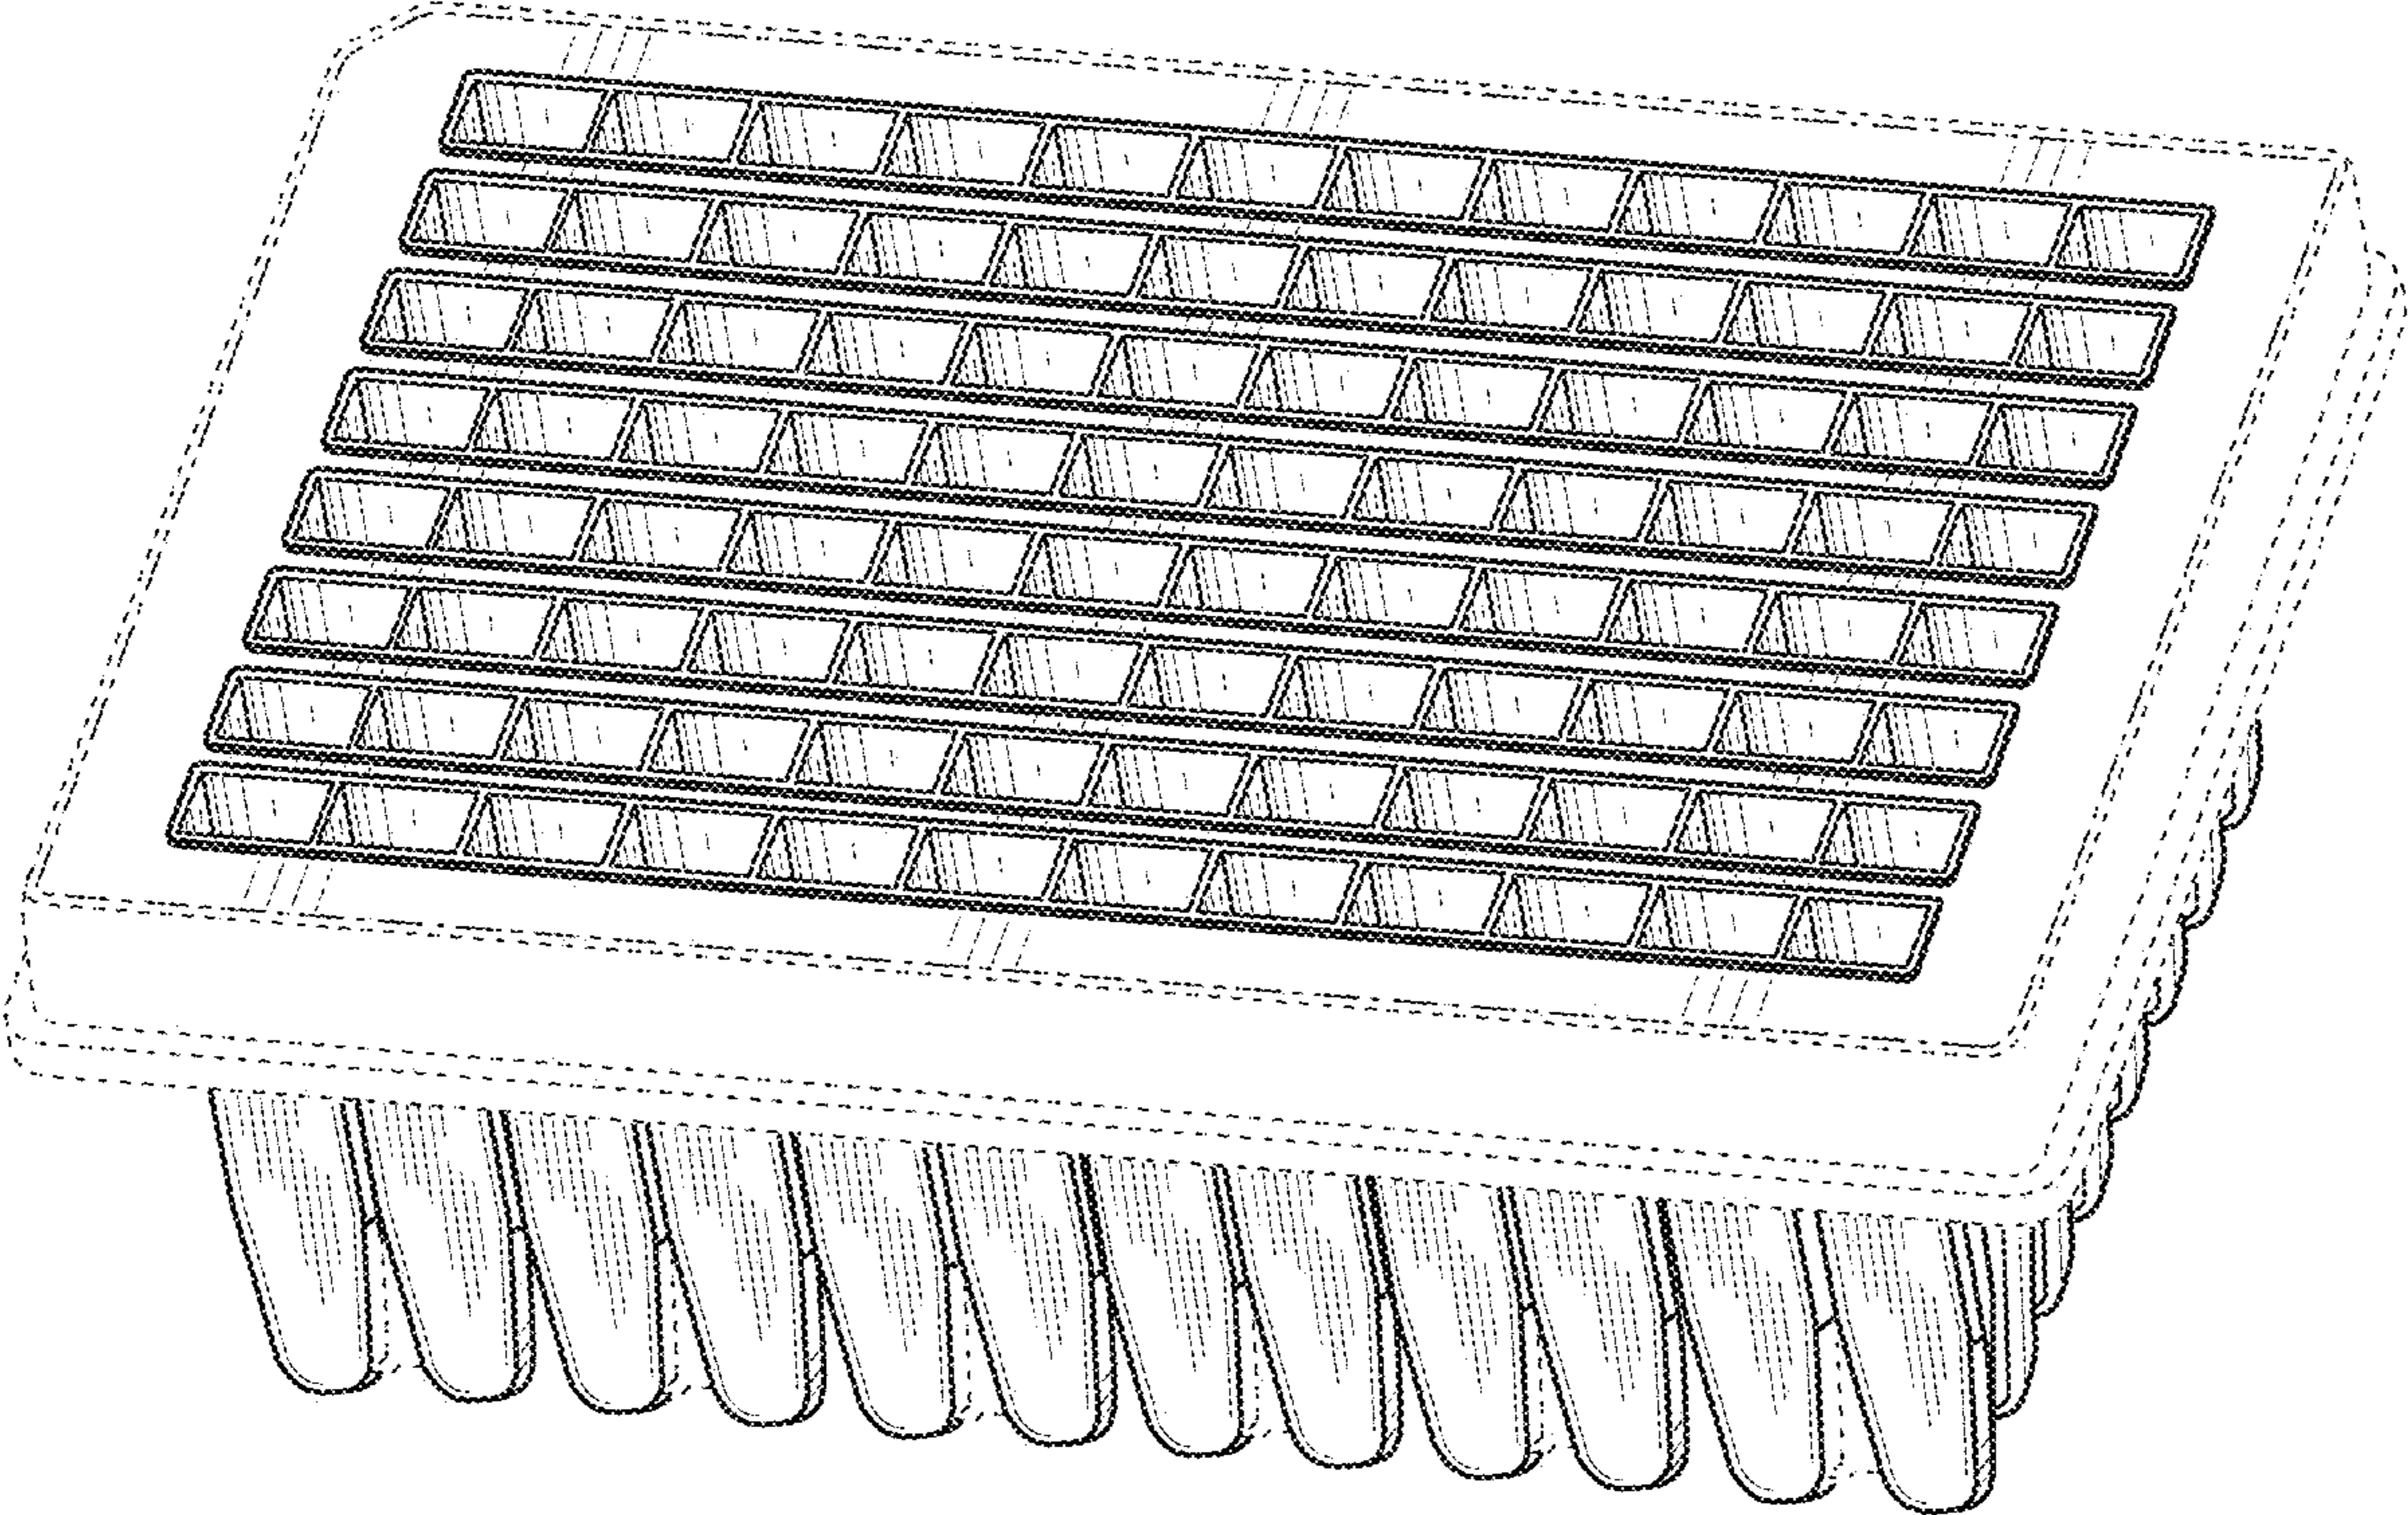


FIG. 1

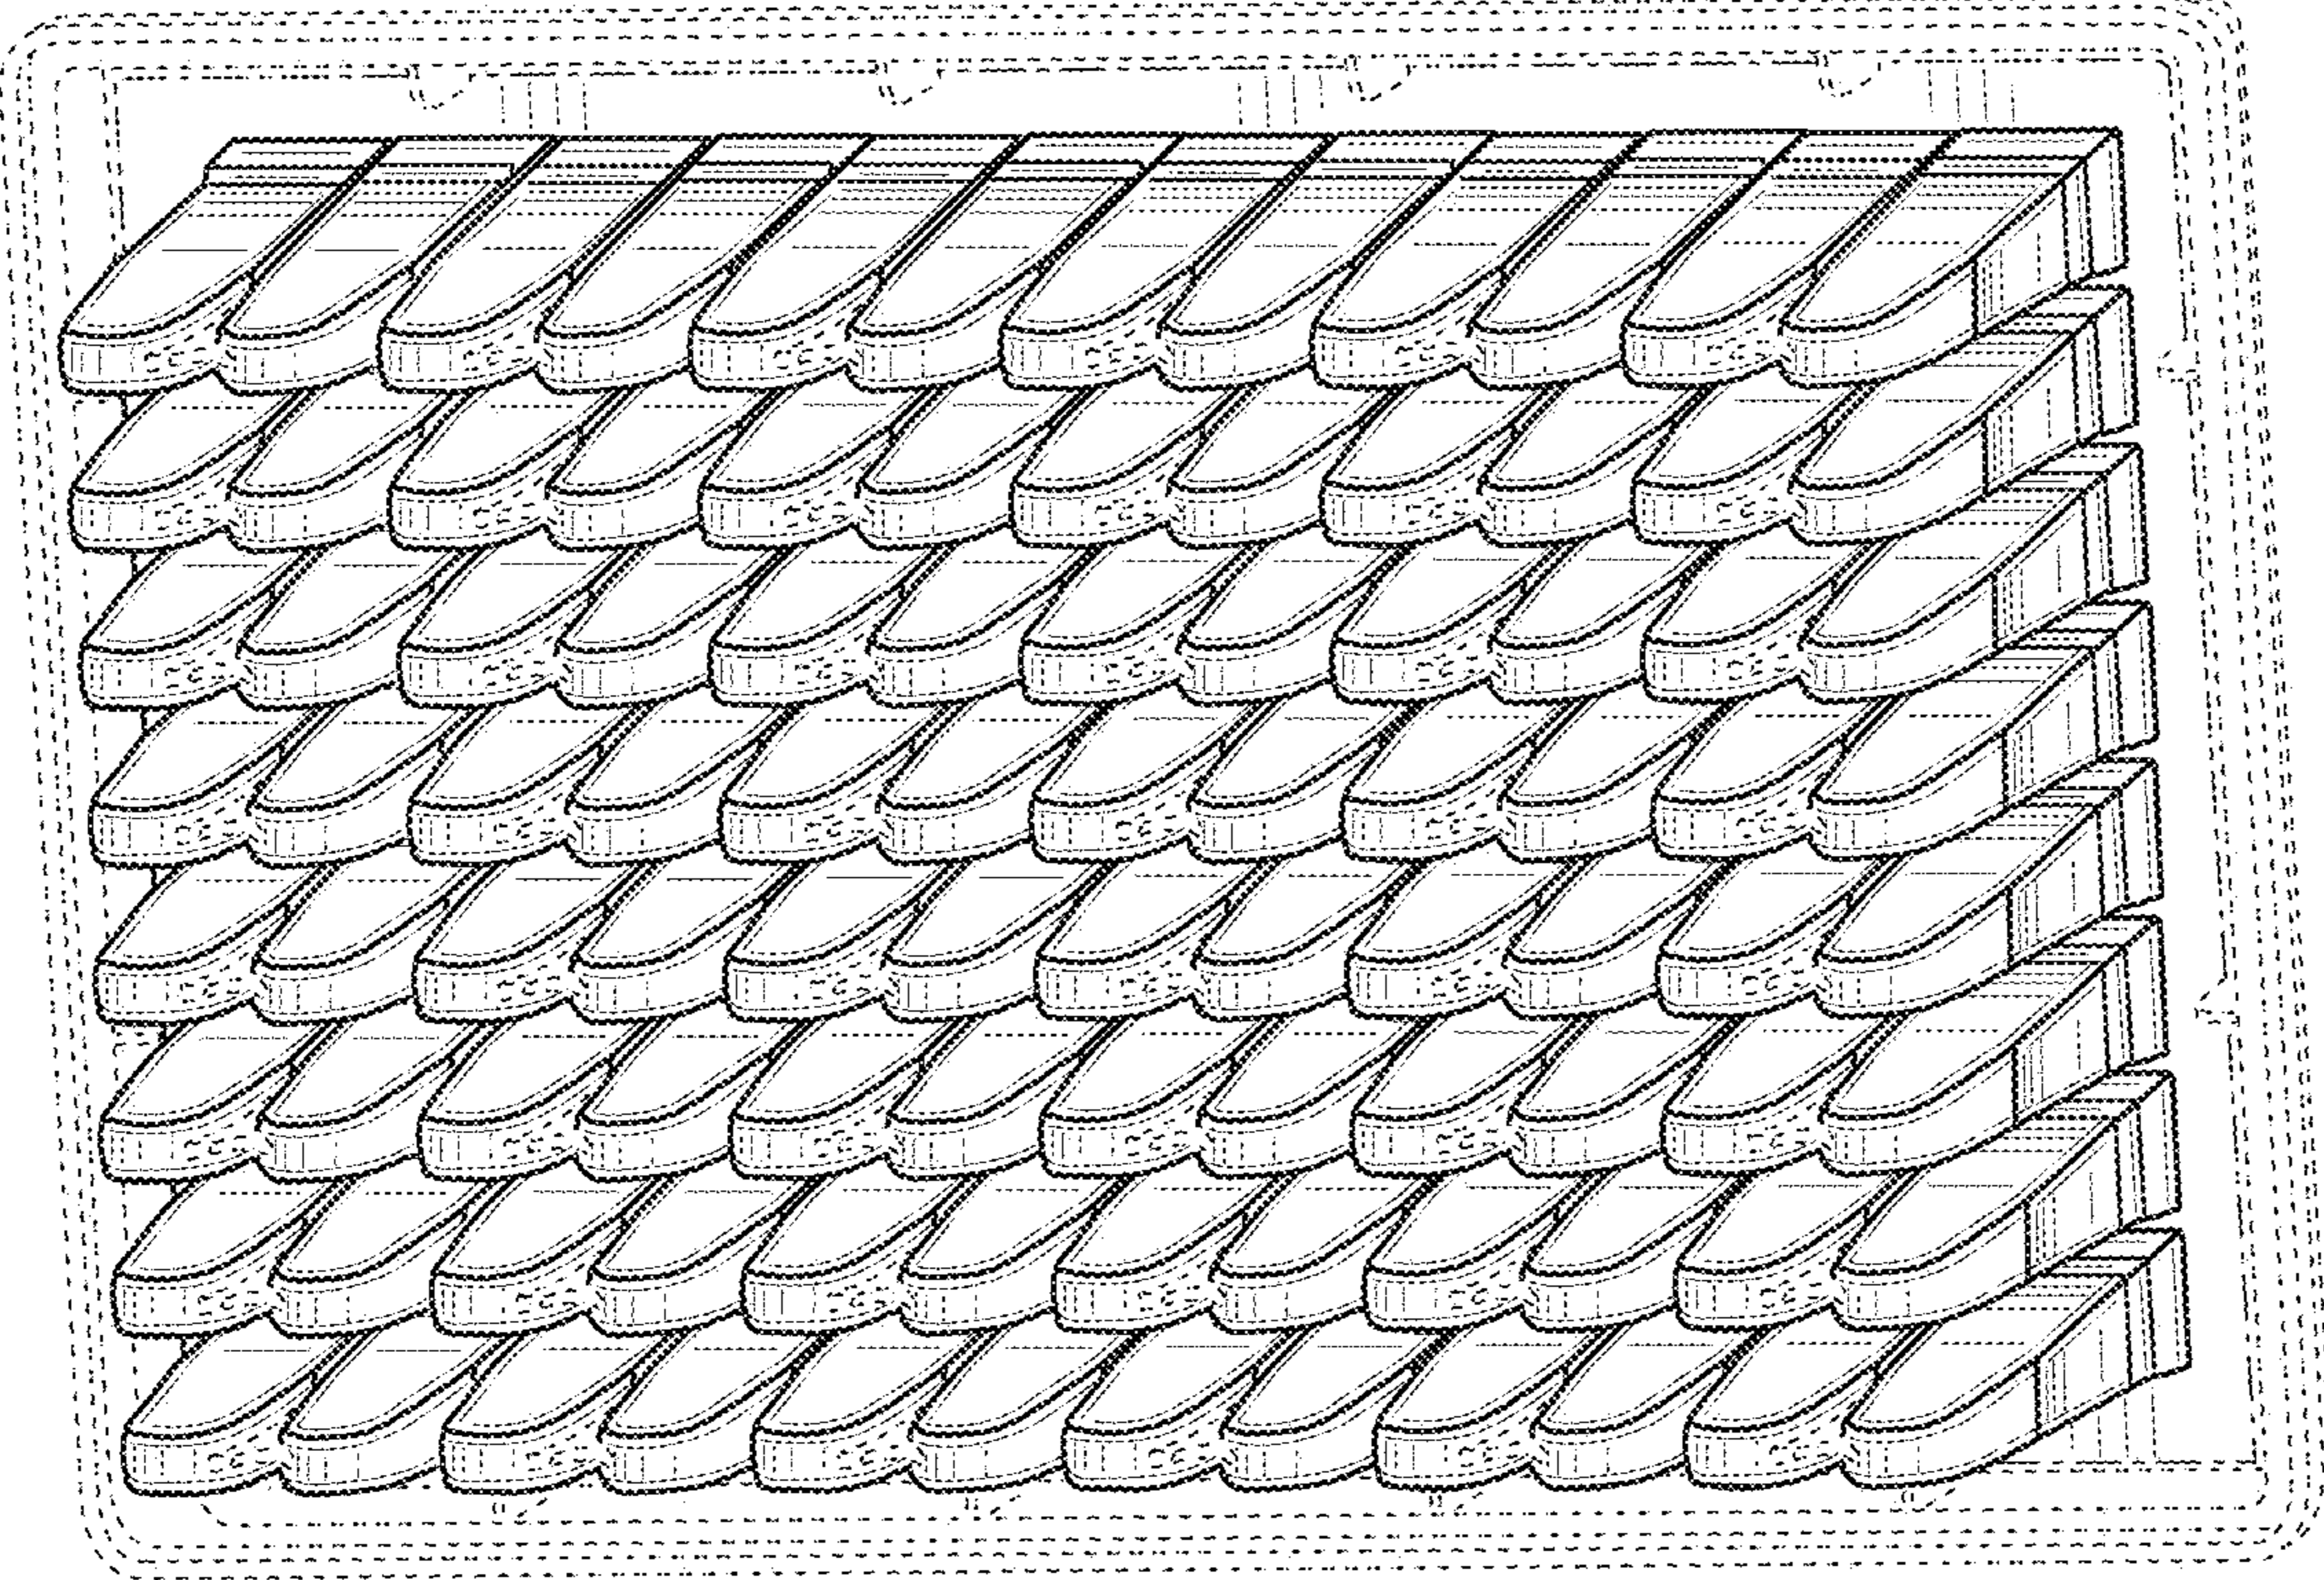


FIG. 2

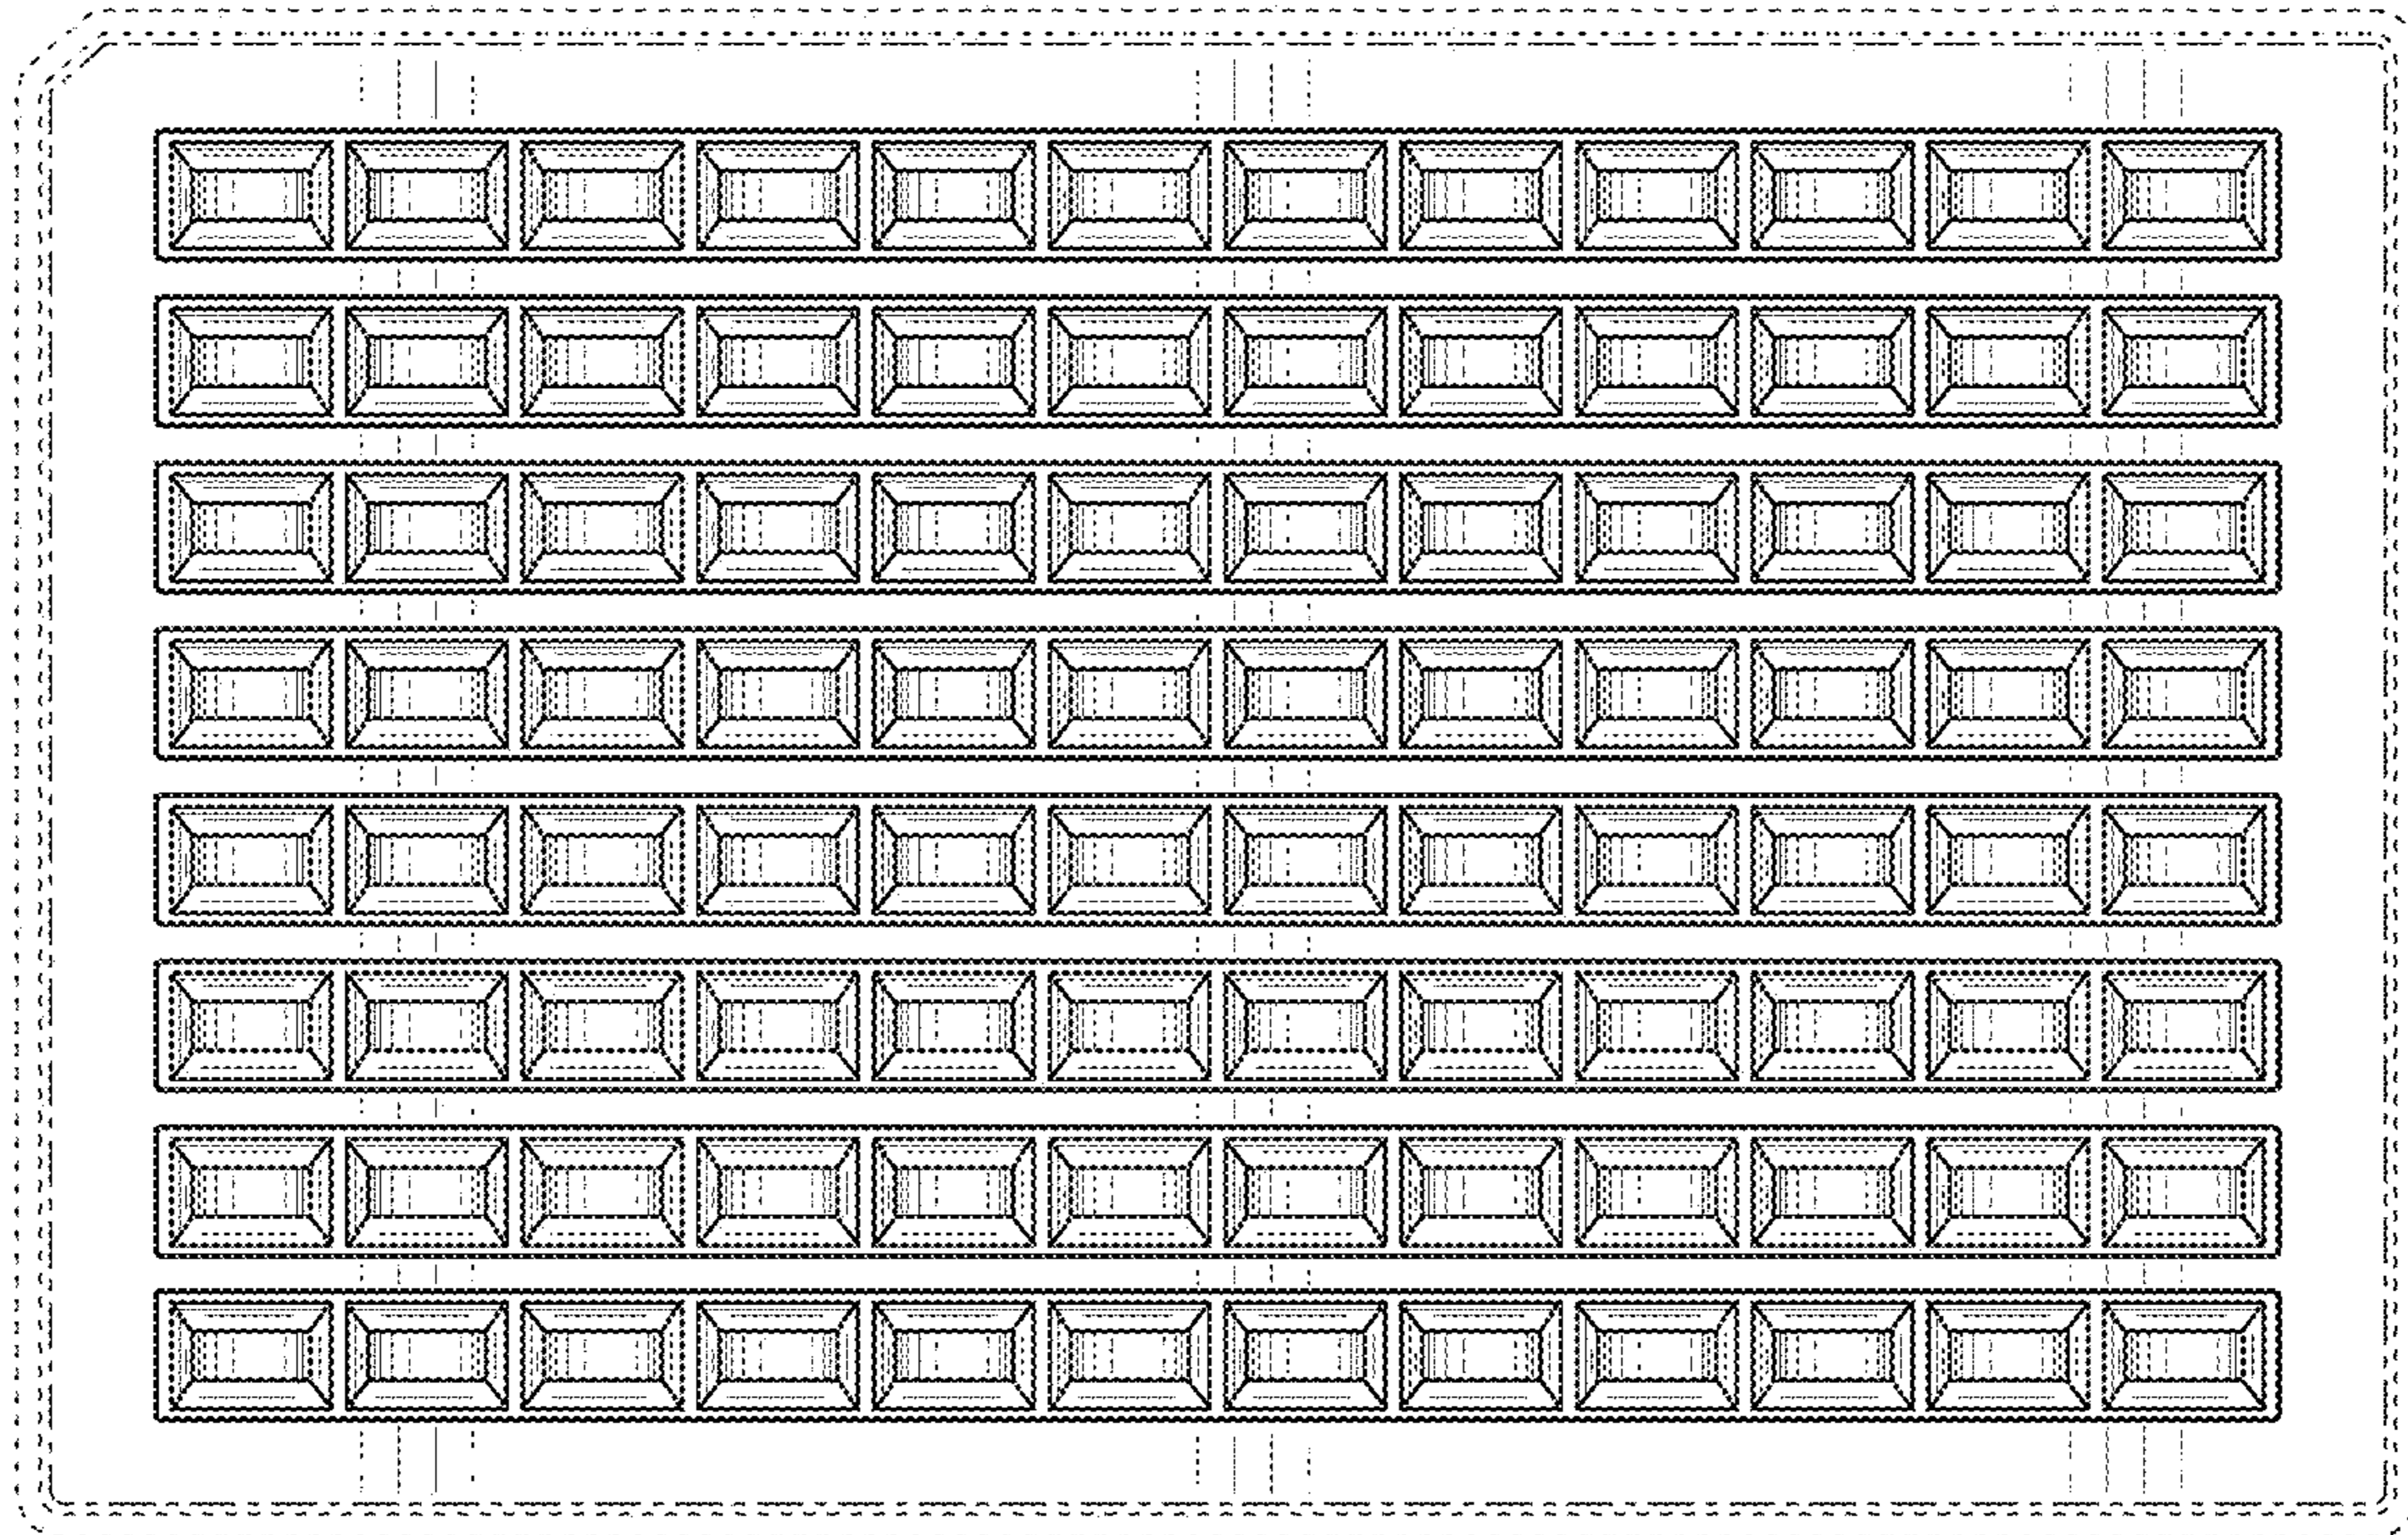


FIG. 3

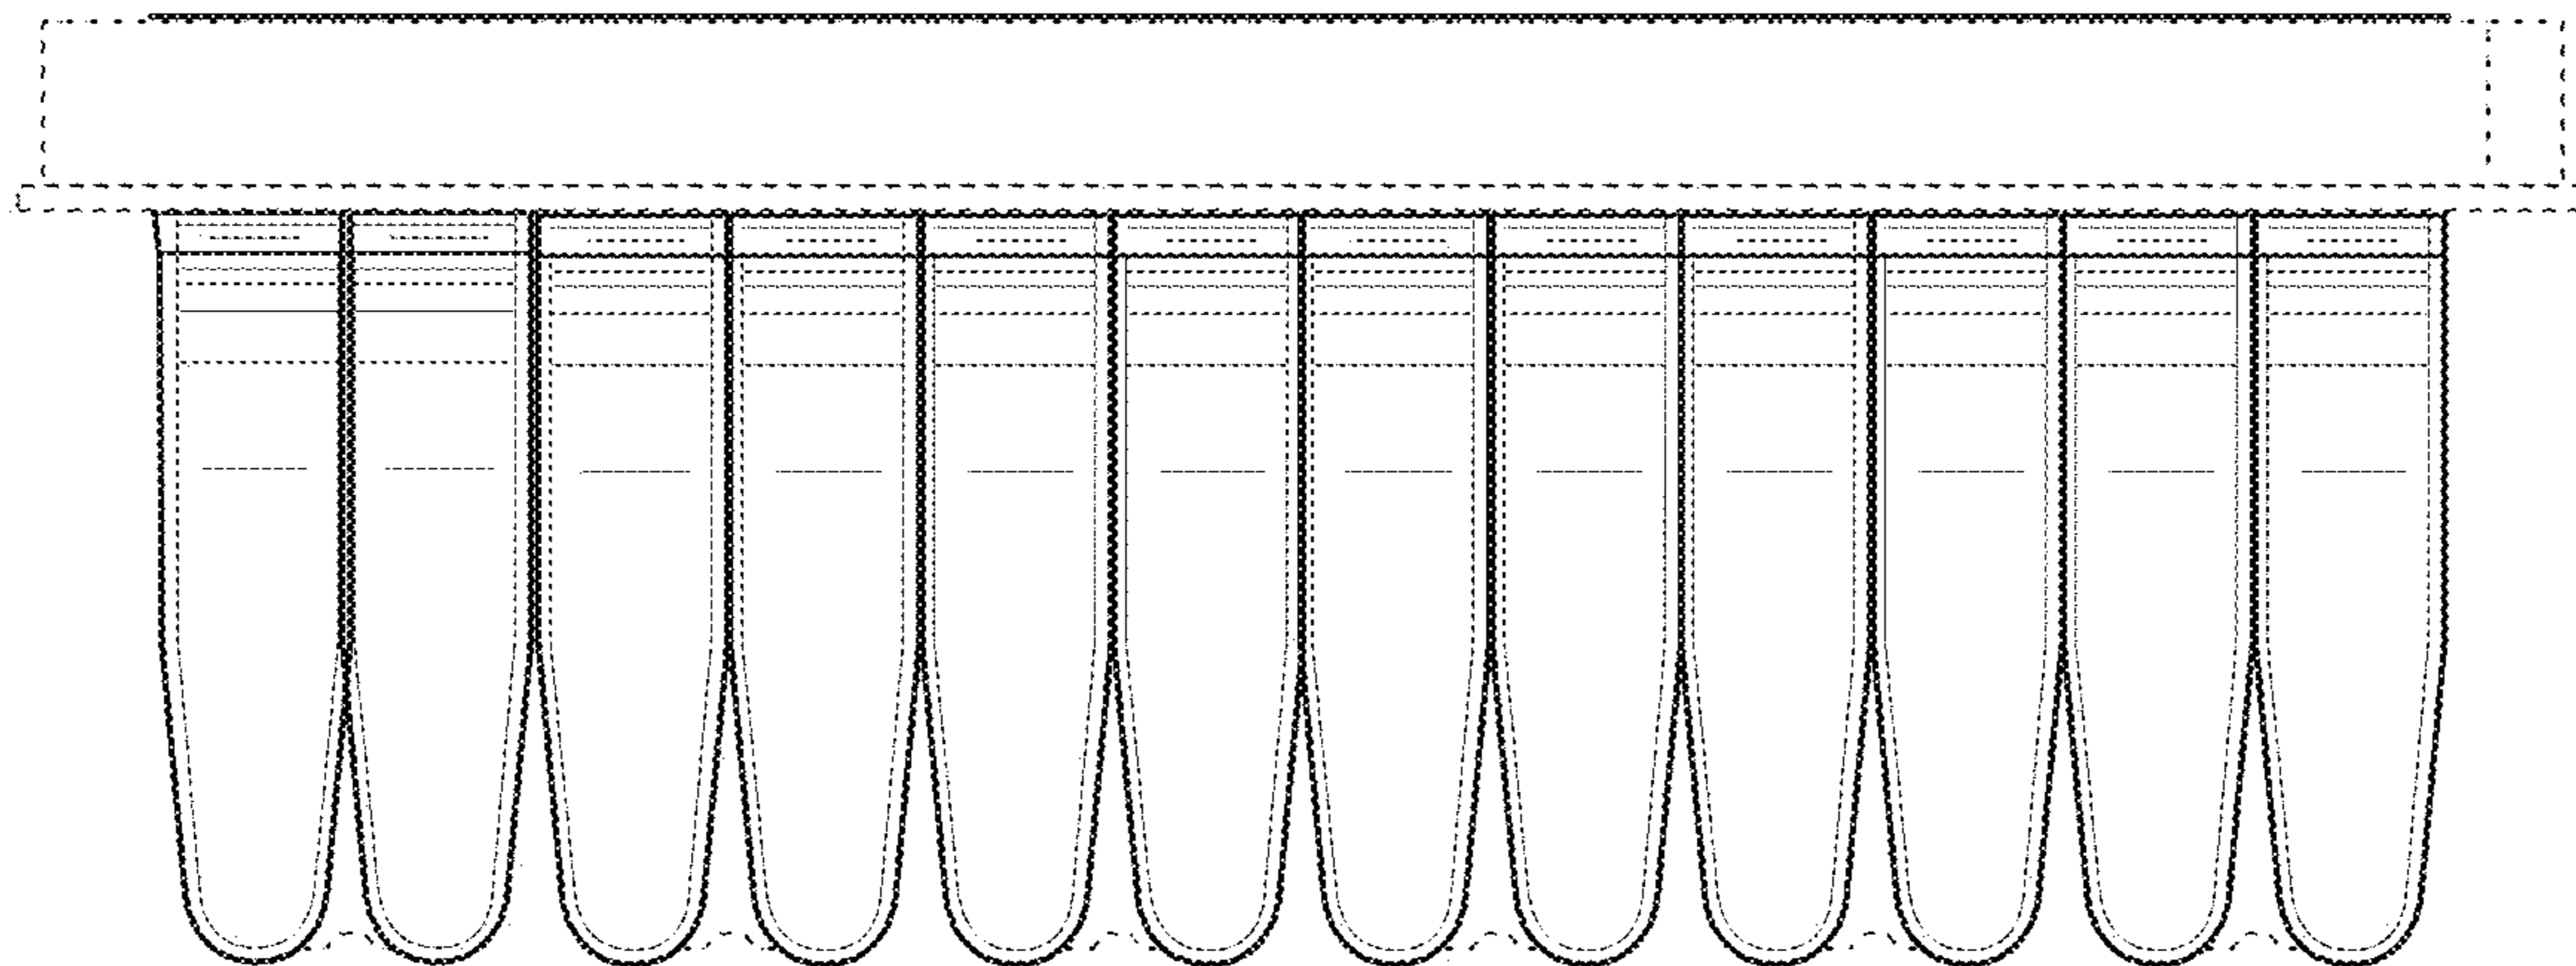


FIG. 4

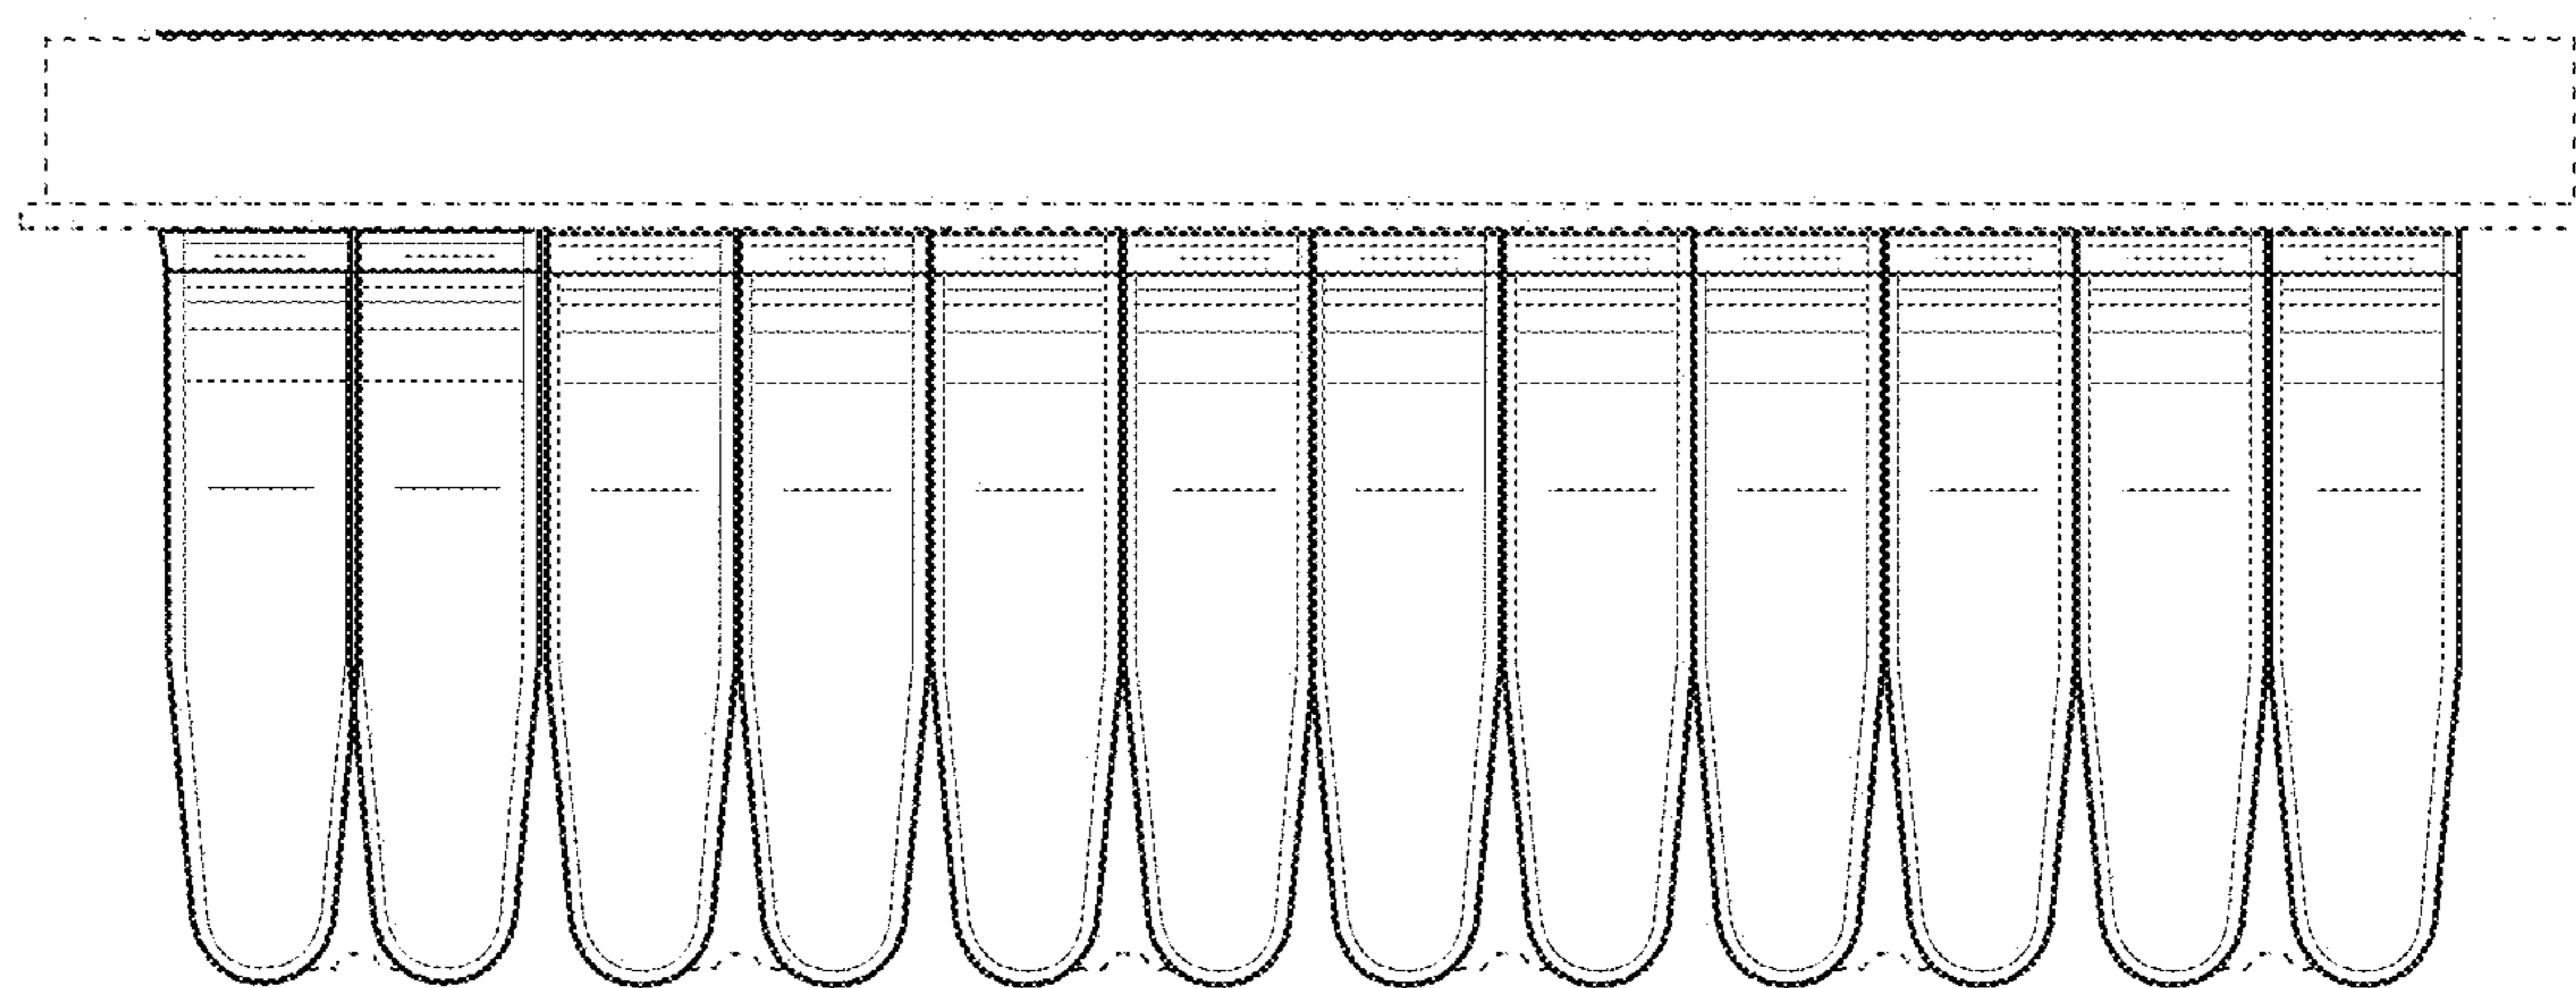


FIG. 5

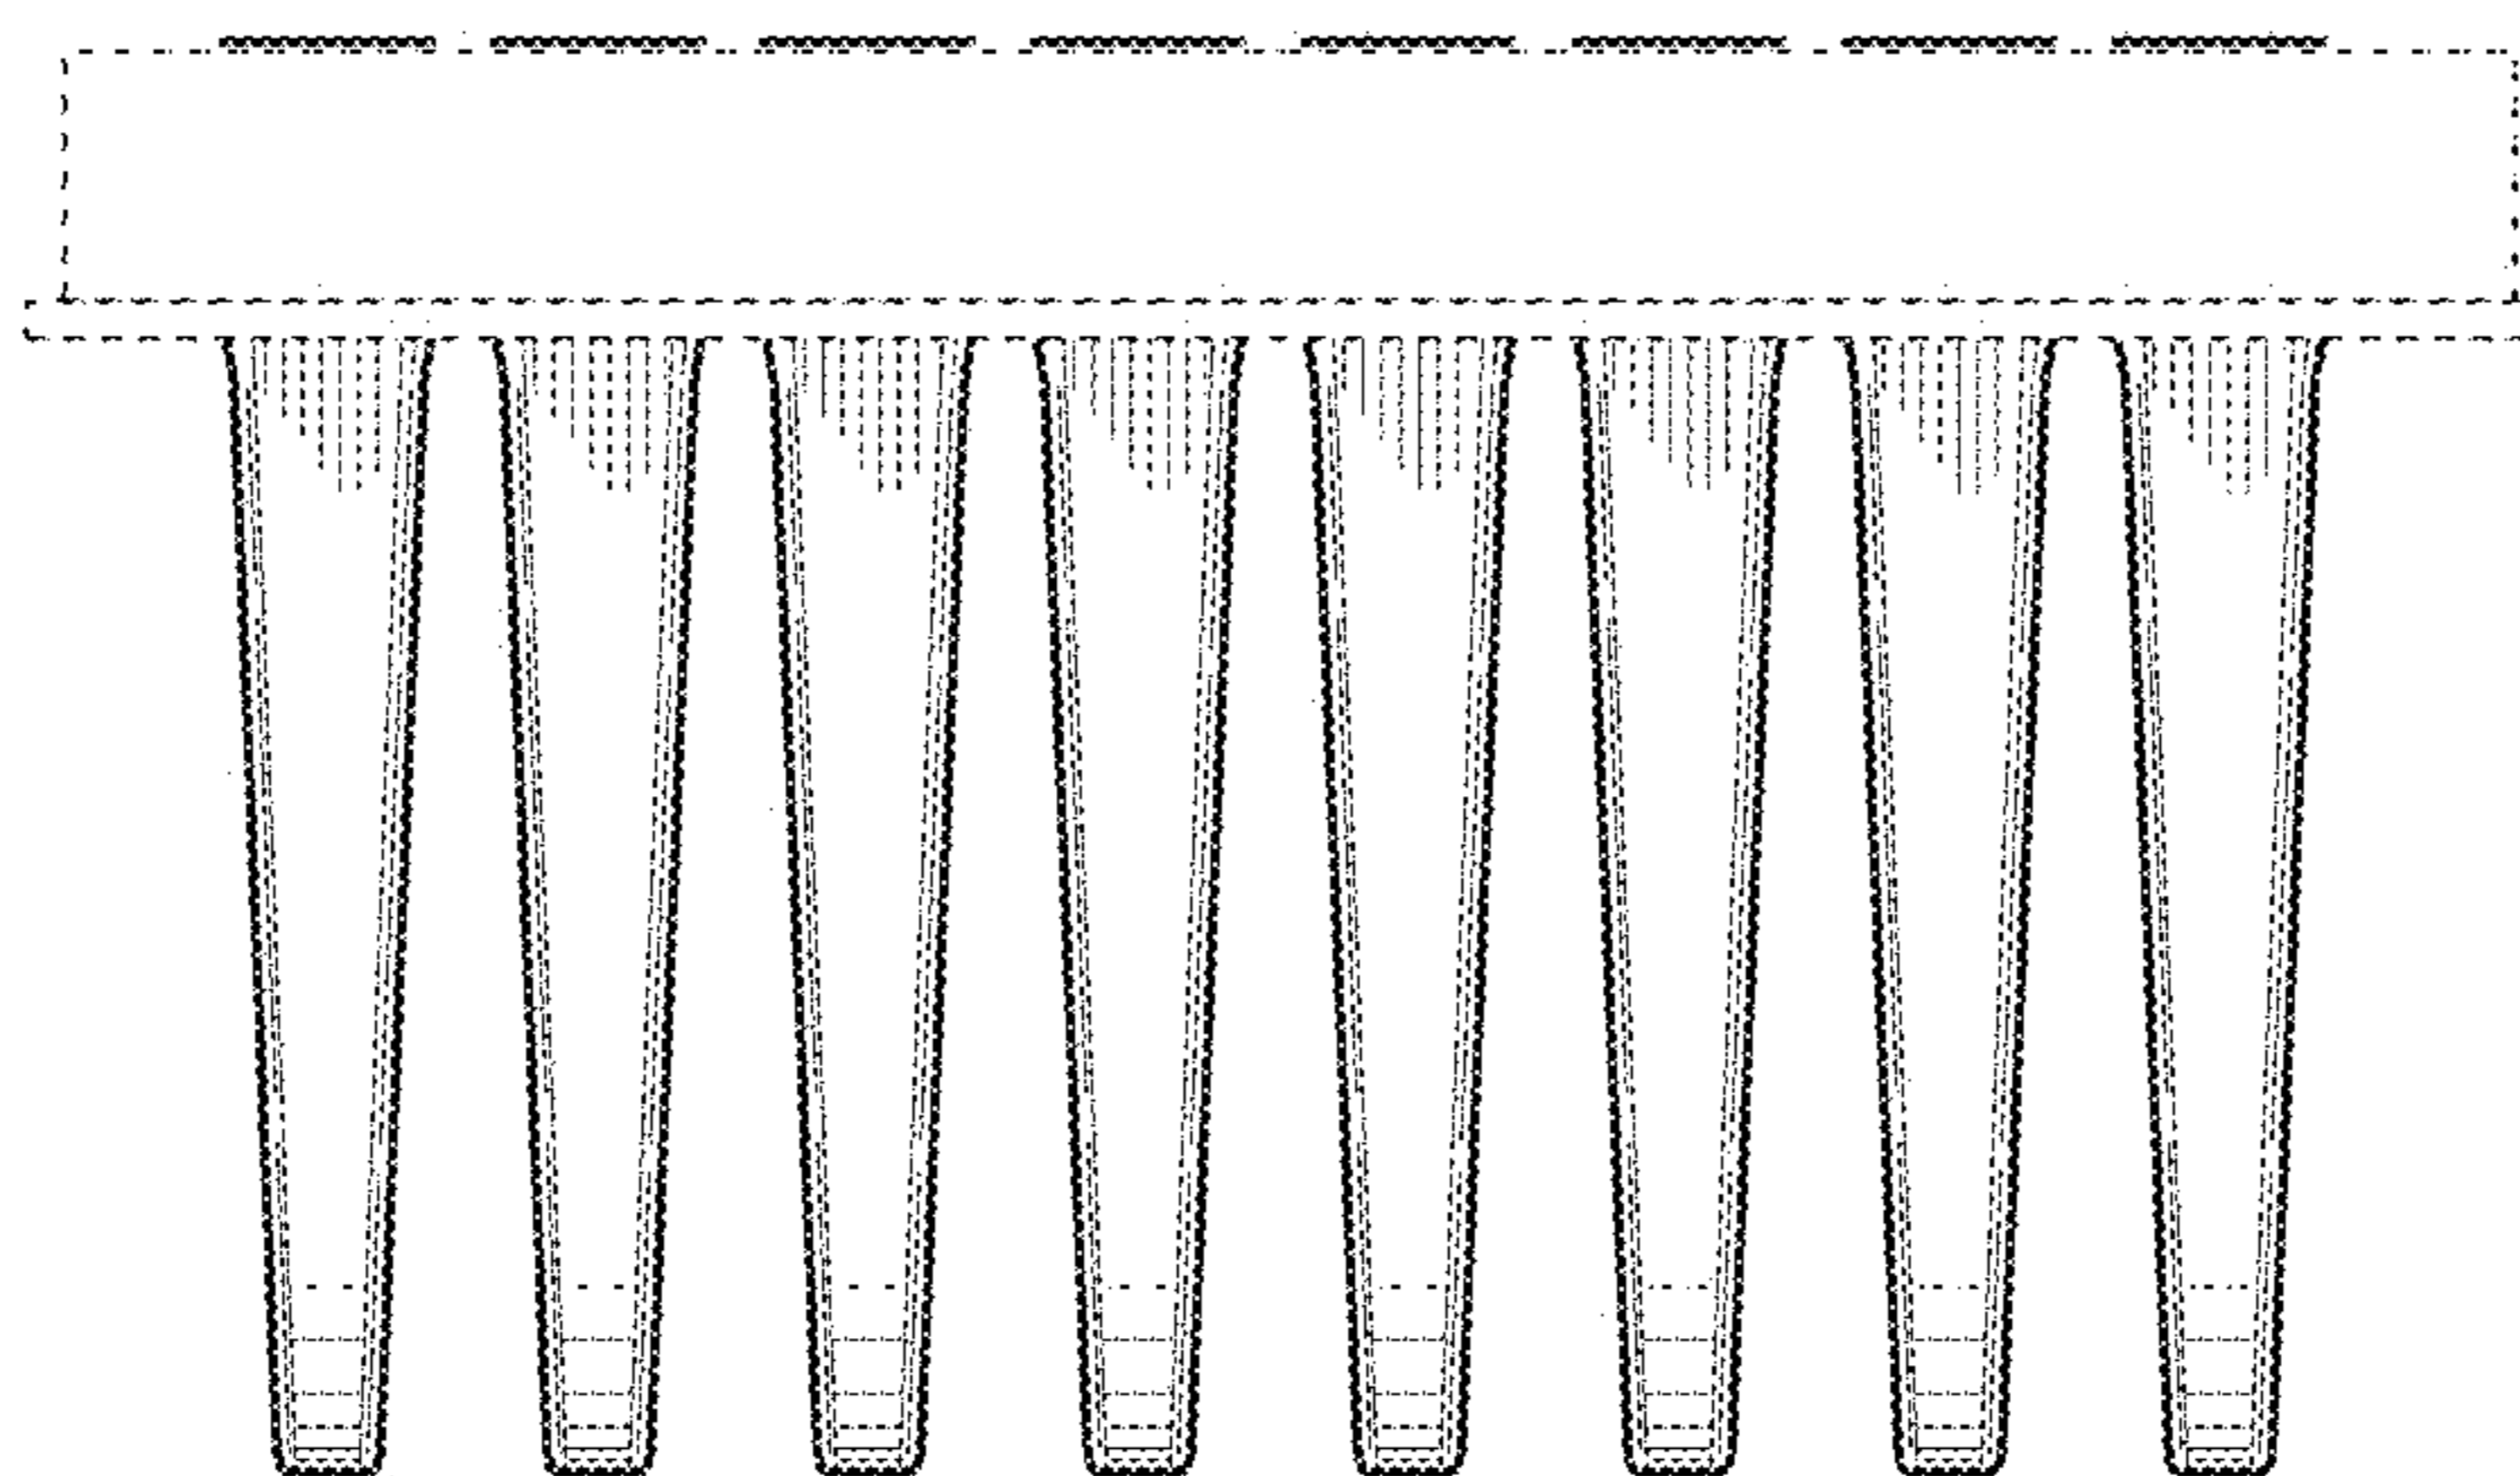


FIG. 6

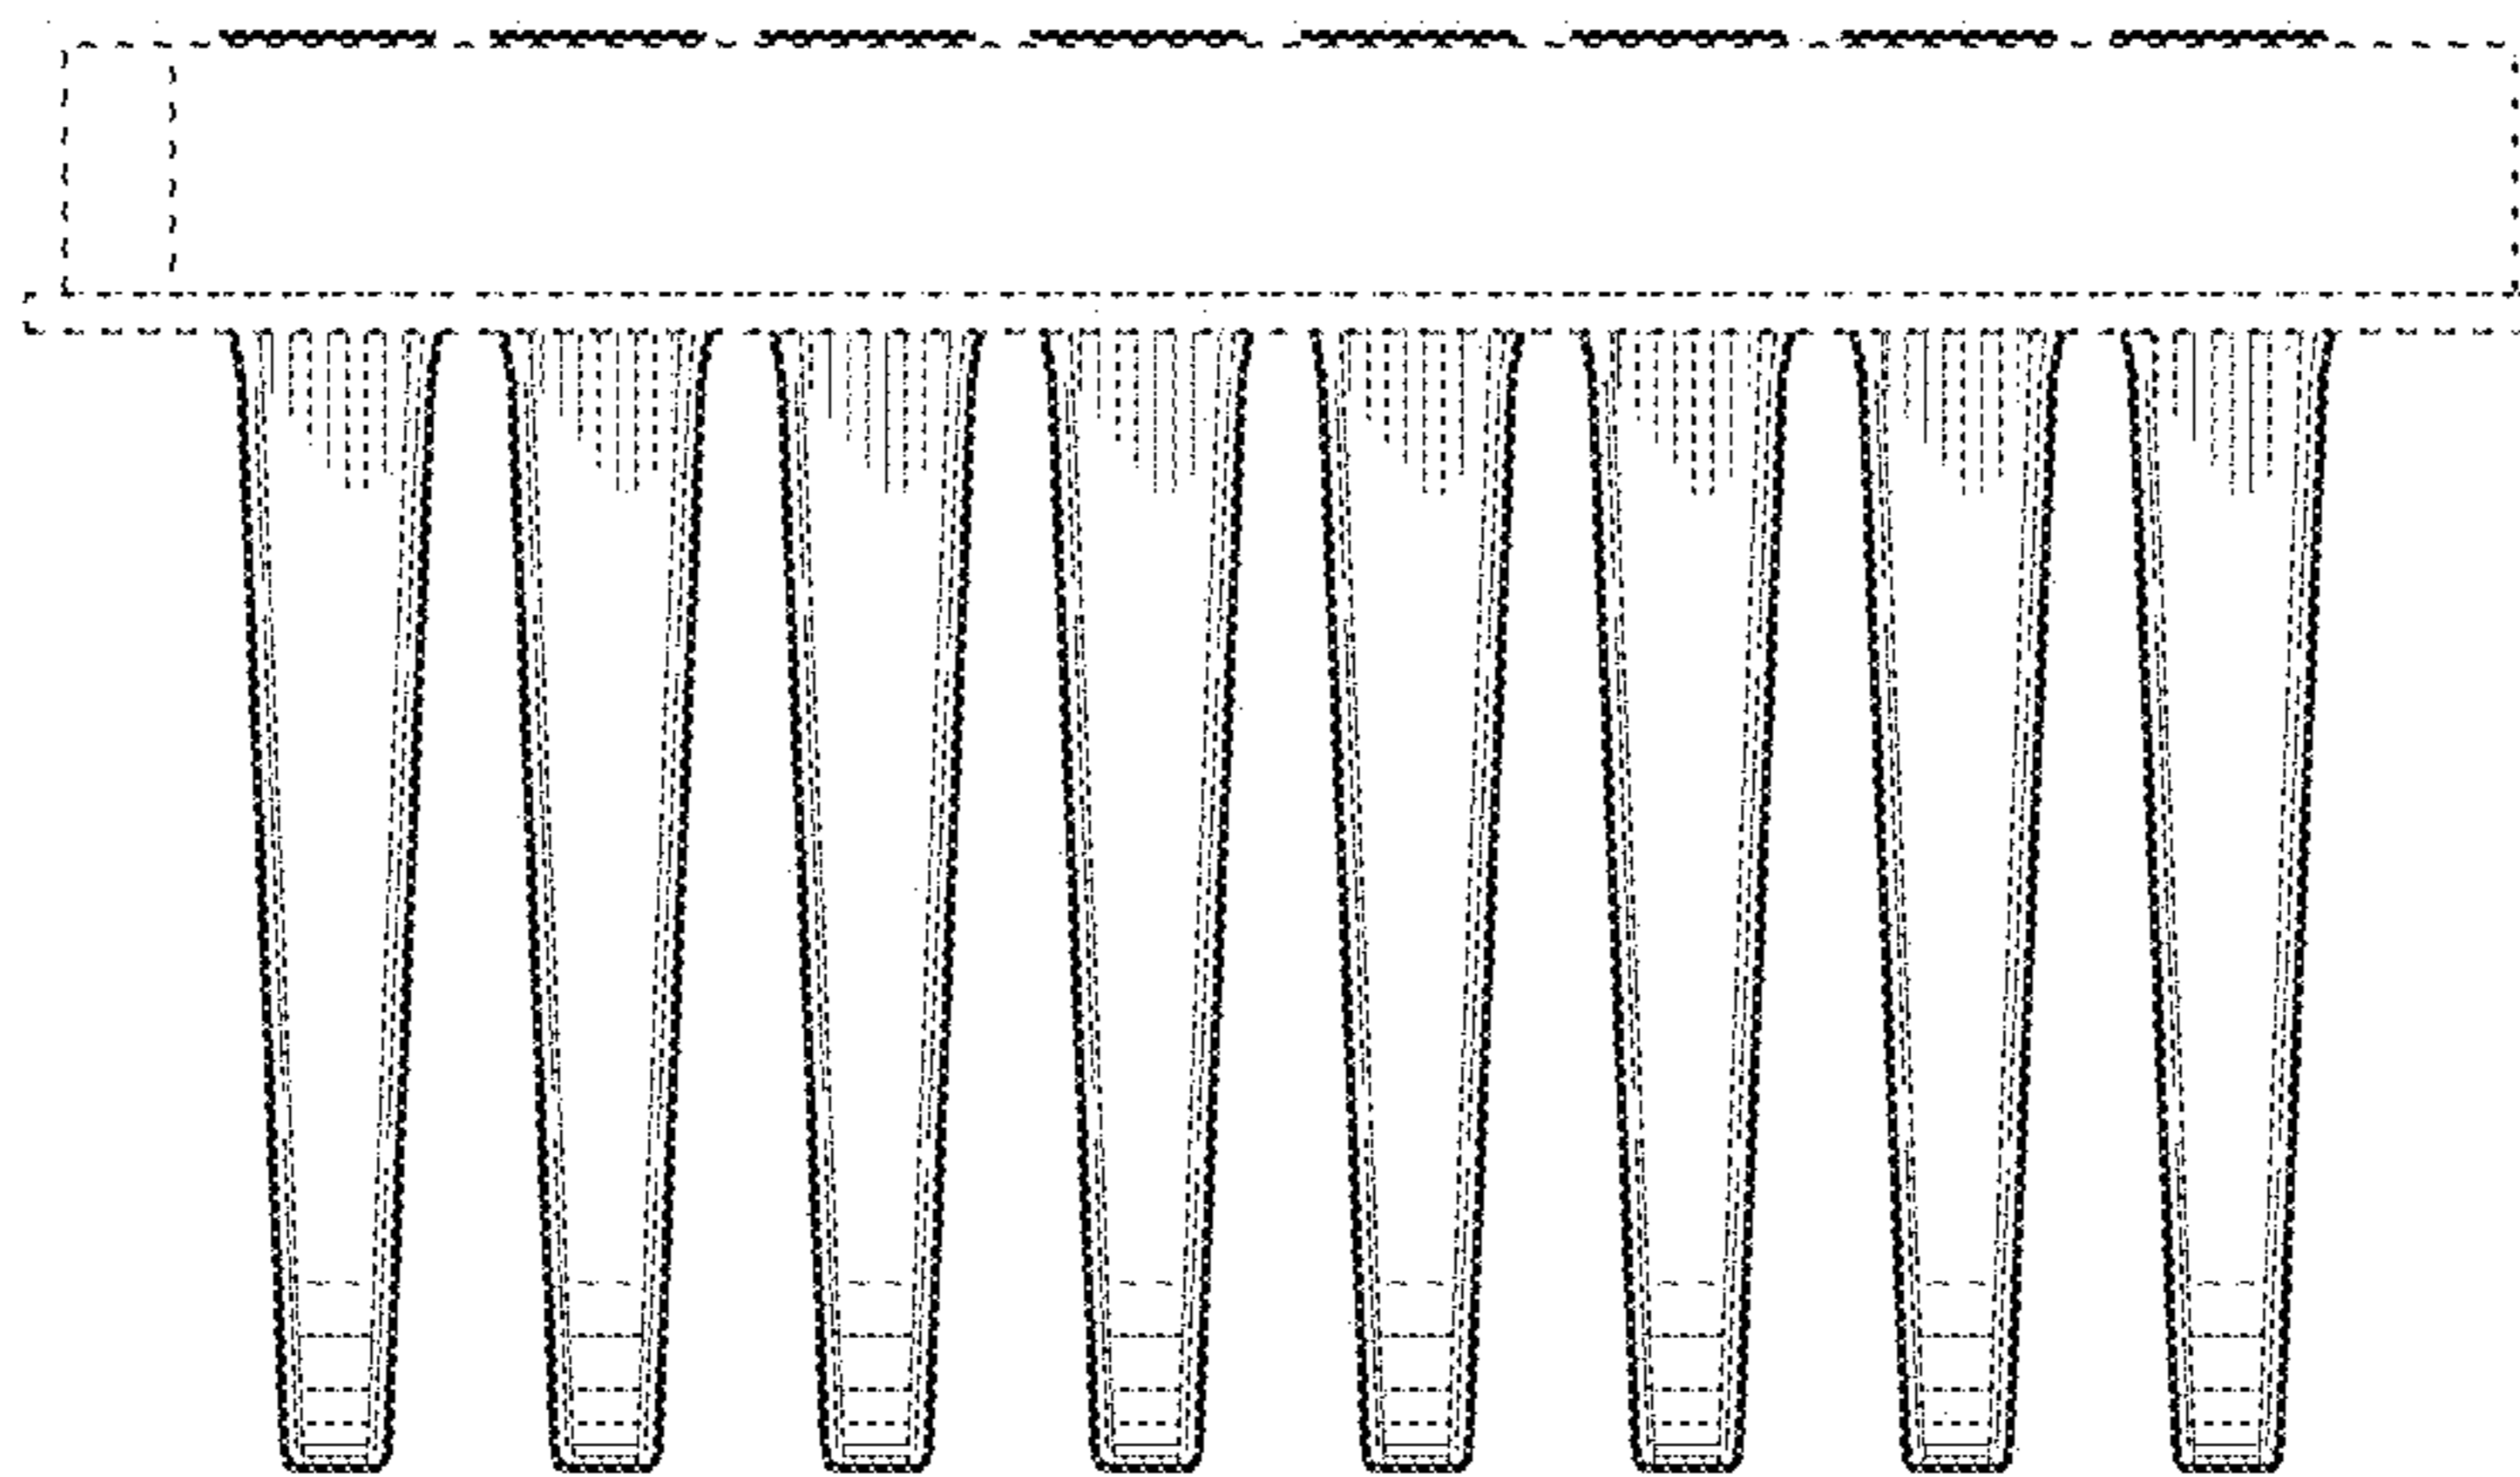


FIG. 7

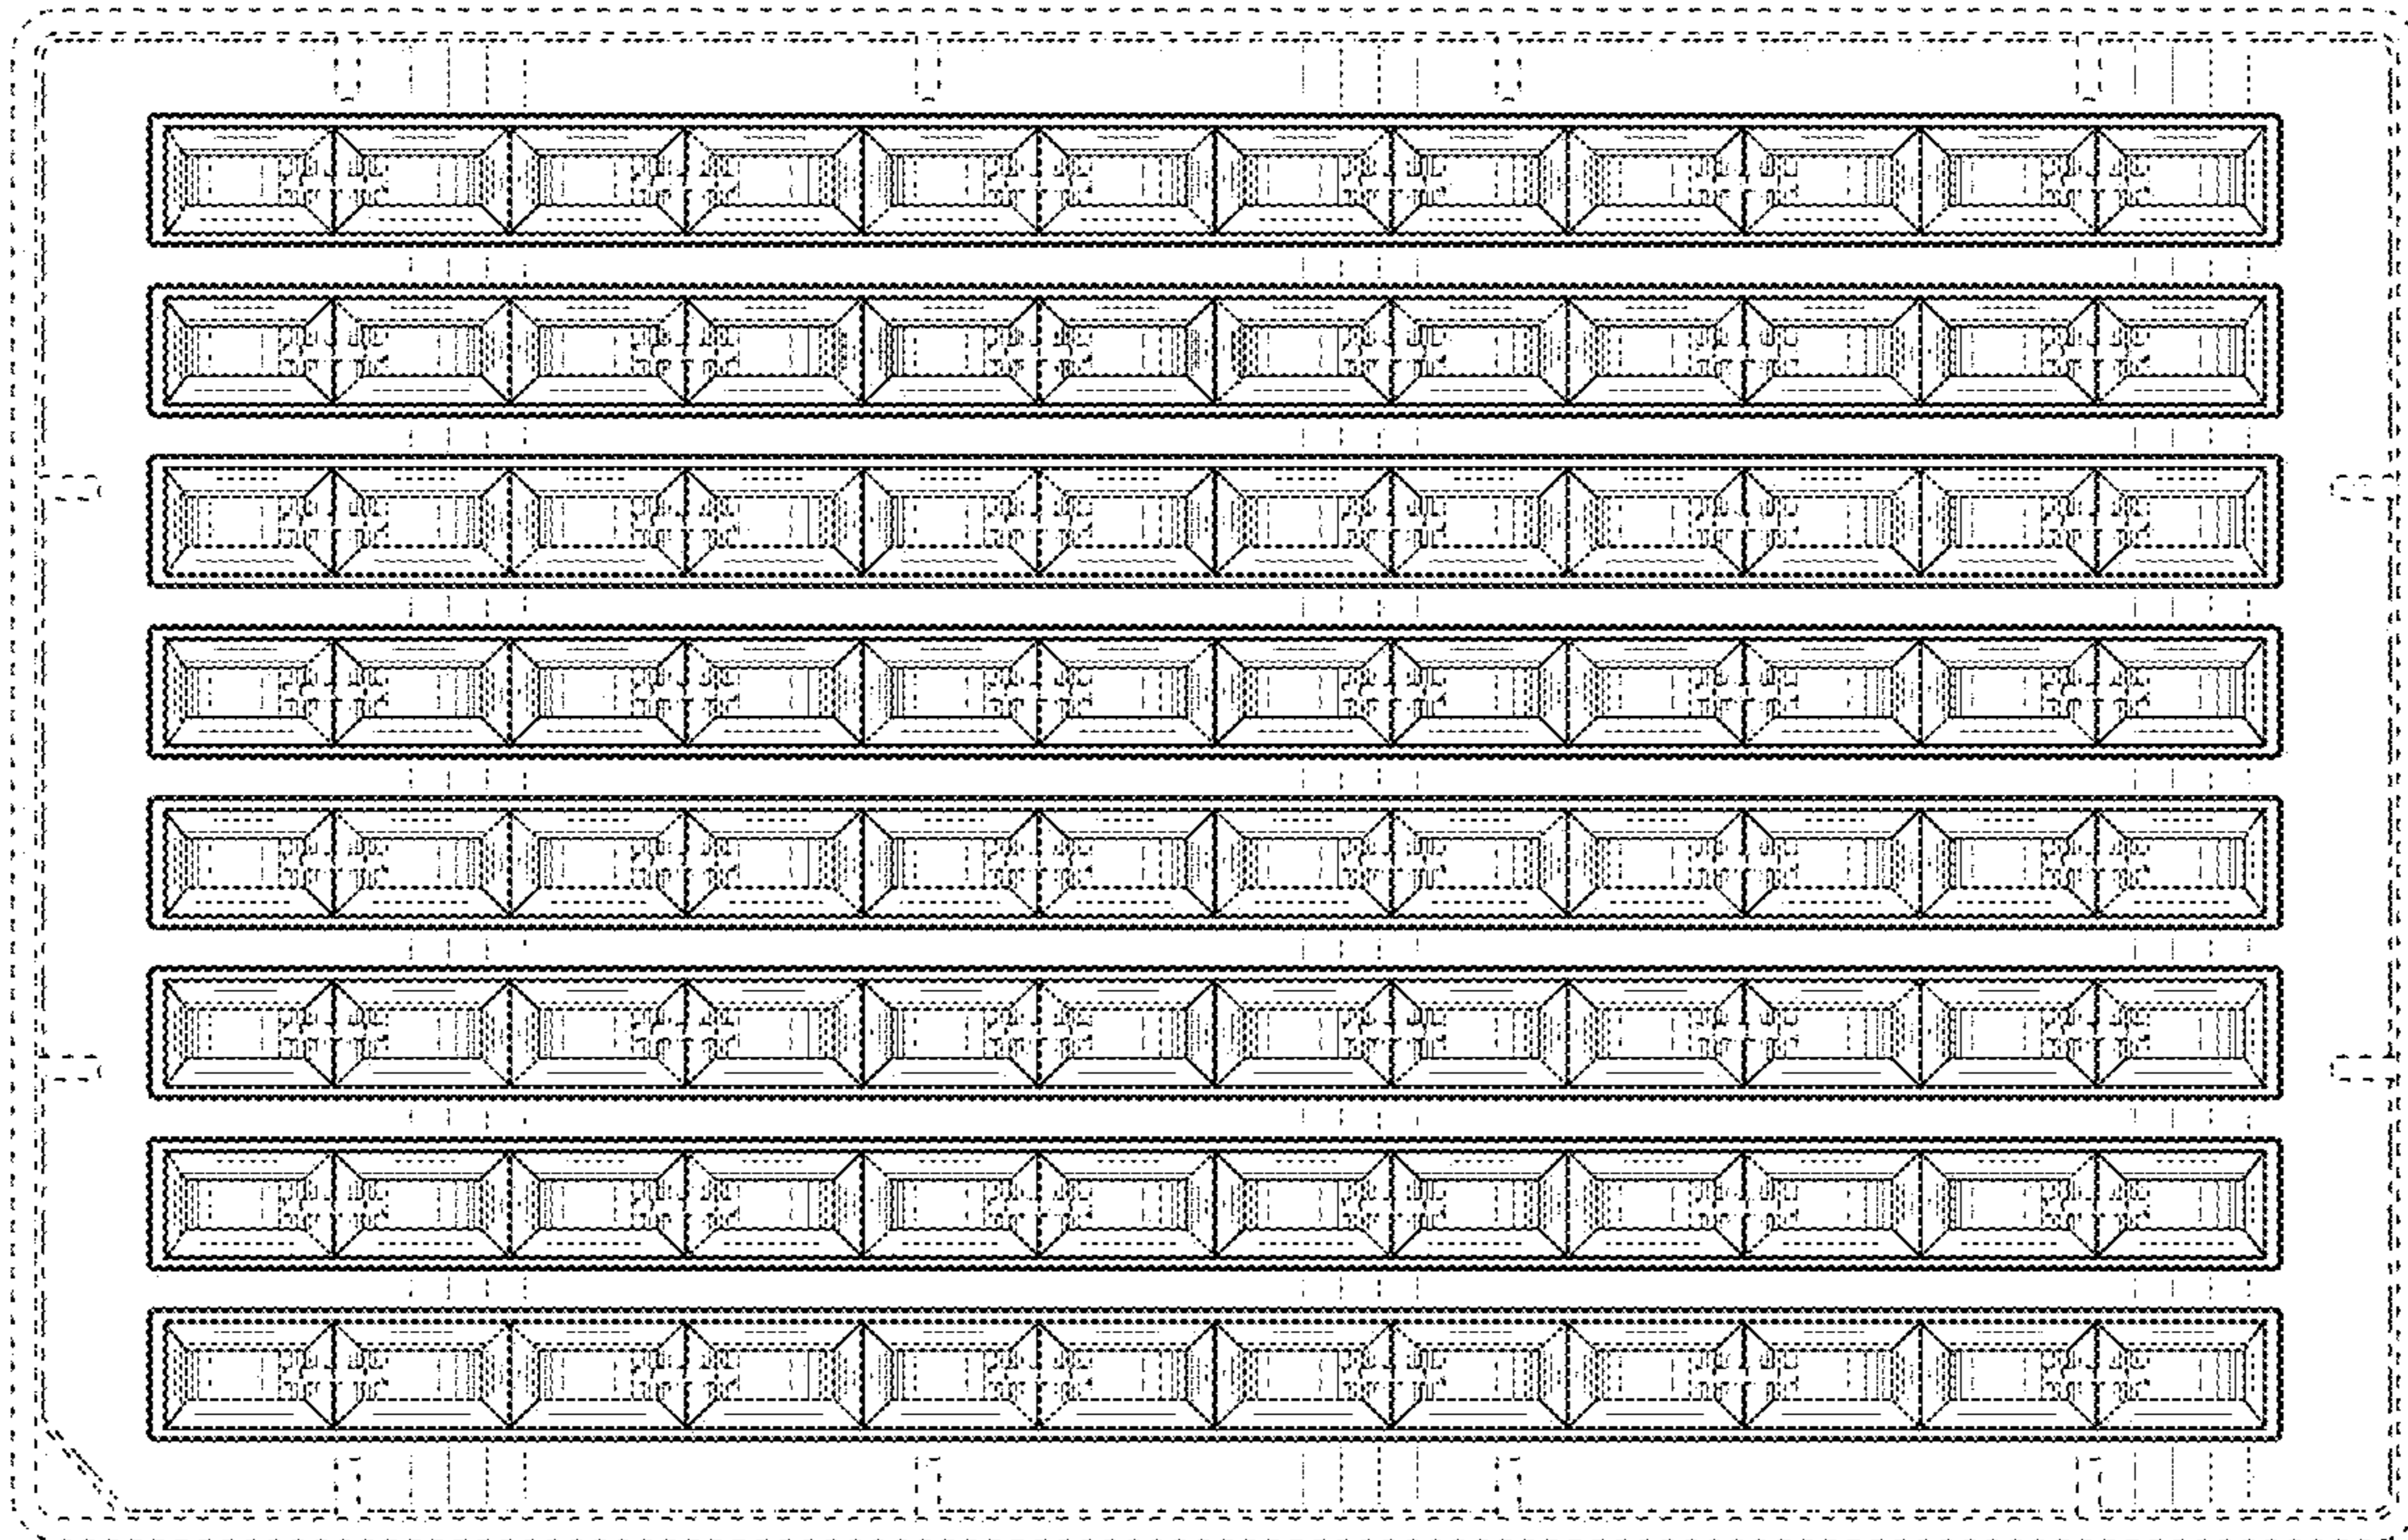


FIG. 8

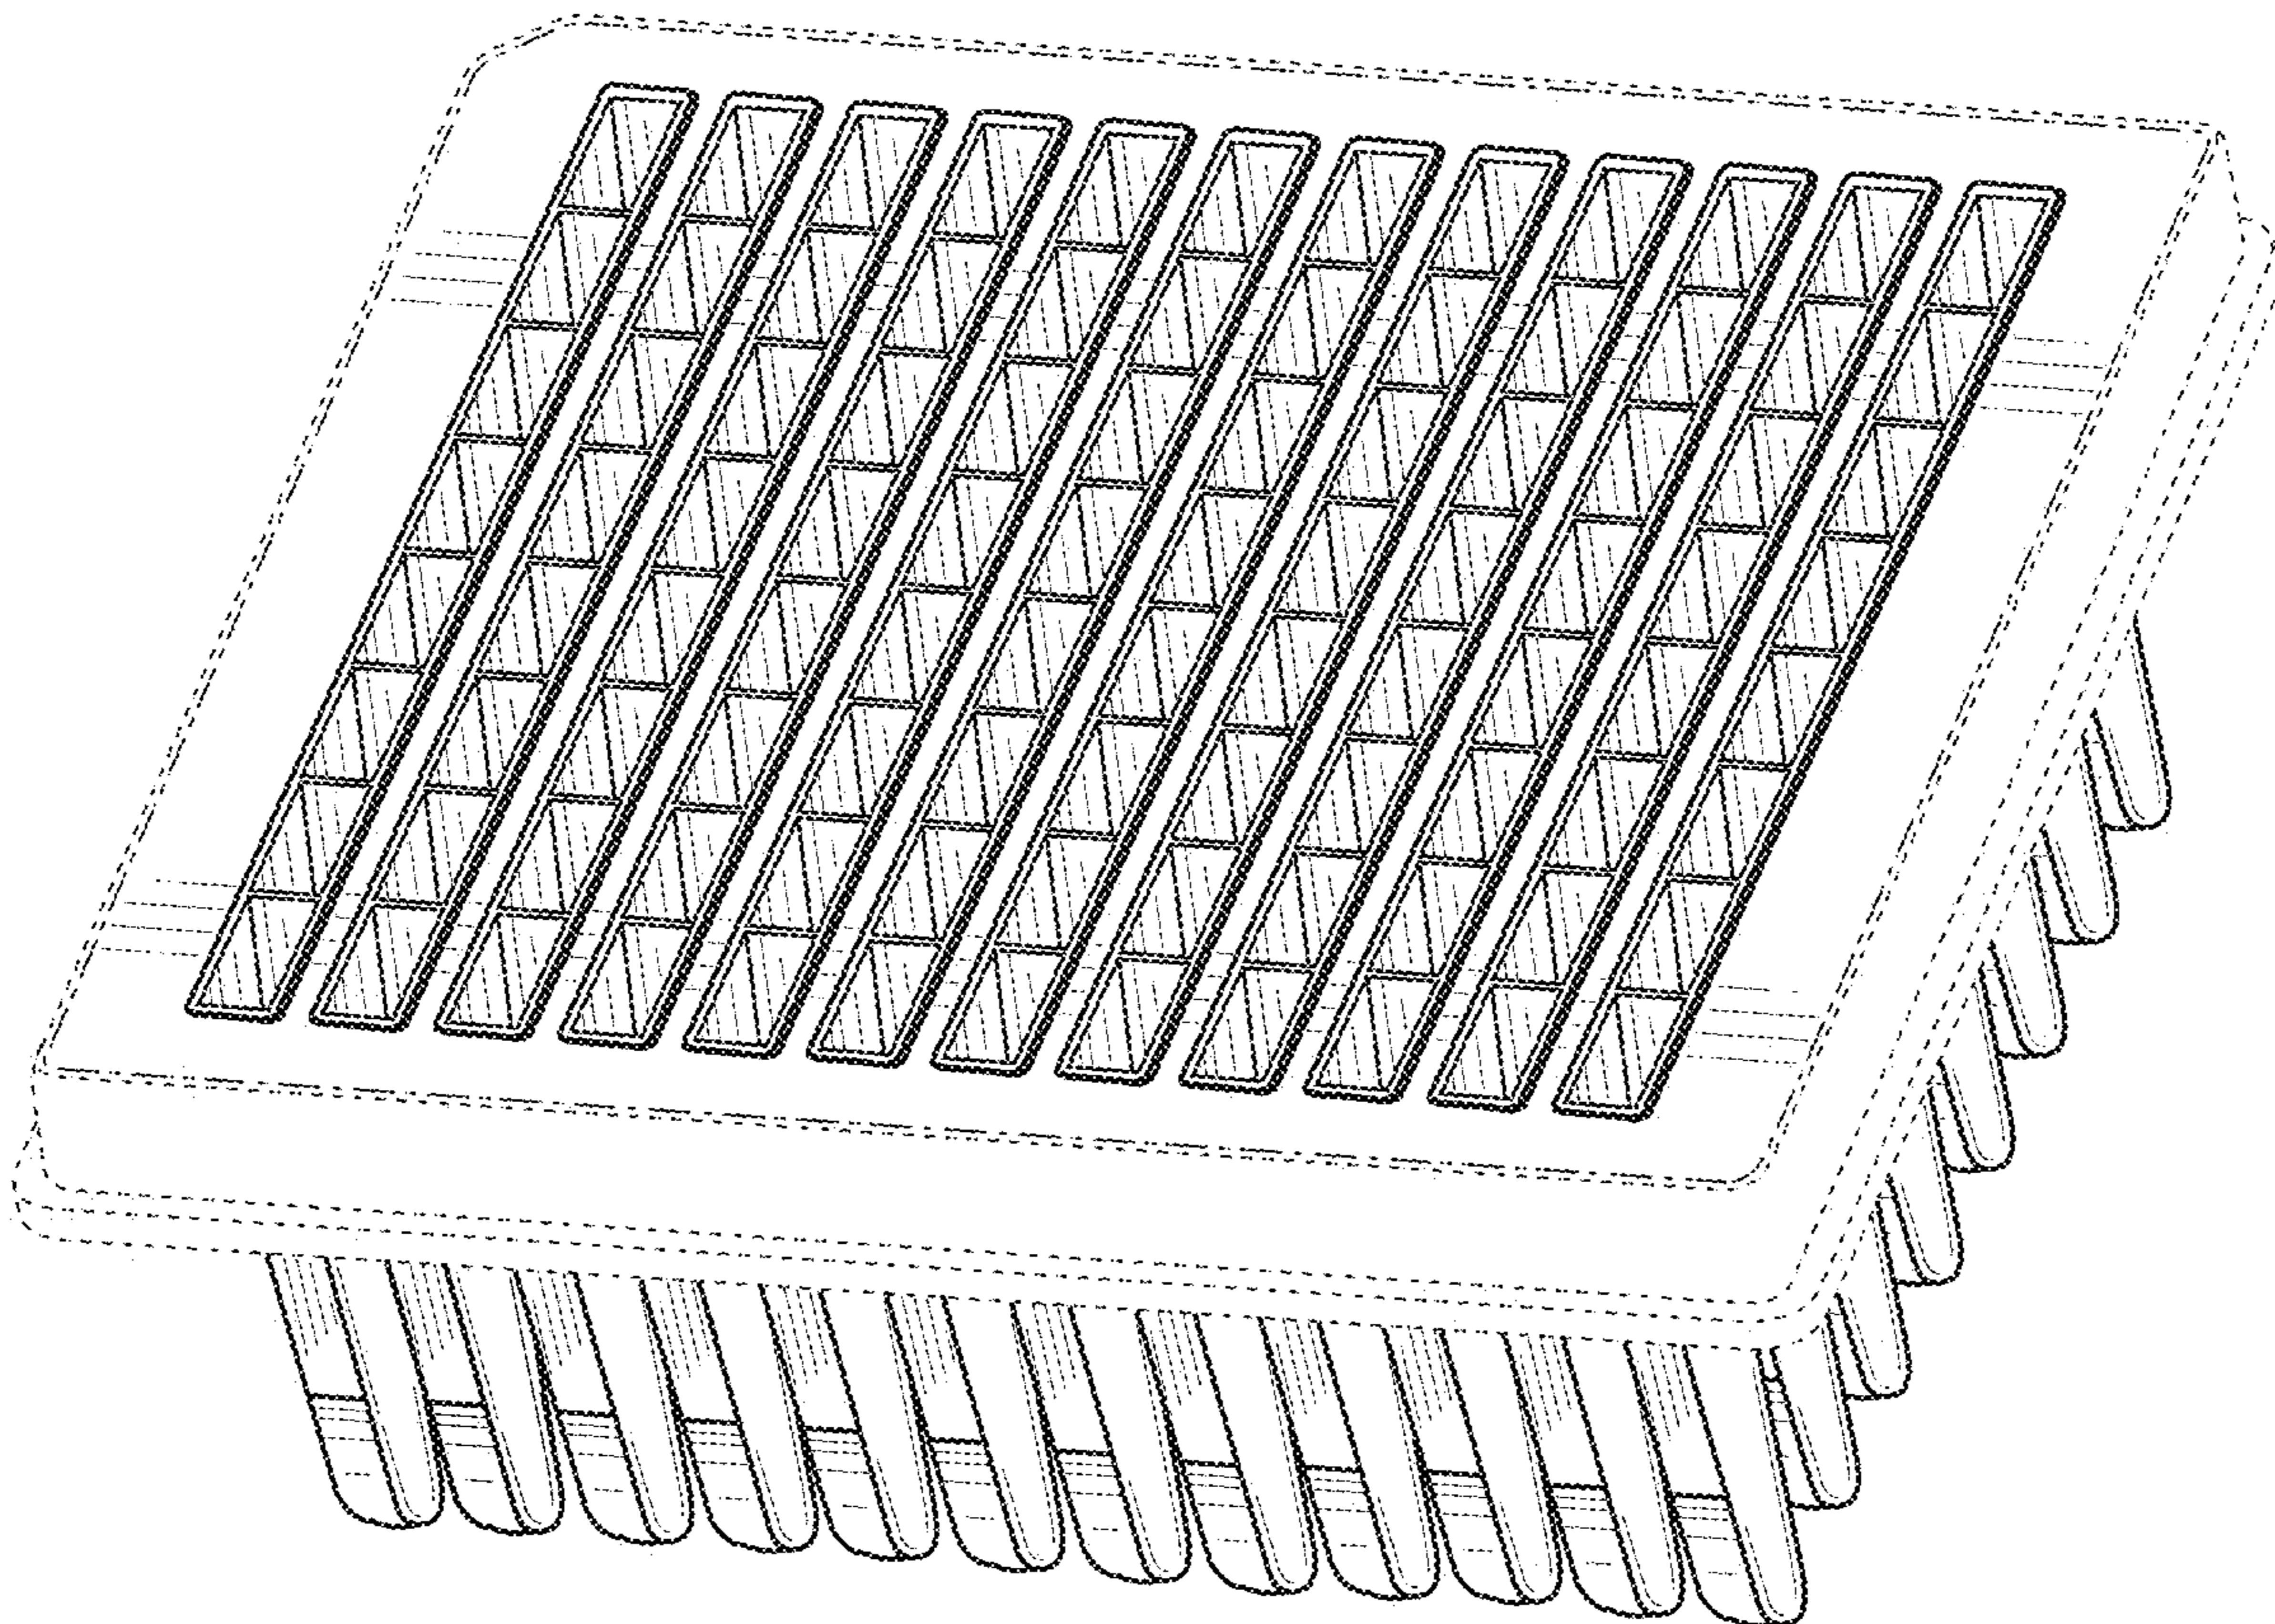


FIG. 9

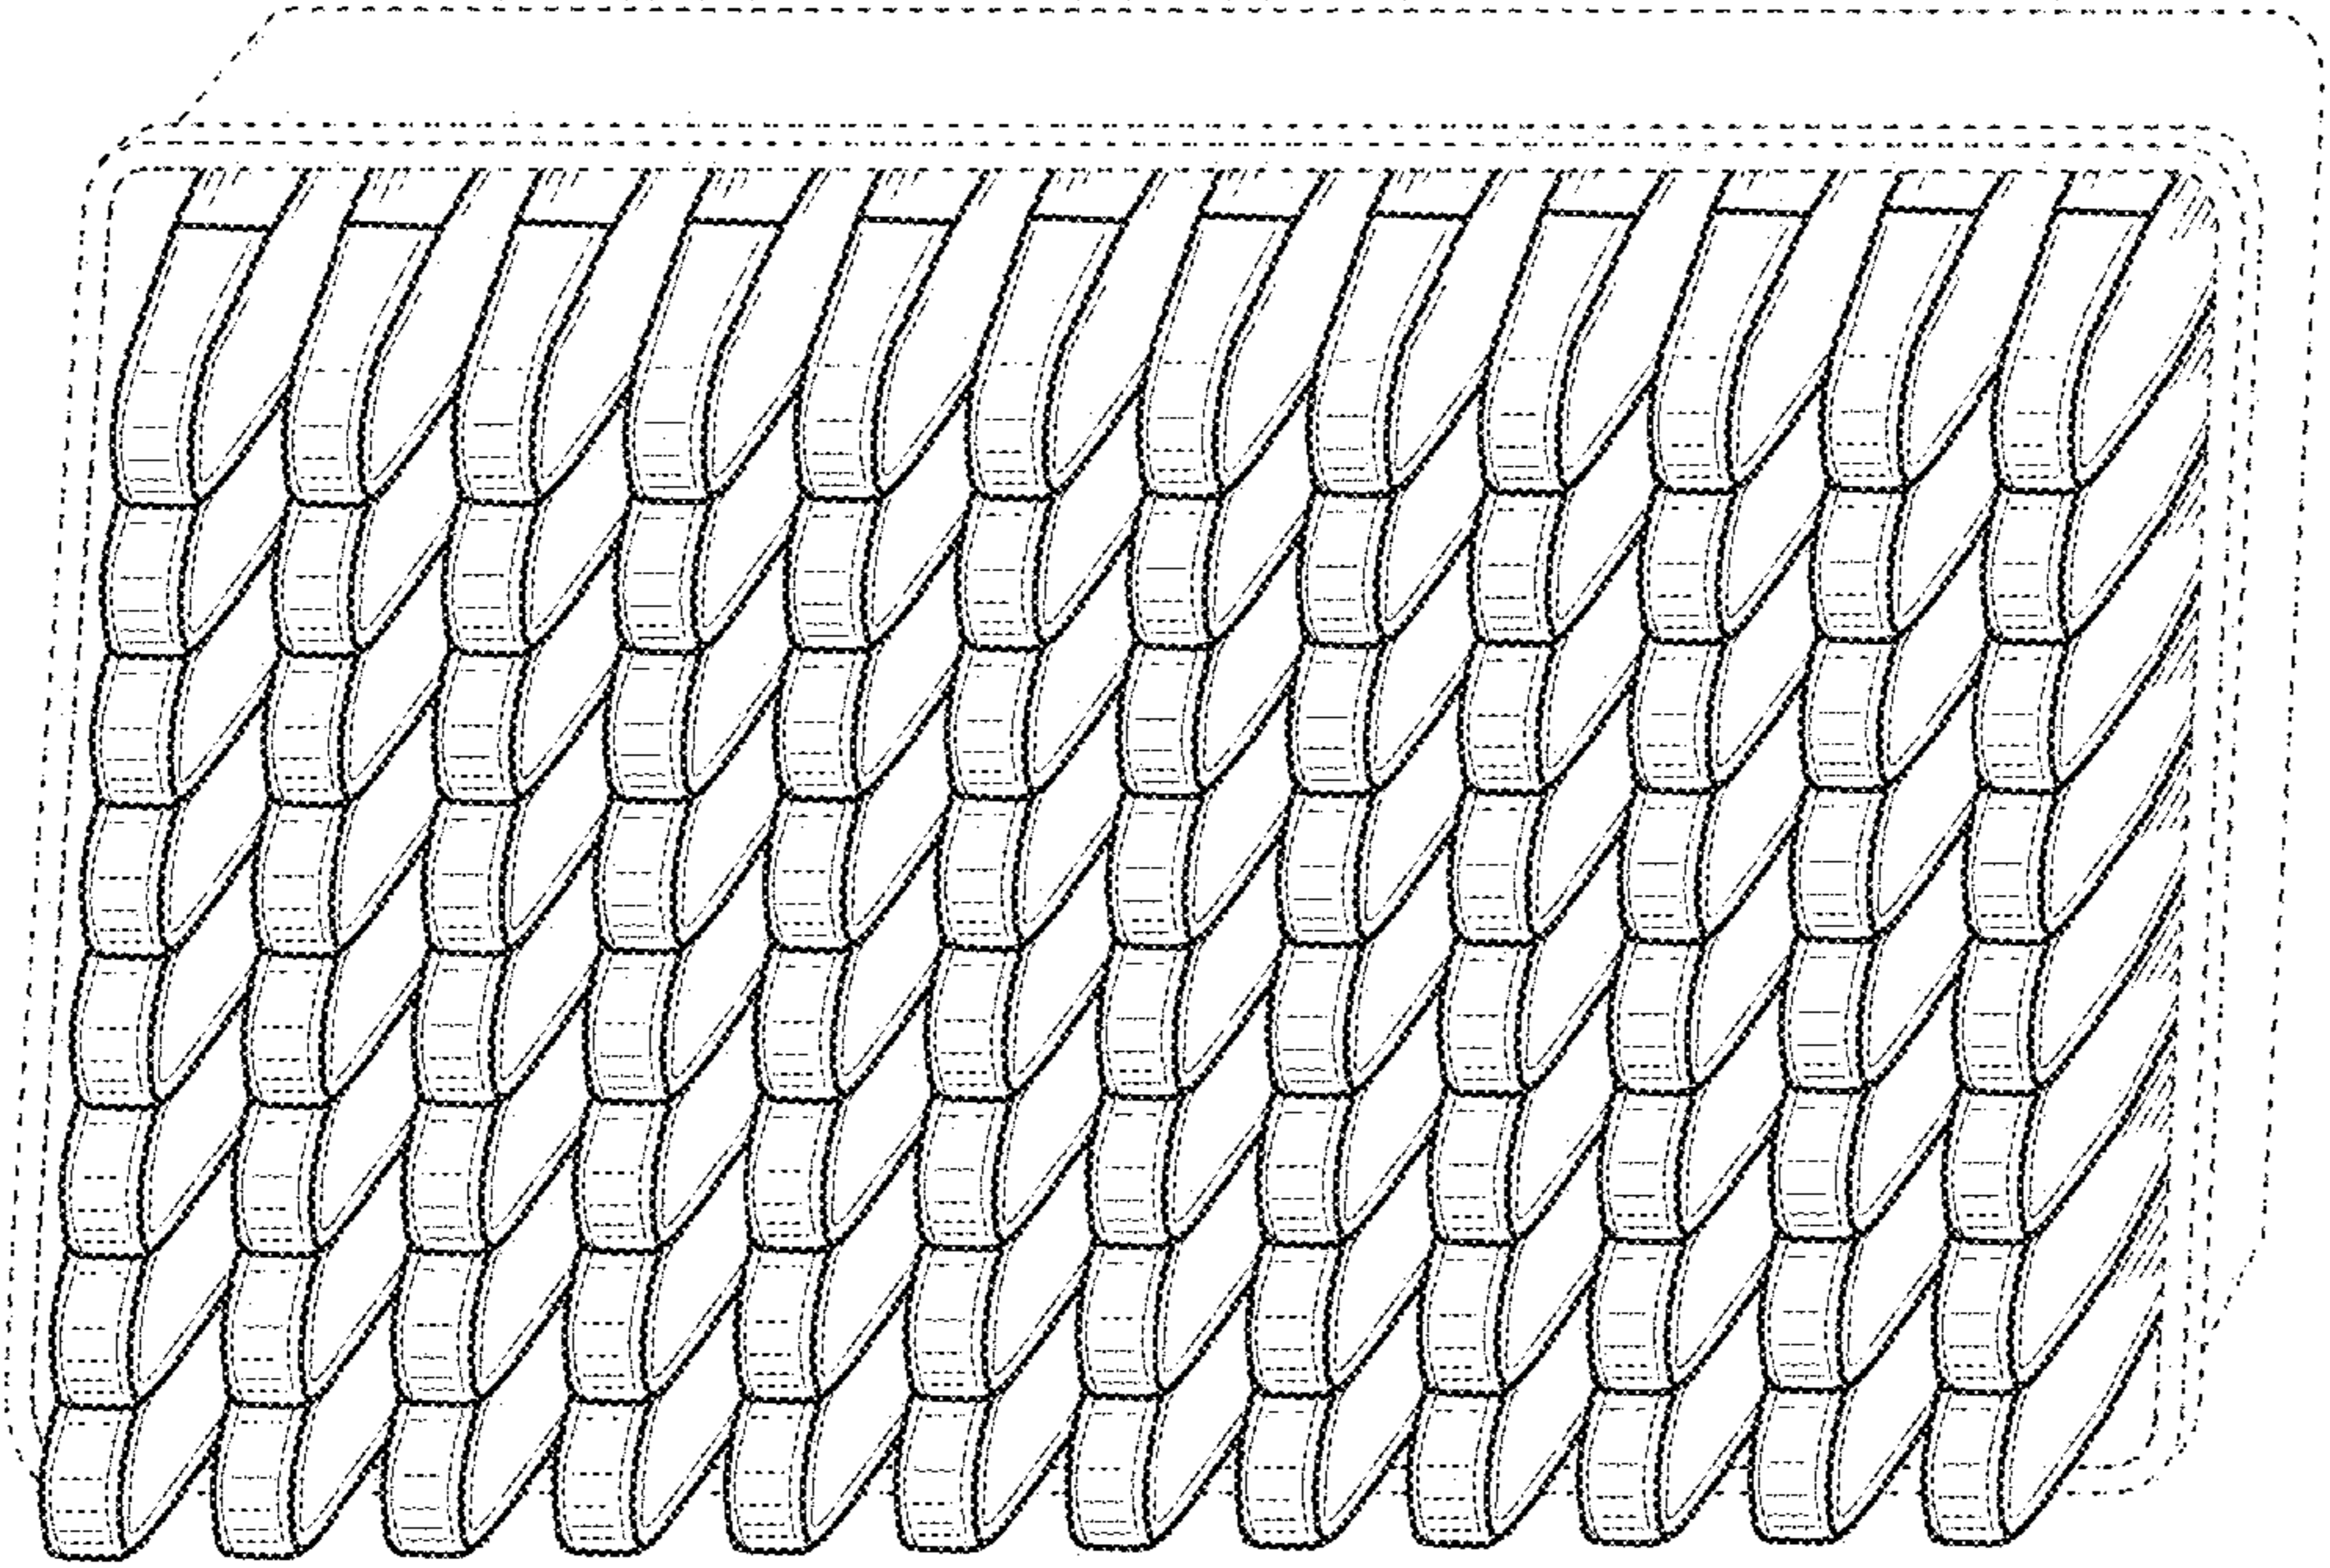


FIG. 10

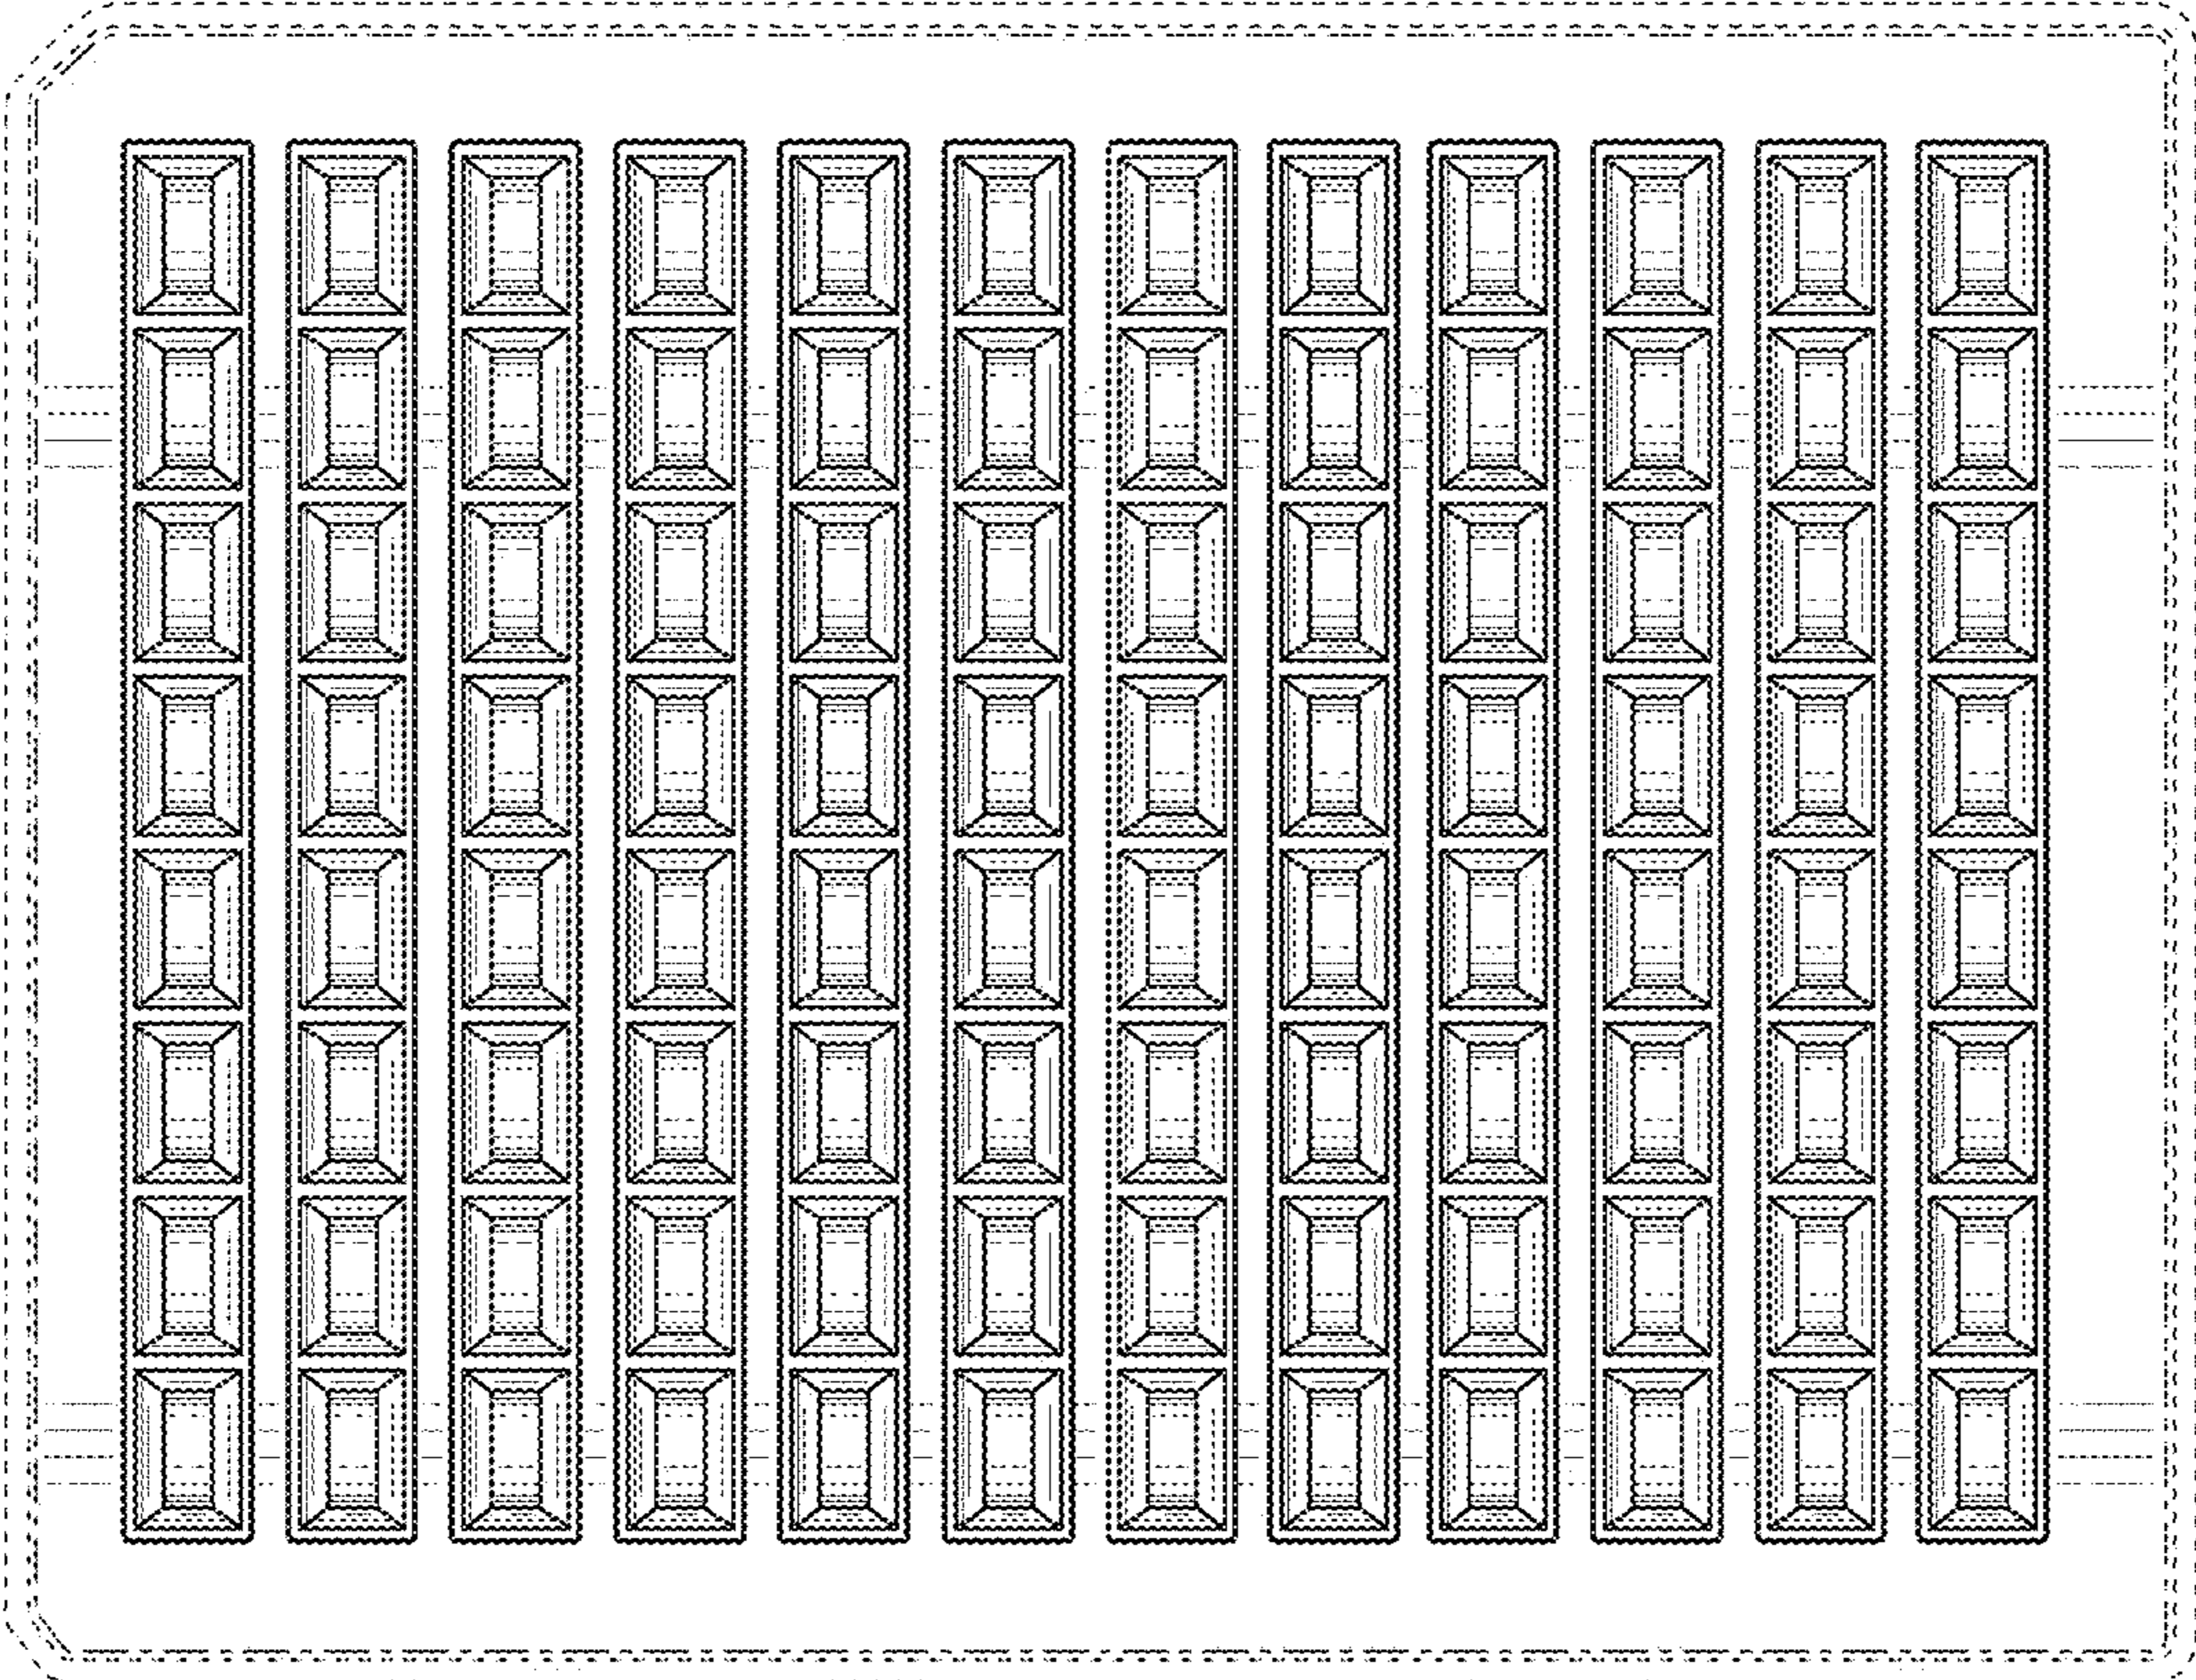


FIG. 11

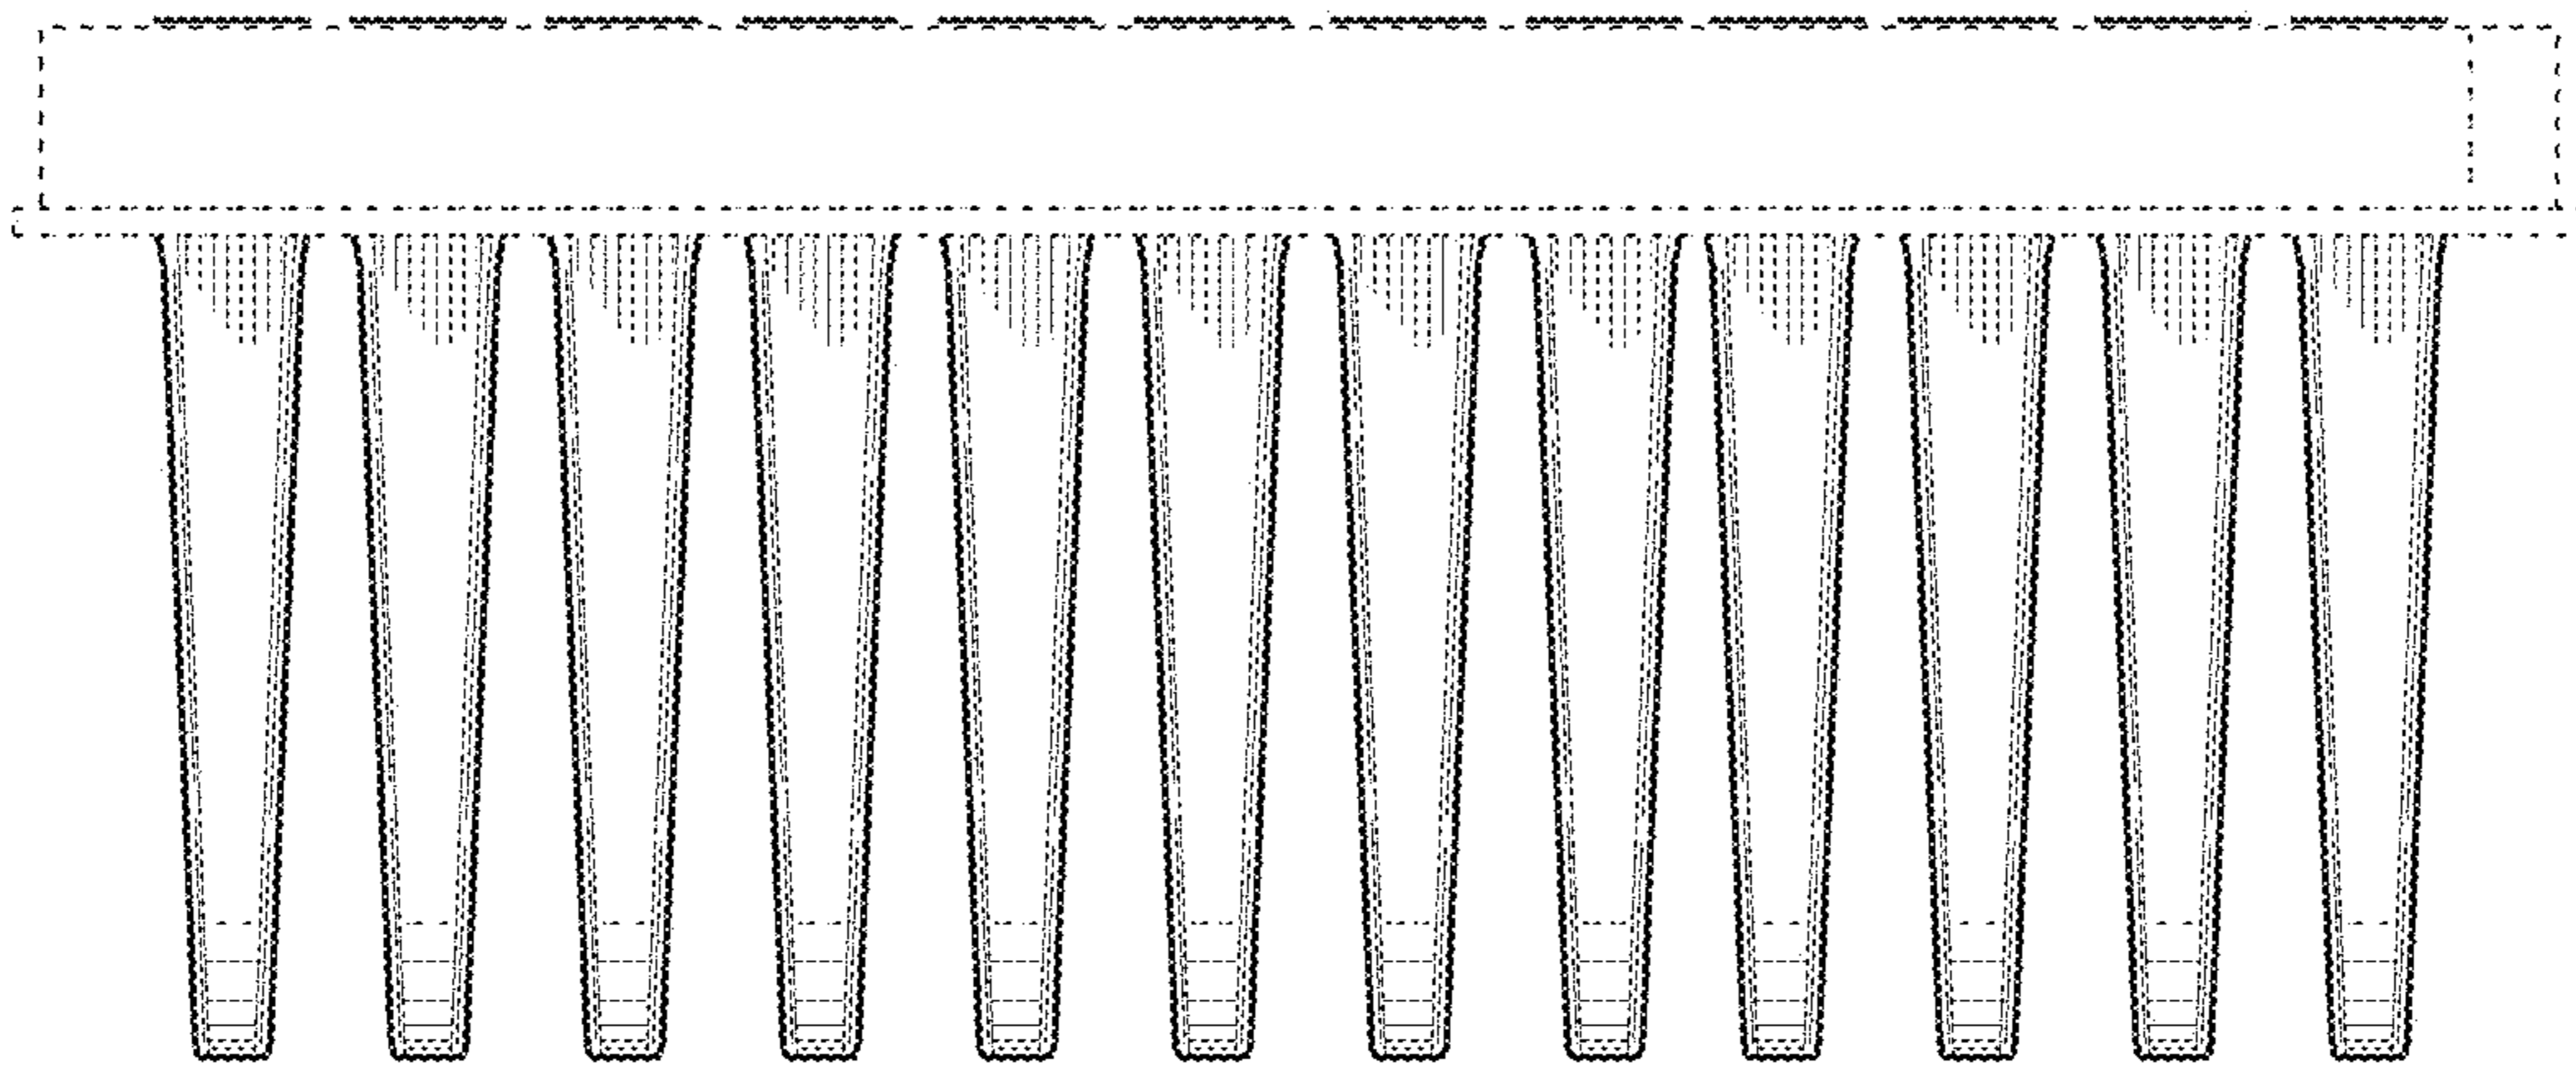


FIG. 12

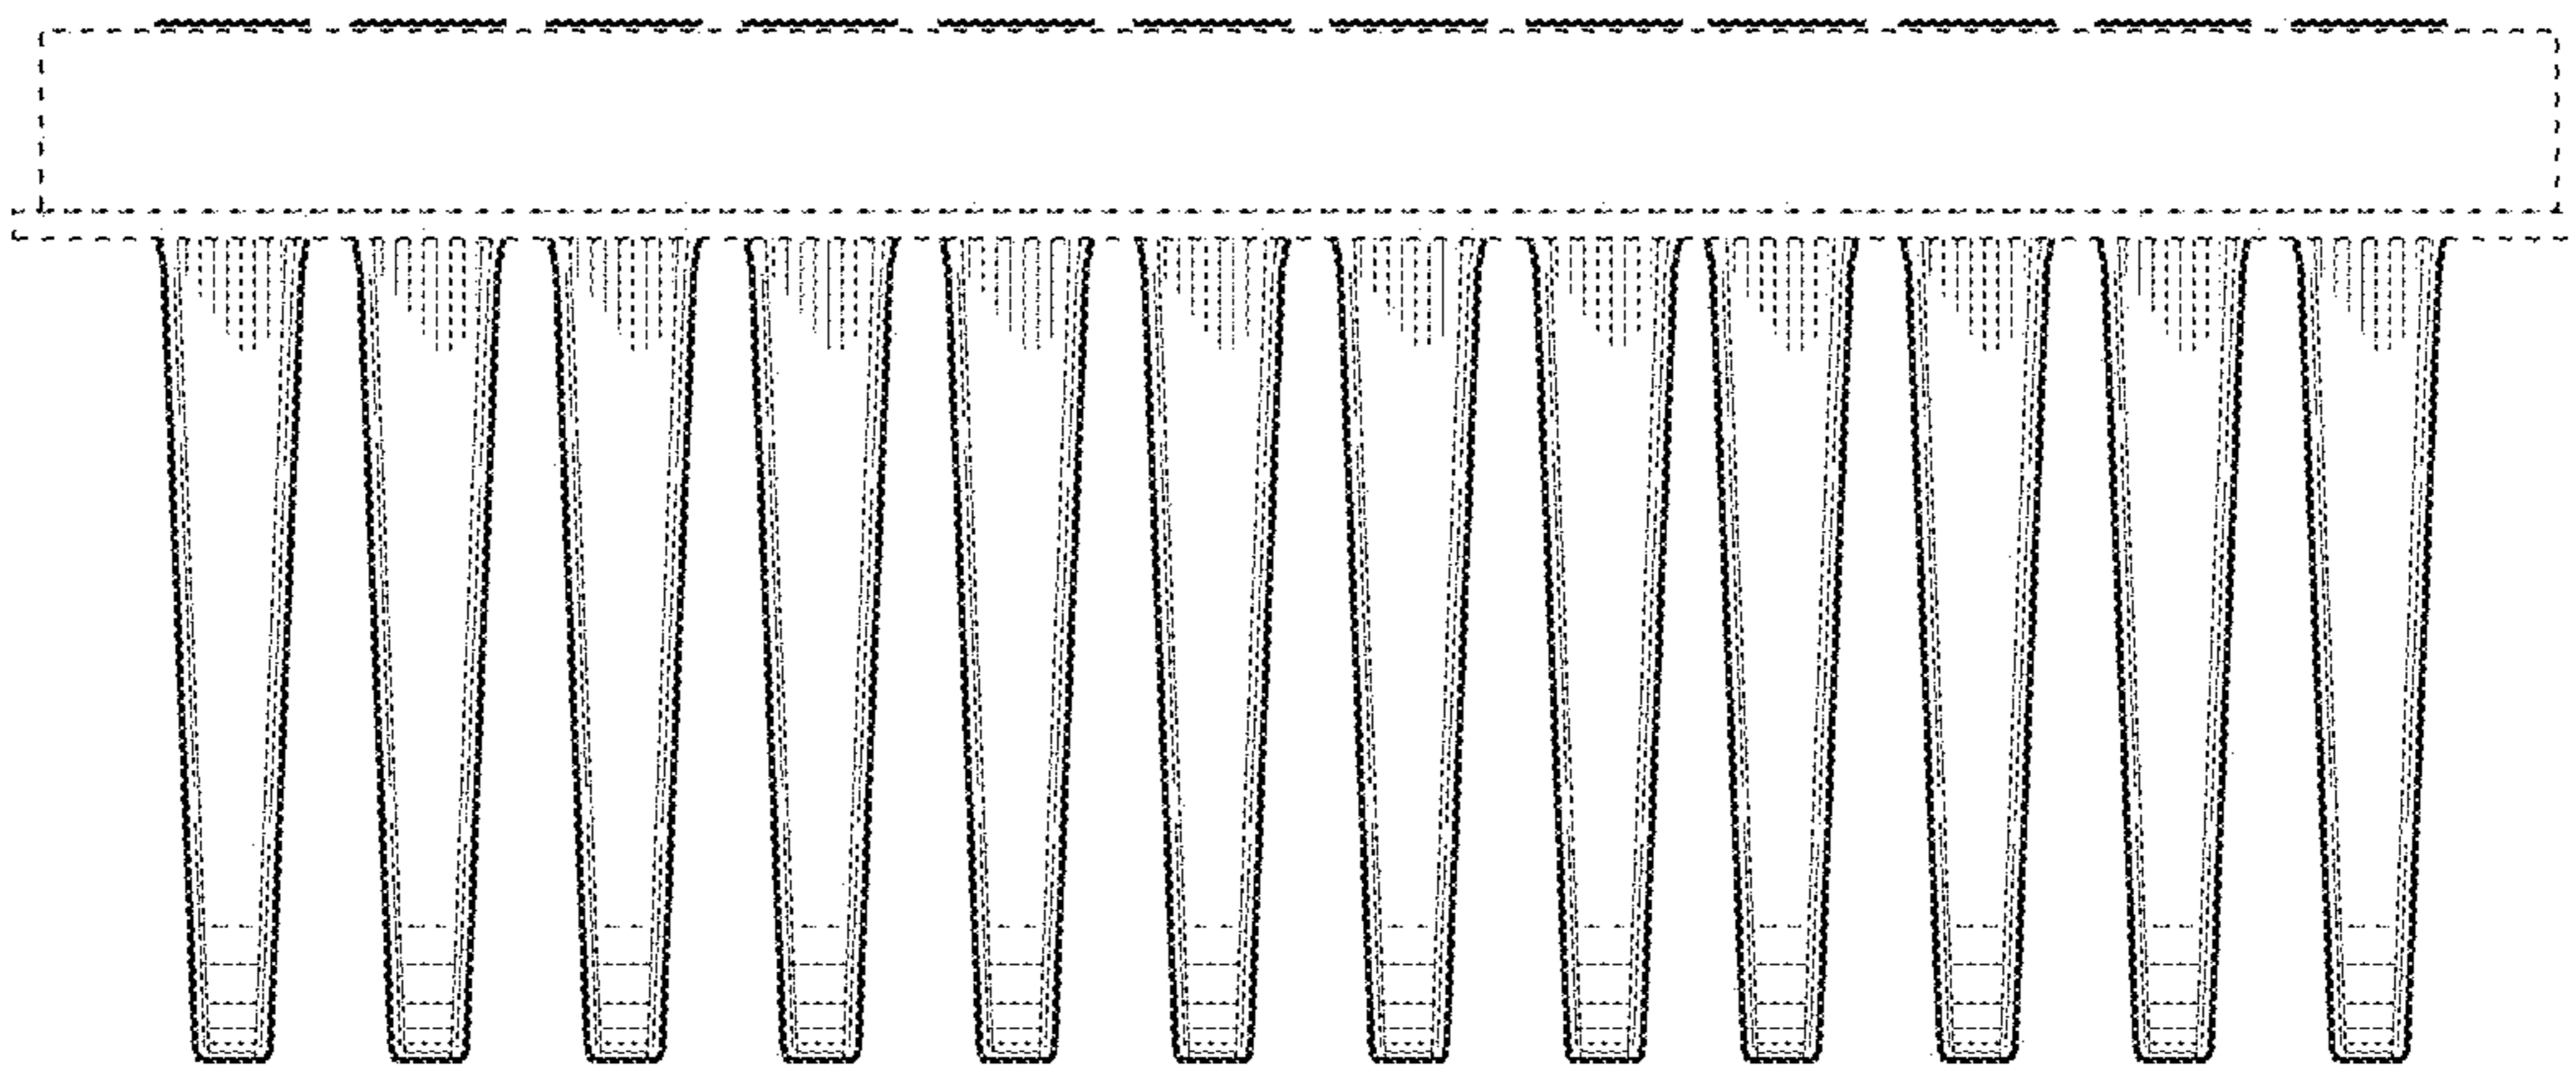


FIG. 13

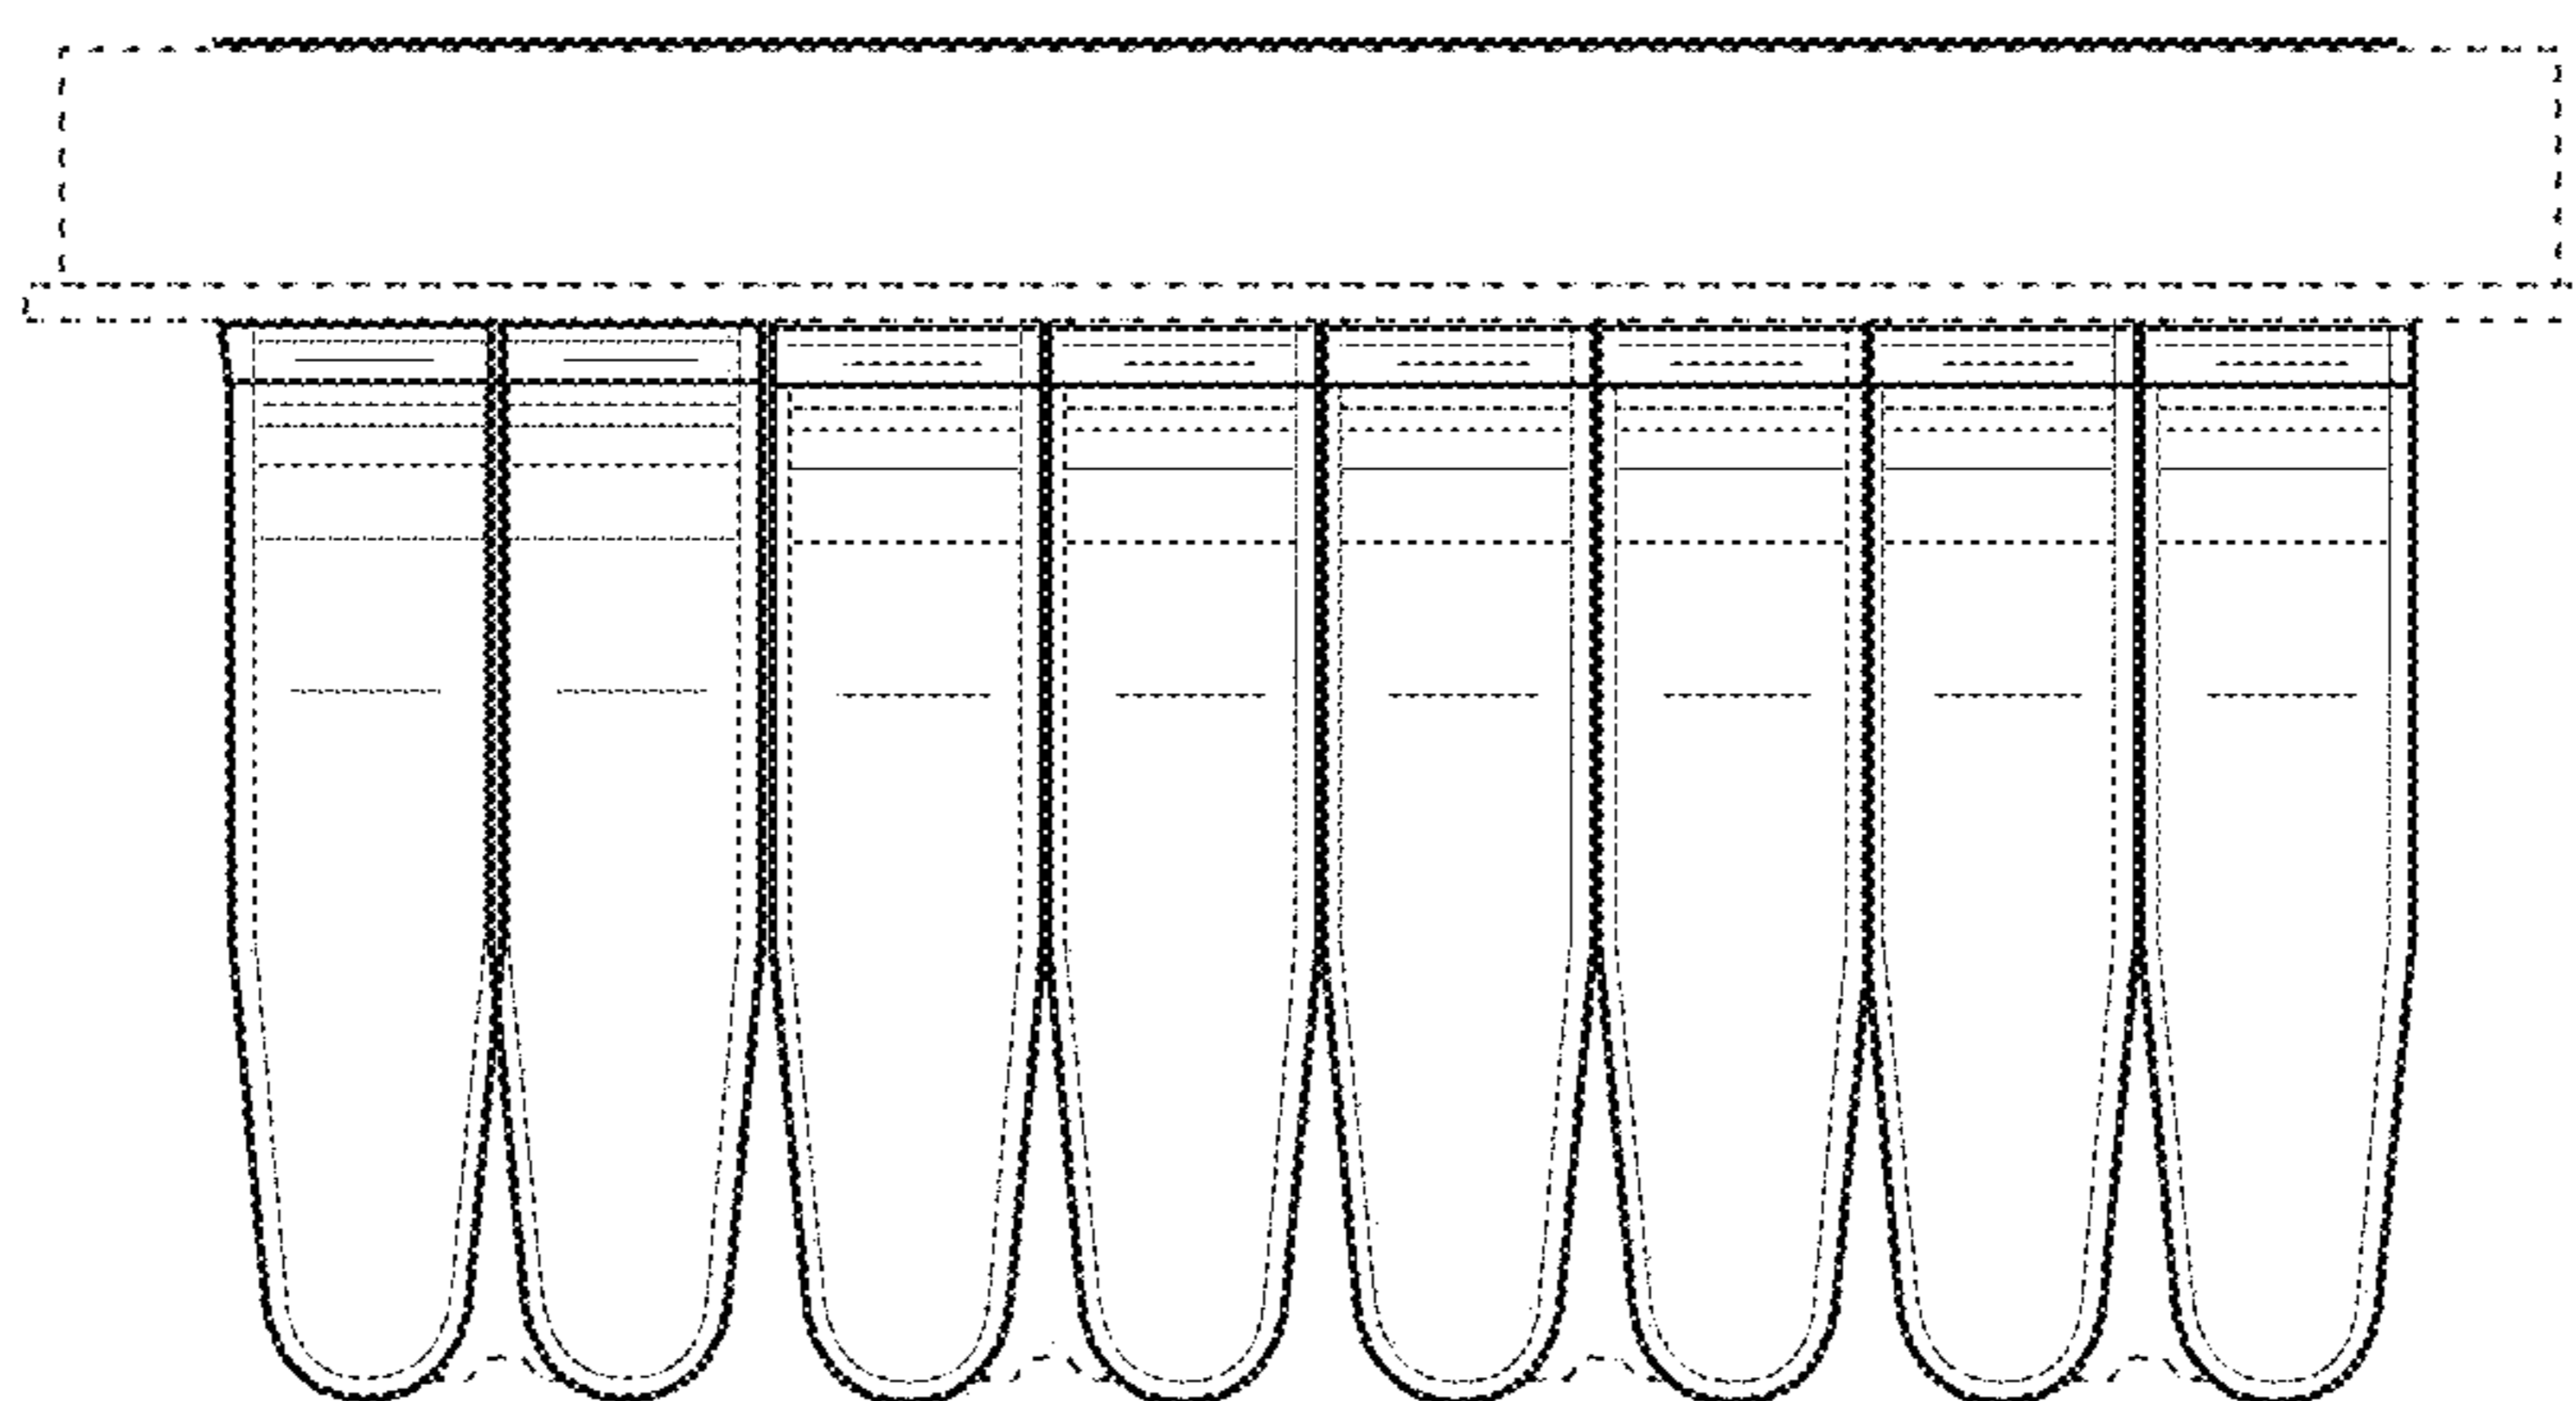


FIG. 14

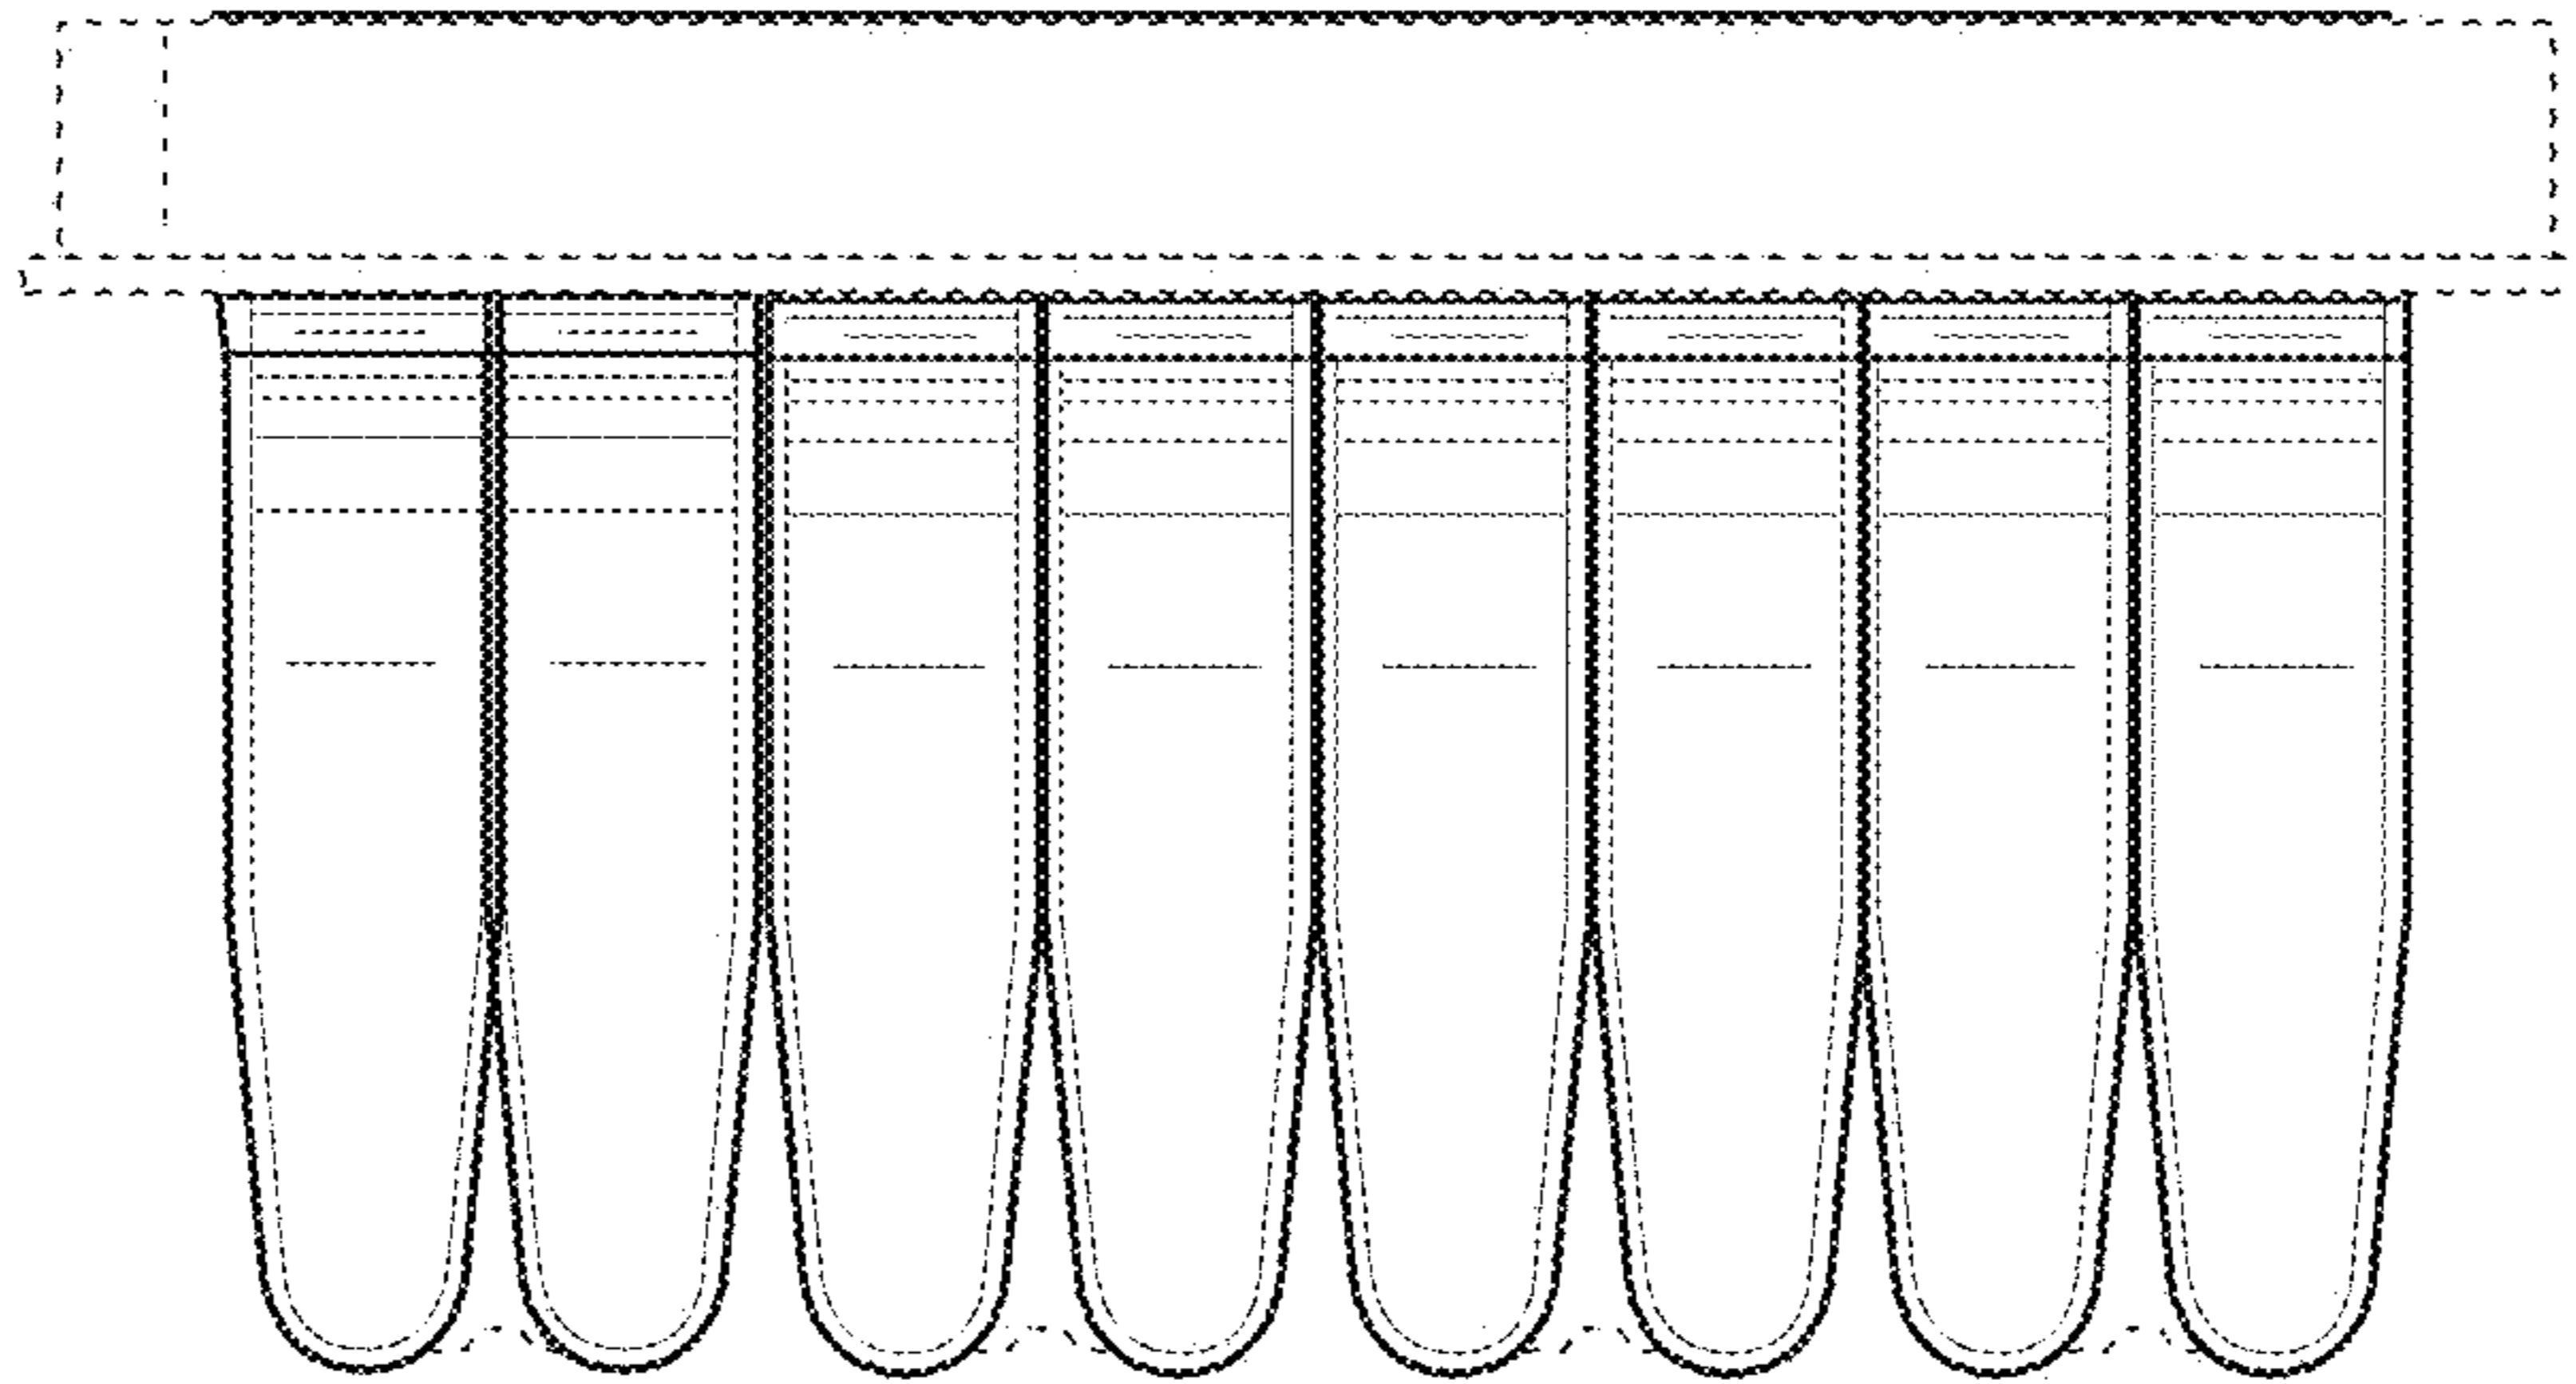


FIG. 15

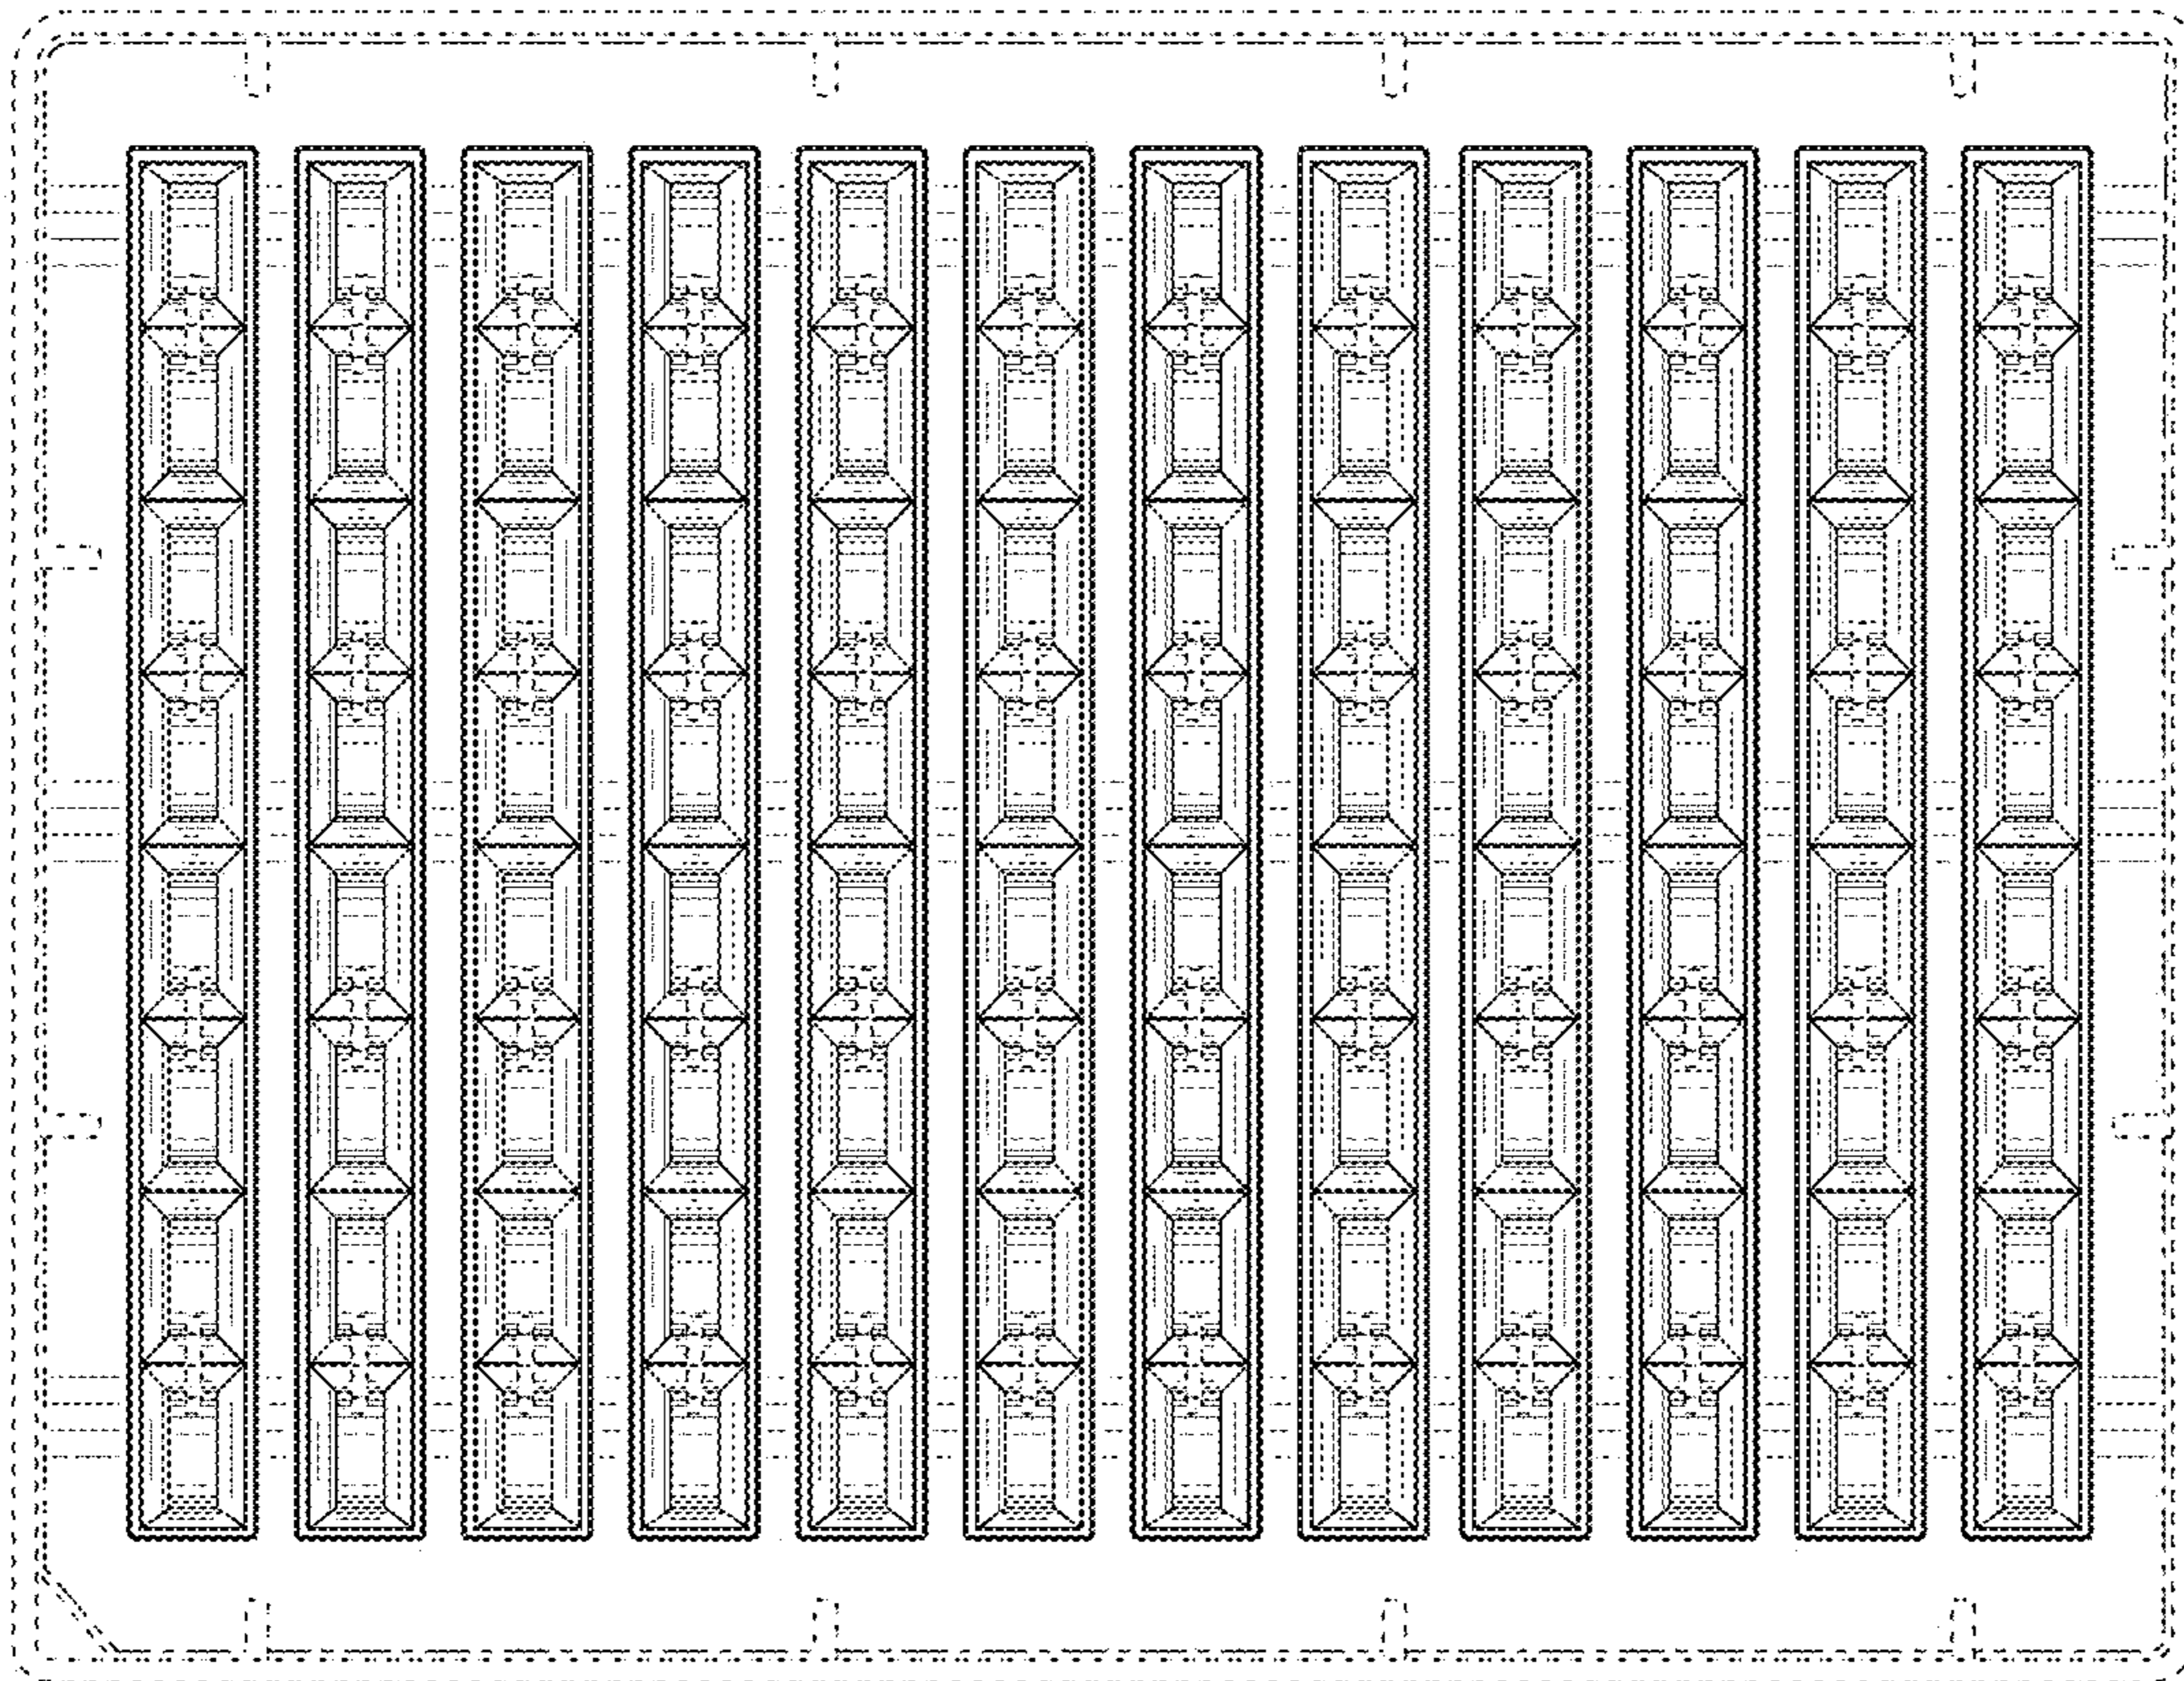


FIG. 16