



US00D956264S

(12) **United States Design Patent**
Purdy et al.

(10) **Patent No.:** **US D956,264 S**
(45) **Date of Patent:** **** Jun. 28, 2022**

- (54) **SPECIMEN IMAGING TRAY**
- (71) Applicant: **Faxitron Bioptics, LLC**, Tucson, AZ (US)
- (72) Inventors: **Ciaran Purdy**, Tucson, AZ (US); **Brad Jackson**, Tucson, AZ (US); **Jared Moore**, Tucson, AZ (US)
- (73) Assignee: **Faxitron Bioptics, LLC**, Marlborough, MA (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/743,508**
- (22) Filed: **Jul. 22, 2020**

Related U.S. Application Data

- (63) Continuation of application No. 29/670,827, filed on Nov. 20, 2018, now Pat. No. Des. 895,838.
- (51) **LOC (13) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/227**
- (58) **Field of Classification Search**
USPC D24/216, 224, 226, 227, 229, 230;
D9/439, 440, 452, 454
CPC B01L 9/00
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,055,808 A * 9/1962 Henderson C12M 23/34
435/305.3
- D237,981 S 12/1975 Mastrell
- D322,323 S 12/1991 Moir
- 5,449,071 A * 9/1995 Levy A61B 10/0096
206/569
- D439,637 S 3/2001 Davies
- D521,381 S * 5/2006 Hicks D9/449
- D535,755 S * 1/2007 Discko, Jr. D24/221

- D674,505 S 1/2013 Cecchi
- D781,437 S 3/2017 Valley
- D787,053 S * 5/2017 Huang D24/130
- D804,051 S * 11/2017 Alexander D24/227
- D827,151 S 8/2018 Nakagawa
- D895,838 S 9/2020 Purdy
- D925,759 S * 7/2021 Suzuki D24/216
- D927,015 S * 8/2021 Thomas D24/224
- D930,850 S * 9/2021 Zollinger D24/224
- 2005/0089997 A1 * 4/2005 Minton C12M 23/38
435/288.3

(Continued)

Primary Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Merchant & Gould P.C.

(57) **CLAIM**

The ornamental design for a “specimen imaging tray,” as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a specimen imaging tray, showing our new design.

FIG. 2 is a bottom perspective view of the specimen imaging tray of FIG. 1.

FIG. 3 is a front view of the specimen imaging tray of FIG. 1.

FIG. 4 is a rear view of the specimen imaging tray of FIG. 1.


FIG. 5 is a left side view of the specimen imaging tray of FIG. 1, the right side view is a mirror image of the left side view.

FIG. 6 is a top view of the specimen imaging tray of FIG. 1; and,

FIG. 7 is a bottom view of the specimen imaging tray of FIG. 1.

The broken lines, the areas within them, and the areas bounded by broken lines and solid lines depict portions of the specimen imaging tray that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

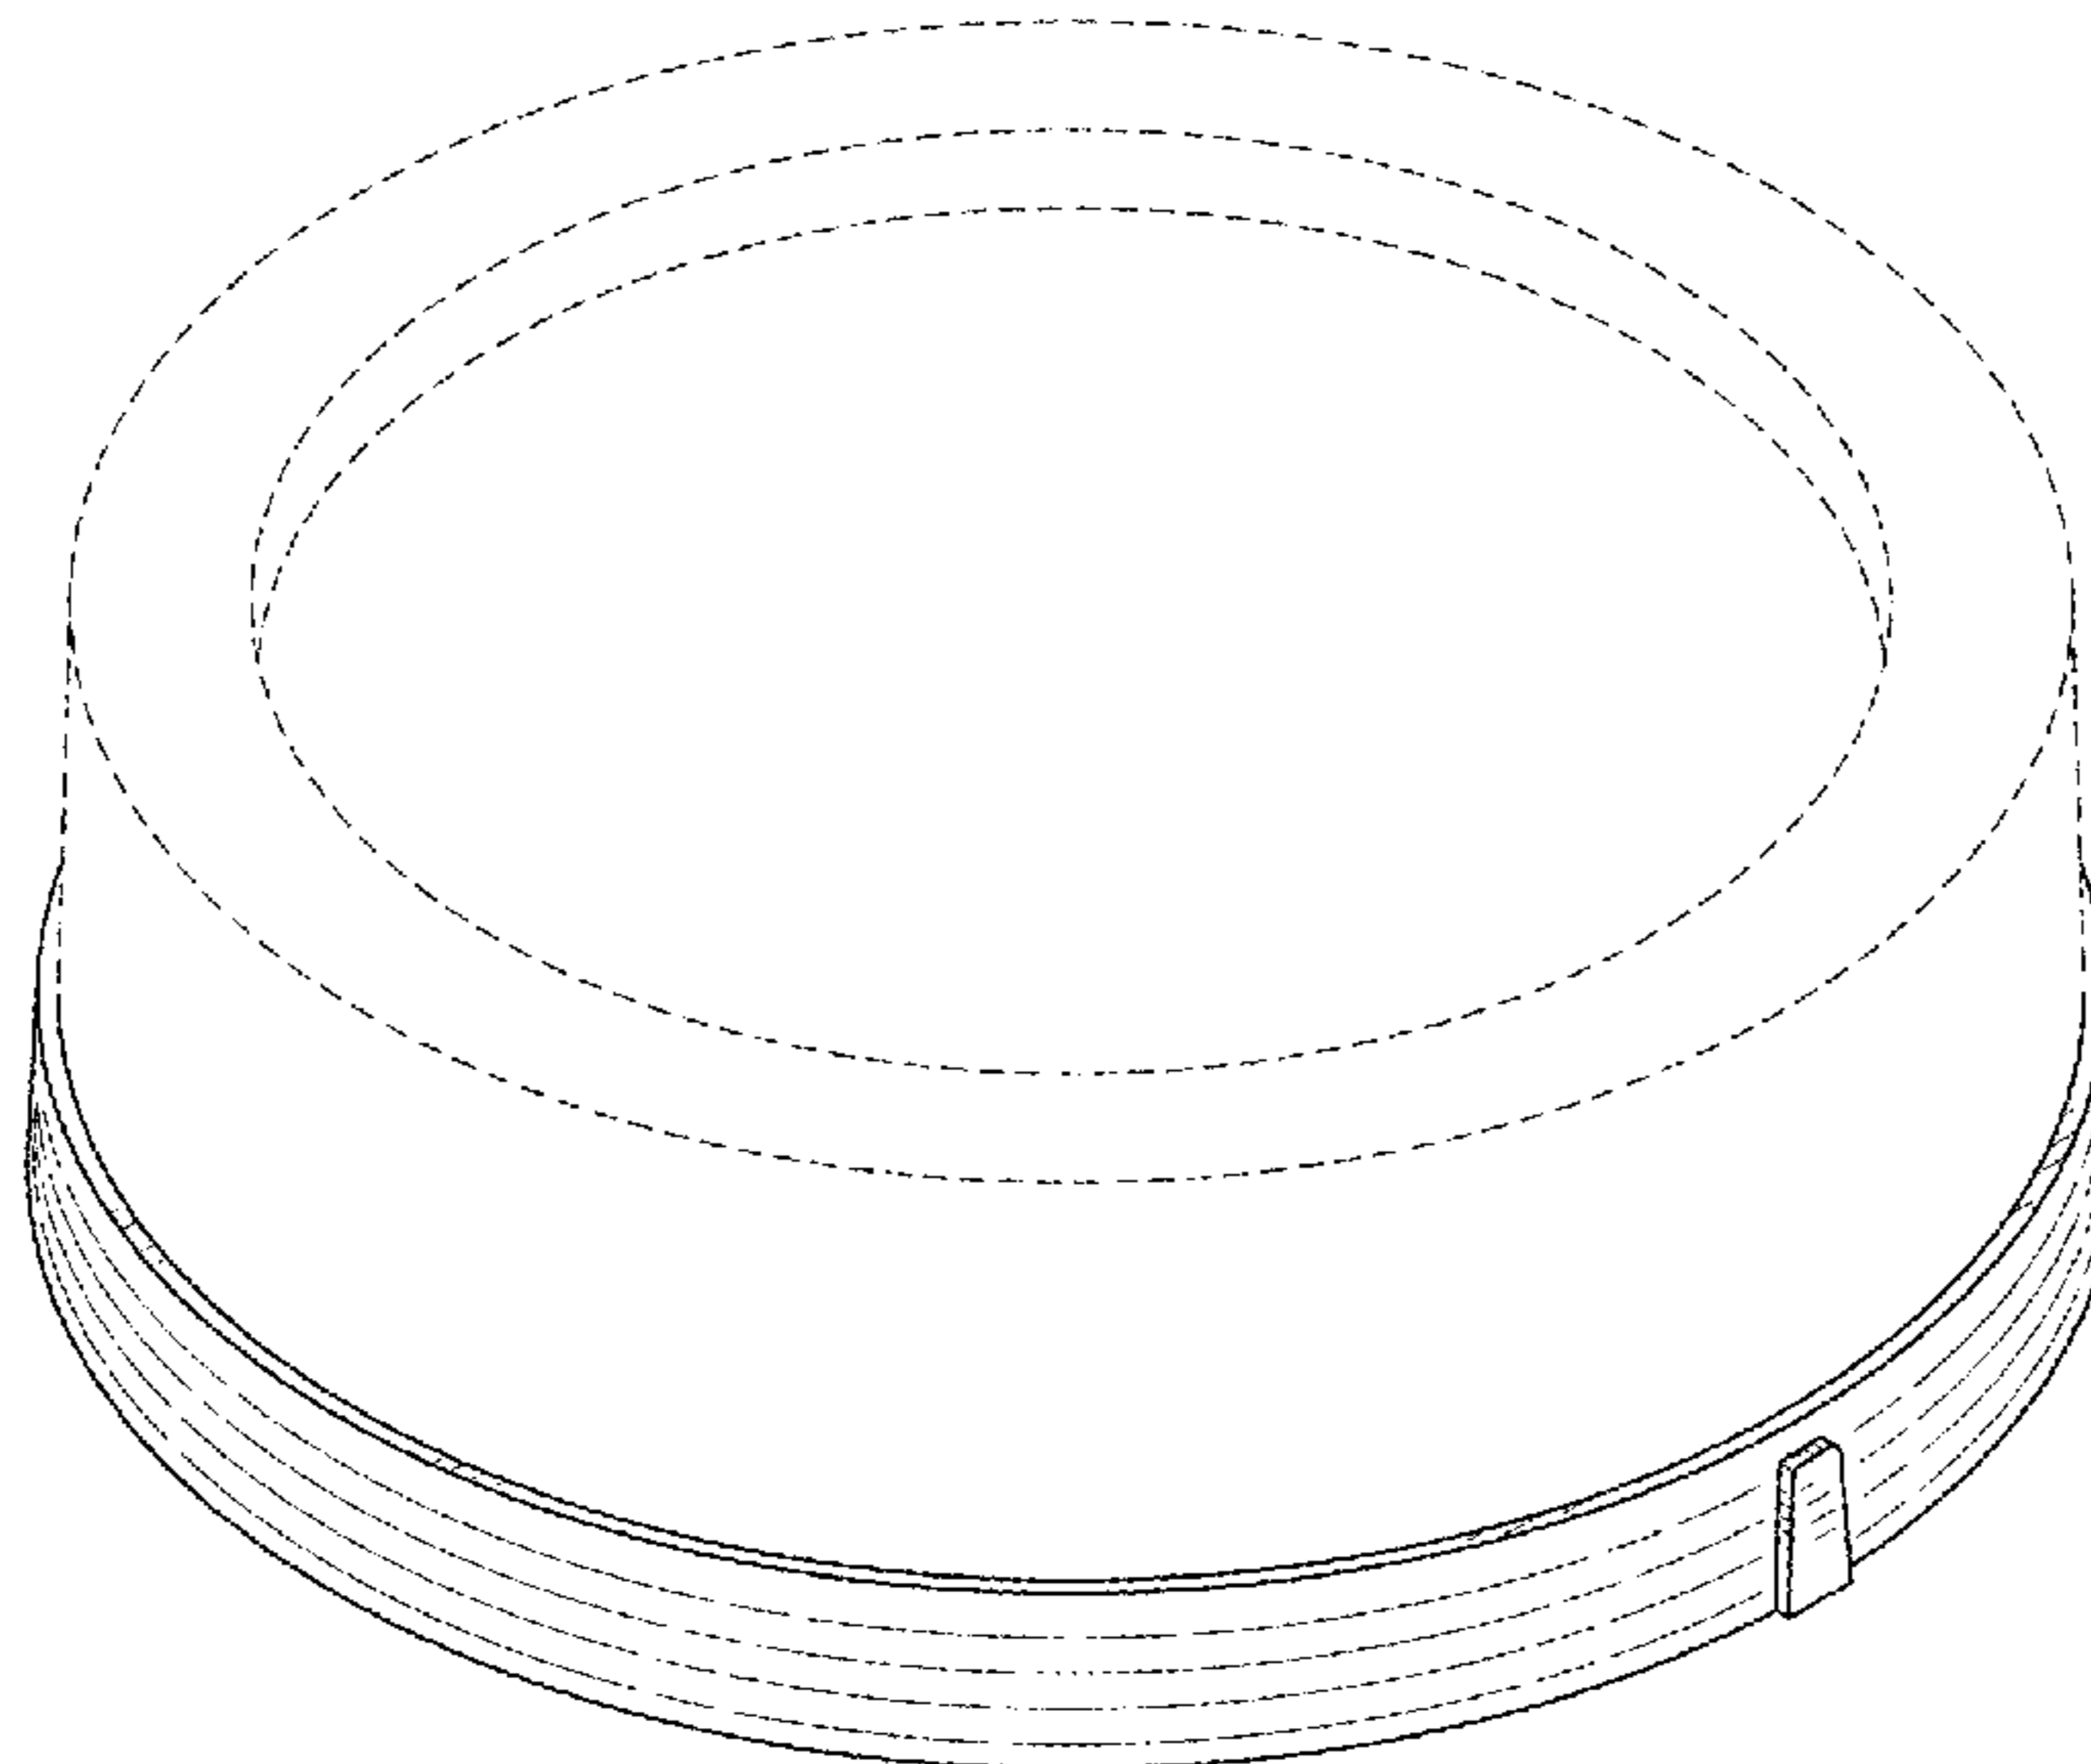

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0210252 A1 9/2007 Miyamoto
2018/0043365 A1 2/2018 Ruby

* cited by examiner

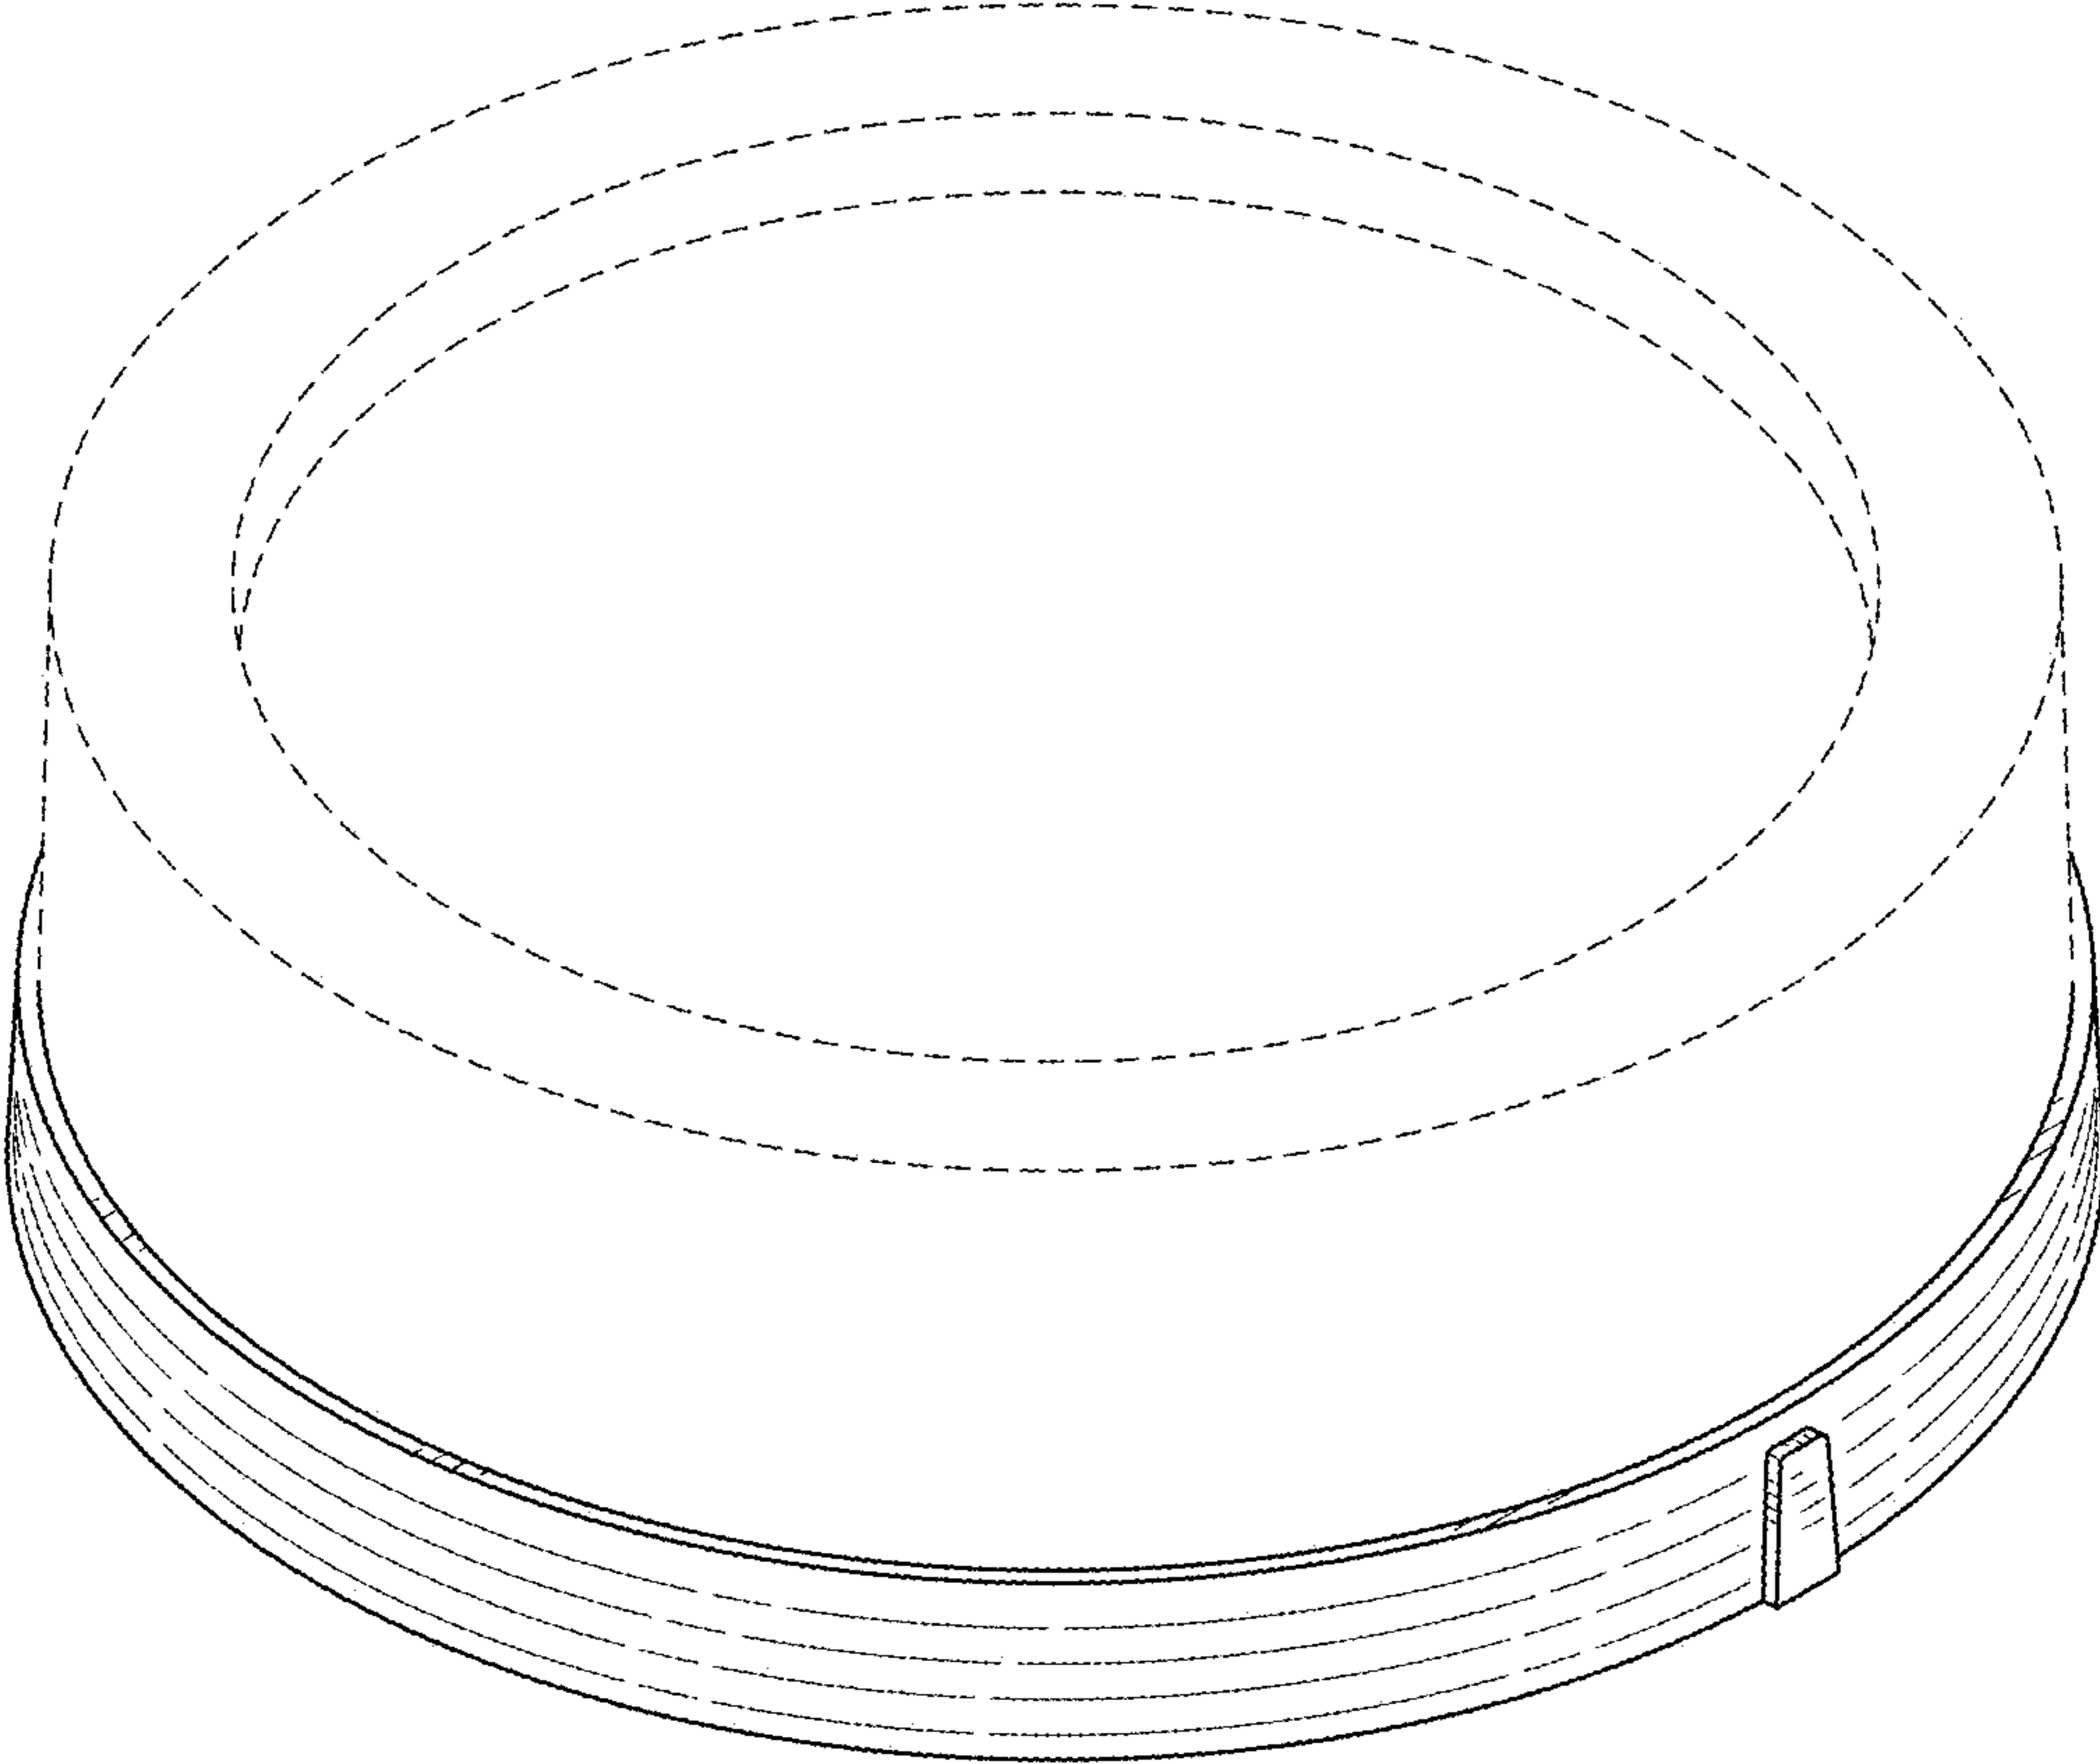


FIG.1

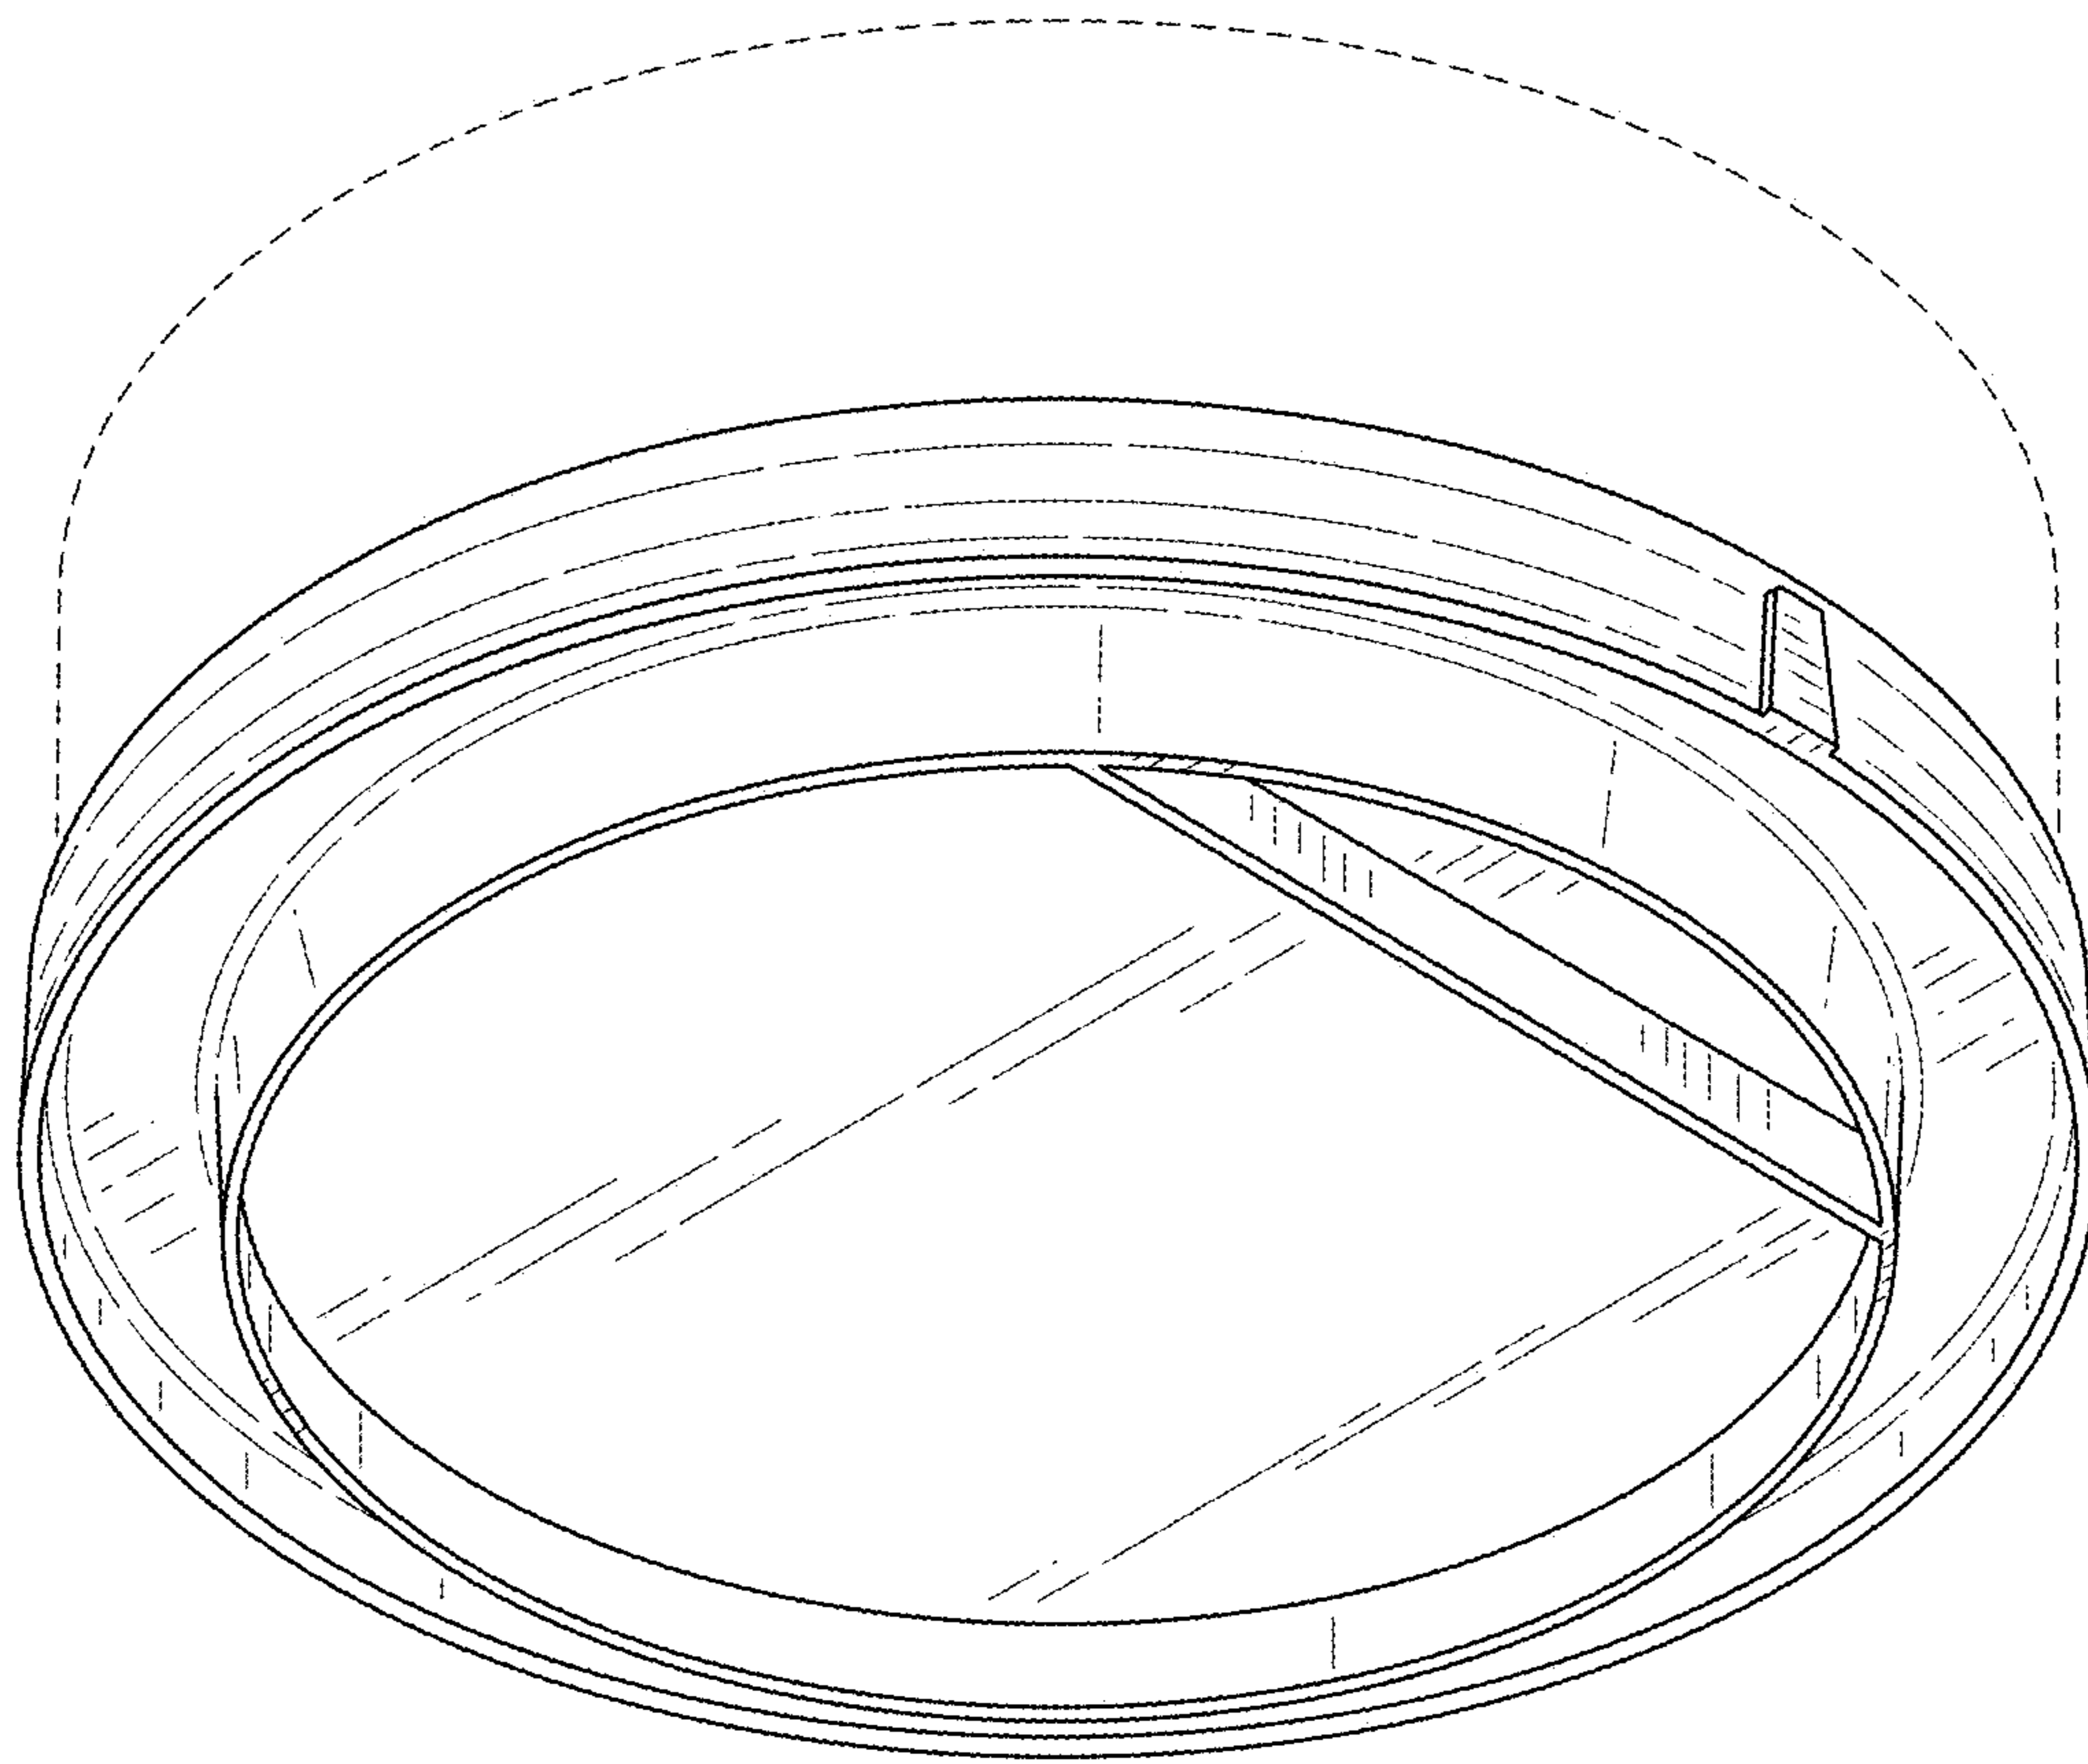


FIG.2

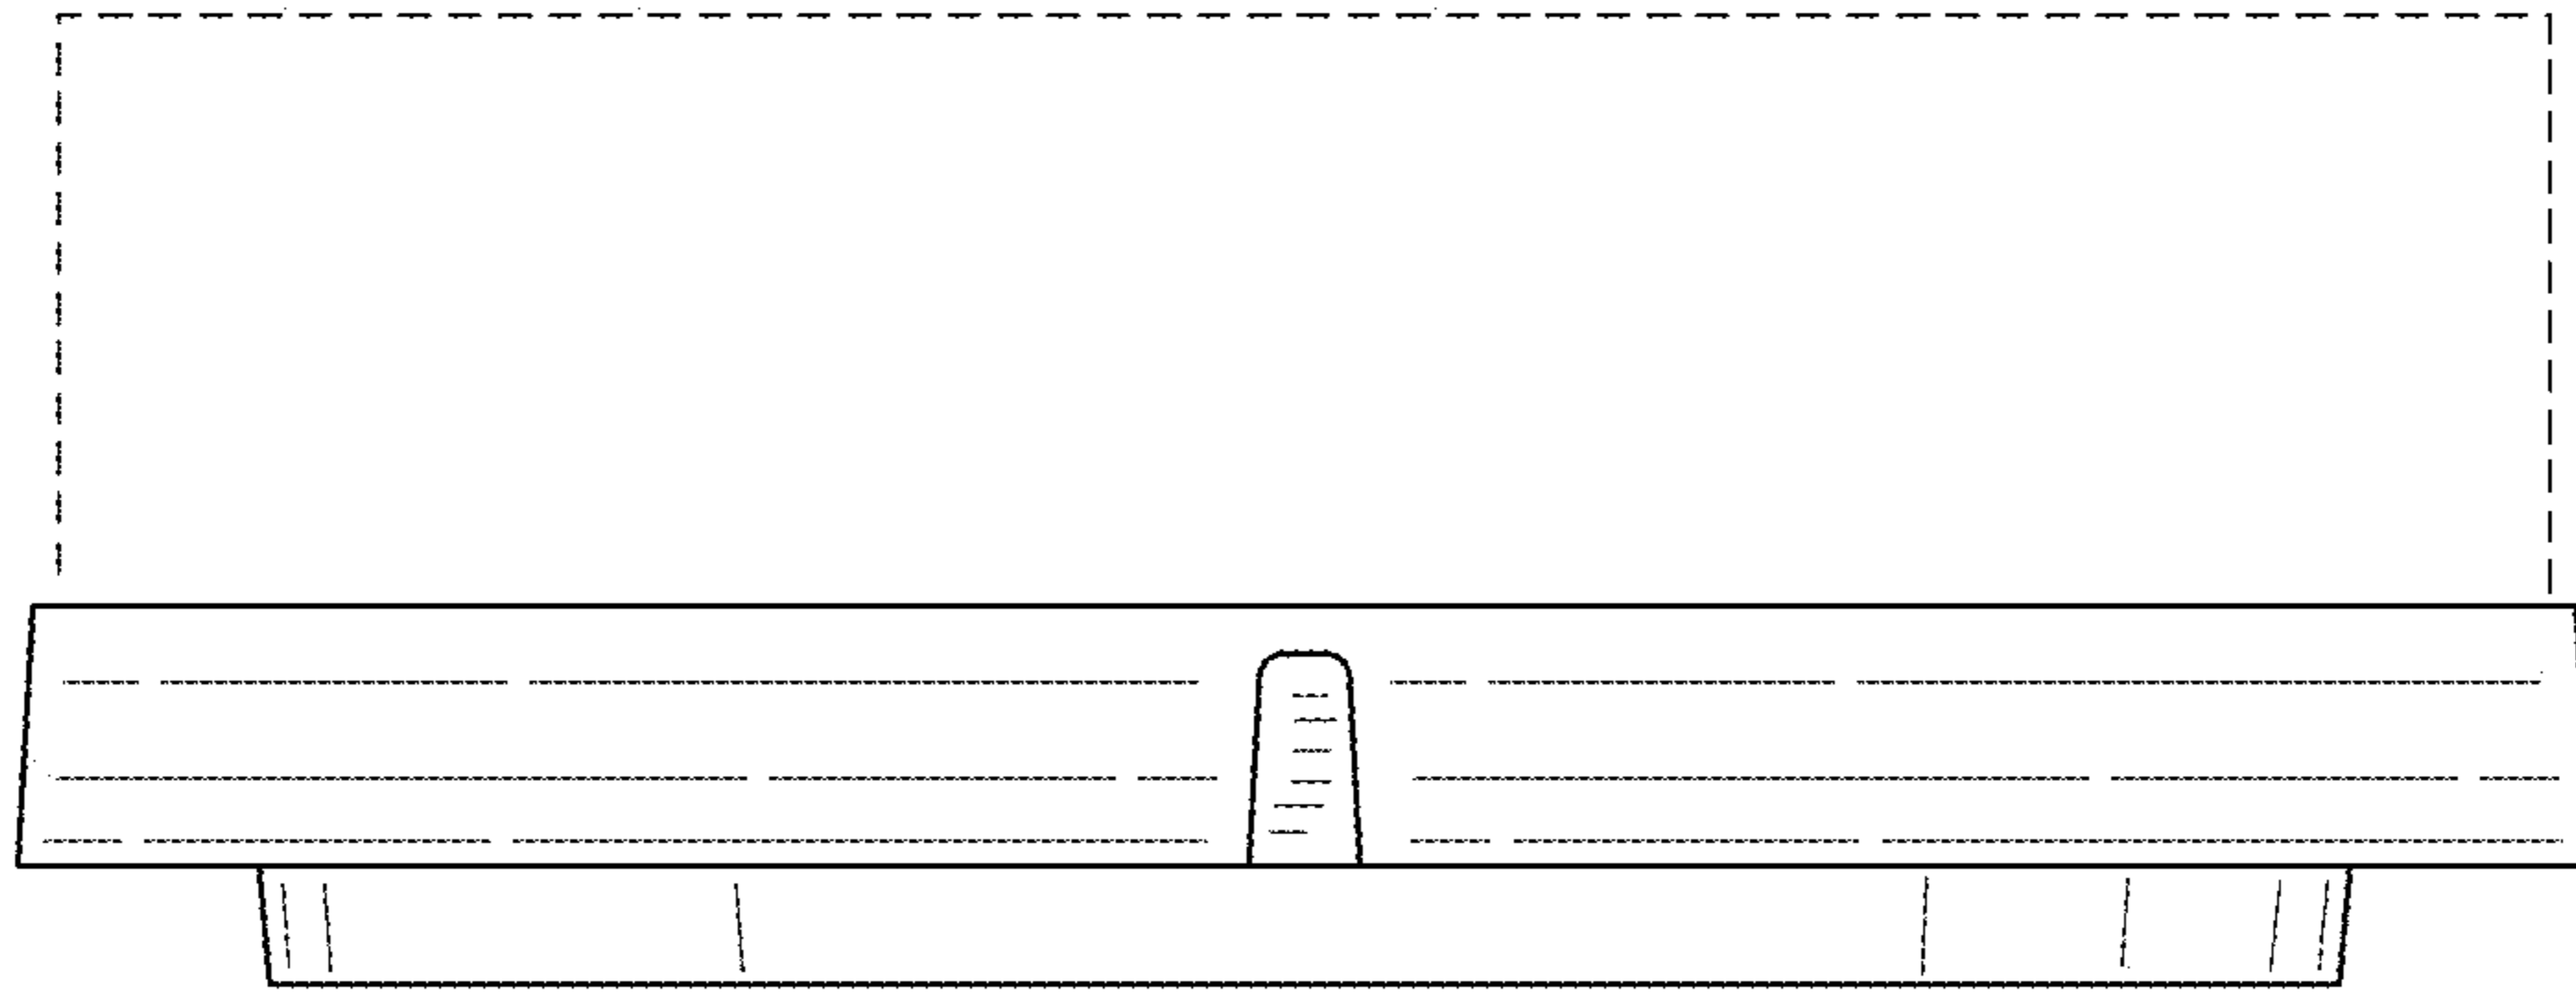


FIG.3

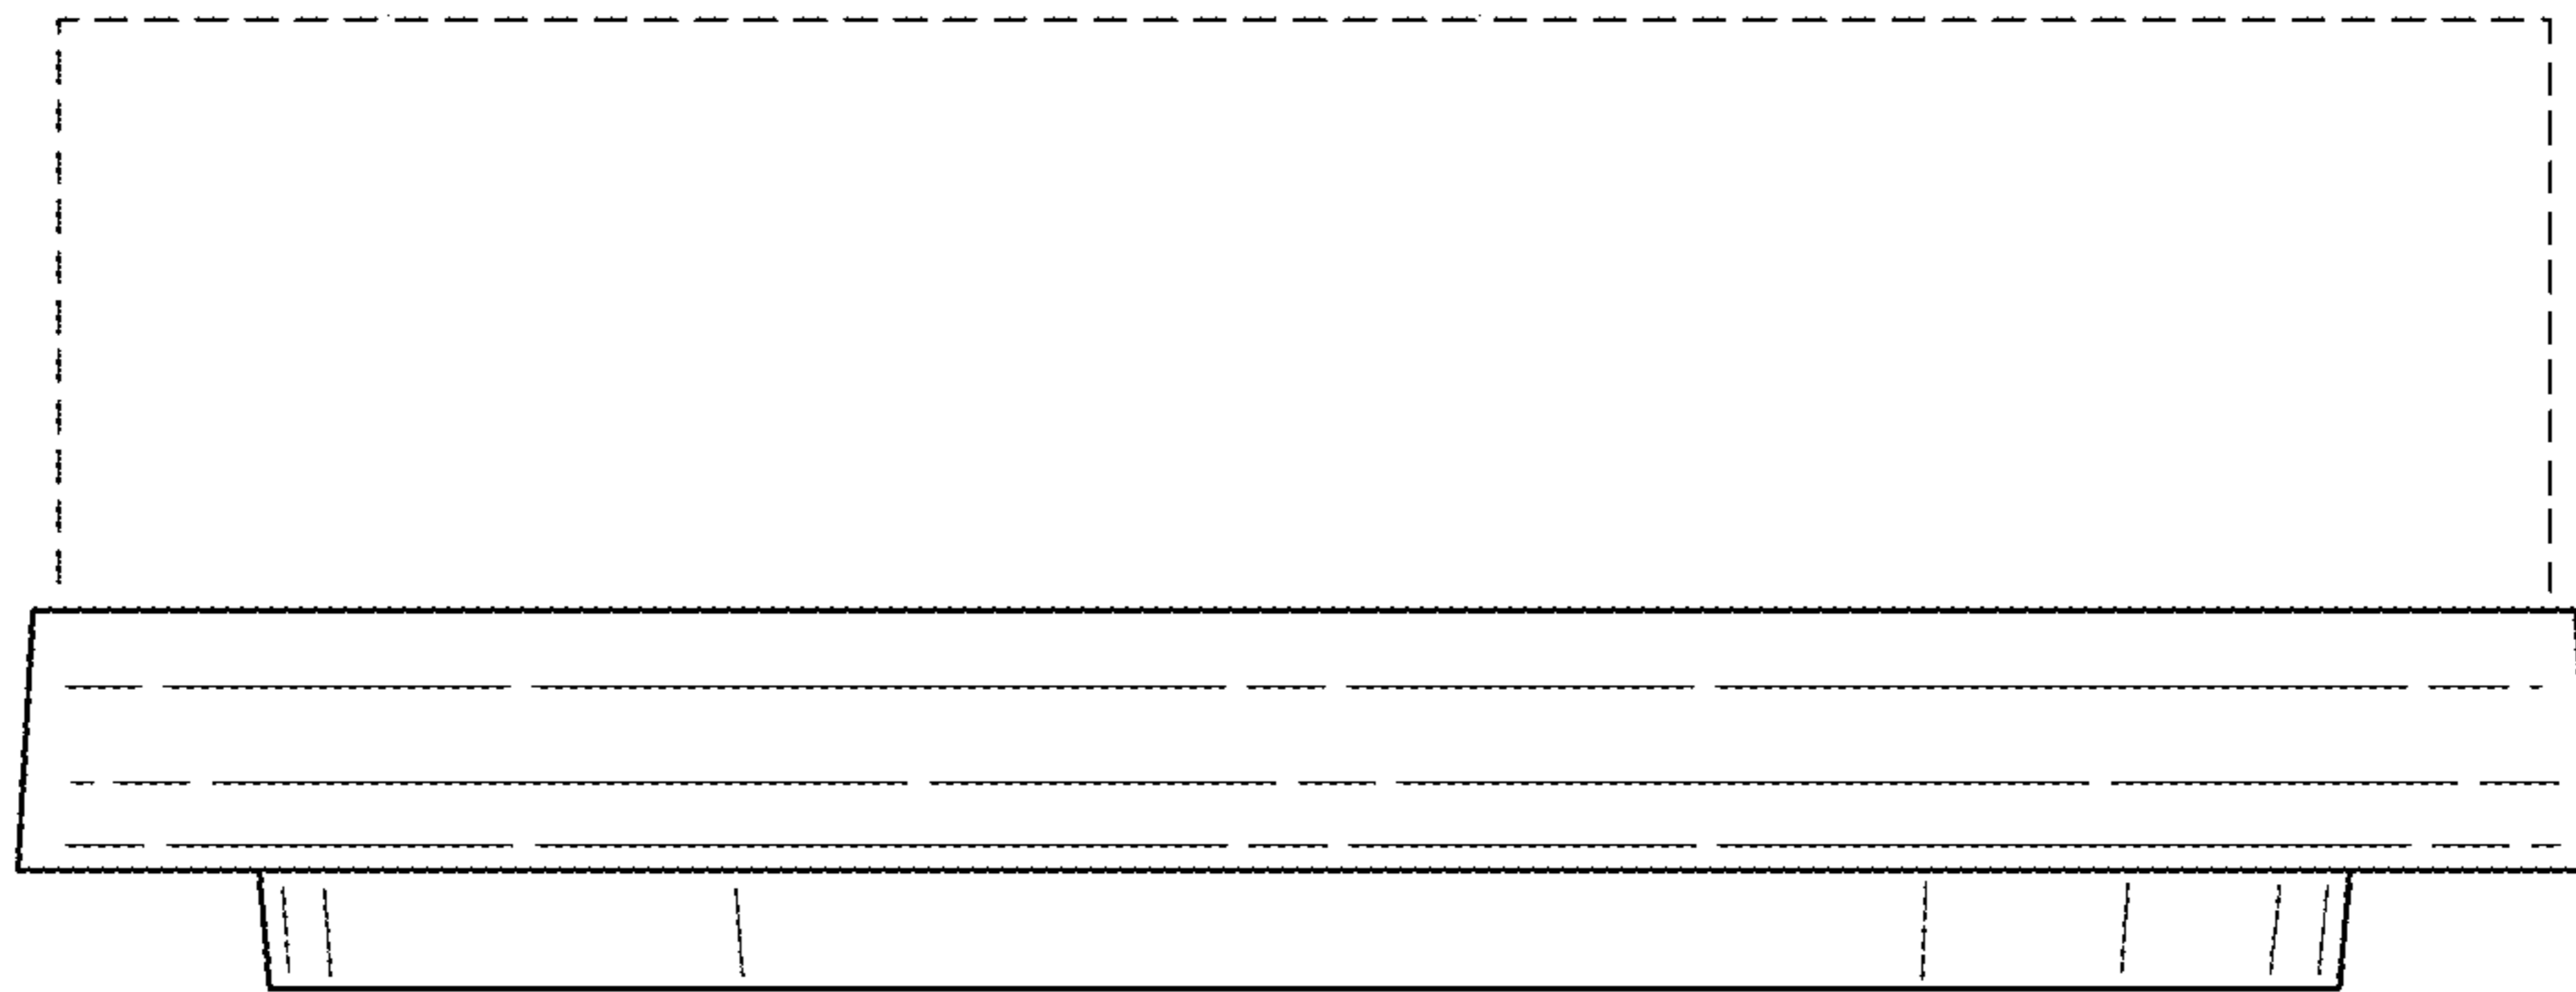


FIG.4

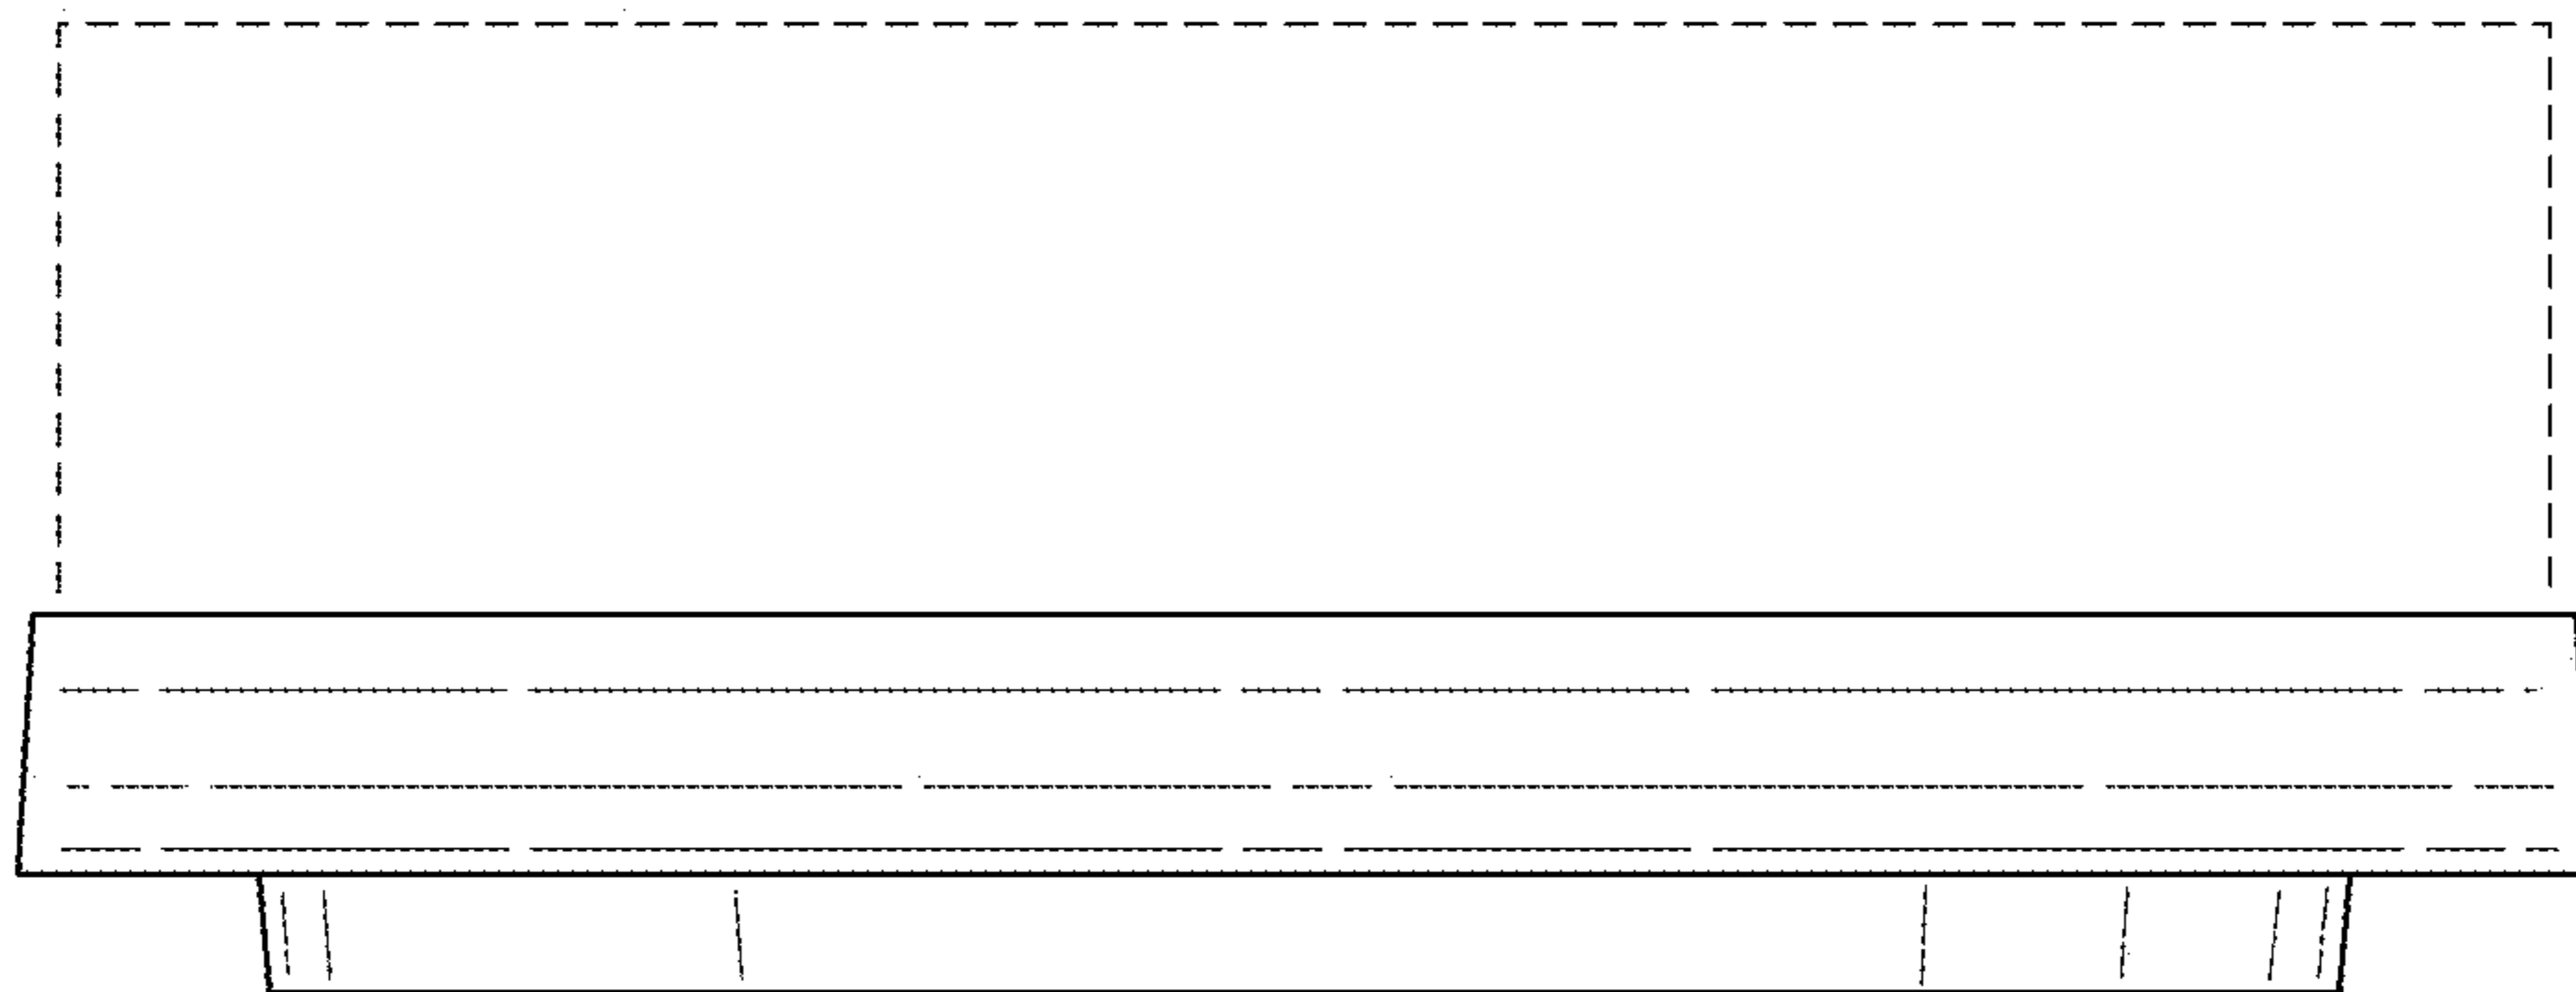


FIG.5

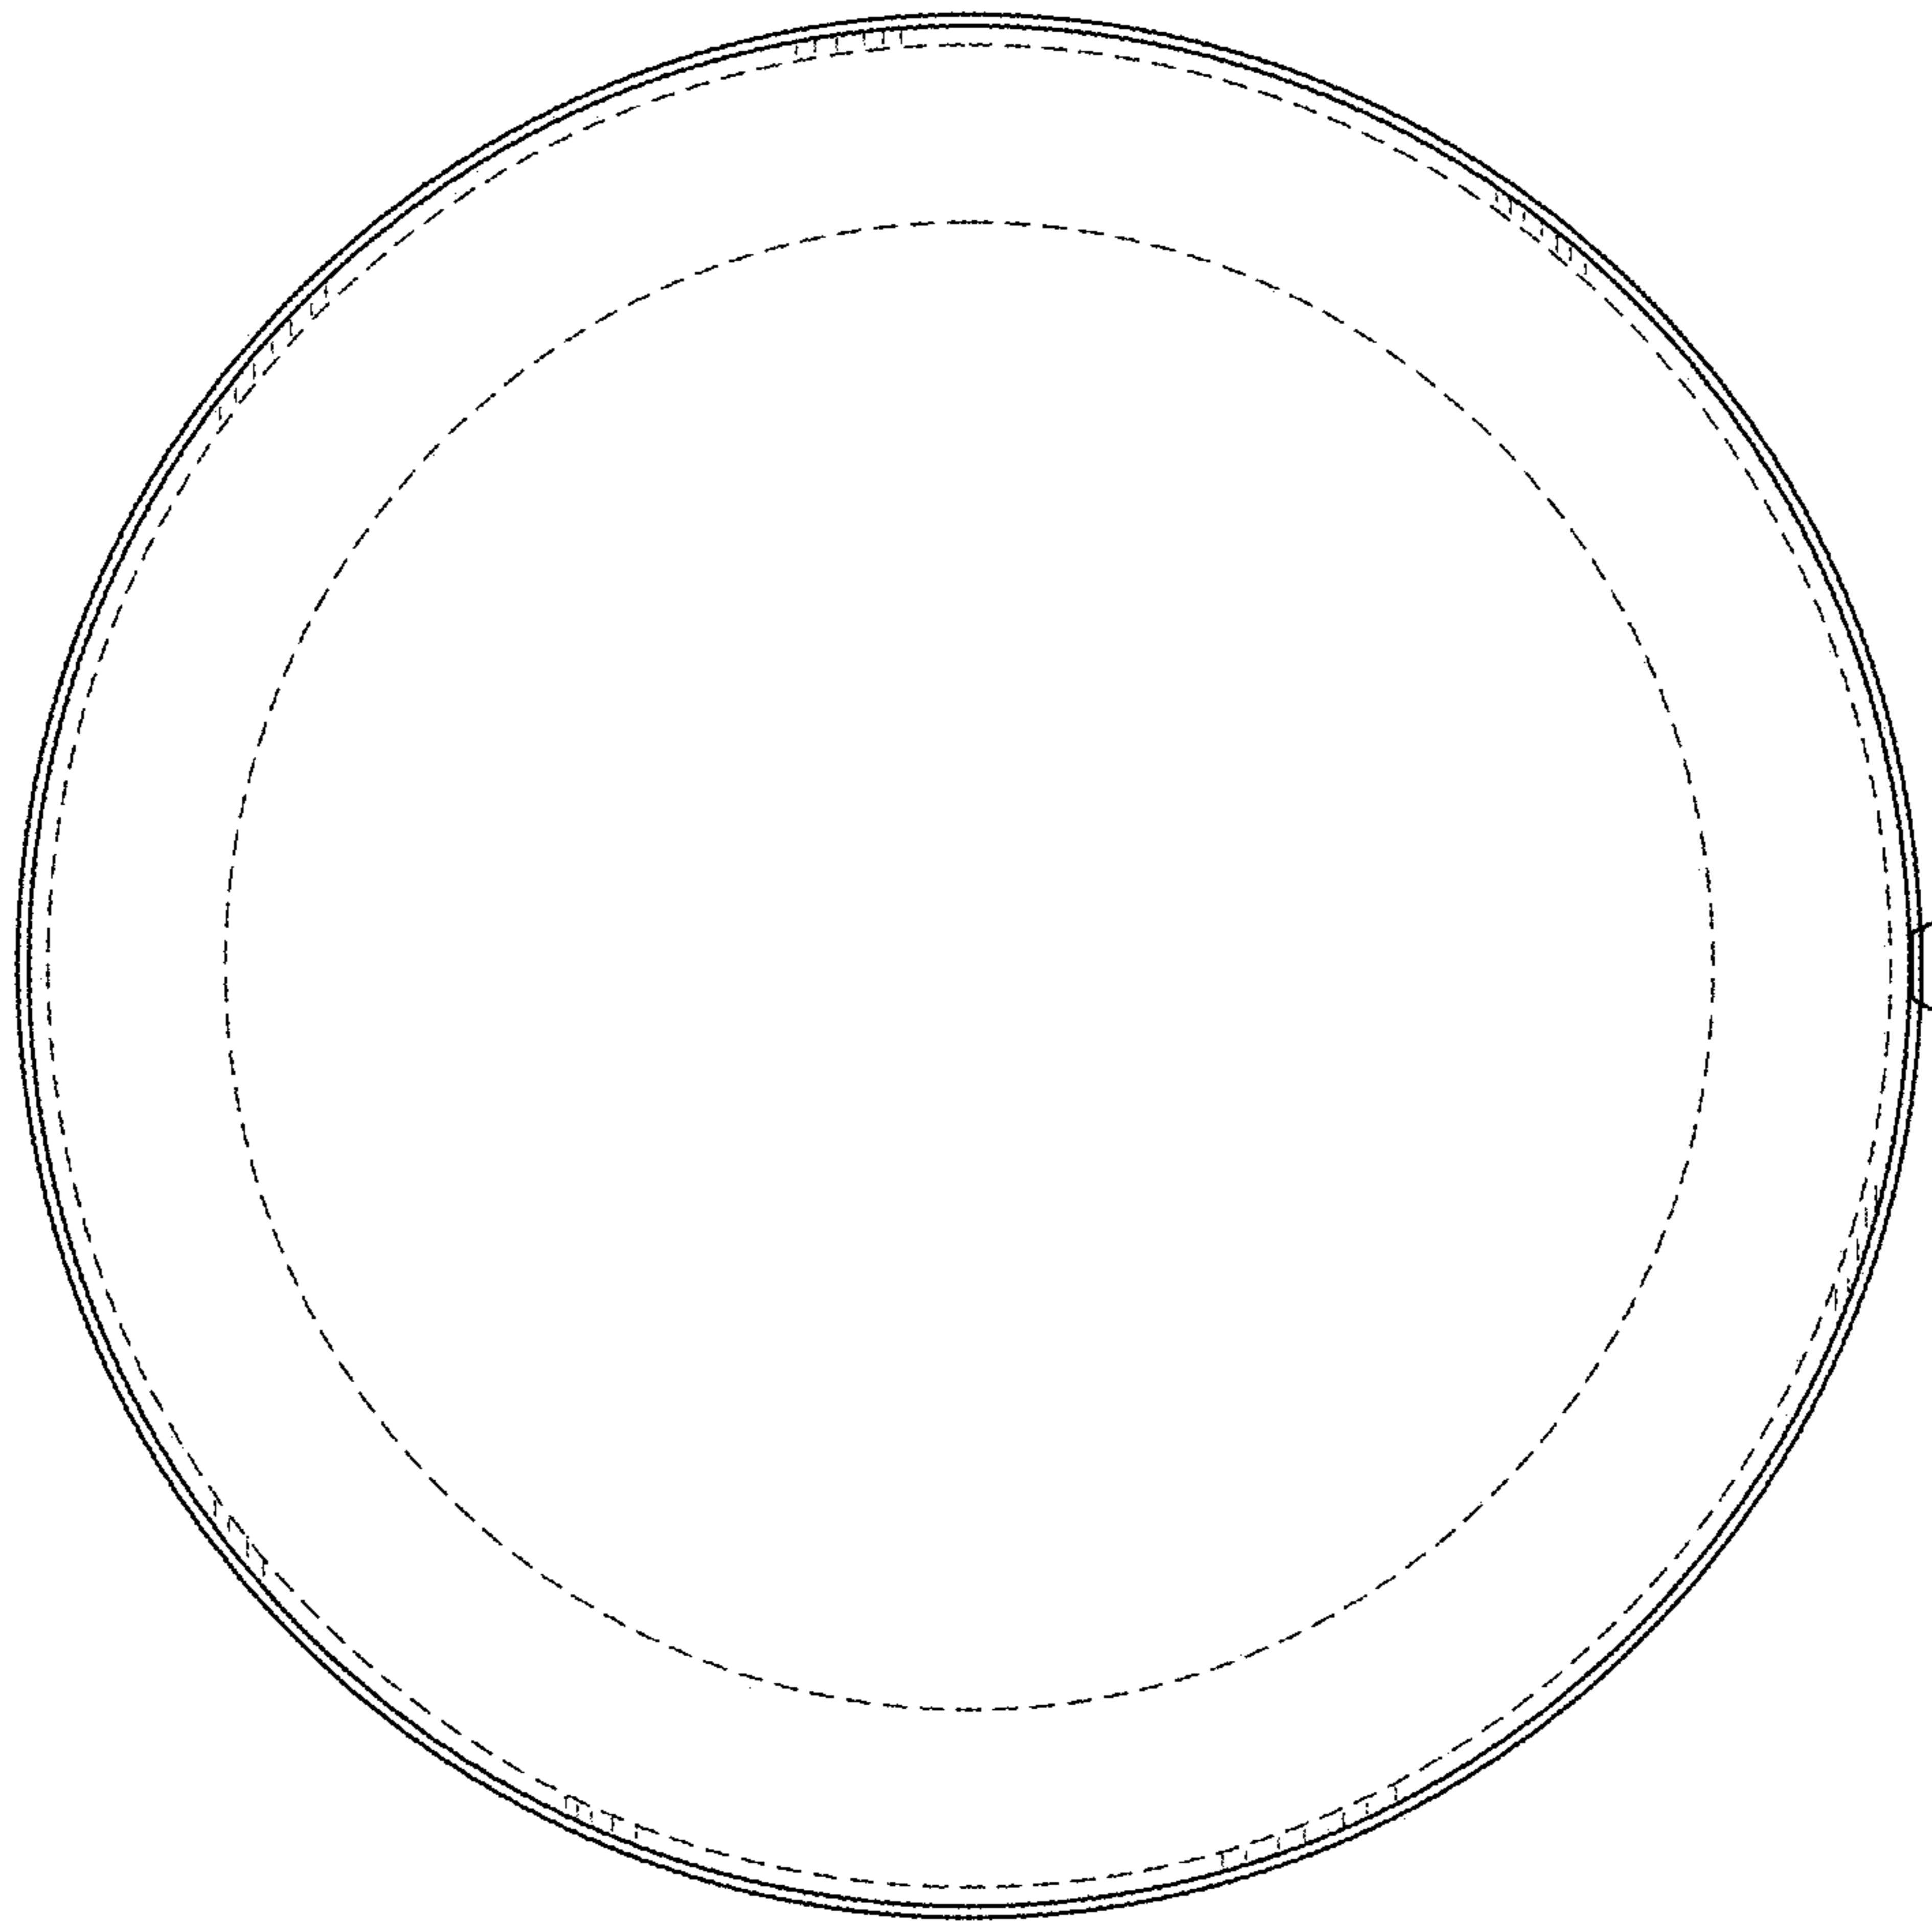


FIG.6

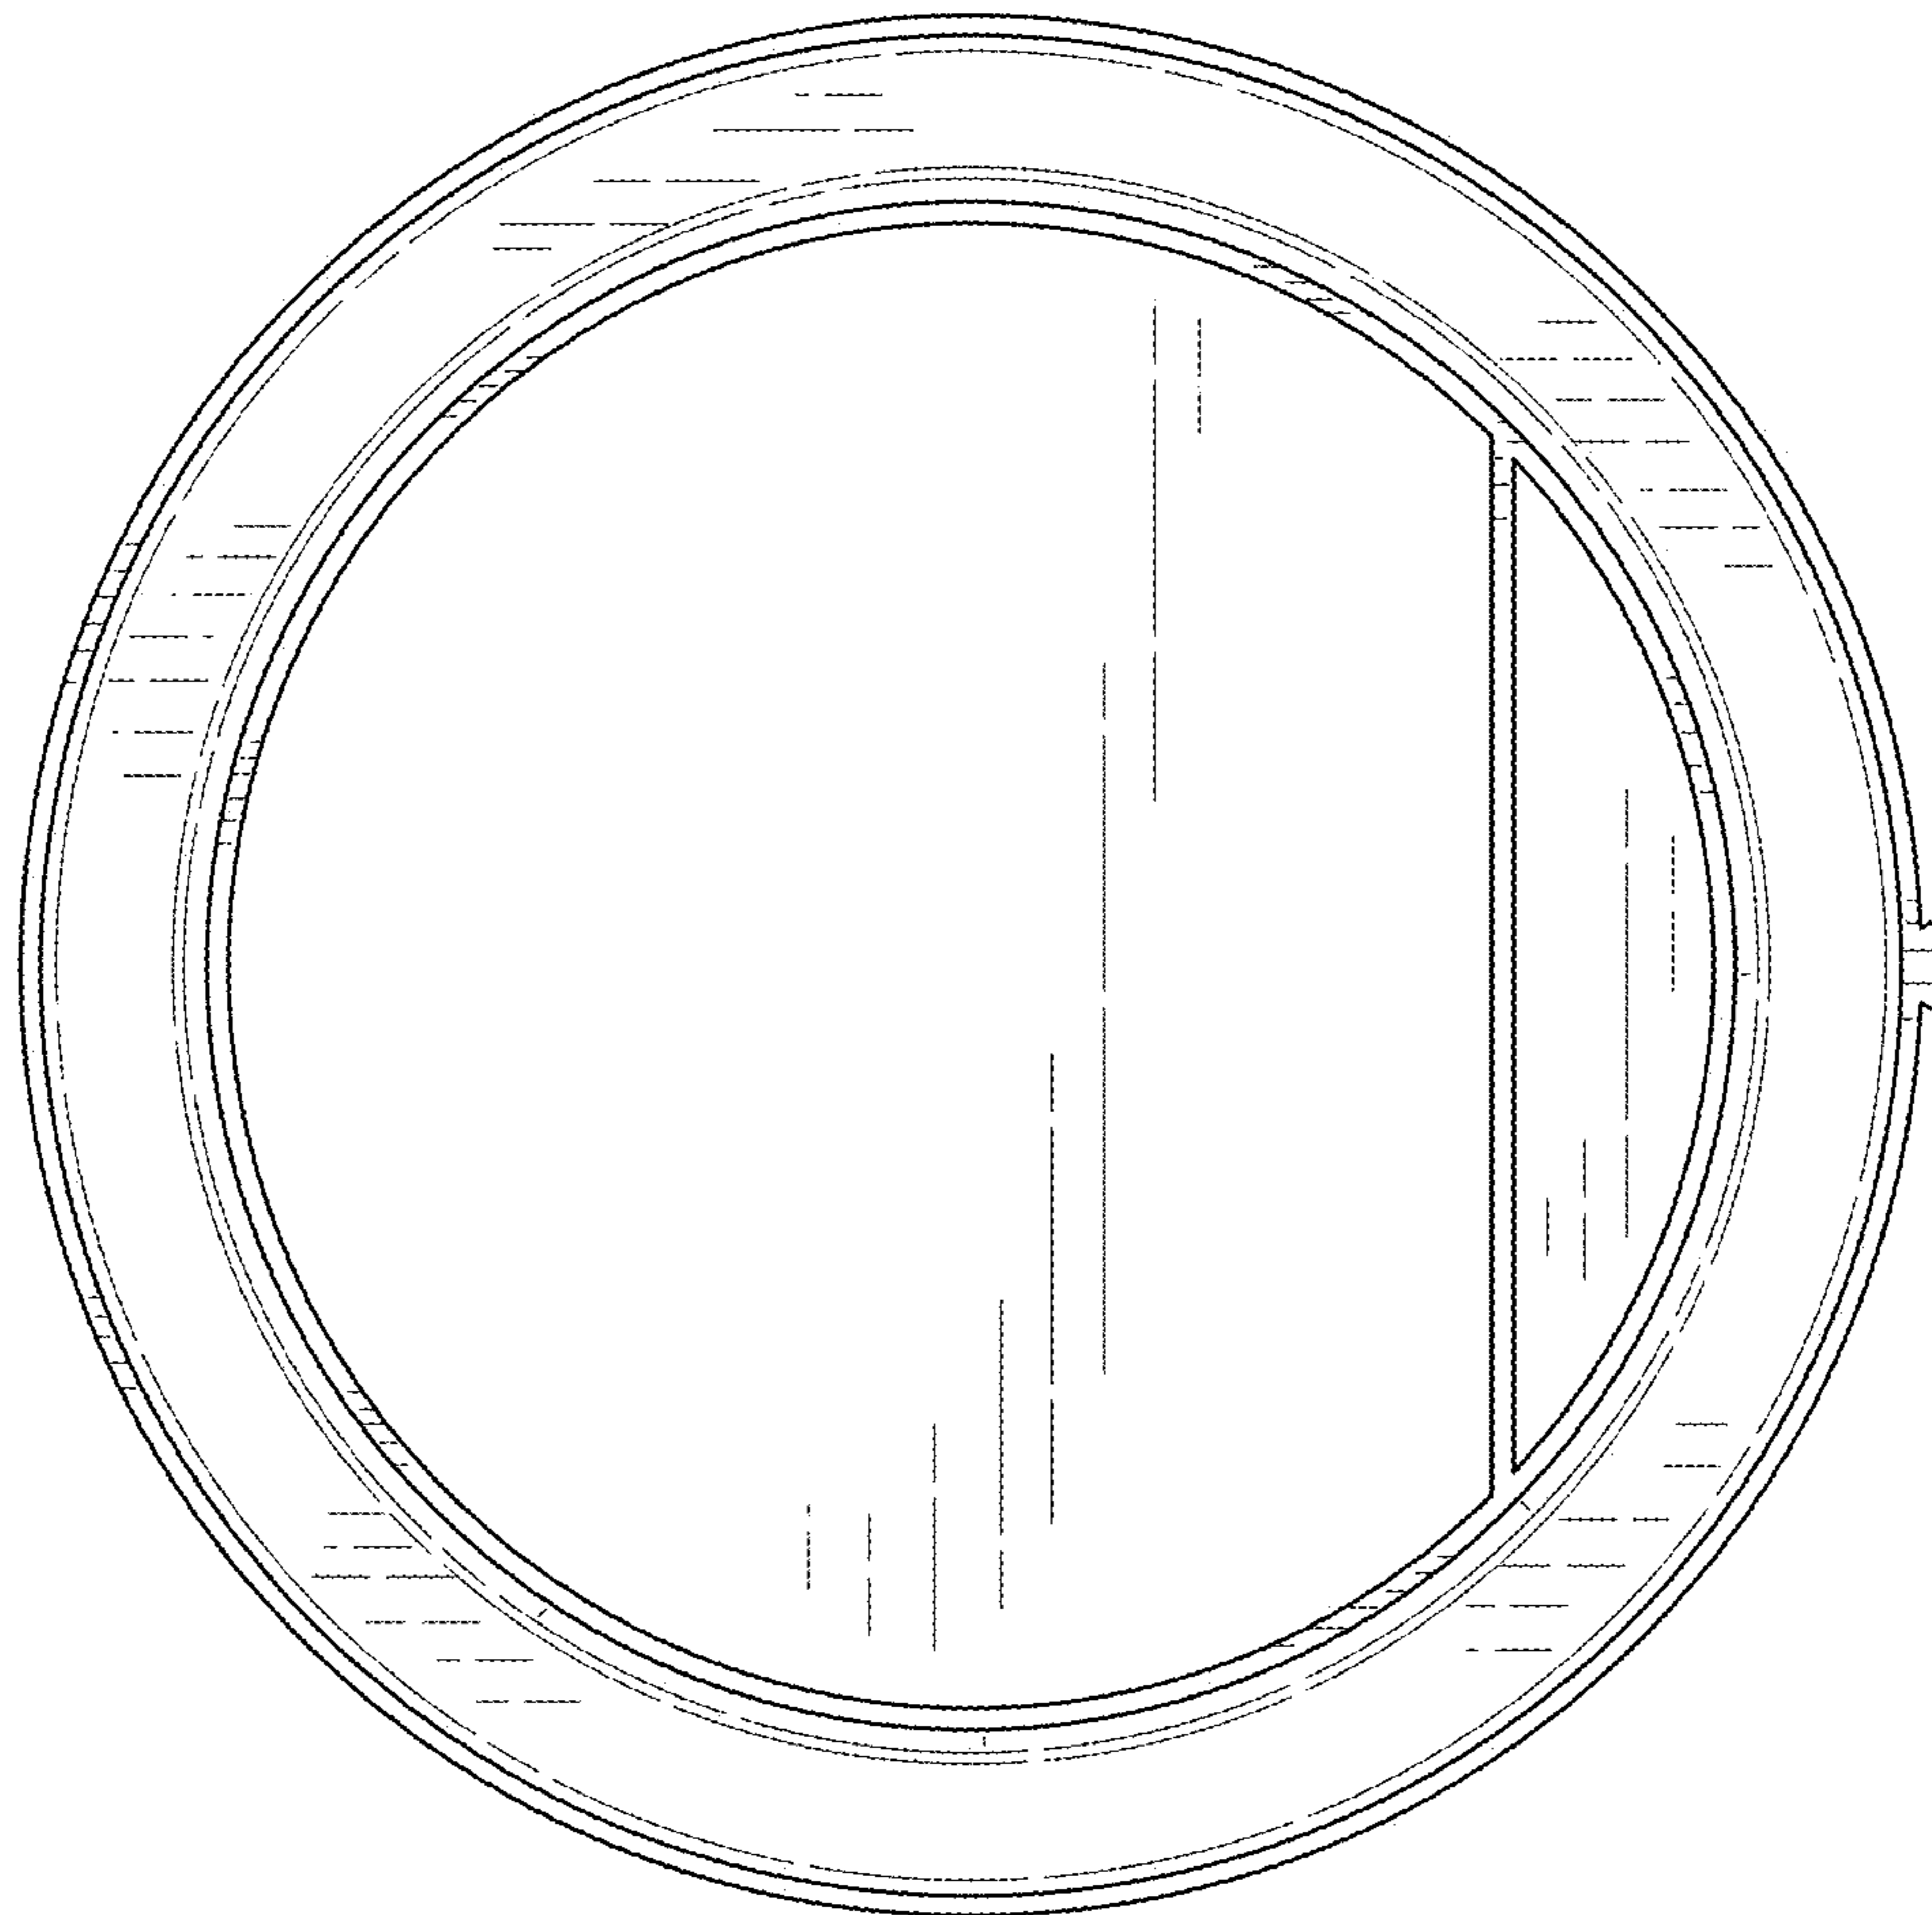


FIG.7