



US00D956983S

(12) **United States Design Patent** (10) **Patent No.:** **US D956,983 S**
Cordle (45) **Date of Patent:** **** Jul. 5, 2022**

(54) **DOCKING STATION OF A RECHARGER FOR AN INTERNAL NEURAL STIMULATOR**

(71) Applicant: **Medtronic, Inc.**, Minneapolis, MN (US)

(72) Inventor: **Glen T. Cordle**, Coon Rapids, MN (US)

(73) Assignee: **Medtronic, Inc.**, Minneapolis, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/812,490**

(22) Filed: **Oct. 21, 2021**

Related U.S. Application Data

(62) Division of application No. 29/710,468, filed on Oct. 23, 2019, now Pat. No. Des. 937,426.

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/133, 167, 168, 170, 177, 186, 187,
D24/209, 210, 231, 232; D14/251, 253,
D14/432, 434; D13/107-110, 118-119,
D13/184

CPC A61N 1/36125; Y02E 60/12; Y02T 90/14;
Y02T 90/122; Y02T 90/128; Y02T
90/163; Y02T 10/7005; Y02T 10/705;
Y02T 10/7088; H02J 7/0003; H02J
7/0034; H02J 7/0054; H02J 7/1423;
H01R 13/6675; H01M 2/1022; H01M
2/1055; H01M 10/425; B60L 11/1809;
B60L 11/1861; B60R 16/03

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D733,888 S 7/2015 Tuhkanen
D755,974 S 5/2016 Chen et al.
D757,275 S 5/2016 Lee

(Continued)

FOREIGN PATENT DOCUMENTS

CN 3374976 6/2004
CN 202130213589.4 * 8/2021
IN 292624 4/2017

OTHER PUBLICATIONS

Precision™ Charger Patient Instructional Video. Online, published date Oct. 1, 2015. Retrieved on Feb. 17, 2022 from URL: <https://www.youtube.com/watch?v=G3xg0eefLIM>.*

(Continued)

Primary Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Patterson Thuent Pedersen, P.A.

(57) **CLAIM**

I claim the ornamental design for a docking station of a recharger for an internal neural stimulator, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a docking station of a recharger for an internal neural stimulator according to my design.

FIG. 2 is a top plan view thereof.

FIG. 3 is a bottom plan view of thereof.

FIG. 4 is a right side elevation view thereof.

FIG. 5 is a left side elevation view thereof.


FIG. 6 is an end elevation view thereof.

FIG. 7 is another end elevation view thereof; and,

FIG. 8 is a bottom perspective view thereof.

In the drawings, the broken lines depict portions of the docking station of a recharger for an internal neural stimulator that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

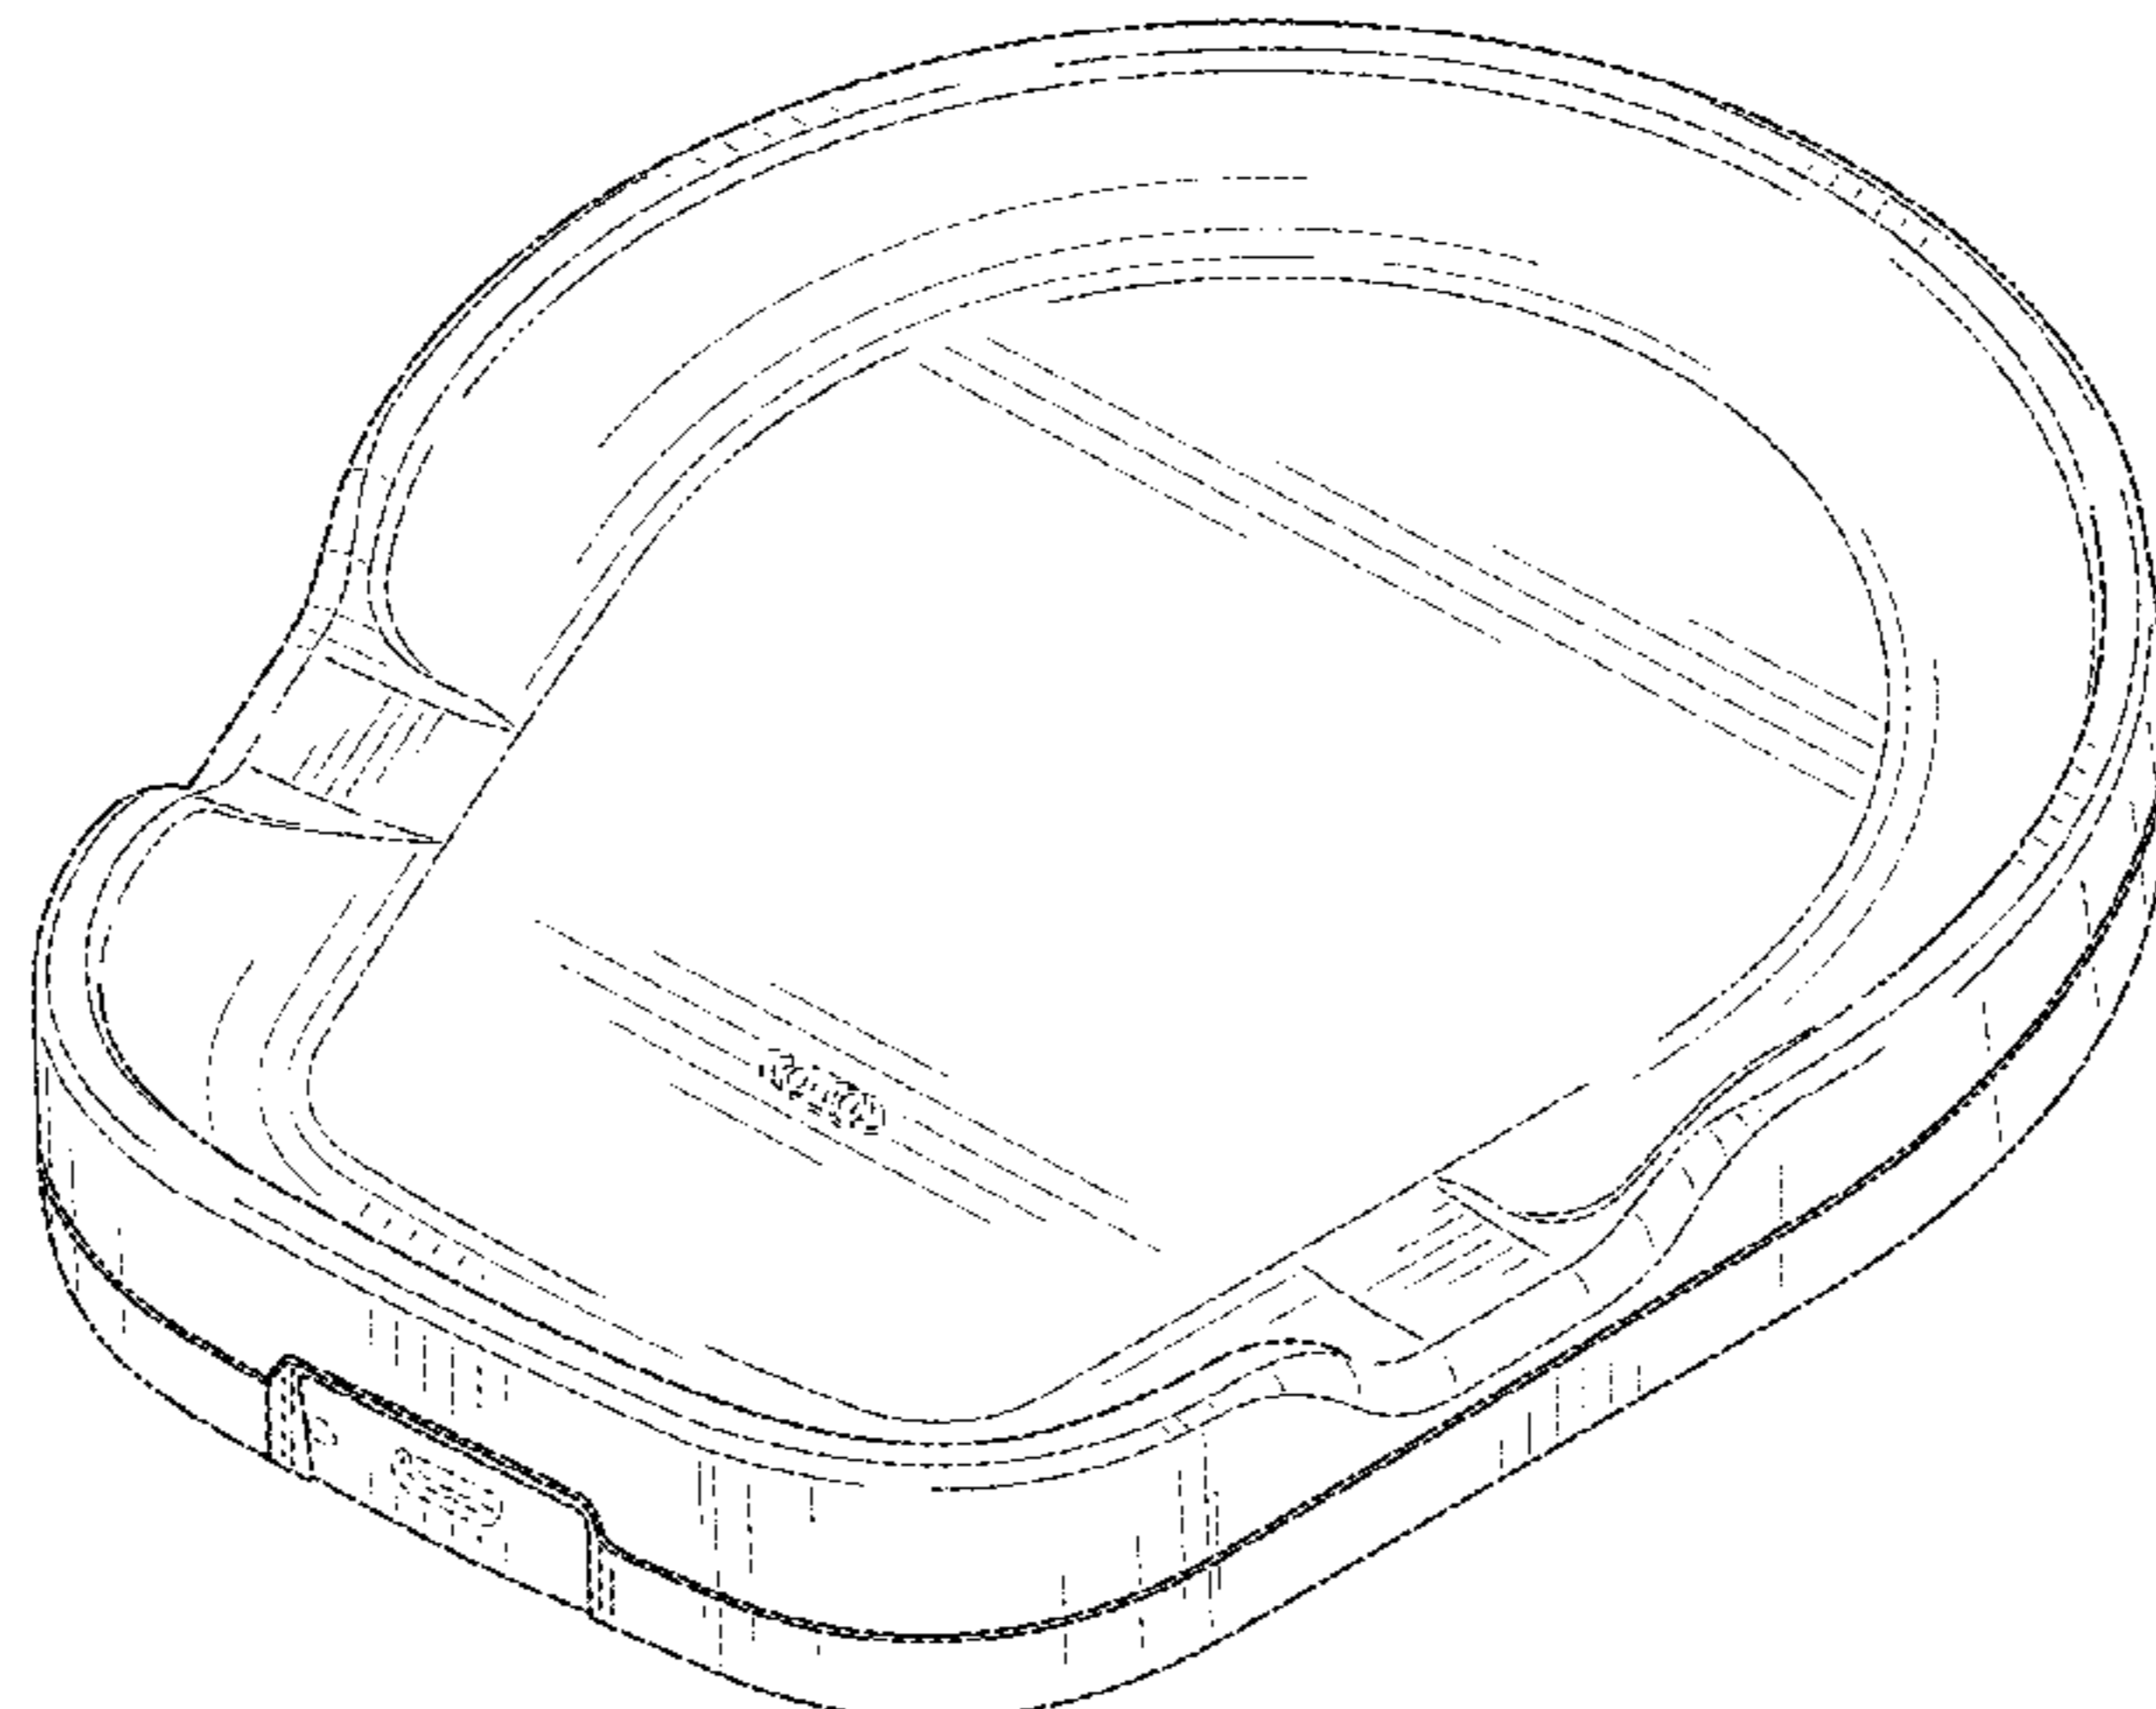

(56)

References Cited

U.S. PATENT DOCUMENTS

D777,331 S 1/2017 Jayalath et al.
 D782,926 S 4/2017 Hojo et al.
 D783,170 S 4/2017 Carreon et al.
 D794,805 S 8/2017 Kranz et al.
 D794,806 S 8/2017 Kranz et al.
 D800,653 S 10/2017 Smiedt et al.
 D810,680 S 2/2018 Carreon et al.
 D812,229 S 3/2018 Al-Siddiq
 D812,556 S * 3/2018 Xu D13/103
 D821,593 S 6/2018 Perez et al.
 D861,599 S 10/2019 Choi et al.
 D881,120 S 4/2020 Ai
 D883,209 S 5/2020 Liao
 D883,921 S 5/2020 Ryu et al.
 D886,302 S 6/2020 Raghavan et al.
 D886,303 S 6/2020 Huang et al.
 D895,543 S 9/2020 Akana et al.
 D897,543 S * 9/2020 Jones D24/187
 D906,958 S 1/2021 Fitzgerald et al.
 D914,604 S 3/2021 Wang
 D918,137 S * 5/2021 Painter D13/108
 D924,221 S * 7/2021 Hong D14/216

D925,119 S * 7/2021 Kim D27/194
 D935,398 S * 11/2021 Wang D13/108
 D937,206 S * 11/2021 Romano D13/108
 D937,426 S 11/2021 Cordle
 D939,438 S * 12/2021 Hu D13/108
 D940,890 S * 1/2022 Cartledge D24/200
 D942,448 S * 2/2022 Hamre D24/186
 D943,437 S * 2/2022 Abellera D12/174
 D943,522 S * 2/2022 Feng D13/108
 D943,524 S * 2/2022 Zheng D13/108
 2013/0165993 A1 6/2013 Aghassian et al.
 2015/0188339 A1 * 7/2015 Green H02J 50/60
 320/108
 2016/0126771 A1 5/2016 Aghassian et al.

OTHER PUBLICATIONS

Recharging a Rechargeable SCS. Online, published date Sep. 7, 2018. Retrieved on Apr. 18, 2021 from URL: <https://www.spine-health.com/treatment/pain-management/recharging-rechargeable-scs>.
 Application and file history from U.S. Appl. No. 29/710,468, filed Oct. 23, 2019, inventor Cordle, now U.S. Pat. No. D. 937,426.

* cited by examiner

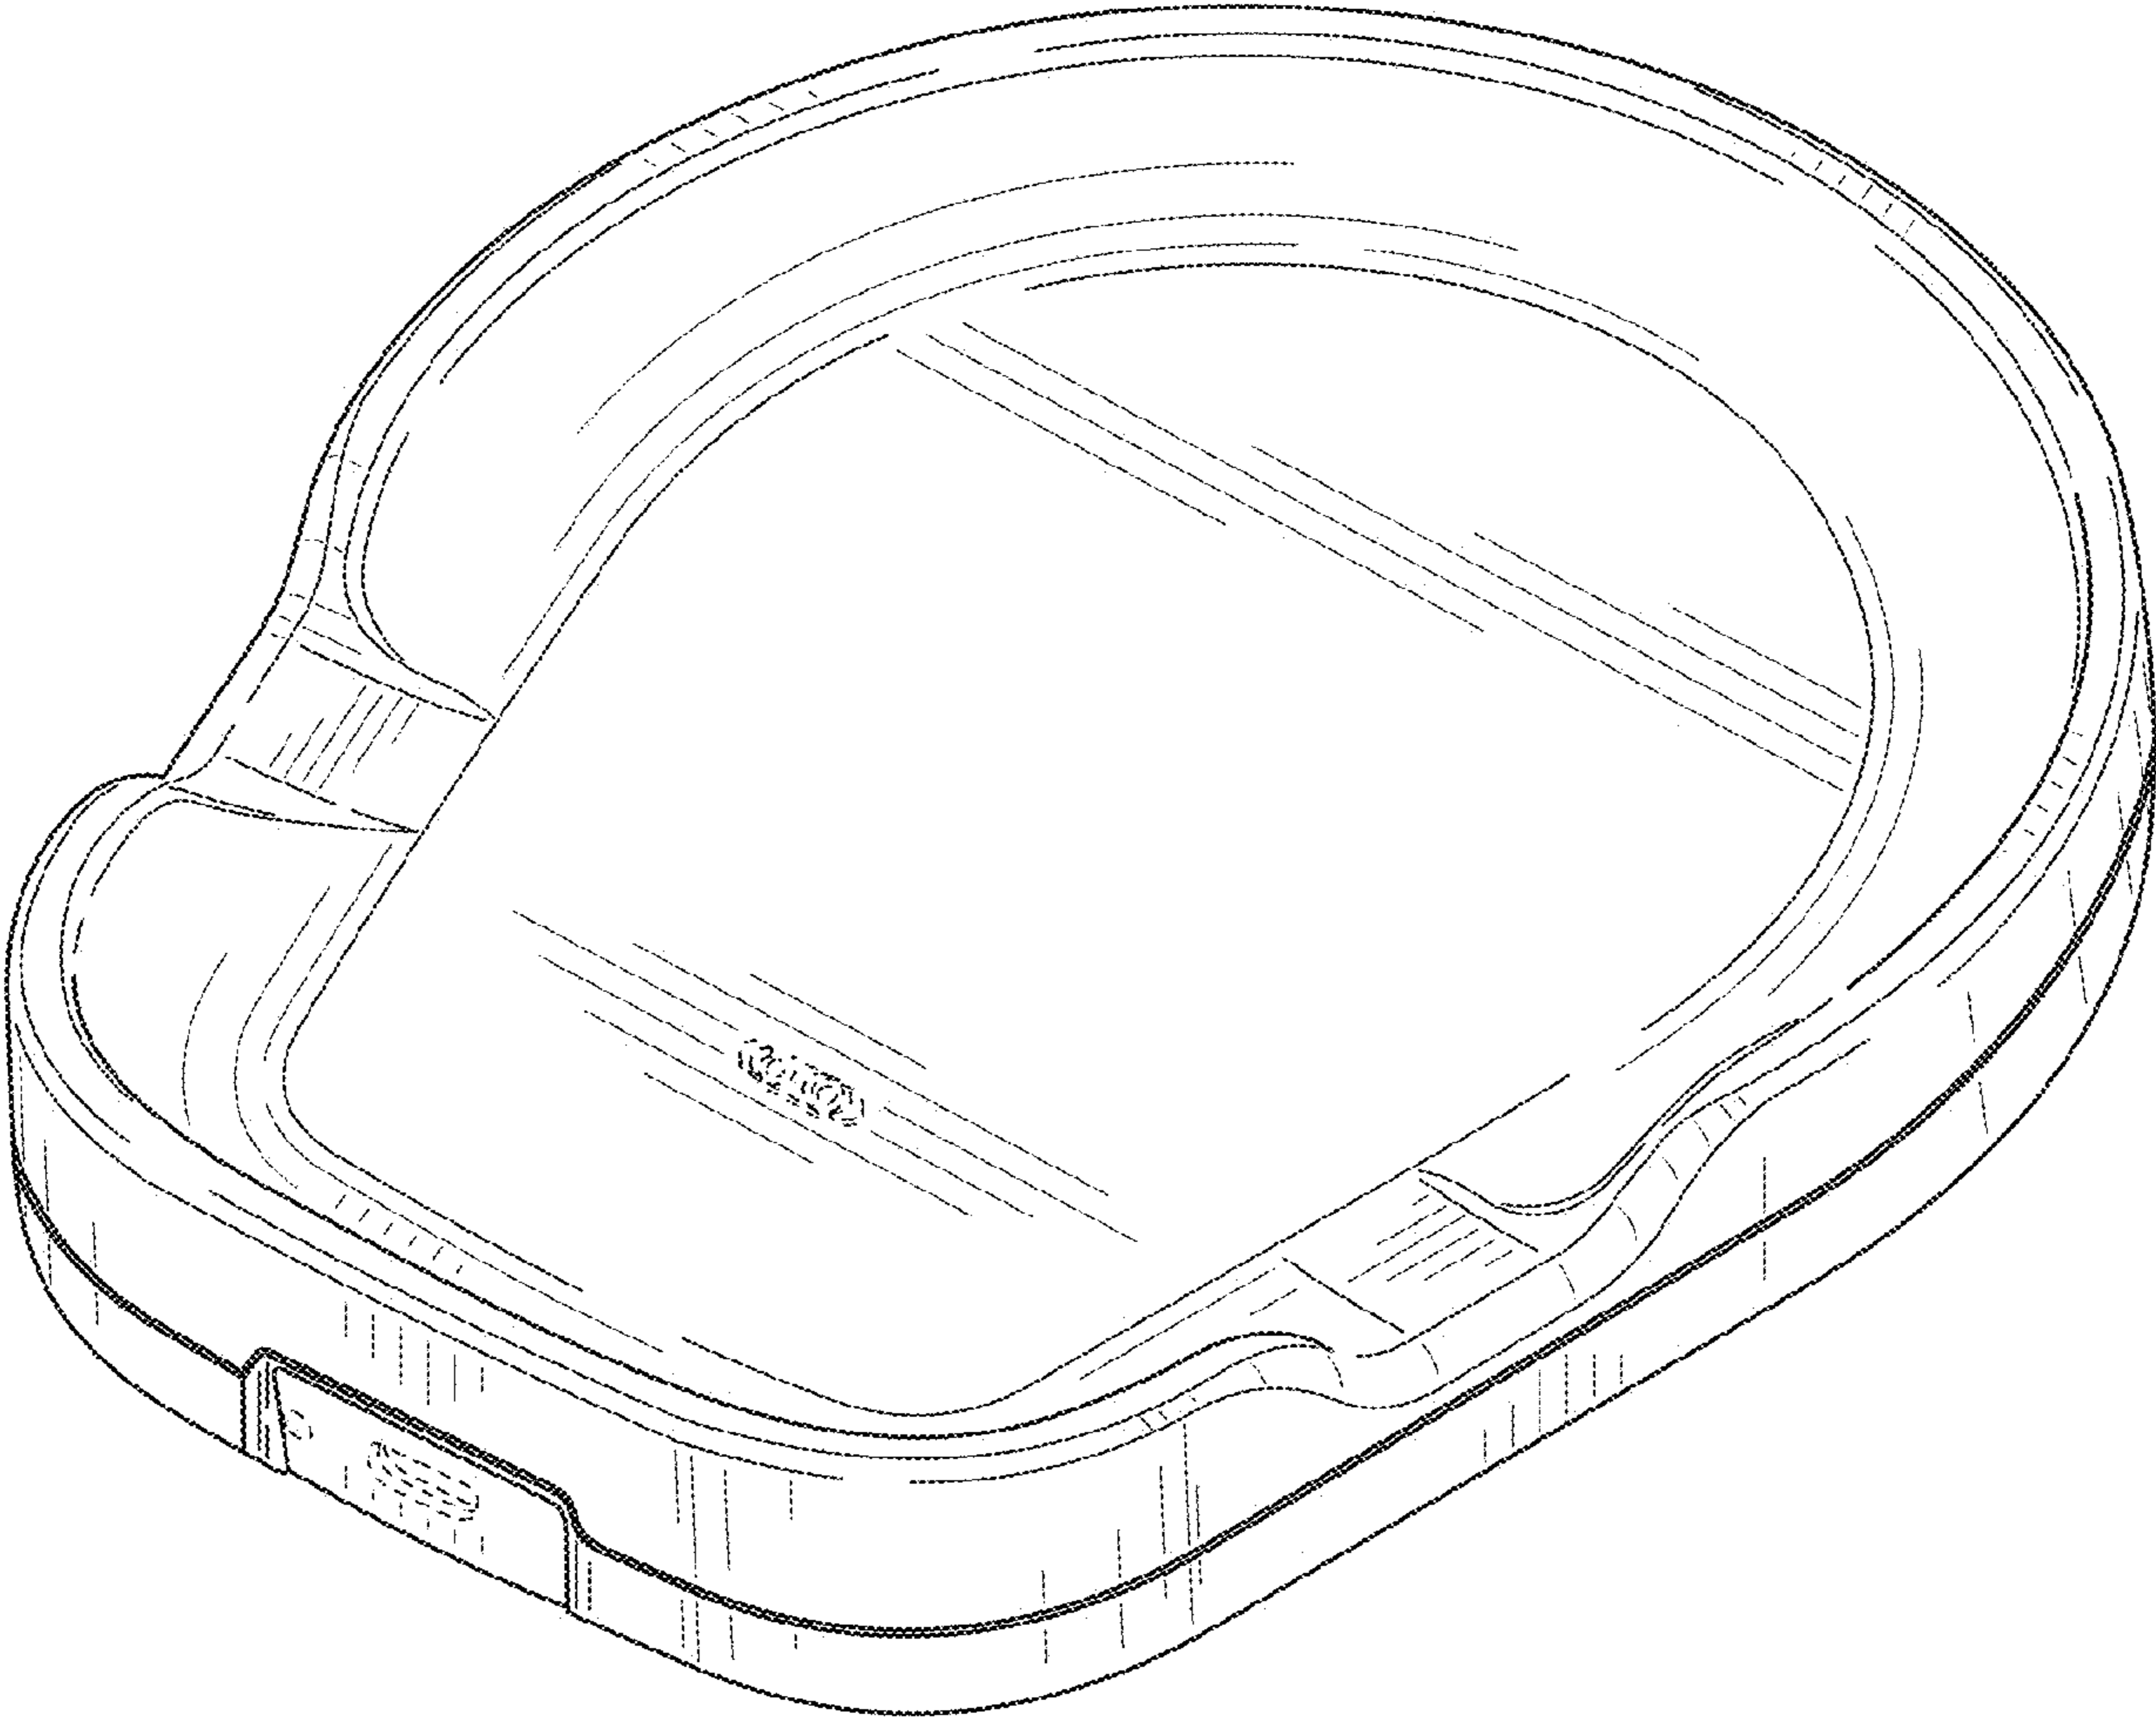


FIG. 1

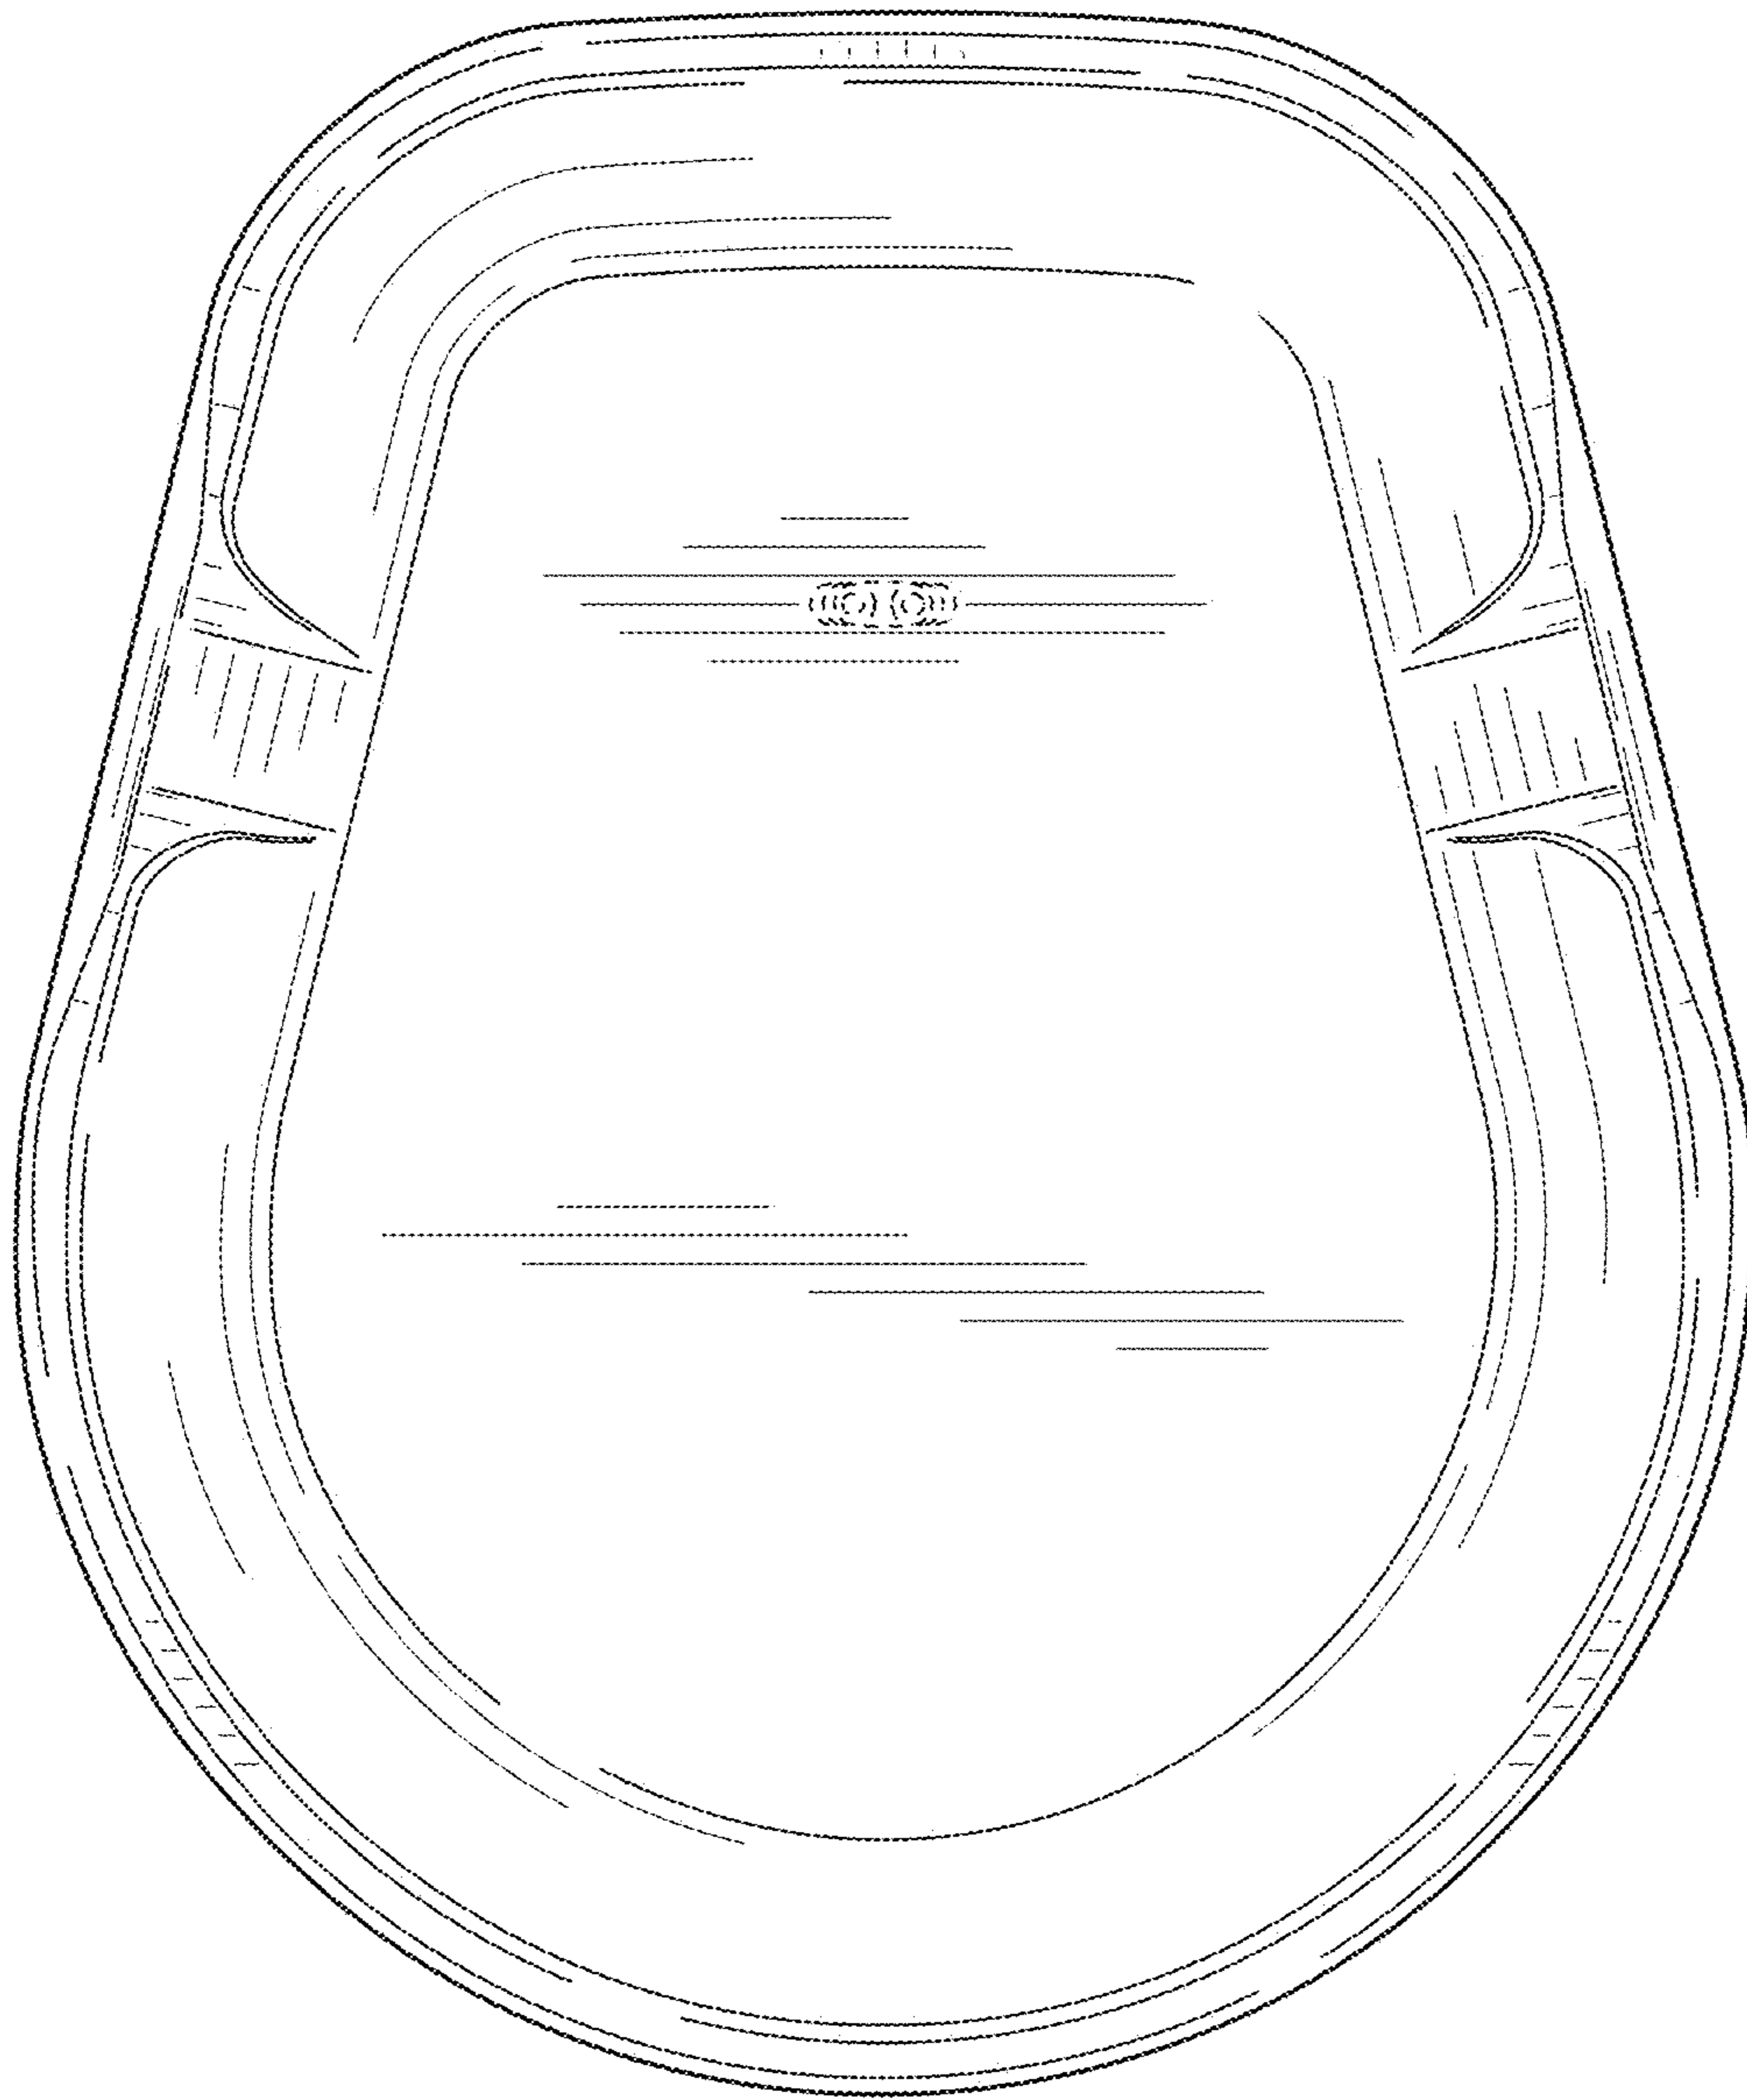


FIG. 2

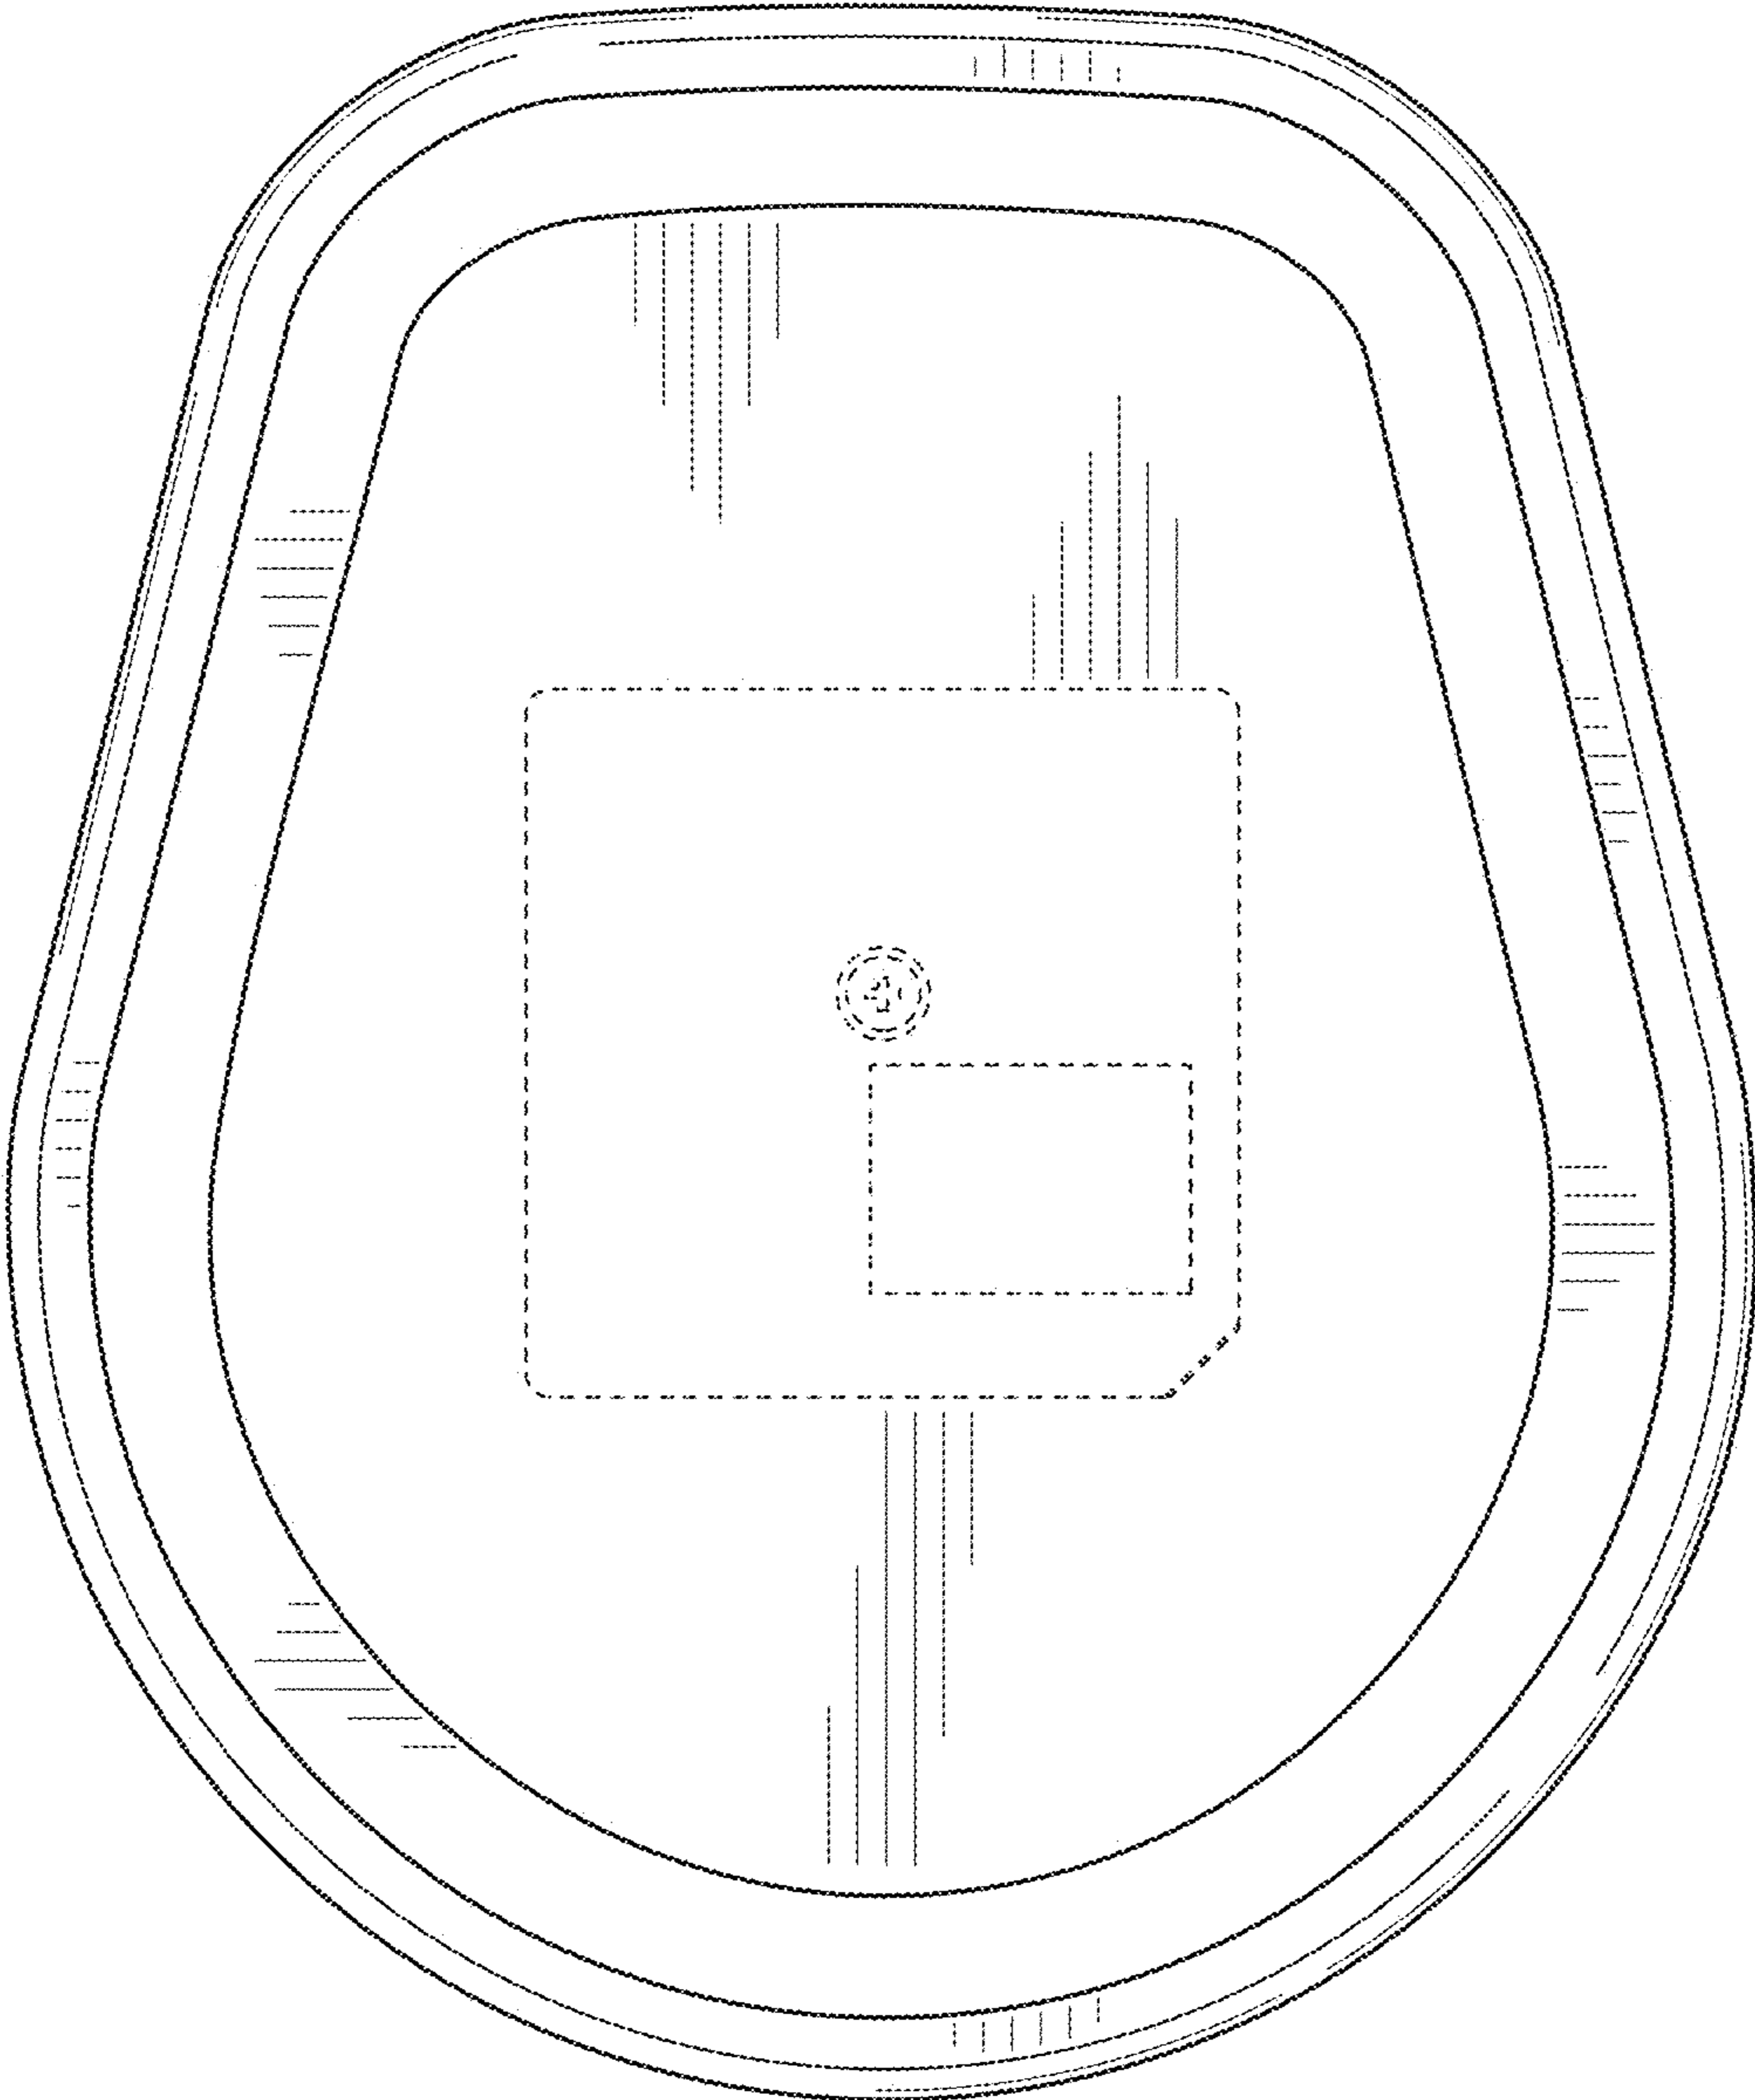


FIG. 3

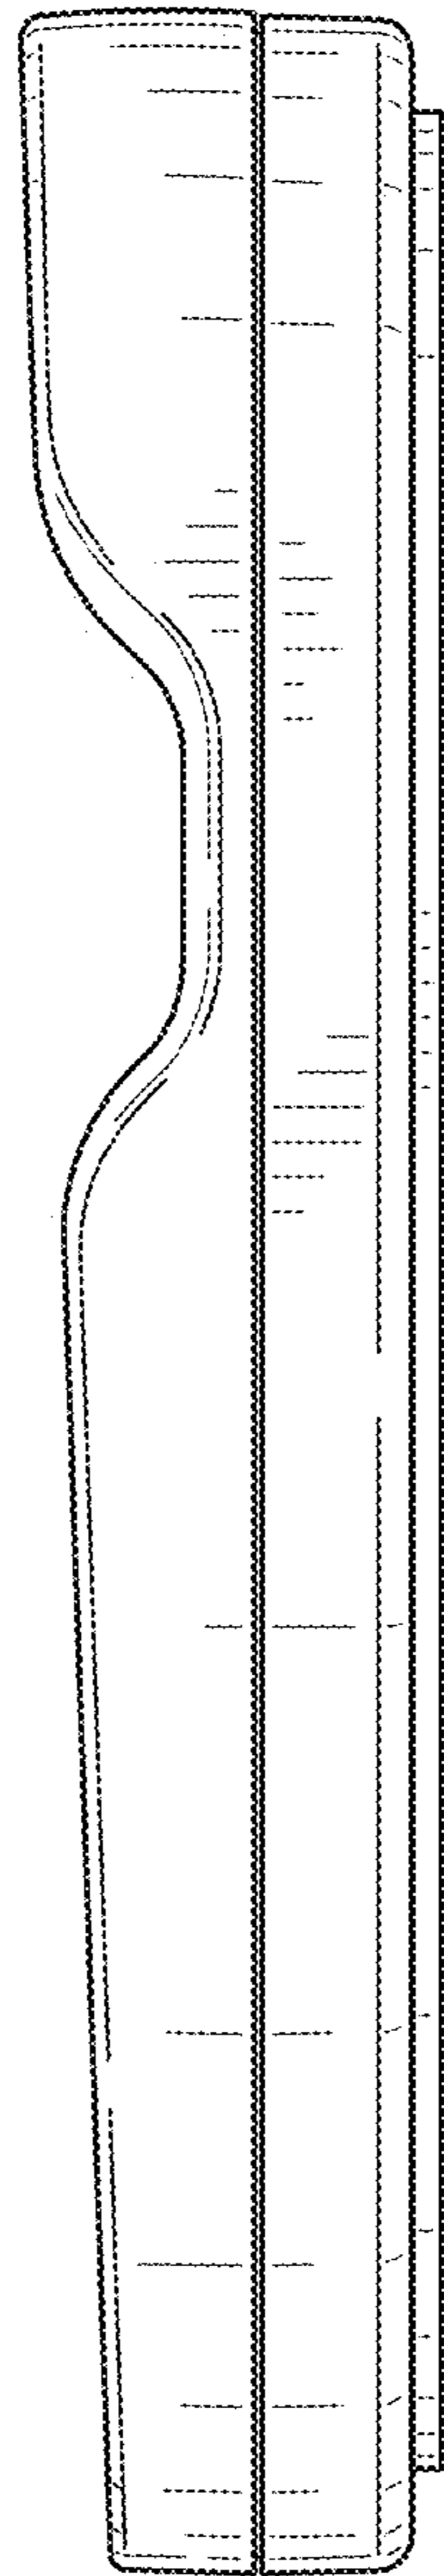


FIG. 4

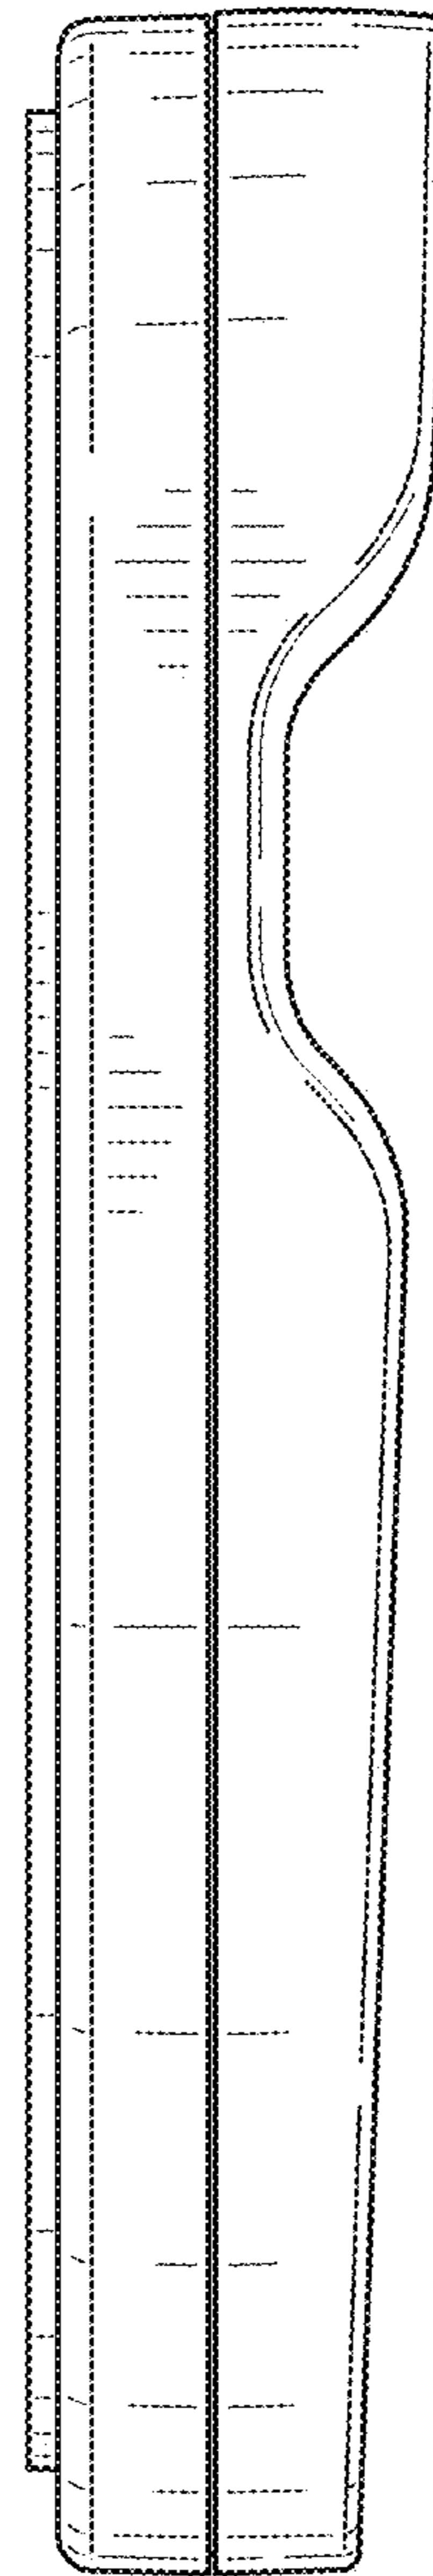


FIG. 5

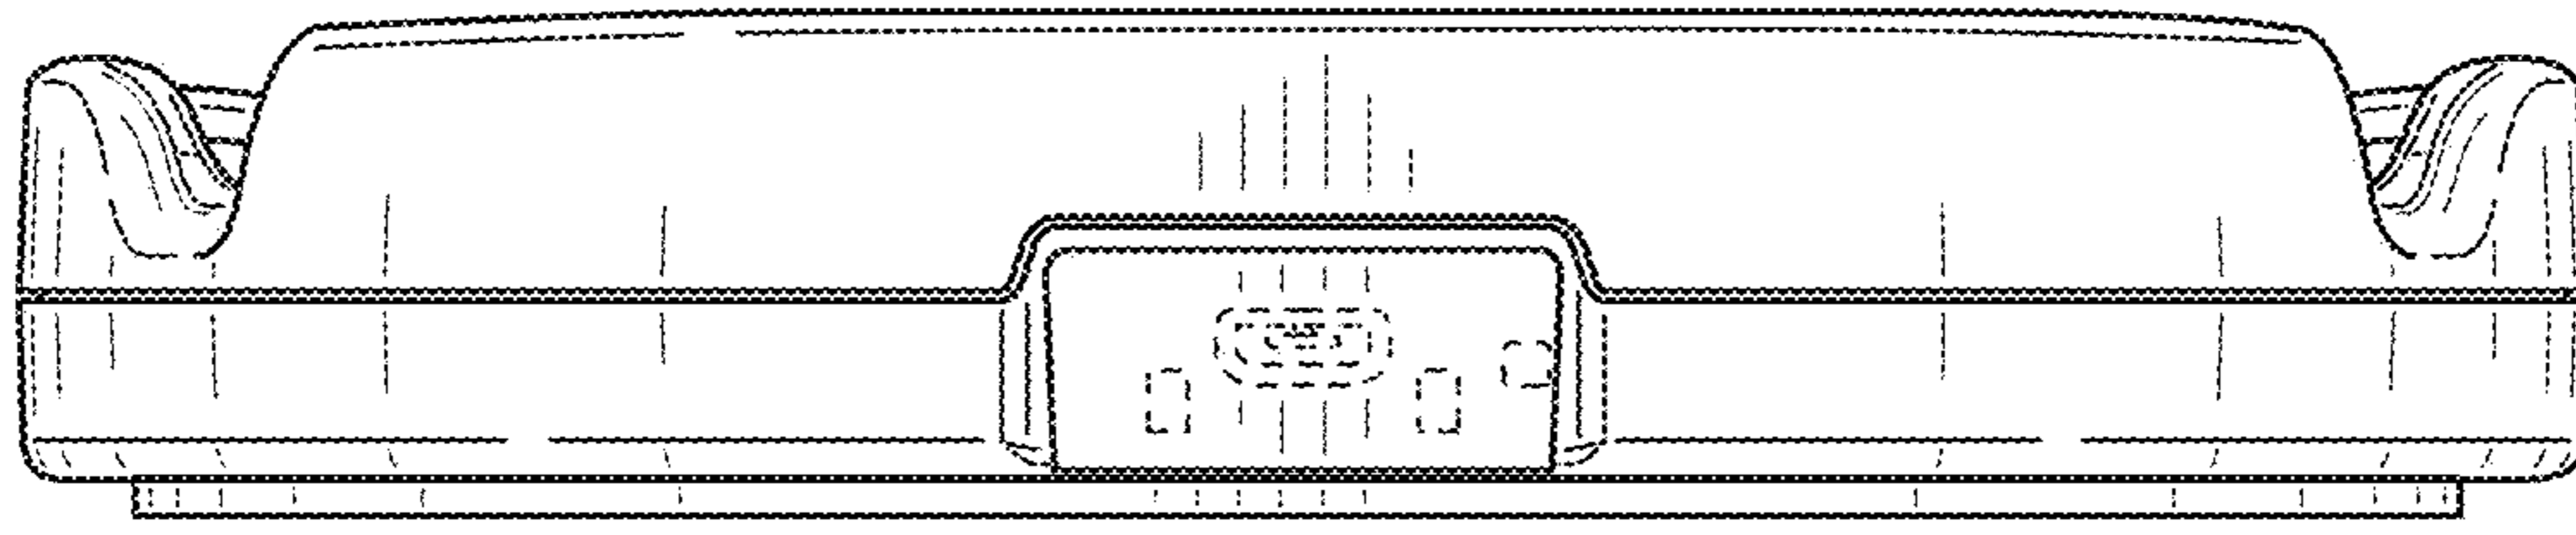


FIG. 6

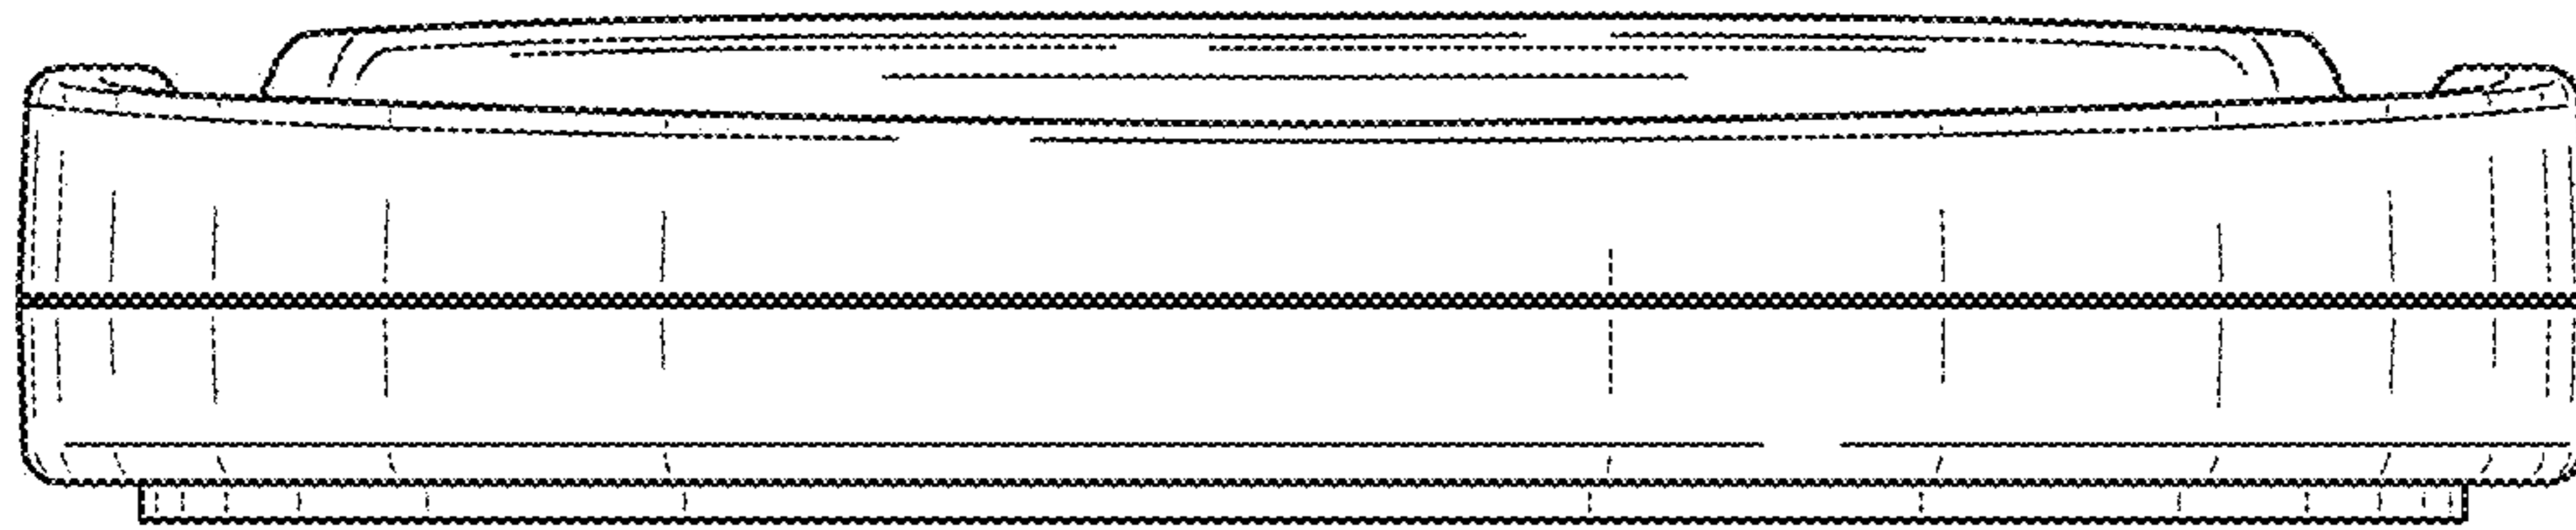


FIG. 7

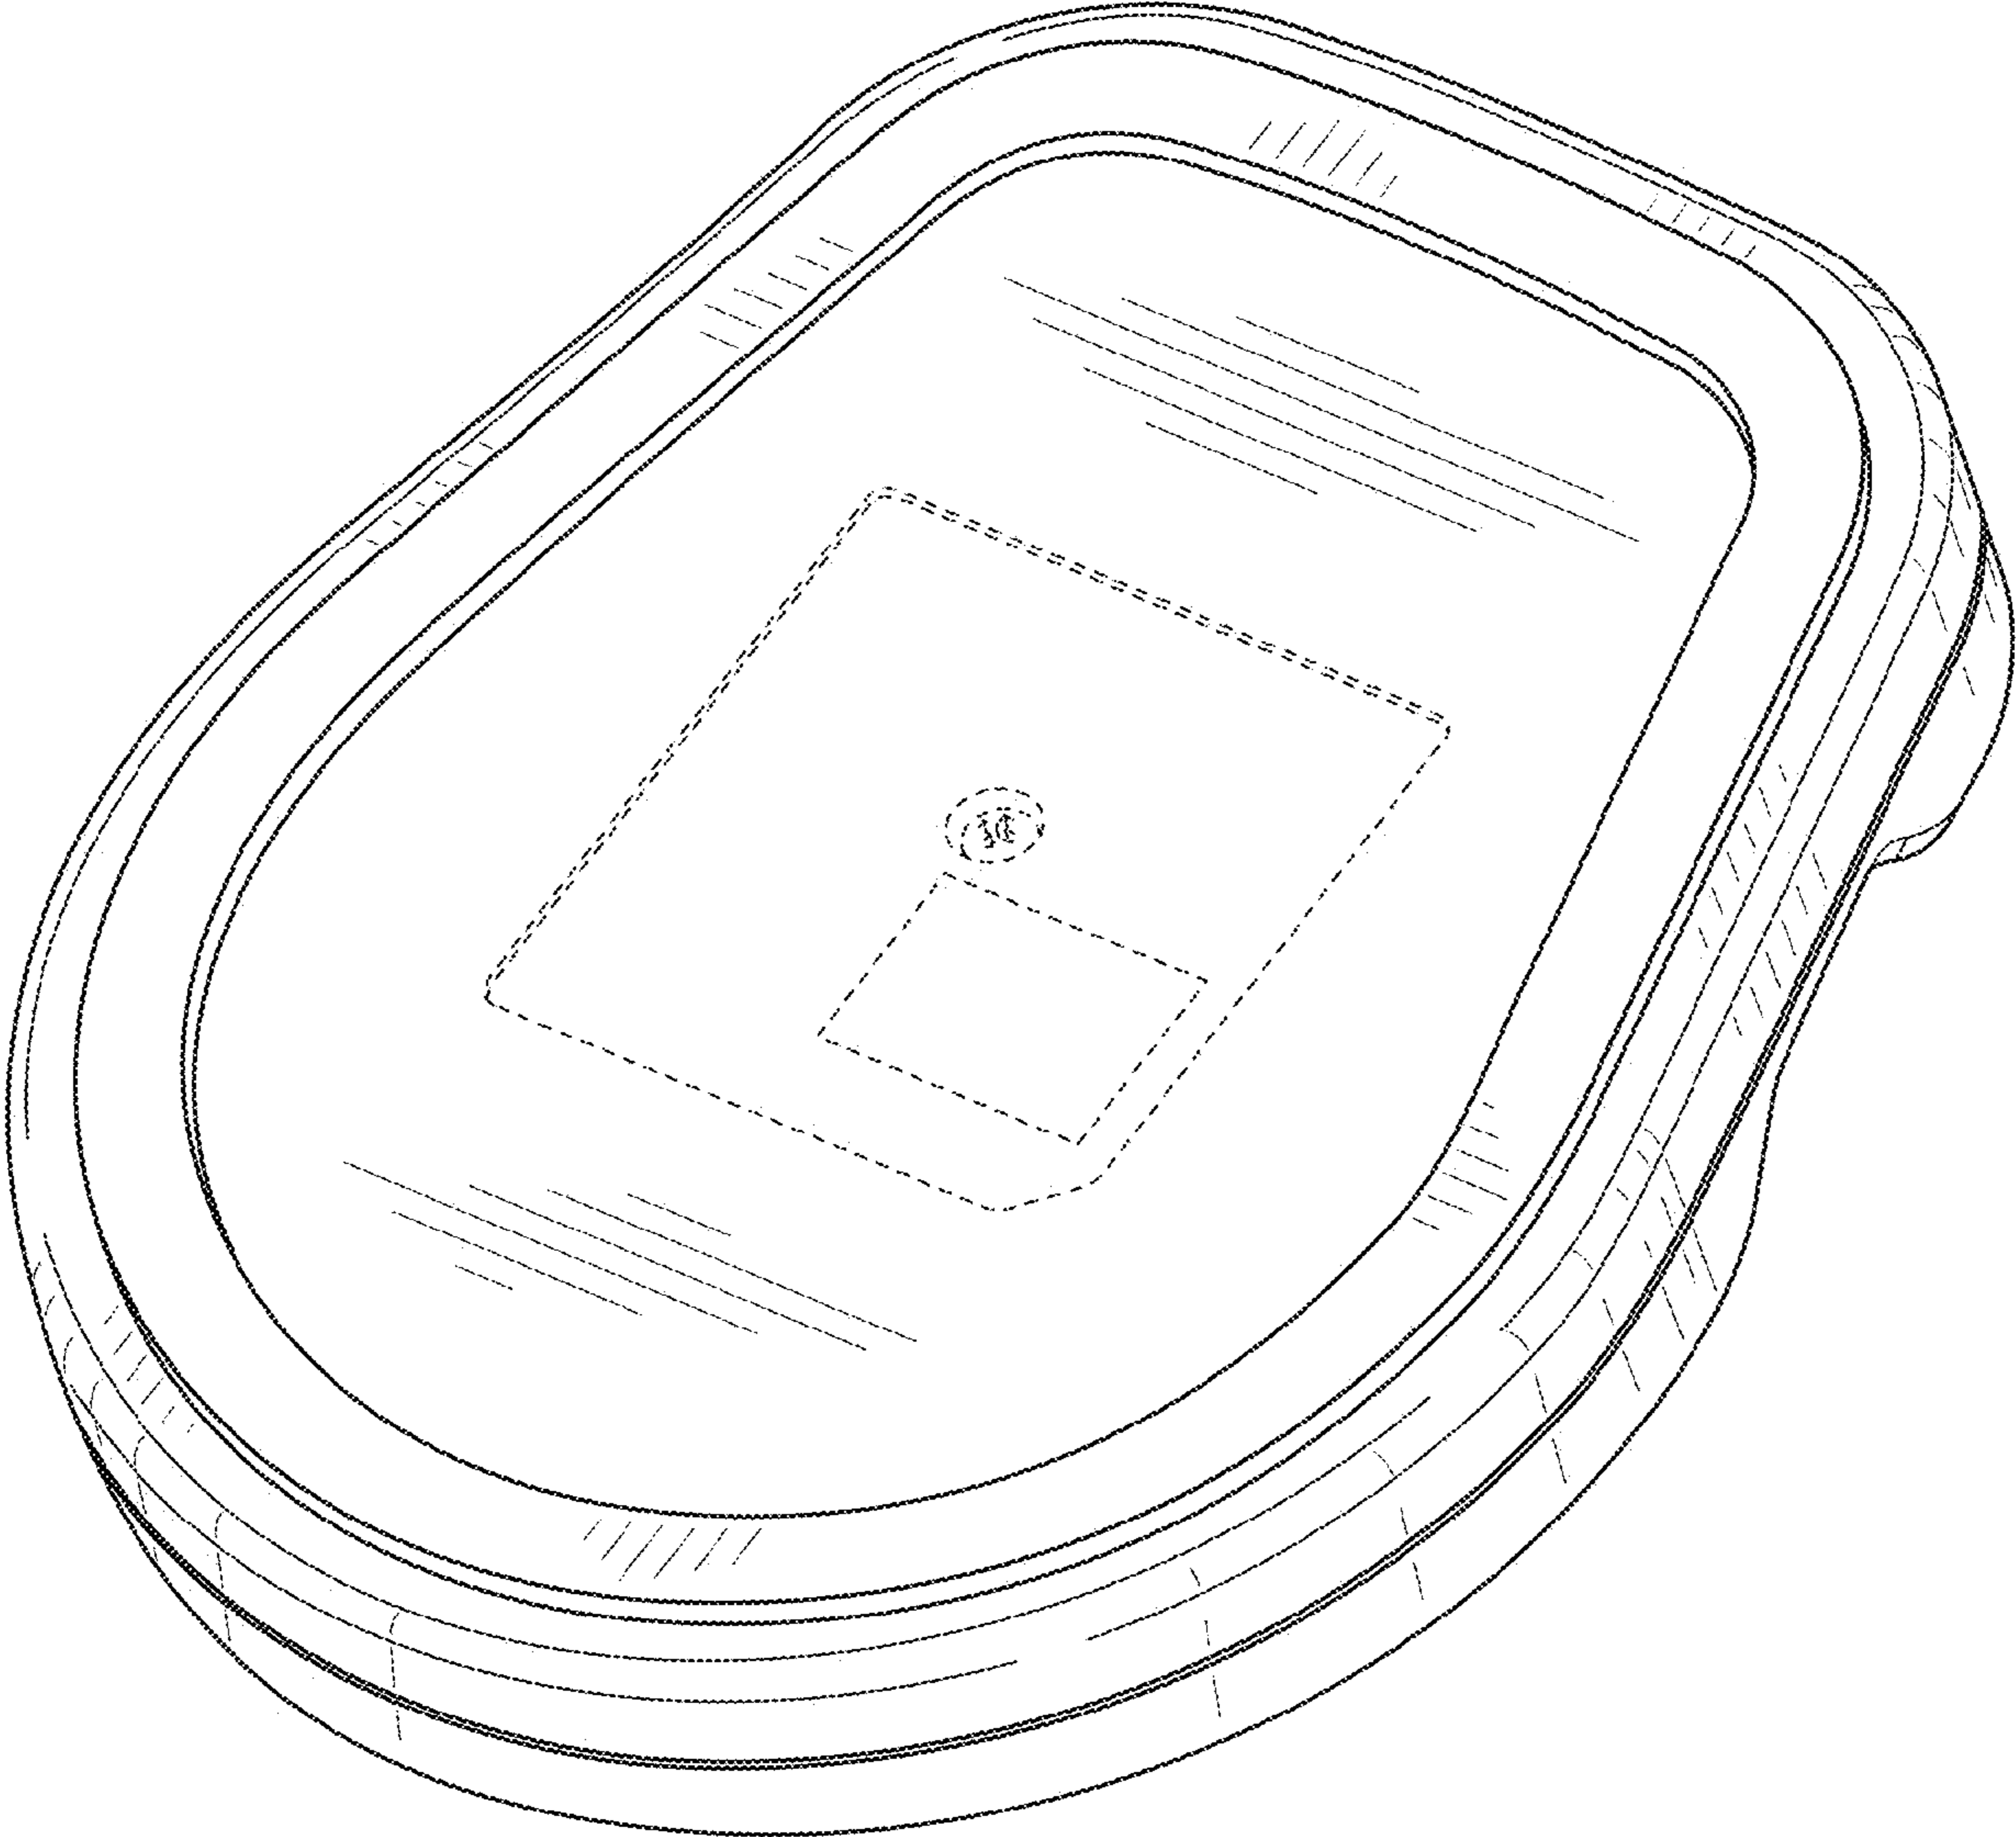


FIG. 8