

US00D957416S

(12) **United States Design Patent**
Everhart et al.

(10) **Patent No.:** **US D957,416 S**
(45) **Date of Patent:** **** Jul. 12, 2022**

(54) **DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE FOR A LABORATORY INSTRUMENT**

(71) Applicant: **Beckman Coulter, Inc.**, Brea, CA (US)

(72) Inventors: **Nicholas Everhart**, Minneapolis, MN (US); **Dana Vajen Habig**, Cincinnati, OH (US); **Shaohui Qiu**, Belmont, MA (US); **Andrew Cottrell**, Minneapolis, MN (US); **Daniel Sunoh Choe**, Minneapolis, MN (US)

(73) Assignee: **BECKMAN COULTER, INC.**, Brea, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/754,097**

(22) Filed: **Oct. 6, 2020**

Related U.S. Application Data

(60) Division of application No. 29/665,995, filed on Oct. 9, 2018, now Pat. No. Des. 898,054, which is a continuation of application No. 29/572,369, filed on Jul. 27, 2016, now Pat. No. Des. 834,044.

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485–486, 487–488, 485–495
CPC H04L 12/1813; H04M 1/72519–72561; G06F 3/048; G06F 3/0481
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D526,655 S 8/2006 McDougall et al.
D527,736 S 9/2006 McDougall et al.
D597,551 S 8/2009 Stone et al.

D637,603 S 5/2011 Godgart
D673,970 S 1/2013 McManigal
D679,284 S 4/2013 Rounding et al.
D689,065 S 9/2013 Glaeske et al.
D689,074 S 9/2013 Talbot et al.
D701,204 S 3/2014 Akana et al.
D733,720 S 7/2015 Mueller et al.
D735,225 S 7/2015 Palestrant et al.
D741,876 S 10/2015 Gaskins et al.
D749,110 S 2/2016 Noack et al.
D750,111 S 2/2016 Walkin
D751,581 S 3/2016 Walker et al.
D751,597 S 3/2016 Pasceri et al.
D756,371 S 5/2016 Bertnick et al.

(Continued)

OTHER PUBLICATIONS

SideFX Houdini. “Workspace.” Vimeo, published Dec. 5, 2014 (Retrieved from the Internet Feb. 17, 2022). Internet URL: <<https://vimeo.com/113734396>> (Year: 2014).*

Primary Examiner — Rachel A. Voorhies
(74) *Attorney, Agent, or Firm* — McAndrews Held & Malloy, Ltd.


(57) **CLAIM**

The ornamental design for a display screen with graphical user interface for a laboratory instrument, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a first embodiment of the display screen with graphical user interface for a laboratory instrument; and,
FIG. 2 is a front view of a second embodiment thereof.
The interior broken lines in the Figures illustrate portions of the graphical user interface that form no part of the claimed design. The broken line perimeter in the Figures is included for the purpose of showing a display screen and forms no part of the claimed design.

1 Claim, 2 Drawing Sheets

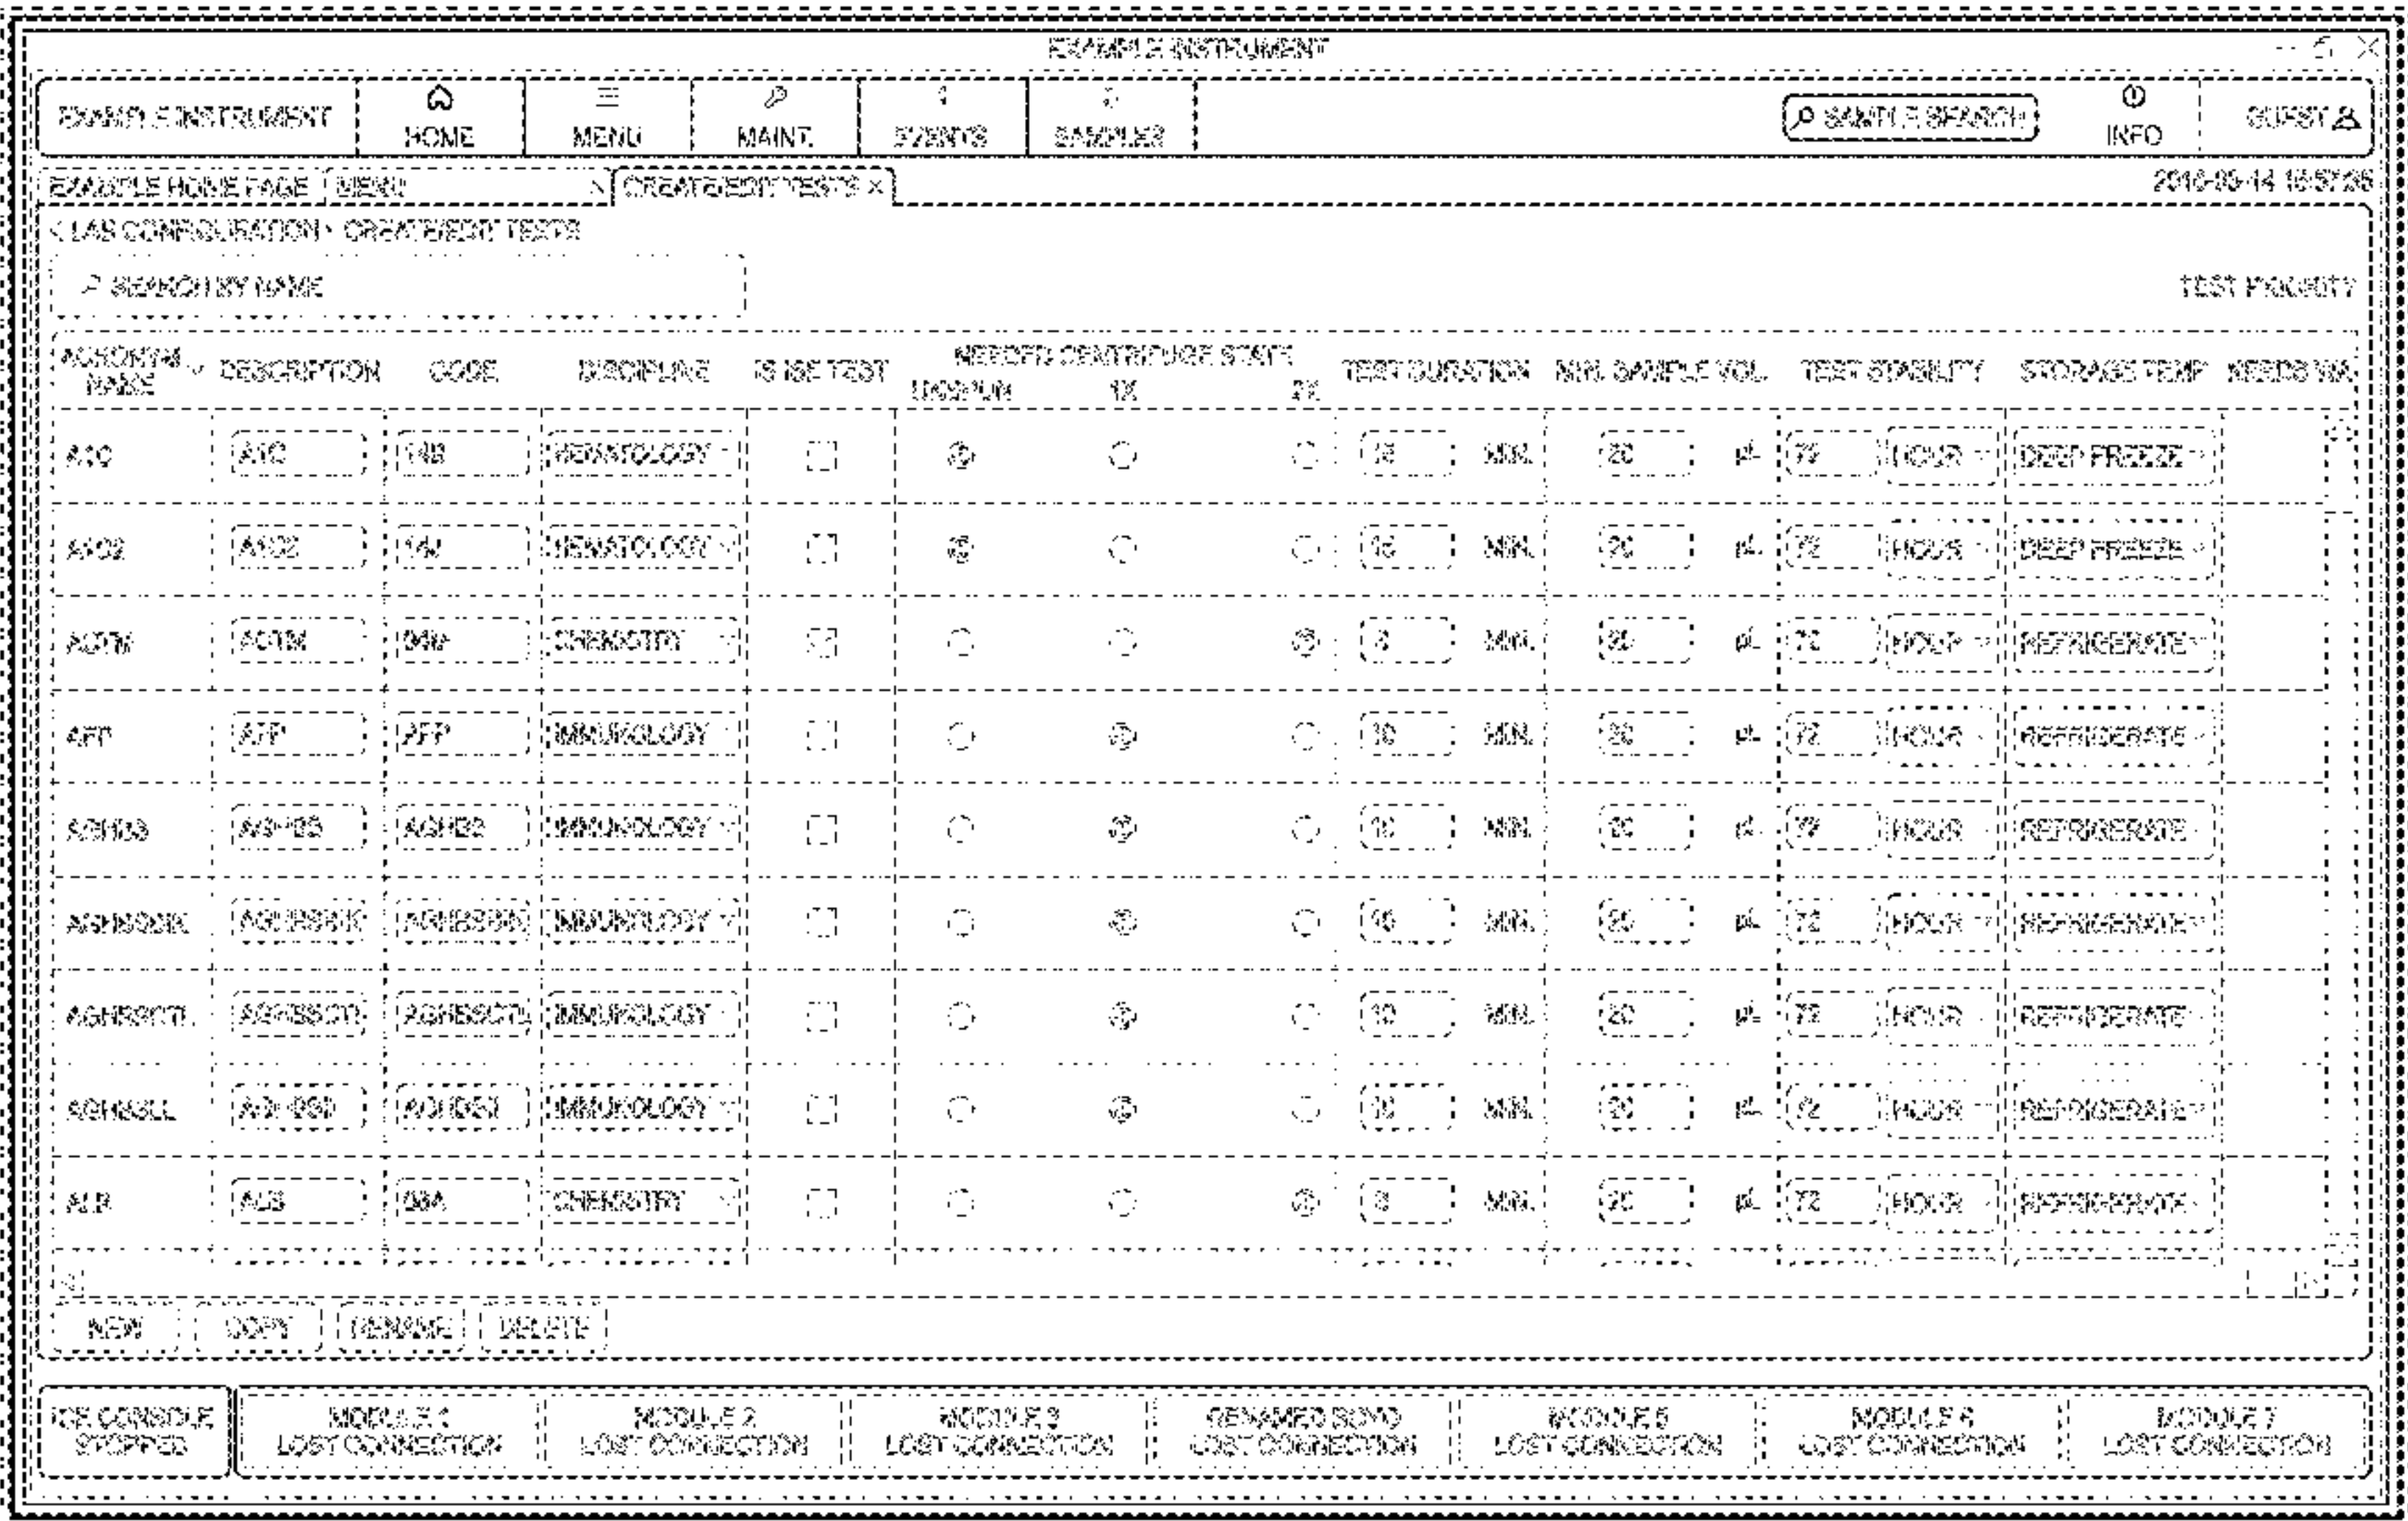

(56)

References Cited

U.S. PATENT DOCUMENTS

D756,372 S 5/2016 Bertnick et al.
D757,050 S 5/2016 Kim
D759,671 S 6/2016 Zarick et al.
D760,248 S 6/2016 Suarez
D762,681 S 8/2016 Sunil
D764,517 S 8/2016 Bachman et al.
D766,256 S 9/2016 Zhang et al.
D766,257 S 9/2016 Zhang et al.
D766,916 S 9/2016 Bertnick et al.
D769,256 S 10/2016 Pickard et al.
D769,932 S 10/2016 Gagnier et al.
D770,467 S 11/2016 Choi
D774,526 S 12/2016 Klein et al.
D780,193 S 2/2017 Pickard et al.
D780,209 S 2/2017 Sabadosh et al.
D784,372 S 4/2017 Kovchiy et al.
D785,008 S 4/2017 Lim et al.
D788,142 S 5/2017 Burke
D788,145 S 5/2017 Sullivan et al.
D789,973 S 6/2017 St. Arnaud et al.
D790,559 S 6/2017 Nogami et al.
D791,154 S 7/2017 Dzierson et al.
D791,792 S 7/2017 Gussev et al.
D791,803 S 7/2017 Lee et al.
D804,500 S 12/2017 Fischer et al.
9,854,411 B2 12/2017 Bargetzi et al.
9,930,497 B2 3/2018 Bargetzi et al.

D864,233 S * 10/2019 Weghorst D14/492
D866,576 S * 11/2019 Devlin D14/486
D869,488 S * 12/2019 Storr D14/486
D871,429 S * 12/2019 Watson D14/486
D874,493 S * 2/2020 Martell D14/486
D877,766 S * 3/2020 Li D14/486
D878,403 S * 3/2020 Watson D14/486
D879,801 S * 3/2020 Edgington, Jr. D14/485
D880,506 S * 4/2020 Watson D14/486
D881,920 S * 4/2020 Argo D14/486
D883,997 S * 5/2020 Einspahr D14/485
D884,008 S * 5/2020 Thornberg D14/486
D898,054 S * 10/2020 Everhart D14/486
D900,132 S * 10/2020 English D14/486
D910,047 S * 2/2021 Einspahr D14/486
10,922,099 B2 * 2/2021 Valtchev G06F 9/454
D912,068 S * 3/2021 Witten D14/485
D916,104 S * 4/2021 Cahill G06F 9/454
D14/486
D916,767 S * 4/2021 VanSickler D14/486
D923,645 S * 6/2021 LaBorde A61B 8/469
D14/490
D927,505 S * 8/2021 Qiu D14/485
D928,194 S * 8/2021 Baker D14/488
D930,703 S * 9/2021 Mast D14/492
D931,869 S * 9/2021 Jung D14/485
2004/0032424 A1 2/2004 Florschuetz
2006/0184966 A1 8/2006 Hunleth et al.
2013/0205244 A1 8/2013 Decker et al.
2019/0365350 A1 * 12/2019 Chiang A61B 8/469

* cited by examiner

EXAMPLE INSTRUMENT
1 2 3 4 5 6 7 8 9 0
INFO
2018-03-14 15:57:35

EXAMPLE INSTRUMENT
HOME
MENU
MAINT.
EVENTS
SAMPLES

1
2
3
4
5
6
7
8
9
0

INFO

EXAMPLE HOME PAGE
MENU
CREATED/EDIT TESTS

2018-03-14 15:57:35

LAB CONFIGURATION
CREATED/EDIT TESTS

SEARCH BY NAME

ACRONYM
DESCRIPTION
CODE
DISCIPLINE
IS USE TEST
NEEDED CENTRIFUGE STATE
TEST DURATION
MIN. SAMPLE VOL.
TEST STABILITY
STORAGE TEMP.
NEEDS WA

UNSPUN
1X
2X

ACRONYM	DESCRIPTION	CODE	DISCIPLINE	IS USE TEST	NEEDED CENTRIFUGE STATE	TEST DURATION	MIN. SAMPLE VOL.	TEST STABILITY	STORAGE TEMP.	NEEDS WA
A1C	A1C	14B	HEMATOLOGY	☐	☐	15	20	72	DEEP FREEZE	
A1C2	A1C2	14J	HEMATOLOGY	☐	☐	15	20	72	DEEP FREEZE	
ACTM	ACTM	94M	CHEMISTRY	☒	☐	3	20	72	REFRIGERATE	
AFP	AFP	AFP	IMMUNOLOGY	☐	☐	10	20	72	REFRIGERATE	
AGHS	AGHS	AGHS	IMMUNOLOGY	☐	☐	10	20	72	REFRIGERATE	
AGHSBK	AGHSBK	AGHSBK	IMMUNOLOGY	☐	☐	10	20	72	REFRIGERATE	
AGHSCTL	AGHSCTL	AGHSCTL	IMMUNOLOGY	☐	☐	10	20	72	REFRIGERATE	
AGHSLL	AGHSLL	AGHSLL	IMMUNOLOGY	☐	☐	10	20	72	REFRIGERATE	
ALB	ALB	ORA	CHEMISTRY	☐	☐	3	20	72	REFRIGERATE	

NEW
COPY
RENAME
DELETE

ICE CONSOLE STOPPED

MODULE 1
LOST CONNECTION

MODULE 2
LOST CONNECTION

MODULE 3
LOST CONNECTION

RENAME BOYO
LOST CONNECTION

MODULE 6
LOST CONNECTION

MODULE 7
LOST CONNECTION

EXAMPLE INSTRUMENT

HOME

MENU

MAINT.

EVENTS

SAMPLES

INFO

QUEST

2016-03-14 15:57:35

EXAMPLE HOME PAGE

MENU

CREATE/EDIT TESTS

LAB CONFIGURATION

CREATE/EDIT TESTS

SEARCH BY NAME

TEST PRIORITY

ACRONYM	DESCRIPTION	CODE	DISCIPLINE	IS USE TEST	NEEDED CENTRIFUGE STATE	TEST DURATION	MIN. SAMPLE VOL.	TEST STABILITY	STORAGE TEMP	NEEDS WA
					UNSPUN 1X	2X				
A1C	A1C	14B	HEMATOLOGY	☐	☒	☐	15 MIN.	72 HOUR	DEEP FREEZE	
A1C2	A1C2	14J	HEMATOLOGY	☐	☒	☐	15 MIN.	72 HOUR	DEEP FREEZE	
ACTM	ACTM	94M	CHEMISTRY	☒	☐	☒	3 MIN.	72 HOUR	REFRIGERATE	
AFP	AFP	A5P	IMMUNOLOGY	☐	☐	☒	10 MIN.	72 HOUR	REFRIGERATE	
AGHS	AGHS	AGHS	IMMUNOLOGY	☐	☐	☒	10 MIN.	72 HOUR	REFRIGERATE	
AGHSBK	AGHSBK	AGHSBK	IMMUNOLOGY	☐	☐	☒	10 MIN.	72 HOUR	REFRIGERATE	
AGHSCTL	AGHSCTL	AGHSCTL	IMMUNOLOGY	☐	☐	☒	10 MIN.	72 HOUR	REFRIGERATE	
AGHSLL	AGHSLL	AGHSLL	IMMUNOLOGY	☐	☐	☒	10 MIN.	72 HOUR	REFRIGERATE	
ALB	ALB	38A	CHEMISTRY	☐	☐	☒	3 MIN.	72 HOUR	REFRIGERATE	

NEW

COPY

RENAME

DELETE

ICE CONSOLE STOPPED

MODULE 1

MODULE 2

MODULE 3

RENAME BOYO

MODULE 5

MODULE 7

2
G

LL