



US00D957641S

(12) **United States Design Patent** (10) **Patent No.:** **US D957,641 S**
Li (45) **Date of Patent:** **** Jul. 12, 2022**

(54) **SPECTROMETRY OXIMETER FOR ADULTS**

D925,742 S * 7/2021 Zhang D24/169
D926,324 S * 7/2021 Zhang D24/169
2010/0317944 A1* 12/2010 Wang A61B 5/6838
600/323
2019/0090795 A1* 3/2019 Boller A61B 5/14552

(71) Applicant: **Guangdong HealthTree Medical Technology Co., Ltd.**, Guangdong (CN)

(72) Inventor: **Dong Li**, Guangdong (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/740,583**

(22) Filed: **Jul. 6, 2020**

(30) **Foreign Application Priority Data**

May 12, 2020 (CN) 202030214823.0

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/169**

(58) **Field of Classification Search**
USPC D24/107, 165-169, 186, 187, 200, 164;
D10/70, 98; D14/341, 344
CPC G01N 33/66; G01N 33/49; G01N 33/493;
A61B 5/0205; A61B 5/02427; A61B
5/02438; A61B 5/14552; A61B 5/6626;
A61B 5/6638

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D670,388 S * 11/2012 Jin D24/169
D691,726 S * 10/2013 Jin D24/169
D903,872 S * 12/2020 Wang D24/169
D918,394 S * 5/2021 Hu D24/169
D922,582 S * 6/2021 Peng D24/169

FOREIGN PATENT DOCUMENTS

GB 6062076 * 5/2019

OTHER PUBLICATIONS

Amazon.com: Fingertip Pulse Oximeter Blood Oxygen Saturation Monitor, Heart Rate and Fast Spo2 Reading Oxygen Meter with OLED Screen 2 X AAA BatteriesProduct first available: Feb. 25, 2020. Retrieved from website: https://www.amazon.com/dp/B0854BM41R/ref=emc_b_5_i.*

* cited by examiner

Primary Examiner — Anhdao Doan

(57) **CLAIM**

The ornamental design for a spectrometry oximeter for adults, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the spectrometry oximeter for adults;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left side elevational view thereof;


FIG. 5 is a right side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines illustrate portions of the spectrometry oximeter for adults that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

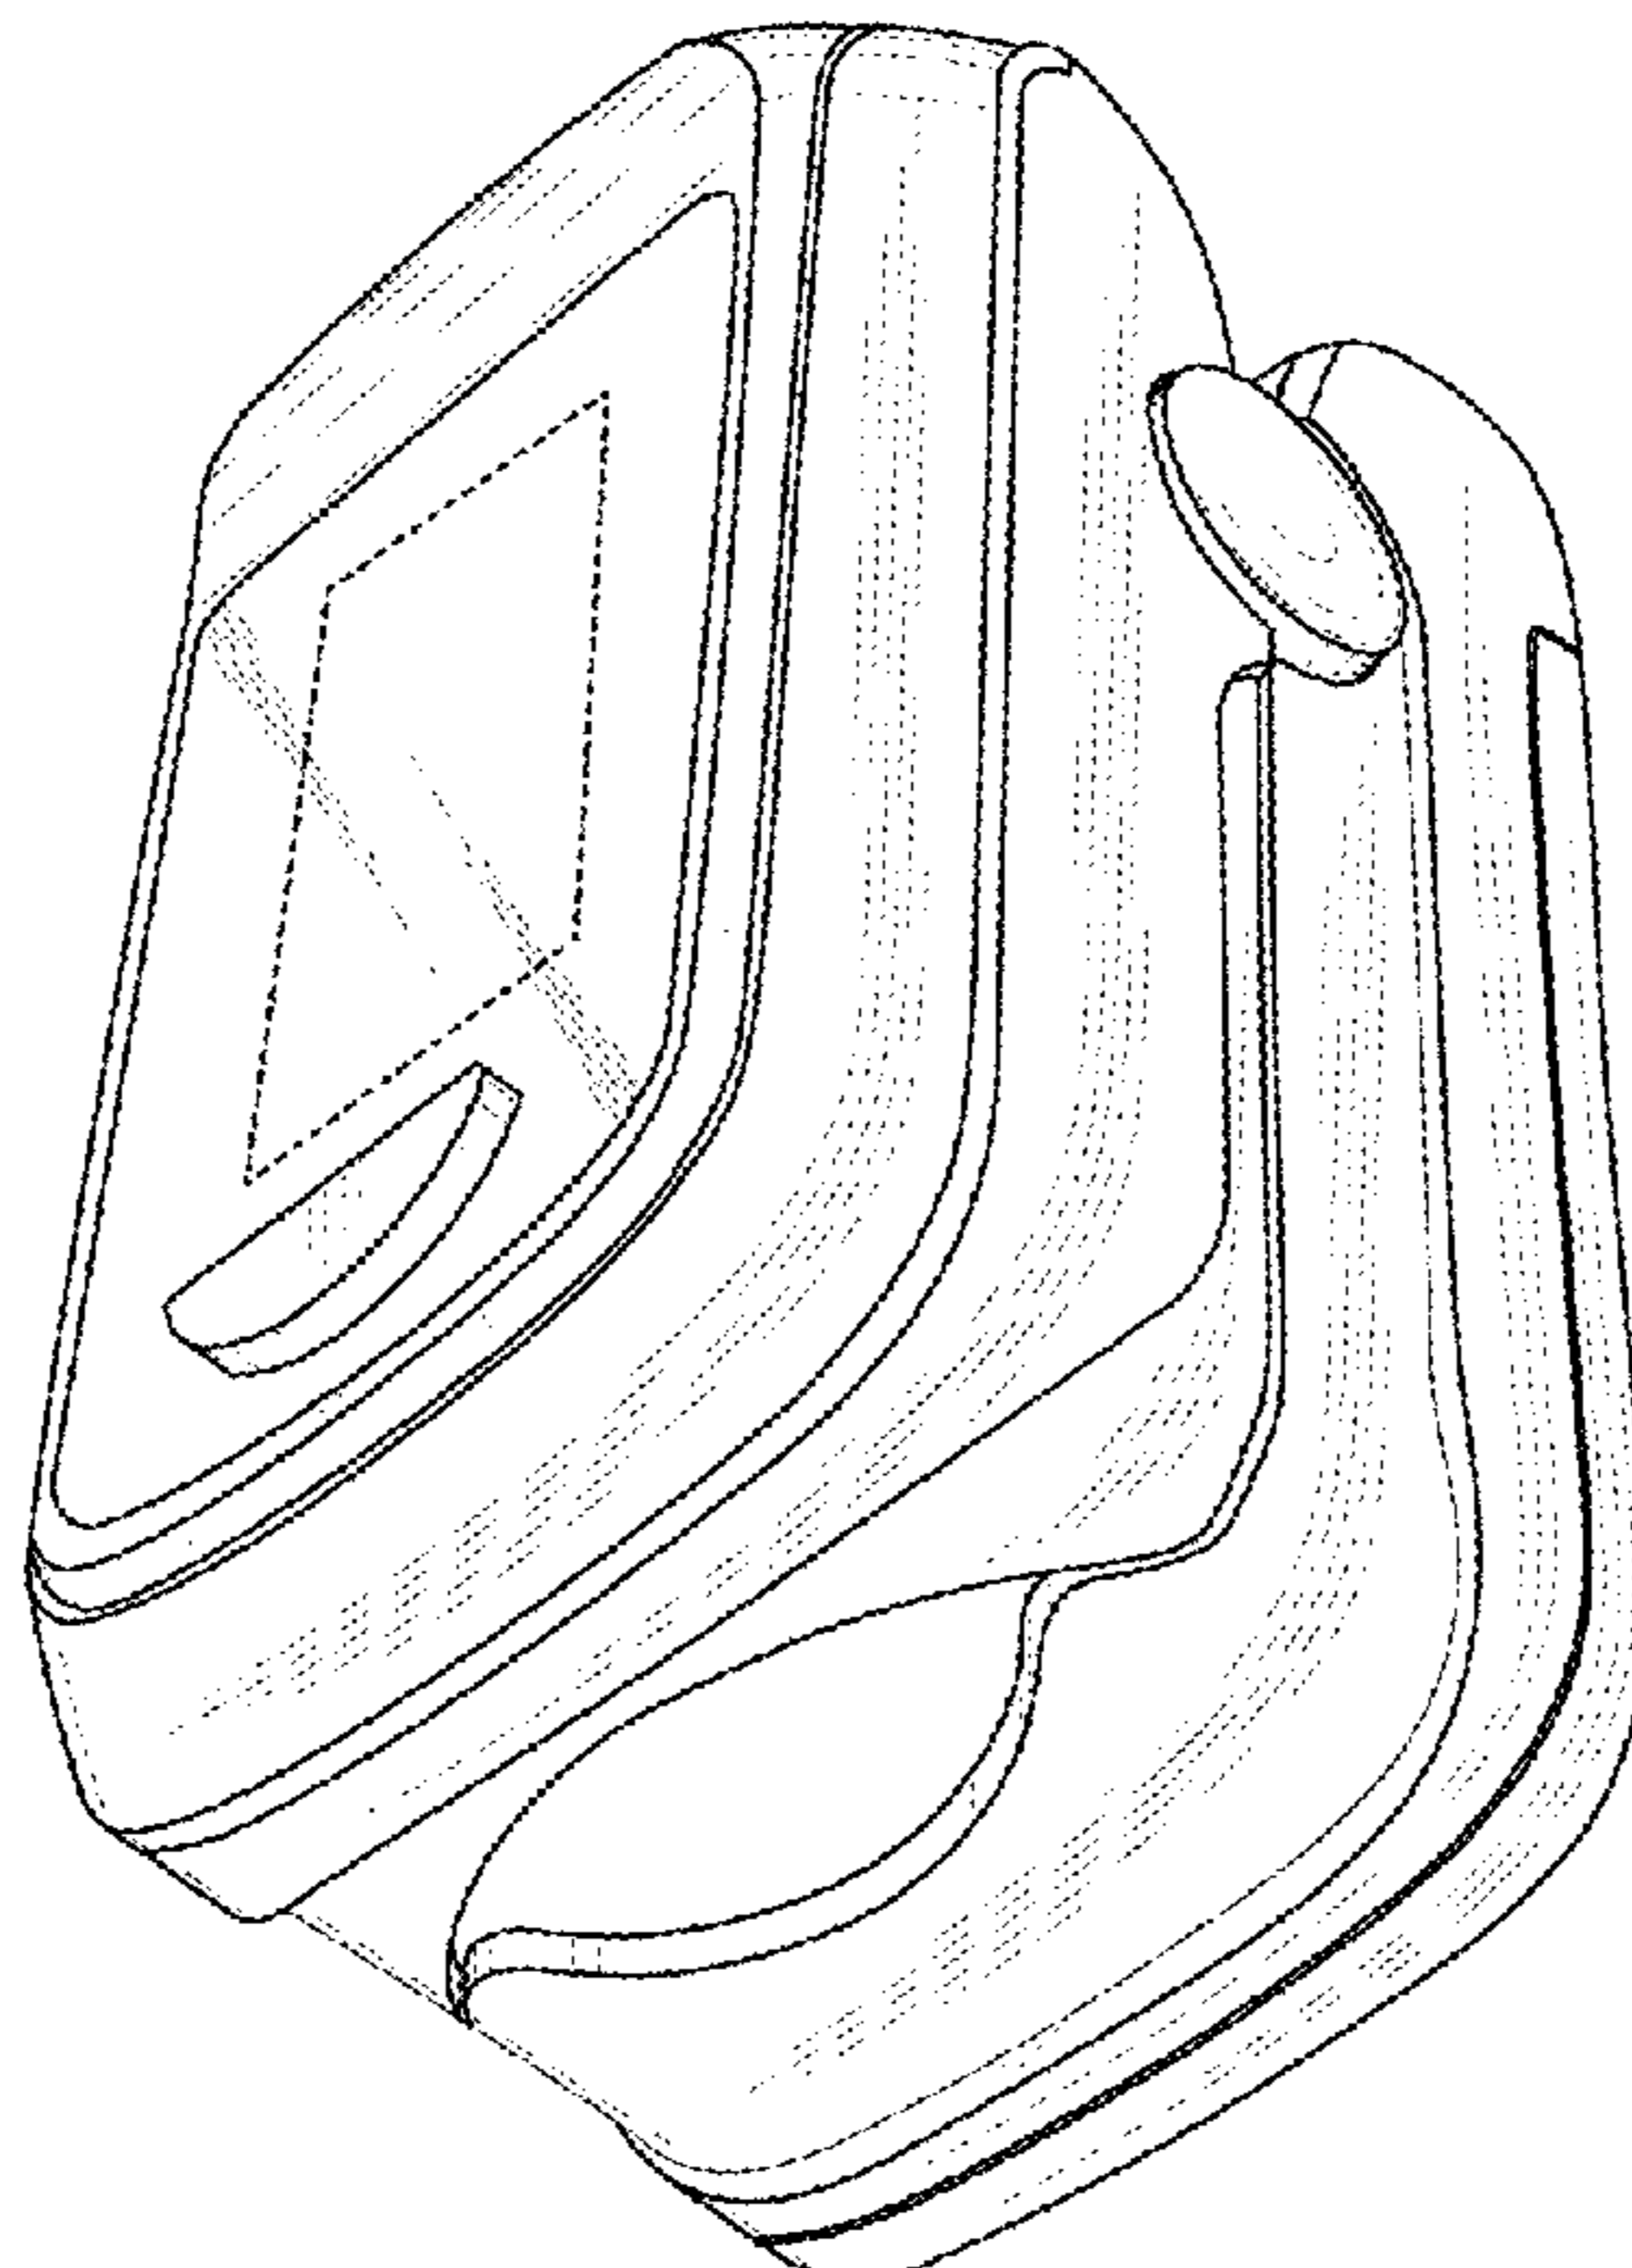

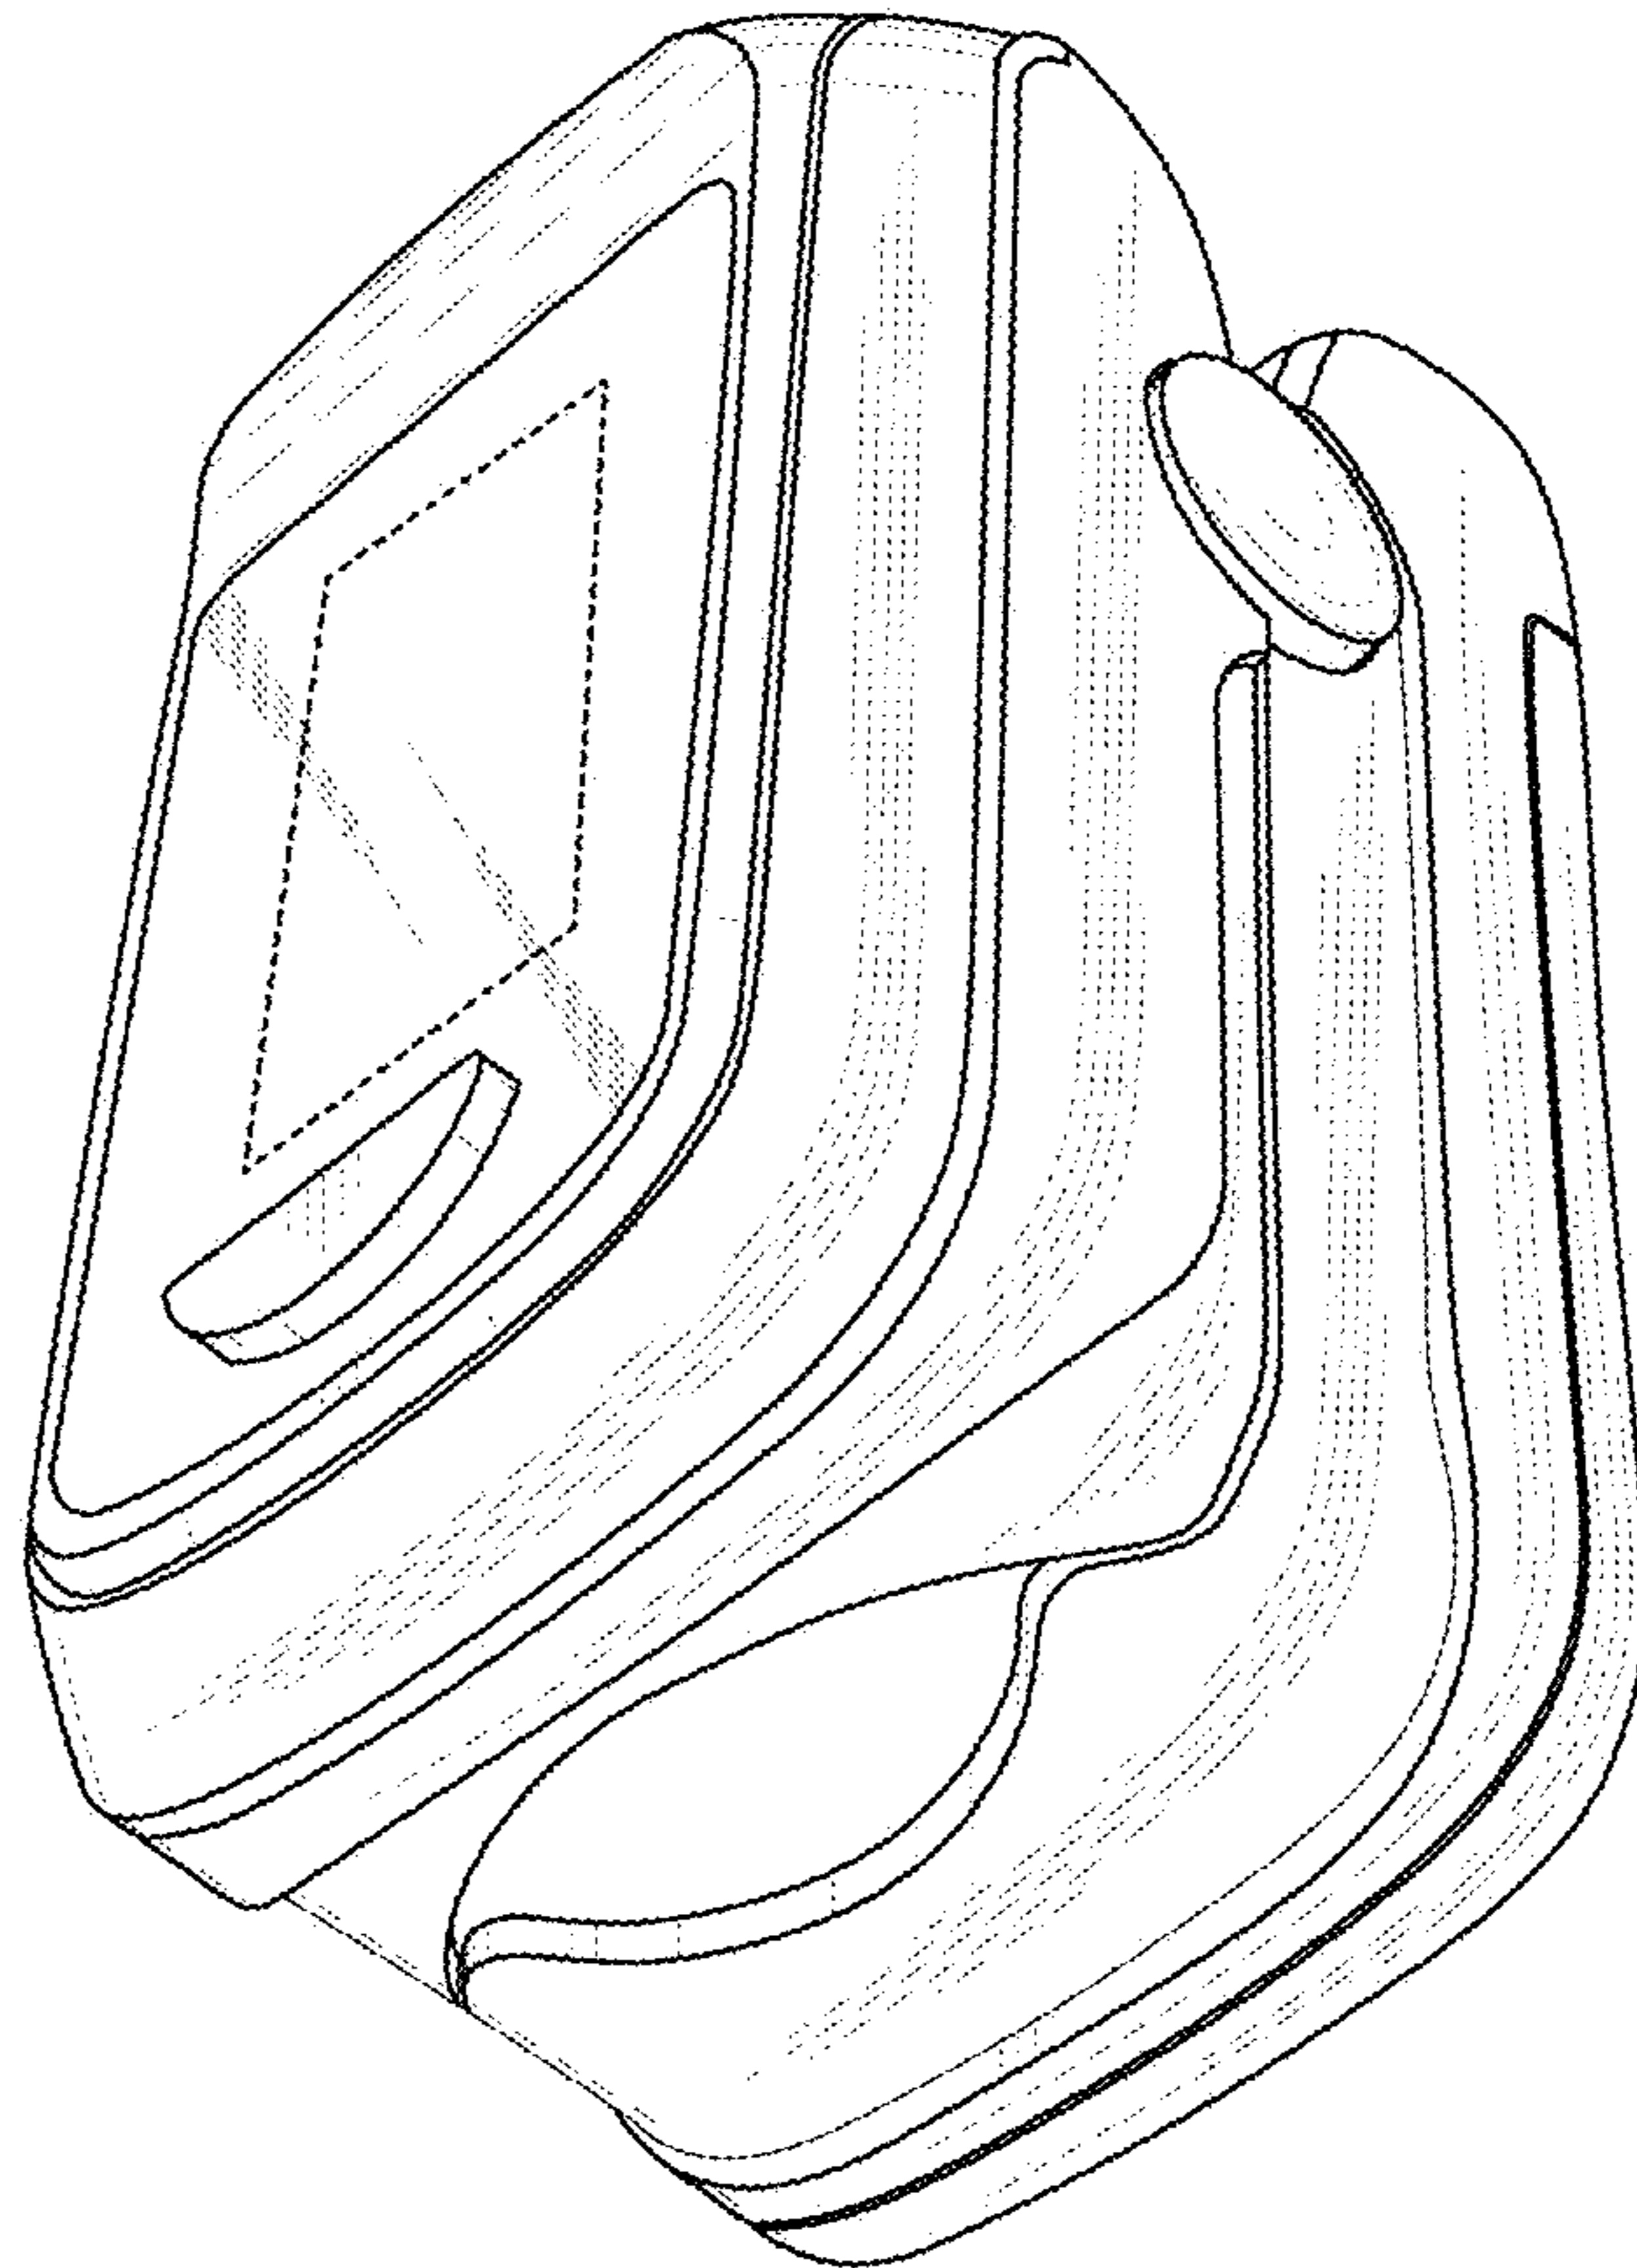


Figure 1

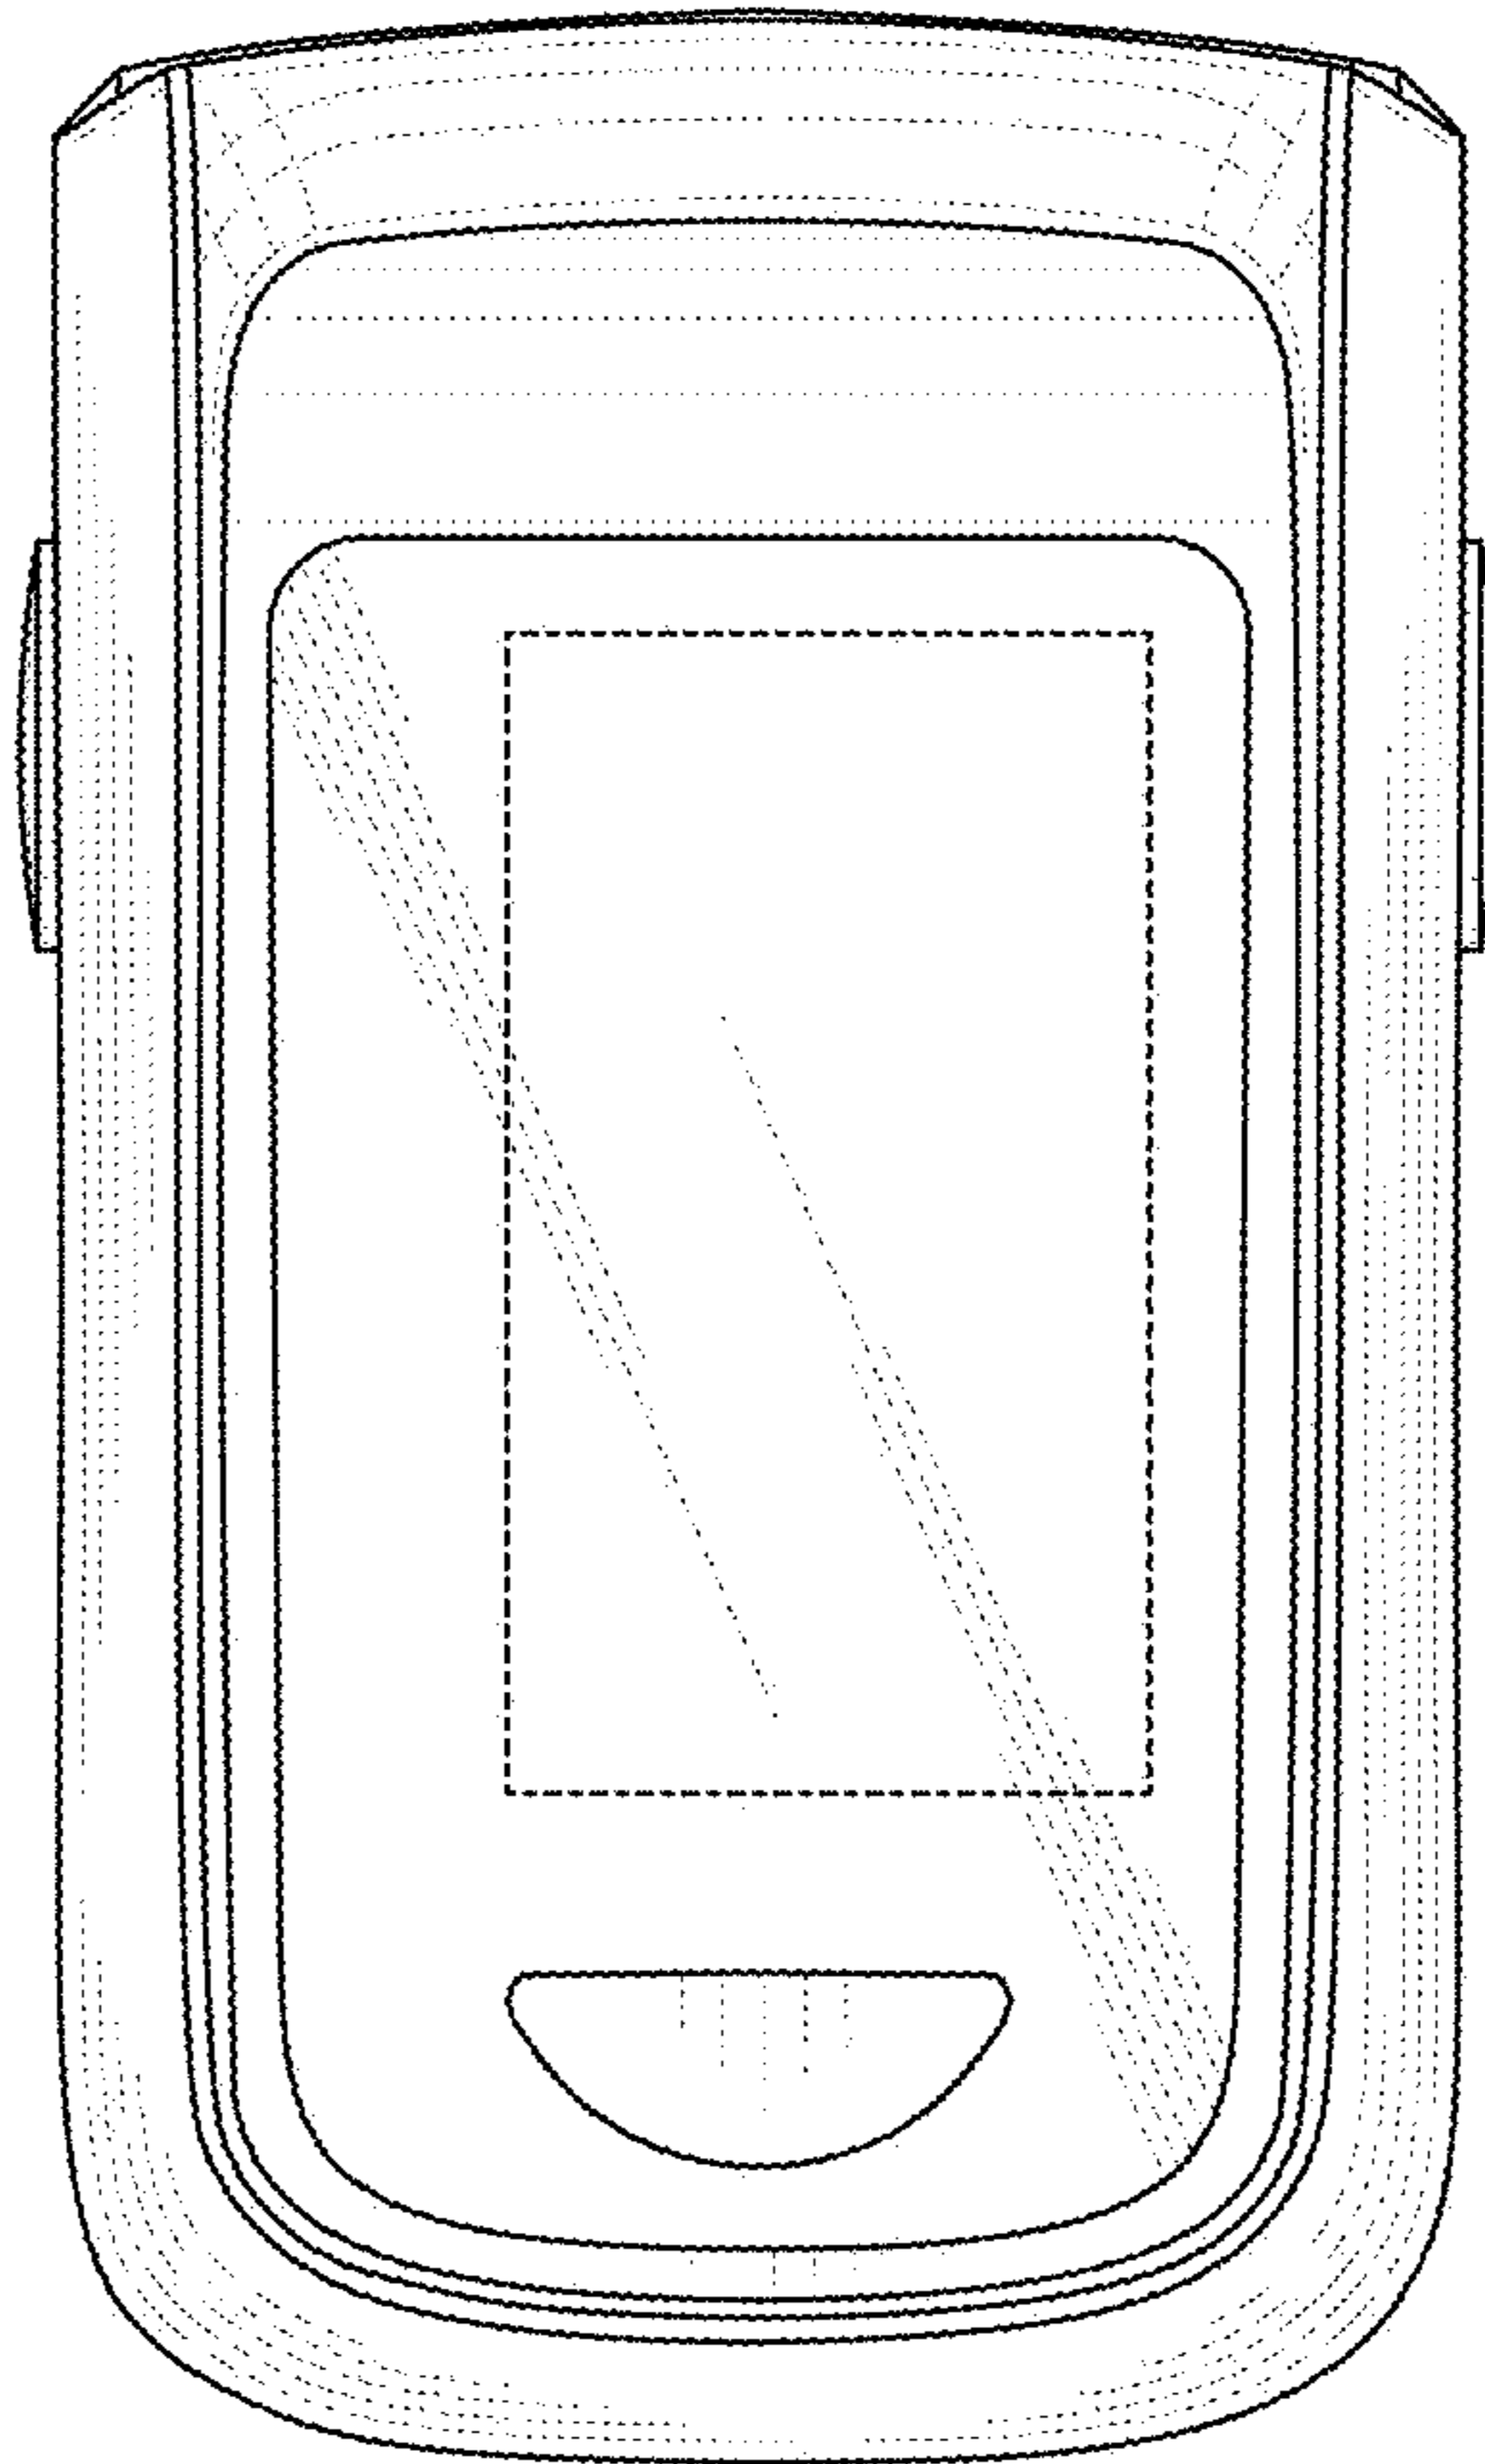


Figure 2

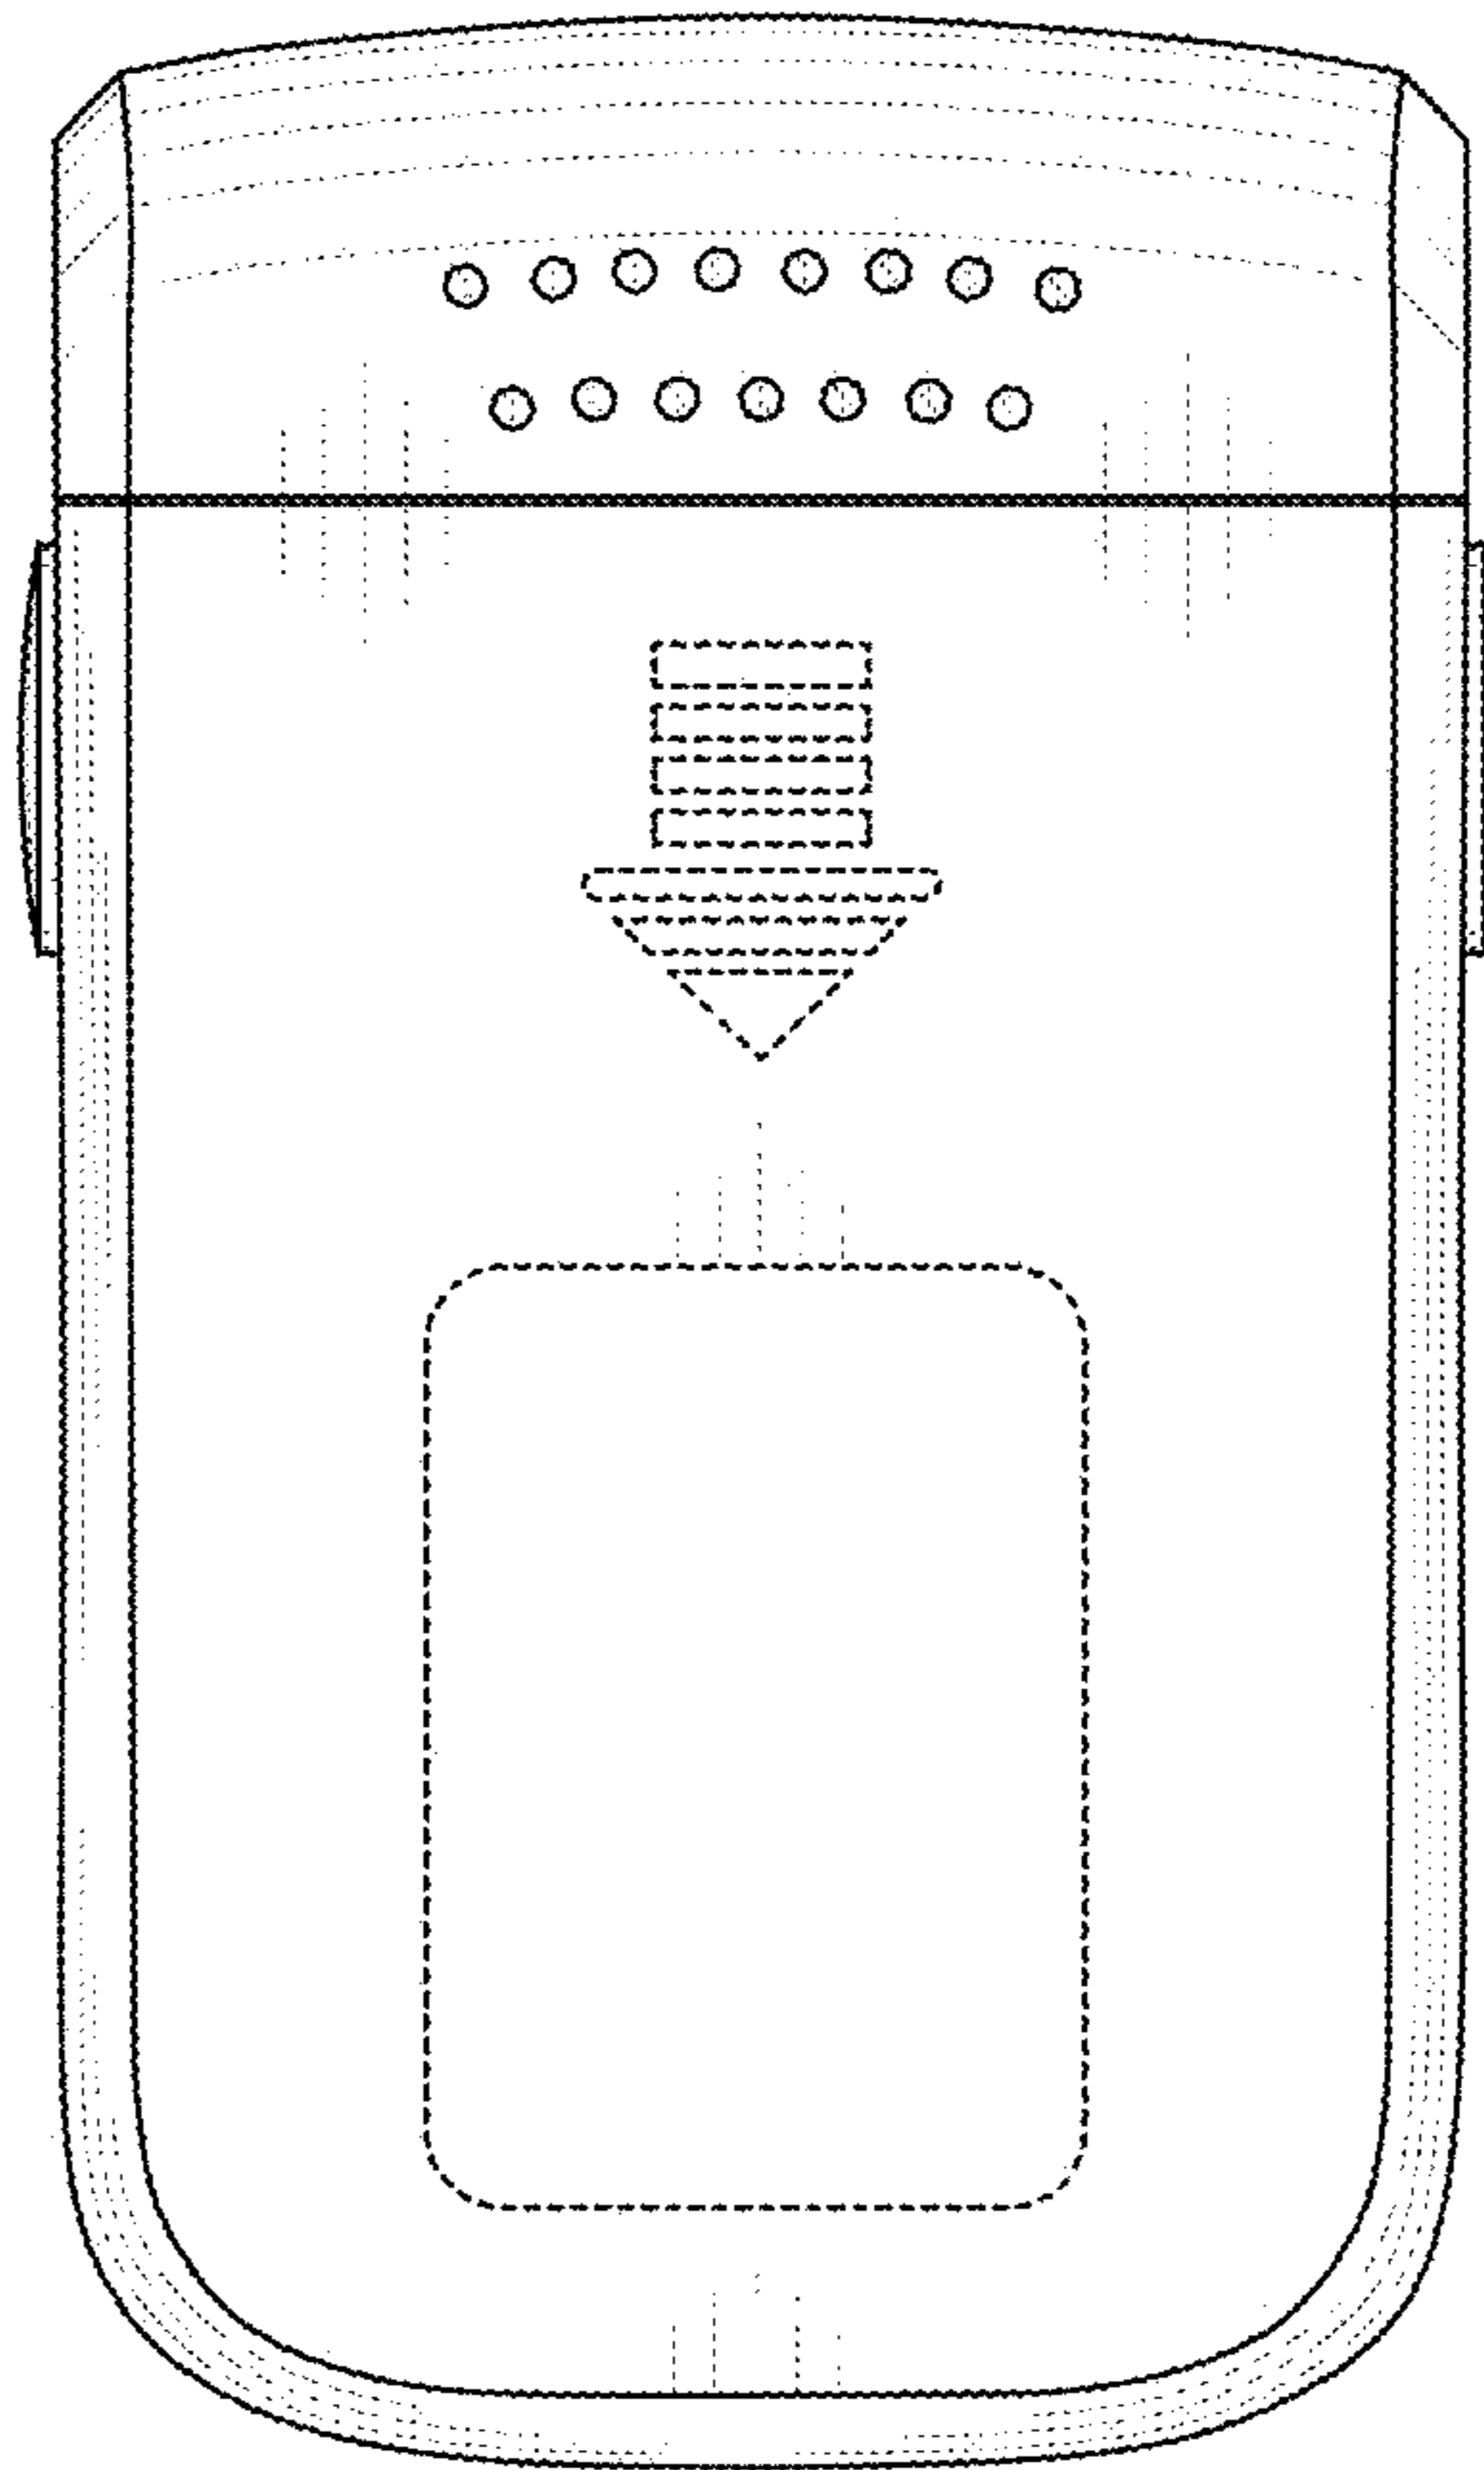


Figure 3

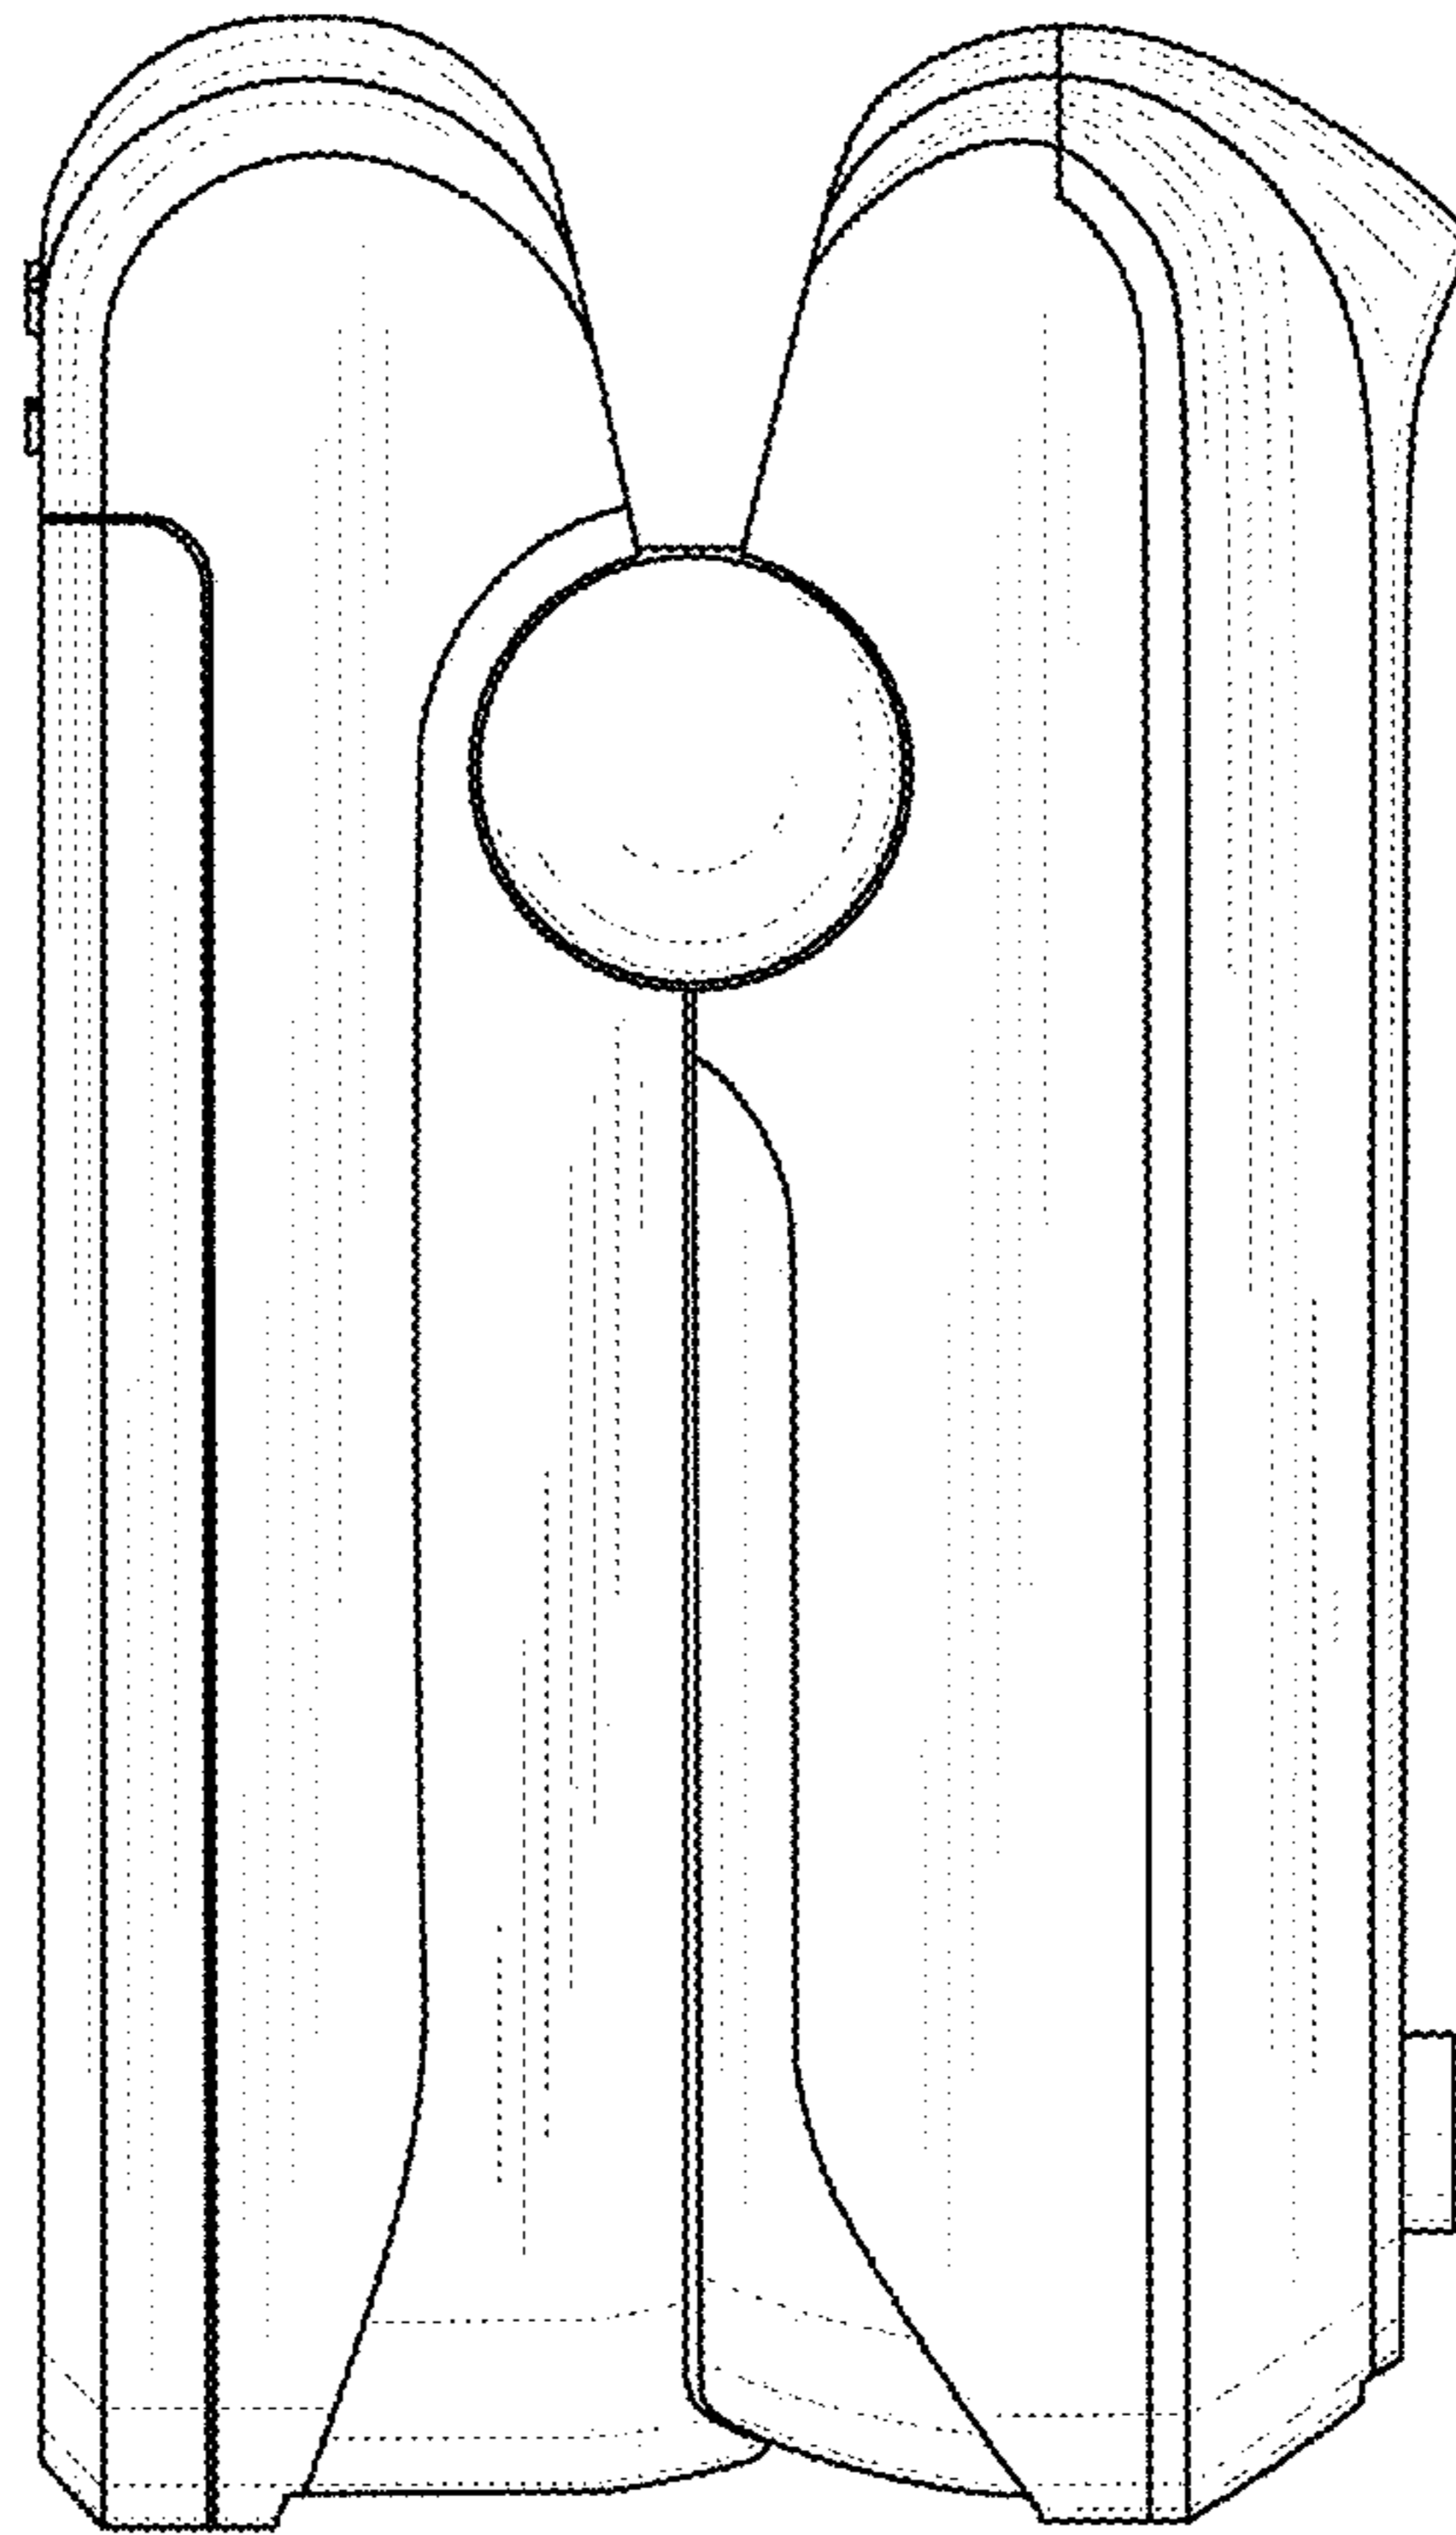


Figure 4

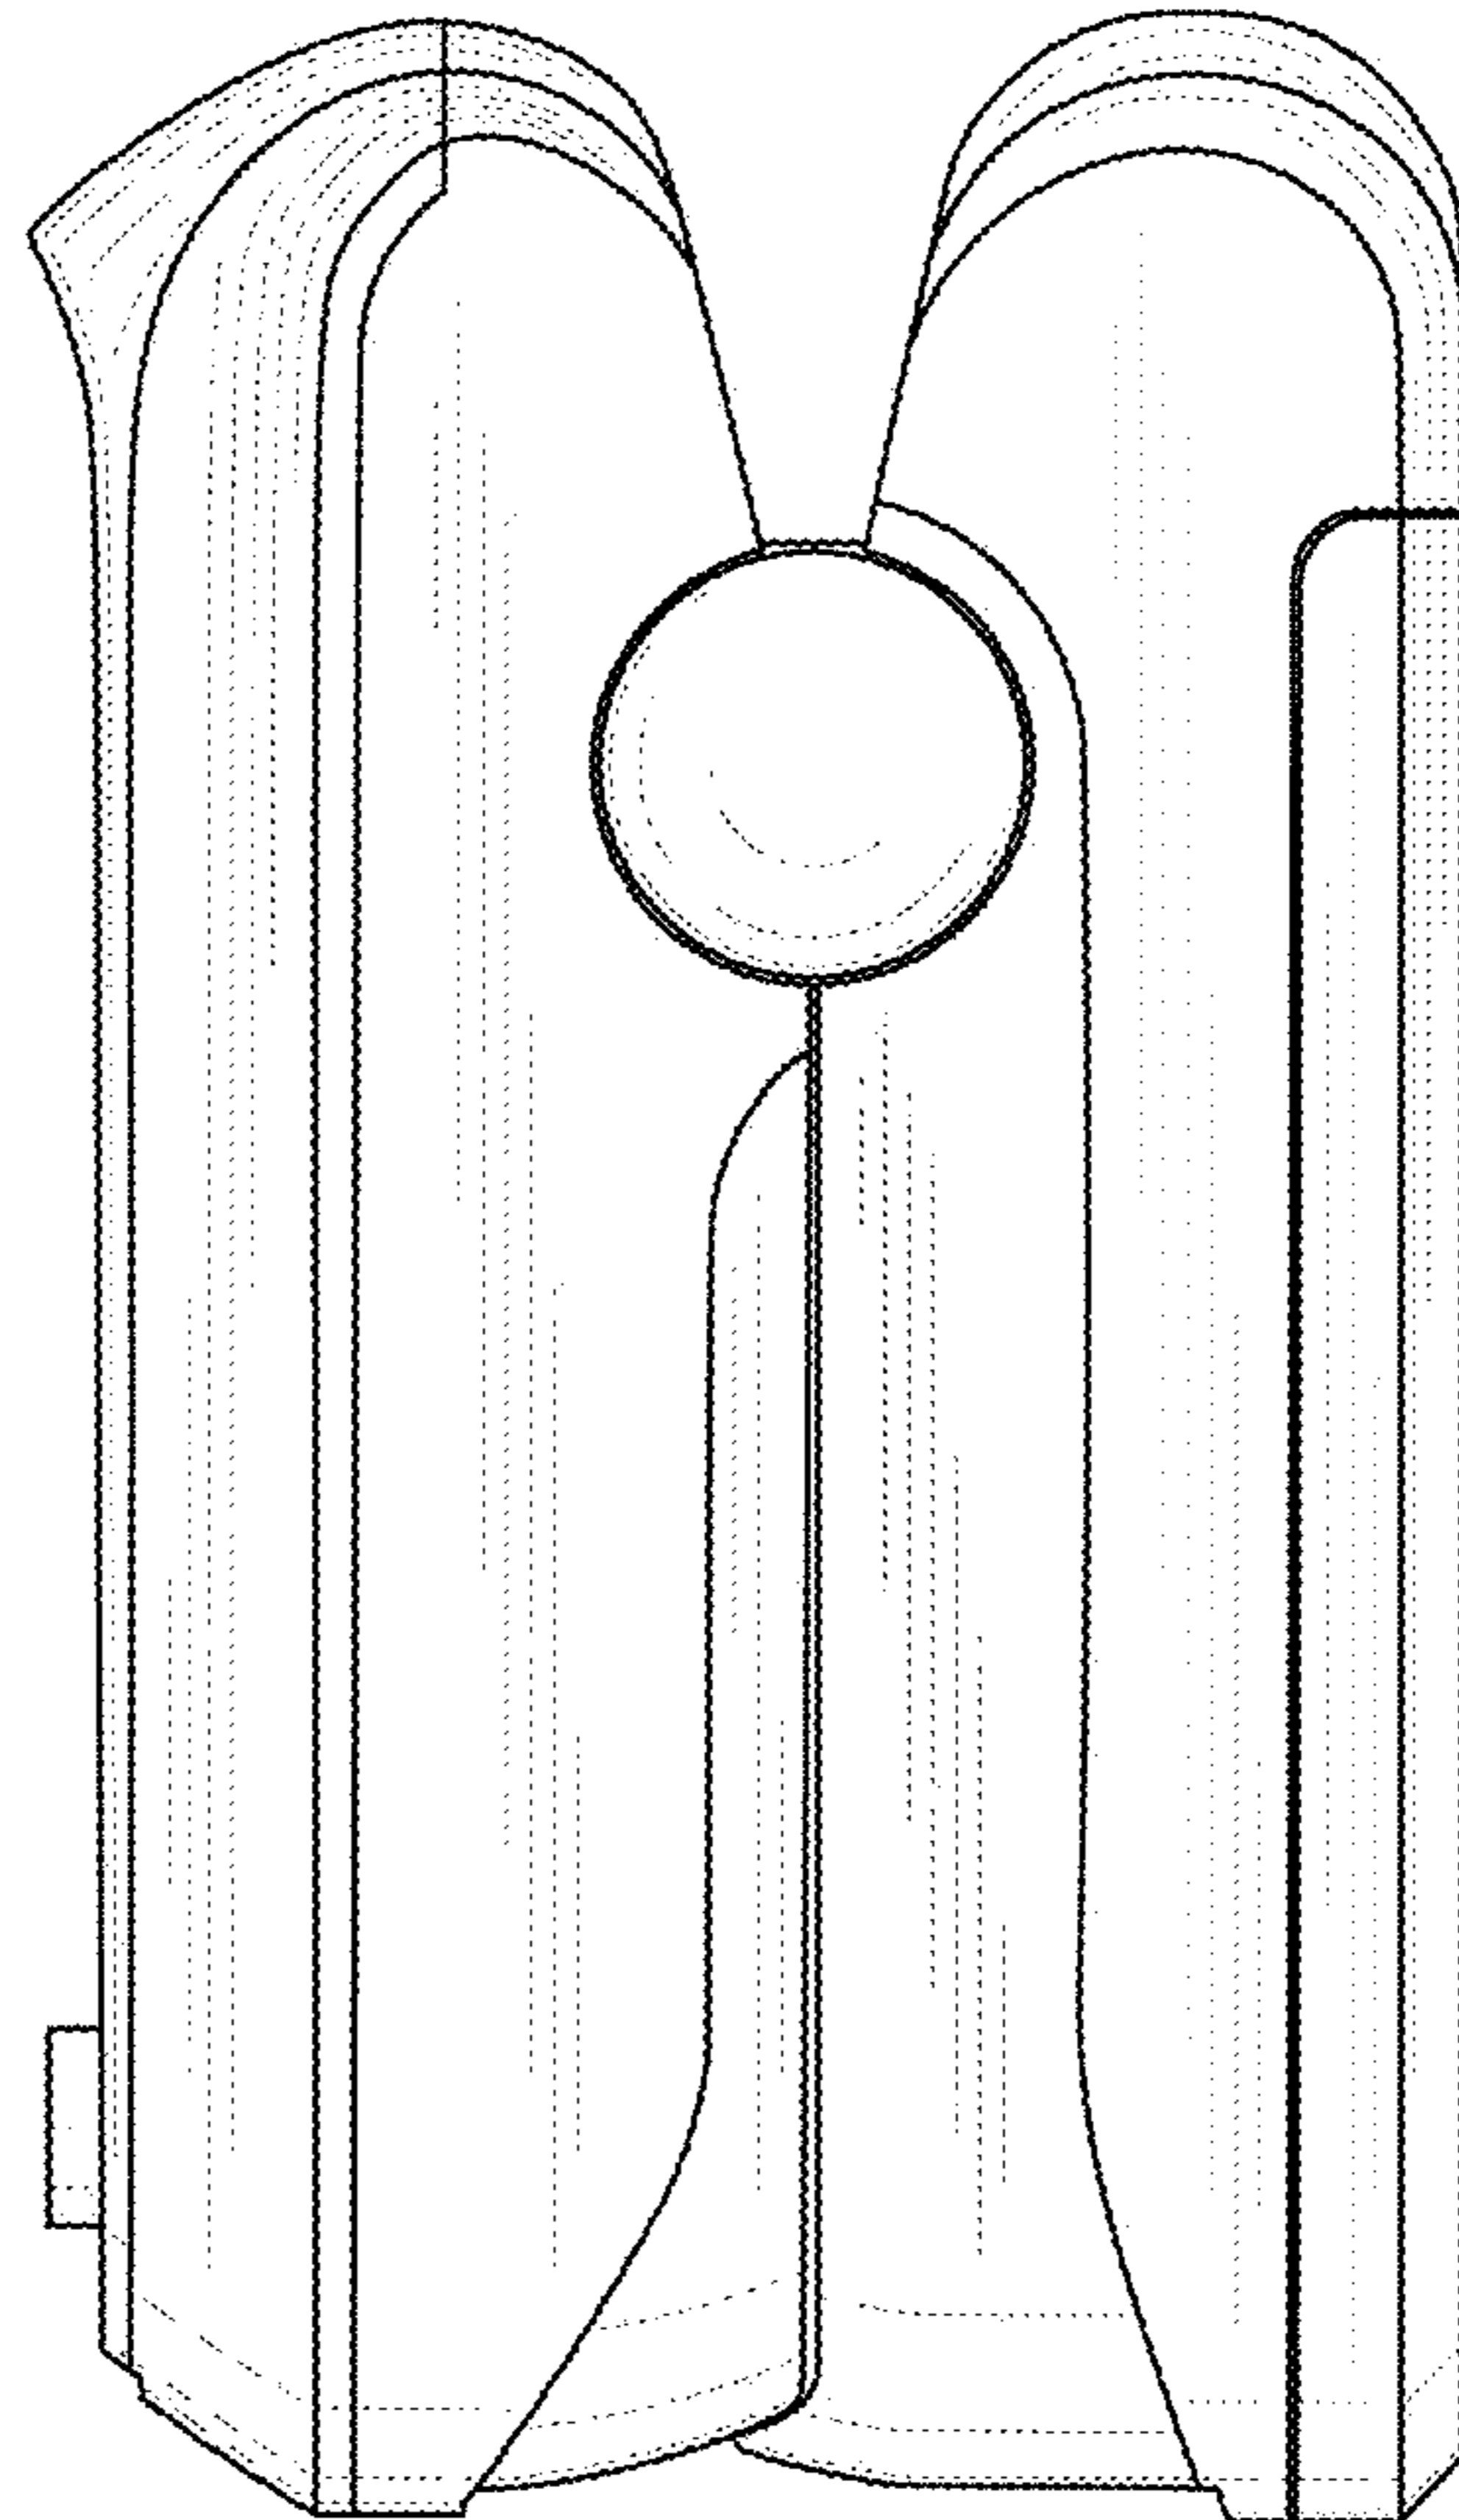


Figure 5

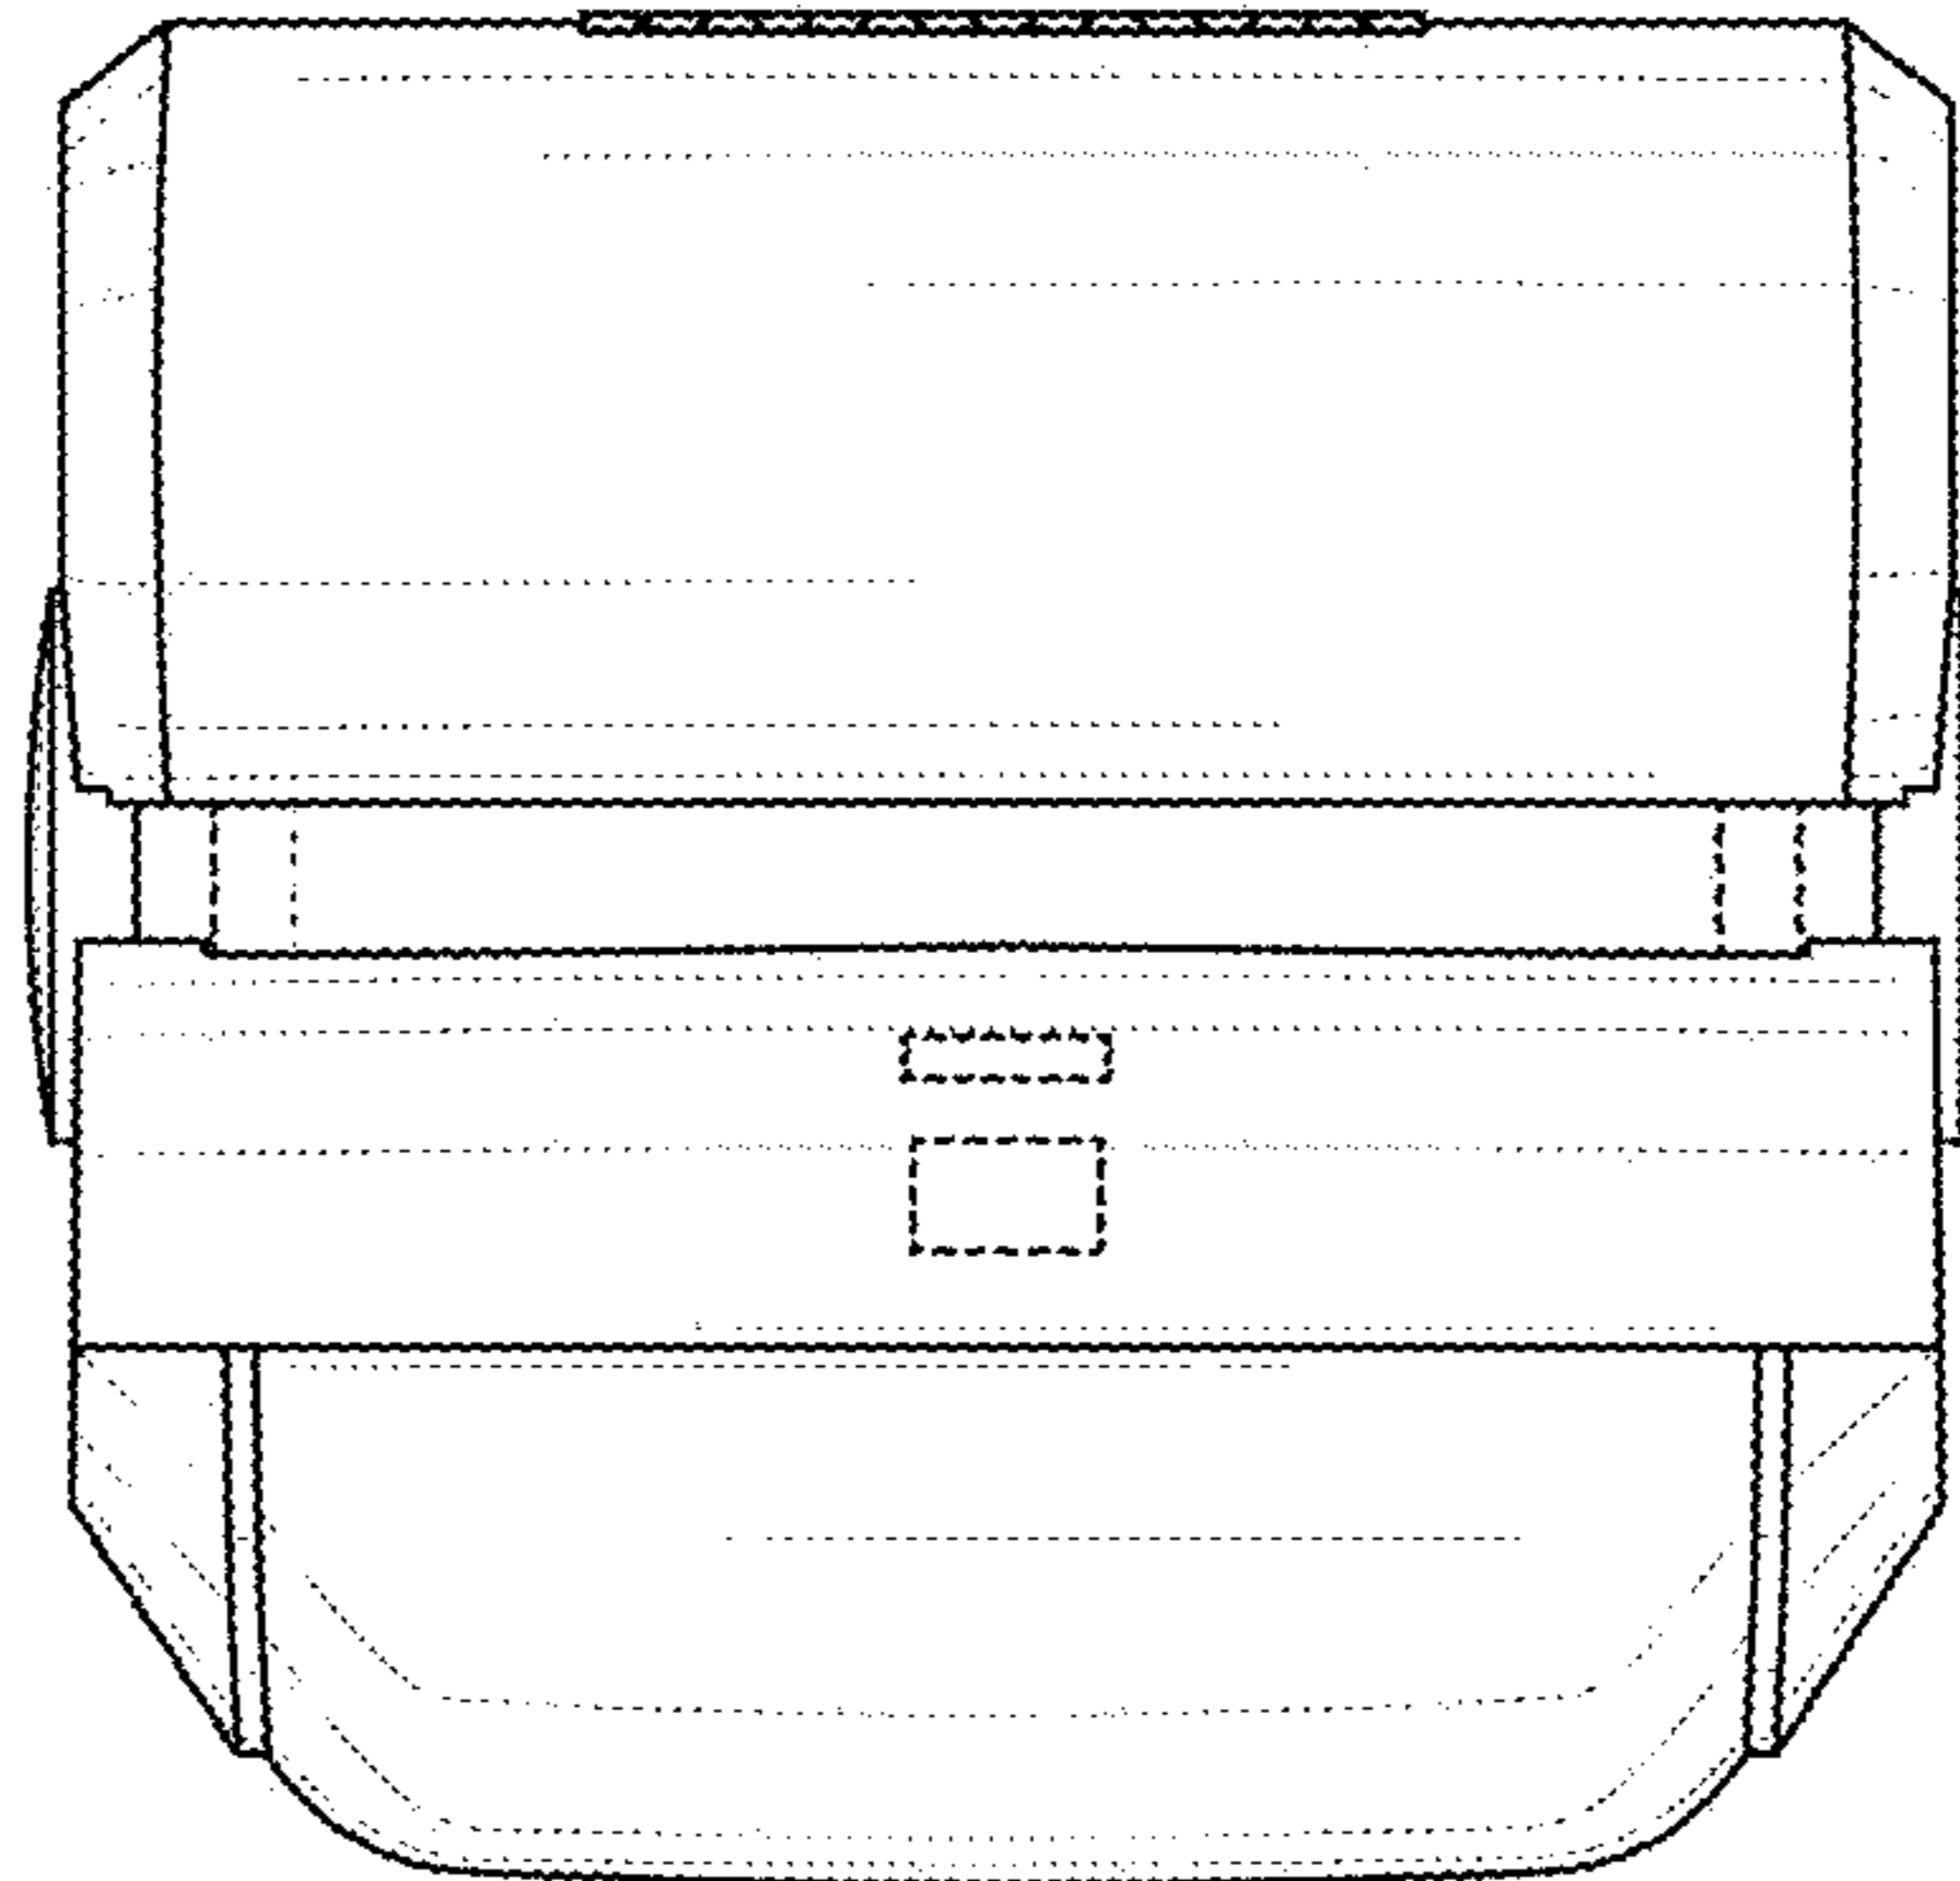


Figure 6

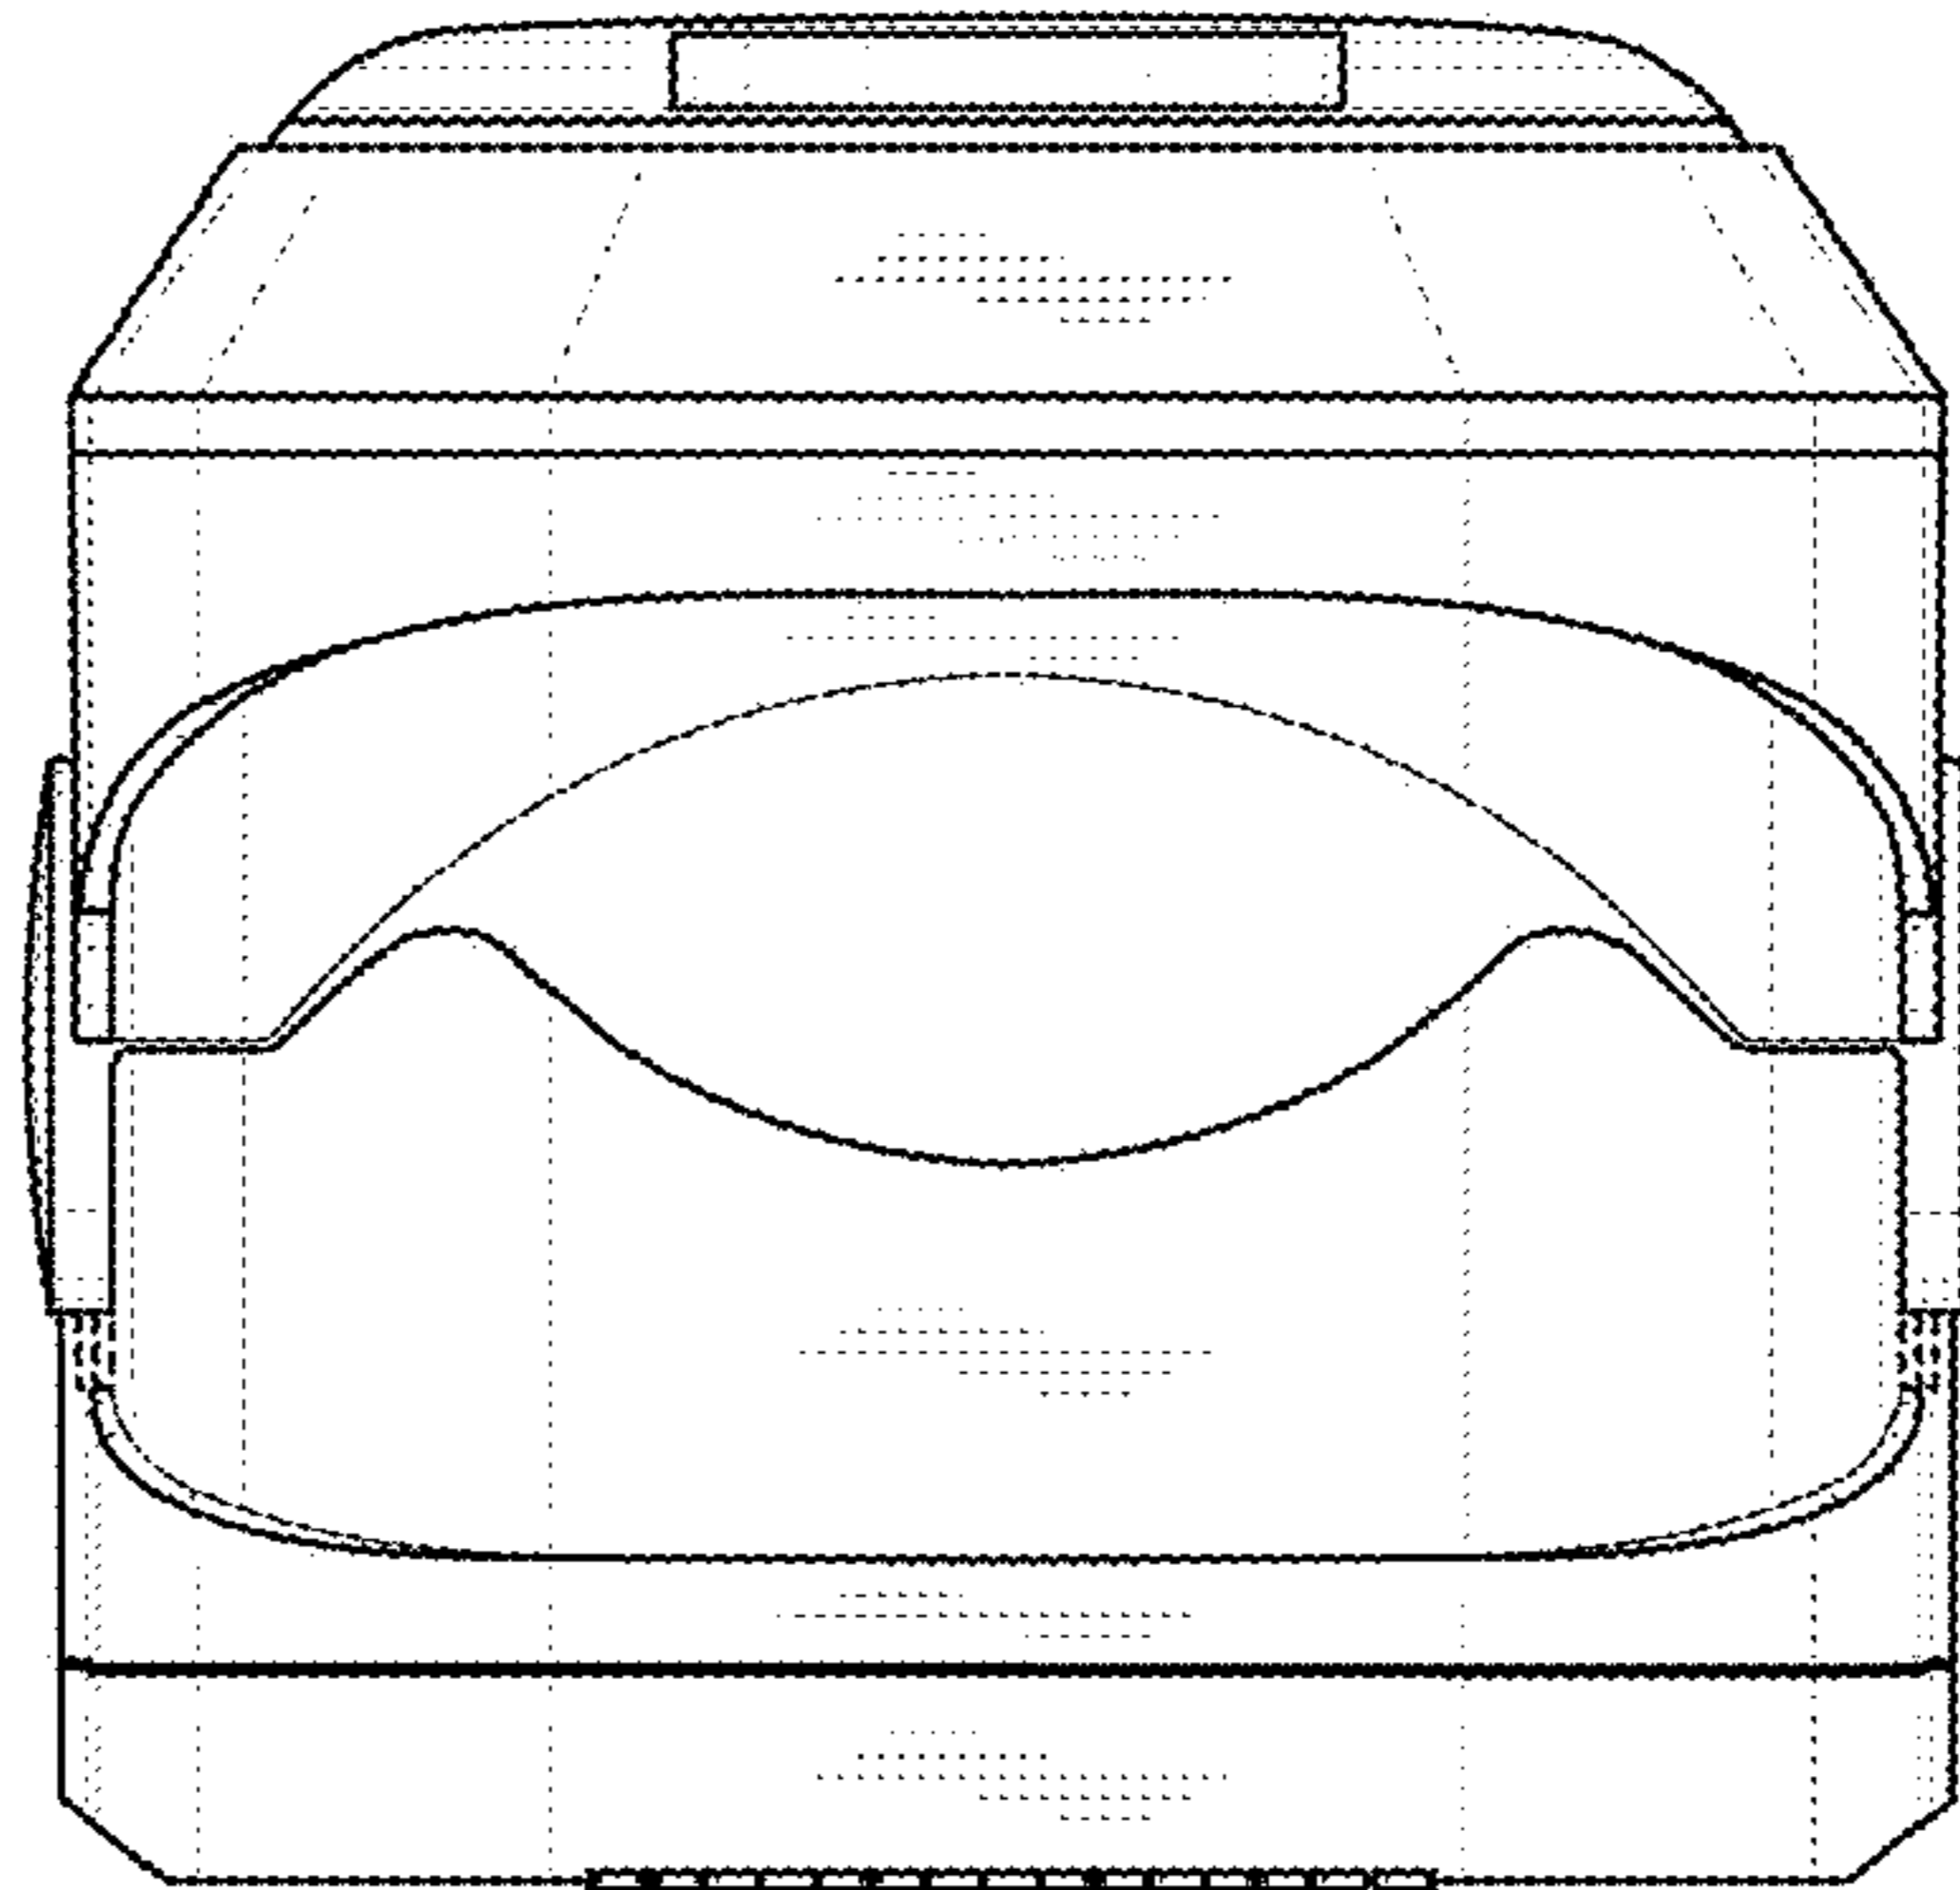


Figure 7