



US00D957660S

(12) **United States Design Patent** (10) **Patent No.:** **US D957,660 S**
Johnson et al. (45) **Date of Patent:** **** Jul. 12, 2022**

(54) **CONTROLLER FOR LIGHT THERAPY SYSTEM**

(71) Applicant: **BioPhotas, Inc.**, Anaheim, CA (US)

(72) Inventors: **Patrick Lamberth Johnson**, Santa Ana, CA (US); **Roger Allen Gibson**, Lake Forest, CA (US)

(73) Assignee: **BioPhotas, Inc.**, Anaheim, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/726,097**

(22) Filed: **Feb. 28, 2020**

(51) **LOC (13) Cl.** **28-03**

(52) **U.S. Cl.**
USPC **D24/209**

(58) **Field of Classification Search**
USPC D24/186, 187, 200, 209, 210, 110.1;
D28/9, 44; D29/108; D26/37; D13/168
CPC A61N 5/0616; A61N 2005/0647; A61N
2005/0651; A61N 2005/0652; A61N
2005/0659; A61N 2005/066; A61N
2005/067; A61B 2018/00452
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,000,752 A	3/1991	Hoskin et al.	
D337,642 S *	7/1993	Yamasaki	D24/200
6,221,095 B1	4/2001	Zuylen et al.	
6,743,249 B1	6/2004	Alden et al.	
D684,269 S *	6/2013	Wang	D24/209
D732,677 S *	6/2015	Kristensen	D24/200
D802,779 S *	11/2017	Inoue	D24/200
D858,463 S *	9/2019	Nien	D13/168
D879,053 S *	3/2020	Yu	D13/168
D879,341 S *	3/2020	Kassin	D26/37
D890,752 S *	7/2020	Huang	D14/358
D894,368 S *	8/2020	Lee	D24/107
D925,046 S *	7/2021	Johnson	D24/209

2002/0143373 A1	10/2002	Courtnage et al.
2003/0009205 A1	1/2003	Biel
2005/0110702 A1	5/2005	Aoki et al.
2006/0217690 A1	9/2006	Bastin et al.
2007/0156208 A1	7/2007	Havell et al.
2007/0208395 A1	9/2007	LeClerc et al.
2007/0217199 A1	9/2007	Adam et al.
2009/0105791 A1	4/2009	McGinnis et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO 2011/001344 A2 1/2011

OTHER PUBLICATIONS

BioPhotas Inc. Introduces the Celluma POD Light Therapy Device. May 31, 2018. Retrieved from website at: <https://www.prnewswire.com/news-releases/biophotas-inc-introduces-the-celluma-pod-light-therapy-device-300657659.html>.*

(Continued)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Robert D. Buyan; Stout, Uxa & Buyan, LLP


(57) **CLAIM**

The ornamental design for a controller for light therapy system, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a controller for light therapy system;
FIG. 2 is a top view thereof;
FIG. 3 is a bottom view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a rear view thereof; and,
FIG. 7 is a front view thereof.
The broken lines show portions of the controller for light therapy system that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

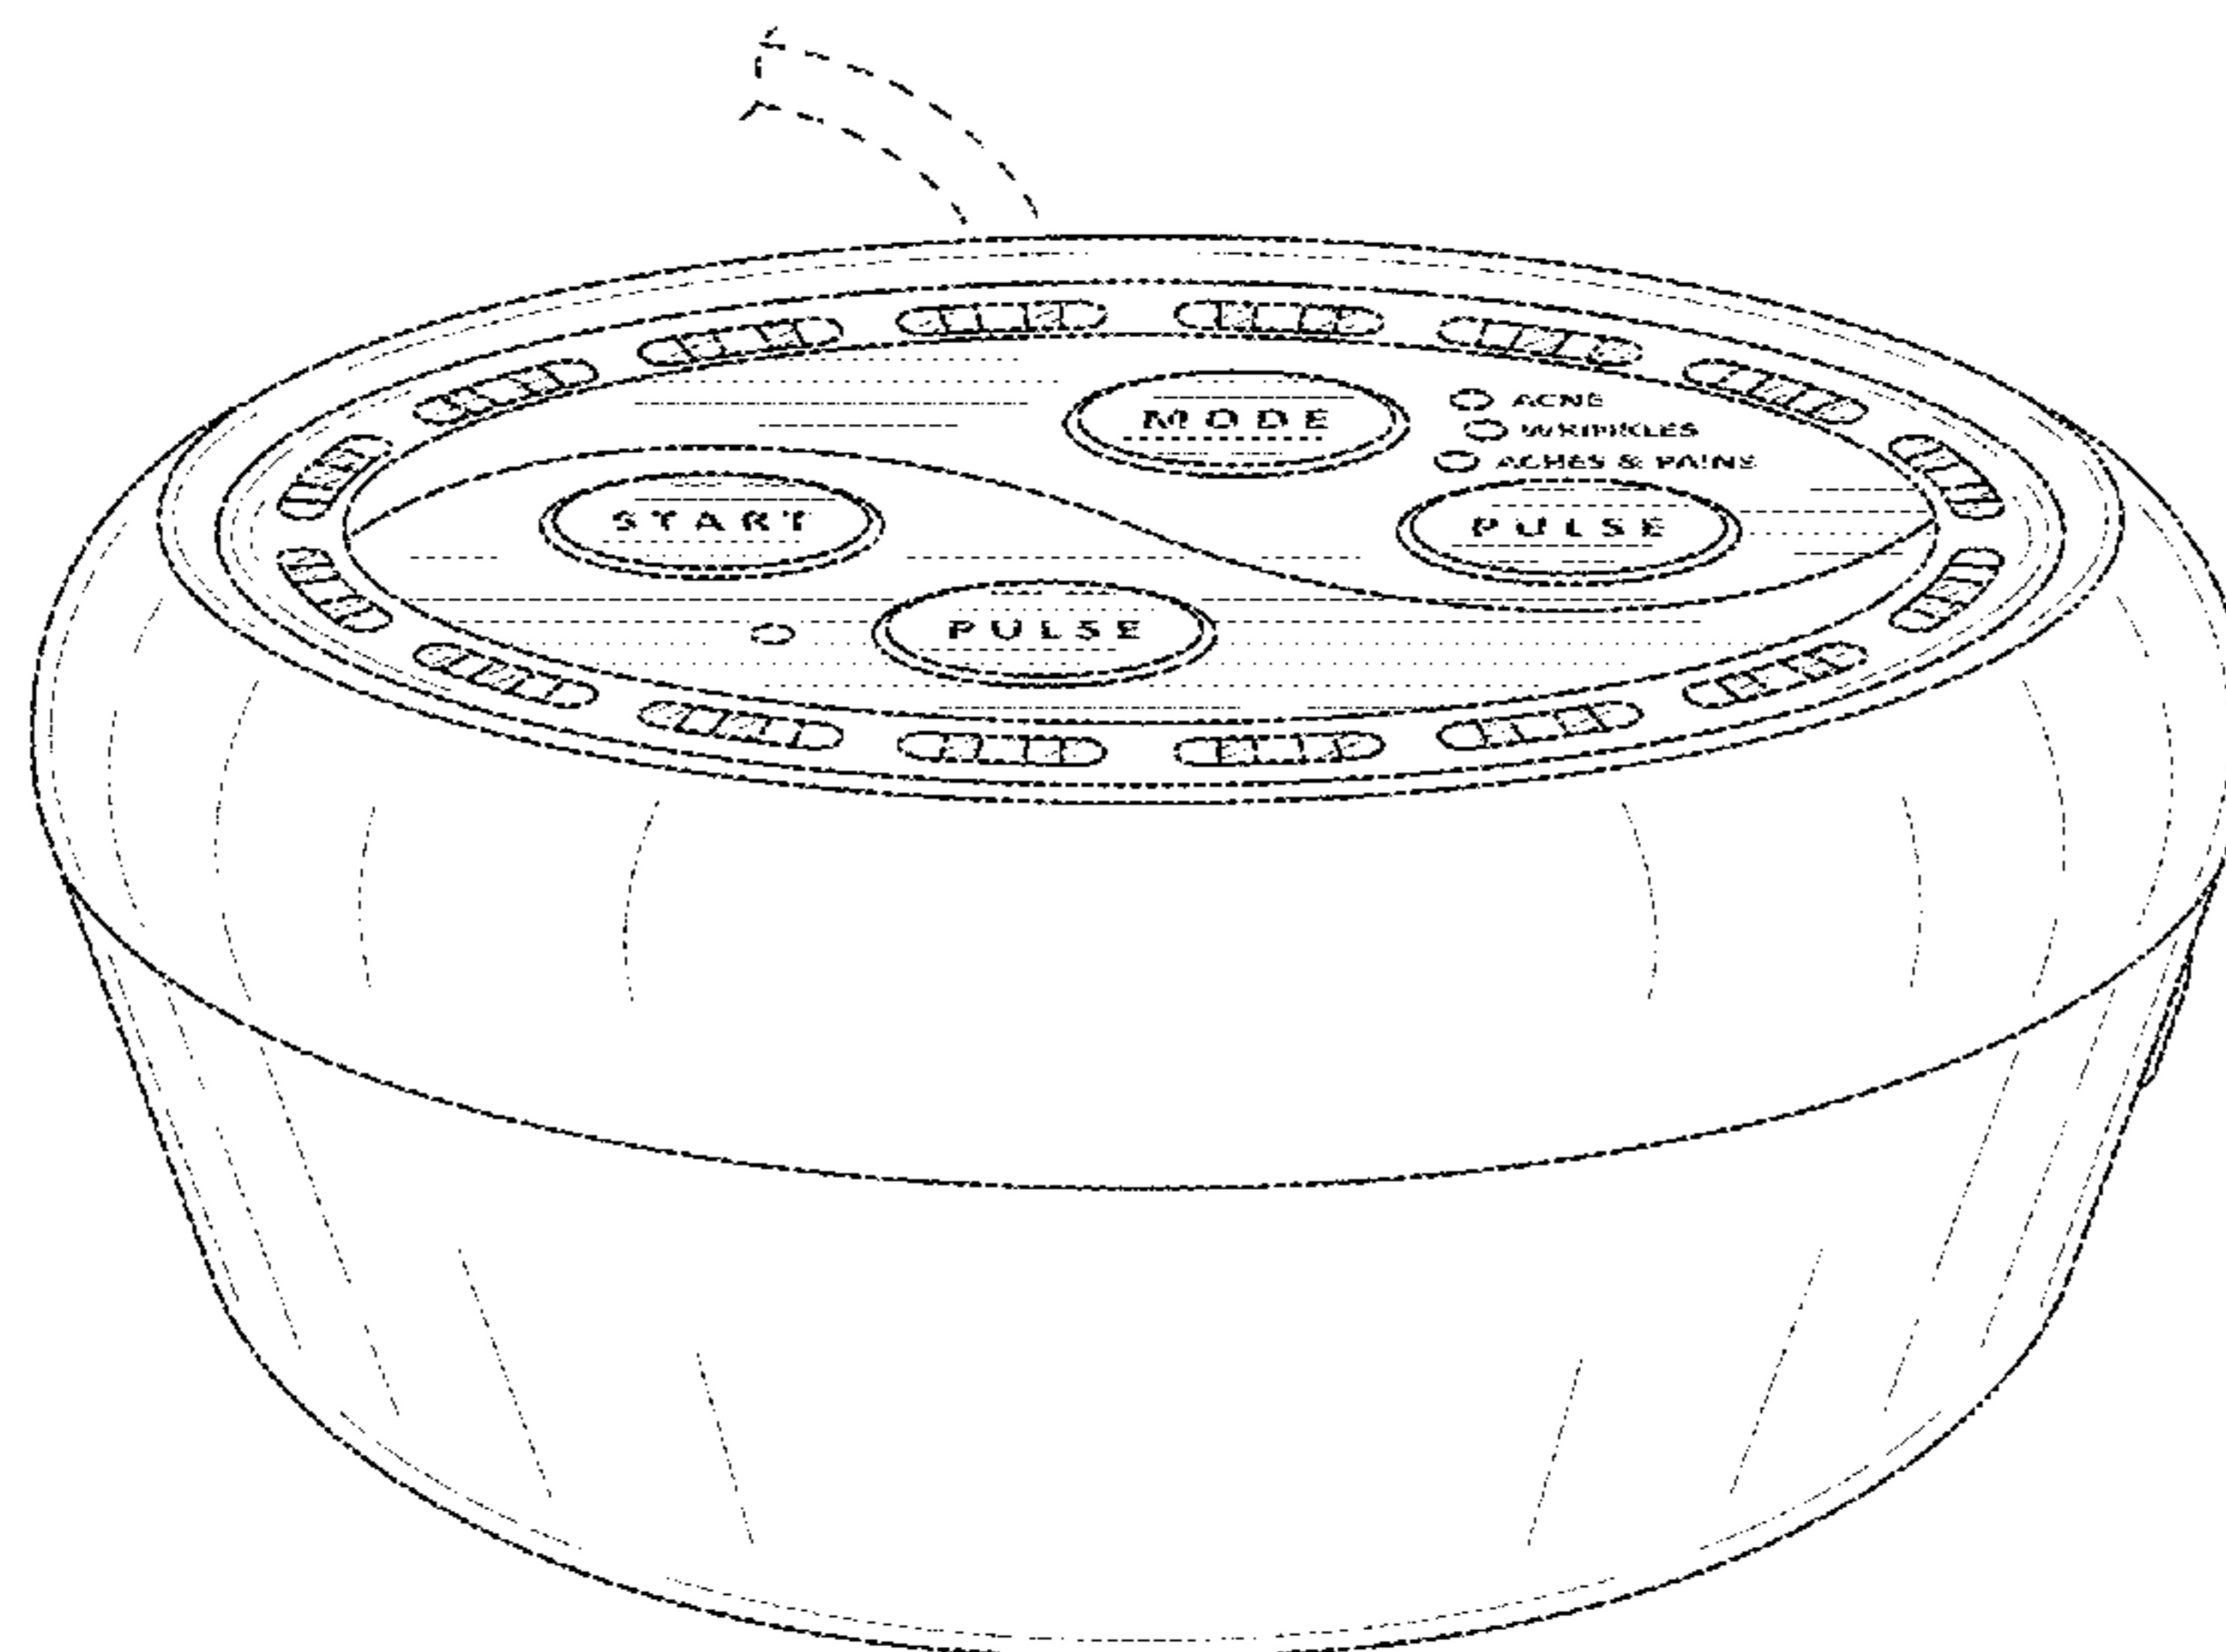

(56)

References Cited

U.S. PATENT DOCUMENTS

2010/0114007 A1 5/2010 Fischer et al.
2010/0234927 A1 9/2010 Lin
2010/0274329 A1 10/2010 Bradley et al.
2010/0318161 A1 12/2010 Brawn
2011/0144724 A1 6/2011 Pryor et al.
2011/0144727 A1 6/2011 Benedict
2013/0274839 A1* 10/2013 Johnson A61N 5/0616
607/90

OTHER PUBLICATIONS

International Search Report and Written Opinion for related PCT application PCT/US2012/064198. International filing date Nov. 8, 2012.

Daniel Barolet, M.D. "Light-Emitting Diodes (LEDs) in Dermatology", *Seminars in Cutaneous Medicine and Surgery*, vol. 27, pp. 227-238, 2008.

Daniel Barolet, et al., Importance of Pulsing Illumination Parameters in Low-Level-Light Therapy, *Journal of Biomedical Optics*, vol. 15, No. 4, pp. 048005-1-048005-8, 2010.

Supplementary European Search Report dated Jul. 23, 2015 for related European Application No. 12847625.6.

* cited by examiner

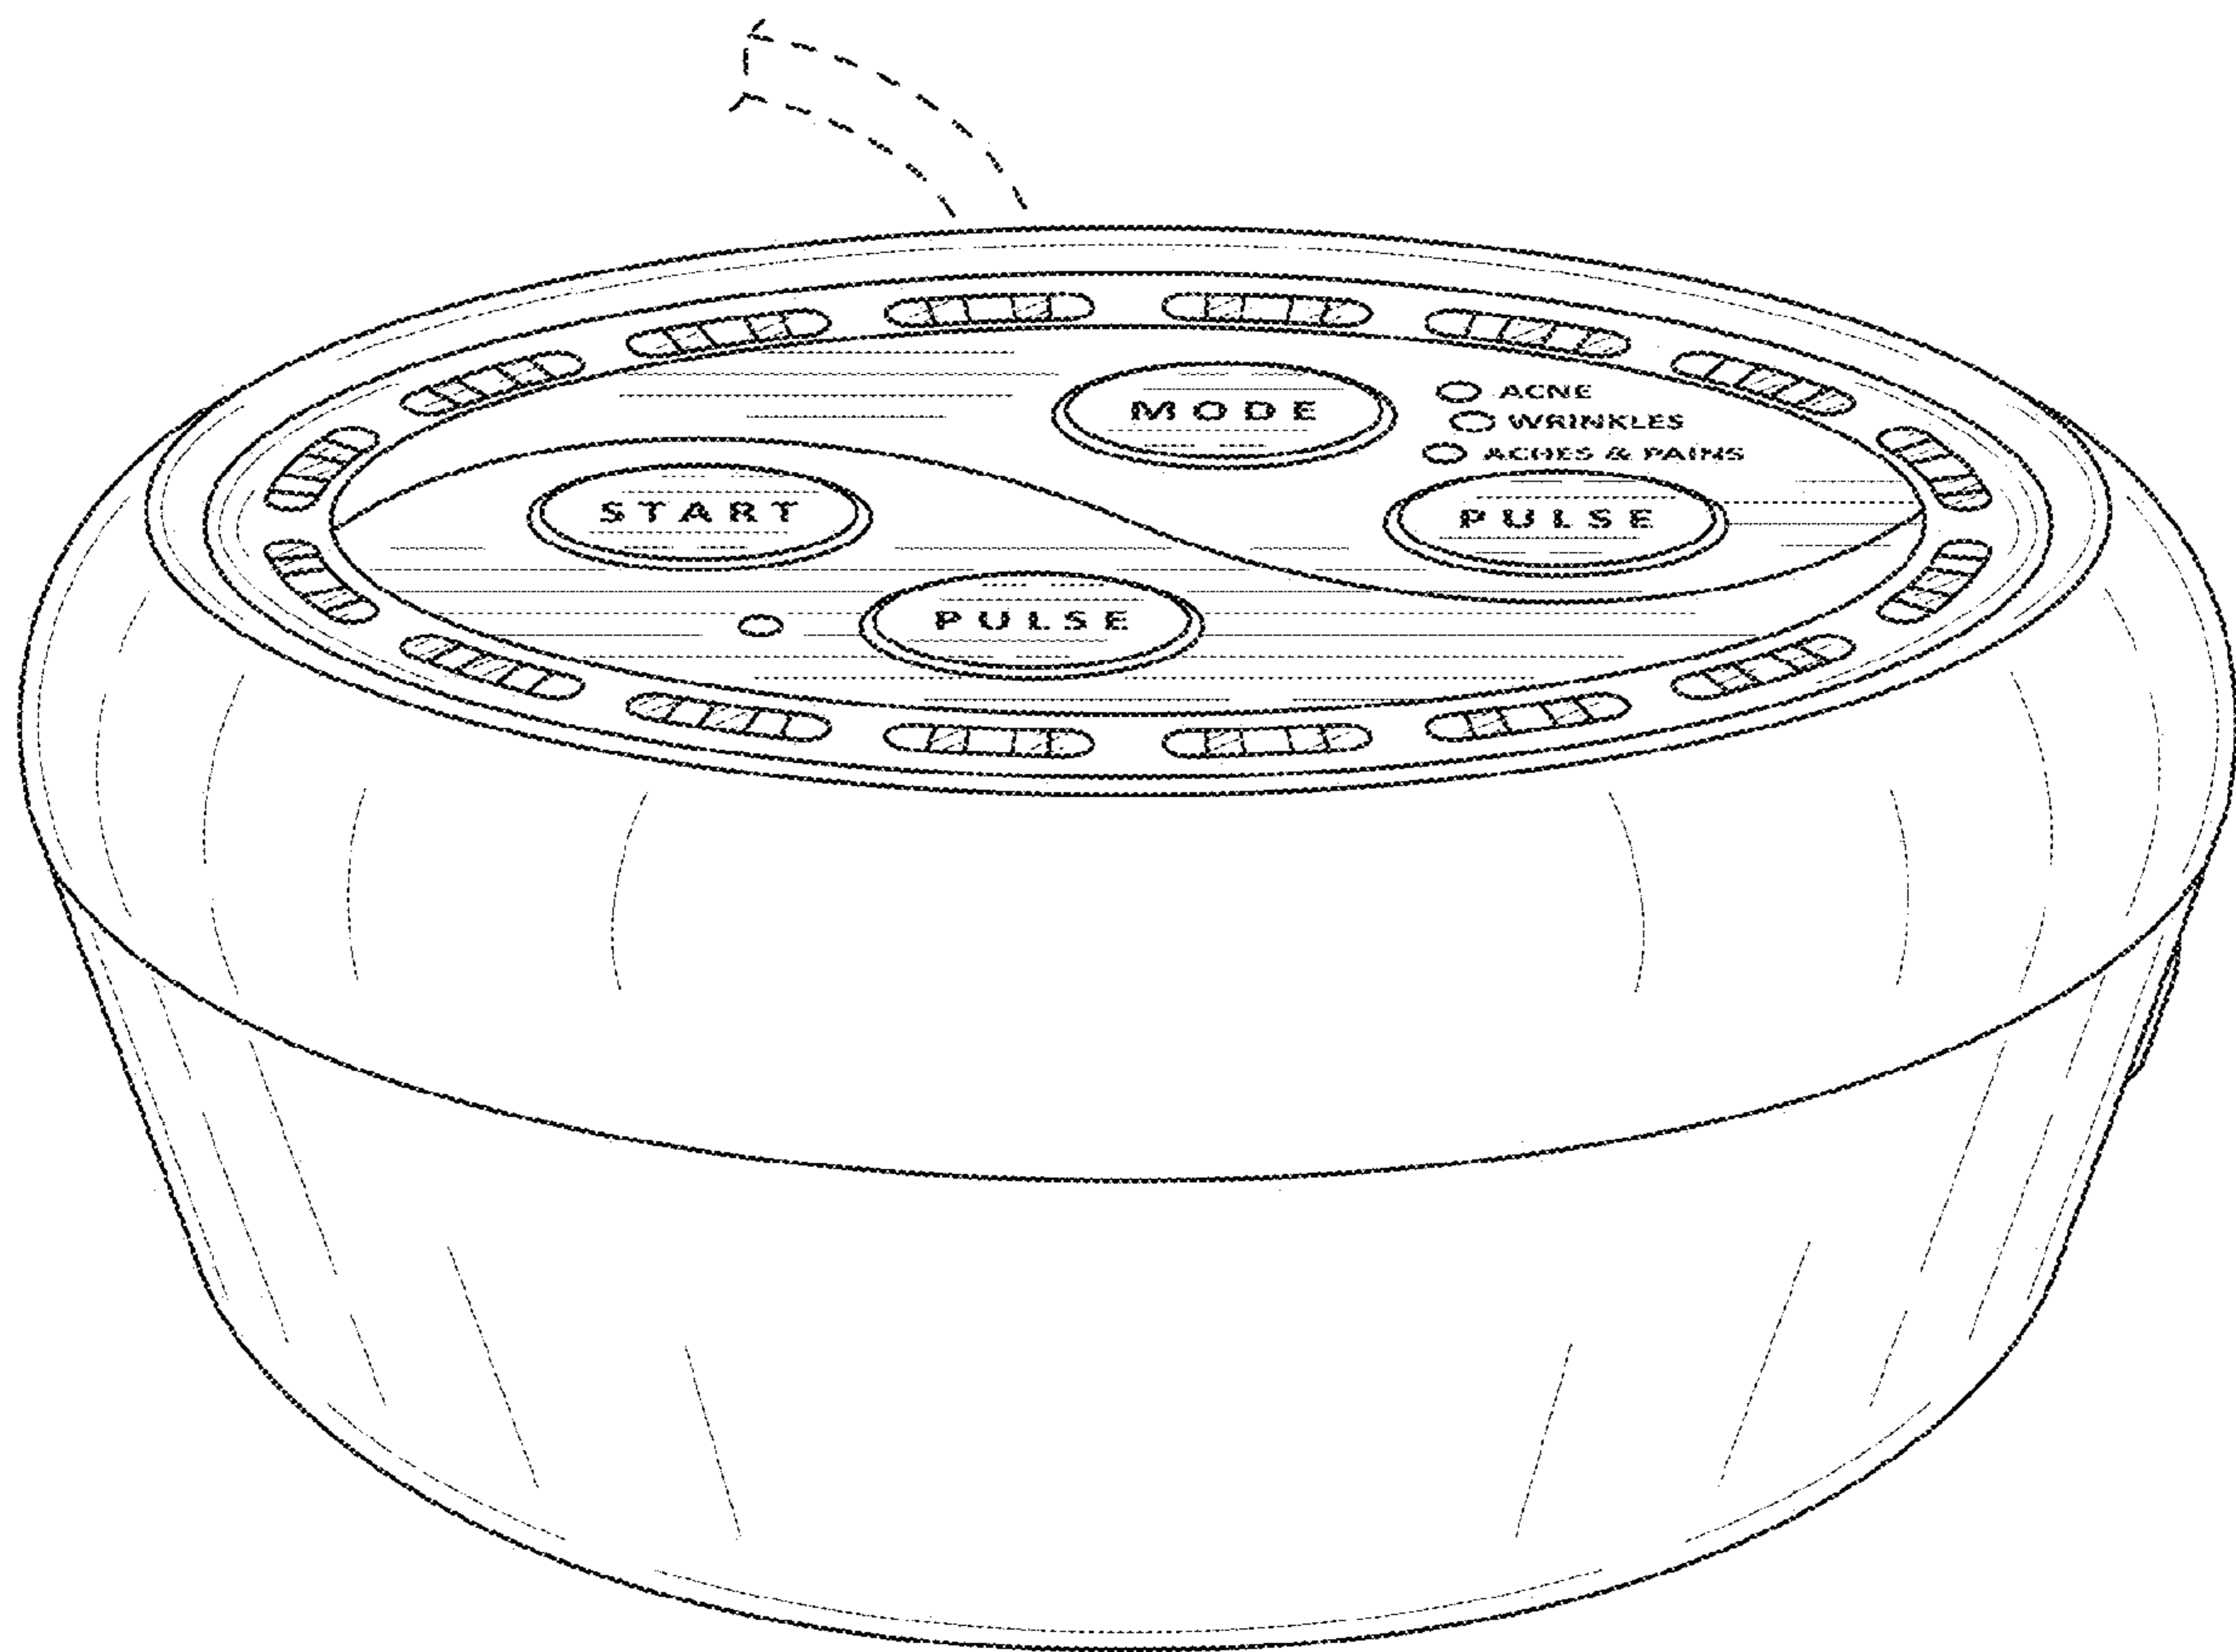


FIG. 1

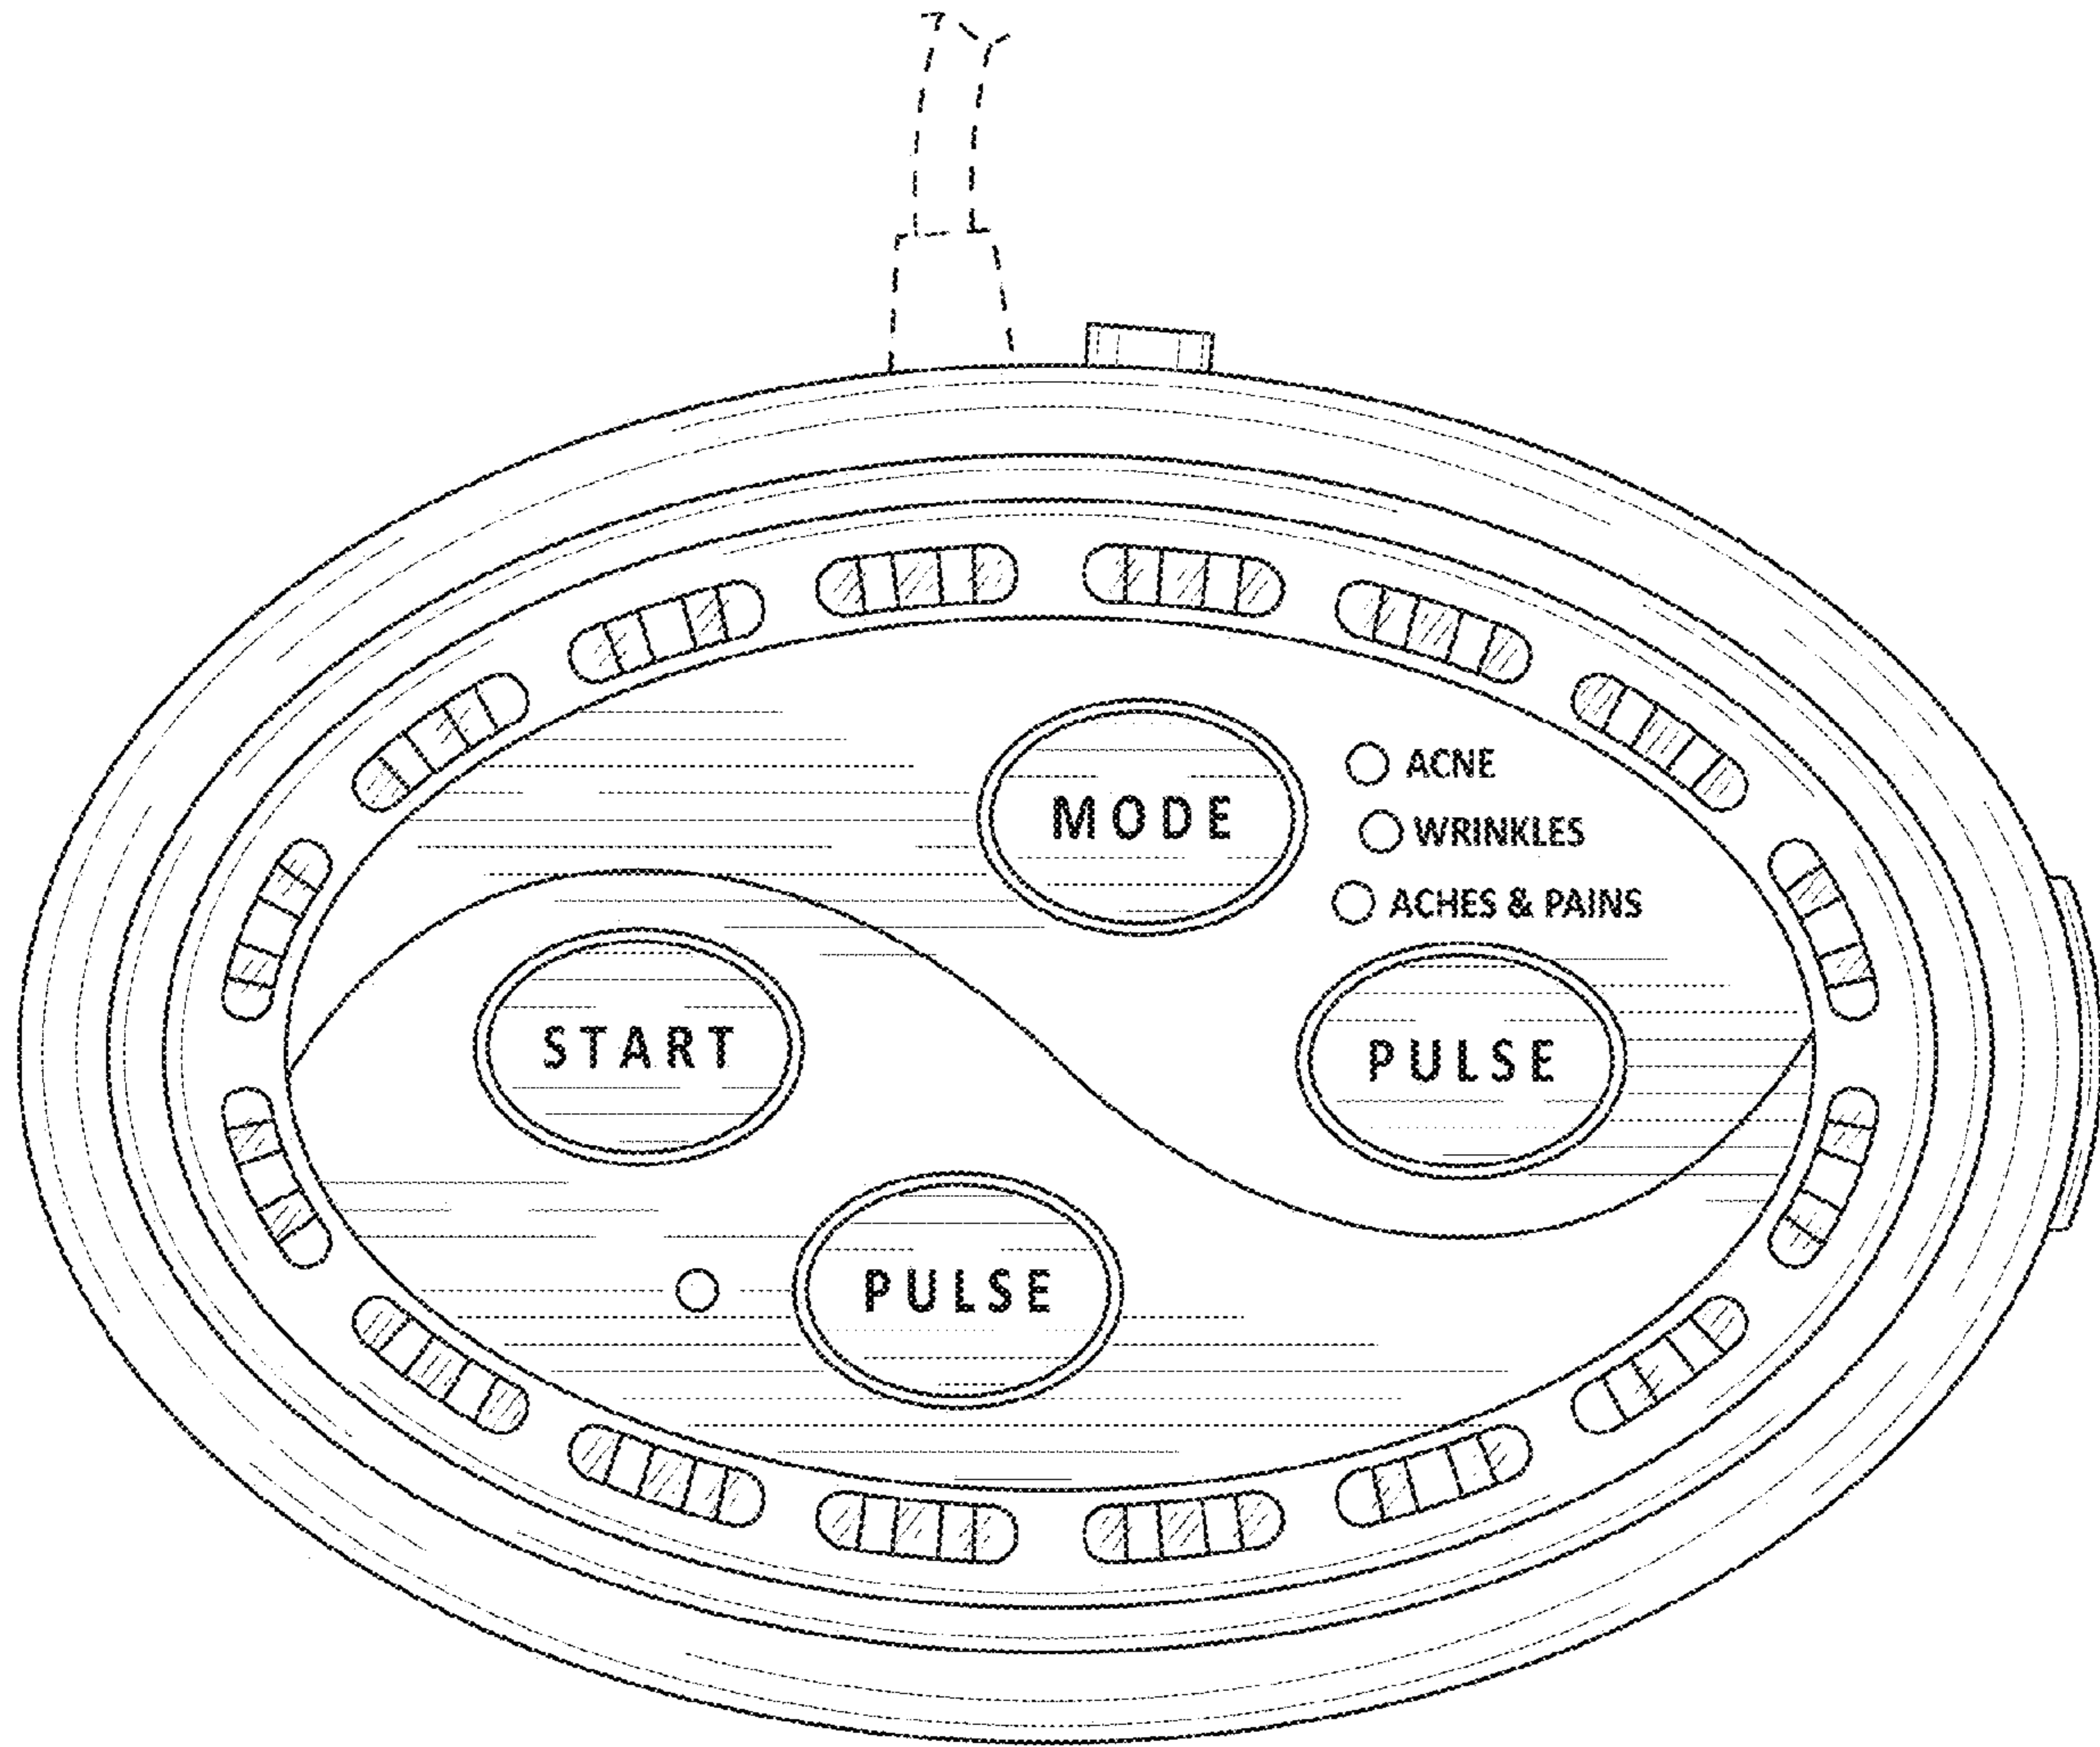


FIG. 2

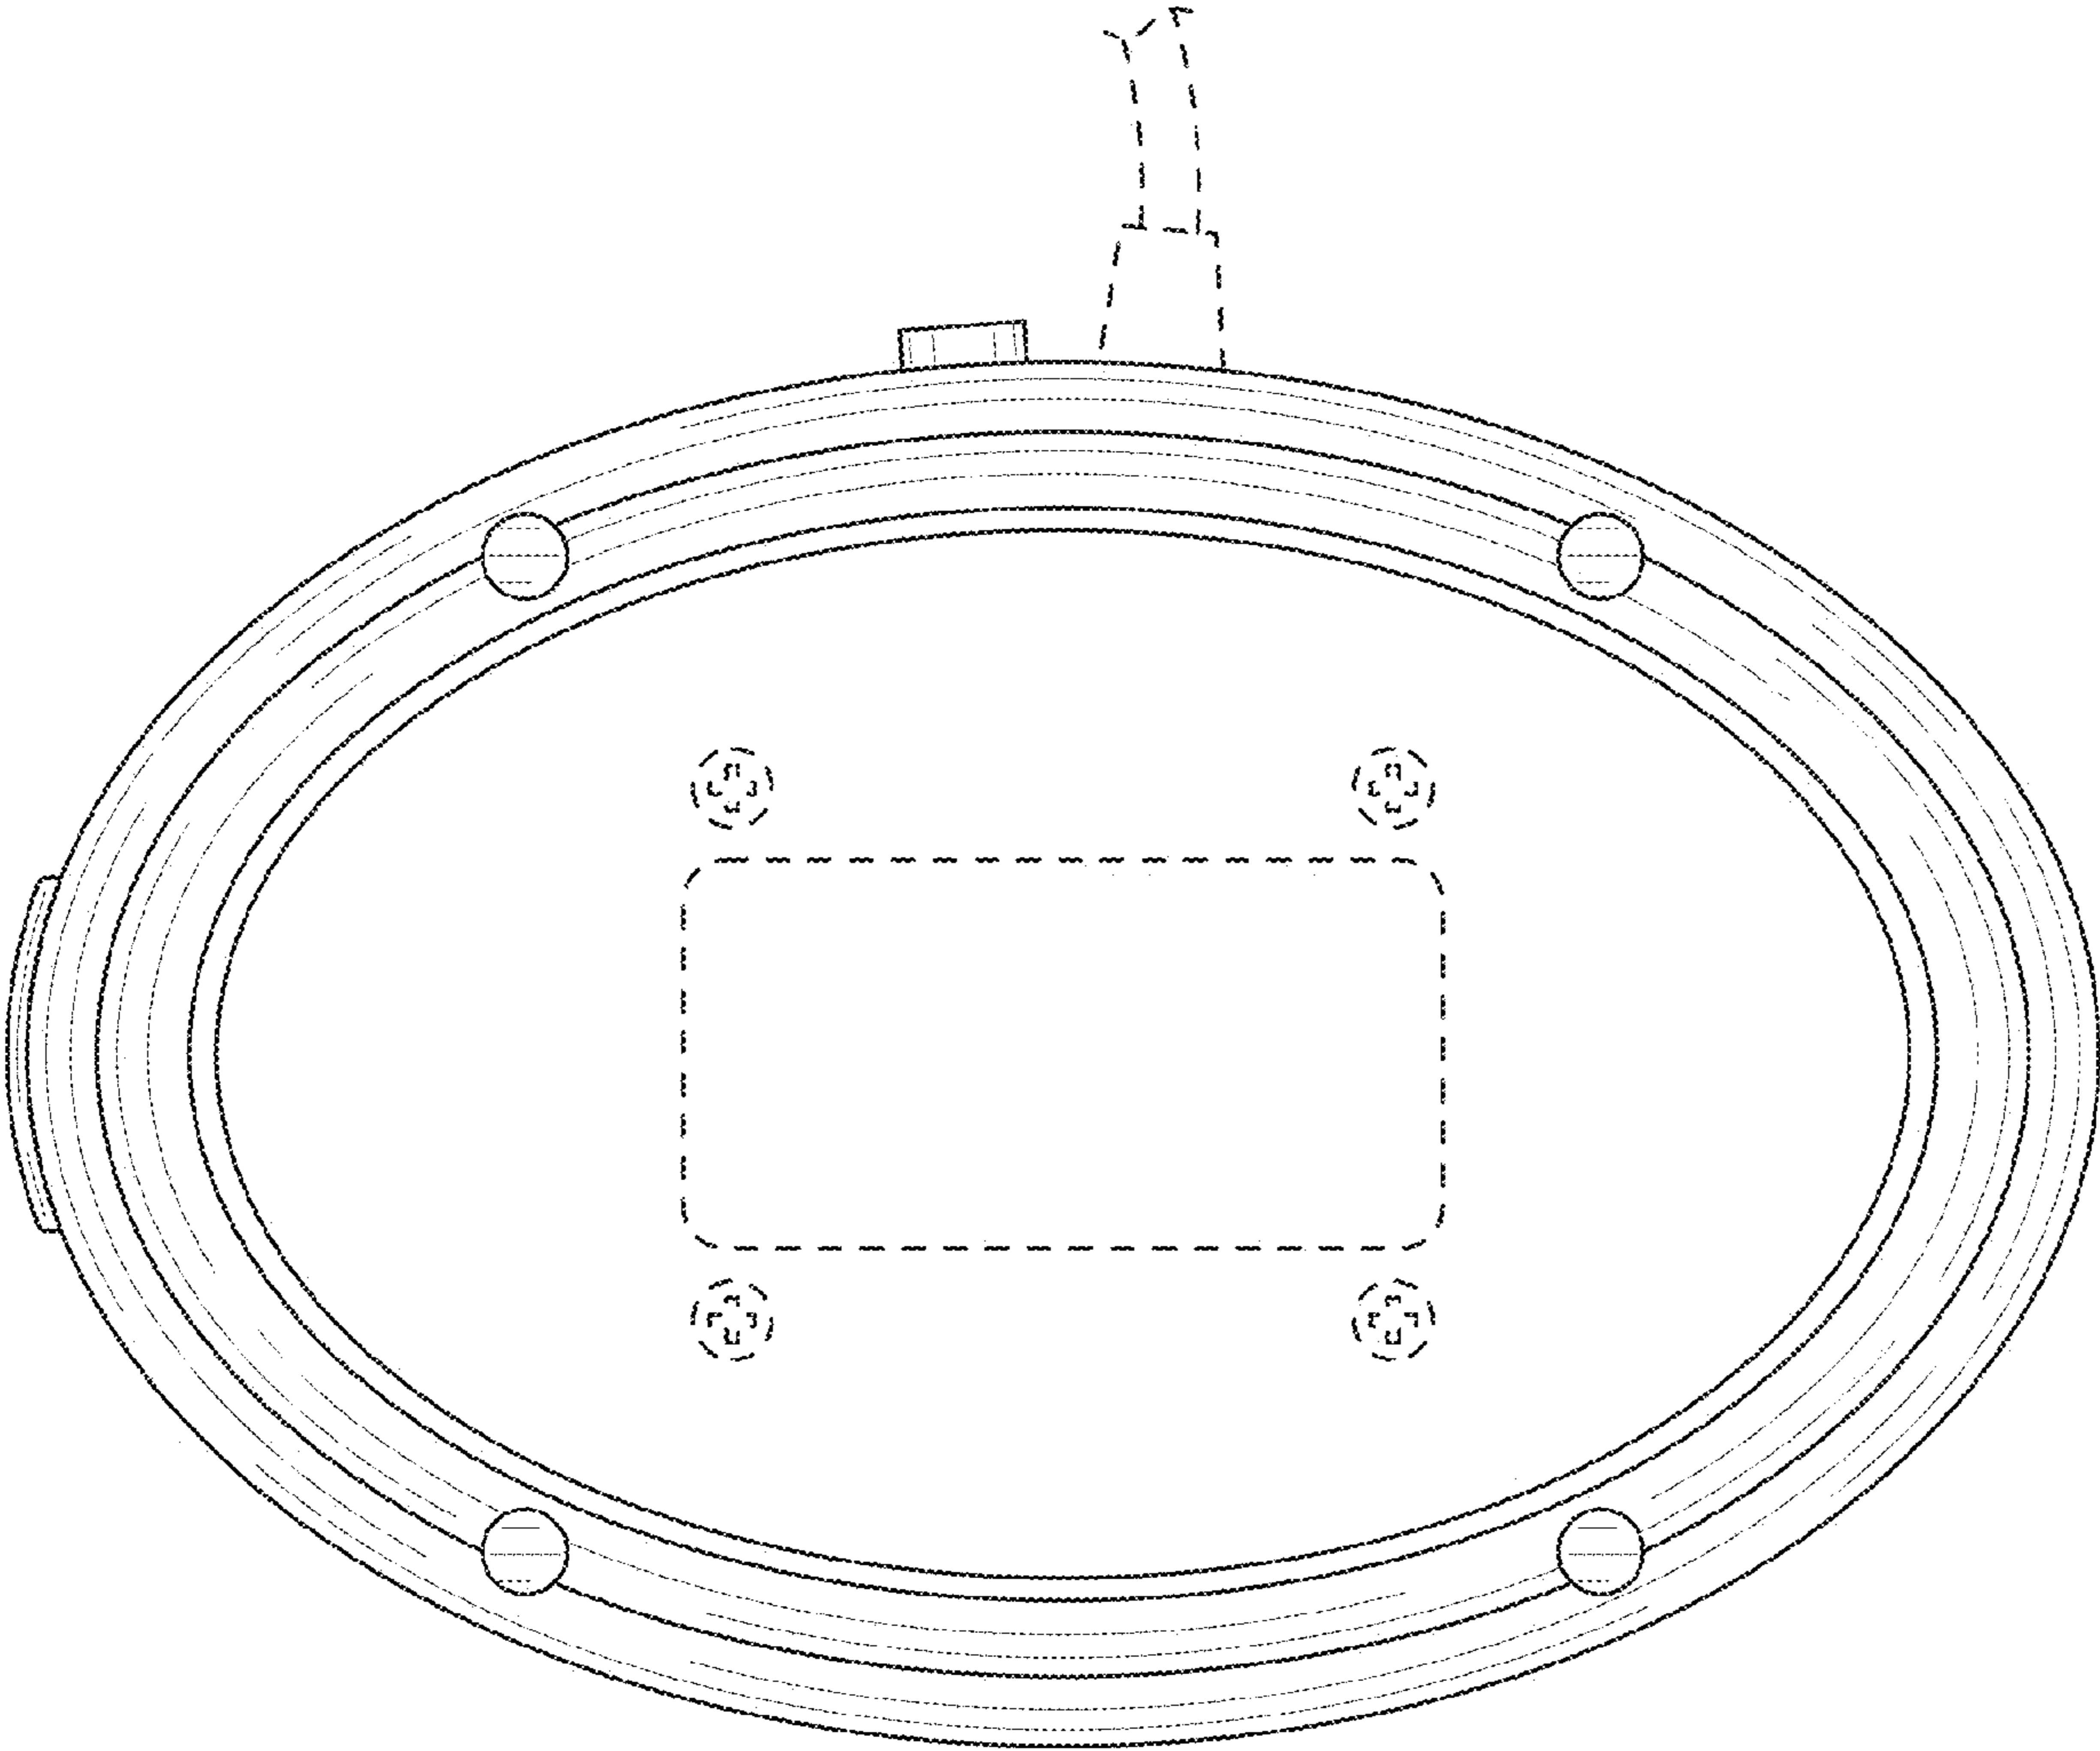


FIG. 3

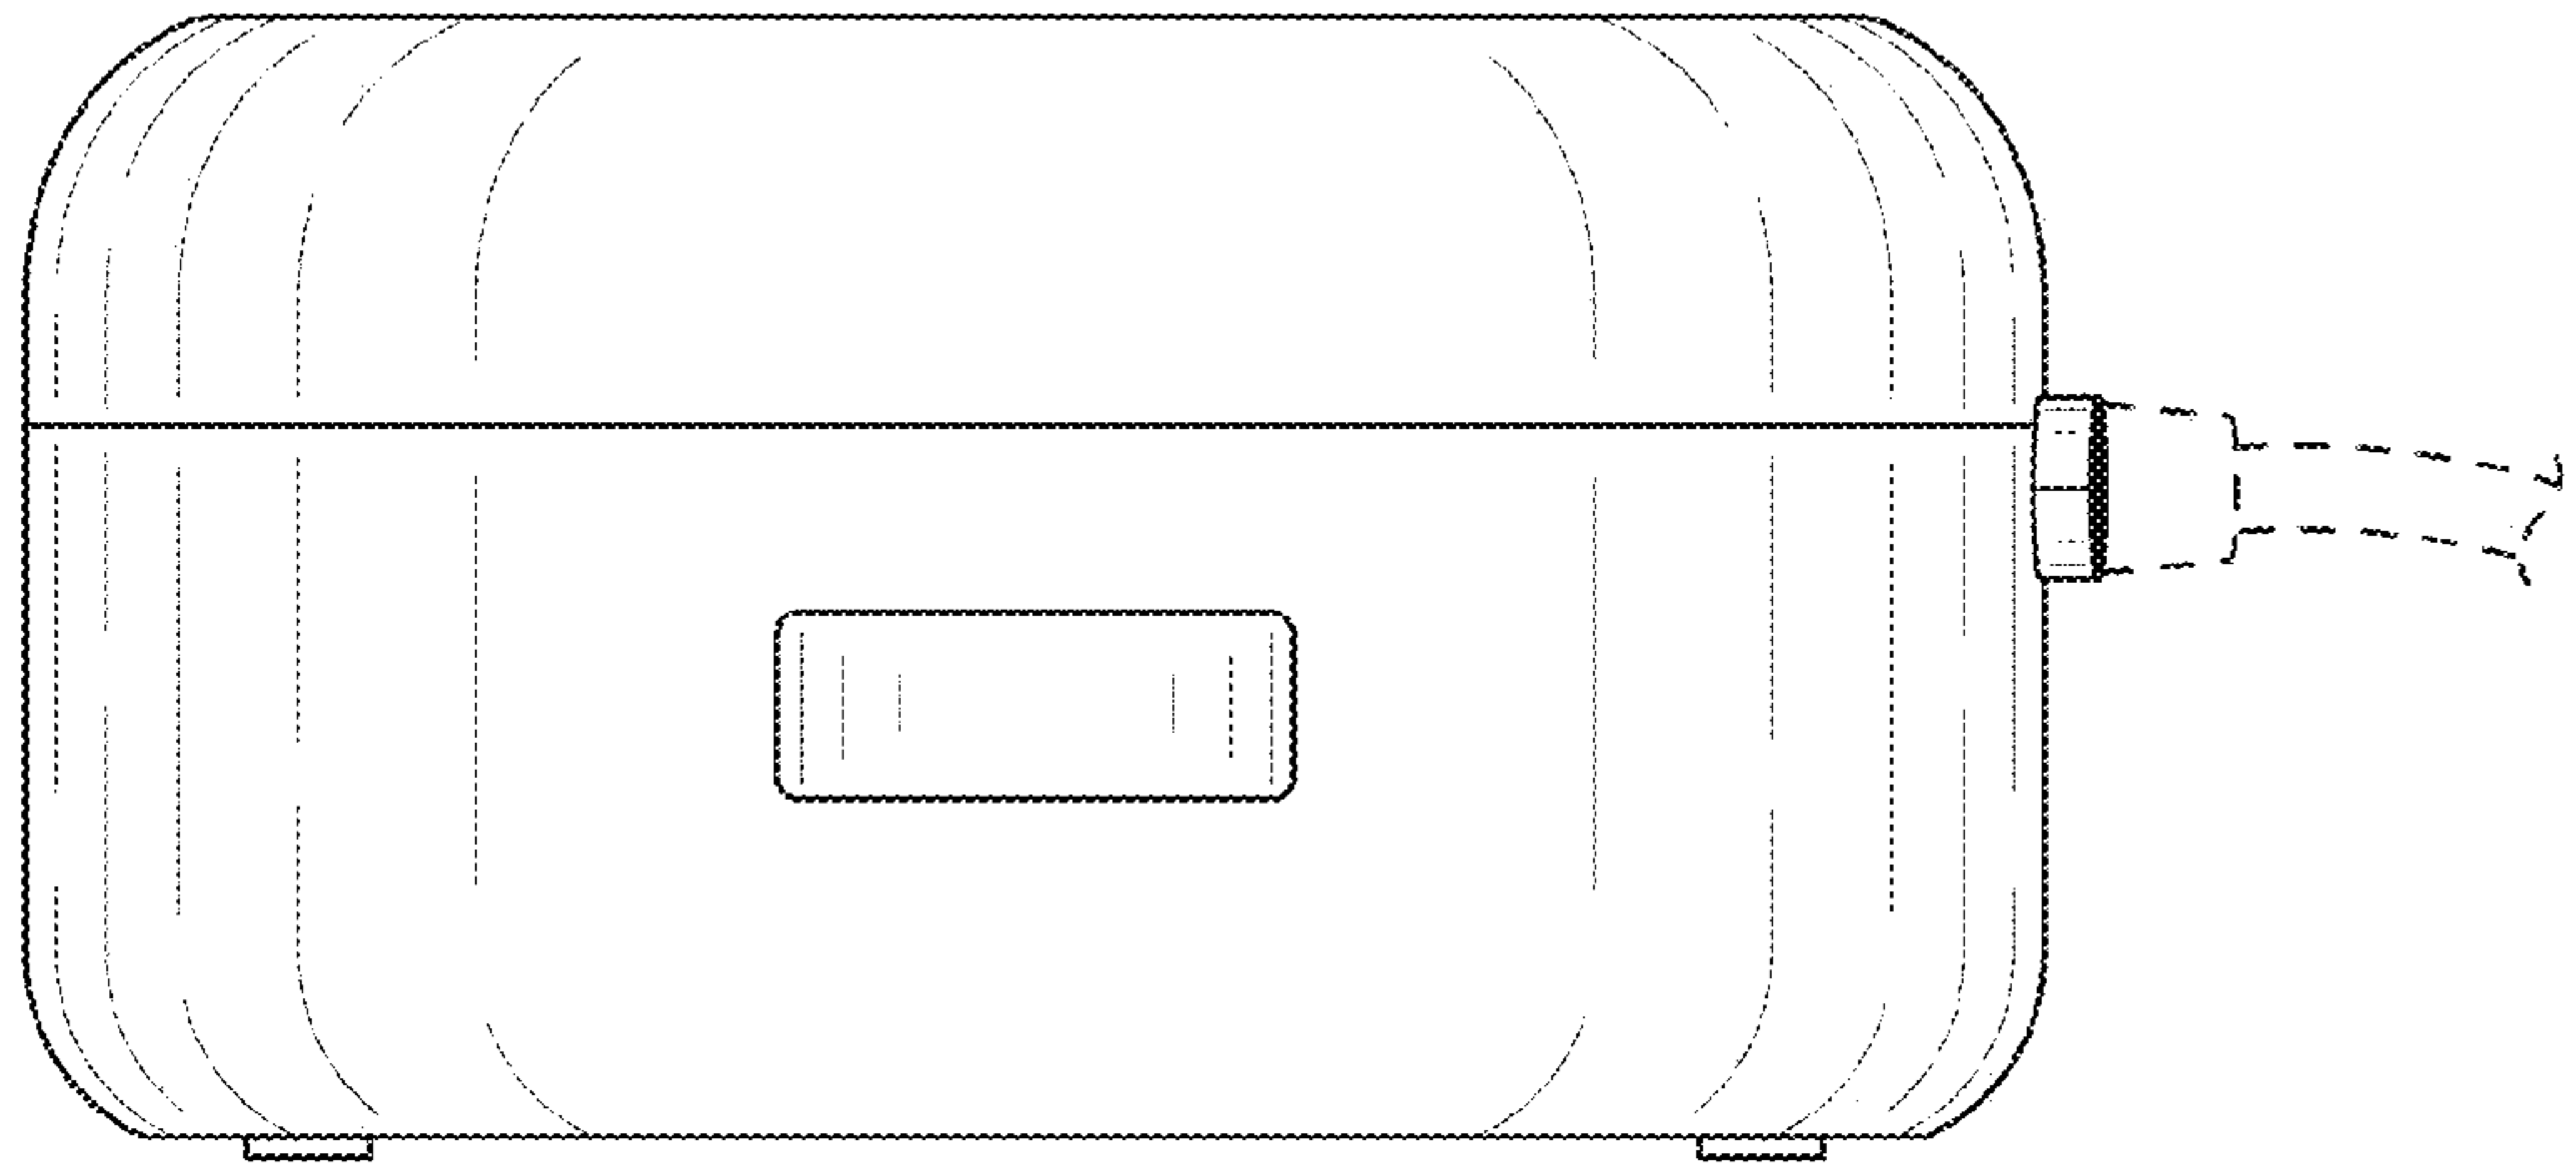


FIG. 4

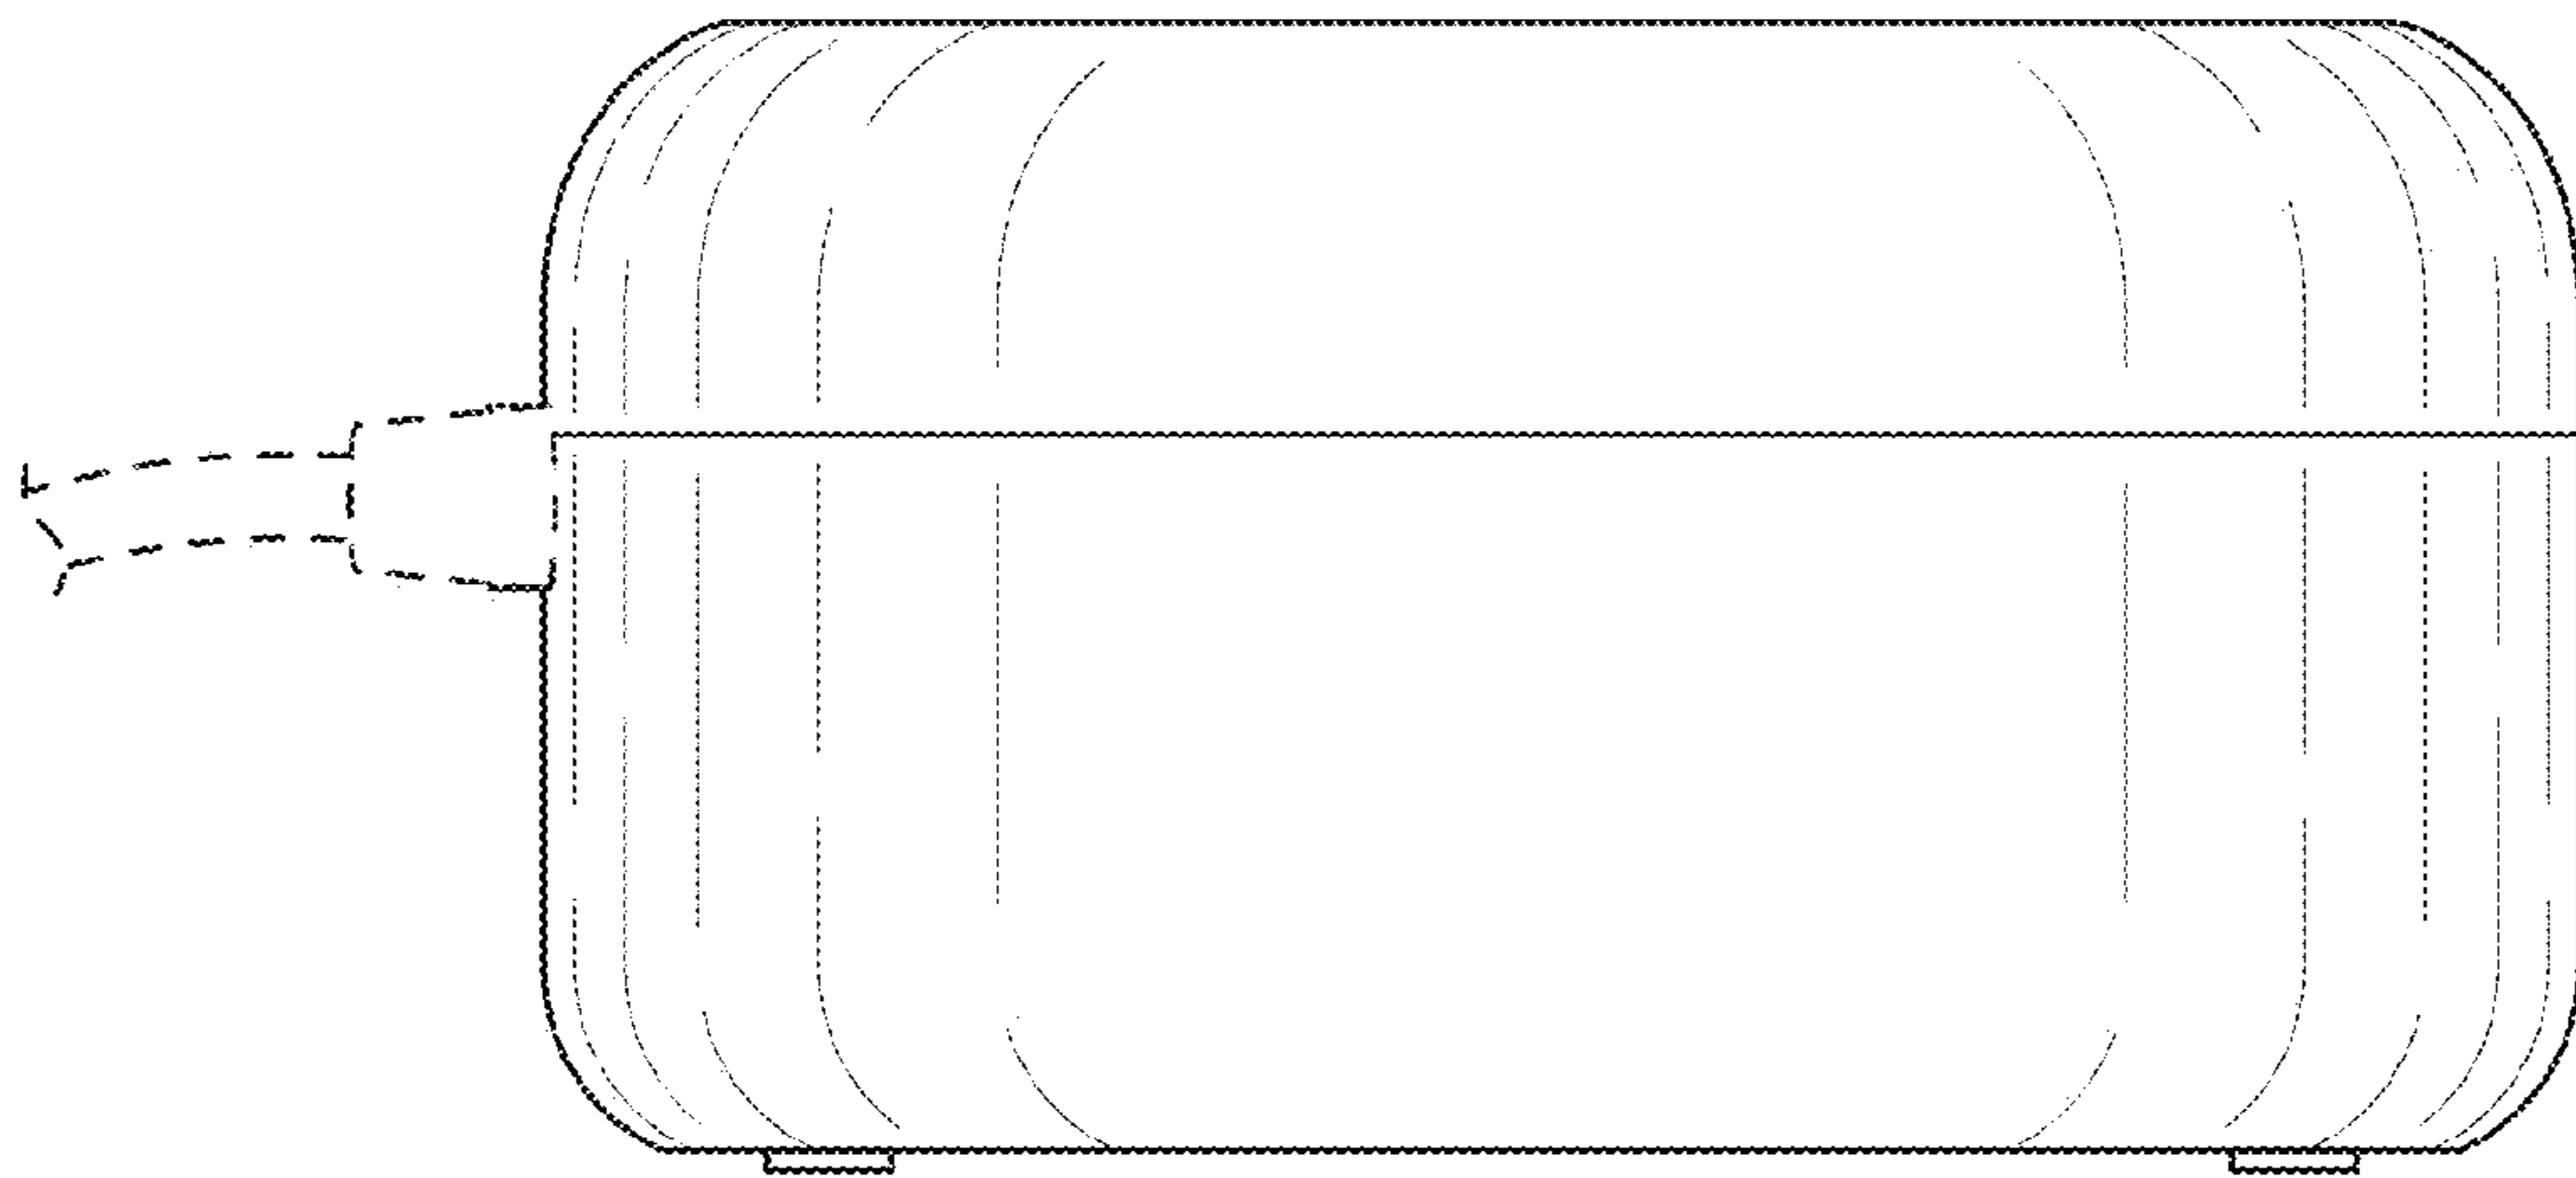


FIG. 5

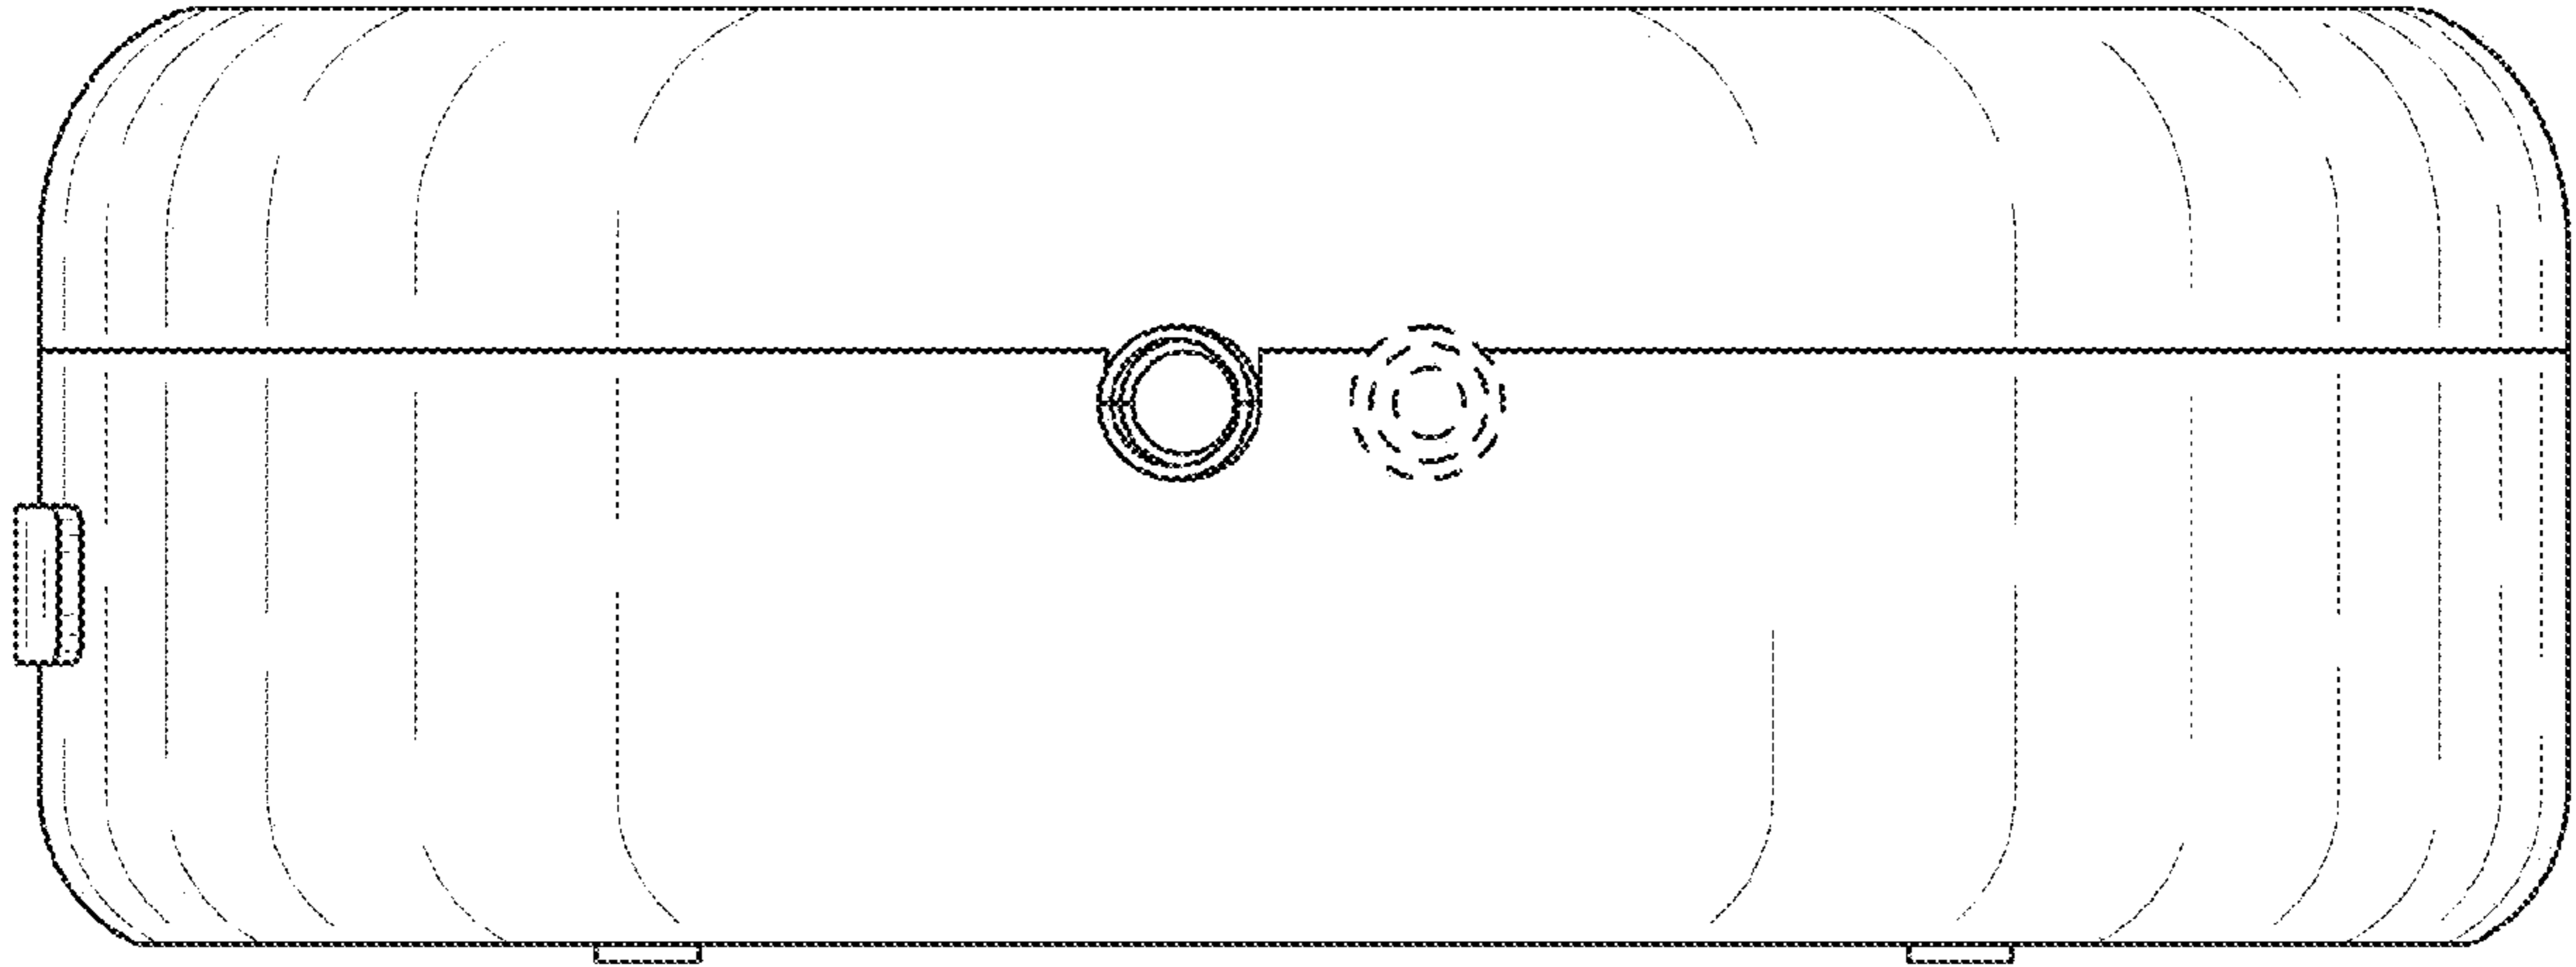


FIG. 6

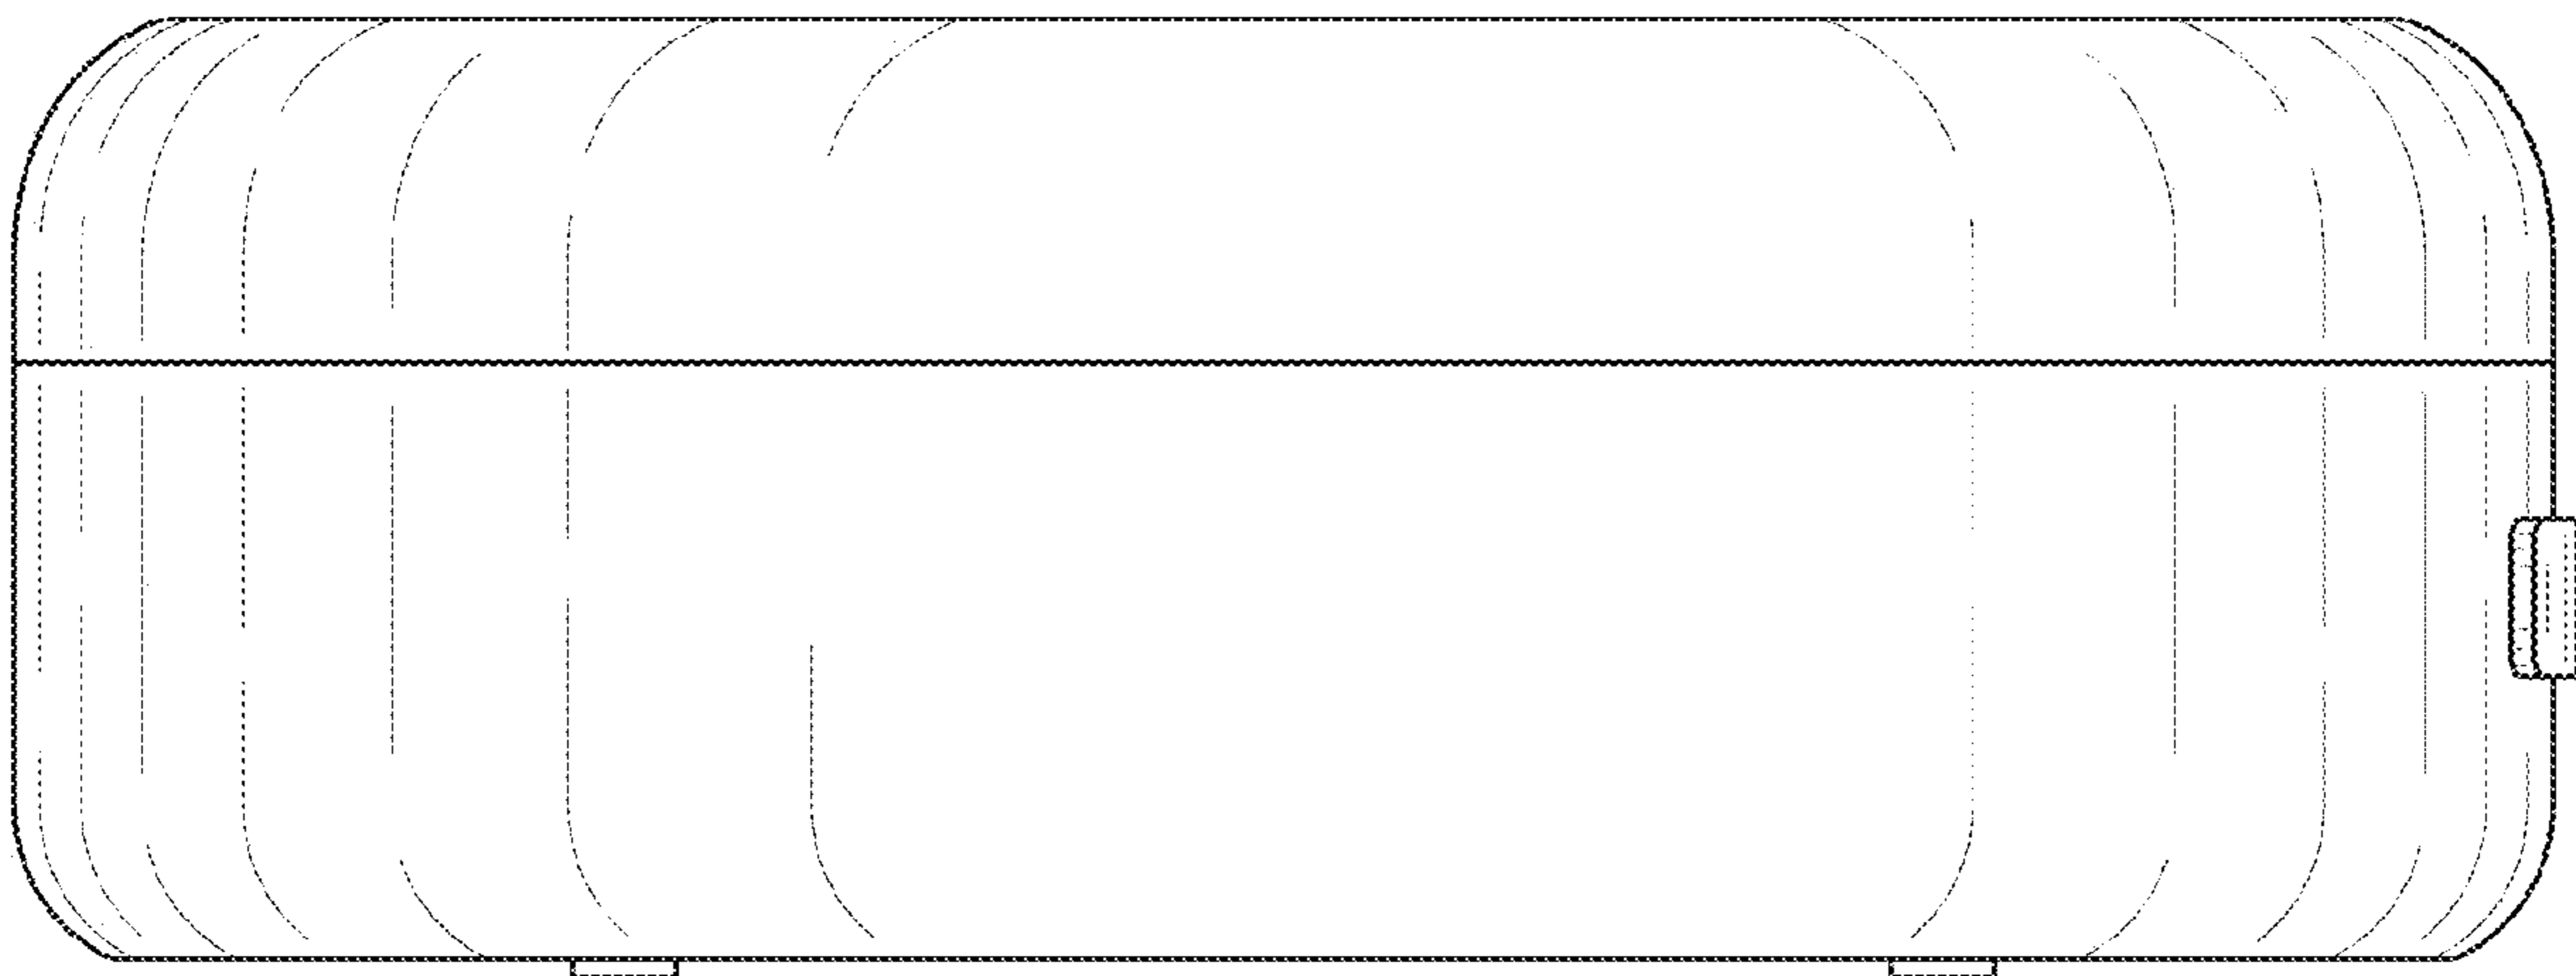


FIG. 7