



US00D957669S

(12) **United States Design Patent** (10) **Patent No.:** **US D957,669 S**
Xia (45) **Date of Patent:** **** Jul. 12, 2022**

(54) **STERILIZER**

(71) Applicant: **SHENZHEN IMDK MEDICAL TECHNOLOGY CO., LTD**, Shenzhen (CN)

(72) Inventor: **Changchun Xia**, Wenzhou (CN)

(73) Assignee: **SHENZHEN IMDK MEDICAL TECHNOLOGY CO., LTD**, Shenzhen (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/737,851**

(22) Filed: **Jun. 12, 2020**

(30) **Foreign Application Priority Data**

May 20, 2020 (CN) 202030236187.1

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/217**

(58) **Field of Classification Search**
USPC D24/107, 186, 200, 209–213, 217–219, D24/224–232; D32/1, 25; D23/366
CPC ... A61L 2/26; A61L 2/10; A61L 2/025; A61L 2202/11; A61L 2202/23; A61L 2202/122; A61L 2202/10
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D800,287 S * 10/2017 Sevy D23/366
D807,524 S * 1/2018 Koh D24/217
D819,191 S * 5/2018 Atabaki D23/366
D893,043 S * 8/2020 Ou Yang D24/217

D893,044 S * 8/2020 Wei D24/217
D893,045 S * 8/2020 Tang D24/217
D897,554 S * 9/2020 Winderlich D24/217
D907,233 S * 1/2021 Wu D24/217
10,905,785 B2 * 2/2021 Lucio A61M 16/0066
D917,065 S * 4/2021 Cui D24/217
D923,156 S * 6/2021 O'Neil D23/265
2020/0405899 A1 * 12/2020 Yang A61L 2/10

OTHER PUBLICATIONS

Shenzhen IMDK Medical Technology Co., Ltd, posted at imdk.en.alibaba, no posting date, retrieved Jul. 30, 2021, online, URL: https://imdk.en.alibaba.com/?spm=a2700.shop_plser.88.28 (Year: 2021).*

* cited by examiner

Primary Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Li & Cai Intellectual Property (USA) Office


(57) **CLAIM**

The ornamental design for a sterilizer, as shown and described.

DESCRIPTION

FIG. 1 is a front, right side and bottom perspective view of a sterilizer showing my new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a left side elevational view thereof;
FIG. 5 is a right side elevational view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The broken lines in the drawing depict portions of the sterilizer that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

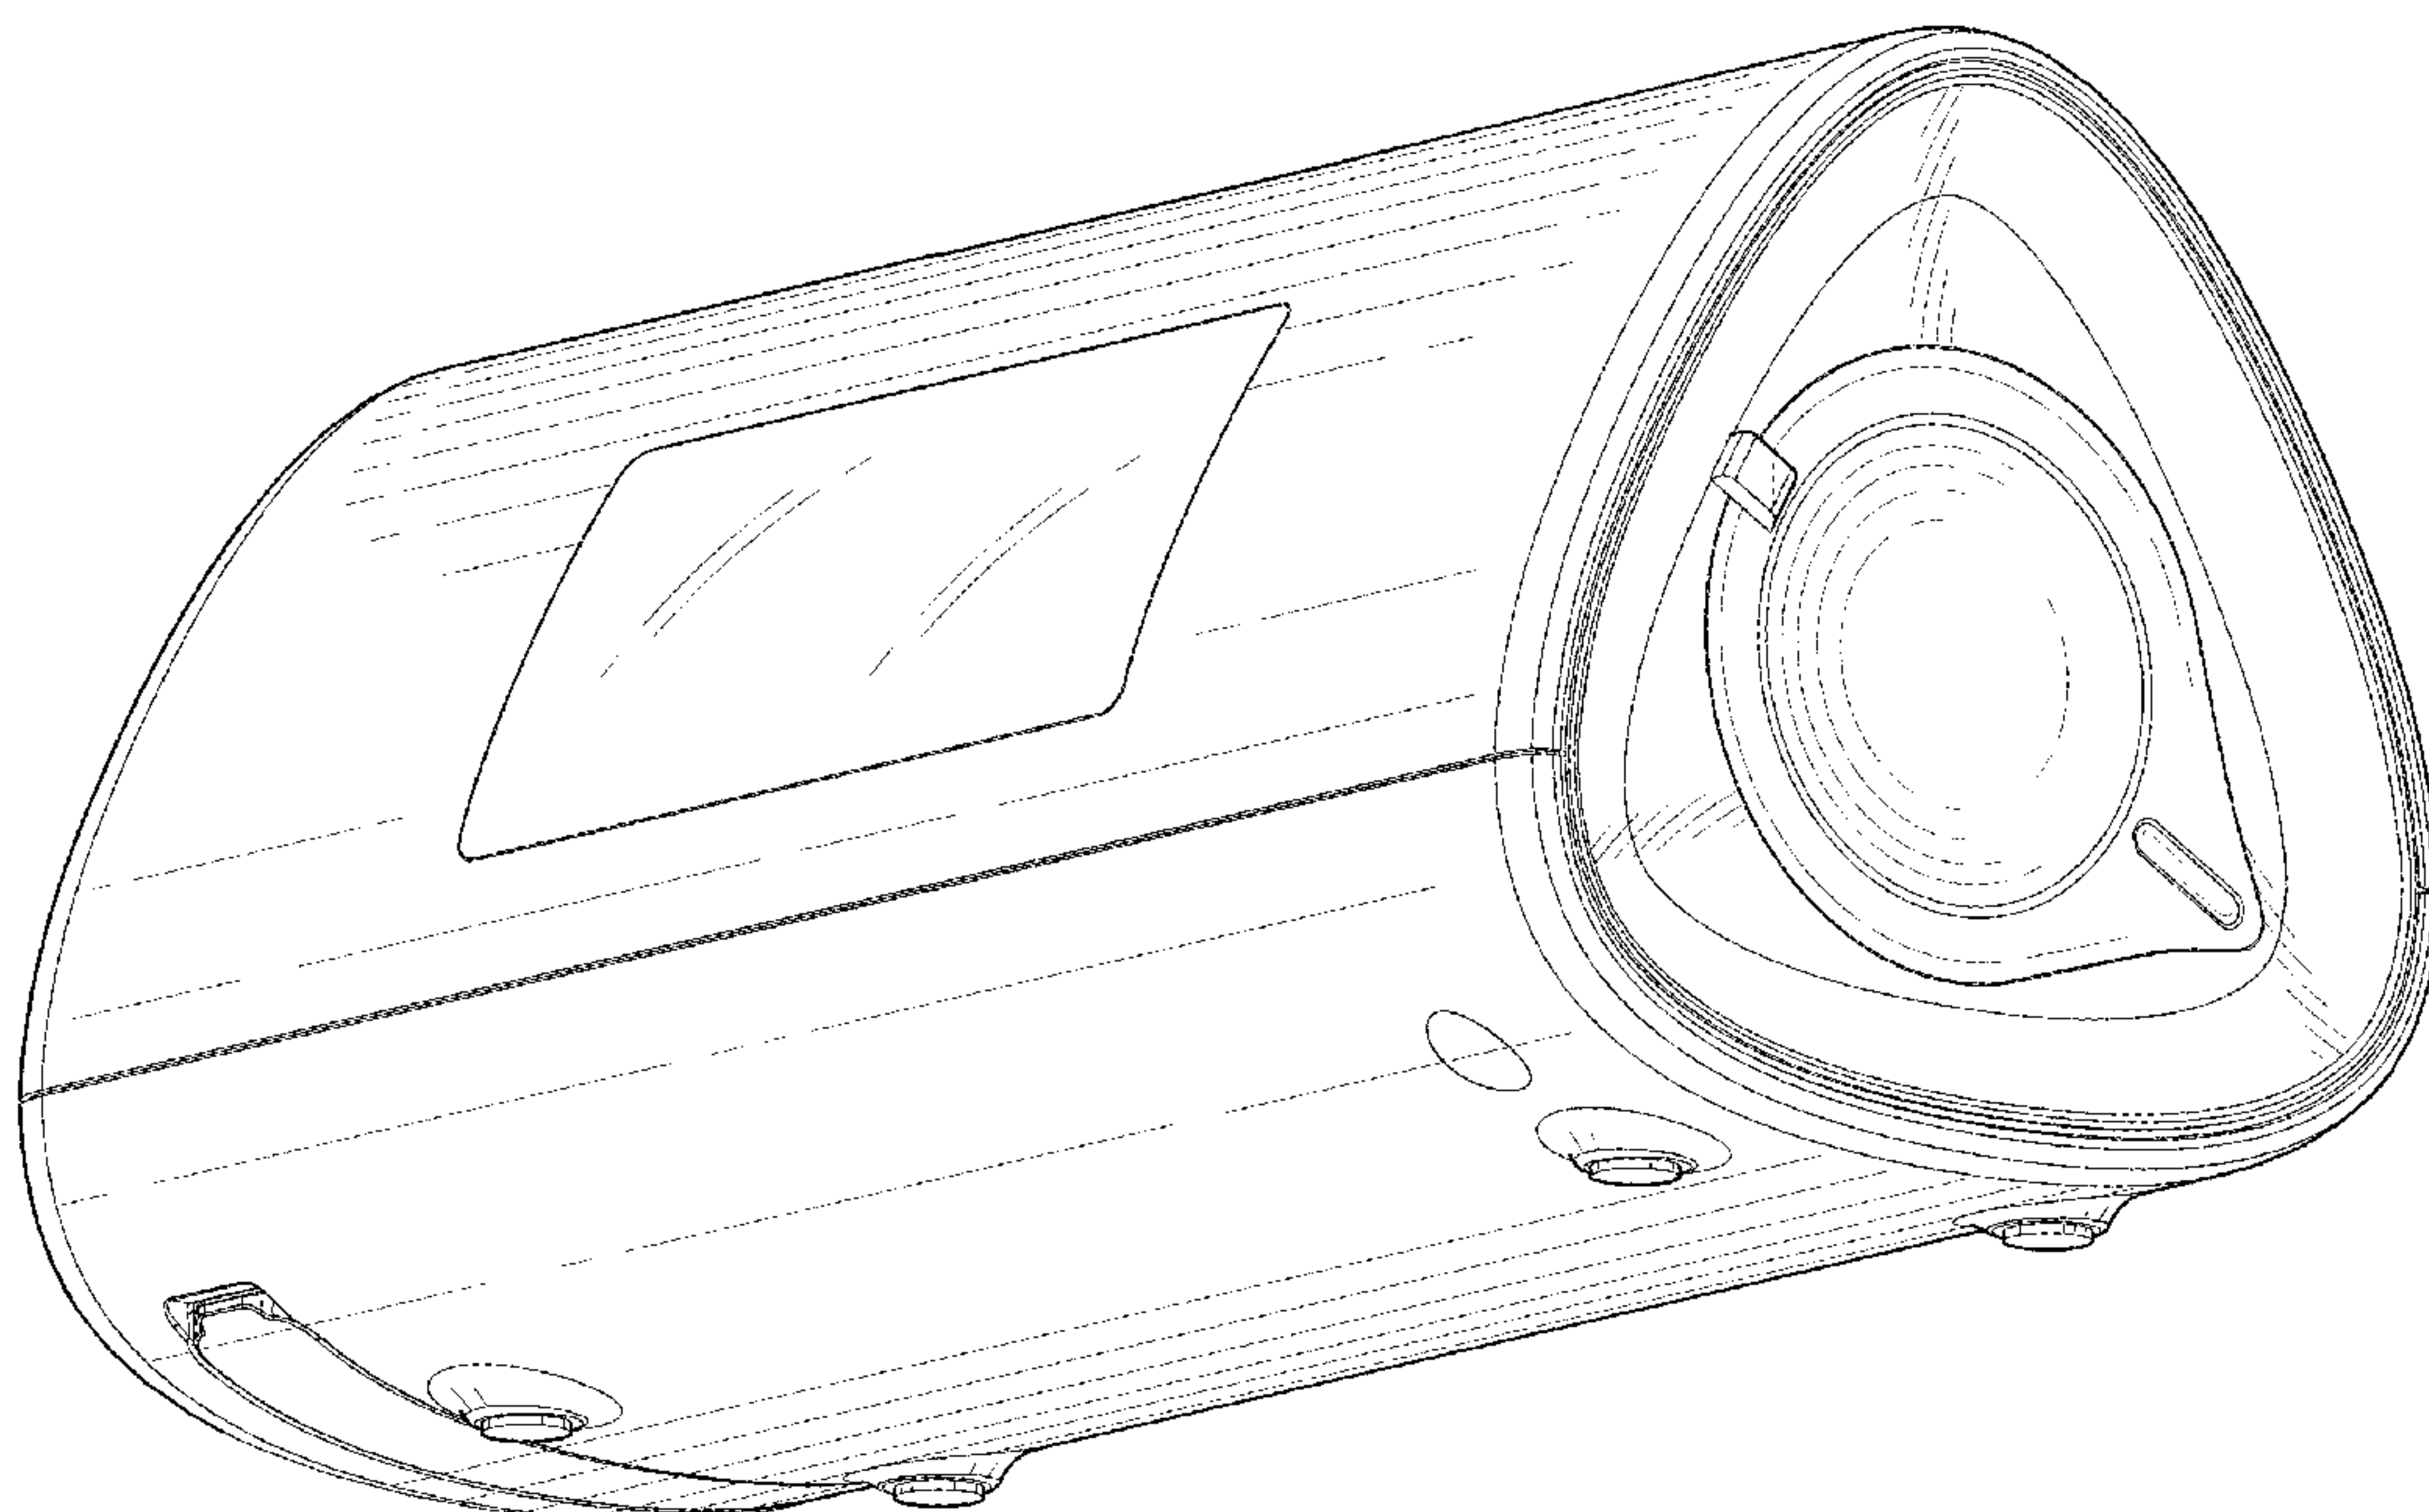

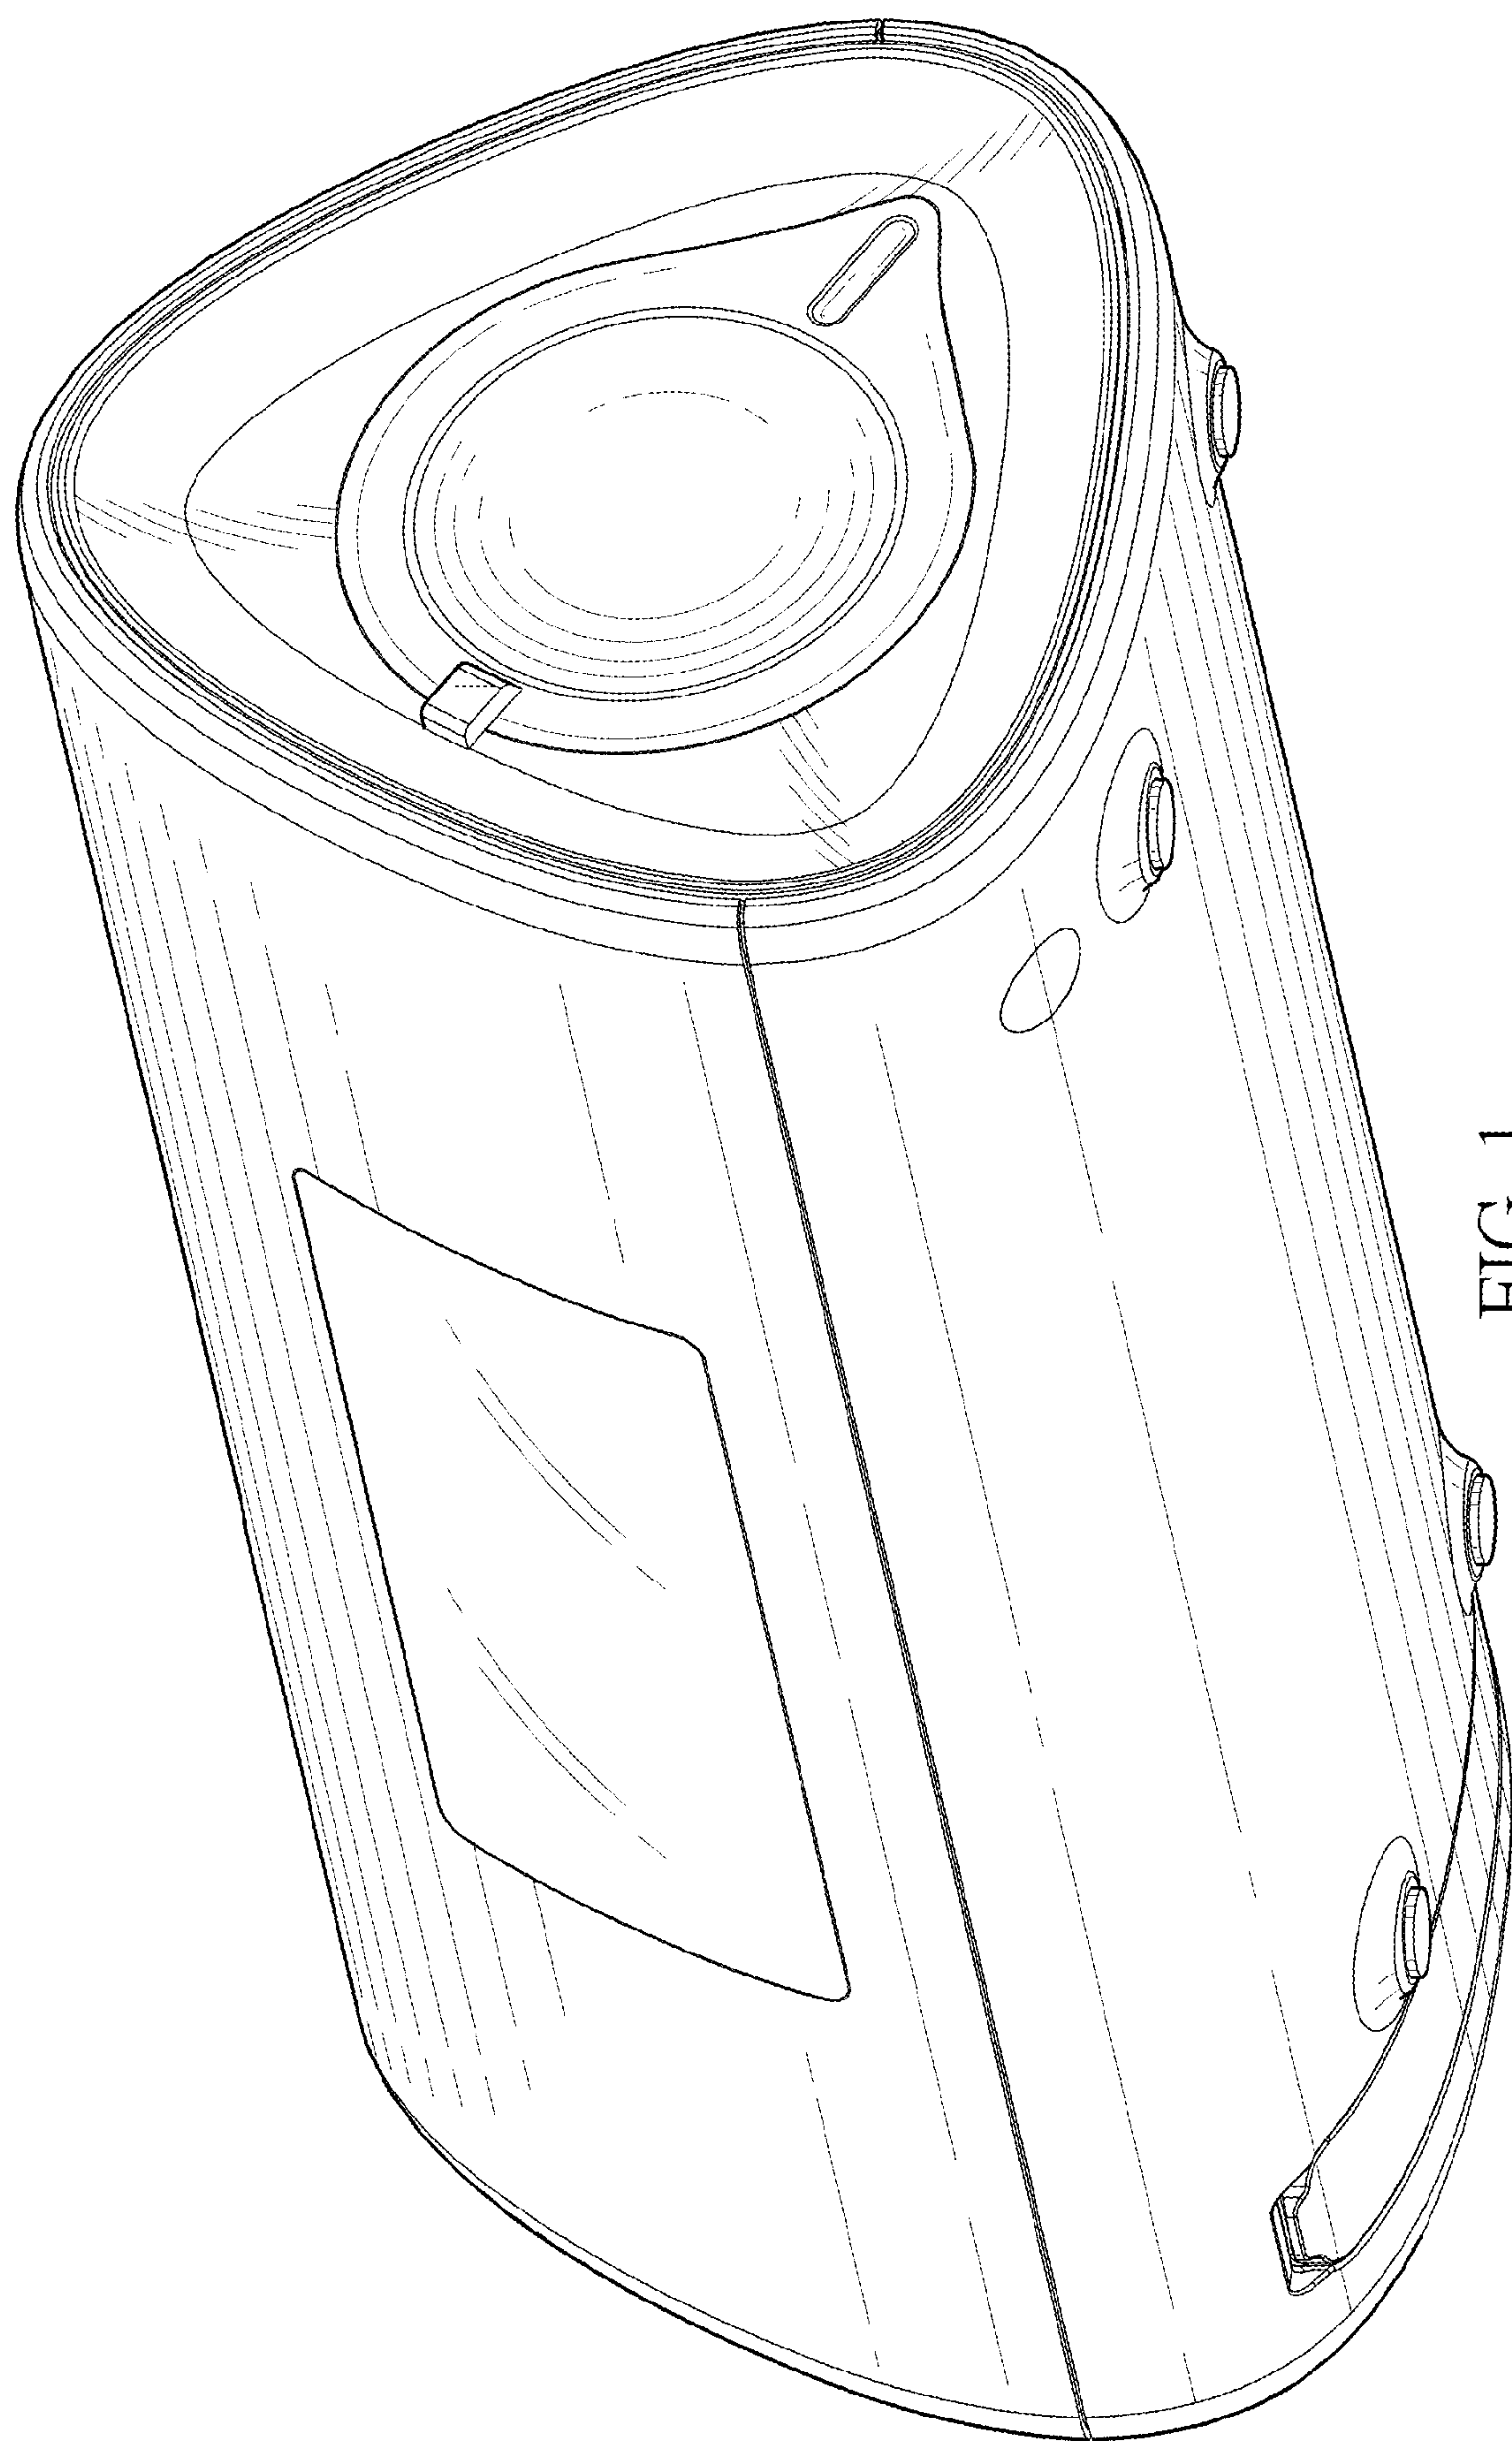


FIG. 1

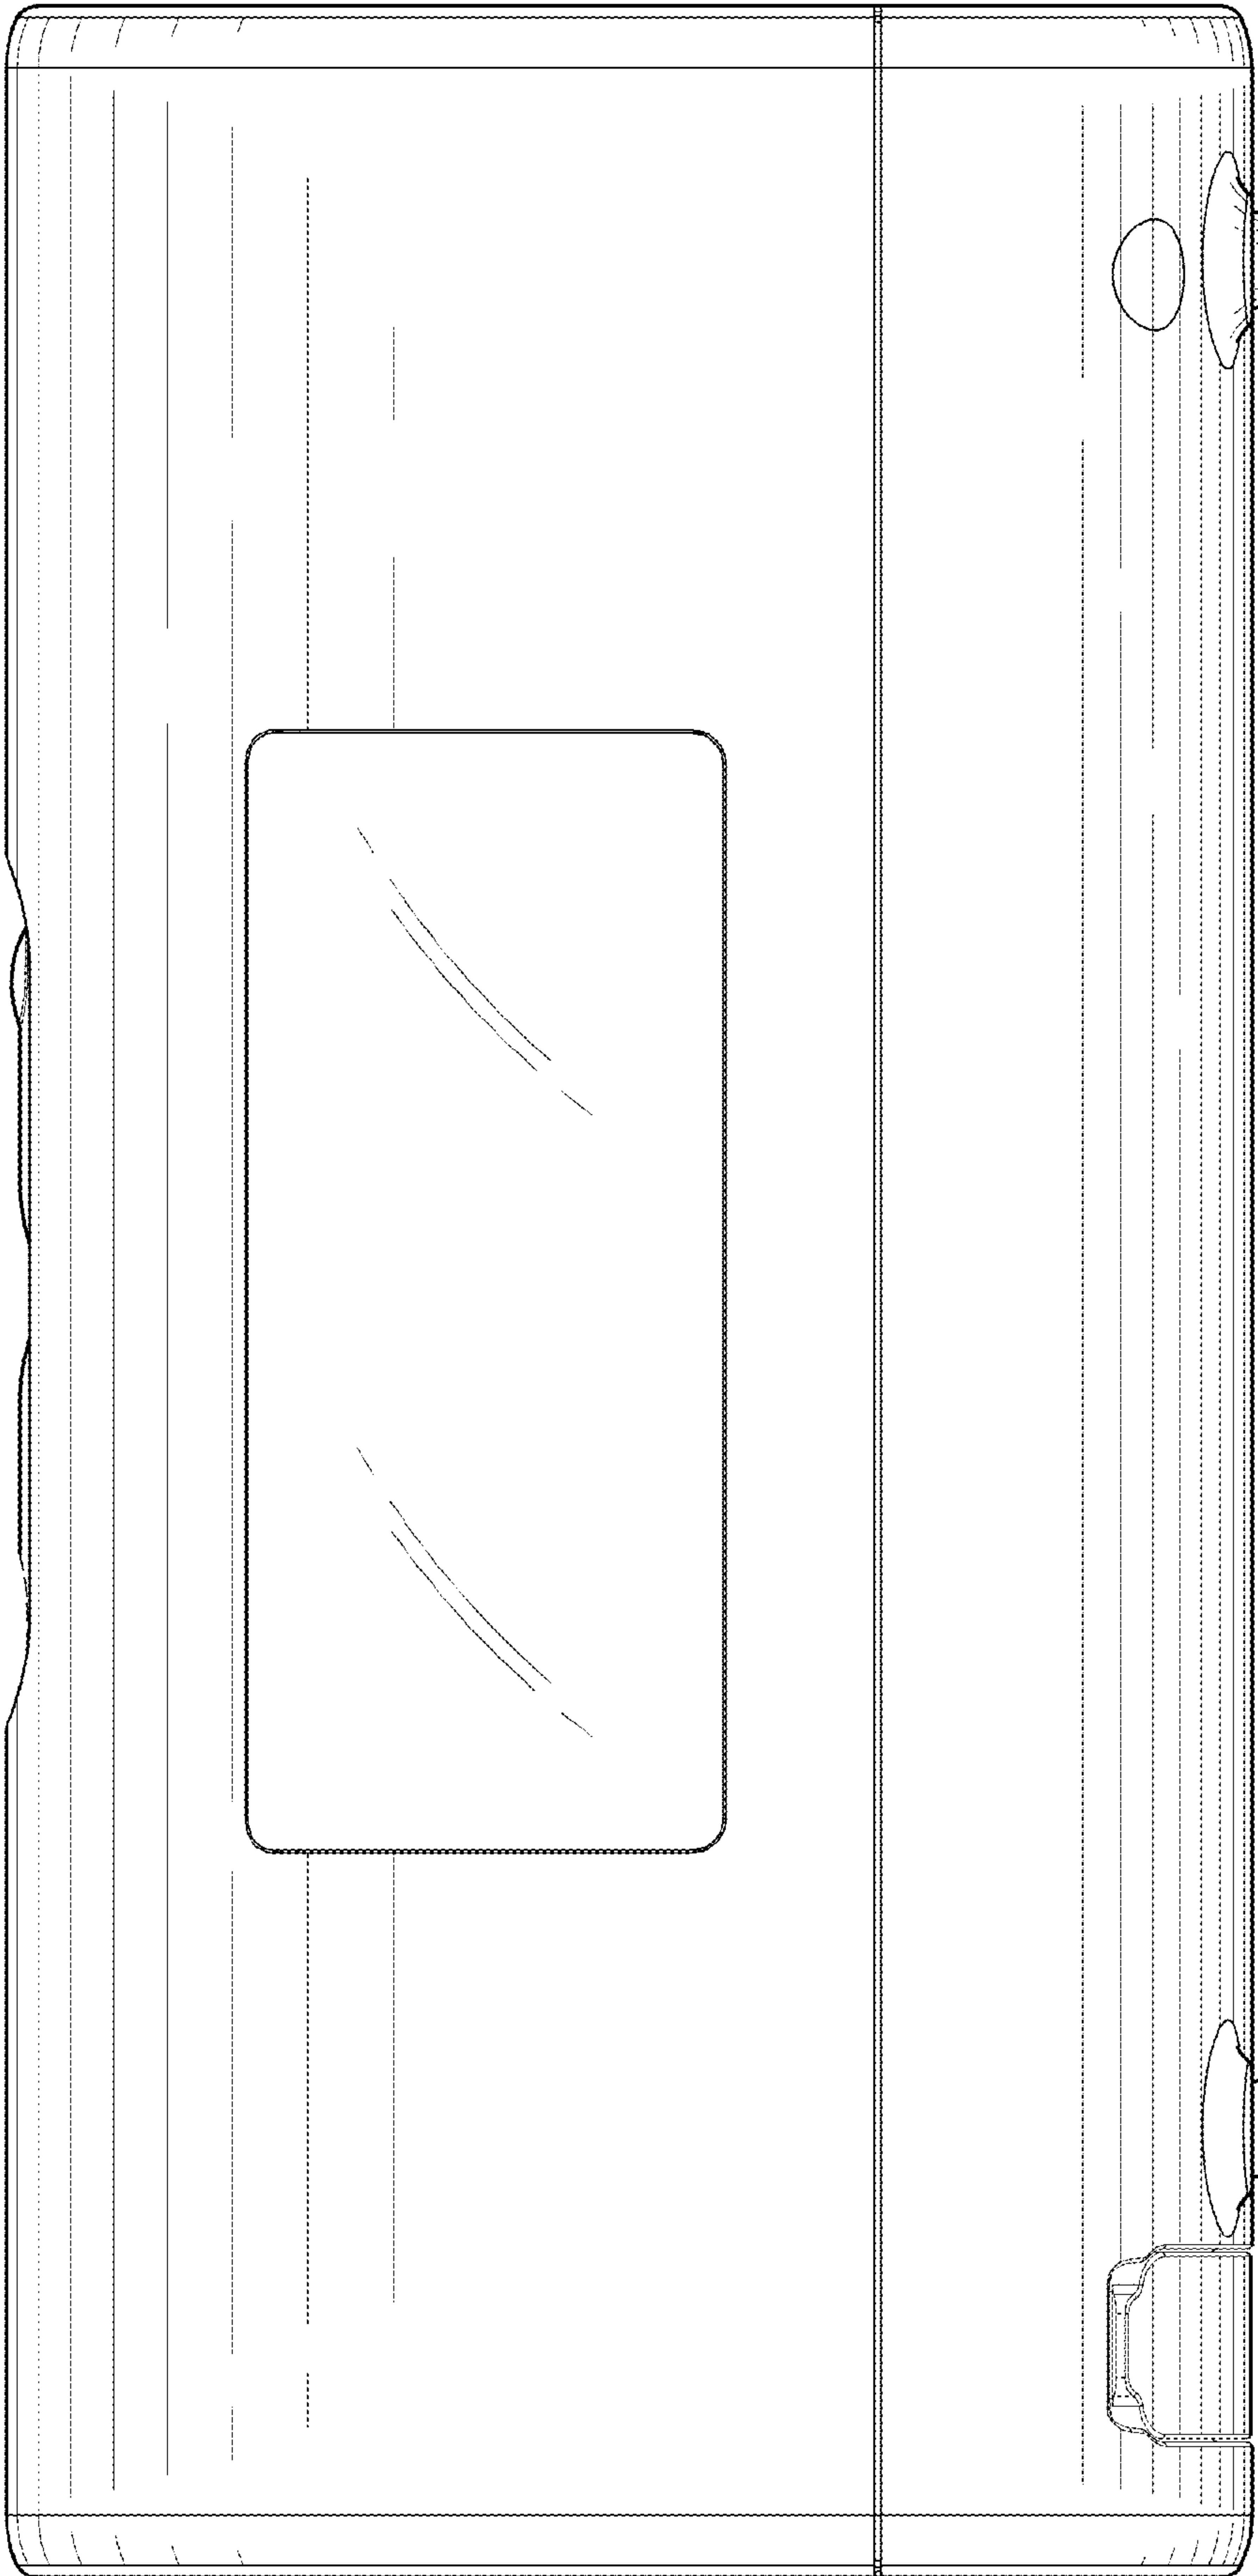


FIG. 2

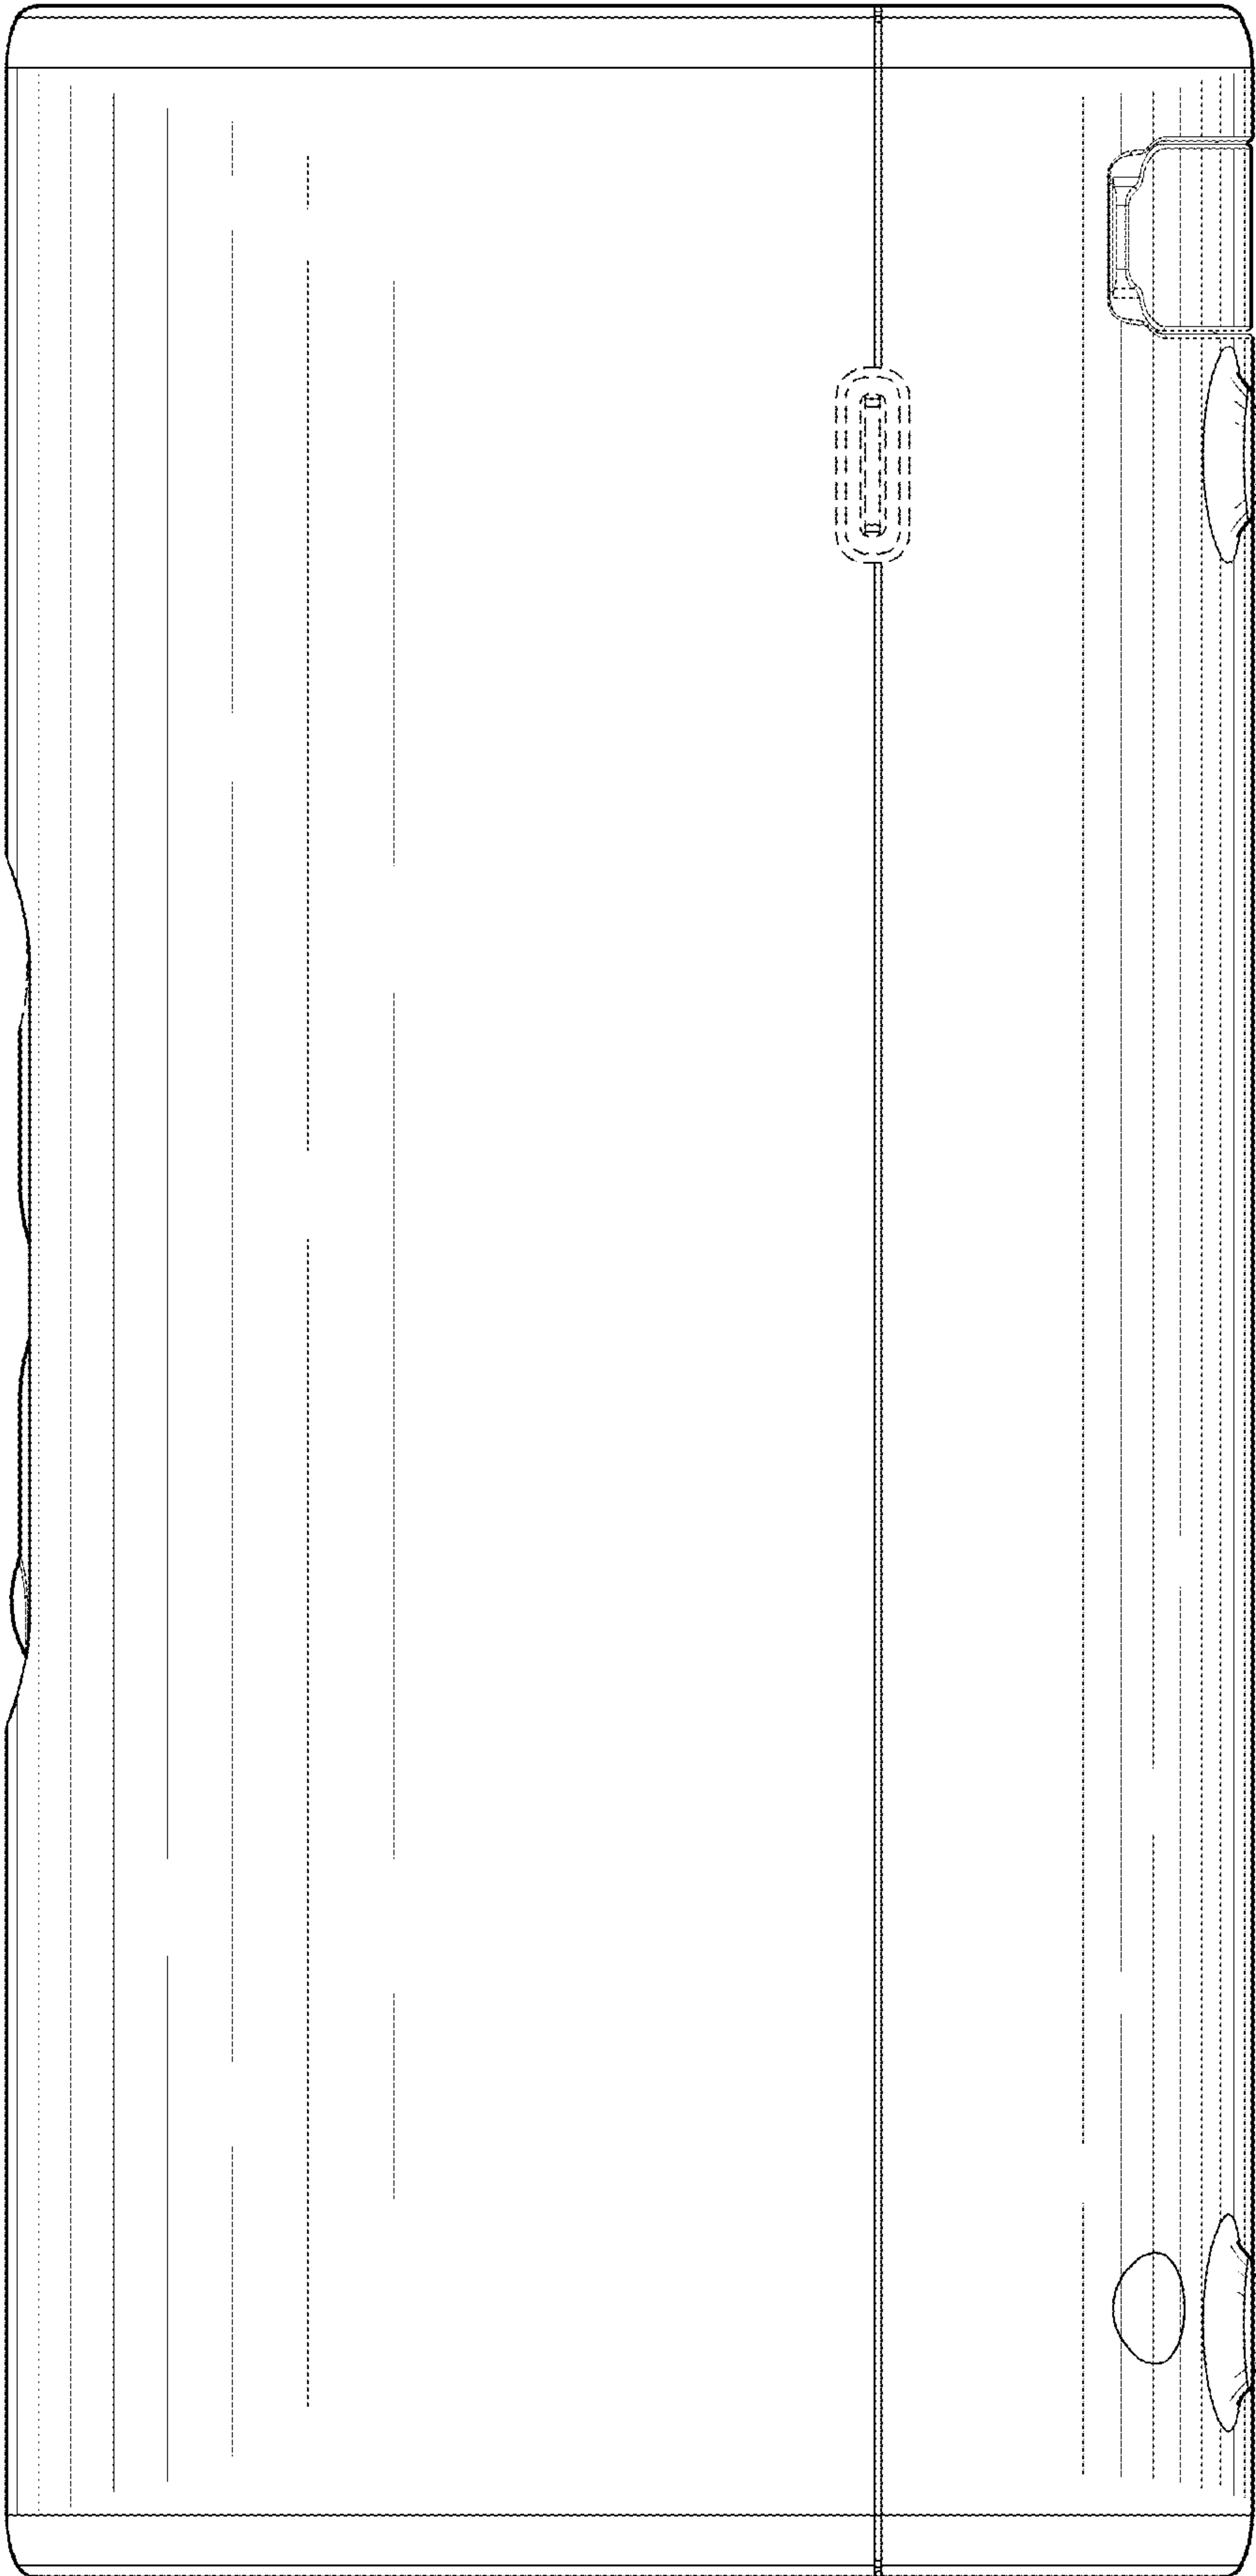


FIG. 3

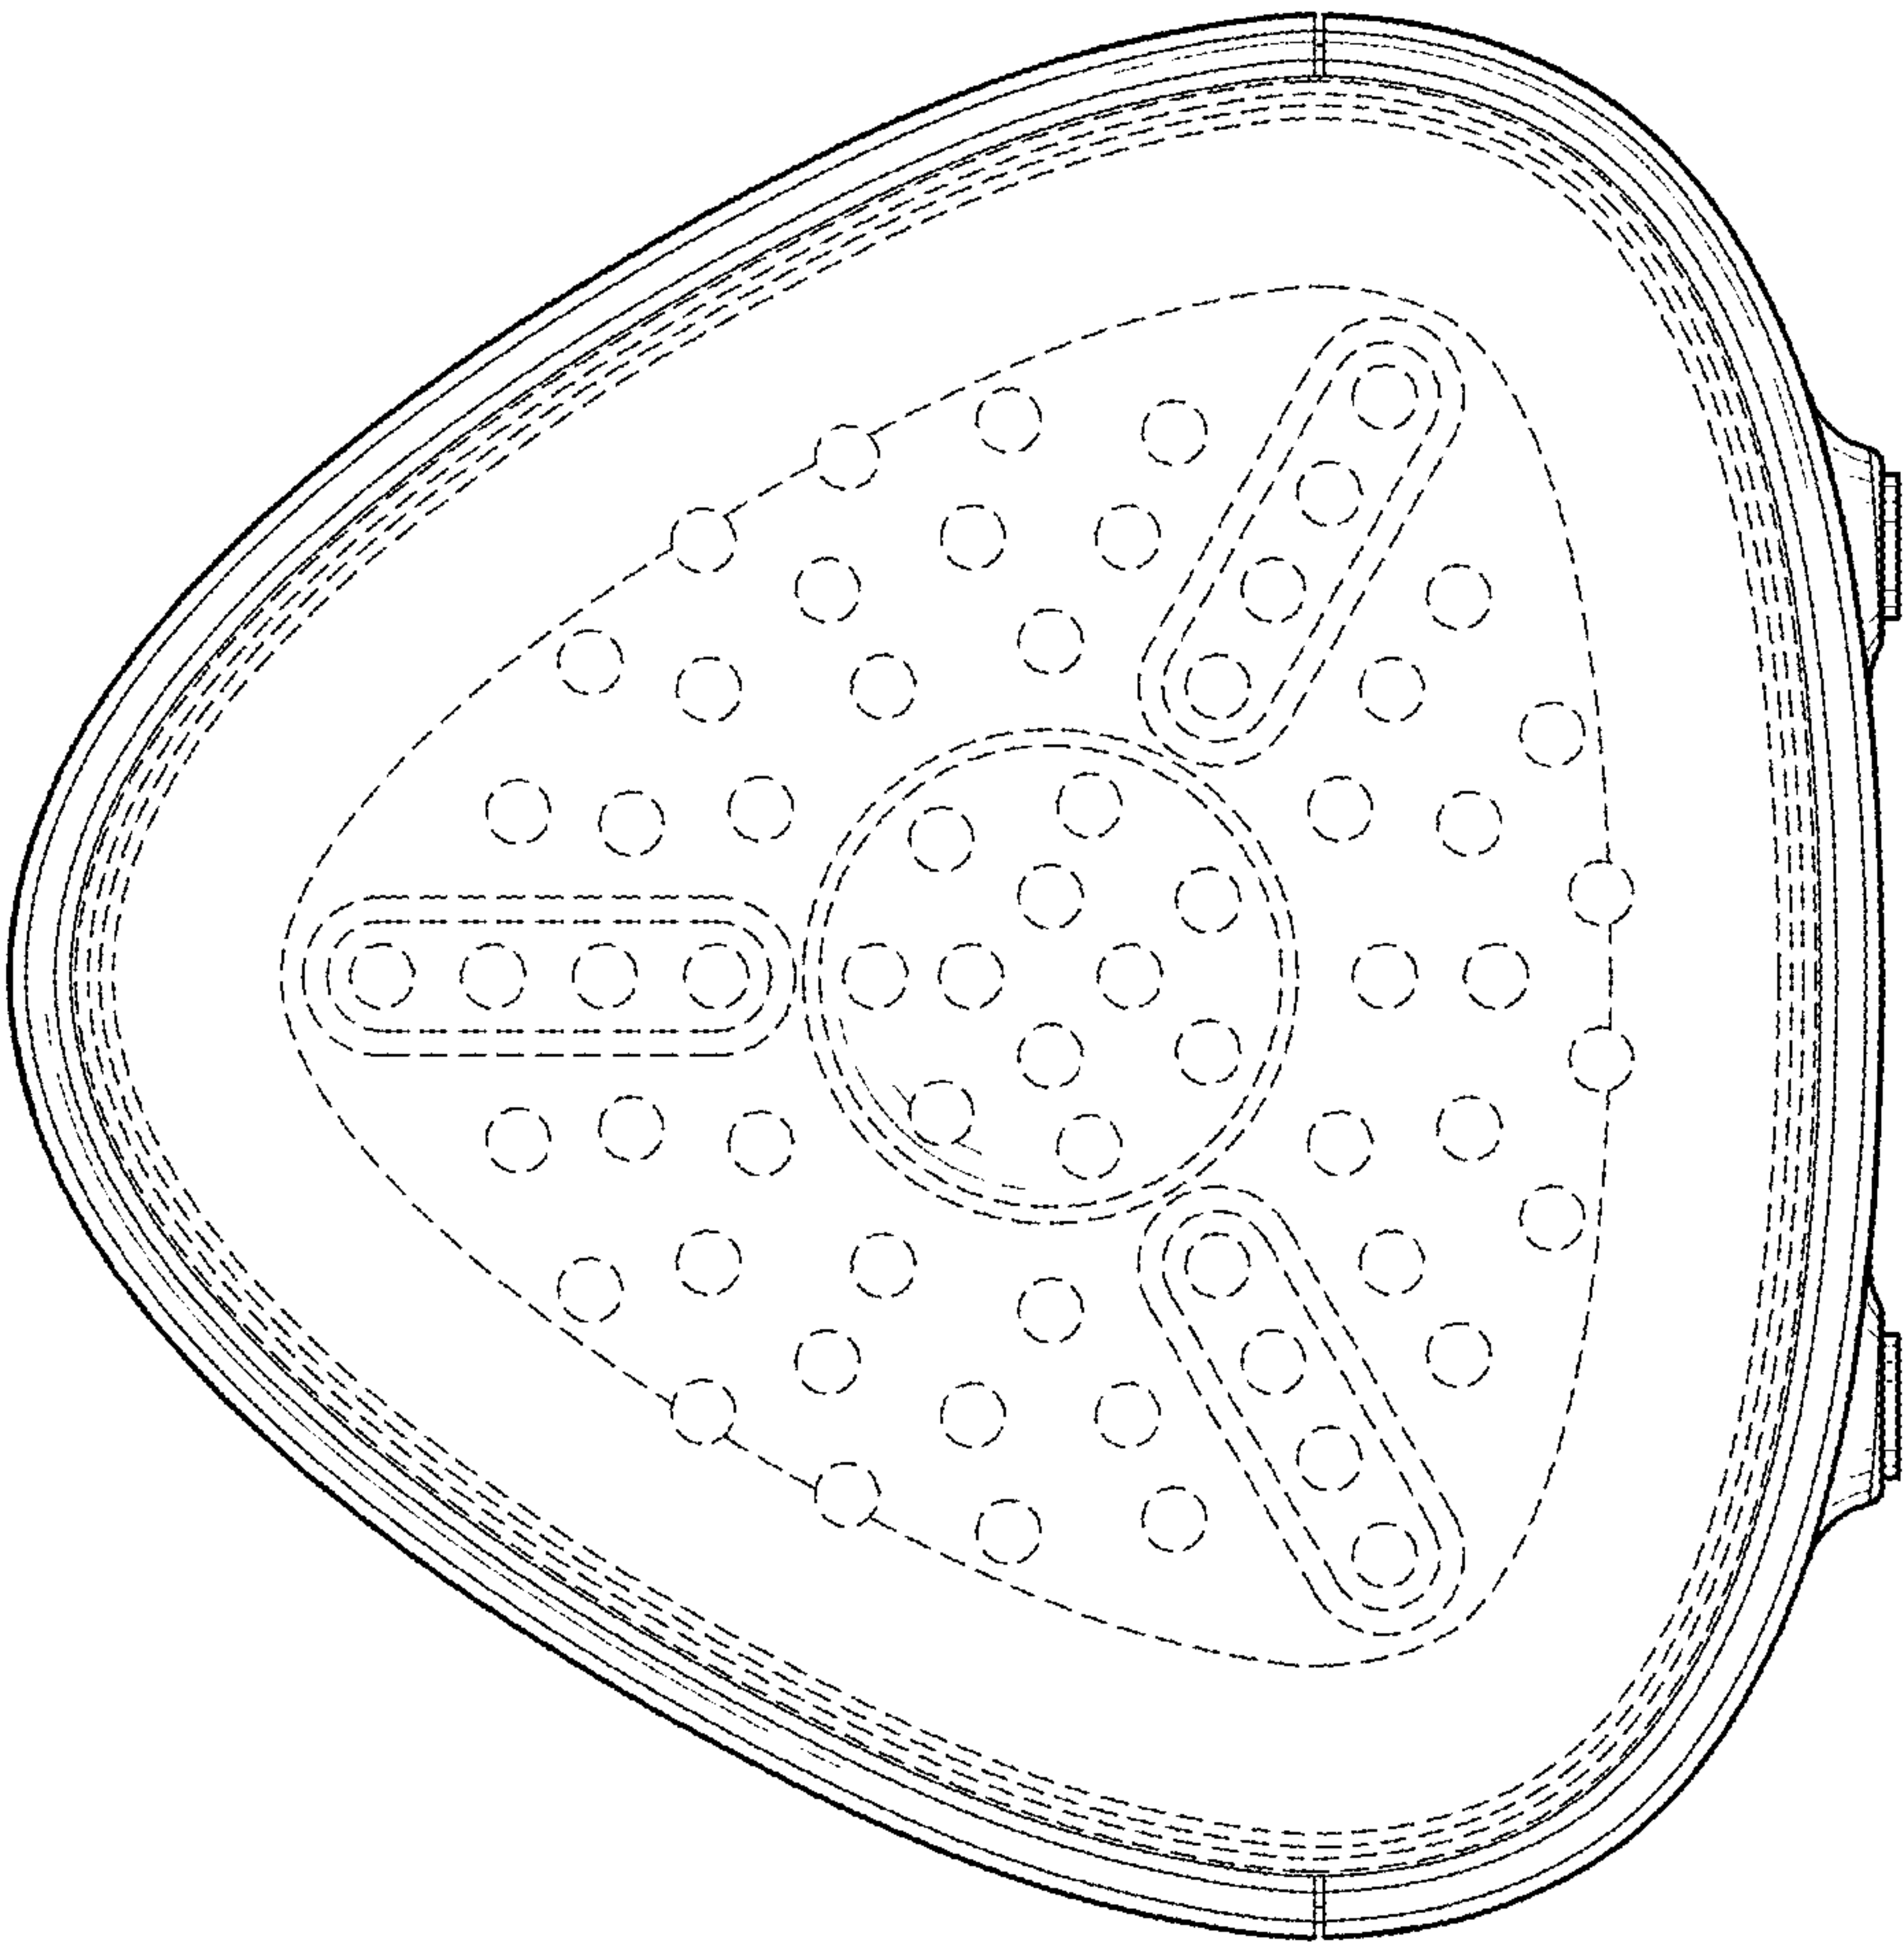


FIG. 4

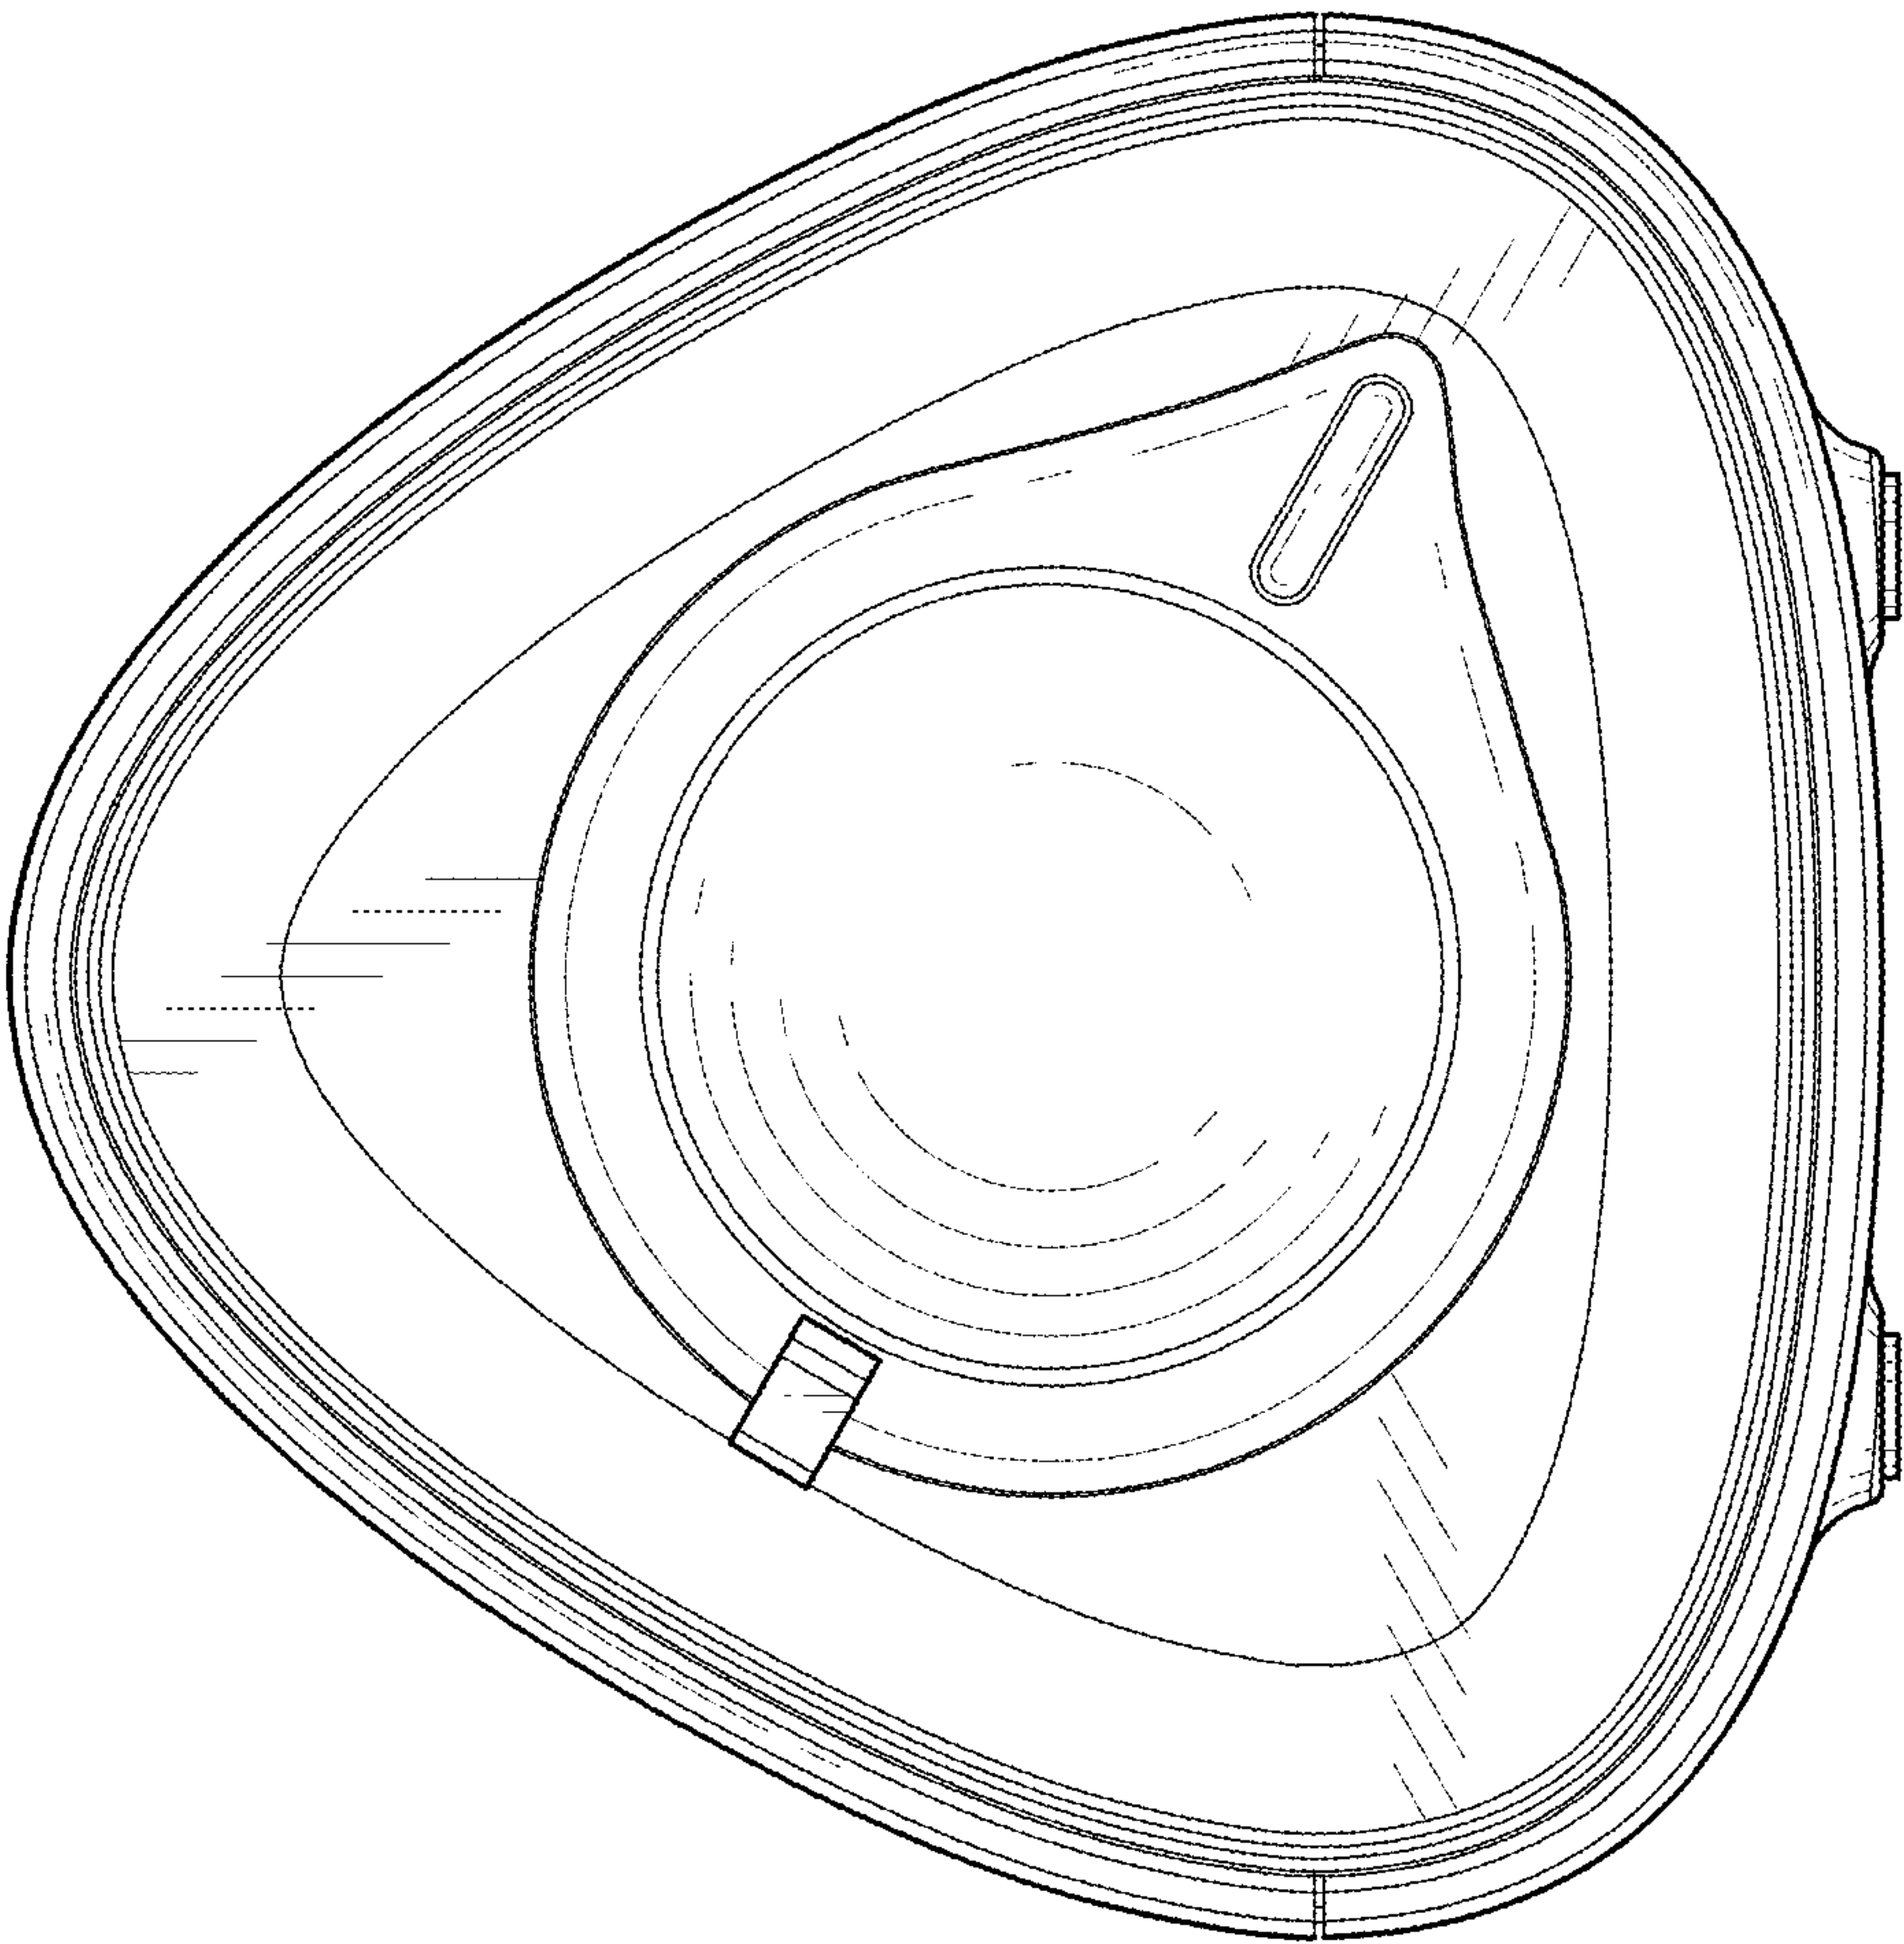


FIG. 5

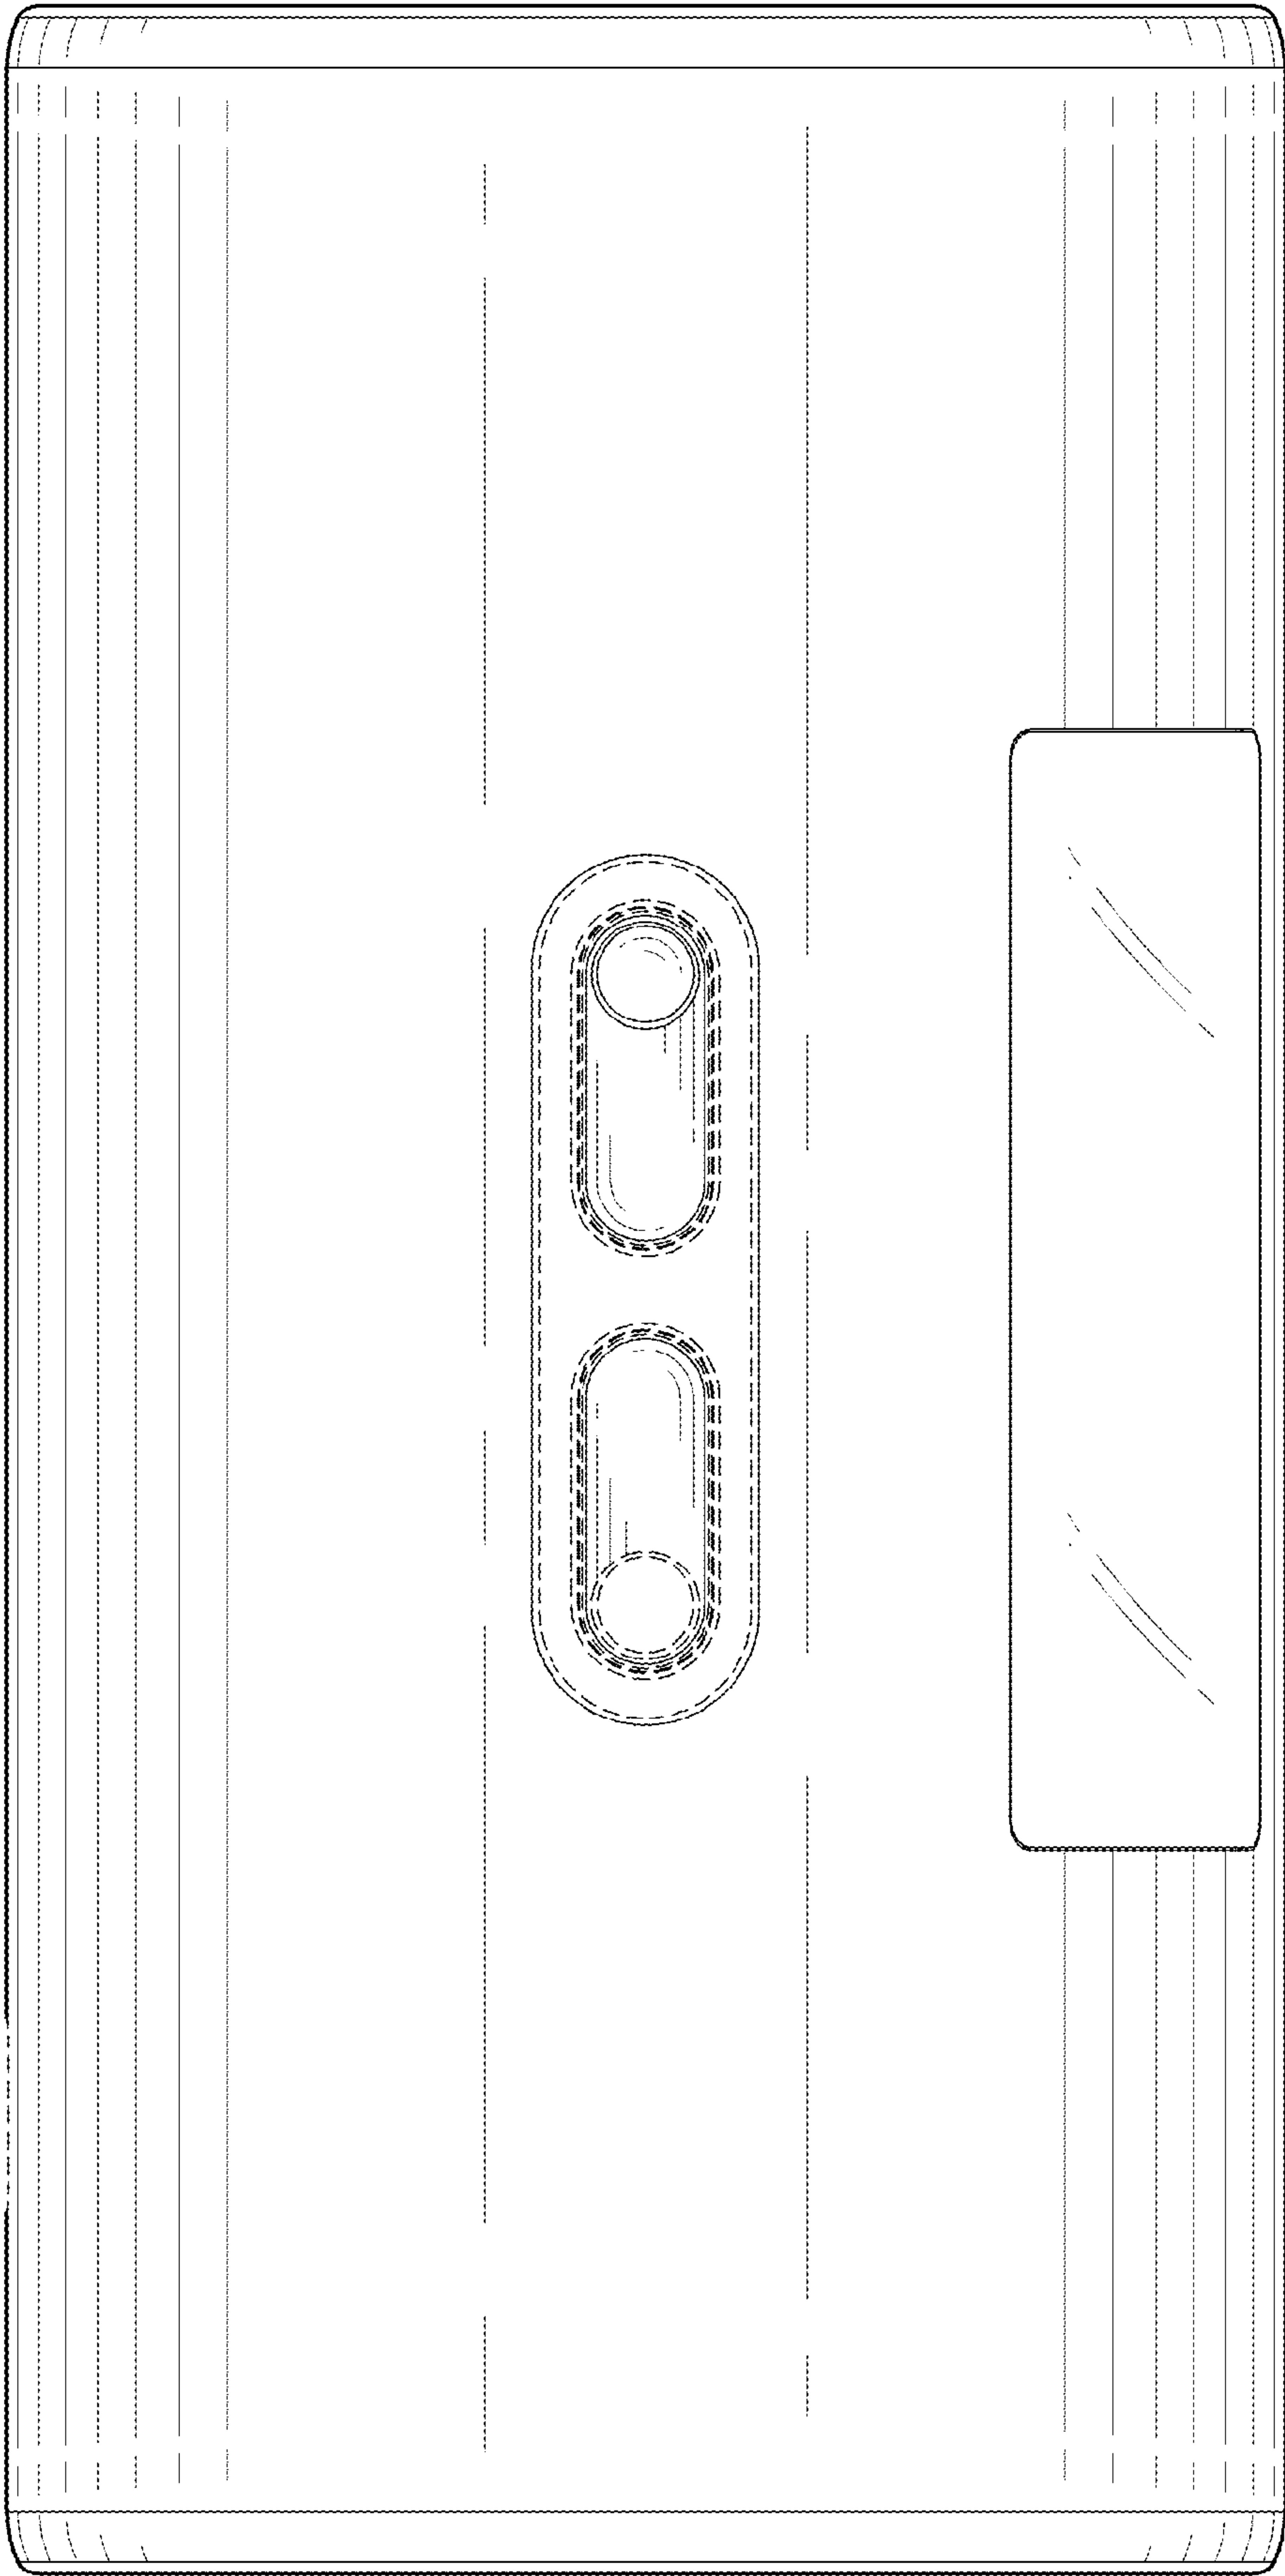


FIG. 6

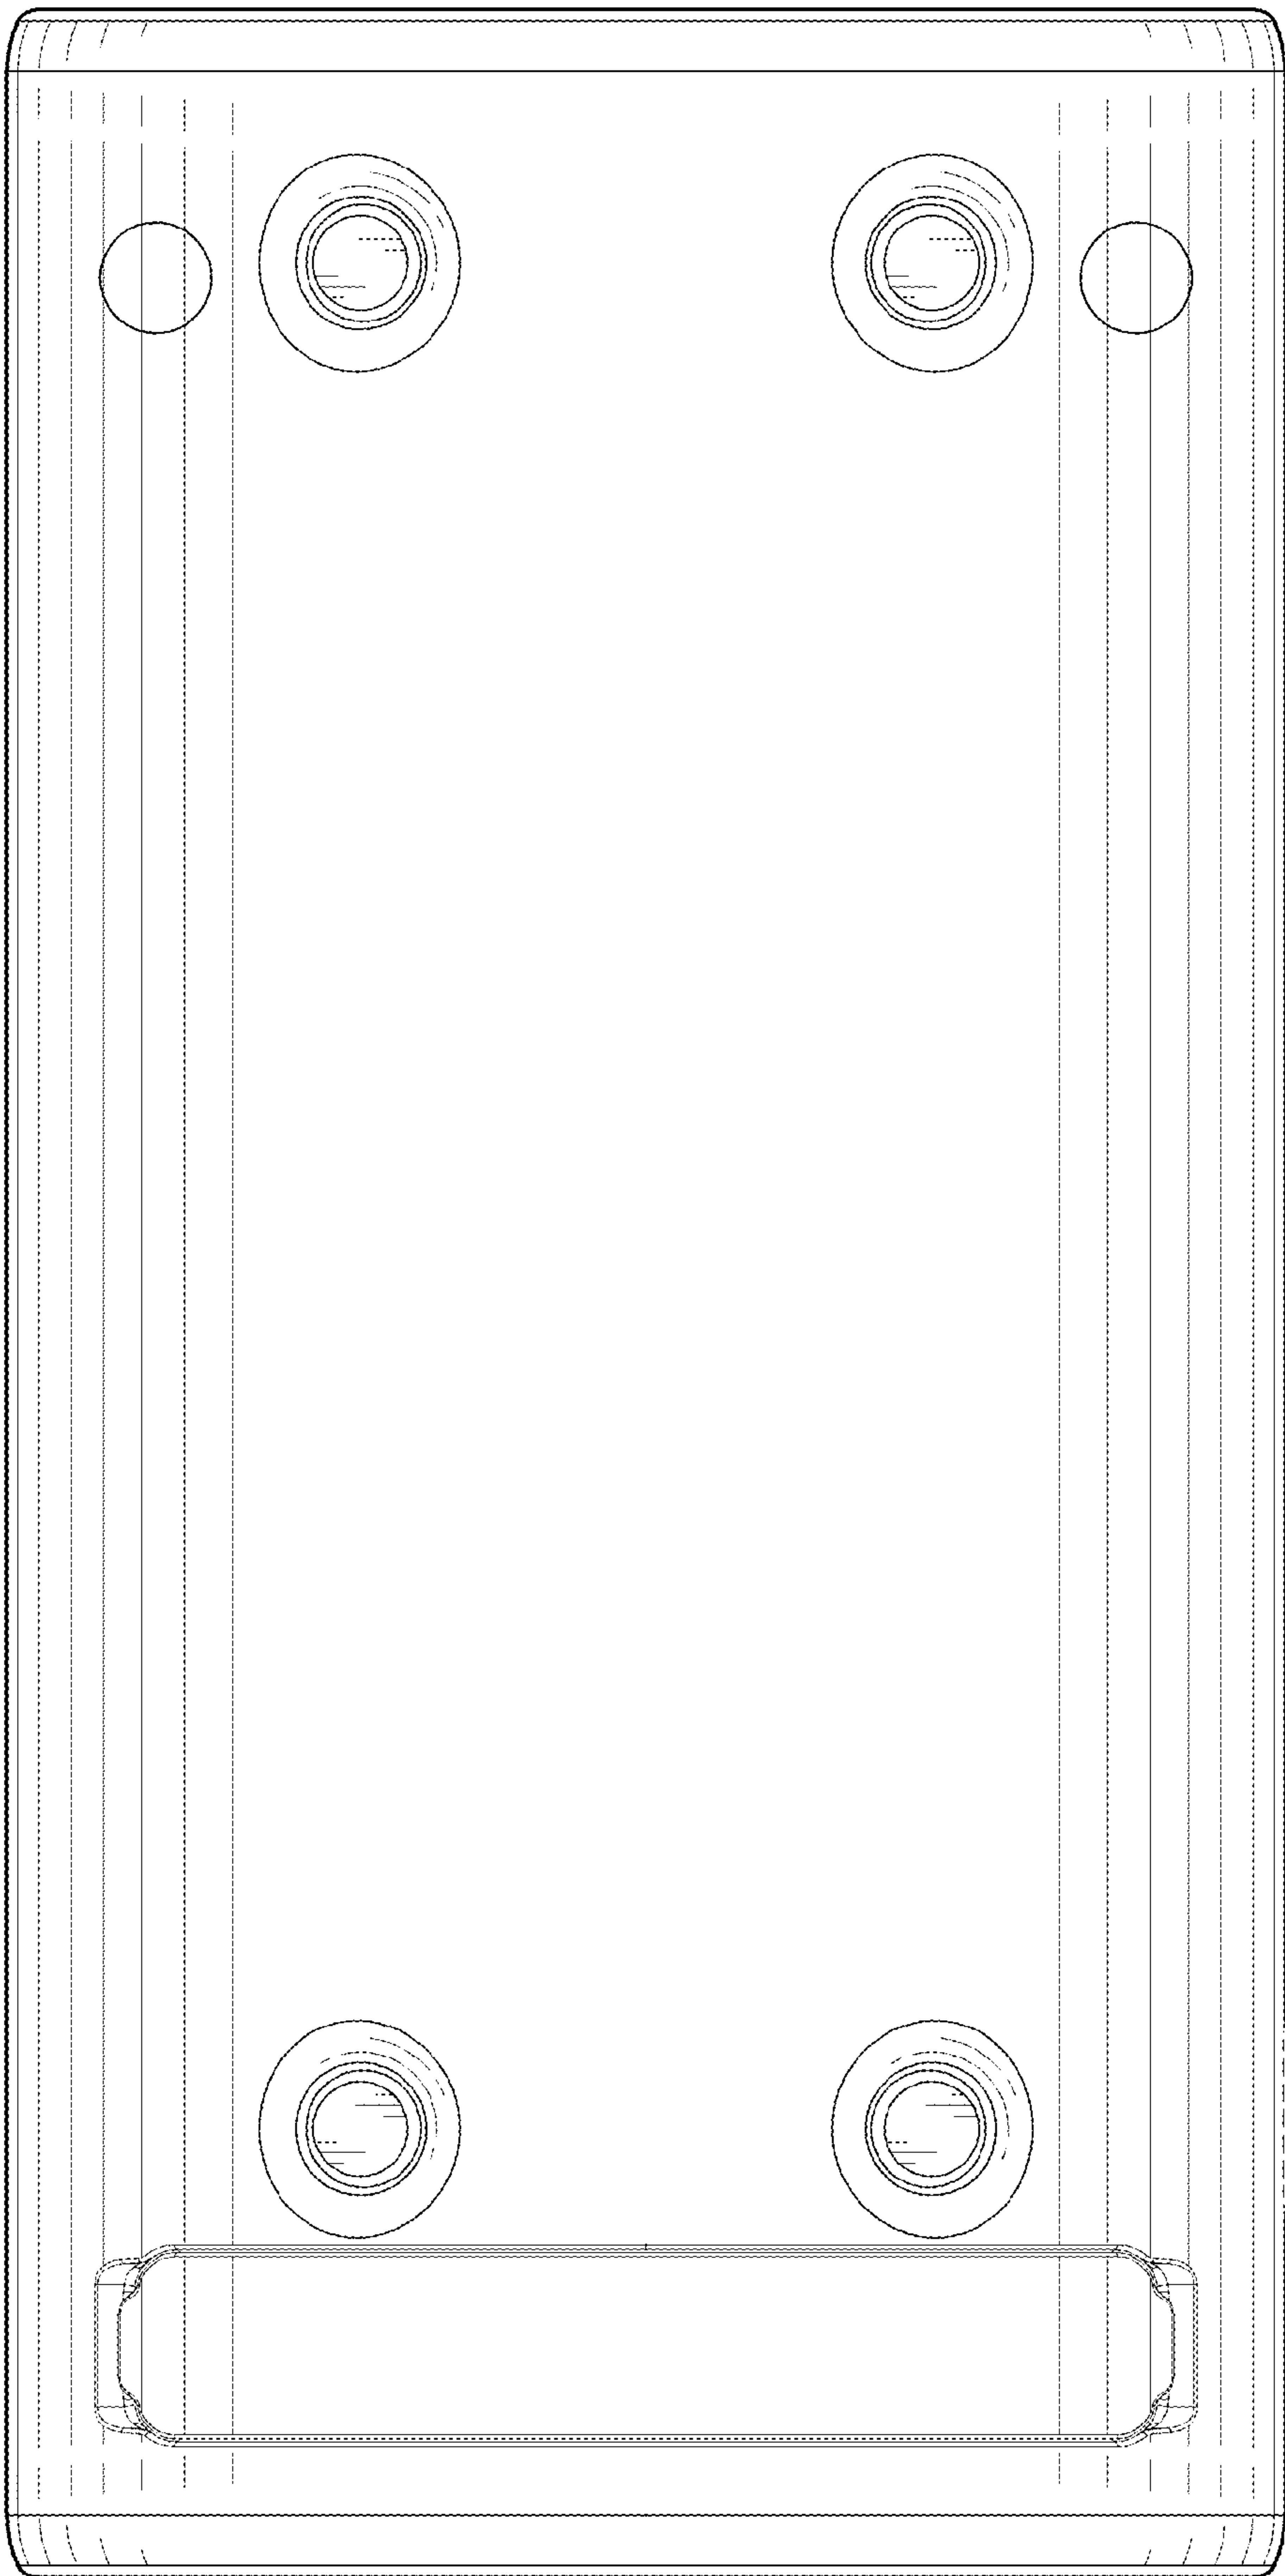


FIG. 7