

US00D958353S

(12)

United States Design Patent

Guimaraes et al.

(10)

Patent No.:

US D958,353 S

(45)

Date of Patent:

** Jul. 19, 2022

(54) CATHETER

(71) Applicant: TERUMO KABUSHIKI KAISHA,
Tokyo (JP)

(72) Inventors: Marcelo Guimaraes, Mount Pleasant,
SC (US); Ryo Okamura, Shizuoka
(JP); Mitsuteru Yasunaga, Shizuoka
(JP)

(73) Assignee: TERUMO KABUSHIKI KAISHA,
Tokyo (JP)

(**) Term: 15 Years

(21) Appl. No.: 29/752,218

(22) Filed: Sep. 25, 2020

(30) Foreign Application Priority Data

Apr. 1, 2020 (JP) 2020-006819
(51) LOC (13) Cl. 24-02
(52) U.S. Cl.
USPC D24/140; D24/130
(58) Field of Classification Search
USPC D24/112–114, 127–131, 133, 140, 146,
D24/108, 186
CPC A61M 25/0108; A61M 2025/09166; A61M
2025/0095; A61M 25/0102
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS
4,838,879 A 6/1989 Tanabe et al.
5,045,072 A * 9/1991 Castillo A61M 25/008
604/529
5,897,537 A * 4/1999 Berg F16L 11/081
604/525
6,036,682 A * 3/2000 Lange A61M 25/0108
604/529
D611,601 S * 3/2010 Tamai D24/140
(Continued)

FOREIGN PATENT DOCUMENTS

EM 008187660-0001 * 11/2020
GB 9007799184-0001 * 4/2020
(Continued)

OTHER PUBLICATIONS

Dr. Vaibhav Jain MD,DNB,MNAMS, “Catheters and Wires,” [Post
date unknown], [Site seen Mar. 3, 2022], Seen at URL: [https://
www.nams-india.in/downloads/cmeevents/ircme/Cathetersandwires_
DrVaibhav.pdf](https://www.nams-india.in/downloads/cmeevents/ircme/Cathetersandwires_DrVaibhav.pdf) (Year: 2022).*
(Continued)

Primary Examiner — Natasha Vujcic
Assistant Examiner — Gilbert B Ford
(74) Attorney, Agent, or Firm — IPUSA, PLLC


(57) CLAIM

We claim, the ornamental design for a catheter, as shown and
described.

DESCRIPTION

FIG. 1 is a front view of a catheter, showing our new design;
FIG. 2 is a rear view thereof;
FIG. 3 is a top plan view thereof;
FIG. 4 is a bottom plan view thereof;
FIG. 5 is a left side view thereof; and,
FIG. 6 is a right side view thereof;
FIG. 7 is a reduced-scale front view showing the catheter in
a wound condition.
The broken lines shown in the drawings represent portions
of the catheter that form no part of the claimed design. The
parallel dash-dot lines in the drawings indicate that the
appearance of any portion of the catheter between the break
lines forms no part of the claimed design.

1 Claim, 5 Drawing Sheets

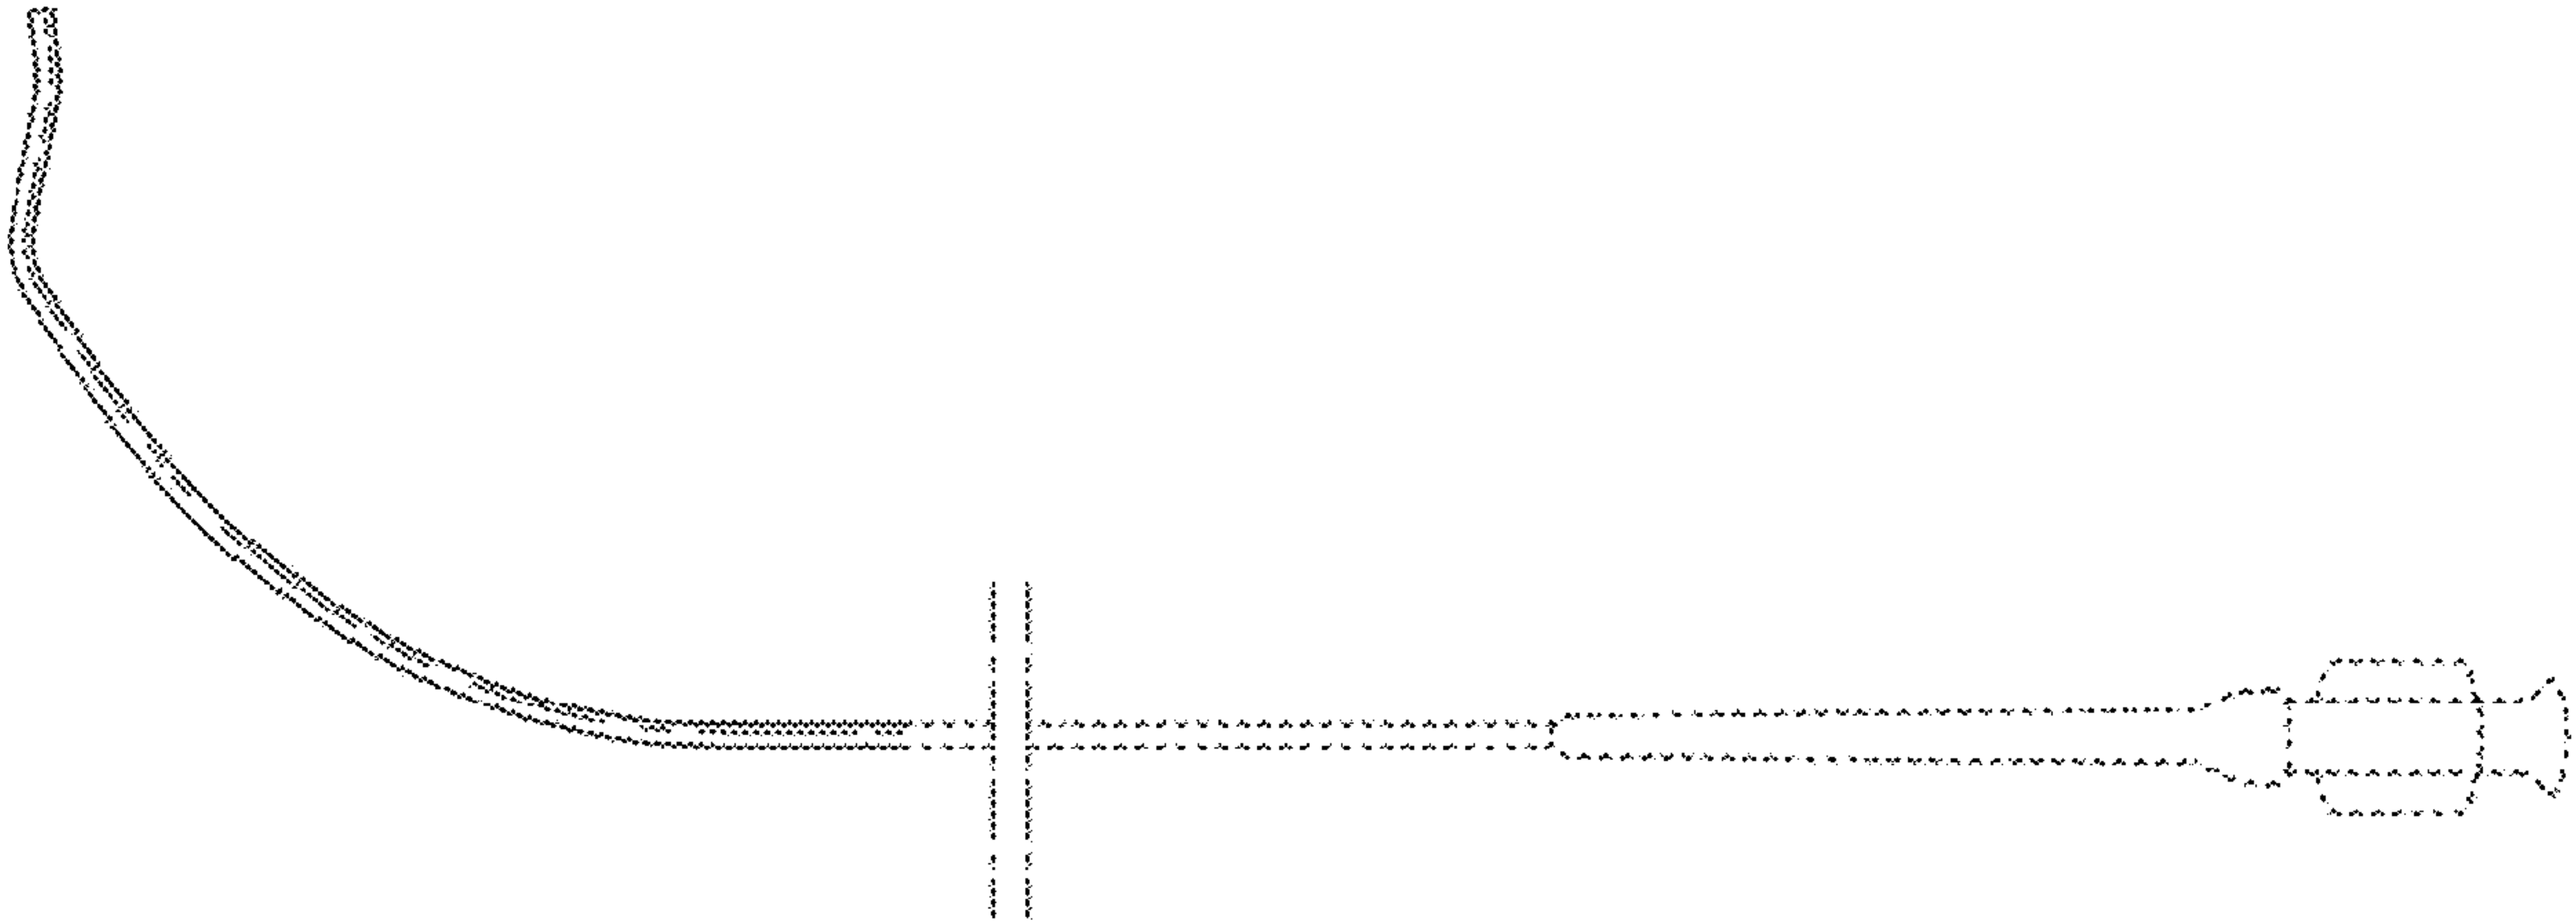

(56)

References Cited

U.S. PATENT DOCUMENTS

D688,797	S	*	8/2013	Nihonmatsu		D24/130
D703,813	S	*	4/2014	Bolia		D24/140
D703,814	S	*	4/2014	Bolia		D24/140
D703,815	S	*	4/2014	Bolia		D24/140
D704,335	S	*	5/2014	Bolia		D24/140
D747,474	S	*	1/2016	Koizumi		D24/130
D755,373	S	*	5/2016	Koizumi		D24/130
D761,959	S	*	7/2016	Wapler		D24/140
D852,353	S	*	6/2019	Paul		D24/127
D858,751	S	*	9/2019	Fischman		D24/112
2004/0171996	A1	*	9/2004	Kiemeneij		A61M 25/0041 604/264
2013/0281850	A1	*	10/2013	Okajima		A61M 25/065 600/433
2019/0117938	A1	*	4/2019	Norman		A61M 25/0052
2019/0159878	A1	*	5/2019	Wasty		A61M 25/0905

FOREIGN PATENT DOCUMENTS

JP	S62-261371		11/1987
JP	D1510449	*	4/2013
JP	D1701218	*	11/2021

OTHER PUBLICATIONS

“What is your primary choice for RadialFirst and FemoralAccess diagnostic catheters?”, youngNIR, Twitter, [Post date: Oct. 8, 2019], [Site seen Mar. 3, 2022], Seen at URL: <https://twitter.com/youngnir/status/1181509668184772608> (Year: 2019).*

“Tools of the Trade” Radiology Key: Fastest Radiology Insight Engine, [Post date unknown], [Site seen Mar. 3, 2022], Seen at URL: <https://radiologykey.com/tools-of-the-trade/> (Year: 2022).*

U.S. Appl. No. 29/752,211, filed Sep. 25, 2020, Terumo Kabushiki Kaisha.

U.S. Appl. No. 29/752,223, filed Sep. 25, 2020, Terumo Kabushiki Kaisha.

U.S. Appl. No. 29/752,208, filed Sep. 25, 2020, Terumo Kabushiki Kaisha.

U.S. Appl. No. 29/752,201, filed Sep. 25, 2020, Terumo Kabushiki Kaisha.

U.S. Appl. No. 29/752,220, filed Sep. 25, 2020, Terumo Kabushiki Kaisha.

U.S. Appl. No. 29/752,209, filed Sep. 25, 2020, Terumo Kabushiki Kaisha.

U.S. Appl. No. 29/752,215, filed Sep. 25, 2020, Terumo Kabushiki Kaisha.

Office Action dated Feb. 2, 2021 (Japanese Design Application No. 2020-009539).

Office Action dated Dec. 1, 2020 (Japanese Design Application No. 2020-006818).

Office Action dated Dec. 1, 2020 (Japanese Design Application No. 2020-006820).

Office Action dated Dec. 1, 2020 (Japanese Design Application No. 2020-009538).

Office Action dated Dec. 1, 2020 (Japanese Design Application No. 2020-009539).

Office Action dated Dec. 1, 2020 (Japanese Design Application No. 2020-009540).

Francesco Burzotta “Diagnostic and Guide Catheter Choices and Manipulation from the Radial Artery for Native and Graft Vessels”, Design of catheter tip listed as “BARBEAU” in f-201111 <URL:<https://www.slideshare.net/theradialist/burzotta>> Jan. 6, 2012 (With Partial Translation).

Francesco Burzotta “Diagnostic and Guide Catheter Choices and Manipulation from the Radial Artery for Native and Graft Vessels”, Design of catheter tip listed as “JACKY” in f-201111 <URL:<https://www.slideshare.net/theradialist/burzotta>> Jan. 6, 2012 (With Partial Translation).

Guido Sandulli “Merit Medical—Merit Medical’s Concierge Guiding Catheter Now Available in Radial-Specific Shapes”, Design of the lowest catheter tip as described in <URL:<https://www.merit.com/articles/merit-medicals-concierge-guiding-catheter-now-available-in-radial-specific-forms/>> Mar. 24, 2015 (With Partial Translation).

Guido Sandulli “Merit Medical—Merit Medical’s Concierge Guiding Catheter Now Available in Radial-Specific Shapes”, Design of the second lowest catheter tip as described in <URL:<https://www.merit.com/articles/merit-medicals-concierge-guiding-catheter-now-available-in-radial-specific-forms/>> Mar. 24, 2015 (With Partial Translation).

* cited by examiner

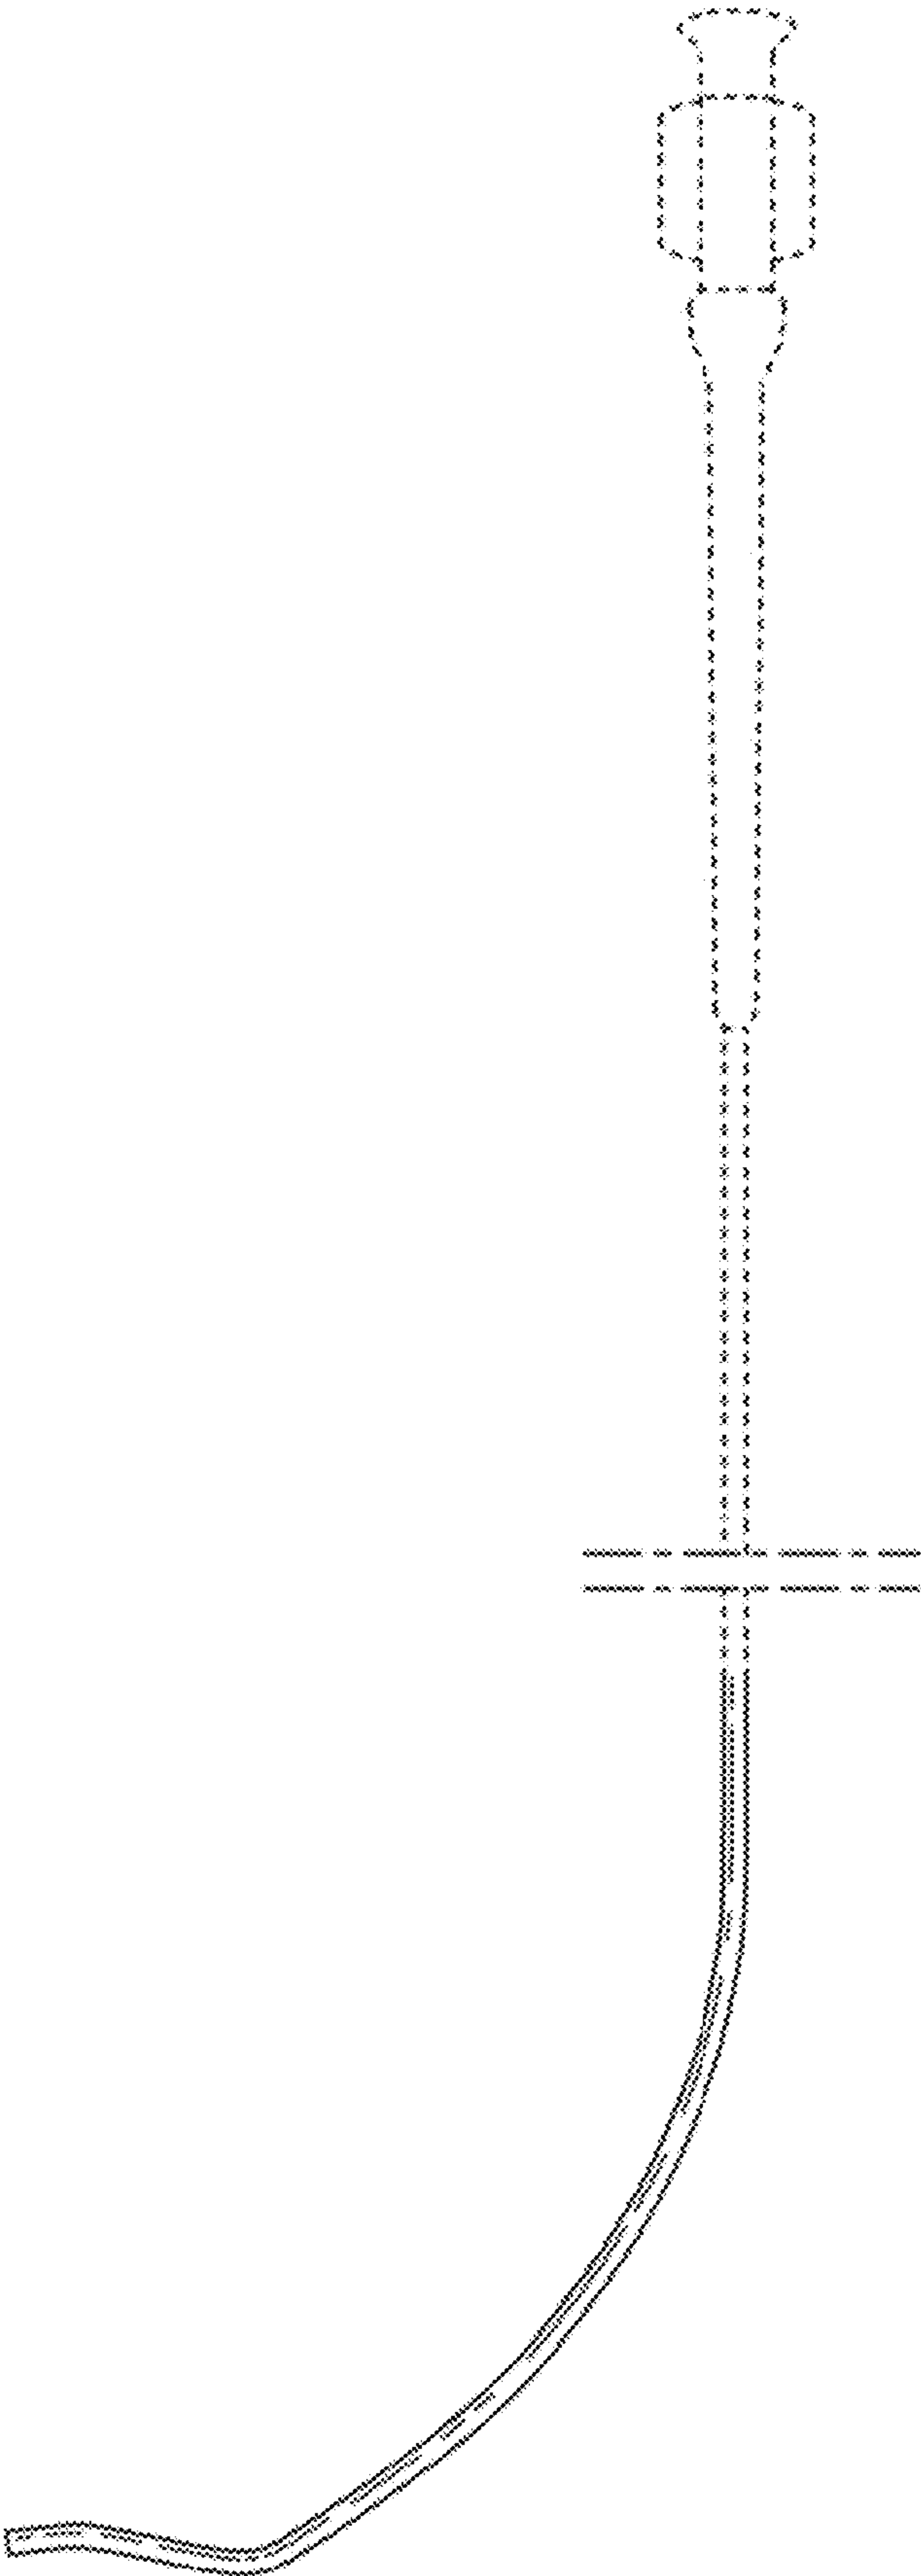


Fig. 1

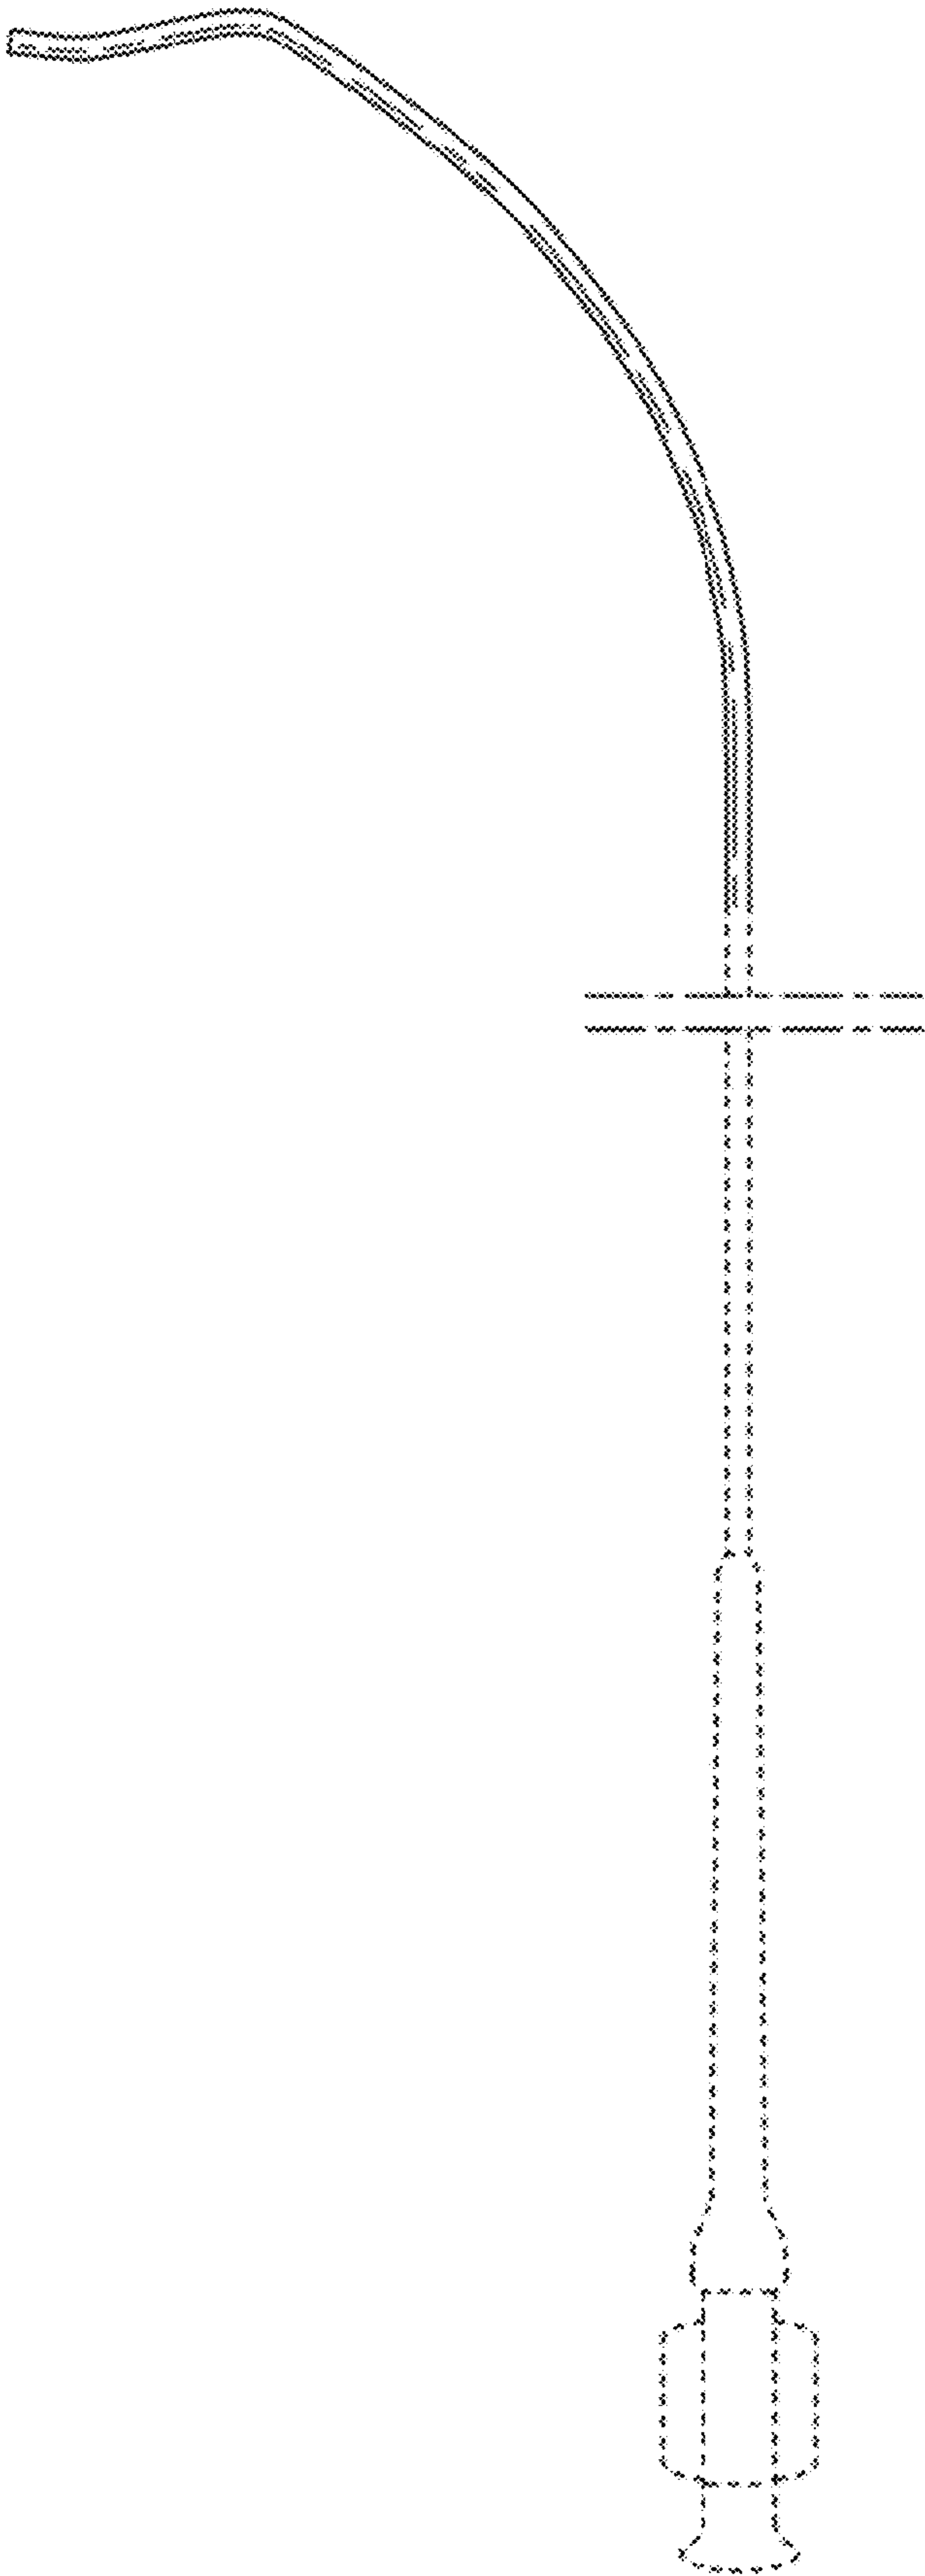


Fig. 2

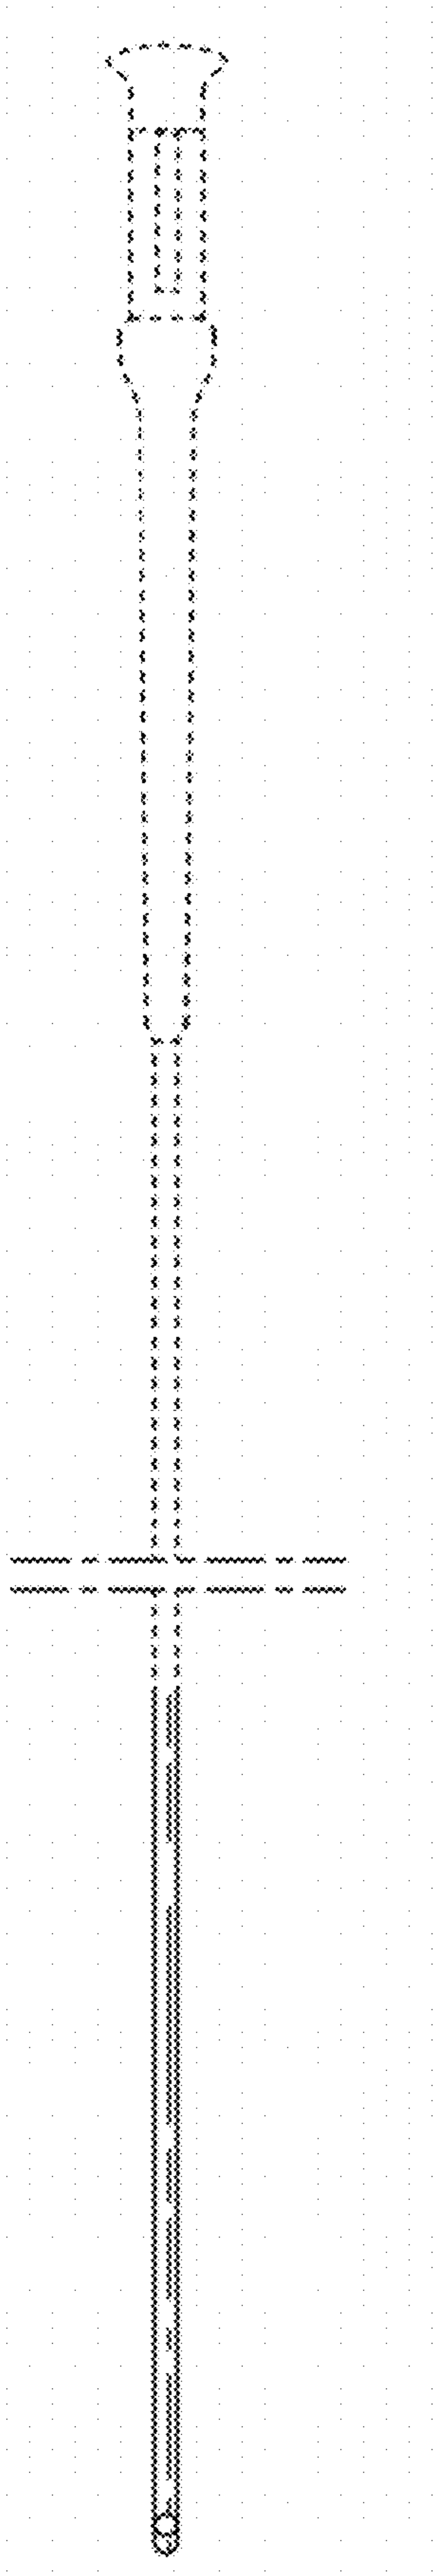


Fig. 3

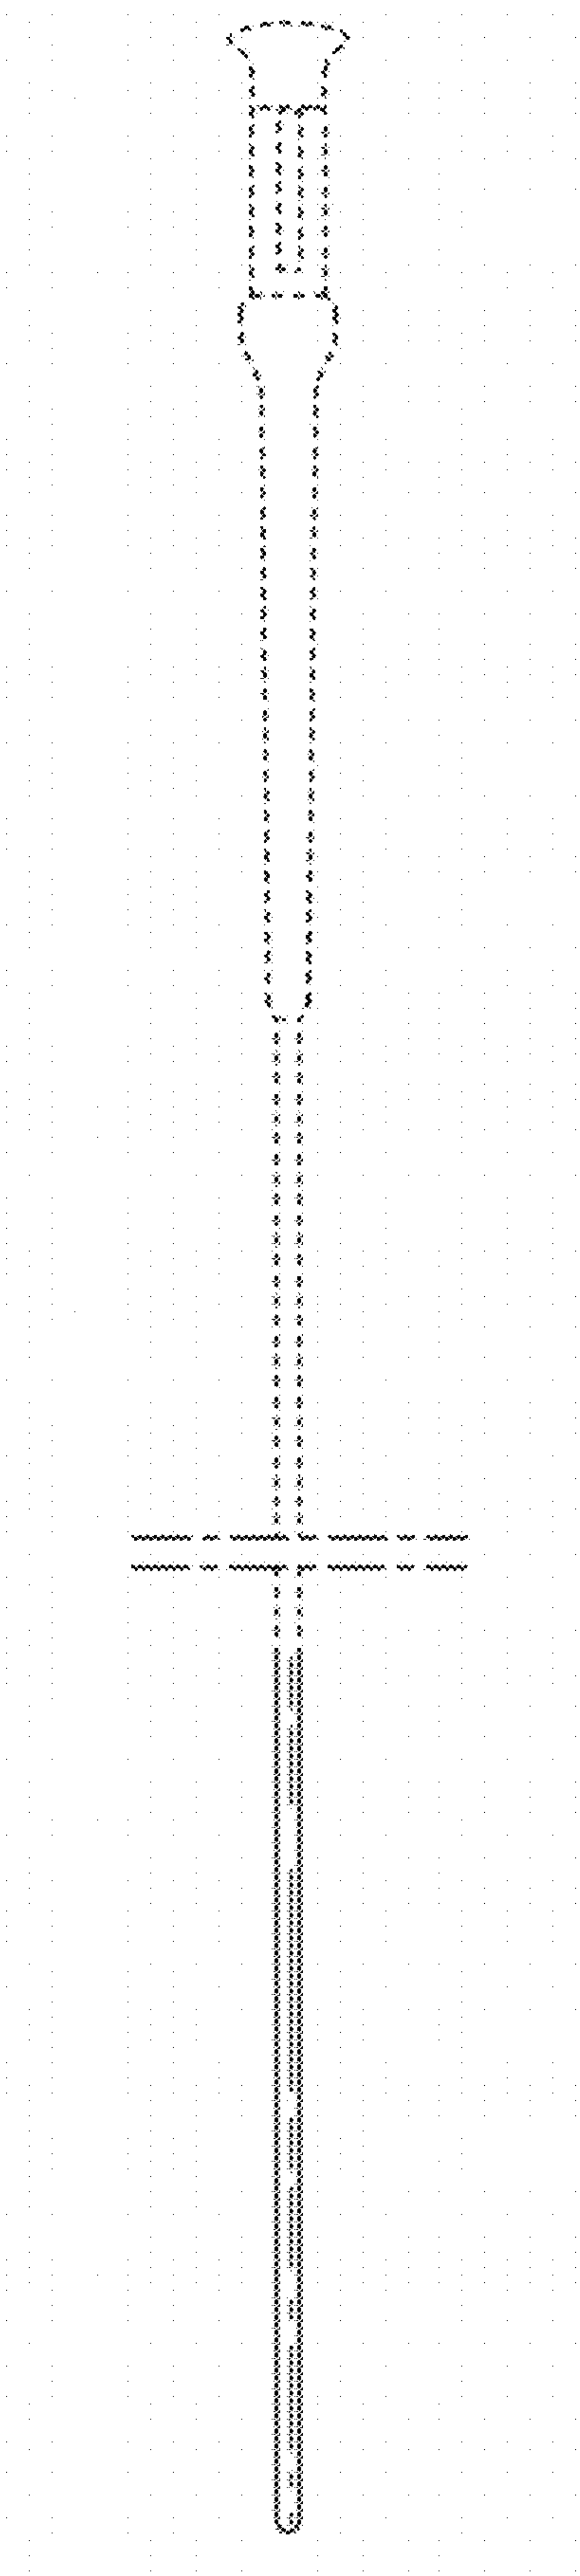


Fig. 4



Fig. 6

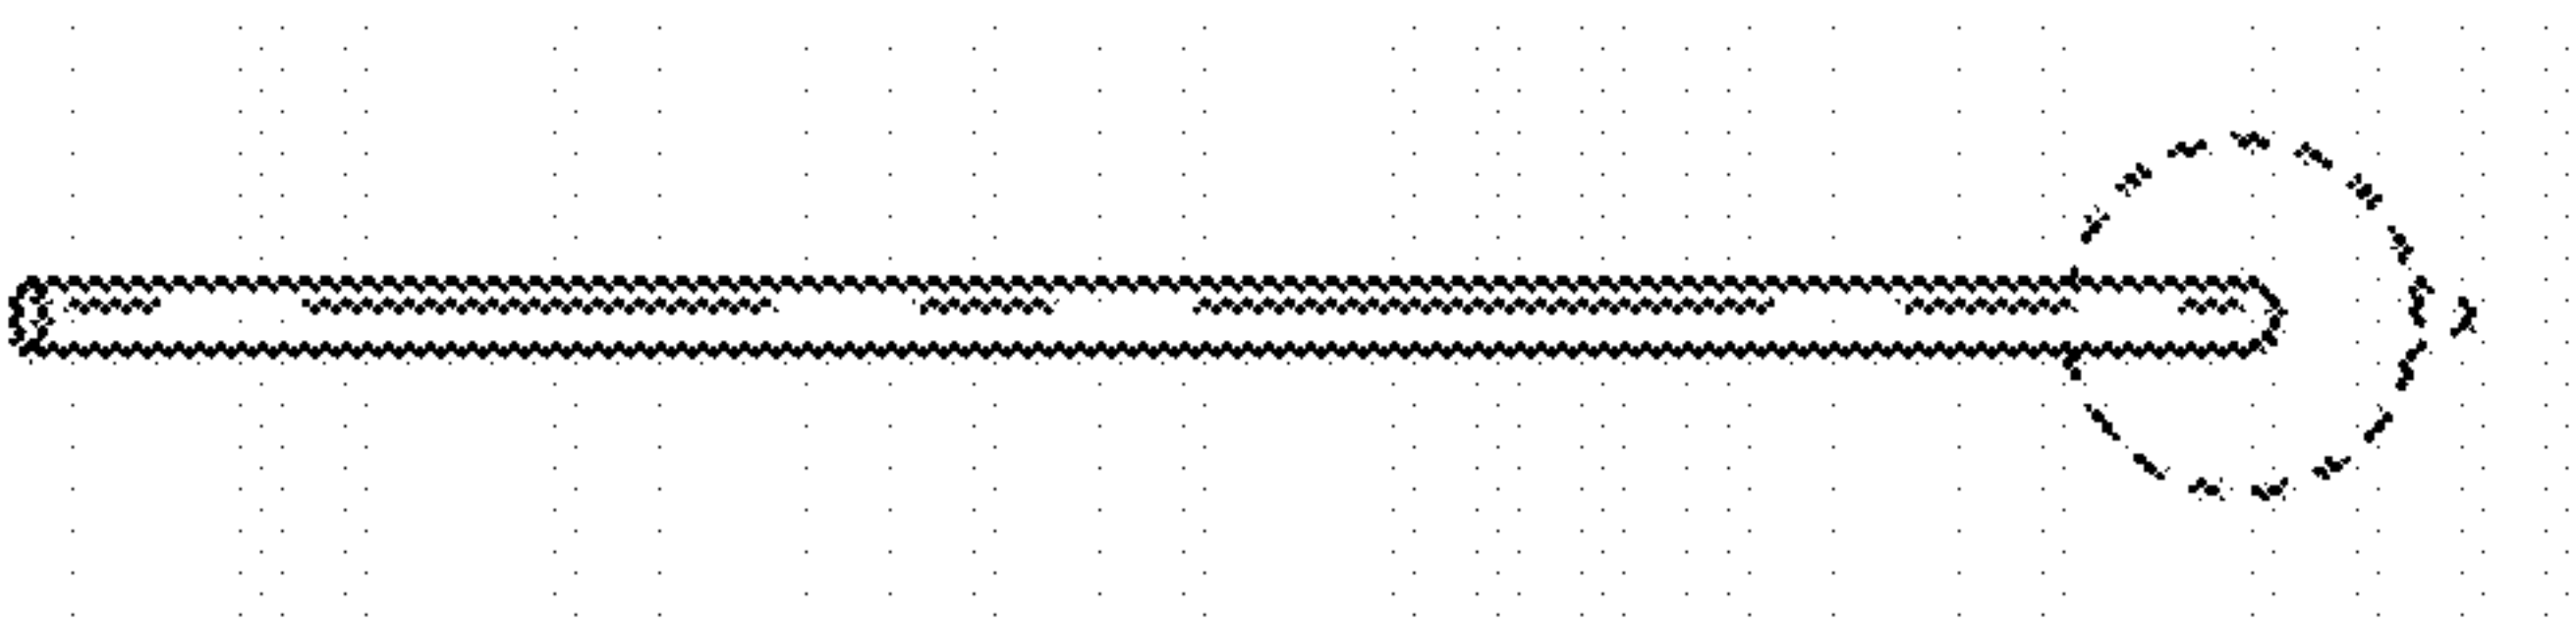


Fig. 5

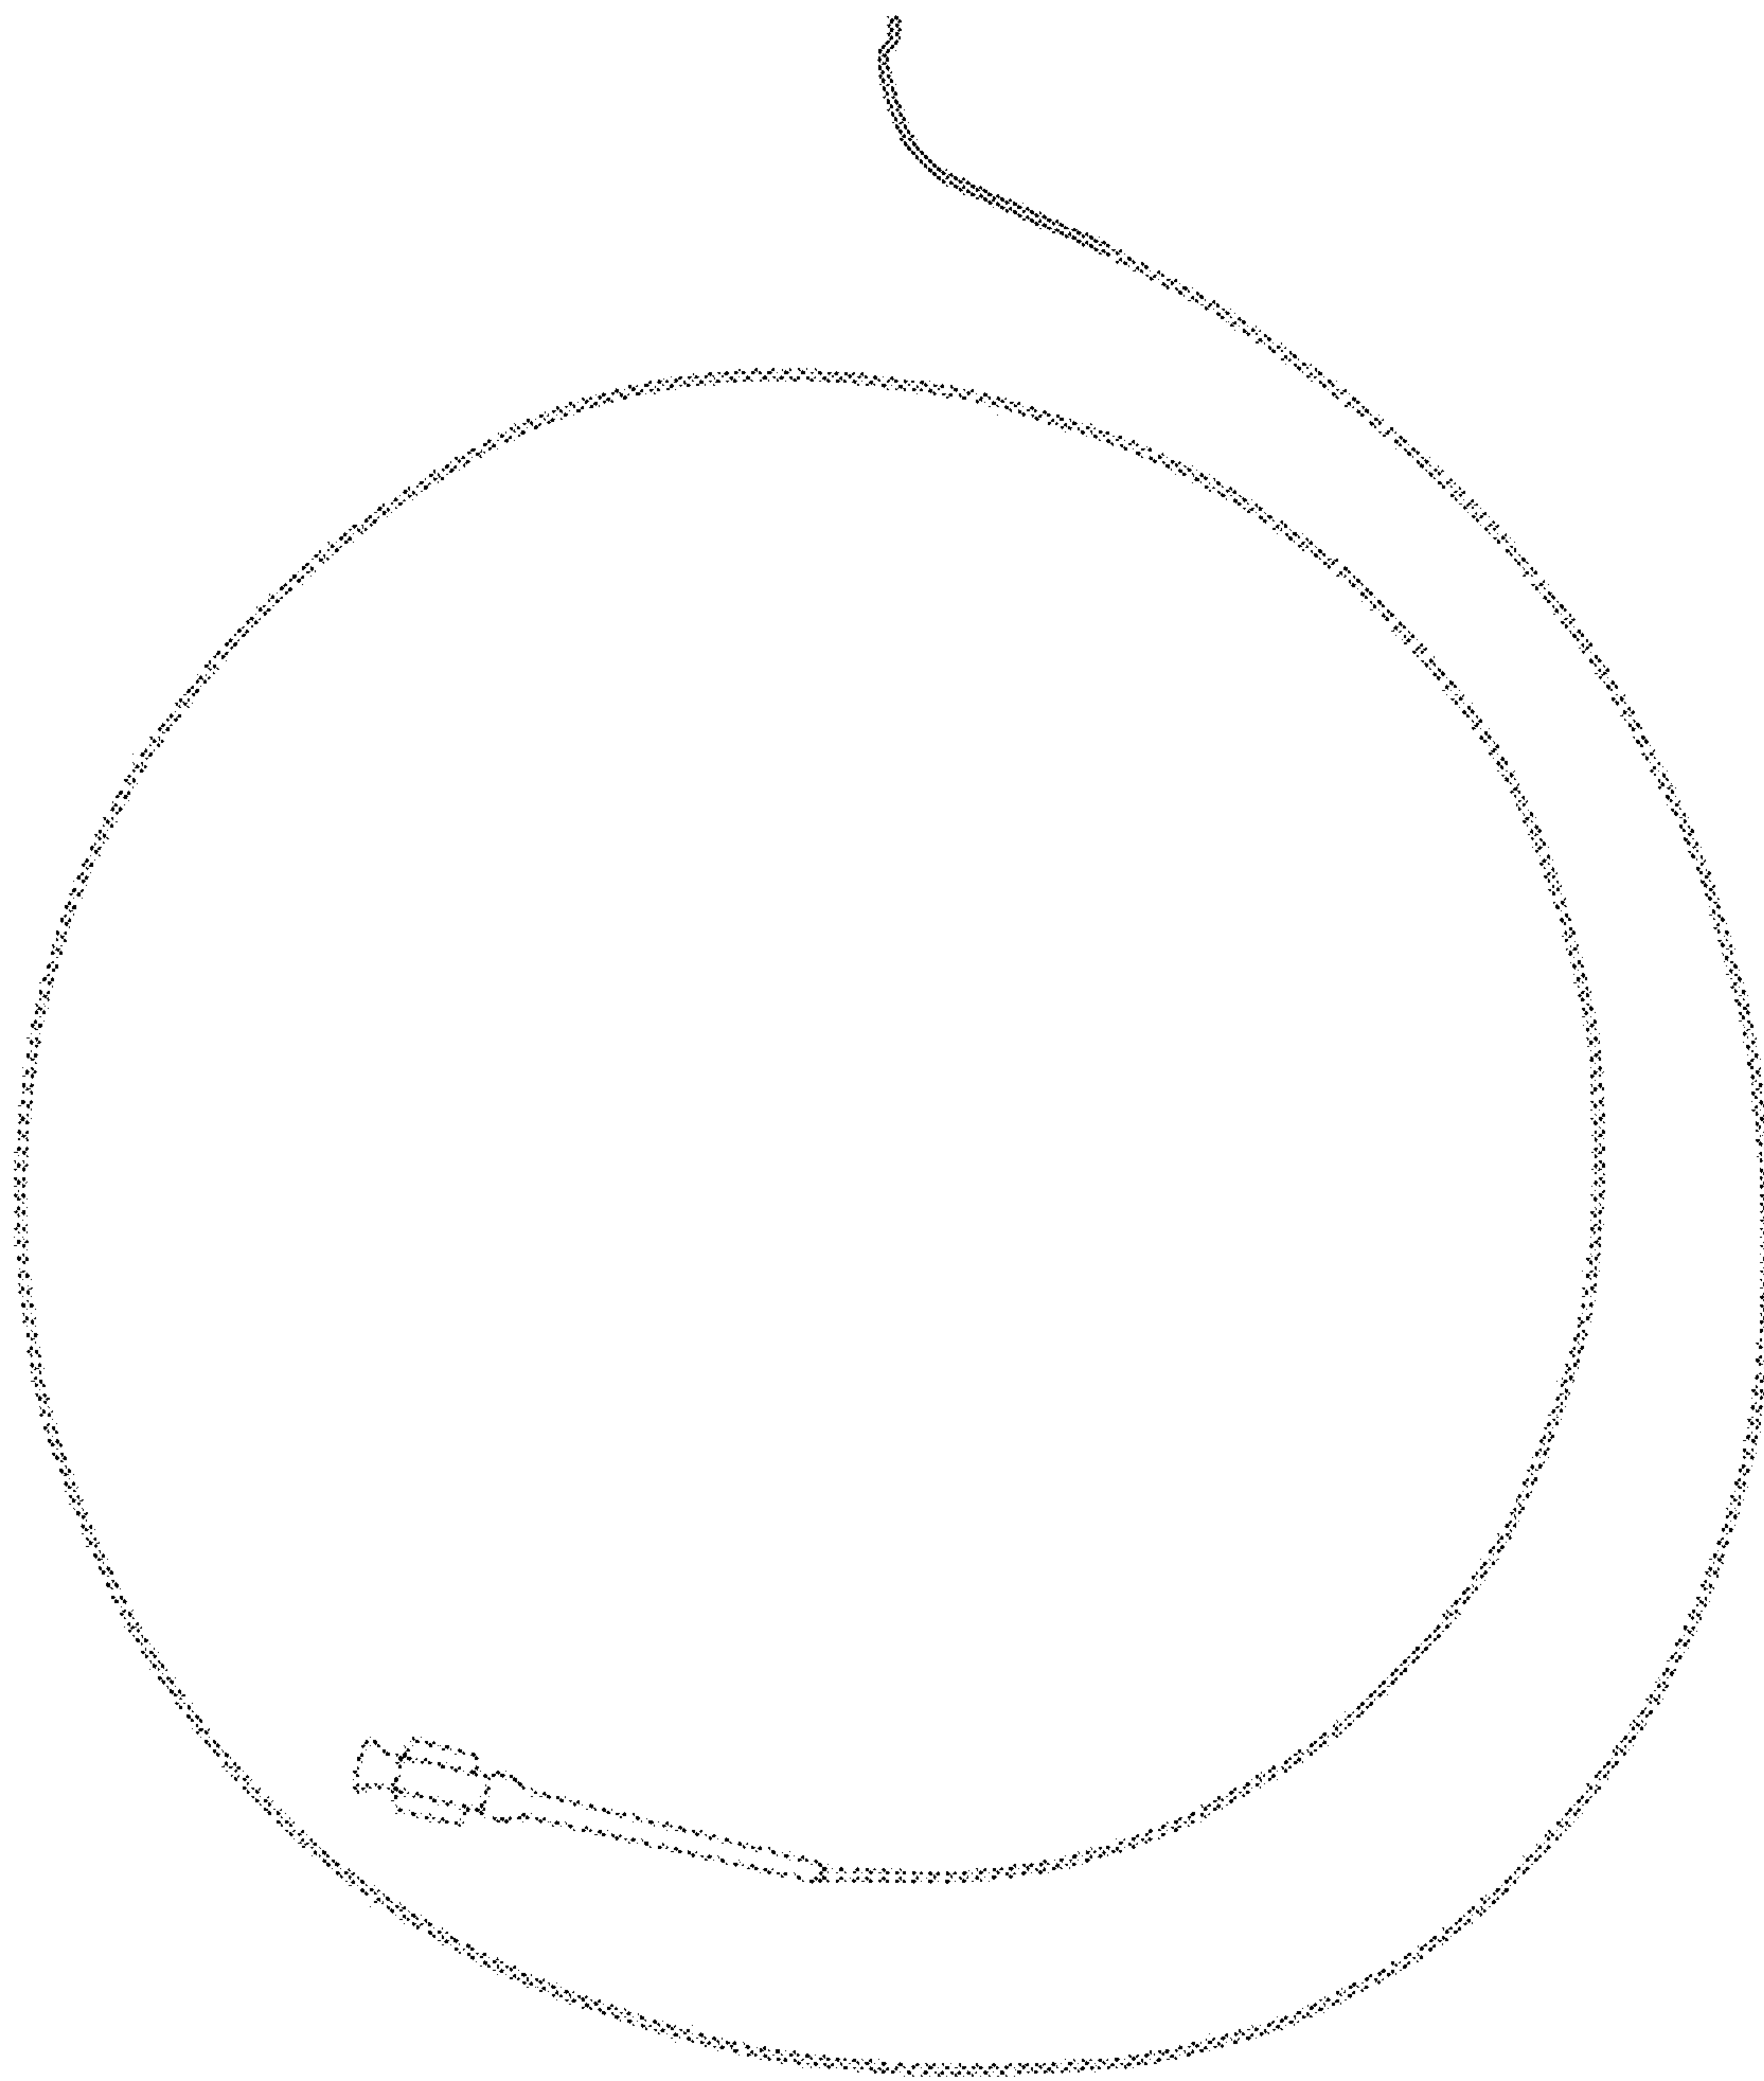


Fig. 7