



US00D958991S

(12) **United States Design Patent** (10) **Patent No.:** **US D958,991 S**  
**Dacosta et al.** (45) **Date of Patent:** **\*\* Jul. 26, 2022**

(54) **HANDHELD MULTI-MODAL IMAGING DEVICE**

(56) **References Cited**

U.S. PATENT DOCUMENTS


(71) Applicant: **SBI ALAPHARMA CANADA, INC.**,  
Toronto (CA)  
(72) Inventors: **Ralph S. Dacosta**, Toronto (CA);  
**Kathryn Ottolino-Perry**, Toronto  
(CA); **Christopher Gibson**, Toronto  
(CA); **Nayana Thalanki Anantha**,  
Toronto (CA); **Simon Treadwell**,  
Toronto (CA); **Connor Wright**, Toronto  
(CA); **Kimberlyn Dampitan**,  
Mississauga (CA); **Todd Daynes**,  
Aurora (CA); **Todd Meaney**, Thornhill  
(CA)  
(73) Assignees: **SBI ALAPHARMA CANADA, INC.**,  
Toronto (CA); **UNIVERSITY**  
**HEALTH NETWORK**, Toronto (CA)

(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/767,874**  
(22) Filed: **Jan. 26, 2021**

**Related U.S. Application Data**

(62) Division of application No. 29/677,154, filed on Jan.  
17, 2019, now Pat. No. Des. 910,182.  
(51) **LOC (13) Cl.** ..... **24-01**  
(52) **U.S. Cl.**  
USPC ..... **D24/158; D24/186**  
(58) **Field of Classification Search**  
USPC ..... D24/107, 158-161, 185, 186, 187, 137,  
D24/138; D14/426; D10/78; D16/202,  
D16/206  
CPC ... A61B 8/0808; A61B 8/4455; A61B 8/4472;  
A61B 8/4483; A61B 8/483; A61B  
5/0075; A61B 5/14553  
See application file for complete search history.

6,601,997 B2	8/2003	Ngo	
D480,478 S	10/2003	Leonard et al.	
D515,214 S *	2/2006	Jackson, III	D24/176
D569,378 S *	5/2008	Wanamaker	D14/426
D585,554 S	1/2009	Suzuki	
D610,178 S	2/2010	Adolfsson et al.	
7,846,091 B2	12/2010	Fulghum	
D636,424 S	4/2011	Lin	
D658,298 S	4/2012	Prpa	
D677,793 S	3/2013	Prpa	
D701,606 S *	3/2014	Ohmukai	D24/187
D703,331 S *	4/2014	Kitayama	D24/187
D703,333 S *	4/2014	Saeki	D24/187
D724,234 S *	3/2015	Hagege	D24/200
9,042,967 B2	5/2015	Dacosta et al.	
D733,595 S	7/2015	Hoshino	
D747,391 S	1/2016	Sakai	
D748,808 S *	2/2016	Matsumura	D24/187
D750,260 S *	2/2016	Sauer	D24/186
D753,308 S	4/2016	Marinkovich et al.	
9,451,882 B2	9/2016	Nie et al.	
D787,684 S	5/2017	Vezina	
D802,777 S *	11/2017	Burachynsky	D24/187
D810,293 S *	2/2018	Peel	D24/152
D822,747 S	7/2018	Van Deusen et al.	
D822,748 S	7/2018	Van Deusen et al.	
D827,014 S	8/2018	Sakai	
D835,271 S	12/2018	Myers et al.	
D849,105 S	5/2019	Hogstedt et al.	
D859,498 S	9/2019	Lin	
D861,176 S	9/2019	Yoon et al.	
D861,764 S	10/2019	Zhao	
D862,697 S *	10/2019	Kenworthy	D24/158
10,438,356 B2	10/2019	Dacosta	
D865,836 S	11/2019	Puusaari	
D865,845 S	11/2019	Sakai	
D866,764 S *	11/2019	Pukall	D24/152
D868,867 S	12/2019	Jean et al.	
D873,890 S	1/2020	Fidler	
D907,097 S	1/2021	Suurmeijer et al.	
D908,161 S	1/2021	Dacosta et al.	
D908,881 S	1/2021	Dacosta et al.	
D921,736 S	1/2021	Yin	
D910,105 S	2/2021	Lin	
D910,182 S *	2/2021	Dacosta	D24/158
D913,354 S	3/2021	Marzette, Jr. et al.	
D914,220 S	3/2021	Nelson et al.	
D916,294 S	4/2021	Murray et al.	
D919,690 S	5/2021	Suurmeijer et al.	

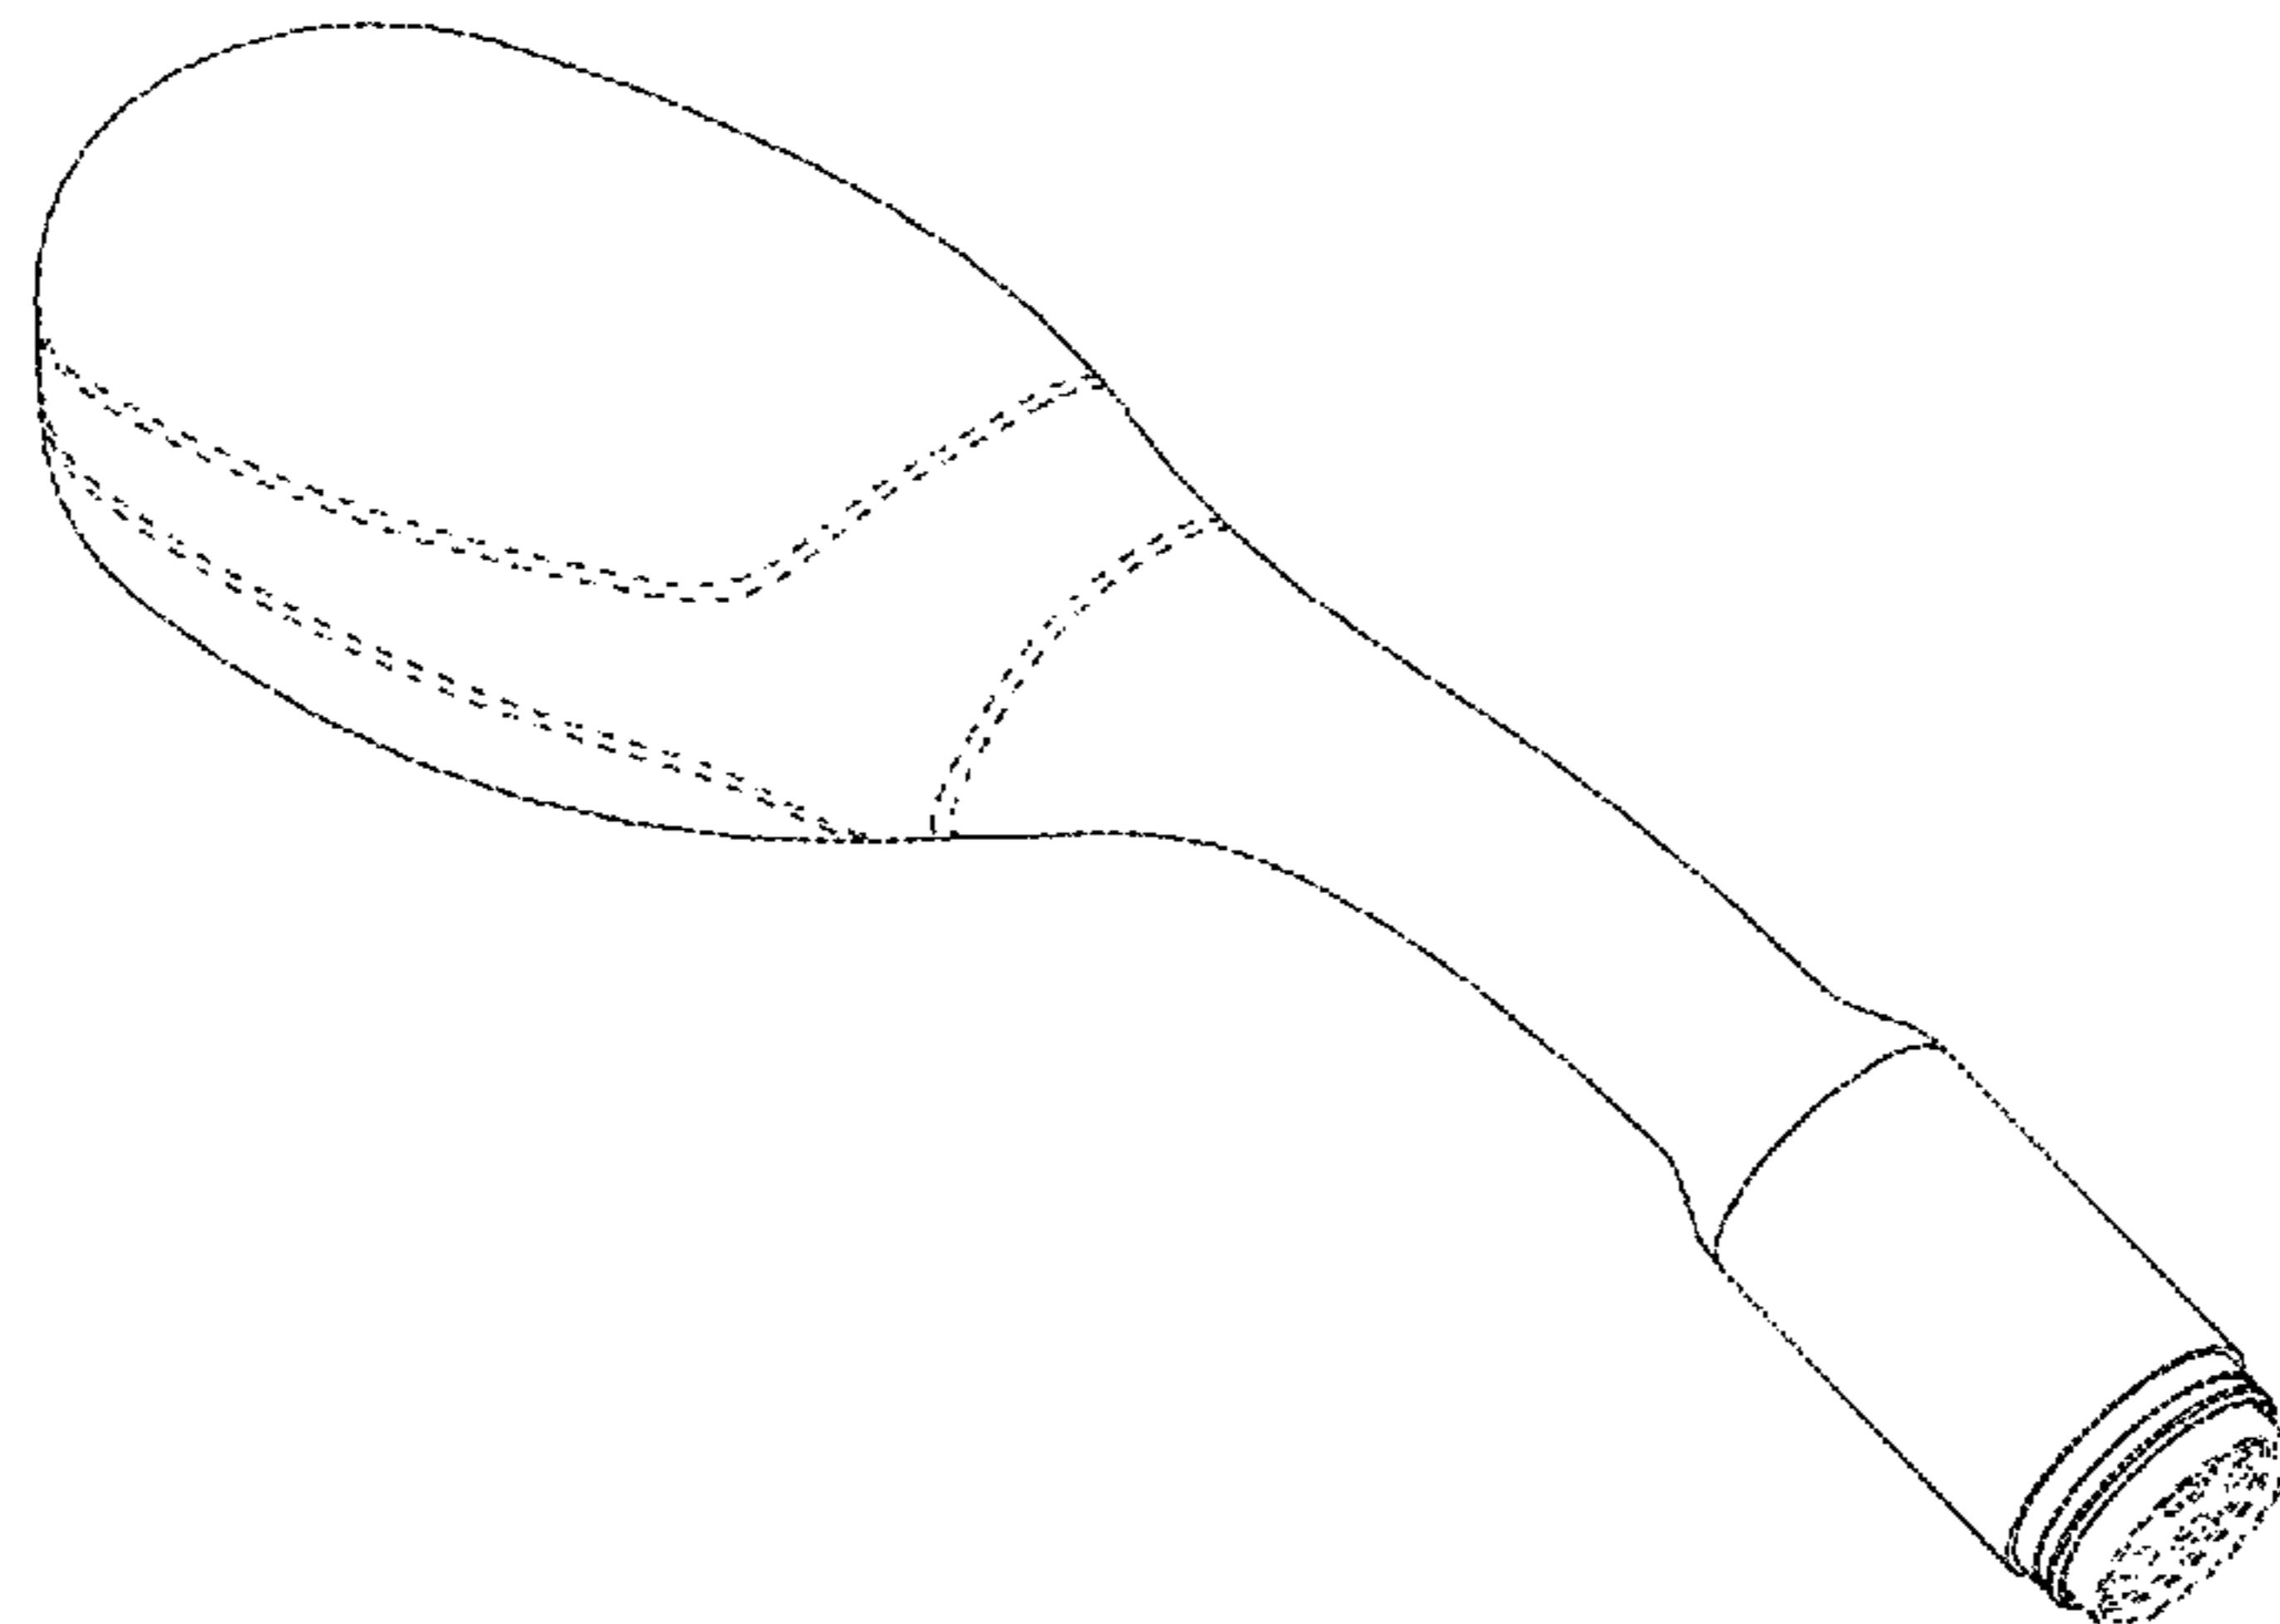

D921,899 S	6/2021	Suarez et al.
D922,469 S	6/2021	Sjogren et al.
D924,306 S	7/2021	Melnicoff
2006/0004292 A1	1/2006	Beylin
2010/0145146 A1	6/2010	Melder
2014/0180116 A1	6/2014	Lindekugel et al.
2014/0276102 A1	9/2014	Lee et al.
2015/0182196 A1	7/2015	Ninomiya et al.
2016/0045114 A1	2/2016	Dacosta et al.
2016/0287211 A1	10/2016	DaCosta et al.
2017/0290515 A1	10/2017	Butte et al.
2018/0242848 A1	8/2018	Dacosta et al.
2018/0279864 A1	10/2018	Frangioni

FOREIGN PATENT DOCUMENTS

EP	2502551	9/2012
EP	3372143	9/2018
WO	2017079844	5/2017
WO	2019148268	8/2019
WO	2019213737	11/2019
WO	2020148724	7/2020
WO	2020148725	7/2020
WO	2020148726	7/2020

OTHER PUBLICATIONS

U.S. Appl. No. 62/793,842, filed Jan. 17, 2019.  
 U.S. Appl. No. 62/793,846, filed Jan. 17, 2019.  
 U.S. Appl. No. 62/857,183, filed Jun. 4, 2019.  
 Design U.S. Appl. No. 29/676,901, filed Jan. 15, 2019.  
 Design U.S. Appl. No. 29/677,152, filed Jan. 17, 2019.  
 International Search Report and Written Opinion from International Patent Application No. PCT/CA2019/000015, dated Jun. 4, 2019.  
 “Fluorescent chemical probes for accurate tumor diagnosis and targeting therapy”, 2017, Gao et al. <https://www.researchgate.net/publication/315469453> Fluorescent chemical probes for accurate tumor diagnosis and targeting therapy.  
 “Current concepts and future perspectives on surgical optical imaging in cancer”, 2010, Ntziachristos et al, <https://www.sniedigitallibrary.org/Mournals/Journal-of-Biomedical-Optics-volume-15issue-61066024/Current-concepts-and-future-perspectives-on-surgical-optical-imaging-in/10.1117/1.3523364.full7SSO=1>.  
 Notice of Allowance in Design U.S. Appl. No. 29/677,154, dated Apr. 1, 2020.  
 Notice of Allowance in Design U.S. Appl. No. 29/677,152, dated Apr. 1, 2020.  
 Ex Parte Quayle Action in Design U.S. Appl. No. 29/676,901, dated Mar. 5, 2020.  
 Notice of Allowance in Design U.S. Appl. No. 29/676,901, dated Jun. 4, 2020.  
 International Search Report and Written Opinion from International Patent Application No. PCT/IB2020/050384 dated Apr. 22, 2020.  
 International Patent Application No. PCT/IB2020/050384, dated Jan. 17, 2020.  
 International Patent Application No. PCT/IB2020/050383, dated Jan. 17, 2020.  
 International Patent Application No. PCT/IB2020/050385, dated Jan. 17, 2020.  
 International Search Report and Written Opinion from International Patent Application No. PCT/IB2020/050385 dated Apr. 8, 2020.  
 Notice of Allowance in Design U.S. Appl. No. 29/677,152, dated Sep. 22, 2020.

Notice of Allowance in Design U.S. Appl. No. 29/676,901, dated Sep. 18, 2020.  
 Ex Parte Quayle Action in Design U.S. Appl. No. 29/677,152, dated Dec. 20, 2019.  
 Design U.S. Appl. No. 29/762,417, filed Dec. 16, 2020.  
 Design U.S. Appl. No. 29/767,502, filed Jan. 22, 2021.  
 U.S. Appl. No. 17/423,447, filed Jul. 15, 2021.  
 U.S. Appl. No. 17/423,576, filed Jul. 16, 2021.  
 U.S. Appl. No. 17/423,609, filed Jul. 16, 2021.  
 Office Action dated Aug. 17, 2021 in related U.S. Appl. No. 29/762,417, 9 pages.  
 Design U.S. Appl. No. 29/804,808, filed Aug. 23, 2021.  
 European Search Report for EP Application No. EP19746801 dated Sep. 13, 2021, 2 pages.  
 Nagaya et al “Fluorescence-Guided Surgery”, *Frontiers in Oncology*, vol. 7, Dec. 22, 2017, 16 pp.

\* cited by examiner

*Primary Examiner* — Anhdao Doan  
 (74) *Attorney, Agent, or Firm* — Jones Robb, PLLC

(57) **CLAIM**

The ornamental design for a handheld multi-modal imaging device, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, left side perspective view of a first embodiment of a handheld multi-modal imaging device showing our new design.  
 FIG. 2 is a bottom, left side perspective view thereof.  
 FIG. 3 is a left side view thereof.  
 FIG. 4 is a right side view thereof.  
 FIG. 5 is a top view thereof.  
 FIG. 6 is a bottom view thereof.  
 FIG. 7 is a front view thereof.  
 FIG. 8 is a back view thereof.  
 FIG. 9 is a top, left side perspective view of a second embodiment of a handheld multi-modal imaging device showing our new design.  
 FIG. 10 is a bottom, left side perspective view thereof.  
 FIG. 11 is a left side view thereof.  
 FIG. 12 is a right side view thereof.  
 FIG. 13 is a top view thereof.  
 FIG. 14 is a bottom view thereof.  
 FIG. 15 is a front view thereof; and,  
 FIG. 16 is a back view thereof.  
 The broken lines on the handle member represent environment and the remaining broken lines illustrate portions of the handheld multi-modal imaging device that form no part of the claimed design.  
 The handheld multi-modal imaging device is shown with a symbolic break in its length. The appearance of any portion of the article between the break lines forms no part of the claimed design.

**1 Claim, 16 Drawing Sheets**

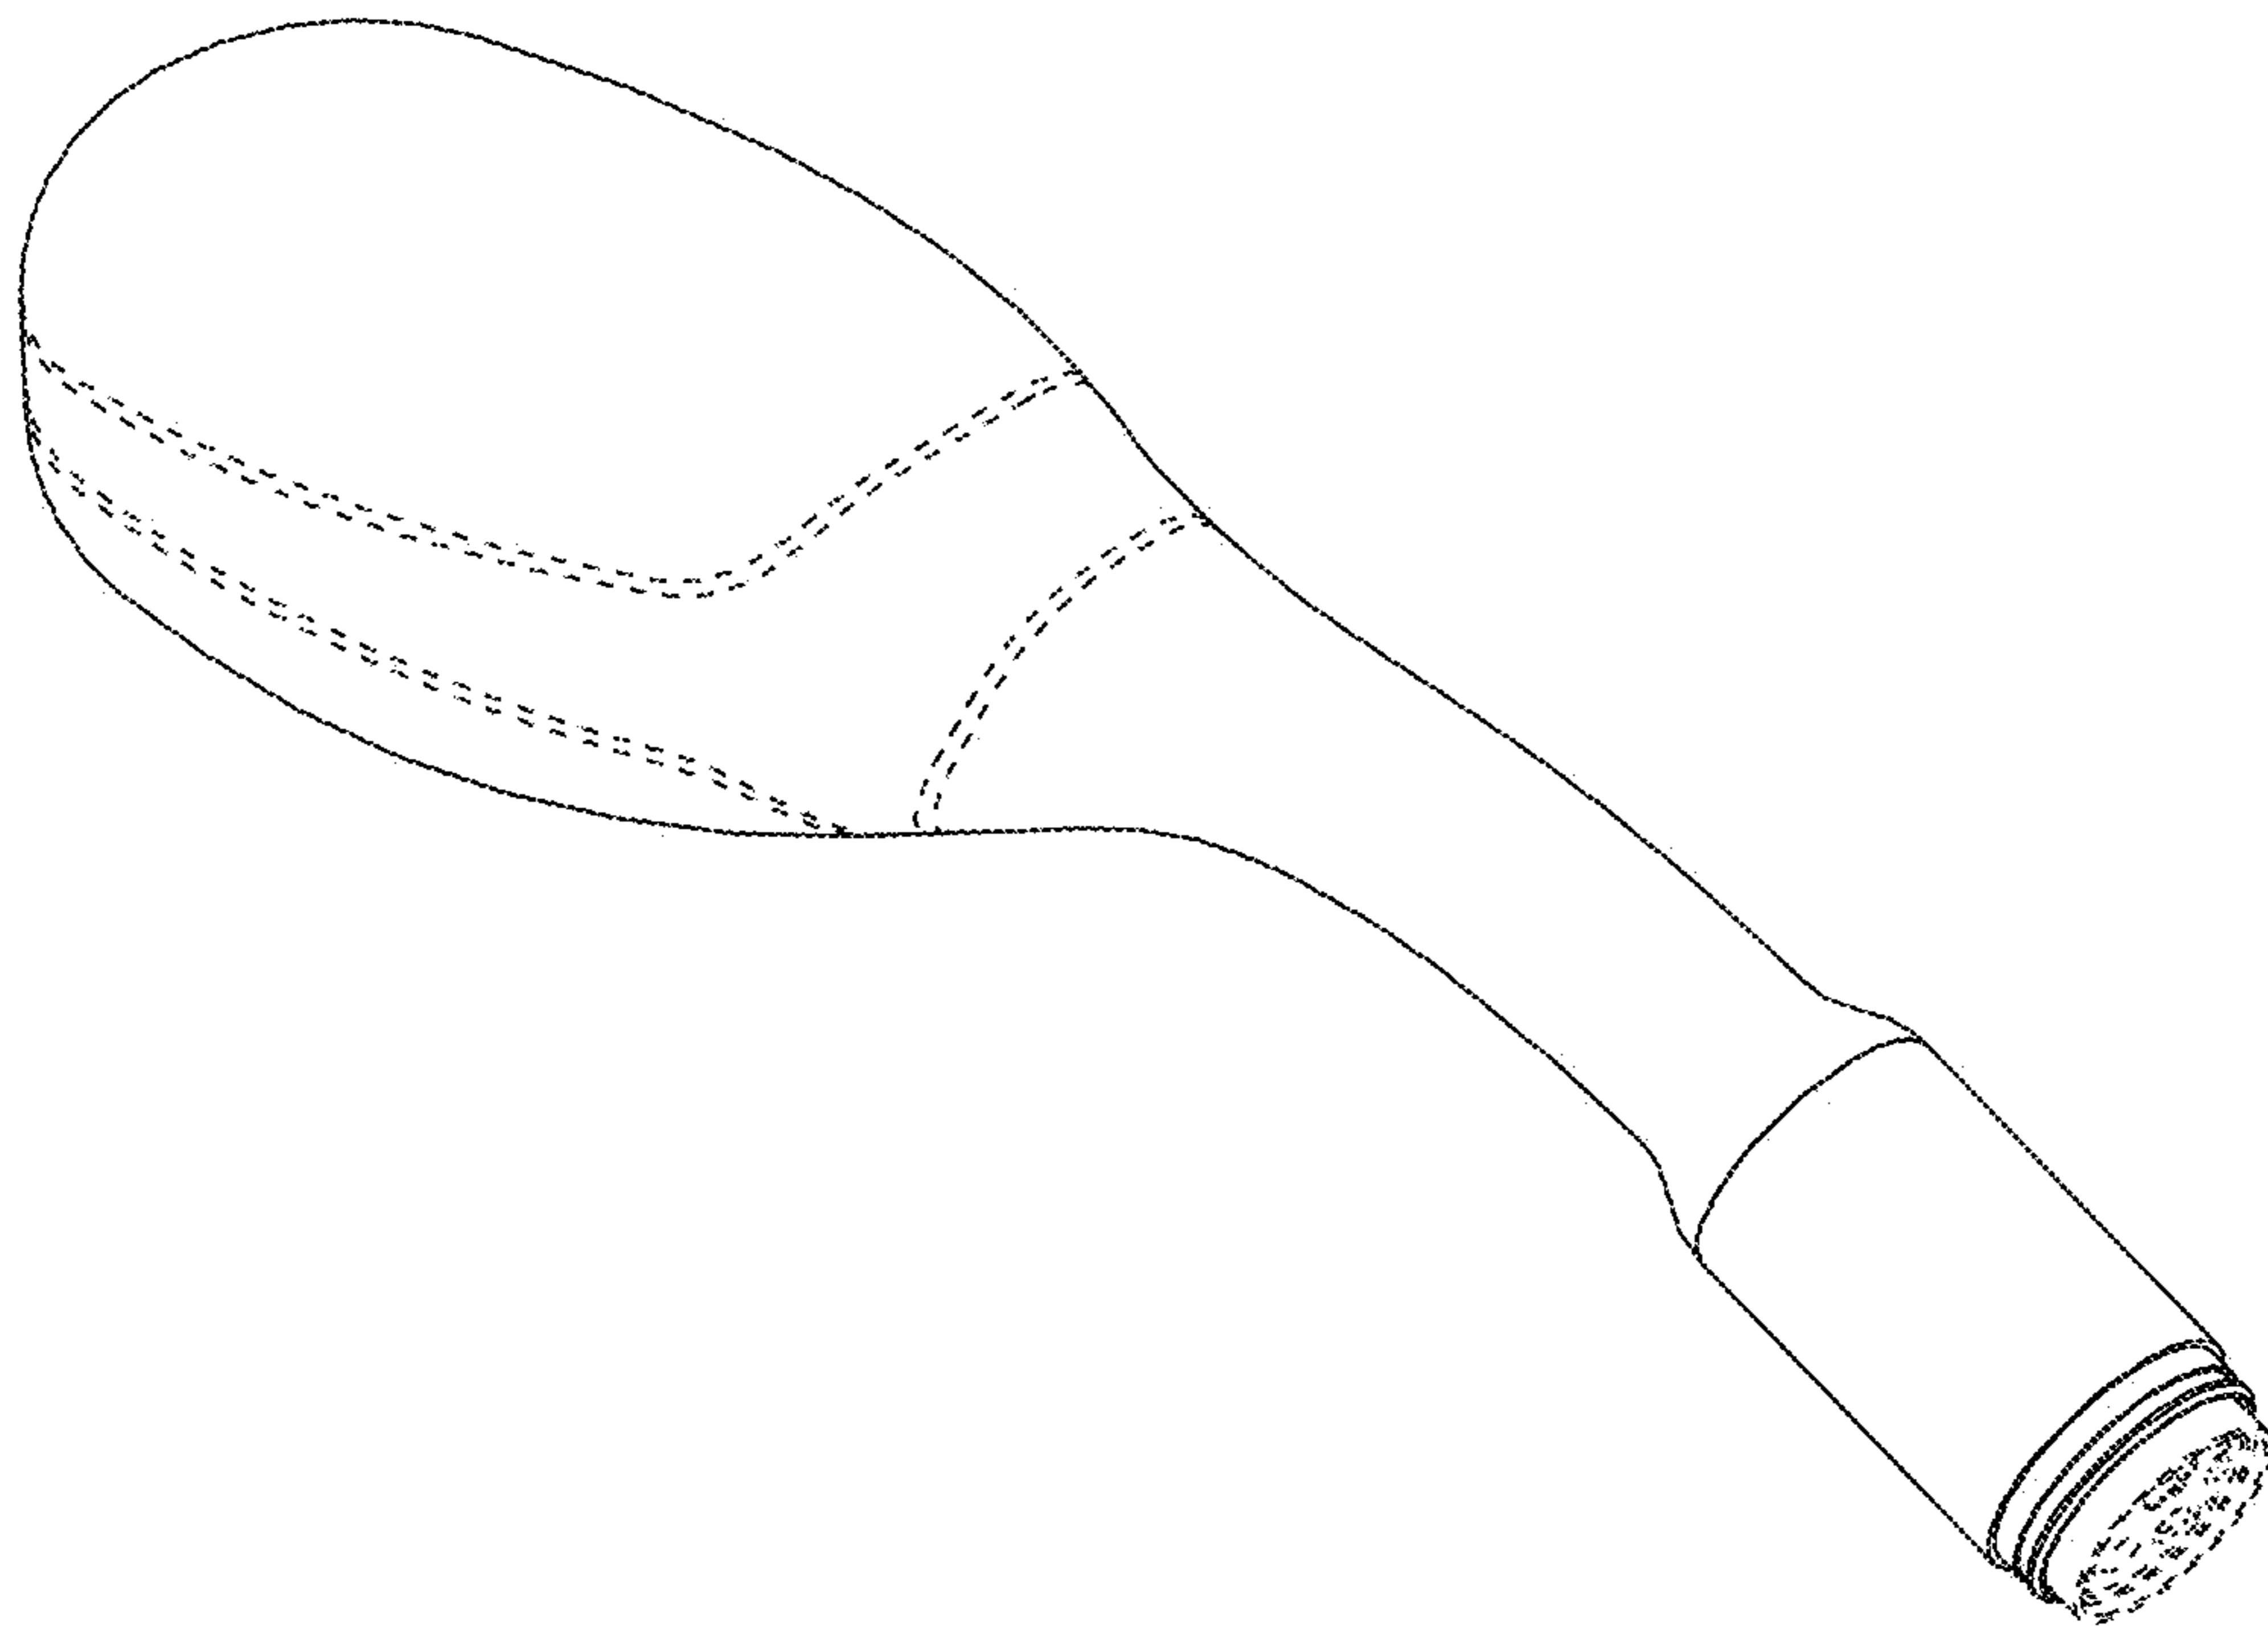


FIG. 1

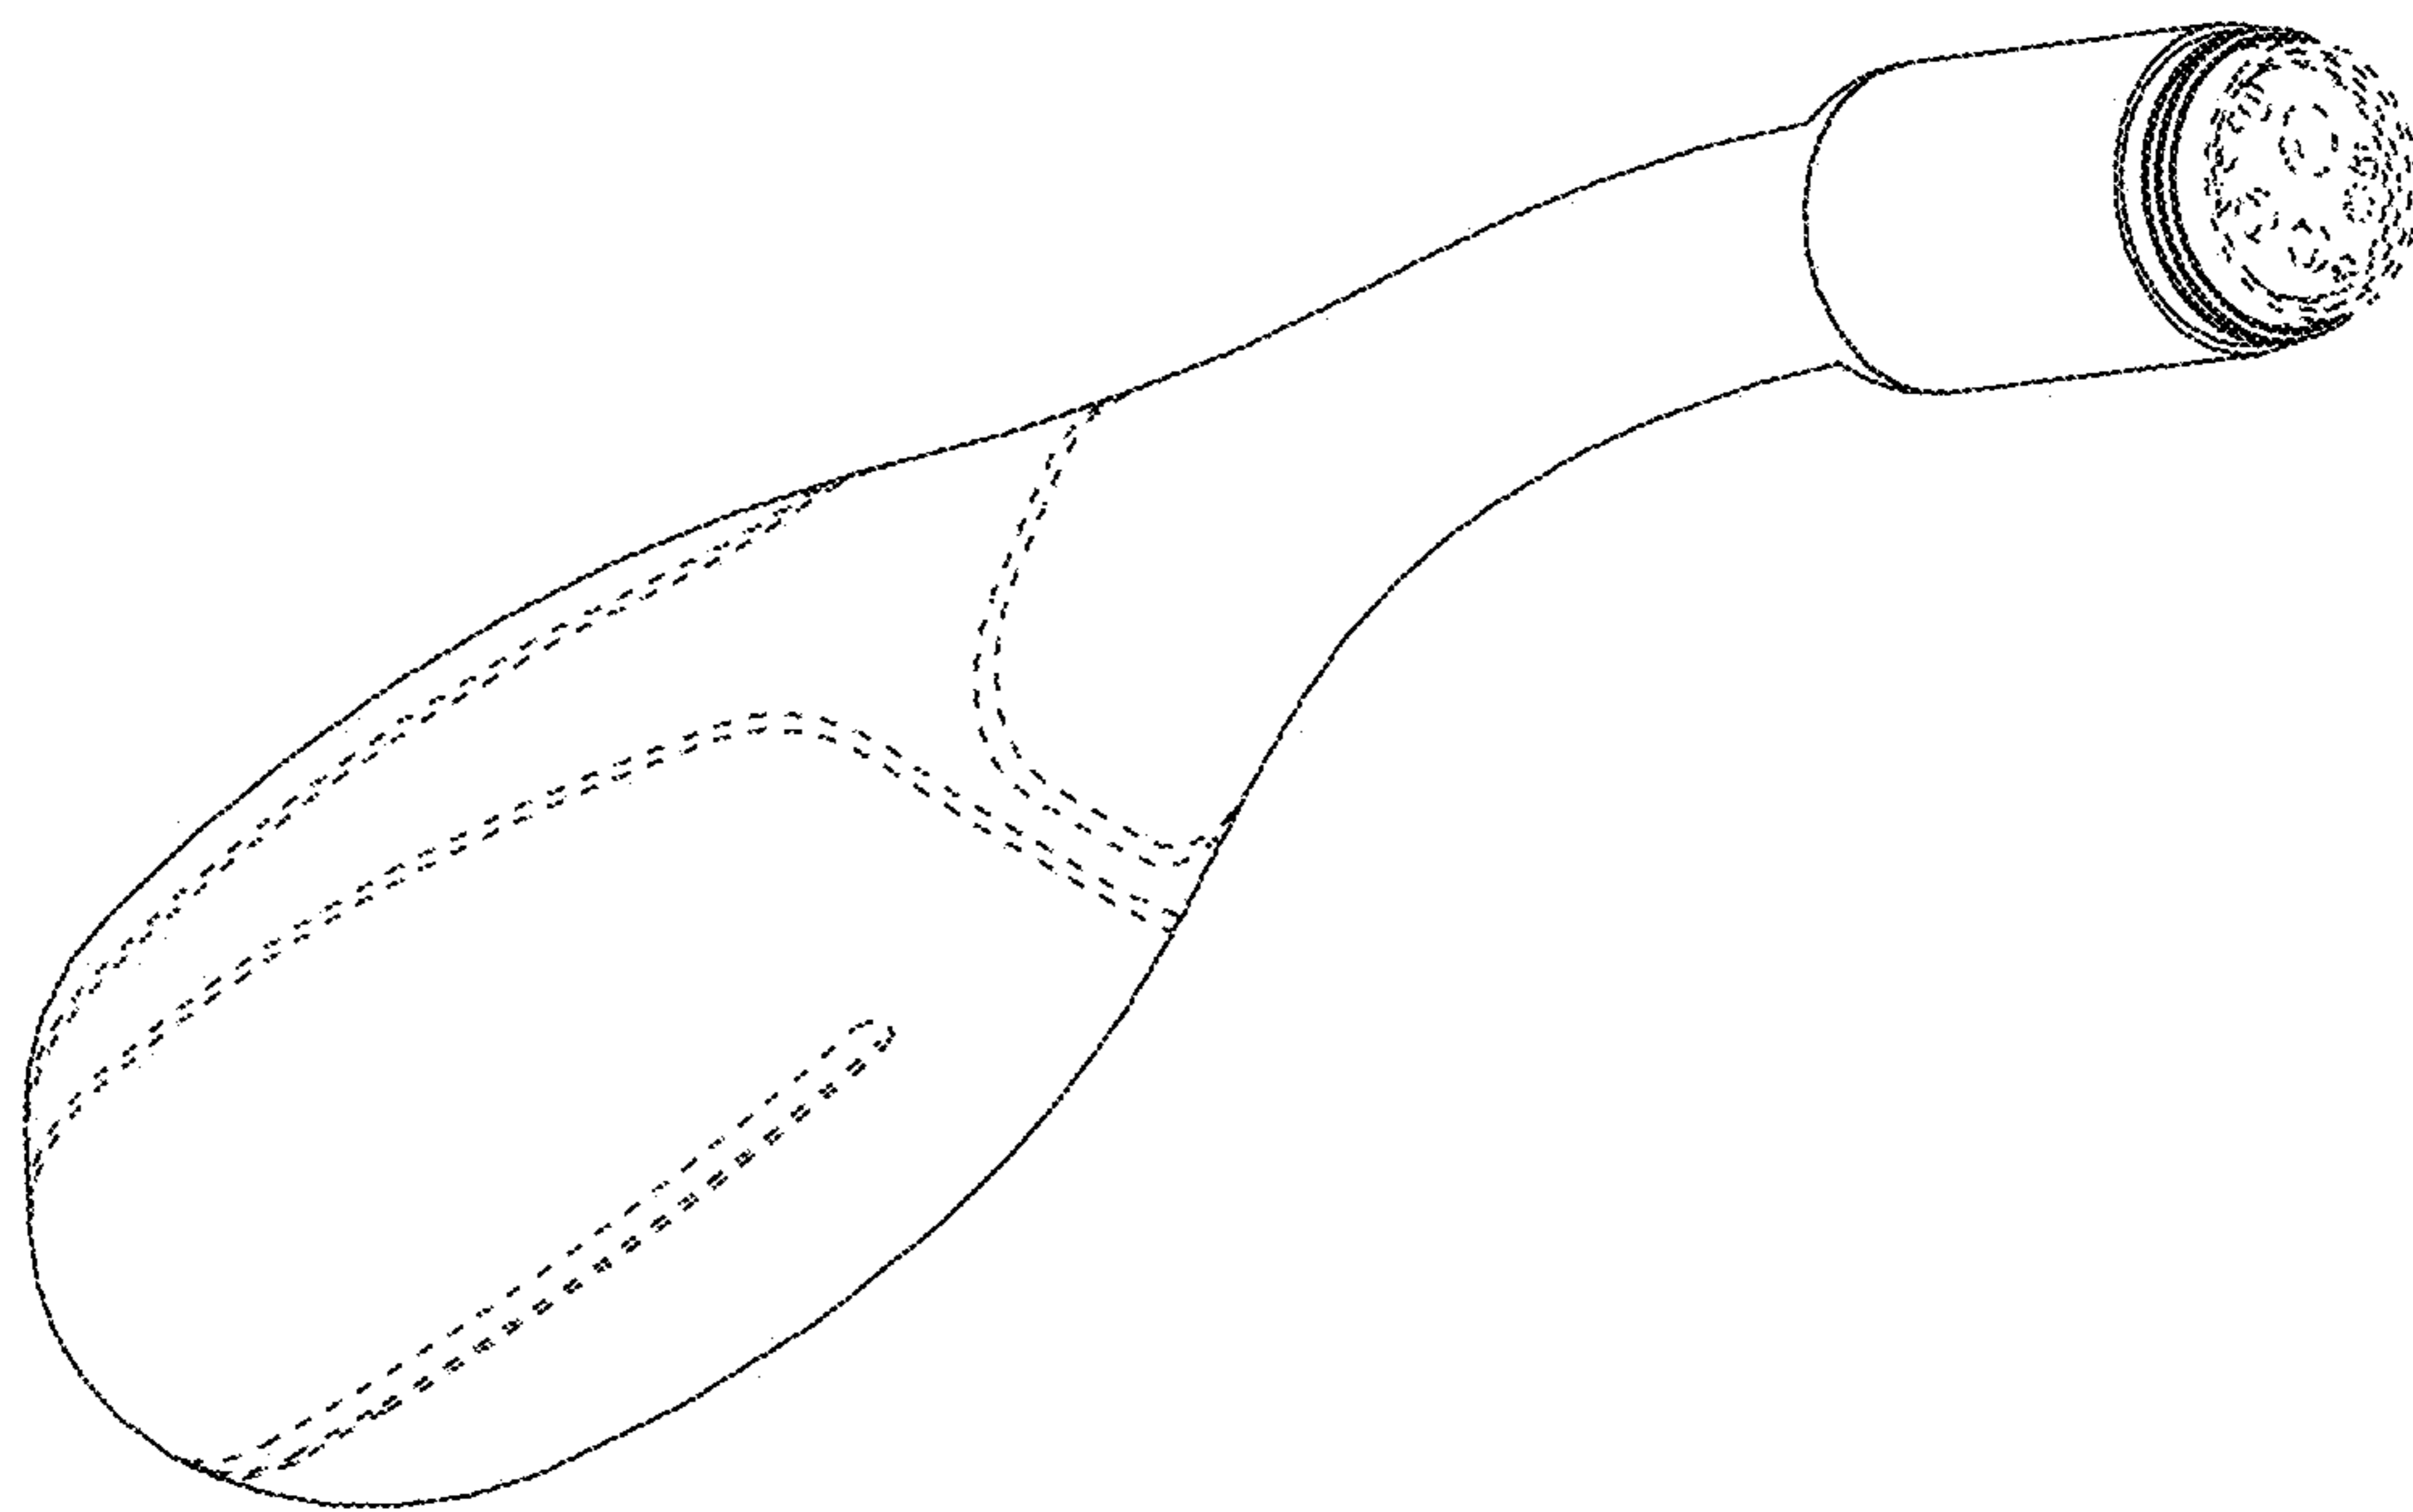


FIG. 2

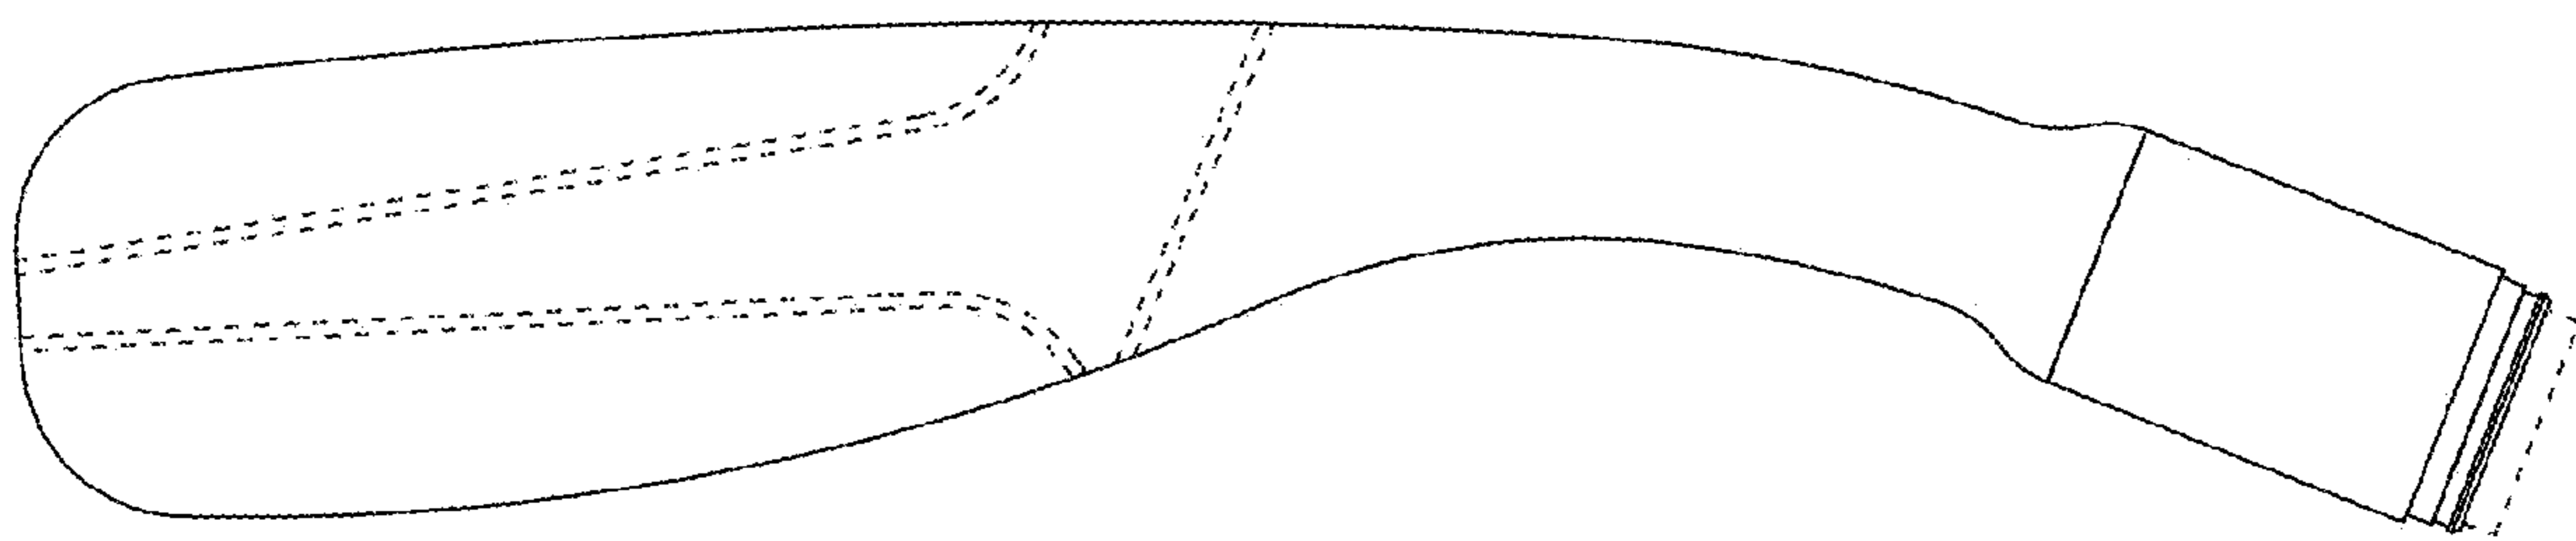


FIG. 3

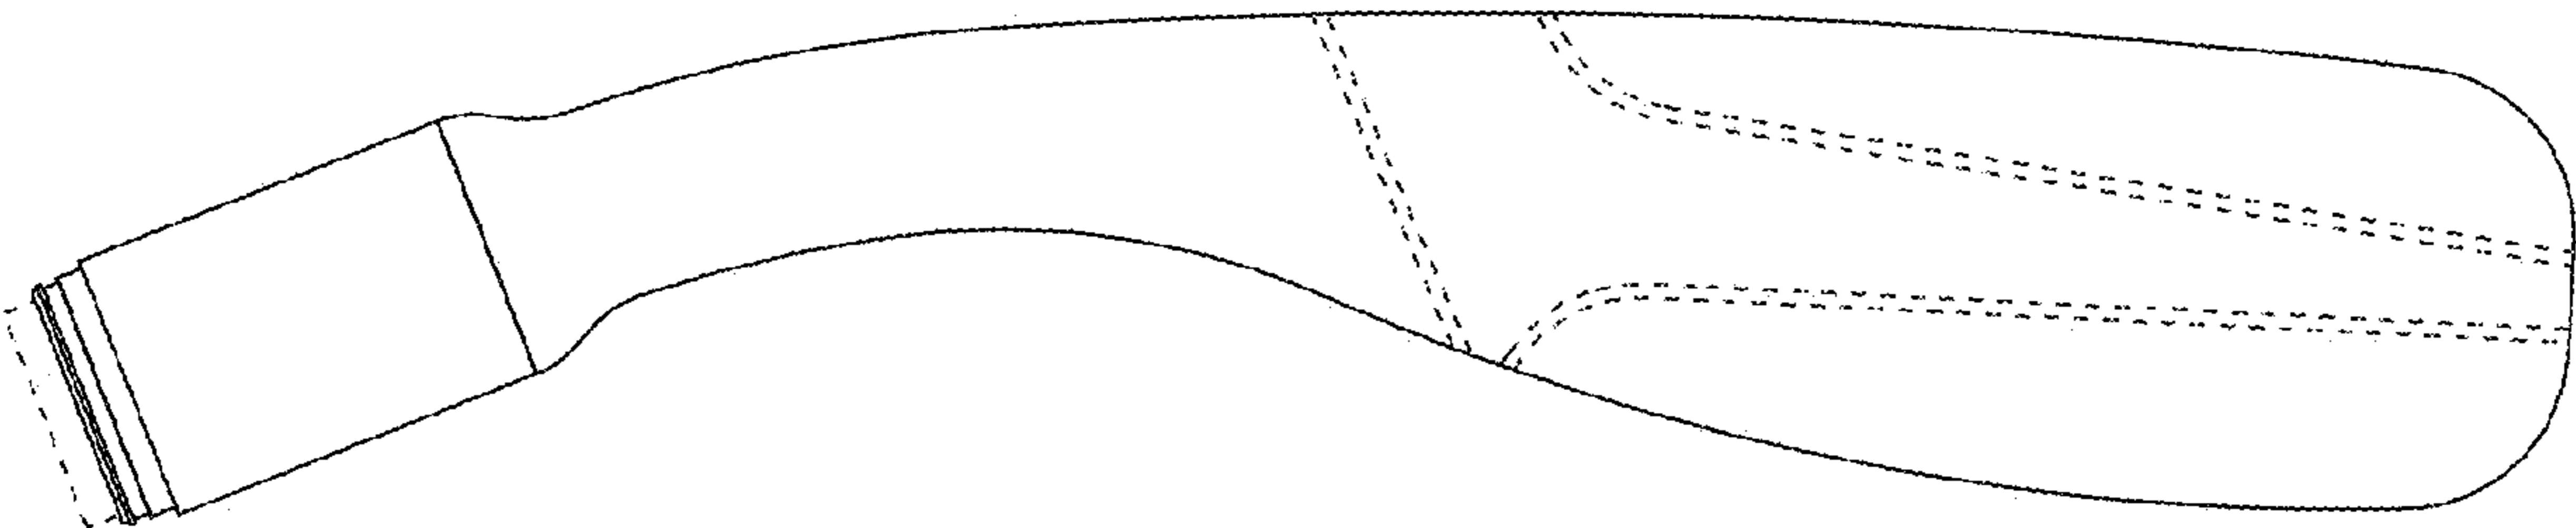


FIG. 4

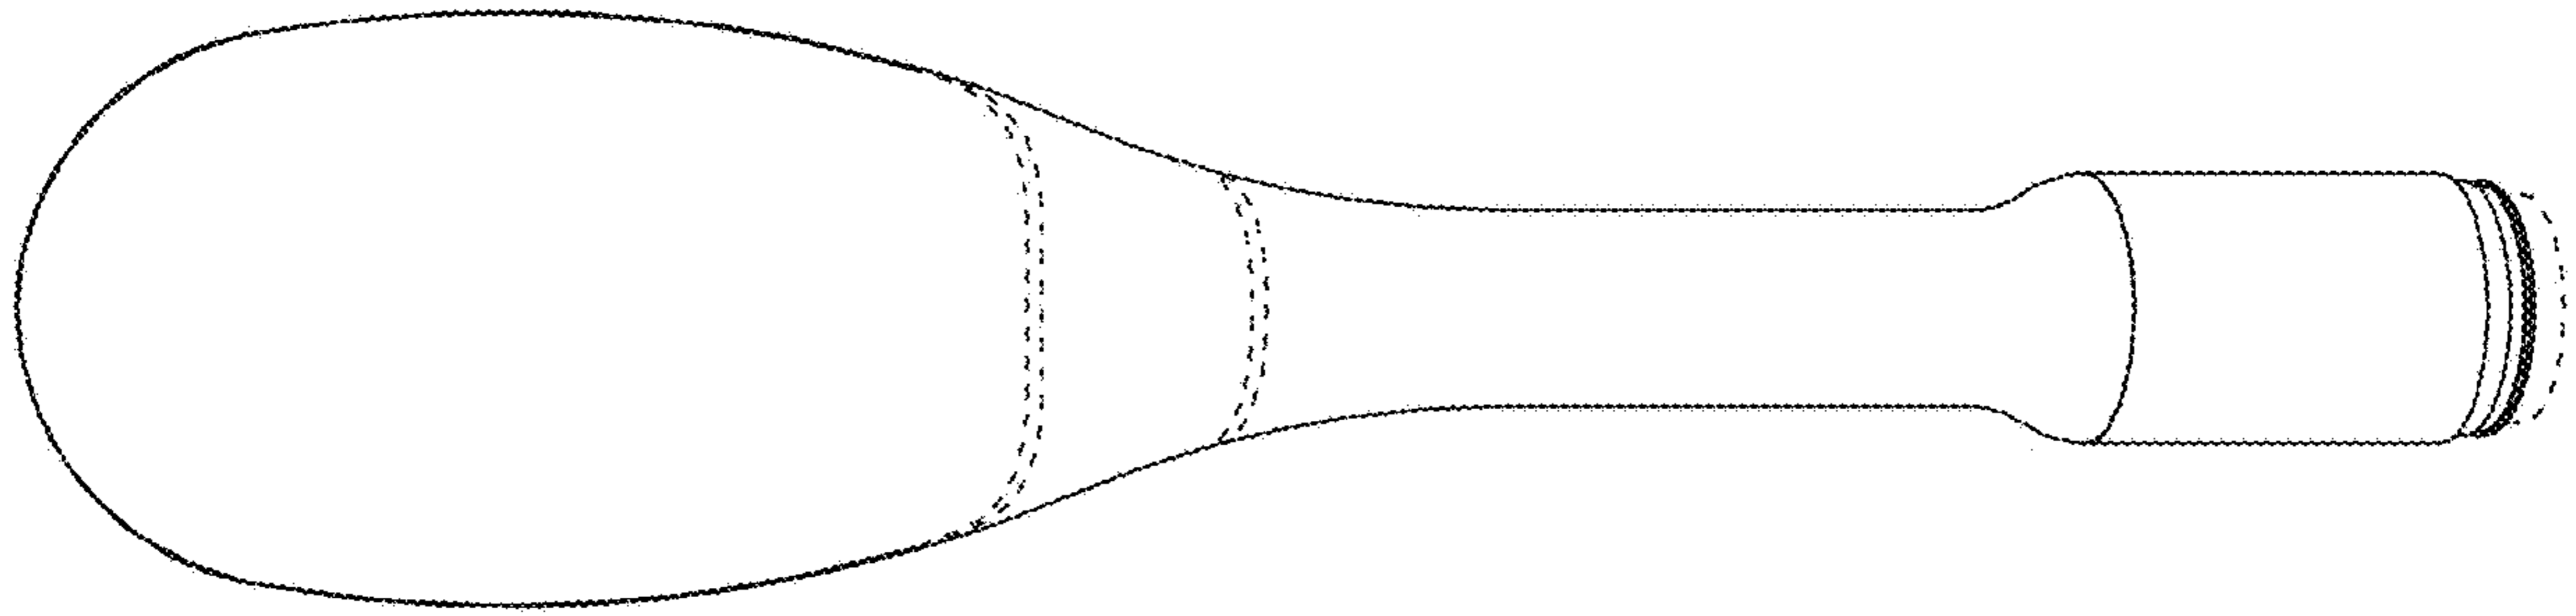


FIG. 5

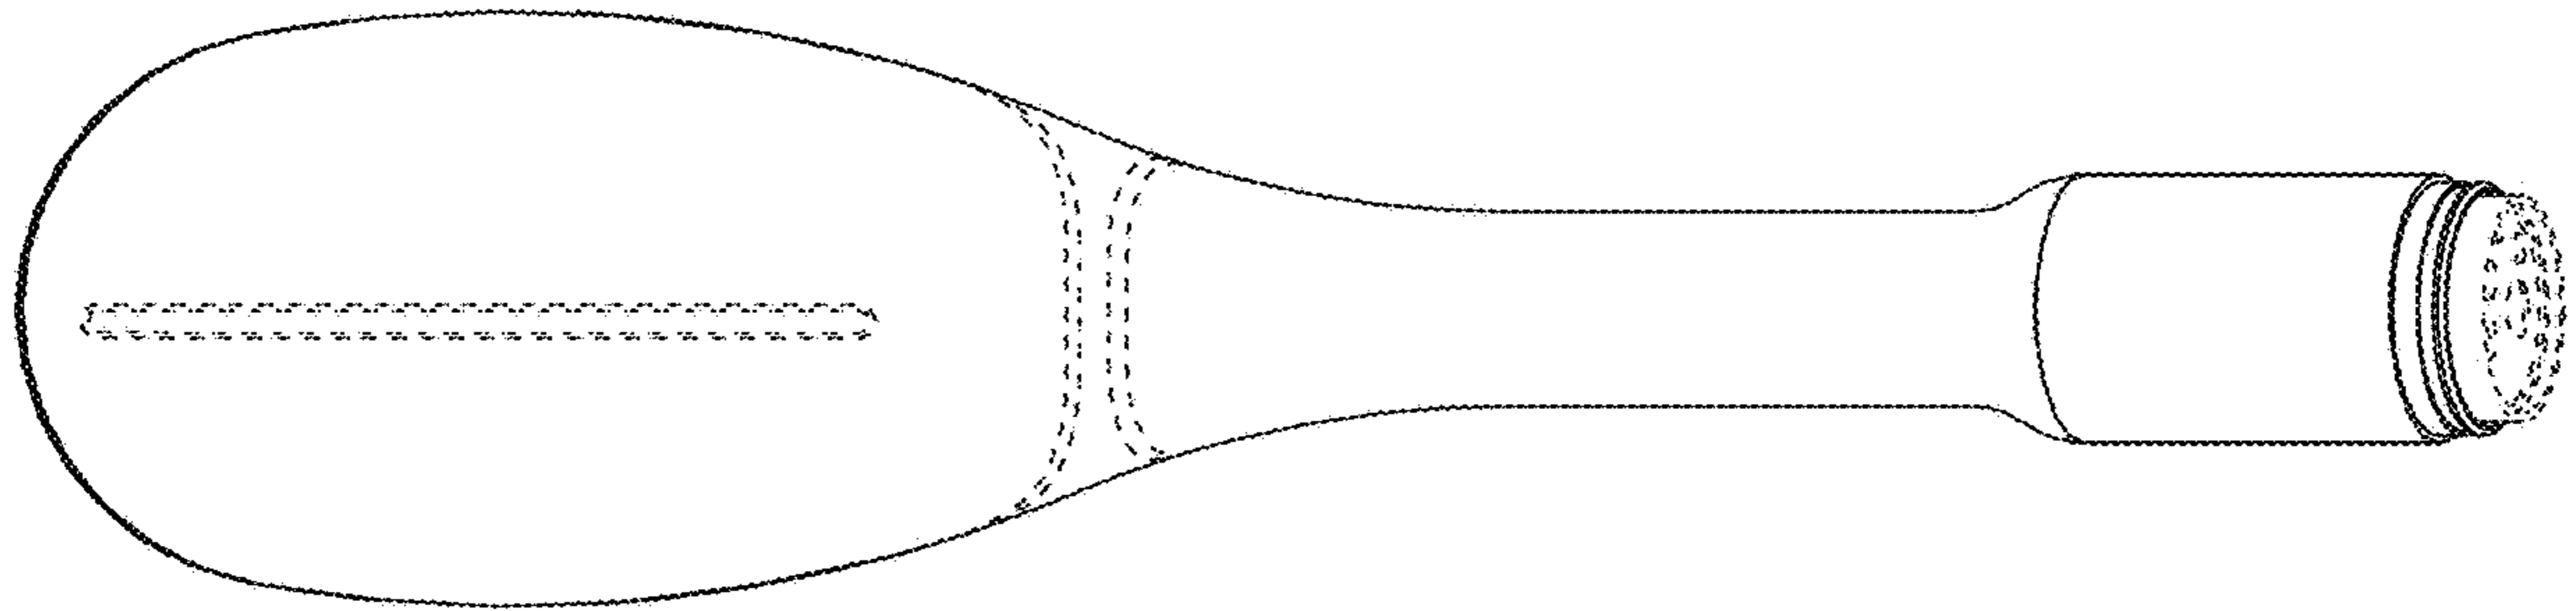


FIG. 6



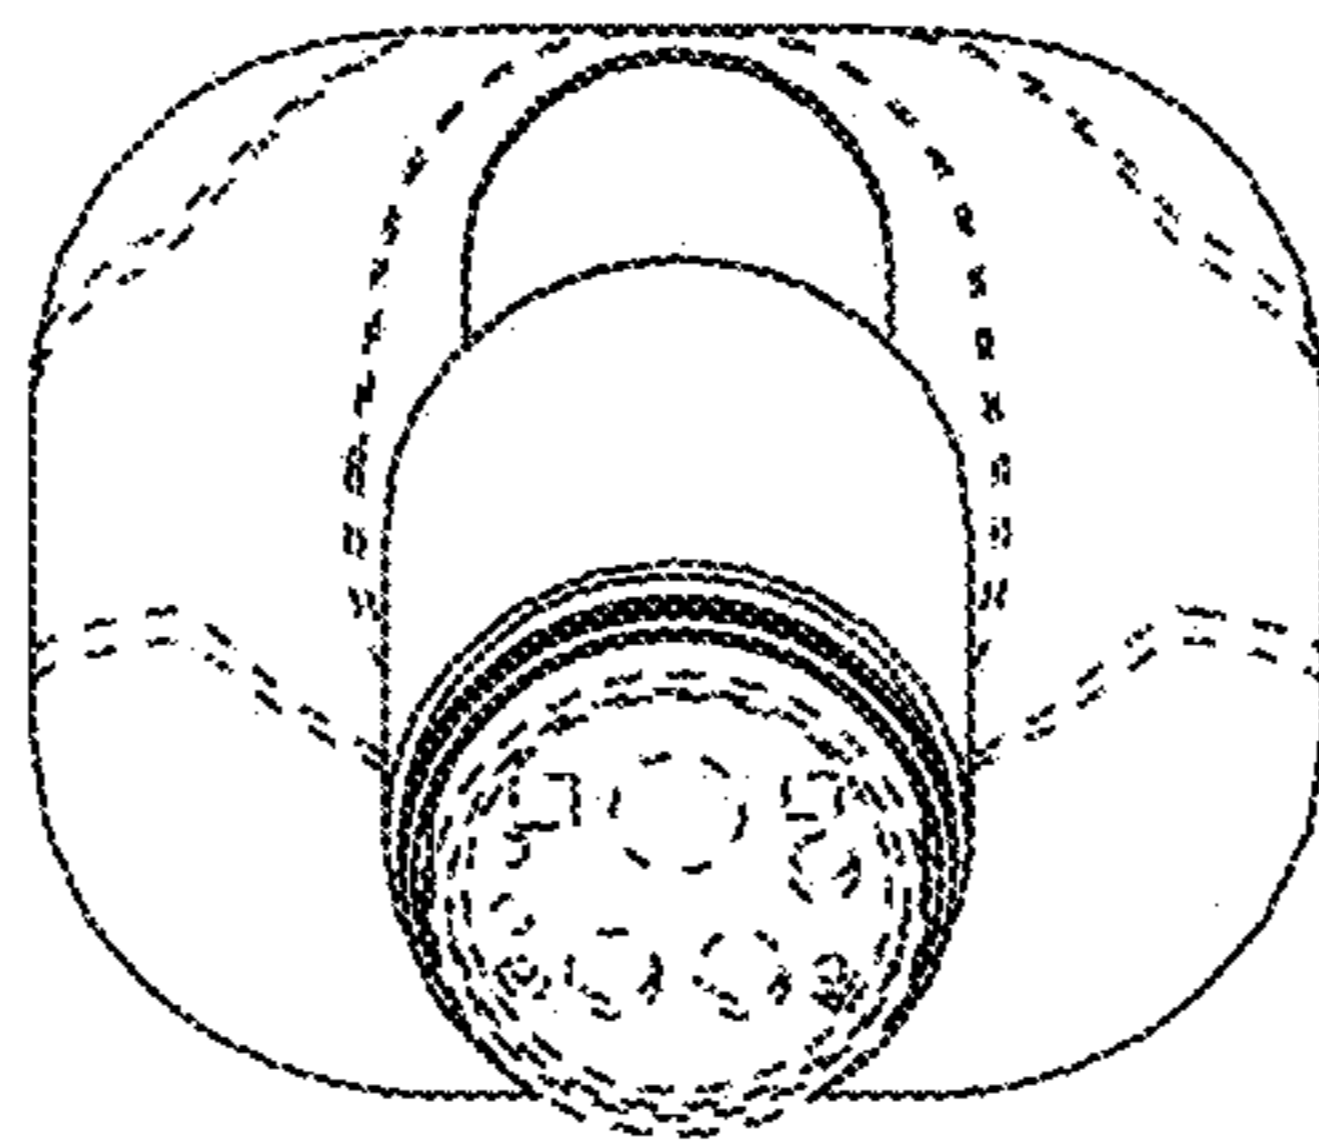


FIG. 7

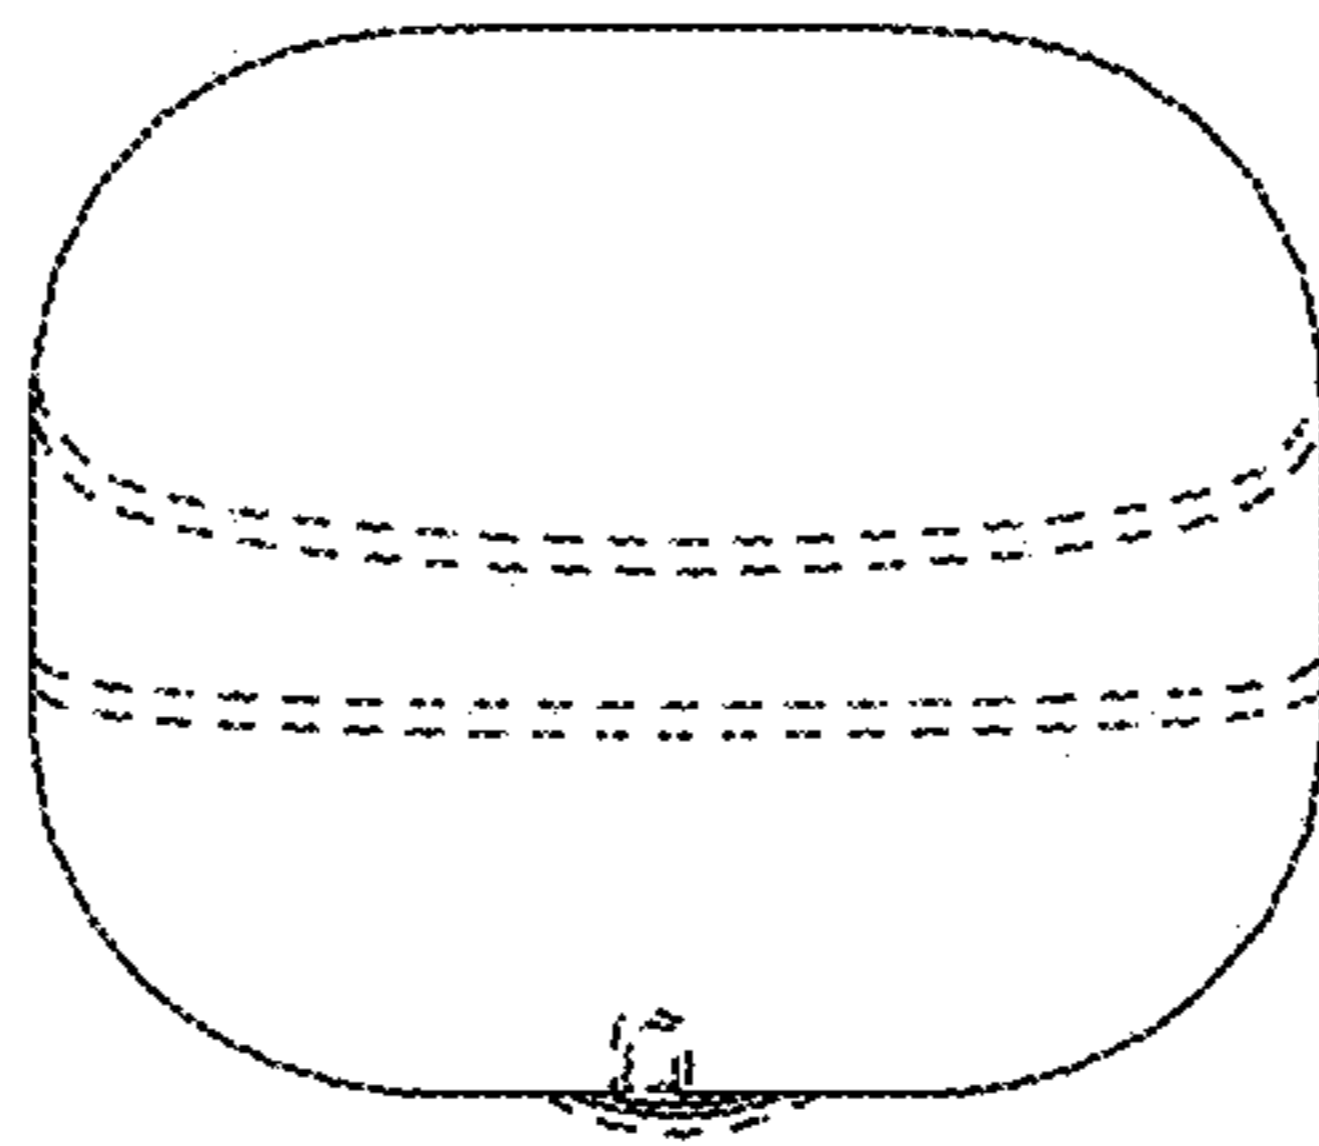


FIG. 8

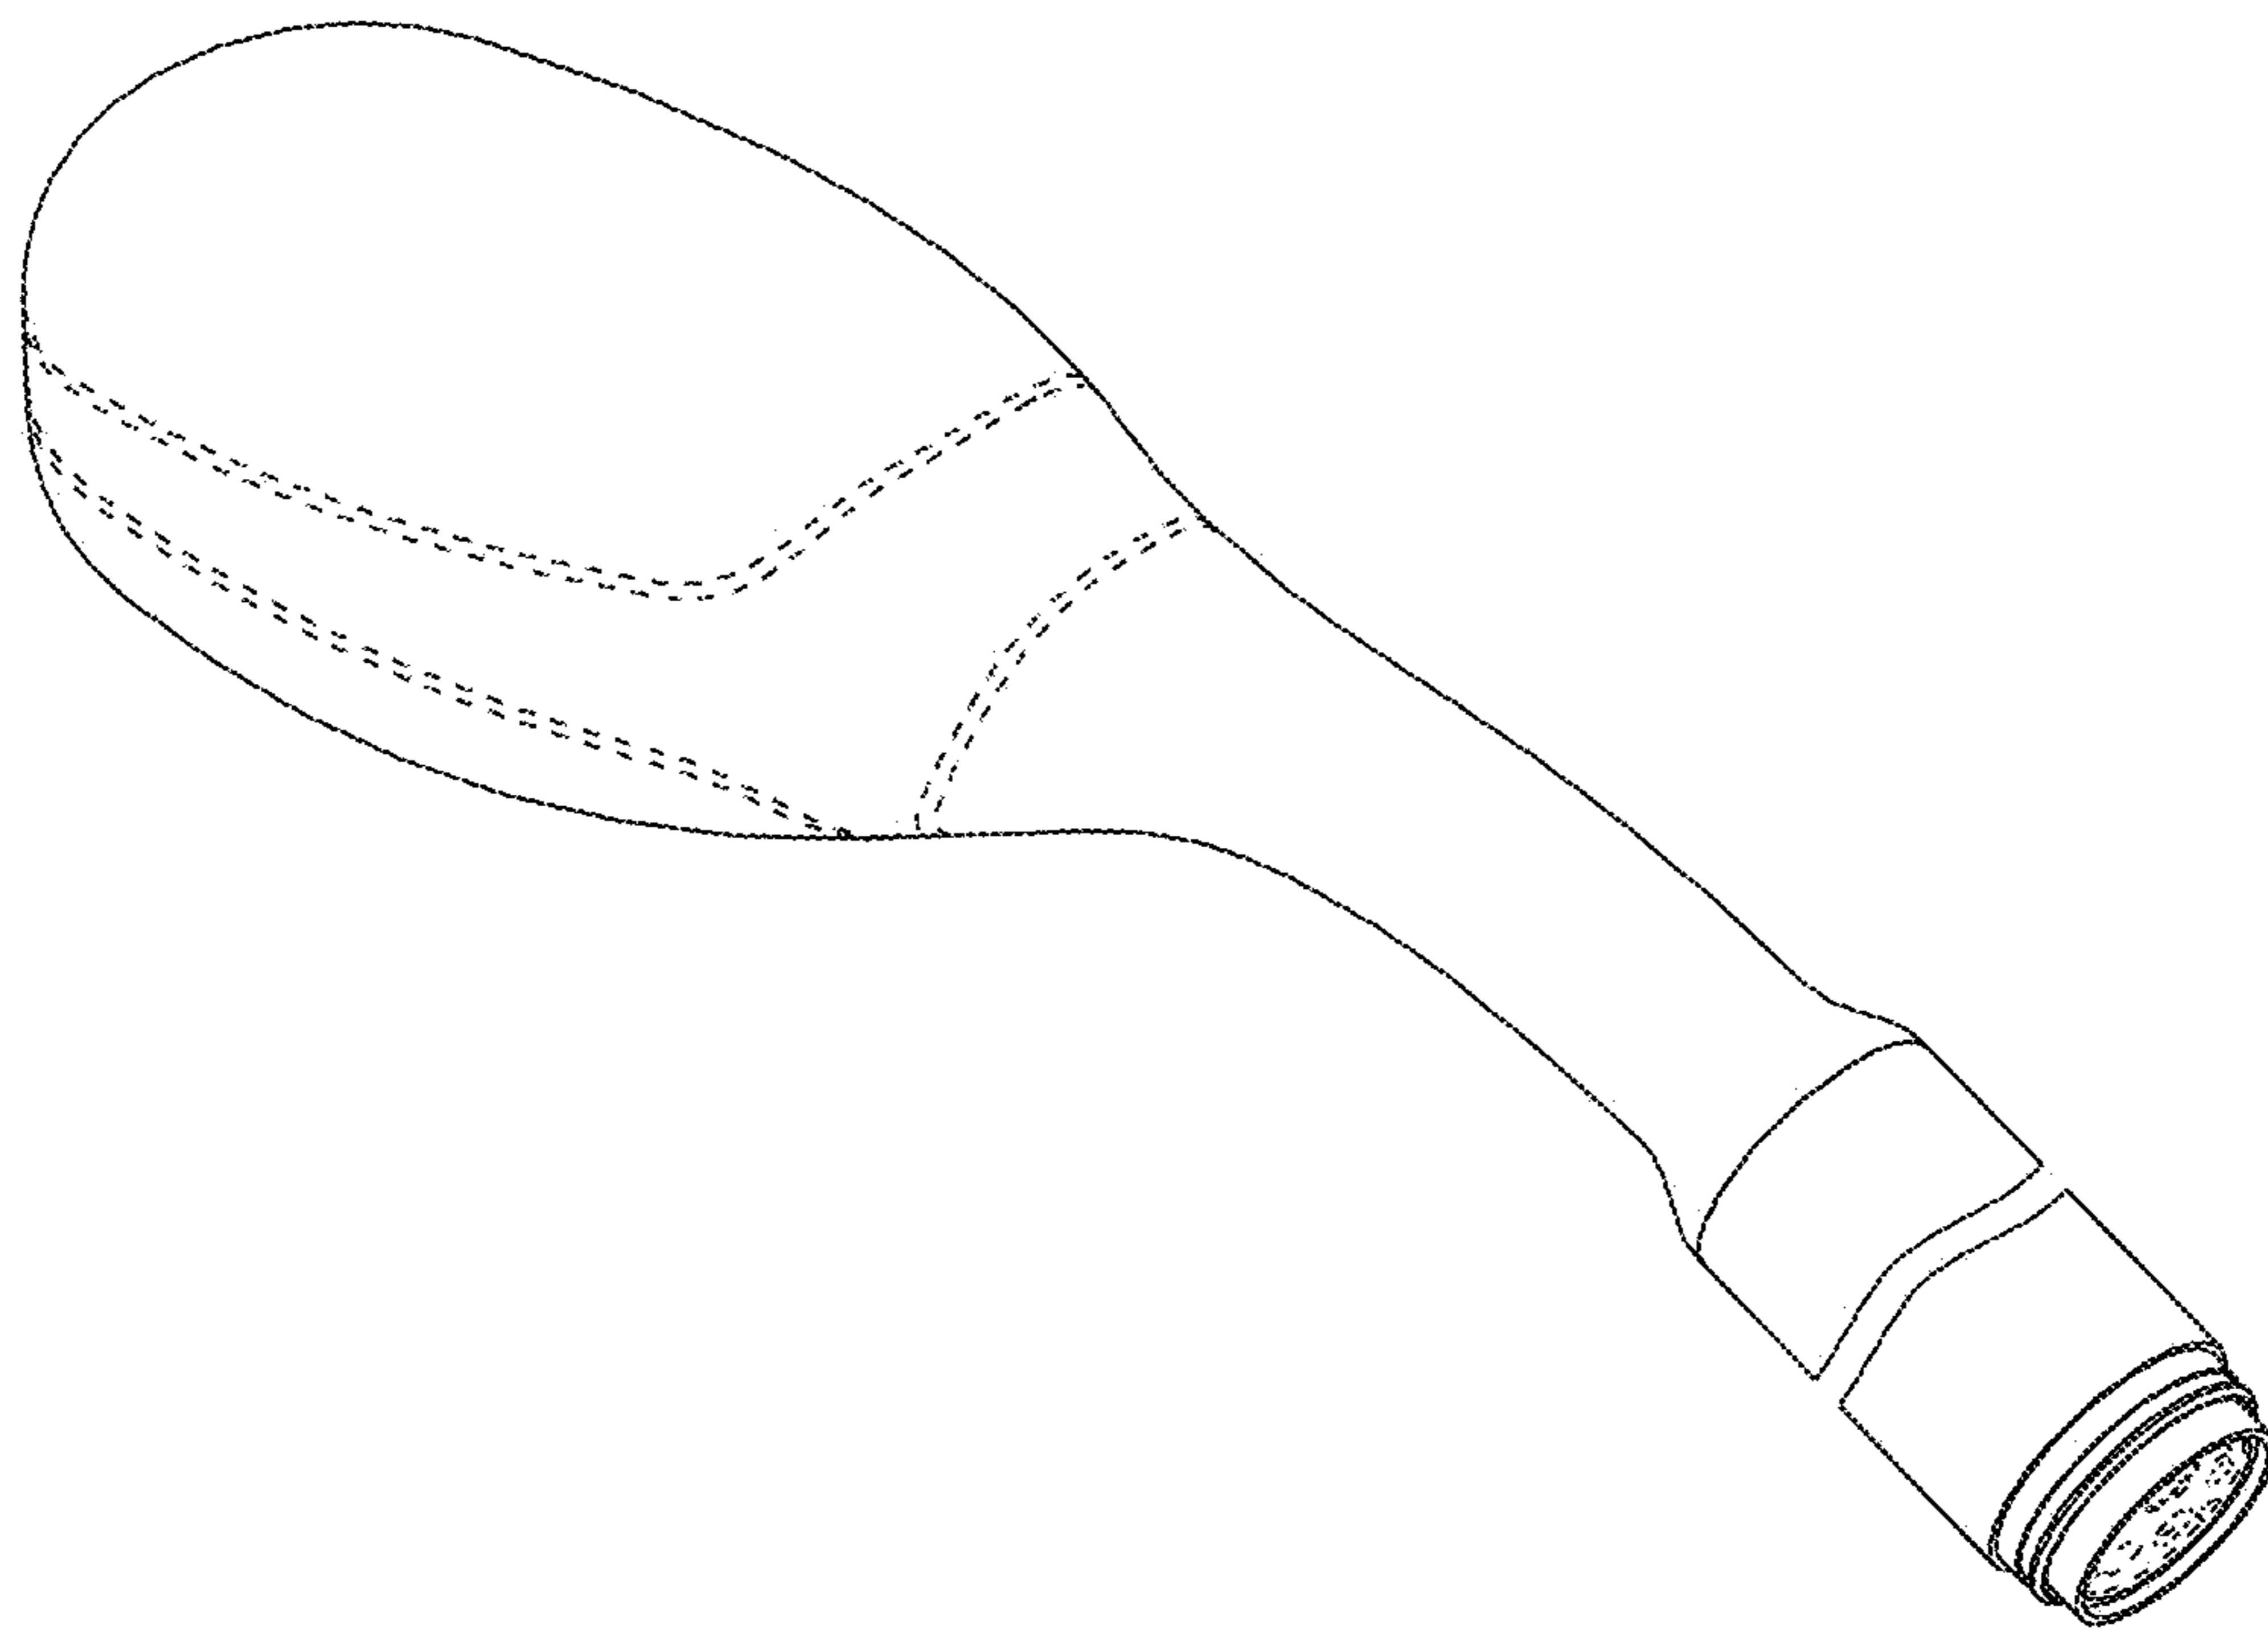


FIG. 9

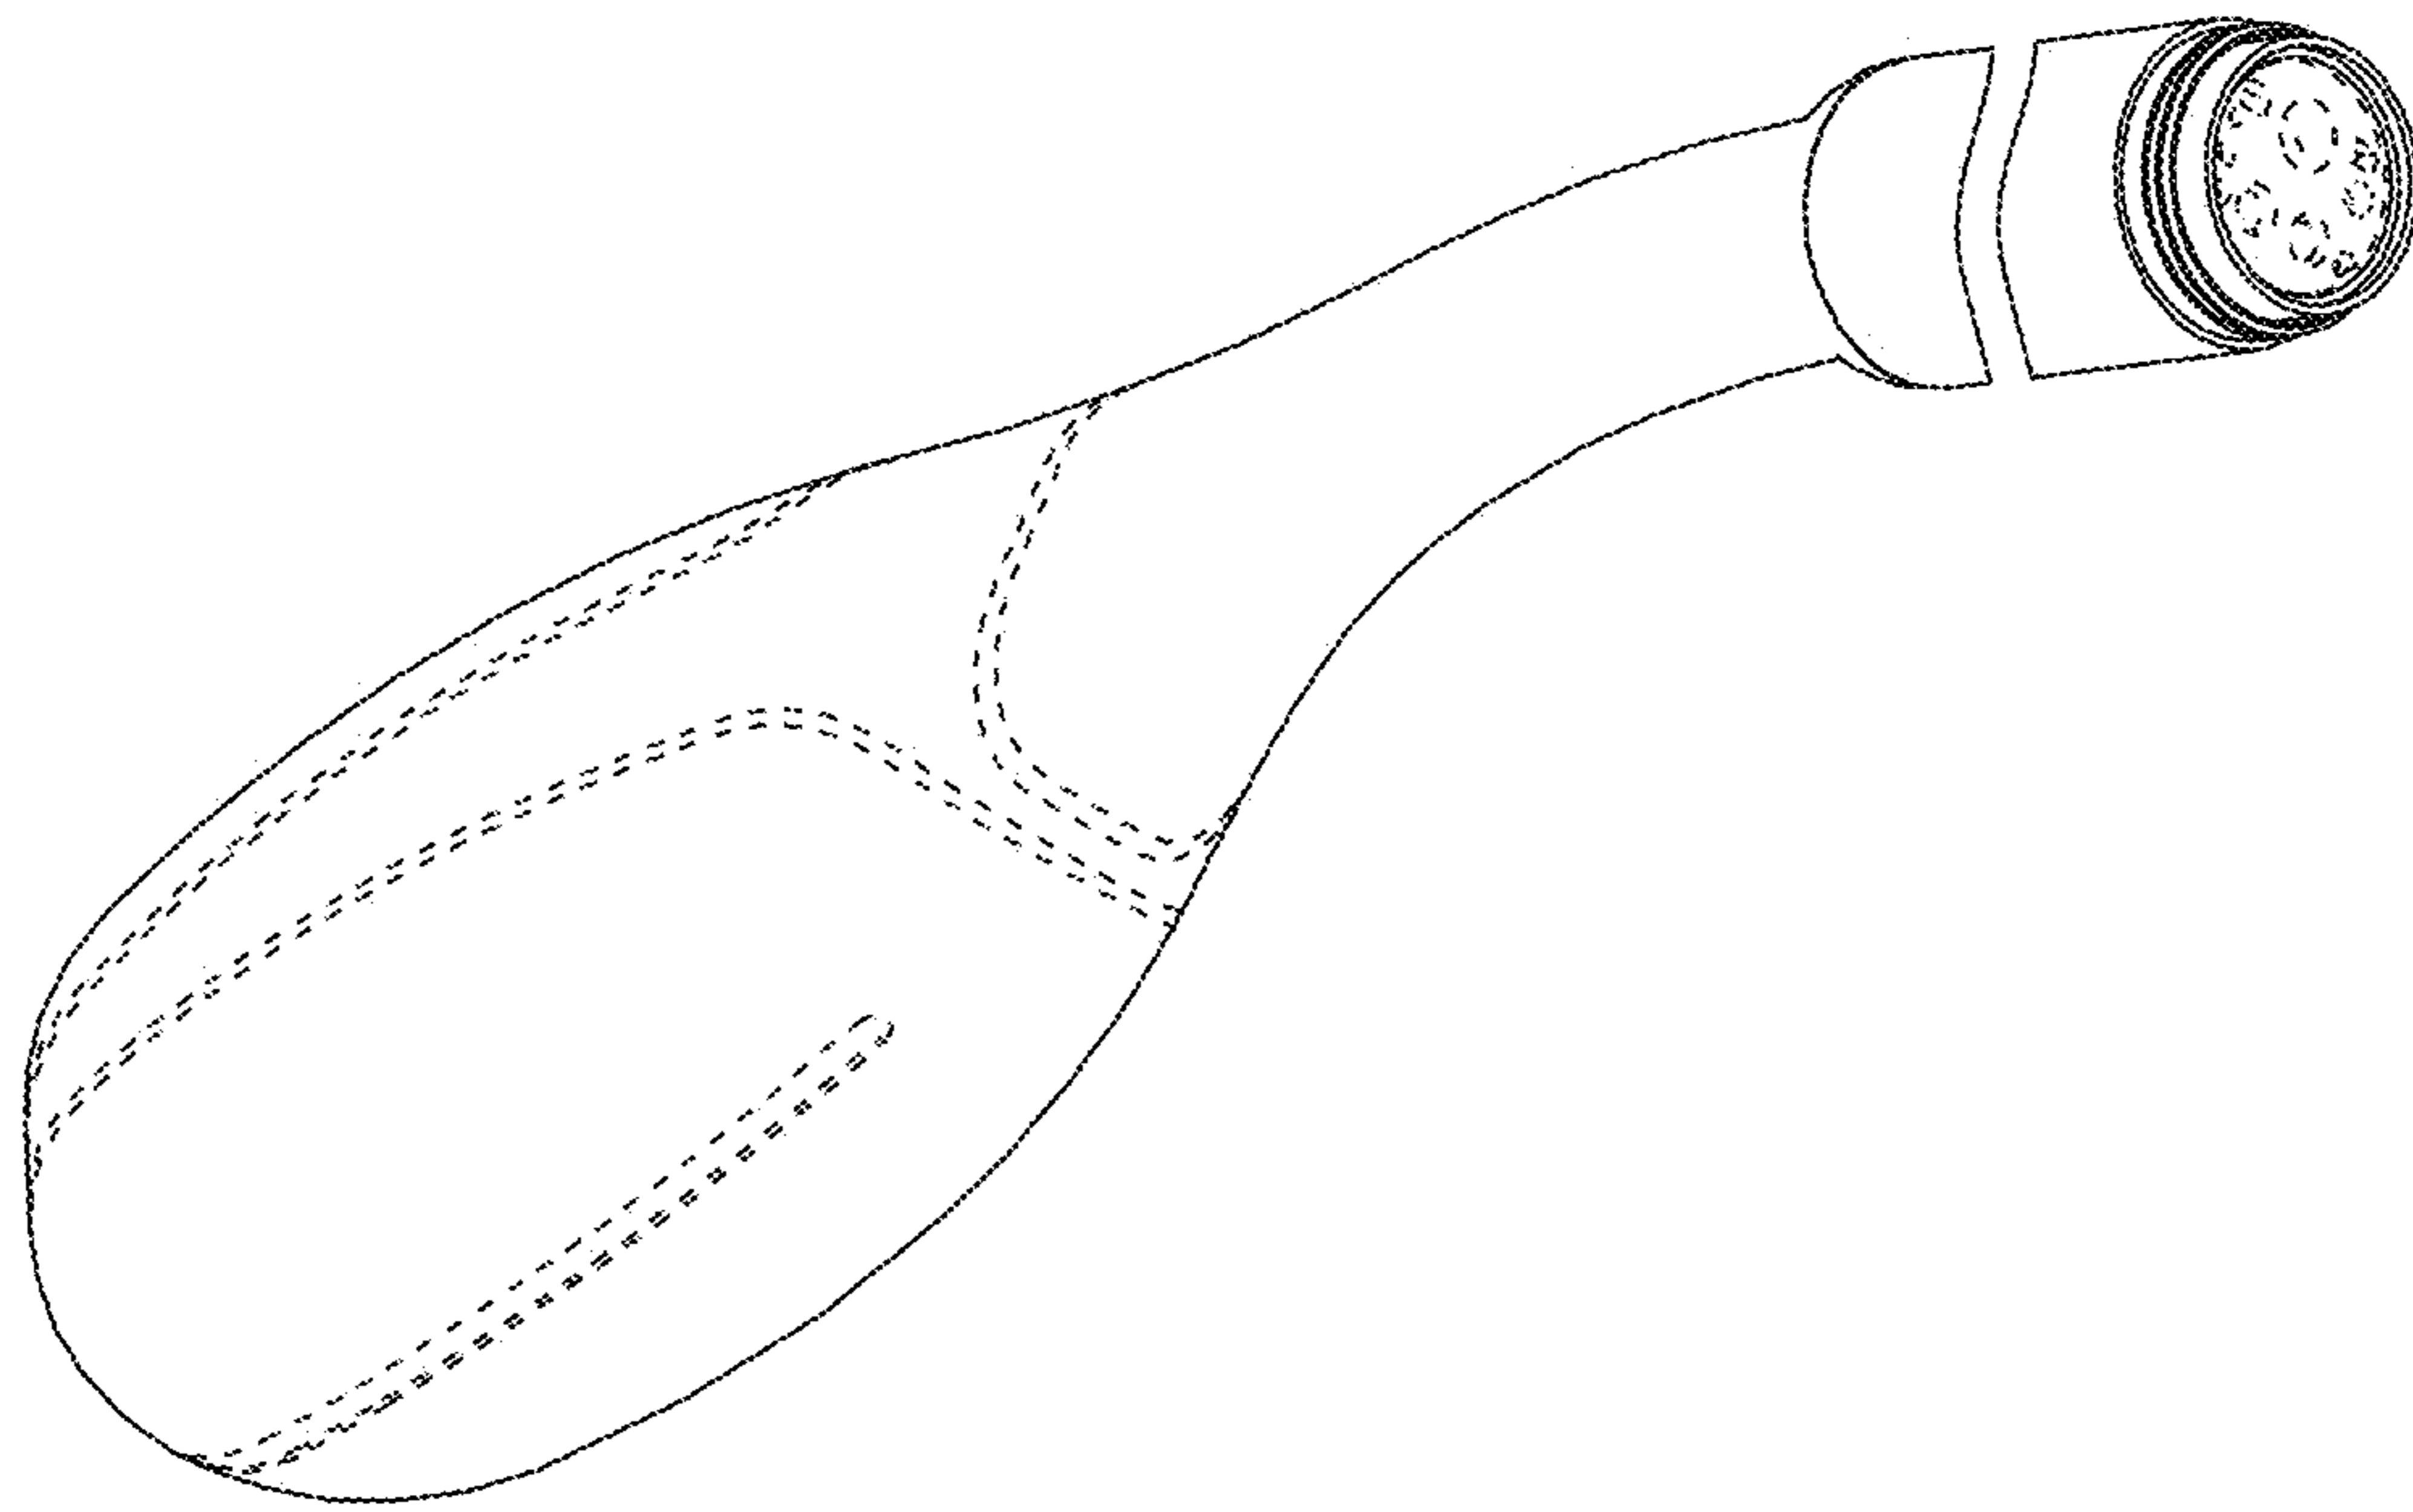


FIG. 10

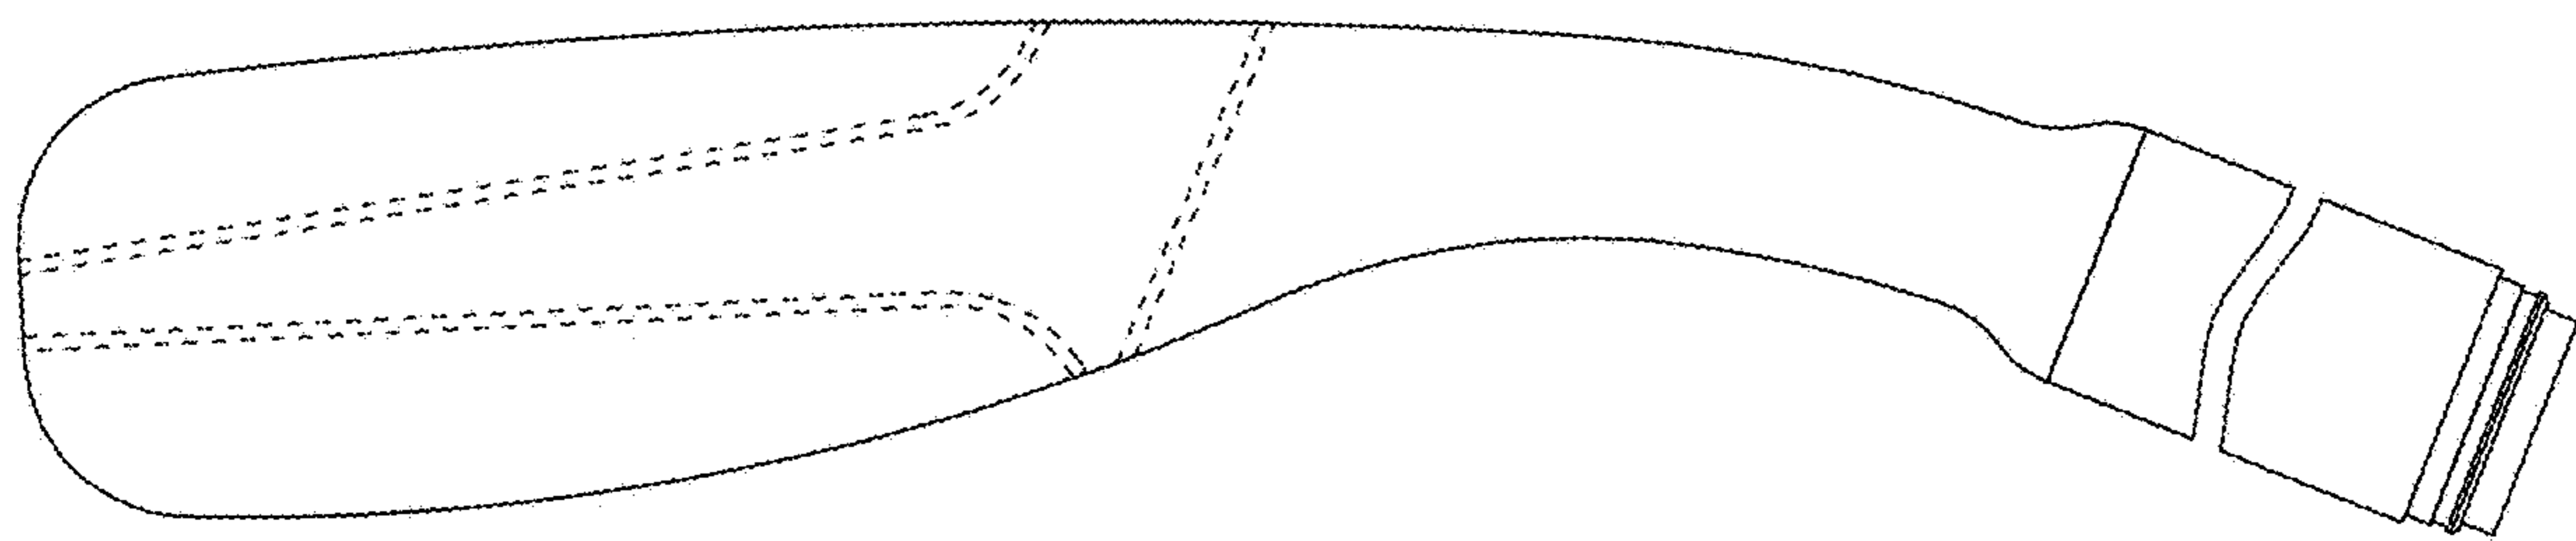


FIG. 11

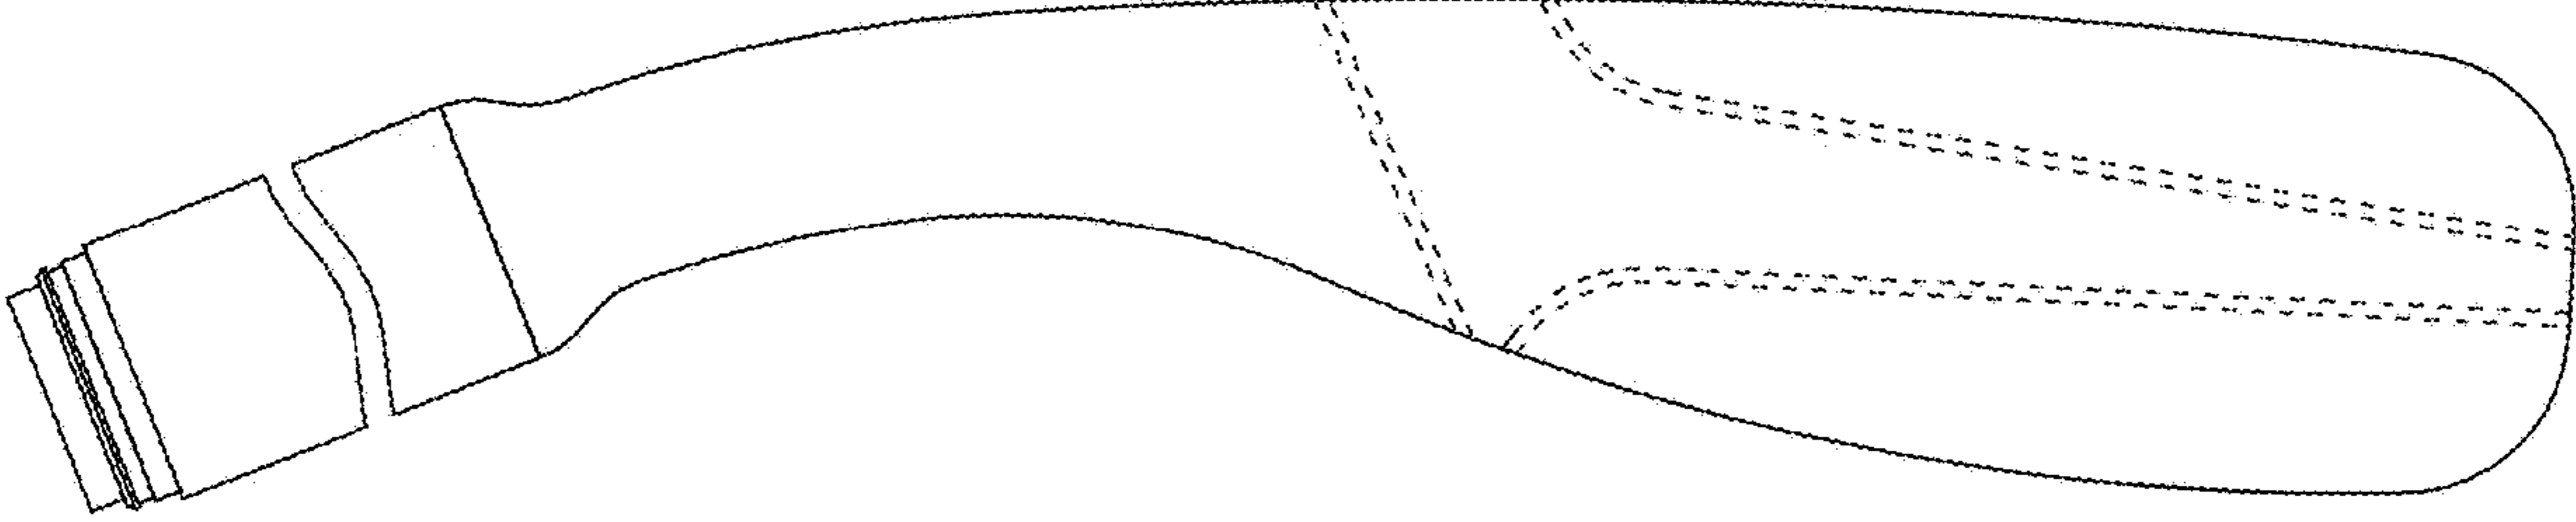


FIG. 12

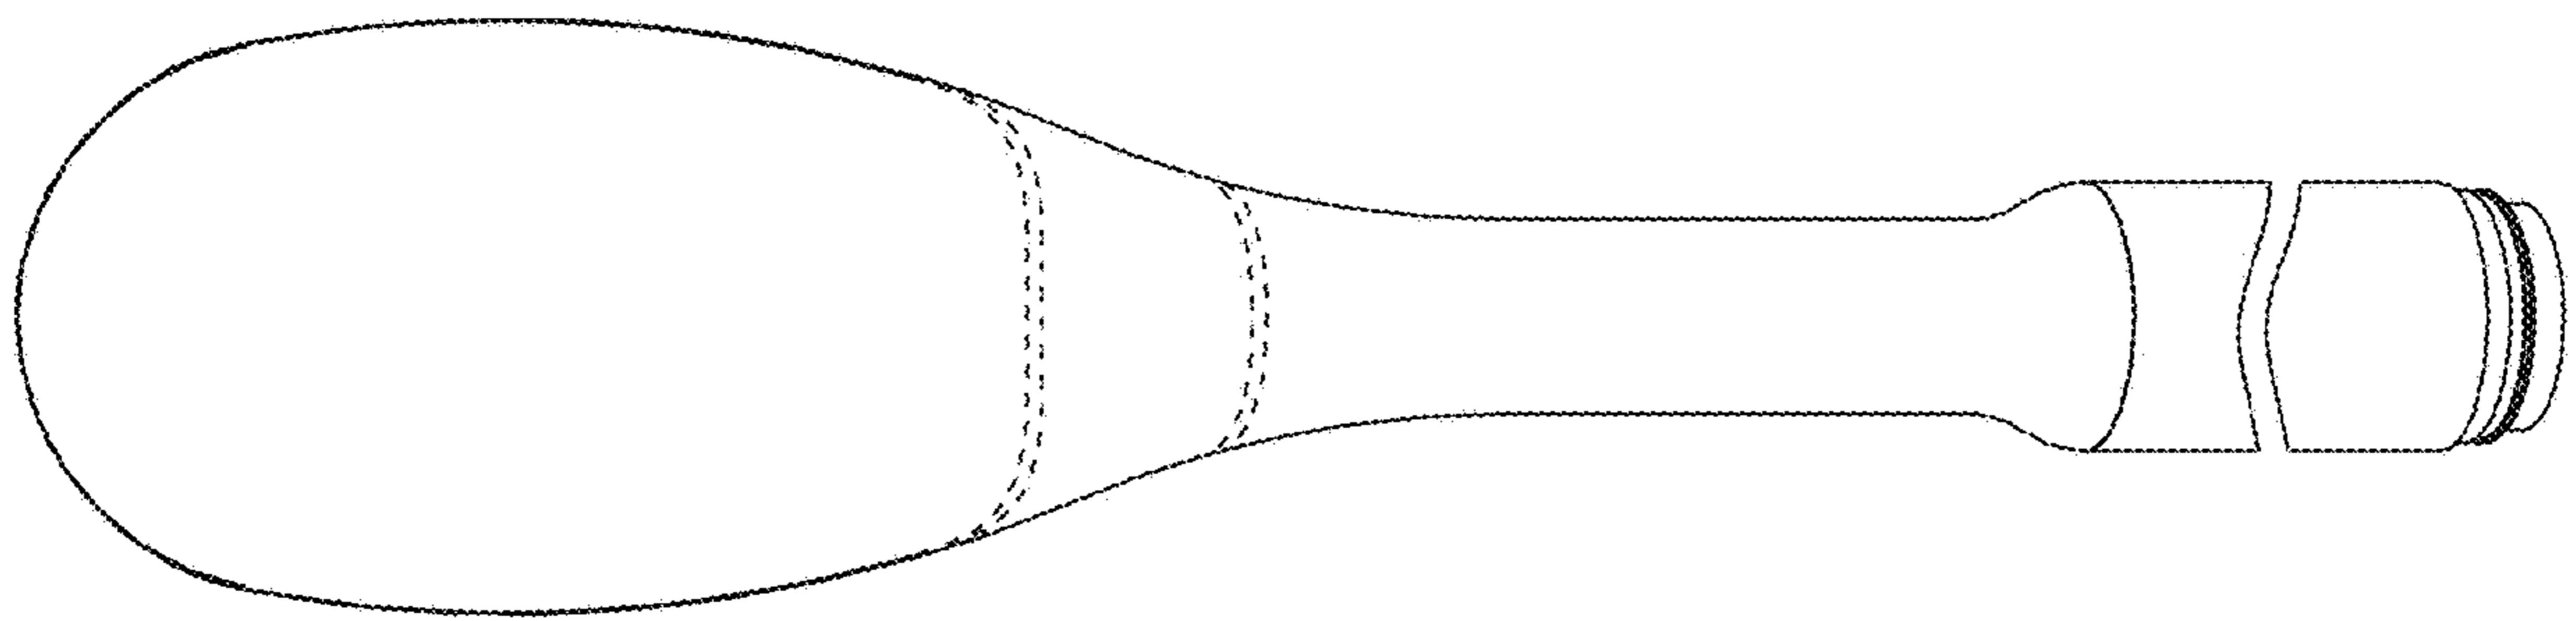


FIG. 13

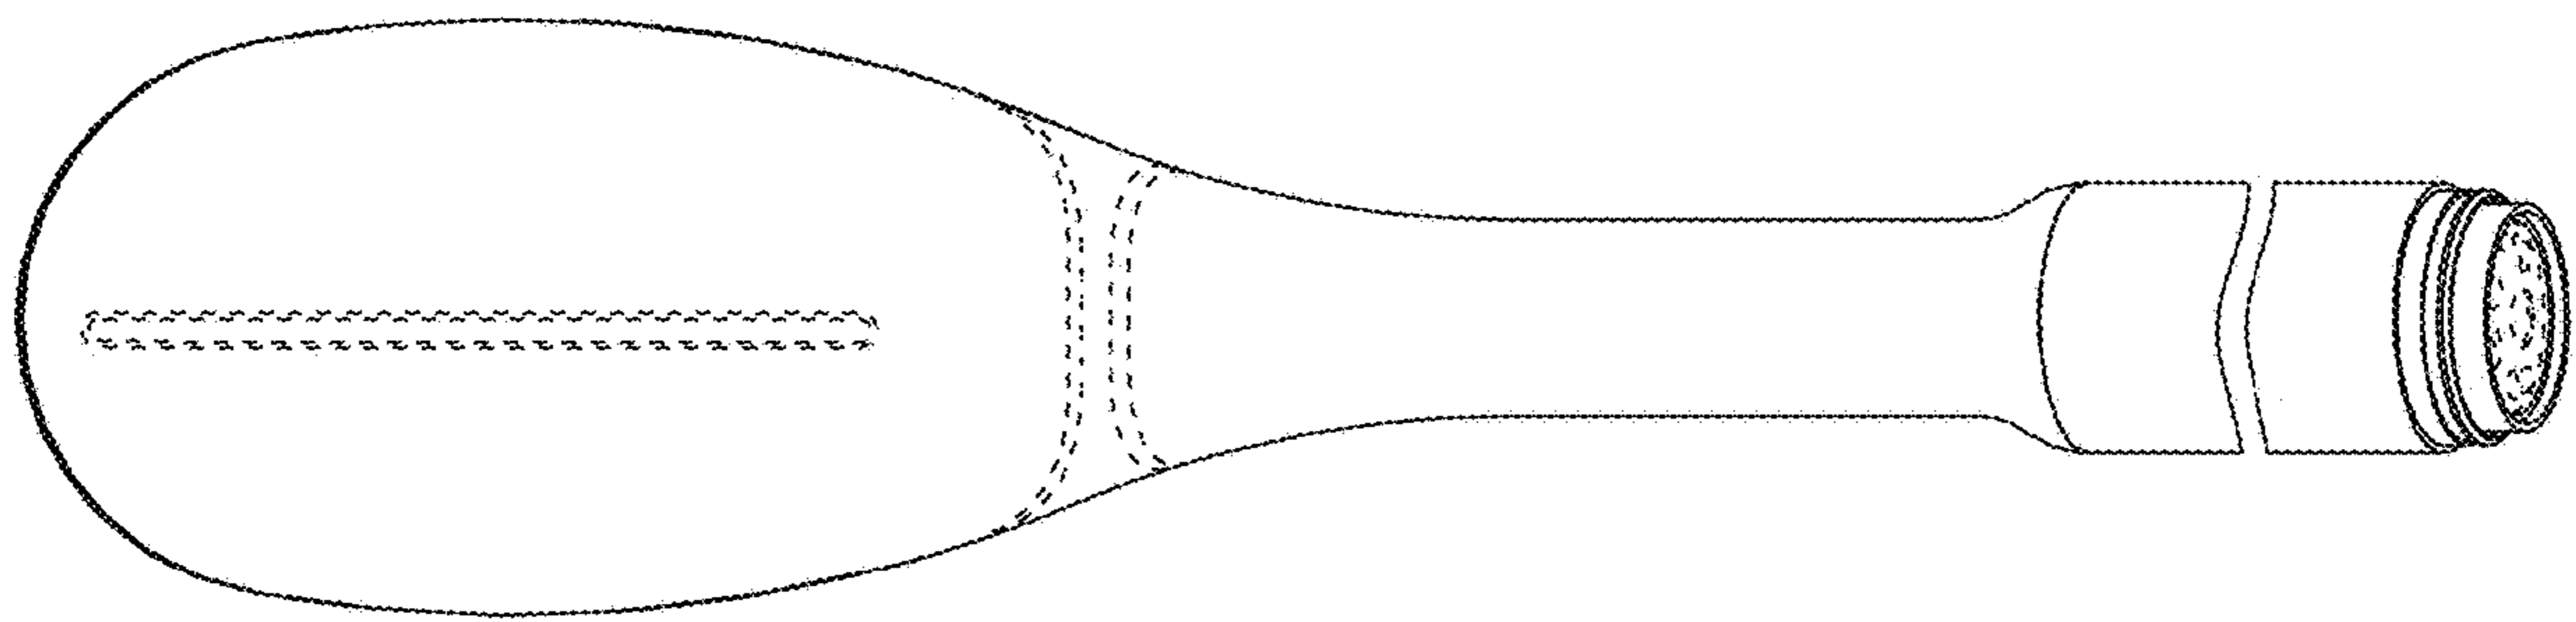


FIG. 14



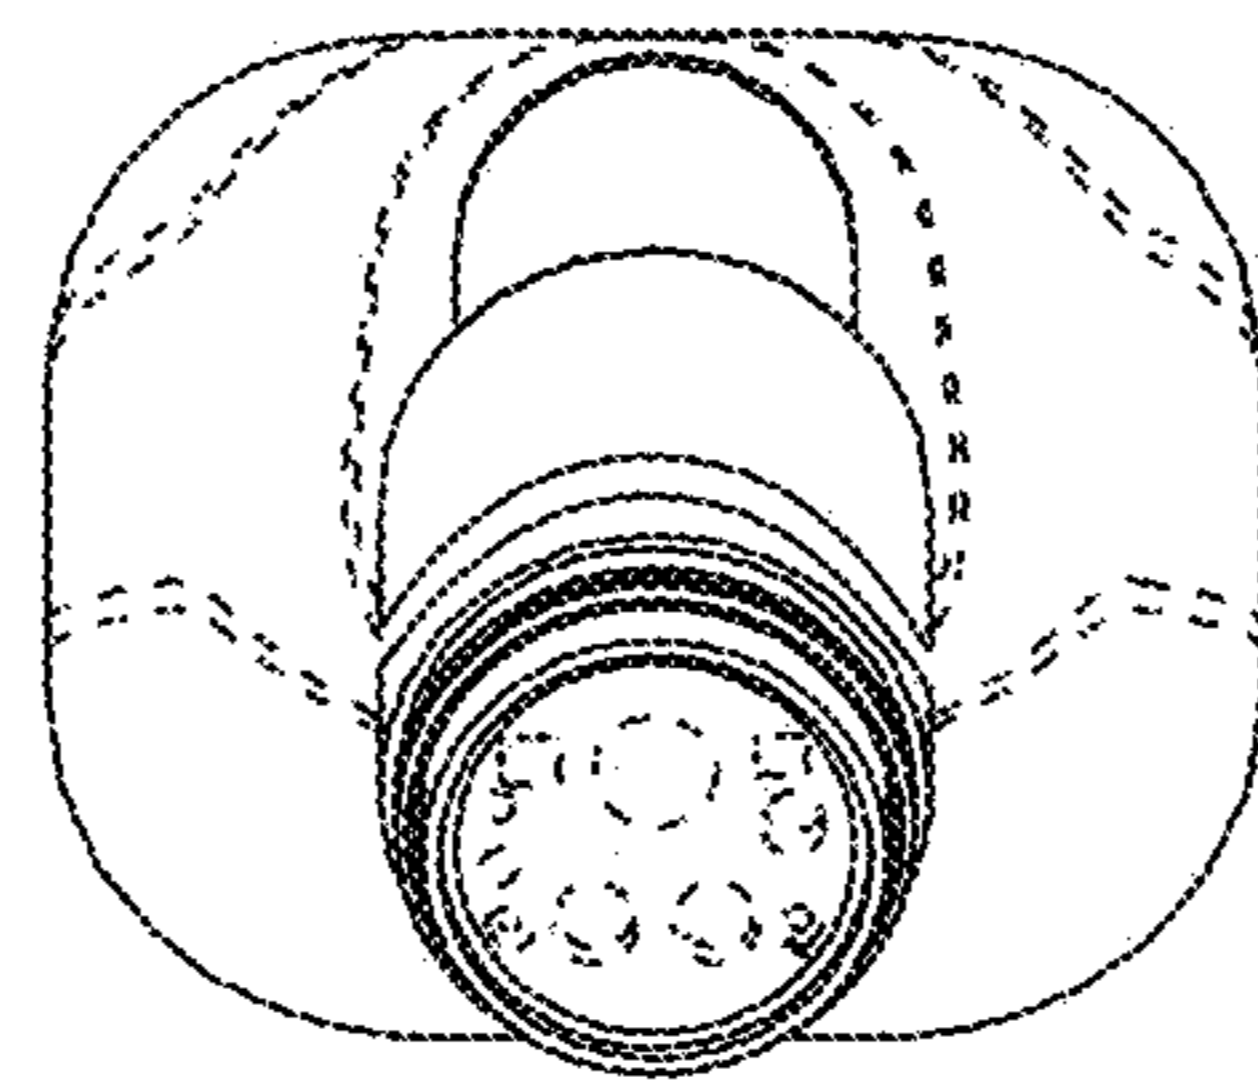


FIG. 15

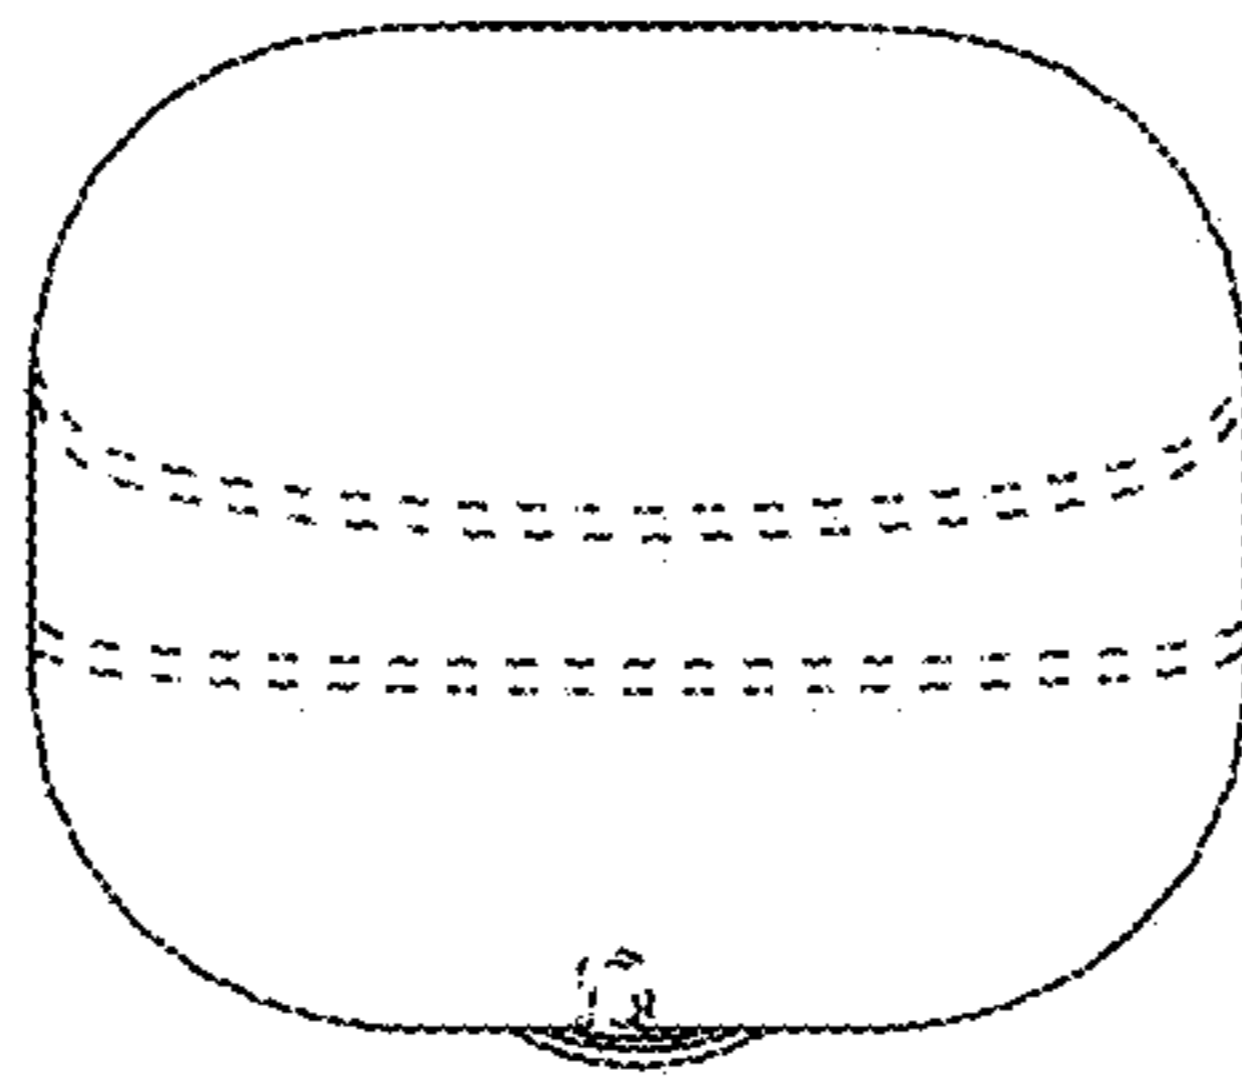


FIG. 16