



US00D960357S

(12) **United States Design Patent**
Balkovec

(10) **Patent No.:** **US D960,357 S**

(45) **Date of Patent:** **** Aug. 9, 2022**

(54) **PIERCING STYLET WITH
NON-CONTACTING DISTAL TIP**

(71) Applicant: **Baylis Medical Company Inc.**,
Montreal (CA)

(72) Inventor: **Christian Balkovec**, Burlington (CA)

(73) Assignee: **Baylis Medical Company Inc.**,
Mississauga (CA)

(**) Term: **15 Years**

(21) Appl. No.: **29/740,458**

(22) Filed: **Jul. 3, 2020**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/112**

(58) **Field of Classification Search**
USPC D24/108, 112, 127, 130, 133, 138, 140,
D24/144, 146, 147; 128/200.26, 207.14;
600/585; 604/170.02, 170.03, 264, 540;
606/129
CPC A61M 25/0102; A61M 25/06; A61M
25/0067; A61M 16/0488; A61B 17/3478
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,945,117 A * 3/1976 Beaver A61B 17/32093
30/287
3,957,055 A * 5/1976 Linder A61M 16/0488
128/200.26
4,185,639 A * 1/1980 Linder A61M 16/0488
128/200.26

(Continued)

FOREIGN PATENT DOCUMENTS

CN 304959208 * 12/2018

OTHER PUBLICATIONS

[Comparison of four methods of endotracheal tube passage in simulated airways: There is room for improved techniques], available on onlinelibrary.wiley.com, by [Kingma, Kirsten et al.], Published [Nov. 7, 2017] [online], [site visited Jan. 20, 2022], Internet URL: <https://onlinelibrary.wiley.com/doi/full/10.1111/1742-6723.12874>. (Year: 2017).*

(Continued)

Primary Examiner — Jonathan J Han

Assistant Examiner — Amanda J Berlinski

(74) *Attorney, Agent, or Firm* — Samuel Tekie; Vincent Man; Glenn Arnold

(57) **CLAIM**


The ornamental design for a piercing stylet with non-contacting distal tip, as shown and described.

DESCRIPTION

FIG. 1 is a right side view of the piercing stylet with non-contacting distal tip;
FIG. 2 is a left side view of the piercing stylet with non-contacting distal tip;
FIG. 3 is a front view of the piercing stylet with non-contacting distal tip;
FIG. 4 is a right side 45 degrees from the front view of the piercing stylet with non-contacting distal tip;
FIG. 5 is a left side 45 degrees from the front view of the piercing stylet with non-contacting distal tip;
FIG. 6 is a right side 45 degrees from the rear view of the piercing stylet with non-contacting distal tip;
FIG. 7 is a left side 45 degrees from the rear view of the piercing stylet with non-contacting distal tip; and,
FIG. 8 is a rear view of the piercing stylet with non-contacting distal tip.

The piercing stylet with non-contacting distal tip is shown with a symbolic break in its length. Any portions not shown after the break line form no part of the claimed design.

1 Claim, 6 Drawing Sheets

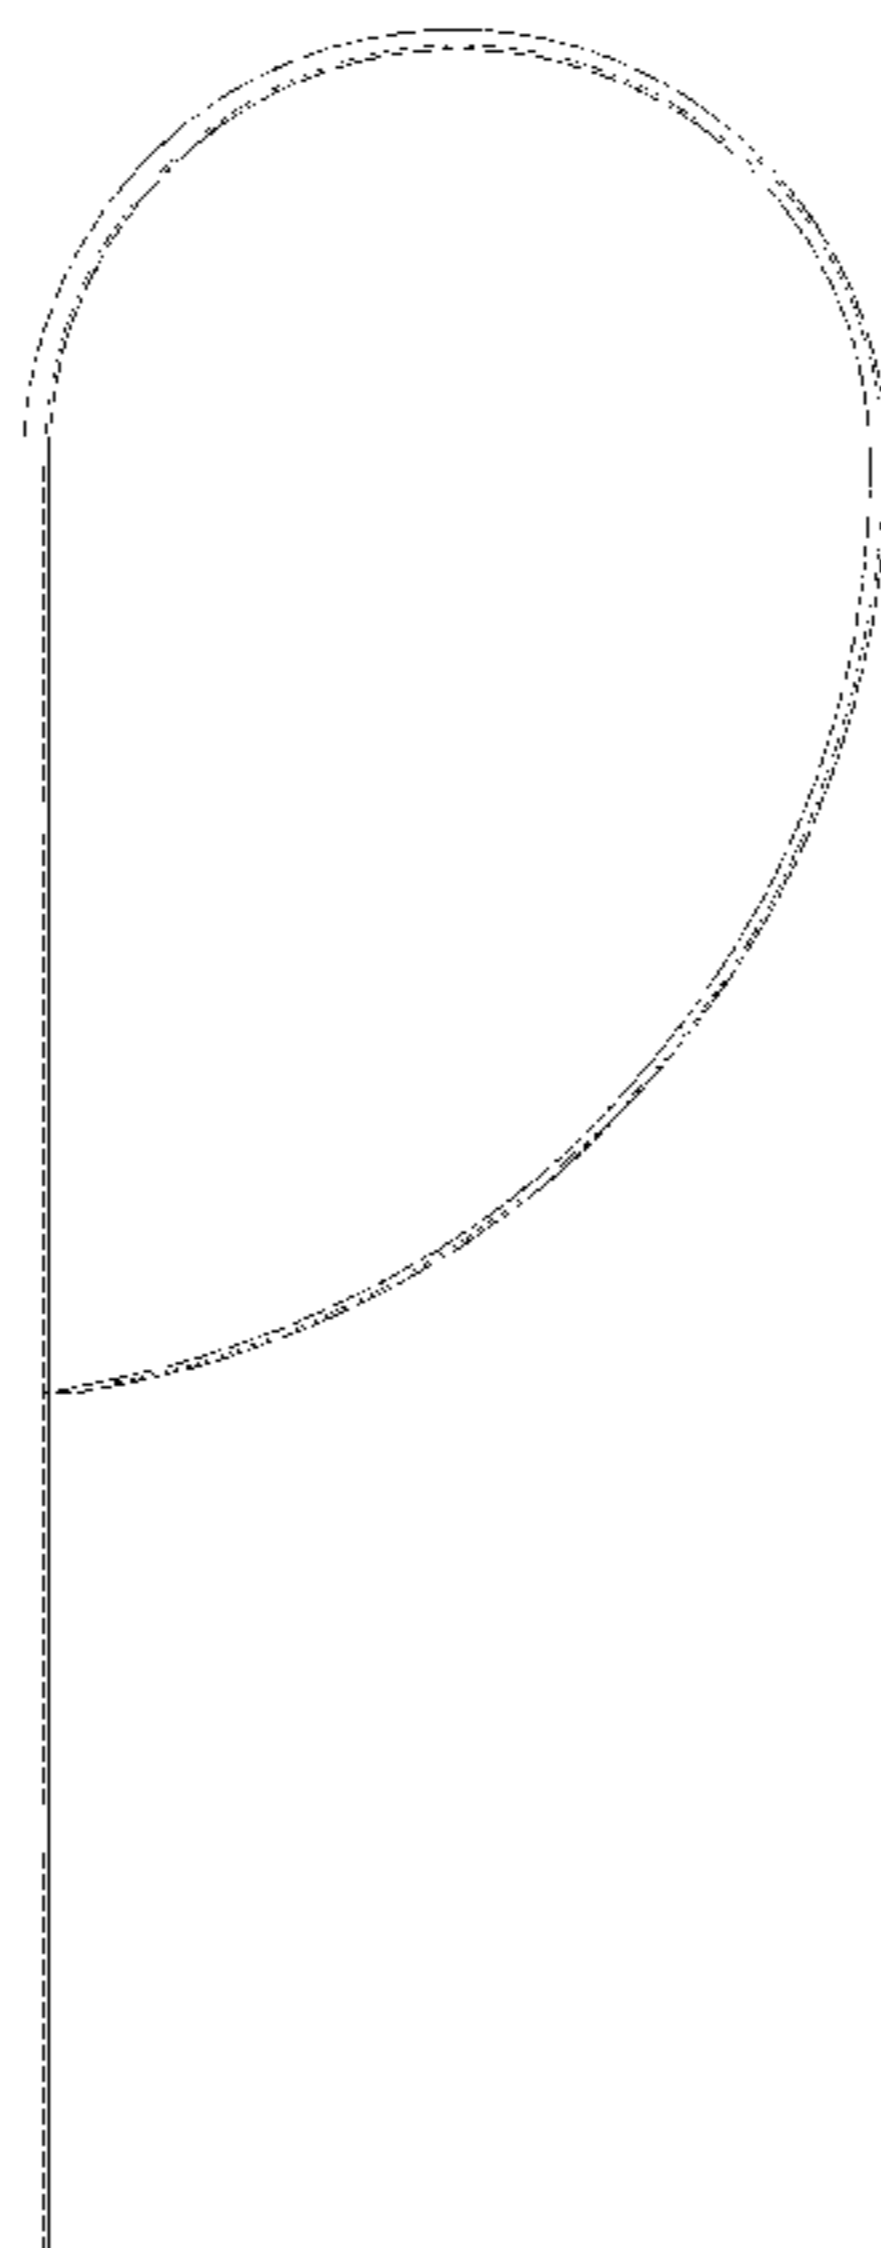

(56)

References Cited

U.S. PATENT DOCUMENTS

4,632,668 A * 12/1986 Wilson, Jr. A61M 27/006
604/540
5,171,232 A * 12/1992 Castillo A61M 25/0054
378/162
5,269,759 A * 12/1993 Hernandez A61M 25/09
600/585
5,318,525 A * 6/1994 West A61B 18/1492
600/585
5,836,926 A * 11/1998 Peterson A61M 25/0012
604/527
6,106,510 A * 8/2000 Lunn A61M 25/0012
600/433
6,503,353 B1 * 1/2003 Peterson A61M 25/0012
156/304.2
6,508,789 B1 * 1/2003 Sinnott A61M 25/0097
604/164.01
8,186,351 B2 * 5/2012 Munro A61M 16/0443
128/207.15
D680,219 S * 4/2013 Davies D24/144
D771,255 S * 11/2016 Weber A61M 16/0434
D24/146
D808,521 S * 1/2018 Bottom A61M 25/013
D24/127
D851,763 S * 6/2019 Mathews D24/147
2003/0045842 A1 * 3/2003 Kawakita A61M 25/007
604/264
2006/0206096 A1 * 9/2006 Accisano, III A61M 25/0082
604/540

2007/0083168 A1 * 4/2007 Whiting A61M 25/0662
604/264
2008/0064988 A1 * 3/2008 Carter A61M 25/09
600/585
2008/0214992 A1 * 9/2008 Haarala A61M 25/0102
604/44
2009/0248035 A1 * 10/2009 Sjostedt A61M 25/0152
606/129
2011/0054447 A1 * 3/2011 Johnson A61M 25/0147
604/540
2012/0078055 A1 * 3/2012 Berci A61M 16/0488
600/188
2013/0150807 A1 * 6/2013 Hamuro A61M 25/0097
604/264
2017/0348467 A1 * 12/2017 Park A61M 25/013
2019/0015644 A1 * 1/2019 Thomspn Smith
A61B 17/3478
2019/0038861 A1 * 2/2019 Bottom A61M 16/04
2021/0205562 A1 * 7/2021 Toth A61M 16/0434
2021/0322730 A1 * 10/2021 Hayzelden A61M 25/0138

OTHER PUBLICATIONS

[Versa Cross RF Transseptal Solution], available on baylismedical.com, Published [2019] [online], [site visited Jan. 20, 2022], Internet URL: <https://www.baylismedical.com/system/resource_files/PRM-00556%20EN%20VersaCross%20Order%20Guide%20DIGITAL%20J-1,2%20V-5.pdf>. (Year: 2019).*

* cited by examiner

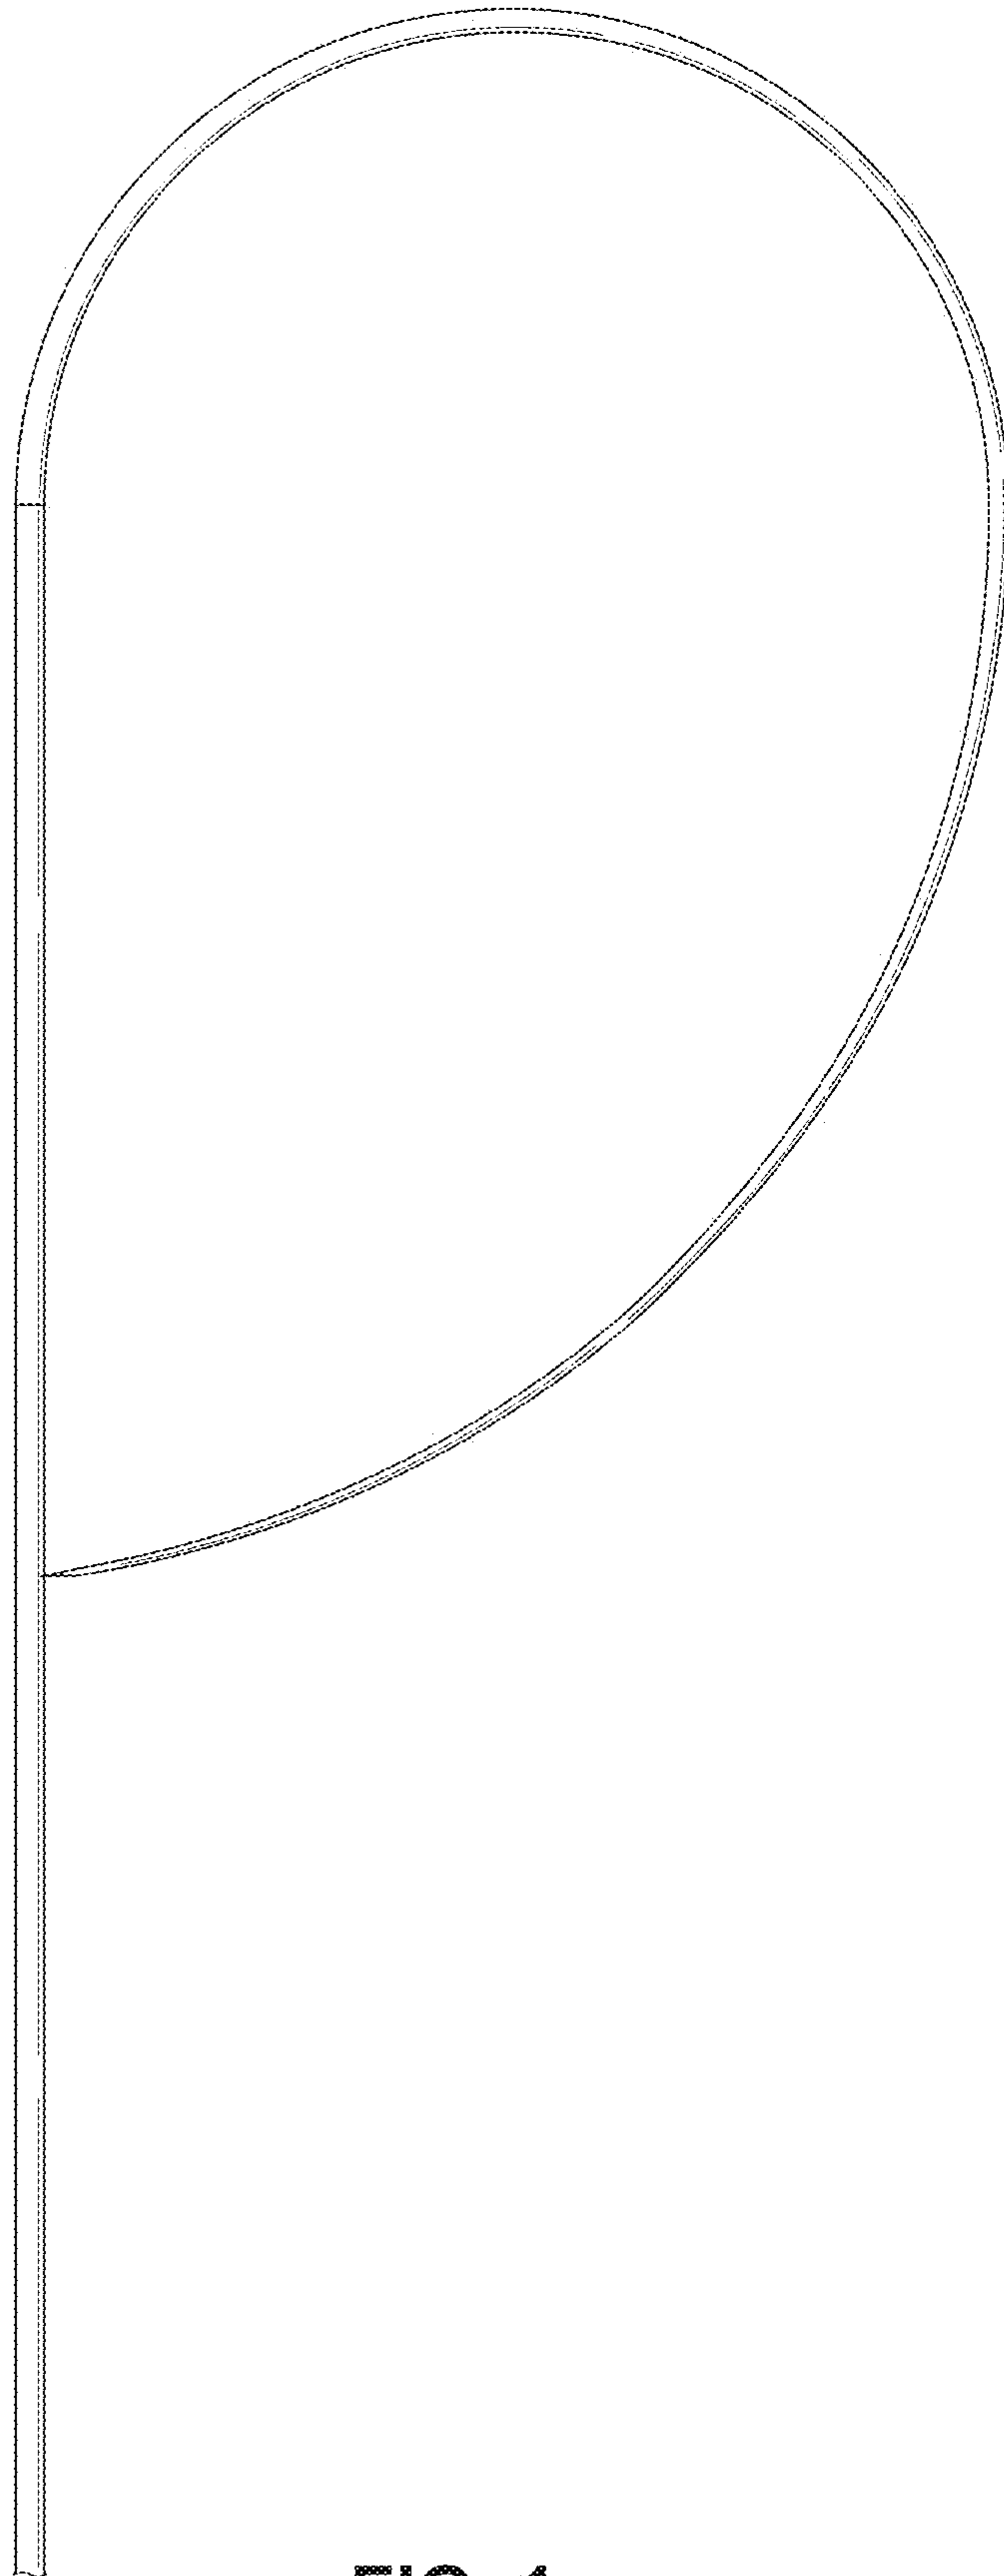


FIG. 1

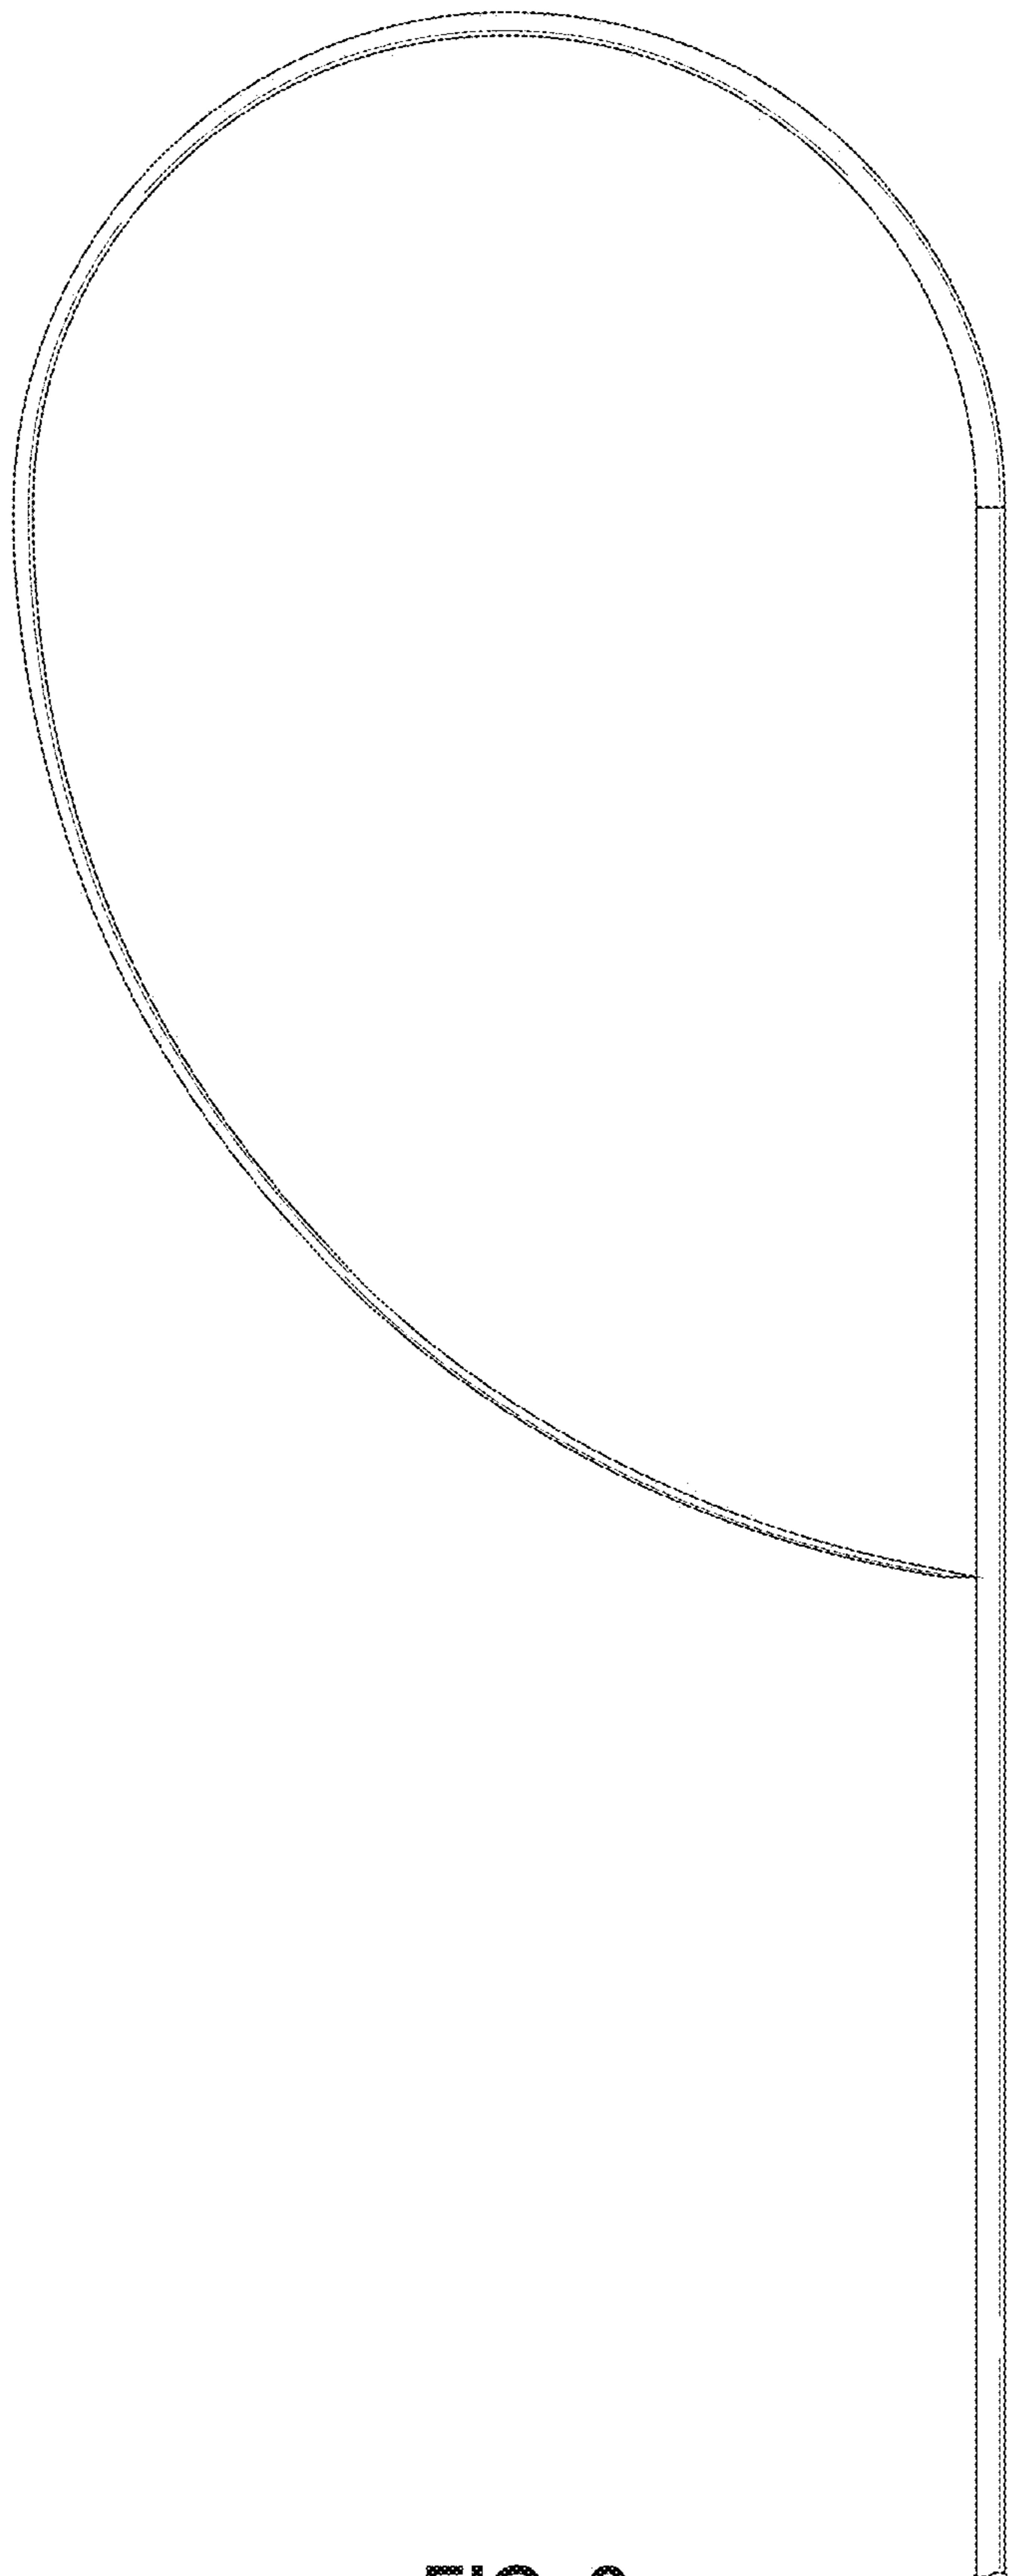


FIG. 2



FIG. 3

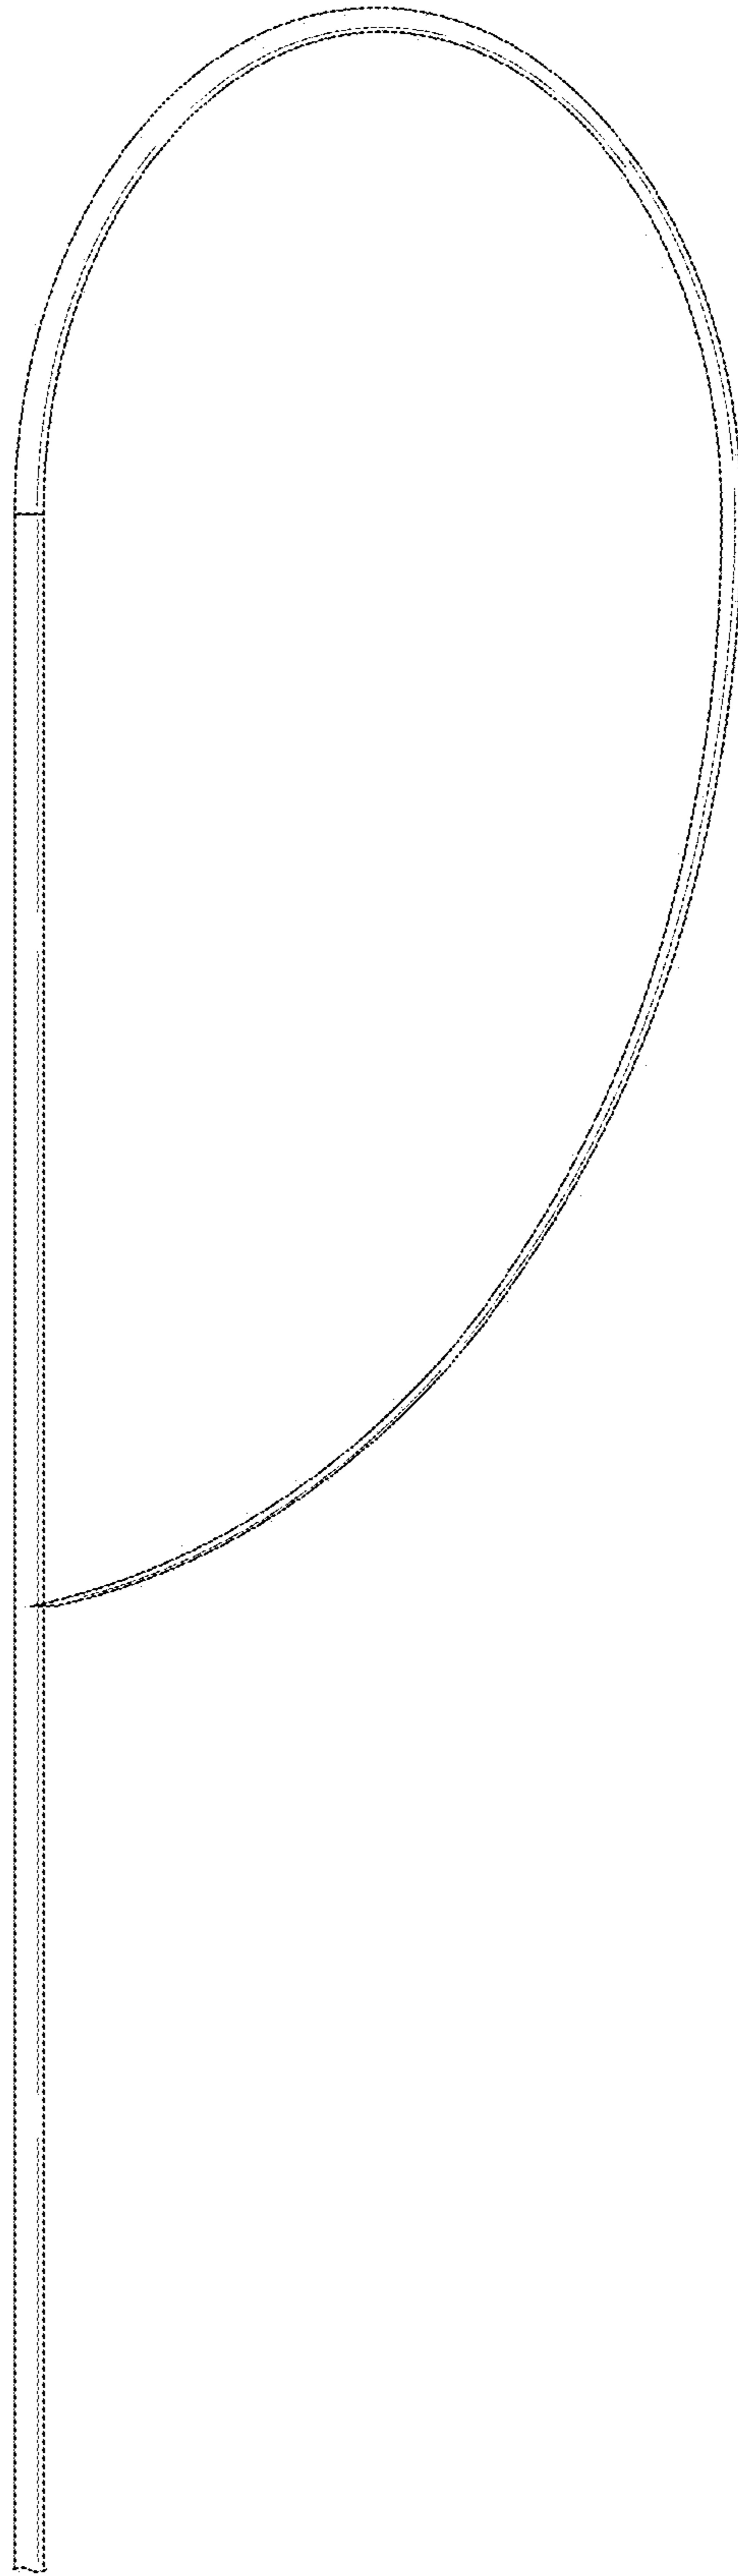


FIG. 4

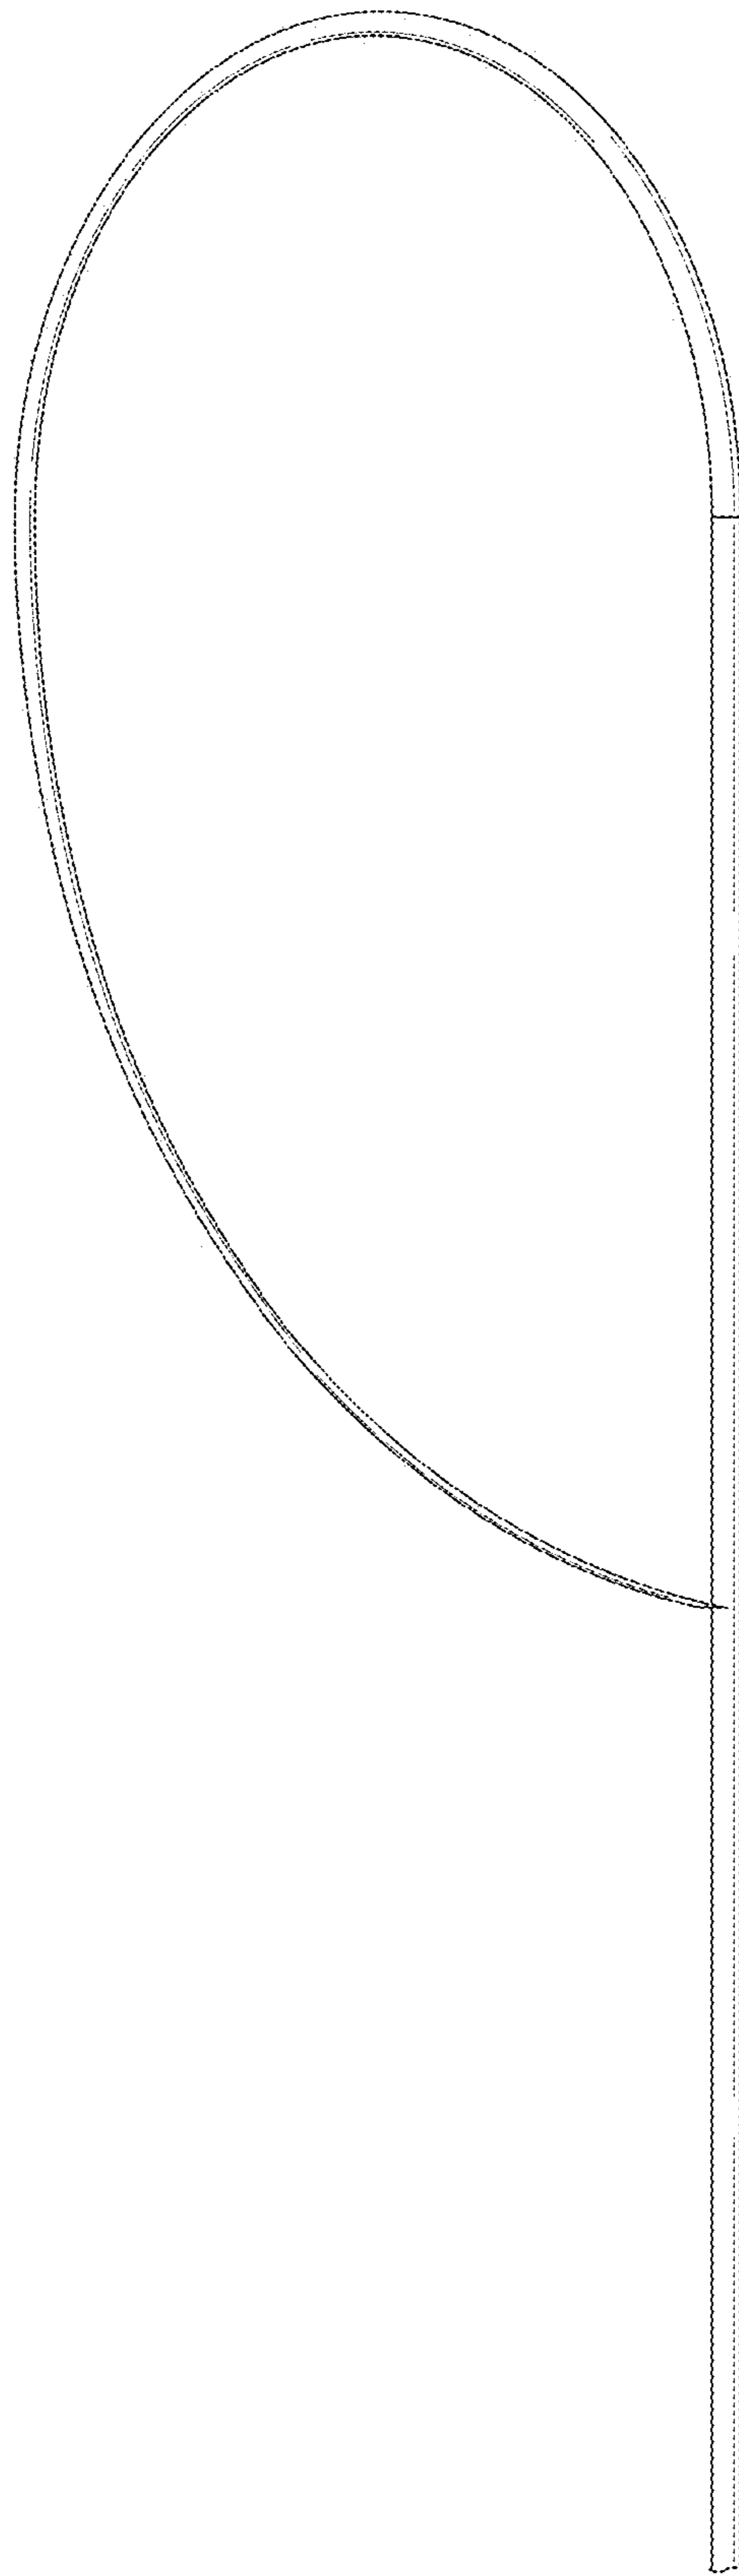


FIG. 5

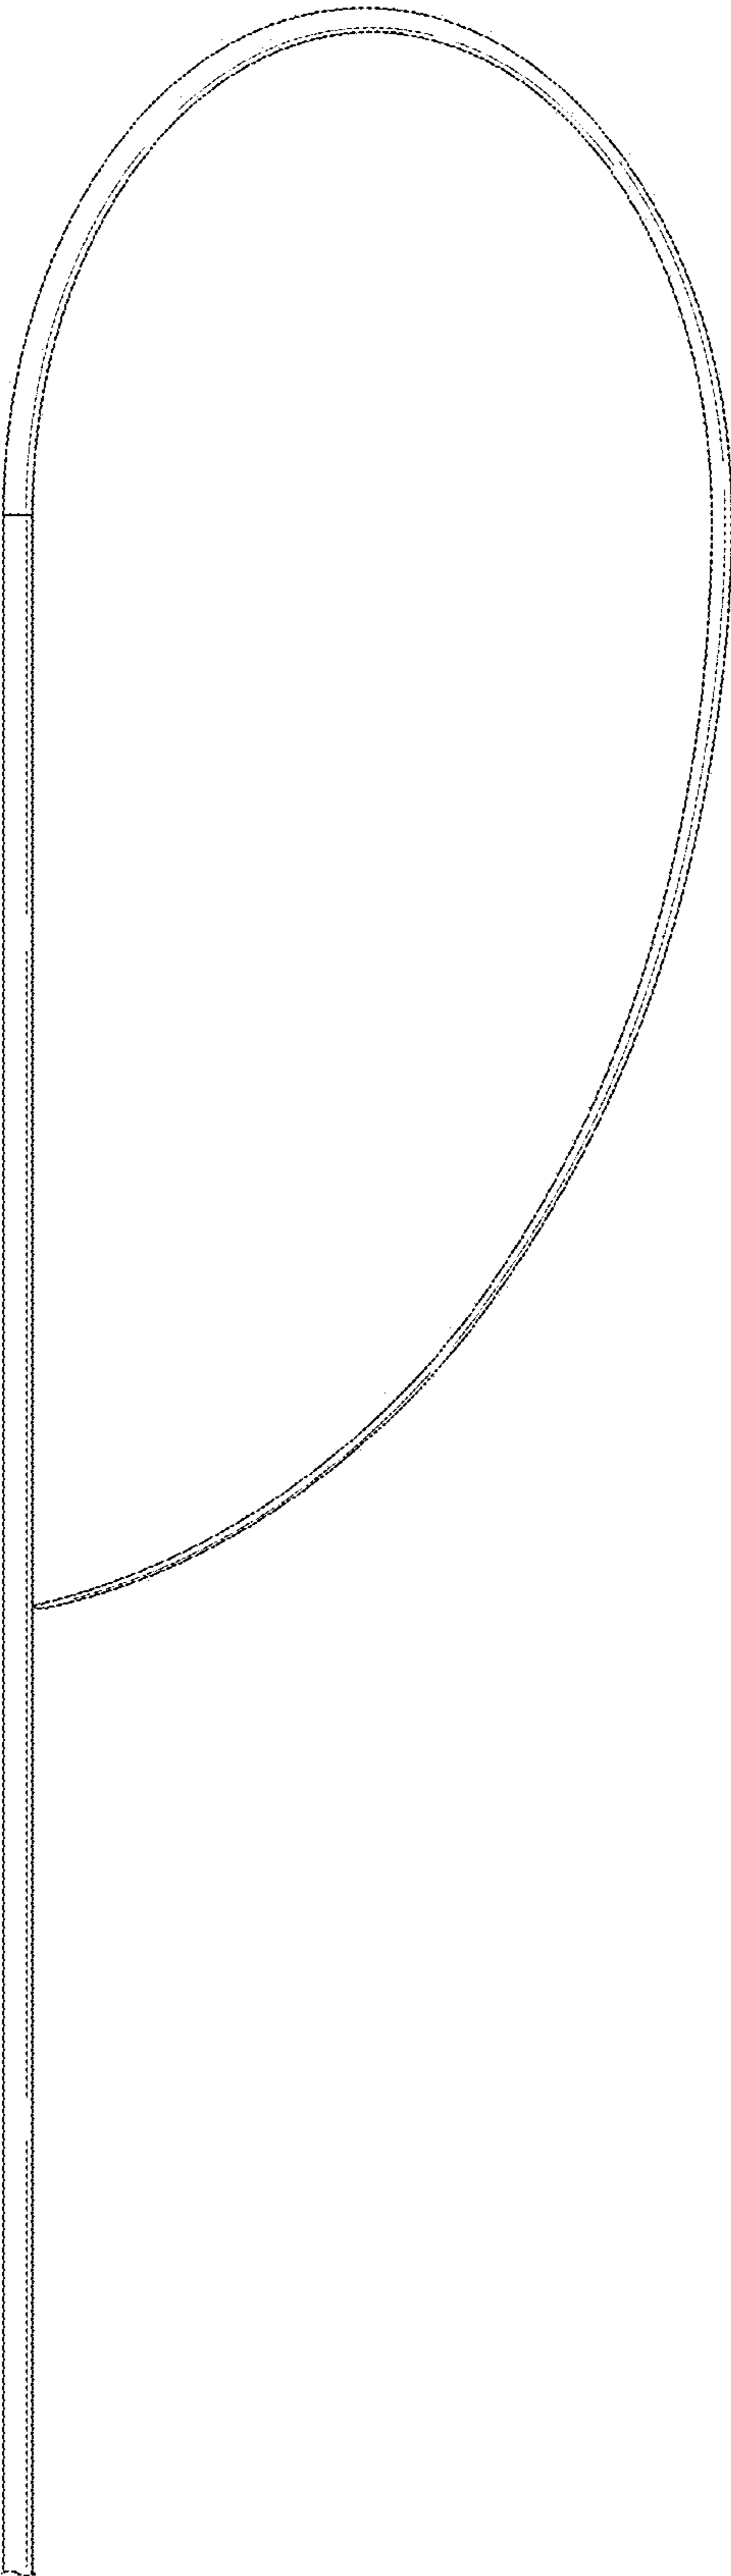


FIG. 6

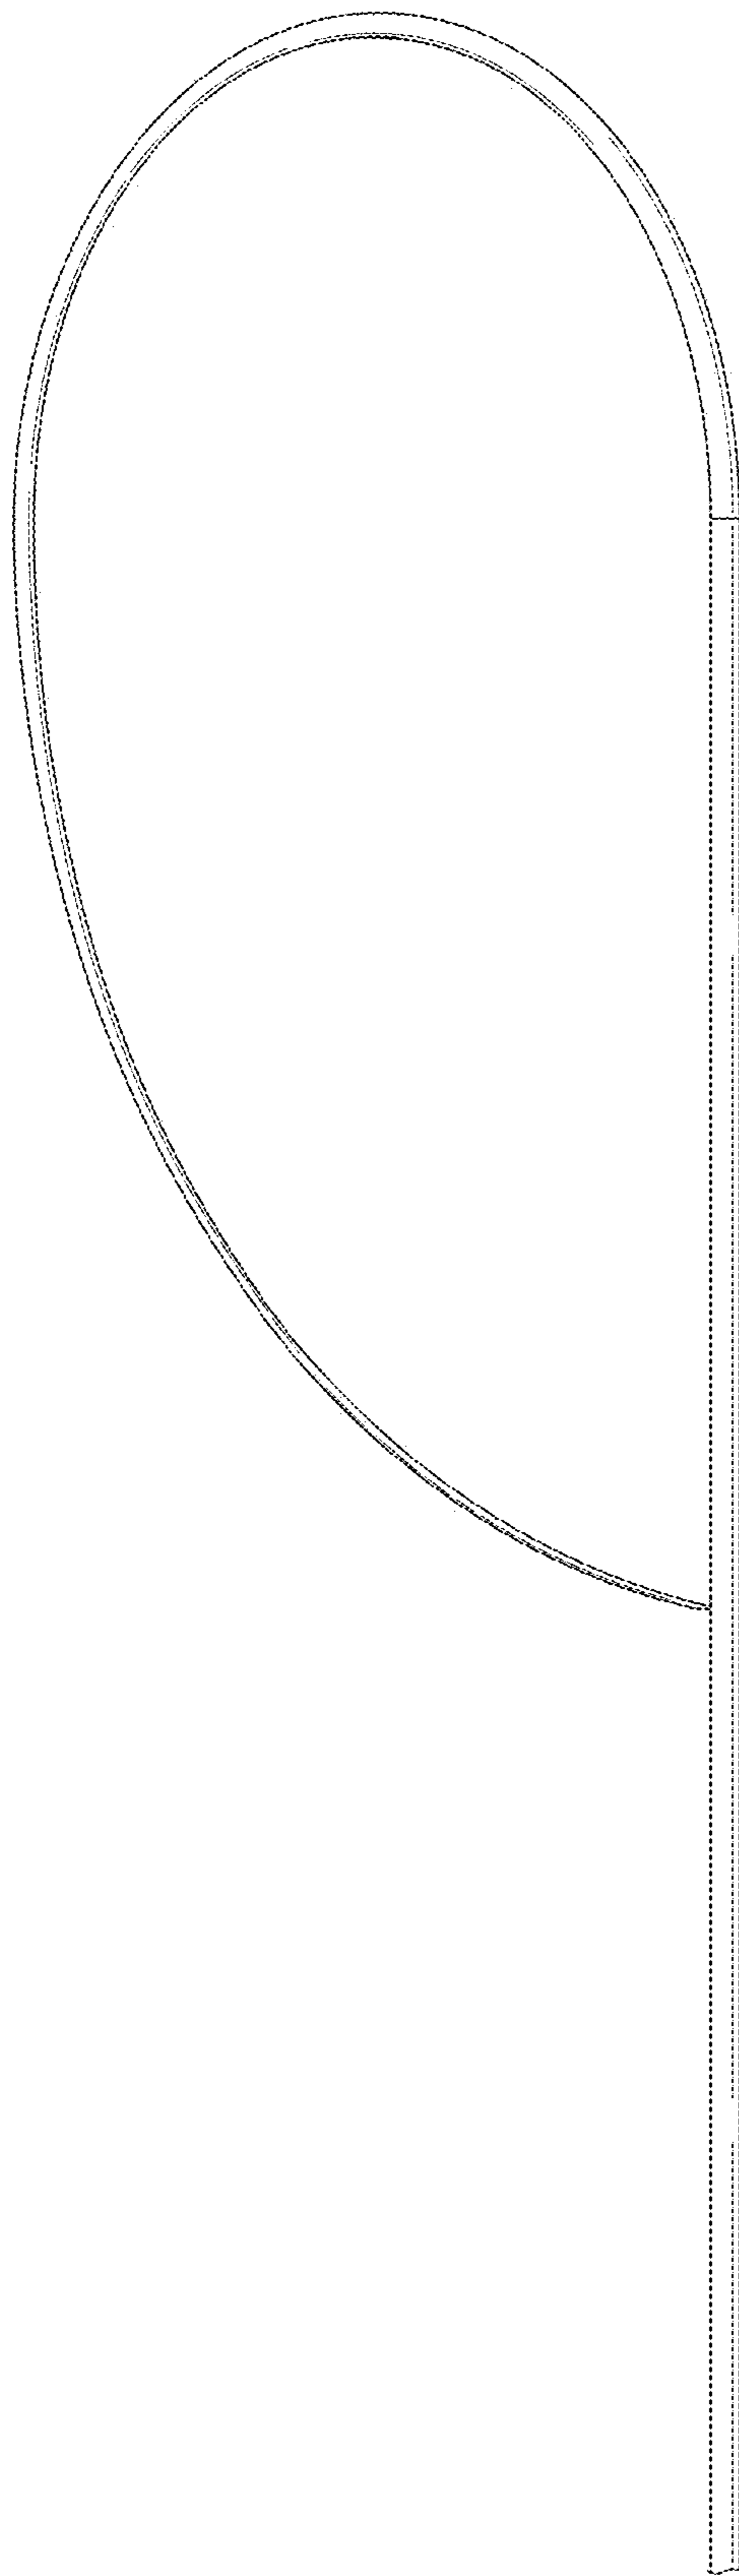


FIG. 7



FIG. 8