



US00D961087S

(12) **United States Design Patent**
Wang

(10) **Patent No.:** **US D961,087 S**

(45) **Date of Patent:** **** Aug. 16, 2022**

(54) **ELECTRONIC SPHYGMOMANOMETER**

(71) Applicant: **SHENZHEN JAMR TECHNOLOGY CO., LIMITED**, Shenzhen (CN)

(72) Inventor: **Liming Wang**, Shenzhen (CN)

(73) Assignee: **SHENZHEN JAMR TECHNOLOGY CO., LIMITED**, Shenzhen (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/714,887**

(22) Filed: **Nov. 26, 2019**

(30) **Foreign Application Priority Data**

May 27, 2019 (CN) 201930265212.6

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/165**

(58) **Field of Classification Search**
USPC D24/165-168, 107, 186-187; D14/344
CPC A61B 5/0404; A61B 5/021; A61B 5/024;
A61B 5/02438; A61B 5/681; A61B
5/0402; A61B 2560/0462
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D566,844 S * 4/2008 Inose D24/165
D700,341 S * 2/2014 Uozumi D24/165
D802,768 S * 11/2017 Rider D24/165
D850,622 S * 6/2019 Noguchi D24/165
D862,702 S * 10/2019 Nishiyama D24/165
D890,346 S * 7/2020 Lam D24/167

D899,599 S * 10/2020 Hirasawa D24/165
D903,120 S * 11/2020 Nishiyama D24/165
2007/0000490 A1 * 1/2007 DeVries F04C 29/0035
128/204.21
2013/0253334 A1 * 9/2013 Al-Ali A61B 5/02416
600/476

OTHER PUBLICATIONS

Series C, posted at jamrmed.com, no posting date, retrieved Dec. 17, 2020, online, URL: http://www.jamrmed.com/pd.jsp?id=65#_pp=105_335 (Year: 2020).*

* cited by examiner

Primary Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Cantor Colburn LLP

(57) **CLAIM**


The ornamental design for an “electronic sphygmomanometer”, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of an electronic sphygmomanometer;
FIG. 2 is a top perspective view thereof;
FIG. 3 is a rear perspective view thereof;
FIG. 4 is a front view thereof;
FIG. 5 is a rear view thereof;
FIG. 6 is a left view thereof;
FIG. 7 is a right view thereof;
FIG. 8 is a top view thereof; and,
FIG. 9 is a bottom view thereof.

The broken lines in the figures depict portions of the electronic sphygmomanometer that form no part of the claimed design.

1 Claim, 9 Drawing Sheets

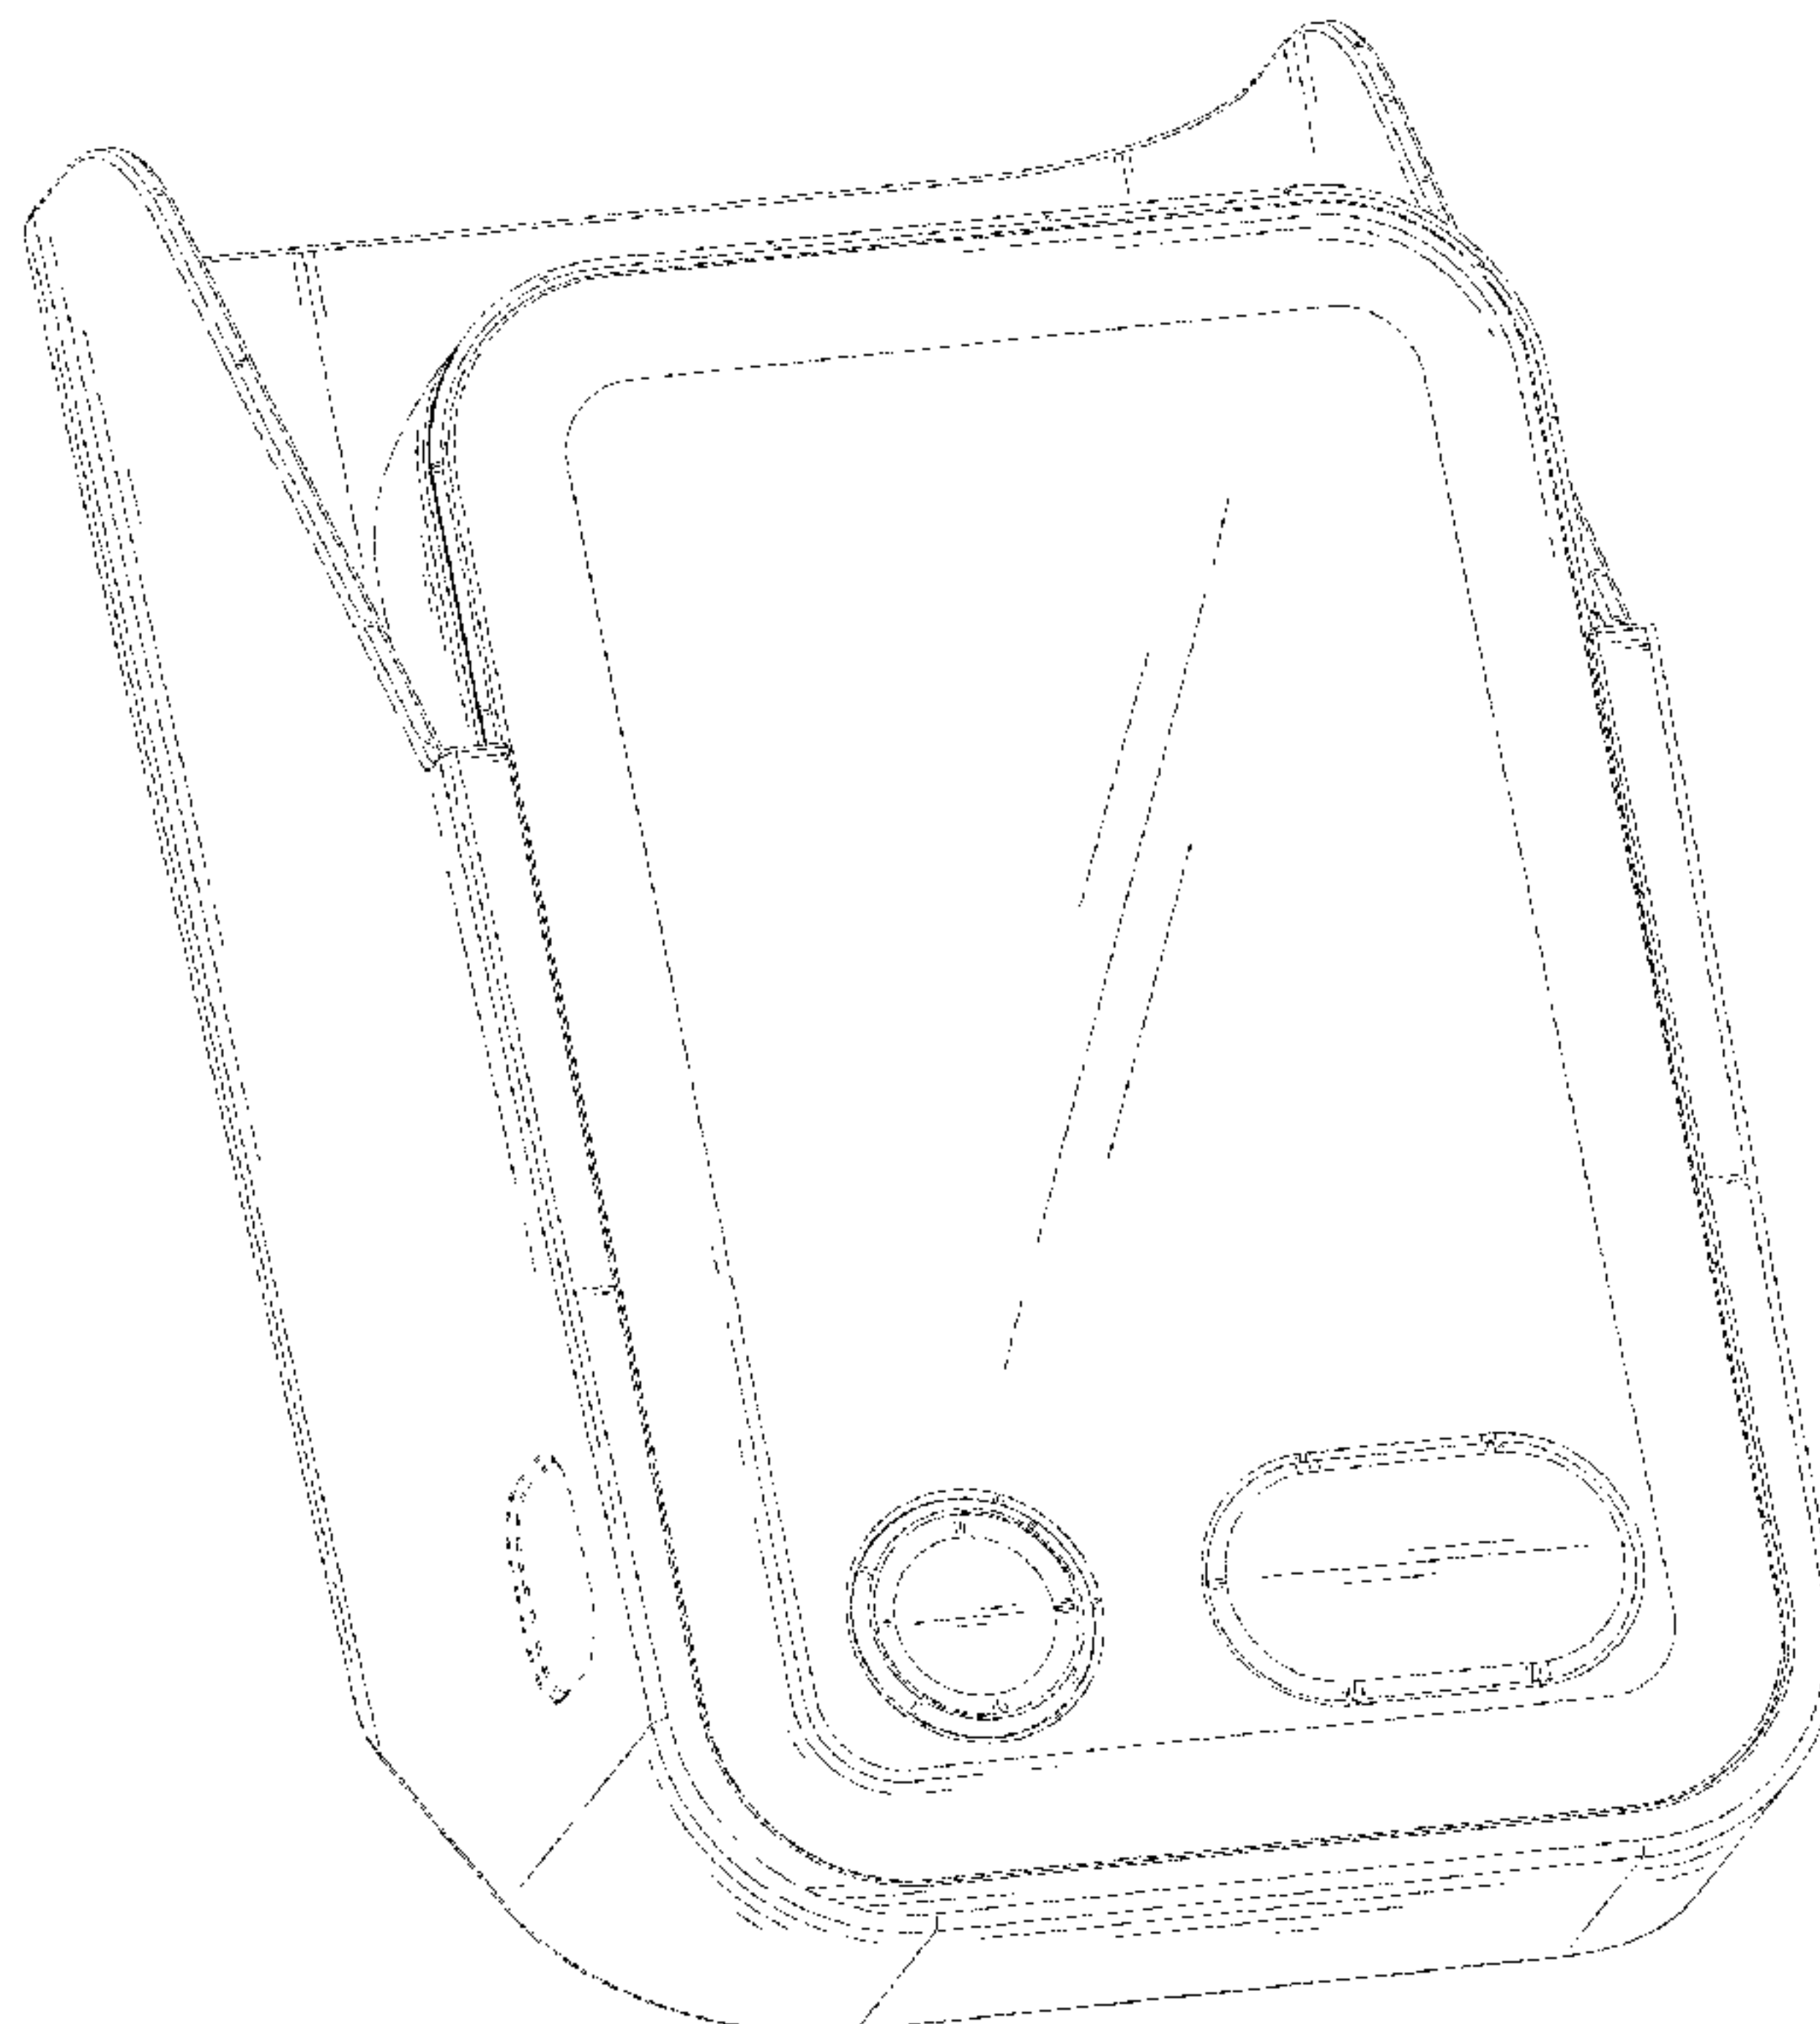

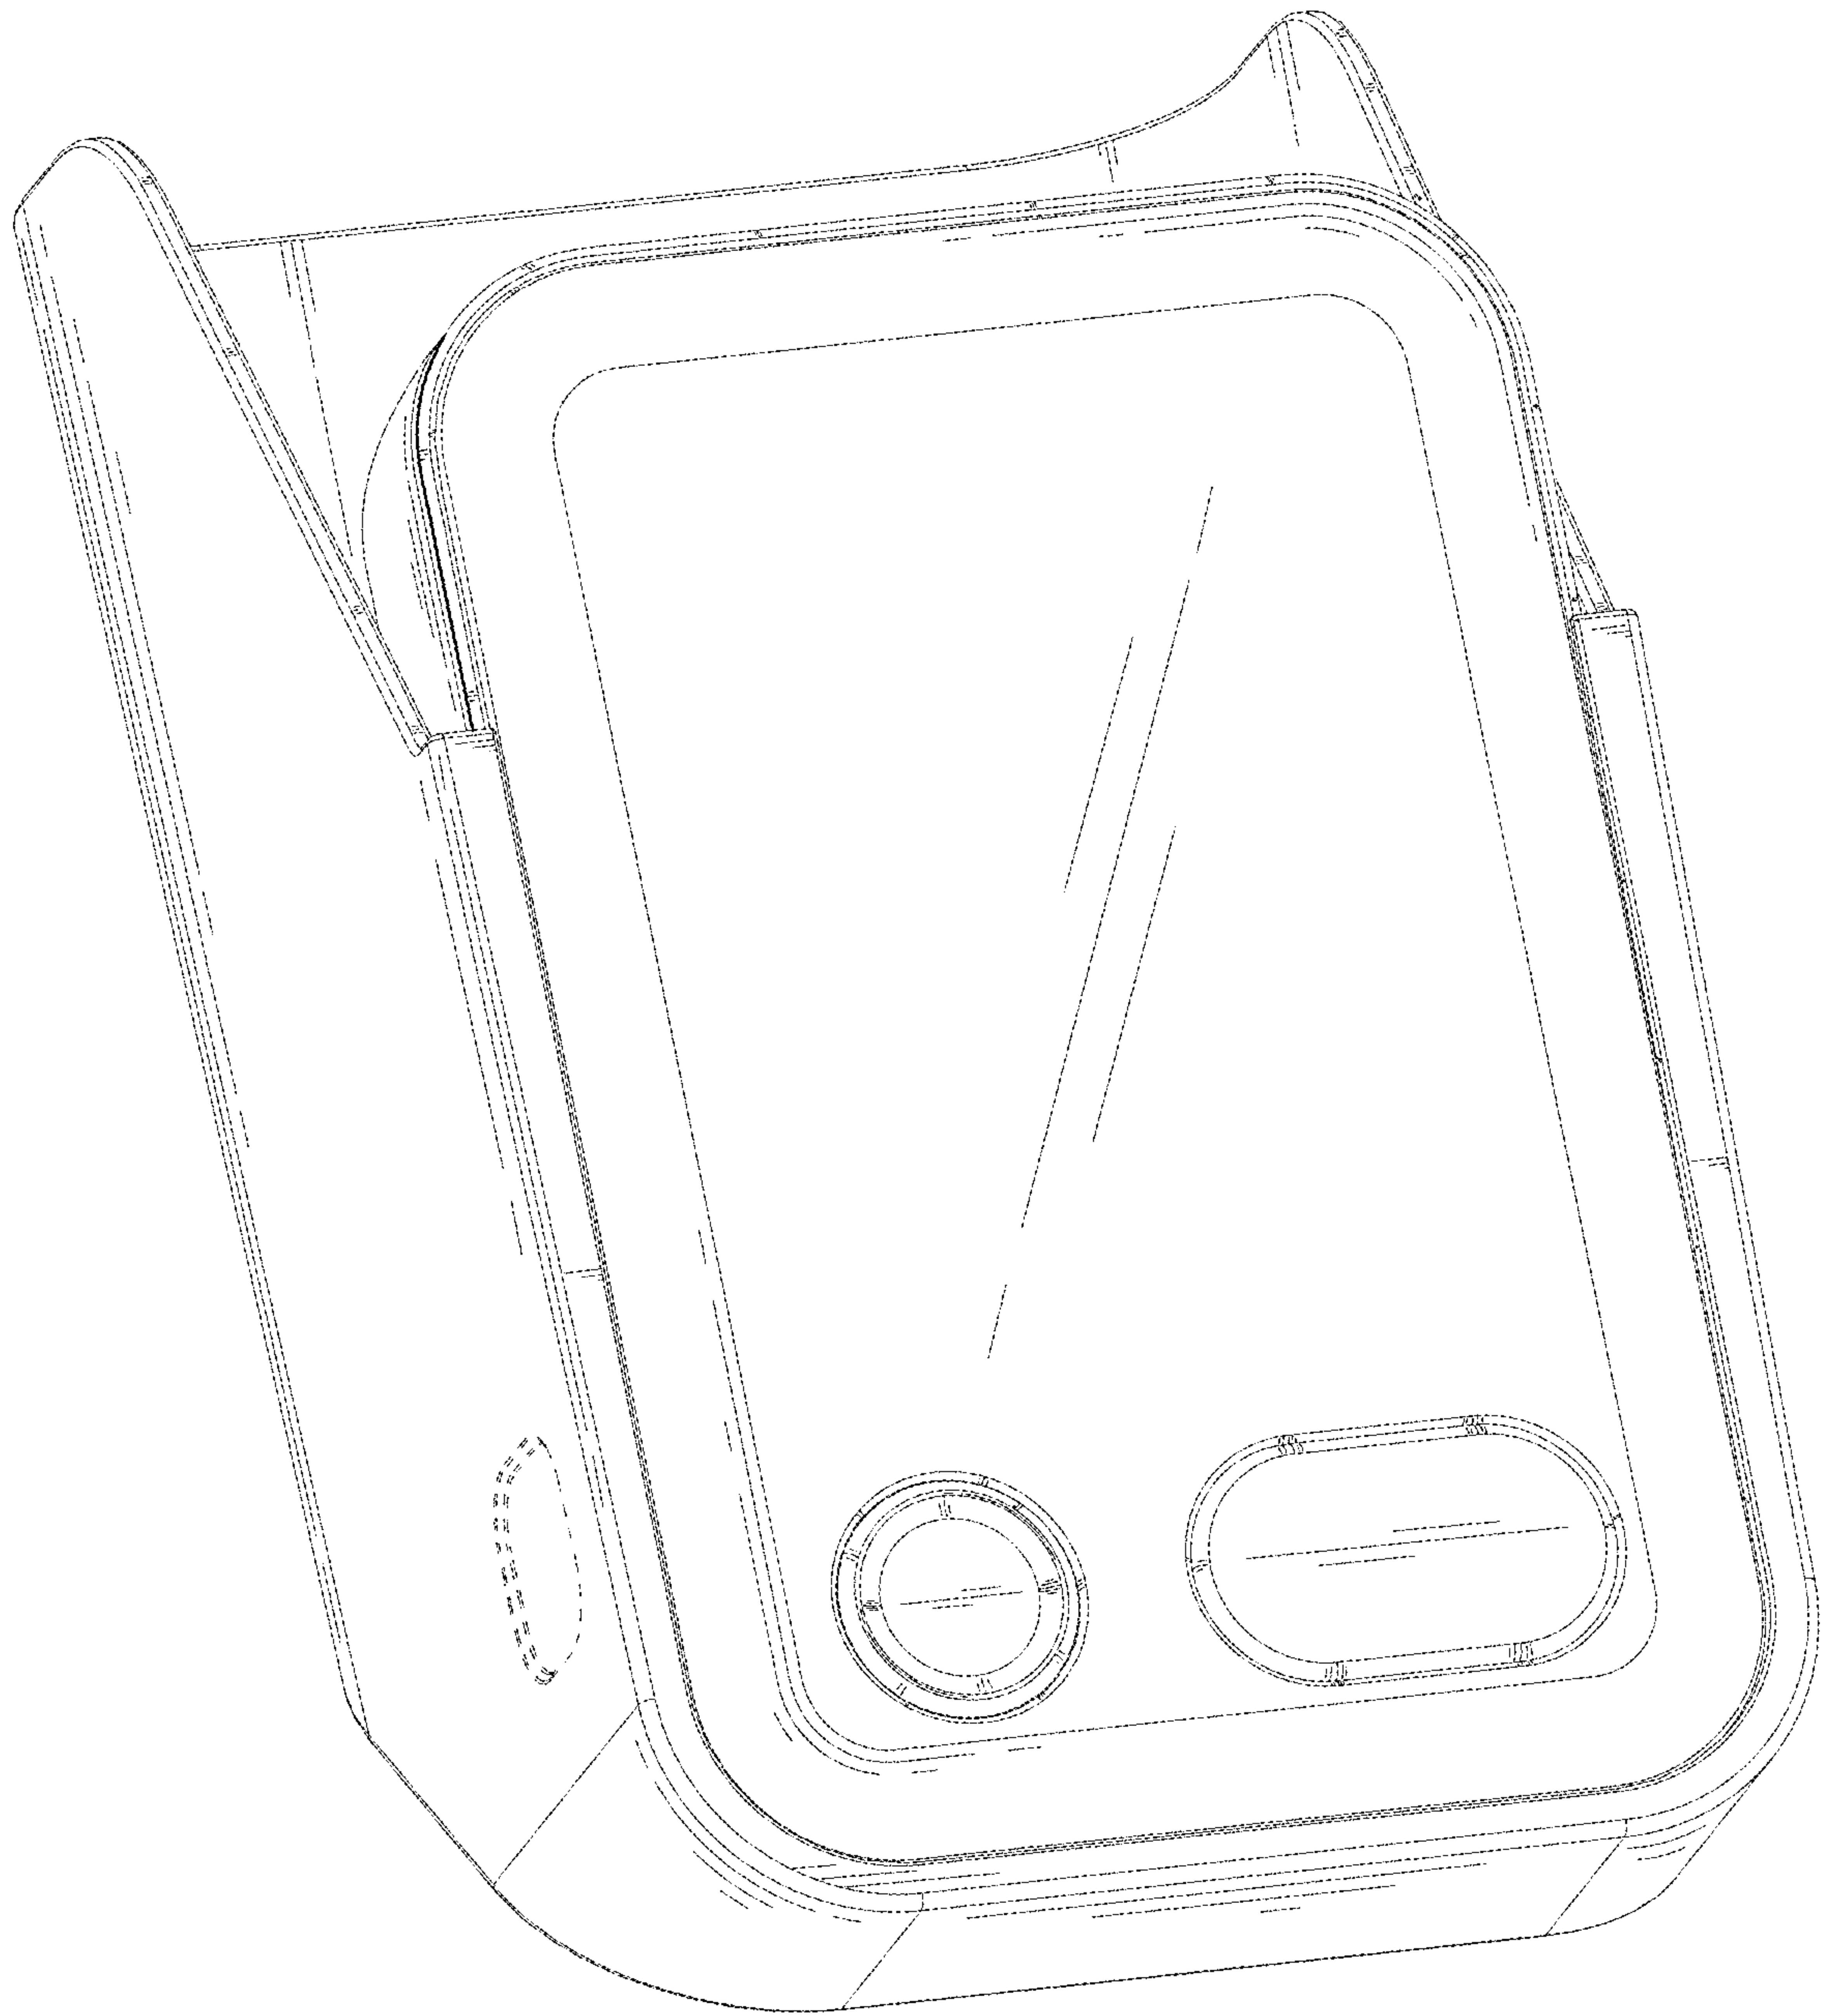


FIG. 1

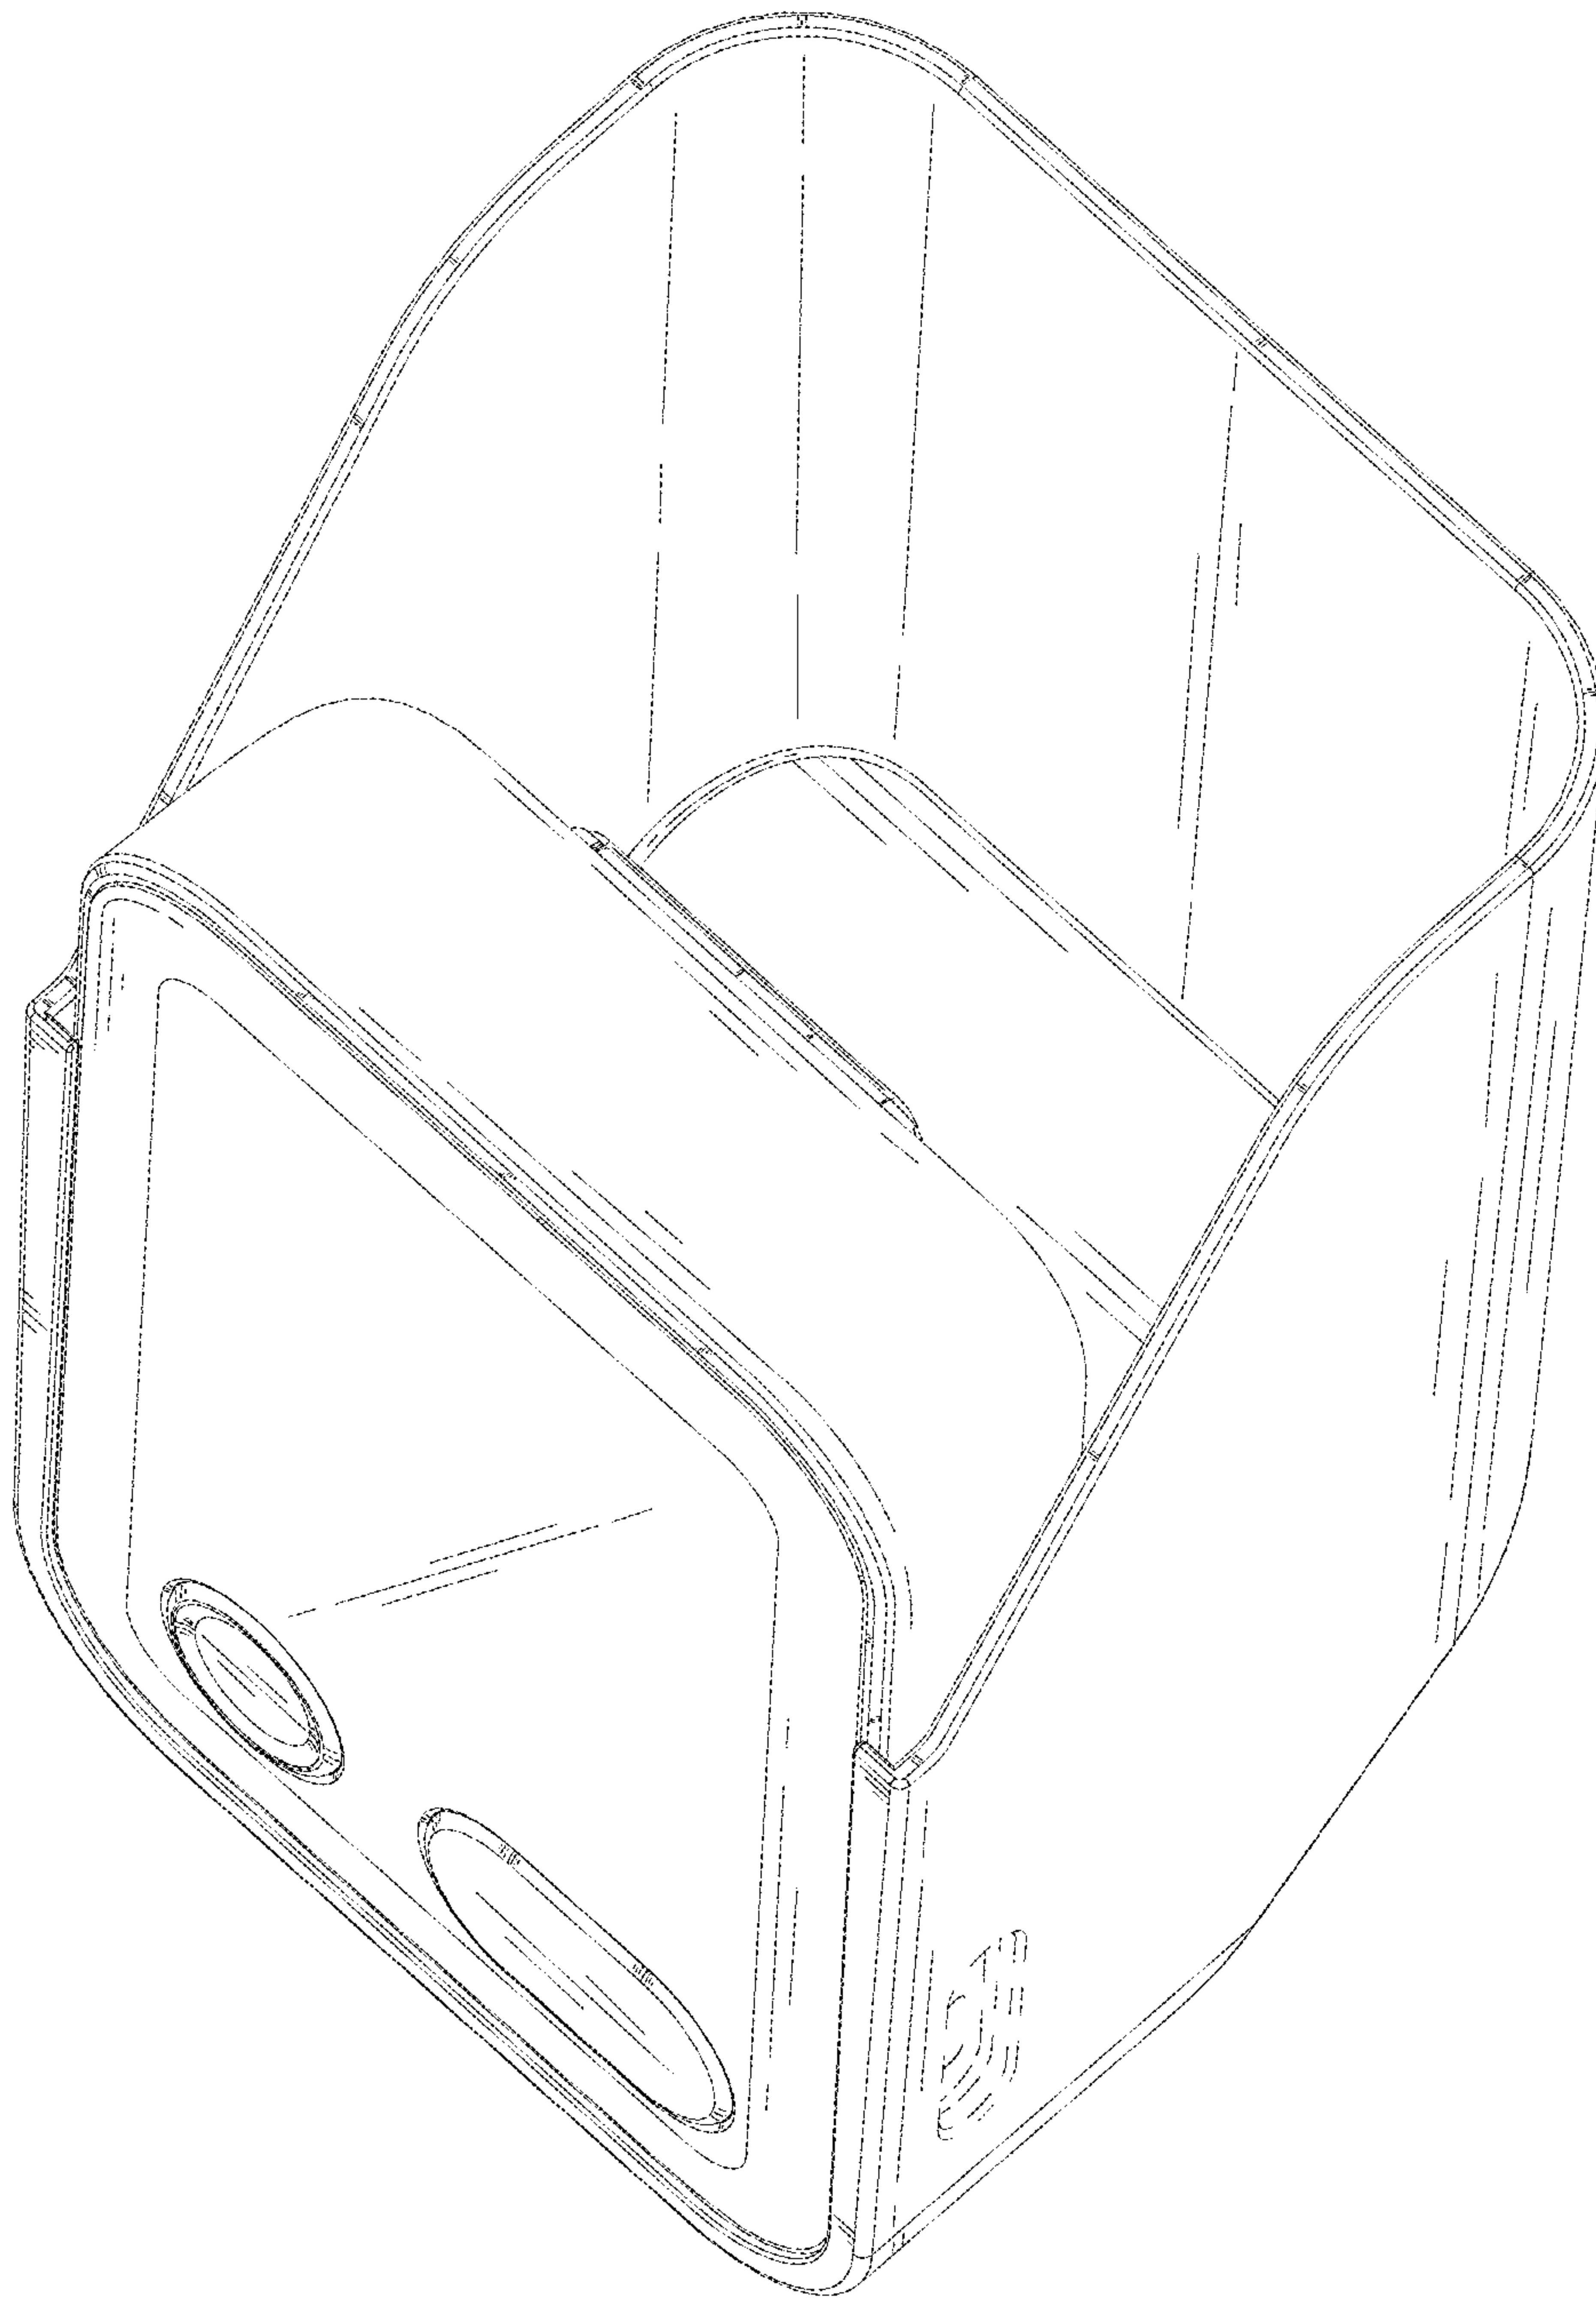


FIG. 2

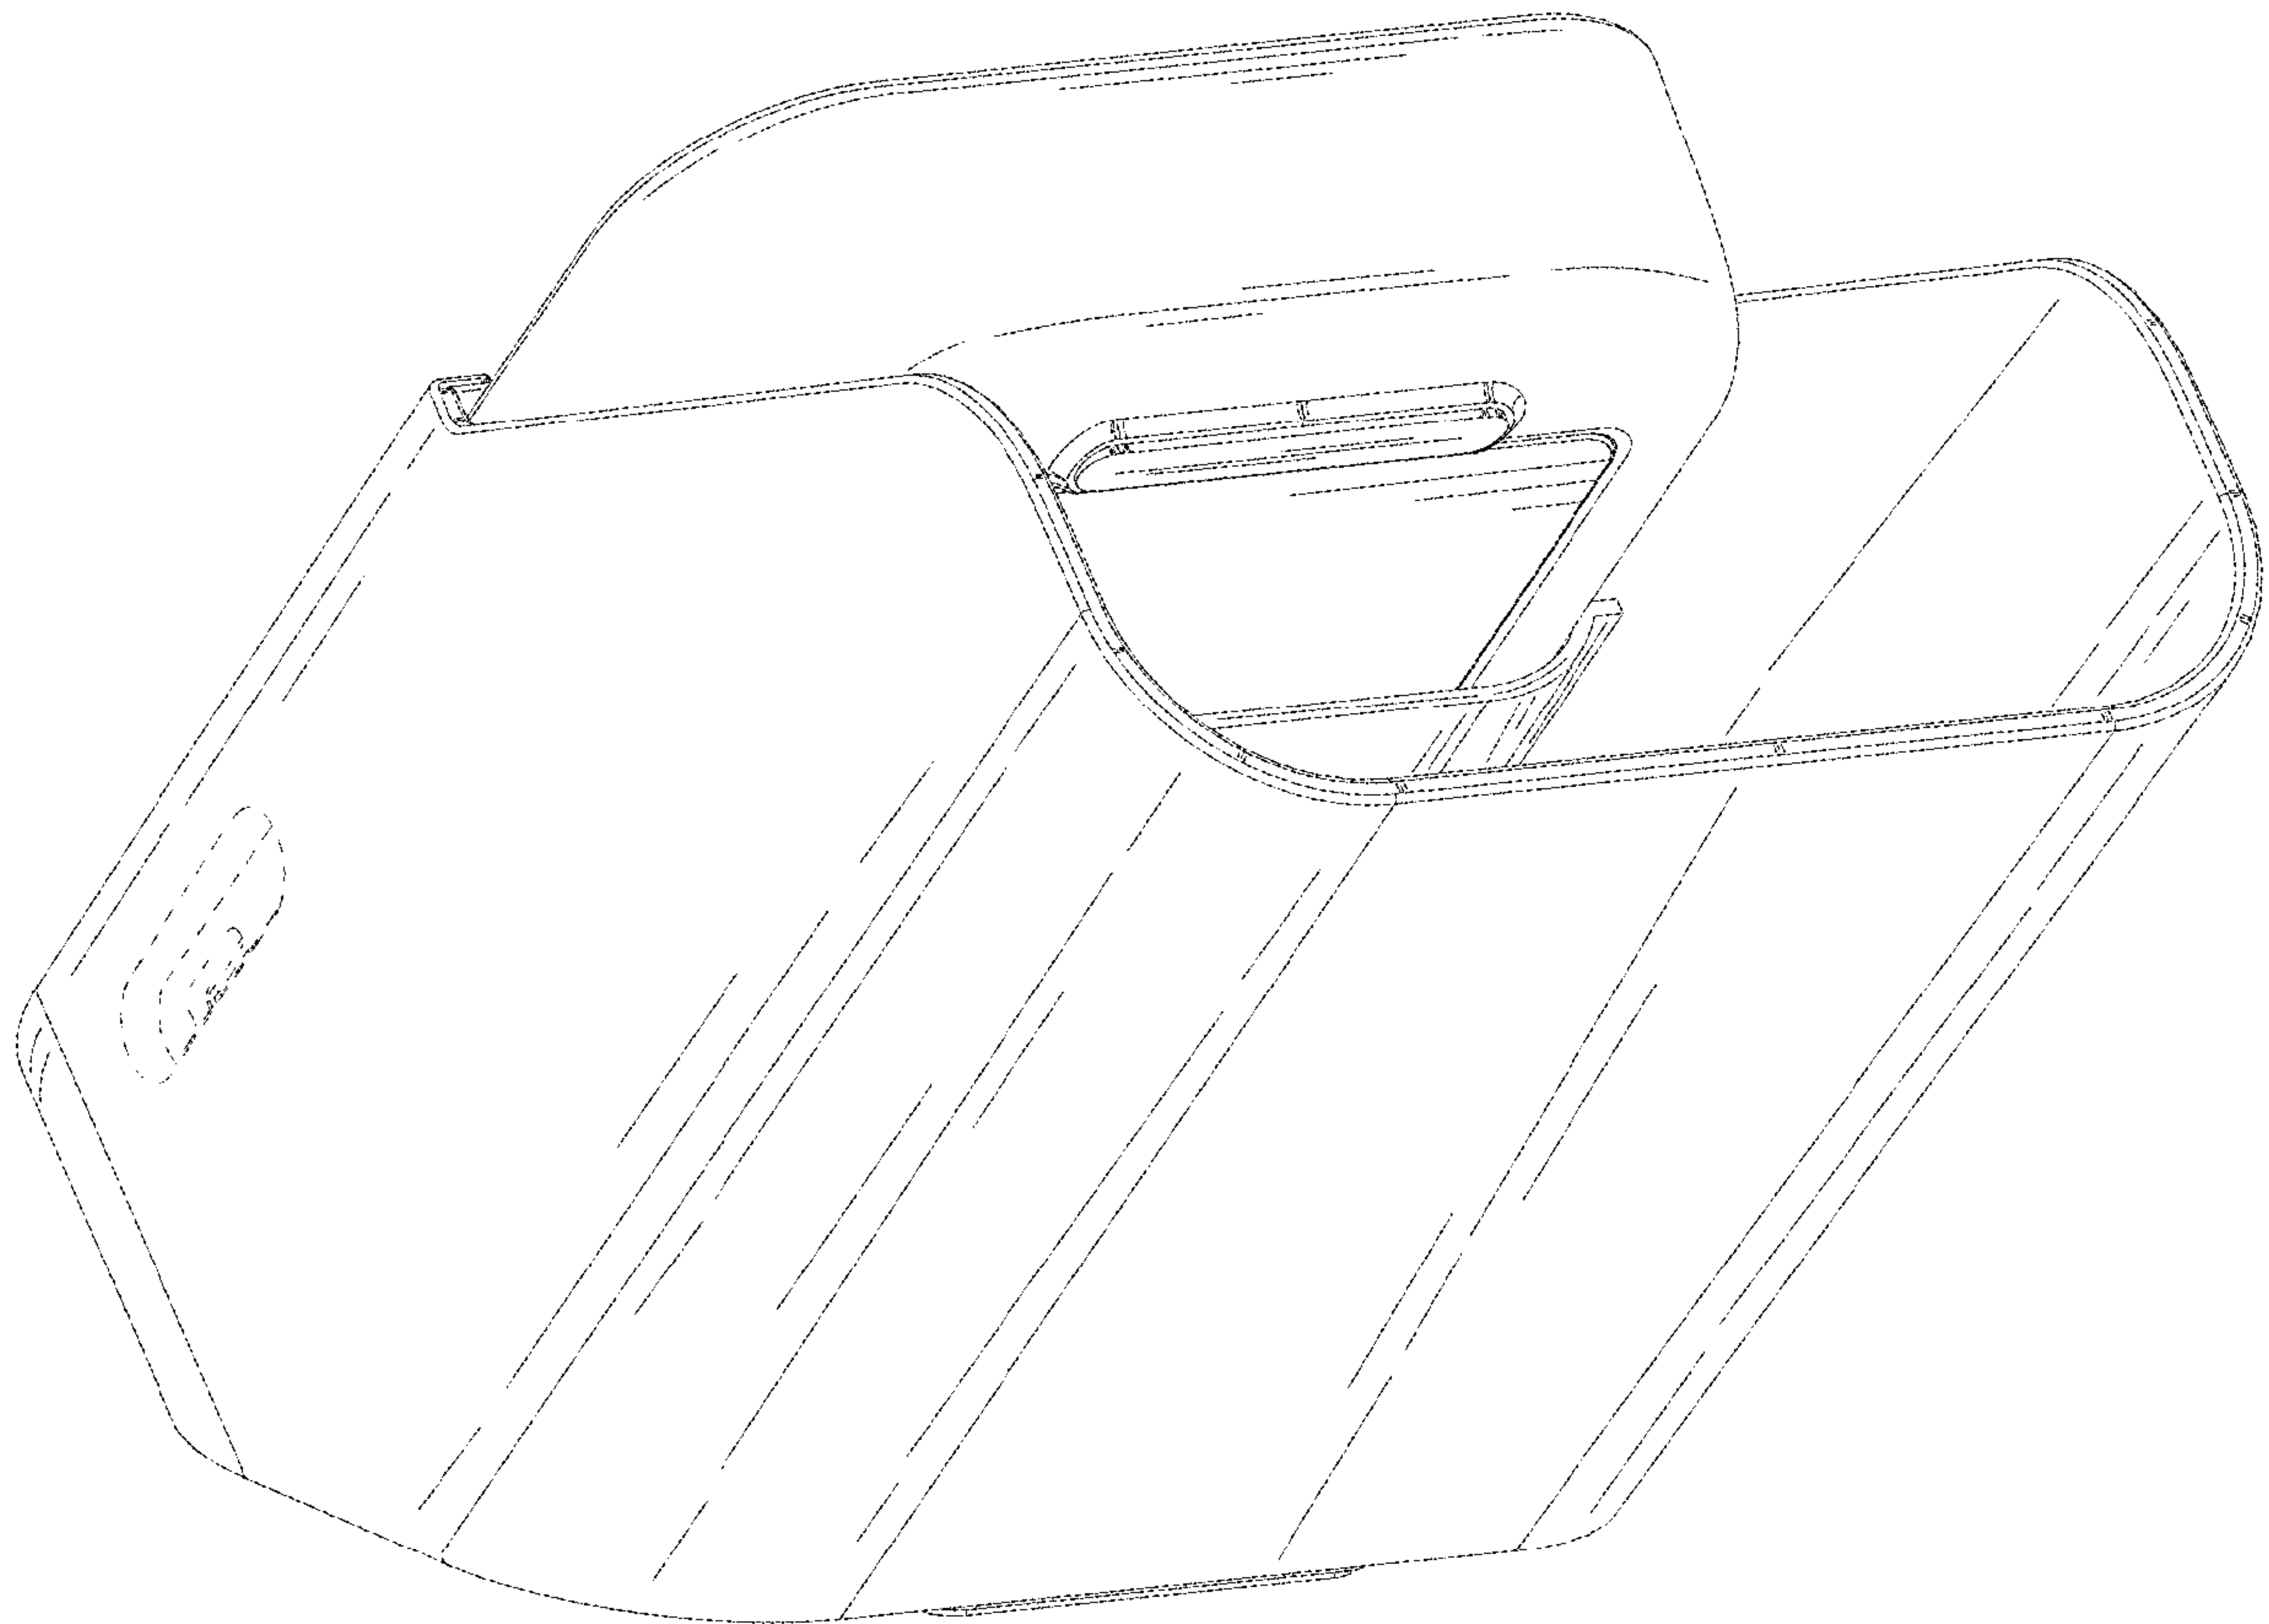


FIG. 3

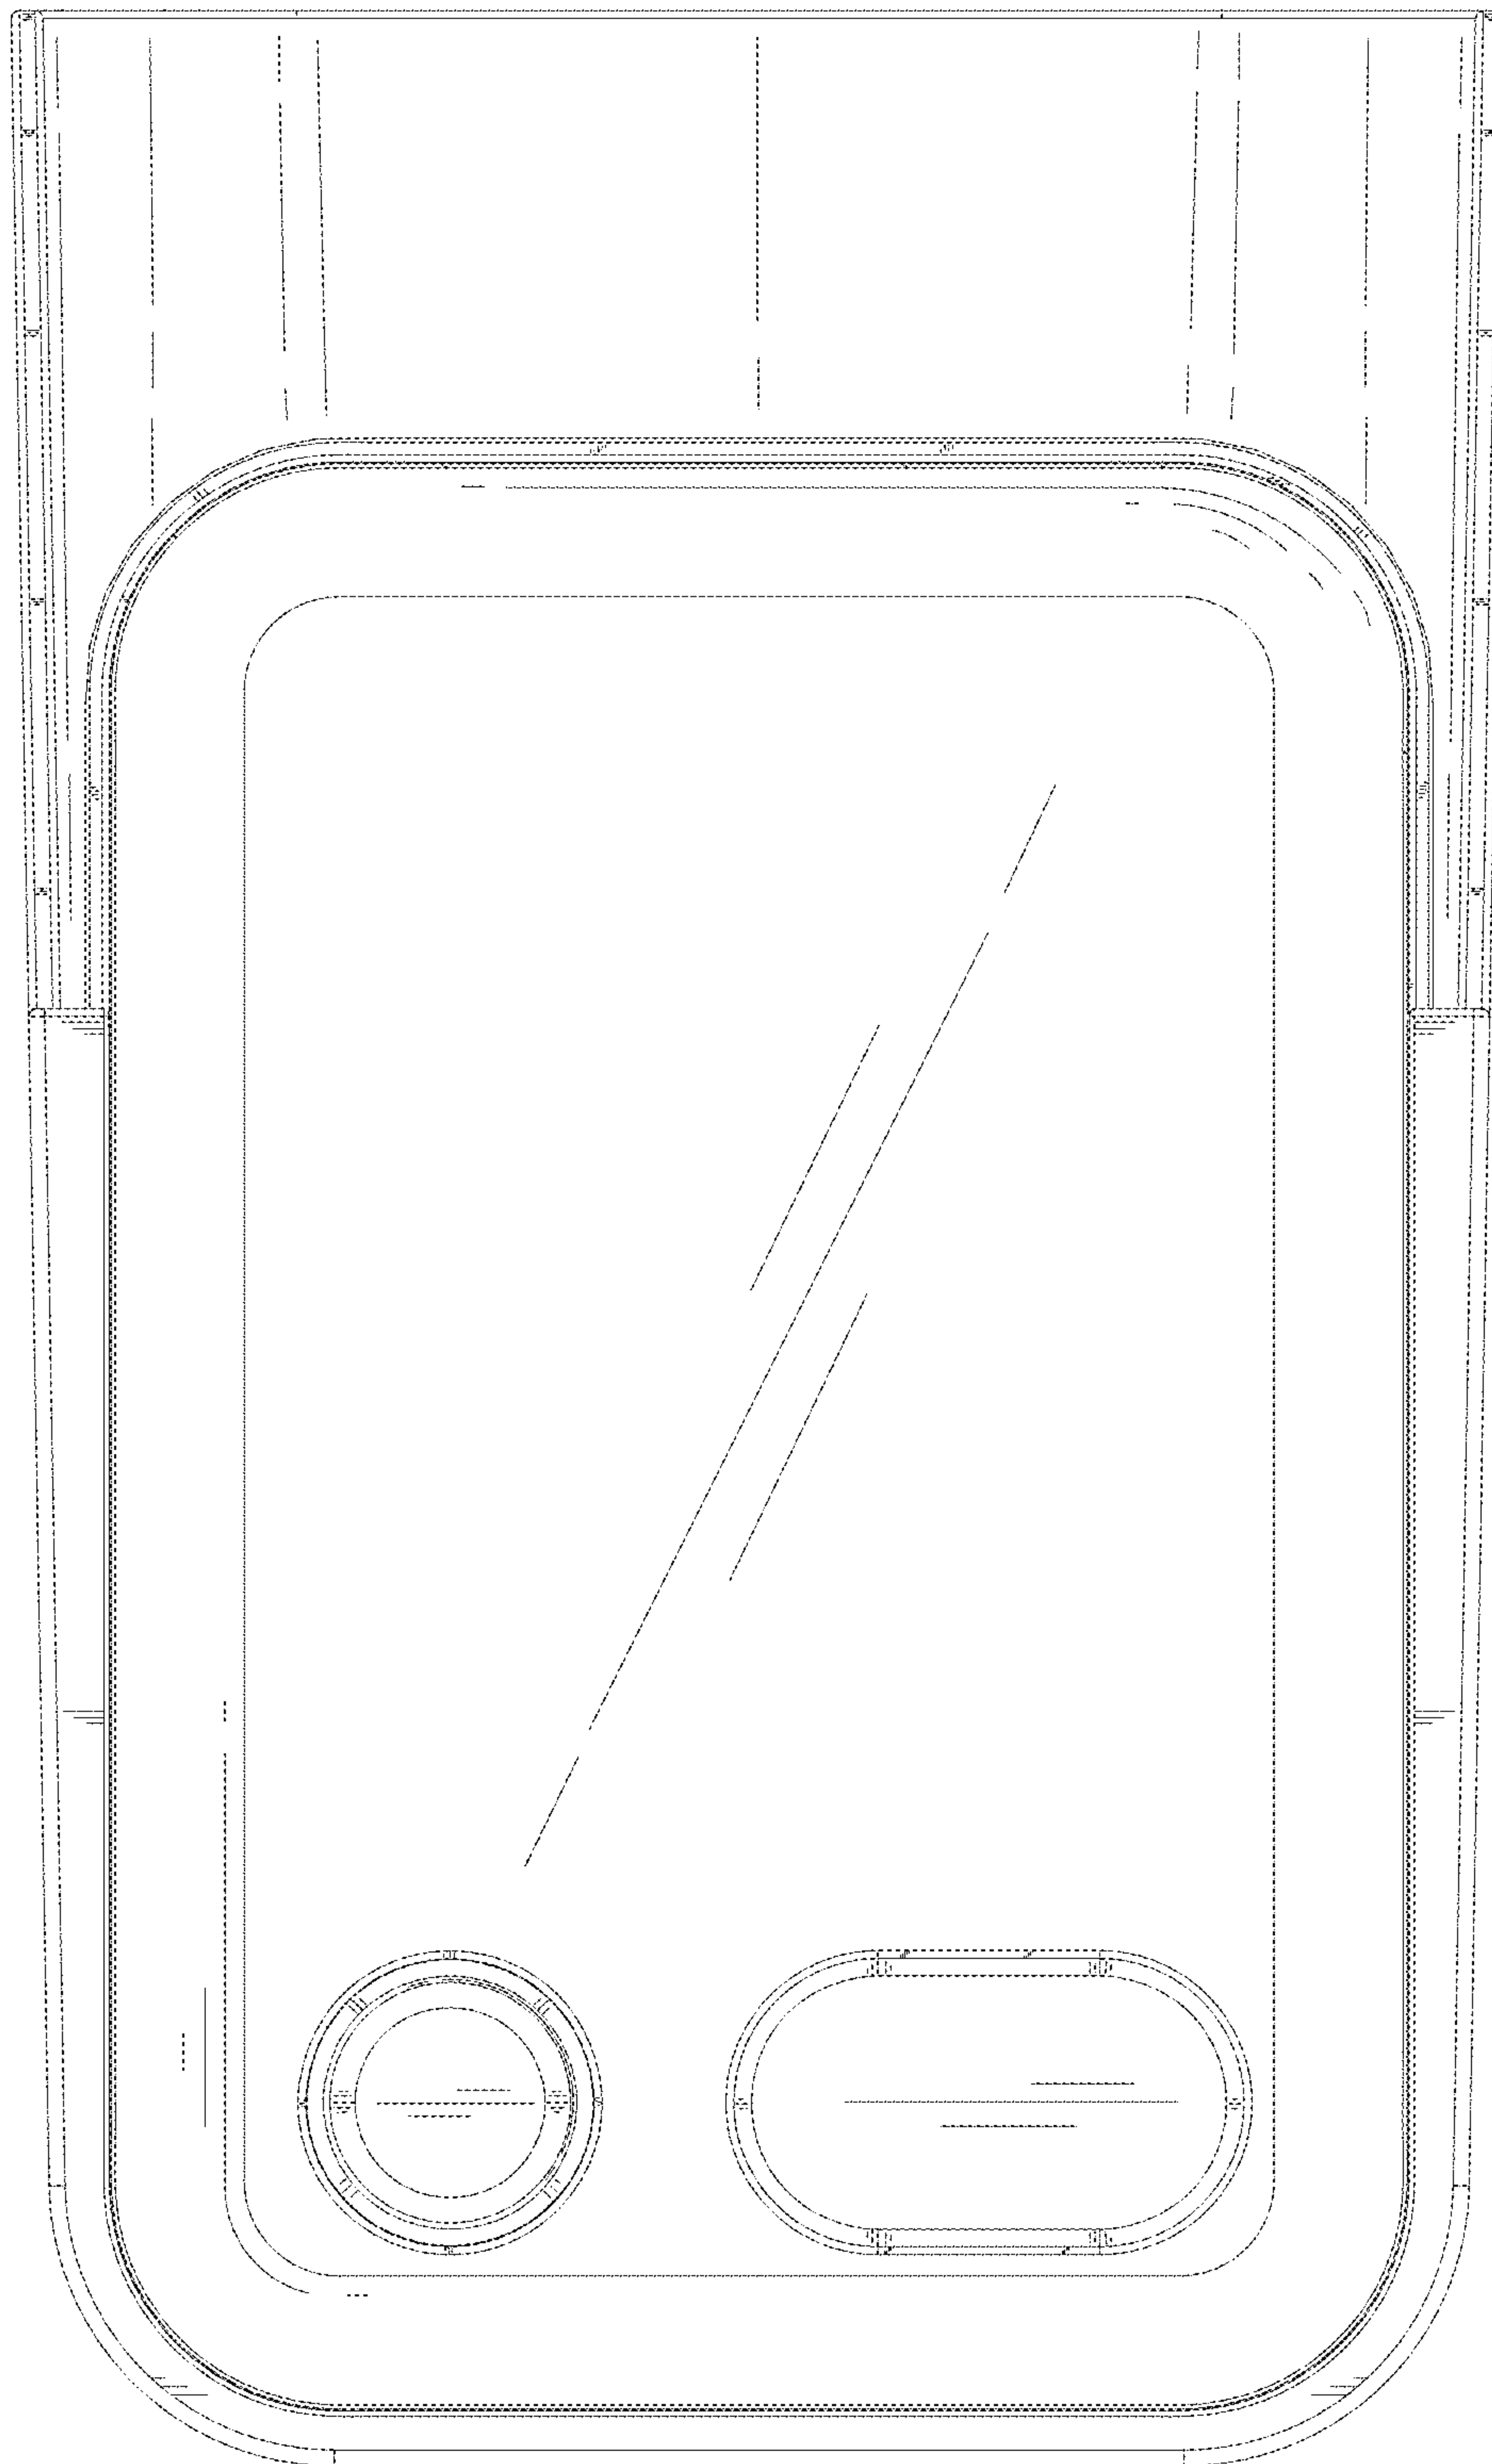


FIG. 4

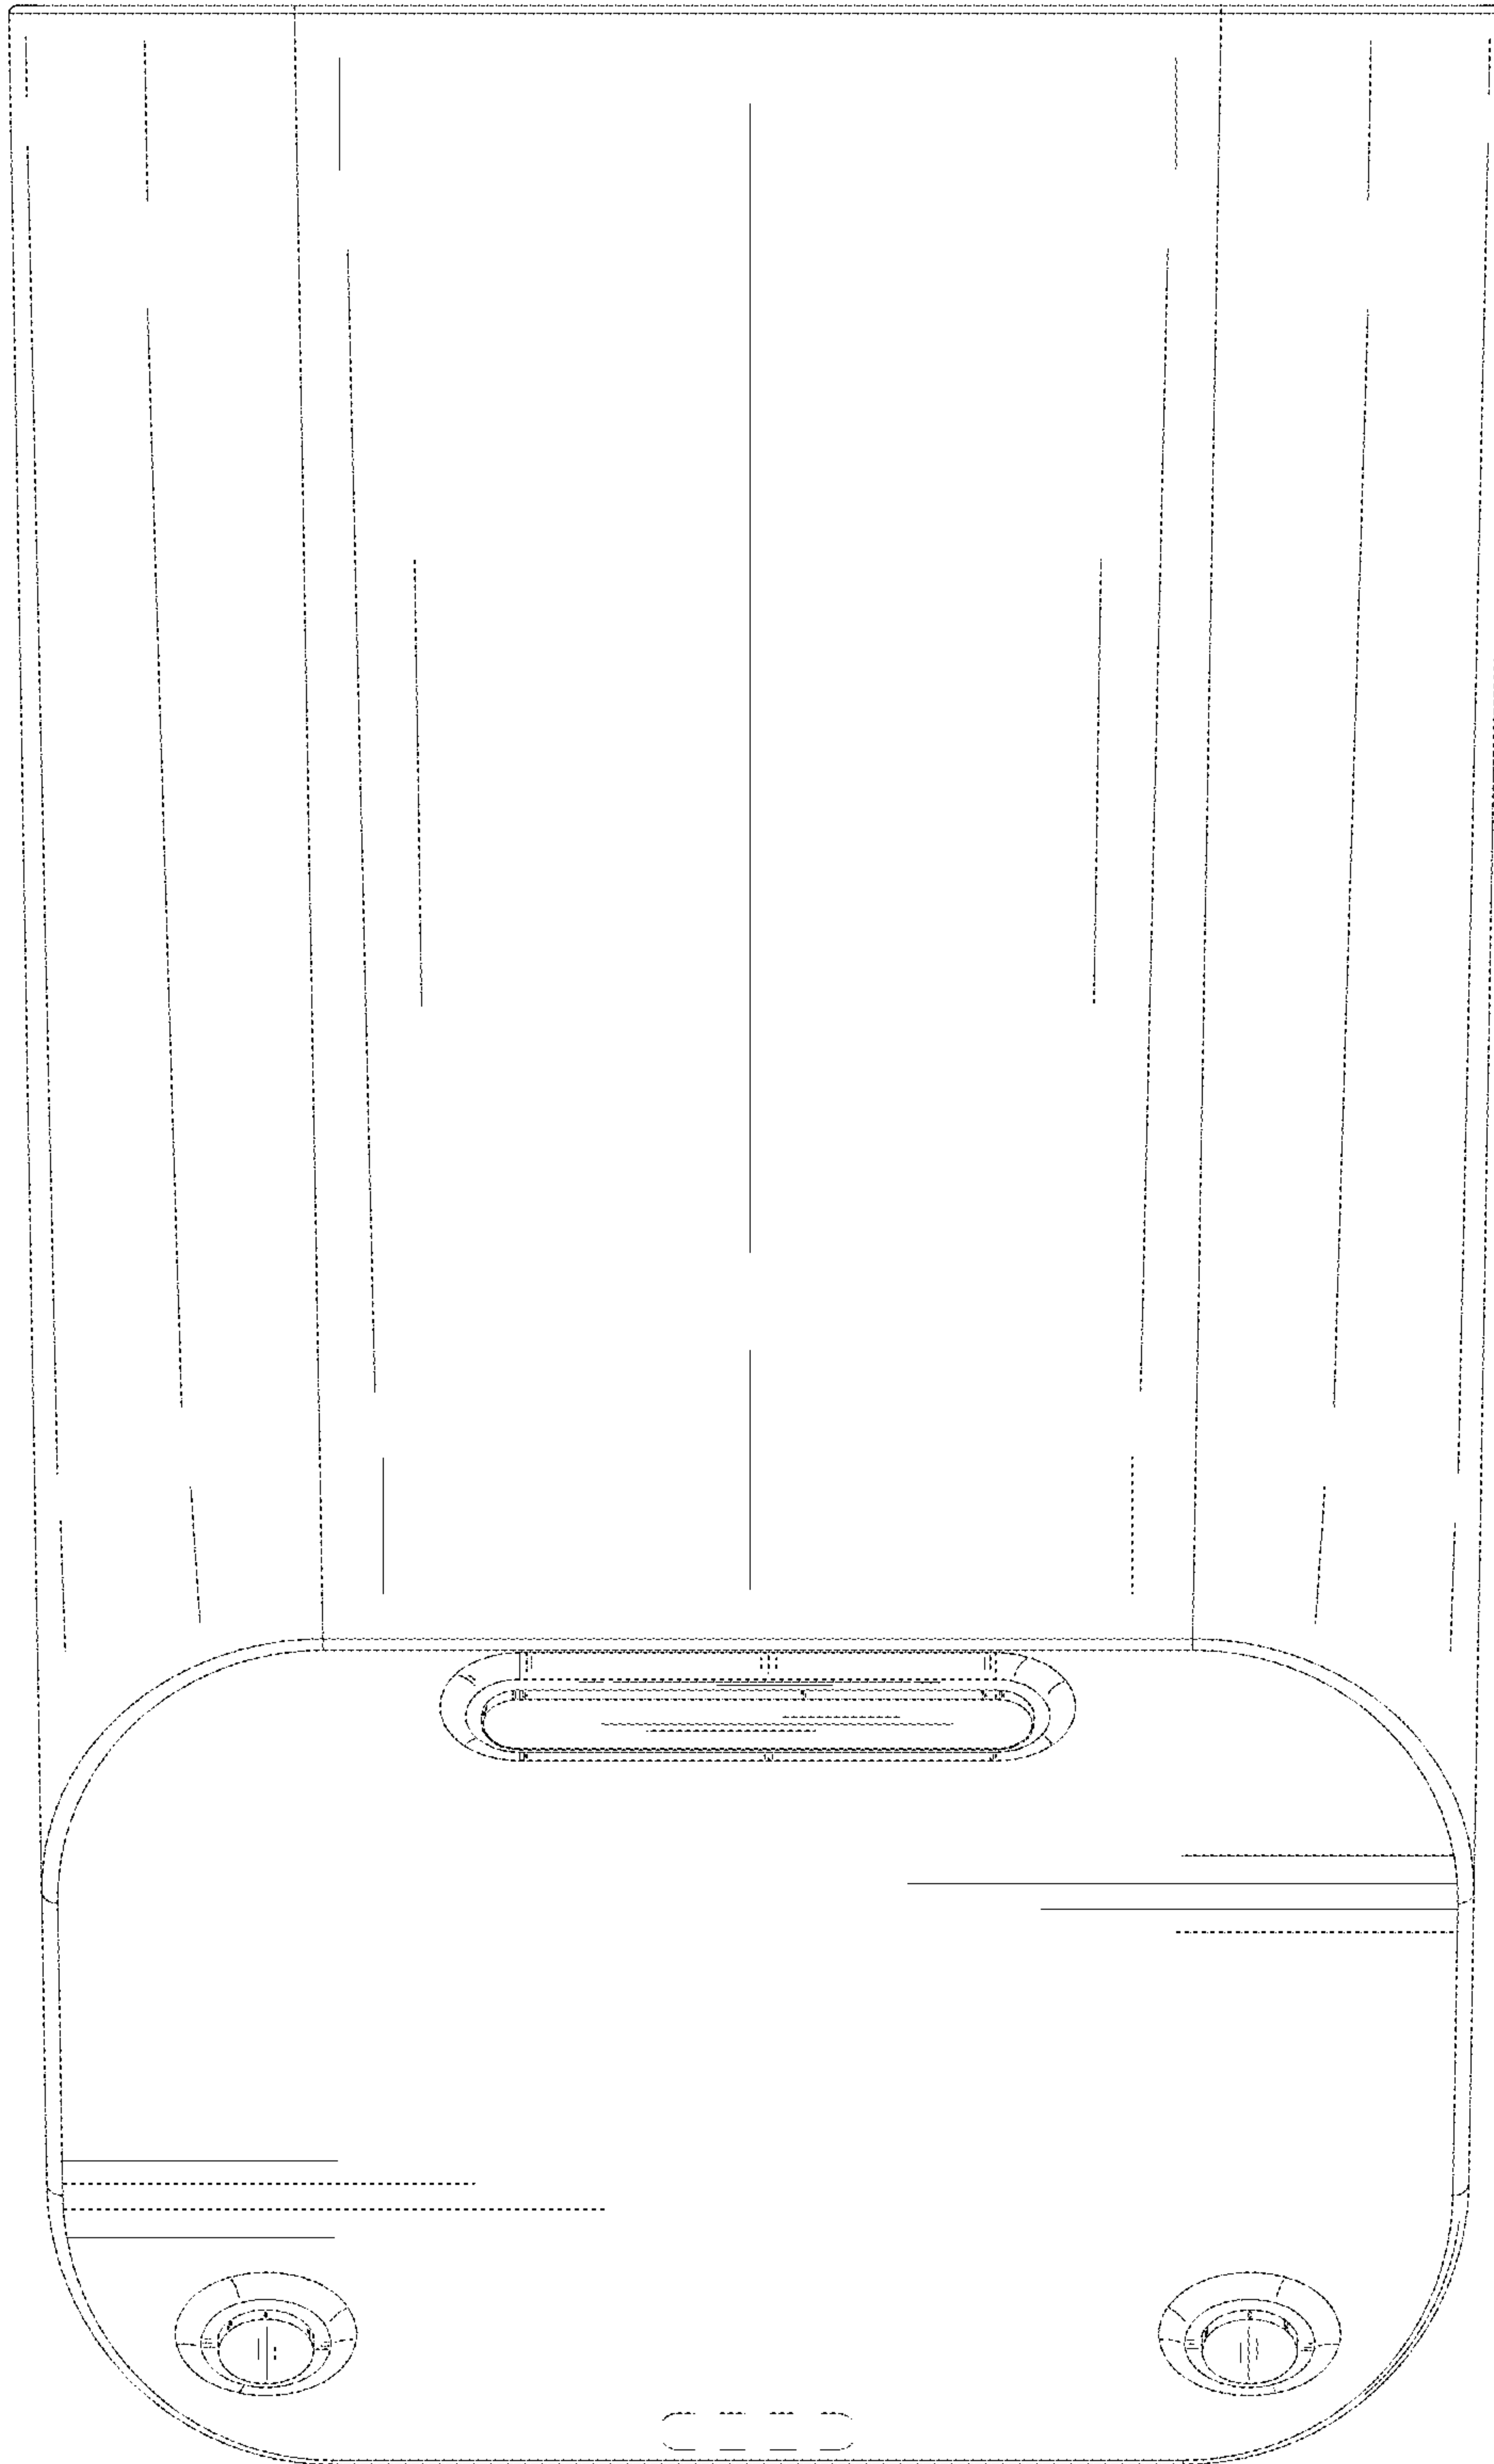


FIG. 5

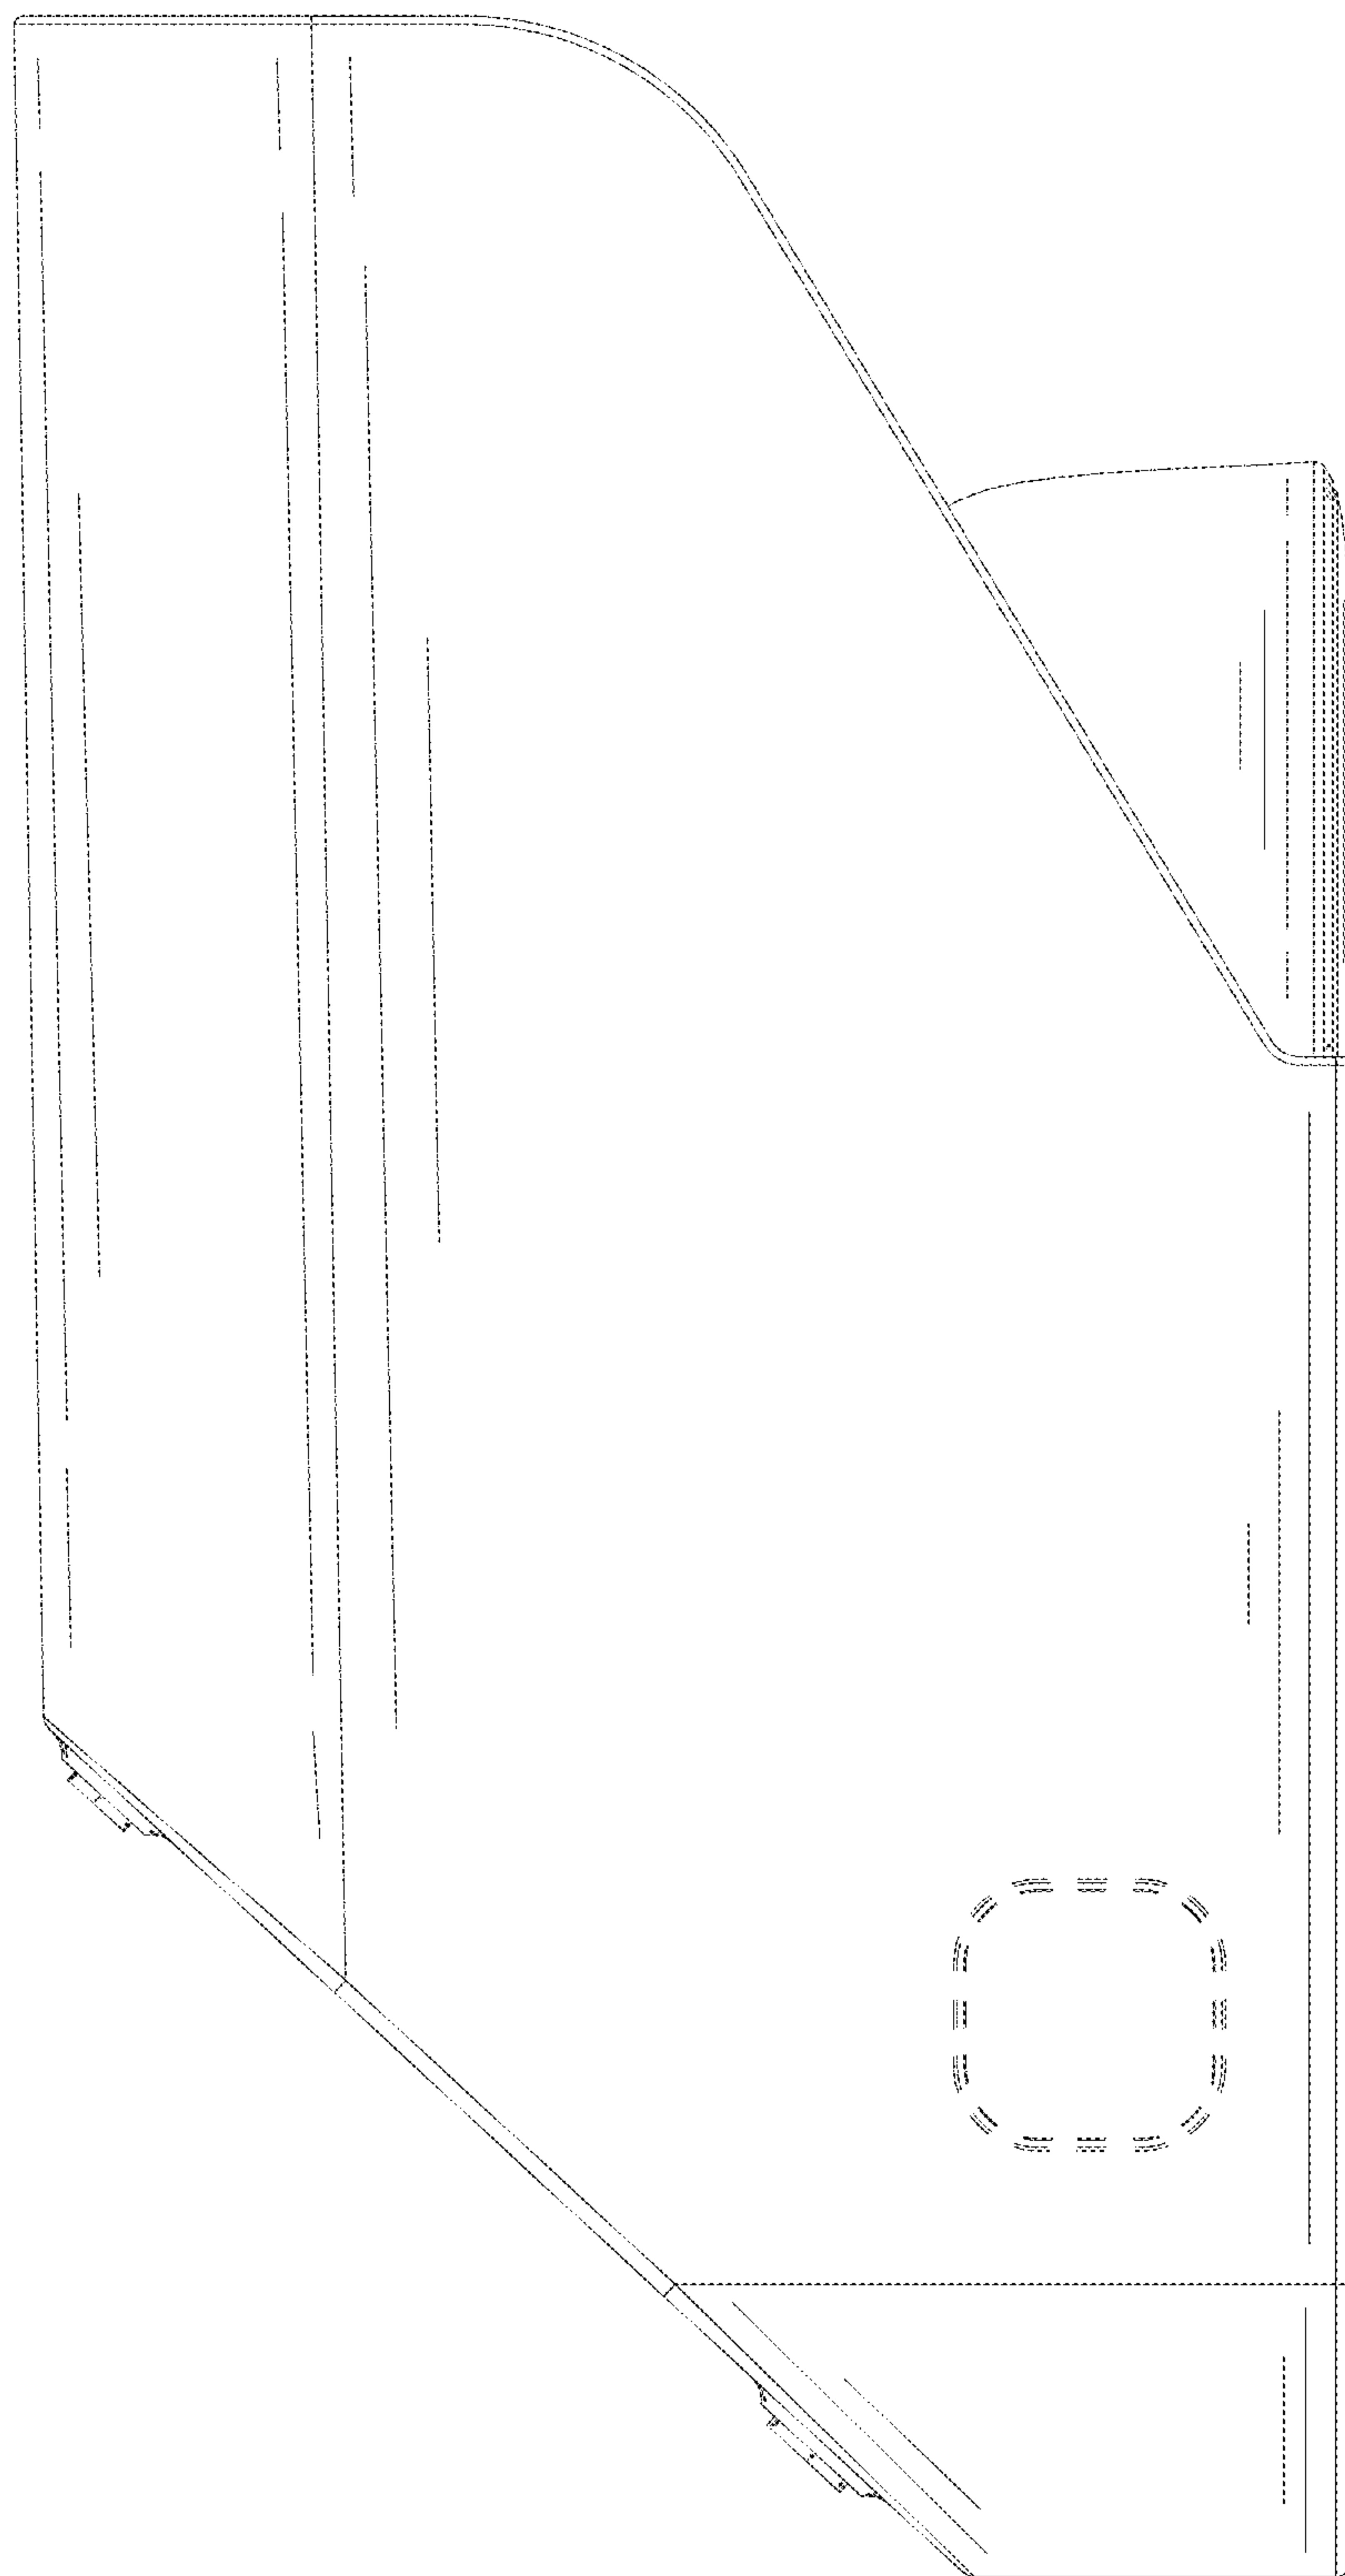


FIG. 6

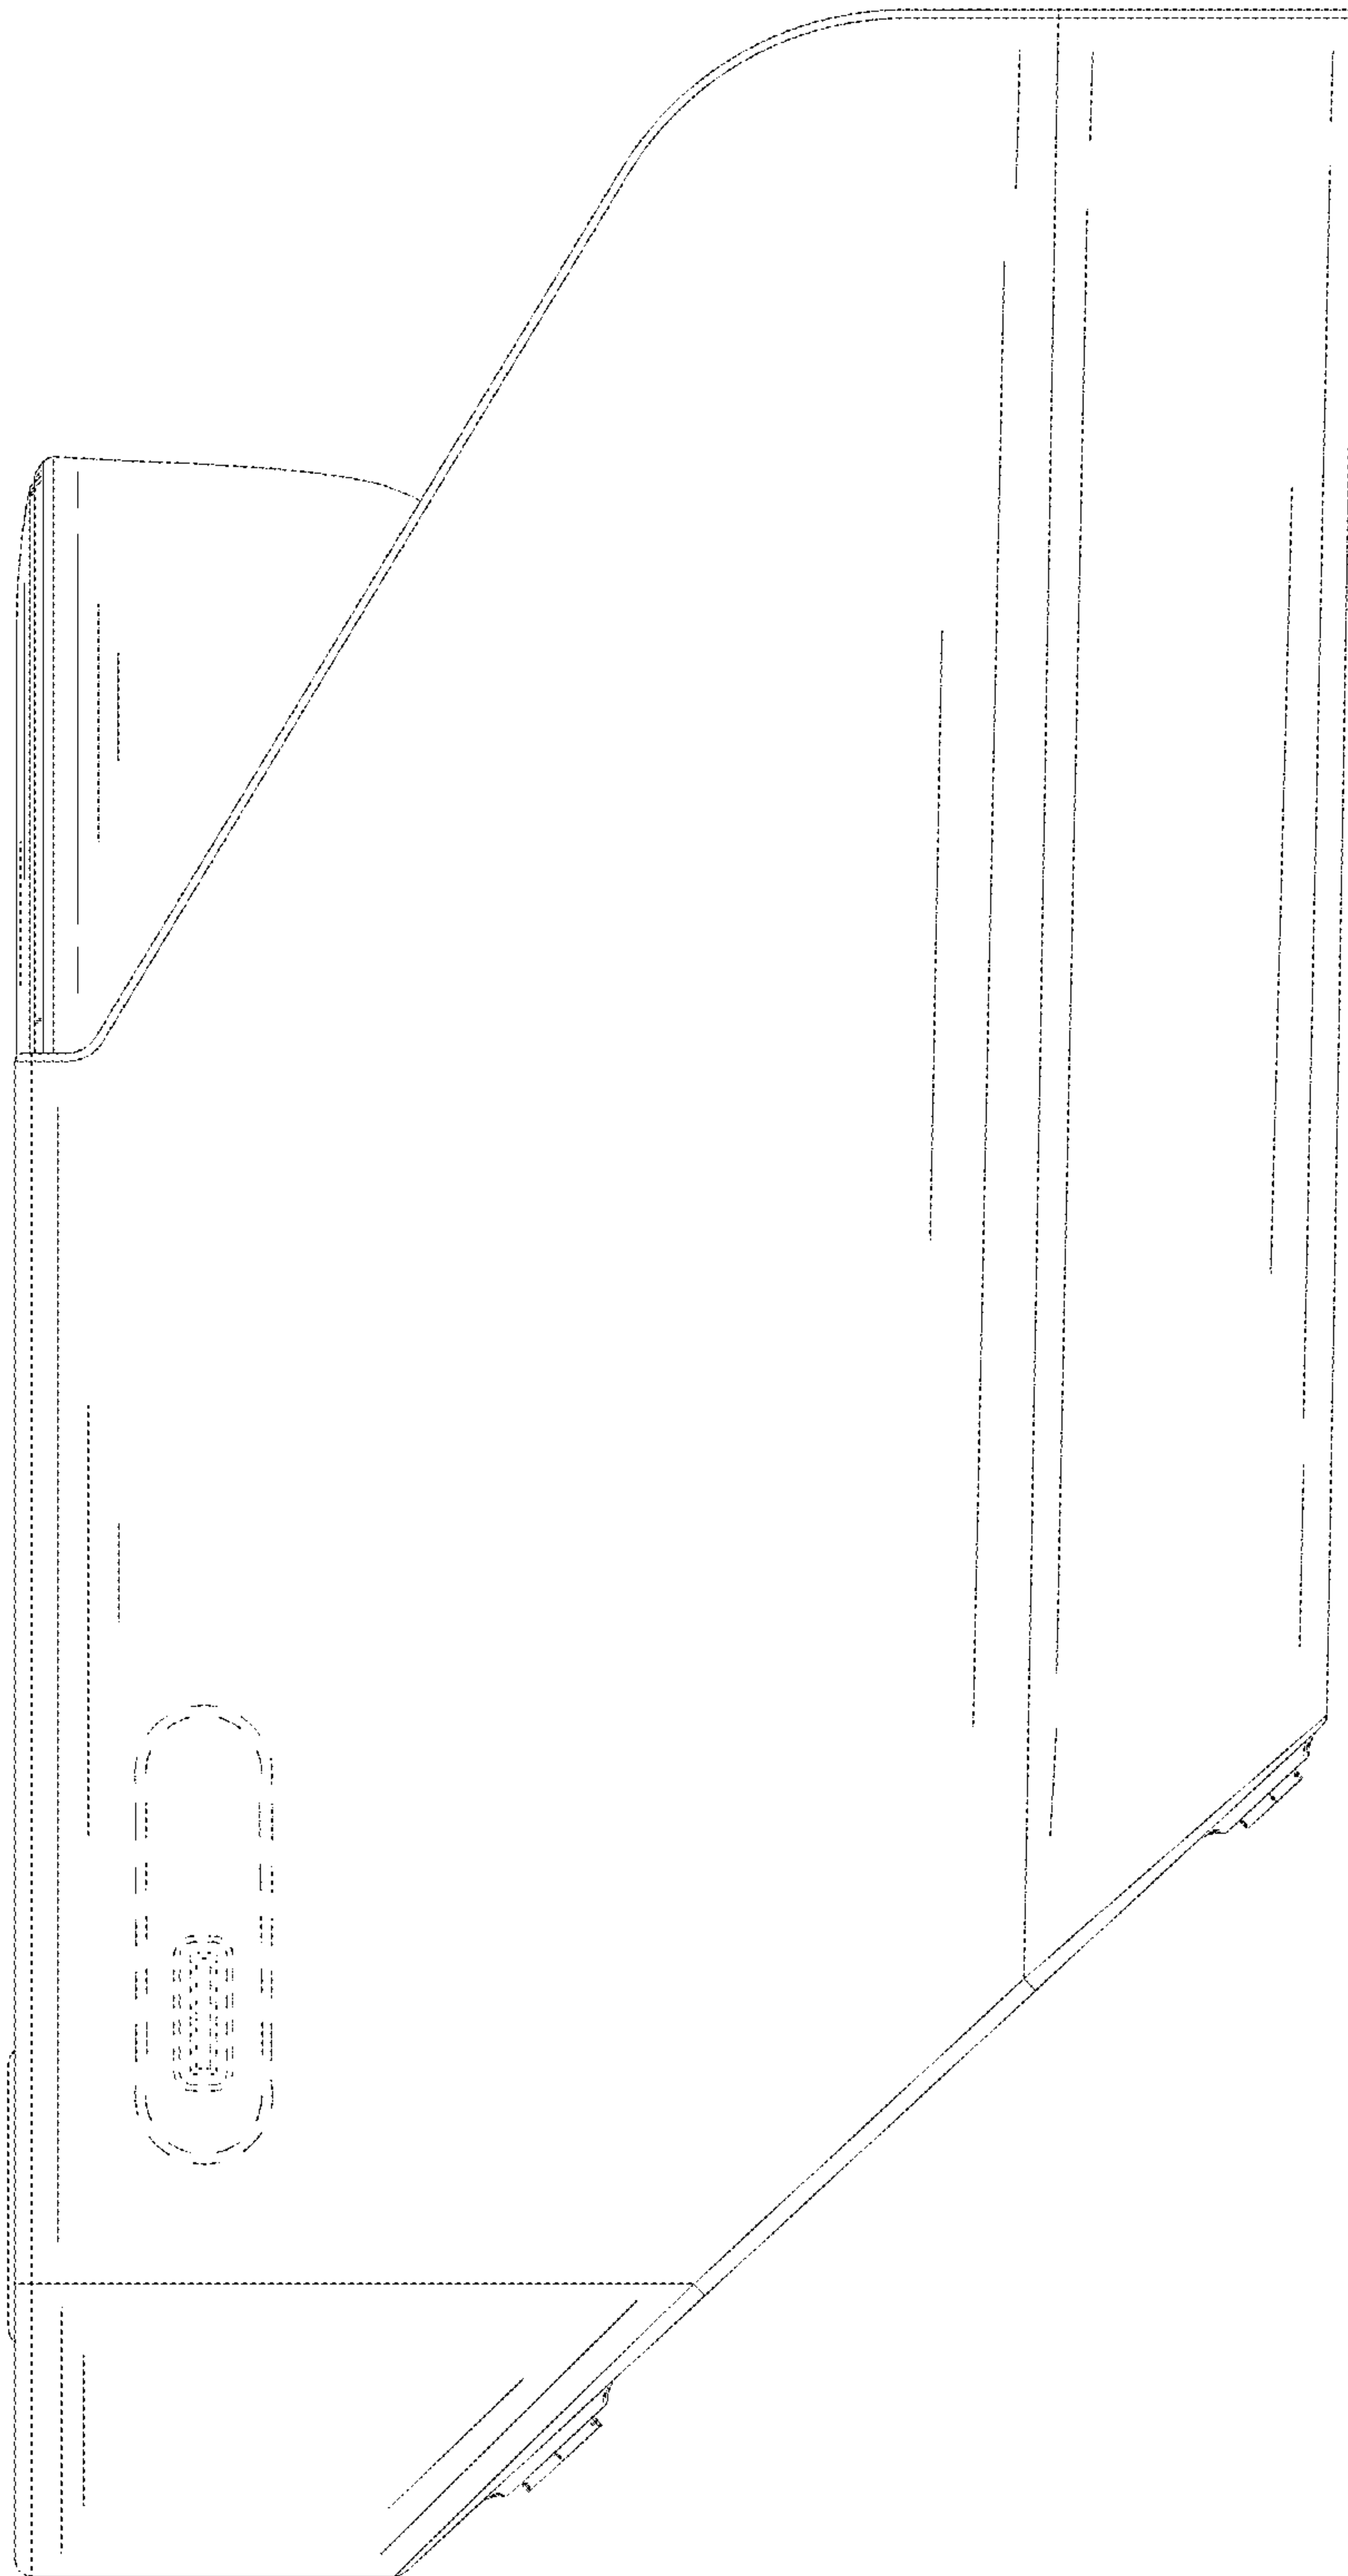


FIG. 7

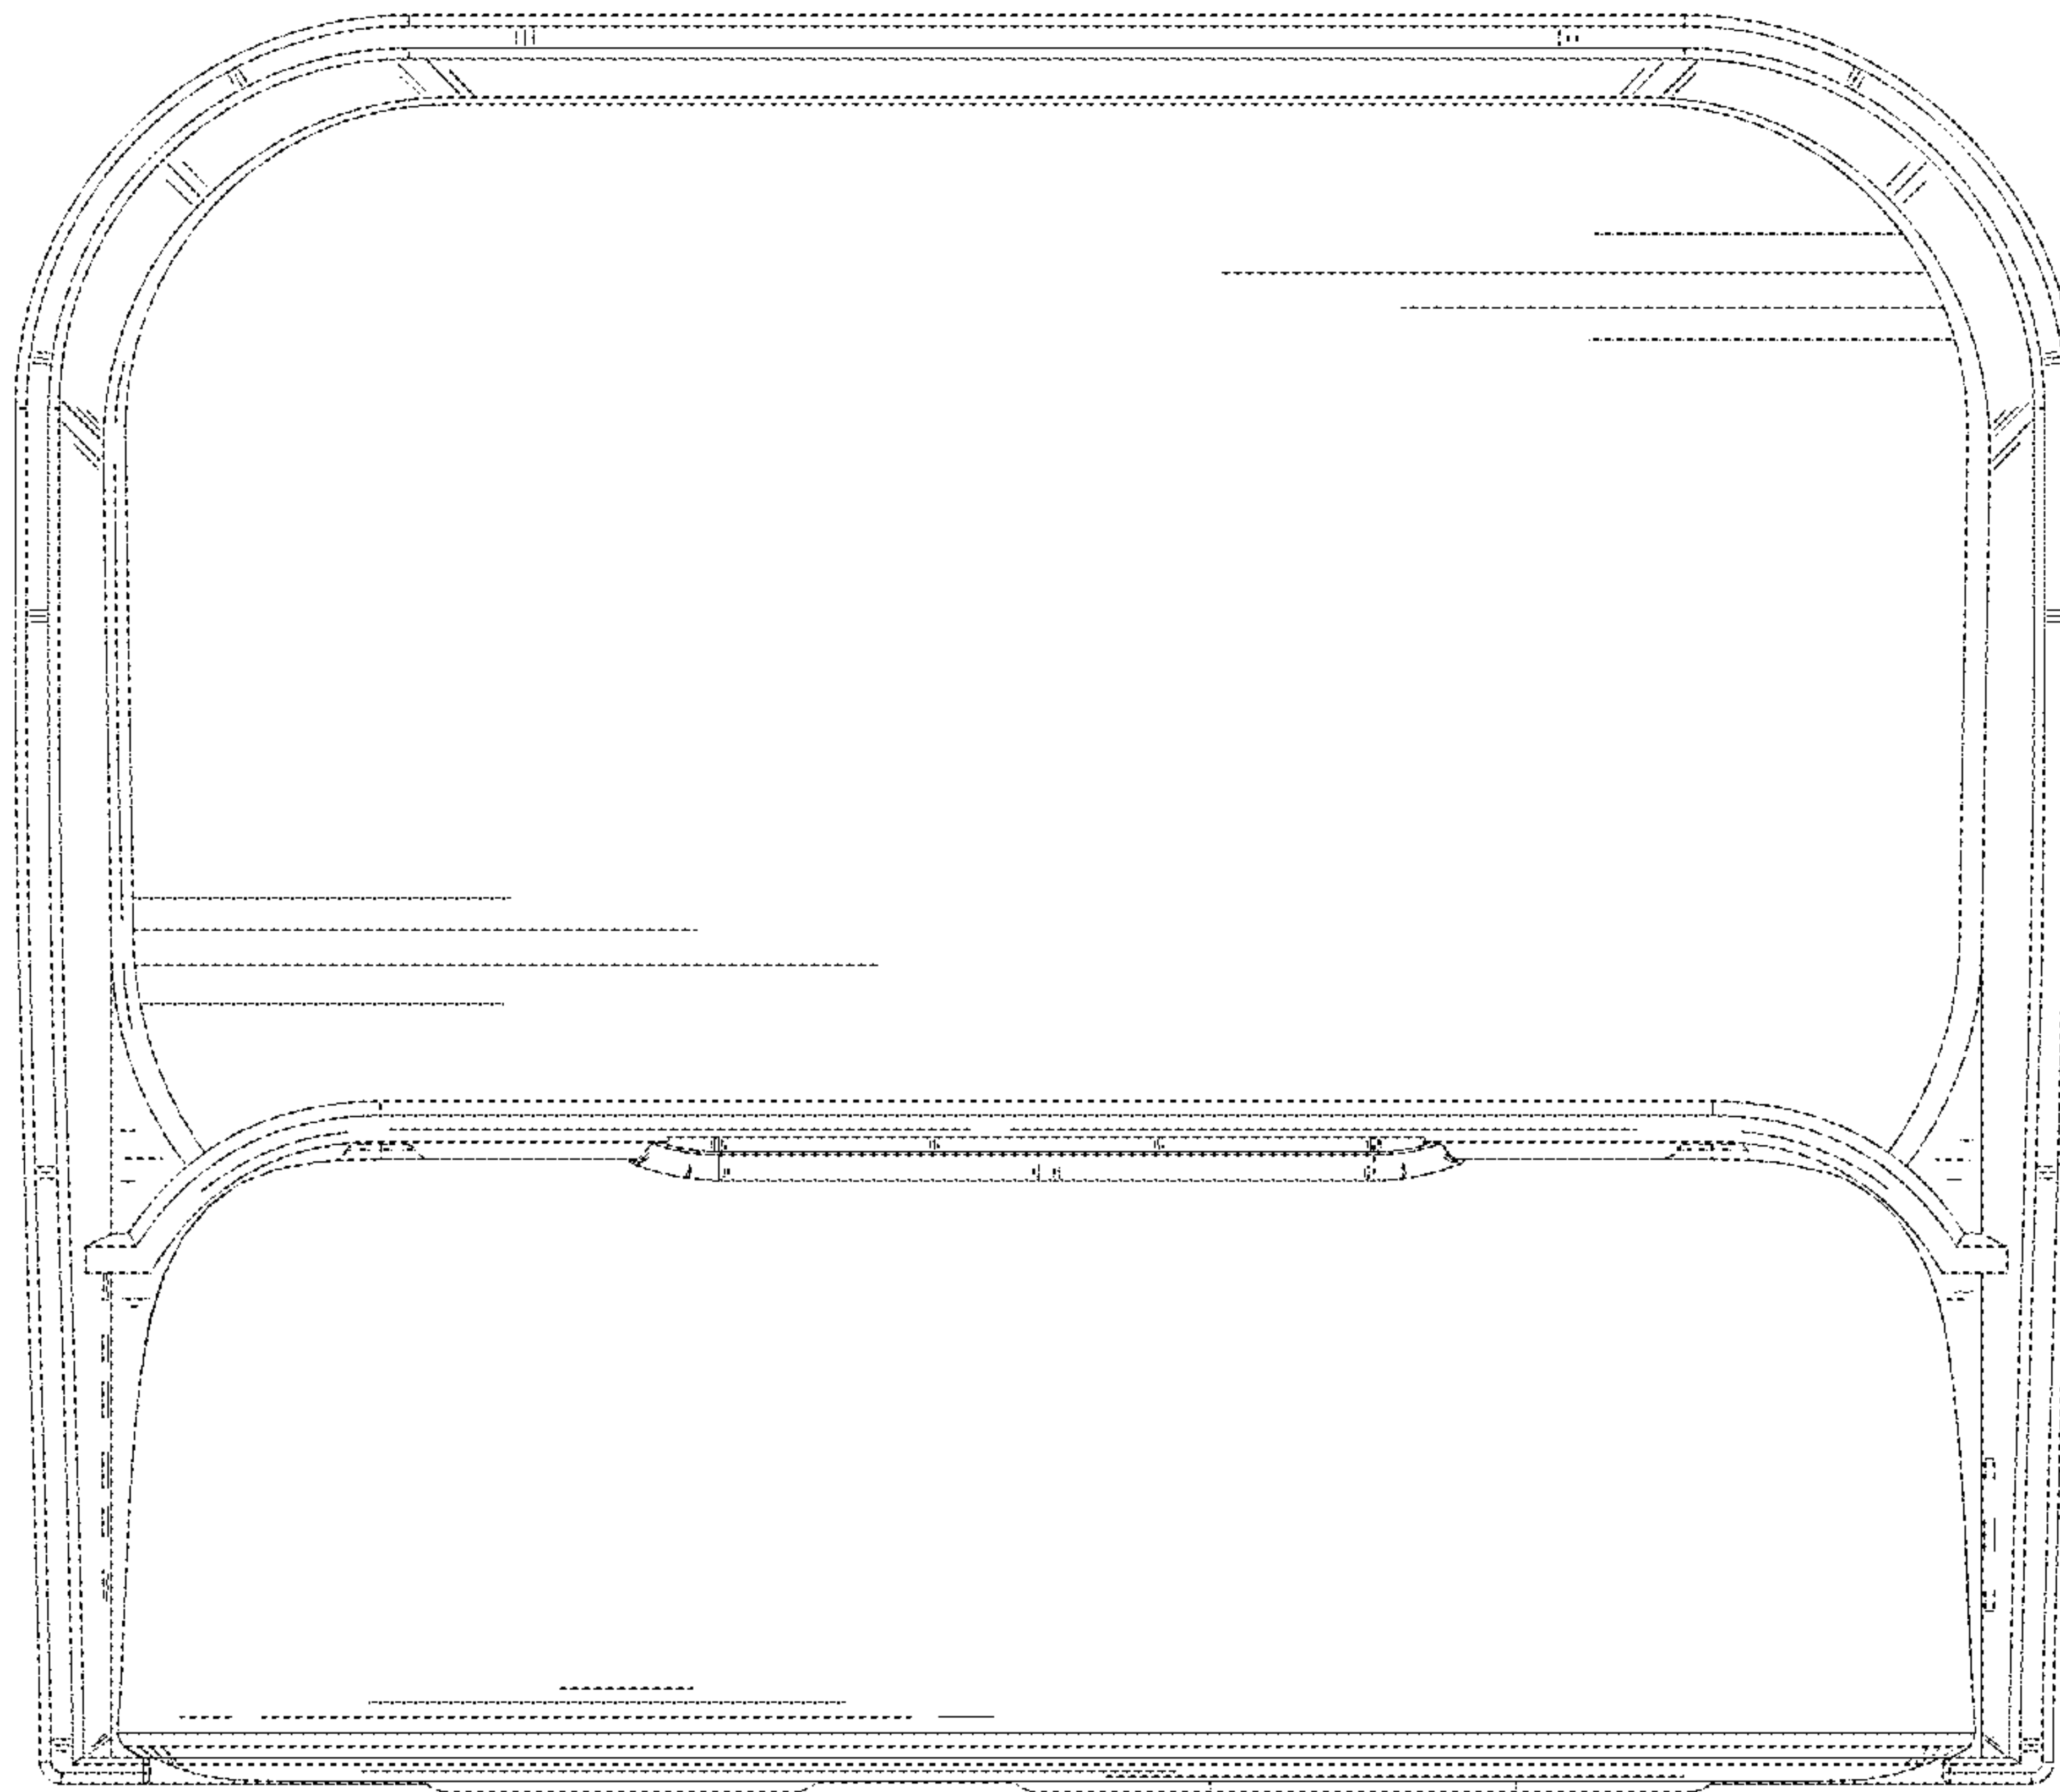


FIG. 8

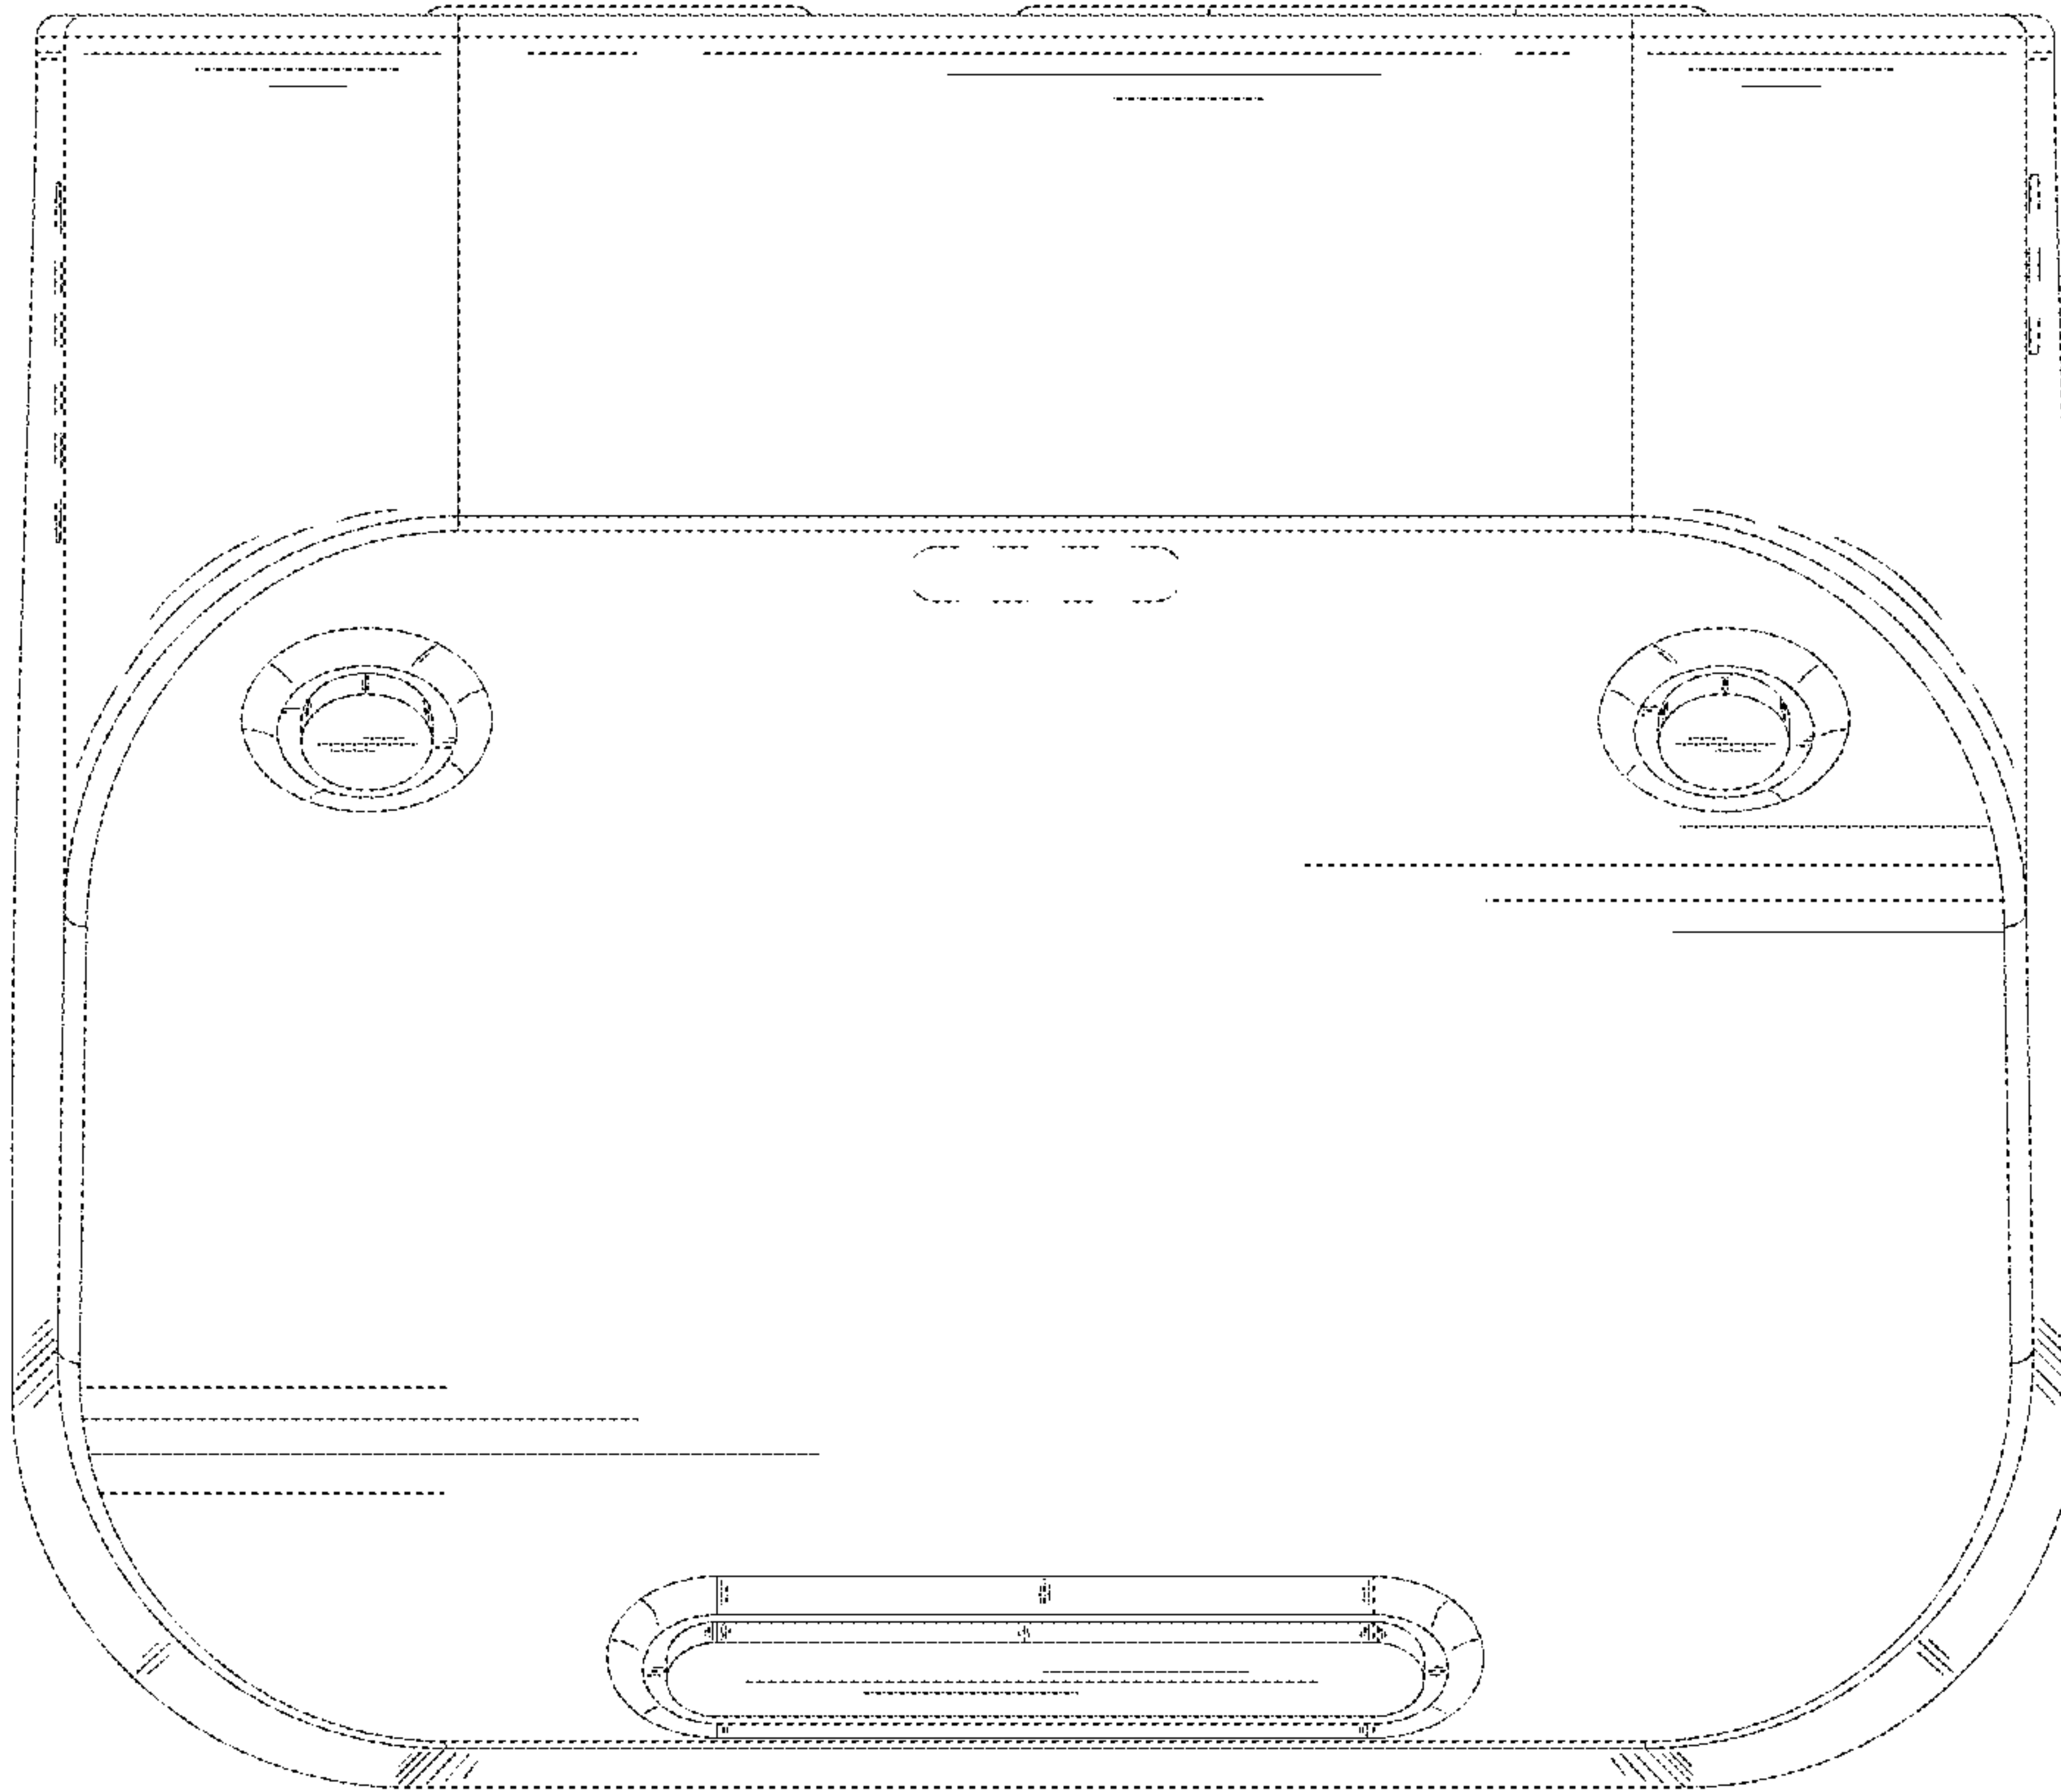


FIG. 9