



US00D961774S

(12) **United States Design Patent** (10) **Patent No.:** **US D961,774 S**
Sekine et al. (45) **Date of Patent:** **** Aug. 23, 2022**

(54) **SCANNER FOR AN X-RAY TOMOGRAPHY DIAGNOSIS APPARATUS**

(71) Applicant: **Canon Medical Systems Corporation**,
Otawara (JP)

(72) Inventors: **Tetsuya Sekine**, Kawasaki Kanagawa
(JP); **Koichiro Oishi**, Wako Saitama
(JP)

(73) Assignee: **Canon Medical Systems Corporation**,
Otawara (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/758,284**

(22) Filed: **Nov. 13, 2020**

(51) **LOC (13) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158**

(58) **Field of Classification Search**
USPC D24/107, 158-161, 185, 186
CPC .. A61B 6/03; A61B 6/035; A61B 5/05; A61B
5/055

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D628,294 S * 11/2010 Baba D24/158
D701,311 S * 3/2014 Ohmukai D24/158

D701,312 S * 3/2014 Ohmukai D24/158
D715,944 S * 10/2014 Yao D24/159
D725,275 S * 3/2015 Matsumura D24/158
D753,828 S * 4/2016 Baba D24/158
D770,624 S * 11/2016 Yao D24/158
D783,830 S * 4/2017 Baba D24/158
D927,691 S * 8/2021 Ooshima D24/158
2017/0105692 A1* 4/2017 Sawanobori A61B 6/035

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson,
Farabow, Garrett & Dunner, L.L.P.

(57) **CLAIM**

The ornamental design for an scanner for an X-ray tomog-
raphy diagnosis apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a scanner for an X-ray
tomography diagnosis apparatus showing our new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a left-side elevational view thereof;
FIG. 5 is a right-side elevational view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.

1 Claim, 7 Drawing Sheets

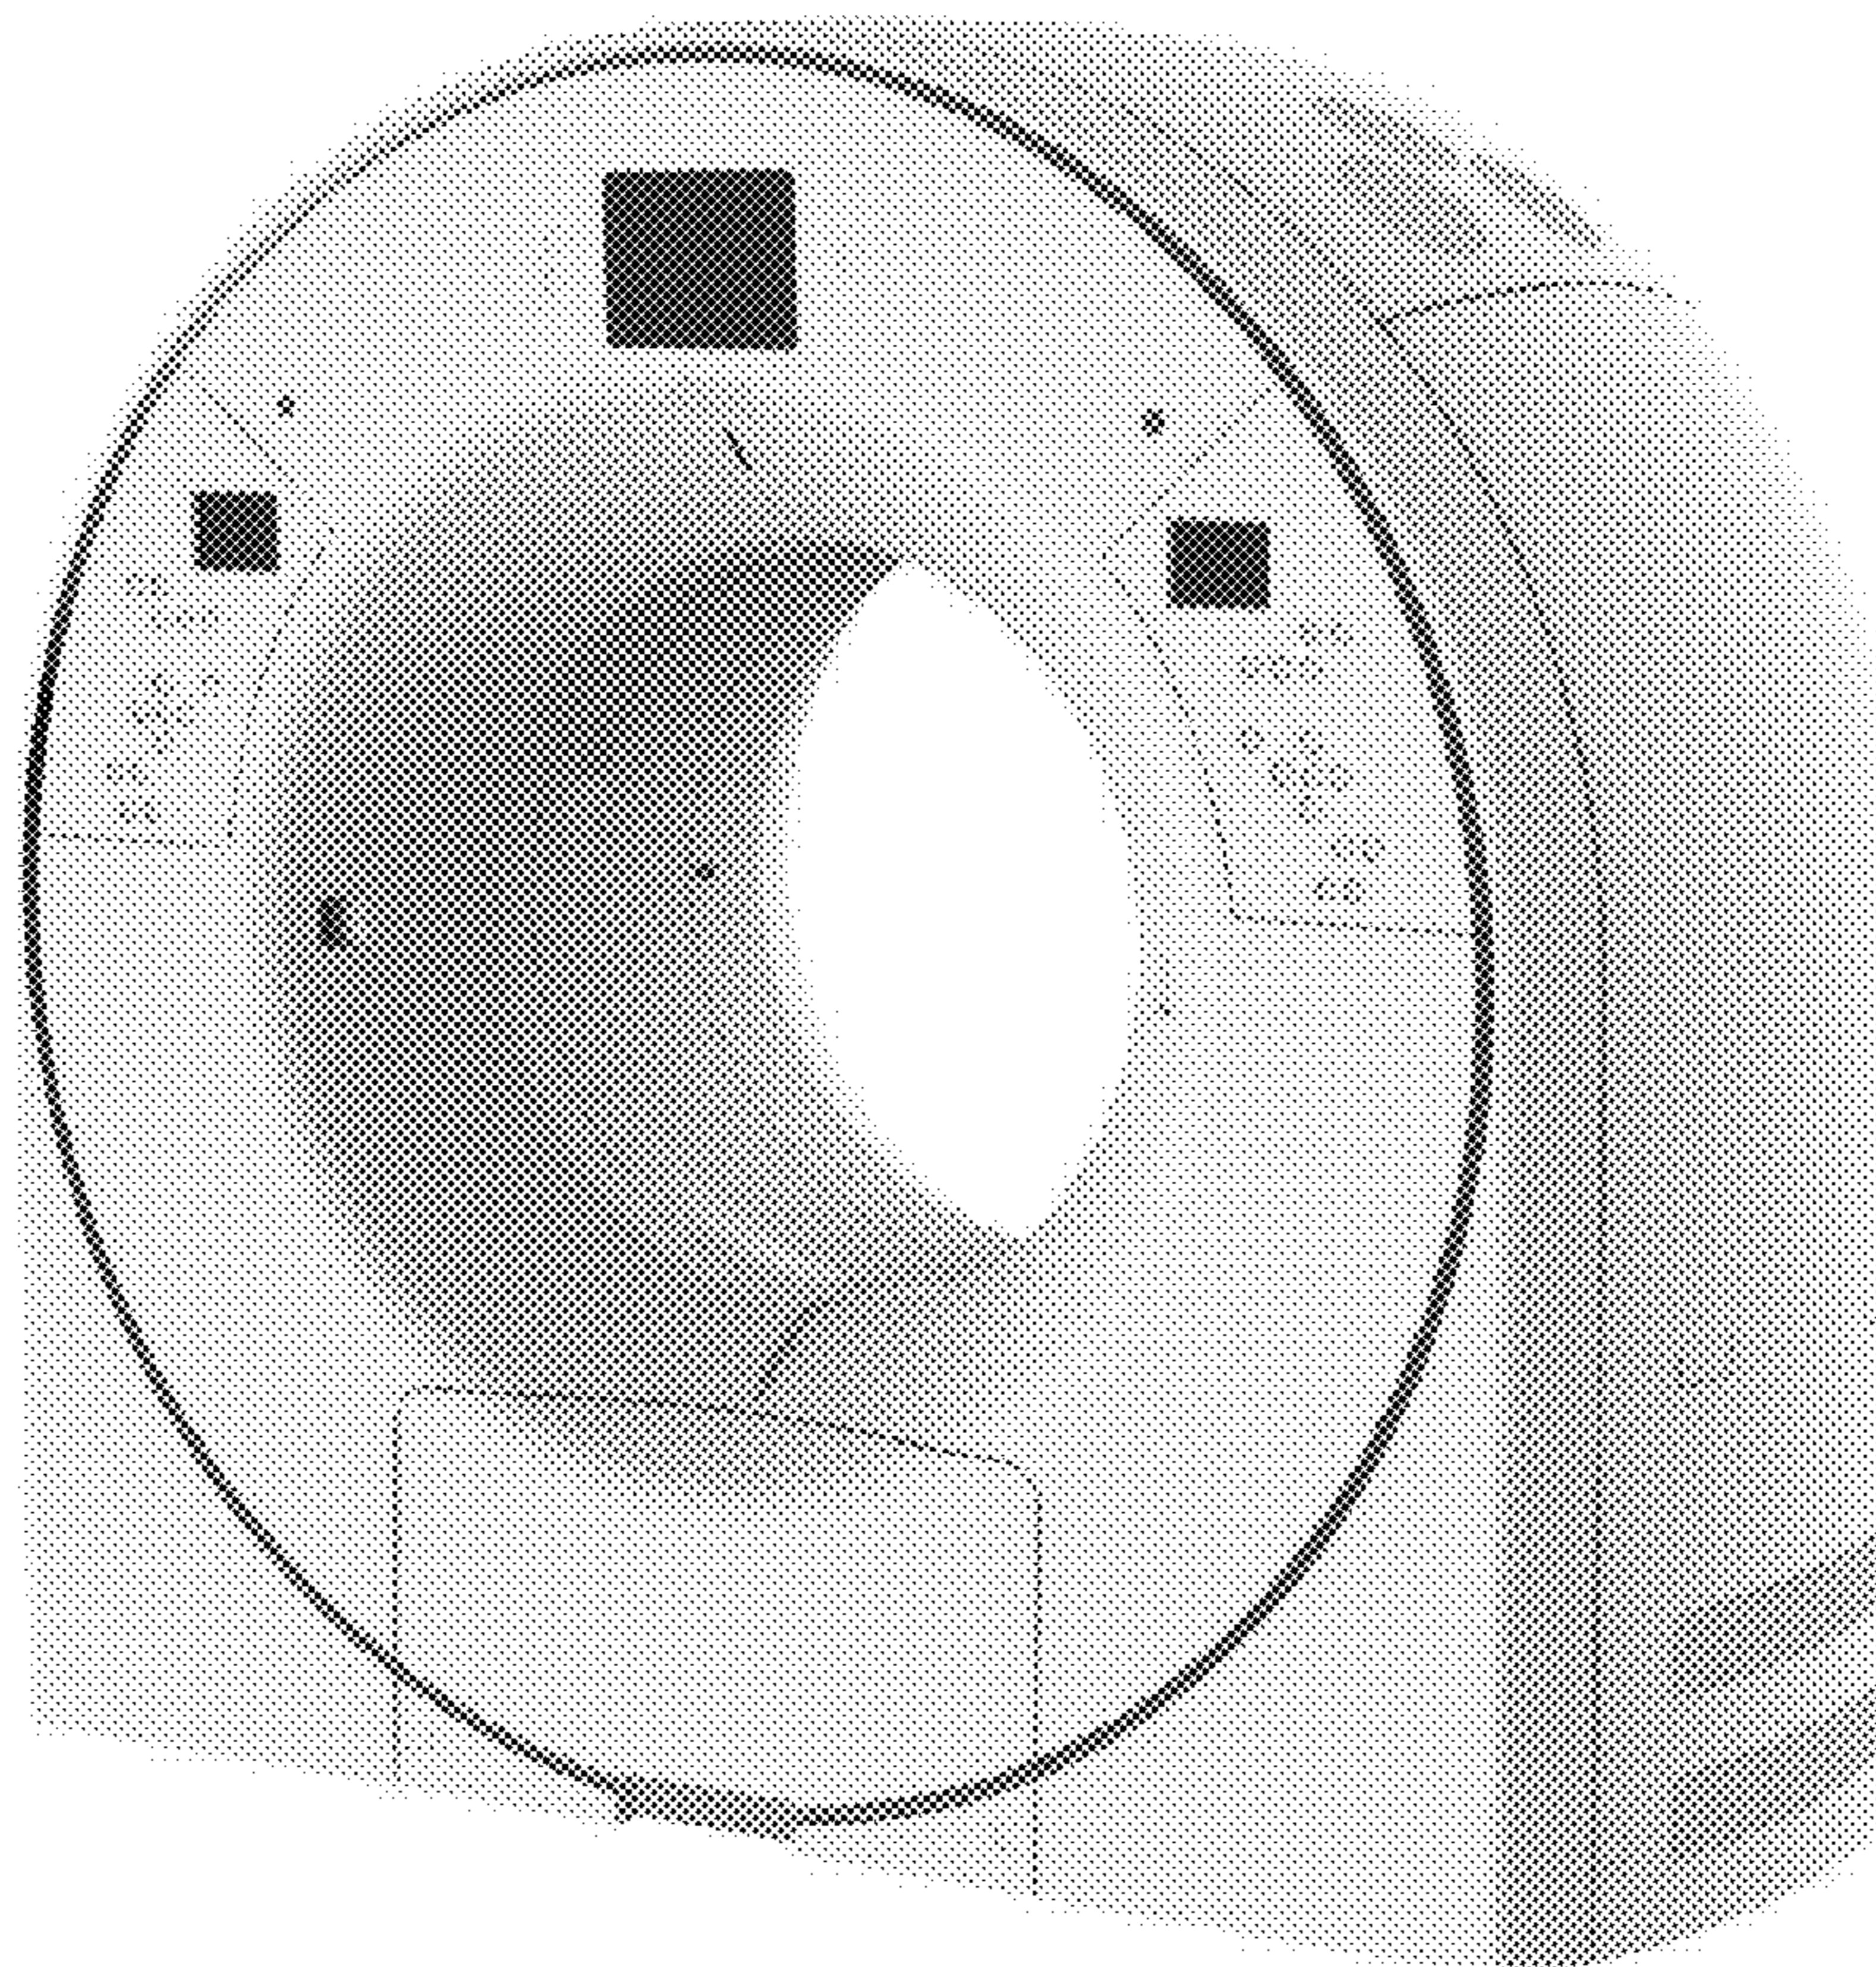




FIG.1

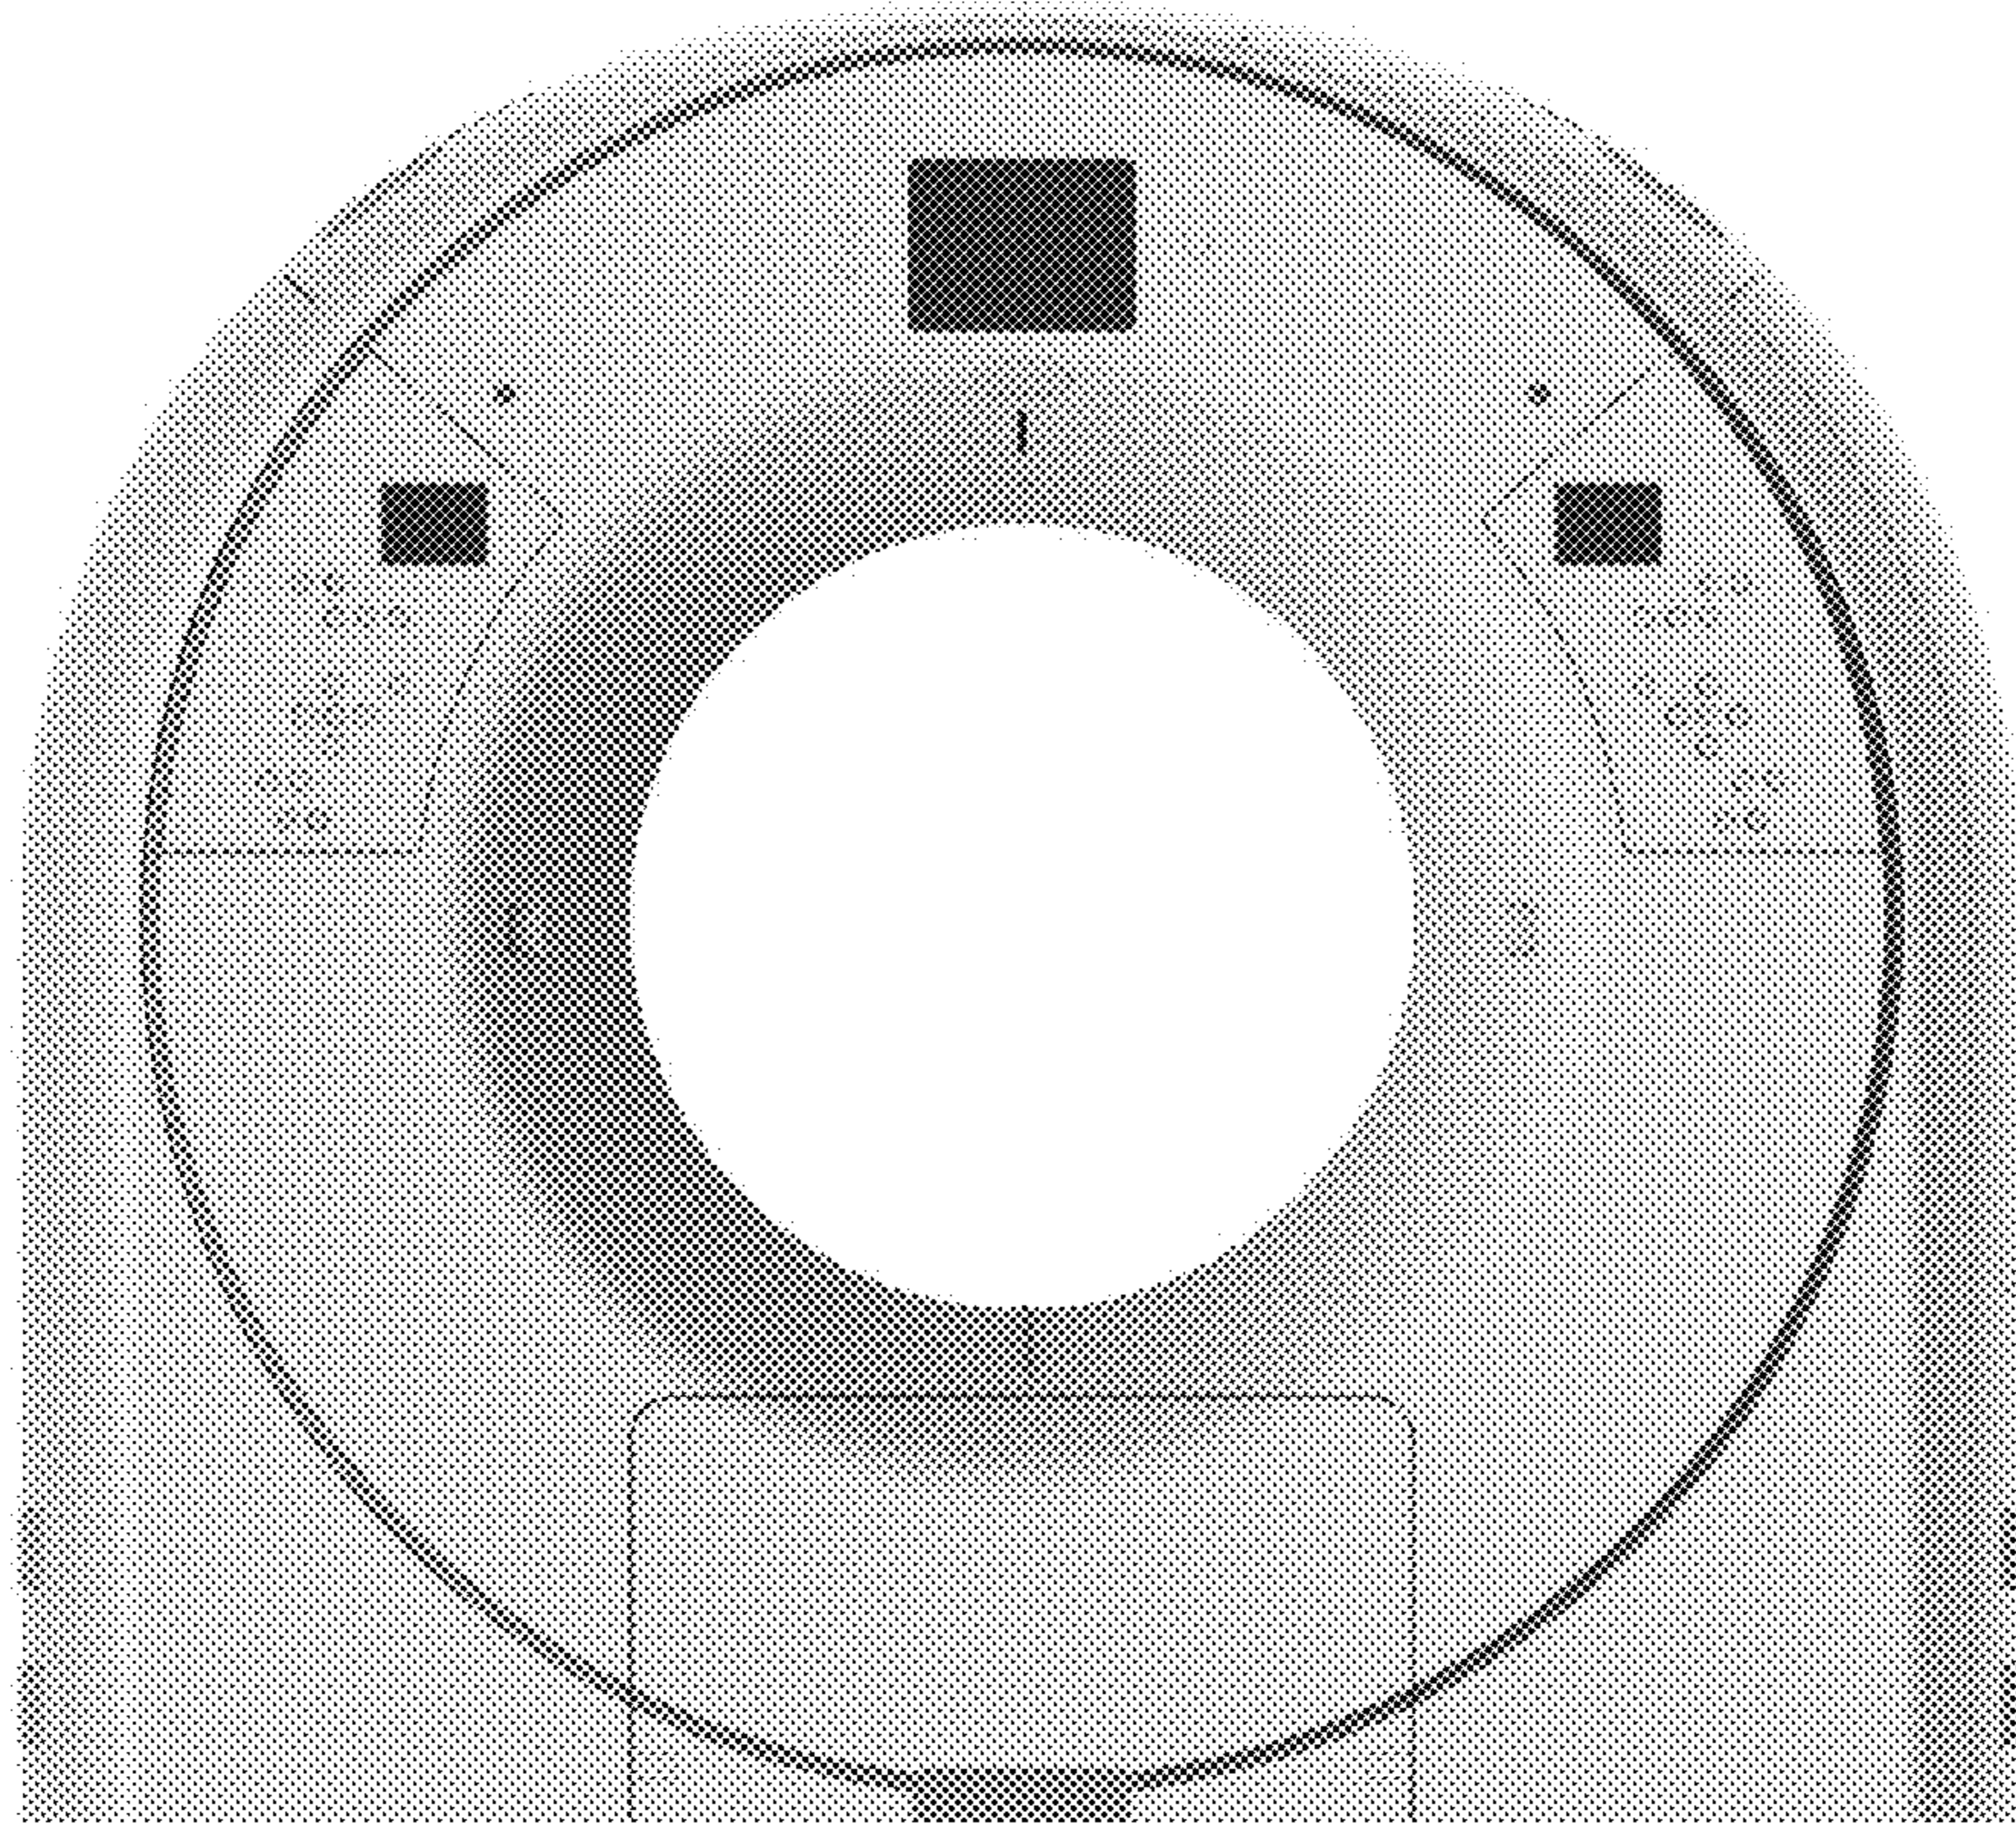


FIG.2

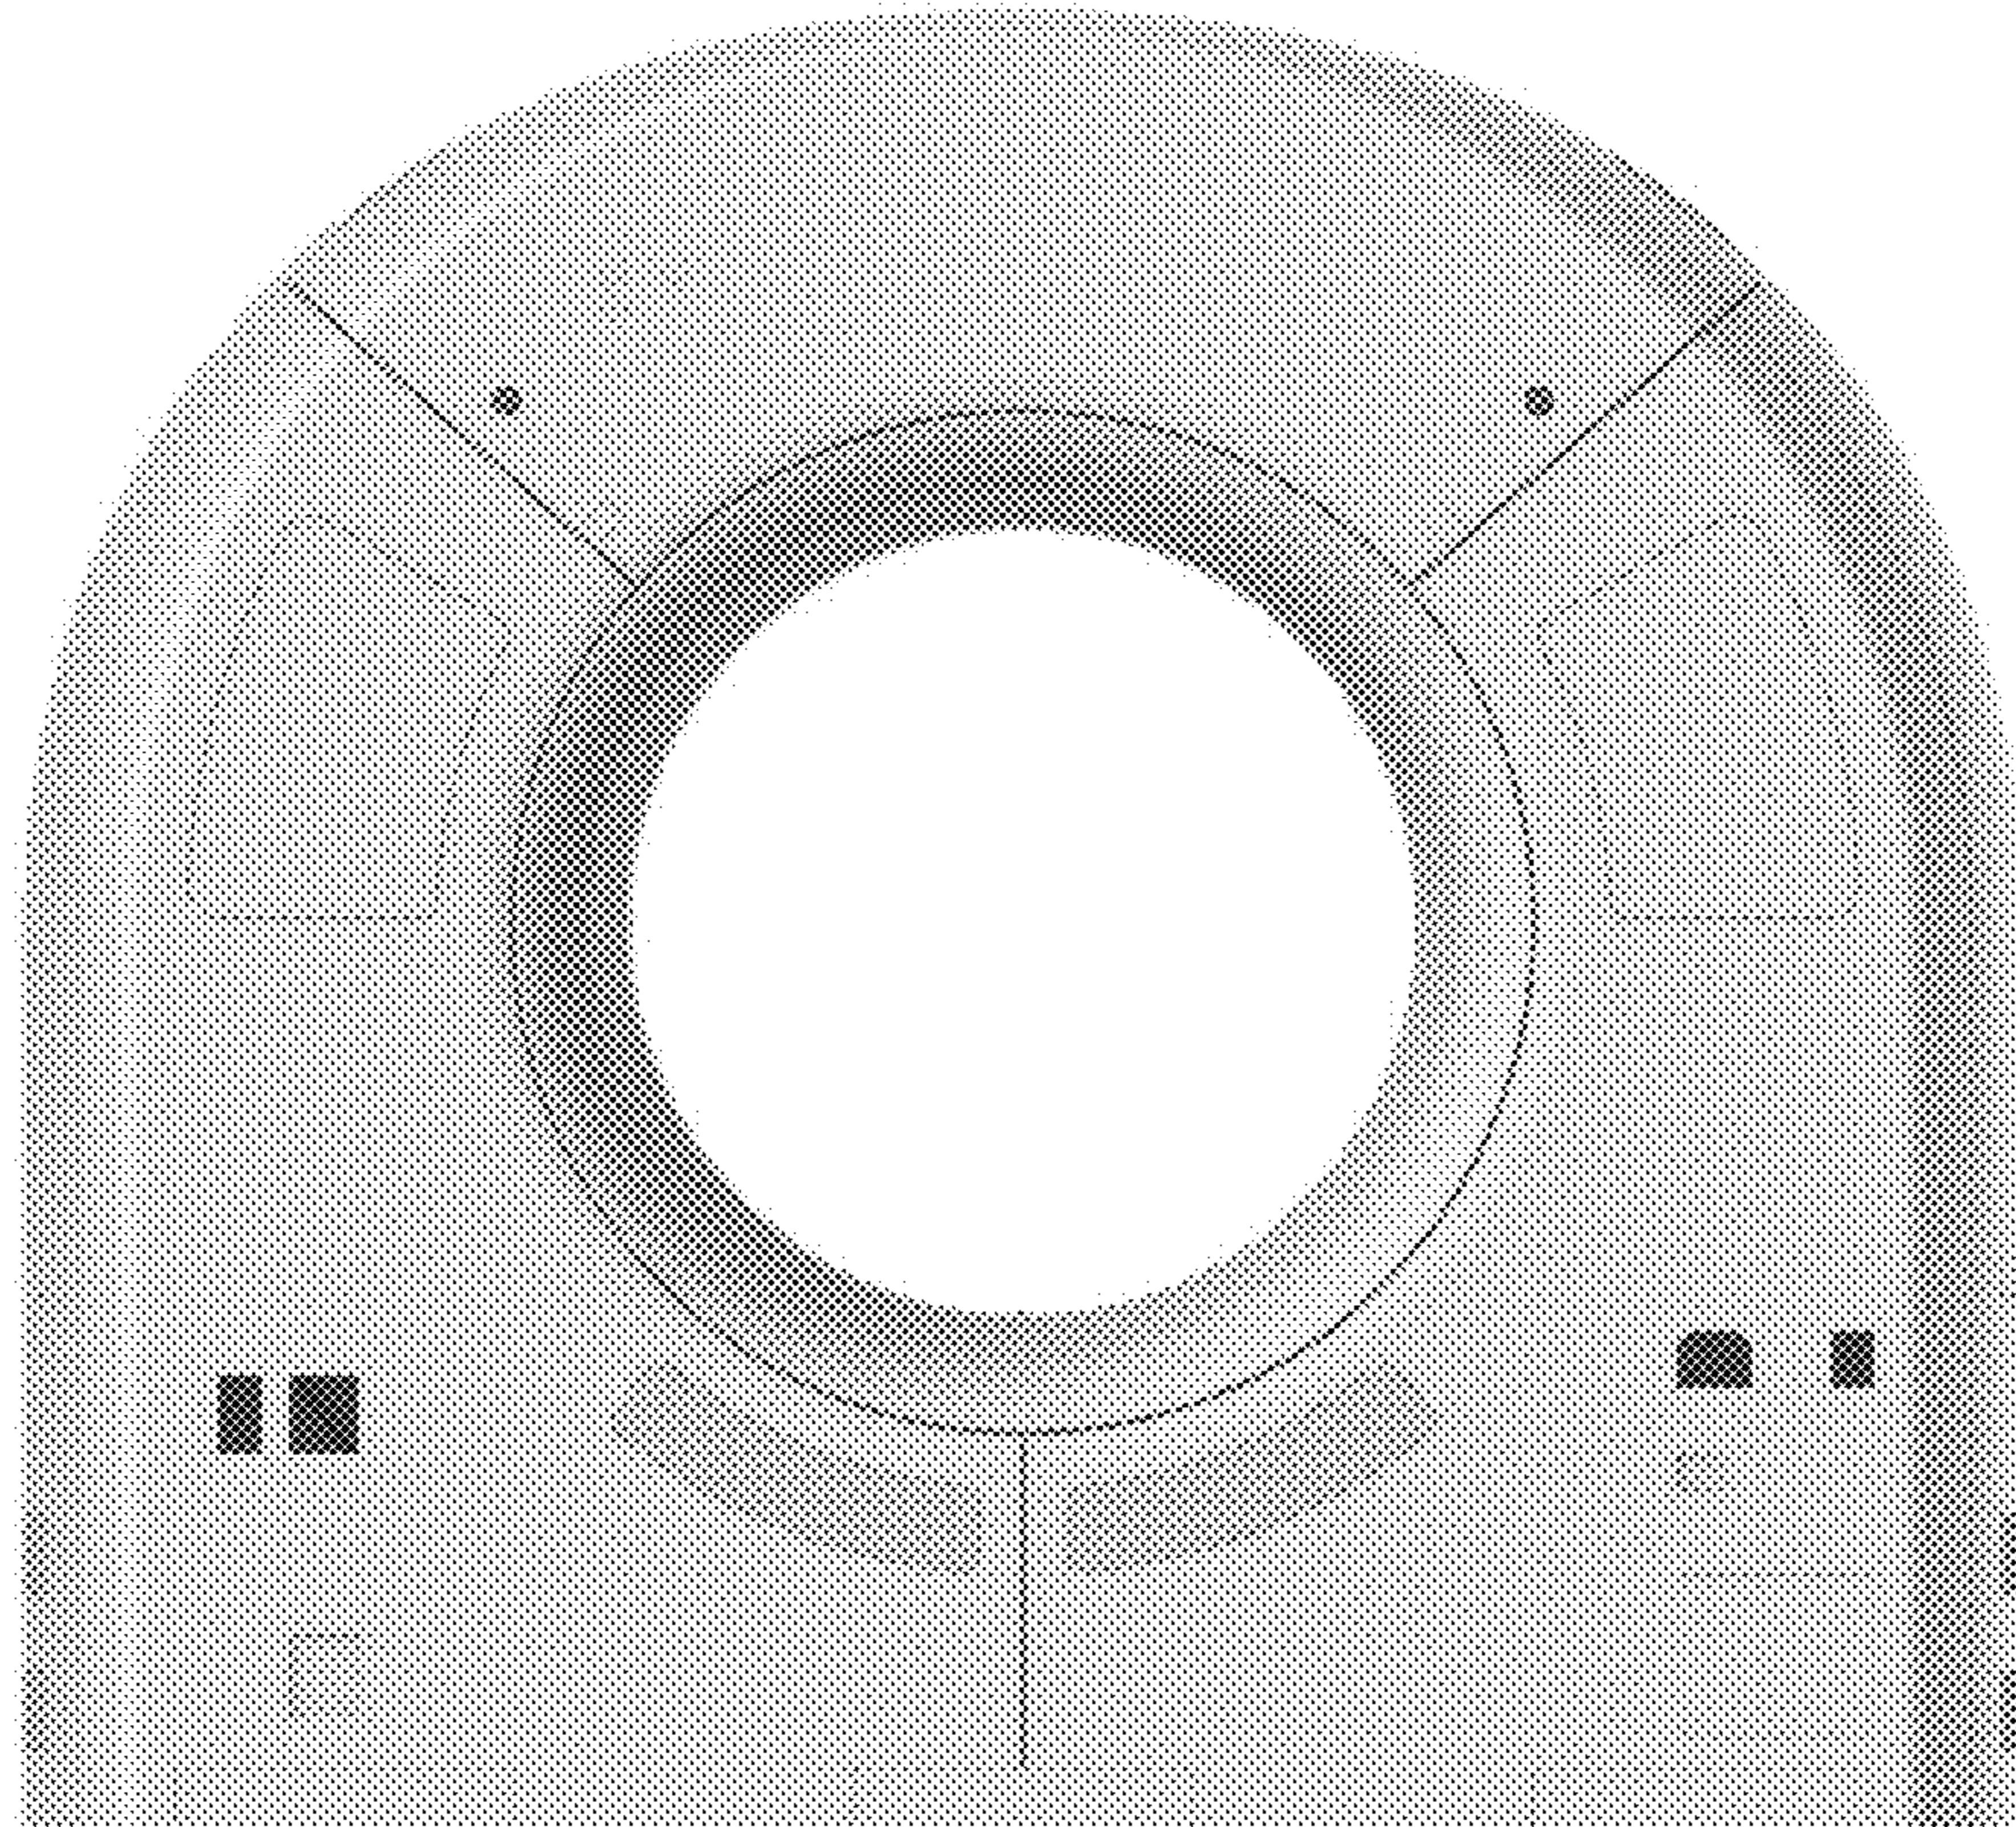


FIG.3

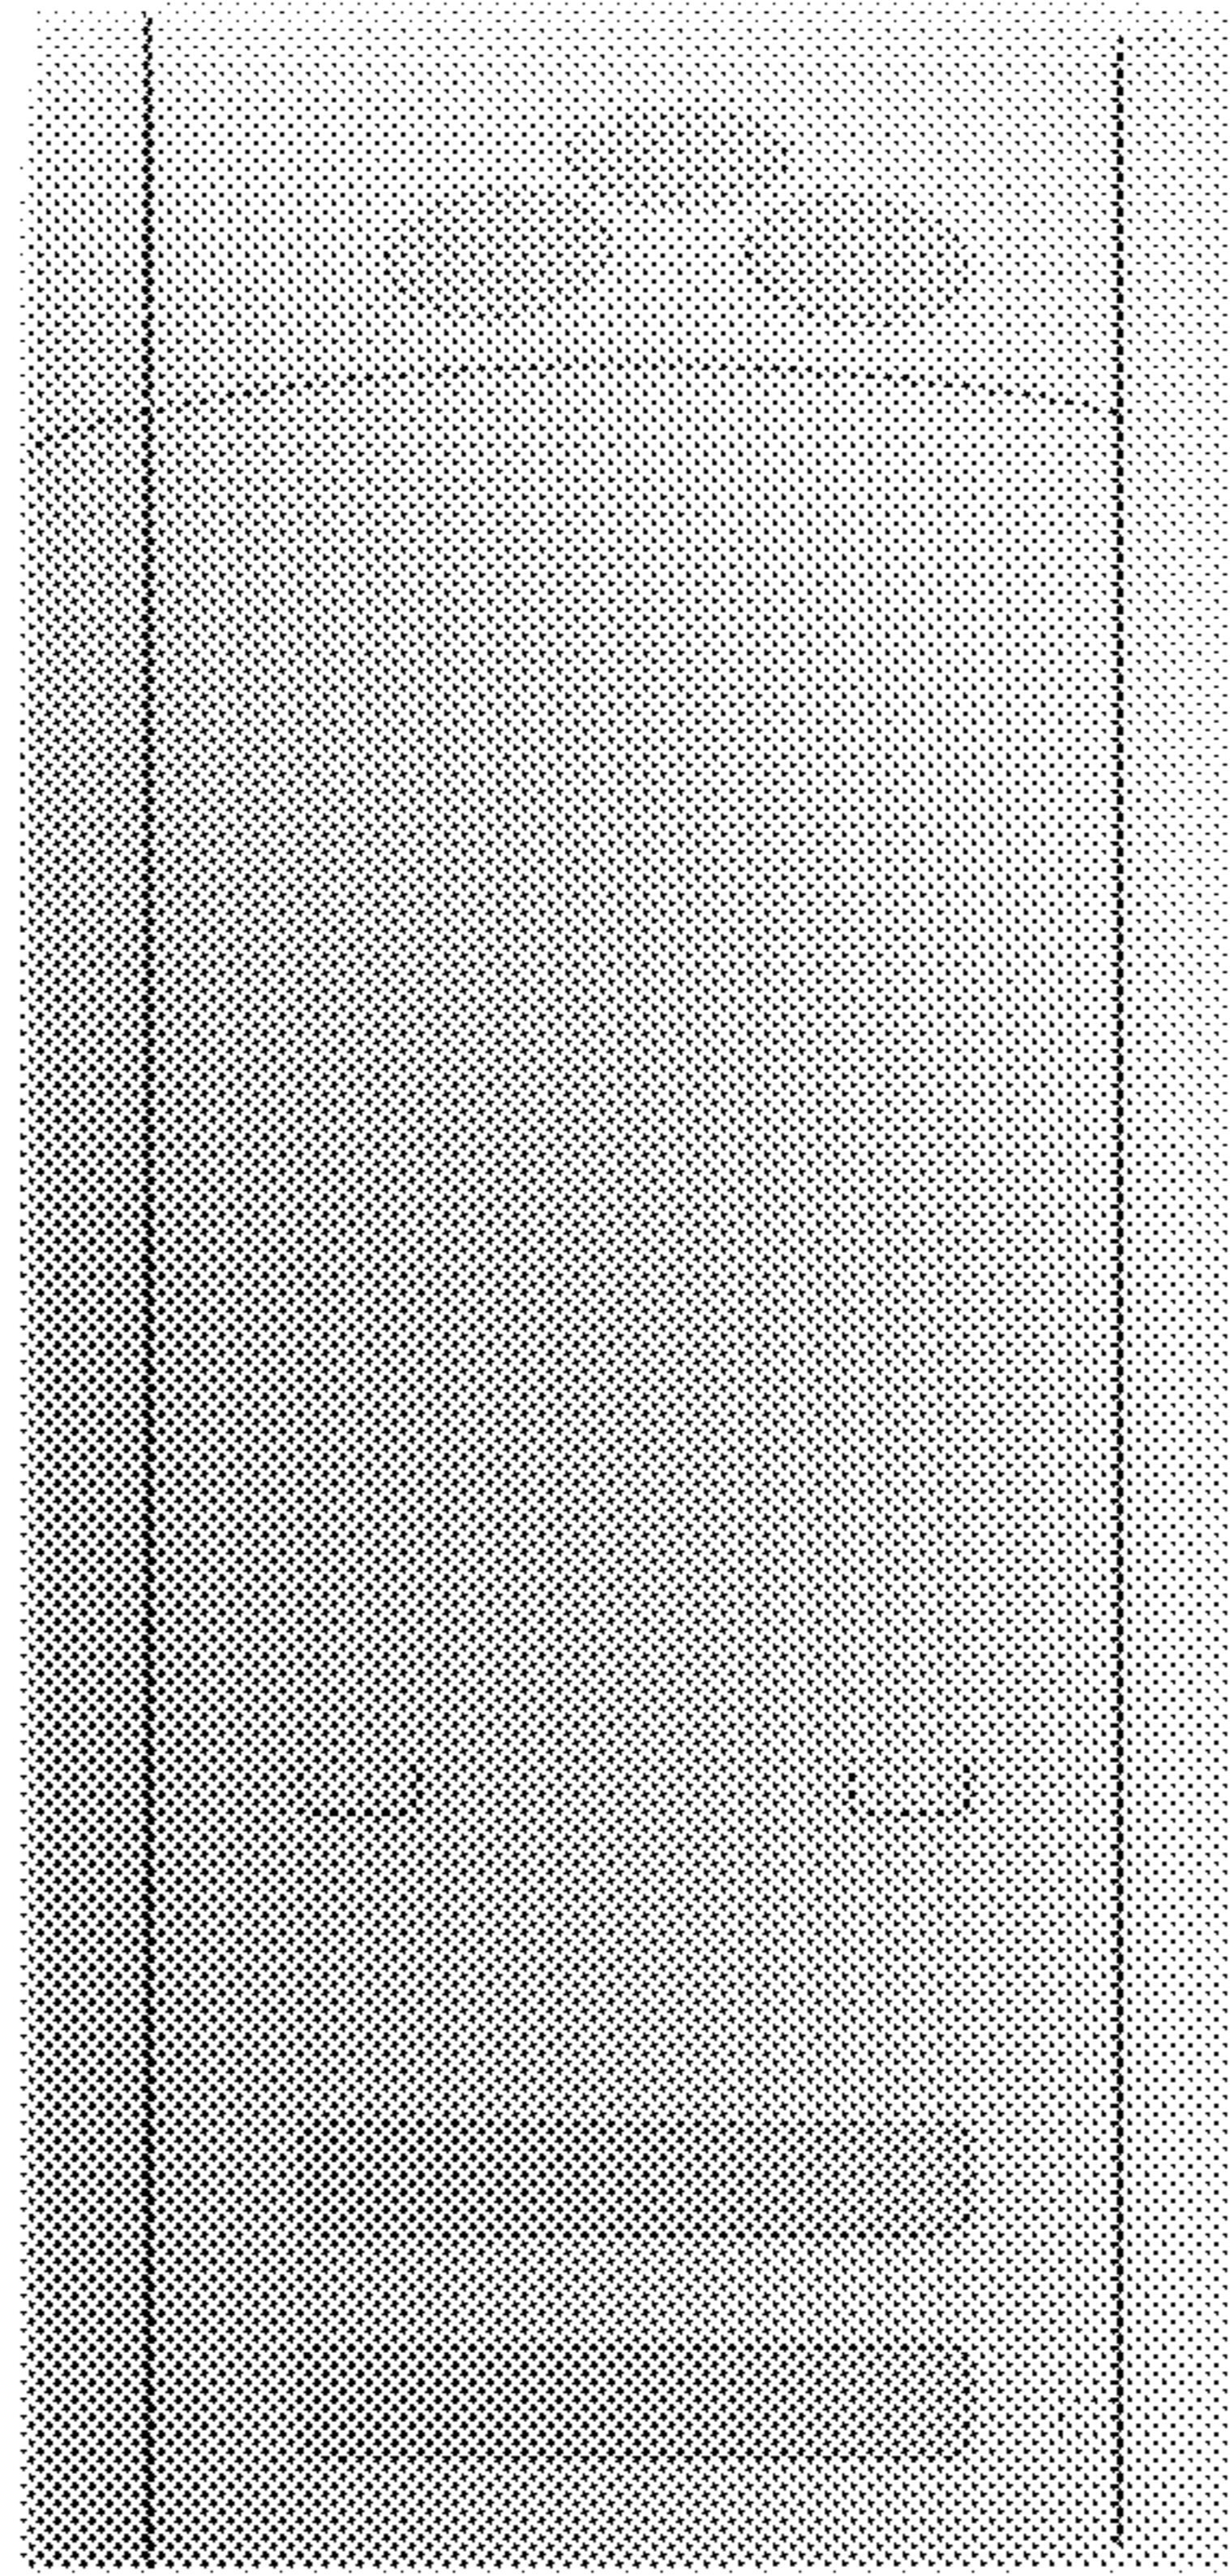


FIG.4

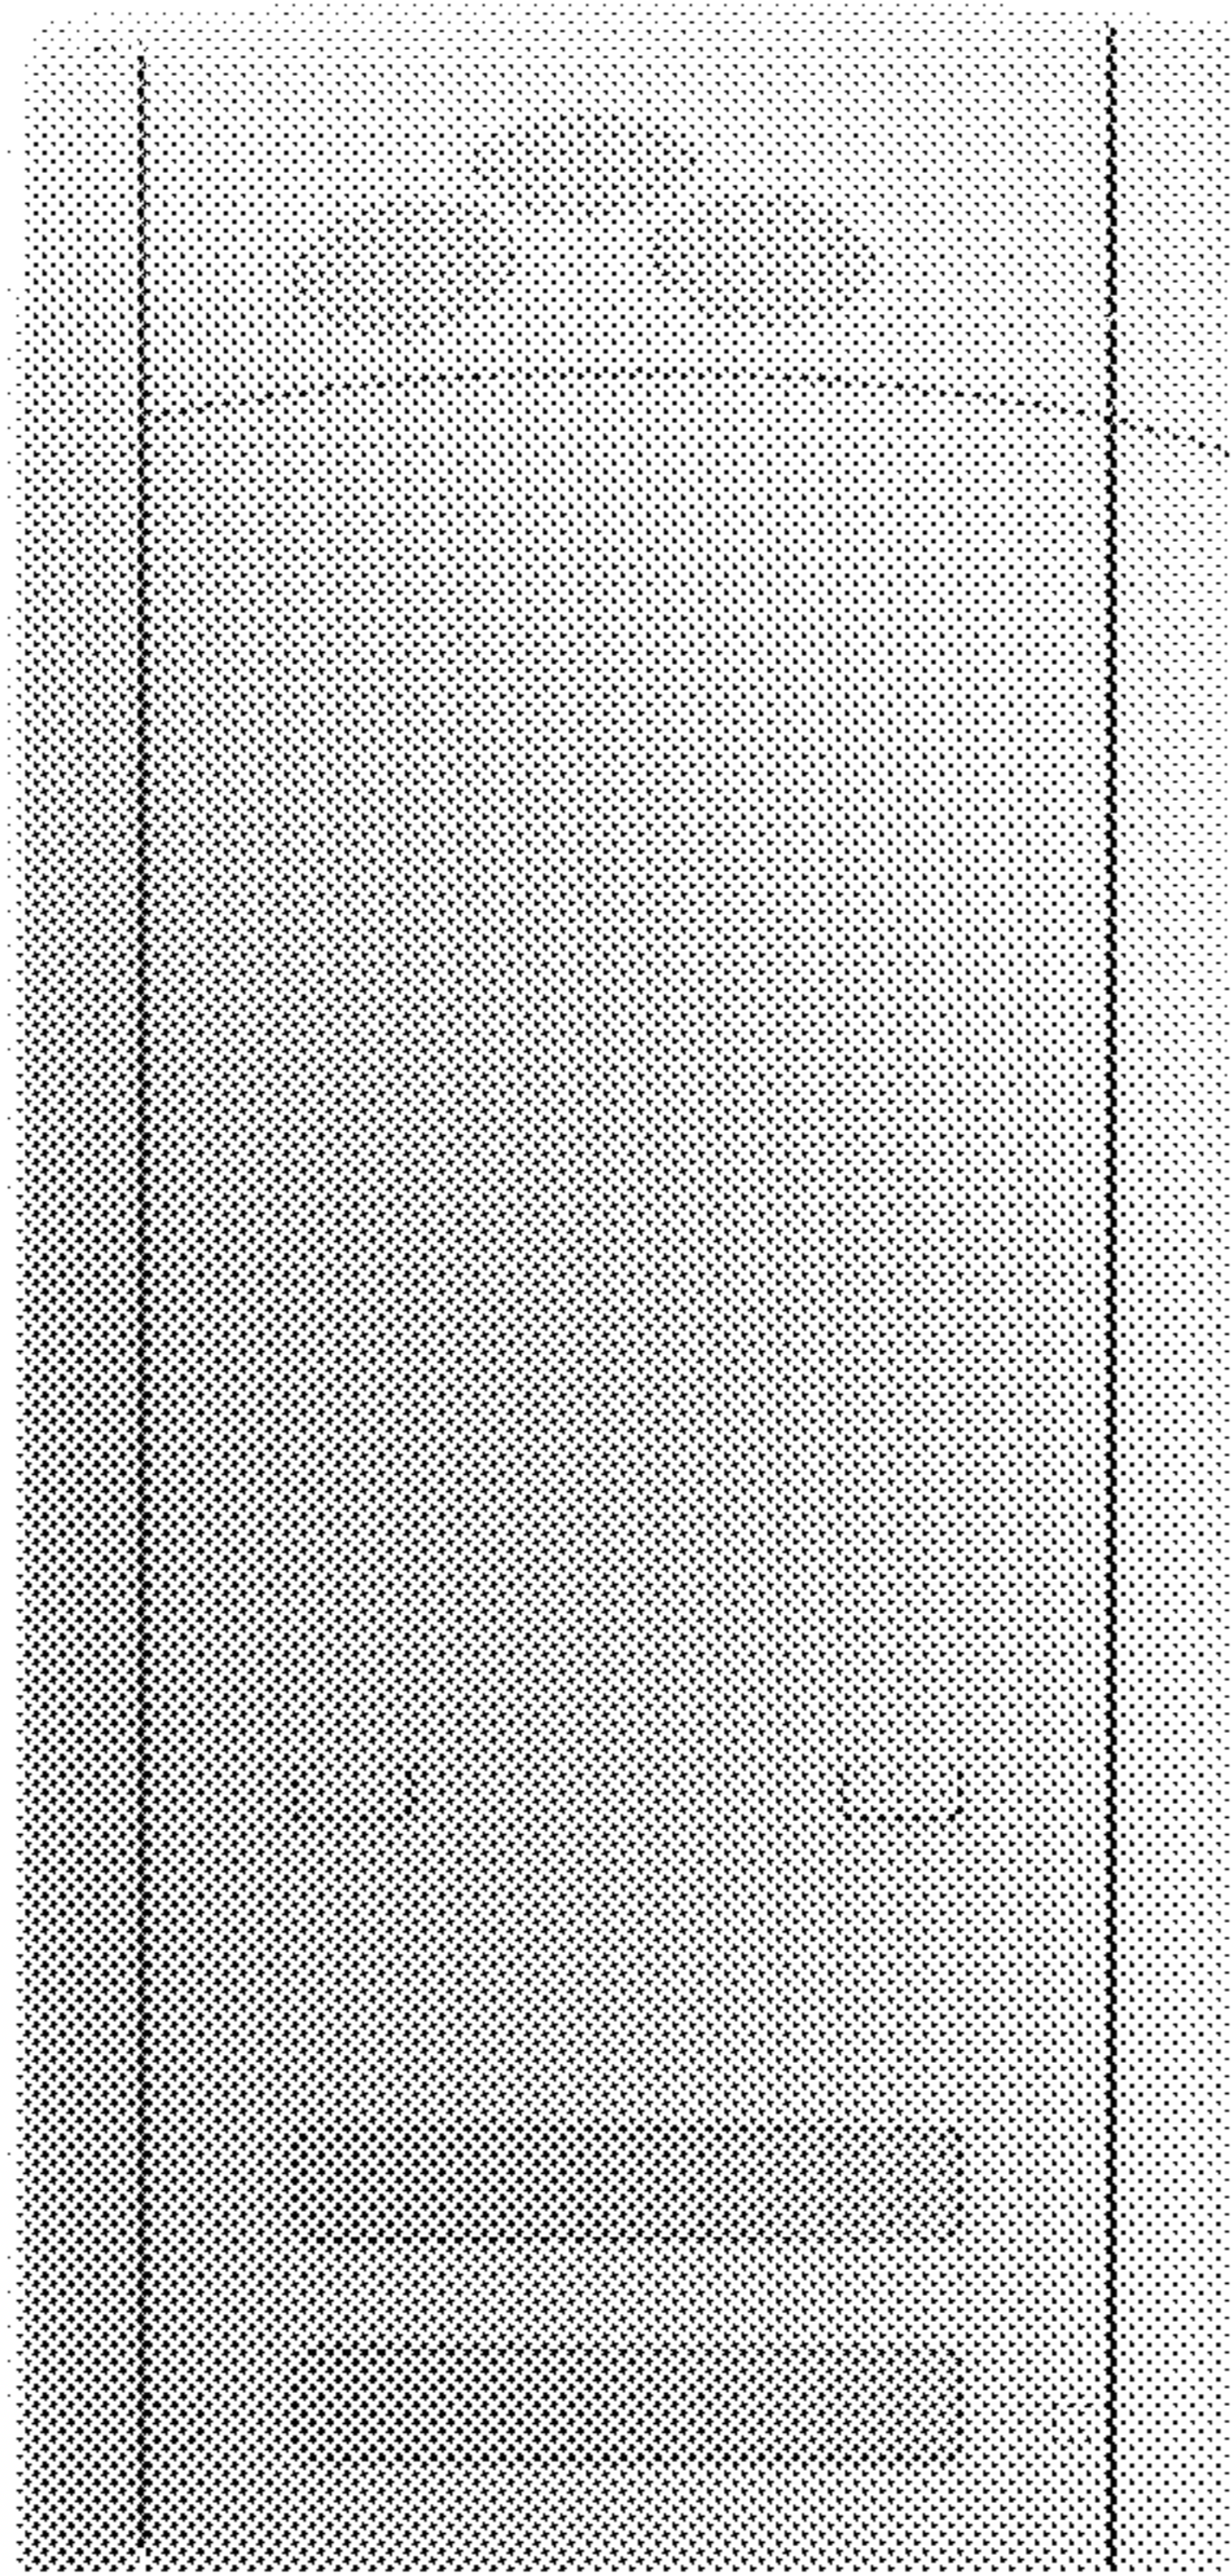


FIG.5

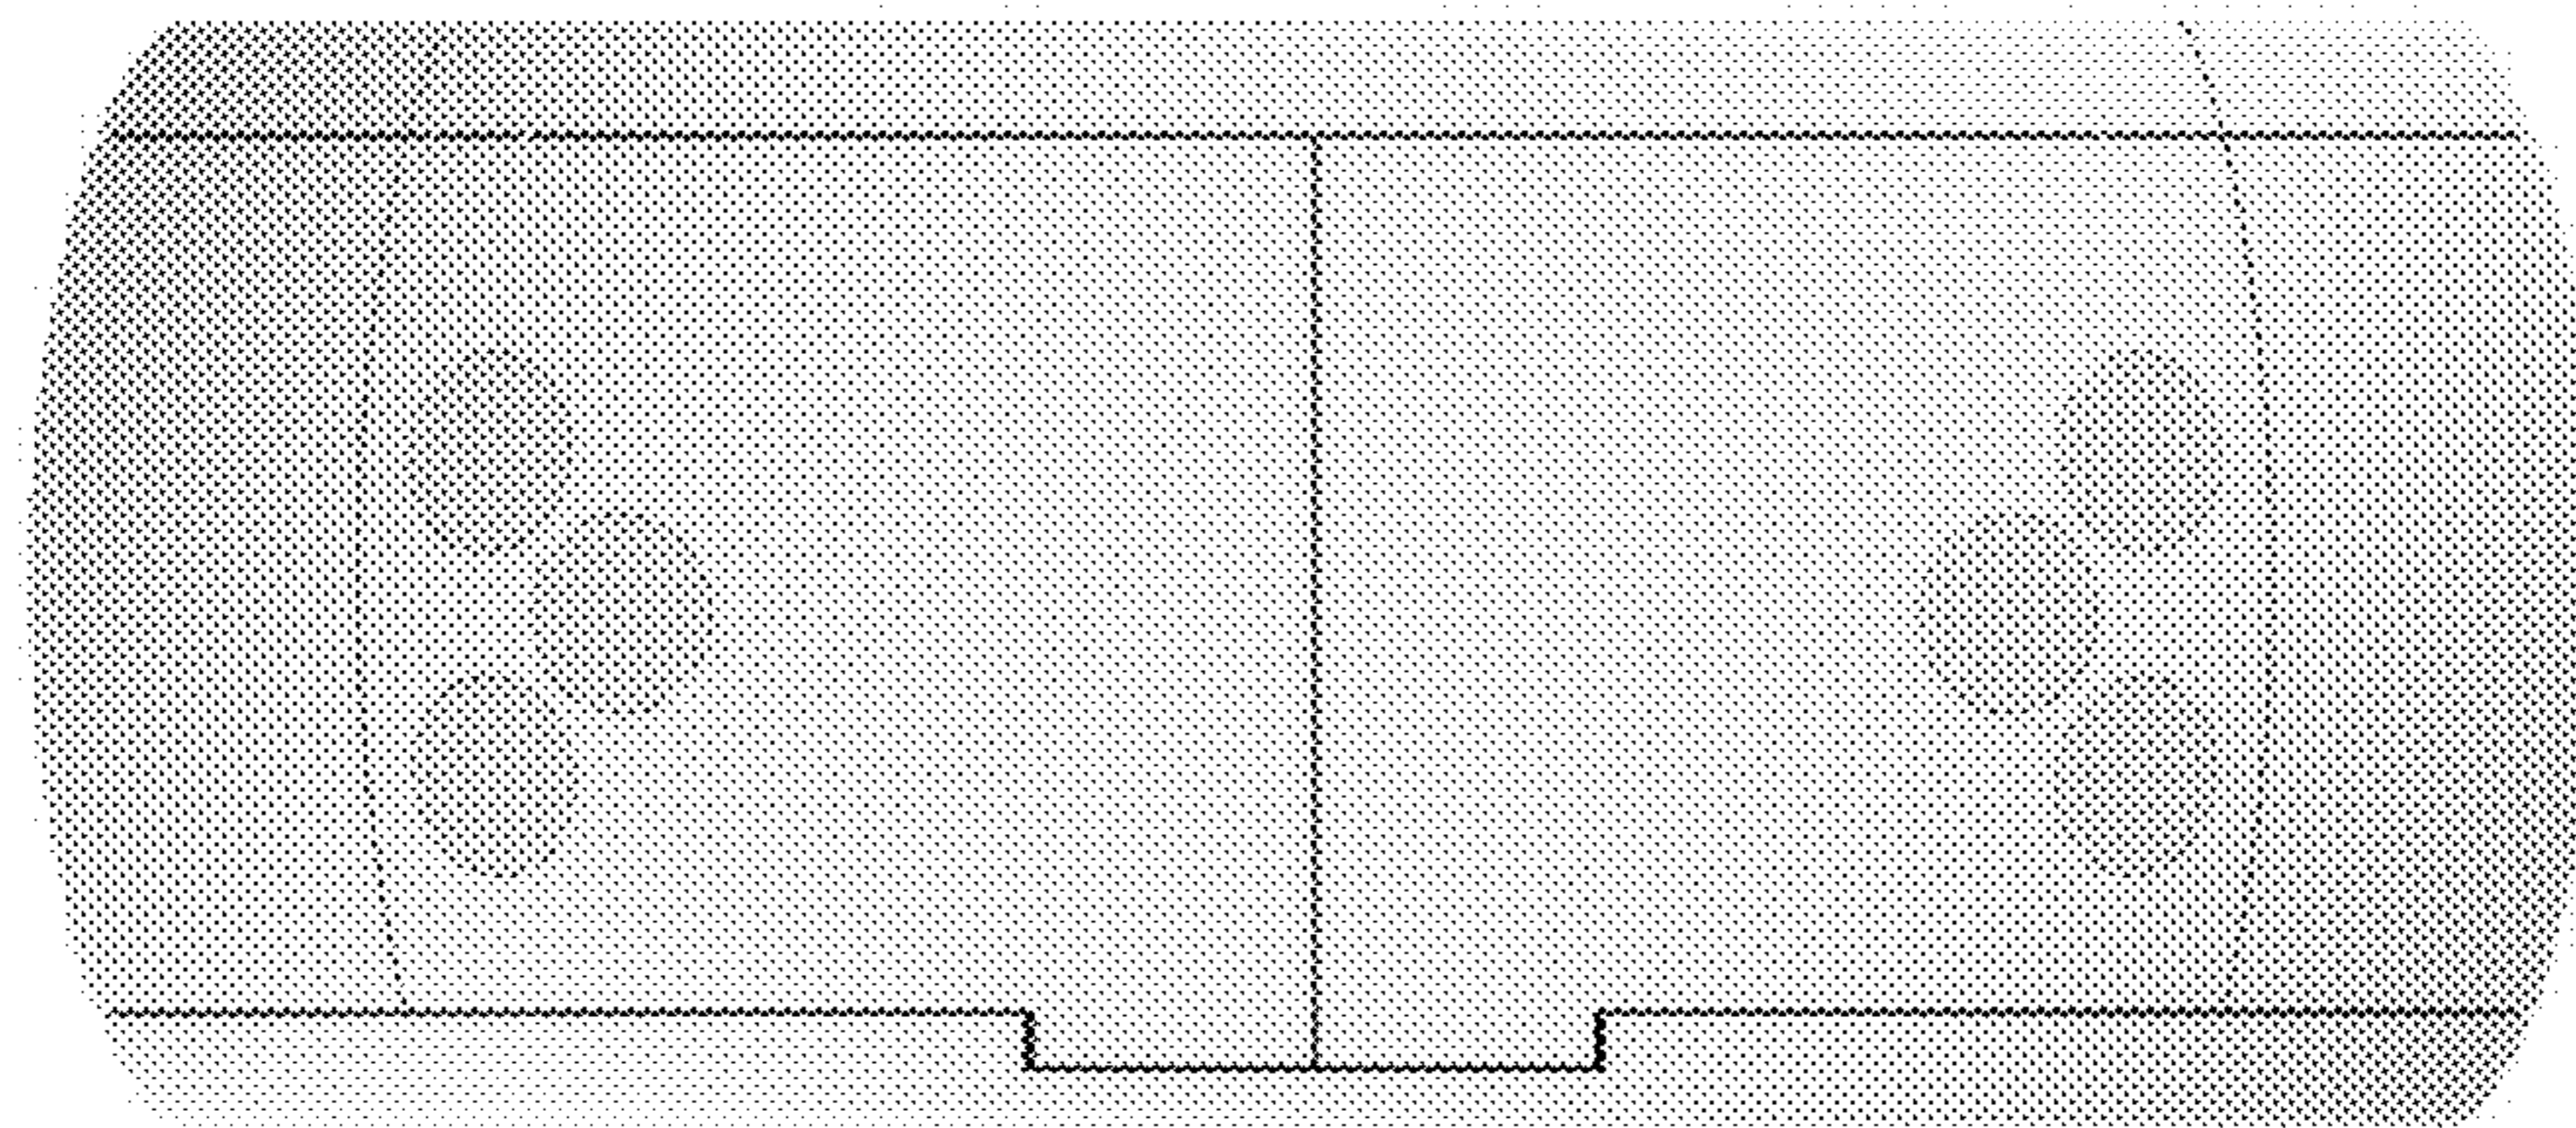


FIG. 6

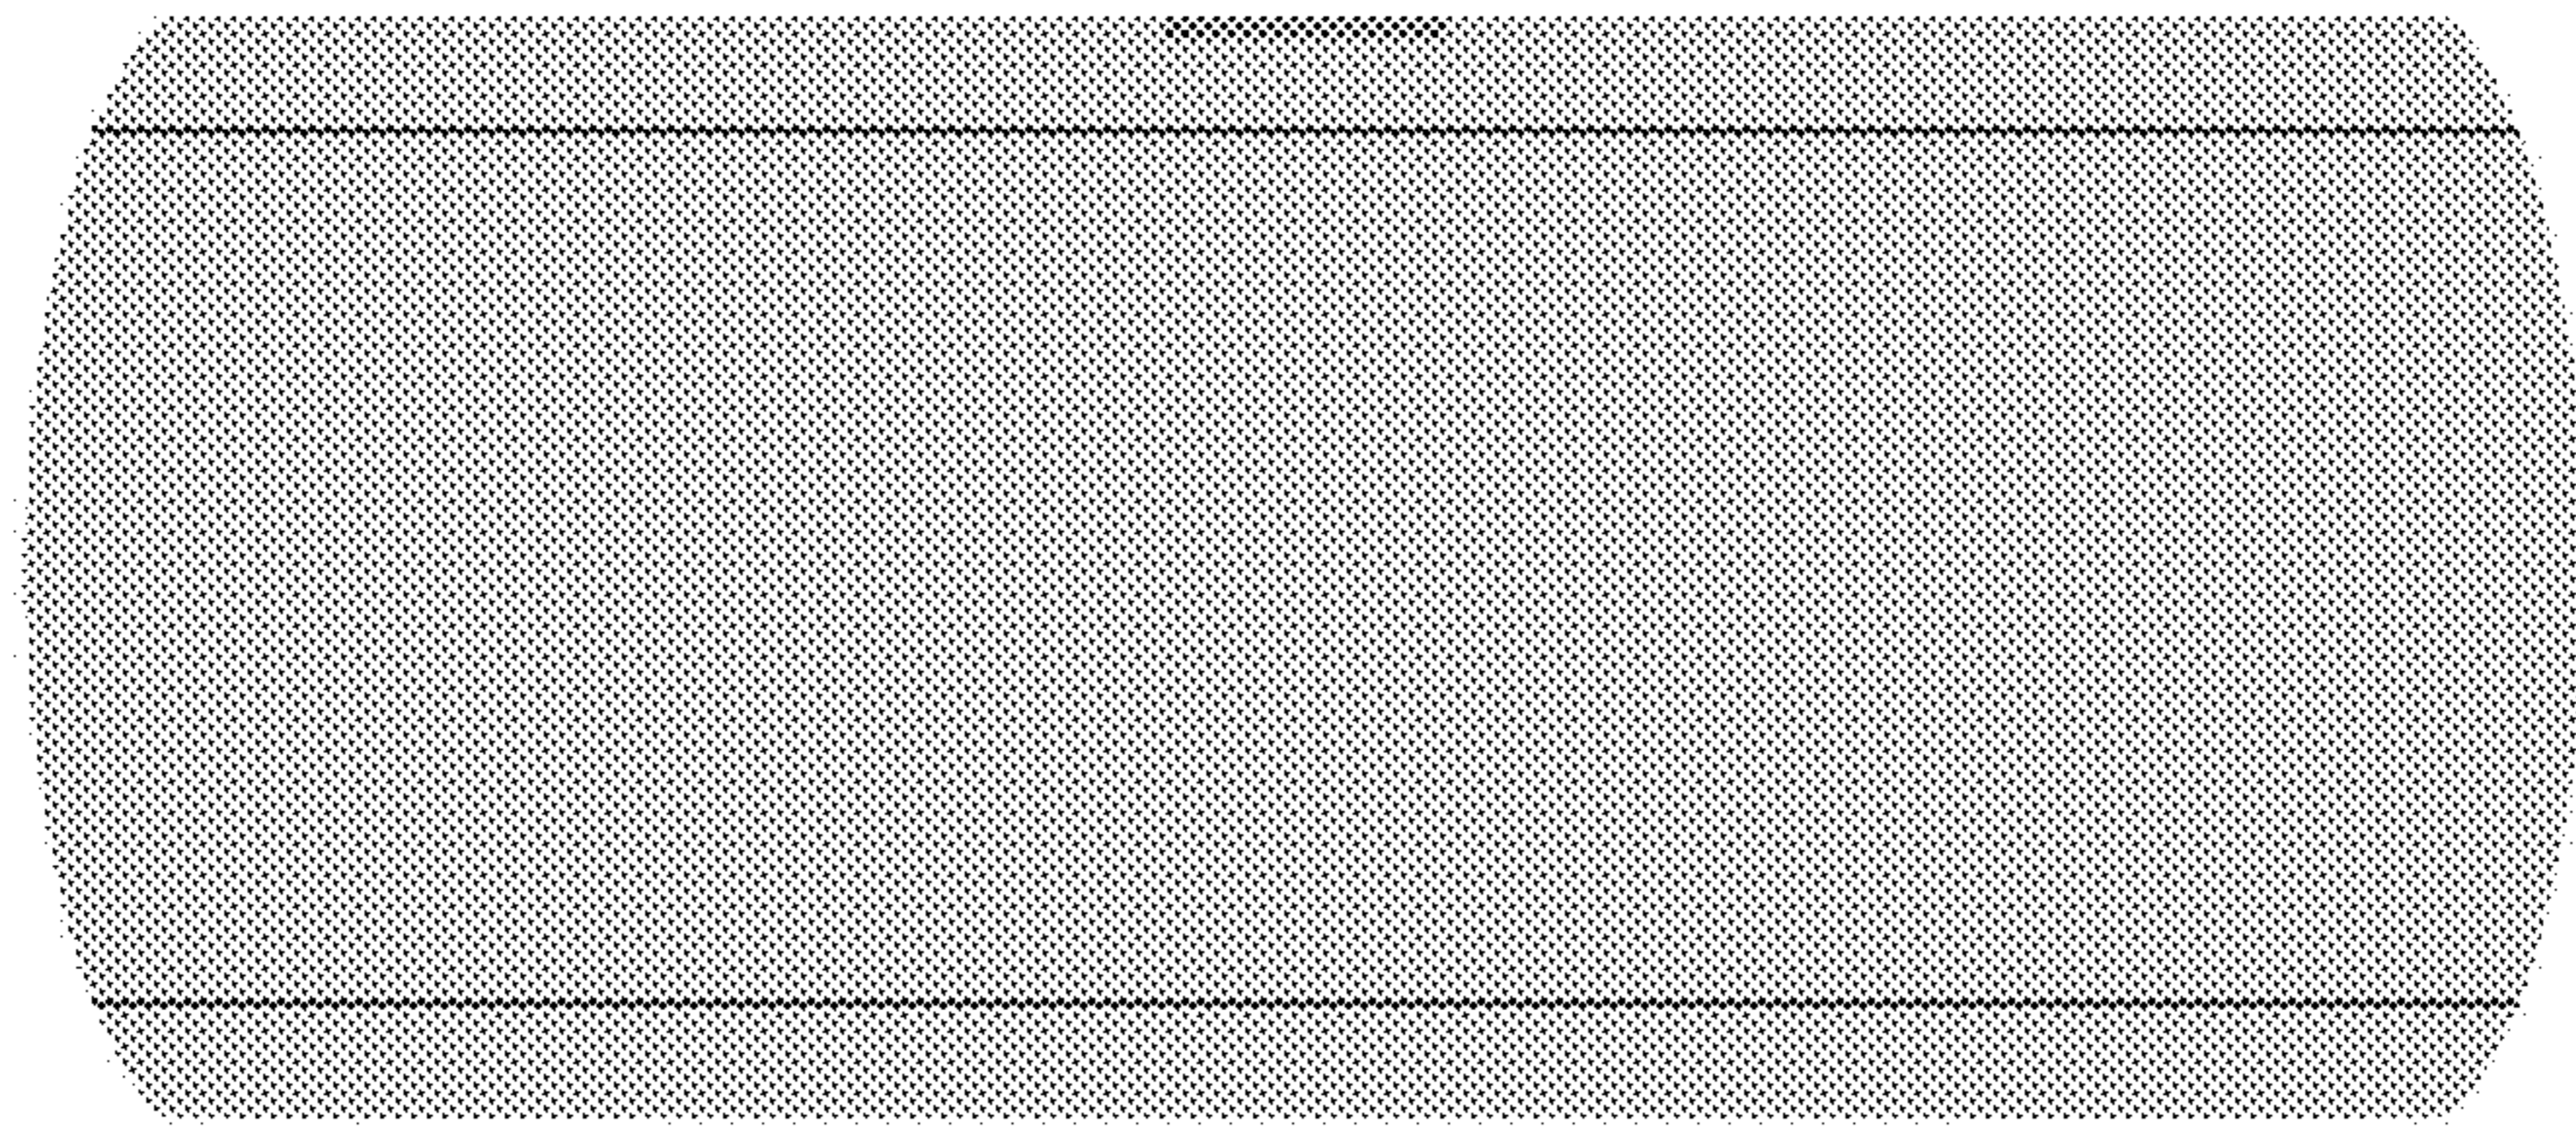


FIG. 7

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D961,774 S
APPLICATION NO. : 29/758284
DATED : August 23, 2022
INVENTOR(S) : Tetsuya Sekine et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

Item (30) The following Foreign Priority section should be added as:

(30) Foreign Application Priority Data
August 5, 2020 (JP)2020-016385 D

Signed and Sealed this
First Day of October, 2024
Katherine Kelly Vidal

Katherine Kelly Vidal
Director of the United States Patent and Trademark Office