



US00D961774S

(12) **United States Design Patent**  
**Sekine et al.**

(10) **Patent No.:** **US D961,774 S**

(45) **Date of Patent:** **\*\* Aug. 23, 2022**

(54) **SCANNER FOR AN X-RAY TOMOGRAPHY  
DIAGNOSIS APPARATUS**

(71) Applicant: **Canon Medical Systems Corporation,**  
Otawara (JP)

(72) Inventors: **Tetsuya Sekine,** Kawasaki Kanagawa  
(JP); **Koichiro Oishi,** Wako Saitama  
(JP)

(73) Assignee: **Canon Medical Systems Corporation,**  
Otawara (JP)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/758,284**

(22) Filed: **Nov. 13, 2020**

(51) **LOC (13) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/158**

(58) **Field of Classification Search**  
USPC ..... D24/107, 158-161, 185, 186  
CPC .. A61B 6/03; A61B 6/035; A61B 5/05; A61B  
5/055

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D628,294 S \* 11/2010 Baba ..... D24/158  
D701,311 S \* 3/2014 Ohmukai ..... D24/158

D701,312 S \* 3/2014 Ohmukai ..... D24/158  
D715,944 S \* 10/2014 Yao ..... D24/159  
D725,275 S \* 3/2015 Matsumura ..... D24/158  
D753,828 S \* 4/2016 Baba ..... D24/158  
D770,624 S \* 11/2016 Yao ..... D24/158  
D783,830 S \* 4/2017 Baba ..... D24/158  
D927,691 S \* 8/2021 Ooshima ..... D24/158  
2017/0105692 A1\* 4/2017 Sawanobori ..... A61B 6/035

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson,  
Farabow, Garrett & Dunner, L.L.P.

(57) **CLAIM**

The ornamental design for an scanner for an X-ray tomog-  
raphy diagnosis apparatus, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a scanner for an X-ray  
tomography diagnosis apparatus showing our new design;  
FIG. 2 is a front elevational view thereof;  
FIG. 3 is a rear elevational view thereof;  
FIG. 4 is a left-side elevational view thereof;  
FIG. 5 is a right-side elevational view thereof;  
FIG. 6 is a top plan view thereof; and,  
FIG. 7 is a bottom plan view thereof.

**1 Claim, 7 Drawing Sheets**





FIG.1

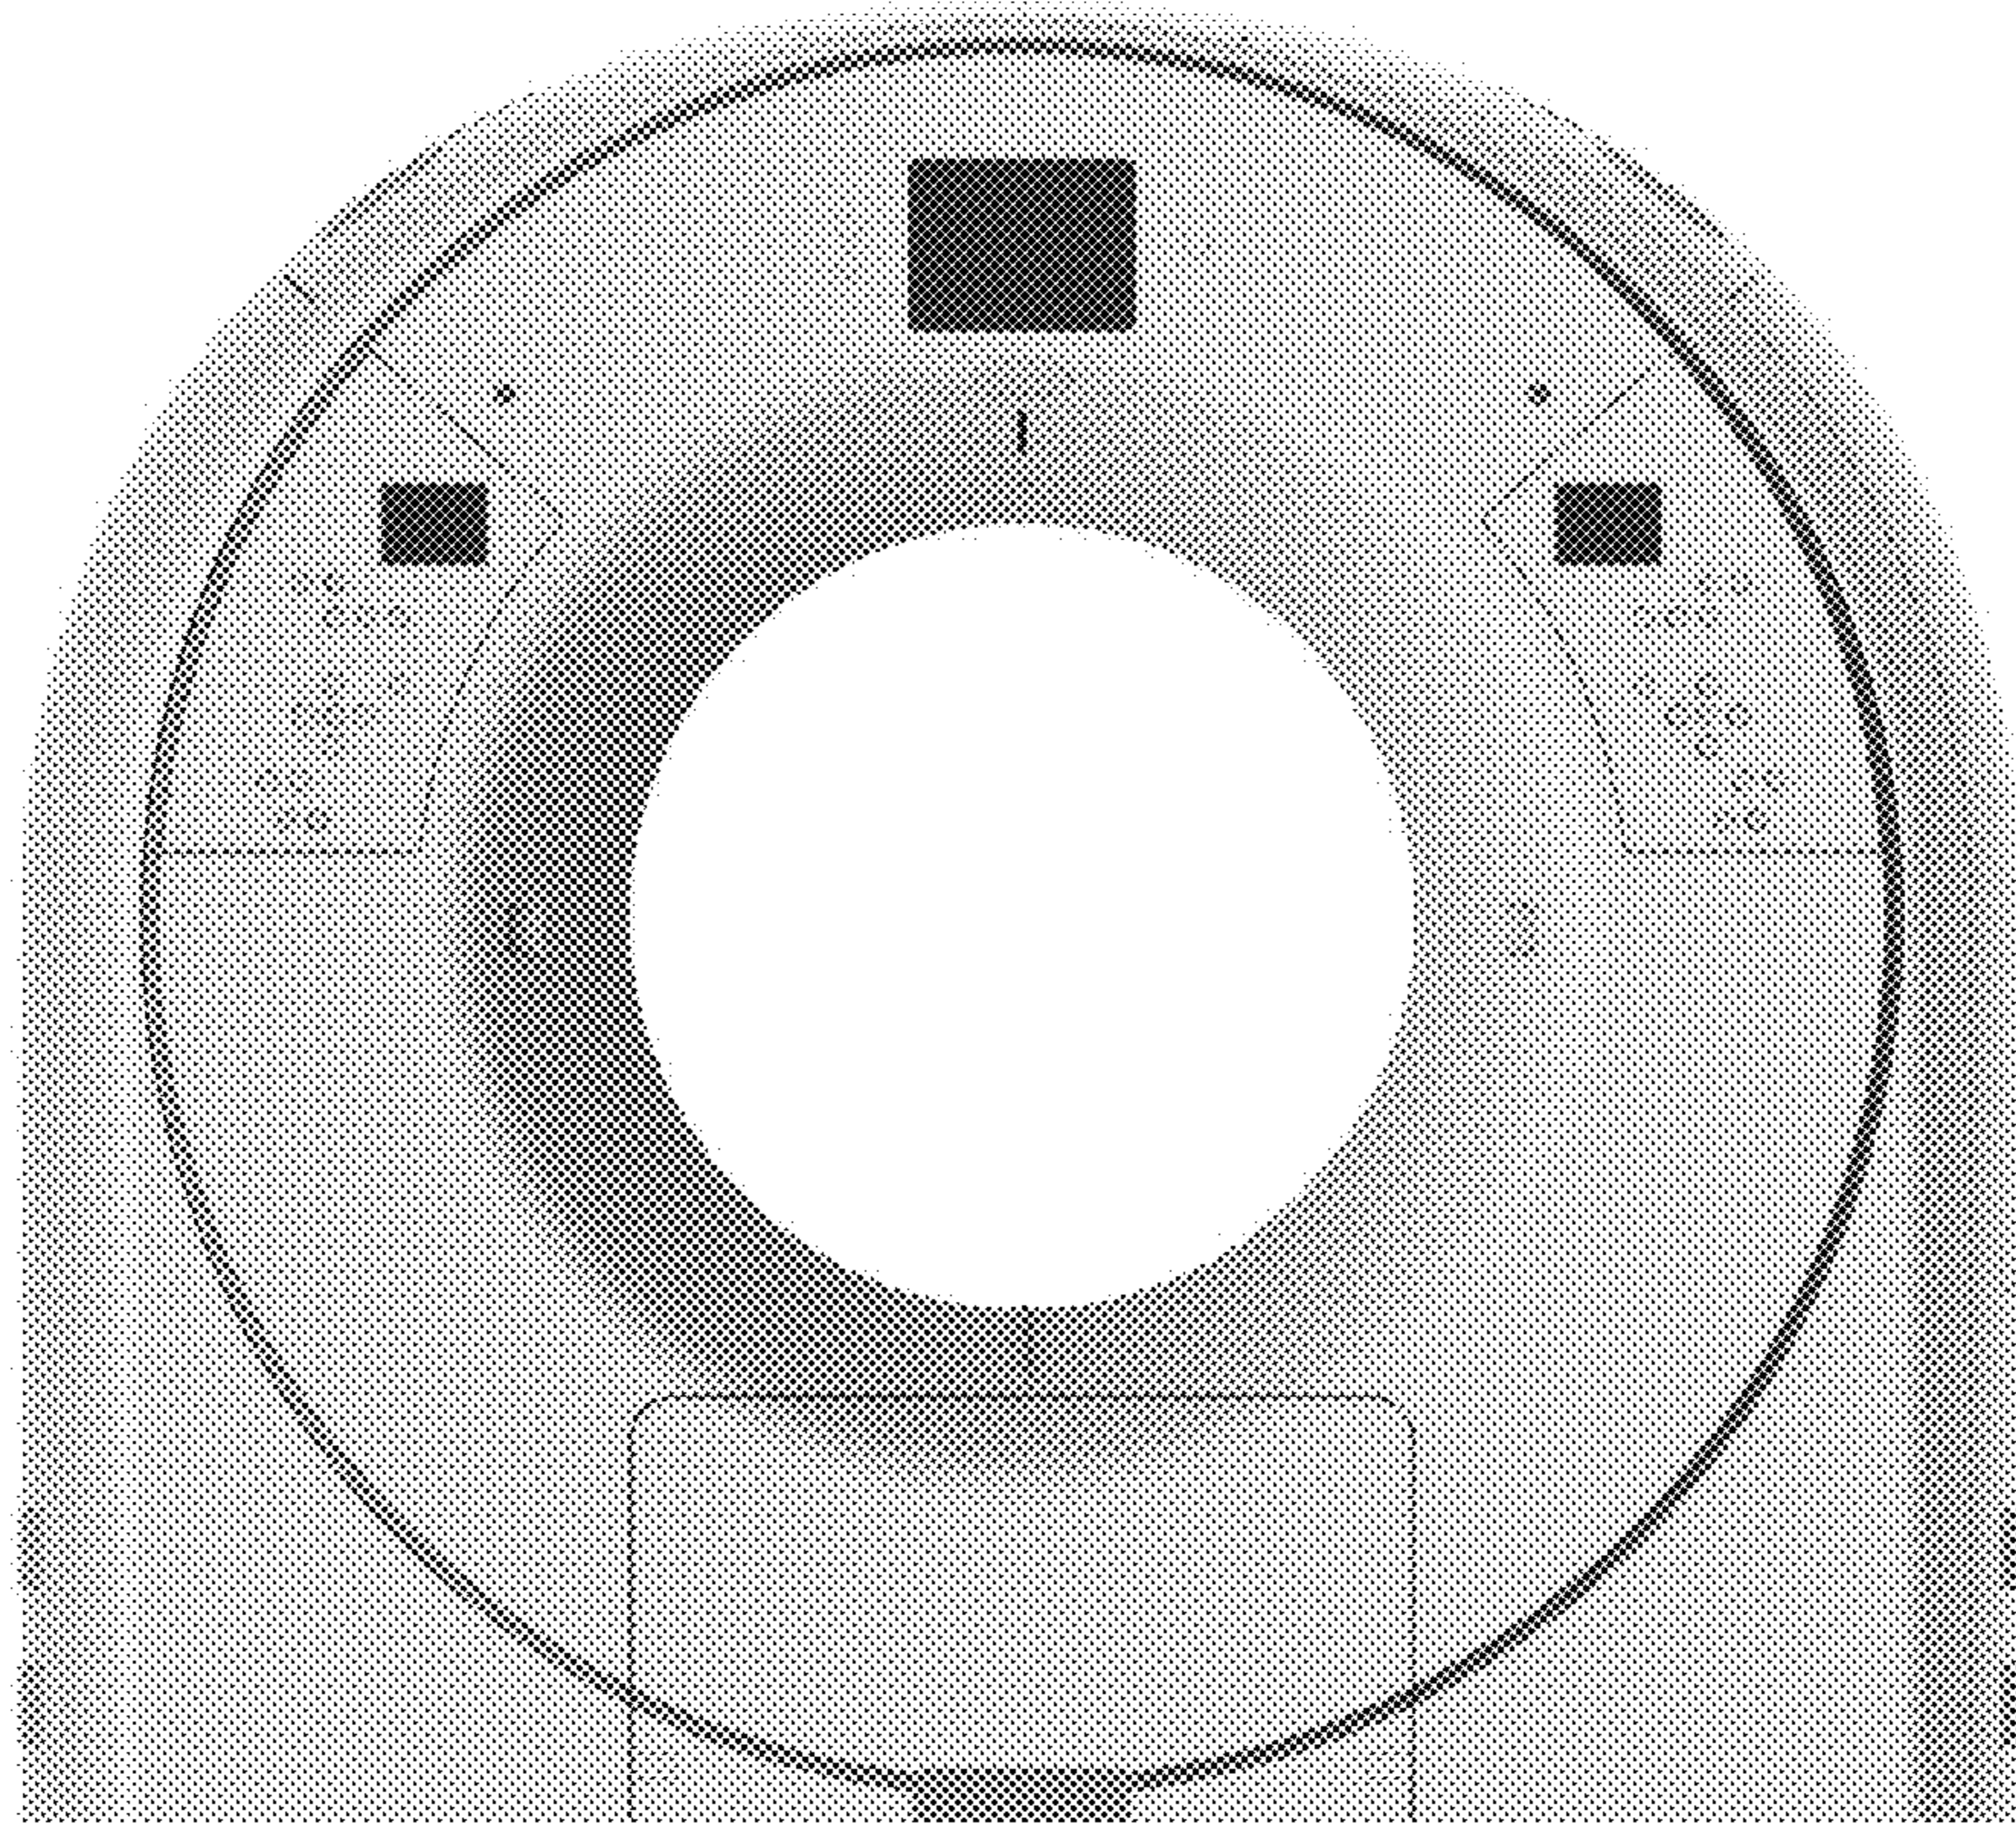


FIG.2

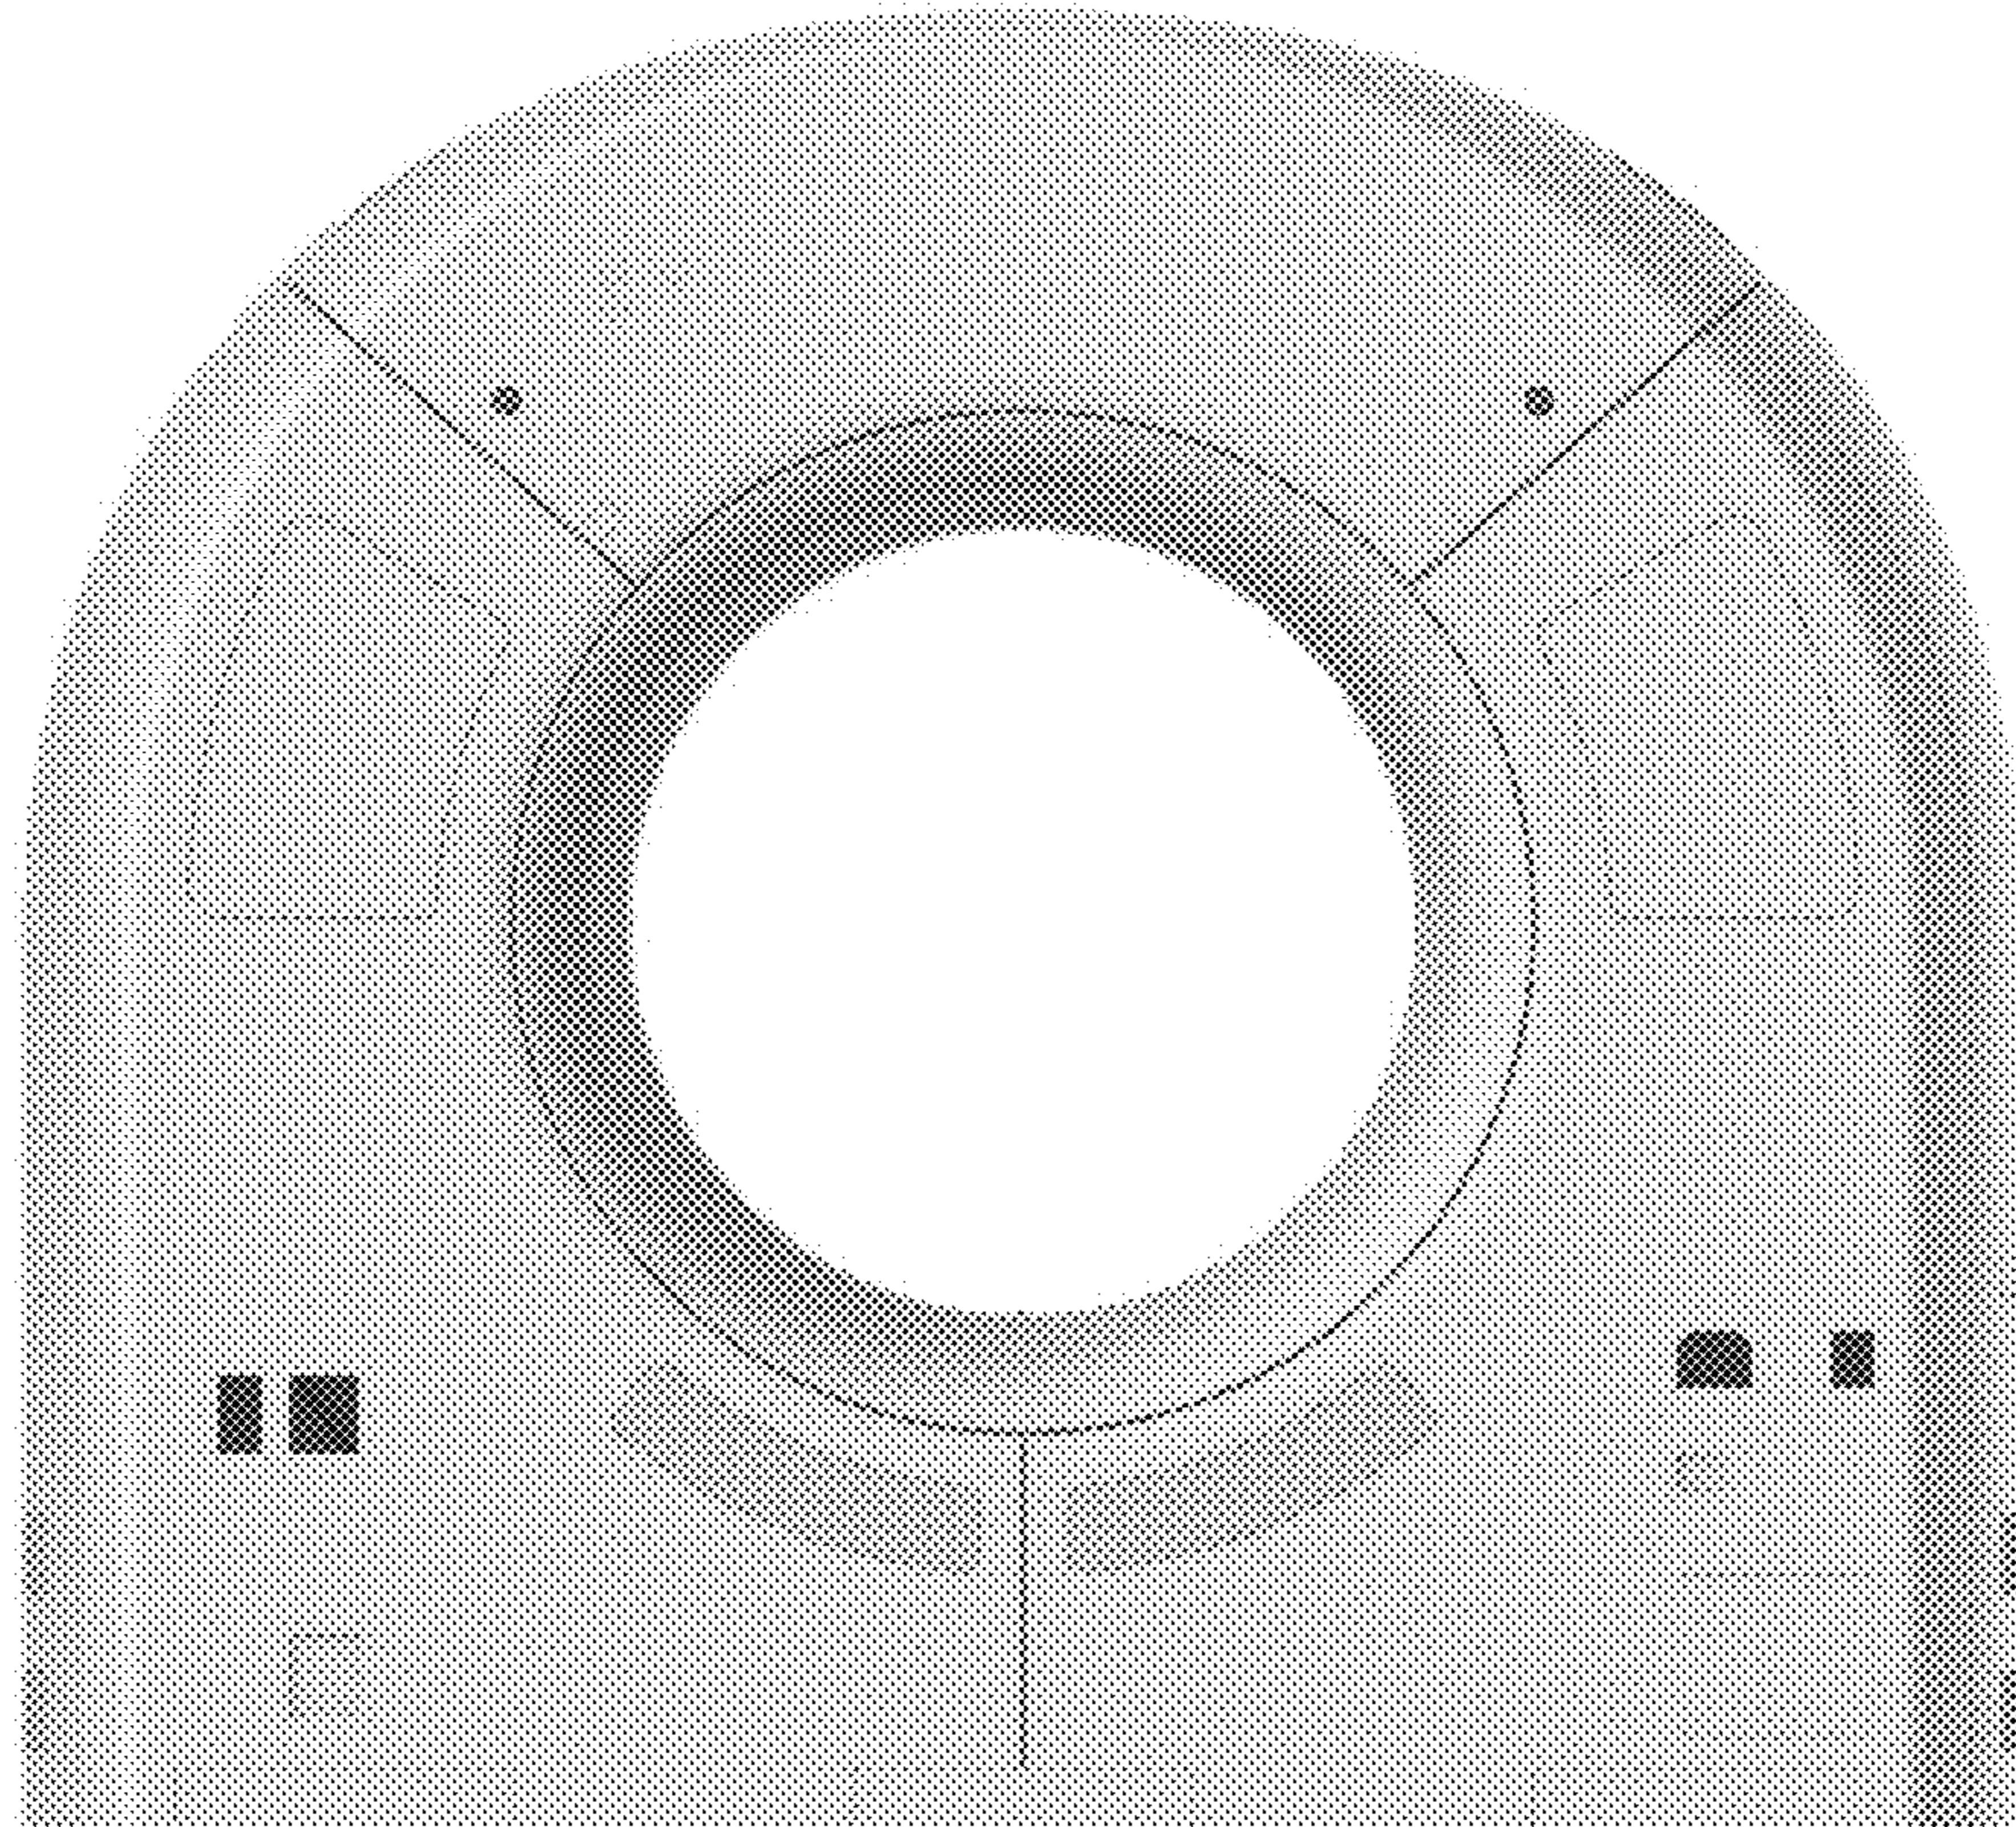


FIG.3

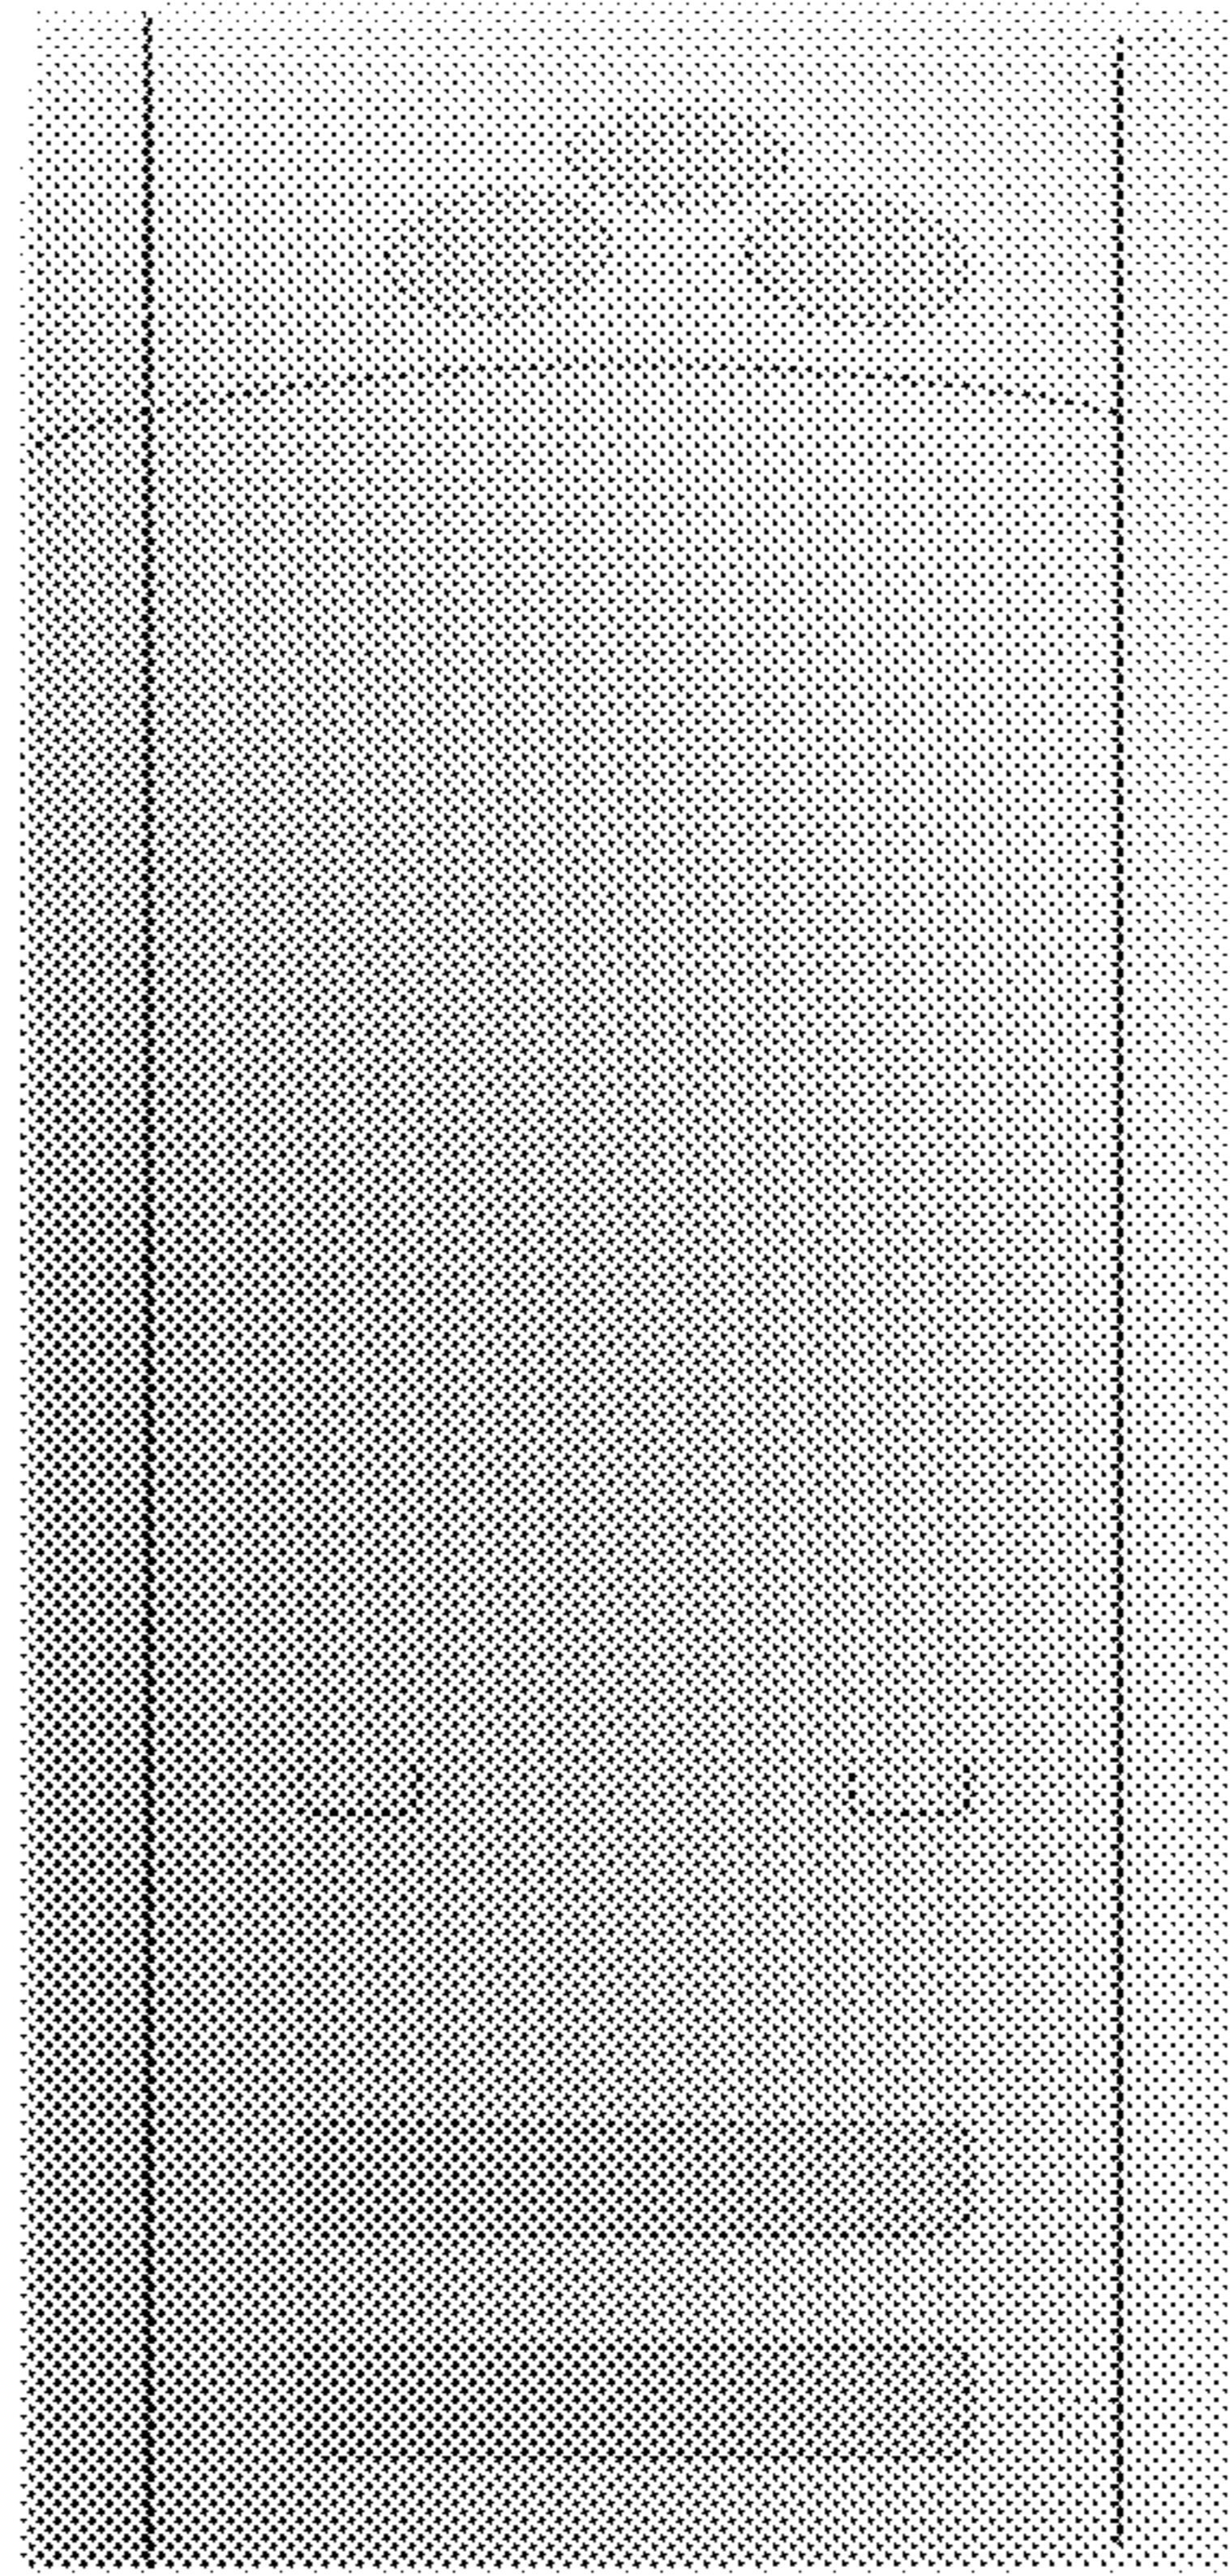


FIG.4

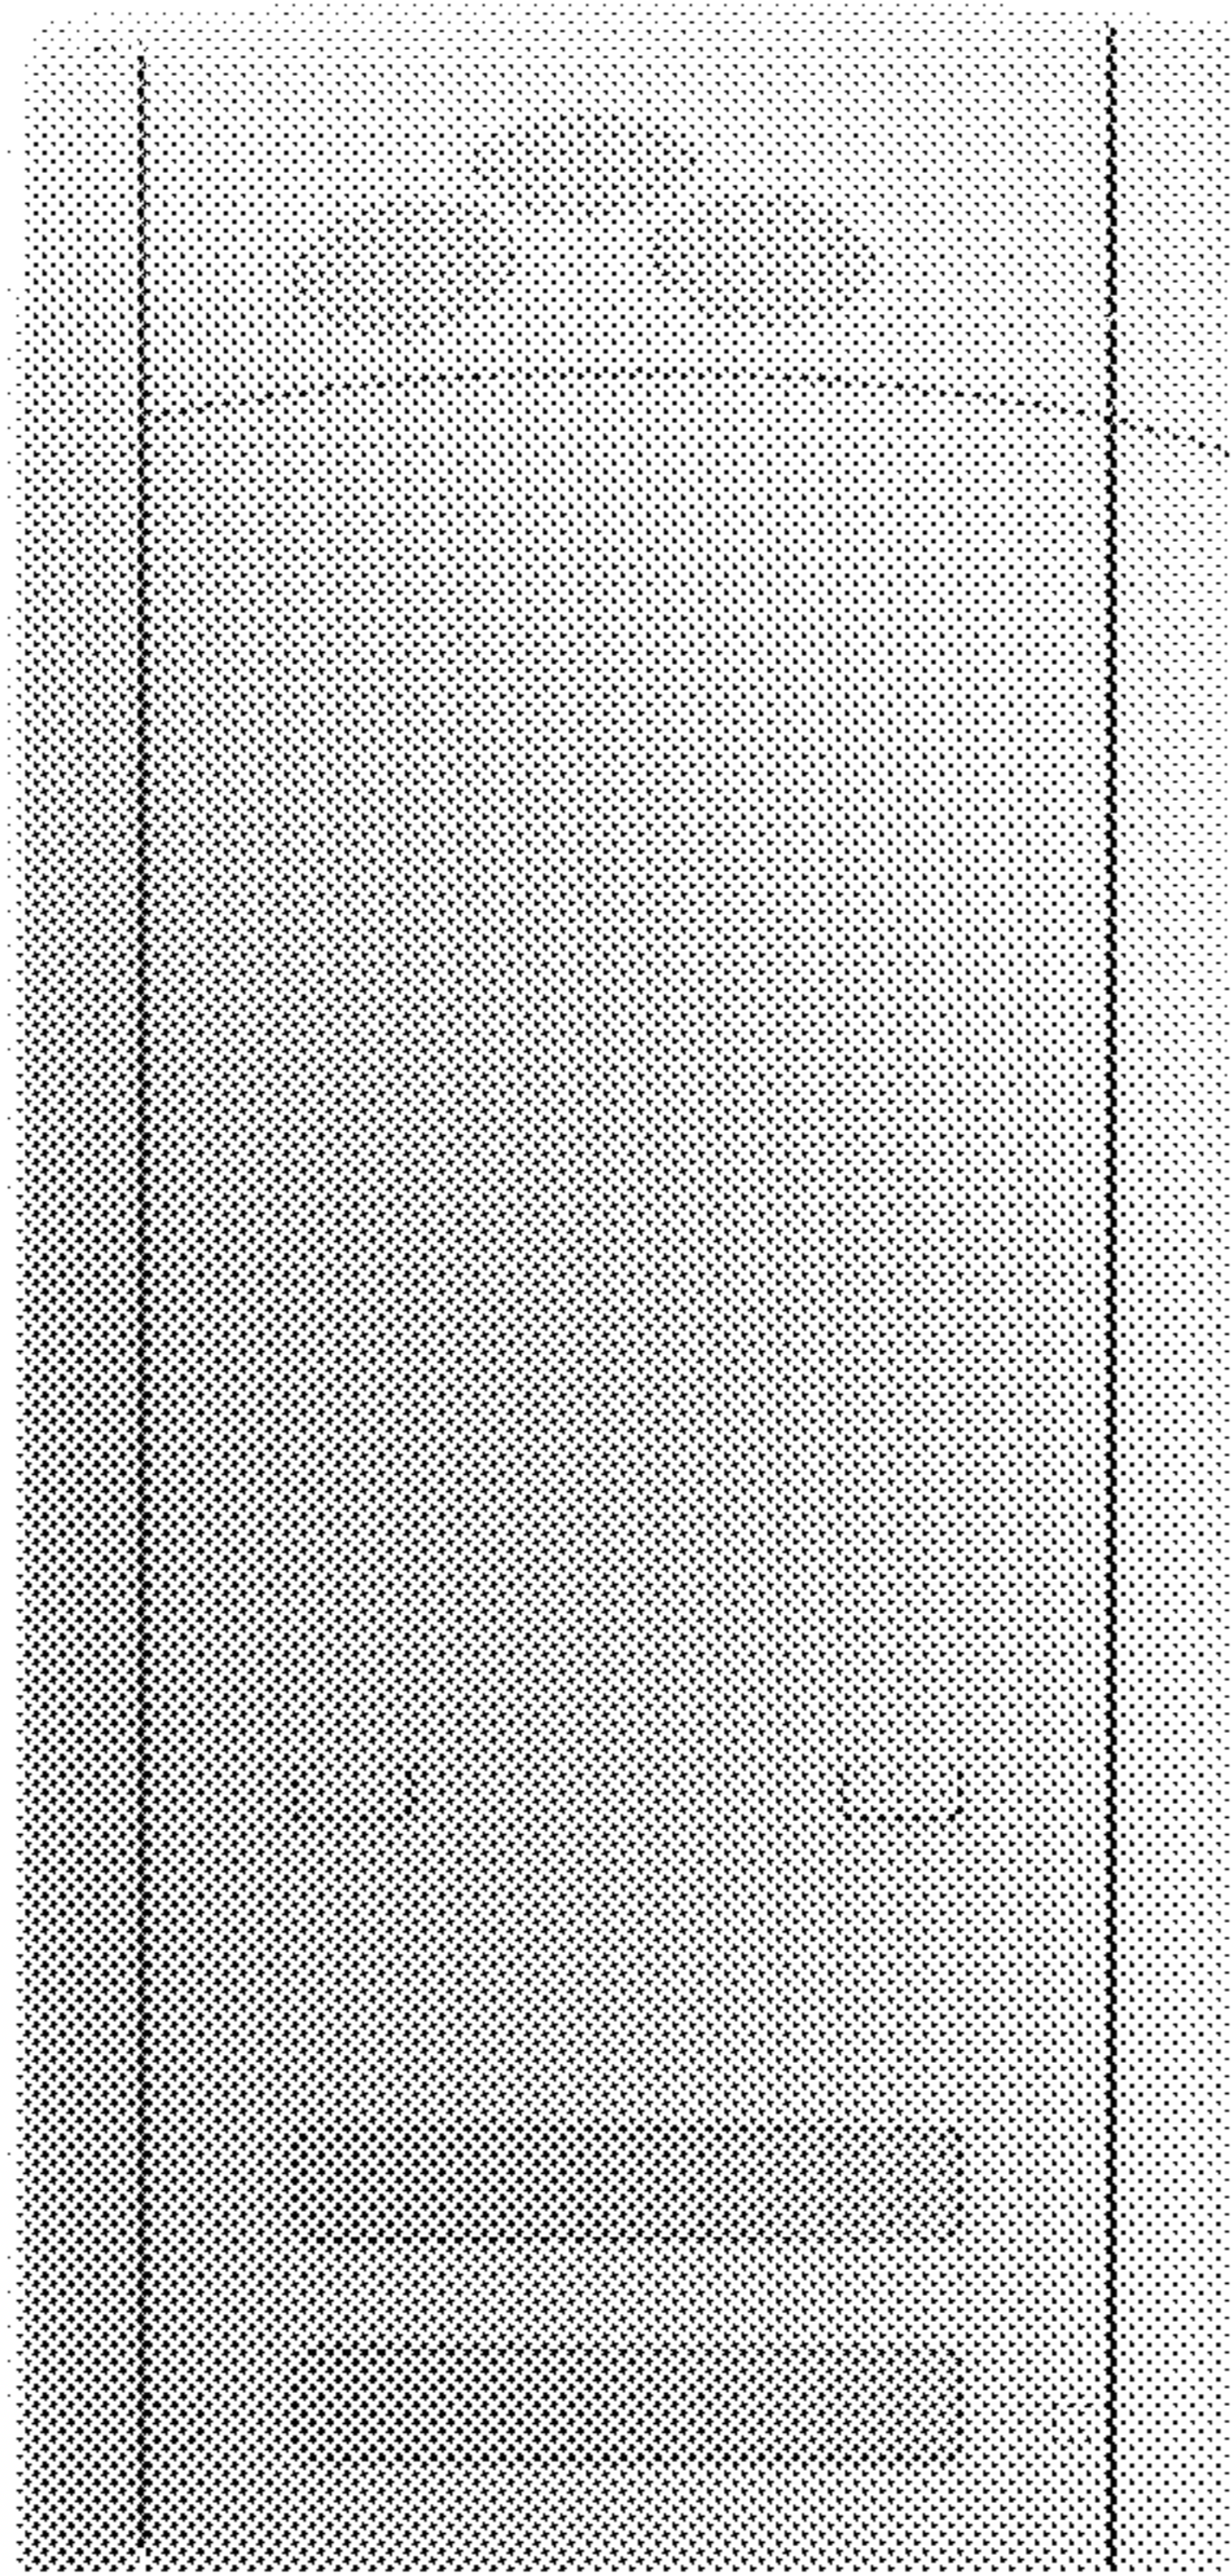


FIG.5

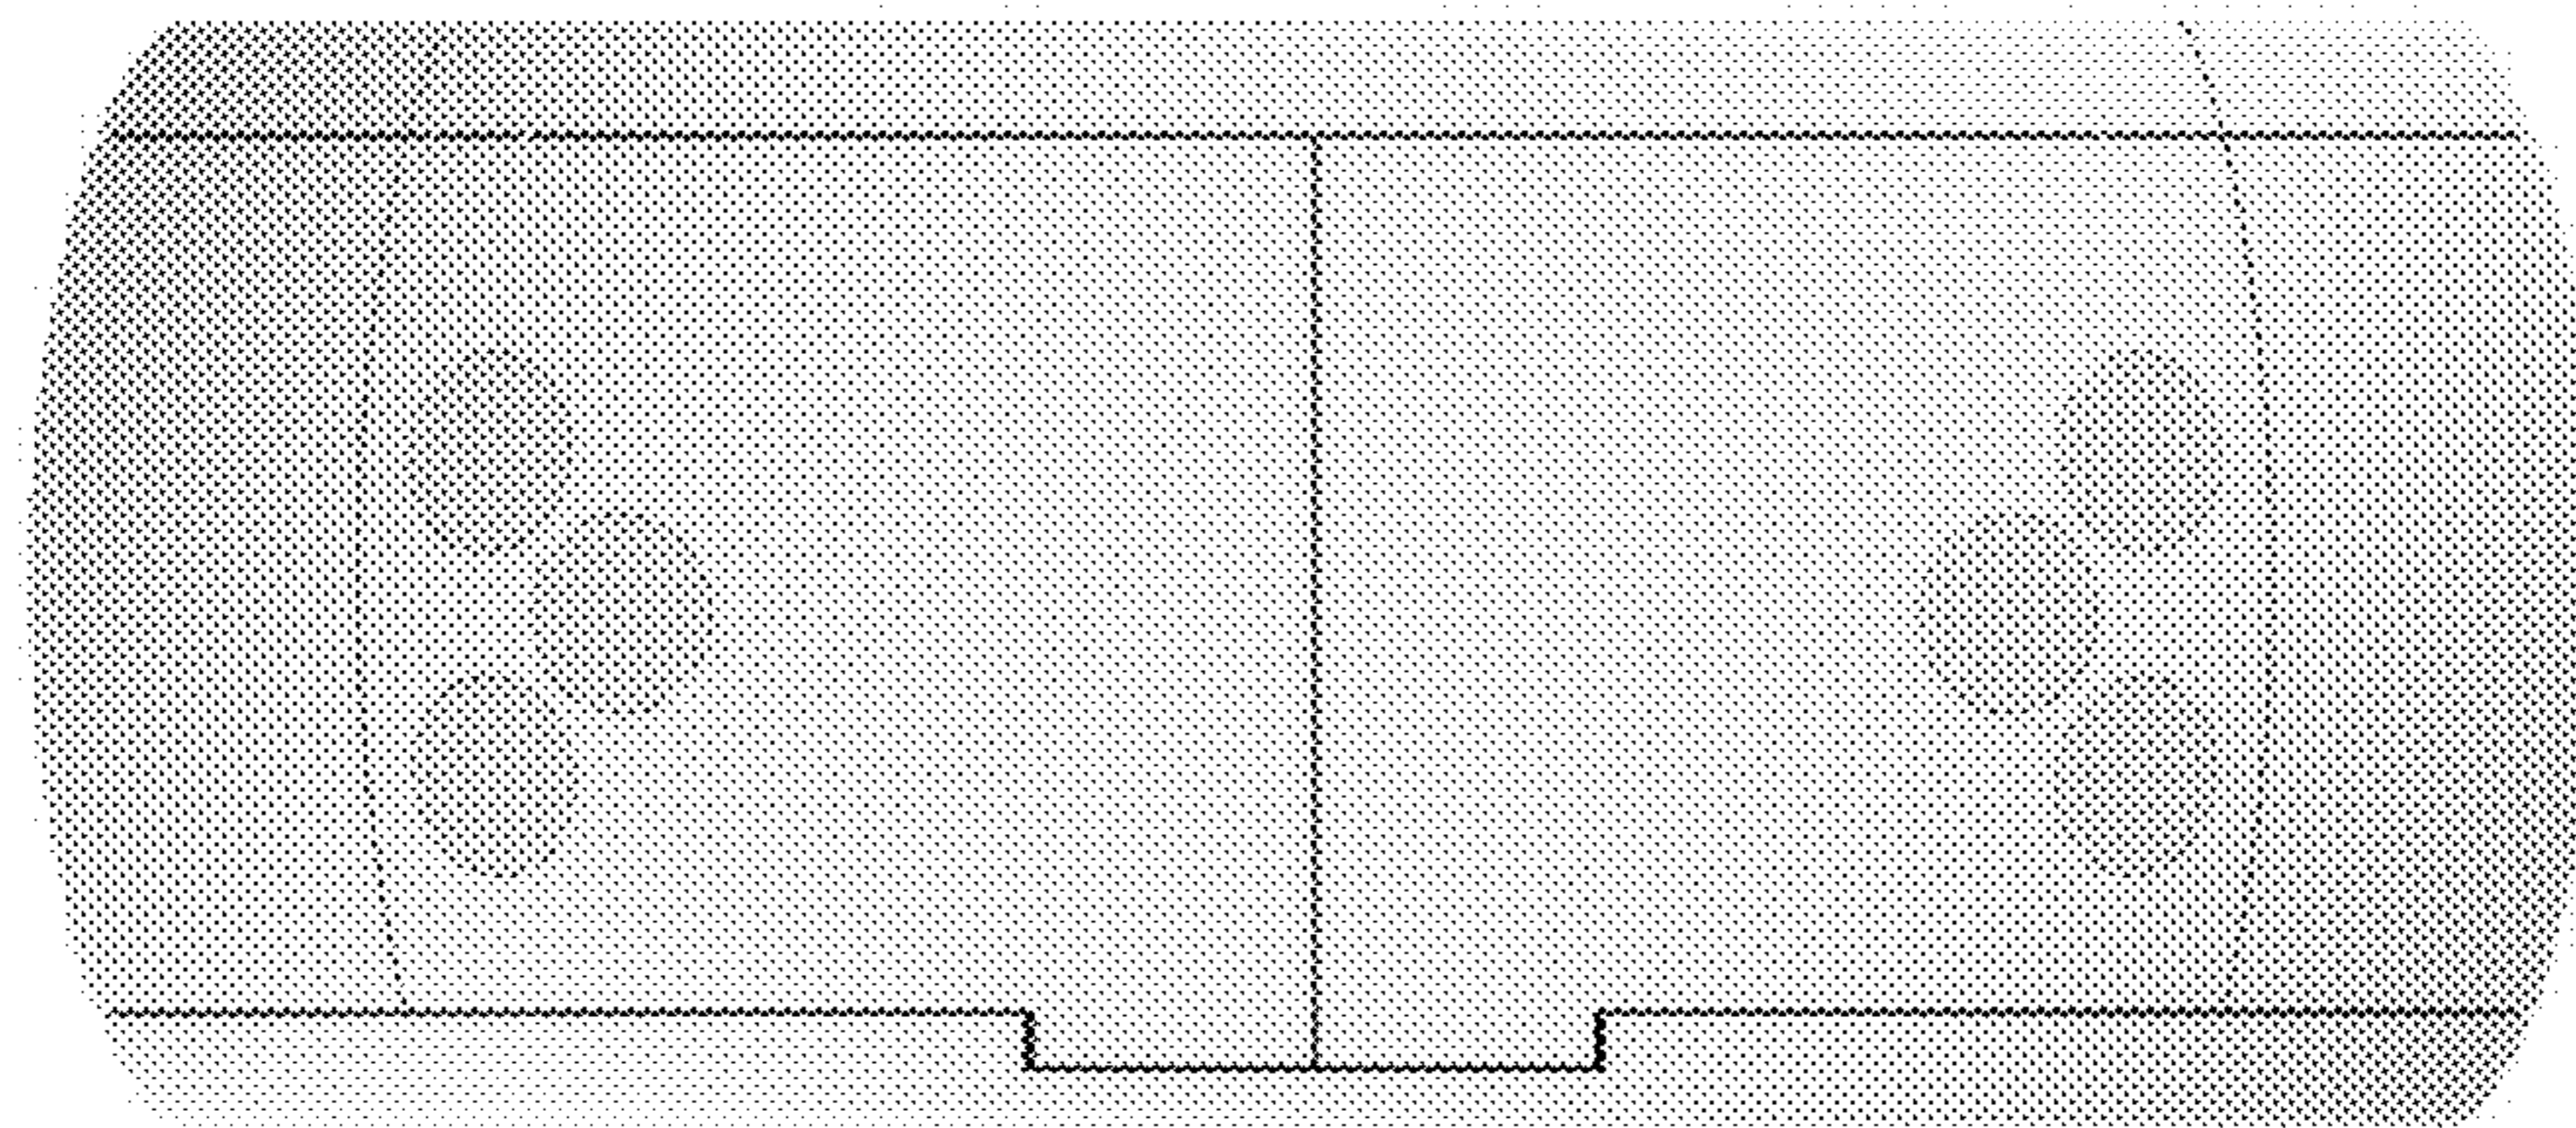


FIG. 6

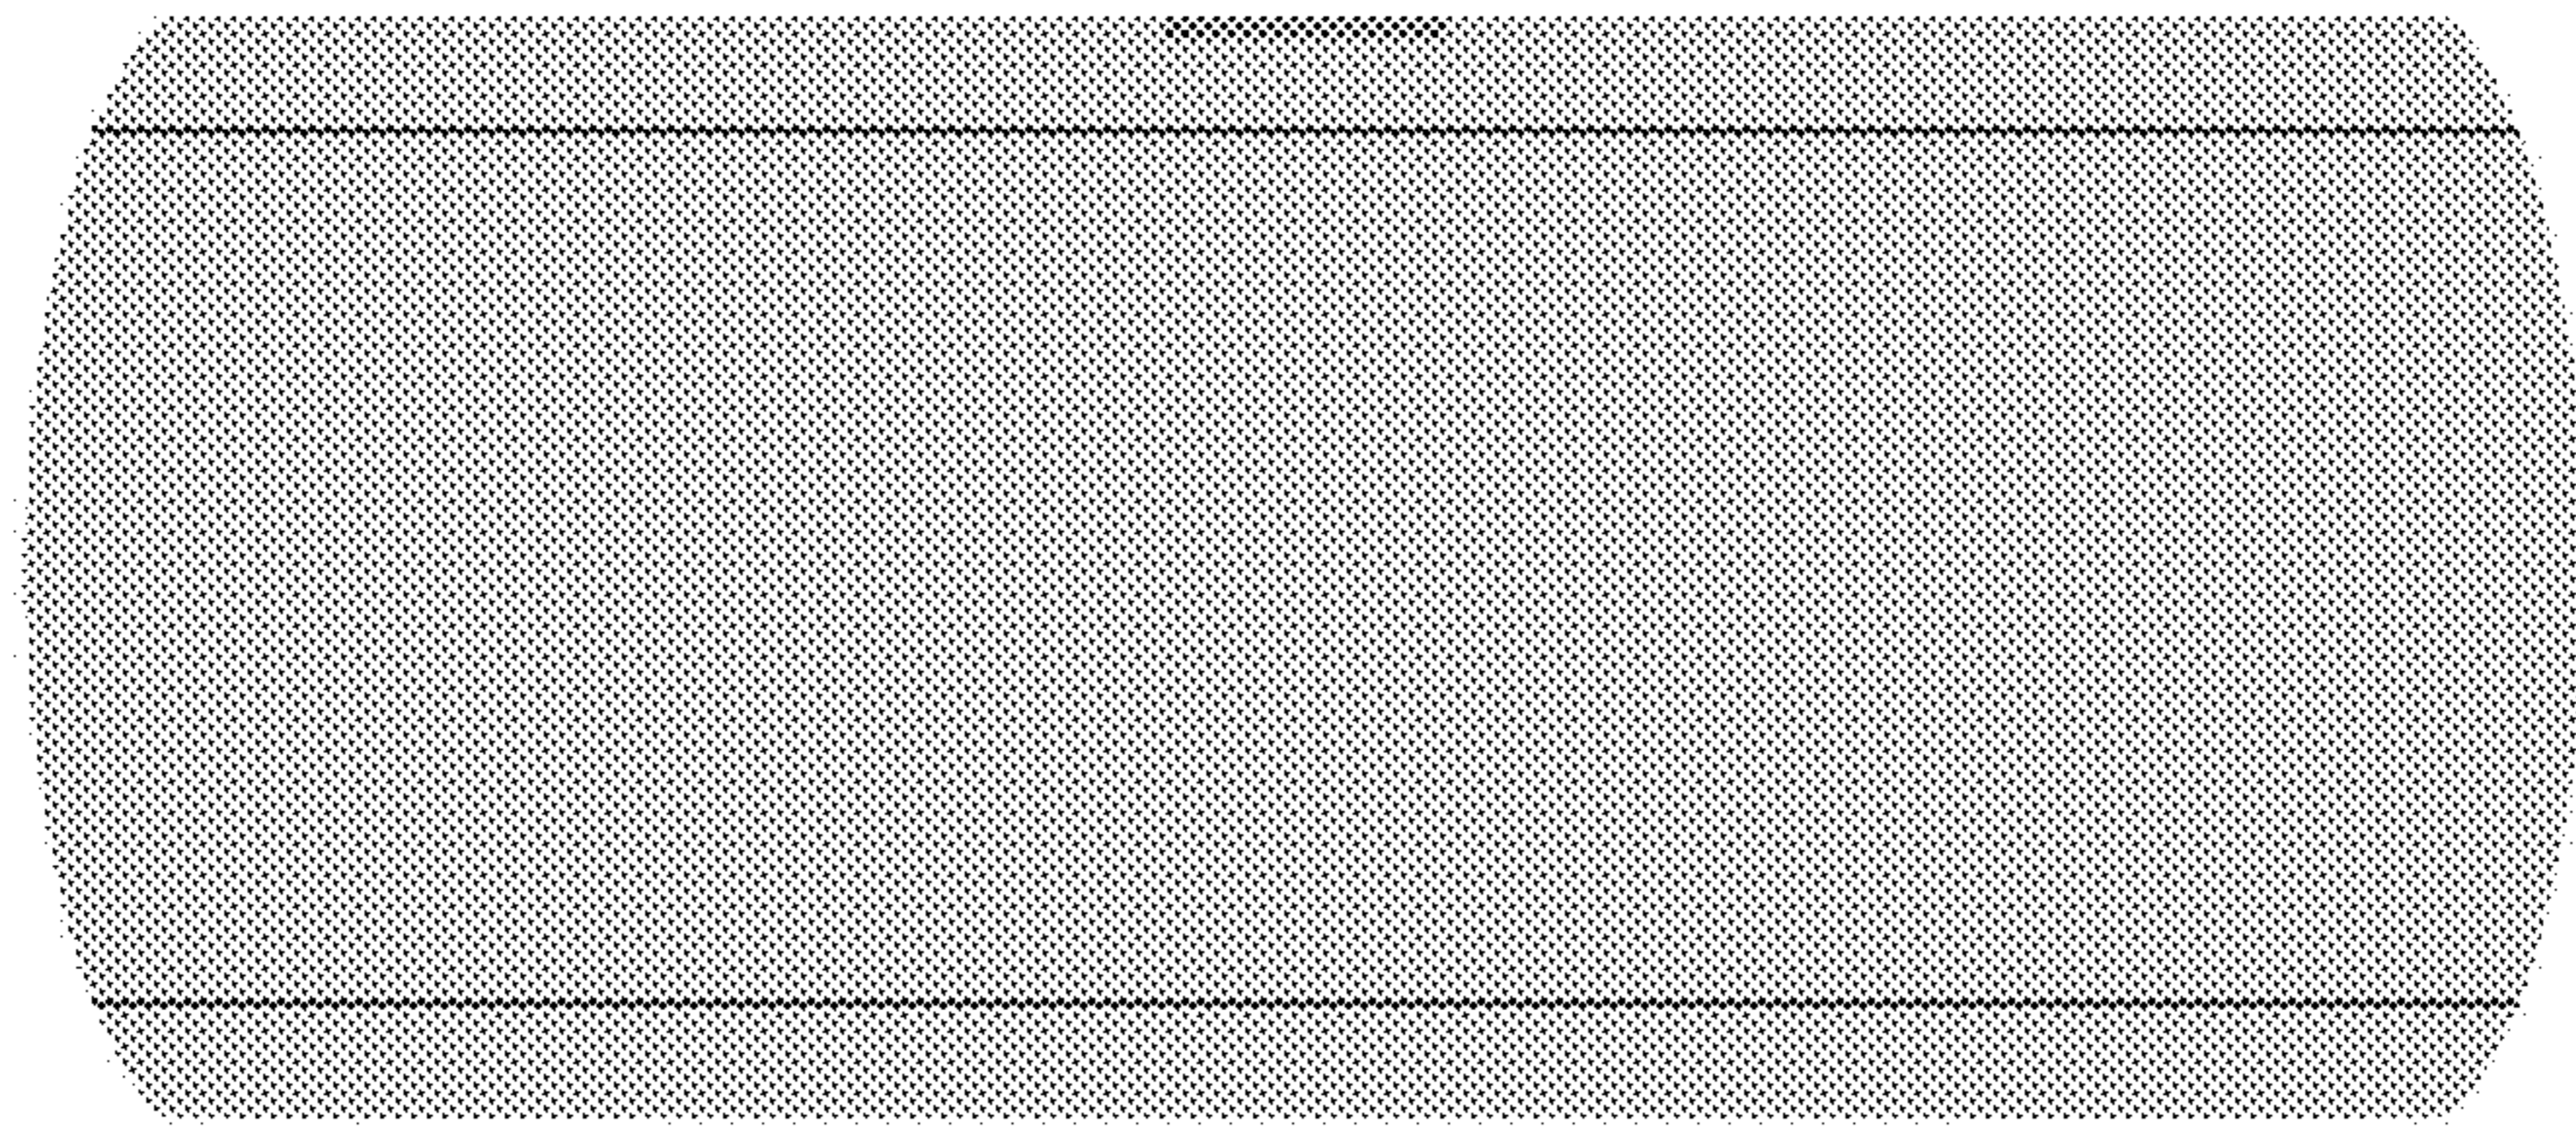


FIG.7



UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : D961,774 S  
APPLICATION NO. : 29/758284  
DATED : August 23, 2022  
INVENTOR(S) : Tetsuya Sekine et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

Item (30) The following Foreign Priority section should be added as:

(30) Foreign Application Priority Data  
August 5, 2020 (JP) .....2020-016385 D

Signed and Sealed this  
First Day of October, 2024  
*Katherine Kelly Vidal*

Katherine Kelly Vidal  
*Director of the United States Patent and Trademark Office*