

US00D962448S

(12) United States Design Patent (10) Patent No.:

Corbett et al.

US D962,448 S

** Aug. 30, 2022 (45) **Date of Patent:**

WEARABLE ULTRASOUND PROBE

Applicant: Sonivate Medical, Inc., Portland, OR

(US)

Inventors: **Scott Corbett**, Portland, OR (US);

Austen Angell, Portland, OR (US); Brion Benninger, Portland, OR (US); James T. Hatlan, Portland, OR (US)

Assignee: Sonivate Medical, Inc., Portland, OR

(US)

- 15 Years Term:
- Appl. No.: 29/731,547
- (22)Apr. 16, 2020 Filed:
- (51)
- U.S. Cl. (52)

USPC **D24/187**

Field of Classification Search (58)

USPC D24/133, 137, 138, 141, 158, 160, 164, D24/165, 167, 170, 186, 187, 200;

D10/57, 60, 78, 80

CPC ... A61B 5/0095; A61B 8/4444; A61B 8/4455; A61B 8/445; A61B 19/5244; A61B

8/485; A61B 8/0825; A61B 8/0875; A61B 8/481; A61B 5/02438; G01S 7/5208; G01N 29/265

See application file for complete search history.

(56)**References Cited**

U.S. PATENT DOCUMENTS

D743,040 S	*	11/2015	Corbett, III	D24/187
D745,687 S	*	12/2015	Kitayama	D24/187
			Vezina	
D787,685 S	*	5/2017	Vezina	D24/187
D870.884 S	*	12/2019	Huels	D24/137

				Wirth D24/138
D934,431	S	*	10/2021	Tsuruoka D24/186
D934,438	S	*	10/2021	deBock
2018/0235441	Al	*	8/2018	Huang A61B 1/00142
2019/0254627	Al	*	8/2019	Corbett A61B 8/467
2019/0357883	A 1	*	11/2019	Steinberg A61B 1/0051

FOREIGN PATENT DOCUMENTS

JP D2020-2756 * 10/2021

OTHER PUBLICATIONS

Intraoperative ultrasound during a laparoscopic myomectomy. Online, published date Jun. 1, 2004. Retrieved on Nov. 7, 2021 from URL: https://www.fertstert.org/article/S0015-0282(04)00347-4/fulltext.* SonicEye® Dual-Array Portable System. Online, published date unknown. Retrieved on Nov. 7, 2021 from URL: https://sonivate. com/soniceye-dual-array/.*

* cited by examiner

Primary Examiner — Omeed Agilee

(74) Attorney, Agent, or Firm — K&L Gates LLP

(57)CLAIM


We claim the ornamental design for a wearable ultrasound probe, as shown and described.

DESCRIPTION


- FIG. 1 is a perspective view of a wearable ultrasound probe;
- FIG. 2 is a bottom view thereof;
- FIG. 3 is a top view thereof;
- FIG. 4 is a right side view thereof;
- FIG. 5 is a left side view thereof;
- FIG. 6 is a top plan view thereof; and,
- FIG. 7 is a bottom plan view thereof.


The broken lines in the drawings depict portions of the wearable ultrasound probe that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

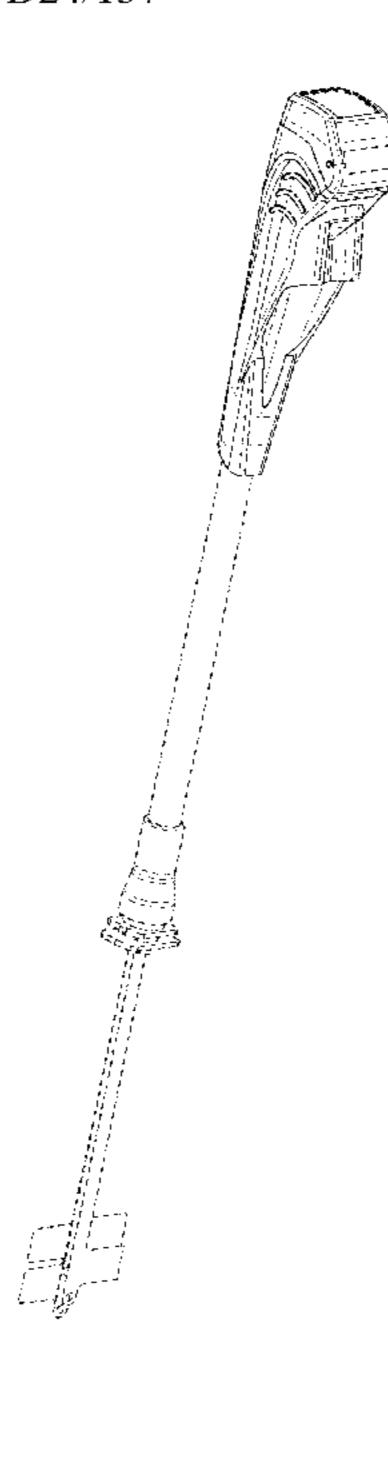

Aug. 30, 2022

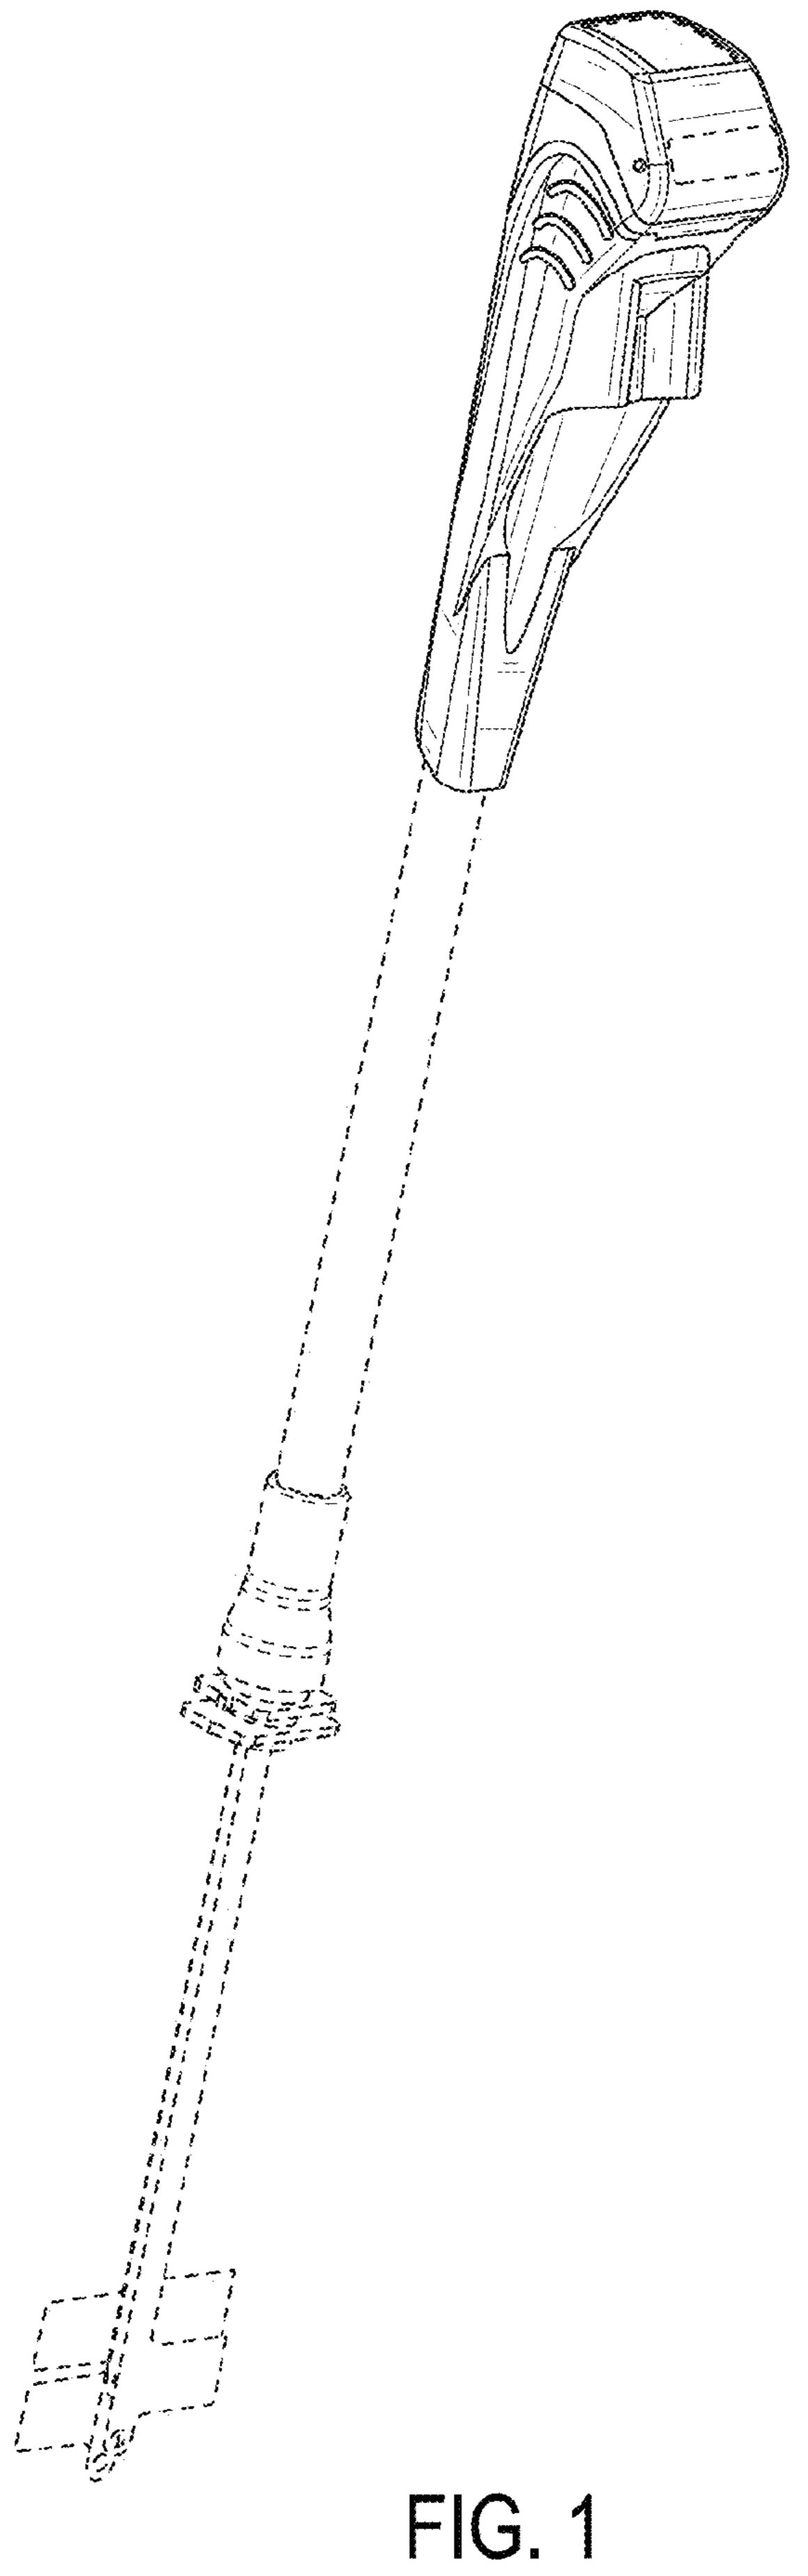

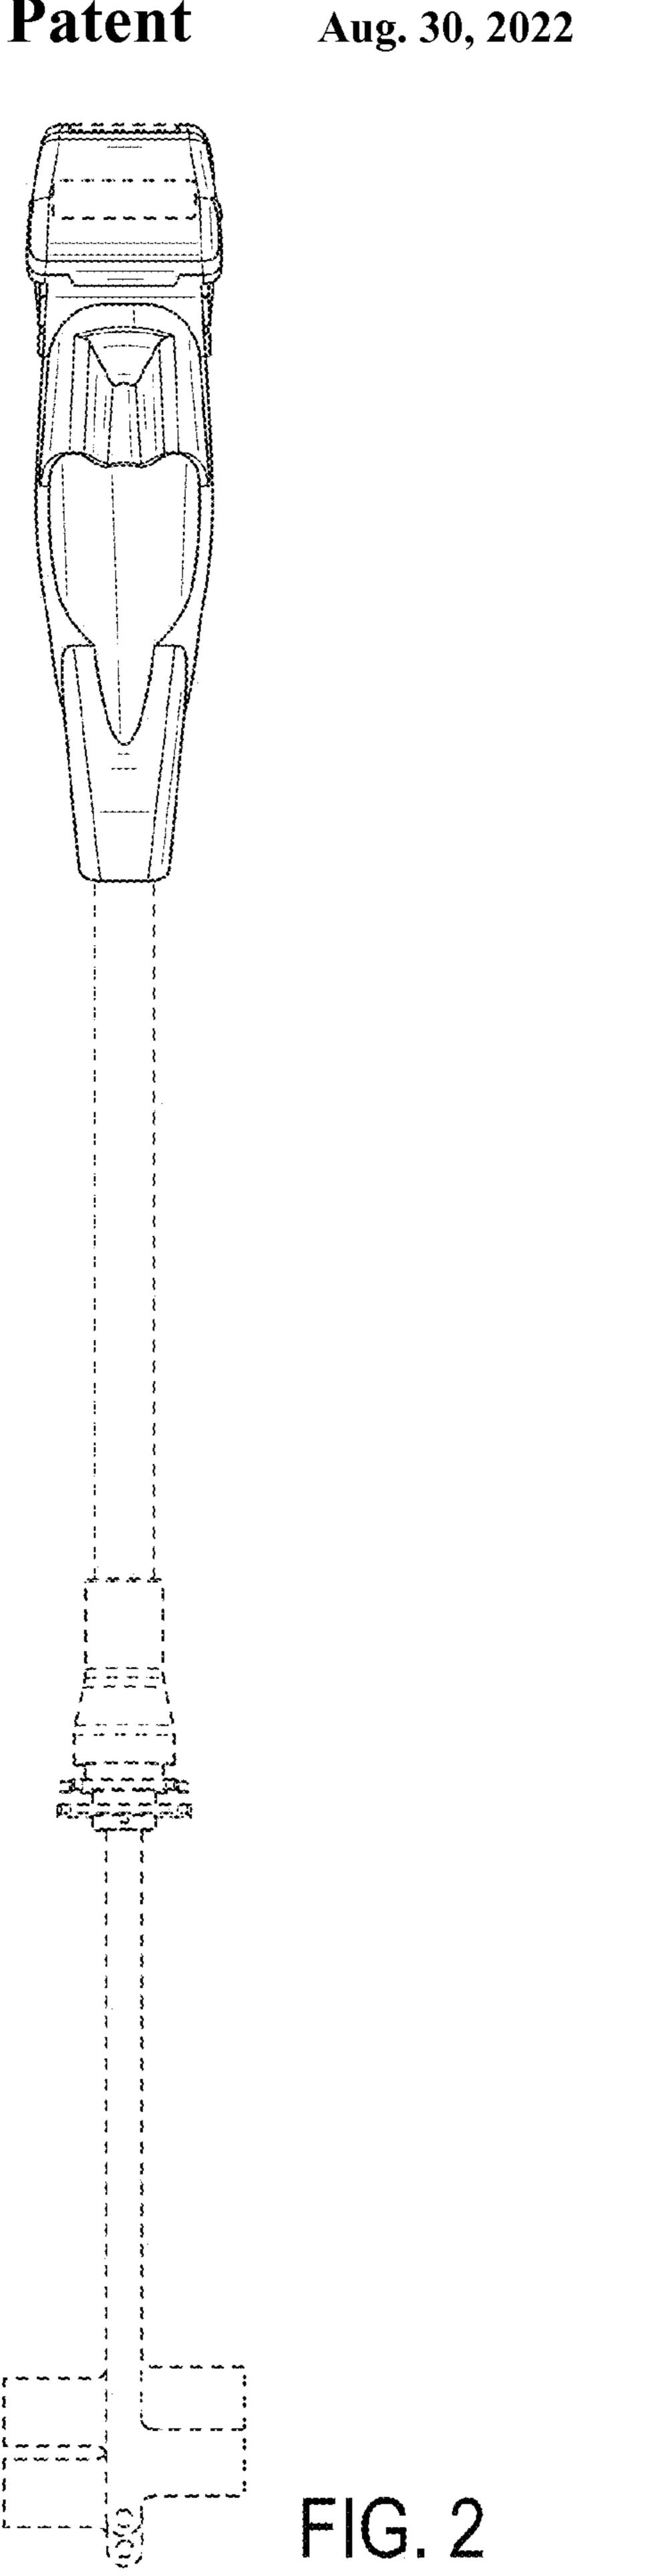

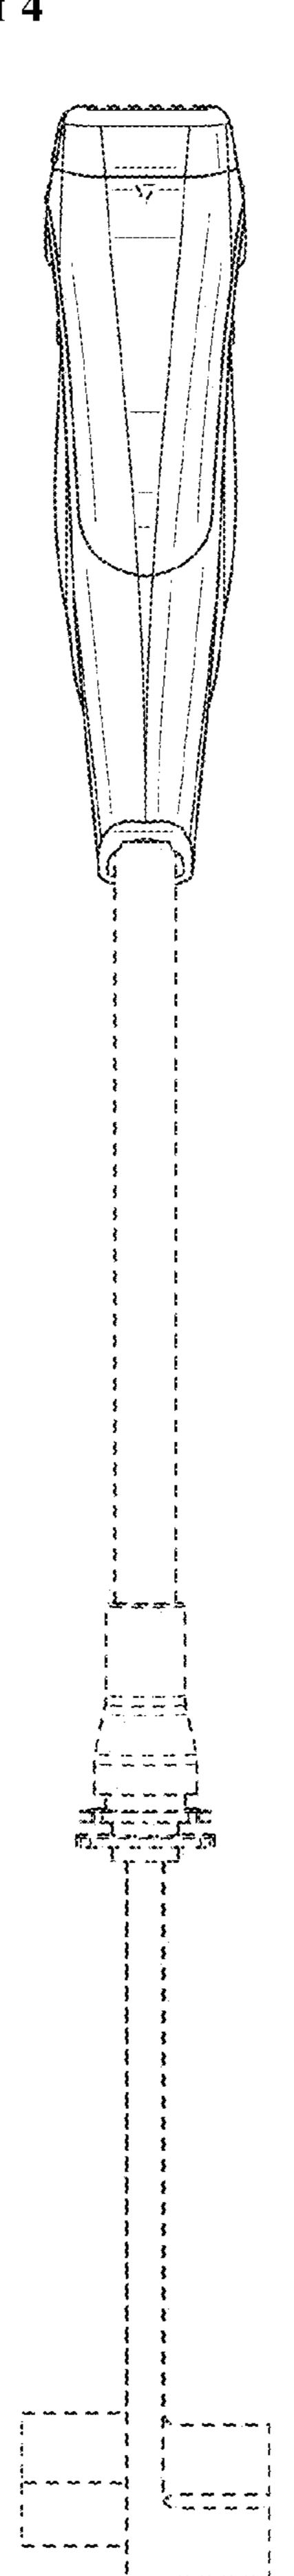
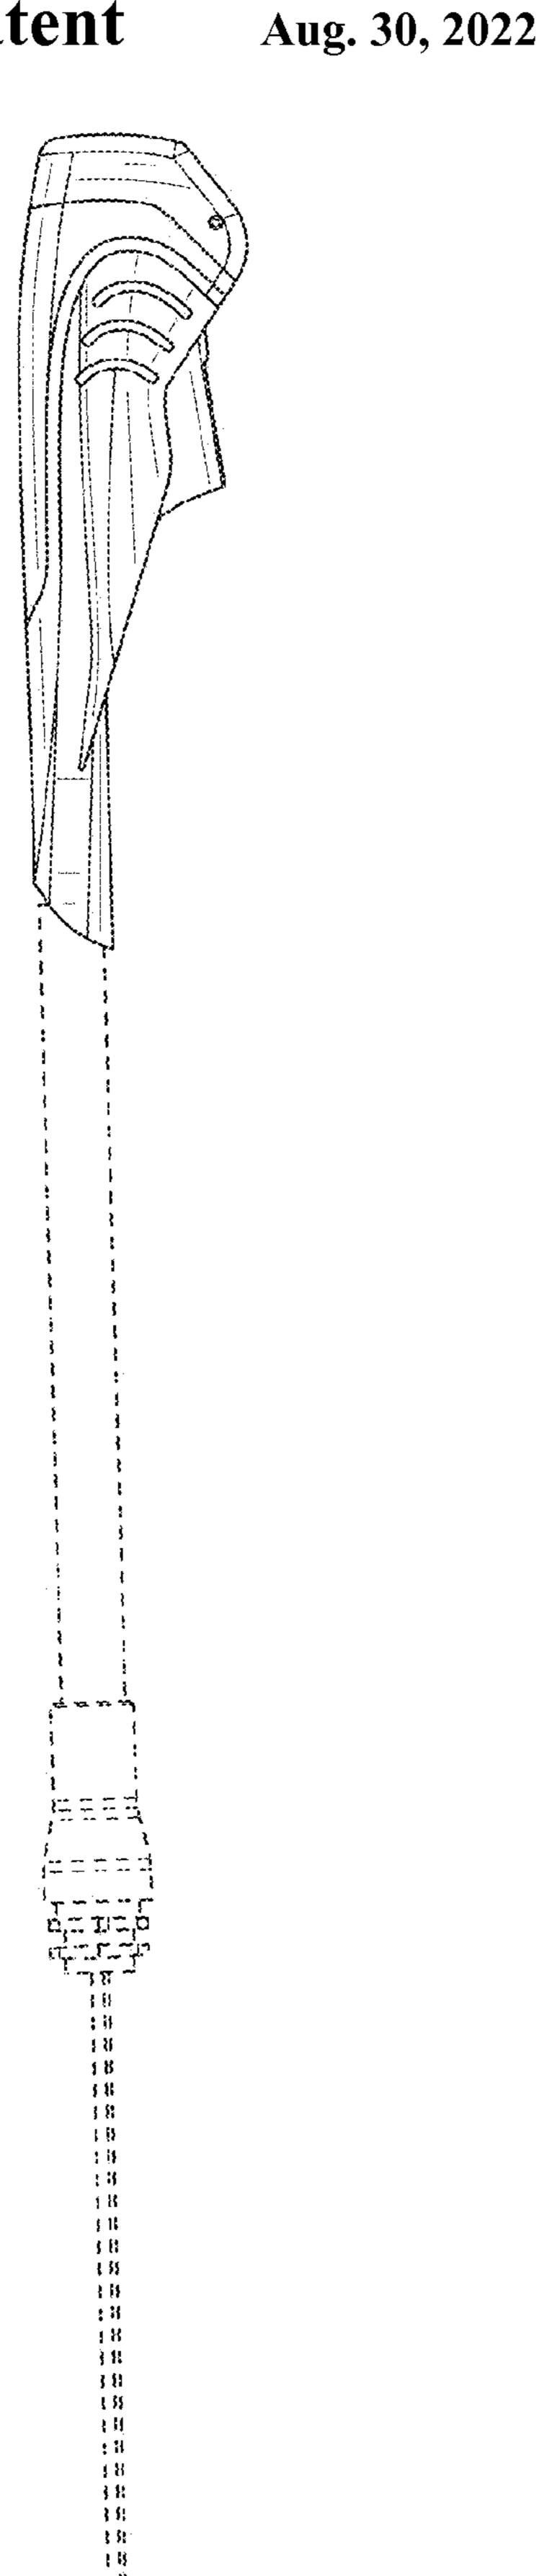


FIG. 3



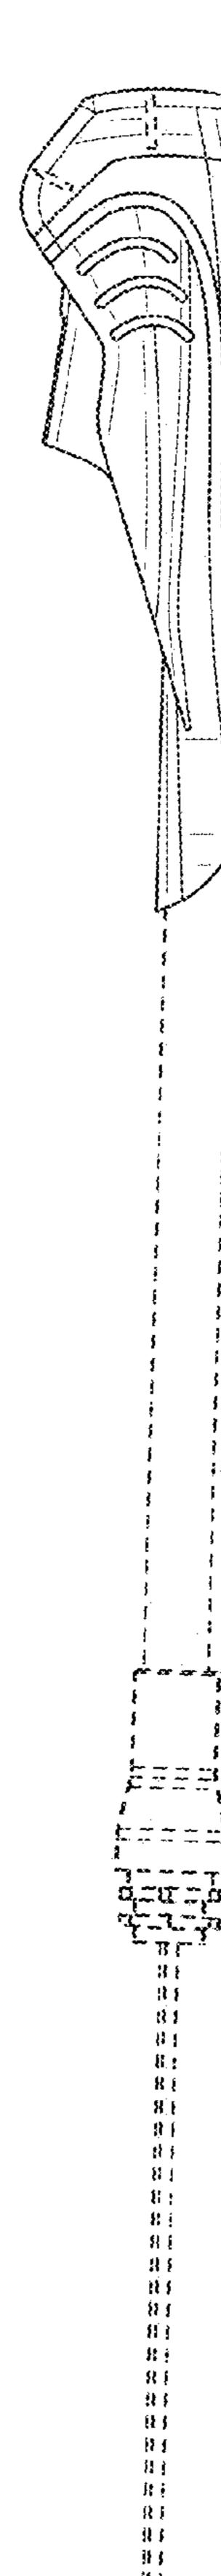


FIG. 4

FIG. 5

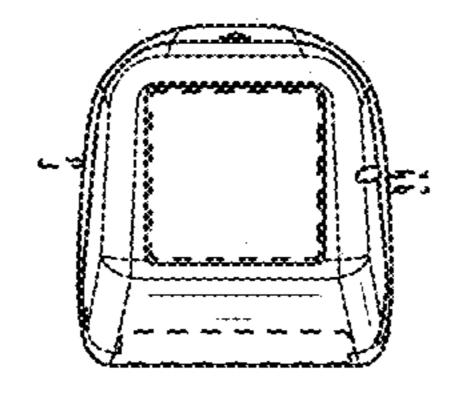


FIG. 6

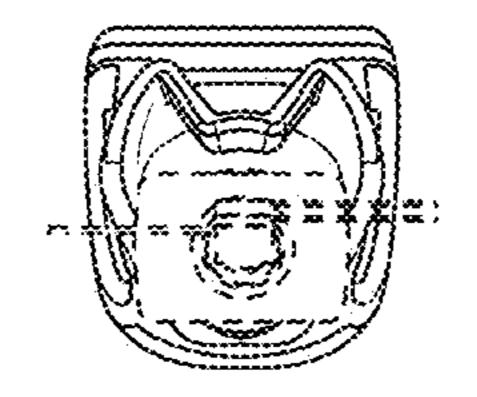


FIG. 7

UNITED STATES PATENT AND TRADEMARK OFFICE CERTIFICATE OF CORRECTION

PATENT NO. : D962,448 S

APPLICATION NO. : 29/731547

DATED : August 30, 2022 INVENTOR(S) : Scott Corbett et al.

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the Title Page

Add before item (57):

"GOVERNMENT SUPPORT ACKNOWLEDGEMENT

This invention was made with government support under contract number W81XWH-17-C-0024 awarded by The United States Army Medical Research and Material Command, and W81XWH-15-C-001 awarded by the Defense Health Program, United States Department of Defense. The government has certain rights in the invention."

Signed and Sealed this Sixteenth Day of September, 2025

Coke Morgan Stewart

Colu-Mon-Shud-

Acting Director of the United States Patent and Trademark Office