



US00D963167S

(12) **United States Design Patent** (10) **Patent No.:** **US D963,167 S**
Young (45) **Date of Patent:** **** Sep. 6, 2022**

(54) **SIZE ADJUSTABLE DEVICE TO COVER AND SECURE IMPLANTABLE DEVICES IN SURGICAL APPLICATIONS**

Primary Examiner — Charles D Hanson
(74) *Attorney, Agent, or Firm* — Goldstein Law Offices, P.C.

(71) Applicant: **Anke Young**, New Canaan, CT (US)

(57) **CLAIM**

(72) Inventor: **Anke Young**, New Canaan, CT (US)

The ornamental design for a size adjustable device to cover and secure implantable devices in surgical applications, as shown and described.

(**) Term: **15 Years**

DESCRIPTION

(21) Appl. No.: **29/698,609**

FIG. 1 is a perspective view of a first embodiment of the size adjustable device to cover and secure implantable devices in surgical applications.

(22) Filed: **Jul. 18, 2019**

FIG. 2 is a top plan view of the size adjustable device to cover and secure implantable devices in surgical applications.

(51) **LOC (13) Cl.** **24-03**

(52) **U.S. Cl.**
USPC **D24/155**

FIG. 3 is a bottom plan view thereof.

(58) **Field of Classification Search**
USPC D24/155

CPC A61F 2/07; A61F 2/90; A61F 2/958; A61F 2002/016; A61F 2002/072; A61F 2002/075; A61F 2002/91541; A61F 2220/0075; A61F 2230/0069

FIG. 4 is a front elevational view thereof.

FIG. 5 is a rear elevational view thereof.

FIG. 6 is a right side elevational view thereof.

FIG. 7 is a left side elevational view thereof.

See application file for complete search history.

FIG. 8 is a perspective view of a second embodiment of the size adjustable device to cover and secure implantable devices in surgical applications.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D363,123 S *	10/1995	Morgan	D24/140
D363,546 S *	10/1995	Morgan	D10/104.1
D369,412 S *	4/1996	Morgan	D24/140
D388,877 S *	1/1998	Morgan	D24/155
D689,913 S *	9/2013	Fu	D15/126
D784,536 S *	4/2017	Freudenthal	D24/140
D794,210 S *	8/2017	Jarvis	D24/225

FIG. 9 is a top plan view of the second embodiment of the size adjustable device to cover and secure implantable devices in surgical applications.

FIG. 10 is a bottom plan view thereof.

FIG. 11 is a front elevational view thereof.


FIG. 12 is a rear elevational view thereof.

FIG. 13 is a right side elevational view thereof; and,

FIG. 14 is a left side elevational view thereof.

* cited by examiner

1 Claim, 10 Drawing Sheets

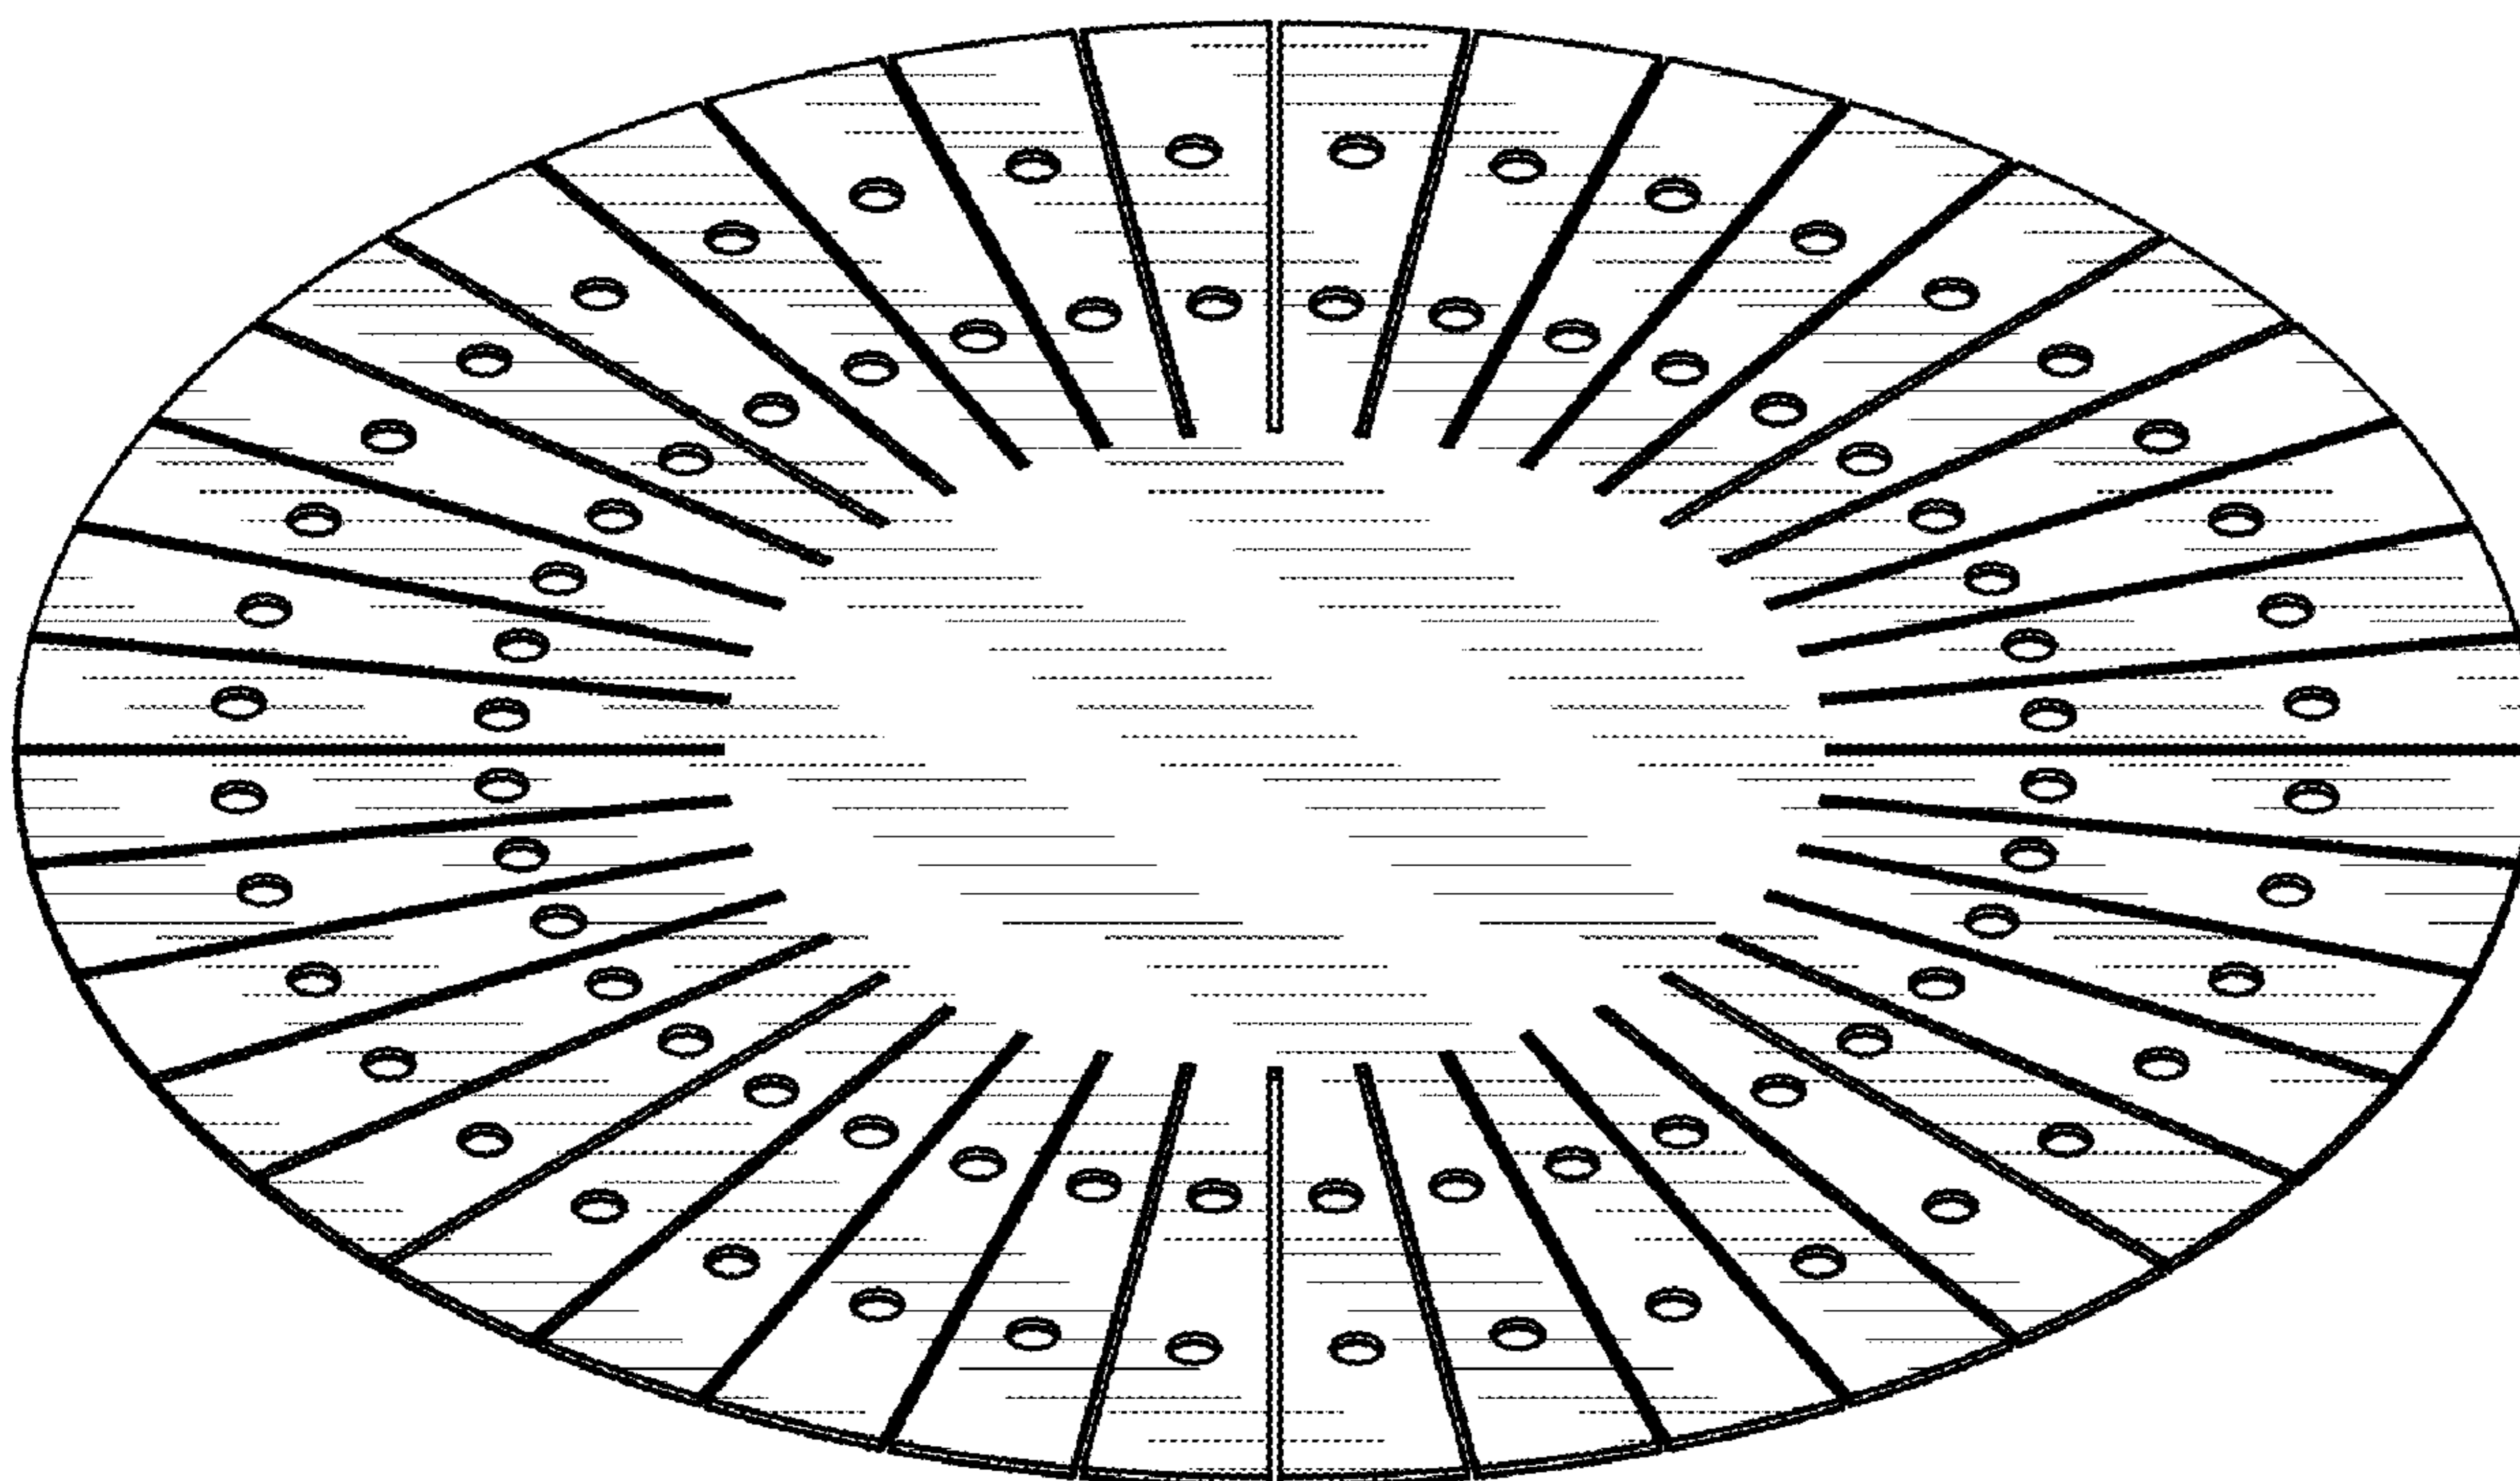

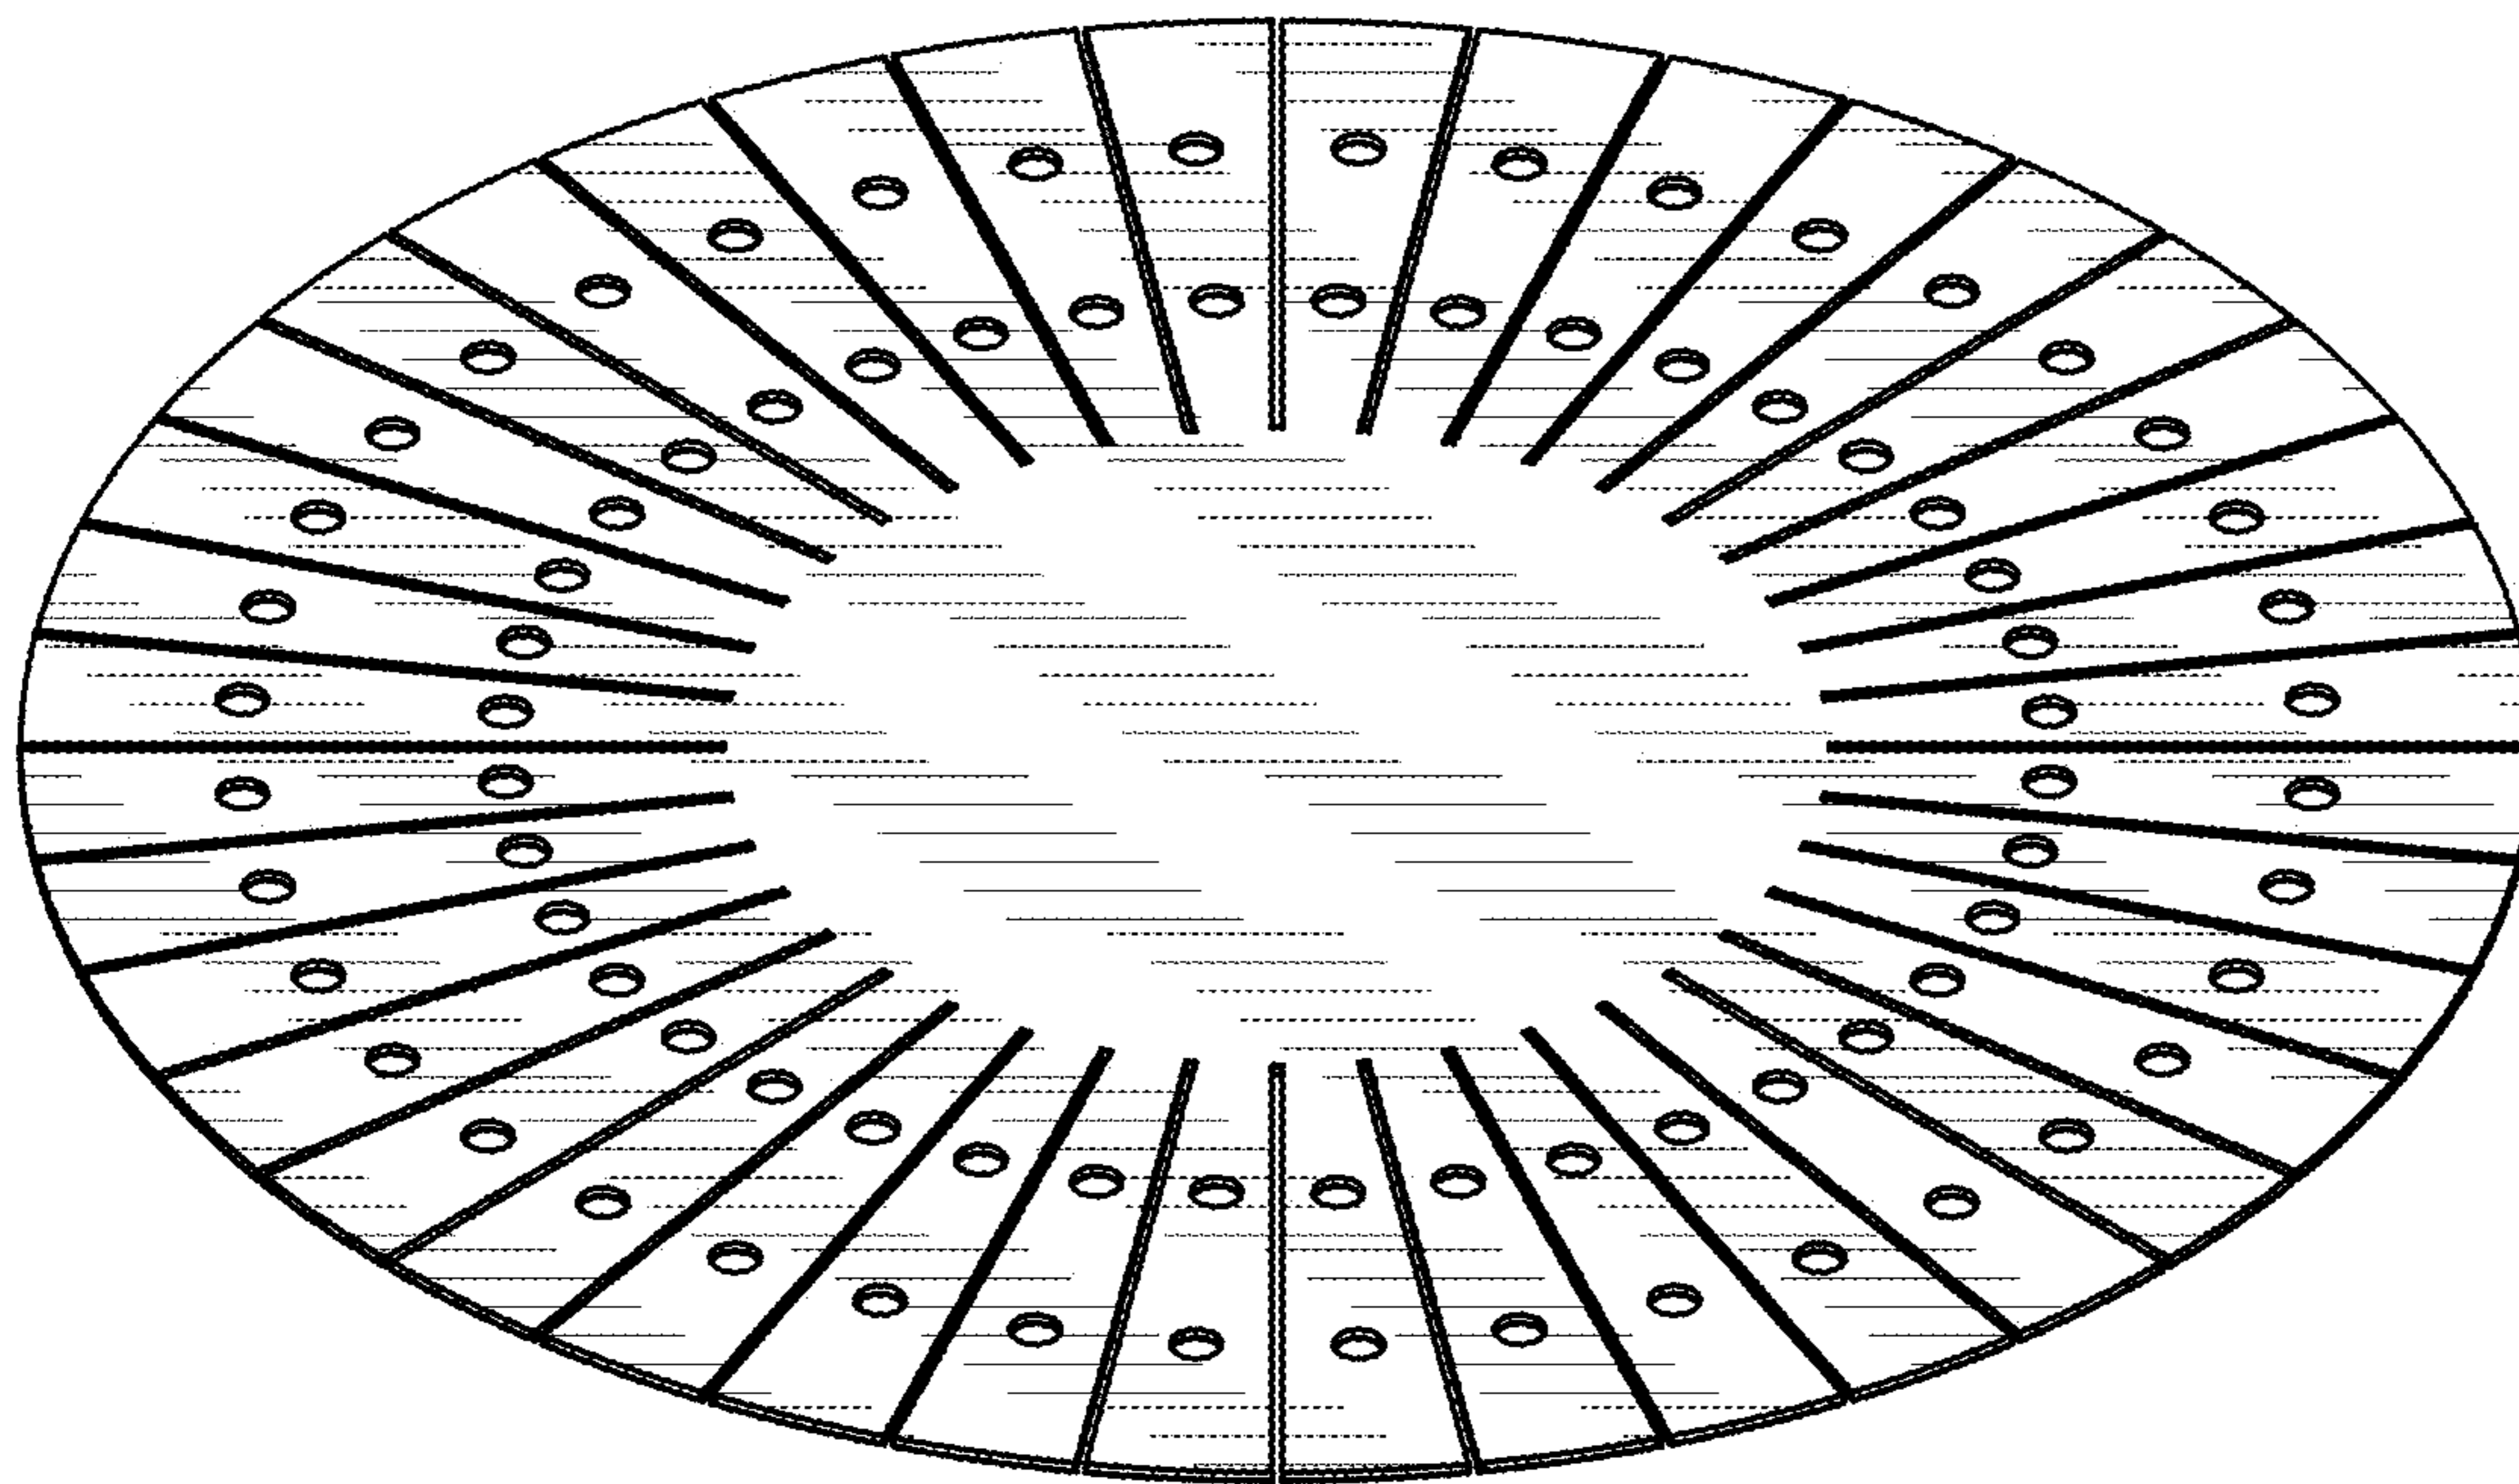


FIG. 1



FIG. 2



FIG. 3

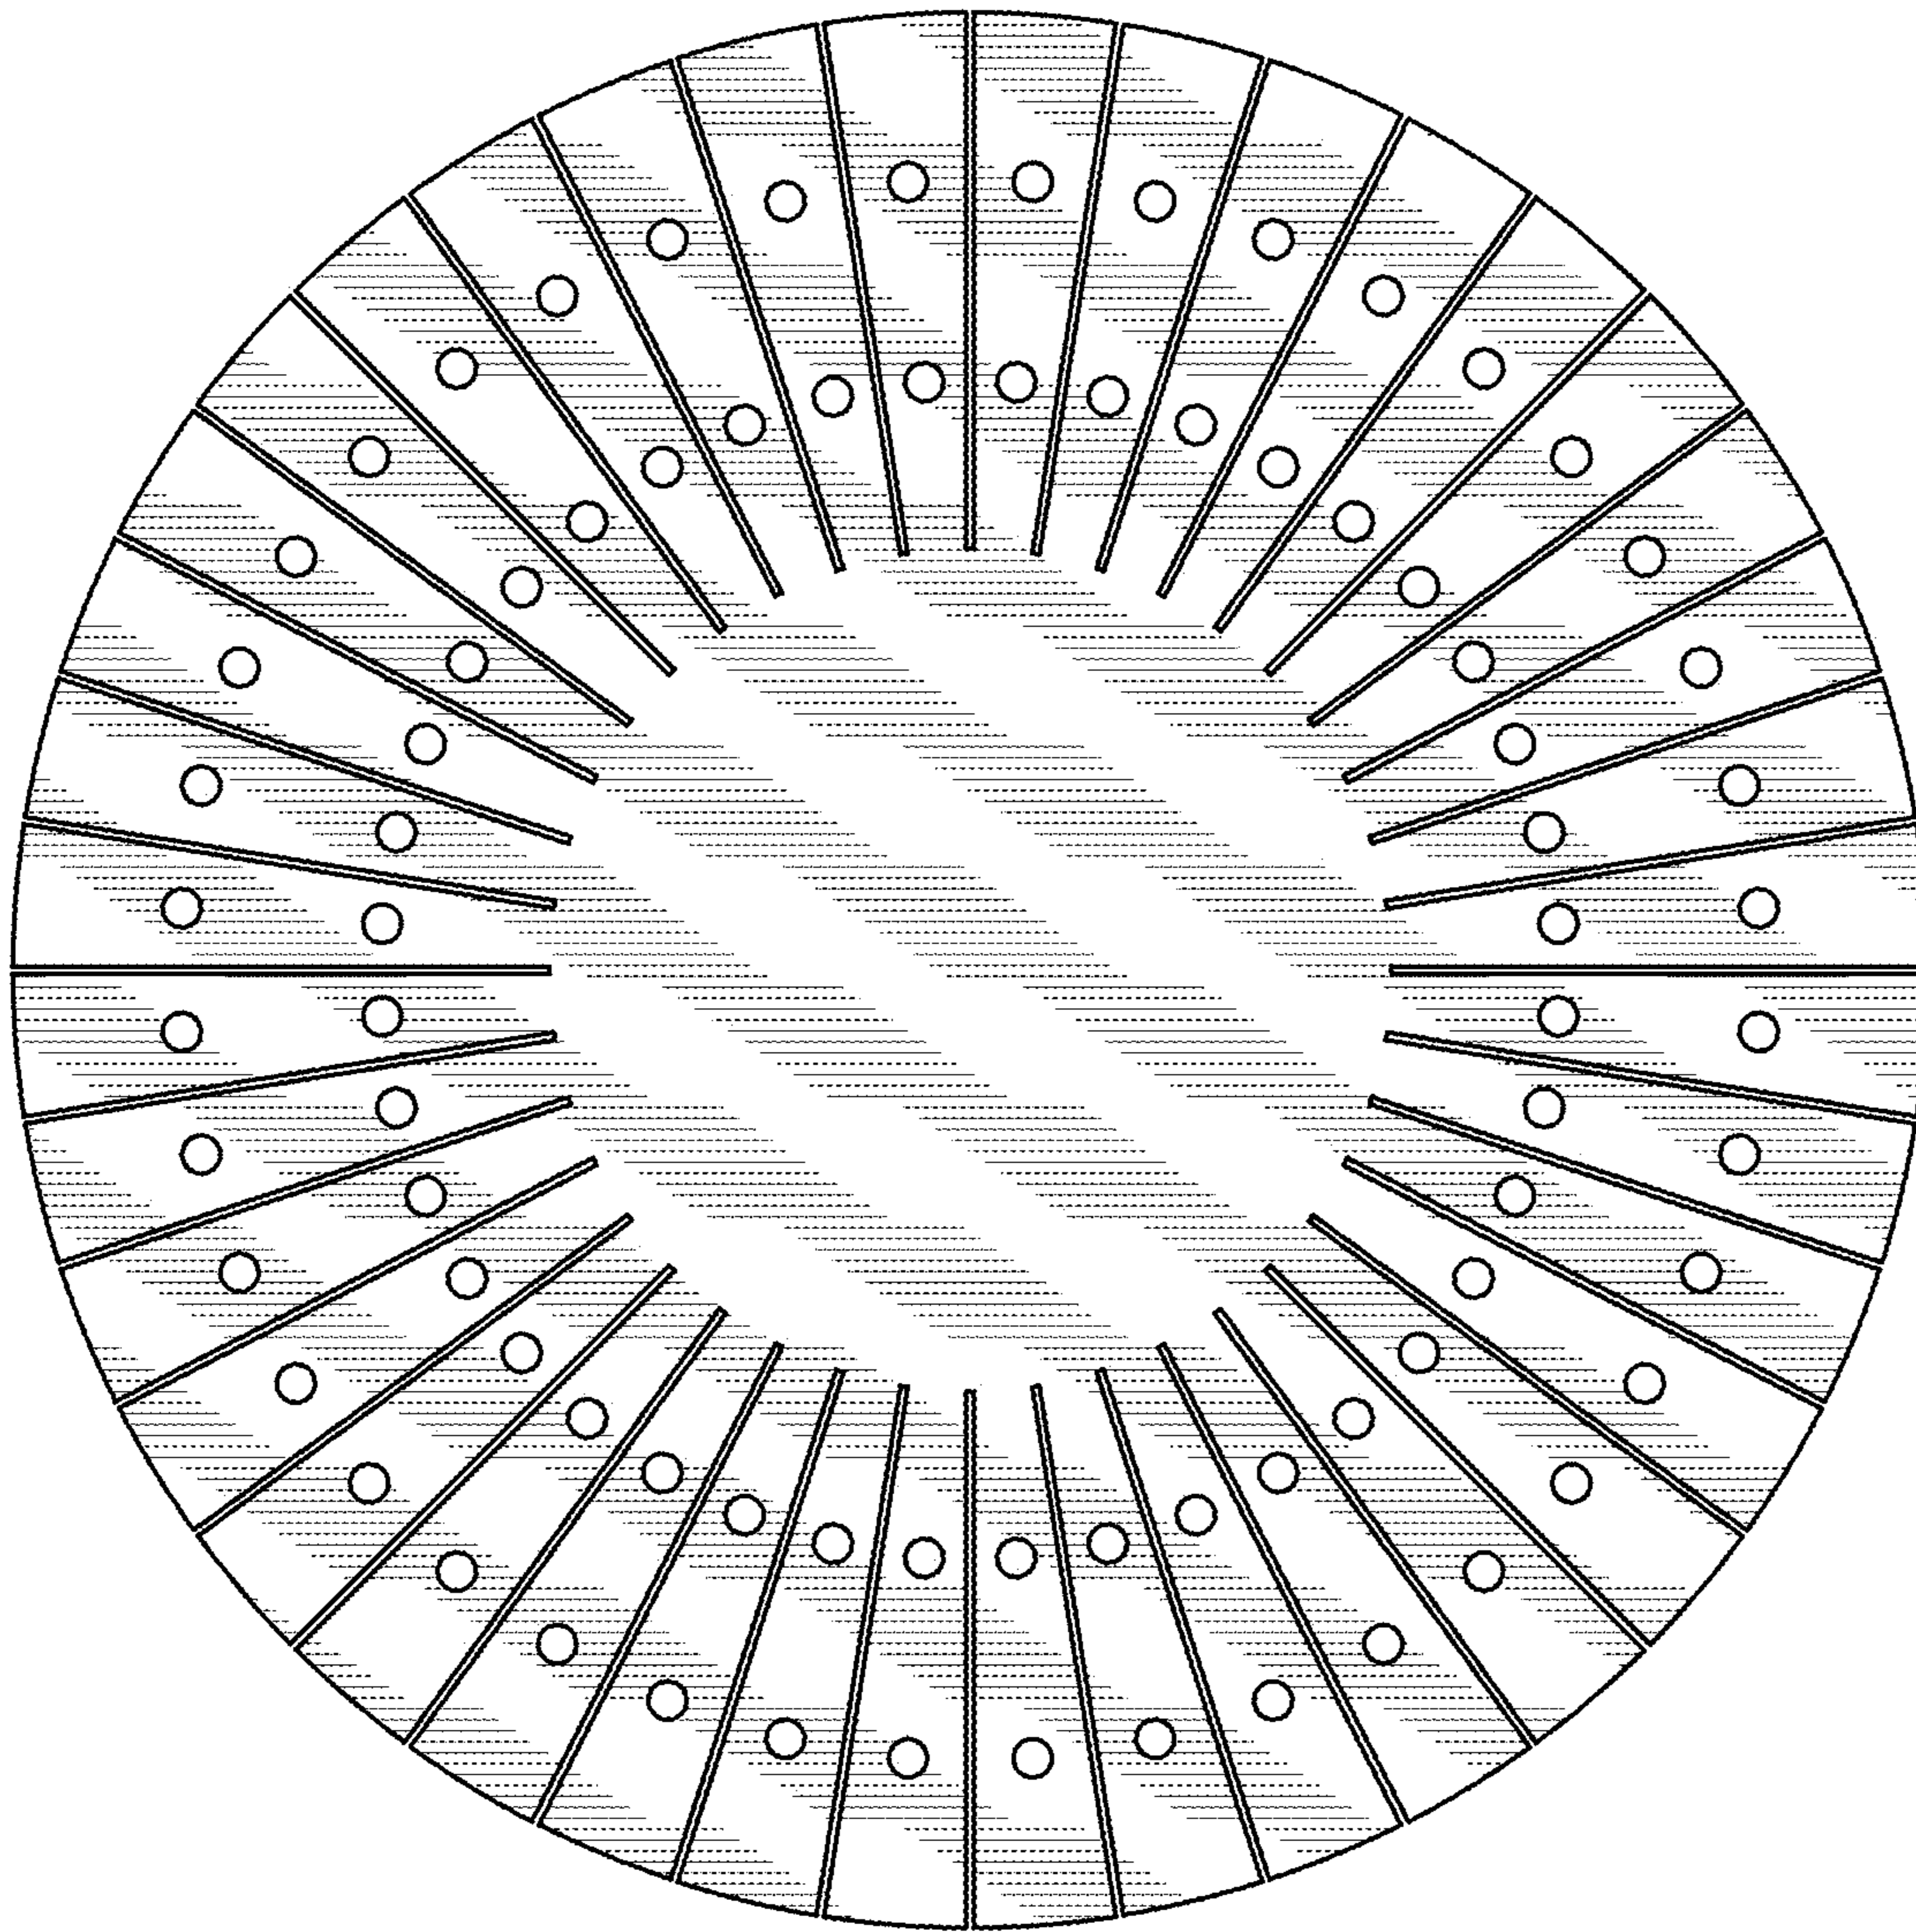


FIG. 4

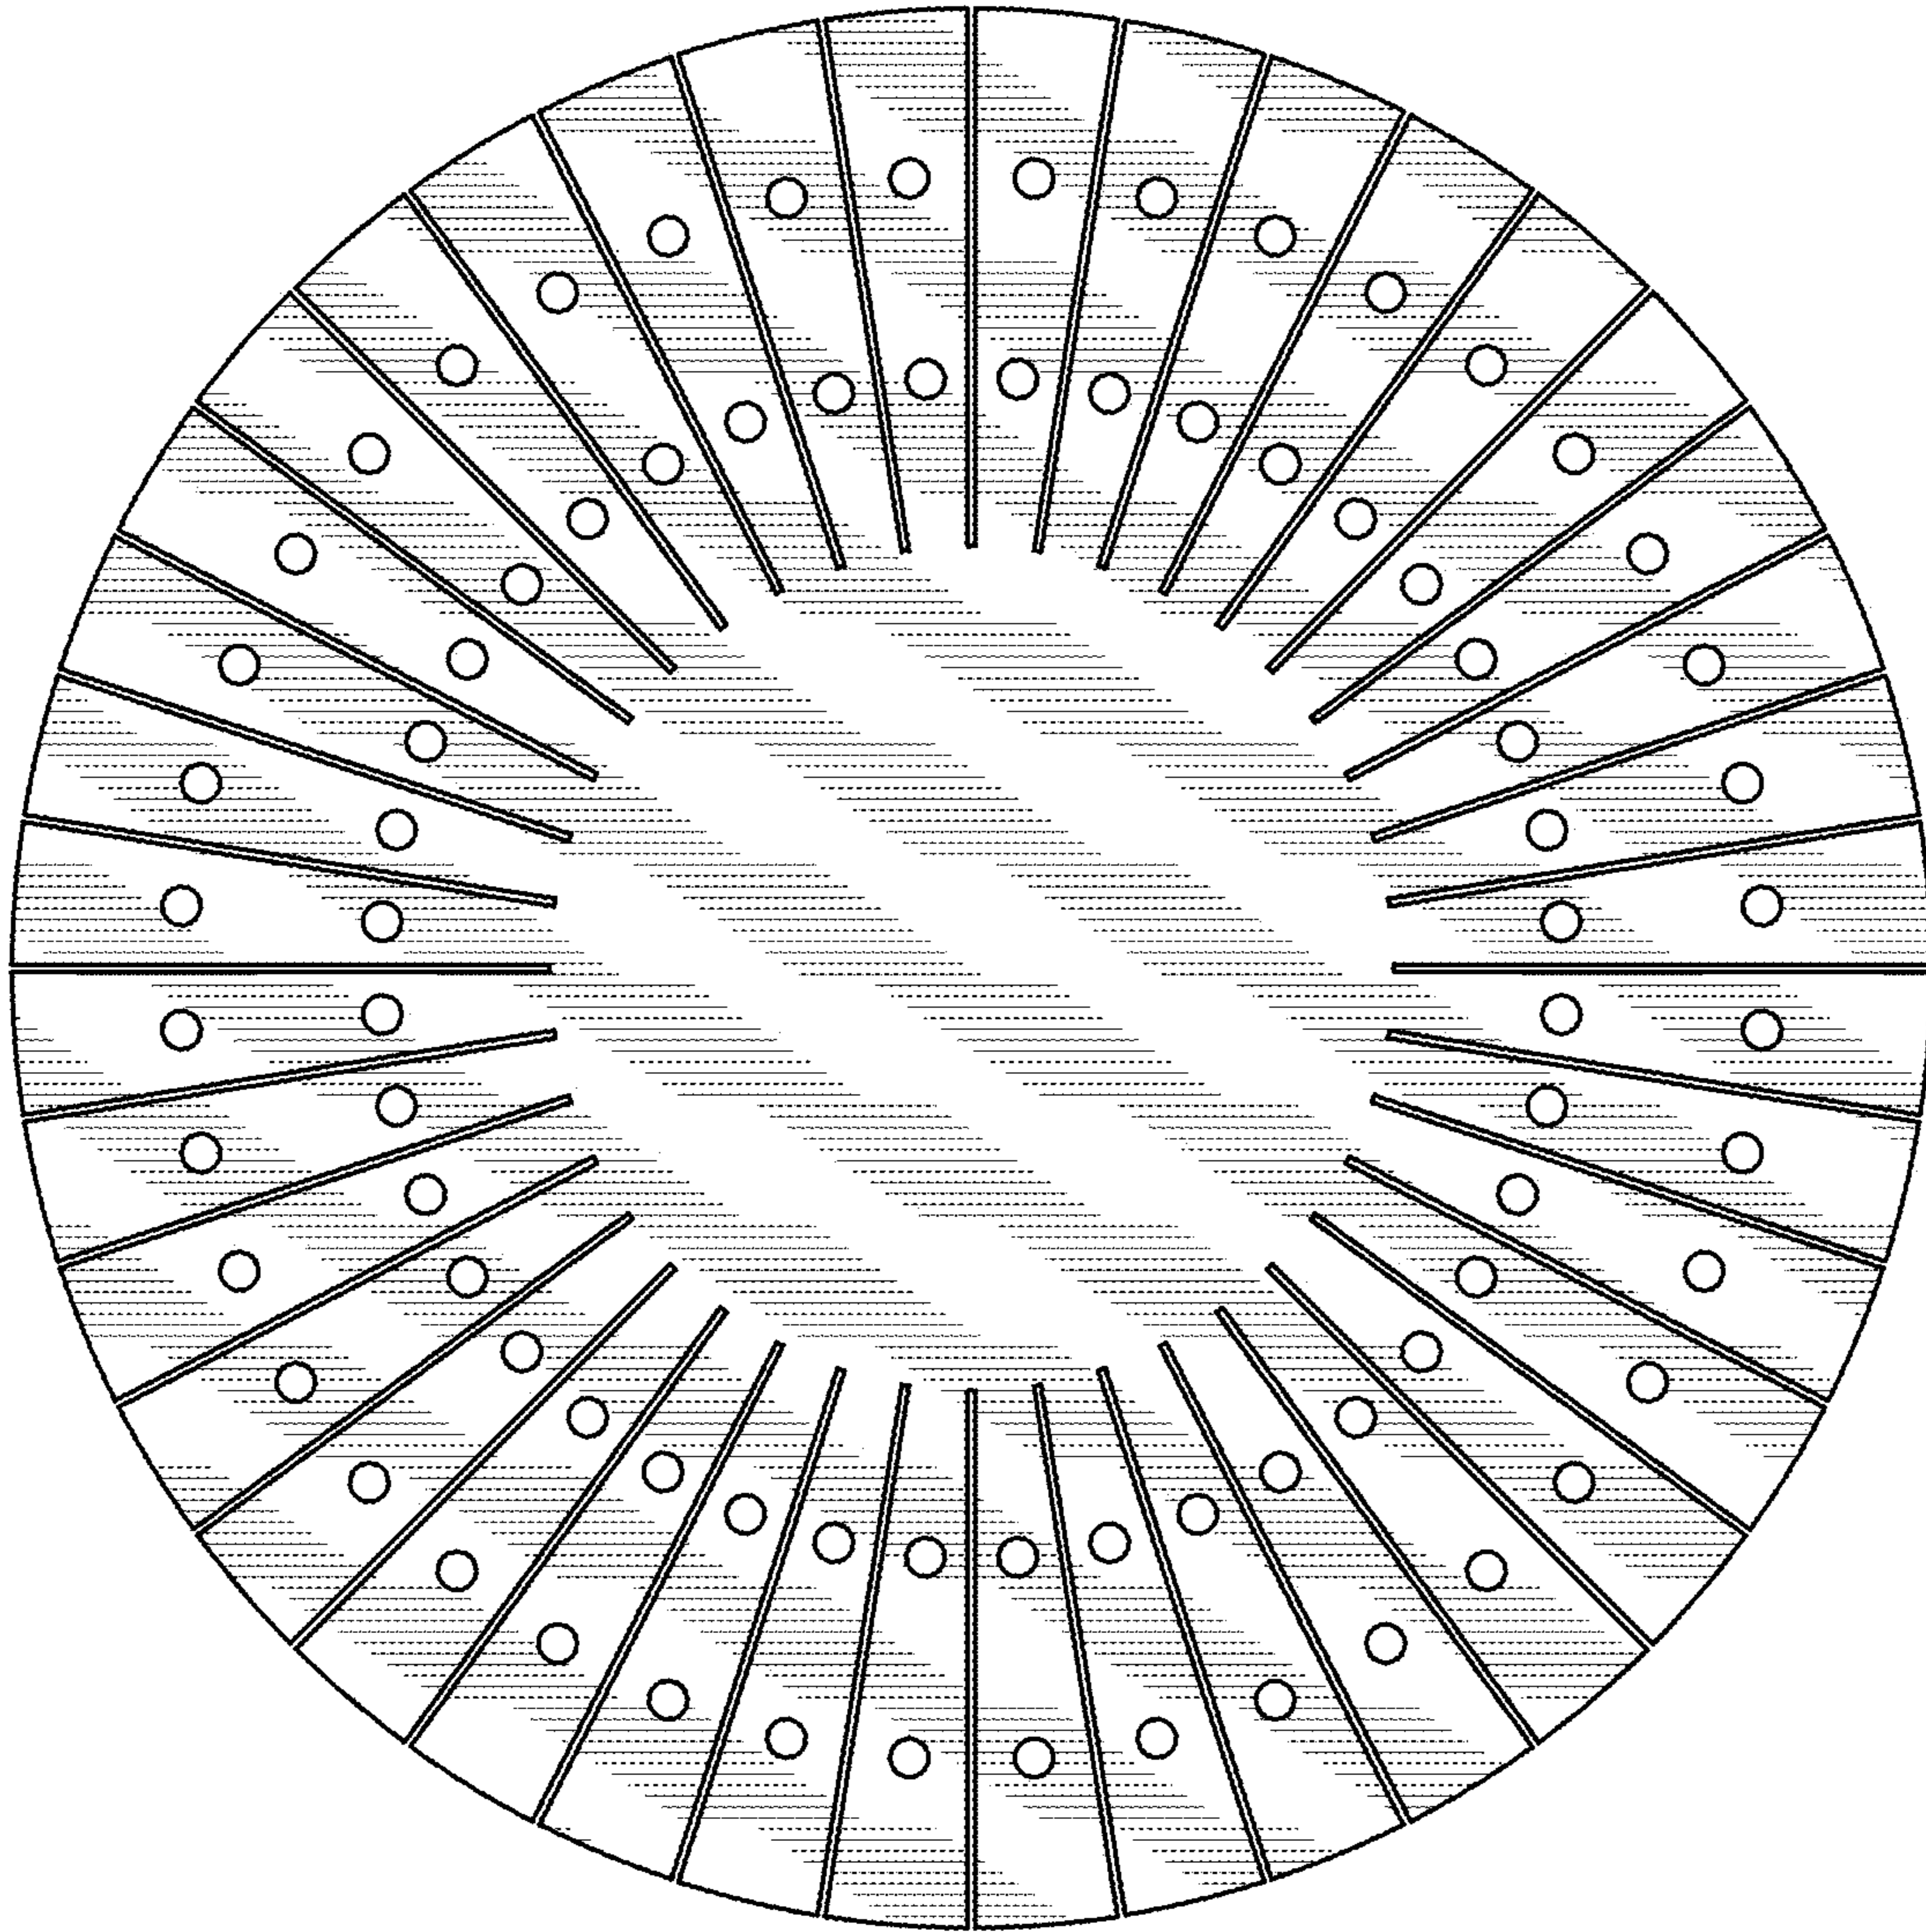


FIG. 5




FIG. 6



FIG. 7

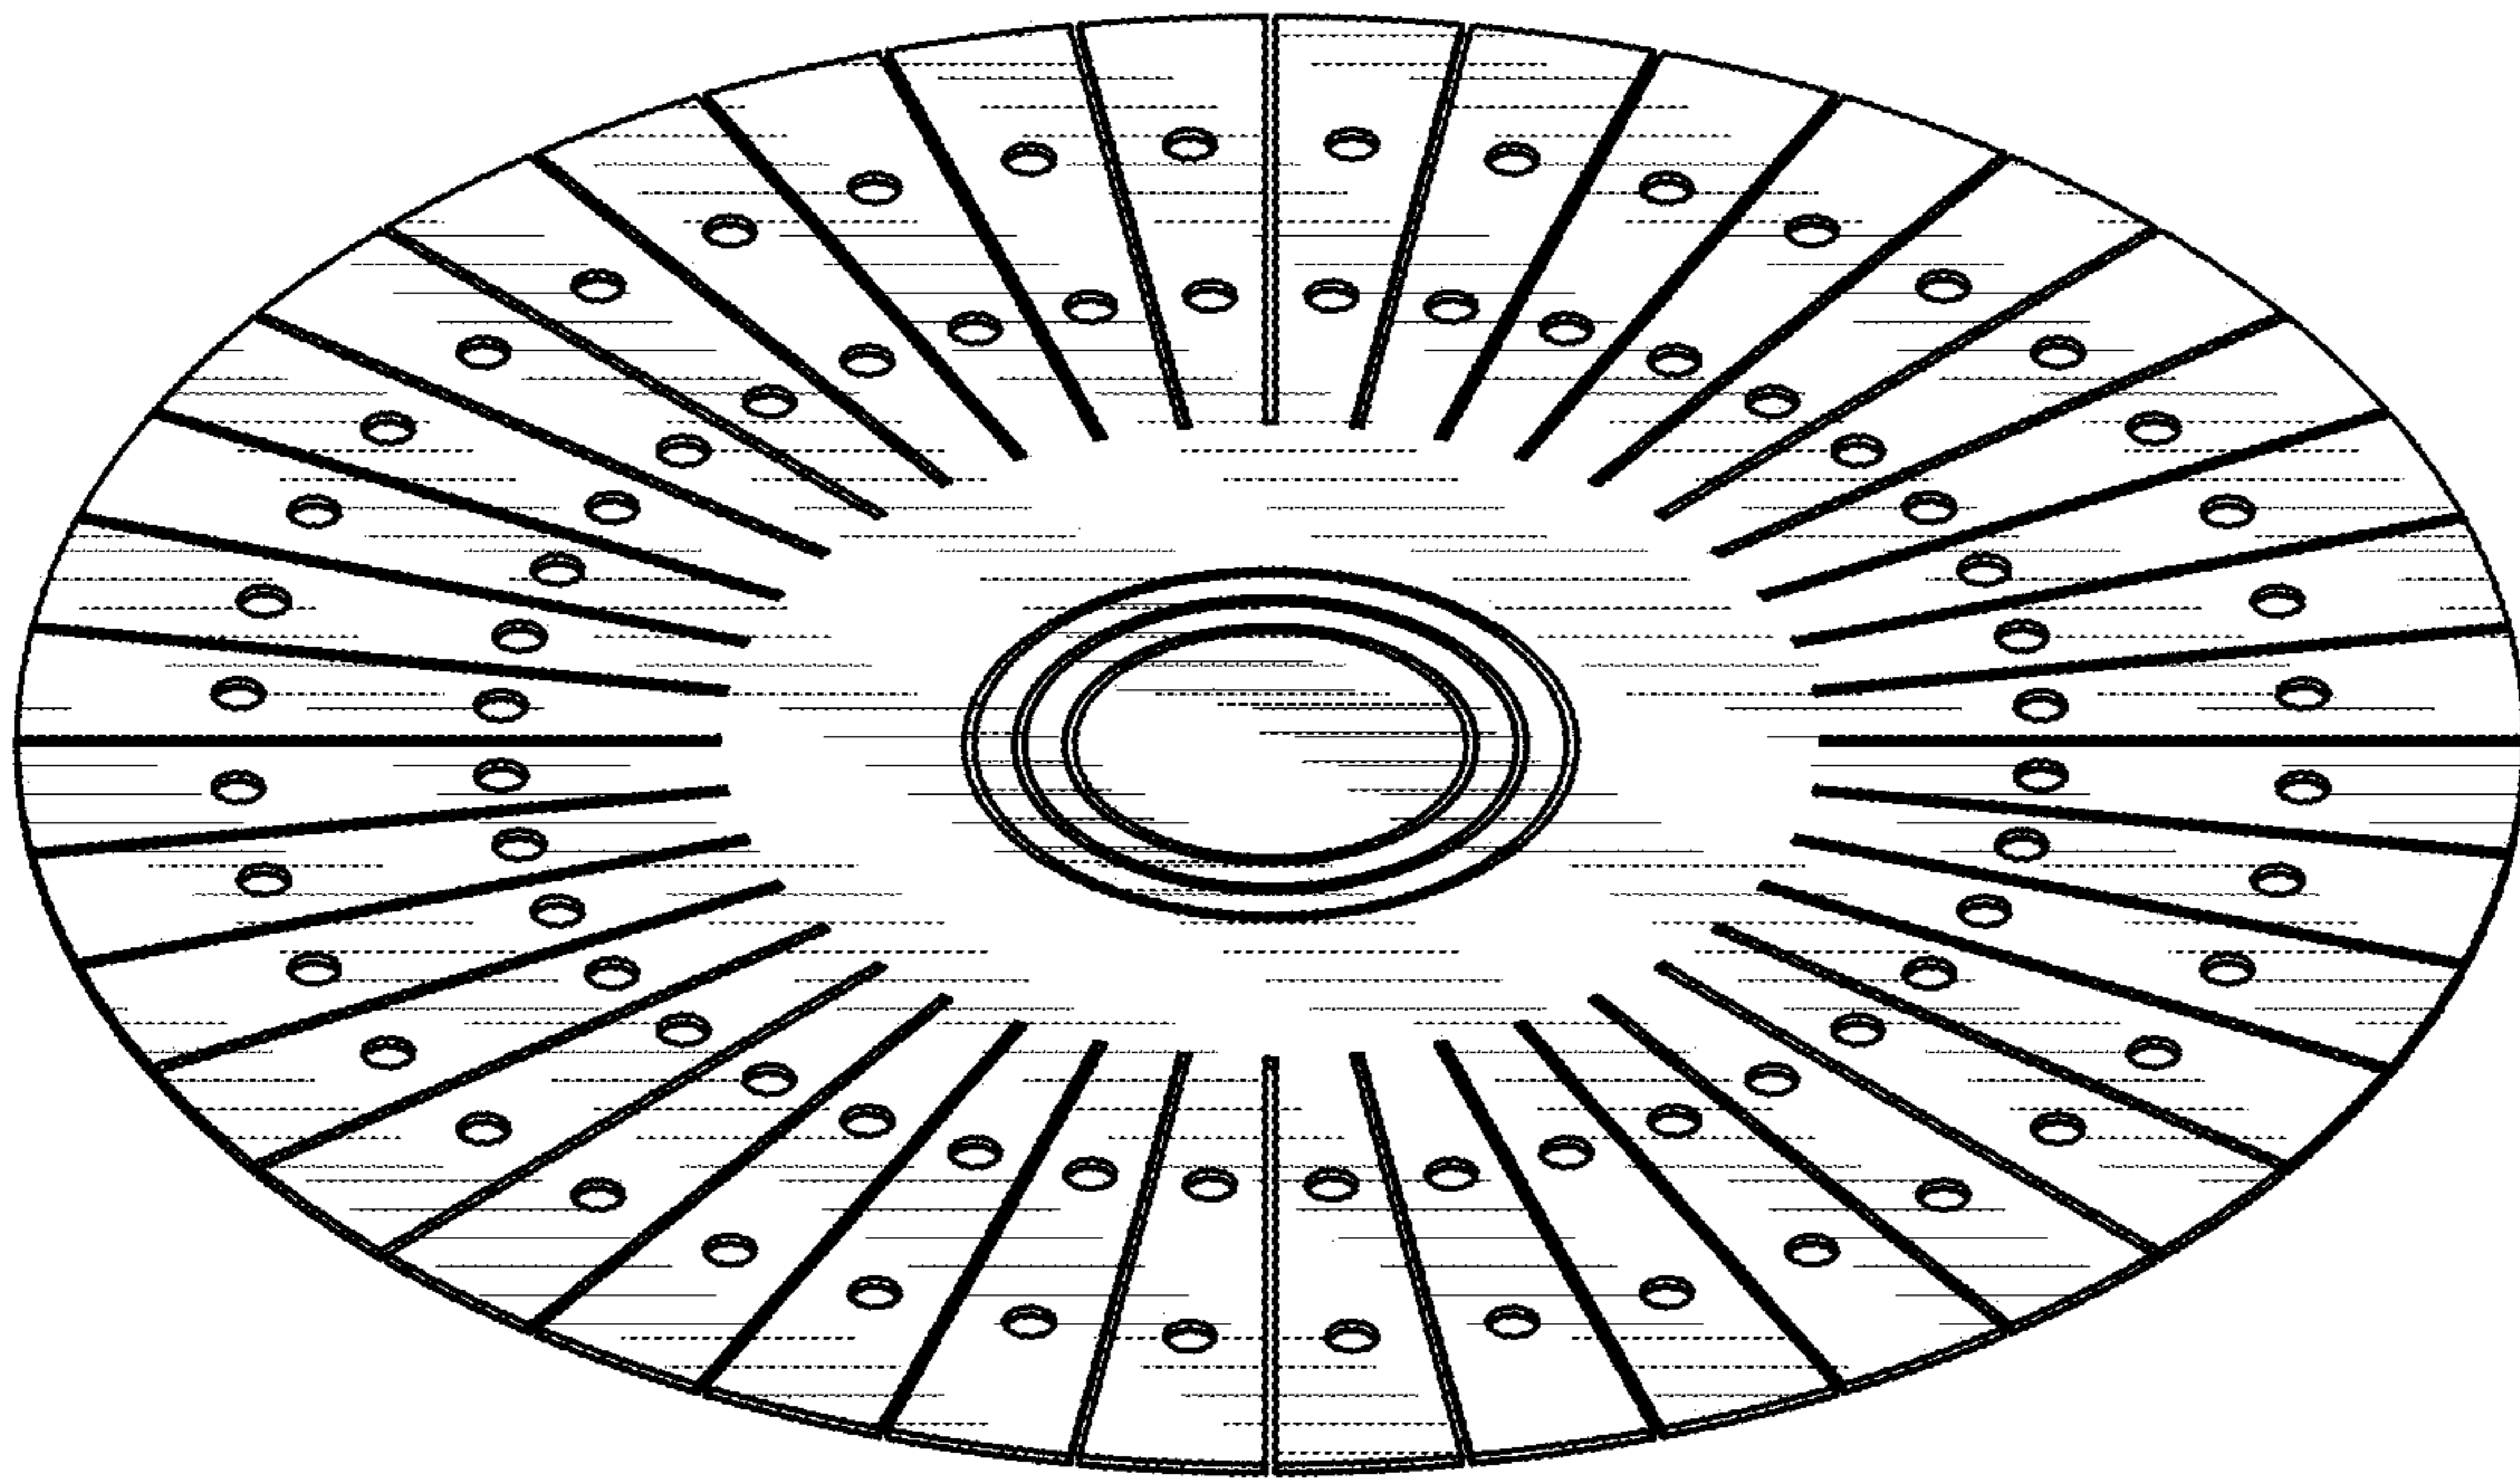


FIG. 8




FIG. 9



FIG. 10

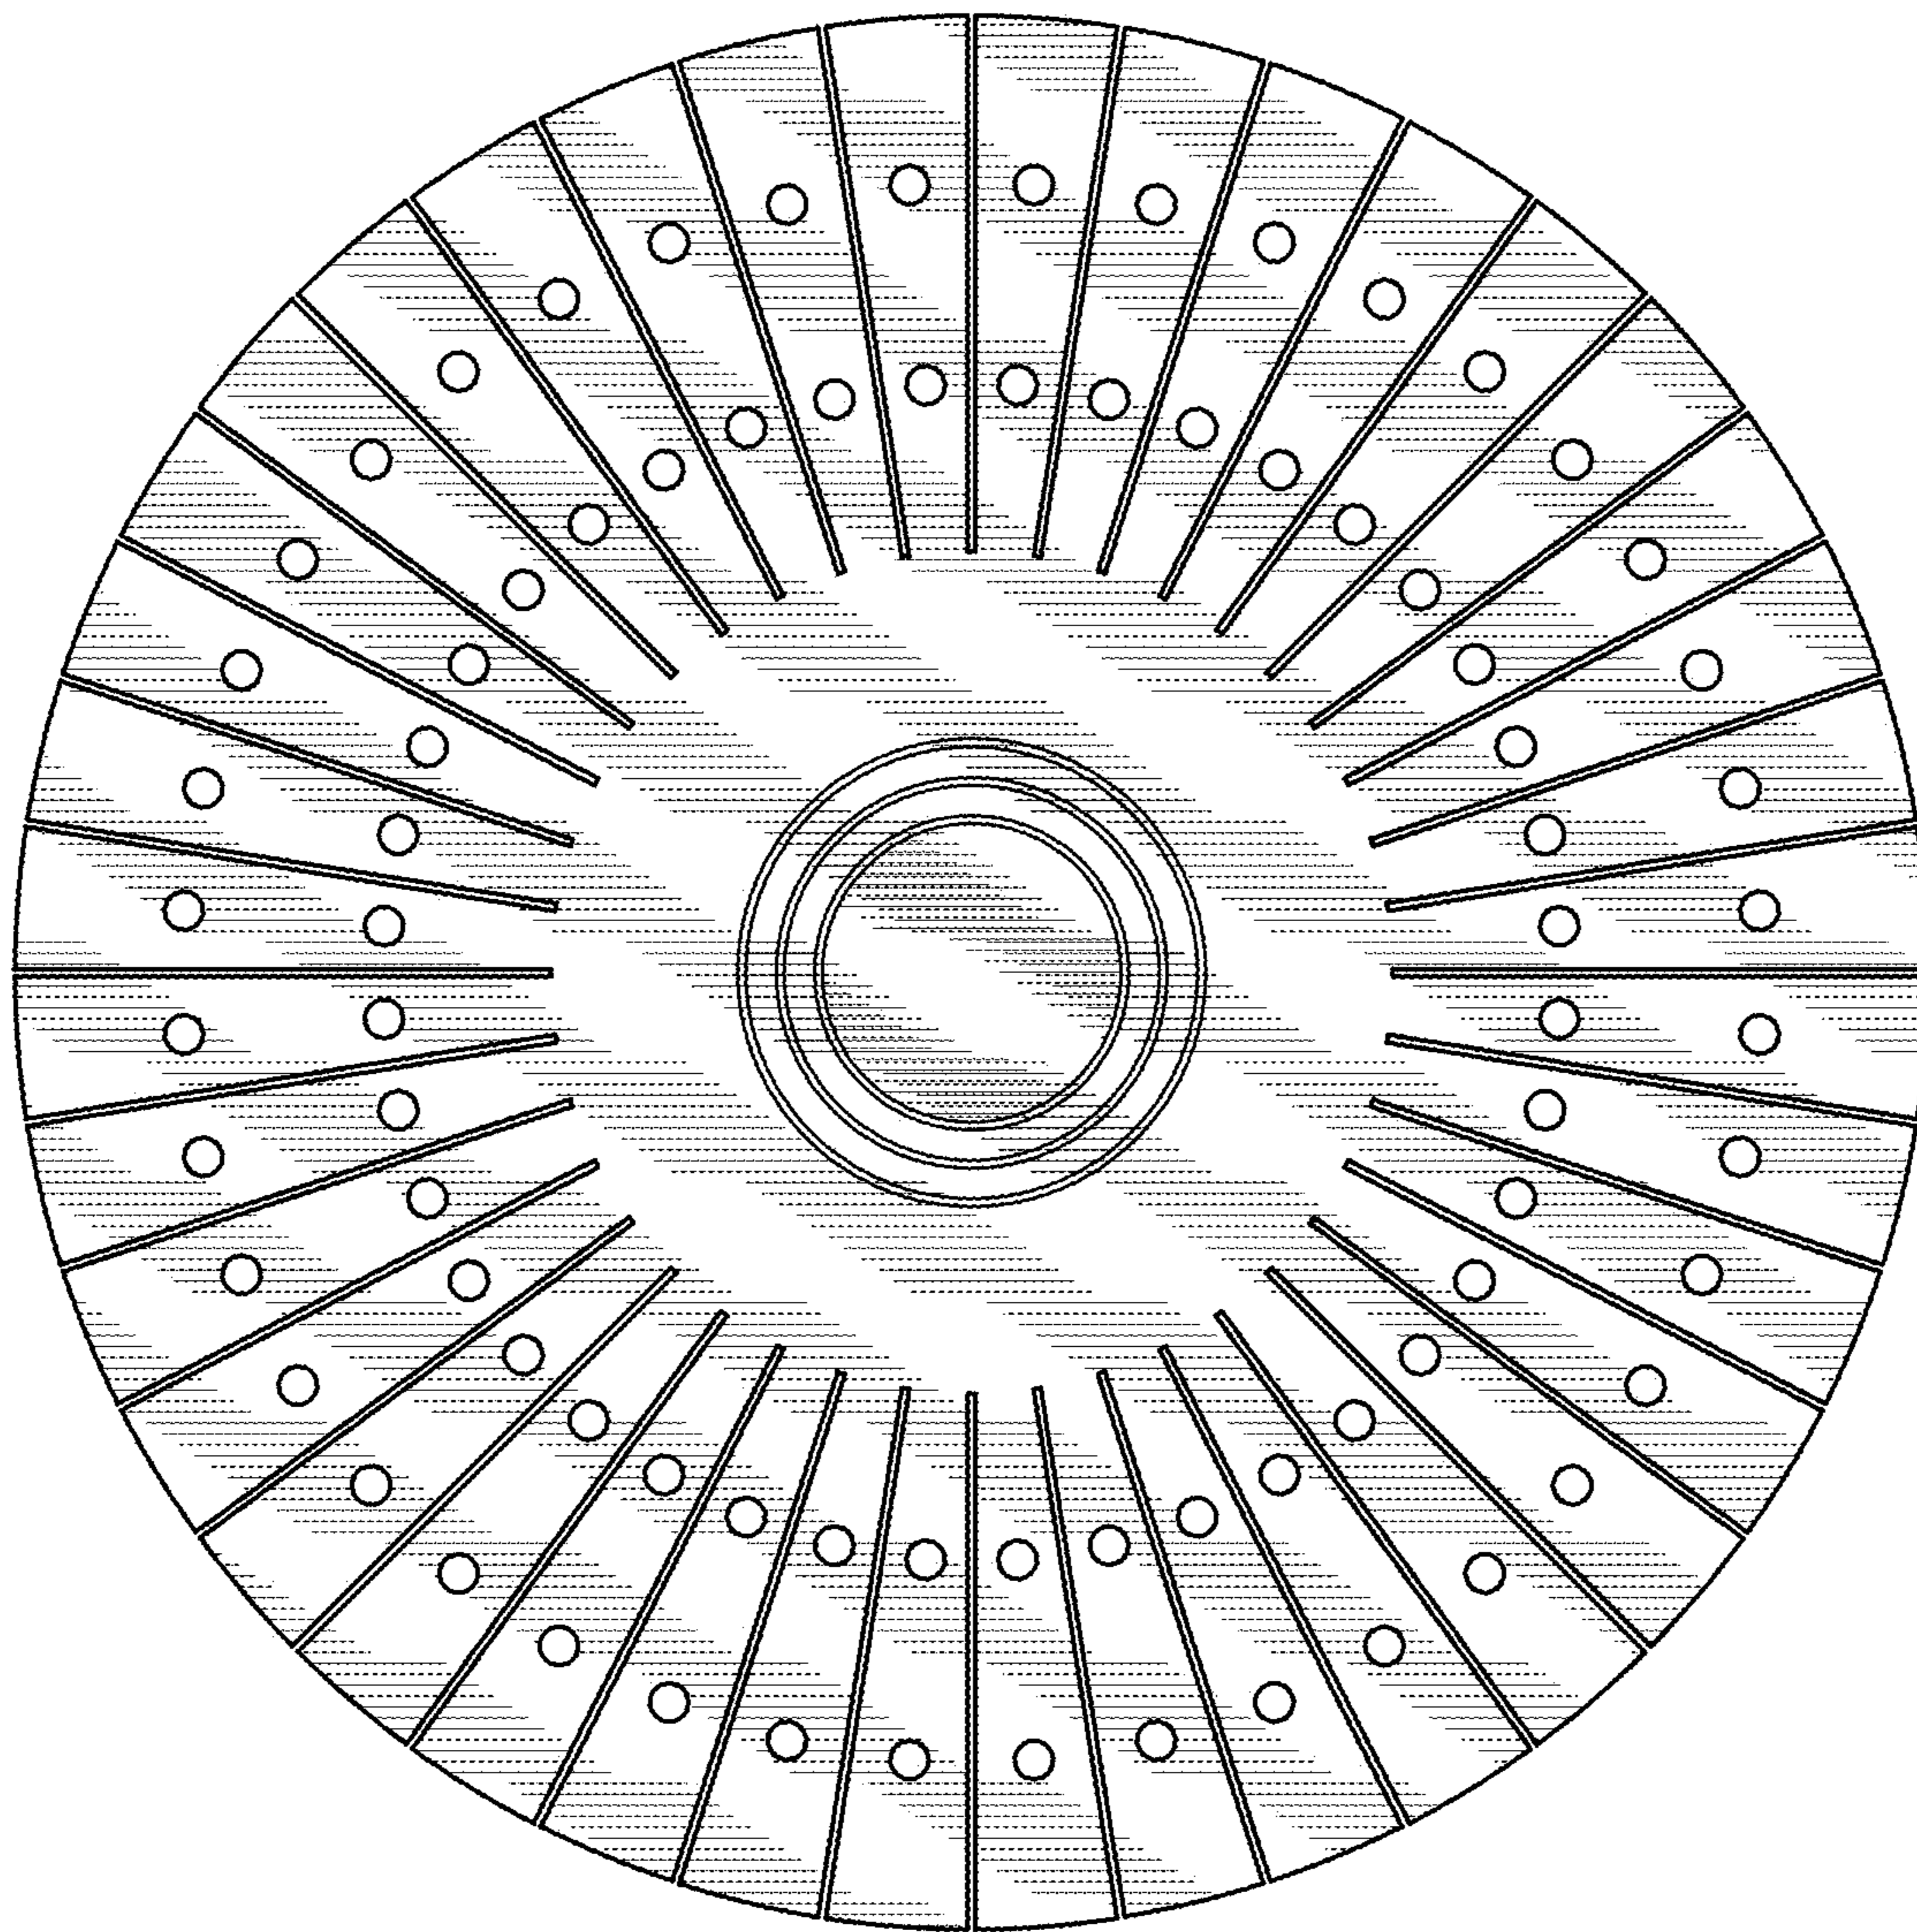


FIG. 11

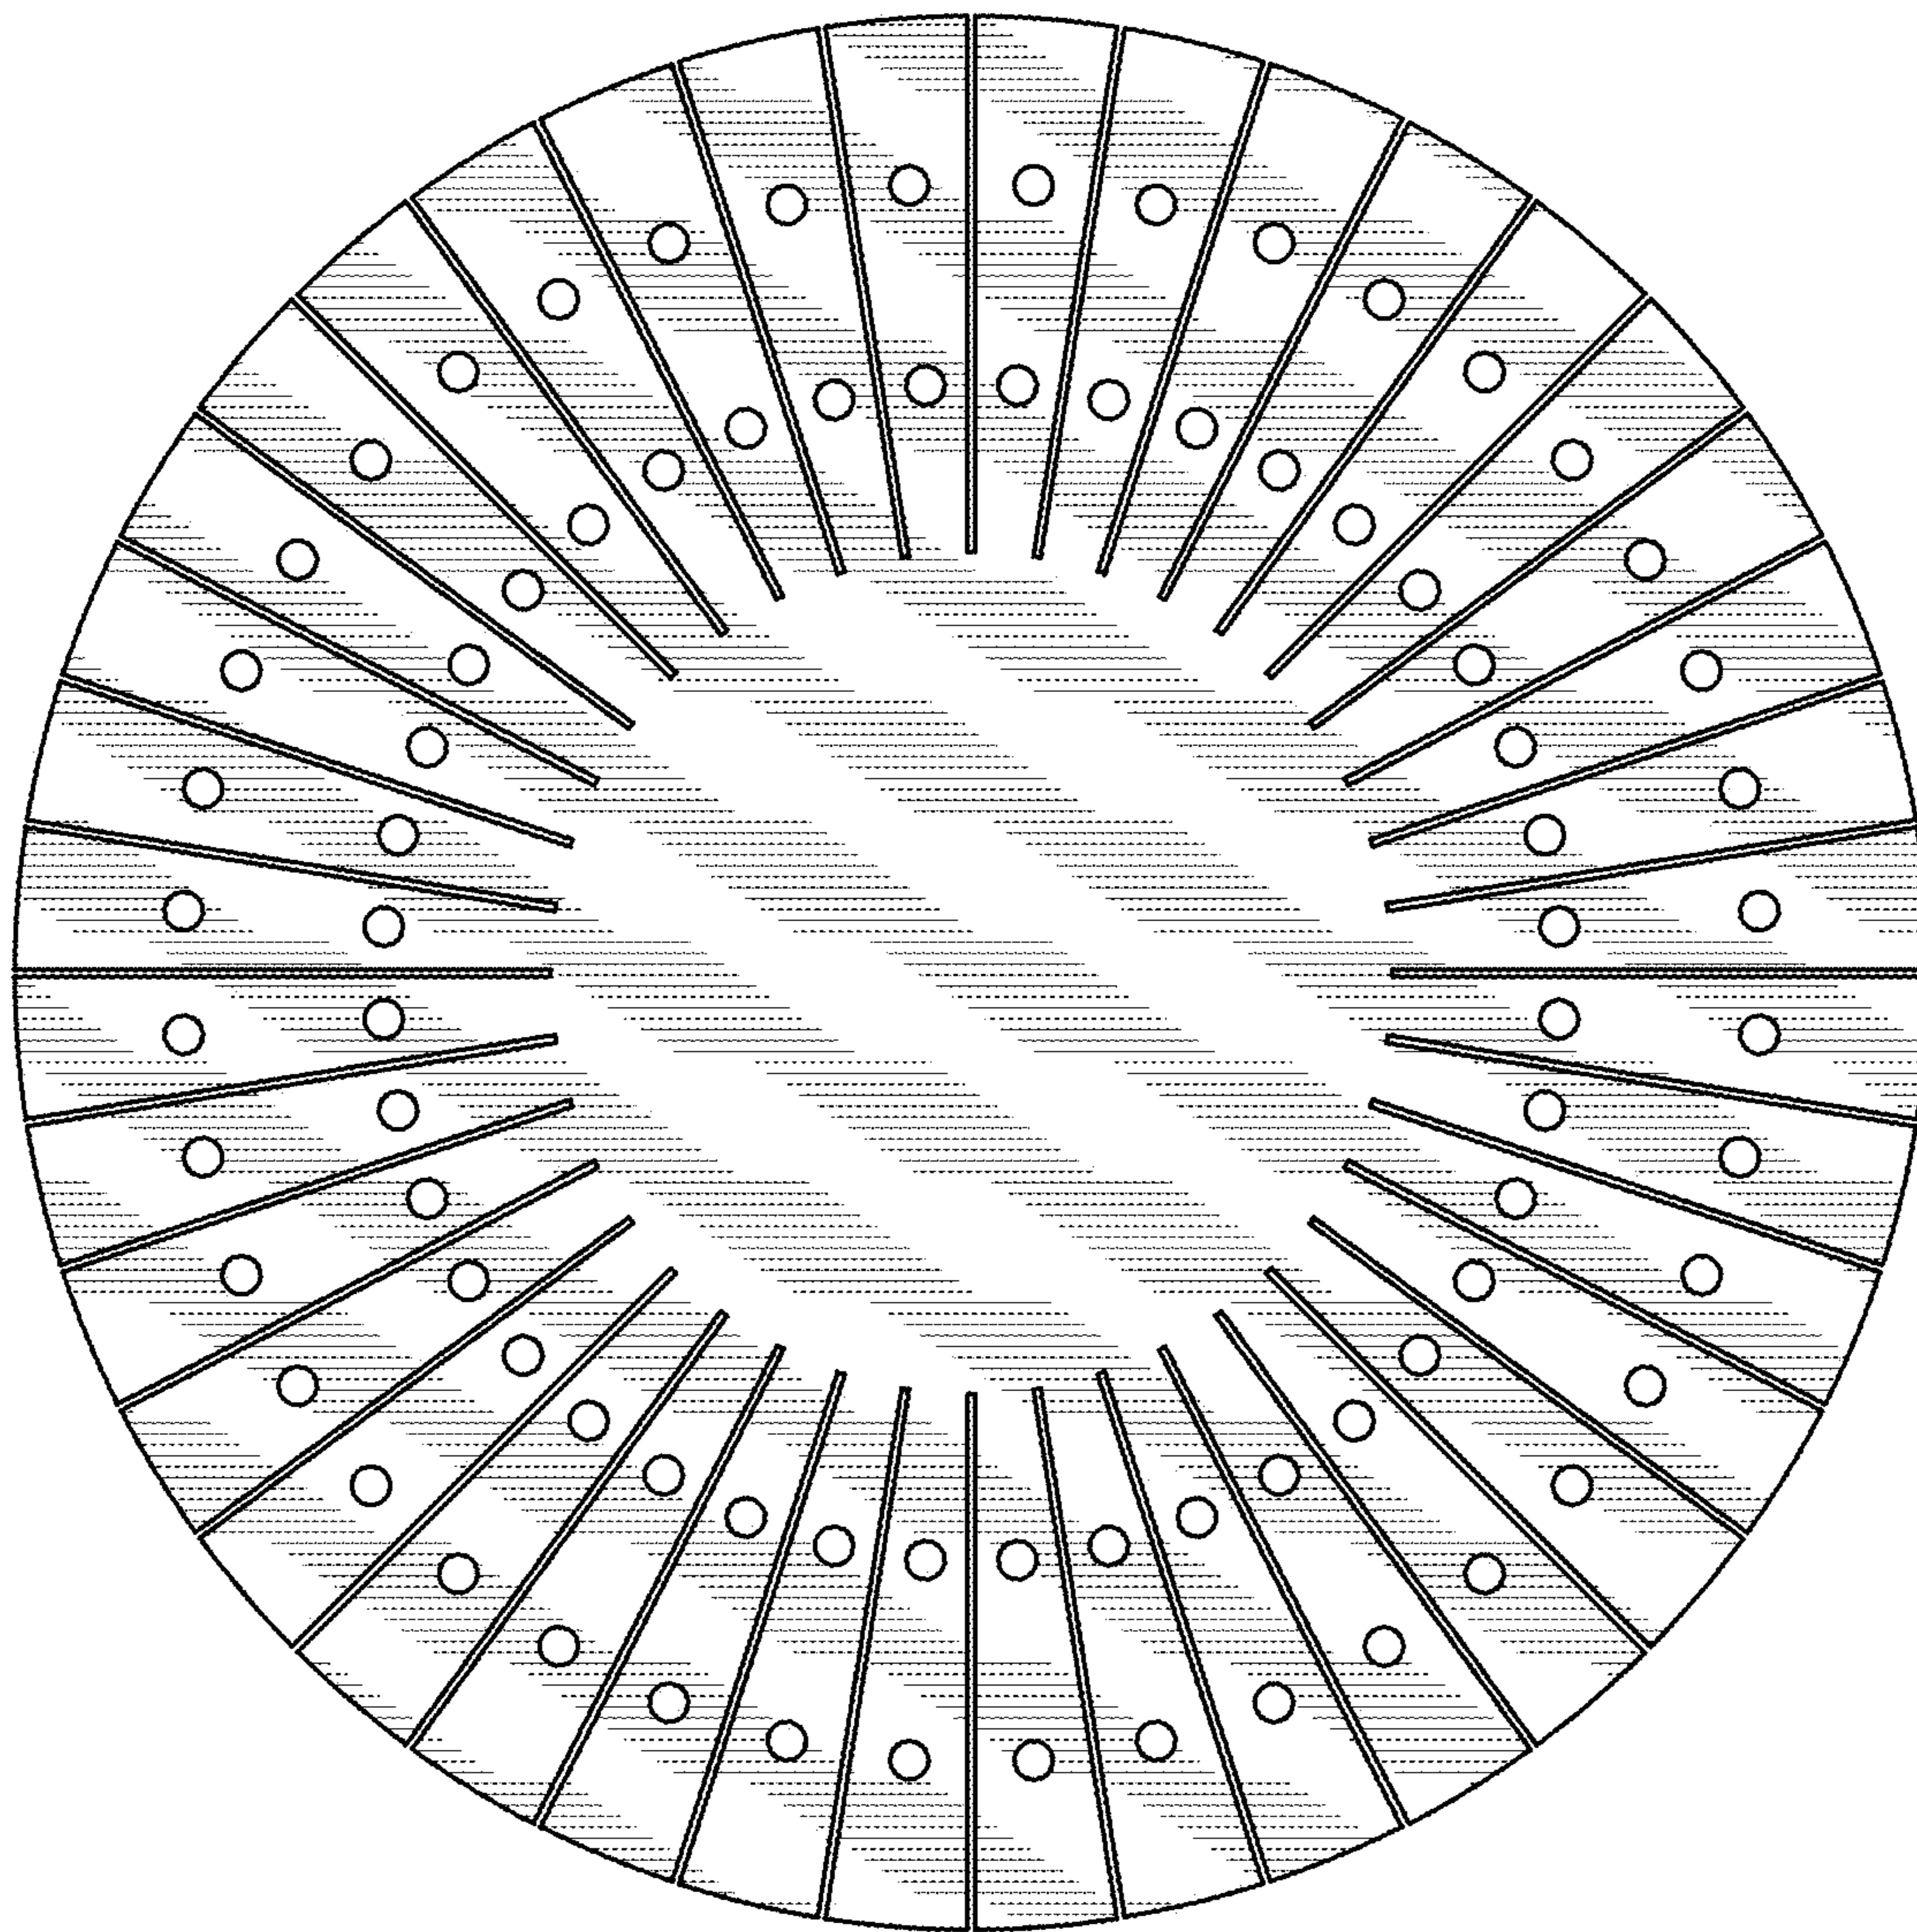


FIG. 12




FIG. 13




FIG. 14