

US00D964390S

(12) **United States Design Patent** (10) **Patent No.:** **US D964,390 S**
Mairs et al. (45) **Date of Patent:** **** Sep. 20, 2022**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH A GRAPHICAL USER INTERFACE**

(71) Applicant: **INSPIRE MEDICAL SYSTEMS, INC.**, Golden Valley, MN (US)

(72) Inventors: **Nicholas Mairs**, Minneapolis, MN (US); **Brody Belland**, St. Louis Park, MN (US); **John Rondoni**, Plymouth, MN (US); **Donovan Fellows**, Lake Elmo, MN (US); **Kathleen Tolmie**, Mendota Heights, MN (US)

(73) Assignee: **INSPIRE MEDICAL SYSTEMS, INC.**, Golden Valley, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/771,461**

(22) Filed: **Feb. 23, 2021**

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485–495
CPC G06F 3/048; G06F 3/0481; G06F 3/04812; G06F 3/04815; G06F 3/04817; G06F 3/0482; G06F 3/0483; G06F 3/0484; G06F 3/04842; G06F 3/04845; G06F 3/04847; G06F 3/0485; G06F 3/04855; G06F 3/0486; G06F 3/0487; G06F 3/0488; G06F 3/04883; G06F 3/04886
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D436,580 S *	1/2001	Navano	D14/486
D614,191 S *	4/2010	Takano	D14/486
D656,153 S *	3/2012	Imamura	D14/486

D681,047 S *	4/2013	Park	D14/486
D691,157 S *	10/2013	Ramesh	D14/486
D691,158 S *	10/2013	Ramesh	D14/486
D712,918 S *	9/2014	Frick	D14/487
D751,085 S *	3/2016	Winther	D14/485
D756,371 S *	5/2016	Bertnick	D14/485
D760,237 S *	6/2016	Sabadosh	D14/485
D761,290 S *	7/2016	Chen	D14/486
D765,120 S *	8/2016	Kim	D14/486
9,452,293 B2	9/2016	Rondoni et al.		
D771,066 S *	11/2016	Alvarez	D14/485
D776,136 S *	1/2017	Chen	D14/485
D777,177 S *	1/2017	Chen	D14/485
D778,928 S *	2/2017	Bertnick	D14/485
D786,891 S *	5/2017	Wright	D14/491
D791,153 S *	7/2017	Rice	D14/486
D794,047 S *	8/2017	Gandhi	D14/485
D797,760 S *	9/2017	Tsujimura	D14/485
D799,522 S *	10/2017	Eder	D14/488

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2021016558 A1 1/2021

Primary Examiner — Daniel J Domino

(74) *Attorney, Agent, or Firm* — Dicke, Billig & Czaja, PLLC

(57) **CLAIM**


The ornamental design for a display screen or portion thereof with a graphical user interface, as shown and described.

DESCRIPTION

The sole FIGURE is a front view of a display screen or portion thereof with a graphical user interface showing our new design.

The outermost broken lines show a display screen or portion thereof and form no part of the claimed design. The remaining broken lines show elements of the graphical user interface that form no part of the claimed design.

1 Claim, 1 Drawing Sheet

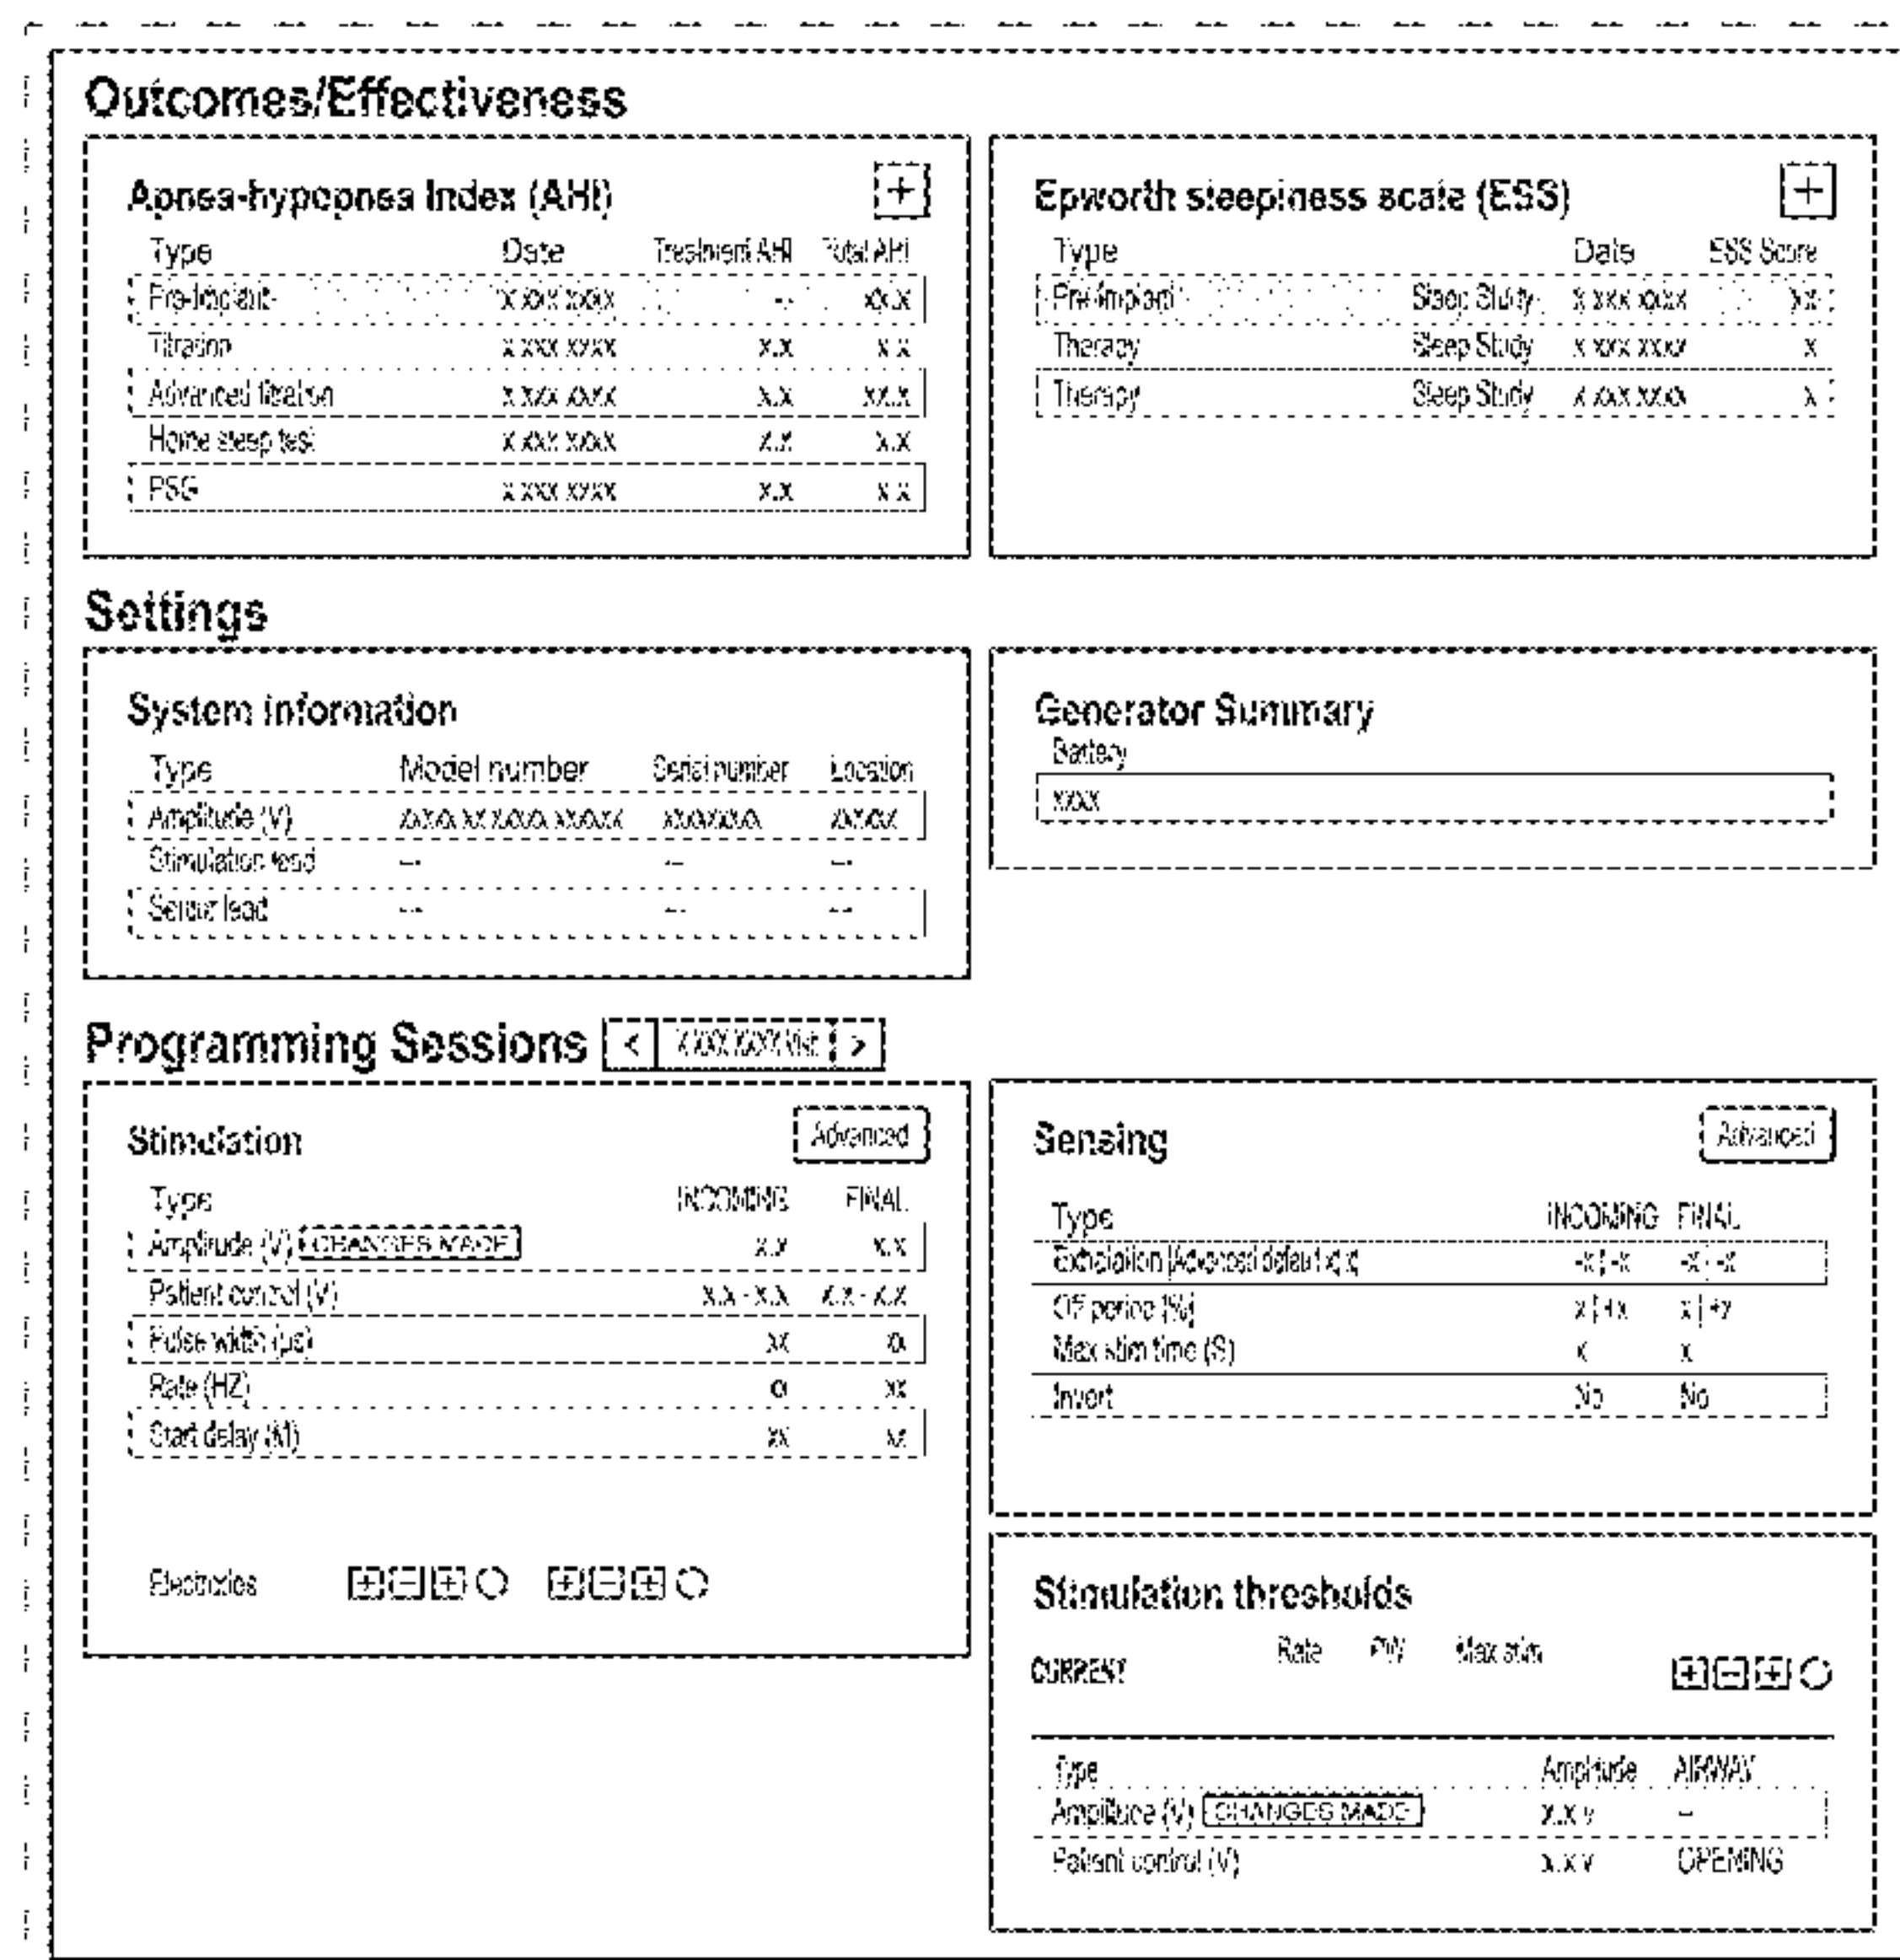

(56)

References Cited

U.S. PATENT DOCUMENTS

9,839,786 B2 12/2017 Rondoni et al.
D809,530 S * 2/2018 Matheson D14/485
D810,106 S * 2/2018 Storm D14/486
D812,081 S * 3/2018 Saneii D14/486
D812,633 S * 3/2018 Saneii D14/486
D820,292 S * 6/2018 Mander D14/486
D823,860 S * 7/2018 Witten D14/485
D826,977 S * 8/2018 Nakajima D14/488
D828,372 S * 9/2018 Kolbenheyer D14/486
D832,865 S 11/2018 Dieken et al.
D833,461 S 11/2018 Dieken et al.
D836,652 S * 12/2018 Fowler D14/486
D836,655 S * 12/2018 Hotchkiss D14/486
D840,426 S 2/2019 Dieken et al.
D841,031 S * 2/2019 Orlando D14/486
D842,313 S * 3/2019 Kagan D14/485
D842,314 S * 3/2019 Govindan Sankar Selvan
D14/485
D847,170 S * 4/2019 Lirov D14/486
D848,468 S * 5/2019 Ng D14/486
D854,560 S * 7/2019 Field D14/486
D854,561 S * 7/2019 Field D14/486
D856,365 S * 8/2019 Lofberg D14/488
D866,577 S * 11/2019 Eisert D14/486
D869,490 S 12/2019 Rondoni et al.
D871,433 S 12/2019 Rondoni et al.
D871,434 S 12/2019 Rondoni et al.
D884,008 S * 5/2020 Thornberg D14/486
D884,717 S * 5/2020 Clymer D14/485
D885,413 S * 5/2020 Ramkumar D14/486
D886,125 S * 6/2020 Kumar D14/485
D888,082 S * 6/2020 Weick D14/486
10,691,304 B1 * 6/2020 Anand G06F 3/0481
D890,783 S * 7/2020 Casse D14/486
D892,143 S * 8/2020 Dascola D14/485

D893,524 S * 8/2020 Sabourenkov D14/486
D896,828 S * 9/2020 Linares D14/486
D916,767 S * 4/2021 VanSickler D14/486
D918,253 S * 5/2021 Choe D14/488
D921,662 S * 6/2021 Giannino D14/486
D921,673 S * 6/2021 Kmak D14/488
D921,675 S * 6/2021 Kmak D14/486
D924,909 S * 7/2021 Nasu D14/486
D927,528 S * 8/2021 Heisler D14/486
D930,677 S * 9/2021 Sastry D14/486
D933,674 S * 10/2021 Doyle D14/485
D937,870 S * 12/2021 Pinto H04L 63/20
D14/486
D937,876 S * 12/2021 Harvey D14/486
D938,461 S * 12/2021 Hoffman D14/486
D940,178 S * 1/2022 Ang D14/488
D941,849 S * 1/2022 Knowles D14/492
D943,605 S * 2/2022 Zheng D14/485
D943,606 S * 2/2022 Zheng D14/485
D946,022 S * 3/2022 Nuttbrown D14/491
D946,023 S * 3/2022 Nuttbrown D14/491
D946,024 S * 3/2022 Vogler-Ivashchanka D14/491
D946,025 S * 3/2022 Vogler-Ivashchanka D14/492
D946,040 S * 3/2022 Kramer D14/487
D946,610 S * 3/2022 VanSickler D14/492
D949,882 S * 4/2022 Mao D14/485
D949,883 S * 4/2022 Francis D14/485
D950,592 S * 5/2022 Kharat D14/486
D950,597 S * 5/2022 Hashimoto D14/487
11,321,767 B1 * 5/2022 Myers G06Q 30/08
2014/0115471 A1 * 4/2014 Demkin G06F 9/451
715/719
2015/0213211 A1 * 7/2015 Zaleski G06F 3/0482
715/753
2019/0175026 A1 6/2019 Verzal et al.
2019/0365228 A1 12/2019 Rondoni et al.
2019/0371478 A1 12/2019 Rondoni et al.
2019/0371479 A1 12/2019 Rondoni et al.

* cited by examiner

Outcomes/Effectiveness

Apnea-hypopnea Index (AHI) +

Type	Date	Treatment AHI	Total AHI
Pre-Implant	X XXX XXXX	-	XX.X
Titration	X XXX XXXX	X.X	X.X
Advanced titration	X XXX XXXX	X.X	XX.X
Home sleep test	X XXX XXXX	X.X	X.X
PSG	X XXX XXXX	X.X	X.X

Epworth sleepiness scale (ESS) +

Type	Date	ESS Score
Pre-Implant	Sleep Study X XXX XXXX	XX
Therapy	Sleep Study X XXX XXXX	X
Therapy	Sleep Study X XXX XXXX	X

Settings

System information

Type	Model number	Serial number	Location
Amplitude (V)	XXXXX XX XXXXX XXXXX	XXXXXXXXXX	XXXXXX
Stimulation lead	--	--	--
Senior lead	--	--	--

Generator Summary

Battery	XXXX
---------	------

Programming Sessions < X XXX XXXX Visit >

Stimulation Advanced

Type	INCOMING	FINAL
Amplitude (V) CHANGES MADE	X.X	X.X
Patient control (V)	X.X - X.X	X.X - X.X
Pulse width (µs)	XX	XX
Rate (HZ)	XX	XX
Start delay (M)	XX	XX

Electrodes +-+○ +-+○

Sensing Advanced

Type	INCOMING	FINAL
Exhalation [Advanced default x x]	-x -x	-x -x
Off period [%]	x +x	x +x
Max stim time (S)	x	x
Invert	No	No

Stimulation thresholds

CURRENT	Rate	PW	Max stim
Type			
Amplitude (V) CHANGES MADE	X.X V		AIRWAY
Patient control (V)	X.X V		OPENING